

**(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE**

(11) Application No. AU 2010328622 B2

(54) Title
Implantable medical device with automatic tachycardia detection and control in MRI environments

(51) International Patent Classification(s)
A61N 1/37 (2006.01) **A61N 1/362 (2006.01)**
A61N 1/08 (2006.01) **A61N 1/39 (2006.01)**

(21) Application No: **2010328622** (22) Date of Filing: **2010.10.19**

(87) WIPO No: **WO11/071597**

(30) Priority Data

(31) Number **61/267,573** (32) Date **2009.12.08** (33) Country **US**

(43) Publication Date: **2011.06.16**
(44) Accepted Journal Date: **2014.09.11**

(71) Applicant(s)
Cardiac Pacemakers, Inc.

(72) Inventor(s)
Stubbs, Scott R.;Gilkerson, James O.;Doshi, Hiten J.;Schuster, Diane

(74) Agent / Attorney
Spruson & Ferguson, L 35 St Martins Tower 31 Market St, Sydney, NSW, 2000

(56) Related Art
US 2009/0157146
US 7369898

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
16 June 2011 (16.06.2011)

(10) International Publication Number
WO 2011/071597 A1

(51) International Patent Classification:
A61N 1/37 (2006.01) A61N 1/362 (2006.01)
A61N 1/08 (2006.01) A61N 1/39 (2006.01)

(74) Agents: KOZIOL, Paul G. et al.; 2200 Wells Fargo Center, 90 South Seventh Street, Minneapolis, Minnesota 55402-3901 (US).

(21) International Application Number:
PCT/US2010/053202

(22) International Filing Date:
19 October 2010 (19.10.2010)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/267,573 8 December 2009 (08.12.2009) US

(71) Applicant (for all designated States except US): CARDIAC PACEMAKERS, INC. [US/US]; 4100 Hamline Avenue North, St. Paul, Minnesota 55112 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): STUBBS, Scott R. [US/US]; 6509 East Fish Lake Road, Maple Grove, Minnesota 55369 (US). GILKERSON, James O. [US/US]; 10800 Kelvin Avenue North, Stillwater, Minnesota 55082 (US). DOSHI, Hiten J. [US/US]; 3925 Zircon Lane North, Plymouth, Minnesota 55446 (US). SCHUSTER, Diane [US/US]; 9900 Xerxes Curve, Bloomington, Minnesota 55431 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: IMPLANTABLE MEDICAL DEVICE WITH AUTOMATIC TACHYCARDIA DETECTION AND CONTROL IN MRI ENVIRONMENTS

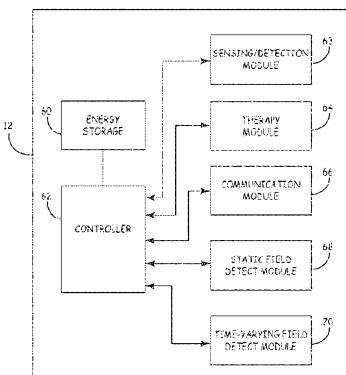


FIG. 2

(57) Abstract: An implantable medical device (IMD) includes a lead having one or more sensing electrodes and one or more therapy delivery electrodes, and a sensor configured to detect the presence of static and time-varying scan fields in a magnetic resonance imaging (MRI) environment. A controller, in electrical communication with the lead and the sensor, is configured to process signals related to tachycardia events sensed via the one or more sensing electrodes and to deliver pacing and shock therapy signals via the one or more therapy delivery electrodes. The controller compares the sensed static and time-varying scan fields to static and time-varying scan field thresholds. The controller controls delivery of anti-tachycardia pacing and shock therapy signals as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds.

WO 2011/071597 A1

IMPLANTABLE MEDICAL DEVICE WITH AUTOMATIC TACHYCARDIA DETECTION AND CONTROL IN MRI ENVIRONMENTS

TECHNICAL FIELD

[0001] The present invention relates to implantable medical devices. In particular, the present invention relates to an implantable medical device with automatic tachycardia detection control in MRI environments.

BACKGROUND

[0002] Magnetic resonance imaging (MRI) is a non-invasive imaging procedure that utilizes nuclear magnetic resonance techniques to render images within a patient's body. Typically, MRI systems employ the use of a magnetic coil having a magnetic field strength of between about 0.2 to 3 Teslas. During the procedure, the body tissue is briefly exposed to RF pulses of electromagnetic energy in a plane perpendicular to the magnetic field. The resultant electromagnetic energy from these pulses can be used to image the body tissue by measuring the relaxation properties of the excited atomic nuclei in the tissue.

[0003] During imaging, the electromagnetic radiation produced by the MRI system may be picked up by implantable device leads used in implantable medical devices such as pacemakers or cardiac defibrillators. This energy may be transferred through the lead to the electrode in contact with the tissue, which may lead to elevated temperatures at the point of contact. The degree of tissue heating is typically related to factors such as the length of the lead, the conductivity or impedance of the lead, and the surface area of the lead electrodes. Exposure to a magnetic field may also induce an undesired voltage on the lead.

SUMMARY

[0004] Discussed herein are various components for implantable medical devices to control delivery of anti-tachycardia pacing and shock therapy signals as a function of detected tachycardia events and sensed static and time-varying MRI scan fields, as well as implantable medical devices including such components and methods related to such implantable medical devices and components.

[0005] A first aspect of the present disclosure provides an implantable medical device (IMD) including a lead having one or more sensing electrodes and one or more therapy delivery electrodes. The IMD also includes a sensor configured to detect the presence of static and time-varying scan fields in a magnetic resonance imaging (MRI) environment. The IMD further includes a controller, in electrical communication with the lead and the sensor, configured to process signals related to tachycardia events sensed via the one or more sensing electrodes and to deliver pacing and shock therapy signals via the one or more therapy delivery electrodes. The controller is also configured to compare the sensed static and time-varying scan fields to static and time-varying scan field thresholds. The controller controls delivery of anti-tachycardia pacing and shock therapy signals as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds.

[0006] In the first aspect the controller disqualifies the tachycardia events to inhibit delivery of the anti-tachycardia pacing and shock therapy signals when the static and time-varying scan field thresholds are exceeded.

[0007] In the first aspect the controller processes sensed tachycardia events, enables delivery of the anti-tachycardia pacing signals, and inhibits delivery of the shock therapy signals when the static scan field threshold is exceeded and the time-varying scan field thresholds are not exceeded.

[0008] The controller may process sensed tachycardia events and enables delivery of the anti-tachycardia pacing and shock therapy signals when the neither of the static and time-varying scan field thresholds is exceeded.

[0009] The controller may be operable to switch the IMD between a normal mode and an MRI mode, and wherein the sensor is disabled in the normal mode and the sensor is enabled in the MRI mode.

[0010] The controller may automatically switch the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.

[0011] The controller may further control delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.

[0012] A further aspect provides a method for operating an implantable medical device (IMD) includes sensing static and time-varying scan fields in a magnetic resonance imaging (MRI) environment and comparing the sensed fields to static and time-varying scan field thresholds. Signals related to tachycardia events are detected, and delivery of anti-tachycardia pacing and shock therapy signals is controlled as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds.

[0013] In the method the controlling step comprises delivering anti-tachycardia pacing and/or shock therapy signals when a tachycardia event is detected and neither of the static and time-varying scan field thresholds is exceeded.

[0014] In the method the controlling step comprises delivering the anti-tachycardia pacing signals and inhibiting delivery of the shock therapy signals when signals related to a tachycardia event is detected and the static scan field threshold is exceeded and the time-varying scan field thresholds are not exceeded.

[0015] In the method the controlling step may comprise inhibiting delivery of the anti-tachycardia pacing and shock therapy signals and disqualifying detected tachycardia events when the static and time-varying scan field thresholds are exceeded.

[0016] In the method the controlling step further comprise controlling delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.

[0017] In the method, prior to the sensing step, the method may further comprise switching the IMD from a normal mode to an MRI mode.

[0018] The method may further comprise automatically switching the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.

[0019] According a further aspect, a method for operating an implantable medical device (IMD) includes sensing static and time-varying scan fields in a magnetic resonance imaging (MRI) environment and comparing the sensed fields to static and time-varying scan field thresholds. Signals related to tachycardia events are detected, and delivery of anti-tachycardia pacing and shock therapy signals is controlled as a function of the detected tachycardia events and the threshold comparisons. Particularly, anti-tachycardia pacing

and/or shock therapy signals are delivered when a tachycardia event is detected and neither of the static and time-varying scan field thresholds is exceeded. In addition, the anti-tachycardia pacing signals are delivered and delivery of the shock therapy signals is inhibited when signals related to a tachycardia event is detected and the static scan field threshold is exceeded and the time-varying scan field thresholds are not exceeded. Furthermore, delivery of the anti-tachycardia pacing and shock therapy signals is inhibited and detected tachycardia events are disqualified when the static and time-varying scan field thresholds are exceeded.

[0020] The method, prior to the sensing step, the method may further comprise switching the IMD from a normal mode to an MRI mode.

[0021] The method may further comprise automatically switching the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.

[0022] The method the controlling step may further comprise controlling delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.

[0023] While multiple embodiments are disclosed, still other embodiments of the present invention will become apparent to those skilled in the art from the following detailed description, which shows and describes illustrative embodiments of the invention. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] FIG. 1 is a schematic view of a cardiac rhythm management (CRM) system including a pulse generator and a lead implanted in a patient's heart according to an embodiment of the present invention.

[0025] FIG. 2 is a functional block diagram of an implantable medical device (IMD) configured to detect fields generated by magnetic resonance imaging (MRI) systems and deliver anti-tachycardia therapy as a function of the detected fields.

[0026] FIG. 3 is a flow diagram of a process for detecting MRI scan fields and controlling delivery of anti-tachycardia therapy as a function of the detected fields.

[0027] While the invention is amenable to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and are described in detail below. The intention, however, is not to limit the invention to the particular embodiments described. On the contrary, the invention is intended to cover all modifications, equivalents, and alternatives falling within the scope of the invention as defined by the appended claims.

DETAILED DESCRIPTION

[0028] FIG. 1 is a schematic view of a cardiac rhythm management (CRM) system 10 according to an embodiment of the present invention. As shown in FIG. 1, the CRM system 10 includes a pulse generator 12 coupled to a plurality of leads 14, 16 deployed in a patient's heart 18. As further shown in FIG. 1, the heart 18 includes a right atrium 24 and a right ventricle 26 separated by a tricuspid valve 28. During normal operation of the heart 18, deoxygenated blood is fed into the right atrium 24 through the superior vena cava 30 and the inferior vena cava

32. The major veins supplying blood to the superior vena cava 30 include the right and left axillary veins 34 and 36, which flow into the right and left subclavian veins 38 and 40. The right and left external jugular 42 and 44, along with the right and left internal jugular 46 and 48, join the right and left subclavian veins 38 and 40 to form the right and left brachiocephalic veins 50 and 52, which in turn combine to flow into the superior vena cava 30.

[0029] The leads 14, 16 operate to convey electrical signals and stimuli between the heart 18 and the pulse generator 12. In the illustrated embodiment, the lead 14 is implanted in the right ventricle 26, and the lead 16 is implanted in the right atrium 24. In other embodiments, the CRM system 10 may include additional leads, e.g., a lead extending into a coronary vein for stimulating the left ventricle in a bi-ventricular pacing or cardiac resynchronization therapy system. As shown, the leads 14, 16 enter the vascular system through a vascular entry site 54 formed in the wall of the left subclavian vein 40, extend through the left brachiocephalic vein 52 and the superior vena cava 30, and are implanted in the right ventricle 26 and right atrium 24, respectively. In other embodiments of the present invention, the leads 14, 16 may enter the vascular system through the right subclavian vein 38, the left axillary vein 36, the left external jugular 44, the left internal jugular 48, or the left brachiocephalic vein 52.

[0030] The pulse generator 12 is typically implanted subcutaneously within an implantation location or pocket in the patient's chest or abdomen. The pulse generator 12 may be any implantable medical device known in the art or later developed, for delivering an electrical therapeutic stimulus to the patient. In various embodiments, the pulse generator 12 is a pacemaker, an implantable cardiac defibrillator, and/or includes both pacing and defibrillation capabilities. The portion of the leads 14, 16 extending from the pulse generator 12 to the vascular entry site 54 are also located subcutaneously or submuscularly. The leads 14, 16 are each connected to the pulse generator 12 via proximal connectors. Any excess lead length, i.e., length beyond that needed to reach from the pulse generator 12 location to the desired intracardiac implantation site, is generally coiled up in the subcutaneous pocket near the pulse generator 12.

[0031] FIG. 2 is a functional block diagram of an embodiment of the IMD 12. The IMD 12 includes an energy storage device 60, a controller 62, a sensing and detection module 63, a therapy module 64, a communication module 66, a static field detect module 68, and a time-varying field detect module 70. The term "module" is not intended to imply any particular structure. Rather, "module" may mean components and circuitry integrated into a single unit as well as individual, discrete components and circuitry that are functionally related. In addition, it should be noted that IMD 12 may include additional functional modules that are operable to perform other functions associated with operation of IMD 12.

[0032] The energy storage device 60 operates to provide operating power to the controller 62, sensing and detection module 63, therapy module 64, communication module 66, static field detect module 68, and time-varying field detect module 70. The controller 62 operates to control and receive signals from the sensing and detection module 63, therapy module 64, communication module 66, static field detect module 68, and time-varying field detect module 70, each of which is operatively coupled to and communicates with the controller 62. For example, the controller 62 may command the therapy module 64 to deliver a desired therapy, such as a pacing or defibrillation stimulus, based on signals received from the sensing and detection module 63. In addition, the controller 62 may command the communication module 66 to transmit and/or receive data from an external device (e.g., a programmer). Furthermore, the controller 62 may receive signals from the static field detect module 68 and/or the time-varying field detect module 70 indicating the presence or absence of fields generated by an MRI scan.

[0033] The IMD 12 may also include timing circuitry (not shown) which operates to schedule, prompt, and/or activate the IMD 12 to perform various activities. In one embodiment, the timing circuitry is an internal timer or oscillator, while in other embodiments, timing may be performed by specific hardware components that contain hardwired logic for performing the steps, or by any combination of programmed computer components and custom hardware components.

[0034] The communication module 66 is configured to both transmit and receive telemetry signals to and from other devices, such as an external programmer. For example, the communication module 66 may be configured to receive signals from the external programmer to switch the operation mode of the communication module 66 between a normal mode and a magnetic resonance imaging (MRI) mode. The IMD 12 may alternatively include at least one transducer configured for receiving a telemetry signal and at least one transducer for transmitting a telemetry signal. The communication module 66 may be any type of device capable of sending and/or receiving information via a telemetry signal, including, but not limited to, a radio frequency (RF) transmitter, an acoustic transducer, or an inductive transducer.

[0035] The sensing and detection module 63 and therapy module 64 operate to perform the therapeutic and/or diagnostic functions of the IMD 12. In some embodiments, the sensing and detection module 63 senses signals related to tachycardia events (e.g., tachyarrhythmia) via one or more sensing electrodes on the lead 14, 16. The sensing and detection module 63 may also be operable to automatically determine the capture threshold of the heart 18 by providing a pacing stimulus to the heart 18 and sensing whether the stimulus results in a contraction of the heart 18. One example circuit arrangement that may be included in the sensing and detection module 63 to determine the capture threshold of heart 18 is disclosed in United States Patent No. 7,092,756, entitled "Autocapture Pacing/Sensing Configuration," which is incorporated herein by reference in its entirety.

[0036] In some embodiments, the therapy module 64 delivers a cardiac pacing and/or defibrillation stimulus to the heart 18 via one or more therapy electrodes on the lead 14, 16. The type and timing of therapy delivered by the therapy module 64 may be controlled by the controller 62. In some embodiments, the therapy delivery is based on sensed static and time-varying fields, as will be described in more detail below. In addition, the controller 62 may control operation of the therapy module 64 based on programmed therapy settings. The therapy module 64 is not limited to performing any particular type of physiologic

therapy, and may be configured to perform other types of physiologic therapy, such as neurological measurements and therapy.

[0037] The static field detect module 68 senses the presence of the static magnetic fields associated with an MRI scan. In some embodiments, the static field detect module 68 includes a power inductor and a core saturation detector. When the power inductor saturates in the presence of a static MRI field, the inductance of the power inductor decreases, which is detected by the core saturation detector. One example module having such a configuration that is suitable for use in static field detect module 68 is disclosed in U.S. Patent No. 7,509,167, entitled "MRI Detector for Implantable Medical Device," which is incorporated herein by reference in its entirety. Any type of sensor or device may alternatively or additionally be incorporated into the static field detect module 68 that is operable to detect the presence of static MRI fields.

[0038] The time-varying field detect module 70 senses the presence of the time-varying gradient magnetic fields and radio frequency (RF) electromagnetic fields associated with an MRI scan. The time-varying field detect module 70 may include a magnetometer or other device employable to detect the gradient field dB/dt (i.e., the time derivative of magnetic field B). In some embodiments, the magnetometer includes a Hall effect sensor, a magnetotransistor, a magnetodiode, a magneto-optical sensor, and/or a giant magnetoresistive sensor. The time-varying field detect module 70 may also include an electromagnetic sensor capable of detecting the presence of RF fields. For example, the time-varying field detect module 70 may include an electromagnetic interference (EMI) detector such as that described in U.S. Patent No. 5,697,958, entitled "Electromagnetic Noise Detector for Implantable Medical Devices," which is herein incorporated by reference in its entirety.

[0039] According to some embodiments, the IMD 12 is configured to detect magnetic and electromagnetic fields generated by an MRI system and to control delivery of anti-tachycardia therapy from the therapy module 64 as a function of the detected fields. In particular, the IMD 12 detects the presence of the static and/or time-varying fields associated with an MRI procedure and automatically adjusts the types of therapy delivered to the heart 18 at various levels of MRI

influence. This reduces the amount of power drawn from the energy storage device 60 due to failed shock therapy attempts when the IMD 12 is under high static field influence and avoids having to manually disable and enable different types of anti-tachycardia therapy before and after the MRI procedure.

[0040] FIG. 3 is a flow diagram of an exemplary process that may be employed by the IMD 12 to detect the fields generated by an MRI system and control delivery of anti-tachycardia therapy based on the detected fields. At step 80, the IMD 12 is switched from a normal mode of operation to an MRI mode of operation. The IMD 12 may be programmed into the MRI mode by wirelessly sending a signal from an external programmer to the controller 62 via the communication module 66, for example. In some embodiments, the field detect modules 68 and 70 are active in both the normal mode and the MRI mode of operation. In other embodiments, switching the IMD 12 to the MRI mode activates the field detect modules 68 and 70 for detection of MRI scan fields.

[0041] The normal operational mode is the operational mode of the IMD 12 as initially programmed. The MRI operational mode can refer to any operational mode of the IMD 12 that is a safe operational mode in the presence of EMI. For example, for a bradycardia engine in a tachycardia device, an MRI mode might be a fixed-rate and/or non-demand (or asynchronous) pacing mode as opposed to a rate-responsive and/or demand pacing mode. In some embodiments, an MRI mode can be both a non-demand mode (i.e., VOO) and a non-rate-responsive mode. Thus, in accordance with one embodiment, switching the IMD 12 to an MRI mode might entail switching the bradycardia engine to a VOO, AOO or DOO pacing mode. The mode to which the device is switched may depend on the original programmed mode of the device. For example, an IMD 12, which is normally programmed to a Dxx mode (i.e., DDDR, DDD, DDI, or DVI) would switch to DOO when in MRI the MRI mode. Similarly, a device programmed to Vxx mode would switch to VOO, and a device programmed to Axx mode would switch to AOO mode.

[0042] It should be noted that there may be other modes of operation that are considered safe in an MRI environment, so the present invention is not limited to the MRI modes discussed herein. Further, as one skilled in the art will

appreciate, other types of IMDs will have different mode types that might be considered safe in an MRI environment, and those modes also are considered MRI modes for purposes of the present invention.

[0043] It should also be noted that step 80 applies to IMDs 12 that are programmed with an MRI mode. In embodiments in which the IMD 12 does not include an MRI mode, the IMD 12 may be configured such that the static field detect module 68 and the time-varying field detect module 70 are maintained in an enabled state such that the presence of static and/or time-varying fields would be detected without being programmed into an MRI mode.

[0044] At step 82, the static field detect module 68 detects the presence of static magnetic fields associated with an MRI procedure, and the time-varying field detect module 70 detects the presence of time-varying magnetic and electromagnetic fields associated with an MRI procedure. The step 82 is continuously performed throughout the process illustrated in FIG. 4. That is, the static and time-varying fields are continuously monitored such that the IMD 12 can continuously respond to the changing presence or absence of each of the fields. In some embodiments, the static field detect module 68 and time-varying field detect module 70 provide signals to the controller 62 related to the magnitude of the detected fields. The controller 62 may determine the magnitude of the gradient field by calculating the mean of dB/dt . In some embodiments, the time-varying field detect module 70 also provides signals to controller 62 related to other characteristics of the detected field, such as field frequency and the slew rate of the gradient magnetic field.

[0045] After detecting the presence of static and/or time-varying fields, then, at step 84, the controller 62 compares the sensed static and time-varying fields to static and time-varying field thresholds, respectively. The static and time-varying field thresholds may be stored or programmed in the controller 62. The time-varying field threshold may include a magnetic component for the gradient field and an electromagnetic component for the RF field. In some embodiments, the static and time-varying field thresholds are set based on common or expected magnetic and electromagnetic field levels in an MRI environment. This differentiates fields generated by an MRI system from those generated by other

sources of magnetic and electromagnetic fields. In one exemplary embodiment, the static field threshold is about 0.2 T, and the gradient field component of the time-varying field threshold is about 10 T/s. The RF component of the time-varying field threshold may be a function of the presence of an RF field associated with an MRI procedure (e.g., 63.864 MHz or 127.728 MHz) in combination with the presence of an electric field having a threshold magnitude.

[0046] In decision step 86, if the time-varying field or fields detected by the time-varying field detect module 70 exceed the time-varying field threshold, then, in step 88, the IMD 12 disqualifies tachycardia events detected by the one or more sensing electrodes on the leads 14, 16. The presence of high time-varying fields indicates that an the IMD 12 is being subjected to an active MRI scan. The time-varying fields can induce a current on the leads 14, 16, which may cause the one or more sensing electrodes to incorrectly detect the occurrence of a tachycardia event. Consequently, when time-varying fields that exceed the time-varying threshold are detected, the IMD 12 disqualifies the tachycardia events detected by the sensing and detection module 63 as being unreliable. The process then returns to step 84 to compare the detected fields to the field thresholds.

[0047] If, in decision step 86, the time-varying fields detected by the time-varying field detect module 70 do not exceed the time-varying field threshold, then, in decision step 90, the controller 62 determines whether the static field detected by the static field detect module 68 exceeds the static field threshold. If the static field threshold is exceeded, then, in step 92, the controller 62 delivers anti-tachycardia pacing (ATP) therapy as programmed via one or more therapy delivery electrodes on leads 14, 16, but inhibits delivery of shock therapy through the leads 14, 16. The ATP therapy is delivered because tachycardia events detected by the leads in the absence of strong time-varying fields are reliable, and the static fields do not have a substantial effect on the delivery of the ATP therapy. However, in alternative embodiments, the controller 62 may be programmed to disable ATP therapy in the presence of a static field that exceeds the static field threshold. The ATP therapy delivery program may also be selected or changed by a clinician by communicating with the controller 62 via the communication module 66.

[0048] Delivery of shock therapy is inhibited in the presence of a strong static field because the strong field may saturate materials associated with the power components of the IMD 12 (e.g., inductors in the energy storage device 60). Under saturation conditions, the time to charge the high voltage capacitor(s) to maximum energy can be protracted, or the maximum energy may not be attainable. Consequently, in order to prevent delayed or failed delivery of the shock therapy, the controller 62 inhibits delivery of shock therapy in the presence of a static field that exceeds the static field threshold.

[0049] If the static field threshold is not exceeded in step 90, then, in step 94, the controller 62 delivers ATP and/or shock therapy as programmed when tachycardia events are detected by the one or more sensing electrodes. Thus, the controller 62 adjusts delivery of ATP and/or shock therapy automatically based on the type and magnitude of fields detected by the field detector modules 68, 70. This assures that safe and reliable anti-tachycardia therapy is provided to the patient for the maximum amount of time when the patient is subjected to MRI fields.

[0050] In embodiments of the IMD 12 that includes an MRI mode of operation, the IMD 12 may subsequently return to the normal mode of operation, in step 96. In some embodiments, the controller 62 automatically switches the IMD 12 to the normal mode of operation when the detected static field falls below the static field threshold. In alternative embodiments, the static field threshold at which the IMD 12 returns to the normal mode of operation is different than the static field threshold discussed above with regard to decision step 90. The switch to the normal mode of operation may also be further triggered by the detection of a tachycardia event after the static field drops below a threshold level.

[0051] In summary, embodiments of the present invention relate to an implantable medical device (IMD) including a lead having one or more sensing electrodes and one or more therapy delivery electrodes. The IMD also includes a sensor configured to detect the presence of static and time-varying scan fields in a magnetic resonance imaging (MRI) environment. The IMD further includes a controller, in electrical communication with the lead and the sensor, configured to process signals related to tachycardia events sensed via the one or more sensing

electrodes and to deliver pacing and shock therapy signals via the one or more therapy delivery electrodes. The controller is also configured to compare the sensed static and time-varying scan fields to static and time-varying scan field thresholds. The controller controls delivery of anti-tachycardia pacing and shock therapy signals as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds. An IMD having this configuration controls the type of anti-tachycardia therapy delivered to the patient at various levels of MRI influence, reduces the power draw on the IMD battery due to failed shock therapy attempts, and avoids having to manually disable and enable anti-tachycardia therapy before and after the MRI procedure.

[0052] Various modifications and additions can be made to the exemplary embodiments discussed without departing from the scope of the present invention. For example, while the embodiments described above refer to particular features, the scope of this invention also includes embodiments having different combinations of features and embodiments that do not include all of the described features. Accordingly, the scope of the present invention is intended to embrace all such alternatives, modifications, and variations as fall within the scope of the claims, together with all equivalents thereof.

CLAIMS

1. An implantable medical device (IMD) comprising:
 - a lead including one or more sensing electrodes and one or more therapy delivery electrodes;
 - a sensor configured to detect the presence of static and time-varying scan fields in a magnetic resonance imaging (MRI) environment; and
 - a controller, in electrical communication with the lead and the sensor, configured to process signals related to tachycardia events sensed via the one or more sensing electrodes and to deliver pacing and shock therapy signals via the one or more therapy delivery electrodes, the controller further configured to compare the sensed static and time-varying scan fields to static and time-varying scan field thresholds, wherein the controller controls delivery of anti-tachycardia pacing and shock therapy signals as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds,
 - wherein the controller processes sensed tachycardia events, enables delivery of the anti-tachycardia pacing signals, and inhibits delivery of the shock therapy signals when the static scan field threshold is exceeded and the time-varying scan field thresholds is not exceeded, and
 - wherein the controller disqualifies the tachycardia events to inhibit delivery of the anti-tachycardia pacing and shock therapy signals when both the static and time-varying scan field thresholds are exceeded.
2. The IMD of claim 1, wherein the controller processes sensed tachycardia events and enables delivery of the anti-tachycardia pacing and shock therapy signals when the neither of the static and time-varying scan field thresholds is exceeded.
3. The IMD of claim 1, wherein the controller is operable to switch the IMD between a normal mode and an MRI mode, and wherein the sensor is disabled in the normal mode and the sensor is enabled in the MRI mode.

4. The IMD of claim 3, wherein the controller automatically switches the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.
5. The IMD of claim 1, wherein the controller further controls delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.
6. A method for operating an implantable medical device (IMD), the method comprising:
 - sensing static and time-varying scan fields in a magnetic resonance imaging (MRI) environment;
 - comparing the sensed static and time-varying scan fields to static and time-varying scan field thresholds;
 - detecting signals related to tachycardia events; and
 - controlling delivery of anti-tachycardia pacing and shock therapy signals as a function of the detected tachycardia events, the comparison of the sensed static scan field to the static scan field threshold, and the comparison of the time-varying scan fields to the time-varying scan field thresholds wherein:
 - the controlling step comprises delivering the anti-tachycardia pacing signals and inhibiting the shock therapy signals when a signal related to a tachycardia event is detected and the static scan field threshold is exceeded and the time-varying scan field threshold is not exceeded, and
 - the controlling step comprises inhibiting the anti-tachycardia pacing and shock therapy signals when both of the static and time-varying scan field thresholds are exceeded.
7. The method of claim 6, wherein the controlling step comprises:

delivering anti-tachycardia pacing and/or shock therapy signals when a tachycardia event is detected and neither of the static and time-varying scan field thresholds is exceeded.

8. The method of claim 6, wherein the controlling step comprises:
disqualifying detected tachycardia events to inhibit the anti-tachycardia pacing and shock therapy signals when the static and time-varying scan field thresholds are exceeded.
9. The method of claim 6, wherein the controlling step further comprises controlling delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.
10. The method of claim 6, wherein, prior to the sensing step, the method further comprises:
switching the IMD from a normal mode to an MRI mode.
11. The method of claim 10, and further comprising:
automatically switching the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.
12. A method for operating an implantable medical device (IMD), the method comprising:
sensing static and time-varying scan fields in a magnetic resonance imaging (MRI) environment;
comparing the sensed static and time-varying scan fields to static and time-varying scan field thresholds;
detecting signals related to tachycardia events; and
controlling delivery of anti-tachycardia pacing and shock therapy signals,
wherein the controlling step comprises:
delivering anti-tachycardia pacing and/or shock therapy signals when a tachycardia event is detected and neither of the static and time-varying scan field thresholds is exceeded;

delivering the anti-tachycardia pacing signals and inhibiting delivery of the shock therapy signals when signals related to a tachycardia event is detected and the static scan field threshold is exceeded and the time-varying scan field thresholds are not exceeded; and
inhibiting delivery of the anti-tachycardia pacing and shock therapy signals and disqualifying detected tachycardia events when the static and time-varying scan field thresholds are exceeded.

13. The method of claim 12, wherein, prior to the sensing step, the method further comprises:
switching the IMD from a normal mode to an MRI mode.
14. The method of claim 13, and further comprising:
automatically switching the IMD from the MRI mode to the normal mode when the static scan field is less than the static scan field threshold.
15. The method of claim 12, wherein the controlling step further comprises controlling delivery of anti-tachycardia pacing and shock therapy signals as a function of programmed therapy settings.

Cardiac Pacemakers, Inc.
Patent Attorneys for the Applicant/Nominated Person
SPRUSON & FERGUSON

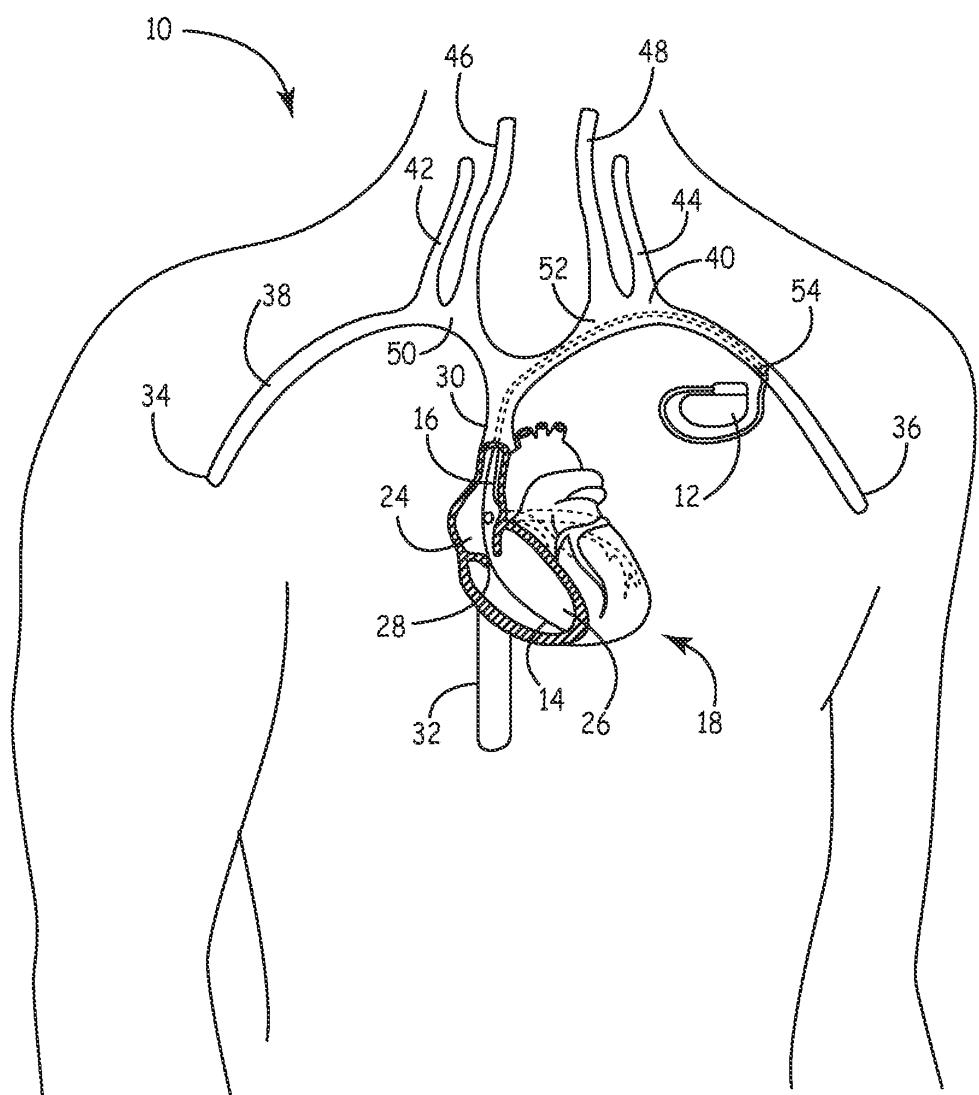


FIG. 1

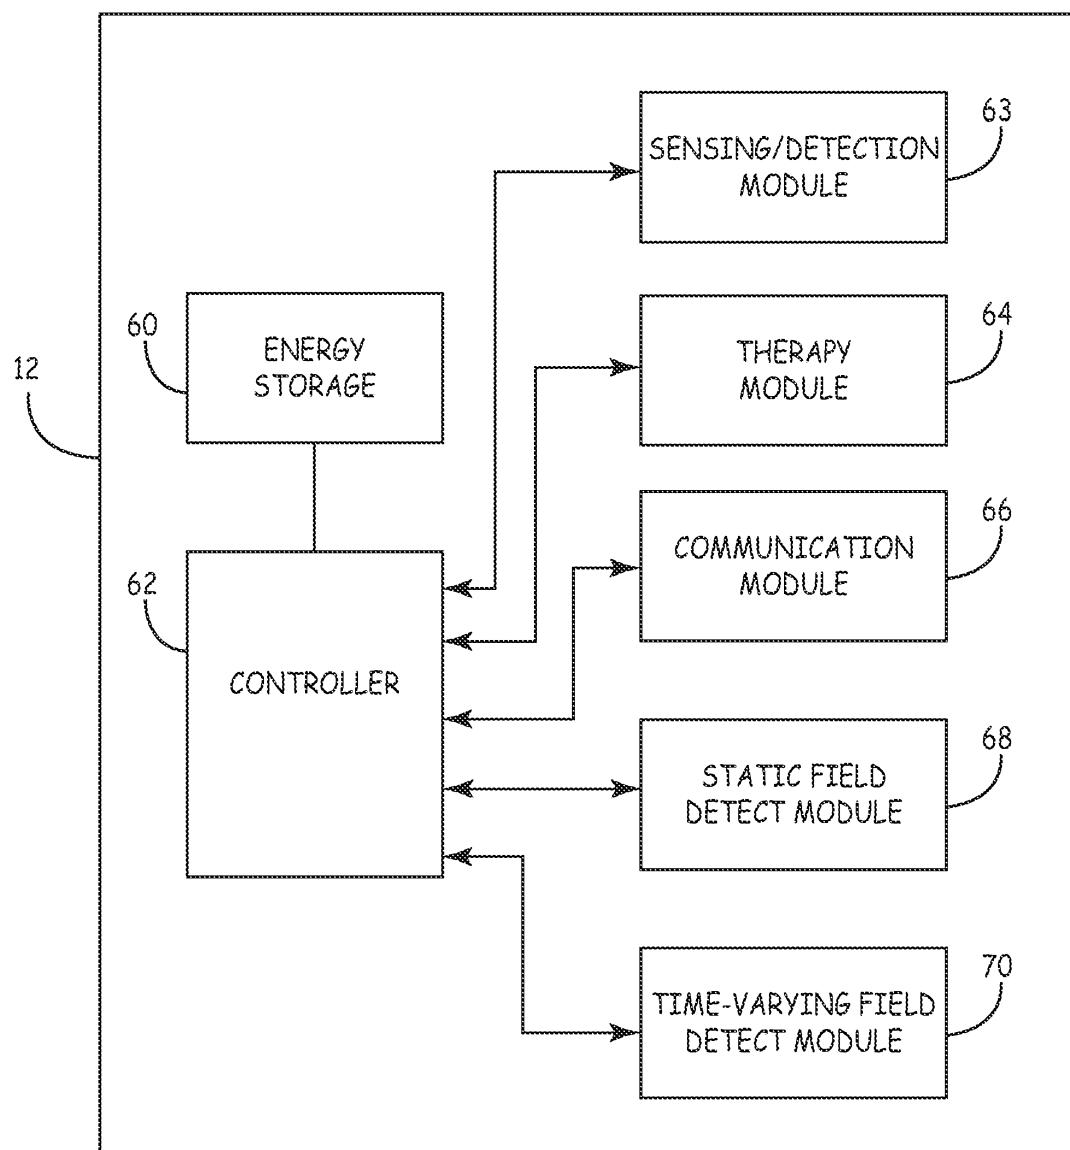


FIG. 2

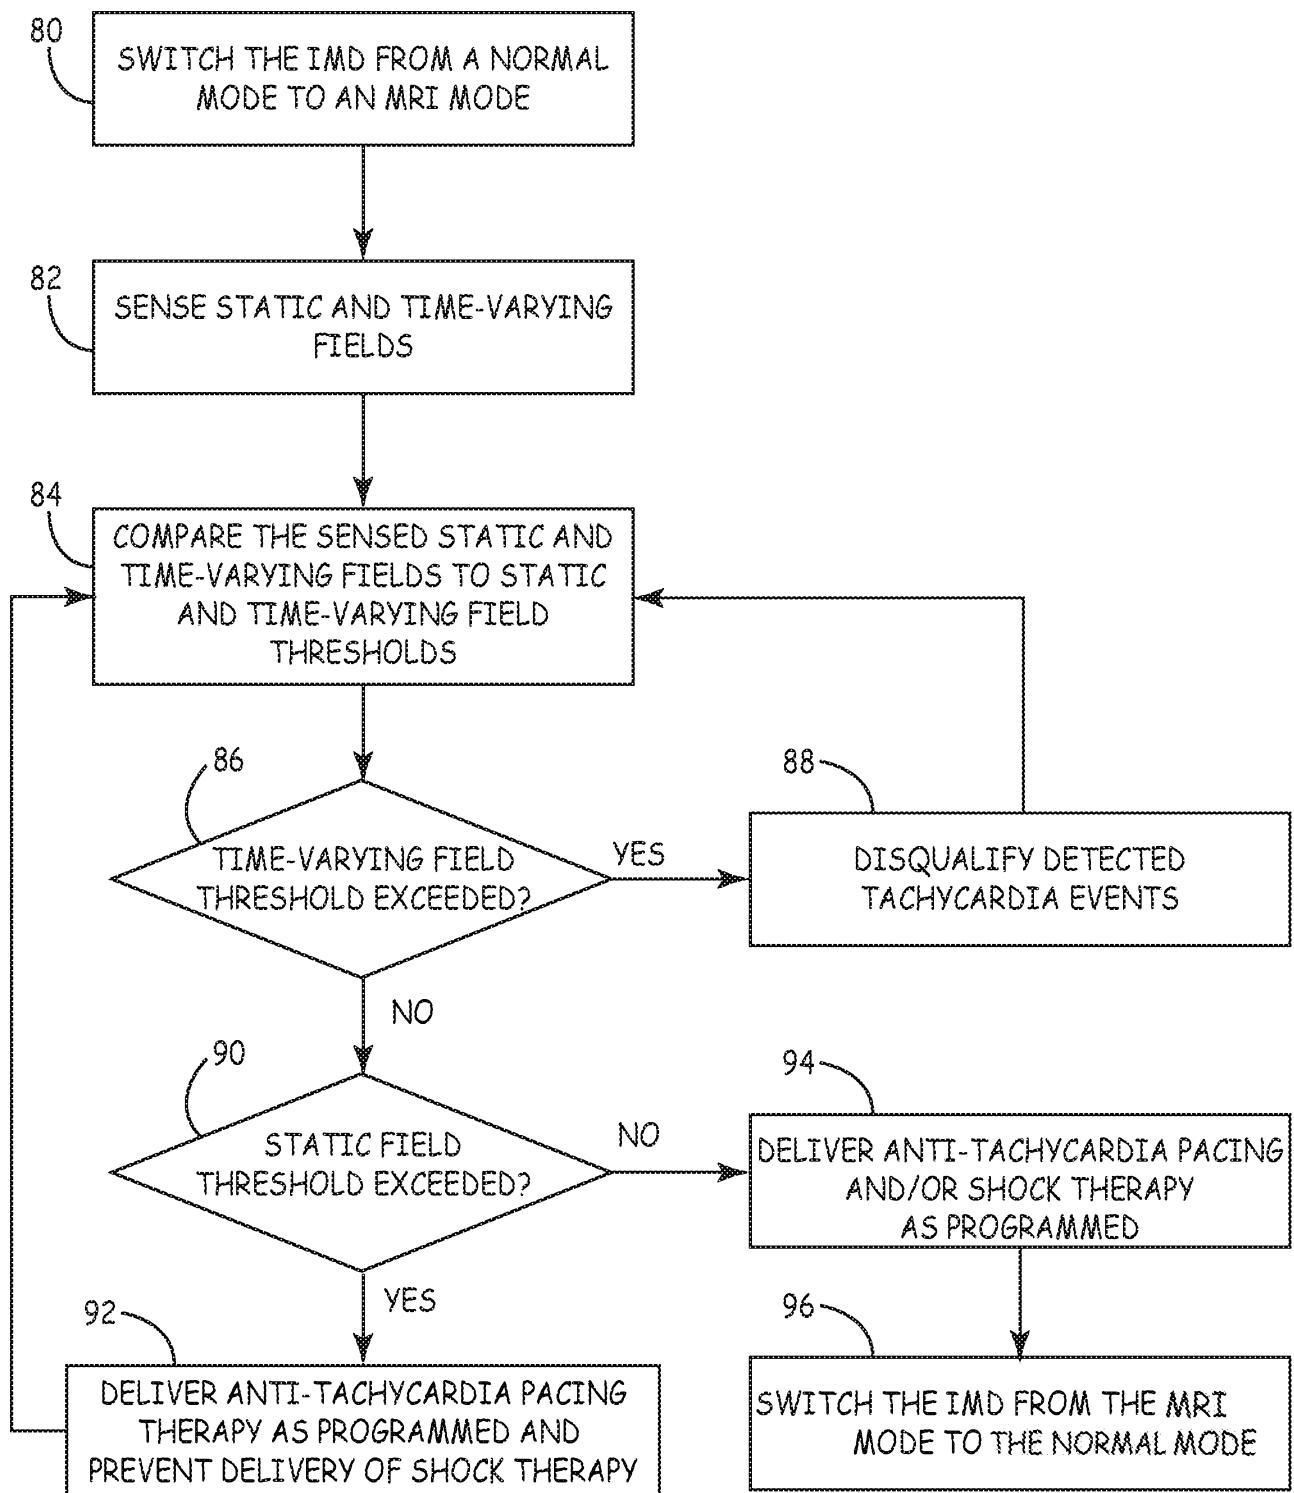


FIG. 3