



- (51) **International Patent Classification:**
A61F 9/00 (2006.01) A61B 3/00 (2006.01)
- (21) **International Application Number:**
PCT/IB2015/056159
- (22) **International Filing Date:**
13 August 2015 (13.08.2015)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
433/DEL/2015 16 February 2015 (16.02.2015) IN
- (72) **Inventor; and**
- (71) **Applicant : ROOP, Prakhyat** [IN/IN]; c/o Dr.Roop, 348, Govind Lok, E.K. Road, -, Uttar Pradesh, Meerut 250001 (IN).
- (74) **Agents: PUTTAIAH, Kartik** et al.; InvenTree IP Services, 399, 15th Cross, 5th Main, Sector-6, HSR Layout, Bangalore 560102 (IN).
- (81) **Designated States** (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,

KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.


- (84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))
- with amended claims (Art. 19(1))

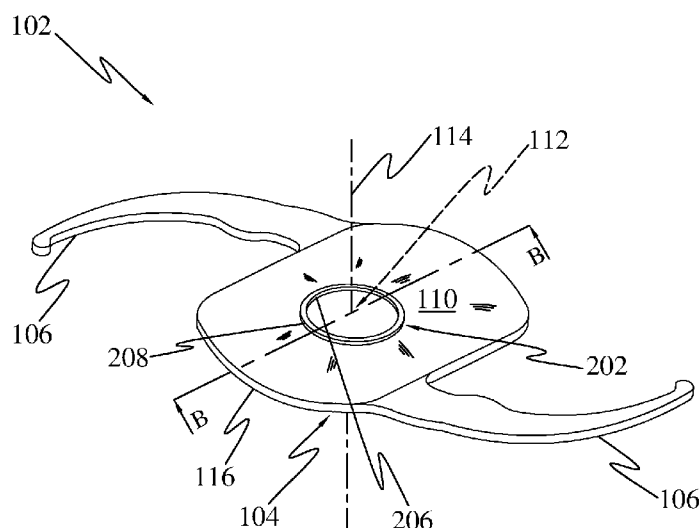(54) **Title:** OPTICAL IMPLANTABLE MEMBER**FIG. 2**

(57) **Abstract:** An optical implantable member (102) is provided. The optical implantable member (102) includes an optic (104). The optic (104) includes an anterior surface (108) and a posterior surface (110), an optical centre (112) and a peripheral edge (116). The optical implantable member (102) is configured to be placed within a capsular bag of the eye. The optic (104) of the optical implantable member (102) includes a barrier (202). The barrier (202) is formed by a protrusion (202) on the posterior surface (110) of the optic (104). The protrusion (202) is concentric to an optical axis (114) of the optic (104). An outer wall (204 or 208) of the protrusion (202) is between the peripheral edge (116) and the optical centre (112). The barrier (202) restricts epithelial cells from migrating towards a central region of the capsular bag.

OPTICAL IMPLANTABLE MEMBER

BACKGROUND

Field

5 **[0001]** The disclosed subject matter in general relates to intraocular/ophthalmic implants, and more particularly, but not exclusively, the subject matter relates to intraocular lens/ophthalmic implants (IOL) with optic that delays development of secondary or after cataract, and facilitates better positioning.

Discussion of related field

10 **[0002]** Clouding of the natural lens in the eye, which leads to decrease in vision, is termed as cataract. A cataractous lens is located within a capsular sac or lens capsule in the posterior chamber of the eye. A method of treating a cataract eye is to remove the clouded natural lens and replace it with an artificial intraocular lens (IOL) in a surgical procedure. Following removal of the cataractous lens, the artificial IOL is typically implanted within the
15 lens capsule in order to mimic the refractive function of the natural lens.

[0003] Although IOL implant provides significant benefits to most cataract patients, in a considerable percentage of all patients who have IOL implants, secondary cataract or after cataract may develop within months to years after surgery. Secondary cataract is caused by the deposit and proliferation of cells and fibres on the posterior capsular membrane, thereby
20 obstructing light passing through the IOL implant and obscuring the patient's vision. These cell deposits may originate from the proliferation of residual lens epithelial cells on the internal surface of the lens capsule after surgery and/or the accumulation of inflammatory cells and protein deposits on the IOL implant. Of these two sources, the major cause of secondary cataract may be the proliferation and migration of the residual lens epithelial cells,
25 which originate from the anterior surface of the residual capsular bag or from the equator of capsular bag, towards the central part of posterior surface of the capsular bag.

[0004] Conventionally, ophthalmic surgeons typically take considerable care in trying to remove all residual lens epithelial cells prior to the implantation of an artificial IOL implant. However, despite these efforts, some amount of lens epithelial cells usually are left on the
30 internal surface of the capsular bag due to the fact that these cells are difficult to identify and are often difficult to reach due to their position on the inside surface of the capsular bag.

[0005] Conventionally, various mechanical means and pharmaceutical means are employed to minimize the formation of secondary cataract. Efforts have been directed at creating an IOL having a posterior peripheral wall with a square edge to present a mechanical barrier to the cells. This wall has, at least to some extent, enabled reduction of growth and migration of the lens epithelial cells towards the centre of the optic of the IOL. However, even with this square edge, there have been several instances of formation of secondary cataract and incidence of after cataract not being eliminated.

[0006] In light of the above discussion, there is a need for a technique that can be employed in mechanically restricting epithelial cells from migrating towards the centre of the IOL, thereby preventing opacification of the visual axis.

[0007] Moreover, conventional IOLs do not conform to the normal structure and function of the eye. In a human eye, the peripheral part of the retina extends more on the nasal side (side of nose) than on the temporal side (side of ear), which causes some people to experience blank space on the side of the ear, commonly referred to as negative dysphotopsia.

[0008] Further, in significant number of cases, the centre of pupil is slightly towards the side of the nose (nasal) and not in the geometrical centre of the cornea/eye, and line of sight (visual axis) is still more nasal to the centre of pupil. This is known as positive angle kappa. In some cases, the line of sight passes away from the centre of eye/cornea and towards temporal side, which is known as negative angle kappa.

[0009] Conventional IOLs have round optic and its optical centre is at its geometrical centre. Thus after implantation, the optical centre does not come in line of the line of sight or visual axis, which leads to deterioration of quality of vision. Besides this, at present there is no provision to make surgeon aware of the position of optical centre of IOL, thereby making it difficult to align the optical centre of the IOL with visual axis.

[0010] In light of the above discussion, there is a need for a technique where the optic of IOL is designed in such fashion that it ameliorates negative dysphotopsia, compensates for angle kappa and at the same time has some provision to guide surgeon to aim for proper centring.

SUMMARY

[0011] An embodiment provides an optical implantable member. The optical implantable member includes an optic. The optic includes an anterior surface and a posterior surface, an optical centre and a peripheral edge. The optical implantable member is configured to be

placed within a capsular bag of the eye. The optic also includes a barrier. The barrier is formed by a protrusion on the posterior surface of the optic. An outer wall of the protrusion is between the peripheral edge and the optical centre. The barrier restricts epithelial cells from migrating towards a central region of the capsular bag. The protrusion is concentric to an optical axis of the optic and hence helps in proper centring of the optical implantable member.

BRIEF DESCRIPTION OF DRAWINGS

[0012] Embodiments are illustrated by way of example and not limitation in the Figures of the accompanying drawings, in which like references indicate similar elements and in which:

[0013] FIG. 1 is an illustration of the anterior surface 108 of exemplary optical implantable member 102, in accordance with an embodiment;

[0014] FIG. 1A is an illustration of the posterior surface 110 of the optical implantable member 102 of FIG. 1, wherein a barrier 202 is visible;

[0015] FIG. 1B is a cross sectional view of the optical implantable member 102 of FIG. 1A along axis A-A;

[0016] FIG. 1C is an isometric view of the optical implantable member 102 of FIG. 1A;

[0017] FIG. 1D is an isometric view of the optical implantable member 102 of FIG. 1, in which the barrier 202 is visible;

[0018] FIG. 2 is an isometric posterior view of another exemplary optical implantable member 102 showing a barrier 202 that resembles the shape of a ring, in accordance with an embodiment;

[0019] FIG. 2A is a cross sectional view of the optical implantable member 102 of FIG. 2 along axis B-B;

[0020] FIG. 3 is an illustration of another exemplary optical implantable member 102 in which optical center 112 of an optic 104 is offset from a geometrical centre 115 of the optic 104, and an indication 302 is provided on the optic 104, in accordance with an embodiment;

[0021] FIG. 3A is an illustration of an exemplary optical implantable member 102, with support members 106 on either side of the optic 104, in which the distance of each of the support members 106, to the geometrical centre 115 of the optic 104 is different, in accordance with an embodiment;

[0022] FIG. 3B is a simplified illustration of the optical implantable member 102 of FIG.

3A received in a capsular bag **304**, in accordance with an embodiment;

[0023] **FIG. 4** is an illustration of the exemplary optical implantable member **102** of **FIG. 1** to be implanted in the eye, in accordance with an embodiment;

[0024] **FIG. 4A** is an illustration of the exemplary optical implantable member **102** (cross section) of **FIG. 1** to be implanted in the eye, in accordance with an embodiment;

[0025] **FIG. 5** is an illustration of the exemplary optical implantable member **102** of **FIG. 1D** restricting the migration of epithelial cells towards the optical centre **112** and the centre of the capsular bag, in accordance with an embodiment; and

[0026] **FIG. 5A** is an illustration of the exemplary optical implantable member **102** of **FIG. 2** restricting the migration of epithelial cells towards the optical centre **112** and the centre of the capsular bag, in accordance with an embodiment.

DETAILED DESCRIPTION

[0027] An embodiment provides an optical implantable member for implantation inside the eye. The optical implantable member reduces the possibility of formation of secondary cataract. The optical implantable member may be an intraocular lens that includes an optic and a plurality of support members. The intraocular lens may be configured to be placed over a posterior wall of the capsular bag of the eye. The optic portion of the intraocular lens may be held against the wall of the capsular bag by means of the support members. The intraocular lens may include a barrier. The barrier may be in the form of a protrusion provided around the optical centre of the optic and away from the periphery of the optic. The protrusion may be concentric to the optical axis of the optic. The protrusion forms a barrier around the central region of the capsular bag, thereby restricting epithelial cells from migrating towards a central region of the capsular bag. Such restriction on migration of the epithelial cells mitigates formation of secondary cataract. This barrier is seen as a circle to the surgeon and helps him in better centring/positioning of the optical implantable member.

[0028] Another embodiment provides an optic that is oblong. For example, the optic may be elliptical or oval. The optic may be asymmetric with respect to a vertical axis of the capsular bag. Vertical axis of the capsular bag is defined as an imaginary line dividing the capsular bag into two equal halves. The vertical axis of the capsular bag may be offset from a vertical axis of the optic, once the optical implantable member is inserted in the capsular bag. The support members are on either sides of the horizontal axis of the capsular bag, thereby enabling the optic to settle asymmetrically in the capsular bag, more on nasal side to ameliorate negative dysphotopsia. The optical centre of the optic is at an offset to its

geometrical centre and is towards the nasal side. Thus, optical centre of the optic aligns with visual axis and decreases aberrations and improves quality of vision.

[0029] Further, an indication may be provided on the optic to enable identification of a side of the optic towards which the optical centre is offset. The indication also enables a surgeon to place the optic inside the capsular bag such that, it settles more on nasal side of capsular bag thereby ameliorating negative dysphotopsia.

[0030] The following detailed description includes references to the accompanying drawings, which form part of the detailed description. The drawings show illustrations in accordance with example embodiments. These example embodiments are described in enough detail to enable those skilled in the art to practice the present subject matter. However, it will be apparent to one of ordinary skill in the art that the present invention may be practiced without these specific details. In other instances, well-known methods, procedures and components have not been described in detail so as not to unnecessarily obscure aspects of the embodiments. The embodiments can be combined, other embodiments can be utilized or structural and logical changes can be made without departing from the scope of the invention. The following detailed description is, therefore, not to be taken as a limiting sense.

[0031] In this document, the terms “a” or “an” are used, as is common in patent documents, to include one or more than one. In this document, the term “or” is used to refer to a nonexclusive “or,” such that “A or B” includes “A but not B,” “B but not A,” and “A and B,” unless otherwise indicated.

EXEMPLARY OPTICAL IMPLANTABLE MEMBER

[0032] Now referring to the figures and more specifically to **FIGs. 1 to 1D**, an embodiment discloses an optical implantable member **102** for implantation inside the eye. The optical implantable member **102** reduces the chances of secondary cataract formation. The optical implantable member **102** may be an intraocular lens. The optical implantable member **102** may include an optic **104** and a plurality of support members **106**. The optic **104** may include an anterior surface **108** and a posterior surface **110**. The optic **104** has an optical centre **112**, an optical axis **114** and a peripheral edge **116**. The support member **106** is configured to hold the optic **104** against the posterior walls of the capsular bag in the eye, thereby preventing displacement of the optic **104** once implanted. One or both of the anterior surface **108** and posterior surface **110** may be spherical, aspherical, toric or multifocal. The

optic **104** of the optical implantable member **102** may be a portion of the optical implantable member **102** having optical properties.

[0033] In an embodiment, the optic **104** of the optical implantable member **102** may be in the shape of an oblong or ellipse. The optic **104** has a horizontal axis **111** and a vertical axis **113**, passing through a geometric centre **115** of the optic **104**. The oblong shaped optic **104** may have a greater length along the horizontal axis **111** as compared to the length along the vertical axis **113**. For example, the length of the oblong along the vertical axis **113** may measure 5.8 mm and the length of the oblong along the horizontal axis **111** may measure 6.2 mm. As an example, the shape of the optic **104** may be defined by two parallel edges connected by an arc on each side. The parallel edges may be separated by a distance of 5.8 mm. In other words, the length of the optic **104** along the vertical axis may be 5.8 mm. The largest distance between two arcs may be 6.2 mm.

[0034] In an embodiment, the capsular bag has a horizontal axis **117** and a vertical axis **118** (shown in **FIG. 3A** and **3B**). Vertical axis **118** of the capsular bag is defined as an imaginary line dividing the capsular bag into two equal halves. The horizontal axis **117** and the vertical axis **118** of the capsular bag intersect at a geometrical centre **119** of the capsular bag.

[0035] In an embodiment, (also referring to **FIGs. 3A** and **3B**), the vertical axis **118** of the capsular bag may be offset from the vertical axis **113** of the optic **104** when the optical implantable member **102** is implanted in the capsular bag. The horizontal axis **117** of the capsular on the other hand, may coincide with the horizontal axis **111** of the optic **104** once the optical implantable member **102** is implanted in the capsular bag. The vertical axis **113** of the optic **104** may be towards the nasal side or towards the temporal side with respect to the vertical axis **118** of the capsular bag once the optical implantable member **102** is implanted.

[0036] In an embodiment, the geometrical centre **115** of the optic **104** may be offset from the geometrical centre **119** of the capsular bag of the eye along the horizontal axis **117** (or **111**), when the optical implantable member **102** is implanted in the capsular bag. The geometrical centre **115** of the optic **104** may be towards the nasal side or towards the temporal side with respect to the geometrical centre **119** of the capsular bag once the optical implantable member **102** is implanted.

[0037] The vertical axis **118** of the capsular bag divides the optic **104** into two asymmetric portions (shown in **FIG. 3A** and **3B**). For example, one edge of the optic **104**, on the horizontal axis **111** may measure 3.2 mm, from the vertical axis **118** of the capsular bag,

and another edge on the horizontal axis **111**, may measure 3 mm from the vertical axis **118** of the capsular bag, once the optical implantable member **102** is implanted in the capsular bag.

[0038] In an embodiment, the longer side on the horizontal axis **111** of the optic **104**, as measured from the vertical axis **118** of the capsular bag, may be on the nasal side. This configuration may help in correcting negative dysphotopsia, thereby shifting the optical centre **112** towards nasal side after insertion into the capsular bag.

[0039] In an embodiment the optic **104** is designed such that its optical centre **112** is offset from its geometrical centre **115** along the horizontal axis **111** of the optic **104** and is towards the nasal side. The optical centre **112** may be away from the geometric centre **115** in either direction and to any extent. Such a configuration may be useful in achieving better alignment of optical centre **112** of the optic **104** with visual axis, thereby decreasing the aberrations and improving quality of vision. The optical centre **112** of the optic **104** may be offset from the geometrical centre **115** along the horizontal axis **111** to compensate angle kappa to any extent as desirable.

[0040] The optic **104** of the optical implantable member **102** is made of suitable transparent material with appropriate refractive index which is bio-compatible to human eye. This material for example can be hydrophilic acrylic, hydrophobic acrylic, silicon, hydrogel or PMMA.

[0041] The optic **104** of the optical implantable member **102** may also have some dye incorporated in its material to block particular wavelength of visible spectrum. The optic **104** of the optical implantable member **102** may also be photo chromatic, which means that it becomes pigmented on exposure to light. The optic **106** of the optical implantable member **102** has some focusing power which is usually converging but may also be diverging in some case.

[0042] The focusing power may be on the anterior surface **108** of the optic **104** of the optical implantable member **102**. The focusing power may also be on the posterior surface **110** of the optic **104** of the optical implantable member **102**. Further, the focusing power may be on both surfaces of the optic **104** of the optical implantable member **102**.

[0043] In an embodiment, the surface of the optic **104** of the optical implantable member **102** may be constructed to provide benefits like asphericity to correct aberrations, or toricity to correct cylindrical power also called astigmatism or multifocality to provide pseudo accommodation and increasing or decreasing the stickiness of the surface, among others.

[0044] In an embodiment, the optical implantable member **102** includes a barrier **202** (also shown in **FIG. 1A**). The barrier **202** may be formed by a protrusion **202**. The protrusion **202** may be concentric to the optical axis **114** of the optic **104**. The protrusion **202** may extend from the posterior surface **110** of the optical implantable member **102** towards a direction away from the posterior surface **110**.

[0045] The protrusion **202** may be in the form of a solid cylinder or disc, and may be concentric to the optical axis **114** of the optical implantable member **102**. Such a configuration enables tracking of the optical centre **112** during implantation. The protrusion **202** is away or at a distance from the peripheral edge **116** of the optic **104**. An outer wall **204** of the protrusion **202** faces the peripheral edge **116** of the optic **104**. In other words, the outer wall **204** or confining structure of the protrusion **202** is between the optical centre **112** and the peripheral edge **116**.

[0046] In an embodiment, the diameter of the protrusion **202** ranges between 2.00 mm and 5.00 mm.

[0047] In another embodiment, preferably, the diameter of the protrusion **202** ranges between 3.0 mm and 4.00 mm.

[0048] In yet another embodiment, more preferably, the diameter of the protrusion **202** is 3.50 mm.

[0049] The protrusion **202** may have a height extending away from the posterior surface **110** of the optic **104**, along the optical axis **114** of the optic **104**.

[0050] In an embodiment, the height of the protrusion **202** may range between 1 micron and 8 microns.

[0051] In another embodiment, preferably, the height of the protrusion **202** may range between 2 microns and 6 microns.

[0052] In yet another embodiment, more preferably, the height of the protrusion **202** is 2 microns.

[0053] In an embodiment, the outer wall **204** of this protrusion **202** is parallel to the optical axis **114** of the optic **104**.

[0054] In another embodiment, the outer wall **204** of the protrusion **202** is angular to the optical axis **114** of the optic **104**.

[0055] The protrusion **202** is constructed such that the posterior surface of the protrusion **202** remains in contact with or adheres to the posterior wall of the capsular bag when implanted.

[0056] Referring to **FIGs. 2** and **2A**, the protrusion **202** that forms the barrier **202** may be in the shape of a ring. As an example, the protrusion **202** may resemble the shape of a circular ring. It may be noted that the protrusion **202**, as an example, can resemble a shape that may resemble a ring (ex: polygon). The circular ring structure of the protrusion **202** may have an inner diameter (ID) and an outer diameter (OD).

[0057] In an embodiment, the ID of the protrusion **202** ranges between 2.00 mm and 5.00 mm.

[0058] In another embodiment, preferably, the ID of the protrusion **202** ranges between 3.00 mm and 4.00 mm.

[0059] In yet another embodiment, more preferably, the ID of the protrusion **202** is 3.50 mm.

[0060] The protrusion **202** may have a height extending away from the posterior surface **110** of the optic **104**, along the optical axis **114** of the optic **104**.

[0061] In an embodiment, the height of the protrusion **202** may range between 1 micron and 8 microns.

[0062] In another embodiment, preferably, the height of the protrusion **202** may range between 2 microns and 6 microns.

[0063] In yet another embodiment, more preferably, the height of the protrusion **202** is 2 microns.

[0064] The protrusion **202** defines an inner wall **206** and an outer wall **208**. The inner wall **204** faces the optical centre **112** and the outer wall **208** faces the peripheral edge **116**.

[0065] In an embodiment the inner wall **206** and the outer wall **208** may be parallel to the optical axis **114**.

[0066] In an embodiment, at least the outer wall **208** is at an angle with respect to the optical axis **114**.

[0067] In an embodiment, at least the inner wall **206** is at an angle with respect to the optical axis **114**.

[0068] In an embodiment, the protrusion **202** that forms the barrier **202** may be in the shape of an ellipse (as opposed to circular) especially in those optical implantable members **102** whose optic **104** has toric power or cylindrical power.

[0069] Referring to **FIG. 3**, a mark or indication **302** is provided near the peripheral edge **116** of the optic **104** to enable identification of a side of the optic **104** towards which the

optical centre **112** is offset. The mark or indication **302** may be a permanent mark or an erasable mark.

[0070] In an embodiment, the optical centre **112** of the optic **104** may be offset from the geometrical centre **115** towards the nasal side, thereby shifting the optical centre **112** towards the nasal side of capsular bag once inserted. The optical centre **112** of the optic **104** may be offset from the geometrical centre **115** along the horizontal axis **111** to compensate angle kappa to any extent as desirable. Such configurations may be useful in decreasing the aberrations and improving quality of vision by better alignment of optical centre **112** of optic **104** with visual axis.

[0071] For those patients whose line of sight is away from the centre of pupil and is towards the nose, the optical implantable member **102** is implanted such that the mark **302** on the optic **104** is on the nasal side (side of the nose).

[0072] For those patients whose line of sight is towards the ear from the centre of pupil, the optical implantable member **102** is implanted such that the mark **302** on the optic **104** is on the temporal side (side of the ear).

[0073] Referring to **FIG. 3A**, a pair of support members **106** (also referred to as haptic) may be provided on either edge of the optic **104**, on either sides of the horizontal axis **111**. In an embodiment, the distance of the support member **106**, which is provided on an upper side of the horizontal axis **111**, to the geometrical centre **115** of the optic **104**, is different from distance of the support member **106**, which is provided on a lower side of the horizontal axis **111**, to the geometrical centre **115** of the optic **104**.

[0074] The support members **106** may be disposed asymmetrically with respect to the geometrical centre **115** of the optic **104** and the vertical axis **113** of the optic **104**. The placement of the support members **106** may however be symmetric with respect to the vertical axis **118** and the geometrical centre **119** of the capsular bag. In other words, the support members **106** may be equidistant from the geometric centre **119** of capsular bag **304** (**FIG. 3B**).

[0075] Referring to **FIG. 3B**, the optical implantable member **102** may be received in the capsular bag **304**. The vertical axis **118** divides the optic **104** asymmetrically once the optical implantable member **102** is implanted in the capsular bag **304**, thereby making the placement of the support members **106** asymmetric to the same extent in relation to the geometric centre **115** and the vertical axis **113** of the optic **104**. Such a configuration enables the optic **104** to settle asymmetrically within the capsular bag **304**. The optic **104** settles more on nasal side,

to ameliorate negative dysphotopsia once the optical implantable member **102** is placed in the capsular bag **304**.

[0076] Referring to **FIGs. 4** and **4A**, the optical implantable member **102** is implanted inside the capsular bag of the eye to replace the natural lens. The anterior surface of the capsular bag is opened to remove the natural lens and insert the optical implantable member **102**. The optical implantable member **102** may be folded and inserted into the capsular bag through a very small incision made on the cornea. The posterior wall of the capsular bag remains intact to support the optic **104** of the optical implantable member **102**. The posterior surface **110** of the optic **104** faces the posterior wall of the capsular bag.

[0077] Referring to **FIG. 5**, the optical implantable member **102**, with the protrusion **202** as illustrated in **FIG. 1D**, which is in the form of a solid cylinder or disc, covers the central region of the posterior wall of the capsular bag. The protrusion **202** is held against the posterior wall of the capsular bag **304** such that penetration/migration of residual lens epithelial cells and fibres towards the central region of the capsular bag is restricted, thereby reducing or delaying the chances of after- cataract formation. Referring to **FIG. 5A**, the optical implantable member **102**, with the protrusion **202** as illustrated in **FIG. 2**, which is in the shape of a ring, covers the central region of the posterior wall of the capsular bag.

[0078] The optical implantable member **102** may have to be placed such that the optical centre **112** of the optic **104** is in line with the visual axis. The alignment of the implanted optical implantable member **102** may be achieved by techniques well known in the art, such as, rotating the optical implantable member **102** inside the capsular bag. The protrusion **202** which is visible through the anterior surface **108** of the optic **104** as a circle is used as a reference to track the optical centre **112** of the optic **104**. As this ring is concentric to the optical axis **114** of the optic **104** co-axially sighted light reflex is brought in the centre of the circle. The surgeon is also guided by permanent indication marks that may be provided on the peripheral edge **116** of the optic **104** of the optical implantable member **102**.

[0079] In an embodiment, temporary indication marks may be provided on the optical centre **112** or around the optical centre **112** of the optic **104** of the optical implantable member **102**. Such a configuration of the optic **104** may enable the surgeon to track the optical centre **112** of the optic **104** even in case of a constricted pupil. In case of toric Intraocular Lens, these temporary marks may help in proper alignment of toric lens with corneal marks in constricted pupil.

[0080] Some of the embodiments may also apply to optical implantable members **102**

implanted in the ciliary sulcus or anterior chamber of the eye. Some of the embodiments may also apply to optical implantable members **102** clawed to the front or back surface of the iris of the eye or fixated to the sclera by stitches or glue. In some instances artificial lens can also be implanted without removal of natural lens for the purpose of correction of refractive power then it is called phakic Intraocular Lens and some embodiments of this invention may also apply to these.

[0081] Embodiments provide an optical implantable member for implantation inside the eye. The optical implantable member significantly reduces the chances of secondary cataract formation.

[0082] Embodiments provide an optical implantable member, such as, an intraocular lens including barrier formed by protrusion towards the central region of the lens, wherein the barrier is configured to adhere to the posterior wall of a capsular bag of the eye thereby forming a blockage that restricts migration of residual lens epithelial cells and fibres towards a central region of the capsular bag, which are among the factors responsible for formation of secondary cataract.

[0083] Embodiments provide an optical implantable member that has an asymmetric optic designed to ameliorate negative dysphotopsia.

[0084] Embodiments provide an optical implantable member, in which the optical centre of the optic is offset from the geometrical centre of the optic and also the geometrical centre of the capsular bag, designed in order to decrease aberrations and achieve proper alignment of the optical centre of the optical implantable member with the visual axis.

[0085] It shall be noted that the processes described above is described as sequence of steps, this was done solely for the sake of illustration. Accordingly, it is contemplated that some steps may be added, some steps may be omitted, the order of the steps may be re-arranged, or some steps may be performed simultaneously.

[0086] Although embodiments have been described with reference to specific example embodiments, it will be evident that various modifications and changes may be made to these embodiments without departing from the broader spirit and scope of the system and method described herein. Accordingly, the specification and drawings are to be regarded in an illustrative rather than a restrictive sense.

[0087] Many alterations and modifications of the present invention will no doubt become apparent to a person of ordinary skill in the art after having read the foregoing description. It is to be understood that the phraseology or terminology employed herein is for the purpose of

description and not of limitation. It is to be understood that the description above contains many specifications, these should not be construed as limiting the scope of the invention but as merely providing illustrations of some of the personally preferred embodiments of this invention. Thus the scope of the invention should be determined by the appended claims and

5 their legal equivalents rather than by the examples given.

CLAIMS

I claim:

1. An optical implantable member comprising:

An optic, comprising an anterior surface and a posterior surface, wherein the optic has a peripheral edge and an optical centre, wherein the optical implantable member is configured to be placed within a capsular bag of the eye; and

a barrier formed by a protrusion on the posterior surface, wherein the protrusion is concentric to an optical axis of the optic, wherein an outer wall of the protrusion is between the peripheral edge and the optical centre, whereby the barrier restricts epithelial cells from migrating towards a central region of the capsular bag.

2. The optical implantable member according to claim 1, wherein the protrusion is a solid cylinder having a height extended from the posterior surface of the optic.

3. The optical implantable member according to claim 1, wherein the protrusion resembles a ring having a height extended from the posterior surface of the optic.

4. The optical implantable member according to any one of claim 2 and 3, wherein diameter of the protrusion ranges between 2.00 mm and 5.00 mm.

5. The optical implantable member according to any one of claim 2 and 3, wherein diameter of the protrusion ranges between 3.00 mm and 4.0 mm.

6. The optical implantable member according to claim 1, wherein height of the protrusion ranges between 1 micron and 8 microns.

7. The optical implantable member according to claim 1, wherein height of the protrusion ranges between 2 micron and 6 microns.

8. The optical implantable member according to claim 1, wherein the outer wall is parallel to or at an angle to the optical axis.

9. The optical implantable member according to claim 1, wherein the protrusion defines an inner wall, wherein the inner wall faces the optical centre and the outer wall faces the peripheral edge of the optic, wherein at least one of the inner wall and the outer wall is angular to the optical axis of the optic.

10. The optical implantable member according to claim 1, wherein the protrusion defines an inner wall, wherein the inner wall faces the optical centre and the outer wall faces the

peripheral edge of the optic, wherein at least one of the inner wall and the outer wall is parallel to the optical axis of the optic.

11. The optical implantable member according to claim 1, wherein the length of the optic along a horizontal axis is greater than the length along a vertical axis of the optic.
- 5 12. The optical implantable member according to claim 1, wherein the optic is asymmetric with respect to a vertical axis of the capsular bag once the optical implantable member is implanted in the capsular bag.
13. The optical implantable member according to claim 1, wherein the optical centre is offset from a geometrical centre of the optic.
- 10 14. The optical implantable member according to claim 1, further comprising an indication on the optic to enable identification of a side of the optic towards which the optical centre is offset.
- 15 15. The optical implantable member according to claim 1, further comprising at least two support members, wherein at least one support member is provided on either sides of a horizontal axis of the optic, wherein distance of the support member, which is provided on an upper side of the horizontal axis, to a geometrical centre of the optic, is different from distance of the support member, which is provided on a lower side of the horizontal axis, to the geometrical centre of the optic.

1. An optical implantable member comprising:

an optic, comprising an anterior surface and a posterior surface, wherein the optic has a peripheral edge and an optical centre, wherein the optical implantable member is configured to be placed within a capsular bag of the eye;

at least two support members, wherein distance of the at least one support member, which is provided on an upper side of the horizontal axis, to a geometrical centre of the optic, is different from distance of the at least one support member, which is provided on a lower side of the horizontal axis, to the geometrical centre of the optic; and

a barrier formed by a protrusion on the posterior surface, wherein the protrusion is concentric to an optical axis of the optic, wherein an outer wall of the protrusion is between the peripheral edge and the optical centre, whereby the barrier restricts epithelial cells from migrating towards a central region of the capsular bag;

2. The optical implantable member according to claim 1, wherein the protrusion is a solid cylinder having a height extended from the posterior surface of the optic.

3. The optical implantable member according to claim 1, wherein the protrusion resembles a ring having a height extended from the posterior surface of the optic.

4. The optical implantable member according to any one of claim 2 and 3, wherein diameter of the protrusion ranges between 2.00 mm and 5.00 mm.

5. The optical implantable member according to any one of claim 2 and 3, wherein diameter of the protrusion ranges between 3.00 mm and 4.0 mm.

6. The optical implantable member according to claim 1, wherein height of the protrusion ranges between 1 micron and 8 microns.
7. The optical implantable member according to claim 1, wherein height of the protrusion ranges between 2 micron and 6 microns.
8. The optical implantable member according to claim 1, wherein the outer wall is parallel to or at an angle to the optical axis.
9. The optical implantable member according to claim 1, wherein the protrusion defines an inner wall, wherein the inner wall faces the optical centre and the outer wall faces the peripheral edge of the optic, wherein at least one of the inner wall and the outer wall is angular to the optical axis of the optic.
10. The optical implantable member according to claim 1, wherein the protrusion defines an inner wall, wherein the inner wall faces the optical centre and the outer wall faces the peripheral edge of the optic, wherein at least one of the inner wall and the outer wall is parallel to the optical axis of the optic.
11. The optical implantable member according to claim 1, wherein the length of the optic along a horizontal axis is greater than the length along a vertical axis of the optic.
12. The optical implantable member according to claim 1, wherein the optic is asymmetric with respect to a vertical axis of the capsular bag once the optical implantable member is implanted in the capsular bag.

13. The optical implantable member according to claim 1, wherein the optical centre is offset from a geometrical centre of the optic.
14. The optical implantable member according to claim 1, further comprising an indication on the optic to enable identification of a side of the optic towards which the optical centre is offset.
15. The optical implantable member according to claim 1, wherein at least one support member is provided on either sides of a horizontal axis of the optic.

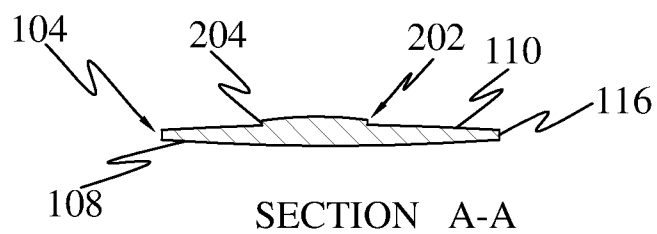
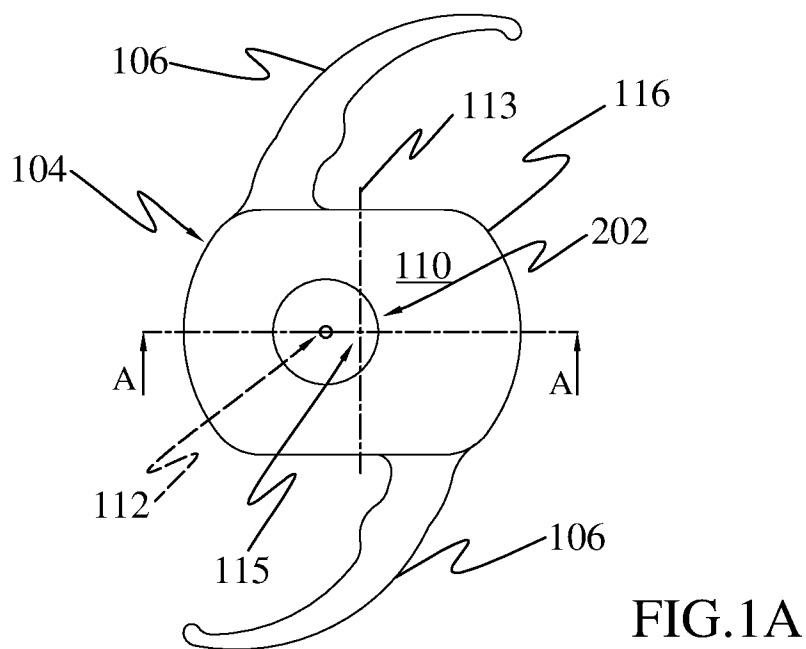
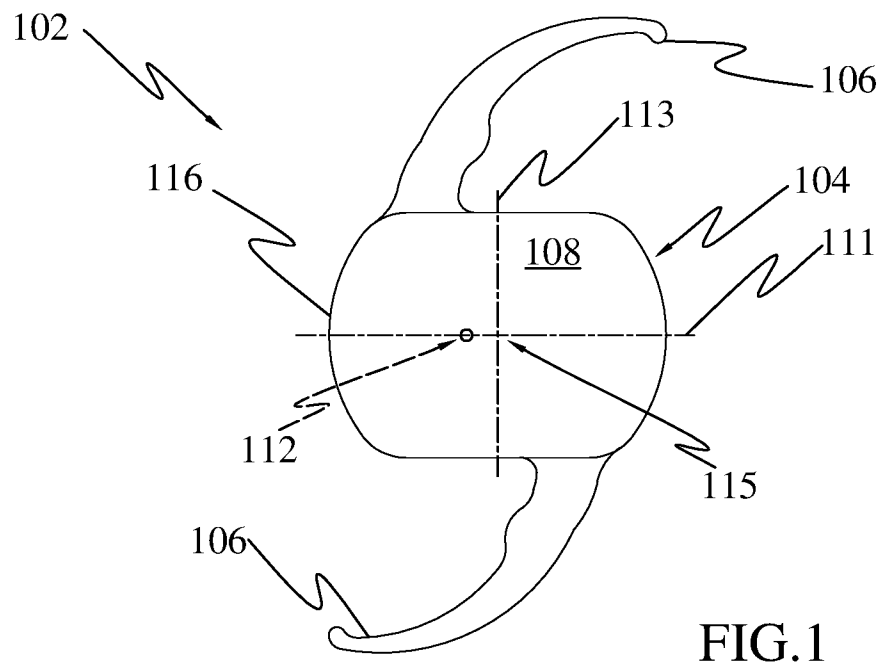
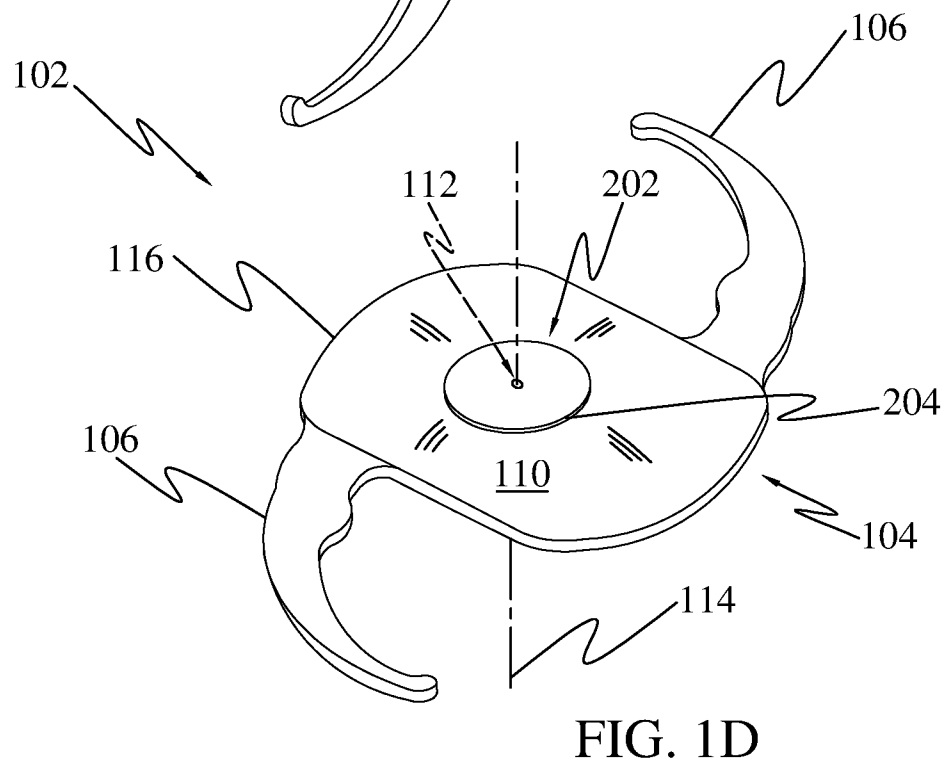
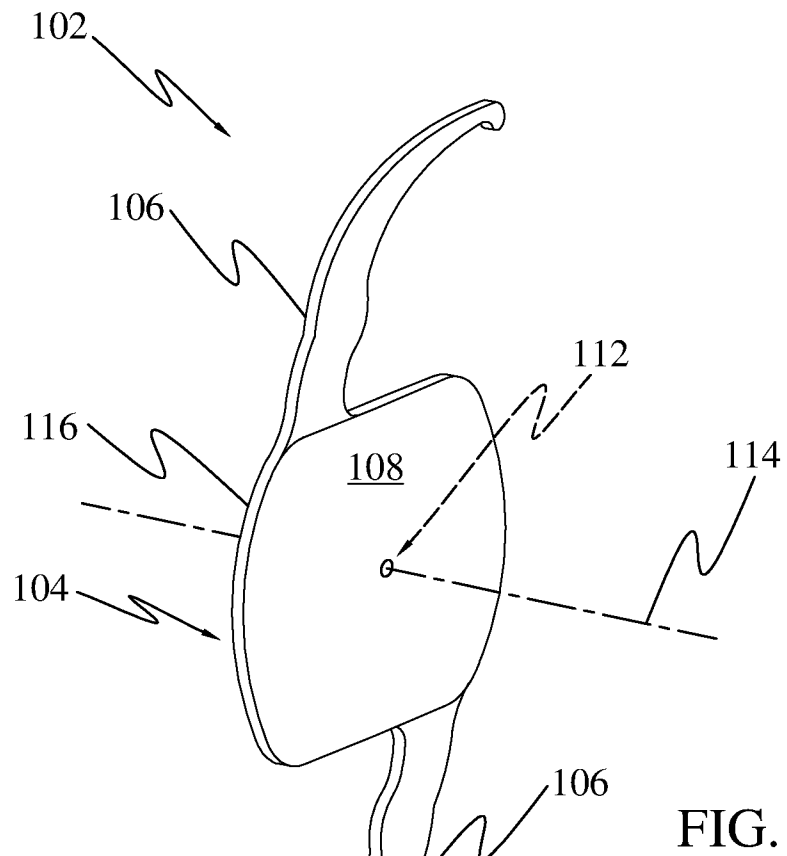


FIG.1B




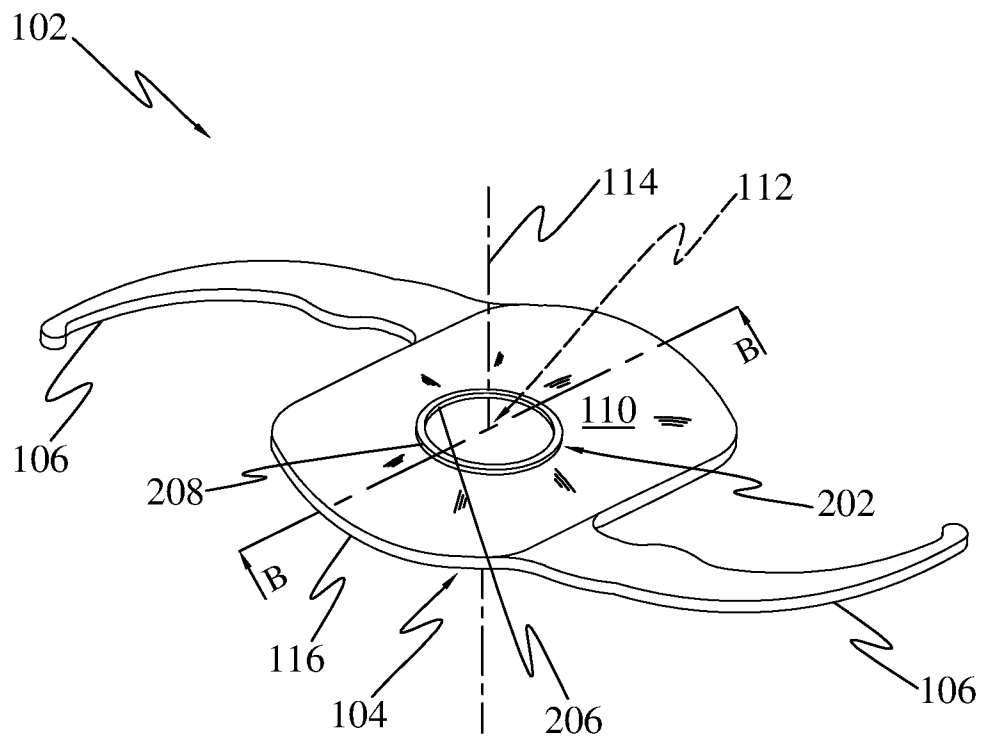


FIG. 2

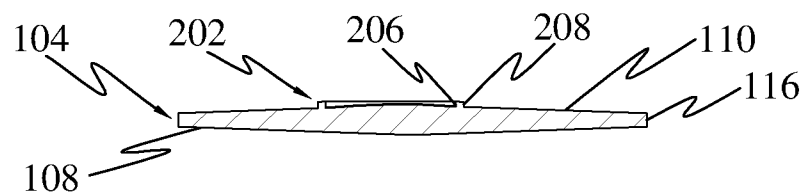

SECTION B-B

FIG. 2A

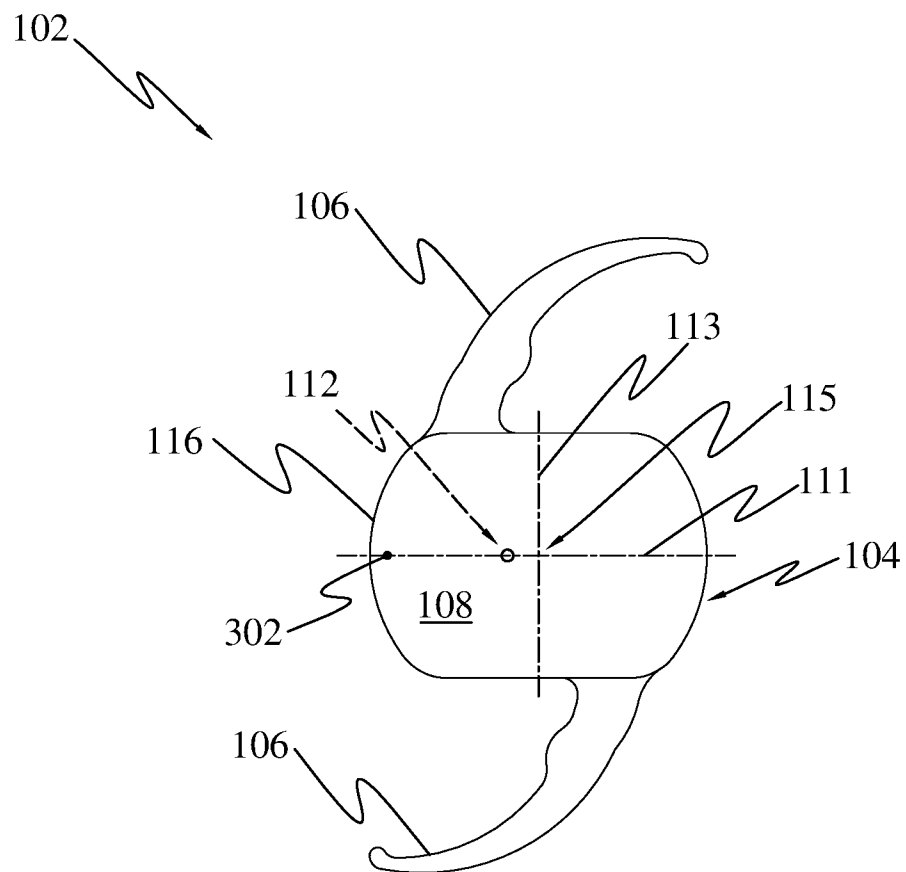


FIG. 3

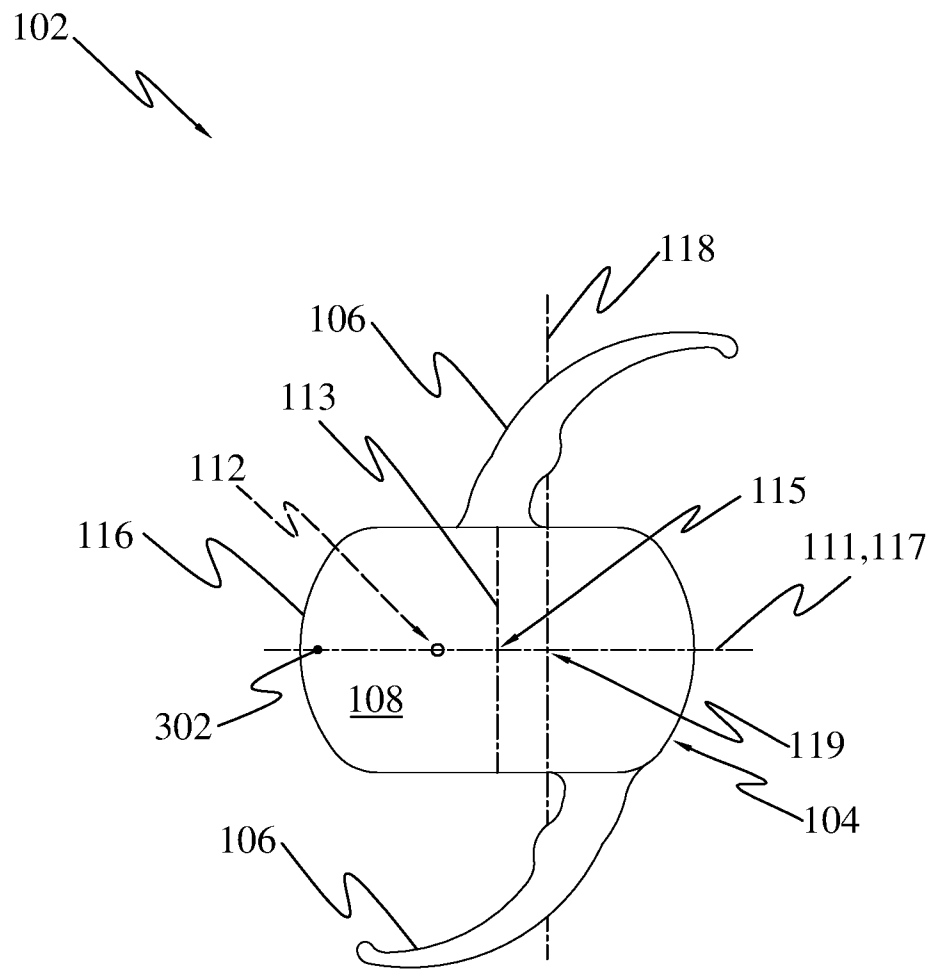


FIG. 3A

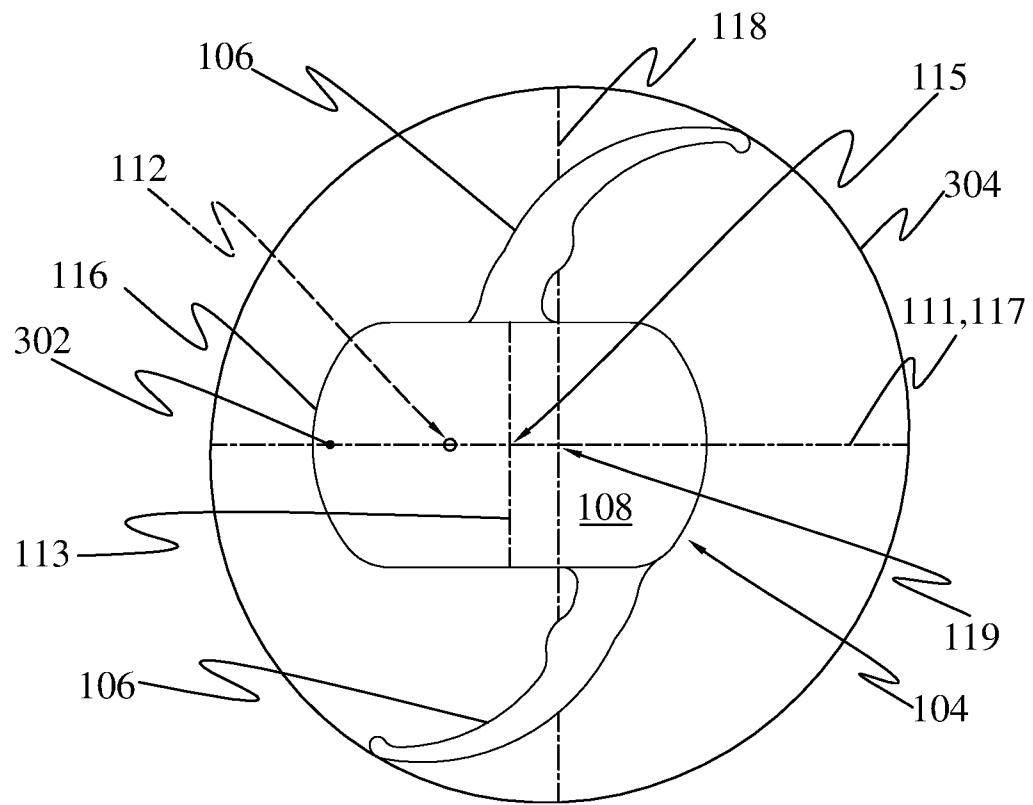


FIG. 3B

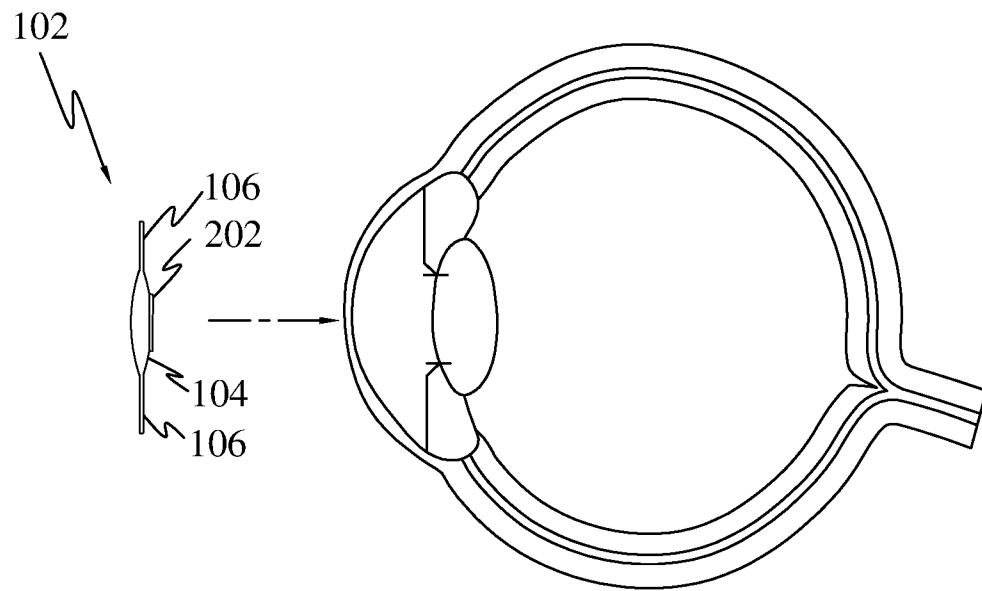


FIG. 4

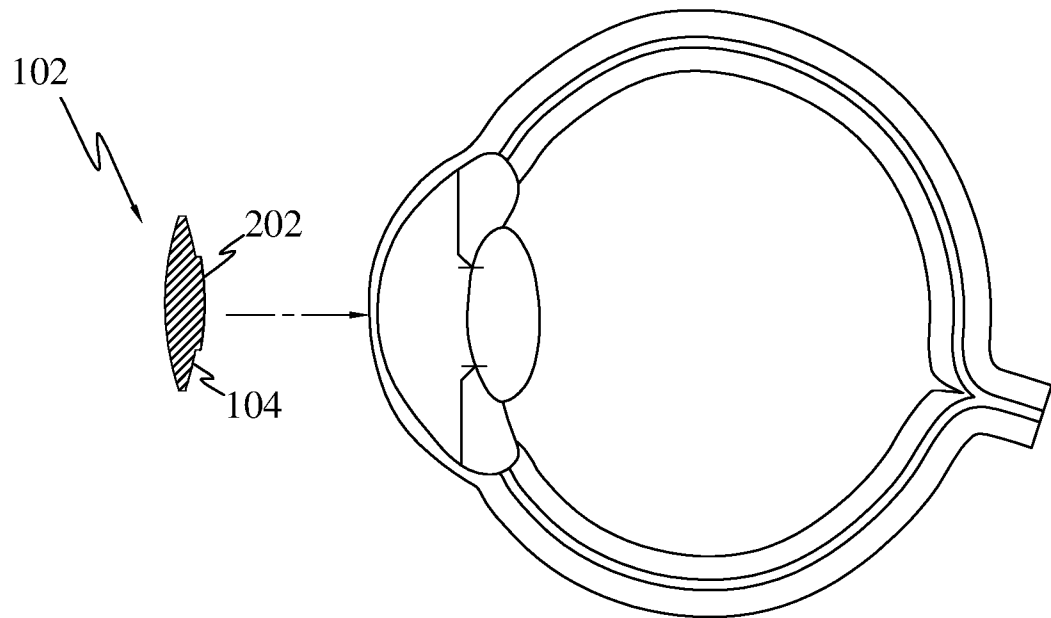


FIG. 4A

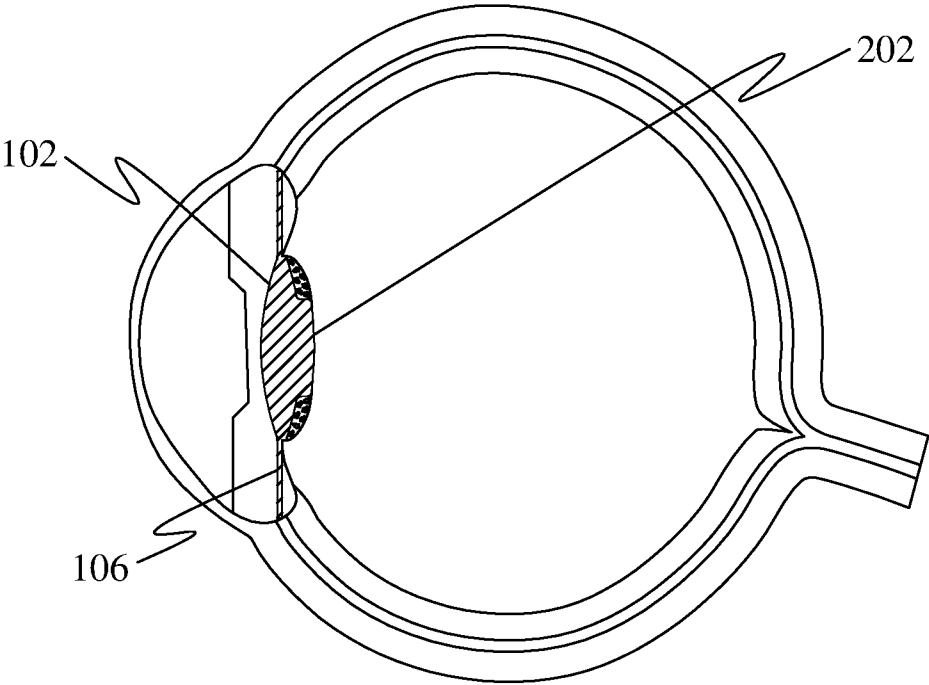


FIG. 5

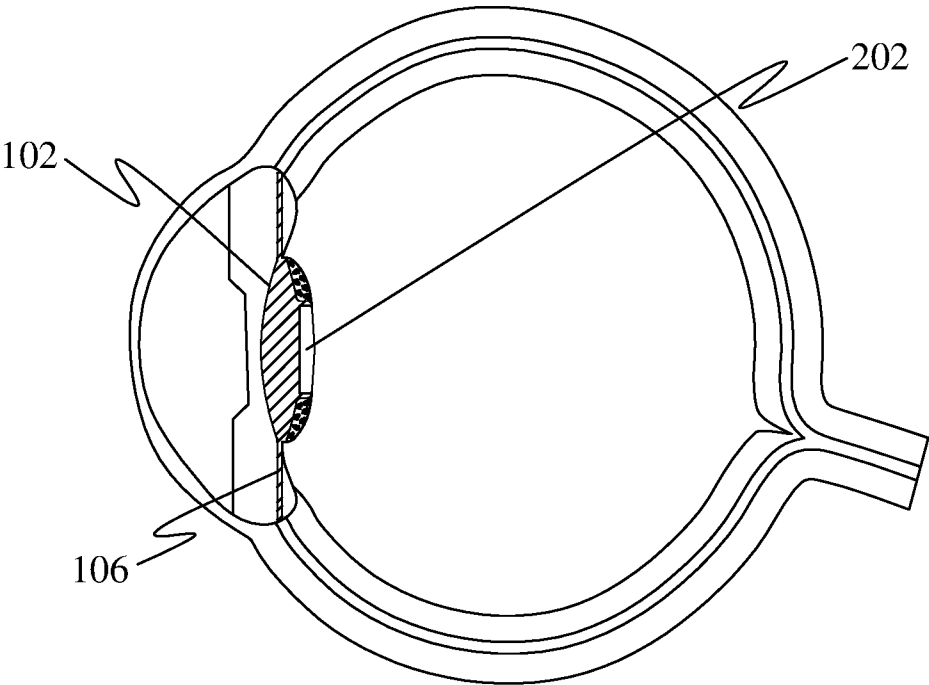


FIG. 5A

INTERNATIONAL SEARCH REPORT

International application No.
PCT/IB2015/056159

A. CLASSIFICATION OF SUBJECT MATTER
A61F9/00, A61B3/00 Version=2015.01

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B, A61F.

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

DATABASES: PATSEER, IPO INTERNAL.

SEARCH TERMS: INTRA OCULAR LENS, OPTIC, EPITHELIAL, PROTRUSION, CAPSULAR BAG.

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 2384166 A2 (Bausch & Lomb Incorporated) 9 November 2011 Abstract, Figures 1-12 and Paragraphs 0020-0033. -----	1-15
X	US 6881225 B2 (Kiyoshi Okada) 19 April 2005 Abstract, Figures 1-14 and Claims 1-14. -----	1-15
X	WO 2008036671 A1 (Advanced Medical Optics Inc, Jim Deacon, Rakhi Jain, Leander Zickler) 27 March 2008 Abstract, Figures 1-11 and Pages 5-19.	1-15

☐ Further documents are listed in the continuation of Box C. ☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

13-10-2015

Date of mailing of the international search report

13-10-2015

Name and mailing address of the ISA/

Indian Patent Office
Plot No.32, Sector 14, Dwarka, New Delhi-110075
Facsimile No.

Authorized officer

Swati Pandey

Telephone No. +91-1125300200

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IB2015/056159

Citation	Pub.Date	Family	Pub.Date
EP EP 2384166 A2	09-11-2011	CA 2744934 A1	17-06-2010
		CN 102245128 A	16-11-2011
		JP 2012511404 A	24-05-2012
		US 2010152846 A1	17-06-2010
		WO 2010068608 A3	11-11-2010
US 6881225 B2	19-04-2005	AU 8002601 A	13-02-2002
		WO 0209619 A3	02-05-2002
WO WO 2008036671 A1	27-03-2008	AT 473708 T	15-07-2010
		AU 2007299913 B2	13-02-2014
		CA 2664104 C	03-02-2015
		EP 2079398 B1	14-07-2010
		US 2008077238 A1	27-03-2008