



- (51) **International Patent Classification:**
G01S 7/52 (2006.01) *GI 0K 11/34* (2006.01)
G01S 15/89 (2006.01)
- (21) **International Application Number:**
 PCT/EP20 17/07 1940
- (22) **International Filing Date:**
 01 September 2017 (01.09.2017)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
 62/382856 02 September 2016 (02.09.2016) US
- (71) **Applicant:** KONINKLIJKE PHILIPS N.V. [NL/NL];
 High Tech Campus 5, 5656 AE Eindhoven (NL).
- (72) **Inventor:** SAVORD, Bernard Joseph; High Tech Campus
 5, 5656 AE Eindhoven (NL).
- (74) **Agent:** STEFFEN, Thomas et al; Philips International
 B.V. - Intellectual Property & Standards High Tech Cam-
 pus 5, 5656 AE Eindhoven (NL).
- (81) **Designated States (unless otherwise indicated, for every
 kind of national protection available):** AE, AG, AL, AM,
 AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
 CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
 DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,

HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,
 KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,
 MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
 OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
 SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
 TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) **Designated States (unless otherwise indicated, for every
 kind of regional protection available):** ARIPO (BW, GH,
 GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,
 UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
 TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
 EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
 MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
 TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
 KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:
 — as to applicant's entitlement to apply for and be granted a
 patent (Rule 4.1 7(H))

Published:
 — with international search report (Art. 21(3))

(54) **Title:** ULTRASOUND PROBE WITH LOW FREQUENCY, LOW VOLTAGE DIGITAL MICROBEAMFORMER

(57) **Abstract:** An ultrasound probe (106) contains an array transducer (101) and a microbeamformer coupled to elements of the array. The microbeamformer comprises analog ASICs (102) with transmitters and amplifiers coupled to elements of the array (101). The microbeamformer also comprises analog to digital converters which convert received echo signals to digital data, and digital beamforming circuitry located in digital ASICs (103). The digital ASICs (103) are clocked at a lower core frequency than that of which the digital integrated circuit process of the digital ASICs (103) is capable, and the digital ASICs (103) are operated at a lower supply voltage than that for which the digital integrated circuit process is designed, both of which reduce power consumption by the microbeamformer.

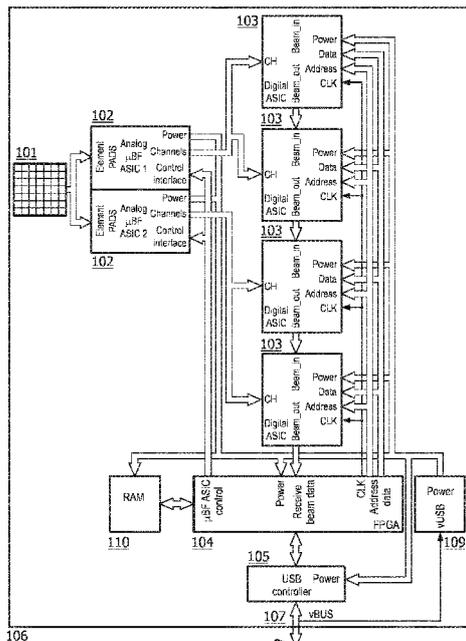


FIG. 2



ULTRASOUND PROBE WITH LOW FREQUENCY,
LOW VOLTAGE DIGITAL MICROBEAMFORMER

5 This invention relates to medical diagnostic
ultrasound systems and, in particular, to ultrasound
probes with digital microbeamformers .

10 Ultrasonic array transducers use beamformers to
transmit and appropriately delay and sum the
ultrasonic echo signals received from elements of the
transducer array. The delays are chosen in
consideration of the direction (steering) and focus
depth of the beams to be formed by the beamformer.
After the signals received from each element have
15 been properly delayed by a channel of the beamformer,
the delayed signals are combined to form a beam of
properly steered and focused coherent echo signals.
During ultrasonic beam transmission, the time of
actuation of individual elements is the complement of
the receive delay, steering and focusing the transmit
20 beam. The choice of delays is known to be
determinable from the geometry of the array elements
and of the image field being interrogated by the
beams .

25 In a traditional ultrasound system the array
transducer is located in a probe which is placed
against the body of the patient during imaging and
contains some electronic components such as tuning
elements, switches, and amplification devices. The
delaying and signal combining is performed by the
30 beamformer which is contained in the ultrasound
system mainframe, to which the probe is connected by
a cable.

35 The foregoing system architecture for an array
transducer and a beamformer suffices quite well for
most one dimensional (1D) transducer arrays, where

the number of transducer elements and the number of beamformer channels are approximately the same. When the number of transducer elements exceeds the number of beamformer channels, multiplexing is generally employed and only a subset of the total number of elements of the transducer can be connected to the beamformer at any point in time. The number of elements in a 1D array can range from less than one hundred to several hundred and the typical beamformer has 128 beamformer channels. This system architecture solution became untenable with the advent of two dimensional (2D) array transducers for two and three dimensional (3D) imaging. That is because 2D array transducers steer and focus beams in both azimuth and elevation over a volumetric region. The number of transducer elements needed for this beam formation is usually in the thousands. The crux of the problem then becomes the cable that connects the probe to the system mainframe where the beamformer is located. A cable of several thousand conductors of even the finest conductive filaments becomes thick and unwieldy, making manipulation of the probe cumbersome if not impossible.

A solution to this problem is to perform at least some of the beamforming in the probe itself, as described in US Pat. 5,229,933 (Larson, III) . In the ultrasound system shown in this patent, the beamforming is partitioned between the probe and the system mainframe. Initial beamforming of groups of elements is done in the probe by microcircuitry known as a microbeamformer, where partially beamformed sums are produced. These partially beamformed sums, being fewer in number than the number of transducer elements, are coupled to the system mainframe through a cable of reasonable dimensions, where the

beamforming process is completed and the final beam produced. The partial beamforming in the probe is done by what Larson, III refers to as intragroup processors, in a microbeamformer in the form of microelectronics attached to the array transducer. See also US Pat. 5,997,479 (Savord et al.); US Pat. 6,013,032 (Savord); US Pat. 6,126,602 (Savord et al.); and US Pat. 6,375,617 (Fraser). The thousands of connections between the thousands of elements of the transducer array and the microbeamformer are done at the tiny dimensions of the microcircuitry and the array pitch, while the many fewer cable connections between the microbeamformer and the beamformer of the system mainframe are done by more conventional cable technologies. Various planar and curved array formats can be used with microbeamformers such as the curved arrays shown in US Pat. 7,821,180 (Kunkel, III) and US Pat. 7,927,280 (Davidsen). Microbeamformers can also be used with one dimensional arrays and with 2D arrays operated as one dimensional arrays. See, e.g., US Pat. 7,037,264 (Poland).

For many years now beamforming in an ultrasound system has been done digitally. The received signals are delayed by clocked shift registers or the time of temporary storage in a random access memory and the delayed signals are summed by digital adders. The digital beamforming can be performed in circuitry such as an FPGA (field programmable gate array) or by software instructions in a microprocessor. But to perform the beamforming digitally the received signals must first be digitized by analog to digital converters. In today's commercially available ultrasound probes with microbeamformers, the partial sum signals are formed in the microbeamformer by

operating on the received echo signals in their native analog domain. The analog partial sum signals are coupled to the system mainframe over the probe cable, where they are digitized and beamformation is completed in the digital domain. Recently, the beamforming technology has been integrated even further in the L12-4 linear and the C5-2 curved array probes of Philips Healthcare's Lumify™ ultrasound products. Digitization and digital beamforming is performed by microcircuitry located in the handle of the probe, as is signal detection and image formation by scan conversion. These probes, however, use 1D (one dimensional) array transducers with far fewer transducer elements than those of a 2D array probe for 3D imaging. It would be desirable for the entire beamformation circuitry to be located in the probe for both 1D array (two dimensional imaging) and 2D array (three dimensional imaging) probes.

A problem which must be surmounted when integrating all of the beamforming circuitry in the probe is due to the power consumption by the microcircuitry. This problem is heat dissipation from the circuitry. Since the probe is held by the hand of an ultrasonographer during scanning, all of the heat generated by the internal circuitry of the probe will cause the probe to feel warm to the touch. At times, the probe handle can feel uncomfortably hot to the touch, a problem which must be prevented. Passive probe cooling arrangements have been devised, as well as active systems which convey heat away from the probe where it dissipated away from the user, such as those described in US Pat. pub. no. 2014/0058270 (Davidsen et al.) and US Pat. pub. no. 2015/0099978 (Davidsen et al.) However, such arrangements significantly increase the cost and

complexity of the probe and its cable. It would be desirable to avoid such arrangements by the far simpler expedient of reduced power consumption by the microcircuitry.

5 In accordance with the principles of the present invention, microbeamformer circuitry is described which performs digital beamforming in an ultrasound probe. Low power performance and circuitry packaging efficiency is accomplished by construction of analog-
10 to-digital converters (ADCs) and digital beamforming circuitry in integrated circuit form. Power consumption is also reduced by using a low power digital-to-analog conversion technique such as delta-sigma or successive approximation analog to digital
15 conversion. Power consumption is further reduced by operating digital ICs at a lower frequency than that of which the IC process is capable, and at a low voltage by use of the lower frequency of operation. The combination of these techniques enables the
20 microbeamformer chip set to operate within a power budget of 3 watts or less, thereby avoiding excessive heat generation within the probe.

In the drawings:

25 FIGURE 1 illustrates in block diagram form an ultrasonic imaging system constructed in accordance with the principles of the present invention.

 FIGURE 2 illustrates in block diagram form the microbeamforming circuits and transducer array of an ultrasound probe of the present invention coupled to
30 a portable computer as the display device.

 FIGURE 3 illustrates in block diagram form the components of an analog ASIC of the microbeamformer of FIGURE 2.

35 FIGURE 4 is a circuit diagram of the analog receive delay of the analog ASIC of FIGURE 3.

FIGURE 5 illustrates in block diagram form the components of a digital ADC and beamforming ASIC of FIGURE 3.

5 FIGURE 5a illustrates in block diagram form a successive approximation analog-to-digital converter suitable for use in the digital ASIC of FIGURE 5.

FIGURE 6 illustrates the digital delay, delay control, and summation circuitry of one channel of the digital ASIC of FIGURE 5.

10 FIGURE 7 illustrates the digital FIR (finite impulse response) filter used for sub sample delay in the digital ASIC of FIGURE 5.

15 FIGURE 8 illustrates echo signal waveforms with different delays as produced by the sub sample delay FIR of FIGURE 7.

Referring first to FIGURE 1, an ultrasound system constructed in accordance with the principles of the present invention is shown in block diagram form. A probe 10 has a two dimensional array transducer 12 which may be planar or curved as shown in this example. The transducer may be formed of MUT devices such as CMUTs (capacitive micro-machined ultrasonic transducers) or PVDF, but is preferably formed of a piezoceramic material such as PZT. The elements of the array are coupled to a digital microbeamformer 14 located in the probe behind the transducer array. A microbeamformer is integrated circuitry located in the probe with beamforming channels coupled to elements of the 2D array transducer 12. The microbeamformer applies timed transmit pulses to elements of each group of elements (patch) of the array to transmit beams in the desired directions and to the desired focal points in the image field in front of the array. The profile of the transmit beams in the elevation dimension can

20
25
30
35

exhibit a point focus, a plane wave, or any intermediate beam profile. Echoes returned by cells and tissue from the transmitted beams are received by the array elements and coupled to channels of the
5 microbeamformer 14 where the analog echo signals are individually delayed. The delayed signals from a contiguous patch of transducer elements are combined to form a partial sum signal for the patch. In the analog section of the microbeamformer described more
10 fully below, combining is done by coupling the delayed signals from the elements of the patch to a common bus, obviating the need for summing circuits. The analog echo signals are then digitized and further beamformed in digital form by a digital ASIC
15 (application specific integrated circuit). The beamformed digital signals of each patch are coupled to a system beamformer 22 in an ultrasound system by way of a cable 16, where the beamforming process is completed. Alternatively, in a preferred
20 implementation all of the beamforming is performed by the microbeamformer in the probe, and fully beamformed digital signals coupled to the system mainframe. The beamformed digital signals are used to form an image by a signal and image processor 24,
25 which may perform operations such as baseband detection, harmonic separation, filtering, Doppler processing, and scan conversion for image formation. The signal and image processor 24 produces 2D or 3D images for display on an image display 30. The
30 signal and image processor may comprise electronic hardware components, hardware controlled by software, or a microprocessor executing image processing algorithms. It generally will also include specialized hardware or software which processes
35 received echo data into image data for images of a

desired display format such as a scan converter.

Control of ultrasound system parameters such as probe selection, beam steering and focusing, and signal and image processing is done under control of a system controller 26 which is coupled to various modules of the system and to the microbeamformer in the probe 10 as described more fully below. The system controller may be formed by ASIC circuits or microprocessor circuitry and software data storage devices such as RAMs, ROMs, or disk drives. In the case of the probe 10 some of this control information is provided to the microbeamformer from the system mainframe over data lines of the cable 16, conditioning the microbeamformer for operation of the transducer array as required for the particular scanning procedure. The user controls these operating parameters by means of a control panel 20.

FIGURE 2 illustrates a digital microbeamformer in an ultrasound probe 106 which operates a 2D (two dimensional) matrix array transducer 101 having 8192 transducer elements operated in 128 groups of sixty-four elements configured as 8x8 patches. The microbeamformer in the illustrated implementation comprises two analog ASICS 102, each coupled to half of the elements of the matrix array 101. The analog ASICS contain transmit circuitry, transmit/receive (T/R) switches, preamplifying amplifiers and analog delays as described more fully below. The analog ASICS 102 are coupled to four digital ASICS 103 of the microbeamformer that contain low power analog to digital converters and digital beamforming circuitry. An FPGA 104 receives control data from the user operating a control and display device, show here as a laptop computer 108. The control and display device can alternatively be a cart-borne ultrasound

system, a tablet computer, a PDA, a smartphone, or similar digital device with a display and user interface. The FPGA is coupled to the microbeamformer ASICs to provide control information for ultrasonic transmission and receive beam formation, and also stores data in a RAM (random access memory) 110 and manages a USB controller 105 and a switching power supply 109. The RAM 110 stores all of the control data necessary for each anticipated scanning mode of the probe. For example, the RAM 110 may be coupled to a write address controller to write digital echo signals into the RAM, and to a plurality of read address controllers, each adapted to controlling the reading of delayed digital echo signals for a different digital multiline echo signal. All of these circuits must operate in accordance with a chosen power budget, which is 3.0 watts in this example, in order to maintain a cool handheld probe. An exemplary power budget for the microbeamformer circuits shown in FIGURE 2 is illustrated in Table 1 below.

Table 1: Power draw of FIGURE 2 circuits for conditions indicated		
Component	Operation	Power
Transmit function of Analog ASIC	Transmit with 4096 elements	0.75W
Preamplifier and Delay circuits of Analog ASIC	Receive with 8192 elements, beamform to 128 partial sum signals	0.5W
USB 3.0 controller	3Gb/s data transfer	0.7W
Control FPGA	Data management	0.25W
Power supply	Assumes 90% efficiency	0.3W
Digital ASIC	128 ADCs sampling at 20Mhz and digital beam formation with 8x multiline outputs	0.5W
Total		3.0W

This power budget shows that the entire microbeamformer circuitry, its control FPGA, power

supply, and USB controller operate within a power allocation of 3.0 watts, thereby generating very little heat in the probe. The analog ASICs 102 produce 128 partial sum analog signals from 128 patches of sixty-four elements each, which are the 128 input signals for 128 ADCs in the digital ASICs. The microbeamformer may thus be viewed as a 128-channel digital beamformer. Dividing the power allocation by the number of channels shows that the microbeamformer consumes only about 23 milliwatts per channel. And each digital channel in the preferred implementation produces eight multilines for high frame rate digital imaging, which is a power consumption of only about 3 milliwatts per multiline scanline.

Thus, the ultrasound probe of the present invention provides a plurality of digital channels, wherein the power consumption per single multiline scanline can be as low as 3 milliwatts. In another embodiment, in which each digital channel produces four multilines, the power consumption is below or about 6 milliwatts per multiline scanline.

In the illustrated implementation of FIGURE 2, the acoustic elements of the matrix array transducer 101 are connected directly to element pads of the analog ASICs 102 in a flip chip type interconnect. Control and group output signals are connected between the analog ASICs and the other components of the microbeamformer through a flexible interconnect (e.g., flex circuit) to a printed circuit board containing the other probe circuitry. Other interconnect techniques such as stacked silicon dies, ceramic circuits or multi-chip modules may also be employed. Each analog ASIC has sixty-four channel line outputs (CHANNELS) which conduct partially

beamformed analog signals of sixty-four patches of elements to the channel inputs (CH) of two of the digital ASICs. Each digital ASIC thus processes thirty-two channels of partial sum signals. The FPGA 5 104 supplies control data to the analog ASICs from its μ BF ASIC CONTROL bus to the CONTROL INTERFACE inputs of the analog ASICs 102. The FPGA supplies digital address data and control data to the digital ASICs 103 over ADDRESS and DATA buses, respectively, 10 as well as a clock (CLK) signal. Digital beamformed output signals are propagated and summed from one digital ASIC to the next using BEAM_IN and BEAM_OUT buses connected from ASIC to ASIC until the fully summed digital echo signal is applied from the last 15 ASIC to the RECEIVE BEAM DATA input of the FPGA. The FPGA applies the fully beamformed output signals to the USB controller 105, which then transmits the digital echo signals as serial data over a USB cable 107 to the user control and display system 108. Other 20 high speed digital interfaces such as HDMI or Ethernet can also be used. A suitable USB controller is the FX3.0s controller available from Cypress Semiconductor of San Jose, California. The switched power supply 109 is shown applying necessary power to 25 the POWER inputs of all of the ICs of the microbeamformer .

FIGURE 3 illustrates the components of one channel 300 of the analog ASIC 102. In the illustrated implementation each analog ASIC has 30 components for 4096 analog channels connected to 4096 elements of the matrix array 101. Transmit data (Tx Data) is received by a transmit pulse generator 302 from the FPGA 104. The FPGA has accessed this data from the RAM memory 110 for a desired 35 transmit /receive sequence in response to a command

previously received from the system controller 26, which itself is acting in response to an imaging selection entered by a user on user interface 20. The Tx Data controls parameters of a transmit pulse such as pulse width, transmit delay relative to a time marker, and pulse count. The Tx Data is clocked into the transmit pulse generator 302 which responds by developing the desired sequence of transmit pulse events. The transmit pulse sequence is applied to the input of a high voltage transmitter 304 at the time of a transmit enable signal (Tx Enable). The high voltage transmitter 304 drives an element 101 η of the matrix array with a high voltage transmit waveform when transmit /receive (T/R) switch 306 is set to couple the transmitter to the transducer element as shown in the drawing. Following the transmission of the waveform into the subject, the T/R switch 306 is set to the alternate position so that the electrical signals transduced in response to received acoustic echoes are coupled to the input of a preamplifier 68 (also referred to as a preamplifying amplifier). A receive enable signal (Rx Enable) enables the preamplifier during the period of echo signal reception. The gain of the preamplifier 68 is increased during the period of echo reception, providing a TGC gain characteristic to signals received from increasing depths of the subject. The gain may be adjusted digitally by a controllable feedback impedance 310 which is implemented in integrated circuit form as a plurality of switchable parallel impedances. As more digitally controlled switches of the parallel impedances are closed, more impedances are coupled in parallel, reducing the feedback impedance 310 of the preamplifier. See, e.g., US patent application no. [2016PF0 0604],

(Freeman et al.) The amplified analog echo signals are coupled to an analog receive delay circuit 320 which delays the received echo signals in relation to the delays applied to other echo signals by the channels of other elements of the patch for analog beamforming. The applied delay is controlled by Delay Data received from the FPGA 104. The delayed echo signals are applied to a summing node with the other analog signals of the patch, shown as Channel Out in the drawing, where the echo signals are summed in the form of patch sum analog signals. In the preferred implementation for a 2D array, there are 128 summing nodes producing the partial sum signals from 128 patches of sixty-four elements each. These 128 partial sum signals are the input signals for the digital ASICs 103 which perform multiline digital beamforming .

FIGURE 4 illustrates an integrated circuit implementation of the analog receive delay circuit 320. The circuit 320 is a capacitive circuit which samples the signal produced by a transducer element 101η by closure of a switch 65, stores the sample on a capacitor 62 of the circuit, and then, at a later time which defines the intended delay, the sample is read from the capacitor by closure of a switch 62. The signal delayed in this manner is then coupled to the patch summing node by an output buffer 74, where it is summed with the analog signals from the other sixty-three elements of the patch. The time that a signal is stored on a capacitor $62_1, 62_2, \dots, 62_M$ is determined by the operation of a write controller 64 and a read controller 66. The write controller is a pointer circuit which determines the closure of one of switches $65_1, 65_2, \dots, 65_M$, the brief closing of which samples the signal of transducer 101η at the output

of preamplifier 68 and stores the sample on a capacitor. After a switch has "written" one sample to a capacitor, the write controller closes another switch 65 to store another sample of the signal on another capacitor 62. The write controller thus stores in rapid succession a plurality of samples of the signals received by transducer element 101 during the period of echo reception. The frequency with which samples are acquired exceeds the Nyquist rate for the received frequency band, and is usually well in excess of this rate. The read controller 66 is a pointer circuit which operates in a similar manner to read the stored signal samples after they have been stored on the capacitors for the desired delay period. The read controller closes one of switches 67, coupling a stored signal sample to an output buffer 74 from which it is available for further processing. In a rapid succession a sequence of the sampled signals are read from capacitors 62 and the now-delayed samples are forwarded for summation at the patch summing node.

The components of the analog ASIC 102 are seen to be digitally controlled analog components, and the transmitter 304 and T/R switch 306 must be capable of operating at the high voltages needed to drive a transducer element. In a preferred implementation the analog ASICs are manufactured by an integrated circuit process suitable for high voltages and with a relatively large feature size such as 0.18 μ M.

The circuitry of the four digital ASICs 103 is shown in FIGURE 5. In the illustrated implementation each digital ASIC contains 32 digital channels 601 to process the summed analog signals from 32 patches of transducer elements. Each digital channel digitizes an analog patch signal and forms eight digital

multiline output signals so that eight receive beams, each of a sequence of digital echo signals, are formed simultaneously. The eight multiline output signals are shown as MLO to ML7 for each channel in the drawing. The degree of multiline may be 4x, 8x as shown in FIGURE 5, 16x or any higher order multiline as determined by the circuit designer. In operation, an analog patch signal is converted to a sequence of digital echo samples by a low power ADC 603, preferably one which consumes 10 milliwatts or less, such as a successive approximation type ADC or a delta-sigma ADC. Each digital echo sample is delayed by eight selectable delay increments by a digital delay circuit 604, producing delayed echo signals for eight multilines. The eight multiline samples ML0-ML7 are coupled to eight digital adders or summers (summing circuits) 605, where the samples are summed with digital echo samples produced by other channels. The digital echo samples of the eight multilines from a preceding digital ASIC are received as a high rate serial data stream by a deserializer 602, which sorts samples of the data stream into eight parallel lines for the eight multilines. The thirty-two channels of the ASIC then add their partial sum multiline signals to the data of these eight parallel lines at a lower data rate than the high rate of the serial data stream. For instance, the serial data stream may run at 160 MHz, whereas other circuitry on the digital ASIC is clocked at 20 MHz. At the output of the ASIC (bottom right in the drawing), the data of the eight parallel lines is rearranged into a high rate serial data stream by a serializer 607, which is coupled to the next digital ASIC for summation with digital partial sum signals from other channels. Like the

deserializer 602, the serializer 607 runs at the higher data rate. At the output of the last digital ASIC in the chain, the fully beamformed serial data (RECEIVE BEAM DATA) is coupled to the FPGA 104 which
5 applies the received beam data to the USB controller 105 for communication to the image display device 108. Each digital ASIC also contains control registers 606 which receive control data from the FPGA to set parameters of the digital conversion and
10 beam formation process, such as sampling times and delay values for the digital delay circuits 604.

In the digital ASIC shown in FIGURE 5, the integrated circuit process used is preferably one with a smaller feature size than that of the analog
15 ASIC, which must operate at high voltages. A suitable feature size for the digital ASIC is 65nm or less, which allows higher circuit density than that of the analog ASIC while conserving power. Reduced power consumption is further facilitated by operating
20 most of the digital ASIC at a lower clock rate than that for which the integrated circuit process is capable. As previously mentioned, the serializer and deserializer operate at a high frequency such as 160 MHz, so the chosen integrated circuit process must be
25 capable of running at that clock frequency. But the digital ASIC core, in particular the digital delays and summers, is clocked at 20 MHz. This low frequency of operation, much lower than that for which the circuitry is designed, further reduces the
30 power required by the digital ASICs 103, since power consumption is proportional to clock frequency. Moreover, the lower clock rate of data reduces the need for resynchronization registers between circuits, further reducing power consumption.
35 Furthermore, by operating the digital ASIC at a lower

clock frequency, lower supply voltages can be used than would otherwise be necessary to maintain the desired precision at a higher clock frequency. Since power consumption is a function of voltage, operation at a lower voltage also saves power. In a preferred implementation the ADCs and the serializers and deserializers of the digital ASICs are operated at a higher voltage and the ASIC core at a lower voltage.

FIGURE 5a illustrates the architecture of a low power successive approximation ADC 603. The analog echo signal to be converted, V_{IN} in the drawing, is sampled and held by sample-and-hold circuit 624. A successive approximation register (SAR) 620 is initialized so that its most significant output bit D_n is set to a value of one. A digital-to-analog converter (DAC) 622 produces a comparison voltage referenced to voltage V_{REF} which is the analog equivalent of an $n+1$ bit digital word with its most significant bit (D_n) set to one. A comparator 626 compares the analog echo signal with the comparison voltage and if the comparison voltage is greater than the analog echo signal, the comparator output causes the SAR to set the most significant bit to zero; otherwise, it is left at a value of one. The next most significant bit of the SAR, D_{n-1} , is set to one, and another comparison is performed to determine the correct setting of the D_{n-1} bit. The process is completed until all of the output bits of the SAR have been correctly set, which is then the digital value of the analog echo signal. An end-of-conversion signal EOC signals this completion of the conversion to the digital delay circuit 604, which then accepts the digital value of the SAR as its next digital signal sample. The sample-and-hold circuit 624 then acquires a new echo signal sample, the SAR

620 is initialized, and the process continues.

The digital delay circuitry, delay control, and summation circuitry of one channel of the digital ASIC of FIGURE 5 is shown in further detail in FIGURE 6. As the low power ADC 603 produces successive digital echo signal samples from a patch, the samples are stored in a multi-port RAM 640 by the indexing of a write address counter (WAC) 642. Delayed echo signals are read out of eight output ports Q_0-Q_7 of the RAM 640 by eight read address counters (RAC) 644₀ to 644₇ for eight multilines, the circuitry of one of which is shown in the drawing. Additional read address counters can be added when more than eight multilines are to be produced. Each RAC 644 applies its read address to one of the eight address ports Ad-r0 to Ad-r7 of the RAM. The address of the read out sample and its timing determine the delay of the digital echo signal. The addresses applied to the RAM for a multiline are set by a focus control circuit 646₀ in response to focus data provided by the FPGA 104, and the output addresses are clocked into the RAC 644₀ and periodically adjusted for dynamic focusing. The delayed digital echo signals produced at the Q outputs of the RAM 640 can be further resolved to a finer delay by a sub sample delay FIR 648₀, which also receives data as required from the focus control circuit. The final delayed digital echo signal for a multiline, shown as CH0 in the drawing, is summed with other samples for that multiline from other digital channels by a summer 605₀. The summed samples up to that point are resynchronized by clocking into a D type flip-flop 650₀ and applied to the summer of the next channel. Each channel thus produces properly delayed digital patch signal samples for eight multilines (Q_0-Q_7)

simultaneously .

A preferred sub sample delay finite impulse response (FIR) filter is shown in FIGURE 7. This preferred FIR filter, unlike conventional FIR
5 filters, uses no multipliers, thereby conserving power. Successive echo signal samples from the RAM 640 are clocked into a register 702, which thus has a current sample Q_n at its input and the previous sample Q_{n+1} at its output. Weighted fractions of the two
10 samples are formed to produce more finely resolved delayed sample values. Instead of using multipliers to do the weighting, the weighting fractions used are to a power of two, formed by forced zero-filling of one or more of the most significant bits of a sample value. Thus, a summer 704 is coupled to receive the
15 Q_n sample weighted twice, once with its most significant bit zeroed ($0, Q_n$) and again with its two most significant bits zeroed ($0, 0, Q_n$). Similarly, the summer 704 is also coupled to receive the Q_{n+1} sample
20 in two weighted forms, once with the two most significant bits zeroed and again with the three most significant bits zeroed. The summer 704 thus produces a weighted echo signal of the form $.75Q_n + .125Q_{n+1}$. In like manner a summer 706 is
25 coupled to produce a weighted echo signal of the form $.125Q_n + .75Q_{n+1}$. The Q_n sample and these two weighted sample values are applied to the three inputs of a multiplexer 708 and one of the applied values is selected as the multiplexer output value by
30 an SSD selection signal provided by the focus control circuit 646. The selected finely delayed value is clocked into a register 710 for resynchronization and applied to a summer 605 for that multiline. FIGURE 8 shows three phase shifts of a typical ultrasound echo
35 signal which can be produced by the sub sample delay

FIR filter of FIGURE 7. As seen, delay values of 0, 1/3 and 2/3 of a base sampling clock frequency can be achieved with this circuitry.

5 An important feature of the digital ASIC of FIGURE 5 for reduced power consumption is that the ADCs 603 and the following digital beamforming (digital delays 604 and summers 605) are located in the same integrated circuit package. This eliminates the need to transfer data from an ADC in one package to the digital beamformer in another package, which would require increased power in order to drive signals from one package to another through the intervening IC pins, PCB traces, and connection pads. Power is saved by this use of in-package interconnection. While the digital ASIC package can employ stacked dies or a multi-chip module, it is preferred that the ADC be on the same silicon die as the digital beamformer circuitry.

10

15

It should be noted that the various embodiments described above and illustrated by the exemplary ultrasound systems of FIGURES 1 and 2 may be implemented in hardware, software or a combination thereof. The various embodiments and/or components of an ultrasound system, for example, the modules, or components and controllers therein, also may be implemented as part of one or more computers or microprocessors. The computer or processor may include a computing device, an input device, a display unit and an interface, for example, for accessing the Internet. The computer or processor may include a microprocessor. The microprocessor may be connected to a communication bus, for example, to access a PACS system. The computer or processor may also include a memory. The memory devices described above may include Random Access Memory (RAM) and Read

20

25

30

35

Only Memory (ROM) . The computer or processor further
may include a storage device, which may be a hard
disk drive or a removable storage drive such as a
floppy disk drive, optical disk drive, solid-state
5 thumb drive, and the like. The storage device may
also be other similar means for loading computer
programs or other instructions into the computer or
processor .

As used herein, the term "computer" or "module"
10 or "processor" may include any processor-based or
microprocessor-based system including systems using
microcontrollers, reduced instruction set computers
(RISC) , ASICs, logic circuits, and any other circuit
or processor capable of executing the functions
15 described herein. The above examples are exemplary
only, and are thus not intended to limit in any way
the definition and/or meaning of these terms.

The computer or processor executes a set of
instructions that are stored in one or more storage
20 elements, in order to process input data. The
storage elements may also store data or other
information as desired or needed. The storage
element may be in the form of an information source
or a physical memory element within a processing
25 machine.

The set of instructions of an ultrasound system
including a microbeamformer may include various
commands that instruct the computer or processor as a
processing machine to perform specific operations
30 such as the methods and processes of the various
embodiments of the invention. The set of
instructions may be in the form of a software
program. The software may be in various forms such
as system software or application software and which
35 may be embodied as a tangible and non-transitory

computer readable medium. Further, the software may be in the form of a collection of separate programs or modules, a program module within a larger program or a portion of a program module. The software also
5 may include modular programming in the form of object-oriented programming. The processing of input data by the processing machine may be in response to operator commands, or in response to results of previous processing, or in response to a request made
10 by another processing machine. In the ultrasound system of FIGURE 2, for instance, software instructions are received by the FPGA 104 of the microbeamformer from the mainframe ultrasound system. The FPGA then applies the software instructions to
15 the analog and digital ASICs 102 and 103 to control the operation of the microbeamformer structural components by software instructions.

Furthermore, the limitations of the following claims are not written in means-plus-function format
20 and are not intended to be interpreted based on 35 U.S.C. 112, sixth paragraph, unless and until such claim limitations expressly use the phrase "means for" followed by a statement of function devoid of further structure.

25

WHAT IS CLAIMED IS:

1. An ultrasound probe for digital
microbeamforming, comprising:

- 5 an array transducer adapted to scan a target
region and coupled to a digital microbeamformer;
wherein the digital microbeamformer comprises:
a plurality of amplifiers configured to
receive analog echo signals from transducer elements
10 of the array;
low power ADCs configured to receive
amplified analog echo signals from the amplifiers and
to convert them to digital echo data;
digital beamforming circuitry coupled to
15 the low power ADCs and configured to produce digital
beamformed echo signals,
and a digital application specific
integrated circuit (ASIC) configured to operate a
core clock frequency.

20

2. The ultrasound probe of Claim 1, wherein
the low power ADCs and the digital beamforming
circuitry are located on the digital ASIC.

25

3. The ultrasound probe of Claim 2, wherein
the low power ADCs and the digital beamforming
circuitry are located on a stacked die in the digital
ASIC.

30

4. The ultrasound probe of Claim 2, wherein
the digital ASIC comprises a multi-chip module
containing the low power ADCs and the digital
beamforming circuitry.

35

5. The ultrasound probe of Claim 2, wherein

the low power ADCs and the digital beamforming circuitry are located on the same silicon die in the digital ASIC.

5 6. The ultrasound probe of Claim 5, wherein the digital ASIC comprises digital circuitry configured to be clocked at a frequency greater than the core clock frequency.

10 7. The ultrasound probe of Claim 6, wherein the digital ASIC comprises digital circuitry configured to be clocked at a frequency that is at least twice the core clock frequency.

15 8. The ultrasound probe of Claim 7, wherein the digital ASIC comprises digital circuitry configured to be clocked at a frequency that is at least eight times the core clock frequency.

20 9. The ultrasound probe of Claim 1, wherein the digital ASIC is configured to operate at a supply voltage of one volt or less.

25 10. The ultrasound probe of Claim 1, wherein the low power ADCs comprise delta-sigma analog to digital converters.

30 11. The ultrasound probe of Claim 1, wherein the low power ADCs comprise successive approximation analog to digital converters.

35 12. The ultrasound probe of Claim 7, wherein the low power ADCs are located on the digital ASIC and the digital beamforming circuitry is located on a separate interconnected ASIC; and

wherein the probe is configured to transfer digitally beamformed data between two ASICs at a frequency that is at least twice the frequency of the core clock frequency of the ASICs.

5

13. The ultrasound probe of Claim 12, wherein the digital beamforming circuitry is configured as thirty-two digital beamforming channels.

10

14. The ultrasound probe of Claim 13, comprising four digital ASICs.

15

15. The ultrasound probe of Claim 1, further comprising a plurality of high voltage transmitters located on an analog ASIC and coupled to elements of the array transducer,

wherein the amplifiers are located on the analog ASIC.

20

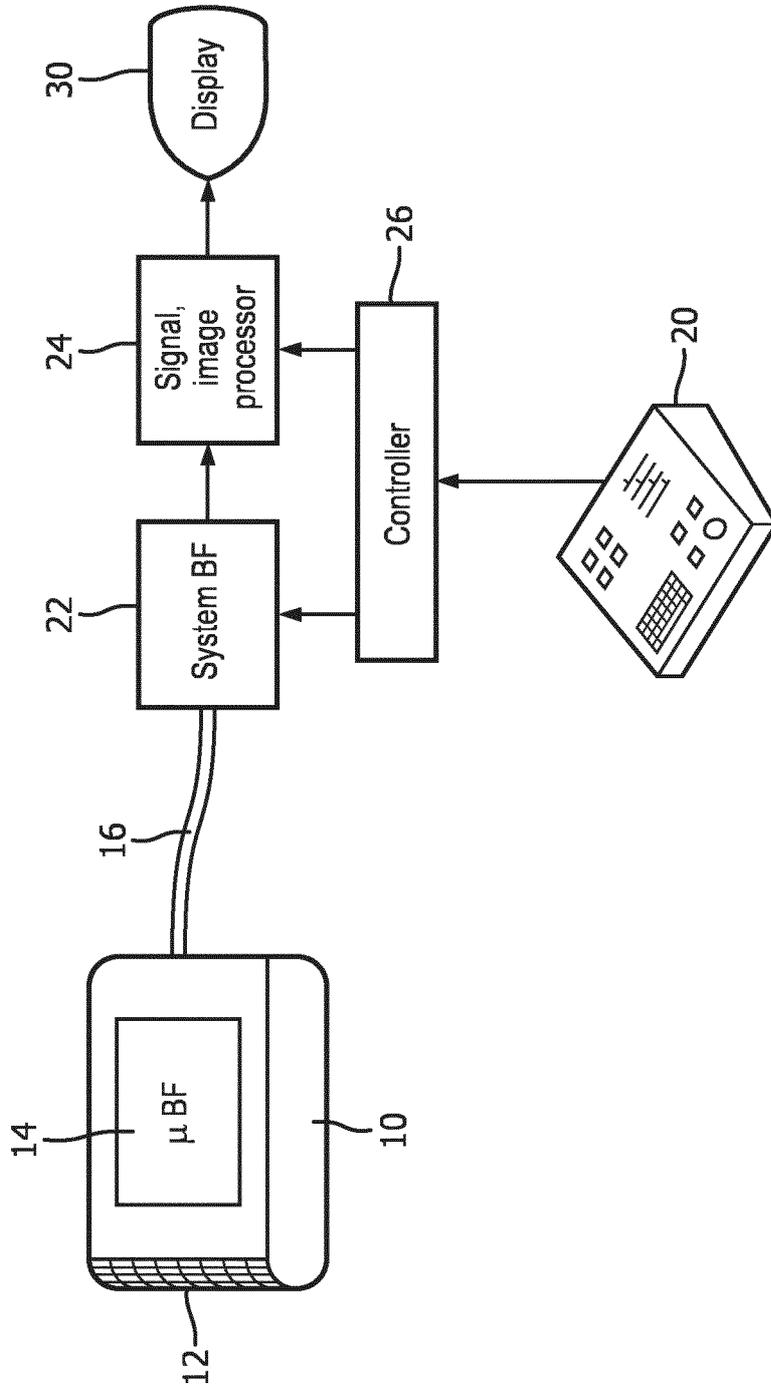


FIG. 1

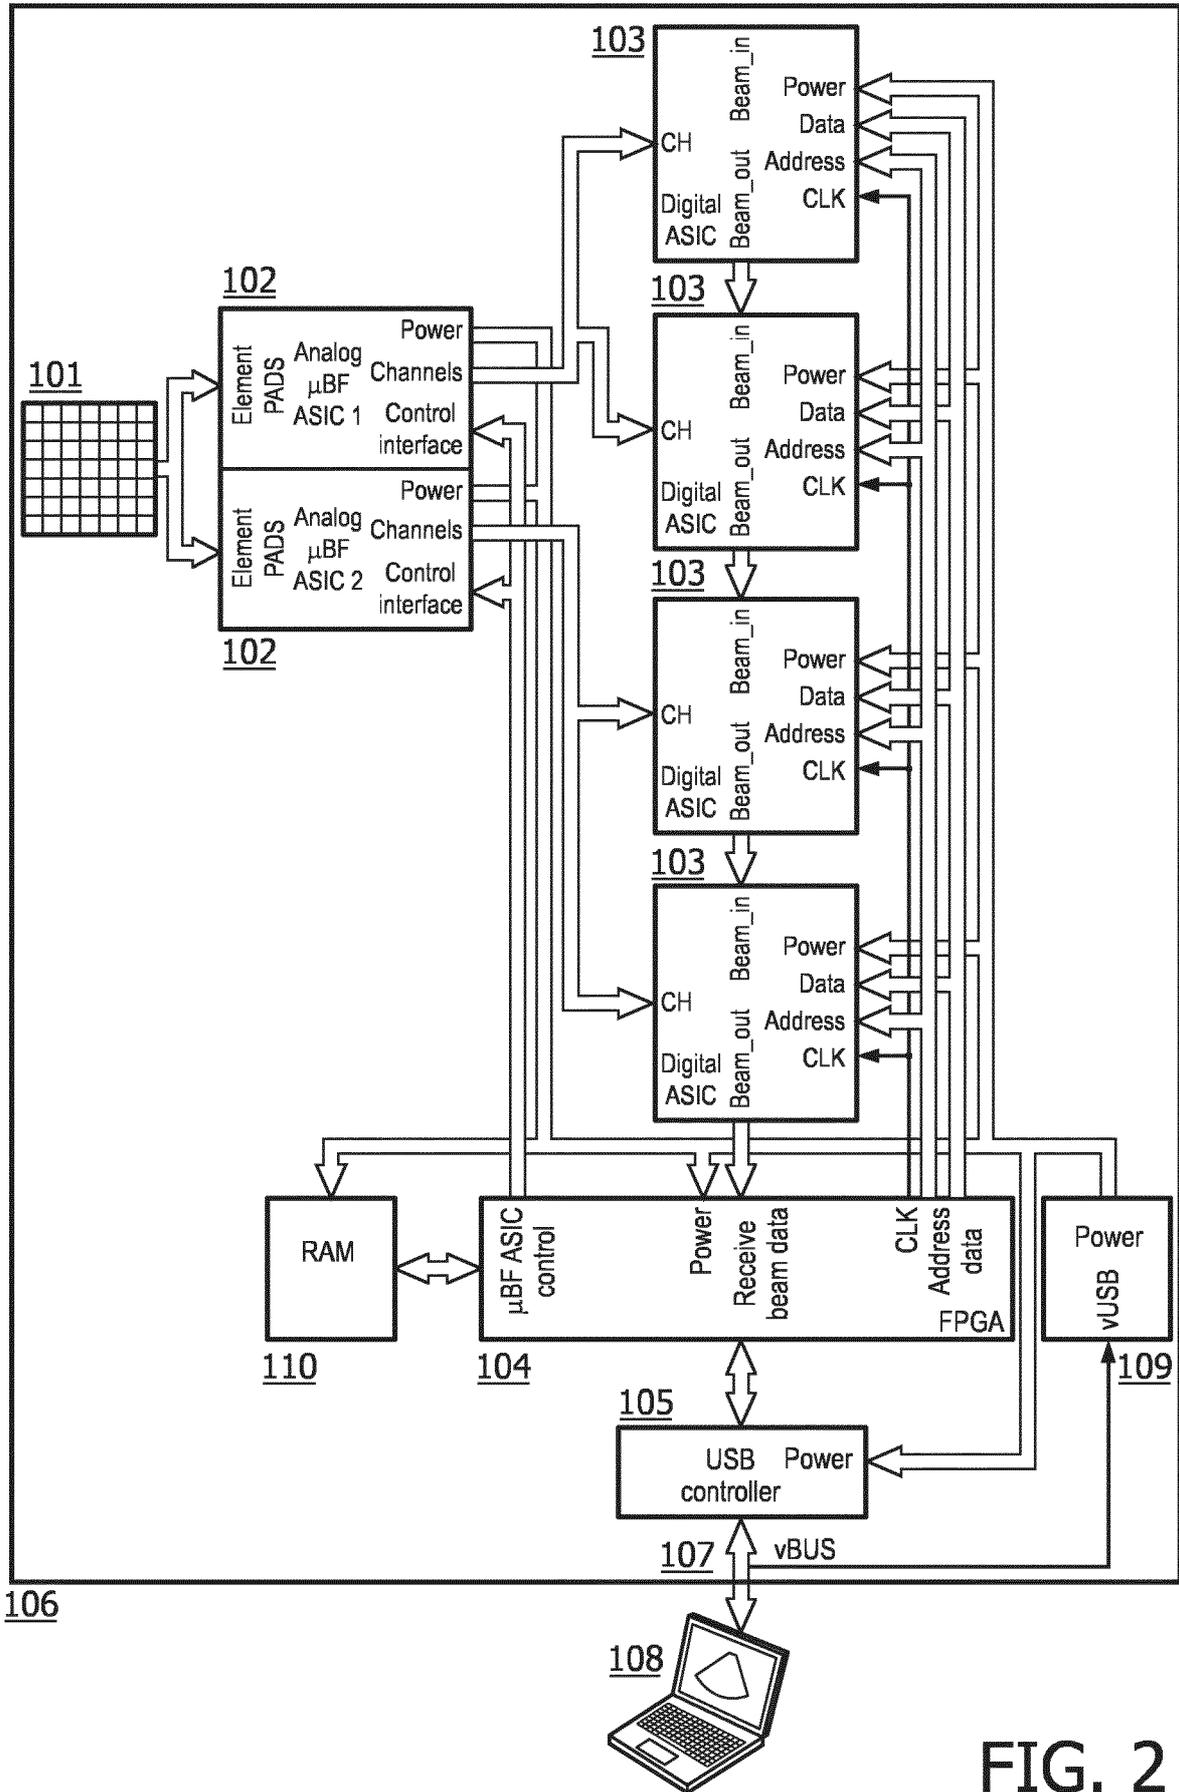


FIG. 2

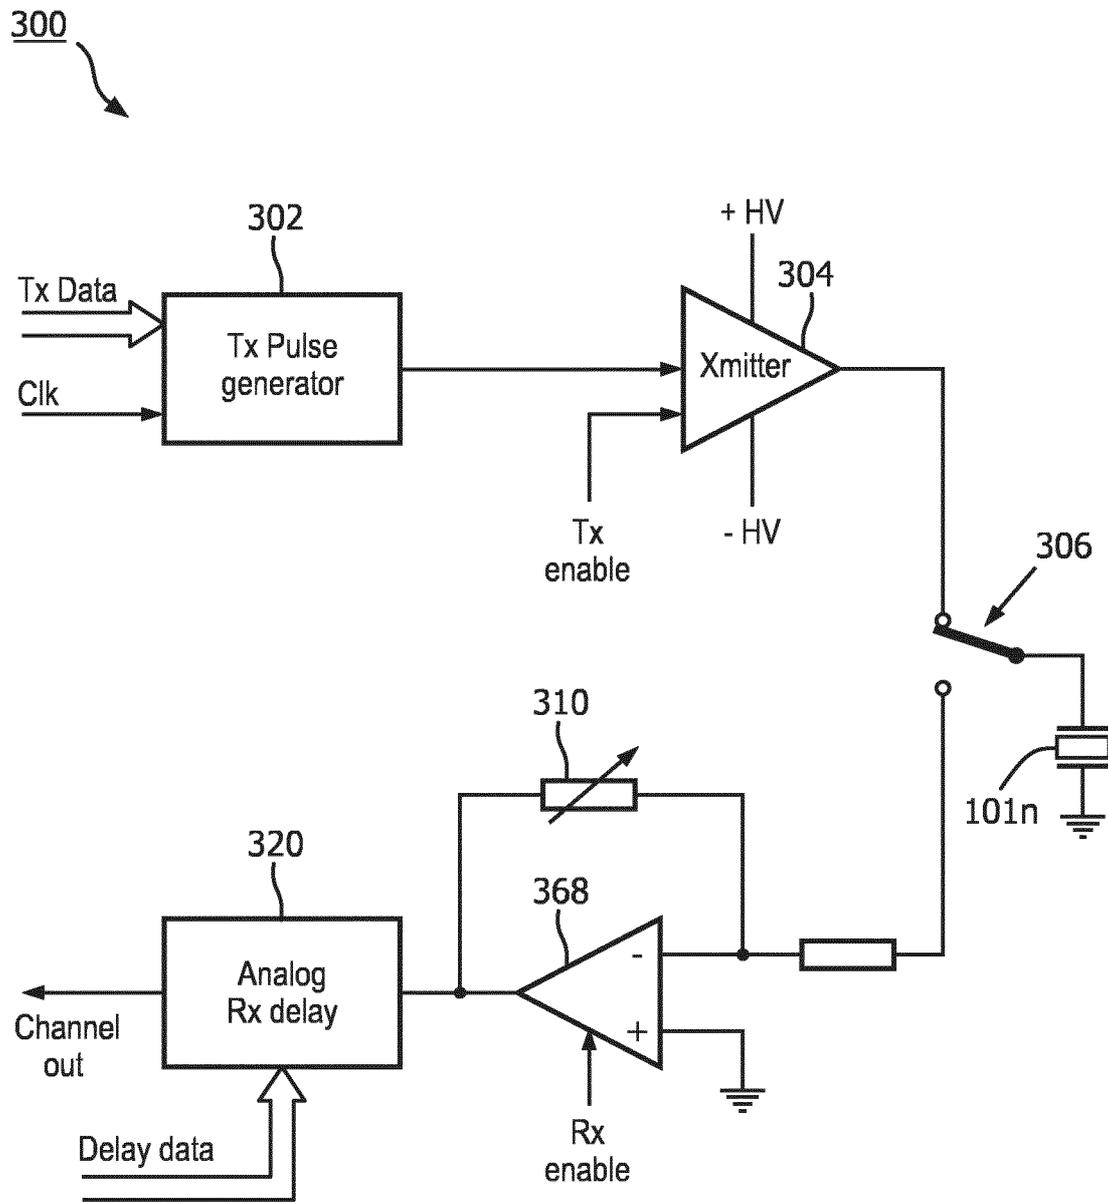


FIG. 3

4/9

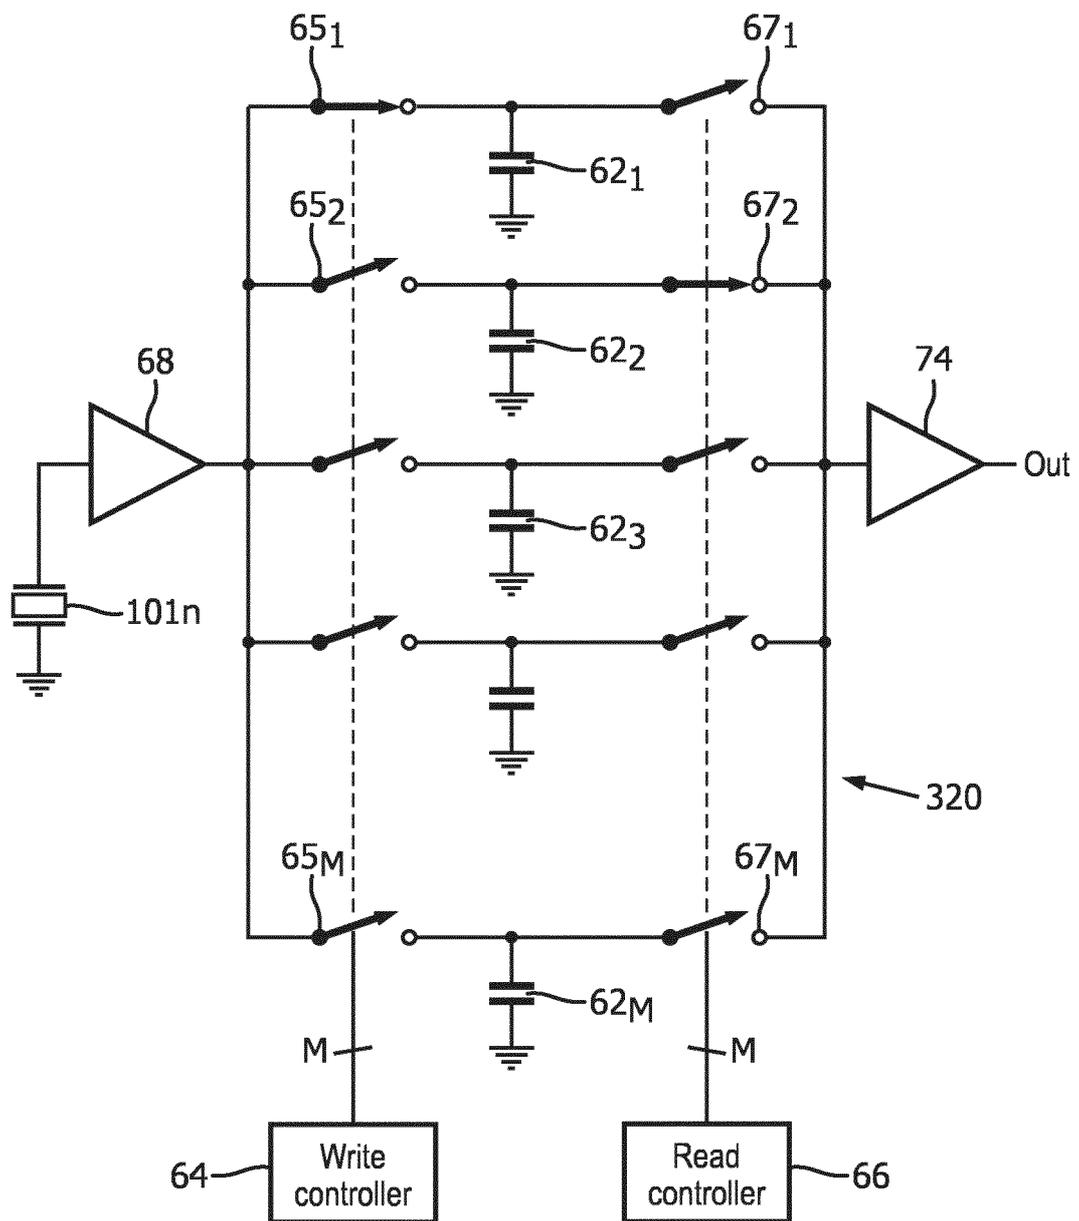


FIG. 4

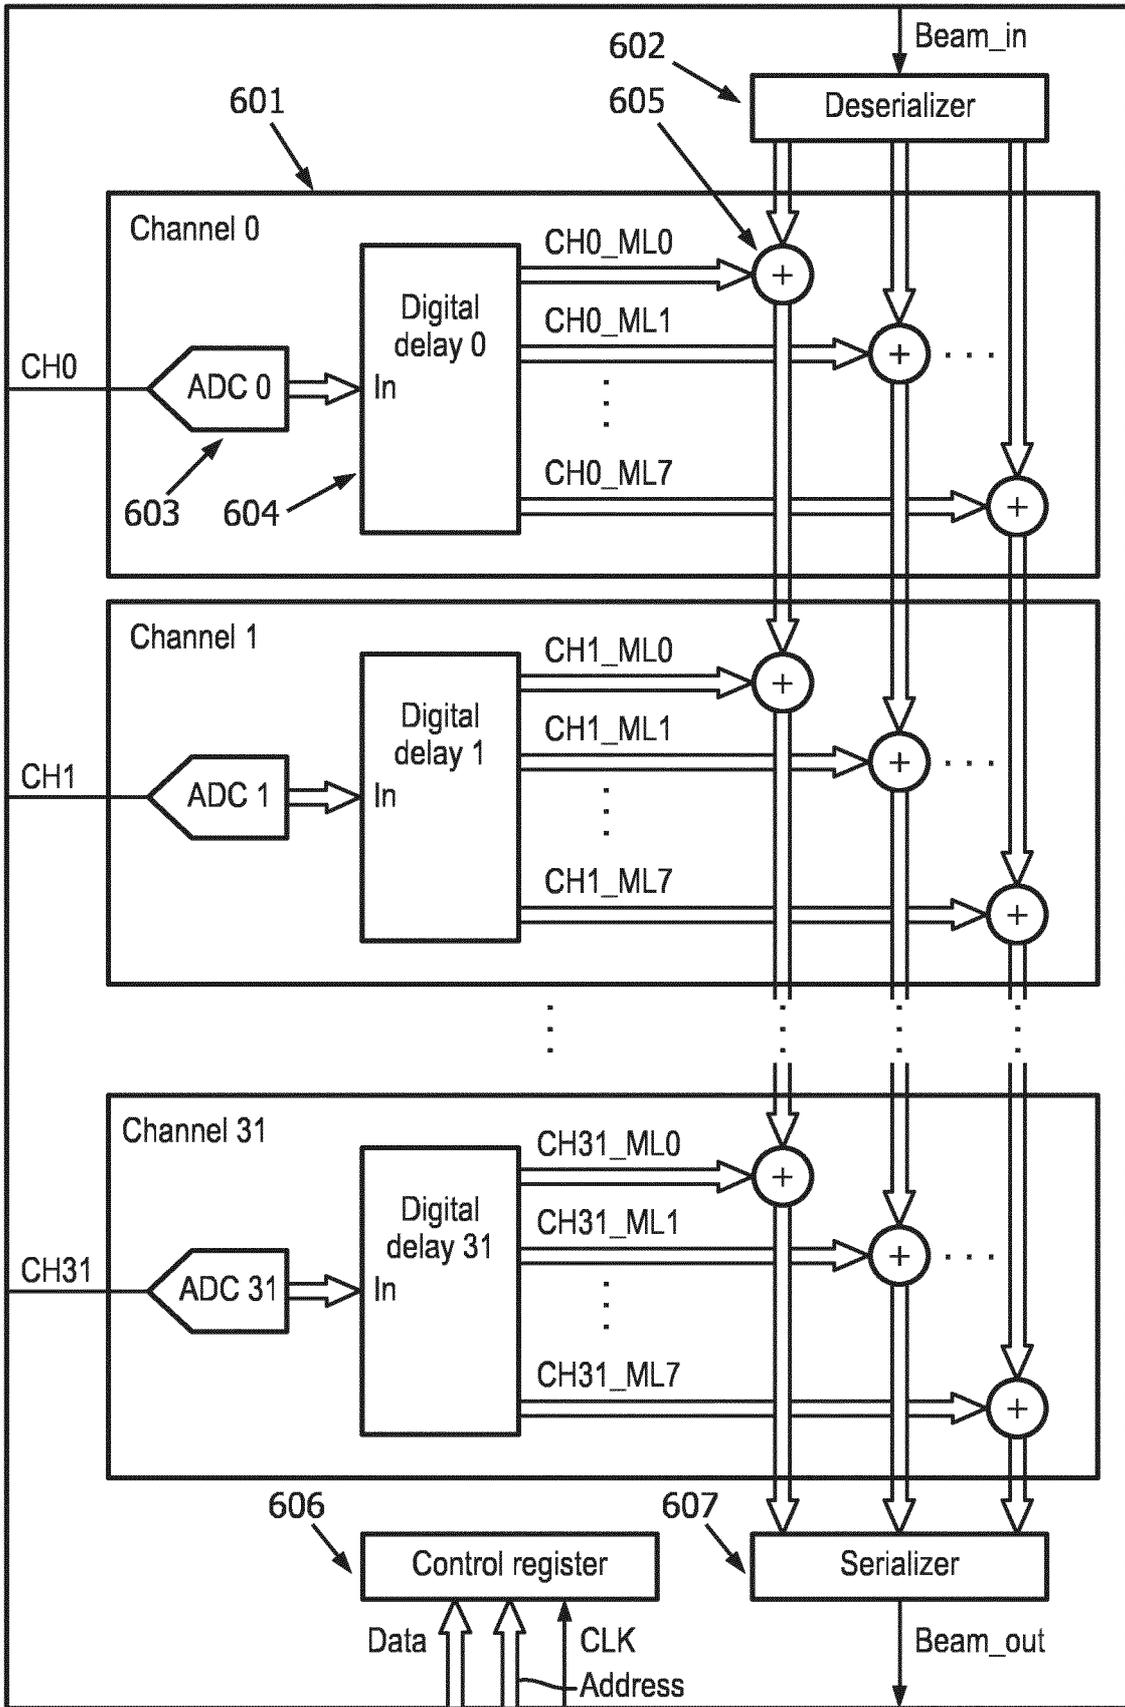


FIG. 5

6/9

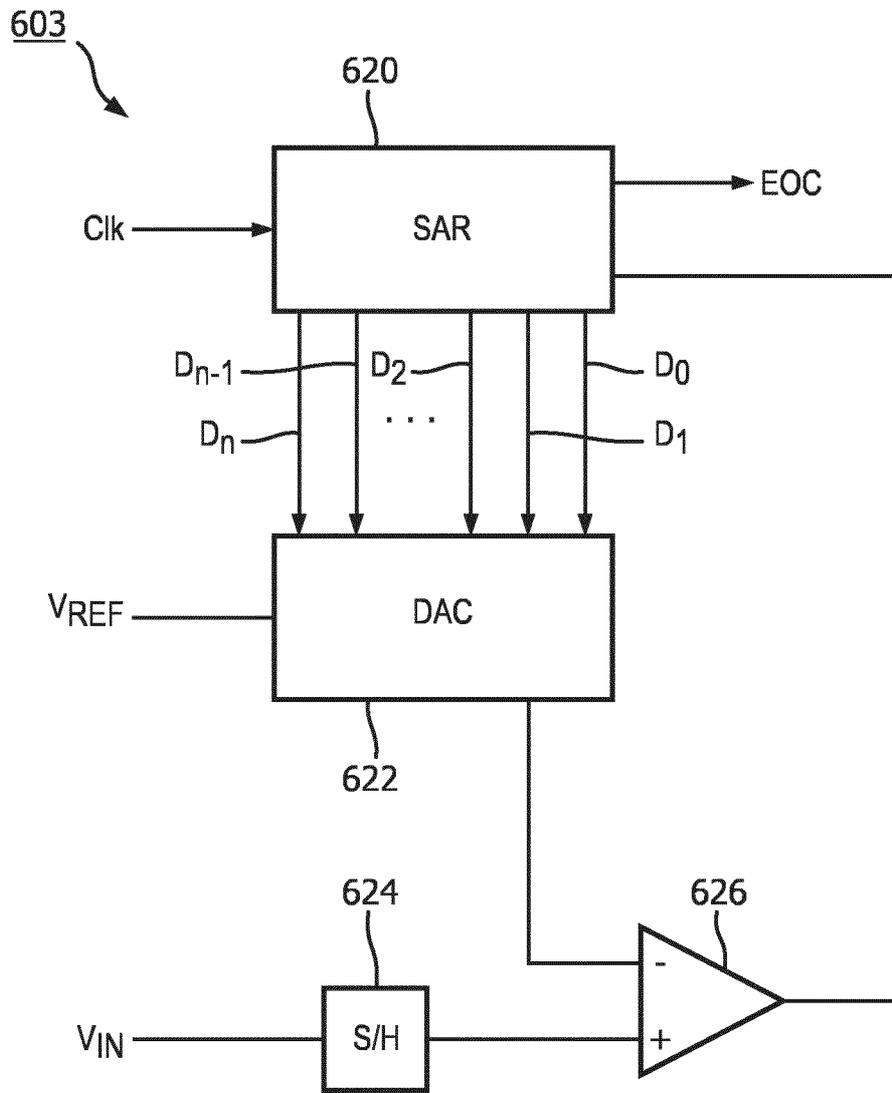


FIG. 5a

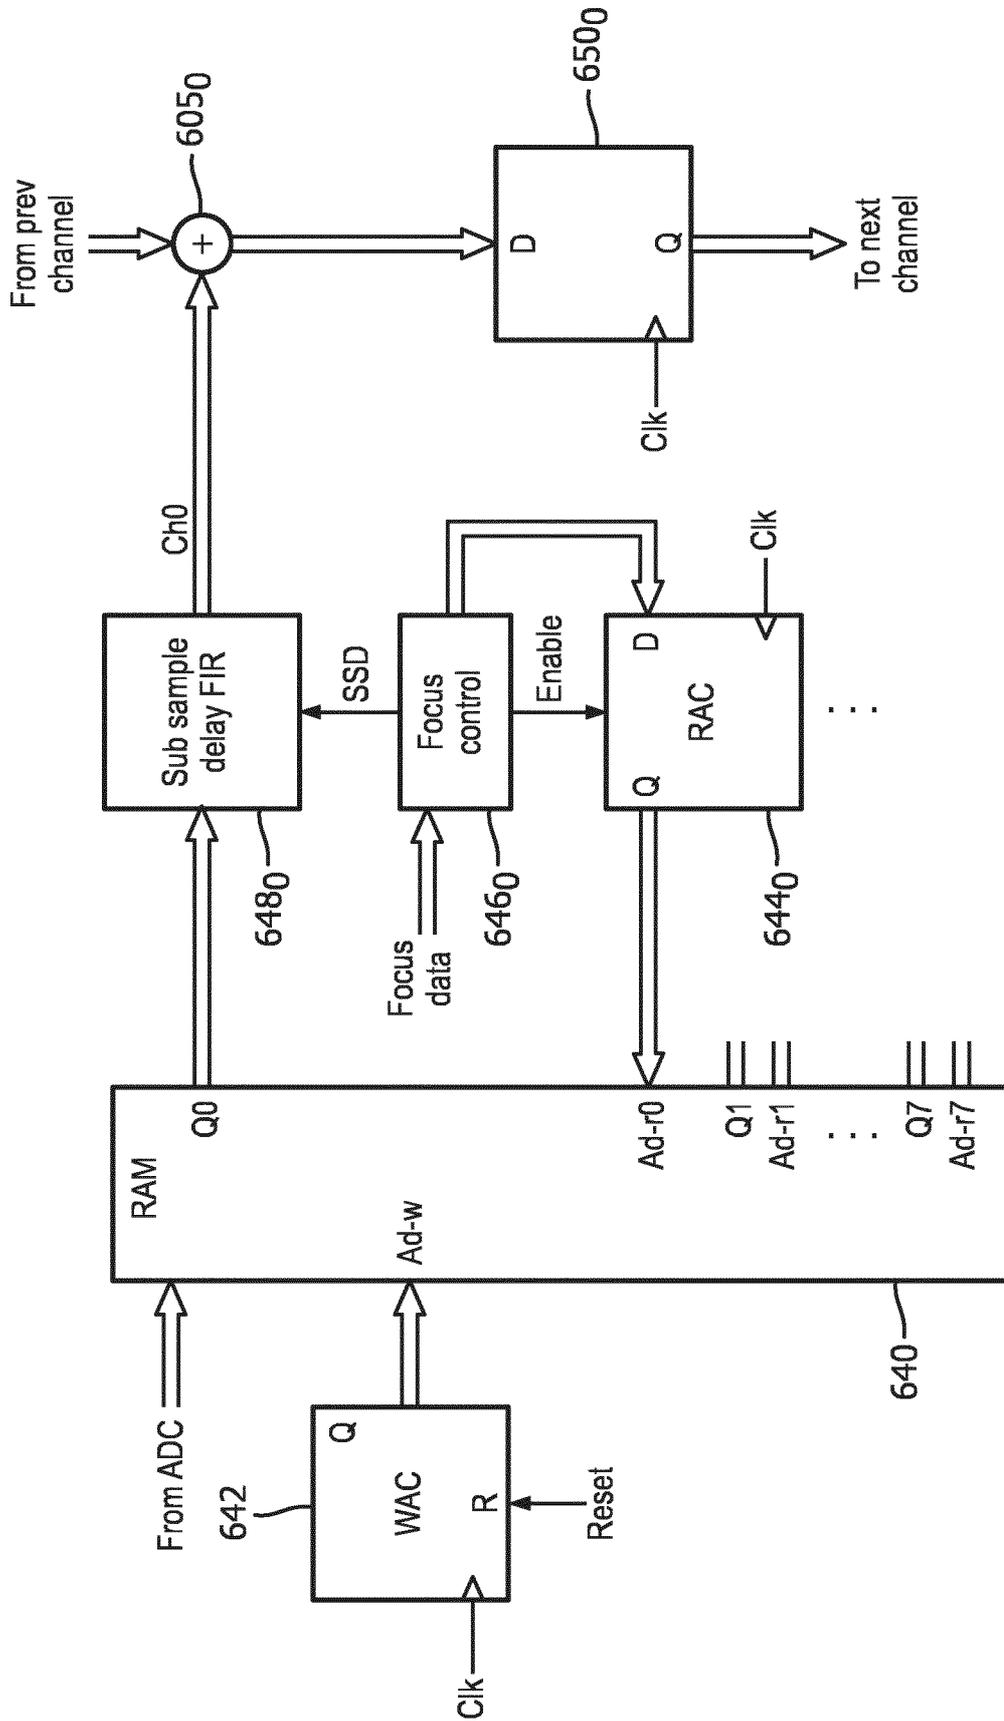


FIG. 6

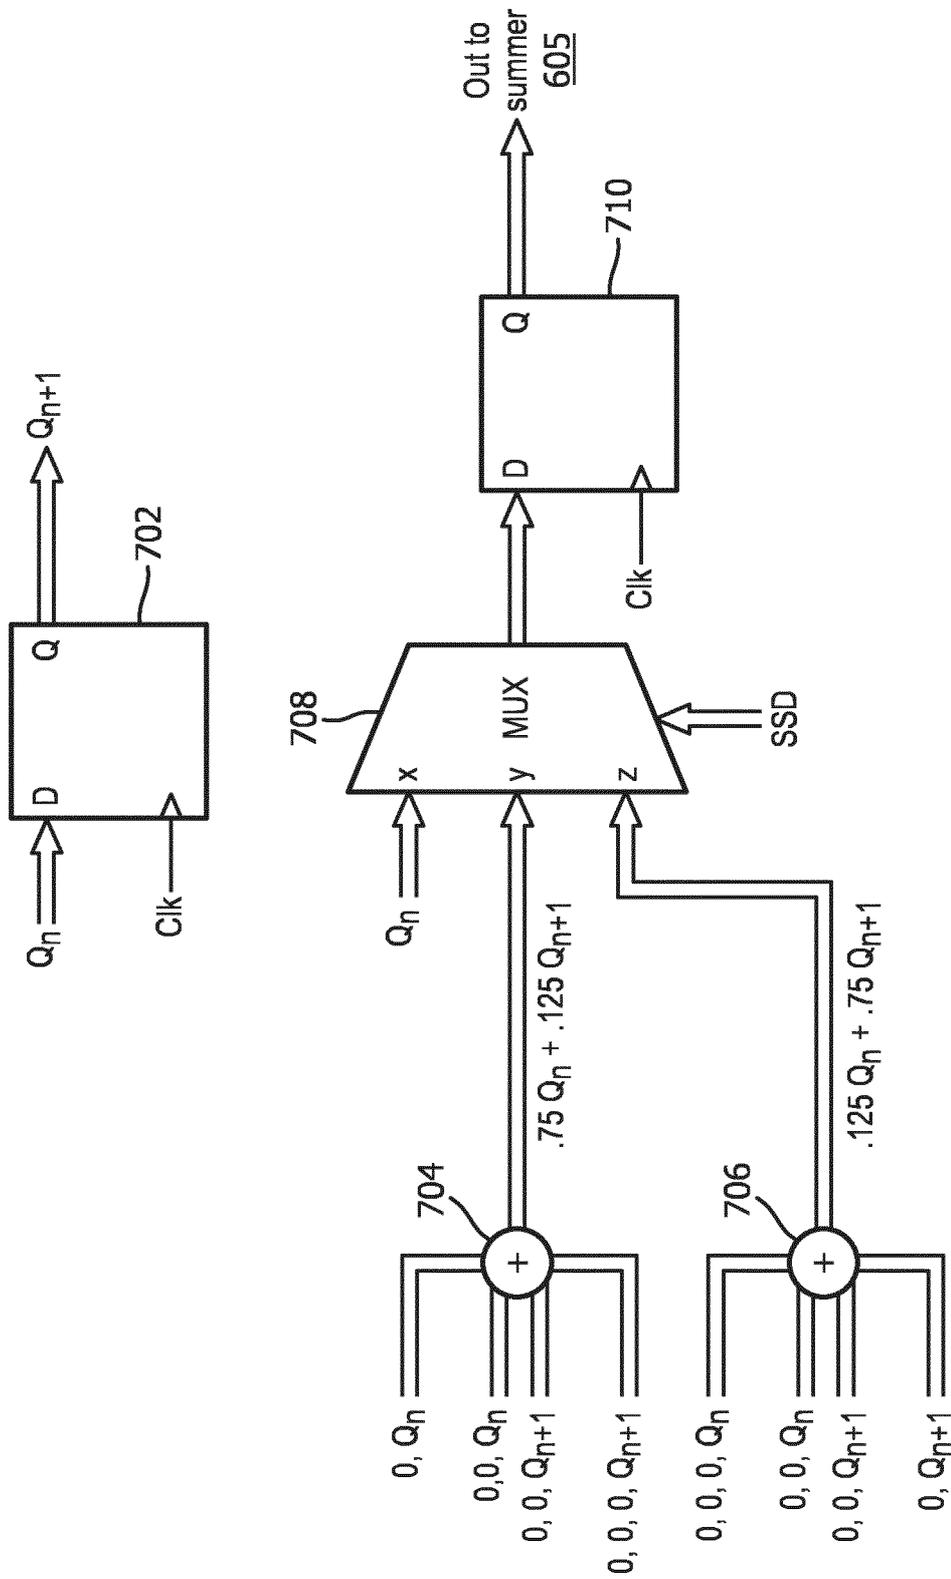


FIG. 7

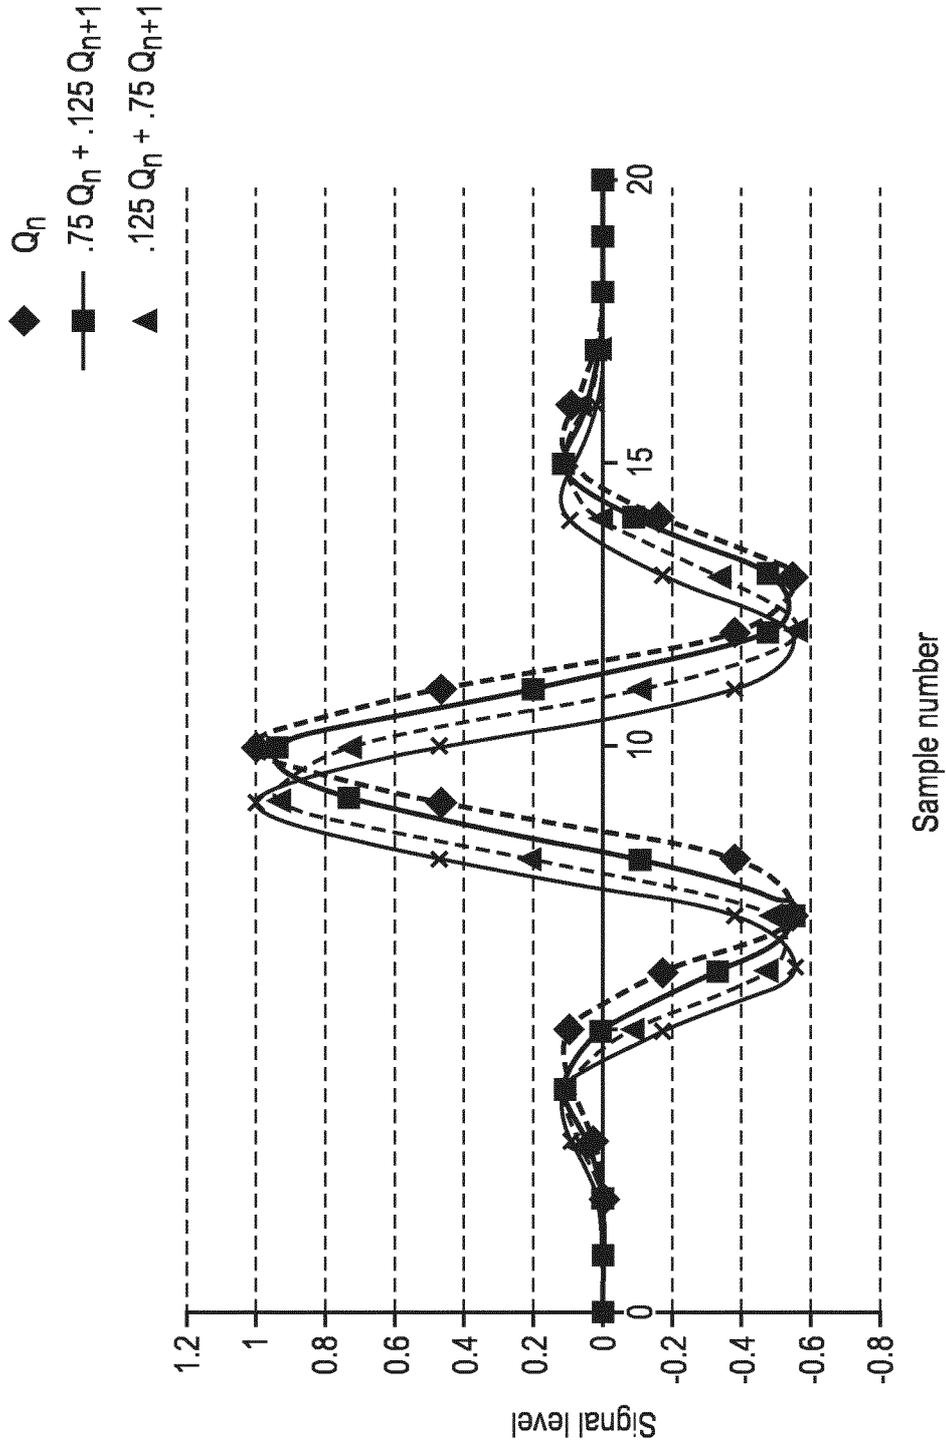


FIG. 8

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2017/071940

A. CLASSIFICATION OF SUBJECT MATTER
 INV. G01S7/52 G01S15/89 G10K11/34
 ADD.
 According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
 Minimum documentation searched (classification system followed by classification symbols)
 G01S G10K

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
 EPO-Internal , INSPEC, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2007/016023 AI (PHELPS ROBERT N [US] ET AL) 18 January 2007 (2007-01-18) abstract; figure 1 paragraphs [0019] , [0020] , [0022] paragraphs [0023] , [0025] , [0026] paragraphs [0030] , [0043] -----	1-15
X	Wo 2016/077822 AI (URSUS MEDICAL LLC [US]) 19 May 2016 (2016-05-19) figure 14 paragraphs [0074] , [0077] ----- -/- .	1-15

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search 8 November 2017	Date of mailing of the international search report 16/11/2017
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Knol I , Bernhard

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2017/071940

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>US 2009/069686 A1 (DAFT CHRISTOPHER M W [US] ET AL) 12 March 2009 (2009-03-12) abstract; figures 2, 3 paragraphs [0035], [0045] - [0048] paragraph [0050] - paragraph [0053] paragraph [0059] - paragraph [0063] paragraph [0066]</p> <p style="text-align: center;">-----</p>	1-15
A	<p>US 2005/068221 A1 (FREEMAN STEVEN R [US] ET AL) 31 March 2005 (2005-03-31) abstract paragraph [0010]</p> <p style="text-align: center;">-----</p>	6-8, 10, 11

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/EP2017/071940
--

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 2007016023	A1	18-01-2007	US 2007016023 A1	18-01-2007
			US 2009007414 A1	08-01-2009

WO 2016077822	A1	19-05-2016	CA 2967646 A1	19-05-2016
			CN 107110826 A	29-08-2017
			EP 3218705 A1	20-09-2017
			WO 2016077822 A1	19-05-2016

US 2009069686	A1	12-03-2009	NONE	

US 2005068221	A1	31-03-2005	JP 2005103290 A	21-04-2005
			US 2005068221 A1	31-03-2005
