



US00D787685S

(12) **United States Design Patent**
Vezina

(10) **Patent No.:** **US D787,685 S**

(45) **Date of Patent:** **** May 23, 2017**

(54) **PROBE FOR A PERIPHERAL ULTRASOUND DEVICE**

4,674,517 A * 6/1987 Barnes G10K 11/004
600/459

(71) Applicant: **Guardspan Scientific, Inc.**, Park City,
UT (US)

4,827,943 A 5/1989 Bornn et al.
4,857,836 A 8/1989 Söelkner
4,908,568 A 3/1990 Söelkner
4,947,853 A 8/1990 Hon
5,022,410 A 6/1991 Hall et al.
5,070,880 A 12/1991 Gomez et al.

(72) Inventor: **Daniel P. Vezina**, Park City, UT (US)

(Continued)

(73) Assignee: **Guardspan Scientific, Inc.**, Park City,
UT (US)

FOREIGN PATENT DOCUMENTS

(**) Term: **14 Years**

EP 0607490 7/1994
JP 05337108 12/1993

(21) Appl. No.: **29/457,201**

(22) Filed: **Jun. 7, 2013**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 158, 186-187, 200, 107, 144;
600/437, 439, 446, 453, 459, 463, 424,
600/443; 128/916; D10/60, 80, 103, 78;
73/634

CPC A61B 5/14532; A61B 5/14546; A61B
5/1455; A61B 5/14551; A61B 5/14552;
A61B 7/003; A61B 5/0476; A61B 5/021;
A61B 5/0478; A61B 8/4281; A61B 8/00;
A61B 5/0002; A61B 5/042; A61B 8/12;
C12Q 1/006

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,165,270 A 8/1979 Ost et al.
4,305,207 A 12/1981 Lantz
4,343,092 A 8/1982 Wahl et al.
4,517,840 A * 5/1985 Thompson G10K 11/004
73/634
4,582,066 A * 4/1986 Barnes A61B 8/065
600/459

Anderson G. Chronic Conditions: Making the Case for Ongoing
Care. Johns Hopkins University, Baltimore, MD. Nov. 2007, 77
pages.

(Continued)

Primary Examiner — Ian Simmons
Assistant Examiner — Mark Cavanna
(74) *Attorney, Agent, or Firm* — Polsinelli PC


(57) **CLAIM**

The ornamental design for a probe for a peripheral ultra-
sound device, as shown and described.

DESCRIPTION

FIG. 1 is a bottom perspective view of a probe for a
peripheral ultrasound device showing my new design.
FIG. 2 is a bottom view thereof.
FIG. 3 is a top view thereof.
FIG. 4 is a left view thereof.
FIG. 5 is a right view thereof.
FIG. 6 is a back view thereof; and,
FIG. 7 is a front view thereof.
In the drawings, the broken line showing of cables illustrates
environment and forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

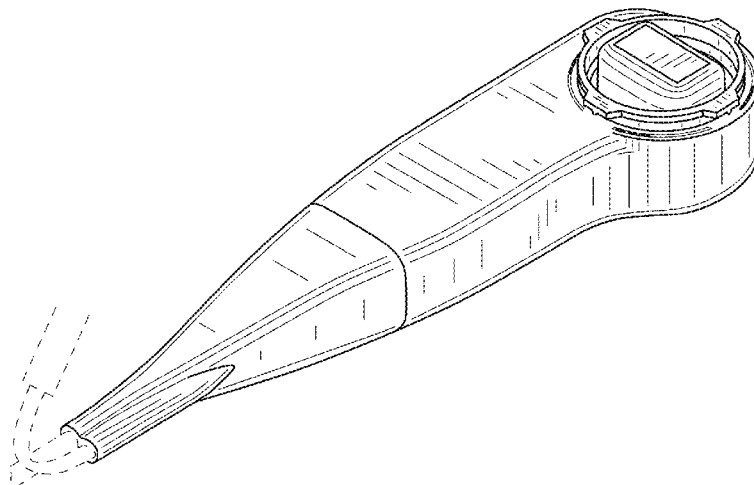

(56)

References Cited

U.S. PATENT DOCUMENTS

D343,801	S *	2/1994	Burns	D10/78
5,394,877	A	3/1995	Orr et al.		
5,469,852	A	11/1995	Nakamura et al.		
D369,307	S *	4/1996	Imling	D10/78
5,558,623	A *	9/1996	Cody	B06B 1/0269 600/439
5,598,845	A	2/1997	Chandraratna et al.		
5,634,468	A	6/1997	Platt et al.		
5,671,747	A *	9/1997	Connor	A61B 8/12 600/459
5,704,352	A	1/1998	Tremblay et al.		
5,740,804	A	4/1998	Cerofolini		
5,771,896	A	6/1998	Sliwa, Jr. et al.		
5,807,268	A	9/1998	Reeves et al.		
5,947,961	A	9/1999	Netherly		
6,031,383	A	2/2000	Streib et al.		
D425,980	S *	5/2000	Last	D24/107
6,124,723	A	9/2000	Costello		
6,126,636	A	10/2000	Naka		
6,132,371	A	10/2000	Dempsey et al.		
6,139,502	A *	10/2000	Fredriksen	A61B 8/4281 600/459
6,248,101	B1	6/2001	Whitmore, III et al.		
6,261,231	B1	7/2001	Damphousse et al.		
6,285,180	B1	9/2001	Pas		
6,577,893	B1	6/2003	Besson et al.		
6,653,825	B2	11/2003	Munniksma		
D536,450	S *	2/2007	Ryan	D24/144
7,215,991	B2	5/2007	Besson et al.		
7,244,230	B2	7/2007	Duggirala et al.		
D550,365	S *	9/2007	Kitayama	D24/186
D623,755	S *	9/2010	Ikegame	D24/186
D638,946	S *	5/2011	Egorov	D24/187
8,348,847	B2	1/2013	Vežina		
D687,153	S *	7/2013	Torzilli	D24/187
2002/0120310	A1	8/2002	Linden et al.		
2003/0187362	A1	10/2003	Murphy et al.		
2003/0220578	A1	11/2003	Ho et al.		
2004/0006278	A1	1/2004	Webb et al.		
2004/0015081	A1	1/2004	Kramer et al.		
2005/0157888	A1	7/2005	Yang		
2005/0232434	A1	10/2005	Andersen		
2005/0288584	A1	12/2005	McMorrow et al.		
2006/0030782	A1	2/2006	Shennib		
2006/0241464	A1	10/2006	Ohtake et al.		
2006/0264767	A1	11/2006	Shennib		
2007/0106751	A1	5/2007	Moore		
2007/0260285	A1	11/2007	Libbus et al.		
2007/0261493	A1	11/2007	Kim		
2007/0276251	A1	11/2007	Orenstein et al.		
2007/0276270	A1	11/2007	Tran		
2008/0004904	A1	1/2008	Tran		
2008/0013747	A1	1/2008	Tran		
2010/0168577	A1	7/2010	Vežina		
2011/0270089	A1	11/2011	Vežina		
2013/0102899	A1	4/2013	Vežina		
2013/0102900	A1	4/2013	Vežina		

OTHER PUBLICATIONS

Devereux et al. A population-based assessment of left ventricular systolic dysfunction in middle-aged and older adults; the Strong Heart Study. *Am Heart J.* Mar. 2001 141(3): 439-46.

Devereux et al. Congestive heart failure despite normal ventricular systolic function in a population-based sample: the Strong Heart Study. *Am. J. Cardiol.* Nov. 15, 2000; 86 (10): 1090-6.

Eagle et al. ACC/AHA Guideline Update for Perioperative Cardiovascular Evaluation for Noncardiac Surgery-Executive Summary. A report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines (Committee to Update the 1996 Guidelines on Perioperative Cardiovascular Evaluation for Noncardiac Summary) *Anesth. Analg.* May 4/5, 2002) 1052-64.

Garrett et al. The boomers are coming; a total cost of care model of the impact of population aging on the cost of chronic conditions in the United States. *Dis Manag.* Apr. 2007; 10(2): 51-60.

Hammill et al. Impact of heart failure on patients undergoing major noncardiac surgery. *Anesthesiology.* 2008; 108:559-567.

International Search Report and Written Opinion, PCT/US2009/052850, Sep. 29, 2009, 11 pages.

International Search Report and Written Opinion, PCT/US2009/069474, 10 pages, Feb. 25, 2010.

Jencks et al. Rehospitalizations among patients in the Medicare fee-for-service program. *N Engl J Med* 2009;360:1418-28.

Maurer et al. Ventricular structure and function in hypertensive participants with heart failure and a normal ejection fraction; the Cardiovascular Health Study. *J. Am. Col. Cardiol.* Mar. 6, 2007; 49(9): 982-85.

Non-Final Office Action, U.S. Appl. No. 12/536,247, mailed Feb. 16, 2012, 24 pages.

Notice of Allowance, U.S. Appl. No. 12/536,247, mailed Sep. 18, 2012, 8 pages.

Owings et al. Ambulatory and Inpatient procedures in the United States, 1996. National Center for Health Statistics. *Vital Health Stat* 13(139), 1998.

Pelletier et al. Increasing US Emergency Department Visit Rates and Subsequent Hospital Admissions for Atrial Fibrillation from 1993 to 2004. *Ann. Emerg Med.* Jan. 2008;51(1):58-65.

Polancyk et al. Right heart catheterization and the cardiac complications in patients undergoing noncardiac surgery: An observational study. *JAMA* 2001; 286: 309-314.

Practice Guidelines for Transesophageal Echocardiography. A report by the American Society of Anesthesiologists and the Society of Cardiovascular Anesthesiologists Task Force on Transesophageal Echocardiography. *Anesthesiology.* 1996: 986-1006.

Redfield et al. Burden of systolic and diastolic ventricular dysfunction in the community: appreciating the scope of the heart failure epidemic. *JAMA.* 2003; 289: 194-202.

Response to Non-Final Office Action, U.S. Appl. No. 12/536,247, filed Jun. 15, 2012, 12 pages.

Sandham et al. A randomized, controlled trial of the use of pulmonary-artery catheters in high-risk surgical patients. *N Engl J. Med.* vol. 348, No. 1, Jan. 2, 2003.

Standards for Basic Anesthetic Monitoring (Approved by the ASA House of Delegates on Oct. 21, 1986, and last amended on Oct. 25, 2005). [Http://www.asahg.org/publicationsAndServices/standards/02.pdf](http://www.asahg.org/publicationsAndServices/standards/02.pdf) last accessed Mar. 12, 2008.

U.S. Census Bureau. U.S. Interim Projections by Age, Sex, Race, and Hispanic Origin. [Http://www.census.gov/pc/www/usinterimproj/](http://www.census.gov/pc/www/usinterimproj/) Mar. 18, 2004. Last accessed Mar. 12, 2008.

U.S. Appl. No. 29/457,196, filed Jun. 7, 2013, Vežina.

U.S. Appl. No. 29/457,200, filed Jun. 7, 2013, Vežina.

U.S. Appl. No. 13/912,763, filed Jun. 7, 2013, Vežina.

* cited by examiner

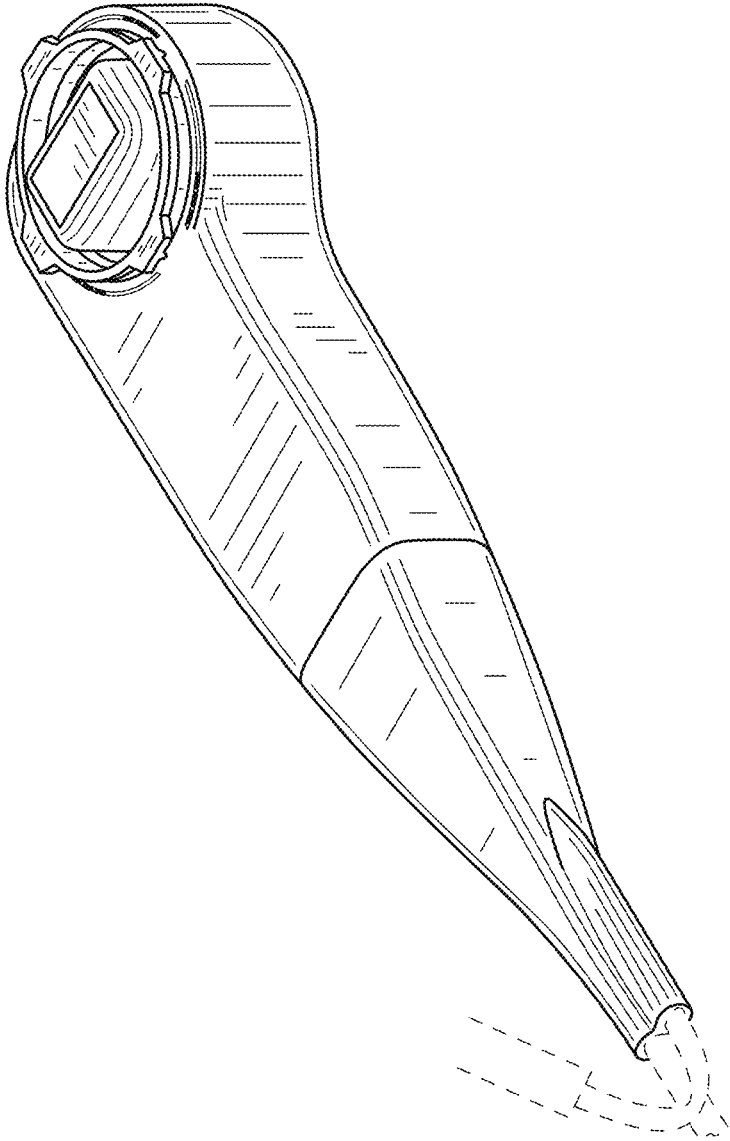


FIG.1

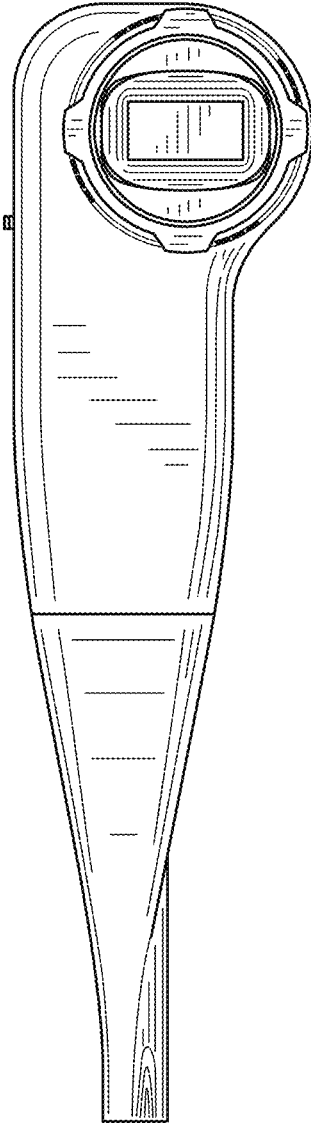


FIG.2

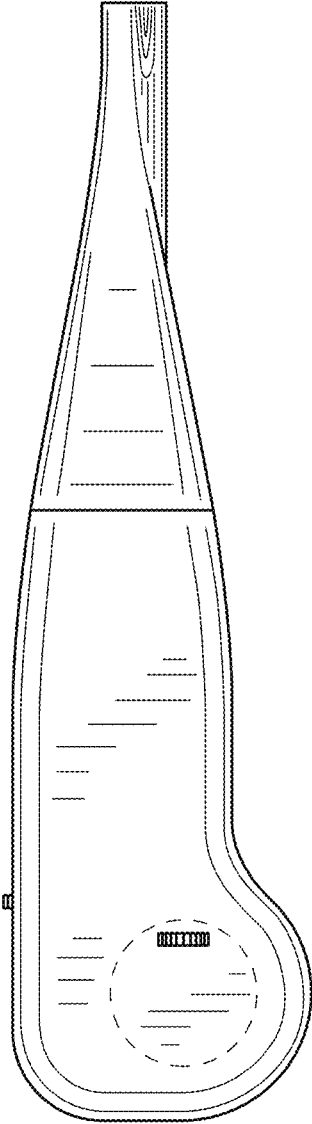


FIG.3

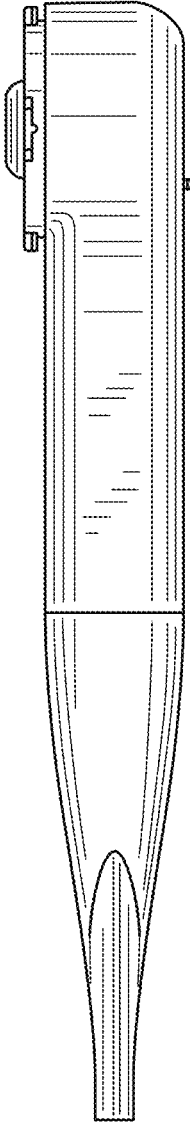


FIG.4

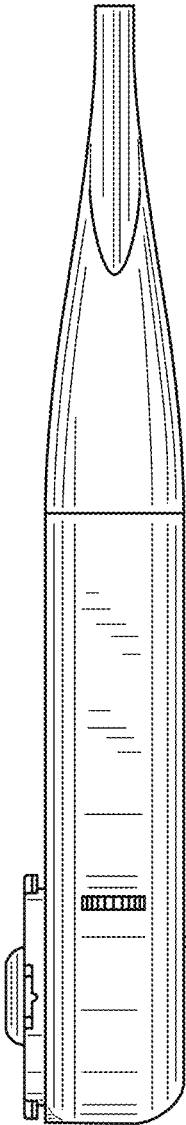


FIG.5

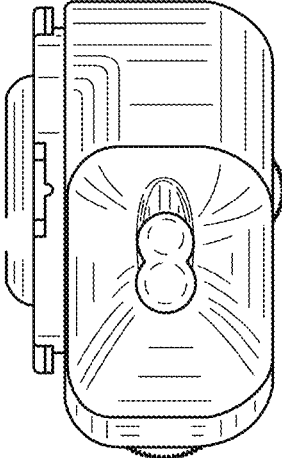


FIG.6

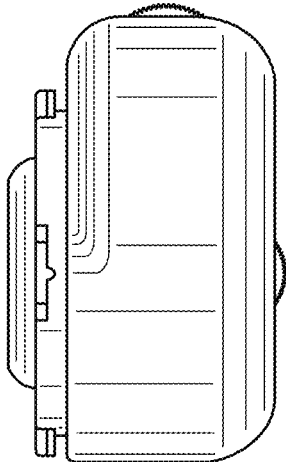


FIG.7