

**(12) PATENT**  
**(19) AUSTRALIAN PATENT OFFICE**

**(11) Application No. AU 199887429 B2**  
**(10) Patent No. 756423**

(54) Title  
Scintillation proximity test

(51) 6 International Patent Classification(s)  
G01N 033/60 G01N 033/543  
G01N 033/542 G01N 033/58

(21) Application No: 199887429 (22) Application Date: 1998.08.17

(87) WIPO No: WO99/09415

(30) Priority Data

(31) Number (32) Date (33) Country  
97306264 1997.08.18 EP

(43) Publication Date : 1999.03.08

(43) Publication Journal Date : 1999.05.06

(44) Accepted Journal Date : 2003.01.09

(71) Applicant(s)  
Amersham PLC

(72) Inventor(s)  
Robert A. Jessop

(74) Agent/Attorney  
DAVIES COLLISON CAVE, 1 Little Collins Street, MELBOURNE VIC 3000

(56) Related Art  
BEVERLOO H B ET AL. (1992) CYTOMETRY 13 PP 561-570

OPI DATE 08/03/99 APPLN. ID 87429/98  
AOJ? DATE 06/05/99 PCT NUMBER PCT/GB98/02459



AU9887429

1)

(51) International Patent Classification 6: G01N 33/60, 33/542, 33/543, 33/58		A1	(11) International Publication Number: <b>WO 99/09415</b> (43) International Publication Date: 25 February 1999 (25.02.99)
(21) International Application Number: PCT/GB98/02459 (22) International Filing Date: 17 August 1998 (17.08.98)		(81) Designated States: AU, CA, JP, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).	
(30) Priority Data: 97306264.9 18 August 1997 (18.08.97) EP  (44) Applicant (for all designated States except US): <del>NYCOMED</del> AMERSHAM PLC [GB/GB]; Amersham Place, Little Chalfont, Buckinghamshire HP7 9NA (GB).		<b>Published</b> <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>	
(72) Inventor; and (75) Inventor/Applicant (for US only): JESSOP, Robert, A. [GB/GB]; 64 Guenever Close, Thornhill, Cardiff CF4 9AH (GB).			
(74) Agents: PENNANT, Pyers et al.; Stevens Hewlett & Perkins, 1 Serjeants' Inn, Fleet Street, London, Greater London EC4Y 1LL (GB).			
(54) Title: SCINTILLATION PROXIMITY TEST			
(57) Abstract  The invention concerns scintillation proximity assays performed in multiwell plates where a charge coupled device is used to image the wells. Conventional phosphors emit blue light (350-450 nm) which is absorbed by yellow or brown assay components. This problem is addressed by the use of phosphors that emit radiation of longer wavelength (480-900 nm).			

SCINTILLATION PROXIMITY TEST

5 This invention concerns scintillation proximity tests, that is to say assays or other experiments involving the scintillation proximity principle.

10 Current scintillation proximity assay (SPA) technology involves the use of scintillant beads made from either cerium-doped yttrium silicate ( $Y_2SiO_5:Ce$ ) (hereafter referred to simply as yttrium silicate or YSi) or polyvinyltoluene (PVT) containing an organic scintillant such as PPO. Assays are carried out in aqueous buffers using radioisotopes such as  $^3H$ ,  $^{125}I$ ,  $^{14}C$ ,  $^{35}S$  or  $^{33}P$ , that emit low-energy radiation, the energy of which is easily dissipated in an aqueous environment. For example, the electrons 15 emitted by  $^3H$  have an average energy of only 6 keV and have a very short path length ( $\sim 1 \mu m$ ) in water. If a molecule labelled with one of these isotopes is bound to the bead surface, either directly or via interaction with another molecule previously coupled to the bead, the emitted radiation will activate the scintillant and produce light. The amount of light produced, 20 which is proportional to the amount of labelled molecules bound to the beads, can be measured conveniently with a liquid scintillation (LS) counter. If the labelled molecule is not attached to the bead surface, its radiation energy is absorbed by the surrounding aqueous solvent before it reaches the bead, and no light is produced. Thus, bound ligands give a 25 scintillation signal, but free ligands do not, and the need for a time-consuming separation step, characteristic of conventional radioligand binding assays, is eliminated. The manipulations required in the assays are reduced to a few simple pipetting steps leading to better precision and reproducibility.

30 PCT WO 91/08489 (Packard Instrument Company Inc.) describes a support body for use in scintillation proximity

radioimmunoassay, the support body being constructed of a scintillating material, having coupled to its surface a multiplicity of ligands such a antigens, antibodies, etc. capable of selectively binding a reactant of interest. Preferably the support bodies consist of yttrium silicate activated 5 with an inorganic cerium salt such as the oxide, carbonate, or chloride.

WO 94/26413 concerns the study of cellular and biochemical processes in living cells or in components of cells. Specifically described are devices and methods for the study of cellular and biochemical processes, using the scintillation proximity principle.

10 The simplicity of the scintillation proximity format allows almost complete automation of assays using robotic sample processors and microtitre plate scintillation counters. Consequently, SPA technology is capable of high throughput, which is particularly valuable in the case of drug- or sample-screening assays. SP assays have been carried out 15 routinely in 96-well microtitre plates which are counted 6 wells at a time in specially designed microtitre plate scintillation counters. The search for increasingly higher throughput has led the manufacturers of these counters to produce instruments capable of counting 12 wells at a time, thus doubling throughput. It has also seen the advent of 384-well plates, 20 although at present these can still only be counted 12-wells at a time.

A problem associated with SPA is that of colour quenching, caused by the presence in the assay medium of coloured compounds that absorb the light emitted by the current SPA bead types. Colour quenching attenuates the signal, thereby decreasing signal to noise and hence the 25 sensitivity. Many of the samples being screened by SPA assays are coloured and the majority of these are yellow or brown in colour and absorb light in the blue region of the visible spectrum. Both PVT- and  $Y_2SiO_5:Ce$ -based SPA beads emit light in the blue region (maximal emission normally in the range 350nm-450nm) and so are susceptible to this effect.

30 An alternative detection system suitable for use in low to ultra-low light level imaging applications in the biological and biomedical

sciences is CCD (Charge Coupled Device) Detection which has been used, for example, in assays which involve chemiluminescent, bioluminescent and fluorescence detection. Applications include immunoassays (Hooper *et al*, *J.Biolum.Chemilum.*, **9**, 113-122, (1994)), and the analysis of specific 5 fluorescent dye-labelled nucleic acids by hybridisation following electrophoretic separation of nucleic acid samples (EP 214713 to Astromed Ltd.). Ultra low-light imaging using CCD technology is quantitative and fast and the new generation of imaging instruments which use CCD cameras for detectors can image the whole of a plate at once and so have great 10 potential for increasing sample throughput compared with microtitre well plate scintillation counters. Area imaging, i.e. the simultaneous imaging by CCD of all wells in a microtitre well plate is considered to be particularly advantageous when used in conjunction with high well-density plates containing 96, 384, 864, or more wells, since the time required to make 15 measurements is significantly reduced compared with conventional scintillation counting techniques.

Imaging technology, in particular area imaging, has also been applied to isotopically labelled materials as an alternative to autoradiography. This approach has been most widely used in applications 20 such as the quantitative analysis of proteins by 2-D gel electrophoresis (Patterson, *et al*, *Biotechniques*, **15**(6), 1076, (1993)) and receptor localisation (Tang, *et al*, *Biotechniques*, **18**(5), 886, (1995)). An imaging 25 plate, coated with a radiation sensitive agent (e.g. strontium sulphide/samarium/cerium or barium fluorobromide/europium) is exposed to a radiolabelled sample and an image is formed due to radiation incident on the lanthanide metal coating of the plate. Following exposure, the image is read by means of an imaging plate reader.

CCD detection of SPA counts has also been reported (Englert, D., *Society for Biomolecular Screening, Second Annual 30 Conference October 14-17, (1996)*, pp209-221) using PVT-based microspheres. However, the photon count from the SPA wells was not

5 sensitive enough to enable usable results to be obtained, due to low light output of the beads, sub-optimal signal detection capability of the system, as well as quenching by coloured samples. For conventional scintillation counting, instruments can be calibrated to take into account colour  
10 5 quenching. However, in the case of CCD detection using conventional SPA beads and under normal assay conditions, the number of photons detected per disintegration was insufficient to enable determination of quenching levels and quench correction was not possible. To date there appear to be no reports of working assays in which sample detection and measurement was obtained using this technique.

15 There is a need for a means to overcome the dual problems of low sensitivity of current CCD-based detection as well as colour quench in conventional SPA bead technology. In one embodiment the invention provides use in a scintillation proximity test of a phosphor that has an emission maximum of 480nm - 900nm, and of a charge coupled device for detecting radiation emitted by the phosphor.

20 A scintillation proximity test is a test in which a surface carrying a phosphor is contacted with a body of fluid containing a radioisotope. Part of the radioisotope becomes immobilised adjacent the surface; the remainder of the radioisotope remains dispersed or dissolved in the fluid. The mean free path of electrons or other particles or radiation resulting from radioactive disintegrations of the radioisotope are small relative to the dimensions of the body of fluid, whereby that part of the radioisotope immobilised adjacent the surface is capable of exciting  
25 25 phosphor carried by the surface, but that part of the radioisotope dispersed or dissolved in the fluid is generally too far from the surface to be capable of exciting phosphor carried by the surface.

30 The surface may be massive, as for example a wall of a vessel or wells of a multiwell or microtitre plate; or particulate, as for example threads or beads. The phosphor may be present as a coating applied on a pre-formed surface; or may be dispersed in or constitute or



form part of the surface.

The test may be a chemical or biochemical assay, for example a competition assay such as an immunoassay or immunometric assay. Or the test may involve a study of living cells which are, or which 5 become, attached to the surface carrying the phosphor. Any test system in which a radioisotope becomes partitioned between a solid phase and a liquid phase is in principle suitable for the method of the invention.

A radioisotope may be present in free form or combined form, e.g. as an atom or ion; this may be useful for example when it is desired to 10 monitor the take up of the radioisotope by cells adhering to the surface carrying the phosphor. Or the radioisotope may be used to label an assay reagent; this may be useful for example when a labelled reagent is caused to compete with an unlabelled reagent for binding to another reagent immobilised on the surface carrying the phosphor.

15 A scintillation proximity test may be performed in a qualitative or more usually in a quantitative manner. For example, measurements may be performed in a static mode, as when the result of a competition assay is determined after a fixed time or at equilibrium. Alternatively a scintillation proximity assay may be performed in a dynamic mode, as when 20 radiolabel uptake by cells is monitored in real time. WO 94/26413 describes a scintillating microtitre plate and methods for studying cellular processes in real time. The scintillating microtitre plate is marketed by Amersham Lifescience under the name Cytostar-T<sup>TM</sup>.

The fluid is generally an aqueous or other liquid. The 25 radioisotope is preferably one which emits electrons having a mean free path up to 2000  $\mu\text{m}$  in aqueous media. These include isotopes commonly used in biochemistry such as  $^3\text{H}$ ,  $^{125}\text{I}$ ,  $^{14}\text{C}$ ,  $^{35}\text{S}$ ,  $^{45}\text{Ca}$ ,  $^{33}\text{P}$  and  $^{32}\text{P}$ , but does not preclude the use of other radioisotopes such as  $^{55}\text{Fe}$ ,  $^{86}\text{Rb}$ ,  $^{109}\text{Cd}$  and  $^{51}\text{Cr}$  which also emit electrons within this range.

30 The scintillation proximity test is preferably performed in the wells of a multiwell plate e.g. a microtitre plate. The phosphor may be

- 6 -

provided as beads dispensed into the wells of such a plate. Or the phosphor may be incorporated into the plate itself, either by direct incorporation into the plastic of the plate, or by coating, together with a binding agent. Examples of possible binding agents are calcium sulphate, 5 as used in the manufacture of tlc plates, and low-melting plastics such as polystyrene or copolymers of  $\alpha$ -methylstyrene and vinyltoluene. These devices may have 24, 96 or 384 wells as in existing plates or may have higher densities of wells such as 864, 1536, 2400 3456 or indeed any desired number. They can be used to perform cell-based or ligand binding 10 assays in conjunction with CCD camera based imagers. The phosphor preferably has an emission maximum of 500 nm – 700 nm, that is to say in the green or yellow or red region of the spectrum. The phosphors are stimulated by low energy electrons or other particles or radiation resulting from radioactive disintegrations of the radioisotope. These phosphors 15 generally have a higher light output than PVT based SPA beads or  $\text{Y}_2\text{SiO}_5:\text{Ce}$  beads and enable SPA assays to be imaged successfully. Moreover, all sample wells of a microtitre well plate can be imaged simultaneously by means of CCD detection. The longer wavelength green or red emissions alleviate the colour quenching problem which is at its 20 greatest in the blue region of the spectrum.

Some phosphors are commercially available for industrial applications, for example in cathode ray tube technology, lamp phosphors and X-ray phosphors. See for example Blasse and Grabmaier, Luminescent Materials, Springer-Verlag, Berlin, (1994) and US Patent 25 5,435,937. The preparation of charge-stabilised suspensions of small phosphor particles (e.g. yttrium oxysulphide- $\text{Eu}^{3+}$ , yttrium oxysulphide- $\text{Tb}^{3+}$ ) and their coupling to antibodies to give immunoreactive conjugates has been described (Beverloo, *et al*, Cytometry, 13, 561-570 (1992)). The phosphor conjugates were used in immunocytochemical applications by 30 binding to cells, followed by visualisation using a fluorescence microscope under UV light excitation. To date however, such phosphors have not been

described for use in counting applications involving radioactive tracers, particularly SPA

There are many suitable phosphors that may be used. Some consist of an inorganic host material doped with an activator. Examples of such host materials are yttrium silicate, yttrium oxide, yttrium oxysulphide, yttrium aluminium gallium oxide (YAG), yttrium aluminium garnet, sodium yttrium fluoride ( $NaYF_4$ ), lanthanum fluoride, lanthanum oxysulphide, yttrium fluoride ( $YF_3$ ), yttrium gallate, gadolinium fluoride ( $GdF_3$ ), barium yttrium fluoride ( $BaYF_5$  or  $BaY_2F_8$ ), gadolinium oxysulphide, zinc silicate, zinc sulphide and yttrium vanadate. The activator is generally a lanthanide or actinide moiety.

Other phosphors are organic chelates of lanthanide or actinide moieties. Light emission may be enhanced by combining or mixing the lanthanide or actinide chelate with a Lewis base enhancer such as for example an imido phosphorane. Examples of phosphors of this kind are described in EPA 556005. They may conveniently be used in solution or dispersion in polystyrene or other organic polymer.

The identity of the lanthanide or actinide moiety determines the emission wavelength of the phosphor. Preferred moieties are selected from terbium, europium, erbium, thulium, holmium, dysprosium, samarium, ytterbium, lutecium, gadolinium, uranium and uranyl  $UO_2$ , generally in the form of +2 or +3 ions.

Reference is directed to the accompanying drawings.

Figure 1 shows CCD detected signal from inorganic phosphor particles with PVT SPA beads and yttrium silicate particles for comparison.

Figure 2 shows CCD detected signal from organic chelate beads with PVT SPA beads for comparison.

Figure 3 shows absorbance spectra for dyes used in Example 2.

Figure 4 shows emission spectra for PVT SPA, yttrium silicate particles,  $Y_2O_3:Eu$  and YAG:Tb particles.

Figure 5 shows evaluation of streptavidin coated inorganic phosphor particles in a reverse transcription scintillation proximity assay detected by a CCD imaging system.

Figure 6 shows inhibition of HIV reverse transcriptase by 5 aurintricarboxylic acid, using streptavidin coated polystyrene beads and CCD imaging.

Figure 7 shows comparison of CCD detected signal; from 10 PST WGA coated beads and ChOA1 receptor/PIA agonist in the [<sup>35</sup>S]GTP $\gamma$ S G-protein coupled receptor assay with scintillation counting signal of PVT WGA coated SPA beads.

Figure 8 shows inhibition of [<sup>125</sup>I]EGF binding to WGA-coated 15 polystyrene beads using CCD imaging.

Figure 9 shows comparison of signal to noise ratios obtained 20 from PST streptavidin-coated beads and streptavidin-coated phosphor particles with CCD imaging and PVT streptavidin-coated SPA beads and scintillation counting.

Figure 10 shows comparison of the use of 2% w/w ALP-1 microplates and Cytostar-T plates used to monitor the uptake of [<sup>14</sup>C] thymidine in proliferating cells, using a CCD imaging system.

Figure 11 shows comparison of the use of 2% w/w ALP-1 25 microplates and Cytostar-T plates used to monitor the uptake of [<sup>14</sup>C] methionine in proliferating cells, using a CCD imaging system.

**Example 1**

Comparison of CCD detected signal from [3H]biotin bound to  
streptavidin coated phosphor particles, streptavidin coated  
5 polystyrene beads containing organic chelates of europium and  
terbium and streptavidin SPA beads

**Introduction**

Inorganic phosphors Y2O3:Eu, Y2O2S:Eu and YAG:Tb and  
10 organic chelate beads prepared from polystyrene containing tris(2,2,6,6-tetramethyl-3,5-heptanedionato)terbium III-diphenyl-phosphonimido-triphenylphosphorane (hereafter called ALP-1) or tris(naphthoyltrifluoroacetonato)europium III-(diphenyl-phosphonimido-triphenyl phosphorane)1 or 2 (hereafter called ALP-7 or ALP-7-diphos  
15 respectively) were surface-coated with streptavidin and were compared with streptavidin coated polyvinyl toluene (PVT) SPA beads and streptavidin coated yttrium silicate particles in a [3H]biotin binding assay. Coating of particles with proteins, such as streptavidin and other bioreactive species either covalently or by physical adsorption is  
20 accomplished by traditional methods known to those skilled in the art.

**Materials and Methods**

Inorganic phosphors used in example experiments are known materials and have been obtained from commercial suppliers in modified  
25 forms to facilitate their use in scintillation proximity assays. Organic chelate beads have been prepared by traditional methods known to those skilled in the art. The particles used for this experiment exemplify the CCD detection of the different reagents but are not necessarily optimal formulations of said reagents. The CCD imager used in the following examples is a prototype  
30 system supplied by Molecular Devices Inc. and incorporates a liquid nitrogen cooled CCD camera, supplied by Princeton Instruments Inc.

- 10 -

Alternative CCD imager detection systems under development are expected to give similar relative response with the different types of particles and plates with enhanced sensitivity. For examples employing white walled microtitre plates an appropriate bandpass filter was used to 5 eliminate phosphorescence from the plates.

Biotin Binding Assay

Streptavidin-coated particles and PVT SPA beads were suspended in phosphate buffered saline pH7.4 containing 0.01%w/v 10 sodium azide (hereafter PBS azide) at 5mg/ml. Stocks of [<sup>3</sup>H]biotin (Amersham TRK753) were made up in PBS azide to contain 5.1,10.3 and 20.7 pmoles of biotin in 100 $\mu$ l. Into the wells of a black microplate was pipetted 100 $\mu$ l samples of particle suspensions. Particle suspensions were mechanically mixed to ensure homogeneity of samples. 100 $\mu$ l of the each 15 of the three [<sup>3</sup>H]biotin solutions was added to the wells containing the different particles. Following the additions the plate was sealed and then incubated on a microplate shaker for 60 minutes at room temperature. The SPA signal was detected using a CCD camera imaging system. Non specific binding of [<sup>3</sup>H] biotin to particles was examined by measuring 20 signal detected in the presence of a large excess of unlabelled biotin. For all particles tested non specific binding of [<sup>3</sup>H] biotin was insignificant (not greater than 3% and typically not greater than 1% of signal from control wells).

25 Results

The results, in Figures 1 and 2, show the imager signal generated using three levels of [<sup>3</sup>H]biotin bound to 500 $\mu$ g of streptavidin coated phosphor particles, polystyrene particles containing organic chelates of europium and terbium and conventional SPA particles.

30

**Conclusions**

The data in Example 1 demonstrates that the CCD imager signal generated from [<sup>3</sup>H]biotin binding to streptavidin coated Y<sub>2</sub>O<sub>2</sub>S:Eu, Y<sub>2</sub>O<sub>3</sub>:Eu and YAG:Tb was at least 10 fold higher than the PVT SPA signal.

5 Polystyrene/ALP-7-diphos beads generate approximately 3 times the signal of PVT SPA beads.

**Example 2**

10 **Colour quench effects of yellow, orange and red dyes in a model**  
**[<sup>3</sup>H]biotin binding assay**

**Introduction**

The quenching of signal (counts) by coloured compounds is a  
15 well known phenomenon in conventional scintillation counting. Spectral  
overlap of the emissions of scintillating materials with the absorption  
spectra of coloured materials is a prerequisite for this to be observed.  
Dyes have been chosen to cover the range of sample colours commonly  
encountered in SPA screening assays (see dye absorption spectra in figure  
20 3 with the emission spectra of PVT SPA, yttrium silicate, Y<sub>2</sub>O<sub>3</sub>:Eu and  
YAG:Tb in figure 4 for reference). A model assay was set up to illustrate  
one of the advantages of the use of long wavelength emitting particles for  
signal detection, in the presence of coloured compounds with a CCD  
imager.

25 A [<sup>3</sup>H]biotin binding assay was used to determine the effect of  
coloured compounds on the imager signal generated using phosphor  
particles Y<sub>2</sub>O<sub>2</sub>S:Eu, Y<sub>2</sub>O<sub>3</sub>:Eu and YAG:Tb compared to yttrium silicate and  
PVT SPA beads. Additionally the relative quenching of organic chelate  
polystyrene beads was compared to PVT SPA beads.

**Materials and Methods**

Streptavidin coated inorganic phosphor particles, organic chelate containing polystyrene, yttrium silicate and PVT SPA beads were suspended in PBS azide, at 5mg/ml.

5 Acid yellow (Sigma A-4520) was dissolved in PBS azide at 360 $\mu$ g/ml.

Tartrazine (Sigma T-0388) was dissolved in PBS azide at 214 $\mu$ g/ml.

10 Methyl orange (Sigma M-3132) was dissolved in PBS azide at 196 $\mu$ g/ml.

Neutral red (Raymond and Lamb lot 5769) was dissolved in PBS azide at 234 $\mu$ g/ml.

15  $[^3\text{H}]$ Biotin (Amersham TRK753) was diluted in PBS azide to 107nM.

15

**Assay Protocol**

100 $\mu$ l aliquots of each bead suspension (500 $\mu$ g) was pipetted into the appropriate number of wells of black microplates followed by 100 $\mu$ l of the stock of  $[^3\text{H}]$  biotin. Plates were incubated for approximately 30 minutes at ambient temperature, to allow complete binding of biotin to particles. 10 $\mu$ l of the 4 dye solutions was added to the wells for each of the particles being tested with 10 $\mu$ l of buffer added to control wells. Plates were incubated on a microplate shaker for 60 minutes at room temperature. The SPA signal was detected using the CCD imaging system.

25

In-well concentrations of dyes were set at levels that give an absorbance in the range 0.3 to 0.5 at the absorption maximum wavelength for each dye, when measured in a 1cm path length spectrophotometer.

**Results**

30 The results, shown in Table 1, indicate that the europium containing phosphor particles or organic chelate beads do not show

quenching of signal by the dyes tested in this experiment. PVT SPA beads and yttrium silicate particles, as employed in conventional SPA assays, exhibit marked quenching of signal by these dyes. Terbium containing phosphor particles and organic chelate beads are quenched to a small extent by neutral red dye. This latter observation would be expected from the partial overlap of the absorption spectrum of neutral red with the emission spectrum of terbium.

Table 1. Comparison of quenching of CCD detected signal from  
inorganic phosphors, organic chelate particles and PVT SPA beads  
and yttrium silicate by yellow, orange and red dyes.

Bead Type	Acid Yellow 25	Tartrazine	Methyl Orange	Neutral Red
Y <sub>2</sub> O <sub>3</sub> :Eu	No quench	No quench	1%	No quench
YAG:Tb	No quench	No quench	No quench	No quench
Y <sub>2</sub> O <sub>2</sub> S:Eu	3%	4%	No quench	No quench
YSi SPA	26%	41%	23%	9%
PVT SPA	19%	10%	11%	25%
ALP-7 (Eu chelate)	No quench	No quench	No quench	No quench
ALP-1 (Tb chelate)	No quench	No quench	No quench	10%
ALP-diphos polystyrene (Eu chelate)	No quench	No quench	No quench	No quench

#### Conclusion

This example demonstrated that dyes which have an absorption spectrum overlapping with the emission spectrum of the scintillants in PVT SPA beads or yttrium silicate, can cause quenching of the emitted light from said species when excited by bound radiolabel. The CCD detected signal from europium or terbium containing phosphor

particles or organic chelates of said materials incorporated in polymeric matrices was not significantly quenched in the presence of these dyes.

### Example 3

5

#### Evaluation of concentration dependence of signal quenching by tartrazine for inorganic phosphor particles, ALP-7- diphos beads and PVT SPA beads and yttrium silicate particles

##### 10 Introduction

An experiment was set up to compare the concentration dependent quenching of signal from the different particles under investigation as detected by a CCD imager and a conventional scintillation counter.

15

##### Materials and methods

Streptavidin coated inorganic phosphor particles, ALP-7-diphos (polystyrene) beads, PVT SPA beads and yttrium silicate particles were suspended in PBS azide, at 10mg/ml.

20 Tartrazine (Sigma T-0388) was dissolved in PBS azide at 1070Tg/ml. [<sup>3</sup>H]Biotin (Amersham TRK 753) was diluted in PBS azide to 103 nM.

##### Assay protocol

25 100µl aliquots of particle suspensions were pipetted into the appropriate number of wells of black microtitre plates. 100µl of the stock solution of [<sup>3</sup>H] biotin (10.3pmoles) was added to each well. Plates were incubated at ambient temperature for 60 minutes to allow complete binding of biotin to particles. Tartrazine solution (1.2,4 or 8µl) was pipetted into appropriate wells of the plate, with PBS azide added to a final volume of

30 208µl per well. Triplicate data points were set up to contain 5.1, 10.2, 20.4 and 40.8 µg/ml of tartrazine respectively. The plates were incubated on a

- 15 -

microplate shaker for 60 minutes at room temperature. The SPA signal was detected using a CCD imaging system. The plate was then counted on a Wallac MicroBeta™ scintillation counter.

5 **Results**

The results of this example are shown in Table 2. For yttrium silicate particles it is observed that high levels of signal quenching are observed in CCD detection (33-58%) and also under conventional SPA counting conditions (54-82%). The observed level of quenching of signal 10 is related to the concentration of tartrazine present, with increasing levels of quench observed at increasing levels of added tartrazine. CCD detected signal for inorganic phosphor particles exhibit insignificant quenching of signal at the highest level of dye used (equivalent to approximately an absorbance reading of 2 at wavelength maximum in a 1cm path length 15 spectrophotometer). Quenching of CCD detected signal from PVT SPA beads (2-15%) is less pronounced than that observed for yttrium silicate particles but is still significant. Conventional scintillation counting of PVT SPA beads with the 4 levels of tartrazine present show very high signal quenching (37-87%) and exemplifies the requirement for colour quench 20 correction for conventional SPA assays. ALP-7-diphos polystyrene beads do not show significant quenching of CCD detected signal in this experiment (not greater than 4%).

**Table 2. Quenching emission of SPA particles by tartrazine at 4 different levels of dye. Comparison of quenching of signal detected by CCD detection and by a scintillation counter.**

CCD Detection	Tartrazine concentration, $\mu\text{g/ml}$			
	5.1	10.2	20.4	40.8
$\text{Y}_2\text{O}_2\text{S:Eu}$	No quench	No quench	No quench	No quench
$\text{Y}_2\text{O}_3\text{:Eu}$	No quench	No quench	No quench	No quench
YAG:Tb	No quench	No quench	No quench	3%
Ysi SPA	33%	44%	52%	58%
ALP-7-diphos polystyrene	No quench	1%	4%	No quench
PVT SPA	2%	4%	6%	15%

5

Microbeta, SPA mode	5.1	10.2	20.4	40.8
Ysi SPA	54%	61%	73%	82%
PVT SPA	37%	46%	69%	87%

### **Conclusions**

Colour quench correction is necessary to successfully carry out SPA assays using PVT SPA beads or yttrium silicate particles. For 10 inorganic phosphors or organic chelate beads containing europium and terbium insignificant levels of quenching is observed. The requirement for colour quench correction with these materials, if CCD imager detection is employed, is therefore obviated.

15

Example 4Assay of reverse transcriptase utilising streptavidin-coated phosphor particles

5

Introduction

The reverse transcriptase enzyme SPA assay ( Amersham NK 8972) is a homogeneous assay system which uses a biotinylated DNA/RNA oligonucleotide enzyme substrate which is captured on 10 streptavidin PVT SPA beads for quantification. Streptavidin-coated  $\text{Y}_2\text{O}_3:\text{Eu}$  and YAG:Tb particles were compared with streptavidin PVT SPA beads in this assay.

Materials and Methods

15

Reverse Transcriptase Assay

Biotinylated, ready annealed primer/template was added to the wells of a black microplate. This was followed by [ $^3\text{H}$ ]TTP (Amersham TRK576) in 75nM mixture of dATP, dCTP, dGTP and TTP buffered in 20 50mM tris/HCl pH 8.0, 80mM KCl, 10mM  $\text{MgCl}_2$ , 10mM DTT and 0.05%w/v Nonidet P40. The reactions were initiated with the addition of 0.075, 0.15 or 0.3 units of HIV reverse transcriptase (Amersham T3610Y). Plates were incubated at 37°C for 30 minutes and were terminated with the addition of stop reagent. 0.5mg of the appropriate streptavidin-coated phosphor or 25 PVT SPA beads was added and the plates were incubated at room temperature for 10 minutes. The signal generated was detected using the CCD imaging system.

Results

30

The results, illustrated in Figure 5, show the incorporation of radiolabelled nucleotide was dependent on the amount of reverse

- 18 -

transcriptase enzyme used. The data shows maximum signals of 3,200, 3,100 and 300 were observed using 0.3 units HIV reverse transcriptase in a 30 minute assay with  $Y_2O_3$ :Eu and YAG:Tb and PVT SPA beads respectively.

5

### Conclusion

This example shows the CCD imager signal generated in the reverse transcriptase SPA system was at least 10 fold higher using  $Y_2O_3$ :Eu and

10 YAG:Tb than with PVT SPA beads.

### Example 5

#### Assay of reverse transcriptase inhibition by aurintricarboxylic acid,

15 utilising streptavidin-coated polystyrene beads

#### Introduction

The reverse transcriptase enzyme SPA assay (Amersham NK8972) is a homogeneous assay system which uses a biotinylated 20 DNA/RNA oligonucleotide enzyme substrate which is captured on streptavidin PVT SPA beads for quantification. In this assay, streptavidin-coated organic chelate beads prepared from polystyrene (PST) containing europium were used and the inhibition of reverse transcriptase by aurintricarboxylic acid determined.

25

#### Materials and Methods

##### Reverse Transcriptase Assay

Biotinylated, ready annealed primer/template was added to 30 the wells of a white microplate. This was followed by [ $^3H$ ]TTP (Amersham TRK576) in 127nM mixture of dATP, dCTP, dGTP, and TTP buffered in

- 19 -

tris/HCl pH 8.0, 80mM KCl, 10mM MgCl<sub>2</sub>, 10mM DTT and 0.05%w/v Nonidet P40. Aurintricarboxylic acid at concentrations between 0.05 and 1 $\mu$ M was added and the reactions were initiated by the addition of 0.05 units of HIV reverse transcriptase (Amersham T3610Y). Plates were 5 incubated at 37°C for 20 minutes and were terminated with the addition of stop reagent. 0.1mg of streptavidin coated PST beads was added and the plates were incubated overnight at room temperature. The signal generated was detected using the CCD imaging system.

10 **Results**

The results, illustrated in Figure 6, show the inhibition of reverse transcriptase activity by aurintricarboxylic acid. The data shows that 85% inhibition can be achieved with 1 $\mu$ M of inhibitor and IC<sub>50</sub> value of 0.23 $\mu$ M was determined. This is comparable to the value of 0.18 $\mu$ M 15 determined for the SPA assay.

**Conclusion**

This example shows that polystyrene europium beads and a known inhibitor of reverse transcriptase can be used to determine IC<sub>50</sub> 20 values in the reverse transcriptase SPA assay with CCD imaging.

**Example 6**

**Evaluation of the GTP $\gamma$ S G-protein coupled receptor assay using wheat germ agglutinin (WGA)-coated polystyrene beads**

25

**Introduction**

The GTP $\gamma$ S G-protein coupled receptor SPA assay (Amersham RPNQ0210) is a homogeneous assay system which uses wheat germ agglutinin (WGA)-coated PVT SPA beads to bind receptor. 30 Agonist-induced or inverse agonist-induced activity for receptors coupled to GTP-binding proteins (G-proteins) can be quantified directly in the

- 20 -

presence of added [<sup>35</sup>S] GTP $\gamma$ S and GDP. Coated organic chelate beads prepared from polystyrene (PST) containing europium were therefore compared with WGA-coated PVT SPA beads in this assay.

5 **Materials and Methods**

**GTP $\gamma$ S G-protein Coupled Receptor SPA Assay**

3.75 $\mu$ g of cloned rat adenosine A1 receptor (BioSignal BSR-MA1R), 0.375mg of appropriate WGA-coated bead, 10 $\mu$ M of (-)-N<sup>6</sup>-(2-10 phenylisopropyl-adenosine) (PIA) agonist, 5 $\mu$ M of GDP, +/- 10 $\mu$ M of GTP $\gamma$ S (to determine non-specific binding) and 0.2-0.4nM of [<sup>35</sup>S]GTP $\gamma$ S were added to the wells of a white microplate in a final volume of 50 $\mu$ l of assay buffer, comprising of 20mM HEPES, 100mM NaCl, 10mM MgCl<sub>2</sub> and 1mM EDTA pH7.4. Plates were incubated at room temperature for 30 15 minutes and then centrifuged for 10 minutes at 1200rpm and 15°C. The signal generated was detected using the CCD imaging system.

**Results**

The results, illustrated in Figure 7, show the scintillation counter and imager signals generated in the GTP $\gamma$ S G-protein coupled receptor SPA assay in the presence and absence of PIA agonist using WGA-coated PST imager beads and PVT SPA beads. The data shows that a similar signal to noise ratio can be achieved in the imaged assay to that achieved in the SPA assay.

25

**Conclusion**

This example shows that polystyrene europium beads can be used with [<sup>35</sup>S] radiolabel in a miniaturized receptor assay to give a comparable signal to noise ratio to that obtained with conventional SPA.

30

Example 7

Assay of Epidermal Growth Factor (EGF) binding to EGF receptor,  
using wheat germ agglutinin (WGA)-coated organic polystyrene  
5 beads containing organic chelates of europium

Introduction

The interaction of [<sup>125</sup>I] EGF (Amersham IM196) with EGF receptor (EGF-R) expressed by the A431 human cell line can be studied  
10 using SPA in a homogeneous assay system in which the receptor is captured onto WGA-coated PVT SPA beads. In this assay, WGA-coated organic chelate beads prepared from polystyrene (PST) containing europium were used and the inhibition of [<sup>125</sup>I] EGF binding by unlabelled EGF determined.

15

Materials and MethodsEGF Receptor Assay

25<sup>g</sup> of A431 membrane (in house preparation) was pre-coupled to 0.25mg of WGA-coated PST bead for 2 hours at room temperature. This was then transferred to a white microplate and 400pM of [<sup>125</sup>I] EGF (Amersham IM196) added in assay buffer, comprising of 20mM HEPES pH7.5, 2mM CaCl<sub>2</sub>, 0.1% (w/v) BSA fraction V, with unlabelled EGF at concentrations between 0 and 100nM. Plates were incubated at 25 room temperature for 3 hours and the signal generated detected using the CCD imaging system.

Results

The results, illustrated in Figure 8, show the inhibition of [<sup>125</sup>I] EGF binding to WGA-coated PST beads. From the data, an IC<sub>50</sub> value of

- 22 -

5nM was determined which is comparable to the value of 2nM determined for the SPA assay.

#### Conclusion

5 This example shows that polystyrene europium beads and unlabelled EGF can be used to determine IC<sub>50</sub> values in the [<sup>125</sup>I] EGF receptor binding assay with CCD imaging.

#### Example 8

10

#### Assay of Mitogen Activated Protein (MAP) Kinase enzyme assay utilising streptavidin-coated organic polystyrene beads and streptavidin-coated inorganic phosphor particles

15

#### Introduction

The mitogen activated protein (MAP) kinase SPA [<sup>33</sup>P] assay (Amersham RPNQ0220) is a homogeneous assay system which uses streptavidin-coated PVT SPA beads to bind [<sup>33</sup>P]-labelled biotinylated myelin basic protein (bMBP) substrate. In this assay, streptavidin-coated organic chelate beads prepared from polystyrene (PST) containing europium and inorganic phosphor particles doped with europium were compared with streptavidin-coated PVT SPA beads in this assay.

#### Materials and Methods

25

#### MAP Kinase Assay

Reaction buffer containing 50pmols of bMBP substrate, 25pmols of ATP, 250nmols MgCl<sub>2</sub> and 50mM MOPS was added to the wells of a white microplate. 0.1 $\mu$ Ci of [<sup>33</sup>P] ATP (BF1000) and ERK-1 enzyme, at 0.01 $\mu$ g to 2 $\mu$ g, were then added. Plates were incubated at 37°C for 30 minutes and the reaction terminated by addition of stop buffer

- 23 -

containing 50mM ATP and 0.25mg of each bead type. The plates were then centrifuged for 10 minutes at 800rpm and 15°C. The signal generated was detected using the CCD imaging system.

5 **Results**

The results, illustrated in Figure 9, show the signal to noise ratios generated in the MAP kinase enzyme assay using streptavidin-coated PST and phosphor imager beads and PVT SPA beads. The data shows that a similar or better signal to noise ratio can be achieved in the 10 imaged assay to that achieved in the SPA assay.

**Conclusion**

This example shows that both phosphor particles and polystyrene europium beads can be used with [<sup>33</sup>P] radiolabel in a 15 miniaturized enzyme assay to give a comparable or better signal to noise ratio to that obtained with conventional SPA.

**Example 9**

20 **Comparison of 2% w/w ALP-1 and Cytostar-T microplates to monitor the uptake of [<sup>14</sup>C]thymidine in proliferating cells using a CCD imaging system**

**Introduction**

25 White 96-well microplates which were manufactured to incorporate the scintillant ALP-1 in the plate base were evaluated in Cytostar-T applications. 2% w/w-ALP-1 plates were compared with Cytostar-T plates in a [<sup>14</sup>C]thymidine uptake assay using adherent cells.

**Materials and Methods****Routine Cell Growth Conditions**

V-79 cells (ECACC no.86041102) were routinely grown at 5 37°C in a humidified 5% CO<sub>2</sub> incubator in DMEM (ICN/FLOW 12-332-54) supplemented with 10% FBS (GIBCO/BRL 10099-117), 2mM L-glutamine (ICN/FLOW 16-801-49), 50IU/ml penicillin and 200µg/ml streptomycin (ICN/FLOW 16-700-49). For routine subculture cells were passaged at 1:20 to 1:40 dilution.

10

**Thymidine uptake assay**

V-79 cells were seeded at 1 x 10<sup>4</sup>/well into 2% w/w ALP-1 and Cytostar-T plates and were incubated for 24 hours at 37°C with 5% CO<sub>2</sub>. Following this initial incubation 0.5µCi [<sup>14</sup>C]thymidine (Amersham CFA532) 15 was added to the cells. Thymidine uptake was followed over 24 hours by counting the plates at intervals. The plates were incubated at 37°C with 5% CO<sub>2</sub> when not being counted. The signal generated was counted using the CCD imaging system.

20

**Results**

The results in Figure 10 show that [<sup>14</sup>C]thymidine uptake by V-79 cells was dependent on the period of incubation. Maximum [<sup>14</sup>C]thymidine uptake signals of 5437 and 6953 were observed for 2% w/w ALP-1 and Cytostar-T plates respectively after 24 hours.

25

**Conclusion**

The data in this example shows that the CCD imager signal generated in a [<sup>14</sup>C]thymidine uptake assay using a 2% w/w ALP-1 plate was comparable to the Cytostar-T plate signal.

30

Example 10

Comparison of 2% w/w ALP-1 and Cytostar-T microplates to monitor  
the uptake of [<sup>14</sup>C]methionine in proliferating cells using a CCD  
imaging system

Introduction

2% w/w ALP-1 plates were compared with Cytostar-T plates in a [<sup>14</sup>C]methionine uptake assay. The procedures and conditions of Example 9 were used in this experiment.

Materials and Methods

Methionine uptake assay

V-79 cells were seeded at 5 x 10<sup>3</sup>/well into 2% w/w ALP-1 and Cytostar-T plates and were incubated for 24 hours at 37°C with 5% CO<sub>2</sub>. Following this initial incubation the medium was aspirated from the wells and the cell monolayer washed once with sterile phosphate buffered saline. 200µl of methionine depleted DMEM (ICN/FLOW 16-422-49) containing 0.5µCi [<sup>14</sup>C]methionine was added to the cells. The uptake was followed over 24 hours by counting the plates at intervals. The plates were incubated at 37°C with 5% CO<sub>2</sub> when not being counted. The signal generated was counted using the CCD imaging system.

Results

The results in Figure 11 show [<sup>14</sup>C]methionine uptake was dependent on the period of incubation, with maximum uptake signals of 15865 and 18455 observed for 2% w/w ALP-1 and Cytostar-T plates respectively after 24 hours.

Conclusion

In this example the results show that the CCD imager signal observed in a [<sup>14</sup>C]methionine uptake assay using a 2% "w/w ALP-1 plate 5 was comparable with the Cytostar-T plate signal.

The reference to any prior art in this specification is not, and should not be taken as, an acknowledgment or any form of suggestion that that prior art forms part of the common general knowledge in Australia.

10 Throughout this specification and the claims which follow, unless the context requires otherwise, the word "comprise", and variations such as "comprises" and "comprising", will be understood to imply the inclusion of a stated integer or step or group of integers or steps but not the exclusion of any other 15 integer or step or group of integers or steps.



THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

5 1. Use in a scintillation proximity test of a phosphor that has an emission maximum of 480 nm – 900 nm, and of a charge coupled device for detecting radiation emitted by the phosphor.

2. Use as claimed in claim 1, wherein the scintillation proximity test is performed in wells of a multiwell plate.

10 3. Use as claimed in claim 2, wherein the charge coupled device is used to simultaneously image all the wells of the multiwell plate.

4. Use as claimed in any one of claims 1 to 3, wherein the phosphor has an emission maximum of 500 nm – 700 nm.

15 5. Use as claimed in any one of claims 1 to 4, wherein the phosphor is an inorganic host material doped with an activator which is a lanthanide or actinide moiety.

6. Use as claimed in any one of claims 1 to 4, wherein the phosphor is an organic chelate of a lanthanide or actinide moiety.

7. Use as claimed in claim 5 or claim 6, wherein the lanthanide or actinide moiety is selected from terbium, europium, erbium, thulium, holmium, dysprosium, samarium, ytterbium, lutecium, gadolinium, uranium and uranyl  $UO_2^{3+}$ .

20 8. A method of performing a scintillation proximity test, by contacting a solid surface comprising a phosphor with a fluid medium, causing a radiolabelled reagent to become divided into two fractions one bound to the solid surface and the other in the fluid medium, and detecting the fraction of the radiolabelled reagent bound to the solid surface, characterised by using a phosphor that has an emission maximum of 480nm - 900nm and a charge coupled device for detecting radiation emitted by the phosphor.

25 9. The method of claim 8, wherein the scintillation proximity test

30



is performed in wells of a multiwell plate and the charge coupled device is used to image simultaneously all the wells of the multiwell plate.

5 10. The method of claim 8 or claim 9, wherein the phosphor is an organic chelate of europium or an inorganic host material doped with europium.

11. Use of a phosphor and a charge coupled device  
10 according to any one of claims 1 to 7 substantially as hereinbefore described with reference to the examples.

12. A method of performing a scintillation proximity test according to any one of claims 8 to 10 substantially as hereinbefore 15 described with reference to the examples.

DATED this 11<sup>th</sup> day of November 2002

Amersham plc

20  
by DAVIES COLLISON CAVE  
Patent Attorneys for the Applicants



1/6

Fig.1.


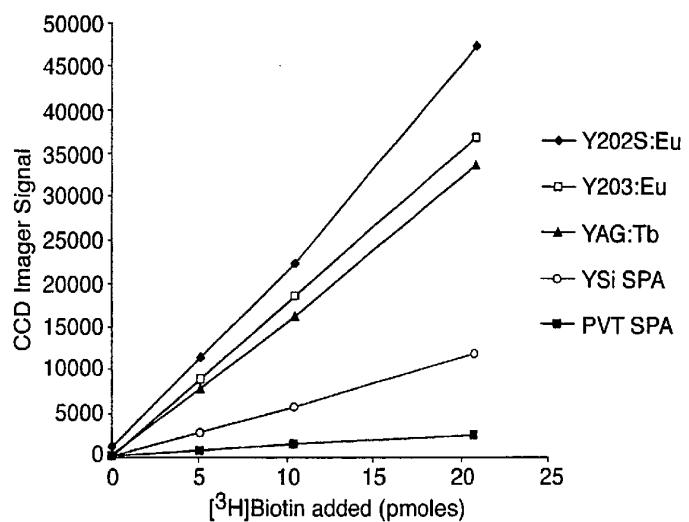


Fig.2.

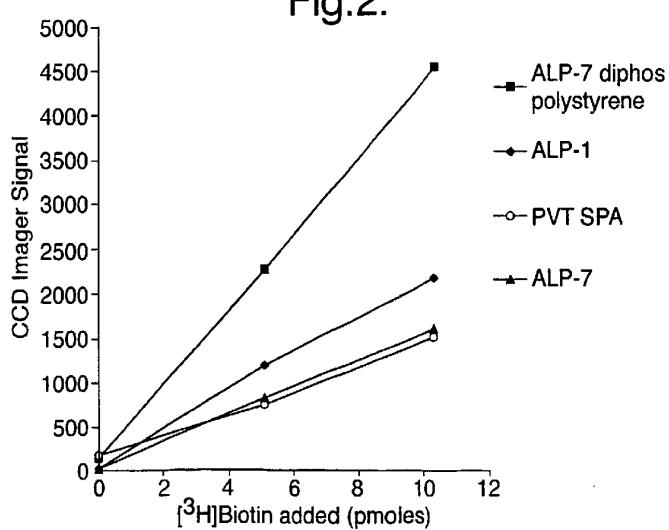

2/6

Fig.3.

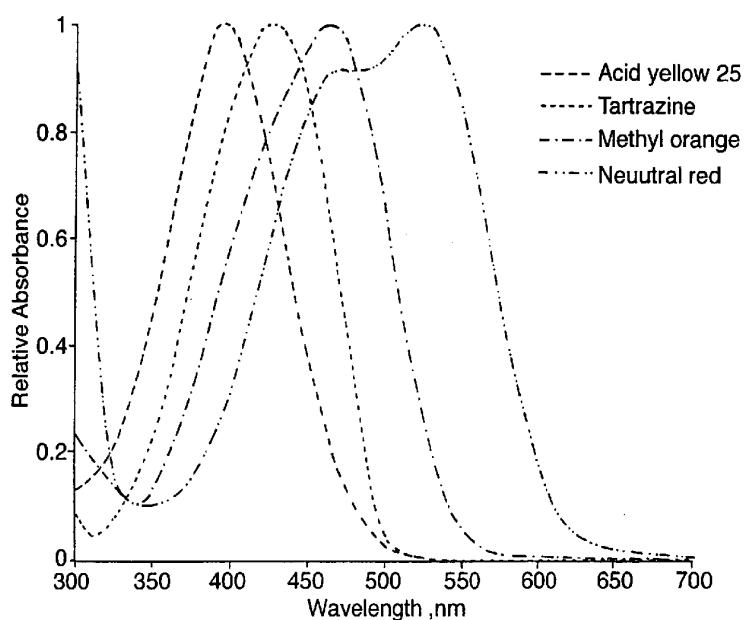


Fig.9.



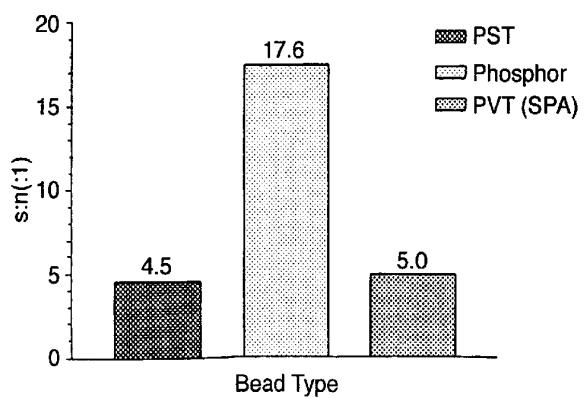


Fig.4.

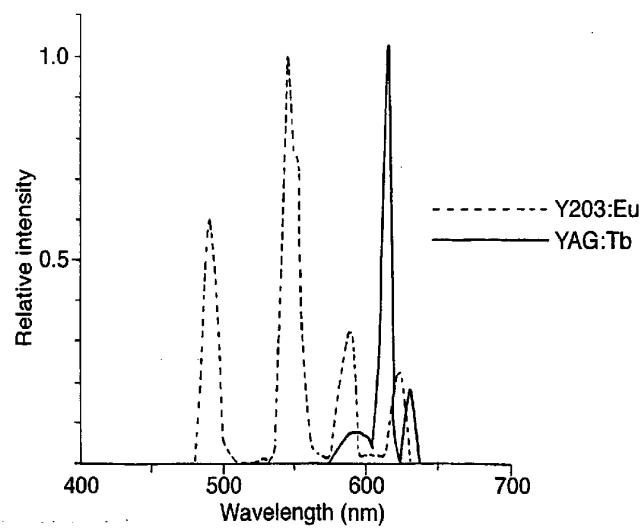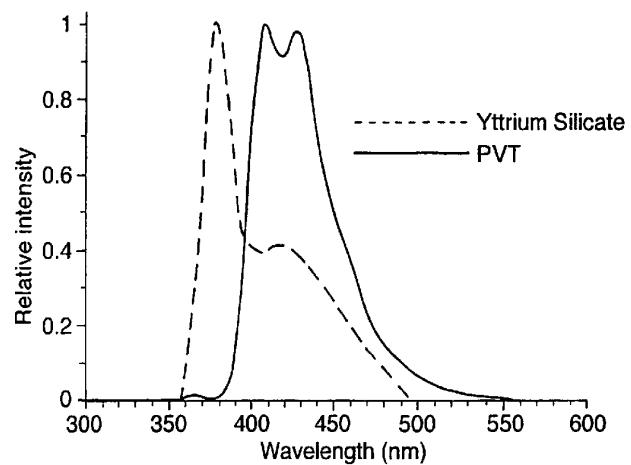

4/6

Fig.5.

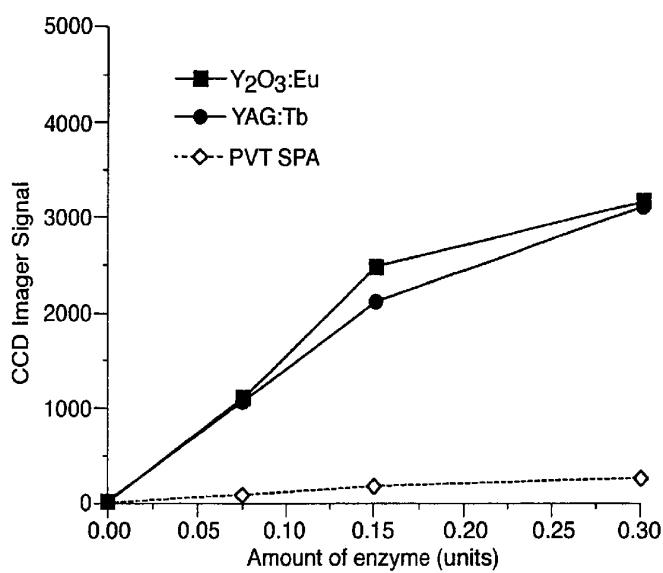


Fig.6.

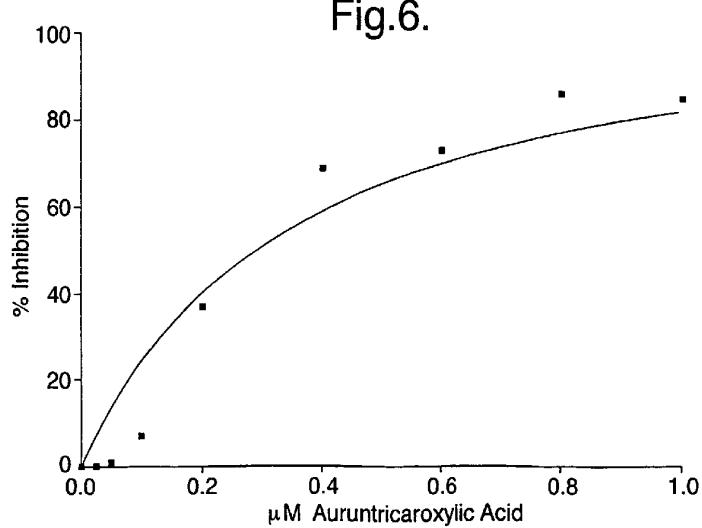


Fig.7.


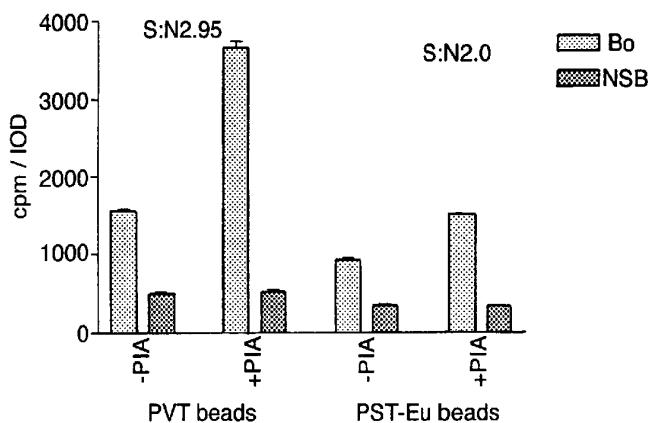


Fig.8.

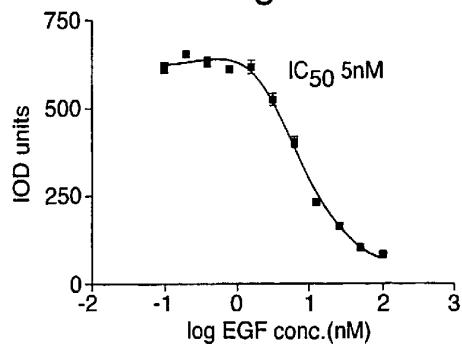

6/6

Fig.10.

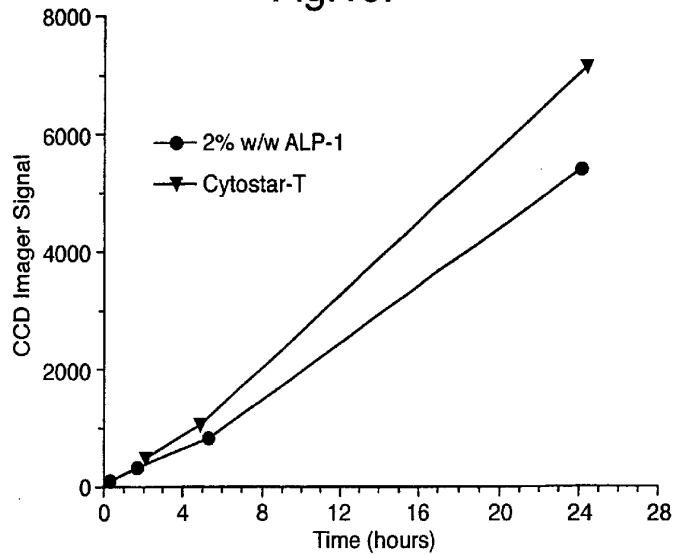


Fig.11.

