

(43) **Pub. Date:** **Feb. 28, 2013**

Publication Classification

(52) **U.S. Cl.** 623/2.19

(57) **ABSTRACT**


A prosthetic mitral valve assembly is disclosed. The assembly comprises a radially-expandable stent including a lower portion sized for deployment between leaflets of a native mitral valve and an upper portion having a flared end. The upper portion is sized for deployment within the annulus of the mitral valve and the flared end is configured to extend above the annulus. The stent is formed with a substantially D-shape cross-section for conforming to the native mitral valve. The D-shape cross-section includes a substantially straight portion for extending along an anterior side of the native mitral valve and a substantially curved portion for extending along a posterior side of the native mitral valve. The assembly further includes a valve portion formed of pericardial tissue and mounted within an interior portion of the stent for occluding blood flow in one direction.

(21) Appl. No.: 13/660,875

(22) Filed: **Oct. 25, 2012**

Related U.S. Application Data

(63) Continuation of application No. 12/113,418, filed on May 1, 2008.

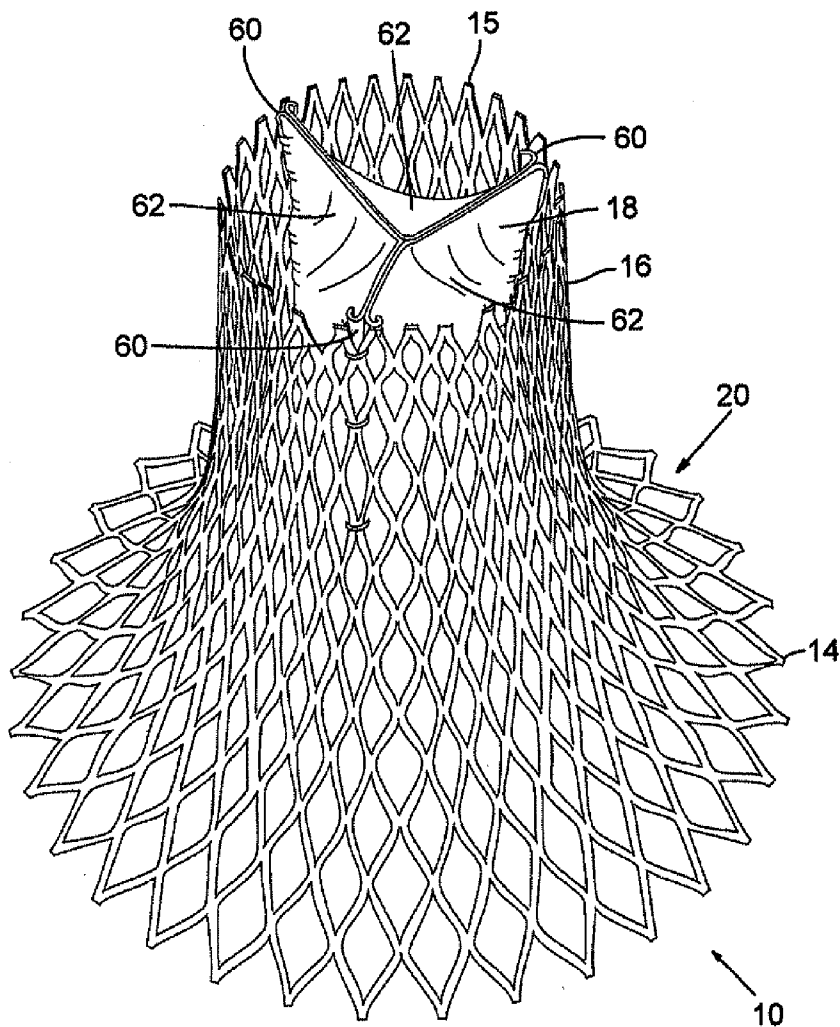

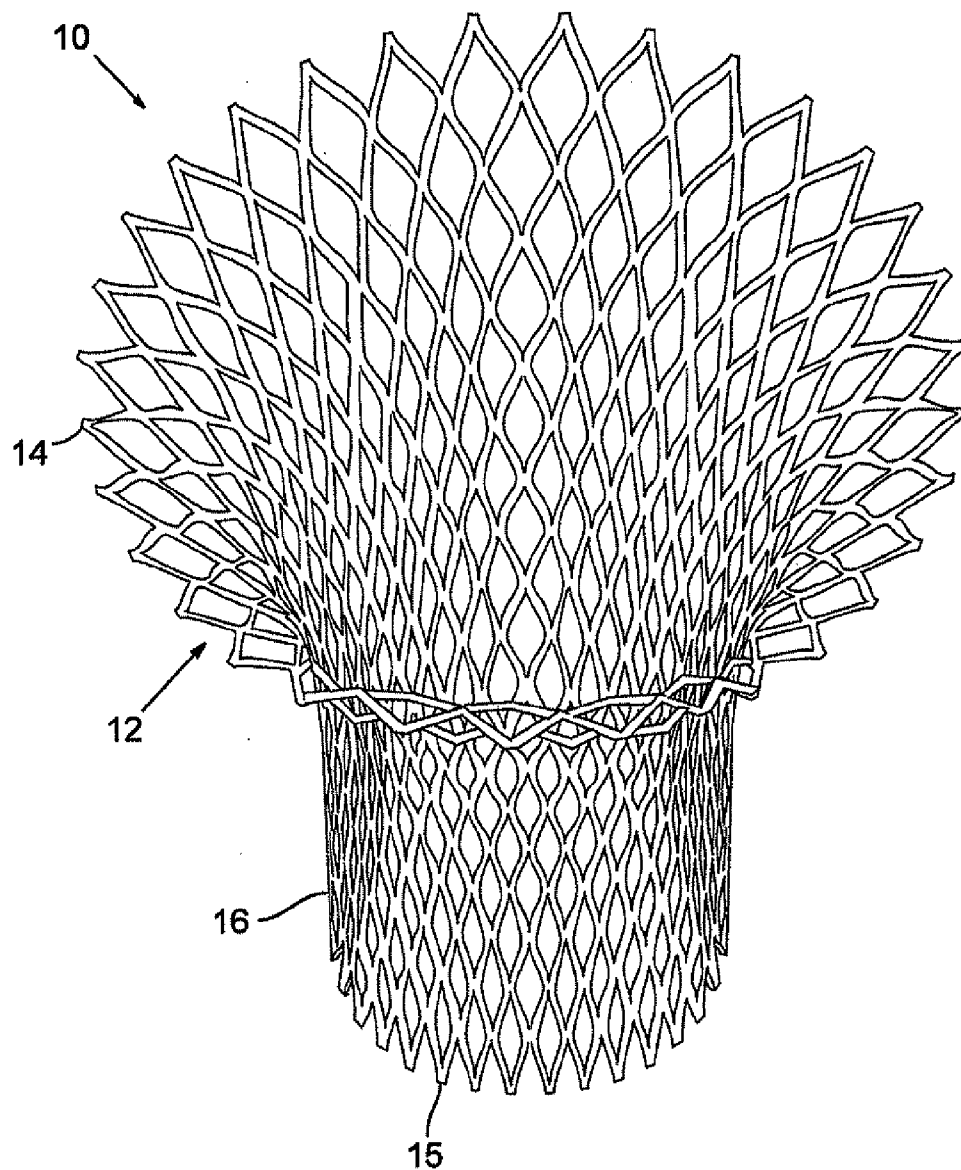


FIG. 1

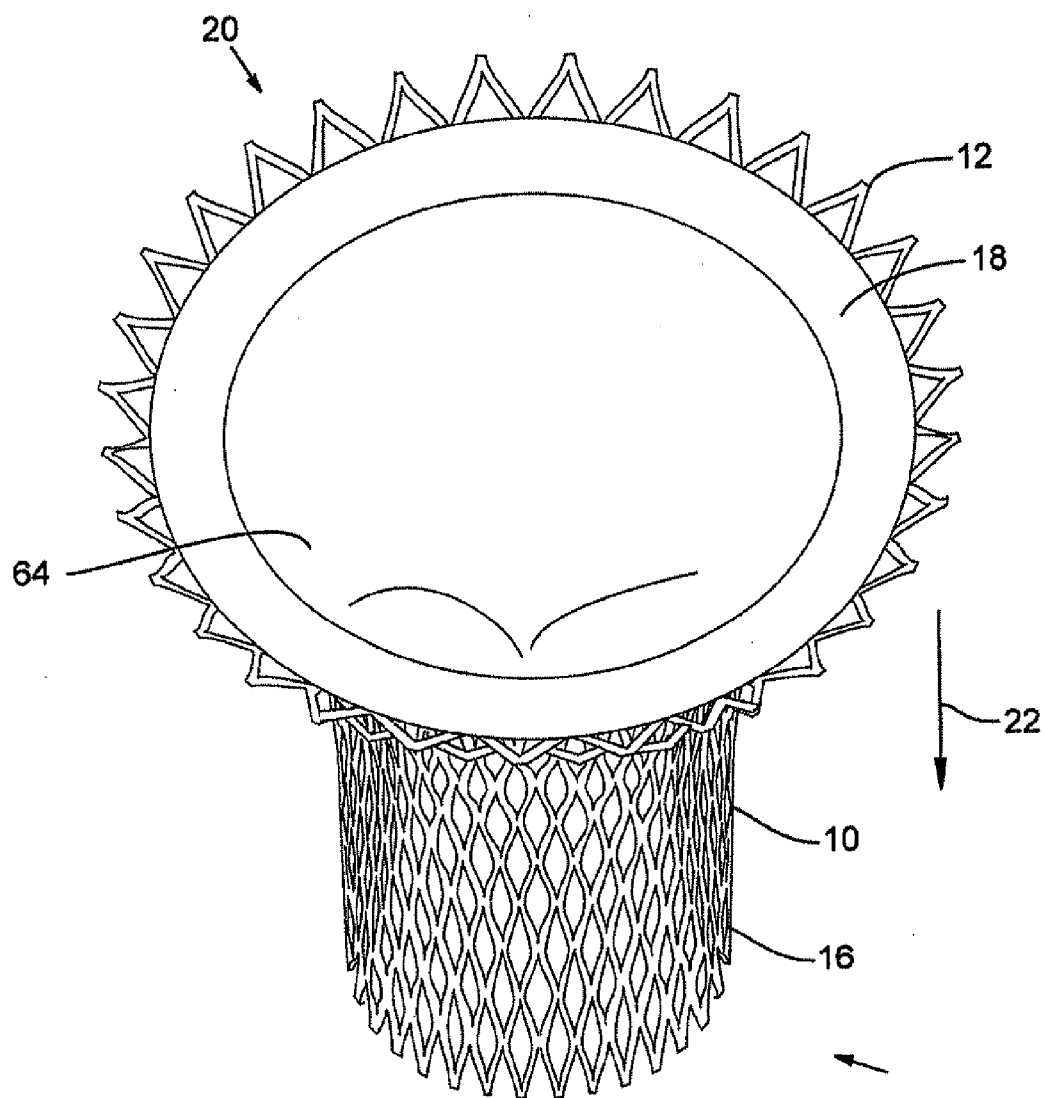


FIG. 2A

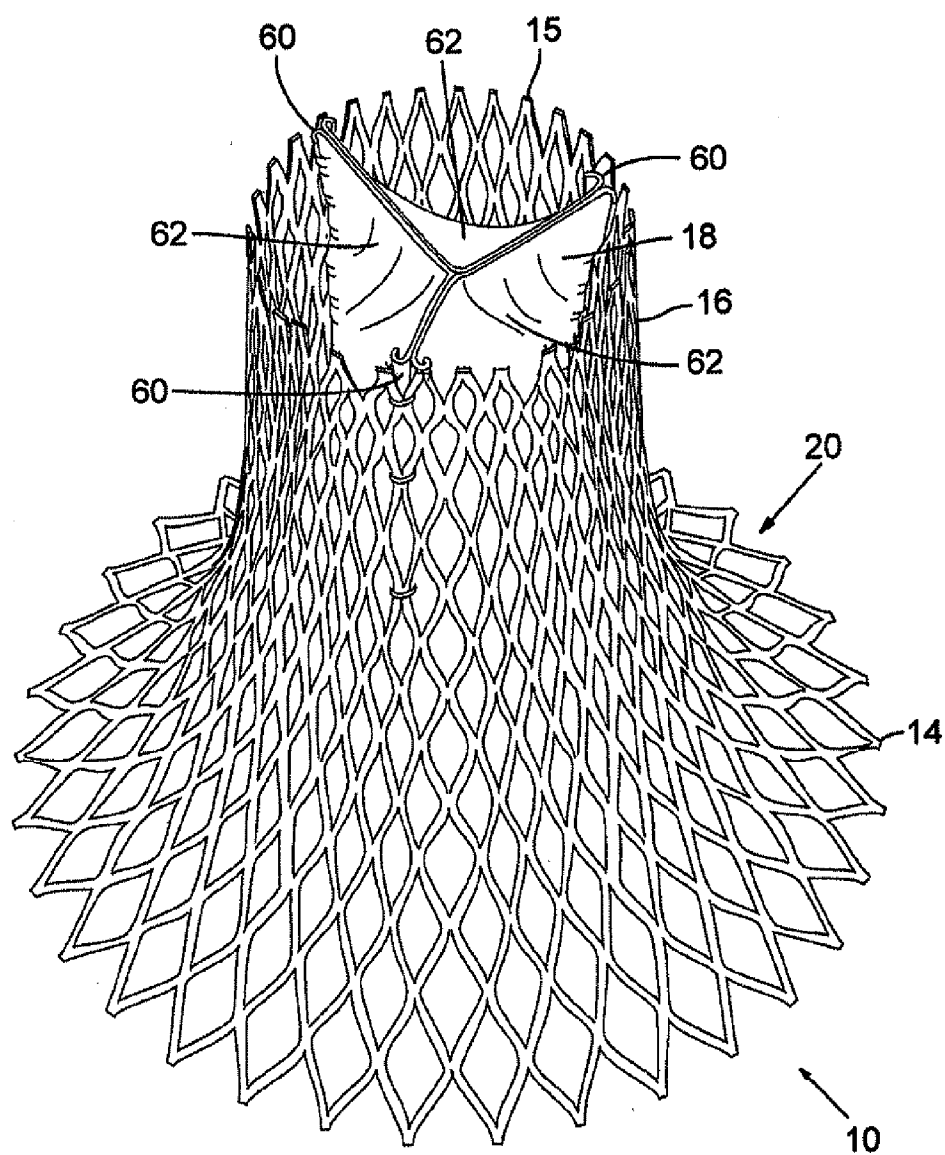
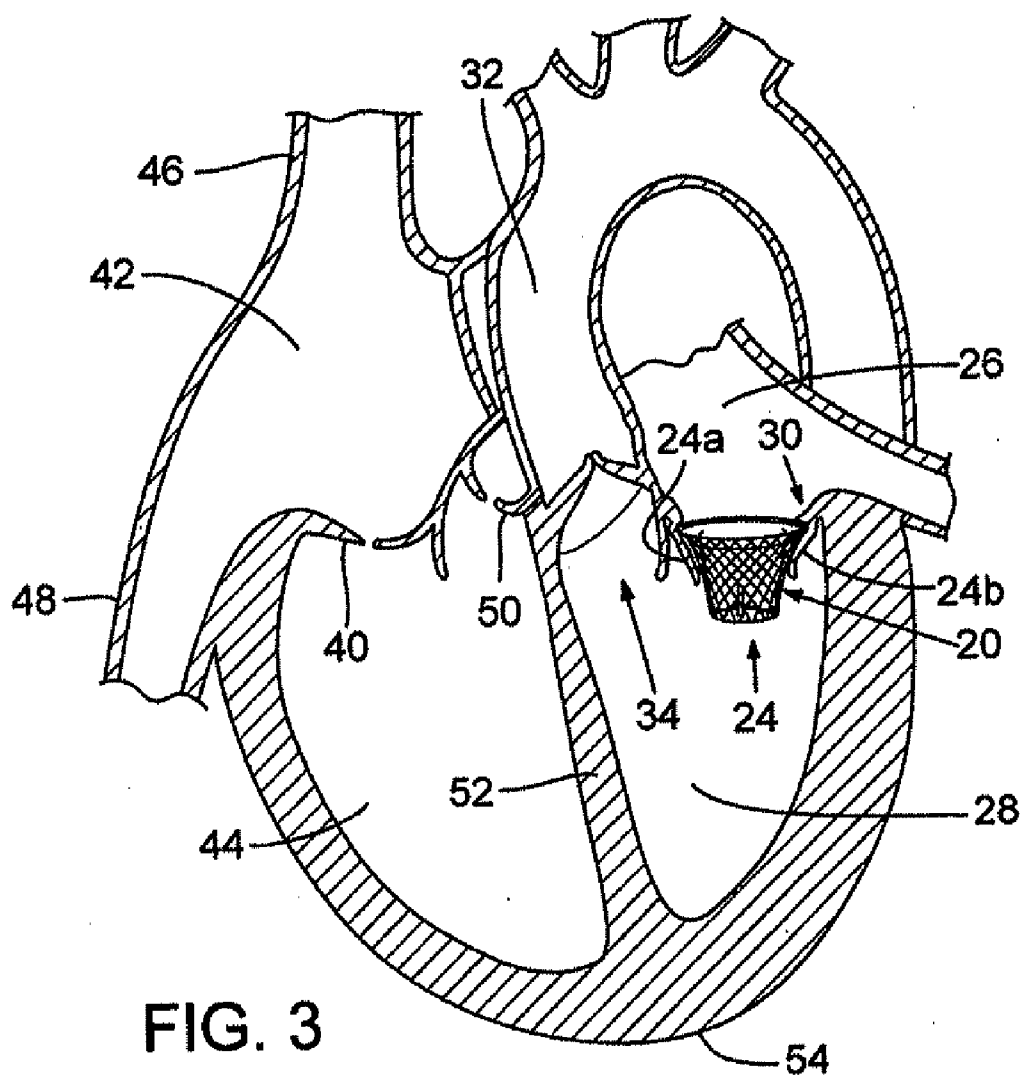
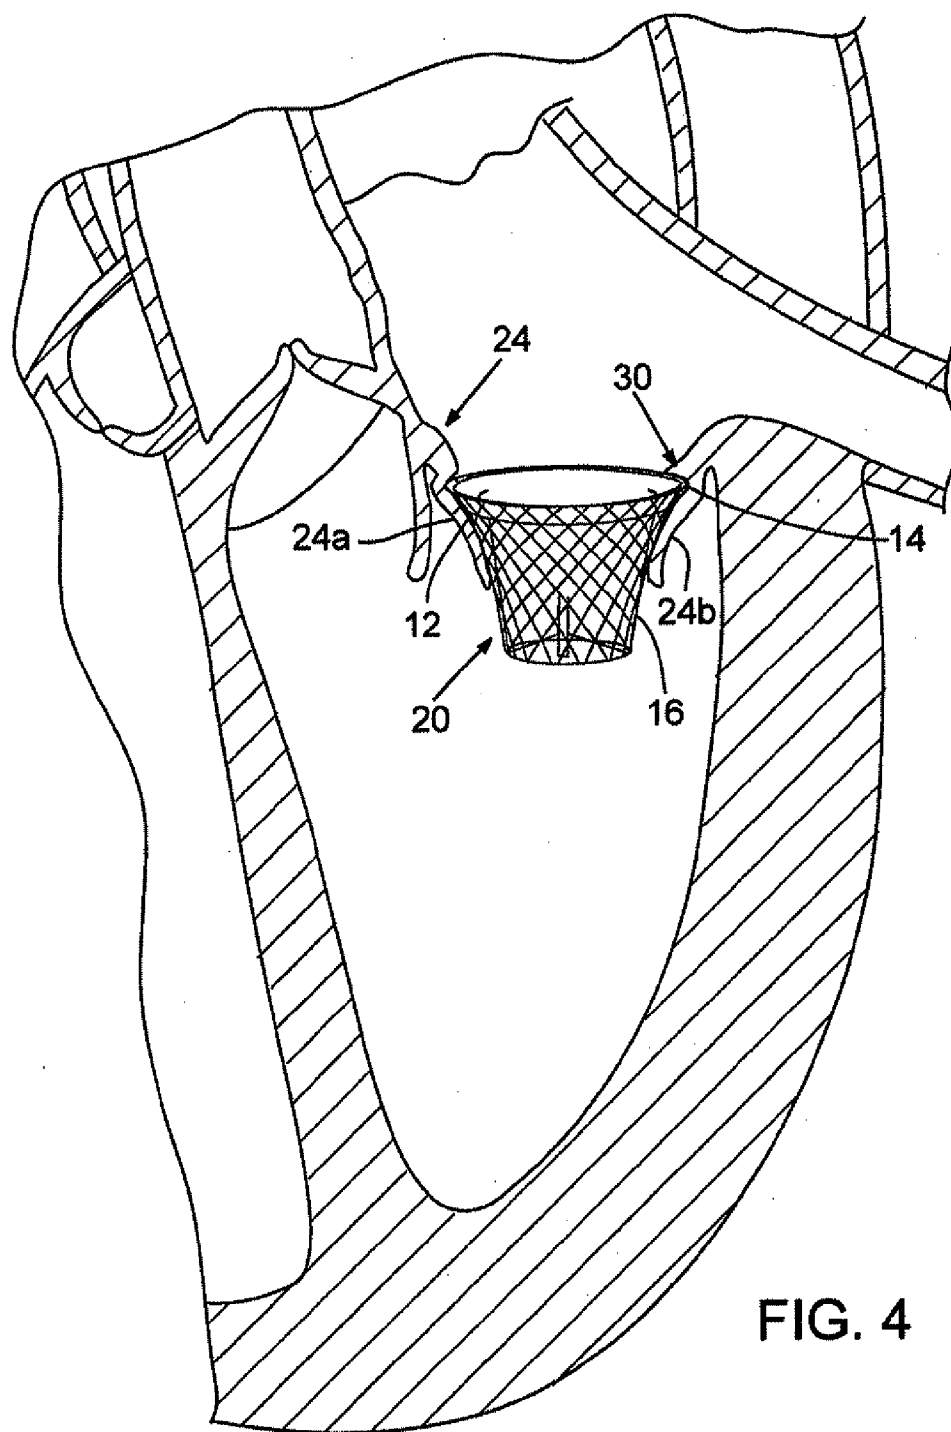


FIG. 2B





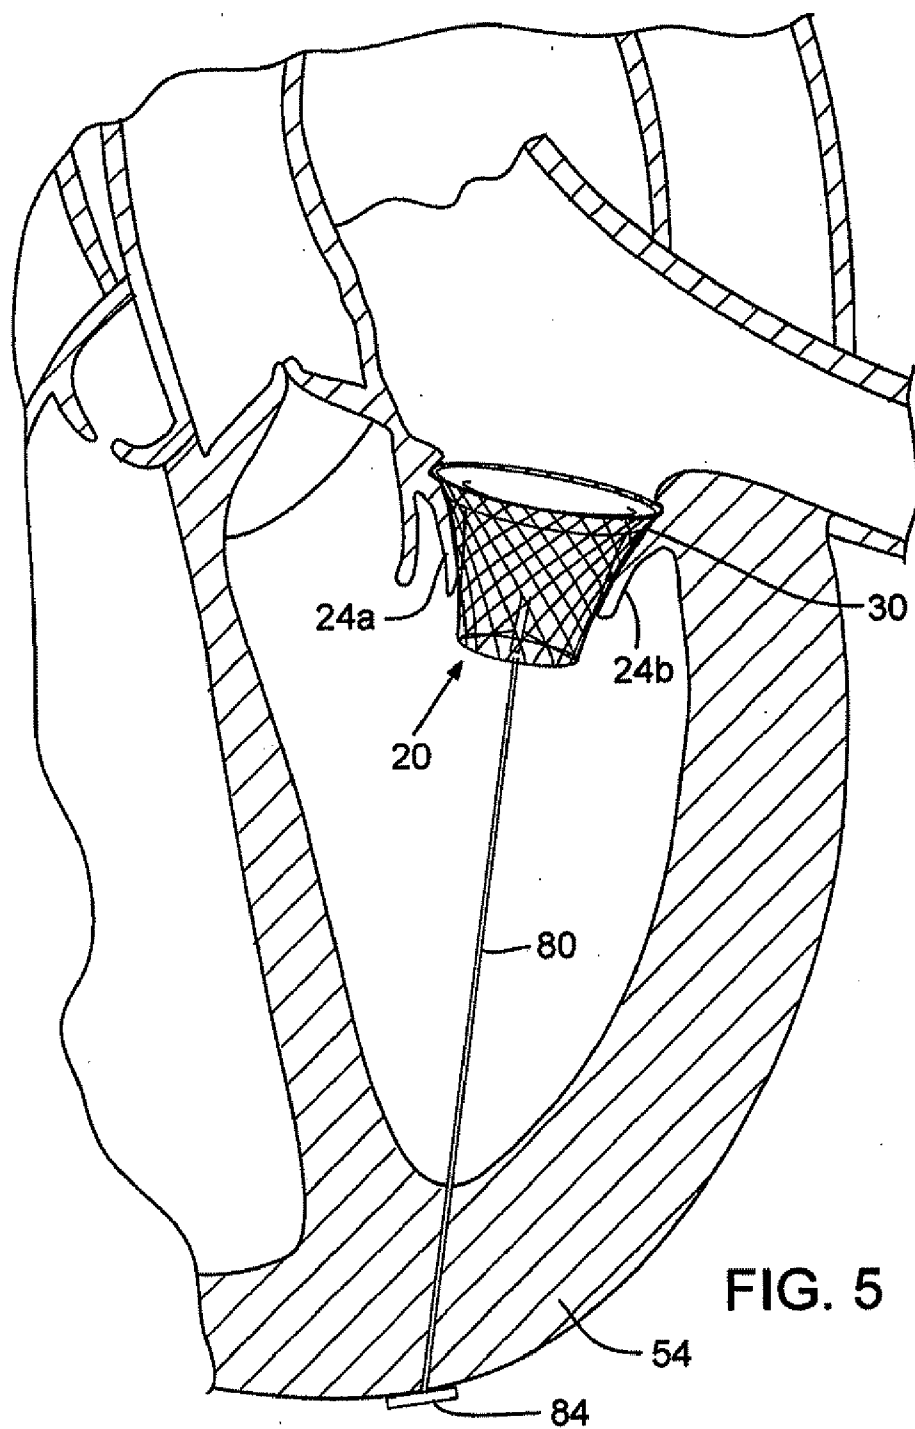


FIG. 5

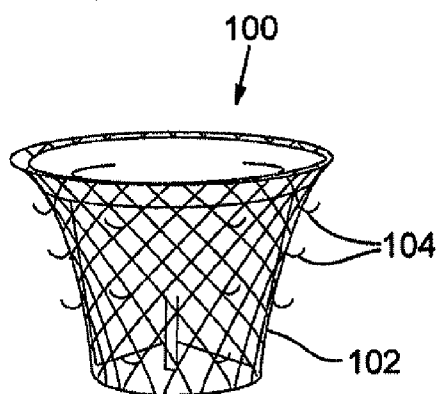


FIG. 6

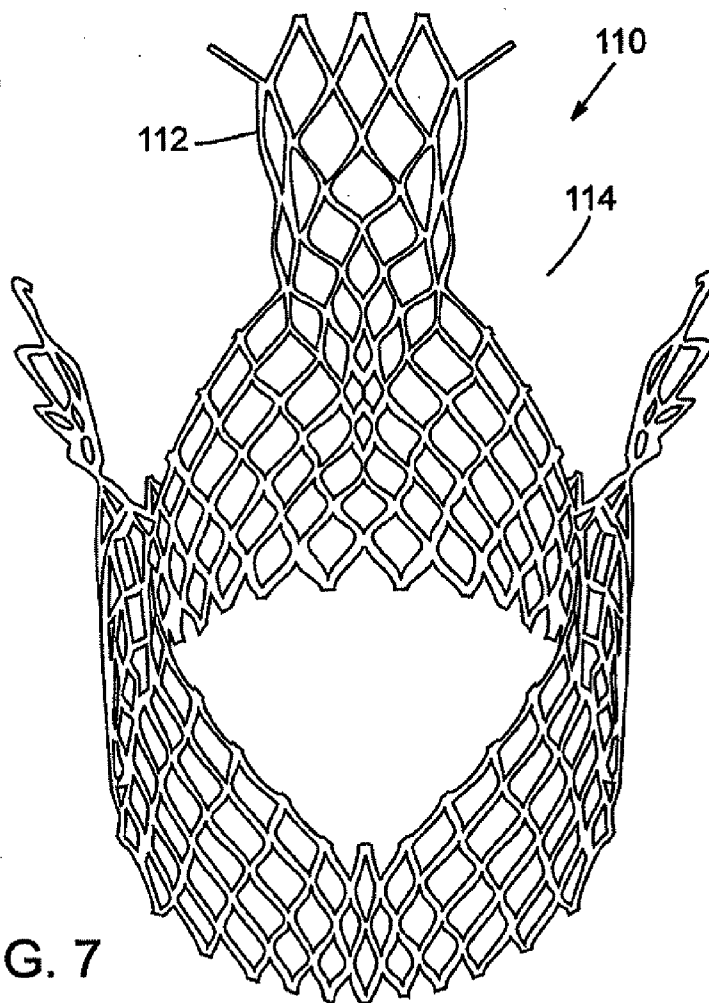
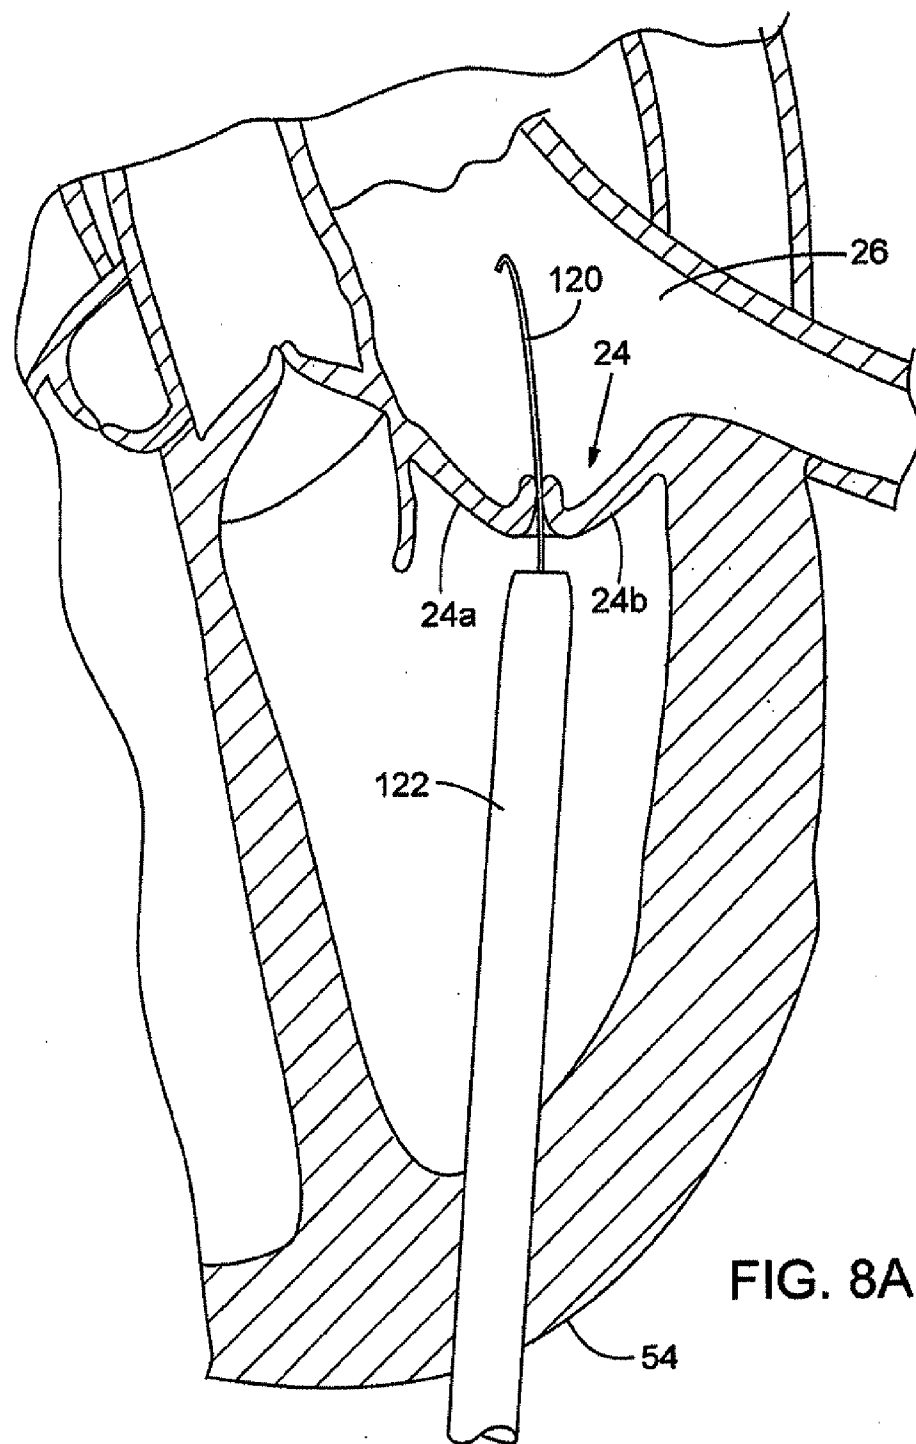
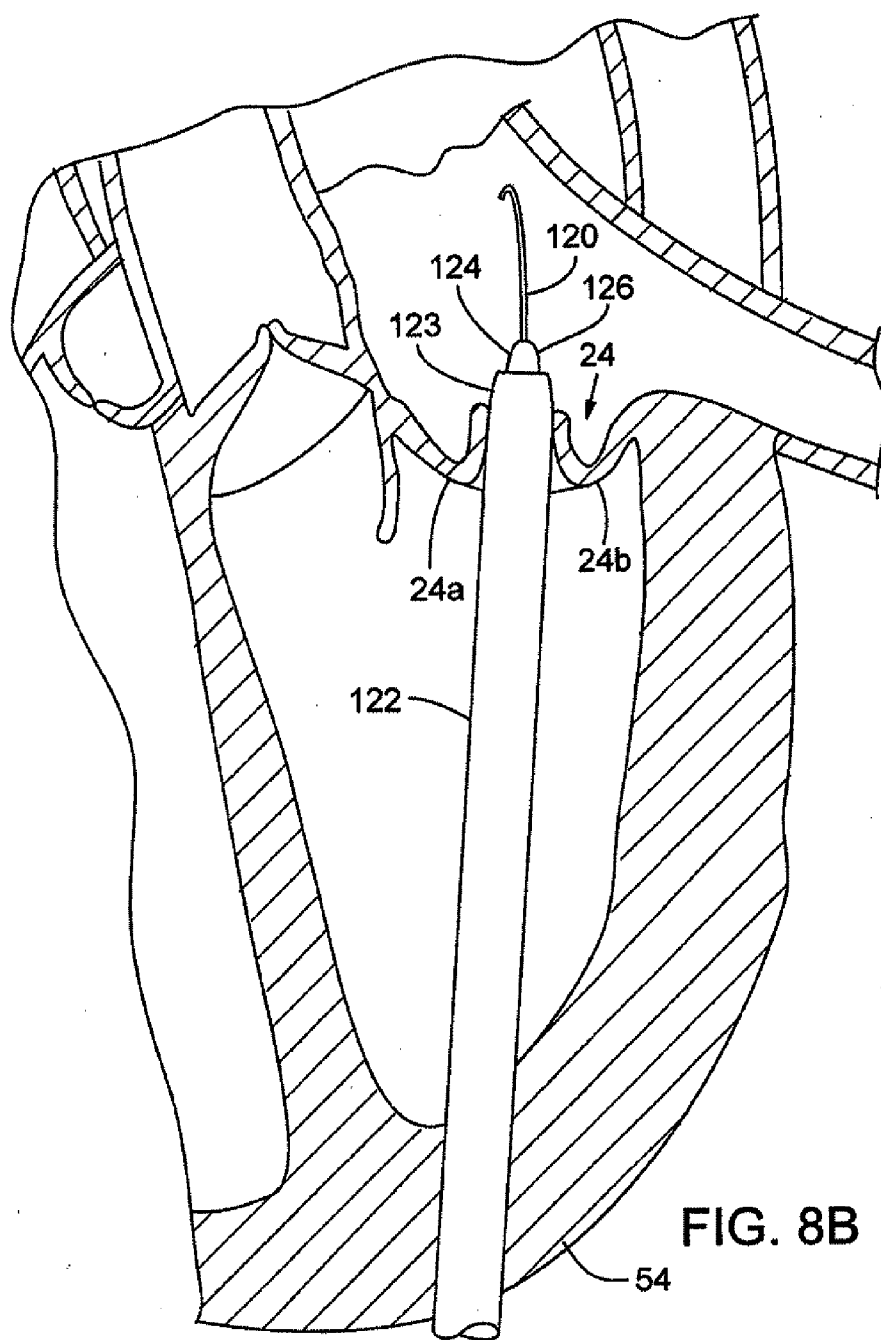
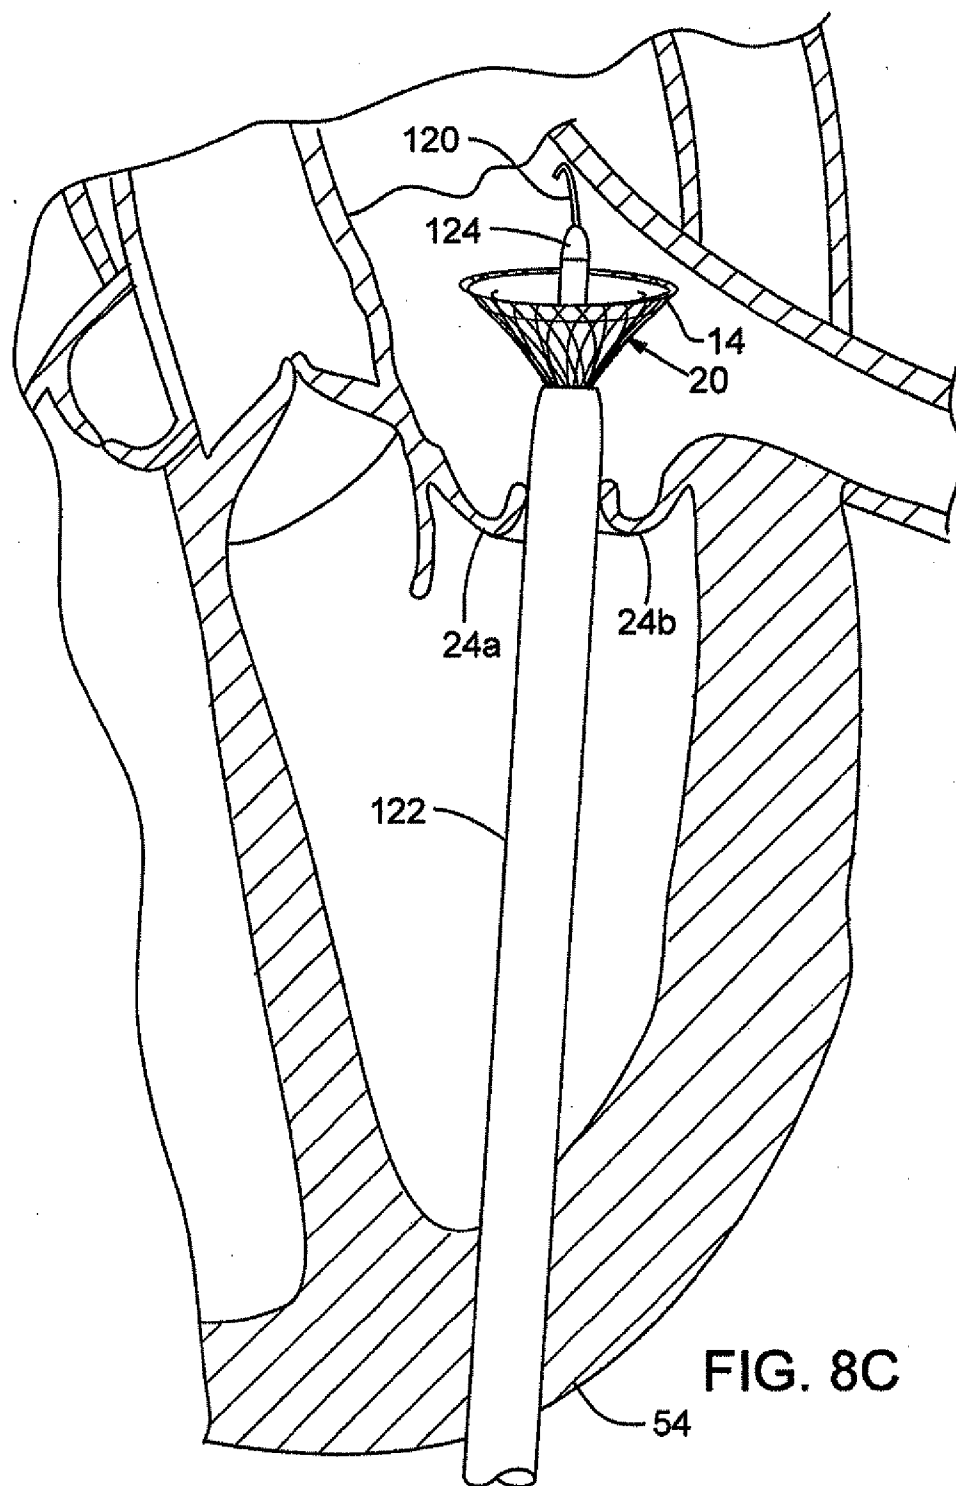
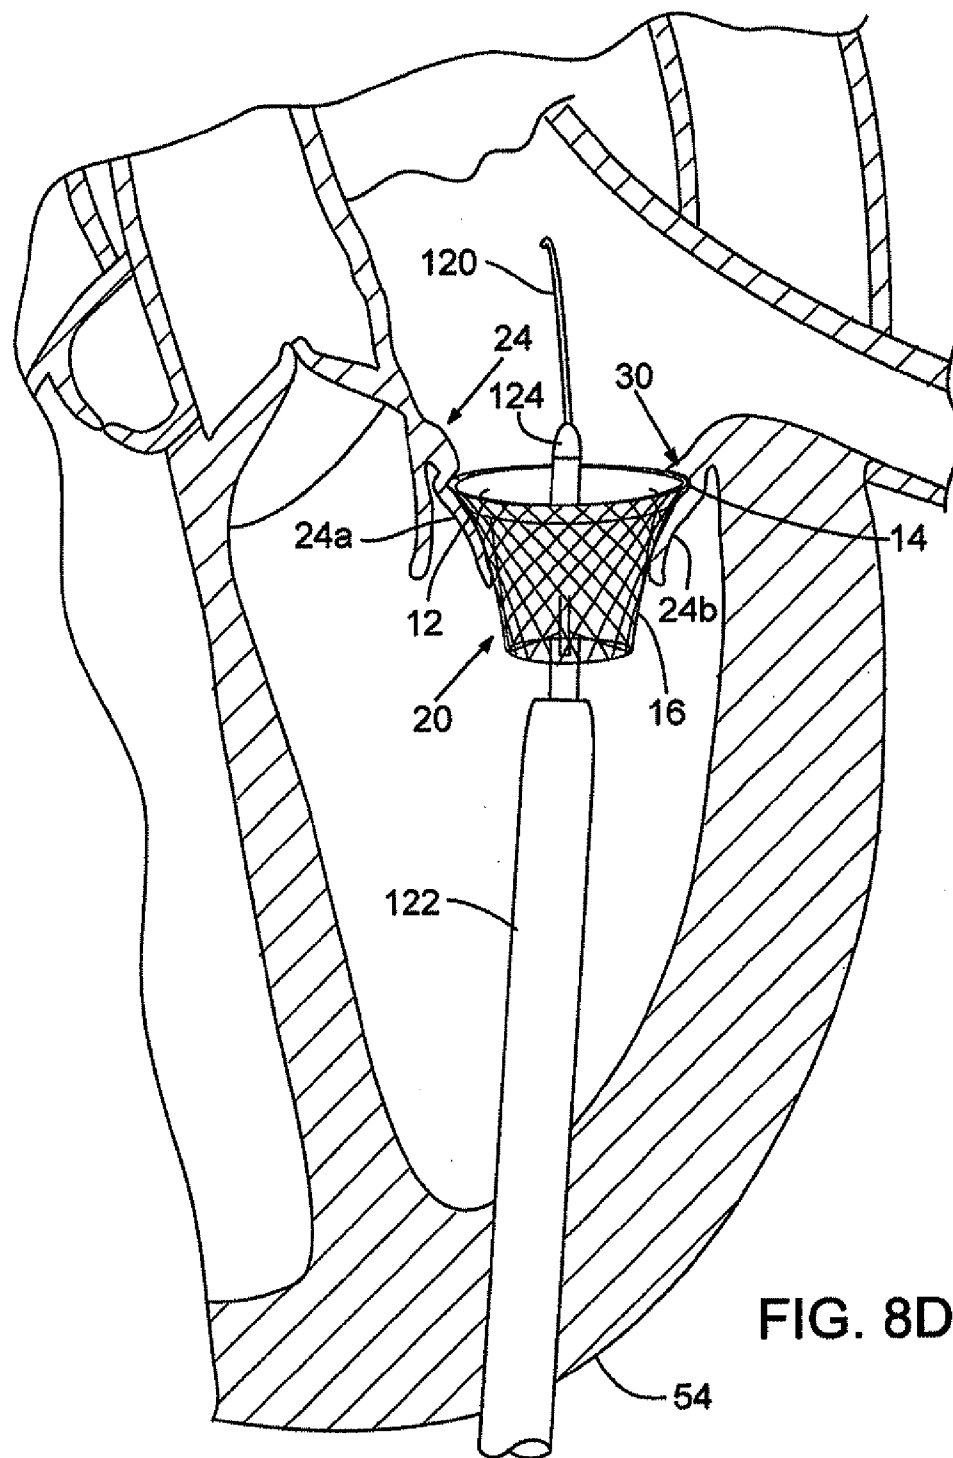



FIG. 7










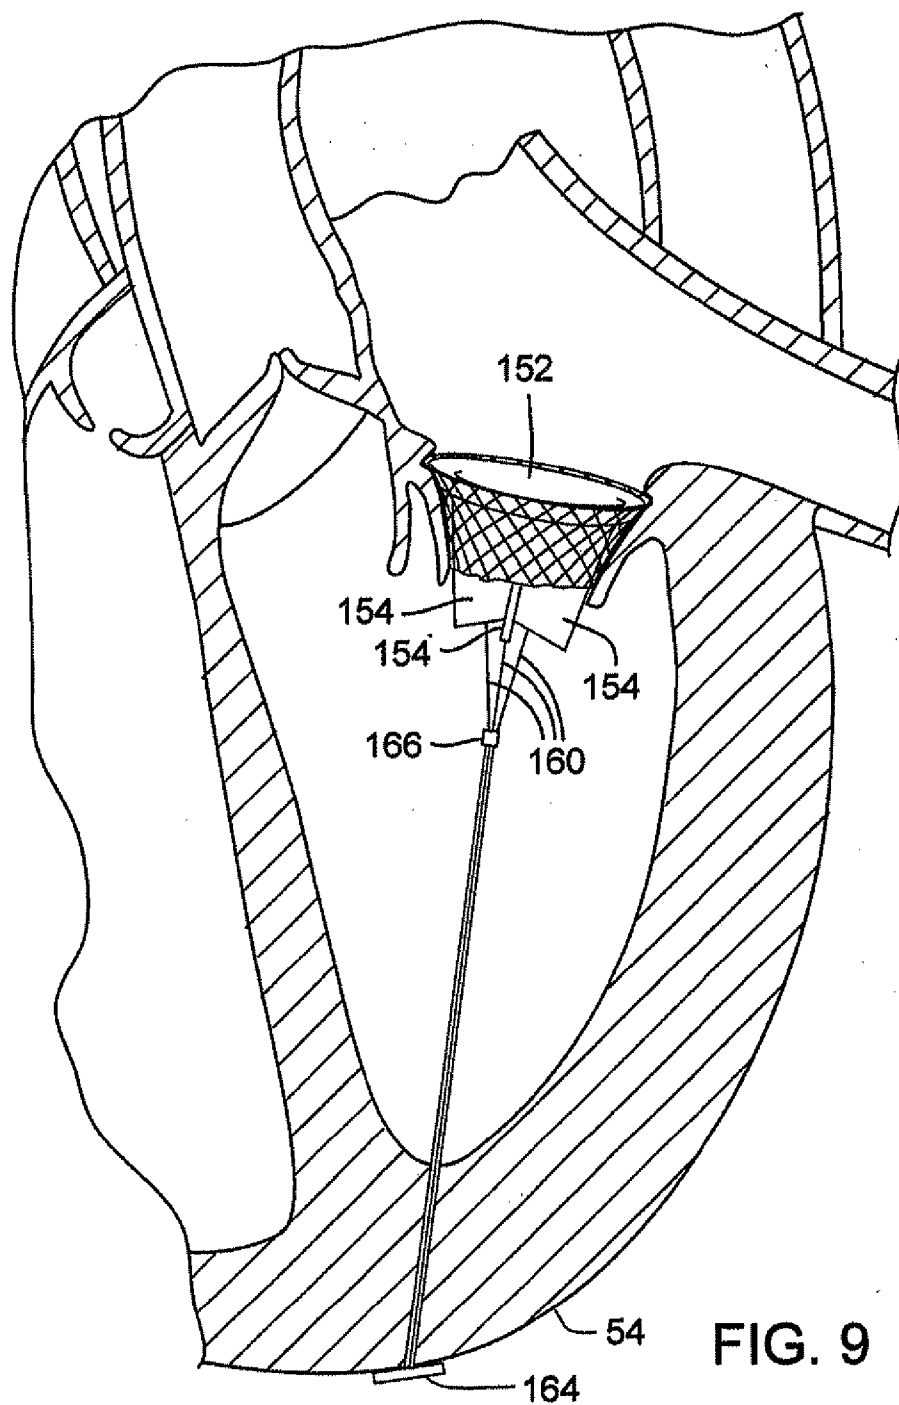

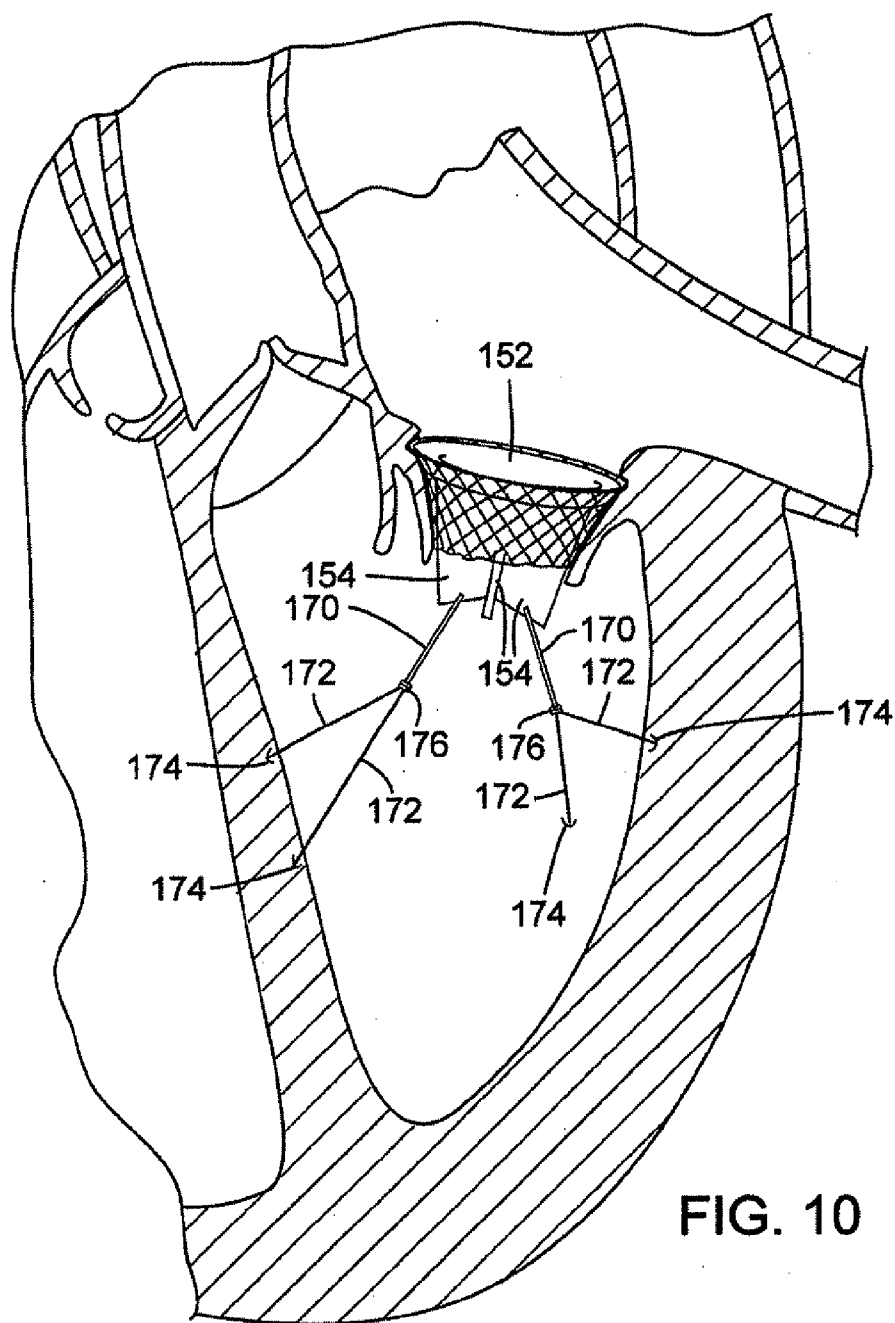

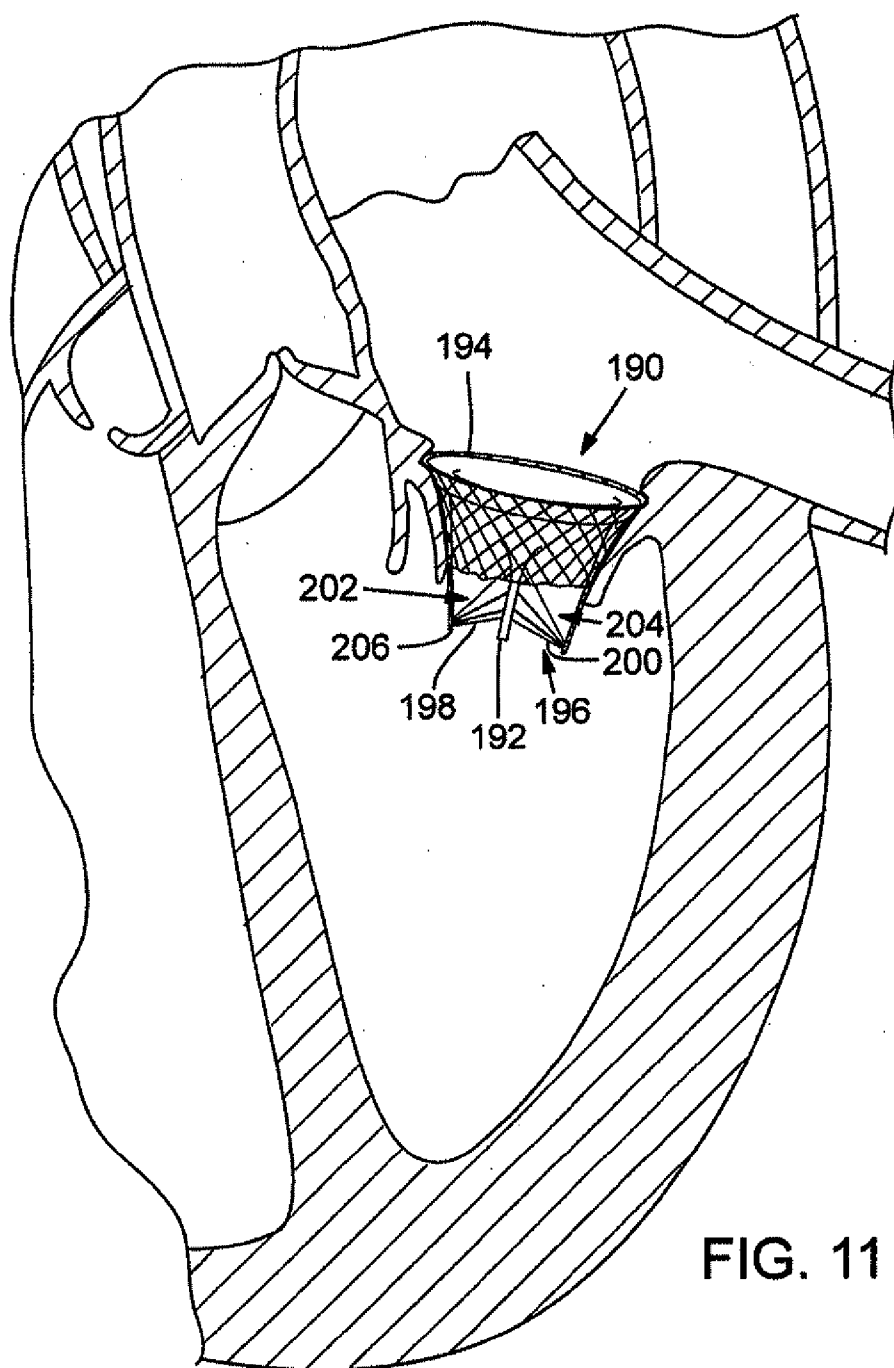


FIG. 11

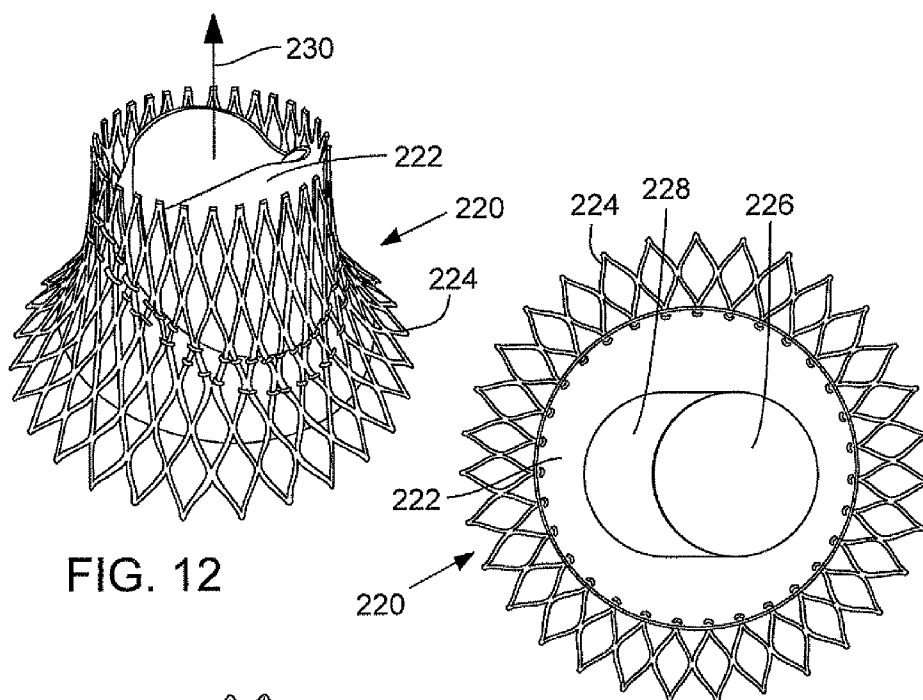


FIG. 12

FIG. 13

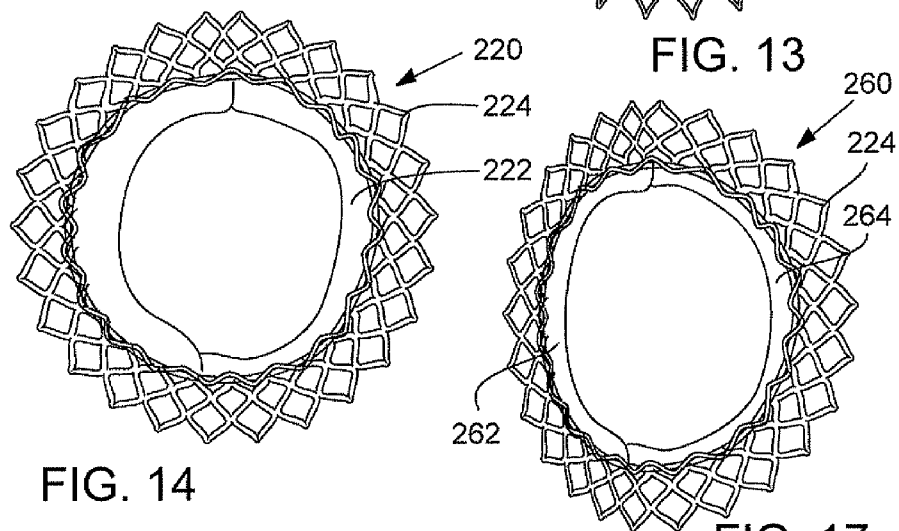


FIG. 14

FIG. 17

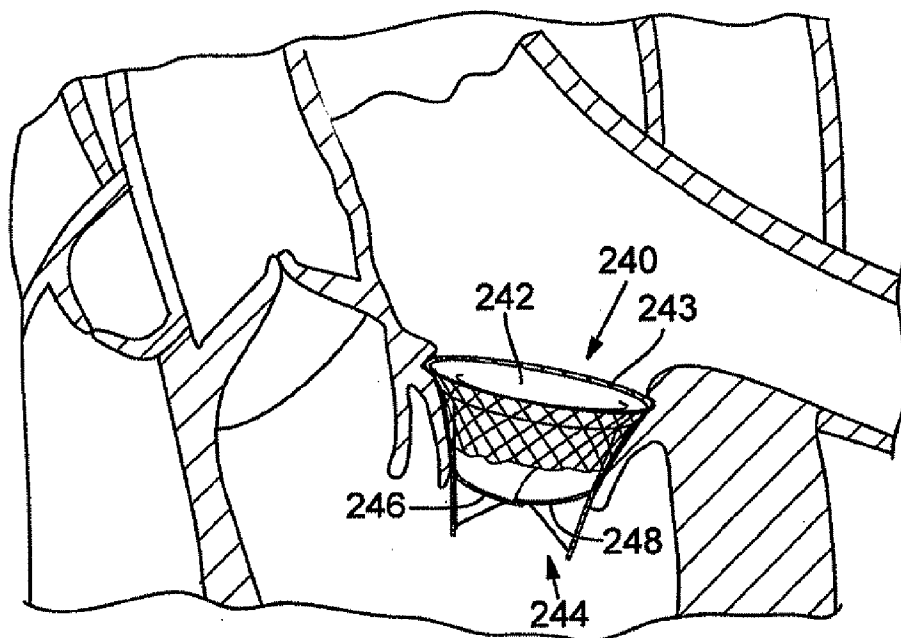


FIG. 15

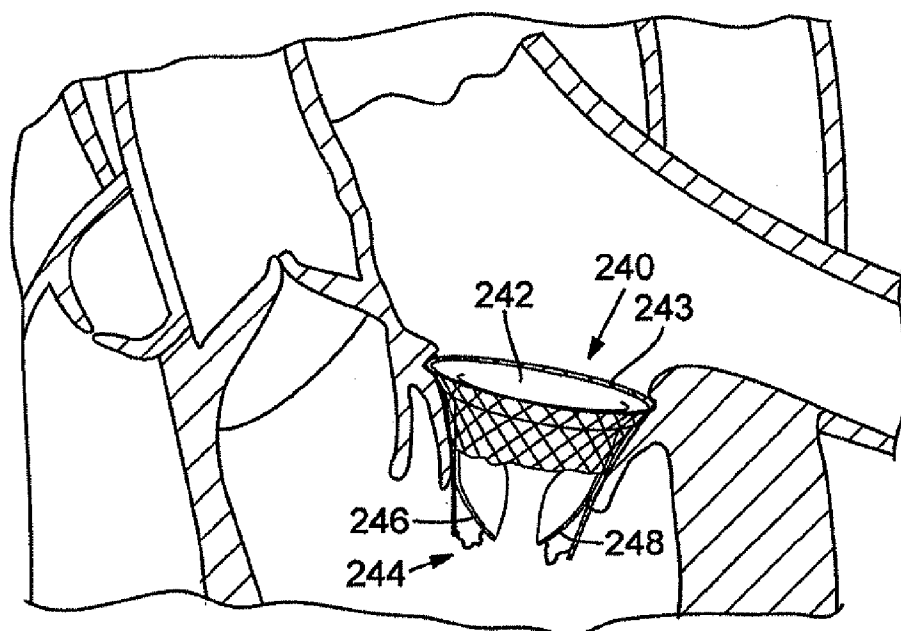


FIG. 16

DEVICE AND METHOD FOR REPLACING MITRAL VALVE

RELATED APPLICATIONS

[0001] This application is a divisional of U.S. patent application Ser. No. 12/113,418, filed May 1, 2008, the disclosure of which is incorporated by reference.

FIELD

[0002] The present disclosure concerns a prosthetic mitral heart valve and a method for implanting such a heart valve.

BACKGROUND

[0003] Prosthetic cardiac valves have been used for many years to treat cardiac valvular disorders. The native heart valves (such as the aortic, pulmonary and mitral valves) serve critical functions in assuring the forward flow of an adequate supply of blood through the cardiovascular system. These heart valves can be rendered less effective by congenital, inflammatory or infectious conditions. Such damage to the valves can result in serious cardiovascular compromise or death. For many years the definitive treatment for such disorders was the surgical repair or replacement of the valve during open heart surgery, but such surgeries are prone to many complications. More recently a transvascular technique has been developed for introducing and implanting a prosthetic heart valve using a flexible catheter in a manner that is less invasive than open heart surgery.

[0004] In this technique, a prosthetic valve is mounted in a crimped state on the end portion of a flexible catheter and advanced through a blood vessel of the patient until the valve reaches the implantation site. The valve at the catheter tip is then expanded to its functional size at the site of the defective native valve such as by inflating a balloon on which the valve is mounted.

[0005] Another known technique for implanting a prosthetic aortic valve is a transapical approach where a small incision is made in the chest wall of a patient and the catheter is advanced through the apex (i.e., bottom tip) of the heart. Transapical techniques are disclosed in U.S. Patent Application Publication No. 2007/0112422, which is hereby incorporated by reference. Like the transvascular approach, the transapical approach includes a balloon catheter having a steering mechanism for delivering a balloon-expandable prosthetic heart valve through an introducer to the aortic annulus. The balloon catheter includes a deflecting segment just proximal to the distal balloon to facilitate positioning of the prosthetic heart valve in the proper orientation within the aortic annulus.

[0006] The above techniques and others have provided numerous options for high-risk patients with aortic valve stenosis to avoid the consequences of open heart surgery and cardiopulmonary bypass. While procedures for the aortic valve are well-developed, such procedures are not necessarily applicable to the mitral valve.

[0007] Mitral valve repair has increased in popularity due to its high success rates, and clinical improvements noted after repair. However, a significant percentage (i.e., about 33%) of patients still receive open-heart surgical mitral valve replacements due to calcium, stenosis, or anatomical limitations. There are a number of technologies aimed at making mitral repair a less invasive procedure. These technologies range from iterations of the Alfieri stitch procedure to coro-

nary sinus-based modifications of mitral anatomy to subvalvular placements or ventricular remodeling devices, which would incidentally correct mitral regurgitation.

[0008] However, for mitral valve replacement, few less-invasive options are available. There are approximately 60,000 mitral valve replacements (MVR) each year and it is estimated that another 60,000 patients should receive MVR, but are denied the surgical procedure due to risks associated with the patient's age or other factors. One potential option for a less invasive mitral valve replacement is disclosed in U.S. Patent Application 2007/0016286 to Herrmann. However, the stent disclosed in that application has a claw structure for attaching the prosthetic valve to the heart. Such a claw structure could have stability issues and limit consistent placement of a transcatheter mitral replacement valve.

[0009] Accordingly, further options are needed for less-invasive mitral valve replacement.

SUMMARY

[0010] A prosthetic mitral valve assembly and method of inserting the same is disclosed.

[0011] In certain disclosed embodiments, the prosthetic mitral valve assembly has a flared upper end and a tapered portion to fit the contours of the native mitral valve. The prosthetic mitral valve assembly can include a stent or outer support frame with a valve mounted therein. The assembly is adapted to expand radially outwardly and into contact with the native tissue to create a pressure fit. With the mitral valve assembly properly positioned, it will replace the function of the native valve.

[0012] In other embodiments, the mitral valve assembly can be inserted above or below an annulus of the native mitral valve. When positioned below the annulus, the mitral valve assembly is sized to press into the native tissue such that the annulus itself can restrict the assembly from moving in an upward direction towards the left atrium. The mitral valve assembly is also positioned so that the native leaflets of the mitral valve are held in the open position.

[0013] In still other embodiments, when positioned above the annulus, prongs or other attachment mechanisms on an outer surface of the stent may be used to resist upward movement of the mitral valve assembly. Alternatively (or in addition), a tether or other anchoring member can be attached to the stent at one end and secured to a portion of the heart at another end in order to prevent movement of the mitral valve assembly after implantation. A tether may also be used to decrease the stress on the leaflets of the replacement valve and/or to re-shape the left ventricle.

[0014] In still other embodiments, the prosthetic mitral valve assembly can be inserted using a transapical procedure wherein an incision is made in the chest of a patient and in the apex of the heart. The mitral valve assembly is mounted in a compressed state on the distal end of a delivery catheter, which is inserted through the apex and into the heart. Once inside the heart, the valve assembly can be expanded to its functional size and positioned at the desired location within the native valve. In certain embodiments, the valve assembly can be self-expanding so that it can expand to its functional size inside the heart when advanced from the distal end of a delivery sheath. In other embodiments, the valve assembly can be mounted in a compressed state on a balloon of the delivery catheter and is expandable by inflation of the balloon.

[0015] These features and others of the described embodiments will be more readily apparent from the following detailed description, which proceeds with reference to the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] FIG. 1 is a perspective view of a stent used in certain embodiments of a mitral valve assembly.

[0017] FIGS. 2A and 2B are a perspective views an embodiment of a mitral valve assembly using the stent of FIG. 1, as viewed from the top and bottom, respectively, of the assembly.

[0018] FIG. 3 is a cross-sectional view of a heart with the mitral valve assembly of FIG. 2 implanted within the native mitral valve.

[0019] FIG. 4 is an enlarged cross-sectional view of a heart with an embodiment of the mitral valve assembly implanted below an annulus of the native mitral valve.

[0020] FIG. 5 is an enlarged cross-sectional view of a heart with an embodiment of the mitral valve assembly implanted within the native mitral valve wherein a tether is attached to the stent for preventing migration of the mitral valve assembly.

[0021] FIG. 6 is a perspective view of a mitral valve assembly having external anchoring members to assist in securing the mitral valve assembly to the surrounding tissue.

[0022] FIG. 7 is a perspective view of an embodiment of a stent having a scalloped end portion.

[0023] FIGS. 8A-8D are cross-sectional views showing an embodiment of the mitral valve assembly inserted using a transapical procedure.

[0024] FIG. 9 is a perspective view of an embodiment of a prosthetic valve assembly having tensioning members coupled to prosthetic leaflets of the valve to simulate chordae tendinae.

[0025] FIG. 10 is a perspective view of a prosthetic valve assembly having tensioning members, according to another embodiment.

[0026] FIG. 11 is a perspective view of a prosthetic valve assembly having tensioning members, according to another embodiment.

[0027] FIG. 12 is a perspective view of a prosthetic valve assembly having a bicuspid valve, according to another embodiment.

[0028] FIG. 13 is a top view of the prosthetic valve assembly of FIG. 12 with the bicuspid valve in a closed or at-rest position.

[0029] FIG. 14 is a top view of the prosthetic valve assembly of FIG. 12 with the bicuspid valve in an open position.

[0030] FIG. 15 is a perspective view of a prosthetic valve assembly having tensioning members coupled to a bicuspid valve in a closed position, according to another embodiment.

[0031] FIG. 16 is a perspective view of the prosthetic valve assembly of FIG. 15 with the bicuspid valve in an open position.

[0032] FIG. 17 is a cross-sectional view of a prosthetic valve assembly having a non-uniform cross-sectional shape.

DETAILED DESCRIPTION

[0033] As used herein, the singular forms “a,” “an,” and “the” refer to one or more than one, unless the context clearly dictates otherwise.

[0034] As used herein, the term “includes” means “comprises.” For example, a device that includes or comprises A and B contains A and B but can optionally contain C or other components other than A and B. A device that includes or comprises A or B may contain A or B or A and B, and optionally one or more other components such as C.

[0035] FIG. 1 is a perspective view of a stent 10 configured for placement in a native mitral valve. The stent in this embodiment includes an upper portion 12 having an enlarged or flared end 14 that tapers to a lower portion 16 having a reduced diameter. The stent generally has a bell shape or a truncated conical shape, but other shapes can be used. The stent 10 can have a continuous taper from the flared end 14 to the lower end 15. As described below, at least the upper portion desirably tapers in a direction from the upper end to the lower end 15 so as to generally conform to the contours of the native leaflets to assist in securing the stent within the native valve. In some embodiments, the portion of the stent extending below the native leaflets can have a generally cylindrical shape or could further taper. Additionally, the length of the stent 10 can vary. In some embodiments the stent can be between 15-50 mm in length. For example, specific testing has been performed on stents having lengths of 24 mm and 46 mm in length. A circumference of the stent 10 varies along a length thereof, but is generally sized for receiving a bicuspid or tricuspid valve. An example circumference of the stent at a point in the upper portion is 30 mm, but other sizes can be used depending on the desired valve. The stent can be a self-expanding stent formed from a shape memory material, such as, for example, Nitinol. In the illustrated embodiment, the stent is formed from multiple somewhat arcuate-shaped fibers extending along the length of the stent with approximately half of the fibers bent in a first direction and half of the fibers bent in a second direction to create a criss-cross pattern. As explained further below, the stent can be delivered in a radially-compressed state using an introducer, such that after reaching the treatment site, it is advanced out of the distal end of the introducer and expands to its functional size in a relaxed state in contact with the surrounding tissue. A specific example of such a technique is shown and described below in relation to FIGS. 8A-8D.

[0036] In other embodiments, the stent 10 can be a balloon-expandable stent. In such a case, the stent can be formed from stainless steel or any other suitable materials. The balloon-expandable stent can be configured to be crimped to a reduced diameter and placed over a deflated balloon on the distal end portion of an elongate balloon catheter, as is well-understood in the art.

[0037] The flared end 14 of the stent 10 helps to secure the stent above or below the annulus of the native mitral valve (depending on the procedure used), while the tapered portion is shaped for being held in place by the native leaflets of the mitral valve.

[0038] FIGS. 2A and 2B are perspective views of the stent 10 with a valve 18 inserted therein to form a mitral valve assembly 20. The valve 18 can have a leafed-valve configuration, such as a bicuspid valve configuration or the tricuspid valve configuration shown in the illustrated embodiment. As shown in FIG. 2B, the valve 18 can be formed from three pieces of flexible, pliant material connected to each other at seams 60 (also referred to as commissure tabs) to form collapsible leaflets 62 and a base, or upper end, portion 64. The valve 18 can be connected to the stent 10 at the seams 60 using, for example, sutures or other suitable connection tech-

niques well-known in the art. Alternatively, the valve **18** can be a mechanical type valve, rather than a leafed type valve.

[0039] The valve **18** can be made from biological matter, such as natural tissue, pericardial tissue (e.g., bovine, porcine or equine pericardium), a harvested natural valve, or other biological tissue. Alternatively, the valve can be made from biocompatible synthetic materials (e.g., biocompatible polymers), which are well known in the art. The valve can be shaped to fit the contours of the stent so as to have a flared upper end portion having an upper circumference larger than a lower circumference at the lower end of the valve. Blood flow through the valve proceeds in a direction from the upper portion **12** to the lower portion **16**, as indicated by arrow **22** (FIG. 2A).

[0040] FIG. 3 shows a cross-sectional view of a heart with the prosthetic mitral-valve assembly inserted into the native mitral valve. For purposes of background, the four-chambered heart is explained further. On the left side of the heart, the native mitral valve **24** is located between the left atrium **26** and left ventricle **28**. The mitral valve generally comprises two leaflets, an anterior leaflet **24a** and a posterior leaflet **24b**. The mitral valve leaflets are attached to a mitral valve annulus **30**, which is defined as the portion of tissue surrounding the mitral valve orifice. The left atrium **26** receives oxygenated blood from the pulmonary veins. The oxygenated blood that is collected in the left atrium **26** enters the left ventricle **28** through the mitral valve **24**.

[0041] Contraction of the left ventricle **28** forces blood through the left ventricular outflow tract and into the aorta **32**. The aortic valve **34** is located between the left ventricle **28** and the aorta **32** for ensuring that blood flows in only one direction (i.e., from the left ventricle to the aorta). As used herein, the left ventricular outflow tract (LVOT) is intended to generally include the portion of the heart through which blood is channeled from the left ventricle to the aorta.

[0042] On the right side of the heart, the tricuspid valve **40** is located between the right atrium **42** and the right ventricle **44**. The right atrium **42** receives blood from the superior vena cava **46** and the inferior vena cava **48**. The superior vena cava **46** returns de-oxygenated blood from the upper part of the body and the inferior vena cava **48** returns de-oxygenated blood from the lower part of the body. The right atrium **42** also receives blood from the heart muscle itself via the coronary sinus. The blood in the right atrium **42** enters into the right ventricle **44** through the tricuspid valve **40**. Contraction of the right ventricle forces blood through the right ventricle outflow tract and into the pulmonary arteries. The pulmonic valve **50** is located between the right ventricle **44** and the pulmonary trunk for ensuring that blood flows in only one direction from the right ventricle to the pulmonary trunk.

[0043] The left and right sides of the heart are separated by a wall generally referred to as the septum **52**. The portion of the septum that separates the two upper chambers (the right and left atria) of the heart is termed the atrial (or interatrial) septum while the portion of the septum that lies between the two lower chambers (the right and left ventricles) of the heart is called the ventricular (or interventricular) septum. A healthy heart has a generally conical shape that tapers from a base to an apex **54**.

[0044] As shown in FIG. 3, the mitral valve assembly **20** is positioned such that the flared end **14** of the upper portion **12** is adjacent the annulus **30** of the native mitral valve **24**, while the leaflets of the native valve bear against and hold the tapered upper end portion **12** of the mitral valve assembly.

The prosthetic mitral valve assembly of FIG. 3 is preferably positioned with the flared end **14** above or just below an annulus **30** of the native mitral valve. The valve assembly is configured to form a “pressure fit” with the surrounding native valve tissue; that is, the outward radial pressure of the stent bears against the surrounding tissue to assist in retaining the valve assembly in place.

[0045] FIG. 4 is enlarged view of the mitral valve assembly **20** positioned below the annulus **30** of the native mitral valve **24**. In particular, the flared end **14** of the stent is tucked under the annulus **30** of the native mitral valve (under the insertion point of the mitral leaflets to the left atrium), but on top of the mitral valve leaflets **24a**, **24b**. When deployed in this position, the mitral valve assembly exerts sufficient radial pressure outwardly to press into the native tissue, as the shape-memory material exerts an outward radial force to return the assembly to its expanded shape. As a result of the positioning of the flared end **14**, the annulus **30** protrudes slightly inwardly past the flared end of the stent and acts as an annular mechanical stop preventing upward movement of the mitral valve assembly **20**. The amount of outward radial pressure exerted by the mitral valve assembly **20** depends partly on the size of the stent and the type of shape-memory material used. The stent size can depend on the particular patient and the desired amount of pressure needed to hold the prosthetic mitral valve in place. The tapered upper portion **12** of the mitral valve assembly **20** desirably is shaped to fit the contours of the native mitral valve leaflets **24a**, **24b**, which bear against the outer surface of the stent and prevent downward motion of the assembly. Thus, due to the unique shape of the mitral valve assembly **20**, it can be held in place solely by the pressure exerted by the stent radially outwardly against the surrounding tissue without the use of hooks, prongs, clamps or other grasping device.

[0046] When properly positioned, the valve assembly avoids or at least minimizes paravalvular leakage. In tests performed on a porcine heart, approximately two pounds of force or greater were applied to stents in the left atrial direction with little or no dislodgement, movement or disorientation.

[0047] FIG. 5 shows an alternative positioning of the mitral valve assembly. In this position, the mitral valve assembly **20** can be secured above the native mitral valve annulus **30**. The mitral valve leaflets **24a**, **24b** still prevent downward movement of the mitral valve assembly. However, to assist in preventing upward movement, the mitral valve assembly **20** can be anchored using a tether **80** coupled between a lower portion of the mitral valve assembly (such as by being tied to the stent) and a portion of the heart (e.g., an opposing wall). In the particular embodiment shown, the tether **80** extends through the apex **54** of the heart and is secured in place by an enlarged head portion **84** connected to the lower end of the tether outside of the apex. The tether and/or head portion can be formed of a bioresorbable material so that it eventually dissolves after the stent has grown into the wall of the native mitral valve.

[0048] FIG. 6 shows another embodiment of a mitral valve assembly **100** that may be used with supra-annular positioning. In particular, an outer surface of a stent **102** includes anchoring members, such as, for example, prongs **104** in the form of upwardly bent hooks, that can penetrate the surrounding tissue to prevent upward migration of the assembly **100**.

when in place. The anchoring members may be made from the same material as the stent, but alternative materials may also be used.

[0049] FIG. 7 shows another embodiment of a stent 110 that can be used. In this embodiment, an upper portion 112 of the stent is scalloped (i.e., the upper edge has one or more indented or cut-out portions 114). In some patients, the pressure exerted by the upper rim of the stent on the anterior mitral leaflet can displace the mitral curtain and anterior leaflet toward the left ventricular outflow track. The stent can be deployed such that the anterior leaflet is generally positioned within a cutout (scalloped) portion of the stent. In this manner, the scalloped stent 110 reduces the pressure on the leaflet to ensure there is no alteration of blood flow in the left ventricle.

[0050] FIGS. 8A-8D depict an embodiment of a transapical procedure for inserting the prosthetic mitral valve assembly into the native mitral valve. The replacement procedure is typically accomplished by implanting the prosthetic mitral valve assembly directly over the native leaflets, which are typically calcified. In this manner, the native leaflets 24a, 24b can assist in securing the mitral valve assembly in place.

[0051] First, an incision is made in the chest of a patient and in the apex 54 of the patient's heart. A guide wire 120 is inserted through the apex 54 and into the left ventricle. The guide wire 120 is then directed up through the mitral valve 24 and into the left atrium 26. An introducer 122 is advanced over the guide wire into the left atrium (see FIGS. 8A and 8B). A delivery catheter 124 is inserted through the introducer (see FIG. 8B). A prosthetic valve assembly 20 is retained in a crimped state on the distal end portion of the delivery catheter as the valve assembly and delivery catheter are advanced through the introducer. In one variation, the introducer 122 is formed with a tapered distal end portion 123 to assist in navigating through the chordae tendinae. The delivery catheter 124 likewise can have a tapered distal end portion 126.

[0052] In FIG. 8C, the introducer 122 is retracted relative to the mitral valve assembly 20 for deploying the mitral valve assembly from the distal end of the introducer. To pull the valve assembly 20 into position at the intended implantation site, the valve assembly desirably is partially advanced out of the introducer to expose the flared upper end portion 12, while the remainder of the valve assembly remains compressed within the introducer (as shown in FIG. 8C). As shown, the flared end portion expands when advanced from the distal end of the introducer. The delivery catheter 124 and the introducer 122 can then be retracted together to pull the flared end into the desired position (e.g., just below the annulus of the native valve). Thereafter, the introducer can be further retracted relative to the delivery catheter to advance the remaining portion of the valve assembly 20 from the introducer, thereby allowing the entire assembly to expand to its functional size, as shown in FIG. 8D. The introducer and catheter can then be withdrawn from the patient.

[0053] Alternatively, the mitral valve assembly can be fully expanded directly in place at the implantation site by first aligning the valve assembly at the implantation site and then retracting the introducer relative to the delivery catheter to allow the entire valve assembly to expand to its functional size. In this case, there is no need to pull the mitral valve assembly down into the implantation site. Additional details of the transapical approach are disclosed in U.S. Patent Application Publication No. 2007/0112422 (mentioned above).

[0054] In another embodiment, the valve assembly 20 can be mounted on an expandable balloon of a delivery catheter and expanded to its functional size by inflation of the balloon. When using a balloon catheter, the valve assembly can be advanced from the introducer to initially position the valve assembly in the left atrium 26. The balloon can be inflated to fully expand the valve assembly. The delivery catheter can then be retracted to pull the expanded valve assembly into the desired implantation site (e.g., just below the annulus of the native valve). In another embodiment, the balloon initially can be partially inflated to partially expand the valve assembly in the left atrium. The delivery catheter can then be retracted to pull the partially expanded valve into the implantation site, after which the valve assembly can be fully expanded to its functional size.

[0055] Mitral regurgitation can occur over time due to the lack of coaptation of the leaflets in the prosthetic mitral valve assembly. The lack of coaptation in turn can lead to blood being regurgitated into the left atrium, causing pulmonary congestion and shortness of breath. To minimize regurgitation, the leaflets of the valve assembly can be connected to one or more tension members that function as prosthetic chordae tendinae.

[0056] FIG. 9, for example, shows an embodiment comprising a prosthetic mitral valve assembly 152 having leaflets 154. Each leaflet 154 can be connected to a respective tension member 160, the lower ends of which can be connected at a suitable location on the heart. For example, the lower end portions of tension members 160 can extend through the apex 54 and can be secured at a common location outside the heart. Tension members may be attached to or through the papillary muscles. The lower ends of tension members can be connected to an enlarged head portion, or anchor, 164, which secures the tension members to the apex. Tension members 160 can extend through a tensioning block 166. The tensioning block 166 can be configured to slide upwardly and downwardly relative to tension members 160 to adjust the tension in the tensioning members. For example, sliding the tensioning block 166 upwardly is effective to draw the upper portions of the tension members closer together, thereby increasing the tension in the tension members. The tensioning block 166 desirably is configured to be retained in place along the length of the tension members, such as by crimping the tensioning block against the tension members, once the desired tension is achieved. The tension members can be made of any suitable biocompatible material, such as traditional suture material, GORE-TEX®, or an elastomeric material, such as polyurethane. The tension members 160 further assist in securing the valve assembly in place by resisting upward movement of the valve assembly and prevent the leaflets 154 from everting so as to minimize or prevent regurgitation through the valve assembly. As such, the tethering de-stresses the moveable leaflets, particularly during ventricular systole (i.e., when the mitral valve is closed). Alternatively or in addition, the stent 10 can be connected to one or more tension members 160 for stabilizing the mitral valve assembly during the cyclic loading caused by the beating heart.

[0057] FIG. 10 shows another embodiment of a mitral valve assembly 152 having prosthetic chordae tendinae. The prosthetic chordae tendinae comprise first and second tension members 170 connected to a respective leaflet 154 of the valve assembly. As shown, the lower end portions 172 of each tension member 170 can be connected at spaced apart locations to the inner walls of the left ventricle, using, for

example, anchor members **174**. A slidable tensioning block **176** can be placed over each tension member **170** for adjusting the tension in the corresponding tension member. In certain embodiments, each tension member **170** can comprise a suture line that extends through a corresponding leaflet **154** and has its opposite ends secured to the ventricle walls using anchor members **174**.

[0058] In particular embodiments, the anchor member **174** can have a plurality of prongs that can grab, penetrate, and/or engage surrounding tissue to secure the device in place. The prongs of the anchor member **174** can be formed from a shape memory material to allow the anchor member to be inserted into the heart in a radially compressed state (e.g., via an introducer) and expanded when deployed inside the heart. The anchor member can be formed to have an expanded configuration that conforms to the contours of the particular surface area of the heart where the anchor member is to be deployed, such as described in co-pending Application No. 11/750,272, published as US 2007/0270943 A1, which is incorporated herein by reference. Further details of the structure and use of the anchor member are also disclosed in co-pending application Ser. No. 11/695,583 to Rowe, filed Apr. 2, 2007, which is incorporated herein by reference.

[0059] Alternative attachment locations in the heart are possible, such as attachment to the papillary muscle (not shown). In addition, various attachment mechanisms can be used to attach tension members to the heart, such as a barbed or screw-type anchor member. Moreover, any desired number of tension members can be attached to each leaflet (e.g., 1, 2, 3 . . . etc.). Further, it should be understood that tension members (e.g., tension members **160** or **170**) can be used on any of the embodiments disclosed herein.

[0060] As discussed above, FIGS. 9-10 show the use of tension members that can mimic the function of chordae. The tethers can have several functions including preventing the valve from migrating into the left atrium, de-stressing the leaflets by preventing eversion, and preserving ventricular function by maintaining the shape of the left ventricle. In particular, the left ventricle can lose its shape over time as the natural chordae become stretched or break. The artificial chordae can help to maintain the shape. Although FIGS. 9 and 10 show a tricuspid valve, a bicuspid valve can be used instead. Particular bicuspid valves are shown in FIGS. 12-16.

[0061] FIG. 11 shows another embodiment of a mitral valve assembly **190** including a valve **192** and a stent **194** (shown partially cut-away to expose a portion of the valve). Tension members, shown generally at **196**, can be connected between leaflets **198**, **200** of the valve **192** and the stent itself. Only two leaflets are shown, but additional tension members can be used for a third leaflet in a tricuspid valve. In the illustrated embodiment, the tension members **196** can include groups **202**, **204** of three tension members each. The three tension members **196** of group **202** can be attached, at one end, to leaflet **198** at spaced intervals and converge to attach at an opposite end to a bottom **206** of the stent **194**. Group **204** can be similarly connected between leaflet **200** and the bottom **206** of the stent **194**. The tension members **196** can be made of any suitable biocompatible material, such as traditional suture material, GORE-TEX®, or an elastomeric material, such as polyurethane. The tension members can prevent the leaflets **198**, **200** from everting so as to minimize or prevent regurgitation through the valve assembly. As such, the tension members de-stress the moveable portions of the leaflets when

the leaflets close during systole without the need to connect the tension members to the inner or outer wall of the heart.

[0062] Although groups of three tension members are illustrated, other connection schemes can be used. For example, each group can include any desired number of tension members (e.g., 1, 2, 3, . . . etc.). Additionally, the tension members can connect to any portion of the stent **194** and at spaced intervals, if desired. Likewise, the tension members can connect to the leaflets at a point of convergence, rather than at spaced intervals. Further, the tension members can be used on bicuspid or tricuspid valves. Still further, it should be understood that tension members extending between the stent and the leaflets can be used on any of the embodiments disclosed herein.

[0063] FIGS. 12-14 show another embodiment of a mitral valve assembly **220** including a bicuspid valve **222** mounted within a stent **224**. The bicuspid valve **222** can include two unequally-sized leaflets, **226**, **228**. FIG. 12 shows a perspective view of the mitral valve assembly **220** with the bicuspid valve **222** in an open position with blood flow shown by directional arrow **230**. FIG. 14 shows a top view of the mitral valve assembly **220** with the valve **222** in the open position. FIG. 13 shows a top view of the mitral valve assembly **220** with the bicuspid valve **222** in a closed position. The leaflet **226** is shown as a larger leaflet than leaflet **228** with the leaflets overlapping in a closed or at-rest position. The overlapping configuration can provide sufficient closure of the valve to prevent central or coaptation leakage and can enhance valve durability by eliminating or minimizing impacts on the leaflet touching or coaptation. The bicuspid valve **222** can be used with any of the stent configurations described herein.

[0064] FIGS. 15 and 16 show another embodiment of a mitral valve assembly **240** including a bicuspid valve **242** mounted within a stent **243**. Tension members, shown generally at **244**, can be connected between leaflets **246**, **248** of the valve and the stent itself. Leaflet **246** is shown as a larger leaflet that overlaps leaflet **248**. FIG. 15 shows the mitral valve assembly **240** in a closed position with the tension members **244** at full extension. FIG. 16 shows the bicuspid valve **242** in the open position with the tension members **244** in a relaxed or slack state. Although the tension members **244** are shown attached at the same relative vertical position or height on the stent **243**, the tension members **244** can be attached asymmetrically relative to each other. In other words, the tension members **244** can be attached at different heights along the length of the stent. Additionally, the tension members **244** can differ in length in order to achieve the asymmetrical coupling between the leaflets **246**, **248** and the stent **243**. The tensioning members **244** can be used on any of the mitral valve assembly embodiments described herein.

[0065] FIG. 17 shows a top view of a mitral valve assembly **260** having a non-uniform cross-sectional shape. The mitral valve assembly **260** can have a shape configured to conform to the natural opening of the native mitral valve. For example, the mitral valve assembly **260** can have a substantially "D" shape, with a substantially straight portion **262** and a substantially curved portion **264**. When implanted, the substantially straight portion **262** can extend along the anterior side of the native mitral valve and the substantially curved portion **264** of the stent can extend along the posterior side of the native mitral valve. Other shapes may also be used.

[0066] Having illustrated and described the principles of the illustrated embodiments, it will be apparent to those

skilled in the art that the embodiments can be modified in arrangement and detail without departing from such principles.

[0067] Although the transapical procedure shown in FIGS. 8A-8D illustrates positioning and deployment of mitral valve assembly 20, other embodiments of the mitral valve assembly disclosed herein can be implanted using the same procedure, such as the mitral valve assembly 100 of FIG. 6, or a mitral valve assembly using the stent of FIG. 7.

[0068] Further, although the mitral valve assembly 20 is shown generally circular in cross section, as noted above, it can have a D-shape, an oval shape or any other shape suitable for fitting the contours of the native mitral valve. Furthermore, although the mitral valve assembly is shown as having a flared upper end, other embodiments are contemplated, such as, for example, wherein the stent is flared at both ends or has a substantially cylindrical shape. Furthermore, the stent may be coated to reduce the likelihood of thrombi formation and/or to encourage tissue ingrowth using coatings known in the art. Still further, it is contemplated that the stent may be replaced with an alternative structure, such as an expandable tubular structure, which is suitable for anchoring the prosthetic valve member in the heart.

[0069] Still further, although a transapical procedure is described in detail in FIGS. 8A-8D, other procedures can be used in conjunction with the above-described embodiments. For example, U.S. Patent Publication 2004/0181238, to Zarbatany et al., entitled "Mitral Valve Repair System and Method for Use", which is hereby incorporated by reference, discloses a percutaneous delivery approach. A guidewire capable of traversing the circulatory system and entering the heart of the patient can be introduced into the patient through an endoluminal entry point, such as the femoral vein or the right jugular vein. The guidewire can then be directed into the right atrium where it traverses the right atrium and punctures the atrial septum using a tran-septal needle. The guidewire can then be advanced through the atrial septum, through the left atrium and through the mitral valve. Once the guidewire is properly positioned, a guide catheter can be attached to the guidewire and advanced proximate the native mitral valve. A delivery catheter for delivery of the prosthetic mitral valve can then be advanced through the guide catheter to deploy the prosthetic valve within the native mitral valve. Various delivery catheters can be used, such as those described in Zarbatany, as well as those described U.S. Patent Publication 2007/0088431, to Bourang et al., entitled "Heart Valve Delivery System With Valve Catheter" and U.S. Patent Publication U.S. 2007/0005131, to Taylor, entitled "Heart Valve Delivery System", both of which are hereby incorporated by reference.

[0070] In view of the many possible embodiments, it will be recognized that the illustrated embodiments include only examples of the invention and should not be taken as a limitation on the scope of the invention. Rather, the invention is defined by the following claims. We therefore claim as the invention all such embodiments that come within the scope of these claims.

What is claimed is:

1. A prosthetic mitral valve assembly, comprising:
a radially-expandable stent including a lower portion sized to held between leaflets of a native mitral valve and an upper portion having a flared end, the upper portion sized for deployment within the annulus of the mitral

valve with a pressure fit, the flared end configured to extend above the annulus, wherein the stent tapers from the upper portion to the lower portion, the stent having a substantially D-shape cross-section for conforming to the native mitral valve, the D-shape cross-section providing a substantially straight portion configured to extend along an anterior side of the native mitral valve and a substantially curved portion configured to extend along a posterior side of the native mitral valve; and
a valve portion formed of pericardial tissue and mounted within an interior portion of the stent, the valve portion having leaflets for occluding blood flow in one direction and replacing the function of the native mitral valve.

2. The prosthetic mitral valve assembly of claim 1, wherein the stent is made of nitinol.

3. The prosthetic mitral valve assembly of claim 1, wherein the valve portion comprises three leaflets.

4. The prosthetic mitral valve assembly of claim 1, wherein the valve portion is a bicuspid valve having only two leaflets.

5. The prosthetic mitral valve assembly of claim 4, wherein the two leaflets differ in size.

6. The prosthetic mitral valve assembly of claim 1, wherein the stent is formed with intercrossing bars.

7. The prosthetic mitral valve assembly of claim 1, further including tension members extending between the leaflets and the stent.

8. The prosthetic mitral valve assembly of claim 7, wherein the tension members are coupled at different heights, relative to one another, along a length of the stent.

9. The prosthetic mitral valve assembly of claim 1, wherein the stent has a truncated conical shape.

10. The prosthetic mitral valve assembly of claim 1, wherein the flared end is scalloped.

11. The prosthetic mitral valve assembly of claim 1, wherein the prosthetic mitral valve assembly is held in place without clamping onto tissue.

12. The prosthetic mitral valve assembly of claim 1, wherein the stent includes external prongs to assist in holding the prosthetic mitral valve assembly in place.

13. The prosthetic mitral valve assembly of claim 1, wherein the stent and the valve portion are collapsible to a reduced diameter for insertion into the heart on a delivery catheter for implantation.

14. The prosthetic mitral valve assembly of claim 1, further including a tether coupled to the stent on one end thereof, the tether being configured to couple the stent to a portion of the heart remote from the stent.

15. The prosthetic mitral valve assembly of claim 1, wherein the valve portion further includes tension members coupled to the prosthetic leaflets for preventing the prosthetic leaflets from everting and reducing stresses induced by ventricular contraction.

16. The prosthetic mitral valve assembly of claim 15, wherein the tension members are coupled to the prosthetic leaflets at a first end of the tension members and coupled at an opposite end to the stent or to a patient's heart.

17. The prosthetic mitral valve assembly of claim 15, wherein the tension members are coupled to the stent at a first end of the tension members and coupled at an opposite end to a portion of the patient's heart.

* * * * *