

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
25 June 2009 (25.06.2009)

PCT

(10) International Publication Number
WO 2009/079502 A1

(51) International Patent Classification:
A61F 2/44 (2006.01)

(21) International Application Number:

PCT/US2008/086977

(22) International Filing Date:

16 December 2008 (16.12.2008)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

11/960,623 19 December 2007 (19.12.2007) US

(71) Applicant (for all designated States except US): **DEPUY SPINE INC.** [US/US]; 325 Paramount Drive, Raynham, Massachusetts 02767 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **SOMMERICH, Robert E.** [US/US]; 5 Beach Street, Norton, Massachusetts 02766 (US). **PRESBREY, Glen A.** [US/US]; 574 Victory Highway, Pascoag, Rhode Island 02859 (US). **MEER,**

Martin [DE/DE]; Birkenweg 7/1, D72189 Vohringen (DE). **POHL, Gerhard** [DE/DE]; Gerhart-Hauptmann Str. 10, D78112 St. Georgen (DE).

(74) Agents: **JOHNSON, Philip S.** et al.; Johnson & Johnson, One Johnson & Johnson Plaza, New Brunswick, New Jersey 08933 (US).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,

[Continued on next page]

(54) Title: EXPANDABLE CORPECTOMY SPINAL FUSION CAGE

FIG. 1A

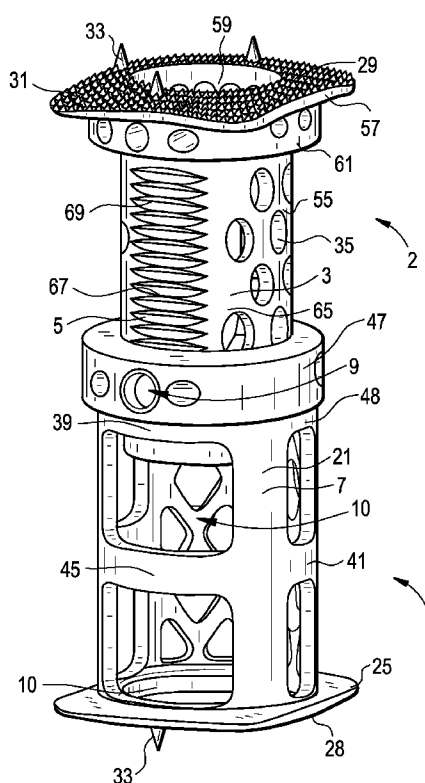

(57) Abstract: An intervertebral expandable spacer having a pair of co-axial annuluses locked together by an engagement member having i) a set screw and ii) a pressure plate having an outer face contacting the set screw and an inner face having teeth adapted to mate with the ratchet notches of the second member.

WO 2009/079502 A1



ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL,
NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG,
CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report*

Expandable Corpectomy Spinal Fusion Cage

5

BACKGROUND OF THE INVENTION

One conventional spinal implant used in corpectomy cases is an intervertebral spacer for insertion between two vertebrae, wherein the spacer has an adjustable axial height, an annular first member and a second member which is guided within the first member and displaceable in axial direction relative to the first member for adjustment of the overall height.

Conventional spacers of this type of are often expanded by a threaded connection between the outer surface of the inner member and the inner surface of the outer member. The opposite ends of the spacer are often provided with spikes for secure seating into the adjacent vertebra. However, the requirement of rotating the members around the longitudinal axis also rotates the spikes, thereby risking injury to the adjacent vertebrae.

US Patent Number 6,200,348 (Biedermann) discloses a spacer that is expandable without the need for rotation. The locking mechanism of the US Patent Number 6,200,348 includes a i) a pair of set screws, each set screw having a hemispherical distal end that seats in an outer annulus, and ii) a row of mating hemispherical recesses extending into an inner annulus.

SUMMARY OF THE INVENTION

The present inventors have appreciated that although the spacer design disclosed in US Patent Number 6,200,348 has advantageously eliminated the need to rotate the pair of sleeved cage components in order to expand its height, it nonetheless does not contain a graft window. A graft window is a large opening in the face of the cage – an opening much larger than the diamond shaped holes provided in US Patent Number 6,200,348- used to insert graft into the cage. Providing a graft window is helpful in that it provides the surgeon with an access port into the center space of the cage through which the surgeon may insert bone graft into the cage. When a graft

window is not provided, bone graft must be inserted into the cage prior to insertion of the cage into the spine (i.e., when the cage is in its unexpanded configuration). Thus, when the cage is later inserted into the spine and then expanded, the newly expanded portion of the cage contains no graft. Providing a graft window is helpful in that it
5 allows the surgeon to place the cage into the spine, expand the cage and then fill the expanded cage with bone graft. Accordingly, there is no unfilled space in the expanded inserted cage having a graft window.

Therefore, in accordance with the present invention, there is provided a spacer
10 for insertion between two vertebrae, the spacer having a variable axial height and comprising a first member and a second member guided within the first member to be slidable relative thereto in an axial direction thereof for adjusting an overall height, wherein the second member comprises an outer wall and ratchet notches provided at its outer wall facing the first member and extending in the axial direction,
15 wherein the first member comprises a wall having an engagement member, which cooperates with the ratchet notches for adjusting the overall height of the spacer, and wherein the first member has a graft window therein for inserting graft material therethrough.

20 However, when the present inventors set out to modify the cage of US Patent Number 6,200,348 with a graft window, they found that inclusion of the graft window would either require removal of the locking mechanism to another location (such as the distal portion of the inner annulus, as shown in FIG. 6 below) or require that the graft window be very small.

25 The present inventors thus set out to redesign the locking mechanism of US Patent Number 6,200,348 so that inclusion of a graft window would not require removal of the locking mechanism to another location, nor require that the graft window be very small.

The present inventors found that replacing the set screw/spherical recess
30 locking mechanism of US Patent Number 6,200,348 with a new mechanism solved the above noted problem. The new mechanism is an engagement member which comprises i) a set screw and ii) a pressure plate having an outer face contacting the set screw and an inner face having teeth adapted to mate with the ratchet notches of the second member

Moreover, the present inventors found that the new locking mechanism imparted a superior strength to the cage so that only one set screw was needed to lock the cage in its expanded condition.

Also in accordance with the present invention, there is provided a spacer for
5 insertion between two vertebrae, said spacer having a variable axial height and comprising a first member and a second member guided within the first member to be slidable relative thereto in an axial direction thereof for adjusting an overall height, wherein the second member comprises an outer wall and ratchet notches provided at its outer wall facing the first member and extending in the axial direction,
10 wherein the first member comprises a wall having an engagement member, which cooperates with the ratchet notches for adjusting the overall height of the spacer, and wherein the engagement member comprises i) a set screw and ii) a pressure plate having an outer face contacting the set screw and an inner face having teeth adapted to mate with the ratchet notches of the second member.

15

DESCRIPTION OF THE FIGURES

FIGS. 1a and 1b disclose front and back views of a cage of the present invention.

20 FIG. 1c discloses a cage of the present invention having windows in both annuluses.

FIG. 2a discloses a cage of the present invention in which the teeth of the pressure plate mate with the notches on the inner annulus.

25 FIG. 2b discloses details of the engagement mechanism of the present invention.

FIG. 3a discloses a perspective view of the engagement member of the present invention.

30 FIG. 3b discloses a cross-section of the engagement mechanism of the present invention having a pressure plate.

FIGS 4a-4c disclose cages of the present invention respectively adapted for lateral, direct anterior and postero-lateral insertion.

FIG. 5 discloses a cage having the graft window on its inner annulus.

FIG. 6 discloses a cage of the present invention wherein the engagement mechanism
5 comprises a pressure plate located on the distal portion of the inner second annulus
and the notches located on the inner portion of the outer first annulus.

FIG. 7 discloses an inserter-expander instrument for inserting and expanding the cage
of the present invention.

10

FIG. 8 discloses an inserter/expander instrument provided with a pistol grip

FIGS. 9a-9c disclose the pistol grip portion of the instrument rotated to three
positions.

15

FIGS 10a-10c disclose an embodiment of the second distractor and various portions
thereof.

FIG.11 discloses a plurality of endplate trials used with a posterior approach cage.

20

FIG. 12 discloses a graft loading block.

FIG. 13 discloses a bone tamp.

25 FIG. 14 discloses a grabber anti-torque instrument.

FIG. 15 discloses a pair of positioning impactors.

DETAILED DESCRIPTION OF THE INVENTION

30

For the purposes of the present invention “spacer” and “cage” are used
interchangeably.

Now referring to FIG. 1 there is provided a spacer for insertion between two
vertebrae, the spacer having a variable axial height and comprising a sleeve-shaped

first member 1 and a second member 2 guided within the first member to be slidable relative thereto in an axial direction thereof for adjusting an overall height,

wherein the second member comprises an outer wall 3 and ratchet notches 5 provided at its outer wall facing the first member and extending in the axial direction,

5 and

wherein the first member comprises a wall 7 having an engagement member 9, which cooperates with the ratchet notches for adjusting the overall height of the spacer,

wherein the first member has a window 10 therein for inserting graft material therethrough, and

wherein the engagement member 9 comprises i) a set screw 11 and ii) a pressure plate 13 having an outer face 15 contacting the set screw and an inner face 17 having teeth 19 adapted to mate with the ratchet notches of the second member.

The first member generally has a tubular shape comprising a first annulus 21. The outer end of the first member should be adapted to seat upon a lower vertebral endplate, and so a substantially flat endplate 25 is generally attached to the outer end 27 of the first annulus. This endplate generally has a hole in its center and extends outwardly substantially radially from the outer end of the annulus. The outer face 28 of the endplate should be adapted to grip the lower vertebral endplate and so is generally provided with roughened features 29. These roughened features may be a plurality of uniformly distributed, pointed teeth 31 that bite into the adjacent endplate. In other embodiments, the teeth may be non-uniformly distributed. For further insuring that the endplate will be stably seated into the vertebral endplate, the outer face of the endplate may also have a few long spikes 33 extending therefrom. In some embodiments, the endplate has an overall convex shape in order to suitably conform to the overall concave shape of the natural vertebral endplate in which it seats. In some embodiments (as in FIG. 1c), the endplate has a wedge cross-section in order to conform to the lordosis adopted by the natural spine in the region of the implant. Typically, the wedge is designed to provided a lordotic angle of between about 0 and about 24 degrees, more typically between about 6 and about 12 degrees . The wedge may also be designed to provided a kyphotic angle of between about 0 and about -12 degrees,

In general, the outer dimensions of the endplates of the present invention are between about 16 mm and about 30 mm (e.g., 16 x 20; 20x23 and 24x30).

The annular portion of the first member also comprises a plurality of uniformly distributed, transverse, through-holes 35. These throughholes are generally about 2-8 mm in diameter, and provide a means for bone growth therethrough. The holes are preferably of diamond shape, although other shapes such as triangles may be used. When in a diamond shape, suitable sizes include 2.5 mm x 3.5 mm shapes to 5 mm x 7 mm shapes. In the particular FIGS. 1a and 1b, the throughholes have a diamond shape. The diamond shape allows the annulus material to make a mesh pattern in the wall that has structural advantages. However, any conventional shape may be used for the through-hole pattern. In some embodiments, the plurality of throughholes occupy only the distal portion 37 of the annulus. In such an embodiment, graft windows may be placed both on the proximal 39 and lateral 41 portions of the annulus. This has the advantage of allowing the surgeon to place bone graft into the cage from a variety of angles. In some embodiments, the plurality of throughholes occupy not only the distal portion of the first annulus, but also the lateral portions as well. In such an embodiment, graft windows may be placed only through the proximal portion of the annulus, but the cage has the structural advantage of extra strength.

The first member generally has at least one graft window 10 therein. The graft window functions both as a path through which the surgeon can place bone graft into the cage, but also as a means for bone growth therethrough. In other embodiments, the first member has a plurality of graft windows therein. When a face of the annulus has been selected for graft windows, in preferred embodiments, two graft windows 43 are placed one on top of the other, being separated by a bar 45. This bar enhances the strength of the cage. In the particular cage shown in FIG. 1a, there are two graft windows on the proximal face of the annulus, two graft windows on the left lateral face of the annulus and two graft windows on the right lateral face of the annulus. This configuration represents a balance between providing surgeon flexibility (through the inclusion of multiple faces with graft windows) and cage strength (through the use of a lateral bar between windows on any face). Each window typically has a diameter of between about 5 mm and about 20 mm. Typical windows measure 5.5 mm x 5.6 mm to 12 mm x 15.75 mm to 17.5 mm x 12 mm.

The first member may preferably include a reinforcing collar 47 surrounding the inner (upper) end portion 48 of the first annulus. The function of the reinforcing collar is to strengthen the first member and reduce deflection when the screw is

tightened. The reinforcing collar also generally has a threaded screw hole extending radially therethrough. This threaded screw hole is adapted for threadable passage of a threaded locking set screw therethrough.

Now referring to FIG. 2a, the first member comprises a collar 47 having an engagement member 9 therein, and the engagement member cooperates with the ratchet notches of the second member for adjusting a desired overall height of the spacer.

Now referring to FIG. 2b, there is provided a more detailed understanding of the engagement member. The engagement member 9 comprises i) a set screw 11 and ii) a pressure plate 13 having an outer face 15 contacting the set screw and an inner face 17 having teeth 19 adapted to mate with the ratchet notches of the second member.

In some embodiments, as in FIG. 2b, a cylindrical outer surface 20 of the set screw is threaded to allow its advance toward the second member. In some embodiments, as in FIGS. 3a and 3b (*invention disclosure-blue*), the set screw is tubular with internal axial recesses 22 therein extending along its axis. These axial recesses mate with a screwdriver, thus allowing the screw to be rotated and thereby advanced towards the second member.

The set screw further has a neck and head extension 49 extending from its distal end 50, wherein the extension is shaped so as to both provide engagement with a corresponding recess 51 of the pressure plate and allow its rotation during that engagement.

Now referring to FIGS. 3a and 3b, the pressure plate 13 has an outer face 15 contacting the set screw and an inner face 17 having teeth 19 adapted to mate with the ratchet notches of the second member. The outer face has a neck and head recess 51 therein that corresponds with the head and neck extension of the set screw so as to both provide engagement with a corresponding extension of the set screw and allow rotation of the set screw during that engagement. The pressure plate is seated on the inside face of the collar.

The inner face of the pressure plate has at least two elongated teeth 19 thereon forming at least one notch therebetween. The tips of the teeth are preferably spaced apart a distance of between about 1 mm and 2 mm, generally about 1.5 mm. The spacing can be larger or smaller than these values, with smaller being preferable.

Now referring to FIG. 1b, the distal 37 portion of the first member also has an assembly pin 53 extending radially inward from the collar. This assembly pin slidably mates with a corresponding assembly groove 54 of the second member in order to maintain the second member in a slidable orientation within the first member,
5 and to retain the first member to the second member.

Still referring to FIG. 1b, the second member generally has a tubular shape comprising a second annulus 55. The outer diameter of the second annulus should be slightly smaller than the inner diameter of the first annulus of the first member, in order to provide slidable reception of the second annulus within the first member.

10 The outer end of the second member should be adapted to seat upon an upper vertebral endplate, and so a substantially flat endplate 57 is generally attached to the outer end 59 of the second annulus 55. This endplate generally has a hole in its center and extends outward substantially radially from the upper end of the annulus. The outer face of the endplate should be adapted to grip the upper vertebral endplate and
15 so is generally provided with roughened features 29. These roughened features may be a plurality of uniformly (or non-uniformly) distributed, pointed teeth 31 that bite into the adjacent endplate. For further insuring that the endplate will be stably seated into the vertebral endplate, the outer face of the endplate may also have a few long spikes 33 extending therefrom. In some embodiments, the endplate has an overall
20 convex shape in order to suitably conform to the overall concave shape of the natural vertebral endplate in which it seats.

The annular portion of the second member also comprises a plurality of uniformly distributed, transverse, through-holes 35. These throughholes are generally of the throughhole size discussed above, , and provide a means for bone growth
25 therethrough. In this particular FIG. 1a, the throughholes have a diamond shape. The diamond shape allows the second annulus material to make a mesh pattern that has structural advantages. However, any conventional shape may be used for the through-hole pattern. In some embodiments, the plurality of throughholes occupy each of the lateral faces of the posterior portion of the second annulus.

30 The second member may preferably include a reinforcing collar 61 surrounding the outer (upper) end portion 59 of the second annulus. The function of this reinforcing collar is to allow for instrument attachment. The reinforcing collar also generally has a plurality of through-holes 63 extending radially therethrough.

These throughholes function as areas for instrument attachment, and as areas for bone growth and vascularization.

The proximal portion 65 of the second annulus has a plurality of elongated teeth 67 thereon forming at least one notch 69 therebetween. These teeth and notches
5 form a row extending up the outside of the annulus. Typically, the annulus of the second member has at least ten elongated notches thereon. These notches are formed to compliment the teeth of the pressure plate. The apices of the notches on the second member are generally spaced apart a distance of between about 1 mm and 2 mm, generally about 1.5 mm. The spacing can be larger or smaller than these values, with
10 smaller being preferable.

The distal 70 portion of the second annulus of the second member also has an assembly groove 54 extending inwardly and axially along the outside 68 of the second annulus. This assembly groove mates with the corresponding assembly pin of the first member in order to maintain the second member in a slidable orientation within the
15 first member.

Once the overall height of the cage has been determined by the surgeon and the relative disposition of the first and second members set accordingly, the set screw is then rotated by the surgeon using a screwdriver. The set screw acts to advance the
20 pressure plate so that the teeth on the pressure plate contact the ratchet notches of the second member, thereby locking the desired overall height of the cage.

The general design of the cage of the present invention provided in FIGS. 1a and 1b may be altered in order to be suit the approach used to implant the cage.

For example, now referring to FIG. 4a, there is provided a cage suited for a
25 lateral approach. A lateral approach is generally characterized by a surgical opening on a lateral side of the spine. Accordingly, the Lateral cage of FIG. 4a possesses a graft window 71 that opens onto a lateral side 73 of the outer annulus. This allows the surgeon to conveniently place graft into the cage through the lateral surgical opening used to approach the spine.

For example, now referring to FIG. 4b, there is provided a cage suited for a
30 direct anterior approach. A direct anterior approach is generally characterized by surgical opening on the anterior portion of the spine. Accordingly, the Direct Anterior cage of FIG. 4b possesses a graft window 75 that opens onto a generally anterior side 77 of the outer annulus. In some embodiments, the window is oriented

45 degrees to the endplates in order to avoid the great vessels. This allows the surgeon to conveniently place graft into the cage through the anterior surgical opening used to approach the spine.

For example, now referring to FIG. 4c, there is provided a cage suited for a postero-lateral approach. A postero-lateral approach is generally characterized by a surgical opening on a postero-lateral side of the spine. Accordingly, the postero-lateral cage of FIG. 4c possesses a graft window 79 that opens onto a postero-lateral side 81 of the outer annulus. This allows the surgeon to conveniently place graft into the cage through the postero-lateral surgical opening used to approach the spine. The window of this cage is placed so that it opens to the surgeon. In some embodiments, the endplates of this cage are substantially circular so as not to be approach-specific.

Typically, the cages of the present invention are designed to occupy either one, two or three levels of a thoracolumbar corpectomy. In some embodiments having either 16 mm or 20 mm endplate dimensions, the height of the cage can be between 22 mm and 72 mm. In some embodiments having 24 mm endplate dimensions, the height of the cage can be between 22 mm and 110 mm. In general, the cage is designed to expand its height in an increment of between about 8.5 mm to about 25 mm. Cages can be designed to overlap in height ranges with their adjacent sizes. For example a first cage can range in height from 25 to 33.5 mm, while a second cage can range in height from 28.5 mm to 38.5 mm in height.

When the cage of the present invention is generally short (i.e., an overall height of less than about 40 mm), it is advantageous to provide the sole graft window on the second (inner) annulus. Now referring to FIG. 5, there is provided a spacer for insertion between two vertebrae, the spacer having a variable axial height and comprising a sleeve-shaped first outer member 83 and a second inner member 84 guided within the first member to be slidable relative thereto in an axial direction thereof for adjusting an overall height,

wherein the second member comprises an outer wall and ratchet notches provided at its outer wall facing the first member and extending in the axial direction, wherein the first member comprises a wall having an engagement member, which cooperates with the ratchet notches for adjusting the overall height of the spacer, and

wherein the second member 84 has a window 85 therein for inserting graft material therethrough.

In cages of the present invention characterized as tall (greater than 40 mm), one annulus has a flange. Now referring to FIG. 1c, there is provided a cage of the present invention having features substantially the same as that of FIG. 1a and 1b, except that the proximal portion of the inner second annulus has a distal flange 87
5 upon its inner end portion 88.

In some embodiments, the features of the engagement mechanism are reversed so that the pressure plate is located on the distal portion of the inner second annulus and the notches are located on the inner portion of the outer first annulus.

10 Now referring to FIG. 6, there is provided a spacer 101 for insertion between two vertebrae, the spacer having a variable axial height and comprising a sleeve-shaped first outer member 103 and a second inner member 105 guided within the first member to be slidable relative thereto in an axial direction thereof for adjusting an overall height,

15 wherein the first outer member comprises an inner wall 107 and ratchet notches 109 provided at its inner wall facing the second member and extending in the axial direction, and

20 wherein the second inner member comprises a wall 111 having an engagement member 113, which cooperates with the ratchet notches of the first outer member for adjusting the overall height of the spacer, and

wherein the engagement member comprises i) a set screw and ii) a pressure plate
25 having an outer face contacting the set screw and an inner face having teeth adapted to mate with the ratchet notches of the first outer member.

In some embodiments, the instrument set used to implant the cage of the present invention includes a) a pistol grip inserter/expander; b) a secondary distractor; c) endplate trials (straight and flexible); d) a bone graft loading block; e) bone tamps;
30 f) a 3 Nm torque limiting driver; g) a grabber/anti-torque instrument; and h) positioning impactors.

Now referring to FIG. 7, there is provided an inserter-expander instrument 115. This instrument is used to hold the cage during its insertion and expand the cage

after it has been inserted. This instrument includes a modular inserter valve 117 for each size of implant; threaded pins 119 adapted for alignment of the cage and a third threaded rod (not shown) for attachment to the cage; a knob 121 for securing implant attachment to the inserter; a handle 123; and a knob 125 for expanding and retracting the cage. Also shown is a stand alone torque driver 124.

In use, the cage of the present invention is attached to the pins 119 by the surgeon using knob 121. Next, the cage is inserted into the implant site. Knob 125 is then rotated to expand the implant to the pre-determined height. Next, the cage height is locked by advancing the set screw of the engagement member. Lastly, knob 121 is then rotated to release the pins from the implant.

Now referring to FIG. 8, in some embodiments, the inserter/expander instrument is provided with a pistol grip 127. The pistol grip provides an advantage in that it provides rapid implant expansion to contact the vertebral endplate.

Now referring to FIG. 9a-9c, the pistol grip portion of the instrument can be adapted to provide rotation. This pistol grip can rotate and then lock into one of three positions. FIG. 9a shows the pistol grip in the 0 degree position. FIG. 9b shows the pistol grip in the 90 degree position. FIG. 9c shows the pistol grip in the 180 degree position.

Now referring to FIGS. 10a-10c, there are provided figures of the second distractor 131. The function of the second distractor is to first distract the vertebral bodies located above and below the implantation site to their normal anatomical position and then to estimate the size of the implant required. . FIG. 10a shows the secondary distractor with lateral attachments 133 and a height indicator 135. FIGS. 10b and 10c provide closeups of the distal end of the secondary distractor having offset lateral attachments 137 (to estimate height for taller implants) and angled posterior attachments 139 (for ease of use during posterior surgical approaches).

Now referring to FIG. 11, there is provided a plurality of endplate trials 141 used with a posterior approach cage. These trials are used to assess the dimensions of the vertebral endplates against which the cage will seat in order to select the appropriate size for an endplate of the cage of the present invention. These trials can be made with varying levels of flexibility in order to allow access around the local tissue and to access the exposed vertebral body endplate .

Now referring to FIG. 12, there is provided a graft loading block 143 having a plurality of recesses 145 conforming to the shapes of various size cages. The surgeon

puts the cage into this block during graft loading in order to enhance the stability of the loading procedure.

Now referring to FIG. 13, there is provided a bone tamp 147, which is used to pack the bone graft into the cage after it has been loaded into the cage.

5 Now referring to FIG. 14, there is provided a grabber anti-torque instrument 149. The function of the grabber anti-torque instrument is to stabilize the implant when the set screw is loosened for retraction and to remove the implant from the site.

Now referring to FIGS. 15a and 15b, there is provided a pair of positioning impactors 151. These instruments may be used to gently reposition the implant.

10 In some embodiments, the graft window of the present invention is used to a deliver either a bone cement or a bone-forming agent into the cage. The bone cement may be any material typically used to augment vertebral bodies, including acrylic-based bone cements (such as PMMA-based bone cements), pastes comprising bone particles (either mineralized or demineralized or both; and ceramic-based bone
15 cements (such as HA and TCP-based pastes). In some embodiments, the bone cement comprises the bone cement disclosed in WO 02/064062 (Voellmicke).

For the purposes of the present invention, the terms "bone-forming agent" and "bone growth agent" are used interchangeably. Typically, the bone-forming agent may be:

- 20 a) a growth factor (such as an osteoinductive or angiogenic factor),
b) osteoconductive (such as a porous matrix of granules),
c) osteogenic (such as viable osteoprogenitor cells), or
d) plasmid DNA.

25 In some embodiments, the formulation comprises a liquid carrier, and the bone forming agent is soluble in the carrier.

In some embodiments, the bone forming agent is a growth factor. As used herein, the term "growth factor" encompasses any cellular product that modulates the growth or differentiation of other cells, particularly connective tissue progenitor cells.

30 The growth factors that may be used in accordance with the present invention include, but are not limited to, members of the fibroblast growth factor family, including acidic and basic fibroblast growth factor (FGF-1 and FGF-2) and FGF-4; members of the platelet-derived growth factor (PDGF) family, including PDGF-AB, PDGF-BB and PDGF-AA; EGFs; VEGF; members of the insulin-like growth factor (IGF)

family, including IGF-I and -II; the TGF- β superfamily, including TGF- β 1, 2 and 3; osteoid-inducing factor (OIF), angiogenin(s); endothelins; hepatocyte growth factor and keratinocyte growth factor; members of the bone morphogenetic proteins (BMPs) BMP-1, BMP-3, BMP-2, OP-1, BMP-2A, BMP-2B, BMP-7 and BMP-14, including
5 MP-52; HBGF-1 and HBGF-2; growth differentiation factors (GDFs), including GDF-5, members of the hedgehog family of proteins, including indian, sonic and desert hedgehog; ADMP-1; bone-forming members of the interleukin (IL) family; GDF-5; and members of the colony-stimulating factor (CSF) family, including CSF-1, G-CSF, and GM-CSF; and isoforms thereof.

10 In some embodiments, the growth factor is selected from the group consisting of TGF- β , bFGF, and IGF-1. These growth factors are believed to promote the regeneration of bone. In some embodiments, the growth factor is TGF- β . More preferably, TGF- β is administered in an amount of between about 10 ng/ml and about 5000 ng/ml, for example, between about 50 ng/ml and about 500 ng/ml, *e.g.*, between
15 about 100 ng/ml and about 300 ng/ml.

In some embodiments, platelet concentrate is provided as the bone forming agent. In one embodiment, the growth factors released by the platelets are present in an amount at least two-fold (*e.g.*, four-fold) greater than the amount found in the blood from which the platelets were taken. In some embodiments, the platelet
20 concentrate is autologous. In some embodiments, the platelet concentrate is platelet rich plasma (PRP). PRP is advantageous because it contains growth factors that can restimulate the growth of the bone, and because its fibrin matrix provides a suitable scaffold for new tissue growth.

In some embodiments, the bone forming agent comprises an effective amount
25 of a bone morphogenic protein (BMP). BMPs beneficially increasing bone formation by promoting the differentiation of mesenchymal stem cells (MSCs) into osteoblasts and their proliferation.

In some embodiments, between about 1 ng and about 10 mg of BMP are intraosseously administered into the target bone. In some embodiments, between
30 about 1 microgram (μ g) and about 1 mg of BMP are intraosseously administered into the target bone.

In some embodiments, the bone forming agent comprises an effective amount of a fibroblast growth factor (FGF). FGF is a potent mitogen and is angiogenic, and

so attracts mesenchymal stem cells to the target area. It is further believed that FGF stimulates osteoblasts to differentiate into osteocytes.

In some embodiments, the FGF is acidic FGF (aFGF).

In some embodiments, the FGF is basic FGF (bFGF).

5 In some embodiments, between about 1 microgram (μg) and about 10,000 μg of FGF are intraosseously administered into the target bone. In some embodiments, between about 10 μg and about 1,000 μg of FGF are intraosseously administered into the target bone. In some embodiments, between about 50 μg and about 600 μg of FGF are intraosseously administered into the target bone.

10 In some embodiments, between about 0.1 and about 4 mg/kg/day of FGF are intraosseously administered into the target bone. In some embodiments, between about 1 and about 2 mg/kg/day of FGF are intraosseously administered into the target bone.

In some embodiments, FGF is intraosseously administered into the target bone
15 in a concentration of between about 0.1 mg/ml and about 100 mg/ml. In some embodiments, FGF is intraosseously administered into the target bone in a concentration of between about 0.5 mg/ml and about 30 mg/ml. In some embodiments, FGF is intraosseously administered into the target bone in a concentration of between about 1 mg/ml and about 10 mg/ml.

20 In some embodiments, FGF is intraosseously administered into the target bone in an amount to provide a local tissue concentration of between about 0.1 mg/kg and about 10 mg/kg.

In some embodiments, the formulation comprises a hyaluronic acid carrier and bFGF. In some embodiments, formulations described in U.S. Patent No. 5,942,499
25 ("Orquest") are selected as FGF-containing formulations.

In some embodiments, the bone forming agent comprises an effective amount of insulin-like growth factor. IGFs beneficially increase bone formation by promoting mitogenic activity and/or cell proliferation.

In some embodiments, the bone forming agent comprises an effective amount
30 of parathyroid hormone (PTH). Without wishing to be tied to a theory, it is believed that PTH beneficially increases bone formation by mediating the proliferation of osteoblasts.

In some embodiments, the PTH is a fragment or variant, such as those taught in U.S. Patent Nos. 5,510,370 (Hock) and 6,590,081 (Zhang), and published patent application 2002/0107200 (Chang), the entire contents of which are incorporated herein in their entirety. In one embodiment, the PTH is PTH (1-34) (teriparatide),
5 *e.g.*, FORTEO[®] (Eli Lilly and Company). In some embodiments, the BFA is a parathyroid hormone derivative, such as a parathyroid hormone mutein. Examples of parathyroid muteins are discussed in U.S. Patent No. 5,856,138 (Fukuda), the entire contents of which are incorporated herein in its entirety.

10 In some embodiments, the bone forming agent comprises an effective amount of a statin. Without wishing to be tied to a theory, it is believed that statins beneficially increase bone formation by enhancing the expression of BMPs.

In some embodiments, the bone forming agent is a porous matrix, and is preferably injectable. In some embodiments, the porous matrix is a mineral. In one embodiment, this mineral comprises calcium and phosphorus. In some embodiments,
15 the mineral is selected from the group consisting of calcium phosphate, tricalcium phosphate and hydroxyapatite. In one embodiment, the average porosity of the matrix is between about 20 and about 500 μm , for example, between about 50 and about 250 μm . In yet other embodiments of the present invention, *in situ* porosity is produced in the injected matrix to produce a porous scaffold in the injected fracture stabilizing
20 cement. Once the *in situ* porosity is produced in the target tissue, the surgeon can inject other therapeutic compounds into the porosity, thereby treating the surrounding tissues and enhancing the remodeling process of the target tissue and the injectable cement.

In some embodiments, the mineral is administered in a granule form. It is
25 believed that the administration of granular minerals promotes the formation of the bone growth around the minerals such that osteointegration occurs.

In some embodiments, the mineral is administered in a settable-paste form. In this condition, the paste sets up *in vivo*, and thereby immediately imparts post-treatment mechanical support to the fragile OP body.

30 In another embodiment, the treatment is delivered via injectable absorbable or non-absorbable cement to the target tissue. The treatment is formulated using bioabsorbable macro-sphere technologies, such that it will allow the release of the bone forming agent first, followed by the release of the anti-resorptive agent. The

cement will provide the initial stability required to treat pain in fractured target tissues. These tissues include, but are not limited to, hips, knee, vertebral body fractures and iliac crest fractures. In some embodiments, the cement is selected from the group consisting of calcium phosphate, tricalcium phosphate and hydroxyapatite.

- 5 In other embodiments, the cement is any hard biocompatible cement, including PMMA, processed autogenous and allograft bone. Hydroxylapatite is a preferred cement because of its strength and biological profile. Tricalcium phosphate may also be used alone or in combination with hydroxylapatite, particularly if some degree of resorption is desired in the cement.

- 10 In some embodiments, the porous matrix comprises a resorbable polymeric material.

In some embodiments, the bone forming agent comprises an injectable precursor fluid that produces the *in situ* formation of a mineralized collagen composite. In some embodiments, the injectable precursor fluid comprises:

- 15 a) a first formulation comprising an acid-soluble type I collagen solution (preferably between about 1 mg/ml and about 7 mg/ml collagen) and
b) a second formulation comprising liposomes containing calcium and phosphate.

- Combining the acid-soluble collagen solution with the calcium- and
20 phosphate-loaded liposomes results in a liposome/collagen precursor fluid, which, when heated from room temperature to 37 °C, forms a mineralized collagen gel.

- In some embodiments, the liposomes are loaded with dipalmitoylphosphatidylcholine (90 mol%) and dimyristoyl phosphatidylcholine (10 mol%). These liposomes are stable at room temperature but form calcium phosphate
25 mineral when heated above 35°C, a consequence of the release of entrapped salts at the lipid chain melting transition. One such technology is disclosed in Pederson, *Biomaterials* 24: 4881-4890 (2003), the specification of which is incorporated herein by reference in its entirety.

- Alternatively, the *in situ* mineralization of collagen could be achieved by an
30 increase in temperature achieved by other types of reactions including, but not limited to, chemical, enzymatic, magnetic, electric, photo- or nuclear. Suitable sources thereof include light, chemical reaction, enzymatically controlled reaction and an electric wire embedded in the material. To further elucidate the electric wire approach, a wire (which can be the reinforcement rod) can first be embedded in the

space, heated to create the calcium deposition, and then withdrawn. In some embodiments, this wire may be a shape memory such as nitinol that can form the shape. Alternatively, an electrically-conducting polymer can be selected as the temperature raising element. This polymer is heated to form the collagen, and is then
5 subject to disintegration and resorption *in situ*, thereby providing space adjacent the mineralized collagen for the bone to form.

In one embodiment, the bone forming agent is a plurality of viable osteoprogenitor cells. Such viable cells, introduced into the bone, have the capability of at least partially repairing any bone loss experienced by the bone during the
10 osteoporotic process. In some embodiments, these cells are introduced into the cancellous portion of the bone and ultimately produce new cancellous bone. In others, these cells are introduced into the cortical region and produce new cortical bone.

In some embodiments, these cells are obtained from another human individual (allograft), while in other embodiments, the cells are obtained from the same
15 individual (autograft). In some embodiments, the cells are taken from bone tissue, while in others, the cells are taken from a non-bone tissue (and may, for example, be mesenchymal stem cells, chondrocytes or fibroblasts). In others, autograft osteocytes (such as from the knee, hip, shoulder, finger or ear) may be used.

In one embodiment, when viable cells are selected as an additional therapeutic
20 agent or substance, the viable cells comprise mesenchymal stem cells (MSCs). MSCs provide a special advantage for administration into an uncoupled resorbing bone because it is believed that they can more readily survive the relatively harsh environment present in the uncoupled resorbing bone; that they have a desirable level of plasticity; and that they have the ability to proliferate and differentiate into the
25 desired cells.

In some embodiments, the mesenchymal stem cells are obtained from bone marrow, such as autologous bone marrow. In others, the mesenchymal stem cells are obtained from adipose tissue, preferably autologous adipose tissue.

In some embodiments, the mesenchymal stem cells injected into the bone are
30 provided in an unconcentrated form, *e.g.*, from fresh bone marrow. In others, they are provided in a concentrated form. When provided in concentrated form, they can be uncultured. Uncultured, concentrated MSCs can be readily obtained by centrifugation, filtration, or immuno-absorption. When filtration is selected, the methods disclosed in U.S. Patent No. 6,049,026 ("Muschler"), the specification of

which is incorporated herein by reference in its entirety, can be used. In some embodiments, the matrix used to filter and concentrate the MSCs is also administered into the uncoupled resorbing bone.

5 In some embodiments, bone cells (which may be from either an allogeneic or an autologous source) or mesenchymal stem cells, may be genetically modified to produce an osteoinductive bone anabolic agent which could be chosen from the list of growth factors named herein. The production of these osteopromotive agents may lead to bone growth.

10 In some embodiments, the osteoconductive material comprises calcium and phosphorus. In some embodiments, the osteoconductive material comprises hydroxyapatite. In some embodiments, the osteoconductive material comprises collagen. In some embodiments, the osteoconductive material is in a particulate form.

Recent work has shown that plasmid DNA will not elicit an inflammatory response as does the use of viral vectors. Genes encoding bone (anabolic) agents such as BMP may be efficacious if injected into the uncoupled resorbing bone. In addition, overexpression of any of the growth factors provided herein or other agents which would limit local osteoclast activity would have positive effects on bone growth. In one embodiment, the plasmid contains the genetic code for human TGF- β or erythropoietin (EPO).

20

Accordingly, in some embodiments, the additional therapeutic agent is selected from the group consisting of viable cells and plasmid DNA.

We Claim:

1. A spacer for insertion between two vertebrae, the spacer having a variable axial
5 height and comprising a first member and a second member guided within the first
member to be slidable relative thereto in an axial direction thereof for adjusting an
overall height,

wherein the second member comprises an outer wall and ratchet notches provided at
10 its outer wall facing the first member and extending in the axial direction,

wherein the first member comprises a wall having an engagement member, which
cooperates with the ratchet notches for adjusting the overall height of the spacer, and

15 wherein the first member has a graft window therein for inserting graft material
therethrough.
2. The spacer of claim 1 wherein the first member comprises a first annulus.
- 20 3. The spacer of claim 2 further comprising an endplate attached to an outer end of the
first annulus.
4. The spacer of claim 2 wherein the endplate has a convex shape or a wedge shape.
- 25 5. The spacer of claim 2 wherein the endplate has an outer face having roughened
features.
6. The spacer of claim 5 wherein the roughened features comprise a plurality of teeth.
- 30 7. The spacer of claim 2 wherein the endplate has an outer face having a plurality of
spikes extending therefrom.
8. The spacer of claim 2 wherein the first annulus of the first member comprises a
plurality of transverse through-holes.

9. The spacer of claim 2 wherein the first member comprises a reinforcing collar surrounding an inner end portion of the first annulus, wherein a distal portion of the first member has an assembly pin extending radially inward from the collar, and a
5 distal portion of the second member has a corresponding assembly groove, and the assembly groove mates with the assembly pin in order to maintain the second member in a slidable engagement within the first member.

10. The spacer of claim 1 wherein the first member has first and second graft
10 windows therein for inserting graft material therethrough, wherein the two graft windows are placed one on top of the other, being separated by a bar.

11. A spacer for insertion between two vertebrae, said spacer having a variable axial height and comprising a first member and a second member guided within the first
15 member to be slidable relative thereto in an axial direction thereof for adjusting an overall height,

wherein the second member comprises an outer wall and ratchet notches provided at its outer wall facing the first member and extending in the axial direction,
20

wherein the first member comprises a wall having an engagement member, which cooperates with the ratchet notches for adjusting the overall height of the spacer, and

wherein the engagement member comprises i) a set screw and ii) a pressure plate
25 having an outer face contacting the set screw and an inner face having teeth adapted to mate with the ratchet notches of the second member.


12. The spacer of claim 11 wherein the set screw is a sole screw of the engagement member.
30

13. The spacer of claim 11 wherein the set screw has a cylindrical outer surface that is threaded.

14. The spacer of claim 11 wherein the set screw is tubular defining an axis with a plurality of internal axial recesses extending along the axis.
15. The spacer of claim 11 wherein the set screw comprises a distal end and a neck
5 and head extension extending from the distal end so as to provide engagement with a corresponding neck and head recess of the pressure plate.
16. The spacer of claim 11 wherein the inner face of the pressure plate has at least two elongated teeth thereon forming at least one notch therebetween.
- 10 17. The spacer of claim 11 wherein the first member has a graft window therein for inserting graft material therethrough.
18. The spacer of claim 11 wherein the second member has a graft window therein for
15 inserting graft material therethrough.
19. The spacer of claim 11 wherein the first and second members each have a graft window therein for inserting graft material therethrough.
- 20 20. The spacer of claim 19 wherein an anterior portion of the second annulus has a cutout upon its inner end that forms the second graft window.
21. The spacer of claim 11 wherein the first member comprises a distal portion having an assembly pin, and the second member comprises a distal portion having a
25 corresponding assembly groove, and the assembly groove mates with the assembly pin in order to maintain the second member in a slidable orientation within the first member.


1/19

FIG. 1A

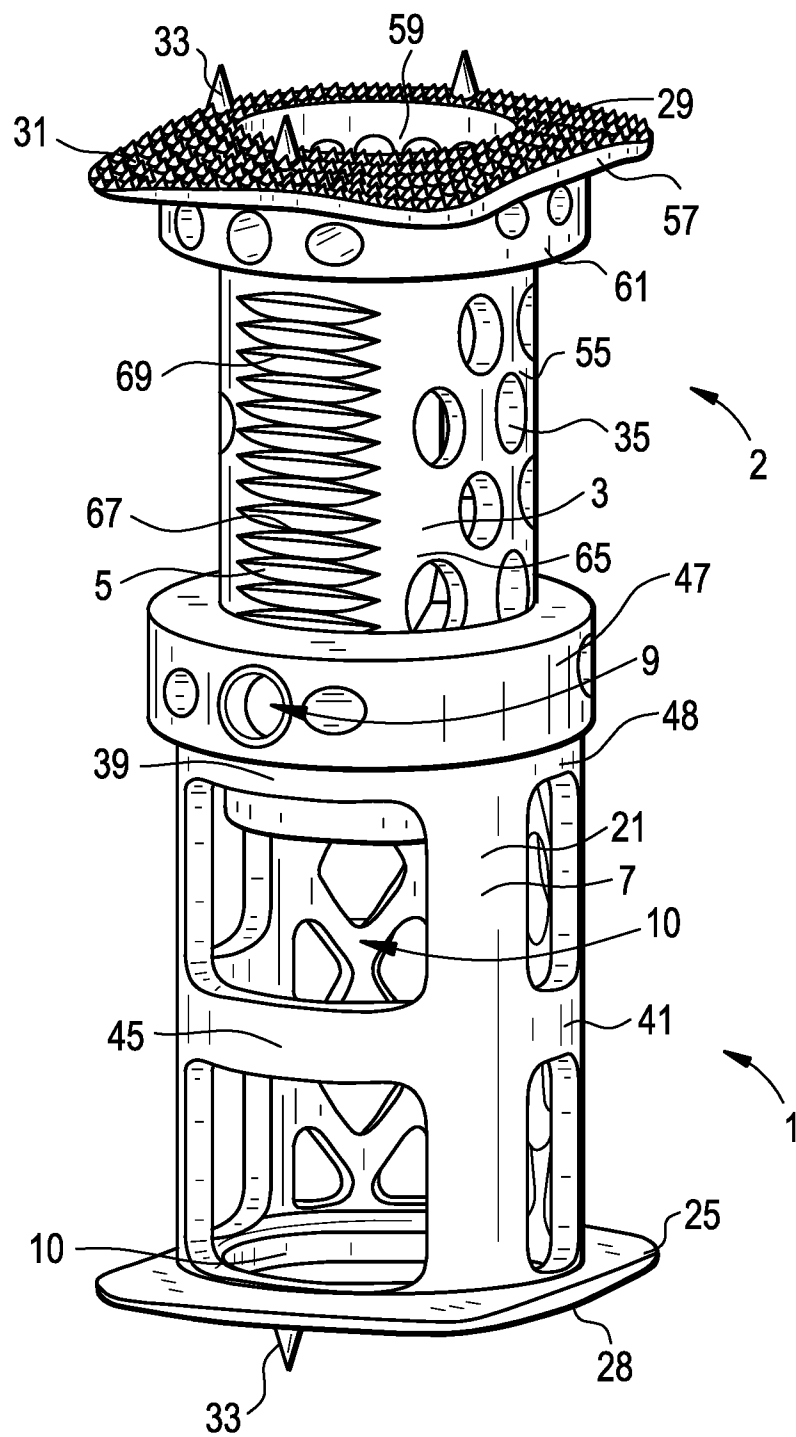


2/19

FIG. 1B

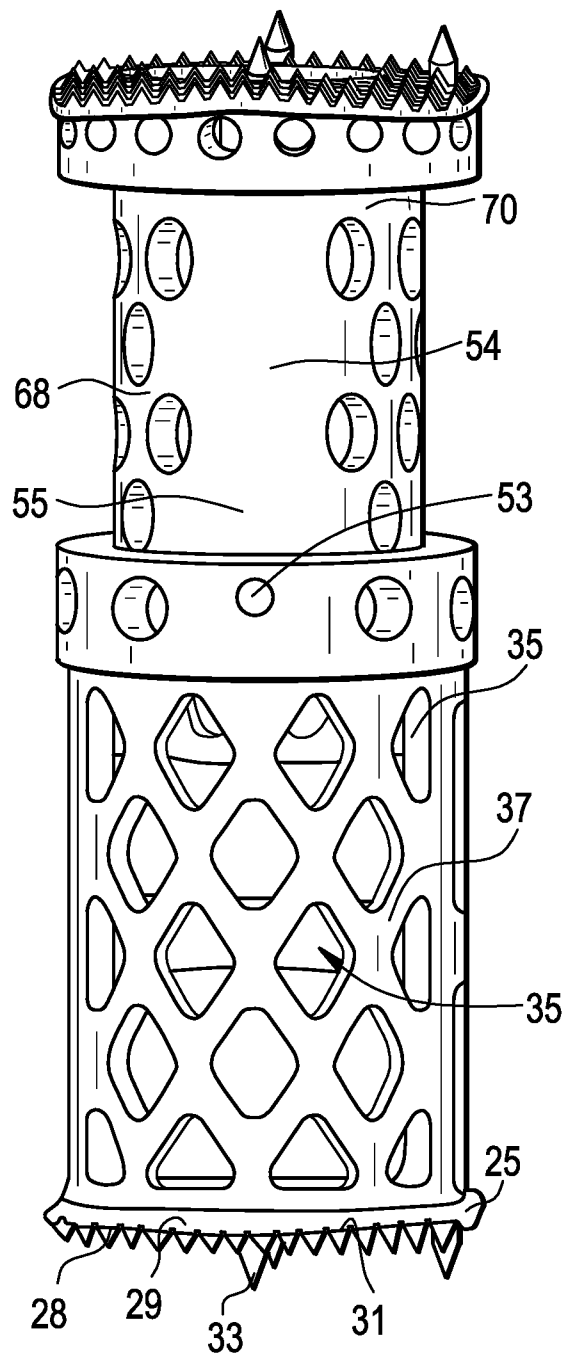

3/19

FIG. 1C

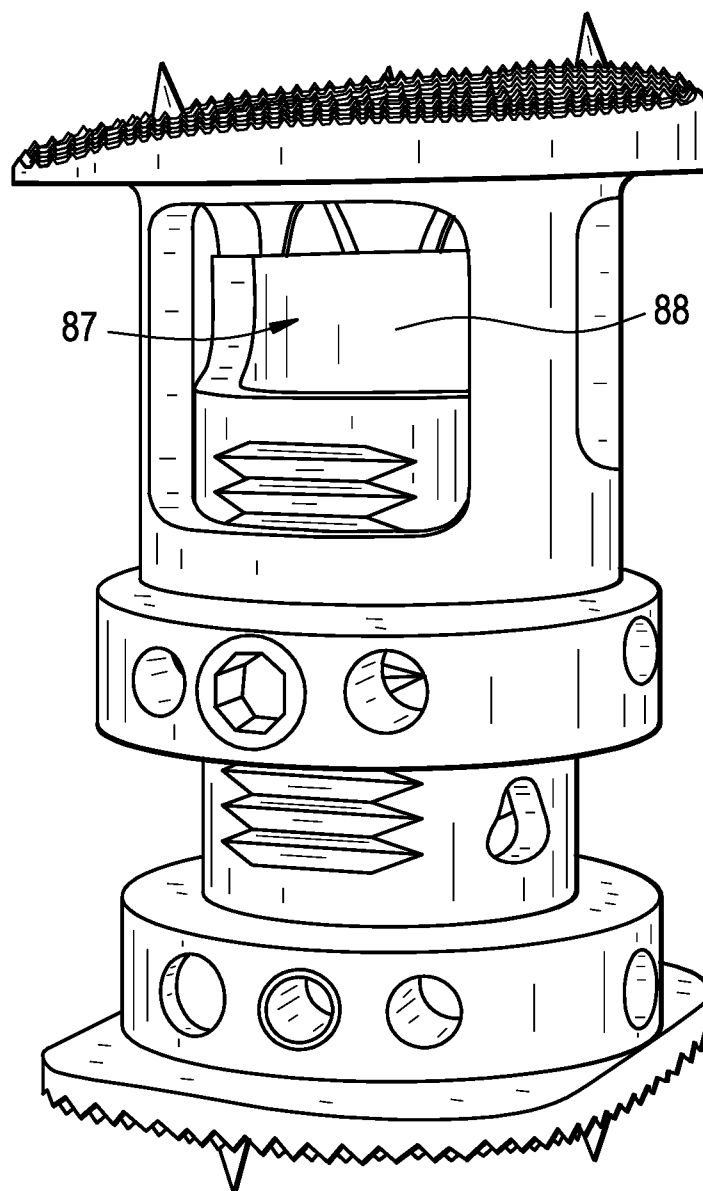

4/19

FIG. 2A


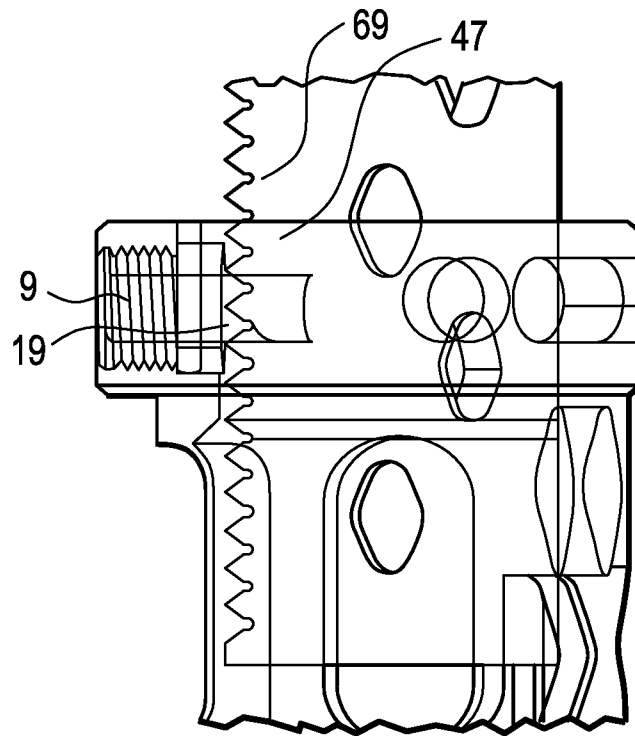


FIG. 2B

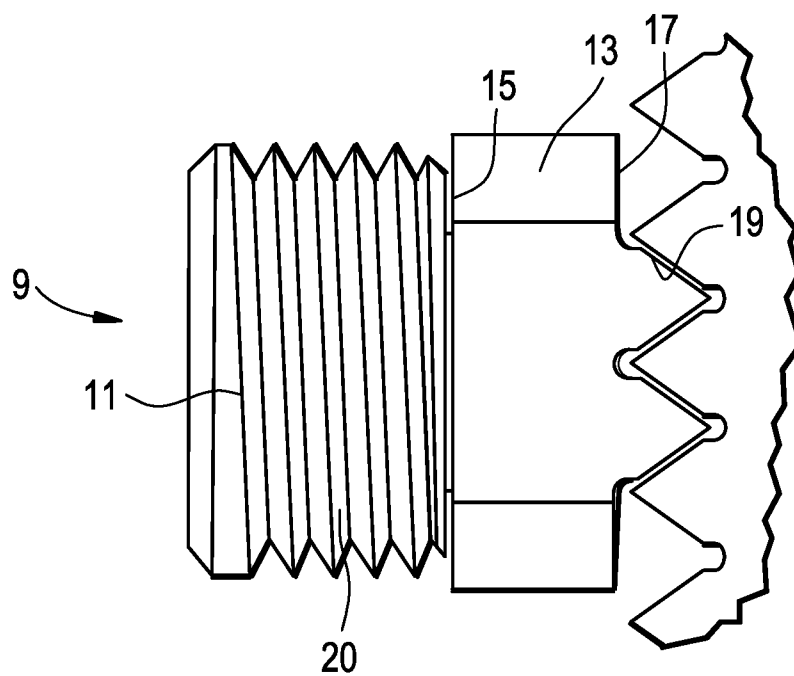

5/17

FIG. 3A



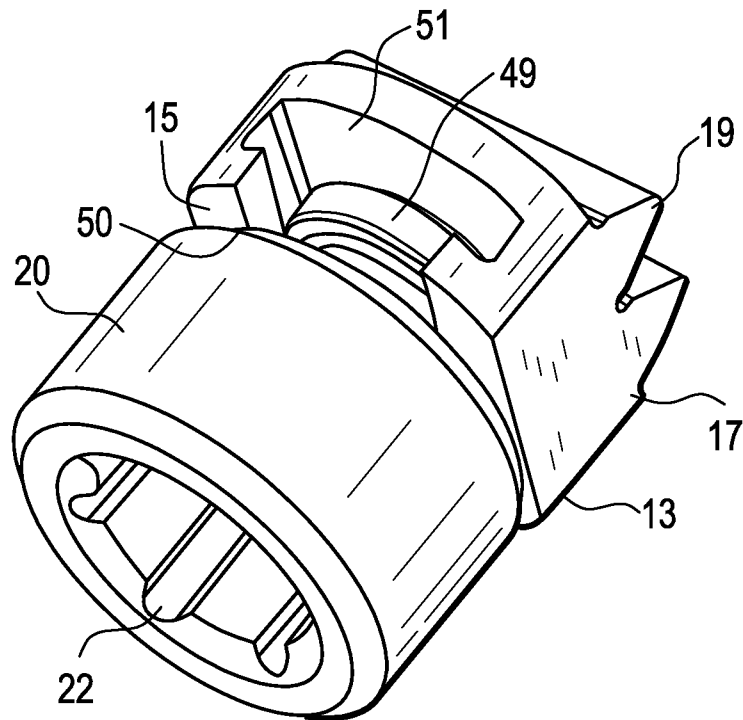


FIG. 3B

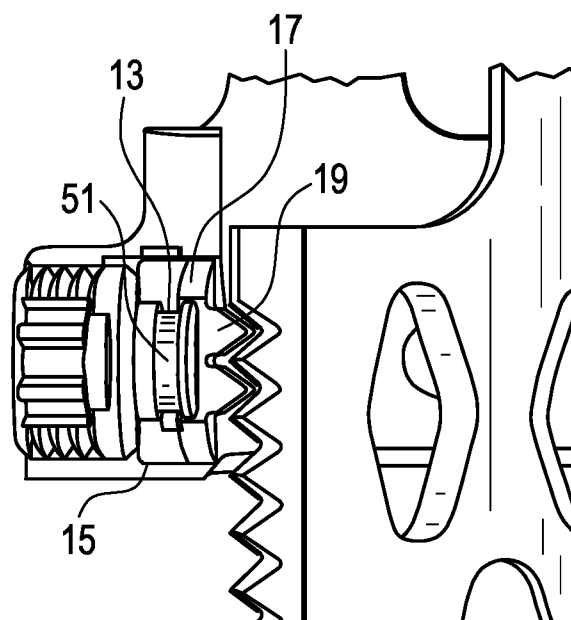


6/19

FIG. 4A

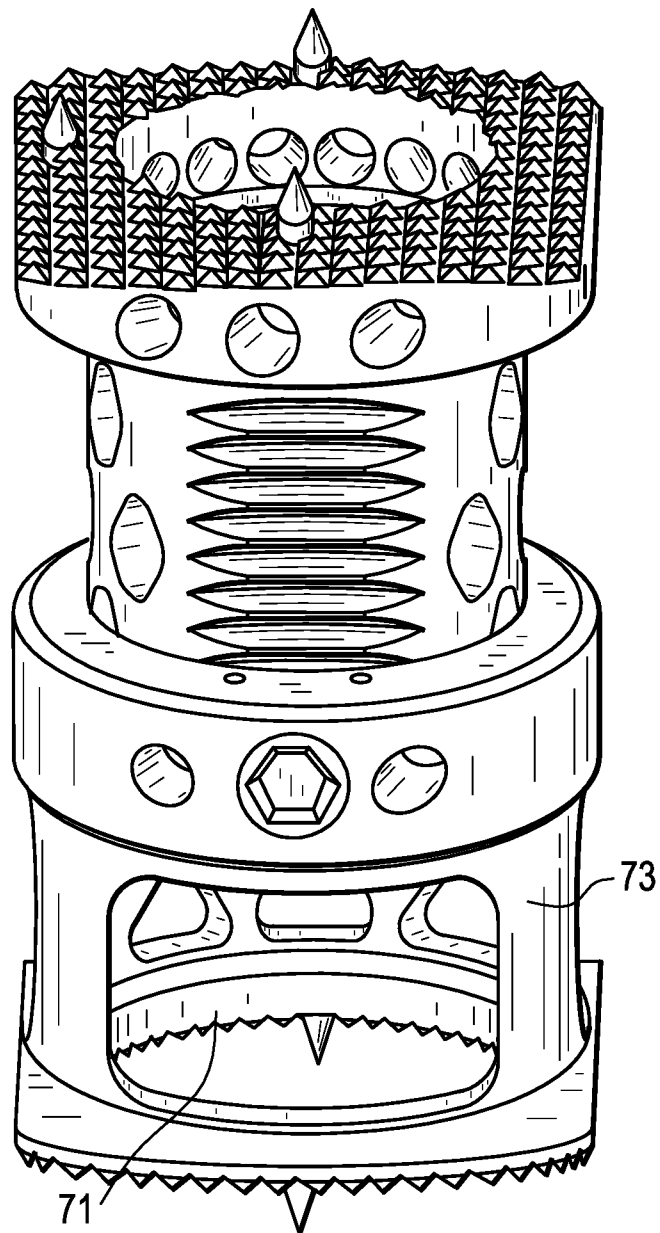

7/19

FIG. 4B

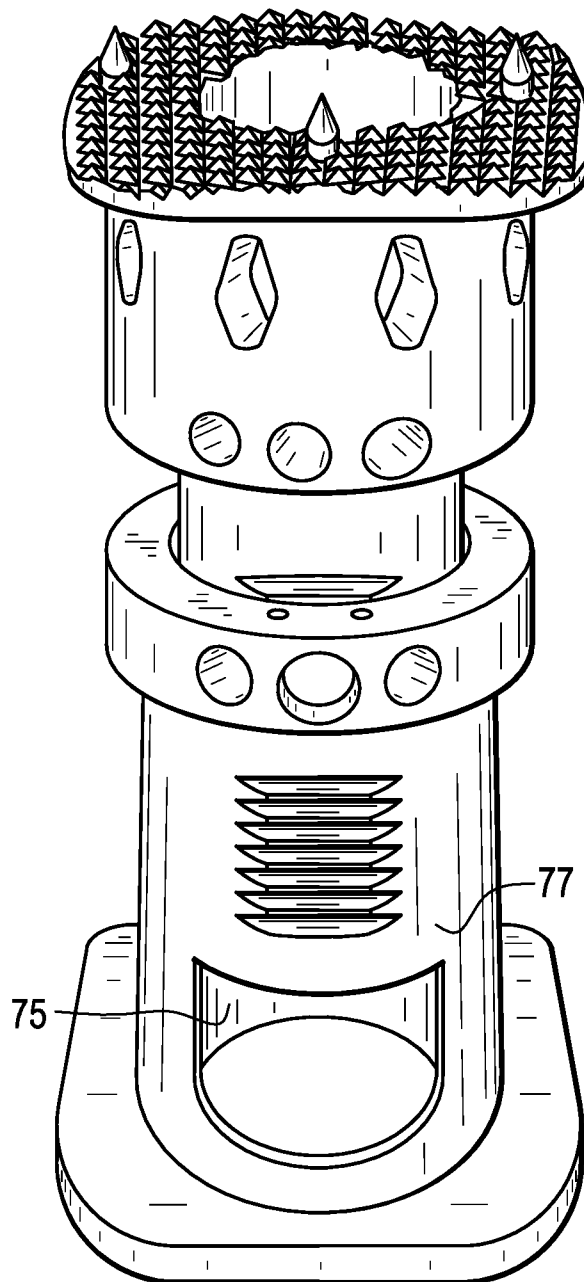

8/19

FIG. 4C



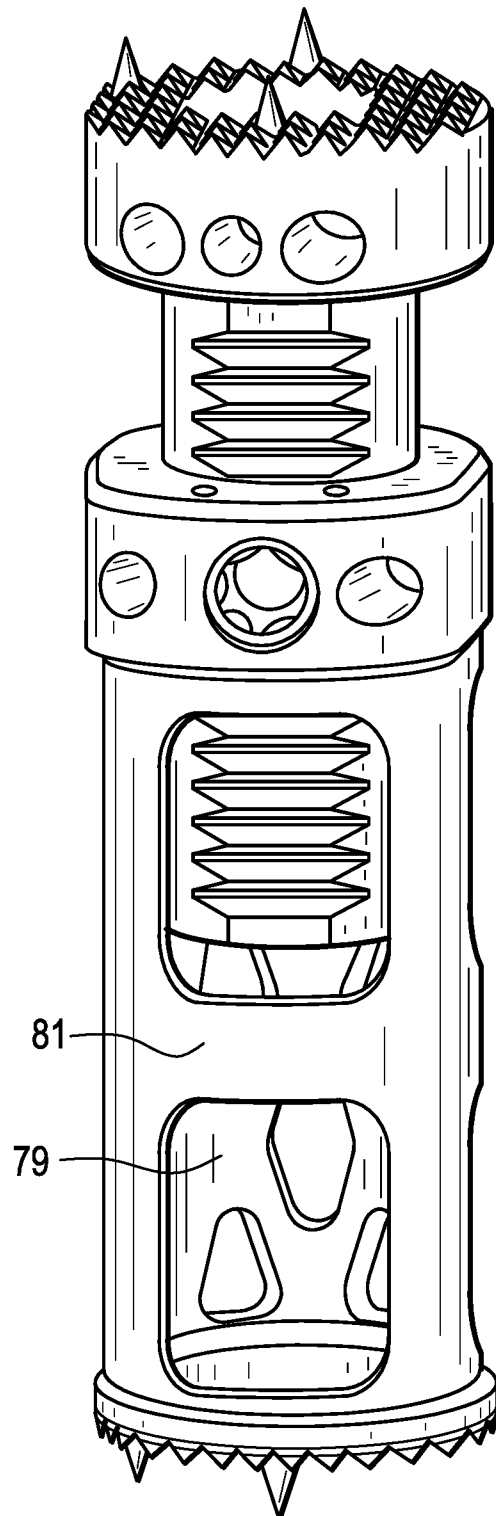


FIG. 5

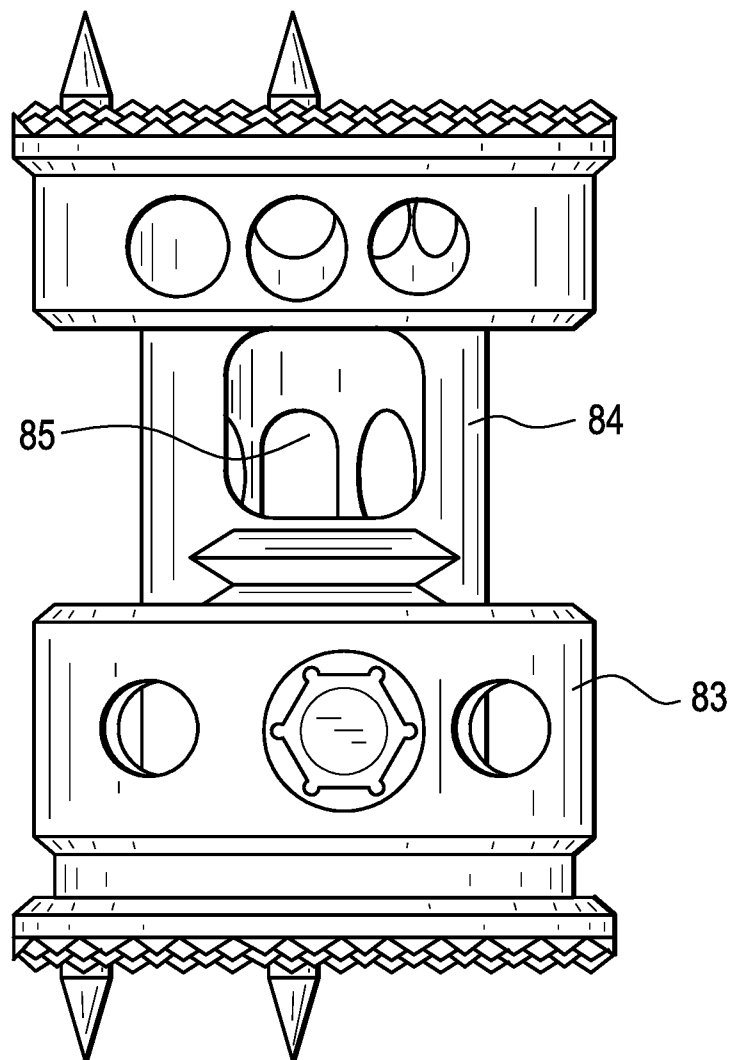

10/19

FIG. 6

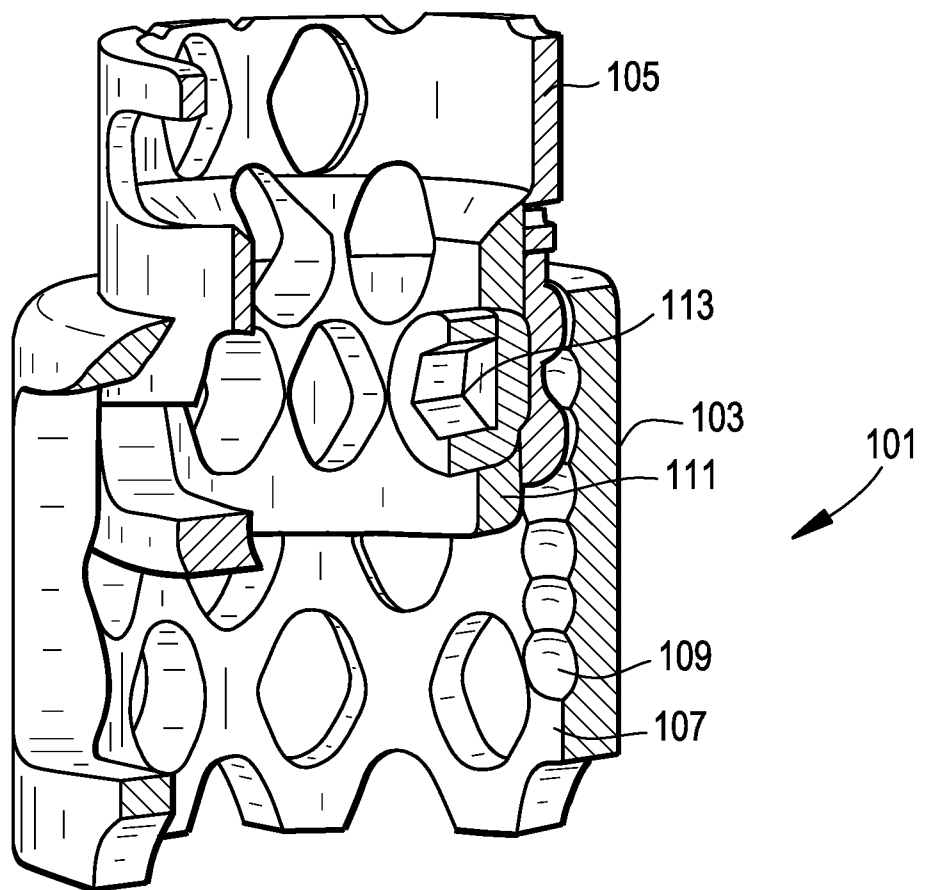

11/19

FIG. 7

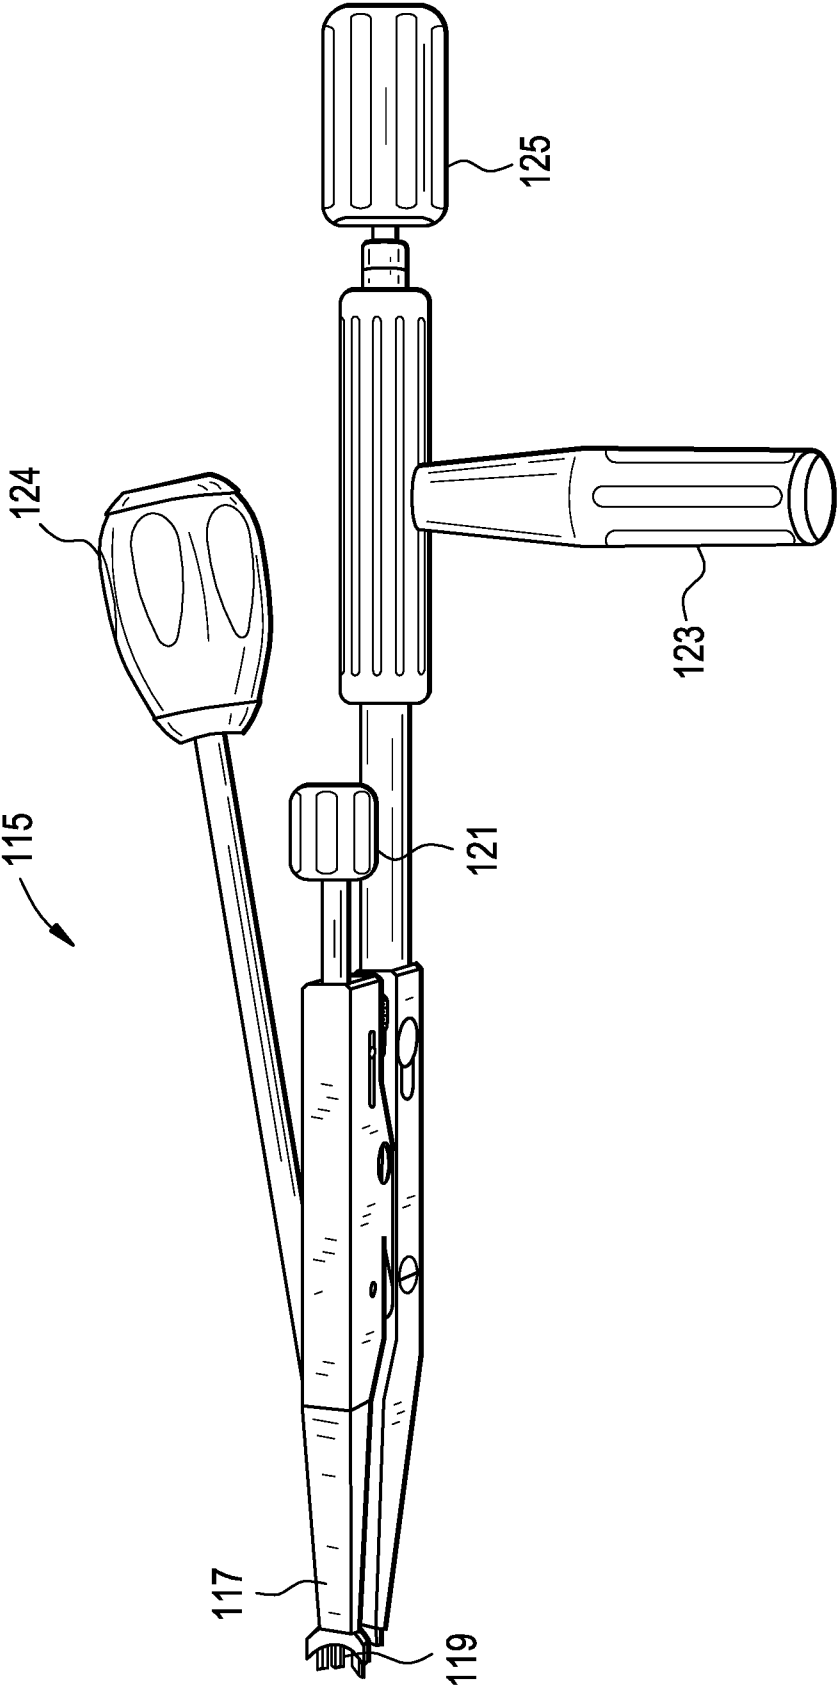


FIG. 8

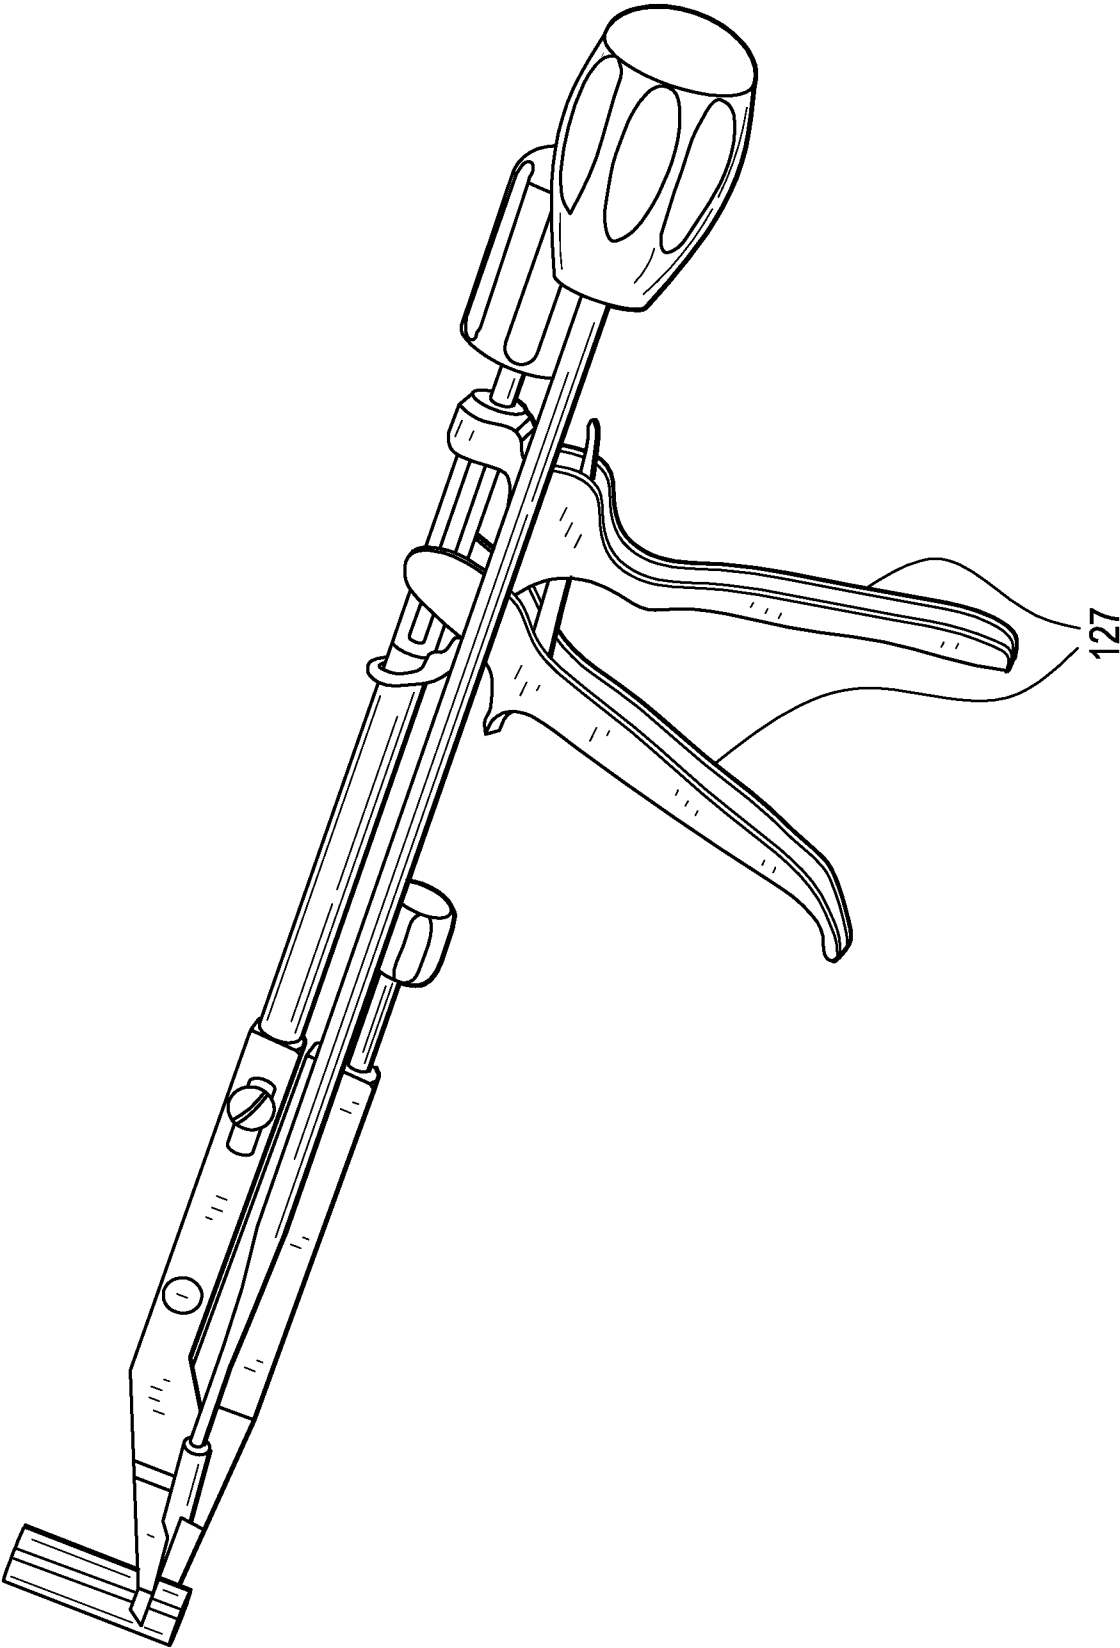


FIG. 9C

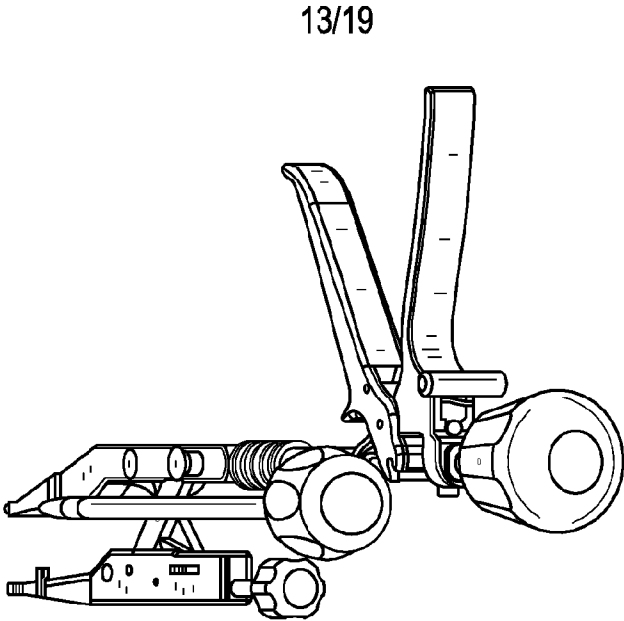


FIG. 9B



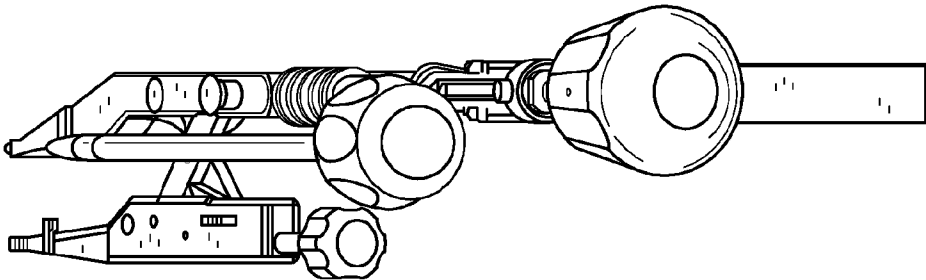


FIG. 9A

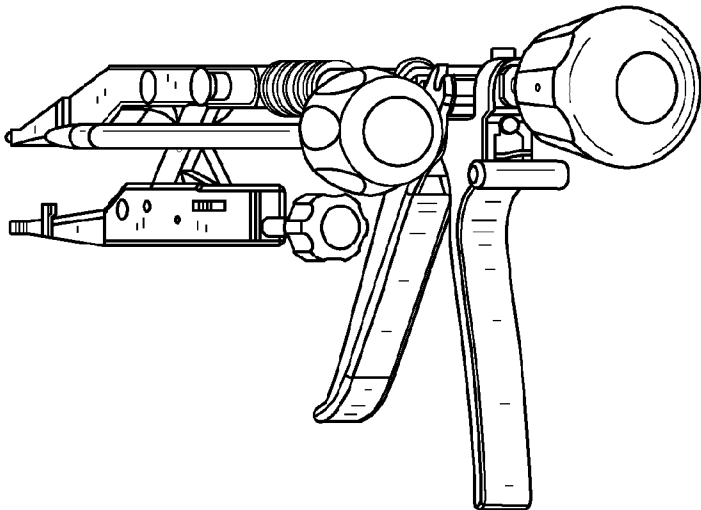

14/19

FIG. 10A

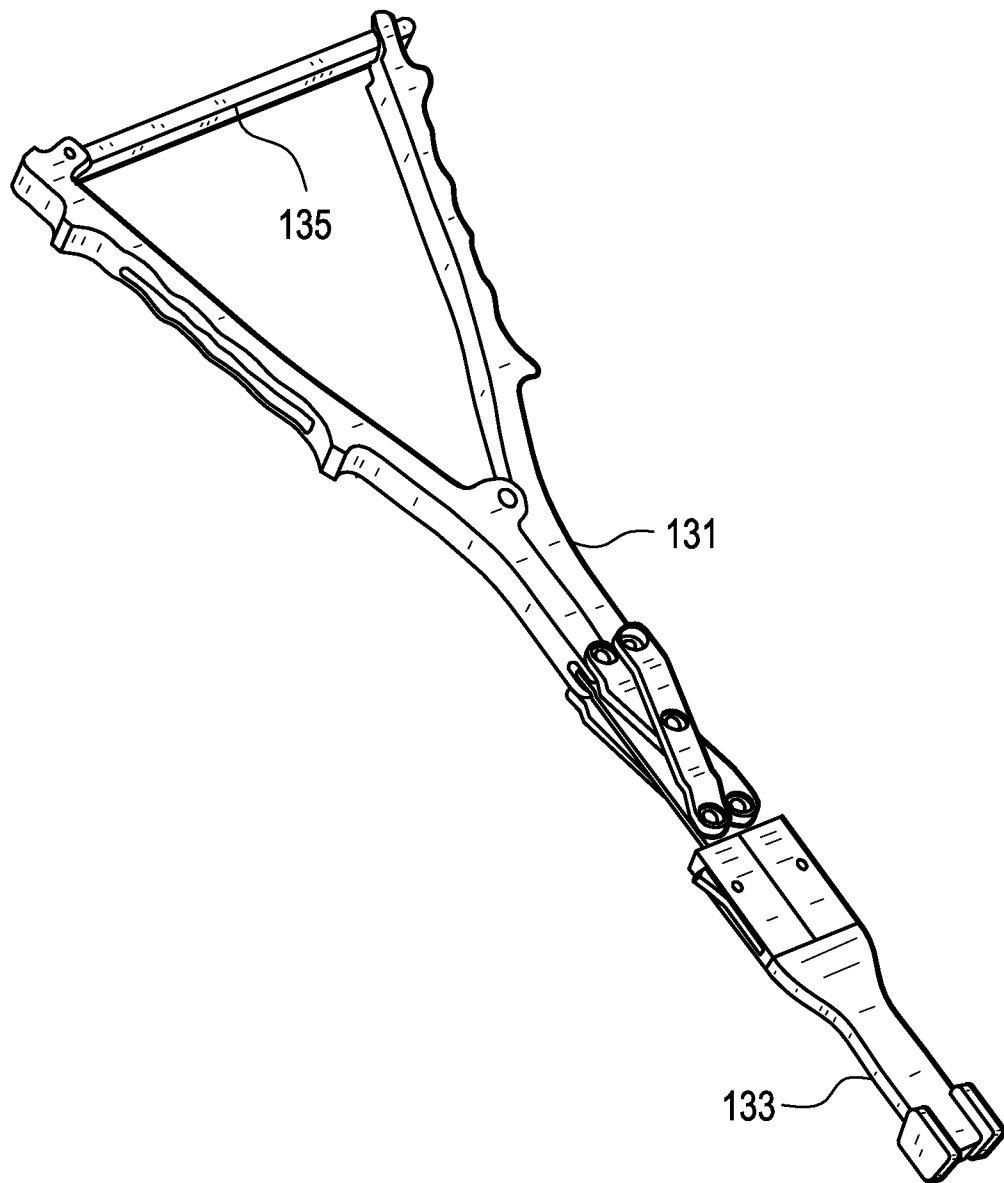

15/19

FIG. 10B



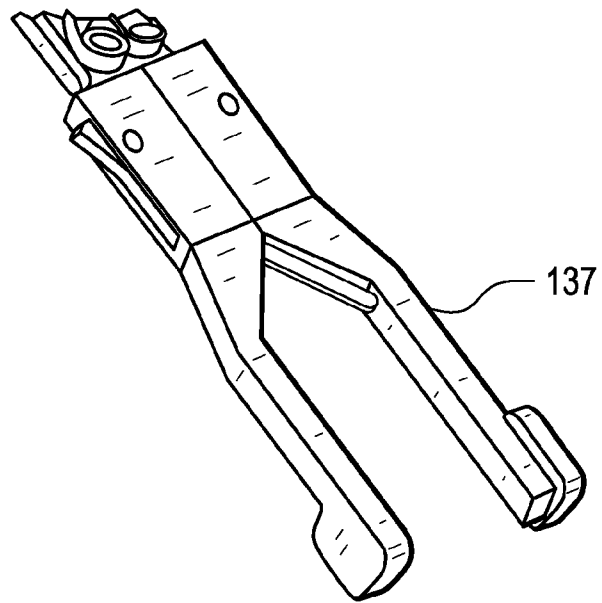


FIG. 10C

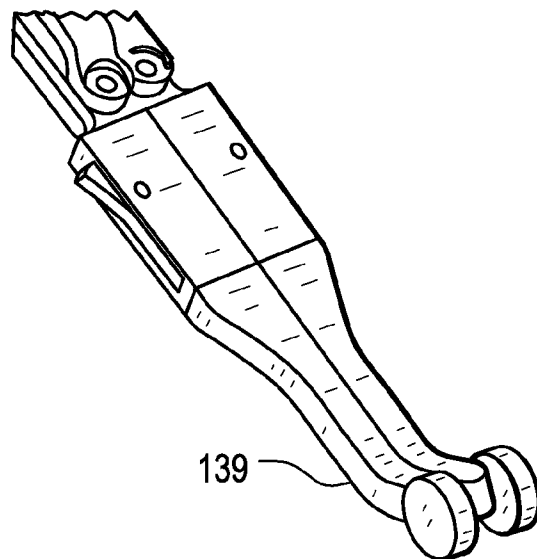

16/19

FIG. 11

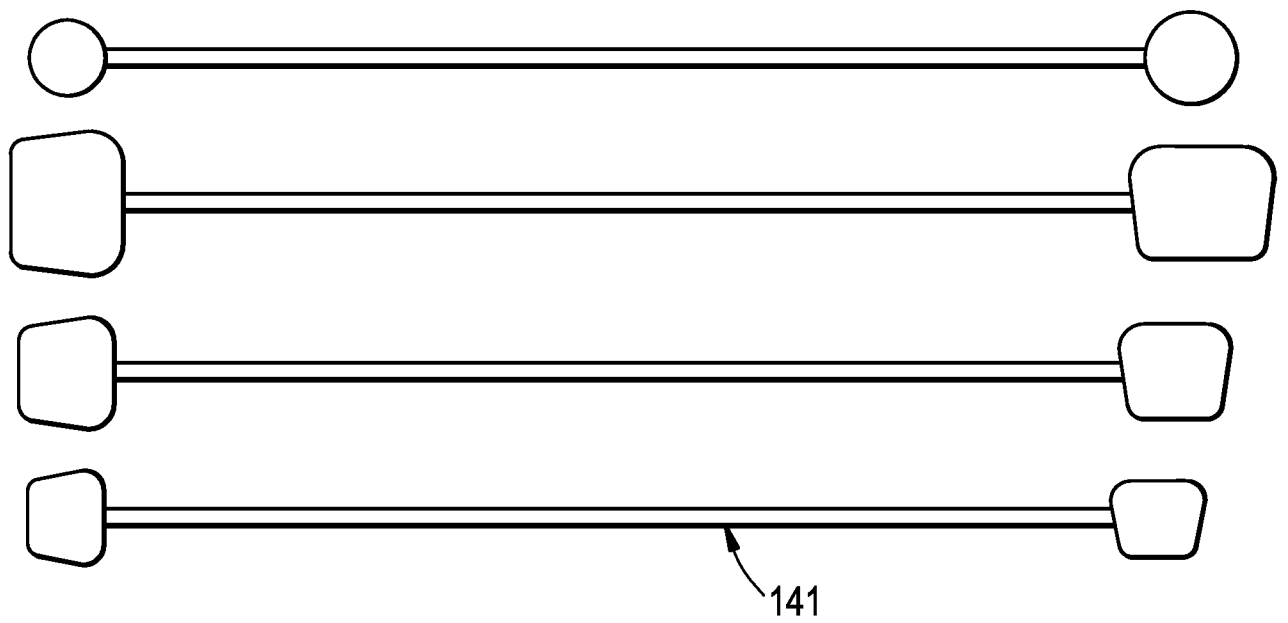

17/19

FIG. 12


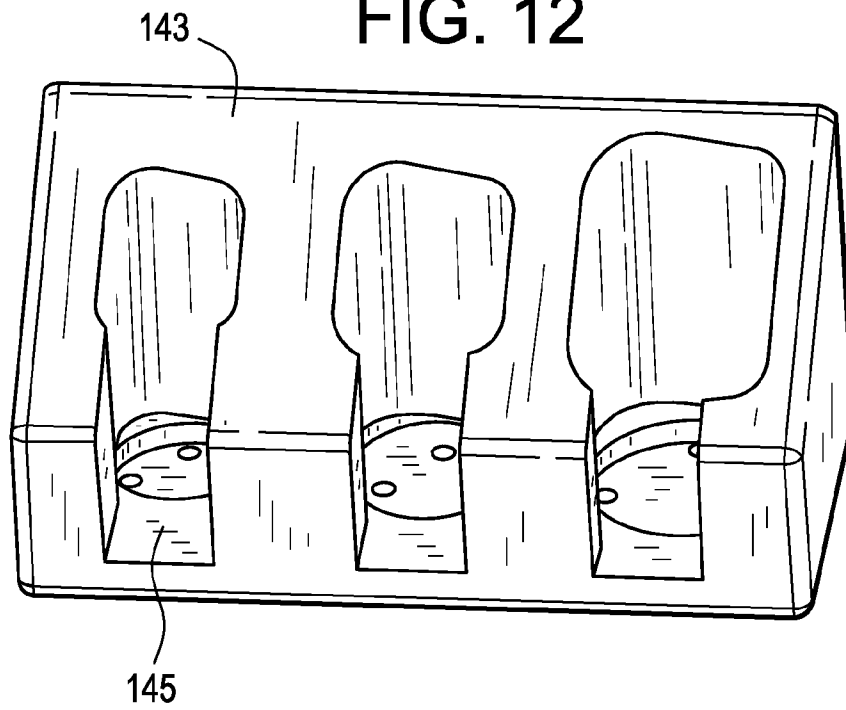


FIG. 13

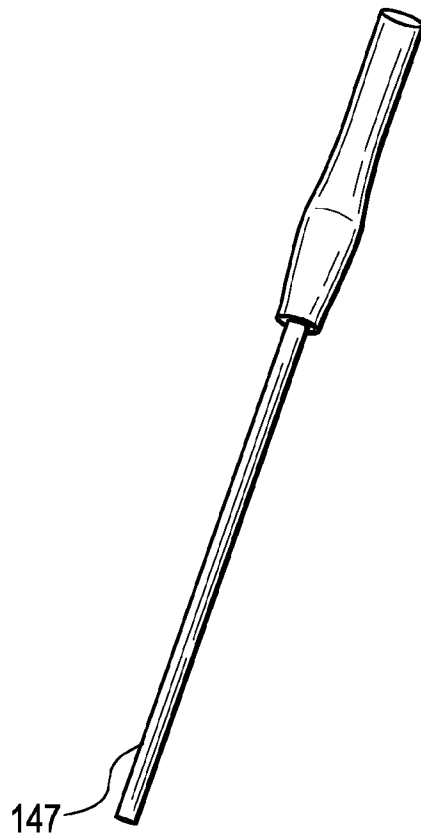

18/19

FIG. 14

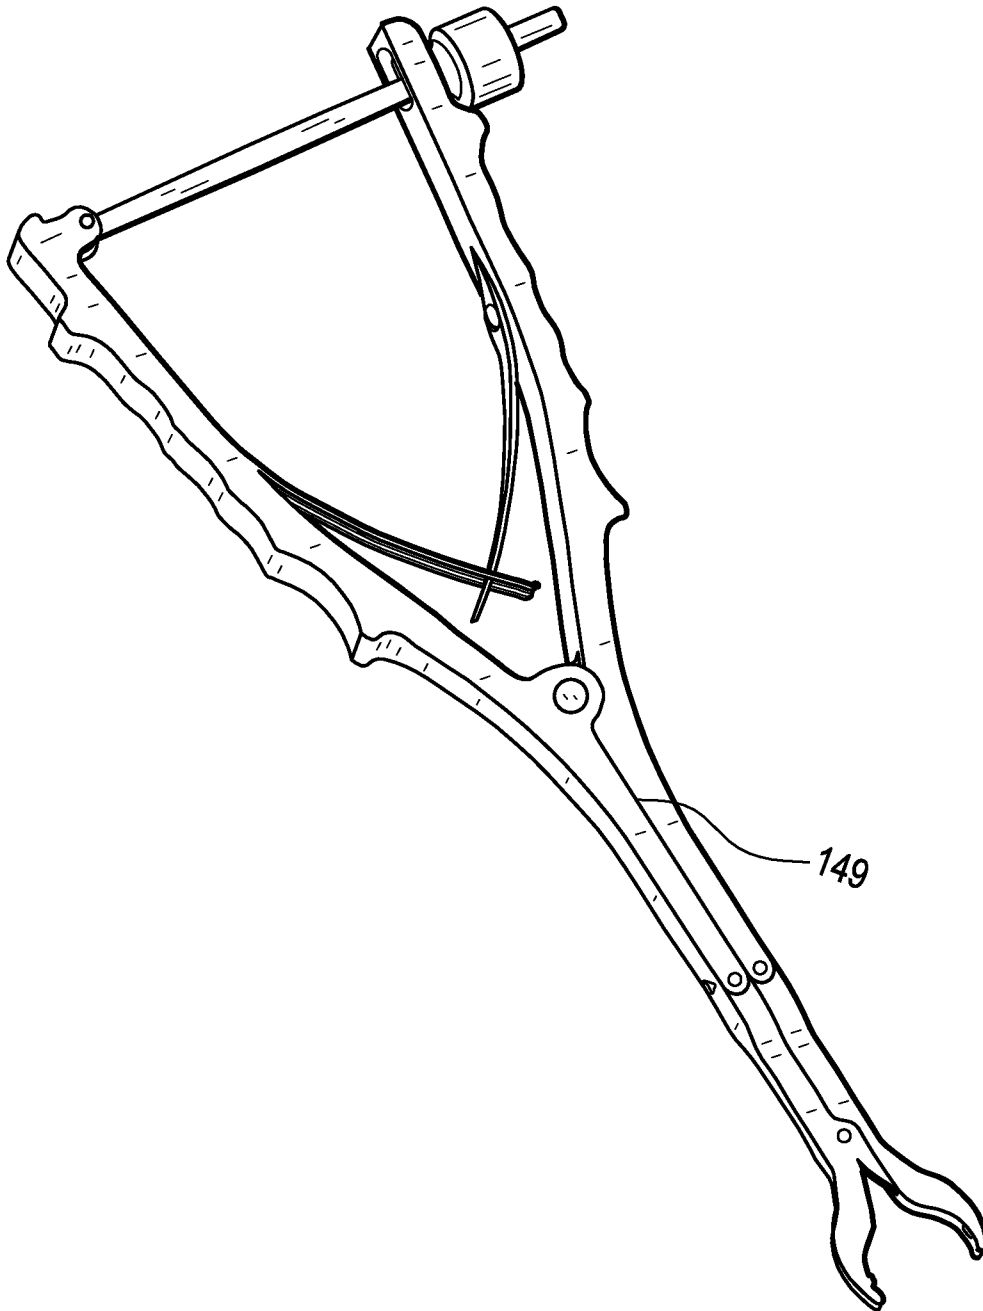


FIG. 15A


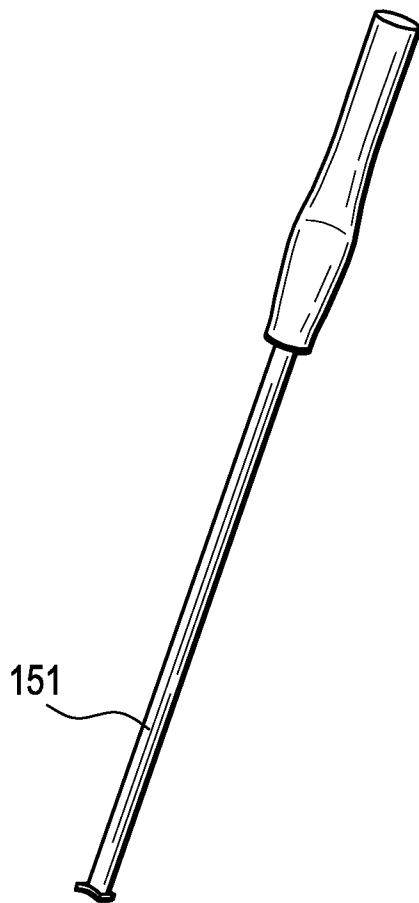


FIG. 15B

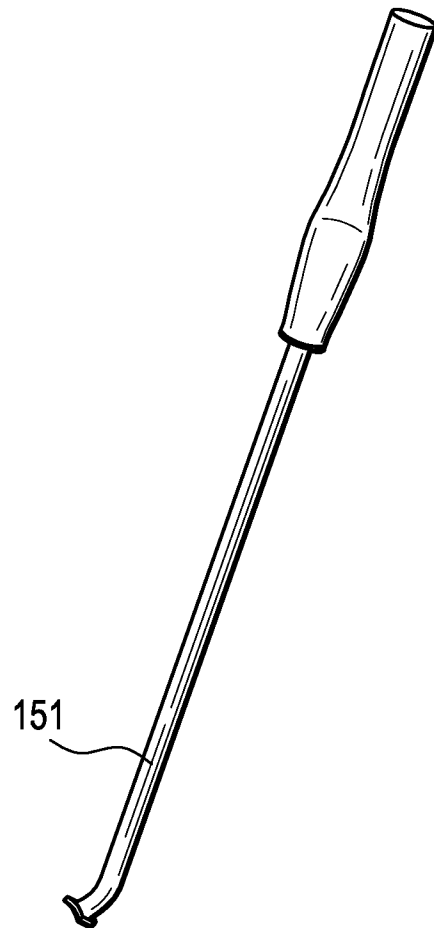

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 08/86977

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61F 2/44 (2009.01)

USPC - 623/17.16

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8): A61F 2/44 (2009.01)

USPC: 623/17.16

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

IPC(8): A61F 2/44; A61F 2/28; A61F 2/30 (2009.01)

USPC: 623/17.16; 623/16.11, 17.11, 17.15

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

USPTO WEST (USPT, PGPUB, EPAB, JPAB)

Google Scholar

spacer, verteb\$, height, adjust\$, ratchet, notch, pin, collar, slid\$, plate, screw, expandable, fusion, cage

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X — Y	US 2007/0123987 A1 (BERNSTEIN) 31 May 2007 (31.05.2007), [Abstract], para[0004], [0015], [0032], Figs. 1, 2	1, 10 2-9, 11-21
Y	US 6,200,348 B1 (BIEDERMANN, et al.) 13 March 2001 (13.03.2001), [Abstract], col 3, ln 42-44; Figs. 4, 9, 13	2-9, 20
Y	US 2006/0217712 A1 (MUELLER, et al.) 28 September 2006 (28.12.2006), para[0112]	9, 21
Y	US 2005/0101960 A1 (FIERE, et al.) 12 May 2005 (12.05.2005), Figs. 1, 2	11-21

☐

Further documents are listed in the continuation of Box C.

☐

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

20 January 2009 (29.01.2009)

Date of mailing of the international search report

05 FEB 2009

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-3201

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774