



US006056769A

United States Patent [19]

Epstein et al.

[11] Patent Number: **6,056,769**
[45] Date of Patent: **May 2, 2000**

[54] **EXPANSILE DEVICE FOR USE IN BLOOD VESSELS AND TRACTS IN THE BODY AND TENSION APPLICATION DEVICE FOR USE THEREWITH AND METHOD**

5,861,003 1/1999 Latson et al. 606/213

OTHER PUBLICATIONS

Oct. 19, 1999, PCT Search Report, US99/17367.
Oct. 29, 1999, PCT Search Report, US99/17372.

[75] Inventors: **Gordon H. Epstein**, Fremont; **Todd E. Lempert**, Piedmont; **Brian B. Martin**, Boulder Creek; **David M. Taylor**, Fremont, all of Calif.

Primary Examiner—Michael Buiz
Assistant Examiner—Vikki Trinh
Attorney, Agent, or Firm—Flehr Hohbach Test Albritton & Herbert

[73] Assignee: **BioInterventional Corporation**, Pleasanton, Calif.

[57] ABSTRACT

[21] Appl. No.: **09/126,969**
[22] Filed: **Jul. 31, 1998**

A device for expansion within a blood vessel having a wall defining a lumen in the body. A first elongate tubular member has proximal and distal extremities and has a longitudinal axis. An expansile member is carried by the distal extremity of the first elongate tubular member and is movable between contracted and expanded positions. The expansile member has a predetermined configuration in the expanded position. A deformable membrane covers the expansile member, and is sized so as to be capable of overlying and underlying the expansile member in the expanded position. A deployment mechanism is carried by the proximal extremity of the first elongate tubular member and is adapted to be operated by the human hand for controlling movement of the expansile member between the contracted and expanded positions. A deployment mechanism includes a push-pull wire with proximal and distal extremities and extends through the first elongate tubular member and is coupled to the expansile member.

Related U.S. Application Data


[63] Continuation-in-part of application No. 08/972,383, Nov. 18, 1997, Pat. No. 5,922,009, which is a continuation-in-part of application No. 08/798,870, Feb. 11, 1997, Pat. No. 5,782,860.
[51] **Int. Cl.⁷** **A61B 17/08**
[52] **U.S. Cl.** **606/213**
[58] **Field of Search** 606/213-215, 606/151, 157


[56] References Cited

U.S. PATENT DOCUMENTS

5,258,000 11/1993 Gianturco 606/151
5,383,896 1/1995 Gershony et al. 606/213

18 Claims, 12 Drawing Sheets

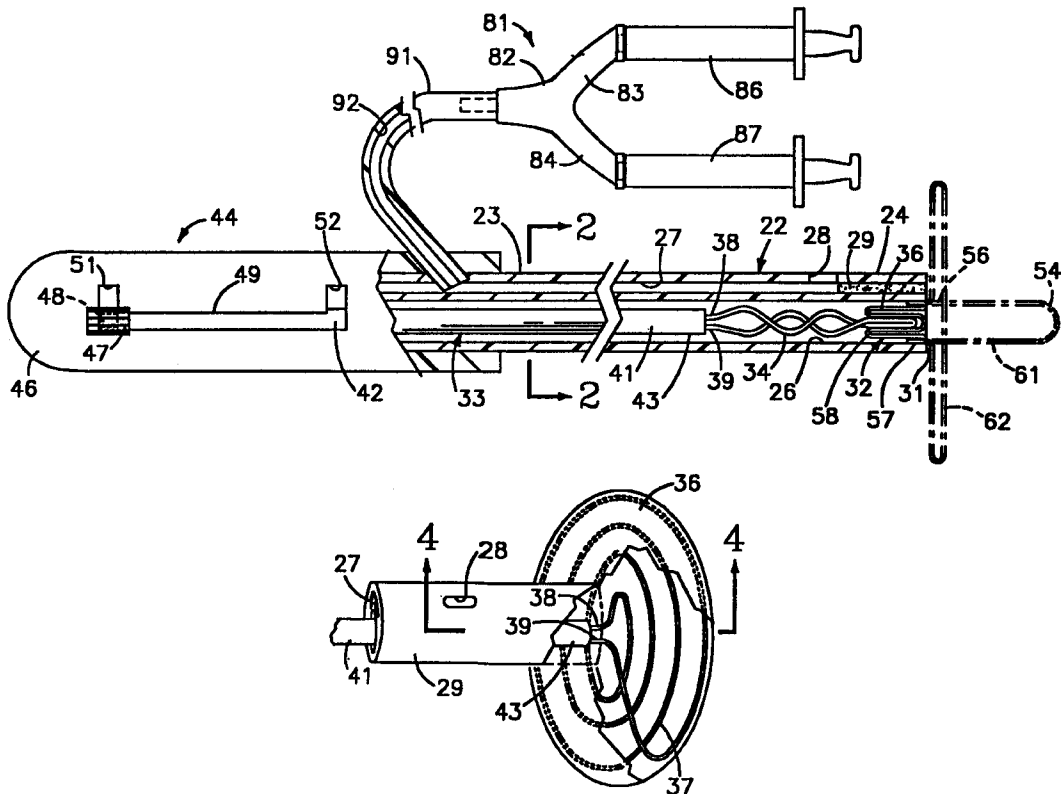

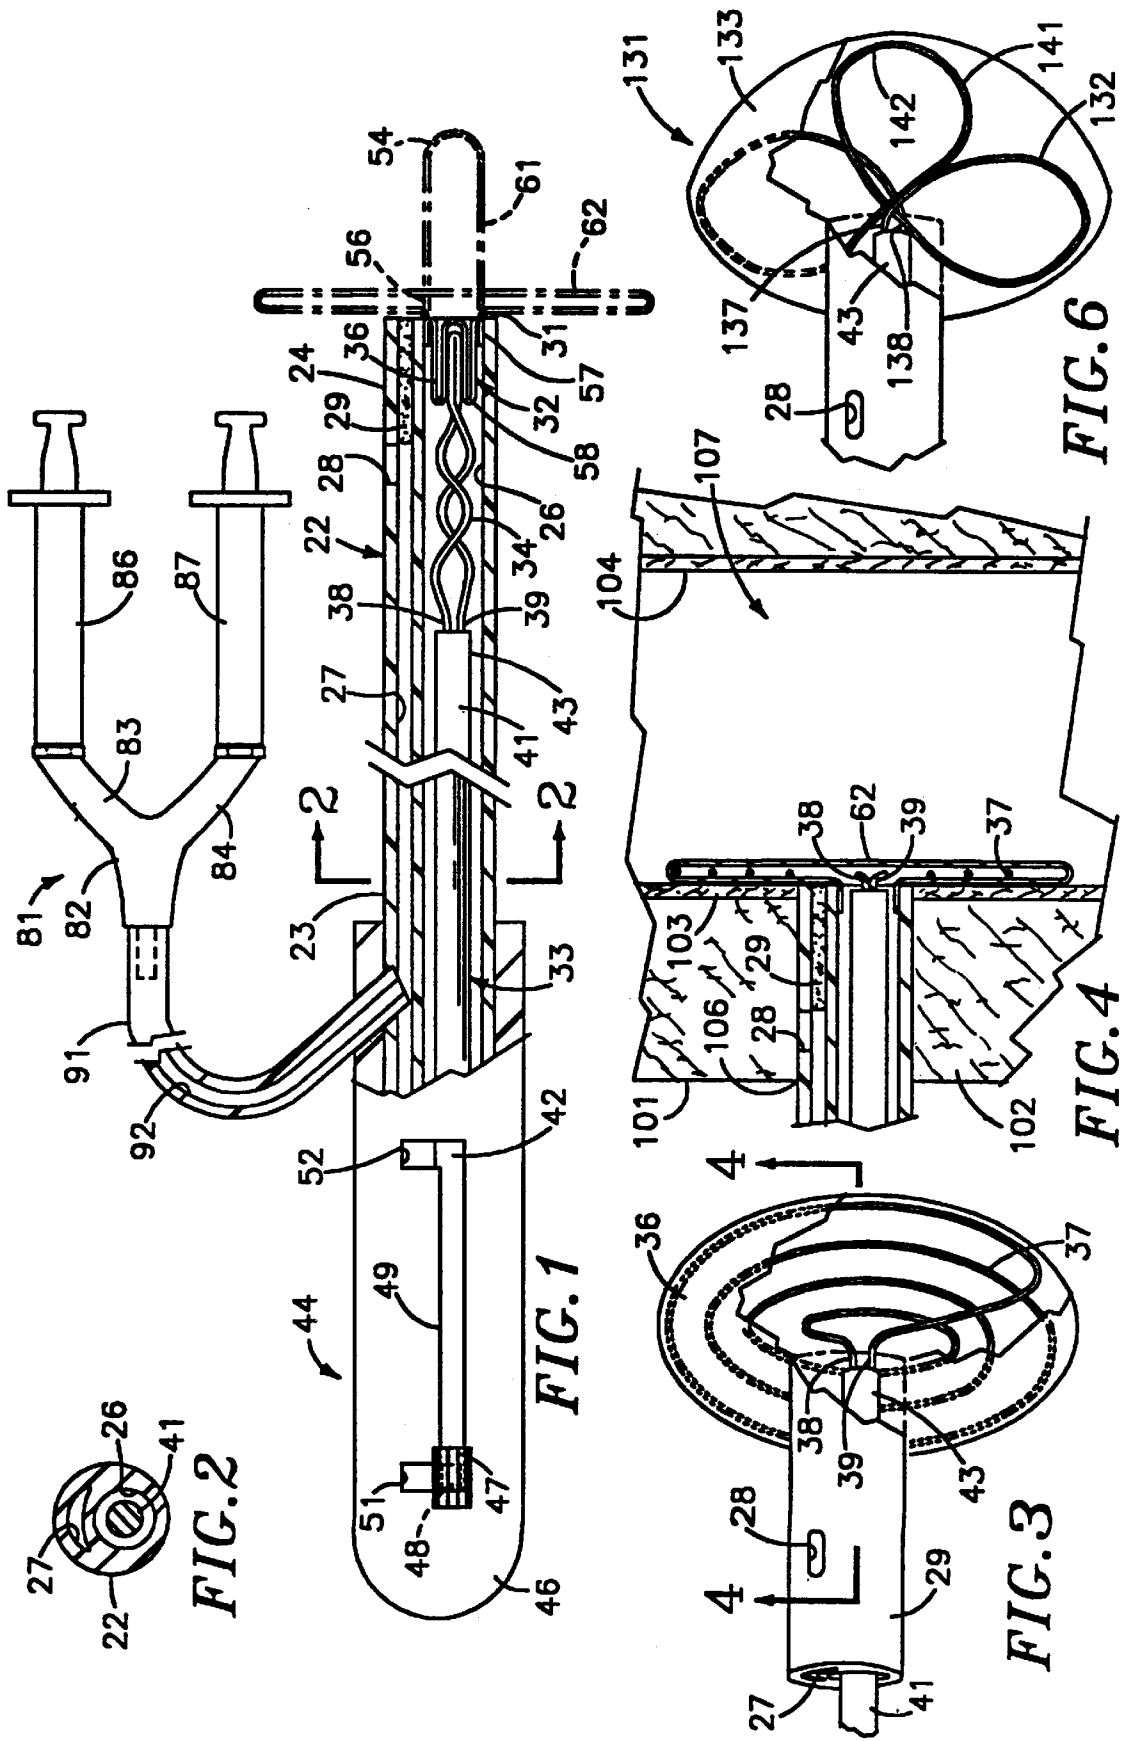

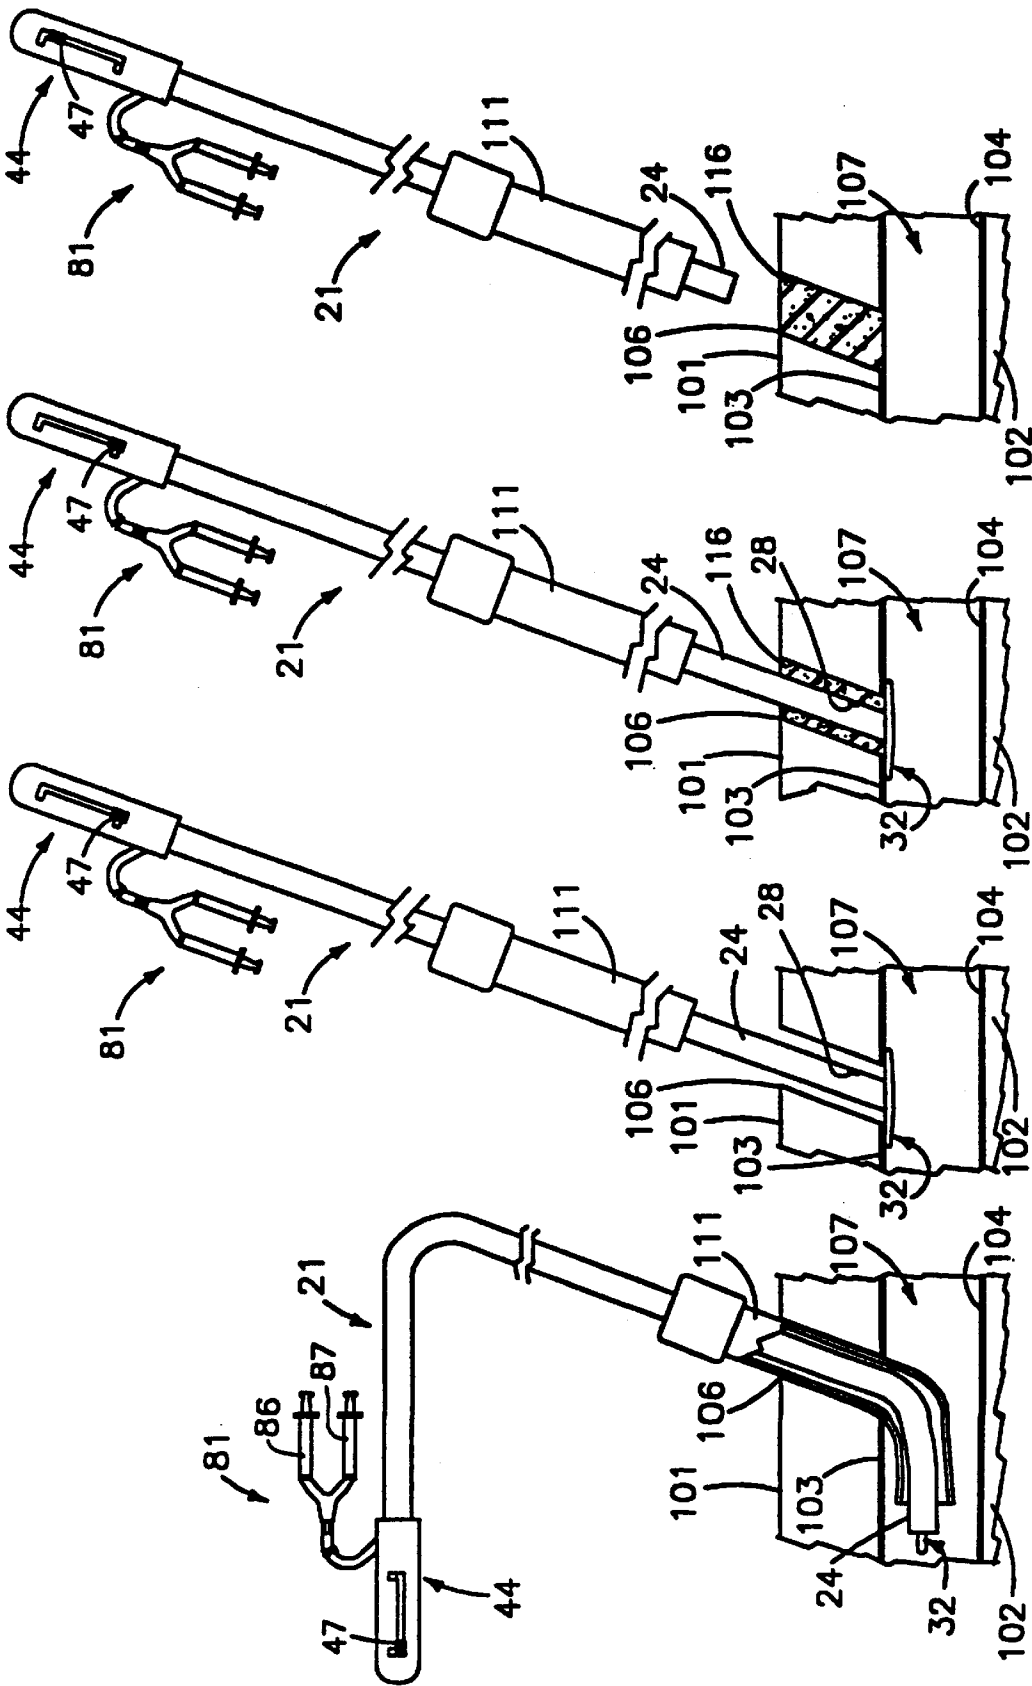
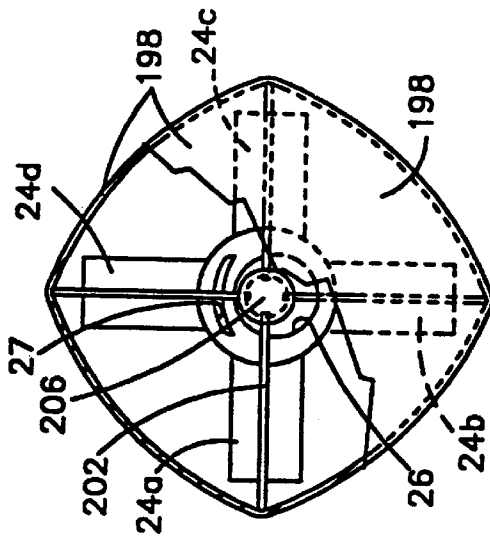
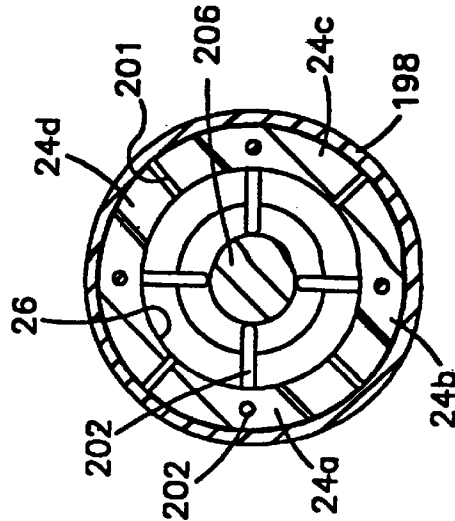
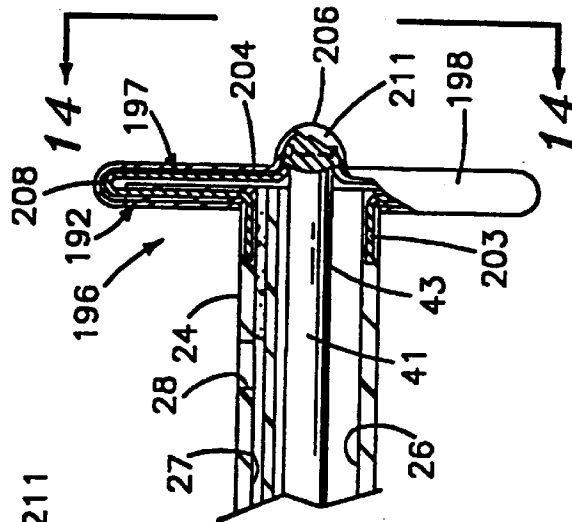
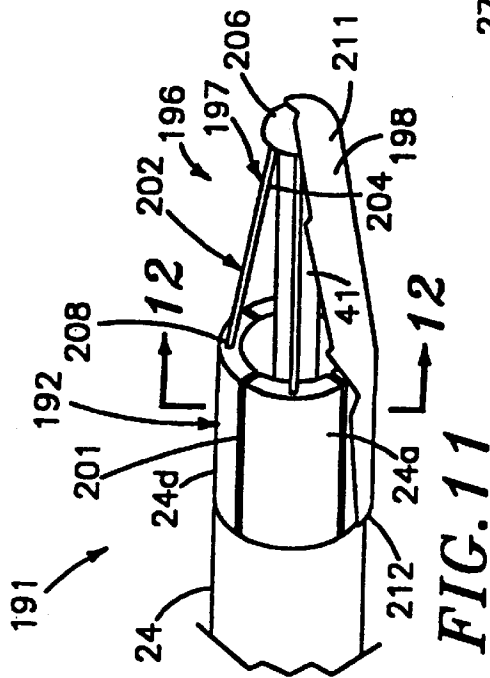






FIG. 5D

FIG. 5C

FIG. 5B

FIG. 5A



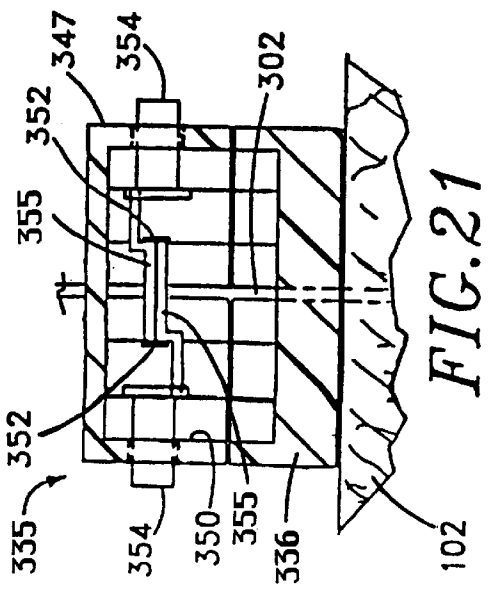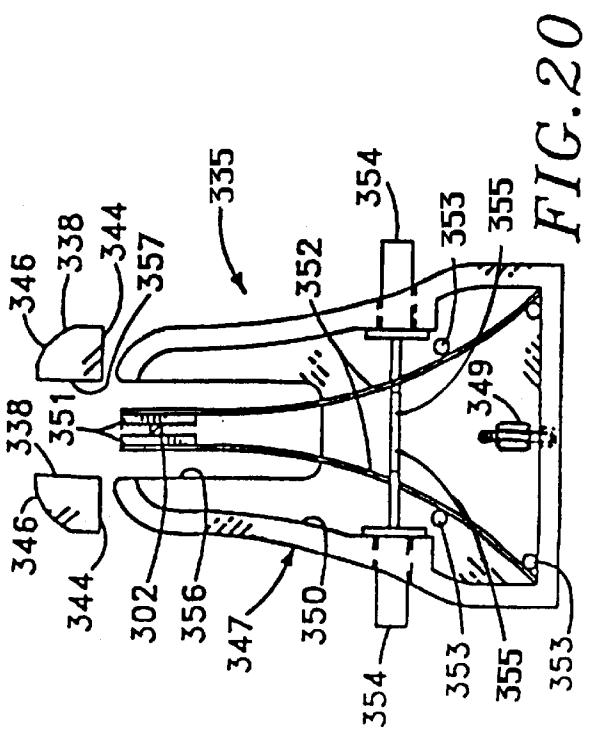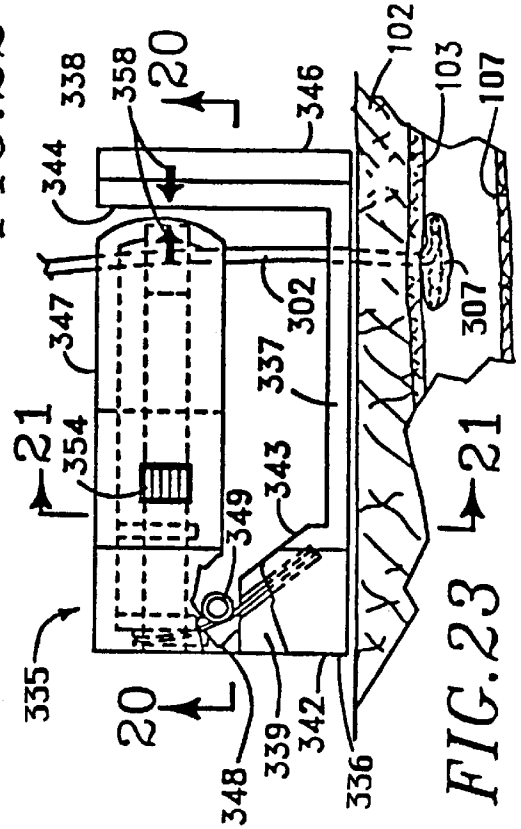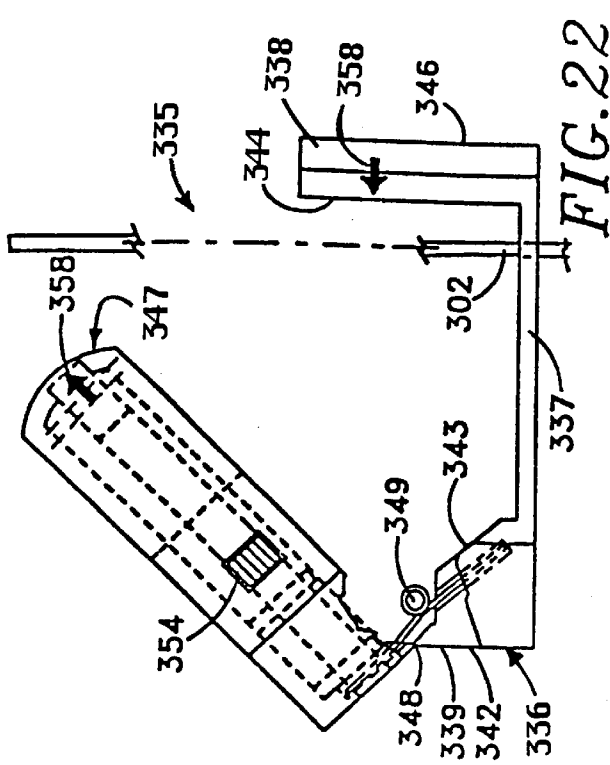

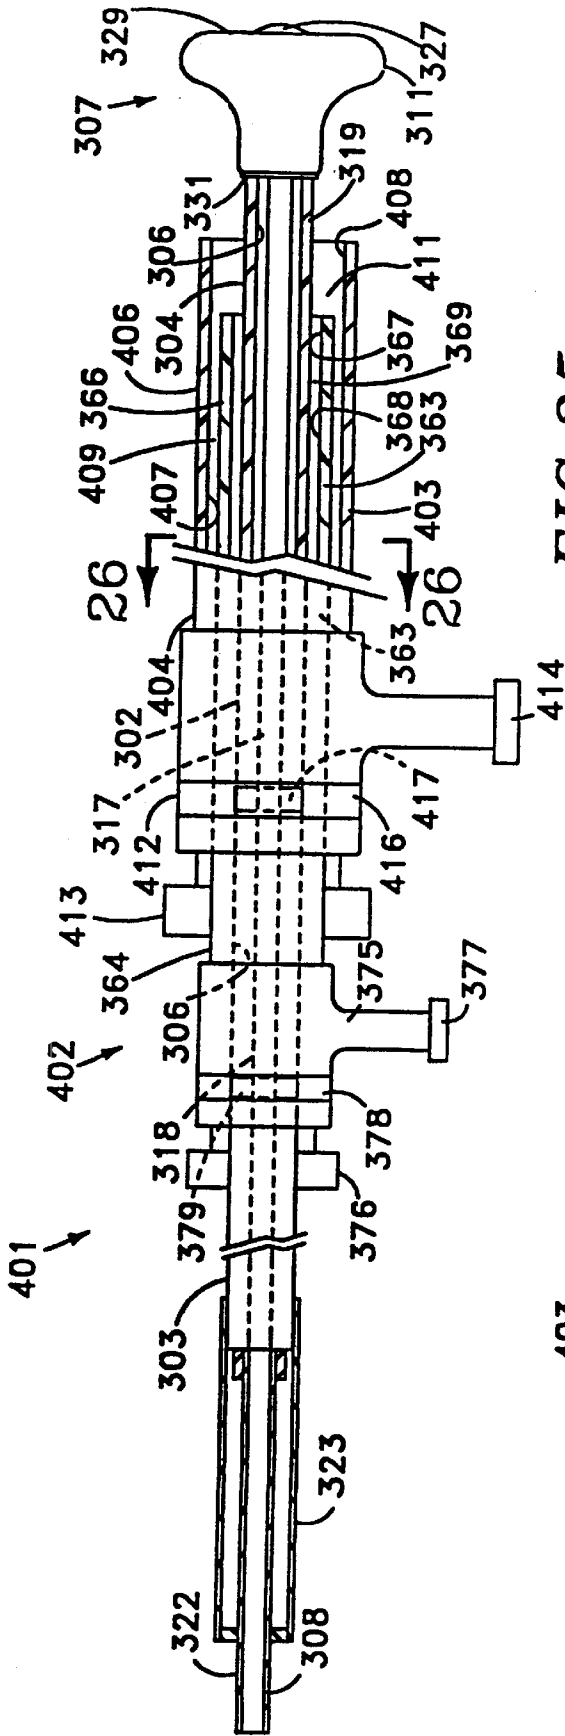


FIG. 25

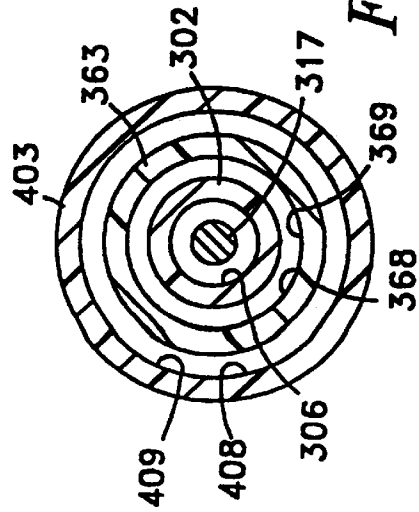


FIG. 26

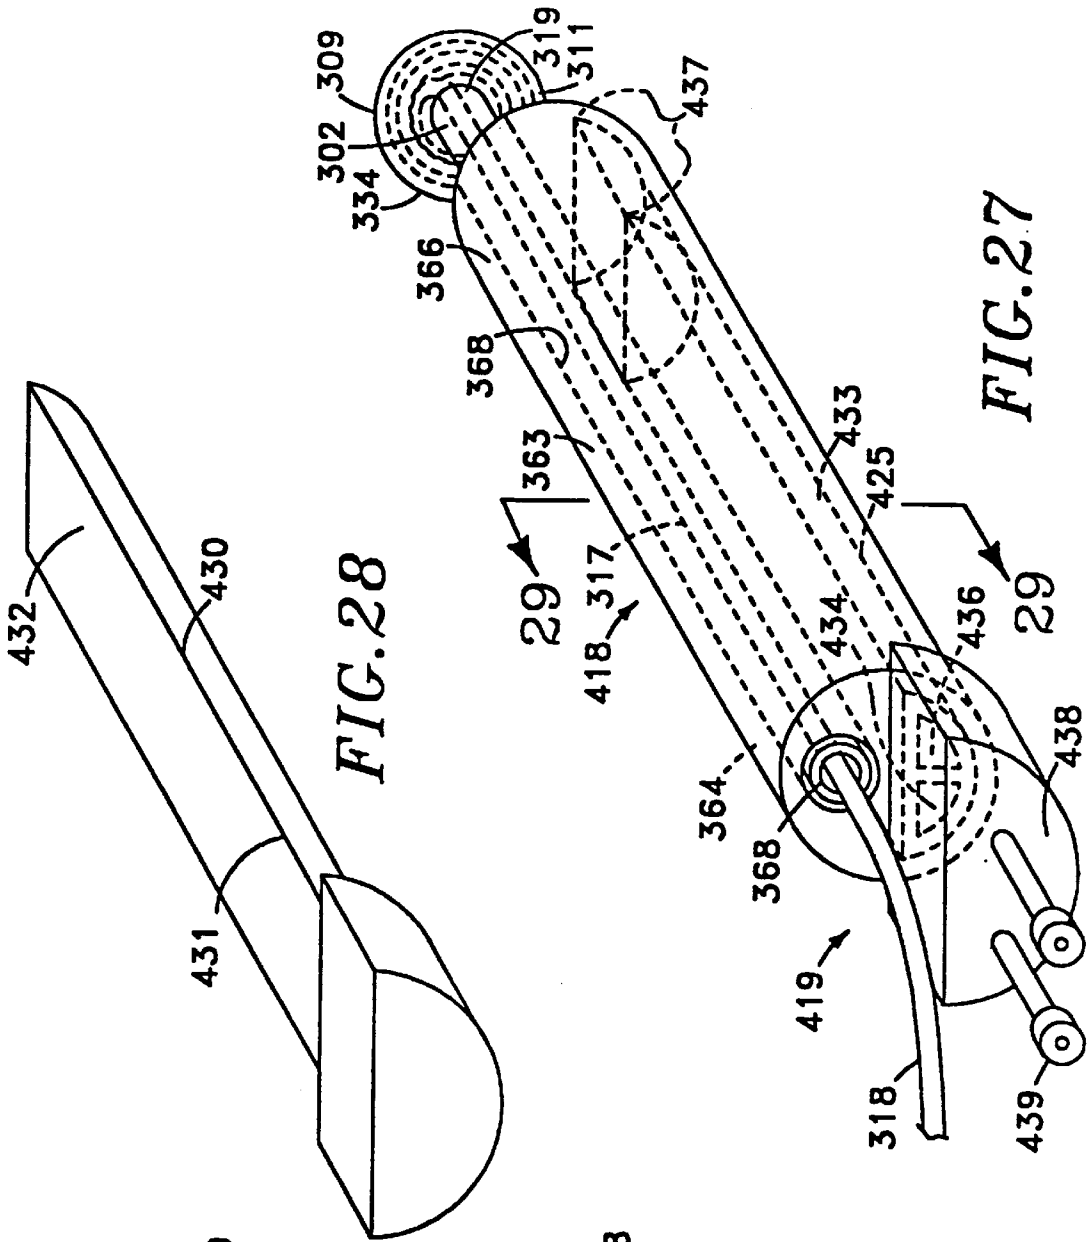


FIG. 27

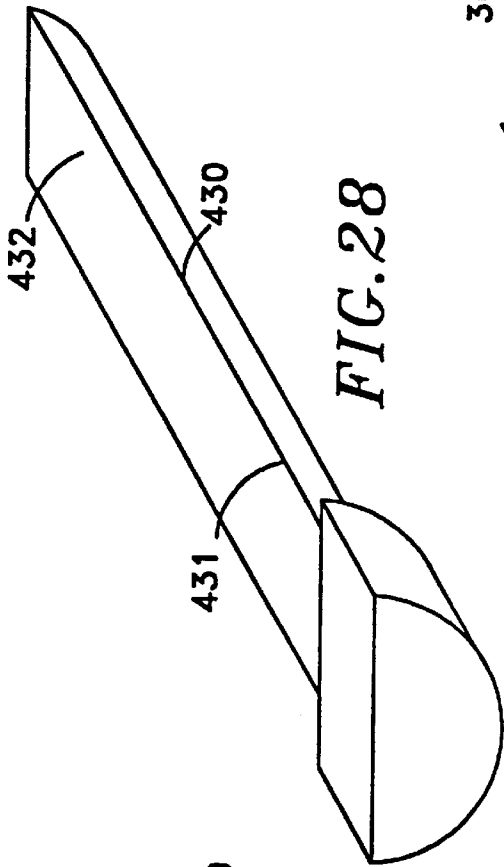


FIG. 28

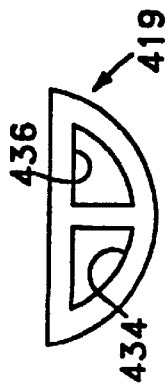


FIG. 30

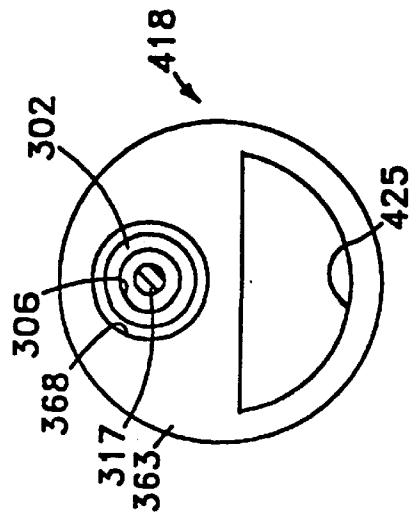
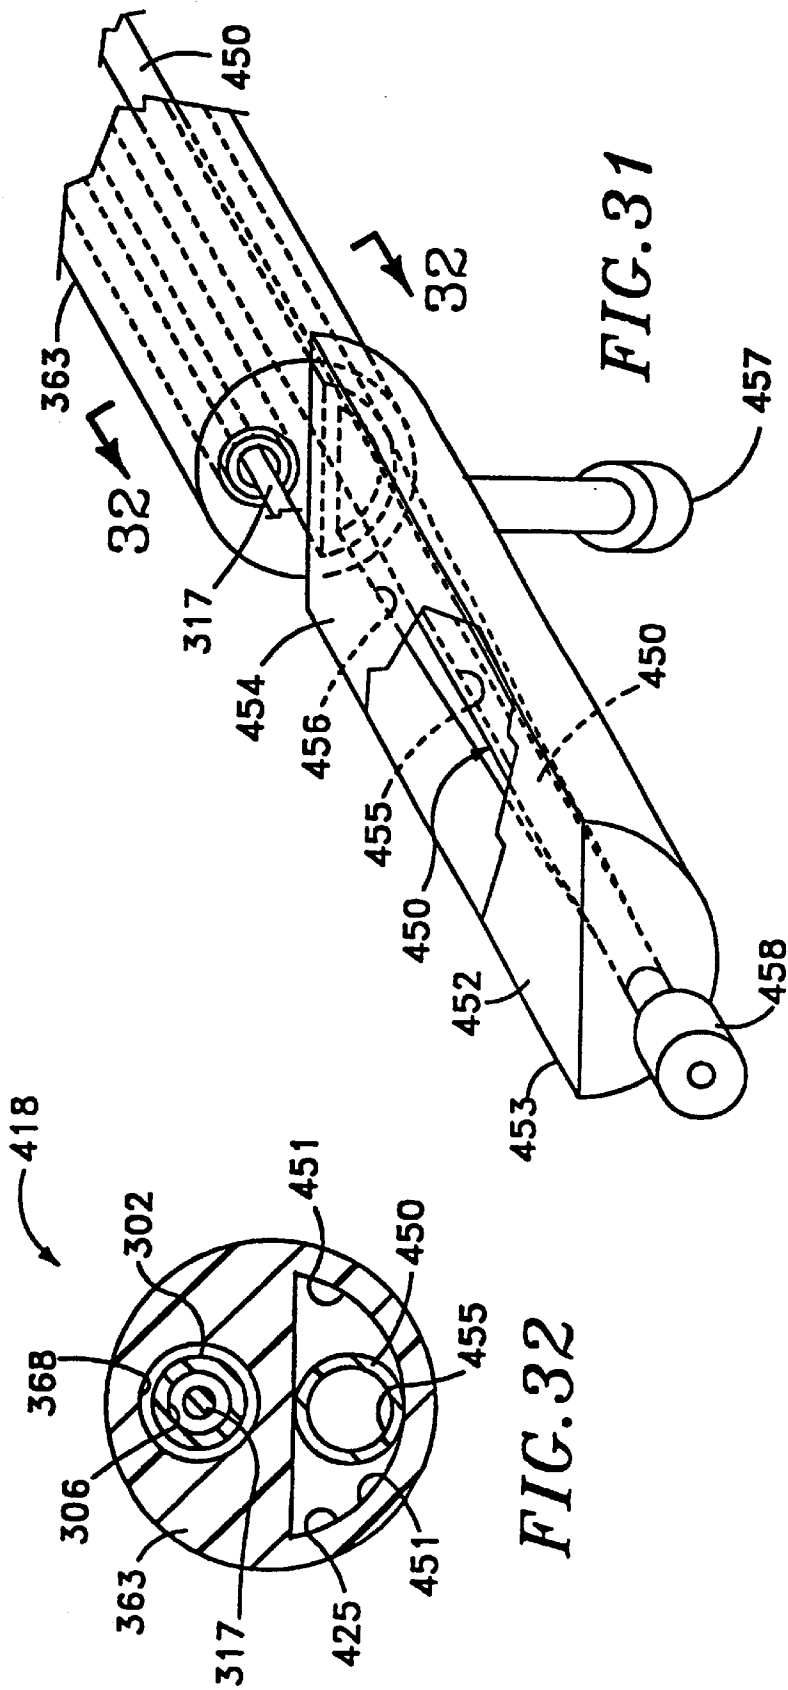


FIG. 29



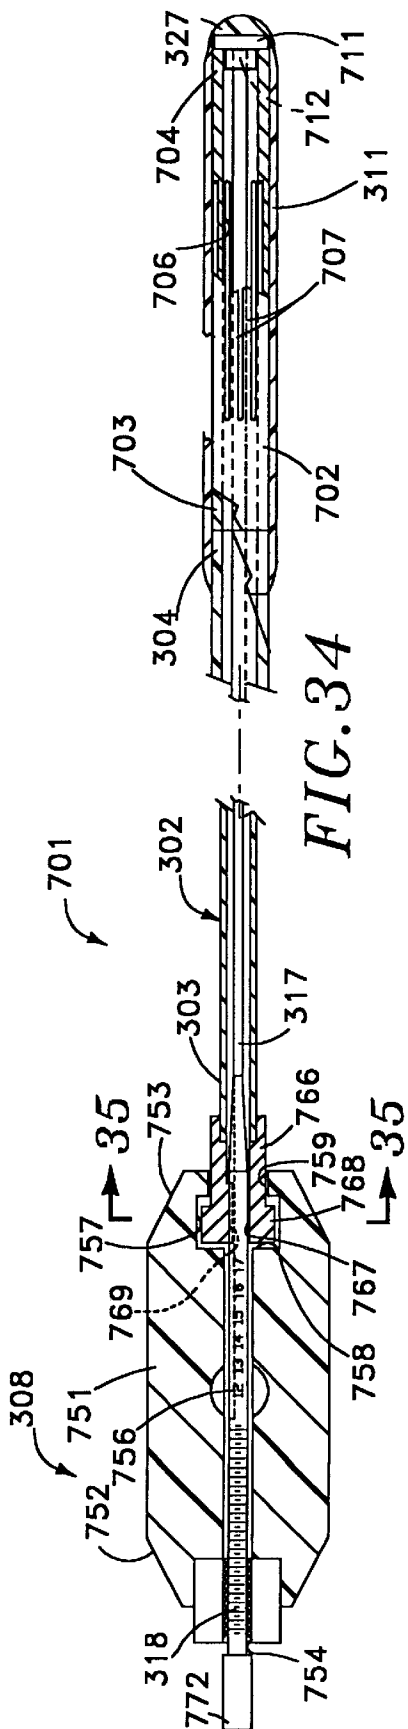


FIG. 34

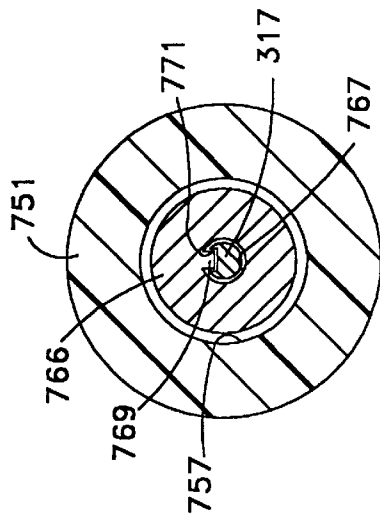


FIG. 35

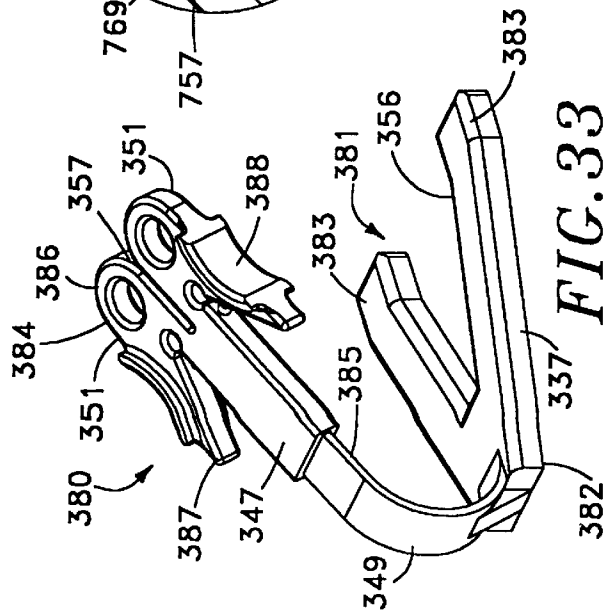


FIG. 33

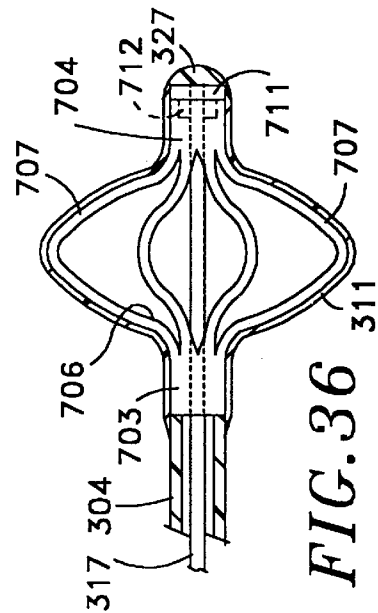


FIG. 36

**EXPANSILE DEVICE FOR USE IN BLOOD
VESSELS AND TRACTS IN THE BODY AND
TENSION APPLICATION DEVICE FOR USE
THEREWITH AND METHOD**

This is a continuation-in-part of prior application Ser. No. 08/972,383, filed Nov. 18, 1997 now U.S. Pat. No. 5,922,009 which is a continuation-in-part of application Ser. No. 08/798,870, filed Feb. 11, 1997 which issued as U.S. Pat. No. 5,782,860 on Jul. 21, 1998.

This invention relates to an expansile device and tension application device for use therewith, for use in vascular and non-vascular tracts in the human body and method and more particularly for percutaneous occlusion of vascular access sites in the human body.

Percutaneous access to the blood vessels and organs of the human body for diagnosis and treatment of disease processes has heretofore been accomplished. Percutaneous vascular procedures are performed involving the coronary, peripheral and cerebral vasculature. These procedures include coronary and peripheral angiography, angioplasty, atherectomies, coronary retroperfusion and retroinfusion, cerebral angiograms, treatment of strokes, cerebral aneurysms and the like. Patients undergoing such procedures are often treated with anti-platelet drugs, anticoagulants such as heparin, thrombolytics, or a combination thereof, all of which interfere with coagulation making it more difficult for the body to seal a puncture site. Various devices and methods have heretofore been utilized, however, they all have had deficiencies, including the use of complicated devices and methods. In addition, difficulties are still encountered in obtaining good seals. There is therefore a need for a device and method for percutaneous access and occlusion of vascular access sites and other puncture sites and natural tracts in the human body which overcome the deficiencies of prior art devices and methods.

In general, it is an object of the present invention to provide a closure device and method for percutaneous access and occlusion of vascular access sites, other puncture sites and natural tracts in the human body which will make possible a positive seal of the puncture site or tract promoting rapid healing of the puncture site or tract.

Another object of the invention is to provide a closure device and method of the above character which can be easily and reliably used.

Another object of the invention is to provide a closure device and method of the above character in conjunction with which a biological sealant is used by introduction into the puncture site or natural tract.

Another object of the invention is to provide a closure device and method of the above character which leaves a small enough opening after removal of the closure device so that the biological sealant will seal the remaining opening.

Another object of the invention is to provide a closure device and method of the above character which enables continued substantially unobstructed blood flow during deployment and use of the closure device.

Another object of the invention is to provide a closure device and method of the above character in which no foreign body remains in the blood vessel.

Another object of the invention is to provide a closure device and method of the above character that permits early ambulation of patients and avoids prolonged bed rest.

Another object of the invention is to provide a closure device and method of the above character which reduces the risk of bleeding, formation of arteriovenous fistula, formation of pseudoaneurysm, thrombosis with distal embolization and infection.

Another object of the invention is to provide a closure device and method of the above character that reduces the risk of causing ischemia of an extremity.

Another object of the invention is to provide a closure device and method of the above character that is inexpensive, quick, safe, easy to use and is disposable.

Another object of the invention is to provide an expansile device and method of the above character in which the configuration of an expansile assembly is determined by countervailing mechanical forces of an expansile member and a membrane.

Another object of the invention is to provide an expansile device and method of the above character in which tensioning means is provided for reversibly maintaining engagement of the expansile assembly against the vessel wall of a puncture and to free the operator's hands from having to hold the device after it is correctly deployed in the puncture.

Another object of the invention is to provide an expansile device and method of the above character in which tensioning means is provided for reversibly maintaining engagement of the expansile assembly against the vessel wall of a puncture by applying a substantially constant force of tension over a range of motion.

Another object of the invention is to provide an expansile device and method of the above character in which the expansile member is capable of being expanded to different sizes and configurations.

Another object of the invention is to provide an expansile device and method of the above character with which the operator is capable of confirming the size to which the expansile member is expanded.

Another object of the invention is to provide an expansile device and method of the above character in which tensioning means is provided for reversibly maintaining engagement of the expansile assembly against the vessel wall of a puncture by applying a varying force of tension over a range of motion.

Additional objects and features of the invention will appear from the following description in which the preferred embodiments and the methods using the same are described in conjunction with the accompanying drawings.

FIG. 1 is a side-elevation view partially in section of a closure device for obtaining percutaneous access and occlusion of puncture sites in the human body incorporating the present invention and having closure means in a de-deployed or retracted position.

FIG. 2 is a cross-sectional view taken along the line 2—2 of FIG. 1.

FIG. 3 is a side-elevation isometric view of the distal end of the device shown in FIG. 1 with the closure means in a deployed or extended position.

FIG. 4 is a cross-sectional view taken along the line 4—4 of FIG. 3 and shows the manner in which a seal is formed with respect to a puncture.

FIGS. 5A—5D are cartoons demonstrating the method of using the device of the present invention for occluding a vascular access or puncture site.

FIG. 6 is a partial isometric view of an alternative closure assembly for the closure device shown in FIG. 1.

FIG. 7 is a side-elevation view partially in section of another embodiment of the closure device incorporating the present invention.

FIG. 8 is a cross-sectional view taken along the line 8—8 of FIG. 7.

FIG. 9 is a cross-sectional view taken along the line 9—9 of FIG. 8.

FIG. 10 is a side-elevation isometric view of the distal end of the device of FIG. 8 with the closure assembly in a deployed or expanded position.

FIG. 11 is a side-elevational view partially in section of another embodiment of the closure device incorporating the present invention.

FIG. 12 is a cross-sectional view taken along the line 12—12 of FIG. 11.

FIG. 13 is a partial side-elevational view of the distal extremity of the closure device of FIG. 11 with the closure mechanism in a deployed position.

FIG. 14 is a view looking along the line 14—14 of FIG. 13.

FIG. 15A is a side-elevational view partially in section of the proximal end of another embodiment of the closure device incorporating the present invention.

FIG. 15B is a side-elevational view partially in section of the distal end of the embodiment shown in FIG. 15A.

FIG. 16 is a side-elevational view partially in section of the distal end of the device of FIG. 15 with the closure assembly in a deployed position.

FIG. 17 is a view partially in section taken along the line 17—17 of FIG. 16.

FIG. 18 is a side-elevational view partially in section of another embodiment of the closure or expansile device incorporating the present invention.

FIG. 19 is a side-elevational view partially in section of the distal end of the device of FIG. 18 with the expansile assembly in an free or expanded position without the covering membrane.

FIG. 20 is an plan view of the top of the tensioning device of the present invention taken along the line 20—20 of FIG. 23.

FIG. 21 is a cross-sectional view taken along the line 21—21 of FIG. 23.

FIG. 22 is a side-elevational view partially in section of the tensioning device of the present invention in the open position.

FIG. 23 is side-elevational view partially in section of the tensioning device of the present invention in the closed, neutral position.

FIG. 24 is a cross-sectional view of the device of FIG. 18 with one embodiment of the biological sealant introducing means.

FIG. 25 is an side-elevational view partially in section of another embodiment of the expansile device of the present invention shown with its biological sealant introducing means.

FIG. 26 is a cross-sectional view taken along the line 26—26 of FIG. 25.

FIG. 27 is an isometric view of the device in FIG. 18 with another embodiment of the biological sealant introducing means.

FIG. 28 is an isometric view the third elongate member that obturates the second lumen in the biological sealant introducing means of FIG. 27.

FIG. 29 is a cross section view taken along the line 29—29 of FIG. 27.

FIG. 30 is a cross-sectional view of another embodiment of the third elongate tubular member which is part of the biological sealant introducing means of FIG. 27.

FIG. 31 is an isometric view of the device in FIG. 18 with another embodiment of the biological sealant introducing means.

FIG. 32 is a cross-section view taken along the line 32—32 of FIG. 30.

FIG. 33 is an isometric view of another embodiment of the tensioning device of the present invention in the open position.

FIG. 34 is a side elevational view partially in section of another embodiment of the closure device incorporating the present invention in the contracted position.

FIG. 35 is a sectional view taken along the line 35—35 of FIG. 34.

FIG. 36 is a side elevational view partially in section of the distal extremity, including the expansile member, of the device in FIG. 34 shown in the expanded position.

In general, the closure device of the present invention is used for the percutaneous occlusion of a puncture site and natural tract in the human body. The human body has an outer layer of skin and inner layers of tissue surrounding a blood vessel having a lumen therein defined by a vessel wall. A puncture site traverses these layers and, in the case of a vascular access puncture, the vessel wall. The closure device comprises a flexible elongate tubular member having proximal and distal extremities, an outer diameter and extending along a longitudinal axis. The flexible elongate tubular member has a first lumen extending therethrough from the proximal extremity to the distal extremity. A closure assembly is carried by the distal extremity and includes a closure mechanism and an impermeable membrane at least partially covering the closure mechanism. Deployment means carried by the proximal extremity of the flexible elongate tubular member are adapted to be operated by the human hand. The deployment means extends through the flexible elongate tubular member, includes a push-pull wire and is coupled to the closure assembly for moving the closure assembly from a de-deployed or contracted position for introduction into and through a puncture to a deployed position for forming a seal occluding the puncture.

More specifically, as shown in FIGS. 1—4, the closure device 21 of the present invention for percutaneous occlusion of puncture sites and natural tracts consists of a flexible elongate tubular member 22 formed of a suitable plastic material such as polyethylene or polyurethane or polyimide. The flexible elongate tubular member 22 has a longitudinal axis and proximal and distal extremities 23 and 24. The flexible elongate tubular member 22 is provided with a main circular in cross-section first lumen 26 which may be centrally disposed extending from the proximal extremity 23 to the distal extremity 24. It is also provided with an additional or second lumen 27 which may be crescent-shaped as shown in cross-section in FIG. 2 extending from the proximal extremity 23 to the distal extremity 24 where it opens through an external port 28. A plug 29 of a suitable material such as plastic is placed in the lumen 27 to occlude the lumen 27 distal of the port 28.

The flexible elongate tubular member 22 is of a suitable size, as for example a diameter ranging from 1—9 French corresponding to an outside diameter ranging from approximately 0.3 to 3.0 millimeters. The flexible elongate tubular member has a suitable length as for example 15—30 centimeters with the external port 28 being disposed a suitable distance adjacent to and proximal of the closure assembly 32, as for example from 1—10 millimeters up to several centimeters. The first lumen 26 may have an inside diameter ranging from 0.015" to 0.080", preferably 0.020"—0.030" while the second lumen 27, if crescent-shaped may have a long axis dimension of approximately 0.015" to 0.080".

Closure means in the form of a closure assembly 32 is carried by the distal extremity 24 of the flexible elongate tubular member 22 and is coupled or secured to deployment means or mechanism 33 for movement from a contracted, retracted or de-deployed position to an expanded or deployed position. The closure assembly 32 includes a closure mechanism 34 and an impervious membrane 36 which covers the closure mechanism 34. The closure mechanism 34 as shown in FIGS. 3 and 4 is in the form of a complex geometrical configuration, as for example a coil,

when in a free state. The coil **34** is formed of a suitable material which can be elongated without permanent deformation but when freed or unconstrained has a substantial portion thereof which will return to a generally planar or disk-like configuration to which it has been annealed. One material found to be particularly suitable for such an application is a super-elastic or shape memory element as formed of a nickel/titanium alloy, often called Nitinol. The coil **34** has a plurality of generally circular turns **37** and has first and second ends **38** and **39** secured to the deployment mechanism **33** in a manner hereinafter described. The turns **37** of the coil **34** lie in a single plane which is generally perpendicular to the longitudinal axis of the flexible elongate tubular member **22**.

The coil **34** has a diameter which is selected to overlap a puncture site as hereinafter described to occlude the puncture site. Typically, a suitable diameter such as 3 to 7 millimeters and preferably approximately 5 millimeters is used. In the de-deployed configuration the constrained coil **34** has a suitable diameter ranging from 0.1 mm to 3.0 mm. The coil **34** can be formed of wire having a diameter ranging from 0.002" to 0.004" (0.05 to 0.1 millimeters) and preferably about 0.003" (0.076 millimeters). Alternatively, it can be formed of ribbon generally rectangular in cross-section and can have a thickness of approximately 0.001" to 0.002" (0.025 to 0.05 mm.) and a width of approximately 0.003" to 0.005" (0.076 to 0.13 millimeters).

The deployment means or mechanism **33** consists of a push-pull wire **41** which is slidably disposed in and extending through the first or main lumen **26** and has proximal and distal extremities **42** and **43**. The push-pull wire **41** is formed of a suitable material such as stainless steel and has a suitable diameter as for example 0.005" to 0.032". Means is provided for securing the two ends **38** and **39** of the coil **34** to the distal extremity **43** of the push-pull wire **41** and consists of solder forming joints or adhesively bonded joints. As shown in FIG. 1 the proximal end **42** of the push-pull wire **41** extends out of the proximal extremity **23** of the flexible elongate tubular member **22** and is operatively connected to a handle assembly **44** as hereinafter described.

The handle assembly **44** is formed of a body **46** of suitable material such as plastic and is mounted on the proximal extremity **23** of the flexible elongate tubular member **22**. The handle **44** is sized so it is adapted to be grasped by the human hand and is provided with means for operation of the push-pull wire **41** which includes a button **47** adapted to be engaged by a finger of the hand holding the handle. The button **47** is mounted on a protrusion **48** which is slidably mounted in a longitudinally extending slot **49** in the handle **44** and is movable between first and second positions for deploying the coil **34** from a retracted or contracted elongate position constrained within the flexible elongate tubular member **22** to an expanded position outside of the tubular member **22**. The proximal extremity **42** of the push-pull wire **41** is secured to the protrusion **48** in a suitable manner such as a wire clamp or adhesive (not shown). The slot **49** opens into sideways extending notches **51** and **52** provided in the body which can receive the protrusion **48** in either the first or second position to retain the push-pull wire **41** in the desired position as hereinafter described.

The closure means **32** also includes a flexible impermeable membrane **36** which is carried by and secured to the distal extremity **24** of the flexible elongate tubular member **22**. It is desired that this membrane **36** be very flexible and it therefore has a wall thickness ranging from 0.0005" to 0.010" (0.0127 to 0.076 millimeters) and preferably 0.001" (0.025 millimeters). It can be formed of any suitable flexible

impermeable material such as elastomeric and non-elastomeric materials. For example, latex or silicone have been found to be suitable. The membrane **36** should be substantially impermeable to blood and other liquids. It is preferably formed as a tubular sock which can have an elongate generally cylindrical configuration with one closed end **54** and the other end circumscribed by an opening **56** which is defined by a rim **57** of the impermeable membrane. This rim **57** is circumferentially secured to the distal extremity **24** in a suitable manner such as by an adhesive (not shown) and preferably interiorly within the first or main lumen **26**. However, if desired, the rim **57** can also be affixed exteriorly to the outer surface of the tip **31** of the distal extremity **24** of the flexible elongate tubular member **22**. The impermeable membrane **36** is formed in such a manner so that it can, upon manufacture of the device **21**, be disposed internally of the distal extremity **24** of the flexible elongate tubular member **22** and be folded inwardly with folds **58** in the main lumen **26** to accommodate closure mechanism **34** in a constrained, retracted or contracted or de-deployed position as shown in FIG. 1. It also has the flexibility of being moved outwardly by operation of the push-pull wire **41** to the sock-like dotted line position **61** shown in FIG. 1.

The impermeable membrane **36** also can be caused to assume a disk-like planar configuration as shown by the dotted-line position **62** in FIG. 1. This is accomplished by operation of the deployment mechanism **33** to move the push-pull wire **41** distally to urge the closure mechanism **34** distally to move out of the lumen **26** into the dotted-line position **61**. As soon as the closure mechanism **34** is clear of the main lumen **26**, it will expand into its memorized configuration. As this expansion is occurring, the membrane **36** covering the coil **34** is caused to move from the sock-like configuration **61** to the disk-like circular configuration **62** so that the membrane **36** is disposed on opposite sides of the closure mechanism **34** and lies in generally parallel planes which are generally perpendicular to the longitudinal axis of the flexible elongate tubular member **22** for percutaneously occluding a puncture as hereinafter described. The deployed closure mechanism **34** is sufficiently rigid so as to provide a supporting framework for the membrane **36**.

The closure device **21** also consists of biological sealant introducer means **81** carried by the handle **44** and the flexible elongate tubular member **22** for introducing a biological sealant into a puncture proximal of the closure assembly **32** after the closure assembly **32** has been positioned. The biological sealant is of a suitable type such as a two-component fibrin glue, thrombin, fibrin, collagen-thrombin, collagen, Avitene (trademark), Gelfoam (trademark), cellulose, gelatin, and mixtures or slurries thereof. It should be appreciated that other biological sealants or pharmacological agents may also be introduced into a puncture utilizing this device.

The biological sealant introducer means **81** can consist of a fitting of a suitable type such as a wye adapter **82** which is provided with first and second arms **83** and **84** with first and second syringes **86** and **87** removably mounted thereon and containing the two separate constituents of fibrin glue being used as the biological sealant. The fitting **82** is connected to a flexible tubular member **91** which is sealed into the handle **44** and is provided with a lumen **92** therein in communication with the lumen (not shown) of the arms **83** and **84**. The distal end of the flow passage **92** in the tubular member **91** is aligned to be in communication with the second lumen **27** of the flexible elongate tubular member **22** so that when the syringes **86** and **87** are operated the biological sealant components are mixed and pass through

the flow passage **92** existing via the external port **28** of the second lumen **27**.

Operation and use of the device **21** in performing the method of the present invention in the percutaneous access and occlusion of vascular access sites and other puncture sites in the human body may now be described in conjunction with the cartoons shown in FIGS. **5A–5D**. Let it be assumed that a percutaneous femoral arterial catheterization is to be performed. After sterile preparation, a thin-walled hollow needle with syringe (not shown) is percutaneously inserted through the skin **101**, the underlying subcutaneous tissue **102** and then through the wall **103** defining the lumen **104** of a vessel **107** such as the femoral artery to form a puncture **106**. Intra-arterial access is confirmed by the aspiration of arterial blood. A flexible wire (not shown) is then passed through the needle into the artery **107** and the needle is removed, leaving only the wire in place in the puncture **106**. A vessel dilator (not shown) with a shorter conventional over-lying sheath **111** is passed over the wire through the puncture **106** into the lumen **104** after which the wire and dilator are removed. The sheath **111** extends from outside the patient through skin **101** and subcutaneous tissues **102** and through the wall **103** into the lumen **104** as shown in FIG. **5A**. Various diagnostic and therapeutic catheters and other similar medical devices can be passed through the sheath **111**, whose diameter can range from 3 to 24 French, to perform desired procedures, as for example an angioplasty procedure during which time anti-coagulants such as heparin have been introduced. At the conclusion of any such procedure, such instruments are removed leaving only the sheath **111** in place.

Let it be assumed that it is now desired to seal the puncture **106**. The closure device **21** of the present invention with the closure assembly **32** in the retracted position as shown in FIG. **1** is inserted into the sheath **111** while maintaining standard sterile precautions. The distal extremity **24** of the flexible elongate tubular member **22** is passed through the sheath **111** and into the lumen **104** so that it extends a short distance up to several inches beyond the distal extremity of the sheath **111** as shown in FIG. **5A**. The sheath **111** is then slowly, incrementally withdrawn proximally while maintaining the device **21** as stationary as possible. As can be seen from FIG. **5B**, the flexible elongate tubular member **22** has a length so that the sheath can be removed from the puncture **106** while retaining the distal extremity **24** in the lumen **104** and without removing the handle **44**. When the sheath **111** has been withdrawn as shown in FIG. **5B**, the closure assembly **32** may be deployed by operation of the deployment mechanism **33**. Alternatively, the distal extremity **24** of the flexible elongate tubular member **22** can be passed into the lumen **104** a slightly greater distance, the device **21** deployed with the sheath **111** still in position, and then both the sheath **111** and device **21** slowly withdrawn so that the sheath **111** is removed from the lumen **104** with the deployed device **21** appropriately positioned in the lumen **104**.

Before deployment of the closure assembly **32**, the finger button **47** is in its most proximal-most position with the protrusion **48** being seated in the notch **51** as shown in FIG. **5A**. Now let it be assumed that it is desired to move the closure assembly **32** from a contracted or retracted position where it is disposed within the first main lumen **26**. When it is desired to move the closure assembly **32** to an expanded or open position, the button **47** is retracted from the notch **51** and slidably advanced along the slot **49** to push the distal extremity **43** of the push-pull wire **41** distally to cause the Nitinol closure mechanism **34** to be advanced distally and to

carry the folded impermeable membrane **36** out of the first or main lumen **26** to cause it to assume a sock-like shape as shown in position **61** in FIG. **1**. Continued forward movement of the finger button **47** causes further longitudinal movement of the push-pull wire **41** which causes further distal movement of the closure mechanism **33** until it clears the first lumen **26** so that it is substantially free to cause it to expand into its super-elastic or shape memory form of a coil to carry with it the flexible impervious membrane **36** to assume the disk-like configuration represented by position **62** as shown in FIGS. **1** and **4**. The finger knob is then positioned so that the protrusion **48** is seated in the notch **52**.

After the closure mechanism has been fully deployed, the handle **44** can be utilized to gradually retract the flexible elongate member **22** to ensure that the proximal surface of the flattened flexible membrane **36** is brought into close engagement with the inner surface of the wall **103** forming the lumen **104** in which the closure assembly **32** is disposed. This forms a liquid tight seal between the closure assembly **32** and the wall **103** immediately adjacent the puncture **106** which in turn enables accurate and effective deposition of the biological sealant into the puncture **106** as hereinafter described. Such a liquid tight seal is also necessary in connection with the present invention to prevent the leakage of blood through the puncture **106**. This serves to prevent blood from interfering with attempts to safely and permanently occlude and seal the puncture **106** and to prevent inadvertent intravascular deposition of sealant.

The formation of a good seal between the occlusion assembly **32** and the wall **103** of the vessel **107** can be ascertained in several ways. By way of example the absence of arterial blood in the puncture **106** serves to verify that a good seal has been made. Attempts to aspirate blood from the second lumen **27** with no blood return therefrom also indicates accurate placement of the device **21**. Alternatively, fluoroscopy can be utilized to check the position of the closure assembly **32**. This is made possible because of the radio opacity of the closure mechanism **34**. Radio opaque dyes may also be utilized to ascertain whether the puncture has been effectively sealed. A small amount of radio opaque dye may be injected into the subcutaneous tissue adjacent the puncture **106**. If fluoroscopy demonstrates intravascular dye then there is inadequate placement of the closure assembly **32**. If perchance there is any leakage, the button **47** can be engaged by the finger and retracted out of the notch **52** and proximally for a slight distance and then moved distally to re-deploy the mechanical assembly **32**, thereafter grasping the handle **44** and pulling the flexible elongate member **22** proximally to again reestablish a seal with the wall **103** adjacent the puncture **106**.

As soon as it has been established that a good seal has been formed in the manner hereinbefore described between the closure assembly **32** and the wall **103** adjacent the puncture **106**, a biological sealant to be utilized can be introduced into the puncture **106** to provide a sealant **116** which extends throughout the puncture **106** from immediately outside the vessel **107** up to as far as the outer surface of the skin **101** as shown in FIG. **5C**. It should be appreciated, however, that it may not be necessary to introduce an amount of sealant so great as to cause it to extend proximally to the skin. Assuming that the biological sealant is a fibrin glue supplied in two ports in the syringes **86** and **87**, the physician utilizing the closure device **21** while holding the handle **44** in one hand utilizes the other hand to operate the syringes **86** and **87** to cause the constituents of the biological sealant to be introduced into the wye adapter **82** where they are mixed with each other and introduced

through the tubular member **91** and into the second lumen **27**, thence through the exit port **28** which is adjacent to the closure assembly **32**. It should be appreciated that in addition to holding the handle **44** in order to maintain engagement of the closure assembly **32** with the vessel wall **103**, any suitable device by way of example a pin-vise may be applied to the flexible elongate tubular member **22** immediately adjacent to the skin **101** so that the engagement is maintained and the physician has a free hand. The fibrin glue seals the innermost tissue layers in the puncture **106** and then, as hereinbefore described, can backfill the puncture **106** through the subcutaneous tissue **102** and to the skin **101**, surrounding the distal extremity **24** of the flexible elongate tubular member **21** as shown in FIG. **5C**. If necessary, the completion of this backfilling can be observed by the fibrin glue exiting from the puncture **106**. As soon as this occurs, the physician terminates further movement of the syringes **86** and **87** and then while still holding the handle **44** to retain the closure assembly **32** in place, permits the fibrin glue to set up or cure within the puncture **106** for a period of time suitable to permit the fibrin glue to form a sticky adherent clot in the puncture **106** but to prevent the fibrin glue forming a clot which is too firm so as to preclude easy withdrawal of the closure device **21**. Typically this ranges from a period of time of 30 seconds to 15 minutes and preferably a period of time of approximately 1–2 minutes. The aforementioned biological sealants only adhere to collagen-containing tissues which prevents them from bonding to the flexible elongate tubular member **22**. As soon as the physician determines that the fibrin glue has assumed the desired state, the button **47** carried by the handle **44** is engaged by the finger of the physician's hand and moved out of the slot **52** and then retracted proximally in the slot **49** to cause proximal movement of the push-pull wire **41** to cause a gradual straightening of the closure mechanism **34** to bring it substantially within the interior of the lumen **26** thereby permitting collapse of the flexible membrane **36** so that it can assume a generally sock-like configuration. Thus as soon as the button **47** has been moved to its most proximal position and moved into the notch **51**, the closure device **21** can gently be pulled from the seal **116** provided in the puncture **107**. The hole (not shown) left in the sealant **116** after withdrawal of the flexible elongate tubular member **22** and the membrane **36** carried thereby closes on itself due to the sufficiently gel-like state of the fibrin glue or other agent. Thereafter, the site of the puncture **106** is observed to ascertain whether or not bleeding is occurring therefrom. An excellent biological seal is formed with nothing remaining at the puncture site except for the biological sealant which within a relatively short period of time as for example 1–2 weeks will be absorbed by the body.

From the foregoing it can be seen that there has been provided a closure device and a method for utilizing the same which makes it possible to quickly and efficaciously close the puncture which has been made necessary for performing a desired medical procedure as for example an angioplasty procedure. An excellent seal is formed even though anticoagulants have been introduced into the blood of the patient during the procedure to prevent the formation of clot. The application of fibrin glue in this manner permits the formation of a good clot to seal the puncture without danger of re-bleeding occurring.

It also should be appreciated that during this procedure in performing the closure of the puncture site, blood can continue to flow substantially unimpeded through the lumen **104** of the vessel. This lack of obstruction is made possible because of the small size of the distal extremity of the

closure device **21** and also because of the small size of the closure assembly **32** carried by the distal extremity **24** of the device **21**. When the closure assembly **32** is deployed as hereinbefore described, it has a relatively small diameter in comparison to the size of the lumen into which it is introduced. In addition it has a flat planar configuration which, when brought into engagement with the inner surface of the wall **103**, is substantially flush with the inner surface of the wall **103**. Even when the closure assembly **32** is being de-deployed it occupies very little space as it is being withdrawn.

Another embodiment of the closure assembly is shown in FIG. **6** which can be utilized in place of the closure assembly **32** on the distal extremity **24** of the flexible elongate tubular member **22** carried by the handle **44**. As shown, the closure assembly **131** consists of a closure mechanism **132** which is covered by a flexible impermeable membrane **133**. The closure mechanism **132** can be formed of the same super-elastic or shape memory material as the closure mechanism **34** but rather than having a coil-like configuration such as shown in FIG. **1**, **3** and **4**, it includes a different complex geometrical configuration as for example a flower-like configuration as shown in FIG. **6**. Thus it can be formed of a Nitinol ribbon or wire of a single length having ends **137** and **138** which are secured to the distal extremity **43** of the push-pull wire **41** in a manner similar to that hereinbefore described. The wire ribbon **136** has been annealed to have a super-elastic or shape memory form for the flower-like configuration shown in which a plurality of loops **141**, as for example three as shown are provided on the wire ribbon **136**. The loops **141** are oval shaped, approximately equal in size and have curved outer extremities **142**. The loops **141** lie in a single plane and have the longitudinal axes of the loops spaced apart by equal angles of about 120°. It should be appreciated that if desired, additional loops can be provided with the loops being spaced equally over 360°. Since the loops **141** correspond to the shape of petals of a flower, the configuration shown in FIG. **6** can be described as a flower-like arrangement in which the loops **141** lie in a common plane which is generally perpendicular to the longitudinal axis of the flexible elongate member **22**.

The membrane **133** which forms a part of the closure assembly **131** can be formed of the same material as the membrane **36** and can be secured in the same manner to the tubular member **22** so that when the closure mechanism **132** is in a retracted position within the lumen **26** it also can be provided with folds in the same manner as the membrane **36**. The closure mechanism **132** can be straightened in a similar manner and brought into a retracted position similar to the closure mechanism **34**. The closure assembly **131** also can be deployed in a similar manner. When deployed, it will cause the impermeable membrane to assume a generally flat planar configuration which is still substantially in the form of a circle as determined by the outer curved extremities **142** of the loops **141** with very slight variations from a circle between the outer extremities of adjacent loops. Thus a good seal can be formed with the wall **103** of the vessel **107** in the same manner as with the closure assembly **32**. Thus it can be seen that the operation and use of the closure assembly of FIG. **6** can be very similar to that described for use of the closure assembly **32** and with generally the same attendant advantages. It should be appreciated that other arrangements of closure mechanisms can be provided for causing appropriate deployment of the impervious membrane to form a seal without departing from the scope of the present invention. The sizes and shapes of the closure assemblies can be selected to be appropriate for the puncture to be occluded.

Thus for example the flower arrangement shown in FIG. 6 can have the same size as the coil arrangement shown in FIGS. 1, 3 and 4 or alternatively can be decreased or increased in size as desired. Furthermore, by altering the number of petals or loops, the shape can also be varied from that of a circle to that of substantially a triangle or square.

Another embodiment of a closure device incorporating the present invention is shown in FIGS. 7-10. The closure device 151 is shown therein. The closure device is very similar to that shown in FIG. 1 with the principal difference being in the type of closure assembly utilized on the distal extremity 24 of the flexible elongate tubular member 22. Thus all of the parts of the closure device 151 carry the same numbers as the closure device 21 shown in FIG. 1 to the distal extremity 24 on which the closure assembly 156 is carried. The closure assembly 156 consists of a closure mechanism 157 which is covered by a flexible impermeable membrane 158. The closure mechanism 157 consists of a plurality of rod-like elements 161, struts or arms of at least three in number which are circumferentially spaced apart and have proximal ends 162 which are embedded in the distal extremity 24 of the flexible elongate tubular member 22. This can be accomplished in a suitable manner such as by extruding the plastic forming the tubular member over the proximal ends 162 or alternatively by placing axially aligned bores in the distal extremity 24 and securing the proximal ends 162 therein by suitable means such as an adhesive. The exposed portions of the rod-like elements 161 as shown in FIG. 7 are formed of a suitable material such as stainless steel or Nitinol and are inclined inwardly in a distal direction to provide a truncated cone-like shape. The distal ends 163 of the rod-like elements 161 can be bonded or fastened together in a suitable manner such as by welding or solder to provide a generally hemispherical tip 166 which is also secured to the distal extremity 43 of the push-pull wire 41. The rod-like elements 161 are provided with weakened regions or notches or memorized bending points 171 approximately a substantially equal distance from the proximal and distal ends 162 and 163 to form hinge points 171. The lengths of the exposed portions of the rod-like elements 161 may be selected to correspond to a selected diameter of the closure mechanism 157.

The membrane 158 which covers the closure mechanism 157 has a sock-like configuration with a closed end 176 which overlies the hemispherical tip 166 and an open end which is defined by the circular rim 177 which is bonded to the exterior surface of the distal extremity 24 of the flexible elongate tubular member 22 by an adhesive (not shown).

Operation and use of the closure device 151 may now be briefly described as follows. It should be appreciated that imposition of the button 47 with respect to the notches 51 and 52 is reversed in that the button is positioned in the notch 52 when the closure assembly 156 is in the de-deployed or unexpanded condition as shown in FIG. 7 rather than in the notch 51. A closure device 151 can be introduced into the sheath 111 in the unexpanded condition shown in FIG. 7 in the manner hereinbefore described with respect to the device 21 and after the closure assembly 156 is within the lumen 104 of the vessel 107 the closure assembly 156 can be deployed or moved to an expanded position by moving the button 47 proximally to cause a pulling force to be applied to the hemispherical tip 166 to cause a pushing force to be applied to the rod-like elements 161 to cause them to be bowed outwardly and to bend or fold about the hinge points 171 and at the same time to carry with them the membrane 158. Continued movement of the button 47 proximally until it reaches the slot 51 will cause the rod-like elements 161 to

cause the portions 161a to generally overlie the portions 161b and to extend radially from the longitudinal axis of the flexible elongate tubular member 22 at substantially right angles thereto as shown in FIG. 10. The membrane 158 covering the same is similarly caused to assume a generally circular disk-like configuration lying in a single plane which can be brought against the inner surface of the wall 103 of the vessel 107 in the same manner that the closure assembly 32 hereinbefore described is brought into contact with the wall. Thereafter the procedure hereinbefore described can be used for forming the seal with the puncture 106 and to permit introduction of the biological sealant. After this procedure has been completed, the closure mechanism 157 can be de-deployed by moving the same to an unexpanded condition by moving the knob 47 proximally to cause the push-pull wire 41 to move the hemispherical tip 166 distally and to carry with it the membrane 158 until the closure assembly 156 assumes its original unexpanded or de-deployed generally cylindrical configuration which is in alignment with the longitudinal axis of the flexible elongate tubular member 22 as shown in FIG. 7 after which the closure device 151 can be removed to form the desired occlusion for the puncture 106. It should be appreciated that by varying the number of rod-like elements the shape of this closure assembly can similarly be varied so that it may be deployed into planar triangular, square or oval configurations as well. This closure assembly 156 also differs from the closure assembly 32 and the closure assembly 131 in that it can be formed without the use of super-elastic or shape memory material.

Another embodiment of a closure device incorporating the present invention is shown in FIGS. 11, 12 and 13 in which a closure device 191 is shown which is very similar to the closure device shown in FIG. 7 with the exception that the closure assembly carried by the distal extremity 24 of the flexible elongate tubular member 22 is of a different construction from the closure assembly 156. The closure assembly 196 differs from the closure assembly 156 in that the distal extremity 24 of the flexible elongate tubular member 22 carries an additional segment 192 of flexible elongate tubular material which has been bonded or annealed to the tip 31 of the distal extremity 24 of the flexible elongate tubular member 22 and which forms a part of a closure mechanism 197 which is covered by an impermeable flexible membrane 198. The additional segment 192 is constructed of a segment of flexible elongate tubular member which is extruded with only a main circular in cross-section first lumen and without an additional lumen. The second lumen 27 in this device 191 is blocked by the bonded or annealed additional segment 192 and thus no plug is required. To form the closure mechanism 197, the additional segment 192 of the flexible elongate tubular member 22 is provided with a plurality of circumferentially spaced apart longitudinally extending slits 201 of a suitable number to provide a plurality of arcuate segments as for example the four segments 24a, 24b, 24c and 24d as shown in FIGS. 11 and 12. As hereinafter described since the segments 24a, b, c and d are formed of a flexible material, they can be bowed outwardly. The closure assembly 196 also includes a plurality of rod-like elements 202 similar to the rod-like elements 161 and formed of a suitable material such as stainless steel or Nitinol but because of the use of the arcuate segments 24a, b, c and d the rod-like elements 202 need only be approximately one-half the length of the rod-like elements 161. The rod-like elements 202 like the rod-like elements 161 can have a suitable diameter as for example 0.002" to 0.015" or preferably 0.002" to 0.003". The rod-like

elements **202** are provided with proximal and distal ends **203** and **204**. The proximal ends are embedded in the arcuate segments **24a, b, c** and **d** in a suitable manner. For example, the plastic forming the segments can be extruded over the ends **203** or, alternatively, the segments can be provided with bores for receiving the ends **203** which are secured therein by suitable means such as an adhesive (not shown). The rod-like elements **202** extend distally and inwardly to form a truncated cone and have their distal ends **204** interconnected by a generally hemispherical tip **206** formed of solder or a weld which is also bonded to the distal extremity **43** of the push-pull wire **41** as shown in FIG. **11**. The rod-like elements **202** are provided with notches or weakened regions or memorized bending points to form hinge points **208** which are preferably in close proximity to the arcuate segments **24a, b, c** and **d** so that the hinge points are close to the junctures between the ends **203** and the adjoining segments **24a, b, c** and **d**. The length of each of the arcuate segments **24a, b, c** and **d** and each of the rod-like elements **202** is approximately equal and corresponds to the desired size of the closure mechanism **197**.

The membrane **198** covers the closure mechanism **197** and has a conformation similar to that of the membrane **158** and is provided with a closed end **211** which overlies the hemispherical tip **206** and an open end circumscribed by a rim **212** which is adhered to the additional portion **192** of flexible elongate tubular material annealed to the tip **31** of the distal extremity **24** of the flexible elongate tubular member **22** just proximal of the slits **201** which form the segments **24a, 24b, 24c** and **24d** and is secured thereto by a suitable means such as an adhesive (not shown).

Operation and use of the closure device **191** as shown in FIGS. **11** and **12** is very similar to that described for the embodiment of the closure device **151** shown in FIG. **7**. The closure device as shown in FIG. **11** has the closure assembly **196** in a de-deployed or un-expanded condition with the button **47** being disposed in the notch **52**. In connection with sealing a puncture after the distal extremity **24** of the device **191**, and in particular the closure mechanism **197**, is disposed within the vessel **107** distal of the puncture **106**, the closure assembly **196** can be deployed by moving the button **47** proximally to cause pulling on the pull wire **41** to apply compressive forces to the strut-like rod-like elements **202** to cause outward bowing of the same as well as the segments **24a, 24b, 24c** and **24d** with sharp bends occurring at the hinge points **208** just distal of the arcuate segments **24a, b, c** and **d**. This outward bowing is continued so that the arcuate segments **24a, b, c** and **d** are bent outwardly with respect to the longitudinal axis of the flexible elongate tubular member **22** and similarly the rod-like strut elements **202** are bowed outwardly with respect to the hemispherical tip **206** while carrying along with them the flexible impermeable membrane **198** until the rod-like elements **202** substantially overlie and are generally parallel with the segments **24a, b, c** and **d** as shown in FIGS. **13** and **14** to form a planar disk-like conformation corresponding generally to the disk-like conformations of the embodiments of the closure devices hereinbefore described. Although the conformation as viewed in FIG. **14** has a generally square configuration it can be readily appreciated that by providing additional segments in the distal extremity **24** and a corresponding number of additional rod-like elements, additional arms can be provided for controlling the movement of the membrane **198** so that the outer margin of the membrane has a more generally circular configuration if that be desired. As heretofore described with other embodiments, the configuration may also be oval, triangular or square depending on the number of elements.

After the closure assembly **196** has been deployed as shown in FIGS. **13** and **14** it can be utilized in the manner hereinbefore described with the previous closure devices for forming a seal with the inner surface of the wall **103** and thereafter introducing a biological sealant. After this has been accomplished, the closure assembly **196** can be contracted and de-deployed by moving the button **47** from the notch **51** and pushing it distally to push the hemispherical tip **206** distally and to cause inward collapsing of the segments **24a, b, c** and **d** and the rod-like strut elements **202** until they have been moved into the original de-deployed or contracted positions as shown in FIG. **11** and with the button **47** in the notch **52**. Thereafter, the closure device **191** can be retracted in a manner similar to that hereinbefore described with respect to the previous embodiments.

Another embodiment of a closure device incorporating the present invention is shown in FIGS. **15** and **16**. The closure device **221** shown therein is similar to that shown in FIG. **1** with the principal differences being that the device **221** utilizes a closure assembly on the distal extremity **24** of the flexible elongate tubular member **22** and a deployment means that incorporate elements that are similar to both the device shown in FIG. **1** and the device shown in FIGS. **7-10**. The closure assembly **222** consists of a closure mechanism **223** and an impervious membrane **224** which covers the closure mechanism **223**. The closure mechanism **223** can be formed of the same super-elastic or shape memory material as the closure mechanism **34** but rather than having a coil-like configuration it consists of a plurality of circumferentially spaced apart rod-like elements **226** or arms of at least three in number having proximal and distal ends **227** and **228**. Thus each rod-like element **226** can be similarly formed of Nitinol ribbon or wire and is annealed with an approximate 180 degree fold located at the midpoint **229** between the proximal **227** and distal **228** ends so that when in a free state the element **226** tends to fold at the midpoint **229** causing the proximal and distal halves **231** and **232** of the rod-like element **226** to substantially overlie one another in a single plane. Means is provided to secure the proximal end **227** of each rod-like element **226** to the deployment mechanism **230** in a manner hereinafter described. The distal ends **228** of the rod-like elements **226** are fastened together in a suitable manner such as by welding or soldering to provide a generally hemispherical tip **233** which is also secured to the deployment mechanism **230** in a manner hereinafter described. Similar to the closure device **151** shown in FIGS. **7-10**, the lengths and number of the rod-like elements **226** may be selected to correspond to a selected diameter and shape of the closure mechanism **223**.

The membrane **224** which forms a part of the closure assembly **222** can be formed of the same material as the membrane **36** and can be secured in the same manner to the tubular member **22** so that it is provided with folds and functions in the same manner as the membrane **36**.

The deployment mechanism **230** consists of a push-pull wire **234** formed of a suitable material such as stainless steel which is slidably disposed in the first or main lumen **26** and has proximal and distal extremities **236** and **237** similar to the push-pull wire **41** with the principal difference being that during formation the push-pull wire **234** is provided with a central lumen or bore **238** extending from the proximal extremity **236** to the distal extremity **237**. The push-pull wire **234** has a suitable outside diameter of approximately 0.020" (0.5 millimeters) and an inside diameter of approximately 0.010" (0.25 millimeters). Means is provided for circumferentially securing the proximal ends **227** of the rod-like elements **226** to the distal extremity **237** of the push-pull

wire 234 with the secured proximal ends 227 of the elements 226 being equally spaced apart over 360 degrees and with the vertex of each midpoint 229 fold directed outwardly and consists of similar welds or solder forming joints 239 and 241. The proximal end 236 of the push-pull wire 234 extends out of the proximal extremity 23 of the flexible elongate tubular member 22 and is connected to a handle assembly 242 in a manner similar to the device 21. The deployment mechanism 230 includes a second, smaller pull wire 243 which is slidably mounted or disposed within the central lumen 238 of the larger push-pull wire 234 and is provided with proximal and distal extremities 244 and 246. The pull wire 243 is similarly formed of a suitable material such as stainless steel and has a suitable diameter as for example 0.005" to 0.030". Means is provided for securing the distal extremity 246 of the pull wire 243 to the hemispheric tip 233 and consists of soldering or welding. The proximal end 244 of the smaller pull wire 243 also extends out of the proximal extremity 23 of the flexible elongate tubular member 22 and is operatively connected to the handle assembly 242 which, in addition to carrying means for causing longitudinal movement of the push-pull wire 234 hereinbefore described and shown in FIG. 1, also carries means for causing movement of the pull wire 243 along the longitudinal axis independent of the movement of the push-pull wire 234 in a manner hereinafter described.

The handle assembly 242 is similar to the handle assembly 44 with the principal difference being that the handle assembly 242 also provides access to the proximal end 244 of the smaller pull wire 243. The protrusion 247 of handle assembly 242 and means of securing the push-pull wire 234 to the same is similar to protrusion 48 but the protrusion 247 is also provided with a lumen 248 extending from the proximal end 249 to the distal end 251 of the protrusion 247 and aligned with the central lumen 238 of the proximal extremity 236 of the push-pull wire 234. A handle lumen 250 is provided which extends proximally from the proximal end of the handle slot 255 and is alignment with both the slot 255 and the proximal end 249 of the lumen 248 in the protrusion 247. The handle lumen 250 is provided with an aperture 252 at the proximal end of the handle 242. The proximal end 244 of the smaller pull wire 243 extends proximally out of the proximal end 236 of the push-pull wire 234 into and through the lumen 248 of the protrusion 247 and through the handle lumen 250 slidably extending proximally out of the handle assembly 242 through the aperture 252. Means for fixing the proximal end 244 of the pull wire 243 in a particular position is provided as for example with a simple releasable clamp or knob 253 that prevents the pull wire 243 from sliding distally.

Operation and use of the closure device 221 may now be briefly described as follows. It should be appreciated that operative positions of the button 254 for operation and use of the closure device 221 are similar to positions for button 47 in the closure device 21 shown in FIG. 1. A closure device 221 can be introduced into the sheath 111 in the un-expanded cylindrical or de-deployed configuration shown in FIG. 15 in the manner hereinbefore described with respect to the device 21. The closure assembly 222 also can be deployed and de-deployed in a similar manner with the principal difference being the additional steps of deploying and de-deploying the pull wire 243 in a manner hereinafter described. After the button 254 is similarly utilized to initiate and maintain deployment of the closure assembly 222 by pushing the closure mechanism 223 out of the distal extremity 24 of the flexible elongate tubular member 22, the rod-like elements 226 and the membrane 224 assume a

configuration which is substantially in the form of a disk or a flattened circle, the shape being partially determined by the number of the rod-like elements 226. In order to assure assumption of a substantially flat planar configuration by the closure assembly 222 the small pull wire 243 is then pulled proximally and fixed in position by using the clamp 253, while the push-pull wire 234 is held stationary, to cause a pulling force to be applied to the hemispherical tip 233 to cause a pushing force to be applied to the rod-like elements 226 to cause them to further fold about their midpoints 229 so that the proximal and distal halves 231 and 232 of the elements 226 substantially overlies one another in a single plane at a substantially right angle to the longitudinal axis of the flexible elongate tubular member 22. Thereafter the procedure hereinbefore described can be used for establishing a seal of the puncture 106 and to permit introduction of the biological sealant. After this procedure has been completed, the closure assembly 222 can be de-deployed by releasing the clamp 253, permitting the small pull wire 243 to be pushed distally and then similarly completing the de-deployment sequence as hereinbefore described for closure device 21.

It should be appreciated that additional variations of the pull wire assembly may be utilized as for example means may be provided for mounting the pull wire within the lumen of the push-pull wire so that the position of the pull wire is fixed in relation to the longitudinal axis of the flexible elongate tubular member so that with independent longitudinal movement of the push-pull wire a similar pulling force is simultaneously applied to the hemispherical tip to cause a pushing force to be applied to the rod-like elements as hereinbefore described.

It should also be appreciated that other embodiments may incorporate closure assemblies utilizing arcuate segments similar to those shown in FIGS. 11, 12 and 13, absent rod-like elements wherein the distal tip of the push-pull wire is bonded directly to the tip of the distal extremity of the flexible elongate tubular member so that with proximal traction on the push-pull wire compressive forces applied to the arcuate segments cause outward bowing of the same with bends or folds occurring at the midpoints of the segments. An additional closure assembly may include a closure mechanism constructed of super-elastic or shape memory alloy that is deployed by pushing the closure mechanism distally out of the distal extremity of the flexible tubular member and then causing the super-elastic or shape memory alloy mechanism to be twisted by turning the proximal end of the push-pull wire. In various embodiments the impermeable membrane may also be secured directly to the closure mechanism instead of being secured to the distal extremity of the flexible elongate tubular member. Alternatively the membrane may be configured so to only partially cover the closure mechanism as for example only the proximal side of the deployed closure mechanism.

Another embodiment of an expansile or closure device incorporating the present invention is shown in FIGS. 18-19. The device 301 shown therein consists of a first elongate tubular member 302, preferably a flexible elongate tubular member 302, formed of a suitable plastic material, preferably a cast thermoset material such as polyimide. The first flexible elongate tubular member 302 has proximal and distal extremities 303 and 304 with a longitudinal axis extending from the proximal 303 to the distal extremity 304 and is provided with a first lumen 306 circular in cross-section which, as shown, may be centrally disposed extending from the proximal extremity 303 to the distal extremity 304. Both the outer and inner surfaces of the polyimide

member **302** may be coated with a lubricious material such as Teflon™. Alternatively, the thermoset material may be a polyimide-Teflon™ or polyimide-Nylon-Teflon™ composite in order to provide the desired lubricious inner and outer surfaces. The first flexible elongate tubular member **302** has an outside diameter ranging from approximately 0.008" to 0.050", preferably approximately 0.018". The first flexible elongate tubular member **302** has a suitable length as for example 10–150 centimeters. The first lumen **306** in the first flexible elongate tubular member **302** may have an inside diameter of approximately 0.003" to 0.030", preferably 0.012".

Expansile means in the form of an expansile assembly **307** is carried by the distal extremity **304** of the first flexible elongate tubular member **302** and is movable between contracted and expanded positions. A deployment mechanism **308** is carried by the proximal extremity **303** of the first flexible elongate tubular member **302** and adapted to be operated by the human hand for movement from a contracted position to an expanded or deployed position.

The assembly **307** includes a expansile member **309** and a membrane **311** which covers the expansile member **309**. The expansile member **309** as shown in FIG. **19** is in a form having a complex geometrical configuration, preferably a helical coil configuration **312**, when in a free state. The helical coil **312** is formed of a suitable material, preferably Nitinol, which can be elongated or constrained without permanent deformation but, at body temperature, when freed or unconstrained returns to the helical coil configuration to which it has been annealed. The helical coil **312** has a plurality of generally circular turns creating, preferably, a proximal turn **313**, a middle turn **314** and a distal turn **316**. The proximal, middle and distal turns **313**, **314**, **316** are generally nonplanar with respect to one another. The proximal and distal turns **313** and **316** each lie in a plane that is generally parallel to one another and generally perpendicular to the longitudinal axis of the first flexible elongate tubular member **302**. The middle turn **314** is non-planar and helical as it connects the proximal and distal turns **313** and **316** so that the unconstrained helical coil configuration assumes a bi-conical shape.

The middle turn **313**, when freed or unconstrained, has a suitable diameter ranging from 2 to 10 millimeters and preferably 4 to 6 millimeters is used. As hereinafter described, during deployment the middle turn **313** is partially flattened and constrained by the membrane **311** to assume a diameter ranging from 1 to 10 millimeters, preferably 11 French, in order to overlap a puncture site to assist in occluding the puncture site. The proximal and distal turns **313** and **316** are of approximately equal size and diameter ranging from 1 to 5 millimeters, preferably 2 to 3 millimeters. The unconstrained helical coil **312** configuration has a distance from the proximal **313** to the distal turns **316** of approximately 3 to 15 millimeters, preferably 5 to 8 millimeters. In the de-deployed configuration the helical coil **312** is retracted into the first flexible elongate tubular member **302** and has a contracted, constrained diameter corresponding to the approximate diameter of the Nitinol wire used to construct the expansile mechanism **309**, ranging from 0.002" to 0.010", preferably 0.005" to 0.006". The distal tip of the Nitinol wire corresponding to the free end of the distal turn **316**, preferably, carries an enlargement, as for example a small ball or flattened tip **310** so as to prevent puncture of the membrane **311** by the wire during operation of the device and so as to decrease friction of the tip **310** against the wall of the lumen **306** of the first flexible elongate tubular member **302** out of which the expansile mechanism **309** is

pushed as hereinafter discussed. The ball **310** may be formed by a suitable method such as arc welding, soldering, applying a polymer to the wire or folding the tip of the wire.

The deployment means or mechanism **308** includes a push-pull element or member **317** preferably in the form of a wire **317**, with proximal and distal extremities **318** and **319** which is slidably disposed in and extending through the first or main lumen **306**. The push-pull element **317** is formed of a suitable material such as stainless steel and has a suitable diameter as for example from 0.005" to 0.030", preferably 0.010". The expansile member **309** and the push-pull element **317** may be separately constructed and subsequently joined together utilizing one of several different methods. The two may be bonded or soldered together. Preferably, in order to provide for optimal torque, the stainless steel wire **317** is ground to provide a tapered portion **317a** formed on the distal end **319**. The tapered portion **317a** is inserted into one end of an elongate member, often called a hypotube **320** made of an appropriate material such as stainless steel and adhesively bonded therein using an appropriate adhesive **325** such as Loctite™. The proximal end **318** of the Nitinol wire expansile member **309** is similarly inserted and bonded into the opposite end of the hypotube **320**. The stainless steel hypotube **320** may be of an appropriate length, such as from 2 to 15 cm, preferably 4.5 cm. It may have an outer diameter ranging from 0.005" to 0.030", preferably 0.010" and an inner diameter ranging from 0.003" to 0.010", preferably 0.006".

Alternatively, both the push-pull wire **317** and the expansile mechanism **309** can be formed from a single piece of Nitinol wire in which case, in order to provide optimal pushability, torquability and column strength of the push-pull wire **317**, two alternative techniques are utilized. First, a Nitinol wire diameter of approximately 0.010" is used by grinding down the distal end **319** to a diameter suitable for subsequent formation of the expansile member **309**.

A second technique utilizes a Nitinol wire having a diameter suitable for formation of the expansile mechanism **309**. In such case, the push-pull wire **317** is covered with a suitable polymer jacket, preferably made of polyimide and having an diameter of approximately 0.005" to 0.0101". The polymer jacket is thicker at the proximal end **318**, necked down at the distal end **319** of the push-pull wire **317** and secured to the push-pull wire **317** at distal and proximal ends by a suitable adhesive such as Loctite™.

As shown in FIG. **18** the proximal end **318** of the push-pull wire **317** extends out of the proximal extremity **303** of the first flexible elongate tubular member **302** so that the deployment means can be operated by the human hand as hereinafter described.

It should also be appreciated that push-pull elements or mechanisms, other than a push-pull wire, can be utilized to deploy and de-deploy the expansile member and the expansile assembly.

A stop mechanism or means **321** is provided to control the range of movement or travel of the push-pull wire **317** during deployment and de-deployment of the expansile assembly **307**. The stop mechanism **321** comprises first and second, slidable nested or coaxially mounted stop tubes **322** and **323** formed of an appropriate material such as plastic or stainless steel. The distal end of the first stop tube **322** carries a bushing **324**. The bushing **324** is secured to the distal end of the first stop tube **322** by suitable means such as an adhesive (not shown). The proximal end **318** of the push-pull element **317** is affixed to the first tube by suitable means such as an adhesive. The push-pull element **317** with the first tube **322** affixed thereto and the bushing **324** carried thereby

is movable longitudinally of the second tube **323** which has its distal extremity secured to the proximal extremity **303** of the elongate tubular member **302**. It is movable from a forward most position with the bushing **324** in engagement with the proximal end **303** and a rearwardmost position in engagement with an annulus **326** mounted in the proximal extremity of the second tube **323** by suitable means such as an adhesive and through which the first tube **322** slidably extends. The lengths of the first and second tubes **322** and **323** are selected so that the travel between the forwardmost and rearwardmost positions ranges between 2 cm and 10 cm.

The expansile assembly **307** also includes a deformable, flexible membrane **311** which is carried by, and as shown, can be secured to the distal extremity **304** of the first flexible elongate tubular member **302** as hereinafter discussed. Since it is desired that this membrane **311** be very flexible it has a wall thickness ranging from 0.001" to 0.015" and preferably about 0.004". It can be formed of any suitable flexible material such as an elastomeric or a non-elastomeric material including latex and silicone. The membrane **311** can also be made of an impermeable or a permeable material providing for multiple uses of the device. A satisfactory membrane **311** can be made of Chemoprene™ or one of the polyurethane elastomers such as Polyblend™ having a shore hardness durometer of 30 to 70A, and preferably 55A, Tecoflex™ having a shore hardness durometer of 60 to 100A or Pellathane™ having a shore hardness durometer of 70 to 100A. Alternatively the membrane **311** can be made of multiple layers including a central Polyblend™ layer having a thickness of approximately 0.005" to 0.010" and a thin outer Tecoflex™ layer having a thickness of approximately 0.0005". This layered membrane **311** is made by dipping the Polyblend™ in a Tecoflex™ solution, for example a Tecoflex™ 85A solution. As shown, the membrane **311** is substantially impermeable to blood and other liquids. It is formed as a tubular sock **333** which has an elongate generally cylindrical configuration with one closed end **329** and the other end circumscribed by an opening **331** which is defined by a rim **332** of the same material. The tubular sock **333** has an appropriate length, as for example ranging from 2–15 mm, preferably 7 mm. When the membrane **311** is made from Polyblend™, typically supplied in a tubular form and cut into lengths of appropriate dimensions with both ends open, the closed end **329** of the membrane **311** is formed by dipping one open end of the Polyblend™ into a Tecoflex™ solution, preferably 10% by weight of 85A Tecoflex™, to provide a sealing plug **327**. The rim **332** of the membrane **311** can be circumferentially secured to the distal extremity **304** of the first flexible elongate tubular member **302** in a suitable manner such as by the Loctite 454™ adhesive (not shown).

A length of stainless steel hypotube **328** has one end secured to the distal end **304** of the first flexible elongate tubular member **302** (see FIG. 18) using an appropriate adhesive such as Loctite 406™. The hypotube **328** has an appropriate length ranging from 2 mm to 10 mm, preferably 5 mm, and is secured to the first flexible elongate tubular member **302** and extends distally of the same by approximately 2–8 mm. The rim **332** of the membrane **311** is affixed exteriorly of the stainless steel hypotube **328** by an adhesive (not shown), preferably, distal to the point at which the hypotube **328** is secured to the first flexible elongate tubular member **302** and with the closed end **329** of the membrane **311** oriented distally thereon as shown in FIG. 18. As such, a portion of the membrane **311** distal to the rim **332** overlies the steel hypotube **328** and is non-adherent thereto. It should be appreciated if desired that the rim **332** can be secured

directly to the outer surface of the distal extremity **304**. In either arrangement, the membrane **311** assumes a sock-like conformation as shown in FIG. 18. Alternatively, the rim **332** of the membrane **311** may be secured interiorly within the hypotube **328** or, if the hypotube **328** is not utilized, within the first or main lumen **306** of the first flexible elongate tubular member **302**. In addition, the membrane **311** may be secured to the Nitinol wire proximal to the expansile member **309**.

The impermeable membrane **311** of the expansile assembly **307** can be caused to assume various configurations including a planar disk-like configuration as shown by the dotted-line position in FIG. 18. This is accomplished by operation of the deployment mechanism **308** to move the push-pull element **317** distally to urge the expansile member **309** distally out of the lumen **306** into the membrane **311**. The operator can assist deployment by applying a slight rotation to the push-pull element **317** as it is moved distally. As soon as the expansile member **309** clears the first lumen **306**, it begins to expand into its shape memory, predetermined configuration. The distal turn **316** of the expansile member **309** in the form of a coil operates to expand the membrane **311** initially to a small degree. This initial process avoids sudden gross distortion of the membrane **311**. As the expansile member **309** moves distally out of the lumen **306** and expands into the membrane **311**, the non-adherent portion of the membrane **311** distal to the rim **332** preferentially begins to move and assume the planar configuration because of the lubricious surface of the stainless steel hypotube **328**. Expansion proceeds with the middle turn **314** forming a coil and causing the membrane **311** to expand to its desired size, approximately 12 French. The proximal turn **313** forming a coil then centralizes and stabilizes the configuration so that the push-pull element **317** is centered with respect to the middle turn **314** and the fully expanded membrane **334**. During expansion of the expansile member **309** the membrane **311** covering the coil **312** constrains the coil **312**, thus exerting counteractive or countervailing contractile forces on the expanding coil **312** which is seeking its memorized, bi-conical, free shape or configuration **312**. Thus, the membrane **311** does not expand passively. Rather, the expanding coil **312** forcibly expands the membrane **311** to cause the non-planar turns **313**, **314** and **316** of the coil **312** to assume a substantially planar or disk-like configuration with the membrane **334** being taut and disposed on opposite sides of the expansile mechanism **309** to form an expansile assembly **307** which when expanded is generally perpendicular to the longitudinal axis of the first flexible elongate tubular member **302**. The expansile mechanism **309** when deployed is sufficiently rigid so as to provide a supporting framework for the membrane **311** to keep it taut.

It should be appreciated that other embodiments may be utilized employing superelastic expansile members with various memorized configurations. In addition, as hereinbefore discussed, different membrane materials may be utilized in order to construct permeable or impermeable assemblies for different functions. The predictability of countervailing, expansile forces and resistive, membrane forces enables the construction of expansile assemblies with predetermined, deployed configurations. In addition, instead of sliding a push-pull wire, the Nitinol member can be secured to a wire which remains stationary. In such an embodiment, the expansile member and wire are sheathed within an elongate tubular member which has a sock-like membrane secured to the distal end thereof and whence the member is deployed into the membrane by sliding the sheath proximally.

Operation and use of the device **301** is very similar to that described for the embodiment of the closure device **21** with the following differences. The expansile device **301** shown in FIGS. **18–19** is not used with biological sealants. Thus, after bringing the expansile assembly **307** into contact with the distal end of the puncture **106**, a proximal force of tension or traction is maintained on the expansile assembly **307** for a predetermined period of time ranging from 2 minutes to several hours, preferably 30 minutes to 1 hour, until the puncture **106** is sealed. Release of the tension is followed by moving the expansile assembly **307** from the deployed or expanded position to the de-deployed or contracted position after which the device **301** may be removed as hereinbefore described.

A second difference is that the radio-opacity of the expansile mechanism **309** is determined by the configuration of the coil **312**. When it is in the unconstrained, memorized, bi-conical configuration, the coil **312** is not fluoroscopically visible due to the small size of the individual turns of the Nitinol wire and the non-planar configuration. When the expansile mechanism **309** assumes the flat disk-like shape within the membrane **334** the cumulative densities of the Nitinol turns can be fluoroscopically visualized. As hereinbefore discussed, this too is an easy method of ascertaining or confirming formation of a good seal between the expansile assembly **307** and the wall **103** of the vessel **107**.

Furthermore, the low profile of the device **301** affords the ability to reenter the vessel **107** with the introducer sheath **111** if there has been inadequate occlusion and bleeding continues or other complications ensue. For example, let it be assumed that the operator believes the puncture **106** is sealed after removal of the sheath **111** and he therefore de-deploys the expansile assembly **307** as hereinbefore described. If, after so doing, he observes continued bleeding from the puncture **106**, the operator can reenter the vessel **107** by releasing tension, pushing the first flexible elongate tubular member **302** distally and reinserting the sheath **111** into the vessel **107** over the first flexible elongate tubular member **302**. The operator can also reenter the vessel for additional medical purposes if necessary. The same approach applies if the membrane **311** breaks or the expansile assembly **307** otherwise malfunctions. In this case the sheath **111** is replaced as hereinbefore described and the malfunctioning expansile device **301** is expeditiously replaced.

A tension applicator or catheter retention means **335** is provided which engages the elongate tubular member **302** and serves to releasably place tensioning forces on the elongate tubular member **302** to maintain engagement of the deployed expansile assembly **307** against the vessel wall **103** having a puncture **106** therein and to free the operator's hands from having to hold the device **301** after it is correctly deployed in the puncture **106**. The catheter retention means **335** provides a predetermined and substantially constant force in a proximal direction on the expansile member **309** over a range of motion or positions of the flexible elongate tubular member **302** which may occur as a result of patient movement or initial positioning.

The tensioning device **335** is shown in FIGS. **20–23** and consists of a fixture **336** or bottom portion which is constructed of a suitable material such as clear plastic and comprises a base plate **337** having an appropriate shape and size, as by way of example a pear-shape and size, as shown in FIG. **20** and adapted to rest on the skin **101** overlying the puncture **106** in the wall **103** forming the lumen **107**. The fixture **336** further comprises anterior and posterior walls **338** and **339** which extend upwardly, preferably at approxi-

mately right angles from the surface of the base plate **337**. The posterior wall **339** has an outer face **342** that is straight and an inner face **343** that is inclined. The anterior wall **338** also has inner and outer faces **344** and **346** that are straight. A swingable arm or top portion **347** is hingedly or pivotally mounted to the top of the posterior wall **339** of the base portion **336** for movement between open and closed positions with respect to the base portion **336**. In the open position, the top portion **347** may assume an angle of up to 180 degrees, preferably 45 degrees, with respect to the base portion **336**. In the neutral or closed position, the top portion **347** substantially overlies and is parallel to the base portion **337**. As hereinafter described however, in the closed position, the top portion **347** is also capable of at least 0.5 cm of additional travel or motion in both closed and open directions, both towards and away from the base portion **336**, respectively.

The arm **347** is hinged and biased or yieldably urged towards the open position, away from the skin of the patient, by spring means capable of providing a predetermined and substantially constant tensioning force over a range of positions. The top and bottom portions **347** and **336** of the tensioning device **335** can be constructed as one piece which incorporates a living hinge **348** formed by scoring or placing a groove in the plastic. Alternatively, a metal or other hinge can be utilized to join separate top and bottom portions. A constant force spring, such as a coil spring **349** capable of providing an appropriate constant force of tension is preferably utilized as hereinbefore discussed. It should be appreciated that any type of spring capable of providing the aforementioned constant force of tension can be used, as, by way of example, flat, leaf, spiral, helical, disk and volute springs.

As shown in FIG. **20**, catheter clamping or grasping means in the form of grasping members **351** are carried by the arm **347** and are movable between open or release, and closed or clamping positions. The grasping members **351** are in the form of serrated pads constructed of an appropriate material, such as plastic, rubber or metal. The grasping members **351** are carried by the distal extremities of flexible elongate curved spring members or grasping arms **352**. The arms **352** may be constructed of a suitable spring material such as plastic or metal and are disposed in a recess **350** of the casing of the top portion **347**. The proximal extremities of the spring arms **352** are disposed on opposite sides of spaced apart pins **352** mounted so that the proximal extremities are biased towards each other into the clamping position.

Means are provided for overcoming the bias of the spring arms **352** and consists of flanged actuator buttons **354** slidably mounted in holes. Actuator arms **355** are secured to the buttons **354** and extend one behind the other to engage the opposite spring arm **352** (see FIG. **21**) so that the spring arms **352** can be moved apart to move the grasping members **351** to the open position.

The fixture and arm portions **337** and **347** may be formed with slots **356** and **357** which are in alignment when the arm **347** is in the closed position and in which the first elongate tubular member **302** or body **362** is disposed when being grasped by the grasping members **351**.

Operation of the tension applicator **335** may now be described in conjunction with FIGS. **21–23**. By placing the fixture **336** against the patient's skin and, as shown in FIGS. **22–23**, urging or forcing the arm **347** towards the fixture **336** until it comes into apposition with the base plate **337** and opening the spring arms **352** in order to grasp the first flexible elongate tubular member **302** or elongate tubular body **362**, the tensioning device **335** can be set or activated

whence it maintains a suitable, constant proximal force of tension, preferably within a range of 0.25 to 3 pounds, over a range of motion. The force applied to the first flexible elongate tubular member **302** attempts to withdraw the member **302** from the puncture **106** in the wall **103** of the vessel **107** so that the expansile device **302** is retained in engagement with the wall **103** of the vessel **107**.

Indicator marks in the form of arrows **358** are placed on the fixture **336** and the arm **347** so that the marks are aligned with one another when the tensioning means **335** is correctly positioned and activated in the neutral, closed position as hereinbefore described. Alternatively, visualization through the clear plastic base plate **337** can serve as indicator means.

It should be appreciated that other embodiments of the tension applicator or tensioning device may be utilized in the present invention without departing from the novelty and the intended uses thereof. For example, the grasping means can be comprised of asymmetrical members and arms, similar to a pin vise or clamp. In such an embodiment one grasping arm is slidably disposed within another and can be spring loaded or otherwise biased into a position in which one grasping member is apposed with the other grasping member. Alternatively, two grasping arms may be constructed from a single arm which has been partially split along its longitudinal axis, providing arms that splay apart. Grasping members may also be comprised of clamps that snap or roll into closed positions. Similarly, the arm may have a length that is shorter than the bottom portion and beyond which the grasping members and arms extend. It should also be appreciated that the tension applicator **335** can be used with other catheters.

The tensioning device **335** with its indicators also serve to confirm formation of a good, occlusive seal of the puncture **106** with the expansile assembly **307**. The deployed expansile assembly **307** withstands the aforementioned proximal force or tension and in so doing maintains the occlusive seal unless the deployed coil **312** and disk-shaped membrane **334** change configurations. For example, if the membrane **311** breaks, the coil **312** once again assumes its memorized bi-conical configuration **312** which cannot maintain a high tensile force and is incompatible with puncture occlusion. As tension is lost the indicator on the tensioning device **335** is activated, alerting the operator to the release of the predetermined force of tension and lack of an adequate seal.

Another embodiment of the tensioning device is shown in FIG. 33. The tensioning device **380** is similar to that shown in FIG. 20 with the principal exception being that the device **380** provides a variable force in a proximal direction on the expansile member **309** over a range of motion or positions of the first flexible elongate tubular member **302** which may occur as a result of patient movement or initial positioning. Thus, all of the parts of the tensioning member **380** that are present in the tensioning member **335** carry the same numbers. The tensioning device **380** is constructed of a suitable material such as plastic and, preferably, comprises an injection molded, one piece body having a base plate **337**, an arm **347**, a spring member **349** connecting said arm **347** to the base **337** and grasping members **351** carried by the arm **347**.

The base plate **337** has anterior and posterior ends **381** and **382** and comprises two legs **383** with a slot **356** therebetween. The base **337** has an appropriate shape, as for example a vee shape as shown in FIG. 33, with the two legs **383** joined at the posterior end **382** of the base **337**.

The spring **349** is a linear spring comprising a ribbon shaped plastic member which is configured substantially as

a cee having ends which join the posterior base **382** to the arm **347** to form a continuous body as hereinbefore described. In the open position, the vertical distance between the anterior end **381** of the base **337** and the arm **347** ranges from 0.5–2.5", preferably being approximately 1.5". The spring **349** is constructed so as to provide increasing tension with increasing compression which results from moving the arm **347** towards the base **337**. Thus, as hereinafter described, the force of tension provided thereby ranges between 0.25–10 ounces, preferably between 0.5–2.5 ounces.

When the tensioning device **380** is set in the closed position so that the arm **347** and base **337** are disposed substantially parallel to one another, the spring **349** is under a force of tension of approximately 1 ounce. Movement of the arm **347** an additional 1 centimeter towards the base **337** increases the spring tension to approximately 2 ounces. Similarly, setting the tensioning member **380**, or movement of the patient, so that the arm **347** is disposed approximately 1 centimeter above a plane parallel with the base **337** provides a force of tension of approximately 0.5 ounces.

As shown in FIG. 33, the arm **347** has anterior and posterior ends **384** and **385**, the anterior end **384** carrying an enlarged, bulbous portion **386** having a slot **357** therein, the slot **357** being anteriorly-posteriorly disposed and substantially in alignment with the slot **356** in the base portion **337** when the tensioning member **380** is closed. The enlarged portion **386** is divided by the slot **357** into two grasping members **351** which are movable between open or release, and closed, or grasping, positions. When an elongate tubular member is disposed in the slot **357** and grasped by the grasping members **351** as hereinafter described, the grasping members **351** are biased into the closed position with a force approximating 5 ounces as a result of the slot **357** having a diameter that is slightly smaller than the diameter of either the first elongate tubular member **302** or the second elongate tubular member **503**.

The bias of the grasping members **351** is overcome, and the slot **357** thereby opened, by the use of actuator finger grips **387** which extend outwardly and posteriorly from the enlarged portion **386** of the anterior end **384** of the arm **347**. The grips **387** are provided with finger indentations **388** for use as hereinafter described.

Operation of the tensioning applicator **380** is similar to that of applicator **335**. By placing the applicator **380** against the patient's skin and urging the arm **347** towards the base **337** until the two are substantially parallel to one another and opening the grasping members **351** by pressing inwardly on the finger indentations **388** of the actuator grips **387** in order to grasp either the first or second elongate tubular member **302** and **503**, the tensioning applicator **380** can be set to approximately 1 ounce of tension as hereinbefore described.

The grasping members **351** are constructed to exert a maximum force of approximately 5 ounces so that a grasped elongate tubular member is permitted to slide between the grasping members **351** if a force of greater than approximately 5 ounces is longitudinally applied to the tubular member.

The remainder of the operation of the tensioning device **380** is as hereinbefore described.

Another embodiment of the expansile device is shown in FIG. 24. The expansile device **360** is very similar to that shown in FIG. 18 with the principal difference being that, in addition, it provides means for introducing a biological sealant into the puncture proximal to the expansile mechanism to seal the puncture. Thus all the parts of the expansile device **301** that are present in the expansile device **360** carry

the same numbers. The biological sealant introducer means **361** is carried by a flexible elongate tubular body **362** comprising first and second flexible elongate tubular members **302** and **363**. The first flexible elongate tubular member **302** is as hereinbefore described. The second flexible elongate tubular member **363** is formed of suitable plastic material, preferably an extruded thermoplastic elastomer such as Pebax™ having a shore hardness durometer of 50D or 72D. The second flexible elongate tubular member **363** has proximal and distal extremities **364** and **366**, extends along a longitudinal axis and has an inner wall **367** defining a lumen **368** extending from the proximal **364** to the distal extremity **366**. The lumen **368** has a diameter greater than the outer diameter of the first flexible elongate tubular member **302**. The first flexible elongate tubular member **302** is disposed or nested within the lumen **368** of the second flexible elongate tubular member **363** thereby defining a first, circumferential or annular space **369** between the outer surface of the first flexible elongate tubular member **302** and the inner wall **367** of the second flexible elongate tubular member **363**. The distal extremity **366** of the second flexible elongate tubular member **363** terminates proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**.

The second flexible elongate tubular member **363** is of a suitable size, as for example an outer diameter ranging from 0.020" to 0.050", an inner or lumen diameter ranging from 0.015" to 0.040" and has a suitable length as for example 10–160 centimeters. As hereinbefore discussed, the distal extremity **366** of the second flexible elongate tubular member **363** terminates proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**, as for example 1–15 millimeters up to several centimeters proximal.

Proximal adaption for sealant introduction into the flexible elongate tubular body **362** includes appropriate tee or wye adapters. Preferably, as shown in FIG. 24, a tee adapter **375** has one end fixed to the proximal extremity **364** of the second flexible elongate tubular member **363** using a suitable adhesive. The second end of the tee adapter **375** carries a compression fitting **376** in order to accommodate the proximal end **303** of the first flexible elongate tubular member **302** which is disposed within and extends proximally out of the tee adapter **375**. The compression fitting **376** provides a leakproof connection between the first and second flexible elongate tubular members **302** and **363** and enables removal of the second flexible elongate tubular member **363** while the first flexible elongate tubular member **302** is maintained in the deployed position. Introduction of sealants is accomplished via a fluid port **377** which communicates with the proximal end **364** of the second flexible elongate tubular member **363** as shown in FIG. 22. An alignment window **378** in the tee adapter **375** is provided which is used to visually align a marker **379** on the proximal extremity **303** of the first flexible elongate tubular member **302** or on the proximal extremity **318** of the push-pull wire **317** so that the distal extremity **366** of the second flexible elongate tubular member **363** is appropriately positioned proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309** as hereinbefore described.

Operation and use of the device **360** is similar to that described for the expansile device **301** except for the ability to introduce biological sealants with the device **360**. As soon as it has been established that a good seal has been formed between the occlusion assembly **307** and the wall **103** adjacent the puncture the operator can introduce the con-

stituents of the biological sealant into the fluid port **377** of the adapter **375** hereinbefore described. The sealant is then introduced into the proximal end **364** of the second flexible elongate tubular member **363** into the first space **369** between the outer surface of the first flexible elongate tubular member **302** and the inner wall **367** of the second flexible elongate tubular member **363**, thence exiting proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**. The remainder of the operation of the device **360** is as hereinbefore described in conjunction with the use of the device **21** and the device **301**.

Another embodiment of a expansile device incorporating the present invention is shown in FIGS. 25–26. The expansile device **401** is very similar to that shown in FIG. 24 with the principal difference being in the biological sealant means utilized in the device **401**. Thus all of the parts of the expansile device **360** that are present in the expansile device **401** carry the same numbers. The biological sealant means **402** is also similar to that shown in FIG. 24 with the principal difference being that the flexible elongate tubular body **362** further includes a third flexible elongate tubular member **403** formed of suitable plastic material, also preferably an extruded thermoplastic elastomer such as Pebax™ having a durometer of 63D or 72D. The third flexible elongate tubular member **403** has proximal and distal extremities **404** and **406**, extends along a longitudinal axis and has an inner wall **407** defining a lumen **408** extending from the proximal **404** to distal extremity **406** and having a diameter greater than the outer diameter of the second flexible elongate tubular member **363**. The second flexible elongate tubular member **363** is nested or disposed within the lumen **408** of the third flexible elongate tubular member **403** thereby defining a second, circumferential or annular space **409** between the second flexible elongate tubular member **363** and the inner wall **407** of the third flexible elongate tubular member **403**. The distal extremity **406** of the third flexible elongate tubular member **403** terminates distal to the distal extremity **366** of the second flexible elongate tubular member **363** and proximal to the distal extremity **304** of the first flexible elongate tubular member **302** thereby defining an annular distal mixing chamber **411** between the first flexible elongate tubular member **302** and the inner wall **407** of the third flexible elongate tubular member **403**.

The third flexible elongate tubular member **403** is of a suitable size, as for example an outer diameter ranging from 0.030" to 0.070", and has a suitable length as for example 10–160 centimeters. As hereinbefore discussed, the distal extremity **406** of the third flexible elongate tubular member **403** terminates distal to the distal extremity **366** of the second flexible elongate tubular member **363**, as for example from 1–15 millimeters distal, preferably 5 millimeters, thus creating the distal mixing chamber **411**. The distal extremity **406** of the third flexible elongate tubular member **403** also terminates proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**, as for example 1–15 millimeters up to several centimeters proximal. In order to affect this configuration, the second flexible elongate tubular member **363** may be of a suitable length that is slightly shorter than the length of the second flexible elongate tubular member **363** in device **360**.

Proximal adaption for sealant introduction into this triple flexible elongate tubular member body is provided so that either the second flexible elongate tubular member **363** or the second and third flexible elongate tubular members **363**

and **403** can be reversibly disengaged and removed. Removing the second flexible elongate tubular member **363** provides access to a larger space between the first and third flexible elongate tubular members **302** and **403** in order to provide for more reliable aspiration attempts. Removing both the second and third flexible elongate tubular members **363** and **403** provides for use of the isolated expansile device **301** as hereinbefore discussed, and also permits cleaning of the removed tubular members as necessary.

The proximal adaption for the device **401** includes appropriate tee or wye adapters as hereinbefore described. The proximal adaption **375** for the second flexible elongate tubular member **363** is similar to the proximal adaption **375** for the second flexible elongate tubular member **363** in device **360**. The third flexible elongate tubular member **403** carries similar proximal adaption **412** in the form of a tee adapter **412**, compression fitting **413** and a fluid port **414** so that, as hereinbefore discussed, the second flexible elongate tubular member **363** can be disposed or nested within the third flexible elongate tubular member **403** with a proximal seal between the two members that is fluid-tight. A second sealant or component thereof can be introduced into the fluid port **414** of the compression fitting **413** on the third flexible elongate tubular member **403** as hereinafter discussed.

In addition, the proximal adapter **412** of third flexible elongate tubular member **403** carries an alignment window **416** in order to permit the operator to visually align a marker **417** on the second flexible elongate tubular member **363** within the window **416** so that during use the second and third flexible elongate tubular members **363** and **403** are appropriately positioned with respect to one another. It should be appreciated that second and third flexible elongate tubular members **363** and **403** can be constructed as a single unit whereby only the unit is capable of being inserted and removed over the first flexible elongate tubular member.

Operation and use of the device **401** is similar to that described for the expansile device **360** except for use of the biological sealant means **402** in the device **401**. As soon as it has been established that a good seal has been formed between the occlusion assembly **307** and the wall **103** adjacent the puncture the physician can introduce the constituents of the biological sealant into the fluid port **377** of the adapter **375** on the proximal end **364** of the second flexible elongate tubular member **363** into the first space **369** and into the fluid port **414** of the adapter **412** on the proximal end **404** of the third flexible elongate tubular member **403** into the second space **409** respectively, causing the constituents to travel separately, distally into the distal mixing chamber **411** where they are well mixed and whence the mixed sealant exits proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**. The remainder of the operation of the device **401** is as hereinbefore described in conjunction with the use of the device **21**.

Another embodiment of a expansile device incorporating the present invention is shown in FIGS. 27-30. The expansile device **418** is also very similar to that shown in FIG. 24 with the principal difference being in the biological sealant means **419** utilized in the device **418**. Thus all of the parts of the expansile device **360** that are present in the expansile device **418** carry the same numbers.

The second flexible elongate tubular member **363** of the device **418** is provided with an additional or second lumen **425** which may be half-circular in cross-section, is laterally disposed and also extends from the proximal extremity **364** to the distal extremity **366** of the second flexible elongate tubular member **363** as shown in FIG. 27. In order for the

second flexible elongate tubular member **363** to carry the second lumen **425**, the first lumen **368** may also be laterally disposed. The second lumen **425** has a suitable chord length ranging from 0.020" to 0.040".

The second lumen **425** of the device **418** may be utilized for introducing biological sealants as hereinbefore described in conjunction with the device **360**. The second lumen **425** can also be used for aspiration attempts, to verify formation of a good seal between the expansile assembly **307** and the wall **103** of the vessel **107** as hereinbefore described in conjunction with the device **21**.

The expansile device **418** is also provided with a third flexible elongate member **430** having proximal and distal extremities **431** and **432** and extending along a longitudinal axis. Shown in FIGS. 27-28 and FIG. 30, the third flexible elongate member **430** is sized and shaped to be reversibly, frictionally disposed within the second lumen **425** of the second flexible elongate tubular member **363** and has a length substantially equal to the length of the second flexible elongate tubular member **363**.

The third flexible elongate member **430** is similarly formed of a suitable plastic material such as Pebax™ and is solid in construction, as shown in FIG. 28, so that it functions as an obturator for the second lumen **425** of the second flexible elongate tubular member **363**, thus keeping the same unobstructed until ready for use.

There is provided an alternate third flexible elongate member **433** which is similarly sized and shaped and functions as a biological sealant introducer means. As shown in FIGS. 27 and 30, this alternate third flexible elongate member **433** carries first and second lumens **434** and **436**, each extending from the proximal to the distal extremity **431** and **432** of the alternate third flexible elongate member **433**. A mixing chamber **437** contiguous with and created by the distal confluence of the first and second lumens **434** and **436** is carried by the distal extremity **432** of the third flexible elongate member **433**. Alternatively, the third flexible elongate member **433** can be without the aforementioned distal confluence of lumens and, in place thereof, have a length slightly shorter than that of the second flexible elongate tubular member **363** so that a mixing chamber **437** is created within the distal end **366** of the second flexible elongate tubular member **363**.

Proximal adaption **438** for sealant introduction into this third flexible elongate member **433** is provided as shown in FIG. 27. The proximal extremity **431** of the third flexible elongate member **433** carries a fitting or adapter **438** having two or more fluid ports **439** in alignment with the first and second lumens **434** and **436** of the third flexible elongate member **433**. The fitting **438** is constructed out of a suitable material such as plastic or nylon, by way of example, polycarbonate or Isoplast™, and is bonded to the third flexible elongate member **433** by an appropriate adhesive. Alternatively, the adapter **438** can be constructed of Pebax™ 82D, and be heat fused to the proximal end **431** of the third flexible elongate member **433**. It should be appreciated that the adapter **438** may be constructed so as to be reversibly connected to the third flexible elongate member **433**.

Operation and use of the device **418** is similar to that hereinbefore discussed in conjunction with the device **401**. Constituents of biological sealants are introduced proximally into the adapter **438** and thence into the first and second lumens **434** and **436** causing the constituents to travel separately, distally into the distal mixing chamber **437** where they are well mixed and whence the mixed sealant exits proximal to the distal extremity **304** of the first flexible elongate tubular member **302** and adjacent to the expansile mechanism **309**.

Alternately, as shown in FIGS. 31–32, a third flexible elongate tubular member 450 is provided which, other than being tubular in shape, is similar in construction to the alternate third flexible elongate members hereinbefore discussed. This third flexible elongate tubular member 450 is also sized to be frictionally disposed within the second lumen 425 of the second flexible elongate tubular member 363 in which case the area in the second lumen 425 of the second flexible elongate tubular member 363 surrounding the third flexible elongate tubular member 450 is used as a second space 451 into which biological sealants are introduced as hereinafter discussed.

Proximal adaption for sealant introduction into the second lumen 425 of the second flexible elongate tubular member 363 and the third flexible elongate tubular member 450 is provided as shown in FIG. 31. The proximal extremity 364 of the second flexible elongate tubular member 363 carries a fitting or adapter 452 constructed in a manner similar to that hereinbefore discussed. The adapter 452 has proximal and distal ends 453 and 454 and carries a variably-shaped lumen 456 extending therethrough. The distal end 454 of the adapter lumen 456 is sized, configured and aligned with the second lumen 425 of the second flexible elongate tubular member 363. The proximal end 453 of the adapter lumen 456 is circular in cross-section and is sized so as to frictionally accept the third flexible elongate tubular member 450. A fluid port 457 is connected to the adapter lumen 456. As shown in FIG. 31, the proximal end 431 of the third flexible elongate tubular member 450 also carries a fluid port 458. The third flexible elongate tubular member 450 is of a slightly shorter length than that of the second flexible elongate tubular member 363 in order to create the distal mixing chamber 437 as hereinbefore discussed. Operation and use is as hereinbefore described.

Alternatively, instead of utilizing a third flexible elongate member the second flexible elongate tubular member of the expansile device is provided with a third lumen (not shown) extending from the proximal to the distal extremity and. A mixing chamber contiguous with and created by the distal confluence of the second and third lumens and is carried by the distal extremity of the second flexible elongate tubular member. Proximal adaption for sealant introduction and a handle assembly can be utilized as hereinbefore discussed. Operation and use is as hereinbefore described.

Another embodiment of an expansile device incorporating the present invention is shown in FIGS. 34–36. The expansile device 701 contains elements similar to those present in the device 301. Thus all parts present in the device 701 that are present in device 301 carry the same numbers. The device 701 differs from the device 301 in that the closure assembly 307 of the device 701 carries an expansile member 309 constructed of an additional segment 702 of nitinol tubing having proximal and distal ends 703 and 704 which has been adhesively bonded or annealed to the distal extremity 304 of the flexible elongate tubular member 302. The additional nitinol segment 702 is of appropriate dimensions, having inner and outer diameters approximating those of the flexible elongate tubular member 302 and having a length ranging from 0.020–0.060". The segment 702 is provided with a plurality of circumferentially spaced apart longitudinally extending slits 706 of a suitable number, preferably eight. The slits 706 form arms or arcuate segments 707 which when the expansile assembly 307 is in a contracted position lie in a generally cylindrical configuration 708 which is in alignment with the longitudinal axis of the flexible elongate tubular member 302 and in an expanded position 709 extend radially from the longitudinal

axis as hereinafter described. The distal end 704 of the additional segment 702 preferably carries a short hypotube segment 711 to which it is appropriately bonded.

The distal end 319 of the push-pull wire 317 of device 701 is coupled or secured to the distal end 704 of the additional segment 702 by being soldered or adhesively bonded to the hypotube segment 711. Alternatively, the distal end 319 of the push-pull wire 317 may extend slightly distal of the distal extremity 304 of the flexible elongate tubular member 302 in which case it carries a small flange 712, the diameter of which approximates the outer diameter of the additional segment 702 and the hypotube segment 711, and the flange 712 is secured to the tip of the distal end 704 of the additional segment 702 by being bonded to the hypotube 711 as hereinbefore described.

The rim 332 of the membrane 311 is affixed exteriorly to the proximal end 703 of the nitinol segment 702, proximal of the slits 706 therein. In lieu of having a closed end as in the device 301, the membrane 311 of device 701 has an open distal end which is circumferentially affixed exteriorly to the distal end 704 of the nitinol segment 702 distal of the slits 706 therein.

The proximal extremity 303 of the flexible elongate tubular member 302 carries deployment means 308 for controlling movement of the expansile member 309 between contracted, or cylindrical configurations 708, and a plurality of predetermined expanded configurations 709 of varying sizes, one of which is shown in FIG. 36.

The deployment means 308 includes a handle housing 751 having proximal and distal ends 752 and 753 and having a lumen 754 which is circular in cross section and extends from the proximal 752 to the distal end 753 of the housing 751. The lumen 754 in the housing 751 is sized so as to accommodate the push-pull wire 317 which is disposed therein as hereinafter described. The housing 751 is molded of a suitable material such as Polycarb™ and carries a display window 756 for displaying the size of a predetermined expanded configuration as hereinafter described.

The distal end 753 of the housing 751 carries a slot 757 which is formed by a circumferential enlargement of the lumen 754. The slot 757 has concentric proximal and distal portions 758 and 759, the distal portion 759 having a diameter which is smaller than the diameter of the proximal portion 758 and slightly larger than the outer diameter of the flexible elongate tubular member 302 thereby providing the distal end 753 of the housing 751 with a circumferential, inwardly extending rim or collar 761 which is rotatably coupled to the proximal extremity 303 of the flexible elongate tubular member 302 as hereinafter described.

The portion of the lumen 754 in the proximal end 752 of the housing 751 is threaded to engage the proximal end 318 of the push-pull wire 317 as hereinafter described. Alternatively, the proximal end 752 of the housing 751 can carry a threaded insert 762 made of a suitable material, preferably stainless steel, and having a lumen extending therethrough and aligned with the lumen 754 of the housing 751. The insert 762 may be bonded to the housing 751 by using an appropriate adhesive or be frictionally retained therein.

As shown in FIG. 34, a fitting 766, preferably made of stainless steel, is adhesively, coaxially mounted over and extends proximally beyond the proximal extremity 303 of the flexible elongate tubular member 302. The fitting 766 carries a lumen 767 aligned with the lumen 306 of the flexible elongate tubular member 302 and is provided with a flanged proximal end 767 which is retained within the slot 757 of the housing 751 and seats against the collar 761

therein so that the housing 751 is rotatably coupled to the flexible elongate tubular member 302 as hereinafter described. The portion of the fitting 766 extending proximally, beyond the proximal extremity 303 of the flexible elongate tubular member 302, is provided with an inwardly extending pin or key 769 so as to be capable of slidingly engaging the push-pull wire 317 as hereinafter described.

The proximal end 318 of the push-pull wire 317 in the device 701 is provided with threads which engage the threaded portion of the lumen 754 in the proximal end 752 of the housing 751. Distal to the threads, the push-pull wire 317 is provided with a longitudinal groove or channel 771 which engages or mates with the key 769 of the fitting 766, as hereinbefore described, so that when the housing 751 is rotated on the push-pull wire 317 and the fitting 766 carried by the flexible elongate tubular member 302, the push-pull wire 317 and the expansile member 309 do not rotate. The portion of the proximal end 318 of the push-pull wire 317 distal to the threads and proximal to the fitting 766 carries numbers representing the sizes of the various predetermined expanded configurations and which are displayed through the display window 756 in the handle housing 751. It should be appreciated that the proximal end 318 of the push-pull wire 317 can be constructed so as to be thicker than the more distal sections with the wire 317 being tapered distal to the key 769 of the fitting 766 as shown in FIG. 34. The proximal end 318 of the push-pull wire 317 is, preferably, also provided with a cap or flange 772 constructed of a suitable plastic or metal material for preventing distal travel of the wire 317 into the housing 751.

Operation and use of the device 701 is similar to that described for the expansile device 301 except for use of the deployment means in device 701. Before the expansile member 309 is deployed to a predetermined expanded position 709, the housing 751 has been rotated on the push-pull wire 317 to its distal-most position and the expansile member 309 is thus in its cylindrical configuration 708. When it is desired to move the expansile assembly 307 to a predetermined expanded configuration 709, the proximal end 318 of the push-pull wire 317 is held with one hand while the handle housing 751 is rotated clockwise on the push-pull wire 317 using the operator's other hand. Clockwise rotation of the housing 751 on the push-pull wire 317 causes pulling on the wire 317 to apply compressive forces to the nitinol additional segment 702 to cause outward bowing or folding of the arms 707 at their mid-points so that the arms 707 extend radially from the longitudinal axis of the flexible elongate tubular member 302. The membrane 311 is carried along with and expanded by the arms 707 so that, as hereinbefore described, it is disposed on both sides of the radially expanded arms 707. The expansile member 309 may be deployed to a predetermined configuration with a specific size by observing the size markers or numbers on the wire 317 in the display window 756. The larger the desired size of expansion, the more the operator rotates the housing 751 clockwise on the push-pull wire 317 while observing the display window 756.

After occlusion of a puncture, the expansile assembly 307 is de-deployed by reversing the rotation of the housing 751 on the wire 317. This releases the compressive forces on the nitinol additional segment 702 which seeks its memorized cylindrical configuration 708 by effecting an inward collapsing of the radially extending arms 707. Thereafter, the closure device 701 can be retracted in a manner similar to that hereinbefore described with respect to other embodiments. It should also be appreciated that the additional

nitinol segment can be annealed so that the memorized configuration is, alternatively, the expanded configuration. In this case the contracted, cylindrical configuration is obtained with longitudinal stretching forces being applied to the segment by the housing and the wire.

It is apparent from the foregoing that there has been provided an expansile or closure device and method for percutaneous access and occlusion of punctures which medical procedures have required being placed in the human body. By varying the free shape or configuration of the super elastic alloy expansile member and the size and material of the membrane, the predetermined configuration and rigidity of the expansile assembly is varied so that it becomes possible to occlude puncture sites and natural tracts of various sizes and in various locations in the body such as laparoscopic puncture sites, pleural-cutaneous fistulas, including chest-tube puncture sites, intestinal-cutaneous fistulas, fistulas between the intestines, biliary tract of the stomach and the like. The expansile assembly establishes the distal boundary for the puncture so that it enables accurate placement of and prevents inadvertent intravascular injection and embolization of the biological sealant. The expansile device of the present invention makes possible the use of biological sealants in which for example fibrin glue is utilized and forms a clot which has greater strength than a natural clot formed by the body. In addition it makes it possible to the bypass the natural coagulation system of the human body even though anticoagulants have been administered to the patient during the prior medical procedure or procedures. Although fibrin glue has been discussed as the principal biological sealant, other sealants may be utilized such as collagen, Avitene™ slurries, Gel Foam™, cellulose, fibrin and thrombin, collagen and thrombin mixtures, all of which are non-adherent to the expansile device. Individual components of multi-component sealants may be separately introduced into the different annular spaces of the expansile device comprising three flexible elongate tubular members. By utilizing an annular distal mixing chamber, component-to-component fluid contact is maximized. A maximized area of contact affords optimal mixing and setting of the sealant at just the site where it is needed. Furthermore, circumferential introduction of mixed biological sealant into the puncture provides better distribution. In addition, it should be appreciated that other means of sealant introduction to the flexible elongate tubular member are available. For example, a multi-component sealant such as fibrin glue may, alternatively, be mixed prior to introduction into the flexible elongate tubular member.

The shape of the expansile mechanism utilized in the expansile device of the present invention that abuts the inner surface of the wall through which the puncture extends enlists the normal pressure of the arterial blood flow to help retain the expansile assembly in contact with the wall. The expansile assembly is small in size and even when being deployed into the blood vessel permits substantially unobstructed blood flow through the vessel to continue during the expansile procedure thus avoiding ischemic and thrombotic complications associated with stasis of blood. The small size similarly prevents the expansile assembly from damaging or impinging on the opposite wall of the blood vessel during deployment or de-deployment of the device.

Since the expansile device and method of the present invention does not require long term intravascular deployment of a foreign body such as collagen, intra-arterial anchors or sutures, nor does it utilize balloon technology with the attendant risks of balloon rupture or tearing, there is a greatly reduced risk of life and limb threatening infec-

tions and the introduction of particulates or air emboli into the bloodstream.

The catheter retention and tension applicator of the present invention provide a constant force of proximal tension on the deployed device. An inherent safety feature is the constant force of tension provided over a range of motion as hereinbefore discussed. In other situations, it is desirable that the tension vary over a range of motion. An embodiment of the tensioning device accomplishes this while maintaining inherent safety features as hereinbefore described. As this obviates the need for manual pressure and clamping devices traditionally used, it frees medical personnel to attend to other duties.

Since the occlusions which are formed in punctures utilizing the expansile device and method of the present invention can be accomplished quickly, this facilitates early ambulation of the patient and helps to avoid traditional complications such as arterio-venous fistulas, pseudoaneurysms, thrombosis and embolism. Since the device is typically disposed of after one use, the danger of transmitting diseases to the blood stream of the patient is greatly reduced. Medical costs to the patient and to society are also thereby reduced.

Although the expansile device and method have been described principally in use with the human body it should be appreciated that the expansile device and method also can be utilized with animals in a similar manner.

In addition, it should be appreciated that the expansile device can be used within other natural tracts in the body in order to provide for other therapeutic or prophylactic modalities.

It is apparent from the foregoing that there has been provided a expansile device and method for percutaneous access and occlusion of puncture sites in the human body that have distinct advantages over those heretofore provided.

Percutaneous methods are widespread techniques that offer less invasive, safer and more cost-effective diagnostic and therapeutic access to organs of the human body. In order to fully realize the advantages of percutaneous access however, morbidity associated with access sites must be anticipated and prevented wherever possible. Indeed, advanced therapeutic interventions have led to a greater range of access site complications. A patient who suffers such complications must often undergo a more invasive procedure in order to prevent devastating injury to life or limb. Such procedures incur additional risks and costs. Effective percutaneous occlusion of a percutaneous vascular access site that proves to be otherwise difficult to manage is a major achievement. Without such treatment many of the advantages of percutaneous diagnostic and therapeutic procedures are lost. Satisfactory solutions have heretofore been absent in the prior art. The device and method of the present invention obviate many of the morbid side effects associated with puncture sites hereinbefore described.

What is claimed is:

1. A device for use by a human hand for expansion within a blood vessel having a wall defining a lumen in the body comprising an elongate tubular member having proximal and distal extremities and having a longitudinal axis, an expansile member carried by the distal extremity of the elongate tubular member and movable between contracted and expanded positions, a deformable membrane covering at least a portion of the expansile member, a handle mechanism adapted to be grasped by the human hand and a push-pull element extending through the elongate tubular member and having a distal extremity coupled to the expansile member and a proximal extremity coupled to said handle mechanism,

said handle mechanism being movable independently relative to said push-pull element so that operation of said handle mechanism causes longitudinal movement of said push-pull element to cause movement of said expansile member between the contracted and expanded positions.

2. A device as in claim 1 wherein the expansile member has proximal and distal extremities, the distal extremity of the push-pull element being secured to the distal extremity of said expansile member.

3. A device as in claim 2 wherein said expansile member in a contracted position includes a plurality of circumferentially spaced apart longitudinal slits forming arms which when the expansile member is in an expanded position extend radially from the longitudinal axis of the elongate tubular member.

4. A device as in claim 3 wherein said expansile member has at least eight circumferentially spaced apart longitudinal slits.

5. A device as in claim 3 wherein said expansile member has a plurality of predetermined expanded configurations.

6. A device as in claim 5 wherein said plurality of predetermined configurations are of varying sizes.

7. A device for expansion within a blood vessel having a wall defining a lumen in the body comprising a first elongate tubular member having proximal and distal extremities and having a longitudinal axis, an expansile member carried by the distal extremity of the first elongate tubular member and movable between contracted and expanded positions, said expansile member having a predetermined configuration in the expanded position, a deformable membrane covering the expansile member, said deformable membrane being sized so as to be capable of overlying and underlying the expansile member in the expanded position and deployment means carried by the proximal extremity of the first elongate tubular member and adapted to be operated by the human hand for controlling movement of the expansile member between the contracted and expanded positions, said deployment means including a push-pull wire having proximal and distal extremities, said push-pull wire extending through the first elongate tubular member and being coupled to the expansile member, the expansile member having proximal and distal extremities, the distal extremity of said push-pull wire being secured to the distal extremity of said expansile member, said expansile member including a plurality of circumferentially spaced apart slits forming arms which when the expansile assembly is in a contracted position lie in a generally cylindrical configuration which is in alignment with the longitudinal axis of the first elongate tubular member and in an expanded position extend radially from the longitudinal axis, said expansile member having a plurality of predetermined expanded configurations, said plurality of predetermined configurations being of varying sizes and a display carried by the deployment means for displaying the size of a predetermined expanded configuration.

8. A device as in claim 6 wherein said expansile member is comprised essentially of a superelastic material.

9. A device as in claim 6 wherein said expansile member is comprised of Nitinol tubing.

10. A device as in claim 1 further including means for applying tension to maintain engagement of said expansile member in the expanded position with the wall in the lumen of the blood vessel.

11. A device as in claim 10 wherein said tension means includes a tensioning member having a base portion, an arm movable between open and closed arm positions with respect to said base portion, a spring member connecting said arm to said base portion, said spring member biasing

35

said arm into the open arm position, at least two cooperative grasping portions carried by said arm and movable between disengaging and engaging positions for grasping said elongate tubular member, said grasping portions being yieldably biased toward said engaging position.

12. A device as in claim 11 wherein said spring is capable of exerting a force ranging from 0.5–4 ounces of tension, said force varying with movement of said arm between open and closed arm positions.

13. A device as in claim 11 wherein said spring, arm and base are constructed of one piece.

14. A device as in claim 11 wherein said tensioning member is constructed of one piece.

15. A device as in claim 11 further including a first slot in the base and a second slot in the arm which is aligned with the first slot when the arm is in the closed position, said elongate tubular member being disposed in said first and second slots when grasped by said grasping portions.

16. A device for expansion within a blood vessel having a wall defining a lumen in the body comprising an elongate tubular member having proximal and distal extremities, an expansile member carried by the distal extremity of the elongate tubular member and movable between contracted and expanded configurations, a deformable membrane covering at least a portion of the expansile member, deployment means carried by the proximal extremity of the elongate tubular member for controlling movement of the expansile member between the contracted and expanded configurations and a display carried by the deployment means for displaying the size of said expanded configuration.

36

17. A device for expansion within a blood vessel having a wall defining a lumen in the body comprising an elongate tubular member having proximal and distal extremities, an expansile member carried by the distal extremity of the elongate tubular member and movable between contracted and expanded positions, a deformable membrane covering at least a portion of the expansile member, deployment means carried by the proximal extremity of the elongate tubular member for controlling movement of the expansile member between the contracted and expanded positions and a handle adapted to be held by the human hand and coupled to said deployment means, said handle being rotatable independently of said deployment means during movement of the expansile member between contracted and expanded positions.

18. A device for expansion within a blood vessel having a wall defining a lumen in the body comprising an elongate tubular member having proximal and distal extremities and a longitudinal axis, an expansile member carried by the distal extremity of the elongate tubular member and movable between contracted and expanded positions, a deformable membrane covering at least a portion of the expansile member, deployment means carried by the proximal extremity of the elongate tubular member for controlling movement of the expansile member between the contracted and expanded positions, a handle adapted to be held by the human hand and coupled to said deployment means, said handle and said deployment means being movable independently of one another.

* * * * *