



(51) International Patent Classification:

A61B 5/055 (2006.01) *G01R 33/36* (2006.01)
A61B 5/302 (2021.01) *G01R 33/565* (2006.01)
A61B 5/00 (2006.01) *G01R 33/567* (2006.01)
G01R 33/3415 (2006.01)

(21) International Application Number:

PCT/EP2020/087584

(22) International Filing Date:

22 December 2020 (22.12.2020)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

19219362.1 23 December 2019 (23.12.2019) EP

(71) Applicant: **KONINKLIJKE PHILIPS N.V.** [NL/NL];
High Tech Campus 52, 5656 AG Eindhoven (NL).

(72) Inventors: **LEUSSLER, Christoph, Günther**; c/o Philips
International B.V. Intellectual Property and Standards High
Tech Campus 5, 5656 AE Eindhoven (NL). **WIRTZ,**
Daniel; c/o Philips International B.V. Intellectual Property
and Standards High Tech Campus 5, 5656 AE Eindhoven
(NL). **SENEGAS, Julien, Thomas**; c/o Philips International
B.V. Intellectual Property and Standards High Tech Cam-
pus 5, 5656 AE Eindhoven (NL).

(74) Agent: **PHILIPS INTELLECTUAL PROPERTY &
STANDARDS**; High Tech Campus 5, 5656 AE Eindhoven
(NL).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,

(54) Title: RF COIL WITH INTEGRATED VITAL SIGNS DETECTOR

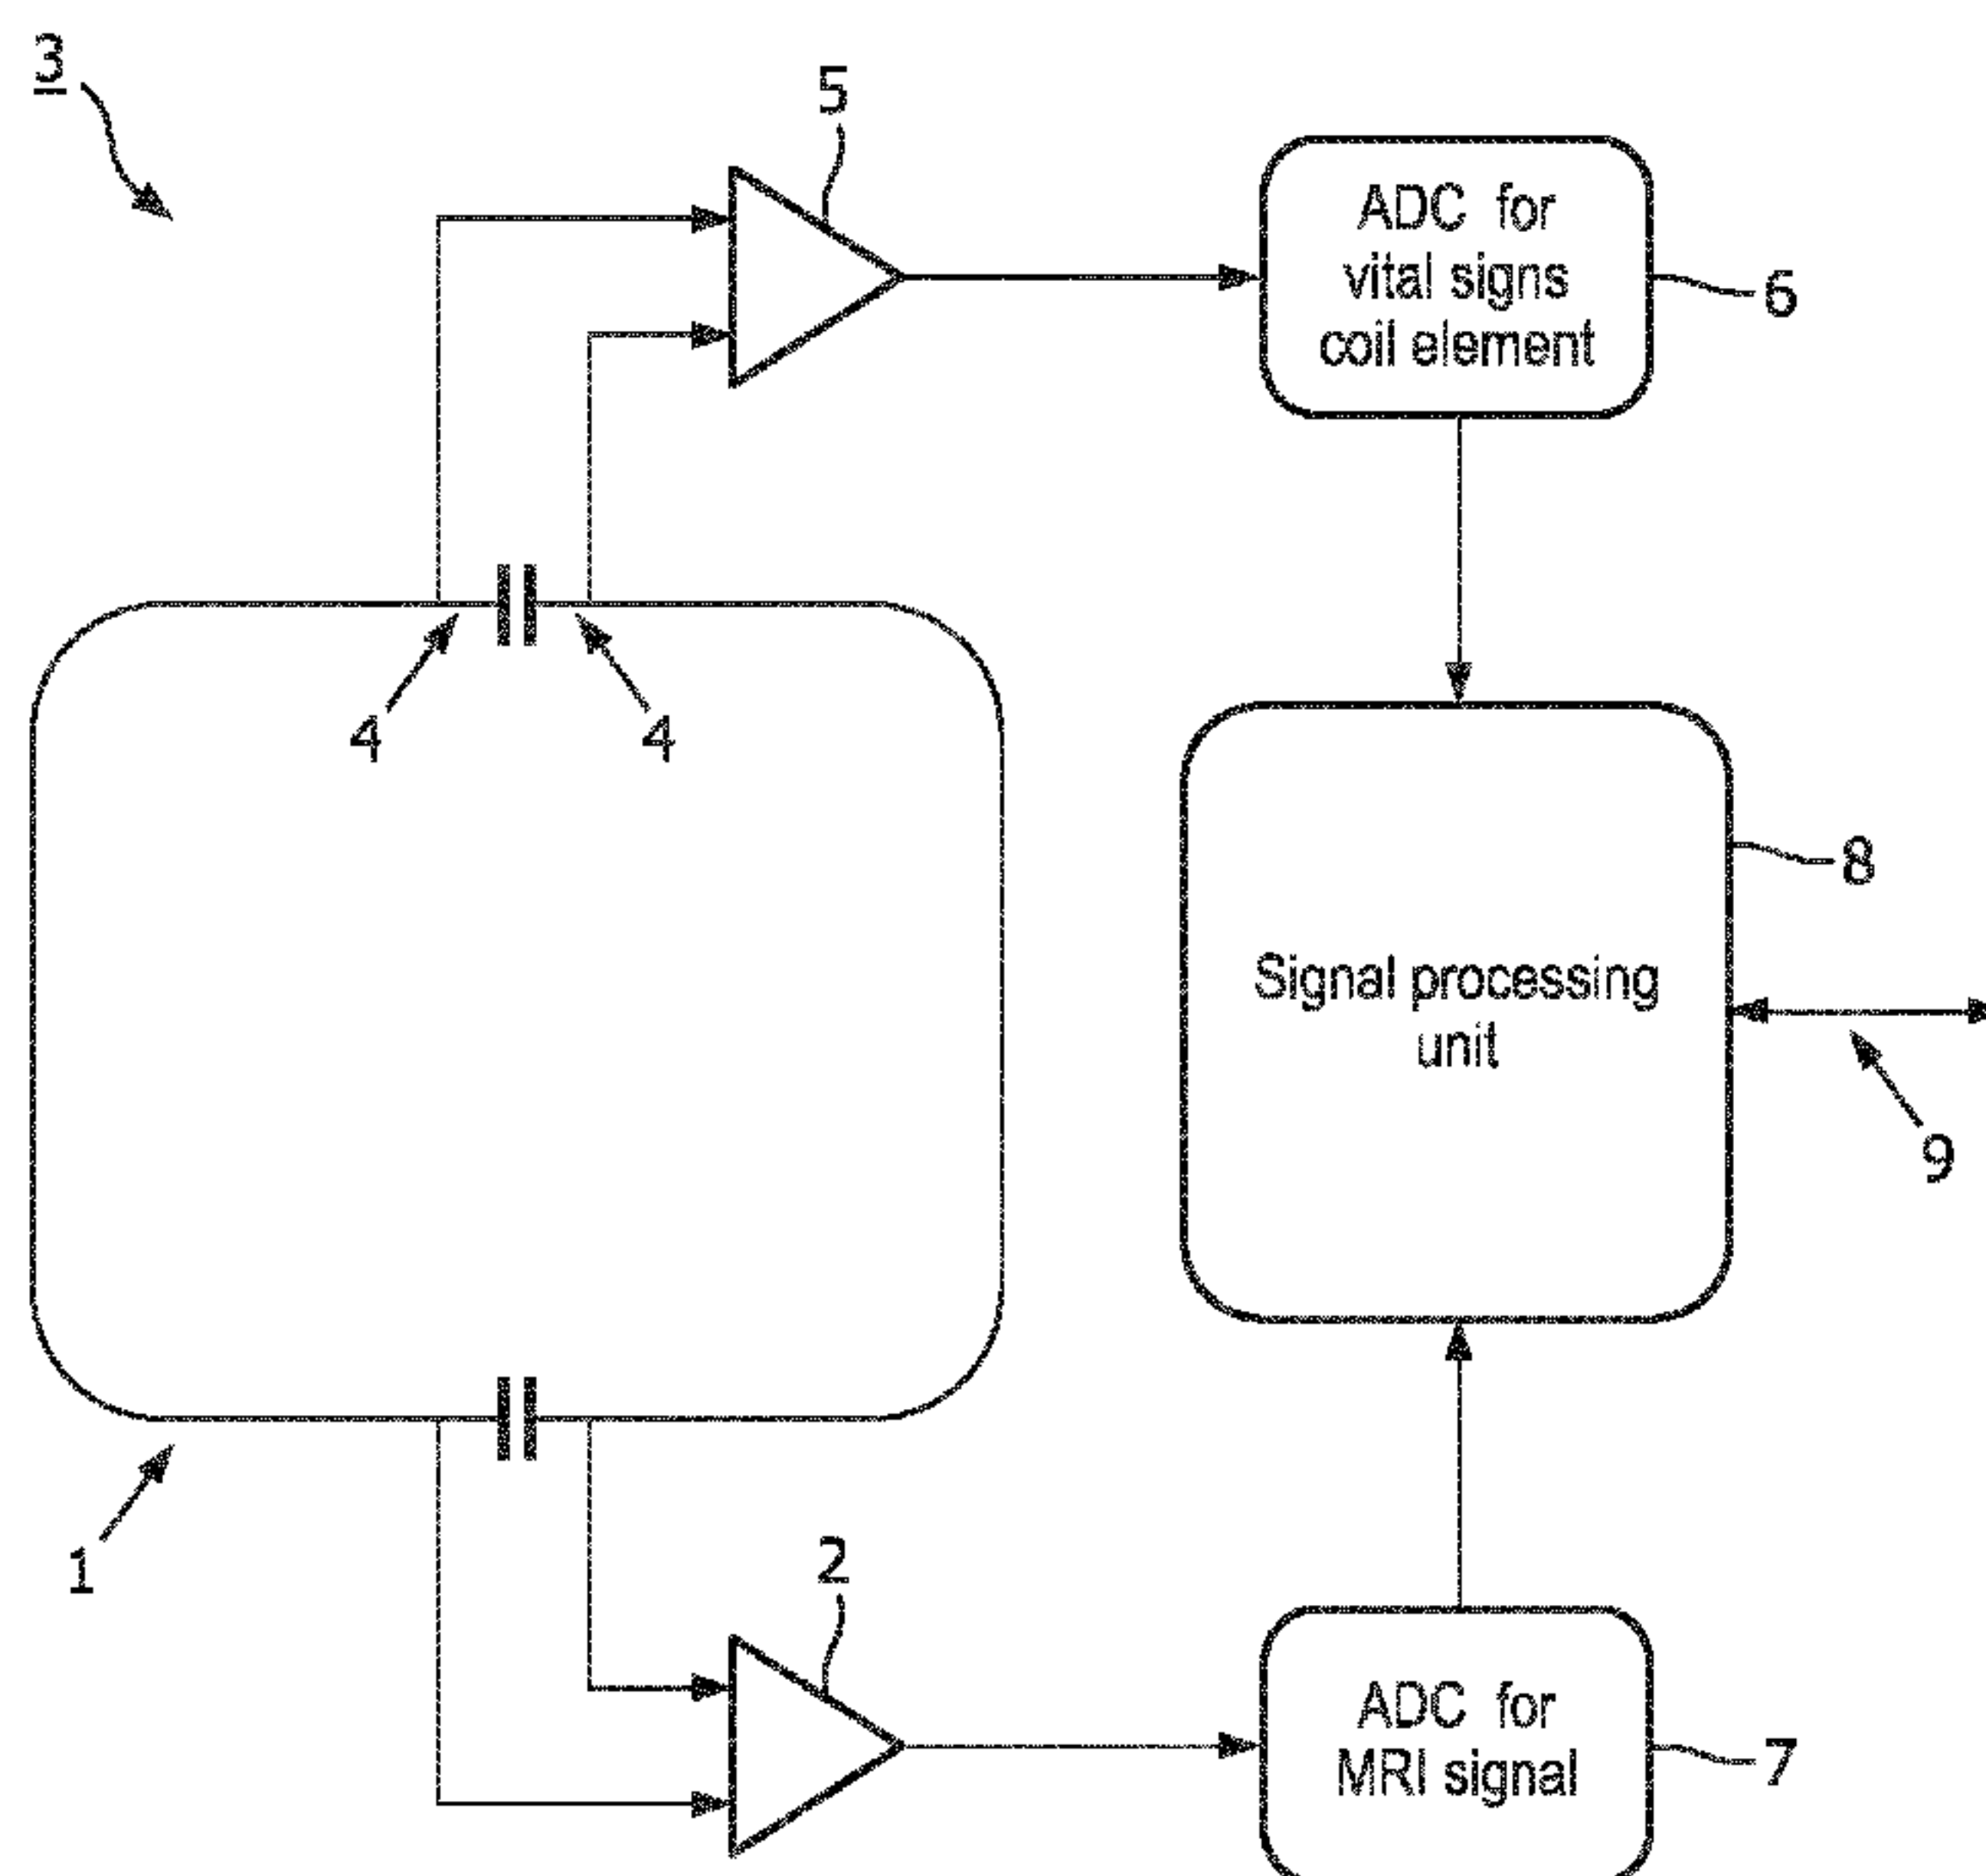


FIG. 1

(57) Abstract: It is an object of the invention to provide a radio frequency (RF) transmit- receive coil (1) for a magnetic resonance (MR) imaging system with an integrated vital signs detector (3) for the detection of vital signs of a patient within the magnetic resonance (MR) imaging system, whereby contact sensors directly attached to the body of the patient, are replaced by a contactless system for monitoring vital signs, which makes it much easier to measure vital signs of the patient. The object is achieved by a RF transmit-receive coil (1) comprising a vital signs detector (3) wherein the vital signs detector (3) is integrated in the RF transmit-receive coil (1), wherein a pair of electrically conducting coil elements (4) of the RF transmit-receive coil (1) forms the vital signs detector (3), wherein the vital signs detector (3) is a capacitive vital signs detector (3), the capacitive vital signs detector (3) being adapted for receiving capacitive vital signs signals. The present invention also concerns a system for the detection of vital signs of a patient within a magnetic resonance

CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, IT, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) Designated States *(unless otherwise indicated, for every kind of regional protection available):* ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

(MR) imaging system, a method for operating the system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system, a software package for a magnetic resonance (MR) imaging system and a software package for upgrading a magnetic resonance (MR) imaging system.

Rf coil with integrated vital signs detector

FIELD OF THE INVENTION

The invention relates to the field of radio frequency (RF) transmit-receive coils for a magnetic resonance (MR) imaging system and in particular to a RF transmit-receive coil with an integrated vital signs detector. The invention also relates to a system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system, to a method for operating the system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system, a software package for a magnetic resonance (MR) imaging system and a software package for upgrading a magnetic resonance (MR) imaging system.

BACKGROUND OF THE INVENTION

High quality triggering in medical imaging (especially MR) is vital for a large number of examinations, e.g. cardiac-, abdominal- or pelvis-imaging. Only with good quality trigger signals the imaging sequence can be carried out at equal expiration states or equal points during the cardiac cycle resulting in superior image quality. Typically, vital signs are recorded using dedicated sensors, which are expensive as well as prone to errors and misplacements. Today, the ECG is used to determine the heartbeat and therewith trigger the imaging device. However, the ECG requires additional effort in preparing the patient (mount and wire electrodes, connect and activate the wireless transmitter). Capacitive electrodes for the evaluation of human body bioelectric potentials are a very attractive alternative to conventional galvanically coupled electrodes for diagnostic applications especially when the signals have to be measured through insulating materials like cloth, which would greatly simplify the current procedure

Capacitive type electrodes are able to detect bio potentials with an explicit gap between the sensor and the body, even through hair and clothing. Compared to standard conductive type electrodes, the surface of these electrodes is electrically insulated and thus remains stable even in long-term applications. The sensor's metal electrode and the body surface are capacitively coupled, forming a capacitance. As such, the capacitive type electrodes detect the so-called displacement current I_D , posited by J. C. Maxwell to explain

magnetic fields around a capacitor, which is proportional to the rate of change of the electric field associated with the ECG signal.

From the document EP2020916 A2 a wireless patient monitor for MRI is known wherein a patient, supported on a movable table, may be positioned outside the bore of the magnet to receive a wireless patient monitor receiving signals from the patient by leads. The patient may then be moved into the bore of the magnet with the wireless patient monitor allowing for continuous monitoring of the patient. The wireless patient monitor may incorporate its own power supply to transmit the monitored signals from the patient via radio transmitted signal or the like to a base station positioned near the magnet but outside of the bore. However, the patient monitor requires additional effort in preparing the patient e.g. mounting and wiring electrodes and connecting the wireless transmitter.

SUMMARY OF THE INVENTION

It is an object of the invention to provide a radio frequency (RF) transmit-receive coil for a magnetic resonance (MR) imaging system with an integrated vital signs detector for the detection of vital signs of a patient within the magnetic resonance (MR) imaging system, whereby contact sensors directly attached to the body of the patient, are replaced by a contactless system for monitoring vital signs, which makes it much easier to measure vital signs of the patient.

According to the invention, this object is addressed by the subject matter of the independent claims. Preferred embodiments of the invention are described in the sub claims.

Therefore, according to the invention, a radio frequency (RF) transmit-receive coil for a magnetic resonance (MR) imaging system is provided, the RF transmit-receive coil comprising a vital signs detector for the detection of vital signs of a patient within the magnetic resonance (MR) imaging system, wherein the vital signs detector is integrated in the RF transmit-receive coil, wherein a pair of electrically conducting coil elements of the RF transmit-receive coil forms the vital signs detector, wherein the vital signs detector is a capacitive vital signs detector, the capacitive vital signs detector being adapted for receiving capacitive vital signs signals. The proposed system consists of a combination of a RF transmit-receive coil with a capacitive vital signs detector for real time vital signs monitoring and simultaneous high-resolution imaging. The capacitive vital signs detector is formed by the conductors of the RF transmit-receive coil. The method is therefore entirely passive as it utilizes the measurement of the local electric field as modified by the movement of the body

(particularly the respiration and cardiac activity). Furthermore, combining RF coil and capacitive vital signs sensor techniques provides improved signal quality using cross correlations between systems, improved calibration schemes, or (spatial) guidance of one system using the other. In an embodiment of the invention the magnetic resonance (MR) imaging system can also be a MR-Therapy system like a MR-LINAC.

In an embodiment of the invention the capacitive vital signs detector is an electrocardiography (ECG) sensor being adapted for receiving ECG signals.

According to an embodiment of the invention the pair of electrically conducting coil elements of the RF transmit-receive coil forming the vital signs detector are covered with a material having a high permittivity. To increase the capacitance of the detector to the human body, the electrodes may be covered with a material having a high permittivity, such as ceramic. Electrodes are integrated in the coil cover (close to the body surface), thus no galvanic contact and galvanically isolated to human body. The capacitance ECG depends on several factors, but usually corresponds to relatively small values between 0.1–10 pF. For low frequency measurements as the ECG, such weak coupling requires high input impedance of the sensor as finite input resistance would attenuate the input voltage V_{in} . Very high impedance nodes are very susceptible to any electromagnetic interference from the environment and motion induced artefacts. Therefore, in an advantageous embodiment of the invention the electrodes can be actively shielded in order to suppress the interference.

In another preferred embodiment of the invention the capacitive vital signs detector and the RF transmit-receive coil being adapted for processing the capacitive vital signs signal and an MRI signal acquired by the RF transmit-receive coil in different frequency spaces.

In an embodiment of the invention the vital signs detector is arranged beneath a patient support of a magnetic resonance (MR) imaging system. The arrangement of the detector below a patient support is advantageous, as ECG can be received here especially well. This position is also particularly advantageous for measuring movements and the position of the patient.

In another aspect of the invention, the object is achieved by a system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system, the system comprising: a radio frequency (RF) transmit-receive coil with a vital signs detector according to any of claims 1 to 4, the system further comprising an output pre-amplifier for amplifying the capacitive vital signs signals, wherein the pair of electrically conducting coil elements is coupled to the output pre-amplifier, the system further comprising a digital signal

processor, wherein the digital signal processor being adapted for further processing the amplified capacitive vital signs signals.

According to a preferred embodiment the digital signal processor is a software defined radio (SDR). SDR's typically comprise analog-to-digital and digital-to-analog
5 converters, RF components for transmitting and/or receiving of signals and, a FPGA for basic filtering, signal down- and up-conversion and bidirectional wireless or optical outputs. The software exists in the computer, where it is executed and sends instructions to the SDR. A received signal is amplified e.g. by a preamp, and returned to the radio where it can be further amplified or attenuated. The ADC converts the signal to a digital signal, where the FPGA and
10 digital signal processor (DSP) handle down converting and filtering the digital signal. The data stream is then returned to the computer and real time signal processing software.

According to another embodiment of the invention the system comprises a relaxation oscillator and/or a microcontroller for the capacitive vital signs signals detection.

In another preferred embodiment of the invention the system comprises a
15 multiplexer for switching between different pairs of electrically conducting coil elements of the RF transmit-receive coil forming the vital signs detector.

In a further aspect of the invention, the object is achieved by a method for operating the system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system as described above comprising the following steps:

- 20 - providing a radio frequency (RF) transmit-receive coil comprising a vital signs detector, wherein the radio frequency (RF) transmit-receive coil and the vital signs detector form a magnetic resonance (MR) imaging coil array,
- receiving at least one vital signs signal from the vital signs detector,
- receiving at least one MRI signal from the radio frequency (RF) transmit-
25 receive coil,
- performing a correction of the MRI signal based on the vital signs signal.

According to an embodiment of the invention the step of performing a correction of the MRI signal based on the vital signs signal comprises a correction based on a deep learning algorithm.

30 In a still further aspect of the present invention, the object is achieved by a magnetic resonance (MR) imaging system comprising a system for the detection of vital signs of a patient as described above.

In a further aspect of the invention, the object is achieved by a software package for a magnetic resonance (MR) imaging system, whereby the software package

contains instructions for controlling a system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system according to the method as described above.

In another aspect of the invention, the object is achieved by a software package for upgrading a magnetic resonance (MR) imaging system, whereby the software package contains instructions for controlling a radio frequency (RF) receiver system comprising a vital signs detector according to the method as described above.

In an embodiment of the invention an AI-based software algorithm for selecting the capacitive electrodes from sensor data and for configuring e.g. filter parameters based on training data obtained with the system can be foreseen. The data can be processed and filtered using e.g. Kalman or SVD filtering. Data processing can, for example, take place remotely in a cloud.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other aspects of the invention will be apparent from and elucidated with reference to the embodiments described hereinafter. Such an embodiment does not necessarily represent the full scope of the invention, however, and reference is made therefore to the claims and herein for interpreting the scope of the invention.

In the drawings:

Fig. 1 schematically depicts a system for the detection of vital signs comprising a radio frequency (RF) transmit-receive coil with a vital signs detector according to an embodiment of the invention,

Fig. 2 schematically depicts a system for the detection of vital signs comprising a radio frequency (RF) transmit-receive coil with a vital signs detector according to another embodiment of the invention,

Fig. 3 schematically depicts a part of a system for the detection of vital signs according to another embodiment of the invention,

Fig. 4 schematically depicts a flow chart of the signal stream of the vital signs detector and the RF transmit-receive coil according to an embodiment of the invention,

Fig. 5 shows a flowchart of a method for operating a system for the detection of vital signs in accordance with an embodiment of the invention,

Fig. 6 shows vital signs detector patches with a RF transmit-receive coil and impedance circuits in accordance with an embodiment of the invention,

Fig. 7 shows a RF coil array with individual hybrid RF transmit-receive coils and vital signs detector patches in accordance with an embodiment of the invention.

DETAILED DESCRIPTION OF EMBODIMENTS

Fig. 1 schematically depicts a system for the detection of vital signs comprising a radio frequency (RF) transmit-receive coil 1 with a vital signs detector 3 according to an embodiment of the invention. The conductor 4 of the radio frequency (RF) transmit-receive coil 1 forms a capacitive electrode with a coupling to the body which is in the order of 5-20 pF. The induced ECG signal can be measured as change in the capacitance. For example, a voltage signal is measured over the capacitance and amplified via the high impedance preamplifier 5. Additionally the capacitance can be modulated by the motion of the body. Having a RF coil array 18, each individual measured signal depends on the local motion and local ECG signal. The amplified signal is further digitally processed e.g. via a FPGA unit 8. The MRI signal of RF transmit-receive coil 1 is received by the resonant coil circuit and amplified by a RF preamplifier 2. Due to the high impedance of the ECG preamplifier 5 the RF signal is not disturbed. The RF transmit-receive coil signal is further digitized and can be used for correction and calibration of the ECG signal, e.g. to remove motion induced artefacts.

The capacitive vital signs signals and the MRI signals are processed in different frequency spaces. Therefore, in an embodiment of the invention two separate ADC channels 6, 7 may be provided. The output of the ADCs is fed to a signal processing device 8. The signal processing device 8 can be e.g. a software defined radio (SDR). The signal processing device 8 can be used e.g. for the correction of motion artefacts in the MRI signal by the vital signs signals. An interface 9 e.g. an optical interface, controls the communication of the signal processing device 8 with other components of the MRI system. As well other circuits schemes can be realized with only one common ADC. In another embodiment of the invention the capacitive sensor signal can be transformed (or modulate a) to a pilot tone and received via the MRI receiver or by separate receiver at a different frequency.

The detection of motion e.g. by breathing or heart beat is one application of the vital signs detector 3, additionally the capacitive vital signs signals can be simultaneously processed by other vital signs detectors such as cameras or RADAR sensors.

Fig. 2 schematically depicts a system for the detection of vital signs comprising a radio frequency (RF) transmit-receive coil 1 with a vital signs detector 3 according to another embodiment of the invention. In Fig. 2 the RF transmit-receive coil 1 is shown with four capacitive conductors 4 forming the capacitive vital signs detector 3. The conductors 4 increase the capacitance for the ECG signal, while the MRI coil resonance is determined by the loop conductor and the lumped capacitors. The MRI signals are received by electrically conducting coil elements of the RF transmit-receive coil 1 and fed to a match and detune circuit 11, amplified by a RF amplifier 2 and further fed to an analog-to-digital converter (ADC) 7. The capacitive vital signs signals are received by the capacitive conductors and fed via two diodes 11 to a relaxation oscillator 12 or a microcontroller for the detection of the capacitive vital signs signals.

Fig. 3 schematically depicts a part of a system for the detection of vital signs according to another embodiment of the invention. In an embodiment of the invention several electrically conducting coil elements 4 of the RF transmit-receive coil 1 forming vital signs detectors 3 can be foreseen. In order to be able to switch between different vital signs detectors 3, a multiplexer 14 is provided which is controlled, for example, by means of a microcontroller 13 by a control signal 15. Also, in this embodiment a relaxation oscillator 12 can be provided for the detection of the vital signs signals.

Fig. 4 schematically depicts a flow chart of the signal stream of the vital signs detector 3 and the RF transmit-receive coil 1 according to an embodiment of the invention. The vital signs signal from the vital signs detector 3 is analyzed in step 400. The MRI signal from the RF transmit-receive coil 1 is analyzed in step 410. In step 420 the best signal is identified either from the vital signs detector 3 or the RF transmit-receive coil 1. Afterwards a signal processing device 8 e.g. a software defined radio (SDR) is used for generating a correlation of the signal in step 430. An improved trigger signal can then be generated from the vital sign signal 450 for improved control of the MRI signal in step 470, e.g. using the correlation of both signals. The MRI signal 440 can also be improved using the vital signs signal. For example, the overall signal quality can be improved by setting a range of interest, which also improves the MRI reconstruction in step 460.

Fig. 5 shows a flowchart of a method for operating a system for the detection of vital signs in accordance with an embodiment of the invention.

The method starts with step 500 in which a radio frequency (RF) transmit-receive coil 1 comprising a vital signs detector 3 is provided, wherein the radio frequency

(RF) transmit-receive coil 1 and the vital signs detector 3 form a magnetic resonance (MR) imaging coil array.

In Step 510 at least one vital signs signal is received from the vital signs detector 3.

5 In step 520 at least one MRI signal is received from the radio frequency (RF) transmit-receive coil 1.

In step 530 a correction of the MRI signal based on the vital signs signal is performed.

Fig. 6 shows vital signs detector patches 16 with a RF transmit-receive coil 1
10 and impedance circuits 17 in accordance with an embodiment of the invention. To increase the capacitance, the additional electrically conducting coil elements 4 forming the vital signs detectors 3 can be formed as patches 16 and combined with the RF transmit-receive coil 1. The patches can be e.g. ECG patches with electrocardiography (ECG) sensors the sensors being adapted for receiving ECG signals. Several patches 16 can be located inside the coil
15 circumference or partly under the coil. The patches 16 are separated from each other in order to prevent B1 shielding effects from the excitation field of the MR body transmit coil. The individual patches 16 are connected via impedance circuits 17. The impedance circuits 17 can be RF chokes or parallel resonant circuits with a high impedance at the MRI frequency and a low impedance at frequencies for ECG and breathing. In Fig. 6 the signals are amplified and
20 processed separately by different optimized amplifiers 2, 5 e.g. low noise amplifiers (LNA).

Fig. 7 shows a RF coil array 18 with individual hybrid RF transmit-receive coils 1 and vital signs detector patches 16 in accordance with an embodiment of the invention. Each coil 1 does see an individual part of the human body. The individual signals of the vital signs detector patches 16 can be selected e.g. using a multiplexer.

25 While the invention has been illustrated and described in detail in the drawings and foregoing description, such illustration and description are to be considered illustrative or exemplary and not restrictive; the invention is not limited to the disclosed embodiments. Other variations to the disclosed embodiments can be understood and effected by those skilled in the art in practicing the claimed invention, from a study of the drawings, the disclosure, and the appended claims. In the claims, the word "comprising" does not exclude
30 other elements or steps, and the indefinite article "a" or "an" does not exclude a plurality. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage. Any reference

signs in the claims should not be construed as limiting the scope. Further, for the sake of clearness, not all elements in the drawings may have been supplied with reference signs.

REFERENCE SYMBOL LIST

	radio frequency (RF) transmit-receive coil	1
	RF amplifier	2
5	capacitive vital signs detector	3
	electrically conducting coil element	4
	capacitive vital signs sensor amplifier	5
	ADC for vital signs signal	6
	ADC for MRI signal	7
10	signal processing unit	8
	interface	9
	match and detune circuit	10
	diode	11
	relaxation oscillator	12
15	microcontroller	13
	multiplexer	14
	control signal	15
	vital signs detector patch	16
	impedance circuit	17
20	RF coil array	18

CLAIMS:

1. A radio frequency (RF) transmit-receive coil for a magnetic resonance (MR) imaging system, the RF transmit-receive coil comprising a vital signs detector (3) for the detection of vital signs of a patient within the magnetic resonance (MR) imaging system, wherein the vital signs detector (3) is integrated in the RF transmit-receive coil (1), wherein a
5 pair of electrically conducting coil elements (4) of the RF transmit-receive coil (1) forms the vital signs detector (3), wherein the vital signs detector (3) is a capacitive vital signs detector (3), the capacitive vital signs detector (3) being adapted for receiving capacitive vital signs signals.
- 10 2. A radio frequency (RF) transmit-receive coil for a magnetic resonance (MR) imaging system as claimed in claim 1, wherein the vital signs detector is configured to measure respiration and/or cardiac activity
3. A radio frequency (RF) transmit-receive coil according to claim 1 or 2,
15 wherein the capacitive vital signs detector (3) is an electrocardiography (ECG) sensor being adapted for receiving ECG signals.
4. A radio frequency (RF) transmit-receive coil according to any preceding claim, wherein the pair of electrically conducting coil elements (4) of the RF transmit-receive
20 coil (1) forming the vital signs detector (3) are covered with a material having a high permittivity.
5. A radio frequency (RF) transmit-receive coil according to any preceding claim, wherein the capacitive vital signs detector (3) and the RF transmit-receive coil (1)
25 being adapted for processing the capacitive vital signs signal and an MRI signal acquired by the RF transmit-receive coil (1) in different frequency spaces.

6. A radio frequency (RF) transmit-receive coil according to any preceding claim, wherein the vital signs detector (3) is arranged beneath a patient support of a magnetic resonance (MR) imaging system.

5 7. A system for the detection of vital signs of a patient within a magnetic resonance (MR) imaging system, the system comprising:

a radio frequency (RF) transmit-receive coil (1) with a vital signs detector (3) according to any of claims 1 to 4, the system further comprising an output pre-amplifier (5) for amplifying the capacitive vital signs signals, wherein the pair of electrically conducting
10 coil elements (4) is coupled to the output pre-amplifier (5), the system further comprising a digital signal processor (8), wherein the digital signal processor (8) being adapted for further processing the amplified capacitive vital signs signals.

8. A system according to claim 7, wherein the digital signal processor (8) is a
15 software defined radio (SDR).

9. A system according to claim 7 or 8, comprising a relaxation oscillator (12) and/or a microcontroller (13) for the capacitive vital signs signals detection.

20 10. A system according to any one of claims 7 to 9, comprising a multiplexer for switching between different pairs of electrically conducting coil elements (4) of the RF transmit-receive coil (1) forming the vital signs detector (3).

11. A method for operating the system for the detection of vital signs of a patient
25 within a magnetic resonance (MR) imaging system according to claim 6 comprising the following steps:

- providing a radio frequency (RF) transmit-receive coil (1) comprising a vital signs detector (3), wherein the radio frequency (RF) transmit-receive coil (1) and the vital signs detector (3) form a magnetic resonance (MR) imaging coil array,
- 30 - receiving at least one vital signs signal from the vital signs detector (3),
- receiving at least one MRI signal from the radio frequency (RF) transmit-receive coil (1),
- performing a correction of the MRI signal based on the vital signs signal.

12. A method for operating the system according to claim 11, characterized in that, the step of performing a correction of the MRI signal based on the vital signs signal comprises a correction based on a deep learning algorithm.

5 13. A magnetic resonance (MR) imaging system comprising a system for the detection of vital signs of a patient according to claims 1 to 10.

14. A software package for a magnetic resonance (MR) imaging system, whereby the software package contains instructions for controlling a system for the detection of vital
10 signs of a patient within a magnetic resonance (MR) imaging system according to the method claims 11 to 12.

15. A software package for upgrading a magnetic resonance (MR) imaging system, whereby the software package contains instructions for controlling a radio frequency
15 (RF) receiver system (1) comprising a vital signs detector (3) according to the method claims 10 to 11.

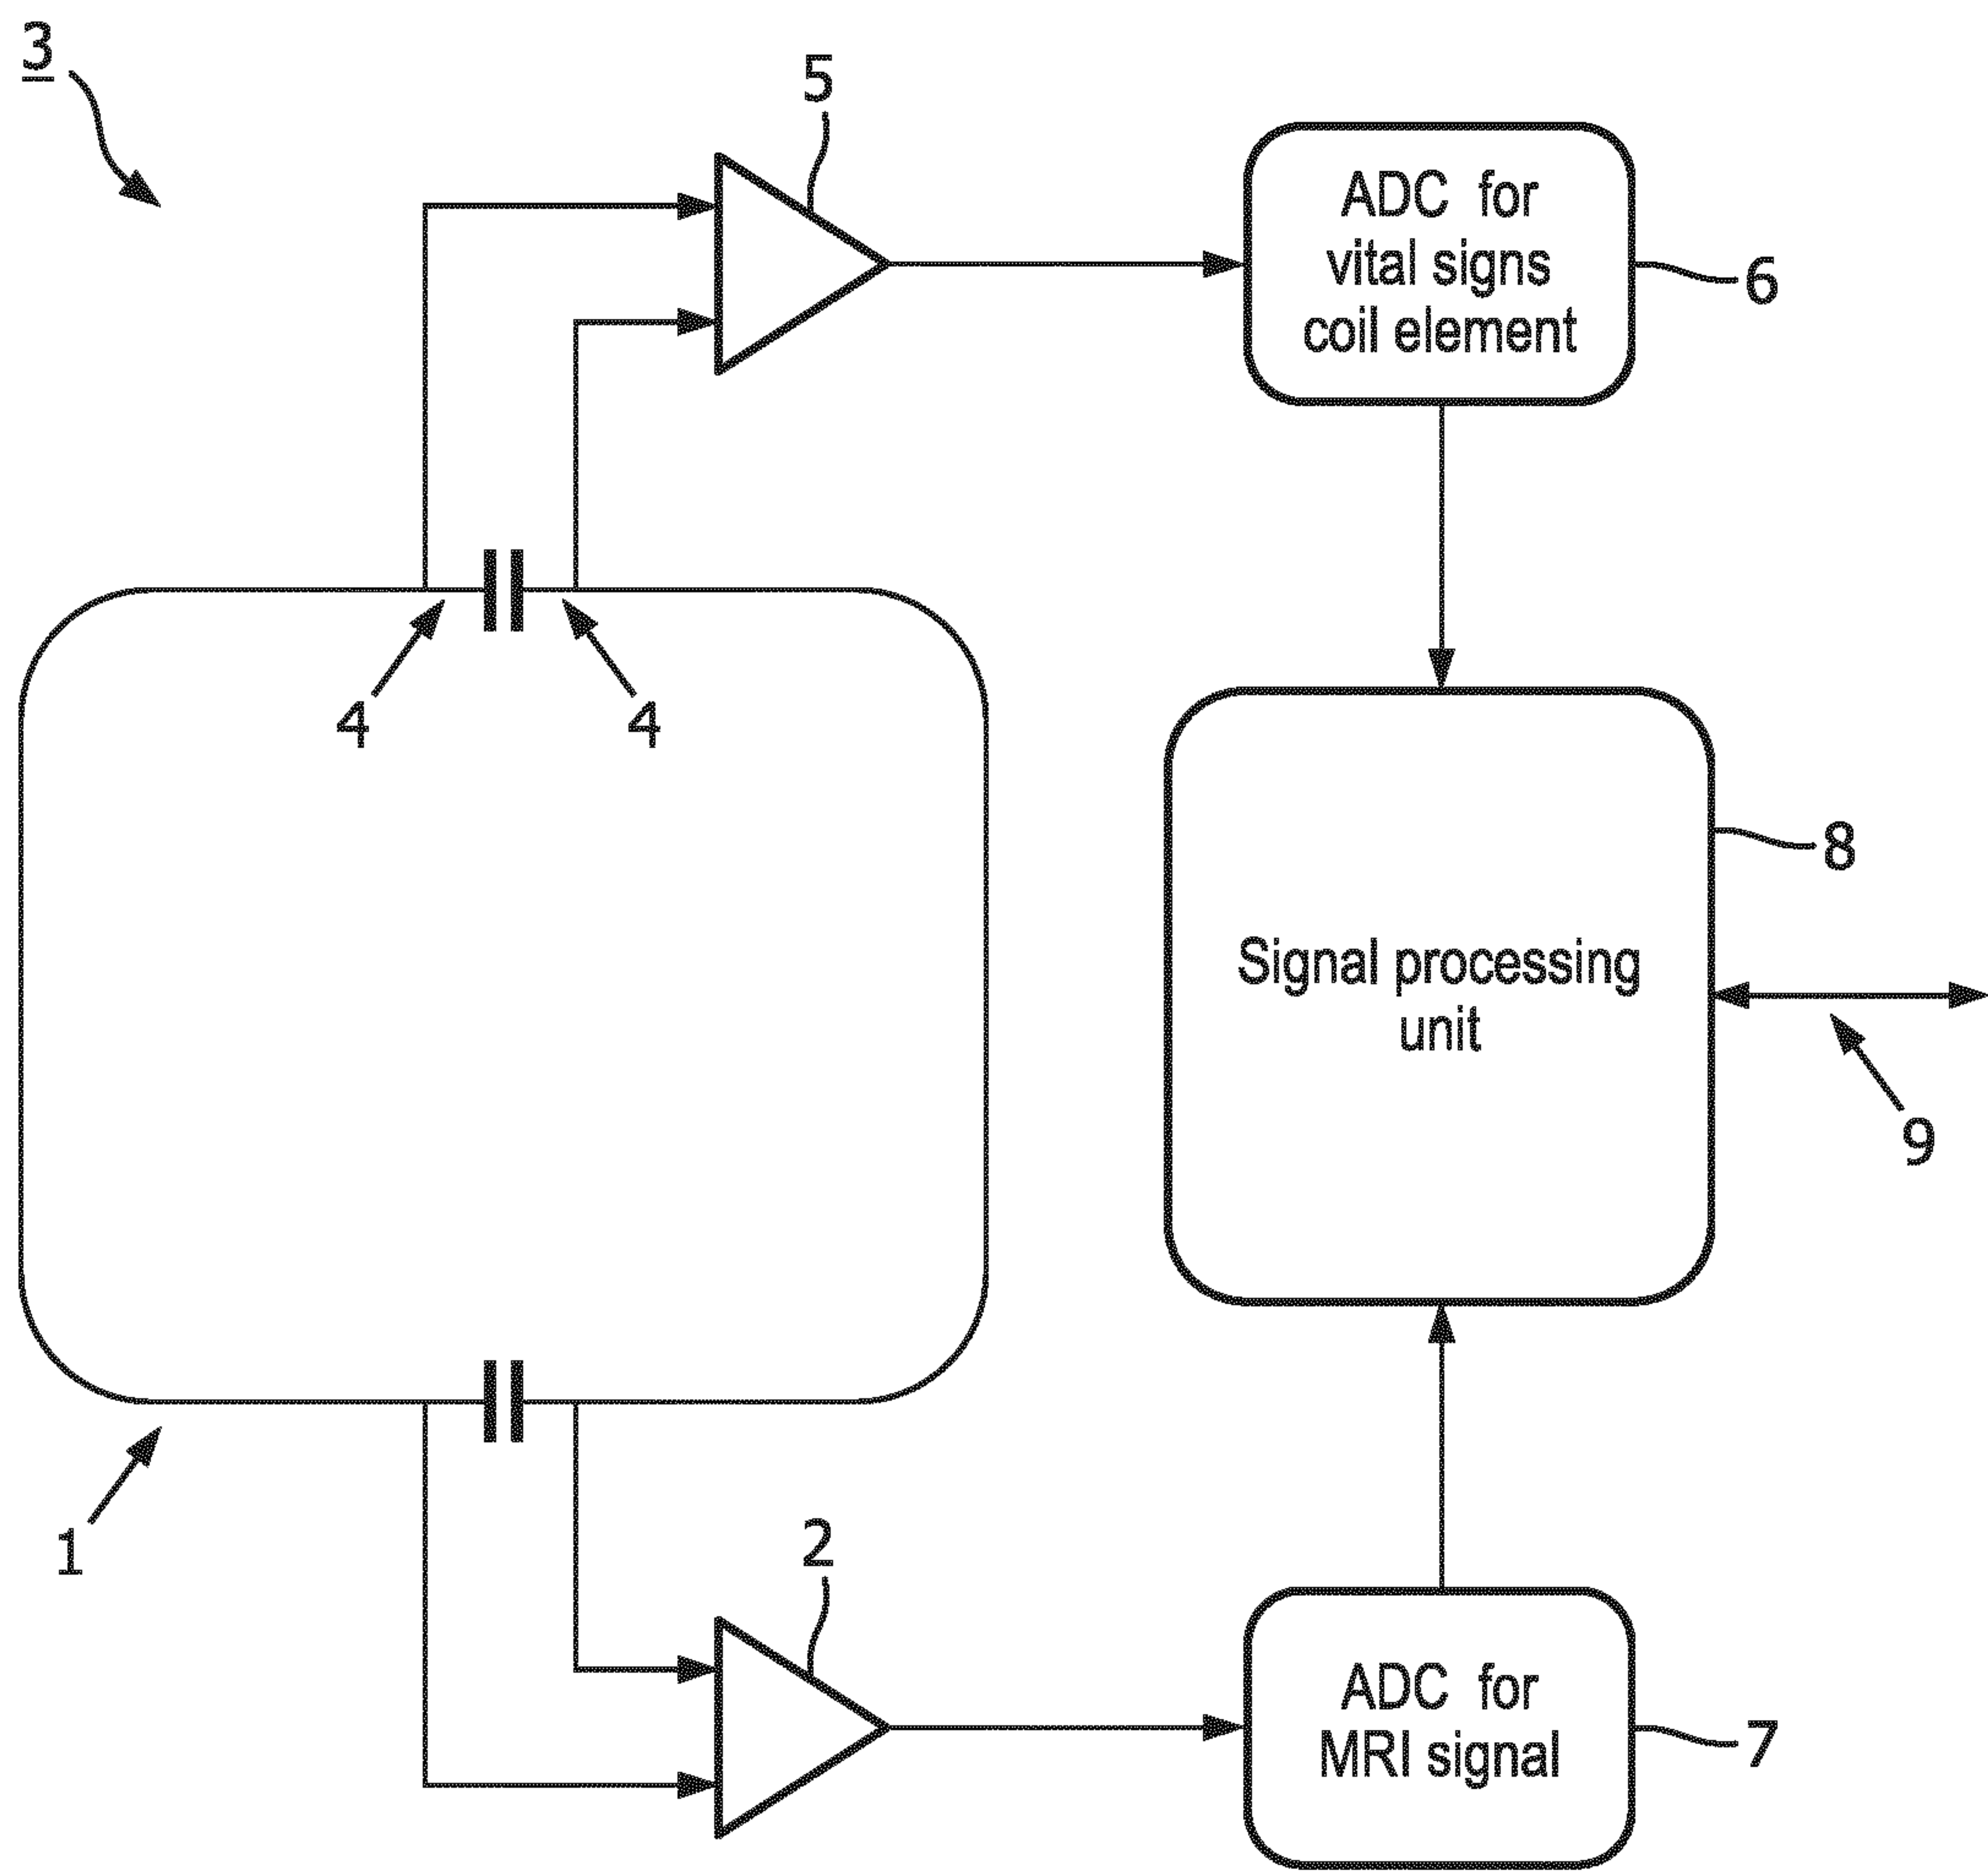


FIG. 1

2/6

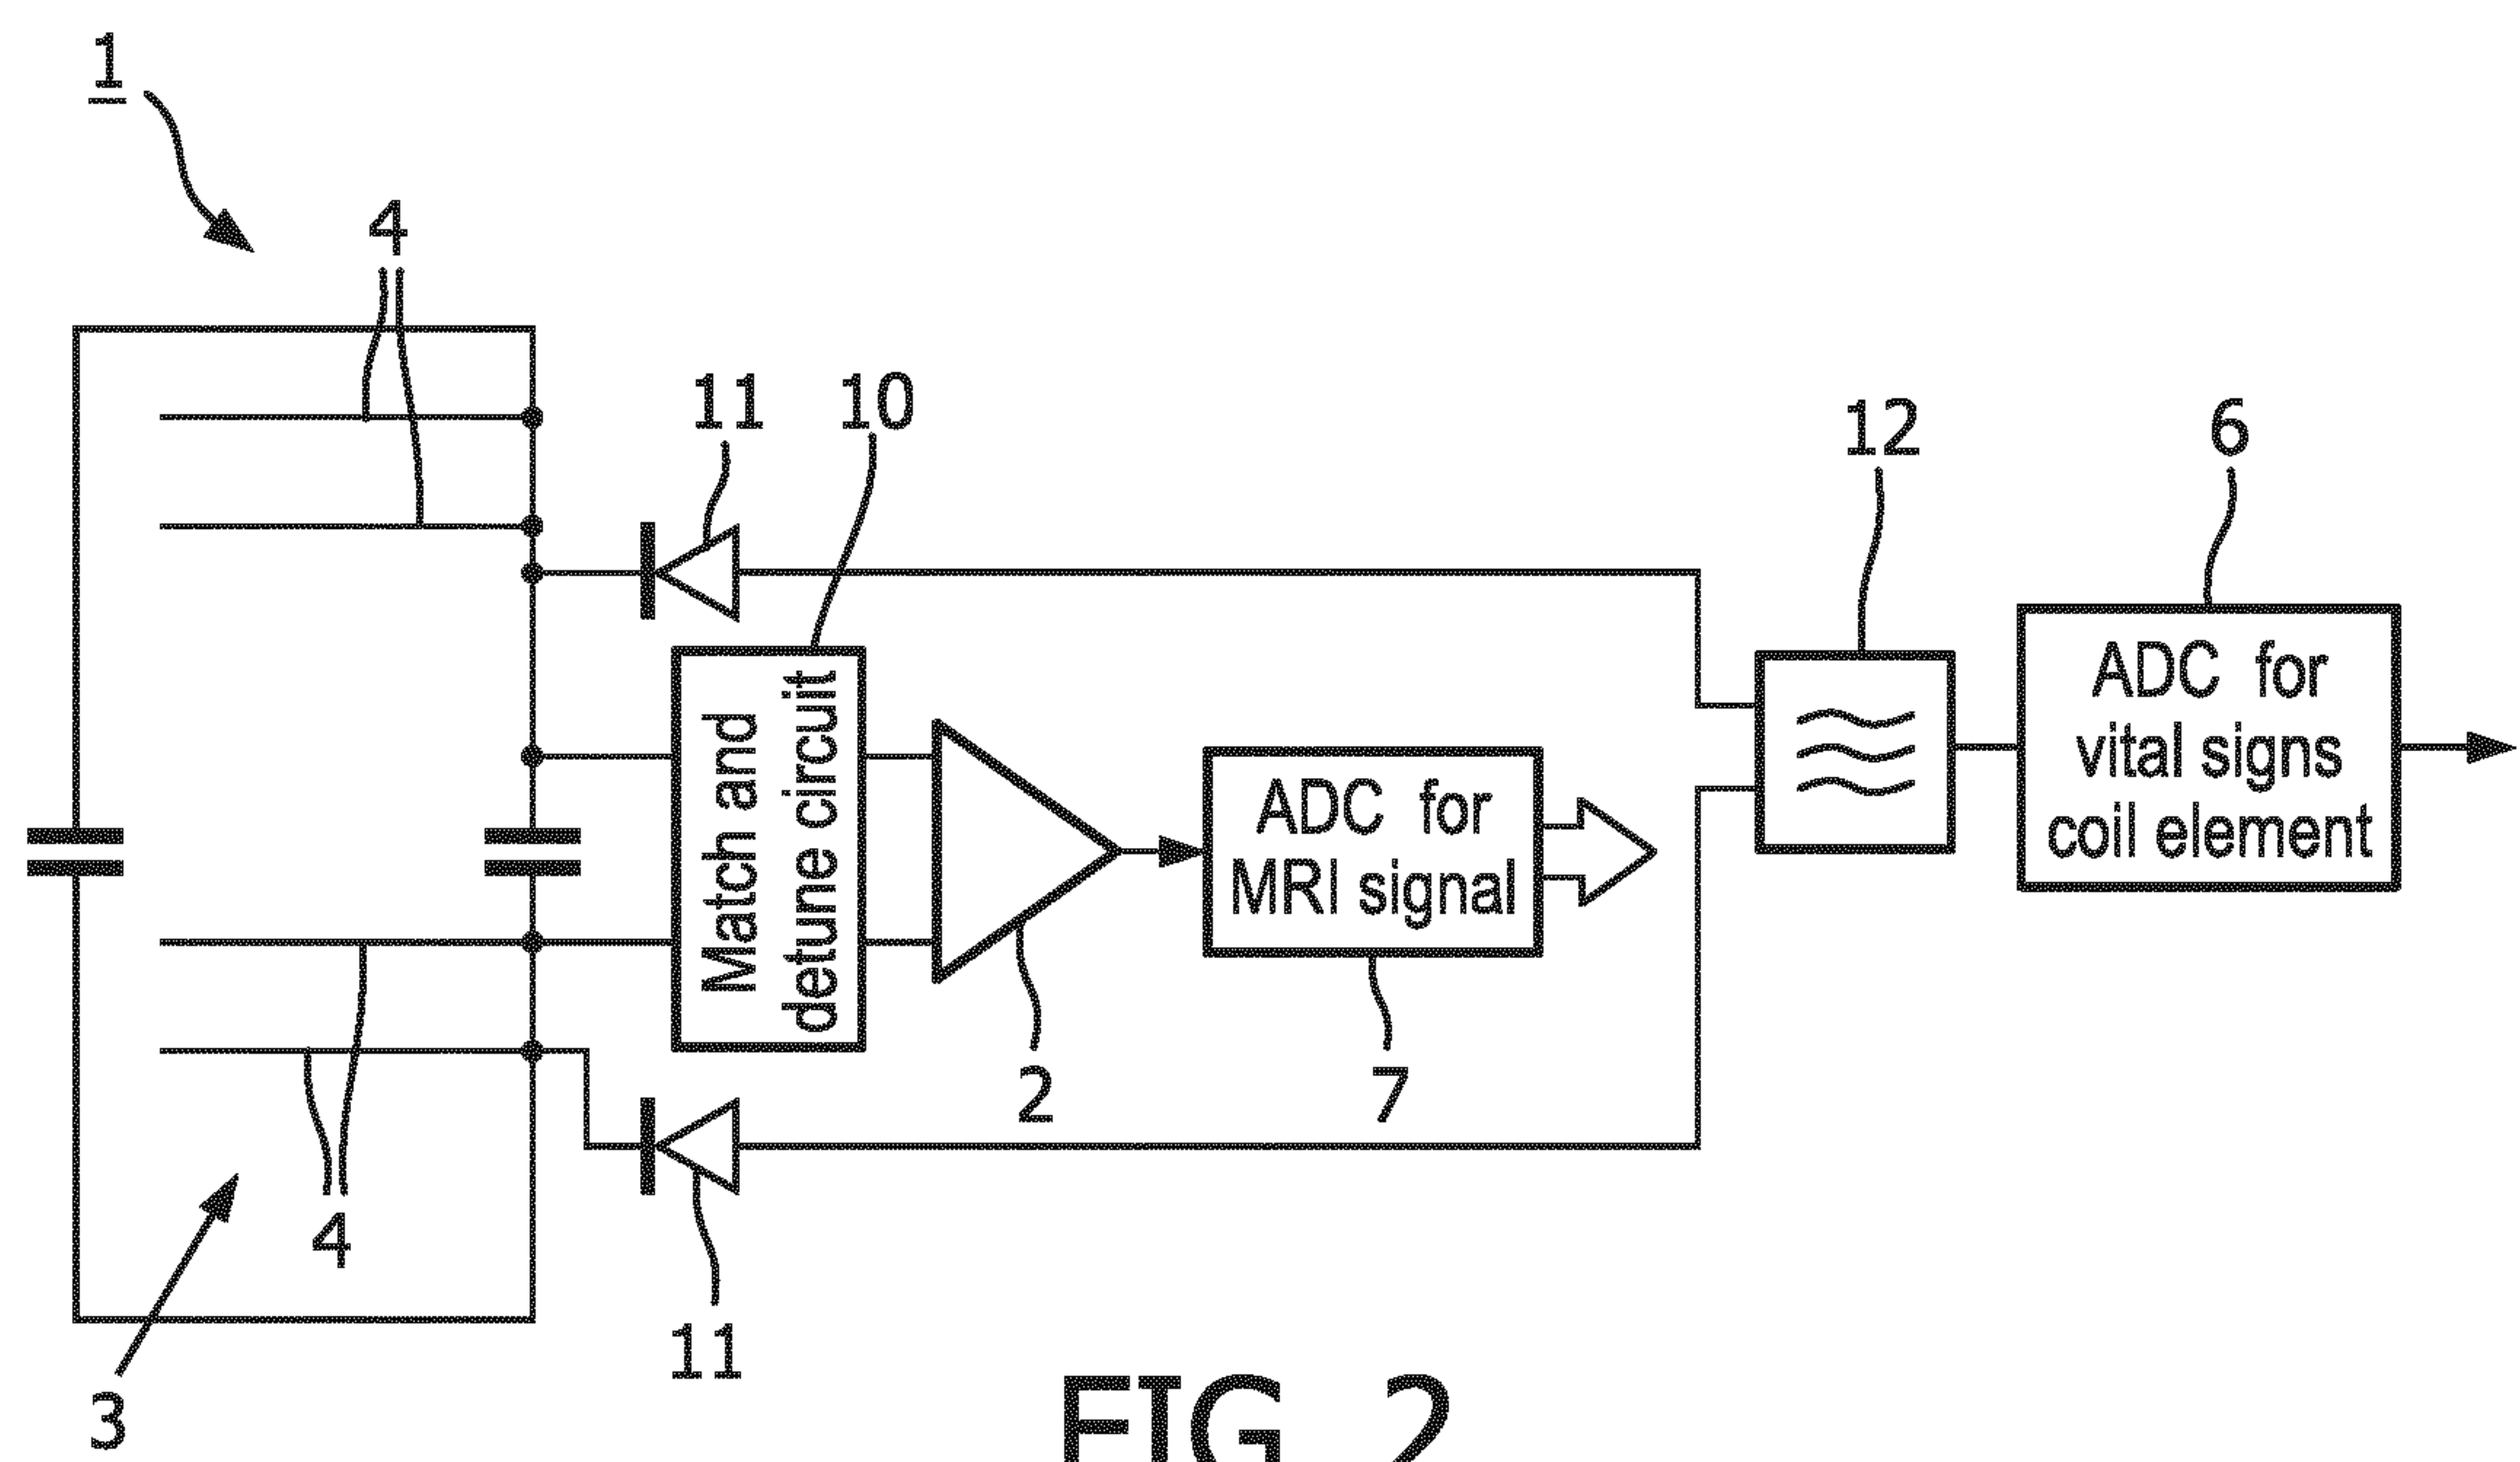


FIG. 2

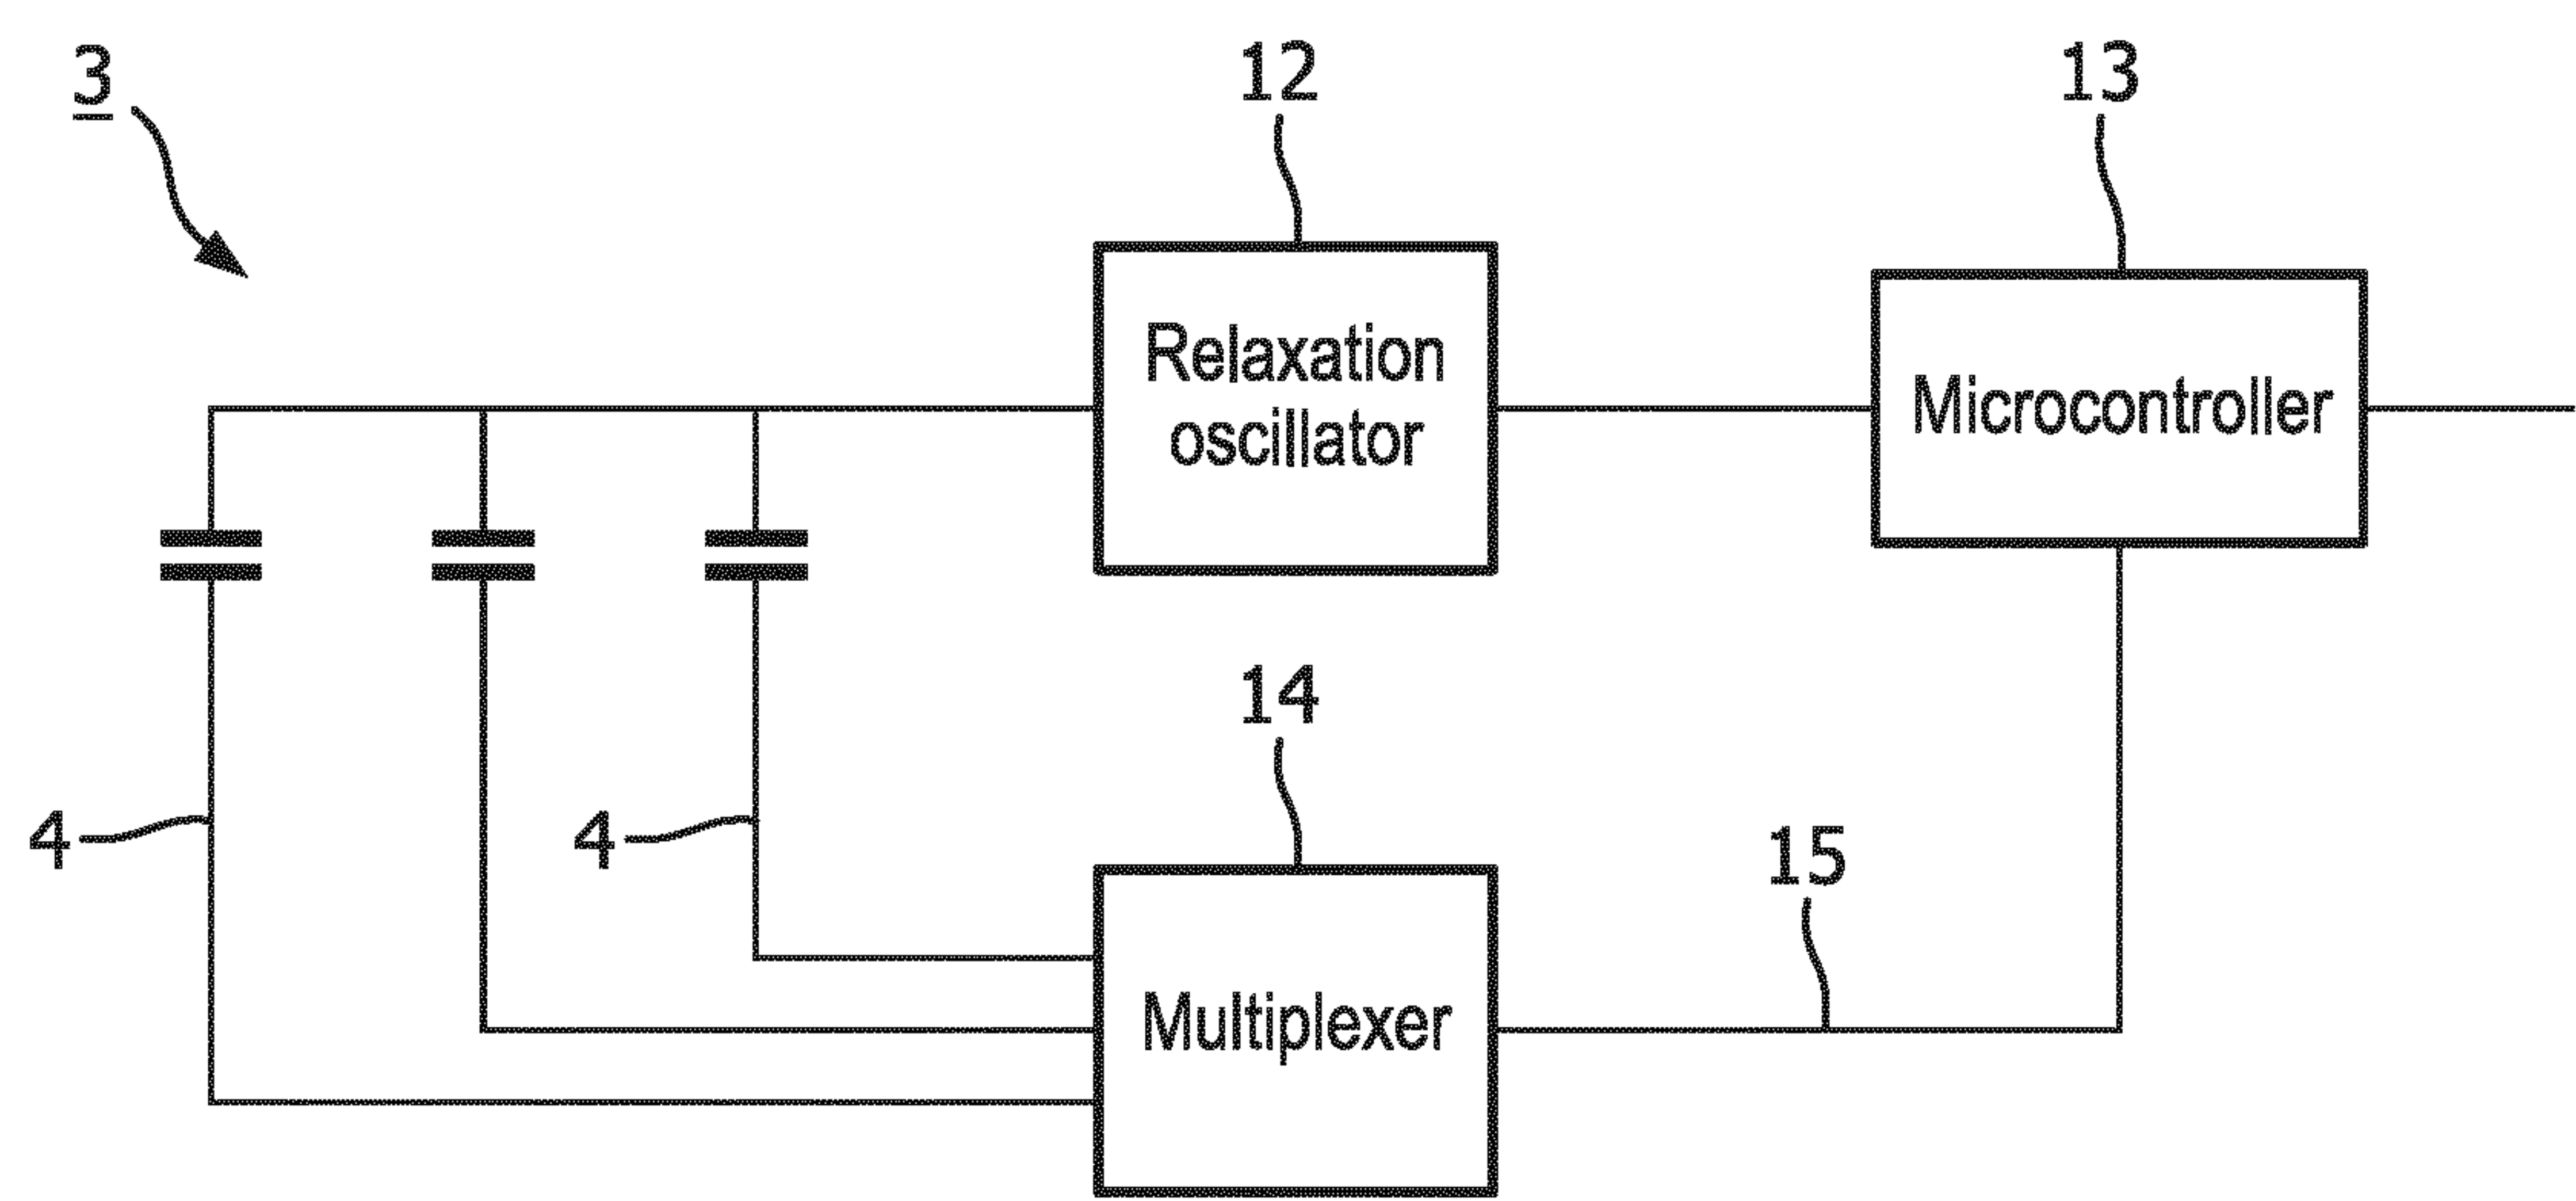


FIG. 3

3/6

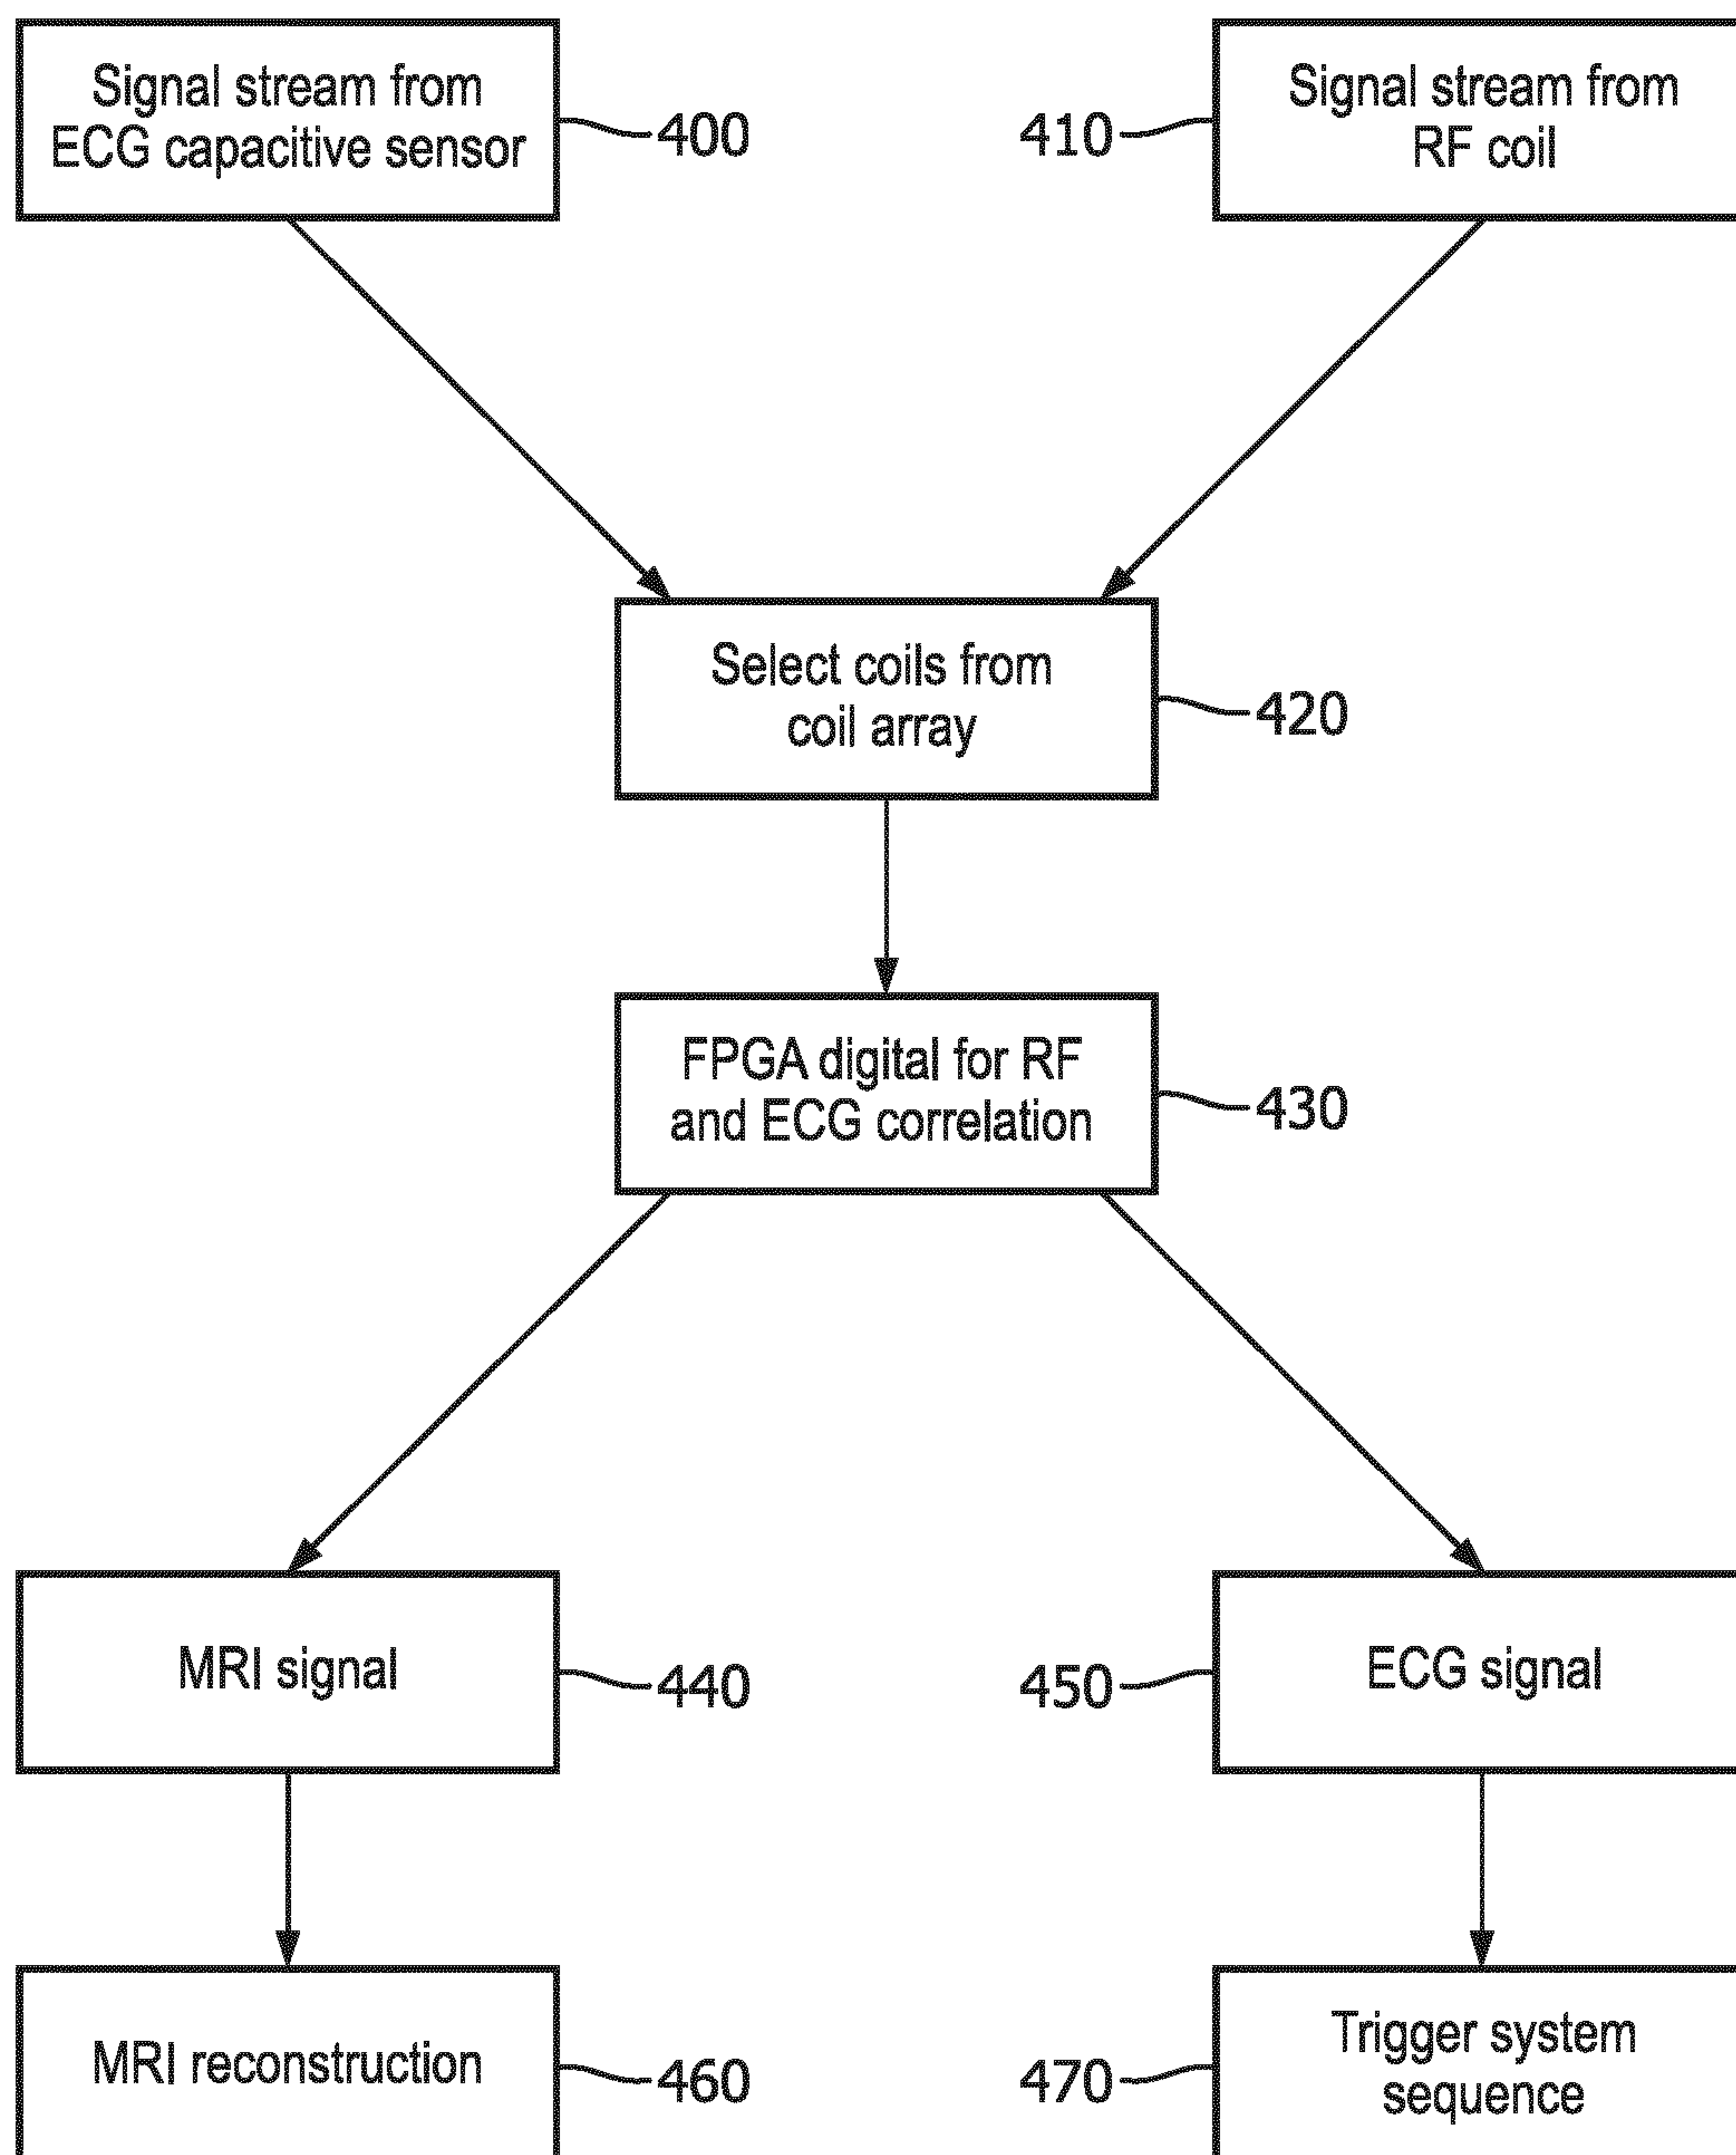


FIG. 4

4/6

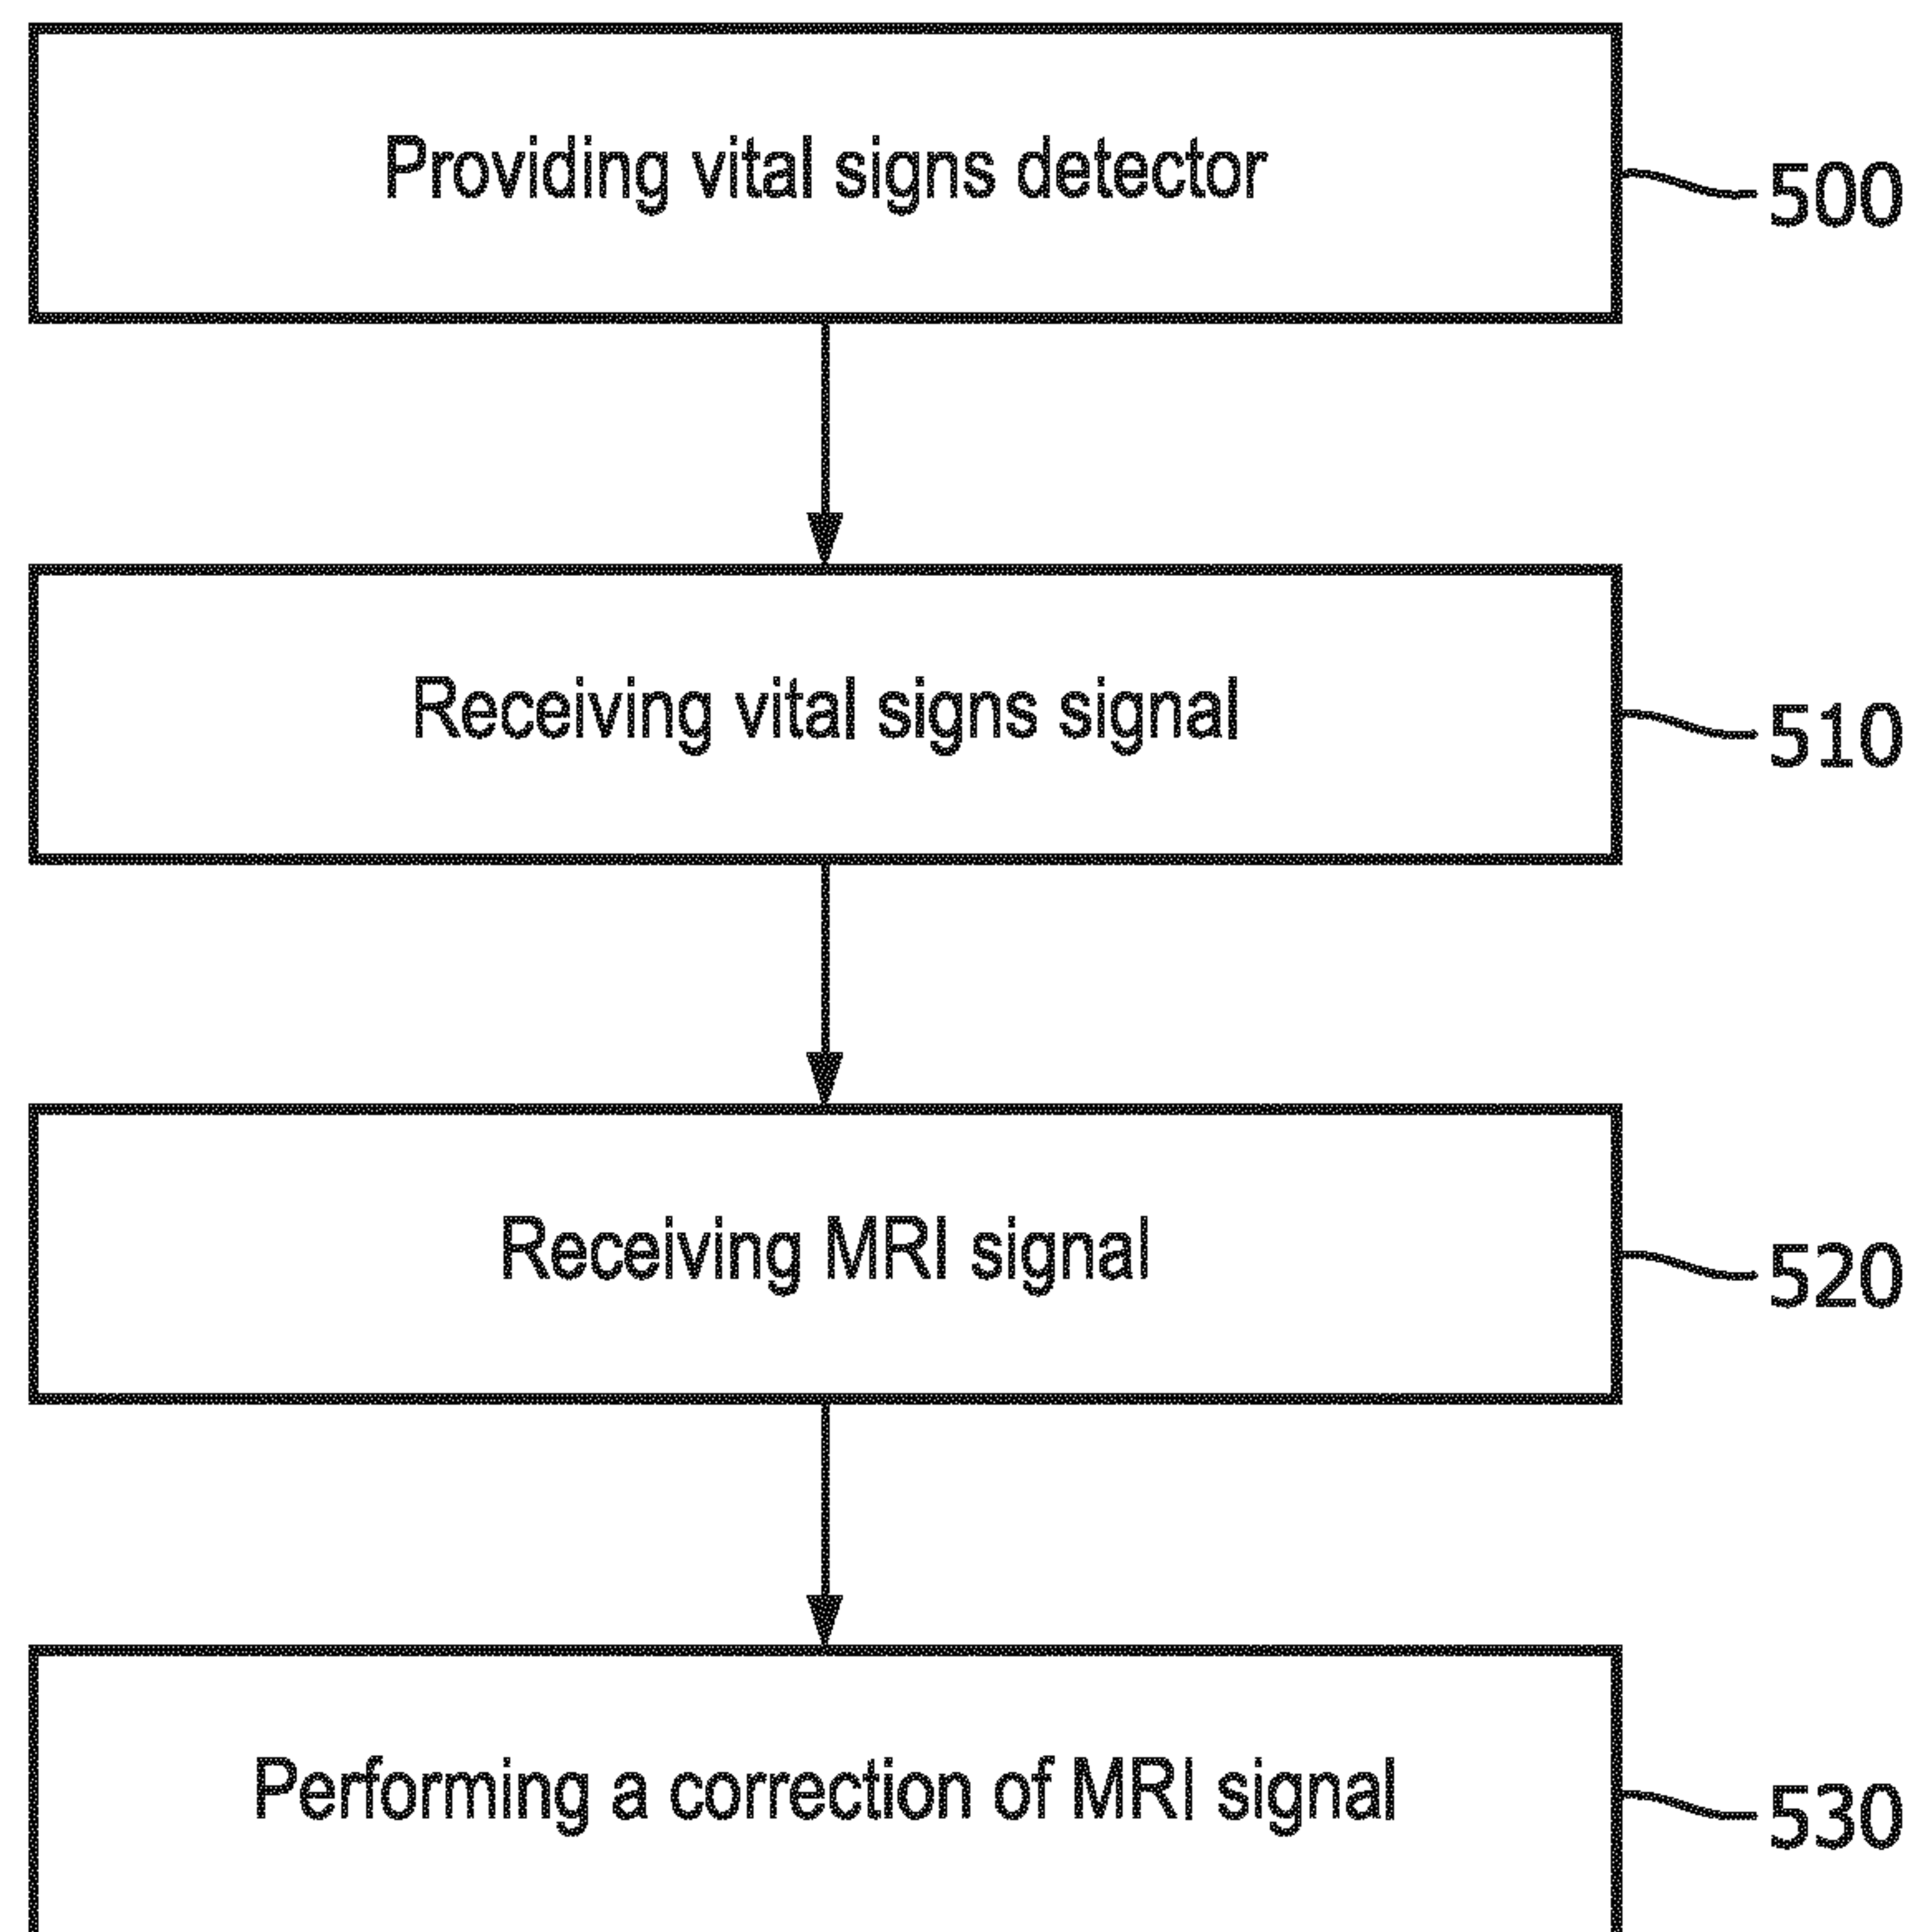


FIG. 5

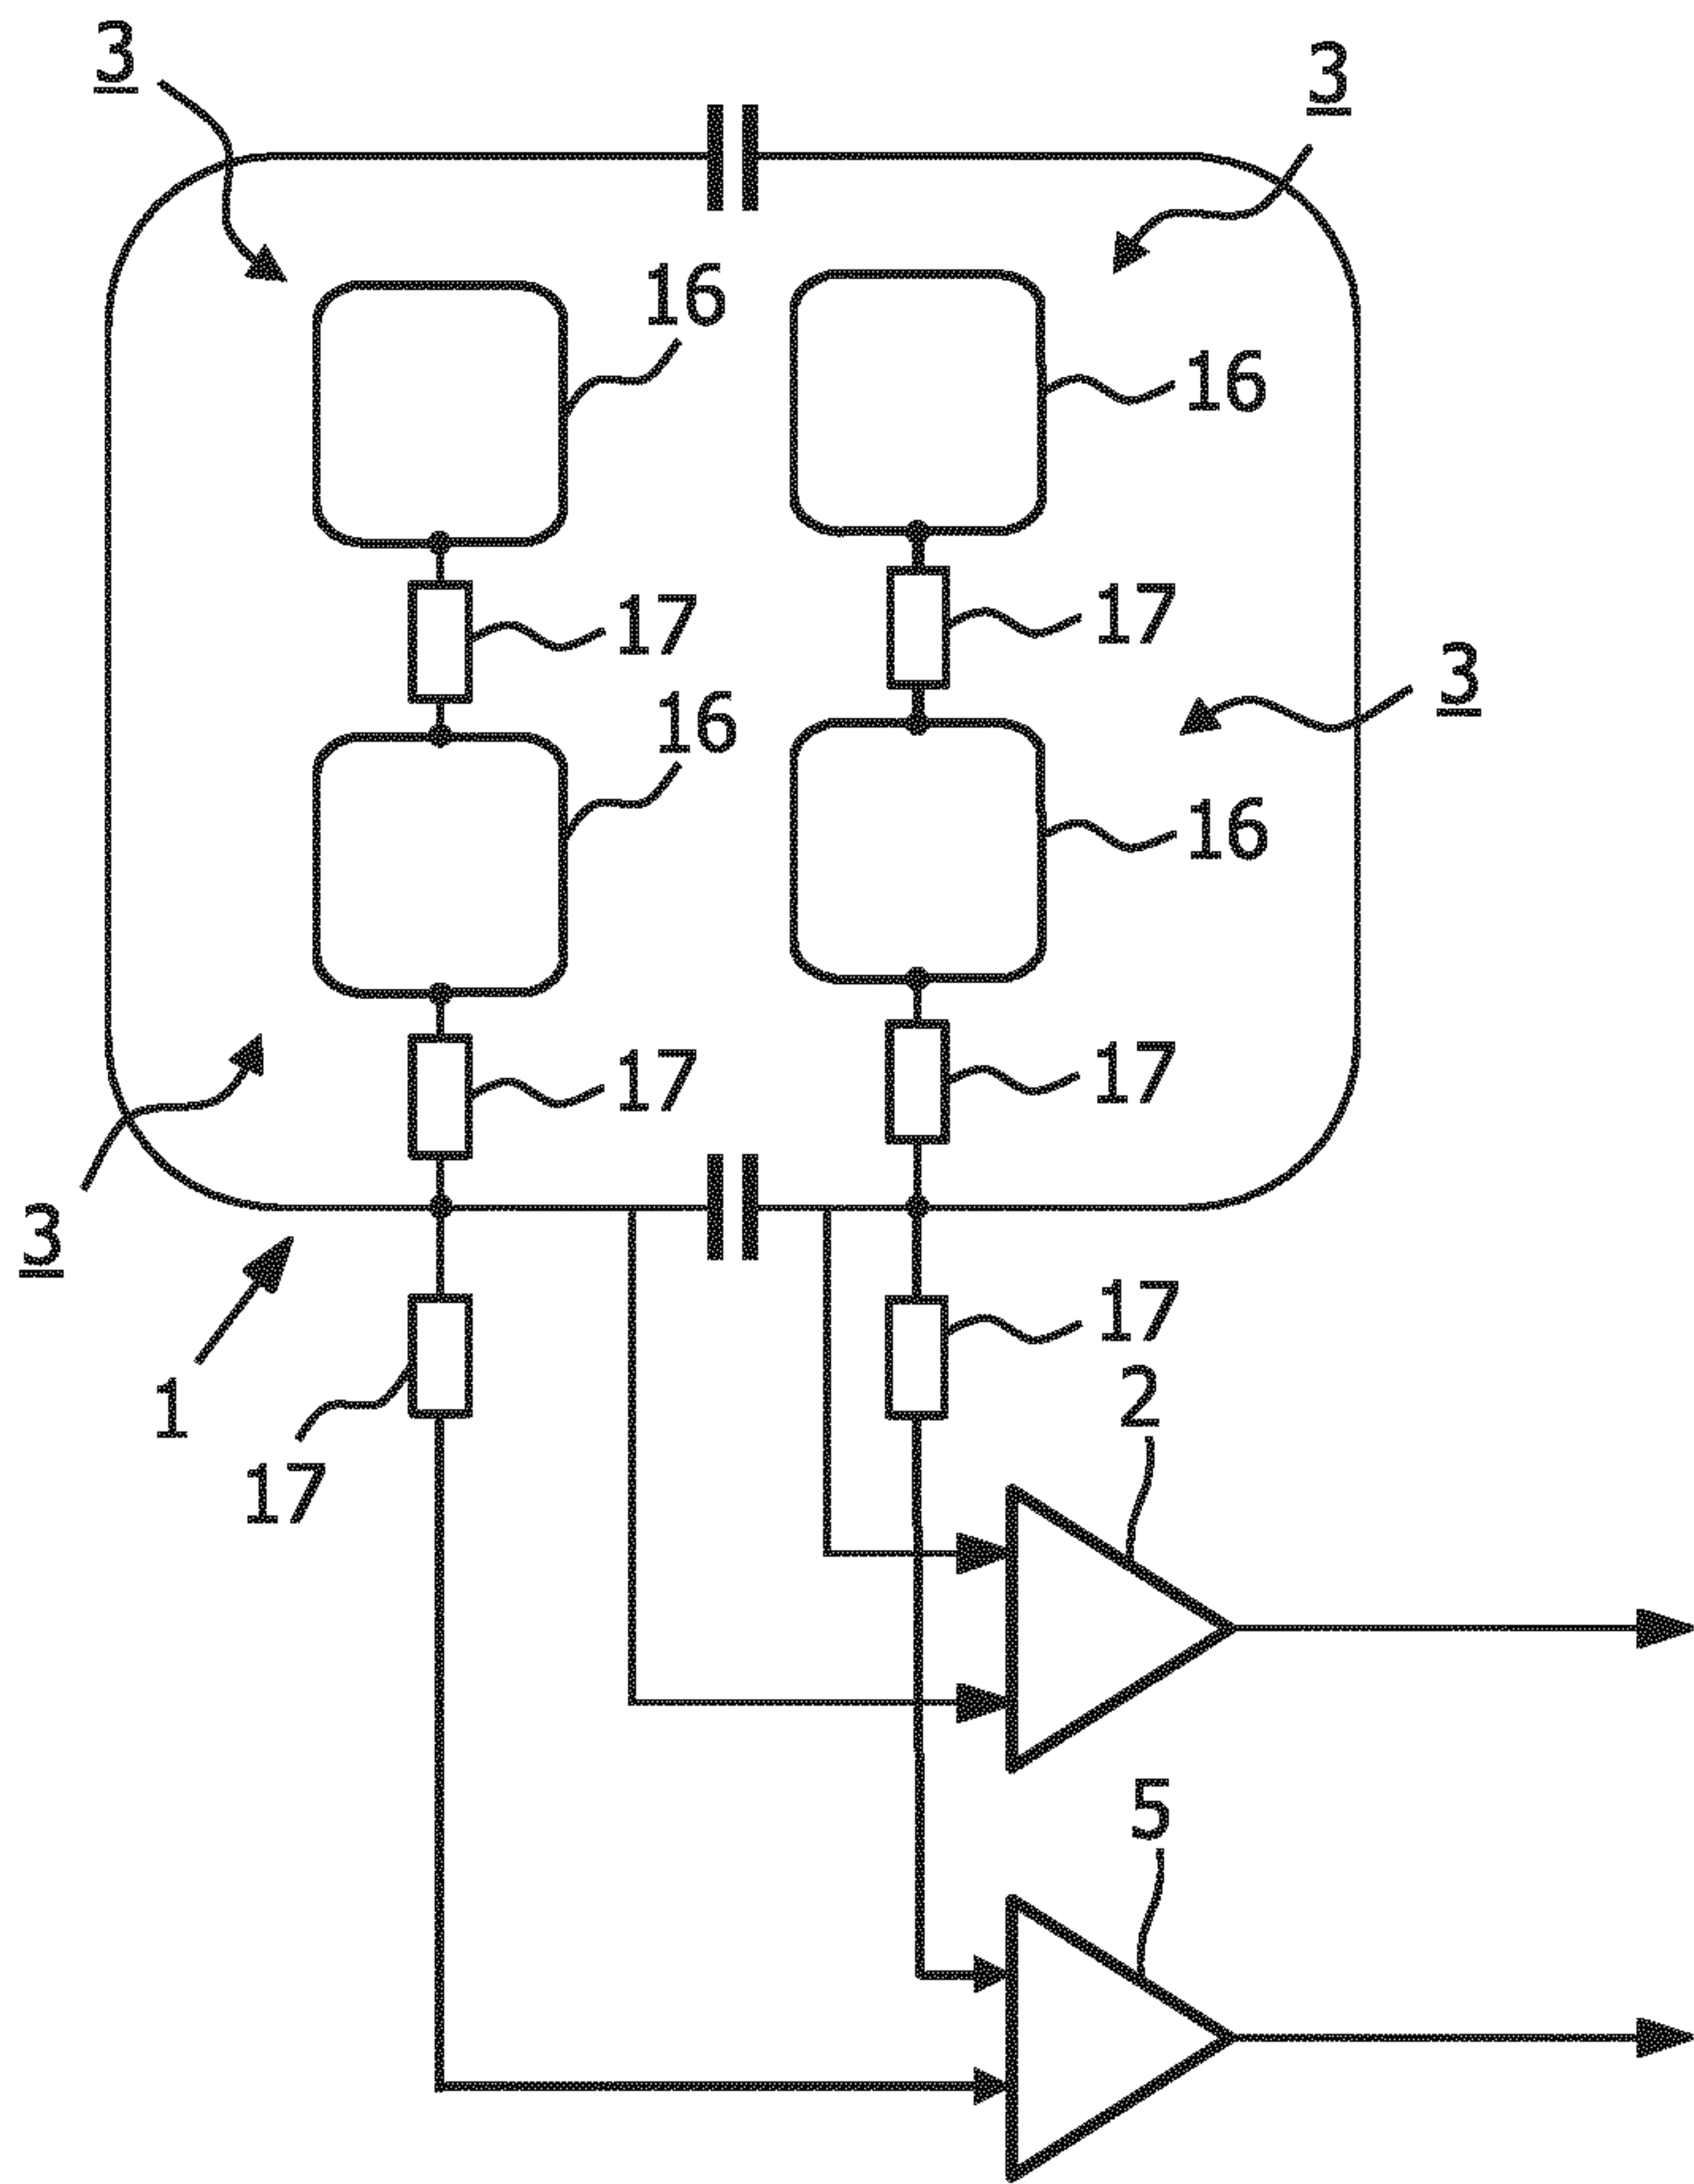


FIG. 6

6/6

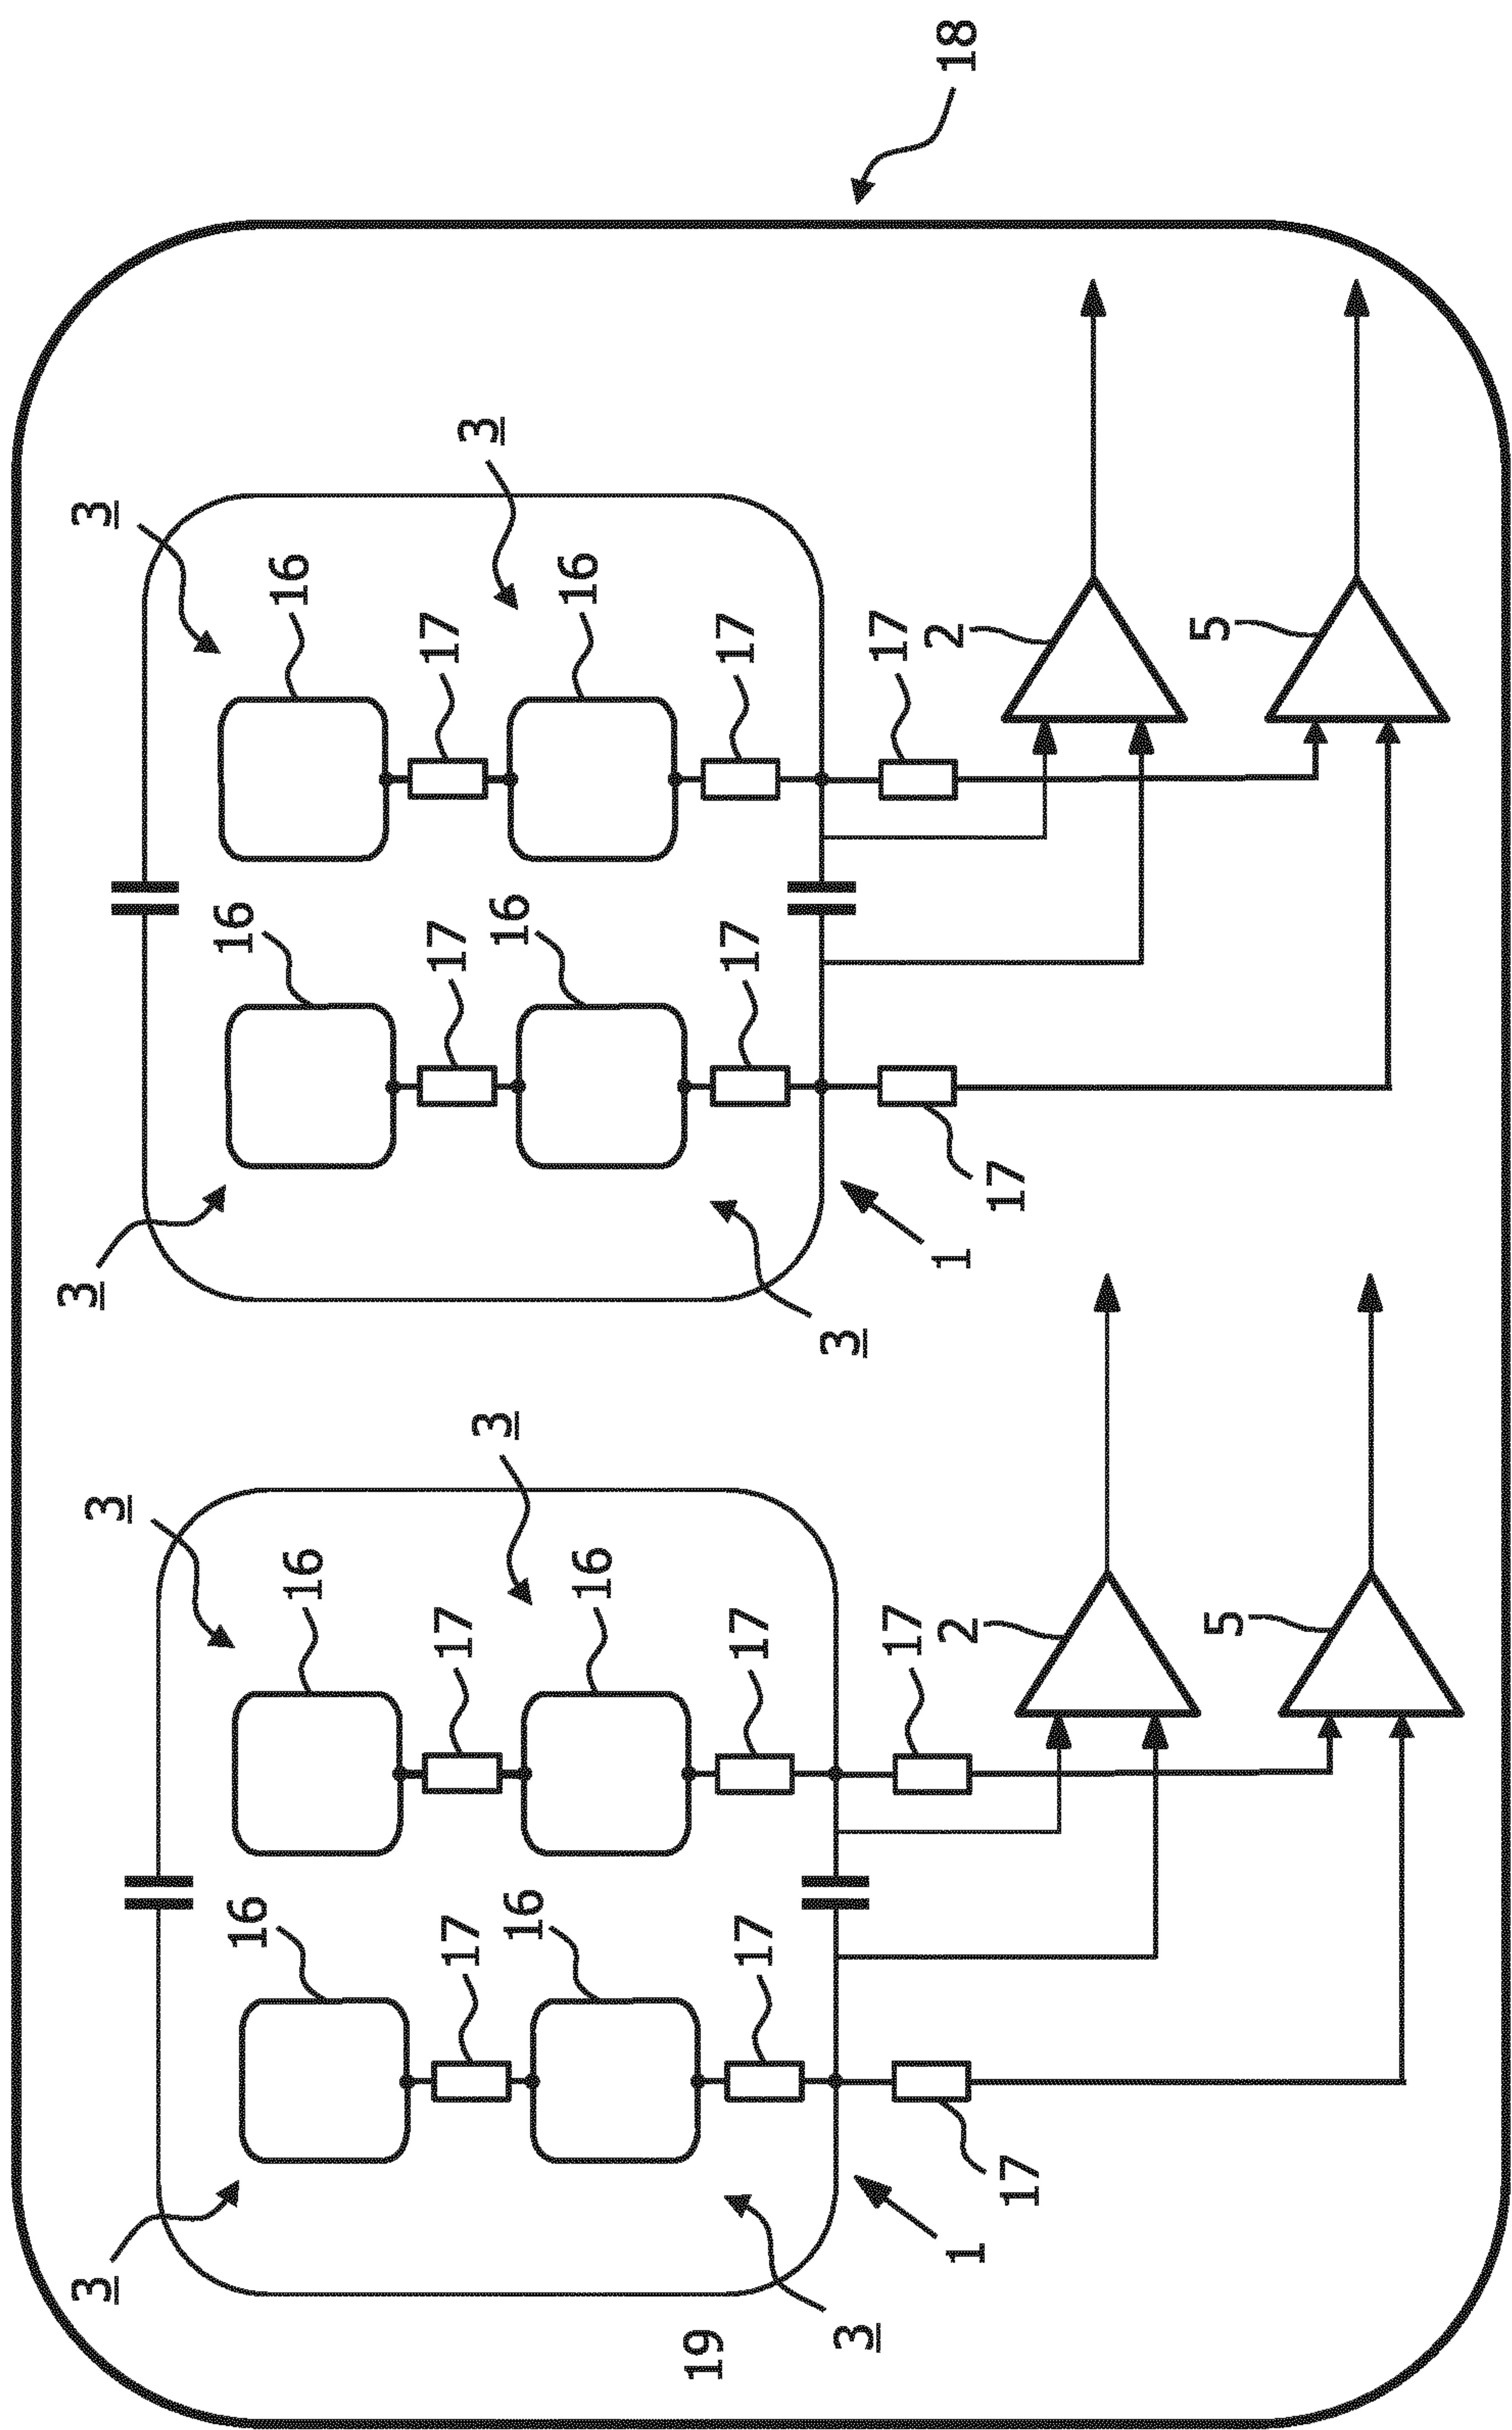


FIG. 7

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2020/087584

A. CLASSIFICATION OF SUBJECT MATTER INV. A61B5/055 A61B5/302 A61B5/00 G01R33/3415 G01R33/36 G01R33/565 G01R33/567 ADD. According to International Patent Classification (IPC) or to both national classification and IPC				
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) A61B G01R Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) EPO-Internal, WPI Data				
C. DOCUMENTS CONSIDERED TO BE RELEVANT				
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.		
X	WO 2014/141109 A1 (KONINKL PHILIPS NV [NL]; PHILIPS DEUTSCHLAND GMBH [DE]) 18 September 2014 (2014-09-18) page 12, line 5 - line 16 figure 1 -----	1,4-15		
X	US 2014/197836 A1 (HAMAMURA YOSHINORI [US] ET AL) 17 July 2014 (2014-07-17) paragraph [0056] figure 8 -----	1,4-15		
A	US 2015/087959 A1 (RÖSSLER JÜRGEN [DE]) 26 March 2015 (2015-03-26) the whole document -----	1-15		
☐ Further documents are listed in the continuation of Box C. ☒ See patent family annex.				
* Special categories of cited documents : <table border="0"> <tr> <td> "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed </td> <td> "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family </td> </tr> </table>			"A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family
"A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family			
Date of the actual completion of the international search 12 April 2021		Date of mailing of the international search report 20/04/2021		
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016		Authorized officer Van Dop, Erik		

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2020/087584

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
WO 2014141109	A1	18-09-2014	CN 105190342 A	23-12-2015
			EP 2972445 A1	20-01-2016
			JP 6351640 B2	04-07-2018
			JP 2016514993 A	26-05-2016
			RU 2015143468 A	19-04-2017
			US 2016033591 A1	04-02-2016
			WO 2014141109 A1	18-09-2014

US 2014197836	A1	17-07-2014	JP 6532647 B2	19-06-2019
			JP 2014133135 A	24-07-2014
			US 2014197836 A1	17-07-2014

US 2015087959	A1	26-03-2015	DE 102013219117 A1	26-03-2015
			US 2015087959 A1	26-03-2015
