

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
12 April 2001 (12.04.2001)

PCT

(10) International Publication Number
WO 01/24745 A1

- (51) International Patent Classification⁷: A61F 9/007, A61B 17/32
- (21) International Application Number: PCT/US00/24240
- (22) International Filing Date: 31 August 2000 (31.08.2000)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
09/411,747 1 October 1999 (01.10.1999) US
- (71) Applicant: ALCON LABORATORIES, INC. [US/US];
6201 South Freeway, Fort Worth, TX 76196 (US).
- (74) Agents: SCHIRA, Jeffrey, S. et al.; R & D Counsel,
Q-148, Alcon Laboratories, Inc., 6201 South Freeway, Fort
Worth, TX 76134-2099 (US).
- (81) Designated States (*national*): AU, BR, CA, JP, MX.
- (84) Designated States (*regional*): European patent (AT, BE,
CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC,
NL, PT, SE).
- Published:**
— With international search report.
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*
- (72) Inventor: COHEN, Donald, M.; 17512 Luther, Irvine,
CA 92614 (US).

(54) Title: LIQUEFRACTURE HANDPIECE

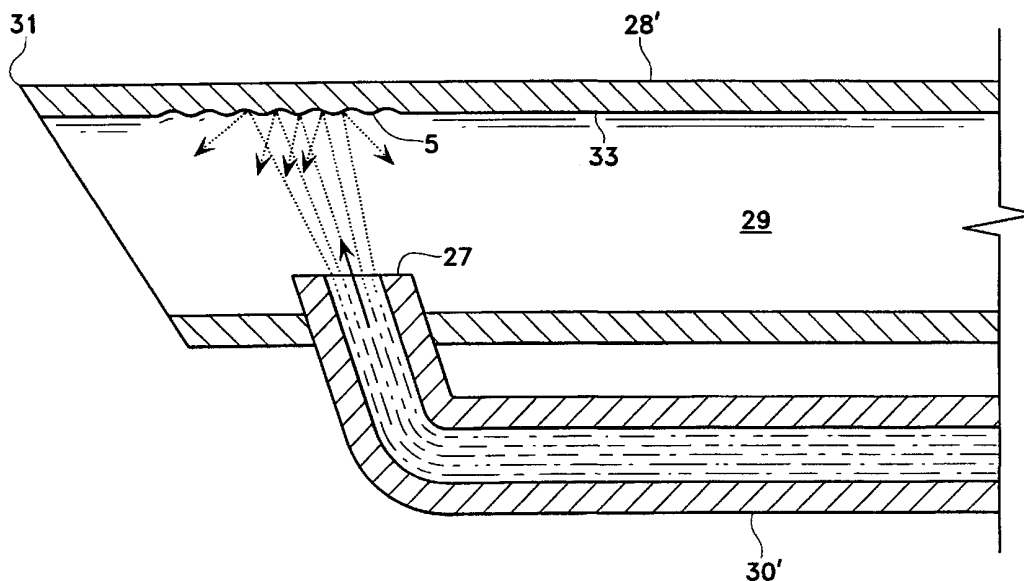

(57) Abstract: A tip for a liquefraction surgical handpiece. The tip uses at least two tubes. One tube is used for aspiration and another, smaller tube is used to inject heated surgical fluid for liquefying a cataractous lens. The distal portion of the injection tube terminates just inside of the aspiration tube so that heated fluid escaping the injection tube is reflected off of the internal wall of the aspiration tube prior to entering the eye. The internal wall is textured or roughened to further diffract the fluid stream. Such an arrangement prevents the injected fluid from directly entering the eye. The handpiece may also contain other tube, for example, for injecting relatively cool surgical fluid.



WO 01/24745 A1

LIQUEFRACTURE HANDPIECE

Background of the Invention

This invention relates generally to the field of cataract surgery and more particularly to a handpiece for practicing the liquefracture technique of cataract removal.

5 The human eye in its simplest terms functions to provide vision by transmitting light through a clear outer portion called the cornea, and focusing the image by way of the lens onto the retina. The quality of the focused image depends on many factors including the size and shape of the eye, and the transparency of the cornea and lens.

10 When age or disease causes the lens to become less transparent, vision deteriorates because of the diminished light which can be transmitted to the retina. This deficiency in the lens of the eye is medically known as a cataract. An accepted treatment for this condition is surgical removal of the lens and replacement of the lens function by an artificial intraocular lens (IOL).

15 In the United States, the majority of cataractous lenses are removed by a surgical technique called phacoemulsification. During this procedure, a thin phacoemulsification cutting tip is inserted into the diseased lens and vibrated ultrasonically. The vibrating cutting tip liquifies or emulsifies the lens so that the lens may be aspirated out of the eye. The diseased lens, once removed, is replaced by an artificial lens.

20 A typical ultrasonic surgical device suitable for ophthalmic procedures consists of an ultrasonically driven handpiece, an attached cutting tip, and irrigating sleeve and an electronic control console. The handpiece assembly is attached to the control console by an electric cable and flexible tubings. Through the electric cable, the console varies the power level transmitted by the handpiece to the attached cutting tip and the flexible tubings supply irrigation fluid to and draw aspiration fluid from the eye through the
25 handpiece assembly.

The operative part of the handpiece is a centrally located, hollow resonating bar or horn directly attached to a set of piezoelectric crystals. The crystals supply the required ultrasonic vibration needed to drive both the horn and the attached cutting tip during phacoemulsification and are controlled by the console. The crystal/horn assembly is
30 suspended within the hollow body or shell of the handpiece by flexible mountings. The handpiece body terminates in a reduced diameter portion or nosecone at the body's distal

end. The nosecone is externally threaded to accept the irrigation sleeve. Likewise, the horn bore is internally threaded at its distal end to receive the external threads of the cutting tip. The irrigation sleeve also has an internally threaded bore that is screwed onto the external threads of the nosecone. The cutting tip is adjusted so that the tip projects only a predetermined amount past the open end of the irrigating sleeve. Ultrasonic handpieces and cutting tips are more fully described in U.S. Pat. Nos. 3,589,363; 4,223,676; 4,246,902; 4,493,694; 4,515,583; 4,589,415; 4,609,368; 4,869,715; 4,922,902; 4,989,583; 5,154,694 and 5,359,996, the entire contents of which are incorporated herein by reference.

In use, the ends of the cutting tip and irrigating sleeve are inserted into a small incision of predetermined width in the cornea, sclera, or other location. The cutting tip is ultrasonically vibrated along its longitudinal axis within the irrigating sleeve by the crystal-driven ultrasonic horn, thereby emulsifying the selected tissue in situ. The hollow bore of the cutting tip communicates with the bore in the horn that in turn communicates with the aspiration line from the handpiece to the console. A reduced pressure or vacuum source in the console draws or aspirates the emulsified tissue from the eye through the open end of the cutting tip, the cutting tip and horn bores and the aspiration line and into a collection device. The aspiration of emulsified tissue is aided by a saline flushing solution or irrigant that is injected into the surgical site through the small annular gap between the inside surface of the irrigating sleeve and the cutting tip.

Recently, a new cataract removal technique has been developed that involves the injection of hot (approximately 45°C to 105°C) water or saline to liquefy or gellate the hard lens nucleus, thereby making it possible to aspirate the liquefied lens from the eye. Aspiration is conducted with the injection of the heated solution and the injection of a relatively cool solution, thereby quickly cooling and removing the heated solution. This technique is more fully described in U.S. Patent No. 5,616,120 (Andrew, et al.), the entire contents of which is incorporated herein by reference. The apparatus disclosed in the publication, however, heats the solution separately from the surgical handpiece. Temperature control of the heated solution can be difficult because the fluid tubings feeding the handpiece typically are up to two meters long, and the heated solution can cool considerably as it travels down the length of the tubing.

Therefore, a need continues to exist for a surgical handpiece that can heat internally the solution used to perform the liquefracture technique.

Brief Summary of the Invention

The present invention improves upon the prior art by providing a tip for a liquefraction surgical handpiece. The tip uses at least two tubes. One tube is used for aspiration and at least one other tube is used to inject heated surgical fluid for liquefying a cataractous lens. The distal portion of the injection tube terminates just inside of the aspiration tube so that heated fluid escaping the injection tube reflects off of the internal wall of the aspiration tube prior to entering the eye. The internal wall is textured or roughened to further diffract the fluid stream. Such an arrangement prevents the injected fluid from directly entering the eye. The handpiece may also contain other tubes, for example, for injecting relatively cool surgical fluid.

Accordingly, one objective of the present invention is to provide a surgical handpiece having at least two tubes.

Another objective of the present invention is to provide a safer tip for a surgical handpiece having a pumping chamber.

Another objective of the present invention is to provide a surgical handpiece having a device for delivering the surgical fluid through the handpiece in pulses that do not directly enter the eye.

These and other advantages and objectives of the present invention will become apparent from the detailed description and claims that follow.

Brief Description of the Drawings

FIG. 1 is a front, upper left perspective view of the handpiece of the present invention.

FIG. 2 is a rear, upper right perspective view of the handpiece of the present invention.

FIG. 3 is a cross-sectional view of the handpiece of the present invention taken along a plane passing through the irrigation channel.

FIG. 4 is a cross-sectional view of the handpiece of the present invention taken along a plane passing through the aspiration channel.

FIG. 5 is an enlarged partial cross-sectional view of the handpiece of the present invention taken at circle 5 in FIG. 4.

5 FIG. 6 is an enlarged partial cross-sectional view of the handpiece of the present invention taken at circle 6 in FIG. 3.

FIG. 7 is an enlarged cross-sectional view of the handpiece of the present invention taken at circle 7 in FIGS. 3 and 4, and showing a resistive boiler pump.

10 FIG. 8 is a schematic cross-sectional view of a heating element boiler pump that may be used with the present invention.

FIG. 9 is an exploded, partial cross-section view of one embodiment of the handpiece of the present invention.

FIG. 10 is an enlarged cross-sectional view of one alternative tip design for use with the present invention.

15 FIG. 11 is an enlarged cross-sectional view of a second alternative tip design for use with the present invention.

Detailed Description of the Invention

Handpiece 10 of the present invention generally includes handpiece body 12 and operative tip 16. Body 12 generally includes external irrigation tube 18 and aspiration fitting 20. Body 12 is similar in construction to well-known in the art phacoemulsification handpieces and may be made from plastic, titanium or stainless steel. As best seen in FIG. 6, operative tip 16 includes tip/cap sleeve 26, tube 28 and tube 30. Sleeve 26 may be any suitable commercially available phacoemulsification tip/cap sleeve or sleeve 26 may be incorporated into other tubes as a multi-lumen tube. Tube 28 may be any commercially available hollow phacoemulsification cutting tip, such as the TURBOSONICS tip available from Alcon Laboratories, Inc., Fort Worth, Texas. Tube 30 may be any suitably sized tubing to fit within tube 28, for example 29 gauge hypodermic needle tubing. Alternatively, as best seen in FIG. 10, tube 30' may be external to tube 28' with a distal tip 27 that terminates within bore 29 of tube 28' near distal tip 31 of tube 28'. Preferably, tube 30' is angled at between 25° and 50° and terminates approximately 0.1 mm

to 3.0 mm from distal tip 31. Such an arrangement causes fluid exiting tube 28' to reflect off of internal wall 33 of tube 28' prior to exiting out of distal tip 31, thereby reducing the force of the pressure pulse prior to contact with eye tissue. The force of the pressure pulse decays with distance from tip 31; consequently, efficiency is best for tissue that is held at or within tip 31.

Alternatively, as seen in FIG. 11, internal wall 33' may contain texturing or roughening at area 5 so as to further diffract the fluid pulse prior to exiting distal tip 31.

As best seen in FIG. 5, tube 30 is free on the distal end and connected to pumping chamber 42 on the proximal end. Tube 30 and pumping chamber 42 may be sealed fluid tight by any suitable means having a relatively high melting point, such as silver solder. Fitting 44 holds tube 30 within bore 48 of aspiration horn 46. Bore 48 communicates with fitting 20, which is journaled into horn 46 and sealed with O-ring seal 50 to form an aspiration pathway through horn 46 and out fitting 20. Horn 46 is held within body 12 by O-ring seal 56 to form irrigation tube 52 which communicates with irrigation tube 18 at port 54.

As best seen in FIG. 7, in a first embodiment of the present invention, pumping chamber 42 contains a relatively large pumping reservoir 43 that is sealed on both ends by electrodes 45 and 47. Electrical power is supplied to electrodes 45 and 47 by insulated wires 49 and 51, respectively. In use, surgical fluid (*e.g.* saline irrigating solution) enters reservoir 43 through port 55, tube 34 and check valve 53, check valves 53 being well-known in the art. Electrical current (preferably Radio Frequency Alternating Current or RFAC) is delivered to and across electrodes 45 and 47 because of the conductive nature of the surgical fluid. As the current flows through the surgical fluid, the surgical fluid boils. As the surgical fluid boils, it expands rapidly out of pumping chamber 42 through port 57 and into tube 30 (check valve 53 prevents the expanding fluid from entering tube 34). The expanding gas bubble pushes the surgical fluid in tube 30 downstream of pumping chamber 42 forward. Subsequent pulses of electrical current form sequential gas bubbles that move surgical fluid down tube 30. The size and pressure of the fluid pulse obtained by pumping chamber 42 can be varied by varying the length, timing and/or power of the electrical pulse sent to electrodes 45 and 47 and by varying the dimensions of reservoir 43. In addition, the surgical fluid may be preheated prior to entering pumping chamber 42.

Preheating the surgical fluid will decrease the power required by pumping chamber 42 and/or increase the speed at which pressure pulses can be generated.

While several embodiments of the handpiece of the present invention are disclosed, any handpiece producing adequate pressure pulse force, rise time and frequency may also be used. For example, any suitable handpiece producing a pressure pulse force of between 0.03 grams and 3.0 grams, with a rise time of between 1 gram/sec. and 3,000 grams/sec and a frequency of between 1 Hz and 200 Hz may be used, with between 20 Hz and 100 Hz being most preferred. The pressure pulse force and frequency will vary with the hardness of the material being removed. For example, the inventors have found that a lower frequency with a higher pulse force is most efficient at debulking and removing the relatively hard nuclear material, with a higher frequency and lower pulse force being useful in removing softer epinuclear and cortical material. Infusion pressure, aspiration flow rate and vacuum limit are similar to current phacoemulsification techniques.

As best seen in FIG. 8, the fluid in reservoir 143 in pumping chamber 142 may also be heated by the use of heating element 145 that is internal to reservoir 143. Heating element 145 may be, for example, a coil of 0.003 inch diameter stainless steel wire which is energized by power source 147. The size and pressure of the fluid pulse obtained by pumping chamber 142 can be varied by varying the length and timing of the electrical pulse sent to element 145 by power source 147 and by varying the dimensions of reservoir 143. The numbers in FIG. 8 are identical to the numbers in FIG. 7 except for the addition of "100" in FIG. 8.

As best seen in FIGS. 3, 4 and 7, surgical fluid may be supplied to pumping chamber 43 through tube 34 or, as seen in FIG. 9, surgical fluid may be supplied to pumping chamber 243 through irrigation fluid tube 234 which branches off main irrigation tube 235 supplying cool surgical fluid to the operative site. As seen in FIG. 9, aspiration tube 237 may be contained internally to handpiece 10. The numbers in FIG. 9 are identical to the numbers in FIG. 7 except for the addition of "200" in FIG. 9.

Any of a number of methods can be employed to order limit the amount of heat introduced into the eye. For example, the pulse train duty cycle of the heated solution can be varied so that the total amount of heated solution introduced into the eye does not vary with the pulse frequency. Alternatively, the aspiration flow rate can be varied as a

function of pulse frequency so that as pulse frequency increases aspiration flow rate increases proportionally.

This description is given for purposes of illustration and explanation. It will be apparent to those skilled in the relevant art that changes and modifications may be made to the invention described above without departing from its scope or spirit. For example, it will be recognized by those skilled in the art that the present invention may be combined with ultrasonic and/or rotating cutting tips to enhance performance.

We claim:

1. A liquefaction handpiece, comprising:

- a) a body having an irrigation tube and an aspiration tube, the irrigation tube having a distal tip that terminates internal to the aspiration tube, the aspiration tube having an internal wall; and
- b) a roughen area on the internal wall opposite the distal tip of the irrigation tube.

2. The handpiece of claim 1 further comprising a second irrigation tube.

3. The handpiece of claim 2 wherein the second irrigation tube is mounted on the exterior of the body.

4. A liquefaction handpiece, comprising:

- a) a body having an irrigation tube and an aspiration tube, the irrigation tube being external to the aspiration tube and having a distal tip that terminates internal to the aspiration tube, the aspiration tube having an internal wall; and
- b) a roughen area on the internal wall opposite the distal tip of the irrigation tube.

5. The handpiece of claim 4 further comprising a second irrigation tube.

6. The handpiece of claim 4 wherein the second irrigation tube is mounted on the exterior of the body.

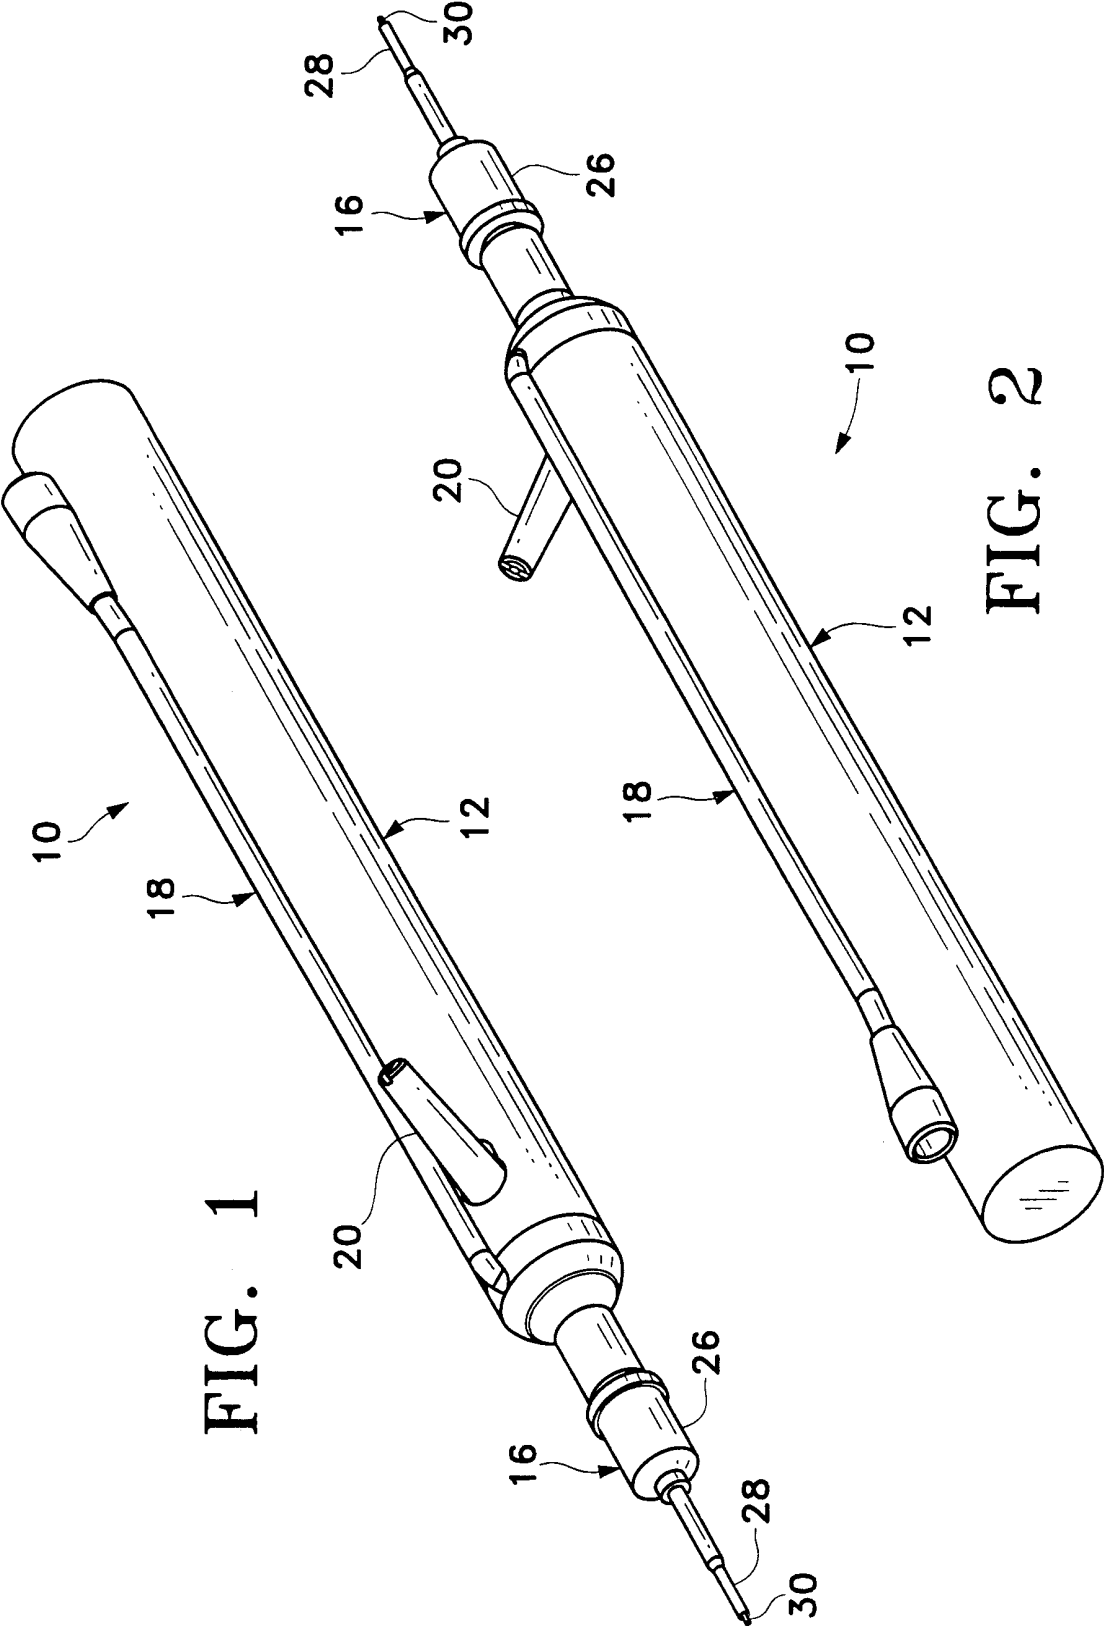
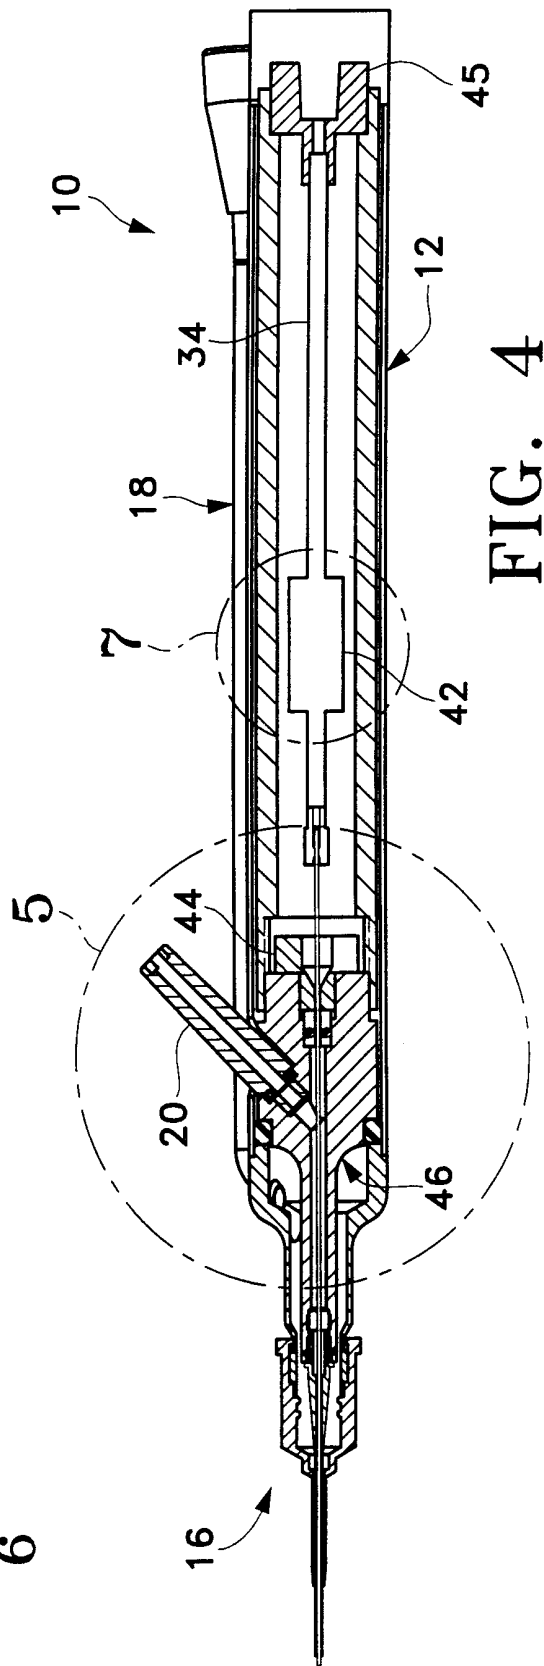
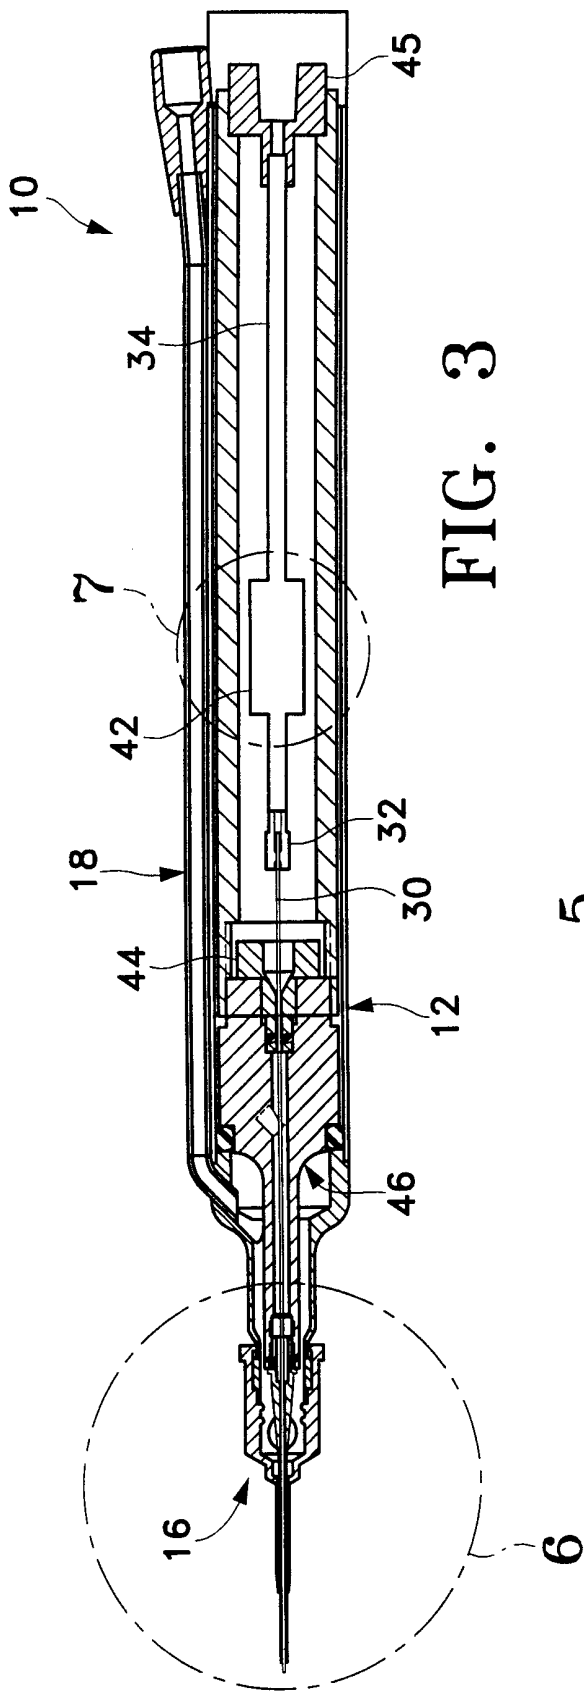
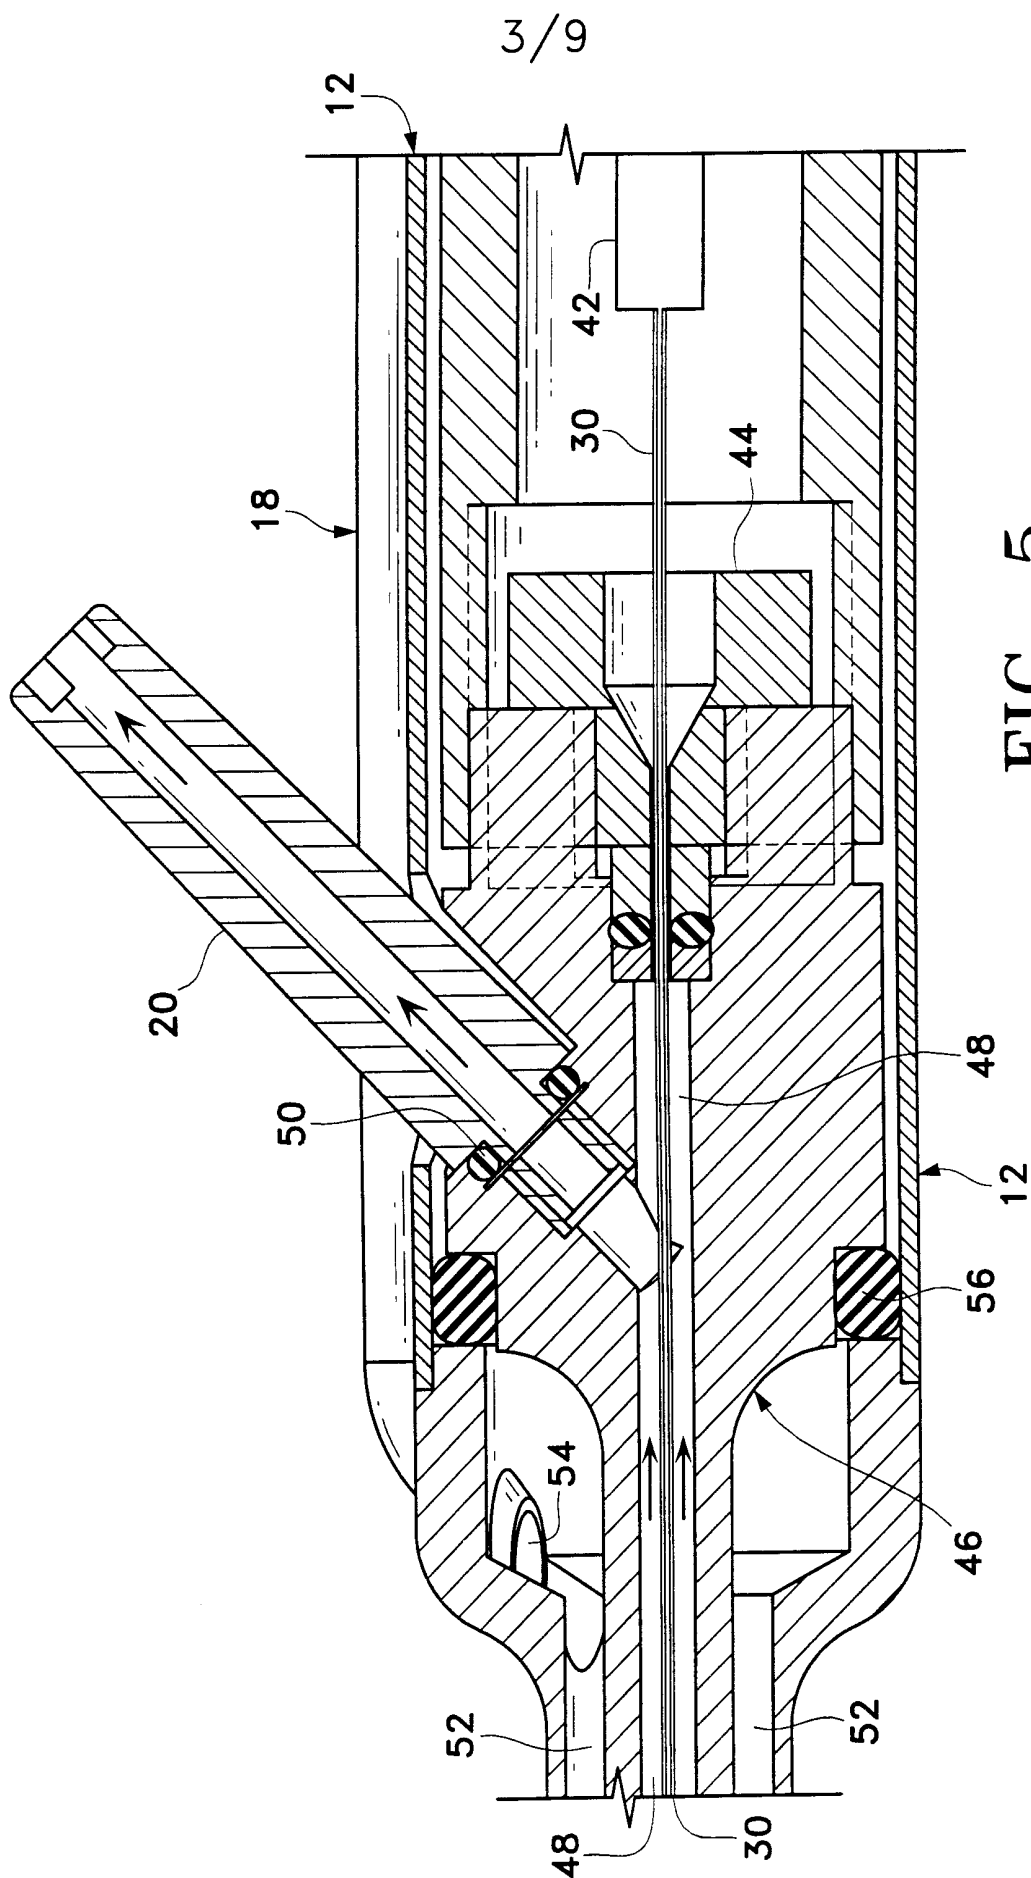


FIG. 1

FIG. 2





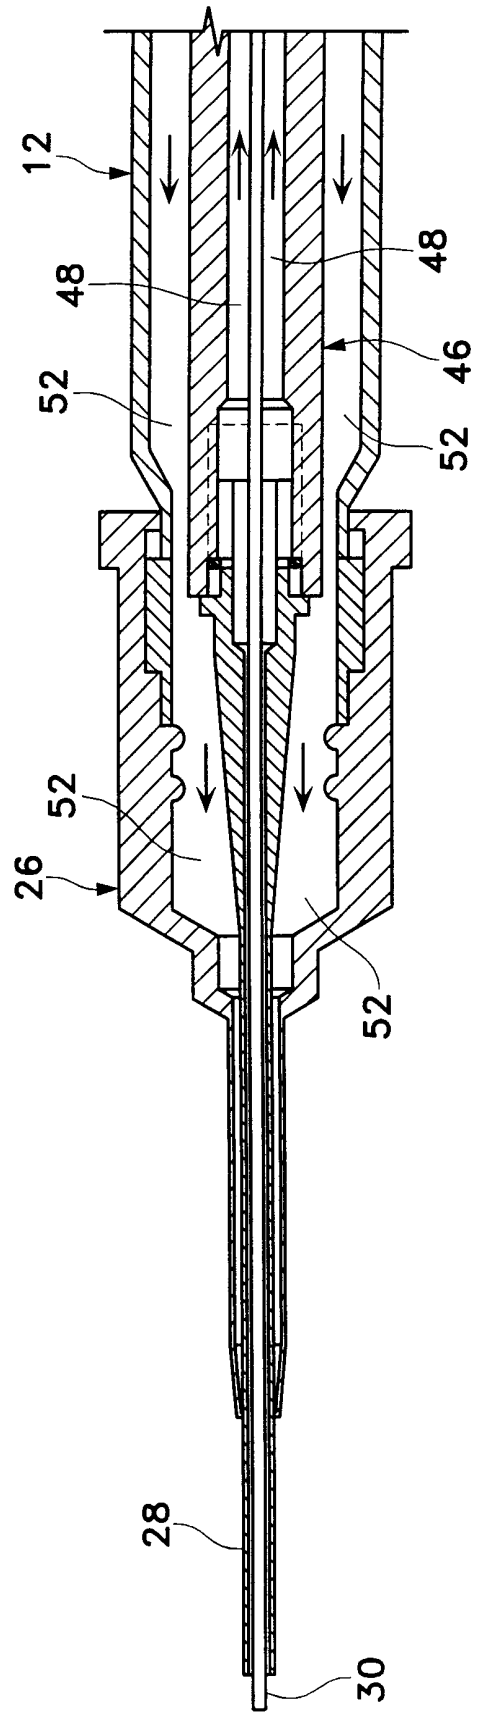


FIG. 6

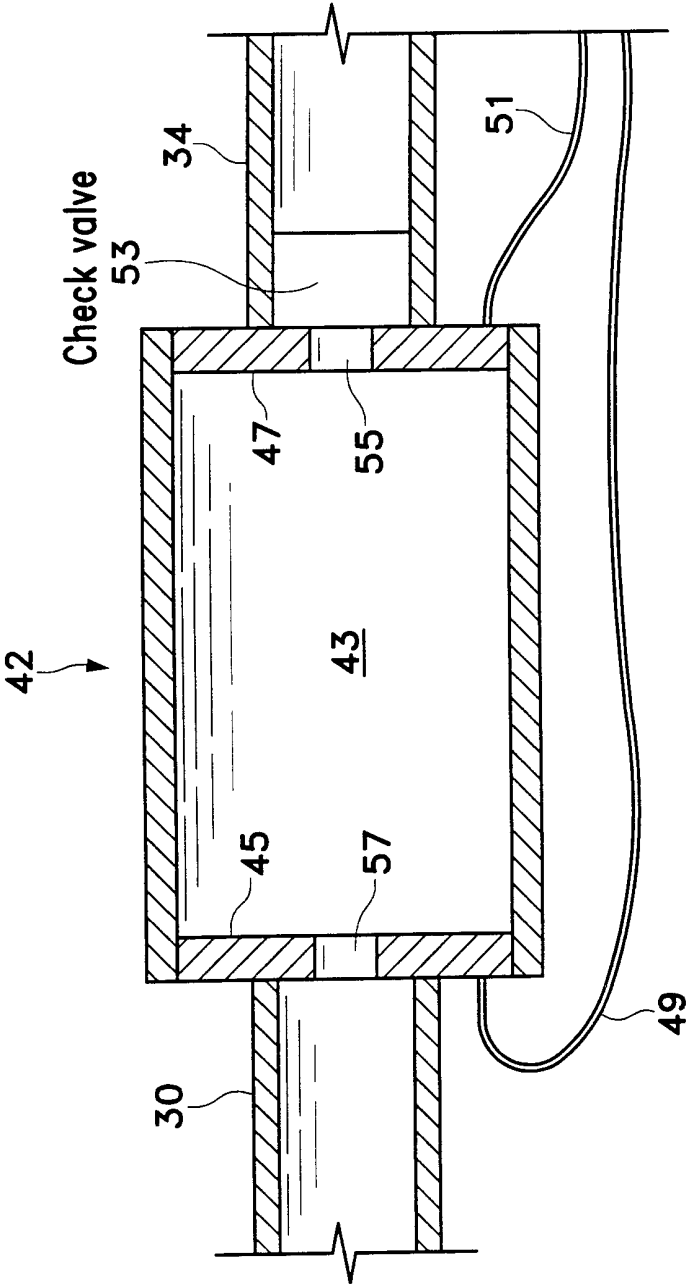


FIG. 7

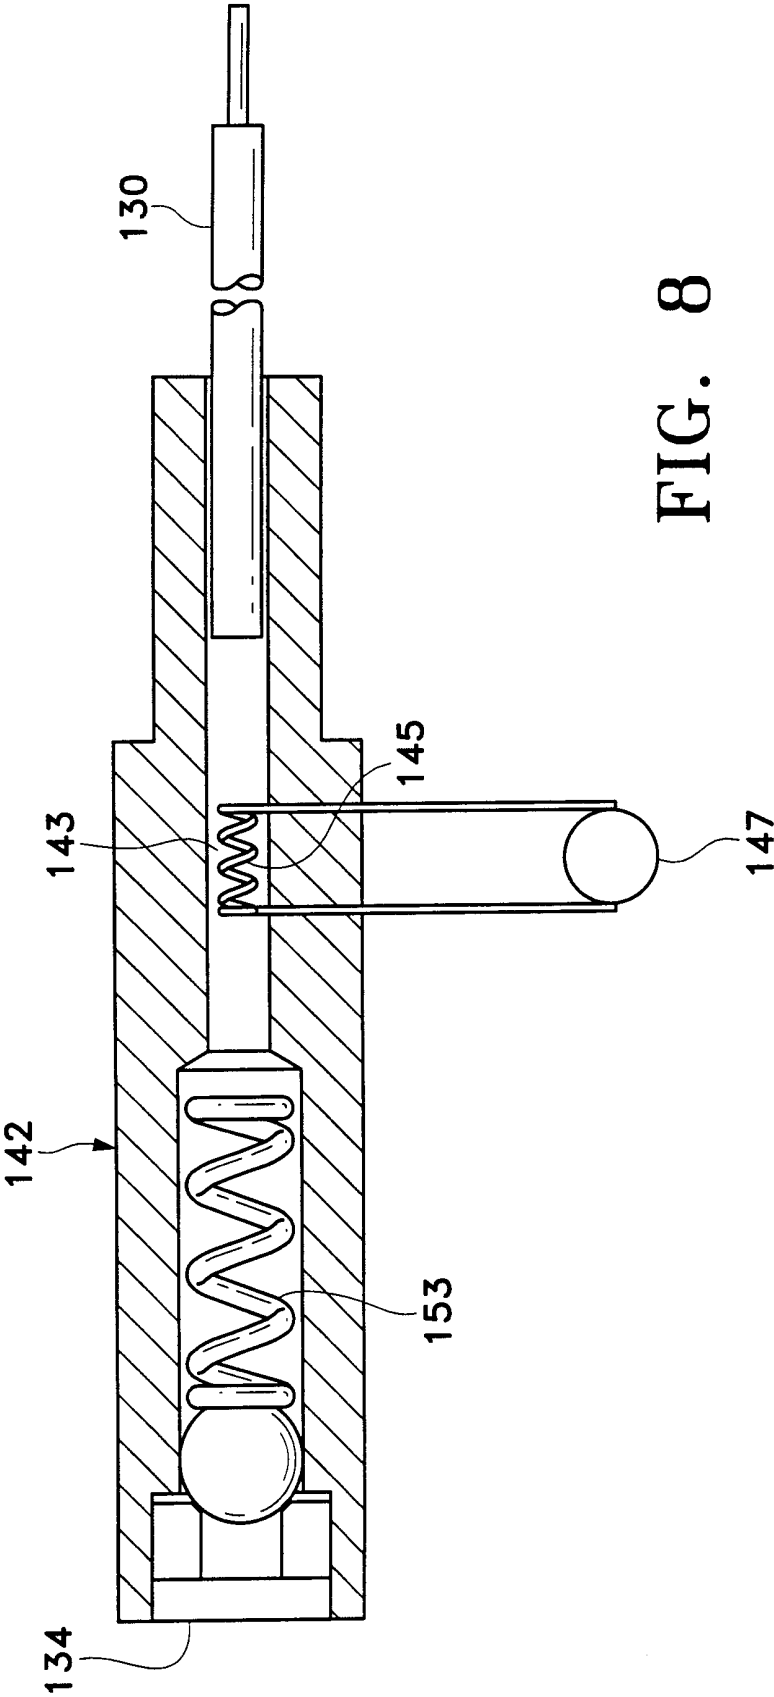


FIG. 8

7/9

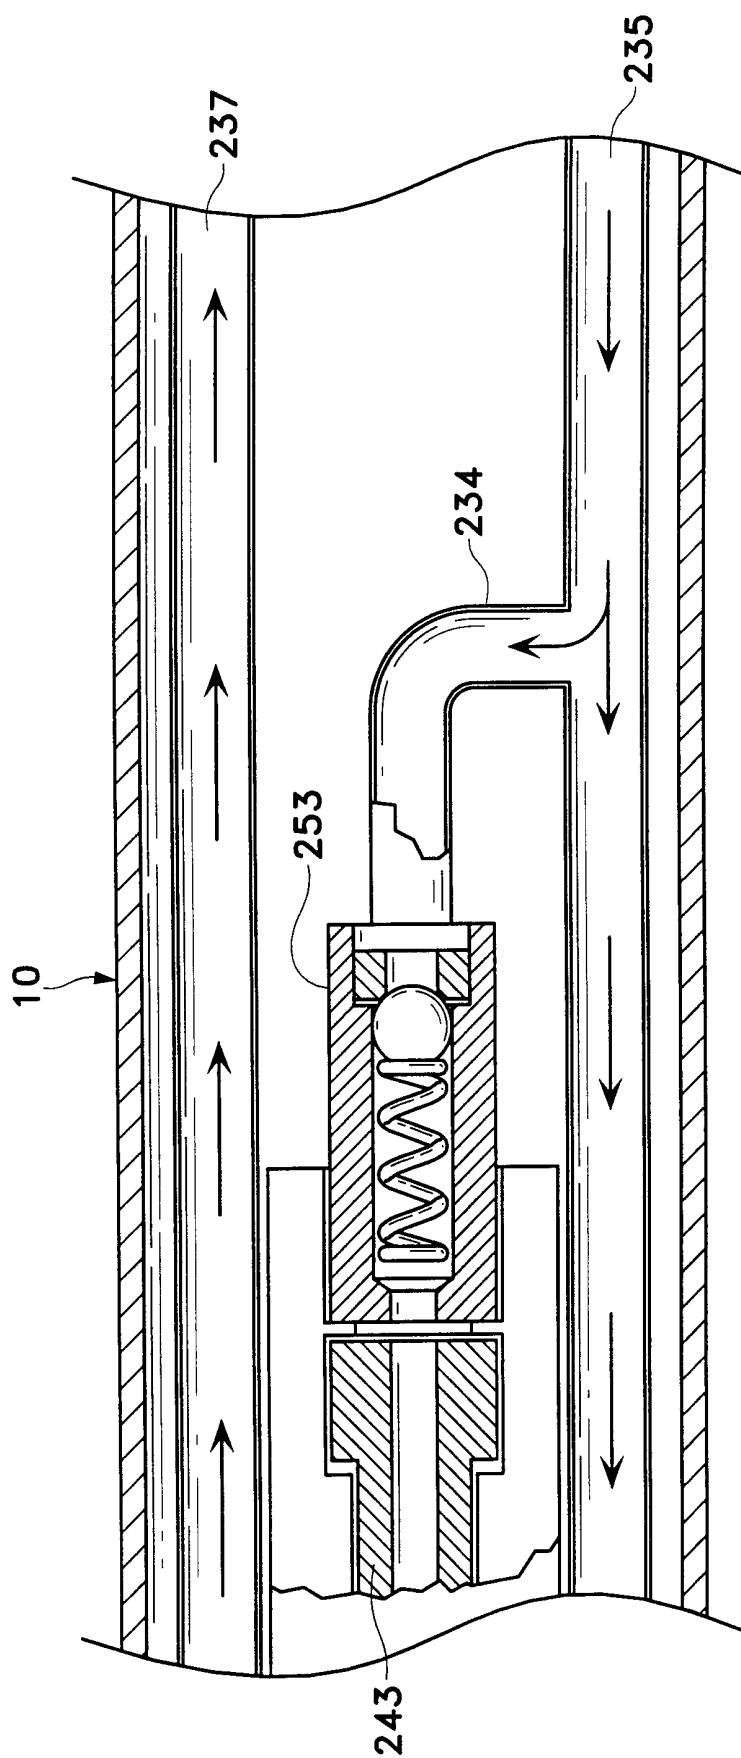


FIG. 9

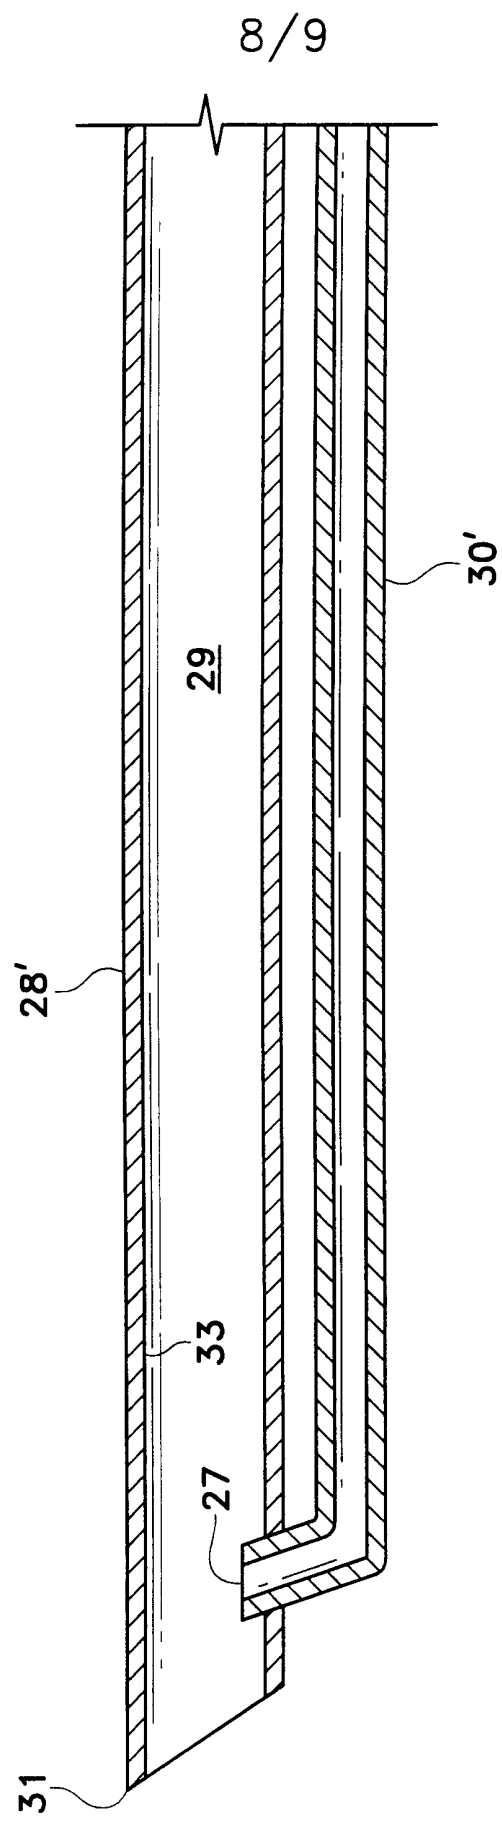


FIG. 10

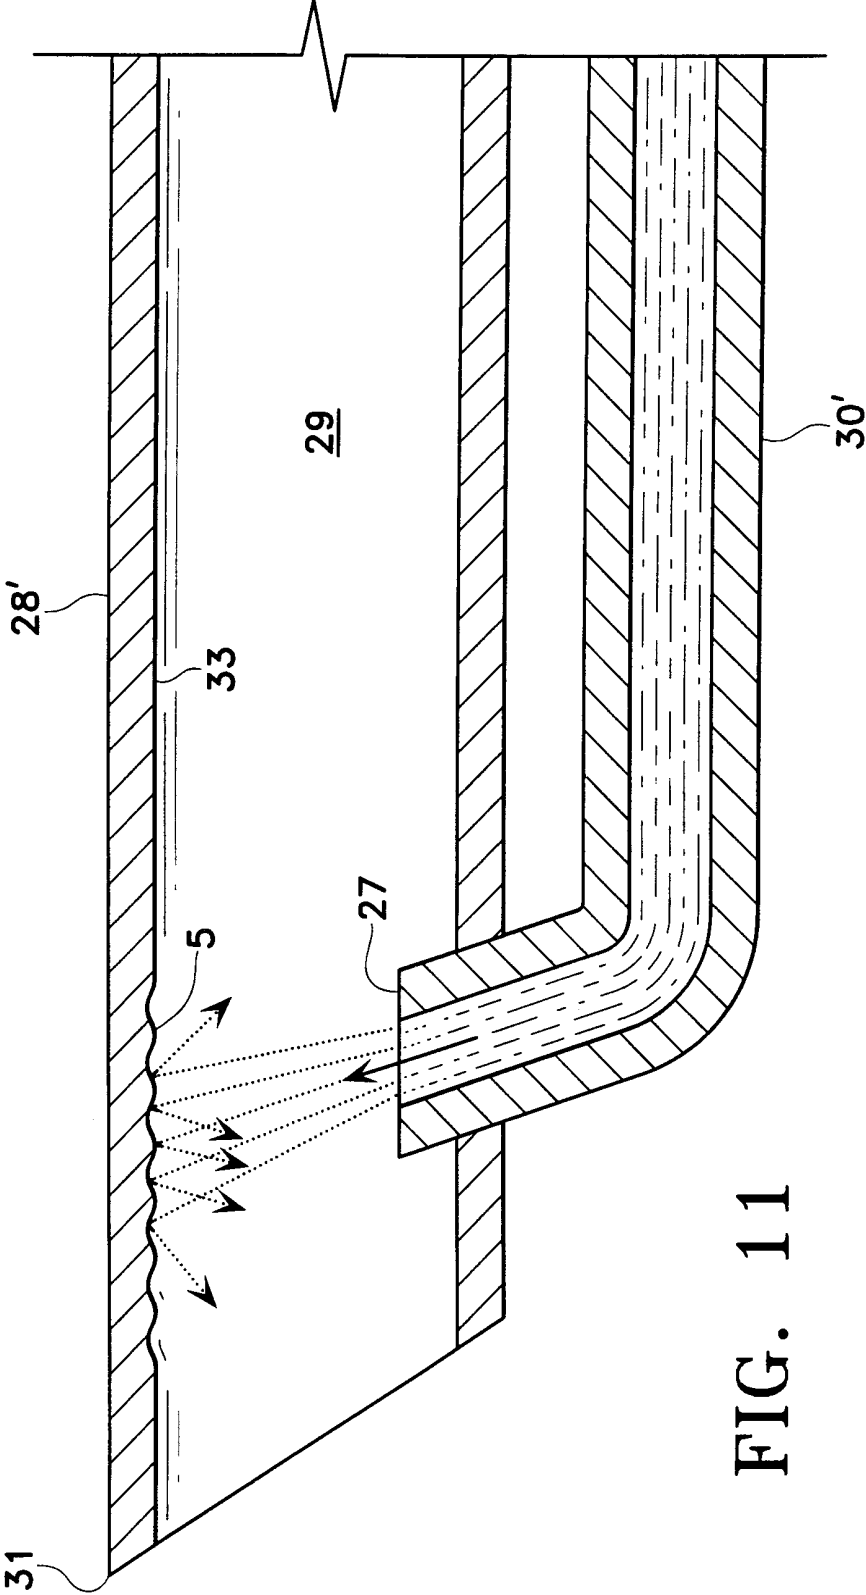


FIG. 11

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/24240

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61F9/007 A61B17/32

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 885 243 A (CAPETAN) 23 March 1999 (1999-03-23) column 2	1,4
A	US 5 674 226 A (DOHERTY) 7 October 1997 (1997-10-07) figures 1,4,6	1,4
A	US 5 865 790 A (BAIR) 2 February 1999 (1999-02-02) figures 2,4	1,4
A	US 5 616 120 A (ANDREW) 1 April 1997 (1997-04-01) cited in the application	

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

& document member of the same patent family

Date of the actual completion of the international search

20 December 2000

Date of mailing of the international search report

02/01/2001

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Barton, S

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 00/24240

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5885243 A	23-03-1999	AU 716239 B	24-02-2000
		AU 5100898 A	03-07-1998
		EP 0948300 A	13-10-1999
		WO 9825557 A	18-06-1998
US 5674226 A	07-10-1997	US 5308673 A	03-05-1994
		BR 9306324 A	13-01-1998
		CZ 9402726 A	14-06-1995
		DE 69304322 D	02-10-1996
		DE 69304322 T	17-04-1997
		EP 0639235 A	22-02-1995
		ES 2093428 T	16-12-1996
		GR 3021183 T	31-12-1996
		JP 7506505 T	20-07-1995
		MX 9302550 A	29-07-1994
		WO 9322485 A	11-11-1993
		US 5368668 A	29-11-1994
US 5865790 A	02-02-1999	US 5735815 A	07-04-1998
		AU 677061 B	10-04-1997
		AU 6746894 A	02-02-1995
		CA 2127637 A	27-01-1995
		DE 69414924 D	14-01-1999
		DE 69414924 T	27-05-1999
		EP 0636345 A	01-02-1995
		ES 2125379 T	01-03-1999
		JP 7313520 A	05-12-1995
		WO 9844853 A	15-10-1998
		US 5853384 A	29-12-1998
		US 5562692 A	08-10-1996
US 5616120 A	01-04-1997	AU 704305 B	22-04-1999
		AU 4691596 A	27-08-1996
		CA 2211031 A	15-08-1996
		EP 0812169 A	17-12-1997
		JP 10513091 T	15-12-1998
		WO 9624314 A	15-08-1996
		US 6074358 A	13-06-2000