



Office de la Propriété

Intellectuelle  
du Canada

Un organisme  
d'Industrie Canada

Canadian  
Intellectual Property  
Office

An agency of  
Industry Canada

CA 2286195 C 2006/02/14

(11)(21) 2 286 195

(12) BREVET CANADIEN  
CANADIAN PATENT

(13) C


(86) Date de dépôt PCT/PCT Filing Date: 1997/08/08  
(87) Date publication PCT/PCT Publication Date: 1998/10/15  
(45) Date de délivrance/Issue Date: 2006/02/14  
(85) Entrée phase nationale/National Entry: 1999/10/05  
(86) N° demande PCT/PCT Application No.: US 1997/014134  
(87) N° publication PCT/PCT Publication No.: 1998/045406  
(30) Priorité/Priority: 1997/04/09 (08/838397) US

(51) Cl.Int./Int.Cl. C12M 1/20 (2006.01),  
C12Q 1/04 (2006.01)

(72) Inventeurs/Inventors:  
WILLIAMS, MICHAEL G., US;  
HALVERSON, KURT J., US;  
KREJCAREK, GARY E., US;  
WEI, AI-PING, US;  
BERG, JAMES G., US;  
WICKERT, PETER D., US;  
CALHOUN, CLYDE D., US;  
...

(73) Propriétaire/Owner:  
MINNESOTA MINING AND MANUFACTURING  
COMPANY, US

(54) Titre : PROCEDE ET DISPOSITIFS POUR DIVISER DES LIQUIDES D'ECHANTILLONS BIOLOGIQUES EN  
MICROVOLUMES  
(54) Title: METHOD AND DEVICES FOR PARTITIONING BIOLOGICAL SAMPLE LIQUIDS INTO MICROVOLUMES

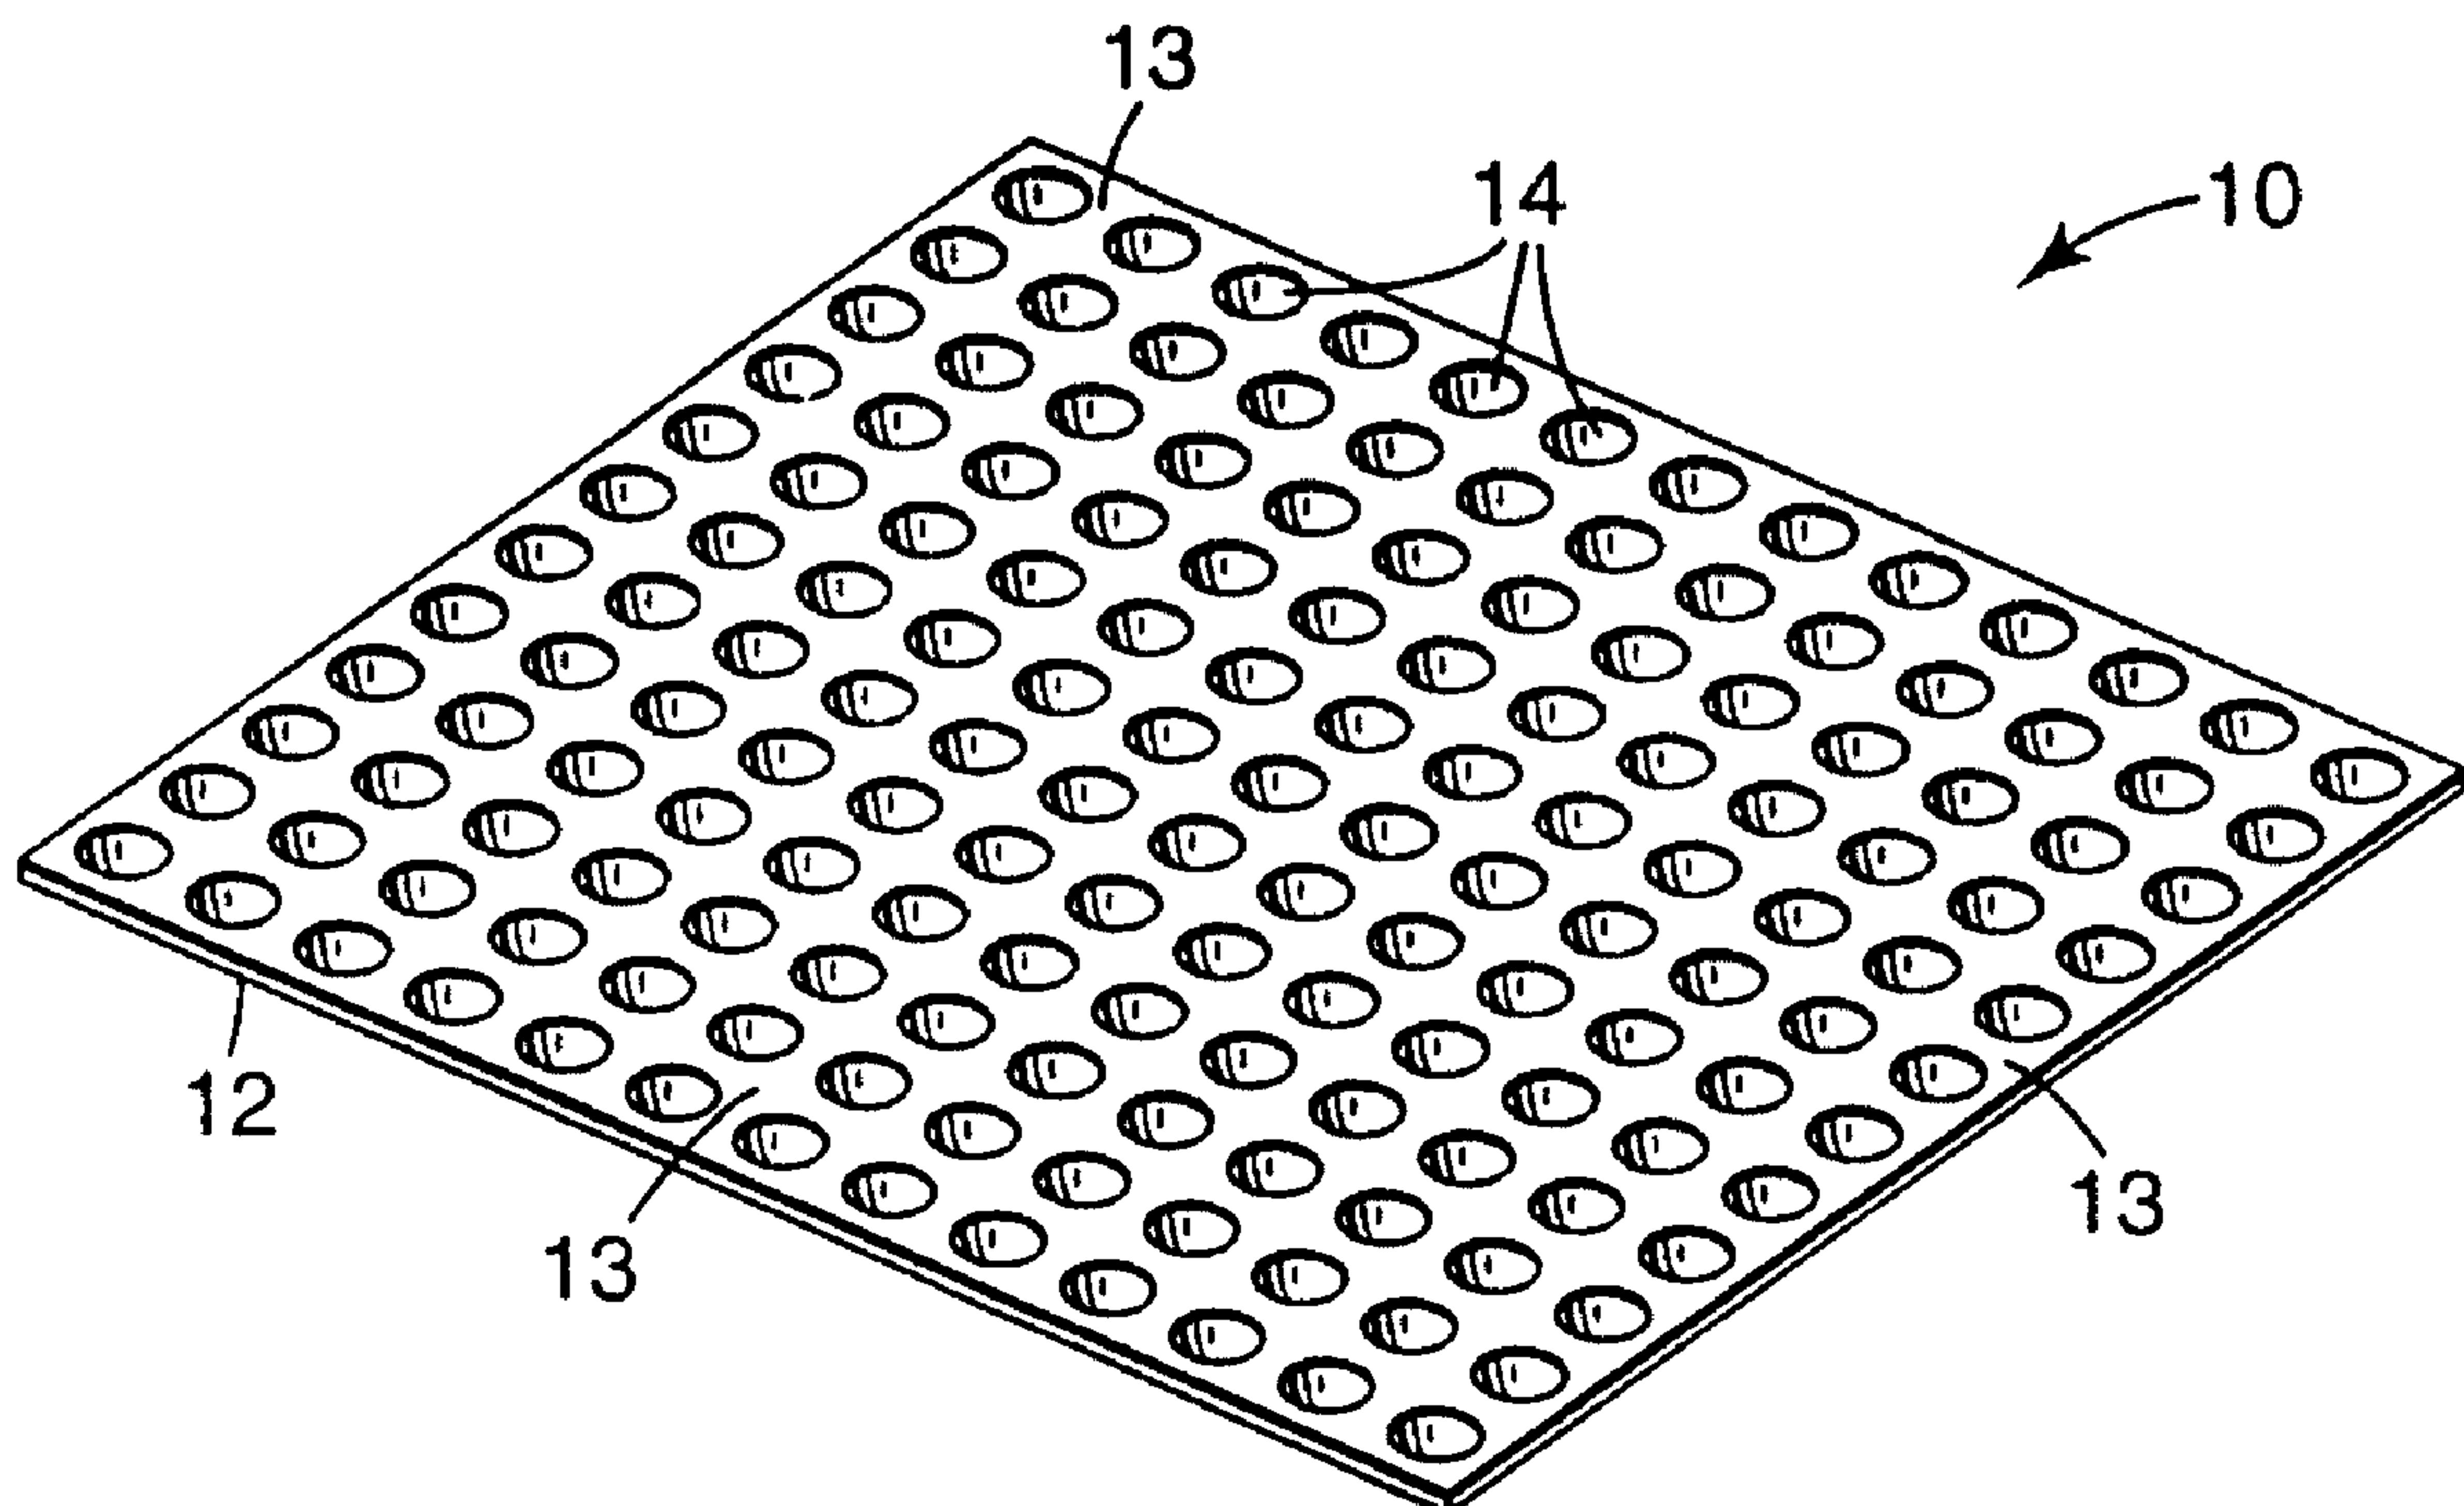

(57) Abrégé/Abstract:

A method for partitioning an aqueous biological liquid sample into discrete microvolumes for detection and enumeration of microorganisms is described. The method involves distributing microvolumes of a sample to a plurality of hydrophilic liquid-retaining zones of a culture device, where each liquid-retaining zone is surrounded by a portion of a hydrophobic "land" area. Also disclosed are devices for carrying out these methods.

(72) Inventeurs(suite)/Inventors(continued): DEBE, MARK K., US; QIU, JUN J., US

(74) Agent: SMART & BIGGAR


PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> :  C12M 1/20, B01L 3/00		A1	(11) International Publication Number: <b>WO 98/45406</b>  (43) International Publication Date: 15 October 1998 (15.10.98)
(21) International Application Number: PCT/US97/14134  (22) International Filing Date: 8 August 1997 (08.08.97)		(74) Agents: ROGERS, James, A. et al.; Minnesota Mining and Manufacturing Company, Office of Intellectual Property Counsel, P.O. Box 33427, Saint Paul, MN 55133-3427 (US).	
(30) Priority Data: 08/838,397 9 April 1997 (09.04.97) US		(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).	
(71) Applicant: MINNESOTA MINING AND MANUFACTURING COMPANY [US/US]; 3M Center, P.O. Box 33427, Saint Paul, MN 55133-3427 (US).		Published <i>With international search report.</i>	
(72) Inventors: WILLIAMS, Michael, G.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). HALVERSON, Kurt, J.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). KREJCAREK, Gary, E.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). WEI, Ai-Ping; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). BERG, James, G.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). WICKERT, Peter, D.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). CALHOUN, Clyde, D.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). DEBE, Mark, K.; P.O. Box 33427, Saint Paul, MN 55133-3427 (US). QIU, Jun; P.O. Box 33427, Saint Paul, MN 55133-3427 (US).			

(54) Title: METHOD AND DEVICES FOR PARTITIONING BIOLOGICAL SAMPLE LIQUIDS INTO MICROVOLUMES

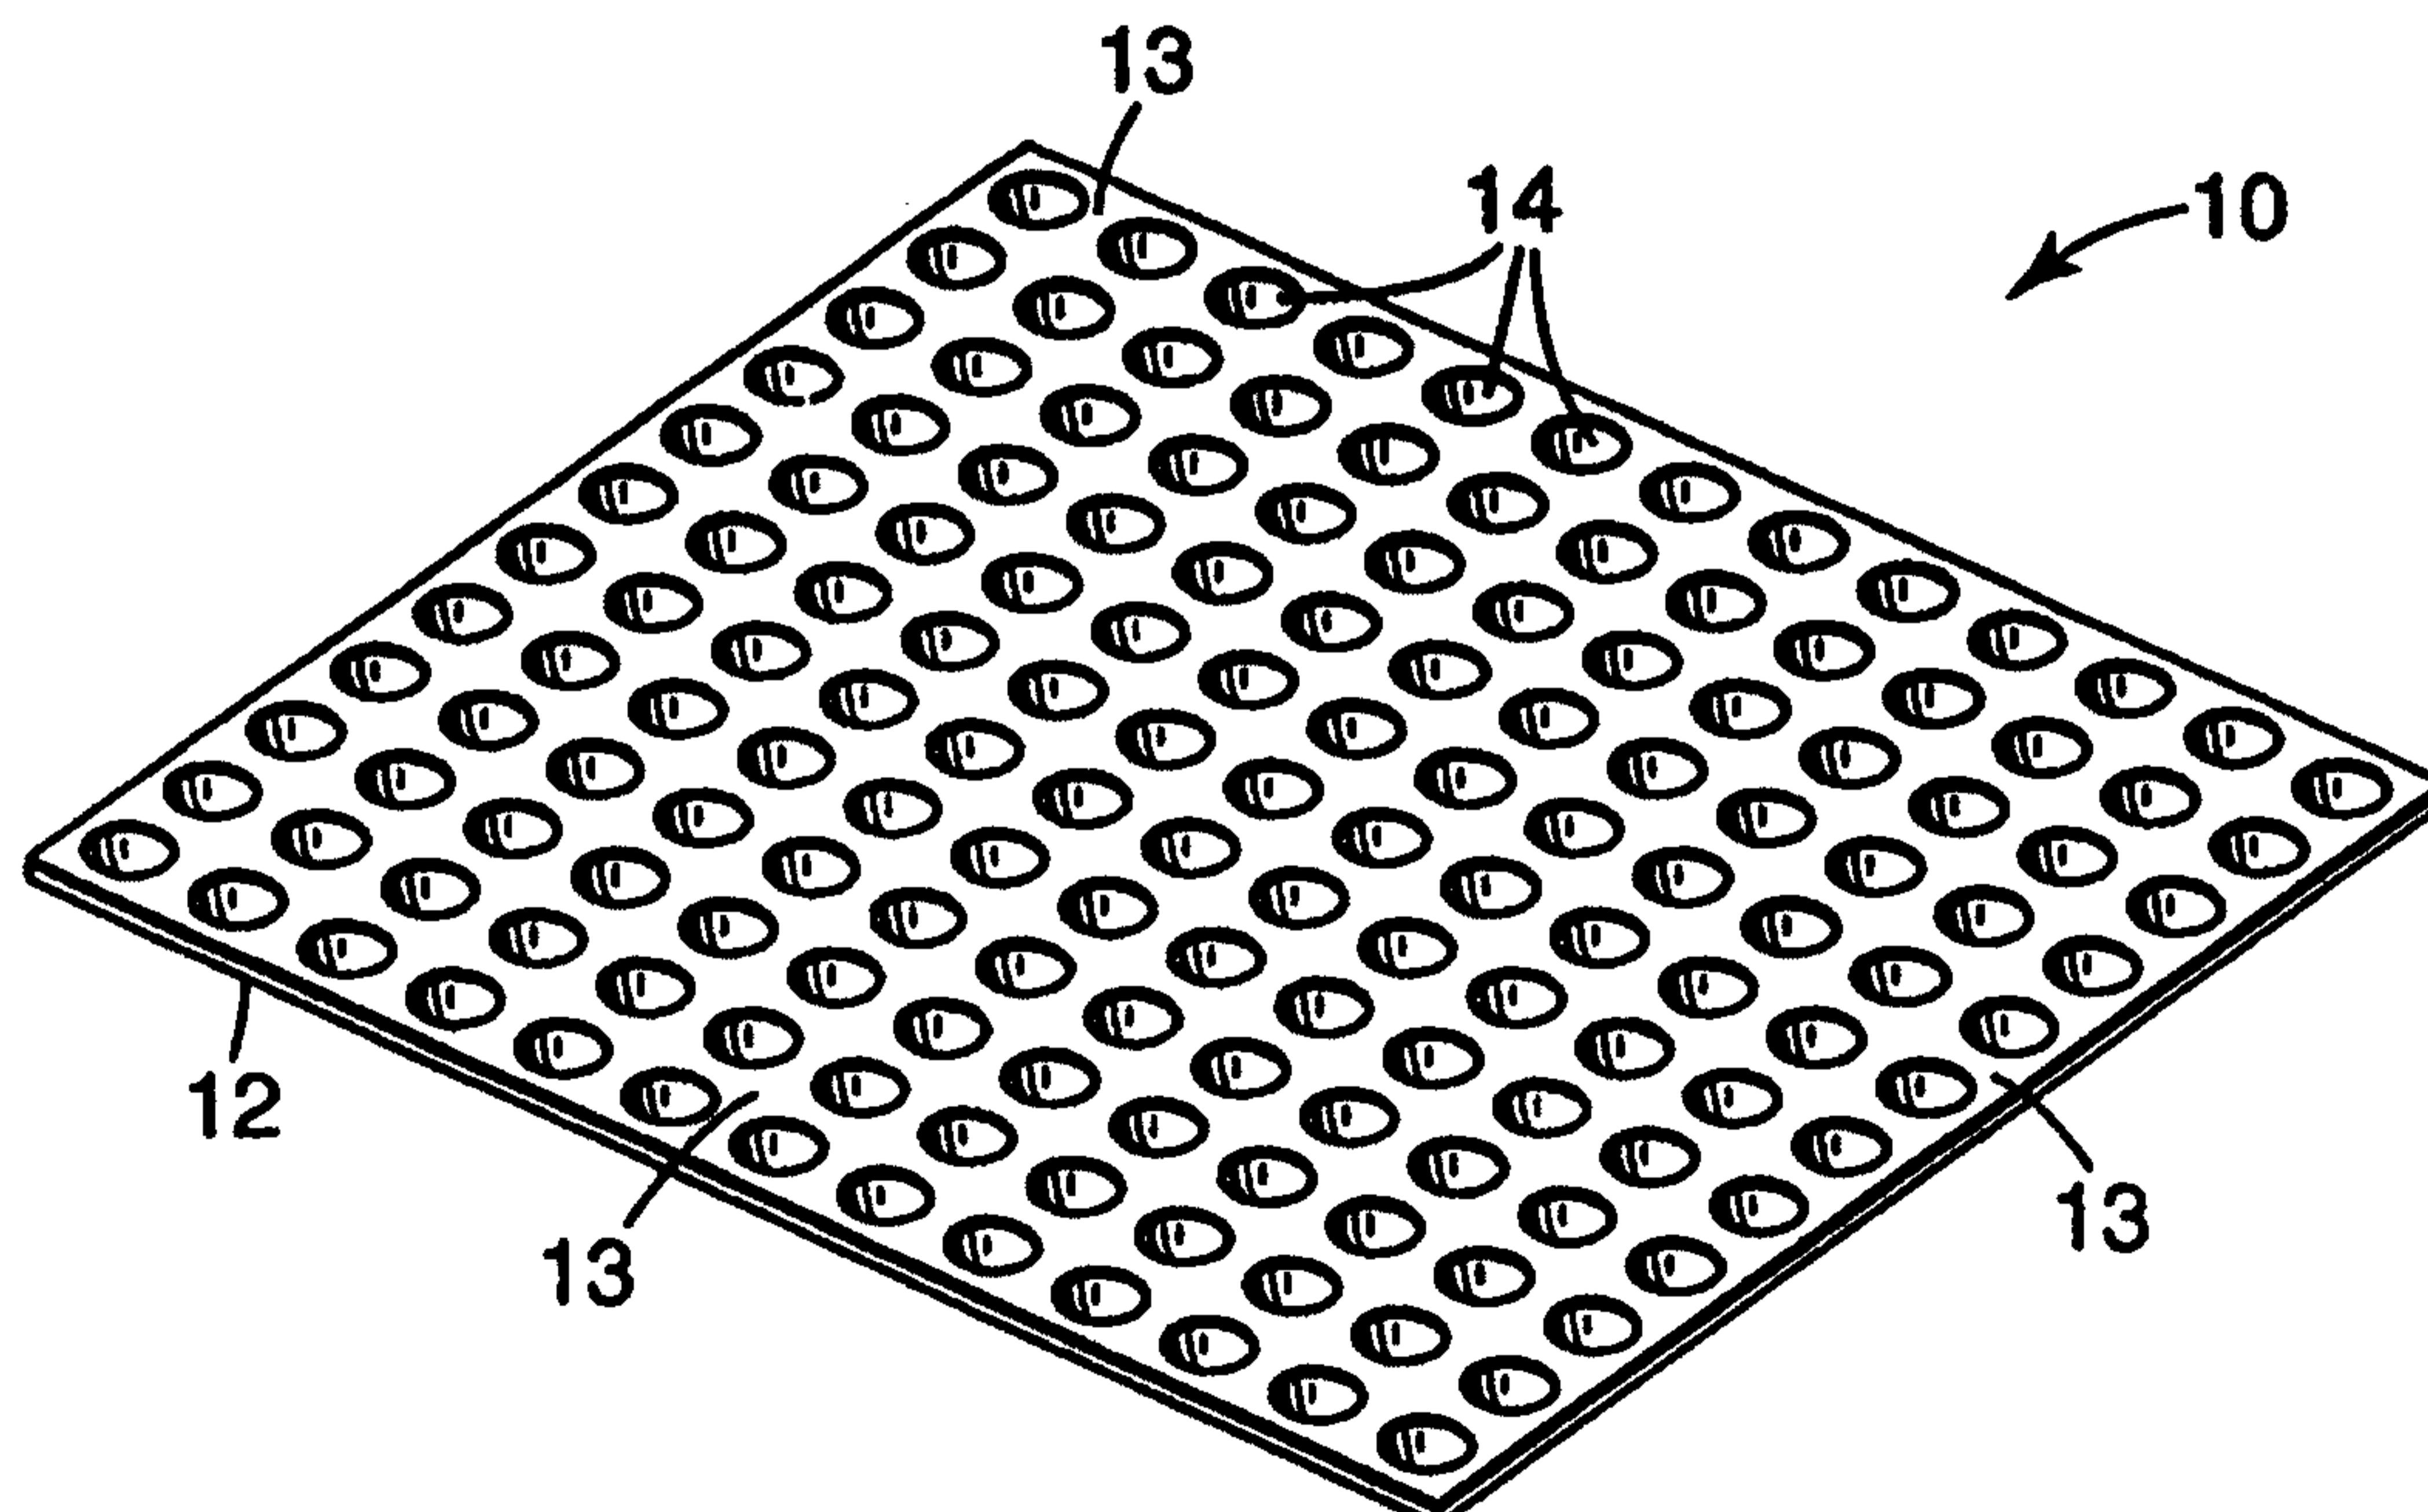

## (57) Abstract

A method for partitioning an aqueous biological liquid sample into discrete microvolumes for detection and enumeration of microorganisms is described. The method involves distributing microvolumes of a sample to a plurality of hydrophilic liquid-retaining zones of a culture device, where each liquid-retaining zone is surrounded by a portion of a hydrophobic "land" area. Also disclosed are devices for carrying out these methods.

METHOD AND DEVICES FOR PARTITIONING BIOLOGICAL SAMPLE

5

LIQUIDS INTO MICROVOLUMES

This invention relates to methods and devices for partitioning biological samples into microvolume aliquots, based on the tendency for aqueous liquids to be retained within hydrophilic zones of the devices while being substantially excluded from hydrophobic areas of the devices.

Background

15 The detection and enumeration of microorganisms is practiced in numerous settings, including the food-processing industry (testing for the contamination of food by microorganisms such as *E. coli* and *S. aureus*), the health care industry (testing of patient samples 20 and other clinical samples for infection or contamination), environmental testing industry, the pharmaceutical industry, and the cosmetic industry.

Growth-based detection and enumeration of microorganisms is commonly practiced using either 25 liquid nutrient media (most probable number analysis (MPN)) or semi-solid nutrient media (agar petri dishes). Enumeration using the liquid MPN method is typically achieved by placing serial 10-fold dilutions of a sample of interest in replicate sets of tubes 30 containing selective media and chemical indicators.

The tubes are incubated at elevated temperature (24-48 hours) followed by examination for growth of organisms.

A statistical formula, based on the number of positive and negative tubes for each set, is used to estimate 35 the number of organisms present in the initial sample.

This method of performing MPN analysis has several disadvantages. It is labor intensive because

WO 98/45406

PCT/US97/14134

of the multiple diluting and pipetting steps necessary to perform the analysis. In addition, in practice it is only practical to use replicate sets of about three to five tubes for each dilution. As a result, the 95%  
5 confidence limits for an MPN estimate for microbial concentration are extremely wide. For example, a three tube MPN estimate of 20 has 95% confidence limits ranging from 7 to 89.

In contrast to the method described above, a direct count of viable microorganisms in a sample can be achieved by spreading the sample over a defined area using nutrient media containing a gelling agent. The gelling agent (agar) prevents diffusion of the organisms during incubation (24-48 hours), producing a  
15 colony in the area where the original organism was deposited. There is, however, a limit to the number of colonies that can fit on a given area of nutrient media before fusion with neighboring colonies makes counting difficult. This usually necessitates performing  
20 several dilutions for each sample. In addition, the classes of chemical indicator molecules that can be used for identifying individual types of microorganisms present within a mixed population are limited to those that produce a product that is insoluble in the gelled  
25 media.

In addition to these disadvantages, both the currently used MPN analysis and gel-based systems require a relatively long incubation time before a positive result can be detected.

30

### Summary

The invention is based on the discovery that biological liquid samples can be partitioned into  
35 discrete microliters with only minimal manipulation on the part of an operator. The method of partitioning employs devices that have hydrophilic liquid-retaining

60557-6162

zones surrounded by hydrophobic "land" areas. The methods and devices provide a system for the detection and enumeration of microorganisms and other biological materials that solves the problems associated with currently used 5 systems. The system is a liquid-base system, allowing efficient and effective partitioning of the sample into discrete microvolumes for testing, and allows for rapid detection and enumeration.

In the case of MPN analysis for the detection and 10 enumeration of microorganisms, the approaches described herein allow for the use of water-soluble indicator species, and reduce or eliminate the need for the several dilutions typically required in current MPN analysis.

In general, the invention features a method for 15 partitioning an aqueous liquid sample into discrete microvolumes, comprising: a) providing a device for culturing a microorganism, the device comprising an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising 20 a hydrophobic material between the zones, each zone comprising dry media for growing microorganisms; and b) contacting the liquid sample with the assay surface such that the liquid sample is partitioned into the liquid-retaining zones.

25 The zones may comprise a coating or deposition of assay reagent, such as a nutrient medium or indicator substance. Appropriate indicator substances include without limitation chromogenic indicators, fluorescent indicators luminescent indicators and electrochemical indicators. For 30 purposes of this application, the term "electrochemical" means a chemical indicator that changes the resistance or

60557-6162

conductance of the sample upon reaction with the microorganism.

The zones may be of uniform size, with each zone having a liquid retention capacity of about 0.01 to about 25 5 microliters, more preferably about 1 to about 2 microliters.

The culture device can have, for example, about 10 to about 10,000 hydrophilic liquid-retaining zones, more preferably about 400 to about 600 hydrophilic liquid-retaining zones.

10 The hydrophilic liquid-retaining zones may comprise microvolume wells surrounded by a hydrophobic land area. Alternatively, the culture device may have a land area comprising a treated nanostructured film. In further alternative embodiments, the hydrophilic liquid-retaining 15 zones may comprise hydrophilic fiber material projecting from the assay surface. The fiber material can be constructed of hydrophilic absorbent discs or of hydrophilic nonwoven fiber loop material.

In an alternative embodiment, the culture device 20 may comprise a plurality of sets of hydrophilic liquid-retaining zones, each of the sets having zones of uniform size, the sets varying in liquid retention capacity, and the device having at least two sets of zones.

In another aspect, the invention features a 25 culture device for detection or enumeration of microorganisms, the device comprising an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising a hydrophobic material between the zones, each zone comprising

60557-6162

dry media for growing microorganisms; and at least one of the zones comprising an assay reagent. Each zone has a microvolume capacity of liquid retention, and at least some of the zones comprising an assay reagent.

5 The invention also provides a culture device for detection or enumeration of microorganism, said device comprising a substrate comprising liquid-retaining discs comprising a hydrophilic material, wherein said substrate comprises a material that is hydrophobic relative to said 10 liquid-retaining discs and wherein the discs comprise dry media for growth of microorganisms.

The invention further provides a method for partitioning an aqueous liquid sample into discrete microvolumes, comprising: a) providing a device for 15 culturing a microorganism, said device comprising an assay surface, said surface comprising liquid-retaining discs comprising a hydrophilic material and a land area comprising a hydrophobic material between said discs, each said disc comprising dry media for growing microorganism; and b) 20 contacting said liquid sample with said assay surface such that said liquid sample is partitioned into said liquid-retaining discs.

The invention still further provides a method for partitioning an aqueous liquid sample into discrete volumes 25 to conduct a most probable number analysis, comprising: a) providing a device for culturing a microorganism, the device including an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising a hydrophobic material between the 30 zones; b) contacting a liquid sample with the assay surface such that the liquid sample partitions into the liquid-

60557-6162

retaining zones; c) incubating the device; d) detecting a signal that indicates microorganisms are growing in a zone; and e) conducting a most probable number analysis based on the number of zones wherein a signal is detected.

5 As used herein, the term "microorganism" includes all microscopic living organisms and cells, including without limitation bacteria, mycoplasmas, rickettsias, spirochetes, yeasts, molds, protozoans, as well as microscopic forms of eukaryotic cells, for example single  
10 cells (cultured or derived directly from a tissue or organ) or small clumps of cells.

WO 98/45406

PCT/US97/14134

Microorganisms are detected and/or enumerated not only when whole cells are detected directly, but also when such cells are detected indirectly, such as through detection or quantitation of cell fragments, cell-derived biological molecules, or cell by-products.

The terms "hydrophobic" and "hydrophilic" are herein given the meanings commonly understood in the art. Thus, a "hydrophobic" material has relatively little or no affinity for water or aqueous media, while a "hydrophilic" material has relatively strong affinity for water or aqueous media. The relative hydrophobicities and hydrophilicities of the devices described herein are such as to ensure partitioning of liquid samples substantially into the described hydrophilic liquid-retaining zones upon application of the sample. The required levels of hydrophobicity and hydrophilicity may vary depending on the nature of the sample, but may be readily adjusted based on simple empirical observations of the liquid sample when applied to the devices.

Other advantages of the invention will be apparent from the following detailed description and the figures.

25

#### Brief Description of the Figures

Figure 1 is a perspective view of one embodiment of an assay device.

Figure 2 depicts a top view of an assay device having sets of hydrophilic liquid-retaining zones varying in microvolume capacity of liquid retention.

Figure 3 is a schematic representation of an assay device including a hydrophobic nanostructured film.

Figure 4 is a schematic representation of an assay device in which the hydrophilic liquid-retaining zones are constructed of paper discs.

Figure 5a is a perspective view of an assay

WO 98/45406

PCT/US97/14134

device in which the hydrophilic liquid-retaining zones are constructed of nonwoven fiber loop material.

Figure 5b is an expanded top view of the device depicted in Figure 5a.

5       Figure 6a is a photograph of a top view of an assay device in which the assay surface is hydrophilic.

Figure 6b is a photograph of a top view of an assay device with hydrophilic liquid-retaining zones and hydrophobic land areas.

10

#### Detailed Description

This invention relates to partitioning of biological samples into microvolume liquid sample aliquots for signal-based detection and enumeration of 15 microorganisms in liquid samples.

Among the problems encountered in the art relating to the testing of liquid samples for microorganisms are relatively lengthy incubation times, the need to undertake multiple pipetting operations for 20 aliquots being tested, and the need for a relatively large volume of sample for testing.

The present invention provides a solution to these and other problems associated with such testing.

Methods and devices are provided for partitioning a 25 liquid sample into microvolume compartments of a test device, with only minimal manipulation of the liquid sample required of the laboratory technician or other operator. A "microvolume," as that term is used herein, refers to a volume of less than about 25 30 microliters, and includes volumes in the sub-microliter range. The present inventors have discovered that the use of microvolumes in signal-based detection of microorganisms in liquid samples results in remarkably shorter incubation times required to produce a 35 detectable signal. Because shorter incubation times are highly desirable in this field, this feature of the invention provides a distinct advantage.

WO 98/45406

PCT/US97/14134

In addition to achieving shorter incubation times, the use of microvolumes in the testing of liquid samples may allow for the use of substantially smaller test samples. Very small volume test samples are 5 sometimes necessary due to very small volume sample sources. Small volume liquid test samples are also sometimes desirable, for example to ease handling or transport of the sample to a testing facility.

The present inventors have developed a number of 10 novel devices for partitioning of biological liquid samples into discrete microvolumes within hydrophilic liquid-retaining zones (also referred to herein as "liquid-retaining zones" or "zones"). Non-limiting examples of these devices include: micro-embossed or 15 pressed films having a plurality of microcompartments, for example microvolume wells, functioning as liquid-retaining zones, with the area between the wells ("land area") being hydrophobic and the wells being hydrophilic; nanostructured hydrophobic films in which 20 discrete liquid-retaining zones of the film are hydrophilic and are adapted to retain microvolumes of a liquid sample for testing; and devices having hydrophilic liquid-retaining zones and hydrophobic land areas, where a given hydrophilic zone is fabricated 25 from hydrophilic fiber material and projects upward or downward from the plane of the surrounding land area.

Advantageously, the above-summarized devices allow for the testing of liquid samples using 30 microvolume aliquots in a single device, eliminating the need for separate vessels in such testing. A test sample may be distributed among hundreds or even thousands of discrete liquid-retaining zones, substantially increasing the number of data points in a test of the liquid sample.

35 A particularly useful application of these methods and devices is in the growth-based detection and enumeration of microorganisms in liquid test

WO 98/45406

PCT/US97/14134

samples. Such growth-based detection and enumeration is very important in the testing of food, environmental, clinical, pharmaceutical, cosmetic, and other samples for contamination by microorganisms. The 5 methods and devices of this invention allow for the efficient, accurate, convenient, and cost-effective testing of such samples.

A preferred use of the methods and devices of this invention in such microbiological testing is in 10 MPN. In traditional MPN, a sample of interest is serially diluted (10 fold) and pipetted in equal amounts into replicate sets of tubes containing selective growth media and chemical indicators. The tubes are incubated at elevated temperature for about 15 24-48 hours followed by examination for growth of organisms. A statistical formula, based on the number of positive and negative tubes for each set, is used to estimate the number of organisms present in the initial sample. As currently used, this traditional method has 20 several disadvantages. It is labor intensive because of the multiple diluting and pipetting steps required to perform the analysis. As a practical matter, only replicate sets of about three to five tubes for each dilution are commonly used. As a result, the 95% 25 confidence limits for an MPN estimate of microbial concentration using this method are extremely wide. For example, a nine tube (3 ten-fold dilutions) MPN estimate of 20 has 95% confidence limits ranging from 7 to 89.

30 The use of the methods and devices of the present invention in MPN analysis overcomes several of the above-noted disadvantages. The amount of labor is greatly reduced because no pipetting into individual tubes is necessary, and very little or no agitation or 35 other manipulations are required. Instead, the liquid sample is distributed to microvolume liquid-retaining zones by simply contacting the liquid sample with the

WO 98/45406

PCT/US97/14134

device. In addition, fewer sample dilutions are necessary when large numbers of liquid-retaining zones are present in the device. The relatively large number of liquid-retaining zones also provides a more accurate 5 estimate of microbial concentration. This is because the correspondingly larger number of data points provides a correspondingly narrower confidence limit interval.

Accordingly, the present invention provides a 10 method for detecting (including enumerating) a microorganism in a liquid test sample. The method involves distributing microvolumes of the test sample to a plurality of hydrophilic liquid-retaining zones of an assay device. The assay device may be any device 15 that includes an assay surface having a plurality of hydrophilic liquid-retaining zones, where each zone has a microvolume capacity of liquid retention. The device also includes a land area between the zones that is hydrophobic and remains substantially free of liquid 20 after the biological sample has become distributed into the liquid-retaining zones. Non-limiting examples of such assay devices include those described herein.

The liquid-retaining zones in the assay device preferably are of uniform size and each zone has a 25 liquid-retention capacity of about 0.01 to about 25 microliters of the liquid sample. Preferably, each zone has a liquid retention capacity of about 0.1 to about 10 microliters, and more preferably about 1 to about 2 microliters. The assay device preferably 30 contains between 1 and about 100,000 liquid-retaining zones, more preferably about 10 to about 10,000 zones, even more preferably about 200 to about 5,000 zones and most preferably about 400 to about 600 zones.

The use of a device having about 400 to about 35 600 hydrophilic liquid-retaining zones is particularly useful in the context of testing a liquid sample for microorganism concentration using MPN. Certain

WO 98/45406

PCT/US97/14134

regulatory requirements may dictate that a testing method must be able to detect one microorganism in a one-to-five-milliliter sample. Such a sample size is standard in the food processing industry for 5 microbiological testing. Thus, for example, an assay device having 500 hydrophilic liquid-retaining zones, where each zone has a liquid capacity of about 2 microliters, would be very useful for testing a 1-ml sample. A liquid-retention zone having a capacity of 2 10 microliters allows for rapid development of a detectable signal in accordance with the invention, and the use of about 400 to about 600 zones provides a sufficiently large number of data points to substantially improve the confidence interval for an 15 MPN calculation. In addition, it is feasible to perform a manual count of liquid-retaining zones testing positive for the microorganism. Use of devices having substantially more than 400 liquid-retaining zones may require, as a practical matter, instrument- 20 assisted or automated counting.

The liquid test sample may be any sample of interest, from any source. The sample may be distributed to the plurality of liquid-retaining zones directly, or the sample may be diluted before 25 distribution to the zones. The determination as to whether sample dilution is necessary will depend on a variety of factors such as sample source and age, and such determination is a routine matter to those of skill in the art.

30 The liquid test sample may include selective nutrient growth media for the microorganism of interest, and/or an indicator substance that produces a signal in the presence of the growing microorganism. Optionally, the nutrient medium may include a gelling 35 agent that assists in "encapsulating" the growing microorganisms. Such gelling agents are known to those of skill in the art, and include any water-absorbing

WO 98/45406

PCT/US97/14134

material that becomes a gel upon addition of an aqueous liquid.

Alternatively, one or both of the selective nutrient growth media and the indicator substance may 5 be present as a coating or other deposition within a liquid-retaining zone, in amounts sufficient to achieve desired concentrations when a microvolume of the liquid test sample is distributed into the zone. Such a coating may be achieved, for example, by placing or 10 distributing a solution of the nutrient medium (with or without gelling agent) and/or indicator substance into the liquid-retaining zone and drying the solution to produce a coating or deposition of the nutrient medium and/or indicator substance in the zone.

15 A wide variety of selective growth media for a wide variety of microorganisms of interest is known, as is a wide variety of indicator substances for a wide variety of microorganisms, and any of these media or indicator substances is suitable for use in the method 20 of the invention. An advantage of the present invention is that soluble indicators can be used; since diffusion is prevented by confinement of the aqueous biological sample liquid in the hydrophilic liquid-retaining zones.

25 Various methods may be employed to distribute a liquid test sample to the liquid-retaining zones. More than one method may be applicable to a particular device, although the preferred method may depend to some extent on the configuration of a particular assay 30 device. For example, for film devices containing hydrophilic microvolume wells or for devices in which the zones comprise hydrophilic fiber material projecting from the plane of the assay surface, the sample may be poured or pipetted over the device and 35 the sample spread to the liquid-retaining zones by tilting or rocking the device. Alternatively, the assay surface of the device can be immersed in the

WO 98/45406

PCT/US97/14134

sample as described in Example 4. Upon removal of the assay surface from the liquid sample, liquid is retained in the hydrophilic liquid-retaining zones and is likewise substantially excluded from the hydrophobic 5 land area.

After the sample is distributed to the hydrophilic liquid-retaining zones of the assay device, various assays may be carried out depending on desired uses. For microbial detection or enumeration, the 10 assay device may be incubated for a time sufficient to permit at least one cell division cycle of the microorganism. For these purposes, the device is generally incubated at about 25°C to about 45°C, more preferably at about 30°C to about 37°C. The incubation 15 time for bacterial detection will vary. The detection time for most bacteria will range from about 20 minutes to about 24 hours in order to produce detectable growth as demonstrated by the indicator substance in the incubated liquid test sample. This relatively short 20 incubation time represents a distinct advantage over detection methods currently used, which typically require incubation times of about 24 hours or more.

Following incubation of the assay device, the presence or absence of the microorganism in the liquid- 25 retaining zones (and thus in the liquid test sample) is detected. The mode of detection depends on the type of indicator substance used in the method. Any indicator substance that is capable of providing a detectable signal may be used. Such indicators include but are 30 not limited to fluorescent, chromogenic, luminescent, and electrochemical indicators. The presence or absence of a microorganism in a zone can be visually detected, with the naked eye or microscopically, if a chromogenic or luminescent indicator is used. If a 35 fluorescent indicator substance is used, equipment and methods for detecting a fluorescent signal may be employed for detection. There are numerous indicator

WO 98/45406

PCT/US97/14134

substances and signal detection systems, including systems for detecting electrochemical changes, known in the art for detecting microorganisms, and any such substance or system may be used in accordance with the 5 present invention.

The detection of microorganisms in the liquid sample may further involve the enumeration of a microorganism count in the liquid test sample. In a preferred embodiment, the enumeration is performed 10 using MPN. Once the number of liquid-retaining zones containing the microorganism of interest is determined, an MPN calculation can be made using known MPN techniques. If desired, the number of microorganisms in an individual zone can then be determined using 15 known techniques, for example, signal intensity compared to a known standard, or by plating the contents of the zone. Advantageously, the large number of liquid-retaining zones used in the method of the invention allows for narrower intervals for the 95% 20 confidence limits in an MPN analysis of a liquid test sample.

Because of the large number of liquid-retaining zones that may be manufactured in a single device, it is possible to use a single device in the detection and 25 enumeration of multiple microorganisms of interest, while retaining the advantages of the invention. For example, a single liquid test sample can be tested for the presence or concentration of *E. coli* and *S. aureus*.

One portion of an assay device can contain hydrophilic 30 liquid-retaining zones for the detection and enumeration of one of these microorganisms, while a second set of zones can be directed to detection and enumeration of another microorganism of interest. This is accomplished, for example, by including 35 microorganism-specific nutrients and/or indicator substances in the respective sets of liquid-retaining zones. Alternatively, all liquid-retaining zones can

WO 98/45406

PCT/US97/14134

contain assay reagents designed for the simultaneous detection of multiple microorganisms. For example, *E. coli* can be detected with a fluorescent indicator substance while, at the same time, other coliforms are 5 detected with a chromogenic indicator substance.

In another embodiment, the distribution step can involve distributing aliquots of the liquid test sample to a plurality of hydrophilic liquid-retaining zones of an assay device, wherein the assay device includes a 10 plurality of sets of zones. Each set has zones of uniform size, and the device has at least two sets of zones. For example, the assay device can include a plurality of lanes, with the hydrophilic liquid-retaining zones in a particular lane having the same 15 liquid-retention capacities. This feature allows for the distribution of the liquid test sample into different test volume sizes within a single assay device. In MPN, this feature provides a significant advantage in that, for a highly concentrated sample, an 20 appropriate volume size may be selected and MPN analysis performed using a single distribution step in a single device without the need for serial dilutions.

As stated above, the methods of this invention may be practiced using any assay device containing 25 hydrophilic liquid-retaining zones and a hydrophobic land area, depending on the particular embodiment being practiced. The present inventors have developed several novel devices suitable for use in the methods of this invention. The following are non-limiting 30 examples of such devices.

Referring to Figure 1, a device 10 comprises a substrate 12 having a plurality of hydrophilic liquid-retaining zones in the form of hydrophilic microvolume wells 14. The substrate 12 can be fabricated from any 35 material in which microvolume wells can be fashioned and in which the microvolume wells retain their respective shapes throughout the useful life span of

WO 98/45406

PCT/US97/14134

the device 10. Substrate 12 can be fabricated, for example, from polymeric films or other appropriate materials. Appropriate polymers include without limitation polyethylene, polypropylene, polyimides, 5 fluoropolymers, polycarbonates, polyurethanes, and polystyrenes. Should a particular polymer not be sufficiently hydrophilic, it can be treated to impart hydrophilicity. For example, a surfactant can be included in the film to impart hydrophilicity. Those 10 skilled in the art will recognize other means to impart surface hydrophilicity. Microvolume wells 14 can be formed by any process appropriate to the substrate 12 material. Such processes include without limitation thermal embossing, cast embossing, laser drilling, 15 etching with reactive materials, or lamination of a sheet of patterned material containing a plurality of small openings onto a support film. Polyethylene or polypropylene films can be, for example, pressed embossed or extrusion embossed, and can include various 20 pigments and surfactants.

Referring again to Figure 1, the area 13 between microvolume wells 14 ("land area") is fabricated to be hydrophobic. This serves to prevent aqueous liquid from bridging between the microvolume wells 14, thereby 25 preventing cross-contamination. The land area 13 can be rendered hydrophobic in various ways. For example, the land area on an extrusion embossed polyethylene film, that had been rendered hydrophilic by incorporation of a surfactant, can be rendered 30 hydrophobic by transferring a thin layer of acrylated silicone or other hydrophobic material to the land area.

The device 10 can include any desired number of microvolume wells. Additionally, the device 10 can 35 include relatively large reservoirs or other compartments adapted to hold larger volumes of liquid for maintenance of an appropriate humidity level within

WO 98/45406

PCT/US97/14134

the device. Although the number of microvolume wells can be relatively small (e.g., 2-50) for certain applications such as preliminary screening, the small sizes of the microvolume wells allow relatively large numbers of wells to be fabricated on a single device 10. Preferably, the device has about 10 to about 10,000 liquid-retaining zones, even more preferably about 200 to about 5,000 zones, and most preferably about 400 to about 600 zones. The device 10 can have a population of uniformly sized microvolume wells 14, although the wells need not be of uniform size. For example, a device 16 as depicted in Figure 2 can have sets (e.g., rows) of microvolume wells in which volumes are constant within a set, but vary between sets. As depicted in Figure 2, the volumes can vary incrementally over an array of sets of wells, with the smaller wells 18 holding sub-microliter volumes and the larger wells 20 holding microliter volumes. It is even possible for the largest wells in a device such as depicted in Figure 2 to include wells 22 that would not be classified as "microvolume" wells. Such wells might have a liquid-retention capacity, for example, of substantially more than 25 microliters.

In an alternative embodiment, the substrate 12 can be coated with a hydrophobic nanostructured film. For example, polyimide or fluoropolymer webs can be vapor coated with organic pigments, lead, gold and other materials to create specific nanostructured films, then made hydrophobic by coating with an organized molecular assembly, such as octadecyl mercaptan or a fluorocarbon-hydrocarbon thiol, as described in Patent Application WO 96/34697. Relatively hydrophilic microvolume wells and other liquid-retaining zones may be fashioned by removing the hydrophobic nanostructured elements from selected areas of the substrate 12. This can be accomplished in various ways, including without limitation

WO 98/45406

PCT/US97/14134

encapsulation/delamination and laser ablation as described in Example 3, below.

A representative hydrophobic nanostructured film device 24 is depicted schematically in Figure 3. Such 5 devices can be loaded with sample simply by dipping in an aqueous sample solution. To this end, the device 24 can include a handle 26. Handle 26 allows an operator to place the device 24 in a liquid sample to any desired depth up to and including total immersion of 10 the device 24 in the liquid sample, while avoiding contact of the operator's fingers with the sample. Upon removal of device 24 from the sample, liquid sample remains attached to the device only at the locations of the hydrophilic liquid-retaining zones 28. 15 Incubation and detection are then performed as described above.

Assay devices also can be manufactured with hydrophilic liquid-retaining zones constructed of hydrophilic absorbent materials arrayed on a 20 hydrophobic surface. For example, the zones can be constructed of absorbent papers having circular, oval, square, polygonal or other appropriate shapes. As illustrated in Figure 4, for example, discs of cotton linter binderless paper 30 can be laminated to a 25 silicone-coated film 32 to form hydrophilic liquid-retaining areas 34 that project from the plane of the surrounding hydrophobic surface 36. Alternatively, the hydrophilic liquid-retaining zones may be constructed of nonwoven fiber loop material that likewise protrudes 30 (projects) from the plane of the surrounding hydrophobic land area. For example, as illustrated in Figures 5a and 5b, the assay device 38 may comprise a sheet of hydrophobic polypropylene film 40 containing arrays of protrusions 42 fabricated from surfactant-containing 35 polypropylene nonwoven fiber loop material.

Assay reagents can be coated or otherwise deposited within the liquid-retaining zones of the

WO 98/45406

PCT/US97/14134

assay devices. Such assay reagents can include without limitation nutrients for growth of microorganisms; gelling agents; indicator substances such as chromogenic indicators, fluorescent indicators, 5 luminescent indicators, and electrochemical indicators.

The assay reagents can be immobilized in the liquid-retaining zones by any of numerous methods for immobilizing assay reagents on solid substrates known to those of skill in the art. Such methods include for 10 example drying down assay reagent-containing liquids in the zones, as well as other methods for noncovalently attaching biomolecules and other assay reagents to a solid substrate. Alternatively, various methods may be employed to covalently attach assay reagents to the 15 substrate 12 material within the wells 14 by methods well known to those of skill in the art.

As discussed above, the presence of hydrophilic liquid-retaining zones with microvolume liquid-retention capacity in an assay device allows for 20 separation of a liquid test sample into a relatively large number of test volumes. The ability to separate a liquid sample into microvolume aliquots and to perform MPN or other assays without cross-contamination between aliquots is an advantage of the present method 25 and devices.

All references and publications cited herein are expressly incorporated herein by reference into this disclosure. Particular embodiments of this invention will be discussed in detail and reference has been made 30 to possible variations within the scope of this invention. There are a variety of alternative techniques and procedures available to those of skill in the art which would similarly permit one to successfully practice the intended invention.

35

#### EXAMPLES

The following examples are offered to aid in understanding of the present invention and are not to

60557-6162

be construed as limiting the scope thereof. Unless otherwise indicated, all parts and percentages are by weight.

5

**Example 1**

**Embossed Film Culture Devices**

Embossed film culture devices containing a plurality of microcompartments and capable of being used for the detection of microorganisms in a liquid 10 test sample were constructed as described in this example.

The hydrophilic liquid-retaining zones can be formed in a substrate by a number of processes, examples of which are thermal embossing, cast 15 embossing, laser drilling, and by etching the surface with a reactive material. Detailed descriptions of how to make recesses or microvolume wells in polymeric films are provided in U. S. Patents 5,192,548; 5,219,462; 5,344,681; and 5,437,754. The following 20 descriptions are representative of specific embossed film culture devices used in the subsequent examples.

**A. Pressed Embossed Films Containing a Plurality of Microvolume Wells**

Polyethylene (Eastman Chemical Company Resin 25 #18BOA) containing 10% by weight TiO<sub>2</sub> (50% TiO<sub>2</sub>/50% Polyethylene Pigment Concentrate) and 0.5% by weight Triton X-35 Surfactant (Sigma Chemical Company) or polypropylene was extrusion cast into a film (4-mil thickness). The film was cut into sheets and stacked 30 (~20 sheets) onto photolithographically etched magnesium alloy tooling as described in U.S. Patent 5,219,462, designed to form a plurality of microvolume wells. The etched magnesium tooling contained protuberances arranged in the patterns described in 35 subsequent examples. The stacked polyethylene sheets were embossed on a heated hydraulic press (132 °C, 1.4 N/m<sup>2</sup>, 120 second dwell) as described in U.S. Patent

WO 98/45406

PCT/US97/14134

5,219,462. The samples were allowed to cool, at which time the tooling was removed to provide a single layer film containing the "negative" image of the tooling.

5 B. Extrusion Embossed Films Containing a Plurality of Microvolume Wells

Photolithographically etched magnesium master tooling was attached to a steel roll using pressure-sensitive transfer adhesive. The polyethylene, pigment, and surfactant composition described in Example 1A was 10 blended together and extrusion cast onto the roll as described in U.S. Patent 5,192,548. Embossed films lacking the Triton X-35 surfactant were also prepared in this manner.

15 C. Extrusion Embossed Films with Hydrophobic "Land" Area

Extrusion embossed polyethylene films containing Triton X-35 Surfactant were prepared according to Example 1B. The area between microvolume wells ("land" area) was rendered hydrophobic by transferring a thin 20 layer of acrylated silicone (Goldschmidt FC 711) containing 4.8% of a cross linking agent (Darocur 1173) with a roll-to-roll coating apparatus (Straub Design Co.). The hydrophobic coating was cured by exposing the film to ultraviolet radiation under nitrogen 25 atmosphere using a Fusion Systems UV lamp with an H bulb providing a dosage of 85 millijoules/cm<sup>2</sup>.

**Example 2**

**Method of Inoculation**

30 **(Method Utilizing Plurality of Microvolume Wells)**

A. Inoculation with Indicator Solution

An aqueous solution containing phenol red indicator (to provide contrast) was applied by pipette onto silicone-treated and silicone-untreated 35 polyethylene embossed films (Examples 1C and 1B, respectively) containing a plurality of microvolume wells (about

WO 98/45406

PCT/US97/14134

1.3  $\mu$ l/well). The microvolume wells were arranged in a hexagonal array (~19 wells/cm<sup>2</sup>) and each well was in the shape of an inverted truncated cone, having a diameter of approximately 1.9 mm at the surface and 1.0 mm at 5 its depth, which was about 1.1 mm. The microvolume wells were filled as described in U. S. Patent 5,219,462 by drawing the diluted sample solution down the film with the edge of a razor blade. The samples treated with the hydrophobic silicone coating were 10 shown to partition liquid into individual microvolume wells without fluid bridging between the wells, whereas bridging of liquid was observed on the untreated films.

B. Inoculation with Microorganism-Containing Samples

15 The method of inoculating embossed film culture devices containing a plurality of microvolume wells with bacteria-containing media was demonstrated in this example. The inoculated devices were utilized to detect and enumerate *E. coli* bacteria.

20 An overnight broth culture of *E. coli* ATCC 51813 (~10<sup>9</sup> CFU/ml in Tryptic Soy Broth (TSB) media) was serially diluted into Violet Red Bile (VRB) media (7.0 g/l Bacto peptone, 3.0 g/l yeast extract, and 1.5 g/l bile salts) containing 4-methylumbelliferyl- $\beta$ -D- 25 glucuronide (0.5 mg/ml) (MUG, Biosynth International, Naperville, IL). The dilution was prepared to the approximate bacterial concentration of 100 CFU/ml. The diluted sample (0.5 ml) was applied by pipette onto silicone-treated and silicone-untreated polyethylene 30 embossed films (406 microvolume wells) as described in Example 2A. The inoculated embossed films 43 were placed inside petri dishes, and incubated for 12 hours at 37°C. Twenty-eight microvolume wells 44 exhibited sharp, discrete fluorescent spots on the silicone- 35 treated film 46 (Figure 6b). In contrast, significant well-to-well cross-contamination was observed on the untreated film (Figure 6a). For the silicone-treated

WO 98/45406

PCT/US97/14134

film, 28 positive wells corresponds to a most probable number (MPN) of 58 CFU/ml, as calculated using the formula  $MPN = N \ln (N/N-X)$  where N is the total number of filled wells and X is the total number of wells showing a positive reaction.

The results of this example show that microorganisms can be readily detected and enumerated using an embossed film culture device having a plurality of microvolume wells and that well-to-well cross-contamination can be eliminated by coating a hydrophobic substance on the land area between wells.

### Example 3

#### Nanostructured Film Culture Devices

15 Nanostructured film culture devices containing a plurality of hydrophilic microvolume liquid-retaining zones arrayed on a substrate coated with a hydrophobic nanostructured film were constructed as described in this example.

20 A. Nanostructured Film

Processes for generating nanostructured surfaces are disclosed in U. S. Patents 4,812,352 and 5,039,561. Briefly, the organic pigment C.I. Pigment Red 149 (American Hoechst-Celanese, Somerset, NJ) was vacuum vapor deposited to a thickness of 250 nm onto a 0.0125-nm thick, 30 x 30 cm sheet of polyimide web, which had previously been metal vapor coated with 700 Å of platinum. The sample was annealed in a vacuum oven at 264 °C for greater than 30 minutes, which was sufficient to convert the PR 149 pigment to a dense distribution of discrete crystalline whiskers oriented perpendicular to the web substrate. The whiskers were vapor coated with a mass equivalent thickness of 2500 Å of gold, which resulted in a conformational coating of gold particles, ~2 µm tall and ~0.15 µm in diameter, with an areal number density of 5 per (µm)<sup>2</sup>, as determined by SEM.

WO 98/45406

PCT/US97/14134

Alternatively, the polyimide was replaced with a transparent fluorenone polyester (FPE, 3M Co.) and vapor coated with 50 Å of gold, which prevented surface charging during deposition of the PR 149, yet remained 5 essentially transparent.

B. Hydrophobic Nanostructured Film

The nanostructured film was then made hydrophobic by immersing in a 0.1mM solution of  $C_8F_{17}(CH_2)_{11}SH$  in ethanol for 4 hours, followed by rinsing with pure 10 ethanol and air drying. The resulting highly hydrophobic surface was measured to have identical advancing and receding contact angles of 178 ° for water. This process is described in Patent Application WO 96/34697.

15 C. Nanostructured Film Culture Devices

Nanostructured film culture devices were constructed by using an encapsulation/delamination of nanostructured films process described in U. S. Patent 5,336,558. Briefly, pieces of the nanostructured 20 hydrophobic film were cut into 1.5 x 2.0 cm strips. A 0.25-mm thick perforated steel sheet, having a square array of 1.5-mm diameter holes spaced ~4 mm apart, was laid over the nanostructured side of the strips. A fast curing vinyl polysiloxane encapsulate (3M EXPRESS 25 dental impression material, 3M Co.) was applied liberally over the steel plate to cause the material to penetrate through the holes and encapsulate the nanostructured whiskers. After several minutes, the impression material was set and the steel sheet was 30 removed, thereby removing the nanostructured elements cleanly from the polyimide web only at the location of the array of holes. The exposed metal-coated polyimide substrate in the areas under the holes was relatively hydrophilic compared to the remainder of the surface. 35 This was demonstrated by dipping the strips into an aqueous solution and observing that small droplets remained attached only at the array of exposed spot or

WO 98/45406

PCT/US97/14134

zone areas.

Alternatively and preferably, laser ablation was utilized for removing the nanostructured elements from the polyimide web to provide the desired array of 5 relatively hydrophilic liquid-retaining zones. The strips of nanostructured hydrophobic film were ablated with a Nd-YAG laser with a collimated beam 1 mm in diameter and operated in a Q-switched mode with approximately 2 mJoule, 60 nanosecond pulses. Single 10 pulses were used to ablate rows of 1-mm diameter zones on 4- and 5-mm center-to-center spacing. Larger zones, ~1.6 x 1.6 mm square, were produced by overlapping a 3 x 3 matrix of nine 1-mm diameter zones. The resulting nanostructured film culture device with 40 (4 x 10) 15 zones was submersed in water for 1 minute initially to make the ablated zone areas hydrophilic. Upon withdrawing the plate, each of the 40 zones had an ~1-mm diameter, hemispherical droplet attached to it.

20

#### Example 4

##### Method of Inoculation

##### (Method Utilizing

##### Nanostructured Film Culture Devices)

###### A. Inoculation with Aqueous Liquid Sample

25 To inoculate and measure the amount of liquid selectively retrieved by the nanostructured film culture devices (Example 3C), a plate with 12 hydrophilic liquid-retaining zones, ranging in size from 1 to 2.5 mm in diameter (average 2 mm), was dipped 30 into pure water and the amount of water extracted onto the zones was measured gravimetrically. The plate was first dipped at a slow withdrawal rate of ~3 seconds/cm. After withdrawal, the back of the plate was touched against tissue paper to remove any water 35 droplets clinging to the back of the polyimide plate, and the plate was then placed on a mass balance (0.1 mg minimum sensitivity) and the mass recorded 15 seconds

WO 98/45406

PCT/US97/14134

later. This was repeated 15 times. The mean and standard deviation of the mass of the 12 water zones was  $3.7 \pm 0.2$  mg, giving an average zone volume of  $0.310 \mu\text{l} \pm 5\%$ . The procedure was then repeated a fast 5 withdrawal rate with the plate pulled from the water in a time estimated to be  $\sim 0.1$  second. At this rate, the amount of liquid that remained on the hydrophilic zones was larger, because the liquid did not have time to "stretch" and dynamically equilibrate. The mean and 10 standard deviation of the 15 trials was  $6.0 \pm 0.5$  mg, giving an average zone volume of  $0.500 \mu\text{l} \pm 12\%$ .

B. Inoculation with *S. Aureus*-Containing Samples

The method of inoculating nanostructured film culture devices containing a plurality of microvolume 15 liquid-retaining zones with bacteria-containing media was demonstrated in this example. The inoculated devices were utilized to detect and enumerate *S. aureus* (Example 4B) and *E. coli* (Example 4C) bacteria.

A mixture (5  $\mu\text{l}$ ) of molten ( $\sim 60$  °C) 20 bacteriological growth media BHI (Brain Heart Infusion, Becton Dickinson and Co.) and agar (1.2% weight/volume) was spotted onto the hydrophilic zones of the nanostructured film culture devices prepared as described in Example 3C. The agar "spots" were allowed 25 to cool and solidify at room temperature. One plate was dipped briefly into a growing culture of *Staphylococcus aureus* ( $\sim 10^8$  cells/ml) in BHI broth medium. Other plates were dipped similarly into 1:10 and 1:1000 dilutions of the *S. aureus* culture, representing  $10^7$  and  $10^5$  30 cells/ml, respectively. The plates were placed into plastic petri dishes containing water-saturated filter paper to maintain humidity, and incubated at 37°C for 4 hours. The plates were then dipped into a solution containing 900  $\mu\text{l}$  of HEPES Buffer (Sigma Chemical Co., 35 pH 8.0); 120  $\mu\text{l}$  of fluorescent indicator solution (1.0 mg/ml Boc-Val-Pro-Arg-AMC HCl (NovaBiochem, San Diego, CA) in 72 mM triethanolamine, 144 mM NaCl, pH

WO 98/45406

PCT/US97/14134

8.4); and, 30  $\mu$ l human prothrombin (Sigma Chemical Co., 50 mg/ml in 5mM Tris buffer, 50mM NaCl, pH 8.0). The plates were incubated for one additional hour under the same conditions described above and then examined under 5 UV light (~366 nm, Mineralite, UVP, Inc., San Gabriel, CA). The zones containing agar media, bacterial suspension, and indicator solution all showed visible, intense bluish fluorescence as compared to no visible fluorescence in the control samples, which were 10 prepared without any added bacteria. No cross-contamination between zones was observed.

C. Inoculation with *E. coli*-Containing Samples

Agar medium was prepared by combining the following ingredients: pancreatic digest of gelatin 15 (10 g, Peptone G, Acumedia Manufacturers, Inc., Baltimore, MD); Bacto Bile Salts Number 3 (2.5 g, Difco Labs, Detroit, MI); Agar (6 g, Difco Labs); and deionized water (500 ml). The mixture was stirred and heated to 100 °C until the agar melted, autoclaved at 20 121 °C for 15 minutes to sterilize, and then cooled to room temperature to solidify. An IPTG stock solution was prepared from filter-sterilized (0.2 mm) isopropyl- $\beta$ -D-galactoside (IPTG, CalBiochem Corp., La Jolla, CA) in deionized water (200 mg/ml) and stored at -20 °C 25 until use. A MU-Gal stock solution was prepared from 4-methylumbelliferyl- $\beta$ -D-galactoside (MU-Gal) in N,N-dimethylformamide (10 mg/ml) and stored at 4 °C until use. Immediately before use the agar medium was melted at 100 °C and 25 ml was transferred to a sterile 50-ml 30 tube. The IPTG stock solution (12.5 ml) and the MU-Gal stock solution (150 ml) were then mixed into the cooled (~60 °C) agar suspension. The mixture was immediately transferred (4- $\mu$ l aliquots) to the nanostructured film culture device zones as described in Example 4B. After 35 cooling to room temperature, the plates were dipped into a mid-exponential growing culture of *E. coli* ATCC 51813 (~10<sup>8</sup> cells/ml in LB medium 3) and incubated in

WO 98/45406

PCT/US97/14134

individual humidified petri dishes at 37°C. After 4 hours of incubation, the plates were checked for fluorescence with a Mineralite UV lamp. The inoculated zones exhibited slightly more fluorescence than that 5 observed in the uninoculated zones. The plates were then incubated for an additional 16 hours and rechecked. The inoculated zones showed significantly more blue fluorescence than the uninoculated zones. The 10 plate prepared with clear-film substrate (Example 3A utilizing FPE) was particularly convenient to measure because it could be illuminated from one side and viewed or photographed from the other side. No cross-contamination between zones was observed.

15

### Example 5

#### Absorbent Disc Culture Devices

Absorbent disc culture devices containing a plurality of hydrophilic absorbent discs arrayed on a 20 hydrophobic surface and capable of being used for the detection and enumeration of microorganisms in a liquid test sample were constructed as described in this example.

A sheet of absorbent material (Scheicher & Schuell 25 Grade 903 Paper; absorbs about 4.5 g of water/100 cm<sup>2</sup>) was laminated to a Rexam silicone-coated film (Grade #15819 D 2MIL CL PET MM34P/000 having a clear 2-mil thick polyester film as a substrate, Rexam Release, Oak Brook, IL) with an acrylate pressure sensitive 30 adhesive (PSA) containing the chromogenic indicator 2,3,5-triphenyl-2H-tetrazolium chloride (TTC) (Amresco, Solon, OH). The material was saturated with TSB growth nutrient containing 0.5% of the fluorescent indicators 4-methylumbelliferyl phosphate (100 µg/ml, Sigma, St. 35 Louis, MO) and 4-methylumbellifery- $\alpha$ -D-glucoside (50 µg/ml, Sigma), wiped with a wire-wound rod, and dried at 110°C for 10 minutes. Circular discs approximately

WO 98/45406

PCT/US97/14134

0.635 cm in diameter were punched out of the laminate and the silicone-coated film backing removed. The discs with PSA were then adhered to another sheet of Rexam silicone-coated film so that the discs were patterned 5 in equally spaced parallel rows. The film and discs assemblies were gamma irradiated to a level of 8.9 kGy, cut to size, and then taped into a petri dish such that each dish contained a piece of film with 20 discs. Based on gravimetric measurements, each disc in the 10 resulting culture devices had a capacity to retain about 40  $\mu$ l of liquid.

#### Example 6

##### Method of Inoculation

###### 15 (Method Utilizing Absorbent Disc Culture Devices)

The method of inoculating absorbent disc culture devices containing a plurality of microvolume liquid-retaining zones (absorbent discs) with bacteria-containing media was demonstrated in this example. The 20 inoculated devices were utilized to detect and enumerate *E. coli* bacteria.

A culture of *E. coli* ATCC 51813 was diluted to produce suspensions containing about 10 CFU/ml and 1 CFU/ml. Samples (1 to 2 ml) of the suspensions were 25 applied by pipette to the absorbent disc culture devices described in Example 5. Excess liquid sample was poured off, thereby leaving about 0.8 ml retained on the device (20 discs, about 40  $\mu$ l of liquid per disc). The inoculated devices were incubated at 35°C 30 for 23 hours and inspected under ultraviolet light. The number of discs exhibiting fluorescence was counted for each device and most probable number (MPN) values calculated using the formula described in Example 2B. The MPN per milliliter was calculated by dividing the 35 value obtained by the total volume of the sample (0.8 ml). Results are provided in Table 6a and are compared with counts obtained from standard testing with

WO 98/45406

PCT/US97/14134

Coliform Count PETRIFILM™ Plates (3M Co.). The fluorescent discs often showed the red TTC color, usually as discrete spots within the discs. No cross-contamination between absorbent discs was observed.

5

Table 6a Enumeration of Microorganisms ( <i>E. coli</i> )			
Bacterial Suspension (~ CFU/ml)	Positive Discs (Out of 20)	MPN (CFU/ml)	Coliform Count PETRIFILM™
10	17	47	22
10	19	74	24
1	2	2.6	5
1	3	4.1	4

The results of this example show that absorbent disc culture devices having a plurality of absorbent discs arrayed on a hydrophobic film can be easily 10 inoculated with bacteria-containing liquid samples and that the inoculated devices can be utilized for the detection and enumeration of *E. coli*, with the values obtained being comparable with those obtained from commercial Coliform Count PETRIFILM™ Plates.

15

#### Example 7

##### Method of Inoculation

##### (Method Utilizing Hydrophilic Fiber Culture Devices)

The method of constructing and inoculating 20 hydrophilic fiber culture devices containing a plurality of microvolume liquid-retaining zones (nonwoven fiber loops) with indicator solution and with bacteria-containing media were demonstrated in this example. The inoculated devices were utilized to detect 25 and enumerate *E. coli* bacteria.

##### A. Device Construction

A sheet of hydrophobic polypropylene film containing an array of relatively hydrophilic surfactant-containing polypropylene nonwoven fiber loop 30 protrusions was prepared as described in U. S. Patent

WO 98/45406

PCT/US97/14134

5,256,231. The sheet was cut to size and taped to the bottom of a petri dish to form a culture device. Each device contained film having about 200 fiber loop protrusions patterned hexagonally in equally spaced 5 parallel rows. Each hemispherical protrusion was hexagonal at its base (side length about 3 mm, height about 2 mm) and had a capacity to retain about 15  $\mu$ l of liquid.

B. Inoculation with Indicator Solution

10 A sample (1 ml) of phosphate buffer ("Butterfield", Fisher Scientific) containing phenol red indicator (to provide contrast) was applied by pipette onto the film in the center of the device. The liquid was observed to wick into the hydrophilic fiber 15 loop protrusions radially from the point of inoculation. The liquid was observed to quickly partition into the loop protrusions while "draining" from the hydrophobic polypropylene land areas. About 65 of the 200 protrusions were filled. No bridging of the 20 colored liquid across the land areas between loop protrusions was observed.

C. Inoculation with Microorganism-Containing Sample

An overnight culture of *E. coli* (ATCC 51813,  $\sim 10^9$  25 CFU/ml in TSB media) was serially diluted into VRB Media (7.0 g/l Bacto peptone, 3.0 g/l yeast extract, 1.5 g/l bile salts) containing 4-methylumbelliflferone- $\beta$ -D-glucuronide (0.5 mg/ml). A dilution of  $10^{-8}$  was prepared corresponding to a bacterial concentration of 30 about 10 CFU/ml. A sample (1 ml) was pipetted onto the film in the center of a hydrophilic fiber culture device (Example 7A) as described in Example 7B. After inoculation, the petri dish was covered and sealed using electrical tape to prevent evaporation. The 35 device was then inverted and incubated at 37°C for 19 hours. After incubation, the number of protrusions

WO 98/45406

PCT/US97/14134

exhibiting fluorescence under 365 nm irradiation were counted. Five separate, discrete protrusions were observed to have significant fluorescence. No fluorescence was observed between protrusions, thereby 5 indicating no cross-contamination. The MPN value was calculated to be 5 CFU/ml, using the formula described in Example 2B.

The results of this example show that hydrophilic fiber culture devices having a plurality of hydrophilic 10 fiber zones arrayed on a hydrophobic film can be easily inoculated with bacteria-containing liquid samples and that the inoculated devices can be utilized for the detection and enumeration of *E. coli*.

Various modifications and alterations of this 15 invention will be apparent to those skilled in the art without departing from the scope and spirit of this invention, and it should be understood that this invention is not limited to the illustrative embodiments set forth herein.

60557-6162

CLAIMS:

1. A culture device for detection or enumeration of microorganisms, said device comprising a substrate comprising liquid-retaining discs comprising a hydrophilic material, wherein said substrate comprises a material that is hydrophobic relative to said liquid-retaining discs and wherein the discs comprise dry media for growth of microorganisms.
2. The culture device of claim 1 wherein said discs are constructed at least in part of a material selected from the group consisting of cellulosics, polyolefins, polyamides and polyesters.
3. The culture device of claim 2 wherein the discs are constructed at least in part of alpha cellulose.
4. The culture device of claim 2 wherein the discs are constructed at least in part of rayon.
5. The culture device of claim 2 wherein the discs are constructed at least in part nylon.
6. The culture device of claim 2 wherein the discs are constructed at least in part of polylactic acid.
7. The culture device of claim 1 wherein said device has about 10 to about 10,000 discs.
8. The culture device of claim 1, wherein said device has about 400 to about 600 discs.
9. The culture device of claim 1, wherein each said disc has a liquid retention capacity of about 1 to about 2 microliters.

60557-6162

10. The culture device of claim 1, having an indicator substance on said discs.

11. The culture device of claim 1 wherein the discs are adhered to the substrate with adhesive, and wherein said 5 adhesive has an indicator for detecting microorganisms.

12. The culture device of claim 10, wherein said indicator substance is selected from the group consisting of a chromogenic indicator, a fluorescent indicator, a luminescent indicator and an electrochemical indicator.

10 13. The culture device of claim 1, wherein said culture device comprises a plurality of at least two sets of liquid-retaining discs, each set comprising discs of uniform size, said sets varying in liquid retention capacity.

14. A method for partitioning an aqueous liquid sample 15 into discrete microvolumes, comprising:

a) providing a device for culturing a microorganism, said device comprising an assay surface, said surface comprising liquid-retaining discs comprising a hydrophilic material and a land area comprising a hydrophobic material between said 20 discs, each said disc comprising dry media for growing microorganisms; and

b) contacting said liquid sample with said assay surface such that said liquid sample is partitioned into said liquid-retaining discs.

25 15. The method of claim 14, wherein the discs are constructed of a material selected from the group consisting of cellulosics, polyolefins, polyamides and polyesters.

60557-6162

16. The method of claim 15, wherein the discs are coated with a growth medium.

17. The method of claim 14, wherein said discs have at least one indicator substance coated thereon.

5 18. The method of claim 17, wherein said indicator substance is selected from the group consisting of a chromogenic indicator, a fluorescent indicator, a luminescent indicator and an electrochemical indicator.

10 19. The method of claim 14, wherein said discs are of uniform size and each said disc has a liquid retention capacity of about 0.01 to about 25 microliters.

20. The method of claim 14 wherein each said disc has a liquid retention capacity of about 1 to about 2 microliters.

15 21. The culture device of claim 1 wherein at least one of the discs has a microvolume capacity of liquid retention.

22. The method of claim 14 wherein at least one of the discs has a microvolume capacity of liquid retention.

20 23. A method for partitioning an aqueous liquid sample into discrete microvolumes, comprising:

25 a) providing a device for culturing a microorganism, the device comprising an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising a hydrophobic material between the zones, each zone comprising dry media for growing microorganisms; and

60557-6162

b) contacting the liquid sample with the assay surface such that the liquid sample is partitioned into the liquid-retaining zones.

24. The method of claim 23 wherein at least one of the 5 liquid-retaining zones has a microvolume capacity of liquid retention.

25. The method of claim 23 wherein the zones comprise a coating or deposition of assay reagent.

26. The method of claim 25 wherein the assay reagent 10 comprises nutrient medium.

27. The method of claim 25 wherein the assay reagent comprises at least one indicator substance.

28. The method of claim 27 wherein the indicator substance is a chromogenic indicator, a fluorescent 15 indicator, a luminescent indicator or an electrochemical indicator.

29. The method of claim 23 wherein the zones are of uniform size and each zone has a liquid retention capacity of about 0.01 to about 25 microliters.

20 30. The method of claim 29 wherein each zone has a liquid retention capacity of about 1 to about 2 microliters.

31. The method of claim 23 wherein the culture device comprises about 10 to about 10,000 liquid-retaining zones.

25 32. The method of claim 31 wherein the culture device comprises about 400 to about 600 liquid-retaining zones.

33. The method of claim 23 wherein the liquid-retaining zones comprise microvolume wells.

60557-6162

34. The method of claim 23 wherein the land area comprises a treated nanostructured film.

35. The method of claim 23 wherein the liquid-retaining zones comprise hydrophilic fiber material 5 projecting from the hydrophobic material.

36. The method of claim 35 wherein at least one of the zones comprises a hydrophilic absorbent disc.

37. The method of claim 35 wherein at least one of the zones comprises protruding hydrophilic nonwoven fiber loop 10 material.

38. The method of claim 23 wherein the culture device comprises a plurality of at least two sets of liquid-retaining zones, each set having zones of uniform size, the sets varying in liquid retention capacity.

15 39. A culture device for detection or enumeration of microorganisms, the device comprising an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising a hydrophobic material between the zones, each zone comprising 20 dry media for growing microorganisms; and at least one of the zones comprising an assay reagent.

40. The culture device of claim 39 wherein at least one of the liquid-retaining zones has a microvolume capacity of liquid retention.

25 41. The culture device of claim 39 wherein the device comprises about 10 to about 10,000 zones.

42. The culture device of claim 41 wherein the device comprises about 400 to about 600 zones.

60557-6162

43. The culture device of claim 39 wherein each zone has a liquid retention capacity of about 0.01 to about 25 microliters.

44. The culture device of claim 43 wherein each zone 5 has a liquid retention capacity of about 1 to about 2 microliters.

45. The culture device of claim 39 wherein the assay reagent comprises a nutrient medium.

46. The culture device of claim 39 wherein the assay 10 reagent comprises an indicator substance.

47. The culture device of claim 46 wherein the indicator substance is a chromogenic indicator, a fluorescent indicator, a luminescent indicator or an electrochemical indicator.

15 48. The culture device of claim 39 wherein the liquid-retaining zones comprise microvolume wells.

49. The culture device of claim 39 wherein the land area comprises a treated nanostructured film.

50. The culture device of claim 39 wherein the liquid-20 retaining zones comprise hydrophilic fiber material projecting from the hydrophobic material.

51. The culture device of claim 50 wherein at least one zone comprises a hydrophilic absorbent disc.

52. The culture device of claim 50 wherein at least 25 one zone comprises protruding hydrophilic nonwoven fiber loop material.

60557-6162

53. The culture device of claim 39 wherein the culture device comprises a plurality of at least two sets of liquid-retaining zones, each set having zones of uniform size, the sets varying in liquid retention capacity.


5 54. A method for partitioning an aqueous liquid sample into discrete volumes to conduct a most probable number analysis, comprising:

- a) providing a device for culturing a microorganism, the device including an assay surface, the assay surface comprising liquid-retaining zones comprising a hydrophilic material and a land area comprising a hydrophobic material between the zones;
- b) contacting a liquid sample with the assay surface such that the liquid sample partitions into the liquid-retaining zones;
- c) incubating the device;
- d) detecting a signal that indicates microorganisms are growing in a zone; and
- e) conducting a most probable number analysis based on the number of zones wherein a signal is detected.


SMART &amp; BIGGAR

OTTAWA, CANADA





PATENT AGENTS

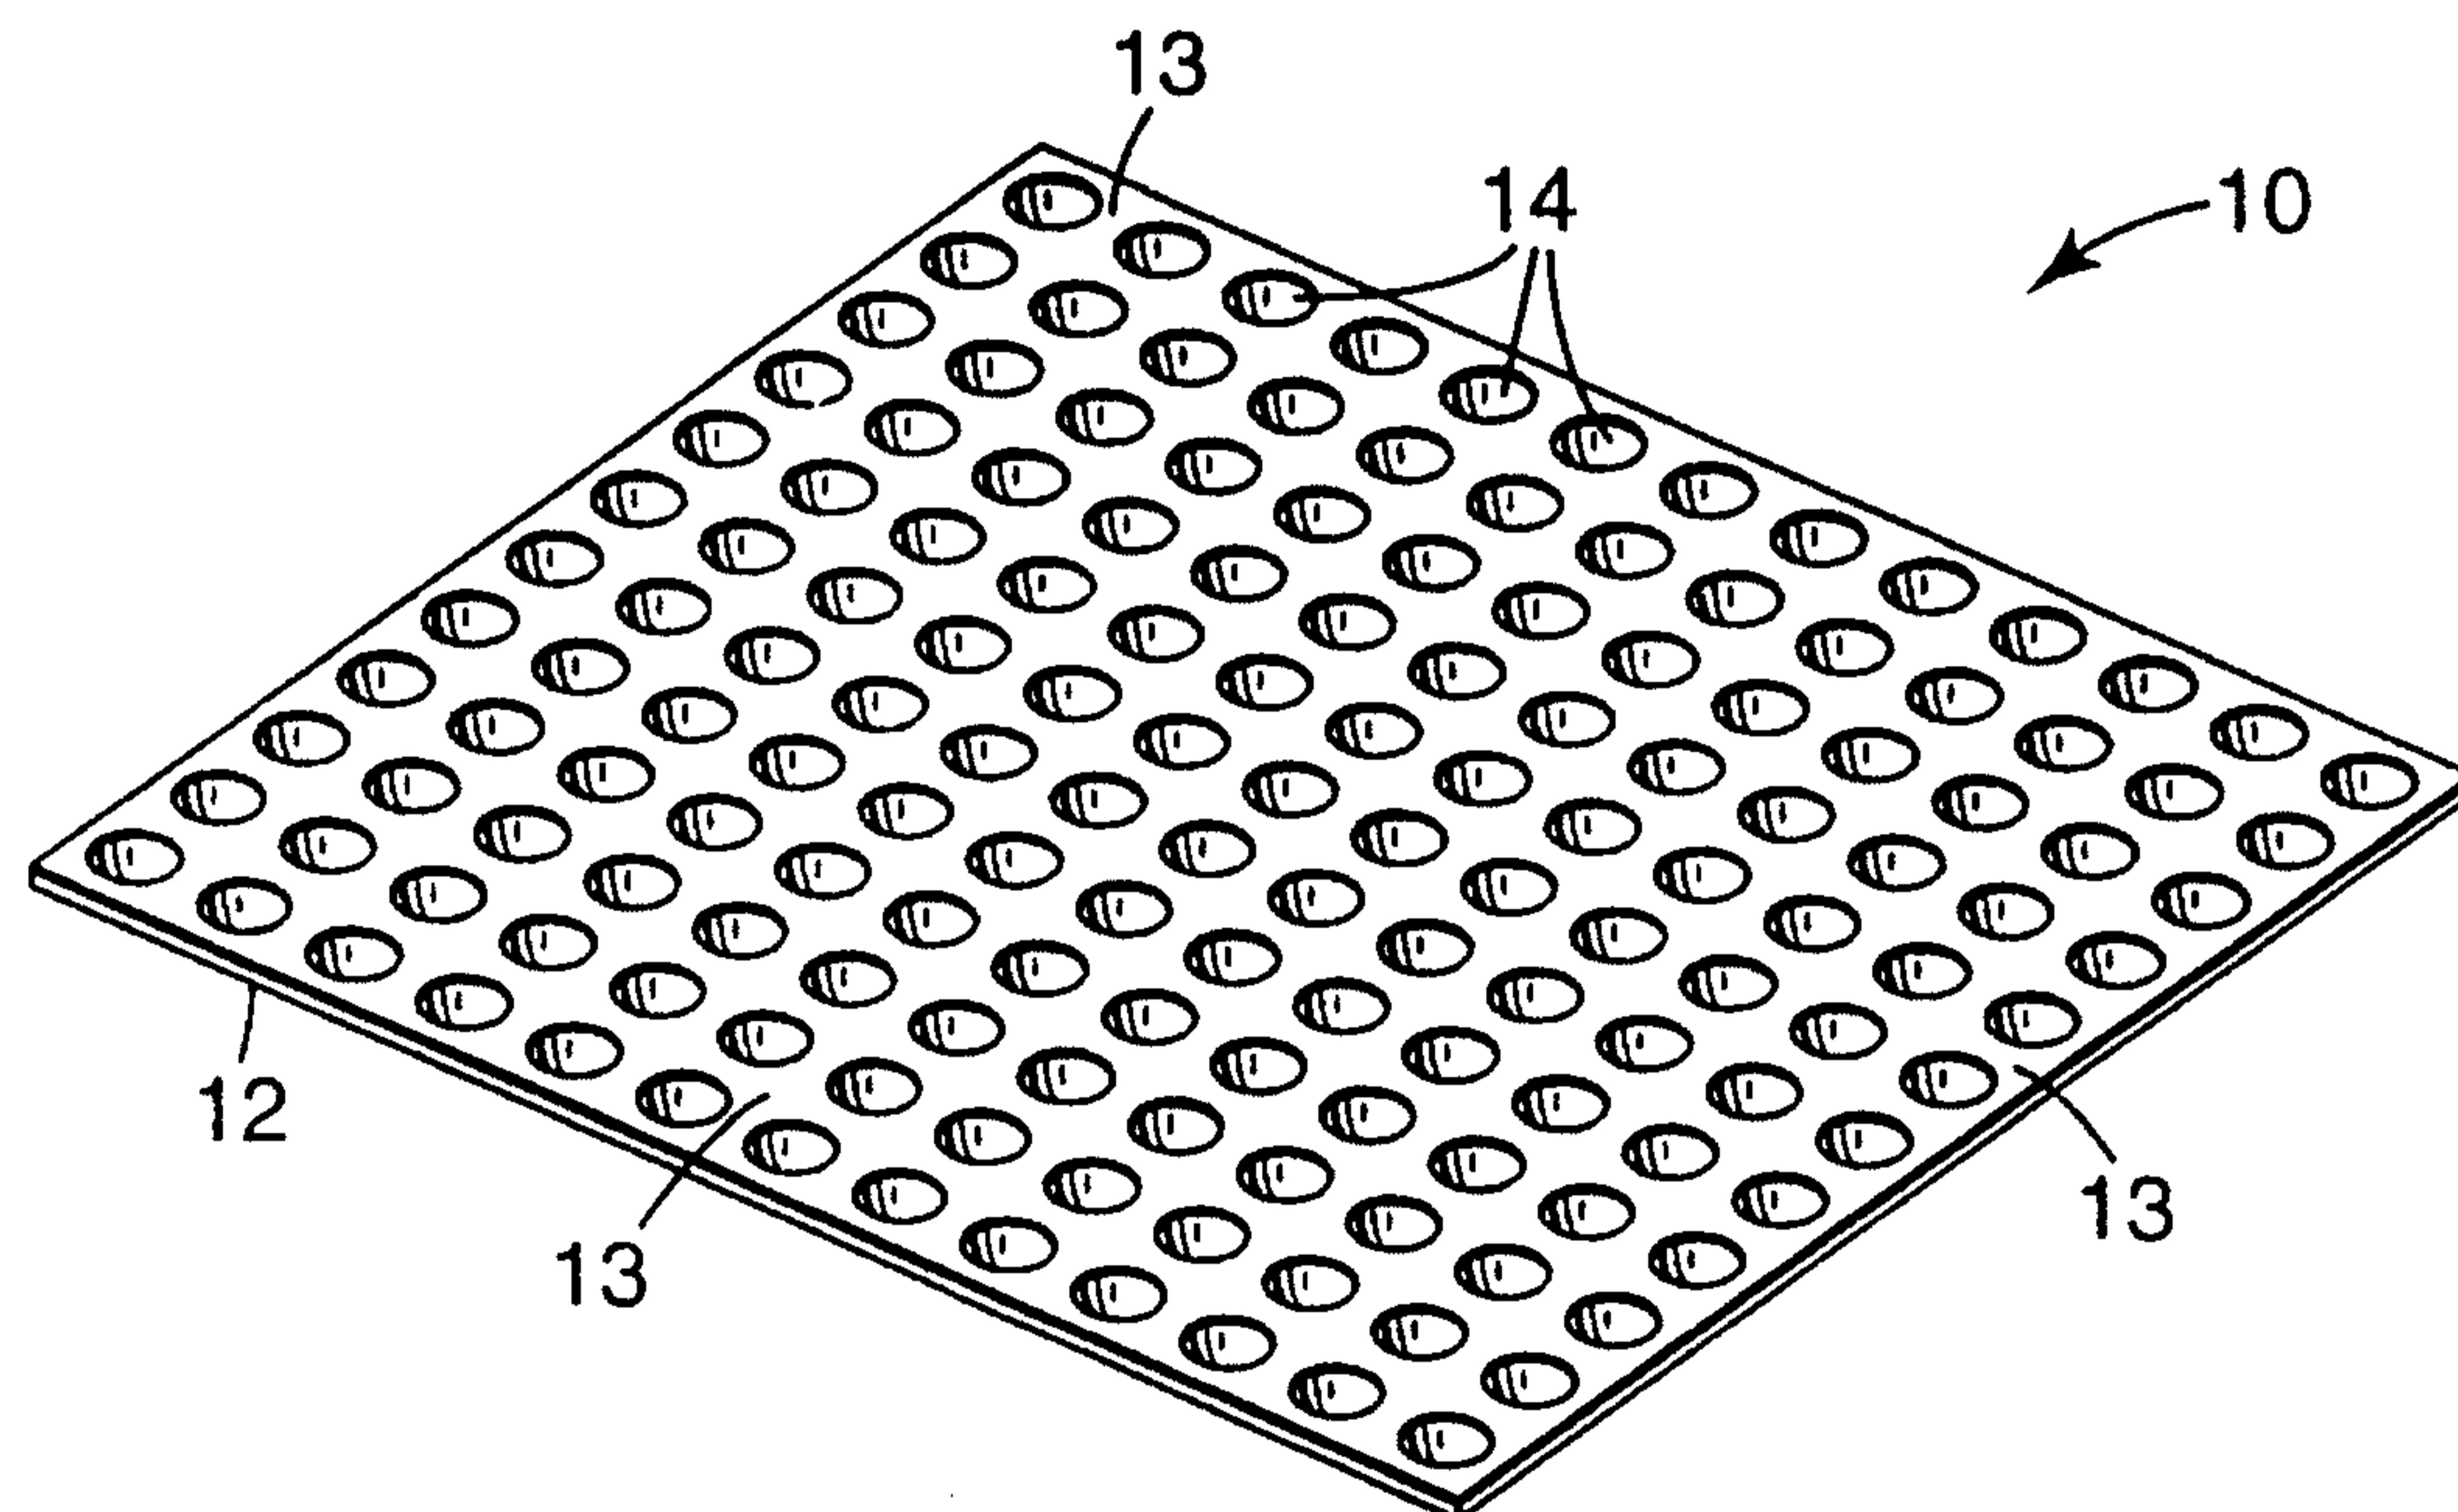

*Fig. 1*

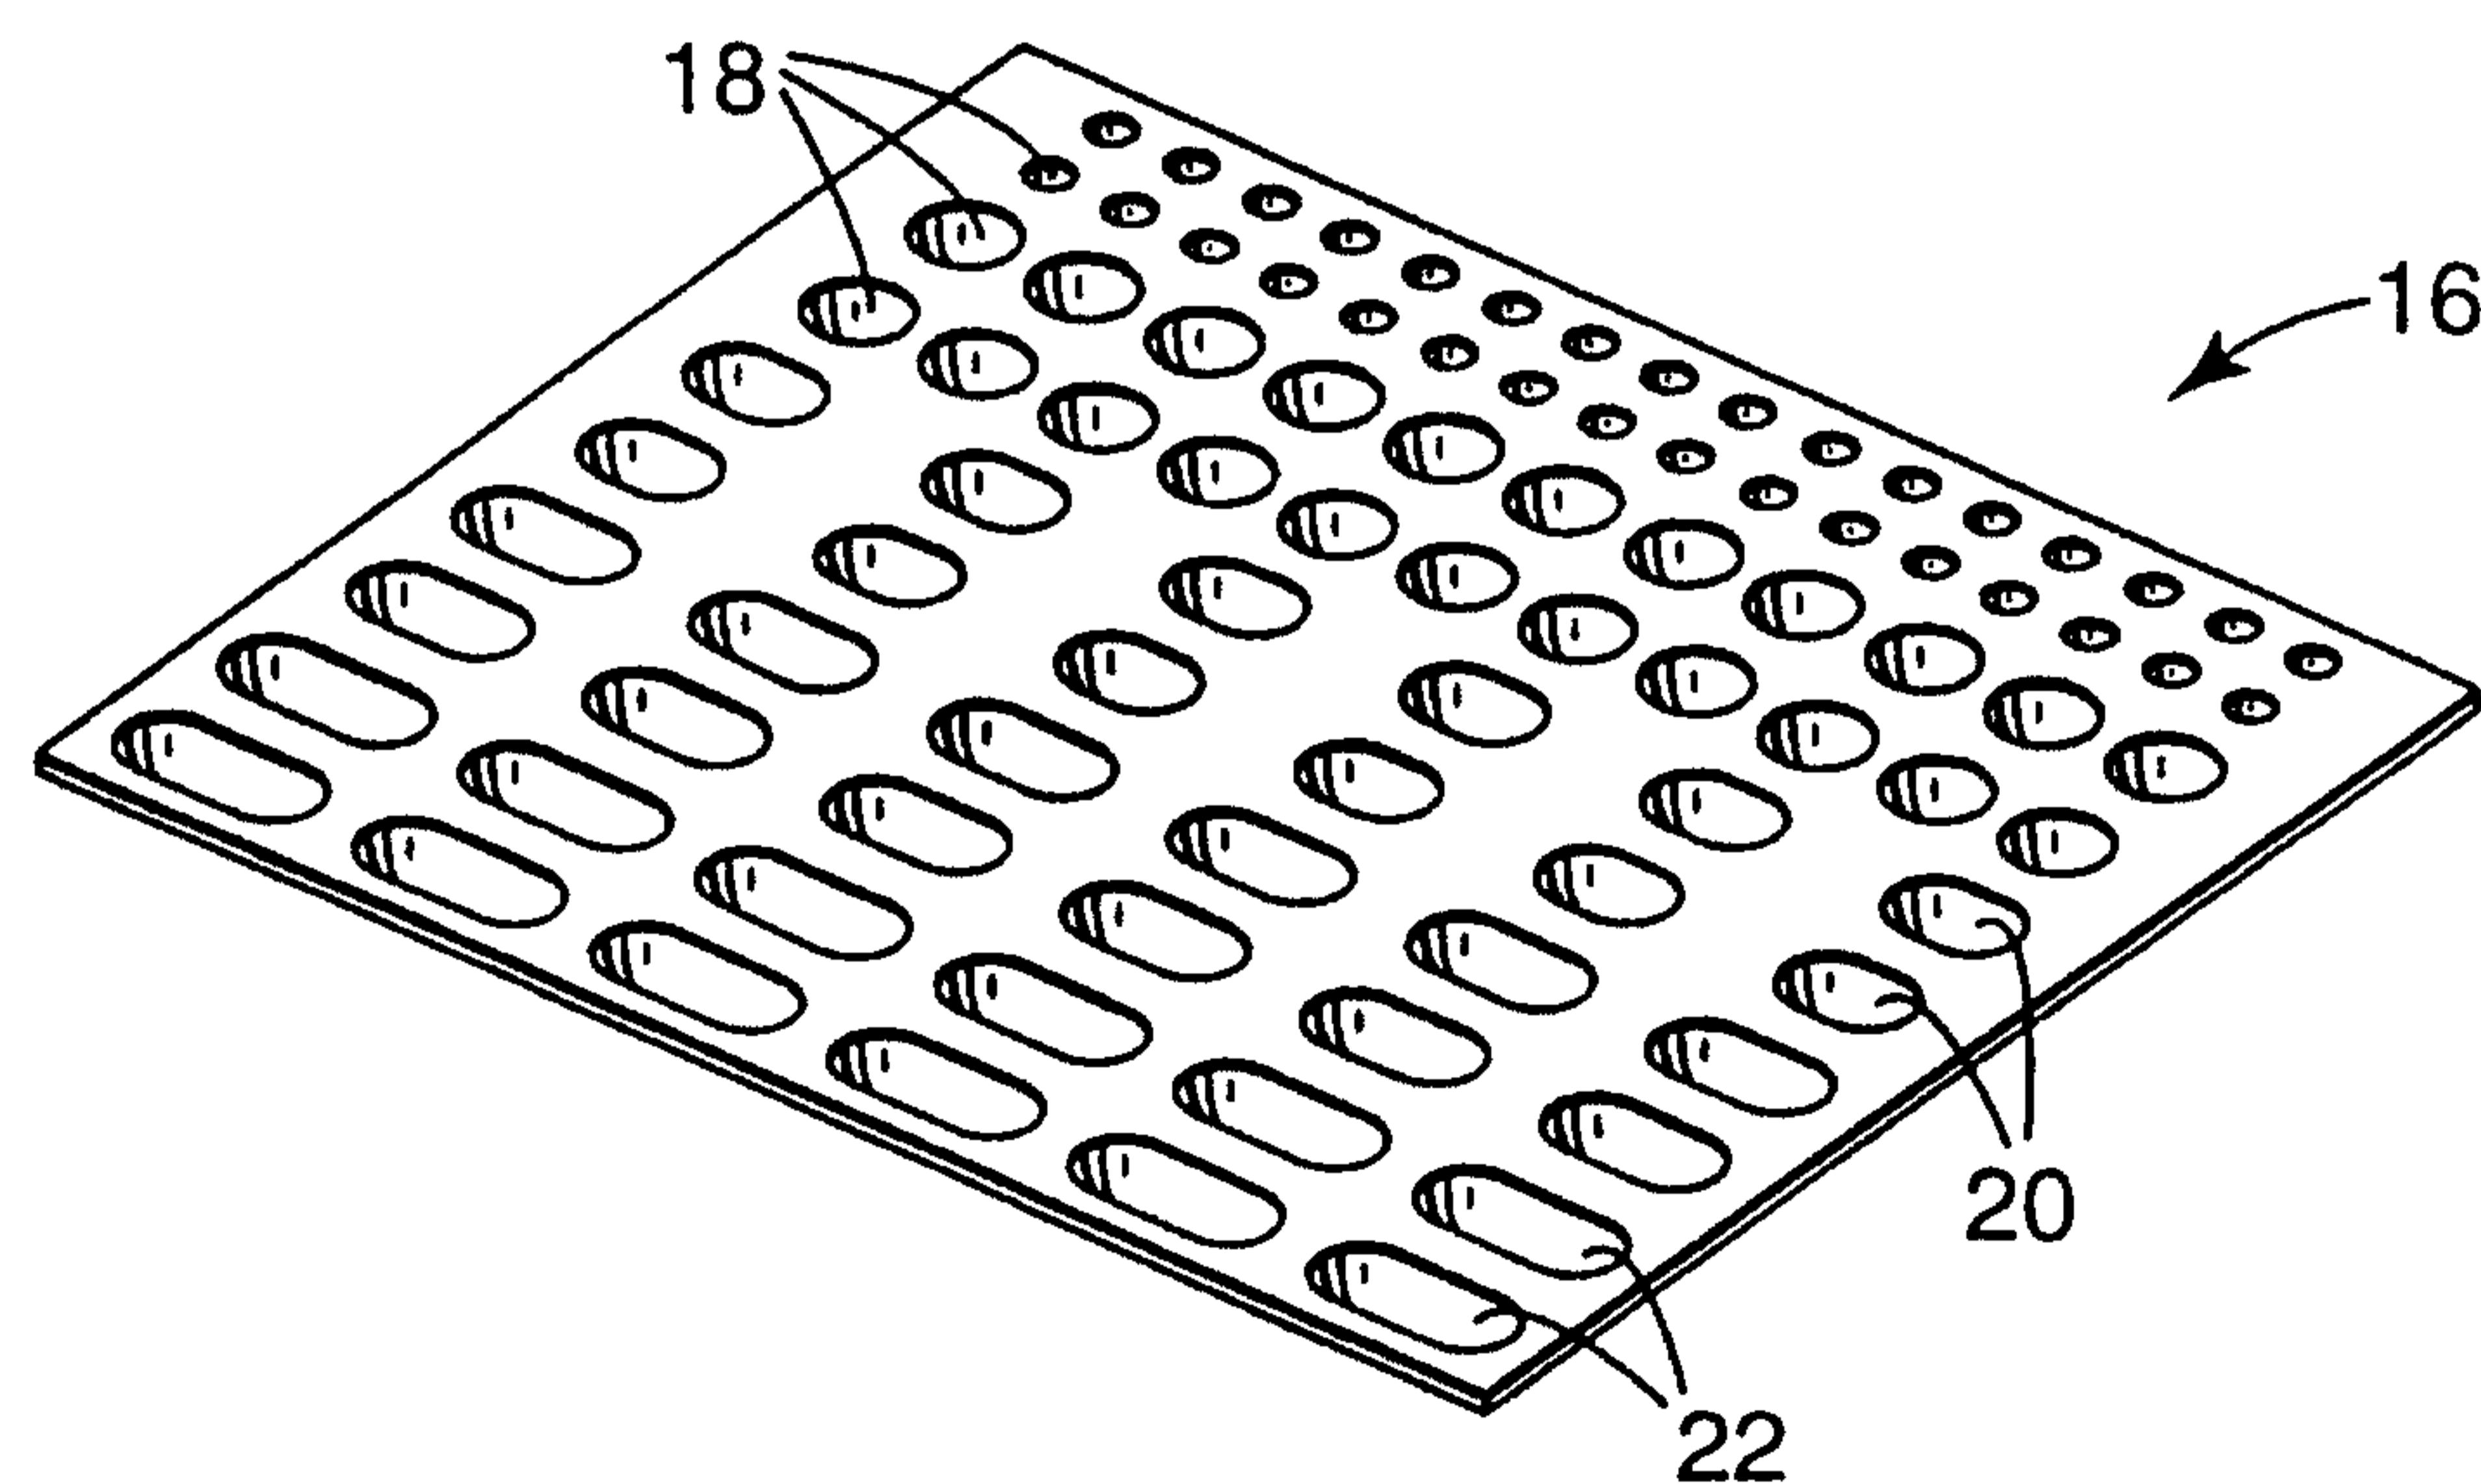

*Fig. 2*

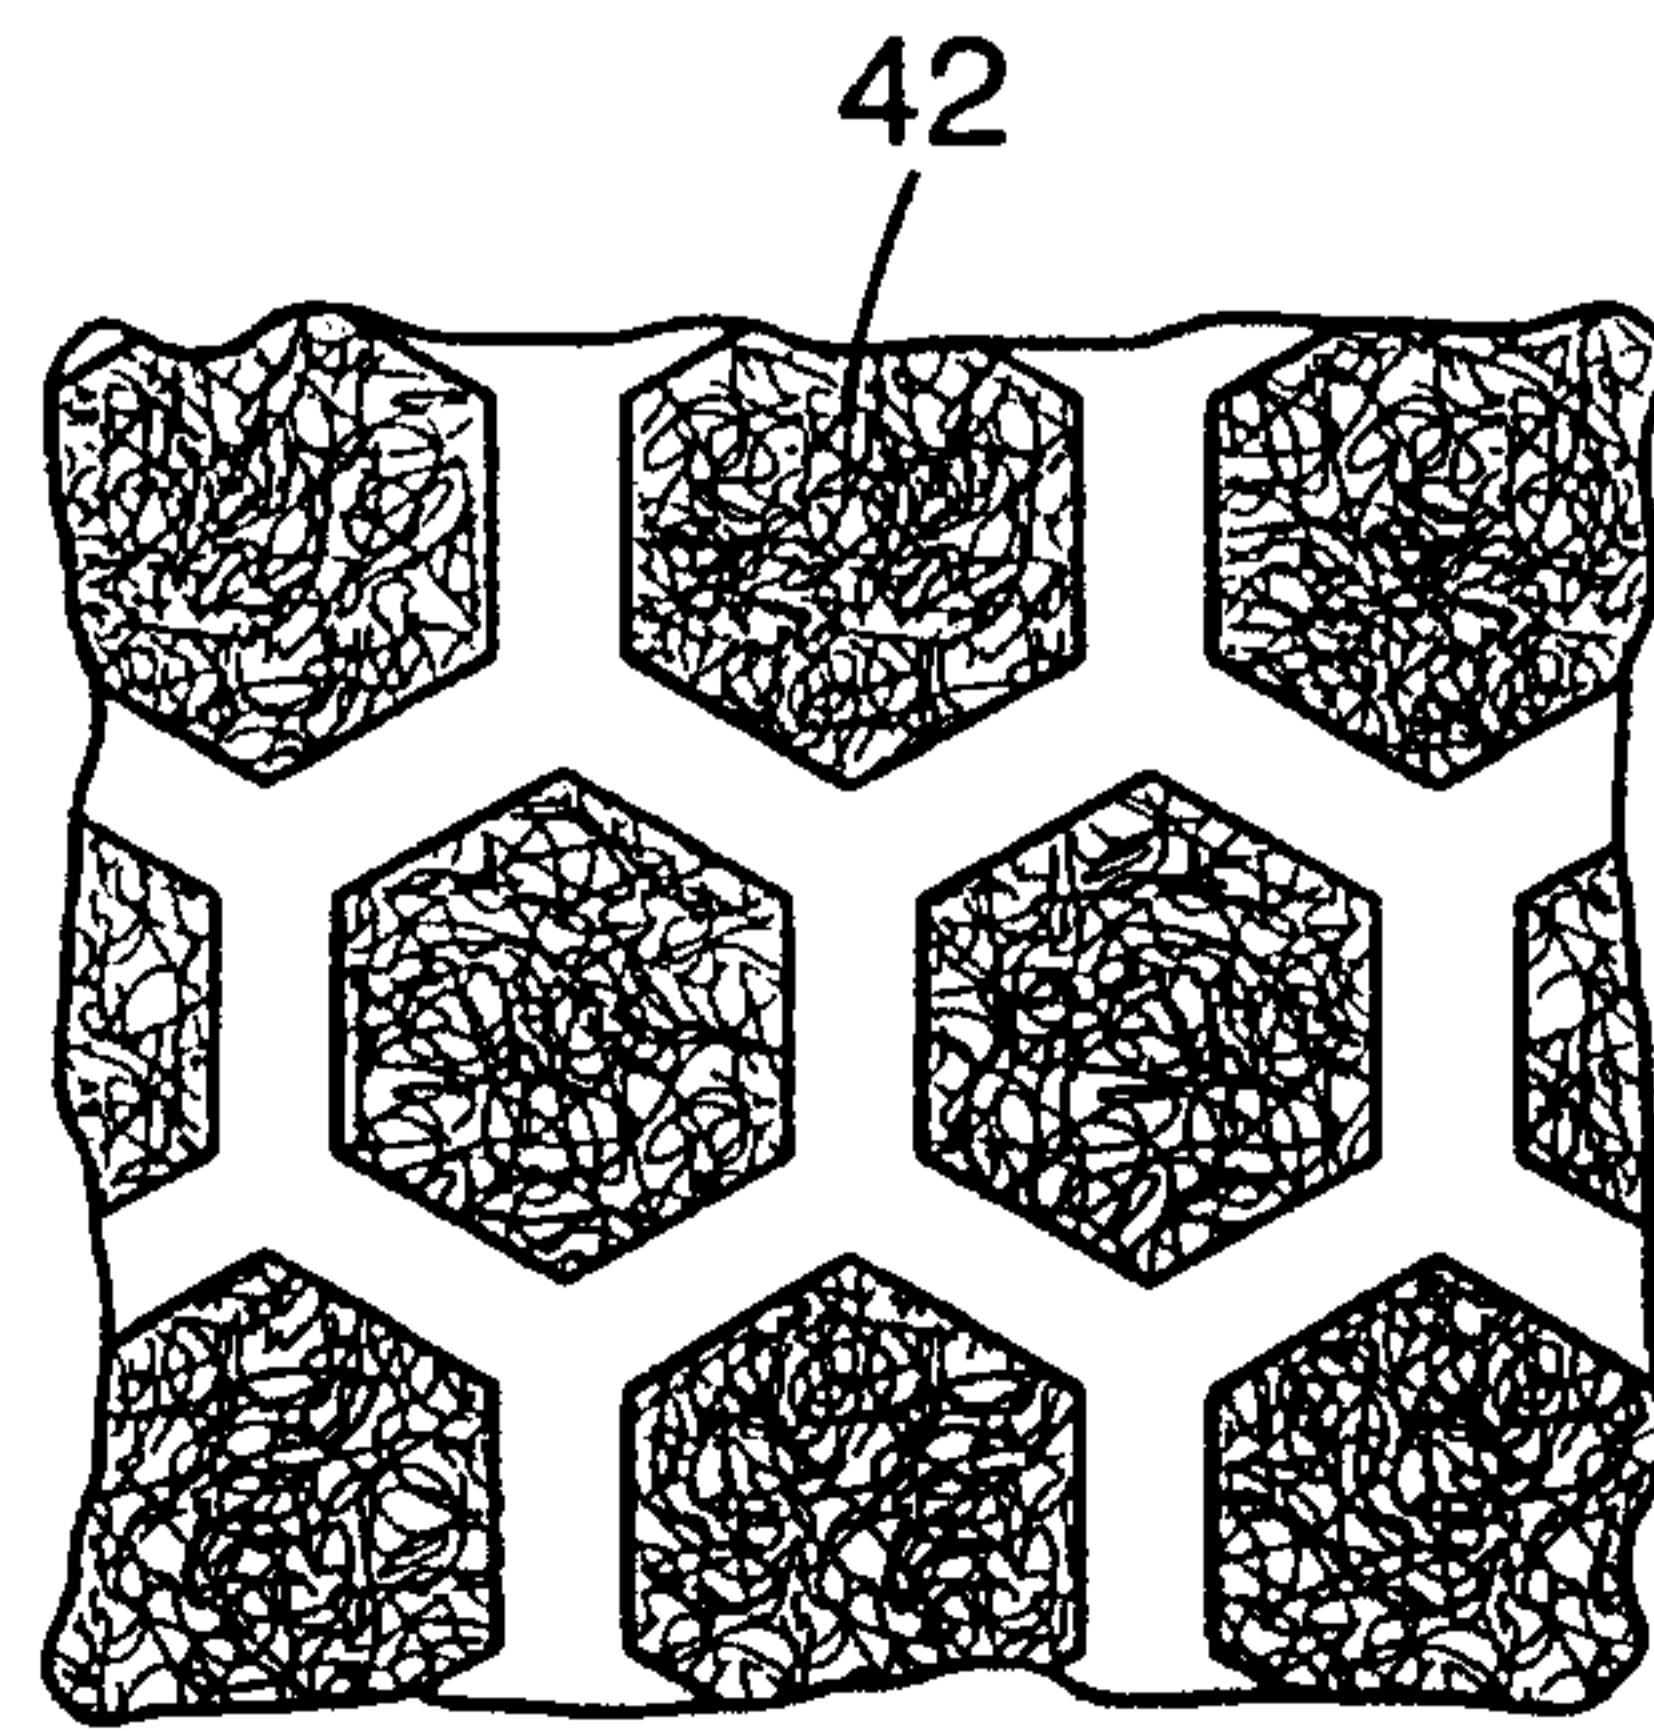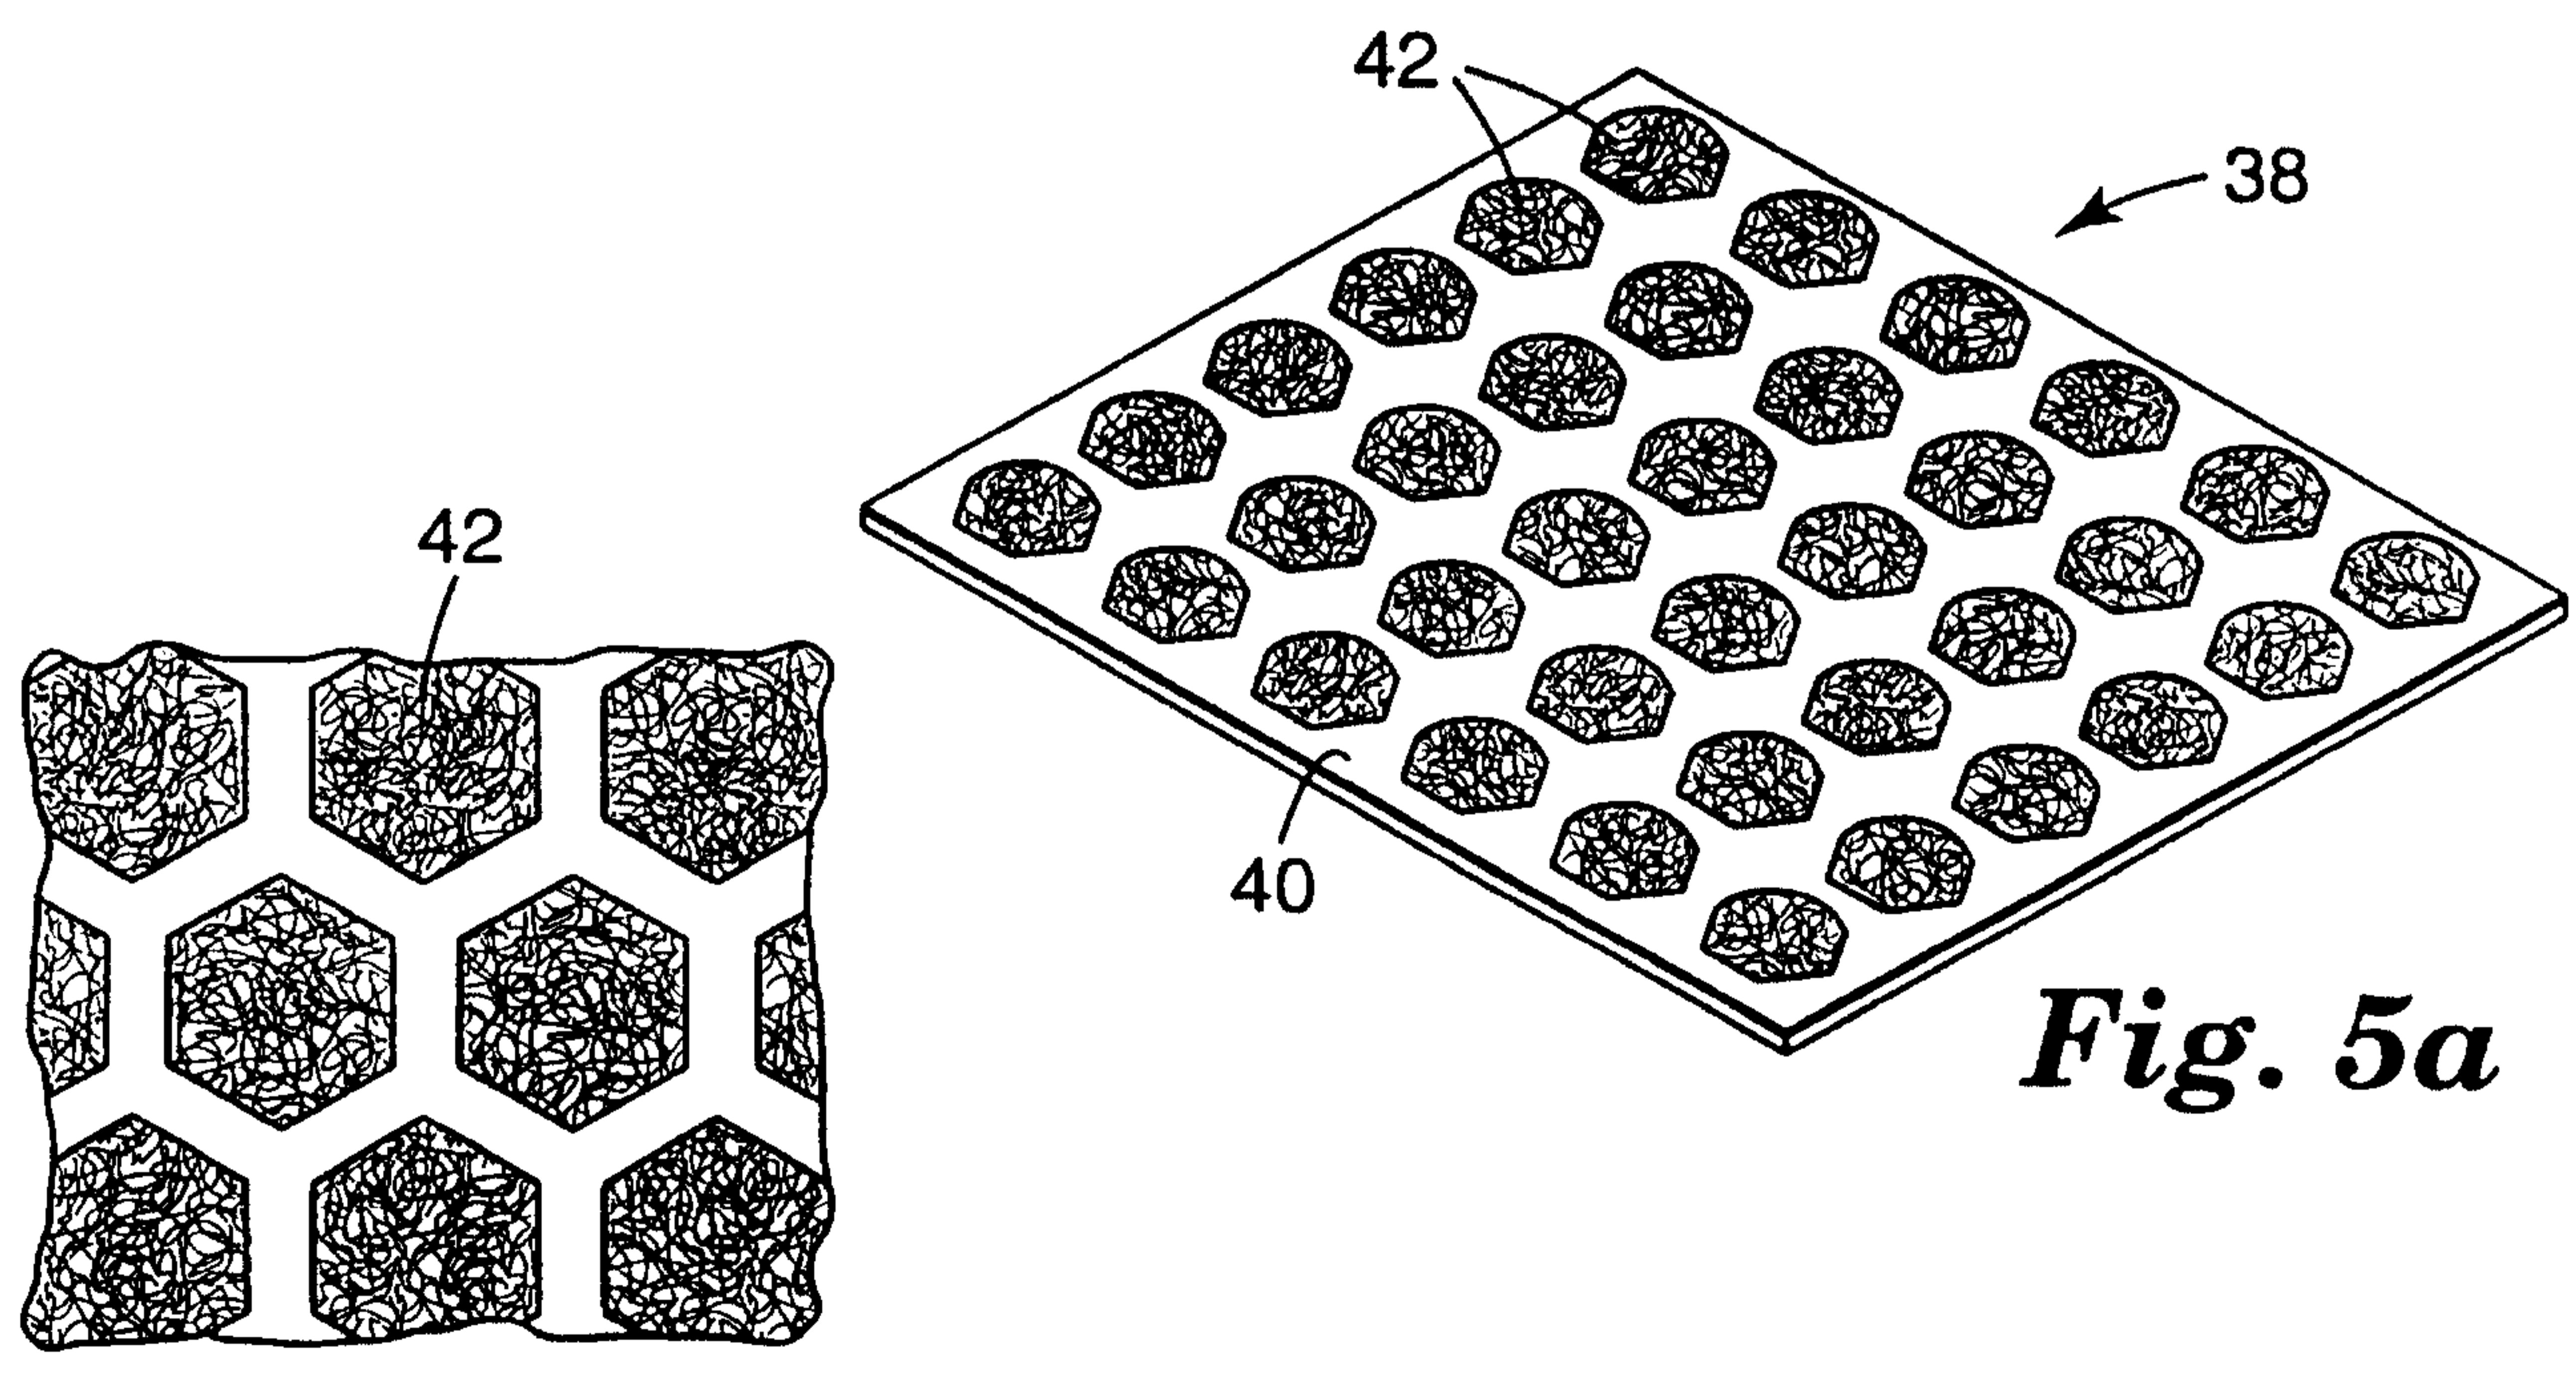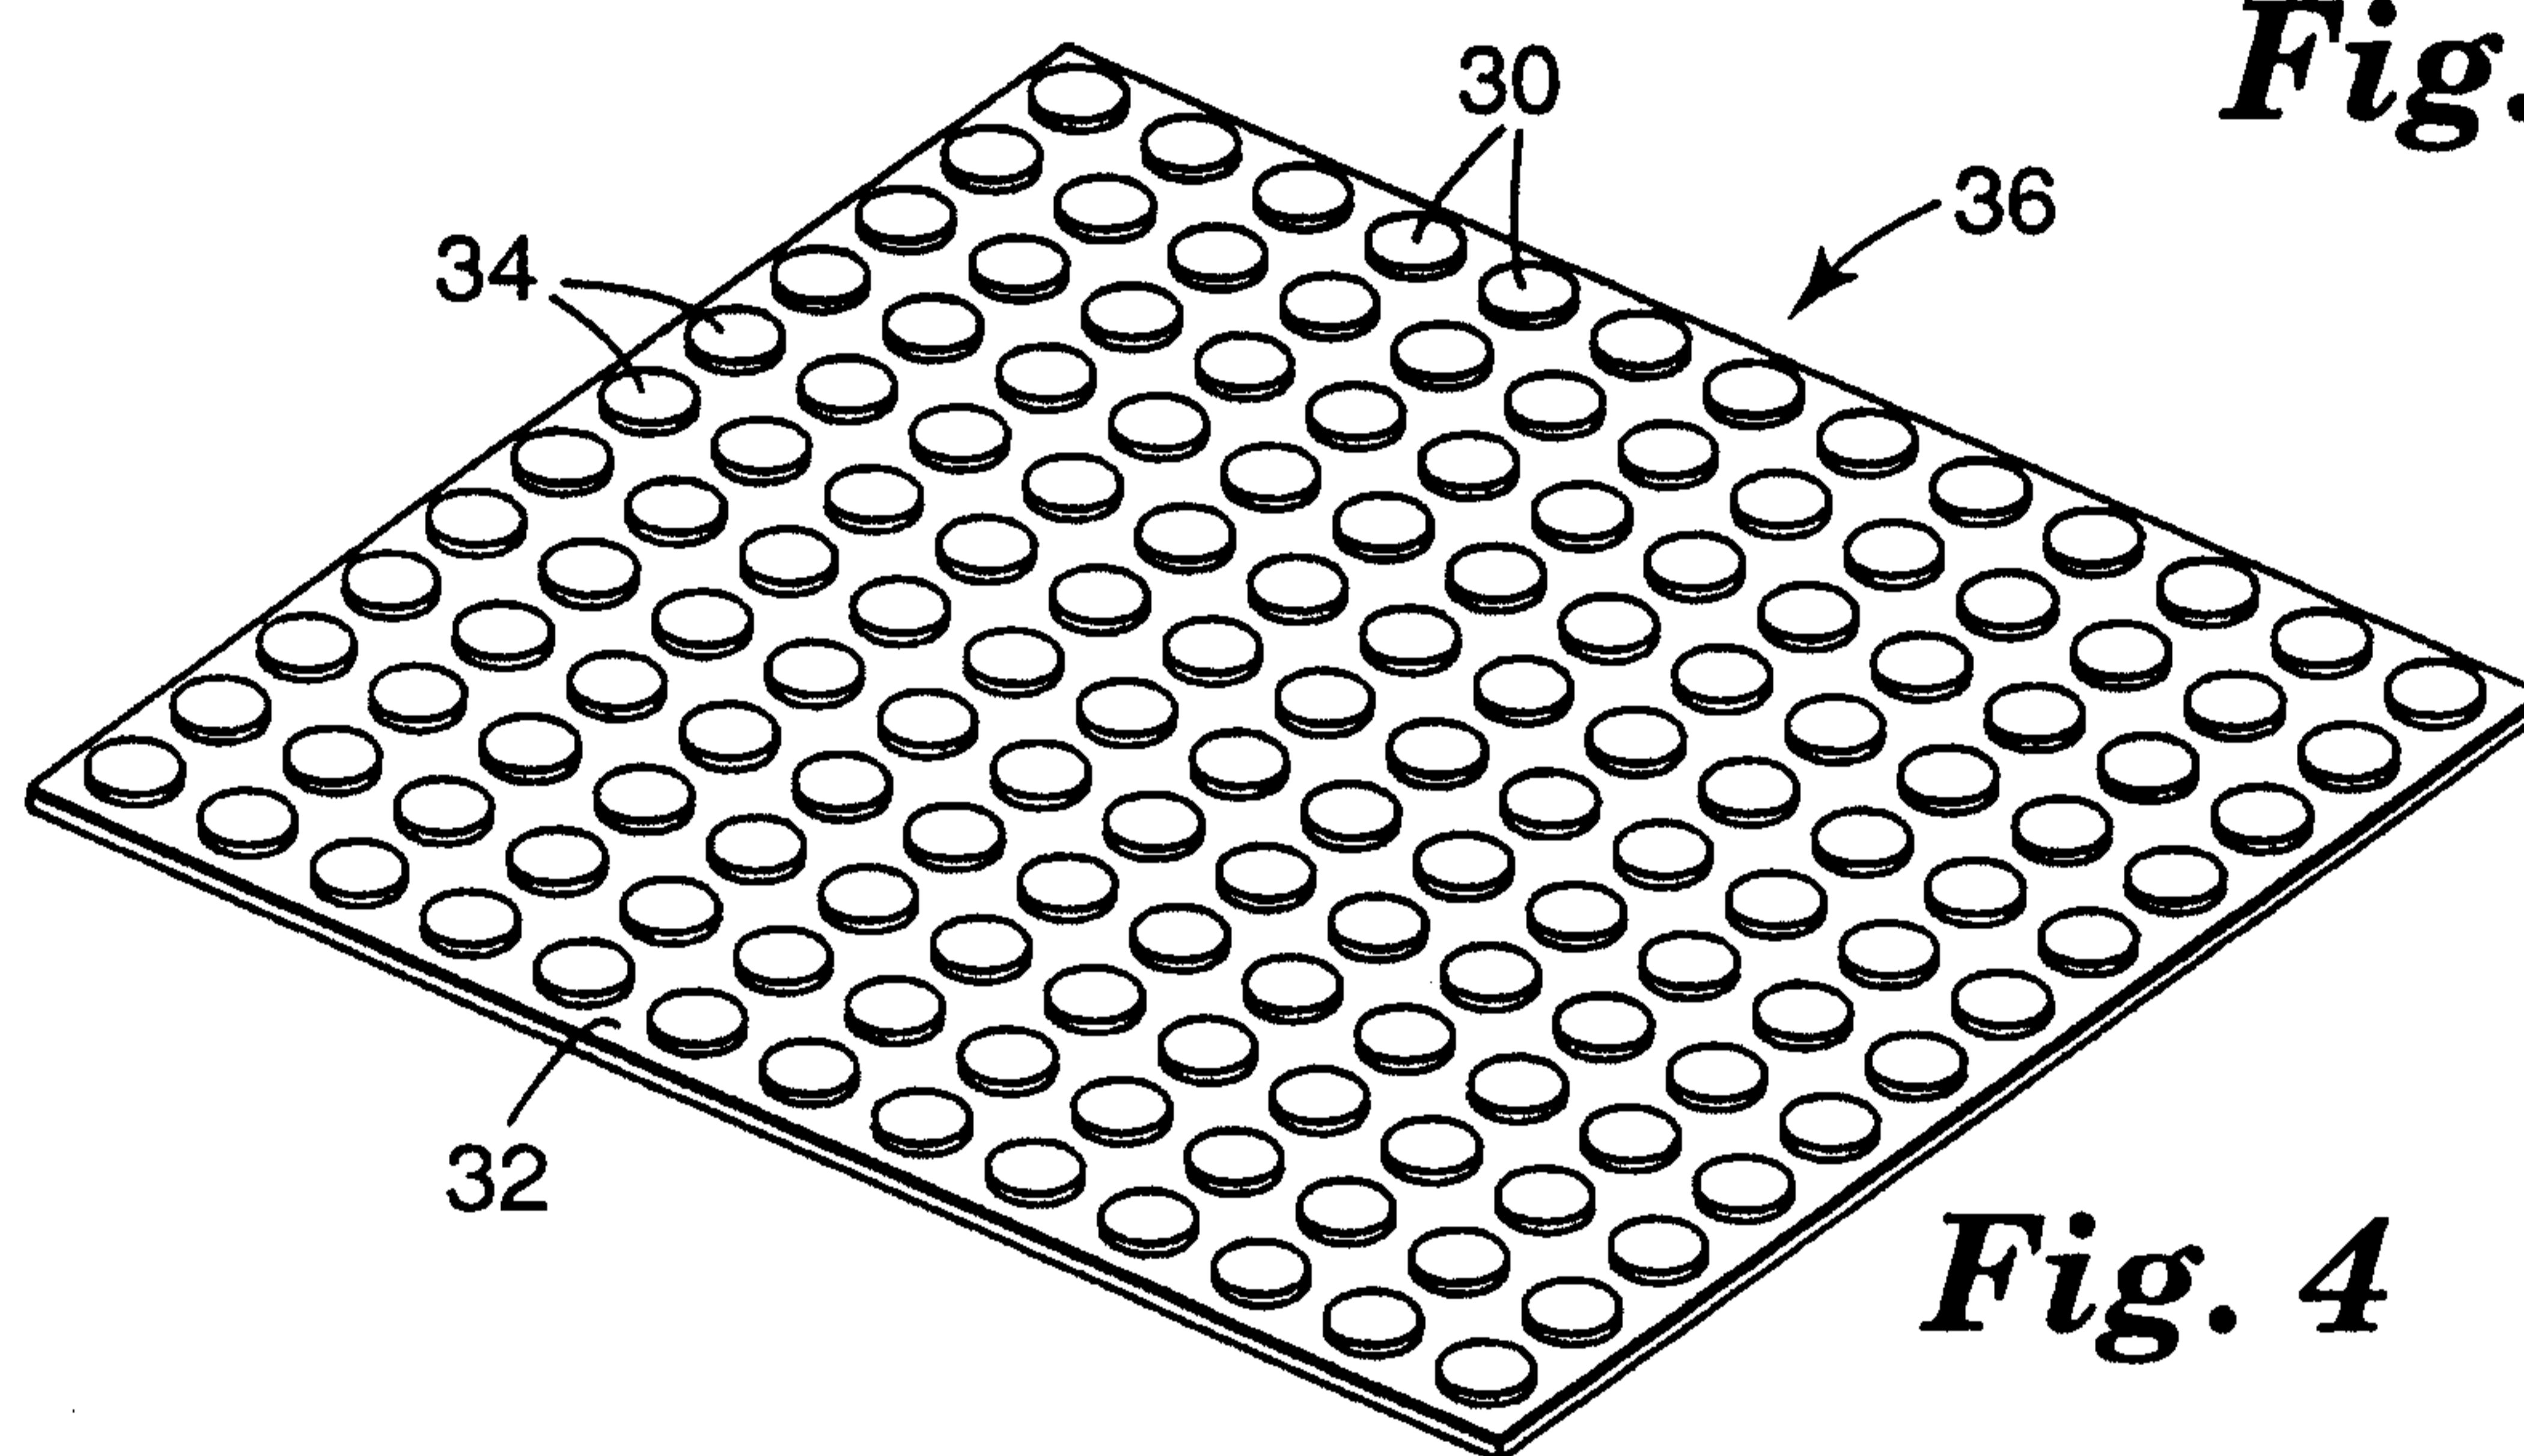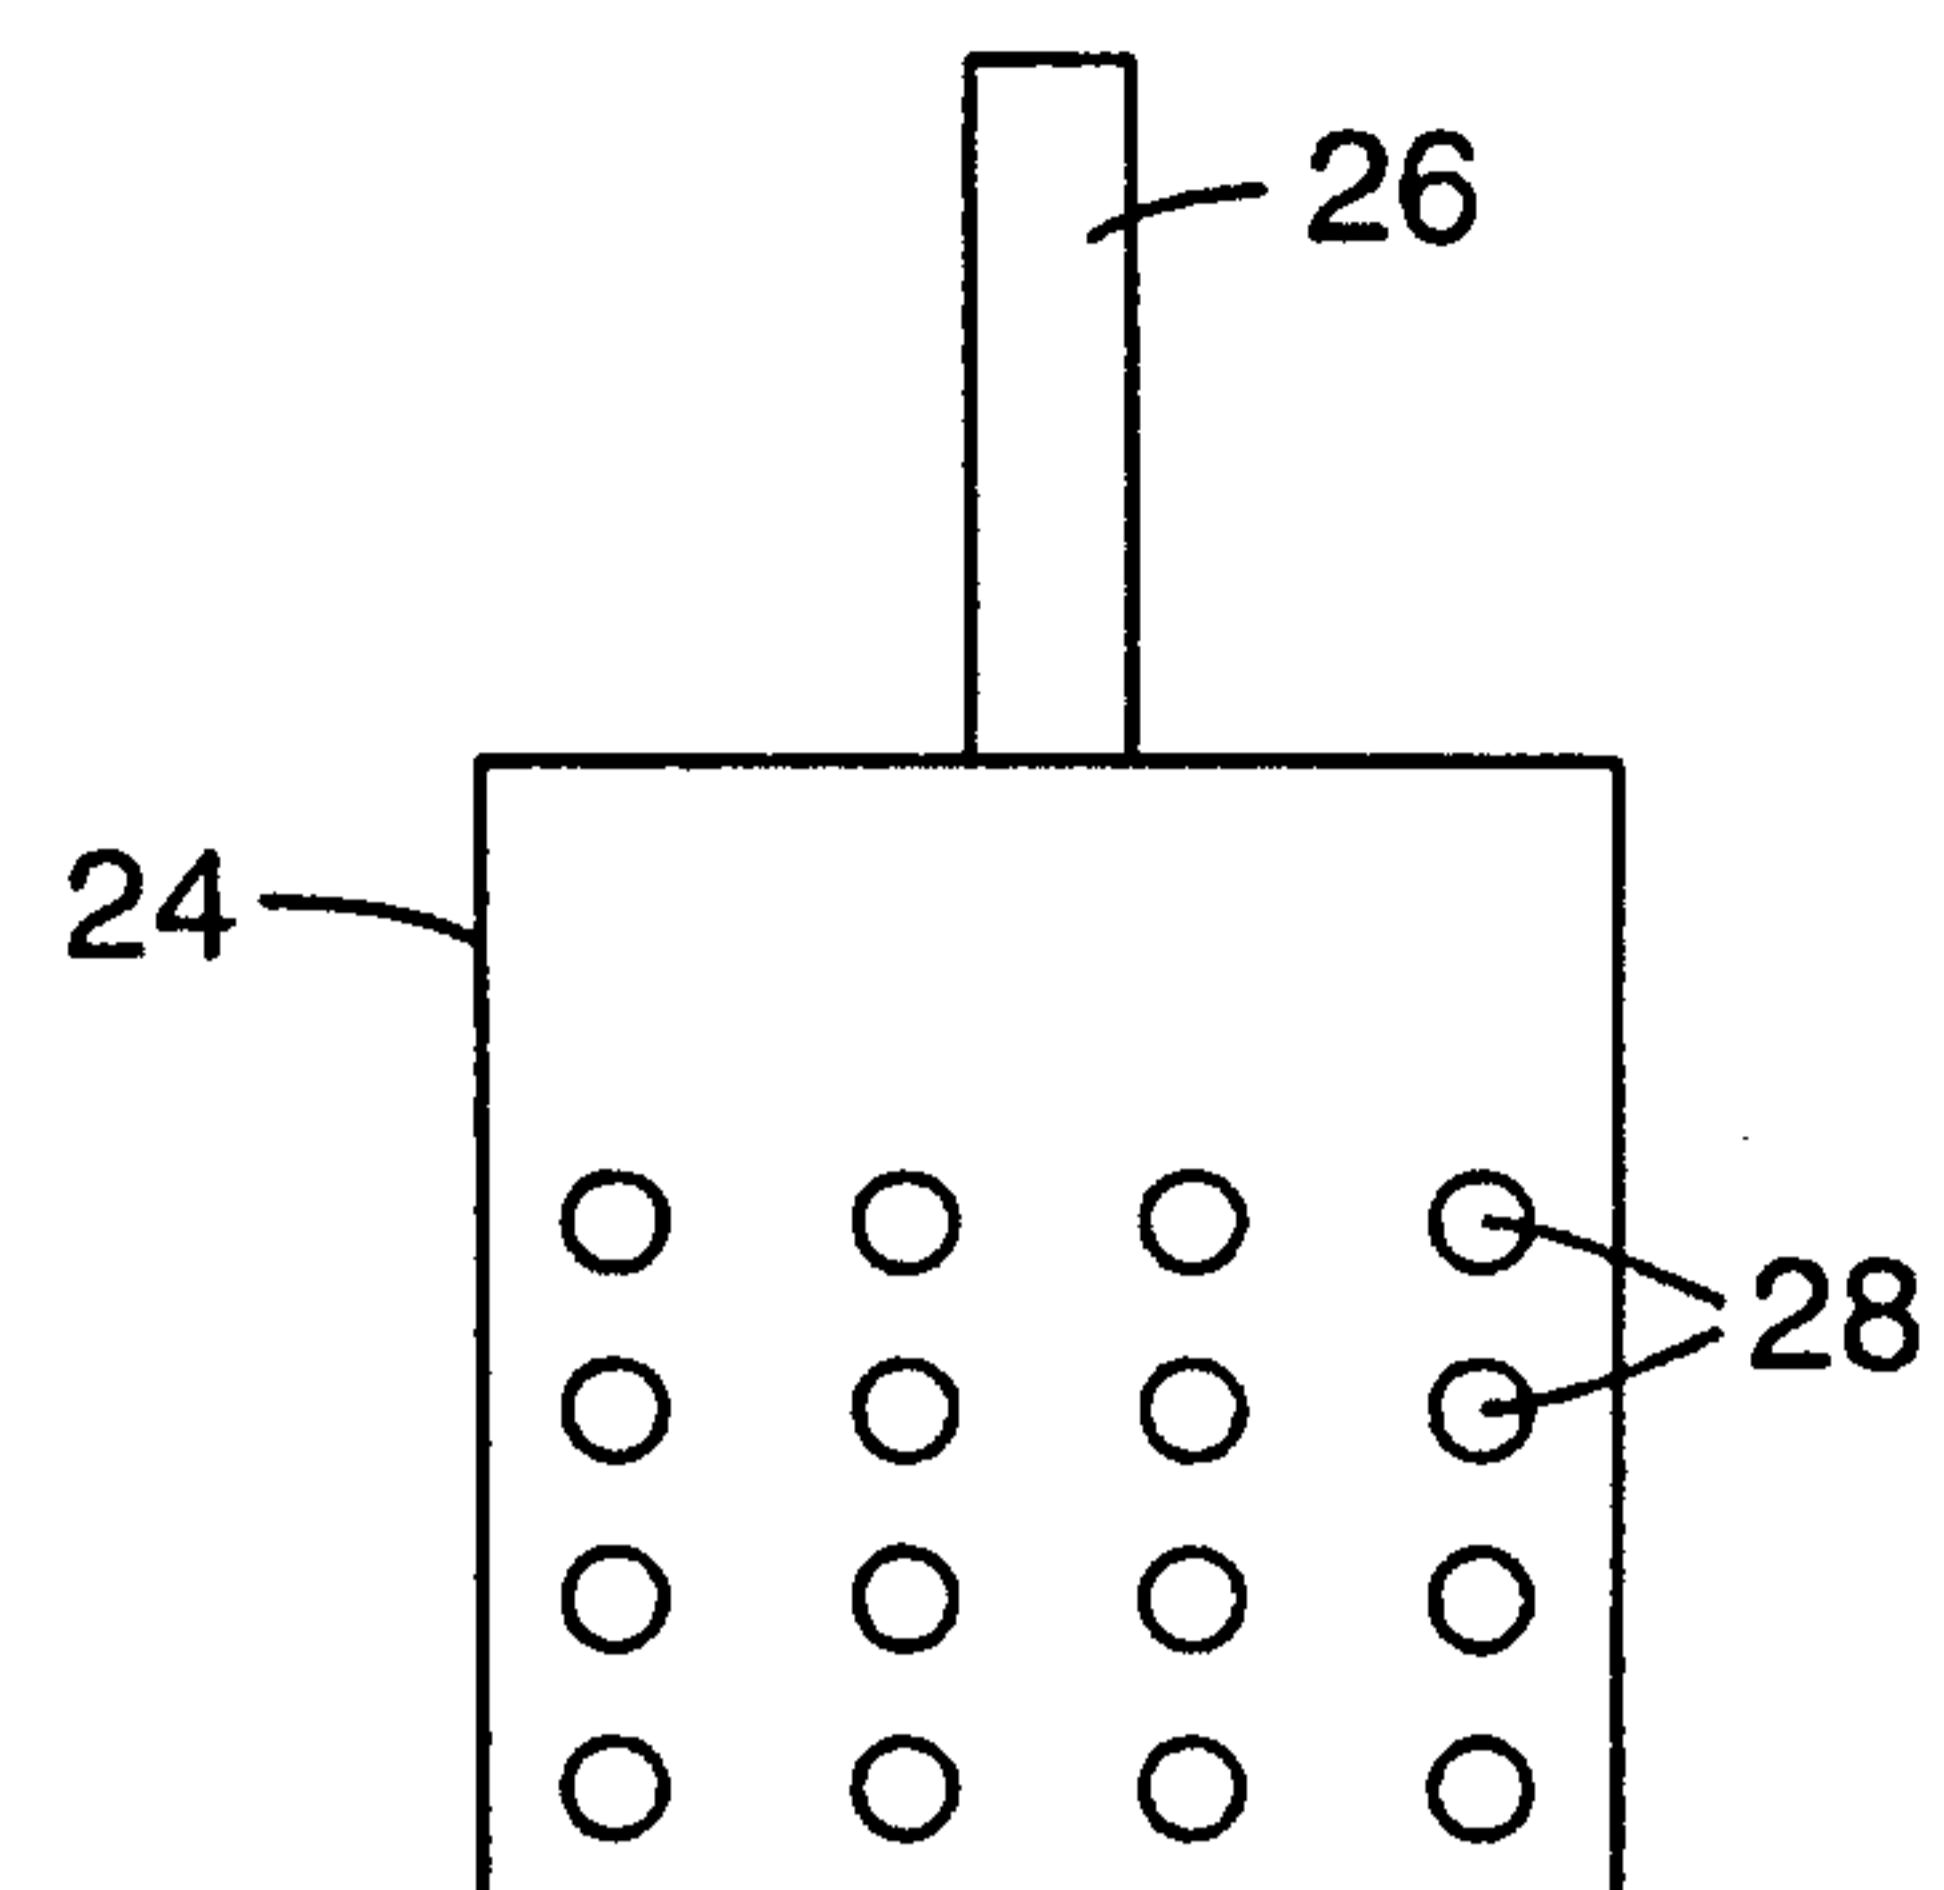

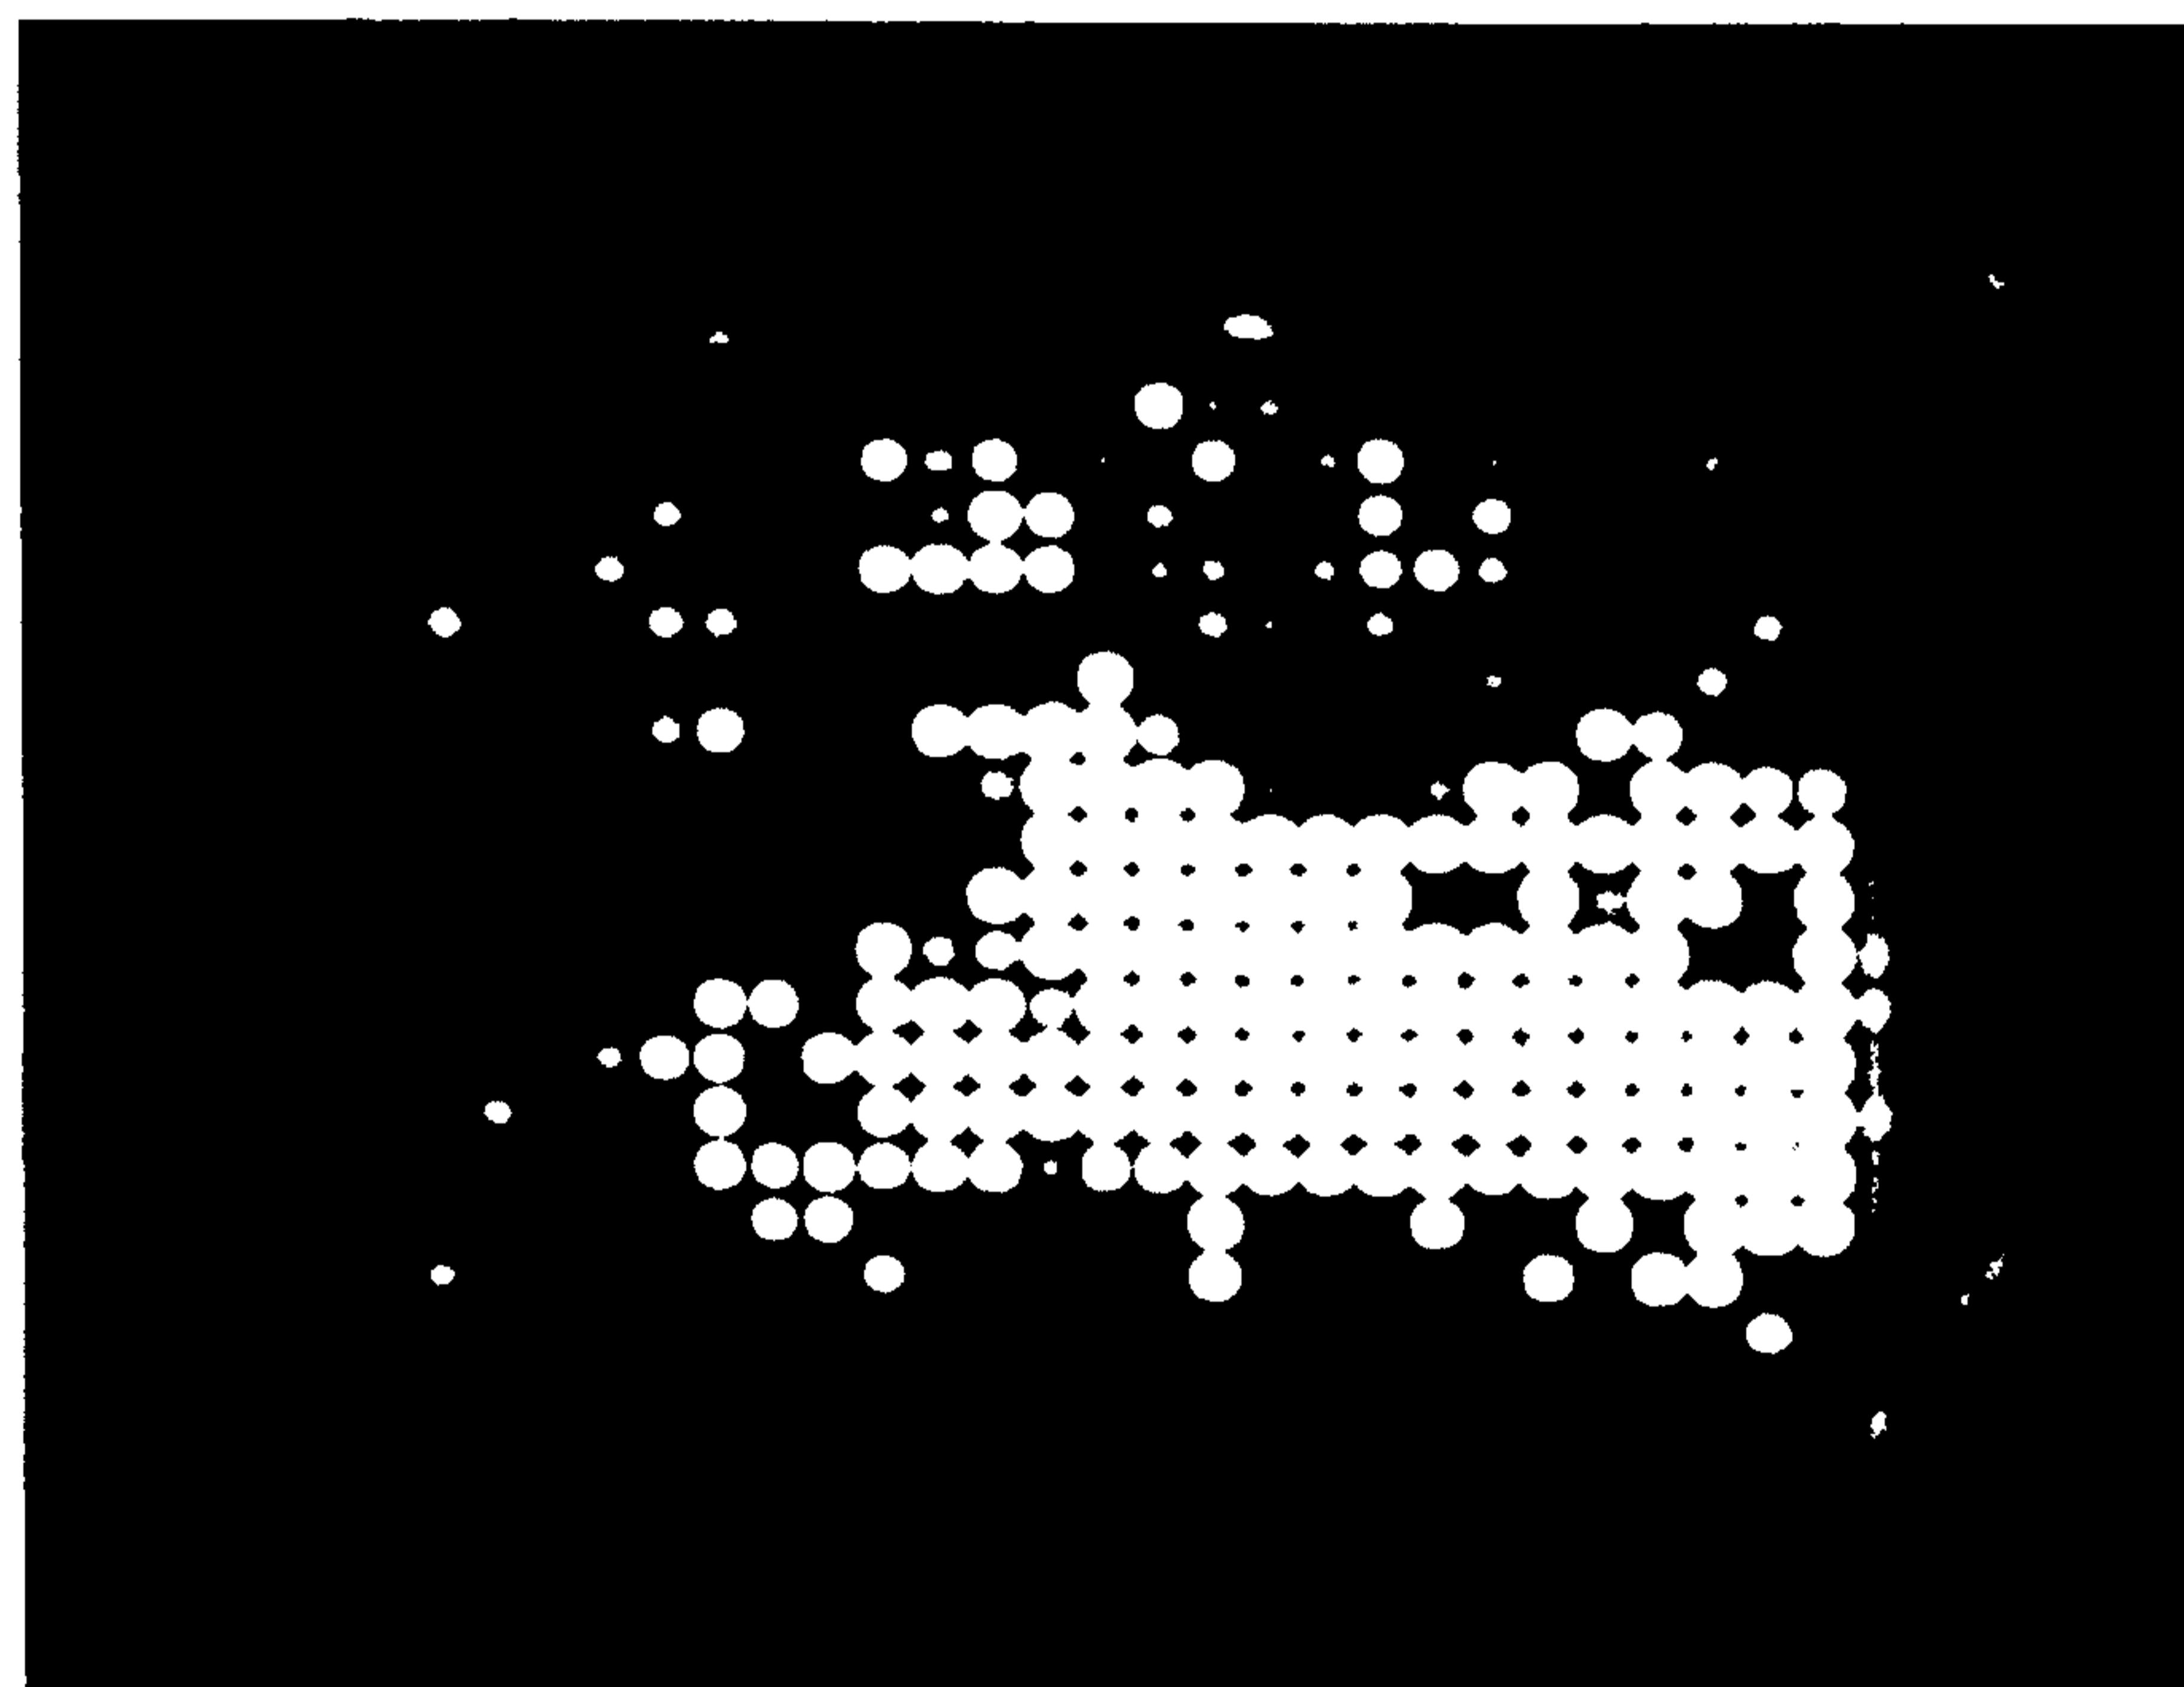


FIG.6A

WO 98/45406

4/4

PCT/US97/14134




FIG.6B

