




(86) **Date de dépôt PCT/PCT Filing Date:** 2013/08/27
(87) **Date publication PCT/PCT Publication Date:** 2014/03/13
(45) **Date de délivrance/Issue Date:** 2018/09/04
(85) **Entrée phase nationale/National Entry:** 2015/02/25
(86) **N° demande PCT/PCT Application No.:** US 2013/056756
(87) **N° publication PCT/PCT Publication No.:** 2014/039320
(30) **Priorité/Priority:** 2012/09/06 (US13/604,700)

(51) **Cl.Int./Int.Cl. A61B 18/14** (2006.01)
(72) **Inventeur/Inventor:**
SHERMAN, MARSHALL L., US
(73) **Propriétaire/Owner:**
MEDTRONIC ABLATION FRONTIERS LLC, US
(74) **Agent:** MOFFAT & CO.

(54) **Titre : DISPOSITIF D'ABLATION ET D'ELECTROPORATION DE CELLULES TISSULAIRES**
(54) **Title: DEVICE FOR ABLATING AND ELECTROPORATING TISSUE CELLS**

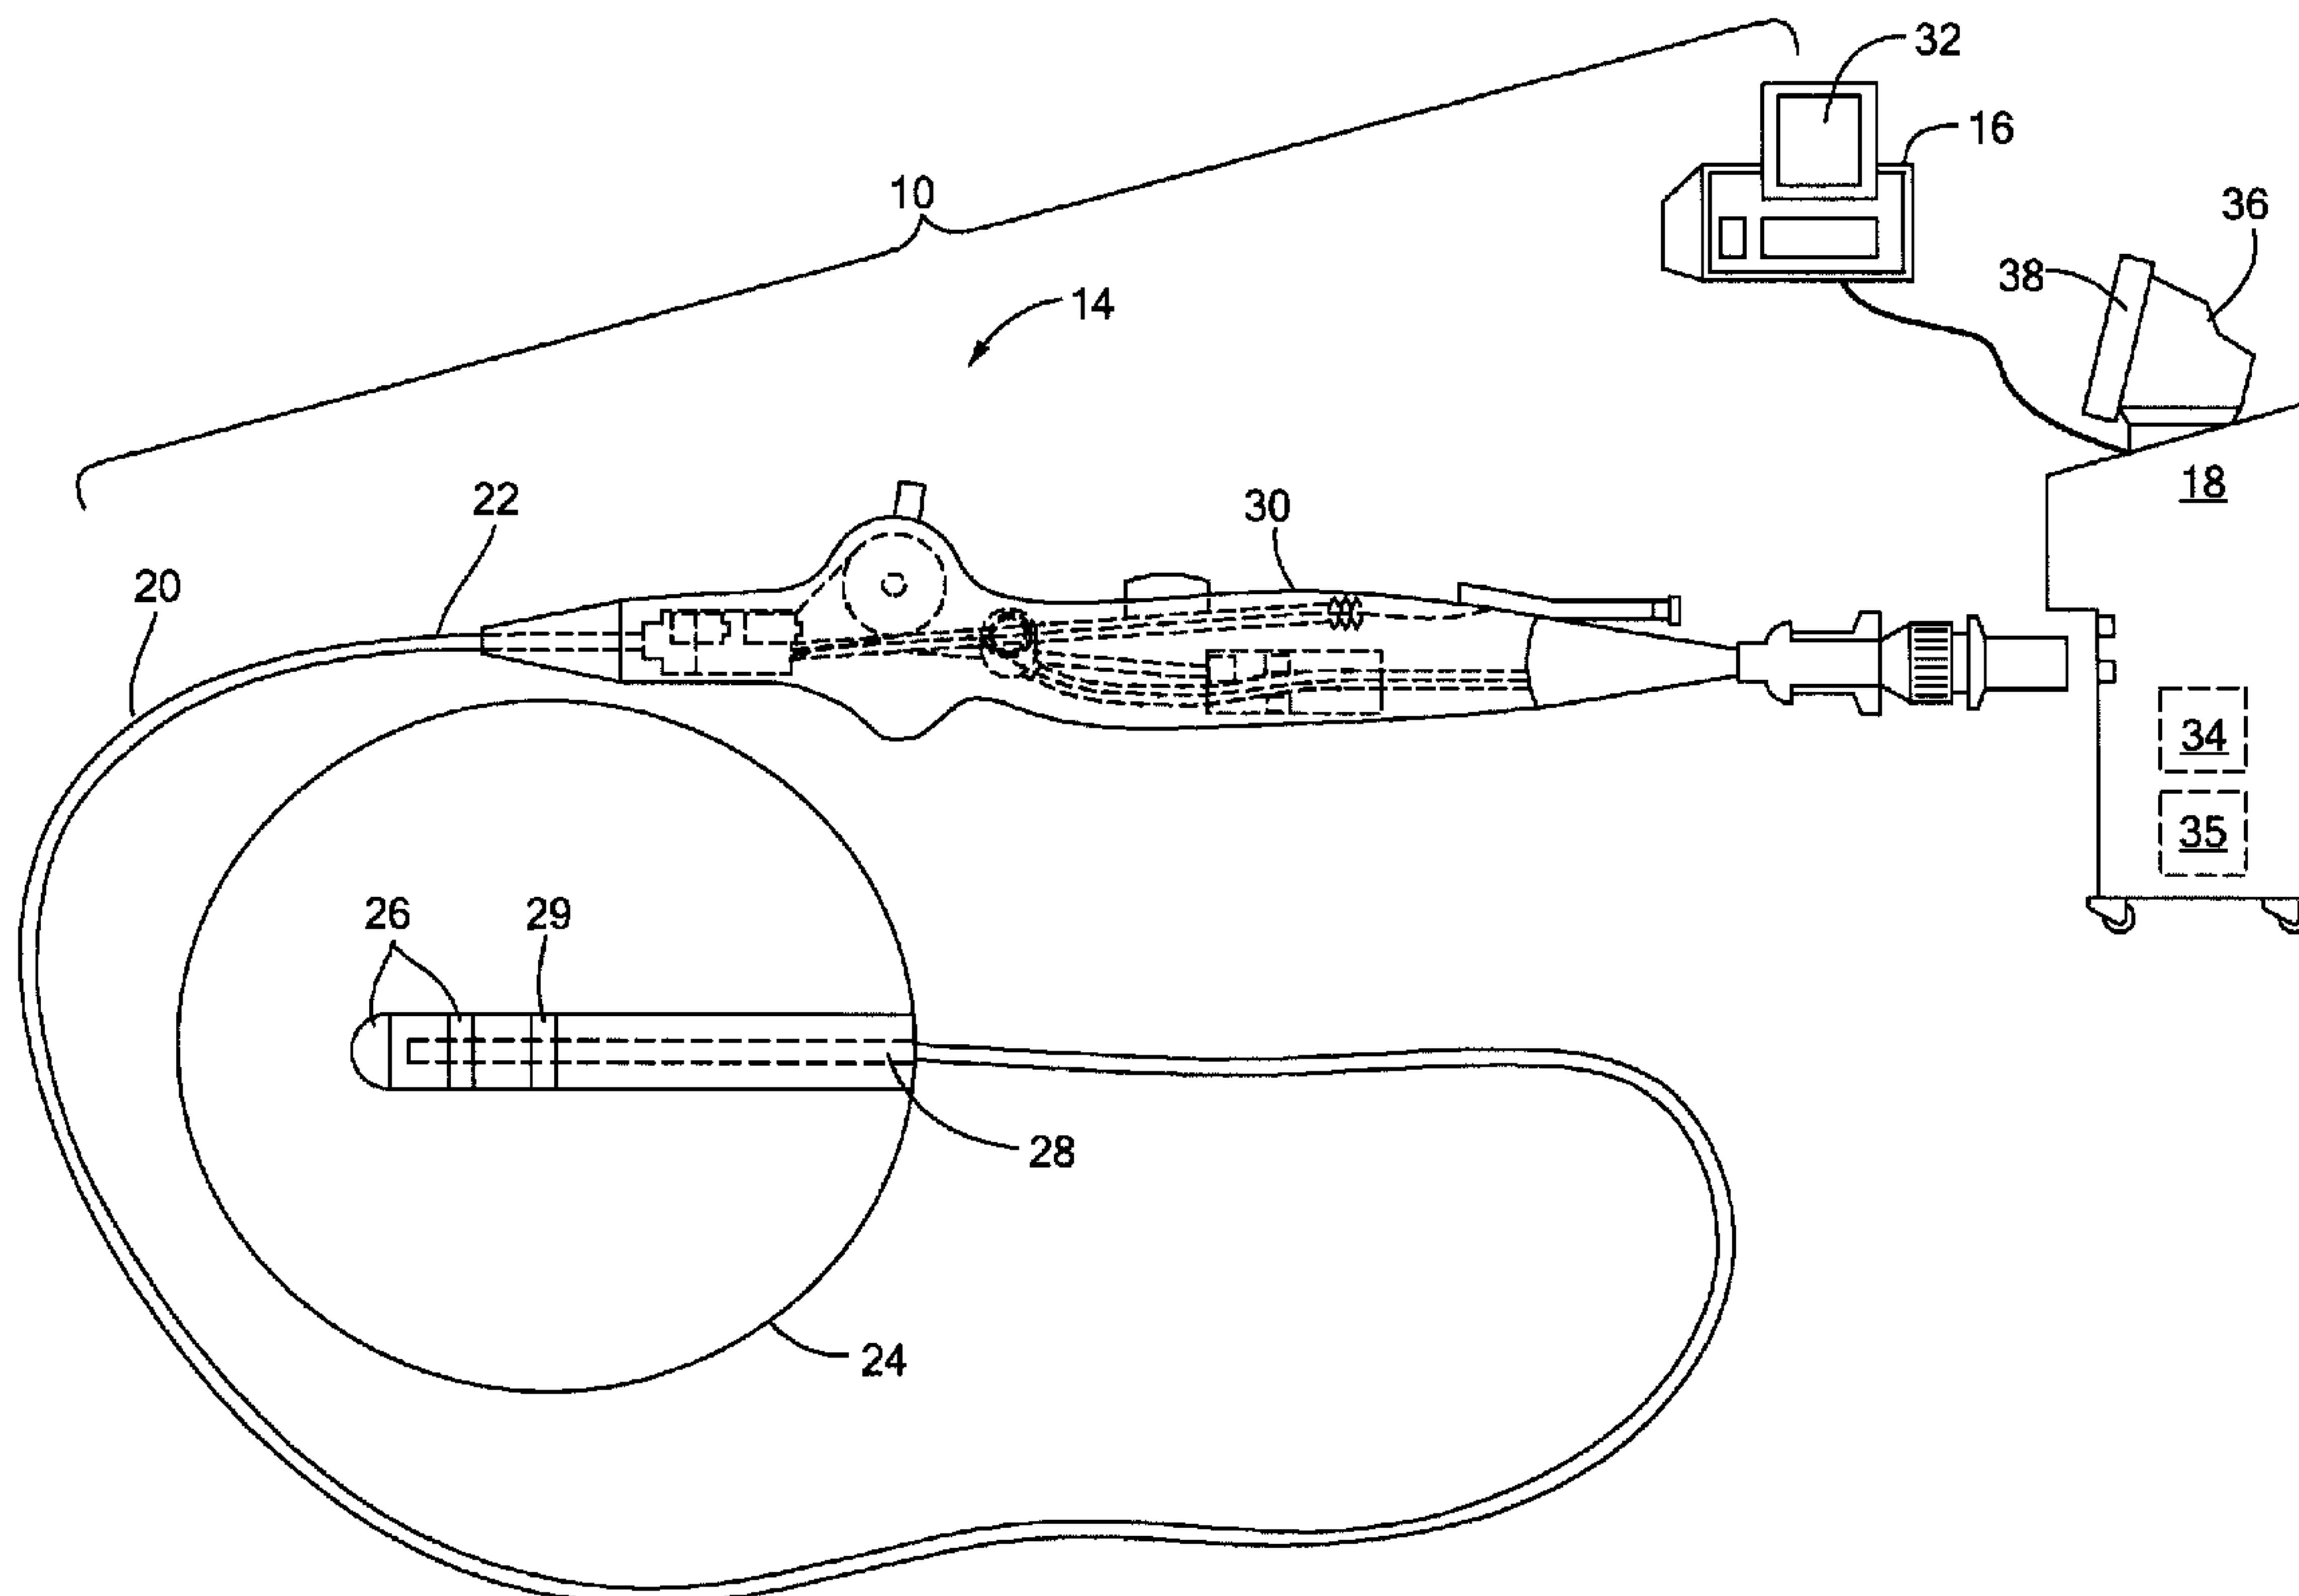

(57) **Abrégé/Abstract:**

A medical system having a medical device and a computer configured to treat target tissue cells using the medical device, the medical device being configured to selectively deliver energy at a voltage at which tissue electroporation occurs, a voltage at which heat ablation occurs, a voltage between the voltage at which tissue electroporation occurs and the voltage at which heat ablation occurs.

Abstract

A medical system having a medical device and a computer configured to treat target tissue cells using the medical device, the medical device being configured to selectively deliver energy at a voltage at which tissue electroporation occur, a voltage at which heat ablation occurs, a voltage between the voltage at which tissue electroporation occurs and the voltage at which heat ablation occurs.

DEVICE FOR ABLATING AND ELECTROPORATING TISSUE CELLS

FIELD OF THE INVENTION

The present invention relates to a method and system for high-voltage
5 radiofrequency ablation using combined heat and electroporation to produce a deeper
lesion while avoiding the production of excess heat at the tissue surface.

BACKGROUND OF THE INVENTION

The use of an electric field is relatively new medical treatment for such
purposes as the enhancement of chemotherapy (electrochemotherapy), cellular
10 ablation, and intracellular electromanipulation. All three treatments involve pulses of
energy, although using different frequencies and pulse durations. Ablation, such as of
tumor or liver cells, occurs when cells are exposed to high-voltage electrical field
pulses. In the presence of these pulses, the electrochemical potential across the cell
membrane is altered and instabilities in the polarized lipid bilayer are induced, which
15 may lead to the development of irreversible pores (or enlargement of existing pores)
in the cell membrane. The phenomenon may cause cell death through the loss of
cellular contents or entry of surrounding contaminants.

This increase in cell membrane permeability when exposed to an electric field
is generally referred to as electroporation, and may be brought about by the
20 application of pulses of direct current (DC) electrical energy applied internally (via,
for example, a catheter) or externally. However, the repetition frequency of electric
pulses is considered to effect muscle contractions, which can produce a burning
sensation or intense pain in patients.

Further, deep lesions are sometimes required to effectively treat some cardiac
25 conditions. For example, atrial fibrillation may be caused by aberrant electrical
conductivity pathways through and around scarred myocardial tissue, which cause an
electrical "feedback loop" and irregular heartbeat. To destroy these aberrant
pathways, the myocardial tissue must be ablated deeply enough to stop the
problematic electrical signals from continuing. The creation of deep lesions requires
30 prolonged application of energy and/or high temperatures. However, the surface of
the tissue must be maintained at cool enough temperatures to avoid charring or micro
embolus formation, which can lead to unintended tissue death or stroke.

Therefore, a system and method are desired that is capable of producing deep lesions without the production of high heat and without causing patient discomfort. The system and method of the present invention involve the application of higher voltage radiofrequency energy to use both heat and electroporation to perform ablation while avoiding undesired tissue damage due to excess heat at the tissue surface.

SUMMARY OF THE INVENTION

The present invention advantageously provides a method and system for producing deep lesions without the production of high heat. The method generally includes treating target tissue cells using a medical device that is configured to selectively deliver energy at a voltage at which tissue electroporation occurs, energy at a voltage at which heat ablation occurs, or any voltage therebetween. The medical device may also be configured to reduce the temperature of the tissue cells to a temperature at which cryoablation occurs. The applied energy may be radiofrequency (RF) energy, and the RF energy may be an alternating current energy having a frequency of between approximately 20 kHz and approximately 1MHz. Electroporation energy may be delivered between approximately 500 volts RMS and approximately 3000 volts RMS. Further, a voltage at which heat ablation occurs is applied to target tissue cells before applying a voltage at which electroporation occurs. Still further, the medical device may include a plurality of electrodes and radiofrequency energy is delivered to each of the plurality of electrodes, the energy delivered to each of the plurality of electrodes being either at in-phase angle or out-of-phase angle relative to the energy delivered to adjacent electrodes.

In an another embodiment, the method may include positioning a medical device in contact with an area of target tissue, the medical device including a plurality of electrodes in communication with a radiofrequency generator, the generator programmable to deliver energy in at least one of bipolar mode and combination of unipolar mode and bipolar mode, delivering to the target tissue both radiofrequency energy from the medical device at between approximately 500 volts RMS to approximately 3000 volts RMS, and delivering alternating current radiofrequency energy from the medical device at between approximately 100 volts RMS to approximately 150 volts RMS to an area of target tissue. The method may further

include delivering alternating current radiofrequency energy at a voltage between approximately 150 volts RMS and approximately 500 volts RMS. The energy delivered to each of the plurality of electrodes may be delivered at either an in-phase angle or out-of-phase angle relative to the energy delivered to adjacent electrodes.

5 The system may generally includes a medical device having a plurality of electrodes at a distal end of the device, and energy generator in communication with the plurality of electrodes, the generator programmable to deliver between approximately 100 volts RMS and approximately 3000 volts RMS. The device may further include one or more sensors at the distal end. The energy generator may be
10 programmable to deliver between approximately 100 volts RMS and approximately 150 volts RMS during a first treatment cycle and between approximately 500 volts RMS and approximately 3000 volts RMS during a second treatment cycle. Further, the energy generator may be programmable to deliver energy to the plurality of electrodes in at least one of unipolar mode, bipolar mode, and combination thereof

15 BRIEF DESCRIPTION OF THE DRAWINGS

A more complete understanding of the present invention, and the attendant advantages and features thereof, will be more readily understood by reference to the following detailed description when considered in conjunction with the accompanying drawings wherein:

20 FIG. 1 shows a first embodiment of a system in accordance with the present invention;

FIG. 2 shows a second embodiment of a system in accordance with the present invention;

25 FIGS. 3A and 3B show a distal portion of a medical device having a plurality of electrodes and lesions created when the device is operating in unipolar or bipolar mode; and

FIG. 4 shows a flow chart of a method in accordance with the present invention.

DETAILED DESCRIPTION OF THE INVENTION

30 The present invention provides systems and methods of use thereof for producing deep lesions without the production of high heat and without causing patient discomfort. High-frequency alternating current (AC) radiofrequency (RF) energy may be used (for example, between approximately 20 kHz and approximately

1MHz, as this range does not stimulate the heart but still provides an electroporetic effect) is used to ablate tissue through either cellular electroporation or heat or a combination thereof, while maintaining tissue surface temperatures below a threshold temperature that causes unintentional charring or the formation of micro emboli.

5 Further, this application of AC RF energy does not cause patient discomfort or pain as does the application of DC energy. Still further, the AC RF energy may be applied at a voltage capable of ablating tissue due to heat energy, a voltage capable of ablating tissue due to electroporation effects, or a voltage at any point along a continuum between heat energy and electroporation energy. Referring now to the drawing
10 figures in which like reference designations refer to like elements, FIG. 1 shows a first embodiment of a system 10 for generating and applying high-voltage RF energy to an area of target tissue 12. The system 10 may generally include a medical device 14, an energy generator 16, and a console 18 for operating, monitoring, and regulating the operation of the device 14.

15 Referring to FIGS. 1 and 2, the medical device 14 may be a catheter, for example, an RF ablation catheter as shown in FIG. 1. The catheter 14 may be adapted for use with a single energy modality only (for example, RF energy), or a combination of energy modalities (for example, RF plus laser, microwave, cryoablation, and/or ultrasound energy). Regardless of the number of energy modalities to which the
20 catheter 14 is suited, however, the catheter 14 must at least be capable of transmitting an electric field that will electroporate target tissue cells 12. For example, the catheter 14 may be capable of transmitting RF energy at a voltage of approximately 2000 V or greater. The catheter 14 may include a flexible elongate body 20 having a proximal portion 22 and a distal portion 24. The distal portion 24 of the elongate body 20 may
25 have a fixed diameter (as shown in FIG. 1), or may include an expandable element (as shown in FIG. 2). The elongate body 20 may include a plurality of treatment elements, such as electrodes 26, at the distal portion 24 for delivering energy to target tissue 12. If a secondary energy modality is used in addition to RF energy, the treatment elements may also include a thermally-transmissive region in addition to the
30 plurality of electrodes 26, such as a balloon or other expandable element, metal structure directly or indirectly exposed to a flow path of cryogenic fluid, or one or more thermally-conductive polymers or composites. For example, FIG. 2 shows a

catheter 14 having a cryoablation balloon 27 in addition to an electrode array 26. The plurality of electrodes 26 may be of any number, configuration, or shape, for example, a plurality of discrete electrodes, band electrodes that partially or entirely circumscribe the elongate body 20 (as shown in FIG. 1) or balloon 27, longitudinally oriented electrodes (as shown in FIG. 2), a tip electrode (as shown in FIG. 2), or clusters of electrodes. The electrodes may be in the form of conductive strips applied to the outer surface of the distal portion 24, and may be made of metal, conductive polymers, conductive ink printing, or micro-capillary printing. The electrodes 26 may be adhesively bonded to the device 14 or applied by ion-deposition or plasma deposition. Alternatively, conductive materials such as silver, platinum, or gold may be doped or otherwise mixed into the balloon 27 material.

The catheter 14 may define one or more lumens 28 for providing mechanical, electrical, and/or fluid communication between the proximal portion 22 and the distal portion 24 of the elongate body 20. The one or more lumens 28 may be thermally insulated to substantially prevent heat exchange between, for example, a lumen 28 (and any devices or components therein) and the plurality of electrodes 26. The distal portion 24 of the elongate body 20 may further include one or more sensors 29 for detecting pressure, temperature, electrical impedance, or other system and/or environmental parameters (for example, the surface temperature of the target tissue 12). The one or more sensors 29 may be of any configuration (for example, ring sensors as shown in FIG. 1, or tip and balloon sensors as shown in FIG. 2), and may be in communication with the console 18, with which the user may control the energy delivered to the catheter 14. For example, if a temperature sensor 29 detects a tissue surface temperature at or near a threshold temperature, the energy application may be stopped (either automatically by the system 10 or manually by the user) and/or the RF voltage reduced in order to avoid unintended tissue damage.

The proximal portion 22 of the elongate body 20 may be coupled to a handle 30, which may include various ports for electrical and fluid connectors, leads, junctions, or tubes, and may also include various control assemblies, such as switches or valves, as well as safety detection or shutdown components. For example, the handle 30 may include connectors that are matable directly or indirectly by way of one or more umbilicals to the console 18. Further, the handle 30 may also include an

element such as a lever or knob for manipulating or deflecting at least a portion of the elongate body 20.

Continuing to refer to FIGS. 1 and 2, the energy generator 16 may be an RF energy generator capable of delivering energy in multiple modes, such as unipolar, bipolar, and combination thereof, such as 4:1, 2:1, and 1:1 (a duty cycle-controlled power delivery system). Further, the generator 16 is capable of delivering pulsed alternating current (AC) RF energy of approximately 500 volts RMS to approximately 2000 volts RMS or more (for example, up to 3000 V). At these higher voltages, the majority of the cell damage would be due to electroporation of the target tissue 12 cells (for example, to a temperature of above 45 °C, without a substantial increase in the temperature of the electrodes 26. During electroporation, the RF energy may be delivered in multiple ON/OFF cycles in which the ON cycle only represents approximately 0.5% to approximately 1% of the total duty cycle time. These quick burst of high-voltage energy create pores in membranes of target tissue cells, but will not damage the tissue with heat. Therefore, deeper lesions may be achieved without a substantial increase in heat energy, and thus unintended damage to non-target tissue or tissue charring may be avoided. For example, the tissue surface temperature may be maintained at a temperature below 45 °C, the temperature at which irreversible unintended damage may occur. This, in turn, reduces the likelihood of potentially lethal complications (for example, the formation of micro emboli) and reduces patient discomfort.

The generator 16 may also be capable of operating at a lower voltage (for example, approximately 100 to approximately 150 volts RMS) for ablating tissue using primarily heat energy. To generate heat energy, the RF energy may be delivered in multiple ON/OFF cycles in which the ON cycle is greater than, for example, 2% of the total cycle. Tissue may be irreversibly damaged at temperatures above 45 °C; however, sub-lethal heat energy may be applied to temporarily “stun” (rather than irreversibly damage) an area of target tissue to help determine whether the area of stunned tissue is perpetuating an aberrant electrical signal involved in an arrhythmia, and therefore whether subsequent electroporation of the stunned area of tissue will block the aberrant electrical signal. Because electroporation may not result in immediate ablation of the treated tissue (that is, the treated cells may continue to

function somewhat normally for a time after electroporation) and thus immediate current blockage, it may be difficult to determine whether the correct area of tissue was electroporated. Therefore, the combination of heat energy and electroporation may result in more effective and efficient ablation.

5 The generator 16 may allow for the selection of simultaneous or selective energy delivery across electrode pairs, and may further include a user interface 32 for monitoring ablation time, electrode temperature, time at temperature, and the like. The energy output scheme of the generator 16 may be programmable independently of the console 18 via the user interface 32. Further, the generator 16 may be capable
10 of delivering an adjustable voltage so ablation may be caused using primarily heat (for example, between approximately 100 V to approximately 150 V), primarily electroporation (for example, between approximately 500V and approximately 2000 V or more), or any combination thereof (a voltage anywhere along the continuum between heat voltage and electroporation voltage). Additionally, the generator 16
15 may be programmable to manipulate characteristics of the energy output, such as the ON cycle percentage of the total duty cycle, the voltage, and the number of ON/OFF sequences. In a non-limiting example, the voltage could be adjusted to alternately ablate tissue 12 using primarily heat, primarily electroporation, or combination thereof. In an additional non-limiting example, cryoablation may be used in addition
20 to electroporation (as shown in FIG. 2), in which case the generator 16 may maintain voltage at approximately 500 to approximately 2000 volts RMS or more to cause electroporation of cells, which may complement the cryoablation. The cryoablation and RF ablation may be used either simultaneously or alternately. The temperature required for cryoablation may be lower than would normally be required to ablate
25 tissue, thus requiring lower coolant flow rates and/or volume. Still further, a second generator 34 may be used if microwave, laser, or ultrasound energy is also used. Thus, the user may have very precise control over the treatment process.

Continuing to referring to FIGS. 1 and 2, the console 18 may be used to control the temperature of one or more components of the medical device 14 during
30 operation of the system 10. The console 18 may include a power source 35, a computer 36 in communication with other system 10 components (such as the plurality of electrodes 26, one or more sensors 29, and/or generator 16) and having

one or more screens or displays 38 with which the user may monitor and/or adjust system 10 parameters. Additionally or alternatively, the computer 36 may be programmed to automatically adjust such parameters as voltage delivered by the generator 16, coolant volume and flow delivered from a coolant source 40 (as shown in FIG. 2), and effective temperature of the one or more treatment elements based at least in part on signals received from the one or more sensors 29. Further, temperature regulation may be achieved through the implementation of one or more active thermal elements coupled to the medical device 14 and/or in communication with the computer 36, such as one or more cooling components (such as subcoolers, Peltier coolers, Joule-Thompson coolers, Stirling engine, or the like) and/or active heat sources (such as heating elements, immersion heaters, circulation heaters, or other devices for warming fluids or gases). If the system 10 is configured for cryoablation, the system 10 may include not only a coolant source 40, but a coolant return reservoir and vacuum pump as well, and the device 14 may include a fluid injection lumen, a fluid return lumen, a fluid injection element, and the like.

Referring now to FIGS. 3A and 3B, the distal portion 24 of the medical device 14 may include a plurality of electrodes 26, with each electrode being capable of operating out of phase from one or more adjacent electrodes. This allows for the device 14 to operate in unipolar mode, bipolar mode, or combination thereof. Further, this mode selection may be used in conjunction with the voltage selection, thereby making possible a wide variety of treatment effects. As shown in FIGS. 3A and 3B, the distal portion 24 may include four electrodes 26A, 26B, 26C, 26D, although it is understood that any number or configuration of electrodes may be used, such as an array or mesh including a plurality of electrodes.

All four electrodes may be activated to apply energy at 1000 V RMS in bipolar mode (as shown in FIG. 3A). As a non-limiting example, electrode 26A may apply energy at 1000 V at 0°, electrode 26B may apply energy at 1000 V at 180° out of phase from electrode 26A, electrode 26C may apply energy at 1000 V at 0° (same phase as electrode A), and electrode 26D may apply energy at 1000 V at 180° out of phase from electrode 26C. In this case, the energy applied between any two electrodes would be twice the voltage applied by either electrode (*e.g.*, 2000 V RMS). However, using a different phase angle would create a different combined voltage.

For example, If electrodes 26A and 26C apply energy at 1000 V at 0° and electrodes 26B and 26D apply energy at 1000 V at 90°, the combined voltage between electrodes 26A and 26B (or any combination of adjacent electrodes) would be approximately 1400 V RMS (or approximately 1.414 times 1000 V). Similarly, a 60° shift would

5 result in a combined voltage between electrodes 26A and 26B (or any combination of adjacent electrodes) of 1000 V (creating no increased effect). In fact, any phase angle between 0° and 180° could be used to create the desired combined voltage between electrodes. Further, the amount of voltage delivered to the target tissue also depends on the distance between electrodes. For example, if electrodes 26A and 26B deliver a

10 combined voltage of 1000 V and the electrodes are spaced 10mm apart, each mm of tissue between the electrodes would receive 100 V. Alternatively, the electrodes may be activated to apply energy in unipolar mode, with no phase difference between electrodes (as shown in FIG. 3B). Therefore, the multi-electrode device 14 is capable of creating a contiguous lesion 42 when operating in bipolar mode or creating discrete

15 lesions 44 when operating in unipolar mode. Thus, the effective voltage applied to the tissue may be manipulated by phase shift in bipolar mode and voltage delivered to each electrode (in either unipolar mode or bipolar mode), calculated as a function of the distance between electrodes. Further, as discussed above, the device 14 may be used to ablate tissue using either thermal energy, electroporation, or a combination

20 thereof. Still further, the device 14 may be used to ablate using electroporation and another energy modality (such as cryoablation) simultaneously.

Referring now to FIG. 4, a flow chart of a method of ablation using electroporation and heat energy is shown. It will be understood that cryoablation is included herein as an “energy modality,” even though cryoablation involves the

25 removal of heat from tissue. The method of FIG. 4 generally includes positioning a medical device 14 proximal to an area of target tissue 12, determining the method with which the target tissue 12 will be ablated, activating one or more treatment elements, and adjusting an energy generator as necessary to ablate the target tissue 12. Step 1 includes positioning a medical device 14 proximal to an area of target tissue

30 12. As non-limiting examples, the target tissue may be cardiac, (such an endocardial or epicardial tissue), liver, pancreatic, renal, or tumor tissue. In fact, the target tissue 12 may be any biological tissue in which electroporation would create pores within

the tissue cellular membranes and in which irreversible electroporation would cause cell death.

In Step 2 of FIG. 4, the treatment elements are placed in contact with the target tissue 12. For example, if cryoablation is used in addition RF energy (for electroporation), the balloon 27 and plurality of electrodes 26 should be placed in
5 contact with the target tissue 12. In Step 3, the method with which the target tissue 12 will be ablated is determined. For example, if only electroporation is desired, the generator 16 may be programmed to deliver energy at between approximately 500 and approximately 2000 V or greater (for example, 3000 V; “electroporation voltage”) to
10 all of the plurality of electrodes 26. If the user desires to ablate the target tissue 12 using only heat energy or cryoablation, the generator 16 may be programmed to deliver energy at between approximately 100 to approximately 150 volts RMS (“ablation voltage”) to all of the plurality of electrodes 26 and/or the flow of coolant initiated. If the user desires to ablate the target tissue 12 using a combination of
15 electroporation and heat energy (and/or cryoablation), the generator may be programmed to deliver energy at a desired voltage anywhere along the continuum between electroporation voltage and heat voltage. This may be accomplished by adjusting the output voltage from the generator 16 or adjusting the phase angle between adjacent electrodes. Or, electroporation voltage to some electrodes 26 and
20 ablation voltage to some electrodes 26. Or, the voltage level output by the plurality of electrodes and/or duration of energy application may be adjusted such that the tissue 12 is ablated by both heat and electroporation. Thus, each activated electrode 26 may receive either electroporation voltage or ablation voltage; some electrodes may not receive voltage at all (that is, may not be activated). Or, each activated electrode 26
25 may receive a voltage that effects both electroporation and heat ablation. Further, the generator 16 may be programmed to deliver heat voltage followed by electroporation voltage to all electrodes 26, such as when testing an area of tissue with heat energy to determine if electroporation of that tissue will effectively block an aberrant electrical current. Therefore, the generator 16 may be programmed to deliver heat energy,
30 electroporation energy, or any combination thereof to the plurality of electrodes 26 as desired (Steps 4A and 4B). Still further, the generator 16 may be programmed to deliver energy in unipolar mode, bipolar mode, or combination thereof.

In Step 5 of FIG. 4, system 10 and tissue 12 parameters may be monitored. During ablation, one or more sensors 29, such as temperature sensors, may measure the temperature of the tissue surface. If the temperature sensors detect a tissue temperature that is above a threshold temperature (for example, 45 °C), the system 10 may be adjusted manually by the user or the energy generator 16 and/or the computer 36 may be programmed to automatically adjust voltage, coolant flow, effective temperature of treatment elements, and/or other system 10 parameters to ensure unintended tissue damage does not occur (Step 6). Additionally, the medical device 14 may include one or more electrical conductivity sensors, which may provide mapping functionality and/or detect the status of the target tissue 12. For example, based at least in part on electrical conductivity measurements, the user and/or system 10 may determine whether the target tissue 12 has been ablated (Step 6B). If the target tissue 12 has not been satisfactorily ablated, the system 10 may likewise be adjusted manually by the user or the energy generator 16 and/or the computer 36 may be programmed to automatically adjust voltage, coolant flow, operating mode, effective temperature of treatment elements, and/or other system 10 parameters to ensure complete ablation of the target tissue 12 (Step 6).

After completion of Steps 1-6, the target tissue 12 is ablated. In Step 7 of FIG. 4, the catheter 14 may be removed from the area of target tissue 12.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described herein above. In addition, unless mention was made above to the contrary, it should be noted that all of the accompanying drawings are not to scale. A variety of modifications and variations are possible in light of the above teachings without departing from the scope and spirit of the invention, which is limited only by the following claims

What is claimed is:

1. A medical system, comprising:

a medical device including a plurality of electrodes;

a radiofrequency energy source in communication with the plurality of electrodes, the radiofrequency energy source being configured to produce sub-lethal thermal energy and non-thermal electroporation energy, the non-thermal electroporation energy being high-frequency alternating current radiofrequency energy; and

a computer being in communication with the radiofrequency energy source, the computer being configured to:

thermally treat tissue by transmitting the sub-lethal thermal energy from the radiofrequency energy source through the plurality of electrodes to stun the tissue;

determine whether the transmission of the sub-lethal thermal energy from the radiofrequency energy source affects a perpetuation of an aberrant electrical signal within a heart; and

when the computer determines that the transmission of the sub-lethal thermal energy from the radiofrequency energy source affects the perpetuation of the aberrant electrical signal within the heart, non-thermally electroporate the tissue by transmitting the high-frequency alternating current radiofrequency energy from the radiofrequency energy source through the plurality of electrodes,

the transmission of energy through each of the plurality of electrodes being at at least one of an in-phase angle and an out-of-phase angle relative to the energy transmitted through adjacent electrodes.


2. The system of Claim 1, wherein the medical device is further configured to reduce the temperature of the tissue to a temperature at which cryoablation occurs.

3. The system of Claim 1, wherein the non-thermal electroporation is irreversible.

4. The system of Claim 3, wherein the radiofrequency energy has a frequency of between approximately 20 kHz and approximately 1MHz.

5. The system of Claim 4, wherein the computer is configured to transmit the radiofrequency energy between approximately 500 volts RMS and approximately 3000 volts RMS.

6. The system of Claim 1, wherein the computer is configured to apply a voltage at which heat ablation occurs to target tissue cells before applying a voltage at which the non-thermal electroporation occurs.
7. The system of Claim 1, wherein the energy transmitted through each of the plurality of electrodes is at an out-of-phase angle between adjacent electrodes, the out-of-phase angle being determined at least in part by a desired voltage to be applied to the tissue.
8. The system of Claim 1, wherein the computer is further configured to maintain a surface temperature of the tissue below a threshold temperature at which unintended tissue damage occurs.
9. The system of Claim 1, wherein the plurality of electrodes are in communication with a radiofrequency generator, the generator being programmable to:
- deliver energy in at least one of bipolar mode and a combination of unipolar mode and bipolar mode;
 - deliver alternating current radiofrequency energy from the medical device at between approximately 500 volts RMS to approximately 3000 volts RMS to an area of target tissue;
 - deliver alternating current radiofrequency energy from the medical device at between approximately 100 volts RMS to approximately 150 volts RMS to the area of target tissue; and
 - deliver alternating current radiofrequency energy from the medical device at a voltage between approximately 150 volts RMS and approximately 500 volts RMS to the area of target tissue.
10. The system of Claim 9, wherein the energy delivered to each of the plurality of electrodes is at an out-of-phase angle between adjacent electrodes, the out-of-phase angle being determined at least in part by a desired voltage to be applied to the target tissue.

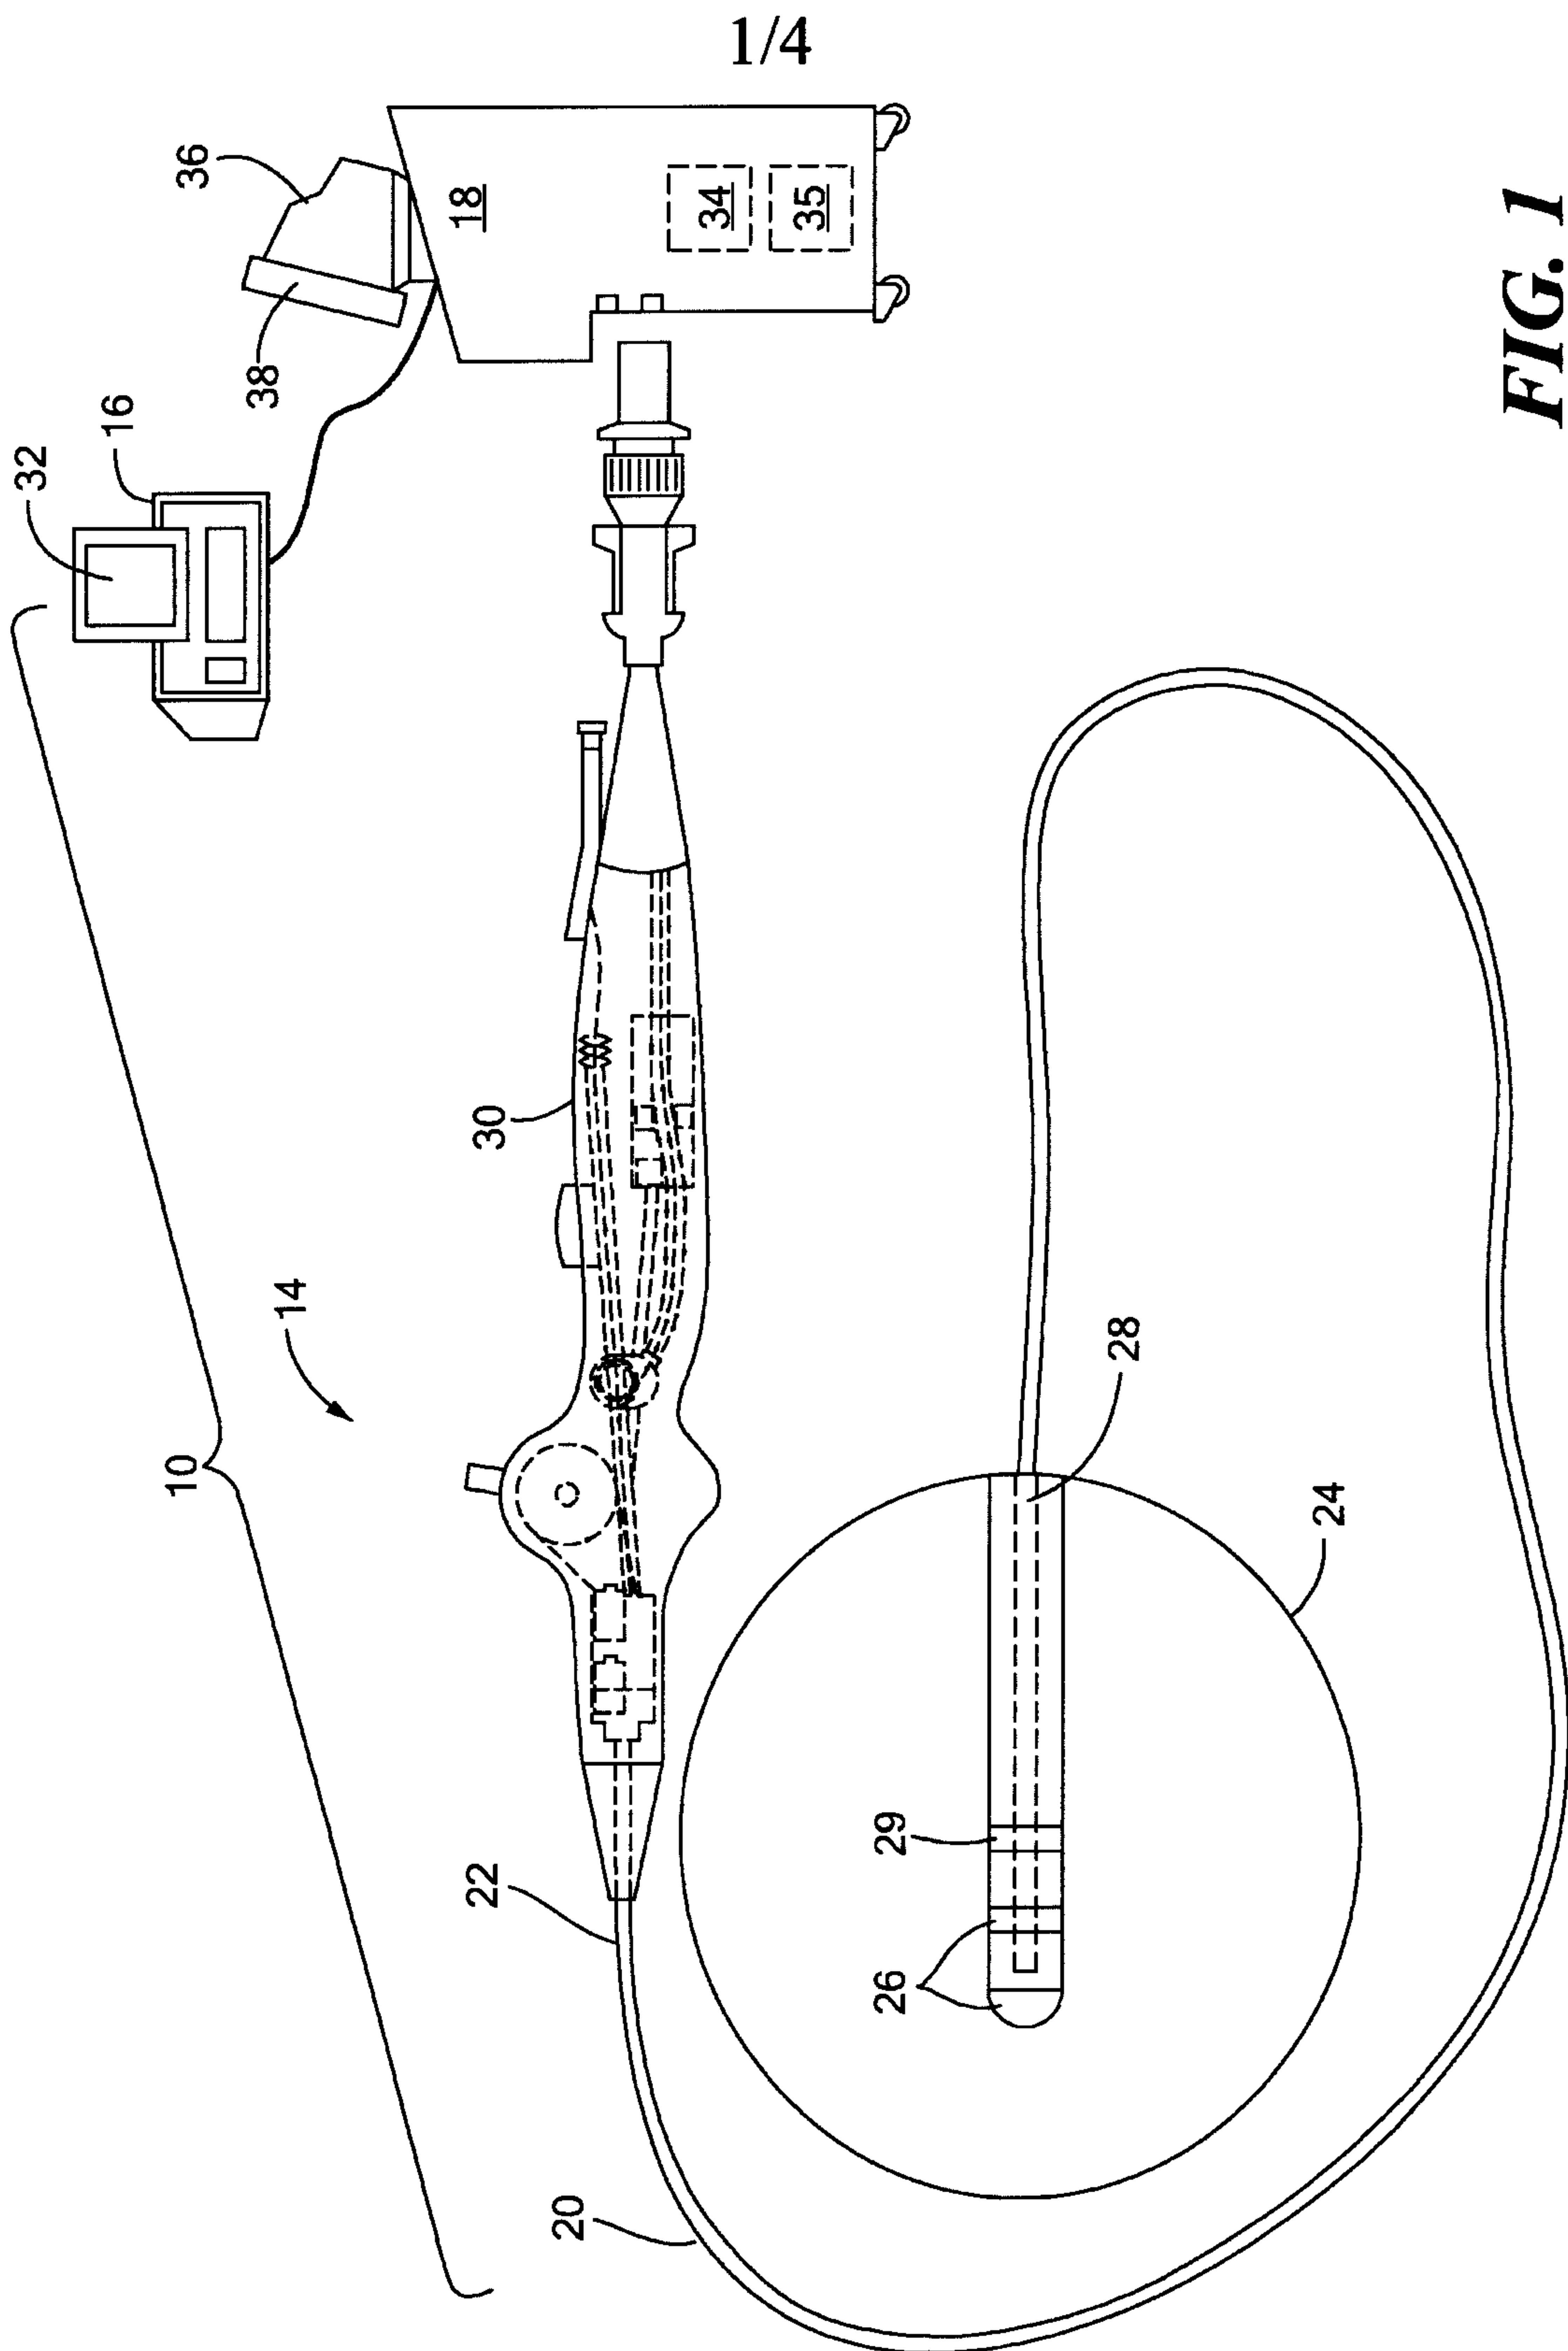

2/4

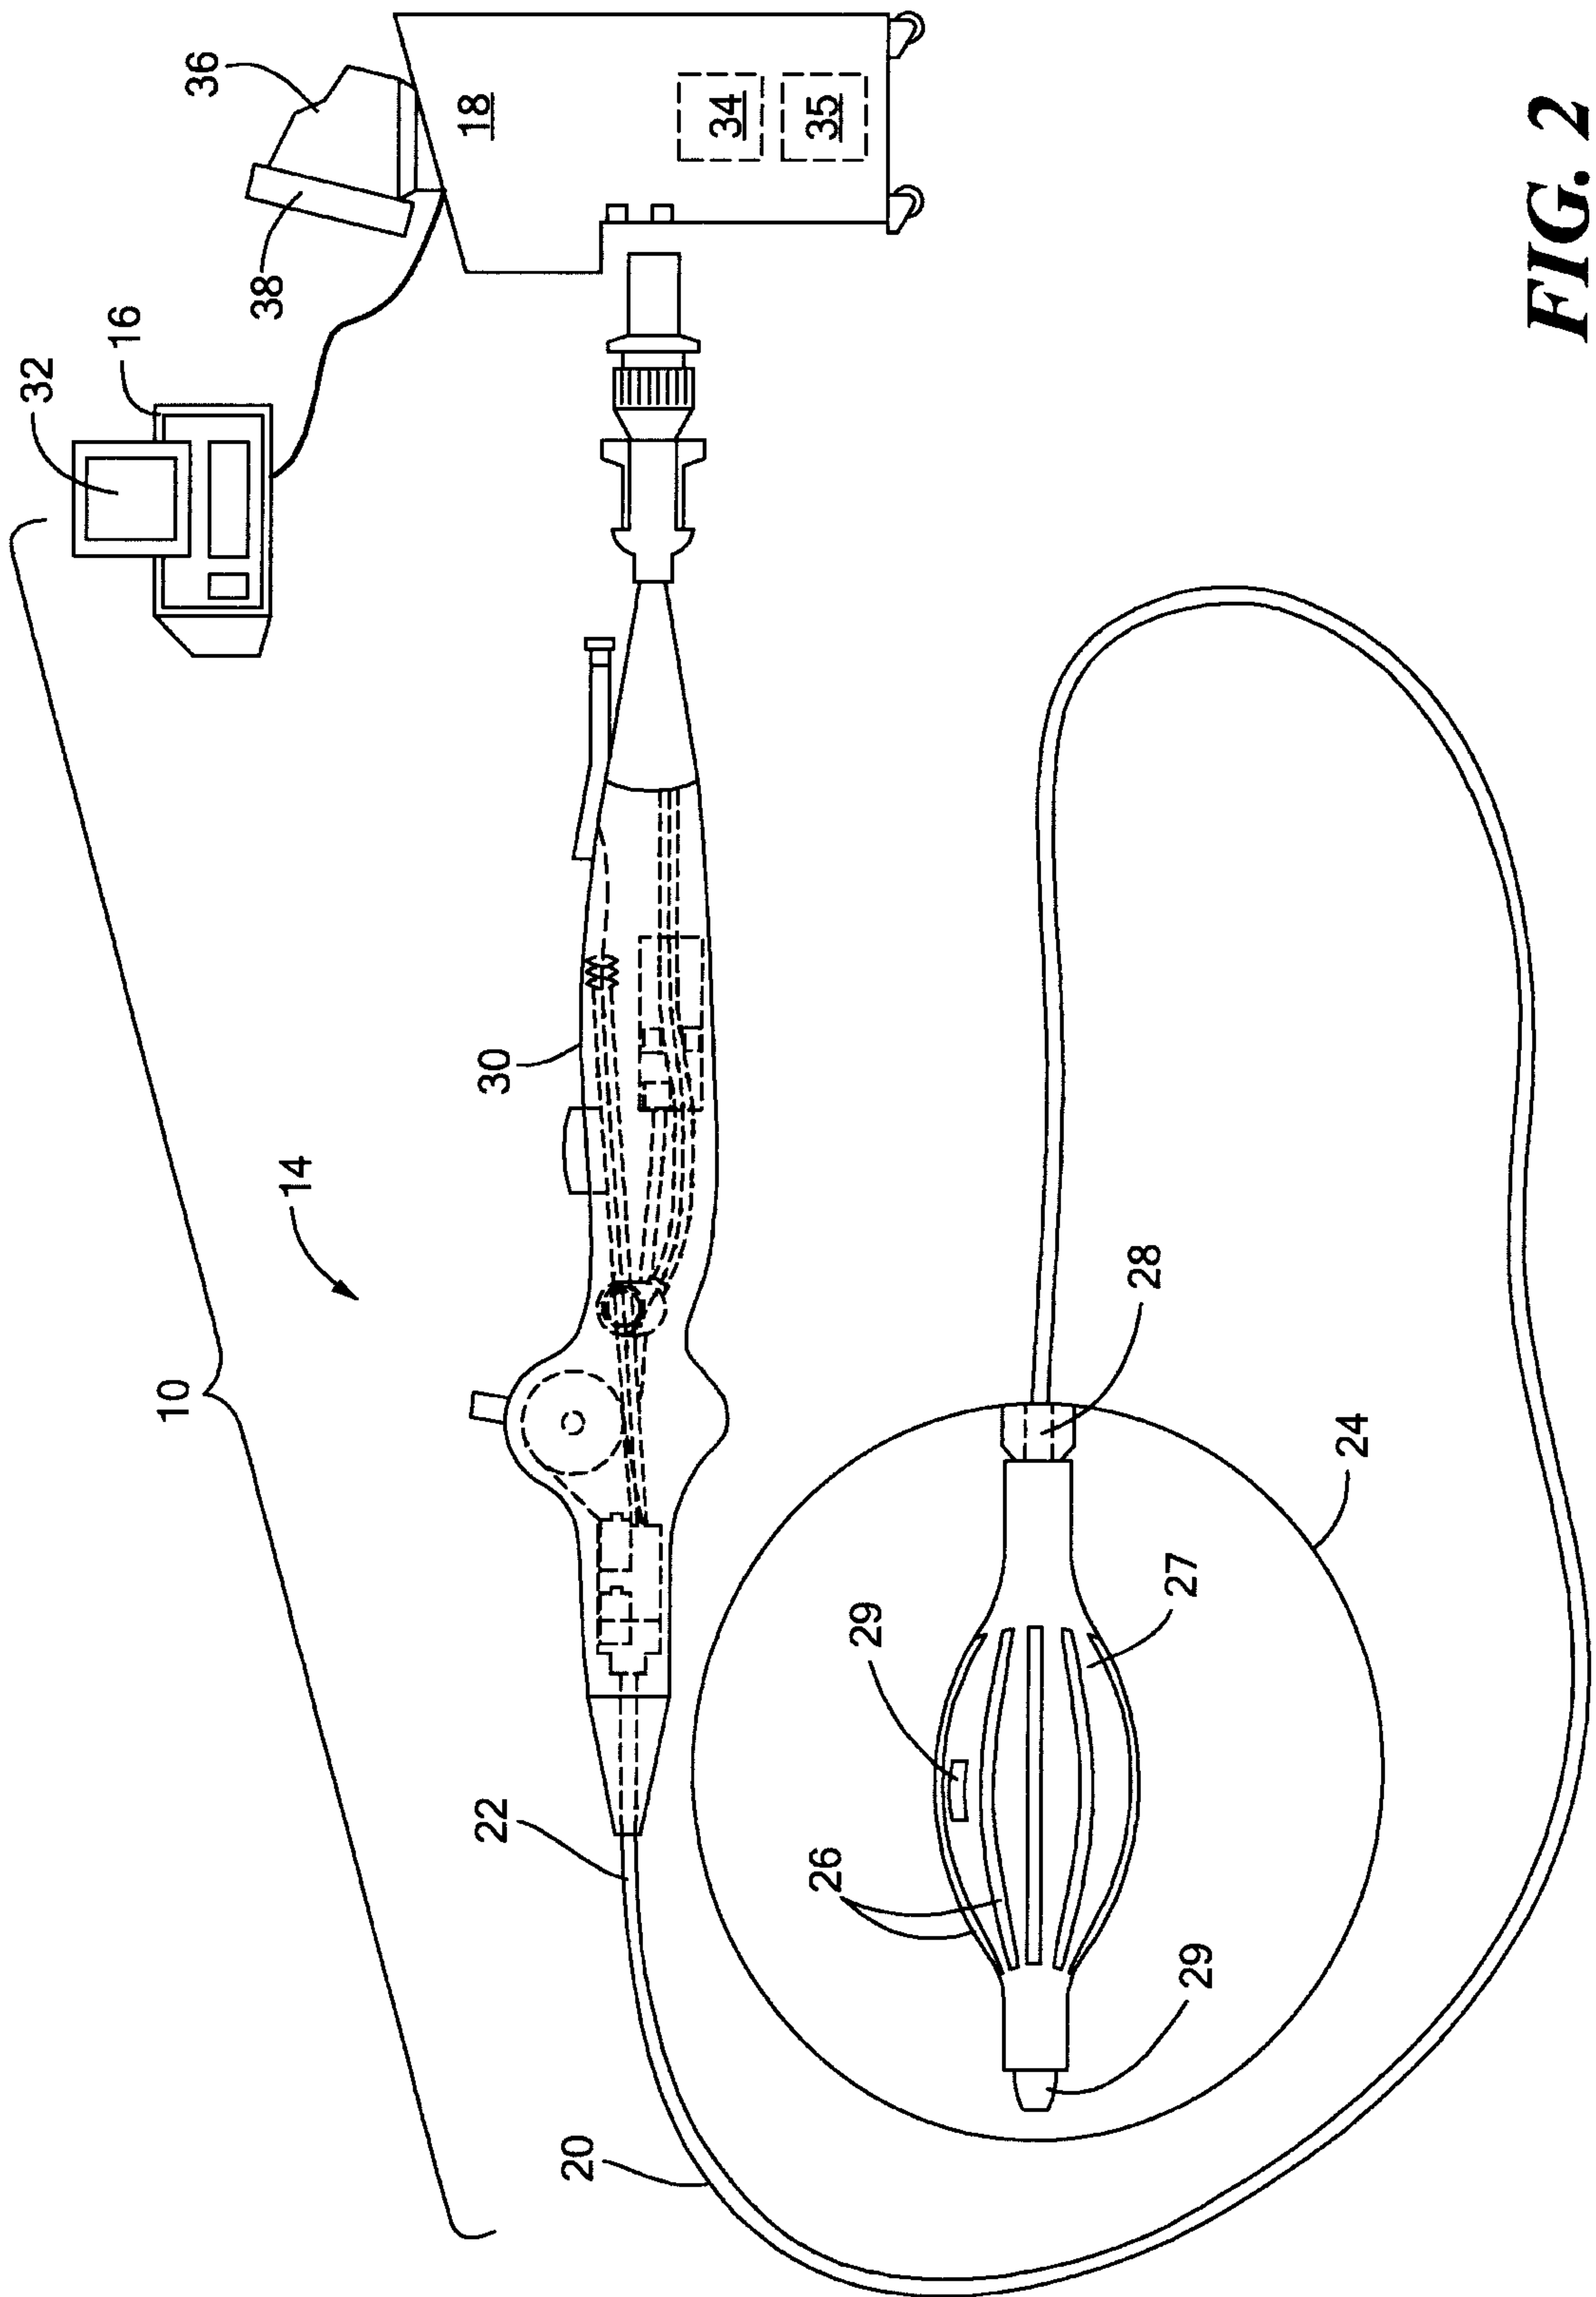
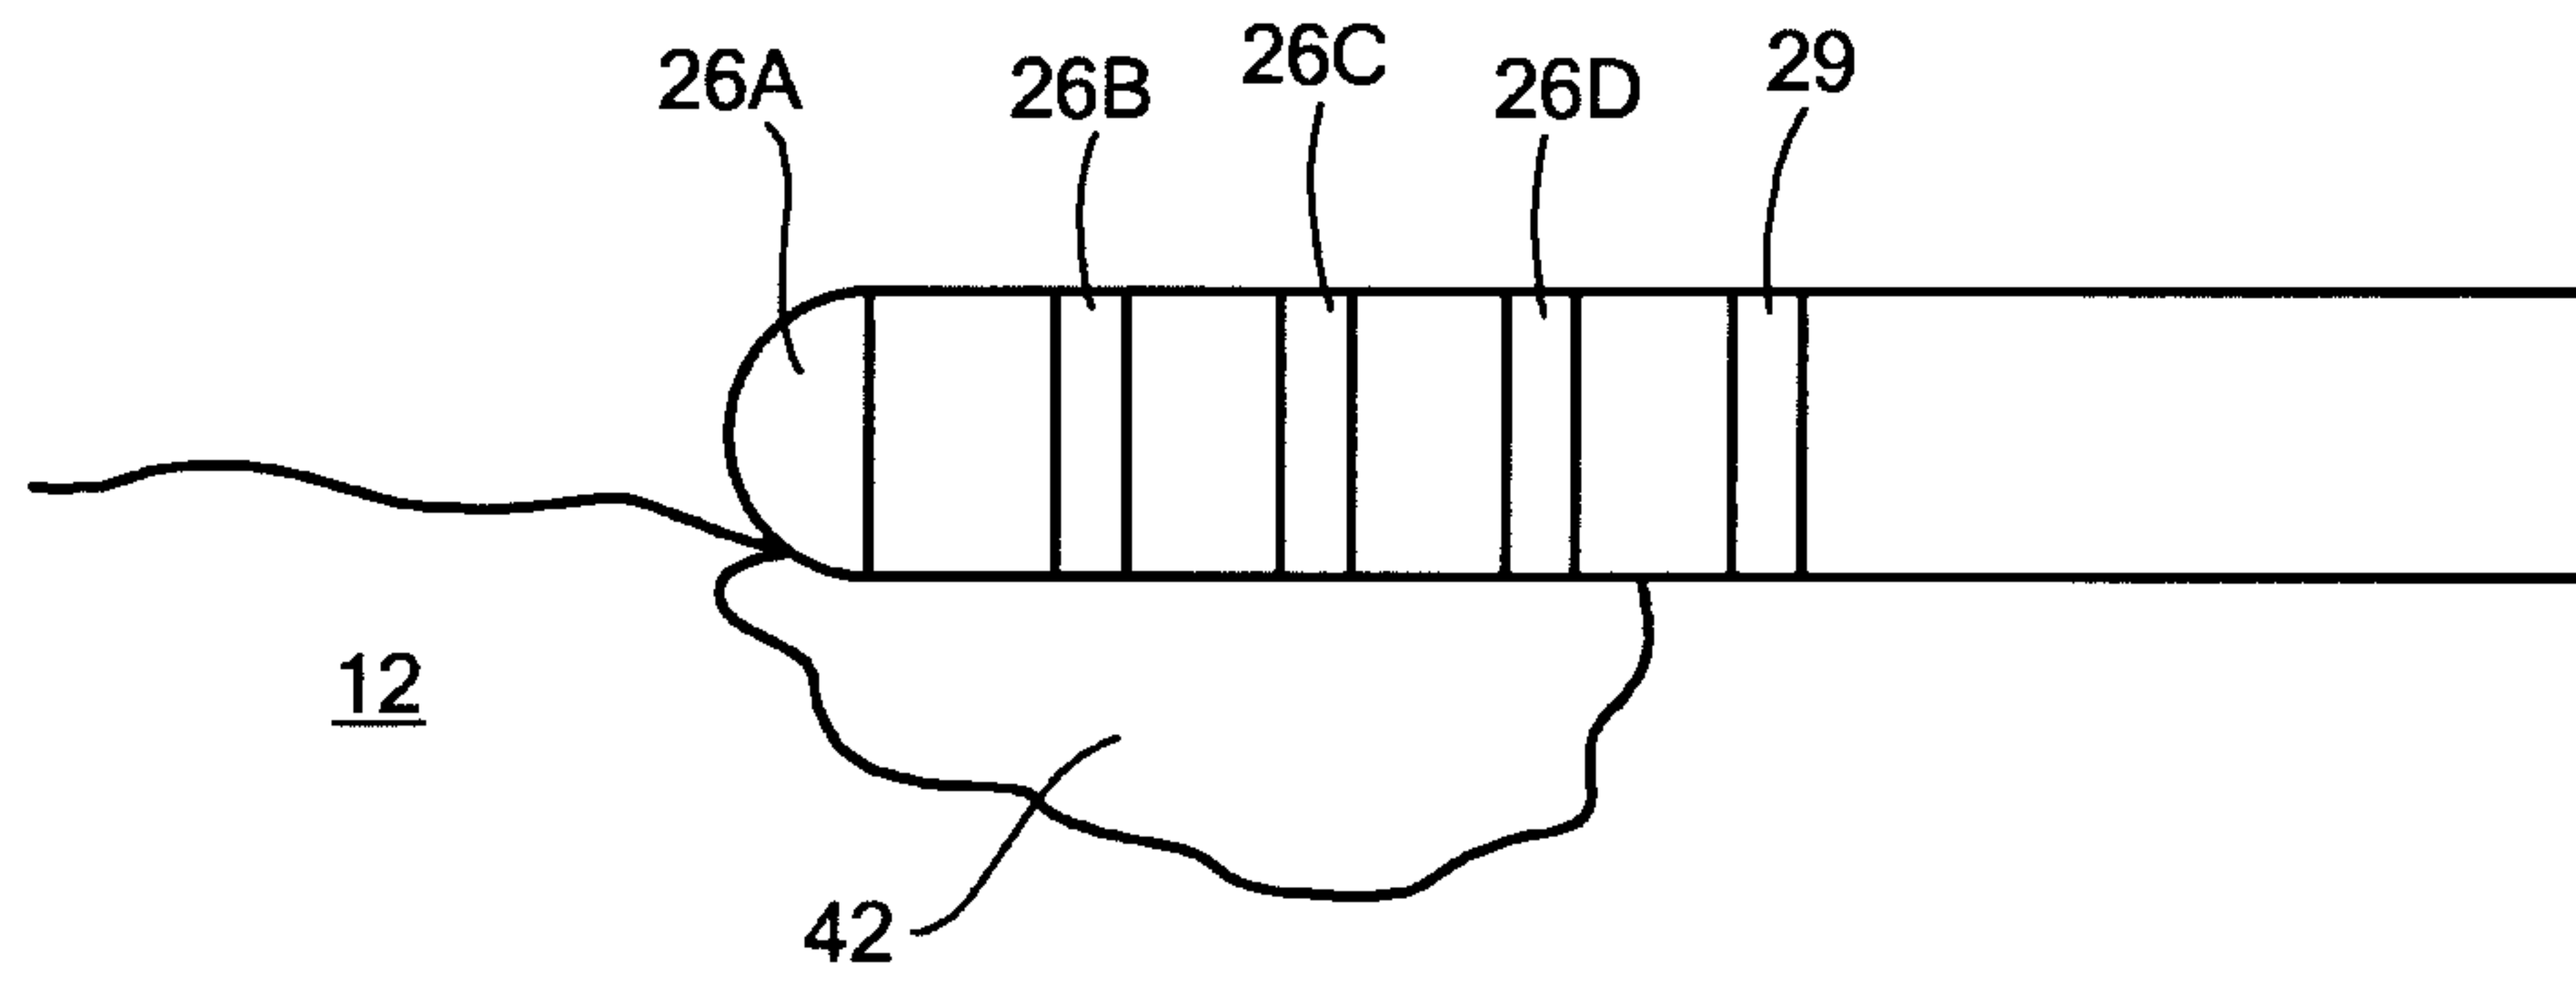
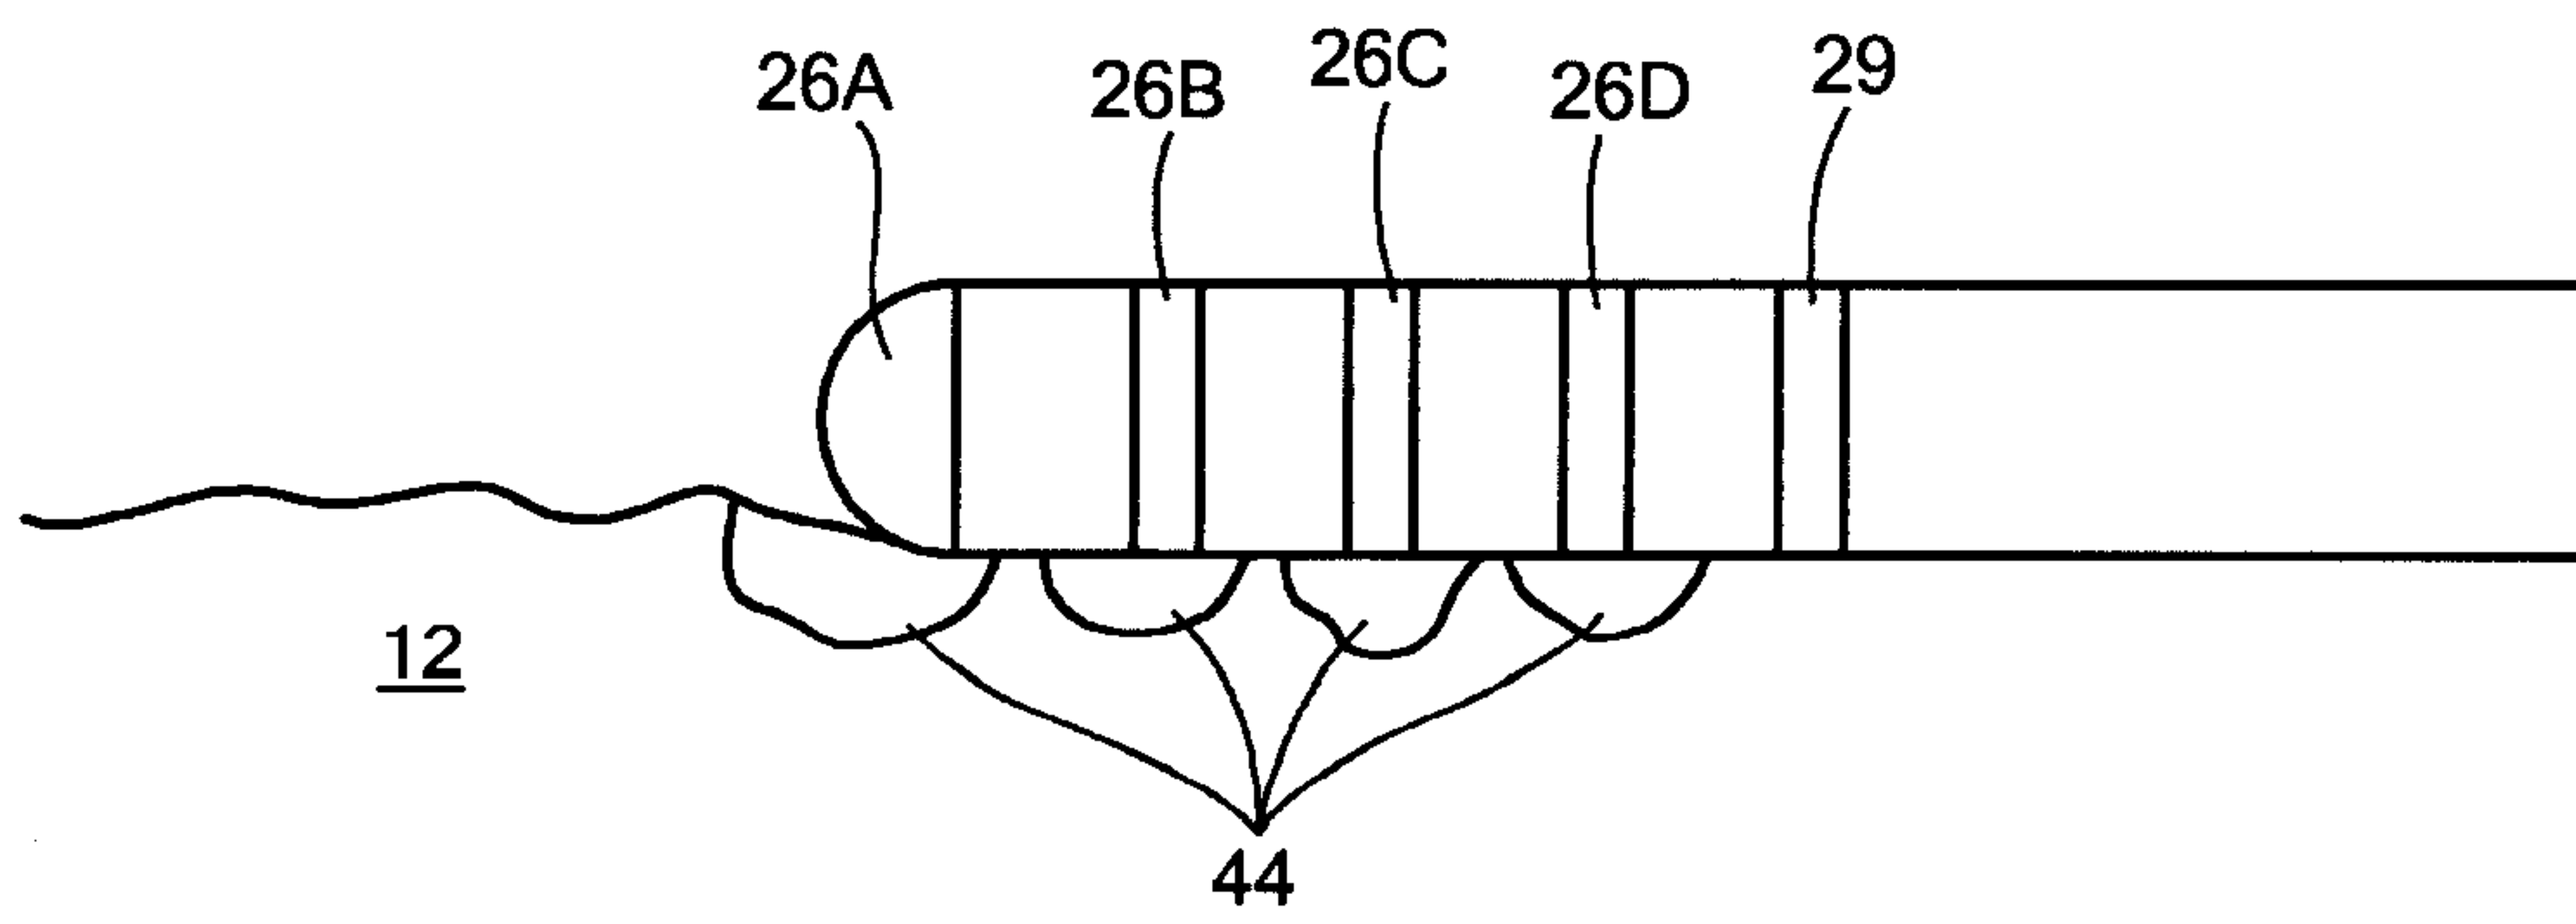
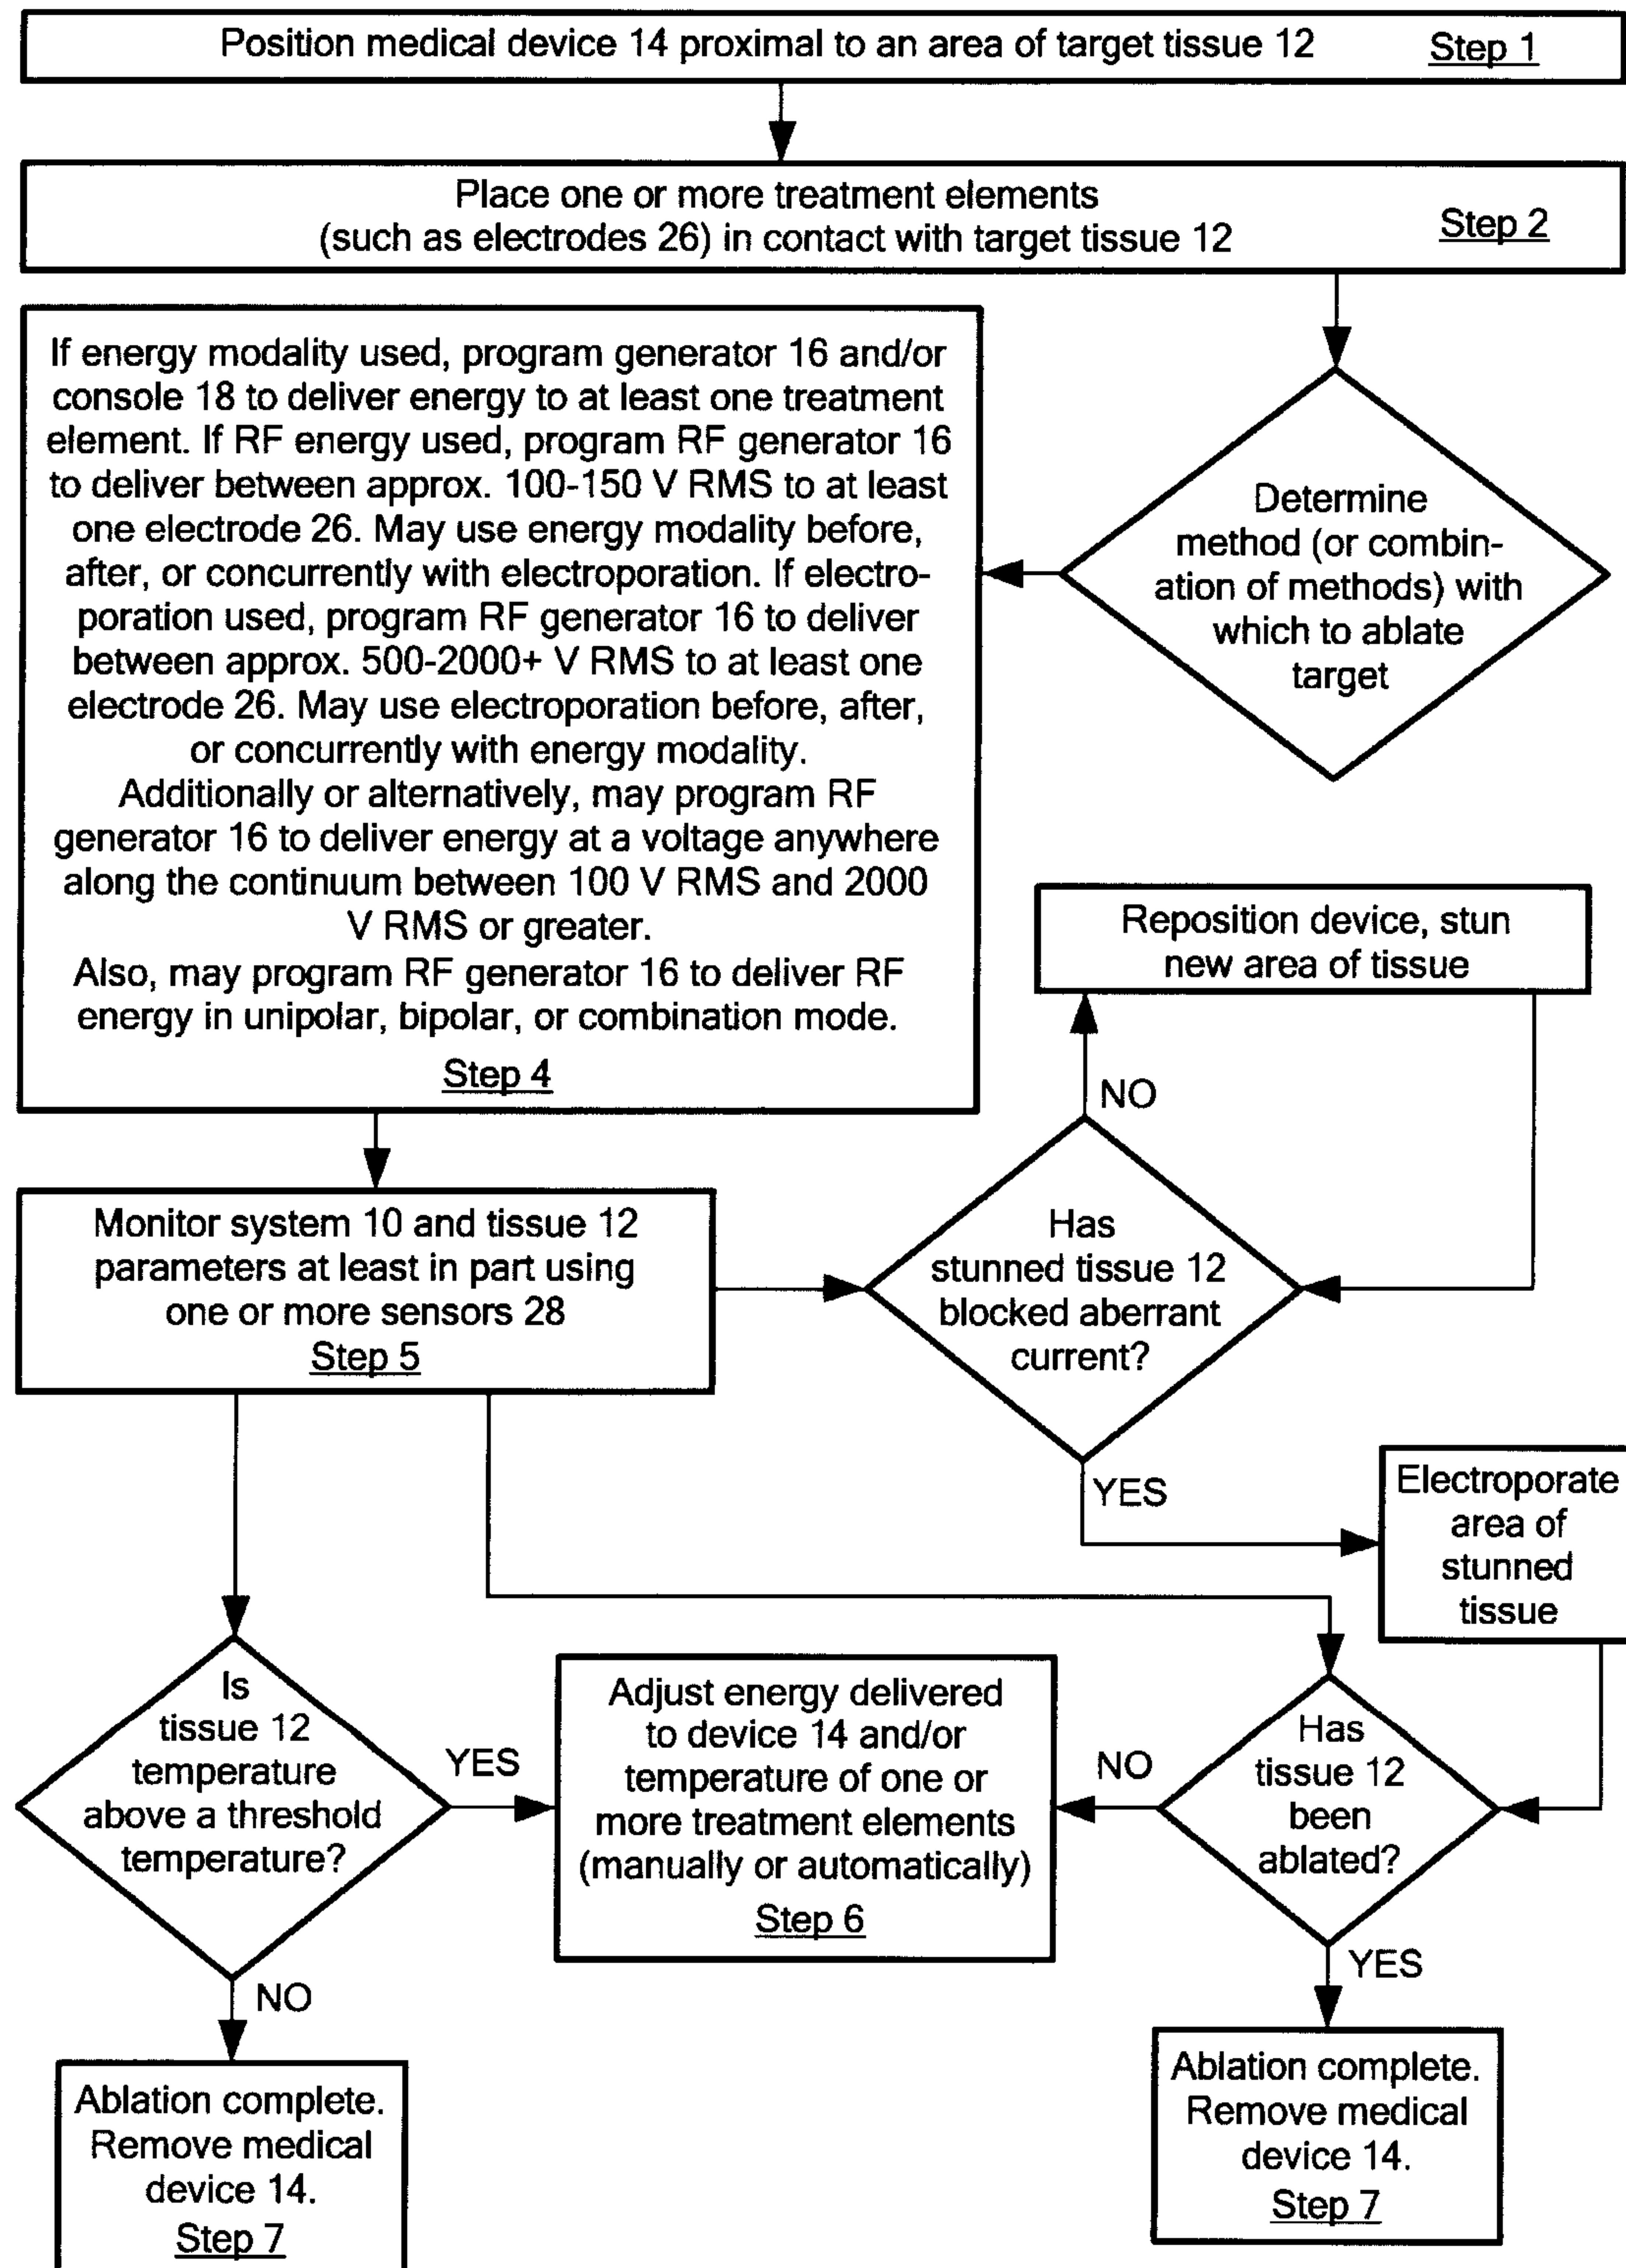


FIG. 2

3/4

**FIG. 3A****FIG. 3B**

4/4

**FIG. 4**

