




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification ⁶ : A61B 8/12</p>	<p>A1</p>	<p>(11) International Publication Number: WO 96/00522</p> <p>(43) International Publication Date: 11 January 1996 (11.01.96)</p>
<p>(21) International Application Number: PCT/US95/07756</p> <p>(22) International Filing Date: 14 June 1995 (14.06.95)</p> <p>(30) Priority Data: 08/267,318 28 June 1994 (28.06.94) US</p> <p>(71) Applicant: ACUSON CORPORATION [US/US]; 1220 Charleston Road, Mountain View, CA 94039 (US).</p> <p>(72) Inventors: HOSSACK, John, A.; Apartment E, 144 Emmerson Street, Palo Alto, CA 94301 (US). JACKSON, John, I.; 941 Laurel Avenue, Menlo Park, CA 94025 (US). EATON, John, W.; 1150 Guinda Street, Palo Alto, CA 94301 (US). COOPER, Thomas, Grosvenor; 304 Concord Drive, Menlo Park, CA 94025 (US).</p> <p>(74) Agent: SAMPSON, Matthew, J.; Willian Brinks Hofer Gilson & Lione, NBC Tower - Suite 3600, 455 North Cityfront Plaza Drive, Chicago, IL 60611-5599 (US).</p>		<p>(81) Designated States: AM, AT, AU, BB, BG, BR, BY, CA, CH, CN, CZ, DE, DK, EE, ES, FI, GB, GE, HU, IS, JP, KE, KG, KP, KR, KZ, LK, LR, LT, LU, LV, MD, MG, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TT, UA, UZ, VN, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG), ARIPO patent (KE, MW, SD, SZ, UG).</p> <p>Published <i>With international search report.</i></p>

(54) Title: ULTRASONIC TRANSDUCER PROBE WITH AXISYMMETRIC LENS

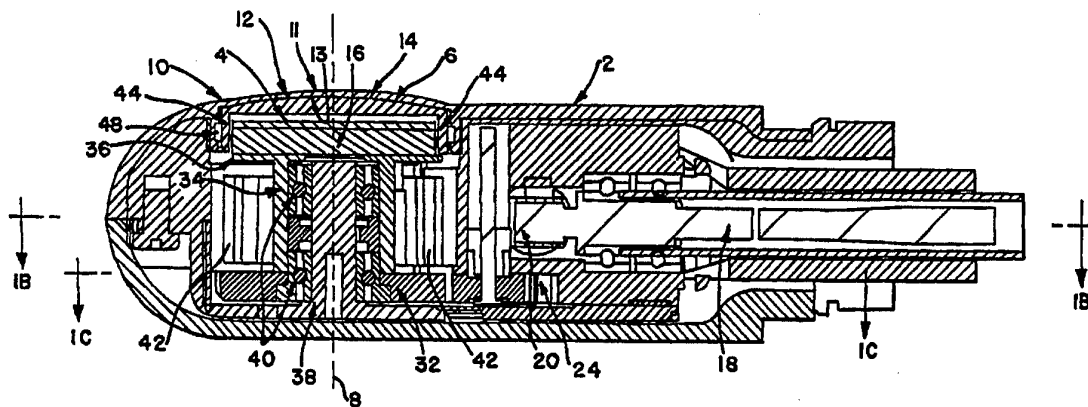

(57) Abstract

According to the present invention, an ultrasonic transducer probe is provided having an array (4) of ultrasonic transducers rotatably mounted about an axis within the ultrasonic transducer probe, a lens (6) mounted to the array (4), and a housing (2) encasing the array and the lens. The lens (6) is symmetric about the axis of rotation (8) of the array. In addition, the housing has a continuous upper surface that is formed in a region adjacent to the symmetric lens (6) to mate with the symmetric lens.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgystan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

- 1 -

**ULTRASONIC TRANSDUCER PROBE
WITH AXISYMMETRIC LENS**

BACKGROUND OF THE INVENTION

5 The invention relates to ultrasonic imaging systems, and more particularly to systems that utilize an acoustic lens to focus ultrasonic energy.

10 The users of medical ultrasonic transducer probes, hereinafter referred to as sonographers, can obtain images of a region within a body by properly positioning a probe against the body. In order to obtain images having diagnostic value, the sonographer may have to physically manipulate the position of the probe by sliding, rotating, and tilting the probe. One area in particular where this manipulation is more
15 challenging is transesophageal cardiac imaging. During transesophageal cardiac imaging, the sonographer positions a transducer housing at the tip of the probe against the esophagus or stomach of a patient in order to obtain different fields of view of the heart.

20 Typically for this application, the transducer housing contains a number of acoustic transducer elements, which may be sequentially electrically excited by an ultrasound control and operating system to obtain an image in an object plane that is perpendicular to the transducer housing and the transducer
25 elements. It has been found desirable to rotate the transducer elements contained within the transducer housing independently from the physical manipulation of

- 2 -

the housing itself. In combination with the ability to slide, rotate and tilt the transducer housing, the ability to independently rotate the transducer elements within the housing gives the sonographer the ability to obtain an ultrasonic image of any or all object planes orthogonal to the upper surface of the transducer elements at each location to which the housing can be moved.

Because the transducer housing on this type of probe may be placed within the body of the patient being examined, it must be sealed to protect against the ingress of bodily fluids, sterilant solutions, and cleaning solutions. The seal may also prevent moving parts, such as the rotating transducer elements, from contacting the body of the patient.

The acoustic energy radiated from the transducer housing may be focused by mounting an acoustic lens to the transducer elements within the housing. A cylindrical lens, which does not vary in thickness along the azimuthal direction, is sometimes used to provide a fixed focus to the transducer array in the elevation direction.

Devices are known that utilize a cylindrical lens. For example, U.S. Patent No. 5,127,410 to King et al. includes a compound lens secured on top of a rotatable transducer. The compound lens may have a convex cylindrical lens of a first material mated to a concave lens of a second material. The second material has substantially the same acoustic properties as the body being scanned. The concave portion of the compound lens is shaped so that the upper surface of the compound lens is flat. The flat upper surface of the compound lens is mated to a flat lens assembly that seals an opening in the transducer housing. The opening is sealed, for example by a thin plastic film that is bonded to the housing in the area around the

- 3 -

opening. A backing layer is formed to the plastic film and an RFI screen is embedded in the backing layer. A grease layer lubricates the interface between the flat upper surface of the compound lens and the flat lens assembly that seals the transducer housing.

A disadvantage of the King device is that a number of material layers are added to the top of the transducer elements, which can cause degraded performance due to attenuation within the layers or reflections at the material interfaces giving rise to reverberation artifacts in the resultant image. In addition, the concave lens may be difficult to fabricate. Few solid materials possess the acoustic properties required of the concave lens, and those materials that do possess the required properties may not adhere to the convex lens material and may absorb certain grease or oil materials causing the concave lens to expand. Expansion of the concave lens may lead to distortion of the transducer housing's component parts, unreliability, and a reduction in image quality. Furthermore, the added process steps in fabricating and assembling each material layer may decrease yield.

A further disadvantage of the King device is that the compound lens may require more space within the transducer housing than would a simple lens. It is desirable to minimize the size of the transducer housing so that it may be easily inserted by the sonographer and manipulated within the body of the patient without causing excessive patient discomfort.

A further disadvantage of the King device is that the flat lens assembly that seals the opening in the transducer housing may deform or make poor contact with the body of the patient upon application of pressure by the sonographer. It is desirable to maintain acoustic contact with the body of the patient because the presence of any gaps between the transducer

- 4 -

housing and the patient will seriously degrade performance.

5 A still further disadvantage of the King device is that additional process steps are required to seal the opening in the housing and the seal may introduce additional material layers between the transducer elements and the body of the patient. As noted above, it is desirable to minimize the number of material layers between the transducers and the patient and to minimize processing steps in constructing the transducer housing.

10 Accordingly, it would be desirable to have an improved ultrasonic transducer probe.

SUMMARY OF THE INVENTION

15 According to a first aspect of the present invention, an ultrasonic transducer probe is provided having an array of ultrasonic transducers mounted within the ultrasonic transducer probe, a lens mounted to the array, and a housing encasing the array and the lens. The housing has a continuous surface adjacent to the lens.

20 According to a second aspect of the present invention, an ultrasonic transducer probe is provided having an array of ultrasonic transducers rotatably mounted about an axis within the ultrasonic transducer probe, a lens mounted to the array, and a housing encasing the array and the lens. The lens is symmetric about the axis of rotation of the array. In addition, the housing has a continuous upper surface that is formed, in a region adjacent to the symmetric lens, to mate with the symmetric lens.

25 According to a third aspect of the present invention, an ultrasound system for providing diagnostic information from the interior of a body is provided having an ultrasonic transducer probe, an operating and

30

35

- 5 -

control system for processing electrical signals produced by the ultrasonic transducer probe, and means for operatively coupling the ultrasonic transducer probe to the operating and control system.

5 The transducer probe has an array of ultrasonic transducers, an axisymmetric lens mounted to the array, and a housing encasing the array and the lens. The housing has a continuous surface adjacent to the lens.

10 According to a fourth aspect of the present invention, a method of providing diagnostic information from the interior of a body is provided having the steps of providing an ultrasound system having transmitting electronics, receiving electronics, an array of
15 ultrasonic transducer elements and an axisymmetric lens attached to the array, storing values corresponding to a propagation time through the axisymmetric lens and an angle of refraction at an interface between the lens and the body for a set of acoustic lines, adjusting the
20 transmitting electronics and the receiving electronics in accordance with the stored values, and transmitting acoustic pressure waves into the body and receiving acoustic echoes from the body through the axisymmetric lens on the set of acoustic lines.

25 BRIEF DESCRIPTION OF THE DRAWINGS

 Figures 1A through 1C are sectional views of a transducer probe in accordance with the present invention.

30 Figure 2 is an isometric view of an upper surface of a transducer housing of the probe of Figure 1.

 Figure 3 is a sectional view along the azimuthal axis of an ultrasonic transducer array and a lens as shown in the probe of Figure 1.

- 6 -

Figure 4 illustrates an image plane formed by scanning a transducer array in a variable vertex format.

5 Figures 5A and 5B illustrate an acoustic scan line emanating from a vertex and propagating through a constant sound velocity medium and an axisymmetric lens, respectively.

DETAILED DESCRIPTION OF THE PRESENTLY PREFERRED EMBODIMENTS

10 The present invention is best understood by reference to the embodiments shown in Figures 1 to 5 where like elements are referred to by like numerals. Figure 1A shows a transducer housing 2 containing a rotating transducer array 4. A lens 6 is positioned adjacent to the transducer array 4. Preferably, the lens 6 is symmetric about an axis of rotation 8 of the transducer array 4. Lenses having the property of being symmetric about an axis of rotation are referred to herein as axisymmetric lenses. Parabolic lenses, 15 spherical lenses, and hyperbolic lenses are examples of axisymmetric lens.

20 As shown in Figures 1A and 2, the transducer housing 2 has a continuous surface 10 adjacent to the axisymmetric lens 6. In the region of the housing 2 that is adjacent to the lens 6, the continuous surface 10 of the transducer housing 2 is formed into a window 12. The window 12 mates to the shape of the lens 6. Preferably, the window 12 is integrally formed with the transducer housing 2, as shown in Figures 1 and 2. In the embodiment shown in Figure 1, the radii of curvature of the window 12 match the radii of curvature of the axisymmetric lens 6.

25 A thin layer of a grease 14 fills an interface within the transducer housing 2 between the window 12 and the axisymmetric lens 6. The grease 14 lubricates the interface between the window 12 and the axi- 30

- 7 -

symmetric lens 6 and displaces air that would otherwise occupy the interface.

The transducer array 4 is mounted on a backing material 16, which is acoustically attenuative. A preferred acoustically attenuative backing material is described in U.S. Patent No. 5,297,553 issued to Sliwa, Jr. et al., which is incorporated herein by reference. Preferably, the backing material 16 is formed from rigid polymeric or polymer-coated particles fused into a macroscopically rigid structure having remnant tortuous permeability, as shown in U.S. Patent No. 5,297,553. This structure provides high acoustic attenuation and permits fluid passage into the backing structure during fabrication. An optional container may provide additional physical integrity to the backing material 16, and the backing material 16 may be attached to the container by an optional bonding adhesive layer. The backing materials described in U.S. Patent No. 5,297,553 provide high acoustic attenuation. This allows a thinner backing material to be used, thereby allowing the transducer probe to be downsized.

A rotatable cable 18 projects into the transducer housing 2, as shown in Figures 1A-1C. Affixed to a distal end of the rotatable cable 18 is a worm 20. The worm 20 engages a worm wheel 22, as shown in Figure 1B. The worm wheel 22 is attached via a vertical shaft 24 to a gear 26. As shown in Figure 1C, the gear 26 engages an idler gear 28, which in turn engages a ring gear 30 attached to a turntable base 32. The turntable base 32 is attached to a pedestal 34 for a platform 36. The platform 36 supports the backing material 16, the transducer array 4, and the axisymmetric lens 6. A stationary pin 38, which is attached at one end to the transducer housing, projects into the pedestal 34.

- 8 -

The platform 36, the pedestal 34, and the turntable base 32 form a bobbin-like structure. A number of ball bearings 40 are contained within the pedestal 34. Preferably, the platform 36 and the pedestal 34 containing the bearings 40 is a single-piece assembly fabricated from hardened stainless steel.

A flexible circuit 42 wraps around and is anchored to the pedestal 34. The flexible circuit 42 electrically couples the transducer array 4 to a remote ultrasound control and operating system. Preferably, the flexible circuit 42 is directly coupled to the elements of the transducer array 4.

During operation of the transducer probe shown in Figures 1 and 2, the transducer array 4 and the axisymmetric lens 6, which is secured thereto, may be rotated by a sonographer or the ultrasound control and operating system coupled to the transducer probe. The housing 2, including the integral window 12, which is in contact with the body of the patient, typically remains stationary during rotation of the array 4 and lens 6.

Rotation of the transducer array 4 and the axisymmetric lens 6 may be brought about by turning the rotatable cable 18, which operates as a worm drive for the gears 26, 28 and 30 coupled to the turntable base 32. During rotation, the layer of grease 14 lubricates the sliding interface between the axisymmetric lens 6 and the window 12 of the housing 2 and ensures that the interface remains void free. Preferably, the turning force applied to the rotatable cable 18 is generated mechanically, such as by an electric motor. Alternatively, the turning force may be generated manually, for example by the sonographer rotating a knob. In a preferred embodiment, the turning force is applied to the rotatable cable remotely from the

- 9 -

transducer housing 2, although a device, such as an electric motor, alternatively may be housed within the transducer housing 2 to directly drive the gear train or the turntable base 32. Although rotation of the transducer array 4 is described herein as being brought about by the rotating cable 18 and the gear train 26, 28 and 30, one of ordinary skill in the art could devise suitable alternative rotational schemes, such as using a linear actuator to slide a cable attached to a rotatably mounted transducer array.

Preferably, the entire transducer housing 2 is formed from an acoustically transmissive material, such as a thermoplastic material. The preferred thermoplastic material is TPX™ from Mitsui Petrochemicals (America) Ltd., 250 Park Ave., Suite 950, New York, New York 10177. Because the entire transducer housing 2 is formed from an acoustically transmissive material, the acoustic window 12 may be integrally formed in the transducer housing 2 by reducing the thickness of the housing 2 in the area above the transducer array 4 and lens 6. It should be noted that formation of the window 12 does not require any opening in the transducer housing 2. The window 12 and the transducer housing 2 form a continuous surface 10 adjacent to the lens 6. Accordingly, additional process steps are not required to seal the window 12 against the ingress of bodily fluids, sterilant solutions, and cleaning solutions.

The thickness of the window 12 portion of the transducer housing 2 may be constant and equal to one-half wavelength of the transmitted acoustic energy at the center frequency of the transducer array 4 in the housing material. For example, if the center frequency of the transducer array 4 is 5 MHz, the window 12 should be 0.2mm thick, where the acoustic velocity in the thermoplastic material is assumed to be 2000ms⁻¹.

- 10 -

Alternatively, the thickness of the window 12 portion of the continuous surface 10 of the transducer housing 2 may vary as a function of distance from the axis 8. For example, the window 12 may be formed into an axisymmetric converging lens by increasing the thickness of the window 12 as a function of increasing distance from the axis 8 (assuming that the velocity of sound in the housing material is greater than the velocity of sound in the body). Similarly, the window 12 may be formed into an axisymmetric diverging lens by decreasing the thickness of the window 12 as a function of increasing distance from the axis 8. Thus, to form the window 12 portion of the continuous surface 10 into a lens, the outer surface 11 of the window 12 will have a different curvature than the inner surface 13 of the window 12. With this alternative embodiment, the probe may be constructed with or without the lens 6. If the lens 6 is present, then the surface 13 of the window 12 that is adjacent to the lens 6 is formed to mate with the lens 6, and the focal length, F , of the assembly is:

$$\frac{1}{F} = \frac{1}{F_{lens}} + \frac{1}{F_{window}} \quad (1)$$

In addition, the thickness of the window 12 portion of the continuous surface 10 may be varied to obviate reverberation artifacts that may otherwise occur if the window 12 is a constant thickness.

The thermoplastic Mitsui TPX™ material is preferred for the housing 2 because of its high modulus and low density, which provide structural rigidity and relative acoustic transparency. In addition, the high dielectric strength of the TPX™ material allows the thickness of the lens 6 to be reduced, further reducing the profile of the transducer housing 2.

- 11 -

The lens 6 is formed from silicone rubber, preferably Dow Corning Q5-8008 having approximately forty-two percent silicon dioxide filler.

Alternatively, Dow Sylgard 577 Primerless Silicone Adhesive RTV-560 may be used, although with a slight degradation in performance.

The grease 14 provides lubrication between the stationary housing window 12 and the rotating lens 6 attached to the transducer array 4. In addition, the grease 14 displaces air that may otherwise be present between the window 12 and the lens 6. The viscosity of the grease 14 should be chosen to minimize air voids and channeling, which may otherwise occur as a result of rotating the array 4 and lens 6. Furthermore, the grease 14 should be chemically compatible with the lens 6 material and housing 2 material. Preferably, the grease 14 is made from synthetic base oils and has a low base-oil kinetic viscosity in the range of 10-40 centistokes measured at 40° C. Acceptable greases include fluorosilicone, polyalphaolefin, and fluoroether greases.

As shown in Figure 1, the axisymmetric lens 6 may have a cylindrical side wall 44, which descends beyond the face of the transducer array 4. A recess 46, shown in Figure 2, may be formed in the continuous surface 10 of the transducer housing 2 to mate with the shape of the lens 6. A grease seal 48 is positioned around the cylindrical wall 44 of the lens 6, as shown in Figure 1, to contain the grease 14 to the volume between the lens 6 and the window 12. Alternatively, a seal may be integrally formed on the cylindrical wall 44 of the lens 6.

Filling ports, such as filling ports 47 and 49 as shown in Figure 2, may be added to the transducer housing 2 to facilitate assembly, minimize air voids, and allow for addition of grease. The filling ports 47

- 12 -

and 49 are substantially cylindrical bores through the transducer housing 2 that are connected by a pathway to the grease-filled interface between the window 12 and the axisymmetric lens 6. A grease plug may be used to seal the filling port. The filling ports 47 and 49 facilitate assembly by providing access to the interface for either adding grease or allowing excess grease to be expelled. Due to the small volume of grease in the interface, thermally induced pressure changes could result in a loss of grease 14 through the seal 48 absent the filling ports. Air voids are minimized by providing pressure relief, under conditions of thermal expansion and contraction, to the grease-filled interface via the grease plugs, which are allowed to slide in the filling ports 47 and 49 in response to expansion or contraction of the grease.

The ultrasonic scanhead shown in Figure 1 may be assembled by casting the lens 6 with the side wall 44 to the transducer array 4. The seal 48 is then positioned around the side wall 44 and grease 14 is applied to the lens 6 and/or the window 12. The array 4, with the previously attached lens 6, is then mated to the housing 2 by inserting the lens portion into the recess 46 and squeezing out any excess grease 14, or air voids within the grease 14, through the filling ports 47 and 49. Alternatively, the lens 6 and array 4 subassembly may be inserted into the recess 46, with the grease 14 being added after assembly through one of the filling ports 47 and 49. Excess grease 14 may exit the housing once the interface is filled through another filling port.

In another embodiment, the axisymmetric lens 6 may be secured to the recess 46 in the housing 2, in which case the lens 6 would remain stationary with the housing 2 and the transducer array 4 would rotate below the lens 6. Alternatively, the recess 46 may be

- 13 -

removed from the transducer housing 2 and the axisymmetric lens 6 secured about its periphery to the transducer housing 2, in place of the recess 46, forming a stationary seal. In this alternative, the transducer array 4 would likewise rotate below the stationary lens 6.

The ultrasonic transducer array 4 may be excited to produce a two-dimensional image of one slice through a three-dimensional target. The plane containing the slice is referred to herein as an object plane. Focusing in one direction, herein referred to as the elevation direction, is provided by the axisymmetric lens 6. For the array and lens geometry shown in Figures 1 through 4, the elevation direction is the direction parallel to the long axis of the elements of the transducer array 4. Focusing in the perpendicular direction, herein referred to as the azimuthal direction, may be achieved electronically using known delay and sum techniques, such as the techniques described in U.S. Patent Nos. 4,140,022 and 4,550,607 issued to Maslak. The azimuthal direction is perpendicular to the long axis of the elements of the transducer array 4. Azimuthal focusing provides focusing of acoustic energy at focal points within the object plane.

Because the thickness of the axisymmetric lens 6 may vary along the azimuthal direction, thereby causing some azimuthal focusing, the delay and sum technique for electronically focusing in the azimuthal direction should be modified to compensate for a lens-induced component of azimuthal focusing. The precise geometry and focusing characteristics of the axisymmetric lens are first determined. The ultrasound control and operating system can then inject compensating electronic delays by the transmitting and receiving

- 14 -

electronics in order to account for the lens-induced component of azimuthal focusing.

5 Timing effects introduced by an azimuthally curved lens may be accounted for by applying Fermat's Shortest Path Law and geometric ray tracing techniques to the lens geometry and adjusting corresponding electronic delays. For a given axisymmetric lens geometry, the minimum time path from each element of the transducer array 4 through the axisymmetric lens 6 to each focal point within the object plane may be 10 computed. For a lens in which the velocity of sound in the lens is less than the velocity of sound in the body, such as a silicone rubber lens, the minimum time path is longer for an array with a lens than it would be if there were no lens. Delay times must, therefore, 15 be modified in both the transmit and receive circuitry to compensate for this increase in propagation time. Alternatively, the required compensating delays may be derived by applying Snell's Law and geometric ray 20 tracing techniques to the lens geometry.

Referring now to Figure 3, a section of the transducer array 4 and the axisymmetric lens 6 assembly is shown, the section being taken along the azimuthal direction through the center of the array. Individual 25 transducer elements 4a . . . 4p are shown adjacent to the axisymmetric lens 6. A focal point 50 within the body is illustrated.

For a given axisymmetric lens geometry, the minimum time path from each element of the transducer array 4 through the axisymmetric lens 6 to each focal point 50 within the object plane is calculated as 30 follows. Given a transducer element 4d centered at the point $(x_1, 0)$ and a desired focal point 50 at (x_3, y_3) , the minimum time path for the transducer element 4d will cross the interface between the lens 6 and the 35

- 15 -

body at some point (x_2, y_2) . The minimum propagation time, t , is:

$$t = \frac{B}{C_{lens}} + \frac{C}{C_{body}} \quad (2)$$

5 In equation 2, B is the path length within the lens and C is the path length within the body corresponding to the minimum time path. C_{lens} and C_{body} are the velocities of sound in the lens and body, respectively.

If the axisymmetric lens 6 is a spherical lens, then the thickness, T, of the lens at the point (x_2, y_2) is:

$$T(x_2) = y_2 = T - R + \sqrt{R^2 - x_2^2} \quad (3)$$

10 In equation 3, T is the maximum thickness of the spherical lens, which is located over the center element of the array 4, and R is the radius of curvature of the lens. The equation for T(x) for a spherical lens may be approximated by the equation
15 for T(x) for a parabolic lens:

$$T(x_2) = y_2 \approx T - \frac{x_2^2}{2R} \quad (4)$$

Substituting for y_2 , equation (2) for the minimum propagation time, t , can be rewritten as a function of the variable x_2 :

$$t = \frac{1}{C_{lens}} \sqrt{(x_2 - x_1)^2 + T^2(x_2)} + \frac{1}{C_{body}} \sqrt{(x_3 - x_2)^2 + [y_3 - T(x_2)]^2} \quad (5)$$

20 The coordinate x_2 that minimizes t can then be found, for example by an iterative search. Once x_2 is found for transducer element 4d, which is centered at x_1 , the difference $(x_2 - x_1)$ can be used as an initial value in the search for x_2 for neighboring transducer elements, 4c and 4e.

- 16 -

Knowing the value of x_2 corresponding to the minimum propagation time t for each element 4a . . . 4p of the array 4, the corresponding increase in propagation time due to the lens 6 for each element of the array 4 is:

$$\begin{aligned} \Delta t &= \frac{1}{C_{lens}} B + \frac{1}{C_{body}} [C-A] \\ &= \frac{1}{C_{lens}} \sqrt{(x_2-x_1)^2 + T^2(x_2)} + \frac{1}{C_{body}} \left[\sqrt{(x_3-x_2)^2 + [y_3-T(x_2)]^2} - \sqrt{(x_3-x_1)^2 + y_3^2} \right], \end{aligned} \quad (6)$$

where A is the distance between the transducer element and the focal point 50 at (x_3, y_3) . The delay for each element of the array is determined by inputting the appropriate value of x_2 . Corresponding delays must be calculated for each focal point within the object plane. Because the minimum time path is greater for an array with a lens than it is without a lens, the change in delay time, Δt , is subtracted from the delay time that the ultrasound control and operating system would apply in the absence of the axisymmetric lens to achieve azimuthal focusing. Determination of the delay time that the ultrasound control and operating system would apply in the absence of a lens is described in U.S. Patent Nos. 4,140,022 and 4,550,607.

The transducer probe described herein may be used with an ultrasound operating and control system for scanning in a variety of scan and display formats, including, but not limited to, a variable vertex format as described in U.S. Patent Nos. 5,148,810, 5,261,408, and 5,235,986 issued to Maslak et al., which are incorporated herein by reference. The variable vertex scan and display format provides an expanded field of view for a given transducer array geometry by transmitting ultrasonic pressure waves and receiving return echoes on a set of spatially non-overlapping acoustic scan lines, wherein each acoustic scan line originates at an arbitrary point on and at an arbitrary angle to the

- 17 -

face of the array. The set of acoustic scan lines is formed by software control. As described in U.S. Patent No. 5,148,810, the set of acoustic scan lines may align with rays emanating from a common vertex located a selectable distance behind the face of the transducer array. The distance between the vertex and the face of the transducer array 4 is referred to herein as the vertex offset 62.

Referring now to Figure 4, the transducer array 4 is shown. A set of acoustic scan lines produces a field of view 52 in the variable vertex format. The set of acoustic scan lines appears to emanate from a common vertex 54. An acoustic scan line 56 from the set of acoustic scan lines is illustrated. The acoustic scan line 56 originates at a point 58 on the face of the transducer array 4 and emanates at an angle θ with respect to the normal 57 to the face of the transducer array 4. The vertex offset 62 is illustrated.

The point 58 on the face of the transducer array 4 at which the acoustic scan line 56 originates is referred to herein as the acoustic line origin. For a given transducer array geometry, the acoustic line origin is selectable under software control. The acoustic line origin for the planar array of Figure 4 occurs on a line 59 connecting the individual transducer elements at the point corresponding approximately to the center of mass of the apodization function applied to the array 4. Thus, controlling the acoustic line origin is achieved by assigning apodization values to each element of the transducer array 4 so that the center of mass of the apodization function corresponds to the desired point 58 on the face of the transducer array 4, as described in U.S. Patent No. 5,148,810.

In order to operate the transducer probe of Figure 1 in the variable vertex scan and display

- 18 -

format, the ultrasound control and operating system compensates for the presence of the axisymmetric lens 6 between the transducer array 4 and the body to be imaged. The axisymmetric lens 6 a) increases the distance between the vertex and the body to be imaged, and b) refracts the acoustic scan lines.

Figure 5A illustrates the increased distance between the vertex 54 and the body to be imaged 60 due to the presence of the lens 6. When scanning without the lens 6, the vertex offset 62 is the distance between the vertex 54 and the face of the transducer array 4. The ultrasound control and operating system assumes, when the lens 6 is present, that the body begins at a plane 60, which is parallel to the face of the transducer array 4. The acoustic scan line 56 originates at the point 58 on the face of the transducer array 4 and at the angle θ with respect to the normal to the face of the array. The acoustic scan line 56 passes through the plane 60 at a point 66.

The ultrasound control and operating system compensates for the increase in distance between the vertex 54 and the body to be imaged by using an adjusted vertex offset 64 that accounts for the thickness of the lens 6. The vertex offset 64, which accounts for the lens 6, VA_{lens} is:

$$VA_{lens} = VA + \frac{C_{body}}{C_{lens}} T \quad (7)$$

where VA is the vertex offset for a constant sound velocity (i.e. lens-less) medium, C_{body} is the sound velocity in the body, C_{lens} is the sound velocity in the lens 6, and T is the maximum thickness of the lens.

The presence of the lens 6 in front of the array 4 will cause the acoustic scan line to refract, thereby requiring a shift in the acoustic line origin by some distance, Δx , in the azimuthal direction. Figure 5B is a sectional view of the transducer array 4

and the axisymmetric lens 6, the section being taken along the azimuthal direction through the array 4. An acoustic scan line 68 originates at a point 70 on the face of the transducer array 4. The acoustic scan line 68 propagates through the lens 6 to the lens/body interface at a point 72. The acoustic scan line 68 then passes through the plane 60, where imaging begins to take place, at a point 74.

The acoustic scan line 68 propagates through the lens 6 at an angle θ_{lens} with respect to a normal 76 to the face of the transducer array 4 and propagates through the body at an angle θ with respect to the normal 76. The angle of the lens/body interface at the point 72 with respect to the plane 60 is designated θ_c .

The appropriate shift, Δx , in the acoustic line origin 70 must be computed for the acoustic scan line 68 so that the point 74, shown in Figure 5B, coincides with the point 66, shown in Figure 5A. The shift in acoustic line origin, Δx , must be computed for each acoustic scan line in the set of acoustic scan lines. The shift in the acoustic line origin, Δx , induced by the lens 6 may be determined as follows.

If x refers to the horizontal position of a point as measured from the center 78 of the transducer array 4, and y refers to the point's vertical position as measured from the plane 60 where imaging begins, then the horizontal position of the point 74 where the acoustic scan line 68 crosses the imaging plane 60 is:

$$x_{74} = x_{66} = VA_{lens} \cdot \tan \theta \quad (8)$$

For a spherical axisymmetric lens 6, the horizontal position of the point 72 where the acoustic scan line 68 crosses the lens/body interface is:

$$\begin{aligned} x_{72} &= x_{74} - y_{72} \cdot \tan \theta, \\ &= VA_{lens} - \frac{x_{72}^2}{2R} \cdot \tan \theta \quad (\text{parabolic approximation}), \\ &= \frac{R}{\tan \theta} \left[-1 + \sqrt{1 + \frac{2VA_{lens} \tan^2 \theta}{R}} \right] \end{aligned} \quad (9)$$

- 20 -

(10)

(11)

where R is the radius of curvature of the lens 6 in the azimuthal direction. Equation (11) is arrived at by solving the quadratic equation (10) and taking the appropriate root. Equation (11) can be simplified using the approximation:

$$\sqrt{1+x} = 1 + \frac{1}{2}x - \frac{1}{8}x^2 + \frac{1}{16}x^3 - \frac{5}{128}x^4 \quad \text{if } |x| < 1. \quad (12)$$

With this approximation, the horizontal position of the point 72 is:

$$x_{72} = VA_{lens} \tan \theta - \frac{VA_{lens}^2}{2R} \tan^3 \theta + \frac{VA_{lens}^3}{2R^2} \tan^5 \theta - \frac{5VA_{lens}^4}{8R^3} \tan^7 \theta. \quad (13)$$

The angle θ_c of the lens/body interface with respect to the imaging plane 60 at the point 72 is:

$$\theta_c = \text{atan} \left[\frac{x_{72}}{\sqrt{R^2 - x_{72}^2}} \right], \quad (14)$$

$$= \text{atan} \left[\frac{x_{72}}{R} \right] \quad (\text{parabolic approximation}) \quad (15)$$

$$\approx \frac{x_{72}}{R} \quad (\text{small angle approximation}). \quad (16)$$

The angle θ_{lens} of the acoustic scan line 68 within the lens 6 with respect to the normal 76 is given by Snell's Law as:

$$\theta_{lens} = \text{asin} \left[\frac{C_{lens}}{C_{body}} \sin(\theta - \theta_c) \right] + \theta_c \quad (17)$$

Using the angle θ_{lens} the horizontal position of the acoustic line origin 70 is:

$$x_{70} = x_{72} - \left(T - R + \sqrt{R^2 - x_{72}^2} \right) \tan \theta_{lens}$$

- 21 -

(18)

and the acoustic line origin shift, Δx , is:

$$\Delta x = x_{70} - VA \cdot \tan \theta \quad (19)$$

The acoustic line origin shift, Δx , provides the
 5 desired point on the face of the transducer array to be
 equated with the center of mass of the apodization
 function for the transducer array.

The start-of-line delay should also be
 adjusted on an acoustic line-by-line basis to reduce
 10 image distortion. The start-of-line delay due to the
 lens 6 is the time it takes to propagate from the face
 of the transducer array, through the lens 6, to a plane
 where the ultrasound control and operating system
 assumes the body begins, i.e. the imaging plane 60, and
 15 back again. The ultrasound control and operating
 system typically assumes that the body begins at the
 plane that is parallel to the face of the transducer
 array 4 and is tangential to the lens 6.

Using the values for the acoustic line
 20 origin, the line-by-line variation in the start-of-line
 delay may be approximated as follows:

$$\Delta SOL = 2 \left[\frac{1}{C_{lens}} \cdot \frac{1}{\cos \theta_{lens}} (T - R + \sqrt{R^2 - X^2}) + \frac{1}{C_{body}} \cdot \frac{1}{\cos \theta} (R - \sqrt{R^2 - X^2}) \right] \quad (20)$$

Ultrasound data acquired after the start-of-line delay
 are displayed by the ultrasound control and operating
 25 system, while earlier received data are discarded.

It is intended that the foregoing detailed
 description be regarded as illustrative rather than
 limiting and that it is understood that the following
 claims, including all equivalents, are intended to
 30 define the scope of the invention.

- 22 -

WE CLAIM:

1. An ultrasonic transducer probe,
comprising:
5 an array of ultrasonic transducers;
a lens positioned adjacent to the array; and
a housing encasing the array and the lens,
wherein the housing has a continuous surface adjacent
to the lens for passing ultrasonic energy.

10 2. An ultrasonic transducer probe as
claimed in claim 1, wherein the lens is axisymmetric.

3. An ultrasonic transducer probe as
claimed in claim 2, wherein the axisymmetric lens is
mounted to the array.

15 4. An ultrasonic transducer probe as
claimed in claim 1, further comprising:
a platform for supporting the array;
a pedestal having a first end coupled to the
platform and a second end coupled to a turntable base;
and
20 a gear coupled to the turntable base.

5. An ultrasonic transducer probe as
claimed in claim 4, further comprising a rotatable
cable coupled to the gear.

25 6. An ultrasonic transducer probe as
claimed in claim 1, further comprising means for
independently exciting each element of the array.

30 7. An ultrasonic transducer probe as
claimed in claim 6, wherein the excitation means
comprises a flexible circuit electrically coupled to
the array.

- 23 -

8. An ultrasonic transducer probe as claimed in claim 1, further comprising a grease layer positioned between the lens and the housing.

5 9. An ultrasonic transducer probe as claimed in claim 1, further comprising a backing material upon which the array is mounted.

10 10. An ultrasonic transducer probe as claimed in claim 9, wherein the backing material provides high acoustic attenuation.

10 11. An ultrasonic transducer probe as claimed in claim 10, wherein the backing material comprises rigid polymeric or polymer-coated particles fused into a macroscopically rigid structure having remnant tortuous permeability to provide high acoustic
15 attenuation and to permit fluid passage into the structure.

20 12. An ultrasonic transducer probe as claimed in claim 1, wherein the continuous surface of the housing that is adjacent to the lens is formed to mate with the lens.

13. An ultrasonic transducer probe as claimed in claim 12, wherein the lens is attached to the continuous surface of the housing.

25 14. An ultrasonic transducer probe as claimed in claim 13, further comprising a grease layer positioned between the lens and the transducer array.

15. An ultrasonic transducer probe as claimed in claim 12, wherein the continuous surface of the housing that is adjacent to the lens has

- 24 -

a thickness of one-half wavelength of the ultrasonic energy within the housing.

5 16. An ultrasonic transducer probe as claimed in claim 12, wherein the continuous surface refracts the ultrasonic energy.

 17. An ultrasonic transducer probe as claimed in claim 16, wherein the continuous surface forms an axisymmetric converging lens.

10 18. An ultrasonic transducer probe as claimed in claim 1, wherein the housing comprises a thermoplastic material.

 19. An ultrasonic transducer probe as claimed in claims 8 or 14, wherein the housing has a filling port connected by a pathway to the grease layer.

 20. An ultrasonic transducer probe, comprising:
 a rotatable array of ultrasonic transducers mounted about an axis within the ultrasonic transducer probe;
 a lens mounted to the array, the lens being symmetric about the axis; and
 a housing encasing the array and the lens, wherein an upper surface of the housing has an integral window that is formed, in a region adjacent to the lens, to mate with the lens.

25 21. An ultrasonic transducer probe as claimed in claim 20, wherein the lens and the region of the housing adjacent to the lens are spherically shaped.

30

- 25 -

5 22. An ultrasonic transducer probe as claimed in claim 20, wherein the housing is formed from a material that passes ultrasonic energy and the integral window has a thickness that is less than the thickness of the remainder of the housing.

 23. An ultrasonic transducer probe as claimed in claim 20, wherein the upper surface of the housing has a recess formed therein for encircling the lens.

10 24. An ultrasonic transducer probe as claimed in claim 20, further comprising:
 a backing material upon which the array is mounted;
 a platform upon which the backing material is mounted;
15 a pedestal having a first end that supports the platform and a second end that is coupled to a turntable base, the pedestal defining the axis;
 at least one gear coupled to the turntable
20 base for rotating the base, the backing material, the array, and the lens about the axis; and
 a flexible circuit electrically coupled to the array.

25 25. An ultrasonic transducer probe as claimed in claim 20, wherein the housing is formed from a thermoplastic material.

 26. An ultrasonic transducer probe as claimed in claim 25, wherein the thermoplastic material is acoustically transparent.

30 27. An ultrasonic transducer probe as claimed in claim 22, wherein the thickness of the

- 26 -

integral window is one-half wavelength of the ultrasonic energy within the housing material.

28. An ultrasonic transducer probe as claimed in claim 20, wherein the lens further comprises
5 a cylindrical side wall descending from the lens, wherein the side wall encircles the array.

29. An ultrasonic transducer probe as claimed in claim 28, further comprising a grease seal positioned around the side wall of the lens.

10 30. An ultrasound system for providing diagnostic information from the interior of a body, comprising:

an ultrasonic transducer probe having an array of ultrasonic transducers, an axisymmetric lens
15 mounted to the array, and a housing encasing the array and the lens, wherein the housing has a continuous surface adjacent to the lens;

an operating and control system for processing electrical signals produced by the
20 ultrasonic transducer probe; and

means for operatively coupling the ultrasonic transducer probe to the operating and control system.

31. An ultrasound system as claimed in claim 30, wherein the operating and control system comprises
25 transmitting electronics and receiving electronics, each of which have variable electronic delays for focusing the array in an azimuthal direction.

32. An ultrasound system as claimed in claim 31, wherein at least one of the variable electronic
30 delays compensates for azimuthal focusing induced by the axisymmetric lens.

- 27 -

33. An ultrasound system as claimed in claim 32, wherein the operating and control system further comprises means for acoustically scanning in a variable vertex format.

5 34. An ultrasound system as claimed in claim 30, wherein the operating and control system further comprises means for displaying acoustic echoes received by the ultrasonic transducer probe.

10 35. An ultrasound system as claimed in claim 30, wherein the ultrasonic transducer probe further comprises means for rotating the array and the axisymmetric lens.

15 36. An ultrasound system as claimed in claim 33, wherein the scanning means adjusts a vertex offset, an acoustic line origin, and a start-of-line delay for a set of acoustic lines to compensate for the axisymmetric lens.

20 37. An ultrasound system as claimed in claim 35, wherein the rotating means comprises an electric motor.

25 38. A method of providing diagnostic information from an interior of a body, comprising:
providing an ultrasound system having transmitting electronics, receiving electronics, an array of ultrasonic transducer elements having a face, and an axisymmetric lens positioned above the array, for transmitting acoustic pressure waves into the body and receiving acoustic echoes from the body through the axisymmetric lens along a set of acoustic lines;
30 storing a value corresponding to an increase in propagation time to a focal point on an acoustic

- 28 -

line from the set of acoustic lines due to the axisymmetric lens for at least one element of the array; and

5 adjusting the transmitting electronics and the receiving electronics in accordance with the stored value.

10 39. A method as claimed in claim 38, wherein the step of adjusting the transmitting and receiving electronics comprises adjusting a delay time provided by variable electronic delays coupled to the elements of the array.

40. A method as claimed in claim 39, wherein the step of adjusting the delay time comprises decreasing the delay time by the stored value.

15 41. A method as claimed in claim 38, wherein the set of acoustic lines is a set of spatially non-overlapping acoustic lines.

20 42. A method as claimed in claim 41, wherein each acoustic line in the set of acoustic lines has an origin at a selectable point on the face of the array.

43. A method as claimed in claim 42, wherein at least one acoustic line is refracted at an interface between the body and the axisymmetric lens.


25 44. A method as claimed in claim 43, wherein each acoustic line origin is selected so that an extension of the acoustic line in the body beyond the interface passes through a substantially common vertex that is not located on the face of the array.

- 29 -

45. An ultrasonic transducer probe as claimed in claim 1, wherein the lens is formed from silicone rubber having 42% silicon dioxide filler.

1/4

FIG. 1A

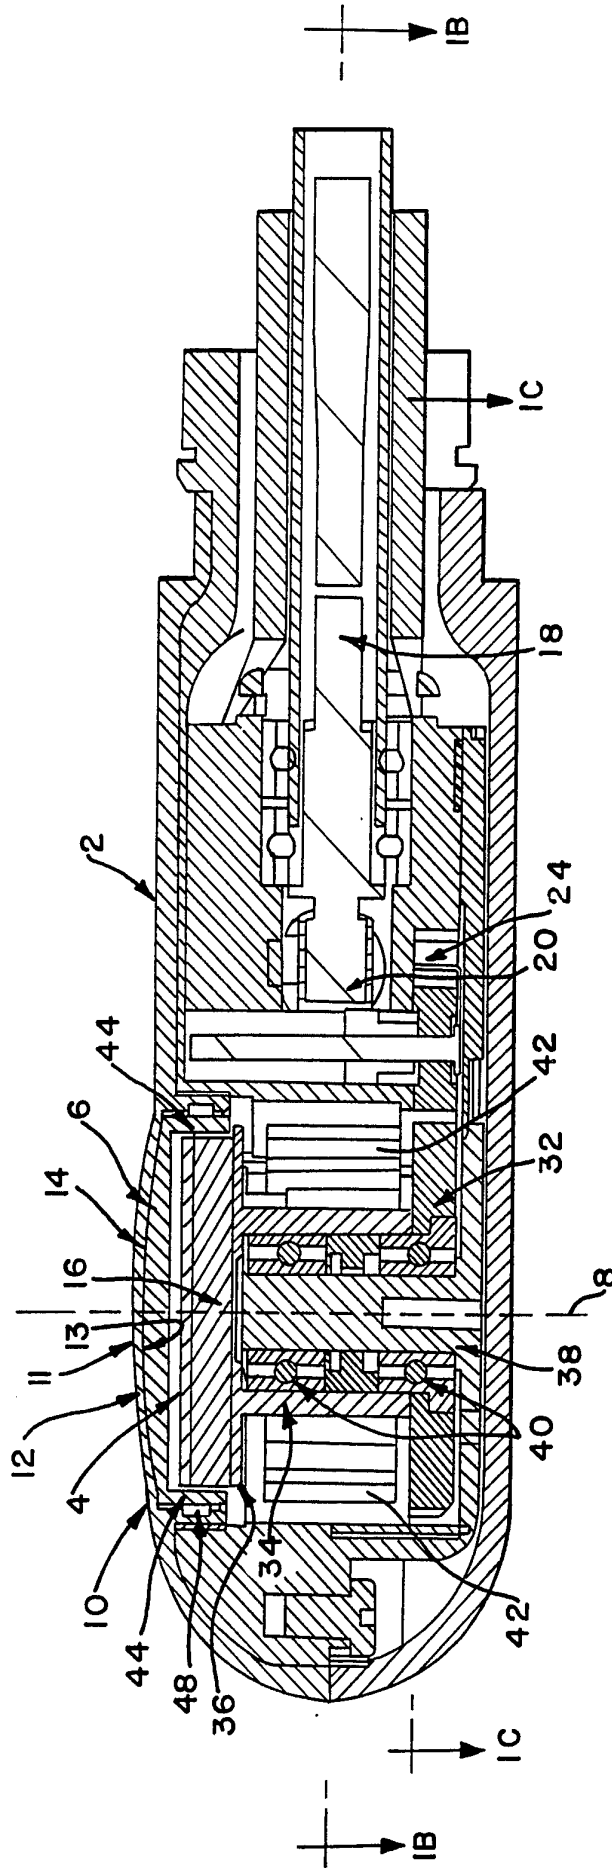

SUBSTITUTE SHEET (RULE 26)

FIG. 1B

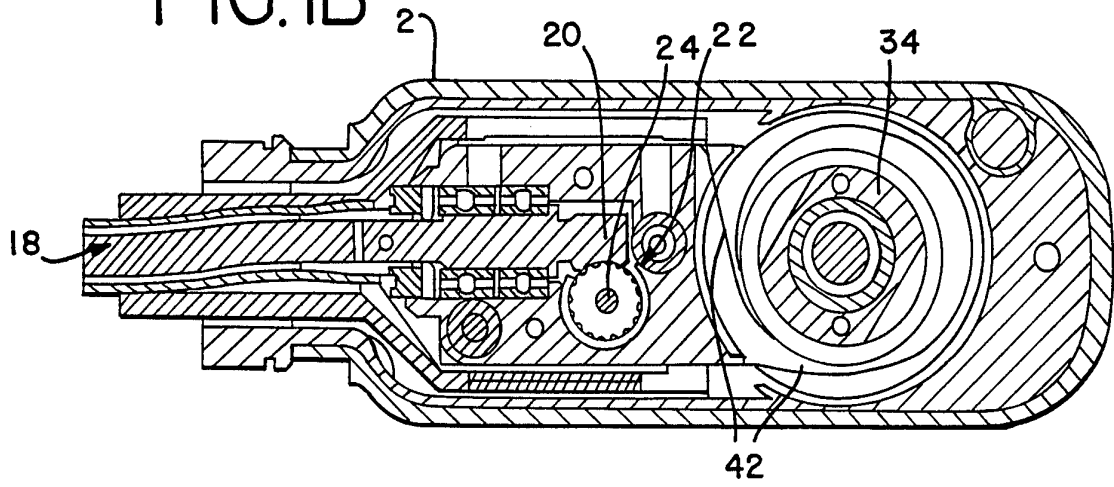


FIG. 1C

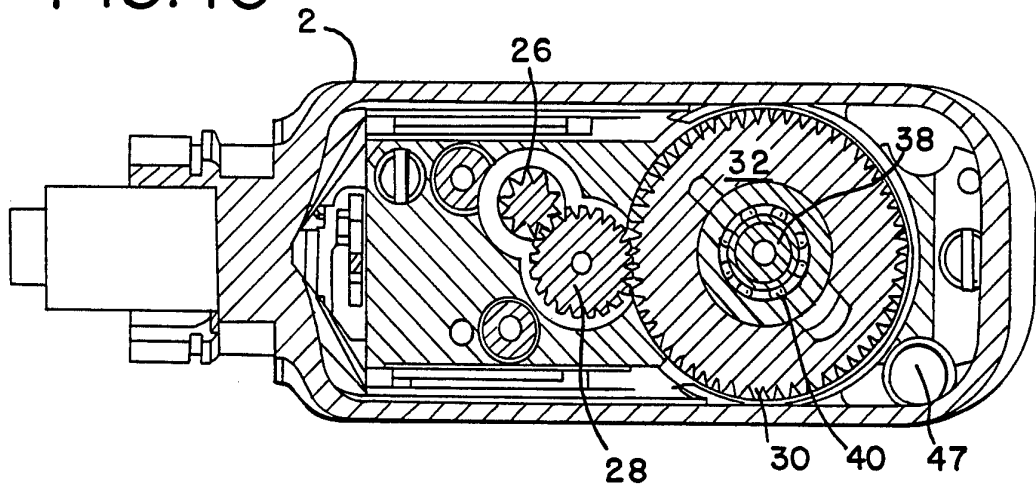
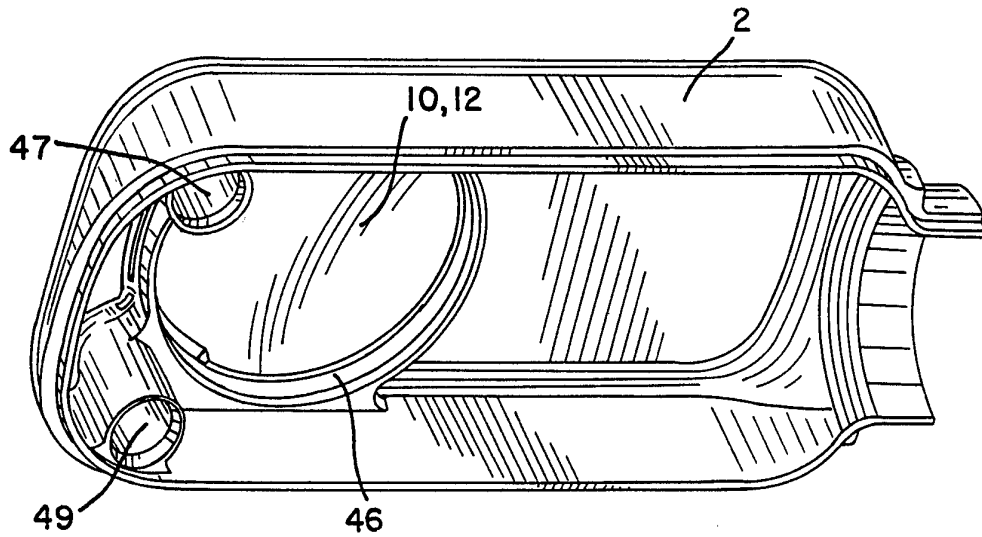


FIG. 2



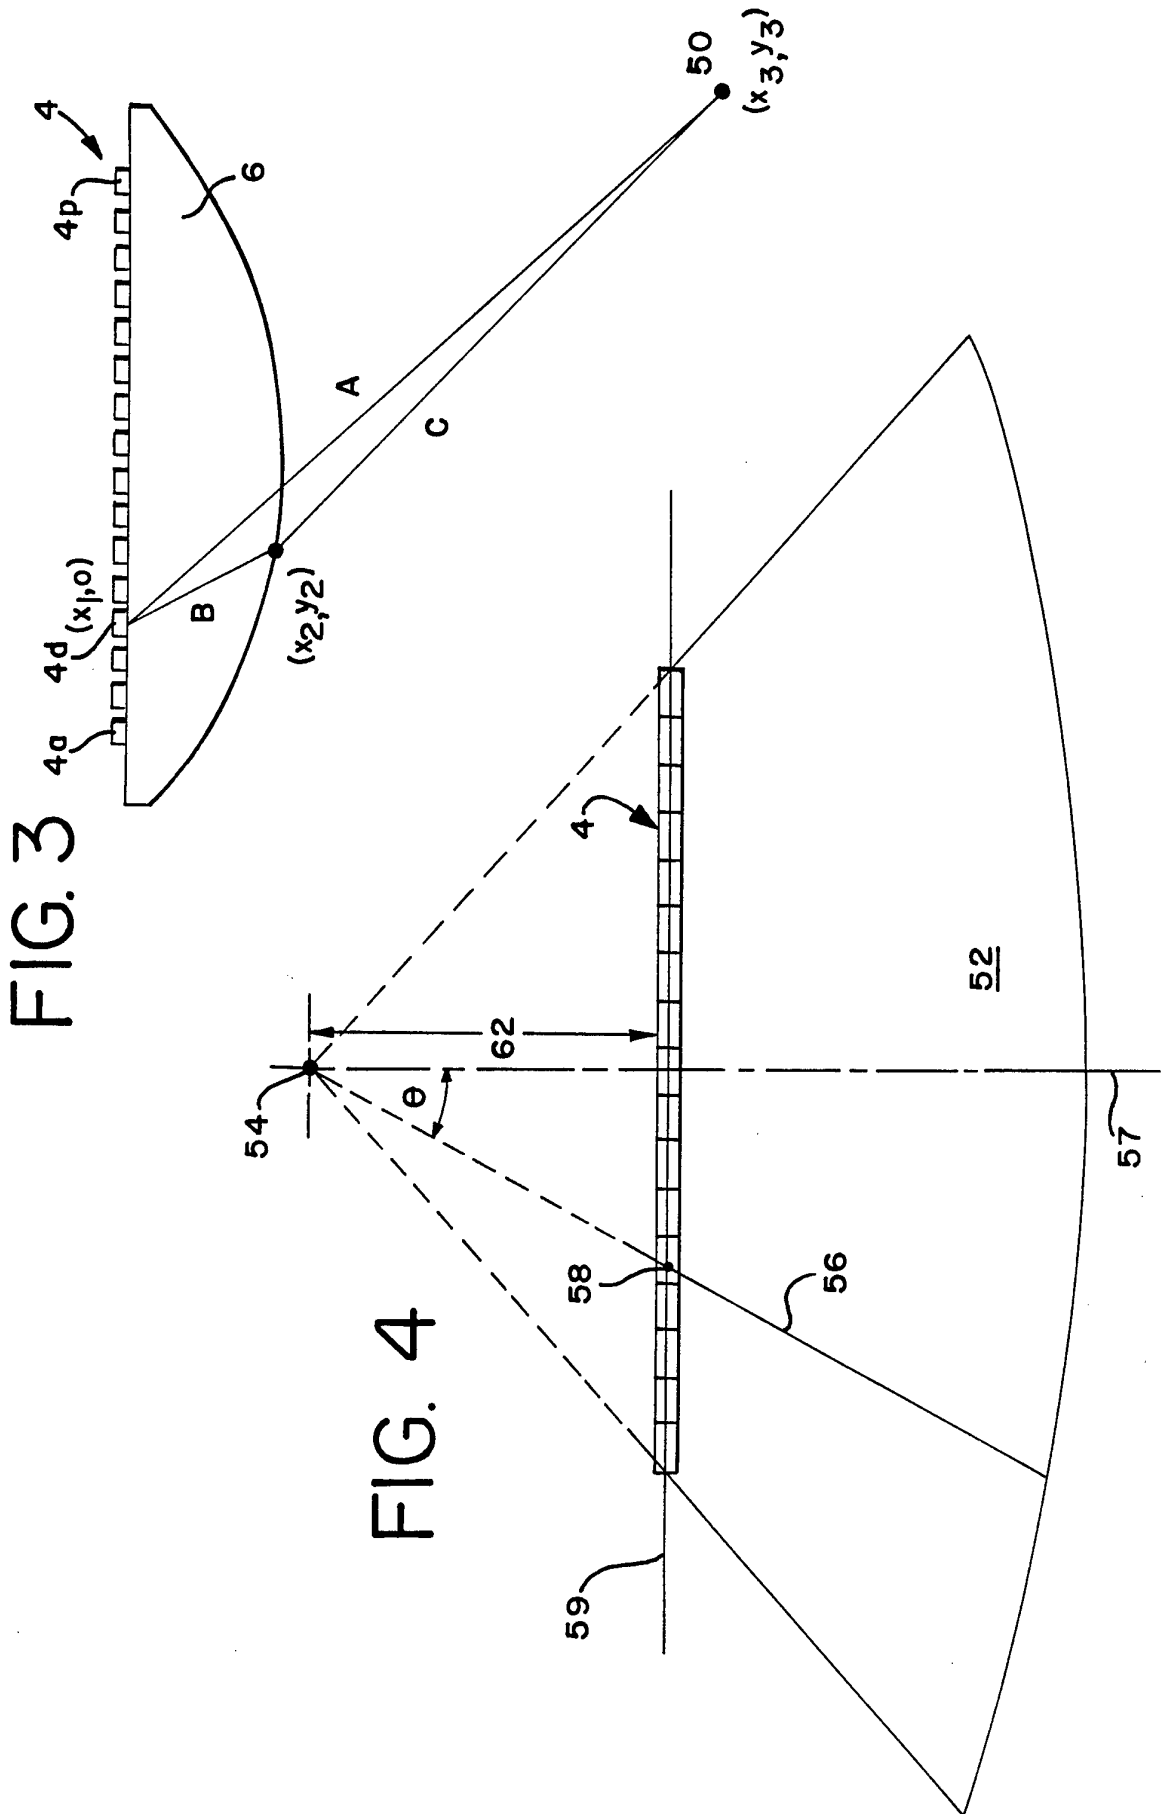


FIG. 5B


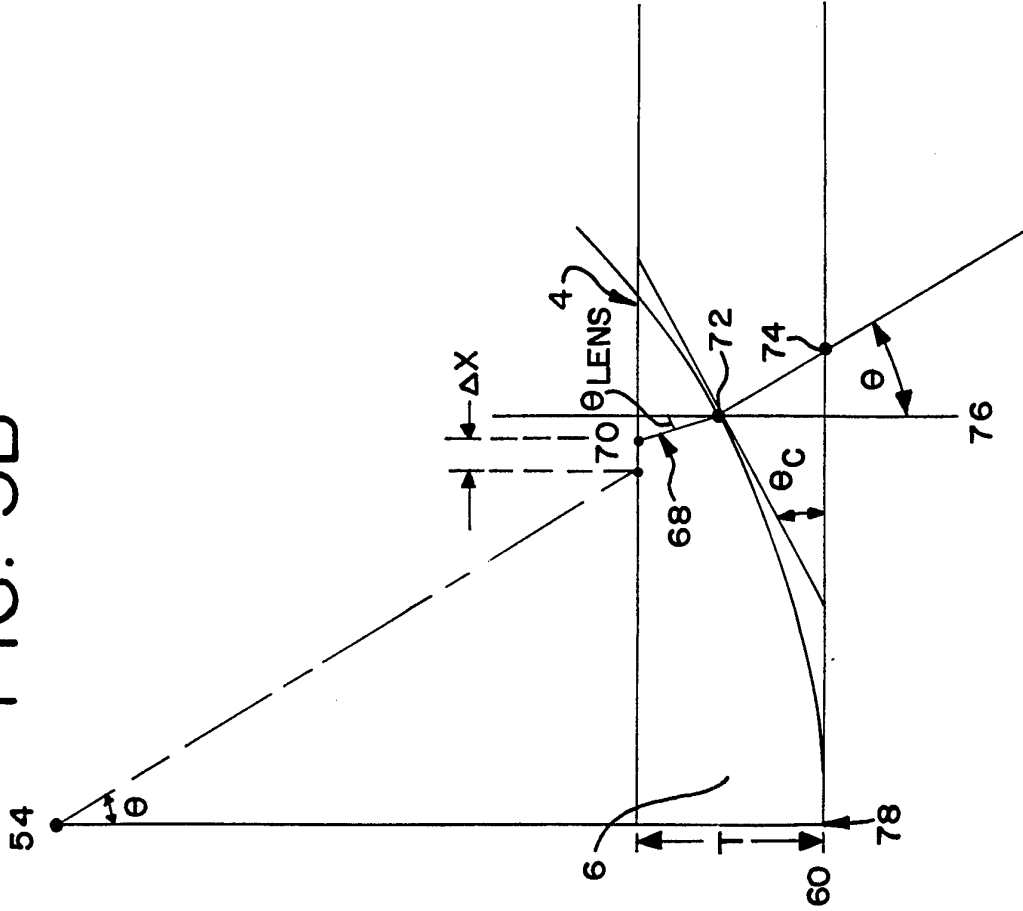


FIG. 5A

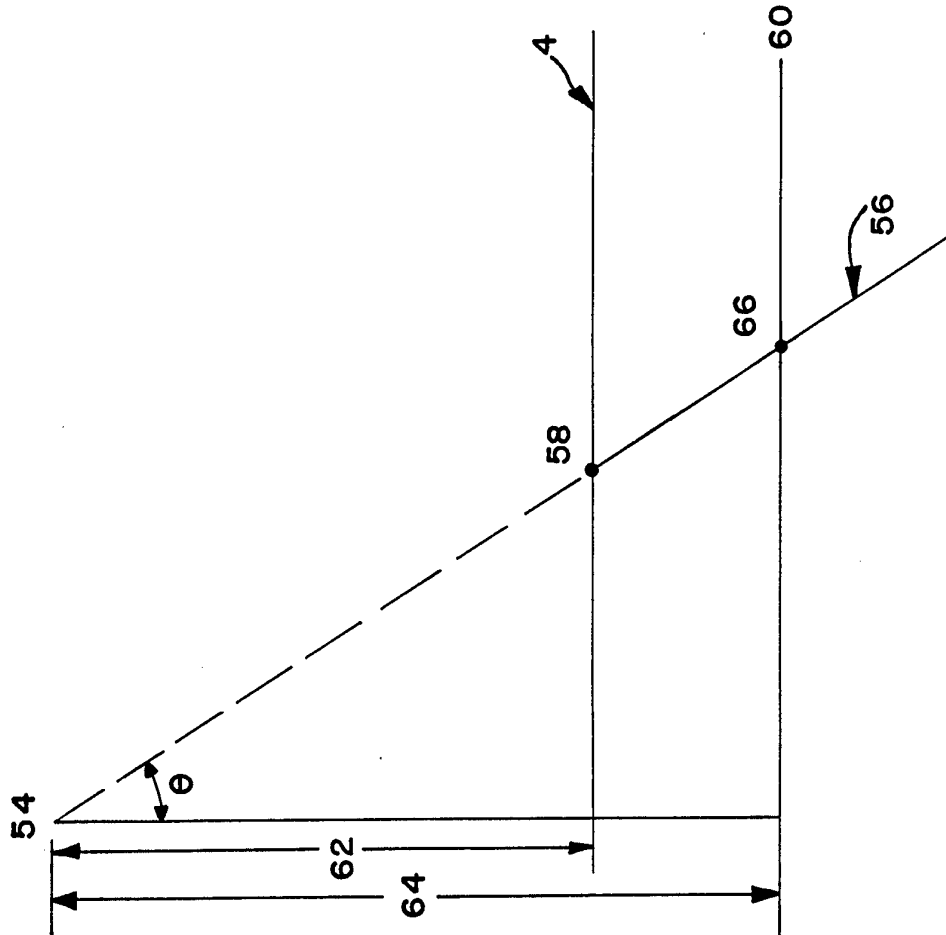

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US95/07756

A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) :A61B 8/12
US CL :128/662.060

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 128/662.060

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

73/642, 644; 128/660.080, 660.100

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

NONE

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X --- Y	US, A, 5,226,422 (McKEIGHEN ET AL.) 13 July 1993, see column 3 lines 23-25, and column 4 lines 13-21.	1-3, 6, 30, 31, 34, 35 ----- 1-13, 15-18, 19/8, 20-31, 34, 35, 37, 45
X --- Y	US, A, 5,305,755 (NAKAO) 26 April 1994, see column 3, lines 15-33.	1-3, 6, 30, 31, 34, 35 ----- 1-13, 15-18, 19/8, 20-31, 34, 35, 37, 45

Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

01 SEPTEMBER 1995

Date of mailing of the international search report

14 SEP 1995

Name and mailing address of the ISA/US
Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

FRANK JAWORSKI

Telephone No. (703) 308-3061

INTERNATIONAL SEARCH REPORT

 International application No.
 PCT/US95/07756

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X ---,P Y	US, A, 5,402,793 (GRUNER ET AL.) 04 April 1995, see column 3 lines 12-21, and column 4 lines 38-57.	1-3, 6, 30, 31, 34, 35 ----- 1-13, 15-18, 19/8, 20-31, 34, 35, 37, 45
Y	US, A, 4,762,002 (ADAMS) 09 August 1988, see column 4 lines 8-16.	1-13, 15-18, 19/8, 20-31, 34, 35, 37, 45
Y	US, A, 5,176,142 (MASON) 05 January 1993, see column 3 lines 28-31, and column 3 line 57 to column 4 line 12.	4, 5, 8, 24
Y	US, A, 5,297,553 (SLIWA, JR. ET AL.) 29 March 1994, see column 3 lines 27-36.	9-11
Y	US, A, 4,567,895 (PUTZKE) 04 February 1986, see column 3 lines 19-22.	19/8
Y	US, A, 4,880,012 (SATO) 14 November 1989, see column 2 lines 64-66.	45