



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> : <b>G01N 27/327</b>	<b>A1</b>	(11) International Publication Number: <b>WO 99/58966</b>  (43) International Publication Date: 18 November 1999 (18.11.99)
<p>(21) International Application Number: PCT/GB99/01425</p> <p>(22) International Filing Date: 7 May 1999 (07.05.99)</p> <p>(30) Priority Data: 9809918.7                      8 May 1998 (08.05.98)                      GB</p> <p>(71) Applicant (for all designated States except US): ISIS INNOVATION LIMITED [GB/GB]; 2 South Parks Road, Oxford OX1 3UB (GB).</p> <p>(72) Inventors; and (75) Inventors/Applicants (for US only): DOBSON, Peter, James [GB/GB]; Isis Innovation Limited, 2 South Parks Road, Oxford OX1 3UB (GB). LEIGH, Peter, Alexander [GB/GB]; Isis Innovation Limited, 2 South Parks Road, Oxford OX1 3UB (GB). NAKAGAWA, Yasue [JP/GB]; Isis Innovation Limited, 2 South Parks Road, Oxford OX1 3UB (GB). HILL, Hugh, Allen, Oliver [GB/GB]; Isis Innovation Limited, 2 South Parks Road, Oxford OX1 3UB (GB).</p> <p>(74) Agents: ELLIS-JONES, Patrick, George, Armine et al.; J.A. Kemp &amp; Co., 14 South Square, Gray's Inn, London WC1R 5LX (GB).</p>	<p>(81) Designated States: JP, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p><b>Published</b> <i>With international search report.</i></p>	
(54) Title: MICROELECTRODE BIOSENSOR AND METHOD THEREFOR		
(57) Abstract		
<p>There is disclosed a biosensor comprising a conducting surface (6), a layer of dielectric material (5) overlying the conducting surface (6), a plurality of micro electrodes constituted by a plurality of pores (7) extending through the thickness of said dielectric layer, a biopolymer positioned on the conducting surface (6) in said pores (7) and a counter electrode arranged such that electrical connection can be made between it and at least part of said conducting surface (6) by a fluid to be assessed. Such a device can be made using a method comprising the steps of providing a conducting surface (6); providing a layer of dielectric material (5) adjacent to said conducting surface (6), said dielectric material (5) comprising a plurality of pores (7) extending through the thickness of the dielectric layer; providing a biopolymer on the conducting surface (6) in said pores (7); and providing a counter electrode insulated from said conducting surface (6).</p>		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

MICROELECTRODE BIOSENSOR AND METHOD THEREFOR

This invention relates to the use of micro-electrode arrays in biosensors and to methods of producing such biosensors.

5

An array of micro electrodes offers many advantages over a large area electrode for use as an amperometric electrochemical sensor. These advantages include a very small charging capacitance, radial diffusion kinetics, a rapid response time and easily interpreted current-voltage behaviour. The present invention relates to a particular arrangement of such an array to provide a biosensor.

The present invention provides a biosensor comprising a conducting surface, a layer of dielectric material overlying the conducting surface, a plurality of micro electrodes constituted by a plurality of pores extending through the thickness of said dielectric layer, each pore being separated from its neighbour, a biopolymer positioned in said pores, and a counter electrode arranged such that electrical connection can be made between it and at least part of said conducting surface by a fluid to be assessed.

The present invention also provides a method of making a biosensor comprising the steps of:

providing a conducting surface;

providing a layer of dielectric material adjacent to said

conducting surface, said dielectric material comprising a plurality of pores extending through the thickness of the dielectric layer, each pore being separated from its neighbour;

- 5           providing a biopolymer in said pores, and  
            providing a counter electrode insulated from said  
conducting surface.

In general, the biosensor comprises one or more areas of  
10   conducting material arranged on an insulating substrate.  
Adjacent to each area of conducting material is a dielectric  
coating which comprises a plurality of pores. These pores are  
the micro electrodes that convert a chemical response into an  
electrical signal. They do this due to the presence of a  
15   biopolymer immobilised on the conducting surface. In use, a  
fluid to be assessed is applied to the pores in the dielectric  
surface so as to be in contact with the biopolymer immobilised  
in the pores. A counter electrode is also provided so as to  
be in electrical connection with at least one of the  
20   conducting areas via the fluid being assessed. A constant  
voltage may be applied between the counter electrode and the  
conducting area and the current that flows therebetween may be  
measured. Any such measured current is indicative of the  
amount of a chosen compound in the assessed fluid. Different  
25   biopolymers may be used to allow different compounds to be  
measured giving great flexibility. The biosensor device  
typically has dimensions of a few millimetres although it  
could of course be made smaller or larger, depending on the  
intended application.

The electrodes typically have areas of 1 to 100  $\mu\text{m}^2$  and are typically separated by distances of about ten times their diameter. The surface of the electrode can be functionalised with various biopolymers, especially enzymes such that they will only give an electrochemical response to a specific compound (or analyte). Other biopolymers include other proteins, as well as nucleic acids, lipids and polysaccharides. For example, enzymes that respond to important body fluid components such as lactate, glucose, creatine, or various antibodies could be used. Typical enzymes include lactate dehydrogenase, glucose dehydrogenase, cytochrome P450 and mutants of the aforesaid enzymes. In addition by ociation of these enzymes, antibodies, nucleic acids, lipids and polysaccharides can be made electrochemically active. Micro-electrode arrays have not, it is believed, previously been activated by biopolymers for use as biosensors. One advantage is that only two electrodes are required *vis* the working electrode and a counter electrode. Although the magnitude of the current from an individual micro-electrode is low, this can be offset by an improved signal to noise ratio if an array of hundreds or thousands of individual micro-electrodes is used. This is because the signal to noise ratio increases as the square root of the number of individual micro-electrodes.

25

Reference will now be made, by way of non-limitative example, to the accompanying drawings in which:-

Figure 1 is a plan view of a biosensor according to a first

embodiment of the invention.

Figure 2 is a plan view of a biosensor according to a second embodiment of the invention.

5

Figure 3 is a plan view of part of a micro-electrode array.

Figure 4 is a sectional side view along the line A-A in Figure 3.

10

Figure 5 is an exploded perspective view of a biosensor according to a third embodiment.

Figures 6a-c show successive steps of one way to make the dielectric coating.

Figure 7 is a perspective view of a fourth embodiment.

Figures 1, 3 and 4 show a first embodiment of the invention. This embodiment is a compact device of size comparable to an integrated circuit package which exploits the advantages of micro-electrode sensors with the specificity brought about by biopolymer coating of the electrode surfaces. An insulating substrate 1 has attached to it a conducting patch or area 6 as shown in Figure 3. The insulating substrate is preferably silicon. The patch 6 could in general be of any conducting material but is preferably carbonaceous.

Upon the patch 6 is a layer of dielectric material 5 which has

a plurality of pores 7 passing therethrough. The dielectric layer is preferably 0.1-0.8  $\mu\text{m}$  thick. The pores 7 present in this coating layer reveal the carbon surface 6 beneath it. This array of pores constitutes an array of micro-electrodes. 5 The conducting layer 6 and dielectric layer 5 are together denoted by the numeral 2 in Figure 1.

Each pore advantageously has a diameter or diagonal (if square) of dimensions in the range 1 to 10  $\mu\text{m}$ , although pores 10 down to, say, 0.2  $\mu\text{m}$  are possible. Individual pores are desirably separated by a distance of 10-100  $\mu\text{m}$  to ensure that each micro-electrode behaves independently of its neighbours. Thus the patch 2 may comprise hundreds or even thousands of micro-electrodes.

15

The insulating substrate may be mounted on to a standard integrated circuit carrier (not shown) and wire bond connections 12 may be made between bonding pads 4 on the insulating substrate and output pins on the carrier (not 20 shown).

As shown in Figure 1, a counter electrode 3 is attached to the insulating substrate so that when a fluid sample to be analyzed is placed on the biosensor, a connection is formed 25 between the conducting surface 6 and counter electrode 3.

In order for the biosensor to provide results about the presence of a specific compound, the pores are "functionalised" with a biopolymer.

The biopolymer is chosen to convert a biochemical response in a liquid sample into a quantifiable and processable electrical signal. In some cases, it is desirable to provide a permeable  
5 membrane (not shown) to cover the assembly.

The top working surface of the device is surrounded by a small polymer wall 13 such that a drop of liquid sample can be placed over the pores and retained there.

10

Figure 2 shows a second embodiment of the invention. In most respects the structure is identical to that of Figure 1. However, here there are two counter electrodes 3 and eight 2mm square patches of micro electrodes 2.

15

A third embodiment of the invention is shown in Figure 5. This embodiment is particularly suited to applications where a compound to be assessed is excreted through the skin, for example perspiration. Lower layer 1 of Figure 5 may consist  
20 of a thin conducting film deposited onto a plastic substrate. Typically the substrate is made of a silicone polymer or PET (polyethylene terephthalate) and the conducting film is carbon based. An electrical connection 11 to this base layer is preferably made at the edge of the structure. The conducting  
25 film has thereover a holey insulating dielectric layer 5, as in the previous two embodiments.

The second layer 10 is a porous membrane or layer to provide a "reservoir" for retaining the analyte, and to provide a



"spacer" between the functionalised electrode and the counter electrode. This layer can be made from any suitable material, ranging from a thin cellulose filter paper to a thicker fibrous polymer mat. In use, the layer retains the analyte as  
5 it is assessed.

The upper layer 9 of Figure 5 is a perforated conducting layer or sheet, typically a metal coated plastic film. The perforations 14 permit the infusion of the liquid that is to  
10 be analyzed. These should be of sufficient size to permit capillary infusion, but not so large as to permit damage to the integrity of the structure. These perforations 14 could also perform a secondary function, namely to keep large cellular structures from interfering with the electrochemical  
15 cell. The perforations 14 may advantageously be produced using a suitable spiked roller. The size of these holes will typically vary from 1 micron diameter to (say) 100 microns. Electrical connection may be made to the metal under surface of the film. The metal could be gold, or any other  
20 appropriate metal. It could be advantageous to include a reference electrode in the form of, e.g., an Ag/AgCl layer, thus providing a familiar electrochemical reference.

The sandwich structure of this embodiment may be laminated,  
25 e.g. by a standard office laminator. Typically, a temperature of 85°C would be used during lamination if the plastic film material is PET for example. Alternatively, the layers may be adhered together using any suitable adhesive.

One of the important attributes of this embodiment is that it is inherently manufacturable, since it consists of three parts only that can be easily made and joined together. The lower layer can also be functionalised with a wide variety of  
5 enzymes.

Of course, the lower layer could comprise an array of patches  
2 as in the second embodiment.

10 Figure 7 shows a fourth embodiment of the invention that takes the form of a wire or filament. Here, the substrate 1, the conducting area 6 and the dielectric ink 5 are wrapped in a cylindrical configuration. The counter electrode is not shown.

15

In each embodiment, the conducting area 6 may be formed by a conventional technique such as screen printing, spin or dip coating, meniscus coating or spray coating an ink, for example.

20

Alternatively the layer can be formed in situ by chemical reaction, for example by heating a carbonaceous material to convert it to carbon. Thus it may be formed by spin coating a concentrated solution of sugar such as glucose, mixed with a  
25 catalyst, followed by heat treatment up to 900°C to carbonize the layer. The catalyst typically is 5% by weight of zinc chloride and with this process a highly conductive (resistivity of about 0.2 ohm cm) glassy film of carbon of around a micron in thickness is formed on the substrate.

30

Similarly, the dielectric area 5 may be formed by conventional techniques, e.g. from silicon nitride using standard semiconductor processing techniques, or by the use of a commercially available dielectric ink.

5

The pores 7 may be formed by conventional means, e.g. by photolithography when the dielectric layer is applied, or afterwards by laser or energetic particle bombardment or by means of a particulate fluid as described in more detail

10 below.

Functionalisation or activation of the micro-electrodes with biopolymers can be done by various methods. When carbon surfaces are used as the conducting surfaces, the biopolymer may be immobilised on the carbon surface directly. Preferably it is covalently bonded to the carbon surface, although simple physical absorption is also possible, particularly for disposable devices. However, in general, it is usual to either modify the surface e.g. by oxidation to produce negatively charged sites that interact with positively charged sites on the enzyme or to attach a layer of linker molecules to the conducting surface to facilitate charge transfer between the electrode and the biopolymer. This can be further modified by changing the concentration of positively charged cations in the environment, for example by having present a cationic species, poly L-lysine. This is generally necessary when the conducting surface is of a metal such as gold or copper-Kapton (polyimide) or other metal-on-polymer film that can be patterned by photographic/electrolytic methods.

25

A typical linker molecule might be poly L-lysine. The chosen biopolymer can be introduced on to the conducting patch via a capillary probe using a modified probe station. Generally, the biopolymer is mixed in a buffer solution before application to the patch. The concentration of the biopolymer in the buffer solution is not critical but is suitably sufficient to give a monolayer coverage of the micro electrode surface.

10 If made thin enough, each embodiment can give a flexible multi-micro electrode assembly that can be applied directly to the skin, for example. In some instances, the flexible biosensor may be kept in place on the skin using an adhesive. This type of sensor is ideal for the detection of substances in body fluid.

Each device is designed to be plugged into an electrochemical potentiostat. Usually, a constant potential difference would be applied between the counter electrode 3 and carbon patch 2. The current that flows between them (i.e. through the liquid to be assessed) can then be measured. Potential differences up to 1V can generally be used. However, any voltage of at least about 150mV is usually sufficient to ensure that operation occurs in a desirable area of the current-voltage characteristic curve where the current reaches a "plateau". Typical currents to be measured are in the range of 0.1 to 1nA so that they can be measured using standard equipment.

The structure of the second embodiment shows improved

flexibility over the first embodiment. On the one hand, eight different biopolymers could be employed, one on each patch, to detect eight different analytes, or alternatively each patch could be activated with the same biopolymer and eight different types of electrochemical measurements made simultaneously. Manifestly, the number of micro-electrode arrays could be more or less than eight.

Each embodiment will permit the use of mediated enzyme action i.e.: a mediator such as ferrocene can be associated with the biopolymer to act as a "shuttle" molecule in order to facilitate the transfer of electrons from the biopolymer to the conducting surface although the preferred method of expressing the electro-analytical response is by direct electron transfer between the enzyme and the micro electrode.

As discussed above, the dielectric layer 5 may be produced using any conventional technique. The following method, which also forms part of the present invention, has been found to be particularly advantageous. The conducting surface 6 is firstly coated with a plurality of particles 8 as shown in Figure 6a. The particles are sized so that their diameter is approximately the same as the required final thickness of the dielectric layer 5 and also of the pores 7. They are also applied in such numbers so as to yield the required spacing between micro electrodes. After the particles have been applied, a layer of insulator (dielectric) 5 is sprayed onto the conducting surface 6 as shown in Figure 6b.

As an alternative to this, a fluid composition containing suspended particles may be used, i.e. desirably, the particles and the fluid dielectric are premixed and are applied to the conducting substrate at the same time. Referring to Figure 6b,  
5 the alternative method comprises applying the particles 8 and fluid 5 at the same time.

Thus, a conducting electrode 6, which may be of metal e.g. gold or of carbon, carries an overlying coating layer 5 of a  
10 dielectric ink containing suspended particles 8. After drying the coating layer, the particles are removed to leave the structure shown in Figure 6c where the array of particles 8 has been replaced by an array of holes 7 which reveal the  
conducting substrate 6 and define micro-electrodes. The  
15 biopolymer is then applied to the pores 7 so as to functionalise the device. Of course, the biopolymer could be applied first to the bare conducting surface.

The fluid composition may be a dielectric ink, such as the  
20 commercially available materials which can be applied as a liquid by a variety of standard coating methods as described earlier and which can be cured (via either ultra-violet, chemical or heat treatment for example) to form a solid insulating dielectric layer. The suspended particles may be of  
25 glass or preferably of a polymer such as polymethylmethacrylate, polystyrene or polyethylene oxide. Alternatively the fluid composition may be in the form of an inorganic colloid. The size and volume fraction of the particles in the dielectric ink determine the diameter and

frequency of the micro-electrodes in the array.

When the particles are water soluble they can be removed by dissolution. If they have a lower combustion point than the dielectric, they can be removed by ashing in an oven or plasma reactor.

In the most preferred method, the dielectric coating 5 comprises a layer of silica which may be formed using a sol-gel layer made from tetraethylorthosilicate (TEOS). The holes 7 may be created by mixing polymer spheres 8 (preferably of polystyrene) into the gel prior to spin coating onto the glassy carbon layer 6. The gel is then heated to around 700°C which causes the polymer beads to dissociate leaving holes in the cured dielectric constituting the micro-electrodes.

20

25

CLAIMS

1. A biosensor comprising a conducting surface, a layer of  
5 dielectric material overlying the conducting surface, a  
plurality of micro electrodes constituted by a plurality of  
pores extending through the thickness of said dielectric layer,  
each pore being separated from its neighbour, a biopolymer  
positioned in said pores, and a counter electrode arranged such  
10 that electrical connection can be made between it and at least  
part of said conducting surface by a fluid to be assessed.
2. A biosensor according to claim 1 wherein said conducting  
surface comprises a carbon surface.
- 15 3. A biosensor according to claim 1 or claim 2 wherein said  
biopolymer is attached to said conducting surface via a linker  
molecule.
- 20 4. A biosensor according to any preceding claim wherein the  
biopolymer is associated with a mediator to facilitate the  
transfer of electrons from said biopolymer to said conducting  
surface.
- 25 5. A biosensor according to any preceding claim wherein said  
conducting surface comprises two or more areas of conducting  
material.
6. A biosensor according to claim 5 wherein said areas of



conducting material are arranged in a substantially uniform formation.

7. A biosensor according to any preceding claim wherein the  
5 biosensor is flexible.
8. A biosensor according to any preceding claim further comprising means for retaining said fluid in said pores.
- 10 9. A biosensor according to any preceding claim wherein said conducting surface and said counter electrode are arranged on a single insulating substrate.
10. A biosensor according to any one of claims 1-8, wherein  
15 said counter electrode comprises a perforated conducting sheet.
11. A biosensor according to claim 8 and 9 wherein said means for retaining said fluid comprises a polymer wall.
- 20 12. A biosensor according to claim 8 or claim 9 when appendant to claim 8, wherein said means for retaining said fluid comprises a layer of permeable material.
13. A biosensor according to claims 10 and 12 wherein the  
25 layer of permeable material is between the perforated conducting sheet and the dielectric layer .
14. A biosensor according to any preceding claim wherein said biopolymer is an enzyme.

15. A biosensor constructed and arranged substantially as hereinbefore described with reference to any one of Figures 1-5 of the accompanying drawings.
- 5 16. A method of making a biosensor comprising the steps of:  
providing a conducting surface;  
providing a layer of dielectric material adjacent to said conducting surface, said dielectric material comprising a plurality of pores extending through the thickness of the  
10 dielectric layer; each pore being separated from its neighbour;  
providing a biopolymer in said pores; and  
providing a counter electrode insulated from said conducting surface.
- 15 17. A method according to claim 16, wherein a substrate layer is provided adjacent to said conducting layer.
18. A method according to claim 16 or claim 17 further comprising the step of providing a layer of permeable material  
20 adjacent to said dielectric layer.
19. A method according to claim 18 further comprising the step of adhering said layers together.
- 25 20. A method according to any one of claims 16-19, wherein the layer of dielectric material is made by applying to said conducting surface particles of substantially the same diameter as said pores;  
applying a dielectric in the form of a fluid containing

it to said conducting surface;

allowing said fluid to dry; and

removing said particles.

5 21. A method according to claim 20 wherein said particles and said fluid dielectric are premixed and are applied to said conducting substrate at the same time.

22. A method according to claim 20 or claim 21, wherein said  
10 particles are water soluble and are removed by dissolution in water.

23. A method according to claim 20 or claim 21, wherein said particles are removed by heat treatment.

15

24. A method according to any one of claims 16-23, wherein the biosensor is one claimed in any one of claims 1 to 15.

25. A method of making a biosensor substantially as  
20 hereinbefore described with reference to Figure 6 of the accompanying drawings.

26. A biosensing system comprising:

a current measuring device;

25 a potential difference generator; and

a biosensor as claimed in any one of claims 1-15 or when made by a method of any one of claims 16-25;

wherein said potential difference is applied between the counter electrode and the conducting surface of said biosensor

and,

said current measuring device is used to measure a current flowing between said counter electrode and said conducting surface.

5

Fig.1.

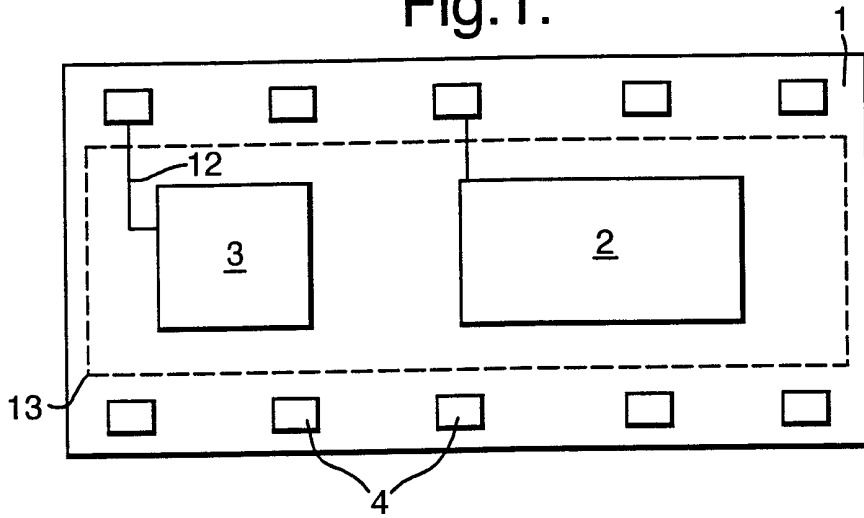


Fig.2.

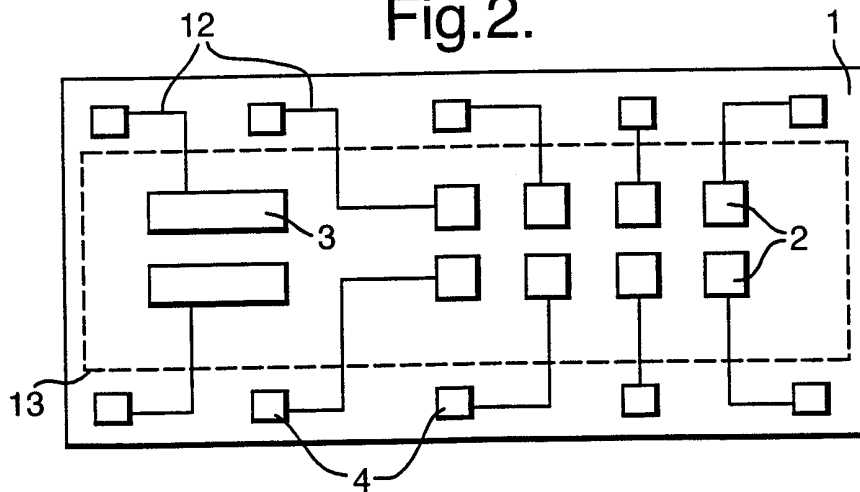


Fig.3.

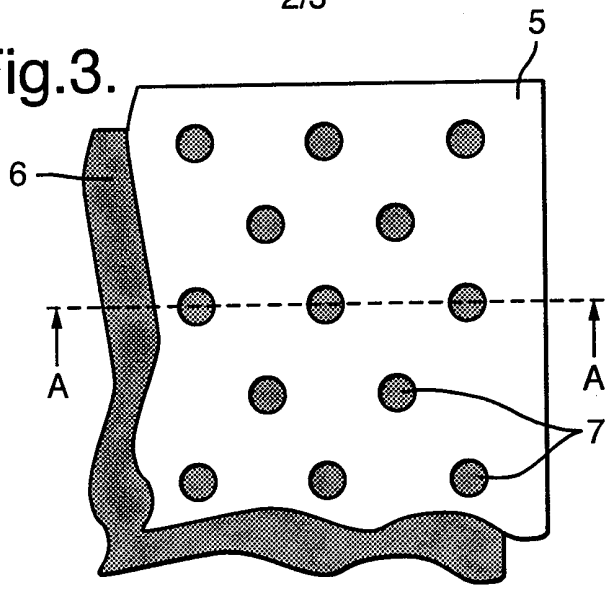


Fig.4.

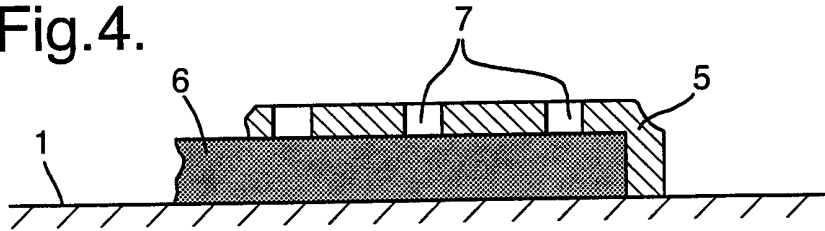


Fig.5.

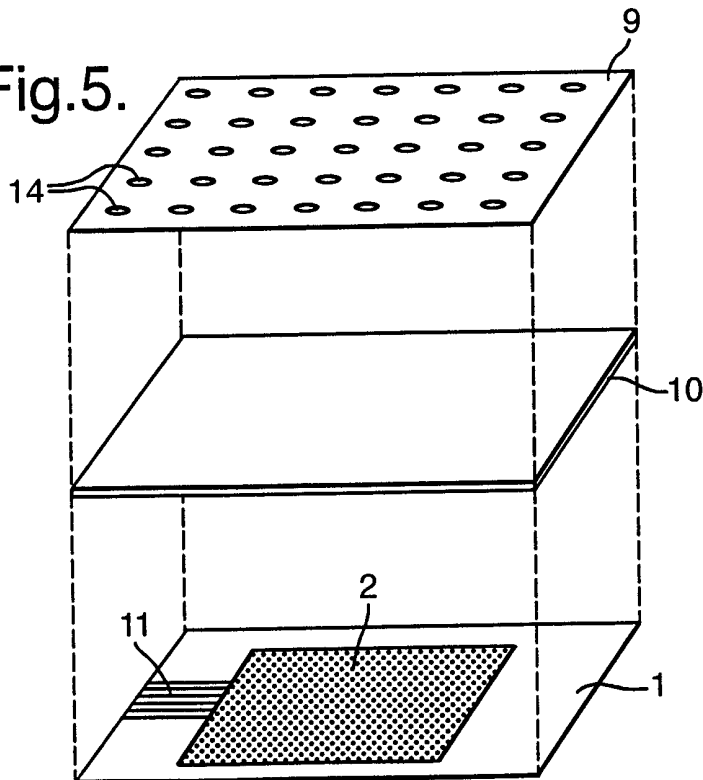


Fig.6a.

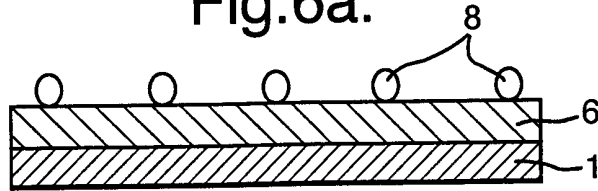


Fig.6b.

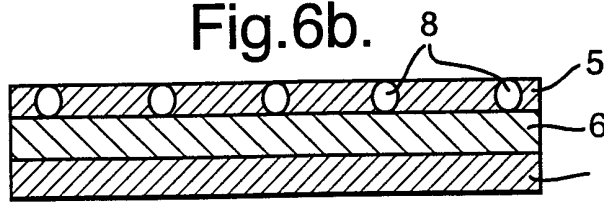


Fig.6c.


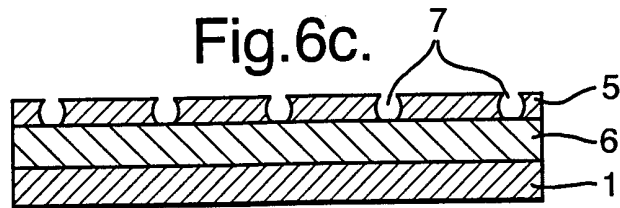


Fig.7.

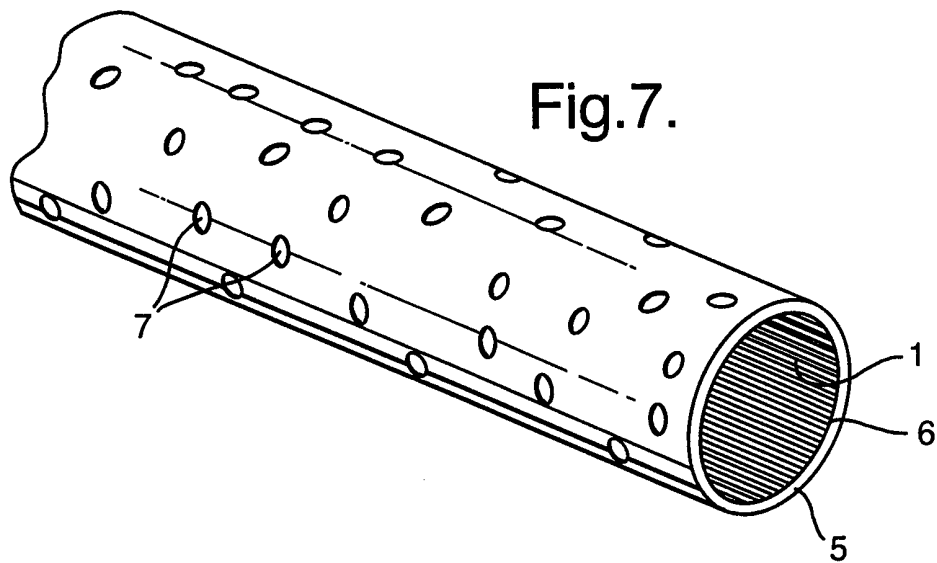

# INTERNATIONAL SEARCH REPORT

International Application No  
PCT/GB 99/01425

## A. CLASSIFICATION OF SUBJECT MATTER

G 01 N 27/327

According to International Patent Classification (IPC) or to both national classification and IPC 6

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G 01 N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4908115 A (MORITA et al.) 13 March 1990.	1, 16, 26
A	GB 2217461 A (UK ATOMIC ENERGY AUTHORITY) 25 October 1989.	1, 16, 26

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

### \* Special categories of cited documents :

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \* & \* document member of the same patent family

Date of the actual completion of the international search

21 July 1999

Date of mailing of the international search report

- 1. 09. 99

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+ 31-70) 340-2040, Tx. 31 651 epo nl,  
Fax (+ 31-70) 340-3016

Authorized officer

NARDAI e.h.



**ANHANG**

zum internationalen Recherchenbericht über die internationale Patentanmeldung Nr.

**ANNEX**

to the International Search Report to the International Patent Application No.

**ANNEXE**

au rapport de recherche international relatif à la demande de brevet international n°

PCT/GB 99/01425 SAE 233799

In diesem Anhang sind die Mitglieder der Patentfamilien der im obengenannten internationalen Recherchenbericht angeführten Patentdokumente angegeben. Diese Angaben dienen nur zur Unterrichtung und erfolgen ohne Gewähr.

This Annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report. The Office is in no way liable for these particulars which are given merely for the purpose of information.

La présente annexe indique les membres de la famille de brevets relatifs aux documents de brevets cités dans le rapport de recherche international visée ci-dessus. Les renseignements fournis sont donnés à titre indicatif et n'engagent pas la responsabilité de l'Office.

In Recherchenbericht angeführtes Patentdokument Patent document cited in search report Document de brevet cité dans le rapport de recherche	Datum der Veröffentlichung Publication date Date de publication	Mitglied(er) der Patentfamilie Patent family member(s) Membre(s) de la famille de brevets	Datum der Veröffentlichung Publication date Date de publication
US A 4908115	13-03-1990	DE C0 3776081	27-02-1992
		DK AO 6731787	21-12-1987
		DK A 6731787	22-12-1987
		DK B1 167716	06-12-1993
		EP A1 266432	11-05-1988
		EP B1 266432	15-01-1992
		WO A1 8706701	05-11-1987
		JP B4 7069289	26-07-1995
GB A1 2217461	25-10-1989	GB A0 8821369	12-10-1988
		GB A0 8905515	19-04-1989
		GB A0 8805751	07-04-1988