



(51) International Patent Classification:
A61M 5/20 (2006.01)

(21) International Application Number:
PCT/US2014/010447

(22) International Filing Date:
7 January 2014 (07.01.2014)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/750,128 8 January 2013 (08.01.2013) US

(71) Applicant: **3M INNOVATIVE PROPERTIES COMPANY** [US/US]; 3M Center, Post Office Box 33427, Saint Paul, Minnesota 55133-3427 (US).

(72) Inventors: **BURTON, Scott A.**; 3M Center, Post Office Box 33427, Saint Paul, Minnesota 55133-3427 (US). **MOECKLY, Craig S.**; 3M Center, Post Office Box 33427, Saint Paul, Minnesota 55133-3427 (US). **SIMMERS, Ryan Patrick**; 3M Center, Post Office Box 33427, Saint Paul, Minnesota 55133-3427 (US).

(74) Agents: **STEWART, Pamela L.** et al.; 3M Center, Office of Intellectual Property Counsel, Post Office Box 33427, Saint Paul, Minnesota 55133-3427 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

[Continued on next page]

(54) Title: APPLICATOR FOR APPLYING A MICRONEEDLE DEVICE TO SKIN

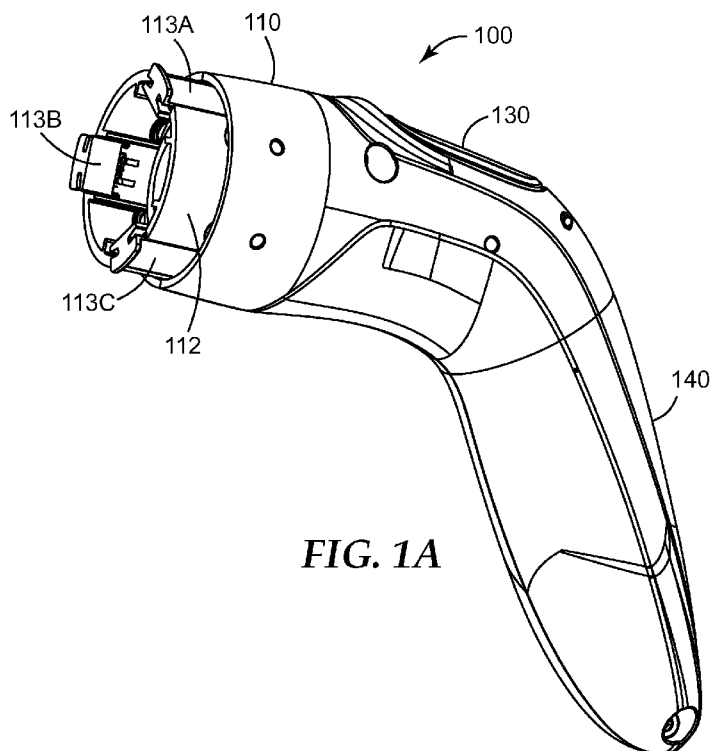


FIG. 1A

(57) Abstract: An applicator and method for applying a microneedle device to skin. The applicator can include a housing and a reciprocating support structure slidably engaged with the housing. The reciprocating support structure can have a plurality of alignment feet. The applicator can have a lockout mechanism that prevents actuation if the alignment feet are not evenly aligned. The applicator can include a device life indicator that is capable of counting the number of use cycles that the applicator has undergone and providing feedback to the user. The applicator can include a dose timer capable of determining the time that has elapsed after actuation of the device and providing feedback to the user.



(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*
- *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*

Published:

- *with international search report (Art. 21(3))*

APPLICATOR FOR APPLYING A MICRONEEDLE DEVICE TO SKIN**CROSS REFERENCE TO RELATED APPLICATIONS**

5 This application claims priority to U.S. Provisional Patent Application No. 61/750,128, filed January 8, 2013, the disclosure of which is incorporated herein by reference in its entirety herein.

FIELD

10 The present disclosure generally relates to applicators and methods for applying a microneedle device to skin to treat an area of the skin and/or to deliver an active agent to the skin.

BACKGROUND

15 Transdermal and topical drug delivery can be used for therapeutic treatment, but the number of molecules that can be effectively delivered using these routes can be limited by the barrier properties of skin. The main barrier to transport of molecules through the skin is the stratum corneum (the outermost layer of the skin).

20 A number of different skin treatment methods have been proposed in order to increase the permeability or porosity of the outermost skin layers, such as the stratum corneum, thus enhancing drug delivery through or into those layers. The stratum corneum is a complex structure of compact keratinized cell remnants separated by lipid domains. The stratum corneum is formed of keratinocytes, which comprise the majority of epidermal cells, that lose their nuclei and become corneocytes. These dead cells comprise the stratum corneum, which has a thickness of only about 10-30 microns and protects the body from invasion by exogenous
25 substances and the outward migration of endogenous fluids and dissolved molecules. Various skin treatment methods include the use of microneedles, laser ablation, RF ablation, heat ablation, sonophoresis, iontophoresis, or a combination thereof.

30 Devices including arrays of relatively small structures, sometimes referred to as microneedles or micro-pins, have been disclosed for use in connection with the delivery of therapeutic agents and other substances through the skin and other surfaces. The devices are typically pressed against the skin in an effort to pierce the stratum corneum such that the therapeutic agents and other substances can sequentially or simultaneously pass through that layer and into the tissues below. Microneedles of these devices pierce the stratum corneum upon contact, making a plurality of microscopic slits which serve as passageways through
35 which molecules of active components can be delivered into the body. In delivering an active component, the microneedle device can be provided with a reservoir for temporarily retaining

an active component in liquid form prior to delivering the active component through the stratum corneum. In some constructions, the microneedles can be hollow to provide a liquid flow path directly from the reservoir and through the microneedles to enable delivery of the therapeutic substance through the skin. In alternate constructions, active component(s) may be coated on the microneedle array and delivered directly through the skin after the stratum corneum has been punctured.

Microneedle arrays and patches can be deployed with an applicator device capable of being used a number of different times. The microneedle arrays and patches are generally used once and then discarded. The applicator devices can be repeatedly reloaded with new microneedle arrays and patches. The present invention provides an alternative microneedle array applicator device.

SUMMARY

The present disclosure relates to applicators that can be used to treat a selected site (e.g., on skin), and/or to apply an active ingredient to the treated site.

One aspect of the present disclosure provides an applicator for applying a microneedle device. The applicator can include a housing having a first open end configured so as to accept the microneedle device and a second end configured as a graspable handle. The applicator can further include a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device and an actuation button in mechanical or electrical engagement with the driving element. The applicator can further include at least one reciprocating support structure slidably engaged with the housing, wherein the reciprocating support structure has a first position where at least a portion of it extends from the first open end of the housing by a first distance and a second position wherein the portion extends from the first open end of the housing by a second distance, the second distance being less than the first distance.

Another aspect of the present disclosure provides an applicator for applying a microneedle device where the applicator can include a housing having a first open end configured so as to accept the microneedle device and a second end configured as a graspable handle. The applicator can further include a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device and an actuation button in mechanical or electrical engagement with the driving element. The applicator can further include a device life indicator in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the device life indicator is capable of counting the number of use cycles that the applicator has undergone and, based on the number of use cycles, providing feedback to the user as to the use status of the applicator.

Another aspect of the present disclosure provides an applicator for applying a microneedle device where the applicator can include a housing having a first open end configured so as to accept the microneedle device and a second end configured as a graspable handle. The applicator can further include a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device and an actuation button in mechanical or electrical engagement with the driving element. The applicator can further include a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that has elapsed after actuation of the device and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.

Other features and aspects of the present disclosure will become apparent by consideration of the detailed description and accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1A is a perspective view of an applicator according to one embodiment of the present disclosure.

FIG. 1B is a side cross sectional view of an applicator according to one embodiment of the present disclosure.

FIG. 2A is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure.

FIG. 2B is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator is in contact with a microneedle device in a priming fixture.

FIG. 2C is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator is in contact with a microneedle device in a priming fixture.

FIG. 2D is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator has been primed.

FIG. 2E is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator is in contact with a skin surface, but prior to actuation.

FIG. 2F is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator employs magnetic attachment means.

FIG. 3A is a side partial cross sectional view of an applicator in contact with a priming fixture according to one embodiment of the present disclosure.

FIG. 3B is a perspective view of microneedle device and a priming fixture according to one embodiment of the present disclosure.

5 **FIG. 3C** is a side partial cross sectional view of an applicator and a priming fixture according to one embodiment of the present disclosure.

FIG. 4 is a top partial cross sectional view of an applicator according to one embodiment of the present disclosure.

10 **FIG. 5** is a side partial cross sectional view of an applicator according to one embodiment of the present disclosure.

FIG. 6A is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator is in contact with a microneedle device in a priming fixture.

15 **FIG. 6B** is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator has been primed.

FIG. 6C is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator has been lifted away from a priming fixture.

20 **FIG. 6D** is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator is in contact with a skin surface, but prior to actuation.

25 **FIG. 6E** is a side partial cross sectional view of the lower, skin-contacting portion of an applicator according to one embodiment of the present disclosure, where the applicator has been actuated.

FIG. 7 is a close-up side elevational view of a microneedle array (shown with the microneedles pointing upwardly).

FIG. 8 is a perspective view of a microneedle device according to one embodiment of the present disclosure.

30 **FIG. 9** is schematic flow-chart of the process by which a device life indicator functions for an applicator according to one embodiment of the present disclosure.

FIG. 10A-F are side elevation views of device life indicators and dose timer countdown features according to various embodiments of the present disclosure.

35 **FIG. 11** is a side elevation view a device life indicator and dose timer countdown feature according to one embodiment of the present disclosure.

FIG. 12A is perspective view of a priming a priming fixture according to one embodiment of the present disclosure.

FIG. 12B is a side cross-sectional view of a priming fixture according to one embodiment of the present disclosure.

5

DETAILED DESCRIPTION

Before any embodiments of the present disclosure are explained in detail, it is to be understood that the invention is not limited in its application to the details of construction and the arrangement of components set forth in the following description or illustrated in the following drawings. The invention is capable of other embodiments and of being practiced or of being carried out in various ways. Also, it is to be understood that the phraseology and terminology used herein is for the purpose of description and should not be regarded as limiting. The use of “including,” “comprising,” or “having” and variations thereof herein is meant to encompass the items listed thereafter and equivalents thereof as well as additional items. Unless specified or limited otherwise, the term “coupled” and variations thereof are used broadly and encompass both direct and indirect couplings. Furthermore, terms such as “front,” “rear,” “top,” “bottom,” “upward,” “downward,” “under,” and the like are only used to describe elements as they relate to one another, but are in no way meant to recite specific orientations of the apparatus, to indicate or imply necessary or required orientations of the apparatus, or to specify how the invention described herein will be used, mounted, displayed, or positioned in use.

The present disclosure generally relates to an applicator and method for applying a microneedle device, comprising an array of microneedles, to skin (or a biological membrane) to treat the skin (i.e., create small holes or perforations or micropores in the skin) and/or to deliver an active agent to the skin.

In one embodiment, as shown in **FIGS. 1-2**, an applicator **100** has a lower housing **110** and an upper housing or handle **140**. The lower housing **110** has an internal cavity **115** with an opening **111** at its lower end. The upper end of the lower housing **110** connects to the handle **140**. The lower housing **110** is configured to accommodate a driving element **120**, such as a piston; a reciprocating support structure, such as a reciprocating collar **112**; a piston latch **124**, reciprocating collar spring **118**; and rocker arms **116A,B**. Alignment feet **113A,B,C**, are in sliding engagement with the reciprocating collar **112**.

The opening **111** and internal cavity **115** are sized so as to allow a microneedle device **106** to be placed inside of the internal cavity. As described in more detail below, the microneedle device **106** will include a microneedle array and may also include other structures or components, such as a backing film and/or adhesive. The reciprocating collar **112** is

35

movable between a first, extended position (as shown in **FIGS. 2A** and **2D**) and a second, retracted position (as shown in **FIG. 2C**). When the reciprocating collar **112** is in the first, extended position, the collar spring **118** urges the collar **112** to its outermost position. The collar **112** is retained within the lower housing **110** by the interaction of collar stop **127** and mechanical stop **121** on the inside of the lower housing **110** which prevents the collar **112** from being ejected from the housing.

As shown in **FIG. 2A**, the applicator **100** is in a first configuration where the piston **120** extends out of the lower housing **110** and just beyond the outer, optionally skin-contacting, edge **114** of the reciprocating collar **112**. The piston **120** is urged outward by driving spring **132** while being retained within the lower housing **110** by the interaction between piston hook **123** and the top of the piston track **125**. In this first configuration the applicator **100** can be brought into contact with a priming fixture **150** upon which a microneedle device **106** is supported. The priming fixture **150** is configured such that the microneedles **108** of the microneedle device **106** face downward, that is, away from the piston face **122**, but are protected from damage. This may be accomplished by having the microneedle device **106** rest on contact surfaces of the priming fixture **150** that contact a portion of the microneedle device **106** that is free of microneedles **108**, thus allowing the microneedles **108** to be suspended in one or more cavities formed in the priming fixture **150**.

In one embodiment, the microneedle device **106** may be provided to a user with a protective cover **156** that protects the microneedle device **106** and in particular the microneedles **108** during storage (see **FIGS. 3B-C**). The cover **156** has protective contact surfaces **152**, **153** that support the microneedle device **106** and allow the microneedles **108** to be suspended in cavity **154**. The cover **156** is sized and shaped so that it may slide in the direction of arrow **A** onto the priming fixture **150**. The cover **156** has an extending lip **157** that mates with a slot **158** in the priming fixture **150**. After the applicator **100** has coupled with the microneedle device **106** (as shown in **FIG. 3A**) and been lifted away from the priming fixture (as shown in **FIG. 3C**), the protective cover **156** remains coupled to the priming fixture **150**. In one embodiment, the protective cover **156** may then be subsequently removed from the priming fixture **150** so that the priming fixture **150** may be reused with another microneedle device **106**. Examples of suitable protective covers are described in more detail in U.S. Patent Application Publication No. US 2010/0256568 A1 (Frederickson et al.), the disclosure of which is incorporated herein by reference.

In one embodiment, the microneedle device **106** may be provided to a user already mounted on the priming fixture **150**, in which instance the priming fixture **150** also serves as a protective cover for the microneedle device **106** during storage.

In one embodiment, the portion of the priming fixture **150** that contacts the microneedle device **106** may comprise narrow pins **159A,B,C** that extend above the cavity **154** as shown in **FIGS. 12A, B**. Minimizing the area of contact between priming fixture **150** and microneedle device **106** is particularly advantageous when the surface of the microneedle device **106** facing the priming fixture **150** has an exposed pressure sensitive adhesive. Minimization of the contact area allows for the microneedle device to be easily removed from the priming fixture **150** when it is temporarily affixed to the applicator **100** (as described in greater detail below).

Although described with relation to a priming fixture **150**, the applicator **100** of the present invention may be coupled to the microneedle device **106** and primed by other methods. For example, a user could manually grasp the microneedle device **106** and attach it to the piston face **122** or the applicator **100** could come preloaded with a microneedle device **106** during initial manufacture. Likewise, the piston **120** could be primed by manually pressing on a portion of the microneedle device **106**, preferably a portion of the microneedle device **106** without protruding microneedles, in order to compress the driving spring **132** and lock it into its primed position as described below.

In use, a user will grasp the applicator **100** by the upper housing (or handle) **140** and bring the applicator **100** into contact with the priming fixture **150** so that the outer edge **114** of the reciprocating collar **112** contacts the base of the priming fixture **150** and the piston **120** is partially retracted into the internal cavity **115** of the lower housing **110**. The driving spring **132** will be partially compressed, thereby causing the piston to press with a predetermined force against the microneedle device **106** (that depends on the spring strength and the height of the priming fixture) that assists in temporarily attaching the microneedle device **106** to the piston face **122**. Various methods of attachment may be used, including, but not limited to, press-fit or friction-fit engagement, snap-fit engagement, magnets, hook-and-loop fasteners, and adhesives, or combinations thereof.

In one embodiment a relatively weak adhesive is used, such that the microneedle device **106** is bonded sufficiently to the piston face **122** to allow it to be retracted into the applicator **100**, but after the applicator **100** is activated and the microneedle device **106** attaches to a skin surface (as described in further detail below), the bond between microneedle device **106** and skin is greater than the bond between microneedle device **106** and piston face **122**, thus allowing the microneedle device to be easily detached from the piston face **122**.

In one embodiment, a small permanent magnet **148** (shown in **FIG. 2F**) is placed inside the piston **120** and just above the piston face **122**. The microneedle device **106** may have a thin metallic foil placed in or on the upper surface of the microneedle device, thus allowing it to be temporarily attached to the piston face **122**.

Following alignment with the priming fixture **150** and temporary attachment of the microneedle device **106** to the piston face **122**, the applicator **100** is pressed further downwards. The resulting compression of the collar spring **118** allows the reciprocating collar **112** to slide into the housing **110** (as shown in **FIG. 2C**) into a second, retracted position. In this position, the rocker arms **116A,B** are compressed between the collar **112** and the piston **120** with a first rocker arm extension member **135** pressed up against the interior of the collar **112** and a second rocker arm extension member **136** pressed up against the exterior of the piston **120**. In this configuration, the rocker arms **116A,B** do not impede motion of either collar **112** or piston **120**. The microneedle device **106** is also temporarily coupled to the piston face **122**. The piston hook **123** slides over the piston catch **124**. Piston contacts **146A,B** are brought into contact with housing contacts **147A,B** which sends a signal to logic board **184** to indicate that the piston **120** is fully retracted. The logic board **184** sends a signal to the solenoid **180** causing the upper end **182** of the solenoid **180** to push in the direction of the arrow **A** thereby causing the piston catch **124** to mate with the piston hook **123** and thus holding the piston **120** in its fully retracted state where the driving spring **132** is fully compressed. The applicator **100** may further provide an optional user feedback signal to inform the user that the piston **120** has been latched to the housing and that the driving spring **132** is fully compressed.

Although attachment of the microneedle device **106** to the piston face **122** and priming are described as sequential steps above, in principle they could occur simultaneously. That is, the force between microneedle device **106** and piston face **122** would only become sufficient to achieve temporary attachment when the driving spring **132** was fully compressed in its primed position. In practice, however, it is preferable that the force necessary to achieve this temporary attachment is less than the force needed to fully compress and prime the driving spring **132**, so as to ensure attachment of the microneedle device **106** to the piston face **122**.

As the applicator **100** is lifted from the priming fixture **150** the collar spring **118** expands back towards its initial state (as shown in **FIG. 2D**). As the collar **112** moves downward in the lower housing **110** the rocker arms **116A,B** and in particular the rocker arm latches **117A,B** are biased away from the piston **120** and the rocker arm latches **117A,B** hook onto the upper edge of the collar **112**. The microneedle device **106**, now coupled to the piston face **122**, is retracted into the internal cavity **115** of the lower housing **110**.

The collar **112** is retained within the lower housing **110** by the interaction of collar stop **127** and mechanical stop **121** on the inside of the lower housing **110** which prevents the collar **112** from being ejected from the housing.

It will be readily appreciated that the ability of the collar **112** to slide into the housing **110** into a second, retracted position allows for use of a relatively low-profile priming fixture

150, while still allowing the piston face **122** to contact and couple to the microneedle device **106** held in the priming fixture. Use of a low-profile priming fixture **150** may be advantageous as it can allow for more compact packaging and even offer the possibility of packaging each microneedle device **106** with its own priming fixture **150**, rather than using a reusable priming fixture.

As shown in **FIG. 2D**, the applicator **100** is loaded and primed and ready to be applied to a patient. In this configuration the piston **120** is coupled to the piston catch **124** via the piston hook **123**. The collar **112** is fixed in its extended position, since it is prevented from moving up into the housing **110** by its interaction with the rocker arm latches **117A,B** and it is prevented from moving further outward from the housing **110** by its interaction with mechanical stop **121**. Thus the collar **112** acts as if it is rigidly attached to the housing **110**. Also shown in **FIG. 2D** is alignment foot **113B** which is biased to partially extend from the internal cavity **115** formed by the collar **112**. Alignment foot **113B** is one of 3 alignment feet **113A,B,C** in this embodiment.

In order to deploy the microneedle device **106**, the user will move the outer edge **114** of the collar **112** towards a skin surface **170**. In doing this the alignment feet **113A,B,C** will first come into contact with the skin surface **170** and retract into the internal cavity **115** formed by the collar **112** as the user presses the applicator **100** closer to the skin surface **170**. Each alignment foot **113A,B,C** has an electrical contact **133** which can contact a complementary contact in the applicator housing and thus send a signal to the logic board **184** when the alignment foot is sufficiently retracted. If one or more of the alignment feet is not sufficiently retracted (and thus not sending a signal to the logic board **184**), then the applicator **100** will be prevented from applying the patch by disabling the piston release mechanism (described in further detail below). The requirement for retraction of all three alignment feet **113A,B,C** minimizes the chance that the applicator **100** could be inadvertently activated before it is brought into contact with the skin surface of a patient. In addition, the requirement for retraction of all three alignment feet **113A,B,C** helps to ensure that the applicator **100** is held firmly against the skin surface **170** and held generally perpendicular to the skin surface **170** prior to applying the microneedle device **106** to the skin surface **170**.

In one embodiment, as shown in **FIG. 2E**, it is desired that the alignment feet **113A,B,C** must be fully retracted into the housing before allowing for activation. This allows the outer edge **114** of the applicator **100** to contact the skin surface **170** before or essentially simultaneously with the signals sent to the logic board **184** which allow for activation of the applicator **100**.

In one embodiment, a visual indicator **137**, visible through an indicator window **134**, would light up, green for instance, to indicate to the user that the alignment feet are all retracted and that the device is ready to be actuated. Alternatively, the visual indicator could change color, from red to green for instance, to indicate to the user that the alignment feet are all retracted and that the device is ready to be actuated.

The user actuates the applicator **100** by pressing on the actuator button **130**, which causes the actuator button **130** to rotate about the actuator button pivot **131**. The actuator button **130** rotates into contact with the actuator contact **138** which causes a signal to be sent to the logic board to indicate that the actuator button **130** has been depressed. When the logic board simultaneously receives the signals indicating that the alignment feet **113A,B,C** are properly retracted and the actuator button **130** is depressed, then it sends a signal to solenoid **180** causing the upper end **182** of the solenoid **180** to rotate the piston release lever **142** about the piston release lever pivot **144** in the direction as shown by arrows **B**. This rotational movement causes piston catch **124** to disengage from the piston hook **123**, thus allowing the piston **120** to be biased out of the housing **110** by the driving spring **132** and thereby applying the microneedle device **106** to the skin surface. The user then lifts the applicator **100** away from the skin surface **170** and the applicator **100** will be in its “free” state as shown in **FIG. 2A**.

In one embodiment, the microneedle device **106** will have a skin-facing adhesive that causes the microneedle device **106** to adhere to the skin surface **170** with a force greater than the connection force between the microneedle device **106** and the piston face **122**. Thus the microneedle device **106** will detach from the piston face **122** when the user lifts the applicator **100** away from the skin surface **170**, thereby allowing the microneedle device **106** to remain for an extended period of time on the skin surface **170**. In an alternative embodiment, the microneedle device **106** will remain attached to the piston face **122** when the user lifts the applicator **100** away from the skin surface **170** and the microneedle device **106** can subsequently be manually removed from the piston face **122** and disposed of by the user prior to reusing the applicator **100**.

Power to the logic board **184**, visual indicator **137**, solenoid **180**, and any other electrical components of the device is provided by battery **190**.

In another embodiment, as shown in **FIGS. 4-6**, an applicator **400** has a lower housing **410** and an upper housing or handle **440**. The lower housing **410** has an internal cavity **415** with an opening **411** at its lower end. The upper end of the lower housing **410** connects to the handle **440**. The lower housing **410** is configured to accommodate a driving element **420**, such as a piston; reciprocating support structures **412A,B,C,D**; a piston latch **424**, reciprocating support structure springs **418A,B,C,D**; and rocker arms **416A,B,C,D**. The reciprocating

support structures **412A,B,C,D** are also referred to below as alignment arms. Likewise, the reciprocating support structure springs **418A,B,C,D** are also referred to below as alignment arm springs.

5 It should be understood that **FIGS. 4-6** show a variety of cross-sectional or partial cut-away views of the applicator **400** and as such only one or two alignment arms **412A,B,C,D** and only one or two alignment arm springs **418A,B,C,D**, etc. are shown in **FIGS. 4-6**, but the applicator **400** described in **FIGS. 4-6** has 4 alignment arms and 4 alignment arm springs, some of which are not shown in the various partial views.

10 The opening **411** and internal cavity **415** are sized so as to allow a microneedle device **106** to be placed inside of the internal cavity. The reciprocating alignment arms **412A,B,C,D** are movable between a first, extended position (as shown in **FIGS. 6A** and **6C**) and a second, retracted position (as shown in **FIG. 6B**). When the reciprocating alignment arms **412A,B,C,D** are in the first, extended position, the alignment arm springs **418A,B,C,D** urge the alignment arms **412A,B,C,D** to their outermost position. The alignment arms **412A,B,C,D** are retained
15 within the lower housing **410** by a mechanical stop (not shown) on the inside of the lower housing **410** that prevents the alignment arms **412A,B,C,D** from being ejected from the housing. As shown in **FIG. 6A**, the applicator **400** is in a first configuration where the piston **420** extends out of the lower housing **410**, but does not extend as far as the alignment arms **412A,B,C,D**. The piston **420** is urged outward by driving spring **432** while being partially
20 retained within the lower housing **410** by the extension of rocker arm **416A**. In this first configuration the applicator **400** can be brought into contact with a priming fixture **150** upon which a microneedle device **106** is resting. The priming fixture **150** is configured such that the microneedles **108** of the microneedle device **106** face downwards, that is, away from the piston face **422**, but are protected from damage. This may typically be accomplished by having the
25 microneedle device **106** rest on contact surfaces **152, 153** of the priming fixture **150** that contact a portion of the microneedle device **106** that is free of microneedles **108**, thus allowing the microneedles **108** to be suspended in one or more cavities **154** formed in the priming fixture **150** (see **FIG. 3A**).

30 In one embodiment, the microneedle device **106** may be provided to a user with a protective cover **156** that protects the microneedle device **106** and in particular the microneedles **108** during storage (see **FIGS. 3B-C**). The cover **156** is sized and shaped so that it may slide in the direction of arrow **A** onto the priming fixture **150**. The cover **156** has an extending lip **157** that mates with a slot **158** in the priming fixture **150**. After the applicator **400** has coupled with the microneedle device **106** (as shown in **FIG. 3A**) and been lifted away
35 from the priming fixture (as shown in **FIG. 3C**), the protective cover **156** remains coupled to

the priming fixture **150**. In one embodiment, the protective cover **156** may then be subsequently removed from the priming fixture **150** so that the priming fixture **150** may be reused with another microneedle device **106**. Examples of suitable protective covers are described in more detail in U.S. Patent Application Publication No. US 2010/0256568 A1 (Frederickson et al.), the disclosure of which is incorporated herein by reference.

In one embodiment, the microneedle device **106** may be provided to a user already mounted on the priming fixture **150**, in which instance the priming fixture **150** also serves as a protective cover for the microneedle device **106** during storage.

Following alignment with the priming fixture **150**, the applicator **400** is pressed downwards, that is, towards the priming fixture **150** thus achieving several results. The resulting compression of the alignment arm springs **418A,B,C,D** allows the alignment arms **412A,B,C,D** to slide into the housing **410** (as shown in FIG. 6B) into a second, retracted position and further allow the piston face **422** and microneedle device **106** to slide past the housing latches **426A,B,C,D**. The top of the piston **420** mates with the piston catch **424** and temporarily locks the two parts together. The rocker arms **416A,B,C,D** rotate up so that the rocker arm latches **417A,B,C,D** rest against the alignment arms **412A,B,C,D**. As shown, the microneedle device **106** is temporarily held against the piston face **422** by the housing latches **426A,B,C,D**. Various alternative methods of attachment may be used, including, but not limited to, press-fit or friction-fit engagement, snap-fit engagement, magnets, hook-and-loop fasteners, and adhesives, or combinations thereof.

As the applicator **400** is lifted from the priming fixture **150** the alignment arm springs **418A,B,C,D** expand back towards their initial state (as shown in FIG. 6C). The microneedle device **106**, now coupled to the piston face **422**, is retracted into the internal cavity **415** of the lower housing **410**. The applicator **400** is loaded and primed and ready to be applied to a patient. In this configuration the piston **420** is coupled to the piston catch **424** and the piston catch **424** is prevented from rotating due to its interaction with the piston catch stop **428**. The actuation button **430** is mechanically coupled to the piston catch **424** (connecting mechanism not shown) so as to be able to rotate the piston catch **424** when the actuation button **430** is depressed. Since the piston catch **424** is prevented from rotating in this configuration, then the actuation button **430** is locked in place and cannot be depressed by the user, thus preventing the applicator **400** from being inadvertently activated before it is brought into contact with the skin surface of a patient.

Upon removal of the applicator **400** away from the priming fixture **150** the alignment arms **412A,B,C,D** extend back to their first position, thus allowing for the microneedle device **106** to be recessed further within the applicator **400** away from the skin-contacting surface **414**.

It will be readily appreciated, however, that the ability of the alignment arms **412A,B,C,D** to slide into the housing **410** into a second, retracted position allows for use of a relatively low-profile priming fixture **150**, while still allowing the piston face **422** to contact and couple to the microneedle device **106** held in the priming fixture. Use of a low-profile priming fixture **150** may be advantageous as it can allow for more compact packaging and even offer the possibility of packaging each microneedle device **106** with its own priming fixture **150**, rather than using a reusable priming fixture.

In use, the skin-contacting surface **414** of the applicator **400** is brought into contact with a skin surface **470** and the applicator **400** is pressed downwards as shown in **FIG. 6D**.

The alignment arm springs **418A,B,C,D** are partially compressed, thus partially retracting the reciprocating alignment arms **412A,B,C,D** into the lower housing **410**. The alignment arms **412A,B,C,D** cannot be completely retracted into the housing **410**, however, since the rocker arm latches **417A,B,C,D** are caught by the alignment arm latch **419**, thus preventing further retraction of the alignment arms **412A,B,C,D**. In this configuration the piston catch **424** has moved downwards and no longer is engaged with the piston catch stop **428**. The device may then be actuated by pressing down on the actuation button **430** which causes the piston catch **424** to rotate, thus releasing the piston **420** which is driven against the skin surface **470** by the expansion of a driving spring (not shown) to attach the microneedle device **106** to the skin surface **470** (as shown in **FIG. 6E**). The force of the driving spring is sufficient to push the microneedle device **106**, which preferably has flexible outer edges past the housing latches **426A,B,C,D** which temporarily retained the microneedle device within the housing of the applicator **400**. In a preferred embodiment, the applicator **400** is then detached from the microneedle device **106** leaving the microneedle device **106** in place on the skin surface **470**. Because the alignment arms **412A,B,C,D** can be independently compressed, the above described mechanism will only release the piston catch **424** if all of the alignment arms **412A,B,C,D** are equally retracted into the housing **410**, thus ensuring that the applicator **400** and microneedle device **106** are aligned perpendicular to the skin surface **470** prior to actuating the applicator **400**.

In one embodiment, the applicator **400** has a battery **490** that may be used to power various electrical or electromechanical functions as described elsewhere in the specification.

Although described in detail above for a device with 4 alignment arms and 4 alignment arm springs, it should be understood that the number of alignment arms (or reciprocating support structures) may vary as desired. In one embodiment, the applicator **400** has a single reciprocating support structure that preferably has a skin contacting surface in the form of a ring. In one embodiment, the applicator **400** has a plurality of support structures, which may

also be referred to as alignment arms. It is a particular advantage of the device that when it contains two or more alignment arms, those alignment arms can be employed to ensure that the device is properly oriented with respect to the skin surface prior to actuation. In one embodiment the applicator **400** has more than two alignment arms and preferably 3 or 4
5 alignment arms. In one embodiment the applicator **400** has less than 10 alignment arms and preferably less than 5 alignment arms. In one embodiment each alignment arm will be coupled to an individual alignment arm spring.

In one embodiment, the applicator or device **200** has a device life indicator **210**. As shown in a process flow diagram in **FIG. 9**, in a first step **240** a user would power on the device
10 **200**, the device **200** would then perform an internal step **250** to check the cycle count, that is, the number of times the device **200** had been previously used. The device **200** could also optionally check the battery life of the device during step **250**. If the cycle count and battery life meet predetermined acceptance criteria, then the device life indicator **210** would indicate that the device was “READY” **220** and the device **200** will undergo an internal step **260** of
15 unlocking the device **200** so that it may be fully primed for use. For example, this may be accomplished by having the driving element or piston locked in place until the device undergoes the device check **250**. The acceptance criteria will depend upon the robustness of the device **200** and the battery. For example, as shown in **FIG. 9**, for a device intended to be used for 1000 cycles and considered to function satisfactorily if the battery has more than 10%
20 of its original charge, the device will indicate “READY” **220** if the device check **252** shows that the cycle count is less than 970 and the battery charge is greater than 10%. If the device check **254** shows that the count is between 970 and 999 and/or the battery is less than 10%, but still functioning, then the device life indicator **210** will indicate “WARNING” **222** to let the user know that the device is near the end of its usable life. If the device check **256** shows that
25 the count is greater than 999 and/or the battery charge is exhausted, then the device life indicator **210** will indicate “INOPERABLE” **224** and the device **200** will remain locked **262** such that it can’t be used further.

As described above, the device life indicator **210** provides feedback of “READY”, “WARNING”, or “INOPERABLE” **220**, **222**, **224**. It should be understood that this feedback
30 may take many other forms. For example, green, yellow, and red lights, may be used to indicate “READY”, “WARNING”, or “INOPERABLE” **220**, **222**, **224** respectively.

In one embodiment, as shown in **FIG. 10A**, the device life indicator **210** may take the form of a curved or U-shaped, “thermometer” type display. The device would initially show a full, green display to indicate that it had not been used. Over time the green color would
35 “drain” from the display to indicate that the device was partially used. As the device approached end of life the color of the device life indicator could optionally change to yellow

and finally red. Optionally, an indicator, such as an arrow, line, or bar, could move through zones colored green, yellow, and red to indicate the device status. It should be understood that any other suitable colored graphic display that changes color as the device approaches end of life or that changes the amount of color displayed as the device approaches end of life may be used as a device life indicator. Additionally, a separate device life warning could illuminate to provide additional feedback to indicate that the device was either near to end of life or at end of life.

In one embodiment, as shown in **FIG. 10B**, the device life indicator **212** may take the form of a circular, “thermometer” type display.

In one embodiment, as shown in **FIG. 10C**, the device life indicator **214** may take the form of a digital read-out indicating the percentage of useful life remaining.

In one embodiment, as shown in **FIG. 10C**, the device may include an optional battery gauge **215** to indicate the amount of usable battery life remaining.

In one embodiment, as shown in **FIG. 10D**, the device life indicator **216** may take the form of a digital read-out **216** indicating the number of remaining cycles or uses that the device may be used for.

In one embodiment, as shown in **FIG. 10E**, the device life indicator **218** may take the form of a linear “thermometer” type display.

In one embodiment, as shown in **FIG. 10F**, the device life indicator **219** may take the form individual icons with, for example, a check mark **219A** indicating that the device is ready to use, an exclamation point **219B** indicating a warning that the device is nearly at the end of life, and an ‘X’ **219C** indicating that the device is at end of life and is inoperable.

In one embodiment, as shown in **FIGS. 10A-F**, an additional dose timer **234** countdown feature can optionally be included on the device **200**. This timer **234** indicates a time, generally in minutes or seconds, that a user is to leave a microneedle device **106** in place upon the skin after application. As the device **200** is actuated to apply the microneedle device **106**, the dose timer **234** initially displays the length of time that the microneedle device **106** is to be worn by the patient prior to removal. The timer **234** then counts down to zero in order to instruct the patient or caregiver to remove the microneedle device **106** from the skin for disposal. For example, as shown in **FIG. 10A**, the dose timer **234** is indicating that the microneedle device **106** should be worn for 12 additional minutes.

In one embodiment, as shown in **FIG. 11**, the dose timer **236** takes the form of a light bar which can indicate one color, such as orange, to instruct the user that the microneedle device **106** is still being worn and a second color, such as green, to instruct the user to remove the microneedle device **106**.

Although the device life indicator **210** and dose timer **234** are described above with respect to visual representations, it should be understood that these can be replaced by or augmented with audible feedback. For example, the device can say “READY” to indicate the ready-to-fire state or it can count down the number of minutes remaining and say “Remove microneedle” when the dose timer **234** reaches zero.

Once the device **200** has been powered on **240** and undergone the device check **250**, the user may then perform the priming step **270**, which is described in more detail above. The device **200** then performs an internal step of incrementing the cycle count **280** and awaits actuation. If the device has not been actuated within a predetermined time, such as 2 minutes, then the device will beep intermittently **282** to alert the user that it is primed and ready to use. In one embodiment, if the device has still not been actuated within a second predetermined time period, such as 30 minutes, then the device will automatically power off **284**.

As described in more detail above, the user performs the step **290** of placing the device on a skin surface and presses down on the device to partially retract the alignment arms **412A,B,C,D**. The device performs an internal checking step **292** to determine if the device is aligned. If the device is not aligned, then the device is in a state **294** where the actuation button **430** will not depress and actuate the device. If the device is aligned, then the user may perform the step **296** of pressing the actuation button **430** which actuates the device and applies the microneedle device **106** to the skin. The dose timer **234**, if included, begins counting down **298** (or optionally counting up) to indicate the proper dosing period. When the dose timer **234** has counted down to zero (or optionally counted up to the full dosing time) it performs an alerting step **299** to inform the user to remove the microneedle device **106** from the skin. The device subsequently powers off **284** and returns to an idle state.

In discussing the applicators of the present disclosure, the term “downward,” and variations thereof, is sometimes used to describe the direction in which microneedles are pressed into skin, and “upward” to describe the opposite direction. However, those of skill in the art will understand that the applicators can be used where the microneedles are pressed into skin at an angle to the direction of the earth’s gravity, or even in a direction contrary to that of the earth’s gravity, and these terms are only used for simplicity and clarity to describe relative directions.

The term “transdermally,” and variations thereof, is generally used to refer to any type of delivery of an active ingredient that crosses any portion of skin. That is, transdermally can generally include systemic delivery (i.e., where the active ingredient is transported across, or substantially through, the dermis such that the active ingredient is delivered into the bloodstream), as well as intradermal delivery (i.e., where the active ingredient is transported partially through the dermis, e.g., across the outer layer (stratum corneum) of the skin, where

the active ingredient is delivered into the skin, e.g., for treating psoriasis or for local anesthetic delivery). That is, transdermal delivery as used herein includes delivery of an active ingredient that is transported across at least a portion of skin (but not necessarily all of the layers of skin), rather than merely being topically applied to an outer layer of the skin.

5 The “microneedle device” **106** can also be referred to as a “microneedle array assembly” and can include the array **107** of microneedles **108** (or, collectively, the “microneedle array” **107**) and any supporting structure or substrate used to support the microneedle array **107** and/or to couple the microneedle array **107** to other structures or components of the applicator **100**.

10 As mentioned above, in some embodiments, active ingredients or agents (e.g., drugs) can be delivered via the microneedles **108** (e.g., via solid or hollow microneedles, as described below). Examples of pharmaceutically active agents (also referred to as “drugs”) that can be incorporated into the applicators of the present disclosure are those capable of local or systemic effect when administered to the skin. Some examples include buprenorphine, clonidine,
15 diclofenac, estradiol, granisetron, isosorbide dinitrate, levonorgestrel, lidocaine, methylphenidate, nicotine, nitroglycerine, oxybutynin, rivastigmine, rotigotine, scopolamine, selegiline, testosterone, tulobuterol, and fentanyl, which are commercially available in the form of transdermal devices. Other examples include antiinflammatory drugs, both steroidal (e.g., hydrocortisone, prednisolone, triamcinolone) and nonsteroidal (e.g., naproxen, piroxicam);
20 bacteriostatic agents (e.g., chlorhexidine, hexylresorcinol); antibacterials (e.g., penicillins such as penicillin V, cephalosporins such as cephalexin, erythromycin, tetracycline, gentamycin, sulfathiazole, nitrofurantoin, and quinolones such as norfloxacin, flumequine, and ibafloxacin); antiprotazoals (e.g., metronidazole); antifungals (e.g., nystatin); coronary vasodilators; calcium channel blockers (e.g., nifedipine, diltiazem); bronchodilators (e.g., theophylline, pirbuterol,
25 salmeterol, isoproterenol); enzyme inhibitors such as collagenase inhibitors, protease inhibitors, acetylcholinesterase inhibitors (e.g., donepezil), elastase inhibitors, lipoxygenase inhibitors (e.g., A64077), and angiotensin converting enzyme inhibitors (e.g., captopril, lisinopril); other antihypertensives (e.g., propranolol); leukotriene antagonists (e.g., ICI204,219); anti-ulceratives such as H₂ antagonists; steroidal hormones (e.g., progesterone); antivirals and/or
30 immunomodulators (e.g., 1-isobutyl-1H-imidazo[4,5-c]quinolin-4-amine, 1-(2-hydroxy-2-methylpropyl)-1H-imidazo[4,5-c]quinolin-4-amine, N-[4-(4-amino-2-ethyl-1H-imidazo[4,5-c]quinolin-1-yl)butyl]methanesulfonamide, and acyclovir); local anesthetics (e.g., benzocaine, propofol, tetracaine, prilocaine); cardiotonics (e.g., digitalis, digoxin); antitussives (e.g., codeine, dextromethorphan); antihistamines (e.g., diphenhydramine, chlorpheniramine, terfenadine); narcotic analgesics (e.g., morphine, fentanyl citrate, sufentanil, hydromorphone
35 hydrochloride); peptide hormones (e.g., human or animal growth hormones, LHRH,

parathyroid hormones); cardioactive products such as atriopeptides; antidiabetic agents (e.g., insulin, exenatide); enzymes (e.g., anti-plaque enzymes, lysozyme, dextranase); anti-nauseants; anticonvulsants (e.g., carbamazepine); immunosuppressives (e.g., cyclosporine); psychotherapeutics (e.g., diazepam); sedatives (e.g., phenobarbital); anticoagulants (e.g., heparin, enoxaparin sodium); analgesics (e.g., acetaminophen); antimigraine agents (e.g., ergotamine, melatonin, sumatriptan, zolmitriptan); antiarrhythmic agents (e.g., flecainide); antiemetics (e.g., metaclopramide, ondansetron, granisetron hydrochloride); anticancer agents (e.g., methotrexate); neurologic agents such as anxiolytic drugs; hemostatics; anti-obesity agents; dopamine agonists (e.g., apomorphine); GnRH agonists (e.g., leuprolide, goserelin, nafarelin); fertility hormones (e.g., hCG, hMG, urofollitropin); interferons (e.g., interferon-alpha, interferon-beta, interferon-gamma, pegylated interferon-alpha); and the like, as well as pharmaceutically acceptable salts and esters thereof. The amount of drug that constitutes a therapeutically effective amount can be readily determined by those skilled in the art with due consideration of the particular drug, the particular carrier, and the desired therapeutic effect.

In some embodiments, peptide therapeutic agents (natural, synthetic, or recombinant) can be delivered via the microneedles 108 (e.g., via solid or hollow microneedles, as described below). Examples of peptide therapeutic agents that can be incorporated into the applicators of the present disclosure include parathyroid hormone (PTH), parathyroid hormone related protein (PTHrP), calcitonin, lysozyme, insulin, insulinotropic analogs, glatiramer acetate, goserelin acetate, somatostatin, octreotide, leuprolide, vasopressin, desmopressin, thymosin alpha-1, atrial natriuretic peptide (ANP), endorphin, vascular endothelial growth factor (VEGF), fibroblast-growth factor (FGF), erythropoietin (EPO), bone morphogenetic proteins (BMPs), epidermal growth factor (EGF), granulocyte colony-stimulating factor (G-CSF), granulocyte macrophage colony stimulating factor (GM-CSF), insulin-like growth factor (IGF), platelet-derived growth factor (PDGF), growth hormone release hormone (GHRH), dornase alfa, tissue plasminogen activator (tPA), urokinase, ANP clearance inhibitors, luteinizing hormone releasing hormone (LHRH), melanocyte stimulating hormones (alpha & beta MSH), pituitary hormones (hGH), adrenocorticotrophic hormone (ACTH), human chorionic gonadotropin (hCG), streptokinase, interleukins (e.g. IL-2, IL-4, IL-10, IL-12, IL-15, IL-18), protein C, protein S, angiotensin, angiogenin, endothelins, pentitide, brain natriuretic peptide (BNP), neuropeptide Y, islet amyloid polypeptide (IAPP), vasoactive intestinal peptide (VIP), hirudin, glucagon, oxytocin, and derivatives of any of the foregoing peptide therapeutic agents.

In some embodiments, drugs that are of a large molecular weight may be delivered transdermally. Increasing molecular weight of a drug typically can cause a decrease in unassisted transdermal delivery. Examples of such large molecules include proteins, peptides, nucleotide sequences, monoclonal antibodies, vaccines, polysaccharides, such as heparin, and

antibiotics, such as ceftriaxone. Examples of suitable vaccines include therapeutic cancer vaccines, anthrax vaccine, flu vaccine, Lyme disease vaccine, rabies vaccine, measles vaccine, mumps vaccine, chicken pox vaccine, small pox vaccine, hepatitis vaccine, hepatitis A vaccine, hepatitis B vaccine, hepatitis C vaccine, pertussis vaccine, rubella vaccine, diphtheria vaccine, encephalitis vaccine, Japanese encephalitis vaccine, respiratory syncytial virus vaccine, yellow fever vaccine, recombinant protein vaccine, DNA vaccines, polio vaccine, therapeutic cancer vaccine, herpes vaccine, human papilloma virus vaccine, pneumococcal vaccine, meningitis vaccine, whooping cough vaccine, tetanus vaccine, typhoid fever vaccine, cholera vaccine, tuberculosis vaccine, severe acute respiratory syndrome (SARS) vaccine, HSV-1 vaccine, HSV-2 vaccine, HIV vaccine and combinations thereof. The term "vaccine" thus includes, without limitation, antigens in the forms of proteins, polysaccharides, oligosaccharides, or weakened or killed viruses. Additional examples of suitable vaccines and vaccine adjuvants are described in U.S. Patent Application Publication No. 2004/0049150 (Dalton et al.), the disclosure of which is hereby incorporated by reference.

In another embodiment, small-molecule drugs that are otherwise difficult or impossible to deliver by passive transdermal delivery may be used. Examples of such molecules include salt forms; ionic molecules, such as bisphosphonates, including sodium alendronate or pamidronate; and molecules with physicochemical properties that are not conducive to passive transdermal delivery.

Microneedle arrays useful for practicing the present disclosure can have a variety of configurations and features, such as those described in the following patents and patent applications, the disclosures of which are incorporated herein by reference. One embodiment for the microneedle arrays includes the structures disclosed in U.S. Patent Application Publication No. 2005/0261631 (Clarke et al.), which describes microneedles having a truncated tapered shape and a controlled aspect ratio. Another embodiment for the microneedle arrays includes the structures disclosed in U.S. Patent No. 6,091,975 (Daddona et al.), which describes blade-like microprotrusions for piercing the skin. Still another embodiment for the microneedle arrays includes the structures disclosed in U.S. Patent No. 6,312,612 (Sherman et al.), which describes tapered structures having a hollow central channel. Yet still another embodiment for the microneedle arrays includes the structures disclosed in U.S. Patent No. 6,379,324 (Gartstein et al.), which describes hollow microneedles having at least one longitudinal blade at the top surface of the tip of the microneedle. A further embodiment for the microneedle arrays includes the structures disclosed in U.S. Patent Application Publication Nos. US2012/0123387 (Gonzalez et al.) and US2011/0213335 (Burton et al.), which both describe hollow microneedles. A still further embodiment for the microneedle arrays includes the

structures disclosed in U.S. Patent Nos. 6,558,361 (Yeshurun) and 7,648,484 (Yeshurun et al.), which both describe hollow microneedle arrays and methods of manufacturing thereof.

Various embodiments of microneedles that can be employed in the microneedle arrays of the present disclosure are described in PCT Publication No. WO2012/074576 (Duan et al.),
5 which describes liquid crystalline polymer (LCP) microneedles; and PCT Publication No. WO2012/122162 (Zhang et al.), which describes a variety of different types and compositions of microneedles that can be employed in the microneedles of the present disclosure.

In some embodiments, the microneedle material can be (or include) silicon, glass, or a metal such as stainless steel, titanium, or nickel titanium alloy. In some embodiments, the
10 microneedle material can be (or include) a polymeric material, preferably a medical grade polymeric material. Exemplary types of medical grade polymeric materials include polycarbonate, liquid crystalline polymer (LCP), polyether ether ketone (PEEK), cyclic olefin copolymer (COC), polybutylene terephthalate (PBT). Preferred types of medical grade polymeric materials include polycarbonate and LCP.

15 In some embodiments, the microneedle material can be (or include) a biodegradable polymeric material, preferably a medical grade biodegradable polymeric material. Exemplary types of medical grade biodegradable materials include polylactic acid (PLA), polyglycolic acid (PGA), PGA and PLA copolymer, polyester-amide polymer (PEA).

In some embodiments, the microneedles can be prepared from a dissolvable,
20 degradable, or disintegratable material referred to herein as “dissolvable microneedles”. A dissolvable, degradable, or disintegratable material is any solid material that dissolves, degrades, or disintegrates during use. In particular, a “dissolvable microneedle” dissolves, degrades, or disintegrates sufficiently in the tissue underlying the stratum corneum to allow a therapeutic agent to be released into the tissue. The therapeutic agent may be coated on or
25 incorporated into a dissolvable microneedle. In some embodiments, the dissolvable material is selected from a carbohydrate or a sugar. In some embodiments, the dissolvable material is polyvinyl pyrrolidone (PVP). In some embodiments, the dissolvable material is selected from the group consisting of hyaluronic acid, carboxymethylcellulose, hydroxypropylmethylcellulose, methylcellulose, polyvinyl alcohol, sucrose, glucose, dextran,
30 trehalose, maltodextrin, and a combination thereof.

In some embodiments, the microneedles can be made from (or include) a combination of two or more of any of the above mentioned materials. For example, the tip of a microneedle may be a dissolvable material, while the remainder of the microneedle is a medical grade polymeric material.

35 A microneedle or the plurality of microneedles in a microneedle array useful for practicing the present disclosure can have a variety of shapes that are capable of piercing the

stratum corneum. In some embodiments, one or more of the plurality of microneedles can have a square pyramidal shape, triangular pyramidal shape, stepped pyramidal shape, conical shape, microblade shape, or the shape of a hypodermic needle. In some embodiments, one or more of the plurality of microneedles can have a square pyramidal shape. In some embodiments, one or more of the plurality of microneedles can have a triangular pyramidal shape. In some embodiments, one or more of the plurality of microneedles can have a stepped pyramidal shape. In some embodiments, one or more of the plurality of microneedles can have a conical shape. In some embodiments, one or more of the plurality of microneedles can have a microblade shape. In some embodiments, one or more of the plurality of microneedles can have the shape of a hypodermic needle. The shape can be symmetric or asymmetric. The shape can be truncated (for example, the plurality of microneedles can have a truncated pyramid shape or truncated cone shape). In a preferred embodiment, the plurality of microneedles in a microneedle array each have a square pyramidal shape.

In some embodiments, the plurality of microneedles in a microneedle array are solid microneedles (that is, the microneedles are solid throughout). In some embodiments, the plurality of solid microneedles in a solid microneedle array can have a square pyramidal shape, triangular pyramidal shape, stepped pyramidal shape, conical shape, or microblade shape. In a preferred embodiment, the plurality of solid microneedles in a solid microneedle array each have a square pyramidal shape.

In some embodiments, the plurality of microneedles in a microneedle array are hollow microneedles (that is, the microneedles contain a hollow bore through the microneedle). The hollow bore can be from the base of the microneedle to the tip of the microneedle or the bore can be from the base of the microneedle to a position offset from the tip of the microneedle. In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have a conical shape, cylindrical shape, square pyramidal shape, triangular pyramidal shape, or the shape of a hypodermic needle.

In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have a conical shape. In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have a cylindrical shape. In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have a square pyramidal shape. In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have a triangular pyramidal shape. In some embodiments, one or more of the plurality of hollow microneedles in a hollow microneedle array can have the shape of a hypodermic needle. In a preferred embodiment, the plurality of hollow microneedles in a hollow microneedle array each have the shape of a conventional hypodermic needle.

FIG. 7 shows a portion of the microneedle array **107** that includes four microneedles **108** (of which two are referenced in **FIG. 7**) positioned on a microneedle substrate **109**. Each microneedle **108** has a height h , which is the length from the tip of the microneedle **108** to the microneedle base at substrate **109**. Either the height of a single microneedle or the average height of all microneedles on the microneedle array can be referred to as the height of the microneedle, h . In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of about 100 to about 3000 micrometers, in some embodiments, about 100 to about 1500 micrometers, in some embodiments, about 100 to about 1200 micrometers, and, in some embodiments, about 100 to about 1000 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of about 200 to about 1200 micrometers, about 200 to about 1000 micrometers, about 200 to about 750 micrometers, or about 200 to about 600 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of about 250 to about 1500 micrometers, about 500 to about 1000 micrometers, or about 500 to about 750 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of about 800 to about 1400 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of about 500.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 3000 micrometers. In other embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 1500 micrometers. In still other embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 1200 micrometers. In yet still other embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 1000 micrometers. In further embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 750 micrometers. In still further embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of less than about 600 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of at least about 100 micrometers. In other embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of at least about 200 micrometers. In still other embodiments, each

of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of at least about 250 micrometers. In further embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of at least about 500 micrometers. In still further embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has a height of at least about 800 micrometers.

In some embodiments employing solid microneedles, each of the plurality of solid microneedles (or the average of all of the plurality of solid microneedles) has a height of about 100 to about 1500 micrometers, about 100 to about 1200 micrometers, about 200 to about 1000 micrometers, about 200 to about 750 micrometers, about 200 to about 600 micrometers, or about 500 micrometers.

In some embodiments employing hollow microneedles, each of the plurality of hollow microneedles (or the average of all of the plurality of hollow microneedles) has a height of about 100 to about 3000 micrometers, about 800 to about 1400 micrometers, or about 500 micrometers.

In some embodiments, each of the plurality of hollow microneedles (or the average of all of the plurality of hollow microneedles) has a height of about 900 to about 1000 micrometers. In other embodiments, each of the plurality of hollow microneedles (or the average of all of the plurality of hollow microneedles) has a height of about 900 to about 950 micrometers. In still other embodiments, each of the plurality of hollow microneedles (or the average of all of the plurality of hollow microneedles) has a height of about 900 micrometers.

A single microneedle or the plurality of microneedles in a microneedle array can also be characterized by their aspect ratio. The aspect ratio of a microneedle is the ratio of the height of the microneedle, h to the width (at the base of the microneedle), w (as shown in **FIG. 7**). The aspect ratio can be presented as $h:w$. In some embodiments, each of the plurality of microneedles (or the average of all the plurality of microneedles) has (have) an aspect ratio in the range of 2:1 to 5:1. In some of these embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) has (have) an aspect ratio of at least 3:1.

In some embodiments, the array of microneedles contains about 100 to about 1500 microneedles per cm^2 of the array of microneedles.

In some embodiments employing solid microneedles, the array of solid microneedles contains about 100 to about 1500 solid microneedles per cm^2 of the array of solid microneedles.

In some embodiments, the array of solid microneedles contains about 200 to about 500 solid microneedles per cm^2 of the array of solid microneedles.

In some embodiments, the array of solid microneedles contains about 300 to about 400 solid microneedles per cm^2 of the array of solid microneedles.

In some embodiments employing hollow microneedles, the array of hollow microneedles contains about 3 to about 30 hollow microneedles per array of hollow microneedles.

5 In some embodiments, the array of hollow microneedles contains about 10 to about 30 hollow microneedles per array of hollow microneedles.

In some embodiments, the array of hollow microneedles contains about 3 to about 20 hollow microneedles per array of hollow microneedles.

In some embodiments, the array of hollow microneedles contains about 13 to about 20 hollow microneedles per array of hollow microneedles.

10 In some embodiments, the array of hollow microneedles contains about 8 to about 18 hollow microneedles per array of hollow microneedles.

In some embodiments, the array of hollow microneedles contains about 18 hollow microneedles per array of hollow microneedles.

15 In some embodiments, the array of hollow microneedles contains about 12 hollow microneedles per array of hollow microneedles.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) in a microneedle array can penetrate into the skin to a depth of about 50 to about 1500 micrometers, about 50 to about 400 micrometers, or about 50 to about 250 micrometers.

20 In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) in a microneedle array can penetrate into the skin to a depth of about 100 to about 400 micrometers, or about 100 to about 300 micrometers.

In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) in a microneedle array can penetrate into the skin to a depth of about 150 to about 1500 micrometers, or about 800 to about 1500 micrometers.

25 In some embodiments, each of the plurality of microneedles (or the average of all of the plurality of microneedles) in a microneedle array can penetrate into the skin to a depth of about 400 to about 800 micrometers.

30 For all of the above embodiments, it will be appreciated that the depth of penetration (DOP) of each of the plurality of microneedles (or the average of all of the plurality of microneedles) in a microneedle array may not be the full length of the microneedles themselves.

In some embodiments, the microneedle device according to the present disclosure can be in the form of a patch. One example of such an embodiment is shown in more detail in **FIG. 8**. **FIG. 8** illustrates a microneedle device **106A** comprising a patch **164A** in the form of a combination of a microneedle array **107A**, pressure sensitive adhesive **166A**, and backing

168A. The microneedle array **107A** is illustrated with microneedles **108A** protruding from a microneedle substrate **109A**. The microneedles **108A** can be arranged in any desired pattern or distributed over the microneedle substrate **109A** randomly. As shown, the microneedles **108A** are arranged in uniformly spaced rows. When arranged in rows, the rows can be arranged so that the microneedles **108A** are aligned or offset. In some embodiments (not shown), the microneedles **108A** can be arranged in a polygonal pattern such as a triangle, square, rectangle, pentagon, hexagon, heptagon, octagon, or trapezoid. In other embodiments (not shown), the microneedles **108A** can be arranged in a circular or oval pattern.

It should be understood that any description herein with respect to the microneedle device **106**, the microneedle array **107**, the microneedles **108**, and the microneedle substrate **109** can equally apply to the microneedle device **106A**, the microneedle array **107A**, the microneedles **108A**, and the microneedle substrate **109A**, respectively, and vice versa.

In some embodiments, the surface area of the substrate **109**, **109A** covered with microneedles **108**, **108A** is about 0.1 cm² to about 20 cm². In some of these embodiments, the surface area of the substrate **109**, **109A** covered with microneedles **108**, **108A** is about 0.5 cm² to about 5 cm². In some other of these embodiments, the surface area of the substrate **109**, **109A** covered with microneedles **108**, **108A** is about 1 cm² to about 3 cm². In still other of these embodiments, the surface area of the substrate **109**, **109A** covered with microneedles **108**, **108A** is about 1 cm² to about 2 cm².

In some embodiments (e.g., as shown in **FIG. 8**), the microneedles of the present disclosure can be disposed over substantially the entire surface of the array. In other embodiments (not shown), a portion of the substrate may not be provided with microneedles (that is, a portion of the substrate is non-structured). In some of these embodiments, the non-structured surface has an area of more than about 1 percent and less than about 75 percent of the total area of the device surface that faces the skin surface. In another of these embodiments, the non-structured surface has an area of more than about 0.65 cm² (0.10 square inch) to less than about 6.5 cm² (1 square inch).

For hollow microneedles, a hollow channel or bore extends through the substrate **109**, **109A** and microneedles **108**, **108A**. In some embodiments, the bore exits at a channel opening at or near the tip of the hollow microneedle. The channel preferably exits at an opening near the tip of the hollow microneedle. Most preferably, the channel or bore continues along a central axis of the microneedle, but exits similar to a hypodermic needle on a sloping side-wall of the microneedle to help prevent blockage of the channel by tissue upon insertion. In some embodiments, the diameter of the channel bore is about 10 to about 200 micrometers. In other

embodiments, the diameter of the channel bore is about 10 to about 150 micrometers. In still other embodiments, the diameter of the channel bore is about 30 to about 60 micrometers.

In some embodiments of hollow microneedles, the average cross-sectional area of the channel bore is about 75 to about 32,000 micrometers. In other embodiments of hollow
5 microneedles, the average cross-sectional area of the channel bore is about 75 to about 18,000 micrometers. In still other embodiments of hollow microneedles, the average cross-sectional area of the channel bore is about 700 to about 3,000 micrometers.

In some embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles (as measured from microneedle tip to microneedle tip) is between about
10 0.7 mm and about 20 mm. In other embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is between about 0.7 mm and about 10 mm. In still other embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is between about 2 mm and about 20 mm. In still other embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is between about 2 mm
15 and about 10 mm. In a preferred embodiment of hollow microneedle arrays, the average spacing between adjacent microneedles is between about 2 mm.

In some embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles (as measured from microneedle tip to microneedle tip) is greater than
20 about 0.7 mm. In other embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is greater than about 2 mm.

In some embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is less than about 20 mm. In other embodiments of hollow microneedle arrays, the average spacing between adjacent microneedles is less than about 10 mm.

In some embodiments of solid microneedle arrays, the average spacing between
25 adjacent microneedles (as measured from microneedle tip to microneedle tip) is between about 200 micrometers and about 2000 micrometers. In other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is between about 200 micrometers and about 600 micrometers. In still other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is between about 200 micrometers and about 300
30 micrometers. In yet still other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is between about 500 micrometers and about 600 micrometers.

In some embodiments of solid microneedle arrays, the average spacing between adjacent microneedles (as measured from microneedle tip to microneedle tip) is greater than
35 about 200 micrometers. In other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is greater than about 500 micrometers.

In some embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is less than about 2000 micrometers. In other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is less than about 1000 micrometers. In still other embodiments of solid microneedle arrays, the average spacing
5 between adjacent microneedles is less than about 600 micrometers. In yet still other embodiments of solid microneedle arrays, the average spacing between adjacent microneedles is less than about 300 micrometers.

The microneedle arrays can be manufactured in any suitable way such as by injection molding, compression molding, metal injection molding, stamping, photolithography, or
10 extrusion. In one embodiment, hollow microneedle arrays can be made by injection molding of a polymer such as medical grade polycarbonate or LCP, followed by laser drilling to form the channels of the microneedles.

Each embodiment shown in the figures is illustrated as a separate embodiment for
15 clarity in illustrating a variety of features of the applicators of the present disclosure. However, it should be understood that any combination of elements and features of any of the embodiments illustrated in the figures and described herein can be employed in the applicators of the present disclosure.

The following embodiments are intended to be illustrative of the present disclosure and
20 not limiting.

EMBODIMENTS

Embodiment 1 is an applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
25 a second end configured as a graspable handle,
a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device,
an actuation button in mechanical or electrical engagement with the driving element,
at least one reciprocating support structure slidably engaged with the housing, wherein
30 the reciprocating support structure has a first position where at least a portion of it extends from the first open end of the housing by a first distance and a second position wherein the portion extends from the first open end of the housing by a second distance, the second distance being less than the first distance.

Embodiment 2 is the applicator of embodiment 1 wherein the reciprocating support
35 structure comprises a plurality of alignment feet

Embodiment 3 is the applicator of embodiment 2 wherein the alignment feet are independently movable.

Embodiment 4 is the applicator of embodiment 2 or 3 and further comprising a lockout mechanism that prevents actuation if the alignment feet are not evenly aligned.

5 Embodiment 5 is the applicator of any of the preceding embodiments wherein the portion of the reciprocating support structure that extends from the first open end of the housing has an open, cylindrical end.

Embodiment 6 is the applicator of any of the preceding embodiments wherein the driving element comprises a magnet.

10 Embodiment 7 is the applicator of any of the preceding embodiments wherein the applicator further comprises a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that has elapsed after actuation of the device and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.

15 Embodiment 8 is the applicator of any one of the preceding embodiments wherein the applicator further comprises a driving spring coupled to the driving element.

Embodiment 9 is the applicator of any of the preceding embodiments wherein the applicator further comprises a device life indicator in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the device life indicator is capable of counting the number of use cycles that the applicator has undergone and, based on the number of use cycles, providing feedback to the user as to the use status of the applicator.

20 Embodiment 10 is an applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
a second end configured as a graspable handle,
25 a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device,
a microneedle device,
an actuation button in mechanical or electrical engagement with the driving element,
a device life indicator in mechanical or electrical engagement with at least one of the
30 driving element or the actuation button, wherein the device life indicator is capable of counting the number of use cycles that the applicator has undergone and, based on the number of use cycles, providing feedback to the user as to the use status of the applicator.

Embodiment 11 is the applicator of embodiment 9 or 10 wherein the device life indicator is a dose counter.

Embodiment 12 is the applicator of any of embodiments 9 to 11 wherein the device includes a lockout mechanism that prevents device actuation when the device life indicator has counted a predetermined number of use cycles.

5 Embodiment 13 is the applicator of any of embodiments 9 to 12 wherein the device life indicator comprises a numeric display.

Embodiment 14 is the applicator of any of embodiments 9 to 13 wherein the device life indicator comprises a colored graphic display that can change in response to changes in device status.

10 Embodiment 15 is the applicator of any of embodiments 9 to 14 wherein the device life indicator comprises one or more words that are visually displayed.

Embodiment 16 is the applicator of any of embodiments 9 to 15 wherein the applicator further comprises a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that has elapsed after actuation of the device and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.

Embodiment 17 is the applicator of any one of the preceding embodiments wherein the device includes a device status indicator, wherein the device status indicator is optionally capable of displaying a message in response to the device being in a specific state.

20 Embodiment 18 is an applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
a second end configured as a graspable handle,
a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device,
an actuation button in mechanical or electrical engagement with the driving element,
25 wherein the driving element is configured to apply the microneedle device to a skin surface when the actuation button is actuated,
wherein the microneedle device is releasably coupled to the driving element, and
a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that
30 has elapsed after actuation of the device and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.

Embodiment 19 is the applicator of any one of the preceding embodiments wherein the applicator further comprises a battery.

35 Embodiment 20 is the applicator of embodiment 19 wherein the applicator further comprises a battery gauge to indicate the amount of usable battery life remaining.

The embodiments described above and illustrated in the figures are presented by way of example only and are not intended as a limitation upon the concepts and principles of the present disclosure. As such, it will be appreciated by one having ordinary skill in the art that various changes in the elements and their configuration and arrangement are possible without departing from the spirit and scope of the present disclosure.

All references and publications cited herein are expressly incorporated herein by reference in their entirety into this disclosure.

Various features and aspects of the present disclosure are set forth in the following claims.

What is claimed is:

1. An applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
5 a second end configured as a graspable handle,
a driving element contained within the housing, the driving element having a first end
configured so as to couple with the microneedle device,
an actuation button in mechanical or electrical engagement with the driving element,
at least one reciprocating support structure slidably engaged with the housing, wherein
10 the reciprocating support structure has a first position where at least a portion of it extends from
the first open end of the housing by a first distance and a second position wherein the portion
extends from the first open end of the housing by a second distance, the second distance being
less than the first distance.
- 15 2. An applicator as claimed in claim 1 wherein the reciprocating support structure
comprises a plurality of alignment feet
3. An applicator as claimed in claim 2 wherein the alignment feet are independently
movable.
20
4. An applicator as claimed in claim 2 or 3 and further comprising a lockout
mechanism that prevents actuation if the alignment feet are not evenly aligned.
5. An applicator as claimed any of the preceding claims wherein the portion of the
25 reciprocating support structure that extends from the first open end of the housing has an open,
cylindrical end.
6. An applicator as claimed in any of the preceding claims wherein the driving element
comprises a magnet.
30
7. An applicator as claimed in any of the preceding claims wherein the applicator
further comprises a dose timer in mechanical or electrical engagement with at least one of the
driving element or the actuation button, wherein the dose timer is capable of determining the
time that has elapsed after actuation of the device and providing feedback to the user as to the
35 time that the microneedle device has been in place on the skin surface.

8. An applicator as claimed in any one of the preceding claims wherein the applicator further comprises a driving spring coupled to the driving element.

5 9. An applicator as claimed in any of the preceding claims wherein the applicator further comprises a device life indicator in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the device life indicator is capable of counting the number of use cycles that the applicator has undergone and, based on the number of use cycles, providing feedback to the user as to the use status of the applicator.

10 10. An applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
a second end configured as a graspable handle,
a driving element contained within the housing, the driving element having a first end
configured so as to couple with the microneedle device,
15 a microneedle device,
an actuation button in mechanical or electrical engagement with the driving element,
a device life indicator in mechanical or electrical engagement with at least one of the
driving element or the actuation button, wherein the device life indicator is capable of counting
the number of use cycles that the applicator has undergone and, based on the number of use
20 cycles, providing feedback to the user as to the use status of the applicator.

11. An applicator as claimed in claim 9 or 10 wherein the device life indicator is a dose counter.

25 12. An applicator as claimed in any of claims 9 to 11 wherein the device includes a lockout mechanism that prevents device actuation when the device life indicator has counted a predetermined number of use cycles.

30 13. An applicator as claimed in any of claims 9 to 12 wherein the device life indicator comprises a numeric display.

14. An applicator as claimed in any of claims 9 to 13 wherein the device life indicator comprises a colored graphic display that can change in response to changes in device status.

35 15. An applicator as claimed in any of claims 9 to 14 wherein the device life indicator comprises one or more words that are visually displayed.

16. An applicator as claimed in any of claims 9 to 15 wherein the applicator further comprises a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that has elapsed after actuation of the device and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.


17. An applicator as claimed in any of the preceding claims wherein the device includes a device status indicator, wherein the device status indicator is optionally capable of displaying a message in response to the device being in a specific state.

18. An applicator for applying a microneedle device, comprising:
a housing having a first open end configured so as to accept the microneedle device,
a second end configured as a graspable handle,
a driving element contained within the housing, the driving element having a first end configured so as to couple with the microneedle device,
an actuation button in mechanical or electrical engagement with the driving element, wherein the driving element is configured to apply the microneedle device to a skin surface when the actuation button is actuated,
wherein the microneedle device is releasably coupled to the driving element, and
a dose timer in mechanical or electrical engagement with at least one of the driving element or the actuation button, wherein the dose timer is capable of determining the time that has elapsed after actuation of the applicator and providing feedback to the user as to the time that the microneedle device has been in place on the skin surface.


19. An applicator as claimed in any one of the preceding claims wherein the applicator further comprises a battery.

20. An applicator as claimed in claim 19 wherein the applicator further comprises a battery gauge to indicate the amount of usable battery life remaining.

1/13

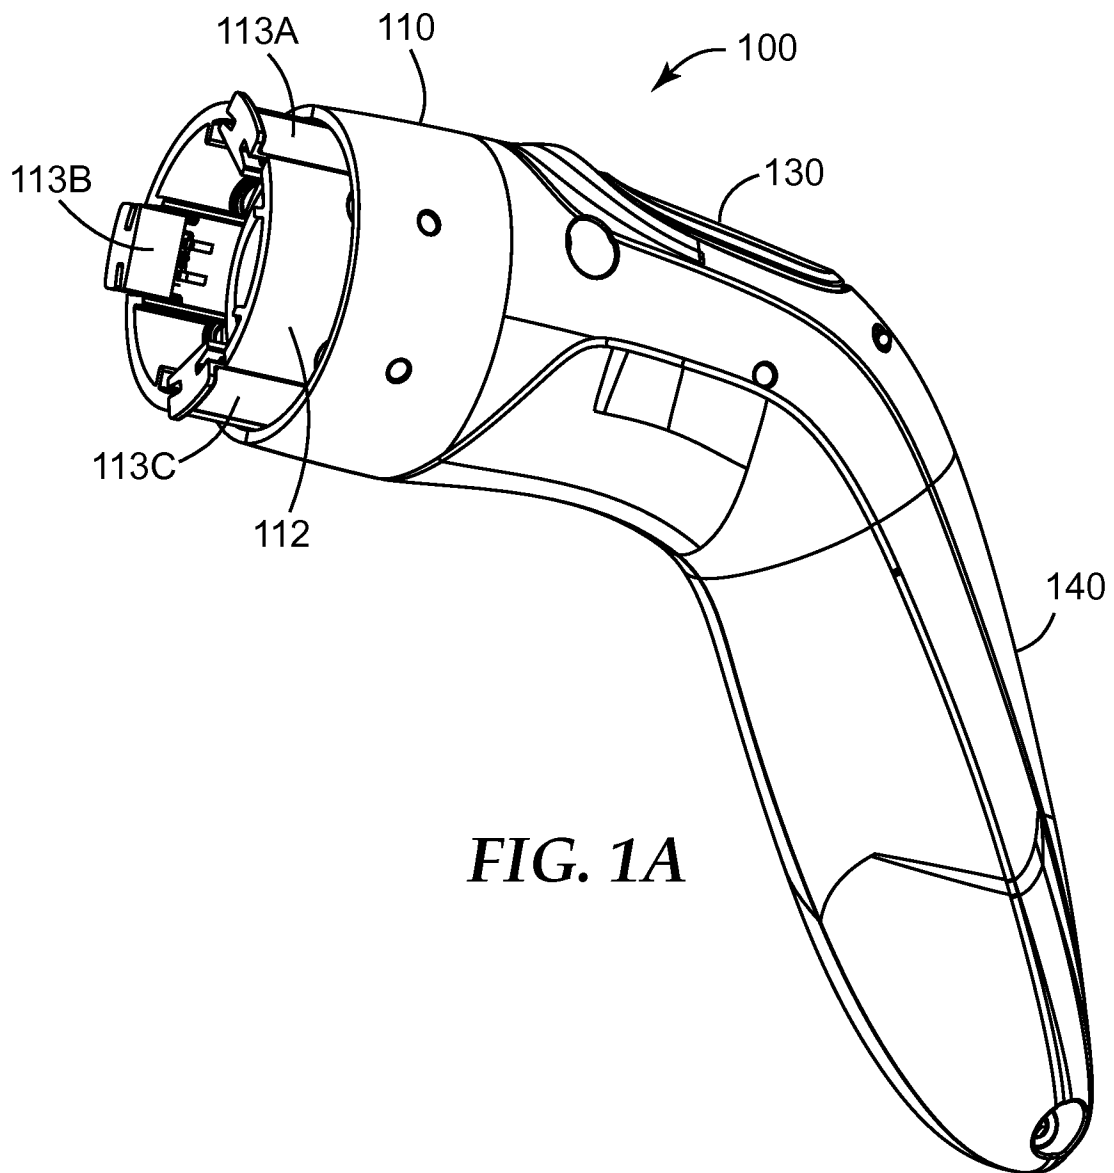

2/13

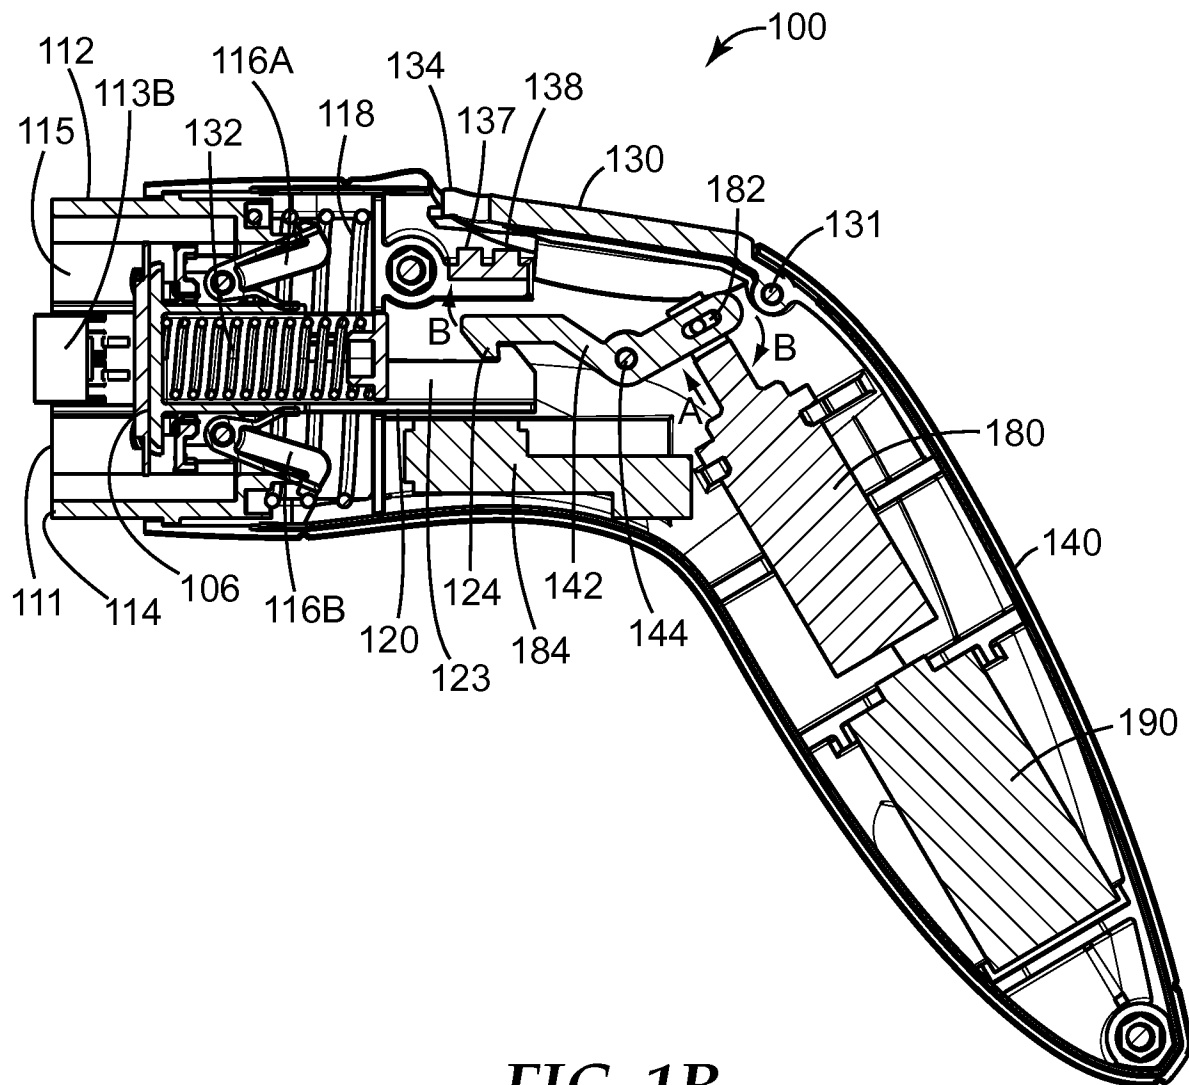**FIG. 1B**

A A

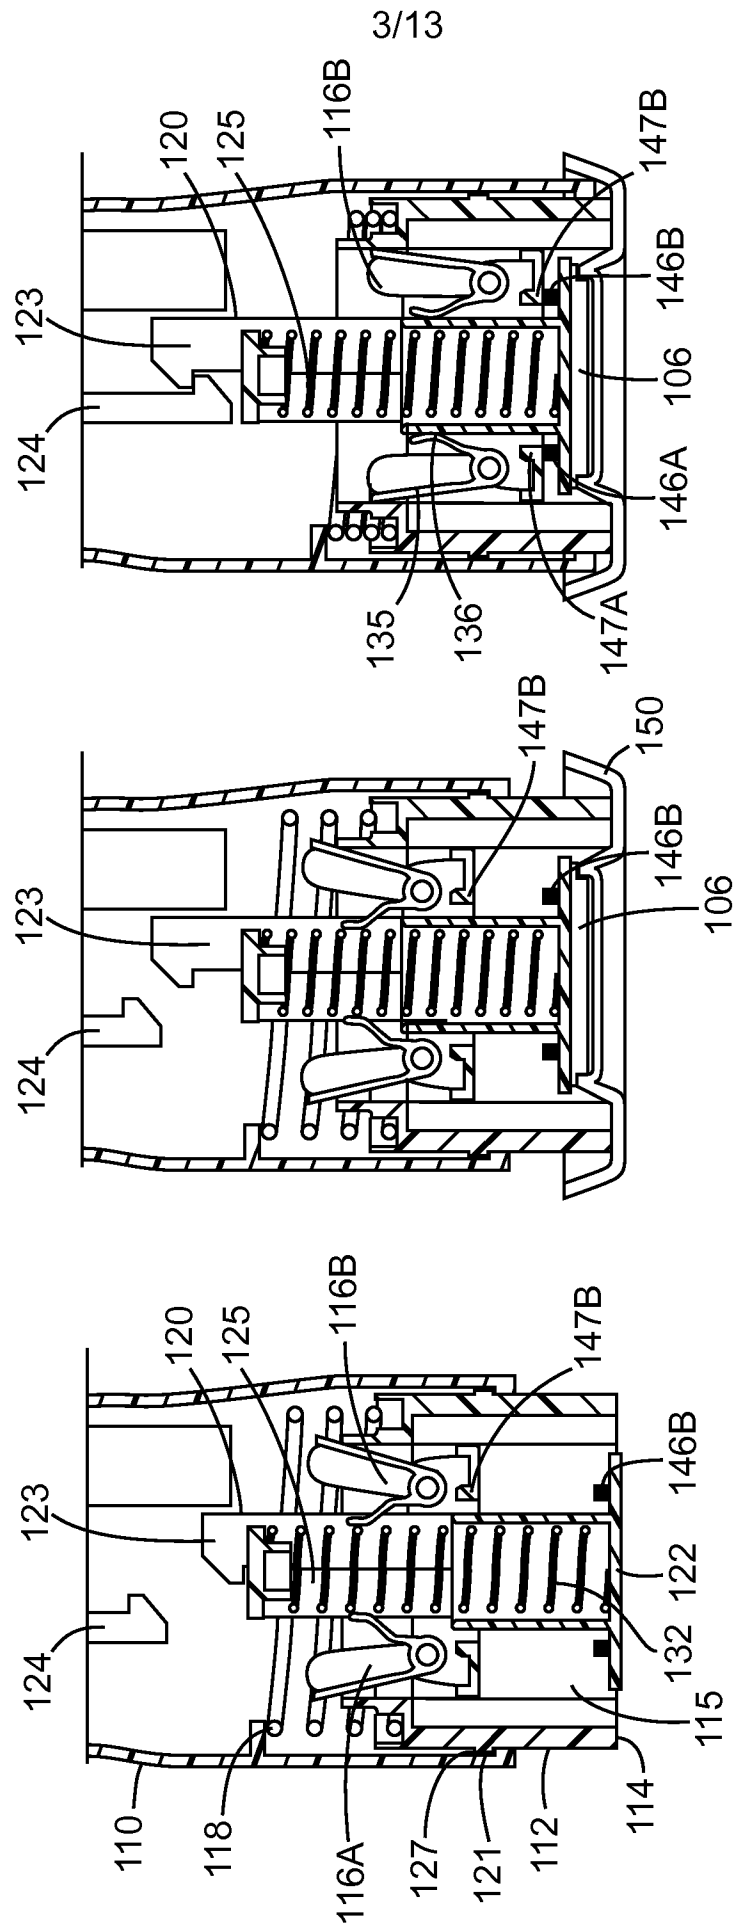


FIG. 2A

FIG. 2B

FIG. 2C

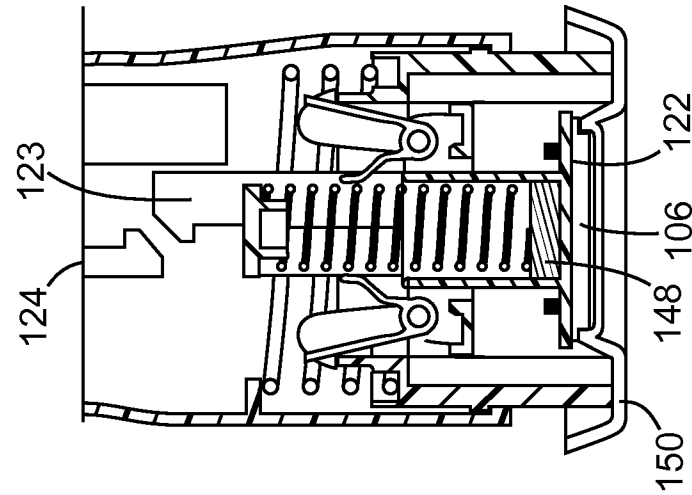


FIG. 2F

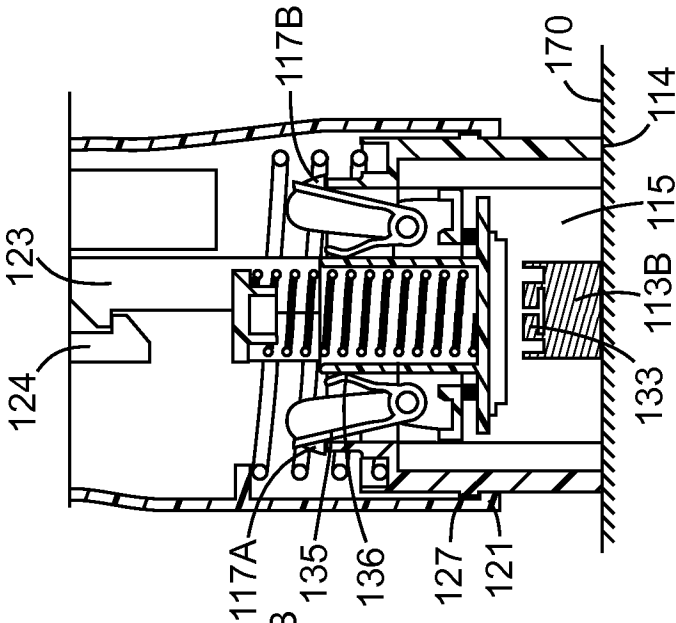


FIG. 2E

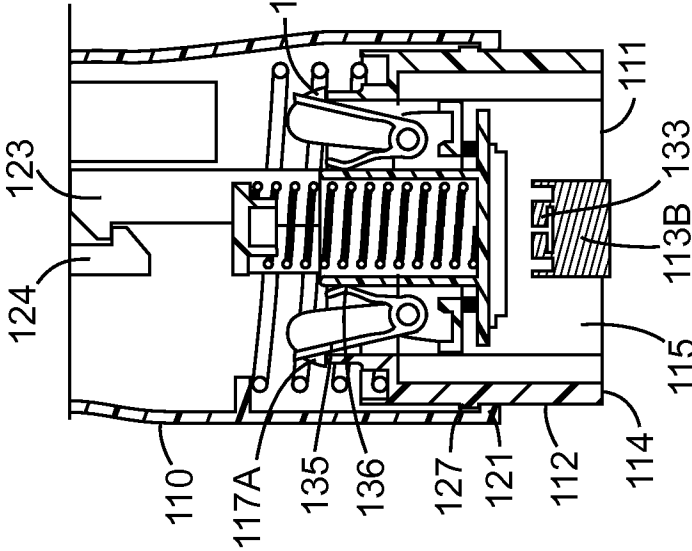


FIG. 2D

5/13

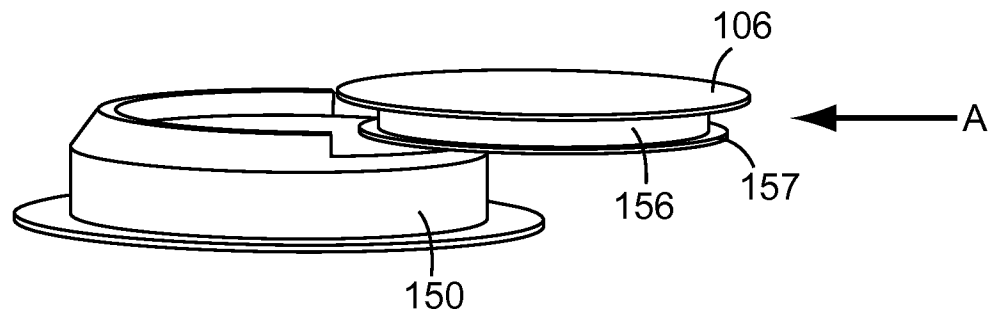


FIG. 3B

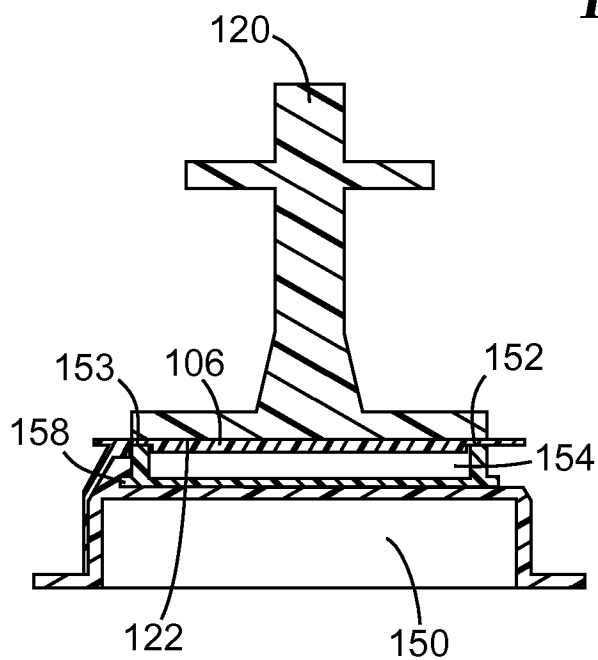


FIG. 3A

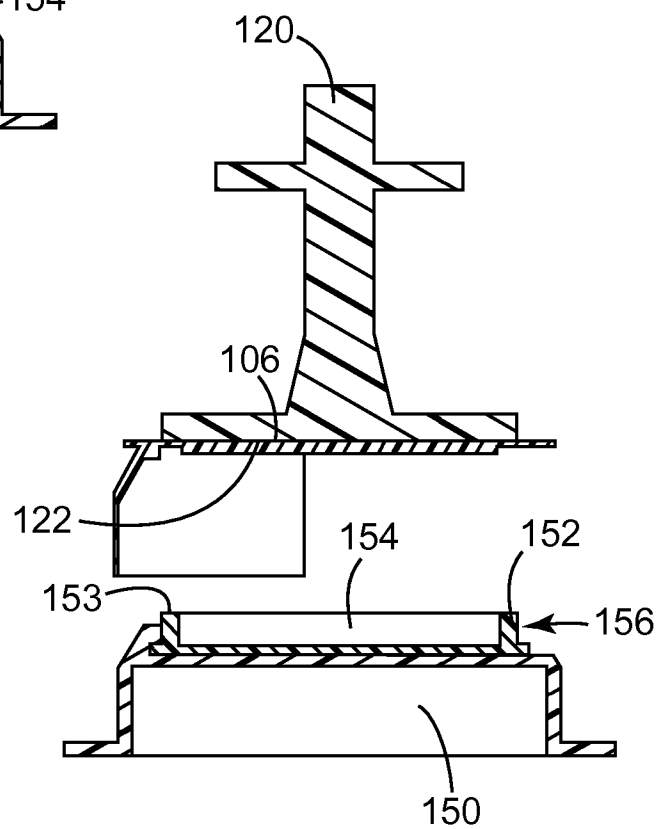


FIG. 3C

6/13

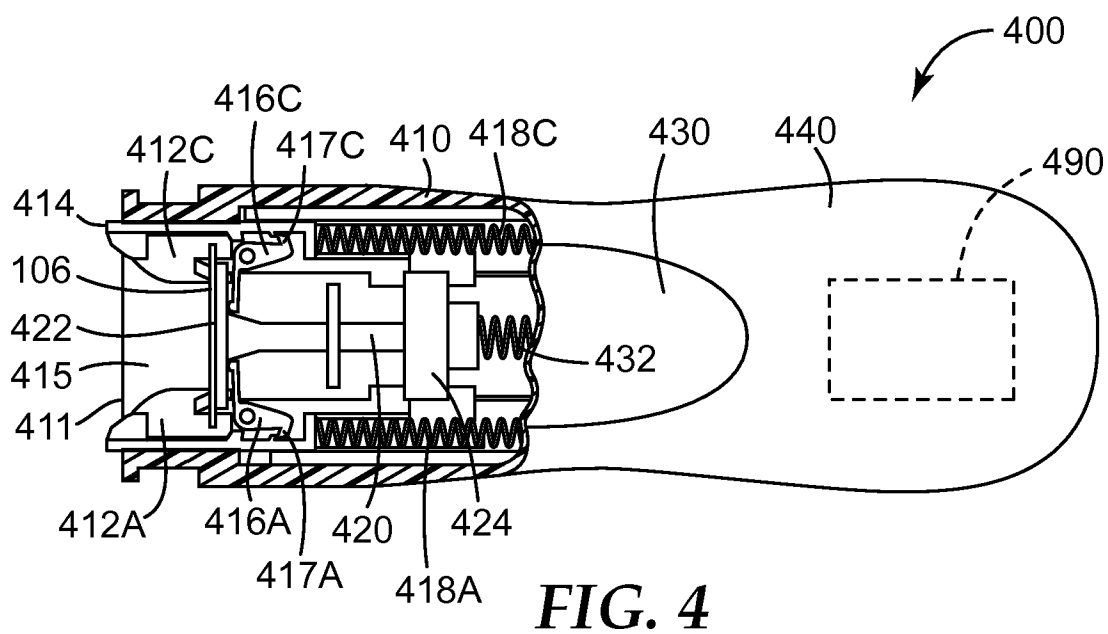


FIG. 4

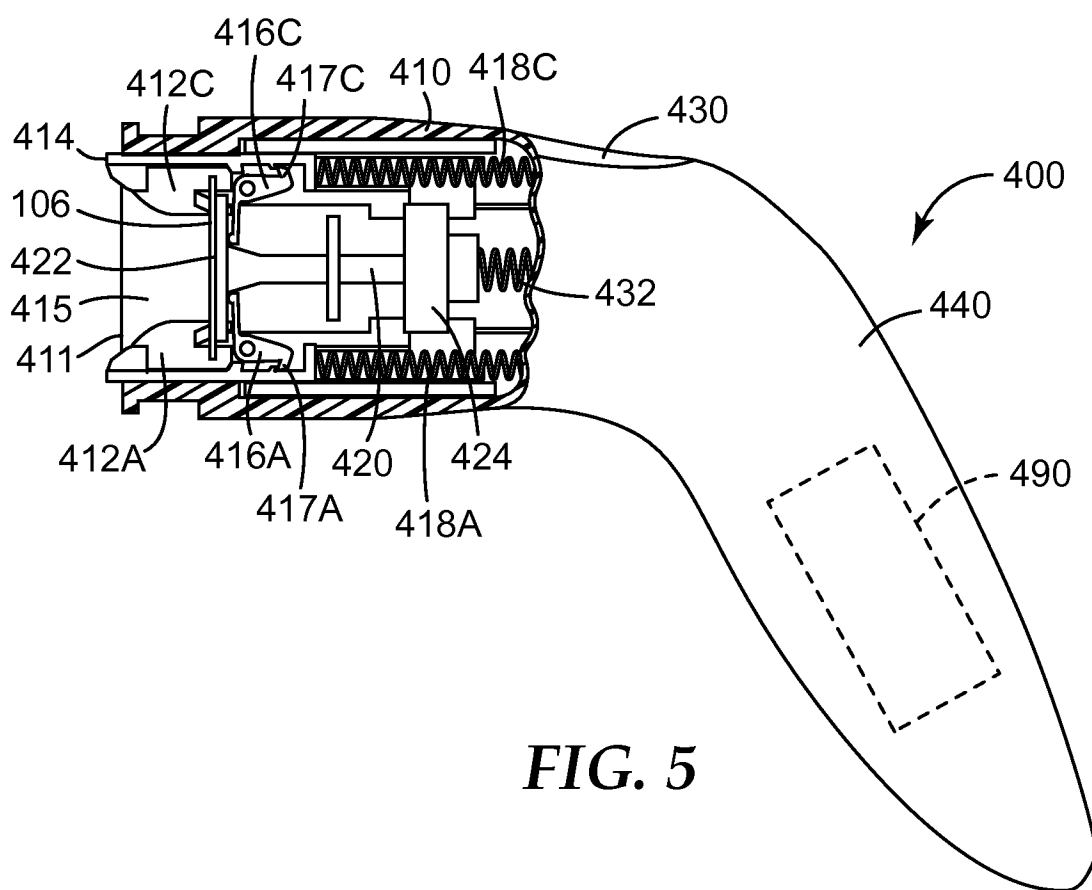


FIG. 5

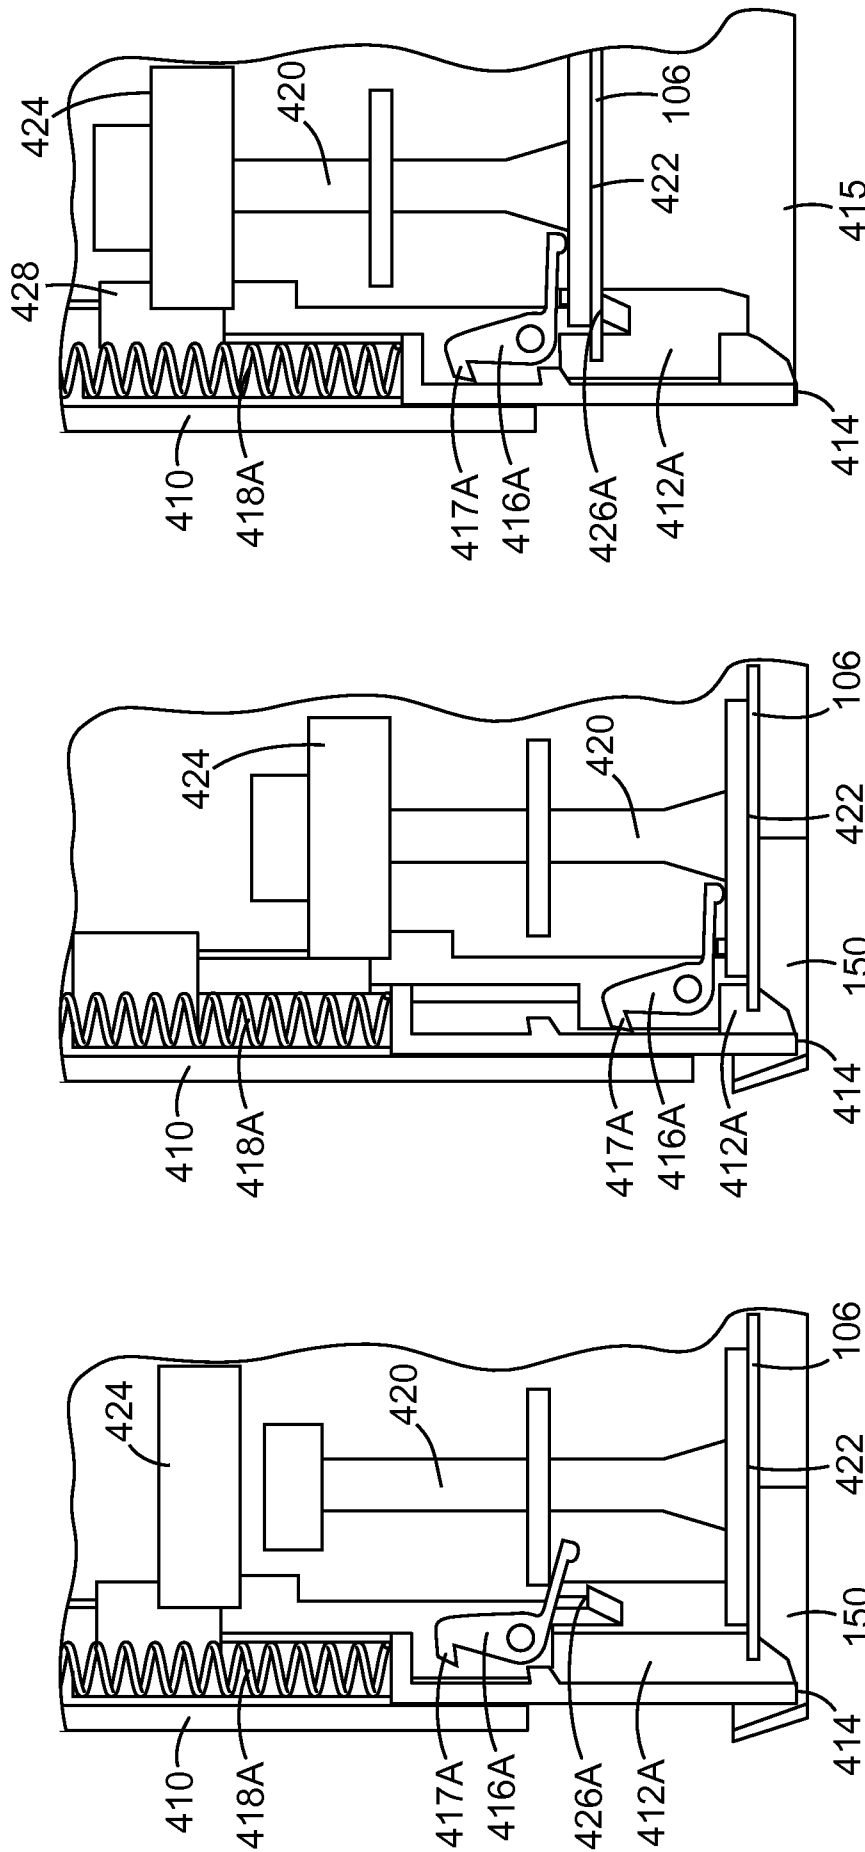


FIG. 6C

FIG. 6B

FIG. 6A

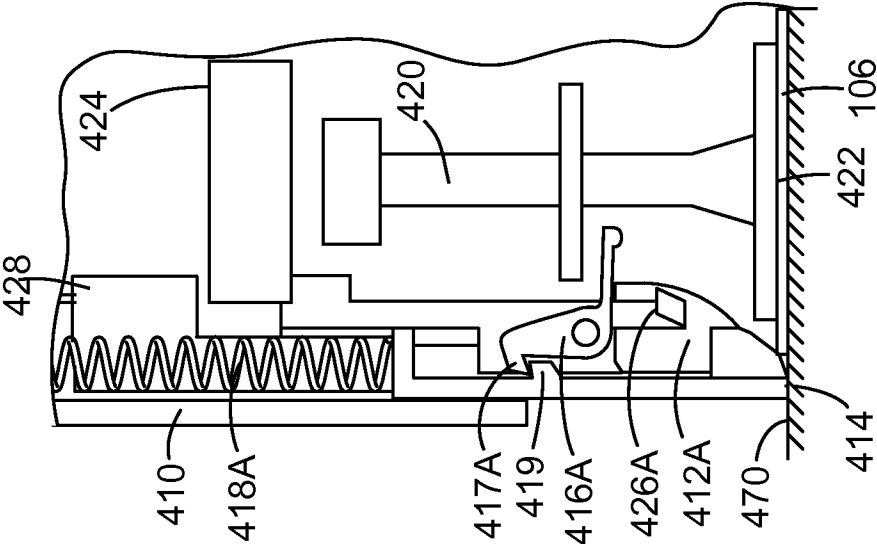


FIG. 6E

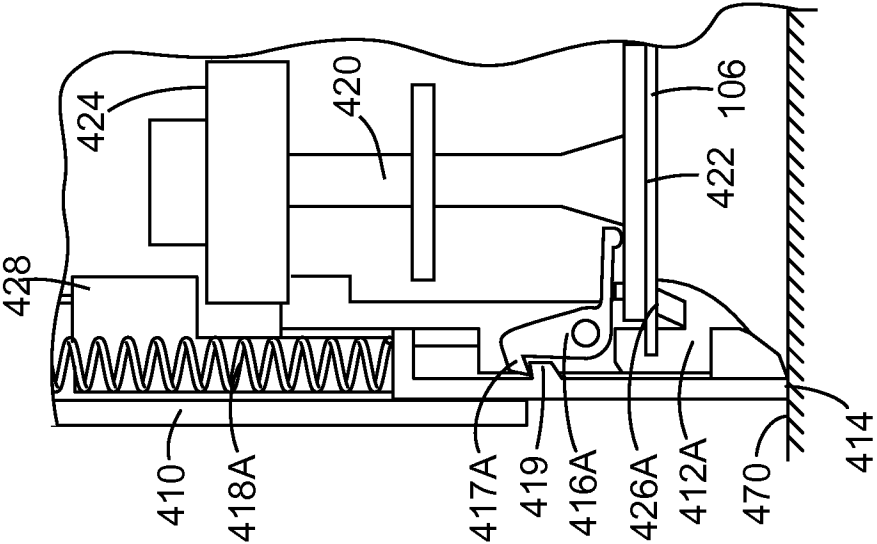
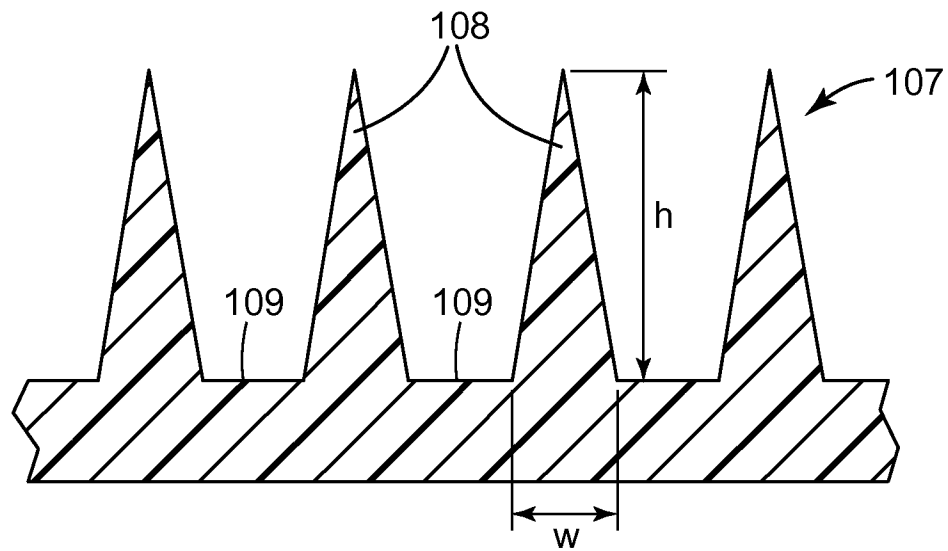
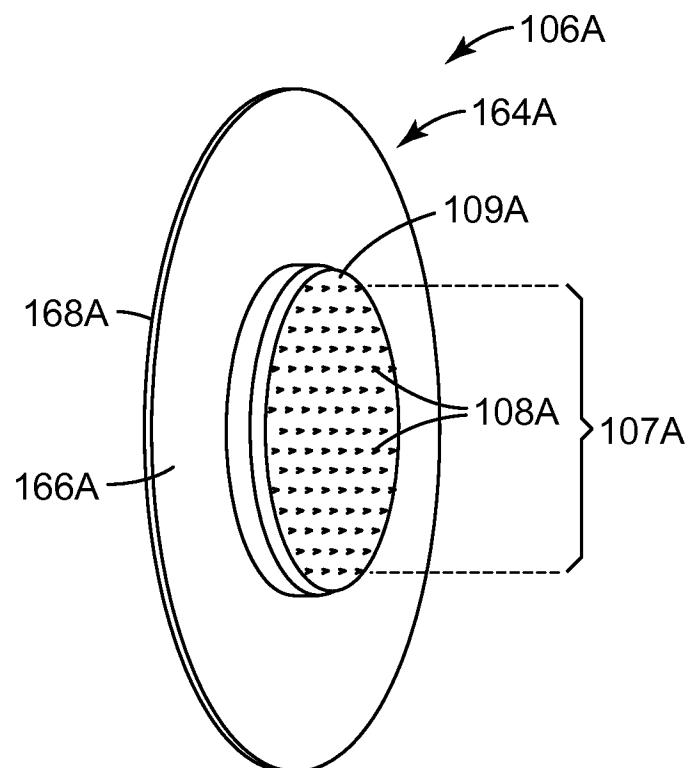
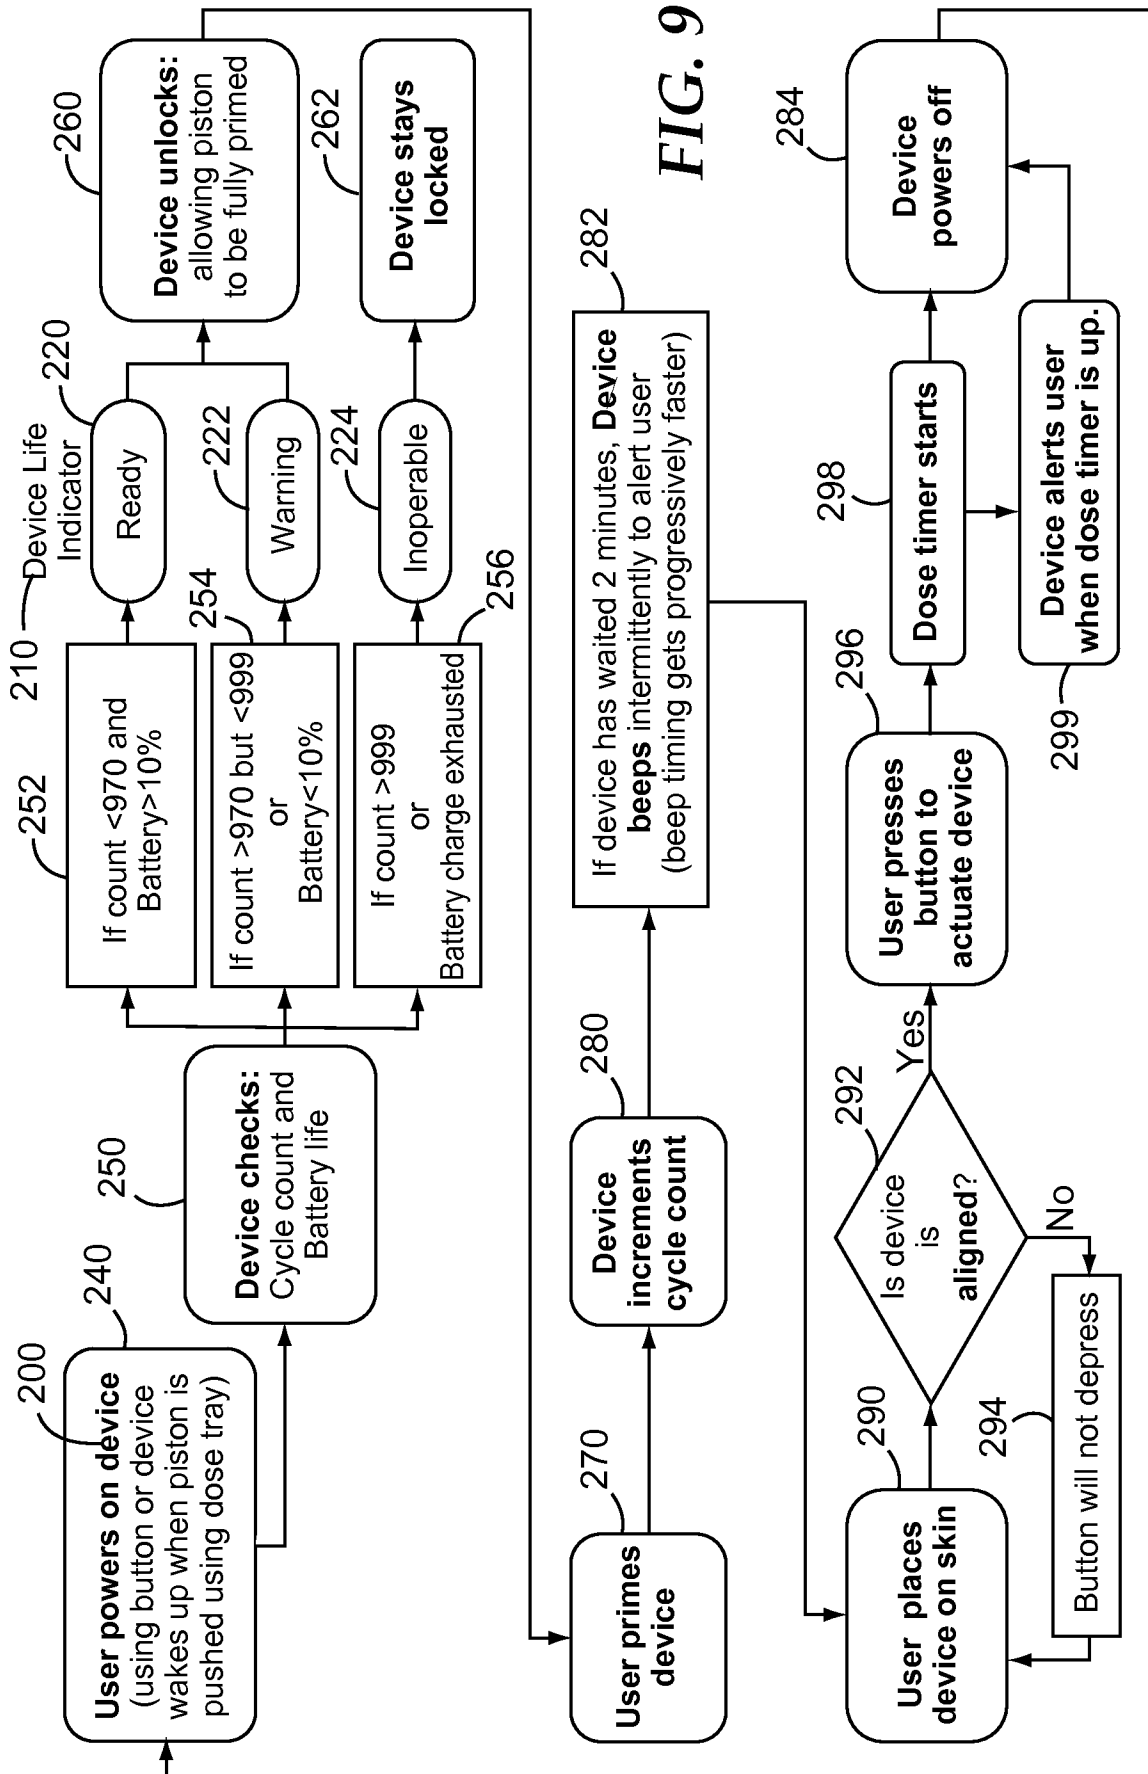


FIG. 6D

9/13

**FIG. 7****FIG. 8**

10/13



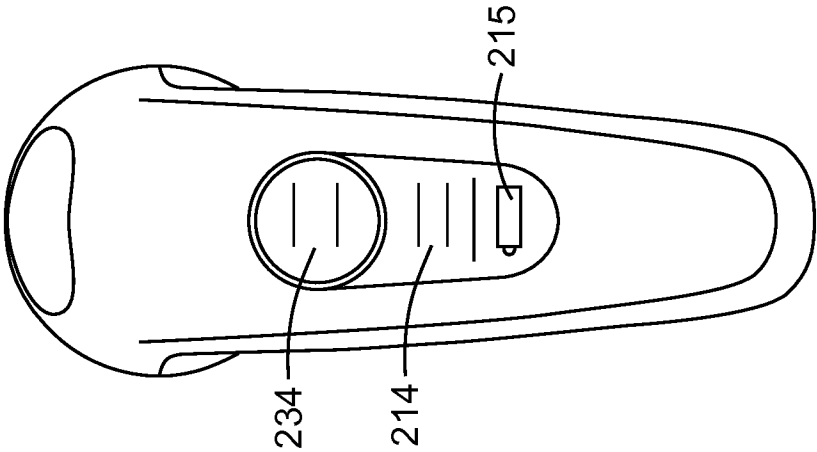


FIG. 10C

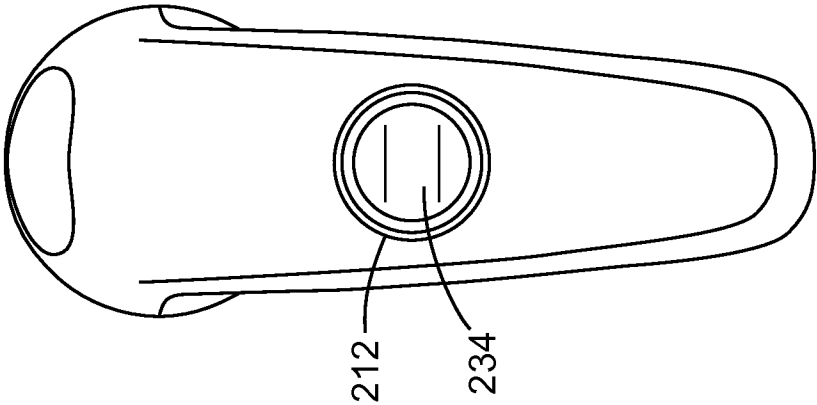


FIG. 10B

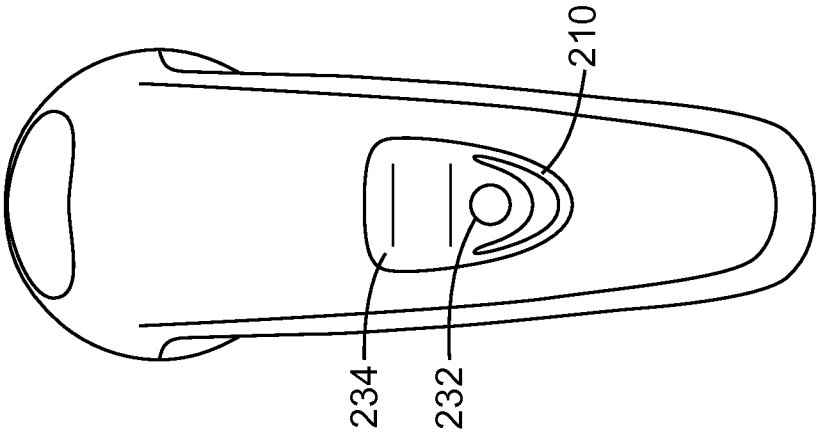


FIG. 10A

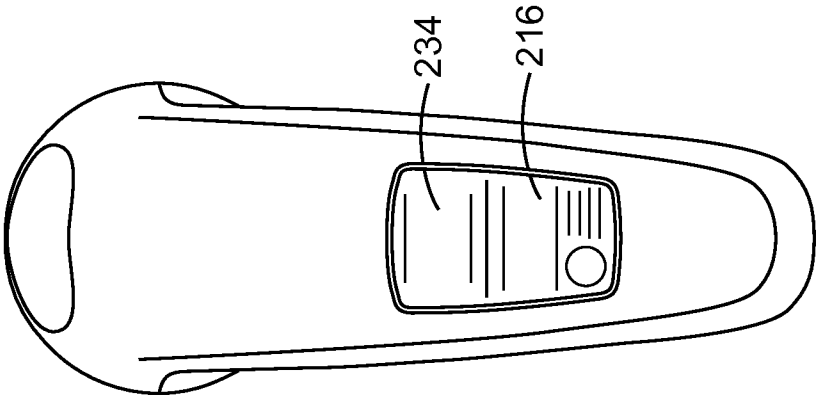


FIG. 10D

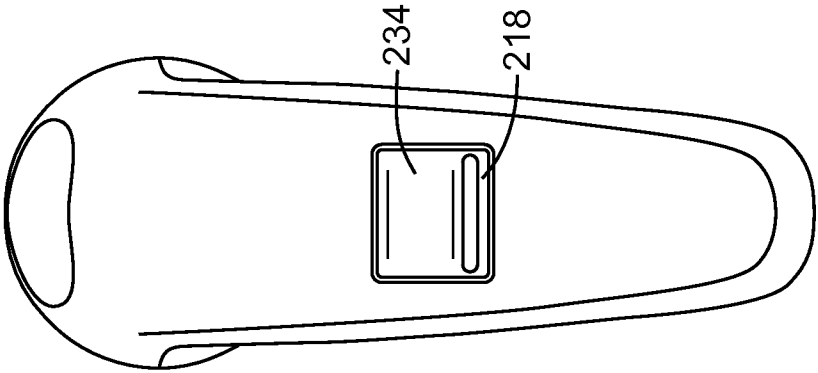


FIG. 10E

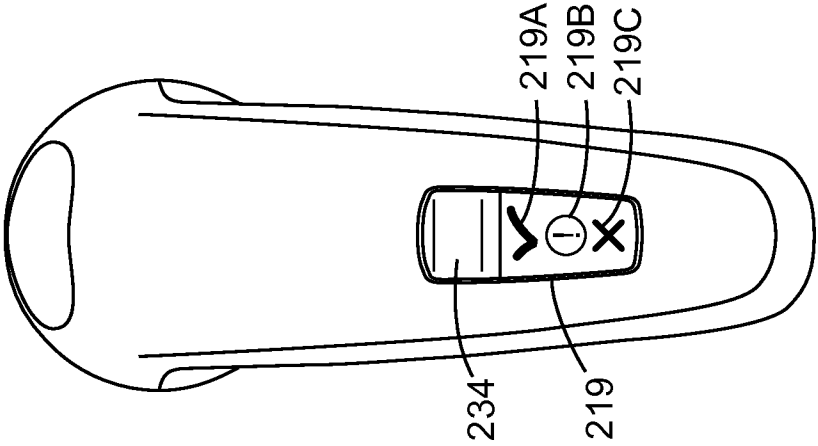


FIG. 10F

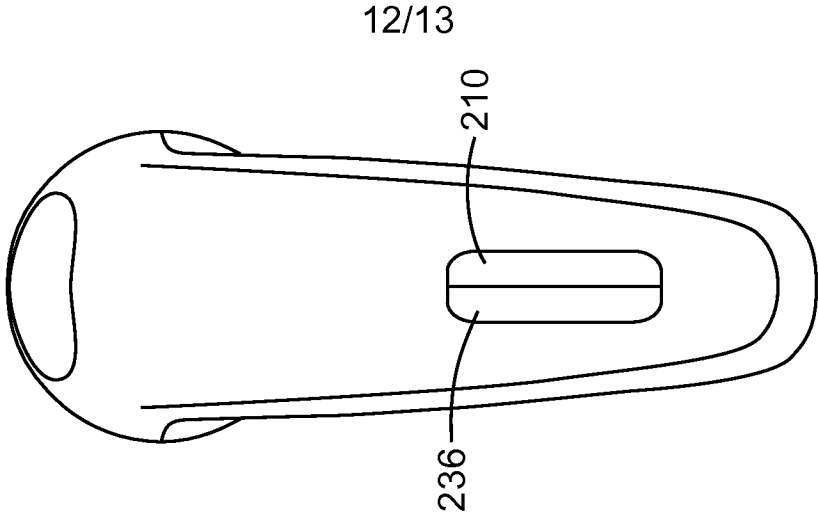


FIG. 11

13/13

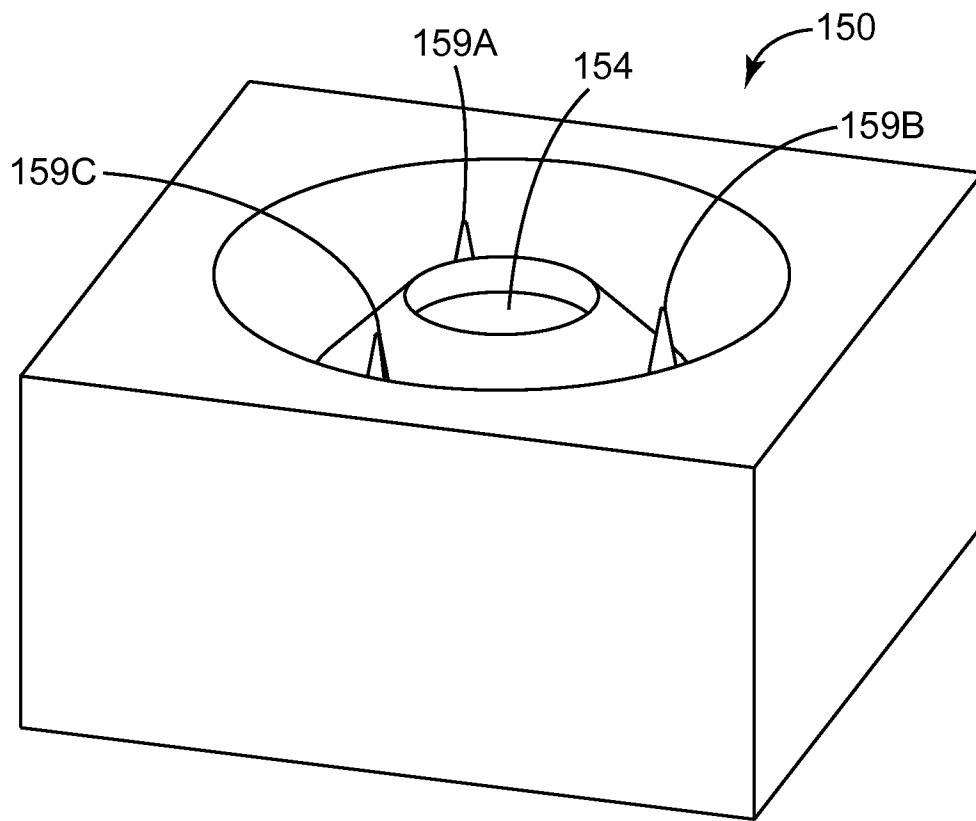


FIG. 12A

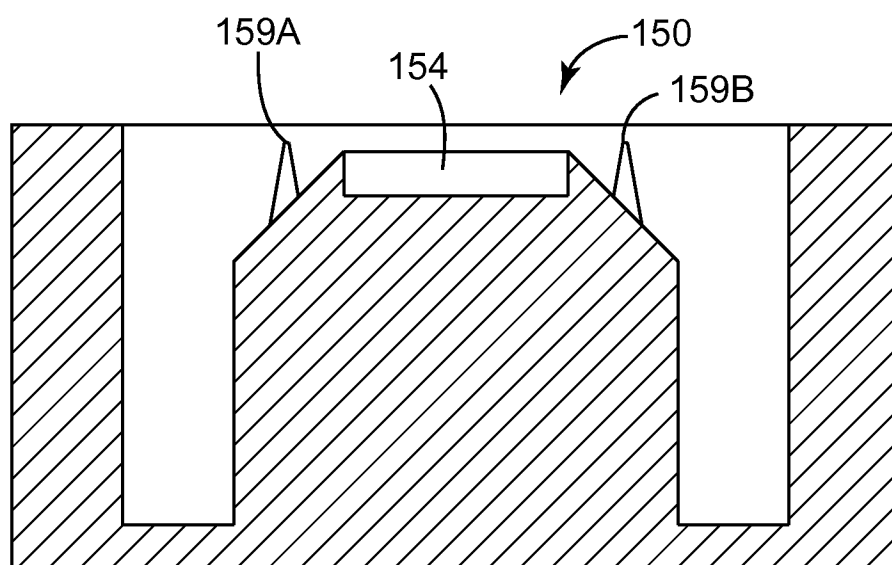


FIG. 12B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2014/010447

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61M 5/20 (2014.01)

USPC - 604/506

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8) - A61M 5/14, 5/20, 5/315 (2014.01)

USPC - 604/136, 140, 218, 506

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

CPC - A61M 5/14, 5/20, 5/315 (2013.01)

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

Orbit, Google Patents, Google Scholar

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2012/0123387 A1 (GONZALEZ et al) 17 May 2012 (17.05.2012) entire document	1-3
Y		4
Y	US 2006/0229570 A1 (LOVELL et al) 12 October 2006 (12.10.2006) entire document	4
A	US 2009/0198189 A1 (SIMONS et al) 06 August 2009 (06.08.2009) entire document	1-4, 10, 18

☐ Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

09 March 2014

Date of mailing of the international search report

21 MAR 2014

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450
Facsimile No. 571-273-3201

Authorized officer:

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2014/010447

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☒ Claims Nos.: 5-9, 11-17, 19, 20
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.