



(51) International Patent Classification:

A61B 34/20 (2016.01) *A61B 34/00* (2016.01)
A61B 17/74 (2006.01) *A61F 2/34* (2006.01)
A61B 17/90 (2006.01) *A61F 2/46* (2006.01)

(21) International Application Number:

PCT/CA2016/050089

(22) International Filing Date:

2 February 2016 (02.02.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/110,872 2 February 2015 (02.02.2015) US

(71) Applicant: **ORTHOSOFT INC.** [CA/CA]; Suite 3300, 75 Queen Street, Montréal, Québec H3C 2N6 (CA).

(72) Inventors: **FALARDEAU, Bruno**; #301, 3964 Bannantyne, Verdun, Québec H4G 1C1 (CA). **DUVAL, Karine**; Apt. 2, 2486 Sherbrooke St. E., Montréal, Québec H2K 1E7 (CA). **MOREAU-BELANGER, Laurence**; 102 rue de Pise, Laval, Québec H7M 4J1 (CA). **PARADIS, François**; 214 De Chartres, Boucherville, Québec J4B 7V1 (CA). **LI, Di**; 6973 rue Marie-Guyart, LaSalle, Québec H8N 3G9 (CA). **VALIN, Myriam**; 284 avenue Brien, Laval, Québec H7N 3M7 (CA). **PELLETIER, Benoit**; 96, 7e rue, Laval, Québec H7N 2C7 (CA).


(74) Agent: **NORTON ROSE FULBRIGHT CANADA LLP/S.E.N.C.R.L., S.R.L.**; Suite 2500, 1 Place Ville-Marie, Montréal, Québec H3B 1R1 (CA).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: ACETABULUM RIM DIGITIZER DEVICE AND METHOD

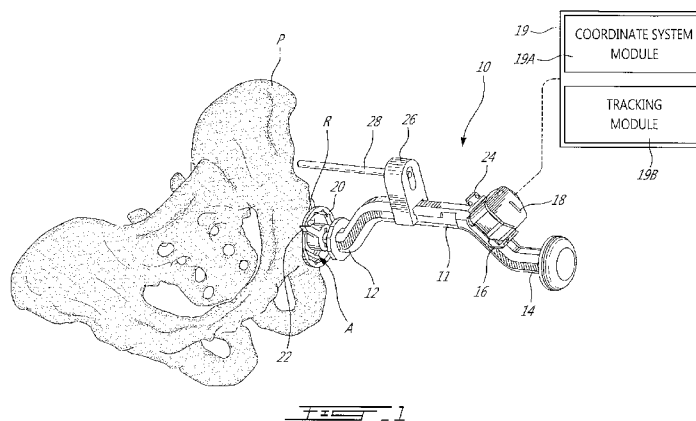

(57) Abstract: A computer-assisted surgery (CAS) system for tracking an orientation of a pelvis comprises at least one instrument, the instrument having an acetabulum abutment end adapted to be received in an acetabulum, a rim abutment adapted to be abutted against a rim of the acetabulum, and an indicator representative of a physical orientation of the instrument. An inertial sensor unit is connected to the at least one instrument, the inertial sensor unit producing readings representative of its orientation. A computer-assisted surgery processor unit comprises a coordinate system module for setting a pelvic coordinate system from readings of the at least one inertial sensor unit when the at least one instrument has the acetabulum abutment end received in the acetabulum, the coordinate system module setting the pelvic coordinate system by obtaining a plurality of orientation values from the at least one inertial sensor unit when the rim abutment is abutted against locations of the rim, one of said orientation values having the indicator aligned with a reference landmark, the coordinate system module defining an acetabular plane representative of the pelvic coordinate system from the plurality of orientation values; and a tracking module for tracking an orientation of the at least one inertial sensor unit relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor unit. An interface outputs orientation data as a function of the pelvic coordinate system.





Published:

— *with international search report (Art. 21(3))*

ACETABULUM RIM DIGITIZER DEVICE AND METHOD

FIELD OF THE APPLICATION

[0001] The present application relates to computer-assisted surgery using inertial sensors and more particularly to tools for determining a pelvic tilt for subsequent acetabular cup positioning procedures in hip surgery.

BACKGROUND OF THE ART

[0002] In hip arthroplasty, the acetabulum is reamed to subsequently receive therein an acetabular cup. The acetabular cup is an implant that is received in the reamed acetabulum and serves as a receptacle for a femoral head or femoral head implant. Accordingly, tools such as a reamer and a cup impactor are used in the procedure. One of the challenges in such procedures is to provide an adequate orientation to the acetabular cup. Indeed, an inaccurate orientation may result in a loss of movements, improper gait, and/or premature wear of implant components. For example, the acetabular cup is typically positioned in the reamed acetabulum by way of an impactor. The impactor has a stem at an end of which is the acetabular cup. The stem is handled by an operator that impacts the free end so as to drive the acetabular cup into the acetabulum. It is however important that the operator hold the stem of the impactor in a precise three-dimensional orientation relative to the pelvis so as to ensure the adequate orientation of the acetabular cup, in terms of inclination and anteversion.

[0003] For this purpose, computer-assisted surgery has been developed in order to help the operator in positioning and orienting the impactor to a desired orientation, notably by enabling the determination of the pelvic tilt, acetabular plane or like orientation data of the pelvis. Among the various tracking technologies used in computer-assisted surgery, optical navigation, C-arm validation and manual reference guides have been used. The optical navigation requires the use of a navigation system, which adds operative time. It also requires pinning a reference on the patient, which adds to the invasiveness of the procedure. It is also bound to line-of-sight constraints which hamper the normal surgical flow. C-arm validation requires the use of bulky equipment and the validation is not cost-effective. Moreover, it does not provide a quantitative assessment of the cup positioning

once done, and is generally used post-operatively as opposed to intra-operatively. Finally, manual jigs, such as an A-frame, do not account for the position of the patient on the operative table. Accordingly, inertial sensors are used for their cost-effectiveness and the valuable information they provide.

SUMMARY OF THE APPLICATION

[0004] It is therefore an aim of the present invention to provide an acetabulum rim digitizer that addresses issues associated with the prior art.

[0005] Therefore, in accordance with a first embodiment of the present disclosure, there is provided a computer-assisted surgery (CAS) system for tracking an orientation of a pelvis comprising: at least one instrument, the instrument having an acetabulum abutment end adapted to be received in an acetabulum, a rim abutment adapted to be abutted against a rim of the acetabulum, and an indicator representative of a physical orientation of the instrument; at least one inertial sensor unit connected to the at least one instrument, the inertial sensor unit producing readings representative of its orientation; a computer-assisted surgery processor unit operating a surgical assistance procedure and comprising a coordinate system module for setting a pelvic coordinate system from readings of the at least one inertial sensor unit when the at least one instrument has the acetabulum abutment end received in the acetabulum, the coordinate system module setting the pelvic coordinate system by obtaining a plurality of orientation values from the at least one inertial sensor unit when the rim abutment is abutted against locations of the rim, one of said orientation values having the indicator aligned with a reference landmark, the coordinate system module defining an acetabular plane representative of the pelvic coordinate system from the plurality of orientation values; and a tracking module for tracking an orientation of the at least one inertial sensor unit relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor unit, and an interface for outputting orientation data as a function of the pelvic coordinate system.

[0006] Further in accordance with the first embodiment, the at least one instrument has a pin guide thereon adapted to position a pin in the acetabulum in a desired location relative to the pelvic coordinate system.

[0007] Still further in accordance with the first embodiment, the indicator is a light source emitting a light beam on the reference landmark.

[0008] Still further in accordance with the first embodiment, a first of the orientation values obtained has the indicator aligned with a reference landmark.

[0009] Still further in accordance with the first embodiment, said first of the orientation values is programmed from preoperative imaging as being representative of a patient orientation.

[0010] Still further in accordance with the first embodiment, the tracking module tracks at least one tool supporting one of the inertial sensor unit relative to the pelvic coordinate system.

[0011] Still further in accordance with the first embodiment, the tracking module calculates at least one of an anteversion and an inclination of the at least one tool relative to the pelvis.

[0012] In accordance with a second embodiment of the present disclosure, there is provided a computer-assisted surgery (CAS) system for tracking an orientation of a pelvis comprising: at least one instrument, the instrument having an acetabulum abutment end adapted to be abutted against a rim of the acetabulum in a planned complementary abutment; at least one inertial sensor unit connected to the at least one instrument, the inertial sensor unit producing readings representative of its orientation; a computer-assisted surgery processor unit operating a surgical assistance procedure and comprising a coordinate system module for setting a pelvic coordinate system from readings of the at least one inertial sensor unit when the at least one instrument has the acetabulum abutment end abutted against a rim of the acetabulum in a planned complementary manner, the coordinate system module setting the pelvic coordinate system by defining an acetabular plane representative of the pelvic coordinate system based on the planned complementary abutment; and a tracking module for tracking an orientation of the at least one inertial sensor unit relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor unit, and an interface for outputting orientation data as a function of the pelvic coordinate system.

[0013] Further in accordance with the second embodiment, the at least one instrument has a pin guide thereon adapted to position a pin in the acetabulum in a desired location relative to the pelvic coordinate system.

[0014] Still further in accordance with the second embodiment, the tracking module tracks at least one tool supporting one of the inertial sensor unit relative to the pelvic coordinate system.

[0015] Still further in accordance with the second embodiment, the tracking module calculates at least one of an anteversion and an inclination of the at least one tool relative to the pelvis.

[0016] Still further in accordance with the second embodiment, the acetabulum abutment end is a tripod having three abutment tabs adapted to be abutted in the planned complementary abutment.

[0017] Still further in accordance with the second embodiment, the acetabulum abutment end is patient-specifically fabricated based on preoperative imaging of the patient.

[0018] Still further in accordance with the second embodiment, the acetabulum abutment end has adjustable prongs connected to a remainder of the instrument by a lockable joints, for the acetabulum abutment end to be arranged for the planned complementary abutment based on preoperative imaging of the patient.

[0019] Still further in accordance with the second embodiment, each said prong has a translational DOF joint and a rotational DOF joint.

[0020] In accordance with a third embodiment of the present disclosure, there is provided a method for tracking an orientation of a pelvis in computer-assisted hip surgery comprising: obtaining an instrument having an inertial sensor unit, an acetabulum abutment end adapted to contact a rim of an acetabulum, and a rotation indicator; initializing an orientation of the instrument with the acetabulum abutment end against the rim of the acetabulum and with the rotation indicator aligned with a pelvic landmark; recording the orientation for at least the initial orientation; defining an acetabular plane representative of a pelvic coordinate system from the orientation; and producing orientation data relative to the pelvic coordinate system using inertial sensor units.

[0021] Further in accordance with the third embodiment, producing orientation data comprises producing anteversion and/or inclination angles of a tool with an inertial sensor unit relative to the pelvis.

[0022] Still further in accordance with the third embodiment, recording the orientation comprises recording a plurality of orientation values each associated with a different contact location between the rim and the acetabulum abutment end.

[0023] Still further in accordance with the third embodiment, guiding an installation of a pin whose orientation is known in the pelvic coordinate system.

[0024] Still further in accordance with the third embodiment, initializing an orientation of the instrument with the acetabulum abutment end against the rim of the acetabulum and with the rotation indicator aligned with a pelvic landmark is based on preoperative imaging representative of a patient orientation.

BRIEF DESCRIPTION OF THE DRAWINGS

[0025] Fig. 1 is a perspective view of an acetabulum rim digitizer device in accordance with the present disclosure, relative to a pelvis;

[0026] Fig. 2 is an enlarged perspective view of a tooling end of the acetabulum rim digitizer device of Fig. 1;

[0027] Fig. 3 is an enlarged elevation view of a tooling end of an acetabulum rim digitizer device with planar surface in accordance with another embodiment of the present disclosure;

[0028] Fig. 4 is a perspective view of the acetabulum rim digitizer device of Fig. 3; and

[0029] Fig. 5 is a perspective view of an acetabulum rim digitizer device with prongs in accordance with another embodiment of the present disclosure.

DESCRIPTION OF THE EXEMPLARY EMBODIMENTS

[0030] Referring to the drawings and more particularly to Figs. 1 and 2, an acetabulum rim digitizer device or instrument is generally shown at 10, relative to a pelvis P having an acetabulum A, the acetabulum having a rim R. The device 10 and method related to the device 10 may be used to determine pelvic orientation data in various forms (e.g., pelvic tilt, anteversion/inclination of acetabulum, etc). The device 10 may also be used to accurately navigate instruments used in hip arthroplasty or like procedures, including bone model and cadaver testing, such as an acetabular reamer, a cup impactor, an impactor guiding pin, using inertial sensors.

[0031] The device 10 has an elongated body 11 having a tooling end 12 and a handle end 14. Although illustrated as having an axially offset portion, the body of the device 10 may also be fully straight or have any other appropriate shape.

[0032] The device 10 has a receptacle 16 for releasably receiving therein an inertial sensor unit 18, in a known manner. Alternatively, the inertial sensor unit 18 may be integral or embedded into the elongated body 11. The inertial sensor unit 18 may have a gyroscope set to track the orientation of the device 10, by integrating the angular velocity data recorded by the sensor through a registration process. The inertial sensor unit 18 may also comprise an accelerometer set used to calibrate an initial position of the device 10, and to correct gyroscope drift when stable positions are recorded. Other types of inertial sensors may be provided in the inertial sensor unit 18 to complement the data or as alternatives to the accelerometer and/or gyroscope, such as inclinometers, magnetometers, among other possible inertial sensors.

[0033] The inertial sensor unit 18 uses its inertial sensor readings to continually calculate the orientation and velocity of a body without the need for an external reference, i.e., no signal transmission from outside of the sensor assembly is necessary, the inertial sensor unit 18 is self-contained. This process is commonly known as dead reckoning and is documented and forms part of the common general knowledge. An initial orientation and velocity must be provided to the inertial sensor unit 18, i.e., the X-Y-Z coordinate system of Fig. 1, after which the orientation is tracked by integrating the angular rates of gyroscope readings at each time step. With an accurate estimate of the orientation of the inertial sensor unit 18 with respect to the World frame of reference, gravitational effects can be

removed and inertial forces acting on the accelerometers can be integrated to track changes in velocity and position. Since the inertial sensor unit 18 has no need for an external reference, it may be immune to environmental factors such as magnetic fields and operate under a wide range of conditions.

[0034] The inertial sensor unit 18 is part of a computer-assisted hip surgery system for navigating instruments, used to implement the method 10, as will be detailed below. The system comprises a computer-assisted surgery (CAS) processing unit 19, that may be a stand-alone computer connected to the inertial sensor unit 18, for instance by wireless communication. It is however pointed out that the CAS processing unit may be partially or entirely integrated into the inertial sensor unit 18, also known as pod. The inertial sensor unit 18, when incorporating the CAS processing unit, may thus be equipped with user interfaces to provide the navigation data, whether it be in the form of LED displays, screens, numerical displays, etc. The computer-assisted surgery (CAS) processing unit 19 may have a coordinate system module 19A and a tracking module 19B, described in further detail hereinafter, and part of a surgical assistance procedure programmed into the CAS processing unit 19.

[0035] A hemispherical base 20 is secured to the tooling end 12. The base 20 may be releasably connected to the body 11 (e.g., by screwing engagement) to enable the selection of a base 20 of appropriate dimension, based on the acetabulum being operated on. The geometry of the base 20 may be known as quasi-hemispherical, frusto-spherical, etc. Indeed, as the base 20 is seated into the acetabulum during registration, it is expected that the base 20 is well seated in the acetabulum and does not shift position during the registration process. For this purpose, pressure sensor(s) may be provided on or near the surface of the base 20. The pressure sensor(s) provides signals that can be monitored to determine whether the base 20 is adequately applied against the surface of the acetabulum.

[0036] The device 10 may additional comprise a tab 22, which is spaced apart from the base 20 and is designed to be seated on the acetabulum rim for each acquired points, as observed in Figs. 1 and 2. The device 10 may further have a rotation indicator 24, used to define a fixed rotation axis, not parallel to the rim plane normal, to build a full coordinate system for the acetabulum. In the illustrated embodiment, the rotation indicator 24 is a light source emitting a visible light beam, although other rotation indicators may be used such as

a mechanical arm, a laser, a marking on the instrument, or any other visual indicator. A pin guide 26 may also be provided as projecting laterally from the elongated body 11, featuring a slot for guiding the insertion of a pin 28 in the pelvis, following the registration. The rotation indicator 24 is in a known physical orientation in the coordinate system of the inertial sensor unit 18.

[0037] The CAS processing unit is programmed with geometric data relating the body 11 (e.g., its axes) to the orientation of the components thereon, such as the base 20, the tab 22 and the rotation indicator 24. This geometric data, obtained pre-operatively, is used by the CAS processing unit (shown as 18) to perform the method and sequence described below.

[0038] Still referring to Fig. 1, the acetabulum rim digitizer device 10 may be used intra-operatively with the following intraoperative method:

1. Either prior to or following reaming of the acetabulum A, the base 20 of the device 10 is seated into the acetabulum A. The base 20 has been selected and installed to have a diameter complementary to that of the acetabulum A.
2. The rotation indicator 24 is used to give a predetermined orientation to the device 10. Depending on the embodiment, this rotation indicator 24 may be oriented to point, mark, touch a pre-operatively identifiable landmark. For example, in the case of the pelvis, the identifiable landmark may be lateral anterior-superior iliac spine (ASIS), the 12 o'clock feature of the acetabulum rim, the acetabulum notch, among other features.
3. Registration may be initiated, through the user interface of the CAS processing unit (e.g., button on the inertial sensor unit 18 is turned on).
4. Without unseating the base 20, for example as confirmed from the pressure sensor(s) in the base 20 or by having the operator applying suitable pressure on the device 10, the device 10 is manually rotated to position the tab 22 onto a different segment of the acetabulum rim R (Fig. 2).
5. Either through a user request or through a stability criterion, the inertial sensor unit 18 records the current orientation of the digitizer device 10 and provides feedback to the user, for confirmation.

6. The steps 4 – 5 are repeated until a sufficient number of acetabulum rim positions are recorded by the inertial sensor unit 18, for instance as indicated by the inertial sensor unit 18 or based on a predetermined number of measurements required.

7. The CAS processing unit (e.g., incorporating the inertial sensor unit 18) then records and provides data related to the acetabulum orientation or pelvic tilt, in any appropriate form (i.e., the pelvic coordinate system).

[0039] To perform the method described above, the CAS processing unit must be programmed in the following sequence:

1. The CAS processing unit sets the initial orientation of the acetabulum rim digitizer device 10 when the user initiates the initial recording. This initial position is recorded by assuming arbitrary yaw, roll and pitch are provided by the accelerometer set in the inertial sensor unit 18. From this initial position, and knowing the orientation of the rotation indicator 24 relative to the rim digitizer device 10, the rotation axis may be defined as:

rotationAxisInWorld

2. After initialization of the registration, the gyroscope set in the inertial sensor unit 18 is used to track the orientation of the acetabulum rim digitizer device 10. The orientation of the device 10 is recorded at the various points of contact between the tab 22 and the acetabulum rim R. The inclination data (roll & pitch) provided by the accelerometer set in the inertial sensor unit 18 may be used to correct drift in the gyroscope data (for instance, using Kalman or Complementary filters). The collection of orientation data at various points provides the orientation of the rim digitizer device 10 in the World coordinate system:

rimDigitizerInWorld

3. At the various points of contact, with the stable orientation the position of the tab 22 may thus be calculated based on the orientation of the rim digitizer device 10 obtained. Each of these positions is recorded in a coordinate system maintained by the CAS processing unit, and is representative of a point on the acetabulum rim R. According to an embodiment, the origin of the coordinate system is located at the center of the

hemispherical base 20. As such the position of each point on the rim can be identified as follow:

$$\text{rimPointInWorld} = \text{rimDigitizerInWorld} * \text{tabInRimDigitizerCenter}$$

4. When a sufficient number of points has been recorded, the rim points registered can be used to define an acetabular rim plane. According to an embodiment, a plane is fitted through the rim points using an appropriate method such as Least Squares Fitting. This acetabular rim plane is therefore known:

$$\text{rimPlaneNormalInWorld}$$

5. The acetabular rim plane is used to build an acetabulum coordinate system, as follows:

$$\begin{aligned} \text{rimXAxis} &= \text{rimPlaneNormalInWorld} \\ \text{rimZAxis} &= \text{rimXAxis} * \text{rotationAxisInWorld} \\ \text{rimYAxis} &= \text{rimZAxis} * \text{rimXAxis} \\ \text{acetabulumInWorld} &= [\text{rimXAxis} \text{ rimYAxis} \text{ rimZAxis}] \end{aligned}$$

6. Using pre-operative planning data (CT-Scan, two-dimensional X-Rays, 3-D modeling, etc...), the pelvis coordinate system is created. Any standard definition may be used, for example the Lewinnek pelvic coordinate system. The pre-operative planning data may be referenced to the acetabulum coordinate system, using the same landmarks and rotation features as used during the registration method. Through data inferred from the pre-operative planning, the relationship between the acetabulum coordinate system and the pelvis coordinate system may be established. By inputting this relationship into the navigation system, the following relationship is obtained:

$$\text{pelvisInWorld} = \text{acetabulumInWorld} * \text{pelvisInAcetabulum}$$

7. The gravity axis of the World coordinate system may also be used to determine the pelvic tilt from the computed pelvisInWorld coordinate system.

[0040] In the embodiment described above, the acetabular rim plane acquired with landmarks may be matched with a plane defined in pre-operative planning. Alternatively, or

additionally, the CAS processing unit may instead match the rim landmarks with a surface defined in pre-operative planning. This surface can be a 3D surface representing the acetabulum rim contour. The CAS processing unit can calculate using Least Squares Fitting the transformation on the acquired rim points which positions the points closest to the pre-planning contour of the acetabulum rim R.

[0041] The surface can also be a set of 2D contours, acquired using X-Rays images, combined with respective projective camera calibrations. In one embodiment, camera calibration could be performed as per F. CHERIET et al, Int. J. Patt. Recogn. Artif. Intell. 13, 761 (1999). DOI: 10.1142/S0218001499000434 TOWARDS THE SELF-CALIBRATION OF A MULTIVIEW RADIOGRAPHIC IMAGING SYSTEM FOR THE 3D RECONSTRUCTION OF THE HUMAN SPINE AND RIB CAGE. The CAS processing unit could compute by Least Squares Fitting the transformation on the acquired rim points for which a retro-projection of the points onto the X-Ray, as defined by the projective camera model, is closest to the defined 2D contour.

[0042] In another embodiment, an ultrasound device may be fixed to the device 10, for ultrasound readings to be obtained when the device 10 is seated into the acetabulum A. The ultrasound readings may be used to create the rim surface, and thus replaces the tab 22 of the device 10, alleviating the need for physical contact with the acetabulum rim R. As the base 20 is seated into the acetabulum A and the ultrasound device is held still relative to the acetabulum, it is possible to rebuild the acetabulum rim surface accurately in space when combining the ultrasound data with the orientation data provided from the inertial sensor unit 18. This information can be used to match the registered rim contour with the pre-operative planned contour.

[0043] Using the device 10, the pin 28 may be positioned to a desired orientation, using the orientation data. For example, the pin 28 may be driven into the pelvis so as to serve as an impactor guide. The longitudinal axis of the pin 28 could thus be driven to an orientation parallel to a normal of the acetabulum rim plane. In an embodiment, the navigation of the device 10 for pin placement is done by providing anteversion and inclination values to the user.

[0044] Referring to Figs. 3 and 4, in yet another embodiment, a planar surface 30, or multiple coplanar features (three fixed tabs in Fig. 4), may be used as an alternative to the

tab 22 at the tooling end 12 of the elongated body 11. The base 20 may or may not be present, although the base 20 may provide some manipulation stability to aid in applying the planar surface 30 to the acetabular rim R. The device 10 of Figs. 3 and 4 could be used to acquire, in a single step, the planar surface as well as the rotation landmark. The device 10 has a configuration that is planned to be in a unique complementary engagement with the rim of the acetabulum, for instance based on pre-operative imaging for instance by having patient specific contact surfaces being negatives of patient tissue for unique complementary engagement. With the embodiment of Figs. 3 and 4, steps 4-6 of the method described above would not be necessary, provided suitable pre-planning is performed. Similarly, steps 2-4 of the sequence performed by the CAS processing unit are no longer required. The inertial sensor unit 18 may not need a gyroscope set for the embodiment of Figs. 3 and 4.

[0045] Referring to Fig. 5, in yet another embodiment, three adjustable prongs 50 may be used as alternatives to the planar surface 30, effectively forming a tripod. When used, the user is requested to position all of the prongs onto known landmarks (e.g., unique complementary engagement, based on pre-operative imaging). The prongs 50 have abutment ends 51, displaceable axially (e.g., along a longitudinal axis of the body 11) and in rotation (e.g., about an axis parallel to the longitudinal axis of the body 11). Hence, the prongs 50 are each provided with a housing 52 enabling lockable translational DOF and rotational DOF.

[0046] The known landmarks against which the ends 51 of the prongs 50 are to be abutted are either defined by identifiable anatomical landmarks, or by for instance, constraining the rotation of the instrument by using a stopper in the acetabulum notch.

[0047] For the embodiment of Fig. 5, the pre-operative planning is be used to define the unique adjustments to the tripod to extend to the prongs 50, and to identify the unique position of the device 10 when positioned into the acetabulum A with the predetermined abutment between the prongs 50 and the pelvis P.

[0048] As the position of the device 10 of Fig. 5 is unique with regards to the pelvis anatomy, a single reading of an inclinometer in the inertial sensor unit 18 would be sufficient to record the current pelvis tilt.

[0049] A method used in combination with the device 10 of Fig. 5 would be as follows:

1. During the pre-operative planning, identify three landmarks to be used.
2. A coordinate system is created from these three landmarks, the relationship between this coordinate system and pelvis coordinate system would also be known from pre-operative planning.
3. From the data computed from the pre-operative planning, the required adjustments on the tripod would be performed to set the position and/or orientation of each prong 50.
4. The device 10 is then positioned in the manner shown in Fig. 5 onto the pre-identified landmarks, either visually or by using a mechanical feature to constrain rotation.
5. When stable, the orientation data for the device 10 is recorded using the inertial sensor unit 18, and this data is used to calculate the pelvis tilt by using the known relationship between the device 10 and the pelvis P.

$$pelvisInWorld = tripodInWorld * pelvisInTripod$$

[0050] The device 10 of any of the preceding figures is therefore used to provide a means for intra-operatively evaluating the tilt of the pelvis and obtain acetabular orientation data, whether the surgery is performed in supine or lateral decubitus. The data provided by the CAS processing unit may be used, for instance, to reposition the pelvis onto the table, to guide the user in aligning a non-navigated instrument with a desired cup alignment or be used as an input for navigation of surgical instruments during total hip arthroplasty procedure. Although cross-products of axes are discussed above, vectors representative of a direction of the axes may be used for the cross-products.

[0051] As shown in Fig. 1, the CAS processor unit 19 may have a coordinate system module 19A and a tracking module 19B. Based on the embodiment the CAS processor unit 19 supports, the modules 19A and 19B may have different functions. For example, for the embodiment of Figs. 1 and 2, the coordinate system module 19A sets a pelvic coordinate

system from readings of the inertial sensor unit 18 when the at least one instrument 10 has the acetabulum abutment end received in the acetabulum. The coordinate system module 19A sets the pelvic coordinate system by obtaining a plurality of orientation values from the inertial sensor unit 18 when the rim abutment tab 22 is abutted against locations of the rim. One of the orientation values has the indicator 24 aligned with a reference landmark. Thus, the coordinate system module 19A defines an acetabular plane representative of the pelvic coordinate system from the plurality of orientation values. The tracking module 19B then tracks an orientation of inertial sensor units relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor units.

[0052] As another example, for the embodiment of Figs. 3-5, the coordinate system module 19A sets a pelvic coordinate system from readings of the inertial sensor unit 18 when the instrument 10 has the acetabulum abutment end abutted against a rim of the acetabulum in the planned complementary manner. The coordinate system module 19A sets the pelvic coordinate system by defining an acetabular plane representative of the pelvic coordinate system based on the planned complementary abutment. The tracking module 19B then tracks an orientation of inertial sensor units relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor units.

CLAIMS:

1. A computer-assisted surgery (CAS) system for tracking an orientation of a pelvis comprising:

at least one instrument, the instrument having an acetabulum abutment end adapted to be received in an acetabulum, a rim abutment adapted to be abutted against a rim of the acetabulum, and an indicator representative of a physical orientation of the instrument;

at least one inertial sensor unit connected to the at least one instrument, the inertial sensor unit producing readings representative of its orientation;

a computer-assisted surgery processor unit operating a surgical assistance procedure and comprising

a coordinate system module for setting a pelvic coordinate system from readings of the at least one inertial sensor unit when the at least one instrument has the acetabulum abutment end received in the acetabulum, the coordinate system module setting the pelvic coordinate system by obtaining a plurality of orientation values from the at least one inertial sensor unit when the rim abutment is abutted against locations of the rim, one of said orientation values having the indicator aligned with a reference landmark, the coordinate system module defining an acetabular plane representative of the pelvic coordinate system from the plurality of orientation values; and

a tracking module for tracking an orientation of the at least one inertial sensor unit relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor unit, and

an interface for outputting orientation data as a function of the pelvic coordinate system.

2. The CAS system according to claim 1, wherein the at least one instrument has a pin guide thereon adapted to position a pin in the acetabulum in a desired location relative to the pelvic coordinate system.

3. The CAS system according to any one of claims 1 and 2, wherein the indicator is a light source emitting a light beam on the reference landmark.

4. The CAS system according to any one of claims 1 to 3, wherein a first of the orientation values obtained has the indicator aligned with a reference landmark.
5. The CAS system according to claim 4, wherein said first of the orientation values is programmed from preoperative imaging as being representative of a patient orientation.
6. The CAS system according to any one of claims 1 to 5, wherein the tracking module tracks at least one tool supporting one of the inertial sensor unit relative to the pelvic coordinate system.
7. The CAS system according to claim 6, wherein the tracking module calculates at least one of an anteversion and an inclination of the at least one tool relative to the pelvis.
8. A computer-assisted surgery (CAS) system for tracking an orientation of a pelvis comprising:
 - at least one instrument, the instrument having an acetabulum abutment end adapted to be abutted against a rim of the acetabulum in a planned complementary abutment;
 - at least one inertial sensor unit connected to the at least one instrument, the inertial sensor unit producing readings representative of its orientation;
 - a computer-assisted surgery processor unit operating a surgical assistance procedure and comprising
 - a coordinate system module for setting a pelvic coordinate system from readings of the at least one inertial sensor unit when the at least one instrument has the acetabulum abutment end abutted against a rim of the acetabulum in a planned complementary manner, the coordinate system module setting the pelvic coordinate system by defining an acetabular plane representative of the pelvic coordinate system based on the planned complementary abutment; and
 - a tracking module for tracking an orientation of the at least one inertial sensor unit relative to the pelvic coordinate system during movements thereof using the readings from the inertial sensor unit, and
 - an interface for outputting orientation data as a function of the pelvic coordinate system.

9. The CAS system according to claim 8, wherein the at least one instrument has a pin guide thereon adapted to position a pin in the acetabulum in a desired location relative to the pelvic coordinate system.
10. The CAS system according to any one of claims 8 and 9, wherein the tracking module tracks at least one tool supporting one of the inertial sensor unit relative to the pelvic coordinate system.
11. The CAS system according to claim 10, wherein the tracking module calculates at least one of an anteversion and an inclination of the at least one tool relative to the pelvis.
12. The CAS system according to any one of claims 8-11, wherein the acetabulum abutment end is a tripod having three abutment tabs adapted to be abutted in the planned complementary abutment.
13. The CAS system according to any one of claims 8-12, wherein the acetabulum abutment end is patient-specifically fabricated based on preoperative imaging of the patient.
14. The CAS system according to any one of claims 8-11, wherein the acetabulum abutment end has adjustable prongs connected to a remainder of the instrument by a lockable joints, for the acetabulum abutment end to be arranged for the planned complementary abutment based on preoperative imaging of the patient.
15. The CAS system according to claim 14, wherein each said prong has a translational DOF joint and a rotational DOF joint.
16. A method for tracking an orientation of a pelvis in computer-assisted hip surgery comprising:
- obtaining an instrument having an inertial sensor unit, an acetabulum abutment end adapted to contact a rim of an acetabulum, and a rotation indicator;
 - initializing an orientation of the instrument with the acetabulum abutment end against the rim of the acetabulum and with the rotation indicator aligned with a pelvic landmark;
 - recording the orientation for at least the initial orientation;
 - defining an acetabular plane representative of a pelvic coordinate system from the orientation; and

producing orientation data relative to the pelvic coordinate system using inertial sensor units.

17. The method according to claim 16, wherein producing orientation data comprises producing anteversion and/or inclination angles of a tool with an inertial sensor unit relative to the pelvis.

18. The method according to claim 16, wherein recording the orientation comprises recording a plurality of orientation values each associated with a different contact location between the rim and the acetabulum abutment end.

19. The method according to claim 16, further comprising guiding an installation of a pin whose orientation is known in the pelvic coordinate system.

20. The method according to claim 16, wherein initializing an orientation of the instrument with the acetabulum abutment end against the rim of the acetabulum and with the rotation indicator aligned with a pelvic landmark is based on preoperative imaging representative of a patient orientation.

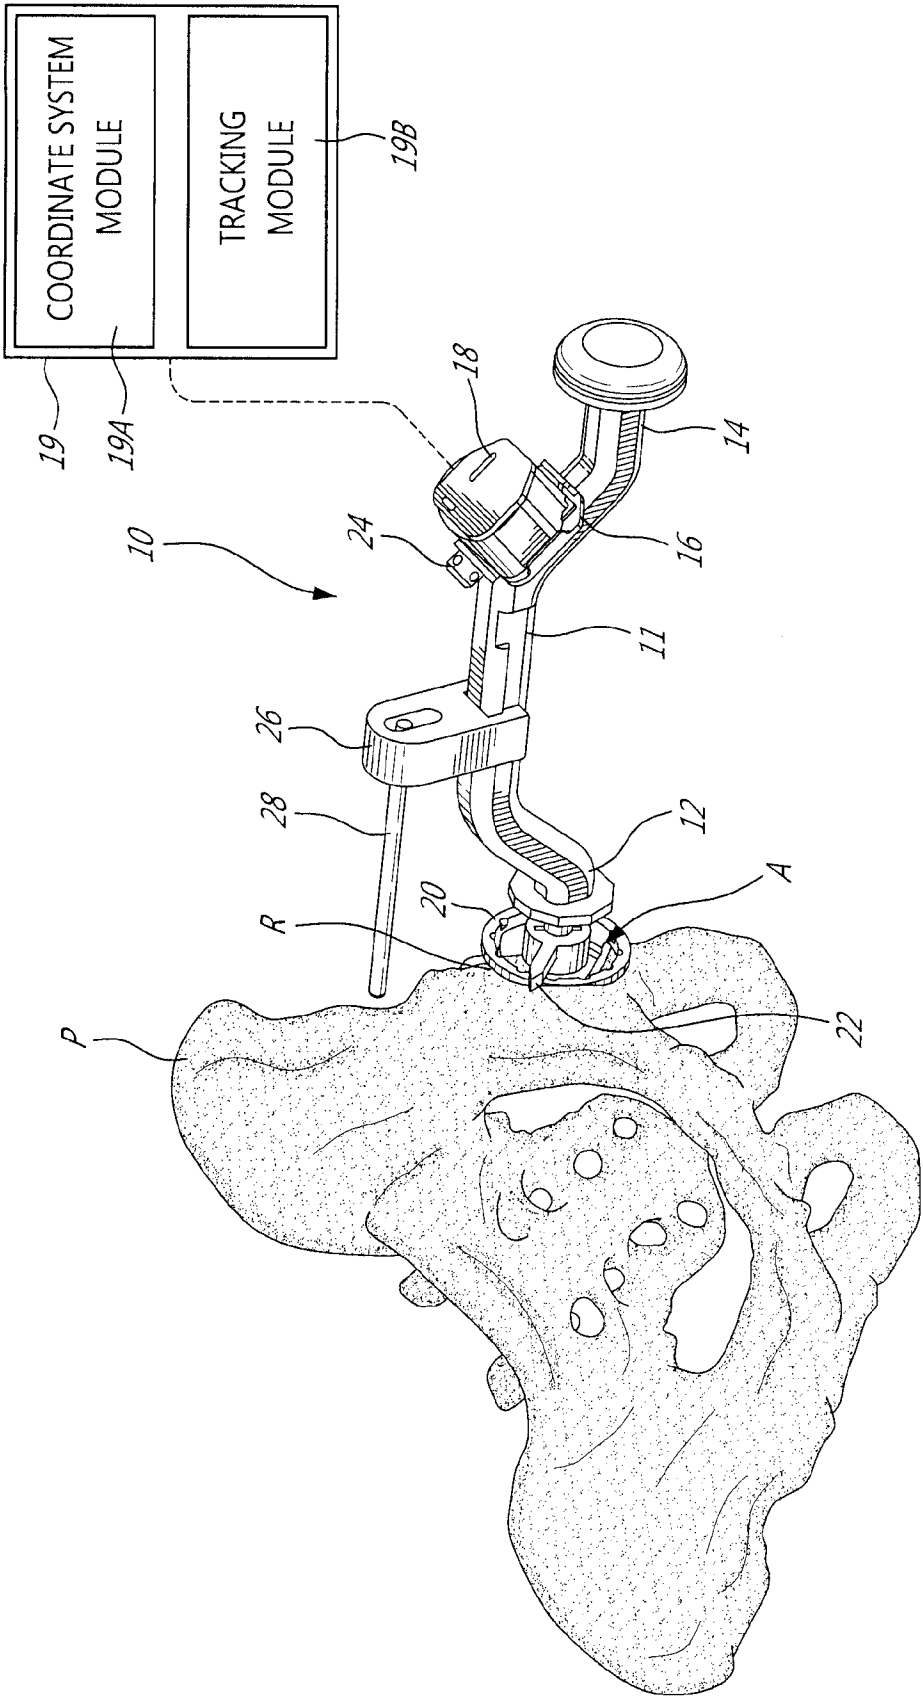


FIG. 1

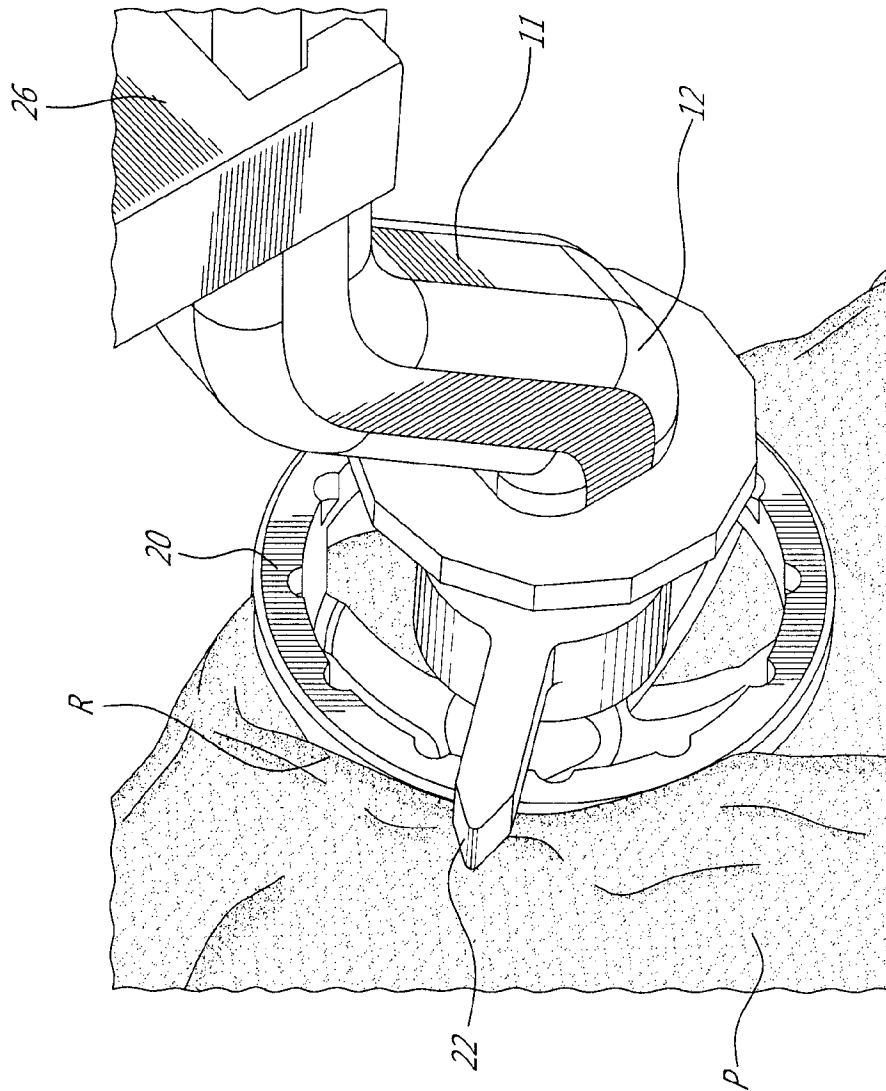
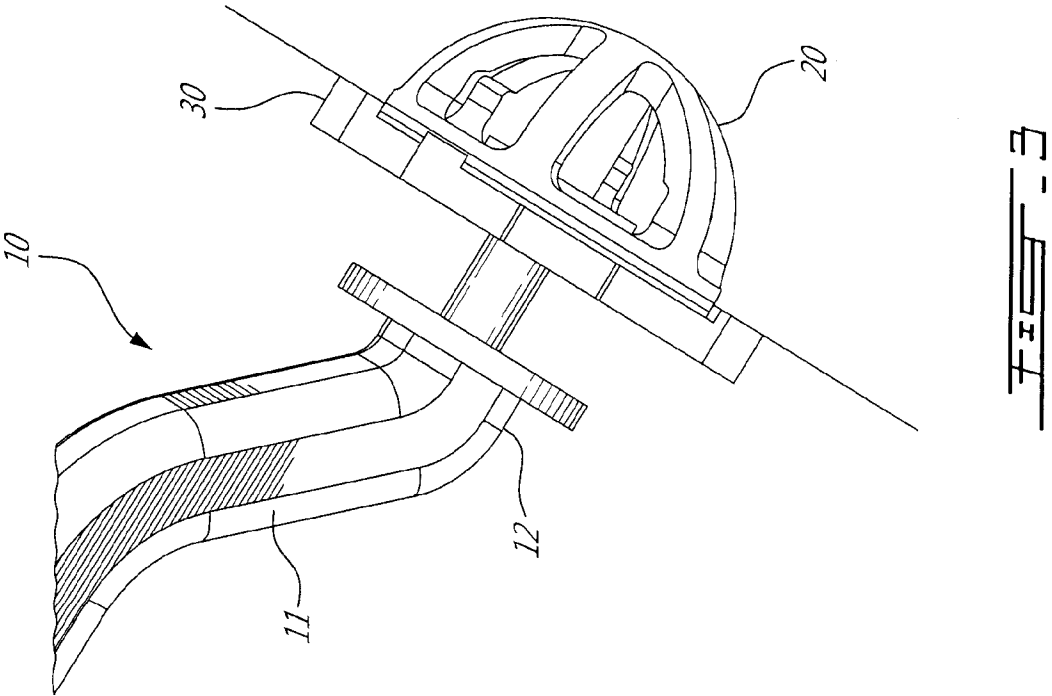


FIG. 2




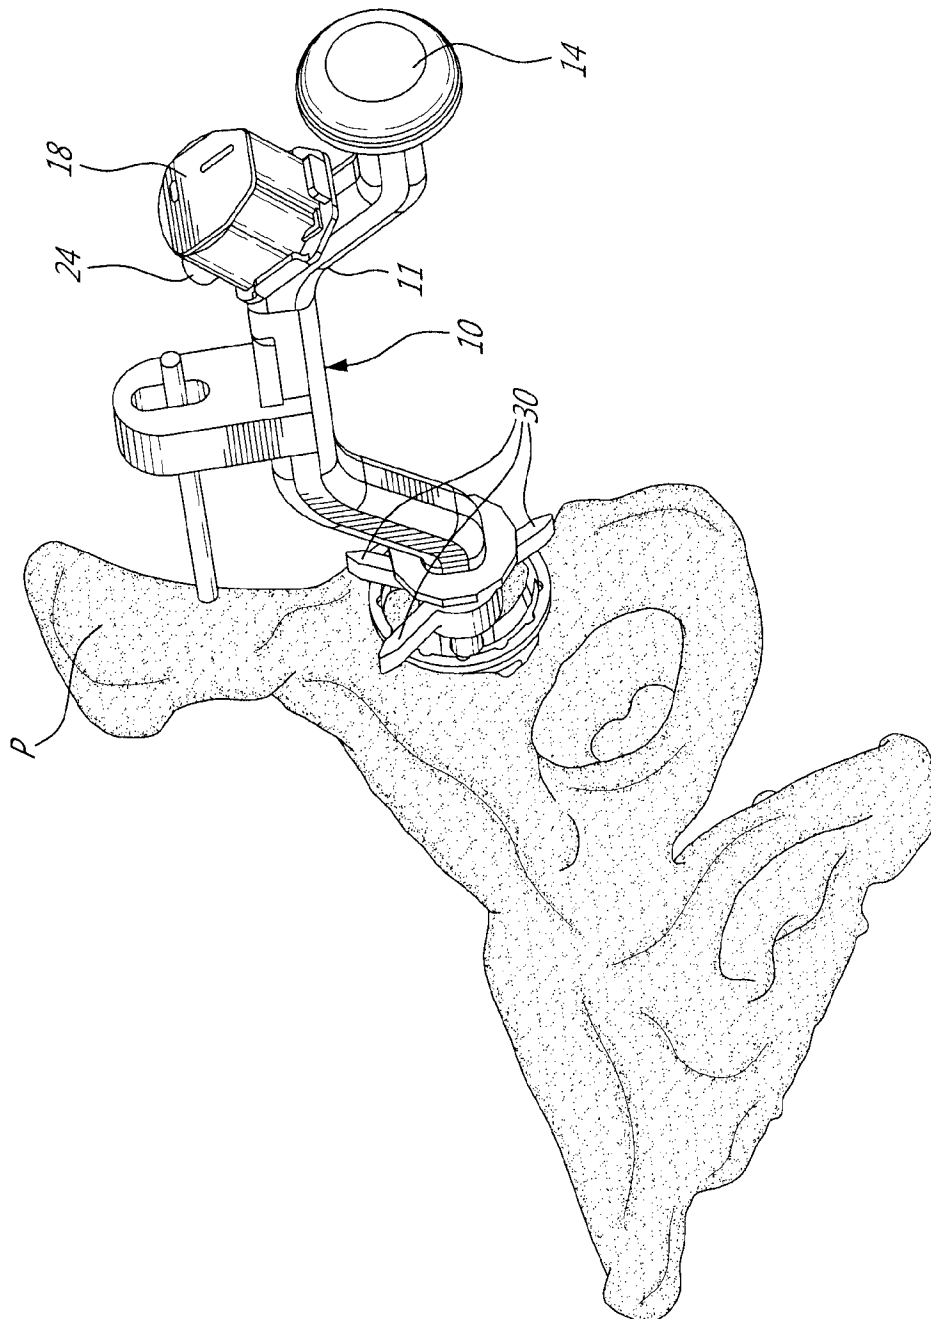


FIG. 4

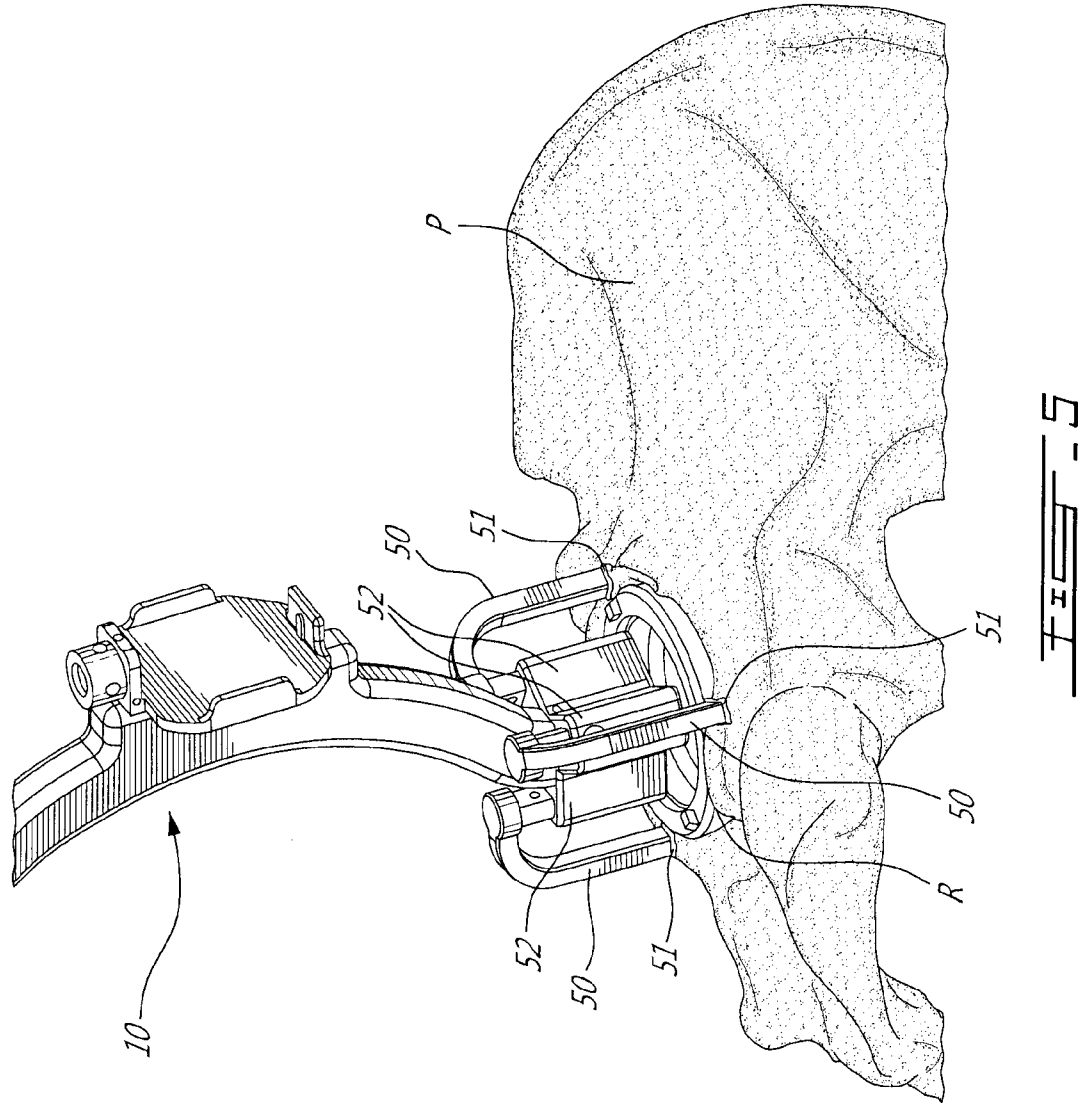

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/050089

A. CLASSIFICATION OF SUBJECT MATTER

IPC: **A61B 34/20** (2016.01), **A61B 17/74** (2006.01), **A61B 17/90** (2006.01), **A61B 34/00** (2016.01), **A61F 2/34** (2006.01), **A61F 2/46** (2006.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC: A61B-all, A61F 2/34, A61F 2/46

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used)

Questel-Orbit (Fulltext), Canadian Patent Database

Keywords: acetabular plane, inertial sensor, rim, stopper, acetabulum, CAS

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US2005/0021044 (STONE et al.) 27-January-2005 (27-01-2005) Figures 17-19B, Paragraphs 0081-0085	8, 10-17, 20
A	US2014/0031722 (LI et al.) 30-January-2014 (30-01-2014) Entire document	1
A	US2014/0052149 (WALT et al.) 20-February-2014 (20-02-2014) Entire document	1
A	US2008/0255584 (BEVERLAND et al.) 16-October-2008 (16-10-2008) Entire document	1
A	US2010/0249796 (NYEZ) 30-September-2010 (30-09-2010) Figures	1
A	US2014/0364858 (LI et al.) 11-December-2014 (11-12-2014) Entire document	1

☐ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* "A" "E" "L" "O" "P"	Special categories of cited documents: document defining the general state of the art which is not considered to be of particular relevance earlier application or patent but published on or after the international filing date document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) document referring to an oral disclosure, use, exhibition or other means document published prior to the international filing date but later than the priority date claimed	"I" "X" "Y" "&"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art document member of the same patent family
--------------------------------------	--	--------------------------	--

Date of the actual completion of the international search
04 March 2016 (04-03-2016)

Date of mailing of the international search report
22 March 2016 (22-03-2016)

Name and mailing address of the ISA/CA
Canadian Intellectual Property Office
Place du Portage I, C114 - 1st Floor, Box PCT
50 Victoria Street
Gatineau, Quebec K1A 0C9
Facsimile No.: 819-953-2476

Authorized officer

Hoan Huynh (819) 639-7857

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/CA2016/050089

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
US2005021044A1	27 January 2005 (27-01-2005)	US2005021044A1 US8057482B2 AT540612T EP1635705A2 EP1635705B1 ES2380100T3 JP2007503289A US2005251026A1 US7559931B2 US2007125928A1 US7784762B2 US2010016705A1 US8057479B2 US2009318931A1 US8888786B2 US2012130279A1 US8974467B2 US2009318836A1 US2009318930A1 US2010288892A1 US2015238204A1 WO2004107932A2 WO2004107932A3 WO2004112610A2 WO2004112610A3	27 January 2005 (27-01-2005) 15 November 2011 (15-11-2011) 15 January 2012 (15-01-2012) 22 March 2006 (22-03-2006) 11 January 2012 (11-01-2012) 08 May 2012 (08-05-2012) 22 February 2007 (22-02-2007) 10 November 2005 (10-11-2005) 14 July 2009 (14-07-2009) 07 June 2007 (07-06-2007) 31 August 2010 (31-08-2010) 21 January 2010 (21-01-2010) 15 November 2011 (15-11-2011) 24 December 2009 (24-12-2009) 18 November 2014 (18-11-2014) 24 May 2012 (24-05-2012) 10 March 2015 (10-03-2015) 24 December 2009 (24-12-2009) 24 December 2009 (24-12-2009) 18 November 2010 (18-11-2010) 27 August 2015 (27-08-2015) 16 December 2004 (16-12-2004) 29 September 2005 (29-09-2005) 29 December 2004 (29-12-2004) 06 May 2005 (06-05-2005)
US2014031722A1	30 January 2014 (30-01-2014)	US2014031722A1 CA2866192A1 CN104220021A EP2879610A1 WO2014019086A1	30 January 2014 (30-01-2014) 06 February 2014 (06-02-2014) 17 December 2014 (17-12-2014) 10 June 2015 (10-06-2015) 06 February 2014 (06-02-2014)
US2014052149A1	20 February 2014 (20-02-2014)	US2014052149A1 AU2013303055A1 CA2879409A1 EP2884921A1 JP2015524733A WO2014028227A1	20 February 2014 (20-02-2014) 05 February 2015 (05-02-2015) 20 February 2014 (20-02-2014) 24 June 2015 (24-06-2015) 27 August 2015 (27-08-2015) 20 February 2014 (20-02-2014)
US2008255584A1	16 October 2008 (16-10-2008)	US2008255584A1 US8206405B2 AT539711T EP1893138A2 EP1893138B1 GB0507243D0 JP2008534208A JP4943419B2 WO2006109022A2 WO2006109022A3	16 October 2008 (16-10-2008) 26 June 2012 (26-06-2012) 15 January 2012 (15-01-2012) 05 March 2008 (05-03-2008) 04 January 2012 (04-01-2012) 18 May 2005 (18-05-2005) 28 August 2008 (28-08-2008) 30 May 2012 (30-05-2012) 19 October 2006 (19-10-2006) 18 January 2007 (18-01-2007)
US2010249796A1	30 September 2010 (30-09-2010)	US2010249796A1 US8337426B2 AU2013222609A1 AU2013222609B2 CA2725220A1 CN101086600A CN100533248C DE102011082902A1 DE112010003901T5 DE112011100810T5	30 September 2010 (30-09-2010) 25 December 2012 (25-12-2012) 11 September 2014 (11-09-2014) 05 November 2015 (05-11-2015) 03 December 2009 (03-12-2009) 12 December 2007 (12-12-2007) 26 August 2009 (26-08-2009) 22 March 2012 (22-03-2012) 15 November 2012 (15-11-2012) 21 February 2013 (21-02-2013)

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/050089

US2011160867A1	30 June 2011 (30-06-2011)
US8535387B2	17 September 2013 (17-09-2013)
US2011093086A1	21 April 2011 (21-04-2011)
US8568487B2	29 October 2013 (29-10-2013)
US2011071533A1	24 March 2011 (24-03-2011)
US8591516B2	26 November 2013 (26-11-2013)
US2011224674A1	15 September 2011 (15-09-2011)
US8603180B2	10 December 2013 (10-12-2013)
US2009024131A1	22 January 2009 (22-01-2009)
US8608748B2	17 December 2013 (17-12-2013)
US2011184419A1	28 July 2011 (28-07-2011)
US8608749B2	17 December 2013 (17-12-2013)
US2011213376A1	01 September 2011 (01-09-2011)
US8632547B2	21 January 2014 (21-01-2014)
US2011086865A1	14 April 2011 (14-04-2011)
US8809346B2	19 August 2014 (19-08-2014)
US2013184764A1	18 July 2013 (18-07-2013)
US8828087B2	09 September 2014 (09-09-2014)
US2009254093A1	08 October 2009 (08-10-2009)
US8858561B2	14 October 2014 (14-10-2014)
US2011166578A1	07 July 2011 (07-07-2011)
US8864769B2	21 October 2014 (21-10-2014)
US2012109138A1	03 May 2012 (03-05-2012)
US8900244B2	02 December 2014 (02-12-2014)
US2013282132A1	24 October 2013 (24-10-2013)
US8979936B2	17 March 2015 (17-03-2015)
US2013131681A1	23 May 2013 (23-05-2013)
US9005297B2	14 April 2015 (14-04-2015)
US2011015639A1	20 January 2011 (20-01-2011)
US9113971B2	25 August 2015 (25-08-2015)
US2010087829A1	08 April 2010 (08-04-2010)
US9173661B2	03 November 2015 (03-11-2015)
US2013116699A1	09 May 2013 (09-05-2013)
US9241745B2	26 January 2016 (26-01-2016)
WO2007145937A2	21 December 2007 (21-12-2007)
WO2007145937A3	14 February 2008 (14-02-2008)
WO2009129063A1	22 October 2009 (22-10-2009)
WO2009129067A1	22 October 2009 (22-10-2009)
WO2009144584A1	03 December 2009 (03-12-2009)
WO2010033431A1	25 March 2010 (25-03-2010)
WO2010048257A1	29 April 2010 (29-04-2010)
WO2010093902A1	19 August 2010 (19-08-2010)
WO2010096557A2	26 August 2010 (26-08-2010)
WO2010096557A3	14 October 2010 (14-10-2010)
WO2010111272A1	30 September 2010 (30-09-2010)
WO2010144705A1	16 December 2010 (16-12-2010)
WO2010148103A1	23 December 2010 (23-12-2010)
WO2011041398A1	07 April 2011 (07-04-2011)
WO2011106711A1	01 September 2011 (01-09-2011)
WO2011109260A1	09 September 2011 (09-09-2011)
WO2012061042A1	10 May 2012 (10-05-2012)
WO2012116206A1	30 August 2012 (30-08-2012)
WO2012158917A1	22 November 2012 (22-11-2012)
WO2013126416A1	29 August 2013 (29-08-2013)
WO2016007631A1	14 January 2016 (14-01-2016)

US2014364858A1	11 December 2014 (11-12-2014)	US2014364858A1	11 December 2014 (11-12-2014)
		CA2908748A1	18 December 2014 (18-12-2014)
		CN105246433A	13 January 2016 (13-01-2016)
		WO2014197988A1	18 December 2014 (18-12-2014)