



US0D1027167S

(12) **United States Design Patent**
Healy et al.

(10) **Patent No.:** **US D1,027,167 S**

(45) **Date of Patent:** **** May 14, 2024**

(54) **URINARY CATHETER**

D421,303 S 2/2000 Cote et al.

D515,206 S 2/2006 Tarumi

D515,209 S 2/2006 Tarumi

(Continued)

(71) Applicant: **Hollister Incorporated**, Libertyville, IL
(US)

(72) Inventors: **Paul Healy**, Claremorris (IE);
Satwinder S. Panesar, Foxford (IE);
Heather O'Connor, Ballina (IE);
Michael G. Murray, Ballina (IE)

FOREIGN PATENT DOCUMENTS

CN 3125873 * 10/1999

CN 107441570 A 12/2017

(Continued)

(73) Assignee: **Hollister Incorporated**, Libertyville, IL
(US)

OTHER PUBLICATIONS

Liposuction and Lipo-modelling Cannula, eurosurgical.co.uk, [Post date: unknown], [Site seen Aug. 31, 2023], Seen at URL: <https://www.eurosurgical.co.uk/plastic-surgery/liposuction-products/liposuction-equipment/cannula-accessories/> (Year: 2023).*

(Continued)

(**) Term: **15 Years**

Primary Examiner — Natasha Vujcic

Assistant Examiner — Gilbert B Ford

(74) *Attorney, Agent, or Firm* — Cook Alex Ltd.

(21) Appl. No.: **29/865,960**

(57)

CLAIM

The ornamental design for a urinary catheter, as shown and described.

(22) Filed: **Aug. 22, 2022**

Related U.S. Application Data

DESCRIPTION

(62) Division of application No. 29/779,193, filed on Apr. 16, 2021, now Pat. No. Des. 967,406.

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/112**

(58) **Field of Classification Search**

USPC D24/112–114, 133, 186, 130, 127, 108

CPC .. A61M 25/065; A61M 5/42; A61M 25/0612;

A61M 25/00; A61M 39/00; A61M 27/00;

A61M 25/0043; A61M 25/0067

See application file for complete search history.

FIG. 1 is a front perspective view of a urinary catheter.

FIG. 2 is a front elevational view thereof.

FIG. 3 is a rear elevational view thereof.

FIG. 4 is a right-side elevational view thereof.

FIG. 5 is a left-side elevational view thereof.

FIG. 6 is a top plan view thereof.

FIG. 7 is a bottom plan view of the thereof; and,

FIG. 8 is a rear perspective view of thereof.

The break lines in FIGS. 1 and 4-8 indicate that the appearance of any portion of the urinary catheter between the break lines forms no part of the claimed design.


The broken lines in FIG. 3 depict portions of the urinary catheter that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,459,188 A	8/1969	Roberts
4,698,058 A	10/1987	Greenfeld et al.
5,163,924 A	11/1992	Beverly
5,853,518 A	12/1998	Utas
5,924,206 A	7/1999	Cote et al.
5,980,483 A	11/1999	Dimitri

1 Claim, 4 Drawing Sheets

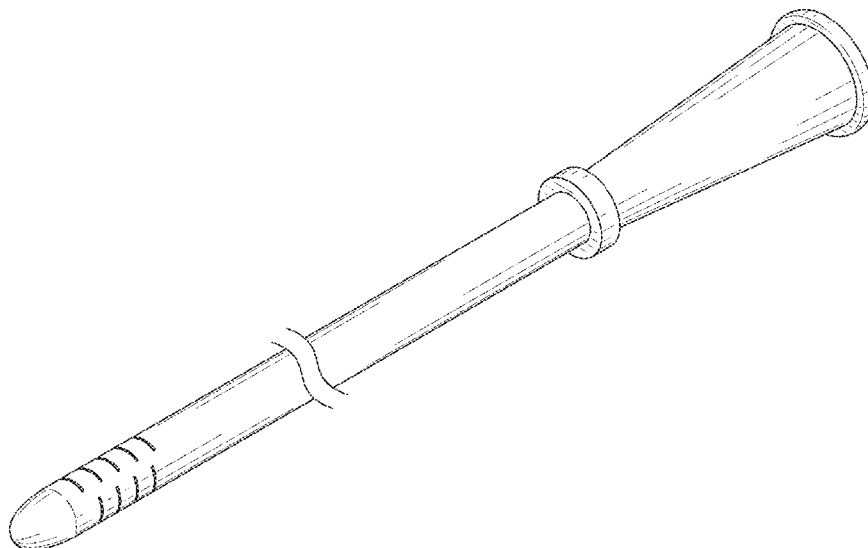

(56)

References Cited

U.S. PATENT DOCUMENTS

D516,716 S 3/2006 Weber et al.
 D603,043 S * 10/2009 Kreidler D24/130
 7,789,873 B2 9/2010 Kubalak et al.
 D658,758 S * 5/2012 Orbay D24/130
 D705,925 S 5/2014 Murray et al.
 D816,217 S * 4/2018 Naughton D24/130
 10,149,961 B2 12/2018 Carleo
 D846,116 S * 4/2019 Naughton D24/130
 D846,736 S 4/2019 Naughton et al.
 10,398,813 B2 * 9/2019 Sforza A61M 1/89
 D864,381 S 10/2019 Miles
 10,549,068 B2 2/2020 Shevgoor et al.
 D902,387 S 11/2020 Oellgaard et al.
 D910,836 S 2/2021 Sandberg et al.
 D918,382 S 5/2021 Naughton et al.
 D956,222 S 6/2022 Vaughton et al.
 11,376,395 B2 7/2022 Montes de Oca et al.
 D967,403 S * 10/2022 Healy D24/112
 D967,404 S * 10/2022 Healy D24/112
 D967,405 S * 10/2022 Healy D24/112
 D967,406 S * 10/2022 Healy D24/112
 D967,407 S * 10/2022 Healy D24/112
 2008/0262369 A1 10/2008 Colman et al.
 2012/0239004 A1 9/2012 Wong
 2015/0352321 A1 12/2015 Hannon et al.
 2017/0007800 A1 1/2017 Chao et al.
 2017/0296221 A1 10/2017 Di Caprio et al.
 2018/0001055 A1 1/2018 Utas et al.
 2019/0262579 A1 8/2019 Lovmar
 2020/0061335 A1 2/2020 Guldager et al.
 2020/0391005 A1 12/2020 Murray et al.
 2021/0370018 A1 12/2021 Murray et al.

2022/0339326 A1 * 10/2022 Farrell A61L 29/16
 2023/0166073 A1 * 6/2023 Radmer A61M 27/00
 604/544
 2023/0191078 A1 * 6/2023 O'Donnell A61M 27/00
 604/544

FOREIGN PATENT DOCUMENTS

CN 107670160 A 2/2018
 FR 2240026 A1 3/1975
 GB 6168877 * 10/2021
 GB 6168879 * 10/2021
 GB 6168881 * 10/2021
 GB 6168883 * 10/2021
 WO 2020103996 A1 5/2020
 WO 2020160738 A1 8/2020

OTHER PUBLICATIONS

Inyna Chic Intermittent, Hollister, A'Design Award Competition, [Post date: Jan. 29, 2022], [Site seen: Aug. 31, 2023], Seen at URL: <https://competition.adesignaward.com/gooddesign.php?ID=83253> (Year: 2023).*

Infyna Chic™ Intermittent Catheter, Hollister, Hollister.com, [Post date: Apr. 12, 2021], [Site seen Jul. 7, 2022], Seen at URL: <https://www.hollister.com/en/products/continence-care-products/intermittent-catheters/hydrophilic-pre-lubricated/infyna-chic-ready-to-use-hydrophilic-intermittent-catheter> (Year: 2021).

Cure Twist Female 6 Inches Intermittent Catheter—12 Fr, Riteway Medical, [Post date unknown], [Site seen Jul. 7, 2022], Seen at URL: <https://ritewaymed.com/product/cure-twist-female-6-inches-intermittent-catheter-12-fr/> (Year: 2022).

Kennelly et al., "Adult Neurogenic Lower Urinary Tract Dysfunction and Intermittent Catheterisation in a Community Setting: Risk Factors Model for Urinary Tract Infections," Apr. 2, 2019, *Advances in Urology*, vol. 2019.

* cited by examiner

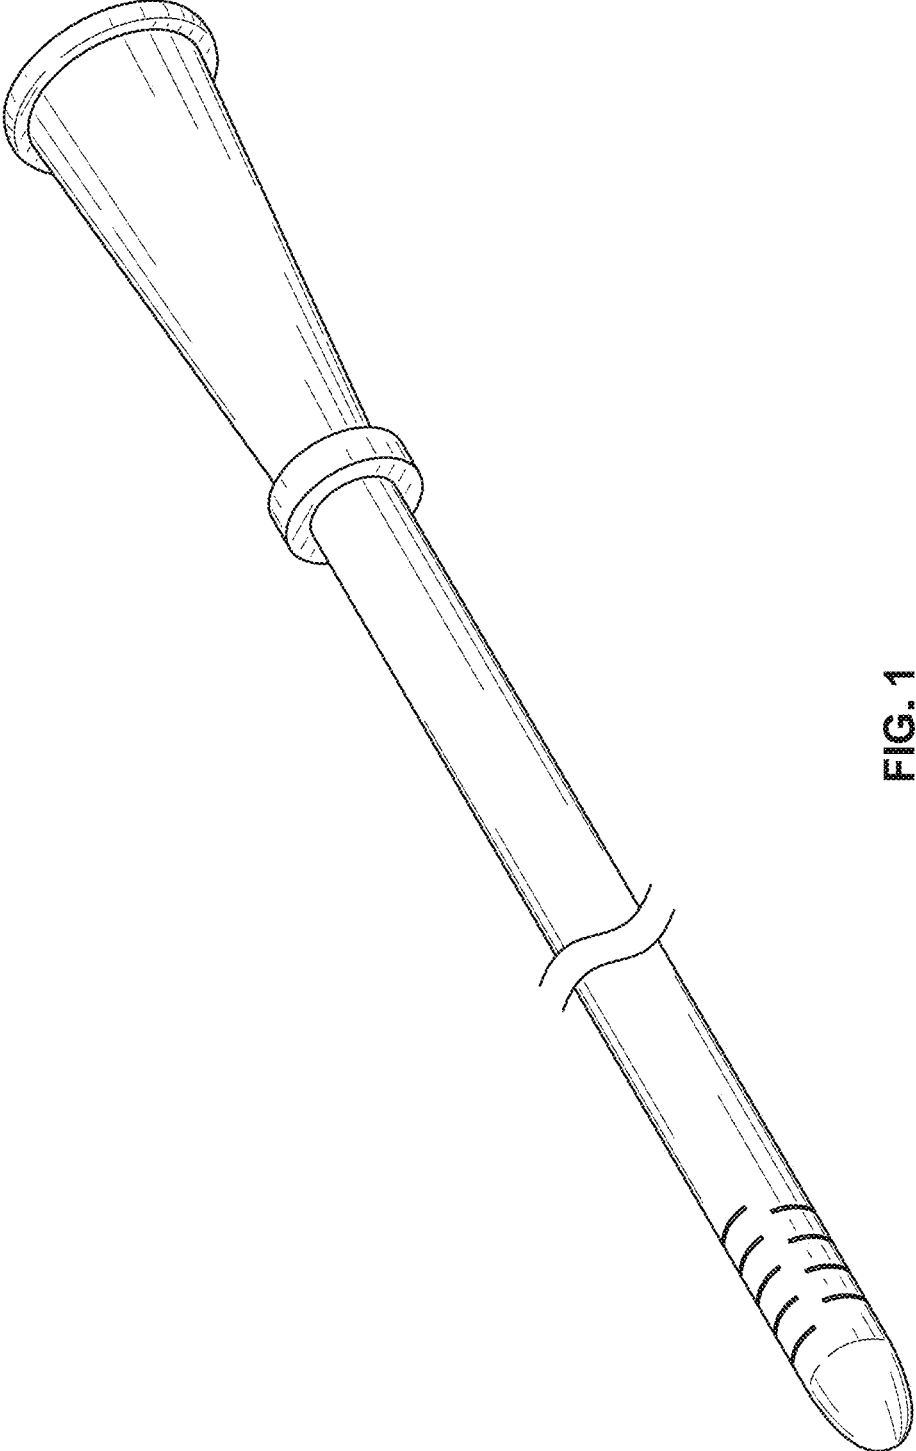


FIG. 1




FIG. 2




FIG. 3

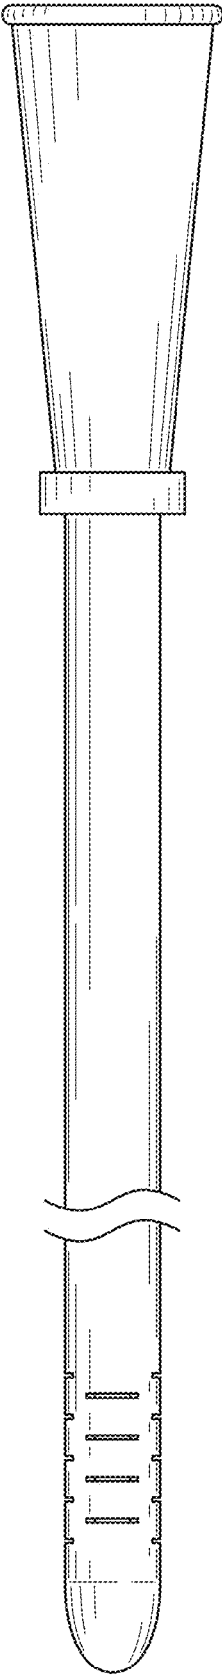


FIG. 4

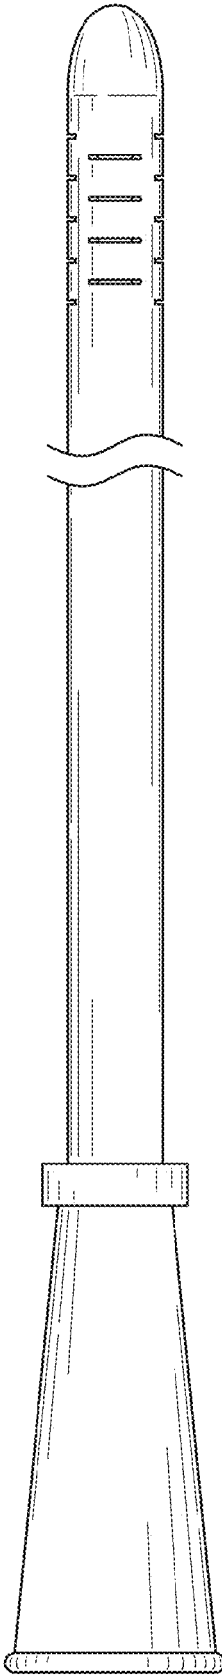


FIG. 5

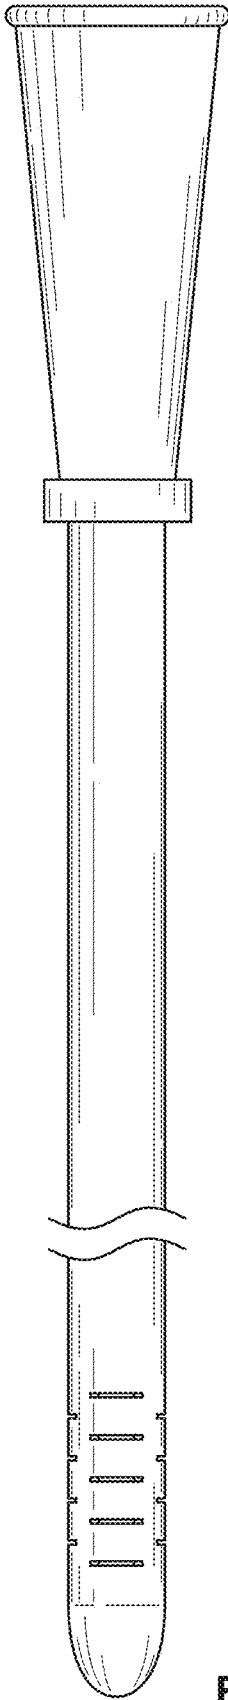


FIG. 6

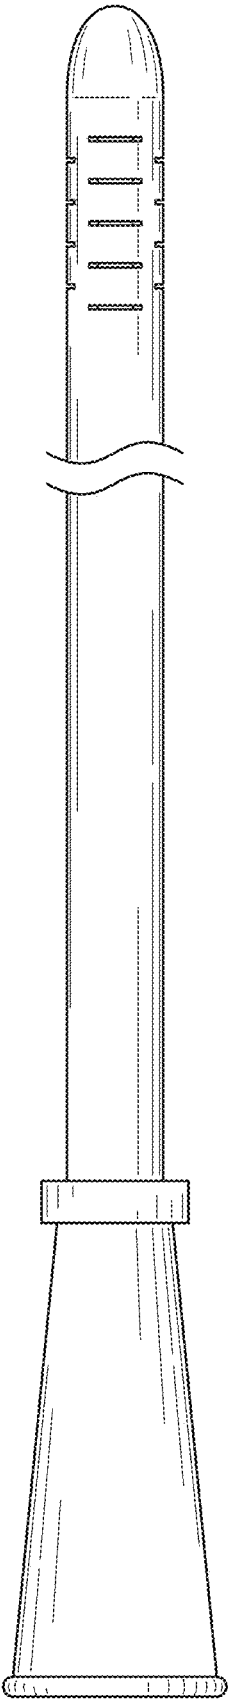


FIG. 7

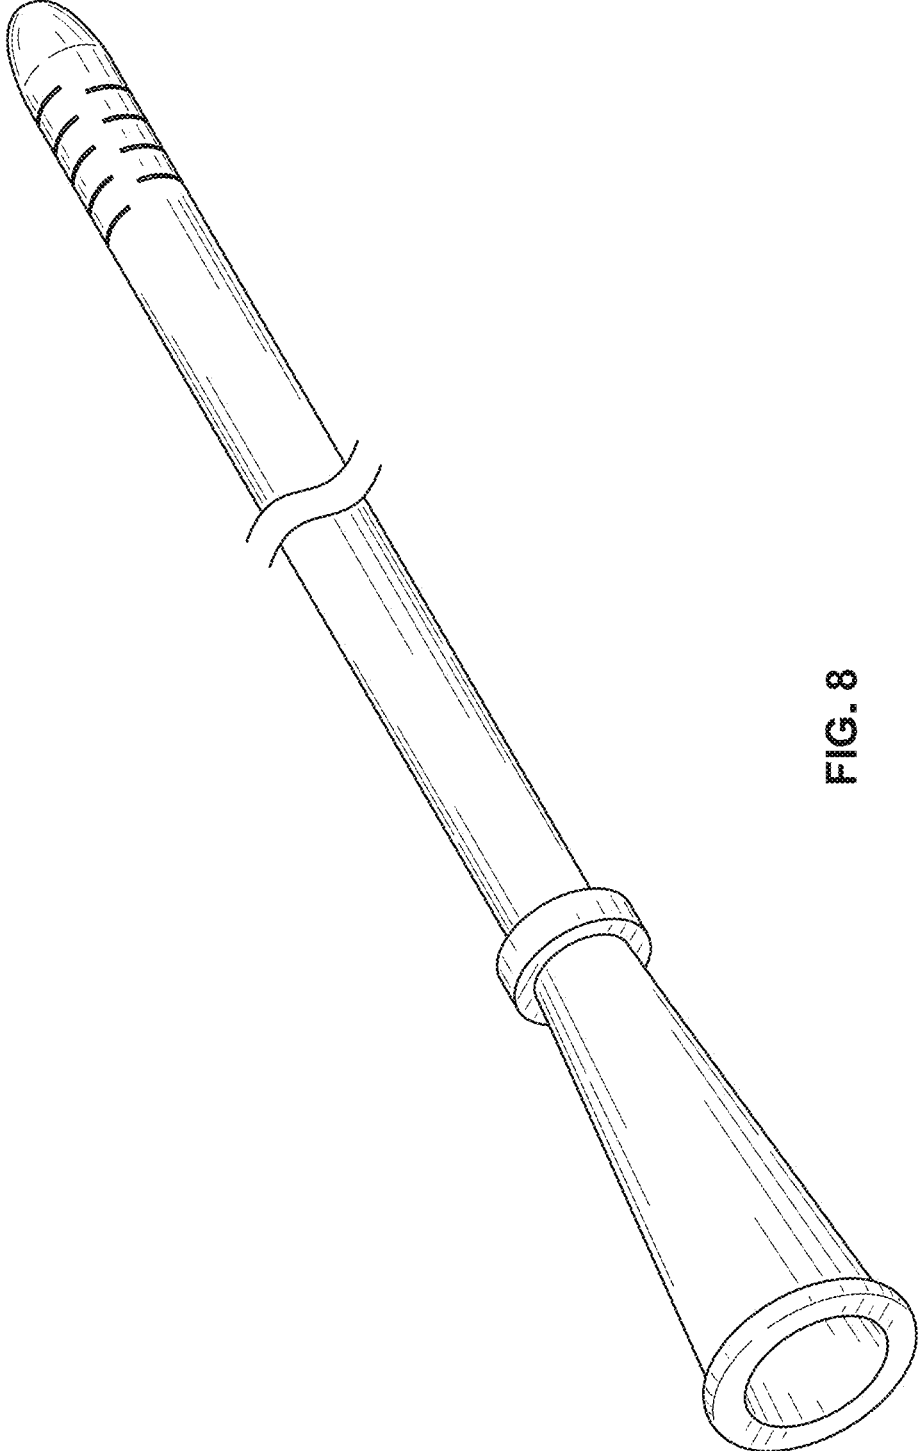


FIG. 8