



(43) International Publication Date
24 January 2019 (24.01.2019)

(51) International Patent Classification:

G16H 20/40 (2018.01) A61M 16/00 (2006.01)
A61B 5/08 (2006.01)

(21) International Application Number:

PCT/EP2018/068872

(22) International Filing Date:

12 July 2018 (12.07.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/533,691 18 July 2017 (18.07.2017) US

(71) Applicant: KONINKLIJKE PHILIPS N.V. [NL/NL];
High Tech Campus 5, 5656 AE Eindhoven (NL).

(72) Inventor: ISAZA, Fernando, Jose; High Tech Campus 5,
5656 AE Eindhoven (NL).

(74) Agent: DE HAAN, Poul, Erik; Philips International B.V.
– Intellectual Property & Standards, High Tech Campus 5,
5656 AE Eindhoven (NL).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) Title: VENTILATOR GAS DELIVERY INITIATION VIA A VIRTUAL PRESSURE TRIGGERING MECHANISM

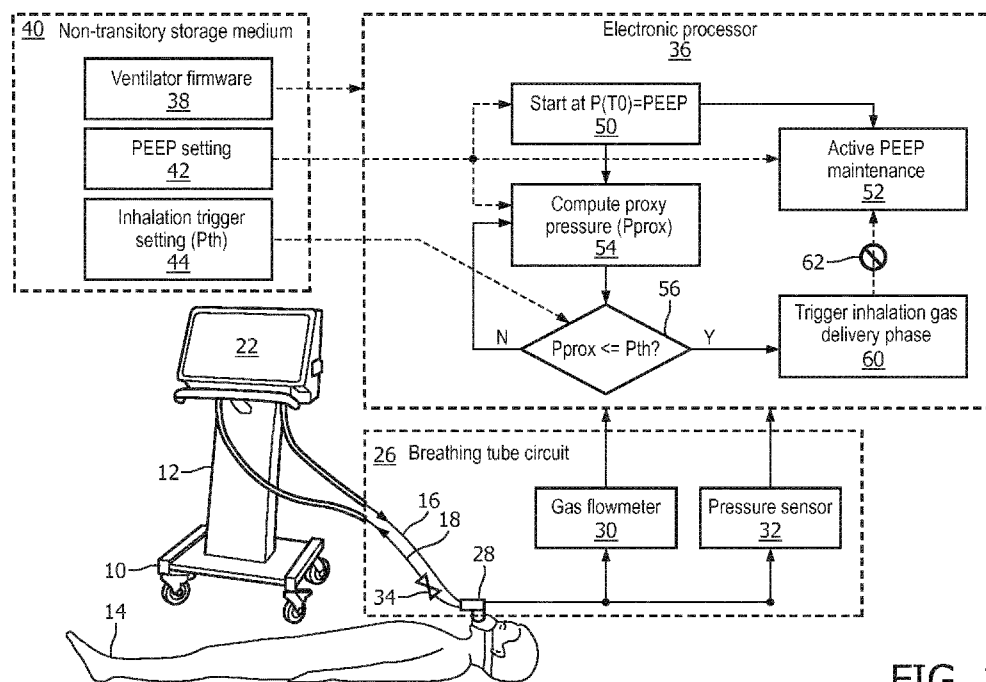


FIG. 1

(57) Abstract: A respiratory monitoring system includes (10) a mechanical ventilator (12) configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level during an exhalation phase. A breathing tubing circuit (26) includes: a patient port (28), a gas inlet line (16) connected to supply gas from the mechanical ventilator to the patient port, a gas flow meter (30) connected to measure gas flow into lungs of the patient, and a pressure sensor (32) connected to measure gas pressure at the patient port. At least one processor (38) is programmed to: compute a proxy pressure comprising an integral of gas flow into the lungs measured by the gas flow meter; and trigger the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.



(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*

Published:

— *with international search report (Art. 21(3))*

VENTILATOR GAS DELIVERY INITIATION VIA A VIRTUAL PRESSURE TRIGGERING MECHANISM

FIELD

The following relates to the medical therapy arts, respiratory therapy arts, medical ventilation arts, and related arts.

BACKGROUND

Detection of a patient's desire to initiate gas delivery during ventilation of the patient has been done in the industry using two primary methodologies. These are referred to as pressure triggering and flow triggering based on pressure and flow signals, respectively. When using the pressure triggering mechanism, initiation of the inhalation gas delivery phase occurs when the pressure at the patient port of the breathing tubing circuit, is reduced by the patient's effort below a pressure threshold previously set by the therapist.

During the use of the pressure triggering method, modern ventilators suspend gas delivery supply to the patient-tubing system throughout the duration of the exhalation phase of the breath cycle. Thus, when the patient initiates an effort to breathe, gas is made to flow between the tubing circuit and the patient lungs since the patient effort lowers the pressure in his/her lungs below the pressure level present in the tubing circuit. As gas migrates to the lung and the tubing circuit gets depleted, the pressure in the tubing circuit descends. When that pressure becomes less than a pre-determined threshold, selected by the care giver, the ventilator initiates the inhalation gas delivery phase in accordance with gas delivery targets appropriate for the ventilation modality (also pre-selected by the care giver).

Modern ventilators typically provide a pressure sensitivity setting (with a typical range: 0.5 to 20 cmH₂O with a resolution of 0.5 cmH₂O) which allows the practitioner to set the appropriate pressure threshold level for triggering the inhalation gas delivery phase.

A complication arises if the mechanical ventilation is configured to maintain a positive pressure at the end of expiration. In one approach for this instance, the ventilator's mechanism for triggering/initiation of the inhalation gas delivery phase of a breath uses the threshold selected and the Positive End Expiratory Pressure (PEEP) level setting (the reference point). If a difference between pre-set threshold and the PEEP level setting is less than or equal

to the pressure measured at the tubing circuit's patient port, then gas delivery is initiated. Otherwise, the pressure at the patient port continues to be monitored.

The following provides new and improved apparatuses and methods which overcome the foregoing problems and others.

BRIEF SUMMARY

In accordance with one aspect, a respiratory monitoring system includes a mechanical ventilator configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level during an exhalation phase. A breathing tubing circuit includes: a patient port, a gas inlet line connected to supply gas from the mechanical ventilator to the patient port, a gas flow meter connected to measure gas flow into lungs of the patient, and a pressure sensor connected to measure gas pressure at the patient port. At least one processor is programmed to: compute a proxy pressure comprising an integral of gas flow into the lungs measured by the gas flow meter; and trigger the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.

In accordance with another aspect, a non-transitory computer readable medium stores instructions executable by at least one electronic processor to perform a respiratory monitoring method. The method includes: computing a proxy pressure comprising an integral of gas flow into the lungs measured by an gas flow meter of a breathing tubing circuit operably connected to a mechanical ventilator configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level; and triggering the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.

In accordance with another aspect, a respiratory monitoring system includes a mechanical ventilator configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level. A breathing tubing circuit includes: a patient port, a gas inlet line connected to supply gas from the mechanical ventilator to the patient port, and a gas flow meter connected to measure gas flow into lungs of the patient, a pressure sensor connected to measure gas pressure at the patient port. At least one processor is programmed to: compute a proxy pressure comprising an integral of gas

flow into the lungs or gas flow supplied by the mechanical ventilator, the proxy pressure computed by the equation: $P_{prox}(t) = PEEP - \int_{T_0}^{t_f} \frac{Q_{lung}(t)}{C_{tube}} dt$ where $P_{prox}(t)$ is the proxy pressure; PEEP is the extrinsic PEEP level; T_0 is a time at which the pressure measured by the pressure sensor at the patient port reaches PEEP; T_f is a time at which an inhalation phase starts, $Q_{lung}(t)$ is the measured gas flow into the lungs or an estimated gas flow supplied by the mechanical ventilator and C_{tube} is a tubing circuit compliance of the breathing tubing circuit; and trigger the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.

One advantage resides in improved monitoring of a pressure level in a patient during ventilation.

Another advantage resides in facilitating the use of pressure triggering of the inhalation gas delivery phase in the case of ventilation employing an active controller for the Positive End Expiratory Pressure (PEEP) maintained, during exhalation, via flow delivered to the patient tubing system by the mechanical ventilator to avoid auto-triggering of the ventilator in the presence of leakages of the disclosed patient tubing system, since the triggering process of the disclosed patient tubing system is not as sensitive to leaks as other triggering methods.

Another advantage resides in providing such pressure triggering in the case of ventilation employing a PEEP setting maintained by delivered gas flow, in which the pressure threshold for triggering the inhalation gas delivery phase is sensibly related to (and in some embodiments equal to) the threshold that would be used if PEEP were maintained passively by modulating or closing off the exhalation valve.

Further advantages of the present disclosure will be appreciated to those of ordinary skill in the art upon reading and understand the following detailed description. It will be appreciated that any given embodiment may achieve none, one, more, or all of the foregoing advantages and/or may achieve other advantages.

BRIEF DESCRIPTION OF THE DRAWINGS

The disclosure may take form in various components and arrangements of components, and in various steps and arrangements of steps. The drawings are only for purposes of illustrating the preferred embodiments and are not to be construed as limiting the disclosure.

FIGURE 1 shows a schematic of a proposed ventilator apparatus in accordance with one aspect of the present disclosure.

FIGURE 2 shows a flow chart of an exemplary method of use for the ventilator apparatus of FIGURE 1.

FIGURE 3 shows a schematic of a proposed ventilator apparatus in accordance with another aspect of the present disclosure.

DETAILED DESCRIPTION

The following relates to an improvement in the triggering of the inhalation gas delivery phase in the context of mechanical ventilation. Traditionally, there are two approaches for this triggering. In pressure-based triggering, onset of spontaneous inspiration is detected as a decrease in pressure at the patient port of the breathing tubing circuit to a value below a triggering threshold. In flow-based triggering, onset of spontaneous inspiration is detected as an increase in positive gas flow into a disclosed patient-tubing system above a triggering threshold.

A difficulty arises if the ventilation system is designed to provide a controlled extrinsic positive end-expiratory pressure (PEEP). This is done for some patients in order to avoid alveolar collapse due to a low pressure level in the lungs. There are two approaches for this. In a valve-based approach, the exhalation valve is closed when PEEP is reached, so that the volume of gas in the breathing circuit is held constant. Here there is no particular difficulty in pressure-based triggering because the pressure will decrease as inhalation begins.

However, in some ventilation systems, such as blower based systems, the maintenance of PEEP can be done actively, by keeping the exhalation valve at least partially open and delivering gas flow via the blower to maintain the target PEEP value. Here, the pressure-based triggering is ineffective since the inhalation effort is simply offset by increased blower flow. Thus, in this operational mode the usual approach is to employ flow-based triggering.

While flow-based triggering is generally effective, it is recognized herein that one difficulty that can arise is flow noise induced triggering. With a blower based ventilator, noise in the breathing circuit generally manifests as flow fluctuations, and if these are too large they can induce spurious triggering of the inhalation gas delivery phase leading to loss of synchronicity with the patient's spontaneous inspiration effort.

A solution to the above-described problem is the triggering of inhalation flow based on a calculated “virtual” or “proxy” pressure decrease. In one embodiment, the virtual or proxy pressure calculation is given by

$$P_{\text{prox}} = \text{PEEP} - \int_{t=T_0}^{t=T_1} Q_{\text{Lung}} dt / C_{\text{tube}}$$

where PEEP is the extrinsic PEEP which is a ventilation parameter, T_0 is the time at which the pressure measured by the pressure sensor at the patient port reaches PEEP (so that $P_{\text{prox}}(t = T_0) = \text{PEEP}$), and $Q_{\text{lung}}(t)$ is the gas flow into the lungs measured by a flow sensor ($Q_{\text{lung}}(t)$ is positive when the gas flow is directed into the lungs). The term C_{tube} is the tubing circuit compliance which may be provided by the ventilator circuit manufacturer or can be measured empirically using the relationship $C = \Delta V / \Delta P$ where ΔP is a pressure change measured for a volume of gas ΔV delivered to the -tubing system.

The inhalation gas delivery phase is then triggered when the proxy pressure $P_{\text{prox}}(t)$ decreases to below a threshold pressure, i.e. when $P_{\text{prox}}(t = T_1) = P_{\text{th}}$ (where P_{th} is some value below PEEP). Advantageously, the proxy pressure mimics the pressure that would actually be measured if the exhalation valve were to be completely closed in order to passively establish PEEP. That is, the proxy pressure is an estimation of the pressure drop that would have been caused by the patient's effort to breathe if PEEP control had operated by completely closing off the exhalation valve. Thus, for example, P_{th} can be set to the "standard" value used -for that type of triggering mechanism when active PEEP control methodology is used.

With reference to FIGURE 1, an embodiment of a respiratory therapy apparatus **10** is shown, which includes a mechanical ventilator **12** configured to deliver mechanical ventilation to a patient **14**. Thus, the respiratory monitoring system **10** may also be referred to as a mechanical ventilation system or apparatus.

The respiratory therapy apparatus **10** is used to provide mechanical ventilation to a patient via the mechanical ventilator **12** that delivers gas flow and/or pressure in accordance with ventilator settings to a ventilated patient **14** via an inlet gas line **16**. Exhaled gas returns to the ventilator **12** via an exhalation gas hose **18**. A patient port **28**, which in the illustrative embodiment is a Y-piece or alternatively may be a tracheal tube, or in some cases a full-face mask) couples gas from the discharge end of the inlet gas line **16** to the ventilated patient **14** during inhalation and

couples exhaled gas from the ventilated patient **14** into the exhalation gas line **18** during exhalation. Not shown in FIGURE 1 are numerous other ancillary components that may be provided depending upon the ventilation mode and other therapy being received by the ventilated patient **14**. Such ancillary components may include, by way of illustration: an oxygen bottle or other medical-grade oxygen source for delivering a controlled level of oxygen to the gas flow, usually controlled by a Fraction of Inspired Oxygen (FiO₂) ventilator setting; a humidifier plumbed into the inlet line **16**; a nasogastric tube to provide the patient **14** with nourishment; and so forth. The mechanical ventilator **12** has a user interface including, in the illustrative example, a touch-sensitive display **22** via which the physician, respiratory specialist, or other medical personnel can visualize the ventilator settings and monitor measured variables (e.g., gas way pressure and gas flow) and operating parameters of the mechanical ventilator **12**. Additionally or alternatively, the user interface may include physical user input controls (buttons, dials, switches, et cetera), a keyboard, a mouse, audible alarm device(s), indicator light(s), or so forth.

As shown in FIGURE 1, the mechanical ventilation apparatus **10** includes a breathing tubing circuit **26** which includes the inlet line **16** and the outlet line **18**, along with the patient port **28**, a gas flow meter **30**, a pressure sensor **32**, and an exhalation valve **34**. The gas flow meter **30** and the pressure sensor **32** can each be hardware sensors known in the art. The gas inlet line **16** is connected to supply gas from the mechanical ventilator **12** to the patient port **28**. The patient port **28** can be secured or otherwise attached to the Y piece. The gas flow meter **30** is shown diagrammatically, and is connected to measure gas flow into lungs of the patient, e.g. by measuring gas or gas flow into the inlet of the patient port **28** or gas flow or gas flow in the inlet line **16**. The pressure sensor **32** is likewise diagrammatically shown, and is connected to measure gas pressure at the patient port **28**. The illustrative exhalation valve **34** is shown mounted on the outlet line **18**, but may alternatively be integrated into the patient port **28** or internal to the ventilator **12**. The exhalation valve is configured to regulate expiration of gas or gas from the lungs of the patient via the gas outlet line **18**, e.g. if the exhalation valve **34** is completely closed then no exhalation gas can flow from the patient port **28** through the outlet line **18**; while, a partially closed setting of the exhalation valve **34** can introduce a controlled resistance to the exhalation gas or gas flow.

The mechanical ventilator **12** also includes an electronic processor **36** for controlling the ventilation cycling by executing firmware **38** stored in a non-transitory storage

medium **40** such as a read only memory (ROM), electronically programmable ROM (EPROM), flash memory, solid state drive (SSD), or other electronic storage medium; or a magnetic disk or other magnetic storage medium. The non-transitory storage medium **40** further stores ventilator parameters or settings, such as the ventilation mode (e.g. pressure support ventilation or PSV as one non-limiting illustrative example), parameters of that ventilation mode (e.g. the support pressure setting in the illustrative PSV mode), or so forth. The electronic processor **36** can be, for example, a microprocessor, an application-specific integrated circuit (ASIC), or a suitable hardware controller known in the art.

In illustrative FIGURE 1, two salient settings are shown: an extrinsic positive end-expiratory pressure (PEEP) setting **42**, and a trigger pressure threshold (P_{th}) **44**, which controls (in conjunction with a proxy pressure as disclosed herein) the triggering of an inhalation gas delivery phase of a ventilation mode. The PEEP setting **42** and the trigger pressure threshold **44** may be input to the respiratory therapy system **10** via the user interface, or by additional automatic controls which determine appropriate values based on known patient characteristics. It should be noted that while FIGURE 1 diagrammatically depicts a single non-transitory storage medium **40**, more generally there may be more than one such medium. For example, in some embodiments the firmware **38** is stored on a different non-transitory storage medium than the ventilator settings **42**, **44**. Furthermore, the electronic processor **36** is operatively connected to receive measurements (e.g. samples) from the sensors **30**, **32** as well as from other components of the mechanical ventilator **12** or that are operatively communicating with the ventilator **12**, e.g. a supplementary oxygen supply, physiological sensors (e.g. heart rate monitor, pulse oximeter), and/or so forth. Typically, the electronic processor **36** and non-transitory storage medium **40** are on-board components of the mechanical ventilator **12** so as to facilitate hard-wired connections providing high reliability; however, more distributed arrangements in which components are operatively connected by external wiring (e.g. USB cables) or wireless connections (e.g. Bluetooth™) are alternatively contemplated.

With continuing reference to FIGURE 1, in an illustrative ventilation process implemented by the ventilator **12**, it is assumed that the ventilator **12** is performing mechanical ventilation which includes an inhalation gas delivery phase during which positive pressure is applied by the ventilator **12** to the patient port **28** via the inlet hose **16**; an expiration phase during which the patient exhales; and during which the ventilator **12** actively maintains an extrinsic

positive end-expiratory pressure (PEEP) at the patient port **28**. Moreover, it is assumed, in the embodiments described herein, that the ventilator actively maintains the extrinsic PEEP by applying positive pressure to the patient port **28** to maintain the pressure at the programmed PEEP setting **42**.

Furthermore, the illustrative ventilation process employs pressure triggering using the trigger pressure threshold **44**. However, this process is complicated by the use of active extrinsic PEEP maintenance. To see why, the situation for passive PEEP maintenance is considered first.

If the ventilator maintained PEEP at the PEEP setting **42** passively, it would do so by modulating and eventually completely closing the exhalation valve **34** when the expiration phase caused the pressure to decrease to the PEEP setting **42**. With the exhalation valve **34** closed, the gas volume is fixed and hence the pressure measured by the pressure sensor **32** will be approximately constant. In this case of passive PEEP maintenance, pressure triggering of the next inhalation gas delivery phase (that is, the inhalation gas delivery phase of the next breathing cycle starting after closure of end-expiration) would be a straightforward matter of monitoring the pressure via the pressure sensor **32** and triggering the inhalation gas delivery phase when the measured pressure decreased below the trigger pressure threshold **44**. This pressure decrease will result naturally because as the patient engages in incipient inhalation, this expands the lungs thereby increasing the volume and consequently decreasing the pressure. The pressure threshold **44** is programmed by the respiratory clinician based on expert knowledge of the particular patient's spontaneous respiration capability together with the known PEEP setting **42**, e.g. a lower P_{th} setting is typically programmed for a patient with weaker respiratory capability, and P_{th} is always lower than the PEEP setting **42**. In general the P_{th} setting may also be tuned by trial and error as the respiratory clinician reviews the patient's breathing as measured by the flow and pressure sensors **30, 32**.

This approach is not applicable in the case of active extrinsic PEEP maintenance, because in this case as the patient begins to inhale to initiate the next spontaneous breath, the decrease in pressure that would be produced by the spontaneous inhalation is canceled by increased positive pressure applied by the mechanical ventilator **12** in order to control the pressure, using the reading of the pressure sensor **32**, at the programmed PEEP setting **42**. Conventionally, this has caused the respiratory clinician to elect to employ flow triggering, which will remain

operative with active extrinsic PEEP maintenance since the gas flow will indeed increase due to both the patient's spontaneous inhalation and the extra pressure applied by the ventilator **12**. However, if there is noise in the breathing circuit **26**, for example, caused by condensate water slushing around in the tubing system, this noise generally manifests as flow fluctuations. If these flow fluctuations are too large they can induce spurious flow-based triggering of the inhalation gas delivery phase leading to loss of synchronicity with the patient's spontaneous inspiration effort. The potential for noise is enhanced in the instant case because there are two sources of gas flow: the patient's spontaneous inhalation effort and the positive pressure applied by the ventilator **12** to maintain extrinsic PEEP.

With continuing reference to FIGURE 1, an improved approach for pressure triggering of the inhalation gas delivery phase is disclosed, which is operative in the case of active extrinsic PEEP regulation. The approach is suitably performed by the electronic processor **36** of the mechanical ventilator **12** executing instructions stored at the non-transitory/volatile storage medium **40** (e.g. the firmware **38**) and read and executed by the electronic processor **36**. In an operation **50**, the pressure read by the pressure sensor **32** is monitored during the exhalation phase to detect when the decreasing pressure falls to the level of the programmed PEEP setting **42**. This triggers the end of the exhalation phase. The time of the end of the exhalation phase, detected by the operation **50**, is denoted herein as T_0 . The exhalation phase includes executing an active PEEP maintenance process **52** that uses the pressure read by the pressure sensor **32**, to control the pressure in the respiratory therapy system **10** to match the PEEP setting **42** by operations that include at least operating the blower or other gas flow generating device to apply positive pressure to the patient port **28** via the inlet hose **16**. This PEEP maintenance process **52** is carried out throughout the exhalation phase. The pressure may cross the PEEP level and return to values above PEEP during the exhalation phase. The active PEEP maintenance process **52** may optionally include other control mechanisms, such as partially closing (or actively modulating) the exhalation valve **34** to increase (or modulate) flow resistance throughout the exhalation phase.

Concurrently with initiating the active PEEP maintenance **52**, a proxy pressure (P_{prox}) monitoring process **54** is initiated. In some embodiments, the proxy pressure is intended to estimate the pressure that would have been observed in the case of a triggering effort by the patient during passive extrinsic PEEP regulation/control. The proxy pressure monitoring process **54** will be described in greater detail with reference to FIGURE 2; however, the concept of the proxy

pressure can be understood as follows. In the case of passive extrinsic PEEP maintenance, the PEEP control is carried out via control of the pressure measured by the pressure sensor **32** at the patient port **28** using modulation of the ventilator's exhalation valve **34**. When in Pressure triggering mode, all gas supply to the patient tubing system is cut off during the exhalation phase and thus all the gas delivered to the patient's lungs, during a triggering effort, comes from the tubing system **26** itself. Therefore, for a system that uses active PEEP control to maintain the pressure level at the PEEP setting **42**, via dynamic control of the gas supplied by the ventilator **12** to the patient port **28** via the inlet hose **16**, it may be assumed that all the gas delivered to the patient lungs would have come from the tubing system (as in the case of the alternate passive PEEP control). Changes to the pressure in the tubing system **26** can be determined via the definition of the pneumatic compliance $C = \Delta V / \Delta P$ where ΔV is the volume change (integral of gas flow measured by the gas flow meter **30**) and ΔP is the pressure change measured by the pressure sensor **32**. Therefore, it is possible to estimate the "virtual" modification to the pressure level (ΔP) in the tubing system as a function of the amount of gas delivered to the lung (ΔV), in a ventilator that controls PEEP by dynamic supply of the gas delivered to the system, and effectively maintains the pressure in the Patient-tubing system at the pre-set PEEP level. To this end, the compliance definition can be rearranged as $\Delta P = \Delta V / C$. The volume change can be computed as $\Delta V(t) = \int_{T_0}^{t_f} Q_{lung}(\tau) d\tau$ where Q_{lung} is the gas flow delivered to the lungs by the ventilator **12** and τ represents time in the integral (to distinguish from time t_f which is the current time at which a new breath occurs and hence the end time of the integral). T_0 refers to a time at which the pressure at the patient port **28** crosses the PEEP level in a downward direction for the first time since the start of the exhalation phase. The compliance $C = C_{tube}$, that is, the compliance of the tubing circuit **26**. This yields $P_{prox}(t) = PEEP - \int_{T_0}^{t_f} \frac{Q_{lung}(\tau)}{C_{tube}} dt$.

With continuing reference to FIGURE 1, in a decision operation **56** it is determined whether the proxy pressure has decreased to the programmed threshold pressure setting **44**. If it has not yet decreased to this threshold, flow returns to block **54** to continue monitoring the proxy pressure. When the decision operation **56** detects that the pressure threshold **44** has been reached, this triggers the next inhalation gas delivery phase (operation **60**) for the next breath. This also entails triggering termination of the active PEEP regulation/control **52**, as indicated by the automatic termination denoted in FIGURE 1 by symbol **62**.

With reference to FIGURE 2, the respiratory monitoring method **100** is diagrammatically shown as a flowchart. At **102**, the electronic processor **38** is programmed to compute a proxy pressure comprising an integral of gas flow into the lungs measured by the gas flow meter **30**. In some embodiments, the proxy pressure comprises the integral computed starting at a time when the gas pressure at the patient port **28** measured by the pressure sensor **32** decreases below a threshold. For example, this threshold is the PEEP level.

In other embodiments, the proxy pressure comprises the integral of gas flow into the lungs measured by the gas flow meter **30** scaled by a tubing circuit compliance value of the breathing tubing circuit. For example, the proxy pressure is calculated according to the equation:

$$P_{prox}(t) = PEEP - \int_{T_0}^t \frac{Q_{lung}(\tau)}{C_{tube}} d\tau \quad \text{Equation 1}$$

where $P_{prox}(t)$ is the proxy pressure; PEEP is the extrinsic PEEP level; T_0 is a time at which the pressure measured by the pressure sensor **32** at the patient port reaches PEEP; $Q_{lung}(t)$ is the gas flow into the lungs measured by the gas flow meter **30**; and C_{tube} is a tubing circuit compliance of the breathing tubing circuit **26**. In other examples, the processor **38** is programmed to compute the integral of flow into the lungs measured by the gas flow meter using a rectangular or trapezoidal numerical integration.

In a further embodiment, as shown in FIGURE 3, the proxy pressure comprises the integral of flow supplied by the mechanical ventilator **12** to the inlet line **16** such that gas flow leakages are taken into account. In this embodiment, since the gas flow supplied by the mechanical ventilator **12** includes the leakage flow and the lung flow, the system **10** does not need the gas flow meter **30** to be positioned at the patient port **28**, but rather gas and oxygen flow sensors can be located in the proximity of the gas and oxygen (if available) sources **70** (i.e., a blower and an oxygen source) of the respiratory therapy system **10**. In this example, $Q_{lung}(t)$ is equal to the sum of the leakage gas flow and the lung gas flow.

In this embodiment, the gas flow meter **30** can comprise three different sensors: a gas flow sensor **72** configured to measure air gas flow (e.g., $FiO_2 = 21\%$); an O_2 flow sensor **74** configured to measure oxygen gas flow; and an exhalation gas flow sensor **76** configured to measure flow of gas exhaled by the patient (air mixed with the oxygen supplied by the ventilator **12**). The lung flow can be estimated using Equation 2:

$$Q_{\text{Lung}} = Q_{\text{air}} + Q_{\text{O}_2} - Q_{\text{exhalation}} - Q_{\text{leak}} - Q_{\text{tube}} \quad \text{Equation 2}$$

where: Q_{air} and Q_{O_2} are flows measured by the sensors **72** and **74**, which are located a gas outlet port **78** internal to the ventilator **12**. $Q_{\text{exhalation}}$ is a flow measured from the sensor **76** located on the inlet port, **80** internal to the ventilator **12** adjacent the exhalation valve **34**. Q_{leak} is a value estimated from Equation 3:

$$Q_{\text{leak}} = G_{\text{Leak}} * (P_p)^{0.5} \quad \text{Equation 3}$$

in which Q_{Leak} is an estimate of the gas exiting a leak orifice (i.e., at the patient port **28**); G_{Leak} is a conductance coefficient for the leak orifice; and P_p is a pressure measured by the pressure sensor **32**. Q_{tube} is a value estimated using Equation 4:

$$Q_{\text{tube}} = C_{\text{tube}} * d(P_p)/dt \quad \text{Equation 4}$$

in which Q_{tube} is an estimate of the gas used in pressurizing or depressurizing the system **10**; $d(P_p)/dt$ is a measure of an expansion or contraction of a tube (e.g., the inlet or outlet line **16** or **18**).

At **104**, once the proxy pressure is computed, the processor **38** is programmed to trigger an inhalation gas delivery phase of a ventilation mode when the proxy pressure decreases below a trigger pressure. For example, the mechanical ventilator **12** is configured to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level. To do so, the mechanical ventilator **12** is configured to set the exhalation valve **34** to at least partially open setting. Simultaneously, the mechanical ventilator **12** is configured to supply gas to the patient port **28** at a gas flow controlled to maintain the pressure at the patient port measured by the pressure sensor **32** at the PEEP level. A trigger pressure at which the ventilation mode occurs is lower than the PEEP level.

The disclosure has been described with reference to the preferred embodiments. Modifications and alterations may occur to others upon reading and understanding the preceding detailed description. It is intended that the disclosure be construed as including all such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

CLAIMS:

1. A respiratory monitoring system (10), comprising:
 - a mechanical ventilator (12) configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level during an exhalation phase;
 - a breathing tubing circuit (26) including:
 - a patient port (28),
 - a gas inlet line (16) connected to supply gas from the mechanical ventilator to the patient port,
 - a gas flow meter (30) connected to measure gas flow into lungs of the patient,
 - a pressure sensor (32) connected to measure gas pressure at the patient port, and
 - at least one processor (38) programmed to:
 - compute a proxy pressure comprising an integral of gas flow into the lungs measured by the gas flow meter; and
 - trigger the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.
2. The system (10) of claim 1, wherein the proxy pressure comprises the integral computed starting at a time when the gas pressure at the patient port (28) measured by the pressure sensor (32) decreases below a start threshold.
3. The system (10) of claim 2, wherein the start threshold is the PEEP level.
4. The system (10) of any one of claims 1-3, further including:
 - an exhalation valve (34) configured to regulate expiration of gas from the lungs of the patient;

wherein the mechanical ventilator (12) is configurable to perform the ventilation mode including providing the extrinsic PEEP at the PEEP level by setting or controlling the exhalation valve (34) to an at least partially open setting while simultaneously supplying gas to the patient port at an gas flow controlled to maintain the gas pressure at the patient port measured by the pressure sensor (32) at the PEEP level.

5. The system (10) of claim 4, wherein the trigger pressure is lower than the PEEP level.

6. The system (10) of any one of claims 1-5, wherein the proxy pressure comprises the integral of gas flow into the lungs measured by the gas flow meter (30) scaled by a tubing circuit compliance value of the breathing tubing circuit.

7. The system (10) of any one of claims 1-6, when the proxy pressure comprises:

$$P_{prox}(t) = PEEP - \int_{T_0}^{t_f} \frac{Q_{lung}(t)}{C_{tube}} dt$$

where $P_{prox}(t)$ is the proxy pressure; PEEP is the extrinsic PEEP level; T_0 is a time at which the pressure measured by the pressure sensor (32) at the patient port reaches PEEP; T_f is a time at which an inhalation phase starts, $Q_{lung}(t)$ is the gas flow into the lungs measured by the gas flow meter (30); and C_{tube} is a tubing circuit compliance of the breathing tubing circuit (26).

8. The system (10) of any one of claims 1-7, wherein the at least one processor (36) is programmed to:

compute the integral of gas flow into the lungs measured by the gas flow meter (30) using a rectangular or trapezoidal numerical integration.

9. A non-transitory computer readable medium storing instructions executable by at least one electronic processor (38) to perform a respiratory monitoring method (100), the method comprising:

computing a proxy pressure comprising an integral of gas flow into the lungs measured by a gas flow meter (30) of a breathing tubing circuit (26) operably connected to a

mechanical ventilator (12) configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level; and

triggering the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.

10. The non-transitory computer readable medium of claim 9, wherein the respiratory monitoring method (100) further includes:

with the at least one electronic processor (38), computing the proxy pressure comprising the integral starting at a time when the gas pressure at the patient port (28) measured by a pressure sensor (32) of the breathing tubing circuit (26) decreases below a threshold.

11. The non-transitory computer readable medium of claim 10, wherein the threshold is the PEEP level.

12. The non-transitory computer readable medium of any one of claims 9-11, wherein the respiratory monitoring method (100) further includes:

controlling the mechanical ventilator (12) to perform the ventilation mode including providing the extrinsic PEEP at the PEEP level by setting or controlling an exhalation valve (34) of the breathing tubing circuit (26) to an at least partially open setting while simultaneously supplying gas to the patient port at a gas flow controlled to maintain the gas pressure at the patient port measured by the pressure sensor (32) at the PEEP level.

13. The non-transitory computer readable medium of claim 12, wherein the trigger pressure is lower than the PEEP level.

14. The non-transitory computer readable medium of any one of claims 9-13, wherein the respiratory monitoring method (100) further includes:

with the at least one electronic processor (38), computing the proxy pressure as the integral of gas flow into the lungs measured by the gas flow meter (30) scaled by a tubing circuit compliance value of the breathing tubing circuit.

15. The non-transitory computer readable medium of any one of claims 9-14, wherein the respiratory monitoring method (100) further includes:

with the at least one electronic processor (38), computing the proxy pressure with an equation:

$$P_{prox}(t) = PEEP - \int_{T_0}^{t_f} \frac{Q_{lung}(t)}{C_{tube}} dt$$

where $P_{prox}(t)$ is the proxy pressure; PEEP is the extrinsic PEEP level; T_0 is a time at which the pressure measured by the pressure sensor (32) at the patient port reaches PEEP; T_f is a time at which an inhalation phase starts, $Q_{lung}(t)$ is the gas flow into the lungs measured by the gas flow meter (30); and C_{tube} is a tubing circuit compliance of the breathing tubing circuit (26).

16. The non-transitory computer readable medium of any one of claims 9-15, wherein the respiratory monitoring method (100) further includes:

with the at least one processor (36), computing the integral of gas flow into the lungs measured by the gas flow meter using a rectangular or trapezoidal numerical integration.

17. A respiratory monitoring system (10), comprising:

a mechanical ventilator (12) configurable to perform a ventilation mode that includes an inhalation gas delivery phase and provides extrinsic positive end-expiratory pressure (PEEP) at a PEEP level;

a breathing tubing circuit (26) including:

a patient port (28),

a gas inlet line (16) connected to supply gas from the mechanical ventilator to the patient port,

a gas flow meter (30) connected to measure gas flow into lungs of the patient, and

a pressure sensor (32) connected to measure gas pressure at the patient port, and

at least one processor (38) programmed to:

compute a proxy pressure comprising an integral of gas flow into the lungs or gas flow supplied by the mechanical ventilator, the proxy pressure computed by the equation:

$$P_{prox}(t) = PEEP - \int_{T_0}^{t_f} \frac{Q_{lung}(t)}{C_{tube}} dt$$

where $P_{prox}(t)$ is the proxy pressure; PEEP is the extrinsic PEEP level; T_0 is a time at which the pressure measured by the pressure sensor (32) at the patient port reaches PEEP; T_f is a time at which an inhalation phase starts, $Q_{lung}(t)$ is the measured gas flow into the lungs or an estimated gas flow supplied by the mechanical ventilator and C_{tube} is a tubing circuit compliance of the breathing tubing circuit (26); and

trigger the inhalation gas delivery phase of the ventilation mode when the proxy pressure decreases below a trigger pressure threshold.

18. The system (10) of claim 17, wherein the proxy pressure comprises the integral computed starting at a time when the gas pressure at the patient port (28) measured by the pressure sensor (32) decreases below the PEEP level.

19. The system (10) of either one of claims 17 and 18, further including:

an exhalation valve (34) configured to regulate expiration of gas from the lungs of the patient;

wherein the mechanical ventilator (12) is configurable to perform the ventilation mode including providing the extrinsic PEEP at the PEEP level by setting the exhalation valve (34) to an at least partially open setting while simultaneously supplying gas to the patient port (28) at a gas flow controlled to maintain the gas pressure at the patient port measured by the pressure sensor (32) at the PEEP level in which the trigger pressure is lower than the PEEP level.

20. The system (10) of any one of claims 17-19, wherein the at least one processor (36) is programmed to:

compute the integral of gas flow into the lungs measured by the gas flow meter **(30)** using a rectangular or trapezoidal numerical integration.

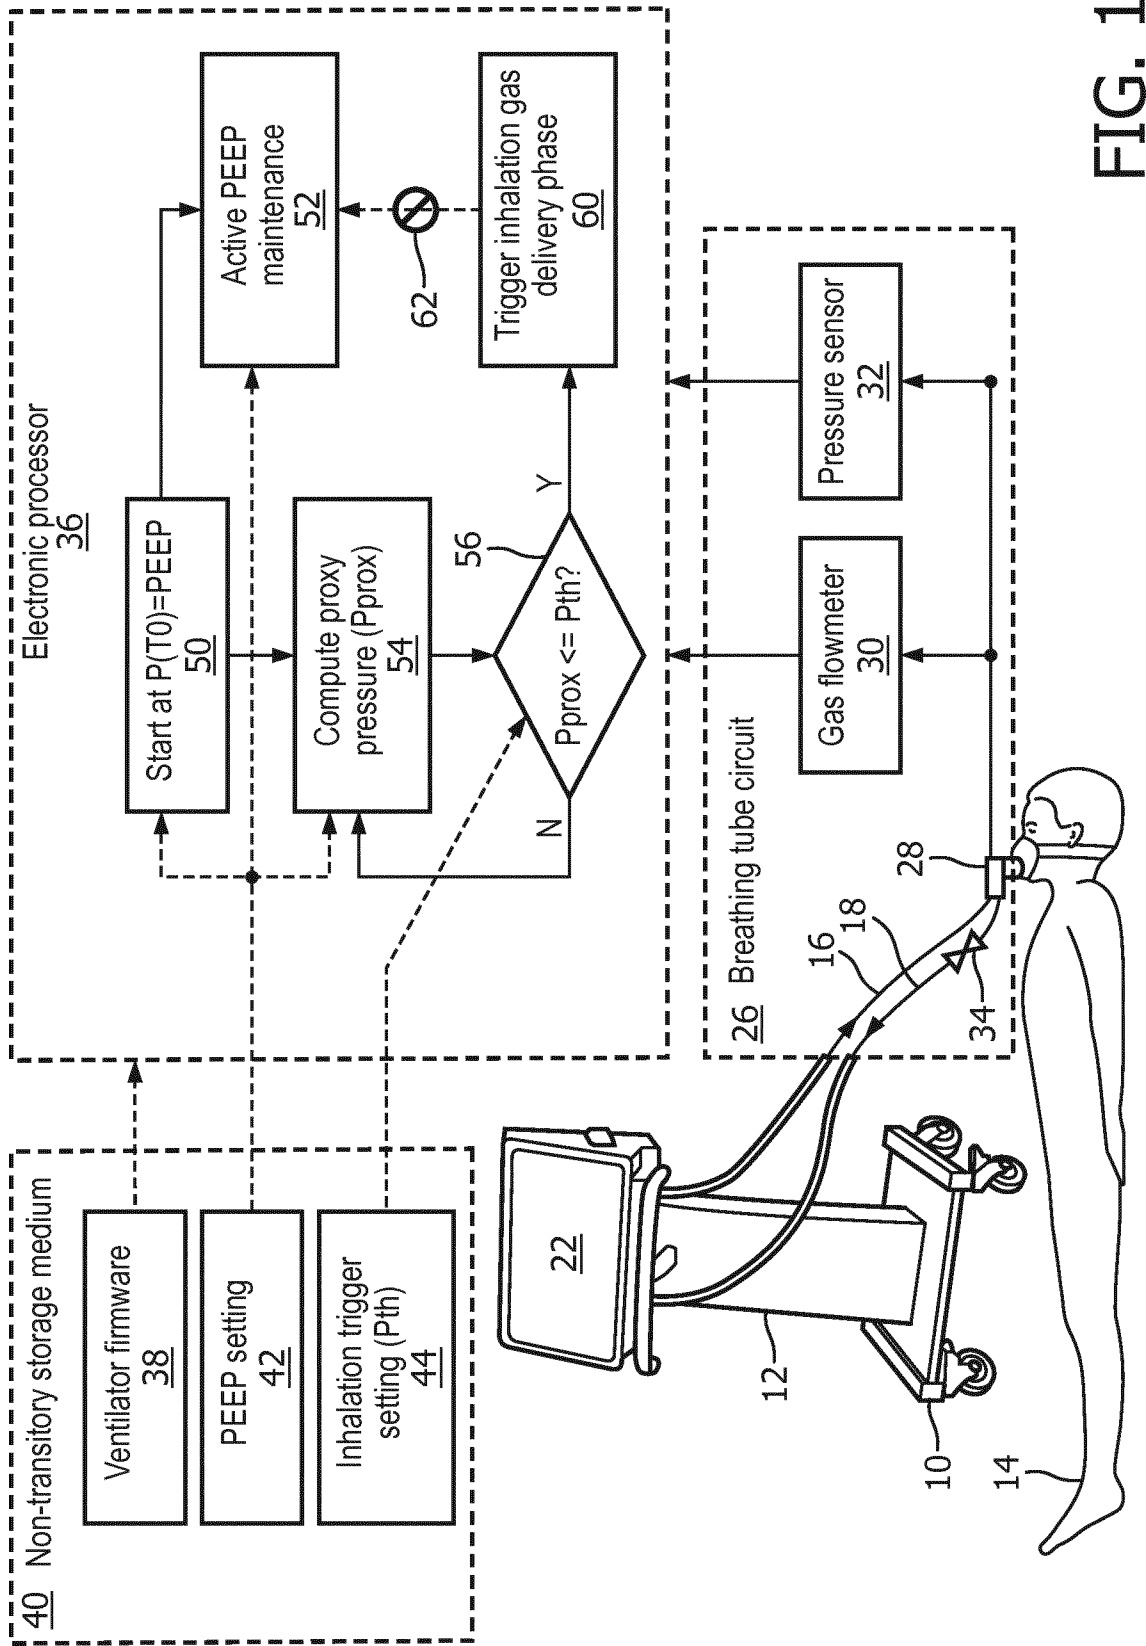


FIG. 1

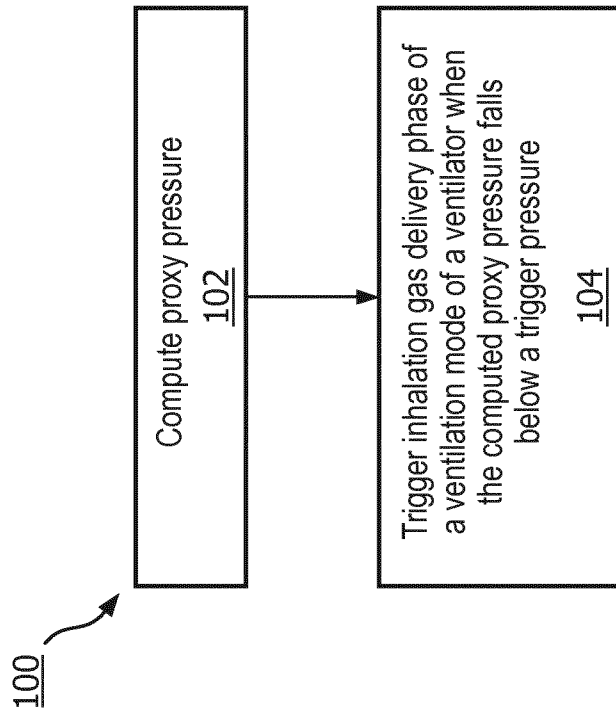


FIG. 2

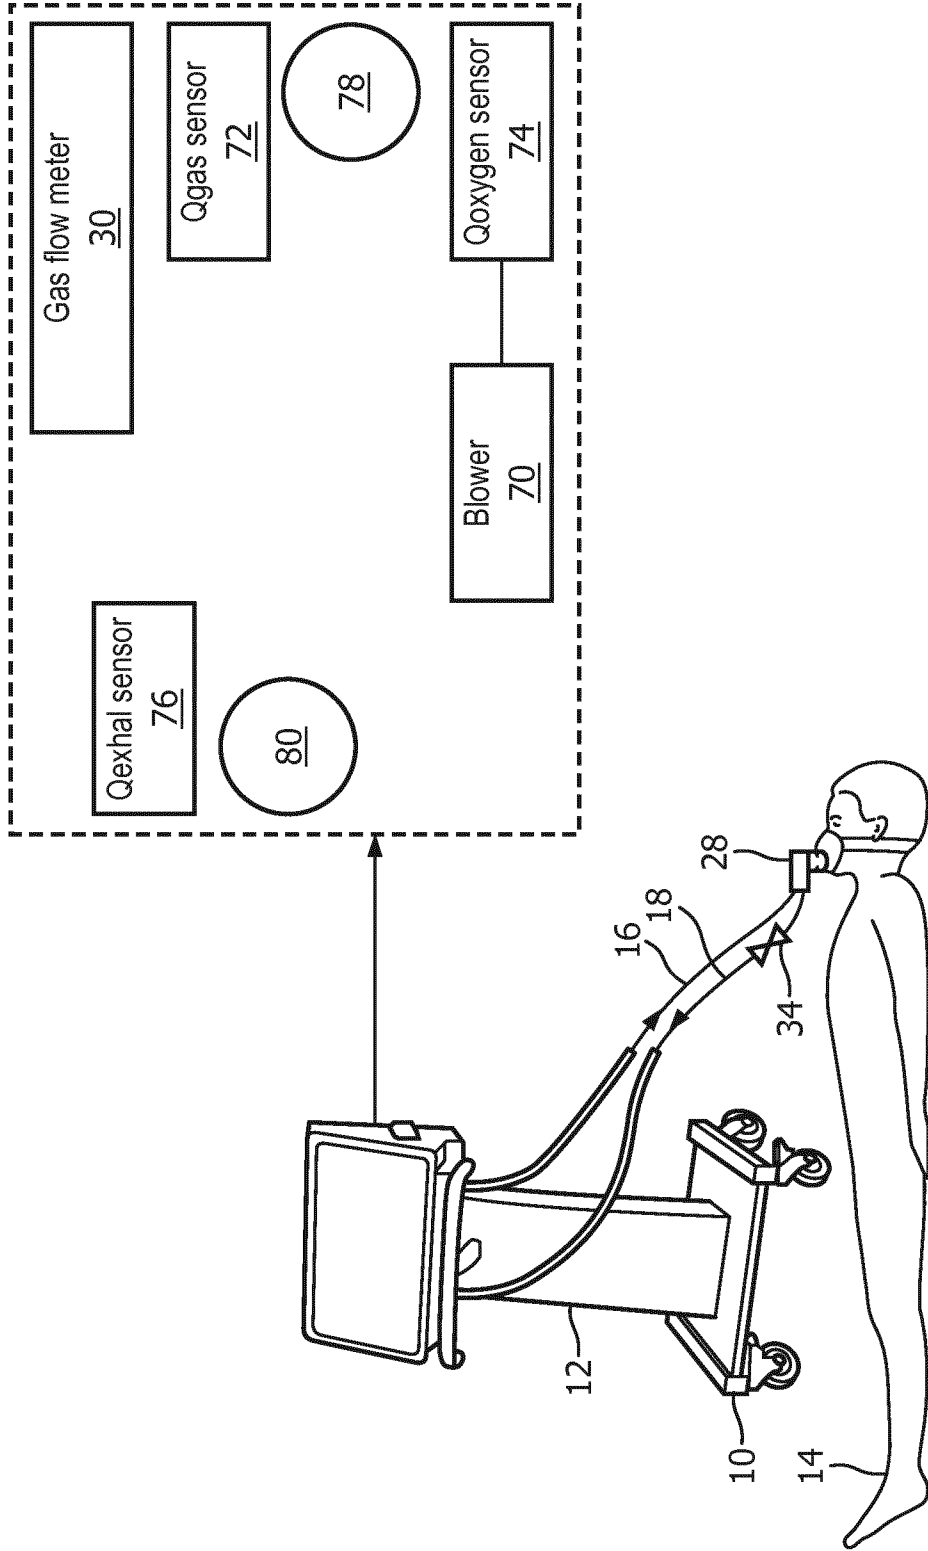


FIG. 3

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2018/068872

A. CLASSIFICATION OF SUBJECT MATTER
INV. G16H20/40 A61B5/08 A61M16/00
ADD.
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
Minimum documentation searched (classification system followed by classification symbols)
G16H A61B A61M G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2014/296730 A1 (STENDQVIST OLA [SE]) 2 October 2014 (2014-10-02) paragraphs [0056] - [0067]; figure 1 -----	1-20
A	US 2014/048072 A1 (ANGELICO PHYLLIS [US] ET AL) 20 February 2014 (2014-02-20) paragraphs [0065] - [0068]; figure 1 -----	1-20
A	EP 2 106 819 A1 (LINDE AG [DE]) 7 October 2009 (2009-10-07) paragraph [0016]; figure 1 -----	1-20
A	US 6 390 091 B1 (BANNER MICHAEL JOSEPH [US] ET AL) 21 May 2002 (2002-05-21) column 9, line 1 - column 10, line 44; figure 2 -----	1-20

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search

27 September 2018

Date of mailing of the international search report

04/10/2018

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Reinbold, Bernhard

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2018/068872

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2014296730	A1	02-10-2014	BR 112012032557 A2
			20-09-2016
			CN 103002802 A
			27-03-2013
			EP 2397074 A1
			21-12-2011
			EP 2582292 A1
			24-04-2013
			EP 2923641 A1
			30-09-2015
			JP 5864562 B2
			17-02-2016
			JP 6162785 B2
			12-07-2017
			JP 2013534844 A
			09-09-2013
			JP 2016104186 A
			09-06-2016
			JP 2017196438 A
			02-11-2017
			US 2013174846 A1
			11-07-2013
			US 2014296730 A1
			02-10-2014
			US 2017332943 A1
			23-11-2017
			WO 2011157855 A1
			22-12-2011

US 2014048072	A1	20-02-2014	NONE

EP 2106819	A1	07-10-2009	NONE

US 6390091	B1	21-05-2002	AU 2866500 A
			25-08-2000
			CA 2362160 A1
			10-08-2000
			EP 1173246 A1
			23-01-2002
			GB 2362109 A
			14-11-2001
			NZ 513864 A
			28-09-2001
			US 6390091 B1
			21-05-2002
			WO 0045880 A1
			10-08-2000
