



US00D643129S

(12) **United States Design Patent**
Talbot et al.

(10) **Patent No.:** **US D643,129 S**

(45) **Date of Patent:** **** Aug. 9, 2011**

(54) **STIMULATION DEVICE**

(75) Inventors: **Nicholas Charles Talbot**, London (GB);
Tanja Langgner, London (GB)

(73) Assignee: **LRC Products Limited**, Slough,
Berkshire (GB)

(**) Term: **14 Years**

(21) Appl. No.: **29/384,808**

(22) Filed: **Feb. 4, 2011**

(30) **Foreign Application Priority Data**

Aug. 11, 2010 (EM) 001229975-0001

(51) **LOC (9) Cl.** **28-03**

(52) **U.S. Cl.** **D24/215**

(58) **Field of Classification Search** D24/200,
D24/211-215; 601/118, 120, 121, 124, 125,
601/130, 131, 134-137

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D496,458 S *	9/2004	Lin	D24/143
D523,958 S *	6/2006	Fang	D24/143
D546,666 S *	7/2007	Mohlin et al.	D8/396
D552,748 S *	10/2007	Gromosaik et al.	D24/215
D552,749 S *	10/2007	Gromosaik et al.	D24/215
D552,750 S *	10/2007	Gromosaik et al.	D24/215
D556,336 S *	11/2007	Talbot et al.	D24/215
D557,805 S *	12/2007	Gromosaik et al.	D24/143
D557,806 S *	12/2007	Gromosaik et al.	D24/143

D566,289 S *	4/2008	Tasker et al.	D24/215
D581,544 S *	11/2008	Adams	D24/215
D637,302 S *	5/2011	Post	D24/215
D637,303 S *	5/2011	Post	D24/215
2005/0155609 A1 *	7/2005	Lin	128/844
2005/0283044 A1 *	12/2005	Chang	600/38
2006/0178602 A1 *	8/2006	Teng et al.	601/70
2007/0038019 A1 *	2/2007	Weng	600/38
2009/0306468 A1 *	12/2009	Tasker et al.	600/41
2009/0318755 A1 *	12/2009	Adams et al.	600/41

* cited by examiner

Primary Examiner — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Ryan A. Schneider;
Troutman Sanders LLP


(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a top front side perspective view of a stimulation device of the present invention;
 FIG. 2 is a top view of the stimulation device of FIG. 1;
 FIG. 3 is a bottom view of the stimulation device of FIG. 1;
 FIG. 4 is a side view of the stimulation device of FIG. 1;
 FIG. 5 is the other side view of the stimulation device of FIG. 1;
 FIG. 6 is a rear view of the stimulation device of FIG. 1;
 FIG. 7 is a front view of the stimulation device of FIG. 1; and,
 FIG. 8 is a bottom rear perspective view of the stimulation device of FIG. 1.

1 Claim, 3 Drawing Sheets

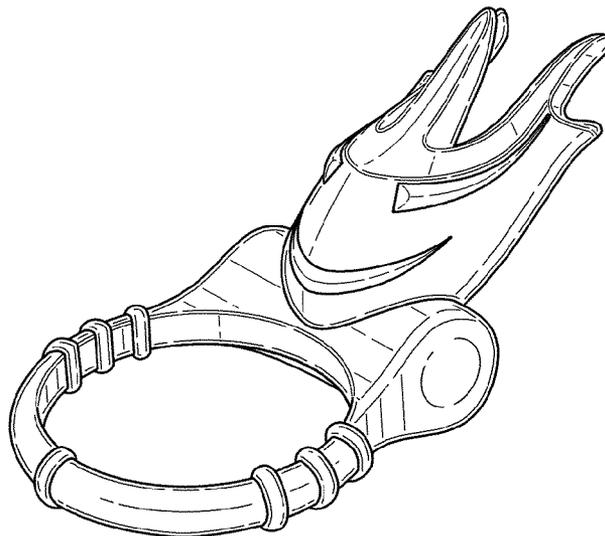

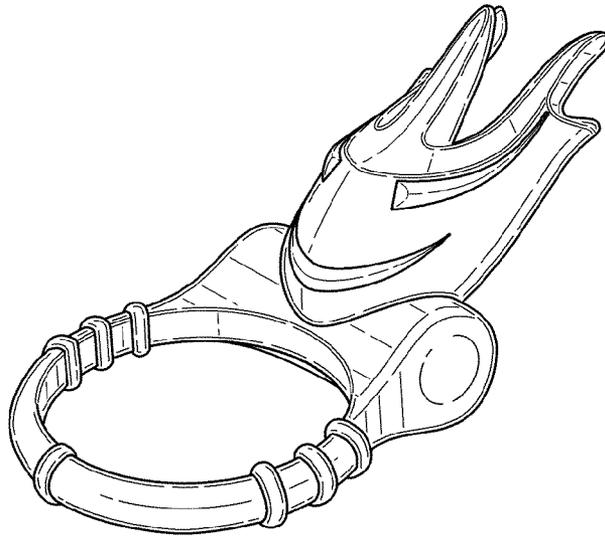


Fig. 1

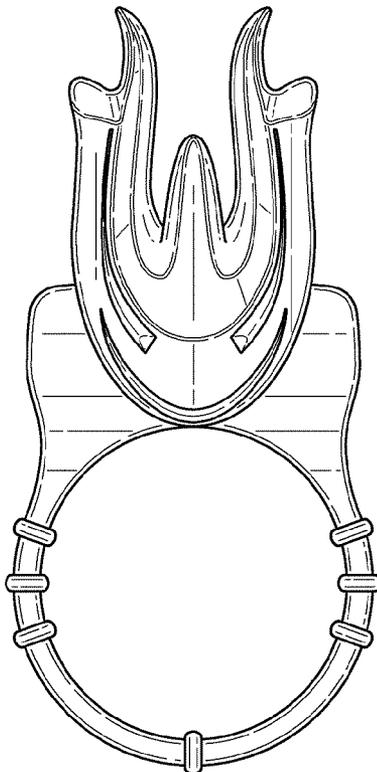


Fig. 2

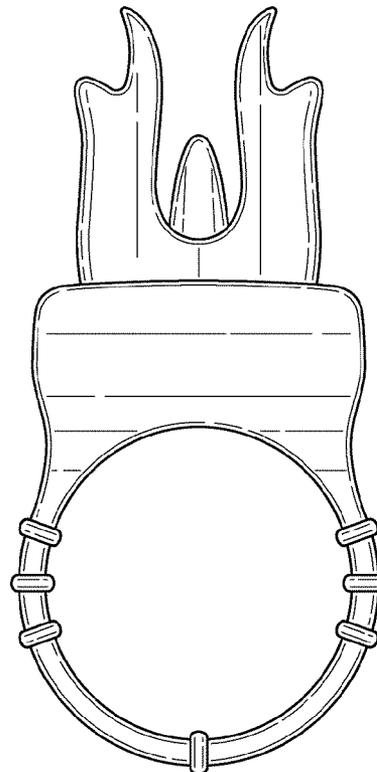


Fig. 3

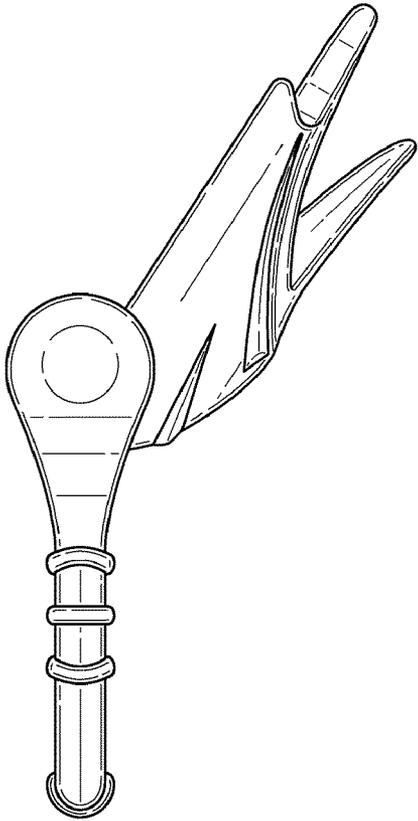


Fig. 4

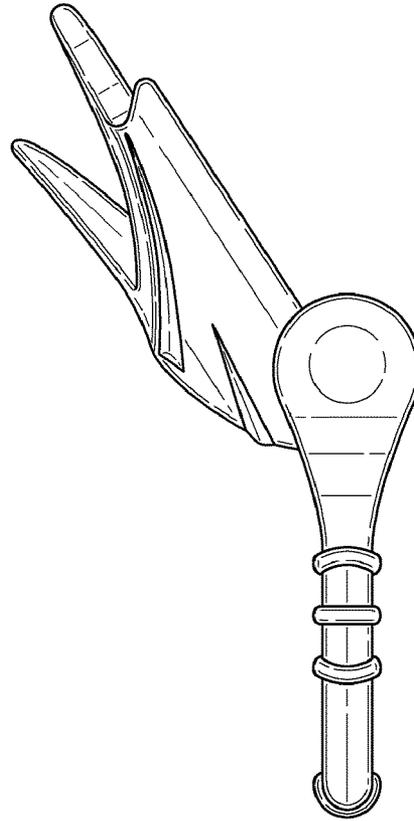


Fig. 5

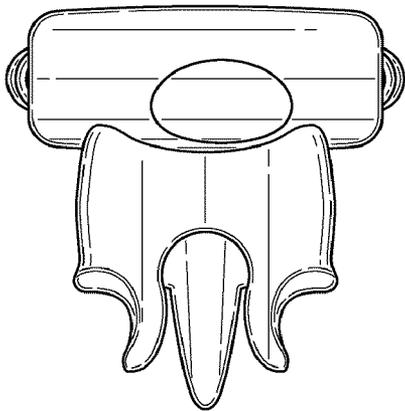


Fig. 6

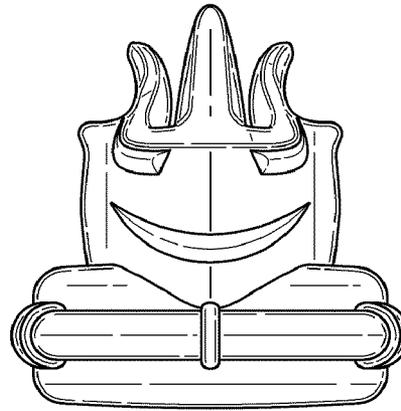


Fig. 7

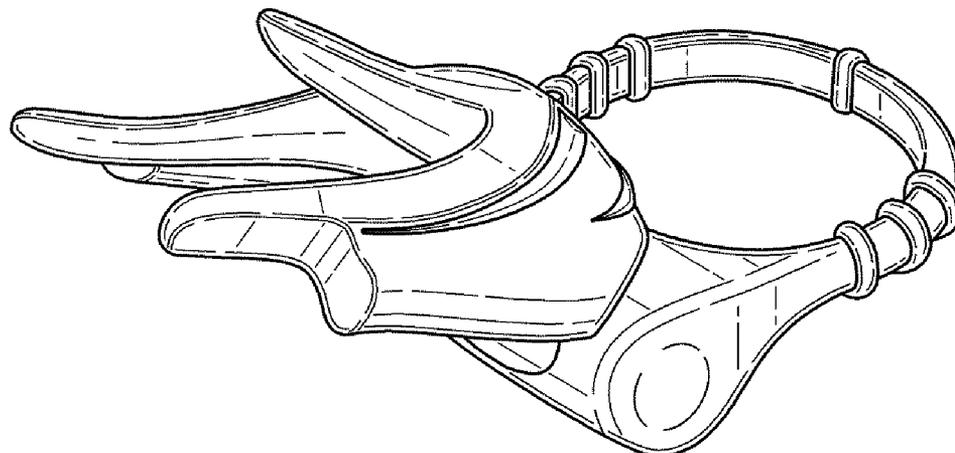


Fig.8