



(12) **DEMANDE DE BREVET CANADIEN
CANADIAN PATENT APPLICATION**

(13) **A1**

(86) Date de dépôt PCT/PCT Filing Date: 2017/07/25
(87) Date publication PCT/PCT Publication Date: 2018/02/01
(85) Entrée phase nationale/National Entry: 2019/01/21
(86) N° demande PCT/PCT Application No.: US 2017/043761
(87) N° publication PCT/PCT Publication No.: 2018/022640
(30) Priorité/Priority: 2016/07/25 (US62/366,509)

(51) Cl.Int./Int.Cl. *A61J 1/10* (2006.01),
A61J 1/20 (2006.01), *A61M 5/172* (2006.01),
B67D 7/76 (2010.01)
(71) Demandeur/Applicant:
ICU MEDICAL, INC., US
(72) Inventeurs/Inventors:
FANGROW, THOMAS F., US;
HACHEY, JAY, US
(74) Agent: AIRD & MCBURNEY LP

(54) Titre : SYSTEMES, PROCEDES ET COMPOSANTS POUR PIEGER DES BULLES D'AIR DANS DES MODULES ET
DES SYSTEMES DE TRANSFERT DE FLUIDE MEDICAL.
(54) Title: SYSTEMS, METHODS, AND COMPONENTS FOR TRAPPING AIR BUBBLES IN MEDICAL FLUID
TRANSFER MODULES AND SYSTEMS

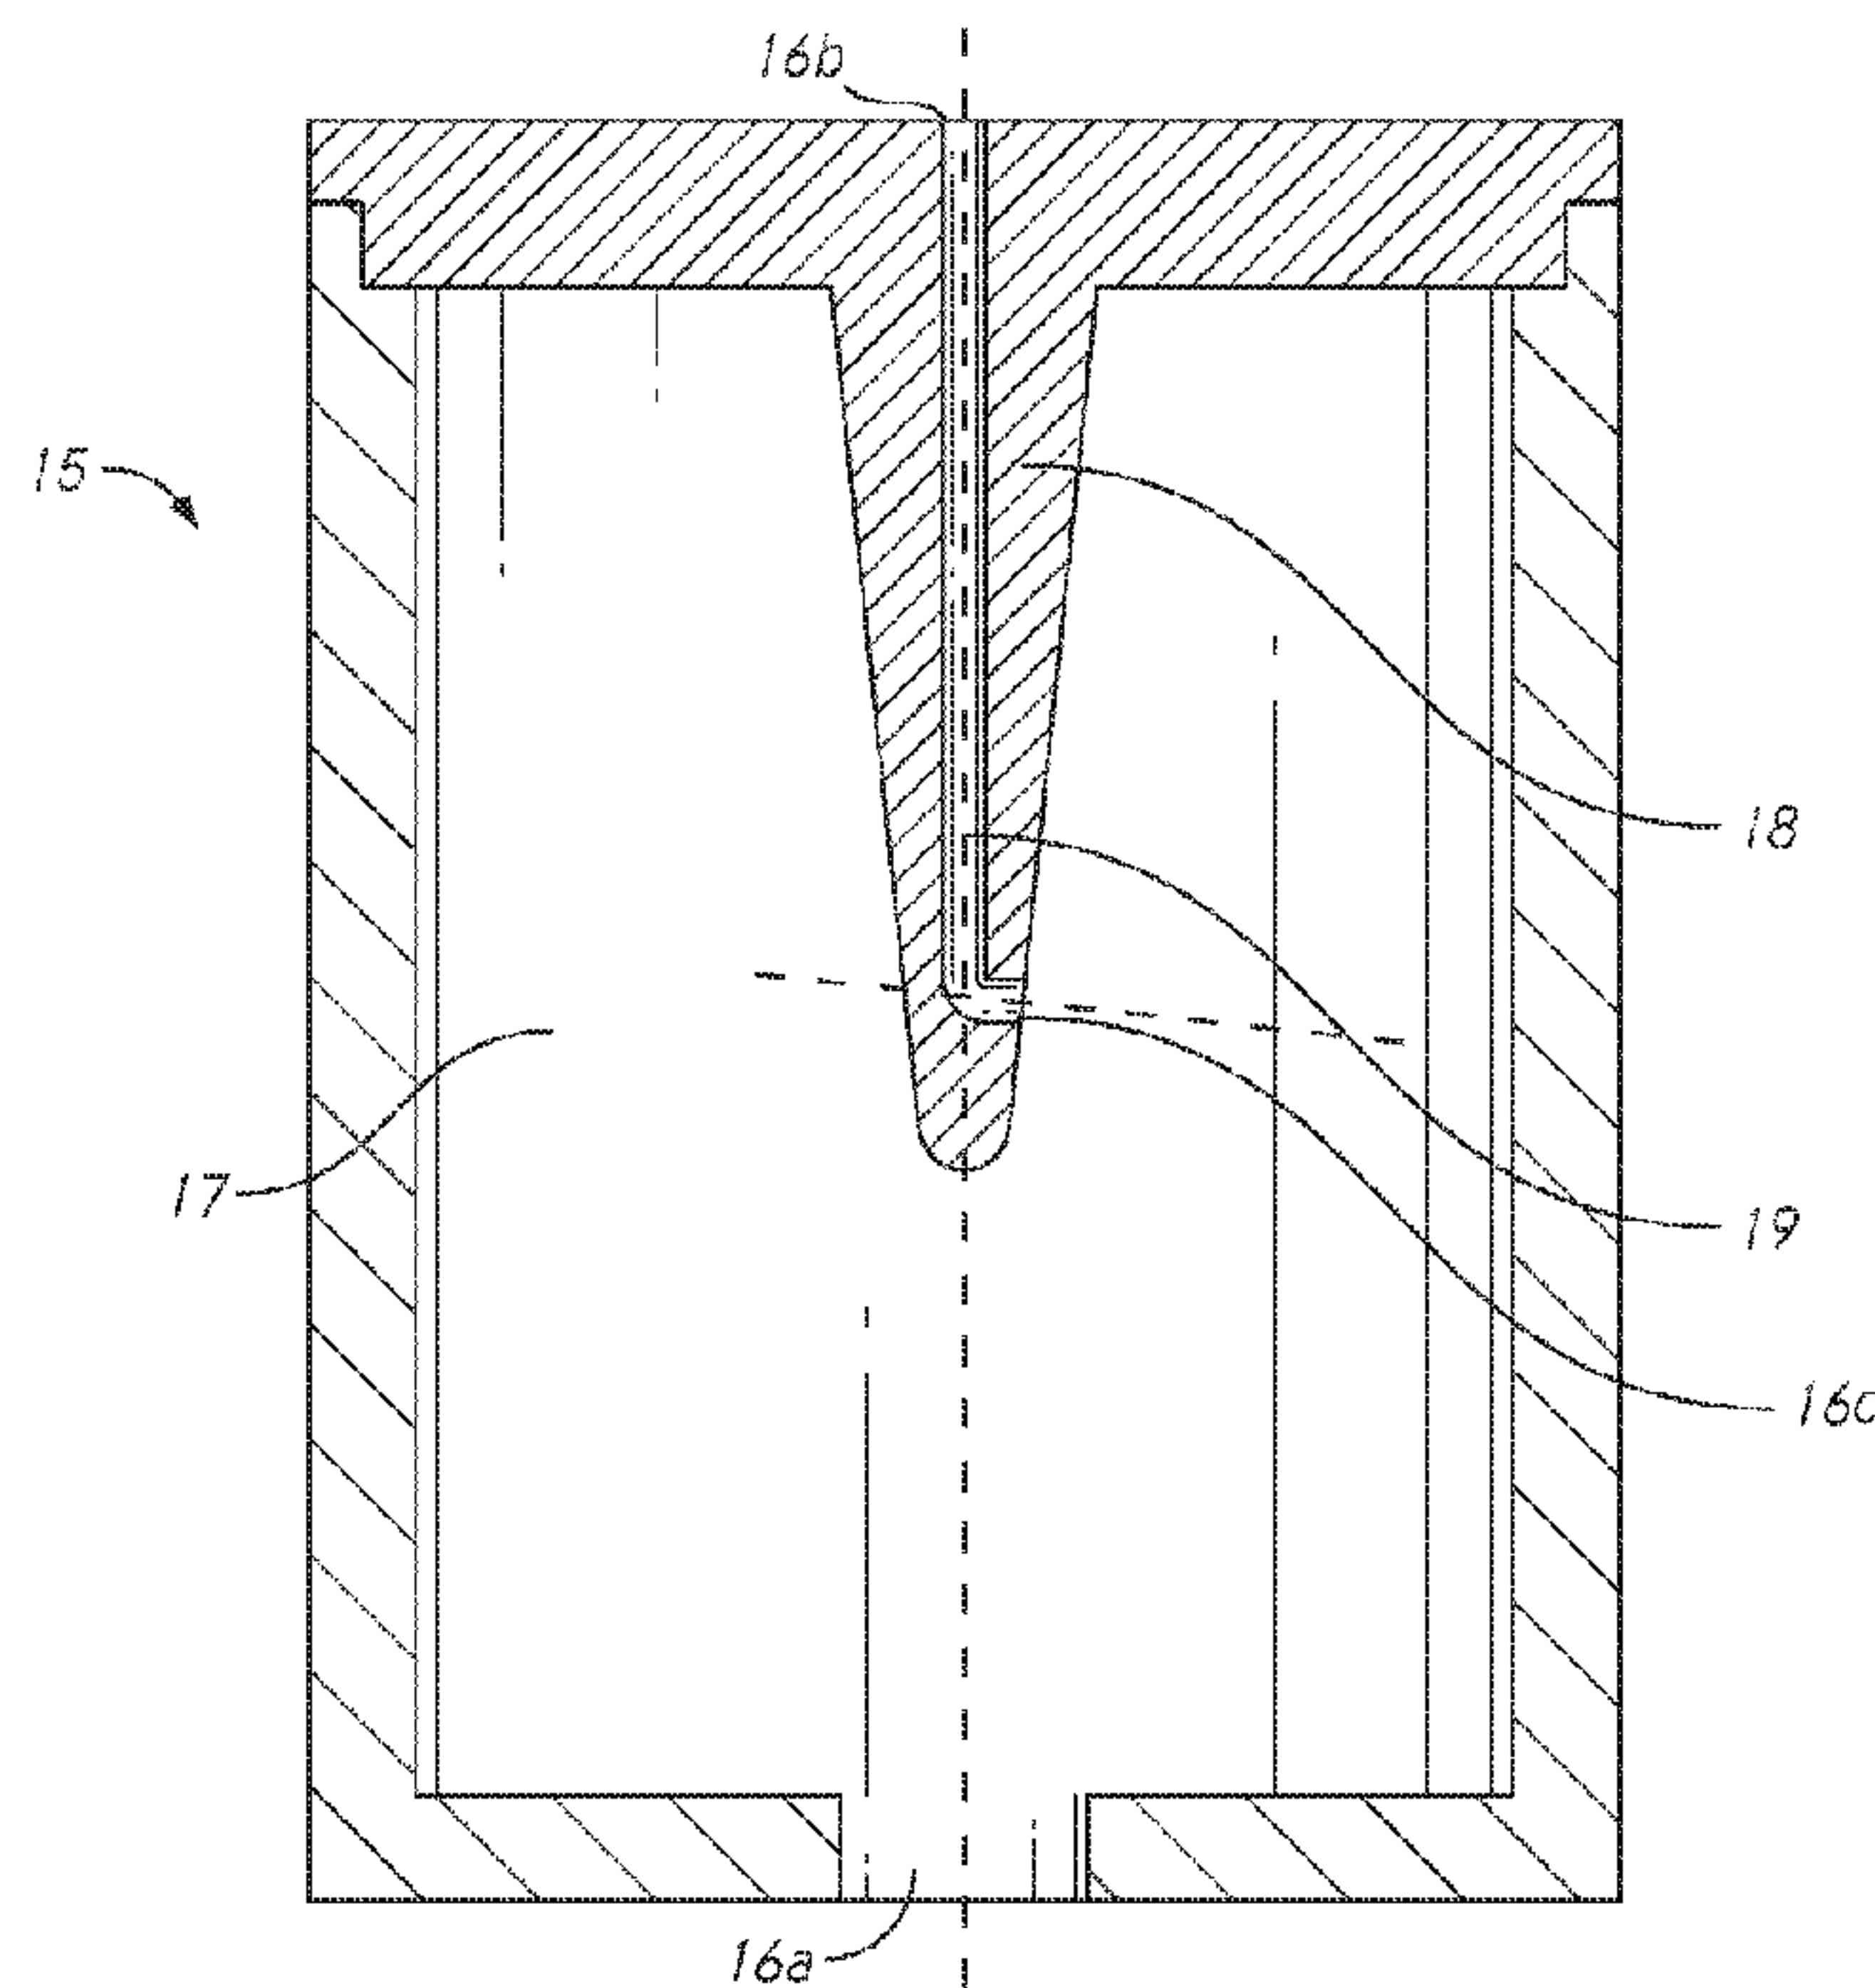


FIG. 6A

(57) **Abrégé/Abstract:**

Bubble traps for use in medical fluid lines and medical fluid bubble trap systems are disclosed herein. In some embodiments, the bubble trap is configured to trap gas (e.g., air) that flows into the bubble trap from a fluid line. In some embodiments, the bubble trap includes an inlet and an outlet and a chamber between the inlet and the outlet. For example, in some embodiments, the bubble trap is configured to inhibit gas from flowing into the outlet once gas flows into the chamber from the inlet. In some embodiments, the bubble trap is in fluid communication with a source container, a destination container, and/or a patient.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau(10) International Publication Number
WO 2018/022640 A1(43) International Publication Date
01 February 2018 (01.02.2018)

(51) International Patent Classification:

A61J 1/10 (2006.01) *A61M 5/172* (2006.01)
A61J 1/20 (2006.01) *B67D 7/76* (2010.01)

(21) International Application Number:

PCT/US2017/043761

(22) International Filing Date:

25 July 2017 (25.07.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/366,509 25 July 2016 (25.07.2016) US

(71) Applicant: **ICU MEDICAL, INC.** [US/US]; 951 Calle Amanecer, San Clemente, CA 92673 (US).(72) Inventors: **FANGROW, Thomas, F.**; 951 Calle Amanecer, San Clemente, CA 92673 (US). **HACHEY, Jay**; 951 Calle Amanecer, San Clemente, CA 92673 (US).(74) Agent: **ALTMAN, Daniel, E.**; Knobbe Martens, 2040 Main Street, 14th Floor, Irvine, CA 92614 (US).(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,

(54) Title: SYSTEMS, METHODS, AND COMPONENTS FOR TRAPPING AIR BUBBLES IN MEDICAL FLUID TRANSFER MODULES AND SYSTEMS

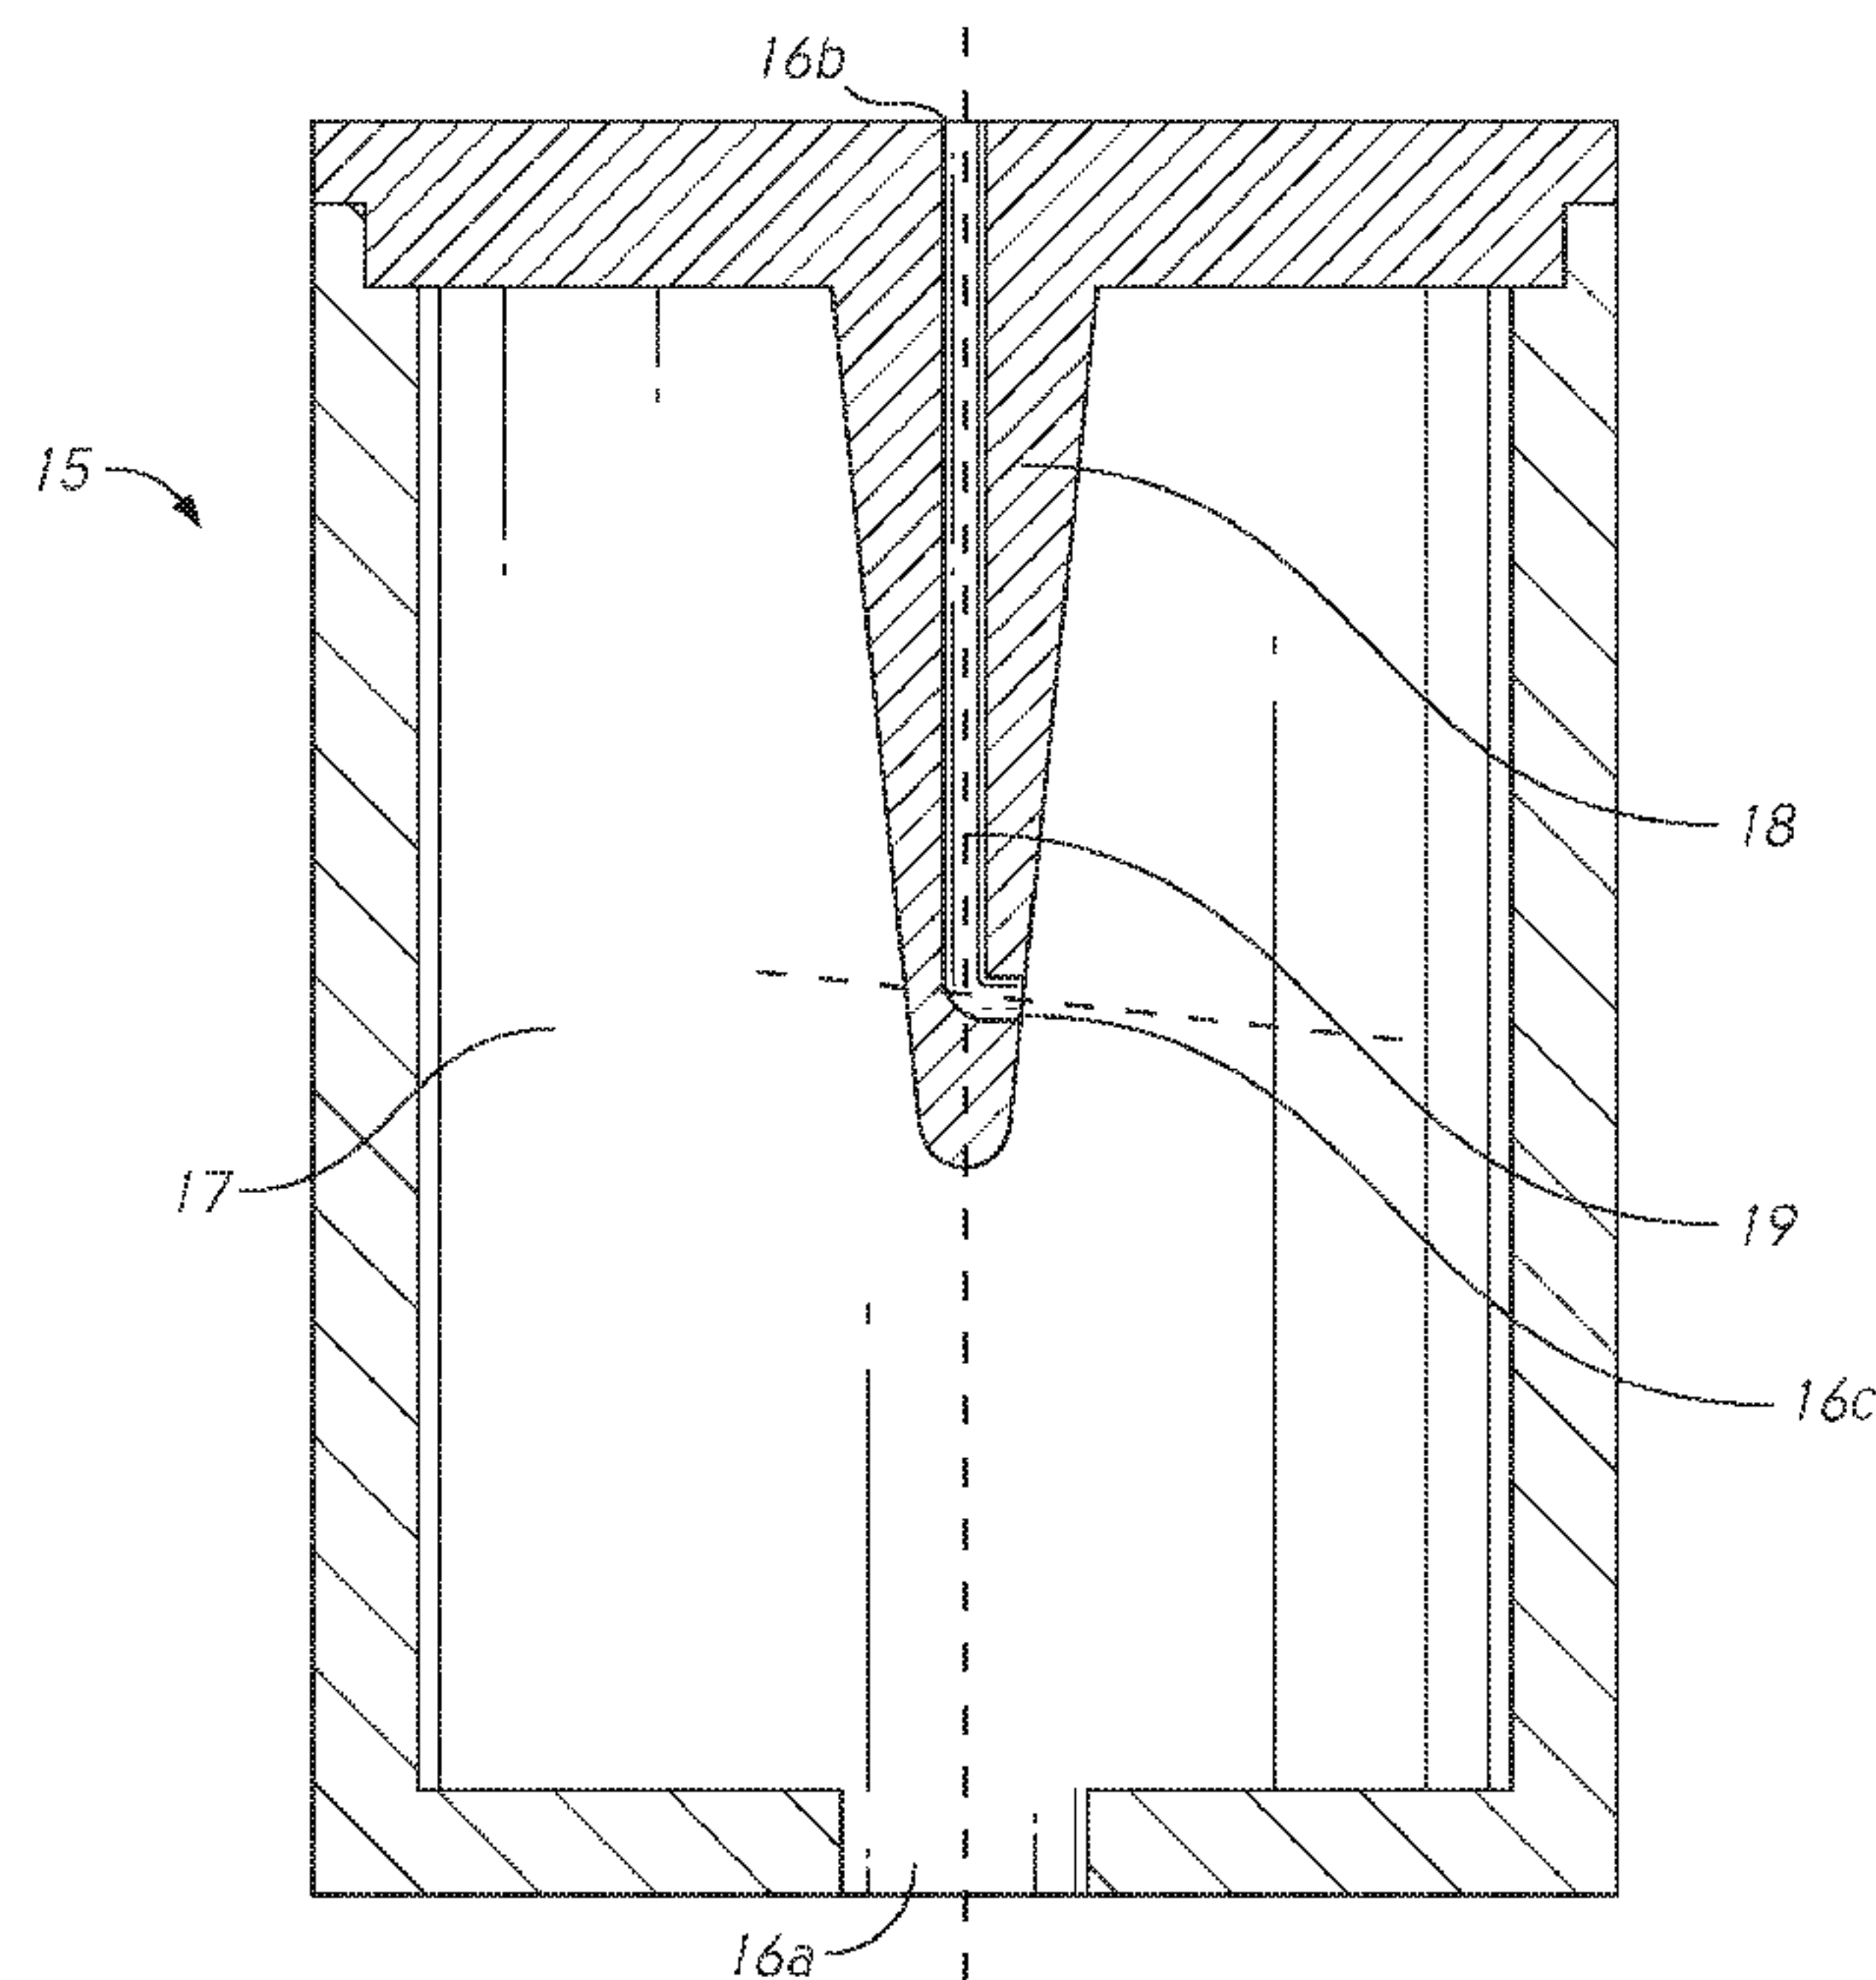


FIG. 6A

(57) Abstract: Bubble traps for use in medical fluid lines and medical fluid bubble trap systems are disclosed herein. In some embodiments, the bubble trap is configured to trap gas (e.g., air) that flows into the bubble trap from a fluid line. In some embodiments, the bubble trap includes an inlet and an outlet and a chamber between the inlet and the outlet. For example, in some embodiments, the bubble trap is configured to inhibit gas from flowing into the outlet once gas flows into the chamber from the inlet. In some embodiments, the bubble trap is in fluid communication with a source container, a destination container, and/or a patient.

[Continued on next page]

WO 2018/022640 A1

TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*
- *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

**SYSTEMS, METHODS, AND COMPONENTS
FOR TRAPPING AIR BUBBLES IN MEDICAL FLUID TRANSFER MODULES
AND SYSTEMS**

BACKGROUND

Field

[0001] This invention relates to controlling the transfer of medical fluids and, more particularly, to limiting the transmission of gas bubbles within the medical fluids.

Description of the Related Art

[0002] Many types of medical fluids are routinely used to treat patients, including chemotherapy drugs, antibiotics, immunosuppressive drugs, antiviral drugs, hydrating fluids, nourishing fluids, anticoagulants, pain management drugs, contrast fluids for medical imaging, etc. All of these fluids, in turn, come in many different varieties with advantages and disadvantages for various types of diseases, conditions, injuries, or therapies. Moreover, particular patients require optimized dosages, concentrations, and combinations of these drugs or other medical fluids to address their specific medical needs. As a result, medical facilities are required to provide many different types of customized medical fluids on a continual basis to meet individual patient needs. In meeting these needs, a small amount of air is often present in the medical fluids that are prepared.

[0003] Systems and methods disclosed herein address various challenges related to medical fluid transfer systems and the presence of air in medical fluids.

SUMMARY

[0004] In some embodiments, a bubble trap for use in a medical fluid line is disclosed.

[0005] In some embodiments, a medical fluid bubble trap system is disclosed. The system can include a bubble trap configured to be in fluid communication with at least one of a source container and a destination container. The bubble trap can be configured to trap gas that flows into the bubble trap.

[0006] In some embodiments, a medical fluid bubble trap system is disclosed. The system can include a source container and a fluid transfer module comprising a bubble

trap and a destination container. The bubble trap can be configured to trap gas that flows into the bubble trap.

[0007] In some embodiments, a medical fluid transfer module comprising a bubble trap configured to trap gas in a chamber is disclosed.

[0008] In some embodiments, an electronic medical fluid transfer device comprising a bubble trap configured to trap gas in a chamber is disclosed.

[0009] In some embodiments, an inline bubble trap device is configured to be in fluid communication with a medical fluid line to inhibit a flow of gas from an inlet to an outlet. The bubble trap device can comprise an inlet comprising an inlet opening having an inlet opening center axis, an outlet comprising an outlet opening having an outlet opening center axis, and a chamber. The inlet opening center axis and the outlet opening center axis can be different from one another such that the inlet opening is misaligned from the outlet opening. In some embodiments, the misalignment of the inlet opening from the outlet opening breaks up a fluid path from the inlet opening to the outlet opening. The chamber can be configured to trap gas that flows into the bubble trap. The chamber can be located between the inlet and the outlet.

[0010] In some embodiments, an outlet can comprise an outlet projection. The outlet projection can comprise an outlet opening and a channel in fluid communication with the outlet. The outlet projection can extend into the chamber away from an inner surface of the chamber. The outlet opening of the outlet projection can be positioned near or at the center of the chamber. The outlet opening of the outlet projection can be positioned on a side of the outlet projection.

[0011] In some embodiments, an inlet comprises an inlet projection. The inlet projection can comprise an inlet opening and a channel in fluid communication with the inlet. The inlet projection can extend into the chamber away from an inner surface of the chamber. The inlet opening can be positioned near or at the center of the chamber. The inlet opening can be positioned on a side of the inlet projection.

[0012] In some embodiments, an inlet projection and an outlet projection can extend past each other such that inlet opening is positioned closer to an outlet than the outlet opening.

[0013] In some embodiments, every flow path from an inlet opening to an outlet opening includes a bend. An inlet and an outlet can be on opposite ends of a chamber.

[0014] In some embodiments, a bubble trap can include a resilient housing at least partially defining a chamber with a rest volume. The housing can be configured to at least partially collapse when subjected to a vacuum so as to reduce the volume of the chamber and configured to return to the rest volume when the vacuum is removed.

[0015] In some embodiments, a medical fluid transfer system is configured to trap air during the transfer of medical fluids. The medical fluid transfer system can comprise a fluid transfer device configured to transfer fluid from a fluid source to a fluid destination and an inline bubble trap, as described herein. The inline bubble trap can comprise a female luer end and a male luer end. The bubble trap can be configured to be in fluid communication with at least one of the fluid transfer device, a fluid source, and a fluid destination. The bubble trap can be configured to inhibit a transfer of gas from the fluid source, through the outlet of the bubble trap, and into the fluid destination. The bubble trap can be in fluid communication with the fluid source. The bubble trap can be in fluid communication with the fluid destination. The female luer end can be adjacent to the outlet. The male luer end can be adjacent to the inlet.

[0016] In some embodiments, a method of transferring fluids from a source container to a destination container can comprise the step of obtaining a fluid transfer module configured to inhibit a transfer of gas from the source container to the destination container. The fluid transfer module can comprise an inline bubble trap. The bubble trap can comprise a chamber, an inlet opening having an inlet center axis, and an outlet opening having an outlet center axis different from the inlet center axis such that the inlet opening is misaligned from the outlet opening. The method of transferring fluids can further comprise the steps of ensuring the fluid transfer module is in fluid communication with the source container and the destination container and transferring fluid from the source container, through the fluid transfer module, and into the destination container. The method can further comprise the step of initiating a vacuum in the destination container and the fluid transfer module such that a volume defined by the chamber of the fluid transfer module is reduced prior to initiating the transferring step. The inlet opening being misaligned from the outlet opening can break up a fluid path from the inlet opening to the outlet opening. The the fluid transfer

module can further comprise an outlet projection having the outlet opening and a channel in fluid communication with the outlet. The outlet projection can extend into the chamber away from an inner surface of the chamber. The outlet opening of the outlet projection can be positioned on a side of the outlet projection. The fluid transfer module can further comprise an inlet projection having the inlet opening and a channel in fluid communication with the inlet. The inlet projection can extend into the chamber away from an inner surface of the chamber. The inlet opening can be positioned on a side of the inlet projection. The method can further comprise disconnecting the fluid transfer module from the source container and the destination container.

[0017] In some embodiments, an inline bubble trap device is configured to be in fluid communication with a medical fluid line to inhibit a flow of gas from an inlet to an outlet. The bubble trap device can comprise a chamber comprising an inner surface and an outer surface, an inlet comprising an inlet projection extending into the chamber, the inlet projection having an inlet channel and an inlet opening being displaced away from the inner surface of the chamber, an outlet comprising an outlet projection extending into the chamber, the outlet projection having an outlet channel and an outlet opening being displaced away from the inner surface of the chamber. The inlet opening and the outlet opening can be oriented away from each other such that fluid moving between the openings need take an indirect path. At least one of the inlet and the outlet channels can comprise a curve that misaligns the inlet opening from the outlet opening and breaks up a fluid path from the inlet opening to the outlet opening through the chamber. The chamber can be configured to trap gas that flows into the bubble trap. The chamber can be collapsible. The outlet opening of the outlet projection can be positioned near or at the center of the chamber. The inlet opening can be positioned near or at the center of the chamber. The inlet projection and the outlet projection can project past each other within the chamber.

[0018] In some embodiments, a patient source bag is for use with a medical fluid infusion pump. The patient source bag can comprise a chamber, an outlet comprising an outlet region in fluid communication with the chamber, and a barrier defining an air collection region in fluid communication with the outlet. The barrier can be configured to maintain air within the air collection region. The barrier can be configured inhibit the transfer of gas through the outlet region. The air collection region can be located outside a

continuous fluid flow path between the chamber and the outlet region. The air collection region can be spaced apart from the outlet. The outlet can be located on an upper region of the chamber. The outlet can be configured to permit the passage of fluid into and out of the chamber. The patient source bag can further comprise a port configured to permit the removal of air from the chamber. The patient source bag can further comprise at least one access port. The access port can be a closeable female luer connector. The access port can be a closeable male luer connector. The patient source bag can further comprise a bubble trap outside the chamber and in fluid communication with the chamber.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] Embodiments will now be described with reference to the following drawings, which are provided by way of example, and not limitation. Like reference numerals indicate identical or functionally similar elements.

[0020] Figure 1A is a schematic illustration of an example of a fluid transfer device removably attached to and/or in selective communication with other components of a fluid transfer system.

[0021] Figure 1B is a schematic illustration of an example of a system for transferring medical fluid that includes the fluid transfer device of Figure 1A.

[0022] Figure 2A_i is a front perspective view of an example of an electromechanical system for transferring medical fluid.

[0023] Figure 2B_i is a rear view of an example of a fluid transfer device.

[0024] Figure 2C_i is a front perspective view of the electromechanical system for transferring medical fluid of Figure 2A_i with the fluid transfer device of Figure 2B_i attached to it.

[0025] Figure 2D_i is a magnified partial front view of the electromechanical system of Figure 2A_i which illustrates an example of a driver.

[0026] Figure 2A_{ii} is a front perspective view of an example of an electromechanical system for transferring medical fluid according to another embodiment.

[0027] Figure 2B_{ii} is a rear view of an example of a fluid transfer device according to another embodiment.

[0028] Figure 2C_{ii} is a front perspective view of the electromechanical system for transferring medical fluid of Figure 2A_{ii} with the fluid transfer device of Figure 2B_{ii} attached to it.

[0029] Figure 2D_{ii} is a magnified partial front view of the electromechanical system of Figure 2A_{ii} which illustrates an example of a driver.

[0030] Figure 2E_{ii} is a rear perspective cross-sectional view of the electromechanical system and fluid transfer device shown Figure 2C_{ii}.

[0031] Figure 3 is a front plan view of an example of a user control device.

[0032] Figure 4 is a schematic illustration of a user interface configured to electronically communicate with a plurality of different types of medical fluid transfer devices.

[0033] Figure 5A is a schematic of a fluid transfer module having a bubble trap in fluid communication with a source container.

[0034] Figure 5B is a schematic of the fluid transfer module of Figure 5A disconnected from the source container and in fluid communication with a patient.

[0035] Figure 5C is a schematic of a fluid transfer module having a bubble trap in fluid communication with the fluid transfer device of Figure 1A.

[0036] Figure 6A is a schematic of a bubble trap, according to some embodiments.

[0037] Figure 6A' is a schematic of the bubble trap of Figure 6A with luer connectors.

[0038] Figure 6B is another schematic of a bubble trap, according to some embodiments.

[0039] Figure 6C is another schematic of a bubble trap, according to some embodiments.

[0040] Figure 7A is a schematic of a bubble trap with fluid flow in a first position, according to some embodiments.

[0041] Figure 7B is a schematic of the bubble trap of Figure 7A rotated 45 degrees counterclockwise.

[0042] Figure 7C is a schematic of the bubble trap of Figure 7B rotated 45 degrees counterclockwise.

[0043] Figure 7D is a schematic of the bubble trap of Figure 7C rotated 45 degrees counterclockwise.

[0044] Figure 7E is a schematic of the bubble trap of Figure 7D rotated 45 degrees counterclockwise.

[0045] Figure 7F is a schematic of the bubble trap of Figure 7E rotated 45 degrees counterclockwise.

[0046] Figure 7G is a schematic of the bubble trap of Figure 7F rotated 45 degrees counterclockwise.

[0047] Figure 7H is a schematic of the bubble trap of Figure 7G rotated 45 degrees counterclockwise.

[0048] Figure 8A is a schematic of a bubble trap with a vacuum applied, according to some embodiments.

[0049] Figure 8B is a schematic of the bubble trap of Figure 8A filled with fluid.

[0050] Figure 9A is a schematic of a bubble trap attached to a cassette with a reservoir, according to some embodiments.

[0051] Figure 9B is a schematic of a bubble trap attached to a cassette without a reservoir, according to some embodiments.

[0052] Figure 9C is an example protocol for filling the cassette of Figure 9A with medical fluid.

[0053] Figure 10A is a schematic of a cassette configured to trap air, according to some embodiments.

[0054] Figure 10B is another schematic of a cassette configured to trap air, according to some embodiments.

DETAILED DESCRIPTION

[0055] Various systems, methods, and components can be used in different embodiments of the inventions. Some embodiments are illustrated in the accompanying figures; however, the figures are provided for convenience of illustration only, and should not be interpreted to limit the inventions to the particular combinations of features shown. Rather, any feature, structure, material, step, or component of any embodiment described and/or illustrated in this specification can be used by itself, or with or instead of any other

feature, structure, material, step, or component of any other embodiment described and/or illustrated in this specification. Nothing in this specification is essential or indispensable.

[0056] Figure 1A is an example of a schematic illustration of a fluid transfer device 30 removably attached to and/or in selective communication with other components of a fluid transfer system. In some embodiments, a fluid transfer device 30 can comprise a source container 39, a fluid transfer module 31, an electromechanical controller 36, and a destination container 44. The source container 39 and the fluid destination container 44 can each comprise any suitable device for holding or supplying medical fluids, such as a vial, a bottle, a bag, a hose, a tube, a tank, a canister, etc. In some embodiments, the fluid destination container 44 is a type of container that is selected to be particularly well suited in size and structure for easy and convenient storage or transportation from a fluid transfer station to a patient treatment location, such as an intravenous fluid storage bag or IV bag, to provide an individual-patient, single-dosage supply of medical fluid. In some embodiments, the source container 39 is a type of container that is sufficiently large to provide multiple single-patient doses to be transferred into multiple destination containers 44 (either serially or in parallel). Some examples of fluid transfer devices 30 are illustrated and described in U.S. Patent No. 8,522,832; U.S. Patent Application Publication No. 2014/0299221; PCT International Application No. US2015/040174; and U.S. Patent Application Publication No. 2015/0283322, all of which are incorporated by reference in their entireties and made a part of this specification, and any feature, structure, material, step, or component of any embodiment described and/or illustrated in any of these can be used with or instead of any other feature, structure, material, step, or component of any embodiment described and/or illustrated elsewhere in this specification.

[0057] The fluid transfer module 31 can comprise a multidirectional flow-control valve 41 and an intermediate container or pumping region 40, as well as any connector(s) and/or conduit(s) that may extend between or among these or any other components of the fluid transfer module 31, and/or any connectors and/or conduits that may extend between or among the fluid transfer module 31 and the source container 39 and/or the destination container 44. For example, the fluid transfer module 31 can comprise an inlet fluid connector 32 and tubing that can be configured to removably attach the multidirectional flow-control valve to the source container 39; and/or the fluid transfer module 31 can

comprise an outlet fluid connector 42 and tubing that can be configured to removably attach the multidirectional flow control valve to the destination container 44.

[0058] As shown in Figure 1A, the fluid transfer module 31 can comprise an intermediate fluid connector 38 that fluidly connects the multidirectional flow-control valve 41 and the intermediate container or pumping region 40. In some embodiments, the intermediate fluid connector 38 is a conduit and/or a tube attached by an appropriate permanent, fluid-tight method (e.g., adhesive, bonding, ultrasonic welding, etc.) between the multidirectional flow-control valve 41 and the intermediate container or pumping region 40. The intermediate container or pumping region 40 can comprise any suitable container or region that is configured to hold and measure fluids and/or to assist in providing an impetus for fluid-flow along a fluid conveying path. For example, in some embodiments, the intermediate container or pumping region 40 can be a syringe or a region of a conduit that is configured to interface with a peristaltic pump, or any other suitable intermediate device. Not all fluid transfer modules 31 will include all of the components or features illustrated or described in this specification; rather, one or more components or features can be omitted in any suitable embodiment.

[0059] The multidirectional flow-control valve 41 can be configured to mechanically attach to or interface with the electromechanical controller 36. For example, in some embodiments, the multidirectional flow-control valve 41 can comprise a driving interface 33 that is configured to attach with and/or interface with a corresponding electromechanical driver (see, e.g., Figures 2Ai, 2Di, 2Aii, 2Dii) of the electromechanical controller 36. The electromechanical controller 36 can actuate the multidirectional flow-control valve 41 under the control of one or more algorithms or instructions provided by a computer processor or a plurality of computer processors in the fluid transfer management system 74 (see Figure 1B) that is or are configured to send one or more electronic signals to the electromechanical controller 36 to select among a plurality of functional positions on the multidirectional flow-control valve 41; however, any suitable computer processing arrangement capable of controlling the multidirectional flow-control valve 41 can be used and is envisioned and contemplated herein. Any disclosure in this specification of a single computer processor applies to and can be used with a plurality of computer processors.

[0060] In some embodiments, the multidirectional flow-control valve 41 can comprise a stopcock with a plurality of functional positions, such as a first position that enables fluid communication between the outlet fluid connector 42 and the intermediate container or pumping region 40 (but not the inlet fluid connector 32, in some embodiments); a second position that enables fluid communication between the inlet fluid connector 32 and the intermediate container or pumping region 40 (but not the outlet fluid connector 42, in some embodiments); and a third position that enables fluid communication between the outlet fluid connector 42 and the inlet fluid connector 32 (but not the intermediate container or pumping region 40, in some embodiments). For example, in some embodiments, when the stopcock is in the first position, fluid can flow from the intermediate container or pumping region 40 to the destination container 44 or vice versa; when the stopcock is in the second position, fluid can flow from the source container 39 to the intermediate container or pumping region 40 or vice versa; and when the stopcock is in the third position, fluid can flow from the source container 39 to the destination container 44 or vice versa. Further, in some embodiments, when the stopcock is in the first position, the intermediate fluid connector 38, the stopcock, and the outlet fluid connector 42 can comprise at least a portion of a flow path between the intermediate container or pumping region 40 and the destination container 44; when the stopcock is in the second or fourth position, the inlet fluid connector 32, the stopcock, and the intermediate fluid connector 38 can comprise at least a portion of a flow path between the source container 39 and the intermediate container or pumping region 40; and when the stopcock is in the third position, the inlet fluid connector 32, the stopcock, and the outlet fluid connector 42 can comprise at least a portion of a flow path between the source container 39 and the destination container 44. In some embodiments, the stopcock can comprise at least a portion of one or more flow paths between or among two or more containers (e.g., the source container 39, the intermediate container or pumping region 40, and/or the destination container 44) without the use of any connectors (e.g., the inlet fluid connector 32, the intermediate fluid connector 38, and/or the outlet fluid connector 42) when in the first, second, third, and/or fourth position. Other arrangements can be used are also appreciated and contemplated herein, including, for example, stopcocks configured to have more or less than three positions (e.g., stopcocks configured to have 2, 4, 5, or more positions).

[0061] In some embodiments, the fluid transfer module 31 can be a single-use or limited-use, disposable device that is configured to be periodically removed from and replaced within the fluid transfer device 30, such as after a single dosage of medication for a particular patient has been transferred and/or after one particular type of medication has passed through the fluid transfer module 31 (e.g., to avoid mixing of medications when not desired).

[0062] Figure 1B is a schematic illustration of a fluid transfer system 86 for transferring medical fluid that includes the fluid transfer device 30 of Figure 1A, according to some embodiments. For example, as shown in Figure 1B, one or more fluid transfer devices 30 can form part of a fluid transfer system 86 that can include one or more of the following components that can be selectively positioned in electronic communication between or among each other: one or more electronic patient and/or drug information storage devices or networks 70; one or more fluid transfer management systems 74 comprising one or more fluid transfer devices 30, a user interface 78, and/or one or more memories 84. In some embodiments, the one or more electronic patient and/or drug information storage devices or networks 70 can be physically remote from the fluid transfer management system 74. For example, in a health clinic or hospital, the one or more electronic patient and/or drug information storage devices or networks 70 can comprise a remote patient information management system with a database that can be queried to provide information about a particular patient's needs for medical fluids (e.g., a drug prescription) that may include the type, dosage, lot number, expiration date, and/or concentration of one or more drugs or other medical fluids to be provided to a patient, and/or identifying information regarding one or more health care provider who prescribed, requested, and/or filled the destination container, and/or the time and/or date associated with any or all of these activities. Any medical information, such as any of the foregoing medical information, can be provided by the one or more fluid transfer devices 30 for recording and storage in the patient information management system.

[0063] The various components of the fluid transfer system 86 can communicate between or among themselves in any suitable manner, as identified in Figure 1B. For example, as illustrated, the one or more patient and/or drug information storage device(s) or network(s) 70 can electronically communicate with the fluid transfer management system 74,

or any components thereof, by way of an electronic communication link 72, formed by any suitable electronic communication device, such as a wired connection, a local area network, a wide area network, the Internet, and/or a wireless connection (including, e.g., Wi-Fi, Bluetooth, Ant+, ZigBee, cellular, etc.), or any other electronic communication device (collectively referred to as “electronic communicators”). The fluid transfer management system 74 may comprise a wireless communication console, such as a Wi-Fi box that is configured to send and/or receive data, including patient data, data regarding a fluid transfer, data regarding the type, dosage, concentration, volume, image, technician, physician, and/or time of a fluid transfer, and/or data to control the electronic fluid transfer system 86, etc. The fluid transfer device 30 can communicate with a memory 84 by any suitable electronic connection, such as a wired connection, or any other electronic communicators. In some embodiments, the memory 84 is part of the fluid transfer device 30, in that a common housing is provided for containing or supporting both.

[0064] The user interface 78 can communicate with one or more fluid transfer devices 30 and/or with one or more patient and/or drug information storage device(s) or network(s) 70 by way of any suitable electronic communication device 76, including by way of any wireless device or by way of any other of the electronic communicators. In some embodiments of the fluid transfer management system 74 in which there are multiple fluid transfer devices 30, a single user interface 78 can electronically communicate with a plurality of fluid transfer devices 30 to control and/or monitor multiple fluid transfers operating generally simultaneously or generally in parallel. In some embodiments of the fluid transfer management system 74 in which there are multiple fluid transfer devices 30, one or more user interfaces 78 can electronically communicate with a plurality of fluid transfer devices 30 to control and/or monitor multiple fluid transfers operating generally simultaneously or generally in parallel. The user interface 78, like the fluid transfer device 30, can electronically communicate with or include a memory 84 by way of a wired connector 80 or any other of the electronic communicators. The memory 84 of the user interface 78 can be part of the user interface 78 in that a common housing can be provided for containing or supporting both. Each of the components of the fluid transfer management system 74 as shown in Figure 1B (e.g., the fluid transfer device(s) 76, the user interface 78, and the

memory or memories 84) can be provided in a single housing, or can be provided as discrete components or discrete collections of components.

[0065] Figures 2A_i-2D_i illustrate various features, components, and arrangements that can be included in some embodiments of the fluid transfer device 30 and fluid transfer module 31 shown in Figure 1A and the fluid transfer management system 74 shown in Figure 1B. As will be described in more detail below, Figure 2A_i illustrates an example of an electromechanical system 200 (also referred to as a fluid transfer unit 200); Figure 2B_i illustrates an example of a fluid transfer module 31 in the form in this example of a fluid pump assembly 224; Figure 2C_i illustrates the fluid pump assembly 224 of Figure 2B_i removably attached to the fluid transfer unit 200 of Figure 2A_i; and Figure 2D_i illustrates an example of a portion of an electro-mechanical controller 36 in the form in this example of a driver 212. Unless otherwise noted, like reference numerals among Figures 2A_i-2D_i indicate identical or functionally and/or structurally similar elements, and reference numerals in the below discussion corresponding to elements labeled in Figures 1A and 1B refer to elements that are the same as or generally similar to the elements of Figures 1A and 1B.

[0066] Turning to Figure 2A_i, this figure illustrates an example of a portion of a fluid transfer management system 74 with a remote user interface 78. For example, in some embodiments, Figure 2A_i illustrates a front perspective view of a fluid transfer unit 200 for transferring medical fluid. In some embodiments, the fluid transfer unit 200 is an example of a portion of the fluid transfer device 30 shown in Figure 1A or the fluid transfer system 86 shown in Figure 1B. As shown in the figures, the fluid transfer management system 74 can comprise a fluid transfer unit 200 that comprises a housing 202, one or more carrying handles 208, one or more base supports 223, a destination-container support (e.g., a generally vertical pole stand 204 and/or a generally horizontal support arm 242), and one or more supports configured to receive and retain at least a portion of the fluid transfer module 31 (e.g., the intermediate container or pumping region 40). In some embodiments, the supports can include one or more protruding holders 220, one or more receptacles 218 (such as a recess 218, as illustrated); one or more sensor devices 214 with one or more channels that include one or more sensors 215; one or more movable platforms 222 for receiving at least a portion of the fluid transfer module 31 and/or for facilitating the transfer of fluid; and/or one or more attachment regions 210 for attaching to or receiving a multidirectional flow-control

valve 41. As will be described in more detail below, the fluid transfer device 30 or the fluid transfer unit 200 can include a driver 212, which can form part of the electro-mechanical controller 36 of Figure 1A, and the one or more sensor devices 214 can include one or more indicators 216. The one or more base supports 223 can be attached to or integrally formed with the housing 202 to help stabilize the fluid transfer unit 200 (e.g., to help prevent it from tipping over). Although not shown in Figure 2A_i, in some embodiments, the one or more base supports 223 can extend across an underside of the housing 202.

[0067] In some embodiments, at least one or more portions of the housing 202, such as the one or more receptacles 218 (e.g., the recess 218 illustrated in Figure 2A_i), can be transparent to enable one or more measuring instruments positioned inside of the housing 202 to capture an image or other data on the outside of the housing. For example, a volume sensor (see Figure 2E_{ii}) can determine the volume of liquid being transferred to one or more containers (e.g., source container 39, intermediate container or pumping region 40, and/or destination container 44). For example, in some embodiments, the volume sensor can be configured to sense the volume in the intermediate container or pumping region 40 through the transparent recess 218. It will be understood that this same volume sensor or one or more other volume sensors can be configured to sense the volume of one or more other containers in addition to or in lieu of the intermediate container or pumping region 40 (e.g., the source container 39 and/or the destination container 44, among others), for example, through one or more transparent receptacles 218 and/or through one or more other sections of the housing 202 that are transparent. The volume sensor can comprise, for example, any appropriate sensor or combination of sensors to provide information about the volume of the liquid in a container, such as an optical sensor (e.g., a camera or a break-beam sensor), an infrared sensor, an acoustic sensor (e.g., an ultrasonic sensor), and/or a mass or weight sensor, among others.

[0068] The volume sensor can be used, for example, to control and/or to provide a record of the volume and/or type of fluid transferred to a patient, such as, for example, by sensing and/or recording the volume and/or one or more other characteristics (e.g., color, viscosity, concentration, lot number, expiration date, etc.) of the liquid in a container (e.g., the intermediate container, or pumping region 40, and/or the source container 39 and/or the destination container 44) before, during, and/or after it is transferred to a patient. For

example, in some embodiments, a camera can be used to capture an image of the intermediate container or pumping region 40 to confirm or measure the volume therein. A data file can then be created and stored in a memory 84 which has one of more items of information, such as patient identifying information, the date and time the liquid was transferred and/or the volume or other characteristic(s) of the liquid was or were confirmed and recorded, the type (name, brand, and/or concentration, etc.) of medical fluid transferred, the volume of medical fluid transferred, and/or one or more images of the intermediate container or pumping region 40 with liquid inside, etc. The same or a similar data file can be created for any one of the suitable volume sensors described above. In some embodiments, the fluid transfer unit 200, the fluid transfer device 30, and/or the fluid transfer system 86 can include one or more measuring instruments, such as one or more volume sensors. In some embodiments, the one or more measuring instruments or volume sensors can be internal and/or external to the fluid transfer unit 220, or partially external and partially internal, such as when a portion of the instrument or sensor is inside of the housing 212 and a portion of the sensor protrudes from the housing 212.

[0069] Figure 2B_i illustrates a rear view of an example of a fluid transfer module 31 of Figure 1A in the form in this example of a fluid pump assembly 224, such as a multi-stroke fluid pump assembly 224. As shown in the figures, in some embodiments, the fluid pump assembly 224 comprises: an inlet fluid connector 32 in the form in this example of a conduit 232 and a selectively openable and closeable fluid connector 226; a multidirectional flow-control valve 41 in the form in this example of a fluid stopcock 230; an outlet fluid connector 42 in the form in this example of a conduit 236 and a selectively openable and closeable fluid connector 234; and an intermediate container 40 in the form in this example of a syringe pump 240 that is attached (e.g., bonded) to the fluid stopcock 230 via a conduit 238. The fluid pump assembly 224 can be a limited-use or single-use, disposable device that is configured to be routinely removed, discarded, and replaced with a new disposable device in position on the fluid transfer unit 200.

[0070] A multidirectional flow-control valve 41, such as a fluid stopcock 230, can be particularly useful in some embodiments because it can permit variability and control of the direction and/or orientation of the fluid pathway within the fluid transfer module 31. In some embodiments, the flow-control valve 41 can be configured, as illustrated throughout

this specification, to selectively enable a plurality of discrete settings, each setting enabling fluid connections within the fluid pathway of the fluid transfer module 31 among two or more different components of the fluid transfer module 31, and closing-off or isolating one or more other fluid connections of one or more other components from the fluid pathway of the fluid transfer module 31. The flow-control valve 41 can be configured to change between the plurality of discrete settings.

[0071] In some embodiments, as illustrated, such change or changes of settings or connections within the flow-control valve 41 can be accomplished electronically and independently of changes to fluid pressure within the fluid transfer module 31. For example, in some embodiments, a pressure differential can arise between two or more parts or components of the fluid transfer module 31 without causing any change of connections within the fluid transfer module 31 and/or without enabling fluid communication between different portions of the fluid transfer module 31 that, before such pressure differential, were not previously in fluid communication with each other.

[0072] In some embodiments, the multidirectional flow-control valve 41 is not a one-way valve or a series of one-way valves; rather, the multidirectional flow-control valve 41, in each particular electronically selectable setting, can provide a full two-way fluid pathway between two or more components of the fluid transfer module 31. For example, in some embodiments, in one or a plurality of discrete, electronically selectable settings, the flow-control valve 41 can provide a two-way fluid pathway between the inlet fluid connector 226 and the outlet fluid connector 234; and/or a two-way fluid pathway between the inlet fluid connector 226 and the intermediate container 40 or syringe pump 240; and/or a two-way fluid pathway between the intermediate container 40 or syringe pump 240 and the outlet fluid connector 234. In some embodiments, the multidirectional flow-control valve 41 can enable fluid withdrawn from a source container 39 to be partially or fully returned to a source container 39, in some situations, which can be particularly advantageous, such as, for example, during priming and/or purging of a fluid transfer module 31, although other situations in which this type of fluid flow are also contemplated and can be used.

[0073] In some embodiments, either or both of the fluid connectors 226, 234 can be industry standard medical connectors (e.g., luer connectors compliant with ISO 594 or compliant with any other industry standard) that are resealable and fluid-tight, such as the

Clave® female medical connector or the Spiros® male medical connector or either of the male or female sides of a Chemolock® medical connector system, all sold by ICU Medical, Inc. Examples of embodiments of these and other devices, among many others, that can be used as fluid connectors 226, 234, or as any portions thereof, are included in U.S. Patent No. 5,873,862; U.S. Patent No. 7,998,134; and U.S. Published Patent Application No. 2014/0246616, all of which are incorporated by reference in this specification in their entireties. Any feature, structure, material, step, or component described and/or illustrated in any of the foregoing patents or published application can be used with or instead of any feature, structure, material, step, or component described and/or illustrated in any other portion of this specification.

[0074] In some embodiments, the fluid stopcock 230 can comprise a device that selectively permits fluid communication between and/or among multiple apertures and/or channels in the stopcock 230. For example, as shown in Figure 2B_i and as described above, the fluid stopcock 230 can selectively permit fluid communication between any two of the inlet fluid connector 226, the outlet fluid connector 234, and the intermediate container 40 or syringe pump 240. The selection between and/or among the multiple apertures and/or channels in the stopcock 230 can be accomplished by actuating the stopcock 230, such as by utilizing an electromechanical controller 36 in the fluid transfer unit 200 to actuate a driving interface 33 on the stopcock 230, such as in the form in this example of a rotatable actuator 228. As described above, the electromechanical controller 36 can be controlled by sending one electronic signal or a series of electronic signals from one or more computer processors associated with the fluid transfer device 30. As shown in Figure 2B_i, the rotatable actuator 228 can include one or more recesses and/or protrusions that are configured to interface with a driver 212 of a fluid transfer unit, such as a driver 212 that includes one or more recesses and/or protrusions that comprise one or more shapes that are complementary with or generally match or correspond with the recesses and/or protrusions of the actuator 228. The driver 212 may be controlled via a driver motor and driver shaft. The electromechanical controller 36 may send a signal activating driver motor and driver shaft to initiate driver 212 movement, and/or to continue and/or stop driver 212 movement. When a rotatable actuator interfaces with the driver 212, the driver 212 may allow the electromechanical controller to select between and/or among the multiple apertures and/or

channels in the stopcock 230. As in every embodiment in this specification, any component, structure, feature, or step that is illustrated and/or described in connection with Figure 2Eii (including the internal components) can be used with or instead of any component, structure, feature, or step that is illustrated and/or described in connection with any other figure or embodiment in this specification.

[0075] Figure 2D_i is a magnified partial front view of the fluid transfer unit 200 of Figure 2A_i, which illustrates an attachment region 210 and the recesses and/or protrusions of the driver 212, according to some embodiments. However, it will be understood that many different types and/or patterns of recesses and/or protrusions can be used, depending, for example, upon functional and aesthetic preferences. In some embodiments, one or more of the types and/or patterns of recesses and/or protrusions, and/or one or more of the types of materials (such as a tacky or slide-resistant material with a high coefficient of friction) can provide resistance to rotational disengagement or slipping during actuation.

[0076] Returning to Figure 2B_i, this figure also illustrates an example of a syringe pump 240. In some embodiments, the syringe pump 240 includes an actuator, such as an actuating stem 241, that can be reciprocated back-and-forth or up-and-down to move an internal plunger, thereby decreasing or increasing the fluid-carrying volume inside of the syringe pump 240. A first stroke of the multi-stroke fluid pump assembly 224 in the form in this example of a syringe pump 240 can be accomplished by drawing the actuating stem 241 at least partially out of the body of the syringe pump 240, thereby drawing fluid into the syringe pump 240, and then reversing the direction of the syringe pump 240, pushing the actuating stem 241 back toward the body of the syringe pump 240, thereby expelling the drawn-in fluid out of the syringe pump 240.

[0077] In some embodiments, as shown, for example, in Figure 2B_i, the conduit 238 of the multi-stroke pump assembly 224 can be longer than the conduits 232, 236 extending between the fluid stopcock 230 and the fluid connectors 226, 235. The conduit 238 can be permanently coupled to the fluid stopcock 230 on one end, and to the syringe pump 240 on the other end. Other arrangements are also contemplated and can be used.

[0078] As illustrated, in some embodiments, the fluid transfer module 31 (such as the fluid pump assembly 224) can form part of or constitute a closed system, in that: (i) liquid, or fluid, and/or vapors contained or sealed within the fluid transfer module 31 are

prevented from exiting or escaping from the fluid transfer module 31, and/or (ii) the exiting or escaping of liquid, or fluid, and/or vapors is resisted in a clinically significant manner to diminish or avoid one or more clinical risks or negative outcomes, when the fluid transfer module 31 is disconnected from other components of the fluid transfer device 30. As shown, in some embodiments, the entire fluid pathway within the fluid transfer device 30 can constitute a closed system or a seal system. As used in this specification, the term “closed system” or “sealed” or any similar terms are used in accordance with their customary meanings in the field of medical infusion, and these terms include the requirement that fluids stay inside of the fluid transfer module 31 or the fluid transfer device 30 (or components thereof) under normal conditions or use such that any small amount of escaping fluid or vapors would not have any significant adverse clinical effects under normal conditions or use. In some embodiments, as shown in Figures 1A and 2B_i, the fluid transfer module 31 can be automatically closeable and resealable at each terminal end of the module 31 (e.g., at the inlet fluid connector 32, at the intermediate fluid connector 38, and/or at the outlet fluid connector 42). When either or both of the fluid transfer module 31 and/or the fluid transfer device 30 are sealed and/or constitute part of a closed system, the risk of ingress of harmful substances (e.g., bacteria or viruses or other microbes) into the fluid pathway is diminished, and the risk of egress of harmful substances (e.g., chemotherapy or immunosuppressive drugs) from the fluid transfer device 30 or the fluid transfer module 31 into the surrounding environment of a healthcare facility is diminished.

[0079] Figure 2C_i is a front perspective view of another type of fluid transfer module 31 that is removably attached to the fluid transfer unit 200 of Figure 2A_i. The fluid transfer module 31 is identical to the fluid pump assembly 224 of Figure 2B_i, except that Chemolock connectors 234a, 226a are used rather than Spiros connectors, in this example. Any suitable type of connector or combination of connectors can be used. As illustrated in Figure 2C_i, the fluid transfer module 31 (also referred to as a multi-stroke fluid pump assembly 224) can be removably attached to the fluid transfer unit 200, such as by using one or more of the supports on the fluid transfer unit 200. For example, as shown in Figure 2C_i, a flat portion or end of the actuating stem 241 can be inserted into or coupled with a receiving region of the movable platform 222; one or more tabs on the syringe pump 240 can be positioned on or inserted between one or more of the protruding holders 220; the body of the

syringe pump 240 can be received in the receptacle 218; the conduit 238 can be inserted into or on the sensor device 214, such as in a channel within the sensor device 214 that includes one or more sensors 215 (also referred to as one or more sensing regions 215; and/or the body of the fluid stopcock 230 can be positioned in or on or inserted into the attachment region 210 of the fluid transfer unit 200. In some embodiments, the fluid transfer device 30, such as in the form in this example of a multi-stroke fluid pump assembly 224, can be attached to the fluid transfer unit 200 in a single motion by simply advancing the transfer device 30 into contact with a face on the fluid transfer unit 200 that includes one or more of the supports 220. The fluid transfer device 30 can be removably retained on the fluid transfer unit 200 by any suitable attachment structure, including a snap-fit, a friction fit, a clasp, a clip, a retaining arm or door, an elastic band, or any other attachment structure.

[0080] When the fluid transfer module 31 (e.g., the fluid pump assembly 224) is removably attached to the fluid transfer unit 200, a fluid-observation region on the conduit 238 of the fluid transfer device 30 can be positioned adjacent to or within an appropriate sensing distance from the one or more sensors 215. In the illustrated example, the fluid-observation region of the fluid transfer device 30 is at least a portion of the conduit 238 positioned between the multidirectional flow-control valve 41 (e.g., the fluid stopcock 230) and/or the intermediate container or pumping region 40 (e.g., the syringe pump 240). In some embodiments, the fluid-observation region of the fluid transfer device 30 can comprise a portion of the conduit 238 positioned between the multidirectional flow-control valve 41 (e.g., the fluid stopcock 230) and/or the intermediate container or pumping region 40 (e.g., the syringe pump 240). In some embodiments, the fluid-observation region can be positioned in another position on the fluid transfer device 30, or there can be multiple fluid-observation regions 30 located at a plurality of positions on the fluid transfer device 30.

[0081] In some embodiments, the one or more sensors 215 can be configured to determine whether there is liquid, gas (e.g., one or more bubbles), and/or a vacuum or partial vacuum, within a particular region or regions of the fluid transfer module 31 (e.g., fluid pump assembly 224). For example, as illustrated in the figures, the one or more sensors 215 can be configured to determine whether there is a medical fluid within at least a portion of the conduit 238 or whether there is a gas (e.g., ambient air or air bubbles) or a vacuum or partial vacuum within the conduit 238. In some embodiments, the one or more sensors 215

can determine whether there is a medical fluid within a portion of the conduit 238 or whether there is a gas (e.g., ambient air) or a vacuum or partial vacuum within a portion of the conduit 238. The one or more sensors 215 can be any suitable type of sensor, including but not limited to one or more acoustic sensors (e.g., ultrasonic sensors), infrared sensors, laser sensors, visual-spectrum optical sensors, motion flow sensors, or any other suitable sensors. One or more indicators 216, such as an indicator light or indicator speaker or other indicator, can be positioned on the sensor device 214 to indicate when the sensor device 214 is sensing a particular condition, such as when liquid is present in the fluid observation-region.

[0082] Figure 2C_i also illustrates a fluid source container 39 in the form in this example of an inverted vial 246 attached to a vial adaptor 248 that is in turn attached to an inlet connector 32 in the form in this example of a male fluid connector 226a with a longitudinal locking mechanism. In some embodiments, the vial adaptor 248 comprises a filtered fluid inlet and/or outlet 250 and securing arms that are configured to securely receive the vial. Figure 2C_i also illustrates a fluid destination container 44 in the form in this example of an IV bag 244 attached to a conduit or hose 252 (in this example by way of a bag spike 254 or other fluid connection point) that is in turn attached to the outlet connector 42 of the fluid transfer module 31. The outlet connector in Figure 2C_i is in the form in this example of a male fluid connector 234a with a longitudinal locking mechanism. The IV bag 244 is suspended from the pole stand 204 by the support arm 242.

[0083] Figures 2A_{ii}-2D_{ii} illustrate various features, components, and arrangements that can be included in some embodiments of the fluid transfer device 30 shown in Figure 1A and the fluid transfer system 86 shown in Figure 1B. Similar to Figures 2A_i-2D_i, Figure 2A_{ii} illustrates an example of an electromechanical system 200 (also referred to as a fluid transfer unit 200), Figure 2B_{ii} illustrates an example of a fluid transfer module 31 in the form in this example of a fluid pump assembly 224; Figure 2C_{ii} illustrates the fluid pump assembly 224 of Figure 2B_{ii} removably attached to the fluid transfer unit 200 of Figure 2A_{ii}; and Figure 2D_{ii} illustrates an example of a driver 212. Unless otherwise noted, reference numerals in Figures 2A_{ii}-2D_{ii} refer to elements that are the same as or generally similar to the components of Figures 1A-2D_i. For example, the fluid transfer unit 200 of Figure 2A_{ii} is generally similar to the fluid transfer unit 200 shown in Figure 2A_i, except that the one or more base supports 223 extend across an underside of the housing 202 at base

support region 223a. Figure 2A_{ii} also illustrates one or more trays 280 attached to the housing 202 configured to support one or more containers and/or conduits described and contemplated herein. The one or more trays 280 may comprise any one of various structures to support containers and/or conduits. For example, in some embodiments, the one or more trays 280 may comprise one or more racks with one or more slots capable of holding vials. In some embodiments, the one or more trays 280 may be configured to support a source bag and/or an IV bag, such as a saline or diluent bag and/or a bag containing therapeutic or medicinal liquid. The one or more trays 280 may be removably attached to the housing 202. In some embodiments, one tray 280 can be configured to support a saline or diluent source container and another tray 280 can be configured to support a source container with therapeutic or medicinal liquid. Among other structural differences, the supports 220 in Figure 2A_{ii} are shaped differently from those shown in Figure 2A_i, albeit their function is the same or similar. As with all embodiments in this specification, any feature, structure, material, step, or component of any embodiment described and/or illustrated in connection with Figures 2A_i-2D_i can be used by itself, or with or instead of any other feature, structure, material, step, or component of any other embodiment described and/or illustrated in connection with Figures 2A_{ii}-2E_{ii}.

[0084] As another example, Figures 2B_{ii} and 2C_{ii} also illustrate an example of a stopcock handle 245. In particular, Figure 2B_{ii} illustrates a rear view of the stopcock handle 245 attached to the fluid pump assembly 224 and Figure 2C_{ii} illustrates a front perspective view of the stopcock handle 245 attached to the fluid pump assembly 224 and removably attached to the fluid transfer unit 200. In some embodiments, the stopcock handle 245 comprises an aid for grasping the fluid pump assembly and/or positioning the fluid pump assembly 224 relative to the fluid transfer unit 200. For example, in some embodiments, the stopcock handle 245 can be configured to help position (e.g., attach, engage, remove, and/or disengage) the fluid pump assembly 224 to and/or from one or more features of the fluid transfer unit 200. The stopcock handle 245 can, for example, help engage or disengage the rotatable actuator 228 to or from the driver 212, help push the conduit 238 into or on the sensor device 214, help remove the conduit 238 from the sensor device 214, help attach or remove the actuating stem 246 to or from the receiving region of the movable platform 222, help position the one or more tabs on the syringe pump 240 on or between one or more of the

protruding holders 220, help position the body of the syringe pump 240 into the one or more receptacles 218, and/or help position the body of the stopcock 230 into or on the attachment region 210, among any other suitable uses.

[0085] In some embodiments, the stopcock handle 245 can be removably attached to the stopcock 230. In some embodiments, the handle is configured to be manipulated (e.g., rotated, slid, pushed, and/or pulled) to manually actuate the stopcock into the various positions described above with reference to, for example, Figure 1A. It will be understood that the stopcock handle 245 can be utilized in any embodiment illustrated and contemplated herein, including, for example, the embodiments shown in Figures 1A, 1B, and 2A_i-2D_i.

[0086] Figure 2E_{ii} is a rear perspective cross-sectional view of the fluid transfer unit 200 and the fluid pump assembly 224 shown in Figure 2C_{ii}, and illustrates various internal and external functional components. For example, as shown in Figure 2E_{ii}, in some embodiments, a measuring instrument such as a sensor 225 (e.g., a camera) can be positioned within the housing 202 to determine one or more features of the contents of the fluid transfer module 31 or fluid pump assembly 224, such as the volume, or type, or concentration, or color, and/or viscosity of fluid in the intermediate container or pumping region 40 (e.g., by capturing an image of the fluid transfer module 31 or fluid pump assembly 224) to provide a data file as described above. In some embodiments, a shroud 255 can be positioned adjacent to or near or generally around the one or more transparent receptacles 218 to advantageously resist the entry of undesired light from aberrant sources in order to increase the accuracy of the sensor 225. For example, in some embodiments, the shroud 255 can be configured to direct light that passes through the one or more transparent receptacles 218 toward the sensor 225, thereby increasing the amount of light available to the sensor 225. When the sensor 225 is a camera, the shroud 255 can help make the images more accurate and easier and faster to process by the processor(s) of the fluid transfer unit 200.

[0087] The fluid transfer unit 200 may comprise one or more computer processors 297, 298, which can form part of or be in electronic communication with any or all of the electro-mechanical controller 36 of Figure 1A, the sensor 214, the volume sensor 225, the stopcock motor 290, and/or the platform motor 296, etc. in some embodiments, the one or more computer processors 297, 298 may comprise a pi box and/or a control board. The fluid transfer unit 200 may contain or support a power supply 295 configured to provide

power to one or more components of the fluid transfer unit 200. The housing 202 may comprise a seal 293 configured to resist or prevent the entrance into and/or escape of fluid from the housing 202.

[0088] In some embodiments, the fluid transfer unit 200 may comprise one or more presence sensors 294a, 294b, 294c. The one or more sensors 294a, 294b, 294c can be positioned within and/or on the housing 202 and can determine the presence or absence of one or more structures. In some embodiments, one or more of the sensors 294a, 294b, 294c can be infrared sensors or any other suitable sensor. One or more of the sensors 294a, 294b can determine whether the fluid source container 39 (such as vial 246), the source adapter 250, and/or the source fluid connector are present and/or connected to the fluid transfer unit 200. In some embodiments, sensor 294a may determine if a source container 246 connector, such as a male or female side of a Chemolock® medical connector system, is properly engaged with a corresponding connector on the fluid transfer unit 200, such as a Chemolock® connector 226a. The sensor 294b may determine if an intermediate container 40, such as fluid pump assembly 224, and/or connector 226a, such as a male or female side of a Chemolock® connector, is present and/or properly engaged with the housing 202 and/or a corresponding connector on a source container 246. The sensor 294c may determine whether the destination container 44, such as IV bag 244, and/or destination fluid connector are present and/or connected to the fluid transfer unit 200. In some embodiments, sensor 294c may determine if a destination container 44 connector, such as a male or female side of a Chemolock® medical connector system, is properly engaged with a corresponding connector on the fluid transfer unit 200, such as a Chemolock® connector 234a. In some embodiments, if any of sensor 294a, 294b, 294c determine that a component of the fluid transfer unit 200 is not present, the sensor 294a, 294b, 294c may send a signal to the controller 36 to prevent initiation of the fluid transfer process and/or terminate an ongoing fluid transfer. The sensor 294a, 294b, 294c may trigger an indicator signaling to a user that not all components are present or properly engaged with the fluid transfer unit 200.

[0089] As shown in Figures 2Ai, 2Aii, and 2Cii, in some embodiments, one or more apertures in the housing can permit one or more of the presence sensors 294a, 294b, 294c to communicate essentially or completely unimpeded from within the housing to a region outside of the housing. As illustrated, one or more of the presence sensors 294a,

294b, 294c can be positioned in substantially a collinear manner with each other and/or with the primary longitudinal axis of the fluid transfer module 31 (e.g., presence sensors 294a, 294b), and/or one or more other of the presence sensors 294a, 294b, 294c can be positioned in a non-collinear manner or at an angle or perpendicular to the primary longitudinal axis of the fluid transfer module 31 (e.g., presence sensor 294c). In some embodiments, as shown, one or more or all of the sensors are positioned and/or recessed inside of the housing of the electronic fluid transfer system, such that a panel through which the sensors are configured to detect items is essentially or substantially or entirely planar. As illustrated, one or more of the sensors does not include and/or is not attached by any external wires outside of the housing of the electronic fluid transfer system.

[0090] In some embodiments, one or more of the sensors 294a, 294b, 294c can be configured to detect the presence or absence of at least a portion of a fluid transfer module attached to the electronic fluid transfer device, such as a connector on the fluid transfer device. In some embodiments, one or more of the sensors (e.g., 294a, 294b) can be configured to additionally or alternatively detect the presence or absence of or connection with at least a portion of a fluid source system, such as a connector or vial adaptor or vial or bag or conduit that forms part of or is connected to a fluid source system. In some embodiments, one or more of the sensors (e.g., 294c) can be configured to additionally or alternatively detect the presence or absence of or connection with at least a portion of a fluid destination system, such as a connector or bag or conduit that forms part of or is connected to a fluid destination system. In some embodiments, the detection of one or more of the fluid transfer module 31, the detection of the connection to the fluid source system, and/or the detection to the connection to the fluid destination system can be a gating step or a required step for the computer processor or other component of the electro-mechanical controller to permit fluid transfer to begin or continue.

[0091] Figure 3 illustrates a user interface 78 that can be used with the fluid transfer unit 200 in the form in this example of a remote tablet. The user interface 78 can comprise a rechargeable internal battery, a touch-sensitive screen to enable user selection and input by way of the screen, and one or more additional or alternative user inputs 256, such as a button (as shown) or a knob or a slider or a rocking switch, or a rolling dial, or any other user input. The user interface 78 can communicate electronically with one or more fluid

transfer units 200 and/or with one or more patient and/or drug information storage devices or networks 70 utilizing any suitable electronic protocols or electronic communicators. In some embodiments, the user interface 78 is fixed to the fluid transfer unit 200, such as being attached to or contained at least partially within the housing of the fluid transfer unit 200.

[0092] The user interface 78 can display or convey various items of information between a user and an electronic storage medium and/or can convey one or more executable instructions to a computer processor in the fluid transfer unit 200, or to electromechanical hardware in the fluid transfer unit 200, to perform one or more actions relating to fluid transfer. For example, the user interface 78 can receive and/or store (e.g., by user input or electronic transmission) the identity of the pharmacist or technician who is performing the fluid transfer, the identity of the patient, the name of the medical fluid, the volume of medical fluid to be transferred, the lot number, the expiration date of the medical fluid, and/or the date and time on which the fluid transfer was performed, etc. Also, as other examples, the user interface 78 can assist in controlling the fluid transfer by receiving and conveying commands from the user via the user interface 78 and/or displaying messages from the fluid transfer unit 200 regarding the progress and/or status of the fluid transfer, such as commands initiating the fluid transfer and/or halting the fluid transfer, and/or one or more messages demonstrating the amount of fluid transferred at any given moment, or the history of fluid transfers for a particular patient or pharmacist over a particular period, or one or more error messages indicating that the fluid transfer was not completed or that the fluid source container 39 is not connected or is empty, or the fluid destination container 44 is not connected or is full, or any other useful message.

[0093] As shown in Figure 4, in some embodiments, the user interface 78 can be universally compatible with a plurality of different fluid transfer devices 30 and a plurality of different types of fluid transfer devices 30. For example, a single user interface 78 can be configured to electronically communicate with (e.g., by transferring data to and/or from) a plurality of different fluid transfer devices 30 of the same type, or a plurality of different fluid transfer devices 30 of a different type, that are performing separate fluid transfer operations, such as filling destination containers with a plurality of different therapeutic fluids and/or for a plurality of different patients. The user interface 78 can be configured to simultaneously or generally concurrently control and/or record information from any or a

plurality or all of such operations. The user interface 78 can comprise a plurality of different communication capabilities, including a plurality of different electronic communicators and/or a plurality of different communication protocols for use with any of such electronic communicators. The user interface 78 can be updated electronically to enable it to communicate electronically using protocols that are not originally used or installed on the user interface, which can enable the user interface 78 to become compatible with future or different types of fluid transfer devices 30, without requiring replacement of the fundamental components of the electronic communication system.

[0094] Figures 5A-5C are various schematics of fluid transfer modules 45, according to some embodiments. Figure 5A is a schematic of a fluid transfer module 45 having a bubble trap 15 in fluid communication with a source container 39. Figure 5B is a schematic of the fluid transfer module 45 of Figure 5A disconnected from the source container 39 and in fluid communication with a patient 70. Figure 5C is a schematic of a fluid transfer module 45 having a bubble trap 15 in fluid communication with the fluid transfer module 31 of Figure 1A. Unless otherwise noted, reference numerals in Figures 5A-5C refer to components that are the same as or generally similar to the components in the preceding figures.

[0095] As shown in Figure 5A, the fluid transfer module 45 can include a bubble trap 15 and a destination container 44 in fluid communication with a source container 39. The destination and source containers 44, 39 can comprise any suitable container as described above with reference to Figure 1A. For example, in some embodiments, the source container 39 can be a vial or a syringe and the destination container 44 can be an IV bag or a cassette reservoir (e.g., a CADD® cassette reservoir). Although not shown in Figure 5A, the bubble trap 15 can be connected to the destination and source containers 44, 39 with any suitable connector or arrangement of connectors. For example, an inlet of the bubble trap 15 can be configured to attach to a needlessly connector (e.g., a NEUTRON CLAVE® connector, a MICROCLAVE® Neutral Displacement connector, and the like) and the opposite end of the needlessly connector can be configured to attach to, for example, a syringe. As another example, an outlet of the bubble trap 15 can be configured to attach to, for example, an open female hub at the end of a fluid line of a CADD® cassette. It will be appreciated that the

open female hub can be any closed connector (luer or not), including, for example, a CLAVE® connector, among others.

[0096] In some embodiments, the bubble trap 15 can be provided as an adapter to be coupled to a container (e.g., the destination and source containers 44, 39). For example, in some embodiments, the bubble trap 15 can be provided in a package with a container. For example, in some embodiments, the bubble trap 15 can be provided in a package with a syringe, with a cassette, with a fluid bag, with a fluid line, etc. It will be appreciated that the package can include more or less components, assembled or disassembled.

[0097] With further reference to Figure 5A, medical fluid can be transferred from the source container 39, through the bubble trap 15, and into the destination container 44. Because the source container 39 and various components of the fluid module 45 (e.g., connectors and fluid lines) often contain gas (e.g., air), when medical fluid is transferred from the source container 39, gas is often transferred as well, either from the source container 39 or from one of the various components along the way. However, the presence of gas is undesirable in the destination container 44 as it poses a risk to the patient if it ever enters their blood stream (e.g., air embolisms can cause medical complications ranging from discomfort to death). As a result, considerable effort is typically spent manually removing all of the gas from the destination container 44 before it is fluidically connected to a patient. Advantageously, the bubble trap 15 in Figure 5A can be configured to prevent or otherwise inhibit the flow of gas into the destination container 44. As will be described in more detail below, the bubble trap 15 can be configured to both capture gas and allow liquid to flow through.

[0098] In some embodiments, once the destination container 44 is filled with fluid, the fluid transfer module 45 can be disconnected from the fluid source 39 and then connected to a patient. For example, Figure 5B is an example schematic of the fluid transfer module 45 of Figure 5A disconnected from the source container 39 and in fluid communication with a patient 70. The source container 39 is shown disconnected from the fluid transfer module 45. It will be appreciated that the destination container 44 in Figure 5B is acting as a source container and that its name was not adjusted to reflect this so that modularity of the fluid transfer module 45 could be emphasized and illustrated. In Figure 5B, the bubble trap 15 can be configured to trap (also referred to as capture) air that is

discharged from the destination container 44 or fluid lines before it reaches the patient. Although not shown in Figure 5B, in some embodiments an air detection system can be positioned between the bubble trap 15 and the patient 70 to sound an alarm and/or stop the transfer of fluid if it detects gas or a bubble.

[0099] Figure 5C is a schematic of a fluid transfer module 45 having a bubble trap 15 in fluid communication with the fluid transfer module 31 of Figure 1A. In some embodiments, the fluid transfer module 45 can be removably attached to the fluid transfer module 31 such that the fluid transfer module 45 can be connected to a patient as shown, for example, in Figure 5B.

[0100] Figures 6A-6C are various schematics of bubble traps 15, according to some embodiments. Figure 6A is a schematic of a bubble trap 15 having an elongated chamber 17 and an outlet projection 18. Figure 6A' is a schematic of the bubble trap 15 of Figure 6A with inlet and outlet luer connectors 20a, 20b. Figure 6B is a schematic of a bubble trap 15 having a curved chamber 17 and an outlet projection 18. Figure 6C is a schematic of a bubble trap 15 having a curved chamber 17 and inlet and outlet projections 12, 18. Unless otherwise noted, reference numerals in Figures 6A-6C refer to components that are the same as or generally similar to the components in the preceding figures.

[0101] As shown in Fig. 6A, the bubble trap 15 can include an inlet 16a, an outlet 16b, and a chamber 17. The chamber 17 can include one or more flow paths between the inlet 16a and the outlet 16b. In some embodiments, the inlet 16a and the outlet 16b can be positioned on opposite ends of the chamber 17, although any suitable arrangement is appreciated (e.g., on the same side, etc.). In some embodiments, the chamber 17 can be configured to trap gas (e.g., air) that flows in from the inlet 16a. To help trap air that flows into the chamber 17, the inlet 16a and/or outlet 16b can include one or more projections that extend into the chamber 17. This can advantageously position an opening of the inlet 16a and/or the outlet 16b away from a wall of the chamber where bubbles typically come to rest and/or accumulate during flow. In this way, the bubble trap 15 can be configured to trap air by confining it to a peripheral region of the chamber 17.

[0102] As shown in Figure 6A, the trap 15 can include an outlet projection 18, including, for example, an outlet projection channel 19 in fluid communication with the outlet 16b. In such embodiments, the bubble trap 15 can define a flow path in which fluid

can be forced to flow through the chamber 17 and the outlet projection channel 19 before it reaches and flows past the outlet 16b. In some embodiments, the one or more projections (e.g., projection 18) can be configured to inhibit bubbles from flowing directly from the inlet 16a to the outlet 16b. Since air tends to move upward against the force of gravity when in a liquid, bubbles tend to move toward the perimeter of the chamber 17 regardless of the bubble trap's orientation during flow. Advantageously, when the outlet 16b is positioned away from the periphery of the chamber 17, such as, for example, via the outlet projection 18, the bubble trap 15 can become an omnidirectional trap such that it is configured to trap air in the chamber 17 regardless of its orientation with respect to fluid flow or frame of reference (e.g., a neutral position). Although the projection channel is discussed herein and illustrated as being in fluid communication with the outlet 16a, it will be understood that any projection channel discussed herein may be an inlet projection channel in fluid communication with the inlet 16a

[0103] In some embodiments, the one or more projections can be configured to maximize the air trapping ability and/or capability of the chamber 17. For example, in some embodiments, one or more projections (e.g., projection 18) can be positioned so that the opening 16c of the outlet projection channel 19 is near or in the center of the chamber 17. This can advantageously minimize the chance of air (e.g., one or more air bubbles) entering the outlet 16b after it comes to rest somewhere along the periphery of the chamber 17. In some embodiments, as shown in the drawings, the opening 16c of the outlet projection channel 19 may have an outlet center axis that is misaligned and/or offset from an inlet center axis of the inlet 16a. For example, as shown in the drawings, the opening 16c may have a center axis that is generally perpendicular to a plane defined by the opening 16c. In some embodiments, the center axis of the opening 16c may be offset from at least one of a center axis of the inlet 16a and a center axis of the outlet 16b. The opening 16c being misaligned from one or more of the inlet 16a and the outlet 16b breaks up a fluid pathway from the inlet 16a to the outlet 16b, thereby causing any air bubbles to rest along a periphery of the chamber 17. This may facilitate the collection of air within the bubble trap 15. As shown in Figure 6A, in some embodiments, the outlet projection channel 19 can have a curved region near the tip of the outlet projection 18 such that the opening 16c of the outlet projection channel 19 is on the side of the outlet projection 18. This can further reduce the

possibility of air entering the outlet projection channel 19 by removing all or the majority of direct paths from the inlet 16a to the opening 16c of the outlet projection channel 19, including, for example, the path that would otherwise exist from the inlet 16a to the outlet 16b in Figure 6A (e.g., straight up) if the outlet projection channel 19 was instead straight and opened on the tip of the outlet projection 18 facing the inlet 16a. It will be appreciated that the outlet projection channel 19 can extend any suitable distance into the outlet projection 18 and that the curved region can be positioned along any suitable portion thereof.

[0104] In some embodiments, as shown in the drawings the opening 16c of the outlet projection channel 19 may be smaller relative to the inlet 16a of the bubble trap 15. The smaller size of the opening 16c can advantageously minimize that amount of air that is transferred through the outlet projection channel 19. The size of the opening 16c may increase the force required to push fluid into and/or through the outlet projection channel 19. The bubble trap 15 may be used with an automated compounder, as described herein, to drive fluid through the opening 16c of the bubble trap 15. However, it will be understood that the opening 16c of the bubble trap 15 may comprise any suitable size and/or shape to permit the transfer of fluid into and/or through the outlet projection channel 19. For example, the opening 16c of the outlet projection channel 19 may be configured to permit the transfer of fluid with the use of a manual compounder (e.g. a syringe). It will also be appreciated that the tips of the one or more projections (e.g., projection 18) can be configured to deflect bubbles that collide or otherwise come in close proximity to the outlet projection 18. It will be further appreciated that the shape of the one or more projections can have any suitable shape, such as, for example, straight, curved, cylindrical, tapered, conical (e.g., projection 18), etc. The flow of fluid and gas through the chamber 17 will be described in more detail below with reference to Figures 7A-7H.

[0105] The bubble trap 15 can have any suitable fluid capacity, or internal volume, including from about 1cc to about 2cc, from about 1cc to about 5cc, from about 1cc to about 10cc, greater than about 1cc, greater than about 2cc, and/or less than about 20cc, among others (e.g., from about 3cc to about 4cc, from about 5cc to about 10cc, etc.). Any suitable portion of this fluid capacity can be used to trap air, such as, for example, 10% or less of the capacity, 20% or less of the capacity, 30% or less of the capacity, 40% or less of the capacity, 50% or less of the capacity, 60% or less of the capacity, or 70% or less of the

capacity. Other percentages, more or less, as well as ranges, narrower or wider, are also appreciated. In some embodiments, the trapping capacity of the bubble trap 15 can be constant irrespective of the position of the bubble trap 15. In other embodiments, the trapping capacity of the bubble trap 15 can depend on myriad factors, such as the size and shape of the chamber 17, the length of the one or more projections and the locations of their openings, and/or the orientation of the bubble trap 15 with respect to fluid flow and gravity. For example, when in the orientation shown in Figure 6A, the bubble trap 15 can be configured to have a trap region that extends from the top surface of the chamber 17 downward to the opening 16c of the outlet projection channel 19. In some embodiments, this trap region can correspond to one of the aforementioned capacities, among others. The bubble trap 15 illustrated in Figure 6A can have the same or nearly the same capacity, for example, when it is rotated 90 degrees along any axis or combination axes, and/or when it is rotated any number of degrees along any combination of axes (e.g., one, two, and/or three axes). And in other embodiments, the bubble trap 15 illustrated in Figure 6A can have one or more different capacities, for example, when it is rotated 90 degrees along any axis or combination axes, and/or when it is rotated any number of degrees along any combination of axes (e.g., one, two, and/or three axes). Various trap capacities as a function of a bubble trap's orientation are illustrated in Figures 7A-7H and will be described below.

[0106] As a result of some or all of the foregoing features, the bubble trap 15 can trap bubbles released from a source container (e.g., source container 39), a destination container (e.g., destination container 44), and/or a component connected to a fluid line. As shown in Figure 6A, the chamber 17 provides a space for bubbles to collect and for liquid to flow through. As a result of this trapping capability, the bubble trap 15 can be used to advantageously reduce the risk of air embolisms, or at a minimum, reduce the frequency at which they occur. By inhibiting the flow of bubbles while permitting the flow of liquid, the bubble trap 15 can act as an air filter and filter air out of the flow path.

[0107] Figure 6A' is a schematic of the bubble trap 15 of Figure 6A with inlet and outlet luer connectors 20a, 20b. The male luer connector 20a can be any suitable male luer and the female luer connector 20b can be any suitable female luer. It will also be understood that, in some embodiments, any suitable arrangement of the male luer connector 20a and the female luer connector 20b is appreciated. For example, the bubble trap 15 may comprise a

male luer connector located at least one of the inlet 16a and the outlet 16b and a female luer connector located at least one of the inlet 16a and the outlet 16b. Figure 6B, as described above, is a schematic of a bubble trap 15 having an outlet projection 18 and a curved as opposed to elongated chamber 17. In Figure 6B, the inlet 16a and the outlet 16b are positioned on the same side of the housing 17 or otherwise in close proximity to one another such that the inlet 16a and the outlet 16b do not face or point toward each other. In such embodiments, the opening 16c of the outlet projection channel 19 can be positioned on the end of the outlet projection 18 without compromising the ability of the bubble trap 15 to trap air. In some embodiments, an inlet conduit 14a can be connected (e.g., attached, bonded, glued, welded, snapped, friction fit, removably attached, etc.) to the inlet 16a and an outlet conduit 14b can be connected to the outlet 16b.

[0108] Figure 6C is a schematic of a bubble trap 15 having a curved chamber 17 and inlet and outlet and inlet and outlet luer connectors 20a, 20b. As shown in Figure 6C, in some embodiments, the bubble trap 15 can include an inlet projection 12 having an inlet projection channel 13 and an outlet projection 18 having an outlet projection channel 19. The inlet projection 12 and the outlet projection 18 can have any suitable shape and/or configuration that inhibit the flow of bubbles into and/or past the outlet 16b. For example, as shown in Figure 6C, the inlet projection 12 and the outlet projection 18 can be positioned on opposite ends of the chamber 17 with each extending toward its center. In such embodiments, both the inlet projection 12 and the outlet projection 18 can be configured to extend past the center of the chamber 17 so that a direct flow path does not exist between the inlet 16a and the outlet 16b. However, as described above with reference to Figure 6A, the one or more inlet and outlet projections shown in Figure 6C and take any suitable form. For example, although not shown, in some embodiments, either or both of the inlet and outlet projection channels 13, 19 can have a curve near the tip of their respective inlet or outlet projection 12, 18. In some embodiments, the inlet projection channel 18 can advantageously inhibit the inlet 16a from disturbing any bubbles that may have formed near the inlet 16a by positioning the inlet 16a away from the periphery of the chamber 17. Without the inlet projection 12, the inlet 16a may otherwise be prone to disturbing bubbles by, for example, ejecting them away from the periphery of the chamber (e.g., toward the opening 16c of the outlet projection

channel 19), splitting large bubbles into smaller bubbles and dispersing them through the chamber 17, and the like.

[0109] Figures 7A-7H illustrate simplified schematics of a bubble trap 15 (e.g., the bubble trap 15 shown in Figure 6A') trapping bubbles during fluid flow in 45 degree increments, according to some embodiments. Unless otherwise noted, reference numerals in Figures 7A-7H refer to components that are the same as or generally similar to the components in the preceding figures. Each Figure 7A-7H illustrates an inlet 16a, a chamber 17, an outlet projection 18, an outlet projection channel 19, and an outlet 16b. More or less features are also appreciated. The direction of fluid flow is indicated by an arrow and air bubbles are represented by small circles. The air trapping capacity of the bubble trap 15 in each of these figures is shown, for example, by the area of the chamber 17 that lies above the dashed line labeled "C." As shown in Figures 7A-7H, in some embodiments, the area above line C can represent about 50% of the total fluid capacity of the chamber 17 in any given orientation, advantageously indicating that the bubble trap 15 in Figures 7A-7H is not only omnidirectional, but substantially uniformly omnidirectional. It will be appreciated that the bubble trap 15 can, in some embodiments, have a plurality of different trap capacities that correspond to two or more different orientations. It should be understood that an omnidirectional bubble trap according to some embodiments disclosed herein means that the bubble trap 15 has a minimum capacity for gas in all orientations. In some embodiments, that minimum is about 0.5cc, about 1cc, about 2cc, about 3cc, or more. As described above, the trap capacity can depend on a number of factors, including the size and shape of the chamber 17, the length and arrangement of the outlet projection 18 and/or an inlet projection 12 (not shown), the orientation of the bubble trap 15 with respect to fluid flow and gravity, and/or the rate of fluid flow. For example, in some embodiments, if the flow rate increases beyond a threshold rate, the trap capacity can decrease as a result of turbulent flow through the chamber 17 that can disturb the air above line C. However, in some embodiments, the bubble trap 15 can be configured to trap its maximum capacity for any suitable flow rate in any orientation. For example, as shown in Figures 7A-7H, the area above the dashed line "C" schematically represents the maximum amount of air that the bubble trap 15 can trap before it starts flowing through the outlet projection channel 19 and into the fluid line beyond the outlet 16b. In some embodiments, as the chamber 17 fills with air, the amount of dead

space can be equally reduced. In some embodiments, a sensor can be configured to monitor and/or determine the amount of air in the bubble chamber 15 and indicate (e.g., audibly, visually, etc.) when the bubble trap 15 is approaching its trap capacity.

[0110] Figures 8A and 8B are two schematics of a bubble trap 15 with and without a vacuum applied. Figure 8A is a schematic of a bubble trap with a vacuum applied and Figure 8B is a schematic of the bubble trap of Figure 8A filled with fluid. Unless otherwise noted, reference numerals in Figures 8A and 8B refer to components that are the same as or generally similar to the components in the preceding figures. In some embodiments, it can be advantageous to purge a fluid line having a bubble trap 15 (e.g., a fluid transfer module 45) of gas before filling a source and/or destination container 39, 45 with fluid. During a purge, a vacuum pressure can be applied to the bubble trap 15. To optimize the amount of air that can be removed from the bubble trap 15 during a purge, in some embodiments, the bubble trap 15 can comprise a rigid and/or semi-rigid outer housing that is configured to flex (e.g., shrink, collapse, etc.) when a vacuum is applied to the chamber 17. In this way, air can be evacuated (also referred to as withdrawn) from the chamber 17 during a purge. This can advantageously reduce the amount of air that needs to be trapped by the bubble trap 15 when delivering fluid to a patient from a source container 39 and/or filling a destination container 44. For example, when a vacuum is applied to the chamber 17, the rigid and/or semi-rigid outer housing can be configured to change shape and shrink as the size of the chamber 17 decreases as the vacuum increases. In some embodiments, the rigid, and/or semi-rigid outer housing can be configured to return to an expanded state (e.g., its original state before the vacuum was applied) after being collapsed by application of a vacuum. In some embodiments, the shape-restoring mechanism of the bubble trap 15 can correspond to the memory of the material (e.g., the material of the rigid and/or semi-rigid outer housing), the subsequent flow of fluid into and/or through the bubble trap 15, and/or one or more separate shape-restoring structures. In some embodiments, the entire bubble trap 15 can comprise the rigid and/or semi-rigid material configured to collapse upon application of a vacuum. In some embodiments, the rigid and/or semi-rigid material can comprise, for example, polyvinyl chloride (PVC), although any suitable material is appreciated. In some embodiments, the walls do not collapse under a vacuum and the vacuum applied is sufficient to remove the desired amount of gas from the system.

[0111] In some embodiments, the bubble trap 15 can be attached to a fluid line for use with any suitable pump and/or fluid transfer device (e.g., fluid transfer device 30, fluid transfer unit 200, and/or fluid pump assembly 224, etc.). For example, in some embodiments, the bubble trap 15 can be configured to be used with and/or fluidically connected to an ambulatory infusion pump, including infusion pumps that are configured to provide computerized ambulatory drug delivery. While the bubble trap 15 is discussed herein for use with a fluid transfer pump, it will be understood by one of skill in the art that a fluid transfer need not be used with the bubble trap 15. For example, the bubble trap 15 may be used to manually fill a destination container by hand.

[0112] In some embodiments, the bubble trap 15 can be configured to be used with and/or fluidically connected to CADD® pumps manufactured by SMITHS MEDICAL®. Figures 9A and 9B are schematics of a bubble trap 15 in line with a fluid transfer module connected to a cassette. Figure 9A is a schematic of a bubble trap 15 in fluid communication with a cassette with a reservoir and Figure 9B is a schematic of a bubble trap 15 in fluid communication with a cassette without a reservoir, according to some embodiments. Figure 9C is an example fluid transfer protocol for filling the cassette of Figure 9A with medical fluid. Unless otherwise noted, reference numerals in Figures 9A-9C refer to components that are the same as or generally similar to the components in the preceding figures.

[0113] As shown in Figure 9A, the pump 22 can include a removably attached cassette 24 with a reservoir 25 (e.g., source container 39 and/or destination container 44), as well as an air detection sensor 26. The air detection sensor 26 can be configured to indicate (e.g., audibly and/or visually) the presence of gas (e.g., air) in the fluid line that is discharged, for example, from the reservoir 25. In some embodiments, a bubble trap 15 can be connected to the fluid line that is connected to the reservoir 25 in the cassette. In Figure 9A, the bubble trap 15, the cassette 24, and the fluid line therebetween can comprise a fluid transfer module (e.g., fluid transfer module 45), although more or less components and/or features are appreciated. For example, in some embodiments, one end of a male-to-male conduit 28 can be attached to the output 16b of the bubble trap 15, and the other end of the male-to-male conduit 28 can be configured to be in fluid communication with a patient and/or fluid destination container 44. A portion of the male-to-male conduit 28 can be positioned in the air detection sensor 26. It will be appreciated that the male-to-male conduit

28 can have any gender connector combination, including, for example, female-female, female-male, male-female, and/or male-male.

[0114] As described above, the position of the bubble trap 15 between the cassette 24a and the air detection sensor 26 can advantageously reduce the number of air detection alarms (e.g., indications) by trapping air before it is allowed to pass through the outlet 16b of the bubble trap 15 and into the male-to-male conduit 28. As a result, the use of the bubble trap 15 can advantageously translate into fewer treatment interruptions, and therefore enable the pump 22 to provide patients with more consistent and continuous treatment. This, in combination with the ability of the bubble trap 15 to reduce the risk of air embolisms, can increase patient confidence in the pump 22. By trapping air, the bubble trap 15 can enhance patient comfort by reducing and/or eliminating minor air embolisms that, while not lethal, can be nevertheless painful or uncomfortable. The bubble trap 15 can also prevent major air embolisms that are potentially lethal or would otherwise require medical intervention if not prevented from being infused into the patient. As will be described in more detail below with reference to Figure 9C, the fluid transfer module 45 of Figure 9A, including the bubble trap 15, the reservoir 25, and the fluid line therebetween, can be manually or automatically compounded to add the desired amount of fluid to the reservoir 25. For example, in some embodiments, the fluid transfer module 45 can be fluidically connected to a fluid transfer device (e.g., fluid transfer device 30, fluid transfer unit 200, and/or fluid pump assembly 224, etc.).

[0115] Figure 9B is similar to Figure 9A except that the cassette 24 does not include a reservoir 25. The fluid module 45 in Figure 9B instead includes an external source container 39 and/or destination container 44, such as, for example, an IV bag, with a portion of the conduit between the IV bag and the bubble trap 15 positioned in the cassette 24.

[0116] Figure 9C is an example fluid transfer protocol for filling the cassette of Figure 9A with medical fluid. Each of the steps illustrated and/or described in connection with Figure 9C can be performed using, for example, a syringe, or controlled or actuated, for example, in whole or in part, manually (e.g., a person) or automatically (e.g., by a computer processor of the pump 22, and/or by the computer processor positioned in or associated with fluid transfer management system 74). An advantage of some embodiments of this fluid transfer protocol 900 is that it can remove substantially all of the air from the reservoir 25 of

the cassette 24 before the reservoir 25 is filled with fluid. Minimization of air in the destination container 44 (e.g., the cassette 24, reservoir 25, container 44, etc.) during the filling process can be particularly advantageous when the destination container is configured to be accessed from the top once it has been filled. As the air bubbles rise to the top of the destination container, they are more likely to be drawn from the container and transmitted toward the patient. The bubble trap 15 can be configured to catch the remaining residual air in the reservoir 25 by being positioned, as described above, anywhere in line with the reservoir 25 before the flow reaches the patient. For example, in some embodiments, an advantage of some embodiments of this fluid transfer protocol 900 is that it can remove about 98% of the air from the reservoir 25 of the cassette 24 before the reservoir 25 is filled with fluid. The bubble trap 15 can be configured to catch the remaining 2% of residual air in the reservoir 25 by being positioned, as described above, anywhere in line with the reservoir 25 before the flow reaches the patient. Other percentages are also appreciated. As with all embodiments in this specification, one or more of the steps of the fluid transfer protocol 900 can be performed alone, in one or more groups, or in a different ordering than is illustrated in Figure 9C and/or than is described herein. For example, in some embodiments, the following steps can be modified and/or reordered to remove air from a fluid transfer module 45 attached to the fluid transfer device 30 shown in Figure 1A, the fluid transfer system 86 illustrated in Figure 1B, and/or the fluid transfer units 200 shown in Figures 2A_i and 2A_{ii} (e.g., shown, for example, in Figures 2C_i and 2C_{ii}), among any other fluid transfer system. Similarly, in some embodiments, the bubble trap 15 can be used during the filling process to limit the air in the destination container and need not be used during the administration of the fluid from the destination container to the patient. Chronological terms such as “before” or “after” or “begin” or “start” or “end,” or any similar terms, are provided only as examples and are not required in all embodiments. None of these steps is essential or indispensable.

[0117] The fluid transfer protocol 900 begins at the start block 902. The protocol 900 continues in block 904 with removing a cassette 24 from a package. In some embodiments, the cassette 24 can include a reservoir 25. In block 906, the protocol continues with attaching a bubble trap 15 (e.g., an omnidirectional bubble trap) to the cassette 24, the source container 39, and/or destination container 44. At block 908, the

bubble trap 15 and the cassette 24 are fluidically connected to an automated or manual compounder (or a compounder capable of both), such as, for example, to a fluid transfer device (e.g., fluid transfer device 30 or a syringe configured to manually deliver fluid to the cassette 24). In 910, the protocol continues with applying a vacuum to the bubble trap 15 and the cassette 24 with the compounder to remove air inside of each and push it into a source container (e.g., source container 39 and/or destination container 44). In some embodiments, the compounder (or any suitable fluid transfer device) is capable of generating a vacuum in the bubble trap 15 and/or the cassette 24 (e.g., in the reservoir 25 of the cassette 24). For example, in some embodiments, the vacuum can be above or below atmospheric pressure. As described above, the vacuum applied can be sufficient to reduce the volume of the bubble trap 15, such as, for example, by collapsing the chamber 17 of the bubble trap 15. The flexible (e.g., collapsible) rigid and/or semi-rigid material of the bubble trap 15 can advantageously allow gas to be removed from the bubble trap 15 at lower vacuum pressure relative to the vacuum that would otherwise be required to remove an equivalent amount of gas from the bubble trap 15 if the material did not comprise flexible rigid and/or semi-rigid material. At block 912, the protocol continues with pushing medical fluid into the reservoir 25 of the cassette 24 with the compounder. In some embodiments, one or more fluids can be pushed into the reservoir 25 by the compounder. Blocks 914 and 916 of the protocol continue with detaching the bubble trap 15 and the cassette 24 from the fluid transfer device and then attaching the bubble trap 15 and the cassette 24 to the pump 22, respectively. At block 918, the process ends with pumping fluid in the reservoir 25 of the cassette 24 past the bubble trap 15 and into a patient. However, it will be understood, that in some embodiments, the process can end with pumping fluid in past the bubble trap 15 and into a source container 39 and/or destination container 44. From there, in some embodiments the fluid can be pumped from the source container 39 to the patient without the use of a bubble trap 15. Similarly, in some embodiments, the fluid can be pumped from the destination container 44 to the patient without the use of a bubble trap 15,

[0118] With continued reference to infusion pumps such as the pump 22 illustrated in Figures 9A and 9B, Figures 10A and 10B illustrate examples of schematics in which the cassette 24 can be modified to trap and/or remove air. This is in contrast to Figures 9A and 9B, which illustrate examples of schematics in which the fluid line can be

modified to trap and/or remove air, such as, for example, with the addition of a bubble trap 15. For example, Figure 10A is a schematic of a cassette configured with a barrier 101. As another example, Figure 10B is a schematic of a cassette configured to trap and/or remove air with a port 104. It will be appreciated that, in various embodiments, any of the features and/or embodiments described herein can be combined, including, for example, the embodiments shown in Figures 9A, 9B, 10A, and/or 10B, among others (e.g., the disclosure contemplated herein, including Figures 1-8B and 9C). Unless otherwise noted, reference numerals in Figures 10A and 10B refer to components that are the same as or generally similar to the components in the preceding figures.

[0119] As shown in Figure 10A, a barrier 101 can be added to the reservoir 25 of the cassette 24 to create a partition in the reservoir 25. In some embodiments, the barrier can be, for example, a heat sealed barrier, although any suitable barrier is appreciated. In some embodiments, the reservoir 25 can include one or more barriers. The barrier 101 can advantageously create a bubble collection region 102 (also referred to as a subreservoir or subchamber) that is spaced apart from the outlet of the reservoir 25, as well as an outlet region 103 (also referred to as an outlet chamber). While the barrier 101 is illustrated in Figure 10A as having a particular shape and size in relation to the reservoir 25, it will be understood by one skilled in the art that the barrier 101 may comprise any shape or size capable of creating a bubble collection region 102. In some embodiments, the barrier 101 can prevent some or all of the air in the reservoir 25 from being pumped from the reservoir 25 by trapping it in the bubble collection region 102.

[0120] In some embodiments, the outlet region 103 may be located on a bottom portion of the reservoir 25. As air bubbles rise to the top of the reservoir 25, the location of the outlet region 103 on the bottom portion can reduce the amount of air bubbles that are passed through the outlet region 103 and one or more connectors 105, 106. As a result, the location of the outlet region 103 may advantageously reduce the number of air detection alarms and translate into fewer treatment interruptions, and therefore enable the pump 22 to provide patients with more consistent and continuous treatment. This, in combination with the ability of the bubble trap 15 to reduce the risk of air embolisms, can increase patient confidence in the pump 22.

[0121] As illustrated in Figure 10B, the port 104 can be, for example, an adapter configured to attach to a fluid transfer device (e.g., fluid transfer device 30, a syringe, etc.) configured to apply a vacuum to the reservoir 25 before it is filled with fluid. In some embodiments, the port 104 may be configured to remove air bubbles present in the reservoir 25 after the pump 22 has filled the reservoir 25 with fluid. The port 104 can be located at a top portion of the reservoir 25, as shown in Figure 10B, to facilitate the removal of air bubbles that rise to the top of the reservoir 25. As described above, this can advantageously reduce the amount of air in the reservoir 25 and thereby reduce the chances of giving a patient an air embolism. It can also advantageously reduce the frequency at which the air detection sensor 26 indicates the presence of air in the line. In some embodiments, the port 104 can allow gas to be evacuated from the reservoir 25 and/or can allow the infusion and/or insertion of drugs into the reservoir 25 when needed. As illustrated in Figures 10A-10B, in some embodiments, the cassette may be in fluid communication with one or more connectors 105, 106. Connectors 105, 106 may comprises one or more luer connectors, such as a female or male medical connector having a luer fitting.

[0122] Any system, method, and device described in this application can include any combination of the preceding features described in this and other paragraphs, among other features and combinations described herein, including features and combinations described in subsequent paragraphs.

[0123] Although this invention has been disclosed in the context of certain embodiments and examples, it will be understood by those skilled in the art that the present invention extends beyond the specifically disclosed embodiments to other alternative embodiments and/or uses of the invention and obvious modifications and equivalents thereof. In addition, while several variations of the invention have been shown and described in detail, other modifications, which are within the scope of this invention, will be readily apparent to those of skill in the art based upon this disclosure. It is also contemplated that various combinations or sub-combinations of the specific features and aspects of the embodiments may be made and still fall within the scope of the invention. It should be understood that various features and aspects of the disclosed embodiments can be combined with, or substituted for, one another in order to form varying modes of the disclosed invention. Thus, it is intended that the scope of the present invention herein disclosed should

not be limited by the particular disclosed embodiments described above, but should be determined only by a fair reading of the claims that follow. Moreover, language such as “up to,” “at least,” “greater than,” “less than,” “between,” and the like includes the number recited. Numbers preceded by a term such as “approximately,” “about”, and “substantially” as used herein include the recited numbers (e.g., about 10% = 10%), and also represent an amount close to the stated amount that still performs a desired function or achieves a desired result. For example, the terms “approximately”, “about”, and “substantially” may refer to an amount that is within less than 10% of, within less than 5% of, within less than 1% of, within less than 0.1% of, and within less than 0.01% of the stated amount.

THE FOLLOWING IS CLAIMED:

1. An inline bubble trap device configured to be in fluid communication with a medical fluid line, the bubble trap device comprising:
an inlet comprising an inlet opening having an inlet opening center axis;
an outlet comprising an outlet opening having an outlet opening center axis;
and
a chamber,
wherein the inlet opening center axis and the outlet opening center axis are different from one another such that the inlet opening is misaligned from the outlet opening, and
wherein the bubble trap is configured to inhibit a flow of gas from the inlet to the outlet.
2. The inline bubble trap of Claim 1, wherein the inlet opening being misaligned from the outlet opening breaks up a fluid path from the inlet opening to the outlet opening.
3. The inline bubble trap of any of Claims 1 and 2, wherein the chamber is configured to trap gas that flows into the bubble trap.
4. The inline bubble trap of any of Claims 1-3, wherein the chamber is located between the inlet and the outlet.
5. The inline bubble trap of any of Claims 1-4, wherein the outlet comprises an outlet projection.
6. The inline bubble trap of Claim 5, wherein the outlet projection comprises the outlet opening and a channel in fluid communication with the outlet.
7. The inline bubble trap of any of Claims 5 and 6, wherein the outlet projection extends into the chamber away from an inner surface of the chamber.
8. The inline bubble trap of any of Claims 5-7, wherein the outlet opening of the outlet projection is positioned near or at the center of the chamber.
9. The inline bubble trap of any of Claims 5-8, wherein the outlet opening of the outlet projection is positioned on a side of the outlet projection.
10. The inline bubble trap of any of Claims 1-9, wherein the inlet comprises an inlet projection.

11. The inline bubble trap of Claim 10, wherein the inlet projection comprises the inlet opening and a channel in fluid communication with the inlet.

12. The inline bubble trap of any of Claims 10, wherein the inlet projection extends into the chamber away from an inner surface of the chamber.

13. The inline bubble trap of any of Claims 10-12, wherein the inlet opening is positioned near or at the center of the chamber.

14. The inline bubble trap of any of Claims 10-13, wherein the inlet opening is positioned on a side of the inlet projection.

15. The inline bubble trap of any of Claims 10-14, wherein the inlet projection and the outlet projection extend past each other such that inlet opening is positioned closer to the outlet than the outlet opening.

16. The inline bubble trap of any of Claims 1-15, wherein every flow path from the inlet opening to the outlet opening includes a bend.

17. The inline bubble trap of any of Claims 1-16, wherein the inlet and the outlet are on opposite ends of the chamber.

18. The inline bubble trap of any of Claims 1-17, wherein the bubble trap includes a resilient housing at least partially defining the chamber with a rest volume, the housing configured to at least partially collapse when subjected to a vacuum so as to reduce the volume of the chamber and configured to return to the rest volume when the vacuum is removed.

19. A medical fluid transfer system configured to trap air during the transfer of medical fluids, the medical fluid transfer system comprising:

a fluid transfer device configured to transfer fluid from a fluid source to a fluid destination; and

the inline bubble trap of any one of Claims 1-18 further comprising a female luer end and a male luer end,

wherein the bubble trap is configured to be in fluid communication with at least one of the fluid transfer device, a fluid source, and a fluid destination, and

wherein the bubble trap is configured to inhibit a transfer of gas from the fluid source, through the outlet of the bubble trap, and into the fluid destination.

20. The system of Claim 19, wherein the bubble trap is in fluid communication with the fluid source.

21. The system of any of Claims 19-20, wherein the bubble trap is in fluid communication with the fluid destination.

22. The system of any of Claims 19-21, wherein the female luer end is adjacent to the outlet.

23. The system of any of Claims 19-22, wherein the male luer end is adjacent to the inlet.

24. A method of transferring fluids from a source container to a destination container, the method comprising:

obtaining a fluid transfer module configured to inhibit a transfer of gas from the source container to the destination container, the fluid transfer module comprising an inline bubble trap, the bubble trap comprising a chamber, an inlet opening having an inlet center axis, and an outlet opening having an outlet center axis different from the inlet center axis such that the inlet opening is misaligned from the outlet opening;

ensuring the fluid transfer module is in fluid communication with the source container and the destination container; and

transferring fluid from the source container, through the fluid transfer module, and into the destination container.

25. The method of Claim 24, further comprising the step of initiating a vacuum in the destination container and the fluid transfer module such that a volume defined by the chamber of the fluid transfer module is reduced prior to initiating the transferring step.

26. The method of any of Claims 24 and 25, wherein the inlet opening being misaligned from the outlet opening breaks up a fluid path from the inlet opening to the outlet opening.

27. The method of any of Claims 24-26, wherein the fluid transfer module further comprises an outlet projection having the outlet opening and a channel in fluid communication with the outlet.

28. The method of Claim 27, wherein the outlet projection extends into the chamber away from an inner surface of the chamber.

29. The method of any of Claims 27 and 28, wherein the outlet opening of the outlet projection is positioned on a side of the outlet projection.

30. The method of any of Claims 24-29, wherein the fluid transfer module further comprises an inlet projection having the inlet opening and a channel in fluid communication with the inlet.

31. The method of Claim 30, wherein the inlet projection extends into the chamber away from an inner surface of the chamber.

32. The method of any of Claims 30 and 31, wherein the inlet opening is positioned on a side of the inlet projection.

33. The method of any of Claims 24-32 further comprising disconnecting the fluid transfer module from the source container and the destination container.

34. An inline bubble trap device configured to be in fluid communication with a medical fluid line, the bubble trap device comprising:

a chamber comprising an inner surface and an outer surface;

an inlet comprising an inlet projection extending into the chamber, the inlet projection having an inlet channel and an inlet opening being displaced away from the inner surface of the chamber;

an outlet comprising an outlet projection extending into the chamber, the outlet projection having an outlet channel and an outlet opening being displaced away from the inner surface of the chamber,

wherein the bubble trap is configured to inhibit a flow of gas from the inlet to the outlet.

35. The inline bubble trap of Claim 34, wherein the inlet opening and the outlet opening are oriented away from each other such that fluid moving between the openings need take an indirect path.

36. The inline bubble trap of any of Claims 34 and 35, wherein at least one of the inlet and the outlet channels comprises a curve that misaligns the inlet opening from the outlet opening and breaks up a fluid path from the inlet opening to the outlet opening through the chamber.

37. The inline bubble trap of any of Claims 34-36, wherein the chamber is configured to trap gas that flows into the bubble trap.

38. The inline bubble trap of any of Claims 34-37, wherein the chamber is collapsible.

39. The inline bubble trap of any of Claims 34-38, wherein the outlet opening of the outlet projection is positioned near or at the center of the chamber.

40. The inline bubble trap of any of Claims 34-39, wherein the inlet opening is positioned near or at the center of the chamber.

41. The inline bubble trap of any of Claims 34-41, wherein the inlet projection and the outlet projection project past each other within the chamber.

42. A medical fluid transfer system configured to trap air during the transfer of medical fluids, the medical fluid transfer system comprising:

a fluid transfer device configured to transfer fluid from a fluid source to a fluid destination; and

the inline bubble trap of any one of Claims 34 to 41 further comprising a female luer end and a male luer end, wherein the bubble trap is configured to be in fluid communication with at least one of the fluid transfer device, a fluid source, and a fluid destination, and

wherein the bubble trap is configured to inhibit a transfer of gas from the fluid source, through the outlet of the bubble trap, and into the fluid destination.

43. The system of Claim 42, wherein the bubble trap is in fluid communication with the fluid source.

44. The system of any of Claims 42 and 43, wherein the bubble trap is in fluid communication with the fluid destination.

45. The system of any of Claims 42-44, wherein the female luer end is adjacent to the outlet.

46. The system of any of Claims 42-45, wherein the male luer end is adjacent to the inlet.

47. A patient source bag for use with a medical fluid infusion pump, the patient source bag comprising:

a chamber;

an outlet comprising an outlet region in fluid communication with the chamber; and

a barrier defining an air collection region in fluid communication with the outlet, the barrier being configured to maintain air within the air collection region.

48. The patient source bag of Claim 47, wherein the barrier is configured inhibit the transfer of gas through the outlet region.

49. The patient source bag of any of Claims 47 and 48, wherein the air collection region is located outside a continuous fluid flow path between the chamber and the outlet region.

50. The patient source bag of any of Claims 47-49, wherein the air collection region is spaced apart from the outlet.

51. The patient source bag of any of Claims 47-50, wherein the outlet is located on an upper region of the chamber.

52. The patient source bag of any of Claims 47-51, wherein the outlet is configured to permit the passage of fluid into and out of the chamber.


53. The patient source bag of any of Claims 47-52 further comprising a port configured to permit the removal of air from the chamber.


54. The patient source bag of any of Claims 47-53 further comprising at least one access port.

55. The patient source bag of Claim 54, wherein the access port is a closeable female luer connector.

56. The patient source bag of Claim 54, wherein the access port is a closeable male luer connector.

57. The patient source bag of any of Claims 47-56, further comprising a bubble trap outside the chamber and in fluid communication with the chamber.

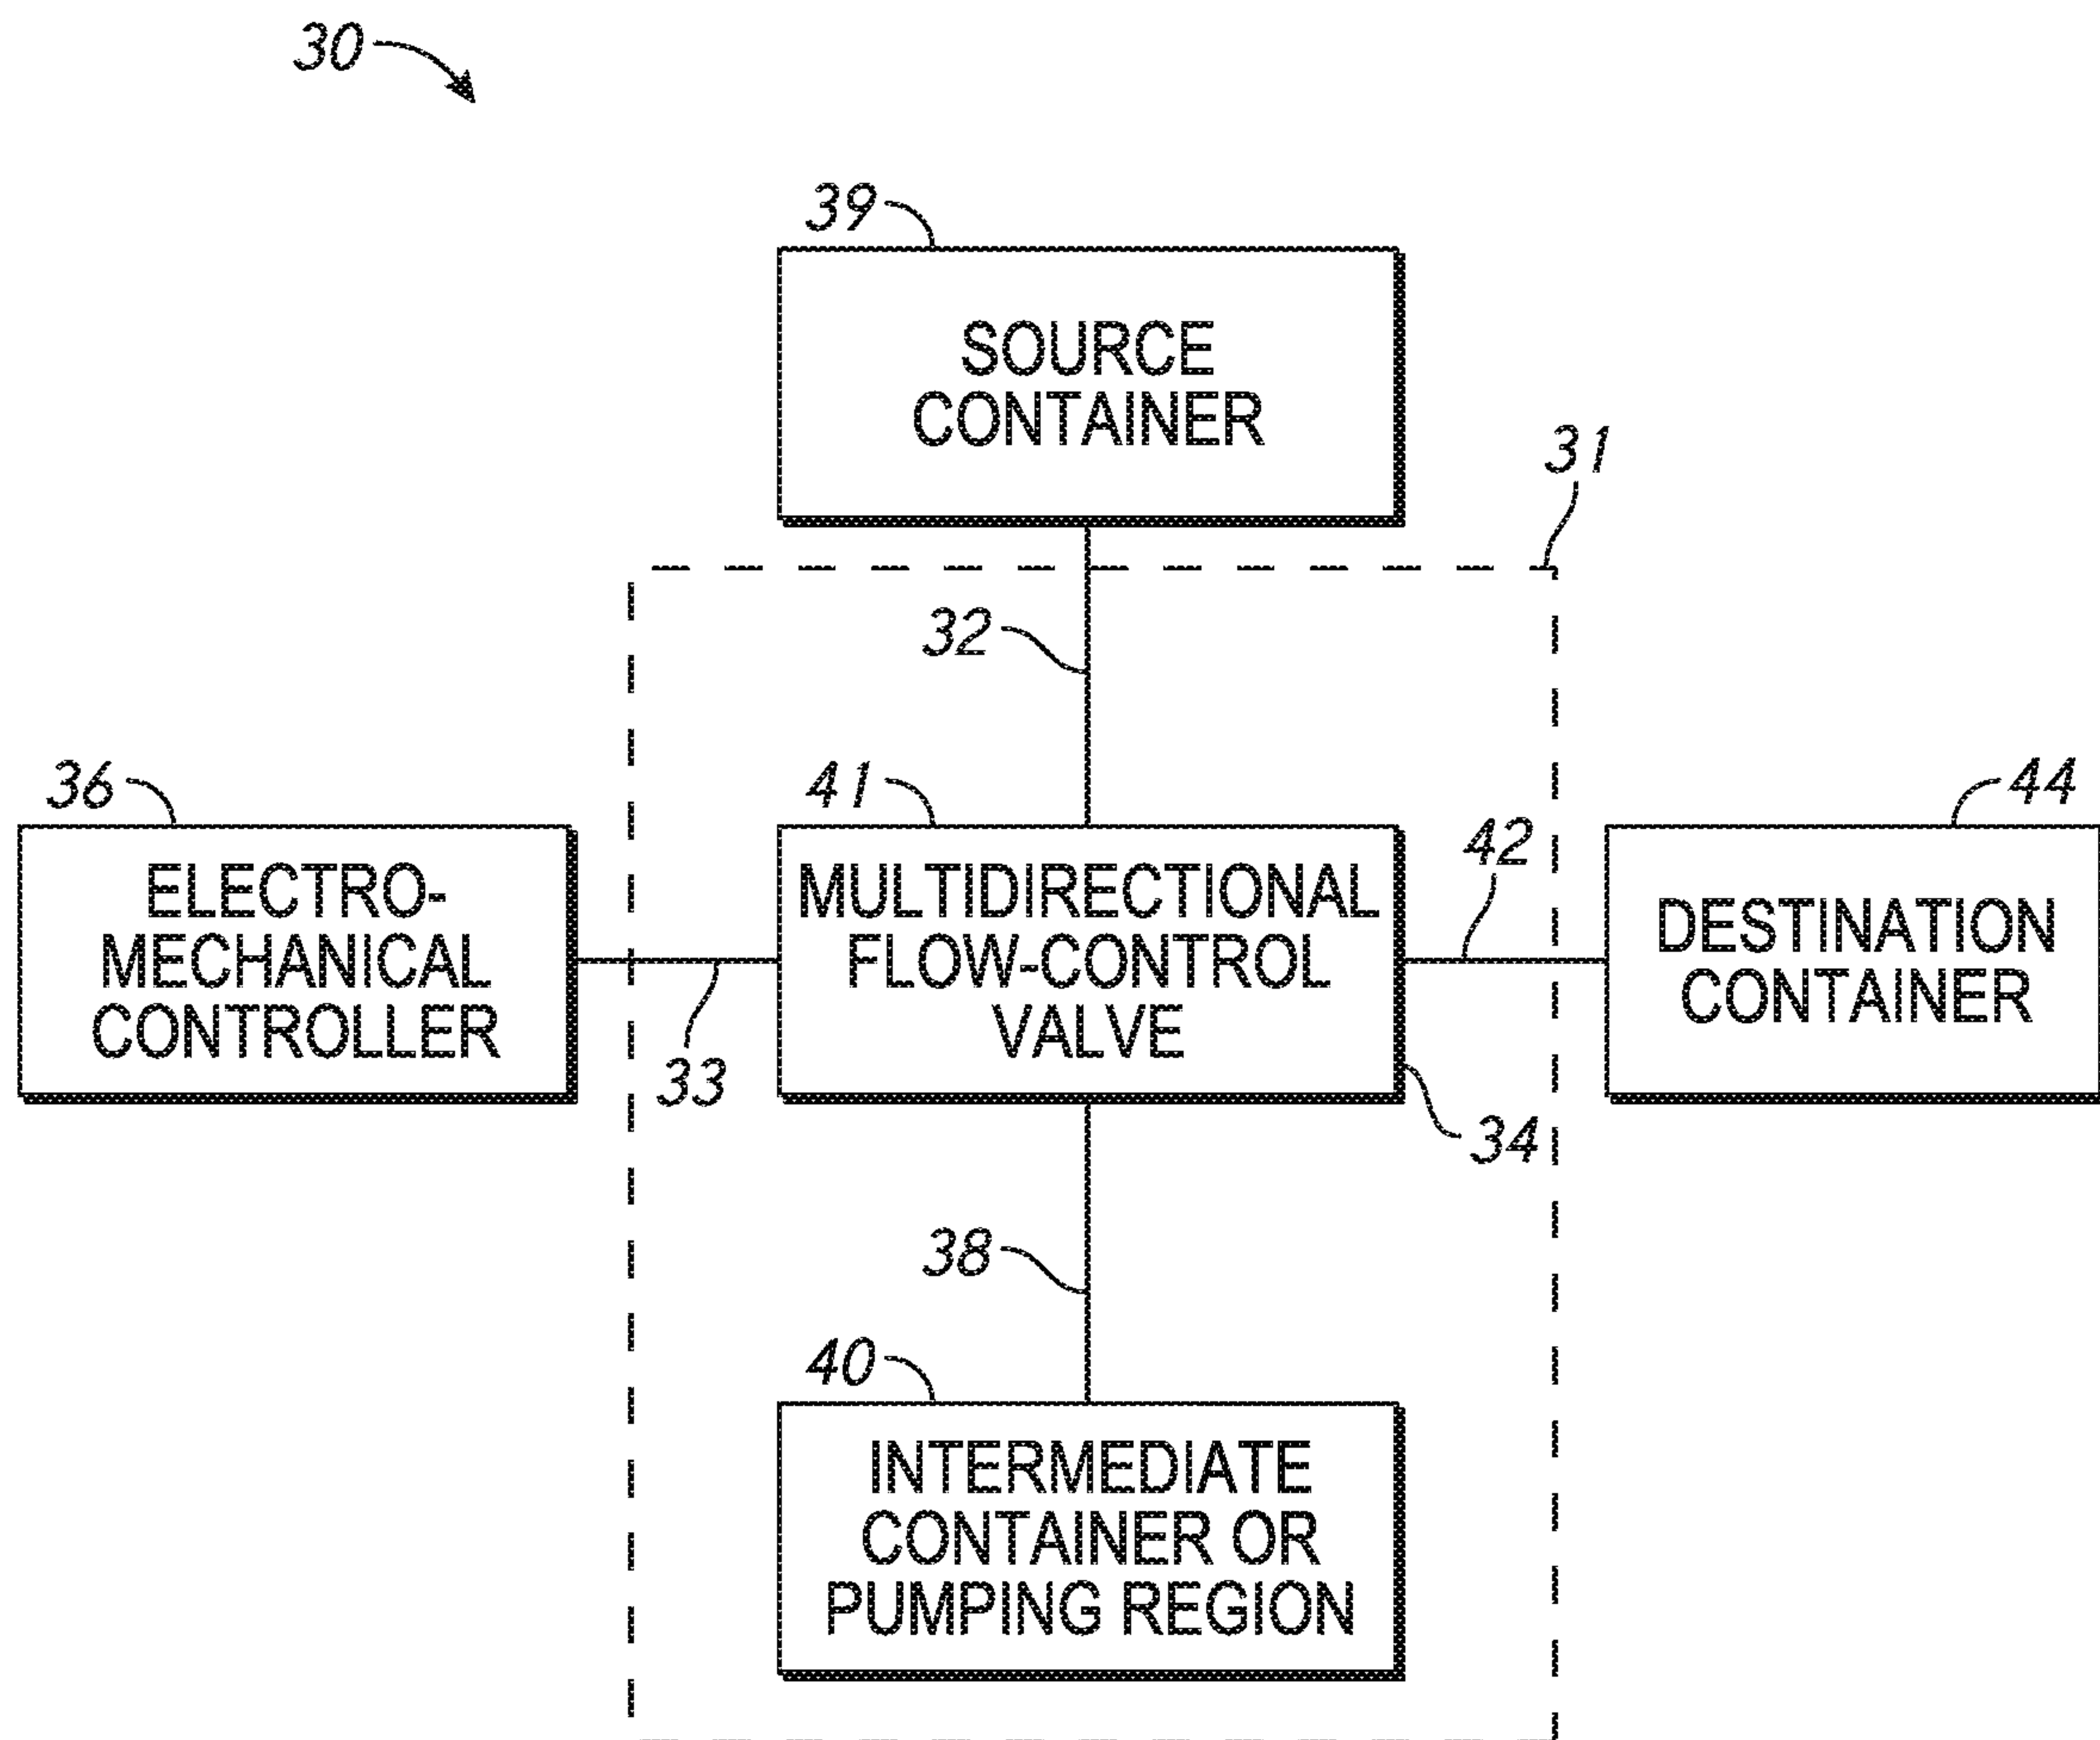*FIG. 1A*

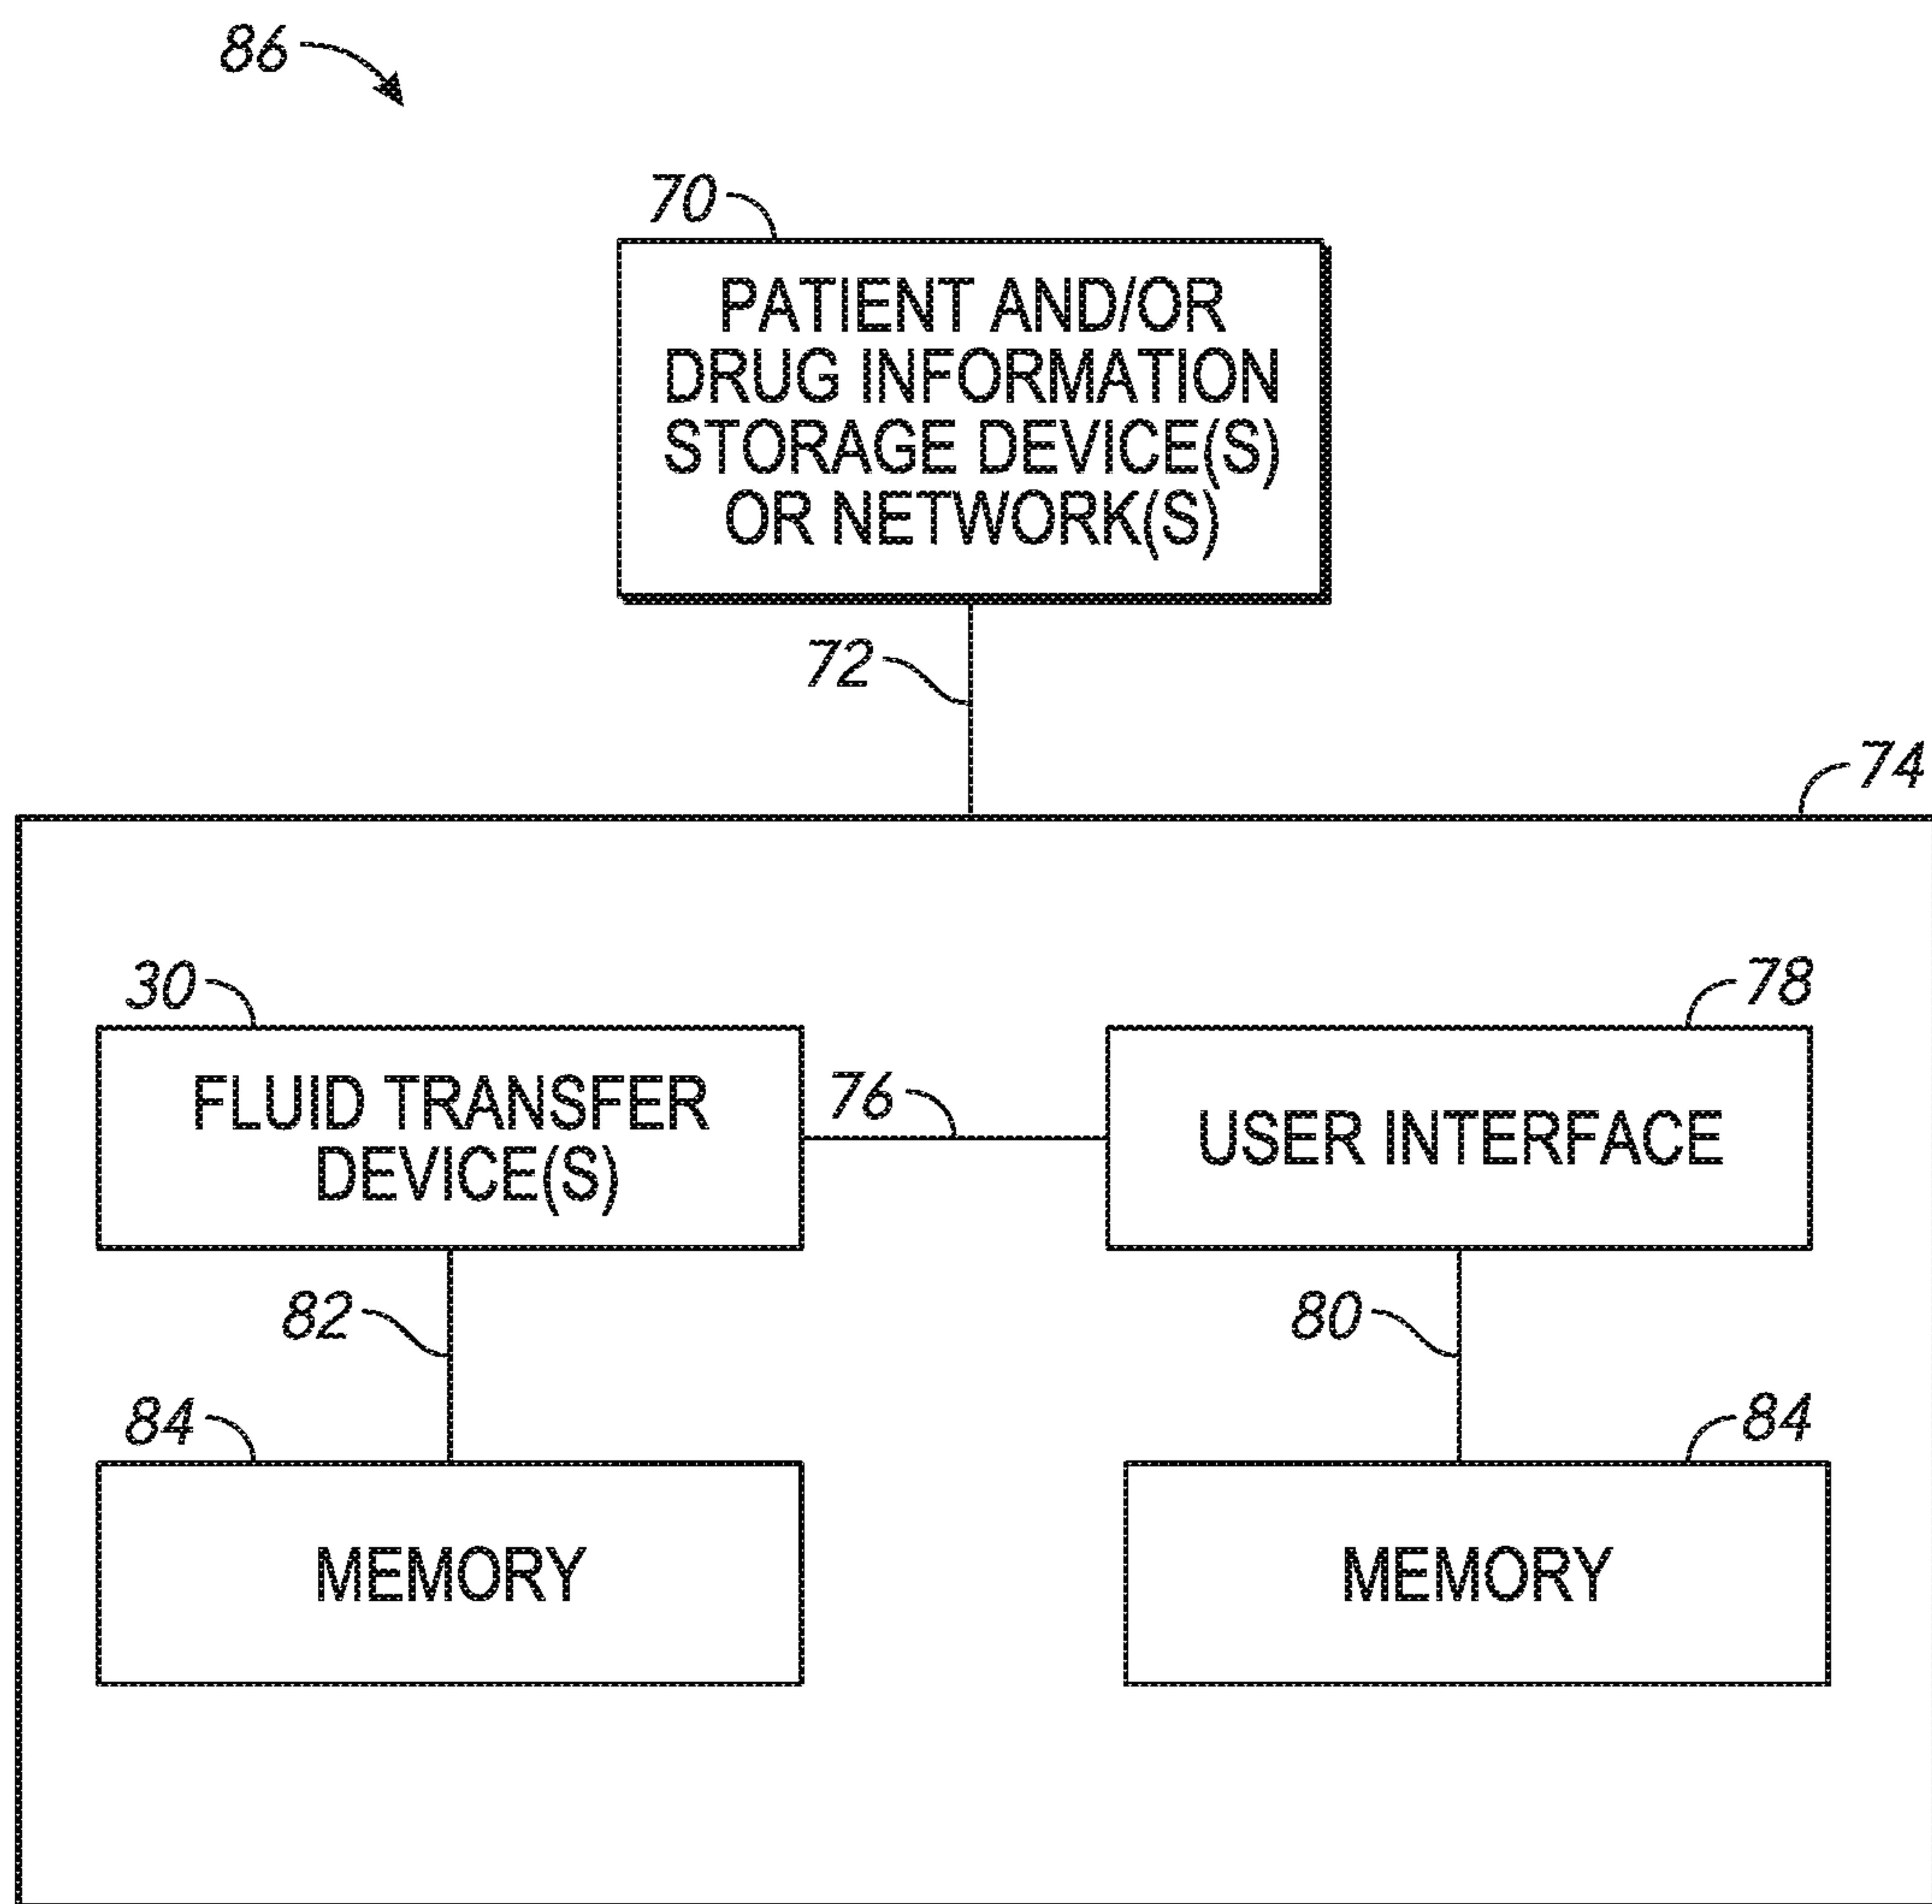*FIG. 1B*

3/24

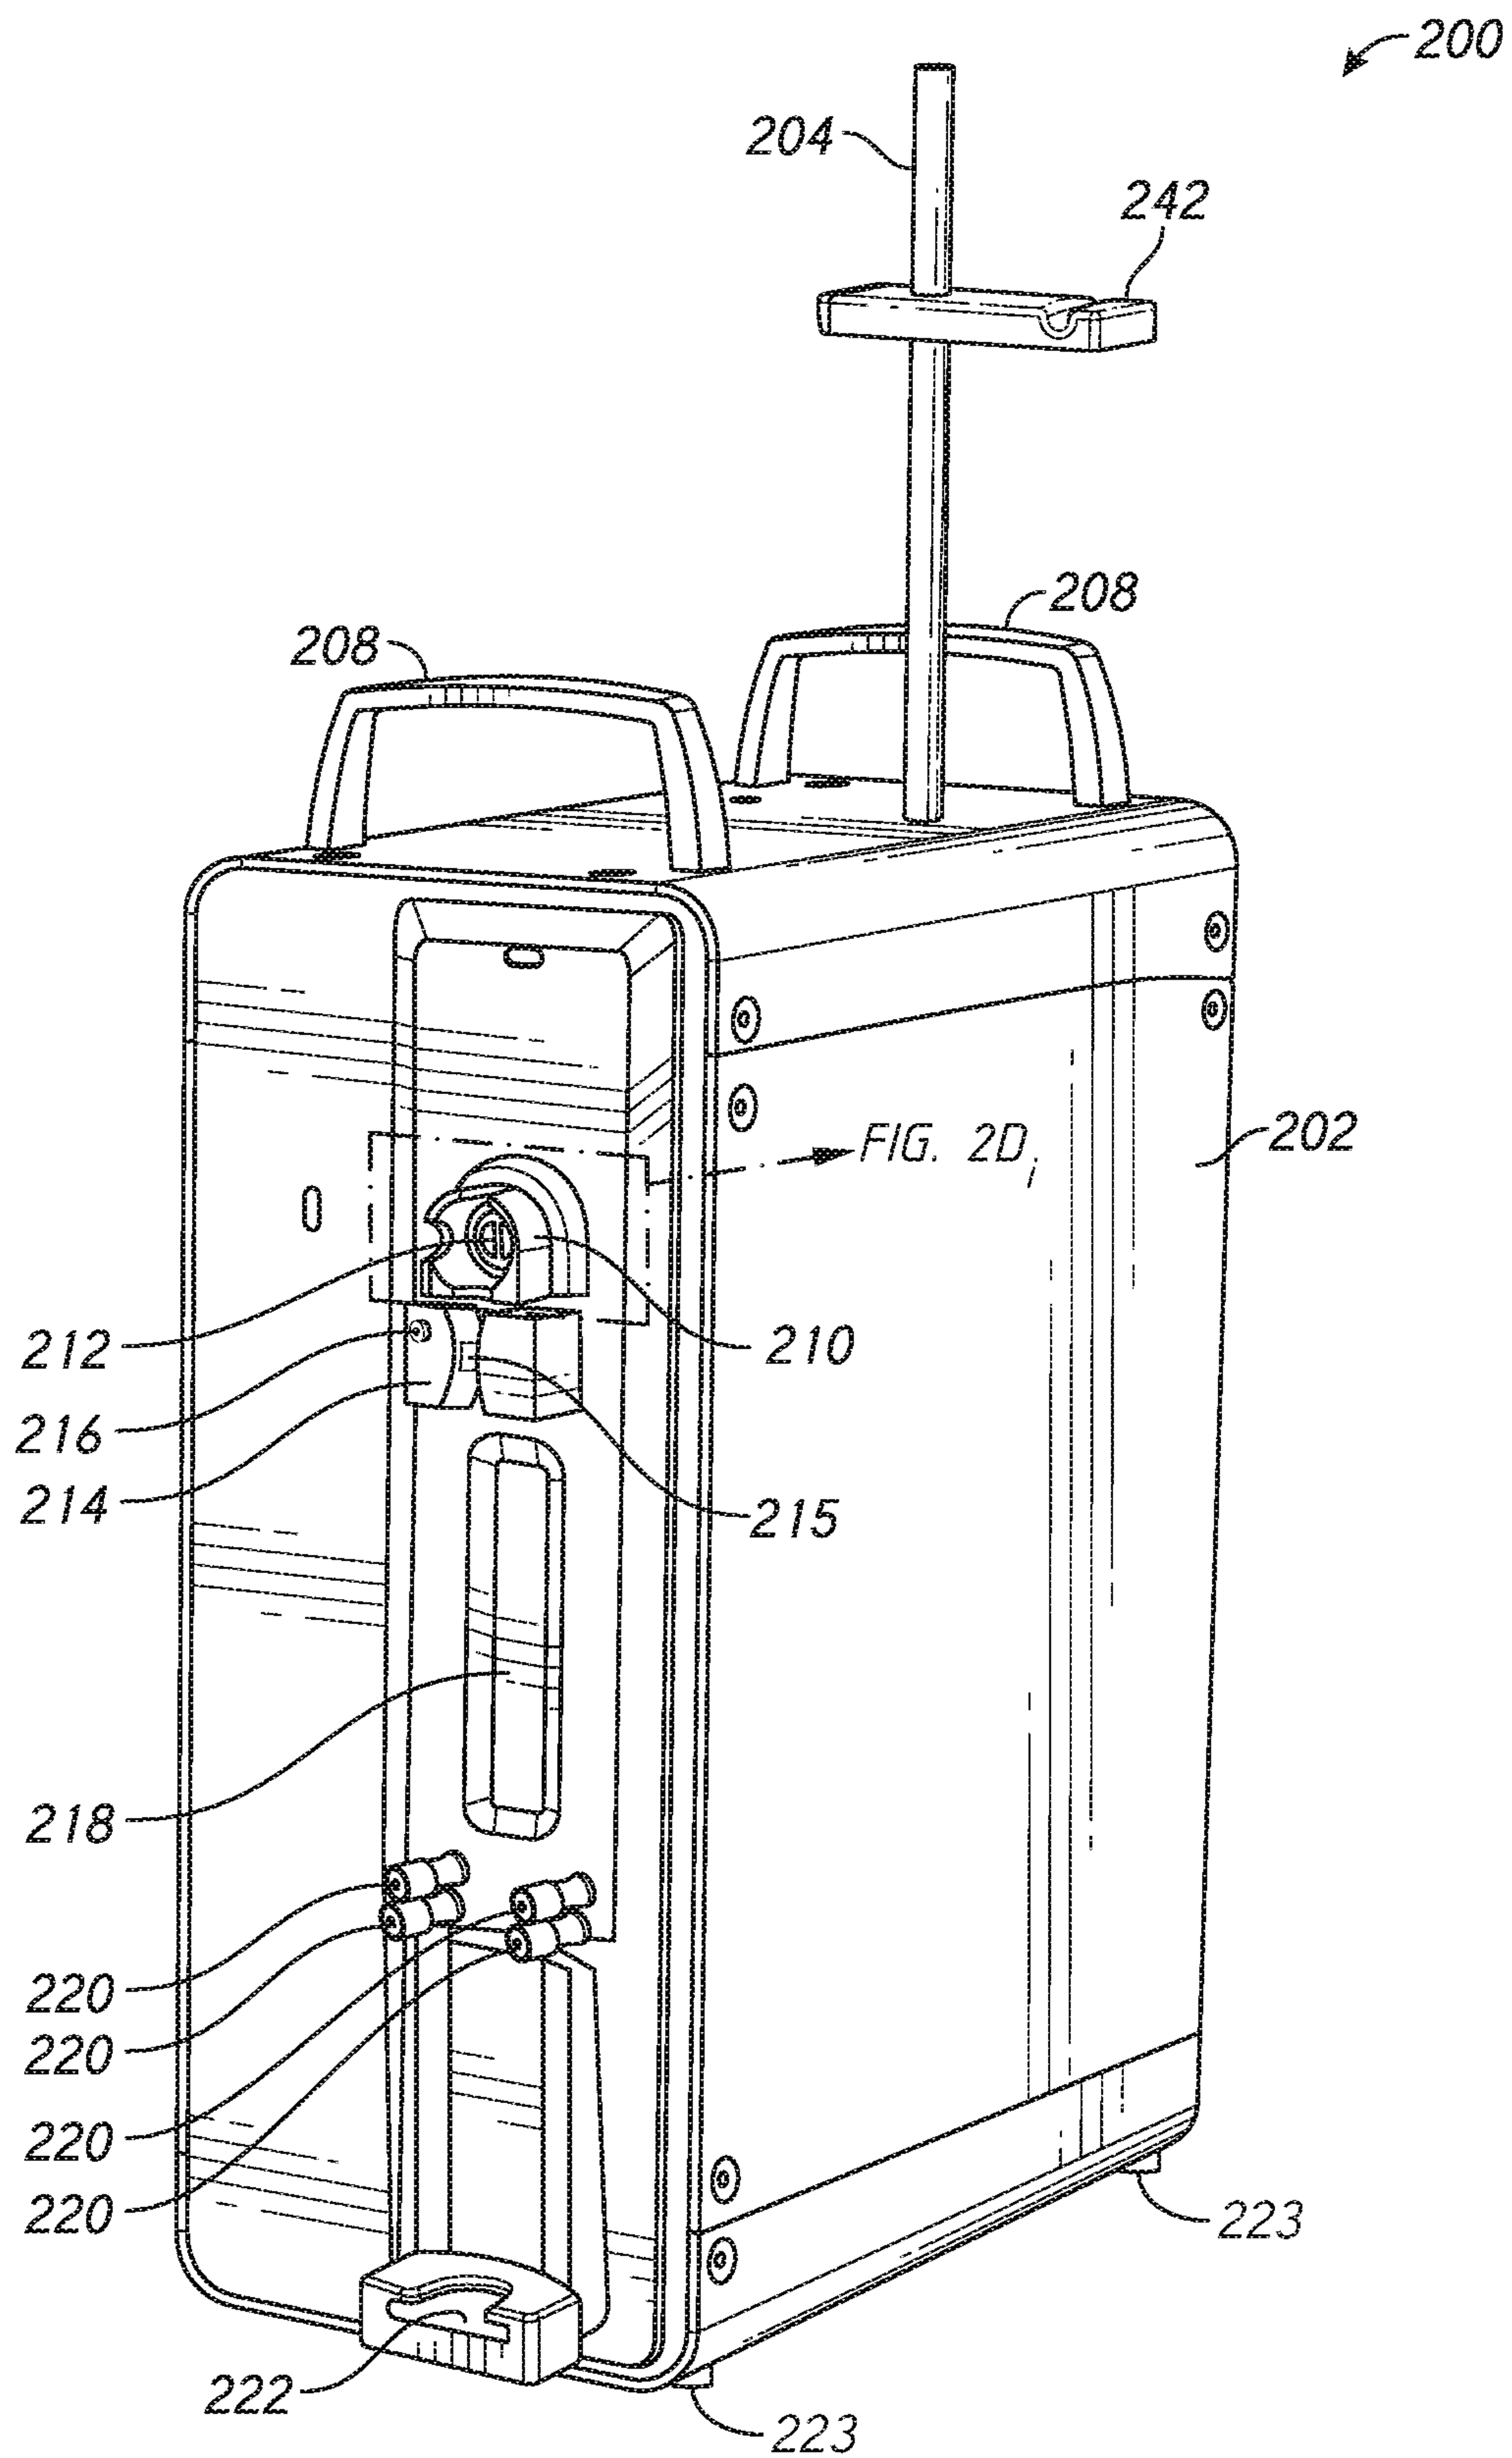
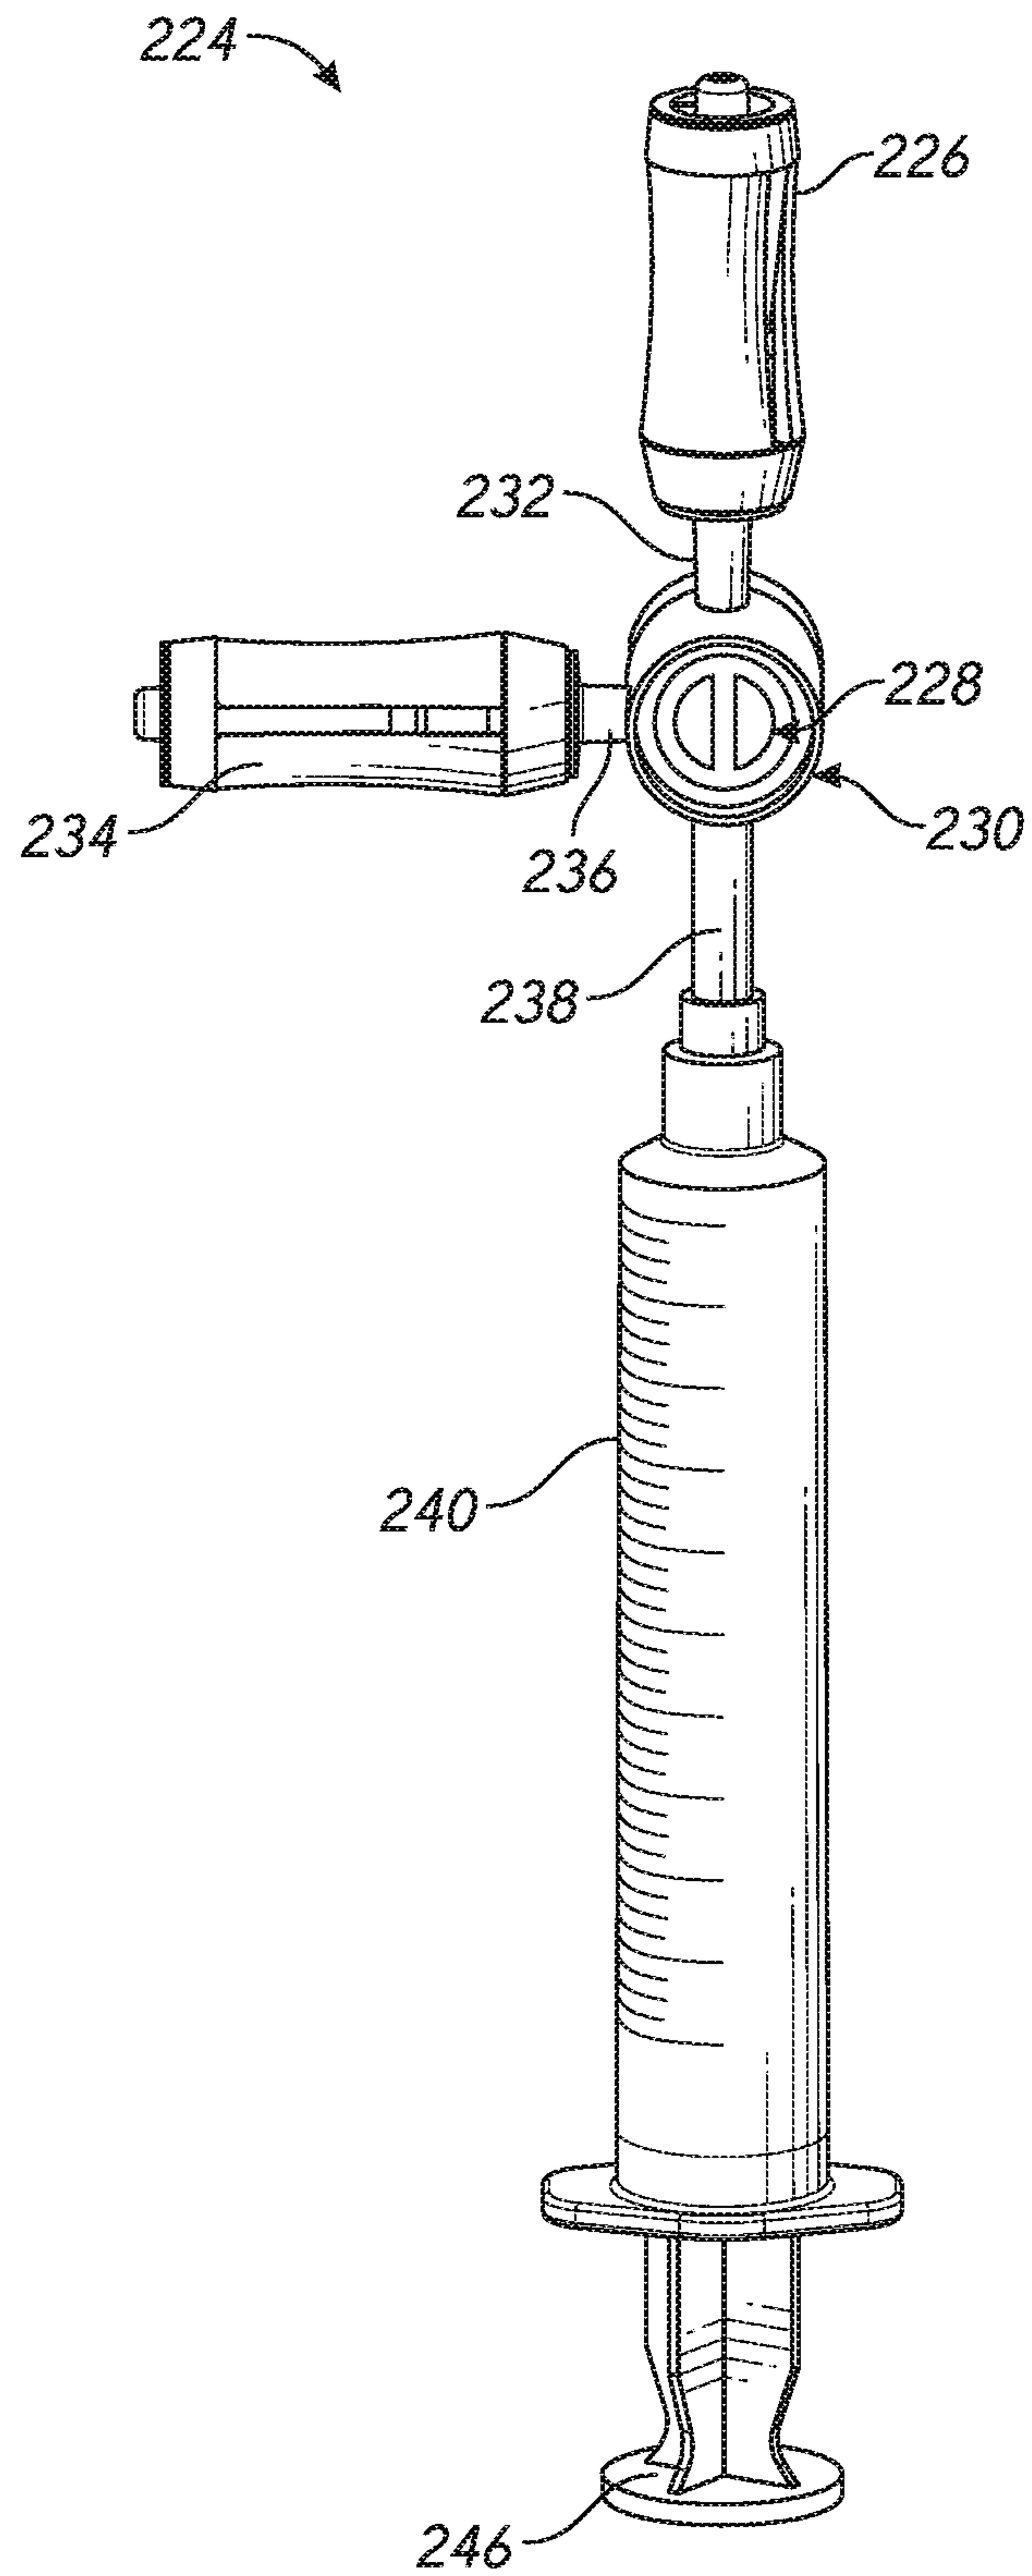
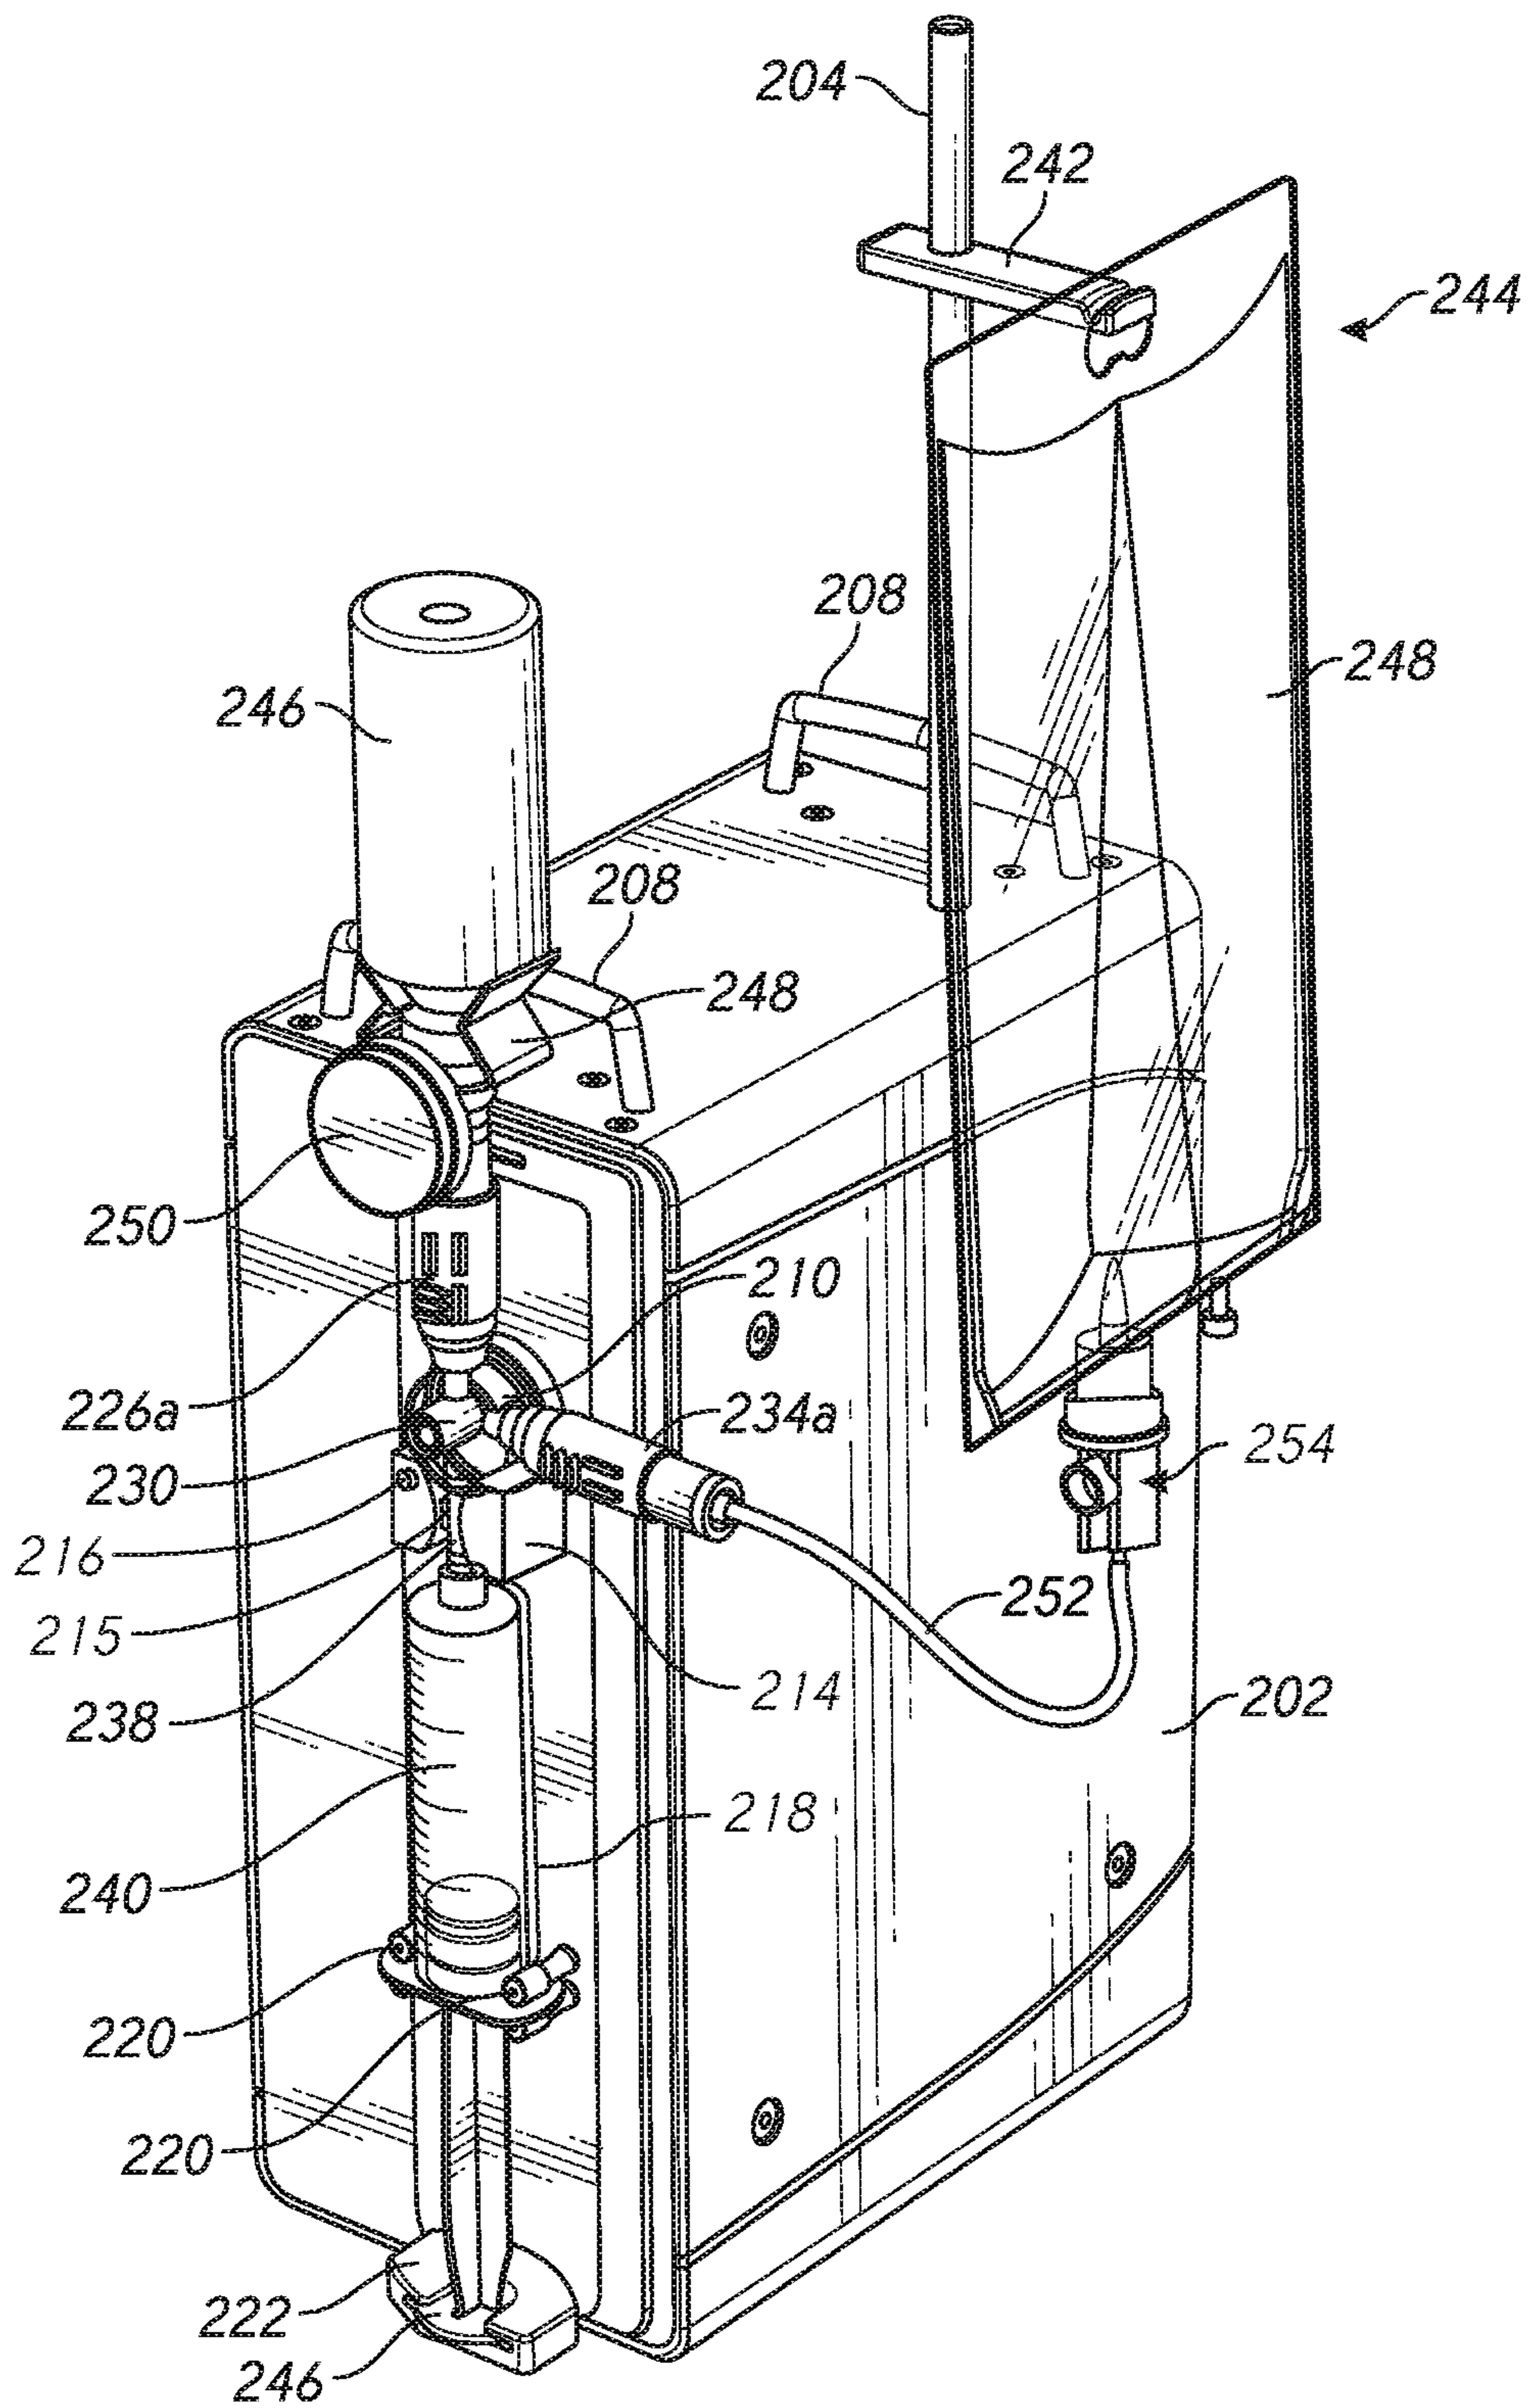


FIG. 2A,

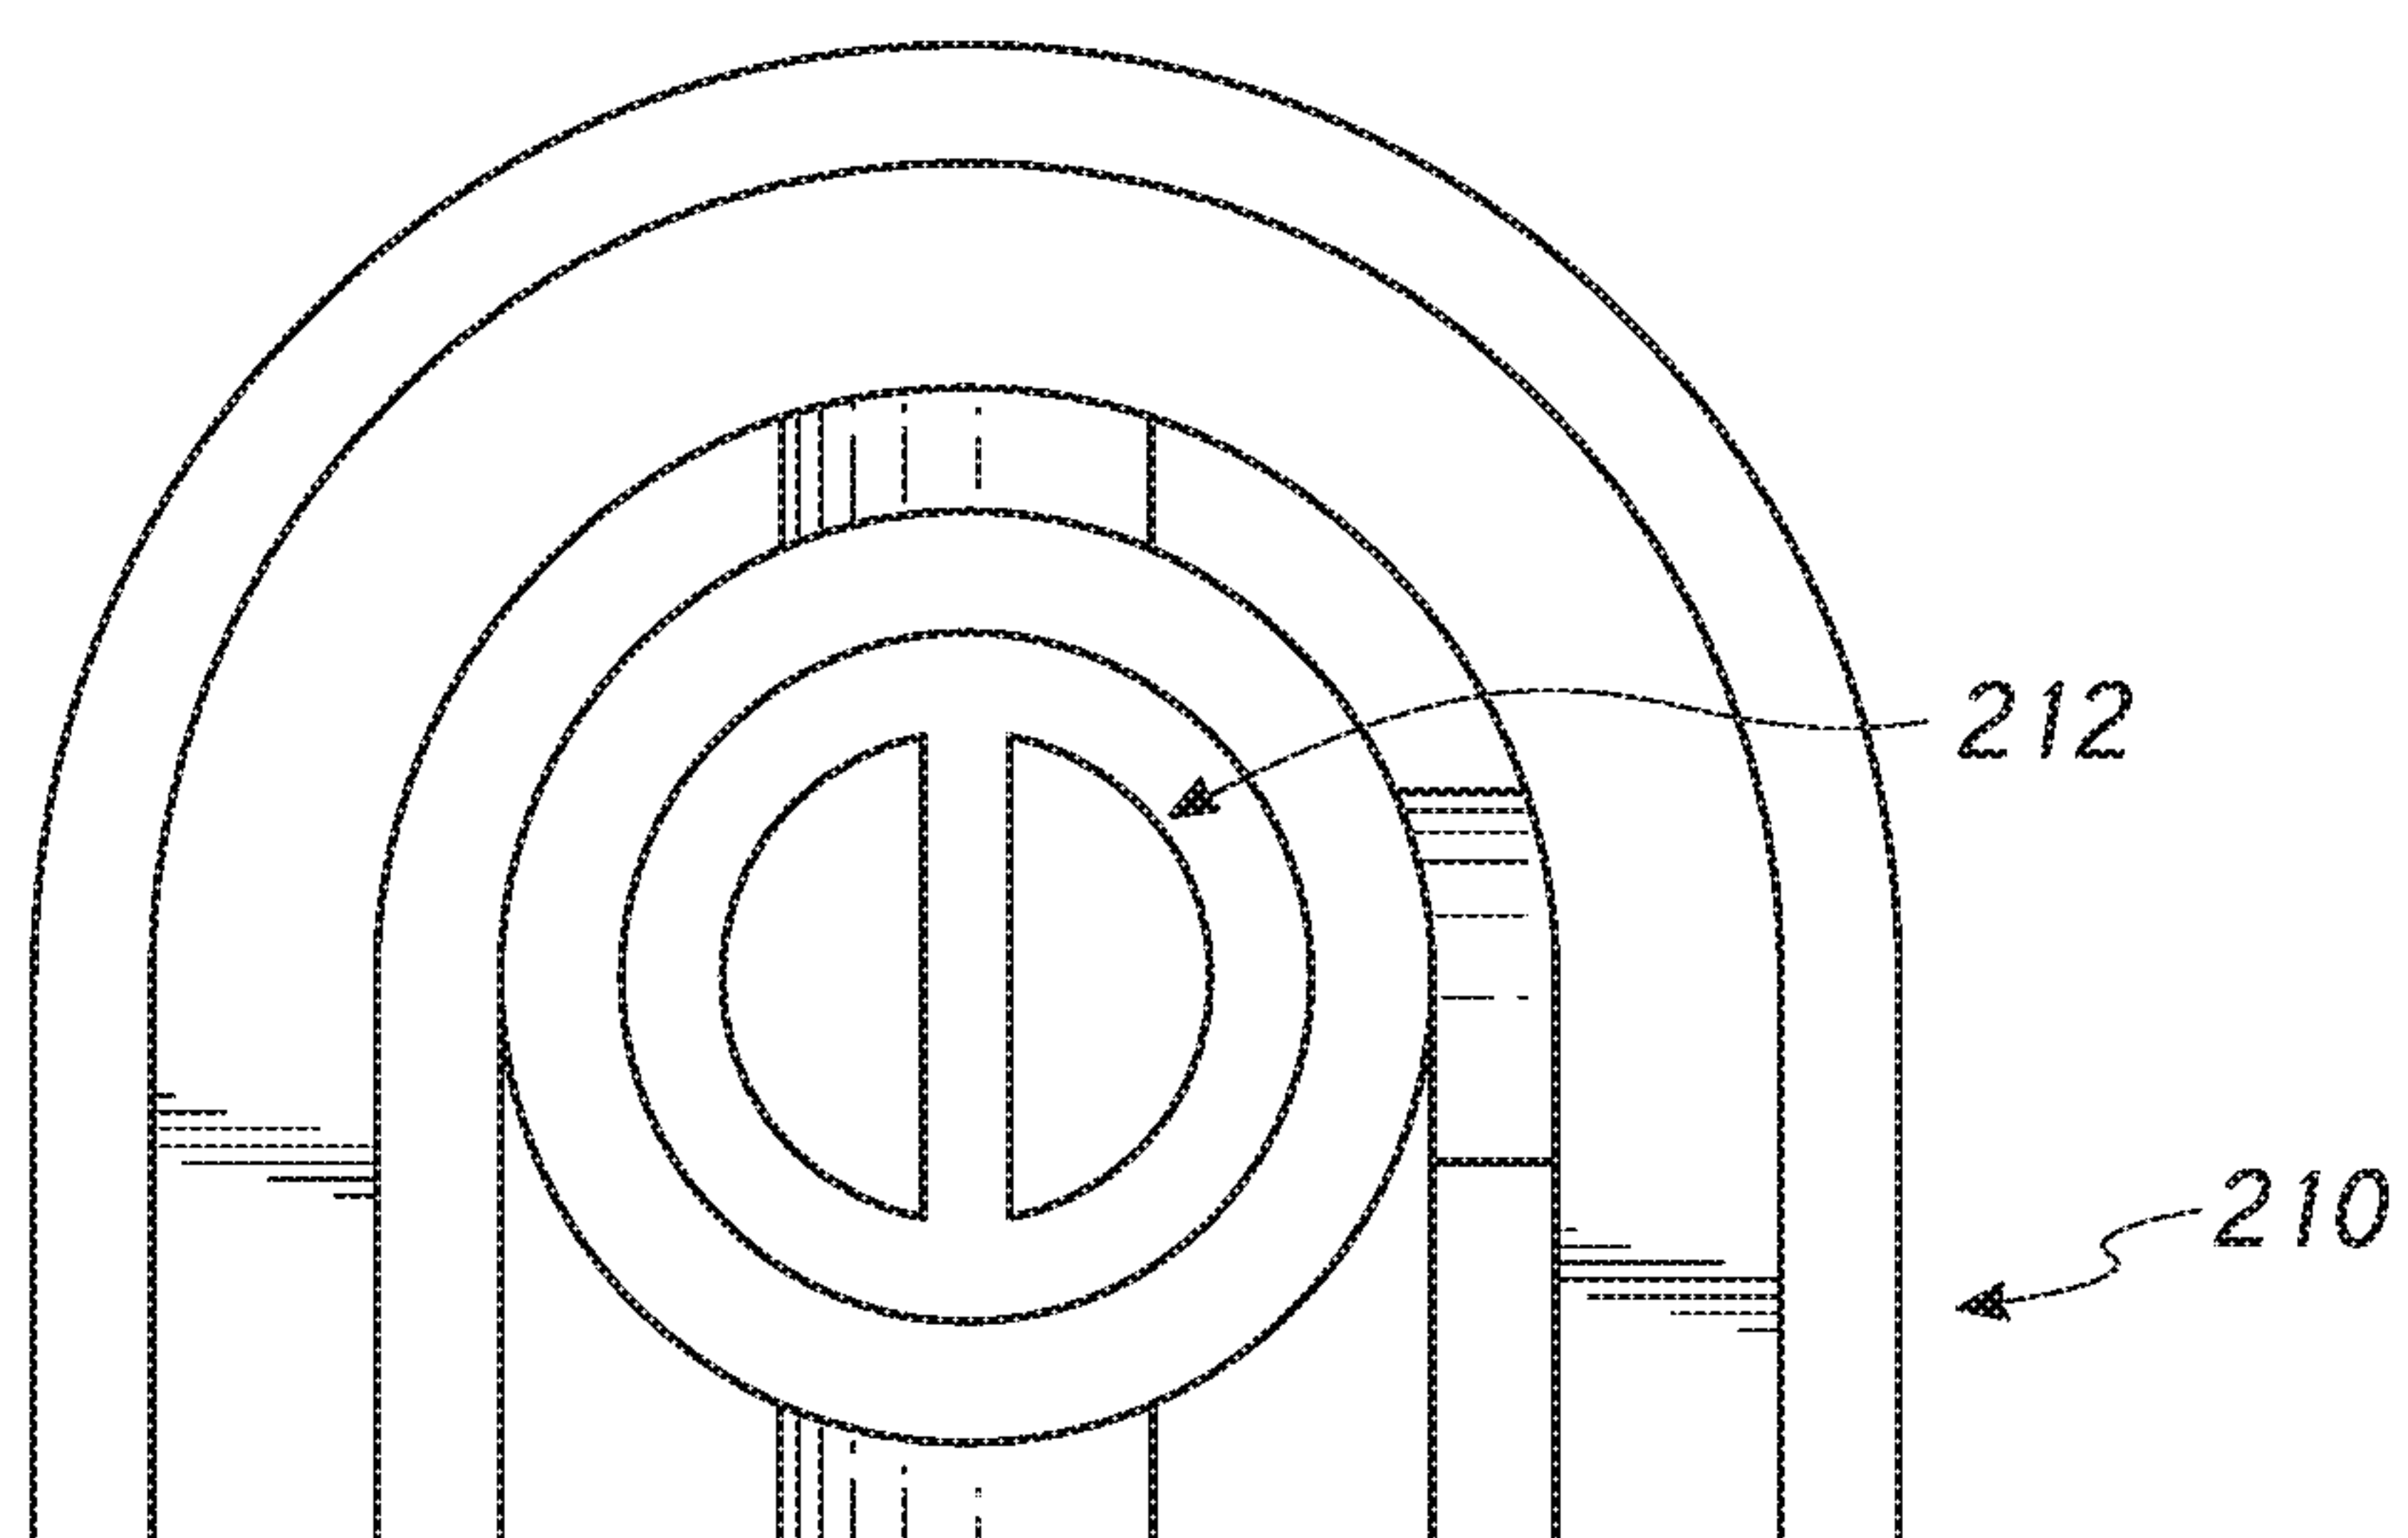
4/24


FIG. 2B_i

5/24


FIG. 2C_i

6/24

*FIG. 2D,*

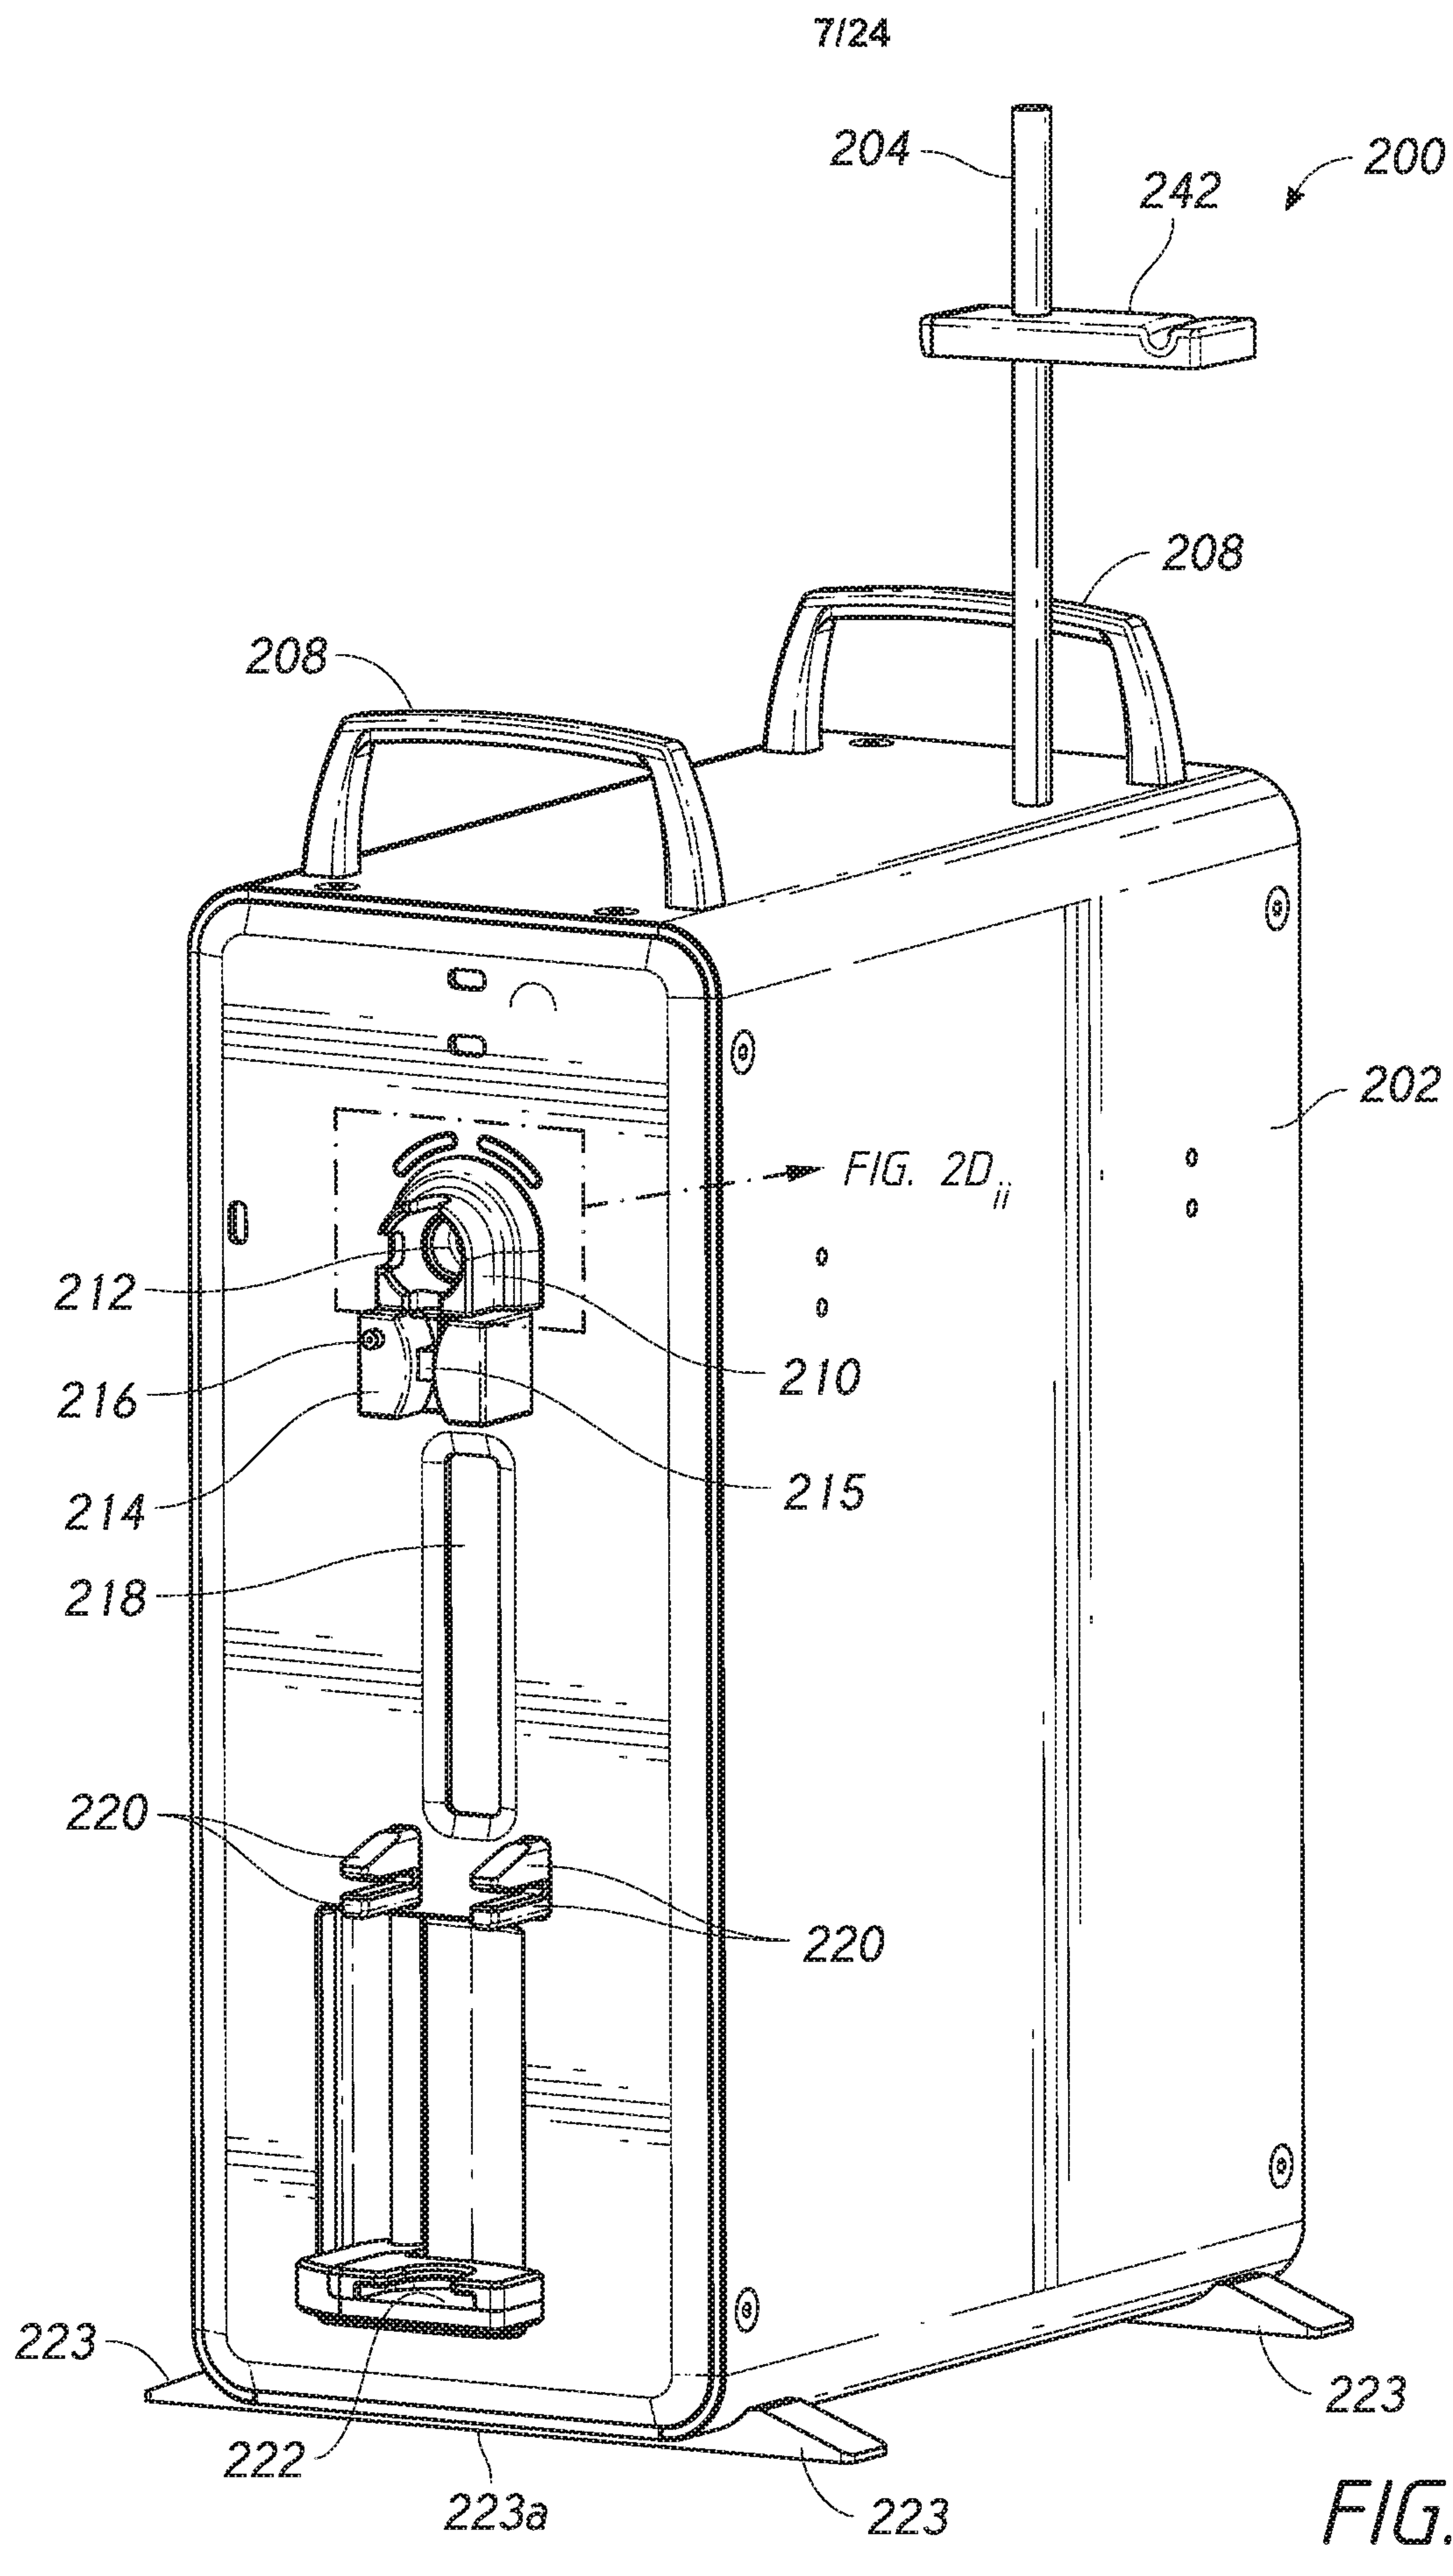

8/24

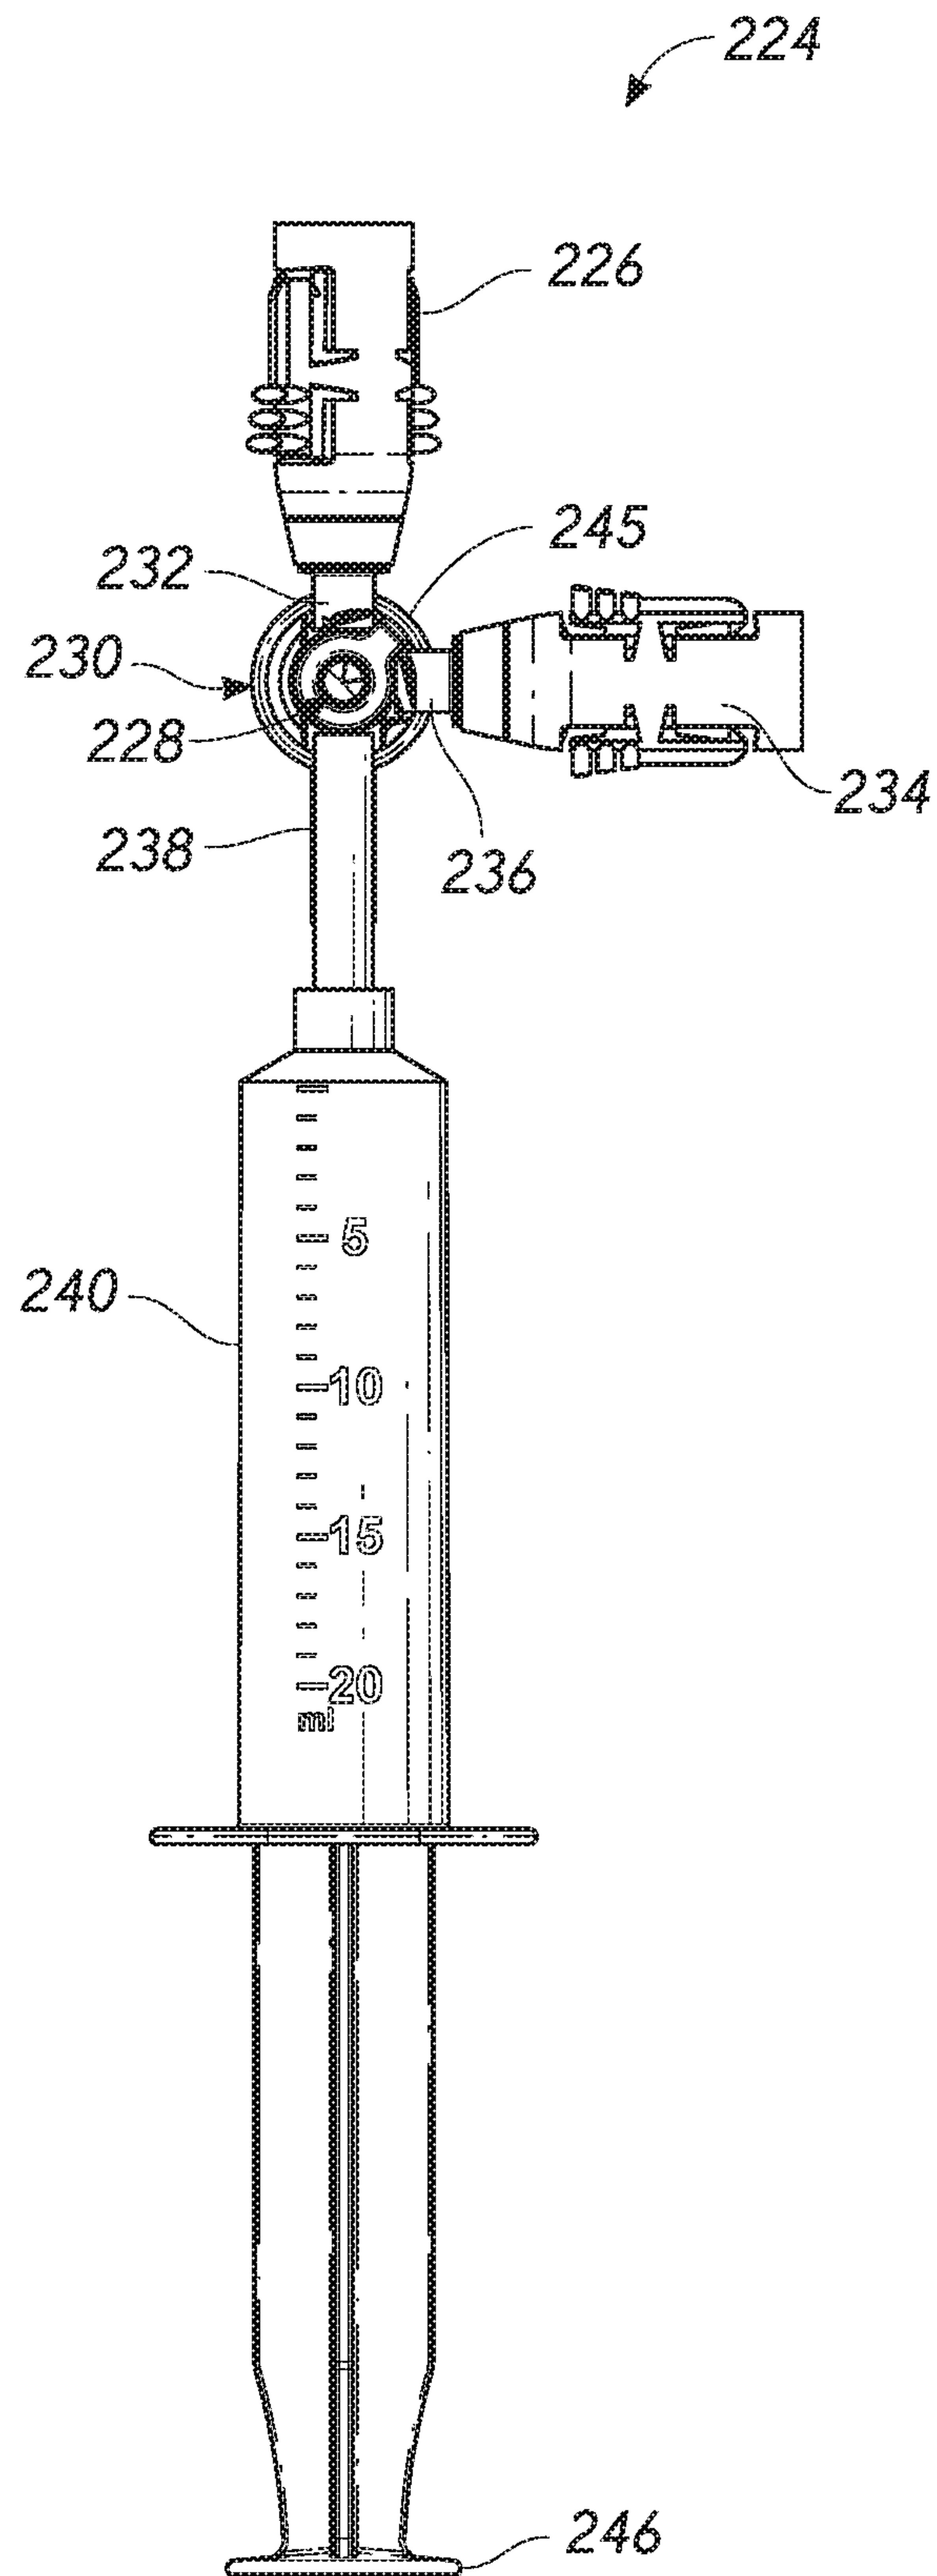FIG. 2B_{ii}

9/24

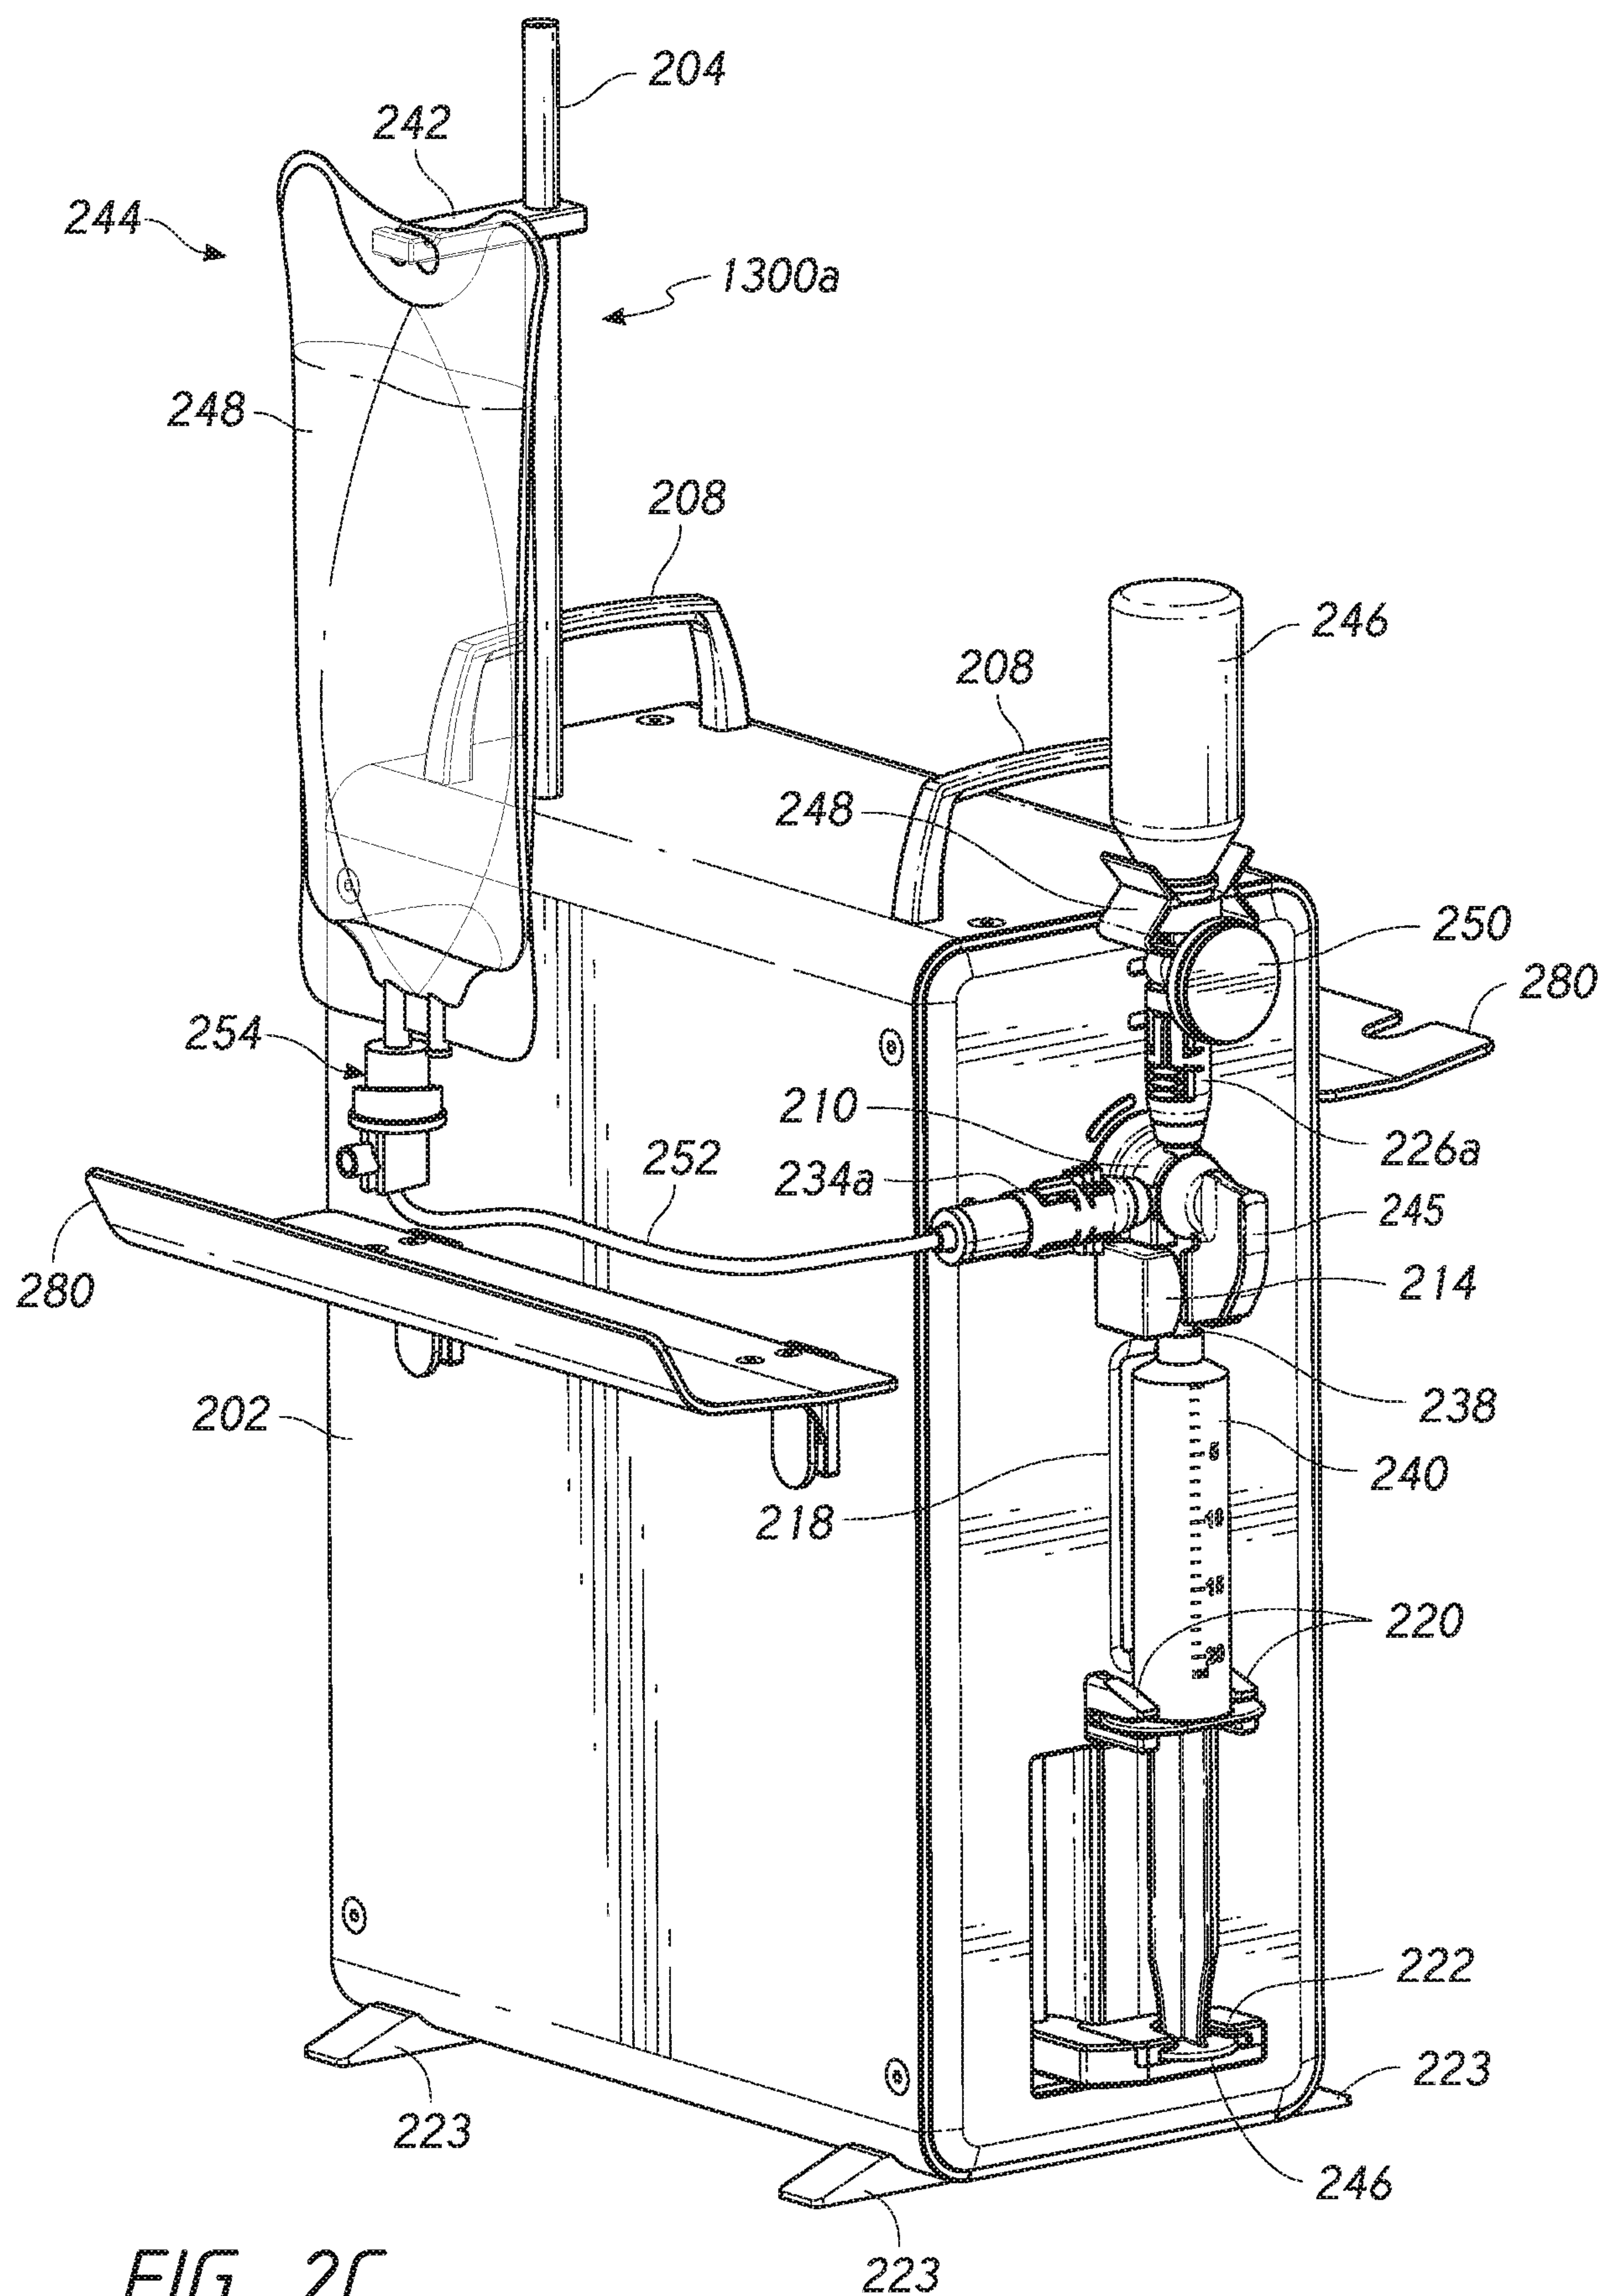
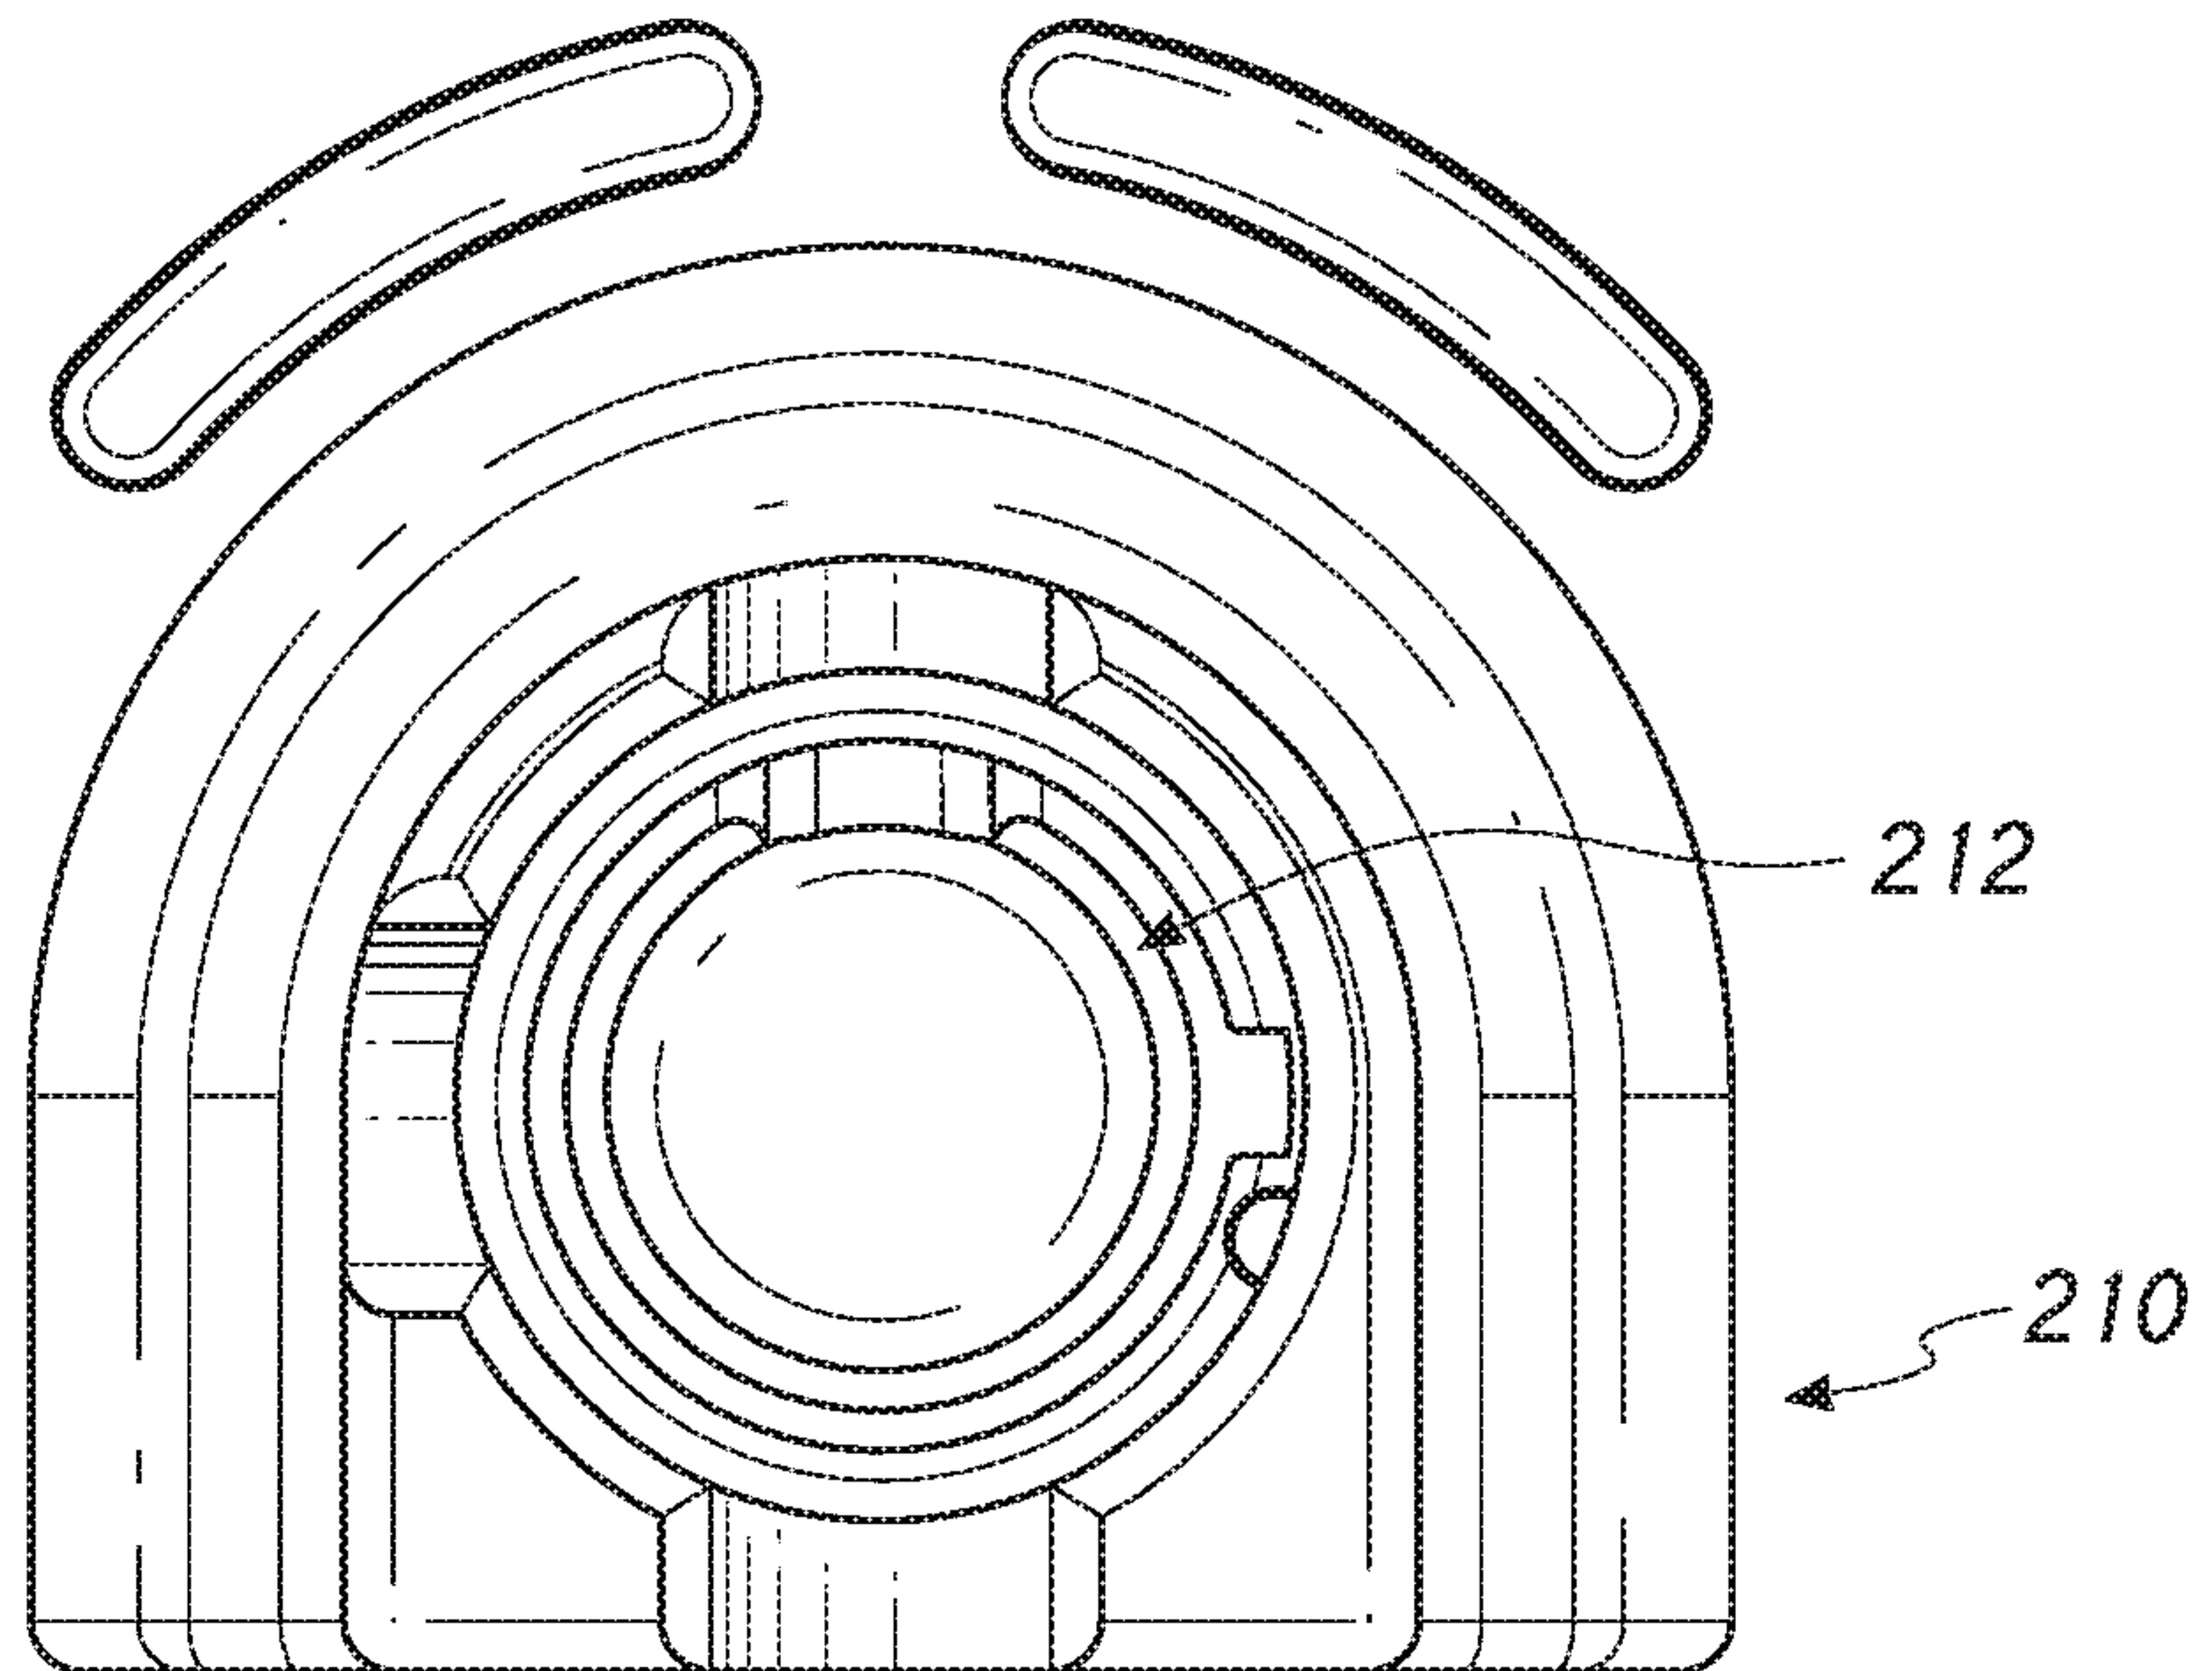
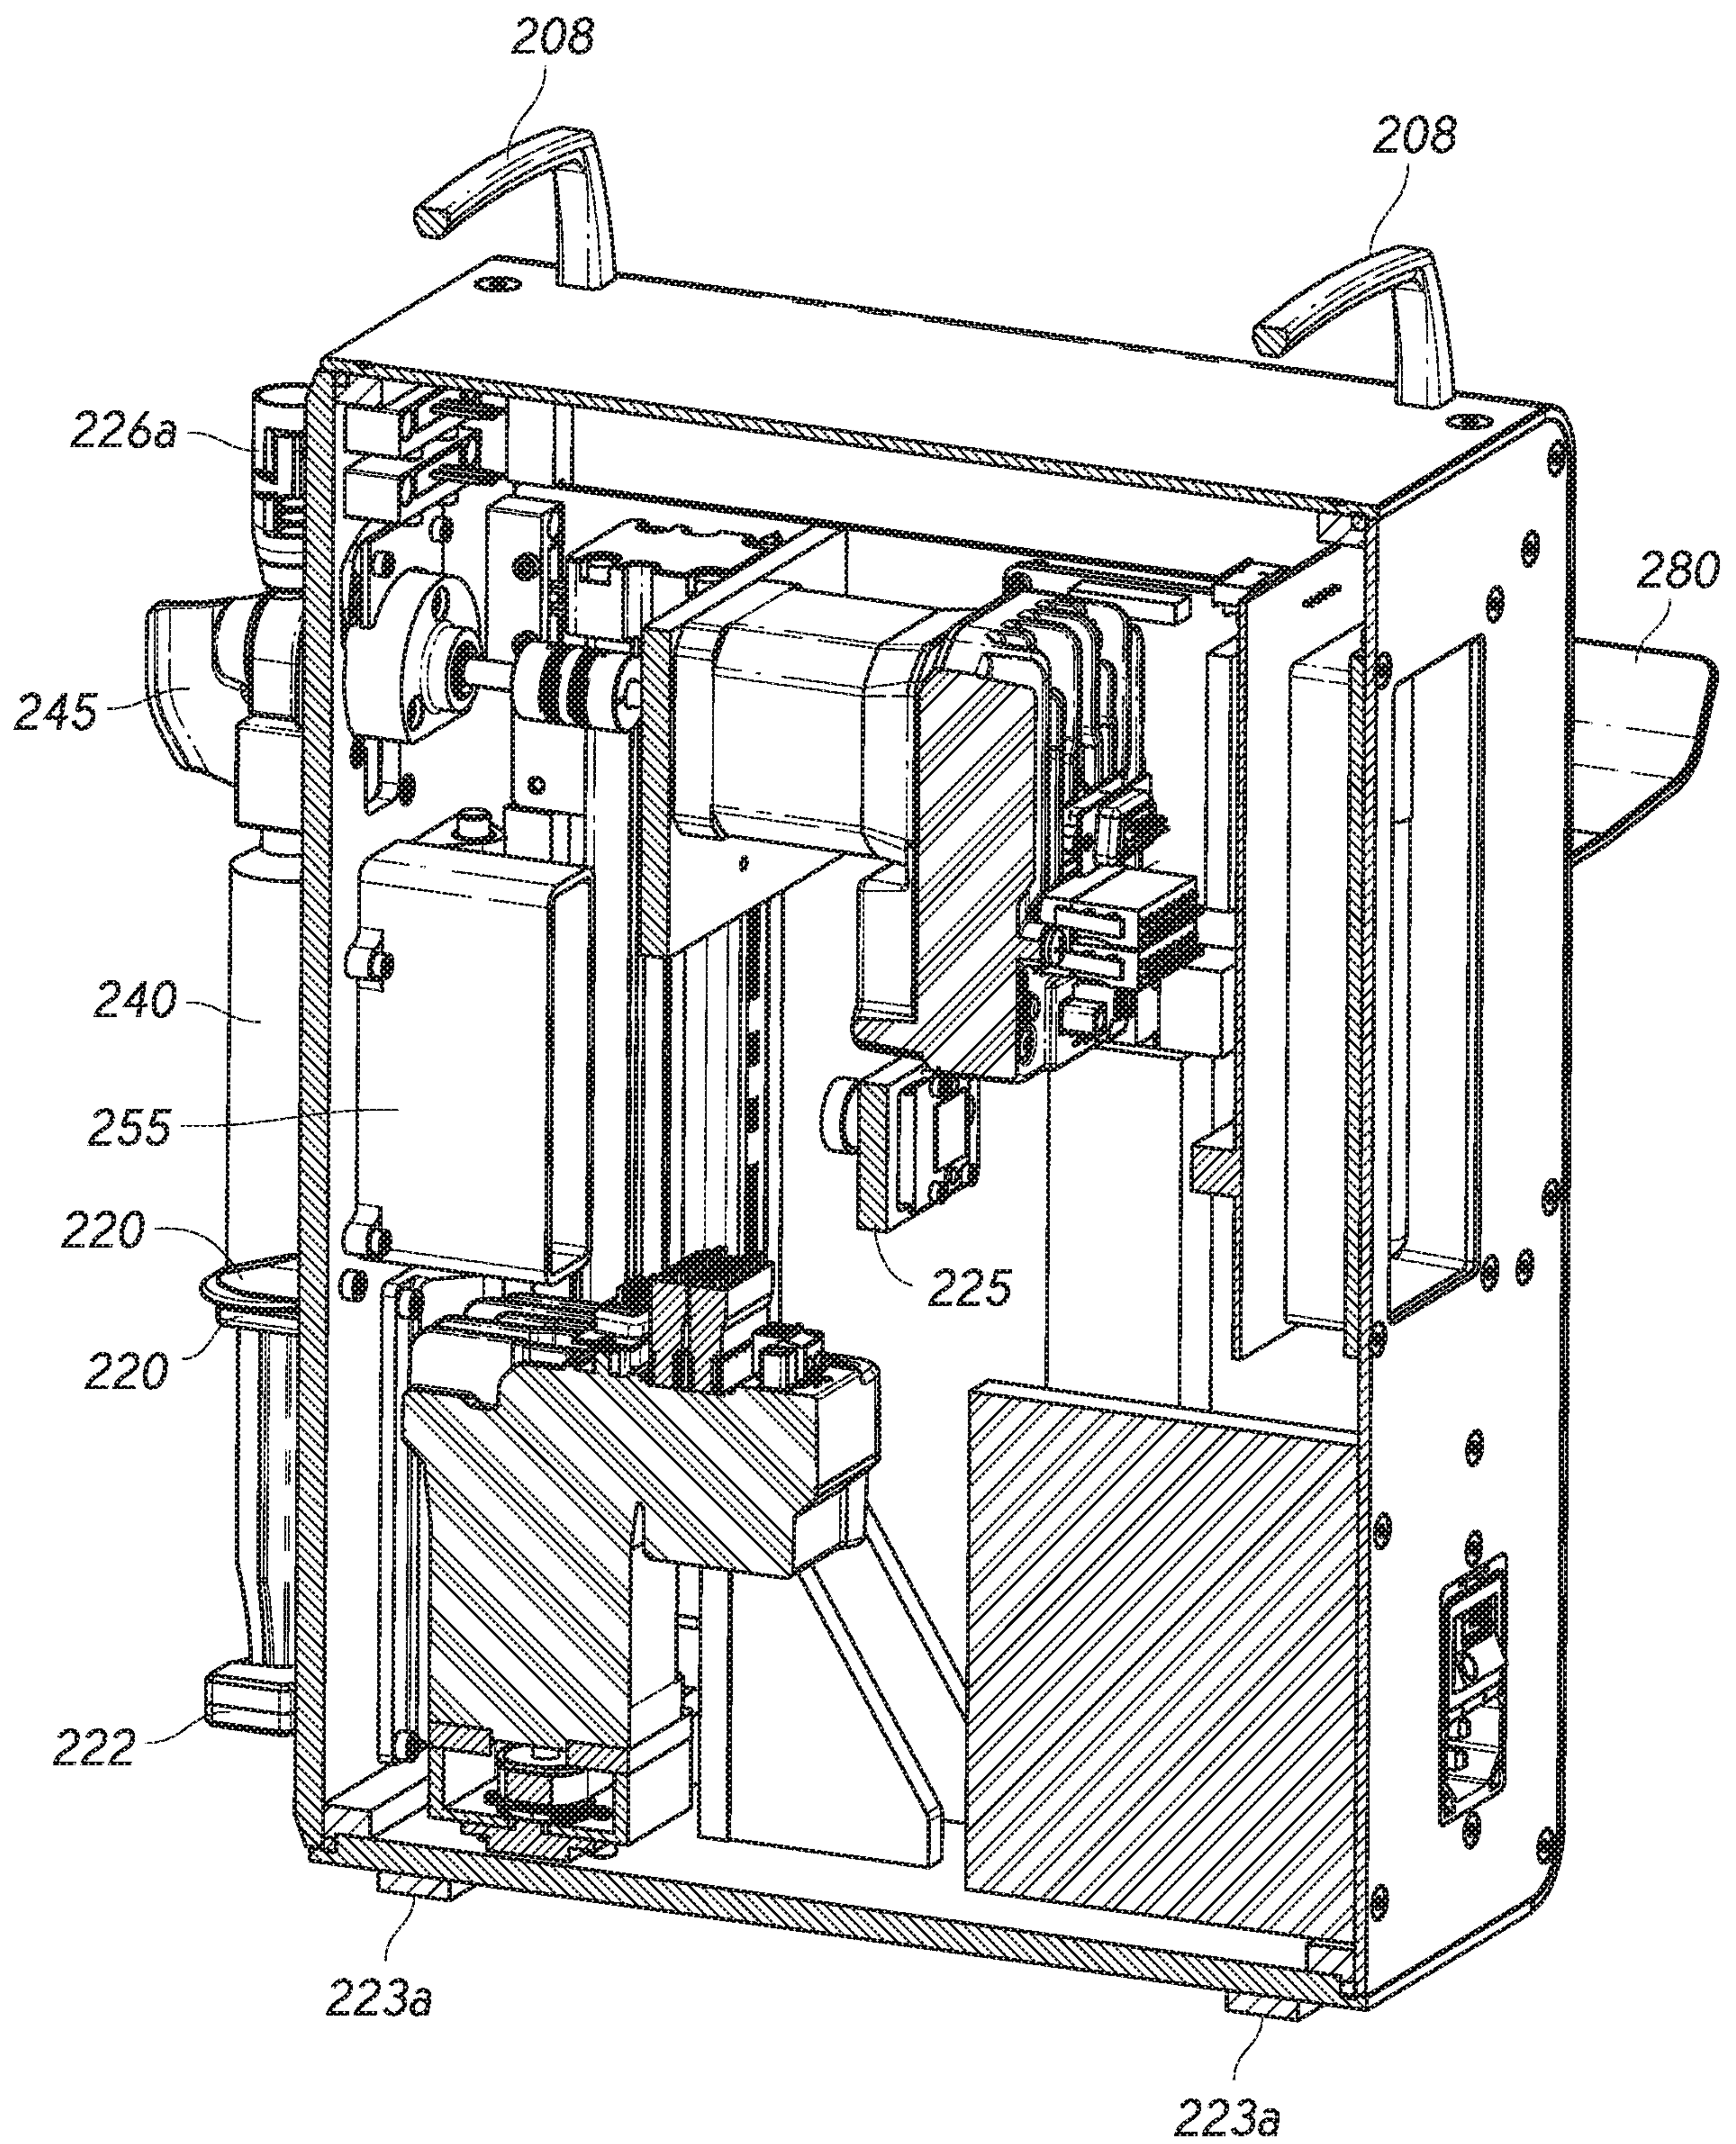


FIG. 2C_{ii}

10/24

*FIG. 2D_{ii}*

11/24

FIG. 2E_{ii}

12/24

78

Admin

New Order

Logout

Pharmacist

John Tag

Scan or Enter Order

Order Number

2

Drug Name

le. doconexent and icosapent

Volume

18mL

NDC

Order Number 2

Drug Name

doconexent and icosapent

Lot Number

NDC 2

Volume 18

Lot Exp Date

Lot Number 1

Lot Exp Date 28/2015

Prepared Date 28/2015

Prepared Time 1:00pm

Prepare By

Verified By

Repeat?



256

254

FIG. 3

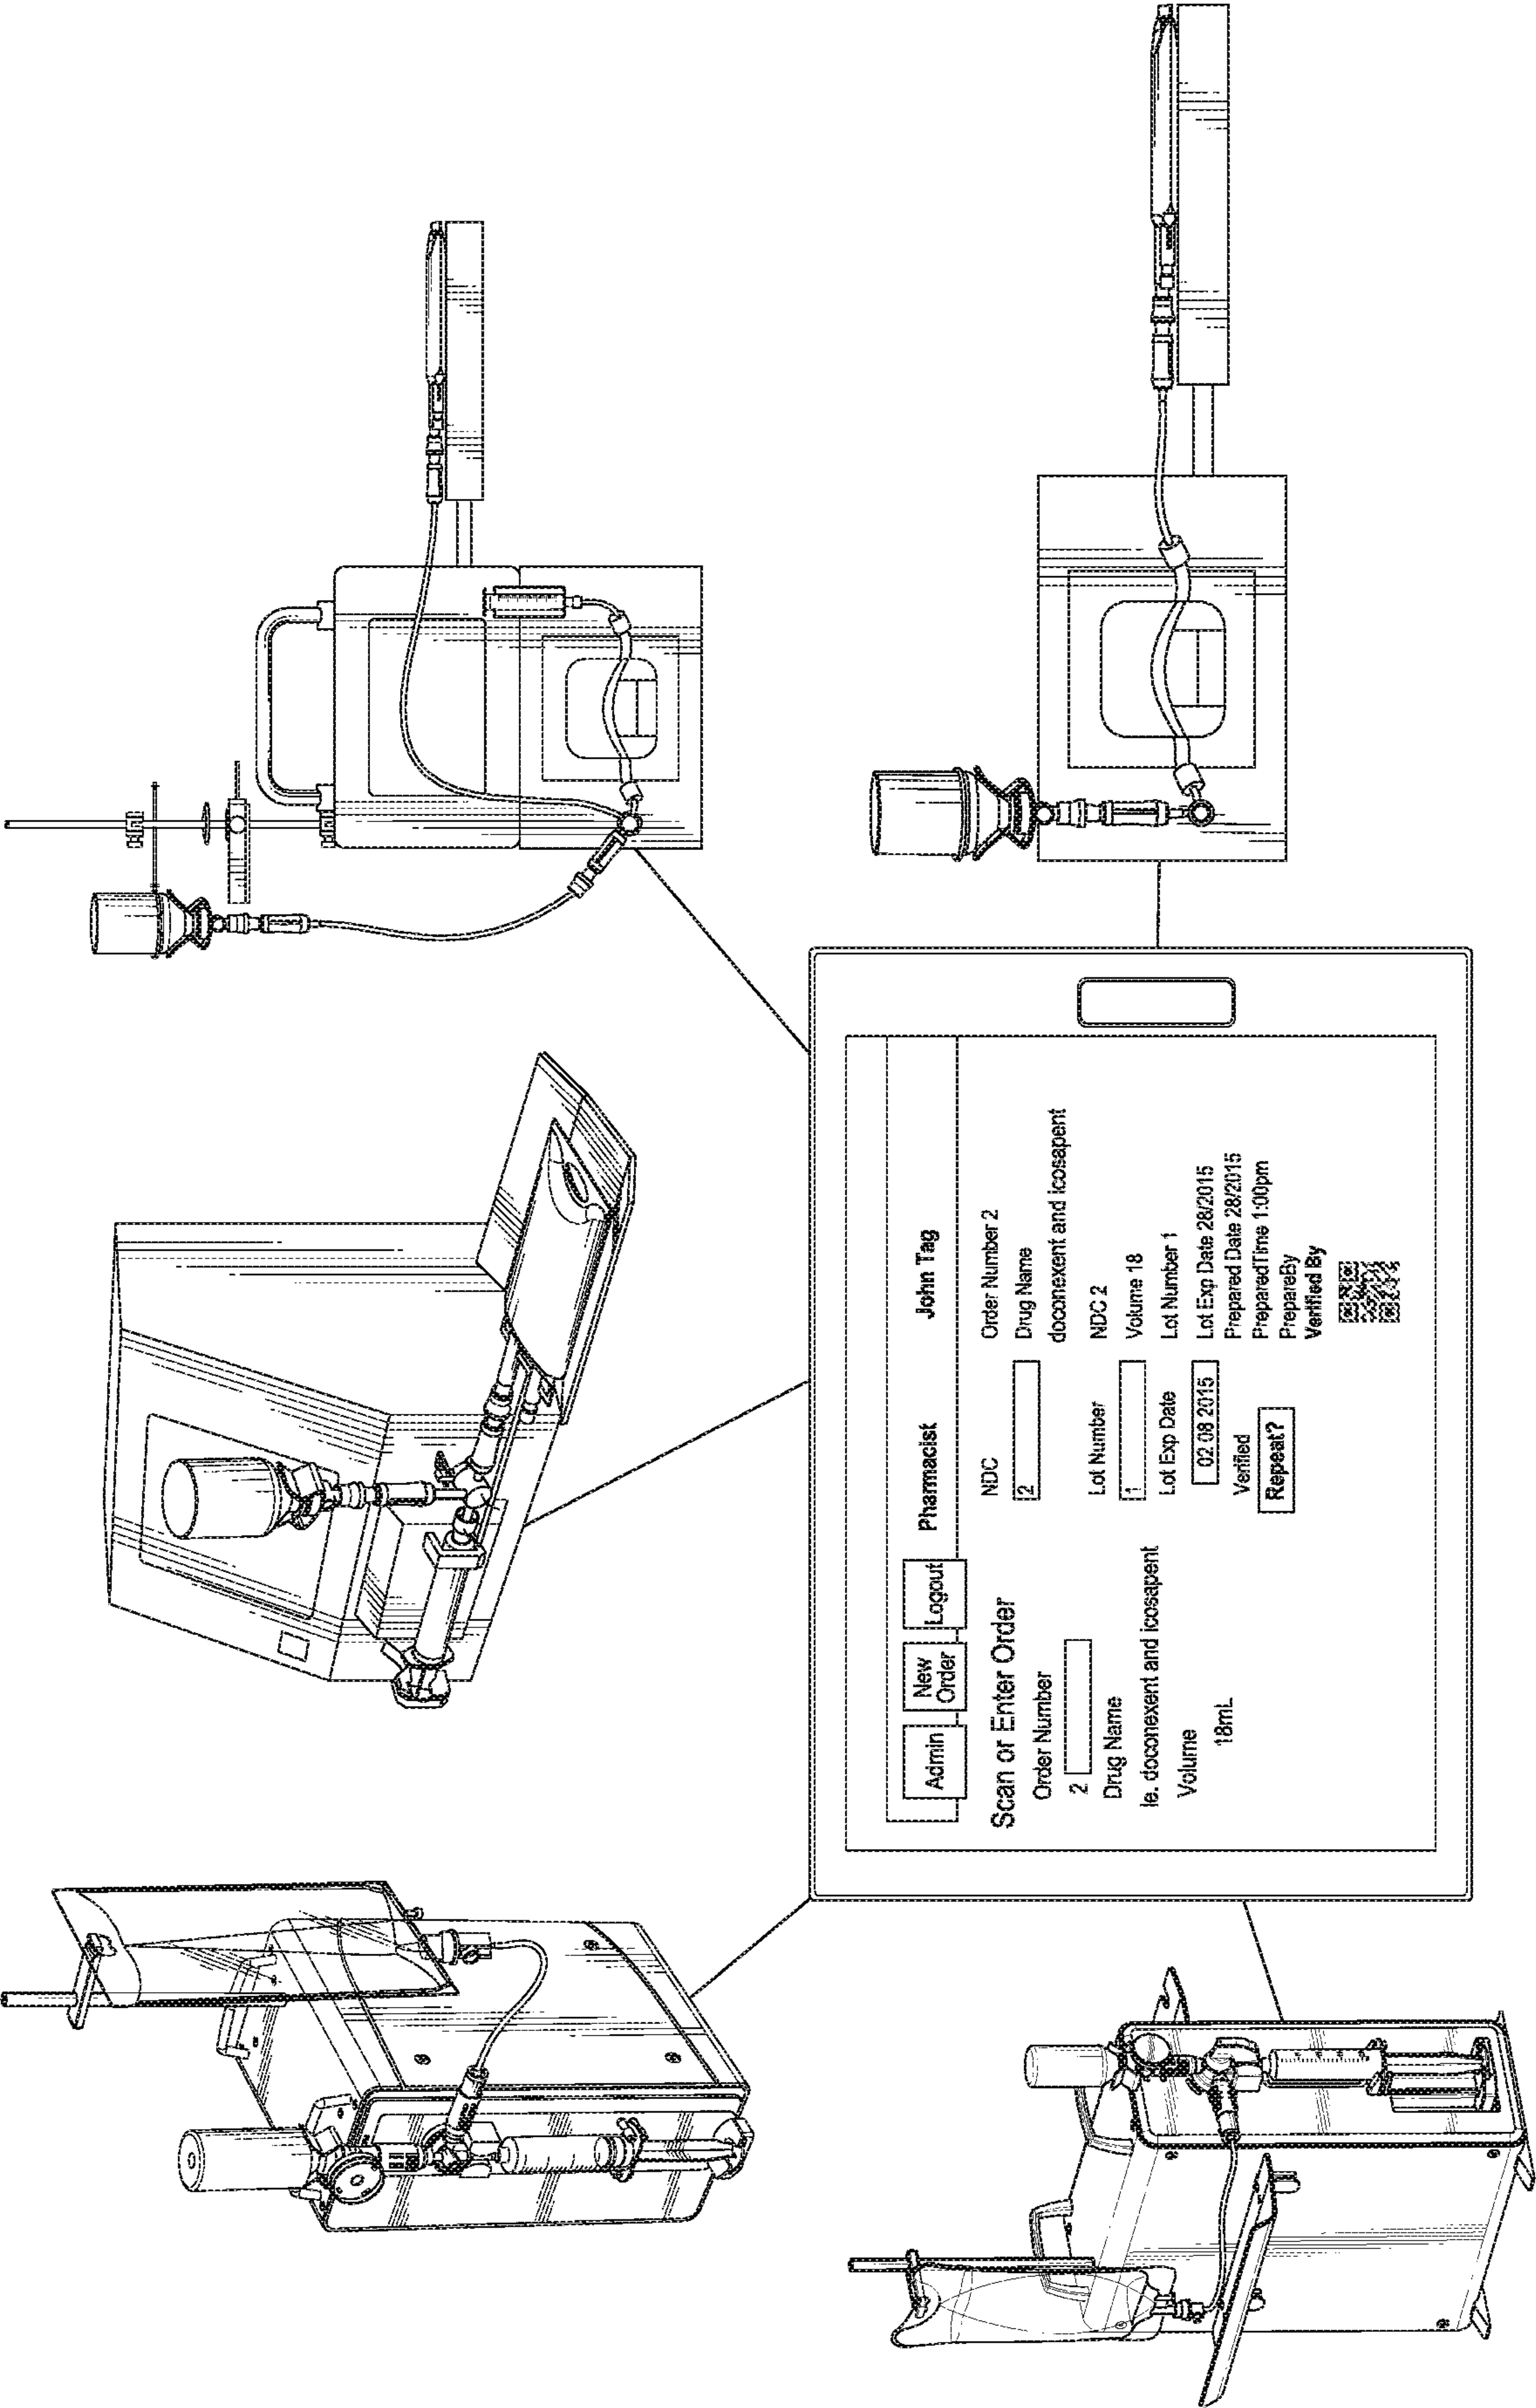


FIG. 4

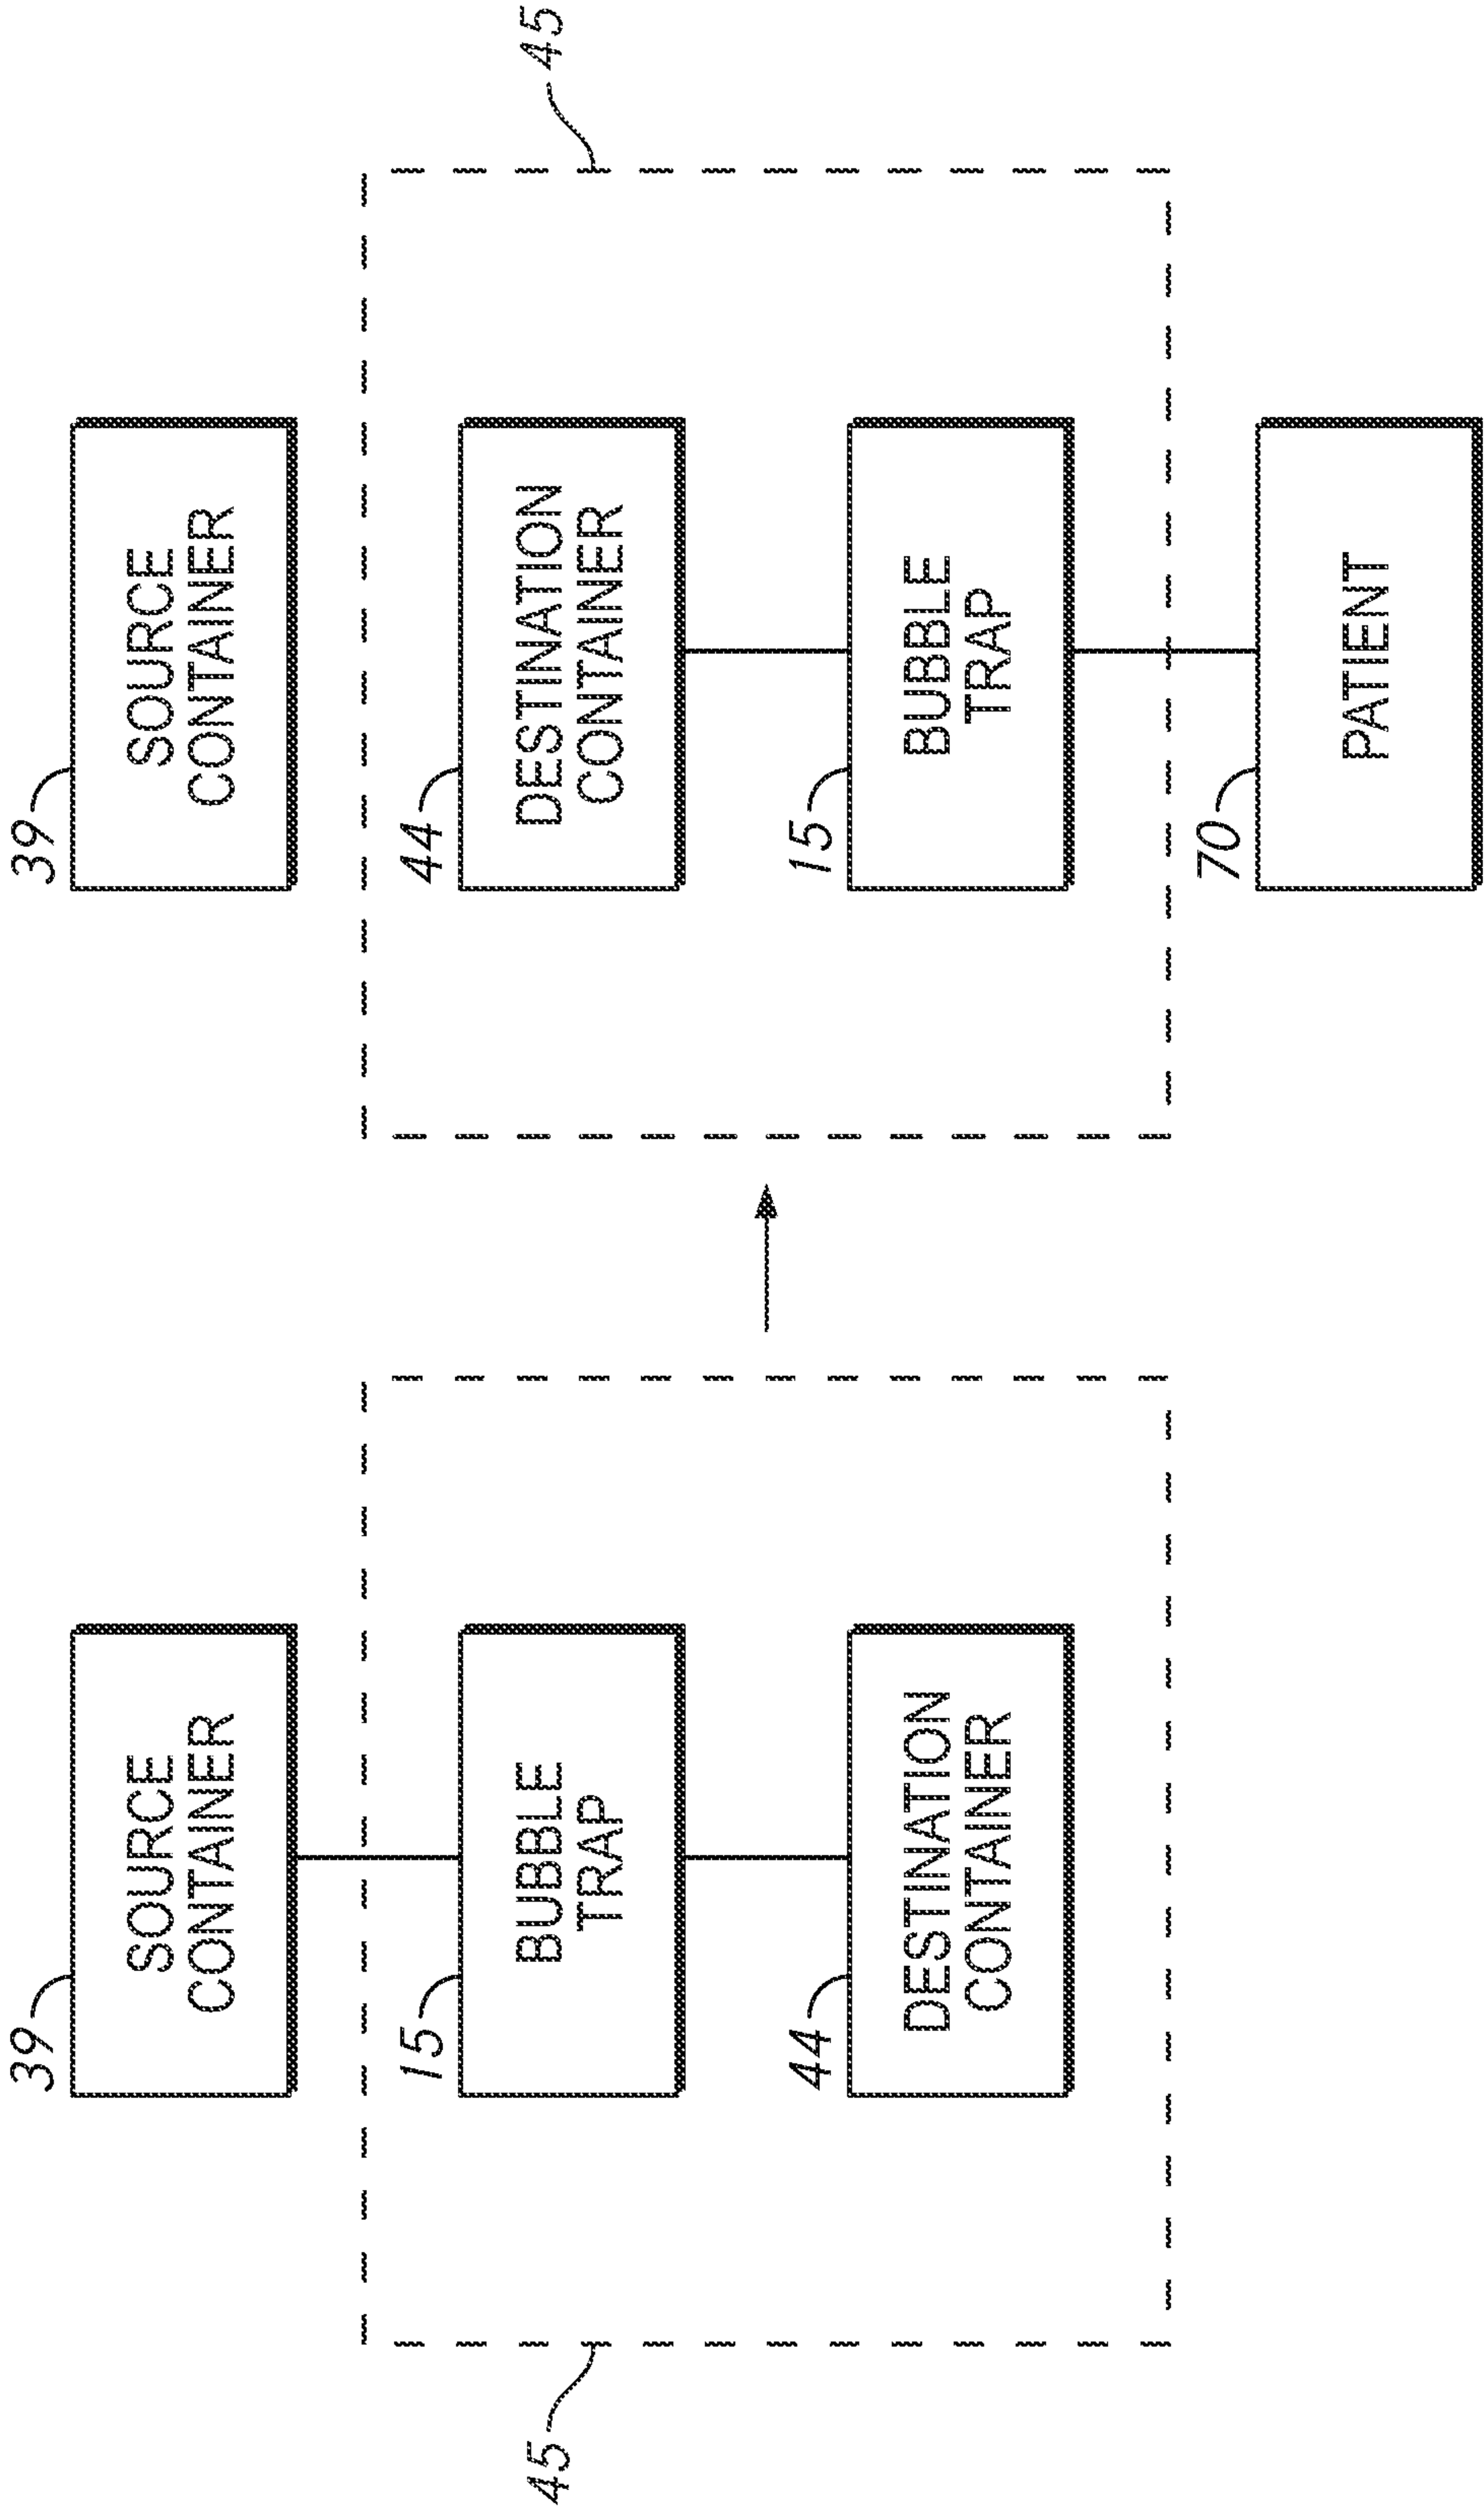


FIG. 5A

FIG. 5B

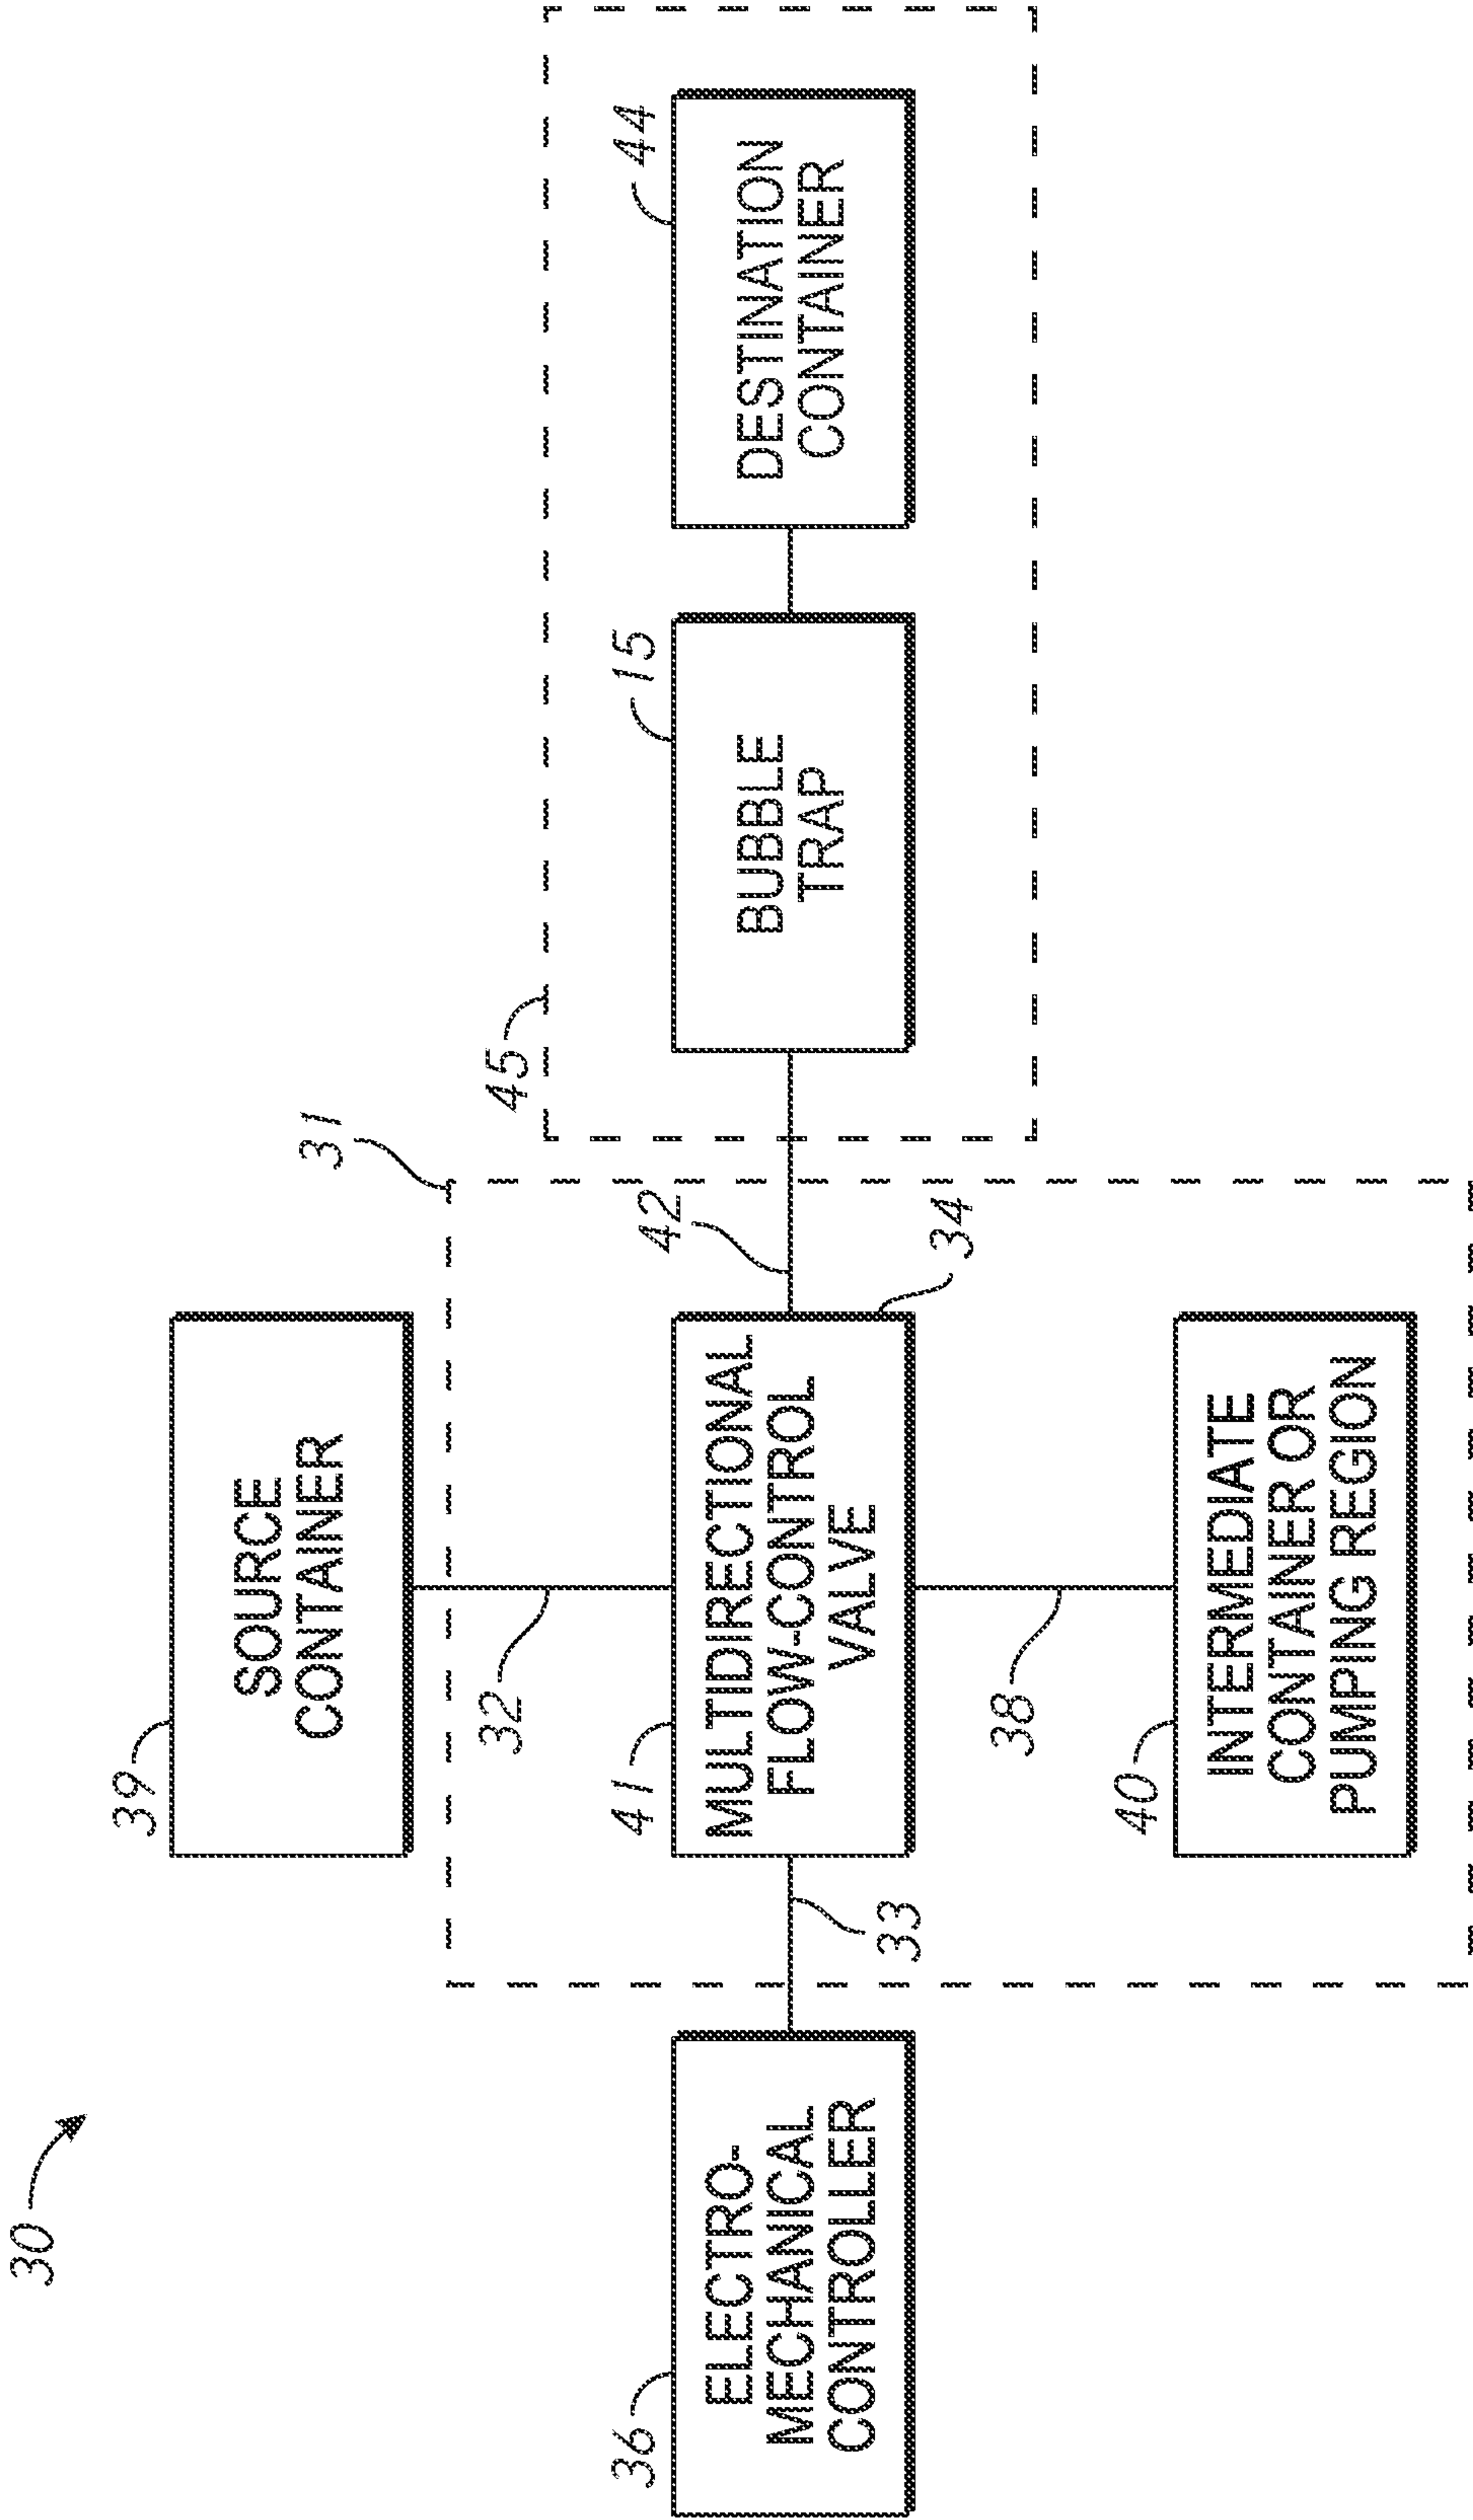


FIG. 5C

16/24

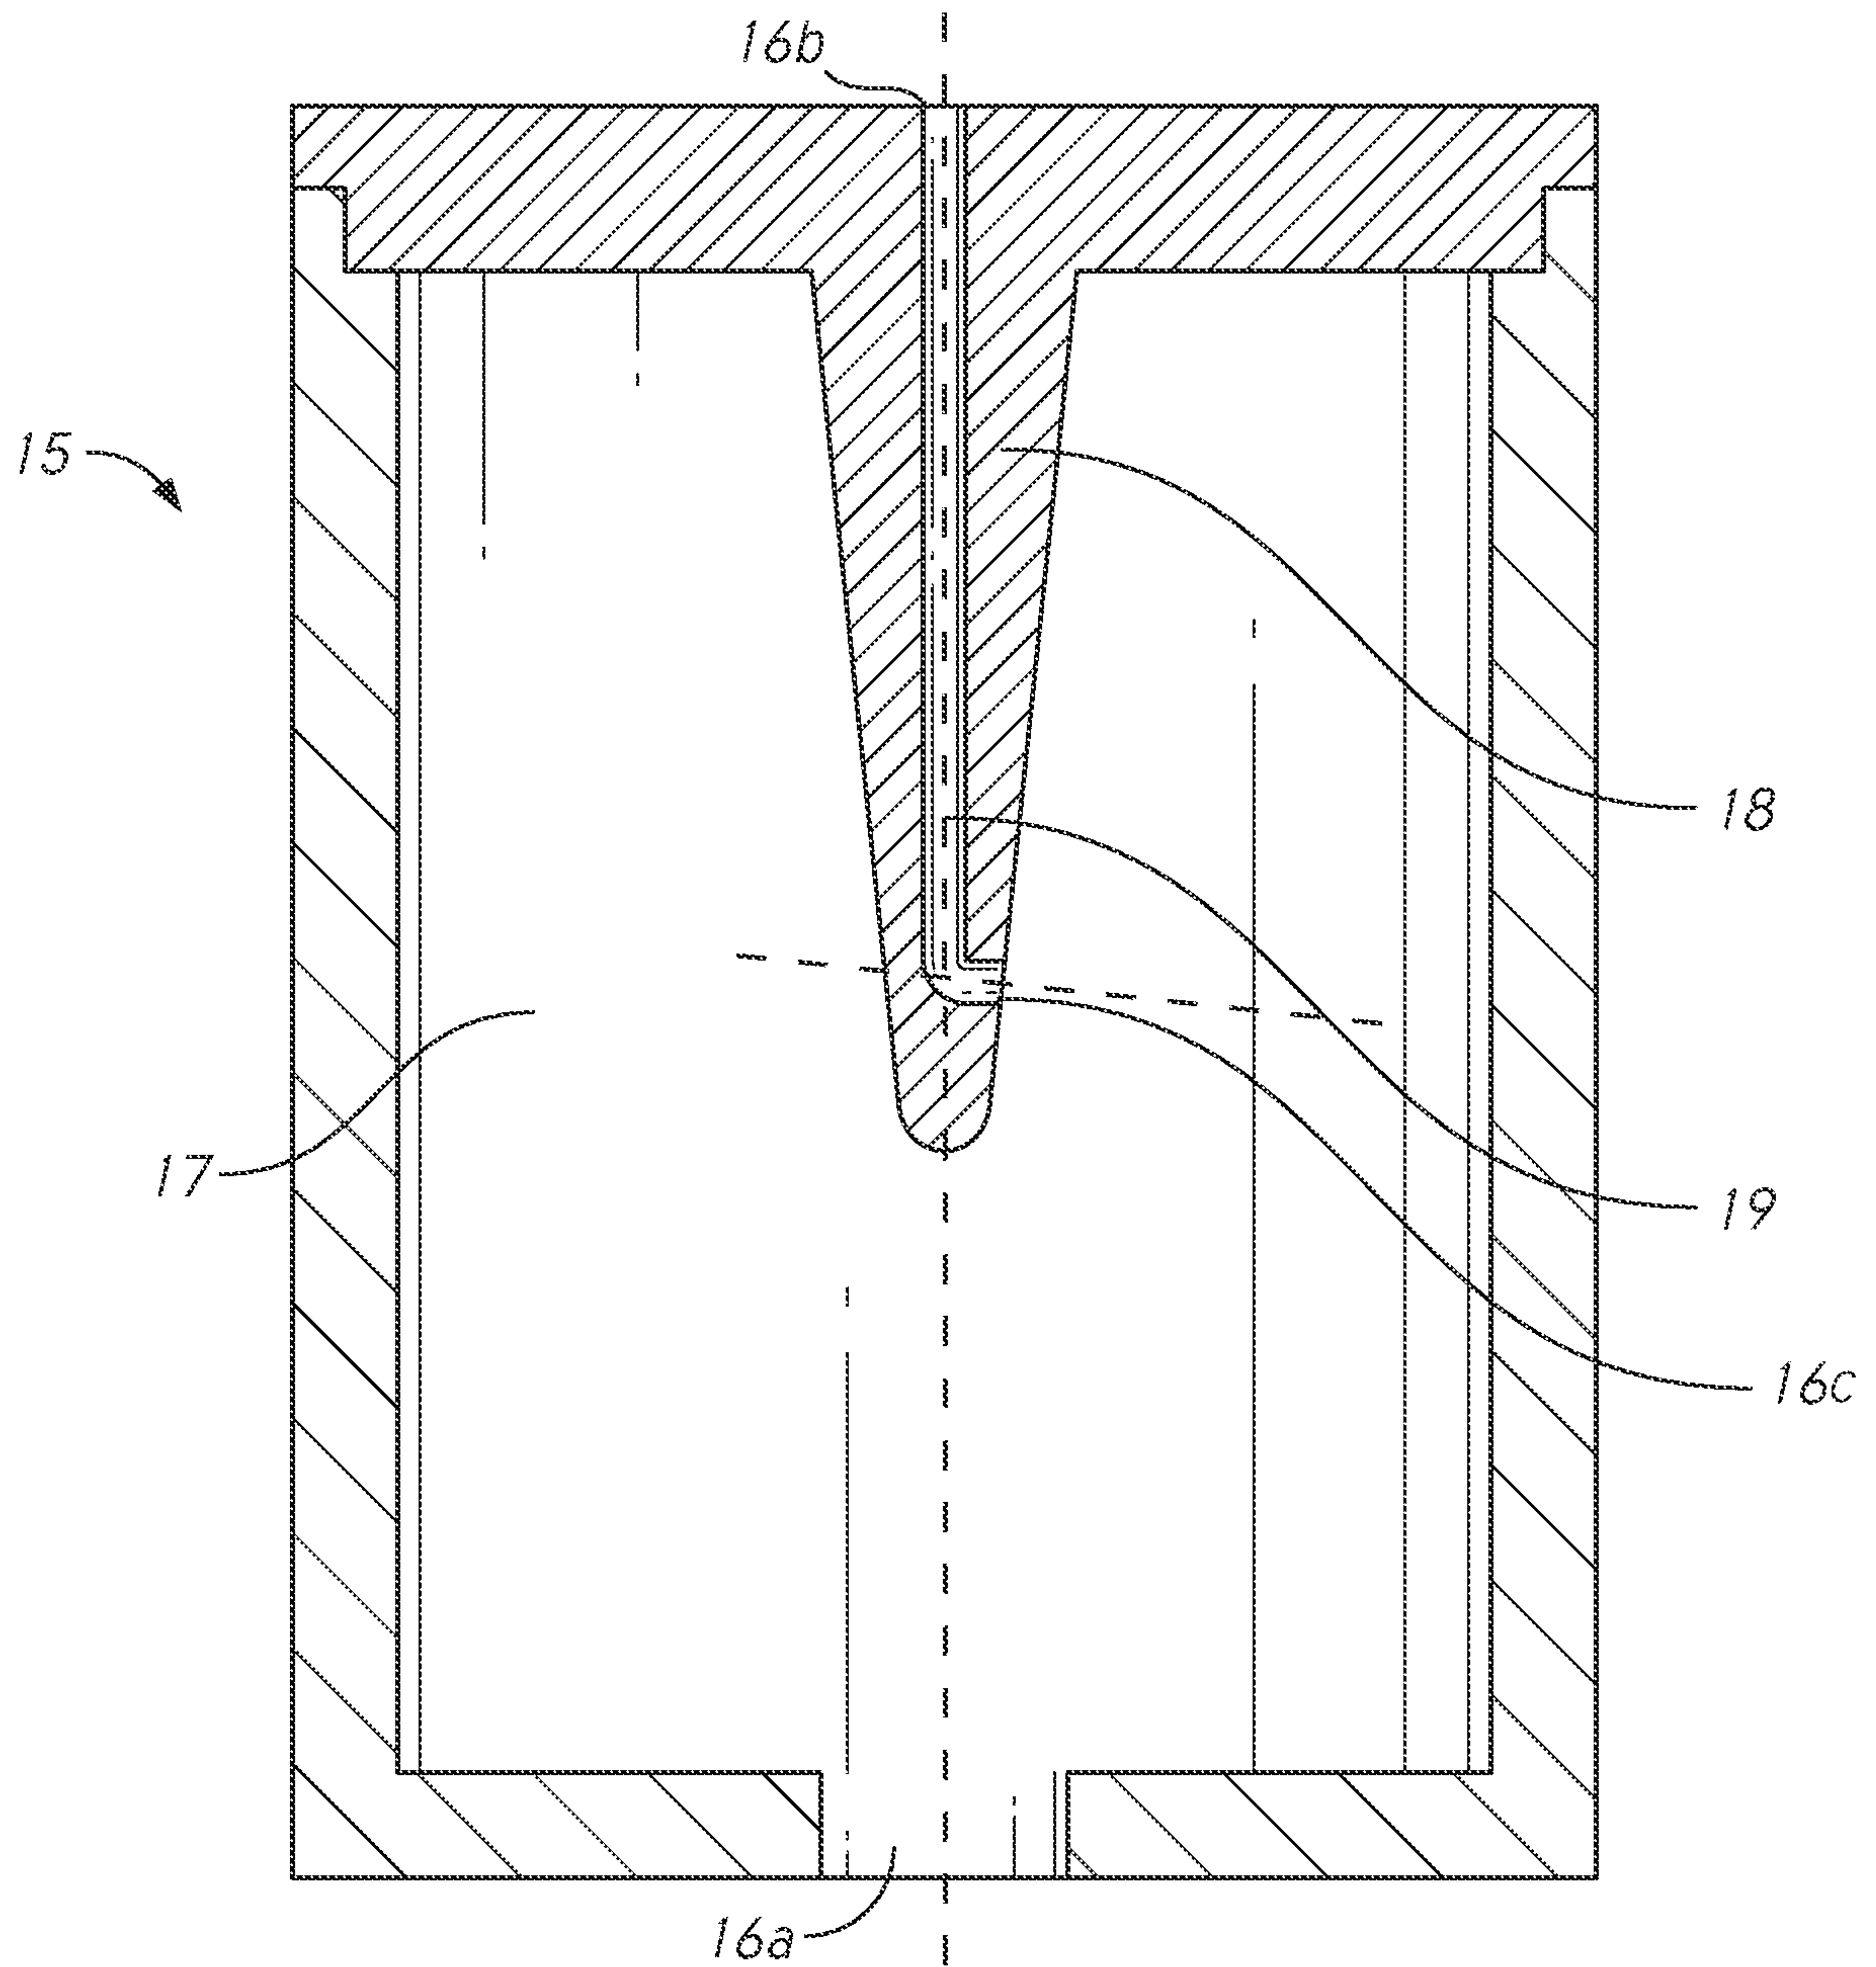


FIG. 6A

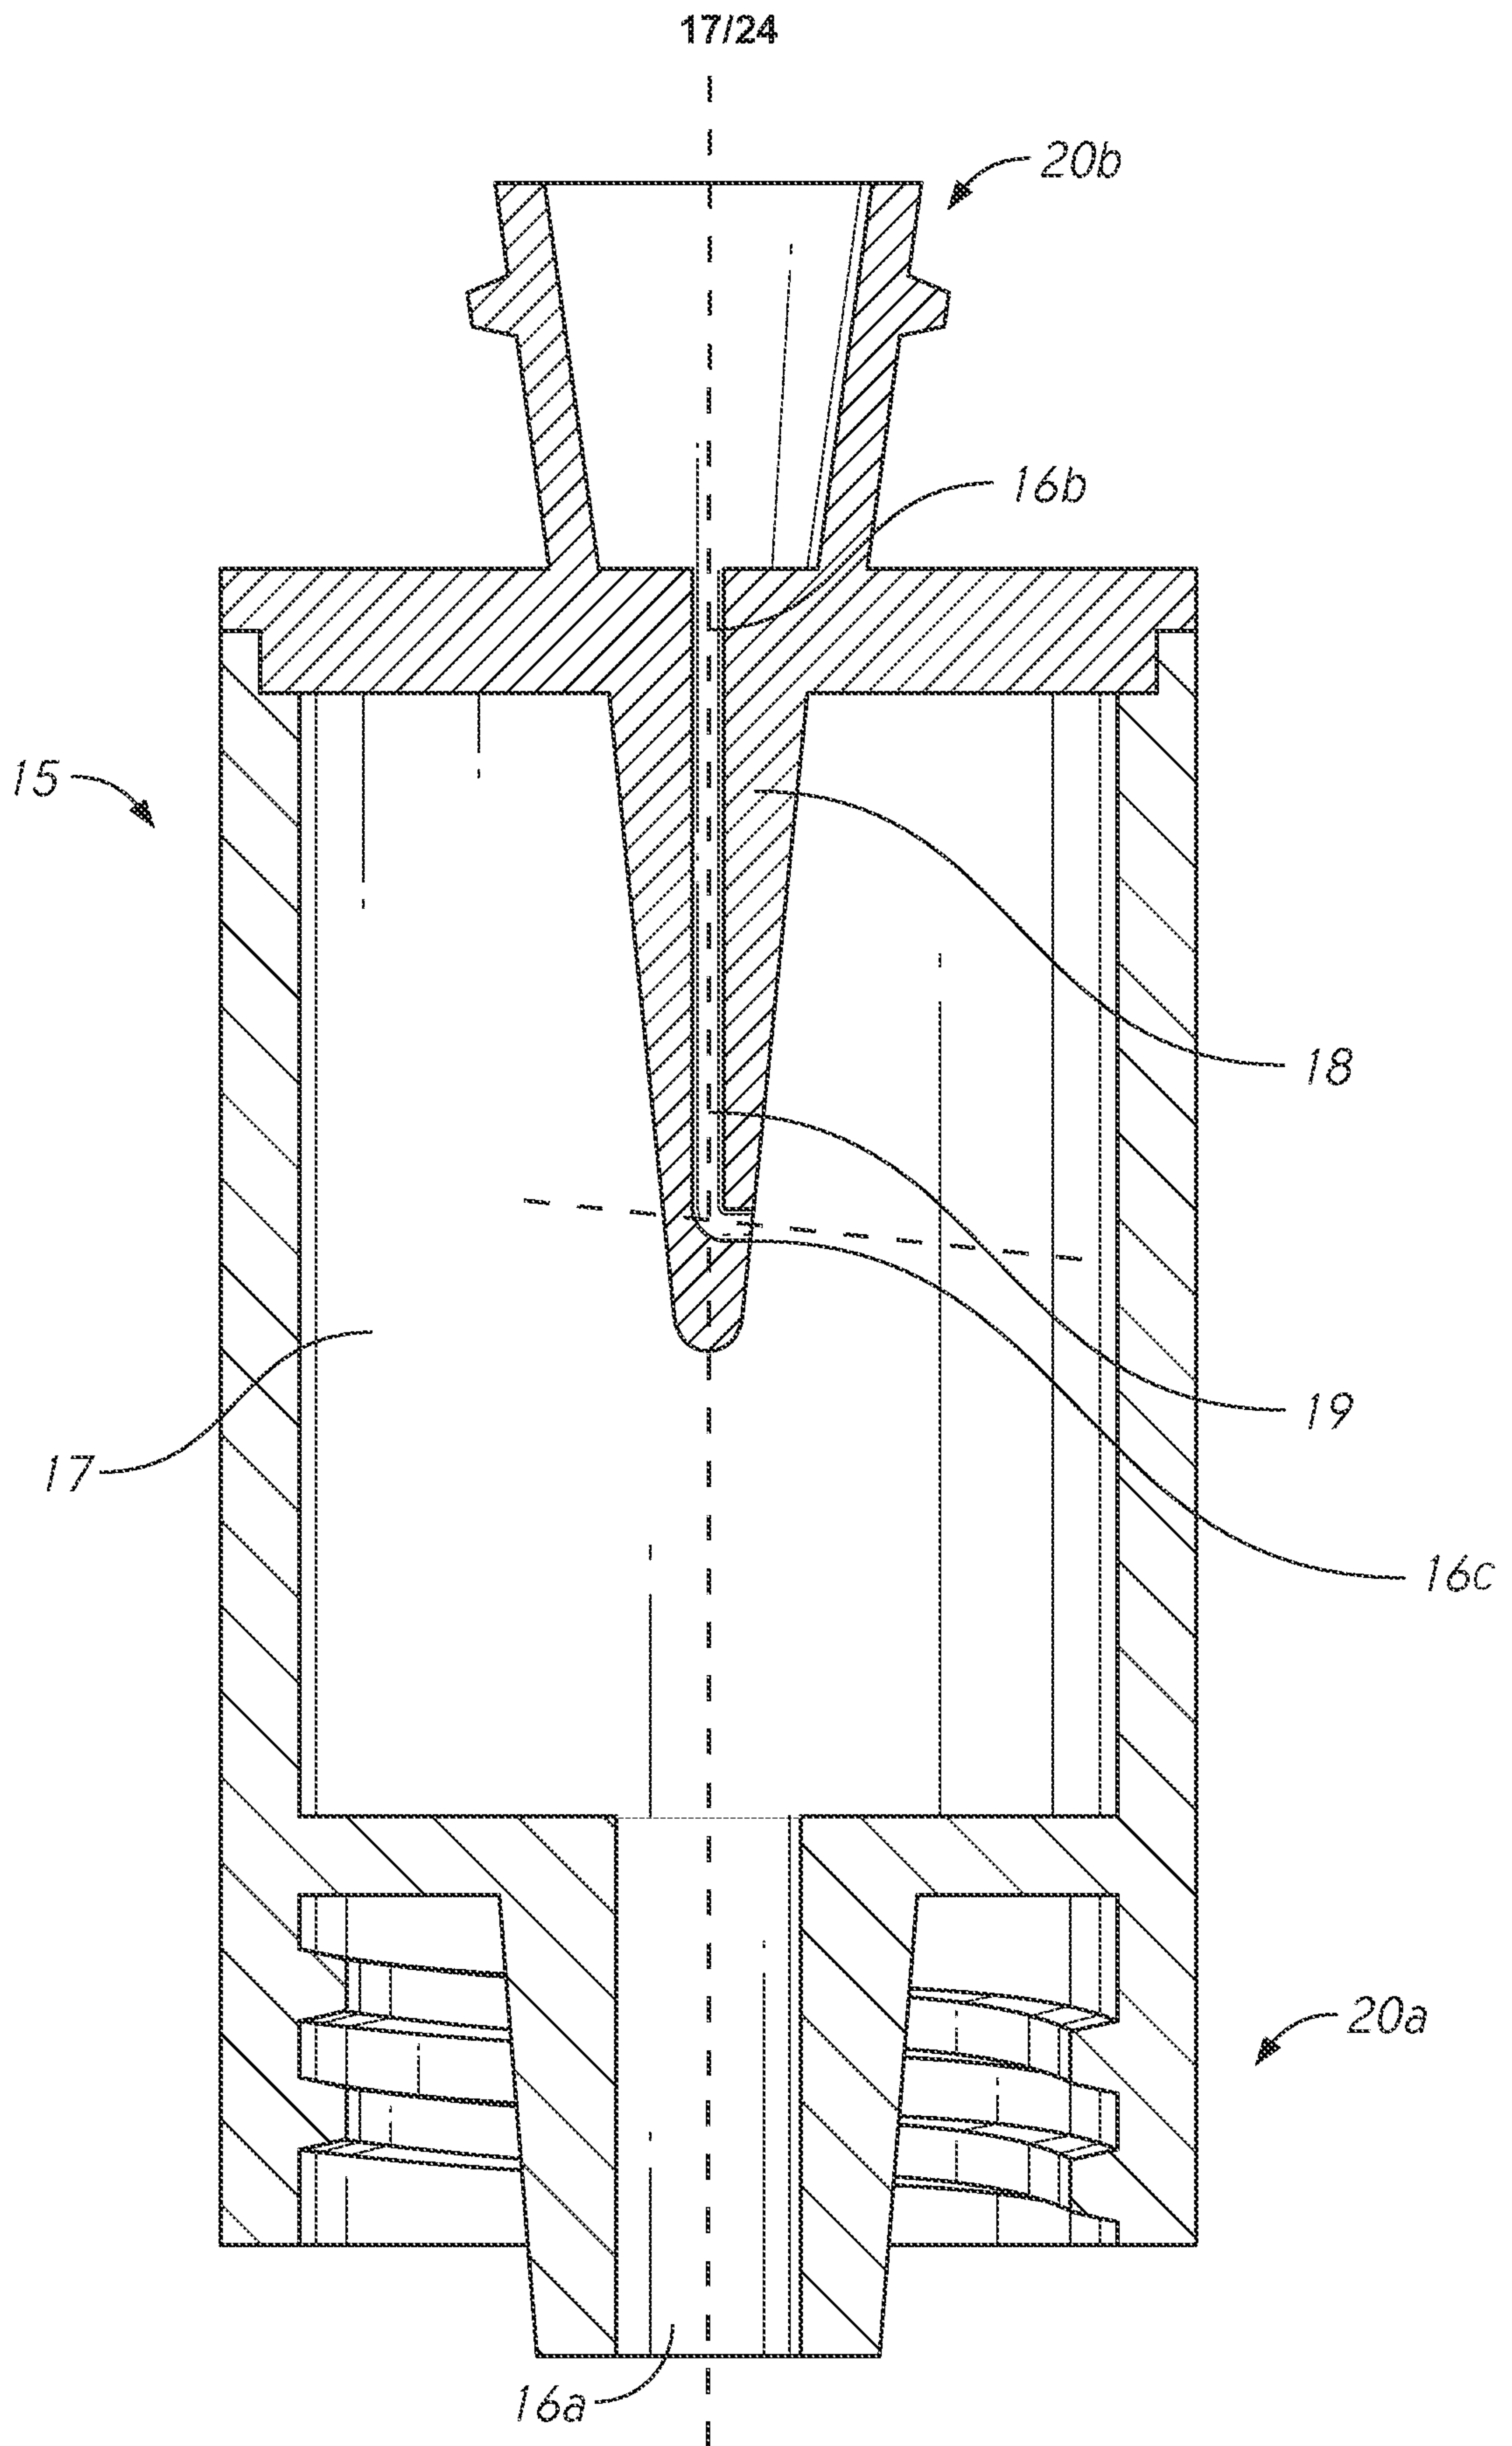


FIG. 6A'

18/24

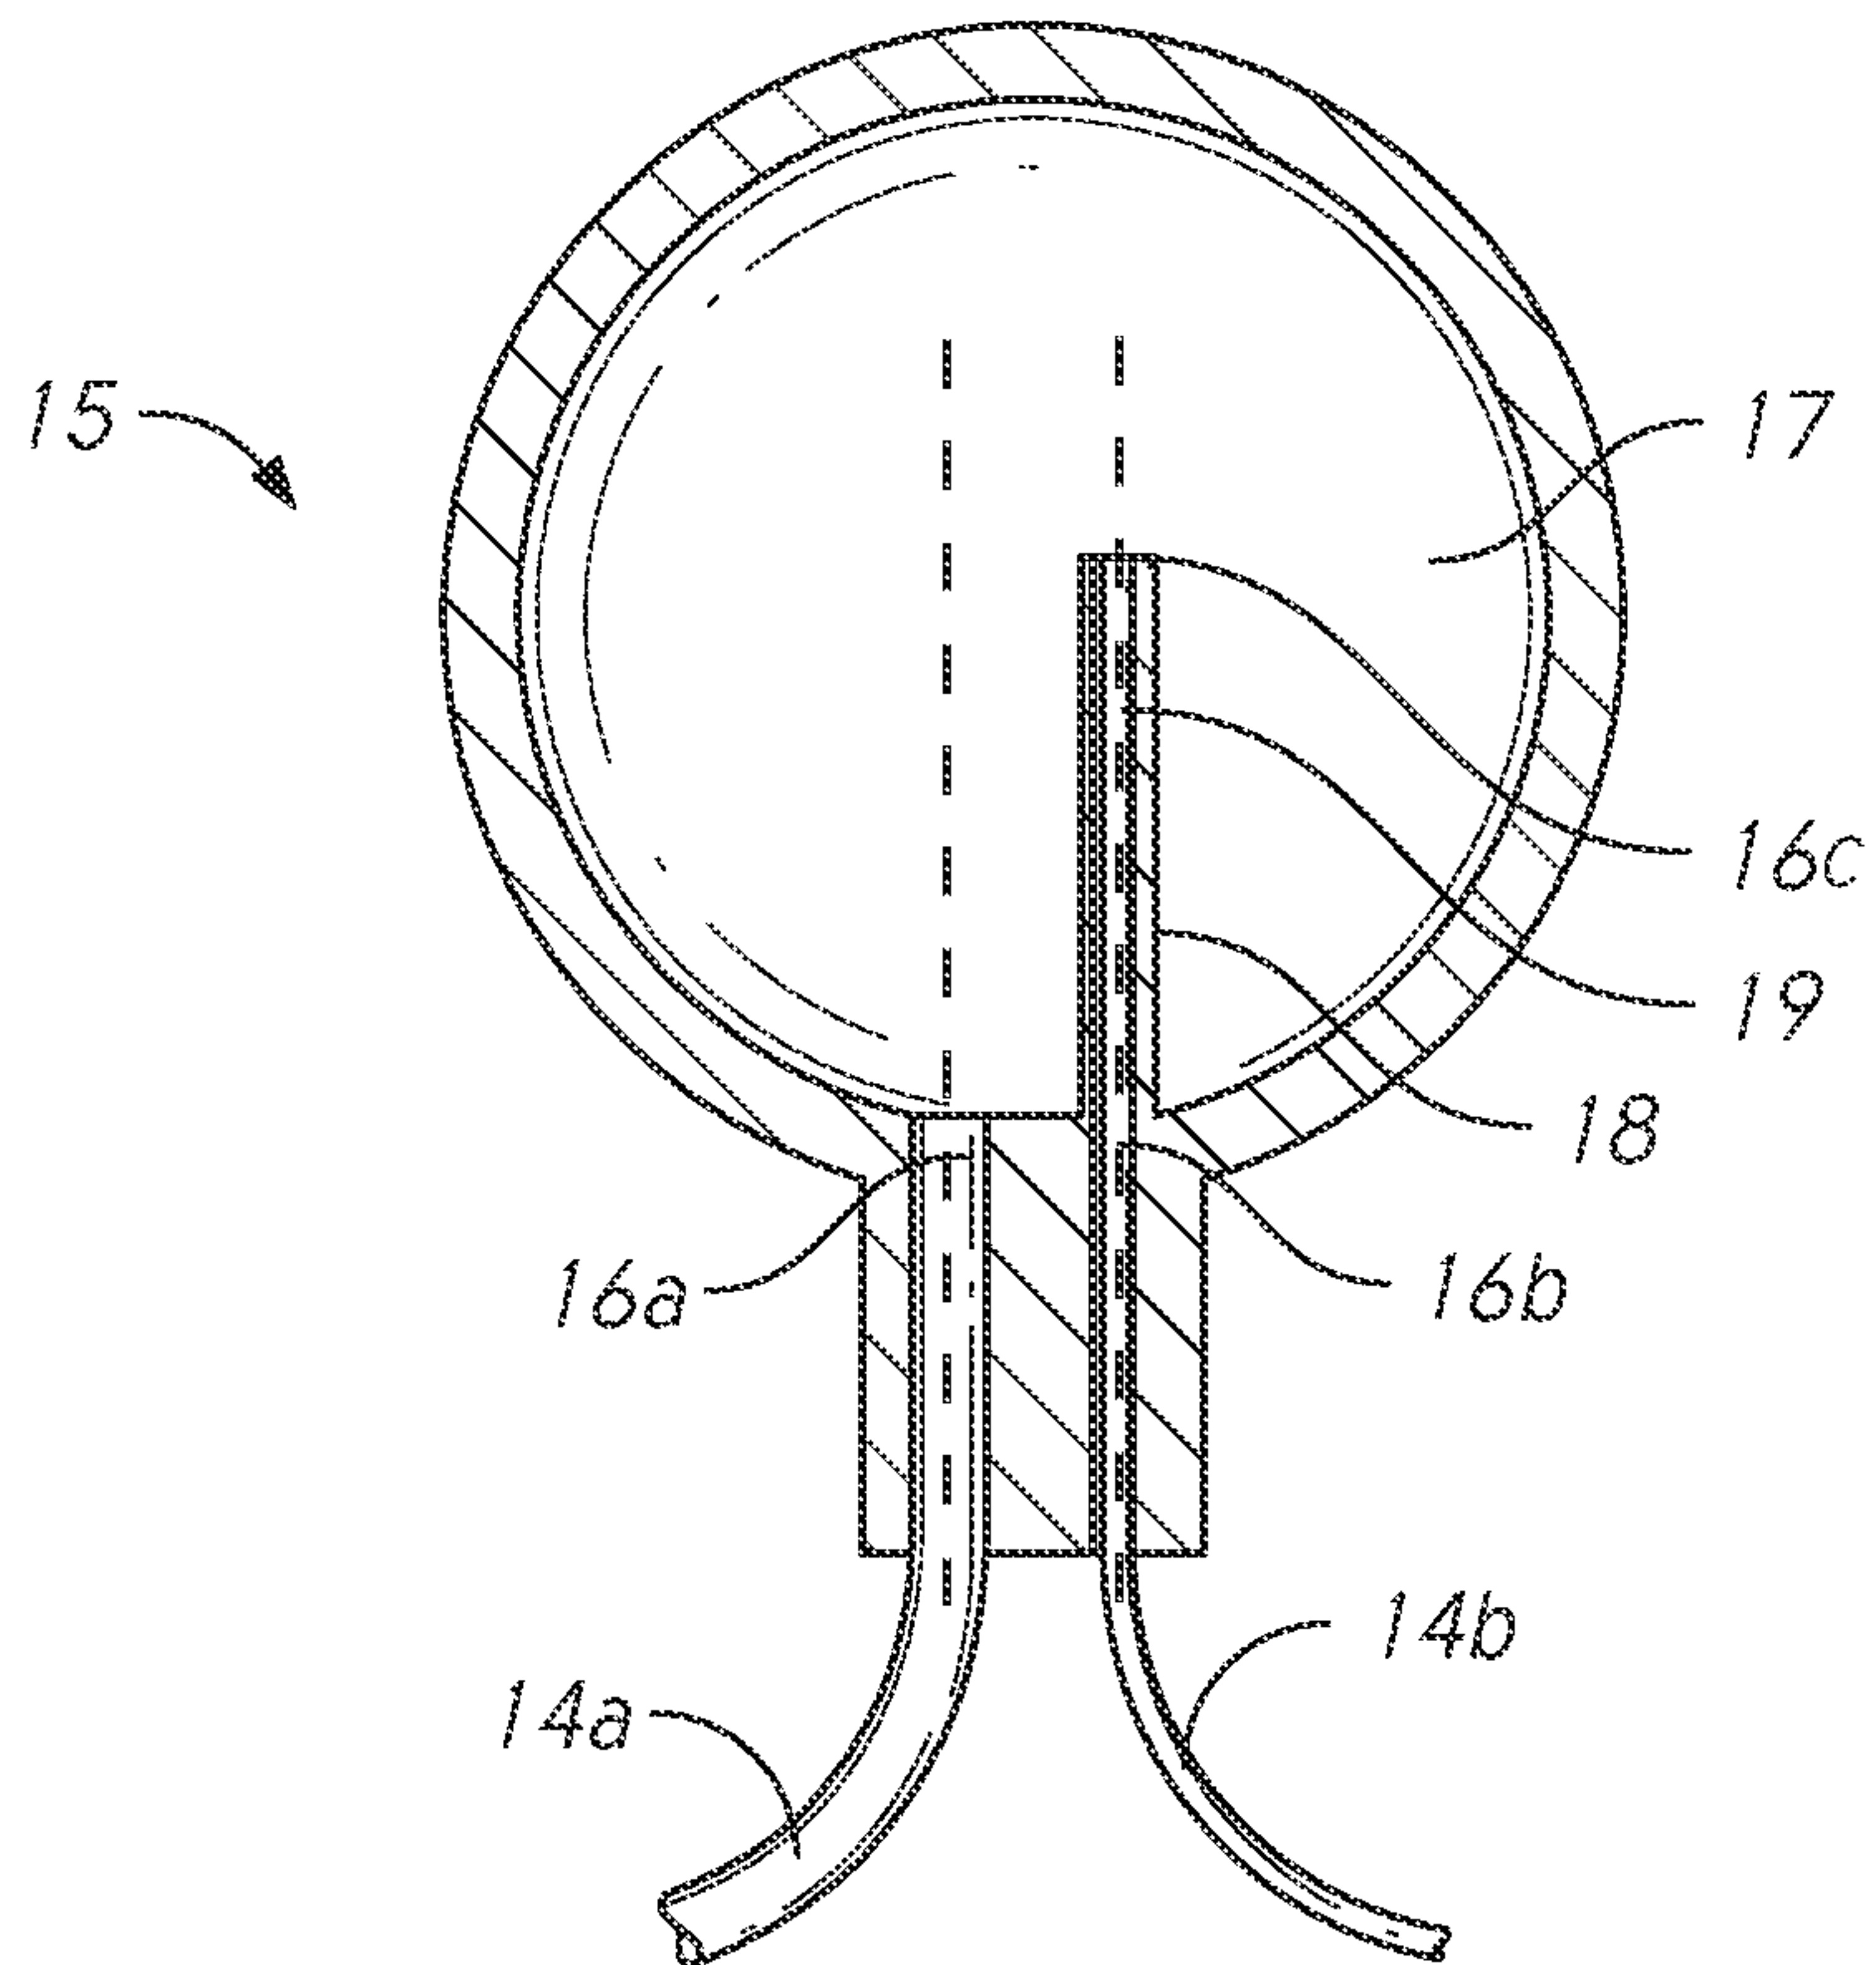


FIG. 6B

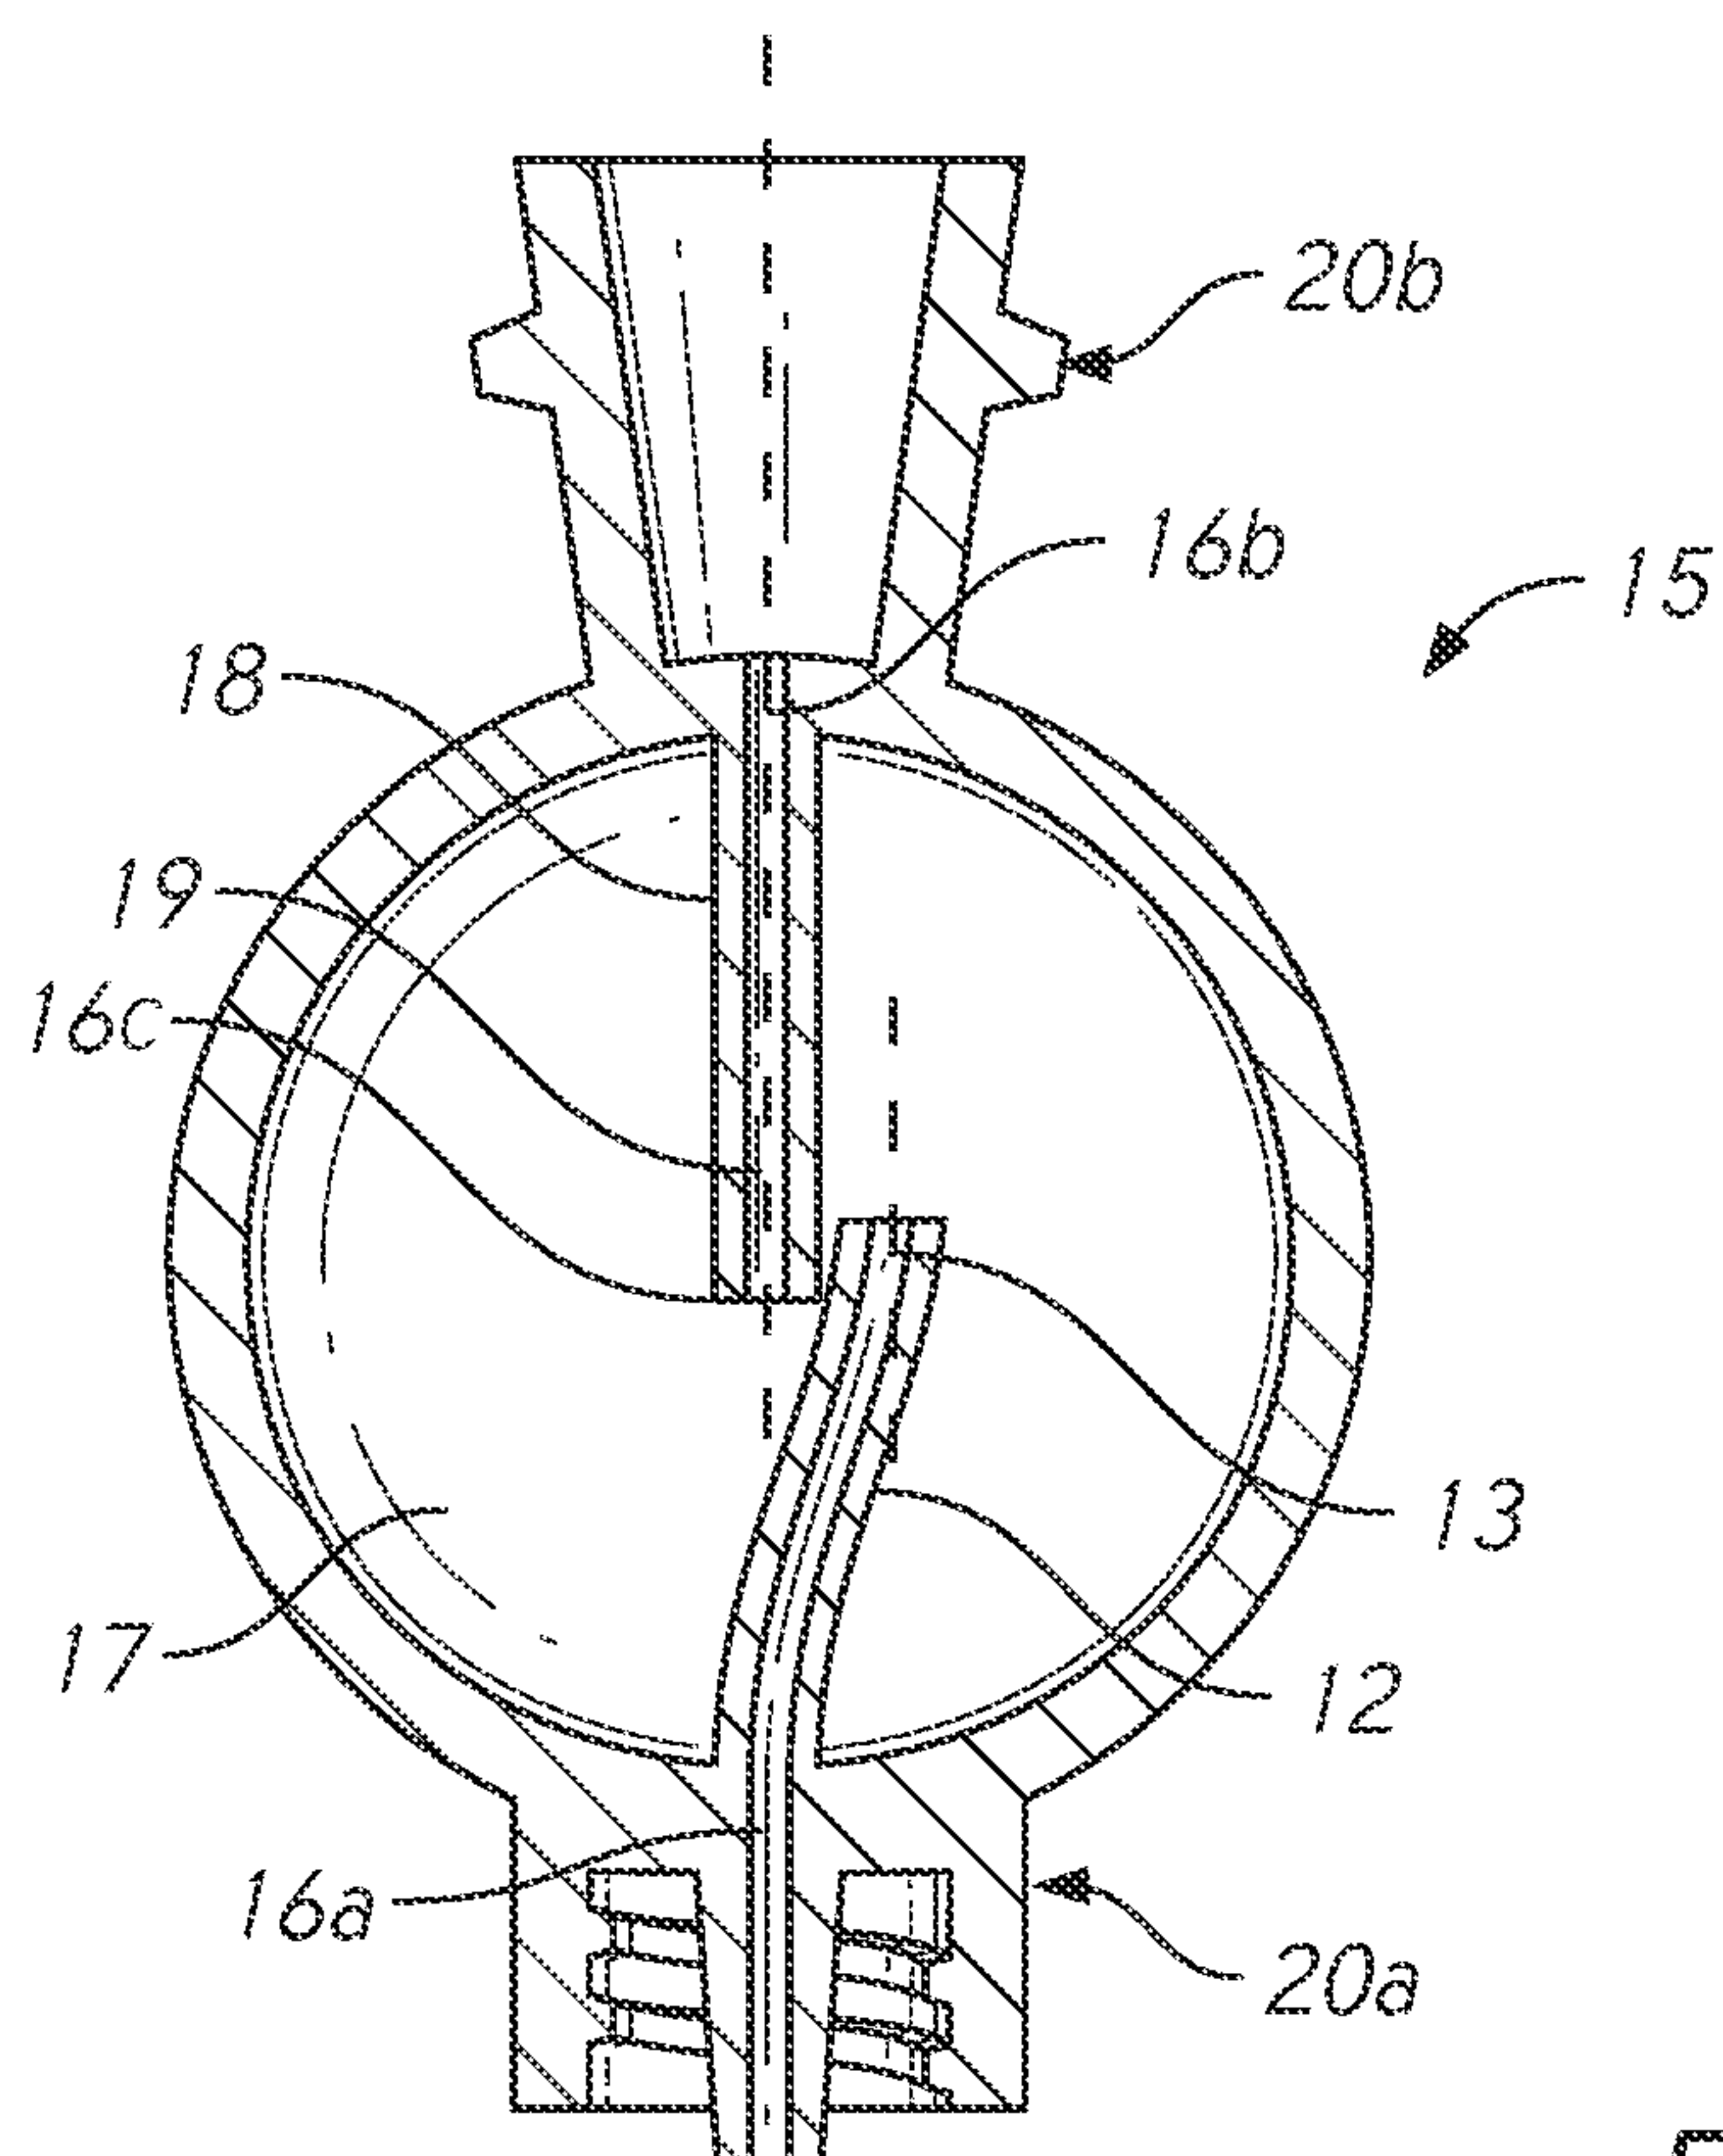


FIG. 6C

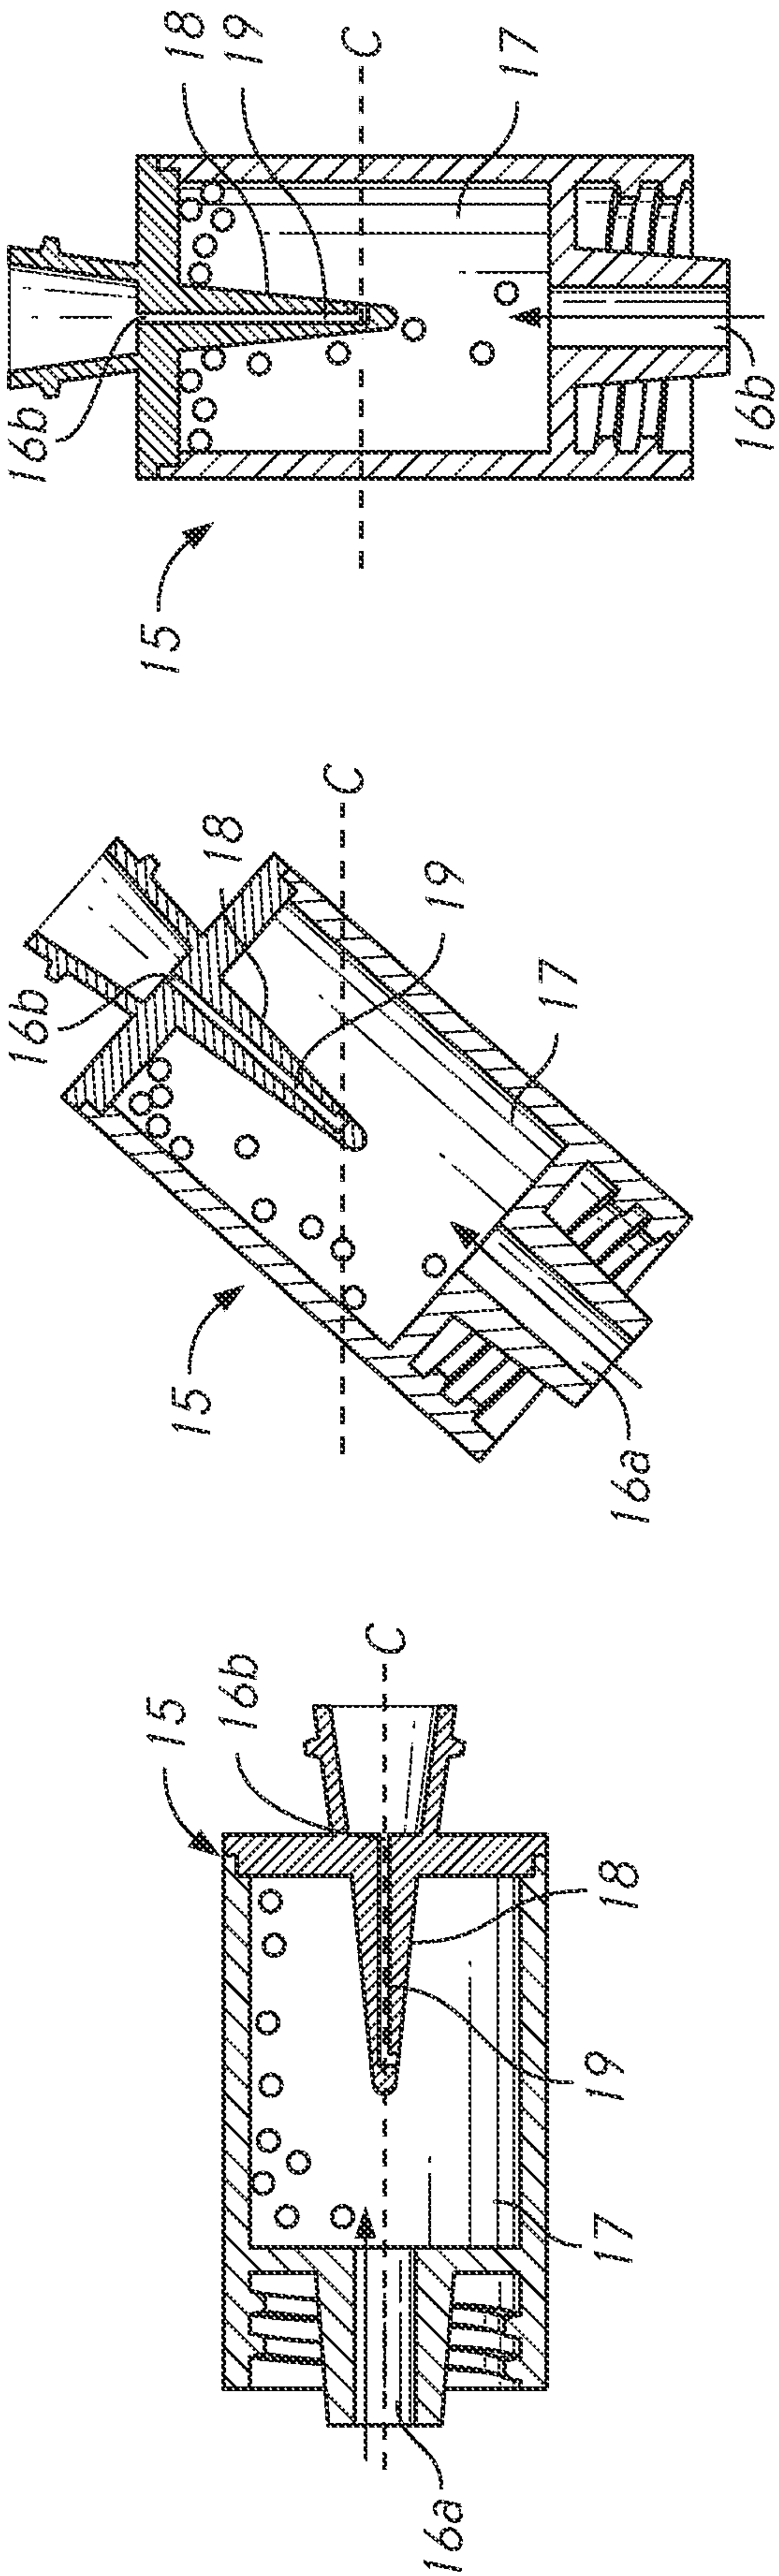


FIG. 7A

FIG. 7B

FIG. 7C

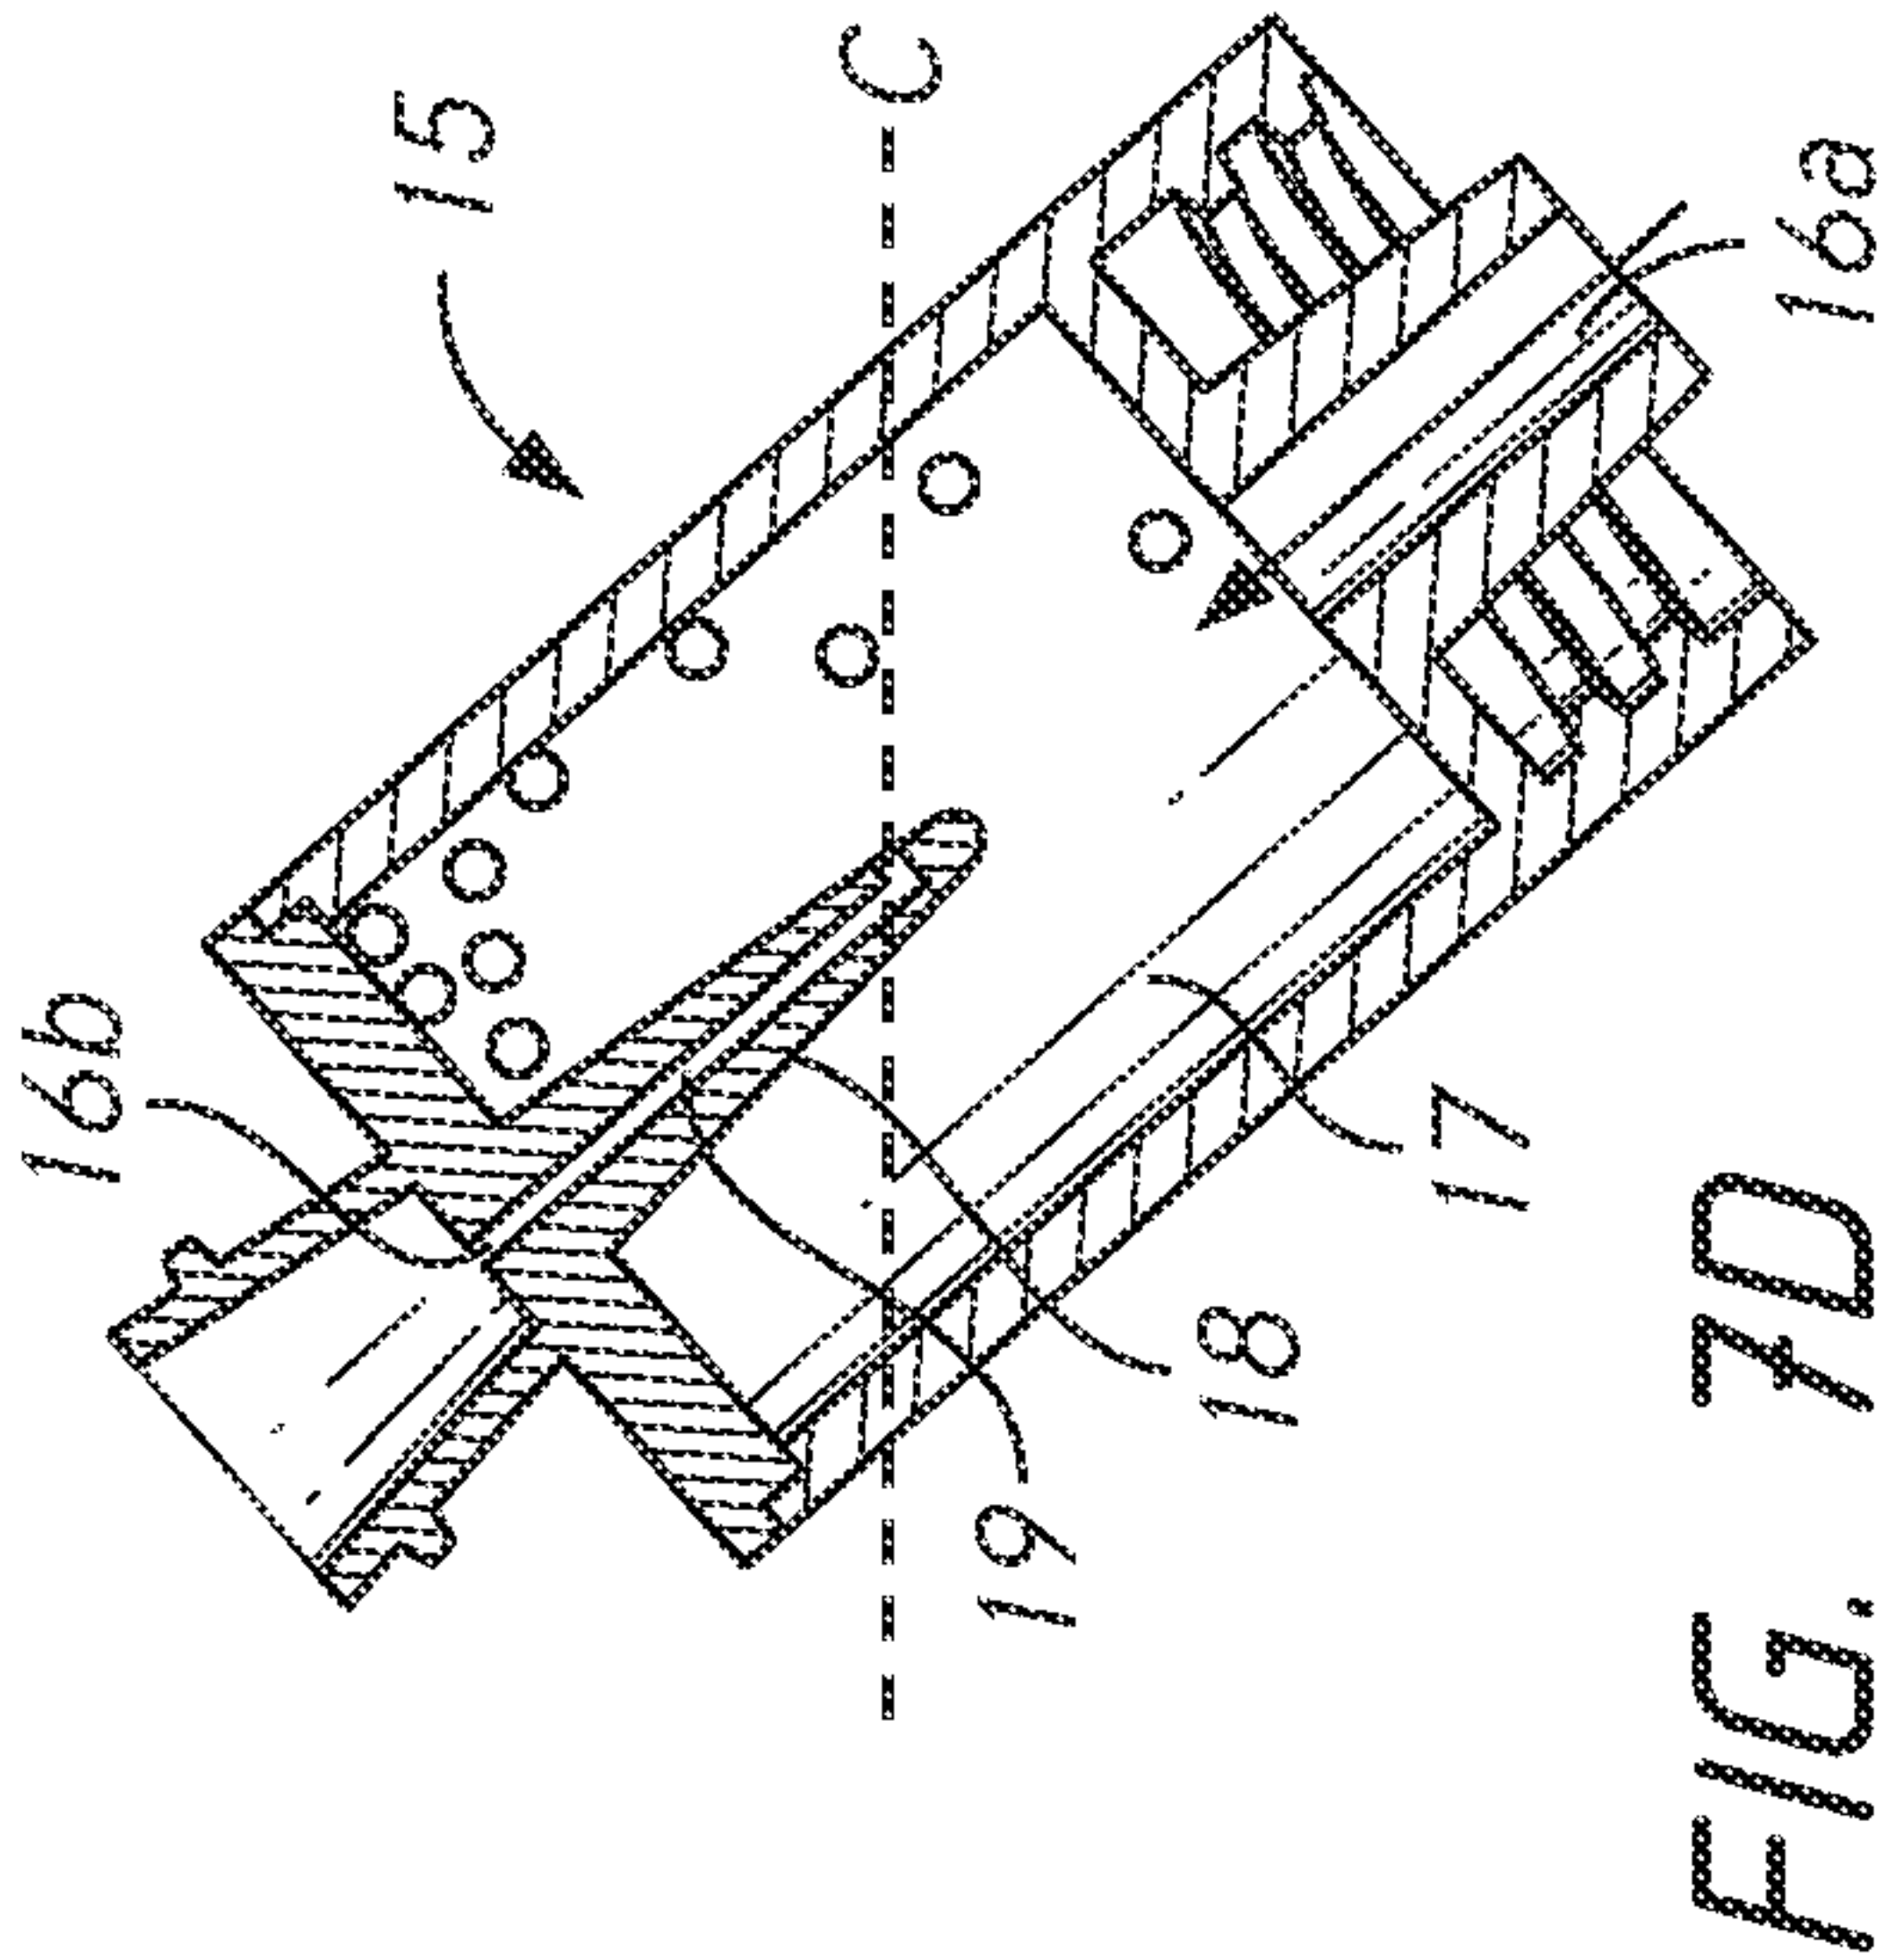


FIG. 7D

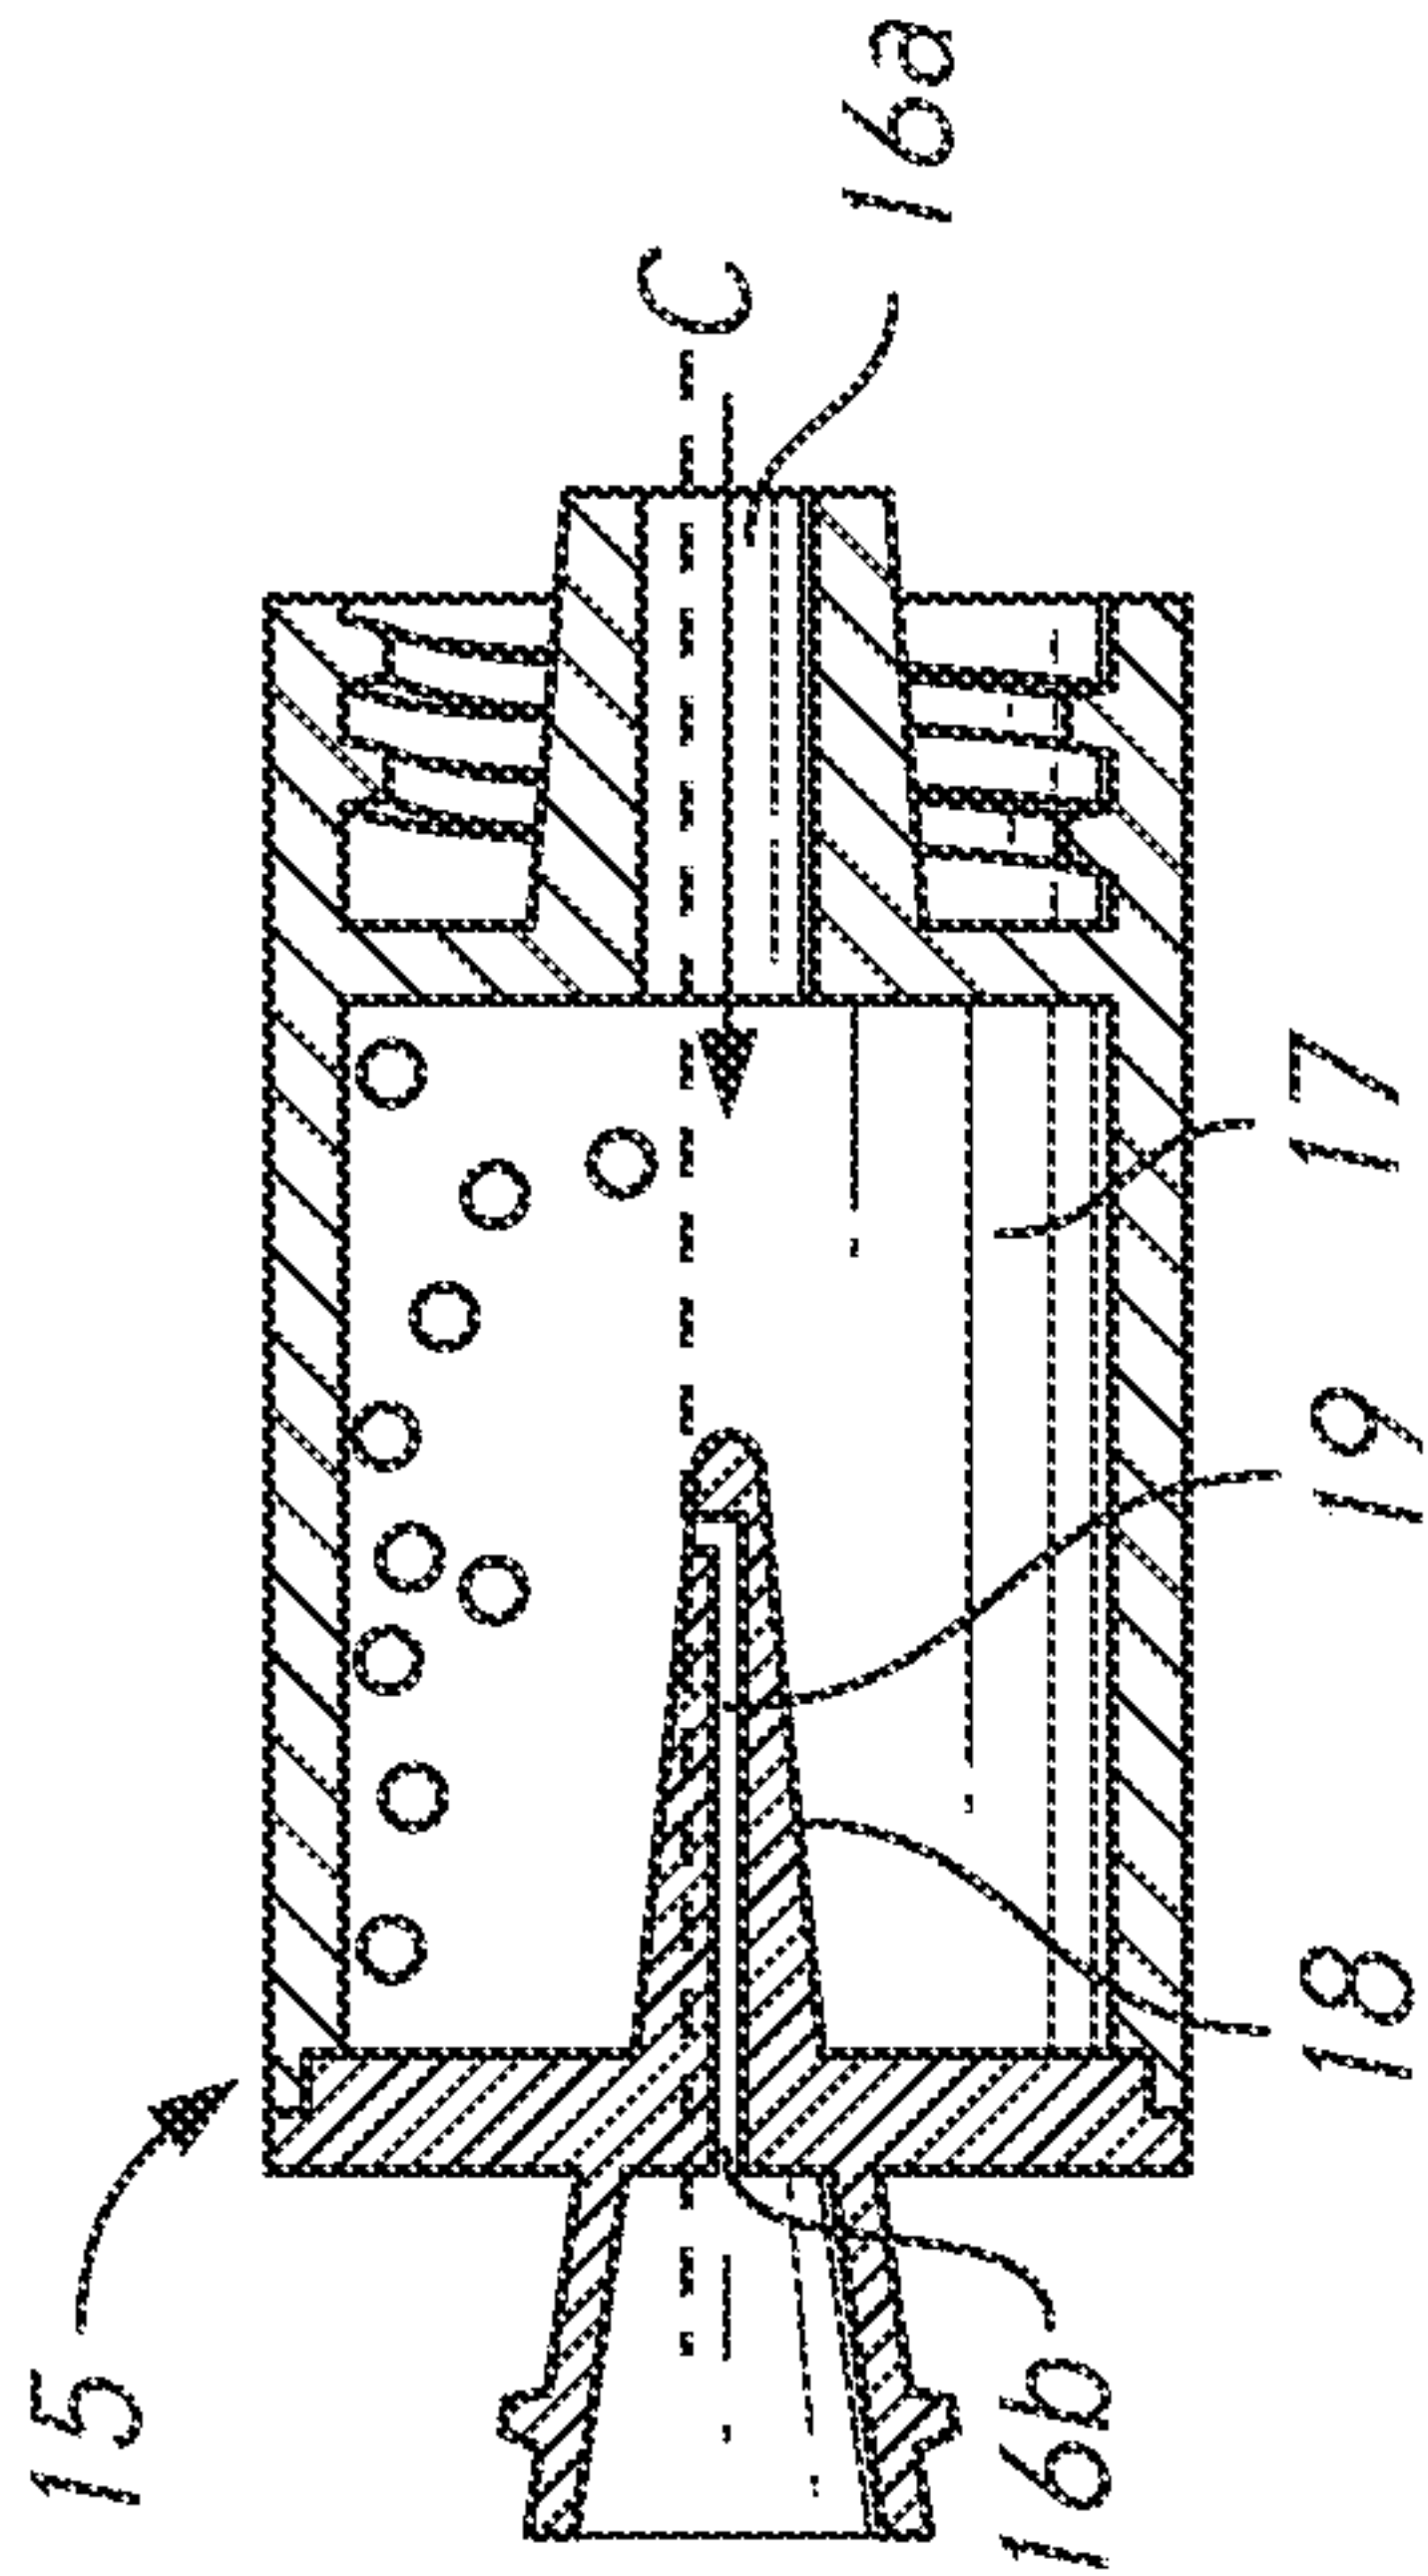


FIG. 7E

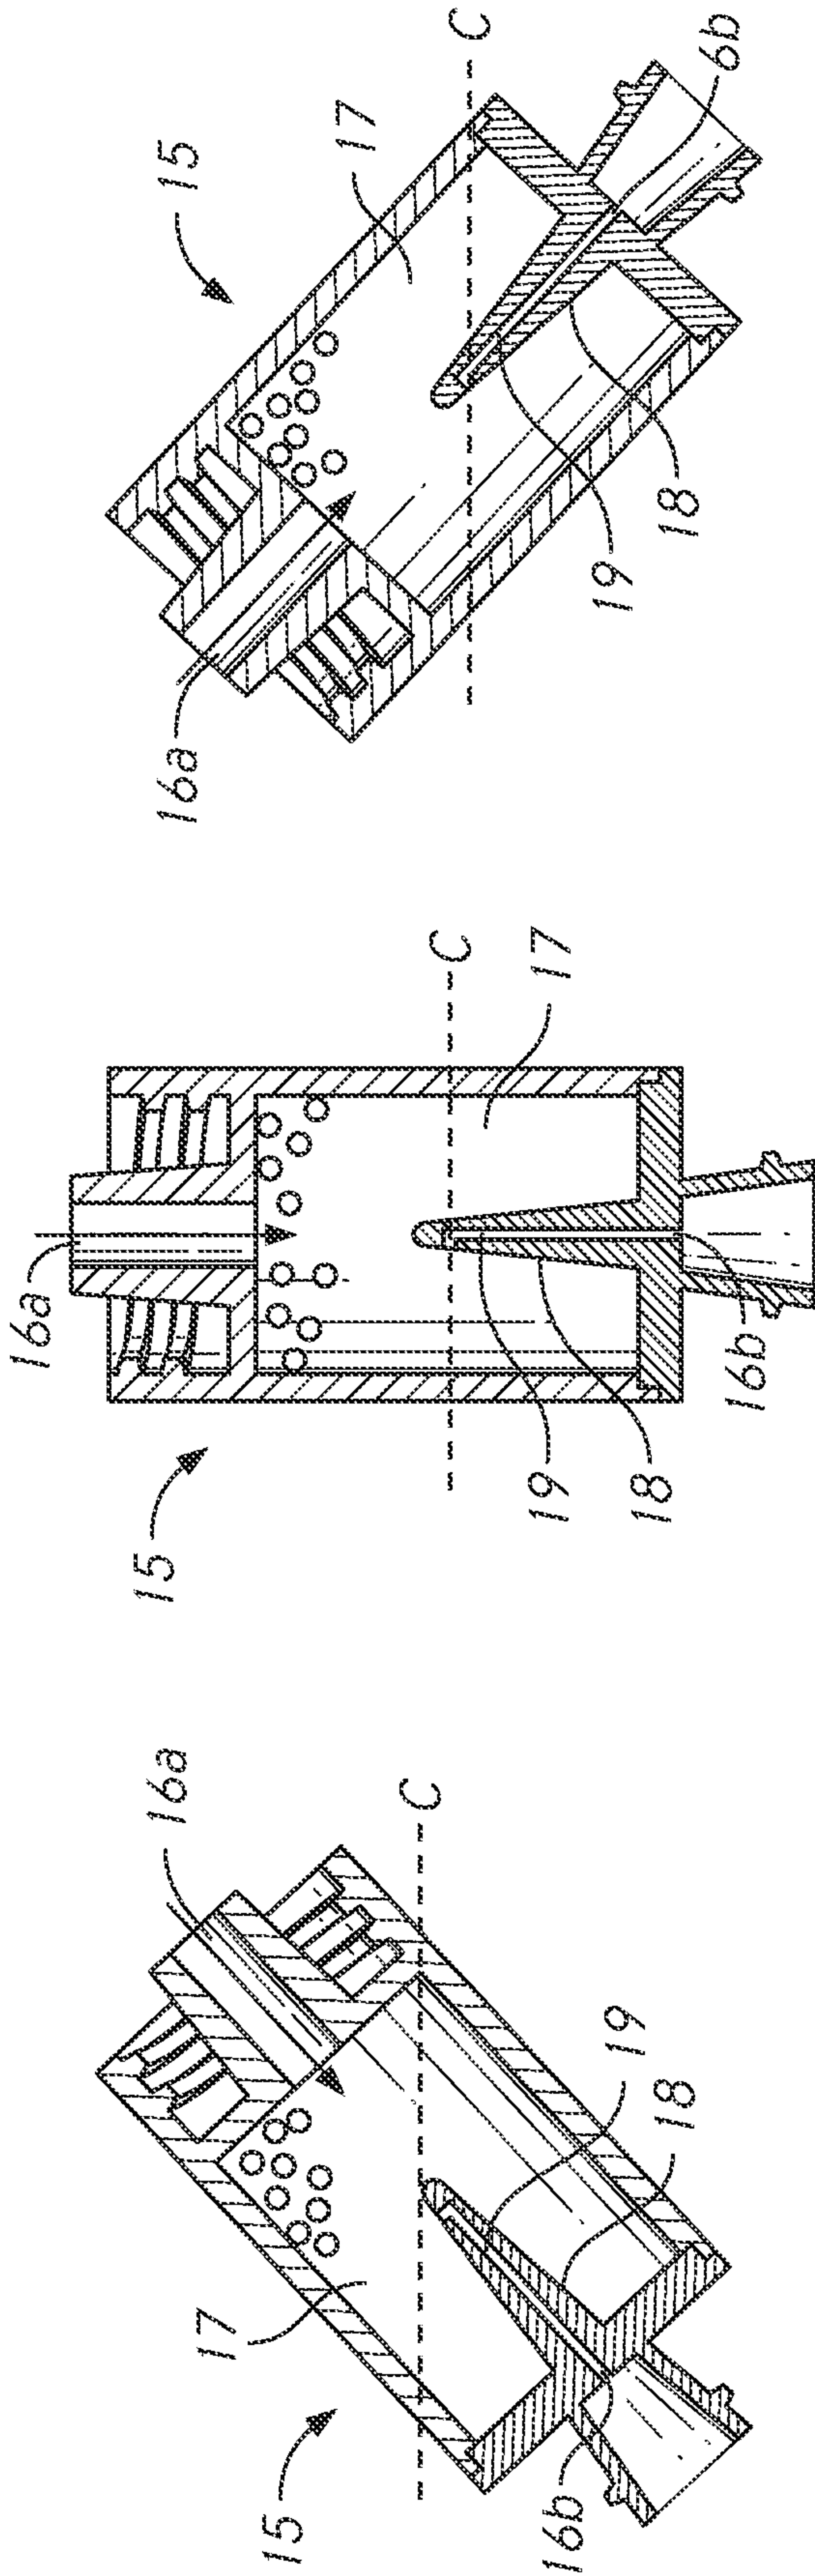


FIG. 7H

FIG. 7G

FIG. 7F

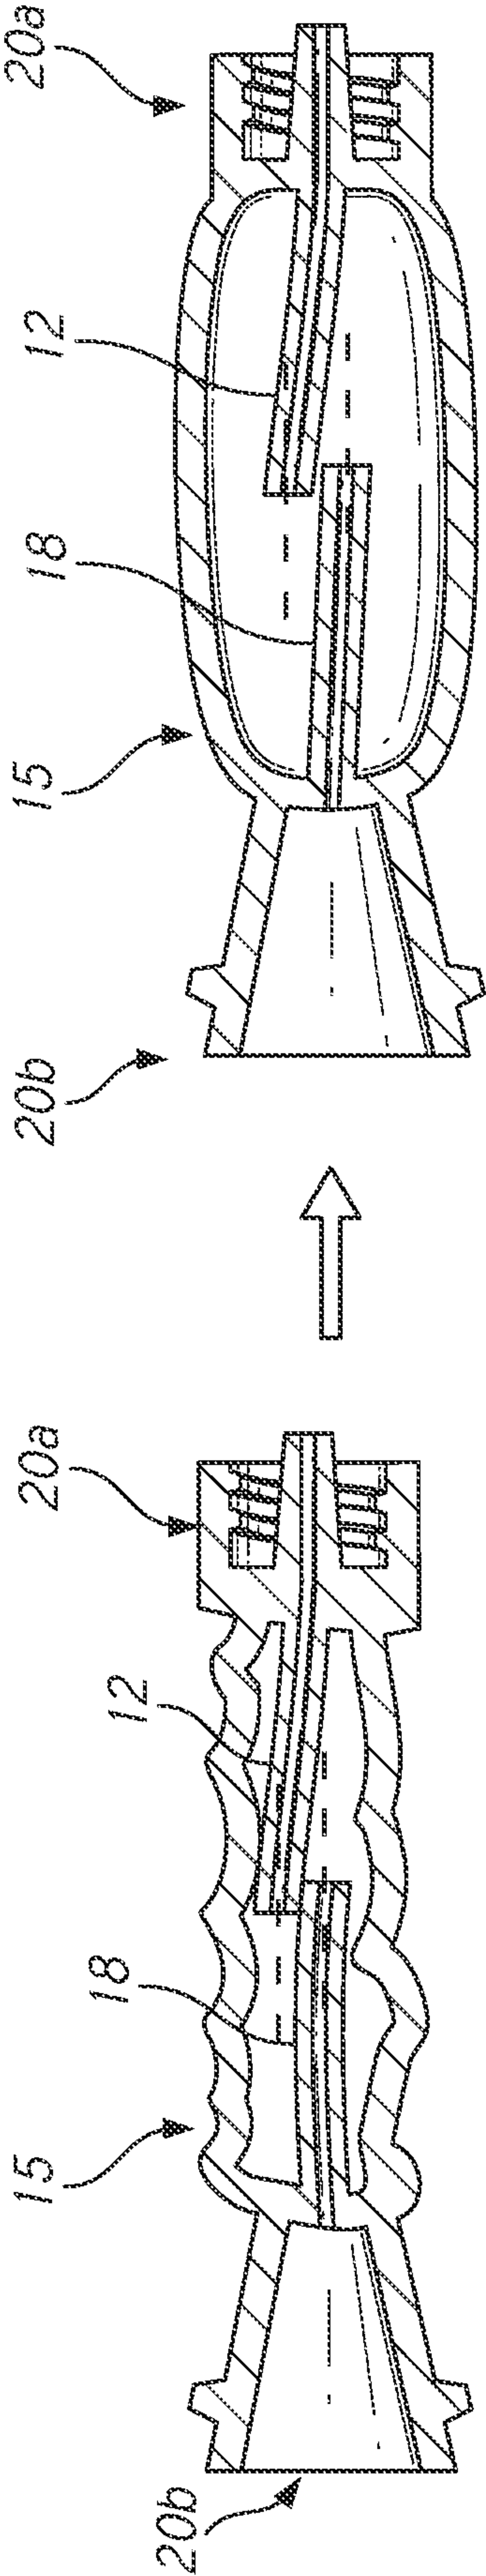


FIG. 8B

FIG. 8A

22/24

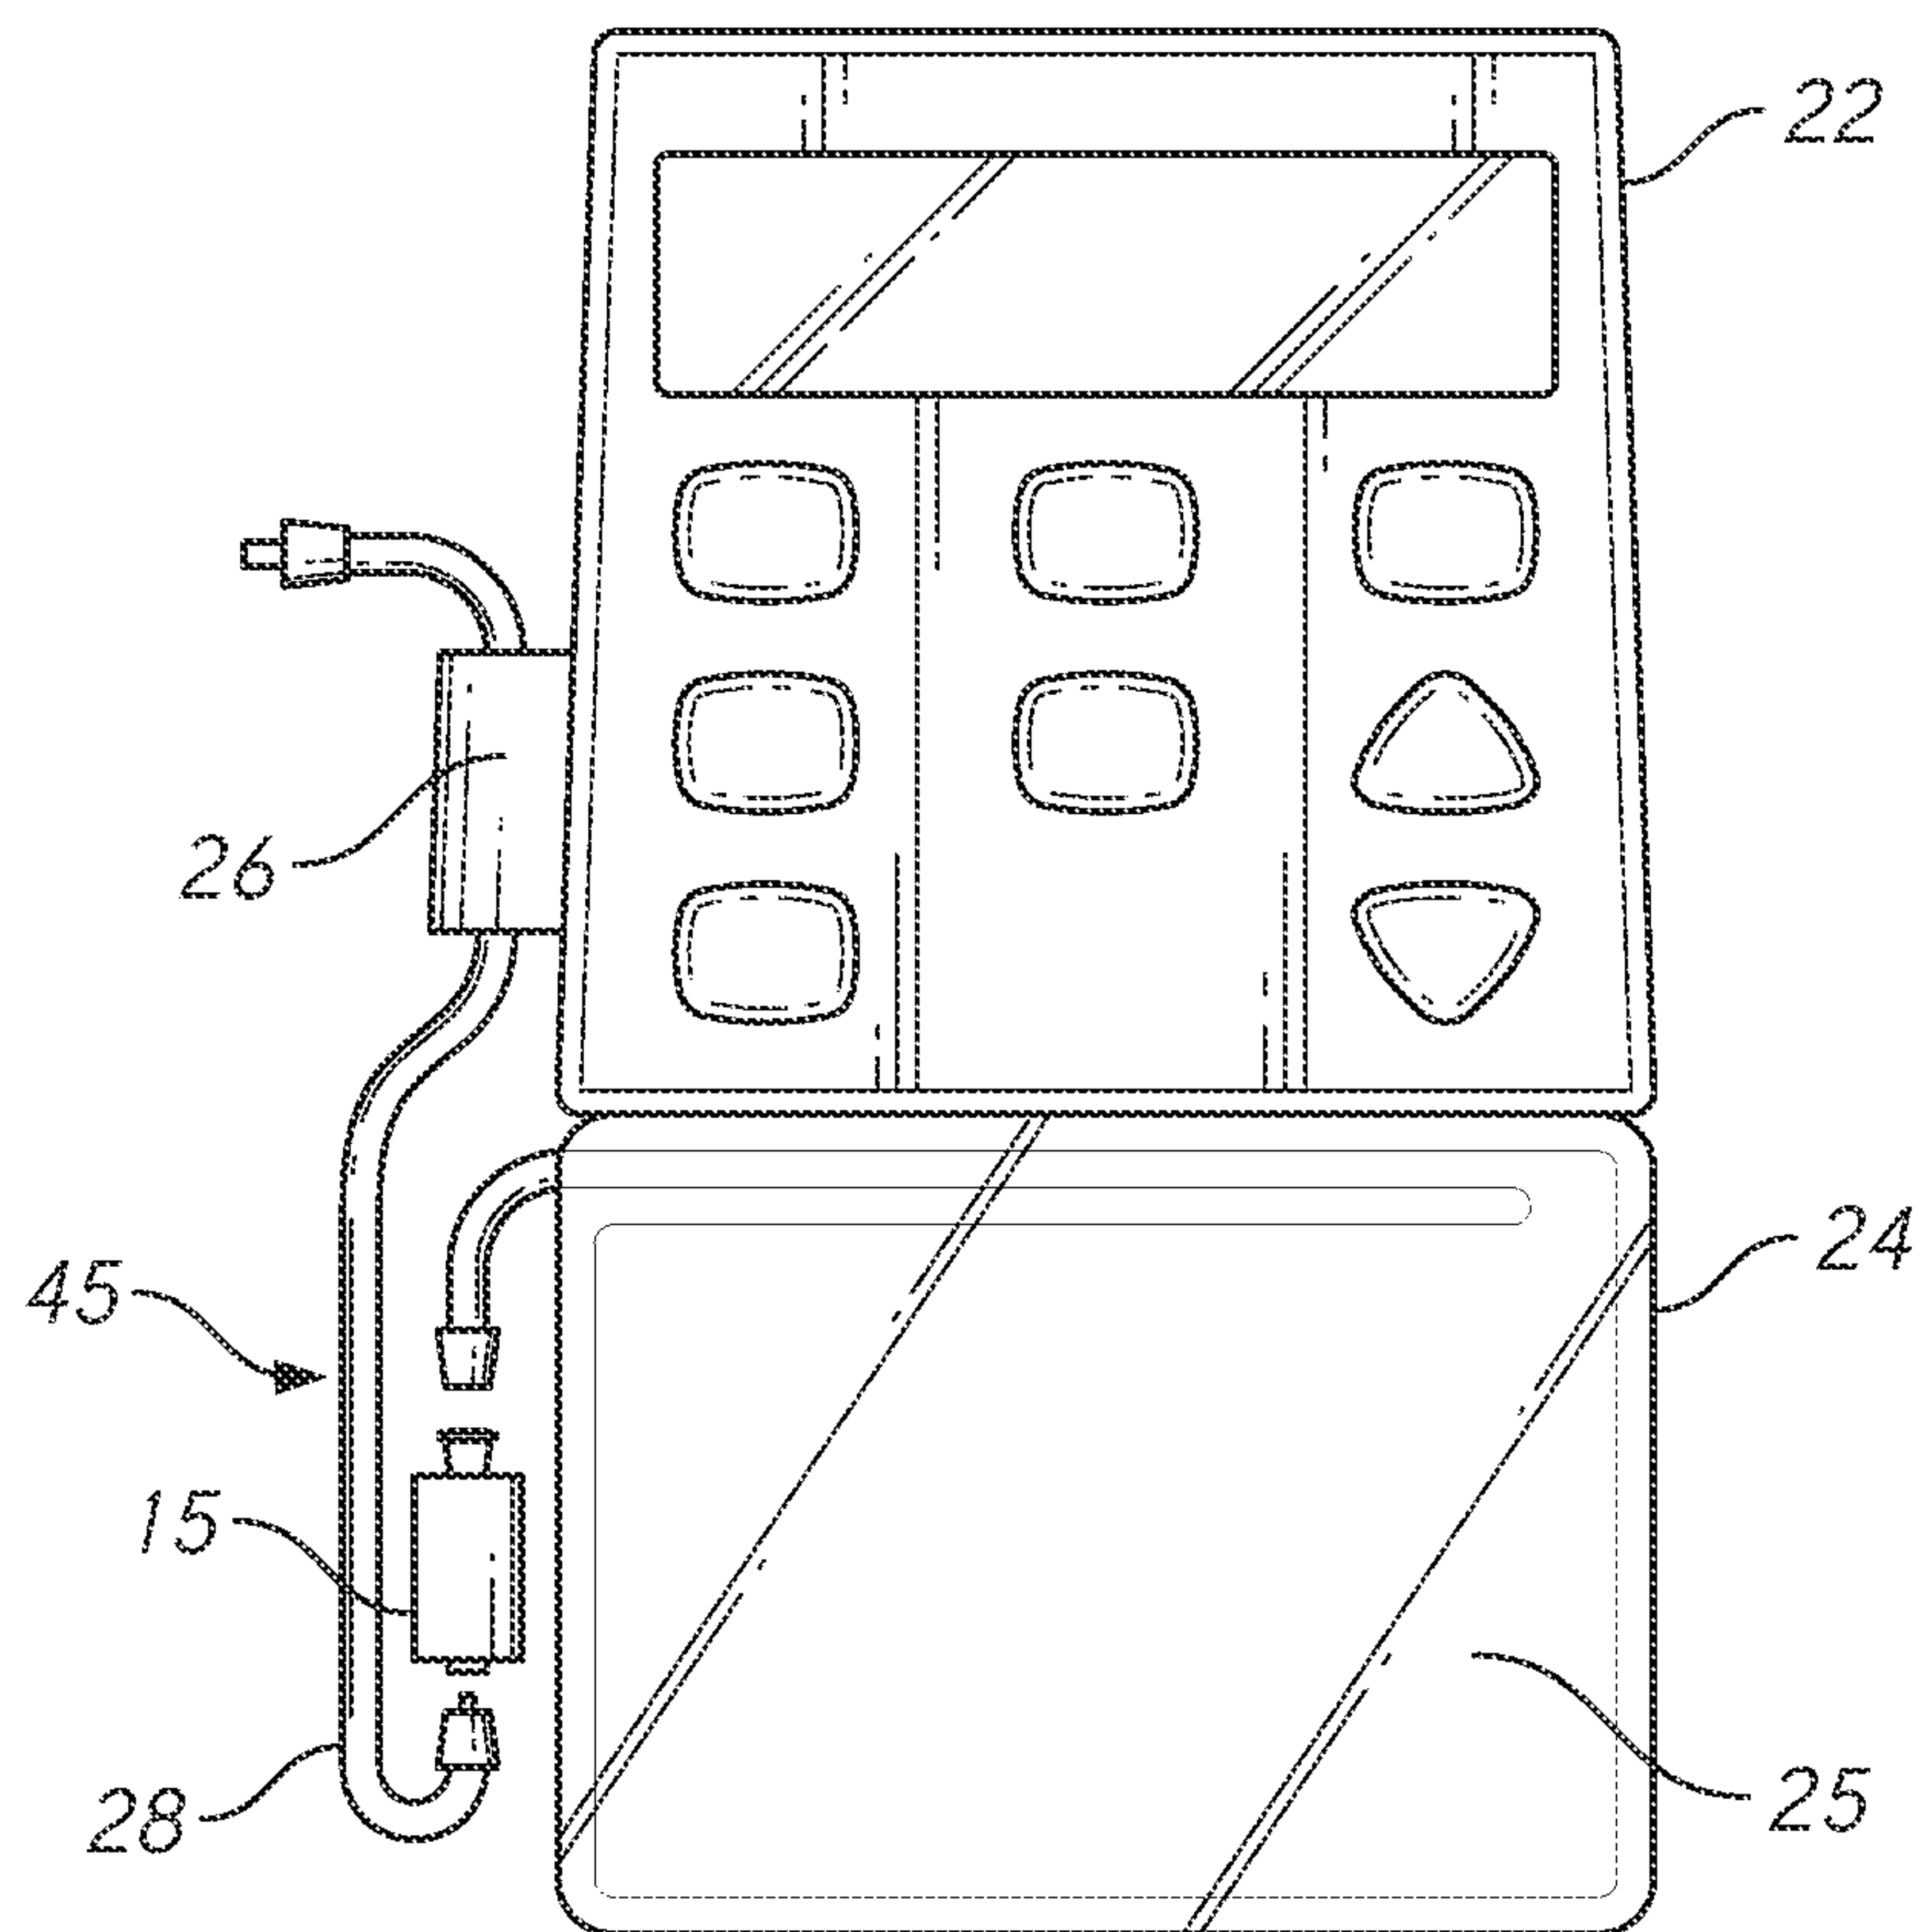


FIG. 9A

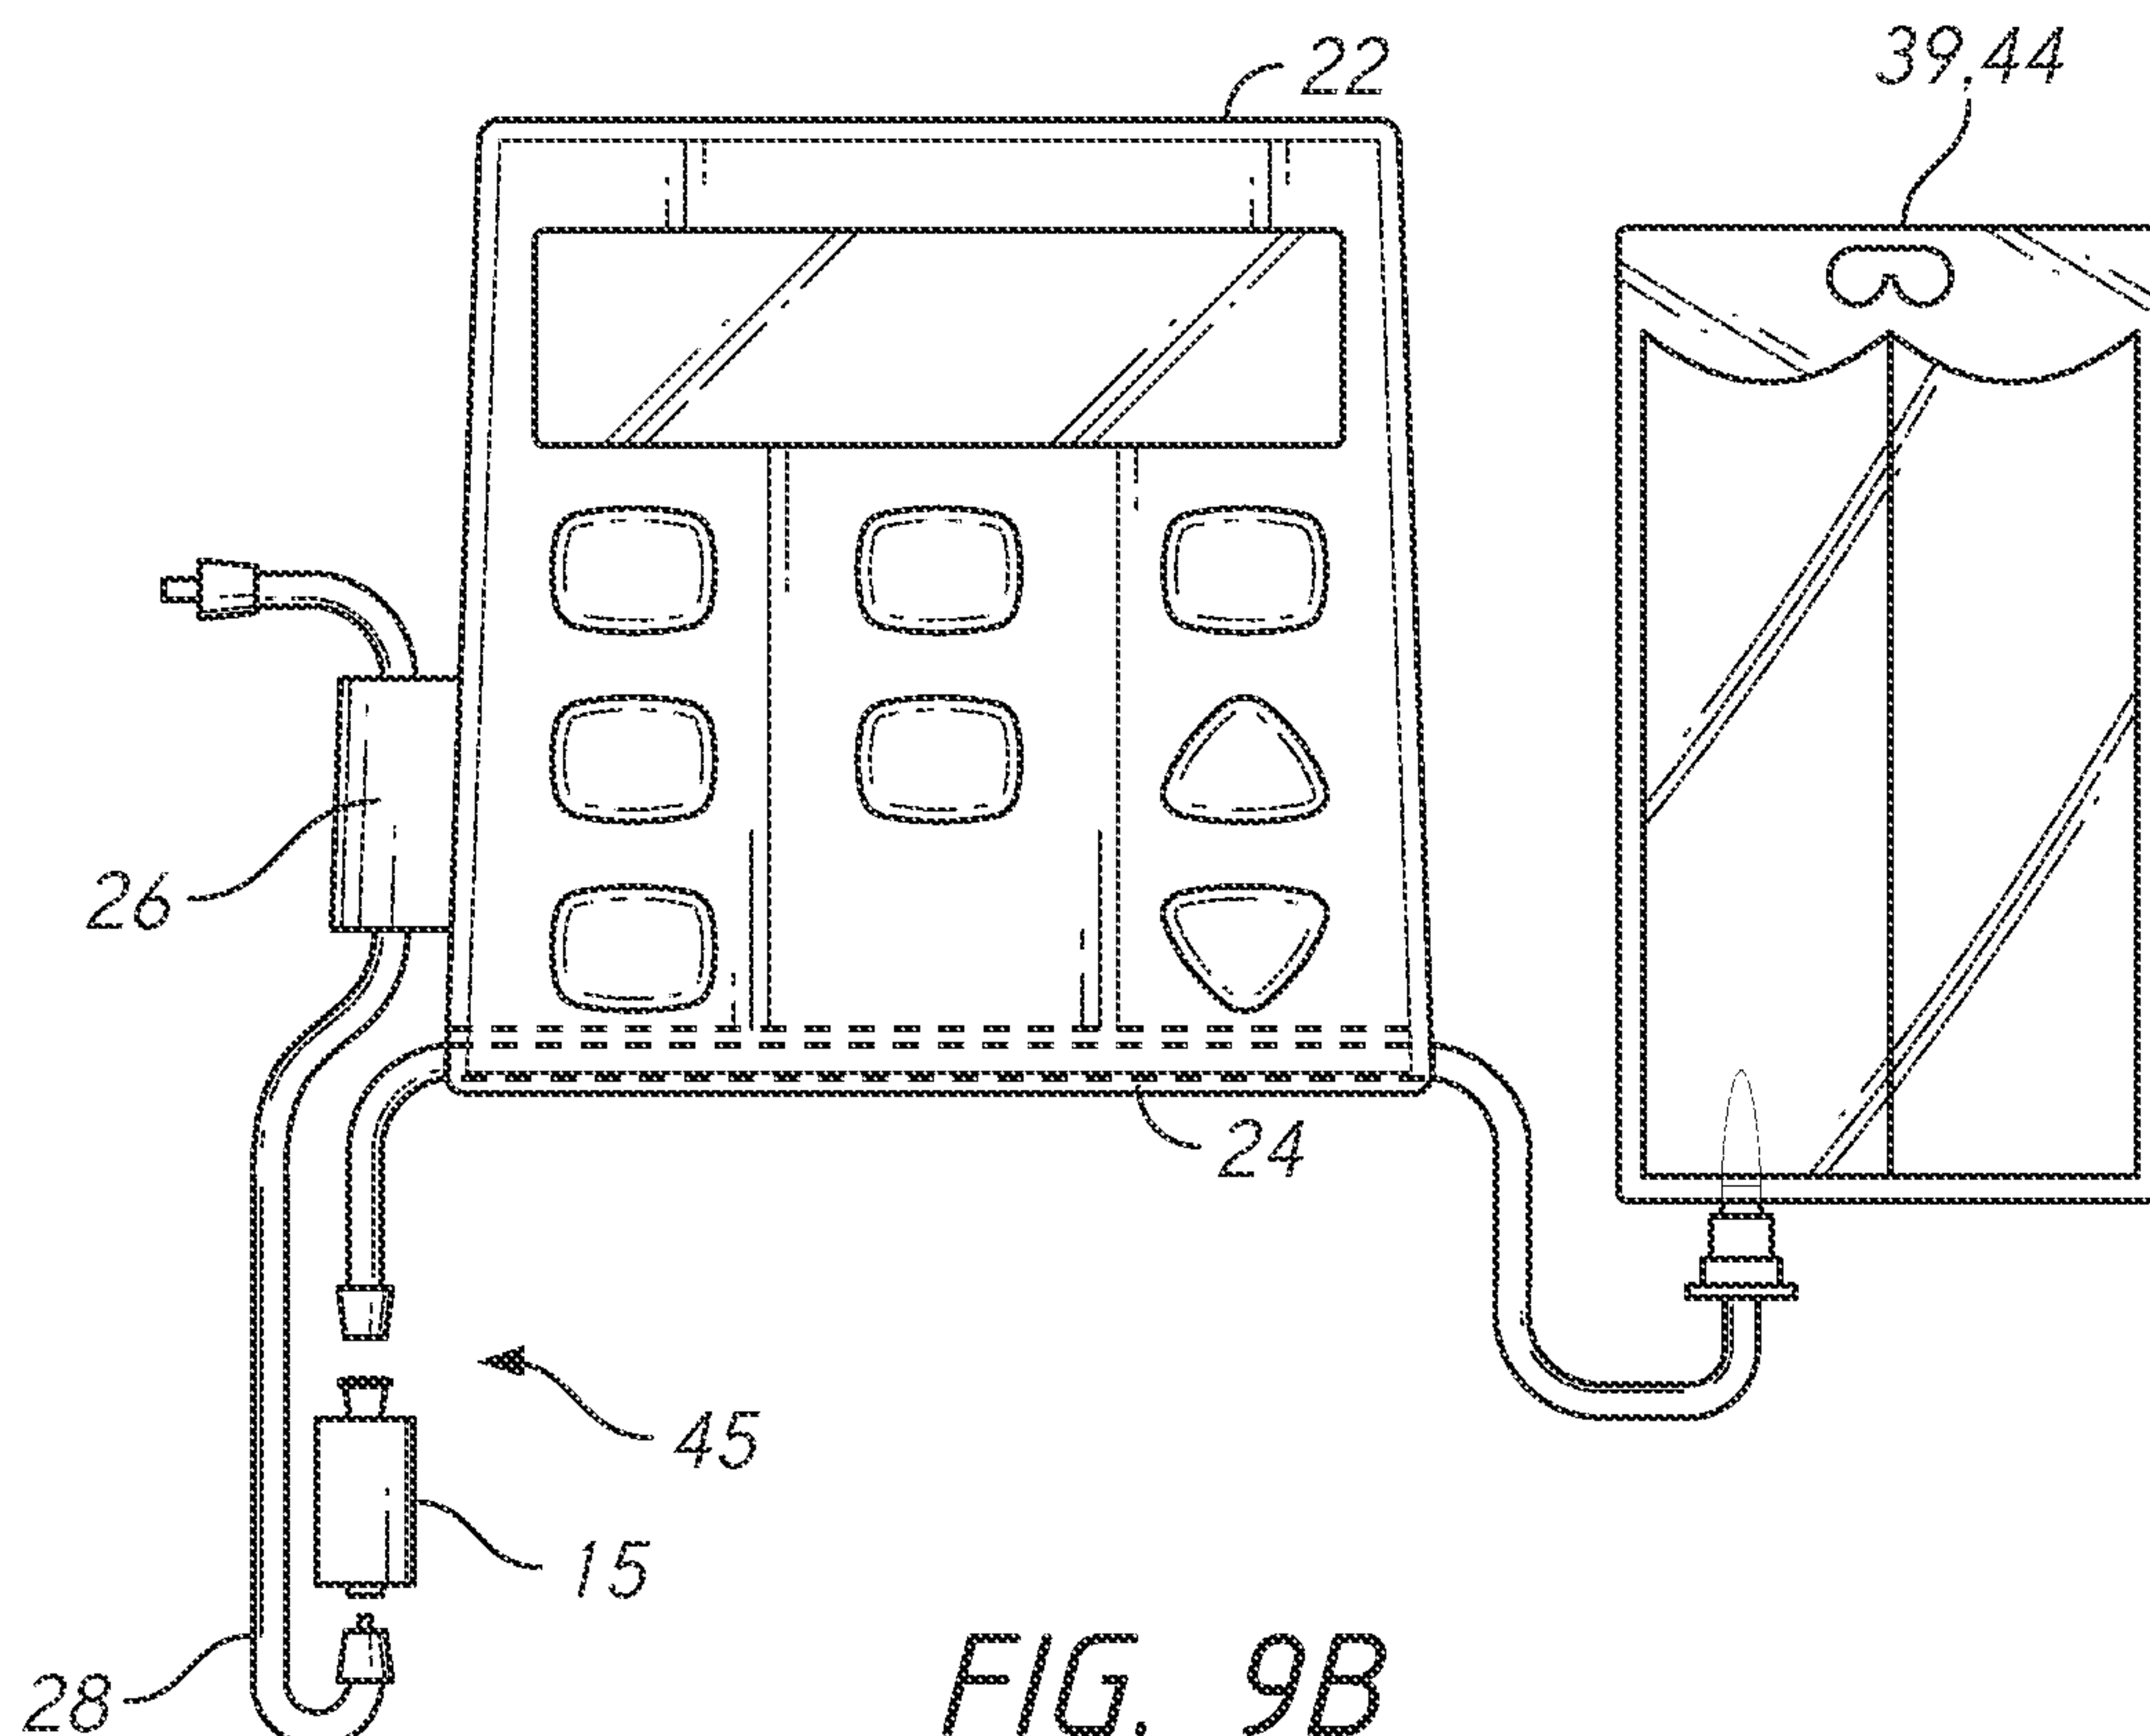


FIG. 9B

23/24

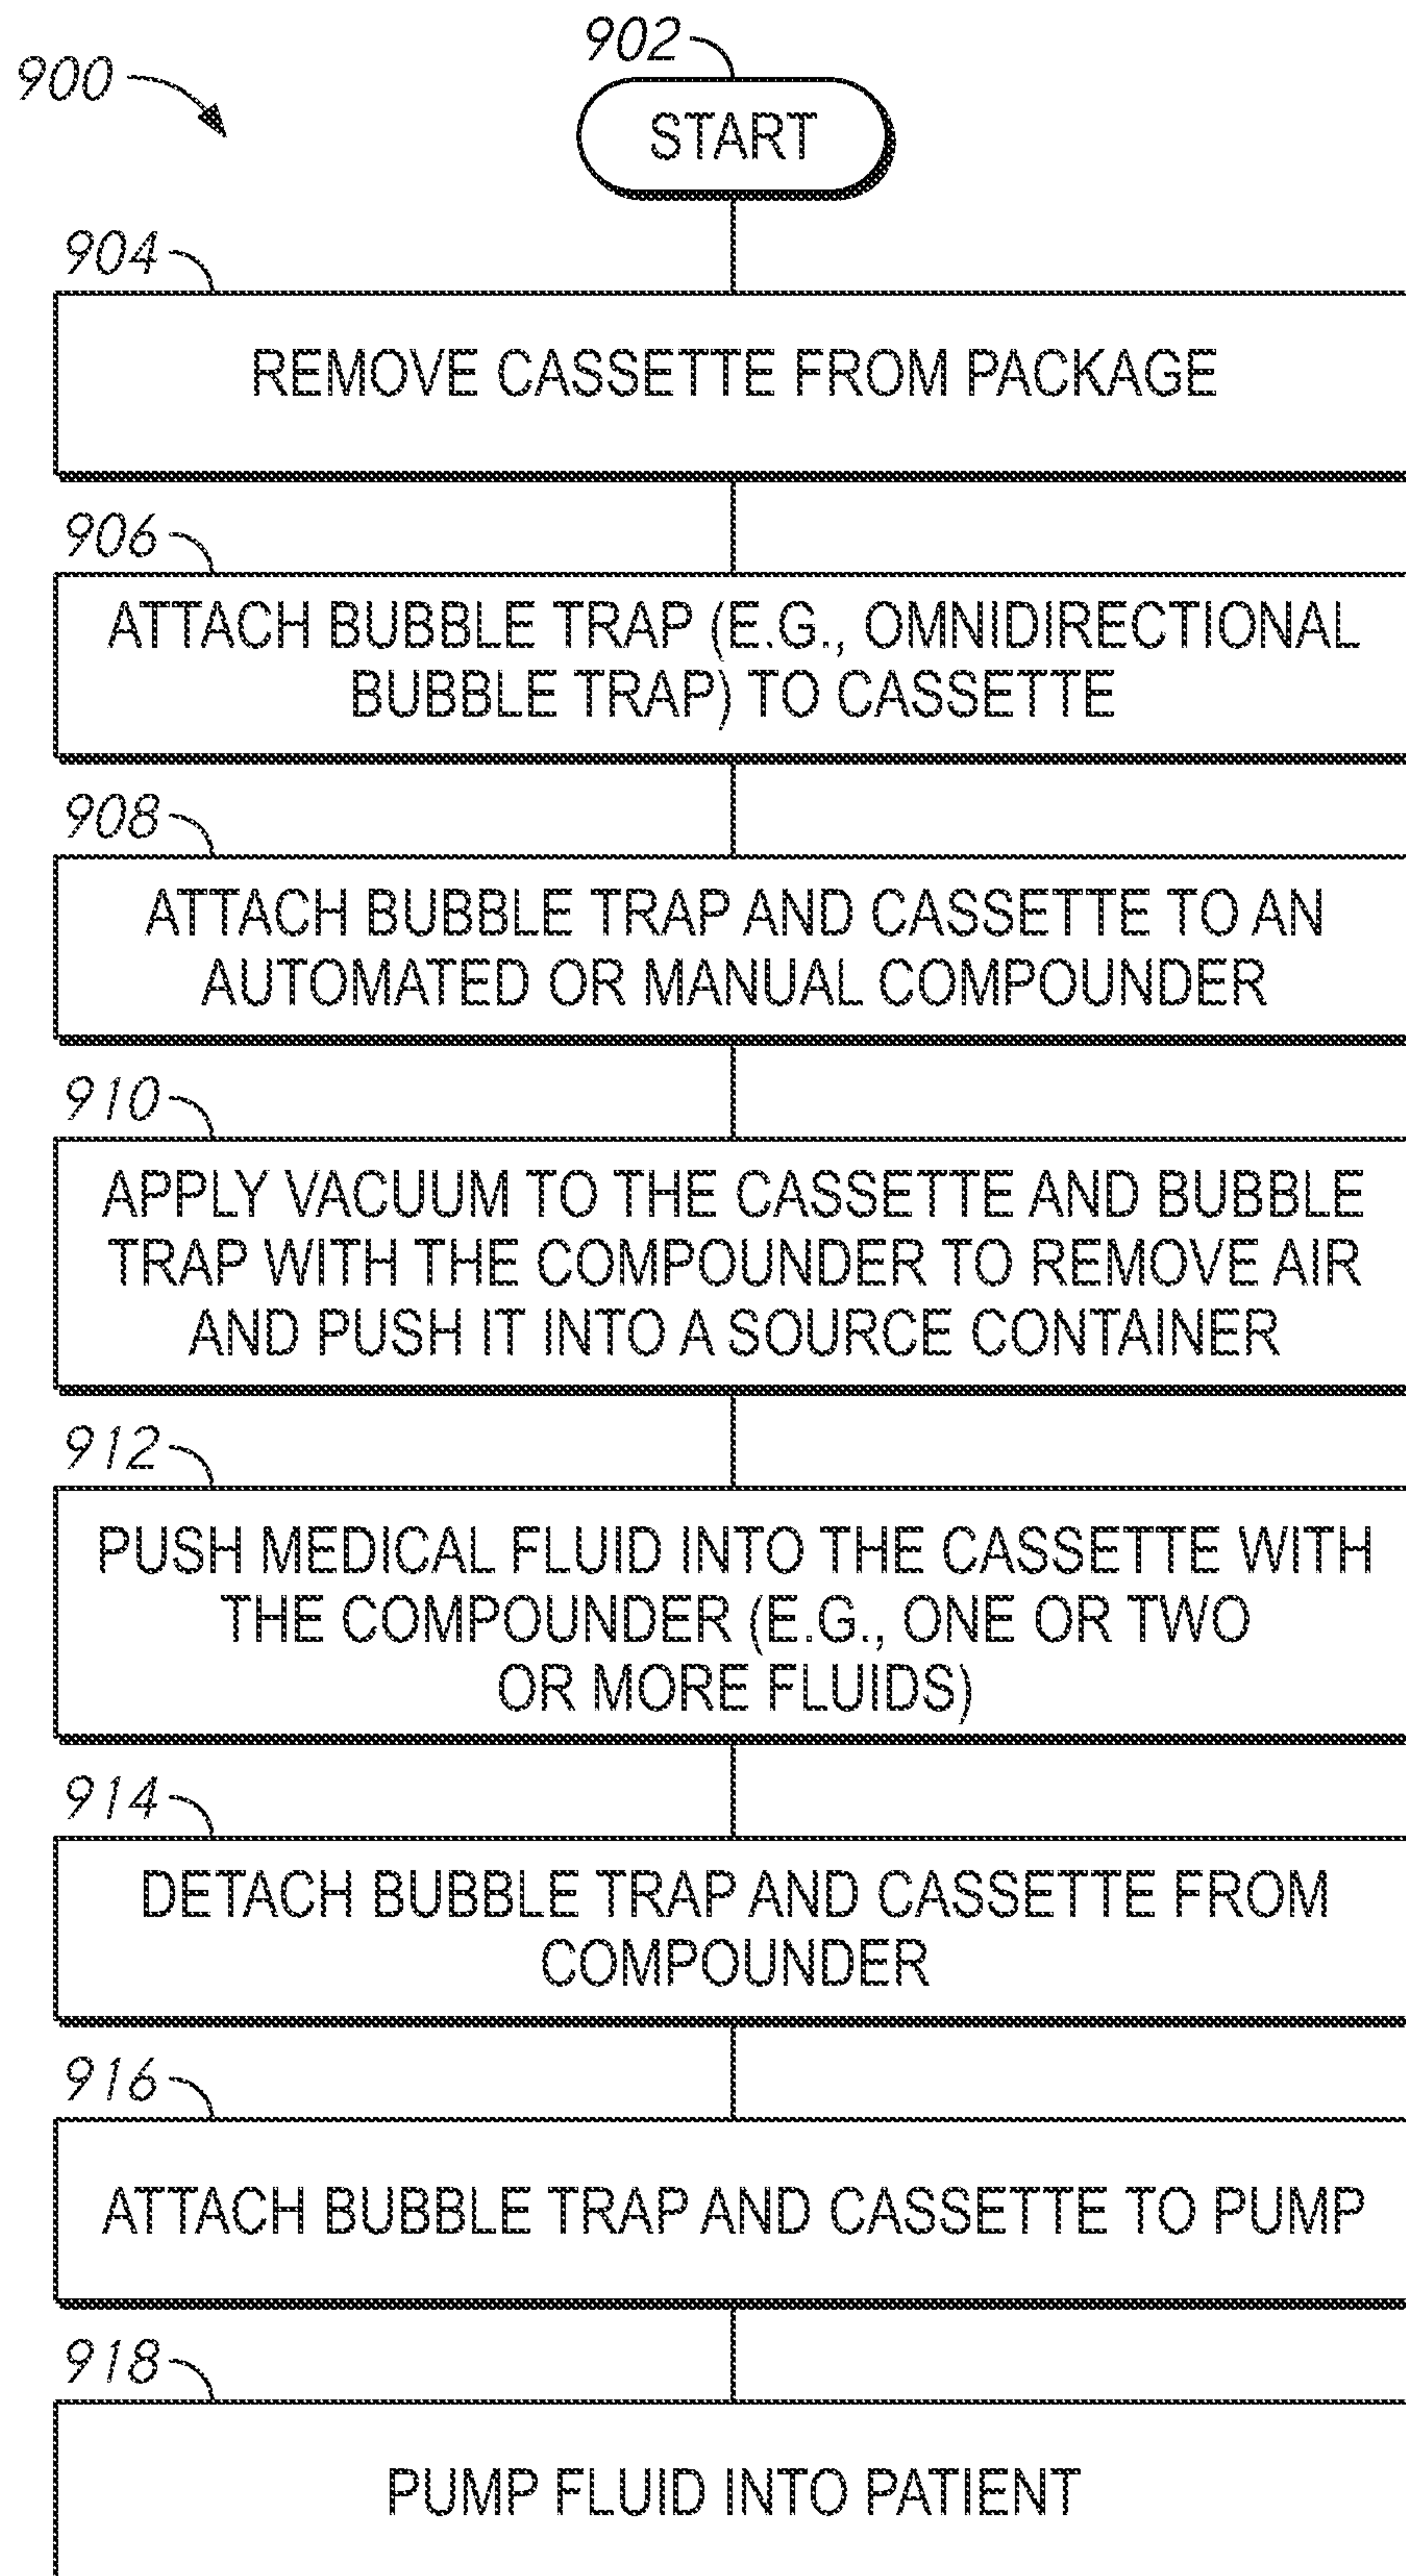


FIG. 9C

24/24

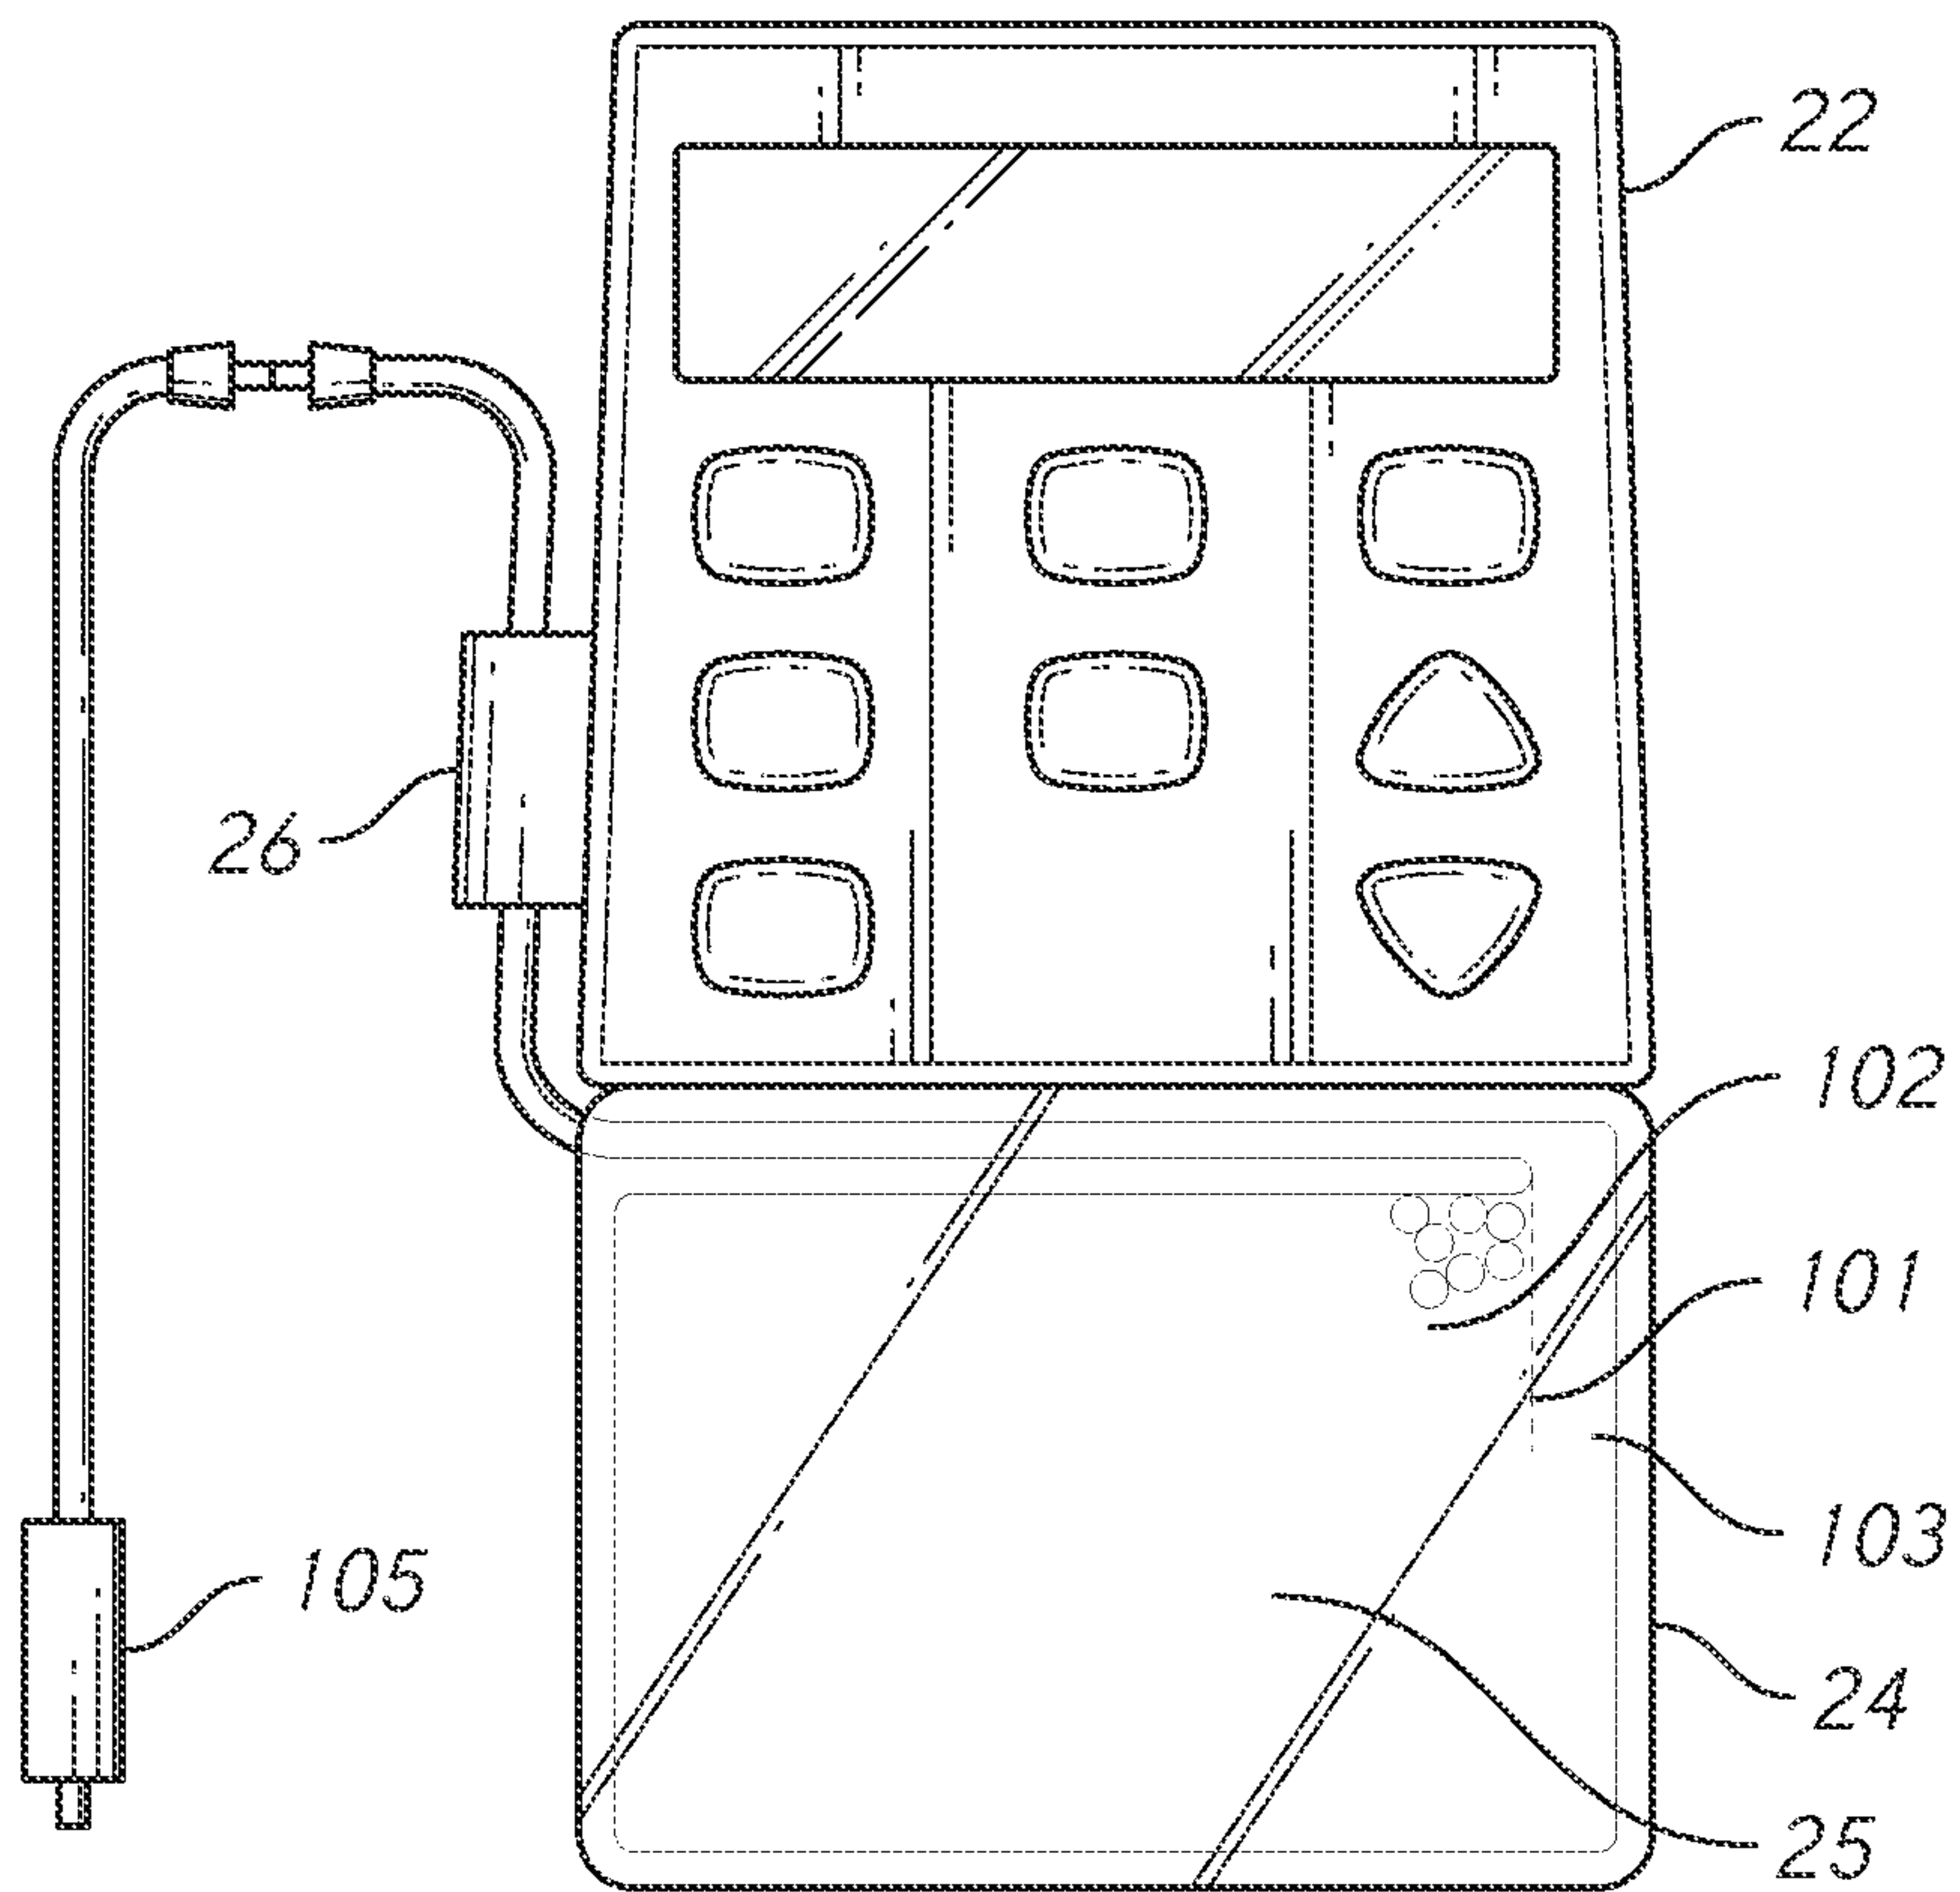


FIG. 10A

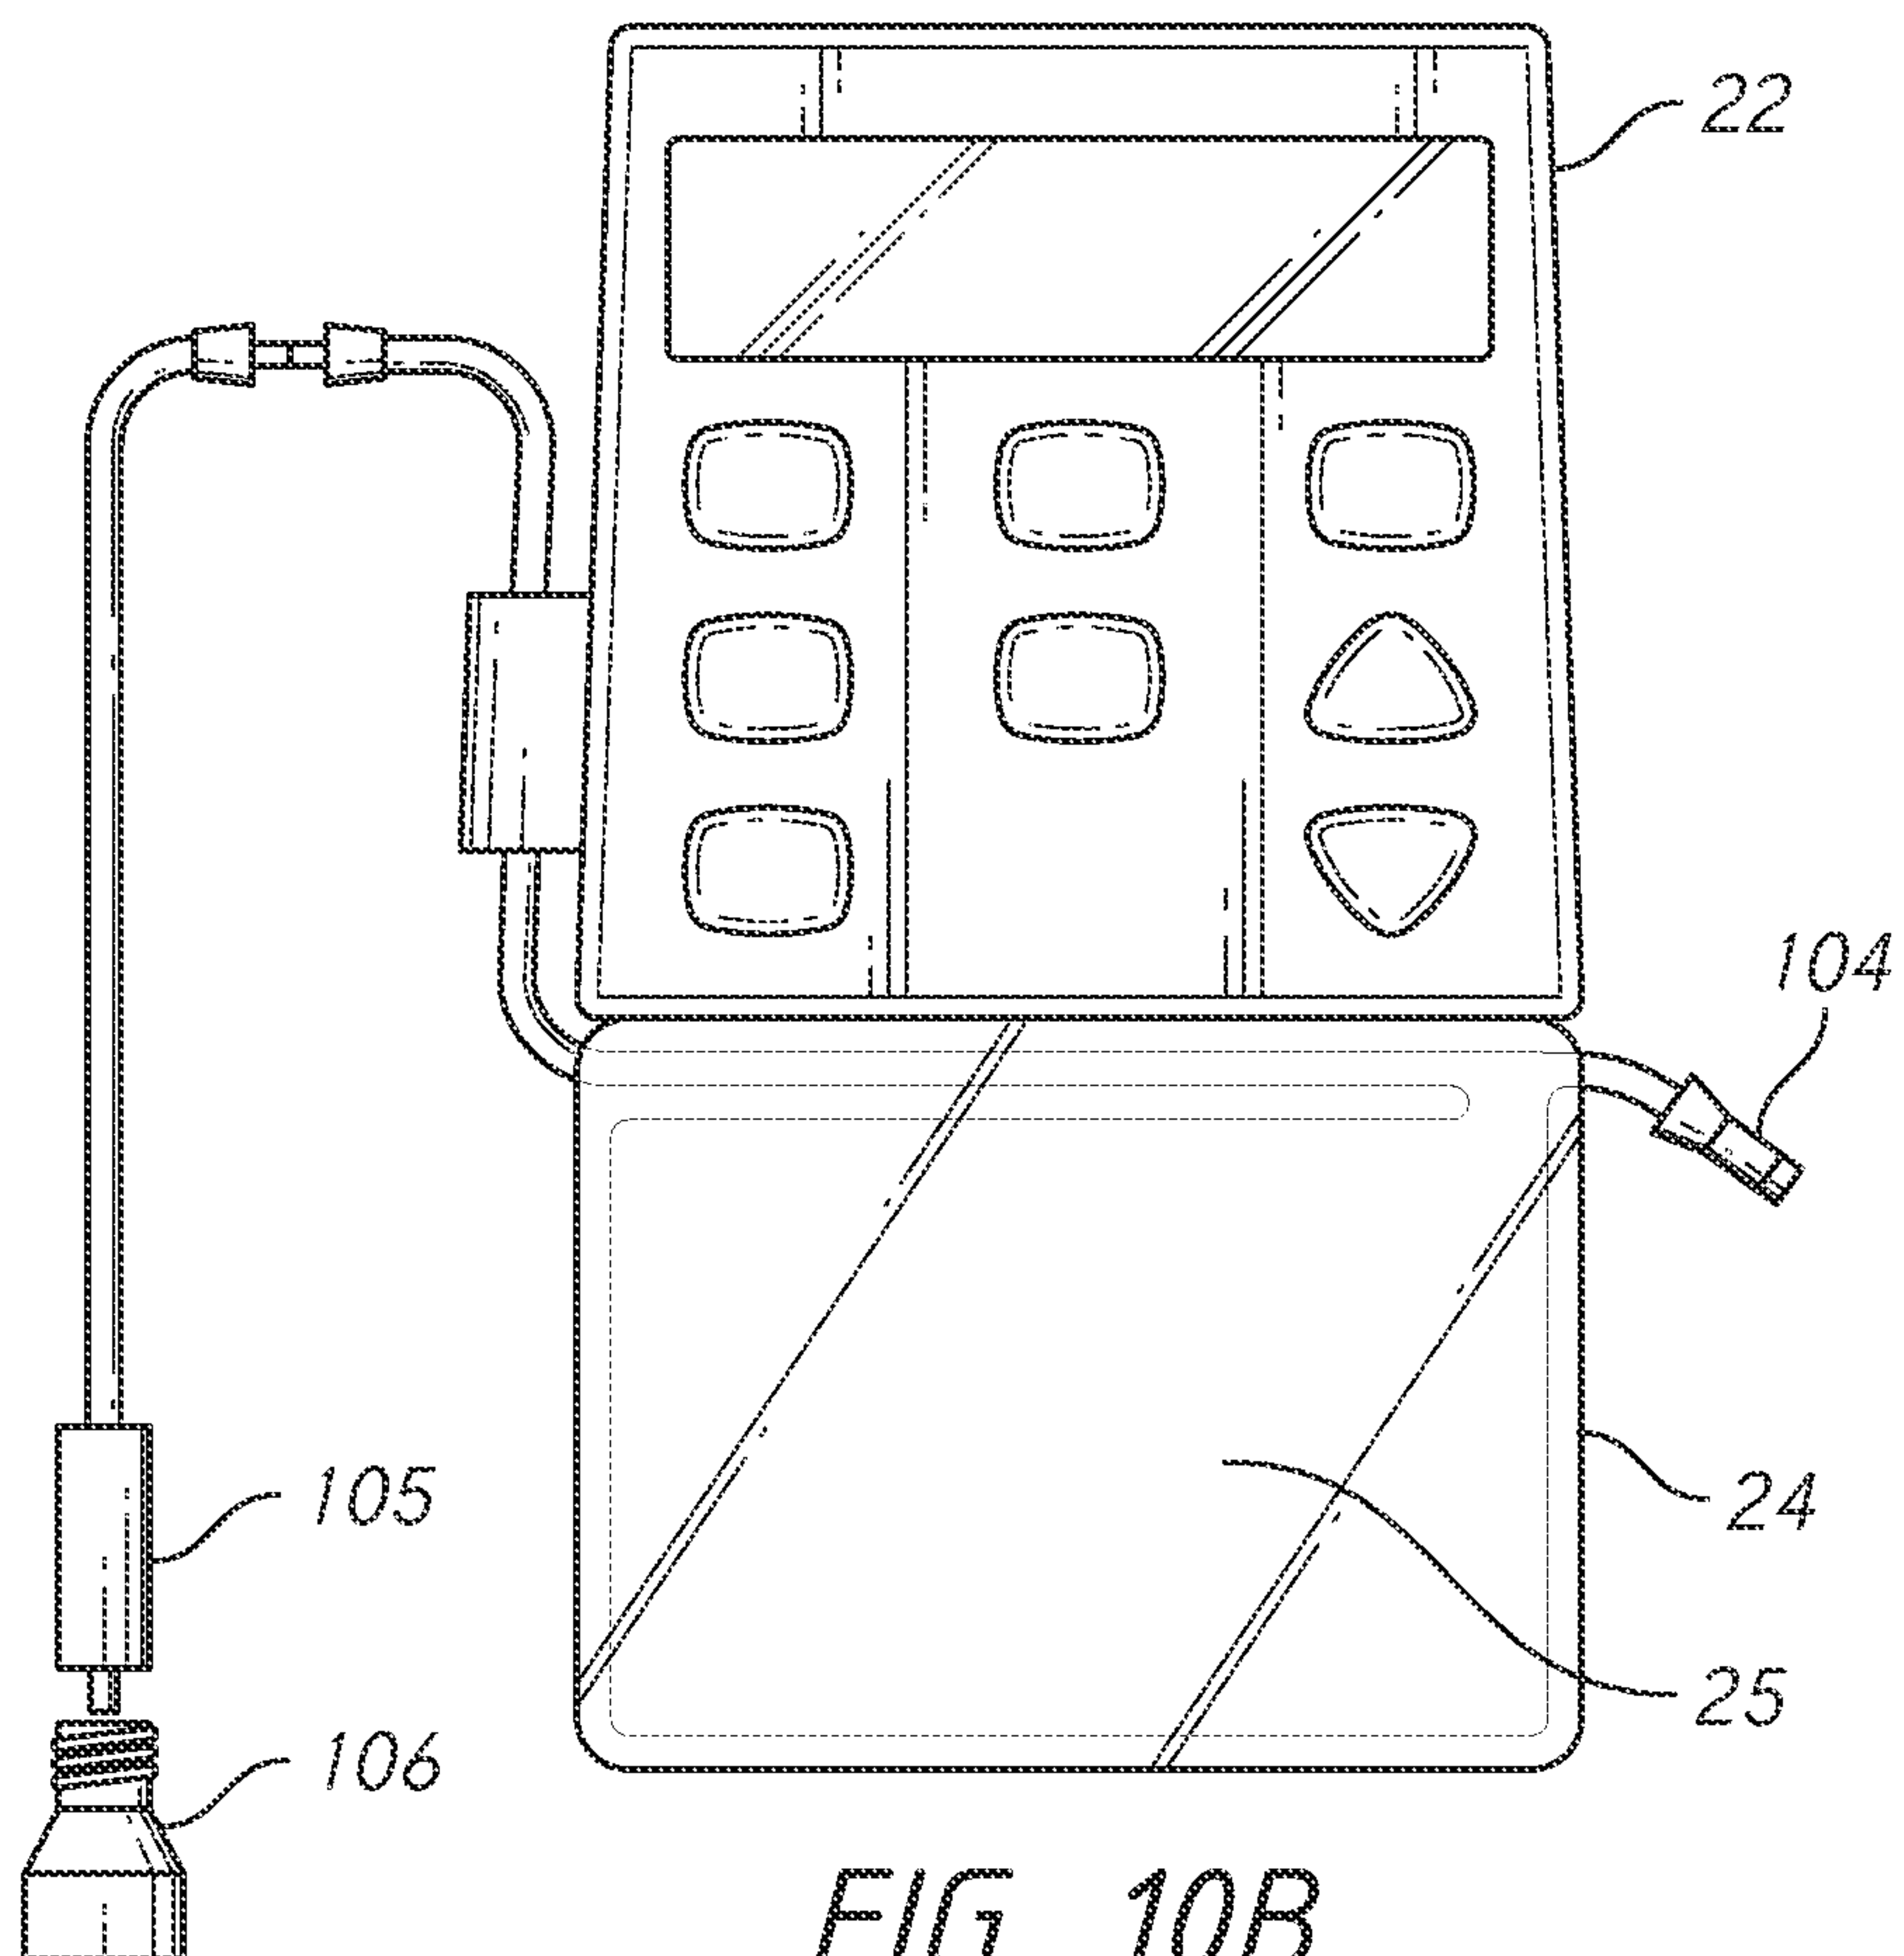


FIG. 10B

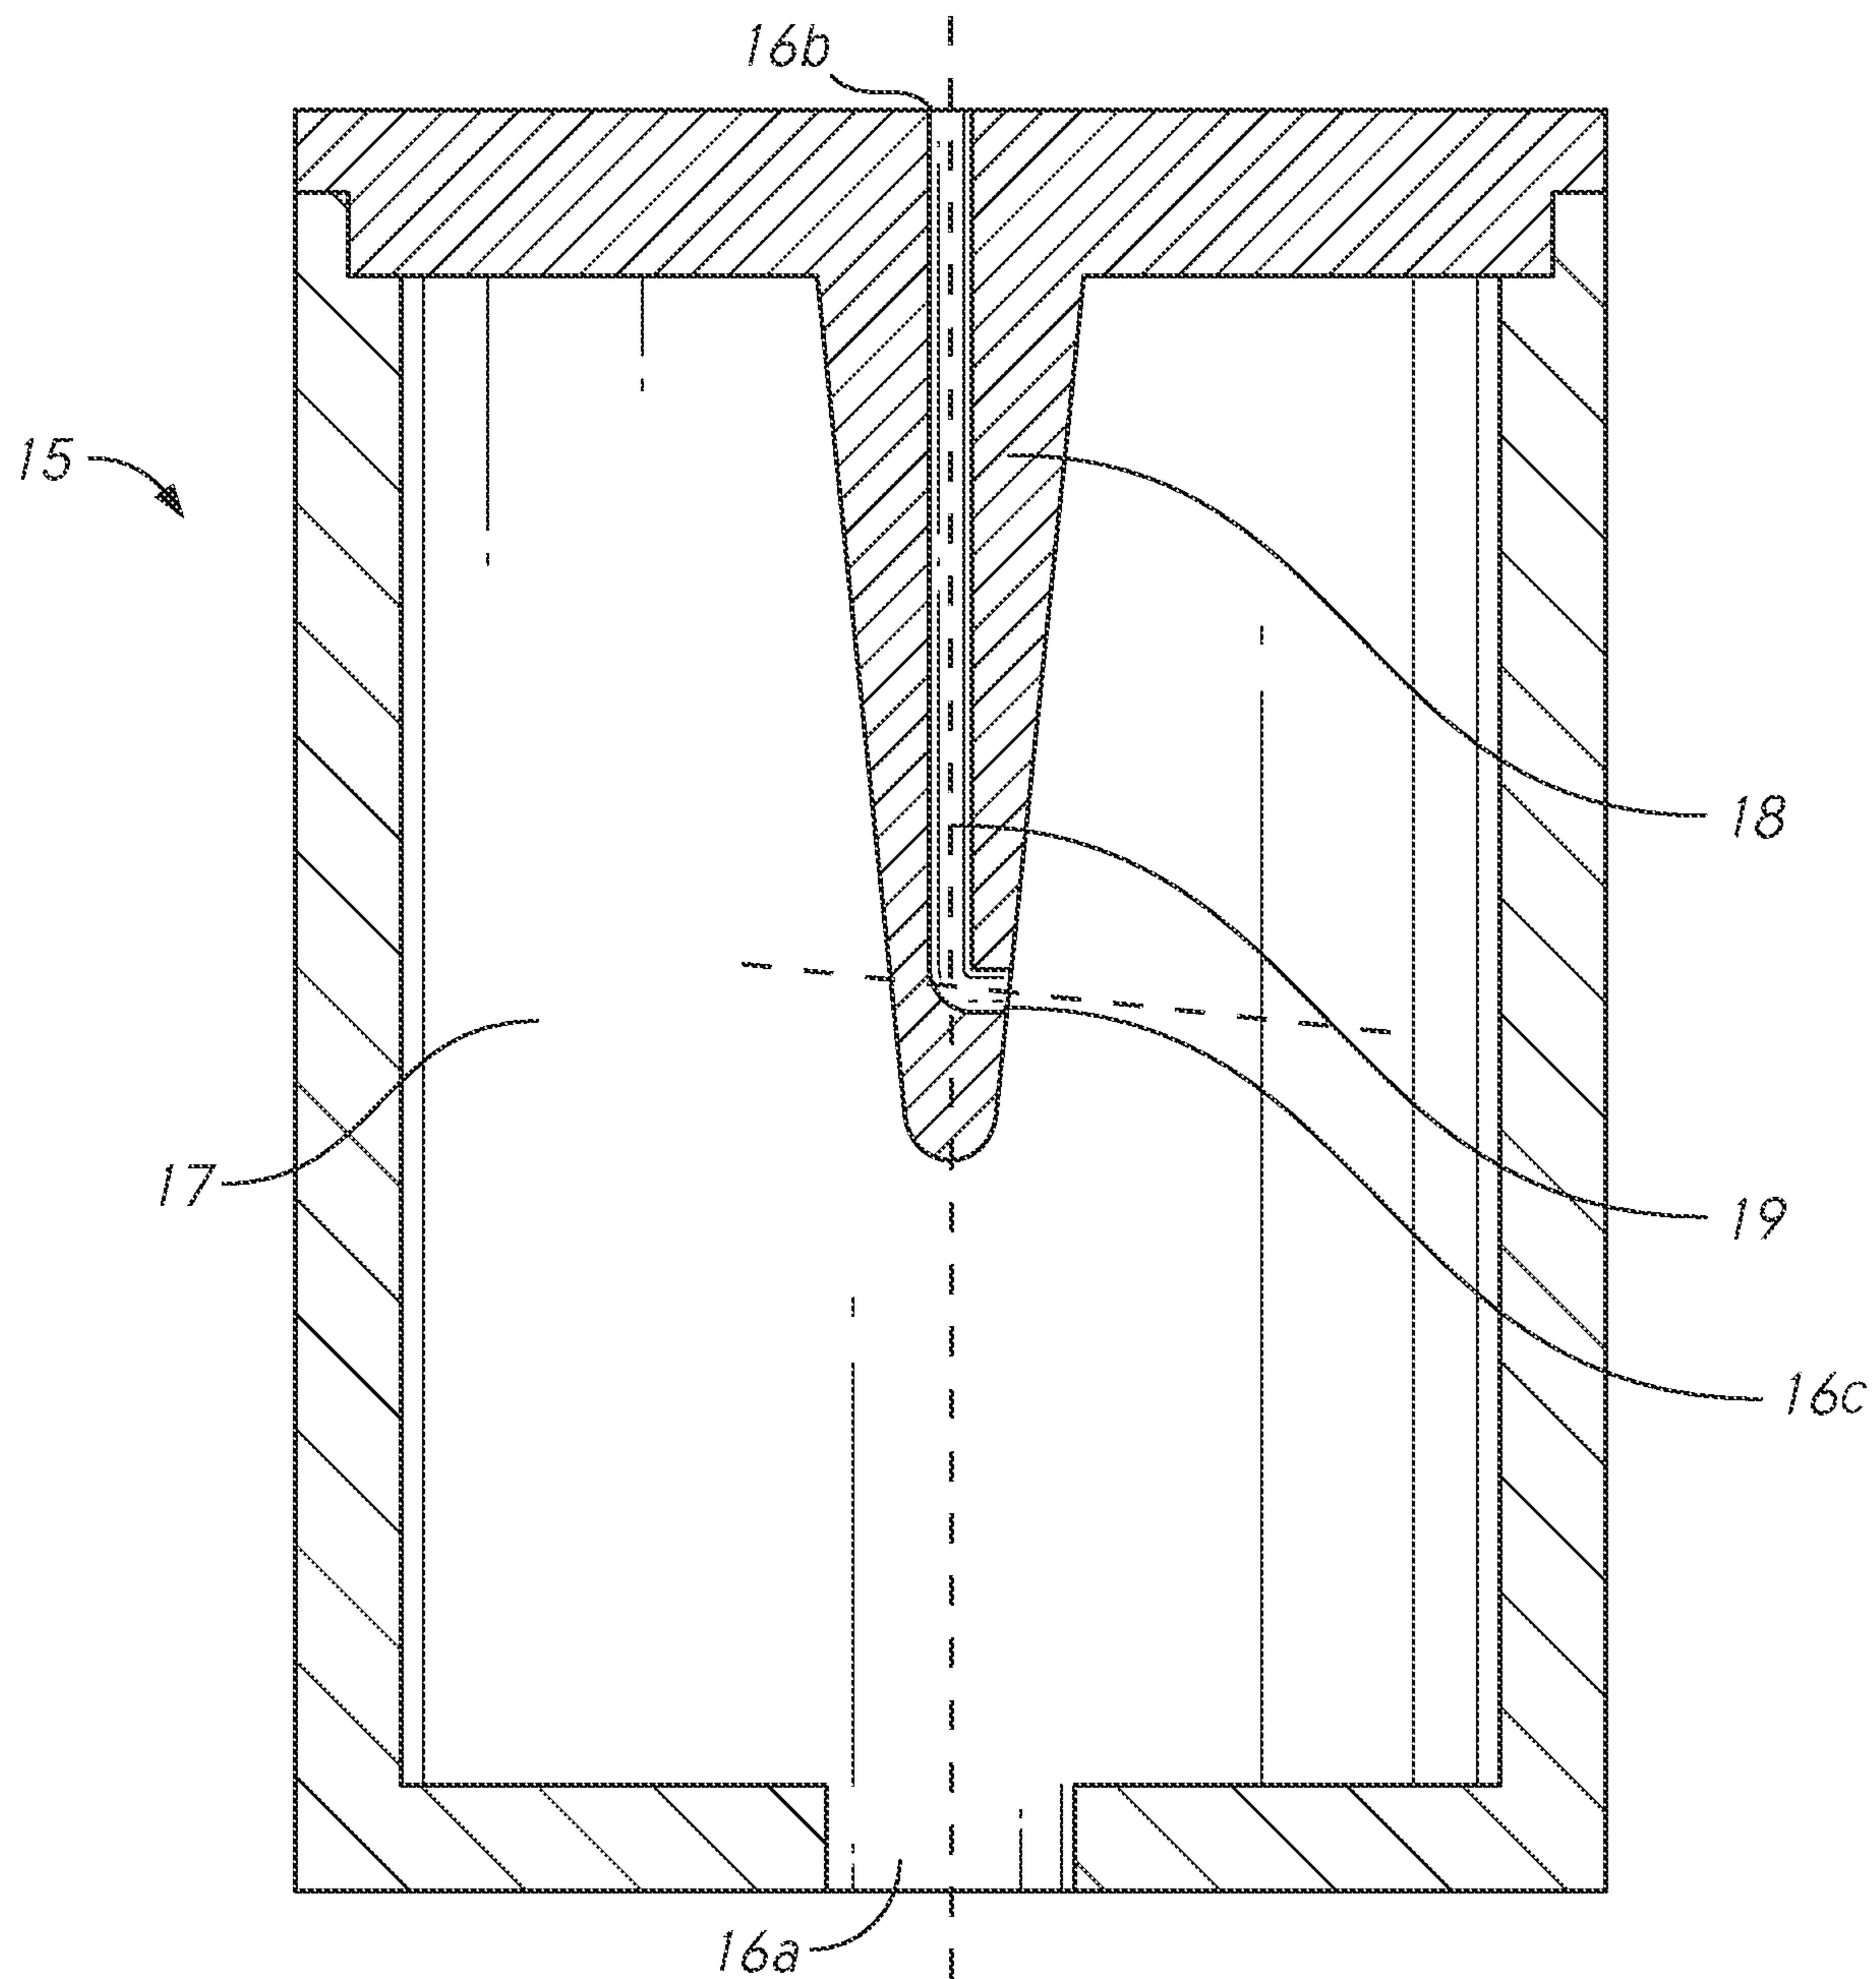


FIG. 6A