

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
2 July 2009 (02.07.2009)

PCT

(10) International Publication Number  
WO 2009/081297 A2

- (51) International Patent Classification:  
G06T 7/00 (2006.01)
- (21) International Application Number:  
PCT/IB2008/055035
- (22) International Filing Date:  
1 December 2008 (01.12.2008)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
61/014,488 18 December 2007 (18.12.2007) US
- (71) Applicant (for all designated States except US): **KONINKLIJKE PHILIPS ELECTRONICS, N.V.** [NL/NL];  
High Tech Campus Building 44, NL-5656 AE Eindhoven (NL).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **ZAGORCHEV, Lyubomir, Georgiev** [BG/US]; P.O. Box 3001, 345 Scarborough Road, Briarcliff Manor, New York 10510-8001 (US). **MANZKE, Robert** [DE/US]; P.O. Box 3001,

345 Scarborough Road, Briarcliff Manor, New York 10510-8001 (US). **CHAN, Raymond** [US/US]; P.O. Box 3001, 345 Scarborough Road, Briarcliff Manor, New York 10510 (US).

(74) Agent: **DAMEN, Daniel, M.**; Philips Intellectual Property & Standards, High Tech Campus 44, P.O. Box 220, NL-5600 AE Eindhoven (NL).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH,

[Continued on next page]

(54) Title: FEATURES-BASED 2D/3D IMAGE REGISTRATION

(57) Abstract: An image registration apparatus comprises: a features detector (34) configured to extract a two-dimensional set of features (36) from a two-dimensional image (30) and to extract a three-dimensional set of features (38) from a three-dimensional image (32); a projection processor (40) configured to project three-dimensional data into two-dimensional projection data; and a registration processor (46, 52) configured to (i) adjust parameters to register the two-dimensional set of features and the three-dimensional set of features projected by the projection processor using a projection geometry (42), and to (ii) use the adjusted parameters to register the two-dimensional image and the three-dimensional image projected by the projection processor using the projection geometry.

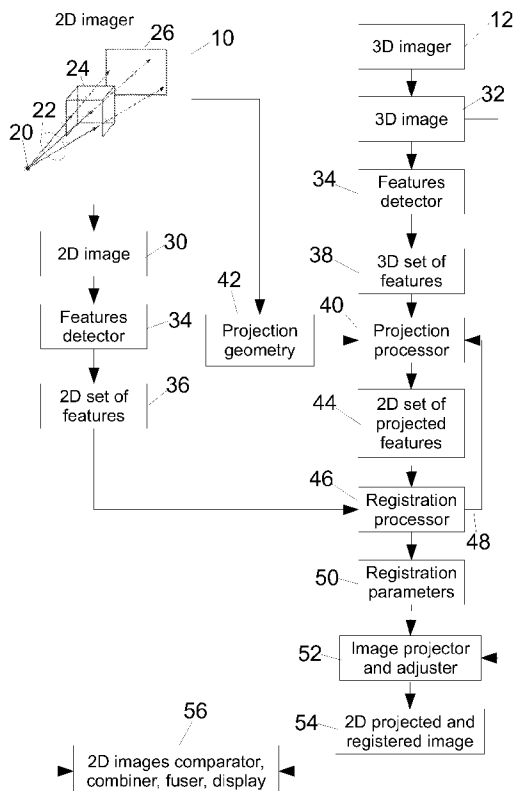


Fig. 1

WO 2009/081297 A2



GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

— *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*

**Published:**

— *without international search report and to be republished upon receipt of that report*

**Declarations under Rule 4.17:**

— *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*

009120US1

## FEATURES-BASED 2D/3D IMAGE REGISTRATION

The following relates to the medical imaging arts. In some embodiments it relates to registering two-dimensional (2D) x-ray fluoroscopy images with three-dimensional (3D) images acquired by computed tomography, magnetic resonance  
5 imaging, or another imaging modality. More generally, however, the following relates to registering two-dimensional images acquired by any medical imaging modality with three-dimensional images acquired by the same or a different medical imaging modality.

In medical imaging procedures, it is sometimes the case that relevant imaging data is acquired using both two-dimensional and three-dimensional imaging. In  
10 some such cases, it is useful to generate and register a two-dimensional representation of the three-dimensional image with a corresponding two-dimensional image, so as to compare or combine information provided by the two techniques.

One example sometimes arises in interventional cardiac electrophysiology. During this procedure, x-ray fluoroscopy is sometimes used to visualize catheters or other  
15 interventional instruments. Advantageously, x-ray fluoroscopy images can be acquired using a "C-arm" type apparatus in which the x-ray tube and x-ray detector are mounted on opposite ends of the C-arm, and the patient is disposed in the gap. A C-arm type apparatus is relatively open, thus making the patient readily accessible to medical personnel. However, some soft tissue anatomy is not effectively imaged by x-ray fluoroscopy.  
20 Further, fluoroscopic images are typically acquired at a low x-ray dose, which can compromise resolution.

Accordingly, it is known to acquire pre-operative images of the patient before undergoing the cardiac electrophysiology procedure, using a three-dimensional imaging technique such as multi-slice computed tomography (CT) or magnetic resonance  
25 imaging (MRI), either of which provide better soft tissue contrast than x-ray fluoroscopy. The pre-operatively acquired CT or MRI images are then fused with the x-ray fluoroscopic images acquired during the cardiac electrophysiology procedure so that the CT or MRI images provide the missing soft tissue contrast.

CT or MRI images are typically generated for a three-dimensional volume;  
30 whereas, the x-ray fluoroscopy images are two-dimensional. It is known to mathematically project a three-dimensional image into a two-dimensional image using

009120US1

ray-casting techniques. Applying ray casting to the CT or MRI image produces a two-dimensional image. However, the mathematically projected CT or MRI image is generally not spatially registered with the x-ray fluoroscopic image, because the projection geometry of the x-ray fluoroscope respective to the patient generally differs  
5 from the projection geometry used in the mathematical generation of the CT or MRI projection. In some cases, further error may result due to distortions or other imperfections or artifacts in the x-ray fluoroscopic image and/or in the three-dimensional CT or MRI image.

10                   The following provides improvements, which overcome the above-referenced problems and others.

                  An image registration process is disclosed, comprising: extracting a two-dimensional set of features from a two-dimensional image; extracting a three-dimensional set of features from a three-dimensional image; mathematically  
15 projecting the three-dimensional set of features into a two-dimensional set of projected features using a projection geometry; first registering the two-dimensional set of features and the two-dimensional set of projected features; and second registering the two-dimensional image and a mathematical projection of the three-dimensional image using parameters derived from the first registering.

20                   A digital storage medium or media is capable of storing instructions executable by a digital system to perform the method of the preceding paragraph.

                  An image registration apparatus is disclosed, comprising: a features detector configured to extract a two-dimensional set of features from a two-dimensional image and to extract a three-dimensional set of features from a three-dimensional image; a projection  
25 processor configured to project three-dimensional data into two-dimensional projection data; and a registration processor configured to (i) adjust parameters to register the two-dimensional set of features and the three-dimensional set of features projected by the projection processor using a projection geometry, and to (ii) use the adjusted parameters to register the two-dimensional image and the three-dimensional image projected by the  
30 projection processor using the projection geometry.

                  Also disclosed is an apparatus comprising: a two-dimensional imager configured to acquire a two-dimensional image; a three-dimensional imager configured to

009120US1

acquire a three-dimensional image; a features detector configured to extract a two-dimensional set of features from the two-dimensional image and to extract a three-dimensional set of features from the three-dimensional image; a projection processor configured to project three-dimensional data into two-dimensional projection data; and a registration processor configured to register the two-dimensional image and the three-dimensional image projected by the projection processor using parameters adjusted to register the two-dimensional set of features and the three-dimensional set of features projected by the projection processor.

One advantage resides in faster 2D/3D image registration.

Another advantage resides in more accurate 2D/3D image registration.

Another advantage resides in faster interventional imaging.

Still further advantages of the present invention will be appreciated to those of ordinary skill in the art upon reading and understand the following detailed description.

The drawings are only for purposes of illustrating the preferred embodiments, and are not to be construed as limiting the invention.

FIGURE 1 diagrammatically shows a 2D/3D multi-modality imaging apparatus.

FIGURE 2 diagrammatically shows a 3D/3D multi-modality imaging apparatus with registration of two-dimensional projections of three-dimensional images acquired by the different modalities.

With reference to FIGURE 1, a 2D/3D multimodality imaging system includes a two-dimensional imager **10**, such as an x-ray fluoroscopy apparatus, and a three-dimensional imager **12**, such as a magnetic resonance imaging (MRI) system, a computed tomography (CT) imaging system, positron emission tomography (PET) scanner, a gamma camera, and so forth. The two-dimensional imager **10** is optionally capable of three-dimensional imaging but is used in the present 2D/3D imaging system as the two-dimensional imager. For example, the two-dimensional imager **10** is contemplated as a CT scanner operating without gantry rotation.

The two-dimensional imager **10** is a projection-type imager including a source **20**, such as an x-ray tube in the case of an x-ray fluoroscopy apparatus, that transmits radiation **22** through an imaging region **24** containing a subject (not shown), such

009120US1

that a generally oppositely positioned two-dimensional detector array **26** detects the transmitted radiation as a function of position to form a two-dimensional image **30** of a projection-type. The two-dimensional image **30** therefore has a projection geometry characterized by projection parameters such as angulation, source position, detector position, or other geometrical parameters, and optionally also by projection parameters related to distortion, such as one or more distortion parameters characterizing the so-called "pincushion" distortion that is sometimes observed in x-ray fluoroscopes and other projection-type 2D imaging apparatuses. The projection geometry is at least approximately known, for example based on the nominal settings of the x-ray source and detector positions. In some embodiments, a precise calibration of the two-dimensional imager **10** provides highly precise projection parameters for the projection geometry, including precise geometrical parameters and quantitative values for the distortion parameters.

The three-dimensional imager **12** acquires a three-dimensional image **32**. For example, if the three-dimensional imager **12** is an MRI, it acquires such a three-dimensional image **32** by sampling k-space three-dimensionally and reconstructing the k-space samples into the three-dimensional image **32**. If the three-dimensional imager **12** is a CT scanner, it acquires projection data while the x-ray tube revolves around the subject, with the third dimension provided by having multiple rows of detectors (multi-slice CT) and/or by moving the patient in discrete increments or continuously (helical CT), followed by filtered backprojection or another reconstruction that reconstructs the projection data into the three dimensional image **32**. Other approaches can be used, depending upon the type of three-dimensional imager **12** and the type of acquisition desired by the radiologist or other medical professional.

The relationship between the projection geometry of the two-dimensional image **30** and the spatial frame of reference of the three-dimensional image **32** is known approximately, based on how the subject is positioned in the two different imagers **10**, **12**. In some embodiments, this relationship is more precisely known, for example if the two different imagers **10**, **12** are embodied integrally together as a hybrid imaging system, or a cross-imager mechanical alignment mechanism is used. In any case, however, there will generally be some misregistration between the two-dimensional image **30** acquired by the two-dimensional imager **10**, on the one hand, and the three-dimensional image **32** acquired by the three-dimensional imager **12**, on the other hand. This misregistration can take

009120US1

various forms or combinations of forms, such as rigid translational misregistration, rigid rotational misregistration, non-rigid translational and/or rotational misregistration, misregistration due to pincushion distortion or other types of distortion in one or both images **30**, **32**, and so forth. Accordingly, it is desired to mathematically project the three-dimensional image **32** to form a two-dimensional projection image, and to register this two-dimensional projection image with the two-dimensional image **30** acquired by the two-dimensional imager **10**.

A features detector **34** processes the two-dimensional image **30** to extract a two-dimensional set of features **36** from the two-dimensional image **30**. The features detector **34** also processes the three-dimensional image **32** to extract a three-dimensional set of features **38** from the three-dimensional image **32**. In the embodiment of FIGURE 1, the same features detector **34** is applied both to the two-dimensional image **30** and to the three-dimensional image **32**; however, it is also contemplated to use two different features detectors, for example, wherein one of the feature detectors is optimized for two-dimensional images and the other feature detector is optimized for three-dimensional images. If two different features detectors are used in this fashion, the detected features should be comparable, such as of the same type.

The features detector **34** is capable of detecting, for example, corner features suitably represented as corner points. For detecting corner features, such a feature detector **34** operates via a corner detection algorithm such as for example by identifying high intensity gradient regions typically corresponding to corners by identifying locally maximum eigenvalues of an inertia matrix of the image gradient along each direction, and identifying a discrete set of line intersections. Advantageously, substantially the same corner features are generally detected for both the two-dimensional and three-dimensional images, even if the contrast mechanisms of the two imagers **10**, **12** are substantially different (for example, x-ray versus magnetic resonance). The derivative-based nature of corner detection, coupled with a high likelihood of contrast for corner structures of the subject, ensures that the corner detection process is generally independent of contrast type, contrast level, and other image characteristics. Another advantage of using corner detection by the features detector **34** is that corner points are discrete in both two-dimensions and in three-dimensions.

009120US1

The features detector **34** is alternatively or additionally also capable of detecting other types of features. For example, the features detector **34** is alternatively or additionally capable of detecting edge features. In some embodiments, the features detector **34** is capable of detecting edge features via an edge detection algorithm which is implemented as follows. Lines in the projected two-dimensional image correspond to the projection of interfaces within the three-dimensional image that are oriented along the x-ray beam **22**. These interfaces are suitably detected by using the voxel intensity gradient magnitude and interface direction, along with the x-ray beam direction known from the projection geometry. The interface locations can be mapped from 3D to 2D using the projection matrix of Equation (2) to form a map of edge and corner locations.

In general, the features detector **34** reduces the respective images **30**, **32** into two-dimensional or three-dimensional sets of features **36**, **38** respectively, that are smaller respective subsets of data and therefore are readily correlated in space and are more efficiently processed from a computational standpoint as compared with the full images **30**, **32**. The respective sets of features **36**, **38** retain the geometries of the source images **30**, **32**. Thus, for a features detector **34** that detects corner features, the two-dimensional set of features **36** comprises a set of points in a plane, while the three-dimensional set of features **38** comprises a three-dimensional "cloud" of points. Similarly, for an edge detector the two-dimensional set of features **36** comprises a set of lines lying coplanar in a plane, while the three-dimensional set of features **38** comprises a three-dimensional arrangement of lines.

A projection processor **40** mathematically projects the three-dimensional set of features **38** in accordance with a projection geometry **42** that is at least initially set to the projection geometry used by the two-dimensional imager **10** in acquiring the two-dimensional image **12**. For an illustrative interventional C-arm x-ray fluoroscopy apparatus such as the Allura XPer FD10 (available from Philips Medical Systems, Eindhoven, the Netherlands), the projection geometry is suitably defined as follows. A vector,  $\mathbf{s}$  extends from iso-center to the x-ray source **20**, while a vector  $\mathbf{d}$  extends from iso-center to a center of the detector **26**. Two normals  $\mathbf{n}_1$  and  $\mathbf{n}_2$  define the detector plane, and are known for every projection. Any three-dimensional point  $\mathbf{P}$  can therefore be mapped (i.e., projected) to a two-dimensional point  $\mathbf{p}$  on the detector **26** given any particular C-arm angulation. Expanding these vectors into Cartesian coordinates yields:

009120US1

$$\begin{aligned}
\mathbf{s} &= [s_x, s_y, s_z]^T \\
\mathbf{d} &= [d_x, d_y, d_z]^T \\
\mathbf{n}_1 &= [n_{1x}, n_{1y}, n_{1z}]^T \\
\mathbf{n}_2 &= [n_{2x}, n_{2y}, n_{2z}]^T \\
\mathbf{P} &= [X, Y, Z]^T \\
\mathbf{p} &= [u, v, \mu]^T
\end{aligned} \tag{1}$$

The matrix vector equation defining the projection geometry **42** can be written as:

$$\begin{bmatrix} u \\ v \\ \mu \end{bmatrix} = \begin{bmatrix} n_{1x} & n_{2x} & s_x - X \\ n_{1y} & n_{2y} & s_y - Y \\ n_{1z} & n_{2z} & s_z - Z \end{bmatrix}^{-1} \begin{bmatrix} s_x - d_x \\ s_y - d_y \\ s_z - d_z \end{bmatrix} \tag{2}$$

Equation (2) is applied by the projection processor **40** to each three-dimensional corner point **P** (in the case of a corner detector) of the three-dimensional set of features **38** using the selected projection geometry **42** to generate corresponding points **p** of a two-dimensional set of projected features **44**.

A registration processor **46** registers the two-dimensional set of projected features **44** with the two-dimensional set of features **36** extracted from the two-dimensional image **30**. If the registration entails adjusting projection parameters, then this registration process is optionally iterative, following an iteration loop **48** to re-project the three-dimensional set of features **38** using projection parameters adjusted by the registration in an iterative manner. The output of the registration processor **46** is a set of one or more registration parameters **50**. The registration may entail adjustment of various parameters such as projection parameters (e.g., angulation, magnification, source/detector locational parameters, a parameter quantifying pincushion distortion, or so forth), rigid translations or rotations, nonrigid translations or rotations, and so forth. The registration may entail selecting or refining projection parameters of the projection geometry used for the mathematical projecting operation. However, computing the registration parameters **50** based on the complete images **30**, **32** is computationally intensive, especially for iterative registration techniques.

The registration parameters **50** are efficiently adjusted by the adjustment processor **46** (optionally including iterative re-projection via loop **48** and projection processor **40**) respective to the smaller sets of features **36**, **38**. As one example, the two-dimensional set of features **36** extracted from the two-dimensional image **30** are taken as the reference, and projection parameters of the projection geometry **42** and/or spatial parameters of the two-dimensional set of projected features **44** are adjusted.

009120US1

If the projection geometry **42** is accurately or precisely known, for example based on calibrations of the two-dimensional imager **10**, and only rigid registration is to be performed, then the optimization space includes only six parameters, e.g. three rotations and three translations respective to the spatial parameters of the two-dimensional set of projected features, and the registration processor **46** can employ a downhill simplex method for numerical adjustment and optimization of these six parameters. The adjustment or optimization is suitably respective to a similarity measure computed (for example) as a sum of the distance squared between each corner point in the two-dimensional set of features **36** and the corresponding projected corner point in the two-dimensional set of projected features **44**.

If the projection geometry **42** is not known with sufficient accuracy or precision, then the registration processor **46** optionally adjusts projection parameters of the projection geometry **42** as part of the registration. For example, the projection processor **40** is applied to the three-dimensional set of features **38** with a plurality of different projection angulations deviating by selected amounts from the nominal angulation used in acquiring the two-dimensional image **30**. The registration is applied to the two-dimensional set of projected features **44** generated by the mathematical projection at each selected angulation, the "best fit" registration is selected, and the angulation corresponding to the best fit is selected as the adjusted angulation of the adjusted projection geometry **42**. This brute force approach is feasible because the dimensionality reduction provided by registering only the features (e.g., corner points) rather than registering entire images provides fast processing. Additionally or alternatively, the angulation or other projection parameters can be included as parameters that are optimized by the registration processor **46** using a least squares minimization or another optimization technique. Optional iterative or exhaustive registration in which the registration processor **46** is applied to different two-dimensional sets of projected features **44** generated by the projection processor **40** with different mathematical projection angulations (or with other variations in the projection geometry **42**) are diagrammatically indicated in FIGURE 1 by an iteration loop arrow **48**.

In most situations, it is anticipated that the projection geometry of the two-dimensional image **30** will be known with a relatively high degree of accuracy, for example based on a calibrated projection geometry of the two-dimensional imager **10** used in acquiring the two-dimensional image **30**. In such embodiments, it is generally suitable to

009120US1

assume that each feature in the two-dimensional set of features **36** and the closest feature in the two-dimensional set of projected features **44** both correspond to the same corner point of the subject. In such a case, the similarity measure optimized by the registration processor **46** is suitably computed as a sum of distances-squared where each distance is  
5 between a feature of the set of two-dimensional features **36** and the closest feature of the set of two-dimensional projected features **44**.

It is contemplated, however, that in some situations, the projection geometry of the two-dimensional image **30** will be known with sufficiently limited precision and/or accuracy that it is not reasonable to assume that each feature in the two-dimensional set of  
10 features **36** and the closest feature in the two-dimensional set of projected features **44** both correspond to the same corner point of the subject. In such cases, it is contemplated for the registration processor **46** to apply a combinatoric algorithm to associate features of the two-dimensional set of projected features **44** with corresponding features of the two-dimensional set of features **36** extracted from the two-dimensional image **30**.

As further shown in Fig. 1, the adjusted registration parameters **50** are used  
15 by an image projector and adjuster **52** to register the respective 2D and 3D images **30**, **32** in a second registration step. The registration parameters **50** are adjusted respective to the two-dimensional set of features **36** and the two-dimensional set of projected features **44**; however, these features **36**, **44** are representative of the spatial characteristics of the  
20 respective two- and three-dimensional images **30**, **32** and accordingly the registration parameters **50** are applicable in the second registration process performed by the image projector and adjuster **52**, which projects the three-dimensional image **32** and adjusts the projected image in accordance with the projection geometry **42** and the registration parameters **50** to produce a two-dimensional projected and registered image **54**, which is  
25 registered with the two-dimensional image **30**.

The projection performed by the image projector and adjuster **52** can employ substantially any type of 3D-to-2D projection method, such as a digitally reconstructed radiograph (DRR) method that sets each point in the projection plane to the  
30 the (virtual) point in the projection plane. Other projection methods are also contemplated, such as a maximum intensity projection (MIP) that sets each point in the projection plane

009120US1

to the largest value along the line connecting the (virtual) source with the (virtual) point in the projection plane.

The two-dimensional projected image **54** is suitably compared or combined with the two-dimensional image **30** acquired by the two-dimensional imager **10** by an image processor **56**, such as an image combiner or fusion processor, an image comparator, an image display (such as a user interface with a graphical display) and so forth. For example, the 2D image **30** and the 2D projected and registered image **54** can be fused by an image fusion technique and the fused image displayed, or the two images **30**, **54** can be displayed side-by-side or in a vertical arrangement. In the latter case, it is contemplated to have locked pointers of a mouse or other pointing device that are displayed at the same spatial position in both of the two displayed images **30**, **54** so that a radiologist can readily locate corresponding features in the two images **30**, **54**.

Although the described registration process is expected to provide accurate and precise results in many cases, in some instances the resulting image registration may be less than fully satisfactory. In some situations, the registered two-dimensional images **30**, **54** are compared and, if not aligned within a preselected threshold or to the satisfaction of the radiologist, then subjected to another image registration procedure such as an intensity-based image registration procedure performed by the image processor **56** or another component.

One contemplated application for the multimodality imaging system of FIGURE 1 is in the area of interventional cardiac electrophysiology. Interventional cardiac electrophysiology procedures are typically performed under x-ray fluoroscopy for visualizing catheters or other interventional devices relative to highly attenuating structures of the patient such as the thoracic spine and ribs. These projections do not however contain information about soft-tissue anatomy. Accordingly, it is advantageous to fuse these two-dimensional x-ray fluoroscopy images with pre-operatively acquired volumetric cardiac helical or multi-slice CT or MRI images. The system of FIGURE 1 provides rapid fusion of the two-dimensional x-ray fluoroscopy images (corresponding to the two-dimensional images **30**) with three-dimensional CT or MRI images (corresponding to the three-dimensional images **32**) by the image comparator or combiner **56** (which in this embodiment is an image fusion processor) so as to provide real-time visualization of the

009120US1

catheters present within the thorax in relation to the cardiovascular anatomy visible in the volumetric dataset **32**.

With reference to FIGURE 2, in another contemplated application both imagers of the multimodality imaging system are capable of, and used to, generate  
5 three-dimensional images. In other words, in the embodiment of FIGURE 2 the two-dimensional imager **10** is replaced by a second three-dimensional imager **60**, which may be of the same modality or a different modality as compared with the three-dimensional imager **12**. The projection processor **40** is applied to the three-dimensional image generated by the second three-dimensional imager **60** to produce  
10 the two-dimensional image **30** having the projection geometry **42**, which in this embodiment is a selected geometry used for the mathematical projection of the three-dimensional image generated by the second three-dimensional imager **60**. From that point on, the components and processing of the multimodality imaging system of FIGURE 2 is analogous to that of the multimodality imager of FIGURE 1. The approach of  
15 FIGURE 2 can provide rapid registration of digitally reconstructed radiographs (DRRs) or other projections generated by different three-dimensional imagers, for example by CT and MRI imagers or by two different CT imagers. Faster processing is possible because the registration is performed in 2D, and moreover is performed only respective to the small features datasets **36, 44**.

20 Those skilled in the art will readily appreciate that the image registration processes disclosed herein can be embodied by a digital storage medium or media storing instructions executable by a digital system to perform the disclosed method. For example, the digital storage medium or media can be a magnetic disk, optical disk, magnetic tape, FLASH memory or other electrostatic memory, random access memory (RAM), read-only  
25 memory (ROM), Internet server, or so forth, or a combination of such media, and the stored instructions can be executable on a digital system such as a computer, digital network, Internet server, or so forth.

The preferred embodiments have been described. Modifications and alterations may occur to others upon reading and understanding the preceding detailed  
30 description. It is intended that the invention be construed as including all such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

009120US1

### CLAIMS

Having thus described the preferred embodiments, the invention is now claimed to be:

1. An image registration process comprising:
  - extracting a two-dimensional set of features **(36)** from a two-dimensional image **(30)**;
  - extracting a three-dimensional set of features **(38)** from a three-dimensional image **(32)**;
  - mathematically projecting the three-dimensional set of features into a two-dimensional set of projected features **(44)** using a projection geometry;
  - first registering the two-dimensional set of features and the two-dimensional set of projected features; and
  - second registering the two-dimensional image and a mathematical projection of the three-dimensional image using parameters derived from the first registering.
2. The image registration process as set forth in claim 1, wherein the extracting operations comprise:
  - applying a corner detection algorithm to extract features comprising corner points.
3. The image registration process as set forth in claim 1, wherein the extracting operations comprise:
  - applying an edge detection algorithm to extract features comprising line segments.
4. The image registration process as set forth in claim 1, wherein the first registering comprises:
  - adjusting spatial parameters of at least one of the two-dimensional set of features **(36)** and the two-dimensional set of projected features **(44)** selected from a group consisting of at least three rotation parameters and at least three translation parameters, the adjusted spatial parameters being used in the second registering.

009120US1

5. The image registration process as set forth in claim 1, wherein the first registering comprises:

adjusting one or more parameters of the projection geometry (42) selected from a group consisting of an angulation parameter, a magnification parameter, a source location parameter, a detector location parameter, and a distortion parameter, the adjusted parameters of the projection geometry being used in the second registering for the mathematical projection of the three-dimensional image.

6. The image registration process as set forth in claim 1, wherein the first registering comprises:

optimizing a distance figure-of-merit statistically characterizing distances between features of the two-dimensional set of features (36) and closest corresponding features of the two-dimensional set of projected features (44).

7. The image registration process as set forth in claim 1, wherein the projection geometry (42) is a projection geometry of a two-dimensional imager (10) during acquisition of the two-dimensional image (30).

8. The image registration process as set forth in claim 1, wherein the first registering applies a combinatoric algorithm to associate features of the two-dimensional set of features (36) with corresponding features of the two-dimensional set of projected features (44).

9. The image registration process as set forth in claim 1, further comprising:  
acquiring the two-dimensional image (30) using a two-dimensional imager (10) comprising an x-ray fluoroscopy apparatus; and

acquiring the three-dimensional image (32) using a three-dimensional imager (12) comprising a magnetic resonance imager (MRI) or a computed tomography (CT) imager.

10. The image registration process as set forth in claim 1, further comprising:  
acquiring a second three-dimensional image; and  
forming the two-dimensional image (30) by mathematically projecting the second three-dimensional image using the projection geometry (42).

008718US1

11. The image registration process as set forth in claim 1, further comprising:  
displaying a combination, fusion, or comparison of the two-dimensional image and a mathematical projection of the three-dimensional image after the second registering using the parameters derived from the first registering.

12. A digital storage medium or media storing instructions executable by a digital system to perform the method of claim 1.

13. An image registration apparatus including one or more processors programmed to perform the method of claim 1.

14. An image registration apparatus comprising:  
a features detector (34) configured to extract a two-dimensional set of features (36) from a two-dimensional image (30) and to extract a three-dimensional set of features (38) from a three-dimensional image (32);

a projection processor (40) configured to project three-dimensional data into two-dimensional projection data; and

a registration processor (46, 52) configured to

(i) adjust parameters to register the two-dimensional set of features and the three-dimensional set of features projected by the projection processor using a projection geometry (42), and to

(ii) use the adjusted parameters to register the two-dimensional image and the three-dimensional image projected by the projection processor using the projection geometry.

15. The image registration apparatus as set forth in claim 14, wherein the features detector (34) comprises a corner detector.

16. The image registration apparatus as set forth in claim 14, wherein the features detector (34) comprises an edge detector.

009120US1

17. The image registration apparatus as set forth in claim 14, wherein the registration processor (46, 52) is configured to adjust the projection geometry (42) to register or contribute to registering the two-dimensional set of features (36) and the three-dimensional set of features (38) projected by projection processor (40).

18. The image registration apparatus as set forth in claim 14, wherein the registration processor (46, 52) is configured to adjust spatial parameters of at least one of the two-dimensional set of features (36) and the three-dimensional set of features (38) projected by projection processor (40) to register or contribute to registering the two-dimensional set of features and the three-dimensional set of features projected by the projection processor.

19. The image registration apparatus as set forth in claim 14, wherein the projection geometry (42) is a predetermined projection geometry of a projection imager (10) used to acquire the two-dimensional image (30).

20. An apparatus comprising:

a two-dimensional imager (10) configured to acquire a two-dimensional image (30);

a three-dimensional imager (12) configured to acquire a three-dimensional image (32);

a features detector (34) configured to extract a two-dimensional set of features (36) from the two-dimensional image and to extract a three-dimensional set of features (38) from the three-dimensional image;

a projection processor (40) configured to project three-dimensional data into two-dimensional projection data; and

a registration processor (46, 52) configured to register the two-dimensional image and the three-dimensional image projected by the projection processor using parameters adjusted to register the two-dimensional set of features and the three-dimensional set of features projected by the projection processor.

21. The apparatus as set forth in claim 20, wherein the registration processor (46, 52) adjusts one or more parameters selected from a group consisting of (i) projection

009120US1

geometry parameters, (ii) two-dimensional translation parameters, and (iii) two-dimensional rotation parameters to register the two-dimensional set of features **(36)** and the three-dimensional set of features **(38)** projected by the projection processor **(40)**.

**22.** The apparatus as set forth in claim **20**, wherein the two-dimensional imager **(10)** comprises an x-ray fluoroscopy apparatus.

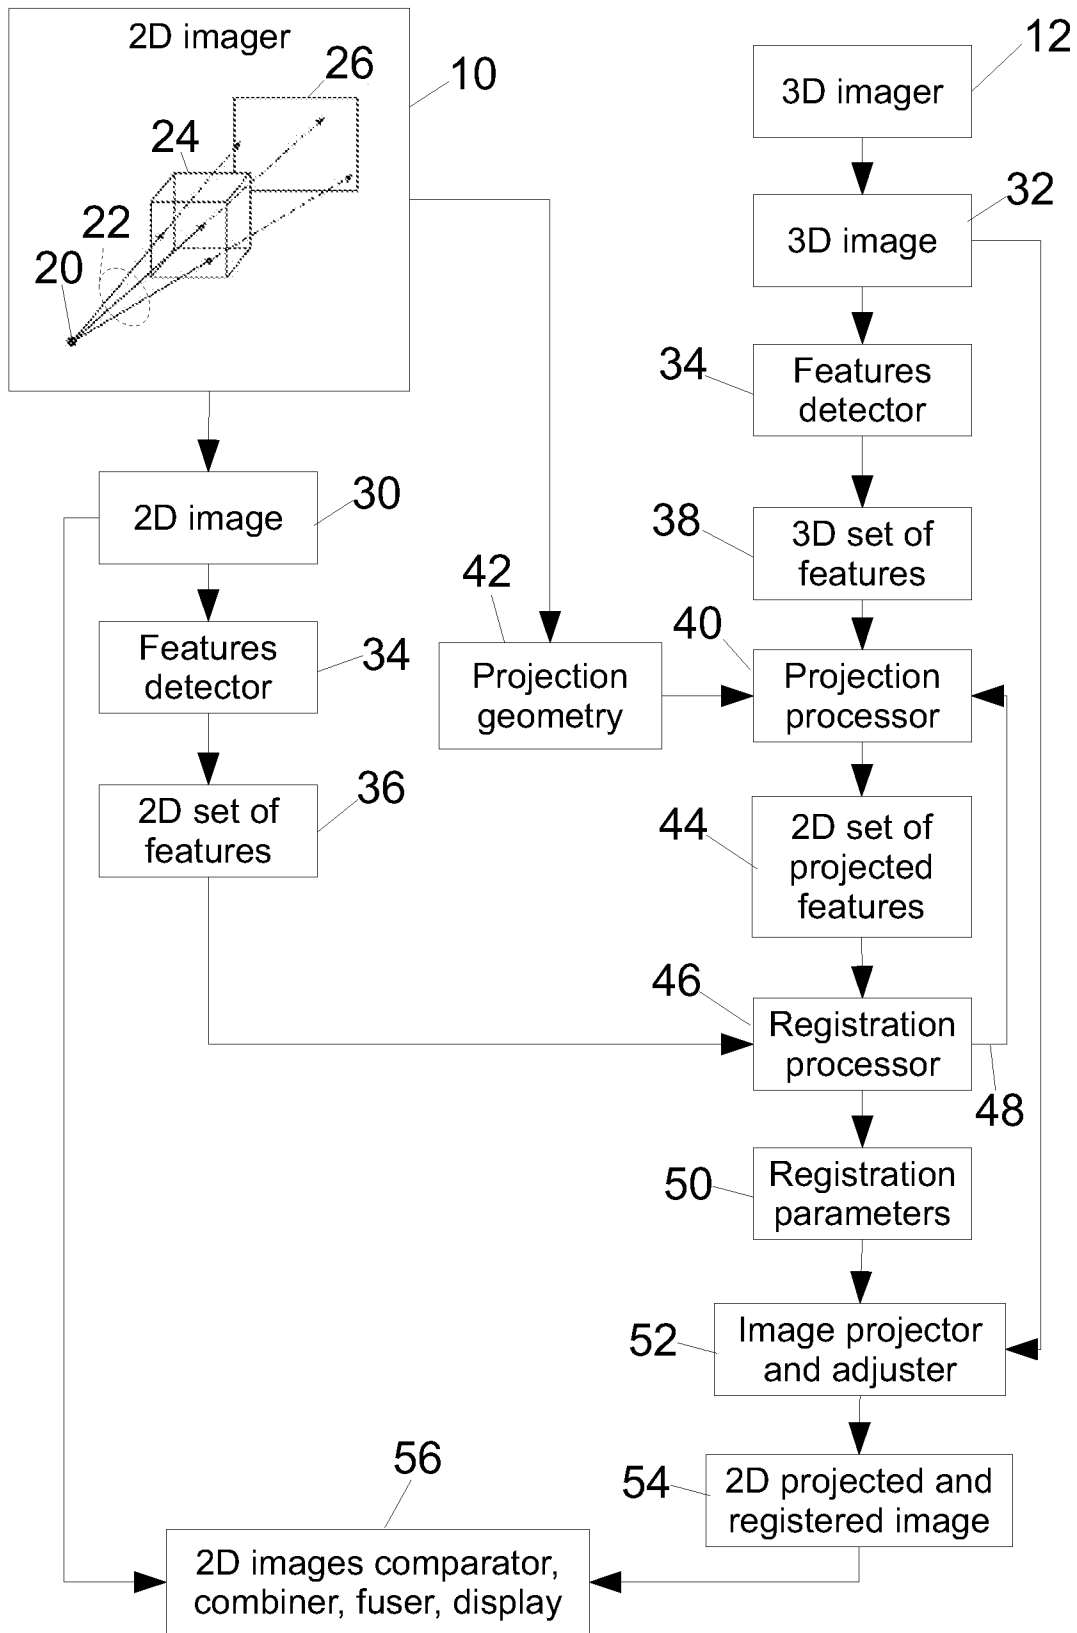


Fig. 1

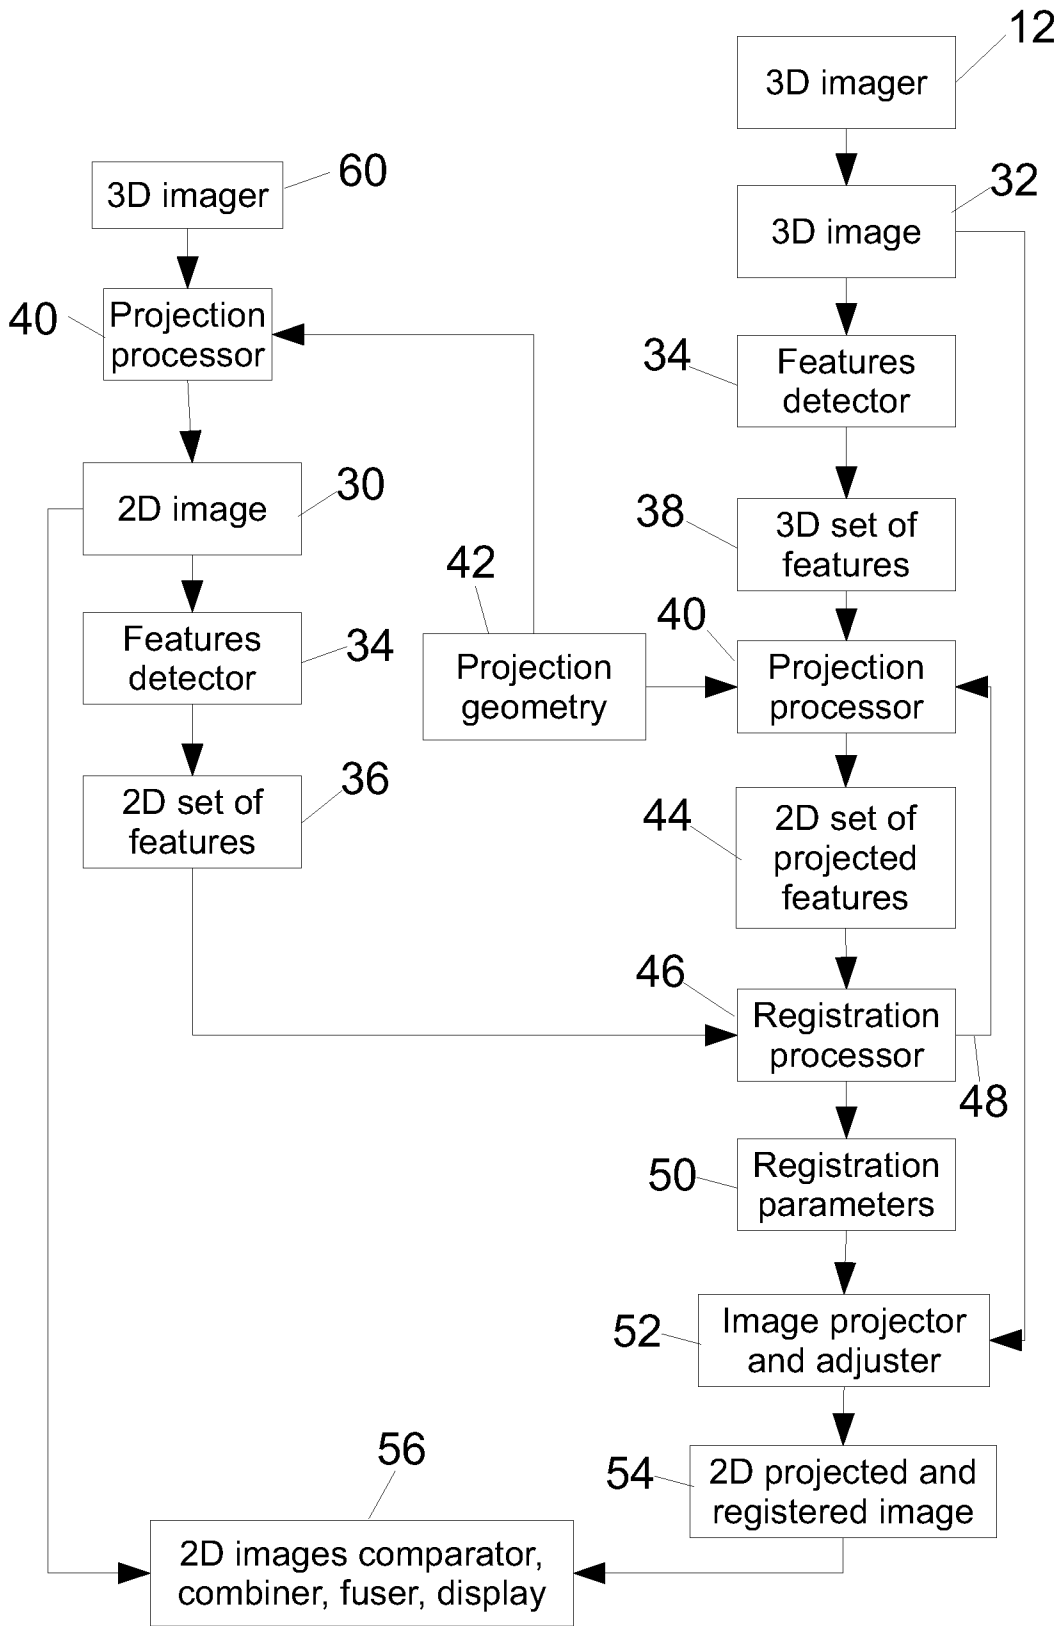


Fig. 2