

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. AU 2016312681 B2

(54) Title
Wearable devices

(51) International Patent Classification(s)
A61B 5/00 (2006.01) **A61B 5/04** (2006.01)
A61B 5/0205 (2006.01) **A61B 5/0402** (2006.01)
A61B 5/024 (2006.01) **A61B 5/0408** (2006.01)

(21) Application No: **2016312681** (22) Date of Filing: **2016.08.26**

(87) WIPO No: **WO17/035502**

(30) Priority Data

(31) Number (32) Date (33) Country
62/210,369 **2015.08.26** **US**
62/210,873 **2015.08.27** **US**

(43) Publication Date: **2017.03.02**
(44) Accepted Journal Date: **2021.01.21**

(71) Applicant(s)
Element Science, Inc.

(72) Inventor(s)
Kumar, Uday N.;Bahney, Timothy;Dinger, Maarten;Afshar, Pedram;Dhuldhoya, Jay;Marangi, Riley;Hasser, Christopher J.;Malchano, Zachary J.;Garcia, Frank;Farino, Kevin M.

(74) Agent / Attorney
RnB IP Pty Ltd, PO Box 9530, Deakin, ACT, 2600, AU

(56) Related Art
US 20140364918 A1

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2017/035502 A1

(43) International Publication Date

2 March 2017 (02.03.2017)

WIPO | PCT

(51) International Patent Classification:

A61B 5/00 (2006.01) *A61B 5/04* (2006.01)
A61B 5/0205 (2006.01) *A61B 5/0402* (2006.01)
A61B 5/024 (2006.01) *A61B 5/0408* (2006.01)

San Francisco, CA 94103 (US). **MALCHANO, Zachary, J.**; 200 Kansas Street, Suite 210, San Francisco, CA 94103 (US). **GARCIA, Frank**; 200 Kansas Street, Suite 210, San Francisco, CA 94103 (US).

(21) International Application Number:

PCT/US2016/049085

(74) Agents: **BUCKINGHAM, David, K.** et al.; Shay Glenn LLP, 2755 Campus Drive, Suite 210, San Mateo, CA 94403 (US).

(22) International Filing Date:

26 August 2016 (26.08.2016)

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/210,369 26 August 2015 (26.08.2015) US
62/210,873 27 August 2015 (27.08.2015) US

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: WEARABLE DEVICES

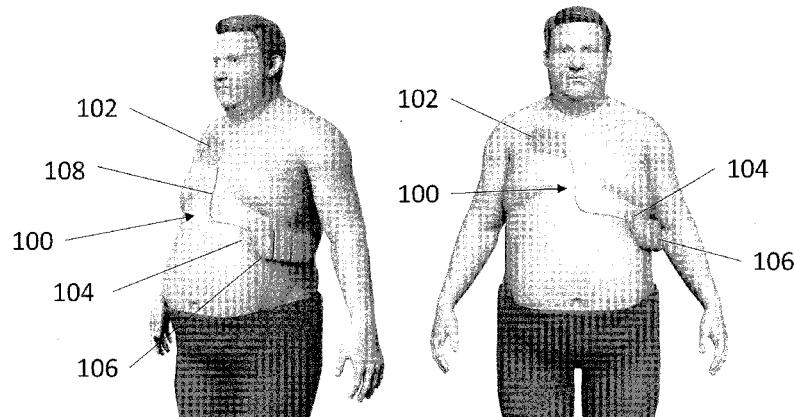


FIG. 1

(57) Abstract: Wearable devices are provided herein including wearable defibrillators, wearable devices for diagnosing symptoms associated with sleep apnea, and wearable devices for diagnosing symptoms associated with heart failure. The wearable external defibrillators can include a plurality of ECG sensing electrodes and a first defibrillator electrode pad and a second defibrillator electrode pad. The ECG sensing electrodes and the defibrillator electrode pads are configured for long term wear. Methods are also provided for using the wearable external defibrillators to analyze cardiac signals of the wearer and to provide an electrical shock if a treatable arrhythmia is detected. Methods are also disclosed for refurbishing wearable defibrillators. Methods of using wearable devices for diagnosing symptoms associated with sleep apnea and for diagnosing symptoms associated with heart failure are also provided.

WO 2017/035502 A1



Published:

— *with international search report (Art. 21(3))*

— *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

WEARABLE DEVICES**CROSS REFERENCE TO RELATED APPLICATIONS**

[0001] The present application claims priority under 35 U.S.C. 119 to U.S. provisional patent application serial number 62/210,369 filed on August 26, 2015 titled "Wearable Defibrillator" and U.S. Provisional Patent Application No. 62/210,873 filed on August 27, 2015 titled "Wearable Defibrillator", the disclosures of each of which are herein incorporated by reference in their entirety.

[0002] The present application is related to U.S. Provisional Patent Application No. 61/944,008 filed on February 24, 2014, and International Patent Application No. PCT/US2015/017366 filed on February 24, 2015, each titled "External Defibrillator," the disclosures of which are both incorporated by reference in their entirety.

INCORPORATION BY REFERENCE

[0003] All publications and patent applications mentioned in this specification are herein incorporated by reference in their entirety to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

FIELD

[0004] The present disclosure relates generally to wearable devices, such as external defibrillators. In particular, the disclosure relates to automatic external defibrillators that can be continuously and comfortably worn by a patient for an extended period of time.

BACKGROUND

[0005] Every year in the US, over 800,000 individuals have a heart attack, or myocardial infarction (MI). After an MI, a patient is at increased risk for experiencing potentially life-threatening abnormal heart rhythms, or arrhythmias. This increased risk is caused by numerous structural and electrical abnormalities in the recently damaged heart. For most patients, however, this increased risk is temporary. After patients have been treated with various procedures and medications to help their heart heal, their risk of experiencing a life-threatening arrhythmia usually drops back to their risk prior to the MI. This drop in risk typically occurs after a few days to weeks after the MI has taken place.

[0006] In addition to the post-MI setting, there are other situations in which a patient's arrhythmia risk is temporarily increased, such as after certain types of heart surgery or when starting certain medications with pro-arrhythmic properties. In patients who are known to be at risk for an arrhythmia and who have an ICD or S-ICD in place, if the ICD/S-ICD needs to be removed for a short period of time due to an infection or malfunction, the patient is also left vulnerable. In other patients, such as those with a condition known as heart failure (new diagnosis or acute exacerbation) or cardiomyopathy, certain medications and/or procedures can lead to an improvement in the heart's function and reduce a patient's

susceptibility to an arrhythmia such that a permanently implanted device, such as an ICD or S-ICD, would not be needed. However, during the time of treatment when heart function is recovering or when the patient is receiving treatment, these patients are still temporarily at risk for a life-threatening arrhythmia.

5 [0007] More than 750,000 patients are at risk for sudden cardiac death (SCD) in the U.S. each year. Based on event rates of up to 4% in the higher risk subgroups of the populations improved treatments could save up to 30,000 lives annually in the U.S. There are about 3.7 million worldwide incidence of SCD due to ventricular arrhythmias with a survival rate of less than 1%. Improved methods and devices are also needed to treat patients at risk for SCD. The devices and methods disclosed herein can be used
10 for patients with a temporarily increased risk for SCD or with a chronically increased risk for SCD. Clinical conditions in which a patient's temporary risk for experiencing a lethal arrhythmia or SCD is elevated include, but are not limited to: in patients after explantation of an ICD or S-ICD (due to infection or a mechanical failure, for instance), in patients with sleep apnea when it is severe, in patients who have certain arrhythmia syndromes, in pediatric patients with structural heart diseases, in certain patients with
15 significant valvular heart disease, in pregnant or recently pregnancy patients who develop pregnancy-related cardiomyopathy, and in patients with end-stage renal disease or on dialysis. Additional examples of conditions that can cause, increase the likelihood of SCD, or make a patient prone to SCD include: after cardiac surgery, new cardiomyopathy, after a heart attack, new heart failure, and heart failure exacerbation.

20 [0008] Various studies of this population of patients have shown that certain medications, especially those with anti-arrhythmic properties, do a poor job at reducing this temporarily increased arrhythmia risk. Implantable cardioverter defibrillators (ICDs) and subcutaneous ICD (S-ICDs), which can continuously monitor the patient for an arrhythmia and effectively reset the heart rhythm when an arrhythmia occurs, carry significant risks during implantation such that their overall benefit during this
25 short period of increased risk is limited. Implanting ICDs and S-ICDs in many patients whose risk of an arrhythmia would eventually return to normal also has significant unwanted health, economic, and societal consequences.

30 [0009] Automatic external defibrillators (AEDs) are stored on walls apart from patients in highly populated places such as airports and do not monitor patients for arrhythmias. They are only useful if an AED is present when the patient needs it and if other people capable of using the AED are present at the time an arrhythmia occurs, can identify that a patient needs defibrillation and is able to apply the sensing and defibrillation electrodes to the patient. Wearable external defibrillators and external cardioverter defibrillators are described in US 5,741,306; US 6,065,154; US 6,280,461; US 6,681,003 and US 2003/0095648. A similar product is currently being sold as the Zoll Lifecor LifeVest™ wearable
35 cardioverter defibrillator (WCD). Wearable cardioverter defibrillators are able to monitor a patient for arrhythmias while they are worn without the need for implantation surgery, and they can be removed when the need for such monitoring (and possible cardioversion or defibrillation shock) has passed.

[0010] One drawback of currently available wearable defibrillators (such as the LifeVest product) is lack of patient compliance. Because of the size, shape and weight of these wearable devices, patients are reluctant to wear them due to discomfort, their bulkiness under clothes or limitations in the devices themselves. In particular, such devices cannot be worn in the shower or bath, and they often are difficult, 5 if not impossible, to sleep in. The device therefore is not useful in providing treatment to the patient while sleeping or in the shower. Patients also complain that the LifeVest is too large and uncomfortable. Many patients also have increased anxiety over the many alarms and notifications from the LifeVest. The increased anxiety further increases instances of non-compliance. Given the bulkiness of these devices, some patients do not like using these wearable devices outside in public as it draws unnecessary attention 10 to them, which they might find uncomfortable or embarrassing. This may affect their well-being and may lead them to avoid performing their normal routine activities. All of these factors increase patient noncompliance and prevent the treatment of a treatable arrhythmia. In one study 60% of LifeVest wearers were not saved due to patient non-compliance (Tanawuttiwat T, et al. *PACE* Online 12.3.2013). The device can also be easily taken off, which prevents the vest from providing treatment to the patient 15 when it is not being worn.

[0011] Another drawback is that it is possible to incorrectly wear a wearable vest like the LifeVest, such that the vest will not properly detect a patient arrhythmia. Incorrectly wearing the vest can also prevent the vest from delivering a defibrillating shock to the patient. The design of the vest can also result in increased false positives of arrhythmias measured by the vest. The vest also has a complicated 20 electrode design. Because the vest is put and taken off multiple times a day, no gel is applied between the defibrillation electrodes and the patient's skin unless and until a shock is required. The gel releasing mechanism can fail or may not work when the vest is worn incorrectly.

[0012] What is needed, therefore, is a non-invasive, temporary device that can continuously monitor the patient's heart rhythm to detect arrhythmias; can record and store all detected rhythms for future 25 evaluation if necessary; can automatically and reliably defibrillate the heart if an arrhythmia is detected; can be used for a short period of time (days to weeks, possibly months) when the temporary risk of an arrhythmia exists; is entirely non-invasive and reversible and causes no significant or potentially permanent bodily harm from its use; and/or, most importantly, is unobtrusive and water resistant and requires only minimal maintenance or care so that it can seamlessly integrate into patients' lives such that 30 they are protected from life-threatening arrhythmias during this entire period of time and can perform their normal daily routines without impediments to their physical or mental well-being. If the device is required to defibrillate a patient during this time, this patient can then be referred for evaluation to determine whether they need a permanent ICD or S-ICD, if appropriate. If nothing occurs and the patient doesn't have persistent pro-arrhythmic risk factors after this temporary period, the device can be removed 35 and the implantation of a permanent device can be avoided. In this way, a functional, easy-to-use device for cardiac defibrillation to protect patients during a period of temporarily increased arrhythmia risk could also more efficiently identify patients who would benefit from more permanently implanted devices and those who would not.

[0013] A need also exists for treating temporary periods of elevated risk for sudden cardiac death in a successful and cost-effective manner while delivering an outstanding patient experience. A need also exists for improved treatment for patients with a need for an ICD but not getting one today, patients not initially indicated for ICD but found to be at elevated risk for SCD, and patients that would die of SCD without wearable defibrillator.

[0014] U.S. Patent Nos. 8,024,037 and 8,364,260 disclose wearable external defibrillators.

Wearable external defibrillators are desired that have improved adhesives for long term-wear, improved electrodes for long-term wear, improved weight distribution of the electrical components, improved and reduced size, and improved comfort to increase patient compliance.

[0015] The Zio® Patch by iRhythm® is designed to record heartbeats for up to 14 days. The Zio Patch has a relatively small profile and is lightweight because it does not have to accommodate the electrodes for delivering a defibrillating shock or support the electronic components required to deliver a defibrillating shock.

[0016] There are many challenges in developing biocompatible adhesives and electrodes for long-term wear. It is difficult to design adhesives that can be worn for longer than 10 days. Skin sloughing also occurs naturally over time, typically on the order of about 10-30 days, with variation related to the age of the patient. The natural sloughing of skin cells also presents technical challenges that need to be solved by the design of the adhesive material and design of the electrodes. Adhesives and electrodes also typically will cause skin irritation and redness during long term wear. It is desirable to also develop an improved adhesive and electrode design that can be used to comfortably attach the wearable defibrillator to the patient for long term wear. Developing a device that also is small enough to allow a weight distribution while adhered to the patients such that the device can be used constantly for long term wear is a challenging task. Additionally, developing a device small enough to be concealed such that its use in public does not draw attention or can be easily hidden under normal clothing is desired.

25

SUMMARY OF THE DISCLOSURE

[0017] The present invention relates generally to improved wearable devices and methods for using such wearable devices. Examples of wearable devices include wearable defibrillators, wearable devices for diagnosing symptoms associated with sleep apnea, and wearable devices for diagnosing symptoms associated with heart failure. The wearable devices disclosed herein can be comfortably worn by the patient around the clock. The wearable devices, including the wearable defibrillators, can be worn during showering, sleeping, and normal activities. The adhesives and electrodes are designed for long term wear. In the wearable defibrillators the electrodes are designed to be worn such that the electrodes are in continuous electrical communication with the skin and are ready to deliver an effective amount of energy for defibrillation.

[0018] In general, in one embodiment, a wearable external defibrillator including one or more sensing electrodes configured to engage with a patient's skin to detect a cardiac signal; a first defibrillator electrode pad configured to engage with the patient's skin and to deliver an electrical therapy to the

patient, the first defibrillator electrode pad configured to be in continuous contact with the patient's skin; a first patient engagement substrate including an adhesive, the first defibrillator electrode pad, a first fluid transport element configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a first vapor permeable layer; a second patient engagement substrate including a second defibrillator electrode pad, a second adhesive, a second fluid transport element in fluid communication with the second patient engagement substrate configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a second vapor permeable layer; an energy source; one or more capacitors in electrical communication with the energy source and the first defibrillator electrode pad and the second defibrillator electrode pad; and a controller configured to detect the cardiac signal with the one or more sensing electrodes and the sensing electrode of the second patient engagement substrate and to charge the one or more capacitors with the energy source followed by discharging the one or more capacitors to deliver a therapeutic shock through the first defibrillator electrode pad and the second defibrillator electrode pad to the patient while the first and second patient engagement substrates are engaged with the patient, wherein the energy source, one or more capacitors, and controller are enclosed within one or more housings.

[0019] This and other embodiments can include one or more of the following features. The first patient engagement substrate can include the one or more sensing electrodes. The first patient engagement substrate can include two or more sensing electrodes. The second patient engagement substrate can include a sensing electrode. The first defibrillator electrode pad and second defibrillator electrode pad can be adapted to detect the cardiac signal. The one or more housings can include a first controller housing, the controller can be included in the first controller housing. The one or more housings can include a first energy source housing, the energy source can be included in the first energy source housing. The one or more housings can include a first capacitor housing and a second capacitor housing, the capacitors can be included in the first capacitor housing and the second capacitor housing. The first controller housing can include a first controller housing electrical connection, the first energy source housing can include a first energy source housing electrical connection, the first capacitor housing can include a first capacitor electrical connection, and the second capacitor housing can include a second electrical connection. The wearable defibrillator can further include a mechanical connection between each of the first controller housing, first energy source housing, first capacitor housing, and second capacitor housing. The wearable defibrillator can further include a flexible circuitry and one or more rigid printed circuit boards (PCBs). The flexible circuitry can be adapted to receive the first controller housing electrical connection, the first energy source housing electrical connection, the first capacitor electrical connection, and the second electrical connection. The flexible circuitry can be in electrical communication with the first controller housing, first energy source housing, first capacitor housing, and second capacitor housing.

[0020] The flexible circuitry can provide electrical communication between the first controller housing and the first energy source housing, first capacitor housing, and second capacitor housing. The flexible circuitry can be supported by the first patient engagement substrate between the first vapor permeable layer and the first defibrillator electrode pad. The first patient engagement substrate can be

adapted to support the one or more housings. The second patient engagement substrate can be adapted to support the one or more housings. The first patient engagement substrate and second patient engagement substrate can be configured to be worn during showering activities. The first patient engagement substrate can include an exterior surface and the second patient engagement substrate can include an exterior surface. A portion of the first vapor permeable layer can represent an exterior surface of the first patient engagement surface. A portion of the second vapor permeable layer can represent an exterior surface of the second patient engagement surface. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can be moisture vapor permeable. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 1000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 2000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 5000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 8000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can be air permeable. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can be waterproof. The exterior surfaces of the first and second patient engagement substrates can be hydrophobic. The first fluid transport element and second fluid transport element can be configured to transport fluid away from the skin. The wearable defibrillator can further include a support chassis disposed between the one or more housings and the first defibrillator electrode pad. The support chassis can be adapted to spread a shear load of the one or more housings across a dominant surface of the support chassis. The wearable defibrillator can further include a pulse oximeter configured to measure an oxygen content of a blood of the patient at a point on a chest of the patient. The wearable defibrillator can further include an ultrasound transceiver or transducer configured to transmit and/or receive ultrasonic signals. The wearable defibrillator can further include a Doppler radar configured to transmit a microwave signal and receive a returned microwave signal. The first defibrillator electrode pad can include a first pair of electrodes. The controller can be configured to measure a first impedance between the first pair of electrodes. The controller can be configured to analyze the first impedance to determine whether the first pair of electrodes are in proper contact with the patient's skin. The second defibrillator electrode pad can include a second pair of electrodes. The controller can be configured to measure a second impedance between the second pair of electrodes. The controller can be configured to analyze the second impedance to determine whether the second pair of electrodes are in proper contact with the patient's skin. The controller can be configured to measure a transthoracic impedance between the first pair of electrodes and the second pair of electrodes. The wearable defibrillator can further include a slip layer disposed between the housing and adhesive configured to allow relative movement between the

housing and the adhesive. The wearable defibrillator can further include a first sealing layer enclosing the energy source, one or more capacitors, and controller. The first sealing layer can be within the housing. The first sealing layer can contact the housing. The wearable defibrillator can further include a second sealing layer containing the housing. The wearable defibrillator can further include a connector plug on the housing with a plurality of electrical connections. The plurality of electrical connections can include a first defibrillator electrode pad connection and a second defibrillator electrode pad connection. The first defibrillator electrode pad connection and the second defibrillator electrode pad connection can be configured to be in electrical communication with the one or more capacitors and the first and second defibrillator electrode pads. The plurality of electrical connections can include a plurality of sensing electrode connections. The plurality of sensing electrode connections can be each configured to be in electrical communication with the controller and one of the one or more sensing electrodes. The wearable defibrillator can further include an enclosure configured to surround the housing, the enclosure can include an enclosure connection and can have a first side with a complementary structure configured to engage with the connector plug on the housing. The wearable defibrillator can further include a second side of the enclosure connection configured to engage with a patient engagement substrate connector on the first patient engagement substrate, the patient engagement substrate connector in electrical communication with the one or more capacitors and the first and second defibrillator electrode pads. The adhesive can include a plurality of pores configured to allow the transport of moisture vapor. The one or more sensing electrodes and defibrillator electrode pads can include a plurality of pores configured to allow the transport of moisture vapor. The first defibrillator electrode pad the second defibrillator electrode pad can include a polyethylene terephthalate (PET) substrate with a conductive ink coating. The first defibrillator electrode pad can include a first conductive adhesive and a first conductive electrode. The second defibrillator electrode pad can include a second conductive adhesive and a second conductive electrode. The first and second conductive electrodes can have a solid construction. The first and second conductive electrodes can be made from a flexible sheet having a plurality of perforations. The first and second conductive electrodes can include a carbon vinyl film, Ag/AgCl coated carbon vinyl film, or Ag coated carbon vinyl film. The first and second conductive electrodes of the first and second defibrillator electrode pads can have a woven structure. The first and second conductive electrodes of the first and second defibrillator electrode pads can include carbon fiber. The first conductive adhesive and the second conductive adhesive can include a conductive hydrogel. The conductive hydrogel can include a salt. The first conductive adhesive and the second conductive adhesive can include an adhesive with a conductive filler. The conductive filler can include one or more of: carbon nanotubes, graphene, carbon black, silver particles, metal particles, and silver nanowires. The first patient engagement substrate can be configured to insulate between the one or more sensing electrodes and the first defibrillator electrode pad. The second patient engagement substrate can be configured to insulate between the sensing electrode and the second defibrillator electrode pad. The adhesive on the first and second patient engagement substrates can be non-conductive. The wearable defibrillator can further include an inclinometer configured to determine the position and orientation of the wearable defibrillator. The wearable defibrillator can further include a

radio beacon configured to transmit the location of the wearable defibrillator. The wearable defibrillator can further include a GPS sensor. The wearable defibrillator can further include a wireless radio configured to wirelessly transmit data from the wearable defibrillator. The wireless radio can be configured to transmit data over a cellular network. The wearable defibrillator can further include a sensor configured to measure a mechanical stretch of a portion of the wearable defibrillator. The one or more capacitors can be configured to be reversibly and removably engaged with the wearable defibrillator. The energy source can be configured to be reversibly and removably engaged with the wearable defibrillator. The controller can be configured to be reversibly and removably engaged with the wearable defibrillator. The wearable defibrillator can further include a first adhesive release liner configured to cover the adhesive on the first patient engagement substrate. The wearable defibrillator can further include a second adhesive release liner configured to cover the adhesive on the second patient engagement substrate. The housing can be configured to receive a plurality of energy sources. The energy source can include a first modular battery and a second modular battery, the first and second modular batteries can be configured to be removably received within the housing. The wearable defibrillator can further include an external pacing module configured to provide a pacing signal to the patient, the external pacing module can be supported by the first or second patient engagement substrate. The wearable defibrillator can further include a skin contact module configured to sense removal of the first and/or second patient engagement substrate from the patient's skin. The skin contact module can be configured to generate an alarm and/or notification to a healthcare provider upon sensing removal of the first and/or second patient engagement substrate from the patient's skin. The wearable defibrillator can further include a cantilever coupled to the housing and the first patient engagement substrate. The housing can include a plurality of compartments containing the energy source, one or more capacitors, and controller. The wearable defibrillator can further include a flexible circuitry and one or more rigid printed circuit boards (PCBs) within the housing. The plurality of compartments can be in fluid communication within the housing. The plurality of compartments may not be in fluid communication with the other of the plurality of compartments. The plurality of compartments can be separate and configured to reversibly engage with the other of the plurality of compartments. The plurality of compartments can be connected with a plurality of waterproof connector segments. The housing can be configured to allow relative movement between the plurality of compartments of the housing. The relative movement can include flexing with a plane of the first patient engagement substrate. The housing can include an outer clam shell and a base. The outer clam shell can be ultrasonically welded to the base. The outer clam shell can be attached to the base with an adhesive. The outer clam shell can be attached to the base through chemical bonding. The one or more sensing electrodes of the first patient engagement substrate and the sensing electrode of the second patient engagement substrate and the first and second defibrillator electrode pads can be configured to sense impedance changes along a plurality of vectors of the patient, the controller can be configured to analyze the impedance changes along the plurality of vectors of the patient to measure a cardiac health of the patient. The first patient engagement substrates can include a patient engagement portion including the one or more sensing electrodes, the adhesive, and first defibrillator

electrode pad. The first patient engagement substrate can include a moisture vapor transport above about 100 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 500 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 1000 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 1500 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first vapor permeable layer. The second patient engagement substrate can include a second patient engagement portion including the sensing electrode, the second adhesive, and second defibrillator electrode pad. The first patient engagement substrate can include a moisture vapor transport above about 100 g/m² per day based on a surface area of the patient engagement portion through the second patient engagement portion and the second vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 500 g/m² per day based on a surface area of the patient engagement portion through the second patient engagement portion and the second vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 1000 g/m² per day based on a surface area of the patient engagement portion through the second patient engagement portion and the second vapor permeable layer. The first patient engagement substrate can include a moisture vapor transport above about 1500 g/m² per day based on a surface area of the patient engagement portion through the second patient engagement portion and the second vapor permeable layer. The first patient engagement substrate can have a preformed curvature. The preformed curvature can correspond to a shape of a human torso. The second patient engagement substrate can have a preformed curvature. The preformed curvature can correspond to a shape of a human chest. The wearable defibrillator can further include a cable forming an electrical communication between the first patient engagement substrate and the second patient engagement substrate. The cable can form the electrical communication between the sensing electrode of the second patient engagement substrate and the controller. The cable can form the electrical communication between the second defibrillator electrode pad and the one or more capacitors. The wearable defibrillator can further include a display indicator. The display indicator can be part of the first patient engagement substrate or second patient engagement substrate. The display indicator can be part of the one or more housings. The display indicator can be part of a cable between the first patient engagement substrate or second patient engagement substrate. The display indicator can be a light emitting diode (LED). The wearable defibrillator can further include a tactile feedback module. The tactile feedback module can be part of the first patient engagement substrate or second patient engagement substrate. The tactile feedback module can be part of the one or more housings. The tactile feedback module can be a vibration motor. The wearable defibrillator can further include one or more buttons on the one or more housings. The wearable defibrillator can further include a first connection between the housing and the first patient engagement

substrate and a second flexible connection between the housing and the first patient engagement substrate, the first connection can be on a first end of the first patient engagement substrate and the second flexible connection can be on a second end of the first patient engagement substrate that opposes the first end of the first patient engagement substrate. The second flexible connection can allow for relative movement

5 between the second end of the first patient engagement substrate and the housing. The wearable defibrillator can further include a first sensing electrode release liner configured to cover the one or more sensing electrodes on the first patient engagement substrate and a first defibrillator electrode pad release liner configured to cover the first defibrillator electrode pad. The wearable defibrillator can further include a second sensing electrode release liner configured to cover the one or more sensing electrodes on

10 the second patient engagement substrate and a second defibrillator electrode pad release liner configured to cover the second defibrillator electrode pad. The housing can be supported by two or more patient engagement substrates. The wearable defibrillator can further include an electroactive polymer. The electroactive polymer can be configured to detect a change in a morphology of the first patient engagement substrate and/or second patient engagement substrate. The electroactive polymer can be

15 configured to vibrate. The electroactive polymer can be configured to deform to change the morphology of the first and/or second patient engagement substrate. The wearable defibrillator can further include a flexible connection between the housing and the first patient engagement substrate configured to support the weight of the housing and components within the housing. The flexible connection can allow for relative movement between the housing and the first patient engagement substrate. The flexible

20 connection can further include one or more electrical connections between the housing and the first patient engagement substrate. The flexible connection can include a removable and reversible connection. The one or more housings each can have a clam shell configuration sealed with an adhesive. The one or more housings each can have a clam shell configuration sealed with ultrasonic welding. The one or more housings each can have a clam shell configuration sealed through chemical bonding. The controller can

25 be configured to analyze an impedance between one or more of: the one or more sensing electrodes, the first defibrillator electrode pad, the second defibrillator electrode pad, and the sensing electrode. The controller can further be configured to measure the impedance using two or more discrete frequencies. The two or more discrete frequencies can include a high frequency measurement and a low frequency measurement. The controller can further be configured to analyze the high frequency measurement and

30 low frequency measurement to determine a power of the therapeutic shock for the patient based on the impedance. The wearable defibrillator can further include a temperature sensor.

[0021] In general, in one embodiment, a method of monitoring and defibrillating a patient's heart, including adhering to a first skin surface portion of the patient a first patient engagement substrate including a first plurality of sensing electrodes and a first defibrillator electrode pad, the first defibrillator electrode pad in electrical communication with an electrical energy source sufficient to provide a defibrillating shock, the first patient engagement substrate part of a wearable defibrillator including a fluid transport element configured to transport fluid away from the first skin surface portion of the patient to allow the wearable external defibrillator to be worn continuously; adhering to a second skin surface

portion of the patient a second patient engagement substrate including a sensing electrode and a second defibrillator electrode pad, the second defibrillator electrode pad in electrical communication with the electrical energy source sufficient to provide the defibrillating shock, the second patient engagement substrate part of the wearable defibrillator, the wearable defibrillator including one or more sensors adapted to detect one or more of the pulse, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient; measuring patient data corresponding to a cardiac signal or other characteristic of the patient with the first plurality of sensing electrodes, the sensing electrode of the second patient engagement substrate, and/or the sensors of the wearable defibrillator; and analyzing the patient data to determine if the patient has an arrhythmia.

5 [0022] This and other embodiments can include one or more of the following features. The method can further include upon detection of an arrhythmia detecting one or more of the pulse, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient using one or more sensors on the wearable defibrillator; and analyzing the detected one or more of the pulse, oxygen content of the blood, breathing rate, heart sounds, and heart rate of the patient

10 to confirm the presence or absence of the arrhythmia. The method can further include sensing impedance changes along a plurality of vectors of the patient with the one or more sensing electrodes of the first patient engagement substrate and the sensing electrode of the second patient engagement substrate and the first and second defibrillator electrode pads. The method can further include comparing the impedance changes to a patient baseline and/or a database to measure a cardiac health of the patient. The method can

15 further include measuring electrical data corresponding to a cardiac signal of the patient with the first plurality of sensing electrodes and the sensing electrode of the second patient engagement substrate. The method can further include detecting one or more of the breathing rate, heart sounds, and heart rate of the patient with a microphone on the wearable defibrillator. The method can further include recording patient movement with an accelerometer integrated with the wearable defibrillator upon detection of an

20 arrhythmia; and analyzing the recorded patient movement to confirm the presence or absence of the arrhythmia. The method can further include detecting the oxygen content of the blood with a pulse oximeter on the wearable defibrillator. Detecting the oxygen content of the blood with a pulse oximeter on the wearable defibrillator can include measuring the oxygen content of the blood of the patient at a point on a chest of the patient. The method can further include measuring a transthoracic impedance

25 between the first defibrillator electrode pad and the second defibrillator electrode pad. The first defibrillator electrode pad can include two separate electrodes, can further include measuring an impedance between the two separate electrodes of the first defibrillator electrode pad. The method can further include analyzing the impedance between the two separate electrodes of the first defibrillator electrode pad to determine whether the two separate electrodes of the first defibrillator electrode pad are

30 in sufficient electrical contact with the skin to deliver an electrical shock. The second defibrillator electrode pad can include two separate electrodes, can further include measuring an impedance between the two separate electrodes of the second defibrillator electrode pad. The method can further include analyzing the impedance between the two separate electrodes of the second defibrillator electrode pad to

35

determine whether the two separate electrodes of the second defibrillator electrode pad are in sufficient electrical contact with the skin to deliver an electrical shock. The method can further include delivering an electrical shock after determining that the patient has an arrhythmia. The method can further include analyzing the measured electrical data corresponding to the cardiac signal of the patient for bradycardia, 5 atrial fibrillation, asystole, heart blocks, pauses, ventricular tachycardia, ventricular fibrillation, tachycardia with aberrancy, or a supraventricular tachycardia (SVT). The method can further include continuously wearing the wearable defibrillator for greater than about 24 hours. The method can further include continuously wearing the wearable defibrillator for greater than about 5 days. The method can further include continuously wearing the wearable defibrillator for greater than about 7 days. The method 10 can further include continuously wearing the wearable defibrillator for greater than about 10 days. The method can further include continuously wearing the wearable defibrillator for greater than about 14 days.

[0023] In general, in one embodiment, a method for refurbishing a wearable defibrillator including receiving a wearable defibrillator including an energy source, a controller, and a memory containing a patient data set collected while the wearable defibrillator was worn by a patient; copying the patient data 15 set from the memory to a computer network or system external to the wearable defibrillator; erasing the patient data set from the memory of the wearable defibrillator; recharging or replacing the energy source of the wearable defibrillator; and running a diagnostic test on the wearable defibrillator after erasing the patient data set and recharging or replacing the energy source.

[0024] This and other embodiments can include one or more of the following features. The wearable 20 defibrillator can be any of the wearable defibrillators described herein. The wearable defibrillator can further include one or more sensing electrodes configured to engage with a patient's skin to detect a cardiac signal; a defibrillator electrode pad configured to engage with the patient's skin and to deliver an electrical therapy to the patient; a patient engagement substrate including an adhesive, the one or more sensing electrodes, and the defibrillator electrode pad; and one or more capacitors in electrical 25 communication with the energy source and the defibrillator electrode pad, wherein the controller is configured to detect the cardiac signal with the sensing electrodes and to charge the one or more capacitors with the energy source followed by discharging the one or more capacitors to deliver a therapeutic shock through the defibrillator electrode pad to the patient while the patient engagement substrate is engaged with the patient. The wearable defibrillator can include one or more modules 30 containing the one or more capacitors, energy source, and controller. The wearable defibrillator can include a module containing the energy source, and replacing the energy source includes replacing the module containing the energy source. The diagnostic test can include testing the one or more capacitors, memory, energy source, and controller. The wearable defibrillator can further include one or more housings containing one or more of the controller, memory, capacitors, and energy source. The controller 35 and memory can be included in a first controller housing, the energy source can be included in a first energy source housing, and the capacitors can be included in a first capacitor housing and a second capacitor housing. The method can further include removing the controller and memory from the first controller housing. The method can further include removing the energy source from the first energy

source housing. The method can further include removing the one or more capacitors from the first capacitor housing and the second capacitor housing. The diagnostic test can include testing the one or more capacitors, memory, energy source, and controller after removal from the one or more housings. The method can further include engaging a data transfer cable with a connector in electrical communication with the memory. The method can further include after running the diagnostic test, placing the controller and memory in a second controller housing. The method can further include after running the diagnostic test, placing the one or more capacitors in a new first capacitor housing and a new second capacitor housing. The method can further include after running the diagnostic test, placing the energy source in a second energy source housing. The method can further include engaging the second controller housing, new first capacitor housing, new second capacitor housing, and second energy source housing with a patient engagement substrate to form a refurbished wearable defibrillator. The method can further include sealing the one or more housings to prevent water ingress. The wearable defibrillator can be configured to support the one or more housings within a waterproof enclosure. The method can further include removing the housing from the waterproof enclosure after receiving the wearable defibrillator.

5 The method can further include engaging a data transfer cable with an exterior connection of the one or more housings. Copying can include a wireless data transfer between the memory and the computer network or system. Copying can include a wired data connection to transfer the patient data set between the memory and the computer network or system. The method can further include after running the diagnostic test, placing the housing within a second waterproof enclosure. The method can further include

10 engaging the housing with the second waterproof enclosure with a patient engagement substrate to form a refurbished wearable defibrillator. The refurbished wearable defibrillator can include one or more sensing electrodes configured to engage with a patient's skin to detect a cardiac signal; a defibrillator electrode pad configured to engage with the patient's skin and to deliver an electrical therapy to the patient; the patient engagement substrate including an adhesive, the one or more sensing electrodes, and the

15 defibrillator electrode pad; and one or more capacitors in electrical communication with the energy source and the defibrillator electrode pad, wherein the controller is configured to detect the cardiac signal with the sensing electrodes and to charge the one or more capacitors with the energy source followed by discharging the one or more capacitors to deliver a therapeutic shock through the defibrillator electrode pad to the patient while the patient engagement substrate is engaged with the patient, wherein the one or

20 more capacitors, energy source, and controller are enclosed within one or more housings. The method can further include forming one or more electrical connections between the one or more housings and the one or more sensing electrodes and defibrillator electrode pads of the refurbished wearable defibrillator. The method can further include packaging the refurbished wearable defibrillator. The method can further include

25 sending the refurbished wearable defibrillator to a second patient. The method can further include receiving the refurbished wearable defibrillator containing a second patient data set collected while the refurbished wearable defibrillator was worn by the second patient. The method can further include

30 copying the second patient data sent from the memory to a computer network or system external to the refurbished wearable defibrillator; and erasing the patient data set from the memory of the refurbished

35

wearable defibrillator. The method can further include replacing or refurbishing the one or more housings in the refurbished wearable defibrillator. The method can further include replacing or refurbishing the one or more housings and reusing the one or more capacitors five or more times. The method can further include replacing or refurbishing the one or more housings and reusing the one or more capacitors ten or 5 more times. The method can further include replacing or refurbishing the one or more housings and reusing the one or more capacitors fifteen or more times. The method can further include replacing or refurbishing the one or more housings and reusing the one or more capacitors twenty or more times. The energy source can include a rechargeable battery. The method can further include recharging the rechargeable battery. The energy source can include a battery. The method can further include replacing 10 the battery. The patient data set can include data from the patient continuously wearing the wearable defibrillator for greater than about 24 hours. The patient data set can include data from the patient continuously wearing the wearable defibrillator for greater than about 5 days. The patient data set can include data from the patient continuously wearing the wearable defibrillator for greater than about 7 days. The patient data set can include data from the patient continuously wearing the wearable 15 defibrillator for greater than about 10 days. The patient data set can include data from the patient continuously wearing the wearable defibrillator for greater than about 14 days.

[0025] In general, in one embodiment, a method for providing instructions for placing a wearable defibrillator on a patient, the method including providing instructions on where to put a first patient engagement substrate of the wearable defibrillator on a torso of the patient, the first patient engagement 20 substrate including one or more sensing electrodes, adhesive, and a first defibrillator electrode pad, the instructions including where to put the one or more sensing electrodes and first defibrillator electrode pad on the chest of the patient; providing instructions on where to put a second patient engagement substrate of the wearable defibrillator, the second patient engagement substrate including a sensing electrode, adhesive, and a second defibrillator electrode pad, the instructions including where to put the one or more 25 sensing electrodes and second defibrillator electrode pad; verifying a first patient engagement substrate placement on the torso of the patient including the placement of the one or more sensing electrodes and first defibrillator electrode pad; and verifying a second patient engagement substrate placement on the chest of the patient including the sensing electrode and second defibrillator electrode pad.

[0026] This and other embodiments can include one or more of the following features. The 30 instructions can be provided to the patient. The person applying the wearable defibrillator can be the patient. The instructions can be provided to a person applying the wearable defibrillator to the patient. The person applying the wearable defibrillator can be a health care provider. The wearable defibrillator can further include a first sensing electrode release liner configured to cover the one or more sensing electrodes on the patient engagement substrate, a first defibrillator electrode pad release liner configured 35 to cover the first defibrillator electrode pad, and a first adhesive release liner configured to cover the adhesive on the first patient engagement substrate; and a second sensing electrode release liner configured to cover the one or more sensing electrodes on the second patient engagement substrate and a second defibrillator electrode pad release liner configured to cover the second defibrillator electrode pad, and a

second adhesive release liner configured to cover the adhesive on the second patient engagement substrate. The method can further include providing instructions to sequentially remove the first sensing electrode release liner, the first defibrillator electrode pad release liner, and the first adhesive release liner. The method can further include providing instructions to sequentially remove the second sensing electrode release liner, the second defibrillator electrode pad release liner, and the second adhesive release liner. The wearable defibrillator can further include a primary patient engagement substrate release liner configured to cover a first portion of the patient engagement substrate; a secondary patient engagement substrate release liner configured to cover a second portion of the patient engagement substrate; a primary second patient engagement substrate release liner configured to cover a first portion of the second patient engagement substrate; and a secondary second patient engagement substrate release liner configured to cover a second portion of the second patient engagement substrate. The method can further include providing instructions to sequentially remove the primary patient engagement substrate release liner, secondary patient engagement substrate release liner, primary second patient engagement substrate release liner, and secondary second patient engagement substrate release liner. The method can further include providing instructions to shave, clip, trim, chemically remove, or otherwise depilate, and clean the skin of the patient. The method can further include measuring an impedance between the first and second defibrillator electrode pad. The method can further include measuring an impedance between a plurality of the one or more sensing electrodes. The method can further include analyzing the impedance between the first and second defibrillator electrode pad and the impedance between a plurality of the one or more sensing electrodes to verifying the correct placement of the first patient engagement substrate and the second patient engagement substrate. Verifying placement can include determining a location of a plurality of low power radios integrated with the wearable defibrillator.

[0027] In general, in one embodiment, a wearable device including one or more sensing electrodes configured to engage with a patient's skin to detect a signal, the one or more sensing electrodes configured to be in continuous electrical communication with the patient's skin; a patient engagement substrate including an adhesive, one or more sensing electrodes, and a fluid transport element configured to transport fluid away from the skin to allow the wearable device to be worn continuously; one or more compartments supported by the patient engagement substrate, the one or more compartments configured to reversibly receive and support one or more of: an energy source, one or more capacitors, and a controller; and an electrical connector configured to removably and reversibly engage with one or more of: the energy source, one or more capacitors, and the controller, the electrical connector supported by the patient engagement substrate and/or the one or more compartments.

[0028] This and other embodiments can include one or more of the following features. The wearable device can further include a second patient engagement substrate including an adhesive, one or more sensing electrodes, and a fluid transport element. The adhesive can include a plurality of pores configured to allow the transport of vapor. The patient engagement substrate can be configured to be worn continuously during movement and showering activities for greater than about 24 hours. The patient engagement substrate can be configured to be worn continuously during movement and showering

activities for greater than about 5 days. The patient engagement substrate can be configured to be worn continuously during movement and showering activities for greater than about 10 days.

[0029] In general, in one embodiment, a method for detecting symptoms associated with sleep apnea including measuring one or more of a heart rate, a breathing rate, and a breathing pattern of the patient

5 with a wearable device including one or more sensing electrodes and a sensor configured to measure the breathing rate and pattern of the patient, the wearable device adhesively attached to a portion of the skin of the patient; and analyzing the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, and breathing pattern to detect a symptom or indication of sleep apnea in the patient.

10 **[0030]** This and other embodiments can include one or more of the following features. The method can further include upon detection of the symptom or indication of sleep apnea in the patient, generating and providing a stimulus to the patient. Providing a stimulus can include a vibration, an electrical shock, a visual alert, or auditory alarm.

15 **[0031]** In general, in one embodiment, a method of detecting symptoms associated with a cardiac health of a patient including measuring one or more of a heart rate, a breathing rate, a breathing pattern of the patient, an impedance across and through a chest and thoracic cavity of the patient, and a size of blood vessels within a body of the patient like an inferior vena cava, blood pressure waveform, lung sounds, patient posture and activity, and pulse oxygenation with a wearable device including one or more sensing electrodes and one or more sensors configured to measure the heart rate, breathing rate and pattern of the 20 patient, the trans-thoracic impedance of the patient, and the size of the blood vessels in the body, blood pressure, wherein the wearable device is adhesively attached to a portion of the skin of the patient; and analyzing the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, breathing pattern, trans-thoracic impedance, blood pressure and blood pressure waveform in different body postures, and size of the blood vessels in the 25 body to detect a symptom or indication of cardiac disease in the patient.

20 **[0032]** This and other embodiments can include one or more of the following features. The method can further include upon detection of the symptom or indication of heart failure in the patient, generating and providing a stimulus to the patient. The stimulus can be one or more of: an electrical shock, a vibration, a visual alert, or an auditory alert to the patient or physician. The method can further include 30 upon detection of the symptom or indication of heart failure in the patient, saving a patient data to memory for later analysis or wirelessly transmitting the patient data to a computer for analysis. The method can further include analyzing the one or more of the measured parameters to determine a derived parameter for the patient for one or more of: ejection fraction, cyanosis, pulse quality, dyspnea, orthopnea, peripheral or pulmonary edema, right heart failure, left heart failure, nocturia, and cardiac 35 arrhythmias, pulsus alternans, S3 cardiac sound, S4 cardiac sound, and splitting in S1 and S2 heart sounds. The derived parameters can include pulmonary edema, ejection fraction, cyanosis, pulse quality, dyspnea, orthopnea, or nocturia. The measurements being used to detect the symptom or indication of cardiac disease can include cardiac arrest and myocardial infarction. The measurements being used to

detect the symptom or indication of cardiac disease can include heart failure, cardiomyopathies, heart blocks, atrial and ventricular arrhythmias. Pulmonary edema can be determined using chest impedance by measuring multiple vectors across the chest from various leads which allows assessment of fluid status in multiple different segments of the thoracic cavity. The method can further include analyzing the heart

5 sounds measured by a microphone to determine the presence or absence of one or more of: rales or rhonchi, the presence of S3 and S4 heart sounds, and pathologies such as splitting in the S1 and S2 heart sounds. Ejection fraction can be determined using ultrasound and localized impedance changes to determine trending information of blood flow over time as a proxy for ejection fraction. Cyanosis can be determined using pulse oxygenation and impedance status to determine changes in blood oxygenation.

10 Pulse quality can be determined using Doppler ultrasound delivered and can be measured by the wearable device together with closely spaced impedance sensors to determine changes in the shape of the pulse wave to indicate changes in cardiac function, including pulsus alternans. Dyspnea can be determined using a combination of accelerometer to determine patient posture and pulse oxygenation with impedance to determine the breathing pattern including accounting for recent activity of the patient to determine

15 whether dyspnea is at rest. Dyspnea can be determined using a combination of accelerometer to determine patient posture and pulse oxygenation with impedance to determine the breathing pattern including accounting for recent activity of the patient to determine whether dyspnea is at rest. Orthopnea can be determined using ultrasound to determine blood pressure together with accelerometer to determine patient posture can give an estimate of orthostasis. Nocturia can be determined using number of times the patient

20 gets up during sleep as a proxy for nocturia.

[0033] In general, in one embodiment, a wearable device including a patient engagement substrate including an adhesive, one or more sensors, a first fluid transport element configured to transport fluid away from the skin to allow the wearable device to be worn continuously, and a first vapor permeable layer, the one or more sensors adapted to detect one or more of a pulse, a cardiac signal, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of a patient; and a controller configured to receive data collected by the one or more sensors and analyze the data to determine if the patient exhibits a symptom associated with sleep apnea.

[0034] This and other embodiments can include one or more of the following features. The wearable device can further be configured to provide a stimulus to the patient upon detection of a symptom associated with sleep apnea. The stimulus can include a vibration, an electrical shock, a visual alert, electronic notification, or auditory alarm. The controller can be configured to apply an algorithm to the data collected by the one or more sensors. The algorithm can adapt to the specific patient wearing the device.

[0035] In general, in one embodiment, a wearable device including a patient engagement substrate including an adhesive, one or more sensors, a first fluid transport element configured to transport fluid away from the skin to allow the wearable device to be worn continuously, and a first vapor permeable layer, the one or more sensors adapted to detect one or more of a pulse, a cardiac signal, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart

rate of a patient; and a controller configured to receive data collected by the one or more sensors and analyze the data to determine if the patient exhibits a symptom associated with heart failure. The wearable device can further be configured to provide a stimulus to the patient upon detection of a symptom associated with heart failure. The stimulus can include a vibration, an electrical shock, a visual alert, electronic notification, or auditory alarm. The controller can be configured to apply an algorithm to the data collected by the one or more sensors. The algorithm can adapt to the specific patient wearing the device. The one or more sensors can include one or more of: accelerometer, ECG sensing electrodes, pulse oximeter, microphone, magnetometer, impedance sensors, and galvanic skin impedance sensor. The controller can further be configured to perform any of the previously described methods.

5 [0036] In general, in one embodiment, a system including any of the previously mentioned wearable defibrillators; and a fitting tool including a first complementary surface and a second complementary surface, the first complementary surface adapted to engage with a complementary surface of the one or more housings of the first patient engagement substrate and the second complementary surface adapted to engage with a complementary surface of the second patient engagement substrate.

10 [0037] This and other embodiments can include one or more of the following features. The fitting tool can further include a plurality of straps configured to secure the first patient engagement substrate and the second patient engagement substrate against a skin of the patient. The methods can further include providing a fitting tool including a first complementary surface and a second complementary surface, the first complementary surface adapted to engage with a complementary surface of the one or more housings 20 of the first patient engagement substrate and the second complementary surface adapted to engage with a complementary surface of the second patient engagement substrate. The method can further include providing instructions for wearing the fitting tool. The method can further include providing instructions for engaging the first complementary surface with the complementary surface of the one or more housings of the first patient engagement substrate to position the first patient engagement substrate on the 25 torso of the patient. The method can further include providing instructions for engaging the second complementary surface with the complementary surface of the second patient engagement substrate to position the second patient engagement substrate on the chest of the patient. The method can further include applying an algorithm to analyze the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, and breathing pattern 30 to detect the symptom or indication of sleep apnea in the patient. The algorithm can be a fixed algorithm. The algorithm can be an adaptive algorithm that adapts to the patient. The method can further include changing a sampling frequency of any of the one or more sensing electrodes and the sensor of the wearable device based on the algorithm. Changing the sampling frequency can be triggered by a predetermined characteristic collected by the one or more sensing electrodes and the sensor. The method 35 can further include applying an algorithm to analyze the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, breathing pattern, trans-thoracic impedance, blood pressure and blood pressure waveform in different body postures, and size of the blood vessels in the body to detect the symptom or indication of cardiac disease

in the patient. The algorithm can be a fixed algorithm. The algorithm can be an adaptive algorithm that adapts to the patient. The method can further include changing a sampling frequency of any of the one or more sensing electrodes and the sensor of the wearable device based on the algorithm. Changing the sampling frequency can be triggered by a predetermined characteristic collected by the one or more 5 sensing electrodes and the sensor.

BRIEF DESCRIPTION OF THE DRAWINGS

[0038] The novel features of the invention are set forth with particularity in the claims that follow.

A better understanding of the features and advantages of the present invention will be obtained by 10 reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying drawings of which:

[0039] FIG. 1 illustrates an embodiment of a wearable defibrillator on a patient in accordance with some embodiments.

[0040] FIGS. 2A-2D illustrate various views of a patient engagement substrate that is part of a 15 wearable defibrillator in accordance with some embodiments.

[0041] FIGS. 3A-3C illustrate an exterior view and two exploded views, respectively, of a patient engagement substrate and a plurality of housings in accordance with some embodiments.

[0042] FIG. 4 illustrates a flexible circuit that can be used in the wearable defibrillators described herein.

[0043] FIGS. 5A-5C illustrate an exterior view and two exploded views, respectively, of a patient 20 engagement substrate and a plurality of housings in accordance with some embodiments.

[0044] FIG. 6 illustrates a method for forming a portion of a wearable defibrillator with a patient engagement substrate having a preformed curvature in accordance with some embodiments.

[0045] FIGS. 7A-7B illustrate an exterior view and exploded view, respectively, of a patient 25 engagement substrate that is part of a wearable defibrillator in accordance with some embodiments.

[0046] FIG. 8 illustrates a side-view of a plurality of housings that can be incorporated into the wearable defibrillators described herein.

[0047] FIGS. 9A-9C illustrate a side view, bottom view, and cross-sectional view of a housing containing a capacitor in accordance with some embodiments.

[0048] FIGS. 10A-10C illustrate electrical connections that can be used in embodiments of the 30 wearable defibrillators described herein.

[0049] FIG. 11A-11B illustrate electrode configurations that can be used in embodiments of the wearable defibrillators described herein.

[0050] FIG. 12 illustrates an example of anatomical locations for sensing electrodes.

[0051] FIG. 13 illustrates a schematic flow chart for how the wearable defibrillators described herein 35 can be used by the patient.

[0052] FIG. 14 is a flow chart of a method of monitoring and defibrillating a patient's heart in accordance with some embodiments.

5 [0053] FIG. 15A is a flow chart of a method of monitoring a patient's heart to detect a symptom or indication of cardiac disease in the patient in accordance with some embodiments. FIG. 15B illustrates a schematic flow chart of a method of detecting symptoms associated with heart failure in accordance with some embodiments.

[0054] FIG. 16 is a flow chart of a method of refurbishing a wearable defibrillator in accordance with some embodiments.

10 [0055] FIGS. 17-20 illustrates examples of refurbishing embodiments of the wearable defibrillators described herein.

[0056] FIGS. 21-23 illustrate a cross-sectional view of embodiments of wearable defibrillators.

[0057] FIG. 24A-24B illustrate examples of release liners that can be used with the patient engagement substrates of the wearable defibrillators described herein.

[0058] FIG. 25 is a wearable defibrillator in accordance with some embodiments.

15 [0059] FIG. 26 is a portion of a wearable defibrillator in accordance with some embodiments.

[0060] FIG. 27 is a portion of a wearable defibrillator in accordance with some embodiments.

[0061] FIG. 28 is a portion of a wearable defibrillator in accordance with some embodiments.

[0062] FIG. 29 is a portion of a wearable defibrillator in accordance with some embodiments.

20 [0063] FIG. 30 is a schematic illustration of an upper and lower patch that can be used with the wearable defibrillators described herein.

[0064] FIG. 31 is a portion of a wearable defibrillator in accordance with some embodiments.

[0065] FIG. 32 is a housing that can be used with the wearable defibrillators described herein.

[0066] FIG. 33 is a cross-sectional view of a portion of a wearable defibrillator.

25 [0067] FIG. 34 illustrates a pair of electrodes that can be used in the wearable defibrillators described herein.

[0068] FIG. 35 illustrates a cross-sectional view of a configuration of a defibrillator electrode that can be used in the wearable defibrillators described herein.

[0069] FIG. 36 illustrates an electrode configuration with micro-needles in accordance with some embodiments.

30 [0070] FIGS. 37A-37C illustrate embodiments of connections between a housing and patient engagement substrate that can be used in the embodiments of the wearable defibrillators disclosed herein.

[0071] FIG. 38 is a schematic illustration of moisture transport across an embodiment of a conductive adhesive that can be used in the wearable defibrillators disclosed herein.

35 [0072] FIG. 39 is a schematic illustration of moisture transport across an embodiment of a conductive adhesive and electrode that can be used in the wearable defibrillators disclosed herein.

[0073] FIG. 40 is a schematic illustration of a portion of a wearable defibrillator measuring a multi-vector trans-thoracic impedance of a patient in accordance with some embodiments.

[0074] FIG. 41A is a flow chart of a method for detecting symptoms associated with sleep apnea in a patient in accordance with some embodiments. FIG. 41B illustrates a schematic flow chart of a method of detecting symptoms associated with sleep apnea in a patient in accordance with some embodiments.

[0075] FIG. 42 is a flow chart illustrating a method of providing instructions for placing the 5 wearable defibrillators described herein.

[0076] FIGS. 43A-43B illustrate a device that can be used to fit the wearable devices described herein to the patient in accordance with some embodiments.

DETAILED DESCRIPTION

10 [0077] Wearable defibrillators are disclosed herein that are configured for long term wear. The wearable defibrillators can include a plurality of different sensors and electrodes to measure and analyze the condition of the wearer of the defibrillator and to deliver a therapeutic electrical shock or other stimulus to the wearer. Methods for using the wearable defibrillators and methods for processing the wearable defibrillators are also disclosed herein.

15 [0078] Wearable external defibrillators are provided herein. The wearable defibrillators can include one or more sensing electrodes configured to engage with a patient's skin to detect a cardiac signal. The wearable defibrillators can include a first defibrillator electrode pad configured to engage with the patient's skin and to deliver an electrical therapy to the patient. The wearable defibrillators can include a first patient engagement substrate including an adhesive, the first defibrillator electrode pad, a first fluid 20 transport element configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a first vapor permeable layer. The first defibrillator electrode pad can be configured to be in continuous contact with the patient's skin. The wearable defibrillator can include a second patient engagement substrate including a second defibrillator electrode pad, a second adhesive, a second fluid transport element in fluid communication with the second patient engagement 25 substrate configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a second vapor permeable layer. The wearable defibrillators include an energy source, one or more capacitors in electrical communication with the energy source and the first defibrillator electrode pad and the second defibrillator electrode pad, and a controller configured to detect the cardiac signal with the one or more sensing electrodes and the sensing electrode of the second patient 30 engagement substrate. The controller can also be adapted to charge the one or more capacitors with the energy source followed by discharging the one or more capacitors to deliver a therapeutic shock through the first defibrillator electrode pad and the second defibrillator electrode pad to the patient while the first and second patient engagement substrates are engaged with the patient. The energy source, one or more capacitors, and controller can be enclosed within one or more housings.

35 [0079] The one or more sensing electrodes can be separate sensors from the first and second patient engagement substrates or can be included in the first and second patient engagement substrates. In some embodiments the first patient engagement substrate includes the one or more sensing electrodes. In one example the first patient engagement substrate comprises two or more sensing electrodes. In some

embodiments the second patient engagement substrate comprises a sensing electrode. In some embodiments the cardiac signal can also be sensed through the defibrillator electrode pads. For example, the first defibrillator electrode pad and second defibrillator electrode pad are adapted to detect the cardiac signal.

5 [0080] The defibrillator electrode pads can be in continuous direct contact with the patient's skin or in electrical contact through a conductive material, such as a conductive hydrogel or gel. The continuous contact between the defibrillator electrode pads and the patient's skin allows the device to deliver the therapeutic shock or therapy to the patient on command. The layered construction and moisture vapor transport properties of the wearable defibrillator devices described herein improve contact between the 10 skin and the device that can allow improved comfort and for long term wear of the device.

[0081] The wearable defibrillator can include electrodes and adhesive that can be modified to improve the long term wearability of the defibrillator. A layered construction can be used to improve fluid transport away from the skin to improve the wearability of the defibrillator.

15 [0082] The wearable external defibrillator can be configured to be worn continuously during movement and showering activities for greater than about 24 hours. The wearable external defibrillator can be configured to be worn continuously during movement and showering activities for greater than about 20 days. The wearable external defibrillator can be configured to be worn continuously during movement and showering activities for greater than about 5 days. The wearable external defibrillator can be configured to be worn continuously during movement and showering activities for greater than about 7 days. The wearable external defibrillator can be configured to be worn continuously during movement and showering activities for greater than about 10 days.

25 [0083] FIG. 1 illustrates a wearable defibrillator 100 on a patient. The wearable defibrillator 100 includes an upper patch or upper patient engagement substrate 102 and a lower patch or lower patient engagement substrate 104. The lower patient engagement substrate 104 supports one or more housings 106 that contain the device electronics. A cable 108 provides electrical communication between the upper patch 102 and lower patch 104. Each of the upper and lower patient engagement substrates include a defibrillator electrode pad and one or more ECG sensing electrodes. The ECG sensing electrodes can provide patient data to the electronics on board the device 100 and upon determination of a treatable arrhythmia a therapeutic electrical shock can be provided to the patient through the defibrillator electrode pads on the patient engagement substrates 102, 104.

30 [0084] The one or more housings can include a first controller housing with the controller included in the first controller housing. The one or more housings can include a first energy source housing with the energy source included in the first energy source housing. The one or more housings can include a first capacitor housing and a second capacitor housing with the capacitors included in the first capacitor housing and the second capacitor housing.

35 [0085] The first controller housing can include a first controller housing electrical connection. The first energy source housing can include a first energy source housing electrical connection. The first capacitor housing can include a first capacitor electrical connection and the second capacitor housing can includes a second electrical connection. The housing electrical connections can engage within the

flexible circuit within the patch. The wearable defibrillator can include a mechanical connection between each of the first controller housing, first energy source housing, first capacitor housing, and second capacitor housing.

[0086] The wearable defibrillator can include a flexible circuitry. The flexible circuitry can include 5 one or more rigid printed circuit boards (PCBs). The flexible circuitry can be within the patient engagement substrate and/or within one or more of the housings. The flexible circuitry can be adapted to receive the first controller housing electrical connection, the first energy source housing electrical connection, the first capacitor electrical connection, and the second electrical connection. The flexible circuitry can be in electrical communication with the first controller housing, first energy source housing, 10 first capacitor housing, and second capacitor housing.

[0087] The flexible circuitry provides electrical communication between the first controller housing and the first energy source housing, first capacitor housing, and second capacitor housing. The flexible circuitry can be supported by the first patient engagement substrate between the first vapor permeable layer and the first defibrillator electrode pad.

[0088] In some embodiments the first patient engagement substrate is adapted to support the one or more housings. In some embodiments the second patient engagement substrate is adapted to support the one or more housings.

[0089] The first patient engagement substrate and second patient engagement substrate can be configured to be worn during showering activities.

[0090] The vapor permeable layer can be made out of flexible material. In some embodiments the vapor permeable layer is a fabric with a woven or non-woven construction. A portion of the first vapor permeable layer can represent an exterior surface of the first patient engagement surface. A portion of the second vapor permeable layer can represent an exterior surface of the second patient engagement surface. The exterior surfaces of the first patient engagement substrate and the second patient engagement 20 substrate can be moisture vapor permeable. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 10 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 1000 g/m² per day based on a surface area of the patient engagement substrate. The exterior 25 surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 2000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 3000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient 30 engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 4000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 5000 g/m² per day based on a surface area of the patient

engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 6000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 7000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 8000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 9000 g/m² per day based on a surface area of the patient engagement substrate. The exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can have a moisture vapor transport above about 10000 g/m² per day based on a surface area of the patient engagement substrate.

[0091] In some cases the exterior surfaces of the first patient engagement substrate and the second patient engagement substrate can be air permeable. In some embodiments the exterior surfaces of the first patient engagement substrate and the second patient engagement substrate are waterproof. The exterior surfaces of the first and second patient engagement substrates can be hydrophobic. In some cases the exterior surfaces of the first and second patient engagement substrates are water resistant. Examples of vapor permeable layers include: Gore Tex®, water proof fabrics, water resistant fabrics, water repellent fabrics, fabrics with a hydrophobic surface, waterproof non-woven fabrics, etc. Other examples of vapor permeable layers include laminated membranes, multi-layer structures, materials with ePTFE (expanded polytetrafluoroethylene) coatings, polyurethanes, etc.

[0092] The first fluid transport element and second fluid transport element can be configured to transport fluid away from the skin. The fluid transport element can be a wicking material that improves fluid transport from the side of the patient engagement substrate that contacts the skin and the outer vapor permeable surface of the wearable defibrillator. The fluid transport element can have a flexible sheet like configuration. The fluid transport element can have a woven or non-woven configuration. Examples of fluid transport materials include cotton, polyester, cellulose, reticulated polyurethane foam, and non-woven constructions.

[0093] The wearable defibrillators can include a support chassis disposed between the one or more housings and the first defibrillator electrode pad. The support chassis can be adapted to spread a shear load of the one or more housings across a dominant surface of the support chassis. The support chassis can have a sheet like configuration. In some embodiments multiple support chassis layers can be used in the patient engagement substrate. One support chassis layer could be made out of a more flexible material and another support chassis material that is more rigid could be attached or engaged with the support chassis layer. The support chassis can have a flexible or semi-rigid structure. Examples of support chassis materials include PVC, EVA, polyethylene, nylon, polyurethane, etc. In some embodiments the support chassis layer may have poor fluid transport properties. A plurality of openings

or pores can be included in the support chassis material to improve fluid movement across the support chassis layer.

[0094] The wearable defibrillators can include a structural ring or other support structure to improve the spread of the weight of the device across the surface area of the patient engagement substrate. The 5 structural rings can be used in combination with the support chassis to support any heavier or rigid components engaged with the patient engagement substrate, such as the housings containing the electronics modules. The structural rings can also provide an opening to accommodate the electrical connection between the electronics components in the one or more housings and a flexible circuit within the patient engagement substrate. The support rings can include a rigid component and flexible 10 component. The support rings can be bonded or attached directly to the support chassis layer. The structural rings can help prevent the patient engagement substrate and prevent or reduce buckling of the patient engagement substrate from the weight of the housings and electronics components. The structural rings can help keep the patient engagement substrate relatively flat and to reduce buckling and separation between the patient engagement substrate and the skin of the patient. The structural rings can include 15 perforations or pores to allow moisture to pass through the structural rings. The structural rings can also include a perforations to allow the structural rings to flex but not buckle. Examples of materials that can be used in the structural rings include nylon, polyethylene, ABS, polypropylene, PET, and other thermoplastic materials that can be molded or cut from sheets.

[0095] A variety of sensors and modules can be included within the one or more housings of the 20 wearable defibrillator. The sensors and modules can be included on a PCB within the housing or in the layered construction of the patient engagement substrates, such as the conductive gels. The controller or processor of the wearable defibrillator can be configured to analyze data recorded by any of the sensors and modules described herein. In one example the wearable defibrillator includes a temperature sensor. In one example the wearable defibrillator includes a pulse oximeter configured to measure an oxygen 25 content of a blood of the patient at a point on a chest of the patient. In one example the wearable defibrillator includes an ultrasound transceiver or transducer configured to transmit and/or receive ultrasonic signals. In one example the wearable defibrillator includes a Doppler radar configured to transmit a microwave signal and receive a returned microwave signal. In one example the wearable defibrillator includes an inclinometer configured to determine the position and orientation of the wearable 30 defibrillator. In one example the wearable defibrillator includes a radio beacon configured to transmit the location of the wearable defibrillator. In one example the wearable defibrillator includes a GPS sensor. In one example the wearable defibrillator includes an accelerometer. In one example the wearable defibrillator includes a microphone. In one example the wearable defibrillator includes a wireless radio configured to wirelessly transmit data from the wearable defibrillator. The wireless radio can be 35 configured to transmit data over a cellular network or Wi-Fi network. In one example the wearable defibrillator includes a sensor configured to measure a mechanical stretch of a portion of the wearable defibrillator. In one example the wearable defibrillator can include a magnetometer. In one example the wearable defibrillator can include impedance sensors, such as galvanic skin impedance sensors.

[0096] In one example the wearable defibrillator includes a tactile feedback module. The tactile feedback module can be part of the first patient engagement substrate or second patient engagement substrate. The tactile feedback module can be part of the one or more housings. In one example the tactile feedback module is a vibration motor.

5 **[0097]** In one example the wearable defibrillator includes an external pacing module configured to provide a pacing signal to the patient. The external pacing module can be supported by the first or second patient engagement substrate.

10 **[0098]** In one example the wearable defibrillator includes a skin contact module configured to sense removal of the first and/or second patient engagement substrate from the patient's skin. The skin contact module can be configured to generate an alarm and/or notification to a healthcare provider upon sensing removal of the first and/or second patient engagement substrate from the patient's skin.

15 **[0099]** The wearable defibrillators can include a connector plug on the housing with a plurality of electrical connections. The plurality of electrical connections can include a first defibrillator electrode pad connection and a second defibrillator electrode pad connection. The first defibrillator electrode pad connection and the second defibrillator electrode pad connection can be configured to be in electrical communication with the one or more capacitors and the first and second defibrillator electrode pads. The plurality of electrical connections can also include a plurality of sensing electrode connections. The plurality of sensing electrode connections can be each configured to be in electrical communication with the controller and one of the one or more sensing electrodes. The wearable defibrillator can include an
20 enclosure configured to surround the housing with an enclosure connection having a first side with a complementary structure configured to engage with the connector plug on the housing. A second side of the enclosure connection can be configured to engage with a patient engagement substrate connector on the first patient engagement substrate. The patient engagement substrate connector can be in electrical communication with the one or more capacitors and the first and second defibrillator electrode pads.

25 **[0100]** In some embodiments the adhesive can include a plurality of pores configured to allow the transport of vapor.

30 **[0101]** In some embodiments ECG sensing electrodes and defibrillator electrode pads can include a plurality of pores configured to allow the transport of vapor. The pores can improve the fluid transport properties of the electrodes. The size, shape, and number of the plurality of pores can be configured to minimize the transport of liquid droplets.

35 **[0102]** In some embodiments the defibrillator electrode pads can include a conductive adhesive and a conductive electrode. In one example the conductive electrodes can have a solid construction. In another example the conductive electrodes can be made from a flexible sheet having a plurality of perforations. Examples of conductive electrode materials include a carbon vinyl film, Ag/AgCl coated carbon vinyl film, polyethylene terephthalate (PET) films, Ag coated carbon vinyl film, electrodes with a conductive ink, PET coated with carbon, PET films with conductive coatings, PET coated with Ag/AgCl, PET coated with Ag, etc.

[0103] The conductive ink can be applied to the electrode substrate with a desired thickness. Generally, the thicker the conductive ink coating the higher the conductivity. The thickness of the conductive ink can be uniform in some embodiments. The conductive ink can be depleted while sending a direct current to the patient through the defibrillator electrode pads. The conductive ink can be provided on the electrode substrate with a thickness sufficient to last through providing a defibrillating shock. In embodiments that use a conductive electrode substrate, like a carbon vinyl substrate, the underlying electrode substrate is conductive and can continue to provide current even in areas where the conductive ink has been depleted.

5 **[0104]** In another example the conductive electrodes of the defibrillator electrode pads can have a woven structure. In one example the conductive electrode can include carbon fiber.

10 **[0105]** In some embodiments the conductive adhesive is a conductive hydrogel. In some embodiments the conductive adhesive can include a salt. In some embodiments the conductive adhesive is an adhesive with a conductive filler. The conductive filler can include one or more of: carbon nanotubes, graphene, carbon black, silver particles, metal particles, and silver nanowires.

15 **[0106]** The first and second patient engagement substrates can be configured to insulate between the sensing electrodes, the defibrillator electrode pad, and other portions of the patient engagement substrate. In one example an adhesive on the first and second patient engagement substrates is non-conductive and can be used to insulate the electrodes.

20 **[0107]** In some embodiments the electronics components can be configured to be reversibly and removably engaged with a portion of the wearable defibrillator. The one or more capacitors can be configured to be reversibly and removably engaged with the wearable defibrillator. The energy source can be configured to be reversibly and removably engaged with the wearable defibrillator. The controller/processer can be configured to be reversibly and removably engaged with the wearable defibrillator.

25 **[0108]** In some embodiments the housing includes a plurality of compartments containing the energy source, one or more capacitors, and controller. The wearable defibrillator can include a flexible circuitry and one or more rigid printed circuit boards (PCBs) within the housing. The plurality of compartments can be in fluid communication within the housing. In some cases the plurality of compartments may not be in fluid communication with the other of the plurality of compartments. In some cases the plurality of 30 compartments are separate and configured to reversibly engage with the other of the plurality of compartments. In some embodiments the plurality of compartments are connected with a plurality of waterproof connector segments.

35 **[0109]** The housing can be configured to allow relative movement between the plurality of compartments of the housing. The relative movement can include flexing with a plane of the first patient engagement substrate.

[0110] The housing can include an outer clam shell and a base. The outer clam shell and base can be secured together with mechanical or chemical fixation. In one example the outer claim shell can be attached and sealed to the base with screws and a gasket, plastic snap hooks and a gasket, or other

mechanical fixation structures. The outer clam shell can be ultrasonically welded to the base. The outer clam shell can be attached to the base with an adhesive. The outer clam shell can be attached to the base through chemical bonding. In some embodiments the one or more housings each have a clam shell configuration sealed with an adhesive. In some embodiments the one or more housings each have a clam shell configuration sealed through chemical bonding. In some examples ultrasonic welding can be used to 5 secure the outer clam shell to the base.

[0111] In some embodiments the one or more sensing electrodes of the first patient engagement substrate and the sensing electrode of the second patient engagement substrate and the first and second defibrillator electrode pads can be configured to sense impedance changes along a plurality of vectors of 10 the patient. The controller can be configured to analyze the impedance changes along the plurality of vectors of the patient to measure a cardiac health of the patient.

[0112] In some embodiments the controller is configured to analyze an impedance between one or 15 more of: the one or more sensing electrodes, the first defibrillator electrode pad, the second defibrillator electrode pad, and the sensing electrode. The controller can also be configured to measure the impedance using two or more discrete frequencies. For example, the two or more discrete frequencies can include a high frequency measurement and a low frequency measurement. The controller can analyze the high frequency measurement and low frequency measurement to determine a power of the therapeutic shock 20 for the patient based on the impedance.

[0113] The moisture vapor transmission rate of the patient engagement substrate can be configured 25 to transport moisture from the skin. The moisture vapor transport properties can also be measured across each of the patient engagement substrates. The ability of the patient engagement substrate to move moisture/vapor from the patient engagement portion (e.g., adhesive, sensing electrode gel, and defibrillator electrode pad gel) of the wearable defibrillator through the device and across the outer surface on the side of the patient engagement substrate opposing the adhesive and gels (e.g., vapor 30 permeable layer) can be measured. The upper and lower patient engagement substrates can have similar moisture vapor transport properties. The moisture vapor transmission rate can be the average moisture vapor transmission across the total surface area of the patient engagement surface. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 10 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 50 g/m² per day based on a surface 35 area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 100 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 150 g/m² per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or

second patient engagement substrate includes a moisture vapor transport above about 100 g/m^2 per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 500 g/m^2 per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 1000 g/m^2 per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer. In some embodiments the first or second patient engagement substrate includes a moisture vapor transport above about 1500 g/m^2 per day based on a surface area of the patient engagement portion through the patient engagement portion and the first or second vapor permeable layer.

5 [0114] In some embodiments the lower or first patient engagement substrate has a preformed curvature. The preformed curvature can correspond to a shape of a human torso. In some embodiments the upper or second patient engagement substrate has a preformed curvature. The preformed curvature of 10 the upper patient engagement substrate can correspond to a shape of a human chest.

15 [0115] A cable can form an electrical communication between the first patient engagement substrate and the second patient engagement substrate. For example the cable forms the electrical communication between the sensing electrode of the second patient engagement substrate and the controller. The cable can also form an electrical communication between the second defibrillator electrode pad and the one or 20 more capacitors.

25 [0116] The wearable defibrillator can include a display indicator. The display indicator can be part of the first patient engagement substrate or second patient engagement substrate. The display indicator can be part of the one or more housings. The display indicator can be part of a cable between the first patient engagement substrate or second patient engagement substrate. In one example the display indicator is a light emitting diode (LED).

[0117] The wearable defibrillators can include one or more buttons on the one or more housings alone or in combination with a display. The buttons can be a mechanical switch, button, or capacitive switch.

30 [0118] FIGS. 2A-2D illustrate various views of the lower patient engagement substrate 104. FIG. 2A illustrates a top exterior of the lower patient engagement substrate 104 without the one or more housings 106 engaged to the lower patient engagement substrate 104. The lower patient engagement substrate 104 includes a border layer 120, a vapor permeable layer 122, a plurality of structural rings 124 at openings of the vapor permeable layer 122, and a cable connection 126 between the cable 108 and an interior of the patient engagement substrate. The border layer 120 can be ultrasonically welded or adhered 35 to seal the edges of the patient engagement substrate to prevent water ingress to the interior of the patient engagement substrate from the sides of the patient engagement substrate. The border layer 120 can be welded to the vapor permeable layer 122 to form a seal. The border layer 120 can also include an adhesive that can adhere the patient engagement substrate to the skin of the patient.

[0119] FIG. 2B illustrates a bottom exterior of the lower patient engagement substrate 104 adapted to contact the skin of the patient. The lower patient engagement substrate 104 includes an adhesive 128 adapted to engage with the skin for long term wear, a plurality of ECG sensing electrode conductive gels 130, and a defibrillator electrode pad gel 132. The ECG sensing electrode conductive gels 130 are in electrical communication with the ECG sensing electrodes. The defibrillator electrode pad gel 132 is in electrical communication with the defibrillator electrode pad to deliver a therapeutic shock upon detection of a treatable arrhythmia. The ECG sensing electrode conductive gels 130 and the defibrillator electrode pad gel 132 are conducive gels that are adapted for long term wear of the device.

[0120] FIG. 2C illustrates the lower patient engagement surface 104 without the cable 108. FIG. 2D 10 illustrates the lower patient engagement surface 104 having a preformed curvature. Some or all of the components in the lower patient engagement surface 104 can be assembled with a preformed curvature or processed during assembly to include a preformed curvature. The preformed curvature can be modeled after the anatomy of a human torso to improve compatibility with the lower patient engagement surface and the body of the patient. The preformed curvature can also reduce residual stresses in the device 15 during use and improve the comfort of the device and other long term wear features of the wearable defibrillator.

[0121] FIG. 3A illustrates the lower patient engagement substrate 104 and one or more housings 106. The one or more housings are illustrated as housings 106a, 106b, 106c, and 106d. The housing 106a includes a button/display 134. The housing 106a can enclose and support the controller and memory 154. 20 The housings 106b, 106c can enclose and support capacitors 156, 158 of the device 100. The housing 106d can support the energy source 160, such as a battery.

[0122] FIG. 3B illustrates an exploded view of the wearable defibrillator 100. The wearable defibrillator 100 can include an adhesive 128, ECG sensing electrode conductive gels 130, and defibrillator electrode pad gel 132. The adhesive 128 includes openings to accommodate the shapes of the 25 ECG sensing electrode conductive gels 130 and defibrillator electrode pad gel 132. The defibrillator electrode pad gel 132 can have a shape that matches the shape of the defibrillator electrode pad 140. Electrical energy can be delivered through the defibrillator electrode pad 140 and defibrillator electrode pad gel 132 to provide a therapeutic electrical shock to the patient. The device can include a fluid transport layer 142 such as a wicking layer. The wicking layer can improve the movement of moisture 30 from the surface of the wearable defibrillator 100 having the gels that contacts the skin through the device. Improved moisture management with the surface of the device that contacts the skins can improve the comfort of the device to the wearer. The wearable defibrillator can include a flexible circuit 144 with a plurality of ECG sensing electrodes 146. The ECG sensing electrodes 146 can be in electrical communication with the ECG sensing electrode conductive gels 130. The wearable defibrillator can 35 include a support chassis 148 that can spread the shear force from the weight of the one or more housings 106 across a larger surface area of the device. The support chassis can improve adhesion between the adhesive 128 and conductive gels 130, 312 and the skin to support the weight of the one or more housings and electrical components. The illustrated support chassis includes a plurality of openings to improve

fluid transport across the support chassis 148. The illustrated wearable defibrillator includes the border layer 120, the vapor permeable layer 122, and the plurality of structural rings 124 at openings of the vapor permeable layer 122. The border layer 120 can form a seal between the vapor permeable layer 122 and the adhesive 128 and conductive gels 130, 132. The structural rings 124 can be configured to allow 5 electrical connections to pass through them from the flexible circuit 144 to one or more housings 106. The structural rings 124 can be engaged with or attached to the support chassis 148 to improve the ability of the device to spread the shear weight of the one or more housings across the support chassis 148 and the surface area of the patient engagement substrate. The one or more housings include an upper shell 150 and lower shell 152 that form a plurality of compartments or individual housings that receive the 10 electrical components of the wearable defibrillator 100. A first compartment of the housing 106 includes a controller and memory 154. A second compartment of the housing 106 includes a first capacitor module 156 and a third compartment of the housing 106 includes a second capacitor module 158. A fourth compartment of the housing 106 includes the energy source 160, shown as a battery. FIG. 3C illustrates a cross-sectional view of the wearable defibrillator 100 that shows the preformed curvature of 15 the patient engagement substrate 104.

[0123] FIG. 4 is an enlarged view of a portion of the flexible circuit 144. The flexible circuit includes a plurality of connections 170 that can be used to engage with and receive signals from the ECG sensors 146. The flexible circuit 144 can include a connector 172 that can engage with a complementary section of the one or more housings 106 to form electrical communication between the flexible circuit 20 144 and one or more housings 106, such as the connector shown in FIG. 9B. The flexible circuit 144 can be in electrical communication with the defibrillator electrode pad and the ECG sensors. The flexible circuit 144 can include a separate connection for each of the one or more housings.

[0124] FIGS. 5A-5C illustrate a lower patient engagement substrate 104 in accordance with some embodiments. A button 134 is illustrated as a switch in the housing 106a. The housing 106 can also 25 include a display as part of one of the housings 106a, 106b, 106c, and 106d. The illustrated lower patient engagement substrate 104 includes a different footprint and complementary shapes for the defibrillator electrode gel 132, defibrillator electrode 140, and adhesive 128. The housings 106a, 106b, 106c, and 106d are mechanically connected but electrically separated. The housings 106a, 106b, 106c, and 106d are illustrated with a preformed curvature that can match the torso anatomy. The housings 106a, 106b, 106c, 30 and 106d also can bend relative to each other to accommodate different curvatures of the patient torso.

[0125] FIG. 6 illustrates an apparatus 180 and process for forming the preformed curvature on the patient engagement substrate. FIG. 6 illustrates the components of a lower patient engagement substrate 104 although a similar process can be used for any of the patient engagement substrates and components described herein. The apparatus 180 includes a curved surface 182 with a curvature designed to mimic the 35 curvature of a typical human torso. The apparatus 180 also includes a roller 184 adapted to apply pressure to the components of the patient engagement substrate to conform the components of the patient engagement substrate to the curvature of the curved surface 182. The illustrated lower patient engagement substrate 104 includes multiple adhesive bonding layers 140a, 148b, and 148c. The adhesive

bonding layers have a plurality of openings that match the layers they are joining, such as the chassis layer 148 and the defibrillator electrode pad 140. The chassis layer 148 includes the structural rings for the housings. The illustrated lower patient engagement substrate 104 includes a multiple layer defibrillator electrode configuration with defibrillator electrode pad 140. The flexible circuit 144 is not shown in FIG. 6 but it can be included between the fluid transport element 142 and the support chassis 148 or between other layers of the patient engagement substrate. The patient engagement substrate can be built layer by layer on the apparatus 180. The roller 184 can be used to apply the curvature to each individual layer as it is added and/or it can be used to apply the curvature to the assembled patient engagement substrate 104. The apparatus 180 can be used to apply a preformed curvature to the patient engagement substrates such that they can have a residual stress that can improve conformity of the patient engagement substrate to the patient anatomy, such as the torso.

[0126] FIGS. 7A and 7B illustrate an upper patch or upper patient engagement substrate 102 in accordance with some embodiments. The upper patient engagement substrate 102 can have a generally similar construction to the lower patient engagement substrate 104. Typically, the footprint of the upper patient engagement substrate 102 can be smaller than the footprint of the lower patient engagement substrate 104 when the one or more housings are supported by the lower patient engagement substrate 104. The upper patient engagement substrate 102 can be adapted to adhere to the upper chest of the patient as shown in FIG. 1. The upper patient engagement substrate 102 has an outer surface that includes a vapor permeable membrane 190 and a border 192. The upper patient engagement substrate 102 also includes a support chassis 194, a flexible circuit 196 with an ECG sensing electrode 198, a fluid transport element 200 like a wicking layer, a defibrillator electrode pad 202, ECG sensing electrode gel 204, a defibrillator electrode pad gel 206, and adhesive 208. The upper patient engagement substrate 102 is illustrated with a single ECG sensing electrode 198. In some embodiments the upper patient engagement substrate can include two or more ECG sensing electrodes. The defibrillator pad electrodes 25 can also be used to detect cardiac signals and work as ECG sensing electrodes. The cable 108 can engage with the upper patient engagement substrate 102 through a connector 210 to be in electrical communication with the flexible circuit 196. Data from the ECG sensing electrodes can be sent via the cable 108 to the controller and electronics in the one or more housings 106. Upon detection of a treatable arrhythmia, the controller can charge the capacitors with the energy source. After the capacitors are charged a therapeutic electrical shock can be provided to the defibrillator electrode pad 202.

[0127] FIG. 8 illustrates a side-view of a plurality of housings 106a, 106b, 106c, and 106d. The housings 106 are formed from an upper shell 150 and lower shell 152 that form separate interior portions for the plurality of housings 106a, 106b, 106c, and 106d of the wearable defibrillator. The housing 106a includes an electrical connector 107a adapted to electrically communicate with the flexible circuit 144. The housing 106b includes an electrical connector 107b adapted to electrically communicate with the flexible circuit 144. The housing 106c includes an electrical connector 107c adapted to electrically communicate with the flexible circuit 144. The housing 106d includes an electrical connector 107d adapted to electrically communicate with the flexible circuit 144. In one example the housing 106a can

enclose and support the controller and memory 154. The electrical connection 107a can facilitate the transmission of signals between the controller and memory 154 and other device hardware via the flexible circuit 144. The housings 106b, 106c can enclose and support capacitors 156, 158 of the device 100. The electrical connections 107b, 107c can facilitate the transmission of signals between the capacitors 156, 158 and other device hardware via the flexible circuit 144. The housing 106d can support the energy source 160, such as a battery. The electrical connection 107d can facilitate the transmission of signals between the battery and other device hardware via the flexible circuit 144. In one example the controller and memory 154 receive and analyze signals from the ECG sensing electrodes to determine if a treatable arrhythmia is present. Upon detection of the treatable arrhythmia the controller 154 can send a signal to the energy source 160 to charge the capacitors 156, 158 via the flexible circuit 144. After the capacitors 156, 158 have been charged to a sufficient level the controller 154 can instruct the capacitors 156, 158 to discharge the electrical energy through the flexible circuit 144 to the defibrillator electrode pads 140, 202. The housing 106 is illustrated with four housings 106a, 106b, 106c, and 106d containing the controller and memory 154, capacitors 156, 158, and energy source 160; however, alternate configurations can be used that use more or less housings to support the electronics such as the controller and memory 154, capacitors 156, 158, and energy source 160. For example, the electronics could be stored in a single housing, two separate housings, three separate housings, five separate housings, or six or more separate housings.

[0128] FIGS. 9A-9C illustrate a housing 106b containing a capacitor 156 in accordance with some embodiments. The housing 106b includes an upper shell 150 and lower shell 152 with capacitors 156 inside. The housing 106b includes electrical connection 107b. The illustrated electrical connection 107b can engage with a complementary structure on the flexible circuit 144, such as the connector 172 shown in FIG. 4. The illustrated capacitor configuration includes two capacitors 156, 156b. In some embodiments a single capacitors can be included within the housing 107b. In other embodiments multiple capacitors can be included the housing 107b.

[0129] FIG. 10A is a schematic illustration of the electrical connection between the cable 108 and the patient engagement substrate. The flexible circuit 144 has a cable connection receptacle 127 engaged with or integral to the flexible circuit 144. The cable connection receptacle 127 has a complementary structure to receive the cable connection 126 of the cable 108. The cable 108 can electrically communicate with the flexible circuit 144 when the cable connection 126 is engaged with the cable connection receptacle 127.

[0130] FIG. 10B illustrates a schematic example of an electrical connection between a circuit board 220 within the housing 106 and the lower patient engagement substrate 104 in accordance with some embodiments. The circuit board 220 can have a connector 222 that engages with an electrical connector 224 of the housing 106 that engages with an electrical connector 226 of the flexible circuit 144. The electrical connection formed between the electrical connector 224 and electrical connector 226 can be reversible or permanent. The configuration of the electrical connectors can vary based on the voltage, current, and number of desired electrical connections. For example, larger and more rugged electrical

connections can be used between the housings containing the capacitors to facilitate providing the voltage and current associated with a therapeutic shock to the patient.

[0131] FIG. 10C illustrates an example of an electrical connection that can be made between the flexible circuit 144, and defibrillator electrodes 140/202 or ECG electrodes 146/198. The electrical connection can include a conductive washer 230, exposed copper 231 on the flexible circuit 144, an electrode substrate 232, a silver base layer 233 of the defibrillator electrode 140/202, a conductive washer 234, and a conductive eyelet 235 contacting both washers 230/234. The conductive washer 230 is in direct electrical contact with the exposed copper 231 of the flexible circuit 144. The conductive washer 234 is in direct electrical contact with the silver base layer 233 of the defibrillator electrode 140/202. The conductive eyelet 235 forms a direct electrical contact between the conductive washers 230/234. The electrical connection illustrated in FIG. 10C can improve the current/voltage load between the capacitors 156/158 and the defibrillator electrodes 140/202.

[0132] FIG. 11A-11B illustrate electrode configurations that can be used in embodiments of the wearable defibrillators described herein. FIG. 11A illustrates a portion of an electrode. The electrode can include a PET substrate 240, a silver base layer 241, carbon intermediate layer 242, and silver/silver chloride layer 243. The electrode construction can include an electrode termination to the silver base layer 244. FIG. 11B is a different view of a portion of an electrode construction. The electrode construction includes a silver base layer 241, silver/silver chloride layer 243, and copper flex line 245.

[0133] FIG. 12 illustrates an example of anatomical locations for sensing electrodes. The wearable defibrillators described herein can include sensing electrodes configured to contact the anatomical locations illustrated in FIG. 12.

[0134] FIG. 13 illustrates a schematic flow chart 280 for how the wearable defibrillators described herein can be used by the patient. Sensors on the device, such as ECG, accelerometer, microphone, temperature, oxygen sensor like a pulse oximeter, magnetometer, impedance, and buttons can extract a plurality of patient parameters. Examples of the plurality of patient parameters include: heart rate, heart rate variability, ECG morphology, ECG spectral content, ECG complexity, posture, activity, heart sounds, breath sounds, voice commands, blood perfusion, oxygen saturation perfusion, presence in EMI environments, patient volitional movement, patient consciousness, fluid volume, body water content, and electrode skin adhesion. The controller can analyze the extracted parameters to determine if a treatment is necessary. Examples of state classifiers that can be determined by the device and controller include: cardiopulmonary state and device state. The determination of the cardiopulmonary state can include determination of: pulse present/absent, cardiac rhythm (e.g., VF), patient consciousness, pulmonary fluid volume, ejection fraction, cardiac function, respiratory rate, and respiratory function. Examples of the device state that can be determined include a device error, electrode failure, electrode migration, and therapy readiness. The controller can analyze the extracted parameters to determine if a notification action is necessary, such as a report to the physician or other healthcare provider or a report to a patient. The controller can further analyze the extracted parameters to determine if a therapeutic action is necessary, such as a shock delivery or patient alert (auditory, visual, tactile). Other examples of actions

include adjusting the device settings, providing error messages, and sending instructions to the user.

Adjusting the device settings can be done automatically, such as changing an ECG sensor.

[0135] FIG. 14 illustrates a method 300 of monitoring and defibrillating a patient's heart in accordance with some embodiments. The method 300 includes adhering to a first skin surface portion of the patient a first patient engagement substrate comprising a first plurality of sensing electrodes and a first defibrillator electrode pad, the first defibrillator electrode pad in electrical communication with an electrical energy source sufficient to provide a defibrillating shock, the first patient engagement substrate part of a wearable defibrillator comprising a fluid transport element configured to transport fluid away from the first skin surface portion of the patient to allow the wearable external defibrillator to be worn continuously 302; adhering to a second skin surface portion of the patient a second patient engagement substrate comprising a sensing electrode and a second defibrillator electrode pad, the second defibrillator electrode pad in electrical communication with the electrical energy source sufficient to provide the defibrillating shock, the second patient engagement substrate part of the wearable defibrillator, the wearable defibrillator including one or more sensors adapted to detect one or more of the pulse, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient 304; measuring patient data corresponding to a cardiac signal of the patient with the first plurality of sensing electrodes, the sensing electrode of the second patient engagement substrate, and/or the sensors of the wearable defibrillator 306; and analyzing the patient data to determine if the patient has an arrhythmia 308.

[0136] The methods can further include upon detection of an arrhythmia detecting one or more of the pulse, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient using one or more sensors on the wearable defibrillator and analyzing the detected one or more of the pulse, oxygen content of the blood, breathing rate, heart sounds, and heart rate of the patient to confirm the presence or absence of the arrhythmia. The methods described herein can include delivering an electrical shock after determining that the patient has an arrhythmia. The use of analyzing additional patient data in addition to the electrical data like the ECG of the patient can further confirm the absence or presence of a treatable arrhythmia. The increased confidence that the patient has a treatable arrhythmia prior to delivering a therapeutic shock reduces the likelihood of a false positive.

[0137] The methods described herein can include sensing impedance changes along a plurality of vectors of the patient with the one or more sensing electrodes of the first patient engagement substrate and the sensing electrode of the second patient engagement substrate and the first and second defibrillator electrode pads. A combination of the ECG sensing electrodes and signals recorded by the defibrillator electrode pads can be analyzed.

[0138] The impedance changes can be compared to a patient baseline and/or a database to measure a cardiac health of the patient.

[0139] The methods described herein can include measuring electrical data corresponding to a cardiac signal of the patient with the first plurality of sensing electrodes and the sensing electrode of the second patient engagement substrate.

[0140] Any of the sensors of the wearable defibrillator can be used to measure and analyze 5 characteristics associated with the health of the patient. The methods described herein can include detecting one or more of the breathing rate, heart sounds, and heart rate of the patient with a microphone on the wearable defibrillator.

[0141] The methods described herein can include recording patient movement with an accelerometer integrated with the wearable defibrillator upon detection of an arrhythmia and analyzing the recorded 10 patient movement to confirm the presence or absence of the arrhythmia. Utilizing additional data measured using the sensors on the wearable defibrillator can reduce the likelihood of a false positive determination of a treatable arrhythmia.

[0142] The methods described herein can include detecting the oxygen content of the blood with a pulse oximeter on the wearable defibrillator. Detecting the oxygen content of the blood with a pulse 15 oximeter on the wearable defibrillator can include measuring the oxygen content of the blood of the patient at a point on a chest of the patient.

[0143] The methods described herein can include measuring a transthoracic impedance (TTI). The transthoracic impedance can be measured using any of the conductive parts of the wearable defibrillator, including the upper patient engagement ECG sensing electrode, the upper patient engagement 20 defibrillator electrode pad, the lower patient engagement ECG electrodes, and the lower patient engagement defibrillator electrode pad. In some embodiments the transthoracic impedance can be measured between the first defibrillator electrode pad and the second defibrillator electrode pad. In some embodiments the transthoracic impedance can be measured simultaneously between multiple different sensing electrodes and defibrillator electrode pads.

[0144] The transthoracic impedance can provide information on the impedance of the body, the 25 electrode-skin interface between the upper patch and the skin and the lower patch and the skin, and the electrode patch itself. The transthoracic impedance frequency can be used to measure specific impedances. The body can be modeled as mostly resistive. The electrode-skin interface can be modeled as a resistor and a capacitor in parallel. The electrode patch can be modeled as mostly resistive. At higher measurement frequencies, the resistance across the capacitive component of the electrode-skin interface 30 can be minimized to get a clearer picture of the true body TTI. At lower frequencies, the capacitive component of the electrode-skin interface starts to dominate and you get a clearer picture of the TTI for the contact area of the electrode on the skin. A high-frequency TTI measurement (~32kHz) can provide data about the power level to use for the therapeutic electrical shock. The lower frequency measurement 35 (~8kHz and lower) can provide information about how well the patch is contacting the skin, especially with continuous or periodic monitoring and analyzing for changes from a baseline value. The methods described herein can include monitoring both high and low frequencies while the device is worn by the patient. The measurements can be made at certain intervals over the duration that the device is worn

by the patient. The TTI measurements can provide data that can be used to determine the total energy delivery for the specific patient based on the TTI of their body. The TTI measurements can be used to provide information as to the quality of the engagement between the skin and the patient engagement substrates. For example, if part of the patch is peeling off and the defibrillator electrode pad is in partial contact with the skin then the electrical energy delivered to the defibrillator electrode pad can be increased such that a sufficient amount of electrical energy is provided to the patient. If the TTI is below a threshold value that indicates a high level of peel-off for the patient engagement substrate then an alarm can be provided to the user that the contact between the patient engagement substrate and skin needs to be improved. Peel-off or poor contact between the patient engagement substrate (e.g., poor contact between the defibrillator electrode pad and the skin) and the skin can result in a smaller surface area to provide the electrical energy to the skin, which can result in more energy lost to the skin and also an increased risk of skin burning.

[0145] The methods described herein can include measuring an impedance between two separate electrodes making up the first or second defibrillator electrode pad. The methods described herein can include analyzing the impedance between the two separate electrodes of the first defibrillator electrode pad to determine whether the two separate electrodes of the first defibrillator electrode pad are in sufficient electrical contact with the skin to deliver an electrical shock. The methods described herein can include measuring an impedance between the two separate electrodes of the second defibrillator electrode pad. The methods described herein can include analyzing the impedance between the two separate electrodes of the second defibrillator electrode pad to determine whether the two separate electrodes of the second defibrillator electrode pad are in sufficient electrical contact with the skin to deliver an electrical shock.

[0146] The methods described herein can include analyzing the measured electrical data corresponding to the cardiac signal of the patient for bradycardia, atrial fibrillation, asystole, heart blocks, pauses, ventricular tachycardia, ventricular fibrillation, tachycardia with aberrancy, or a supraventricular tachycardia (SVT).

[0147] The methods can include continuously wearing the wearable defibrillator for greater than about 24 hours. The methods can include continuously wearing the wearable defibrillator for greater than about 5 days. The methods can include continuously wearing the wearable defibrillator for greater than about 7 days. The methods can include continuously wearing the wearable defibrillator for greater than about 10 days. The methods can include continuously wearing the wearable defibrillator for greater than about 14 days.

[0148] The devices described herein can be used to monitor a patient for symptoms associated with heart failure or monitoring the cardiac health of the patient. In some embodiments the wearable defibrillators can be modified to be adapted to monitor a patient for heart failure and/or to determine a cardiac health of the patient. For example a single patient engagement substrate can be used in the heart failure monitoring device. The capacitors can be omitted in the heart failure monitoring device. The controller and energy source can be adapted to power and process the sensors used to detect the

symptoms associated with heart failure. In some embodiments a wearable device for treating a patient to monitor for symptoms associated with heart failure are provided. The wearable devices can include a patient engagement substrate comprising an adhesive, one or more sensors, a first fluid transport element configured to transport fluid away from the skin to allow the wearable device to be worn continuously, and a first vapor permeable layer, the one or more sensors adapted to detect one or more of a pulse, a cardiac signal, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient; and a controller configured to receive data collected by the one or more sensors and analyze the data to determine if the patient exhibits a symptom associated with heart failure.

5 [0149] The wearable device can be adapted to perform any of the heart failure monitoring methods described herein. The wearable devices can be configured to provide a stimulus to the patient upon detection of a symptom associated with heart failure. Examples of the stimulus include a vibration, an electrical shock, a visual alert, electronic notification, or auditory alarm. Any of the sensors described herein can be used with the device to detect the symptoms associated with heart failure in the patient wearing the device. Examples of the one or more sensors include one or more of: accelerometer, ECG sensing electrodes, pulse oximeter, microphone, magnetometer, impedance sensors, and galvanic skin impedance sensor. The controller can be configured to apply an algorithm to the data collected by the one or more sensors. The controller can be configured to apply an algorithm to the data collected by the one or more sensors. In some embodiments the algorithm adapts to the specific patient wearing the device.

10 15 [0150] The controller can be adapted to modify the frequency of the sampling of the sensor data to efficiently receive and analyze the collected data. The controller can be adapted to selectively turn sensors on and off based on the relevant data collected with each sensor for the specific heart failure symptoms and the specific patient characteristics. The controller can be adapted to change the sensitivity of each of the sensors for the specific heart failure symptoms and the specific patient characteristics. The one or more sensors can be onboard the device or part of the patient engagement substrate or separate from the patient engagement substrate. For example, a wireless sensor can transmit data wirelessly to the device or a wired sensor can transmit data via a wired connection to the device. The wearable device can be adapted to transmit data wirelessly over a computer network to communicate with or provide information via a companion smart phone application.

20 25 [0150] FIG. 15B illustrates a schematic 326 of how the devices described herein can be used to detect symptoms associated with heart failure or to measure the cardiac health of the patient. The device can obtain data from the patient from sensors on board the device or in communication with the device. The sensors can be placed at different locations, can include different sensors, and a combination of different sensors. The device can modify the sampling frequency of any of the sensors. The sampling frequency can be fixed or can be variable. The device controller can process the collected data using a fixed algorithm or an adaptive algorithm. The adaptive algorithm can adapt to the specific patient using the device. The adaptive algorithm can analyze and make changes in the sensors, changes in the frequency/timing of the sampling, changes in the sensitivity of the sensors, and changes to the algorithm

30 35

features. If the device detects a symptom associated with a cardiac health of the patient or other data of interest the device can provide an intervention to the patient. Examples of interventions include a vibration alert, a shock, an auditory alert, and a visual alert. Visual alerts can be provided through the device or as part of a hand held computer application like a smartphone application or tablet computer application. The alerts can be provided directly to the patient, a healthcare provider, family member, or other person based on the user preferences or severity of the detected medical issue.

5 [0151] FIG. 15A is a flow chart of a method 320 of monitoring a patient's heart to detect a symptom or indication of cardiac disease in the patient in accordance with some embodiments. The method 320 includes measuring one or more of a heart rate, a breathing rate, a breathing pattern of the patient, an 10 impedance across and through a chest and thoracic cavity of the patient, and a size of blood vessels within a body of the patient like an inferior vena cava, blood pressure waveform, lung sounds, patient posture and activity, and pulse oxygenation with a wearable device including one or more sensing electrodes and one or more sensors configured to measure the heart rate, breathing rate and pattern of the patient, the 15 trans-thoracic impedance of the patient, and the size of the blood vessels in the body, blood pressure, wherein the wearable device is adhesively attached to a portion of the skin of the patient 322; analyzing the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG 20 amplitude, chest movement, breathing rate, breathing pattern, trans-thoracic impedance, blood pressure and blood pressure waveform in different body postures, and size of the blood vessels in the body to detect a symptom or indication of cardiac disease in the patient 324.

20 [0152] In some embodiments the methods include upon detection of the symptom or indication of heart failure in the patient, generating and providing a stimulus to the patient. Examples of the stimulus include one or more of: an electrical shock, a vibration, or an auditory alerts to the patient or physician.

25 [0153] The method can include upon detection of the symptom or indication of heart failure in the patient, saving a patient data to memory for later analysis or wirelessly transmitting the patient data to a computer for analysis.

30 [0154] The measurements being used to detect the symptom or indication of cardiac disease can include cardiac arrest and myocardial infarction. The measurements being used to detect the symptom or indication of cardiac disease can include heart failure, cardiomyopathies, heart blocks, atrial and ventricular arrhythmias.

35 [0155] Pulmonary edema can be determined using chest impedance by measuring multiple vectors across the chest from various ECG sensors and leads which allows assessment of fluid status in multiple different segments of the thoracic cavity.

[0156] The methods can further include analyzing the heart sounds measured by a microphone to determine the presence or absence of one or more of: rales or rhonchi, the presence of S3 and S4 heart sounds, and pathologies such as splitting in the S1 and S2 heart sounds.

35 [0157] The methods can also include analyzing the one or more of the measured parameters to determine a derived parameter for the patient for one or more of: ejection fraction, cyanosis, pulse quality, dyspnea, orthopnea, peripheral or pulmonary edema, right heart failure, left heart failure, nocturia, and

cardiac arrhythmias, pulsus alternans, S3 cardiac sound, S4 cardiac sound, and splitting in S1 and S2 heart sounds. Examples of the derived parameters include pulmonary edema, ejection fraction, cyanosis, pulse quality, dyspnea, orthopnea, or nocturia. The ejection fraction can be determined using ultrasound and localized impedance changes to determine trending information of blood flow over time as a proxy for ejection fraction. Cyanosis can be determined using pulse oxygenation and impedance status to determine changes in blood oxygenation. Pulse quality can be determined using Doppler ultrasound delivered and measured by the wearable device together with closely spaced impedance sensors to determine changes in the shape of the pulse wave to indicate changes in cardiac function, including pulsus alternans. Dyspnea can be determined using a combination of accelerometer to determine patient posture and pulse oxygenation with impedance to determine the breathing pattern including accounting for recent activity of the patient to determine whether dyspnea is at rest. Dyspnea can be determined using a combination of accelerometer to determine patient posture and pulse oxygenation with impedance to determine the breathing pattern including accounting for recent activity of the patient to determine whether dyspnea is at rest. Orthopnea is determined using ultrasound to determine blood pressure together with accelerometer to determine patient posture can give an estimate of orthostasis. Nocturia can be determined using number of times the patient gets up during sleep as a proxy for nocturia.

[0158] FIG. 16 is a flow chart of a method 340 of refurbishing a wearable defibrillator in accordance with some embodiments. The wearable defibrillator that is refurbished can be any of the wearable defibrillators described herein. FIG. 16 shows a method 340 for refurbishing a wearable defibrillator that includes: receiving a wearable defibrillator comprising an energy source, a controller, and a memory containing a patient data set collected while the wearable defibrillator was worn by a patient 342; copying the patient data set from the memory to a computer network or system external to the wearable defibrillator 344; erasing the patient data set from the memory of the wearable defibrillator 346; recharging or replacing the energy source of the wearable defibrillator 348; and running a diagnostic test on the wearable defibrillator after erasing the patient data set and recharging or replacing the energy source 350. FIGS. 17-20 illustrates examples of refurbishing methods for the wearable defibrillators described herein. At a high level the refurbishment includes receiving data from the wearable defibrillator and refurbishing the electronics and any other expensive parts. Re-using the refurbished expensive components of the device can help lower the overall device cost. The more expensive device components typically include the electronics, such as the controller/processor, memory, capacitors, and energy source. The energy source can be replaced or recharged in the refurbished wearable defibrillator. After the electronics are refurbished the electronics can be used in a refurbished wearable defibrillator. New patient engagement substrates can be used in the refurbished wearable defibrillators.

[0159] In some embodiments the wearable defibrillator includes one or more modules containing the one or more capacitors, energy source, and controller. The refurbishment methods described herein can include replacing the energy source by replacing the module containing the energy source. Additional examples of refurbishment of the energy source include replacing the battery or recharging a rechargeable battery.

[0160] The diagnostic test can include testing the one or more capacitors, memory, energy source, and controller.

[0161] In some embodiments the refurbishment methods include refurbishing a wearable defibrillator that includes one or more housings containing one or more of the controller, memory, 5 capacitors, and energy source. The controller and memory can be included in a first controller housing. The energy source can be included in a first energy source housing. The capacitors can be included in a first capacitor housing and a second capacitor housing. The refurbishment methods can include removing the controller and memory from the first controller housing. The refurbishment methods can include removing the energy source from the first energy source housing. The refurbishment methods can include 10 removing the one or more capacitors from the first capacitor housing and the second capacitor housing. The diagnostic test can include testing the one or more capacitors, memory, energy source, and controller after removal from the one or more housings. After the electronics components have been removed from their respective housings they can be tested, refurbished, and placed in new housings.

[0162] The refurbishment methods can include engaging a data transfer cable with a connector in 15 electrical communication with the memory. The refurbishment methods can include after running the diagnostic test, placing the controller and memory in a second controller housing. The refurbishment methods can include after running the diagnostic test, placing the one or more capacitors in a new first capacitor housing and a new second capacitor housing. The refurbishment methods can include after running the diagnostic test, placing the energy source in a second energy source housing. The 20 refurbishment methods can include sealing the one or more housings to prevent water ingress. The refurbishment methods can include engaging the second controller housing, new first capacitor housing, new second capacitor housing, and second energy source housing with a patient engagement substrate to form a refurbished wearable defibrillator.

[0163] In some embodiments the wearable defibrillator can be configured to support the one or more 25 housings within a waterproof enclosure. The refurbishment methods can include removing the housing from the waterproof enclosure after receiving the wearable defibrillator. The refurbishment methods can include after running the diagnostic test, placing the housing within a second waterproof enclosure. The refurbishment methods can include engaging the housing with the second waterproof enclosure with a patient engagement substrate to form a refurbished wearable defibrillator.

[0164] The refurbishment methods can include engaging a data transfer cable with an exterior 30 connection of the one or more housings. Copying can include a wired data connection to transfer the patient data set between the memory and the computer network or system. Copying can also include a wireless data transfer between the memory and a computer network or system.

[0165] The refurbished wearable defibrillator can be refurbished to include any of the wearable 35 defibrillator configurations described herein. The refurbished one or more housings can be electrically connected to the flexible circuit, ECG sensing electrodes, and defibrillator electrode pads.

[0166] After refurbishment the refurbished wearable defibrillator can be packaged. After 40 refurbishment the refurbished wearable defibrillator can be sent or provided to a second patient. The data

collection and refurbishment steps described herein can be applied to the refurbished wearable defibrillator after it has been used by the second patient and returned. The methods can include receiving the refurbished wearable defibrillator containing a second patient data set collected while the refurbished wearable defibrillator was worn by the second patient. The methods can include copying the second

5 patient data sent from the memory to a computer network or system external to the refurbished wearable defibrillator and erasing the patient data set from the memory of the refurbished wearable defibrillator. These steps can be repeated each time the wearable defibrillator or refurbished wearable defibrillator is returned after use by the patient.

[0167] The electronics components used in the wearable defibrillator can be refurbished multiple 10 times. The one or more housings and associated electronics can be replaced or refurbished in the refurbished wearable defibrillator. In some embodiments the refurbishment methods include replacing or refurbishing the one or more housings and reusing the one or more capacitors five or more times. In some embodiments the refurbishment methods include replacing or refurbishing the one or more housings and reusing the one or more capacitors ten or more times. In some embodiments the refurbishment 15 methods include replacing or refurbishing the one or more housings and reusing the one or more capacitors fifteen or more times. In some embodiments the refurbishment methods include replacing or refurbishing the one or more housings and reusing the one or more capacitors twenty or more times.

[0168] The patient data set can include data from the patient continuously wearing the wearable defibrillator for greater than about 24 hours. The patient data set includes data from the patient 20 continuously wearing the wearable defibrillator for greater than about 5 days. The patient data set includes data from the patient continuously wearing the wearable defibrillator for greater than about 7 days. The patient data set includes data from the patient continuously wearing the wearable defibrillator for greater than about 10 days. The patient data set includes data from the patient continuously wearing the wearable defibrillator for greater than about 14 days.

25 [0169] The refurbishment process can vary based on the type of housings used to hold the electronics components. In some embodiments the electronics components can be removed from the housings and placed in new housings as part of the refurbishment process (see FIGS. 17A-17D). In some embodiments the housings including the electronics can be covered with the covers being replaced as part of the refurbishment process with the electronics components staying inside the housings.

30 [0170] FIGS. 17A-17D illustrate an example of a part of a refurbishment process. FIGS. 17A-17B show the upper shell 150 being disconnected from the lower shell 152 to provide access to the processor and memory 154 within the housing 106. The processor and memory 156 can then be removed from the housing 106 for further refurbishment. After the processor and memory 156 is tested and refurbished it can be placed in a new housing 106 and be used in a refurbished wearable defibrillator. FIGS. 17C-17D show the removal of the energy source 160 from the housing 106 after separating the upper shell 150 from the lower shell 152. The energy source 160 can be recharged or a portion, such as the battery, can be replaced. After the energy source 160 has been refurbished it can be placed in a new housing 106 and used in a refurbished wearable defibrillator.

[0171] FIG. 18 illustrates a schematic showing the refurbishment of a used wearable defibrillator. The used wearable defibrillator is processed to separate the housings 106 from the patient engagement substrate 104. The removed patient engagement substrate 104 can be disposed of and is not typically reused. FIG. 18 shows the electronics components (processor and memory 156, capacitors 156, 158, and energy source 160) removed from outer shell housings. The outer shell housings can be placed in the trash. The electronics components can each be processed and refurbished. The energy source, such as the battery can be recharged or replaced. The capacitors, memory, and processor can be each tested to verify that they still meet the desired specifications prior to reusing them. FIG. 18 illustrates the discrete electronics components as being part of individual enclosures for simplicity. The refurbishment process can include removing the electronics components from any enclosures as shown in FIGS. 17A-17D. The refurbished electronics components can be placed in new outer shells and attached to a new patient engagement substrate. After refurbishment the new refurbished wearable defibrillator is ready for use.

[0172] FIG. 19 shows a refurbishment process similar to FIG. 18 but with electronics components included in modules that are enclosed in removable covers. The electronics components in the modules are separated from the plurality of removable covers, refurbished, and placed in new removable covers and engaged with a new patient engagement substrate. FIG. 20 shows a refurbishment process similar to FIG. 19 but with a removable cover that covers the electronics components instead of a multiple removable covers covering each of the electronics components.

[0173] FIGS. 21-23 illustrate a cross-sectional view of portions of embodiments of wearable defibrillators. The illustrated housings 400 in FIGS. 21-23 include a flexible circuit within the housings in contrast to the wearable defibrillator 100 with the flexible circuit 144 within the patient engagement substrate 104. The housing 400 includes an upper shell 402 and lower shell 404 that define a plurality of enclosures containing the electronics components 406a-e. The electronics components 406a-e can be in electrical communication via a flexible circuit 408 containing printed circuit boards (PCBs) 410a-410e. The housing 400 can include a plurality of flexible joints 412. The upper shell 402 can form a seal 414 with the lower shell 404. FIG. 22 illustrates the use of ultrasonic welding to form the seal 414 between the upper shell 402 and the lower shell 404. FIG. 23 shows another view of the upper shell 402 separate from the lower shell 404 and the electronics section 416 defined by the electronics components 406a-e, flexible circuit 408, and PCBs 410a-410e. The wearable defibrillators illustrated in FIGS. 21-23 have a plurality of compartments with a flexible configuration that can bend to improve engagement with the wearer. The plurality of compartments can contain the electronics within the housing, such as the energy source, one or more capacitors, controllers, etc. The housing can contain a substrate with rigid printed circuit board (PCB) sections, flexible circuit sections, wires, and flexible housing joints.

[0174] FIG. 24A-24B illustrate examples of release liners 420, 422 that can be used with the patient engagement substrates 102/104 of the wearable defibrillators described herein. The release liner 420, 422 can be used to cover the conductive gels and adhesives on the surface of the patient engagement substrate 102/104 prior to placing the wearable defibrillator on the patient. The release liners 420, 422 can be removed sequentially during the placement process to improve the process for correctly placing the

patient engagement substrates and forming a good adhesion to the surface of the skin. The release liner 420 can be removed first followed by contacting the exposed adhesive and conductive gel with the skin of the patient followed by removing the release liner 422 and engaging the remaining portion of the adhesive and conductive gel with the skin of the patient.

5 [0175] FIG. 25 illustrates a wearable defibrillator 500 with an upper patch 502 having two sensor electrodes and a defibrillator electrode and a lower patch 504 having three sensor electrodes and a defibrillator electrode. The patient engagement substrate of the upper patch 502 and lower patch 504 includes the defibrillator electrode pads and the sensing electrodes. The lower patch 504 supports a housing 506 that includes a LED light indicator 508 to provide system feedback. The housing 506 includes buttons 510 that can be pushed by the user. The upper patch electrodes are connected to the electronics in the lower patch by conductive cabling 512. The lower patch 504 has a larger surface area than the upper patch 502 that can be used to spread the shear weight of the electronics module (e.g. battery, capacitors, and controller). The lower patch 504 is configured to follow the lower rib line of the wearer. The ECG sensors can be evenly spread across the vector. The housing 506 on the lower patch 10 15 20 25 30 35 40 45 50 55 60 65 70 75 80 85 90 95 100 105 110 115 120 125 130 135 140 145 150 155 160 165 170 175 180 185 190 195 200 205 210 215 220 225 230 235 240 245 250 255 260 265 270 275 280 285 290 295 300 305 310 315 320 325 330 335 340 345 350 355 360 365 370 375 380 385 390 395 400 405 410 415 420 425 430 435 440 445 450 455 460 465 470 475 480 485 490 495 500 505 510 515 520 525 530 535 540 545 550 555 560 565 570 575 580 585 590 595 600 605 610 615 620 625 630 635 640 645 650 655 660 665 670 675 680 685 690 695 700 705 710 715 720 725 730 735 740 745 750 755 760 765 770 775 780 785 790 795 800 805 810 815 820 825 830 835 840 845 850 855 860 865 870 875 880 885 890 895 900 905 910 915 920 925 930 935 940 945 950 955 960 965 970 975 980 985 990 995 1000 1005 1010 1015 1020 1025 1030 1035 1040 1045 1050 1055 1060 1065 1070 1075 1080 1085 1090 1095 1100 1105 1110 1115 1120 1125 1130 1135 1140 1145 1150 1155 1160 1165 1170 1175 1180 1185 1190 1195 1200 1205 1210 1215 1220 1225 1230 1235 1240 1245 1250 1255 1260 1265 1270 1275 1280 1285 1290 1295 1300 1305 1310 1315 1320 1325 1330 1335 1340 1345 1350 1355 1360 1365 1370 1375 1380 1385 1390 1395 1400 1405 1410 1415 1420 1425 1430 1435 1440 1445 1450 1455 1460 1465 1470 1475 1480 1485 1490 1495 1500 1505 1510 1515 1520 1525 1530 1535 1540 1545 1550 1555 1560 1565 1570 1575 1580 1585 1590 1595 1600 1605 1610 1615 1620 1625 1630 1635 1640 1645 1650 1655 1660 1665 1670 1675 1680 1685 1690 1695 1700 1705 1710 1715 1720 1725 1730 1735 1740 1745 1750 1755 1760 1765 1770 1775 1780 1785 1790 1795 1800 1805 1810 1815 1820 1825 1830 1835 1840 1845 1850 1855 1860 1865 1870 1875 1880 1885 1890 1895 1900 1905 1910 1915 1920 1925 1930 1935 1940 1945 1950 1955 1960 1965 1970 1975 1980 1985 1990 1995 2000 2005 2010 2015 2020 2025 2030 2035 2040 2045 2050 2055 2060 2065 2070 2075 2080 2085 2090 2095 2100 2105 2110 2115 2120 2125 2130 2135 2140 2145 2150 2155 2160 2165 2170 2175 2180 2185 2190 2195 2200 2205 2210 2215 2220 2225 2230 2235 2240 2245 2250 2255 2260 2265 2270 2275 2280 2285 2290 2295 2300 2305 2310 2315 2320 2325 2330 2335 2340 2345 2350 2355 2360 2365 2370 2375 2380 2385 2390 2395 2400 2405 2410 2415 2420 2425 2430 2435 2440 2445 2450 2455 2460 2465 2470 2475 2480 2485 2490 2495 2500 2505 2510 2515 2520 2525 2530 2535 2540 2545 2550 2555 2560 2565 2570 2575 2580 2585 2590 2595 2600 2605 2610 2615 2620 2625 2630 2635 2640 2645 2650 2655 2660 2665 2670 2675 2680 2685 2690 2695 2700 2705 2710 2715 2720 2725 2730 2735 2740 2745 2750 2755 2760 2765 2770 2775 2780 2785 2790 2795 2800 2805 2810 2815 2820 2825 2830 2835 2840 2845 2850 2855 2860 2865 2870 2875 2880 2885 2890 2895 2900 2905 2910 2915 2920 2925 2930 2935 2940 2945 2950 2955 2960 2965 2970 2975 2980 2985 2990 2995 3000 3005 3010 3015 3020 3025 3030 3035 3040 3045 3050 3055 3060 3065 3070 3075 3080 3085 3090 3095 3100 3105 3110 3115 3120 3125 3130 3135 3140 3145 3150 3155 3160 3165 3170 3175 3180 3185 3190 3195 3200 3205 3210 3215 3220 3225 3230 3235 3240 3245 3250 3255 3260 3265 3270 3275 3280 3285 3290 3295 3300 3305 3310 3315 3320 3325 3330 3335 3340 3345 3350 3355 3360 3365 3370 3375 3380 3385 3390 3395 3400 3405 3410 3415 3420 3425 3430 3435 3440 3445 3450 3455 3460 3465 3470 3475 3480 3485 3490 3495 3500 3505 3510 3515 3520 3525 3530 3535 3540 3545 3550 3555 3560 3565 3570 3575 3580 3585 3590 3595 3600 3605 3610 3615 3620 3625 3630 3635 3640 3645 3650 3655 3660 3665 3670 3675 3680 3685 3690 3695 3700 3705 3710 3715 3720 3725 3730 3735 3740 3745 3750 3755 3760 3765 3770 3775 3780 3785 3790 3795 3800 3805 3810 3815 3820 3825 3830 3835 3840 3845 3850 3855 3860 3865 3870 3875 3880 3885 3890 3895 3900 3905 3910 3915 3920 3925 3930 3935 3940 3945 3950 3955 3960 3965 3970 3975 3980 3985 3990 3995 4000 4005 4010 4015 4020 4025 4030 4035 4040 4045 4050 4055 4060 4065 4070 4075 4080 4085 4090 4095 4100 4105 4110 4115 4120 4125 4130 4135 4140 4145 4150 4155 4160 4165 4170 4175 4180 4185 4190 4195 4200 4205 4210 4215 4220 4225 4230 4235 4240 4245 4250 4255 4260 4265 4270 4275 4280 4285 4290 4295 4300 4305 4310 4315 4320 4325 4330 4335 4340 4345 4350 4355 4360 4365 4370 4375 4380 4385 4390 4395 4400 4405 4410 4415 4420 4425 4430 4435 4440 4445 4450 4455 4460 4465 4470 4475 4480 4485 4490 4495 4500 4505 4510 4515 4520 4525 4530 4535 4540 4545 4550 4555 4560 4565 4570 4575 4580 4585 4590 4595 4600 4605 4610 4615 4620 4625 4630 4635 4640 4645 4650 4655 4660 4665 4670 4675 4680 4685 4690 4695 4700 4705 4710 4715 4720 4725 4730 4735 4740 4745 4750 4755 4760 4765 4770 4775 4780 4785 4790 4795 4800 4805 4810 4815 4820 4825 4830 4835 4840 4845 4850 4855 4860 4865 4870 4875 4880 4885 4890 4895 4900 4905 4910 4915 4920 4925 4930 4935 4940 4945 4950 4955 4960 4965 4970 4975 4980 4985 4990 4995 5000 5005 5010 5015 5020 5025 5030 5035 5040 5045 5050 5055 5060 5065 5070 5075 5080 5085 5090 5095 5100 5105 5110 5115 5120 5125 5130 5135 5140 5145 5150 5155 5160 5165 5170 5175 5180 5185 5190 5195 5200 5205 5210 5215 5220 5225 5230 5235 5240 5245 5250 5255 5260 5265 5270 5275 5280 5285 5290 5295 5300 5305 5310 5315 5320 5325 5330 5335 5340 5345 5350 5355 5360 5365 5370 5375 5380 5385 5390 5395 5400 5405 5410 5415 5420 5425 5430 5435 5440 5445 5450 5455 5460 5465 5470 5475 5480 5485 5490 5495 5500 5505 5510 5515 5520 5525 5530 5535 5540 5545 5550 5555 5560 5565 5570 5575 5580 5585 5590 5595 5600 5605 5610 5615 5620 5625 5630 5635 5640 5645 5650 5655 5660 5665 5670 5675 5680 5685 5690 5695 5700 5705 5710 5715 5720 5725 5730 5735 5740 5745 5750 5755 5760 5765 5770 5775 5780 5785 5790 5795 5800 5805 5810 5815 5820 5825 5830 5835 5840 5845 5850 5855 5860 5865 5870 5875 5880 5885 5890 5895 5900 5905 5910 5915 5920 5925 5930 5935 5940 5945 5950 5955 5960 5965 5970 5975 5980 5985 5990 5995 6000 6005 6010 6015 6020 6025 6030 6035 6040 6045 6050 6055 6060 6065 6070 6075 6080 6085 6090 6095 6100 6105 6110 6115 6120 6125 6130 6135 6140 6145 6150 6155 6160 6165 6170 6175 6180 6185 6190 6195 6200 6205 6210 6215 6220 6225 6230 6235 6240 6245 6250 6255 6260 6265 6270 6275 6280 6285 6290 6295 6300 6305 6310 6315 6320 6325 6330 6335 6340 6345 6350 6355 6360 6365 6370 6375 6380 6385 6390 6395 6400 6405 6410 6415 6420 6425 6430 6435 6440 6445 6450 6455 6460 6465 6470 6475 6480 6485 6490 6495 6500 6505 6510 6515 6520 6525 6530 6535 6540 6545 6550 6555 6560 6565 6570 6575 6580 6585 6590 6595 6600 6605 6610 6615 6620 6625 6630 6635 6640 6645 6650 6655 6660 6665 6670 6675 6680 6685 6690 6695 6700 6705 6710 6715 6720 6725 6730 6735 6740 6745 6750 6755 6760 6765 6770 6775 6780 6785 6790 6795 6800 6805 6810 6815 6820 6825 6830 6835 6840 6845 6850 6855 6860 6865 6870 6875 6880 6885 6890 6895 6900 6905 6910 6915 6920 6925 6930 6935 6940 6945 6950 6955 6960 6965 6970 6975 6980 6985 6990 6995 7000 7005 7010 7015 7020 7025 7030 7035 7040 7045 7050 7055 7060 7065 7070 7075 7080 7085 7090 7095 7100 7105 7110 7115 7120 7125 7130 7135 7140 7145 7150 7155 7160 7165 7170 7175 7180 7185 7190 7195 7200 7205 7210 7215 7220 7225 7230 7235 7240 7245 7250 7255 7260 7265 7270 7275 7280 7285 7290 7295 7300 7305 7310 7315 7320 7325 7330 7335 7340 7345 7350 7355 7360 7365 7370 7375 7380 7385 7390 7395 7400 7405 7410 7415 7420 7425 7430 7435 7440 7445 7450 7455 7460 7465 7470 7475 7480 7485 7490 7495 7500 7505 7510 7515 7520 7525 7530 7535 7540 7545 7550 7555 7560 7565 7570 7575 7580 7585 7590 7595 7600 7605 7610 7615 7620 7625 7630 7635 7640 7645 7650 7655 7660 7665 7670 7675 7680 7685 7690 7695 7700 7705 7710 7715 7720 7725 7730 7735 7740 7745 7750 7755 7760 7765 7770 7775 7780 7785 7790 7795 7800 7805 7810 7815 7820 7825 7830 7835 7840 7845 7850 7855 7860 7865 7870 7875 7880 7885 7890 7895 7900 7905 7910 7915 7920 7925 7930 7935 7940 7945 7950 7955 7960 7965 7970 7975 7980 7985 7990 7995 8000 8005 8010 8015 8020 8025 8030 8035 8040 8045 8050 8055 8060 8065 8070 8075 8080 8085 8090 8095 8100 8105 8110 8115 8120 8125 8130 8135 8140 8145 8150 8155 8160 8165 8170 8175 8180 8185 8190 8195 8200 8205 8210 8215 8220 8225 8230 8235 8240 8245 8250 8255 8260 8265 8270 8275 8280 8285 8290 8295 8300 8305 8310 8315 8320 8325 8330 8335 8340 8345 8350 8355 8360 8365 8370 8375 8380 8385 8390 8395 8400 8405 8410 8415 8420 8425 8430 8435 8440 8445 8450 8455 8460 8465 8470 8475 8480 8485 8490 8495 8500 8505 8510 8515 8520 8525 8530 8535 8540 8545 8550 8555 8560 8565 8570 8575 8580 8585 8590 8595 8600 8605 8610 8615 8620 8625 8630 8635 8640 8645 8650 8655 8660 8665 8670 8675 8680 8685 8690 8695 8700 8705 8710 8715 8720 8725 8730 8735 8740 8745 8750 8755 8760 8765 8770 8775 8780 8785 8790 8795 8800 8805 8810 8815 8820 8825 8830 8835 8840 8845 8850 8855 8860 8865 8870 8875 8880 8885 8890 8895 8900 8905 8910 8915 8920 8925 8930 8935 8940 8945 8950 8955 8960 8965 8970 8975 8980 8985 8990 8995 9000 9005 9010 9015 9020 9025 9030 9035 9040 9045 9050 9055 9060 9065 9070 9075 9080 9085 9090 9095 9100 9105 9110 9115 9120 9125 9130 9135 9140 9145 9150 9155 9160 9165 9170 9175 9180 9185 9190 9195 9200 9205 9210 9215 9220 9225 9230 9235 9240 9245 9250 9255 9260 9265 9270 9275 9280 9285 9290 9295 9300 9305 9310 9315 9320 9325 9330 9335 9340 9345 9350 9355 9360 9365 9370 9375 9380 9385 9390 9395 9400 9405 9410 9415 9420 9425 9430 9435 9440 9445 9450 9455 9460 9465 9470 9475 9480 9485 9490 9495 9500 9505 9510 9515 9520 9525 9530 9535 9540 9545 9550 9555 9560 9565 9570 9575 9580 9585 9590 9595 9600 9605 9610 9615 9620 9625 9630 9635 9640 9645 9650 9655 9660 9665 9670 9675 9680 9685 9690 9695 9700 9705 9710 9715 9720 9725 9730 9735 9740 9745 9750 9755 9760 9765 9770 9775 9780 9785 9790 9795 9800 9805 9810 9815 9820 9825 9830 9835 9840 9845 9850 9855 9860 9865 9870 9875 9880 9885 9890 9895 9900 9905 9910 9915 9920 9925 9930 9935 9940 9945 9950 9955 9960 9965 9970 9975 9980 9985 9990 9995 9999 10000 10005 10010 10015 10020 10025 10030 10035 10040 10045 10050 10055 10060 10065 10070 10075 10080 10085 10090 10095 10099 10100 10101 10102 10103 10104 10105 10106 10107 10108 10109 10110 10111 10112 10113 10114 10115 10116 10117 10118 10119 10120 10121 10122 10123 10124 10125 10126 10127 10128 10129 10130 10131 10132 10133 10134 10135 10136 10137 10138 10139 10140 10141 10142 10143 10144 10145 10146 10147 10148 10149 10150 10151 10152 10153 10154 10155 10156 10157 10158 10159 10160 10161 10162 10163 10164 10165 10166 10167 10168 10169 10170 10171 10172 10173 10174 10175 10176 10177 10178 10179 10180 10181 10182 10183 10184 10185 10186 10187 10188 10189 10190 10191 10192 10193 10194 10195 10196 10197 10198 10199 10199 10200 10201 10202 10203 10204 10205 10206 10207 10208 10209 10210 10211 10212 10213 10214 10215 10216 10217 10218 10219 10220 10221 10222 10223 10224 10225 10226 10227 10228 10229 10230 10231 10232 10233 1

[0177] A wicking layer 614 can be in contact with the layer 608 containing one or more of the adhesive 610, hydrogel electrodes, sensor electrodes, and defibrillation pads 612. In some embodiments the wicking layer 614 is part of a fluid transport element. The wicking layer 614 can improve the diffusion of fluid, such as water liquid, vapor and moisture, from the skin across the layer (e.g. adhesive and electrodes) contacting the patient's skin. In addition to wicking fluid across the adhesive and electrodes the wicking layer can also diffuse fluids across a dominant surface area of the wicking layer. The wicking layer can have a flexible sheet-like structure that can conform to the desired surface morphology for the device and skin of the patient. The flexible sheet-like structure has a dominant surface area that is the surface area of the flat sheet surface of the layer. The dominant surface area can be either the side of the layer closer to the patient engagement / skin side of the layer or the side of the layer closer to the external housing side of the layer. Spreading the fluid out across the dominant surface area of the wicking layer can greatly improve the fluid transport properties of the device by spreading the fluid out over a larger surface area to improve evaporation and fluid transport across the outer housing. The improved fluid transport can increase the comfort for the user and increase the long term wearability of the device by, e.g., preventing skin perspiration from affecting the electrical contact between the sensing and defibrillation electrodes and the skin and from interfering with the adhesive properties of the adhesive. An absorbing section 616 or plurality of sections 616 can be used in conjunction with the wicking layer 614 to further improve the moisture transport between the skin and the device. In some embodiments the absorbing section can be part of the fluid transport element. The adhesive 610 used in the patient engagement substrate can also be perforated in some embodiments to further improve moisture transport across the adhesive layer. The perforated adhesive layer can be part of the fluid transport element.

[0178] A semi rigid base chassis 618 can be used to provide additional structural support for the heavier components of the device, such as the device electronics. The illustrated chassis can have the electronics module 620 or modules mounted to the chassis 618. The illustrated defibrillator mounts the electronics 620 to the chassis 618 using a mount frame 622. The electronics can be included within one or more waterproof housings within the device housing(s). The electronics can be connected to the sensor electrodes and defibrillator electrode pads using flexible conductive material that can be routed through the multi-layer structure in the device. Examples of materials that can be used for the semi-rigid chassis 618 include polyester, polyethylene, polystyrene, polyurethane, and vinyl.

[0179] The housing 602 can be flexible. In some embodiments the flexible housing can be used to hold the device together. The flexible housing can also be elastic. The housing can be resistant to impacts, tearing, dirt, chemicals, and bacteria. The outer surface of the housing can be low friction to reduce wear and decrease the likelihood of catching on clothing and objects. In some embodiments the outer surface of the housing is water resistant. In some embodiments the outer surface of the housing is hydrophobic. The housing can be waterproof to prevent water from entering the interior of the device through the housing. In some embodiments the housing can be permeable to air. Examples of materials that can be used for the housing include polyester or polyurethane based fabrics. The fabric can be

knitted, woven, or non-woven. In some embodiments the housing can be part of the fluid transport element.

[0180] The properties of the individual layers can be selected to achieve a wearable defibrillator with the desired mechanical, strength, flexibility, adhesive, electrical, and chemical properties.

5 **[0181]** FIG. 27 illustrates an embodiment of a portion 700 of a wearable defibrillator with a multi-layer construction. FIG. 29 shows discrete sections of the sensor electrode hydrogel 702, the defibrillator electrode hydrogel 704, and the adhesive 706 having complementary shapes such that the sensor electrode hydrogel 702, defibrillator electrode hydrogel 704, and adhesive 706 can be combined and arranged in one substrate having a substantially planar layer or shape such that each of the sensing electrodes, 10 defibrillator electrode pad, and adhesive can conform to the skin of the patient. The patient engagement substrate includes the sensor electrode hydrogel 702, defibrillator electrode hydrogel 704, and adhesive 706 and is configured to contact the patient's skin and be suitable for long term wear. The sensor electrode hydrogel 702 can be arranged in multiple discrete electrodes to sense or acquire a cardiac signal 15 at different contact points. The defibrillator electrode hydrogel 704 has a larger surface area to provide sufficient contact with the skin while delivering a defibrillating energy pulse. The adhesive 706 can be a high-tack breathable adhesive. In some embodiments the adhesive 706 can be a gel that is perforated as shown in FIG. 29 to improve the breathability and/or moisture transport properties of the adhesive. The hydrogels used for the defibrillator electrode pad 704 and sensing electrodes 702 can also have adhesive properties to improve electrical contract with the skin and to provide additional structural support for the 20 device.

25 **[0182]** The adhesive can be selected to support the weight of the wearable defibrillator through activities for a duration of 10-14 days. The adhesive can also be selected for moisture management, to be comfortable and non-irritating, and to be easy to remove. In some embodiments multiple different types of adhesives can be used. Examples of adhesive types that can be used include hydrocolloid, silicone, acrylic, polyolefin, etc. Hydrocolloid adhesive typically have high strength but can be more difficult to remove. Silicone has good strength and can be removed more easily. Perforated silicone in combination with a wicking layer can achieve excellent moisture transport properties while maintaining adhesion to the skin.

30 **[0183]** A conductive electrode film 708 is illustrated. The conductive electrode film 708 can be in electrical communication with one or more of the sensing electrodes 702 and defibrillator electrode hydrogel 704. In some embodiments the conductive electrode film 708 can be laminated to the support structure, such as a polyester (PET) chassis 710, to form a flex circuit. In some embodiments the additional sensors described herein can also be manufactured within the flex circuit for easier manufacturing. A support structure 710 is illustrated in FIG. 29. The support structure 710 can be used 35 to support the device electronics and spread the shear load of the device across the footprint of the device. The support structure 710 can be semi-rigid to provide support for the electronics and to improve weight distribution. A moisture transport material 712 can be used to improve moisture transport from the electrode and adhesive side of the device towards the exterior of the device. The moisture transport

material 712 can be a wicking fabric. Examples of wicking materials include materials such as cotton, polyester, and non-woven constructions. The moisture transport layer can pull moisture from the skin through the adhesive and hydrogels. In some embodiments the moisture or fluid transport layer has an absorption capacity of greater than about 500%. In some embodiments the fluid transport or wicking layer is a non-woven fabric that is a mixture of polyester and cellulose. In some embodiments the ratio of cellulose to polyester can be from about 45/55 to 65/35 with a basis weight from 30-120 g/m². In one example the layer is a 50/50 mixture of cellulose and polyester with a basis weight of 70 g/m² and has an absorption capacity of about 850%.

5 [0184] An outer housing material 714 is illustrated. The outer housing material 714 can be made out of a fabric, laminate, or other material or structure that is breathable and has some water resistance. The outer housing material 714 can be flexible and abrasion resistant to reduce friction between the outer housing material and clothing. Examples of outer housing materials 714 include nonwoven fabrics, laminate structures, and laminate fabric structures. In some embodiments a non-woven polyurethane fabric material can be used as the outer housing. Laminate structures can include an outer layer, 10 membrane layer, and inner layer. The outer layer, membrane layer, and inner layer materials can be selected to provide a breathable laminate structure with a hydrophobic outer surface to provide water resistance. In some embodiments the outer housing material is water resistant. In some embodiments the outer housing material is hydrophobic. In some embodiments the outer housing material is waterproof.

15 [0185] An outer adhesive border 716 is illustrated. The adhesive border 716 is configured to connect to the perimeter of the device and to adhesively engage with the skin to improve adhesion between the portion of the wearable defibrillator and the patient's skin. The adhesive border 716 can be made out of a thin and flexible non-woven polyurethane with a high-tack adhesive. The adhesive border 716 can form a substantially waterproof seal between the perimeter of the device and the patient's skin to prevent water from passing from the exterior of the device to the area between the electrodes and the patient's skin. The 20 adhesive border 716 can have a tapered cross section.

25 [0186] The wearable defibrillators described herein can include additional sensors. Examples of sensors include: a voice recognition module, an ultrasound transceiver or transducer configured to transmit and/or receive ultrasonic signals, a Doppler radar configured to transmit a microwave signal and receive a returned microwave signal, a pulse oximeter configured to measure an oxygen content of a 30 blood of the patient at a point on a chest of the patient, an inclinometer configured to determine the position and orientation of the wearable defibrillator, a radio beacon configured to transmit the location of the wearable defibrillator, a GPS sensor, a wireless radio configured to wirelessly transmit data from the wearable defibrillator, and a sensor configured to measure a mechanical stretch of a portion of the wearable defibrillator. In some embodiments an accelerometer, such as a 1g accelerometer, can be used 35 with the wearable defibrillator to indicate the rotation of the device in one to three axes of rotation. The orientation can be useful during device application to indicate whether the device is right side up and whether it is tilted at an appropriate or inappropriate angle.

[0187] FIG. 28 is a portion of a wearable defibrillator in accordance with some embodiments. FIG. 28 illustrates a housing 500 contained within a sealed enclosure 502. The exterior of the housing can be water resistant. The sealed enclosure 502 can also be water resistant or water proof to prevent moisture or other fluids from contacting the housing 500. The illustrated housing 500 has a connector plug receptacle 504 configured to engage with a connector 506 embedded with the sealed enclosure 502. The connector 506 can engage with a connector 508 that is part of the flex circuit 510 of the patient engagement substrate. The connector plug 504 / connector 506 / connector 508 can include a plurality of electrical connections that can allow for electrical communication between the housing and the electrodes and sensors that are engaged with the wearable defibrillator. For example, the connector plug can include 10 connections corresponding to the defibrillator electrode pads, the plurality of sensing electrodes, and any additional sensors. FIG. 29 is an enlarged view of the connector plugs 504, 506, 508. The connector 506 and connectors 504/508 include complementary surfaces for ECG sensing electrode electrical connections 512 and for the defibrillator electrical connection 514. The flexible circuit 510 also includes a plurality of rivets 516 for the electrical connections from the connectors 504, 506, and 508 and the flexible circuit 15 510.

[0188] The use of the sealed enclosure can make it easier to download data from the housing and refurbish the housing for subsequent use with another patient engagement substrate. Refurbishing the housing can include one or more of the following steps: 1) receiving the device after use; 2) cutting through the sealed enclosure/waterproof skin to expose the housing; 3) removing the housing (containing 20 batteries, caps, electronics, memory) from the disposable patch (patient engagement structure); 4) the housing may not get opened, except (potentially) for a battery compartment to replace/recharge batteries; 5) batteries could also be charged through a sealed connector on housing (i.e. don't have to open housing at all); 6) plugging into the housing to extract data from the memory; 7) copying data to an external 25 system; 8) erasing memory on the device; 9) recharging or replacing the battery; 10) running a functional test / diagnostics; 11) reprogramming; and 12) sealing the housing with a new sealed enclosure / waterproof skin and adding to a new patient engagement structure to create a new device for use by the next patient/wearer.

[0189] FIG. 30 is a schematic illustration of an upper and lower patch that can be used with the 30 wearable defibrillators described herein. The illustrated lower patch can be used to support the housing as described herein and can include the universal connector/connector plug engaged with the housing.

[0190] FIG. 31 illustrates a battery charger and/or programmer cable 800 that can be used to engage with an exterior electrical contact 802 of the housing 804 to download data and/or charge the batteries within the housing. The electrical contact 802 can utilize a spring connector 806 to facilitate electrical contact with the PCB 808. FIG. 32 is a housing 804 showing the exposed electrical contacts 802 that can 35 be used to transmit data and/or receive an electrical charge.

[0191] FIG. 33 is cross-sectional view of a portion of a wearable defibrillator. FIG. 33 illustrates a device 8420 that can include an adhesive 8422, a bonding layer 8424 and a stretchable anchor 8426 to support the defibrillator components 8428 off of the body. The stretchable anchors 8426 can be used with

the bonding layer to allow relative movement between the adhesive 8422 and bottom of the more rigid defibrillator components 8428 to improve the overall flexibility of the device and to decrease the likelihood of the adhesive 8422 pulling off of the skin of the wearer during movement.

[0192] FIG. 34 illustrates a pair of electrodes 900, 902 that can be used in the wearable defibrillators described herein. The impedance between the pair of electrodes 900, 902 can be analyzed to determine the quality of the electrical contact between the electrodes and the skin of the patient. The pair of electrodes 900, 902 can make up one of the defibrillator electrode pads. In some cases a transthoracic impedance between the first pair of electrodes and a second pair of electrodes (e.g. second defibrillator electrode pad) can be determined.

[0193] FIG. 35 illustrates a cross-sectional view of a configuration of a defibrillator electrode 950 that can be used in the wearable defibrillators described herein. The illustrated electrode configuration 950 in FIG. 35 can be used for the defibrillator electrode pad. The illustrated electrode 950 includes a perforated electrode 952 engaged with a conductive adhesive/hydrogel 954 and an electrical connection that traces back to the housing. The electrode could be made of a carbon vinyl film. The carbon vinyl film could be with or without an Ag or Ag/AgCl coating on one or both sides. The electrode film could be solid or have perforations to allow moisture to move through. In some cases the electrode can have a woven structure that is air permeable. In one example the electrode is a woven carbon fabric. In some cases the electrode is a conductive hydrogel. The conductive hydrogel can be a cross-linked polymer with water and a salt to promote conductivity. In some cases a conductive hydrocolloid can be used. The conductive hydrocolloid can be a mixture of rubber, tackifier, absorber, and conductive filler. Examples of conductive fillers include: carbon nanotubes, graphite, carbon black, silver nanowires, and graphene sheets.

[0194] FIG. 36 illustrates a picture of microneedles and an electrode configuration with micro-needles 970 in accordance with some embodiments. In some embodiments any of the electrodes disclosed herein can include micro-needles. The micro-needles can be configured to penetrate the stratum corneum (SC) to deliver the electrical energy to the epidermis.

[0195] FIGS. 37A-37C illustrate embodiments of connections between a housing 1000 containing electronics components and patient engagement substrate 1002 that can be used in the embodiments of the wearable defibrillators disclosed herein. As shown in FIGS. 37A-37C a flexible connection 1004 can be used between the housing 1000 and patient engagement substrate 1002. The flexible connection 1004 can be used to support the weight of the housing 1000, such as the weight of the battery, capacitors, and energy source within the housing. The flexible connection can also include electrical interconnects between the housing and the one or more sensing electrodes, defibrillator electrode pads, and any other sensors or electrical components on the wearable defibrillator. The use of the flexible connection can allow the housing to articulate away from the body during movement to reduce the likelihood of the patient engagement substrate losing adhesion with the skin. FIG. 37A illustrates the housing 1000 supported by a flexible connector 1004 at one end of the housing. FIG. 37B illustrates the housing 1000 supported with a flexible hinge 1006 at one end of the housing 100 along with a connector 1008 running

along one surface of the housing. FIG. 37C illustrates a housing 1000 with a fabric covering 1010 that is supported by a flexible hinge 1012 and connector 1014. All three of the flexible connections illustrated in FIGS. 37A-37C include a plurality of electrical connections between the housing and the patient engagement substrate. The flexible connection can include a plug connection that can reversibly and removably connect the housing with the patient engagement substrate.

5 [0196] FIG. 38 is a schematic illustration of moisture transport across an embodiment of a conductive adhesive 1020 that can be used in the wearable defibrillators disclosed herein. FIG. 38 shows a conductive adhesive hydrogel 1020 that is hydrophobic but includes a hydrophilic structure. FIG. 38 illustrates a hydrophilic mesh/non-woven material 1022 within the hydrophobic bulk layer. The hydrophilic mesh/non-woven material 1022 provides a water transport mechanism to transport water from one side of the adhesive 1020 to the other side of the adhesive as shown in FIG. 38.

10 [0197] FIG. 39 is a schematic illustration of moisture transport across an embodiment of a conductive adhesive 1020 and electrode 1024 that can be used in the wearable defibrillators disclosed herein. FIG. 39 illustrates a conductive adhesive 1020, such as a hydrocolloid or hydrogel bulk material with a non-woven wicking material 1022 within the adhesive 1020. The conductive adhesive contacts an electrode layer 1024 having a plurality of openings. The electrode layer also contacts a non-woven wicking material 1028. The configuration illustrated in FIG. 39 can move moisture from the surface of the skin through the non-woven wicking material 1022 present in the conductive adhesive 1020 through the plurality of openings in the electrode layer 1024 and through the non-woven wicking material 1028. 15 The improved moisture transport can increase the long term wearability of the electrode and wearable defibrillators disclosed herein. The non-woven wicking material 1028 can include a hydrophilic fiber sewn through the thickness of the configuration shown in FIG. 39. The hydrophilic fiber can be sewn through at regular intervals or at certain points of the electrode. The hydrophilic fiber improves water transport and also improves the mechanical properties and adhesion between different layers of the 20 device.

25 [0198] FIG. 40 is a schematic illustration of a portion of a wearable defibrillator measuring a multi-vector trans-thoracic impedance of a patient in accordance with some embodiments. FIG. 40 illustrates the upper patch 102 and lower patch 104 of a wearable defibrillator. The sensing electrodes on each of the upper patch 102 and the lower patch 104 can measure a multi-vector trans-thoracic impedance 1050 of the patient 1052 as shown in FIG. 40. The multiple vectors create numerous pathways to assess the 30 impedance of the patient, which allows for sampling of various lung lobes 1054 on both the right and left side of the chest. Assessing different lobes can provide more accuracy regarding fluid states and also help with clarifying fluid changes due to patient position.

35 [0199] The devices described herein can be used to monitor a patient for symptoms associated with sleep apnea. In some embodiments the wearable defibrillators can be modified to be adapted to monitor a patient for sleep apnea. For example a single patient engagement substrate can be used in the sleep apnea monitoring device. The capacitors can be omitted in the sleep apnea monitoring device. The controller and energy source can be adapted to power and process the sensors used to detect the symptoms

associated with sleep apnea. In some embodiments a wearable device for treating a patient and detecting symptoms associated with sleep apnea are provided. The device can include a patient engagement substrate comprising an adhesive, one or more sensors, a first fluid transport element configured to transport fluid away from the skin to allow the wearable device to be worn continuously, and a first vapor permeable layer, the one or more sensors adapted to detect one or more of a pulse, a cardiac signal, oxygen content of the blood, impedance, galvanic skin impedance, temperature, breathing rate, heart sounds, and heart rate of the patient; and a controller configured to receive data collected by the one or more sensors and analyze the data to determine if the patient exhibits a symptom associated with sleep apnea. The wearable device can be configured to provide a stimulus to the patient upon detection of a symptom associated with sleep apnea. Examples of stimuli include a vibration, an electrical shock, a visual alert, electronic notification, or auditory alarm. Any of the sensors described herein can be used with the device to detect the symptoms associated with sleep apnea in the patient wearing the device. The controller can be configured to apply an algorithm to the data collected by the one or more sensors. In some embodiments the algorithm adapts to the specific patient wearing the device. The controller can be adapted to modify the frequency of the sampling of the sensor data to efficiently receive and analyze the collected data. The controller can be adapted to selectively turn sensors on and off based on the relevant data collected with each sensor for the specific sleep apnea symptoms and the specific patient characteristics. The controller can be adapted to change the sensitivity of each of the sensors for the specific sleep apnea symptoms and the specific patient characteristics. The one or more sensors can be onboard the device or part of the patient engagement substrate or separate from the patient engagement substrate. For example, a wireless sensor can transmit data wirelessly to the device or a wired sensor can transmit data via a wired connection to the device. The wearable device can be adapted to transmit data wirelessly over a computer network to communicate with or provide information via a companion smart phone application.

[0200] FIG. 41B illustrates a schematic of a method of detecting symptoms associated with sleep apnea in a patient 1110 using the devices described herein. The device can obtain data from the patient from sensors on board the device or in communication with the device. The sensors can be placed at different locations, can include different sensors, and a combination of different sensors. The device can modify the sampling frequency of any of the sensors. The sampling frequency can be fixed or can be variable. The device controller can process the collected data using a fixed algorithm or an adaptive algorithm. The adaptive algorithm can adapt to the specific patient using the device. The adaptive algorithm can analyze and make changes in the sensors, changes in the frequency/timing of the sampling, changes in the sensitivity of the sensors, and changes to the algorithm features. If the device detects a symptom associated with sleep apnea or other data of interest the device can provide an intervention to the patient. Examples of interventions include a vibration alert, a shock, an auditory alert, and a visual alert. Visual alerts can be provided through the device or as part of a hand held computer applications, such as a smartphone application or tablet computer application. The alerts can be provided directly to

the patient, a healthcare provider, family member, or other person based on the user preferences or severity of the detected medical issue.

[0201] In some embodiments the devices described herein can be adapted to monitor and treat sleep apnea in the wearer. FIG. 41A is a flow chart of a method 1100 for detecting symptoms associated with

5 sleep apnea in a patient in accordance with some embodiments. The method 1100 for treating sleep apnea includes measuring one or more of a heart rate, a breathing rate, and a breathing pattern of the patient with a wearable device including one or more sensing electrodes and a sensor configured to measure the breathing rate and pattern of the patient, the wearable device adhesively attached to a portion of the skin of the patient 1102; and analyzing the one or more of the measured heart rate, oxygen saturation, ECG 10 rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, and breathing pattern to detect a symptom or indication of sleep apnea in the patient 1104. In some embodiments the methods include upon detection of the symptom or indication of sleep apnea in the patient, generating and providing a stimulus to the patient. Examples of providing a stimulus include providing a vibration, electrical shock, or auditory alarm.

15 **[0202]** FIG. 42 is a flow chart illustrating a method 1120 of providing instructions for placing the wearable defibrillators described herein. The method 1120 for providing instructions for placing a wearable defibrillator on a patient includes: providing instructions on where to put a first patient engagement substrate of the wearable defibrillator on a torso of the patient, the first patient engagement substrate including one or more sensing electrodes, adhesive, and a first defibrillator electrode pad, the 20 instructions including where to put the one or more sensing electrodes and first defibrillator electrode pad on the chest of the patient 1122; providing instructions on where to put a second patient engagement substrate of the wearable defibrillator, the second patient engagement substrate including a sensing electrode, adhesive, and a second defibrillator electrode pad, the instructions including where to put the one or more sensing electrodes and second defibrillator electrode pad 1124; verifying a first patient 25 engagement substrate placement on the torso of the patient including the placement of the one or more sensing electrodes and first defibrillator electrode pad 1126; and verifying a second patient engagement substrate placement on the chest of the patient including the sensing electrode and second defibrillator electrode pad 1128.

[0203] Instructions can be provided to the patient or to a person applying the wearable defibrillator 30 to the patient. In one example the person applying the wearable defibrillator is a health care provider. Typically a health care provider will apply the wearable defibrillator the first time the patient uses the wearable defibrillator. Second and subsequent applications of the wearable defibrillator can be done by the patient, a health care provider, or person assisting the patient.

[0204] A variety of release liners can be used to cover the portions of the wearable defibrillator that 35 contact the skin of the patient. Instructions can also include instructions for removing release liners that cover portions of the patient engagement substrate such as the ECG sensing electrode gels, adhesive, and defibrillator electrode pad gels.

[0205] In one embodiment a first sensing electrode release liner is configured to cover the one or more sensing electrodes on the patient engagement substrate, a first defibrillator electrode pad release liner is configured to cover the first defibrillator electrode pad, and a first adhesive release liner configured to cover the adhesive on the first patient engagement substrate. In one embodiment a second 5 sensing electrode release liner is configured to cover the one or more sensing electrodes on the second patient engagement substrate and a second defibrillator electrode pad release liner is configured to cover the second defibrillator electrode pad, and a second adhesive release liner is configured to cover the adhesive on the second patient engagement substrate. The instructions can be provided to sequentially remove the first sensing electrode release liner, the first defibrillator electrode pad release liner, and the 10 first adhesive release liner. The instructions can be provided to sequentially remove the second sensing electrode release liner, the second defibrillator electrode pad release liner, and the second adhesive release liner.

[0206] In some embodiments two or more release liners are used to cover the surfaces of each of the patient engagement substrates. In one embodiment a primary patient engagement substrate release liner is 15 configured to cover a first portion of the patient engagement substrate; a secondary patient engagement substrate release liner is configured to cover a second portion of the patient engagement substrate; a primary second patient engagement substrate release liner is configured to cover a first portion of the second patient engagement substrate; and a secondary second patient engagement substrate release liner configured to cover a second portion of the second patient engagement substrate. The instructions can be 20 provided to sequentially remove the primary patient engagement substrate release liner, secondary patient engagement substrate release liner, primary second patient engagement substrate release liner, and secondary second patient engagement substrate release liner.

[0207] The methods can include providing instructions to shave, clip, trim, chemically remove, or otherwise depilate, and clean the skin of the patient.

[0208] The methods for providing instructions can include measuring data using any of the 25 electrodes and sensors provided on the wearable defibrillators described herein. For example, the methods can include measuring an impedance between the first and second defibrillator electrode pad. The methods can include measuring an impedance between a plurality of the one or more sensing electrodes. The methods can include analyzing the impedance between the first and second defibrillator electrode pad 30 and the impedance between a plurality of the one or more sensing electrodes to verifying the correct placement of the first patient engagement substrate and the second patient engagement substrate. The methods can include verifying placement of the wearable defibrillator by determining a location of a plurality of low power radios integrated with the wearable defibrillator.

[0209] In some embodiments the first defibrillator electrode pad can include a first pair of 35 electrodes. The controller can be configured to measure a first impedance between the first pair of electrodes. The controller can be configured to analyze the first impedance to determine whether the first pair of electrodes are in proper contact with the patient's skin.

[0210] In some embodiments the second defibrillator electrode pad includes a second pair of electrodes. The controller can be configured to measure a second impedance between the second pair of electrodes. The controller can be configured to analyze the second impedance to determine whether the second pair of electrodes are in proper contact with the patient's skin. The controller can be configured to 5 measure a transthoracic impedance between the first pair of electrodes and the second pair of electrodes.

[0211] In some embodiments the wearable defibrillator includes a slip layer disposed between the housing and adhesive configured to allow relative movement between the housing and the adhesive.

[0212] In one example the wearable defibrillator includes a first sealing layer enclosing the energy source, one or more capacitors, and controller. The first sealing layer can be within the housing. The first 10 sealing layer can contact the housing. In one example the wearable defibrillator includes a second sealing layer containing the housing.

[0213] In some embodiments the wearable defibrillator includes a first connection between the housing and the first patient engagement substrate and a second flexible connection between the housing and the first patient engagement substrate. The first connection can be on a first end of the first patient 15 engagement substrate and the second flexible connection can be on a second end of the first patient engagement substrate that opposes the first end of the first patient engagement substrate. The second flexible connection can allow for relative movement between the second end of the first patient engagement substrate and the housing.

[0214] In some embodiments the wearable defibrillator includes a first sensing electrode release liner 20 configured to cover the one or more sensing electrodes on the first patient engagement substrate and a first defibrillator electrode pad release liner configured to cover the defibrillator electrode pad. In some embodiments the wearable defibrillator includes a second sensing electrode release liner configured to cover the one or more sensing electrodes on the second patient engagement substrate and a second defibrillator electrode pad release liner configured to cover the second defibrillator electrode pad.

[0215] In some embodiments the wearable defibrillator housing is supported by two or more patient 25 engagement substrates.

[0216] In some embodiments the wearable defibrillator includes an electroactive polymer. The electroactive polymer can be configured to detect a change in a morphology of the first patient engagement substrate and/or second patient engagement substrate. The electroactive polymer can 30 be configured to vibrate. The electroactive polymer can be configured to deform to change the morphology of the first and/or second patient engagement substrate.

[0217] In some embodiments the wearable defibrillator housing is configured to receive a plurality of energy sources. The energy source can include a first modular battery and a second modular battery. The first and second modular batteries can be configured to be removably received within the housing.

[0218] In some embodiments the wearable defibrillator includes a flexible connection between the housing and the first patient engagement substrate configured to support the weight of the housing and components within the housing. The flexible connection can allow for relative movement between the housing and the first patient engagement substrate. The flexible connection can include one or more 35

electrical connections between the housing and the first patient engagement substrate. The flexible connection can include a removable and reversible connection.

[0219] In some embodiments the wearable defibrillator includes a cantilever coupled to the housing and the first patient engagement substrate.

5 **[0220]** In some embodiments the wearable defibrillator includes a first adhesive release liner configured to cover the adhesive on the first patient engagement substrate. In some embodiments the wearable defibrillator includes a second adhesive release liner configured to cover the adhesive on the second patient engagement substrate.

10 **[0221]** In some embodiments a fitting tool can be provided with the wearable devices described herein. The fitting tool can be part of a system with the wearable devices and can be used in methods for placing the wearable device on the patient. FIGS. 43A-43B illustrate a fitting tool 1200 that can be used to fit the wearable devices described herein to the patient in accordance with some embodiments. The fitting tool can be custom fit and sized to the individual patient. The measurements can be set and noted for future reference using a pre-defined system guide. The fitting tool 1200 can include an adjustable 15 upper/top patch arm brace 1202 and an adjustable shoulder strap 1204 for height alignment. The upper patch of the wearable device can be stored on the main fitting tool either on the shoulder strap or the belt 1206 while the patient positions and fastens the tool on the body. The upper patch fitting tool 1200 can be sized to fit the circumference of the shoulder/ armpit area of the specific patient. The height and angle of the patch in the tool can be set during an initial fitting process. The fitting tool 1200 can include a main 20 belt 1206 for lateral chest alignment of the wearable device. The fitting tool 1200 can include an adjustable buckle strap 1208. The belt 1206 can be adjustable and extendable to fit patients with a torso circumference (at xiphoid height) from about 27" up to about 56". The fitting tool 1200 can include an inner frame 1210 with a foam support for the wearable device. The inner frame 1210 can include a complementary surface to an outer portion of the surface of the wearable devices described herein, such 25 as the wearable defibrillators. The inner frame 1210 can engage with the wearable device to securely hold the outer portion of the surface of the wearable device with the complementary surface. The inner frame can include a foam pad with a complementary surface to the wearable device having an undercut edge such that the fitting tool and foam pad can interface with the housing modules with the undercut edge. In some instances the foam of the fitting tool 1200 can be removed from the frame to help simplify 30 loading the device from shipping package to the fitting tool 1200. The fitting tool 1200 can include an extended back belt brace 1212. The fitting tool 1200 can be used when the device is initially provided to the patient and placed on the patient. The fitting tool 1200 and any of the belt sections included in the fitting tool 1200 can be packaged in a compact and folded arrangement.

[0222] EXAMPLE 1:

35 **[0223]** The moisture vapor transmission rate (MVTR) were tested for various components and wearable defibrillator patient engagement substrates described herein. Adhesive conductive hydrogels were tested and had a MVTR rate of 4,000-5,000 g/m² per day. Vapor permeable fabric materials were tested and had MVTR of 3,500-3,600 g/m² per day.

[0224] Patient engagement substrates were tested that included: adhesive, conductive hydrogels, defibrillator electrode pad, wicking layer, flexible circuit, chassis support layer, and vapor permeable outer layers. The tested MVTR rates in g/m² per day were around 1,800-1,900 for the tested patient engagement substrates.

5 **[0225]** Other combinations of materials were also tested. In another example the MVTR was tested across a carbon vinyl defibrillator electrode layer with 0.16" diameter perforations, an acrylic defibrillator electrode adhesive, a non-woven wicking material layer, an acrylic chassis adhesive, a PVC chassis layer with a thickness of 16mil. The MVTR was 6,000 g/m² per day for this tested configuration.

10 **[0226]** In another example the MVTR was tested across a carbon vinyl defibrillator electrode layer with 0.085" diameter perforations, an acrylic defibrillator electrode adhesive, a non-woven wicking material layer, an acrylic chassis adhesive, a PVC chassis layer with a thickness of 16mil. The MVTR was 6,000 g/m² per day for this tested configuration.

15 **[0227]** When a feature or element is herein referred to as being "on" another feature or element, it can be directly on the other feature or element or intervening features and/or elements may also be present. In contrast, when a feature or element is referred to as being "directly on" another feature or element, there are no intervening features or elements present. It will also be understood that, when a feature or element is referred to as being "connected", "attached" or "coupled" to another feature or element, it can be directly connected, attached or coupled to the other feature or element or intervening features or elements may be present. In contrast, when a feature or element is referred to as being 20 "directly connected", "directly attached" or "directly coupled" to another feature or element, there are no intervening features or elements present. Although described or shown with respect to one embodiment, the features and elements so described or shown can apply to other embodiments. It will also be appreciated by those of skill in the art that references to a structure or feature that is disposed "adjacent" another feature may have portions that overlap or underlie the adjacent feature.

25 **[0228]** Terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. For example, as used herein, the singular forms "a", "an" and "the" are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms "comprises" and/or "comprising," when used in this specification, specify the presence of stated features, steps, operations, elements, and/or components, but 30 do not preclude the presence or addition of one or more other features, steps, operations, elements, components, and/or groups thereof. As used herein, the term "and/or" includes any and all combinations of one or more of the associated listed items and may be abbreviated as "/".

35 **[0229]** Spatially relative terms, such as "under", "below", "lower", "over", "upper" and the like, may be used herein for ease of description to describe one element or feature's relationship to another element(s) or feature(s) as illustrated in the figures. It will be understood that the spatially relative terms are intended to encompass different orientations of the device in use or operation in addition to the orientation depicted in the figures. For example, if a device in the figures is inverted, elements described as "under" or "beneath" other elements or features would then be oriented "over" the other elements or

features. Thus, the exemplary term "under" can encompass both an orientation of over and under. The device may be otherwise oriented (rotated 90 degrees or at other orientations) and the spatially relative descriptors used herein interpreted accordingly. Similarly, the terms "upwardly", "downwardly", "vertical", "horizontal" and the like are used herein for the purpose of explanation only unless specifically indicated otherwise.

5 [0230] Although the terms "first" and "second" may be used herein to describe various features/elements, these features/elements should not be limited by these terms, unless the context indicates otherwise. These terms may be used to distinguish one feature/element from another feature/element. Thus, a first feature/element discussed below could be termed a second feature/element, 10 and similarly, a second feature/element discussed below could be termed a first feature/element without departing from the teachings of the present invention.

10 [0231] As used herein in the specification and claims, including as used in the examples and unless otherwise expressly specified, all numbers may be read as if prefaced by the word "about" or "approximately," even if the term does not expressly appear. The phrase "about" or "approximately" may 15 be used when describing magnitude and/or position to indicate that the value and/or position described is within a reasonable expected range of values and/or positions. For example, a numeric value may have a value that is +/- 0.1% of the stated value (or range of values), +/- 1% of the stated value (or range of values), +/- 2% of the stated value (or range of values), +/- 5% of the stated value (or range of values), +/- 10% of the stated value (or range of values), etc. Any numerical range recited herein is intended to 20 include all sub-ranges subsumed therein.

20 [0232] Although various illustrative embodiments are described above, any of a number of changes may be made to various embodiments without departing from the scope of the invention as described by the claims. For example, the order in which various described method steps are performed may often be changed in alternative embodiments, and in other alternative embodiments one or more method steps may 25 be skipped altogether. Optional features of various device and system embodiments may be included in some embodiments and not in others. Therefore, the foregoing description is provided primarily for exemplary purposes and should not be interpreted to limit the scope of the invention as it is set forth in the claims.

30 [0233] The examples and illustrations included herein show, by way of illustration and not of limitation, specific embodiments in which the subject matter may be practiced. As mentioned, other embodiments may be utilized and derived there from, such that structural and logical substitutions and changes may be made without departing from the scope of this disclosure. Such embodiments of the inventive subject matter may be referred to herein individually or collectively by the term "invention" merely for convenience and without intending to voluntarily limit the scope of this application to any 35 single invention or inventive concept, if more than one is, in fact, disclosed. Thus, although specific embodiments have been illustrated and described herein, any arrangement calculated to achieve the same purpose may be substituted for the specific embodiments shown. This disclosure is intended to cover any and all adaptations or variations of various embodiments. Combinations of the above embodiments, and

other embodiments not specifically described herein, will be apparent to those of skill in the art upon reviewing the above description.

CLAIMS

What is claimed is:

1. A wearable external defibrillator comprising:
 - 5 two or more sensing electrodes configured to engage with a patient's skin to detect a cardiac signal;
 - a first defibrillator electrode pad configured to engage with the patient's skin and to deliver an electrical therapy to the patient, the first defibrillator electrode pad configured to be in continuous contact with the patient's skin;
 - 0 a first patient engagement substrate comprising an adhesive, the first defibrillator electrode pad, a first fluid transport element configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a first vapor permeable layer;
 - 5 a second patient engagement substrate comprising a second defibrillator electrode pad, a second adhesive, a second fluid transport element in fluid communication with the second patient engagement substrate configured to transport fluid away from the skin to allow the wearable external defibrillator to be worn continuously, and a second vapor permeable layer;
 - an energy source;
 - one or more capacitors in electrical communication with the energy source and the first defibrillator electrode pad and the second defibrillator electrode pad;
 - 0 a controller configured to detect the cardiac signal with the two or more sensing electrodes and to charge the one or more capacitors with the energy source followed by discharging the one or more capacitors to deliver a therapeutic shock through the first defibrillator electrode pad and the second defibrillator electrode pad to the patient while the first and second patient engagement substrates are engaged with the patient, wherein the energy source, one or more capacitors, and controller are enclosed within a plurality of housings supported by at least one of the first patient engagement substrate and the second patient engagement substrate; and
 - 5 a flexible circuitry providing electrical communication between the housings.
2. The wearable defibrillator of claim 1, further comprising: one or more mechanical connections between two or more of the housings.
- 30 3. The wearable defibrillator of claim 1, wherein the flexible circuitry is adapted to receive an electrical connection from one or more of the plurality of housings.
4. The wearable defibrillator of any of the preceding claims, wherein the flexible circuitry is supported by the first patient engagement substrate.
- 35 5. The wearable defibrillator of any of the preceding claims, further comprising: a support chassis disposed between the housings and the first defibrillator electrode pad and adapted to spread a shear load of the housings.

6. The wearable defibrillator of claim 1, wherein the controller is configured to measure an impedance between a pair of electrodes selected from the group consisting of the first defibrillator electrode pad, the second defibrillator electrode pad and the two or more sensing electrodes.
7. The wearable defibrillator of claim 6, wherein the controller is configured to analyze the impedance to determine whether the pair of electrodes are in proper contact with the patient's skin.
8. The wearable defibrillator of any of the preceding claims, wherein the first defibrillator electrode pad and the second defibrillator electrode pad each comprises a conductive adhesive.
9. The wearable defibrillator of any of the preceding claims, wherein the first and second defibrillator electrode pads each comprises a plurality of perforations.
10. The wearable defibrillator of any of the preceding claims, wherein the first and second defibrillator electrode pads each comprises a carbon vinyl film, Ag/AgCl coated carbon vinyl film, or Ag coated carbon vinyl film.
11. The wearable defibrillator of claim 8, wherein the conductive adhesive comprises a conductive hydrogel.
12. The wearable defibrillator of any of the preceding claims, further comprising: a wireless radio configured to wirelessly transmit data from the wearable defibrillator.
13. The wearable defibrillator of any of the preceding claims, wherein the controller is configured to measure impedances between pairs of electrodes selected from the group consisting of the first defibrillator electrode pad, the second defibrillator electrode pad and the one or more sensing electrodes to sense impedance changes along a plurality of vectors of the patient, wherein the controller is configured to analyze the impedance changes along the plurality of vectors of the patient.
14. The wearable defibrillator of any of the preceding claims, further comprising: a tactile feedback module.
15. The wearable defibrillator of claim 14, wherein the tactile feedback module is a vibration motor.
16. The wearable defibrillator of any the preceding claims, further comprising: a connection between the one or more of the plurality of housings and the at least one of the first patient engagement substrate and the second patient engagement substrate, the connection configured to support the weight of the plurality of housings and components within the plurality of housings.
17. The wearable defibrillator of claim 16, wherein the connection allows for relative movement between the plurality of housings and the first patient engagement substrate.

18. The wearable defibrillator of claim 16, wherein the connection further comprises one or more electrical connections between the plurality of housings and the first patient engagement substrate.
19. The wearable defibrillator of any of claims 16-18, wherein the connection comprises a removable and reversible connection.
- 5 20. The wearable defibrillator of claim 6, wherein the controller is further configured to measure the impedance using two or more discrete frequencies.
21. The wearable defibrillator of claim 20, the controller further configured to analyze the impedance measured at the two or more discrete frequencies to determine a power of the therapeutic shock for the patient based on the impedance.
- 0 22. A method of monitoring and defibrillating a patient's heart, comprising:
 - adhering to a first skin surface portion of the patient a first patient engagement substrate comprising a first sensing electrode and a first defibrillator electrode pad, the first defibrillator electrode pad in electrical communication with one or more capacitors and an electrical energy source sufficient to provide a defibrillating shock;
 - 5 adhering to a second skin surface portion of the patient a second patient engagement substrate comprising a second sensing electrode and a second defibrillator electrode pad, the second defibrillator electrode pad in electrical communication with the one or more capacitors and the electrical energy source, the one or more capacitors and the energy source being enclosed within a plurality of housings supported by at least one of the first patient engagement substrate and the second patient engagement substrate, the plurality of housings being in electrical communication via flexible circuitry;
 - 0 measuring patient data corresponding to a cardiac signal or other characteristic of the patient with the first sensing electrode and the second sensing electrode; and
 - analyzing the patient data to determine if the patient has an arrhythmia.
- 25 23. The method of claim 22, further comprising: sensing impedance changes along a plurality of vectors of the patient between pairs of electrodes selected from the group consisting of the first defibrillator electrode pad, the second defibrillator electrode pad the first sensing electrode and the second sensing electrode.
24. The method of claim 22 or 23, further comprising: delivering an electrical shock after 30 determining that the patient has an arrhythmia.
25. The wearable defibrillator of claim 1, wherein the housings are each configured to reversibly receive and support one or more of the energy source, the one or more capacitors, and the controller.
26. The wearable defibrillator of claim 25, further comprising one or more connectors each configured to reversibly engage with one or more of the energy source, the one or more capacitors, and

the controller, the electrical connector supported by the first patient engagement substrate, the second patient engagement substrate and/or the housings.

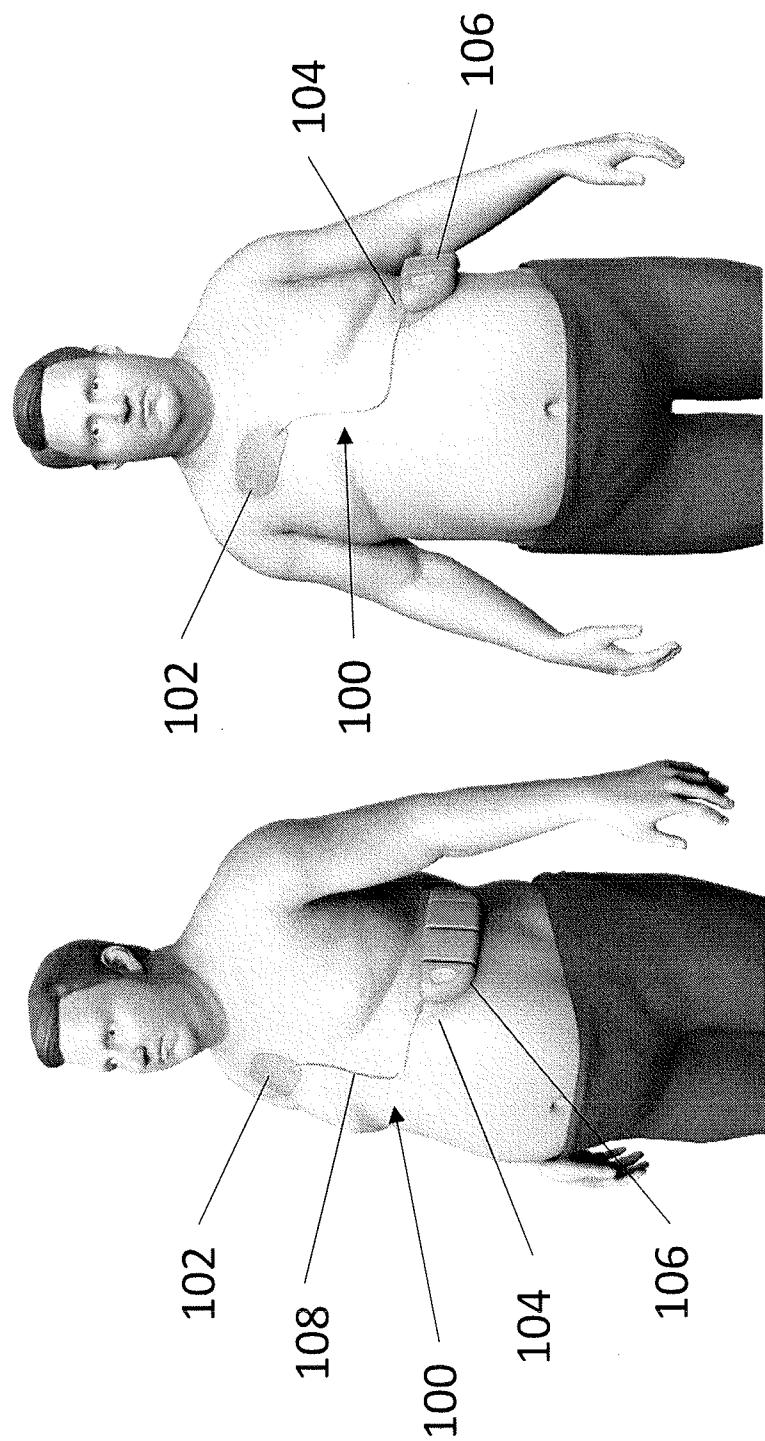
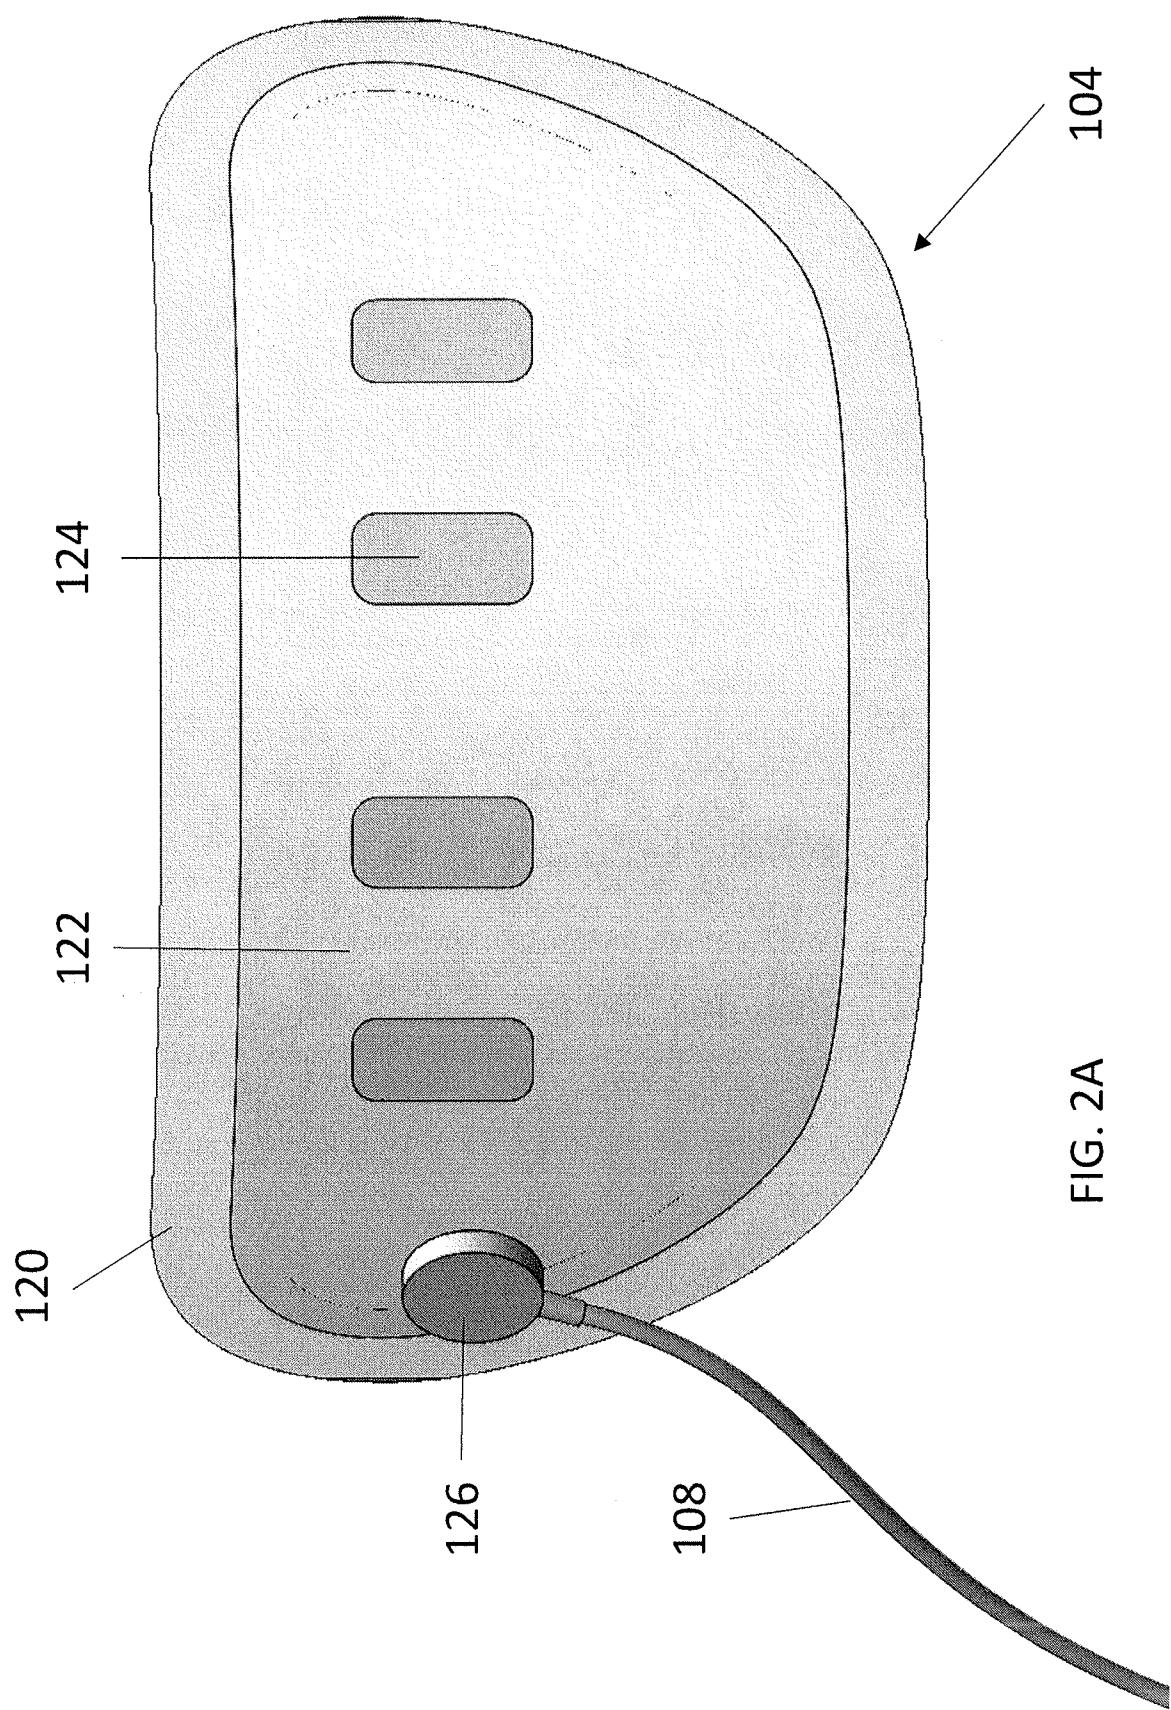


FIG. 1



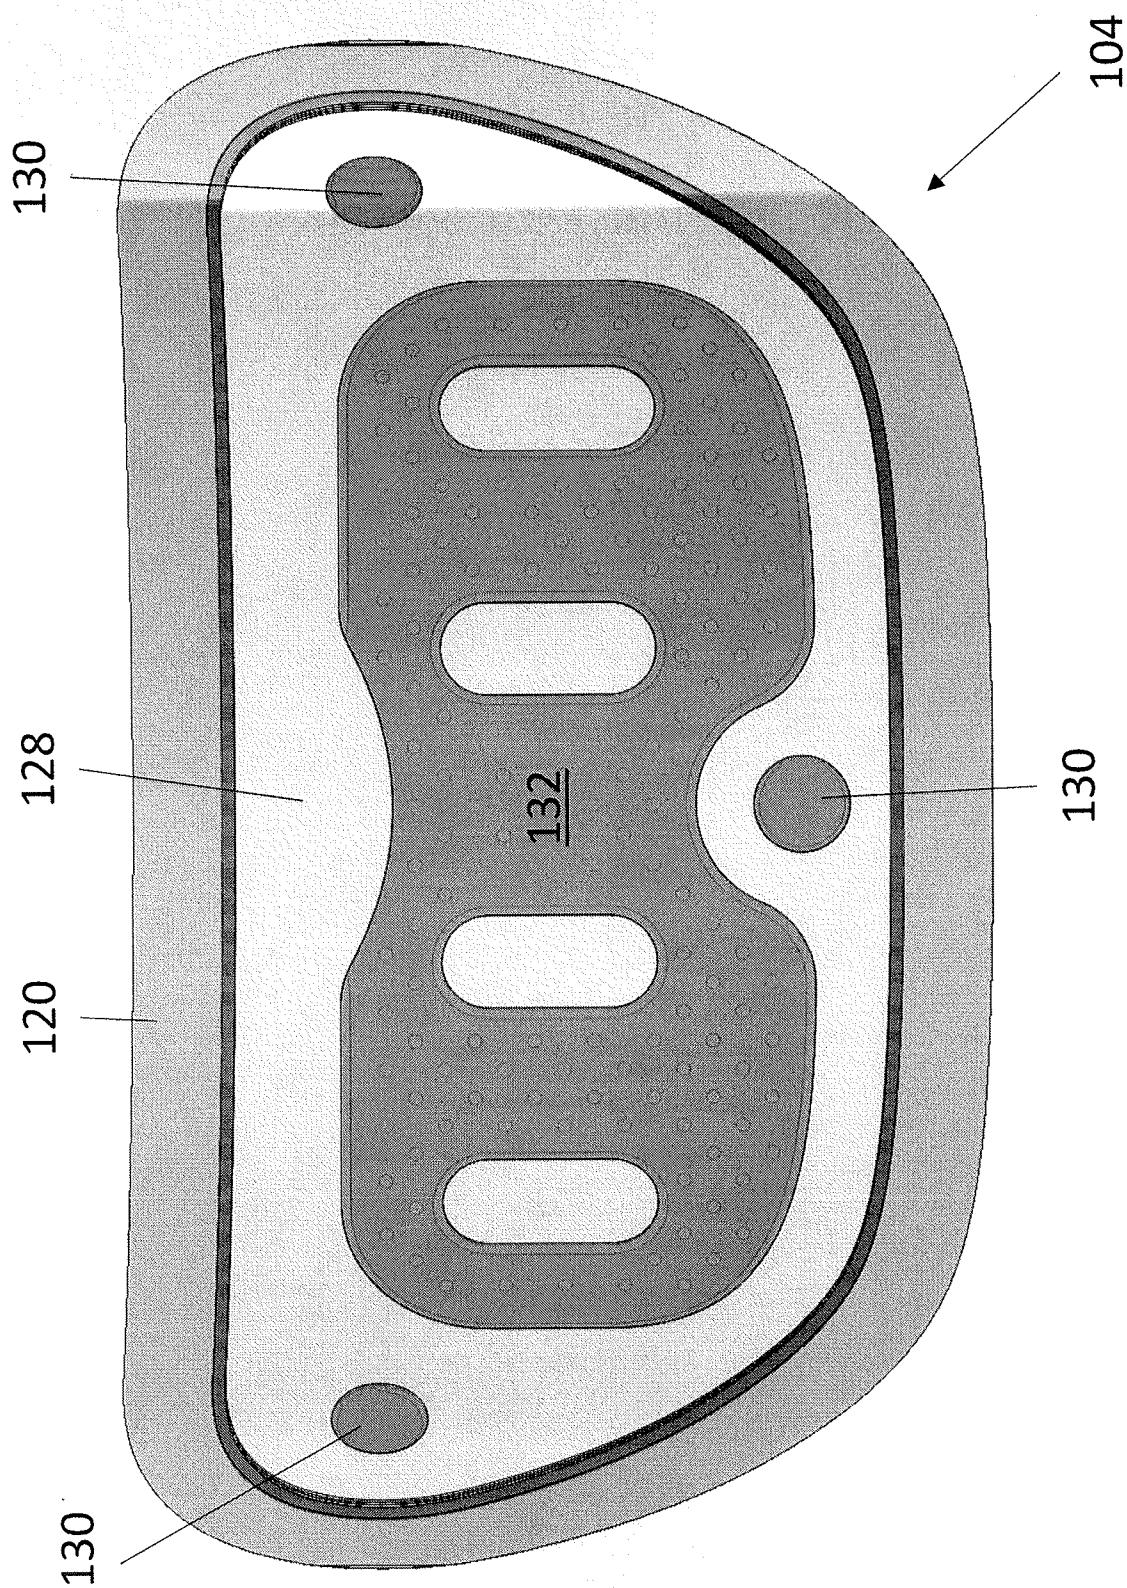


FIG. 2B

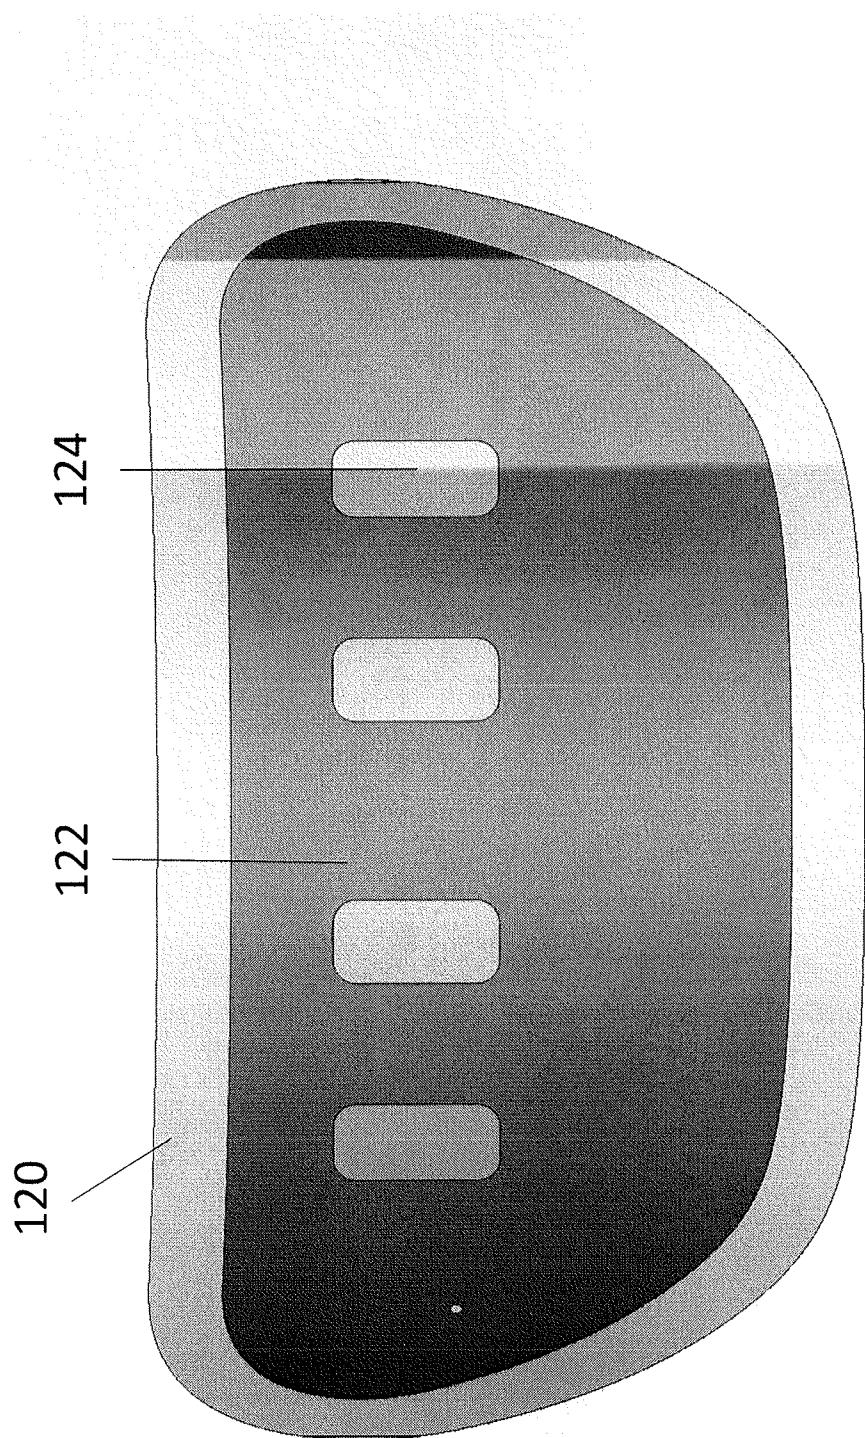


FIG. 2C

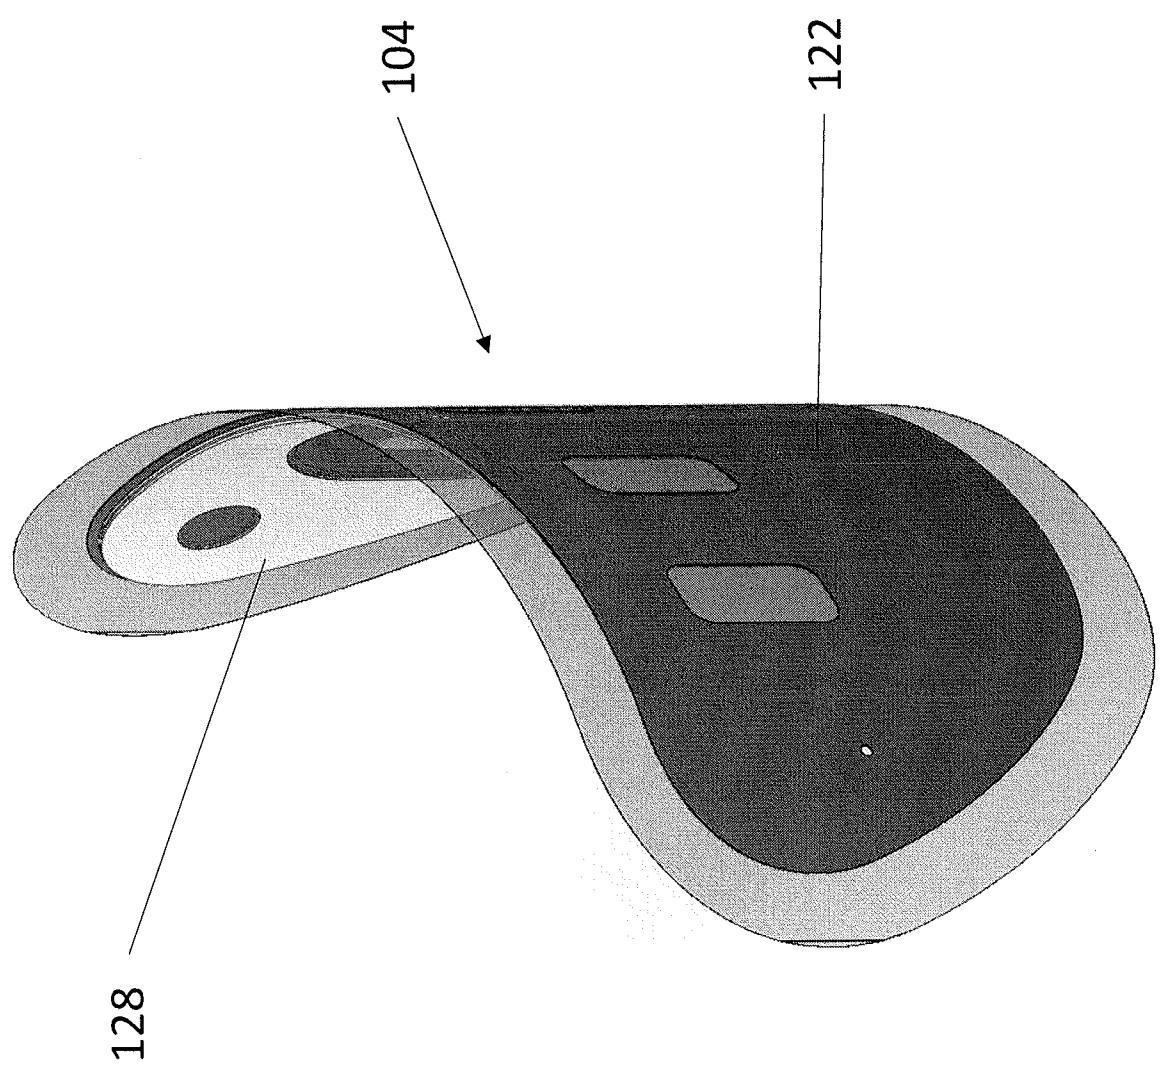


FIG. 2D

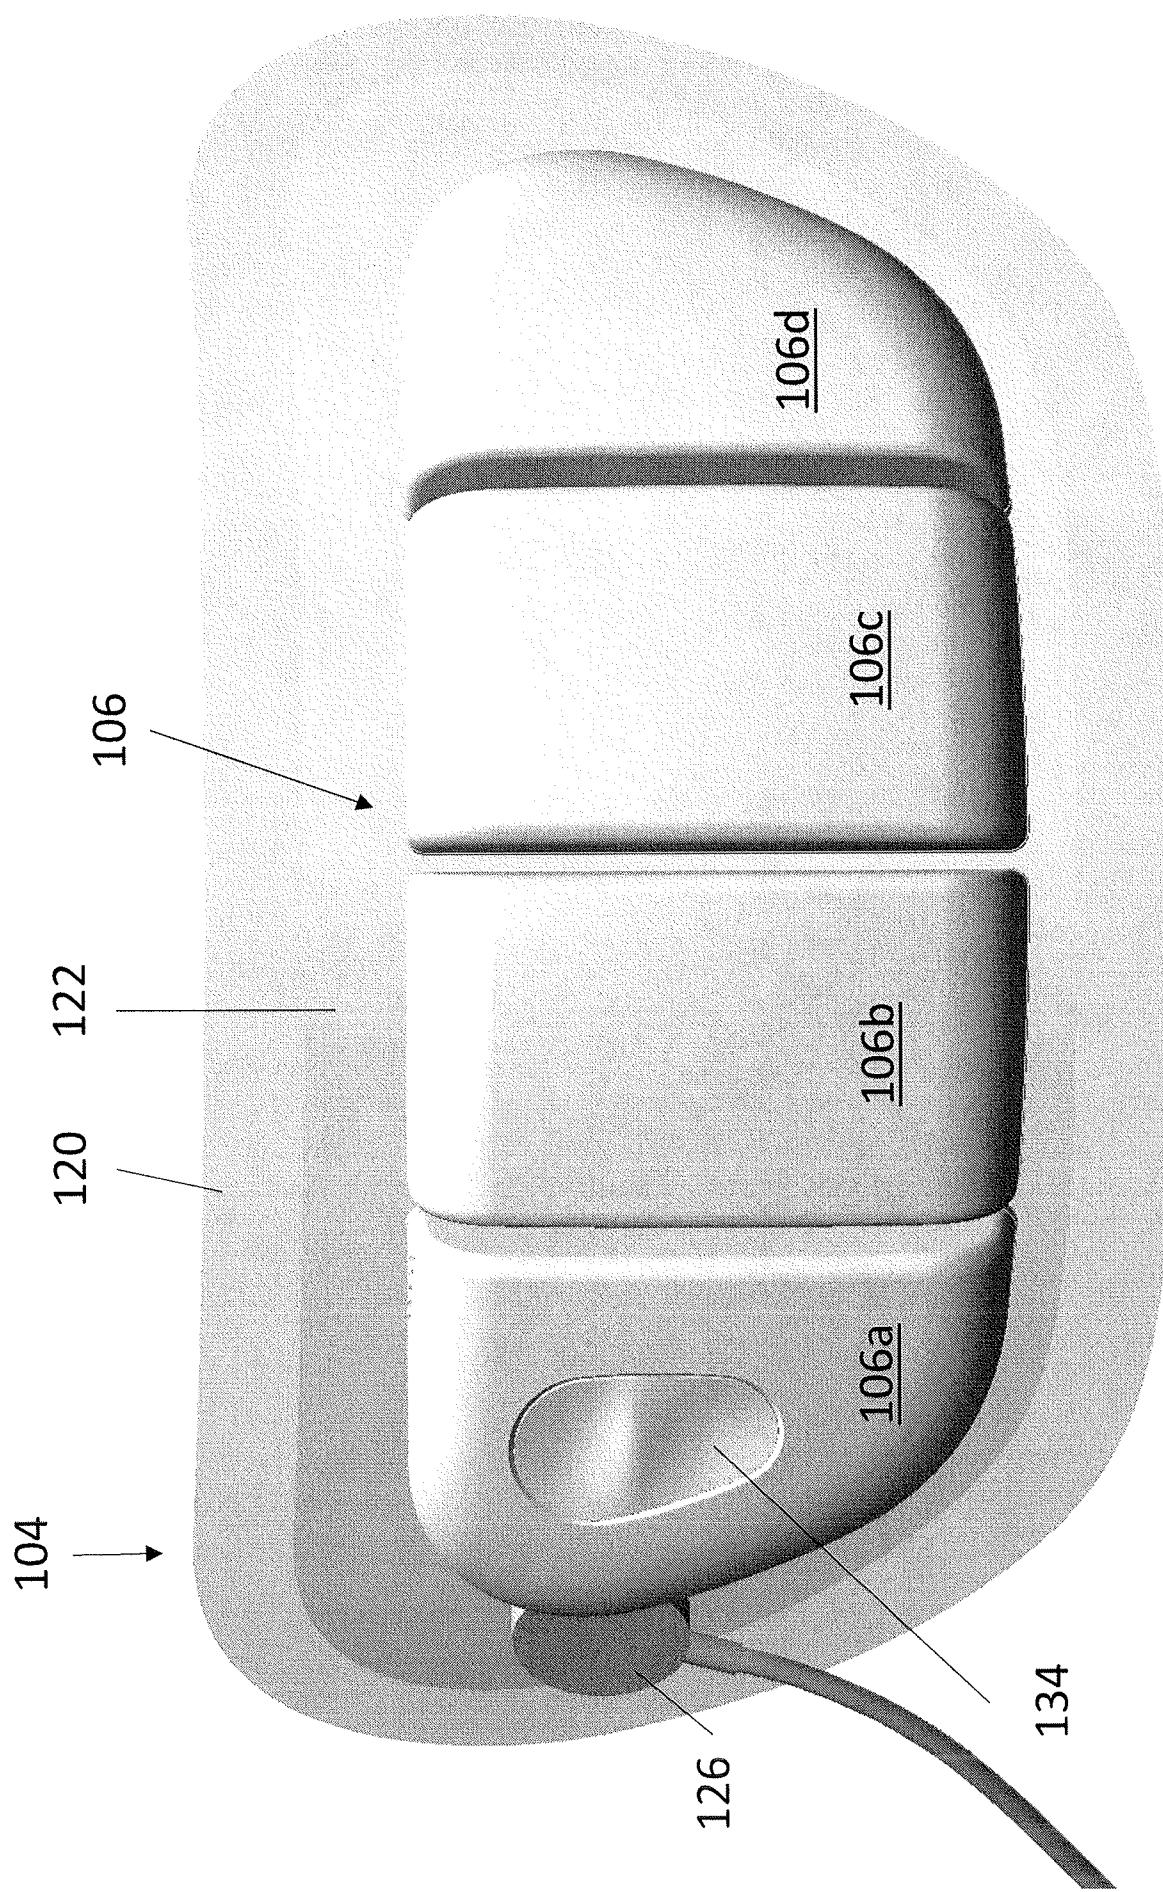


FIG. 3A

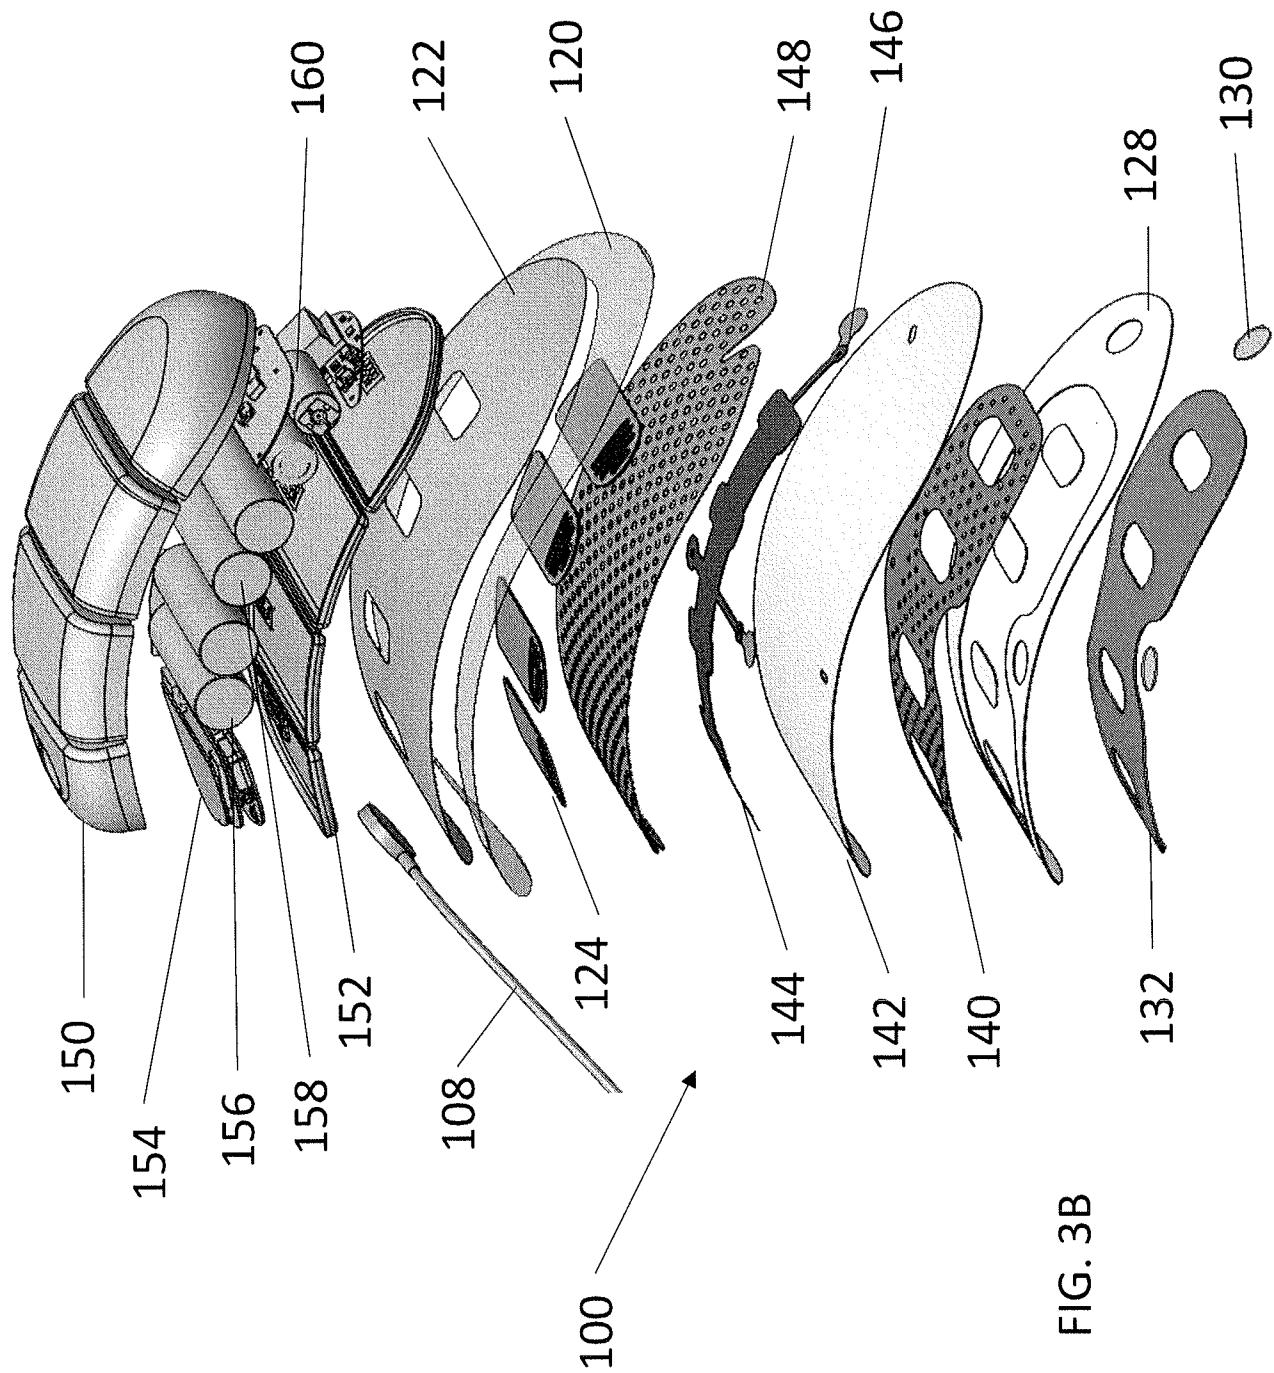


FIG. 3B

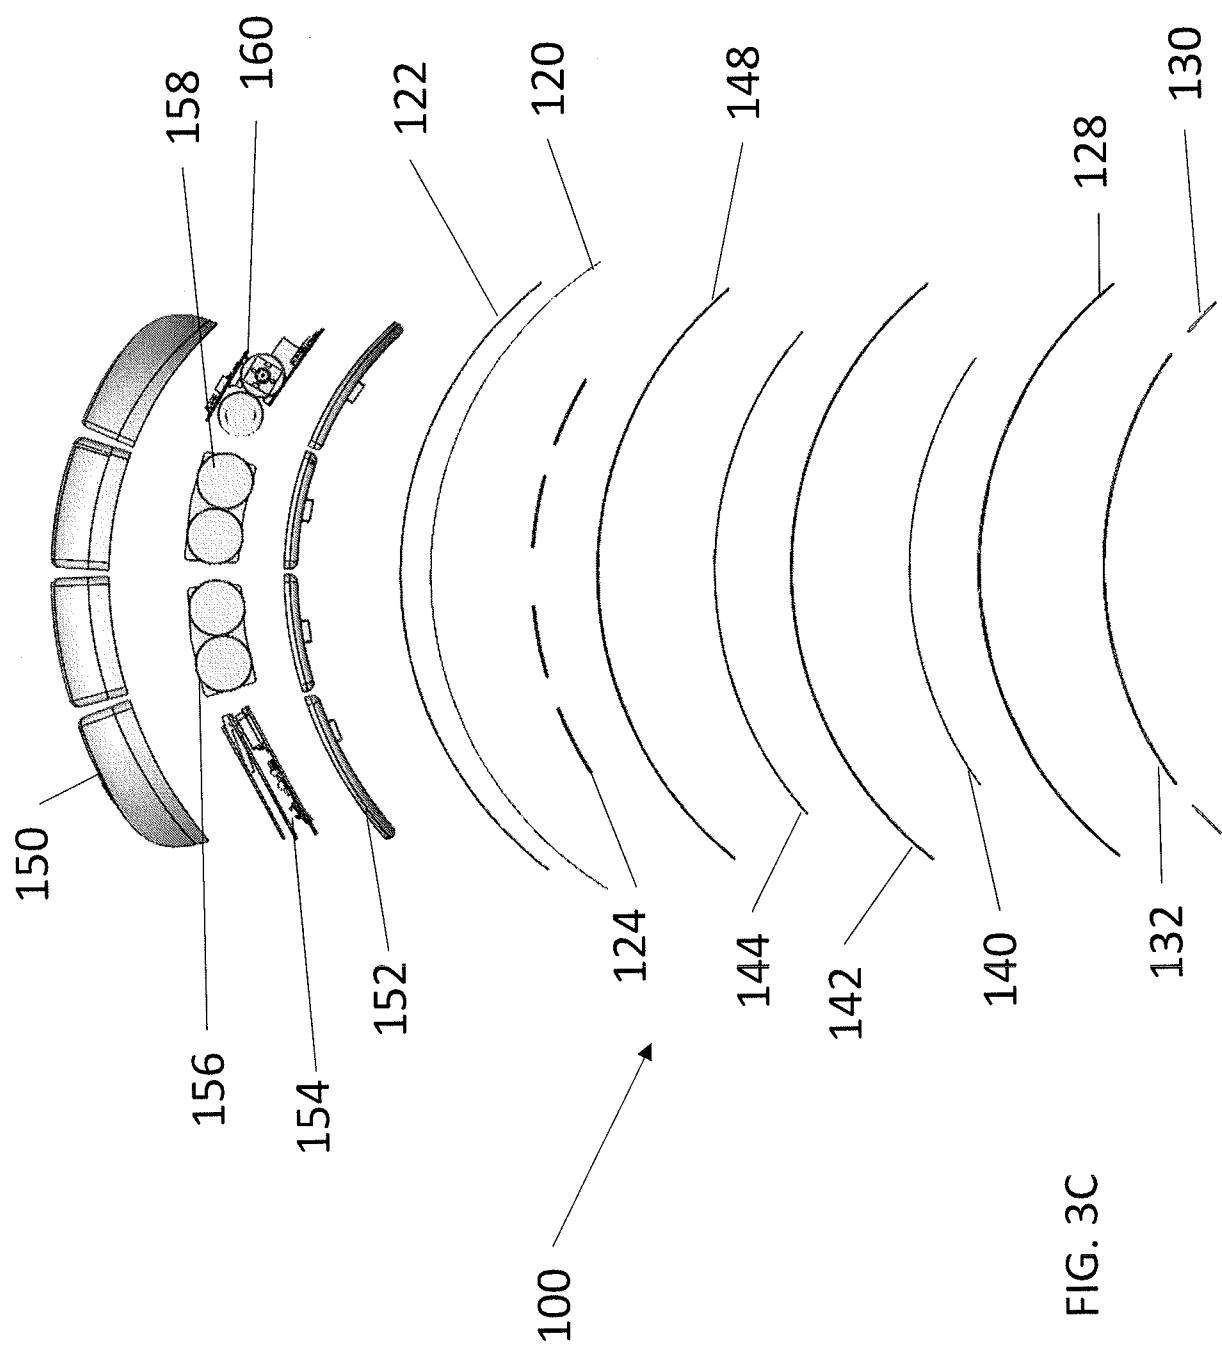


FIG. 3C

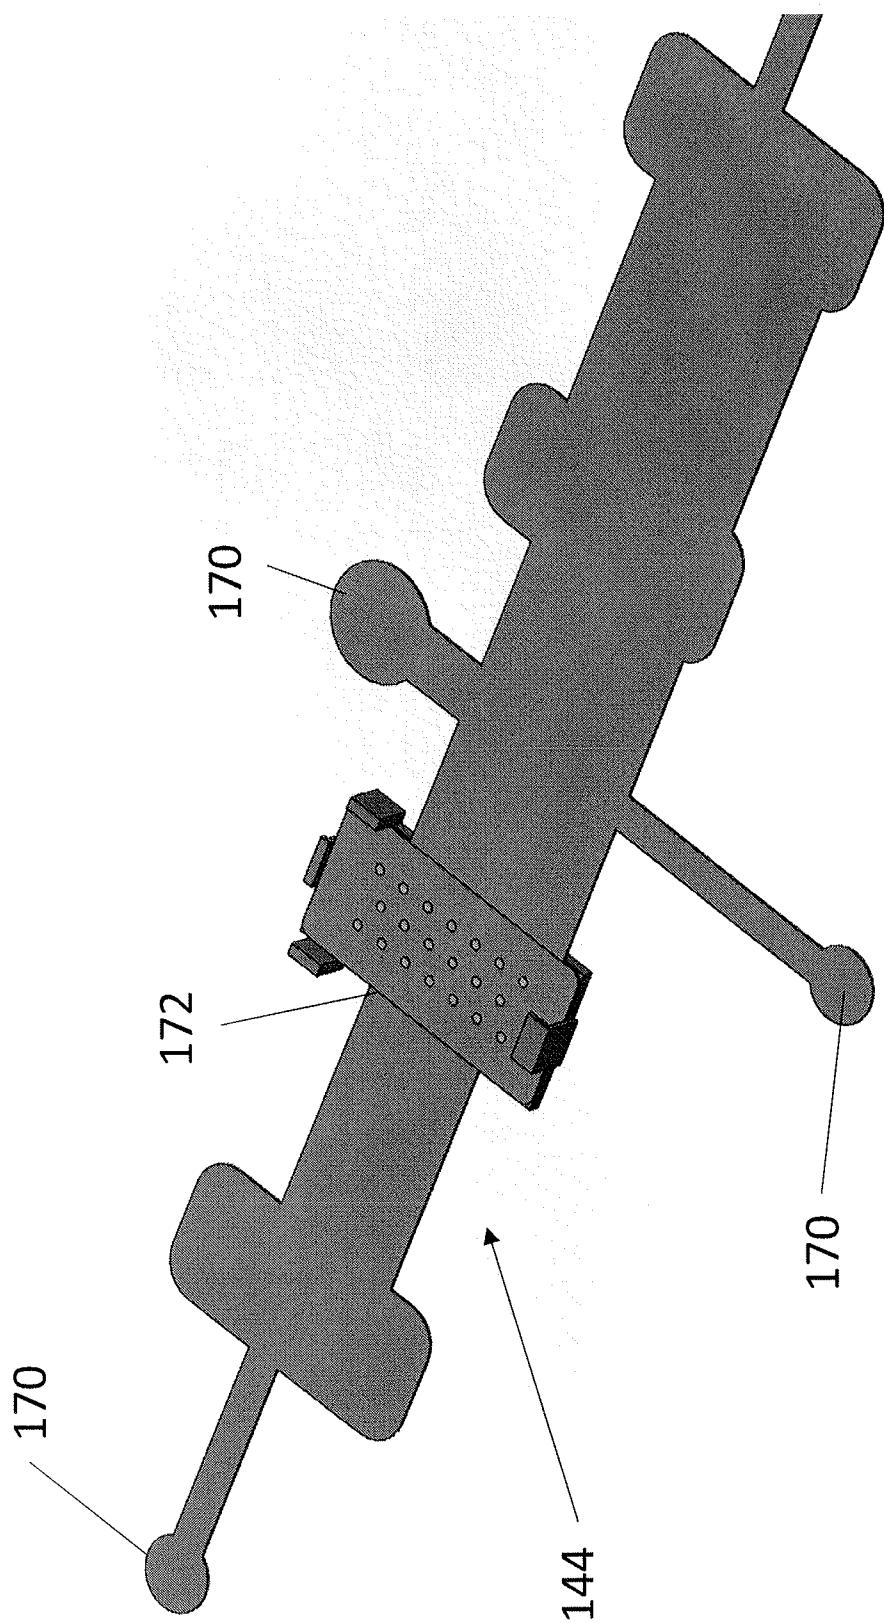


FIG. 4

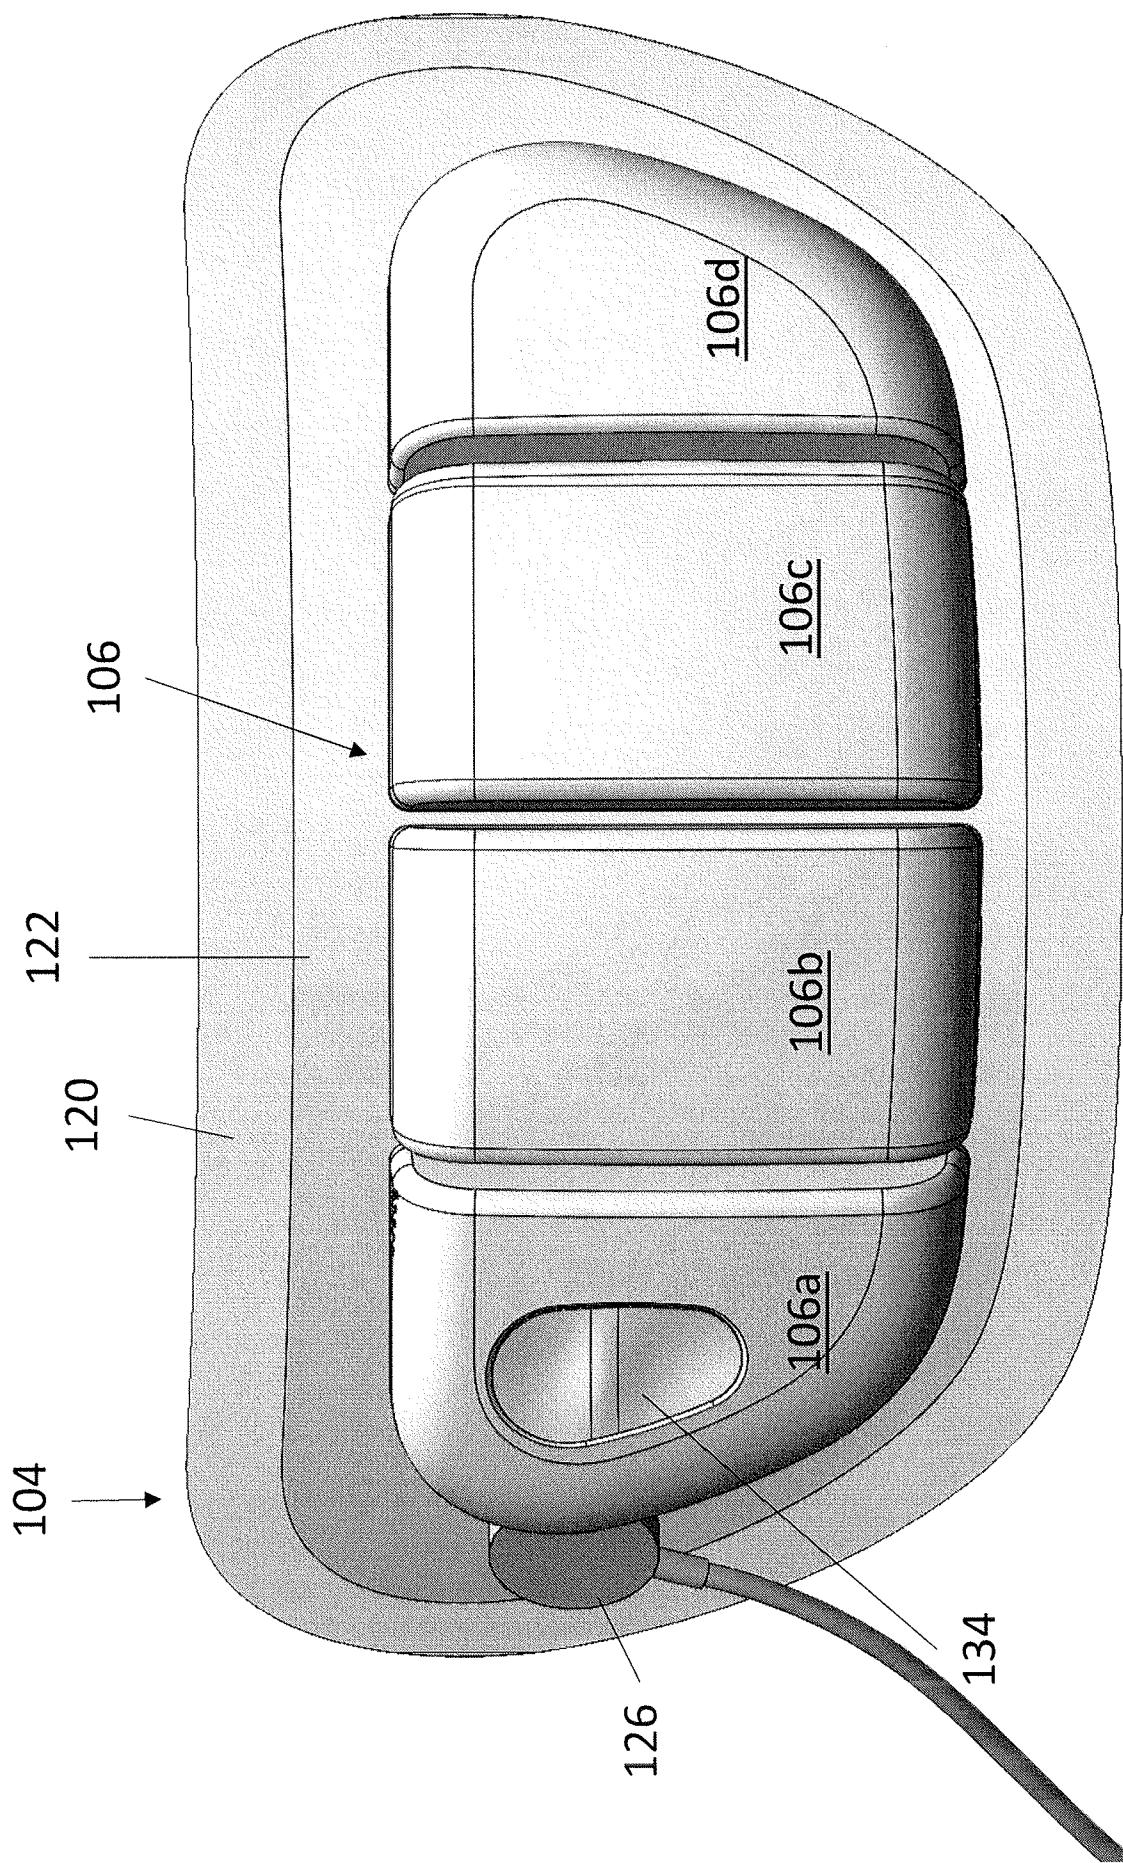


FIG. 5A

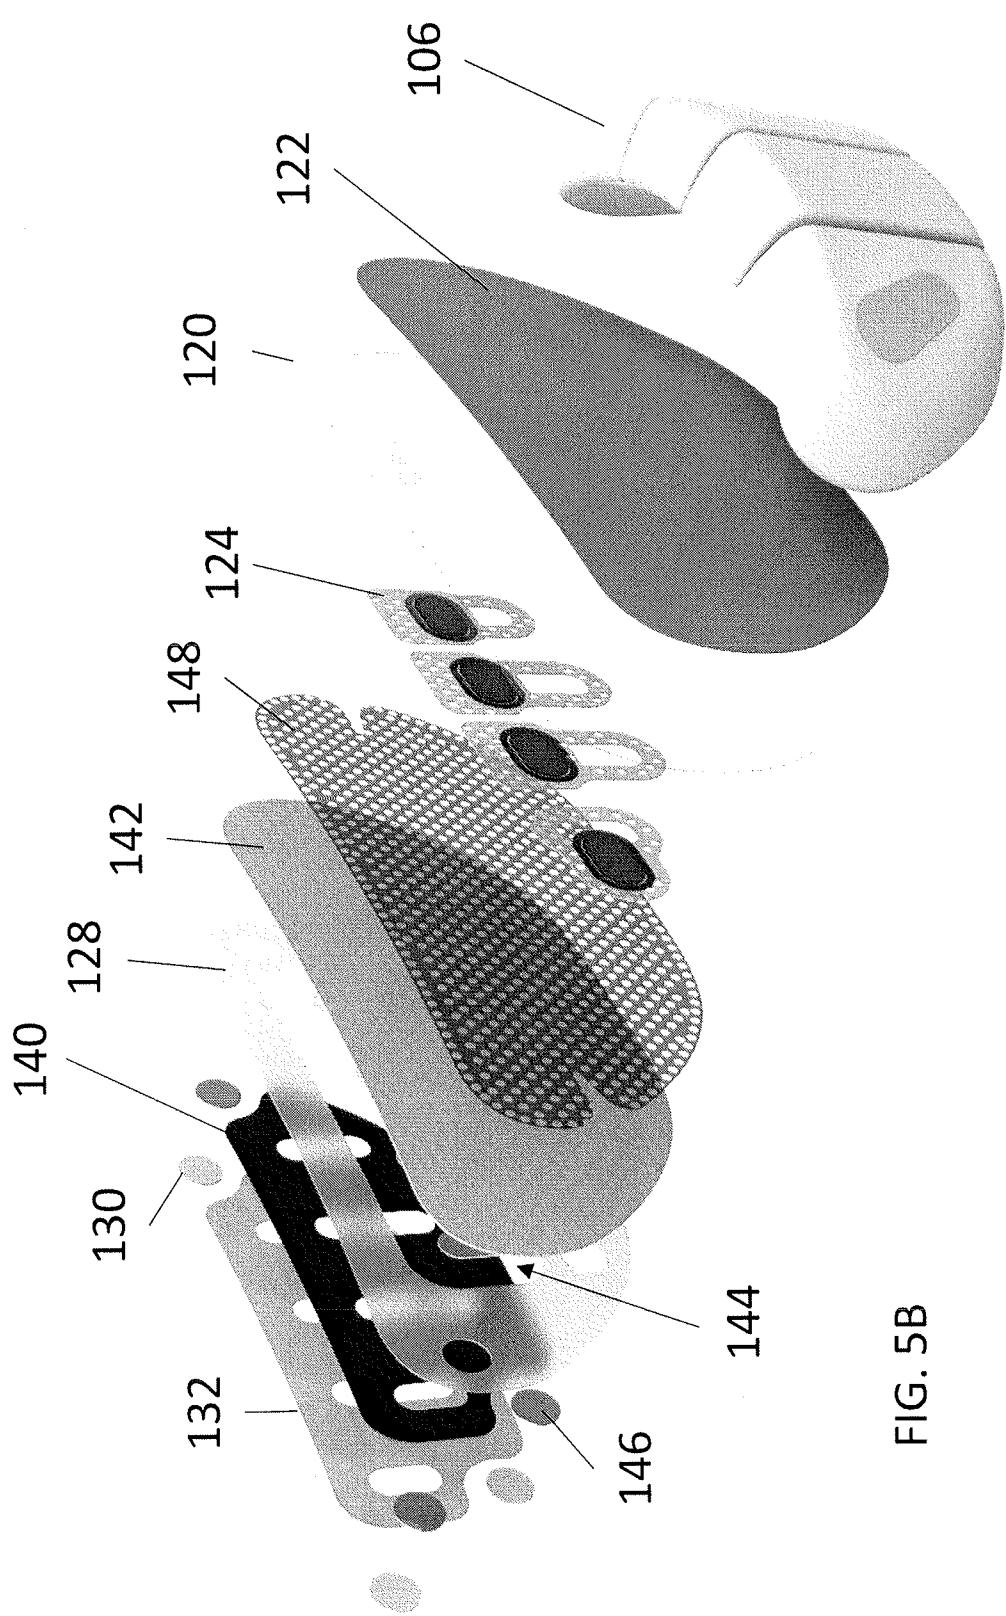


FIG. 5B

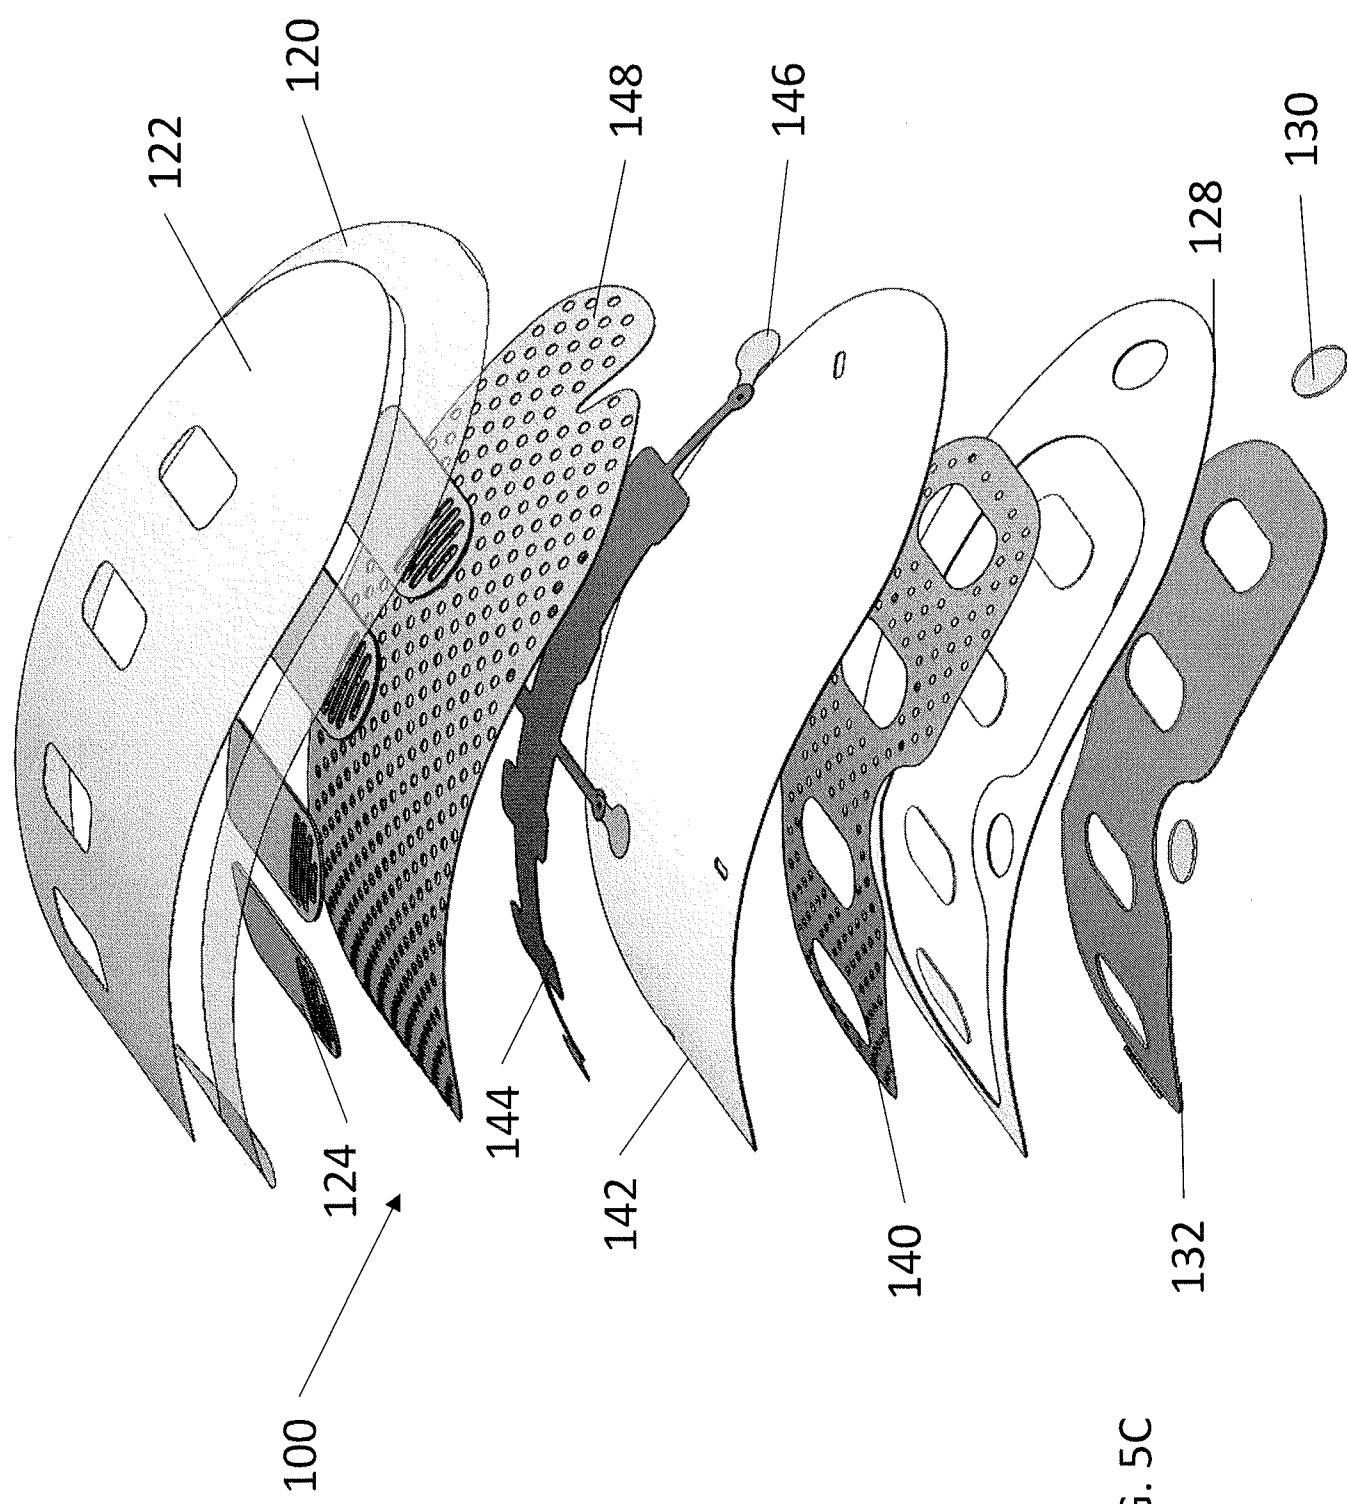


FIG. 5C

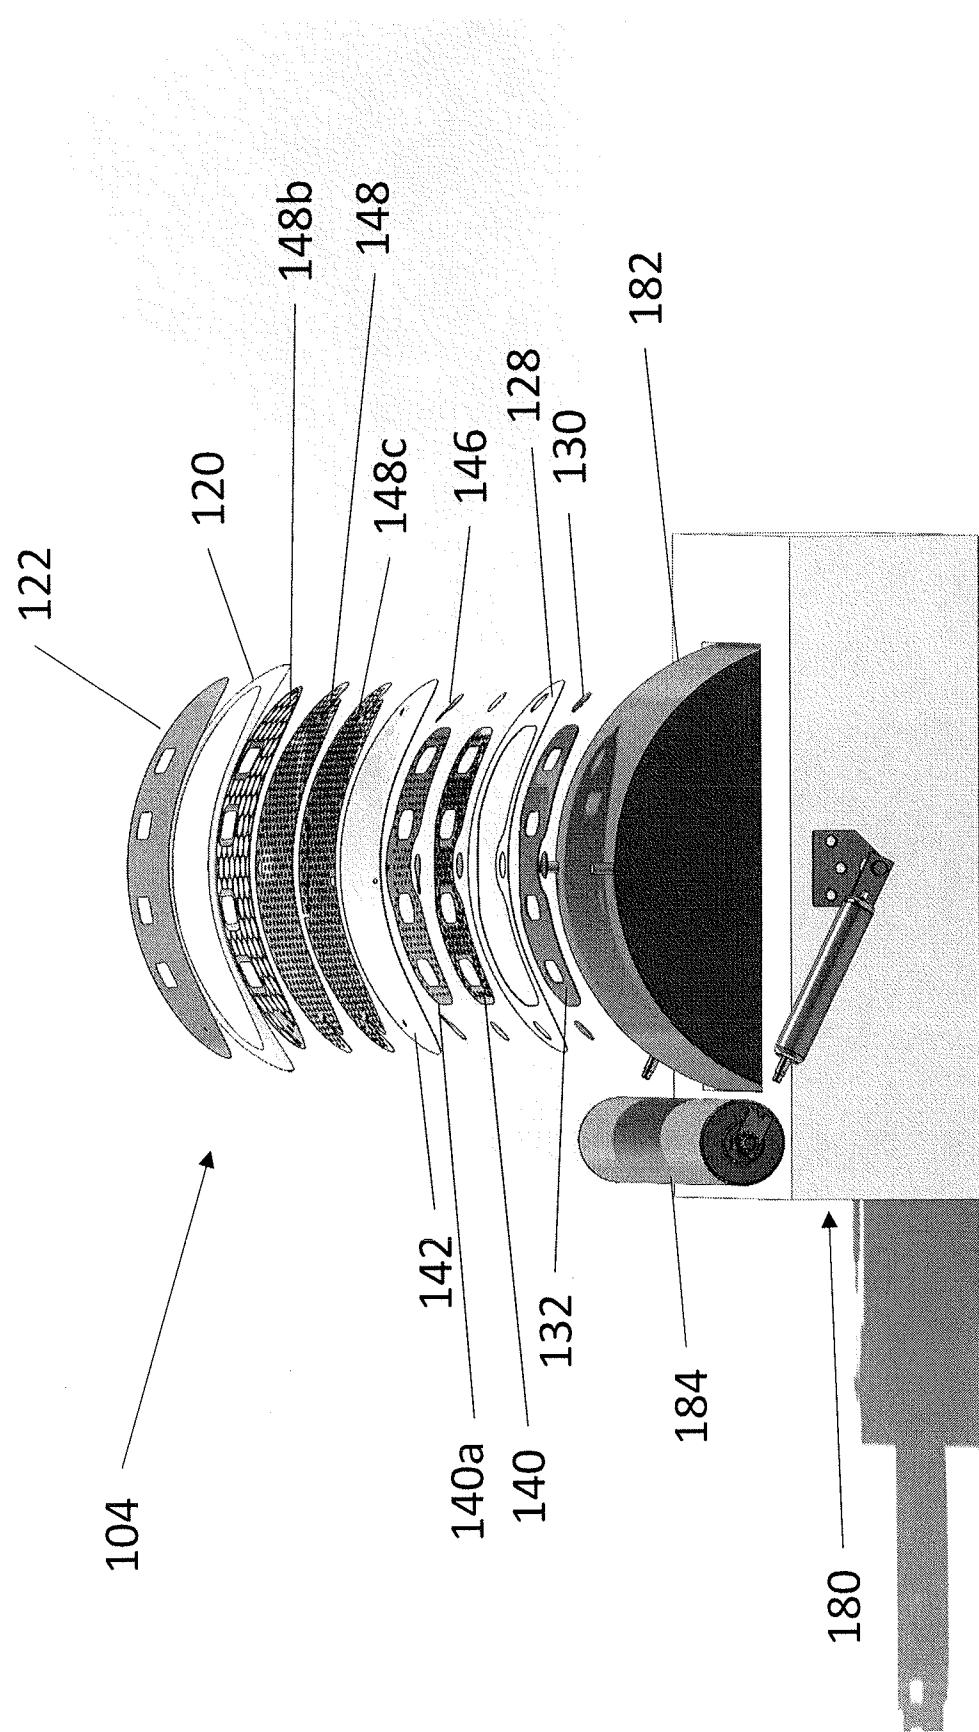


FIG. 6

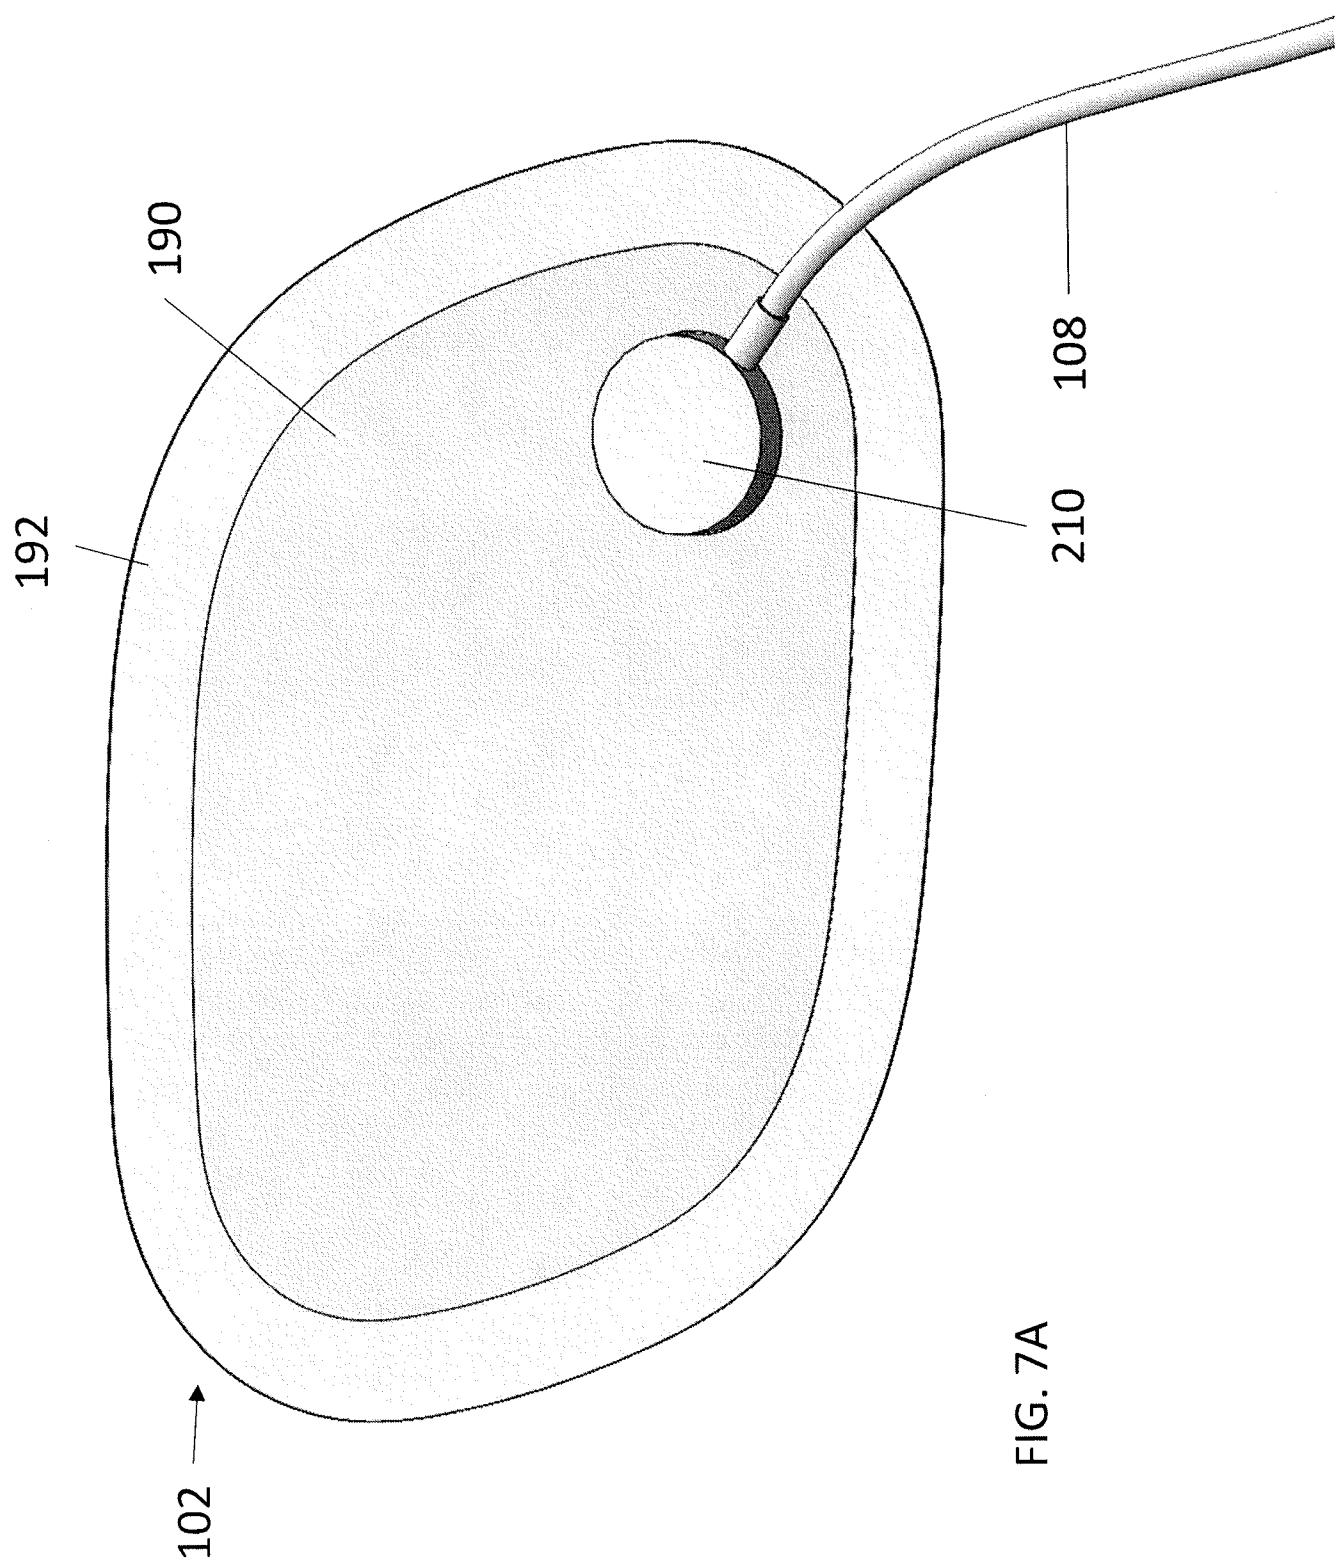


FIG. 7A

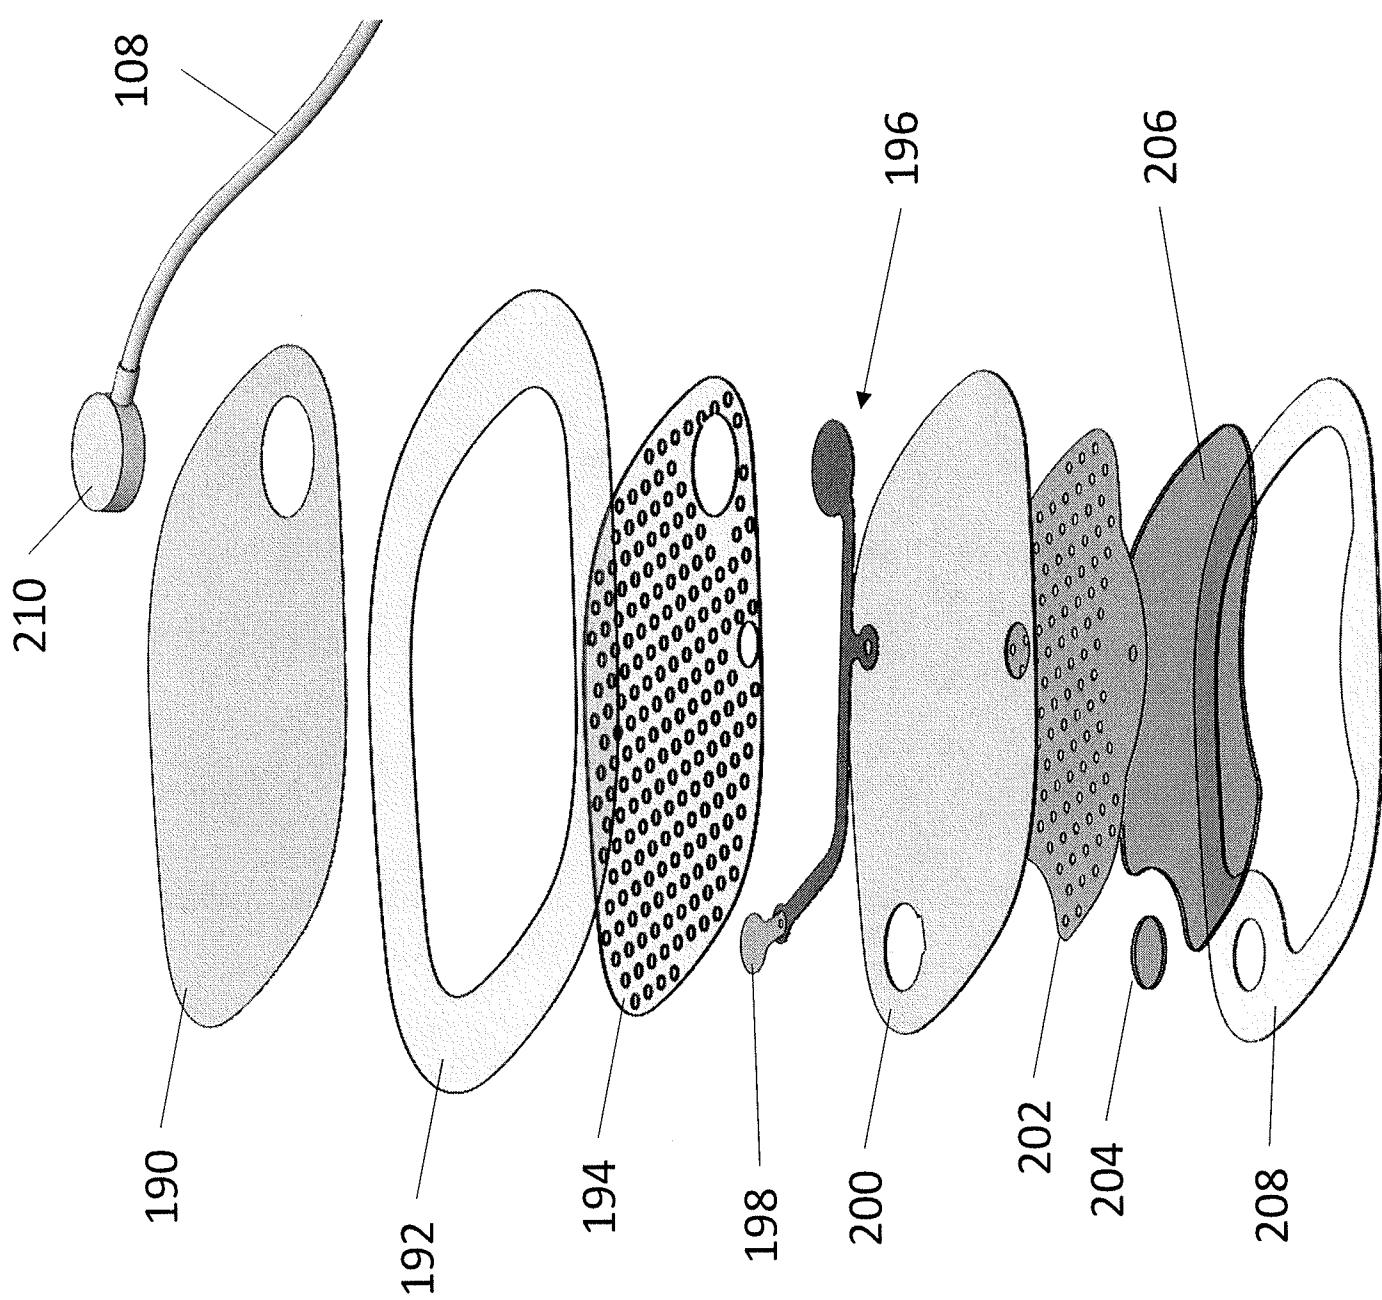


FIG. 7B

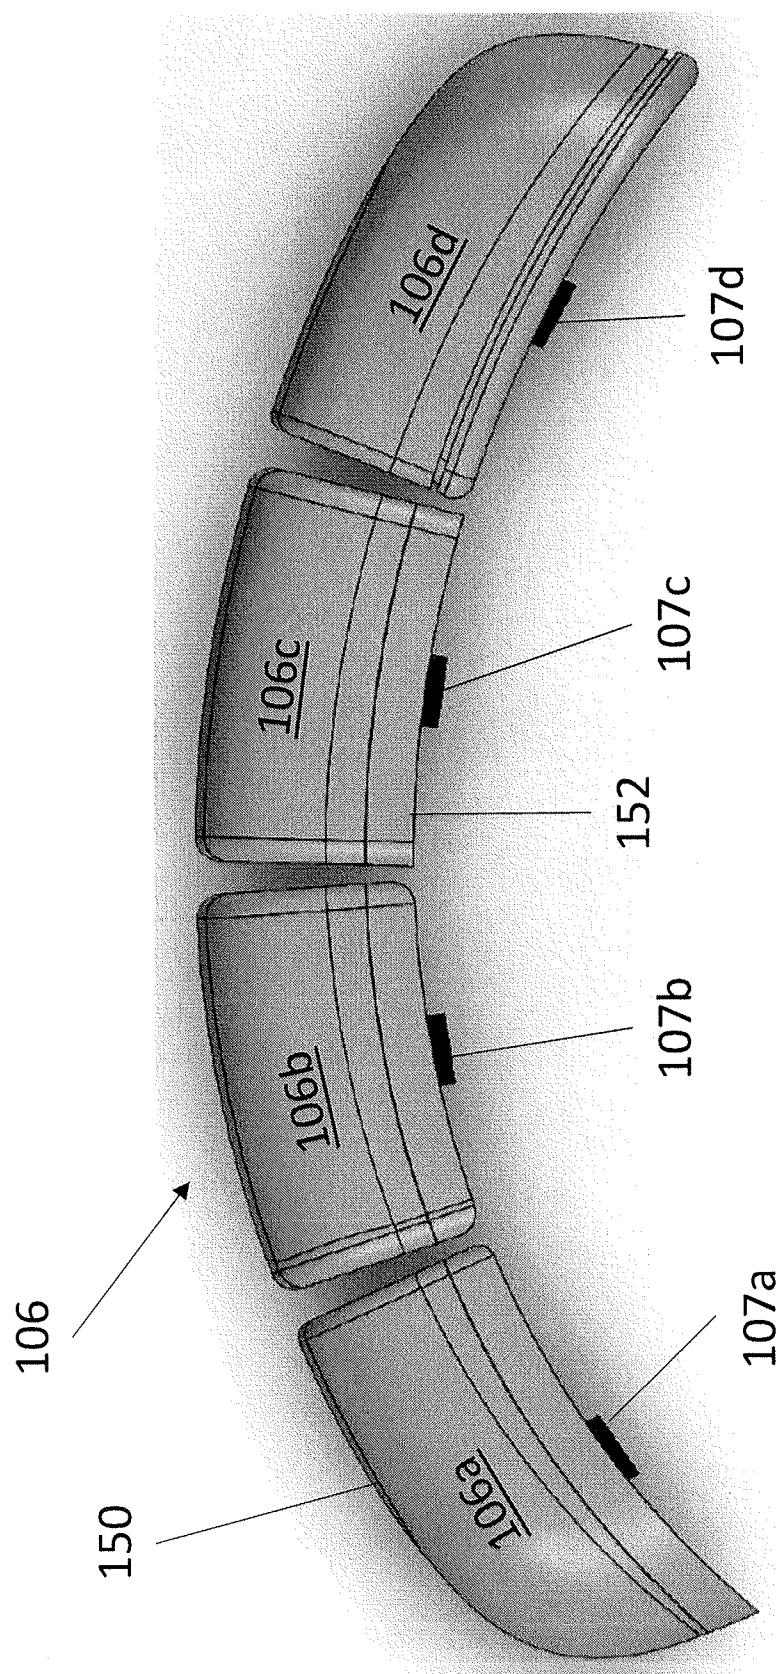


FIG. 8

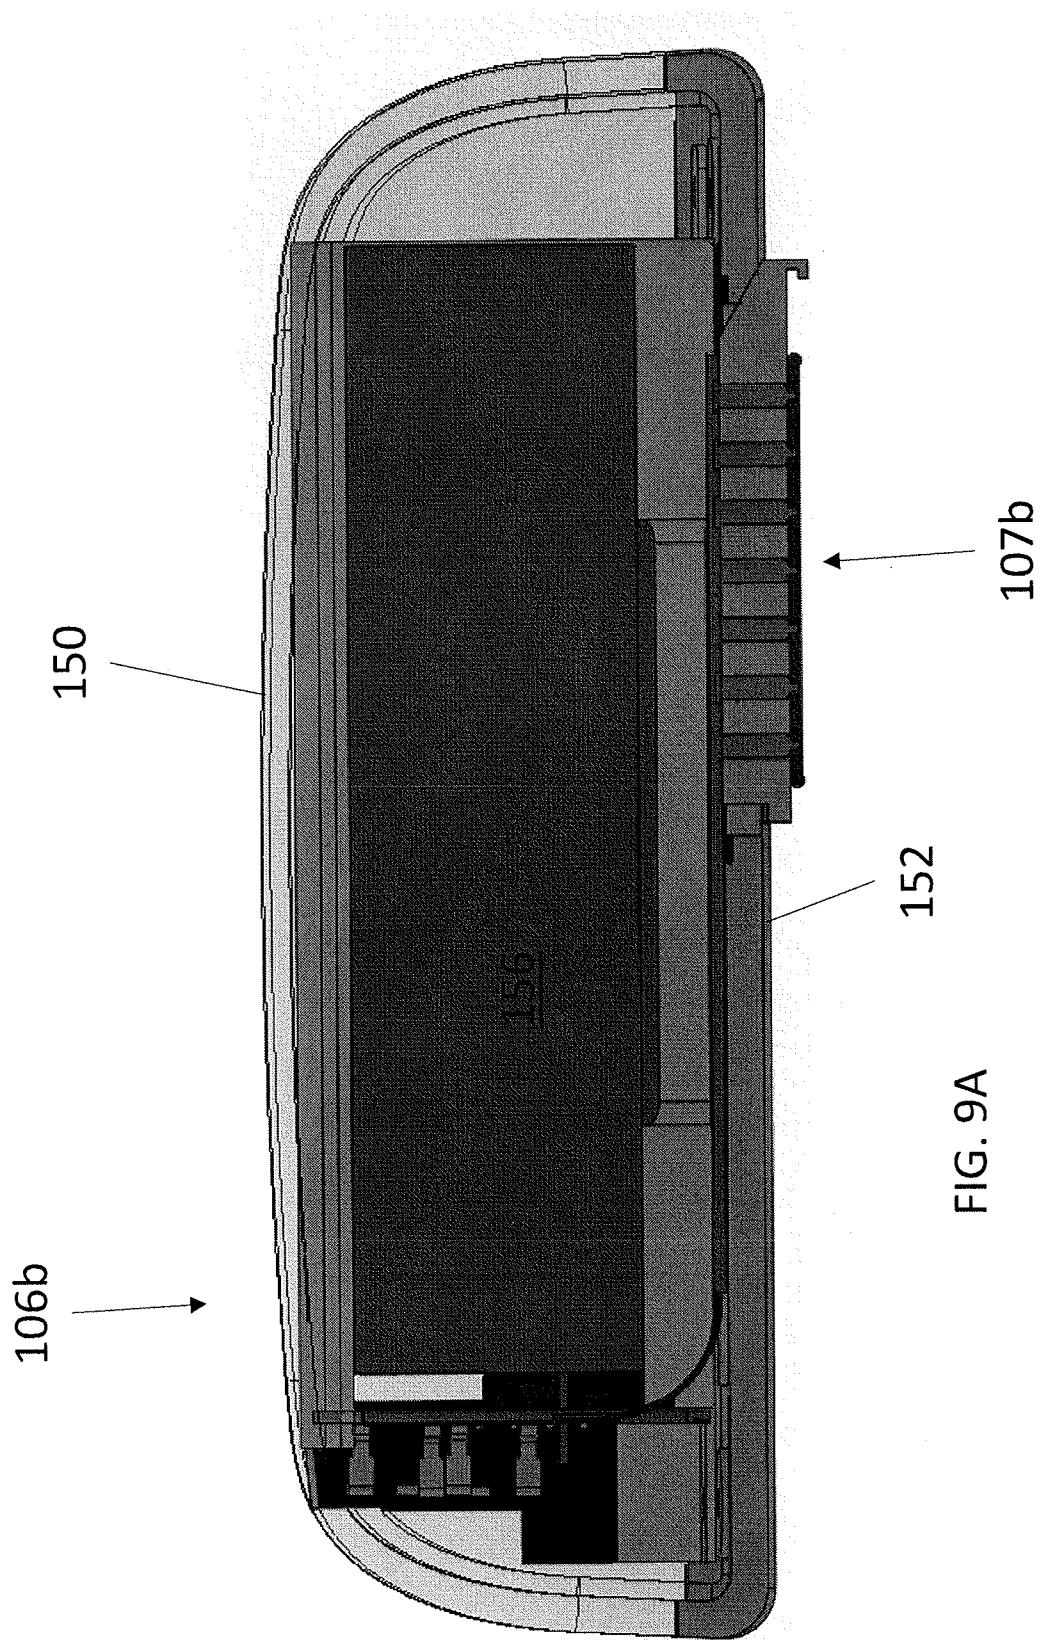


FIG. 9A

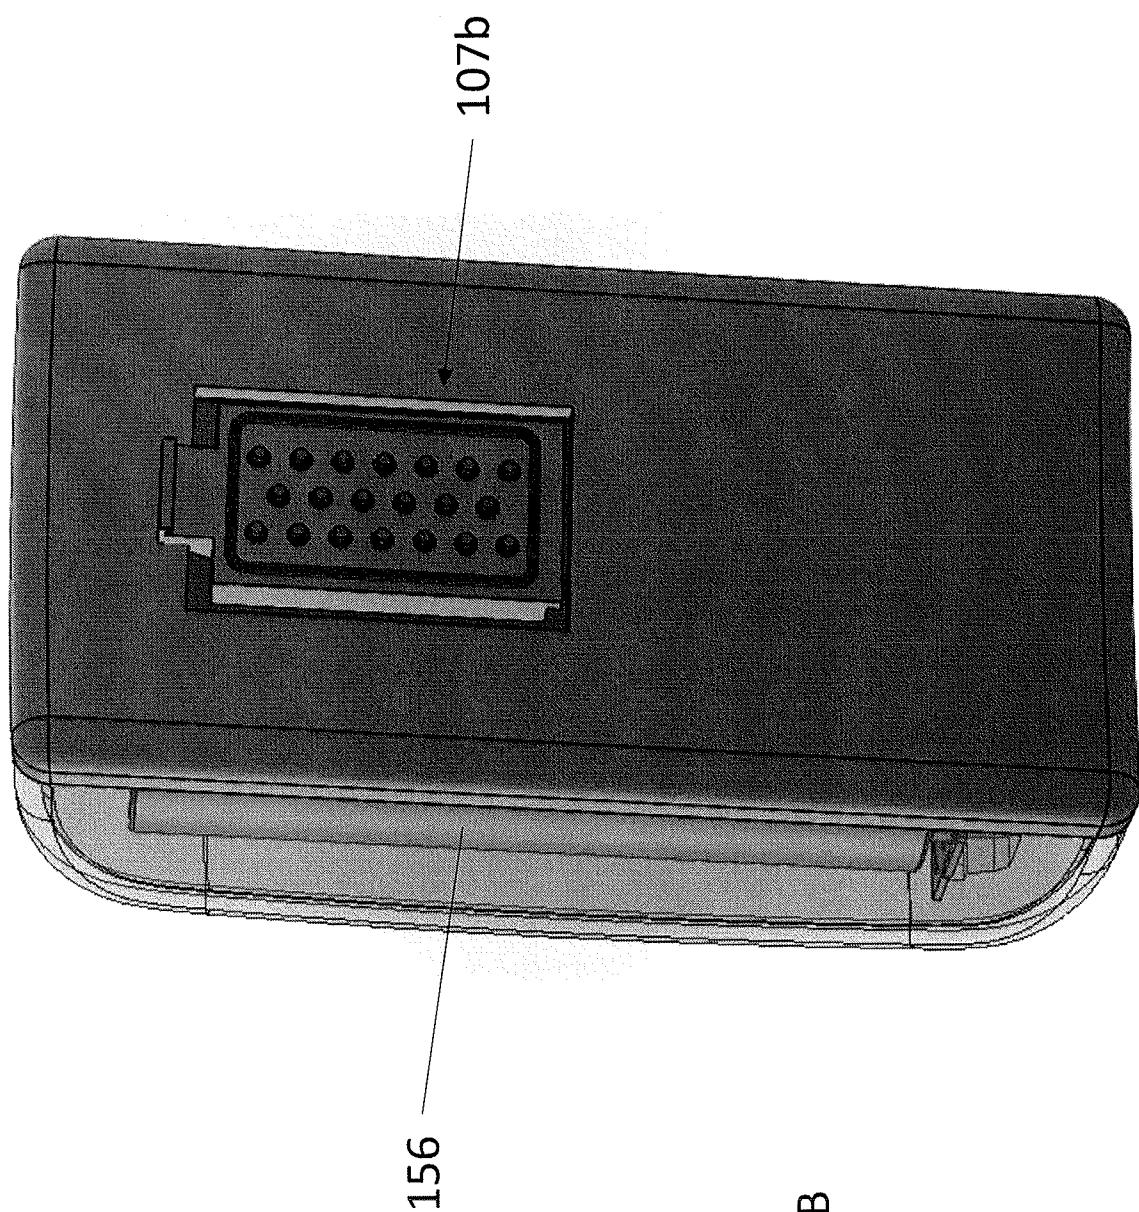
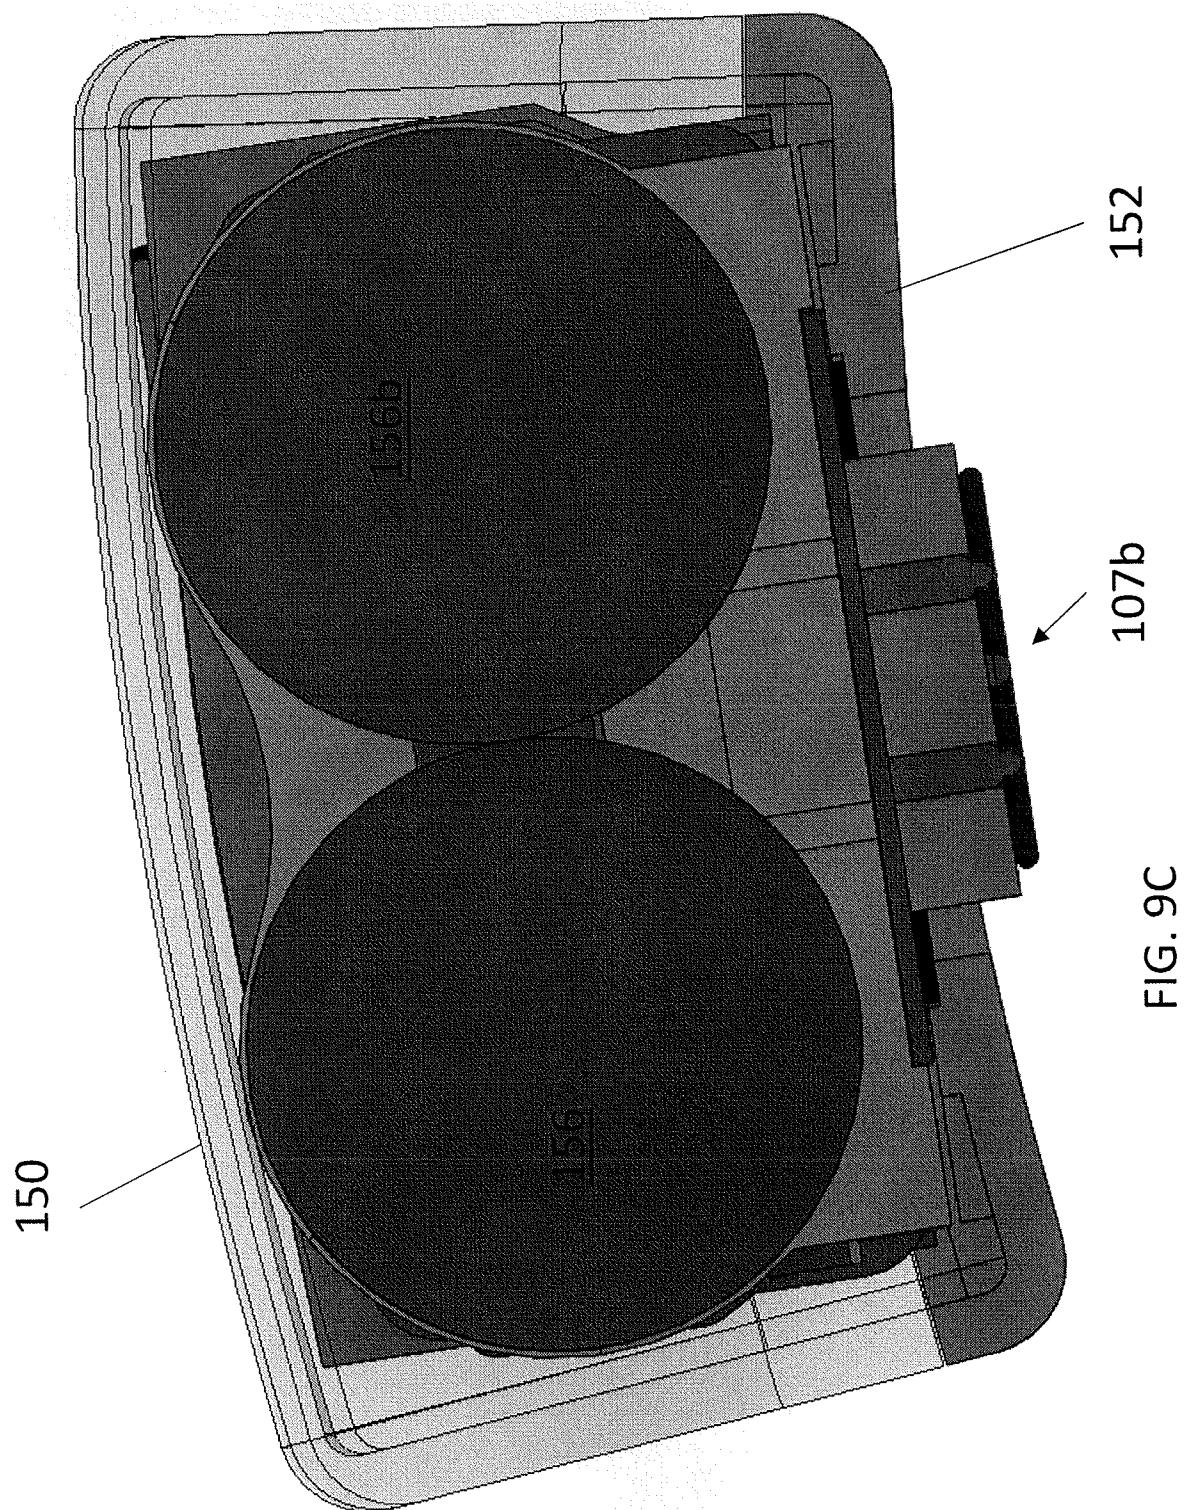


FIG. 9B



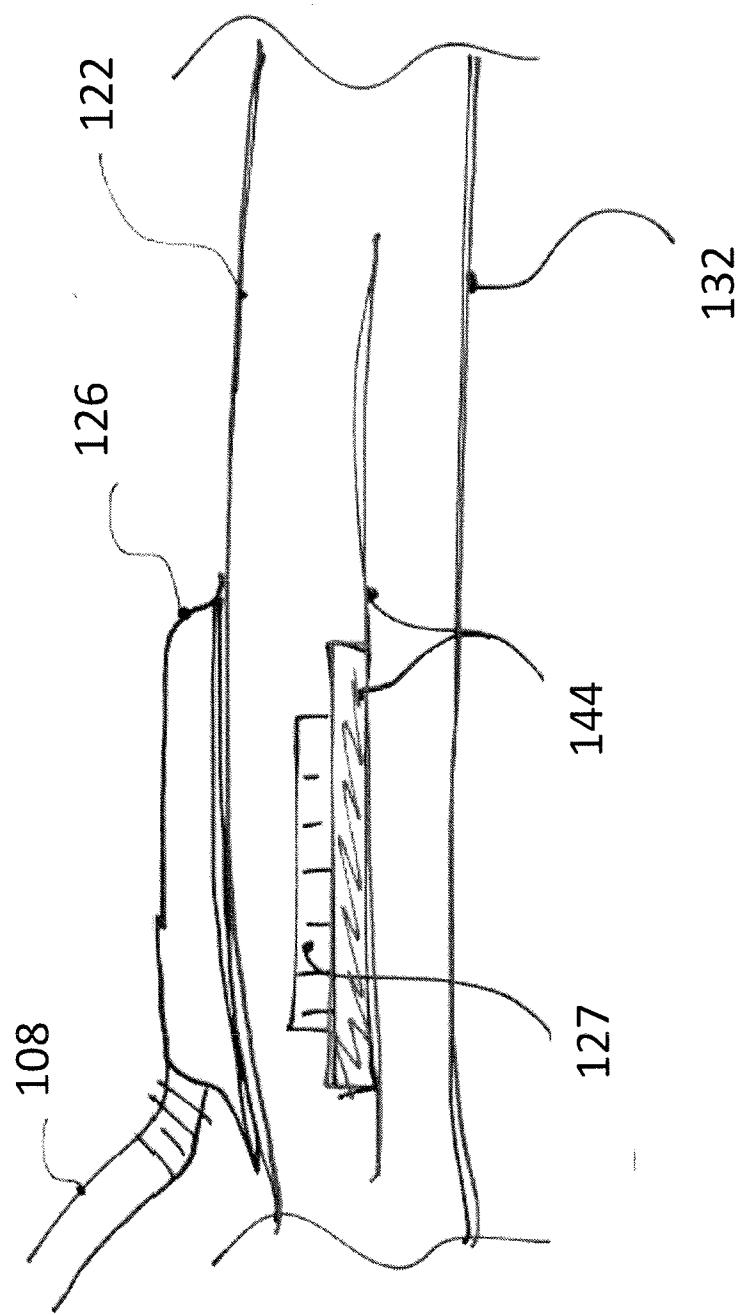


FIG. 10A

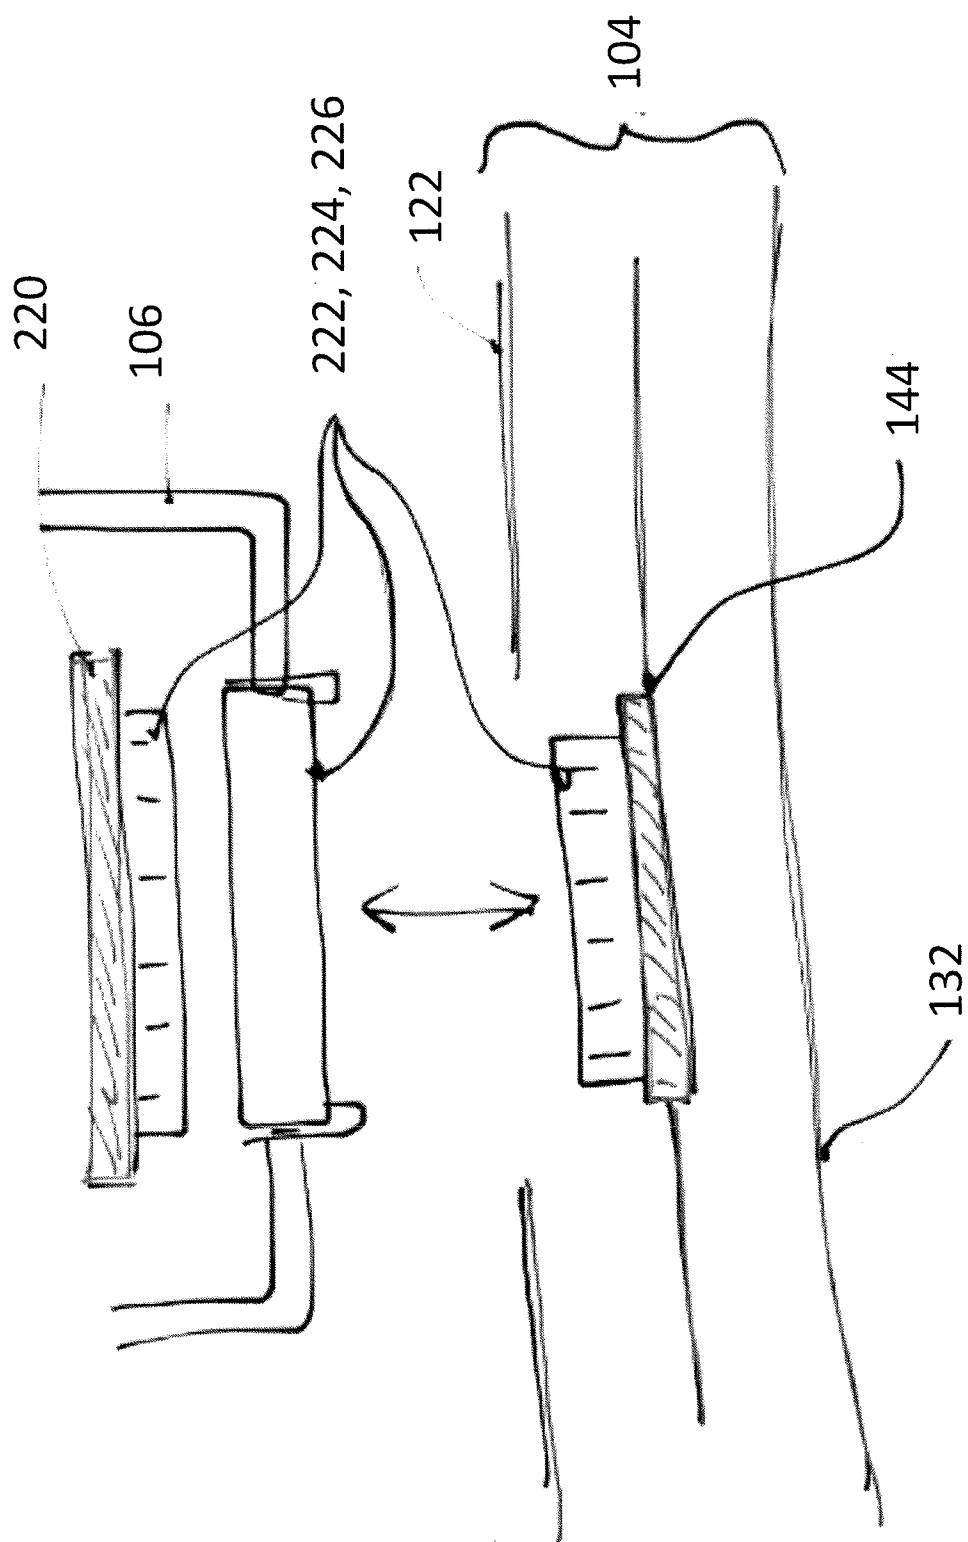


FIG. 10B

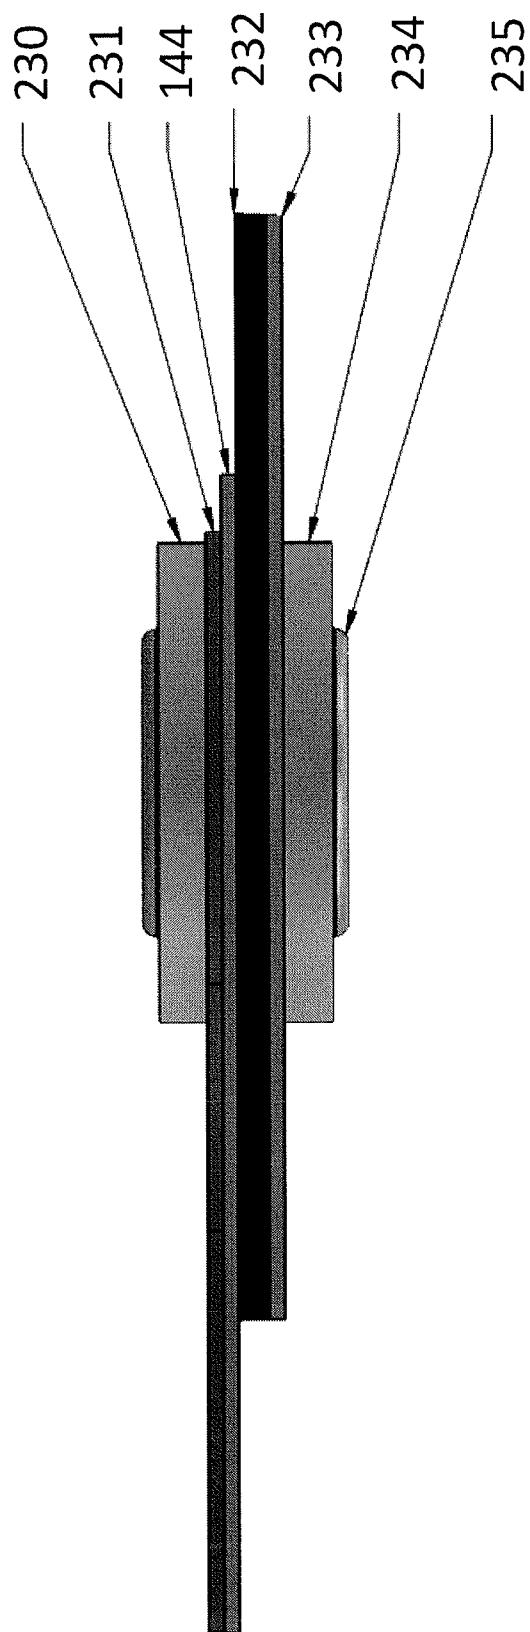


FIG. 10C

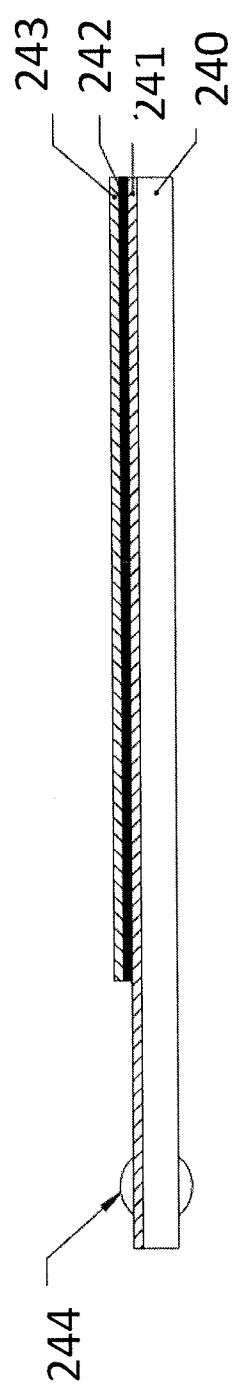


FIG. 11A

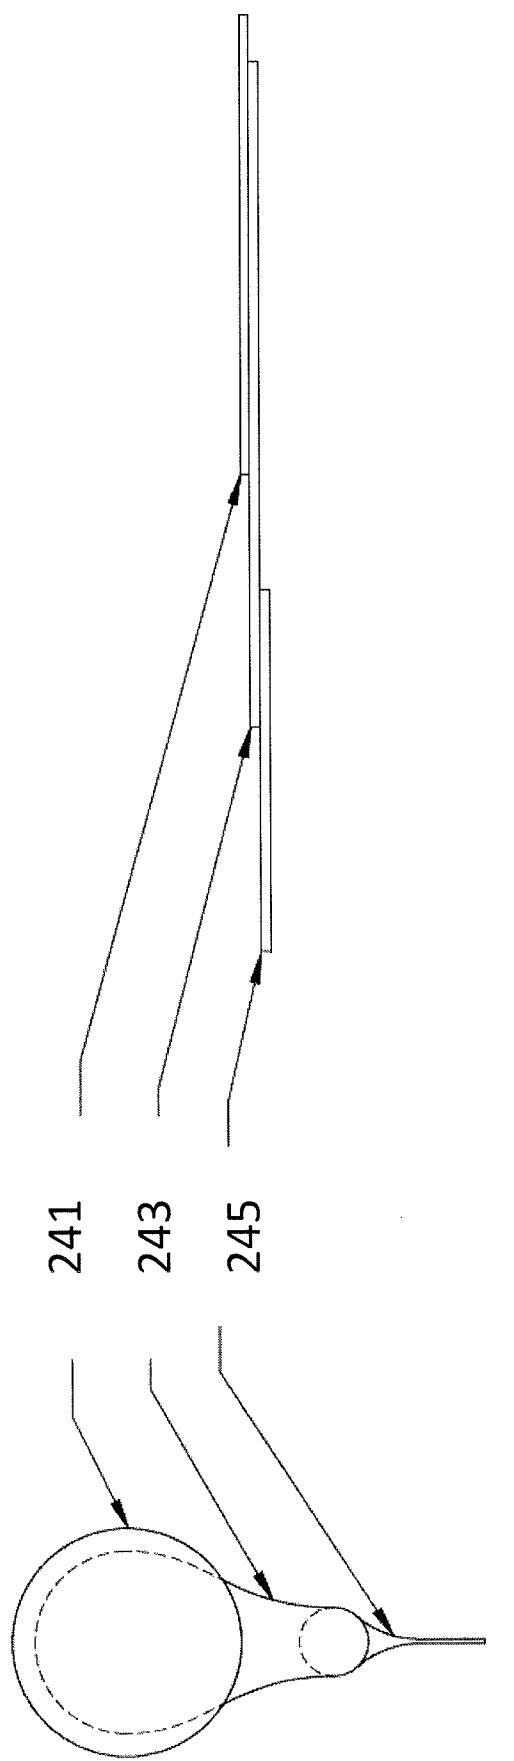


FIG. 11B

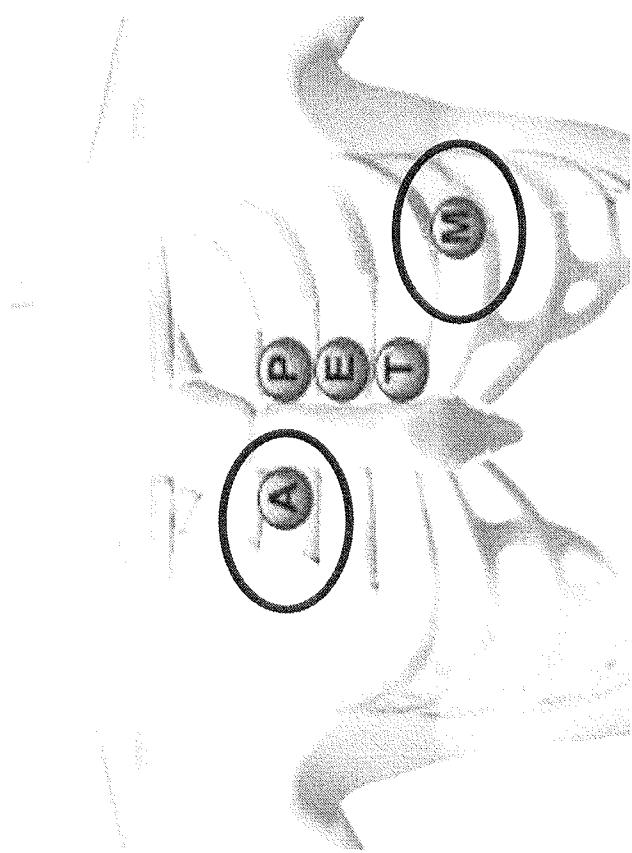


FIG. 12


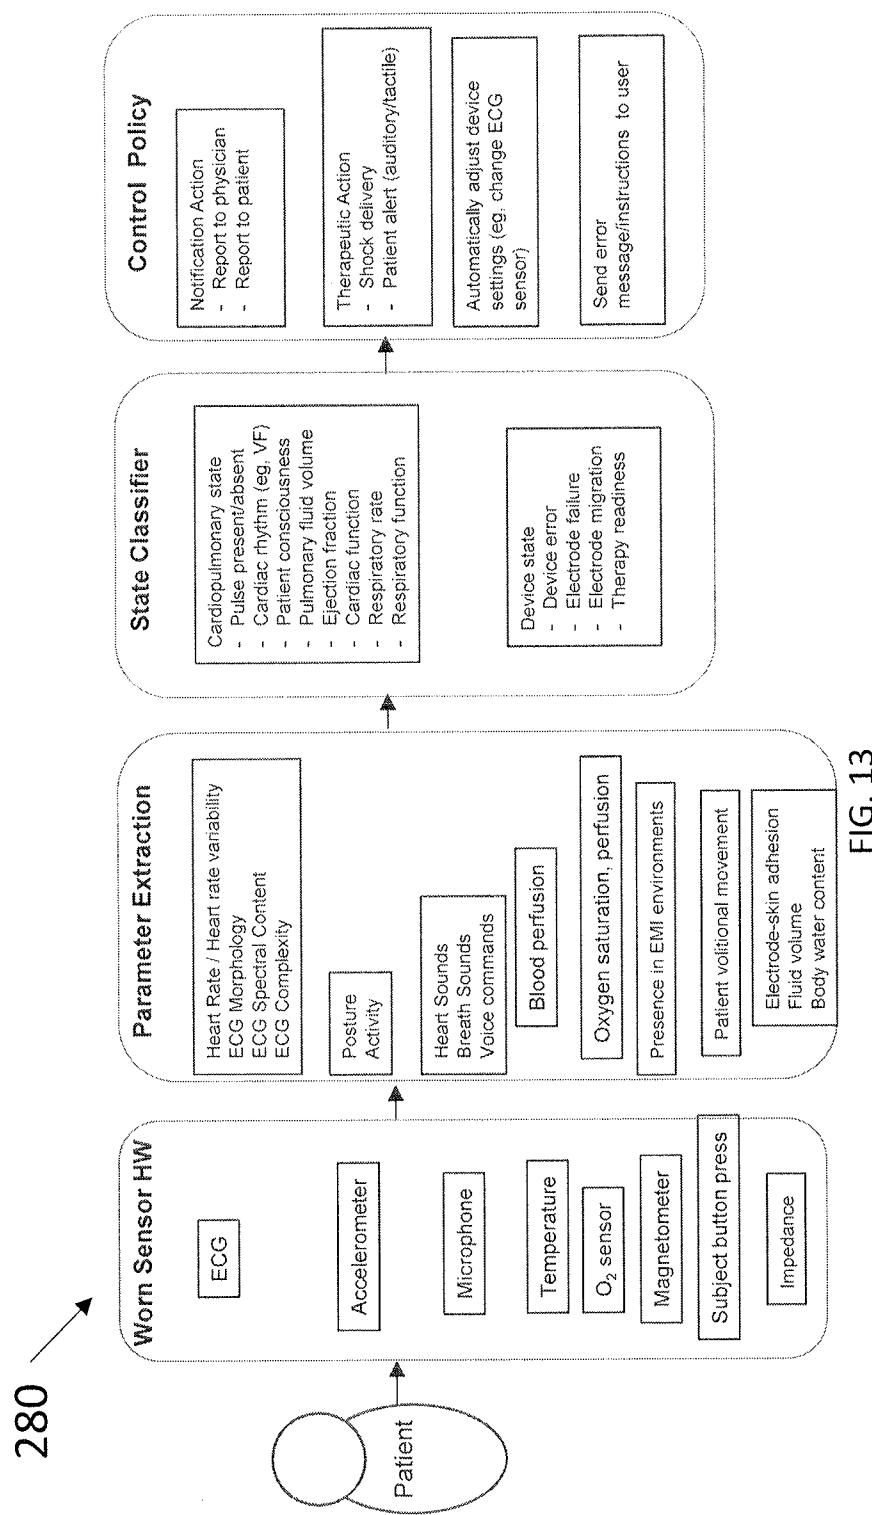


FIG. 13

300
FIG. 14
302

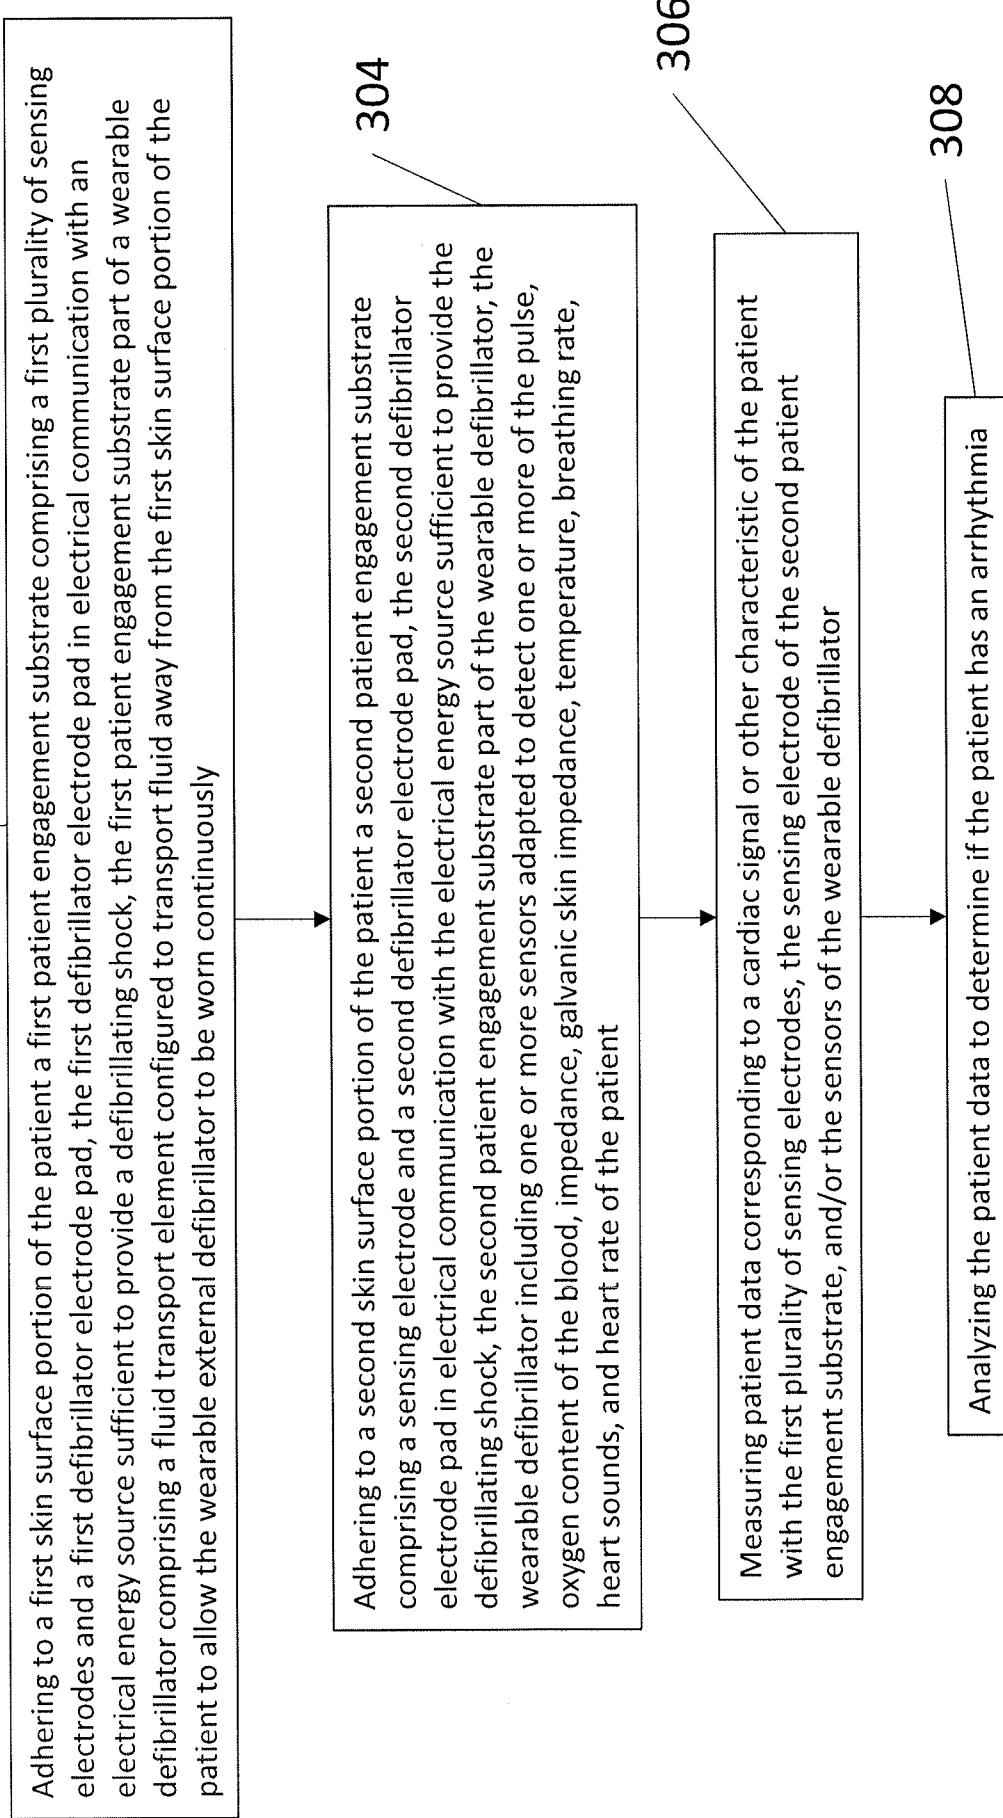

320 →

Measuring one or more of a heart rate, a breathing rate, a breathing pattern of the patient, an impedance across and through a chest and thoracic cavity of the patient, and a size of blood vessels within a body of the patient like an inferior vena cava, blood pressure waveform, lung sounds, patient posture and activity, and pulse oxygenation with a wearable device including one or more sensing electrodes and one or more sensors configured to measure the heart rate, breathing rate and pattern of the patient, the trans-thoracic impedance of the patient, and the size of the blood vessels in the body, blood pressure, wherein the wearable device is adhesively attached to a portion of the skin of the patient

322

Analyzing the one or more of the measured heart rate, oxygen saturation, ECG rhythm, ECG morphology, ECG amplitude, chest movement, breathing rate, breathing pattern, trans-thoracic impedance, blood pressure and blood pressure waveform in different body postures, and size of the blood vessels in the body to detect a symptom or indication of cardiac disease in the patient

324

FIG. 15A

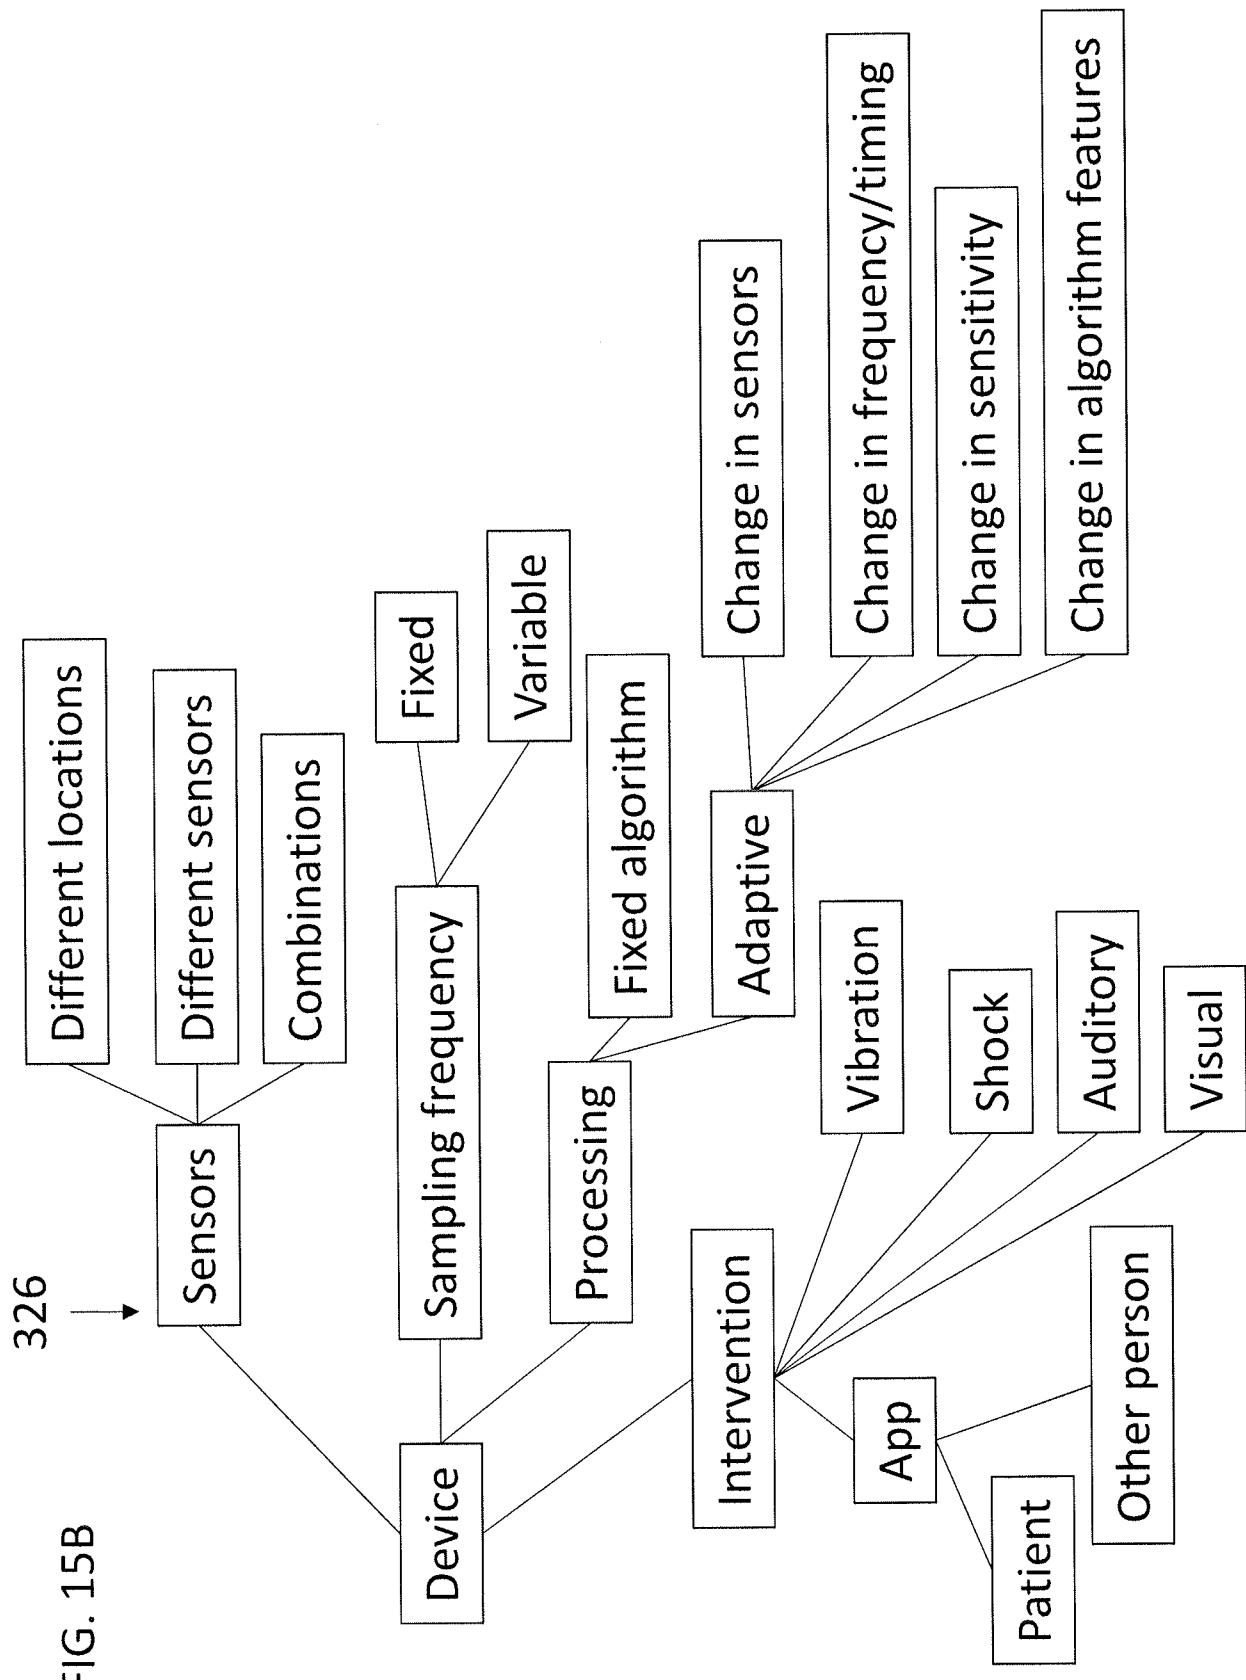
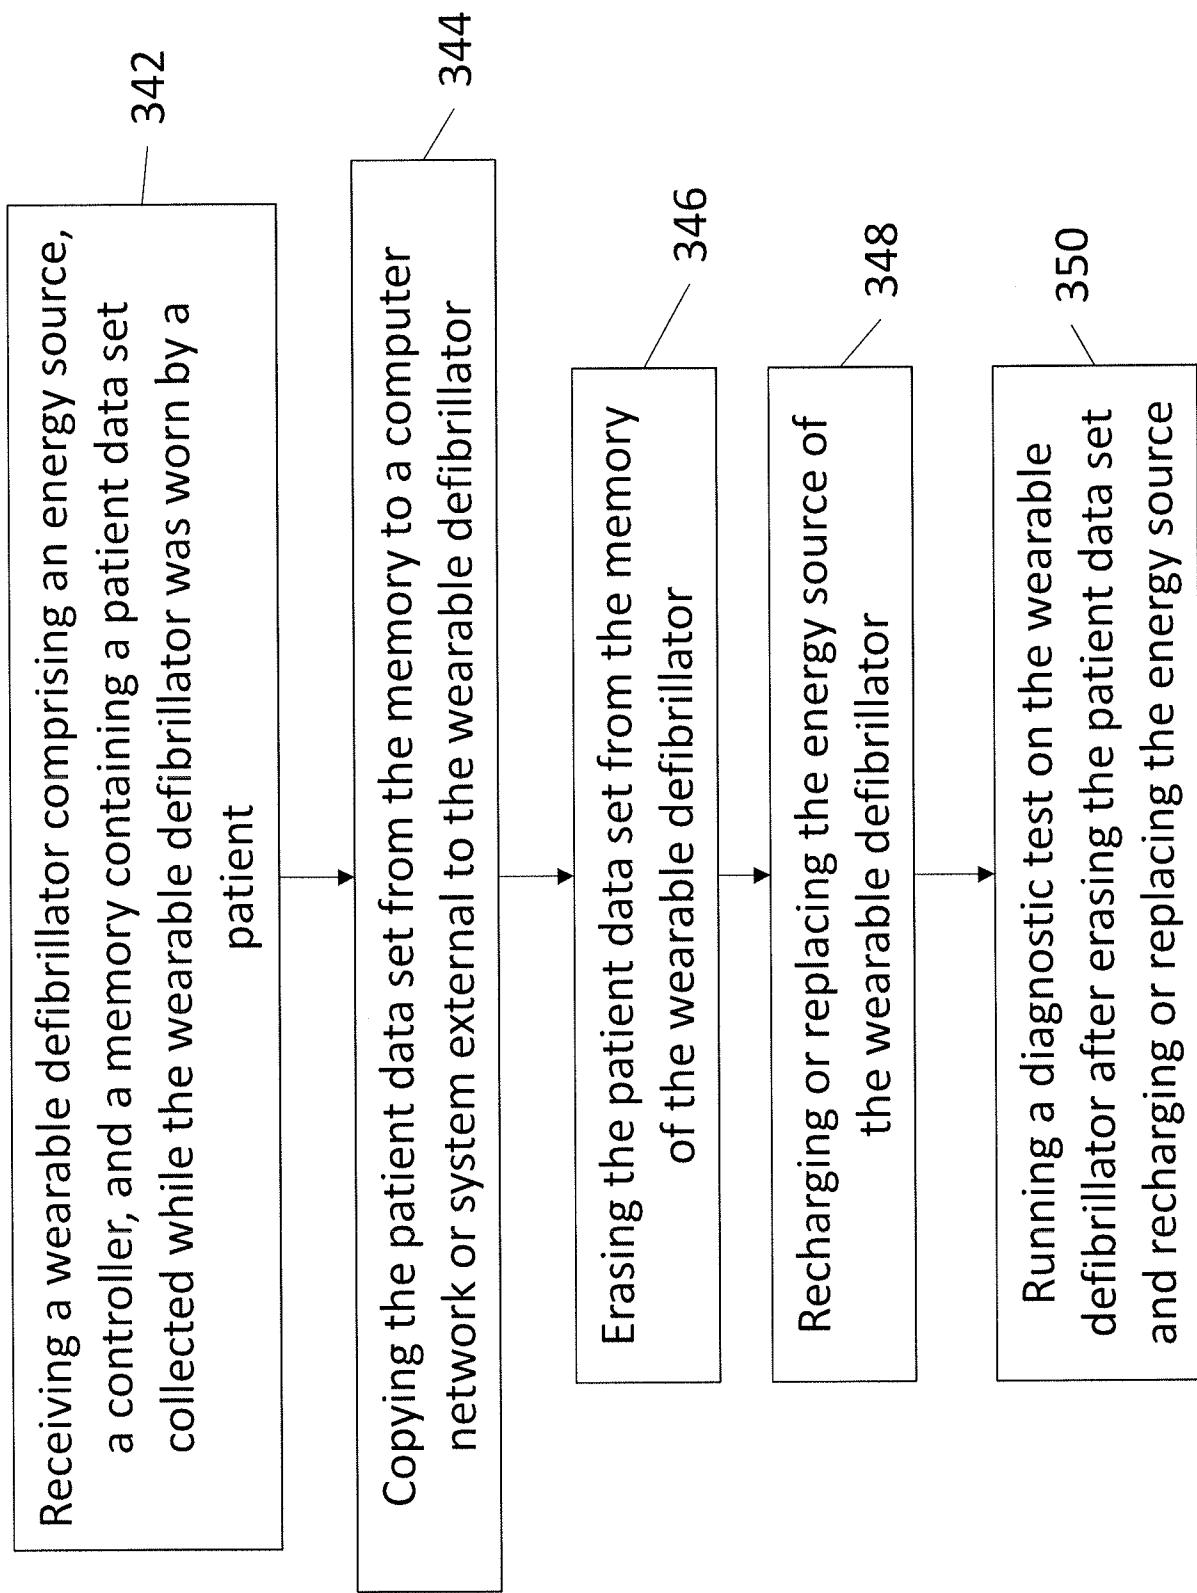
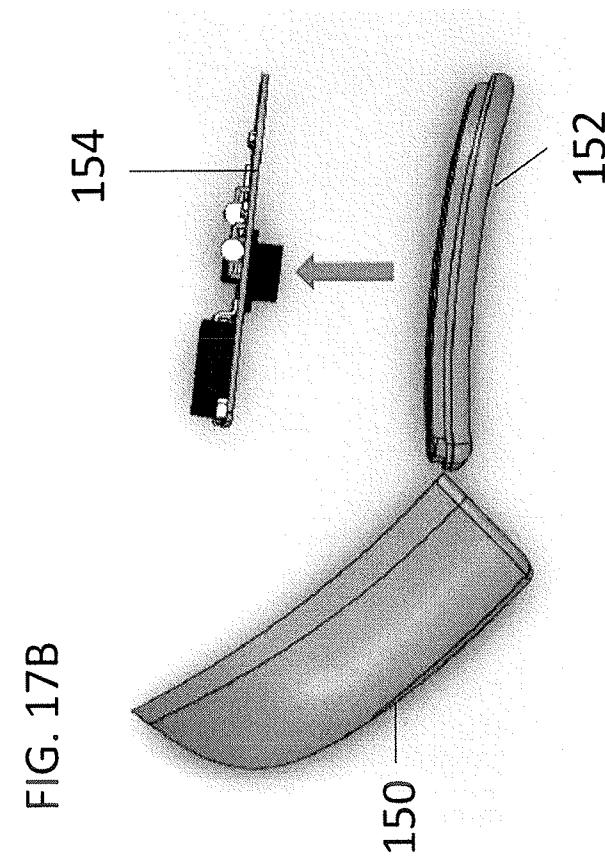
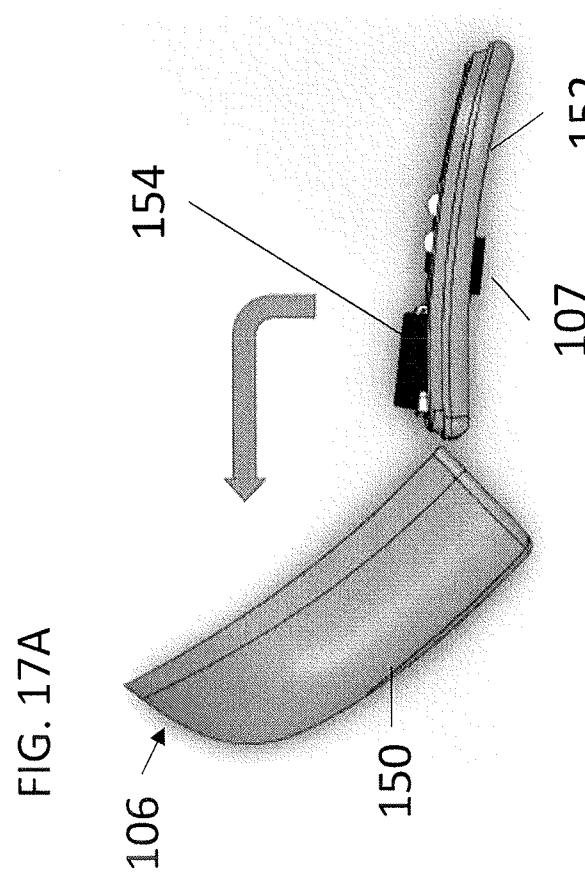
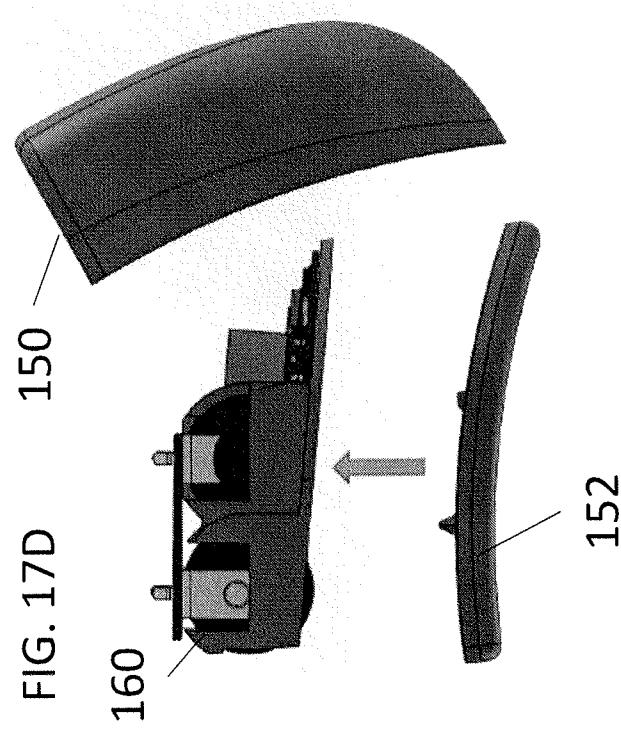
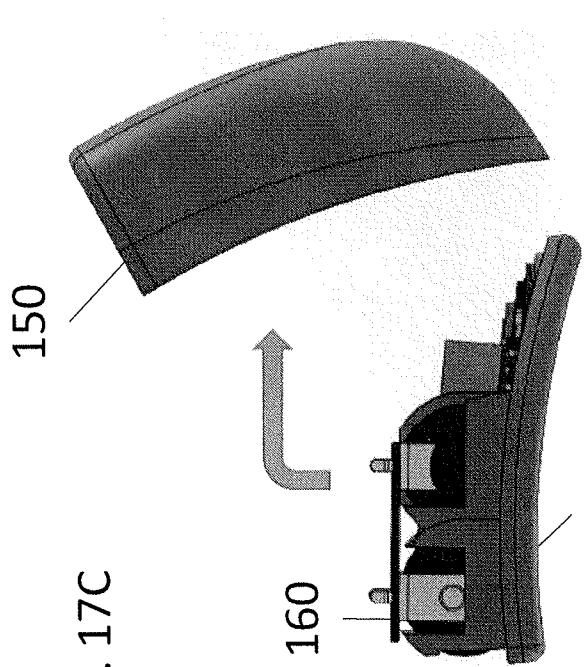


FIG. 16 340 ↗





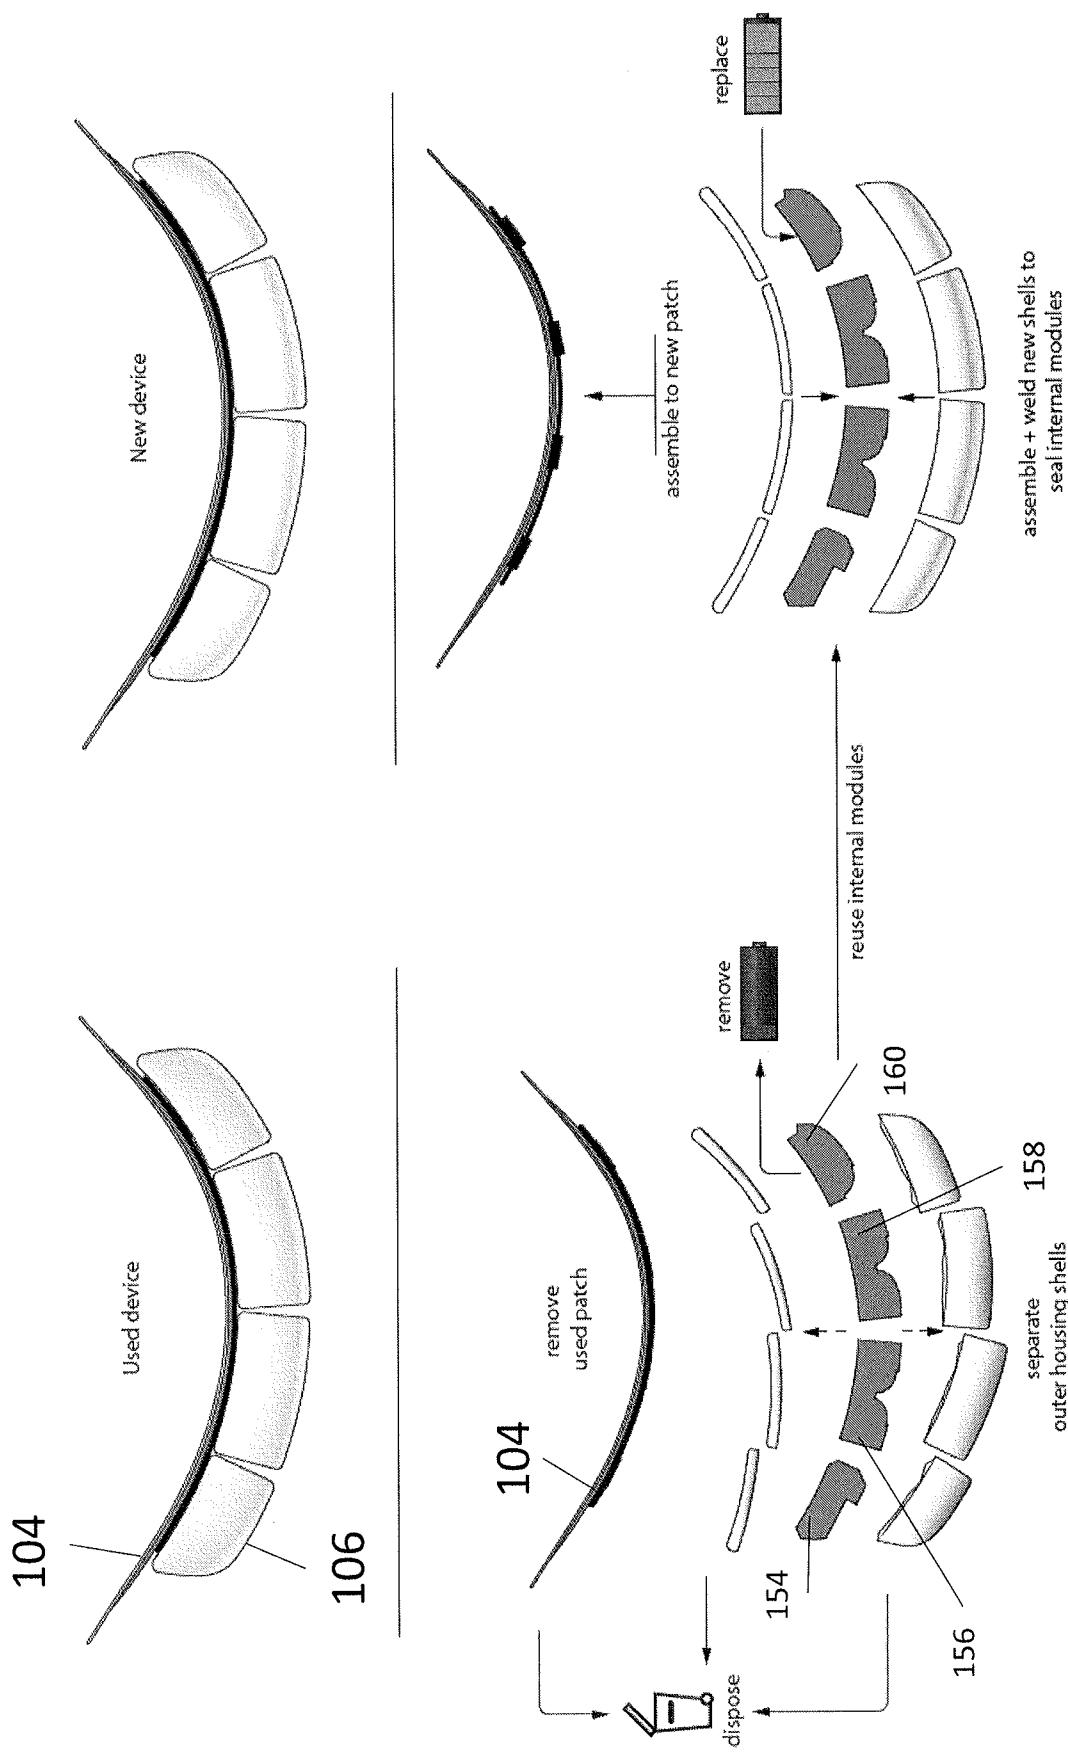


FIG. 18

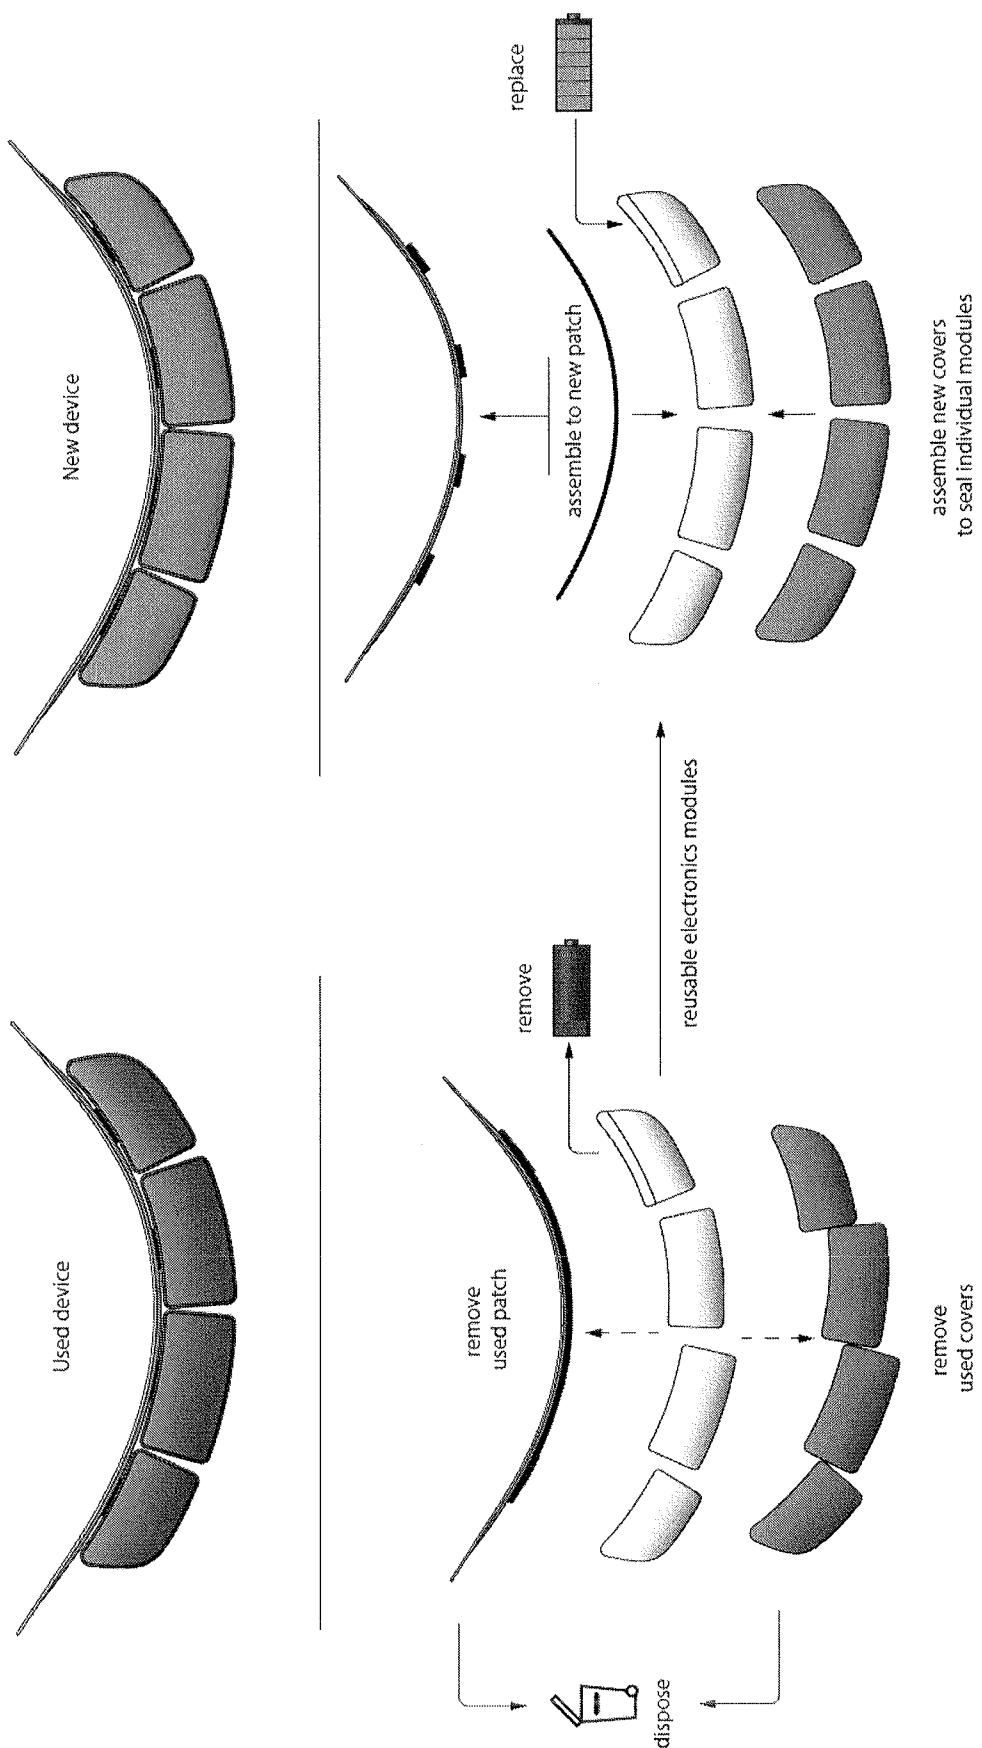


FIG. 19

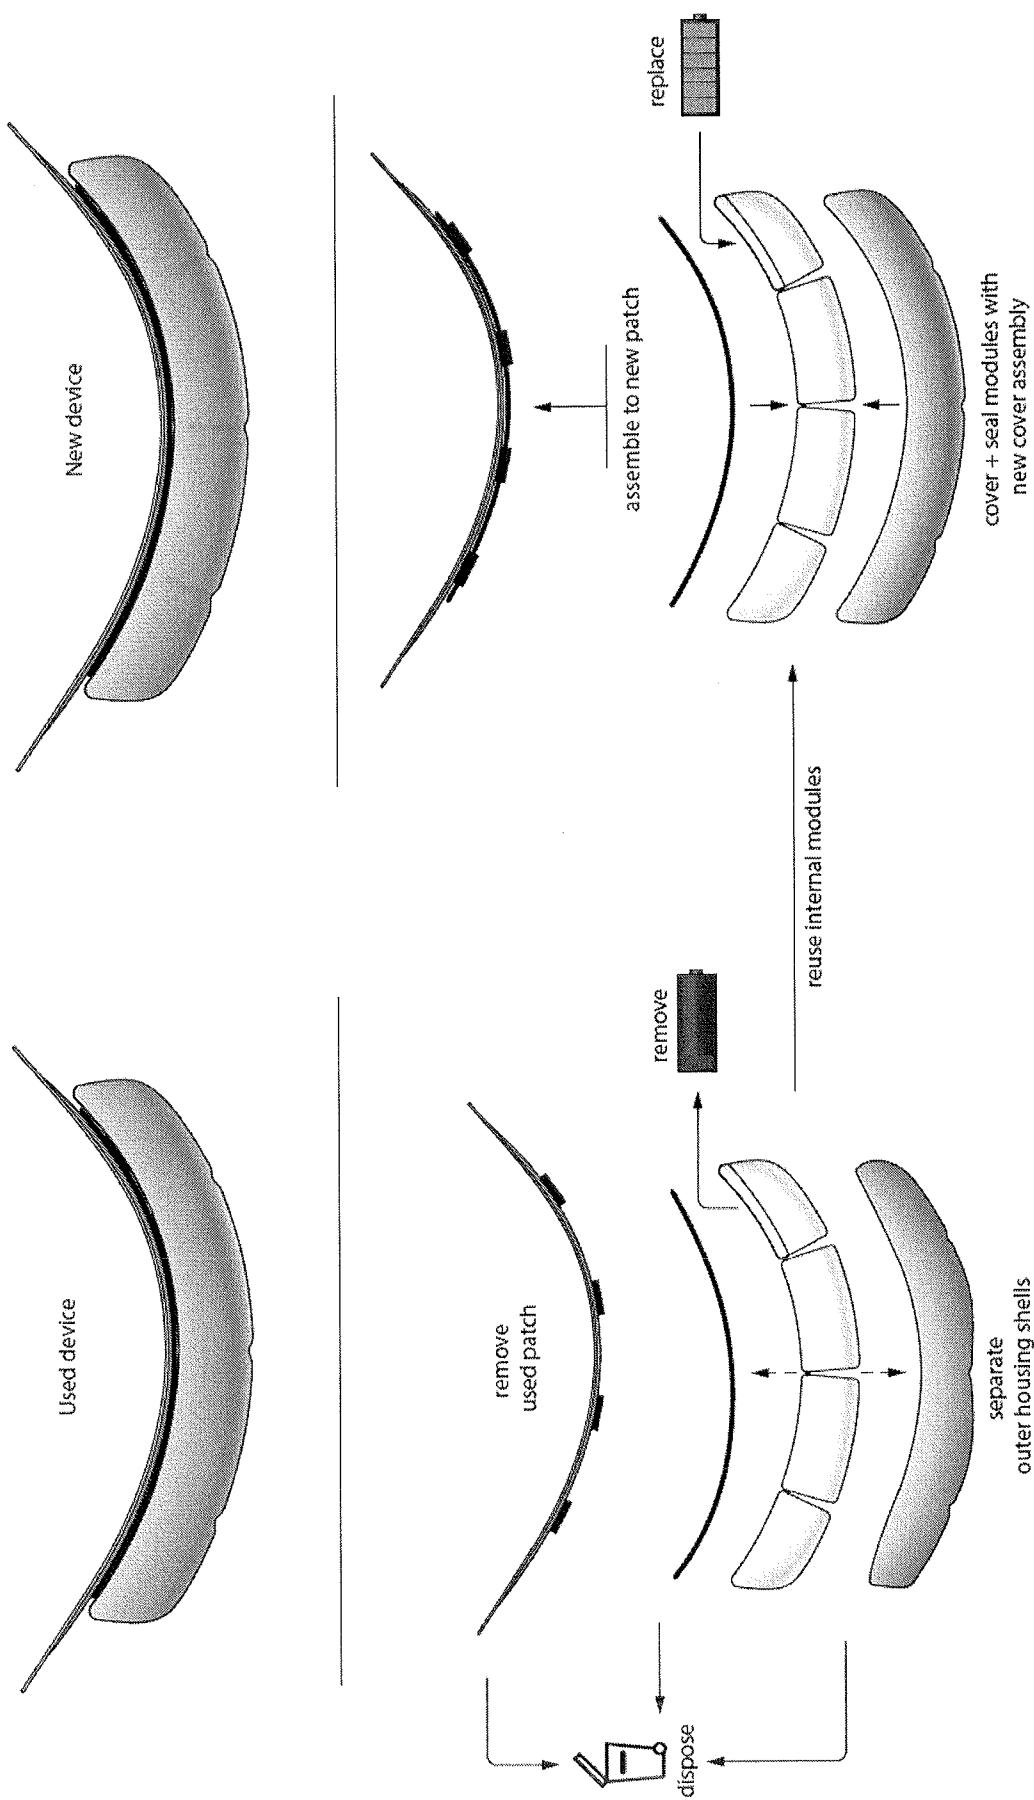


FIG. 20

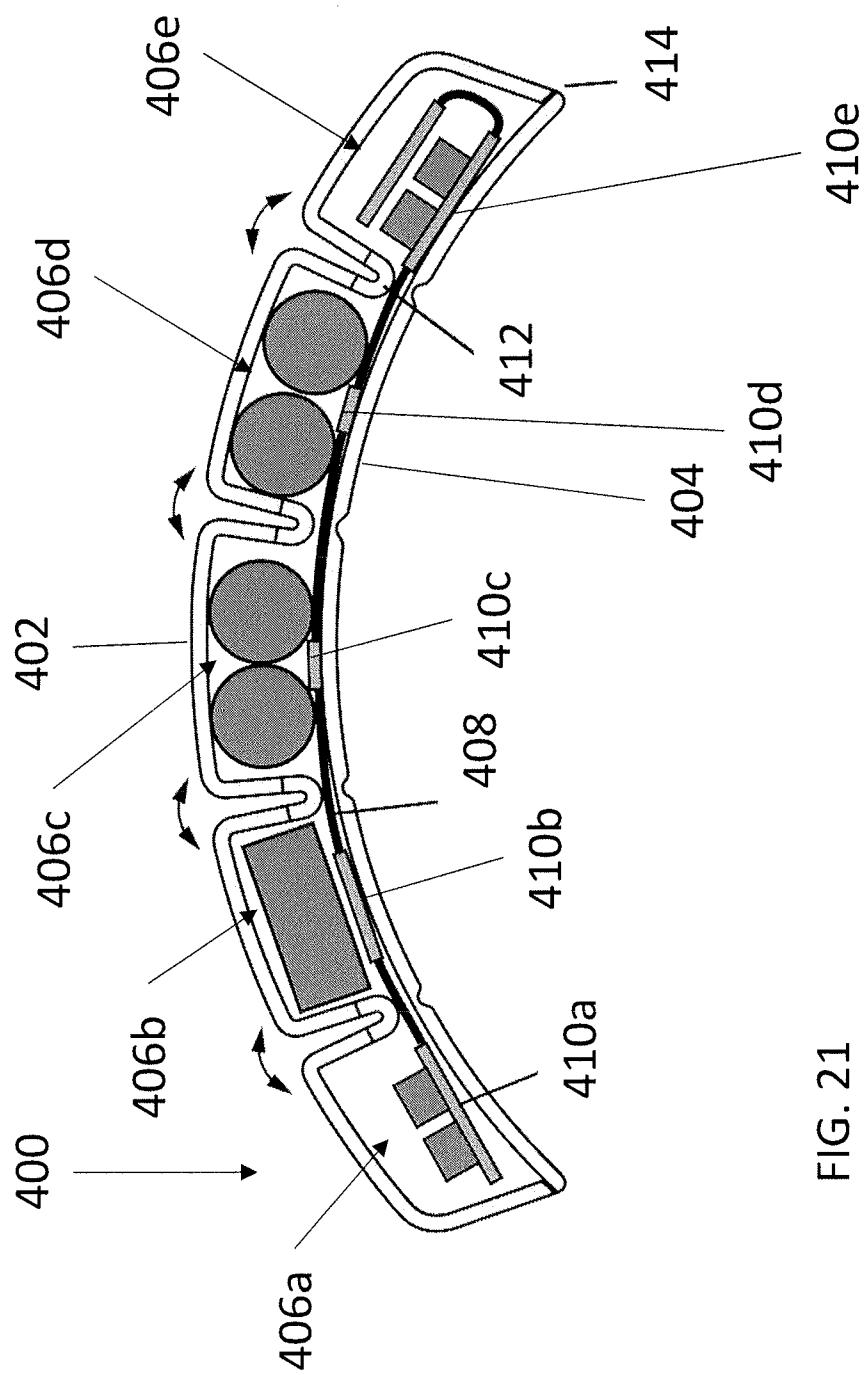


FIG. 21

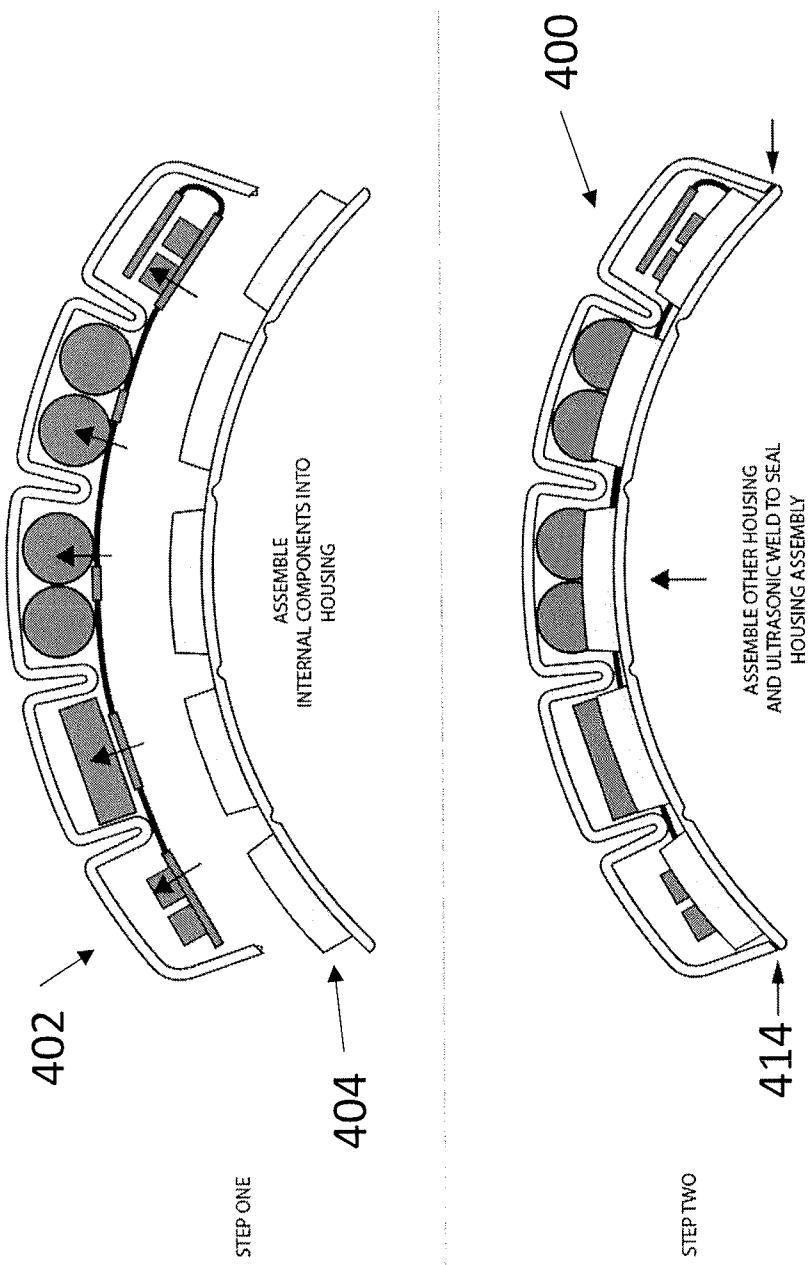


FIG. 22

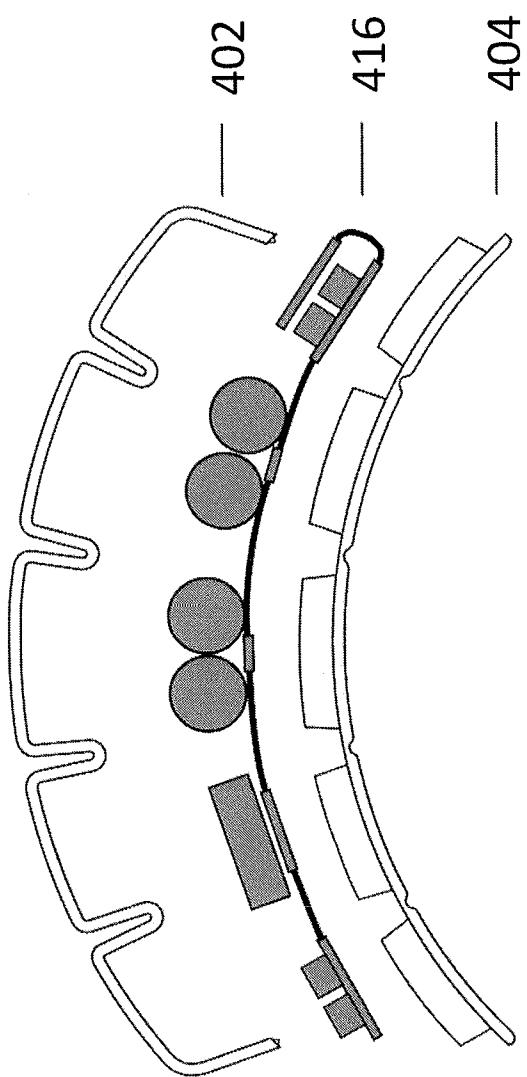
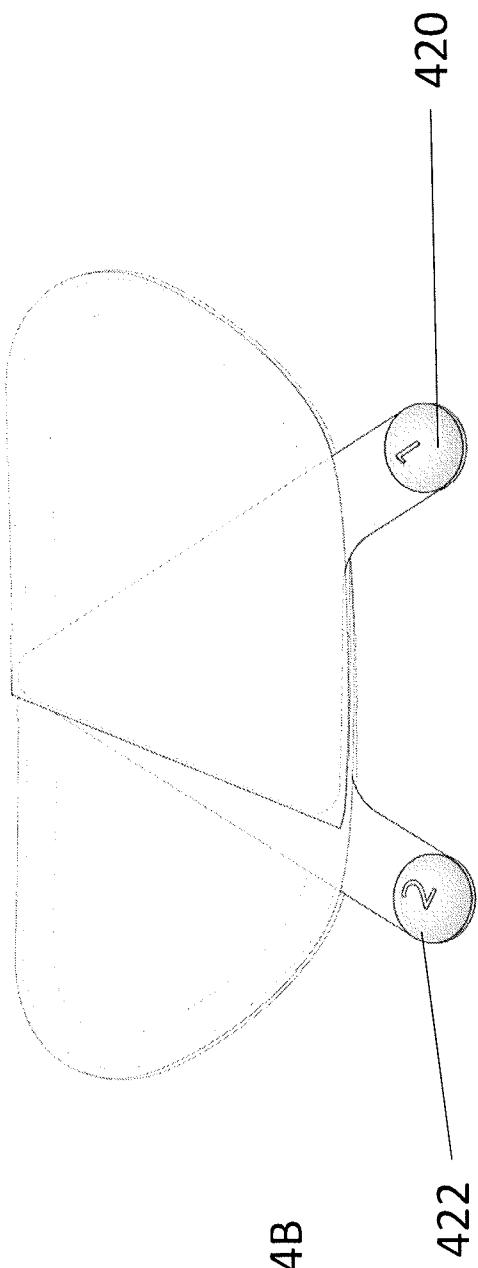
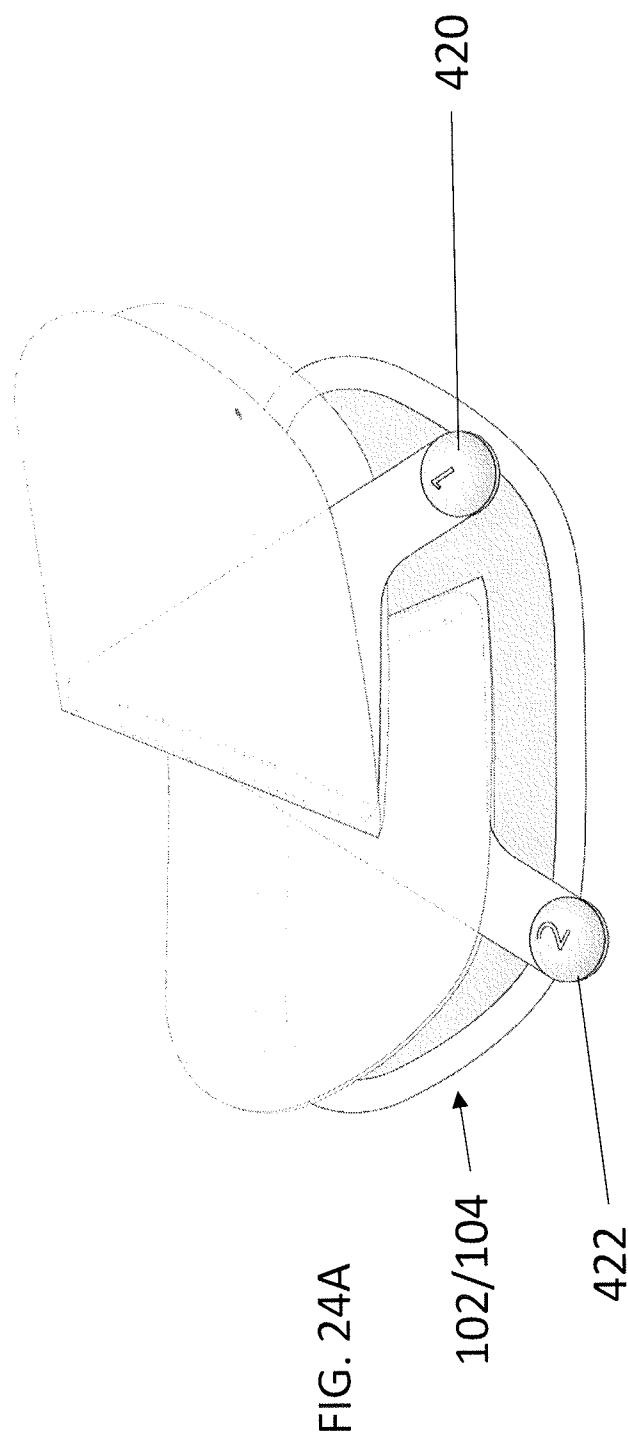


FIG. 23



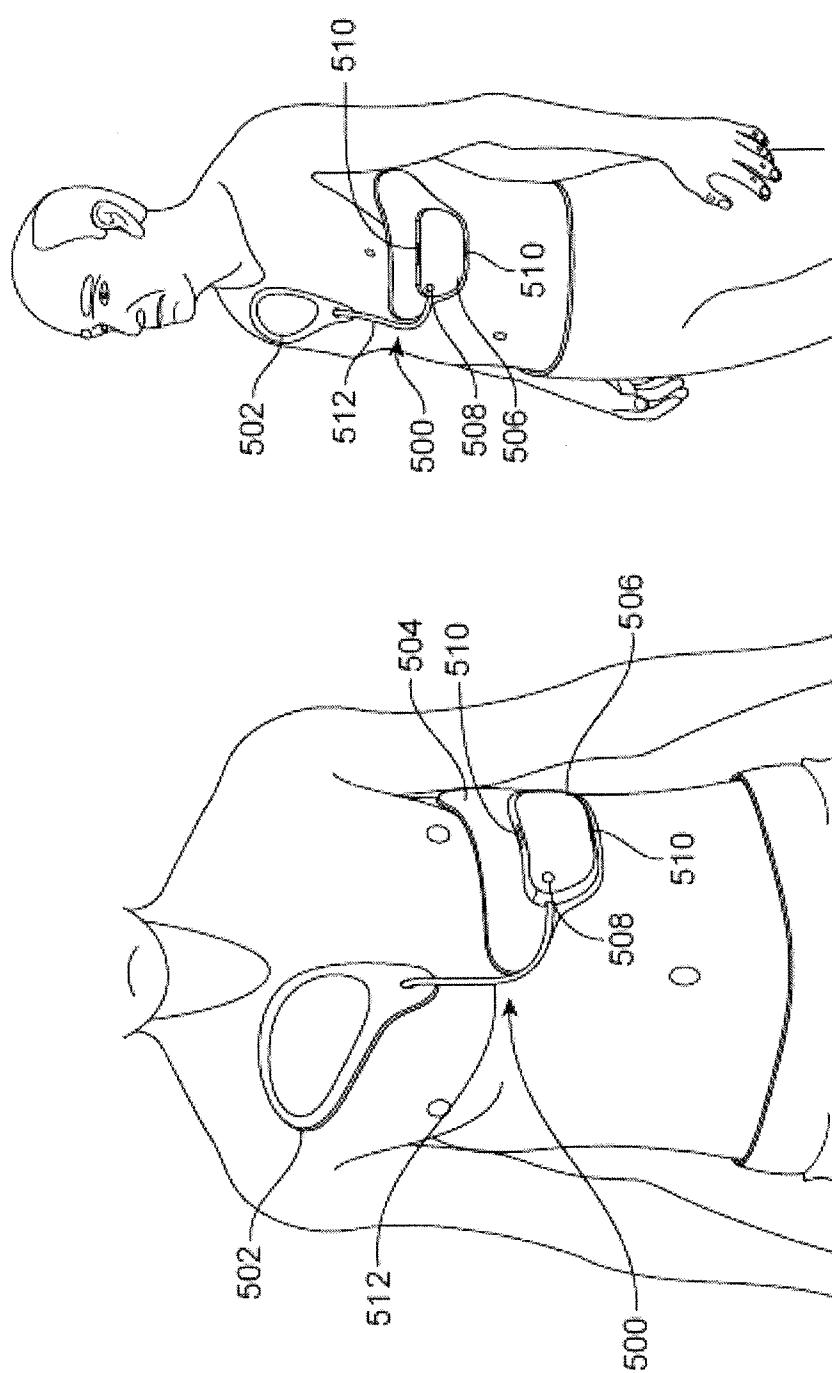


FIG. 25

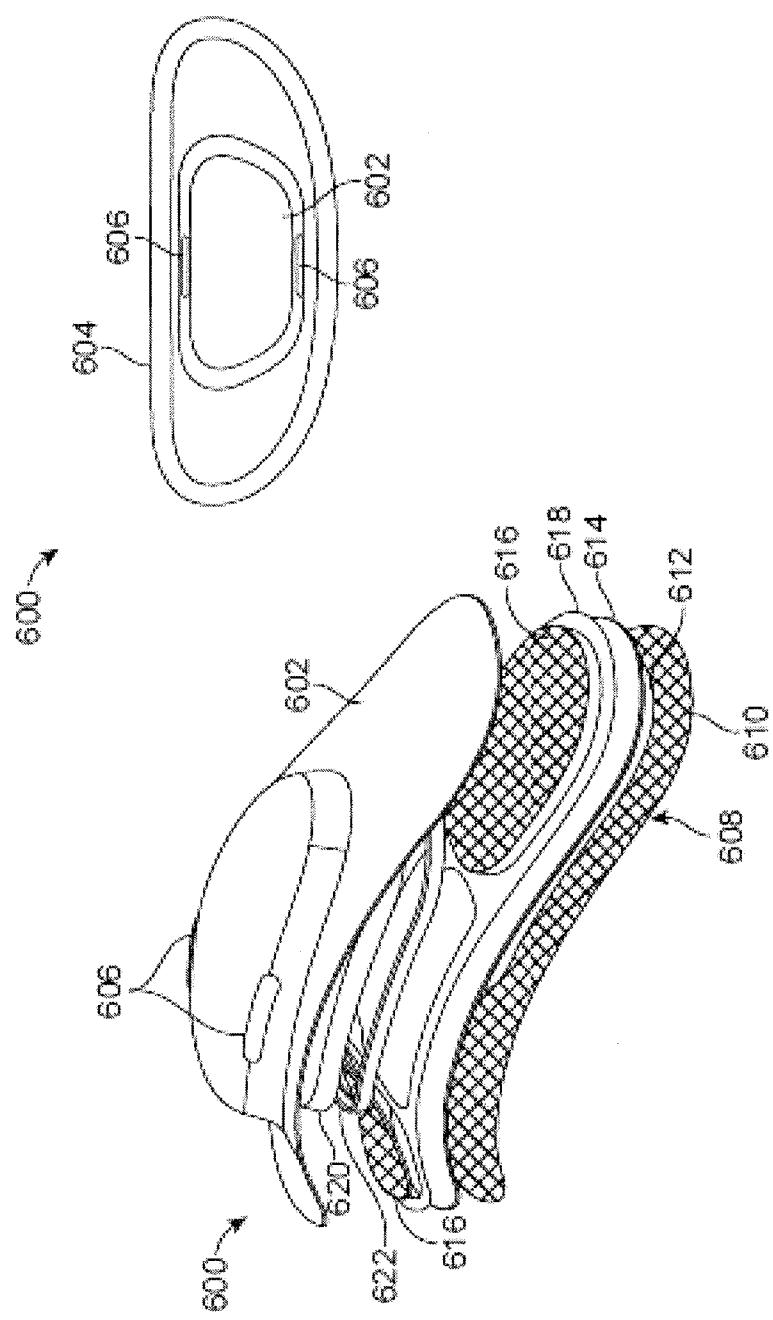


FIG. 26

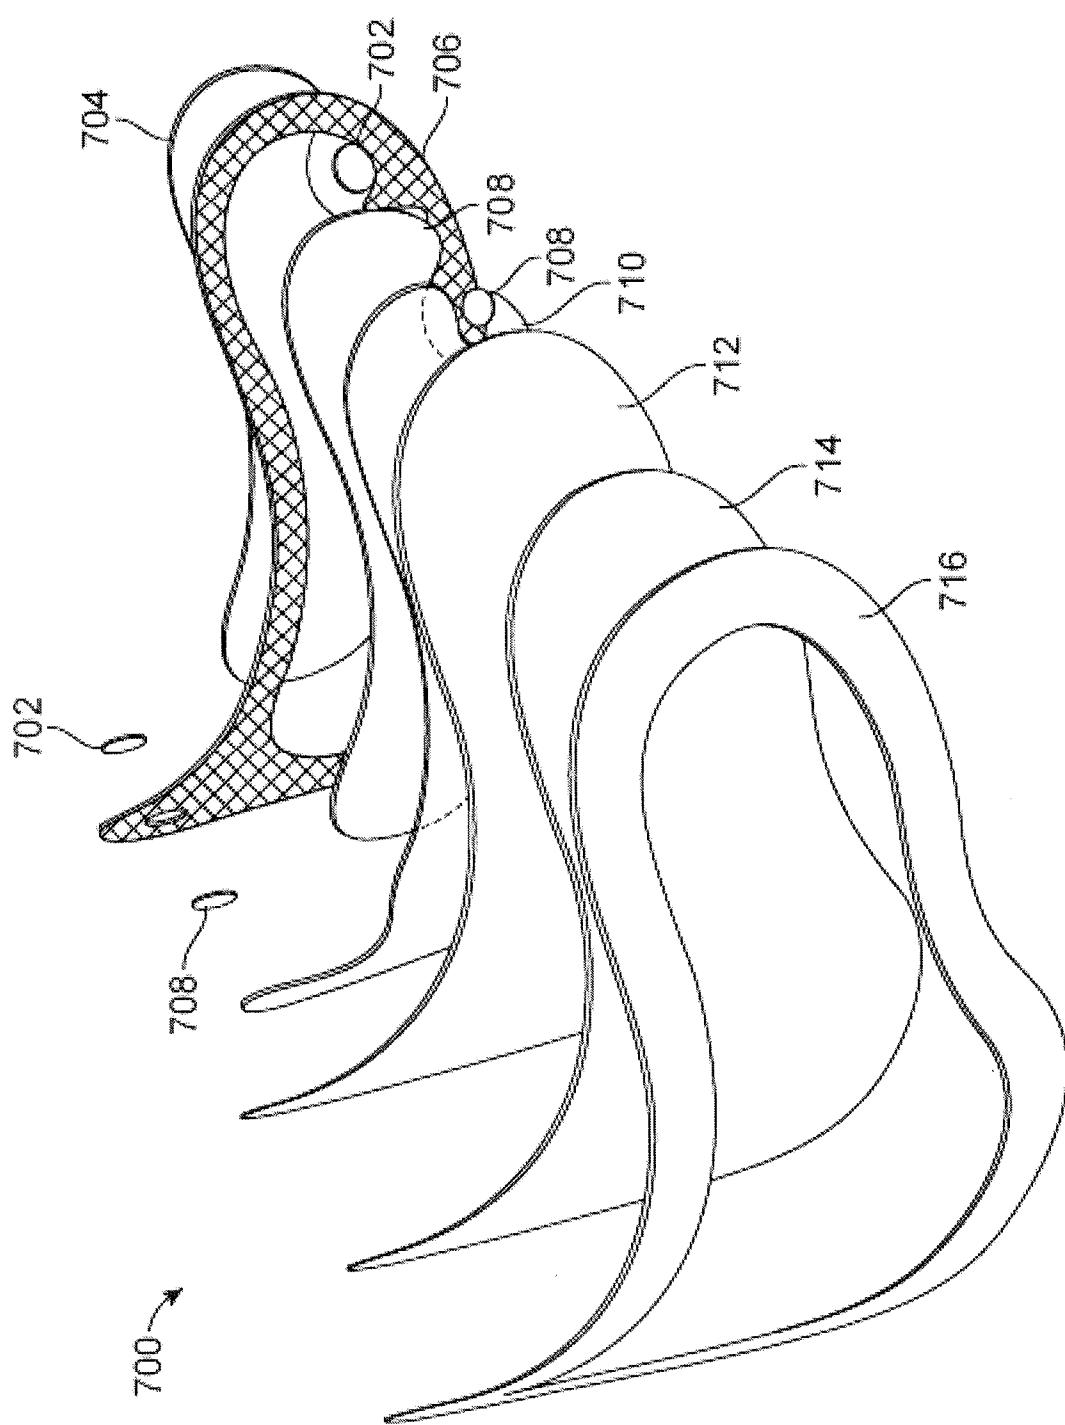


FIG. 27

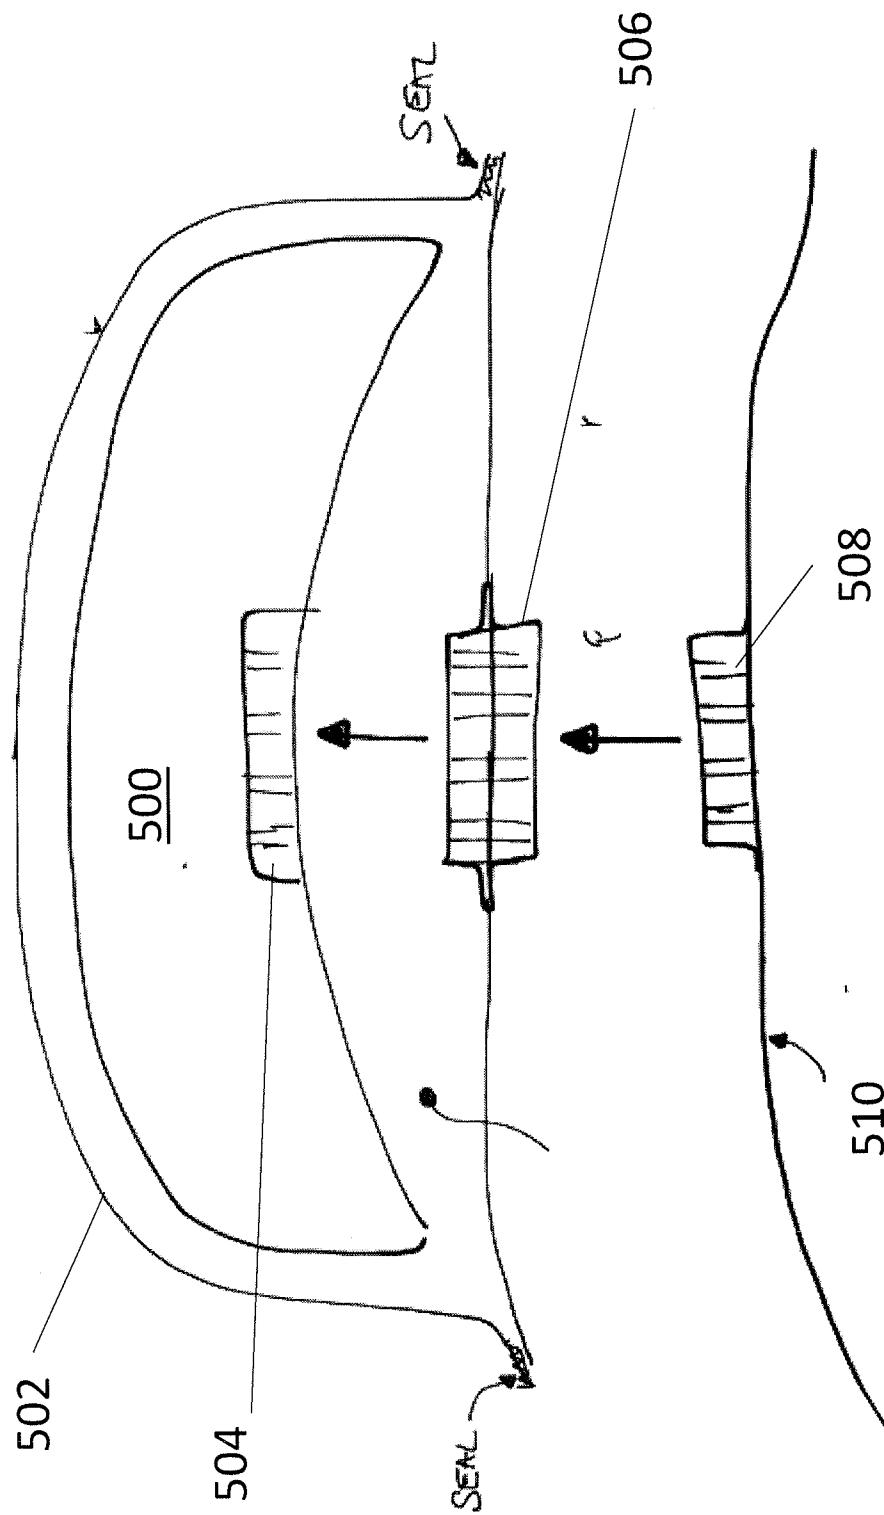


FIG. 28

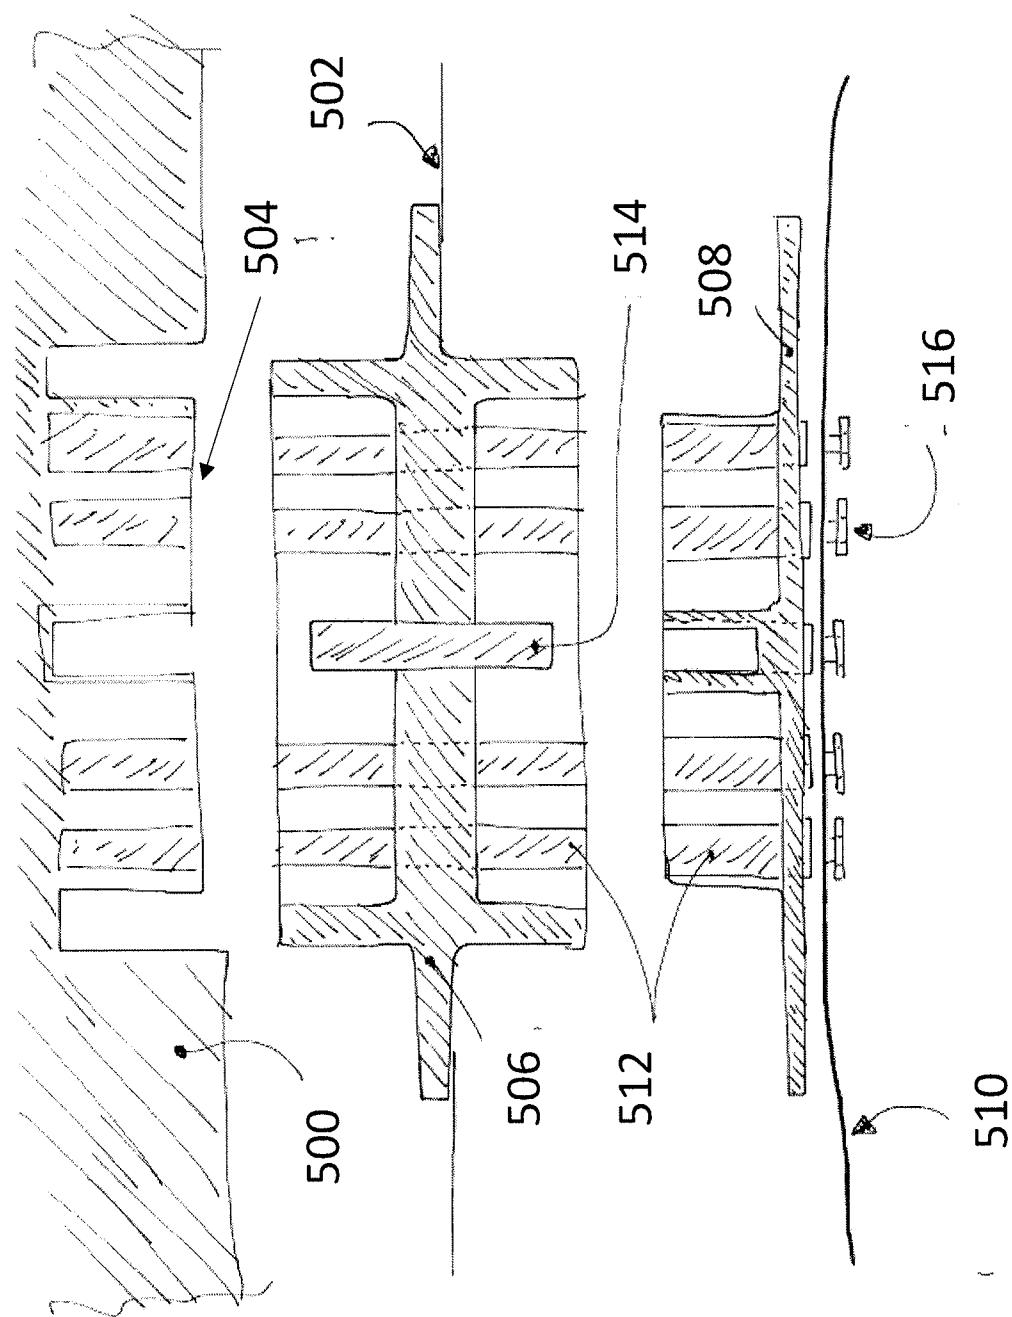


FIG. 29

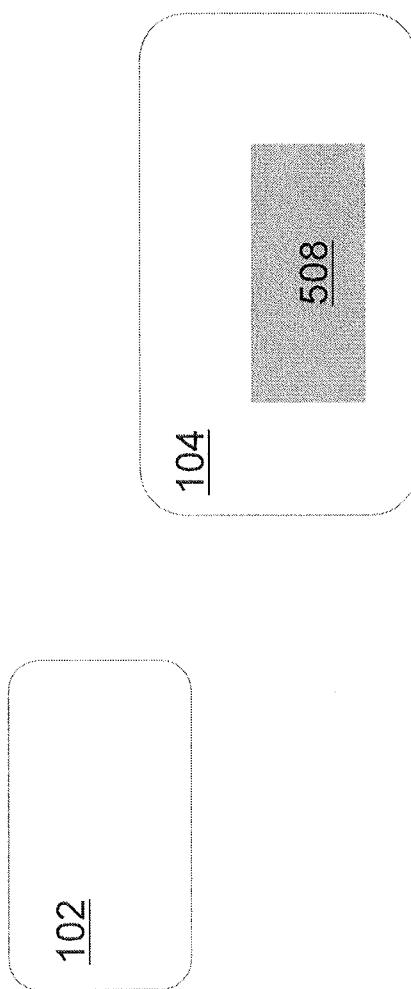


FIG. 30

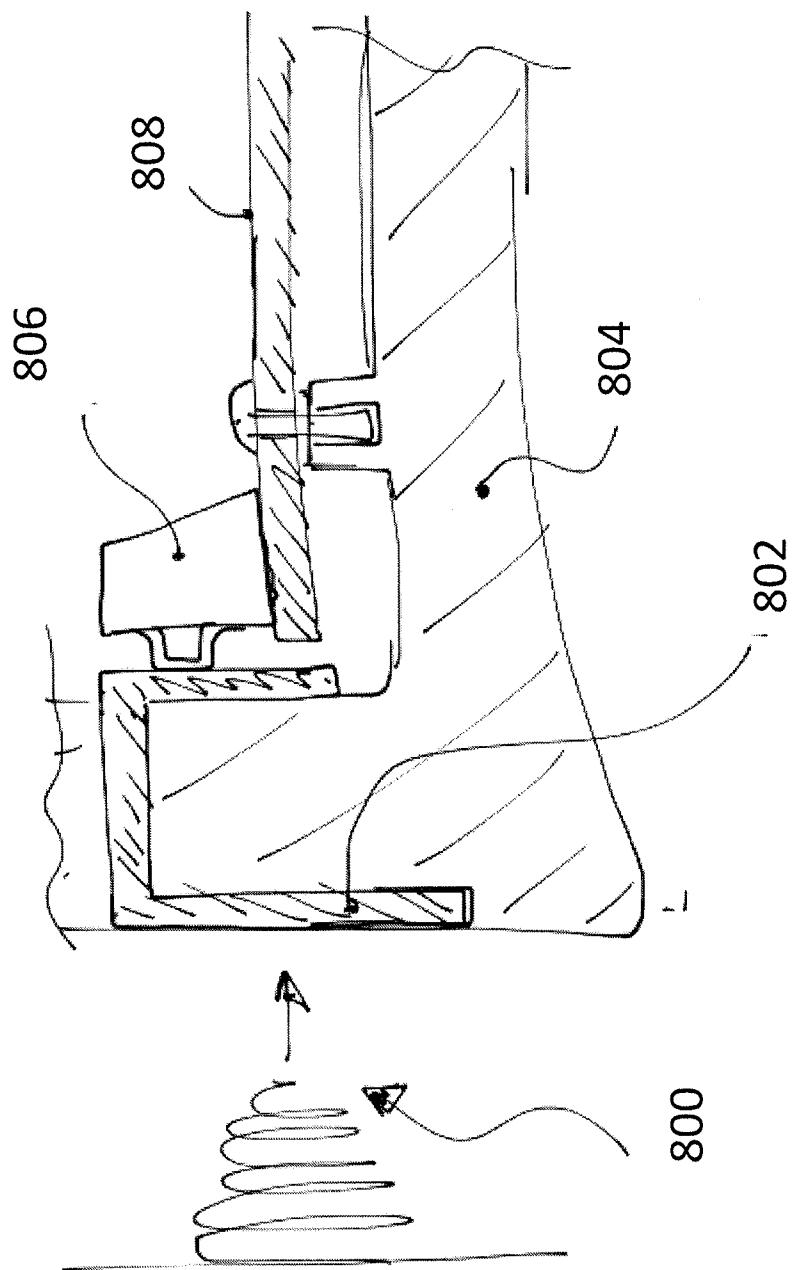


FIG. 31

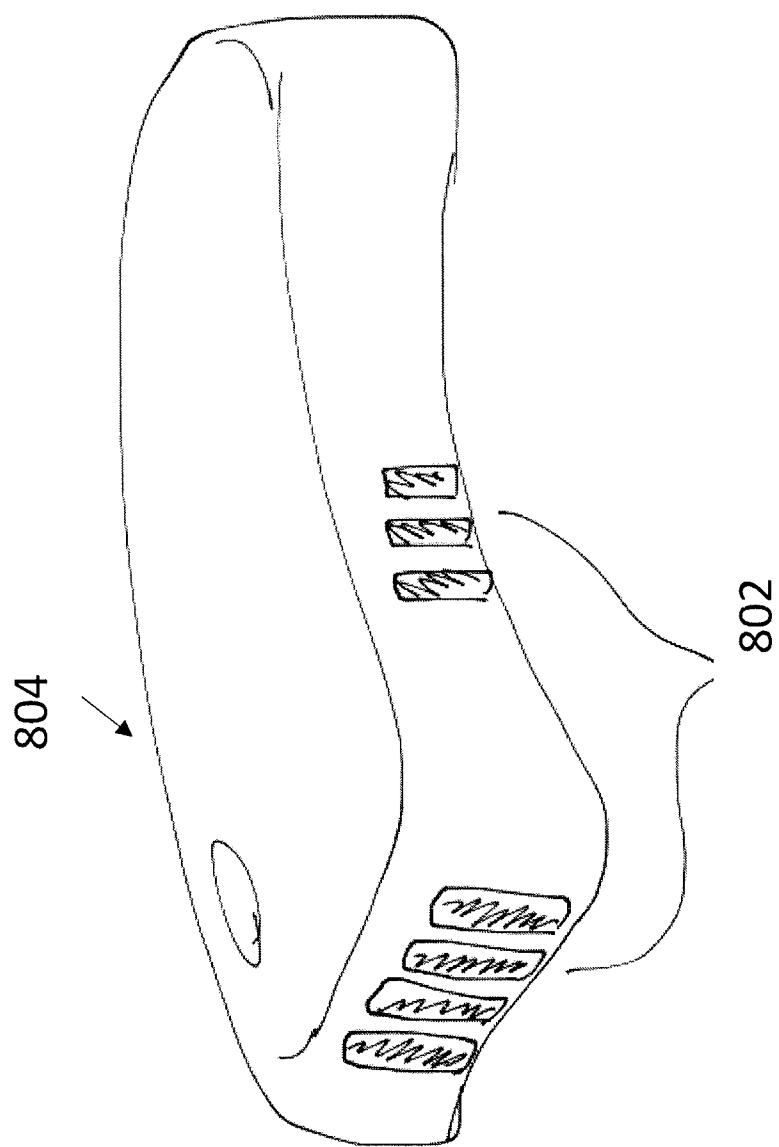


FIG. 32

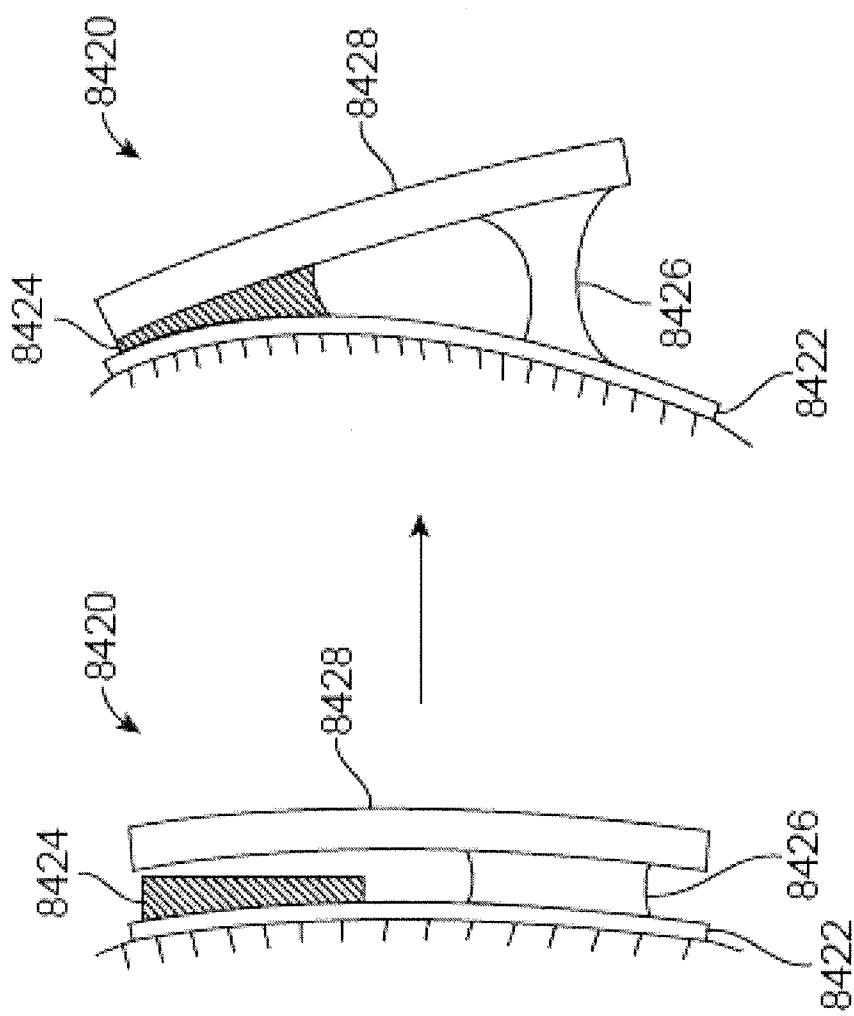


FIG. 33

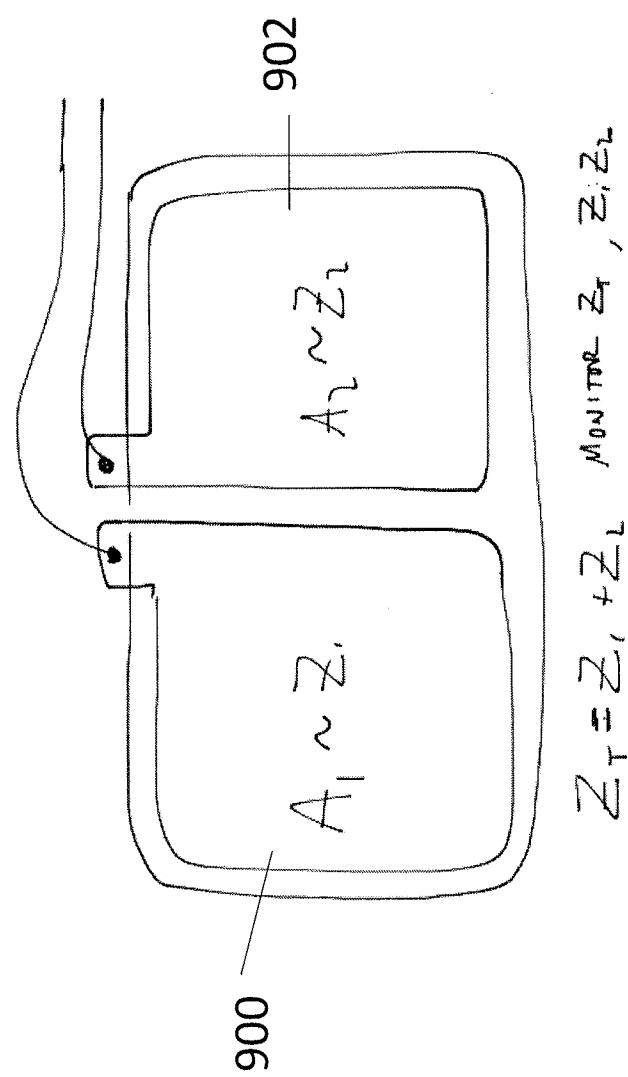


FIG. 34

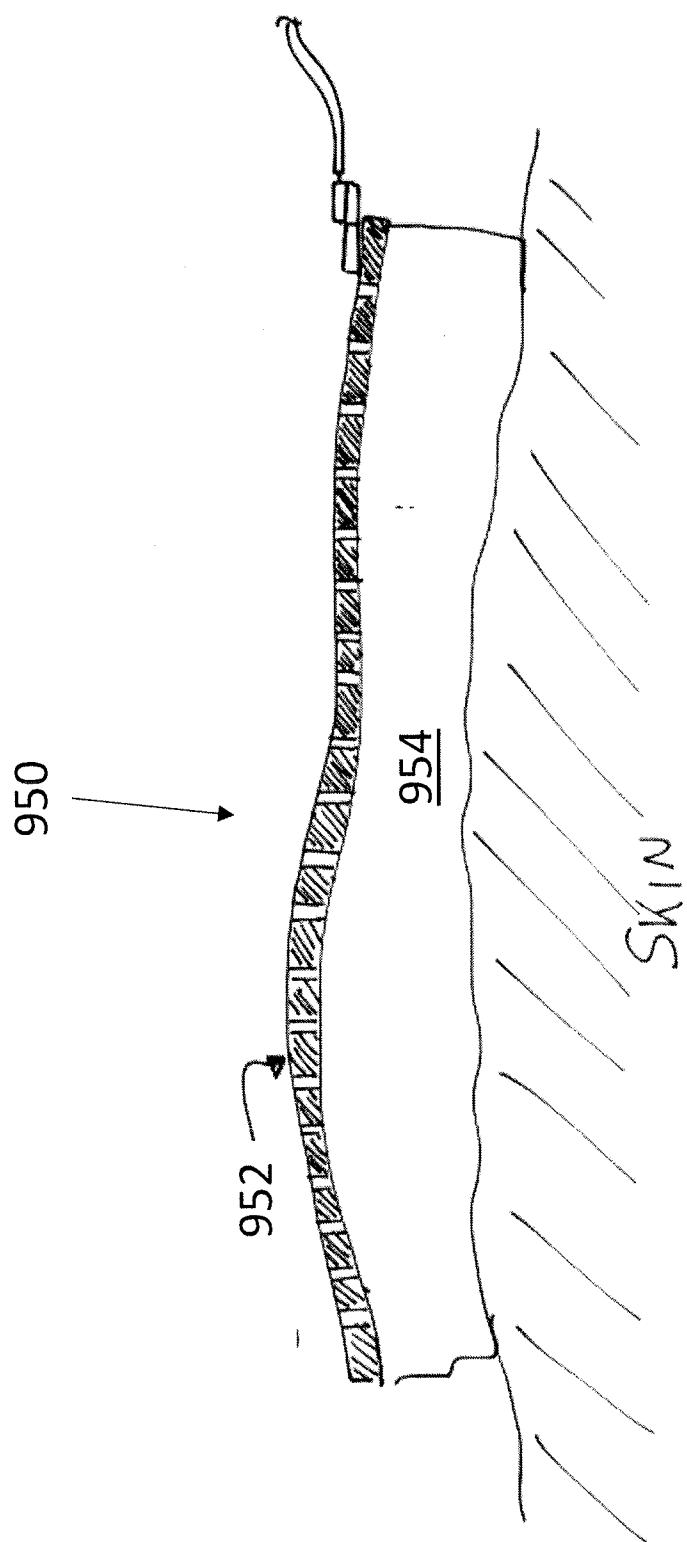


FIG. 35

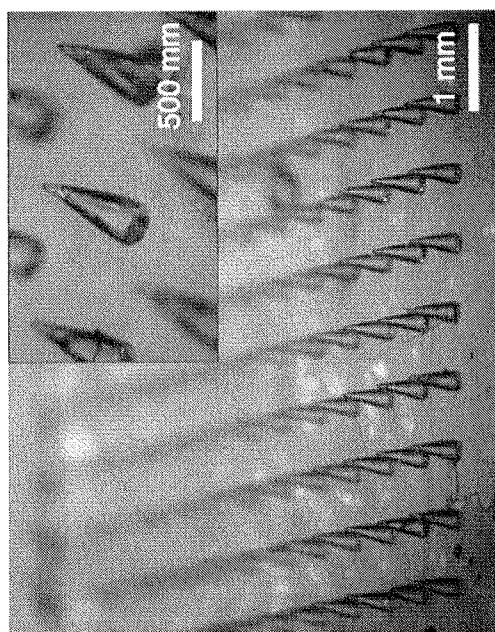
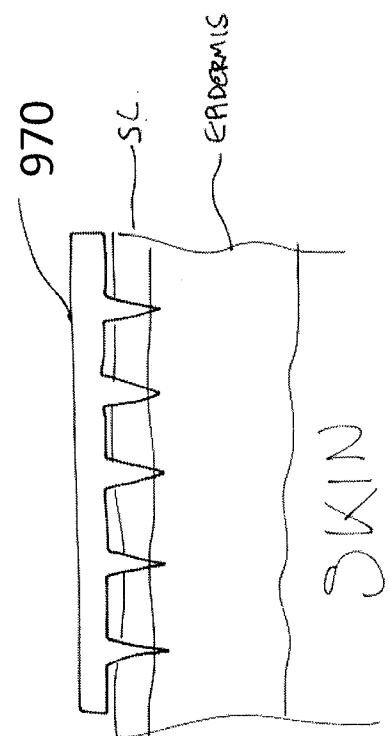


FIG. 36

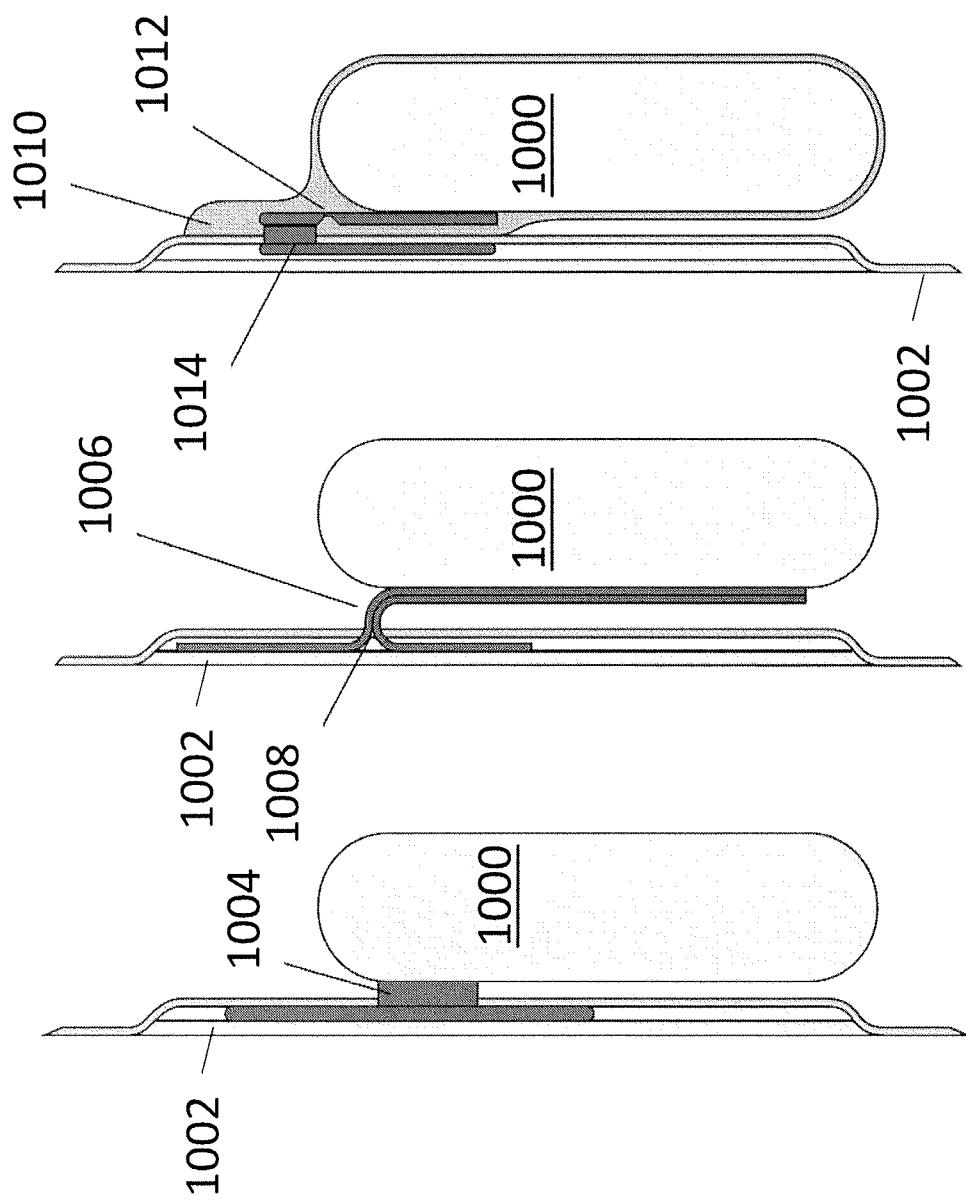


FIG. 37A

FIG. 37B

FIG. 37C

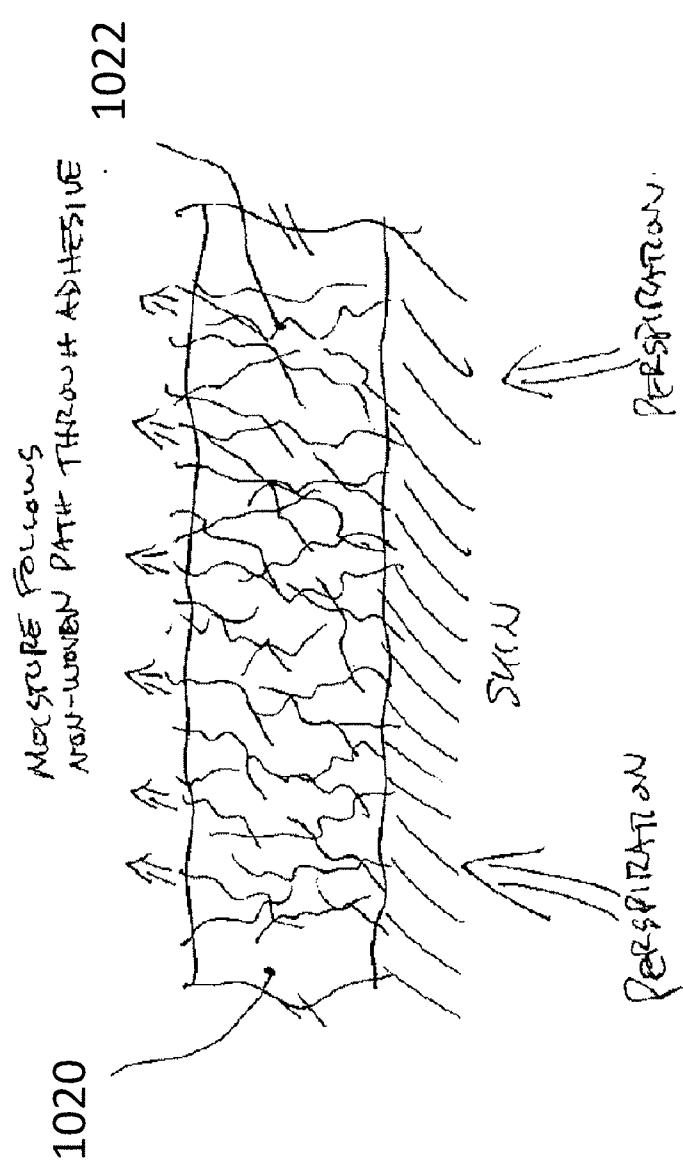


FIG. 38

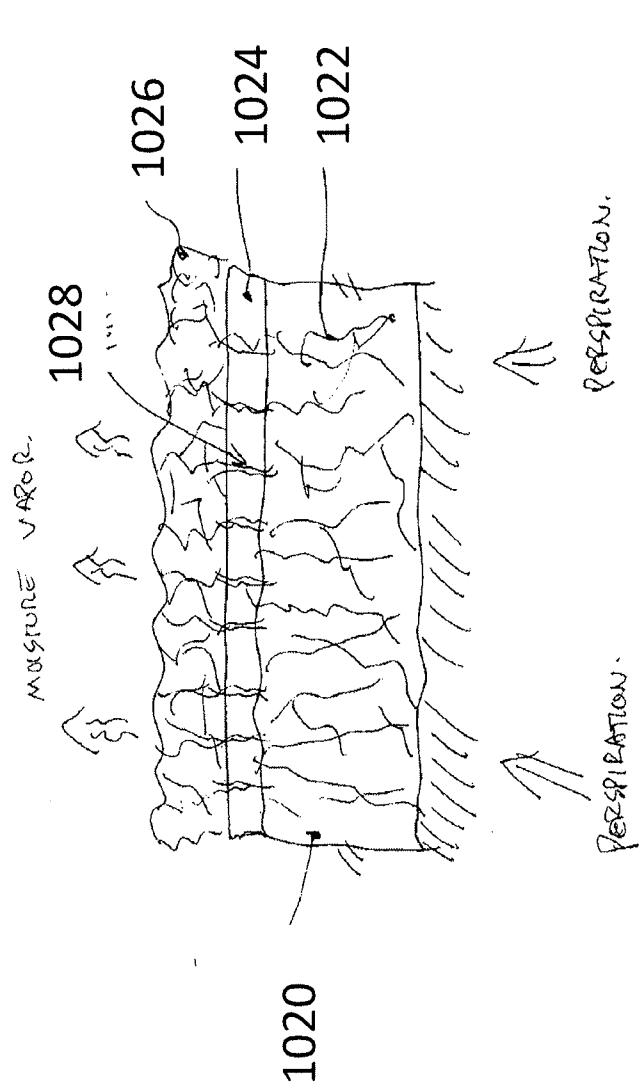


FIG. 39

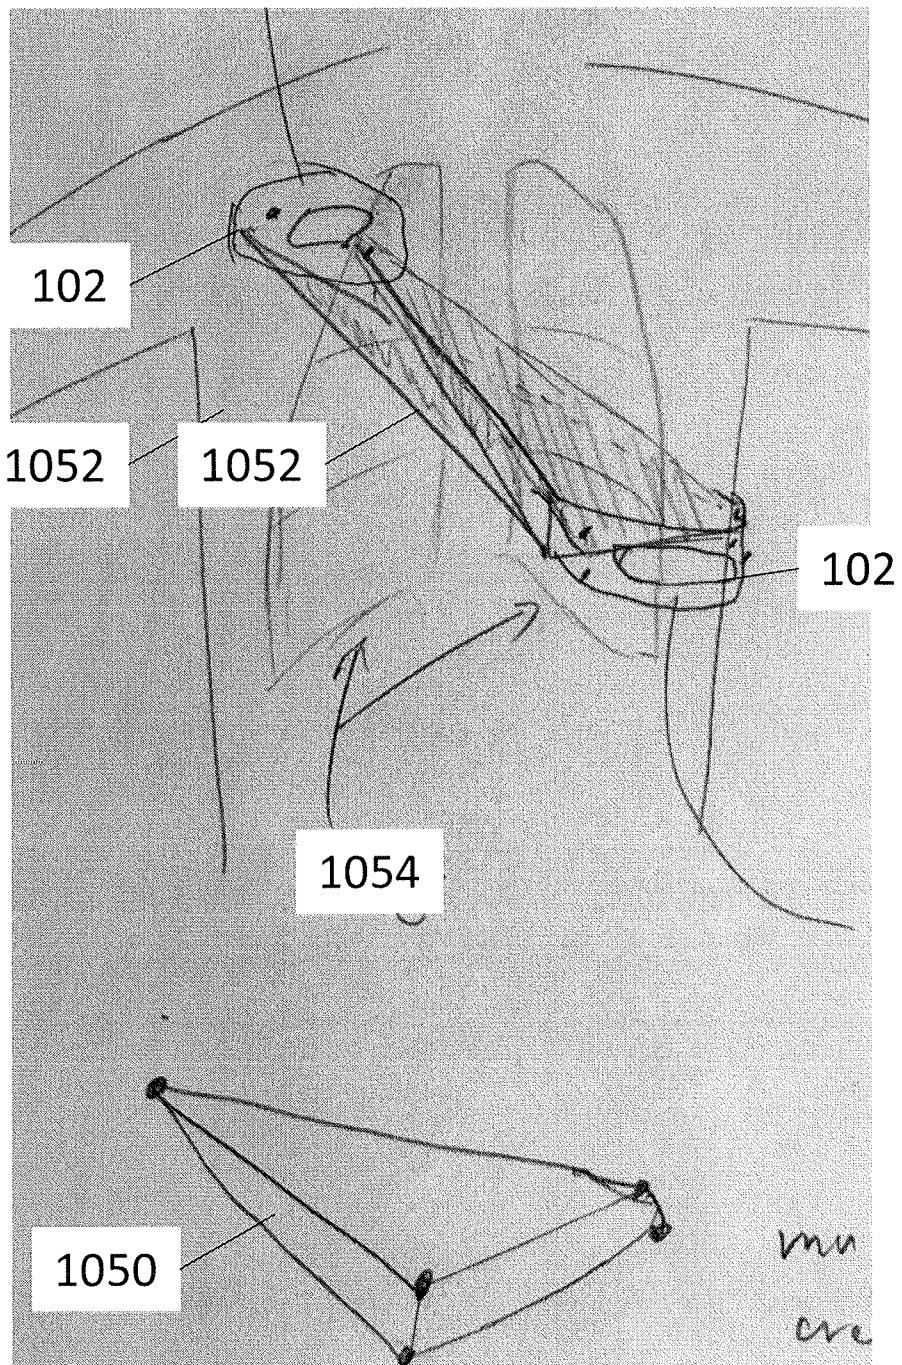
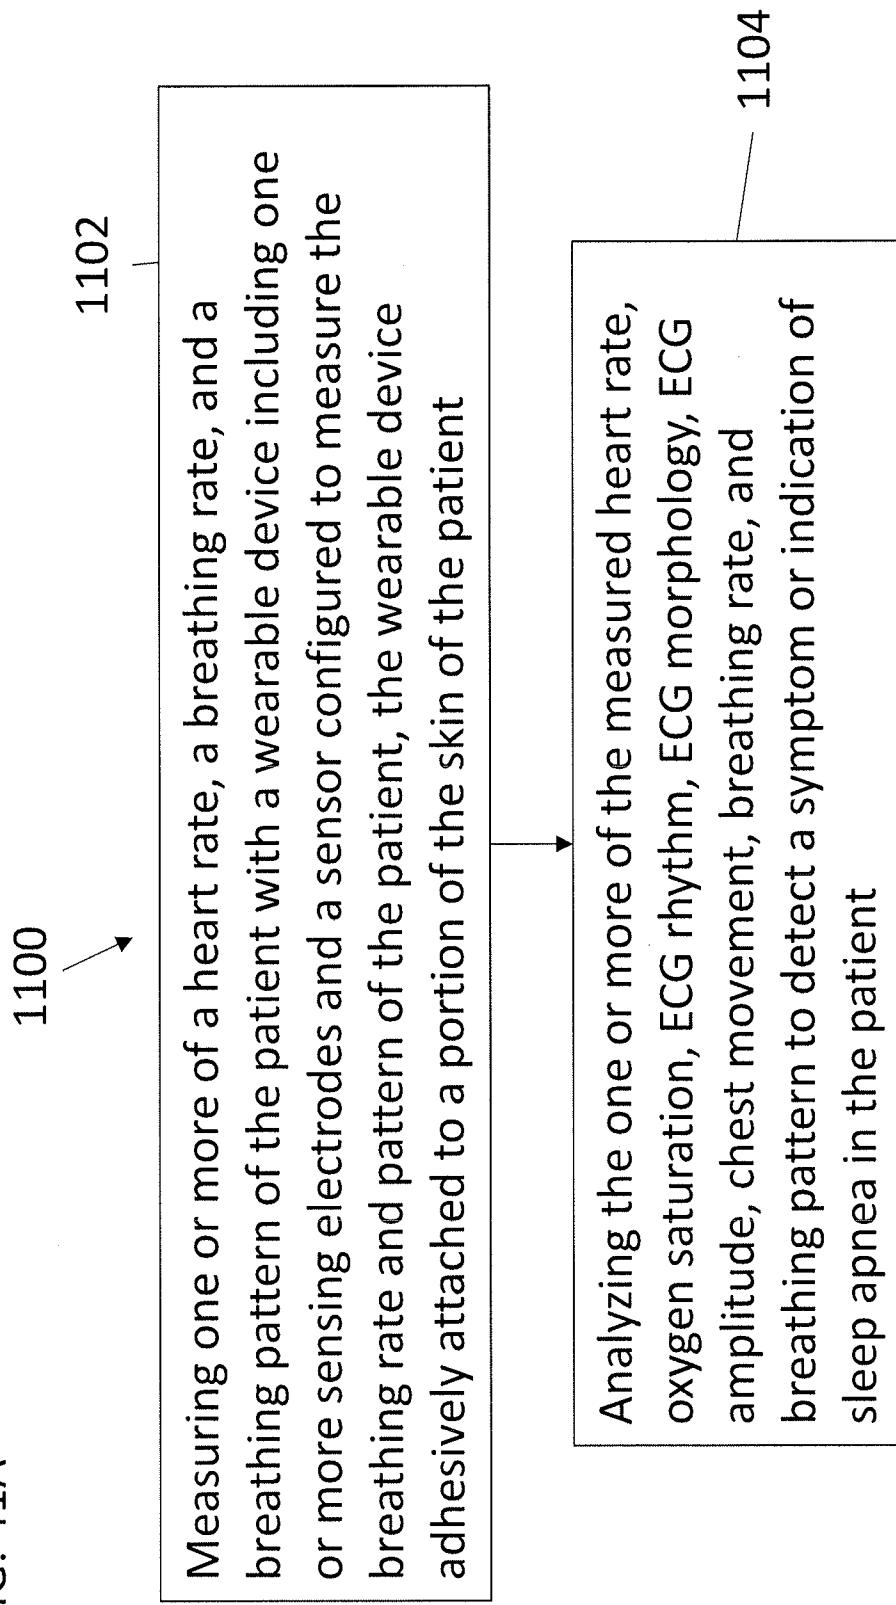


FIG. 40

FIG. 41A



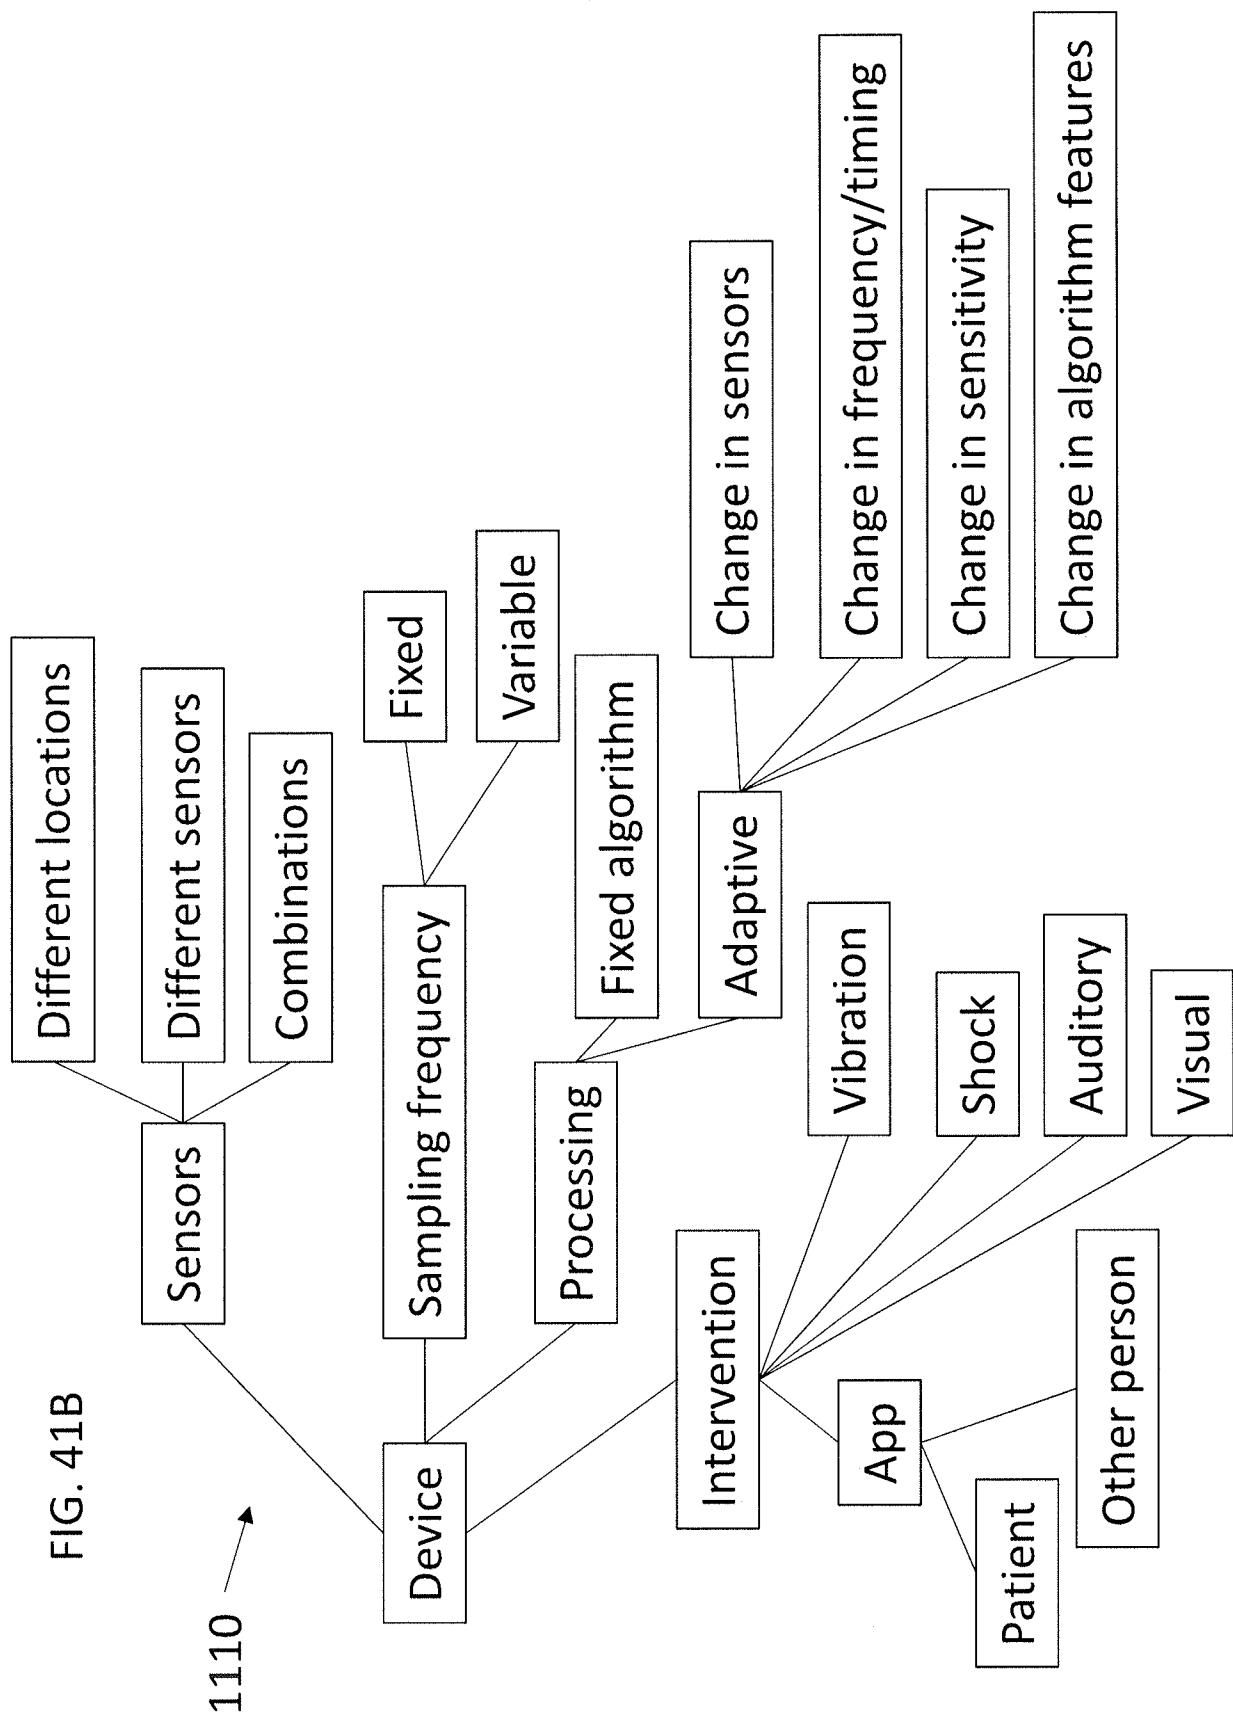


FIG. 42 1120

1122



Providing instructions on where to put a first patient engagement substrate of the wearable defibrillator on a chest of the patient, the first patient engagement substrate including one or more sensing electrodes, adhesive, and a first defibrillator electrode pad, the instructions including where to put the one or more sensing electrodes and first defibrillator electrode pad on the torso of the patient



Providing instructions on where to put a second patient engagement substrate of the wearable defibrillator, the second patient engagement substrate including a sensing electrode, adhesive, and a second defibrillator electrode pad, the instructions including where to put the one or more sensing electrodes and second defibrillator electrode pad



1124
Verifying a first patient engagement substrate placement on the torso of the patient including the placement of the one or more sensing electrodes and first defibrillator electrode pad

1128

Verifying a second patient engagement substrate placement on the chest of the patient including the sensing electrode and second defibrillator electrode pad.

1126

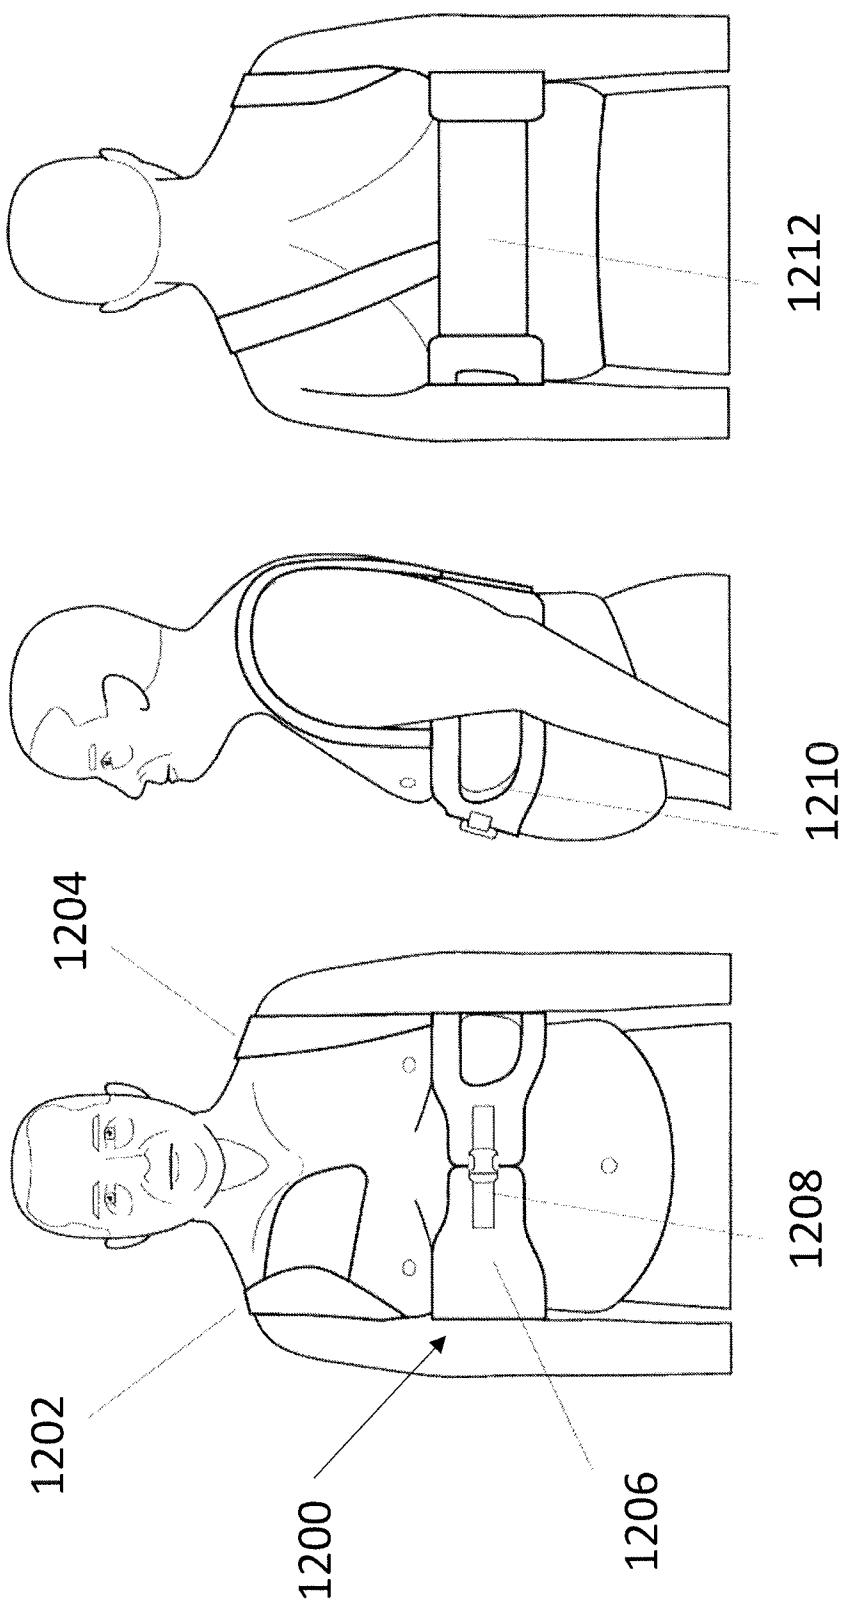


FIG. 43A

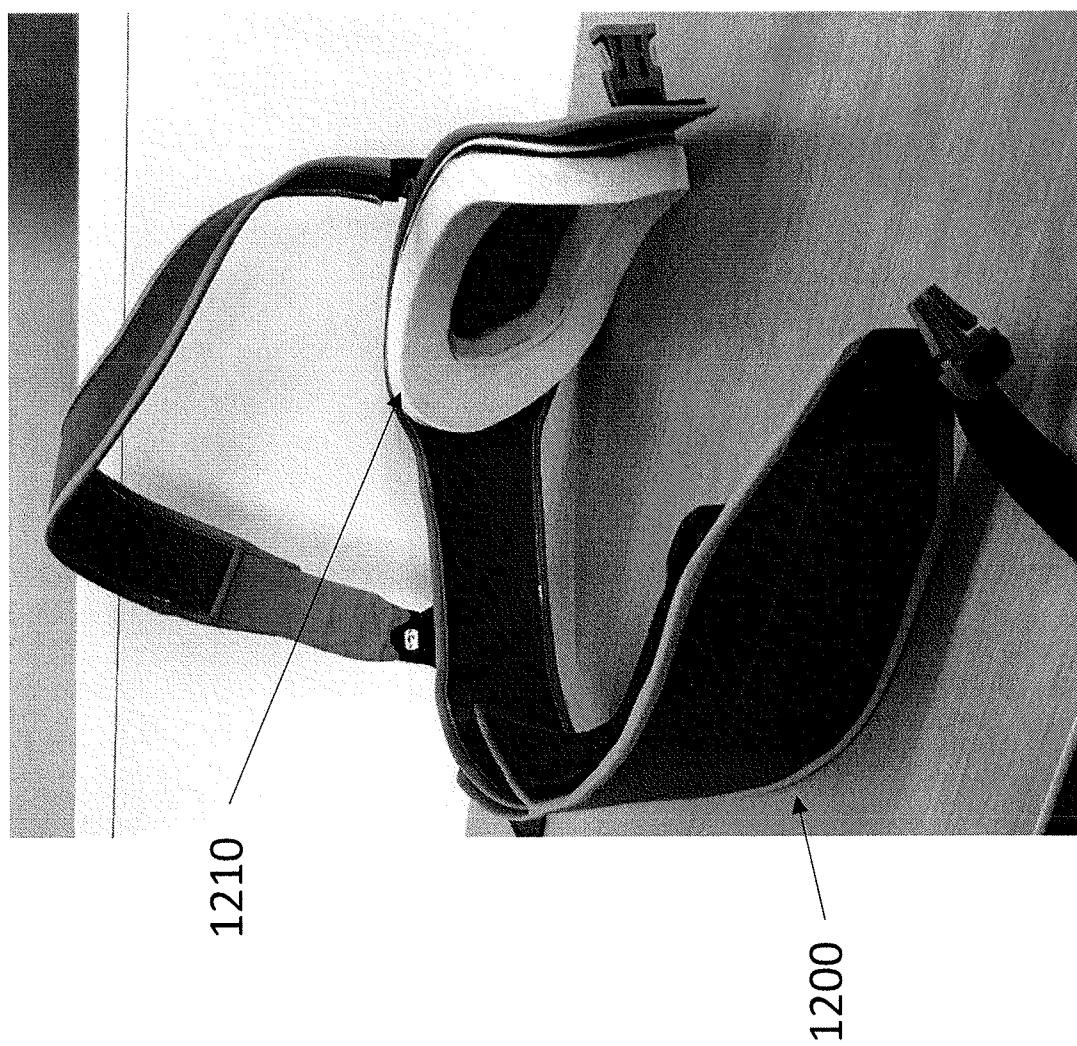


FIG. 43B