




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁵ : A61F 2/02	A1	(11) International Publication Number: WO 94/04094 (43) International Publication Date: 3 March 1994 (03.03.94)
(21) International Application Number: PCT/US93/07499 (22) International Filing Date: 5 August 1993 (05.08.93) (30) Priority data: 07/934,785 24 August 1992 (24.08.92) US (71) Applicant: LIPOMATRIX INCORPORATED [US/US]; 1850 Embarcadero Road, Palo Alto, CA 94303 (US). (72) Inventors: KNAPP, Terry, Russell ; 915 Sierra Vista Drive, Redding, CA 96001 (US). MONSEES, Thomas, Lawrence ; 920 Singlepath Lane, St. Louis, MO 63122 (US). ANDREWS, Winston, A. ; 575 El Capitan Drive, Danville, CA 94526 (US).		(74) Agent: HAFERKAMP, Richard, E.; Rogers, Howell & Haferkamp, 7777 Bonhomme, Suite 1700, St. Louis, MO 63105 (US). (81) Designated States: AU, BB, BG, BR, BY, CA, CZ, FI, HU, JP, KP, KR, KZ, LK, MG, MN, MW, NO, NZ, PL, RO, RU, SD, SK, UA, VN, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i>

(54) Title: IMPLANT WITH ELECTRICAL TRANSPONDER MARKER**(57) Abstract**

A passive transponder (28) may be encoded with a number or code of up to 64 binary bits and then mounted to virtually any prosthesis implanted in a human, such as a breast implant. After implantation, the transponder's code may be conveniently read with a hand held electromagnetic reader (24) which may merely be brought within proximity of the transponder (28). The encoded transponder (28) may thus be read in a non-invasive procedure and without the use of any sophisticated or potentially harmful medical equipment or technology such as X-ray. The information encoded in the transponder (28) may correspond to patient demographics and implant data to aid in tracking the implant's manufacturer and use for medical as well as legal reasons.

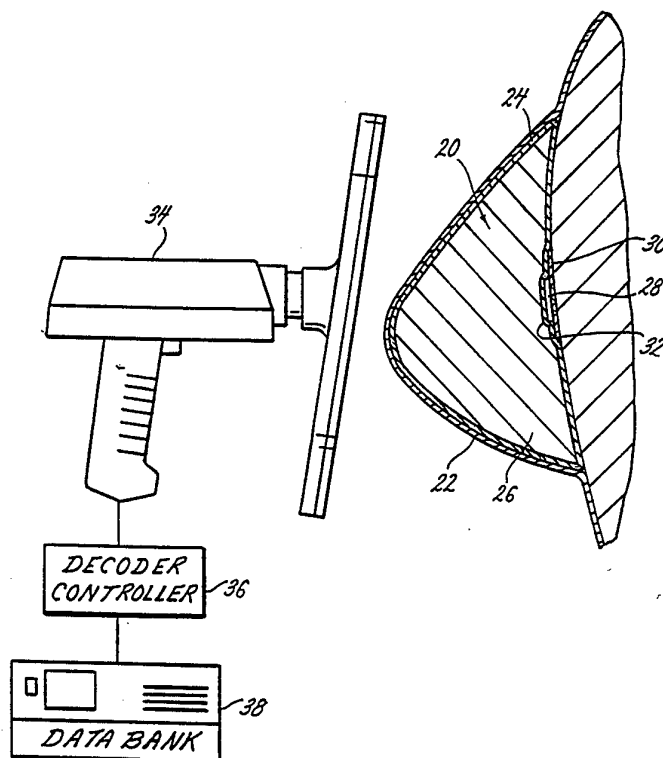

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	FR	France	MR	Mauritania
AU	Australia	GA	Gabon	MW	Malawi
BB	Barbados	GB	United Kingdom	NE	Niger
BE	Belgium	GN	Guinea	NL	Netherlands
BF	Burkina Faso	GR	Greece	NO	Norway
BG	Bulgaria	HU	Hungary	NZ	New Zealand
BJ	Benin	IE	Ireland	PL	Poland
BR	Brazil	IT	Italy	PT	Portugal
BY	Belarus	JP	Japan	RO	Romania
CA	Canada	KP	Democratic People's Republic of Korea	RU	Russian Federation
CF	Central African Republic	KR	Republic of Korea	SD	Sudan
CG	Congo	KZ	Kazakhstan	SE	Sweden
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovak Republic
CM	Cameroon	LU	Luxembourg	SN	Senegal
CN	China	LV	Latvia	TD	Chad
CS	Czechoslovakia	MC	Monaco	TC	Togo
CZ	Czech Republic	MG	Madagascar	UA	Ukraine
DE	Germany	ML	Mali	US	United States of America
DK	Denmark	MN	Mongolia	UZ	Uzbekistan
ES	Spain			VN	Viet Nam
FI	Finland				

IMPLANT WITH ELECTRICAL TRANSPONDER MARKERBackground and Summary of the Invention

With the advance of medical technology, there are a number of medical prostheses and devices which are implantable in humans for re-constructive and/or cosmetic purposes. These include breast implants; penile im-
5 plants; musculature and other soft tissue implants; pace makers; valves; artificial joints and limbs such as knees, shoulders, legs, fingers, etc.; pins; screws; plates; rods; nails and other braces and supports. In order to ensure the continued safety and health of pa-
10 tients receiving these implants, the Safe Medical Device Act of 1990 has been enacted which dictates that manufacturers of Class III implantable medical devices institute a device registry for tracking of their devices, notification of patients, and otherwise monitoring these im-
15 plants after they have been placed in a patient. Compliance with this Act has been proposed through a method of tracking which requires the surgeon who implants the device to complete and return a form or card with patient demographic data and implant data to the manufacturer or
20 to a third party registry service. This method requires

careful accumulation of data by a surgeon or his staff as well as secure inventory control procedures in order to ensure that the data is properly associated with the correct implant. Additionally, there is a risk of loss
5 of the data entirely resulting from misdirected or lost communications. Furthermore, access to this data can be impeded in the event of an emergency situation or other circumstances which interfere with a patient's ability to recall or report the proper information which medical
10 personnel may then use to access the registry and data contained therein.

There have been some suggestions in the prior art of marking the implants themselves with, for example, a radiopaque marker or other marker which contains the
15 information relating to the implant. Ideally, this data could then be viewable by X-ray or some other non-invasive manner. However, there are difficulties with these prior art approaches. First of all, a breast implant with a radiopaque marker would at least partially obscure
20 or mask tissue which is desired to be viewed in order to detect artifacts relating to tumors or the like for diagnosing cancer. Obviously, this is highly undesirable as the incidence of breast cancer presents a significant risk to many females. Additionally, repeated exposure to
25 X-ray is not generally considered healthful or desirable and represents at least an added inconvenience entailing some degree of expense to recall or access the implant data. Therefore, radiopaque markers have not been viewed as a suitable long-term solution to this problem.

30 In order to solve these and other problems in the prior art, and in order to provide a convenient, fool proof marker secured to the implant itself and yet readable in a non-invasive manner, the inventors herein have succeeded in designing and developing an implant which
35 incorporates a passive transponder which may be encoded and subsequently accessed with a hand held electromagnet-

ic reader in a quick and inexpensive procedure. The passive transponder may be secured to the implant by any convenient means. For example, in a breast implant, the multi-layered shell for the implant may be laminated
5 around the transponder to thereby be permanently and securely fixed to the implant. The transponder may be laminated in the sidewall of the shell, or between layers which comprise the seal patch which is applied to the shell to seal the mandrel opening. Similarly, the tran-
10 sponder may be laminated onto the surface of most other implants in an unobtrusive location. In some other implants, the transponder may be inserted into a hole or inlay and sealed in place.

As passive transponders are commercially available
15 in a cylindrical shape sized at 2 mm in diameter and 11 mm in length, the patient will not sense any discomfort or even the presence of the transponder. Also, the transponder may be encoded with any suitable encoding scheme. A commercially available transponder presently
20 provides for the storage of up to 64 binary bits of data. This data capacity may accommodate the direct storage of much, if not all, of the information desired to be recorded and maintained in a device registry. Furthermore, the storage capacity of the transponder is expected to be
25 increased as further development occurs over time. Alternately, a number, collection of numbers, combination of numbers and letters, or other indirect code may be stored which after reading may be used to access a data bank which itself contains the desired information. Of
30 course, if information is directly stored in the implant, it becomes immediately available upon reading the transponder. This provides ready access to information in emergency situations. Alternately, with the widespread availability, accessibility, and use of computers over
35 telecommunications networks including telephone lines, it is not generally considered to be unduly limiting to

provide that the code read from the transponder be then used to access an appropriate data bank in order to obtain the patient demographics, manufacturer's name, date of manufacture, surgeon's name, date of implantation, etc.

A companion hand held electromagnetic reader is also commercially available which emits a low frequency magnetic field to activate the passive transponder and thereby cause it to transmit its encoded data to the reader. With this particular commercial device, no battery or other source of electrical power need be included in the passive transponder. This further reduces the size required for the transponder and renders it particularly suitable to this application.

While the principal advantages and features of the present invention have been described above, a more complete and thorough understanding of the invention may be attained by referring to the drawings and description of the preferred embodiment which follow.

Brief Description of the Drawings

Figure 1 is a perspective view of a breast implant containing a passive transponder with a hand held reader in position to read the encoded data contained therein;

Figure 2 is a partial cross-sectional view of the transponder as laminated between the multiple layers of a seal patch for a breast implant;

Figure 3 is a perspective view of a pectoralis muscle implant with a passive transponder mounted therein;

Figure 4 is a perspective view of a soft chin implant with passive transponder mounted therein;

Figure 5 is a perspective view of a rigid chin implant with a passive transponder mounted therein;

Figure 6 is a perspective view of a nipple transplant with a passive transponder mounted therein;

Figure 7 is a perspective view of an otoplasty implant with a passive transponder mounted therein;

Figure 8 is a perspective view of a penile implant, surgically implanted, with a passive transponder
5 mounted therein;

Figure 9 is a top view of a pace maker with a passive transponder mounted thereon;

Figure 10 is a top view of a heart valve with a passive transponder mounted to the edge thereof;

10 Figure 11 is a perspective view of a total knee joint prosthesis with a passive transponder mounted thereon;

Figure 12 is a perspective view of a shoulder arthroplasty system with a passive transponder mounted
15 therein;

Figure 13 is a partial cross-sectional view of a passive transponder inlaid into and below the surface of an implant;

Figure 14 is a perspective view of a femoral fixation system implanted in a femur with a passive transponder mounted thereto;
20

Figure 15 is a perspective view of an orthopedic nailing system with a passive transponder mounted therein;

25 Figure 16 is a perspective view of a finger joint prosthesis with a passive transponder mounted therein;

Figure 17 is a perspective view of a craniomaxillofacial plating system with a passive transponder mounted therein;

30 Figure 18 is a perspective view of still another plating system with a passive transponder mounted therein; and

Figure 19 is a partial cross-sectional view of a typical implant with a passive transponder mounted within
35 a cored hole drilled therein.

Detailed Description of the Preferred Embodiment

As shown in Figure 1, a breast implant 20 has been implanted in a female's breast 22 and includes a silicone shell 24 inflated with an appropriate fill material 26.

5 At the posterior side of the implant 20 is shown the transponder 28 which has been laminated between adjacent layers 30, 32 of the shell 24. Transponder 28 may be any passive transponder such as a Trovan Model ID100 available from Electronic Identification Systems Ltd. of Santa
10 Barbara, California. This particular transponder is designed to be environmentally independent and suitable for operation while being directly submerged in liquids. Furthermore, it may be read spherically from any direction through most materials, and including most impor-
15 tantly those materials comprising implants for the human body. The transponder may be directly encoded with up to 64 binary bits of data to provide almost one trillion possible different code combinations. It is anticipated that FDA approval will be forthcoming for its use as part
20 of the invention disclosed and claimed herein.

A hand held reader 34 is also shown in Figure 1 and may be a Trovan Model LID500, or other suitable device. Its principle of operation includes emitting a low frequency magnetic field for activating the passive tran-
25 sponder 28. As such, transponder 28 has no power source and instead derives the energy needed for its operation from the magnetic field generated by the reader 34. This permits the transponder 28 to have a virtually unlimited life span. The hand held reader 34 is shown connected to
30 a decoder controller 36 which accesses a data bank 38 in response to the detected code contained within transponder 28 to thereby access such data which has been stored corresponding to transponder 28. Alternately, as mentioned above, the hand held reader 34 may be used to ac-
35 cess the code contained within transponder 28 and then other means used to access a data bank for the retrieval

of the desired information. Such means might include the use of a telephone and modem to access a registry contained in a geographically centrally located site.

As shown in Figure 2, the transponder 28 may be
5 laminated between adjacent layers 40, 42 of the seal patch 44 which is commonly used to seal the mandrel opening 46 in a shell 48 of a breast implant 50. For other implants, convenient mounting locations may be readily
10 determined with due consideration given to avoiding discomfort to the patient as well as optimizing readability of the transponder with the hand held reader.

As shown in Figure 3, a pectoralis muscle implant 52 may conveniently have a passive transponder 54 contained therein. The passive transponder 54 may be molded
15 in place, or a hole or inlay drilled for placement of the implant, after which the implant surface may then be refinished.

As shown in Figures 4 and 5, a soft chin implant 56 or a hard chin implant 58 may also have a passive
20 transponder 60, 62 mounted therein. As shown in Figure 6, a nipple implant 64 has a passive transponder 66 mounted internally. In all of these transplants, the mounting of the passive transponder is achieved to provide minimal discomfort or sensation to the patient, as
25 well as to avoid interference with the cosmetic appearance of the implant. As shown in Figure 7, an otoplasty implant 68 may have a passive transponder 70 mounted therein. As shown in Figure 8, a penile implant 72 may have a passive transponder 74 mounted therein.

30 As shown in Figure 9, a pace maker 76 may also have a passive transponder 78 mounted either on its surface or below the protective metal casing thereof. The inventors have found that reading of the passive transponder by the hand held reader may be achieved even when
35 the transponder is obscured by metallic surfaces. As shown in Figure 10, a heart valve 80 may have a passive

transponder 82 mounted to its edge in order to avoid interference with the operability thereof, or fixation thereof.

As shown in Figures 11 and 12, a total knee joint prosthesis 84 or a shoulder prosthesis 86, either one of which includes a majority of parts made from titanium or the like, may also conveniently carry a passive transponder 88, 90.

As shown in Figure 13, the passive transponder 92 may be placed within a trough 94 or the like and covered with a sealant 96 so that the surface of the transponder 98 is uninterrupted and smooth as is desirable in many transponders.

As shown in Figures 14 and 15, a femoral fixation implant 100, or an orthopedic nailing system 102 may conveniently have a passive transponder 104, 106 inlaid therein. As shown in Figure 16, a finger joint prosthesis 108 may also have a passive transponder 110 located in a position which does not interfere with the movable joint portion 112 of the prosthesis 108. As shown in Figures 17 and 18, a craniomaxillofacial plating system 114 or any other plating system 116 may also conveniently include a passive transponder 118, 120. As an alternative to the inlay mounting shown in Figure 13, a hole 122 may be drilled in any convenient location of an implant 124 and the passive transponder 126 inserted therein and sealed in place by sealer 128, with the outer surface of sealer 128 being finished to provide a smooth surface on implant 124.

As disclosed herein, a wide variety of implants made of all sorts of material may conveniently include a passive transponder which may be implanted, and then read by the hand held reader. This compatibility and ease of operation permits the use of a passive transponder with virtually any implant. The inventors have disclosed herein a representative sample of such implants. Howev-

er, the scope of the present invention is broad enough to encompass any implant presently known to the inventors herein.

There are various changes and modifications which
5 may be made to the invention as would be apparent to those skilled in the art. However, these changes or modifications are included in the teaching of the disclosure, and it is intended that the invention be limited only by the scope of the claims appended hereto.

What Is Claimed Is:

1. In an implantable prosthesis adapted for im-
plantation in a human, the improvement comprising a tran-
sponder mounted thereto so that said transponder is im-
planted as said prosthesis is implanted, said transponder
5 having means for being encoded with a unique tag so that
said transponder may be readily identified after implan-
tation by reading said unique tag.
2. The prosthesis of Claim 1 wherein said tran-
sponder has means for its tag to be read with a non-inva-
sive protocol.
3. The prosthesis of Claim 2 wherein said tran-
sponder has means for its tag to be read electromagneti-
cally.
4. The prosthesis of Claim 3 wherein said tran-
sponder has means for being energized by a remote reader
thereby obviating a need for a battery to be contained in
said transponder.
5. The prosthesis of Claim 4 wherein said tran-
sponder has means for being encoded with a number select-
ed from within a range of 0 to 64 bits, binary.
6. The prosthesis of Claim 5 wherein said prosthe-
sis is a breast implant including an envelope.
7. The prosthesis of Claim 6 wherein said tran-
sponder is mounted to said implant by being laminated
between layers of said envelope.
8. The prosthesis of Claim 7 wherein said implant
further comprises a seal patch on said envelope, said
transponder being laminated into said seal patch.
9. The prosthesis of Claim 1 wherein said tran-
sponder is mounted within the profile of said prosthesis.
10. The prosthesis of Claim 9 wherein said tran-
sponder is sealed within a hole in said prosthesis.
11. The prosthesis of Claim 1 wherein said prosthe-
sis is a soft tissue implant.

12. The prosthesis of Claim 1 wherein said prosthesis is a reconstructive bone implant.

13. The prosthesis of Claim 1 wherein said prosthesis is a joint reconstructive implant.

14. The prosthesis of Claim 13 wherein said prosthesis is a replacement joint.

15. A prosthesis intended for human implantation, said prosthesis including a transponder mounted thereto so that said transponder is implanted as said prosthesis is implanted, said transponder having means for being
5 encoded with a unique identifier so that said transponder's identifier may be read after implantation and associated with a data base for reporting selected data corresponding to said implant.

16. The prosthesis of Claim 15 wherein said transponder has means for its identifier to be read remotely.

17. The prosthesis of Claim 16 wherein said transponder has means for its identifier to be read electromagnetically.

18. The prosthesis of Claim 17 wherein said transponder has means for being energized by a remote reader thereby obviating a need for a battery to be contained in said transponder.

19. The prosthesis of Claim 18 wherein said prosthesis is a breast implant comprised of an envelope with a multi-layered seal patch, said transponder being mounted therein by being sealed between the layers of said
5 seal patch.

20. The prosthesis of Claim 19 wherein said transponder has means for being encoded with a number selected from within the range of 0 to 64 bits, binary.

21. The prosthesis of Claim 15 wherein said transponder is mounted within the profile of said prosthesis.

22. The prosthesis of Claim 21 wherein said transponder is sealed within a hole in said prosthesis.

23. The prosthesis of Claim 15 wherein said prosthesis is a soft tissue implant.

24. The prosthesis of Claim 15 wherein said prosthesis is a reconstructive bone implant.

25. The prosthesis of Claim 15 wherein said prosthesis is a joint reconstructive implant.

26. The prosthesis of Claim 25 wherein said prosthesis is a replacement joint.

27. A breast implant comprised of an elastomeric shell, a multi-layered elastomeric seal patch adhered to said shell, and an electromagnetically readable transponder laminated between the layers of said seal patch,
5 said transponder having means for being encoded with a unique code so that after implantation said code may be read by a remote, non-invasive reader to thereby learn selected data concerning said implant.

1/3

FIG. 1.

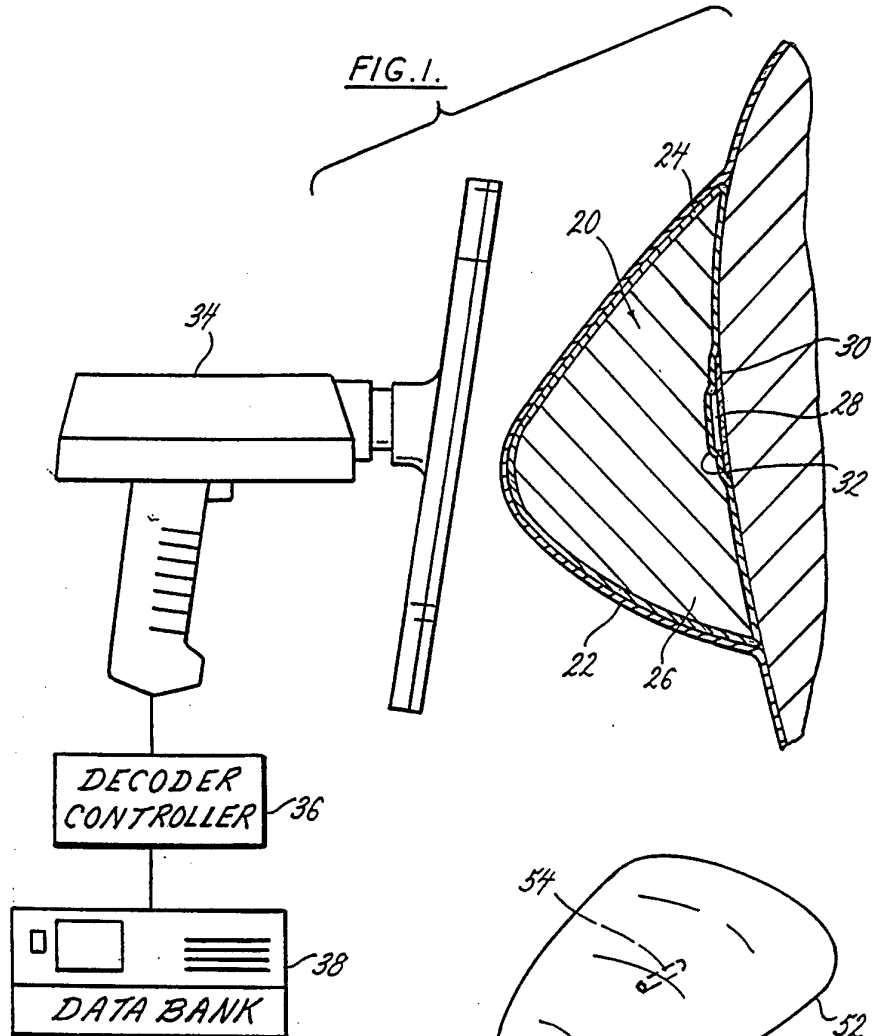


FIG. 3.








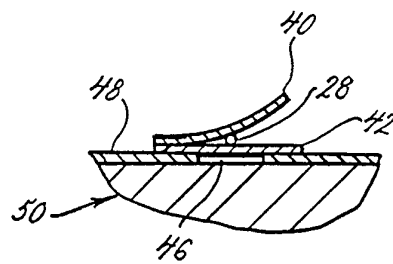


FIG. 2.

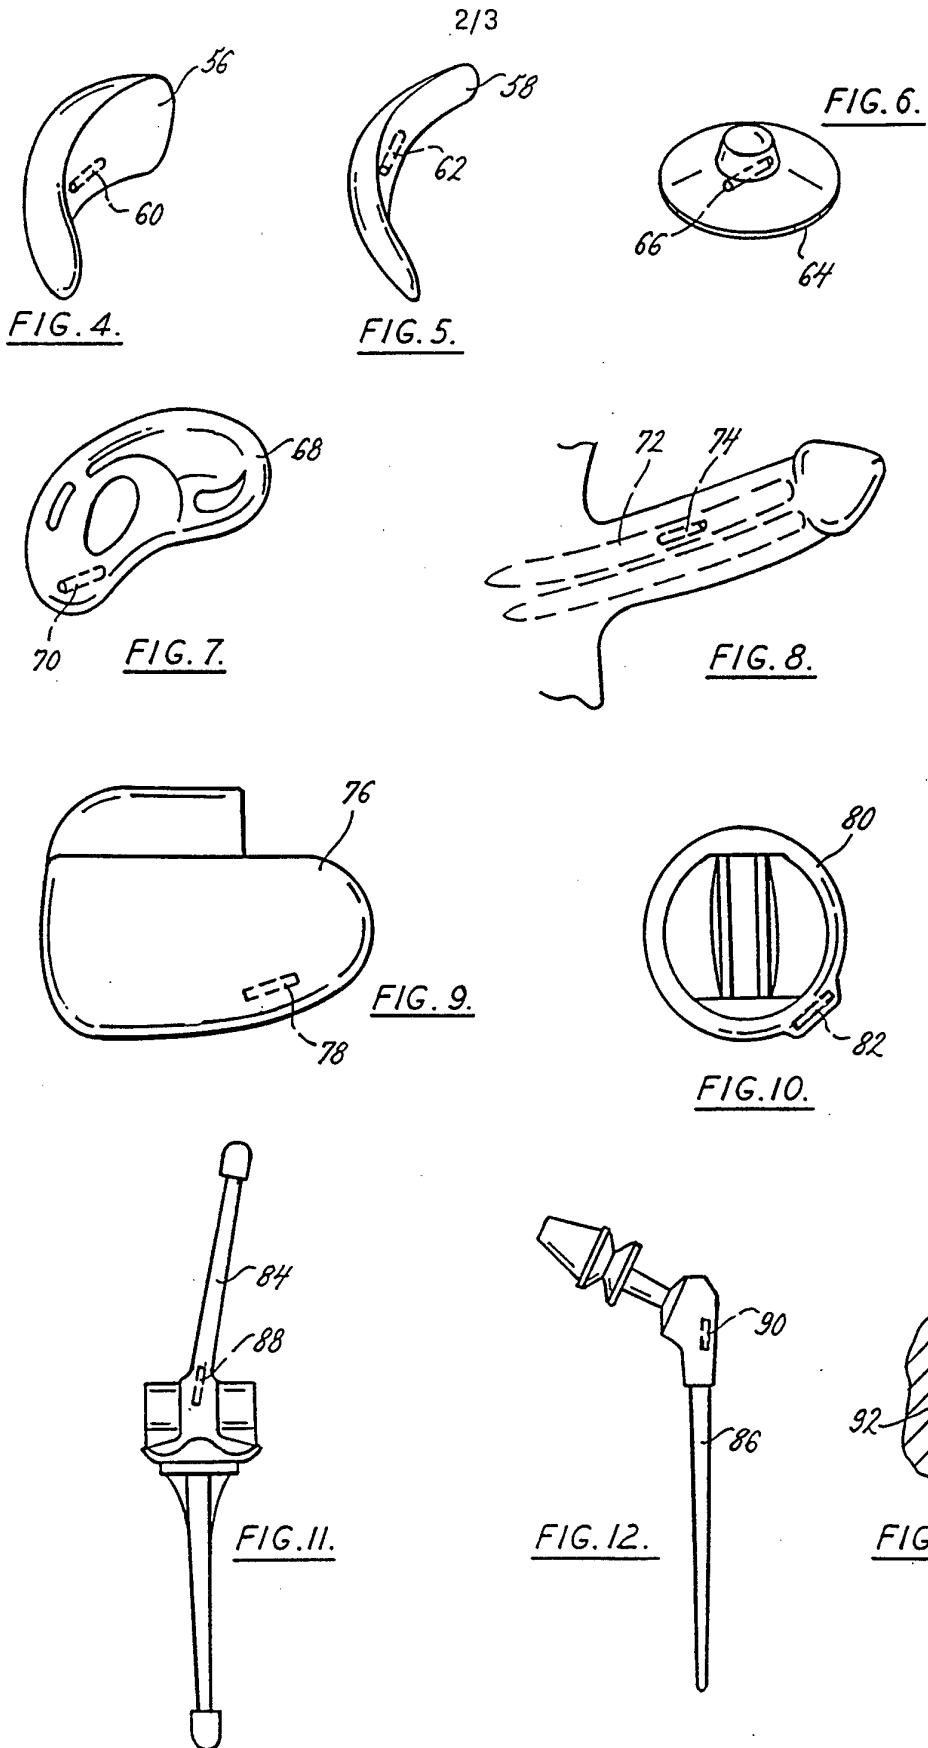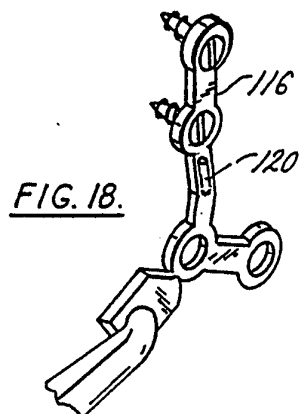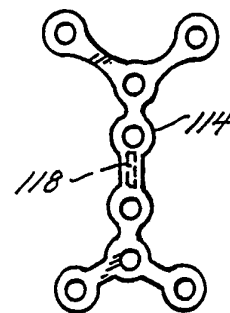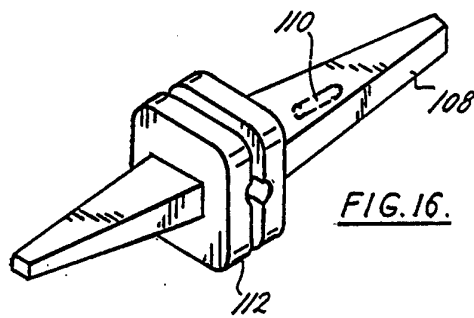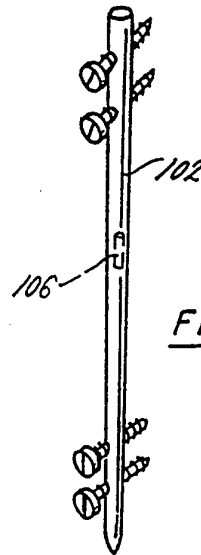

3/3

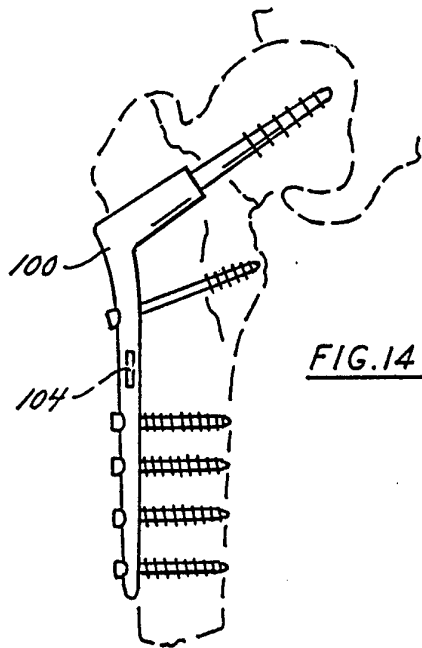

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US93/07499**A. CLASSIFICATION OF SUBJECT MATTER**

IPC(5) :A61F 2/02

US CL :623/11

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 623/11; 623/8; 128/419PG

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X --- Y	US, A, 875, 483 (Vollmann et al) 24 October 1989 See column 4, lines 17-34; column 7, lines 53-56; column 25, lines 40-47; column 29, lines 26-64; column 3, lines 13-24; column 28, lines 26-35.	1-3,5 ----- 4,10, 18, 22
X --- Y	US, A, 5, 084, 699 (DiMichele) 28 January 1992 See column 1, line 45 - column 2, line 3.	1-3,5 ----- 4, 18, 10, 22

☒ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search 18 October 1993	Date of mailing of the international search report 12 NOV 1993
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. NOT APPLICABLE	Authorized officer  Debra S Brittingham Telephone No. (703) 308-3401

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US93/07499

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US, A, 4,863,470 (CARTER), 05 SEPTEMBER 1989, SEE COLUMN 1, LINES 44-47 AND COLUMN 2, LINES 34-46.	1-3,5-11, 15-17,19- 23 AND 27