



(86) Date de dépôt PCT/PCT Filing Date: 1997/01/31  
 (87) Date publication PCT/PCT Publication Date: 1997/08/07  
 (45) Date de délivrance/Issue Date: 2010/04/20  
 (85) Entrée phase nationale/National Entry: 1998/07/30  
 (86) N° demande PCT/PCT Application No.: US 1997/001815  
 (87) N° publication PCT/PCT Publication No.: 1997/027801  
 (30) Priorité/Priority: 1996/01/31 (US08/594,758)


(51) Cl.Int./Int.Cl. *A61B 8/13* (2006.01),  
*A61B 5/00* (2006.01), *A61B 6/00* (2006.01),  
*A61B 8/08* (2006.01), *A61K 49/22* (2006.01),  
*G01N 21/17* (2006.01), *A61B 17/00* (2006.01),  
*A61F 9/008* (2006.01)

(72) Inventeurs/Inventors:  
 ORAEVSKY, ALEXANDER A., US;  
 JACQUES, STEVEN L., US;  
 ESENALIEV, RINAT O., US

(73) Propriétaires/Owners:  
 ORAEVSKY, ALEXANDER A., US;  
 JACQUES, STEVEN L., US;  
 ESENALIEV, RINAT O., US

(74) Agent: BORDEN LADNER GERVAIS LLP

(54) Titre : SYSTEME D'IMAGERIE OPTO-ACOUSTIQUE LASER  
 (54) Title: LASER OPTO-ACOUSTIC IMAGING SYSTEM

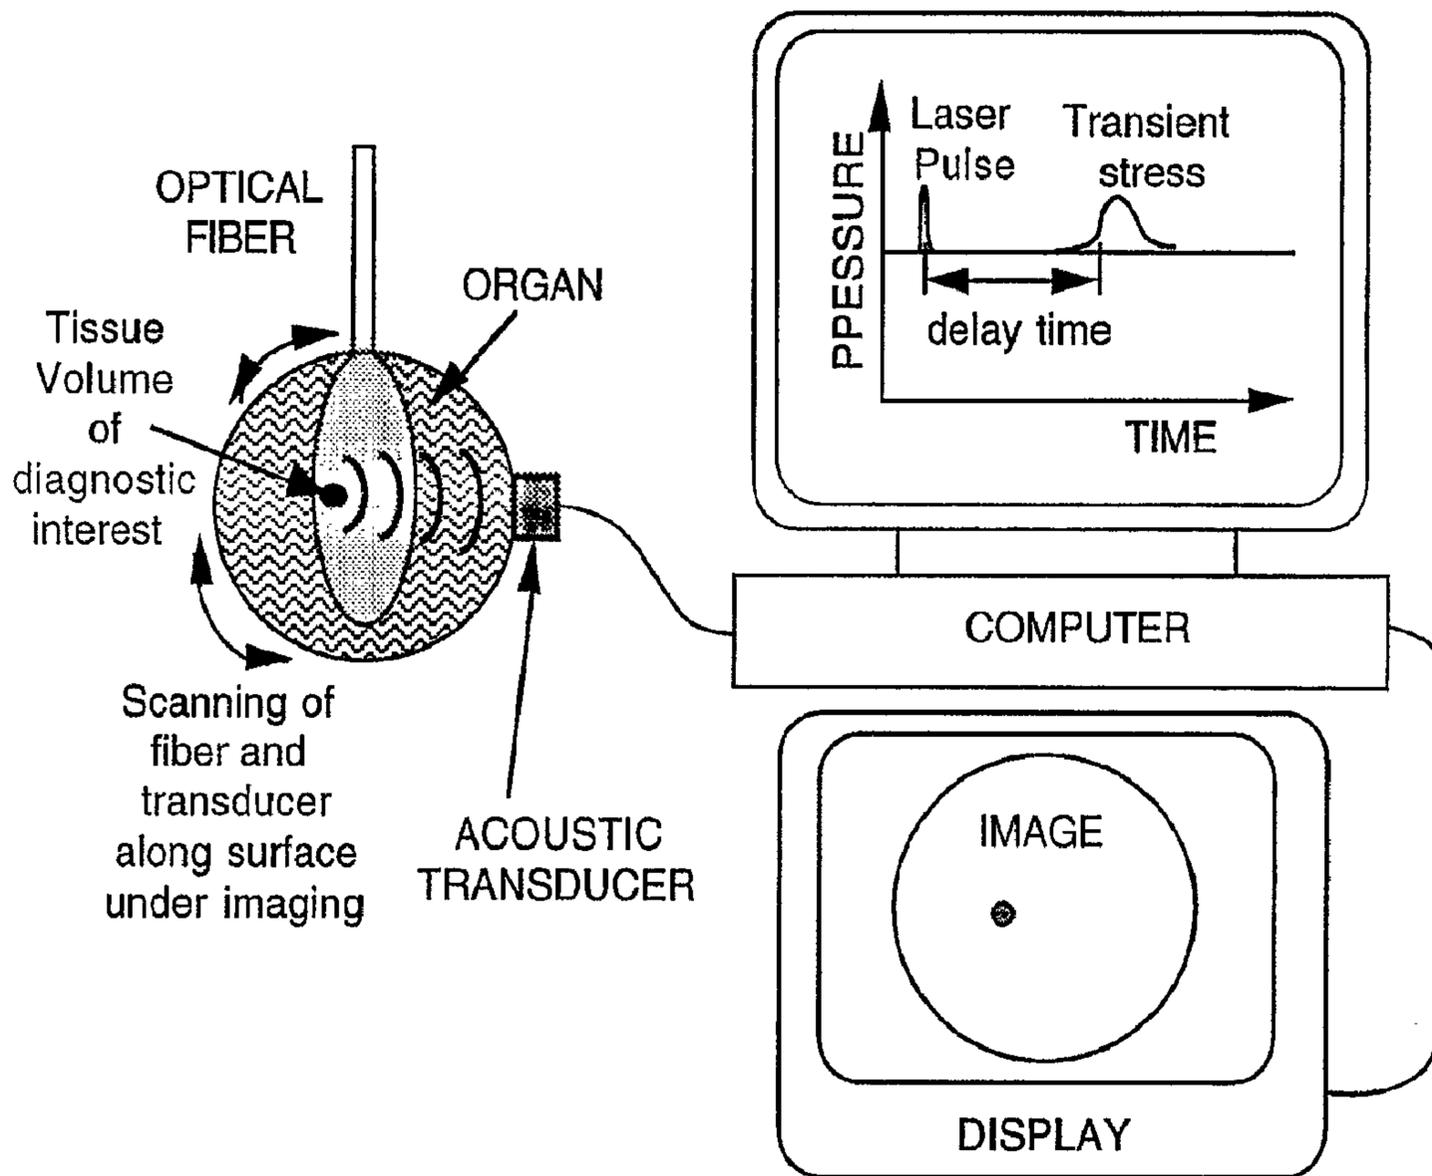

(57) Abrégé/Abstract:

The present invention provides a system and principles of laser photo-acoustic imaging and tomography. The basis for laser photo-acoustic tomography is the time resolved detection of laser induced transient stress waves, selectively generated in absorbing

(57) **Abrégé(suite)/Abstract(continued):**

tissues of diagnostic interest. Such a technique allows to visualize absorbed light distribution in turbid biological tissues irradiated by short laser pulses. Laser photo-acoustic tomography can be used for detection of tissue pathological changes that result in increased concentration of various tissue chromophore such as hemoglobin or development of enhanced micro-circulation in diseased tissue. The invented technology combines the advantages of pulsed laser excitation with time resolved detection of acoustic transients. The invented technology can be used for determination of optical heterogeneities in biological tissues. These heterogeneities include blood vessels, tissue layers, abnormal tissues and damaged tissues with further reconstruction of 3D tomographic images of human organs or portions thereof.



PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)


(51) International Patent Classification <sup>6</sup> : <b>A61B 5/00, 8/13</b>	<b>A1</b>	(11) International Publication Number: <b>WO 97/27801</b> (43) International Publication Date: 7 August 1997 (07.08.97)
<p>(21) International Application Number: PCT/US97/01815</p> <p>(22) International Filing Date: 31 January 1997 (31.01.97)</p> <p>(30) Priority Data: 08/594,758 31 January 1996 (31.01.96) US</p> <p>(71) Applicant: THE BOARD OF REGENTS OF THE UNIVERSITY OF TEXAS SYSTEM [US/US]; 201 West 7th Street, Austin, TX 78701 (US).</p> <p>(72) Inventors: ORAEVSKY, Alexander, A.; 5038 Lympar Drive, Houston, TX 77096 (US). JACQUES, Steven, L.; 4302 Brompton Circle, Bellaire, TX 77401 (US). ESENALIEV, Rinat, O.; Apartment 401, 7600 Kirby, Houston, TX 77030 (US).</p> <p>(74) Agent: ADLER, Benjamin, A.; McGregor &amp; Adler, P.C., 8011 Candle Lane, Houston, TX 77071 (US).</p>	<p>(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p><b>Published</b> <i>With international search report.</i></p>	

(54) Title: LASER OPTO-ACOUSTIC IMAGING SYSTEM

## (57) Abstract

The present invention provides a system and principles of laser photo-acoustic imaging and tomography. The basis for laser photo-acoustic tomography is the time resolved detection of laser induced transient stress waves, selectively generated in absorbing tissues of diagnostic interest. Such a technique allows to visualize absorbed light distribution in turbid biological tissues irradiated by short laser pulses. Laser photo-acoustic tomography can be used for detection of tissue pathological changes that result in increased concentration of various tissue chromophore such as hemoglobin or development of enhanced micro-circulation in diseased tissue. The invented technology combines the advantages of pulsed laser excitation with time resolved detection

of acoustic transients. The invented technology can be used for determination of optical heterogeneities in biological tissues. These heterogeneities include blood vessels, tissue layers, abnormal tissues and damaged tissues with further reconstruction of 3D tomographic images of human organs or portions thereof.

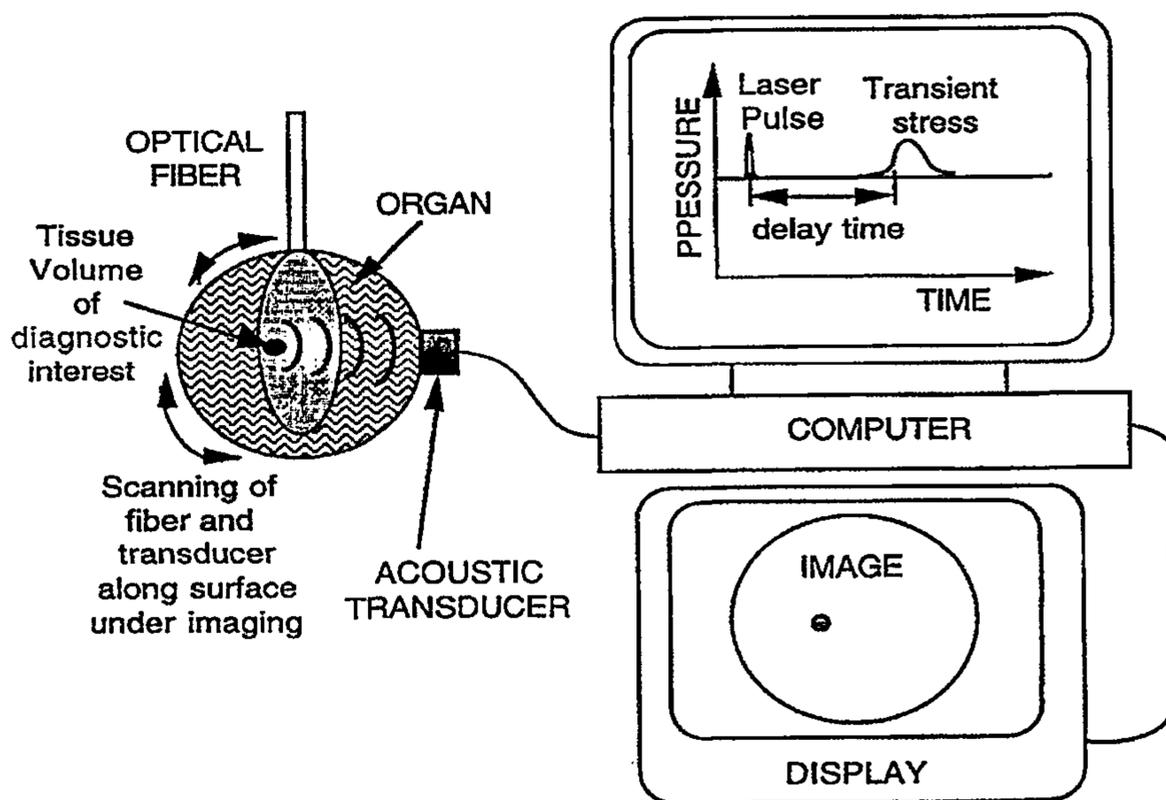

5                   **LASER OPTO-ACOUSTIC IMAGING SYSTEM**10                   **BACKGROUND OF THE INVENTION**

10

Field of the Invention

15                   The present invention relates generally to the fields of optics, lasers and medical diagnostic devices. More specifically, the present invention relates to a laser opto-acoustic imaging system capable of producing a three-dimensional image (tomography scan) of human organs.

Description of the Related Art

20                   Ultrasonic imaging is currently used widely in clinical medical practice to detect abnormalities in soft tissue organs with acoustic boundaries such as one type of tissue embedded within another type. Ultrasonic imaging has, however, several limitations. For example, ultrasonic imaging is incapable of detecting  
25                   acoustically homogeneous tissues, i.e., when ultrasonic properties of all of the tissues scanned are similar).

30                   Optical imaging technologies are based on time-resolved or phase-resolved detection of diffusely reflected light pulses or photon density waves. Optical tomographic technologies take advantage of differences in tissue optical properties for diagnostic purposes. However, ubiquitous light scattering in tissues has been a great obstacle to laser imaging.

35                   Optoacoustic spectroscopy methods utilize light to excite an object of interest (molecules or atoms). Using acoustic (piezoelectric) detectors, optoacoustic spectroscopy methodology can measure stress amplitude for obtaining absorption spectra. This represents not an imaging or tomographic technology per se.

Principles of laser optoacoustics, i.e., methods of stress generation and detection have been described. Relationships between spatial distribution of acoustic sources and temporal profile of laser-induced stress waves have been derived. However, methods of laser optoacoustics have not been proposed as means for medical diagnostics.

The prior art is deficient in the lack of functional laser opto-acoustic imaging system. The present invention fulfills this longstanding need and desire in the art.

10

### SUMMARY OF THE INVENTION

Photo-acoustic ultrasound technology for medical imaging has been described in the prior art. However, the prior art has not understood and correctly manipulated three principles of laser optoacoustic imaging important for sensitivity, spatial resolution and correct interpretation of images. These principles are: (1) short-pulse laser irradiation to generate transient stress waves under conditions of temporal stress confinement. Such irradiations provides the highest possible amplitude of generated stress with profiles resembling that of light distribution in tissues, which yields sharp images with accurate localization; (2) time-resolved detection of a stress profile for obtaining diagnostic information not from the fact of any signal detection, but from the temporal profile of generated stress wave; (3) use of wide-band piezoelectric detectors to correctly reproduce stress profiles (acoustic waves with wide spectrum of ultrasonic frequencies) to obtain high spatial resolution of tomography. The laser opto-acoustic imaging system (LOAIS) of the present invention partially combines elements of (1) ultrasonic scanning, (2) optical time-resolved tomography and (3) selective pulsed excitation of tissue heterogeneous structures and time-resolved detection of laser-induced stress waves for obtaining detailed medical diagnostic information.

The present invention is directed to both a technique and a device and can be used to image a complex tissue structure on the basis of optical contrast. The technique of the present

invention uses a pulsed laser to slightly but quickly heat a specific tissue region with an optical absorption that differs relative to its surroundings. This slight heating converts to a pressure wave, i.e., a sound wave which propagates outward from the source of the heating. A transducer detects the time, magnitude and shape of the arriving pressure waves. The transducer may be a piezoelectric transducer at the tissue surface or an imbedded transducer. The laser pulse must be sufficiently short to allow the pressure to build up before the pressure can dissipate at the speed of sound (approximately 1500 m/s). For example, a 10-ns laser pulse can image absorbing objects with the spatial resolution of  $(1500 \text{ m/s}) (10 \text{ ns}) = 15 \text{ } \mu\text{m}$ . Thus, the invention allows imaging of tissue structures with high spatial resolution within turbid media such as biological tissues. The imaging techniques of the present invention are based on optical contrast rather than density changes such as in ultrasound, magnetic resonance imaging or x-ray computed tomography. The method of the present invention, therefore, can be used to image contrast objects not well imaged by these other state of the art imaging techniques.

Thus, in one aspect, the present invention provides a method of characterizing a tissue using high spatial resolution laser optoacoustic imaging, comprising the steps of: illuminating a volume of said tissue with at least one laser pulse having a pulse length or a pulse duration shorter than a time required for a transient pressure wave generated by said laser pulse(s) to propagate a distance equal to a length of a selected spatial resolution; selectively heating with said laser pulse(s) at least one object or layer of diagnostic interest within said illuminated volume; generating the pressure profile, wherein said pressure profile characterizes the distribution of said tissue optical properties in said illuminated volume and represents a value of pressure as a function of depth within said illuminated volume; detecting said pressure profile with at least one acoustic transducer; recording an amplitude and temporal profile of said pressure profile by an electronic system; analyzing said pressure profile using a computer; and reconstructing a high resolution image of said characterized tissue for display from the analyzed pressure profile using the computer.

5  
10  
15  
In one embodiment of the present invention, there is provided a method of diagnosing a diseased tissue within a normal tissue using laser optoacoustic tomography, comprising the steps of: irradiating the surface of the normal tissue with at least one laser pulse so as to penetrate to a sufficient depth and selectively heat a small volume or layer of diseased tissue with a higher optical absorption; causing the diseased tissue to produce a stress wave with a profile resembling that of diseased tissue, said stress wave propagates with minimal alterations to the surface of normal tissue; detecting said stress wave with at least one acoustic transducer; recording the amplitude and temporal profile of laser-induced stress wave by digital oscilloscope; analyzing the amplitude and temporal profile of laser-induced stress wave with a computer.

15  
In another embodiment of the present invention, there is provided a novel device as a tomography system for biomedical diagnostics comprising: a pulsed laser; a light delivery system; at least one acoustic detector; an electronic system for signal

recording and processing; and a computer with software for image reconstruction and analysis.

Other and further aspects, features, and advantages of the present invention will be apparent from the following  
5 description of the presently preferred embodiments of the invention given for the purpose of disclosure.

### BRIEF DESCRIPTION OF THE DRAWINGS

10 So that the matter in which the above-recited features, advantages and objects of the invention, as well as others which will become clear, are attained and can be understood in detail, more particular descriptions of the invention briefly summarized  
15 above may be had by reference to certain embodiments thereof which are illustrated in the appended drawings. These drawings form a part of the specification. It is to be noted, however, that the appended drawings illustrate preferred embodiments of the invention and therefore are not to be considered limiting in their scope.

20 Figure 1 shows a schematic of the laser optoacoustic tomography system in transmission mode.

Figure 2 shows that an acoustic transducer signal can be detected *in vitro* from small volume of liver placed inside large volume of chicken breast muscle tissue.

25 Figure 3 shows that an acoustic transducer signal can be detected from a phantom pathologic tissue (2.5 mm colored gel sphere) embedded within large volume of optically turbid gel cylinder simulating woman's breast. Signal recorded from gel cylinder in case when laser pulse misses and therefore does not  
30 heat small color sphere is also presented for comparison.

Figure 4 shows a schematic of laser optoacoustic tomography in reflection mode.

Figure 5 shows an acoustic transducer signal detected  
35 *in vivo* from chicken cockscomb best known model for port-wine stains.

Figure 6 shows an acoustic transducer signal detected *in vivo* from small tumor located underneath the skin of mouse's lower back.

## DETAILED DESCRIPTION OF THE INVENTION

### Definitions

5 As used herein, the term "laser optoacoustic tomography" refers to a laser optoacoustic tomography system that employs detection of stress waves reflected from the volume of their generation back to the irradiated tissue surface. In other words, laser optoacoustic tomography is a diagnostic procedure to obtain optical images of layered tissue while detecting laser  
10 induced stress profiles.

As used herein, the term "tomography in reflection transmission mode" refers to the laser optoacoustic tomography system of the present invention that employs the detection of stress waves transmitted from the volume of their generation to  
15 rear tissue surfaces, i.e., opposite to irradiated.

As used herein, the term "transient stress waves" refers to a stress wave that has limited duration and occupies limited volume.

20 As used herein, the term "temporal stress confinement" refers to the confinement of laser-induced stress within heated volume during the course of laser energy deposition.

As used herein, the term "time-resolved detection of stress profile" refers to the detection of transient stress waves  
25 with temporal resolution sufficient to reconstruct a pressure wave profile with precision.

As used herein, the term "optical time-resolved tomography" refers to a tomography based on time-resolved detection of ultrashort laser pulses transmitted through biological  
30 tissue of diagnostic interest.

As used herein, the term "piezoelectric detectors" refers to detectors of acoustic, e.g., stress waves utilizing the principle of electric charge generation upon a change of volume within crystals subjected to a pressure wave.

35 As used herein, the term "ultrasonic scanning" refers to a diagnostic procedure that employs delivery of ultrasonic stress waves to a tissue surface followed by the detection of the signals reflected from boundaries within the tissue under diagnosis.

As used herein, the term "pulsed heating of tissue" refers to the heating of a tissue volume irradiated with laser pulses.

5 The present invention utilizes the time-resolved  
detection of laser-induced stress (ultrasonic) waves to obtain  
tomography images of human organs or cellular structures for  
diagnostic purposes. Diagnostic procedures in which the laser  
opto-acoustic imaging system of the present invention are useful  
include: (1) short laser pulses delivered to the front surface of  
10 human organ under investigation. Laser wavelength must be  
selected to achieve desirable light penetration depth and maximum  
contrast between normal and abnormal tissues. Heterogeneous  
absorption of photons and heating of tissue causes generation of  
thermo-elastic stress that is temporarily confined in the irradiated  
15 volume. Short laser pulses serve three purposes: (1) obtain the  
most effective generation of transient stress, (2) obtain a stress  
profile which resembles the profile of heterogeneous light  
distribution, (3) to obtain images with ultimate accuracy of  
localization of tissue layer or volume of diagnostic interest.

20 Transient stress waves will propagate toward acoustic  
transducer (detector). A transducer, e.g., a piezoelectric  
transducer, will convert the stress profile into an electrical signal.  
The temporal profile of the electrical signal recorded by a digital  
oscilloscope is converted into a spatial profile of a transient stress  
25 distribution. Transient stress distribution resembles a profile of  
absorbed laser energy distribution, which in turn carries certain  
diagnostic information. Both a laser beam and a piezoelectric  
transducer (detector) are scanned over the area under diagnosis.  
Positioning of a detector at various locations permits reconstruction  
30 of a three dimensional opto-acoustic image from transient stress  
profiles and time-delays between moments of laser pulsed  
irradiation and moments of stress detection (the speed of acoustic  
waves propagation is known for vast majority of tissues). Stress  
detection can be performed in both, the transmission mode and the  
35 reflection mode, which allows substantial flexibility for *in*  
*vivo* diagnostics of various human organs and other biological  
systems.

Laser opto-acoustic imaging systems (LOAIS) can be used in diagnostic screening of breast cancer (mammography), skin tumors and various other lesions (like port-wine stains etc.) whether accessible externally or via endoscopes, detection of brain  
5 hematomas (hemorrhages), atherosclerotic lesions in blood vessels, and for general characterization of tissue composition and structure. In addition, laser opto-acoustic imaging can provide feedback information during laser medical treatments.

Thus, the present invention is directed to a method of  
10 diagnosing a diseased tissue within a normal tissue using laser optoacoustic tomography, comprising the steps of: irradiating the surface of the normal tissue with at least one laser pulse so as to penetrate to a sufficient depth and selectively heat a small volume or layer of diseased tissue with a higher optical absorption; causing  
15 the diseased tissue to produce a stress wave with a profile resembling that of diseased tissue, said stress wave propagates with minimal alterations to the surface of normal tissue; detecting said stress wave with at least one acoustic transducer; recording the amplitude and temporal profile of laser-induced stress wave  
20 by digital oscilloscope; analyzing the amplitude and temporal profile of laser-induced stress wave with a computer.

Preferably, the stress profiles are recorded and analyzed by the computer to reconstruct a three-dimensional image. Generally, the laser pulse heats certain tissue structures  
25 with different light absorption thereby generating stress profiles resembling profiles of absorbed laser energy distribution in heterogeneous tissues followed by time-resolved detection of ultrasonic stress waves. The shape and dimensions of the diseased tissue volume or layer is generally determined from the temporal  
30 profile of laser-induced stress, the time of stress wave arrival to the acoustic transducer, and the direction of the stress detection.

Preferably, the acoustic transducer is a piezoelectric detector and the acoustic transducer uses temporal resolution. Ordinarily, the transducer determines the geometry of the  
35 diagnosed tissue volume without scanning of acoustic transducer at a fixed location of the laser beam. However, multiple separate optical fibers or laser beams can be used to irradiate large volume of tissue to reduce time of scanning and incident laser fluence.

Generally, the amplitude and temporal profile of laser-induced stress wave is recorded by a digital oscilloscope.

In the methods of the present invention, stress detection can be in transmission mode and stress detection of tissue optical heterogeneities occurs at a tissue depth of up to about 12 cm. Alternatively, stress detection can be in reflection mode. Generally, the irradiating is in spectral range of therapeutic window from about 600 nm to about 1400 nm. It is further contemplated that one with ordinary skill in this art could use exogenous molecular probes or dyes to enhance contrast of tomographic image.

Generally, the methods of the present invention may be used to diagnose a wide variety of diseased tissue. Preferably, the diseased tissue is breast carcinoma, brain hemorrhages, hematomas, atherosclerotic plaques, polyarthritis, port-wine stains, skin disorders, melanomas or ocular diseases.

When the diseased tissue is an internal organ, the irradiation may be delivered via an endoscope and the acoustic transducer may be positioned on the skin surface. Alternatively, the irradiation may be delivered onto the skin surface and the transducer is incorporated with an endoscope and positioned inside the organs. Further, when the diseased tissue is an internal organ, the optical fiber and transducer may be incorporated in endoscope and positioned inside the organs.

The present invention also provides a novel device as a tomography system for biomedical diagnostics comprising: a pulsed laser; a light delivery system; at least one acoustic detector; an electronic system for signal recording and processing; and a computer with software for image reconstruction and analysis.

The following examples are given for the purpose of illustrating various embodiments of the invention and are not meant to limit the present invention in any fashion.

With reference to the appended drawings, Figure 1 illustrates one embodiment of the present invention, i.e., an example of the utility of laser optoacoustic tomography in diagnosing a small diseased tissue volume (black circle) within a large volume of normal tissue. The laser pulse irradiates the surface of the normal tissue and penetrates to a sufficient depth to

selectively heat a small volume of diseased tissue with a higher optical absorption. Instantly, the heated volume of diseased tissue produces a stress wave with a profile resembling that of diseased tissue. The stress wave propagates with minimal alterations to the surface of normal tissue where it is detected by an acoustic transducer with temporal resolution. The amplitude and temporal profile of laser-induced stress wave is recorded by digital oscilloscope and transferred via an interface to a computer for data analysis. Scanning of laser beam (optical fiber) allows the irradiation of the entire volume of the tomographically scanned organ and definite heating of any diseased tissues that exist within normal tissue. Scanning of the acoustic transducer along the surface of the organ permits a determination of the exact location of any diseased tissue volumes. The stress profiles are recorded and analyzed by the computer to reconstruct three dimensional images which can be displayed.

Tomography (imaging) in stress transmission mode utilizes detection of stress transients transmitted from the laser-excited volume toward the depth through thick layers of tissue. The emphasis in transmission mode tomography is made on sensitive detection of tissue optical heterogeneities located at substantial depth of tissue (up to 12 cm).

Figure 2 depicts an example of a measurement of laser-induced transient stress in a small piece of bovine liver tissue placed between muscle tissues slabs (chicken breast). Duration of the transient stress wave and amplitude were equal to 300 ns and 4 mbar, respectively, in accordance with sample thickness and optical absorption coefficient. This experiment demonstrated the ability of laser optoacoustic tomography to detect small volumes of tissue (3 mm x 2 mm x 0.5 mm) with absorption coefficient,  $\mu_a = 0.215 \text{ cm}^{-1}$ , that is slightly higher than that of surrounding tissue,  $\mu_a = 0.09 \text{ cm}^{-1}$ , at the depth of more than 4 centimeters.

Figure 3 shows an acoustic transducer signal detected from a phantom pathologic tissue (2.5 mm colored gel sphere) embedded within large volume of optically turbid gel cylinder. A control signal was used in case the laser irradiation "missed" the colored sphere and is also shown. The gel phantom simulated a woman's breast by having optical properties of a colored gel

sphere similar to those found in breast carcinoma. Moreover, the optical properties of the surrounding gel were similar to those in a woman's breast tissue. The geometry of the experiment is also shown. A laser pulse was delivered from one side of the gel cylinder and a transient stress wave was detected from the opposite side. The location of colored gel sphere which simulated the tumor was not known to the person who performed the diagnostic procedure. Simultaneous scanning of laser beam and acoustic transducer revealed both the location and dimensions of the "tumor".

Figure 4 shows a schematic diagram of the laser optoacoustic tomography of the present invention in the reflection mode embodiment of stress detection. A laser pulse irradiates the surface of tissue with a wavelength chosen to penetrate the tissue superficially (about 1 mm) and to heat selectively all microstructures within the tissue with the objective of obtaining high contrast and high spatial resolution. Instantly heated volume of layered tissue produces a stress wave that has profile indicating tissue structure. Stress waves were reflected toward the irradiated surface and were detected with minimal alterations by an acoustic transducer with nanosecond temporal resolution. Laser pulses were delivered to the same tissue surface where a stress wave was detected. The amplitude and temporal profile of a laser-induced stress wave was recorded by a digital oscilloscope and transferred via an interface to a computer for data analysis. Scanning by acoustic transducer-reflectometer with the laser beam permitted the irradiation of the entire area of diagnostic interest. Recorded stress profiles were analyzed by the computer to reconstruct a three dimensional image which was displayed and processed by special software.

Tomography (imaging) in stress reflection mode utilizes detection of stress transients generated in superficial tissue layer and reflected back toward tissue surface. The emphasis in reflection mode tomography is made on high spatial resolution of measured image (up to 1.5  $\mu\text{m}$ ).

Figure 5 depicts a z-axial optoacoustic image of absorbed laser fluence distribution in cock's comb. The transient stress profile induced by a 14-ns pulse at 532 nm in a cock's comb

of a rooster was measured *in vivo* by an acoustic transducer. The laser beam was about 1 cm in diameter. Time "0" corresponds to a signal detected from the tissue surface. Distinct layers were observed in the cock's comb tissue. Alteration of the detected stress transient due to diffraction of acoustic waves generated in distributed capillary blood vessels (layer 2) yields negative signal. When diffraction effects are compensated, or the transient stress measured under diffraction-free conditions such as in a layered system with homogeneous absorption within each layer, the stress profile will have only positive components. Signals 1-6 were induced in blood vessels, located at different depths in the tissue. Numbers 1-5 correspond to the acoustic transducer signals detected in layers with either enhanced density of small blood vessels (1 and 2) or in separated large blood vessels (3, 4 and 5). The layered structure of the cock's comb is clearly depicted (the layer with dense small dermal blood vessels that lies just below the epidermis, the layer of less vascular loose connective tissue, the comb core layer with arteries and veins that supply the more superficial vascular layers of the cockscomb). The depth of their location is measured correctly if compared with cockscomb histology. The lateral position can be found by scanning a focused laser beam along the tissue surface.

Figure 6 shows a display of a typical profile of a stress wave induced by nanosecond laser pulses at 532 nm in tissues of a mouse with a small tumor beneath the skin. Signals detected from the volume with cancer and from the tissue with no cancer are presented for comparison. The difference between two presented signals indicate that breast tumor can be diagnosed with laser optoacoustic tomography system of the present invention in a mice model *in vivo*. This is another example of laser optoacoustic tomography system of the present invention in the reflection embodiment performed *in vivo*. The object of study was a mouse with a cancer modeling female's breast tumor grown inside the muscle of the mouse. The imaging experiment was performed twice with two different mice with similar tumor conditions. These embodiments presented demonstrated laser optoacoustic imaging in tissues by time-resolved detection of laser-induced stress transients.

Any patents or publications mentioned in this specification are indicative of the levels of those skilled in the art to which the invention pertains.

One skilled in the art will readily appreciate that the present invention is well adapted to carry out the objects and obtain the ends and advantages mentioned, as well as those inherent therein. The present examples along with the methods, procedures, treatments, molecules, and specific compounds described herein are presently representative of preferred embodiments, are exemplary, and are not intended as limitations on the scope of the invention. Changes therein and other uses will occur to those skilled in the art which are encompassed within the spirit of the invention as defined by the scope of the claims.

**CLAIMS:**

1. A method of characterizing a tissue using high spatial resolution laser optoacoustic imaging, comprising the steps of:

illuminating a volume of said tissue with at least one laser pulse having a pulse length or a pulse duration shorter than a time required for a transient pressure wave generated by said laser pulse(s) to propagate a distance equal to a length of a selected spatial resolution;

selectively heating with said laser pulse(s) at least one object or layer of diagnostic interest within said illuminated volume;

generating the pressure profile, wherein said pressure profile characterizes the distribution of said tissue optical properties in said illuminated volume and represents a value of pressure as a function of depth within said illuminated volume;

detecting said pressure profile with at least one acoustic transducer;

recording an amplitude and temporal profile of said pressure profile by an electronic system;

analyzing said pressure profile using a computer; and

reconstructing a high resolution image of said characterized tissue for display from the analyzed pressure profile using the computer.

2. The method of claim 1, further comprising:

positioning a plurality of said acoustic transducers at fixed locations along the surface of said illuminated volume of tissue in order to reconstruct said high resolution image.

3. The method of claims 1 or 2, further comprising:  
  
positioning separately a plurality of pulsed laser sources or of optical fibers to illuminate a larger volume of said tissue thereby improving image quality.
  
4. The method of claim 1, further comprising:  
  
incorporating one or both of said at least one acoustic transducers and said pulsed laser source or said optical fiber into a means of positioning on said tissue.
  
5. The method of any one of claims 1 to 4, further comprising:  
  
enhancing contrast between pressure profiles of different tissues with an exogenous contrast agent.
  
6. The method of claim 5, wherein said exogenous contrast agent is at least one molecular dye or probe.
  
7. The method of any one of claims 1 to 6, wherein said at least one acoustic transducer is an ultrasonic transducer having a band width sufficiently wide to detect said pressure profile without distortion for the pulse length or duration at the selected length of spatial resolution.

8. The method of any one of claims 1 to 7, wherein said acoustic transducer(s) detects said pressure profile with temporal resolution defined by the selected spatial resolution.

9. The method of any one of claims 1 to 8, wherein said acoustic transducer(s) detects a pressure profile originating at a tissue depth of up to 12 cm.

10. The method of any one of claims 1 to 9, wherein said laser pulse(s) has a wavelength within a spectral range from about 600 nm to about 1400 nm.

11. The method of any one of claims 1 to 10, wherein said wavelength corresponds to the absorption band of molecules, cells or tissues of diagnostic interest.

12. The method of any one of claims 1 to 11, wherein said characterized tissue comprises breast cancer, prostate cancer, a brain hemorrhage or cancer, a hematoma, blood or blood vessel, atherosclerotic plaque, an arthritic joint, a port-wine stain, a melanoma, a skin lesion, colon cancer, esophageal cancer, oral cancer, or an ocular diseased tissue.

13. An imaging system configured to reconstruct an image of high spatial resolution of a tissue of diagnostic interest, comprising:

a pulsed laser source to produce conditions of pressure profile confinement in a volume of tissue of diagnostic interest; wherein said pulsed laser source has a pulse length

or a pulse duration shorter than a time required for a pressure wave comprising said pressure profile to propagate a distance equal to a length of spatial resolution;

a light delivery system for delivery of illumination to said tissue of diagnostic interest;

at least one acoustic transducer to detect said pressure profile in said volume of tissue of diagnostic interest;

an electronic system for recording and processing said detected pressure profile, and

a computer with software for analysis of said detected pressure profiles and for image reconstruction with high spatial resolution from at least one of said detected pressure profiles.

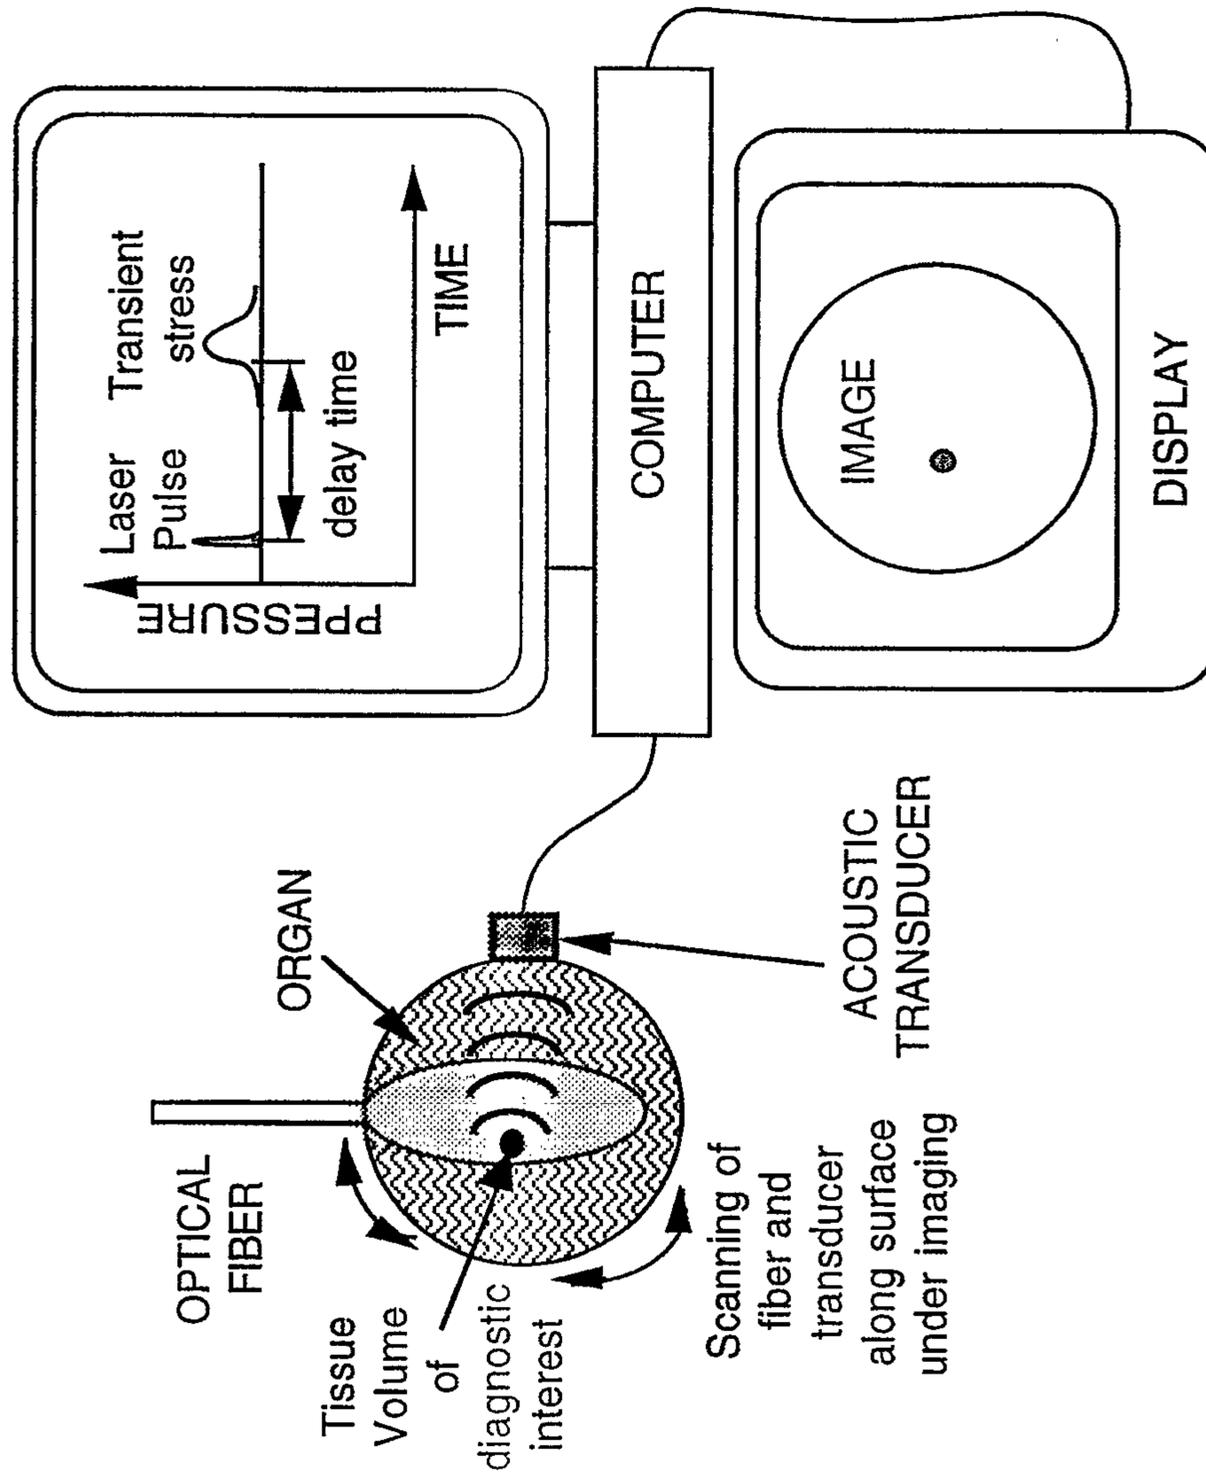


FIGURE 1

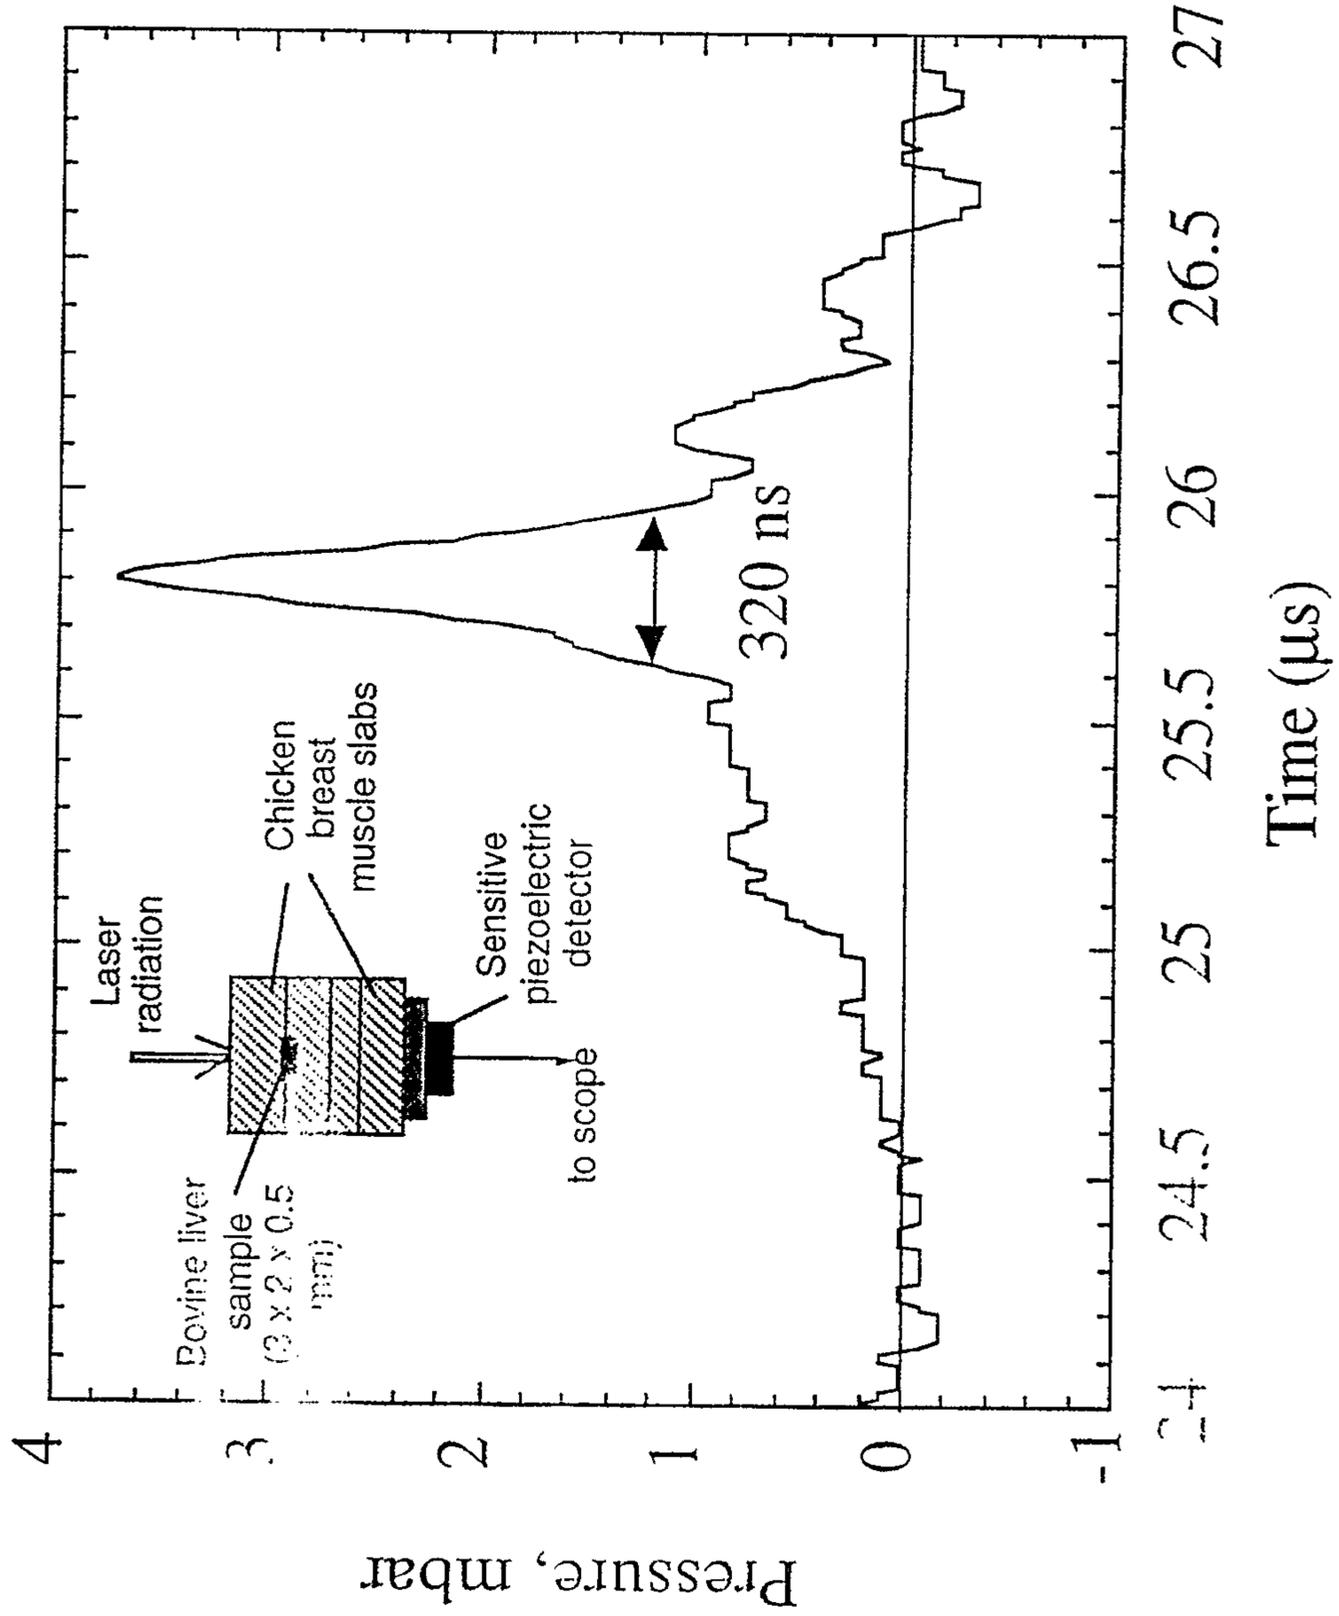


FIGURE 2

3/6

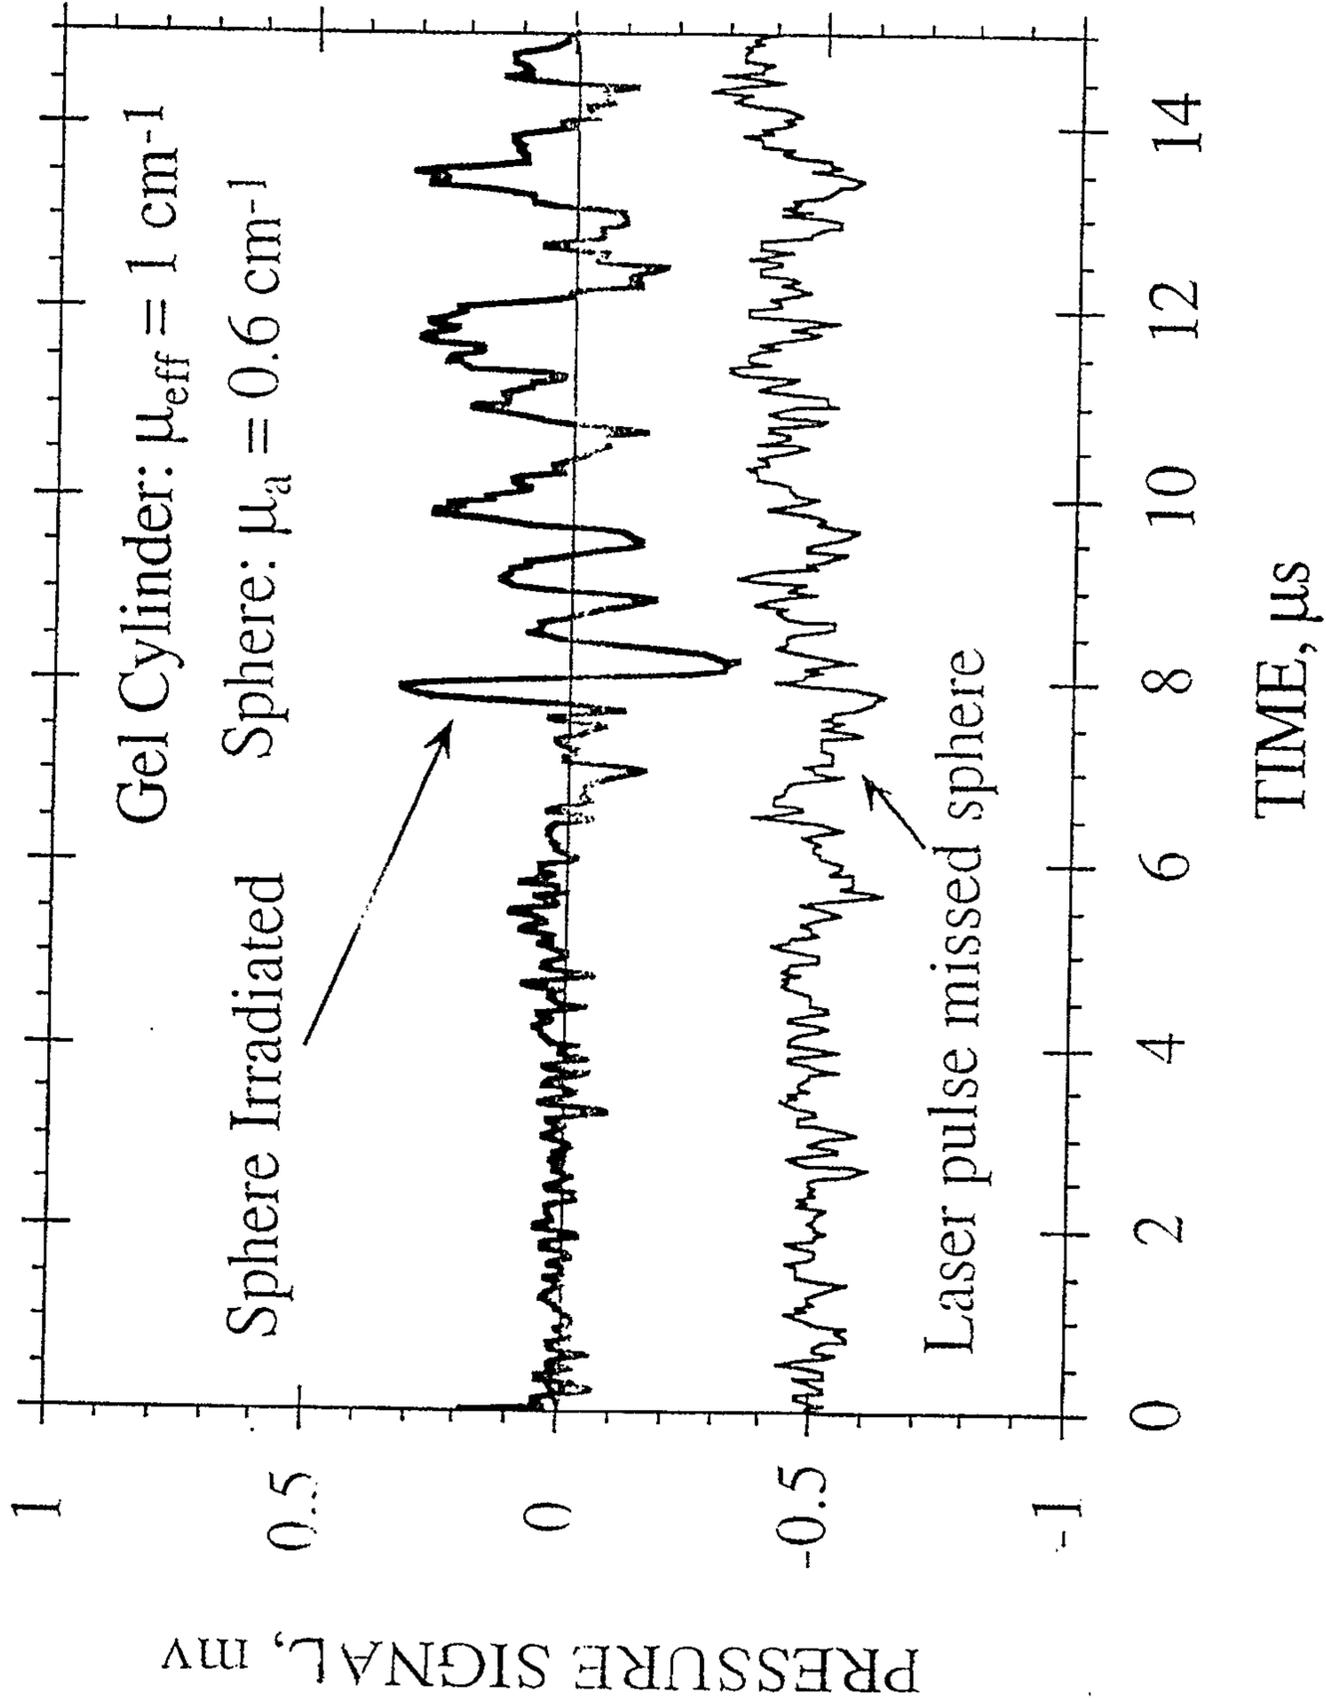


FIGURE 3

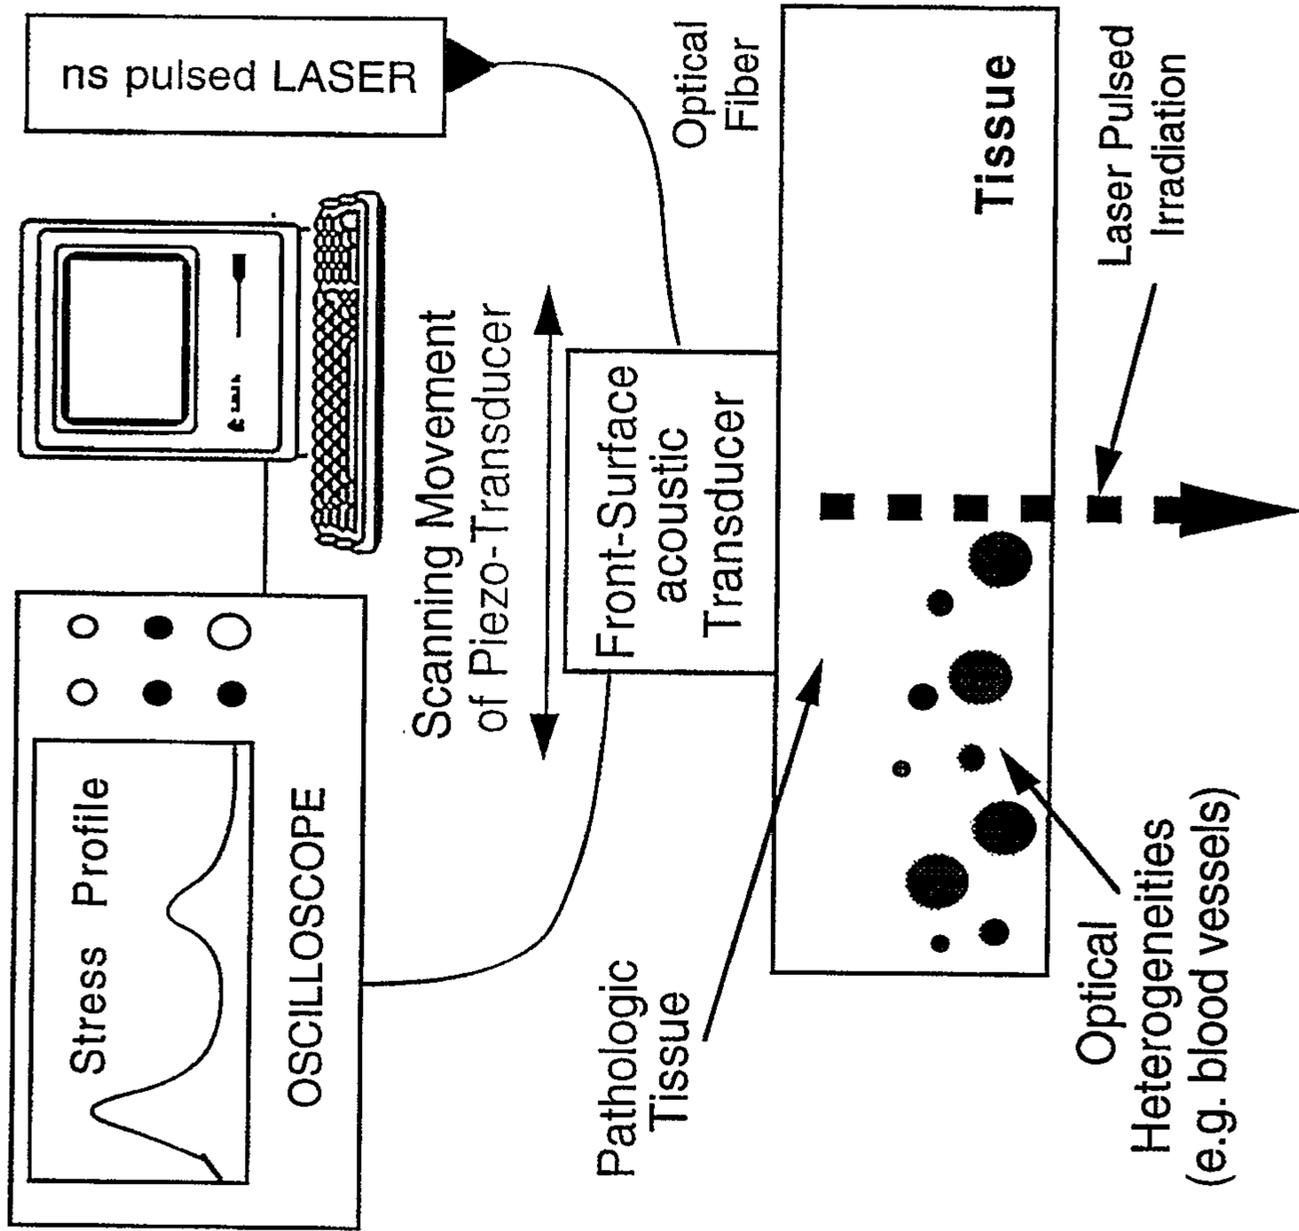


FIGURE 4

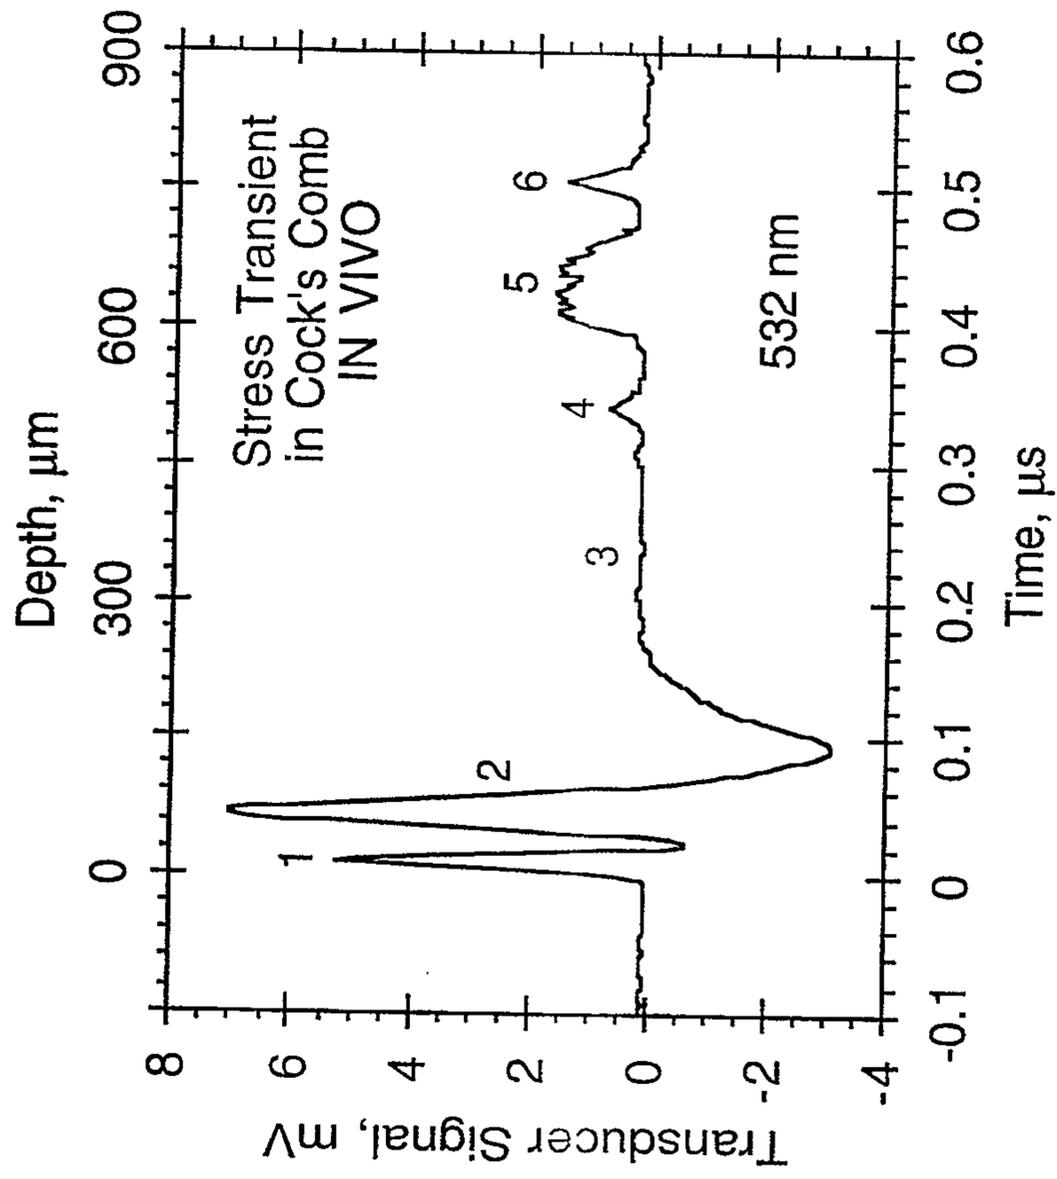


FIGURE 5

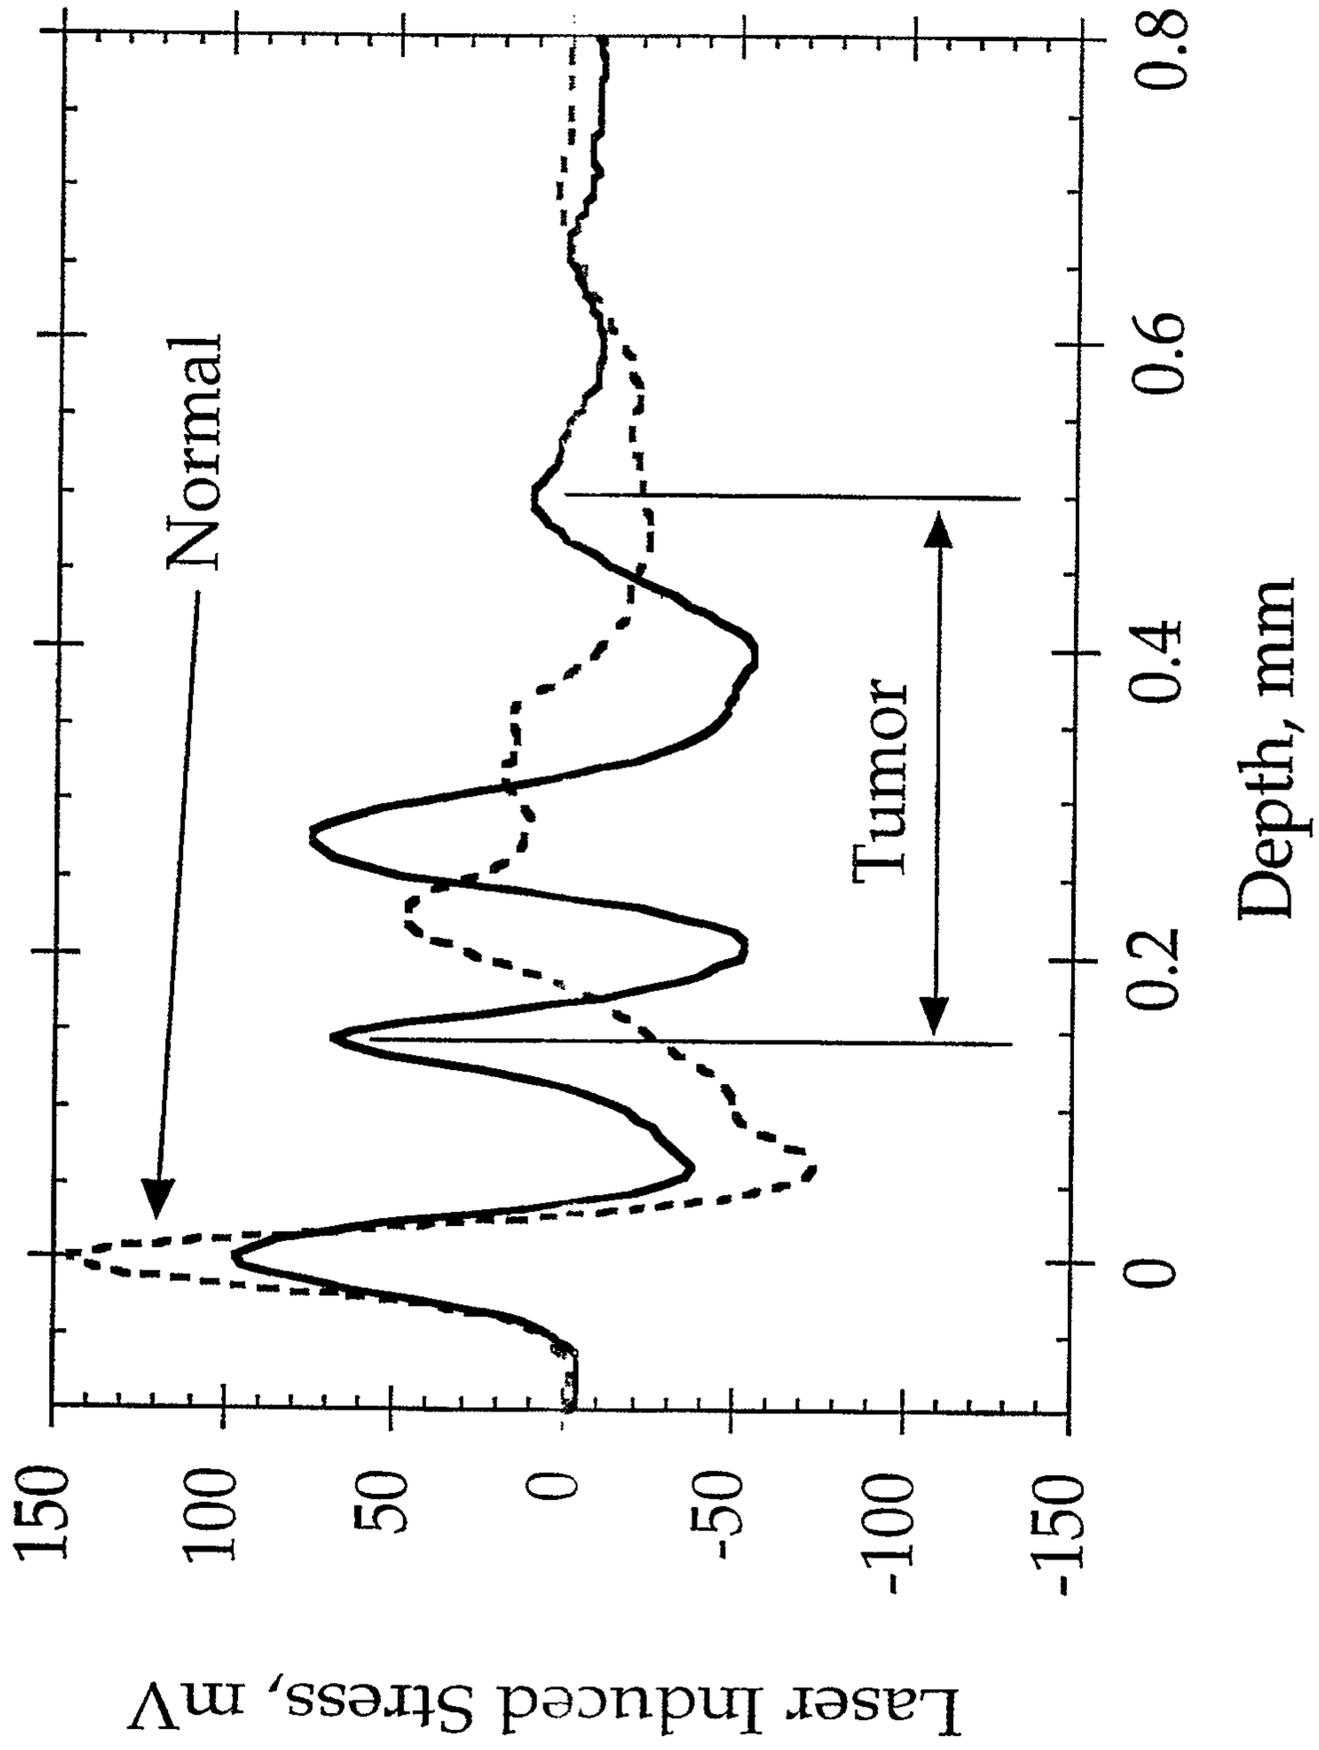


FIGURE 6

