



(43) International Publication Date
18 September 2014 (18.09.2014)

(51) International Patent Classification:
A61F 2/44 (2006.01)

(21) International Application Number:
PCT/US2014/030585

(22) International Filing Date:
17 March 2014 (17.03.2014)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/792,173 15 March 2013 (15.03.2013) US

(71) Applicant: **PARADIGM SPINE, LLC** [US/US]; 505
Park Avenue, 14th Floor, New York, NY 10022 (US).

(72) Inventors: **GANTER, Detlev**; Goethestrabe 9, D-78199
Braunlingen (DE). **ECKHOF, Stephan**; Schuberstrabe 16,
78604 Rietheim-weilheim (DE). **EISEN, Guntmar**;
Heubergweg 8, 78532 Tuttlingen (DE). **MUCKENFUB,**
Sven, Oliver; Aldinger Strabe 52, 78549 Spaichingen
(DE). **SALVERMOSER, Markus**; Am Muhlberg 14,
78532 Tuttlingen-mohringen (DE).

(74) Agent: **NGUYEN, Tram, Anh**; Monument IP Law Group,
1717 Pennsylvania Avenue, NW, Suite 900, Washington,
DC 20006 (US).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,


AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.

(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments (Rule 48.2(h))*

(54) Title: MODULAR, CUSTOMIZABLE SPINE STABILIZATION SYSTEM

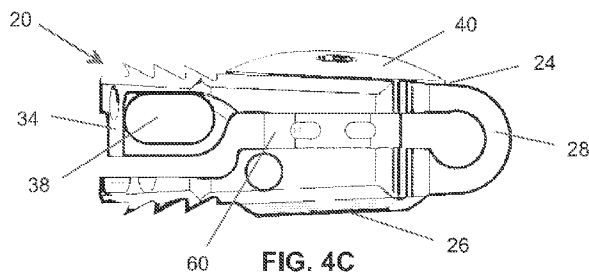

(57) Abstract: A modular, customizable system that provides components for assembling an implantable device is provided. The system allows the user to assemble an implantable spine stabilization device that is flexible and allows dynamic stabilization. The same system also provides components for assembling a rigid or non-flexible fusion-enabling spine stabilization device. The components of the system are easily interchangeable, allowing the user the ability to customize the assembled device for a true fit with the patient, as well as allow an easy conversion of the dynamic device into a fusion-enabling device. Associated insertion instruments and methods of use are also disclosed.



WO 2014/145766 A1

MODULAR, CUSTOMIZABLE SPINE STABILIZATION SYSTEM

TECHNICAL FIELD

The present disclosure relates to implantable spine stabilization devices, associated insertion instruments and related methods. More specifically, the present disclosure relates to a modular, customizable system that provides components for assembling an implantable spine stabilization device that can be flexible and allow dynamic stabilization in one application, and converted into a rigid or non-flexible fusion-enabling device in another application.

BACKGROUND ART

Fusion of the spine is a well-known and widely practiced medical procedure to alleviate severe back and/or neck pain due to misaligned, damaged or otherwise diseased spines. In some cases, the fusion is carried out by implanting a cage, or implantable device having an opening for the ingrowth of tissue therethrough, at the level of the spine to be fused. The opening may be filled with, or contain, bone graft material, bone chips or other biologically active material that enhances fusion.

Where it is difficult to maneuver and insert a rigid implantable device due to the size limitations or delicate anatomical site (i.e., closeness to nerves or spinal cord, e.g.) of the area to be implanted, it is desirable to provide an implant that may be converted from a flexible implant into a rigid one that can promote fusion. Expandable fusion cages are well known in the art. Most of these fusion cages comprise two or more components that cooperate together to form a fusion promoting device. For instance, a typical expandable spinal implant can comprise a flexible fusion cage and a corresponding insert that, when inserted, expands the fusion cage.

As further examples of expandable spinal implants, U.S. Patent Application Publication No. 2010/0234956 entitled "EXPANDING CAGE FOR VERTEBRAL SURGERY" to Attia et al. describes an expanding intervertebral implant comprising

an intervertebral fusion cage and an insertable rod for placement inside the cage to expand the cage after implantation. U.S. Patent No. 7,578,849 entitled “INTERVERTEBRAL IMPLANTS AND METHODS OF USE” by Trieu described another two-component intervertebral spinal stabilization implant having a fusion cage and an elastic component for insertion into the fusion cage. U.S. Patent No. 6,102,950 entitled “INTERVERTEBRAL BODY FUSION DEVICE” by Vaccaro describes a two-component fusion promoting implant comprising an intervertebral body fusion device having a cage component for placement intervertebrally, and a wedge body that is insertable into the cage component.

However, these expandable spinal implants are not intended for use without their inserts. In other words, these implants are not configured for conversion from a functional dynamic implant into a fusion implant at a later time.

Dynamic implants having the desired anatomical shape and size conducive for dynamic spinal stabilization are known. One such implant is described in U.S. Patent No. 7,867,276 entitled “DYNAMIC INTERVERTEBRAL IMPLANT” by Matge. However, this dynamic intervertebral implant is not configured to be easily converted into a fusion promoting implant at a later time.

Accordingly, there exists a need for a modular, convertible implant system that can be used in either dynamic or fusion-promoting modes, or both, at different points of time.

SUMMARY OF THE INVENTION

The present disclosure provides a modular, customizable system that provides components for assembling an implantable spine stabilization device that can be flexible and allow dynamic stabilization in one application, and converted into a rigid or non-flexible fusion-enabling device in another application. The assembled devices may be configured for use in the lumbar, thoracic, or cervical region of the spine. Methods for implantation and use are also disclosed, along with associated insertion instruments and tools.

In one exemplary embodiment, an implantable spine stabilization device is provided. The device may comprise a main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates, the superior plate having an opening extending therethrough for receiving a domed cap, the domed cap comprising a domed top and a stem configured for insertion into the opening on the superior plate, wherein the main body is compressible and distractable.

In one embodiment, the domed cap may be eccentric. In another embodiment, the cap may be centric. In still another embodiment, the inferior plate may also include an opening for receiving a domed cap. The device is configured to be implantable in both a lateral and a ventral approach.

In another exemplary embodiment, an implantable spine stabilization device is provided. The device may comprise a compressible and distractable main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates, the superior plate having an opening extending therethrough for receiving a domed cap, the domed cap comprising a domed top and a stem configured for insertion into the opening on the superior plate, the domed top including a through-hole. A compression-blocking insert configured for placement in between the superior and inferior plates may also be provided, the insert being sized to fit entirely within the main body.

In one embodiment, the through-hole of the domed top may be filled with bone graft material, bone cement, bone substitute material, bone hardening material, bone void filler, demineralized bone matrix, or other similar materials. The domed

cap may be eccentric, or it may be centric, and may also include surface features or a coating to enhance bone growth. In still another embodiment, the inferior plate may also include an opening for receiving a domed cap. The device is configured to be implantable in both a lateral and a ventral approach.

In still another exemplary embodiment, a modular spine stabilization system is provided. The system may comprise a plurality of compressible and distractable main bodies, each main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates. The system may further include a plurality of domed caps, each domed cap comprising a domed top and a stem configured for insertion into an opening on the superior plate. A plurality of compression-blocking inserts can also be provided with the system. Each of the inserts may be configured for placement in between the superior and inferior plates, the insert being sized to fit entirely within the main body.

In yet another embodiment, the domed top may include a through-hole that can also be filled with bone graft material, bone cement, bone substitute material, bone hardening material, bone void filler, or other similar materials. The domed cap may be eccentric, or it may be centric, and may also include surface features or a coating to enhance bone growth. In still another embodiment, the inferior plate may also include an opening for receiving a domed cap. This domed cap for the inferior plate may optionally include a through-hole that can also be filled with bone graft material, bone cement, bone substitute material, bone hardening material, bone void filler, demineralized bone matrix, or other similar materials.

In yet another exemplary embodiment, a method of treating a spinal instability of an intervertebral space is provided. The method may comprise the steps of: providing a modular spine stabilization system comprising: a plurality of compressible and distractable main bodies, each main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates; a plurality domed caps, each domed cap comprising a domed top and a stem configured for insertion into an opening on the superior plate; and a plurality of compression-blocking inserts, each insert being configured for placement in between the superior and inferior plates, the insert being sized to fit entirely within the main body; selecting

a main body for insertion into the intervertebral space; selecting a domed cap based on a morphological profile of the intervertebral space; attaching the domed cap to the superior plate of the main body; compressing the main body; and inserting the main body into the intervertebral space.

A trial may be used prior to implantation to ascertain the morphology of the intervertebral space, and to determine the appropriate sized and/or shaped domed cap to insert into the main body. The step of inserting the compression-blocking insert may also comprise selecting an insert having a height that adjusts lordotic curvature, such as a height greater than the device. The insert may also be angled and thus provide distraction as well as lordotic adjustment to achieve sagittal balance. Additionally, a compression-blocking insert may be selected having an appropriate angle such that, when inserted, will adjust the angle of the device itself.

The implantable devices of the present disclosure may be suitable for either dynamic spine stabilization, or for fusion applications, or both. For example, it is possible to convert a previously dynamic spine stabilization device into a fusion-enabling device by the introduction of the compression-blocking inserts of the present disclosure. In some cases, it is also possible to implant the device with the insert in a fusion-promoting situation, and then remove the insert at a later time to allow dynamic stabilization with the device.

The devices are configured to be stand-alone devices. However, it is also possible to utilize these devices with a posterior fixation device or system for total 360 degree stabilization. In some embodiments, the devices may be configured for use with fixation screws. For instance, in one exemplary embodiment, the compression-blocking insert may be configured for attachment to the vertebral bodies with fixation screws. In one embodiment, the inserts may comprise an attachment plate for receiving the fixation screws. In another embodiment, the fixation screws may be attached to the main body.

It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory only and are not restrictive of the disclosure. Additional features of the disclosure will be set forth in part in the description which follows or may be learned by practice of the disclosure.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate several embodiments of the disclosure and together with the description, serve to explain the principles of the disclosure.

FIG. 1 illustrates an exemplary spine and an intervertebral space to be stabilized using the device of the present disclosure.

FIG. 2 illustrates a graphical representation of the morphological profile of the intervertebral space of FIG. 1.

FIGS. 3A—3G illustrate an exemplary embodiment of a spine stabilization device of the present disclosure, in which:

FIG. 3A shows an exploded view of the spine stabilization device;

FIG. 3B shows a top planar view of the spine stabilization device of FIG. 3A;

FIGS. 3C and 3D illustrate alternative ways to attach the body of the spine stabilization device with the domed cap;

FIG. 3E shows a cutaway view of the domed cap attached to the body of the spine stabilization device;

FIG. 3F shows a side view of the spine stabilization device of FIG. 3E; and

FIG. 3G shows a bottom perspective view of the spine stabilization device of FIG. 3E.

FIGS. 4A—4D illustrate an exemplary embodiment of another spine stabilization device, in which:

FIG. 4A shows an exploded view of the spine stabilization device;

FIG. 4B illustrates a partial cutaway view of the spine stabilization device of FIG. 4A;

FIG. 4C illustrates a side view of the spine stabilization device of FIG. 4A; and

FIG. 4D illustrates a front view of the spine stabilization device of FIG. 4A.

FIGS. 5A—5C illustrate a method of using a trial to assess the anatomical site for implantation in a lateral approach.

FIGS. 6A—6G illustrate a method of inserting the spine stabilization device of FIG. 4A in a lateral approach using exemplary embodiments of insertion instruments of the present disclosure.

FIGS. 7A—7E illustrate a method of inserting a fusion-enabling insert into the spine stabilization device of FIG. 6H in a lateral approach using exemplary embodiments of insertion instruments of the present disclosure.

FIGS. 8A—8C illustrate a method of using a trial to assess the anatomical site for implantation in a ventral approach.

FIGS. 9A—9F illustrate a method of inserting the spine stabilization device of FIG. 4A in a ventral approach using exemplary embodiments of insertion instruments of the present disclosure.

FIGS. 10A and 10B illustrate a method of inserting a fusion-enabling insert into the spine stabilization device of FIG. 9F in a ventral approach using exemplary embodiments of insertion instruments of the present disclosure.

FIGS. 11A—11F illustrate another exemplary embodiment of a spine stabilization device of the present disclosure having a fusion-enabling insert configured for external fixation, in which:

FIGS. 11A—11C show the spine stabilization device secured to the side of the vertebral bodies, wherein FIG. 11A shows a side perspective view, FIG. 11B shows a front perspective view, and FIG. 11C shows an enlarged cutaway view in situ; and

FIGS. 11D—11F show the spine stabilization device secured to the front of the vertebral bodies, wherein FIG. 11D shows a side perspective view, FIG. 11E shows a front perspective view, and FIG. 11F shows an enlarged cutaway view in situ.

FIGS. 12A—12D illustrate still another exemplary embodiment of a spine stabilization device of the present disclosure having a fusion-enabling insert configured for external fixation, in which:

FIGS. 12A and 12B show the spine stabilization device secured to the side of the vertebral bodies, wherein FIG. 12A shows a side perspective view and FIG. 12B shows a front perspective view in situ; and

FIGS. 12C and 12D show the spine stabilization device secured to the front of the vertebral bodies, wherein FIG. 12C shows a front perspective view and FIG. 12D shows a side perspective view in situ.

FIGS. 13A and 13B illustrate yet another exemplary embodiment of a spine stabilization device of the present disclosure configured for external fixation, wherein FIG. 13A shows a front perspective view and FIG. 13B shows a side perspective view in situ.

The foregoing and other features of the present disclosure will become apparent to one skilled in the art to which the present disclosure relates upon consideration of the following description of exemplary embodiments with reference to the accompanying drawings.

DETAILED DESCRIPTION OF THE EMBODIMENTS

A modular, customizable system that provides components for assembling an implantable device is provided. The system allows the user to assemble an implantable spine stabilization device that is flexible and allows dynamic stabilization. The same system also provides components for assembling a rigid or non-flexible fusion-enabling spine stabilization device. The components of the system are easily interchangeable, allowing the user the ability to customize the assembled device for a true fit with the patient, as well as allow an easy conversion of the dynamic device into a fusion-enabling device, if so desired. For instance, implantable spine stabilization devices that can be compressed for ease of insertion, and structurally strong enough to dynamically stabilize the spine are desirable. The present system provides a compressible spine stabilization device that is easy to insert and use to dynamically stabilize the region of the spine for some duration of time. Then, when it is desired or necessary to fuse the same region, that dynamic device may be easily converted into a rigid or non-flexible fusion-enabling device. In other cases, the user may simply elect to assemble a dynamic or a fusion device initially, and select those components from the system to achieve that goal. The devices may be configured for use in the lumbar, thoracic, or cervical region of the spine. Methods for implantation and use are also disclosed, along with associated insertion instruments and tools.

FIG. 1 illustrates an exemplary spine and an intervertebral space that can receive the spine stabilization device of the present disclosure. As shown, the space may be located in the lumbar region of the spine. However, it is understood that the spine stabilization device of the present disclosure may be sized and configured for insertion in the thoracic or cervical region, if so desired.

The spine stabilization devices provided herein are configured to be inserted between the vertebrae of a spine. The devices may be used either with or without additional fixation elements, such as for example, screws, nuts, bolts, fasteners, glue, etc. In order to be able to stabilize the intervertebral space, the devices are customizable and configured to closely match the morphology of the intervertebral space. In developing the interchangeable components of the device, certain physical

parameters that were evaluated included: A—P diameter, wedge angle, disc height, apex height, apex diameter, and apex position, etc. These parameters provided a basis to model the morphological profile of the physical implantation site, particularly the endplate morphology, and thus to also model the overall geometry of the spine stabilization devices of the present disclosure. FIG. 2 shows an exemplary morphological profile created using the data listed above.

Accordingly, the present disclosure provides spine stabilization devices that are customizable and configured to closely match the morphology of the implantation site, particularly the endplates, such that the devices can be securely positioned in the intervertebral space, either with or without the use fixation elements. The system of the present disclosure provides the user with the ability to assemble anterior stand-alone devices that can act as either a dynamic cage or a fusion cage.

The system provides interchangeable components to create spine stabilization devices with any number of footprint sizes, with any number of lordotic angles and heights, to provide a combination of geometries that are morphologically suitable for the implantation site. For example, in one exemplary embodiment the spine stabilization device may have a footprint size of about 30 mm by about 39 mm. In another exemplary embodiment, the footprint size may be about 27 mm by about 35 mm. Generally speaking, the footprint may be in the range of about 20 mm by about 50 mm, depending on the region of the spine to be treated, and the size of the patient. Likewise, the system may provide devices with various lordotic angles, including but not limited to 0 degrees, 3 degrees, and 7 degrees. Of course, it is understood that other angles may also be provided, and fractions thereof, such as for example, 2.75 degrees or 8.24 degrees. Generally speaking, the lordotic angle may be in the range of 0 to about 12 degrees. Additionally, the devices may be provided with any number of different heights. Some exemplary heights may include: about 8, about 10, and about 12 mm. Generally speaking, the devices may have heights ranging from about 3 mm to about 18 mm. It is understood, of course, that the dimensions provided herein are merely exemplary and not to be limiting. These specific examples are intended to show the many different ways the devices may be assembled to provide numerous configurations for the final geometry of the device.

As mentioned, the system provides spine stabilization devices that are able to be compressed for easy insertion. To assemble, or later convert the spine stabilization devices to, fusion-enabling implants, the devices may be easily blocked using an insert such that no compression is possible. Additionally, these devices may be able to distract for sagittal adjustment in the case of fusion. The system provides these blocking inserts in a variety of heights, thereby allowing the user to effectively customize the height of the implantable device by the use of differently sized blocking inserts. In other words, putting in different sized inserts alters the curvature of the device as well as alters the angle between different implant sizes. For example, it is possible to go from 5 degrees to 7 degrees with the use of a larger blocking insert. Accordingly by this manner, the spine stabilization devices of the present disclosure are considered to provide standalone devices that allow 360 degrees of stabilization, i.e., without the need for a posterior stabilization component.

Turning now to the drawings and particularly to FIGS. 3A—3G, an exemplary embodiment of a modular, customizable system 10 is shown. The system allows a dynamic spine stabilization device 20 to be assembled. This device may comprise a main body 22 having a superior plate 24 and inferior plate 26 connected by a sidewall 28 for compressibility. The superior plate 24 may include an opening 32 for receiving a domed cap 40, as shown in FIG. 3A. The domed cap 40 may comprise a domed upper surface 42 and a stem 46 that is configured to lock into the opening 32 on the superior plate 24. The domed upper surface 42 may comprise ridges, cutout portions, teeth, or other surface features 36. These surface features may also be provided on the superior and inferior plates of the main body as well.

FIG. 3B shows a top planar view of the spine stabilization device of FIG. 3A. As shown in FIGS. 3C and 3D, the domed cap 40 is not symmetrical, and thus can be snapped onto the main body 22 in different directions. This eccentric domed cap allows for variations the direction of the cap, and hence the curvature of the superior plate. For example, as shown in FIGS. 3C and 3D, the domed cap may be positioned in inapposite directions relative to the main body 22 of the spine stabilization device. This gives the user the ability to adjust the curvature of the device to closely match the patient's anatomy. In other words, the user may adapt morphologically by

adjusting the position of the domed cap. As shown, the domed cap 40 may be eccentric. However, in other embodiments the domed cap 40 may be centric.

FIG. 3E shows a cutaway view of the domed cap 40 attached to the body of the spine stabilization device 20, which shows the close fit between the cap and the superior plate of the main body. It is intended that the domed cap 40 be configured to easily snap onto the superior plate 24 such that the surgeon may be able to perform this task very quick prior to implantation. The domed cap 40 may comprise a stem 46 which comprises a plurality of movable fingers, thus allowing the stem to be snapped onto the superior plate. However, other mechanisms for attaching the domed cap to the plate may be utilized, such as by threads, dovetail connection, press-fit, etc.

FIG. 3F shows a side view of the spine stabilization device of FIG. 3E. As can be seen, within the main body, tool-engaging openings 38 are provided on the superior plate 24 to allow the user a way to manipulate the main body and control the manner of compression. These tool-engaging openings may be provided on an undermounted bracket or panel 34 that extends from the underside of the superior plate 24.

FIG. 3G shows a bottom perspective view of the spine stabilization device of FIG. 3G. The inferior plate 26 may also include an opening within which resides a bottom cap 50. This bottom 50 cap may also contain an opening, as shown. This bottom cap 50 may be configured with a curved, round, or chamfered edge so that the inferior plate closely matches the lower endplate of the intervertebral space. Like the other domed cap 40, this domed cap 50 may be eccentric or centric.

FIGS. 4A—4D illustrate an exemplary embodiment of another spine stabilization system that provides an implantable device similar to the one previously described for FIGS. 3A—3G, except that the domed cap may be provided without surface features. These surface features are optional, of course, and if so desired, could be included with the domed cap 40 of the present disclosure. In addition, as shown in FIG. 4A the system may include a fusion-enabling insert 60 that, when inserted into the main body 22, acts as a pillar to block or prevent compression.

The inferior plate 26 may also include an opening within which resides a bottom cap 50, as previously described. This bottom cap 50 may be configured with a curved, round, or chamfered edge so that the inferior plate closely matches the lower endplate of the intervertebral space. Like the other domed cap 40, this domed cap 50 may be eccentric or centric. In addition, this domed cap 50 for the inferior plate may optionally include a through-hole that can also be filled with bone graft material, bone cement, bone substitute material, bone hardening material, bone void filler, demineralized bone matrix, or other similar materials.

The domed caps 40, 50 may also comprise a bioactive coating for promoting fusion to anchor to bone tissue. This coating could contain a biological agent such as bone morphogenic protein (BMP), a peptide, a bone growth factor such as platelet derived growth factor (PDGF), stem cells, bone marrow, and platelet rich plasma (PRP), to name a few examples.

FIG. 4B illustrates a partial cutaway view of the spine stabilization device of FIG. 4A, showing the close fit between the insert 60 and the main body 22 when placed between the superior 24 and inferior 26 plates. This close fit is also seen in FIG. 4C which illustrates a side view of the spine stabilization device of FIG. 4A. As FIG. 4D illustrates, a front view of the spine stabilization device of FIG. 4A shows that the insert 60 can be inserted so as to reside entirely inside the main body itself and does not extend out of the main body 22.

FIGS. 5A—5C illustrate a method of using a trial 120 to determine the morphological profile of the intervertebral space, and assess the anatomical site for implantation in a lateral approach. As shown in FIG. 5A, a trial 120 similar to the spine stabilization device of FIGS. 3A and 4A is attached to an inserter tool. Trial 120 shares similar structural features as spine stabilization device 20, with the same features having the same reference number following the prefix “1”.

As FIG. 5B shows, the inserter tool 110 may comprise a stationary arm 112 and a movable arm 114 that engage the tool-engaging openings 138 of the trial 120. The insertion tool 110 may be configured so that the movable arm 114 is operable from the handle end such that the user can control the movement of the arm as indicated by the arrows. FIG. 5C shows a different angular view as the movable arm

114 is raised thereby causing the superior plate 124 to be lifted or extended up. The trial 120 and these steps allow the user to assess the morphological profile of the intervertebral space, examine the form-fit of the domed cap to be used on the spine stabilization device, footprint size and angulation. Any adjustments can then be made prior to implantation.

FIGS. 6A—6H illustrate a method of inserting the spine stabilization device 20 of FIG. 4A in a lateral approach. After trialing, the trial 120 may be removed from the insertion tool 110 and replaced with the actual spine stabilization device 20, complete with the domed cap 40 of choice, as shown in FIG. 6A. As the partial cutaway view of FIG. 6B and the side perspective view of FIG. 6C shows, the stationary arm 112 may extend in the hinged portion of the main body 22, while the movable arm 114 extends through the tool-engaging opening 38 in the undermounted panel 34 of the superior plate 24.

FIG. 6B shows the device 20 in a neutral position. To compress the main body 22 for insertion, the movable arm 114 may be lowered in the direction of the arrows as shown in FIGS. 6C and 6D. For example, the main body 22 may be compressed in a range from approximately 2 to 12 degrees, without limitation, such as 5 to 6 degrees, for insertion of the spine stabilization device 20.

If distraction is desired, such as for lordotic alignment, the movable arm 114 would be raised upward in the direction of the arrows as shown in FIGS. 6E and 6F. Such movement would cause the superior plate 24 to be raised or distracted. For example, the angle of distraction may lie in a range from approximately 2 to 12 degrees, without limitation, such as approximately 3 to 5 degrees. Of course, these ranges are merely exemplary and are not intended to be limiting.

FIG. 6G shows the spine stabilization device 20 fully implanted within the intervertebral space 6 and seated securely between the intervertebral bodies 2. As illustrated, the spine stabilization device 20 is intended to be inserted entirely within the space 6, does not extend beyond the borders of the vertebral bodies 2 and does not require additional external fixation elements. In this mode, the spine stabilization device 20 serves as a stand-alone dynamic stabilization device. In the present example, the device is used in the lumbar spine. However, it is contemplated that the

devices of the present disclosure may be configured and sized to be used in the thoracic and cervical spine if so desired.

To convert the dynamic stabilization device into a fusion-enabling device, a blocking insert 60 may be placed within the main body 22 to prevent compression. FIGS. 7A—7E illustrate a method of inserting a fusion-enabling insert 60 into a spine stabilization device 20 similar to FIG. 6H in a lateral approach. The fusion-enabling insert 60 may first be attached to an insert delivery instrument 160. The instrument may comprise an operable end 162, a catch and release switch 166, and arms 164 that extend into the tool-engaging holes 66 of the insert 60. As shown in FIG. 7A, the insert may be placed onto the arms of the insert delivery instrument. Once the insert 60 is on the arms 164, the catch and release switch 166 may be activated in the direction of the arrow shown in FIG. 7B. To release the insert, the user would simply need to reactivate the switch 166.

Next, as shown in FIG. 7C, the spine stabilization device 20 for implantation is attached to the inserter tool 110 similar to the process previously described at FIG. 6A. Once the spine stabilization device is properly positioned in the intervertebral space, the handle portion 118 of the inserter tool 110 is removed as indicated by the arrow shown in FIG. 7C. Then, the insert delivery instrument 160 is slid into the inserter tool 110, as shown in FIG. 7D. The insert 60 may be placed within the main body 22, the insert delivery instrument 160 removed, and then the inserter tool 110 removed to leave behind the spine stabilization device 20 in a fusion-enabling mode, as shown in FIG. 7E.

As mentioned, the present device 20 may be inserted in either a lateral or ventral approach. FIGS. 8A—8C illustrate a method of using a trial to determine the morphological profile of the intervertebral space, and assess the anatomical site for implantation in a ventral approach. To insert the devices of the present disclosure by a ventral approach, the process of trialing may again precede the actual implantation steps. As shown in FIGS. 8A—8C, the trial 120 may be used to examine dome form-fit, footprint size and angulation. Once those parameters are defined, the user can then determine what configuration the final device needs to have.

In a ventral approach, another insertion tool may be provided that allows the superior plate to be lifted from the front, as indicated by the arrow in FIG. 8C. The ventral insertion tool may have a single movable arm along with a rest plate with extending pins that are inserted into the inferior plate for stability.

FIGS. 9A—9G illustrate a method of inserting the spine stabilization device 20 of FIG. 4A in a ventral approach. After trialing, the actual spine stabilization device 20, complete with the domed cap 40 of choice, may be attached to the ventral delivery instrument 130 as shown in FIGS 9A—9D. As shown, the stabilizing pins 132 of the ventral delivery instrument 130 may extend in the openings of the inferior plate of the main body, while the movable pins 134 may be positioned to extend through the tool-engaging openings 38 in the undermounted panel 34 of the superior plate.

FIGS. 9A—9C show the device in a neutral position. To compress the main body 22 for insertion, the movable arms 134 may be lowered in the direction of the arrows as shown in FIG. 9D. The main body 22 may be compressed for insertion of the spine stabilization device 20.

If distraction is desired, such as for lordotic alignment, the movable arm would be raised upward in the direction of the arrows as shown in FIGS. 9E and 9F. Such movement would cause the superior plate 24 to be raised or distracted. Thereafter, an insert 60 may be placed in between to adjust the height of the device as well as the angle of the device (lordotic curvature) to achieve sagittal balance. Accordingly, inserts 60 provided by the present disclosure have varying heights and/or angles.

FIGS. 10A and 10B illustrate a method of inserting a fusion-enabling insert into the spine stabilization device of FIG. 9G in a ventral approach. Similar to the method described above, the fusion-enabling insert 60 may be positioned within the main body 22 of the spine stabilization device by sliding an insert 60 along with the insert delivery instrument 160 into the ventral delivery instrument 130 and releasing the insert 60 into the main body of the device 20.

The devices are configured to be stand-alone devices. However, it is also possible to utilize these devices with a posterior fixation device or system for total 360 degree stabilization. Suitable posterior fixation devices may include interspinous stabilization devices such as the one described in U.S. Patent Nos. 5,645,599 and 7,922,750, to name a few examples.

In some embodiments, the devices may be configured for use with fixation screws. For instance, the compression-blocking insert may be configured for attachment to the vertebral bodies with fixation screws. In one embodiment, the inserts may comprise an attachment plate for receiving the fixation screws. In another embodiment, the fixation screws may be attached to the main body.

Turning now to the drawings, FIGS. 11A—11F illustrate another exemplary embodiment of a spine stabilization device of the present disclosure having a fusion-enabling insert configured for external fixation. As shown in FIGS. 11A—11C, the spine stabilization device 20 can be secured to the side of the vertebral bodies 2 with fixation screws 80. In the present embodiment, the insert 60 may extend into a screw holding block 70 that is configured to reside outside of the vertebral bodies 2. The screw holding block 70 would include screw holes for receiving the screws 80. The device 20 may be secured to the sides of the vertebral bodies 2, as shown.

FIGS. 11D—11F show the same spine stabilization device 20 as above, but secured to the front of the vertebral bodies 2. By rotating the insert 60 90 degrees such that the screw holding block 70 extends toward the front of the spine, the entire construct may be secured using the same screws 80 to the front of the vertebral bodies 2, as shown.

FIGS. 12A—12D illustrate still another exemplary embodiment of a spine stabilization device 20 of the present disclosure having a fusion-enabling insert configured for external fixation. FIGS. 12A and 12B show the spine stabilization device 20 secured to the side of the vertebral bodies 2. In the present embodiment, the insert 60 extends into an attachment plate 90 that resides outside the bodies 2, as shown. The entire construct may be secured with fixation elements like bone screw 80, through the attachment plate 90, and to the vertebral bodies 2.

The insert 60 of FIGS. 12A and 12B may be rotated about 90 degrees to allow the device 20 to be secured to the front of the vertebral bodies 2, as shown in FIGS. 12C and 12D. show the spine stabilization device secured to the front of the vertebral bodies.

FIGS. 13A and 13B illustrate yet another exemplary embodiment of a spine stabilization device of the present disclosure configured for external fixation. In the present embodiment, the device 20 may simply be provided with screw holes to allow insertion of fixation elements or bone screw 80. Thus, in some cases, the device 20 may be directly secured to the endplates of the vertebral bodies 2, as shown, by inserting screws 80 through the device into the vertebral bodies 2 above and below the device 20.

The description of the invention is provided to enable any person skilled in the art to practice the various embodiments described herein. While the present invention has been particularly described with reference to the various figures and embodiments, it should be understood that these are for illustration purposes only and should not be taken as limiting the scope of the invention.

There may be many other ways to implement the invention. Various functions and elements described herein may be partitioned differently from those shown without departing from the spirit and scope of the invention. Various modifications to these embodiments will be readily apparent to those skilled in the art, and generic principles defined herein may be applied to other embodiments. Thus, many changes and modifications may be made to the invention, by one having ordinary skill in the art, without departing from the spirit and scope of the invention.

A reference to an element in the singular is not intended to mean “one and only one” unless specifically stated, but rather “one or more.” The term “some” refers to one or more. Underlined and/or italicized headings and subheadings are used for convenience only, do not limit the invention, and are not referred to in connection with the interpretation of the description of the invention. All structural and functional equivalents to the elements of the various embodiments of the invention described throughout this disclosure that are known or later come to be known to those of ordinary skill in the art are expressly incorporated herein by

reference and intended to be encompassed by the invention. Moreover, nothing disclosed herein is intended to be dedicated to the public regardless of whether such disclosure is explicitly recited in the above description.

Other embodiments of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the disclosure provided herein. It is intended that the specification and examples be considered as exemplary only, with a true scope and spirit of the disclosure being indicated by the following claims.

What is claimed is:

1. An implantable spine stabilization device comprising:

a main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates, the superior plate having an opening extending therethrough for receiving a domed cap, the domed cap comprising a domed top and a stem configured for insertion into the opening on the superior plate;

wherein the main body is compressible and distractable.
2. The device of claim 1, wherein the main body includes surface features for anchorage to bone tissue.
3. The device of claim 2, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.
4. The device of claim 1, wherein the domed cap comprises surface features for anchorage to bone tissue.
5. The device of claim 4, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.
6. The device of claim 1, wherein the superior plate has a panel extending from an underside thereof, the panel including at least one tool-engaging opening.
7. The device of claim 1, wherein the domed cap may be eccentric or centric, and is attachable to the superior plate in different orientations.
8. The device of claim 1, further including a cap attached to the inferior plate.
9. The device of claim 1, wherein the domed cap comprises a bioactive coating for promoting fusion to anchor to bone tissue.
10. An implantable spine stabilization device comprising:

a compressible and distractable main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates, the superior plate having an opening extending therethrough for receiving a domed cap, the domed cap comprising a domed top and a stem configured for insertion into the opening on the superior plate, the domed top including a through-hole; and

a compression-blocking insert configured for placement in between the superior and inferior plates, the insert being sized to fit entirely within the main body.

11. The device of claim 10, wherein the opening of the superior plate and through-hole of the domed cap align to create a receiving channel when the domed cap is attached to the superior plate.

12. The device of claim 11, further including bone graft material, bone cement, bone void filler, bone substitute material, bone hardening material, bone chips, or demineralized bone matrix for insertion into the bone graft receiving channel.

13. The device of claim 10, wherein the main body includes surface features for anchorage to bone tissue.

14. The device of claim 13, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.

15. The device of claim 10, wherein the domed cap comprises surface features for anchorage to bone tissue.

16. The device of claim 15, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.

17. The device of claim 10, wherein the superior plate has a panel extending from an underside thereof, the panel including at least one tool-engaging opening.

18. The device of claim 17, wherein the panel further includes a cutaway slot for allowing passage of the compression-blocking insert into the main body.

19. The device of claim 10, wherein the domed cap may be eccentric or centric, and is attachable to the superior plate in different orientations.

20. The device of claim 10, further including a cap attached to the inferior plate.

21. The device of claim 10, wherein the domed cap comprises a bioactive coating for promoting fusion to anchor to bone tissue.

22. The device of claim 10, wherein the insert comprises an attachment plate for securing the device to vertebral bodies.

23. The device of claim 10, further comprising screw holes for receiving fixation screws.

24. A modular spine stabilization system comprising:

a plurality of compressible and distractable main bodies, each main body having a superior plate, inferior plate, and a flexible sidewall connecting the superior and inferior plates;

a plurality of eccentric domed caps, each domed cap comprising a domed top and a stem configured for insertion into an opening on the superior plate; and

a plurality of compression-blocking inserts, each insert being configured for placement in between the superior and inferior plates, the insert being sized to fit entirely within the main body.

25. The system of claim 24, wherein the plurality of main bodies have different heights, angles or footprints.

26. The system of claim 24, wherein the plurality of eccentric domed caps have different curvatures, sizes or angles.

27. The system of claim 24, wherein the plurality of compression-blocking inserts have different heights.

28. The system of claim 24, wherein the domed top includes a through-hole and the compression-blocking insert includes a central opening.

29. The system of claim 28, wherein the opening of the superior plate, central opening of the compression-blocking insert, and through-hole of the domed cap align to create a receiving channel when the domed cap is attached to the superior plate.

30. The device of claim 29, further including bone graft material, bone cement, bone void filler, bone substitute material, bone hardening material, bone chips, or demineralized bone matrix for insertion into the bone graft receiving channel.

31. The device of claim 24, wherein the main body includes surface features for anchorage to bone tissue.

32. The device of claim 31, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.

33. The device of claim 24, wherein the domed cap comprises surface features for anchorage to bone tissue.

34. The device of claim 33, wherein the surface features comprise teeth, ridges, spikes, or roughened surfaces.

35. The device of claim 24, wherein the superior plate has a panel extending from an underside thereof, the panel including at least one tool-engaging opening.

36. The device of claim 35, wherein the panel further includes a cutaway slot for allowing passage of the compression-blocking insert into the main body.

37. The device of claim 24, wherein the domed cap may be eccentric or centric, and is attachable to the superior plate in different orientations.

38. The device of claim 24, further including a cap attached to the inferior plate.

39. The device of claim 24, wherein the domed cap comprises a bioactive coating for promoting fusion to anchor to bone tissue.

40. The device of claim 24, wherein the insert comprises an attachment plate for securing the device to vertebral bodies.

41. The device of claim 24, further comprising screw holes for receiving fixation screws.

42. The device of claim 24, wherein the compression-blocking insert has a height greater than the device, and insertion of the insert distracts the device.

43. The device of claim 24, wherein the compression-blocking insert is angled, and insertion of the insert adjusts the lordotic curvature of the device.

44. The device of claim 24, further comprising screw holes for receiving fixation screws, and further securing the device to the vertebral bodies with fixation screws.

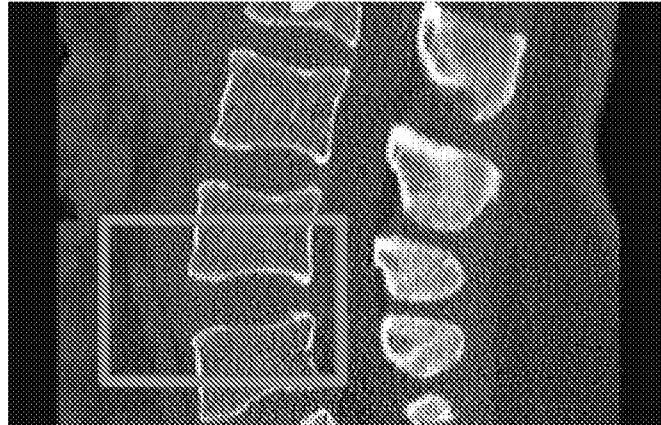


FIG. 1

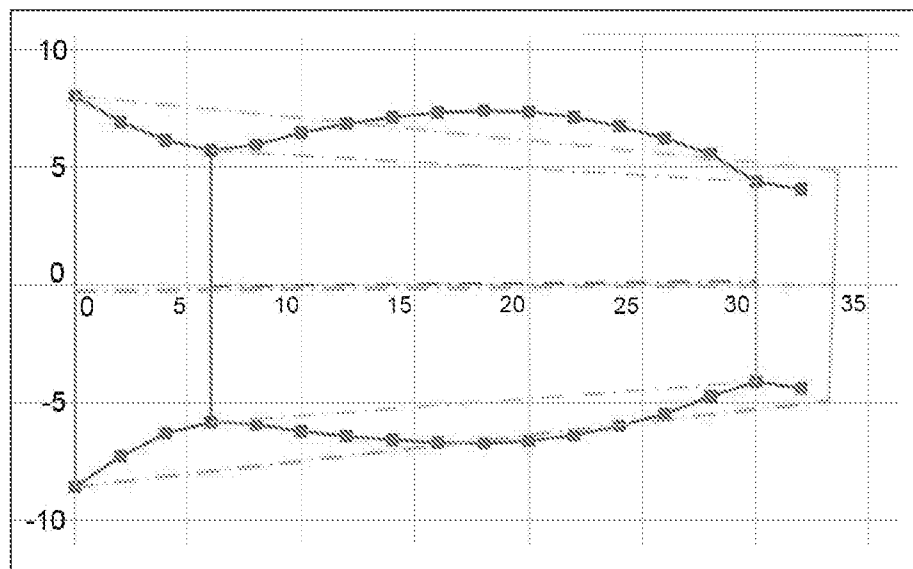
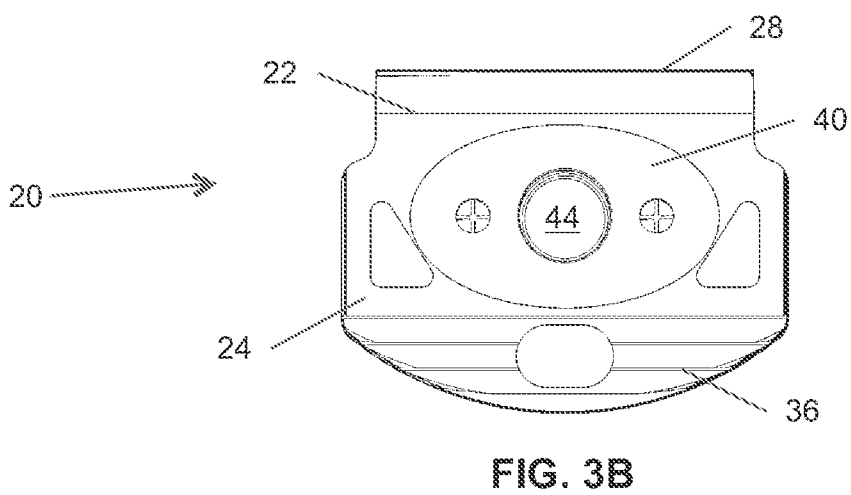
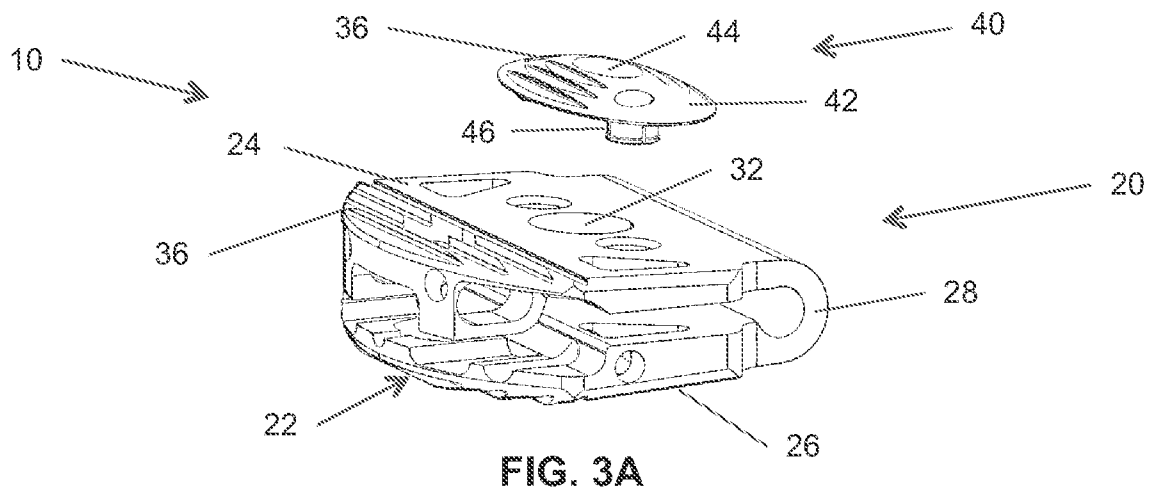
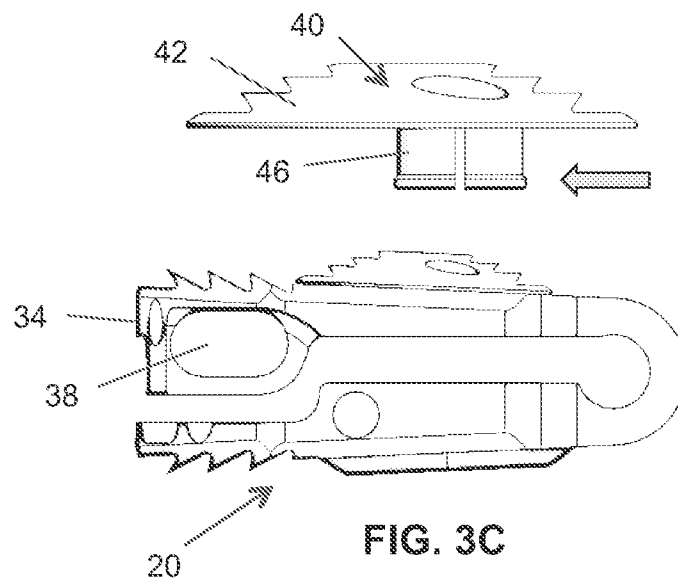
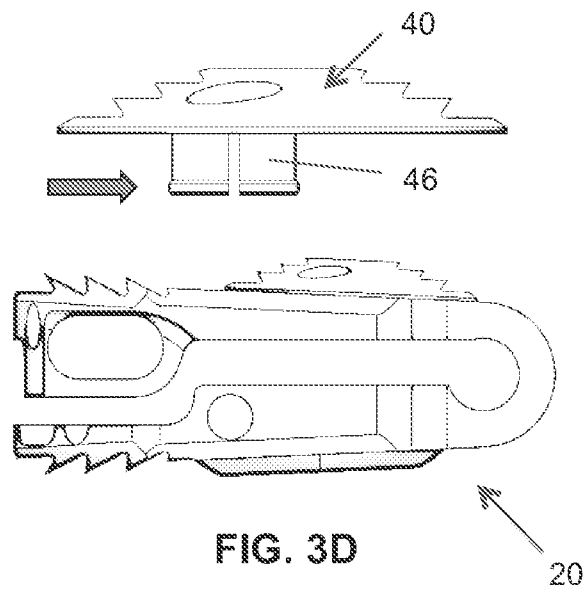


FIG. 2





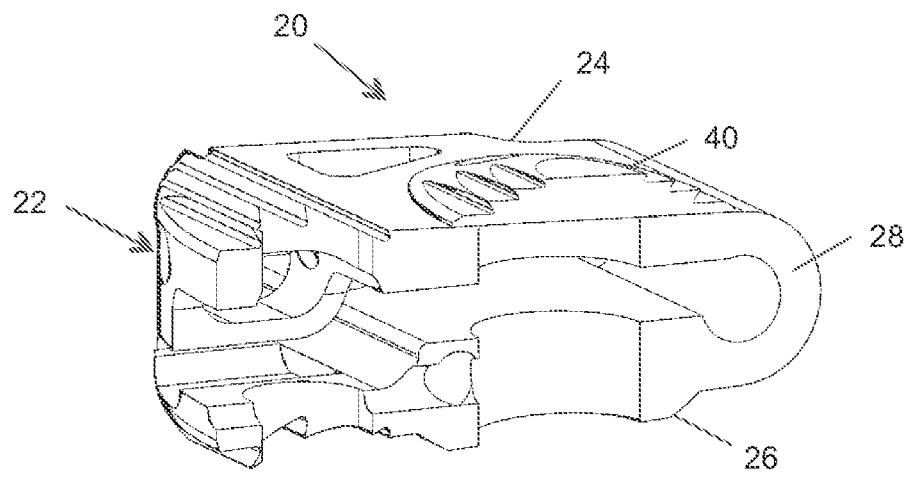


FIG. 3E

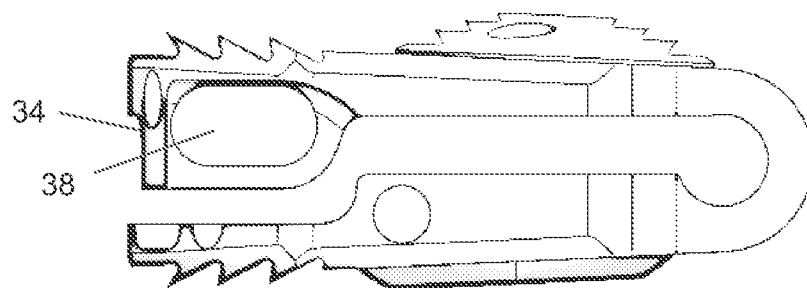


FIG. 3F

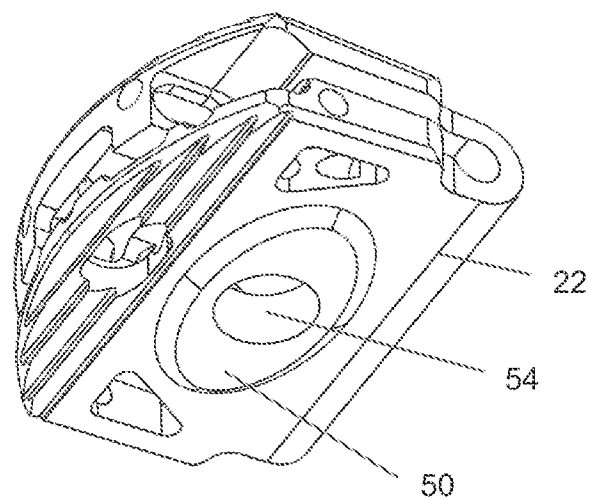


FIG. 3G

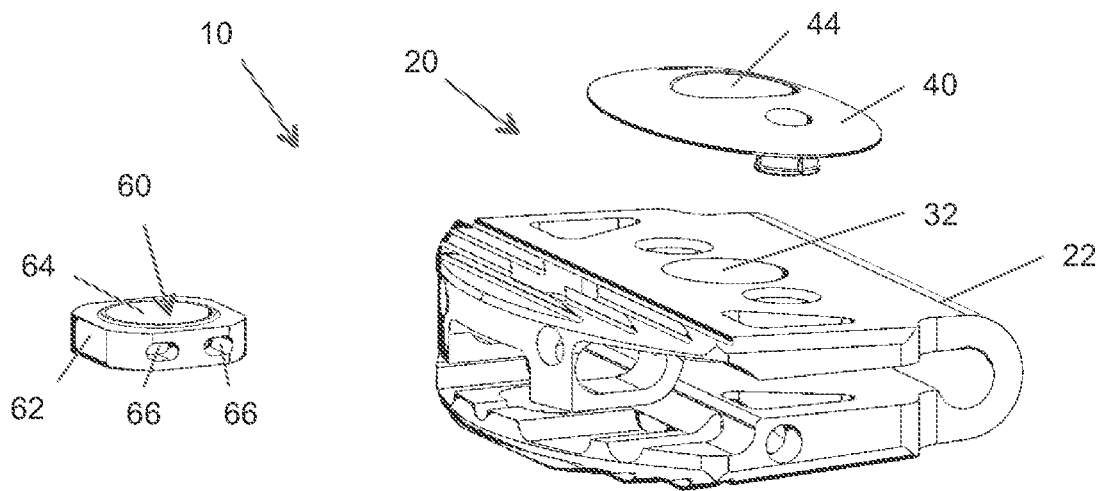


FIG. 4A

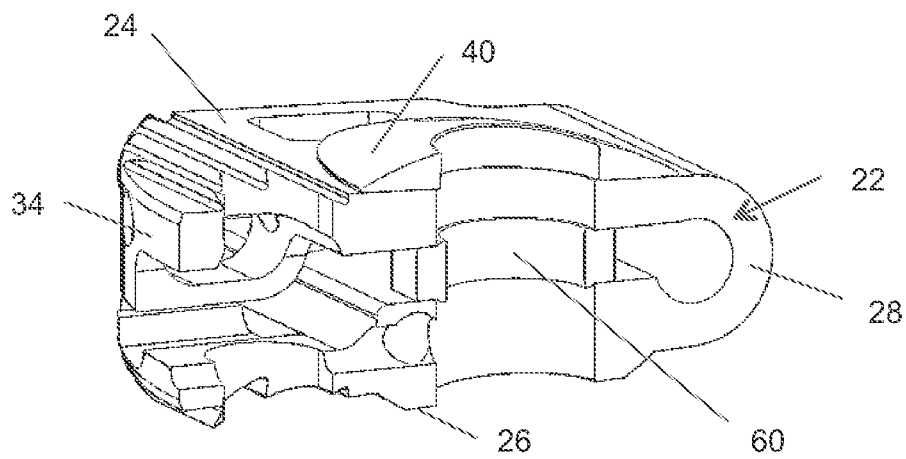
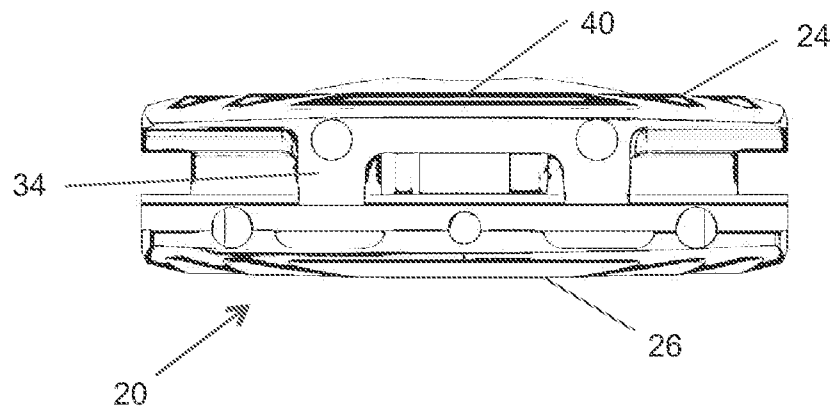
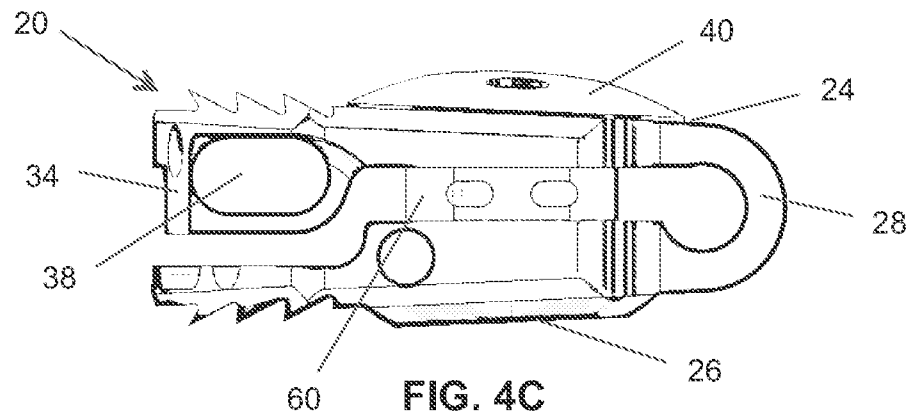


FIG. 4B



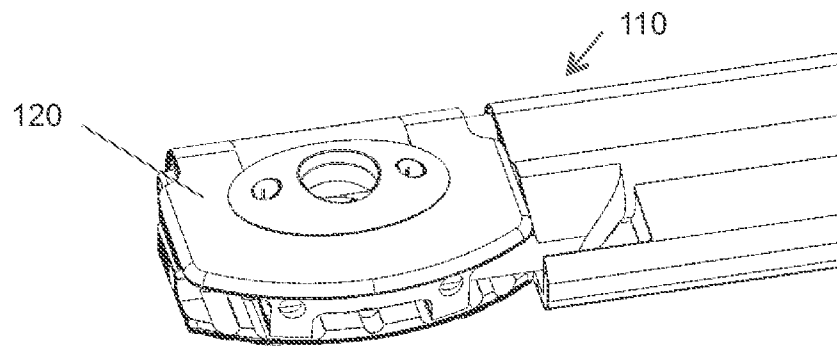


FIG. 5A

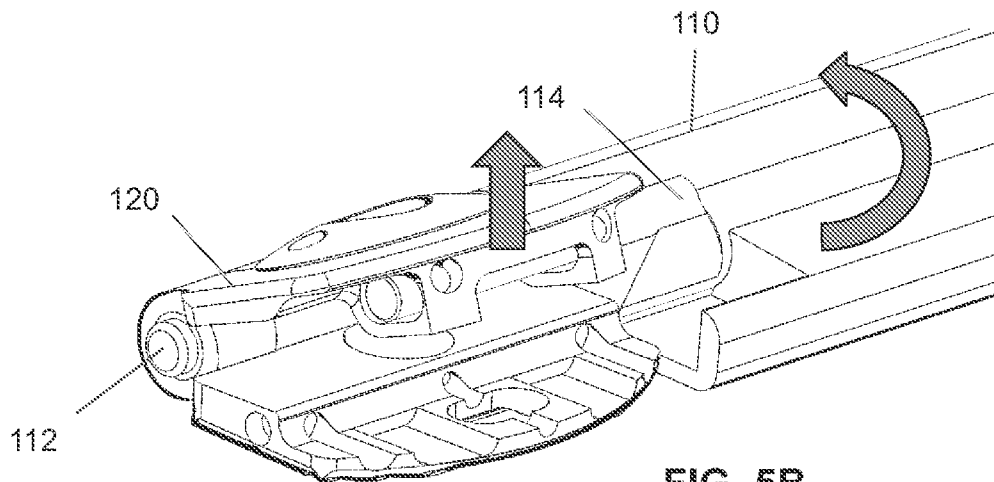


FIG. 5B

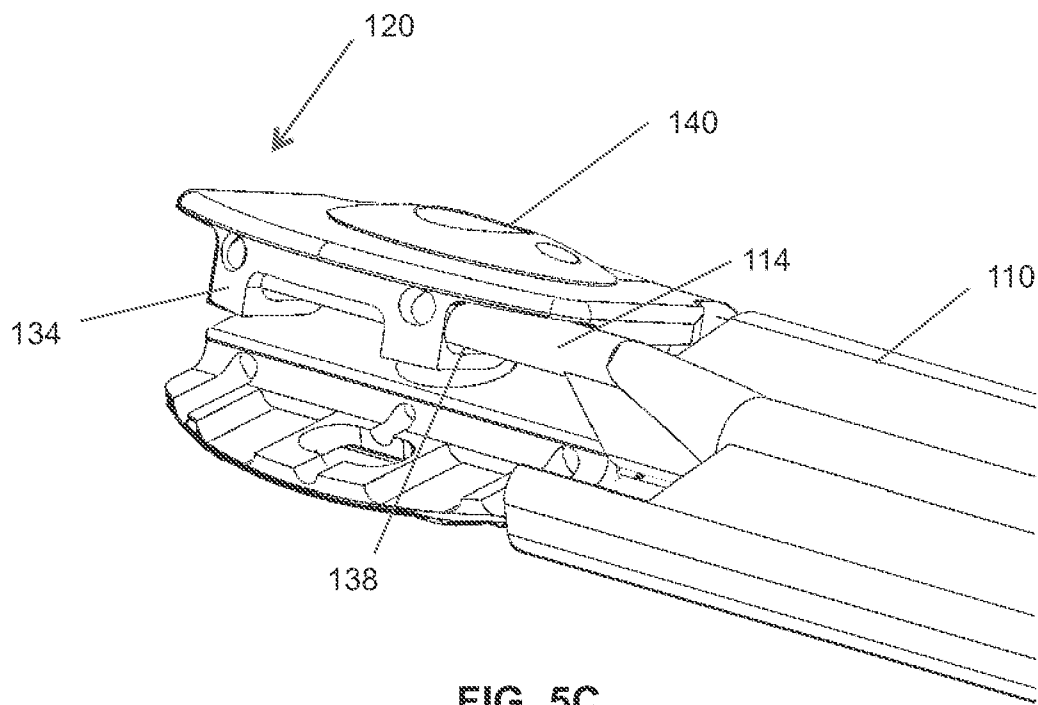


FIG. 5C

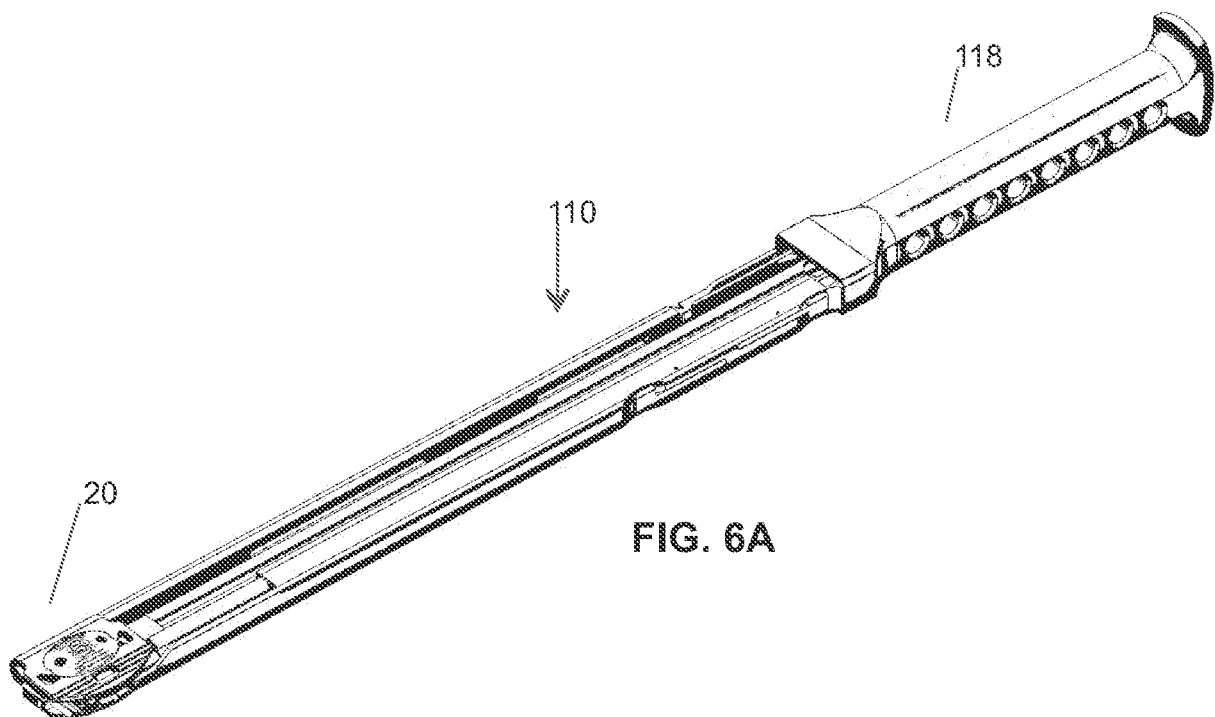


FIG. 6A

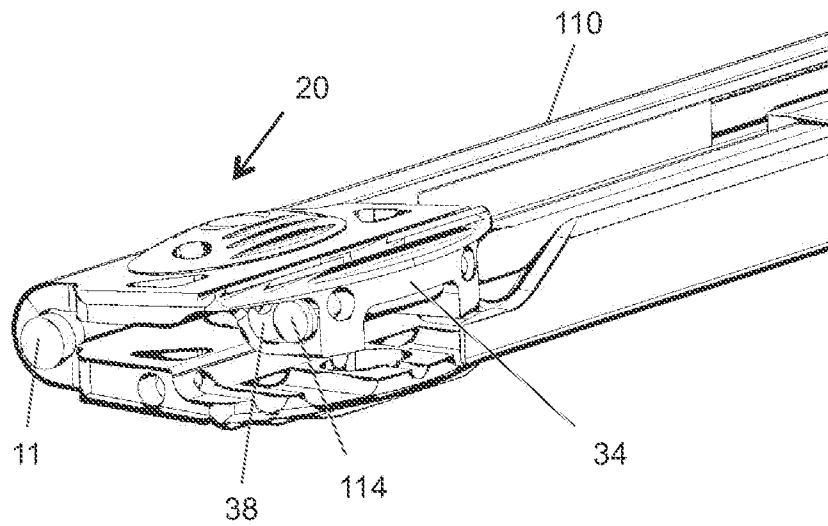


FIG. 6B

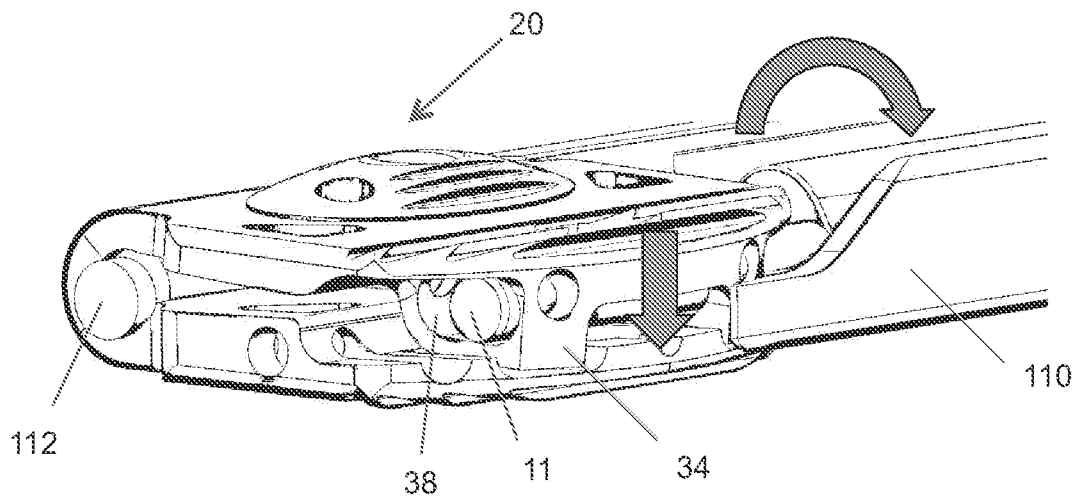


FIG. 6C

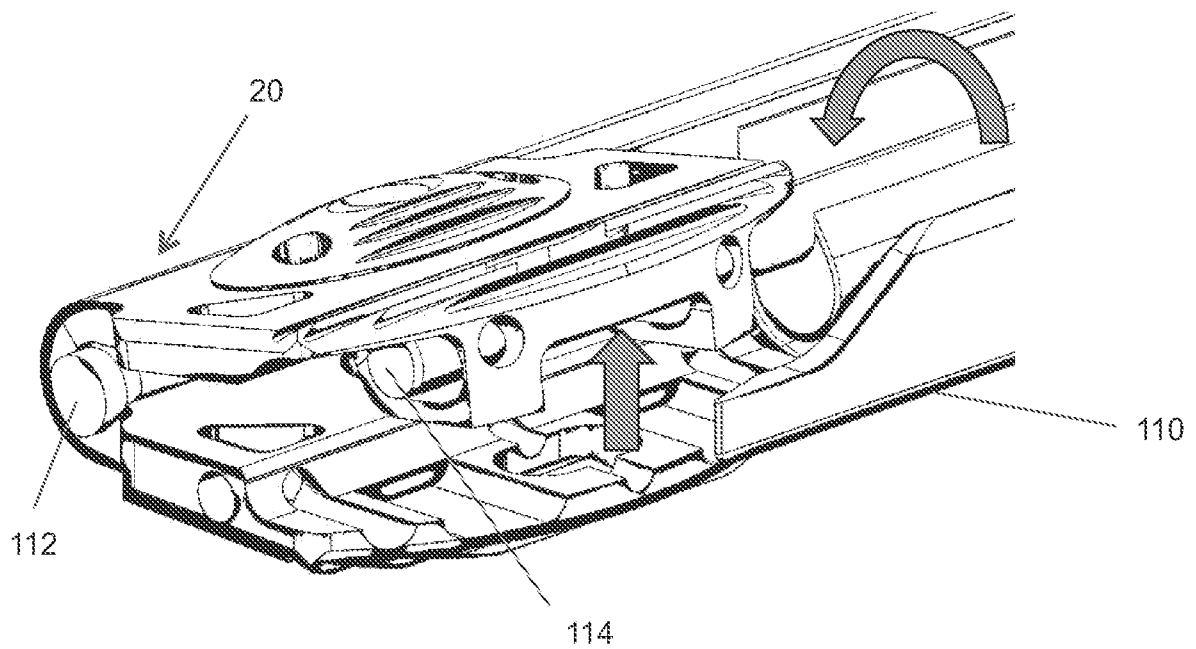
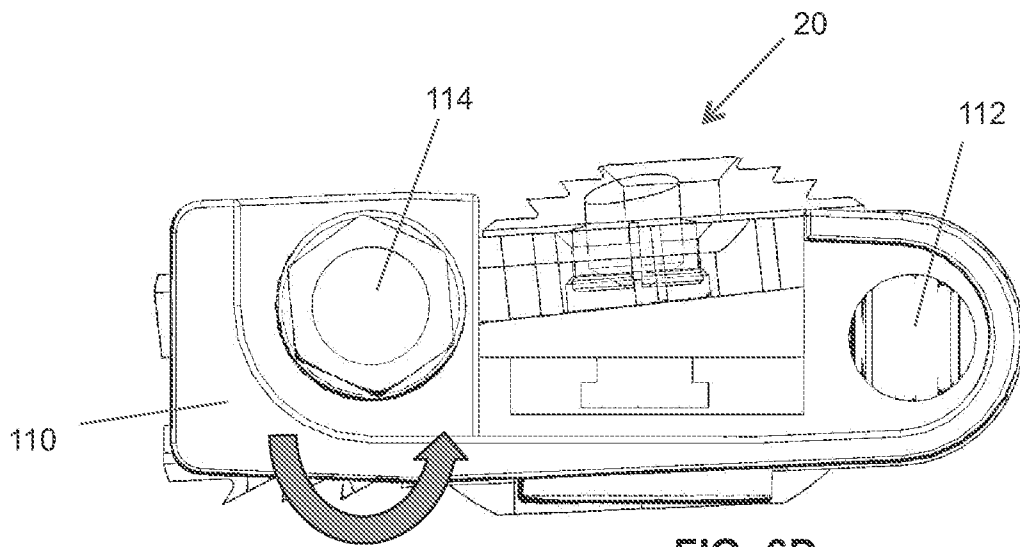
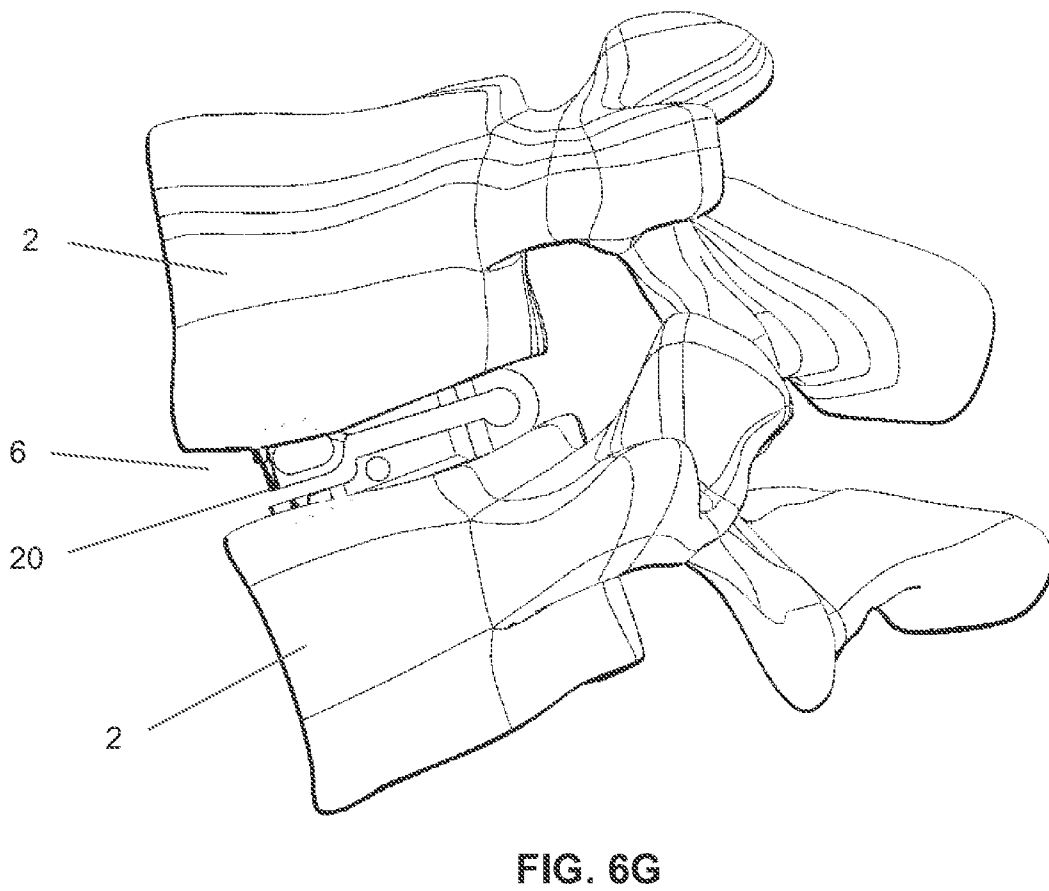
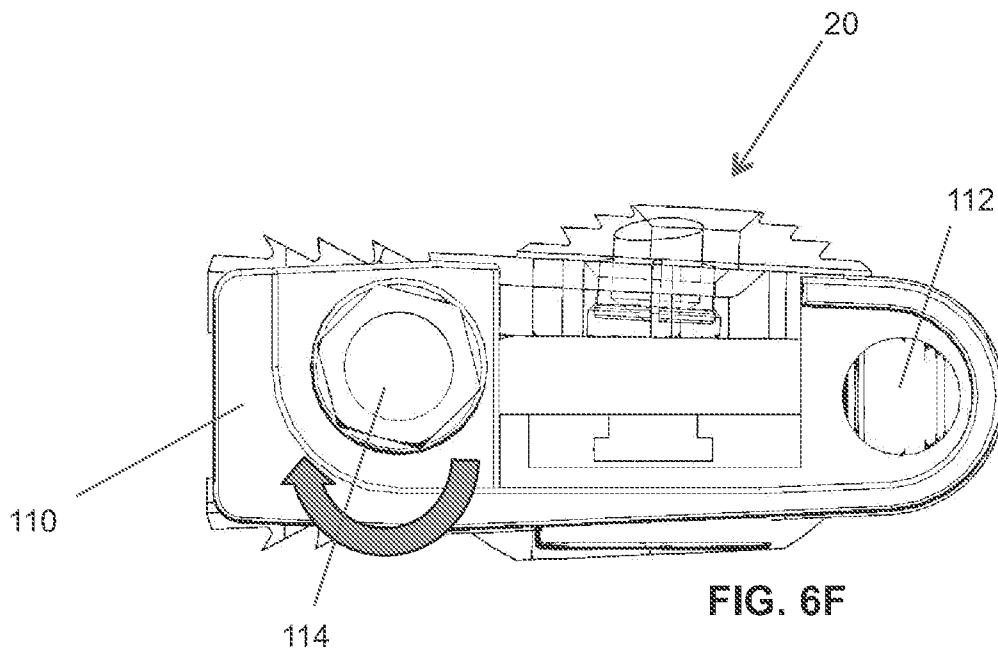
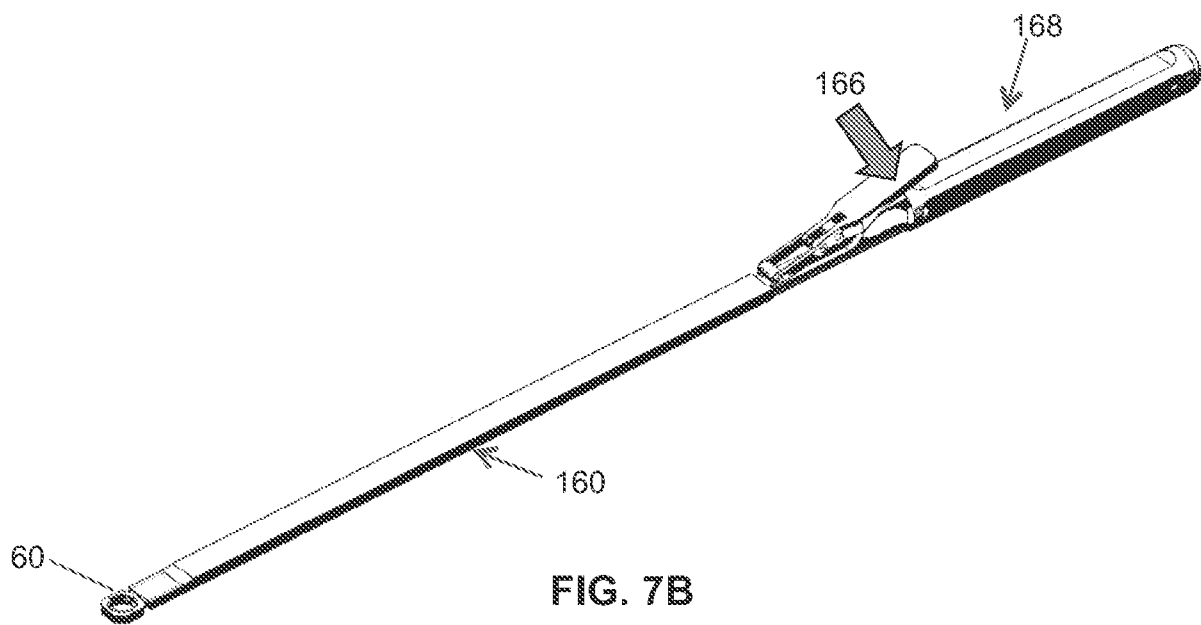
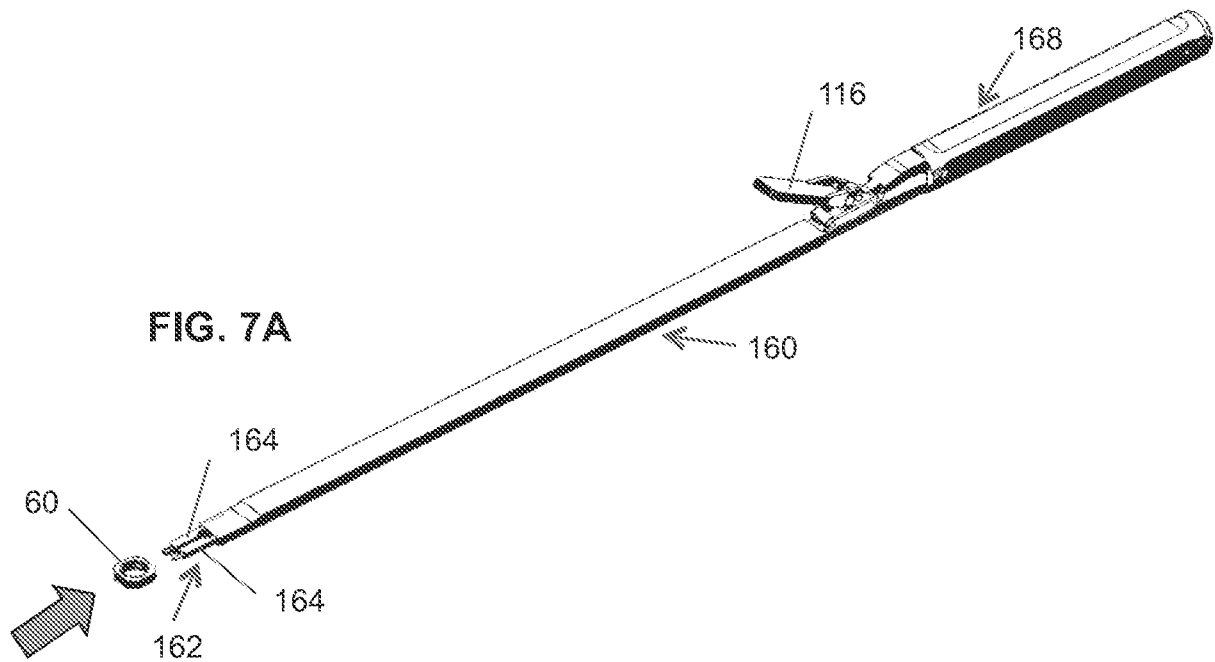


FIG. 6E





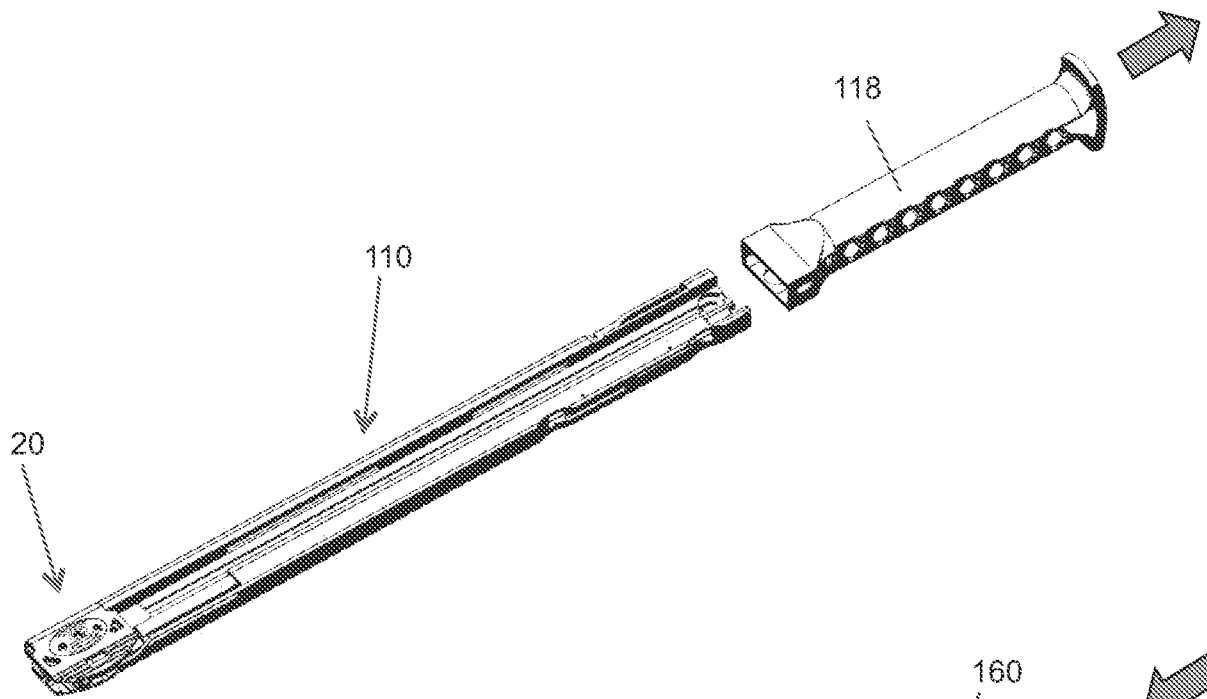


FIG. 7C

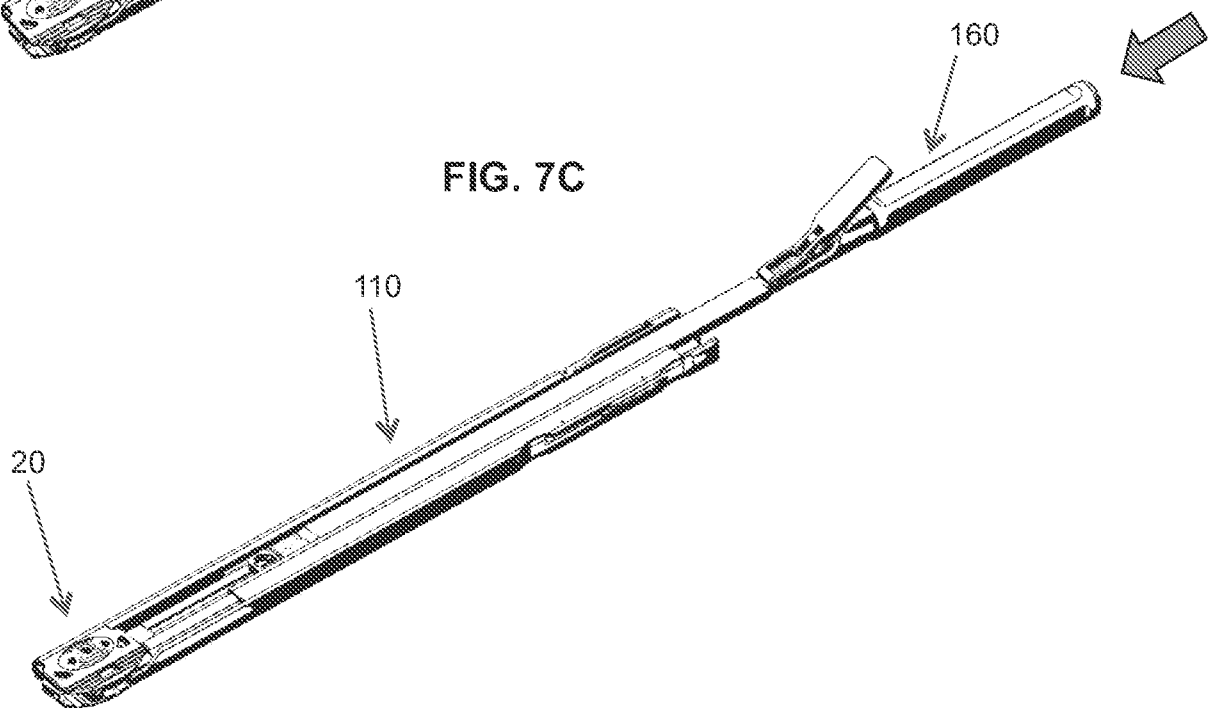


FIG. 7D

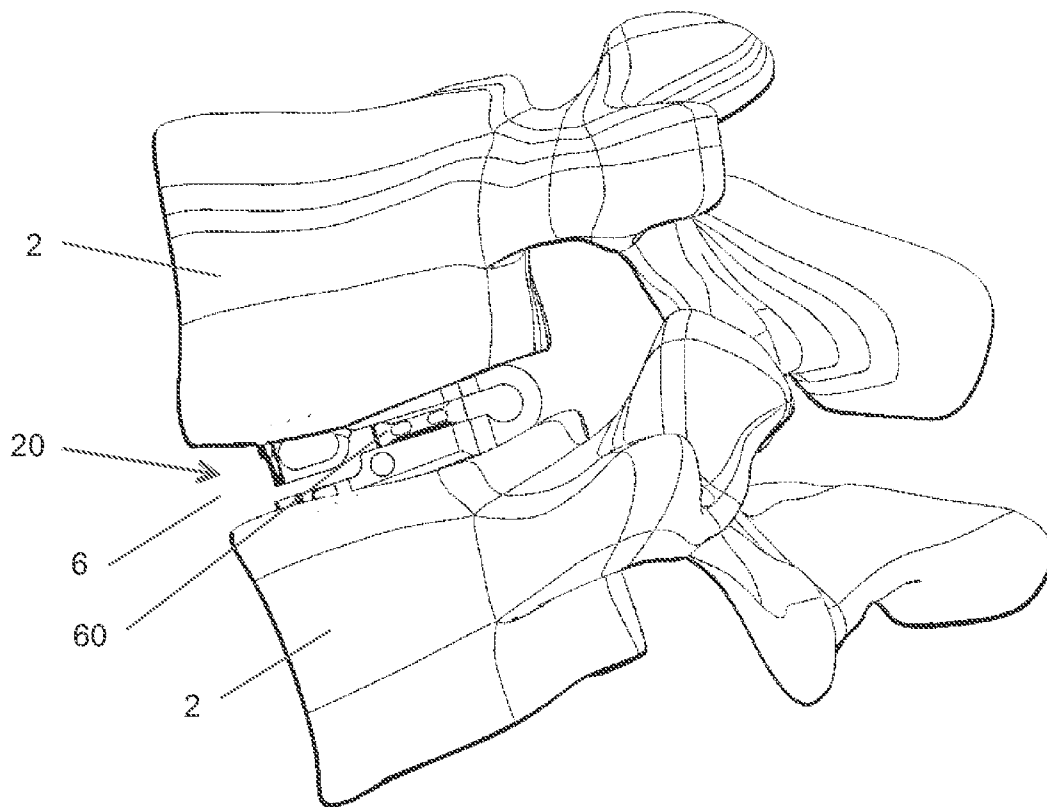


FIG. 7E

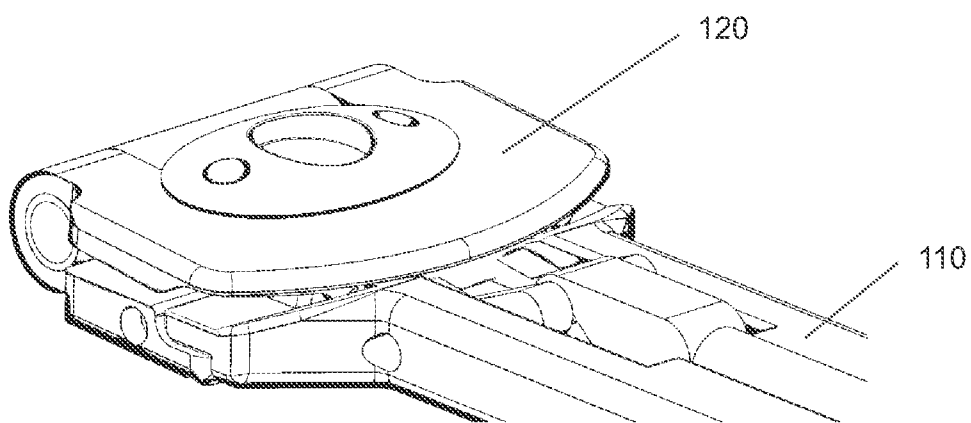


FIG. 8A

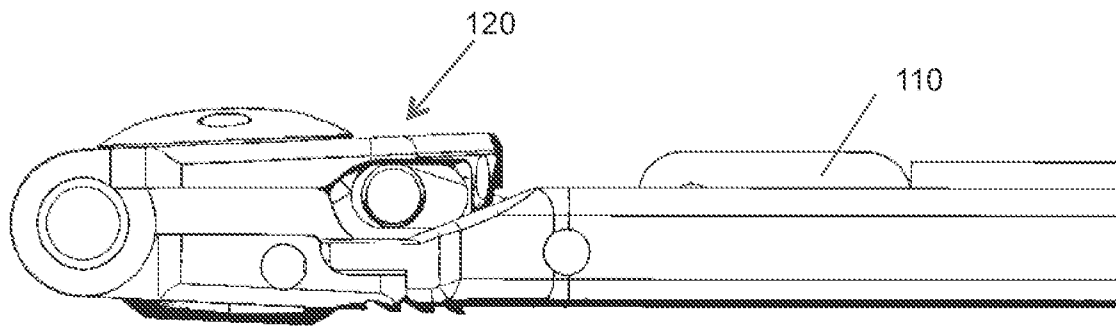


FIG. 8B

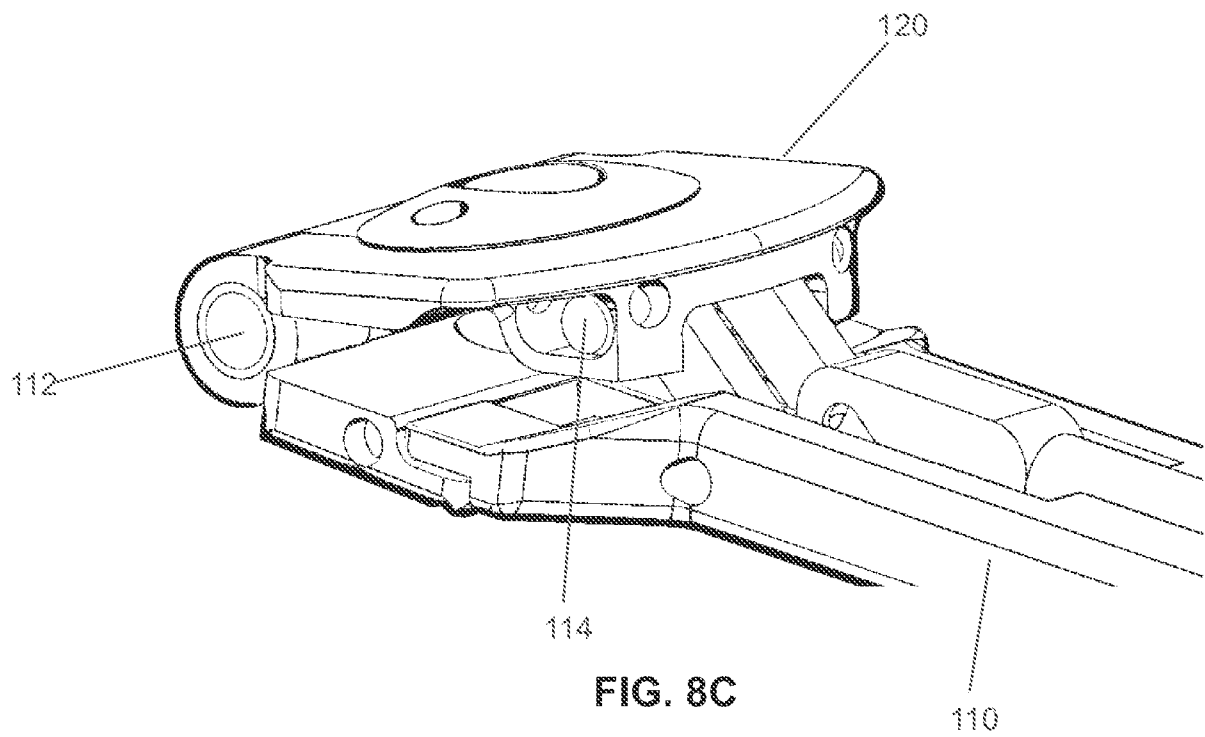


FIG. 8C

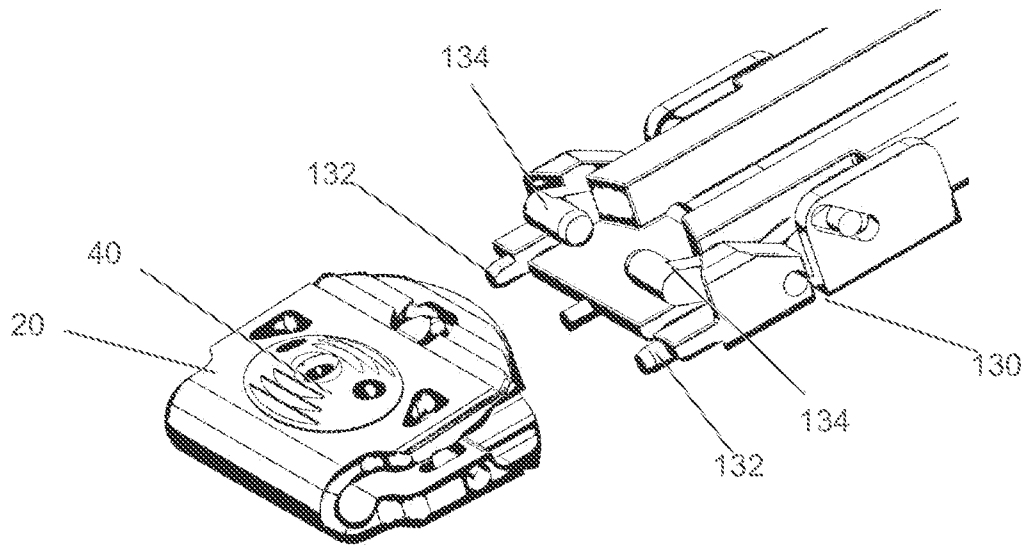


FIG. 9A

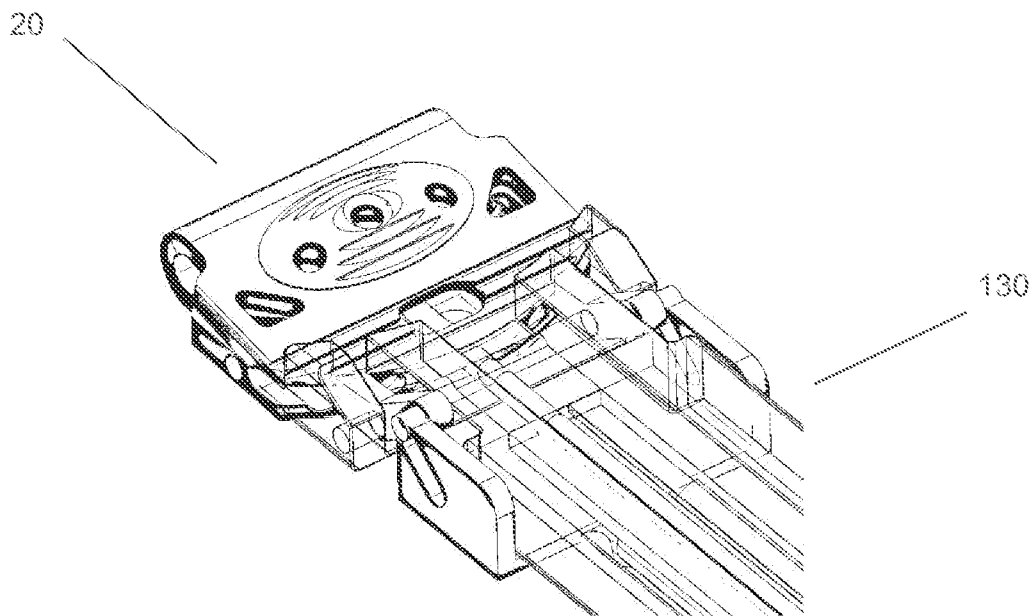


FIG. 9B

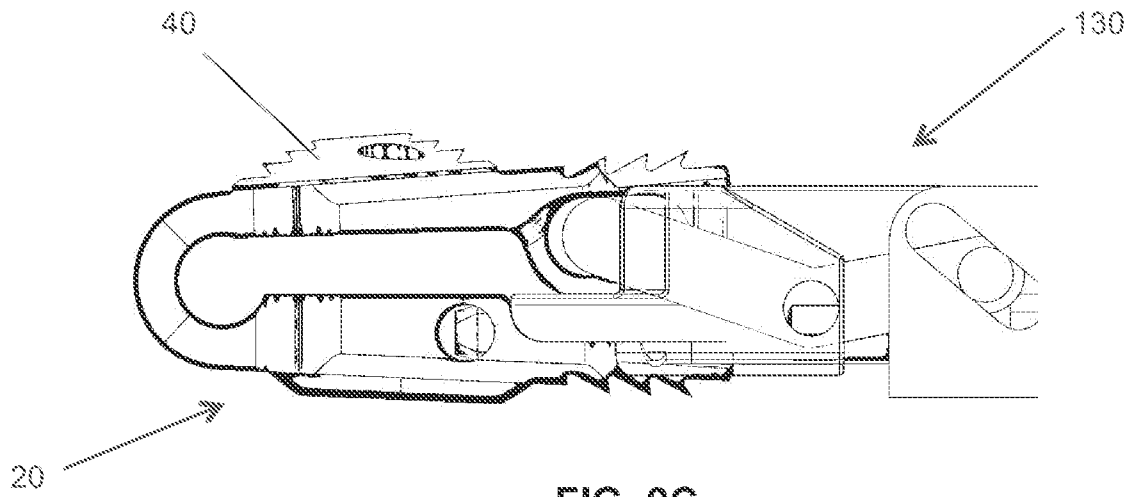


FIG. 9C

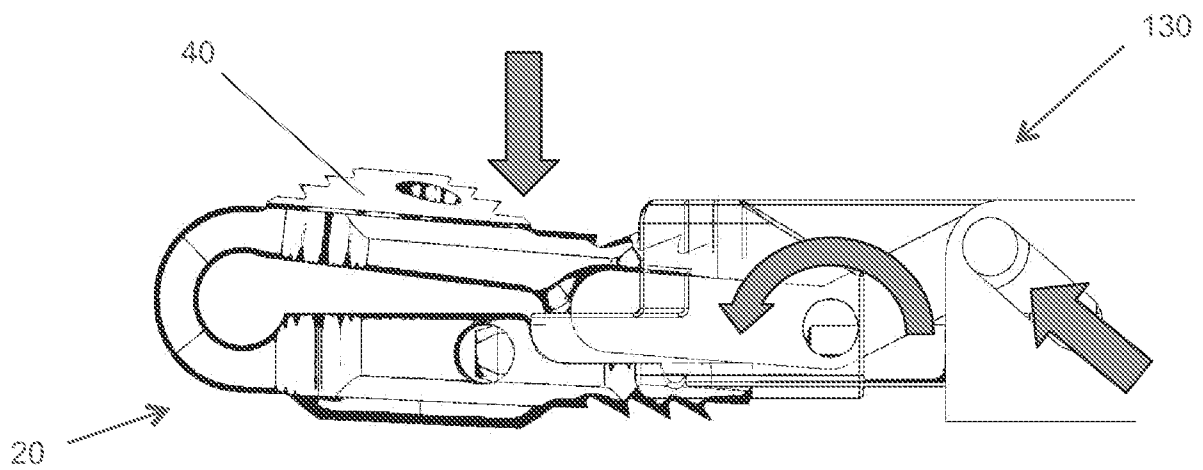


FIG. 9D

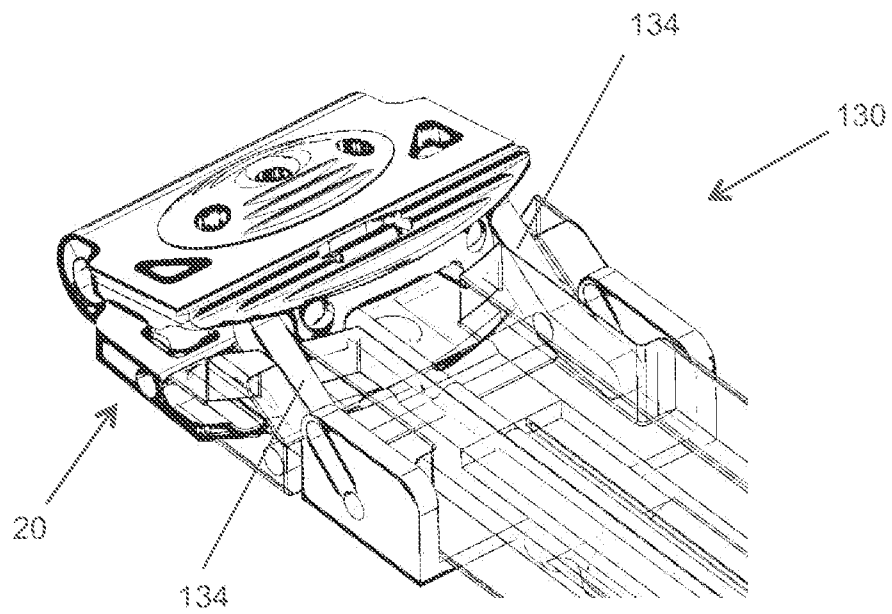


FIG. 9E

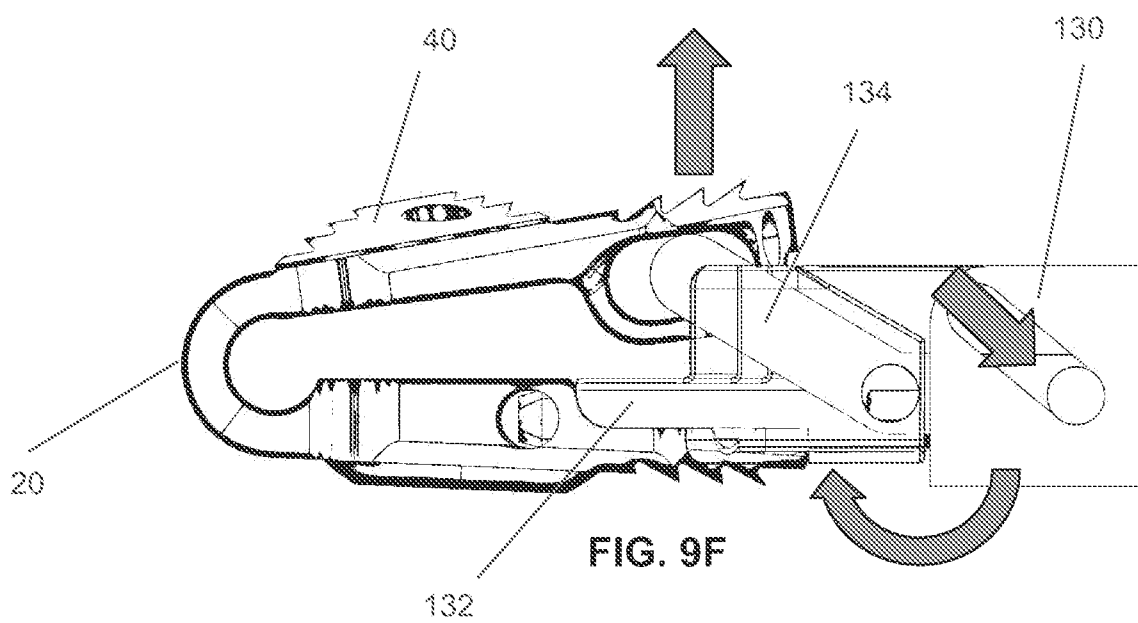


FIG. 9F

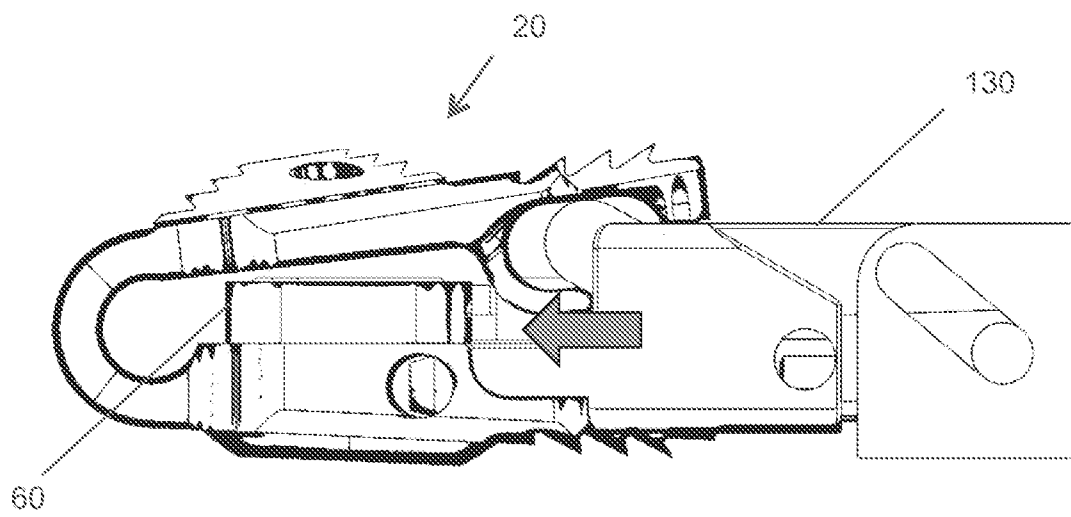
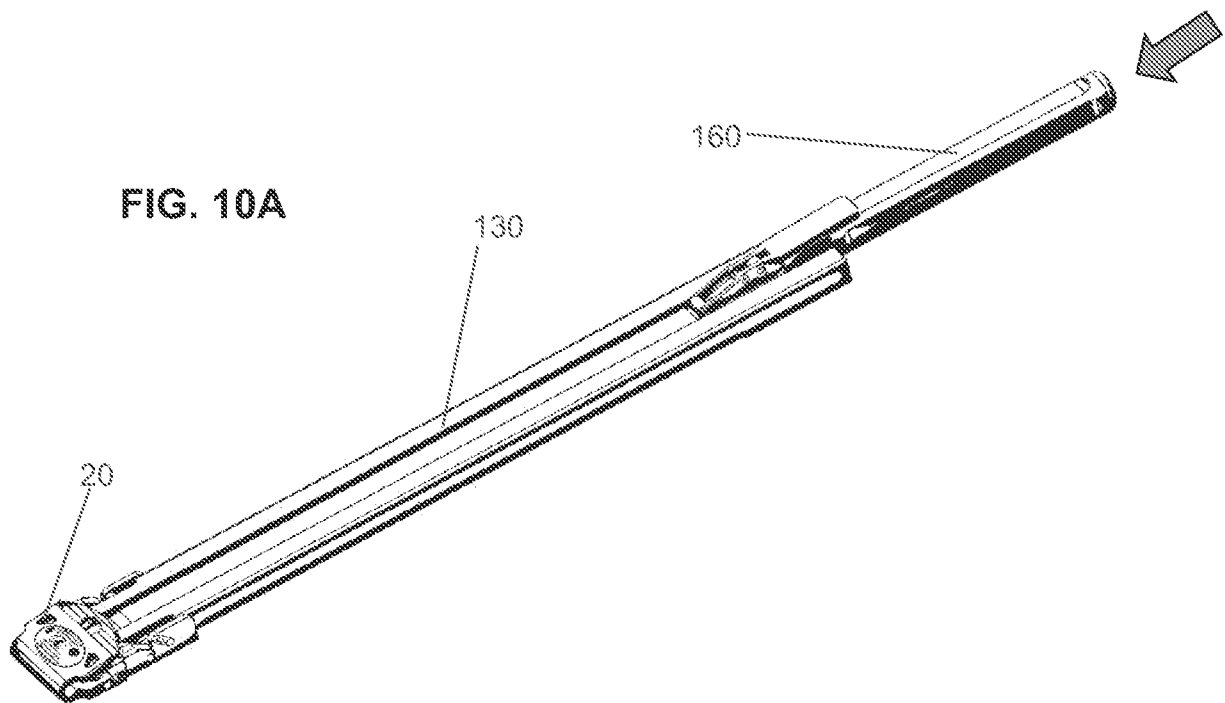


FIG. 10B

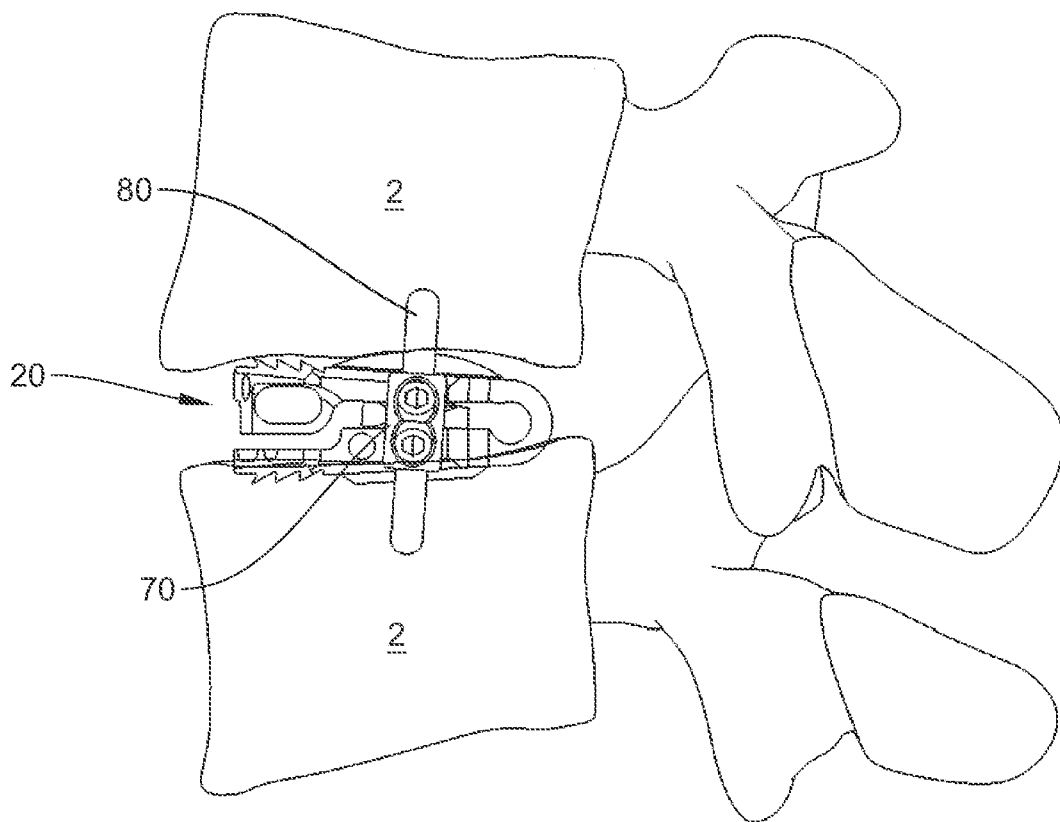


FIG. 11A

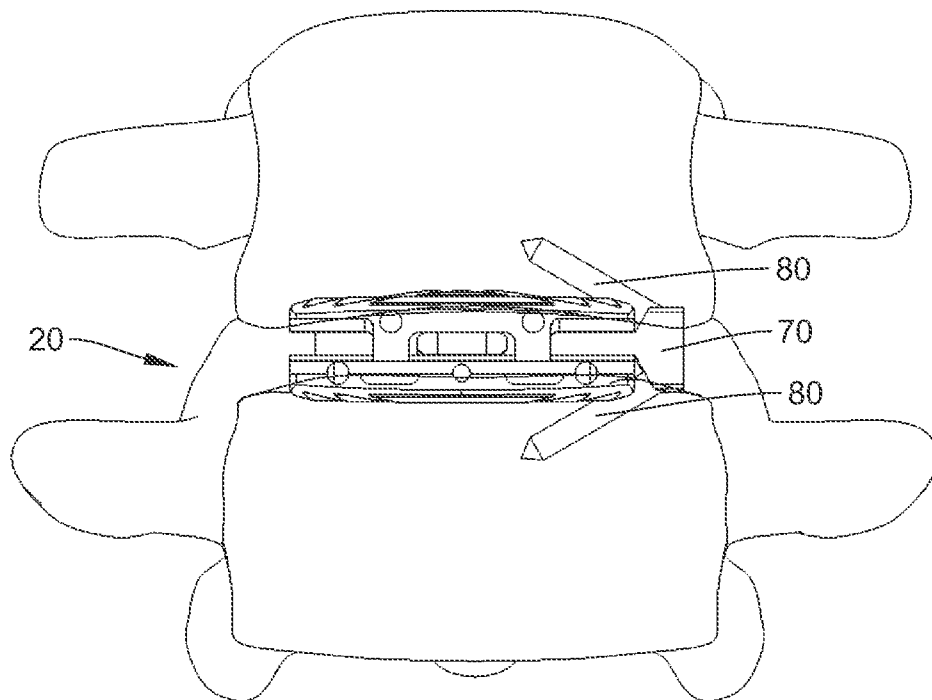


FIG. 11B

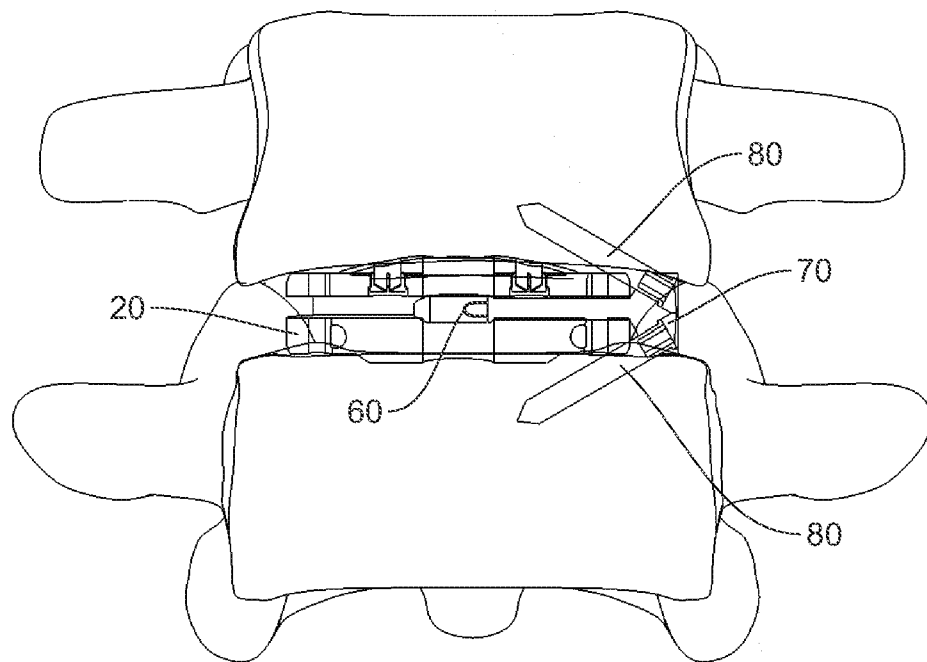


FIG. 11C

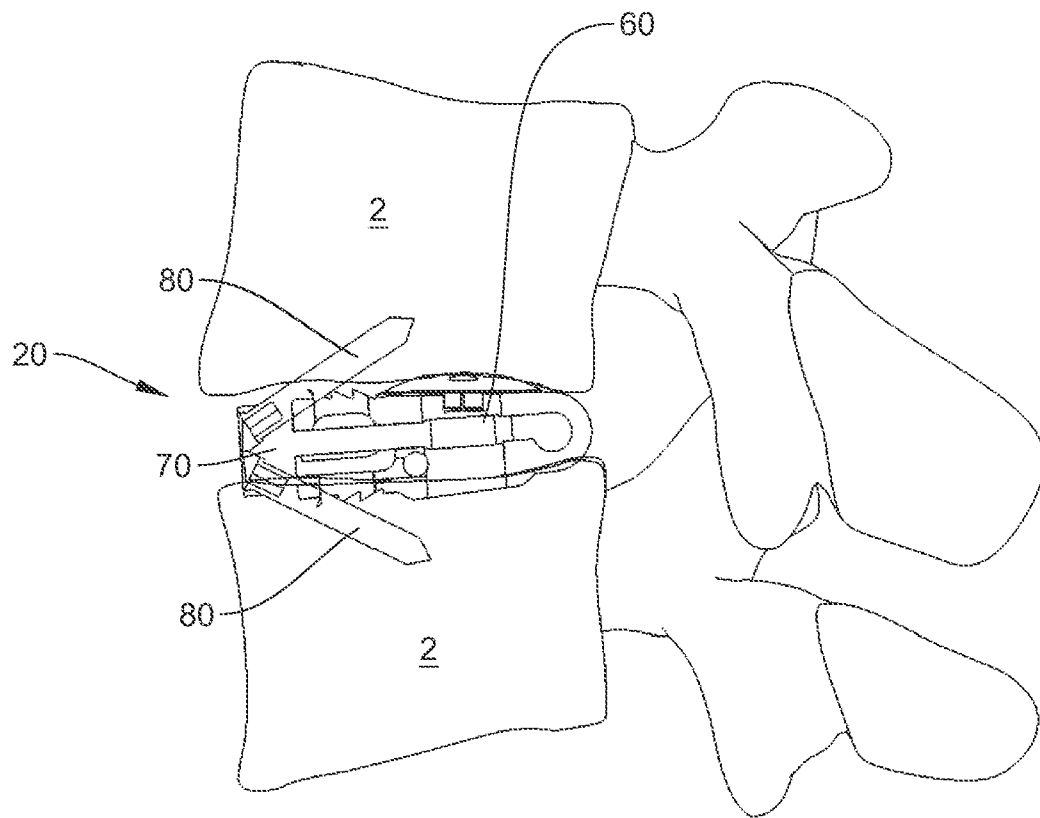


FIG. 11D

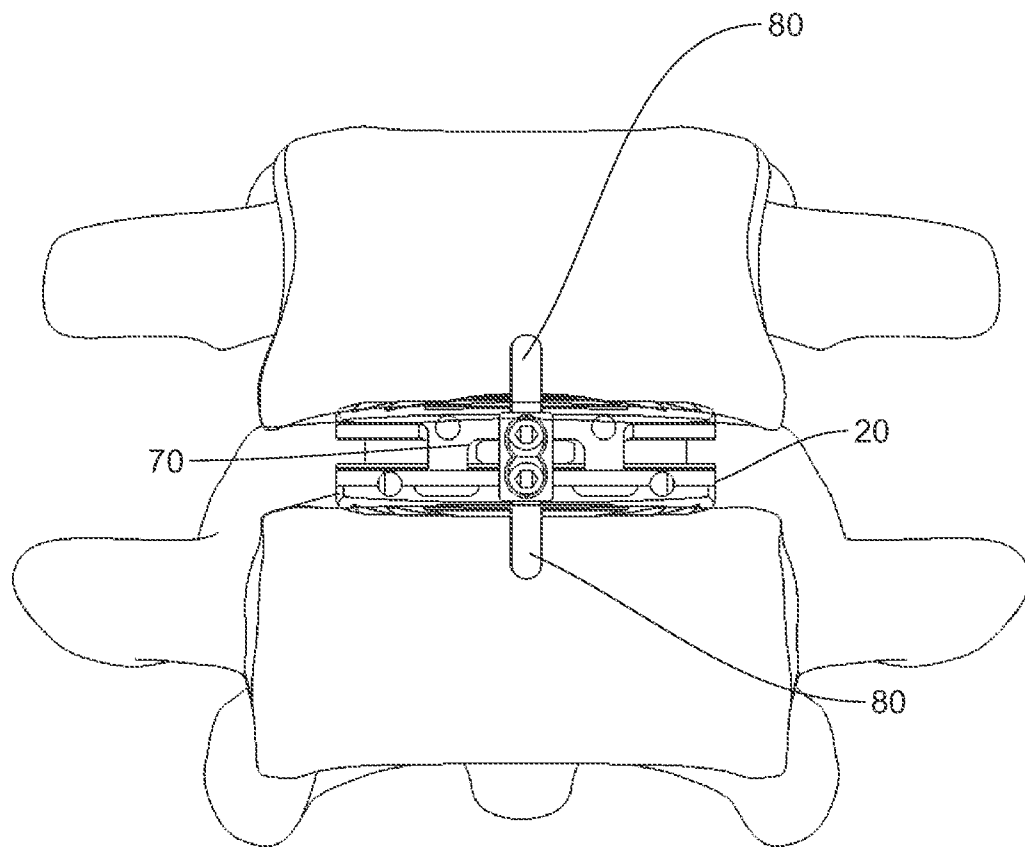


FIG. 11E

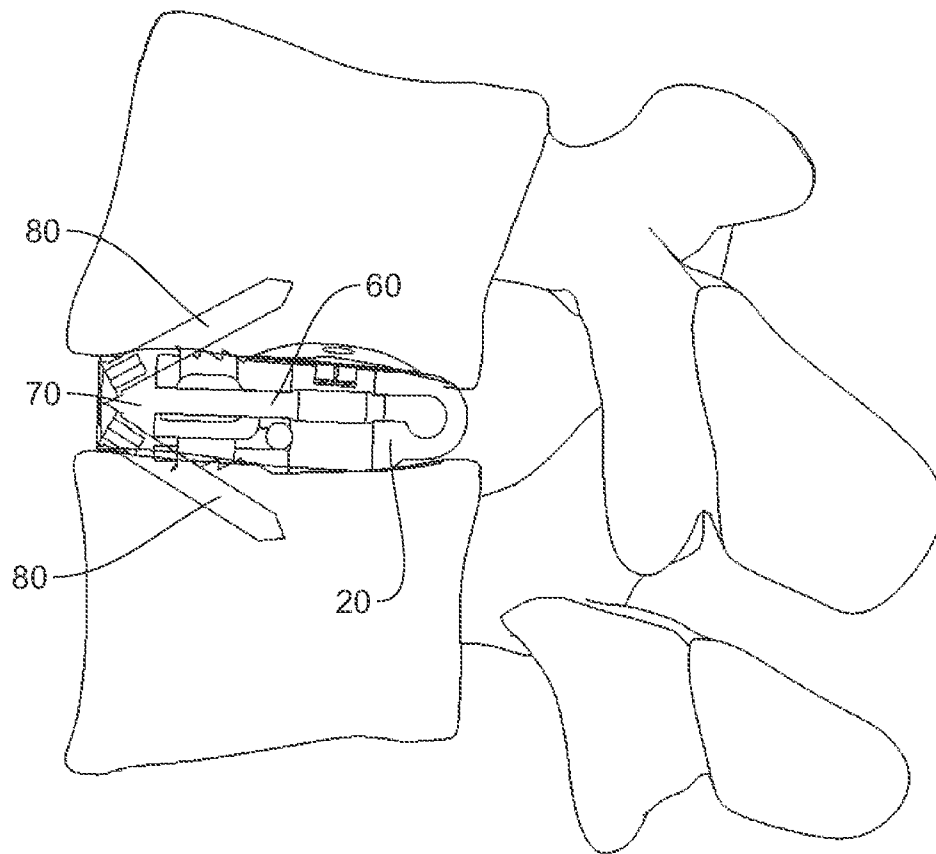


FIG. 11F

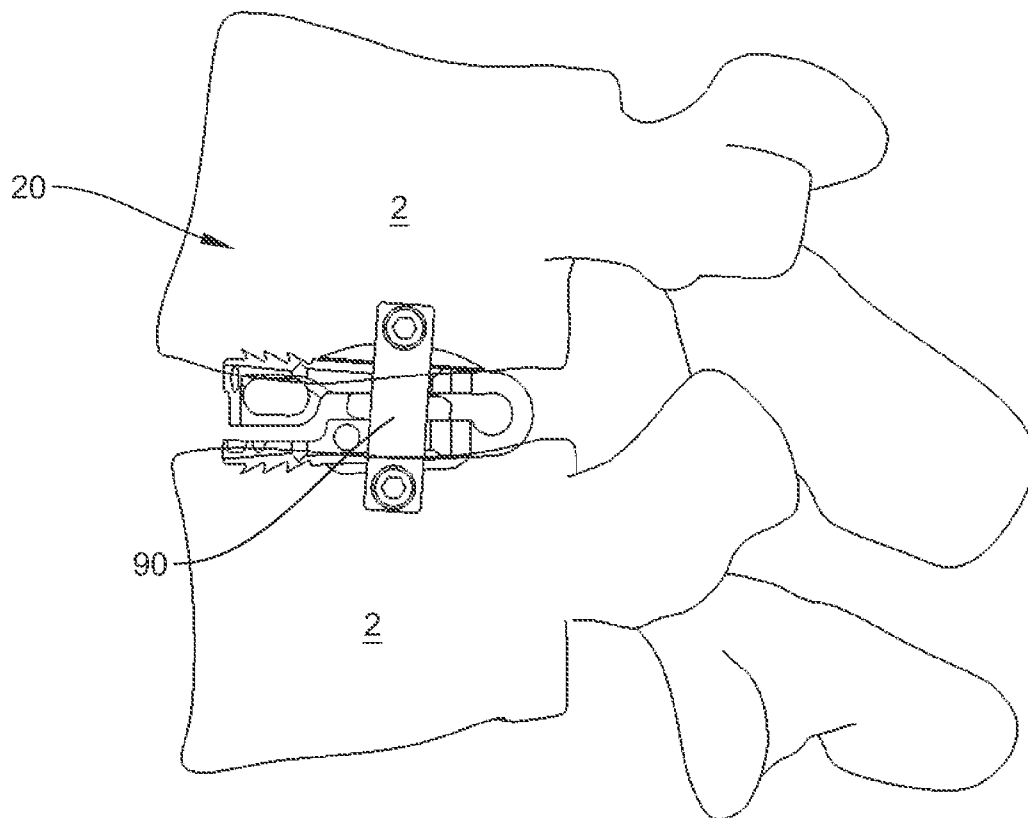


FIG. 12A

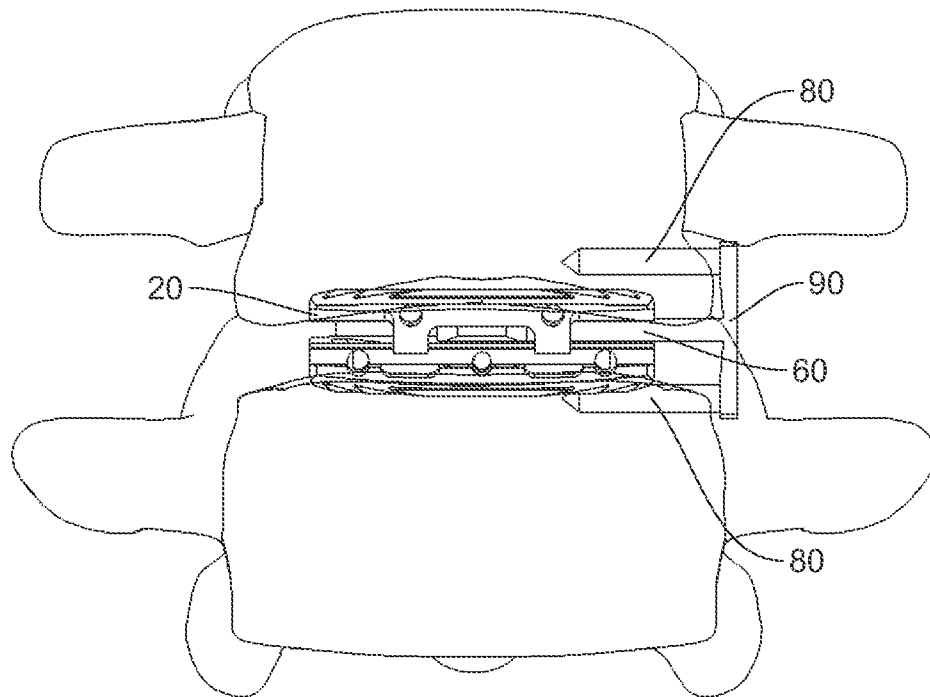


FIG. 12B

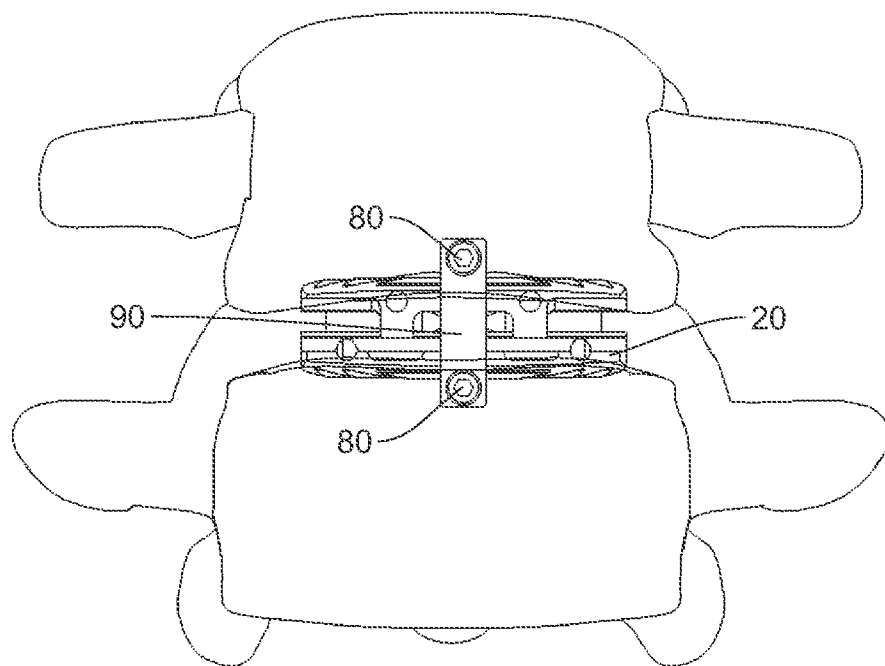


FIG. 12C

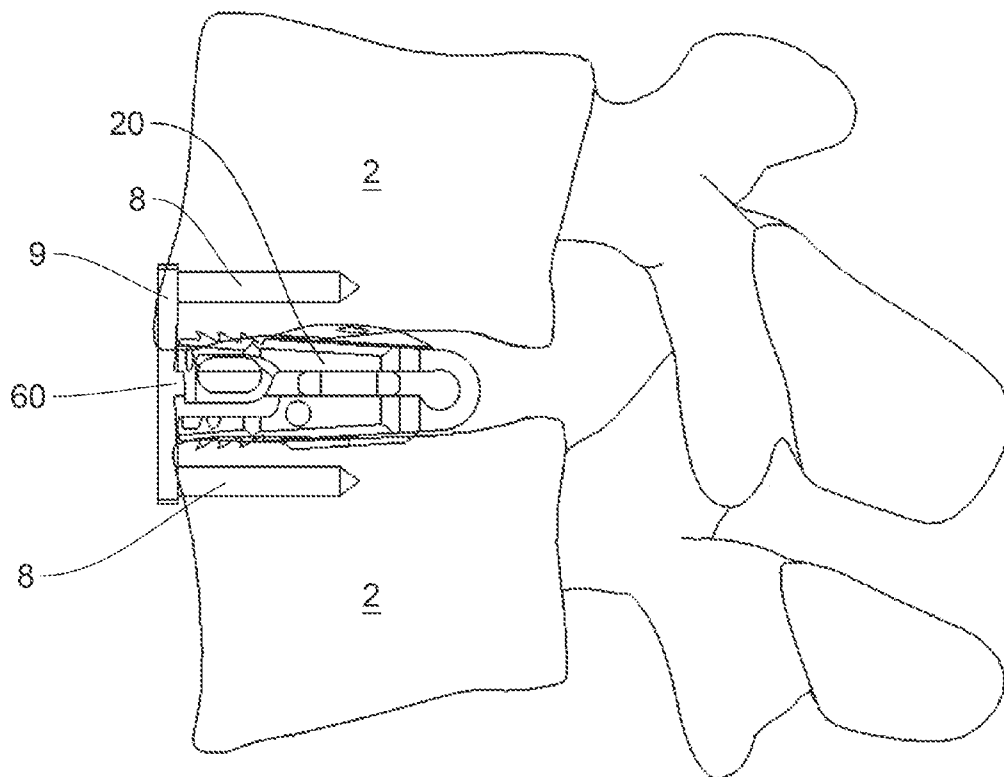


FIG. 12D

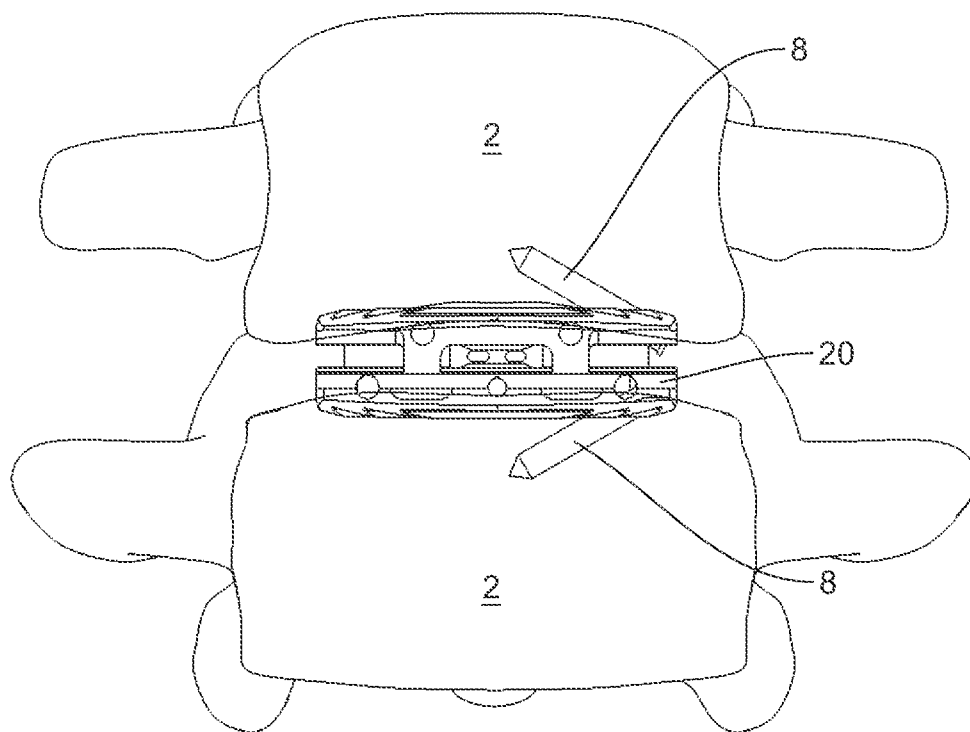


FIG. 13A

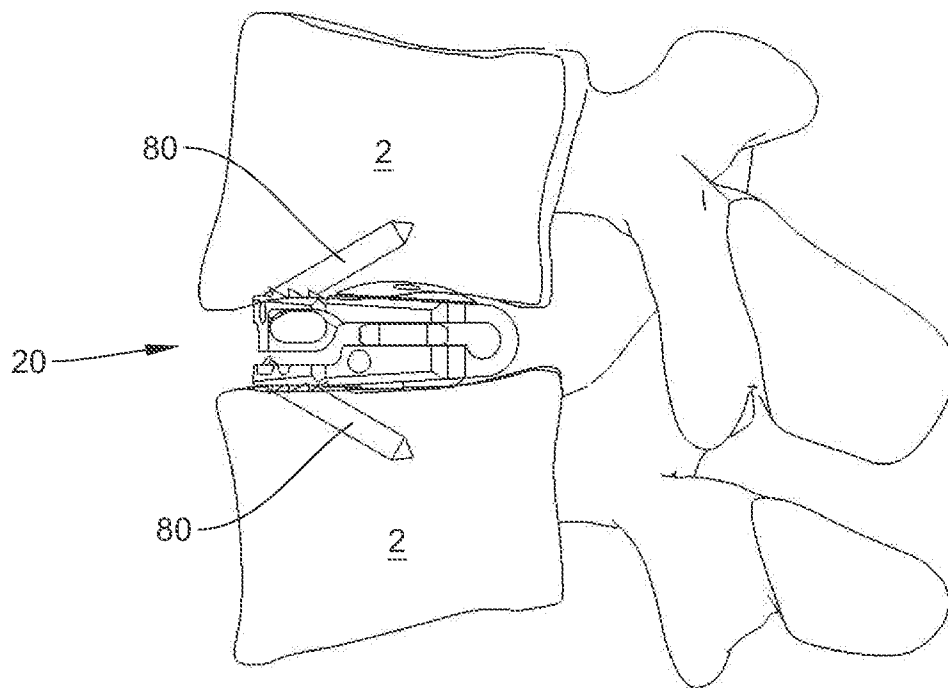


FIG. 13B

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2014/030585

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61F 2/44 (2014.01)

USPC - 606/249; 623/17.16

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8) - A61B 17/70, 17/72; A61F 2/02, 2/30, 2/44 (2014.01)

USPC - 606/246, 247, 248, 249, 279; 623/17.11, 17.15, 17.16

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
CPC - A61F 2/44, 2/442, 2/4425, 2/4455, 2002/44, 2002/442, 2002/4425, 2002/443, 2002/4435 (2014.07)

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

PatBase, Google Patents, Google Scholar, Google

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2006/0247770 A1 (PETERMAN et al) 02 November 2006 (02.11.2006) entire document	1-44
A	US 2010/0234956 A1 (ATTIA et al) 16 September 2010 (16.09.2010) entire document	1-44
A	US 2006/0089714 A1 (LIU et al) 27 April 2006 (27.04.2006) entire document	1-44

☐ Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

06 August 2014

Date of mailing of the international search report

22 AUG 2014

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-3201

Authorized officer:

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774