

(12) United States Design Patent (10) Patent No.:

Brigham et al.

US D885,581 S

(45) Date of Patent: May 26, 2020

(54) SPHYGMOMANOMETER WITH WIRELESS COMMUNICATION DEVICE

(71) Applicant: OMRON HEALTHCARE Co., Ltd.,

Muko-shi, Kyoto (JP)

Inventors: Brian Brigham, Muko (JP); Tsuyoshi

Ogihara, Muko (JP)

Assignee: OMRON HEALTHCARE Co., Ltd.,

Kyoto (JP)

(**) Term: 15 Years

(21) Appl. No.: 29/654,499

(22) Filed: Jun. 25, 2018

(30)Foreign Application Priority Data

Dec	e. 27, 2017	(JI	?)	2017-0	29359
(51)	LOC (12)	Cl.			24-02
(52)	U.S. Cl.			D	24/165
	USPC	• • • • • •		D	24/105

(58) Field of Classification Search

USPC D24/107, 165-168, 186, 187; D10/32, D10/70, 98; D14/344; D11/5 CPC A61B 5/0402; A61B 5/0404; A61B 5/021; A61B 5/024; A61B 5/02438; A61B 5/681; A61B 2560/0205; A61B 2560/0462

See application file for complete search history.

(56)References Cited

U.S. PATENT DOCUMENTS

			Russold				
			Schempp				
			Ogihara				
D800,311 S	*	10/2017	Nishiyama	D24/166			
D801,527 S	*	10/2017	Nishiyama	D24/166			
(Continued)							

Primary Examiner — Anhdao Doan

(74) Attorney, Agent, or Firm — Capitol City TechLaw

(57)**CLAIM**

The ornamental design for a sphygmomanometer with wireless communication device, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, and right side perspective view of a sphygmomanometer with wireless communication device showing our new design;

FIG. 2 is a rear, bottom, and left side perspective view thereof:

FIG. 3 is a front view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a left side view thereof;

FIG. 6 is a front, top, and right side perspective view showing a condition in which a wrist band is unfastened thereof:

FIG. 7 is a rear, bottom, and left side perspective view showing a condition in which the wrist band is unfastened thereof;

FIG. 8 is a right side view showing a condition in which the wrist band is unfastened thereof;

FIG. 9 is a left side view showing a condition in which the wrist band is unfastened thereof;

FIG. 10 is an enlarged partial view in the area of arrow lines 10-10 in FIG. 6;

FIG. 11 is an enlarged partial view in the area of arrow lines 11-11 in FIG. 7;


FIG. 12 is an enlarged partial view in the area of arrow lines 12-12 in FIG. 8;

FIG. 13 is an enlarged partial view in the area of arrow lines 13-13 in FIG. 9; and,

FIG. 14 is an enlarged partial view in the area of arrow lines 14-14 in FIG. 8.

The lighter gray scale showing in the figures illustrate portions of the sphygmomanometer with wireless communication device that form no part of the claimed design.

1 Claim, 14 Drawing Sheets

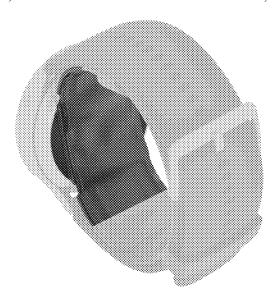

US D885,581 S Page 2

(56) **References Cited**

U.S. PATENT DOCUMENTS

		Brigham D24/165 McKinney A61B 5/02438
		600/509
2018/0192892 A1*	7/2018	Brigham A61B 5/022

^{*} cited by examiner

FIG.1

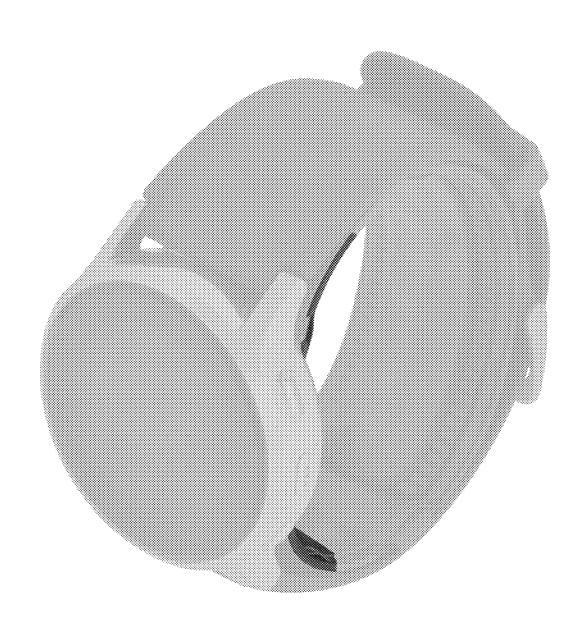


FIG.2

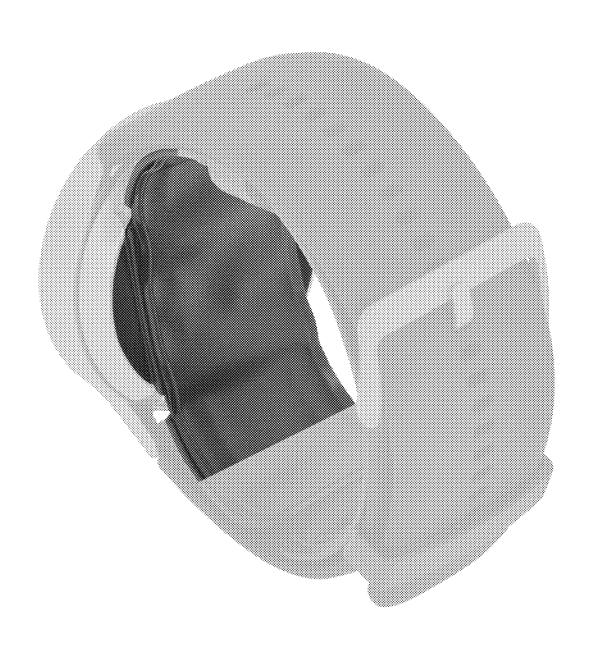


FIG.3

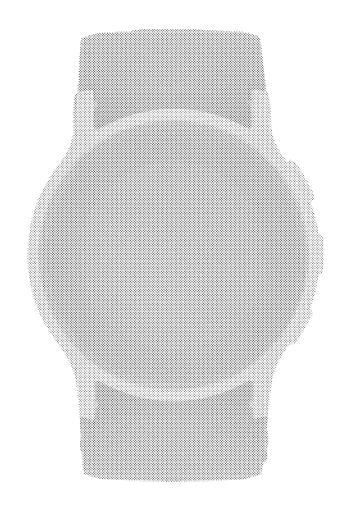


FIG.4

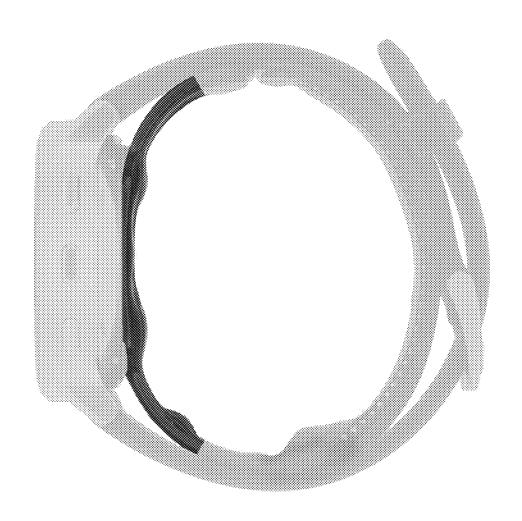


FIG.5

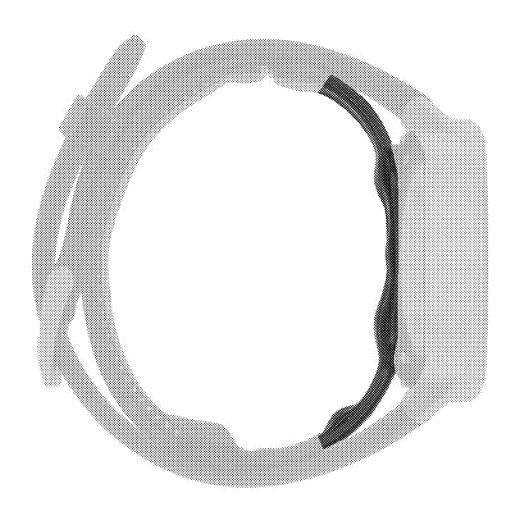


FIG.6

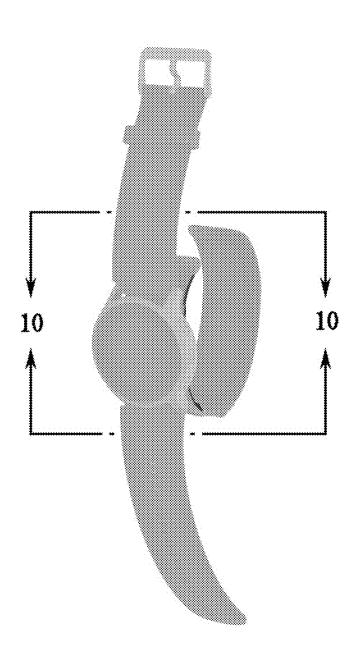


FIG.7

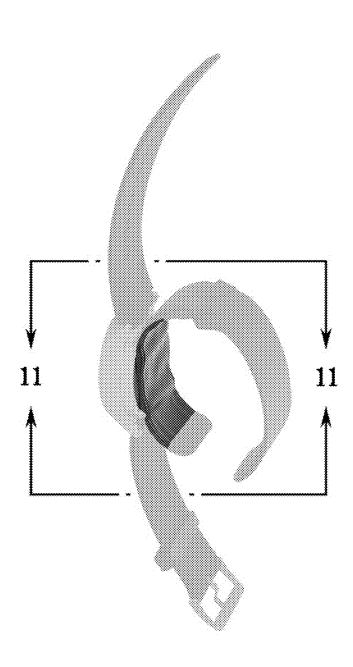


FIG.8

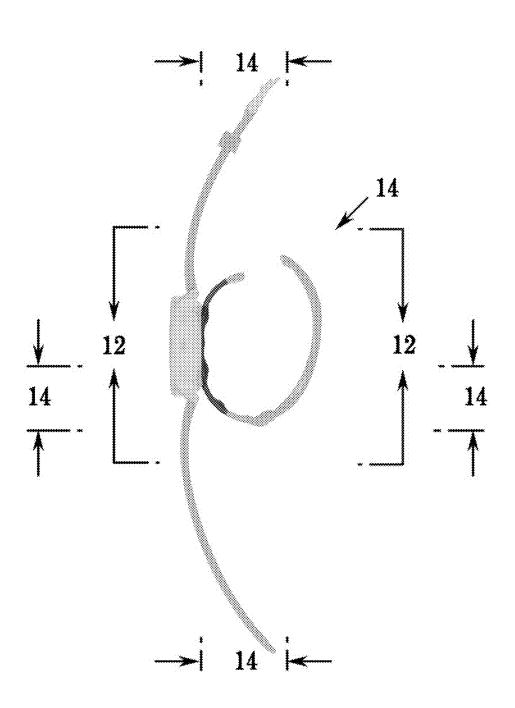


FIG.9

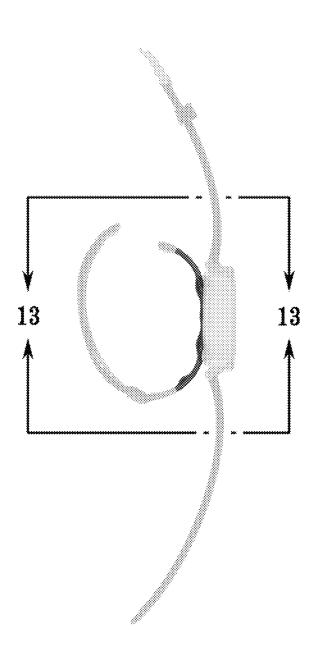


FIG.10

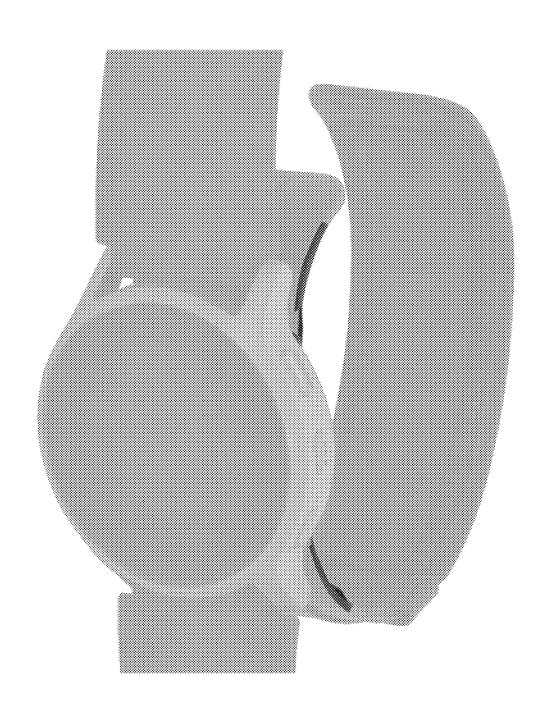


FIG.11

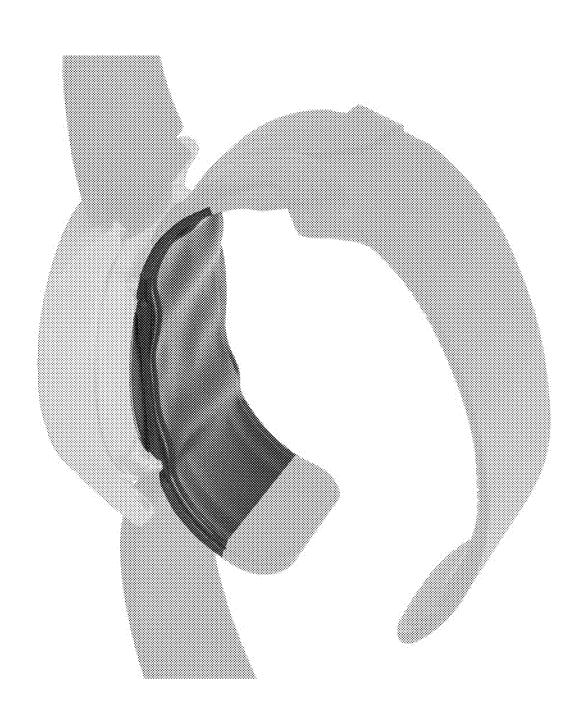


FIG.12

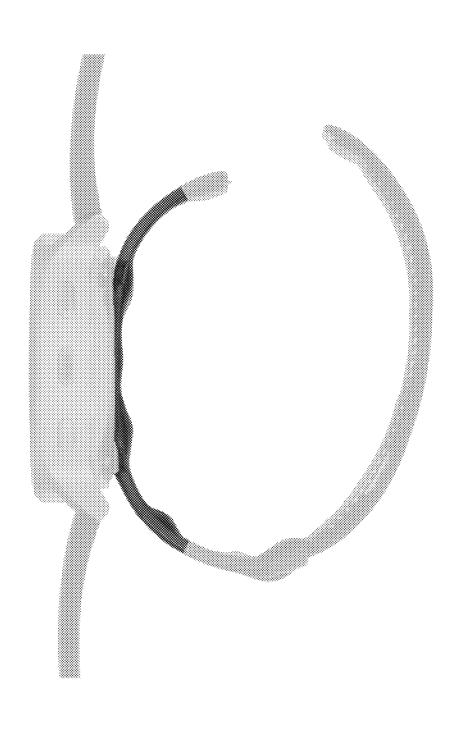


FIG.13

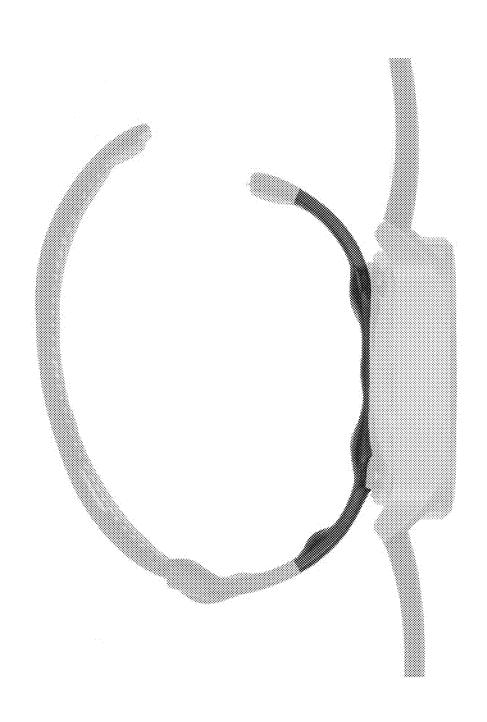


FIG.14

