



(86) Date de dépôt PCT/PCT Filing Date: 2009/04/01
(87) Date publication PCT/PCT Publication Date: 2009/12/03
(85) Entrée phase nationale/National Entry: 2010/09/17
(86) N° demande PCT/PCT Application No.: US 2009/039169
(87) N° publication PCT/PCT Publication No.: 2009/146080
(30) Priorités/Priorities: 2008/04/01 (US61/041,291);
2009/04/01 (US61/165,592)

(51) Cl.Int./Int.Cl. *A61M 5/142* (2006.01),
G05D 7/06 (2006.01), *G06F 3/048* (2006.01)
(71) Demandeur/Applicant:
DEKA PRODUCTS LIMITED PARTNERSHIP, US
(72) Inventeurs/Inventors:
BRYANT, ROBERT J., JR., US;
SPENCER, GEOFFREY P., US;
MANDRO, MARC A., US;
ARMSTRONG, PATRICIA M., US
(74) Agent: GOWLING LAFLEUR HENDERSON LLP

(54) Titre : PROCÉDES ET SYSTÈMES POUR COMMANDER UNE POMPE D'INFUSION
(54) Title: METHODS AND SYSTEMS FOR CONTROLLING AN INFUSION PUMP

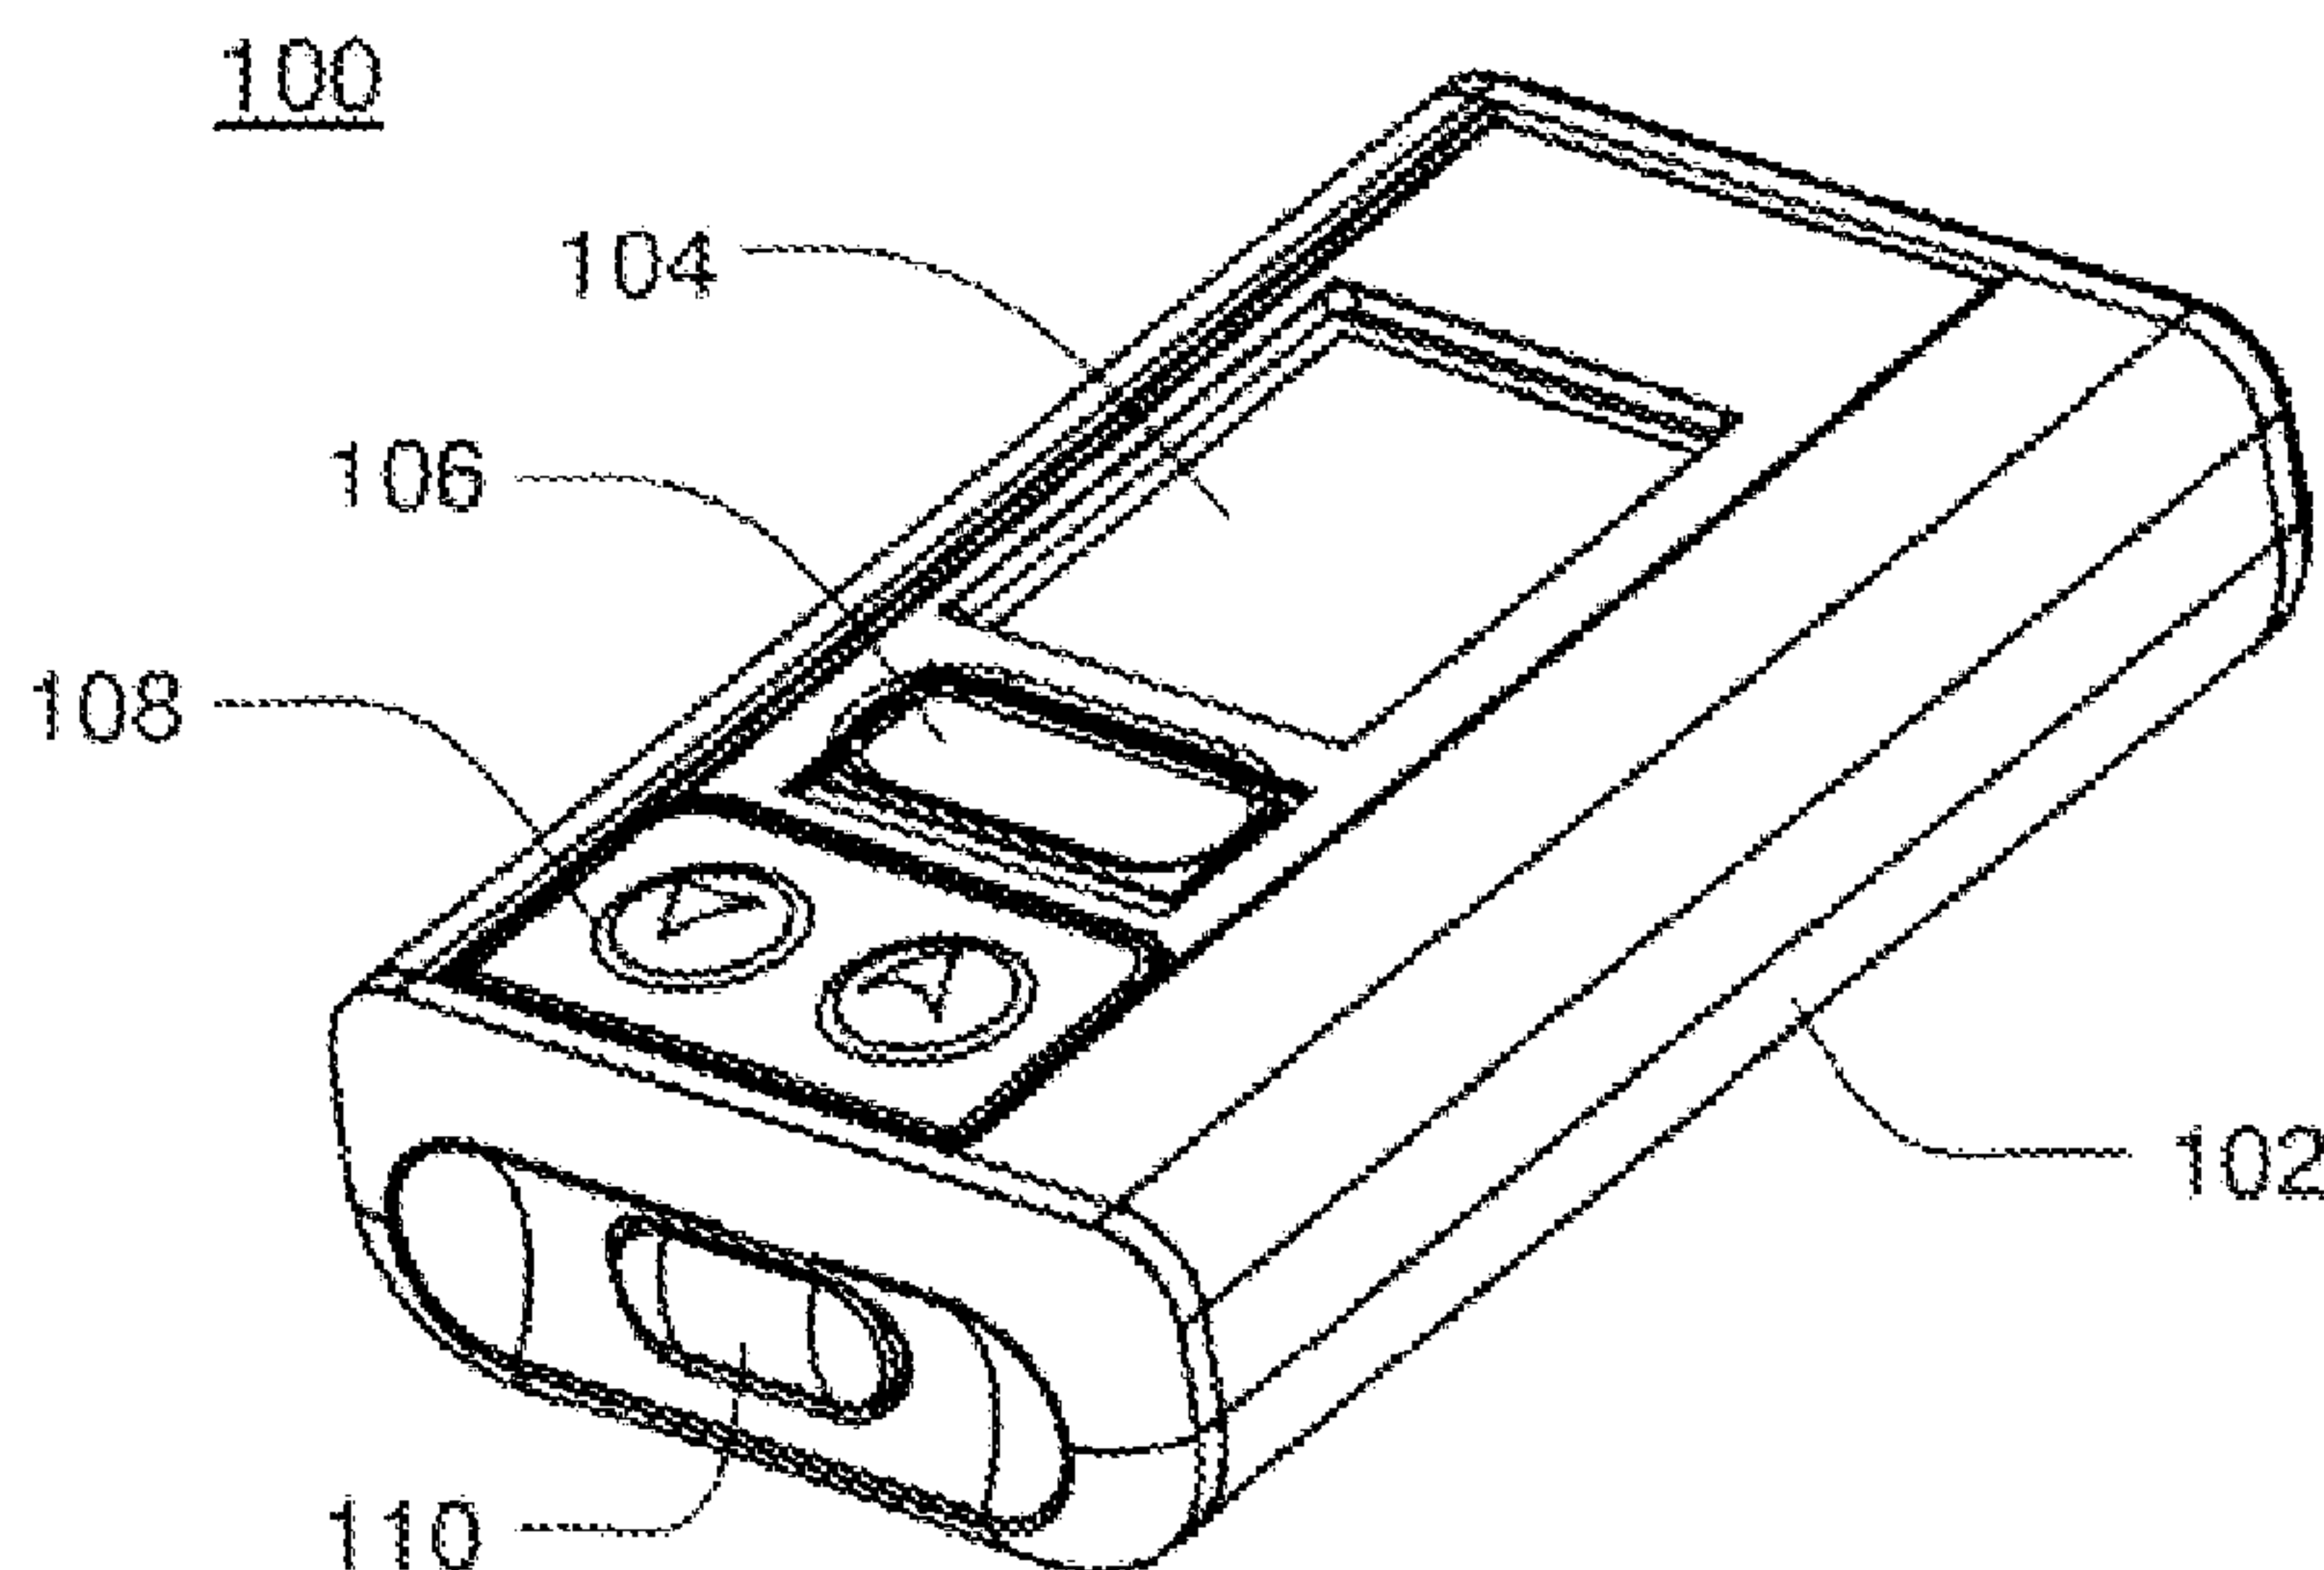


FIG. 1A

(57) **Abrégé/Abstract:**

A system for pairing a controller and an infusion pump is disclosed. The system includes an infusion pump, a controller device and a user interface residing on both the infusion pump and the controller. The user interface includes a pairing mode for enabling wireless communication between the infusion pump and the controller device, wherein the user interface requires both the infusion pump and the controller to be in the pairing mode simultaneously. Also, a method of changing a power source in a infusion pump is disclosed. The method includes placing the infusion pump in idle mode wherein the infusion pump stops delivery. Removing the first power source from the infusion pump. Replacing the first power source with a second power source in the infusion pump, and maintaining the insulin on board during the changing of the first power source with the second power source.



(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

CORRECTED VERSION

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
3 December 2009 (03.12.2009)(10) International Publication Number
WO 2009/146080 A9

(51) International Patent Classification:

A61M 5/142 (2006.01) *G05D 7/06* (2006.01)
G06F 3/048 (2006.01)US]; 199 Woodhill Hooksett Road, Bow, NH 03304 (US). **ARMSTRONG, Patricia, M.** [US/US]; 135 Mc-collum Road, New Boston, NH 03070 (US).

(21) International Application Number:

PCT/US2009/039169

(74) Agent: **TEMPLE, Michelle, Saquet**; Deka Research & Development Corp., 340 Commercial Street, Manchester, NH 03101-1129 (US).

(22) International Filing Date:

1 April 2009 (01.04.2009)

(81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/041,291 1 April 2008 (01.04.2008) US
61/165,592 1 April 2009 (01.04.2009) US(71) **Applicant** (*for all designated States except US*): **DEKA PRODUCTS LIMITED PARTNERSHIP** [US/US]; 340 Commercial Street, Manchester, NH 03101-1129 (US).

(72) Inventors; and

(75) **Inventors/Applicants** (*for US only*): **BRYANT, Robert, J.** [US/US]; 222 Blucher Street, Manchester, NH 03102 (US). **SPENCER, Geoffrey, P.** [US/US]; 40 Fogg Court, Manchester, NH 03104 (US). **MANDRO, Marc, A.** [US/(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR),

[Continued on next page]

(54) Title: METHODS AND SYSTEMS FOR CONTROLLING AN INFUSION PUMP

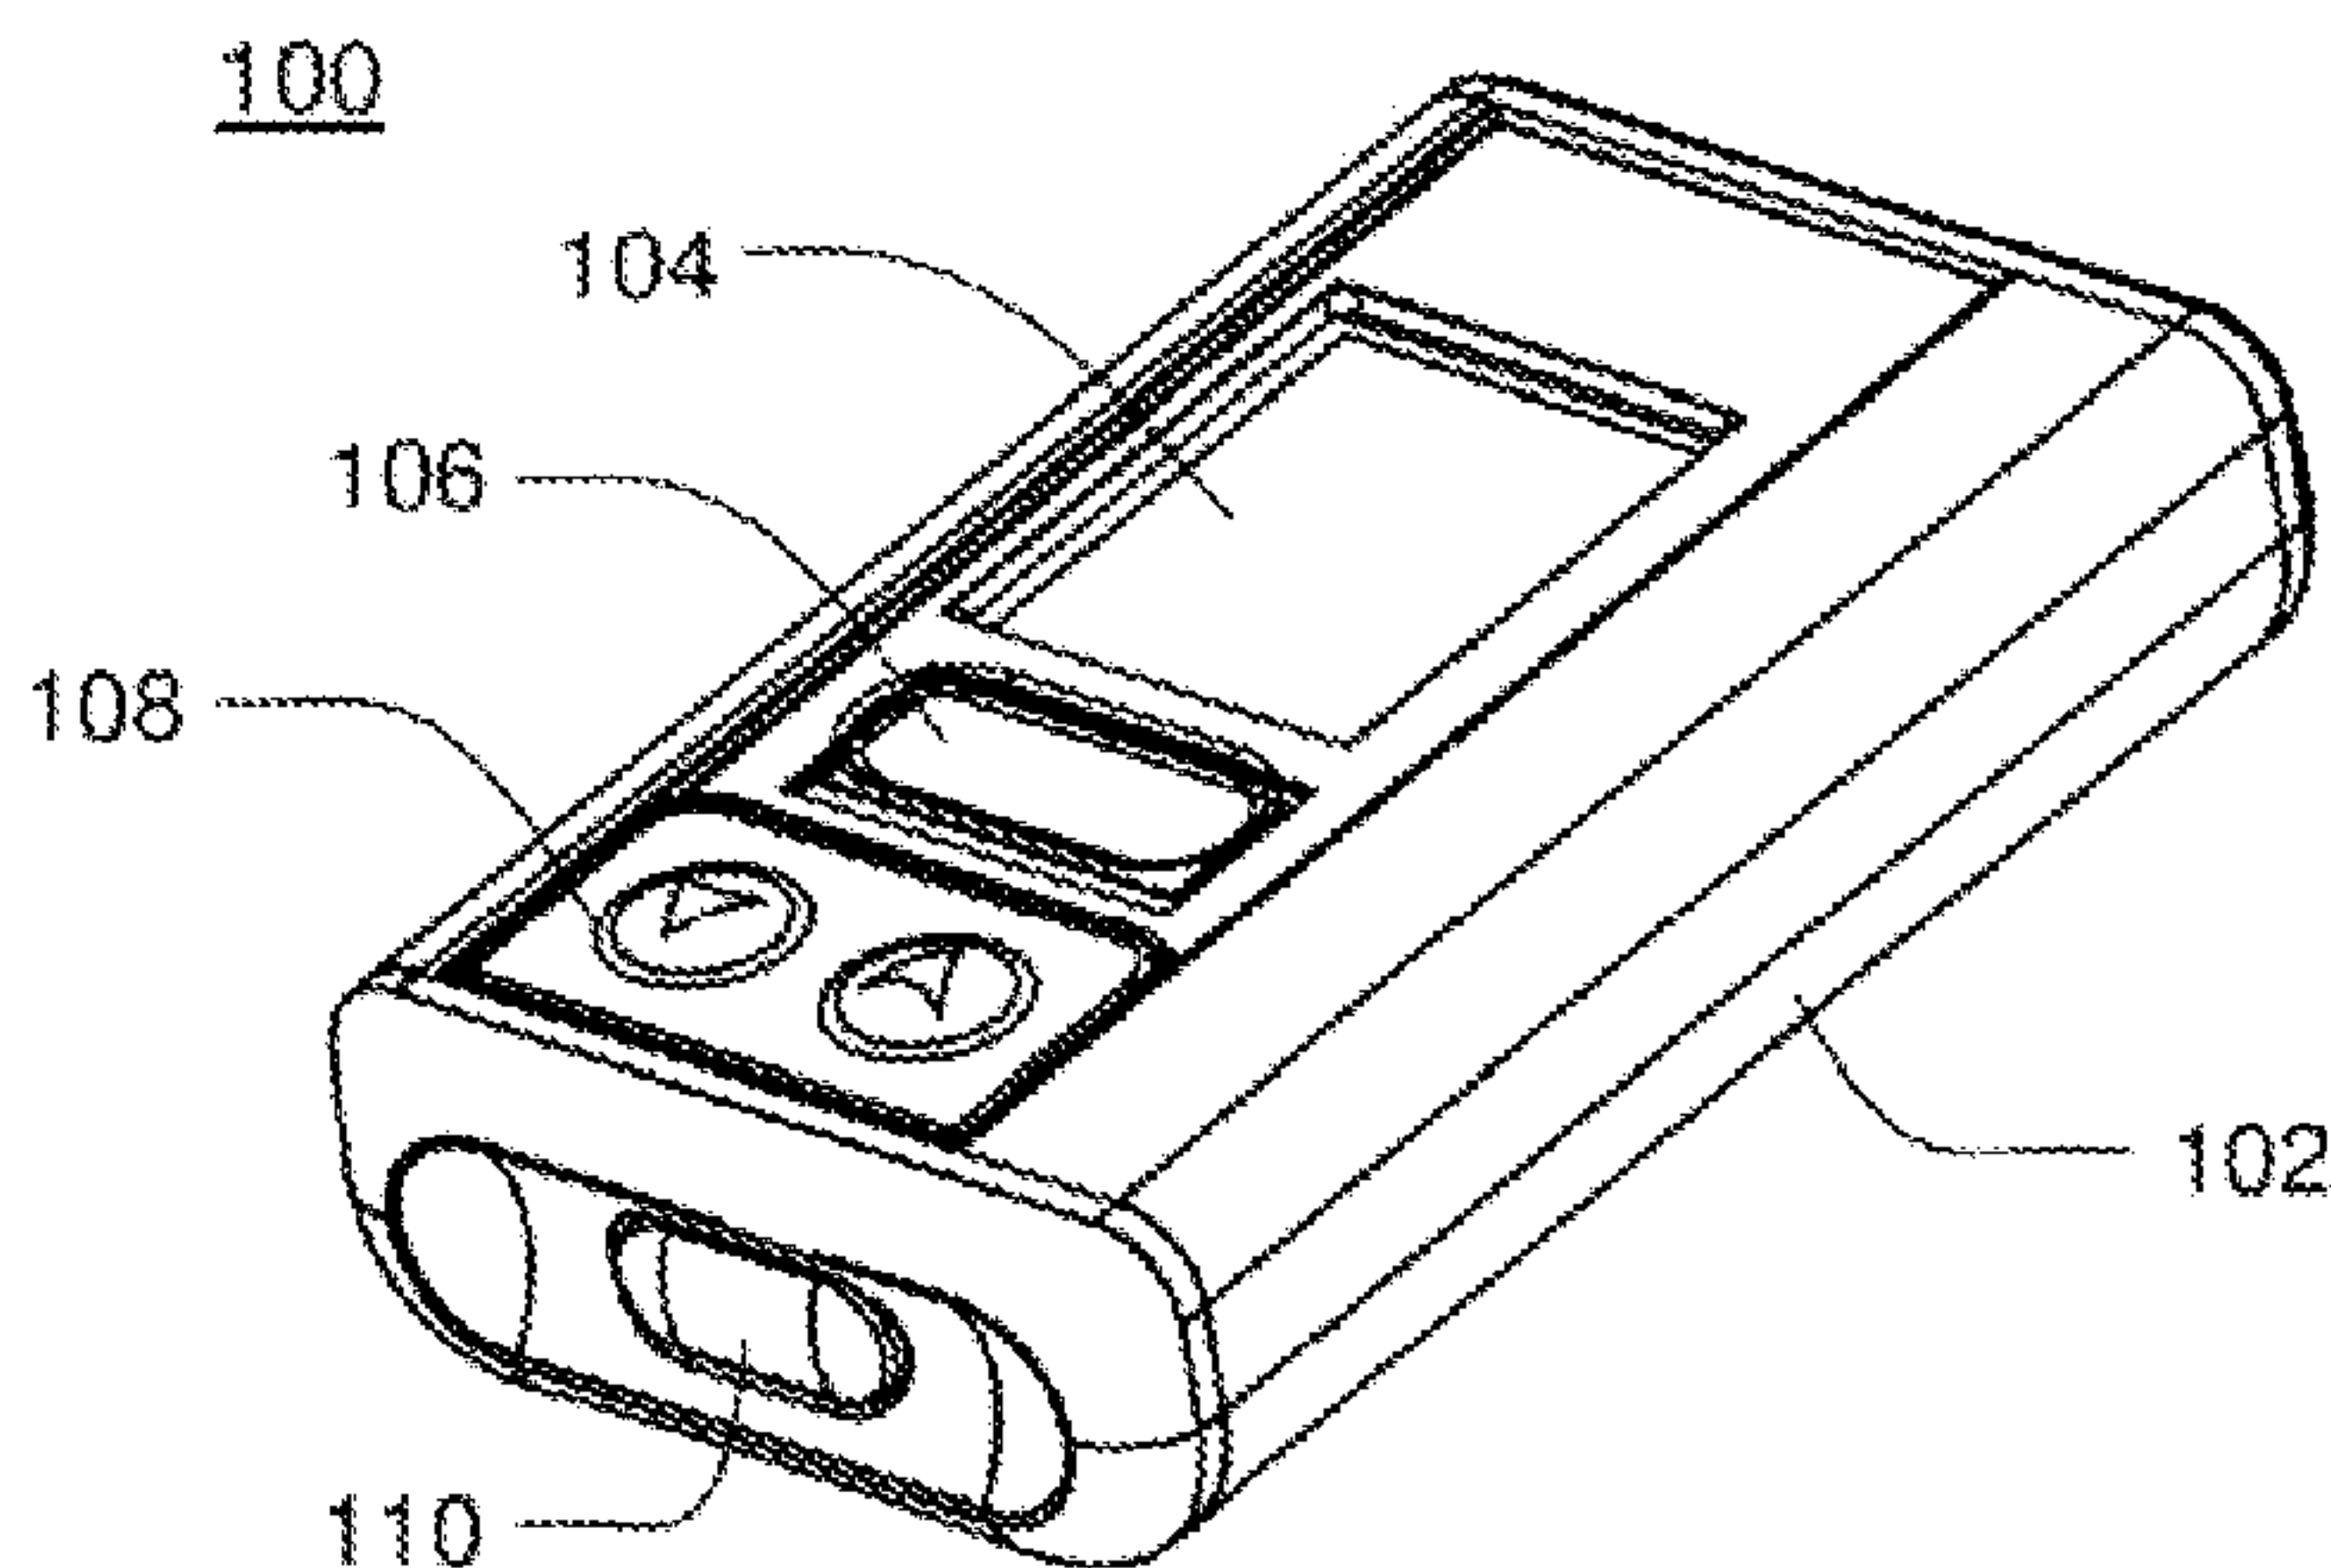


FIG. 1A

(57) **Abstract:** A system for pairing a controller and an infusion pump is disclosed. The system includes an infusion pump, a controller device and a user interface residing on both the infusion pump and the controller. The user interface includes a pairing mode for enabling wireless communication between the infusion pump and the controller device, wherein the user interface requires both the infusion pump and the controller to be in the pairing mode simultaneously. Also, a method of changing a power source in a infusion pump is disclosed. The method includes placing the infusion pump in idle mode wherein the infusion pump stops delivery. Removing the first power source from the infusion pump. Replacing the first power source with a second power source in the infusion pump, and maintaining the insulin on board during the changing of the first power source with the second power source.

WO 2009/146080 A9

OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG). **(48) Date of publication of this corrected version:**

4 March 2010

Declarations under Rule 4.17:

— *of inventorship (Rule 4.17(iv))*

(15) Information about Correction:

see Notice of 4 March 2010

Published:

— *without international search report and to be republished upon receipt of that report (Rule 48.2(g))*

METHODS AND SYSTEMS FOR CONTROLLING AN INFUSION PUMP

5 CROSS REFERENCE TO RELATED APPLICATIONS

This application claims priority from the following United States Provisional Patent Applications: U.S. Provisional Patent Application Serial No. 61/041, 291 filed on April 1, 2008 and entitled Methods and Systems for Controlling a Medical Device and U.S.
10 Provisional Patent Application Serial No. 61/165,592 filed on April 1, 2009 and entitled Methods and Systems for Controlling a Medical Device, both of which are incorporated by reference herein in their entireties.

TECHNICAL FIELD

15 The present invention relates to infusion pumps and more particularly, to methods and systems for controlling an infusion pump.

BACKGROUND INFORMATION

Many potentially valuable medicines or compounds, including biologicals, are not
20 orally active due to poor absorption, hepatic metabolism or other pharmacokinetic factors. Additionally, some therapeutic compounds, although they may be orally absorbed, are sometimes required to be administered so often it is difficult for a patient to maintain the desired schedule. In these cases, parenteral delivery is often employed or could be employed.

25 Effective parenteral routes of drug delivery, as well as other fluids and compounds, such as subcutaneous injection, intramuscular injection, and intravenous (IV) administration include puncture of the skin with a needle or stylet. Insulin is an example of a therapeutic fluid that is self-injected by millions of people living with diabetes. Users of parenterally delivered drugs may benefit from a wearable device that would automatically deliver
30 needed drugs/compounds over a period of time.

To this end, there have been efforts to design portable and wearable devices for the controlled release of therapeutics. Such devices are known to have a reservoir such as a cartridge, syringe, or bag, and to be electronically controlled. These devices suffer from a

number of drawbacks. Reducing the size, weight and cost of these devices is also an ongoing challenge.

Additionally, many of these devices require frequent and direct interaction between the device and the user, or the device and a caregiver. Thus, in these cases, it is often
5 desired that the device be worn clipped to clothing or a belt, or in a pocket, thus being accessible in any situation. However, this is not always practical or possible. Thus, there is a desire for a device that may be controlled by a remote device such that the user or caregiver does not require frequent direct interaction.

Further, safety is an ongoing concern with any medical device. Thus, systems and
10 methods that impart added safety to the user are desired.

SUMMARY

In accordance with one aspect of the present invention, a system for pairing a controller and an infusion pump is disclosed. The system includes an infusion pump, a
15 controller device and a user interface residing on both the infusion pump and the controller. The user interface includes a pairing mode for enabling wireless communication between the infusion pump and the controller device, wherein the user interface requires both the infusion pump and the controller to be in the pairing mode simultaneously.

Some embodiments of this aspect of the present invention may include one or more
20 of the following. Where the controller includes a display. Where the infusion pump includes a display. Where both the controller and the infusion pump include a display. Where the pairing mode further includes a timeout feature, wherein the pairing mode will timeout if the pairing is not completed within a predetermined time. Where the pairing mode further includes an indicator to indicate the user interface has found a device in which
25 to pair, the indicator comprising a serial number. Where the pairing mode requires the infusion pump and the controller to be set to the same glucose units.

In accordance with one aspect of the present invention, a method of changing a power source in an infusion pump is disclosed. The method includes placing the infusion pump in idle mode wherein the infusion pump stops delivery. Removing the first power
30 source from the infusion pump. Replacing the first power source with a second power source in the infusion pump, and maintaining the insulin on board during the changing of the first power source with the second power source.

Some embodiments of this aspect of the present invention may include one or more of the following. Where the method further includes sending a notification when the time

between the first power source being removed and the second power source being replaced exceeds a threshold.

In accordance with one aspect of the present invention, a system for determining the internal temperature of an infusion pump. The system includes an infusion pump, the
5 infusion pump including a temperature sensor. The temperature sensor located such that it may determine the internal temperature of the infusion pump and send information to a processor in the infusion pump. When the temperature either exceeds a predetermined maximum threshold, or falls below a predetermined minimum threshold, the infusion pump notifies the user.

10 These aspects of the invention are not meant to be exclusive and other features, aspects, and advantages of the present invention will be readily apparent to those of ordinary skill in the art when read in conjunction with the appended claims and accompanying drawings.

15 BRIEF DESCRIPTION OF THE DRAWINGS

These and other features and advantages of the present invention will be better understood by reading the following detailed description, taken together with the drawings wherein:

FIGS. 1A-1B are front and back isometric views of one embodiment of an infusion
20 pump assembly;

FIGS. 1C-1E are side and front views of one embodiment of an infusion pump assembly of FIG. 1;

FIG. 1F is a front isometric view of one embodiment of an infusion pump assembly of FIG. 1;

25 FIGS. 2A-2D are various view of an exemplary embodiment of an infusion pump assembly;

FIG. 3 is an illustrative view of one embodiment of a remote controller or companion assembly;

FIG. 4 is a diagrammatic view of the infusion pump assembly of FIG. 1;

30 FIGS. 5A-5C shows exemplary embodiments of select Time and Date Wizard screens according to one embodiment;

FIG. 6 shows an exemplary embodiment of the Cancel Changes Confirmation Screen;

FIGS. 7A-7C shows an exemplary embodiment of at least a selection of the pair device screens;

FIGS. 8A-8B shows an exemplary embodiment of at least a selection of the insulin profile screens;

5 FIGS. 9A-9B shows an exemplary embodiment of at least a selection of the display screens;

FIGS. 10A-10E shows an exemplary embodiment of at least a selection of the home screens;

10 FIGS. 11A-11B shows an exemplary embodiment of at least a selection of IU DROP screens;

FIG. 12 shows an exemplary embodiment of at least a selection of LOCKED ITEMS screens;

FIGS. 13A-13B shows an exemplary embodiment of at least a selection of WARNING screens;

15 FIGS. 14A-14B shows an exemplary embodiment of at least a selection of Companion WARNING screens;

FIG. 15 shows an exemplary embodiment of at least a selection of Companion Temporary Lockout;

FIG. 16 shows an exemplary embodiment of at least a selection of Radio screens;

20 FIG. 17 shows an exemplary embodiment of at least one alert, reminder and recoverable screens;

FIGS. 18A-18B shows an exemplary embodiment of at least a selection of REMINDER and SET SLEEP TIME screens according to an exemplary embodiment;

25 FIGS. 19A-19E shows exemplary embodiments of at least a selection of ALARM screens;

FIGS. 20A-20I shows exemplary embodiments of at least a selection of ALERT screens;

FIGS. 21A-21B show exemplary embodiments of at least a selection of REMINDER screens;

30 FIG. 22 shows an exemplary embodiment of at least a selection of screens for setting the Frequency of a SITE CHANGE Care Comment;

FIGS. 23A-23B, show exemplary embodiments of at least a selection of BOLUS screens;

FIGS. 24A-24D shows exemplary embodiments of at least a selection of

WARNING and CONFIRM screens;

FIG. 25 shows an exemplary embodiment of at least a selection of HISTORY screens;

FIG. 26 shows an exemplary embodiment of at least a selection of REPORTS
5 screens;

FIG. 27 shows an exemplary embodiment of at least a selection of DIARY screens;

FIG. 28 shows an exemplary embodiment of at least a selection of DAILY THERAPY screens;

FIGS. 29A-29B shows an exemplary embodiment of at least a selection of EVENT
10 SUMMARY screens;

FIG. 30 shows an exemplary embodiment of at least a selection of ALARM SUMMARY screens;

FIG. 31 shows an exemplary embodiment of at least a selection of SEND DIARY screens;

FIG. 32 shows an exemplary embodiment of at least a selection of screens related to
15 the PC Connection;

FIG. 33 shows an exemplary embodiment of at least a selection of screens related to the diary log transfer to a PC; and

FIGS. 34A-34D shows an exemplary embodiment of at least a selection of screens
20 related to the diary log transfer to a PC.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Definitions

As used in this description and the accompanying claims, the following terms shall
25 have the meanings indicated, unless the context otherwise requires:

A “device” shall mean a medical device, which includes, but is not limited to, an infusion pump and/or a controller, i.e., a device for wireless control of another medical device. In some embodiments, the word “device” is used interchangeably with “pump”,
30 “infusion pump” and/or “controller” and/or “Companion” and/or “remote controller device” and/or “remote controller assembly”.

A "Companion" shall mean a device for wireless control of another medical device. In the exemplary embodiments, the Companion may also include a glucose meter/ strip reader.

5 An "input" of a device includes any mechanism by which a user of the device or other operator/caregiver may control a function of the device. User inputs may include mechanical arrangements (e.g., switches, pushbuttons, jogwheel(s)), electrical arrangements (e.g., a slider, touch screen), wireless interfaces for communication with a remote controller (e.g., RF, infrared), acoustic interfaces (e.g., with speech recognition), computer network
10 interfaces (e.g., USB port), and other types of interfaces.

A "button" in the context of an input such as the so-called "bolus button" discussed below may be any type of user input capable of performing a desired function, and is not limited to a pushbutton, a slider, switch, touch screen or a jog wheel.

15

An "alarm" includes any mechanism by which an alert may be generated to a user or third party. Alarms may include audible alarms (e.g., a speaker, a buzzer, a speech generator), visual alarms (e.g., an LED, an LCD screen), tactile alarms (e.g., a vibrating element), wireless signals (e.g., a wireless transmission to a remote controller or caretaker),
20 or other mechanism. Alarms may be generated using multiple mechanisms simultaneously, concurrently, or in a sequence, including redundant mechanisms (e.g., two different audio alarms) or complementary mechanisms (e.g., an audio alarm, a tactile alarm, and a wireless alarm).

25 "Fluid" shall mean a substance, a liquid for example, that is capable of flowing through a flow line.

A "user" includes a person or animal who receives fluid from a fluid delivery device, whether as part of a medical treatment or otherwise, or a caregiver or third party
30 involved in programming the device or otherwise interacting with the device to infuse fluid to another.

"Cannula" shall mean a disposable device capable of infusing fluid to a user. A cannula as used herein may refer to a traditional cannula or to a needle.

“Disposable” refers to a part, device, portion or other that is intended to be used for a fixed duration of time, then discarded and replaced.

5 “Reusable” refers to a portion that is intended to have an open-ended duration of use.

“Acoustic volume measurement” shall mean quantitative measurement of a relevant volume using acoustical techniques such as described in U.S. Patent Nos. 5,349,852 and
10 5,641,892, as well as other techniques incorporated by reference herein.

A “temperature sensor” includes any mechanism for measuring temperature and communicating temperature information to a controller or to a pump processor. The devices described herein may include one or more temperature sensors for measuring such
15 things as including, but not limited to, one or more of the following: skin temperature, AVS temperature, ambient temperature, internal temperature and fluid temperatures.

An exemplary use of embodiments of the devices, methods and systems described here is for the delivery of insulin to people living with diabetes, but other uses include
20 delivery of any fluid, as described above. Fluids include analgesics to those in pain, chemotherapy to cancer patients and enzymes to patients with metabolic disorders. Various therapeutic fluids may include small molecules, natural products, peptide, proteins, nucleic acids, carbohydrates, nanoparticulate suspensions, and associated pharmaceutically acceptable carrier molecules. Therapeutically active molecules may be modified to improve
25 stability in the device (e.g., by pegylation of peptides or proteins). Although illustrative embodiments herein describe drug-delivery applications, embodiments may be used for other applications including liquid dispensing of reagents for high throughput analytical measurements such as lab-on-chip applications and capillary chromatography. For purposes of description below, terms “therapeutic”, “insulin” or “fluid” are used interchangeably,
30 however, in other embodiments, any fluid, as described above, may be used. Thus, the device and description included herein are not limited to use with therapeutics.

Some embodiments of the fluid delivery device are adapted for use by people living with diabetes and/or their caregivers. Thus, in these embodiments, the devices, methods

and systems work to deliver insulin which supplements or replaces the action of the person living with diabetes' (referred to as the user) pancreatic islet beta cells. Embodiments adapted for insulin delivery seek to mimic the action of the pancreas by providing both a basal level of fluid delivery as well as bolus levels of delivery. Basal levels, bolus levels and timing may be set by the user or a caregiver by using a wireless handheld user interface or directly by using a pump. Additionally, basal and/or bolus levels may be triggered or adjusted in response to the output of a glucose meter, which in the exemplary embodiments, is integral to the controller. In other embodiments, the controller additionally includes a glucose monitoring device which receives data from a blood glucose sensor. In some embodiments, a bolus may be triggered by a user using a designated button or other input means located on a device, i.e., on the controller and/or on an infusion pump. In still other embodiments, the bolus or basal may be programmed or administered through a user interface located either on the fluid delivery device/infusion pump and/or on the controller.

With respect to the names given to screens and types of screens, as well as proper names given to various features, throughout various embodiments, these terms may vary.

The systems and methods described herein may be used to control an infusion pump. For purposes of this description, the various embodiments of the user interface and the infusion pump may be described with reference to an insulin pump, or a pump which infuses insulin. However, it should be understood that the user interface may be on an infusion pump and/or on a controller. Additionally, where the description pertains to an infusion pump "screen", this "screen" may also appear on a controller, or may appear on a controller in lieu of a pump. Infusion pumps contemplated by this description include a pump which may pump any fluid, including, but not limited to, a therapeutic fluid, which includes, but is not limited to, insulin. Thus, where this description describes the exemplary embodiment as pertaining to insulin, this is meant merely for descriptive purpose only as the device is not intended to be limited to insulin. Other fluids are also contemplated.

The infusion pump may be any infusion pump, for example, but not limited to, the pump devices shown and described with respect to FIGS. 1A-1F and 2A-2D, and include, but are not limited to, those described in U.S. Publication No. US-2007-0228071, published on October 4, 2007 entitled Fluid Delivery Systems and Method; U.S. Publication No. US-2007-0219496, published on September 20, 2007 entitled Pumping Fluid Delivery Systems and Methods Using Force Application Assembly; U.S. Publication No. US-2007-0219480,

published on September 20, 2007 entitled Patch-Sized Fluid Delivery Systems and Methods; U.S. Publication No. US-2007-0219597, published on September 20, 2007 entitled Adhesive and Peripheral Systems and Methods for Medical Devices; U.S. Patent Application Serial No. 12/347,985, filed December 31, 2008 and entitled Infusion Pump
5 Assembly; U.S. Patent Application Serial No. 12/347,982, filed December 31, 2008 and entitled Wearable Pump Assembly; U.S. Patent Application Serial No. 12/347,981, filed December 31, 2008 and entitled Infusion Pump Assembly; U.S. Patent No. 7,306,578, issued on December 11, 2007 and entitled Loading Mechanism for Infusion Pump; U.S. Patent Application Serial No. 12/249,891, filed October 10, 2008 and entitled Infusion
10 Pump Assembly; U.S. Patent Application Serial No. 12/249,882, filed October 10, 2008 and entitled Infusion Pump Assembly; U.S. Patent Application Serial No. 12/249,636, filed October 10, 2008 and entitled System and Method for Administering an Infusible Fluid; U.S. Patent Application Serial No. 12/249,621, filed October 10, 2008 and entitled Occlusion Detection System and Method; U.S. Patent Application Serial No. 12/249,600,
15 filed October 10, 2008 and entitled Multi-Language/Multi-Processor Infusion Pump Assembly; U.S. Patent Application Serial No. 12/249,540, filed October 10, 2008 and entitled An Infusion Pump Assembly with a Backup Power Supply; and U.S. Patent Application Serial No. 12/249,496, filed October 10, 2008 and entitled Pump Assembly with a Removable Cover Assembly, all of which are herein incorporated by reference in
20 their entireties. In the exemplary embodiment, the infusion pump includes hardware for wireless RF communication with a controller. However, in various embodiments, the infusion pump may be any infusion pump. Referring to FIGS. 1A-1F and 2A-2D, in some exemplary embodiments, the infusion pump may include a display assembly 104, however, in other exemplary embodiments, such as those shown in FIGS. 2A-2D, the infusion pump
25 may not include a display assembly. In these embodiments, a display assembly which may be similar to the one shown in FIGS. 1A, 1D and 1F, or may be larger or smaller, is included on a controller or companion device. An embodiment of the controller or companion device is shown in FIG. 3.

Referring to FIGS. 1A-1F, an embodiment an infusion pump assembly 100 that may
30 be housed within enclosure assembly 102 is shown. Infusion pump assembly 100 may include a display system 104 that may be visible through the enclosure assembly 102. One or more switch assemblies / input devices 106, 108, 110 may be positioned about various portions of the enclosure assembly 102. The enclosure assembly 102 may include infusion port assembly 112 to which cannula assembly 114 may be releasably coupled. A removable

cover assembly 116 may allow access to a power supply cavity 118 (shown in phantom on FIG. 1D).

Referring to the infusion pump assemblies shown in FIG. 1A-1F, infusion pump assembly 100 may include processing logic (not shown) that executes one or more processes that may be required for infusion pump assembly 100 to operate properly. Processing logic may include one or more microprocessors (not shown), one or more input / output controllers (not shown), and cache memory devices (not shown). One or more data bases and/or memory buses may be used to interconnect processing logic with one or more subsystems. In some embodiments, at least one of the subsystems shown in FIG. 4 is also included in the embodiment of the infusion pump assembly 200 shown in FIGS. 2A-2D.

The various embodiment of the infusion pump shown in FIGS. 2A-2D include those described in U.S. Patent No. 5,575,310, issued November 19, 1996 and entitled Flow Control System with Volume-Measuring System Using a Resonatable Mass; and U.S. Patent No. 5,755,683, issued May 26, 1998 and entitled Cassette for Intravenous-Line Flow-Control System both of which are assigned to DEKA Products Limited Partnership, as well as U.S. Patent Application Publication No. US-2007-0228071, published on October 4, 2007 and entitled Fluid Delivery Systems and Methods; U.S. Patent Application Publication No. US-2007-0219496, published on September 20, 2007 and entitled Pumping Fluid Delivery Systems and Methods Using Force Application Assembly; U.S. Patent Application Publication No. US-2007-0219480, published on September 20, 2007 and entitled Patch-Sized Fluid Delivery Systems and Methods; U.S. Patent Application Publication No. US-2007-0219597, published on September 20, 2007 and entitled Adhesive and Peripheral Systems and Methods for Medical Devices; and U.S. Patent Application Serial No. 12/347,985, filed December 31, 2008 and entitled Infusion Pump Assembly.

Referring to FIGS. 2A-2D, infusion pump assembly 200 may include a reusable housing assembly 202. Reusable housing assembly 204 may be constructed from any suitable material, such as a hard or rigid plastic, that will resist compression. For example, use of durable materials and parts may improve quality and reduce costs by providing a reusable portion that lasts longer and is more durable, providing greater protection to components disposed therein.

Reusable housing assembly 204 may include a mechanical control assembly (not shown) having a pump assembly and at least one valve assembly. The reusable housing assembly 204 may also include an electrical control assembly configured to provide one or more control signals to the mechanical control assembly and effectuate the basal and/ or

bolus delivery of an infusible fluid to a user. Disposable housing assembly 202 may include at least one valve assembly which may be configured to control the flow of the infusible fluid through a fluid path. Reusable housing assembly 204 may also include a pump assembly which may be configured to pump the infusible fluid from the fluid path to the user.

An electrical control assembly may be housed in the reusable housing assembly 204 and may monitor and control the amount of infusible fluid that has been and/or is being pumped. For example, electrical control assembly may receive signals from a volume sensor assembly and calculate the amount of infusible fluid that has just been dispensed and determine, based upon the dosage required by the user, whether enough infusible fluid has been dispensed. If enough infusible fluid has not been dispensed, electrical control assembly may determine that more infusible fluid should be pumped. Electrical control assembly may provide the appropriate signal to mechanical control assembly so that any additional necessary dosage may be pumped or electrical control assembly may provide the appropriate signal to mechanical control assembly so that the additional dosage may be dispensed with the next dosage. Alternatively, if too much infusible fluid has been dispensed, electrical control assembly may provide the appropriate signal to mechanical control assembly so that less infusible fluid may be dispensed in the next dosage.

The mechanical control assembly may include at least one shape-memory actuator. The pump assembly and/or valve assembly of the mechanical control assembly may be actuated by at least one shape-memory actuator, e.g., shape-memory actuator, which may be a shape-memory wire in wire or spring configuration. Shape memory actuator may be operably connected to and activated by an electrical control assembly, which may control the timing and the amount of heat and/or electrical energy used to actuate mechanical control assembly. Shape memory actuator may be, for example, a conductive shape-memory alloy wire that changes shape with temperature. The temperature of shape-memory actuator may be changed with a heater, or more conveniently, by application of electrical energy. Shape memory actuator may be a shape memory wire constructed of nickel/titanium alloy, such as NITINOL™ or FLEXINOL®.

Infusion pump assembly 200 may include a volume sensor assembly configured to monitor the amount of fluid infused by infusion pump assembly. For example, the volume sensor assembly may employ, for example, acoustic volume sensing using acoustic volume measurement technology, including, but not limited to, technologies described in the following references: U.S. Patent Nos. 5,575,310 and 5,755,683 assigned to DEKA

Products Limited Partnership, as well as U.S. patent application Publication Nos. US 2007/0228071 A1, US 2007/0219496 A1, US 2007/0219480 A1, US 2007/0219597 A1, all of which are incorporated herein by reference in their entirety. Other alternative techniques for measuring fluid flow may also be used; for example, Doppler-based methods; the use of
5 Hall-effect sensors in combination with a vane or flapper valve; the use of a strain beam (for example, related to a flexible member over a fluid reservoir to sense deflection of the flexible member); the use of capacitive sensing with plates; or thermal time of flight methods. One such alternative technique is disclosed in U.S. Publication No. US-2007-0228071, published on October 4, 2007 entitled Fluid Delivery Systems and Methods, of
10 which is incorporated herein by reference in its entirety. Infusion pump assembly 200 may be configured so that the volume measurements produced by the volume sensor assembly may be used to control, through a feedback loop, the amount of infusible fluid that is infused into the user.

Infusion pump assembly 200 may further include a disposable housing assembly
15 202. For example, disposable housing assembly 202 may be configured for a single use or for use for a specified period of time, e.g., three days or any other amount of time. Disposable housing assembly 202 may be configured such that any components in infusion pump assembly 200 that come in contact with the infusible fluid are disposed on and/or within disposable housing assembly 202. For example, a fluid path or channel including a
20 reservoir, may be positioned within disposable housing assembly 202 and may be configured for a single use or for a specified number of uses before disposal. The disposable nature of disposable housing assembly 202 may improve sanitation of infusion pump assembly 200.

The disposable housing assembly 202 may be configured to releasably engage
25 reusable housing assembly 204, and includes a cavity that has a reservoir for receiving an infusible fluid (not shown), e.g., insulin. Such releasable engagement may be accomplished by a screw-on, a twist-lock or a compression fit configuration, for example. Disposable housing assembly 202 and/or reusable housing assembly 204 may include an alignment assembly configured to assist in aligning disposable housing assembly 202 and reusable
30 housing assembly 204 for engagement in a specific orientation. Similarly, base nub 206 and top nub 208 may be used as indicators of alignment and complete engagement.

Referring now to FIGS. 2A-2B, in this particular embodiment of the infusion pump assembly 200, infusion pump assembly 200 may include switch assembly 210 positioned about the periphery of infusion pump assembly 200. In other embodiments, for example,

those shown in FIGS. 2C-2D, the switch assembly 216 may be positioned elsewhere on the reusable housing assembly 204, including but not limited to, on the top surface. Referring back to FIGS. 2A-2B, in the exemplary embodiment shown, switch assembly 210 may be positioned along a radial edge of infusion pump assembly 200, which may allow for easier use by a user. Switch assembly 210 may be covered with a waterproof membrane configured to prevent the infiltration of water into infusion pump assembly 200. Reusable housing assembly 204 may include main body portion (housing the above-described mechanical and electrical control assemblies) and locking ring assembly 212 that may be configured to rotate about main body portion (in the direction of arrow 214).

In a fashion similar to reusable housing assembly 204 and disposable housing assembly 202, reusable housing assembly 204 may be configured to releasably engage disposable housing assembly 202. Such releasable engagement may be accomplished by a screw-on, a twist-lock or a compression fit configuration, for example. In an embodiment in which a twist-lock configuration is utilized, the user of infusion pump assembly 200 may first properly position reusable housing assembly 204 with respect to disposable housing assembly 202 and may then rotate locking ring assembly 212 (in the direction of arrow 214) to releasably engage reusable housing assembly 204 with disposable housing assembly 202.

Through the use of locking ring assembly 212, reusable housing assembly 204 may be properly positioned with respect to disposable housing assembly 202 and then releasably engaged by rotating locking ring assembly 212, thus eliminating the need to rotate reusable housing assembly 204 with respect to disposable housing assembly 202. Accordingly, reusable housing assembly 204 may be properly aligned with disposable housing assembly 202 prior to engagement, and such alignment may not be disturbed during the engagement process. Locking ring assembly 212 may include a latching mechanism (not shown) that may prevent the rotation of locking ring assembly 212 until reusable housing assembly 204 and disposable housing assembly 202 are properly positioned with respect to each other.

Referring now to FIGS. 1A-1F and FIG. 4, examples of the subsystems interconnected with processing logic 400 may include but are not limited to memory system 402, input system 404, display system 406, vibration system 408, audio system 410 motor assembly 416, force sensor 412, temperature sensor (not shown) and displacement detection device 418. Infusion pump assembly 100 may include primary power supply 420 (e.g. a battery) configured to be removable installable within power supply cavity 118 and to provide electrical power to at least a portion of processing logic 400 and one or more of the

subsystems (e.g., memory system 402, input system 404, display system 406, vibration system 408, audio system 410, motor assembly 416, force sensor 412, and displacement detection device 418).

Infusion pump assembly 100 may include reservoir assembly 430 configured to
5 contain infusible fluid 422. In some embodiments, reservoir assembly 430 may be a reservoir assembly similar to that described in U.S. Patent No. 7,498,563, issued March 3, 2009 and entitled Optical Displacement Sensor for Infusion Devices, which is herein incorporated by reference in its entirety, and/or as described in U.S. Patent No. 7,306,578, issued December 11, 2007 and entitled Loading Mechanism for Infusion Pump; U.S. Patent
10 Application Serial No.12/249,882, filed October 10, 2008 and entitled Infusion Pump Assembly; and U.S. Patent Application Serial No. 12/249,891, filed October 10, 2008 and entitled Infusion Pump Assembly all of which are herein incorporated by reference in their entireties. In other embodiments, the reservoir assembly may be any assembly in which fluid may be acted upon such that at least a portion of the fluid may flow out of the reservoir
15 assembly, for example, the reservoir assembly, in various embodiments, may include but is not limited to: a barrel with a plunger, a cassette or a container at least partially constructed of a flexible membrane.

Plunger assembly 424 may be configured to displace infusible fluid 422 from reservoir assembly 430 through cannula assembly 450 (which may be coupled to infusion
20 pump assembly 100 via infusion port assembly 424) so that infusible fluid 422 may be delivered to user 454. In this particular embodiment, plunger assembly 424 is shown to be displaceable by partial nut assembly 426, which may engage lead screw assembly 428 that may be rotatable by motor assembly 416 in response to signals received from processing logic 400. In this particular embodiment, the combination of motor assembly 416, plunger
25 assembly 424, partial nut assembly 426, and lead screw assembly 428 may form a pump assembly that effectuates the dispensing of infusible fluid 422 contained within reservoir assembly 430. An example of partial nut assembly 426 may include but is not limited to a nut assembly that is configured to wrap around lead screw assembly 426 by e.g., 30 degrees. In some embodiments, the pump assembly may be similar to one described in U.S. Patent
30 No. 7,306,578, issued December 11, 2007 and entitled Loading Mechanism for Infusion Pump; U.S. Patent Application Serial No.12/249,882, filed October 10, 2008 and entitled Infusion Pump Assembly; and U.S. Patent Application Serial No. 12/249,891, filed October 10, 2008 and entitled Infusion Pump Assembly all of which are herein incorporated by reference in their entireties.

USER INTERFACE

Throughout this description, screens may be referenced with respect to the “pump” or “Companion” or “Controller”. However, in various embodiments, a similar screen or a similar method may be accomplished on another device. For example, where the screen or method is referenced with respect to the “pump”, a similarly functional screen or method may be used on the “Companion” in other embodiments. As this description includes embodiments related to both pumps having displays and pumps having no displays, it should be evident that where the embodiment includes an infusion pump without a display, any screens will be visible on a Companion. Similarly, where a method requires an interaction between the user and the pump, the interaction may be accomplished via a switch assembly on the pump where the pump is an infusion pump without a display.

Processing logic which in some embodiments, includes at least one element as shown in described with respect to FIG. 4, is used to receive inputs from a user or caregiver. The user or caregiver uses one or more input devices or assemblies, including but not limited to, one or more of the following: button / switch assembly, slider (for example, including but not limited to any slider described in U.S. Publication No. US-2008-0177900, published July 24, 2008 and entitled Medical Device Including a Slider Assembly, which is herein incorporated by reference in its entirety), jog wheel or touch screen. The infusion device additionally received inputs from internal systems, including but not limited to occlusion detection process 438, confirmation process 440, volume measurement technology (e.g., acoustic volume sensing). Using these inputs, the infusion device produces outputs, for example including, but not limited to, infusion fluid delivery to the user or comments, alerts, alarms or warnings to the user. The inputs are thus either directly from the user to the pump, directly from the pump systems to the processing logic, or from another device, e.g., a remote controller device (described in more detail below), to the pump. The user or caregiver interaction experience thus includes, but is not limited to, one or more of the following: interaction with a display (either on the infusion pump device itself or a remote controller device or both), which includes but is not limited to, reading/seeing text and/or graphics on a display, direct interaction with a display, for example, through a touch screen, interaction with one or more buttons, sliders, jog wheels, one or more glucose strip readers, and sensing either through touch sensation or audio, one or more vibration motors, and/or an audio system. Thus, the term “user interface” is used to encompass all of the systems and methods a user or caregiver interacts with the infusion pump, to control the infusion pump.

Referring now to FIG. 3, in some embodiments of the infusion pump system, the infusion pump may be remotely controlled using a remote controller assembly 300, also referred to as a controller or a companion. Remote control assembly 300 may include all, or a portion of, the functionality of the infusion pump assembly shown in FIGS. 1A-1F, itself.

5 Thus, in some exemplary embodiments of the above-described infusion pump assembly, the infusion pump assembly (not shown, see FIGS. 1A-1F, amongst other FIGS.) may be configured via remote control assembly 300. In these particular embodiments, the infusion pump assembly may include telemetry circuitry (not shown) that allows for communication (e.g., wired or wireless) between the infusion pump assembly and e.g., remote control

10 assembly 300, thus allowing remote control assembly 300 to remotely control infusion pump assembly 100. Remote control assembly 300 (which may also include telemetry circuitry (not shown) and may be capable of communicating with infusion pump assembly) may include display assembly 302 and an input assembly, which may include one or more of the following: an input control device (such as jog wheel 306, slider assembly 310, or

15 another conventional mode for input into a device), and switch assemblies 304, 308. Thus, although remote control assembly 300 as shown in FIG. 3 includes jog wheel 306 and slider assembly 310, some embodiments may include only one of either jog wheel 306 or slider assembly 310, or another conventional mode for input into a device. In embodiments having jog wheel 306, jog wheel 306 may include a wheel, ring, knob, or the like, that may

20 be coupled to a rotary encoder, or other rotary transducer, for providing a control signal based upon, at least in part, movement of the wheel, ring, knob, or the like.

Remote control assembly 300 may include the ability to pre-program basal rates, bolus alarms, delivery limitations, and allow the user to view history and to establish user preferences. Remote control assembly 300 may also include a glucose strip reader 312.

25 During use, remote control assembly 300 may provide instructions to the infusion pump assembly via a wireless communication channel established between remote control assembly 300 and the infusion pump assembly. Accordingly, the user may use remote control assembly 300 to program / configure the infusion pump assembly. Some or all of the communication between remote control assembly 300 and the infusion pump assembly

30 may be encrypted to provide an enhanced level of security.

In the exemplary embodiments of the user interface, the user interface requires user confirmation and user input. The exemplary embodiments of the user interface are centered on ensuring the user knows the effect of various interactions on the pump. Many examples will be presented throughout this description of the pump communicating the result of the

user's actions to the user. These features ensure the user understands their actions and therefore, imparts greater safety onto the user. One such example is throughout the exemplary embodiment of the user interface, where the user presses the back button on a screen after a value has been changed, the user interface displays the Cancel Changes
5 confirmation screen, as shown in FIG. 6. If the user selects "Yes", the user interface discards any pending changes, closes the confirmation screen and goes back to the previous screen (i.e., the screen previous to the screen where the user pressed the Back button). When the action selection is "No", on the "Cancel Changes?" confirmation screen, the user presses the enter button or other depending on the embodiment, and the user interface closes
10 the confirmation screen and returns to the screen with pending changes. This feature prevents the outcome where the user assumes the changes have been implemented, but in fact, they have not been. Thus, this feature prevents that circumstance and ensures the user understands that the changes have not been implemented.

15 **Power Up**

Generally, an infusion pump is used for therapy by a user almost continuously, with some exceptions. Thus, from the time an infusion pump is "powered up", i.e., a battery is inserted into the pump and the pump is "Setup" for use for therapy, the infusion pump remains on and in many cases, connected to the user by way of a cannula. Oftentimes, a
20 user will "disconnect", i.e., disrupt the fluid connection of the tubing to the cannula, for short and predicted periods of time. For example, users often disconnect while changing the cannula, changing the infusion set, changing the reservoir, priming the tubing, bathing/showering, undergoing tests such as an MRI, or otherwise being exposed to harmful forces, for example, electromagnetic forces, or, in some circumstances, while exercising or
25 being exposed to potentially corrosive water, for example, salt water. There are many additional circumstances where users may disconnect. However, generally, these disconnection events are planned and the user understands they will not receive therapy from the infusion pump while disconnected from the pump.

Thus, once infusion pump therapy has begun with a given pump, the user will
30 remain connected and will likely receive their therapy from the infusion pump until and unless the infusion pump is replaced by another form of therapy, for example, another pump or multiple daily injections.

The power up user interface is visible when a battery is inserted into the infusion pump. If the infusion pump has been in use by the user prior to the battery change, then the

pump will initialize. If the pump had not been previously used by the user (i.e., the pump is new to the user), on first use of the pump, the user interface automatically guides the user through programmable settings that must be initialized before insulin delivery or other fluid therapeutic delivery may occur.

5 Referring now to FIG. 5A, after the initialization period, the user interface advances to Time and Date Wizard, which takes the user through the TIME/DATE, SET TIME and SET DATE screens, and then advances to the Home screen (as also discussed with respect to FIGS. 10A-10E). As shown in FIG. 5A, if a valid time is detected, the default selection for the user is "next" on the TIME/DATE screen **500**, wherein the user interface proceeds to
10 an initializing screen **502** then to the Home Screen **504**.

However, referring now to FIGS. 5B-5C, if the system does not detect a valid time and date, the Time and Date Wizard shall display the TIME/DATE screen with the Time values set to dashes (--) to indicate that no values are currently set. The Date value is not displayed until a valid time has been set.

15 Amongst other advantages, where the system detects a valid TIME/DATE, the Time and Date Wizard automatically fills the TIME/DATE with the detected valid TIME/DATE. However, the system still ensures that the user reviews the detected TIME/DATE and presents an opportunity for the user to change the TIME/DATE if the TIME/DATE on the screen is incorrect. In fact, in the exemplary embodiment shown, the system will not
20 complete initializing and will not advance to the Home Screen until the user has selected "next", i.e., affirming the TIME/DATE is acceptable.

Conversely, where an invalid date is detected, the system does not automatically fill the TIME/DATE but rather requires the user to do so. Thus, the user interface system, in the exemplary embodiment, requires the user to always review the TIME/DATE.

25 Some embodiments of the user interface include a Trainer Mode. This mode is generally used when a user or caregiver is initially using the pump and thus may take additional time to review and enter information into the user interface. The Trainer Mode allows for the user to select a duration that the user interface will disable timeouts. In normal mode, the user interface otherwise includes timeouts as a power conservation
30 measure, where the screen will timeout at a preset interval of user inactivity. However, in this embodiment, the timeouts are disabled. In the exemplary embodiment, when the Trainer Mode is initialized, a "duration" is set by the user or caregiver, for example, 2 hours, and during this duration, timeouts are disabled.

User Setup

User Setup includes many features to the user and those used by the pump for therapy. These include but are not limited to setting the: pairing with a companion, time, date, time/date format, time format, glucose units (mg/dL vs. mmol/L), language, blood glucose targets by time of day, basal rate by time of day or preprogrammed title, insulin
5 type, duration of action of insulin, cursor preference, magnify preference, bolus button, bolus and basal limits, "1 U Drop" (one unit drop), display/button side, carbohydrate to insulin ratio, alarm features including alarm types where options exist, sensitivity to occlusion, inactivity alarm, therapy lockouts, care comments and reminders.

As discussed above, in the exemplary embodiments, the infusion pump system
10 includes a controller or companion device, for example, similar to one described above. In these embodiments, at Power Up, if the pump is not currently paired and not fully initialized the user is first prompted to pair the pump with a remote control device, i.e., a controller or Companion, as discussed above. The user may choose to skip this option, for example, where the user does not desire to pair with a companion device. In this case, the user
15 interface advances the user to other Setup screens.

Referring to FIG. 7A, if the user chooses to initiate the pairing (by selecting OK); the user interface displays the PUMP Searching for Companions screen (it should be noted that where the pump is an embodiment that does not include a display, the Companion will be the only screens during the pairing process. Thus, similar screens will appear on the
20 Companion only). The remote Companion must be in pairing mode for the pairing to be completed. Thus, for pairing an infusion pump with a Companion, both devices must be in pairing mode. This feature serves as one of many safety features during the pairing process. Requiring both devices to be in pairing mode ensures an infusion pump is not "hijacked" by a non-intended Companion. If the pairing fails or is cancelled, when the user selects OK on
25 the Pairing Failed or Pairing Cancelled warning screen, the user interface displaces the STEP 1 screen on the Setup Wizard and sets the Radio setting to "Off". Thus, where the system is not paired, the pump user interface automatically turns the radio off and proceeds to continue Setup Wizard.

Referring now to FIG. 7B, to pair a pump and Companion device for remote
30 communications, the pairing process requires user interaction on both the pump and Companion. In the exemplary embodiment, the user interface displays the PUMP "Searching for Companions" screen on the pump when the user selects and accepts the "PAIR DEVICE" item on the "SETUP" screen. The user selects the "PAIR DEVICE" item to initiate the pairing process with and begin searching for a remote control Companion

device in pairing mode. On the Companion, the user selects "PAIR PUMP" on the "SETUP" screen, then selects the "Yes" action selection on the "Is pump ready?" confirmation screen. Before selecting "Yes", the user needs to start the search on the pump. Thus, in pairing mode, both the infusion pump and the Companion must be in pairing mode, simultaneously, for the pairing mode to commence.

When the user selects the "PAIR DEVICE" item on the pump "SETUP" screen and presses the enter button, the user interface: 1) turns on the radio if it is turned off; 2) initiates a search for Companion devices that are in pairing mode (where pairing has been initiated on the Companion); and 3) displays the "Searching for Companions" pairing screen.

Referring now to FIG. 7C, the user interface displays the PUMP "Found Companion {Companion Serial #}" screen on the pump following the PUMP "Searching for Companions" screen, when a Companion in pairing mode has been found. The serial number of the Companion is displayed on the screen in place of the "{Companion Serial #}". This screen indicates a Companion in pairing mode has been found, but the pairing has not been completed. The user must confirm the pairing on the Companion device for the pairing process to be complete. This feature ensures the user has an opportunity to confirm that the pump found is indeed the pump in which the user intends to pair with the Companion device.

The user interface displays "No Companions Found" warning screen on the pump when the user initiated pairing, and the search for Companions in pairing mode failed after searching for approximately 1 minute. In other embodiments, the amount of searching time may vary. The pump user interface, in the exemplary embodiment, turns off the radio and warns the user when no Companions were found after searching for Companions for a defined time period without button press interruptions (See FIG. 7D). This ensures that where pairing mode has commenced on one side, for example, on the Companion but not the pump, a timeout period will end the pairing mode.

Referring to FIG. 7E, the user interface displays the PUMP "Paired with {Companion Serial #}" screen on the pump when the pairing has been confirmed on the Companion device. In the exemplary embodiment, the user interface displays an indication to the user of the Companion device serial number to which a pump is paired when a pump and Companion have been successfully paired. This feature allows the user opportunity to confirm the Companion serial number indicates the intended Companion is paired with the pump.

Once the "Done" is selected, where the pump is fully initialized, the pump will proceed to the Home screen. Where the pump is not fully initialized, the user interface will display the Setup Wizard Step 1 screen.

Although the above embodiments are described with reference to the PUMP screens, similar screens are displayed on the Companion throughout the pairing process.

During pairing, the user interface displays the "Pairing cancelled" warning screen on either the pump or the Companion device, when the user presses a button on the pump while displaying the PUMP "Searching for Companion" screen, or on the Companion while displaying the COMPANION "Searching for Pumps" screen. If the pump or Companion were paired before attempting to pair them again, and the user cancelled the pairing, the existing pairing is not lost.

Pairing may be cancelled where the user presses a button on the pump or the Companion while the "Searching for ..." screen is displayed. Referring now to FIG. 7F, the user interface displays an indication to the user that the pairing process was cancelled before the pump and Companion were successfully pairing. Thus, the user will be aware that the pump and Companion may not be paired (in the exemplary embodiment, if the pump and Companion were paired, a screen or audio signal will indicate same).

In the exemplary embodiment, the user interface displays the "Incompatible pump found. Pairing failed" WARNING screen on the Companion during the pairing process, when a pump in pairing mode is found that has a serial number that indicates different glucose units than the units configured on the Companion (i.e., mg/dL vs. mmol/L). As a safety feature, the user interface considers a pump and Companion with different glucose units incompatible and disallows pairing the two devices. When the user attempts to pair the pump and Companion with different glucose units, any previous pairing is lost.

Either after pairing is completed or once pairing has been skipped, the user completes the "Setup Wizard", setting various features of the user interface.

As discussed above with respect to FIGS. 5B-5C, because the infusion pump delivers insulin (or another fluid) based on time of day (in the exemplary embodiment, however, in other embodiments, the pump may deliver based on another criteria, for example, every "2 hours", or "once daily"), it is important that the time settings are accurate. Also, in the exemplary embodiment, the pump device logs a history of insulin (or other fluid) delivery. Therefore, it is important that the date settings are accurate. When the user first initializes the pump, or when the system does not detect a valid time, the Current Time settings have no default values, and the user interface requires the user to set the

current time. Additionally, when the user changes the battery in the pump, the user interface requires the user to review the settings for the current time to ensure that they are accurate.

After the user has set a valid time, the time is continuously updated by the device's real-time clock. After the device has fully initialized, the user may change the current time by entering either the Setup Wizard or the Time and Date Wizard through the SETUP screen.

If the user changes the time and/or date on the pump and then accesses the user interface on the Companion device, the time and date on the Companion is synchronized with the pump's time and date, and a warning screen is displayed on the Companion to indicate the time on the Companion has been changed to the pump time.

When the user first initializes the pump, or when the system does not detect a valid date, the Current Date settings have no default values, and the user interface requires the user to set the current date. Additionally, when the user changes the battery in the pump, the user interface requires the user to review the settings for the current date to ensure that they are accurate.

After the user has set a legal date value, the date is maintained and updated by the pump's real-time clock. If the user enters a non-legal date, then the pump will indicate same with an audio and/or visual indication that the date is not accepted. After the device has fully initialized, the user may change the current date by entering either the Setup Wizard or the Time and Date Wizard through the SETUP screen.

The user interface includes a preprogrammed list of "legal dates". These may be based on the Gregorian calendar, or within any other pre-definable parameters. These may include, for example, but not limited to, the number of days for particular months, the years in which a date of Feb 29 is a legal date. In the exemplary embodiment, the user interface may only allow these parameters to be changed at a system level, i.e., not by the user. However, in other embodiments, the user interface may allow the user to change the parameters.

In the exemplary embodiment of the pump, as discussed above, the pump is an insulin pump. The insulin concentration value (Units/mL) is preprogrammed to be "U100" and cannot be changed by the user. This is a safety measure, as generally, a user on insulin therapy uses U100 insulin. However, in various embodiments where either a different insulin therapy is contemplated, or, if a different fluid is infused, this feature may require user input to specify the concentration of the fluid.

Related settings that the user may specify include the insulin type and action time. The user interface uses these settings to determine the amount of Insulin on Board or "IOB". IOB refers to a number which serves as a gauge to the "action" of the insulin currently in the user. The gauge is comparing the action available to a quantitative "amount
5 of insulin" currently in the user. Thus, as the Action Time and Insulin Type are used to calculate IOB, which is used, as described later, in bolus calculations, it is critical this information be entered.

When the pump is fully initialized, the user may change the insulin settings by entering the Setup Wizard through the SETUP screen, or by selecting INSULIN on the
10 SETUP screen. Referring to FIG. 8A, the exemplary embodiment of these screens are shown.

Referring now to FIG. 8B, the user interface opens the SET TYPE edit item screen when the user accepts the Type item on the Insulin Profile select item for edit screen, and Magnify is set to On. "Magnify" refers to an option in the exemplary embodiment of the
15 user interface, where the user may prefer that the text in the curser and in various screens, be "magnified" so as to be better visible. Various embodiments of this feature may be used in the user interface, including those described in pending U.S. Publication No. US-2008-0177900, published July 24, 2008 and entitled Medical Device Including a Slider Assembly, which is herein incorporated by reference in its entirety.

When Magnify is "Off", or when the user accesses the screen on the Companion
20 device, the user interface opens the Type item for editing. The Type value identifies the type of insulin being used. Two options are available in the exemplary embodiment, either Rapid or Short. In various other embodiments, additional options may be pre-programmable and selectable options.

The exemplary embodiment of the user interface includes various safety features related to the INSULIN PROFILE screens. For example, when the Type item on the INSULIN PROFILE screen is open for editing and the user presses a soft-key button for "Next" or "Done" action selection, the user interface will either: 1) accept and close the selected value; or if the user changed the Type value, the user interface will change the
25 Action Time value to dashes and display a warning message in language dependant text: "Dashed items must be set". This is to prompt the user that an Action Value must be entered; or, 3) if the user did not change the Type value, select the action selection, save any
30 pending changes and advance to the next screen.

Referring to FIGS. 9A-9B, in the exemplary embodiment of the user interface, the user may configure display settings for the pump to have the user interface screens oriented such that the enter and back buttons, for example, are either on the right side of the LCD display, or the left side. Additionally, the device uses screen timeouts to conserve energy
5 by turning off the display and entering into a low-power sleep state when the user has stopped interacting with the device within a period of time. The user configures this timeout value as part of the display settings. Screen timeouts are not in effect until after the pump is fully initialized.

Another display setting that the user may configure is the whether to display an
10 activity-based home screen or an information-based home screen. The Home screen is further described below with reference to FIGS. 10A-10E. In the exemplary embodiment, the user interface allows the user to access the display settings for the pump through the Setup Wizard STEP 2 screen, by advancing the DISPLAY screen. The display settings that also apply to the Companion are accessible on the Companion by selecting REFERENCES
15 on the SETUP screen.

Referring to FIG. 9A, the user interface allows the user to set a duration value for the timeout feature of the display. Additionally, the user may select the home screen feature using the DISPLAY screens.

Referring now to FIG. 9B, the user interface includes a feature which allows the user
20 to configure the display orientation of the user interface screen on the pump as it relates to the position of the buttons (i.e., referring to FIG. 1A, the switch assemblies 108). For example, the user interface allows the user to designate whether the buttons are on the left of the display, or the right. In the exemplary embodiment, the user interface may have a default setting, for example, buttons on right or buttons on left.

Referring now to FIG. 9A, the user interface opens the SET BUTTONS edit item
25 screen when the user accepts the Buttons item on the DISPLAY select item for edit screen, and the user-programmable settings for Magnify is set to "On". When Magnify is "Off", or when the user accesses the screen on the Companion device, in the exemplary embodiment, the user interface opens the Buttons item for editing. The user accept the Buttons item to
30 configure the device to orient the user interface screens such that the buttons are either on the right of the LCD display, or on the left. An exemplary embodiment of the BUTTON screens are shown in FIG. 9B.

The ability of the user to set the side of the buttons allows the user to customize the pump to their preferred hand. Thus, this is an advantage for ease of use to the user.

Additionally, in some embodiments of the infusion pump, as shown in FIGS. 1A-1F, where a slider 106 may be used as input device, the ability of the user to set the user interface such that they are free to use their preferred hand in all inputs is an advantage and may allow the user to be more efficient and safe in the handling of inputs to the pump.

5 In the exemplary embodiment, the user interface includes a bolus calculator. The user must provide particular input information regarding their therapy into the user interface while using the bolus calculator option. However, in some cases, the user may choose to enter this information in advance through Setup screens. The information entered in advance may then be used in any calculators requiring this information. However, the
10 information may be entered at the time of the use of the calculator.

The information used by the calculator is typically based on a user's medical team's recommendation. The bolus calculator requires this information. In addition to the INSULIN screens discussed above, the user may also enter information regarding "1U DROP", carbohydrate ratios and Blood Glucose targets.

15 Referring now to FIGS. 11A-11B, various 1U DROP screens are shown according to an exemplary embodiment. In the exemplary embodiment, the user may set from 1 to 24 1U DROP values based on the time of day. In addition, the user may set from 1 to 24 insulin to carbohydrate ratios (i.e., I:CHO) based on the time of day. However, in various other embodiments, the user may set more than 24 1U DROP values (and/or I:CHO values),
20 and may also specify the day of the month or the day of the week, amongst many additional factors that may be specified. The 1U DROP values are known insulin sensitivity values (i.e., how much insulin causes how much change) for the user. The I:CHO value defines the default ratio of carbohydrate grams to 1 Unit of insulin for a specified time period. The 1U DROP value is used to calculate how much insulin the pump may recommend the user
25 deliver to bring the user's blood glucose value to a desired level. The 1U DROP values may be programmed on the hour. In some instances, the 1U DROP value may not have been previously set by the user. In these cases, while using the bolus calculator option, the user may specify the 1U DROP value when programming a correction bolus.

In the exemplary embodiment, and as may be seen in FIGS. 11A-11B, the user
30 interface may allow the user to program 1 to 24 correction factor values, based on the time of day, that estimates how much change to a user's blood glucose level is effected by 1 unit of insulin.

The I:CHO value may be used in bolus calculations where the user enters an amount of carbohydrates and the bolus calculator suggests an insulin dosage. Further, the I:CHO may be used during a correction and food bolus calculation.

In the exemplary embodiment of the user interface, the user interface allows the user to define the Increment of insulin Units that will be used for each click of the slider when delivering either a normal bolus or an extended bolus through the user interface bolus screens. Additionally, in the exemplary embodiment, the user interface allows the user to define the Increment of insulin Units that will be used for each click of the slider when setting or editing a Rate value for a Basal program. In various embodiments, in addition to the slider, the Increment may be used to define the Increment of insulin Units used for each press of a button or each step movement of a jog wheel, for example. However, the Increment function may be used in various embodiments to apply to any input device or assembly desired.

The Increment item allows the user to customize the user interface for their general therapy needs. For example, the user interface may allow the user to select an increment of "0.10U", "0.05U", or "1.00U" for example. Thus, a user having a therapy that typically includes bolus or basal program amounts of "0.30U" may select the "0.10U" Increment, whereas a user having a therapy that typically includes bolus or basal program amounts of "10.0U" may select the "1.00U" Increment. Thus, this allows for more efficient use by the user in delivering their therapy.

The user interface includes an option for SET TEMP, i.e., setting a temporary basal. In the exemplary embodiment, the SET TEMP option includes the option of the user setting or configuring the temporary basal amount in terms of delivery rate (i.e., Units/hour), or in terms of a percentage of the active basal program rate. Thus, in the exemplary embodiment a user may define the temporary basal rate or may request a temporary basal reduction, based on the current basal program.

Referring now to FIG. 12, the user interface additionally includes, in the exemplary embodiment, a LOCKED ITEMS settings feature which allows the user to lock or unlock certain features of the device to restrict access to those features. These features include, but may not be limited to:

- 1) the basal menu features that allow the user to activate an existing basal program, start temporary bases, edit, delete or rename an existing basal program;

- 2) the bolus features that allow the user to deliver one-button, normal, extended, and dual boluses;
- 3) the prime feature allowing the user to prime the pump.

Thus, in the exemplary embodiment, the user interface allows flexibility by allowing the user to lockout features separately, rather than either locking the whole pump, or unlocking the whole pump. This feature may be advantageous with respect to child users or other users that may not be capable of making therapy decision, but may, when necessary, need access to priming or basal changes.

In the exemplary embodiment, the user interface includes various features that inform the user when various screens are exited or information is missing. These features ensure the user knows the impact of their actions. For example, referring now to FIG. 13A, in the exemplary embodiment, when initializing the device settings, the user must set values for any default settings that have no initial value, i.e., in the exemplary embodiment, those settings displayed as dashes, before advancing to the next screen. The user interface displays the Warning screen "Dashed items must be set" when the user fails to complete these settings. In particular, in the exemplary embodiment, this Warning screen will appear where the user:

- 1) when initializing device setting values through the Setup Wizard and the user presses the back button the STEP 1 screen;
- 2) when programming a temporary basal or a bolus, when any items are set to dashes on the screen and the user accepts the "Activate" or "Deliver" action selection;
- 3) when initializing device setting values in the Setup Wizard for the following when the user accepts the "Next", "Accept" or "Done" action selection:
 - The TIME/DATE screen when either a time or date has not been set.
 - The CURRENT TIME screen when all fields of the time value have not been set .
 - The CURRENT DATE screen when all fields of the date value have not been set.
 - The INSULIN PROFILE screen when a value has not been set for the Time item.
 - The CARB RATIOS BLOCK n screen when a value has not been set for one or more items.

- The IU DROP BLOCK n screen when a value has not been set for one or more items.
- The BG TARGET BLOCK n screen when a value has not been set for one or more items.
- 5 - The DAILY basal program BLOCK n screen when a value has not been set for one or more items.

Referring now to FIG. 13B, while the device is in a delivery mode, the user interface, in the exemplary embodiment, prevents the user from changing certain settings. For example, when the user selects and accepts the BASAL LIMITS or WIZARD item on the SETUP screen, if the basal is currently running, the user interface displays the warning "Stop delivery before using this function". Additionally, when the user selects either the Time or the Date values on the TIME/DATE screen when basal delivery is in progress, the user interface will display this Warning. This is a safety feature in the exemplary embodiment of the user interface. Where a user change or edit may cause confusion during delivery, for example, a rate change of a basal profile while that basal profile is delivering, or changing the TIME/DATE while in delivery, the user interface may use the Warning screen shown in FIG. 13B. In the exemplary embodiments, additional features may not be changed during delivery. These include but are not limited to lockout features.

Referring now to FIG. 14A, in embodiments where a pump and Companion are paired, there are various changes that, made on the Companion, may not be accepted by the pump. For example, when the user sets the time and date through the Companion-specific time/date screen, if the Companion is paired with the pump and the pump is delivering basal, in the exemplary embodiment, the pump cannot accept a new time, and the Companion displays the warning "Time and date cannot be saved on pump". Once the pump and Companion are communicating, upon background synchronization, the pump time will be sent to the Companion, and the Companion will display the warning "Companion time changed to pump time". This warning screen may be used in many different like scenarios to inform the user both that their requested changes have not been made, and when the change has been made. Thus, the user is informed of the outcome of their actions and thus is regularly aware of the impact on the pump.

Referring now to FIG. 14B, in the exemplary embodiment, the user interface may display a warning on the Companion when the user exits the Companion PREFERENCES screen, and the pump is either busy or communication with the pump is down. Thus, the

user is aware that their preferences have not been saved onto the pump, and thus, know that they should re-enter those preferences at a time when communications are restored.

Referring now to FIG. 15, in the exemplary embodiment, the Companion may be configured to enable a temporary lockout from certain functions, for example, functions that affect starting and stopping delivery on the pump. However, additional functions may also be locked out temporarily in some embodiments. The THERAPY LOCKOUT settings screen, shown in FIG. 15, allows the user to turn the lockout on, and to specify a duration for the lockout to be in effect. If the user chooses a duration of "Once", the lockout is in effect until the user selects Unlock on the THERAPY LOCKOUT Unlock screen.

Referring now to FIG. 16, the user interface allows a user to turn the radio off when the pump is paired with a Companion. Changing the setting on the pump turns off the radio only on the pump; similarly, changing the setting on the Companion turns off the radio only on the Companion. This feature allows a user to turn the radio off in cases where radio communication when desired, for example, when radio communication between devices is not advisable, allowed or safe.

Home screen

Referring now to FIGS. 10A-10E, in the exemplary embodiment, the user interface opens the SET HOME edit item screen when the user accepts the Home item on the DISPLAY select item for edit screen, and the user-programmable setting for Magnify is set to "On". When Magnify is "Off", or when the user accesses the screen on the Companion device, the user interface opens the Home item for editing. The user accepts the Home item to specify the content of the Home screen as either information-based or activity-based.

The Home screen provides access to device features and displays information about the status of the pump and the delivery. The Home screen may be configured to display an activity-based menu (i.e., Activity-Based home screen), or to display information about the current delivery status and last bolus information (i.e., Information-Based Home screen). The Home screen is configured through the PREFERENCES option on the SETUP screen.

Still referring to FIGS. 10A-10E, in the exemplary embodiment, for both the Information-Based and Activity-Based Home screens, the user interface displays the current time as maintained by the device's real-time clock, icons that provide an indication of the remaining battery capacity and insulin volume (or reservoir volume), and the amount of IOB. In some instances, a greater-than or equal to symbol may be displayed next to the IOB label. Specifically, if the bolus log contains a corrupt record, or if the time has been lost and needs to be set at powerup, the bolus log is reinitialized. However, simply replacing the

battery does not erase the bolus log when there is a valid time and date at powerup. Thus, the IOB is not lost due to a battery being replaced and in the exemplary embodiment, on the Activity-Based Home screen is indicated to the user each instance the pump display is shown. This feature in the exemplary embodiment imparts to the user clearly and efficiently the amount of IOB such that the user may use this information in their therapy. Additionally, as the IOB is not lost when the battery is replaced, the user may rely on bolus calculators and other indications on the display by the user interface, for their therapy, without interruption. However, in some embodiments, the IOB may timeout in certain situations, for example, where the pump determines that power was lost for more than a threshold time or if the pump is unable to determine the date and time, or the amount of time in which the pump did not have power. Thus, a correct or true determination of the IOB may not be possible in these circumstances. However, in the exemplary embodiment of the infusion pump, the safety processor maintains the date and time of the devices. Thus, IOB recovery is possible because of the internal clock.

15 Additionally, in the exemplary embodiment, the IOB may also be recovered after a reservoir change.

 Still referring to FIGS. 10A-10E, in the exemplary embodiment, when the magnify setting is "Off" on the pump, the cursor type on the Information-based Home screen always is displayed as Highlight regardless of the Cursor setting. This allows for the screen selection to always be distinguishable.

 In the exemplary embodiment, when delivering an extended bolus, the bolus section of the Information-Based Home screen displays the details of the running extended bolus, including the amount that has been delivered, the full programmed amount, and how much time has elapsed since the start of the extended bolus. If an extended bolus is stopped before any of the extended bolus insulin has been delivered, the Last Bolus information on the Home screen may be updated to reflect the previous bolus that delivered greater than 0.0U. However, in the exemplary embodiment, where the user power cycles the pump (i.e., the power supply is removed and replaced, this may occur when the user is changing the battery, i.e., removing the first power supply and replacing the first power supply with a second power supply, or removing the first power supply and replacing it back into the pump), and an extended bolus that was stopped before any insulin was delivered is the last bolus in the history, the Last Bolus details on the Home screen reflect that extended bolus.

 Additionally, in the exemplary embodiment, the user interface displays the last bolus details on the Information-Based Home screen as follows:

- 1) The last non-zero bolus is displayed in the history if that bolus occurred after the most recent power cycle. If there are no boluses in the history other than a zero extended bolus, the user interface with display "None".
- 2) The most recent bolus in the history is displayed which may be an extended
5 bolus of 0.0U, if a power cycle occurred more recently than the last bolus.
- 3) If there are no boluses in the history, the user interface displays "None".

Thus, in the exemplary embodiment, the user interface provides quick access to starting and stopping basal delivery, starting a temporary basal, and switching basal
10 programs on the Information-Based Home Screen. Additionally, using the Information-Based Home screen, the user the user interface provides quick access to bolus features (when in delivery mode). Also, the user interface displays may display a greater-than or equal to symbol to the right of the IOB label on the Home screen when any of the following are true:

- 15 1) The Bolus date for the entire action time period is not available;
- 2) More than a predefined number, e.g., 10, boluses were given within the action time;
- 3) There is no bolus history, and less time than the duration specified by the user-programmable action time has passed since the bolus log was initialized;
- 20 4) The IOB amount is great than a predefined number, e.g., 300.

Thus, in the exemplary embodiment, the user interface provides information regarding IOB where that information is safe to provide within a predetermined threshold. That is, the user interface ensures the user has access only to information on which may be
25 correct and safe for the user to base therapy decisions.

Alert and Recoverable Alarm Notification

For purposes of the current description and in the exemplary embodiments described herein, notifications include alarms, alerts and reminders. Alarms are either recoverable or non-recoverable. Alerts, reminders and recoverable alarms notify the user of conditions that
30 may affect normal operation of the pump that the user may need to address. For alerts, the user generally has some period of time in which to address the condition; whereas recoverable alarms stop delivery and should be addressed as soon as possible.

Non-recoverable alarms may also be referred to herein as system alarms. For recoverable alarms, the user may physically correct the problem (i.e., change the battery,

replace the reservoir, etc.), and through the features of the user interface, the pump may resume delivery. System alarms are no recoverable via the user interface. System alarms stop all processes, including delivery, and render the user interface unusable.

When the user interface is displaying a screen other than the Home screen, or when
5 a normal bolus or device prime is in progress, in the exemplary embodiments, alert and alarm notifications generated on the pump are suspended. If a normal bolus or device prime is in progress, the user interface presents the notification after the prime or normal bolus completes or is stopped, either by the user, or in the case of a recoverable alarm, the alarm condition itself stops delivery. If the user interface is displaying a screen other than the
10 Home screen, the notification is suspended until the user interface transitions to the Home screen. When a recoverable alarm that stops delivery is suspended, the user interface suspends just the notification; the delivery is stopped as soon as the alarm condition is detected.

In the exemplary embodiment, when more than one notification is pending, the
15 notifications are presented in order of priority. Also, in the exemplary embodiment, where a Companion is used with an infusion pump, all of the alerts, alarms, and reminder screen described herein are generated on the pump. If an alert or recoverable alarm condition occurs when the user interface is displaying the Home screen, the user interface produces the attention sequence on the pump and displays a notification screen that described the
20 condition. If the pump is asleep, it wakes up to display the notification. If the pump is not fully configured, notifications are suspended on the pump and are not sent to the Companion. When the Companion is awake and displaying the Home screen, if there is a notification being displayed on the pump, the notification also is displayed on the Companion. The user may silence the notification on either the pump or the Companion.

25 In the exemplary embodiment, when the Companion is displaying a screen other than the Home screen and the Companion receives a notification from the pump, the Companion displays a flashing notification bar at the top of the screen that indicates there is a pending notification. When the user interface returns to the Home screen, if the user has not already silenced the notification on the pump, the notification is displayed on the
30 Companion.

Alert and recoverable alarm notifications are accompanied by audio or vibratory feedback on the pump, referred to herein as the attention sequence. In the exemplary embodiment, the sequence starts as a single tone (sounded from the safety processor speaker), pause, triple tone (sounded from the H8 processor speaker) sequence (or three

vibrations when feedback is set to vibration). The sequence repeats every 15 second, in the exemplary embodiment, but in some embodiments, may repeat more regularly or less often, until the device times out or until the user interacts with the device. After a device time out, if there is no user interaction within 1 minute (in other embodiments, this duration may be longer or shorter), the user interface wakes up the pump and repeats the notification using an escalated attention sequence: when the feedback is set to vibration, feedback switches to audio; if the feedback was audio, the audio sequence escalates to a single short ton (from the safety processor speaker), pause, single long (siren) tone (from the H8 processor speaker) sequence. The siren tone is an uninterrupted succession of tones of increasing frequency.

Once the feedback has been escalated to siren, subsequent sounding of the attention sequence rotates from vibration, to audio, to siren. If the user interacts with the device after the attention sequence has been escalated, the next time the attention sequence is sounded, it reverts to the original attention sequence feedback. If the notification is sounded for 15 minutes without user interaction while the pump is in a delivery mode, delivery is stopped and the Inactivity Alarm notification is generated.

In the exemplary embodiments, when the user accepts the "Clear" action selection on a notification screen, the notification is cleared and the user interface closes the notification screen. When the pump checks again for the alert or alarm condition, if the alert or alarm condition still exists, the notification is repeated.

When the user accepts the "Sleep Time" item on a notification screen, the user interface displays the SET SLEEP TIME or opens the Sleep Time item for editing where the user may program the sleep time value. Accepting the "Sleep" action selection on the notification screen dismisses the notification for that user-programmable amount of time (15 minutes to up to 12 hours, depending on the notification). The user interface postpones checking for the condition or presenting the reminder alert again until the amount of time specified in Sleep Time has passed. If the user changes the clock time during the sleep period of an alert, the alert expiration time is adjusted accordingly, so that the alert (or check for the alert condition) is repeated when the amount of time is adjusted accordingly, so that the alert (or check for the alert condition) is repeated when the amount of time specified in the Sleep Time has elapsed, regardless of the clock time. In the exemplary embodiment, a date change has no effect on the expiration time of a reminder that has been slept.

With respect to clock time and date adjustments, in the exemplary embodiment, when the user changes the pump clock time or the date, the pump user interface adjusts the

expiration time for all sleeping alerts, except the low insulin alert, to a time equal to the current expiration time plus (if time or date was adjusted forward) or minus (if time or date was adjusted backwards) the time or date adjustment. However, in the exemplary embodiment, as discussed herein, to change the clock time, basal delivery must first be
5 stopped. When basal delivery is again started, both sleeping pump idle and low insulin alerts are reset.

With respect to the date, when the user changes the pump date forward in time, the pump user interface generates a reminder alert for all user programmable reminders that either have been cleared or have not yet expired (excluding reminders that have been slept).
10 When the user changes the pump clock time only (no date change) to a time earlier than the time of a cleared user-programmable reminder alert, the pump user interface shall reset the reminder alert.

In the exemplary embodiment, when the pump clock time is changed to a time later than the user-programmed times of a user-programmable reminder alert that has not yet
15 expired (i.e., has neither been cleared nor slept) the user interface generates a reminder alert notification.

Where an alert, reminder or recoverable alarm condition occurs on the pump when the user interface is displaying the Home screen, the user interface produces the attention sequence on the pump and displays the notification screen that describes the condition.
20 Referring now to FIG. 17, examples of alert, reminder and recoverable alarm screens are shown. If the pump is in a sleep state, the user interface wakes up the pump to present the notification. With respect to embodiments including a Companion, in the exemplary embodiment, on the Companion, if the Companion is awake and displaying the Home screen, the notification screen also is displayed on the Companion. If the Companion
25 screen is asleep and the user wakes it up when the pump is displaying a notification, when communication with the pump resumes, the notification also is displayed on the Companion. The user interface allows the user to dismiss an alert or reminder for a programmable amount of time, which the user selects on the notification screen itself. There may be a few exceptions, in the exemplary embodiment, of alert screen that cannot be
30 dismissed, but only cleared.

Referring now to FIG. 18A, in the exemplary embodiment, the user opens the SET SLEEP TIME edit item screen when the user accepts the Sleep Time item on an alert or reminder notification screen. The user accepts the Sleep Time item to define the period of time for which to sleep the notification. Referring now to FIG. 18B, in the exemplary

embodiment, the user may program up to six reminders (however, in some embodiments, the user may program a greater number of reminders) specifying a time of day and choosing to enable or disable the reminder. The user interface generates a reminder alert for enabled reminders when the clock time changes to the user-programmed time for the reminder. The
5 expiration time for all reminders that are "sleeping" is adjusted whenever the user changes the pump clock time and/or date, so that the actual amount of time for which the alert is sleeping reflects elapsed time that matches the user-specified sleep time. When the user changes the clock time to a time later than the user-programmed expiration time for a reminder that has not expired, the reminder will be detected when the user returns to the
10 Home screen, and the alert will be generated. Additionally, if the user changes the date forward, the pump user interface generates an alert for all enabled reminders that are not "sleeping" when the user returns to the Home screen.

For a bolus reminder, if the start of the normal bolus delivery (either a normal bolus, or the normal bolus portion of a dual bolus) occurred within 2 hours of an enabled bolus
15 reminder time, the user interface clears the bolus reminder alert. If the start of a normal bolus has not occurred within 2 hours of the programmed bolus reminder time, the user interface displays the reminder alert at the programmed time.

For a bolus reminder, if the start of a normal bolus delivery (either a normal bolus, or the normal bolus portion of a dual bolus) occurred within 2 hours of an enabled bolus
20 reminder time, the user interface clears the bolus reminder alert. If the start of the normal bolus has not occurred within 2 hours of the programmed bolus reminder time, the user interface displays the reminder alert at the programmed time.

In the exemplary embodiment, clearing a reminder does not disable the reminder. The alert condition will be detected again when the reminder expires (when the clock
25 changes to the user-programmed time for the enabled reminder, or a time/date change causes the reminder to expire). The user interface will generate the reminder alert notification until the user disables the reminder through the ALARM SETUP: REMINDERS screen.

The user interface generates a reminder alert notification once a day for all user-
30 programmable reminders that are enabled, provided the user does not change the clock time to a time earlier than the reminder after the reminder already expired; or does not change the date. When the user enables a reminder alert, if the user programmed time is later than the current clock time, the user interface generates the reminder alert notification before the end of the current 24-hour period. Conversely, when the user enables a reminder, if the user-

programmed time for the reminder is earlier than the current time within the current 24-hour period, the user interface does not generate the reminder alert until the next day.

Referring to FIGS. 19A-19E, in the exemplary embodiment, with respect to alarm conditions, these include, but are not limited to: "OCCLUSION ALARM", "RESERVOIR
5 ALARM", "BAD BATTERY ALARM", "NO INSULIN ALARM", and "INACTIVITY ALARM".

Referring to FIGS. 20A-20I, in the exemplary embodiment, with respect to alert conditions, these include, but are not limited to: "LOW BATTERY ALERT", "LOW
INSULIN ALERT", "INACTIVITY ALERT", "PUMP IDLE ALERT", "STOPPED
10 ALERT", "CANCELLATION ALERT" (i.e., when the device times out after a value has been changed but not saved), "CHECK BG ALERT" (when the CHECK BG care comment is enabled, this alert is generated by the user interface when 2 hours has elapsed since the last cannula prime), "SITE CHANGE ALERT" alert (when this user-programmable care
comment is enabled by the user, the user interface generates this alert when the amount of
15 time between the last cannula prime and the time specified by the user-programmable setting for the SITE CHANGE care comment Frequency item elapses), and "INSULIN TEMP ALERT" (when this user-programmable care comment is enabled, the user interface generates an INSULIN TEMP ALERT notification when the internal temperature of the Pump exceeds a threshold preset temperature, or is less than a threshold, preset temperature,
20 which, in the exemplar embodiment is 96.8 ± 3.6 degrees Fahrenheit (36 ± 2 degrees Celsius) and 37.0 ± 3.6 degrees Fahrenheit (2.8 ± 2 degrees Celsius) respectively. In the exemplary embodiment, the infusion pump includes at least one temperature sensor inside the pump housing or pump body (and either in the reusable portion or the disposable portion of one embodiment of the infusion pump). In some embodiments, the infusion pump
25 includes more than one temperature sensor.

As discussed above, Reminders may be user-programmed by the user into the user interface. In the exemplary embodiment, six reminders may be programmed, however, in other embodiments; a greater number of Reminders may be user-programmed. Each Reminder includes specified time for the reminder, a message and an indication of whether
30 the Reminder is "on" or "off". Thus, the user may set up different Reminders in the six Reminder screens and save those settings, whether or not any of the Reminders are turned on. On any given day, the user may turn on or off any of the six reminders.

In the exemplary embodiment, the user interface presents a list of programmable values for the Message item, which include, but are not limited to: "Check BG", "Wakeup",

“Basal”, “Bolus”, “Exercise”, “Meeting”, “Pickup”, “Snack”, “Meds”. Referring now to FIGS 21A-21B, an example of the REMINDER format screens are shown for both the 12-hour Time Format and the 24-Hour Time Format respectively.

In the exemplary embodiment, Care Comments, for example, “INSULIN TEMP”, “SITE CHANGE”, “CHECK BG”, may be individually enabled or disabled by the user. The Care Comments generate a CARE COMMENT ALERT at the specified time. With respect to INSULIN TEMP, as discussed above, once this Care Comment is enabled, a CARE COMMENT ALERT will be generated when the temperature inside the pump either exceeds or goes below the set threshold. With respect to CHECK BG, this Care Comment, when enabled, will ALERT 2 hours following a cannula prime.

Referring now to FIG. 22, with respect to the SITE CHANGE, this Care Comment requires the user to select the Frequency based on the last cannula prime. For example, if the user sets the Frequency to “3.0 days”, when the SITE CHANGE care comment is enabled, the pump with SITE CHANGE ALERT 3.0 days following the latest in time cannula prime.

With respect to the Care Comments, in the exemplary embodiment, the user interface provides a “Disable All” option that allows the user to disable all Care Comment alerts. When the “Disable All” items on the OPTIONS screen is set to “Yes”, this setting overrides the individual settings for the INSULIN TEMP, SITE CHANGE and CHECK BG Care Comment settings.

Basal and Pump Idle

In the exemplary embodiments, the infusion pumps may deliver a “basal” of fluid or insulin, in the exemplary embodiment. In the exemplary embodiments, the term “basal” takes on its accepted meaning of a dose of insulin or other fluid delivered at a “rate”, typically, Units/Hour. The infusion pump may be placed in an “IDLE” mode by the user through the “STOP BASAL” function of the user interface. Also, as discussed herein, the pump may place itself into IDLE mode in some circumstances. Thus, IDLE is a mode in which the pump stops delivery of the basal rate. Additionally, in IDLE mode, the pump, in the exemplary embodiment, can not deliver any insulin, thus, the pump’s delivery is suspended or “idle”.

In the exemplary embodiments, IDLE mode is required for functions where there delivery may be affected. Those functions may include, but are not limited to: change to the date and/or time; change of hardware, i.e., reservoir or battery; and/or a change in the currently active basal rate; and/or change to basal limits.

In the exemplary embodiment, once the pump is placed into IDLE mode, the pump will alert the user at an interval, e.g., every 5 minutes. This is a safety measure to ensure the user is aware the pump is not delivering. Thus, the IDLE mode is instigated by the user, and therefore, the user is aware the pump is not delivering. As the pump will remind the user of the IDLE mode, this ensures the user is continuously aware the pump is not delivering.

With respect to power, in the exemplary embodiment, where the pump senses there is no power, the pump will notify the user as the pump will assume there has been a battery failure. However, where a user is changing the battery (i.e., changing the power source), the user is aware that there will not be power for the time it takes to replace the battery. In the exemplary embodiment, the user may place the pump into IDLE while changing the battery. Thus this tells the pump that the power failure is expected. Thus, this failure analysis feature assists the pump in distinguishing between a power failure and an intended power supply removal.

In this way, the pump only allows a silent shutdown (a shutdown not accompanied by a notification from the pump) when the user places the pump in IDLE before removing the battery. As a safety, however, in the exemplary embodiments, the pump will continue its IDLE TIMER, and will alert the user at an interval, that the pump remains in idle. This also will occur where the battery or power source has been removed, as in the exemplary embodiment; the infusion pump includes a super capacitor back-up power supply that will prevent the infusion pump from having a silent shutdown as the infusion pump will have the power to alert the user of the shutdown. Further, the super capacitor/ back-up power supply allows the infusion pump to notify the user at intervals during IDLE mode, even when the power supply has been removed and before a power supply has been replaced.

25 Bolus

In the exemplary embodiments, the term "bolus" takes the meaning of a volume of insulin delivered upon request. The term "normal" bolus equates to a bolus where delivery commences upon request. The term "extended bolus" refers to a volume of insulin delivered over a user-programmed period of time. Thus, for example, a "normal" bolus may be 5.5 U, where delivery is commenced at request. An "extended" bolus or 5.5U may be delivered over 2 hours. A "dual" bolus is a combination of a normal bolus and an extended bolus, where the user specifies the units to be delivered as a normal bolus, and the time over which the extended bolus is to be delivered. For example, a dual bolus of 6.5 U may be delivered as follows: 1U delivered as a normal bolus, and 5.5 U delivered over 2

hours. Additionally, in the exemplary embodiment, a bolus termed a "Qbolus" refers to a QUICK BOLUS, which is a normal bolus in which the user interface immediately brings the user to a screen where the user simply scrolls to enter the Units for the normal bolus.

Referring now to FIGS. 23A-23B, a selection of at least some BOLUS screens are shown. Referring first to FIG. 23A, one of the methods of programming and delivering a normal bolus is by selecting the MANUAL item on the BOLUS MENU screen, which displays the BOLUS select item for edit screen. Through the BOLUS screen, the user may program a Normal, Extended or Dual bolus. The values that appear on the screen vary depending on the bolus type that the user selects.

The Extended bolus features allow the user to deliver a bolus over a longer period of time by specifying a length of time over which the bolus should be delivered. When programming an Extended bolus without using a bolus calculator, the Bolus item is set to dashes. When using the Food only calculator, the Bolus item is set to the calculated Carb Insulin value; for a Food and Correct or Food & Correction bolus, the Bolus item is set to the calculated Carb Insulin value minus the IOB amount. For any calculated bolus, the bolus amount is based on the pump delivery resolution (which may vary between pump embodiments) regardless of the user-programmable bolus increment. However, when the user makes a change to a calculated value on the BOLUS screen, the user-programmed bolus increment is used. For example, if the calculated value was 0.55 U, and the bolus increment settings is 1.0U, when the user edits the Bolus value, a downward increment changes the value to 0.0U, and an upward increment changes the value to 1.0U.

Also, in the exemplary embodiment, if the user changes the Bolus amount for an extended bolus to 0.0U, the Duration item is removed from the BOLUS screen. The user is allowed to accept Deliver for a 0.0U bolus, but no bolus history is generated for a 0 bolus.

A dual bolus allows the user to program and deliver a bolus that consists of a normal bolus that is delivered immediately, and an extended bolus that is delivered over an extended (user-defined) period of time. When an extended bolus is currently running, the user is not allowed to program a dual bolus. If the user changes the Extended amount of 0.0U, the Duration item is removed from the BOLUS screen. The user is allowed to accept Deliver for a 0.0U bolus, but no bolus history is generated for a 0 bolus.

Referring now to FIG. 23B, QUICK BOLUS screens are shown. A QUICK BOLUS, or QBOLUS screen displays a programmable number, allowing the user to quickly program a normal bolus, bypassing the screen on which the bolus type is selected. In the exemplary embodiment, a QUICK BOLUS is delivered as a Normal bolus.

In the exemplary embodiment, while the pump is in IDLE, a bolus may not be delivered. If a user requests a bolus delivery and the pump is in IDLE, the user interface will remind the user to "Start Basal before bolusing". This serves as a reminder to the user that the pump is in IDLE, and thus, the user must start basal prior to bolusing.

5 Additionally, in the exemplary embodiment, while the pump is delivering an extended bolus, if the user requests a second extended bolus, the user interface will display a WARNING "Extended Bolus already in progress". This serves to remind the user they have already programmed an extended bolus.

10 A correction bolus is a bolus calculated using the 1U DROP value discussed above, and used to calculate how much insulin to deliver to bring the user's blood glucose value to a desired level. In the exemplary embodiment, when CORRECTION is selected from the BOLUS, if this is done within 2 hours of the last bolus when the Insulin Profile Type setting is Rapid, or 3 hours of the last bolus when the Insulin Profile Type setting is Short, the user interface displays the "Less than 2/3 hours since last bolus" WARNING. The user may still
15 continue programming a correction bolus after accepting "OK". This WARNING screen serves to inform the user of the duration since their last bolus before they proceed with requesting a correction.

Referring now to FIG. 24A, in the exemplary embodiment, when bolus data is not available for the entire action time period, the user interface displays the IOB value on the
20 Home screen with a greater than or equal symbol, and generated the "IOB may not include all boluses" WARNING when one or more of the following are true, which include, but are not limited to:

- 1) When less time than the user-programmed action time has elapsed since the bolus log was initialized, and the user accepts the Next action selection on the
25 BLOOD GLUCOSE screen (in the exemplary embodiment, the bolus log is initialized when the pump is without power for at least 15 minutes and the time and date is set to dashes at power up);
- 2) When the number of boluses in the bolus history that occurred with the user-programmable action time exceeds 10, or the IOB amount is greater than 300,
30 and the user accepts Next action selection on the BLOOD GLUCOSE screen.
- 3) When there is no bolus history due to loss of time and date, and the user accepts then Next action selection on the BLOOD GLUCOSE screen.
- 4) When the user presses the back button on the BOLUS screen that was populated with a calculated Insulin value from the BLOOD GLUCOSE screen, and the

IOB value is displayed on the BG CALC DETAILS screen with a question mark.

Referring to FIG. 24B, in the exemplary embodiment, with respect to programming a bolus using one or both calculators (correction calculator or food and correct calculator), if
5 the Bolus amount calculates to a value less than or equal to 0.0U, the user interface displays the "Zero bolus calculated. Cancel bolus?" CONFIRM screen.

Referring to FIG. 24C, when a bolus history has been established (which, in the exemplary embodiment, is established when at least one bolus has been delivered); the user interface calculates the amount of IOB that is still active to subtract from the calculated
10 insulin amount for a Correction bolus. When there is no bolus history and at least 2 hours (when insulin profile setting is Rapid) or 3 hours (when insulin profile setting is Short) have not yet elapsed since the bolus log was initialized, if the user programs a bolus using the Correction calculator, the user interface displays the "Last bolus time unknown. Continue?" CONFIRMATION screen, when the user accepts the FOOD & CORRECT or just
15 CORRECTION item on the BOLUS MENU screen.

Referring now to FIG. 24D, in the exemplary embodiment, the user interface imposes a maximum bolus for all types of boluses, defined by the user-programmable setting, Bolus Limits Maximum (SETUP:BOLUS LIMITES). The user interface displays the "Maximum bolus of [nn.nn] U exceeded. Cancel Bolus?" CONFIRMATION screen
20 when the user does at least, but not limited to, any one of the following:

- 1) Programs a bolus using either the Correction or Food calculator, and attempts to deliver a bolus with a calculated insulin value that is greater than the maximum bolus limit. In the confirmation message text, [nn.nn] U is the value of the maximum bolus limit setting (SETUP: BOLUS LIMITS). The user interface
25 displays the confirmation screen when the user selects "Next" on the FOOD or BLOOD GLUCOSE, and the bolus value calculation is greater than the user-programmable setting for bolus maximum limit.
- 2) Programs a dual bolus and the total bolus amount for the combined Normal and Extended exceeds the maximum bolus amount. The user interface displays the confirmation screen when the user selects Deliver on the Dual Bolus screen
30 when the combined bolus amount is greater than the user-programmable setting for bolus maximum limit.

As discussed above with respect to the Home screen, the user interface includes readily available information regarding the IOB and the last bolus. In the preferred

embodiment, the Units and the amount of time elapsed since the last bolus may be on the Home screen. Additionally, in the exemplary embodiment, the user interface includes a series of HISTORY screens. Referring now to FIG. 25, when the user accepts the HISTORY item on the BOLUS MENU or REPORTS MENU screen, the user interface
5 displays the HISTORY 1 of n screen. The user may clock through history details for the 10 most recently delivered boluses. In other embodiments, more than the 10 most recently delivered boluses may be available using this feature. The HISTORY screens show records for completed boluses, including normal (which includes one-button and Qboluses), and extended boluses. The records are ordered by completion time, with the most recently
10 completed boluses displayed first. Thus, the user interface provides easy access to the last 10 bolus records, including both the Units, the type of bolus (e.g., normal, extended, etc.) and the elapsed time since the bolus was completed.

Diary and Reports

Referring now to FIG. 26, in the exemplary embodiment, the REPORTS MENU
15 screens provides access to the pump diaries and the bolus history. After the pump is fully initialized, the user accesses the REPORTS MENU screen by selecting REPORTS on either the MAIN MENU screen, or the Activity-Based Home screen. On the pump, when engineering access is enabled, the REPORTS MENU screen includes a SEND DIARY option for sending pump logs to a PC. These are described with respect to FIGS. 31-34D.

20 Referring now to FIG. 27, in the exemplary embodiment, when the user selects and accepts the PUMP DIARY items on the REPORTS MENU screen, the user interface displays the PUMP DIARY screen, from which the user may select to view or send diaries.

Referring now to FIG. 28, in the exemplary embodiment, when the user accepts the THERAPY item on the PUMP DIARY screen, the user interface displays the Daily Therapy
25 Summary screen for the current day (the 24-hour period beginning at 12 AM in the exemplary embodiment). The Daily Therapy Summary screen shows the total daily dose, which includes all basal and boluses delivered for that 24 hour period, and excludes volume delivered through device primes. For an extended bolus that spans more than one day, the total daily dose includes that portion of the extended bolus that was delivered within the 24
30 hour period. The user may scroll through Daily Therapy Summary screens for up to the previous 30 days. The first entry is the current calendar day; the 30th entry is 30 calendar days ago. For example, if the current date is June 14, 2008, the first daily therapy entry is June 14 and the 30th entry is May 16. If there is no delivery data in the therapy diary for 29

days earlier than the current date, the user interface displays Daily Therapy Summary screens for the number of days from the current date to the earliest date in the therapy diary.

The therapy diary is read from the most recent date to backwards in time. While reading the therapy diary, if the user interface encounters an entry with a later date than the
5 last event that was read, the delivery data for that day (the day of the last event that was read) is considered complete with all entries are ignored until an earlier date is found. When there is no delivery data for a given date the total daily dose summaries for that date are 0.0U and the % Basal item is removed form the Therapy Summary screen.

If the diary entries indicate a basal rate other than 0 when a powerup event was
10 encountered, the summary details for that day are removed from the Therapy Summary screen, and "Invalid data" is displayed instead. If the current day is the first day of pump usage and the first basal delivery begins later than 12 AM, the period of time between 12 AM and the first basal delivery date is represented as 0.0U/h. Similarly, the period of time between the time when the user accepted the THERAPY item on the PUMP DIARY screen
15 and the end of the current 24-hour period also is represented as 0.0U/h.

Referring now to FIGS. 29A and 29B, in the exemplary embodiment, when the user accepts the EVENTS item on the PUMP DIARY screen, the user interface displays the Event Summary screen for the pump event that occurred most recently. The Event Summary screen displays the date and time that the event occurred, a description of the
20 event, and may or may not include additional details, depending on the event. For example, related to delivery include programmed and delivered amounts; other events such as extended boluses and temporary basals include durations. The user may review Event Summary screens for at least 150 events (however, in other embodiments, additional events, i.e., greater than 150, may be viewable), which are ordered from the event that occurred
25 most recently (first entry) to the event that occurred farthest in the past (last entry).

Referring now to FIG. 30, in the exemplary embodiment, when the user accepts the ALARMS item on the PUMP DIARY screen, the user interface displays the Alarm Summary screens for the most recent recoverable or non-recoverable alarm. The user may scroll through Alarm Summary screens from past alarms.

30 Referring now to FIG. 31, in the exemplary embodiment, when the engineering access is enabled, the REPORTS MENU screen includes a SEND DIARY item. When the user accepts the SEND DIARY item on the REPORTS menu screen, the user interface displays the SEND DIARY screen. Here, the user may select from a list of logs to send to a PC.

Referring now to FIG. 32, in the exemplary embodiment, when the user accepts the SEND DIARY item on the REPORTS MENU screen, then accepts any item other than DONE on the SEND DIARY select item screen; the user interface displays the "In the PC Connection Ready?" confirmation screen. When the user interface displays the SEND
5 DIARY screen after the user selected "Yes" on the "Transfer Another Log?" confirmation screen, and the user selects any item other than "Done", the "Is the PC Connection Ready?" screen is not displayed.

Referring now to FIG. 33, when engineering access is enabled, the user may send diary logs to the PC. In the exemplary embodiment, while transferring a diary log, the user
10 may choose to write the resulting log file to the PC in ASCII format. After the user has confirmed that the PC connection is ready by selecting "Yes" on the "Is the PC Connection Ready?" confirmation screen, the user interface displays the "Ascii format?" confirmation screen.

Referring now to FIG. 34A, in the exemplary embodiment, when engineering access
15 is enabled, the user may send diary logs to the PC. While transferring a diary log, the user may choose to prepend configuration information in the resulting log file on the PC. After the user has selected "Yes or "No" on the "Ascii format?" confirmation screen, the user interface displays the "Prepend config info?" confirmation screen.

Referring next to FIG. 34B, in the exemplary embodiment, when engineering access
20 is enabled, the user may send diary logs to the PC. While transferring a diary log, the user may choose whether to include record numbers in the resulting log file on the PC. After the user has selected "Yes or "No" on the "Prepend config info?" confirmation screen, the user interface displays the "Include record number?" confirmation screen.

Referring now to FIG. 34C, in the exemplary embodiment, when engineering access
25 is enabled, the user may send diary logs to the PC. While transferring a diary log, the user may choose to erase the log on the pump. The user interface transitions from the SENDING screen to the "Transfer Complete Erase Log?" confirmation screen when the data transfer has finished.

Referring now to FIG. 34D, in the exemplary embodiment, when engineering access
30 is enabled, the user may send diary logs to the PC. Once one log has been transferred, the user interface displays the "Transfer Another Log?" screen. Where the user selects "Yes", the user interface returns to the SEND DIARY menu.

While the principles of the invention have been described herein, it is to be understood by those skilled in the art that this description is made only by way of example and not as a

limitation as to the scope of the invention. Other embodiments are contemplated within the scope of the present invention in addition to the exemplary embodiments shown and described herein. Modifications and substitutions by one of ordinary skill in the art are considered to be within the scope of the present invention.

CLAIMS

What is claimed is:

1. A system for pairing a controller and an infusion pump, the system comprising:
 - an infusion pump;
 - a controller device; and
 - a user interface residing on both the infusion pump and the controller, the user interface comprising a pairing mode for enabling wireless communication between the infusion pump and the controller device, wherein the user interface requires both the infusion pump and the controller to be in the pairing mode simultaneously.
2. The system of claim 1 wherein the controller includes a display.
3. The system of claim 2 wherein the infusion pump comprising a display.
4. The system of claim 1 wherein the pairing mode further comprising a timeout feature, wherein the pairing mode will timeout if the pairing is not completed within a predetermined time.
5. The system of claim 1 wherein the pairing mode further comprising an indicator to indicate the user interface has found a device in which to pair, the indicator comprising a serial number.
6. The system of claim 1 wherein the pairing mode requires the infusion pump and the controller to be set to the same glucose units.
7. A method of changing a power source in an infusion pump comprising:
 - placing the infusion pump in idle mode wherein the infusion pump stops delivery;
 - removing the first power source from the infusion pump;
 - replacing the first power source with a second power source in the infusion pump; and
 - maintaining the insulin on board during the changing of the first power source with the second power source.

8. The method of claim 7 further comprising sending a notification when the time between the first power source being removed and the second power source being replaced exceeds a threshold.

1/42

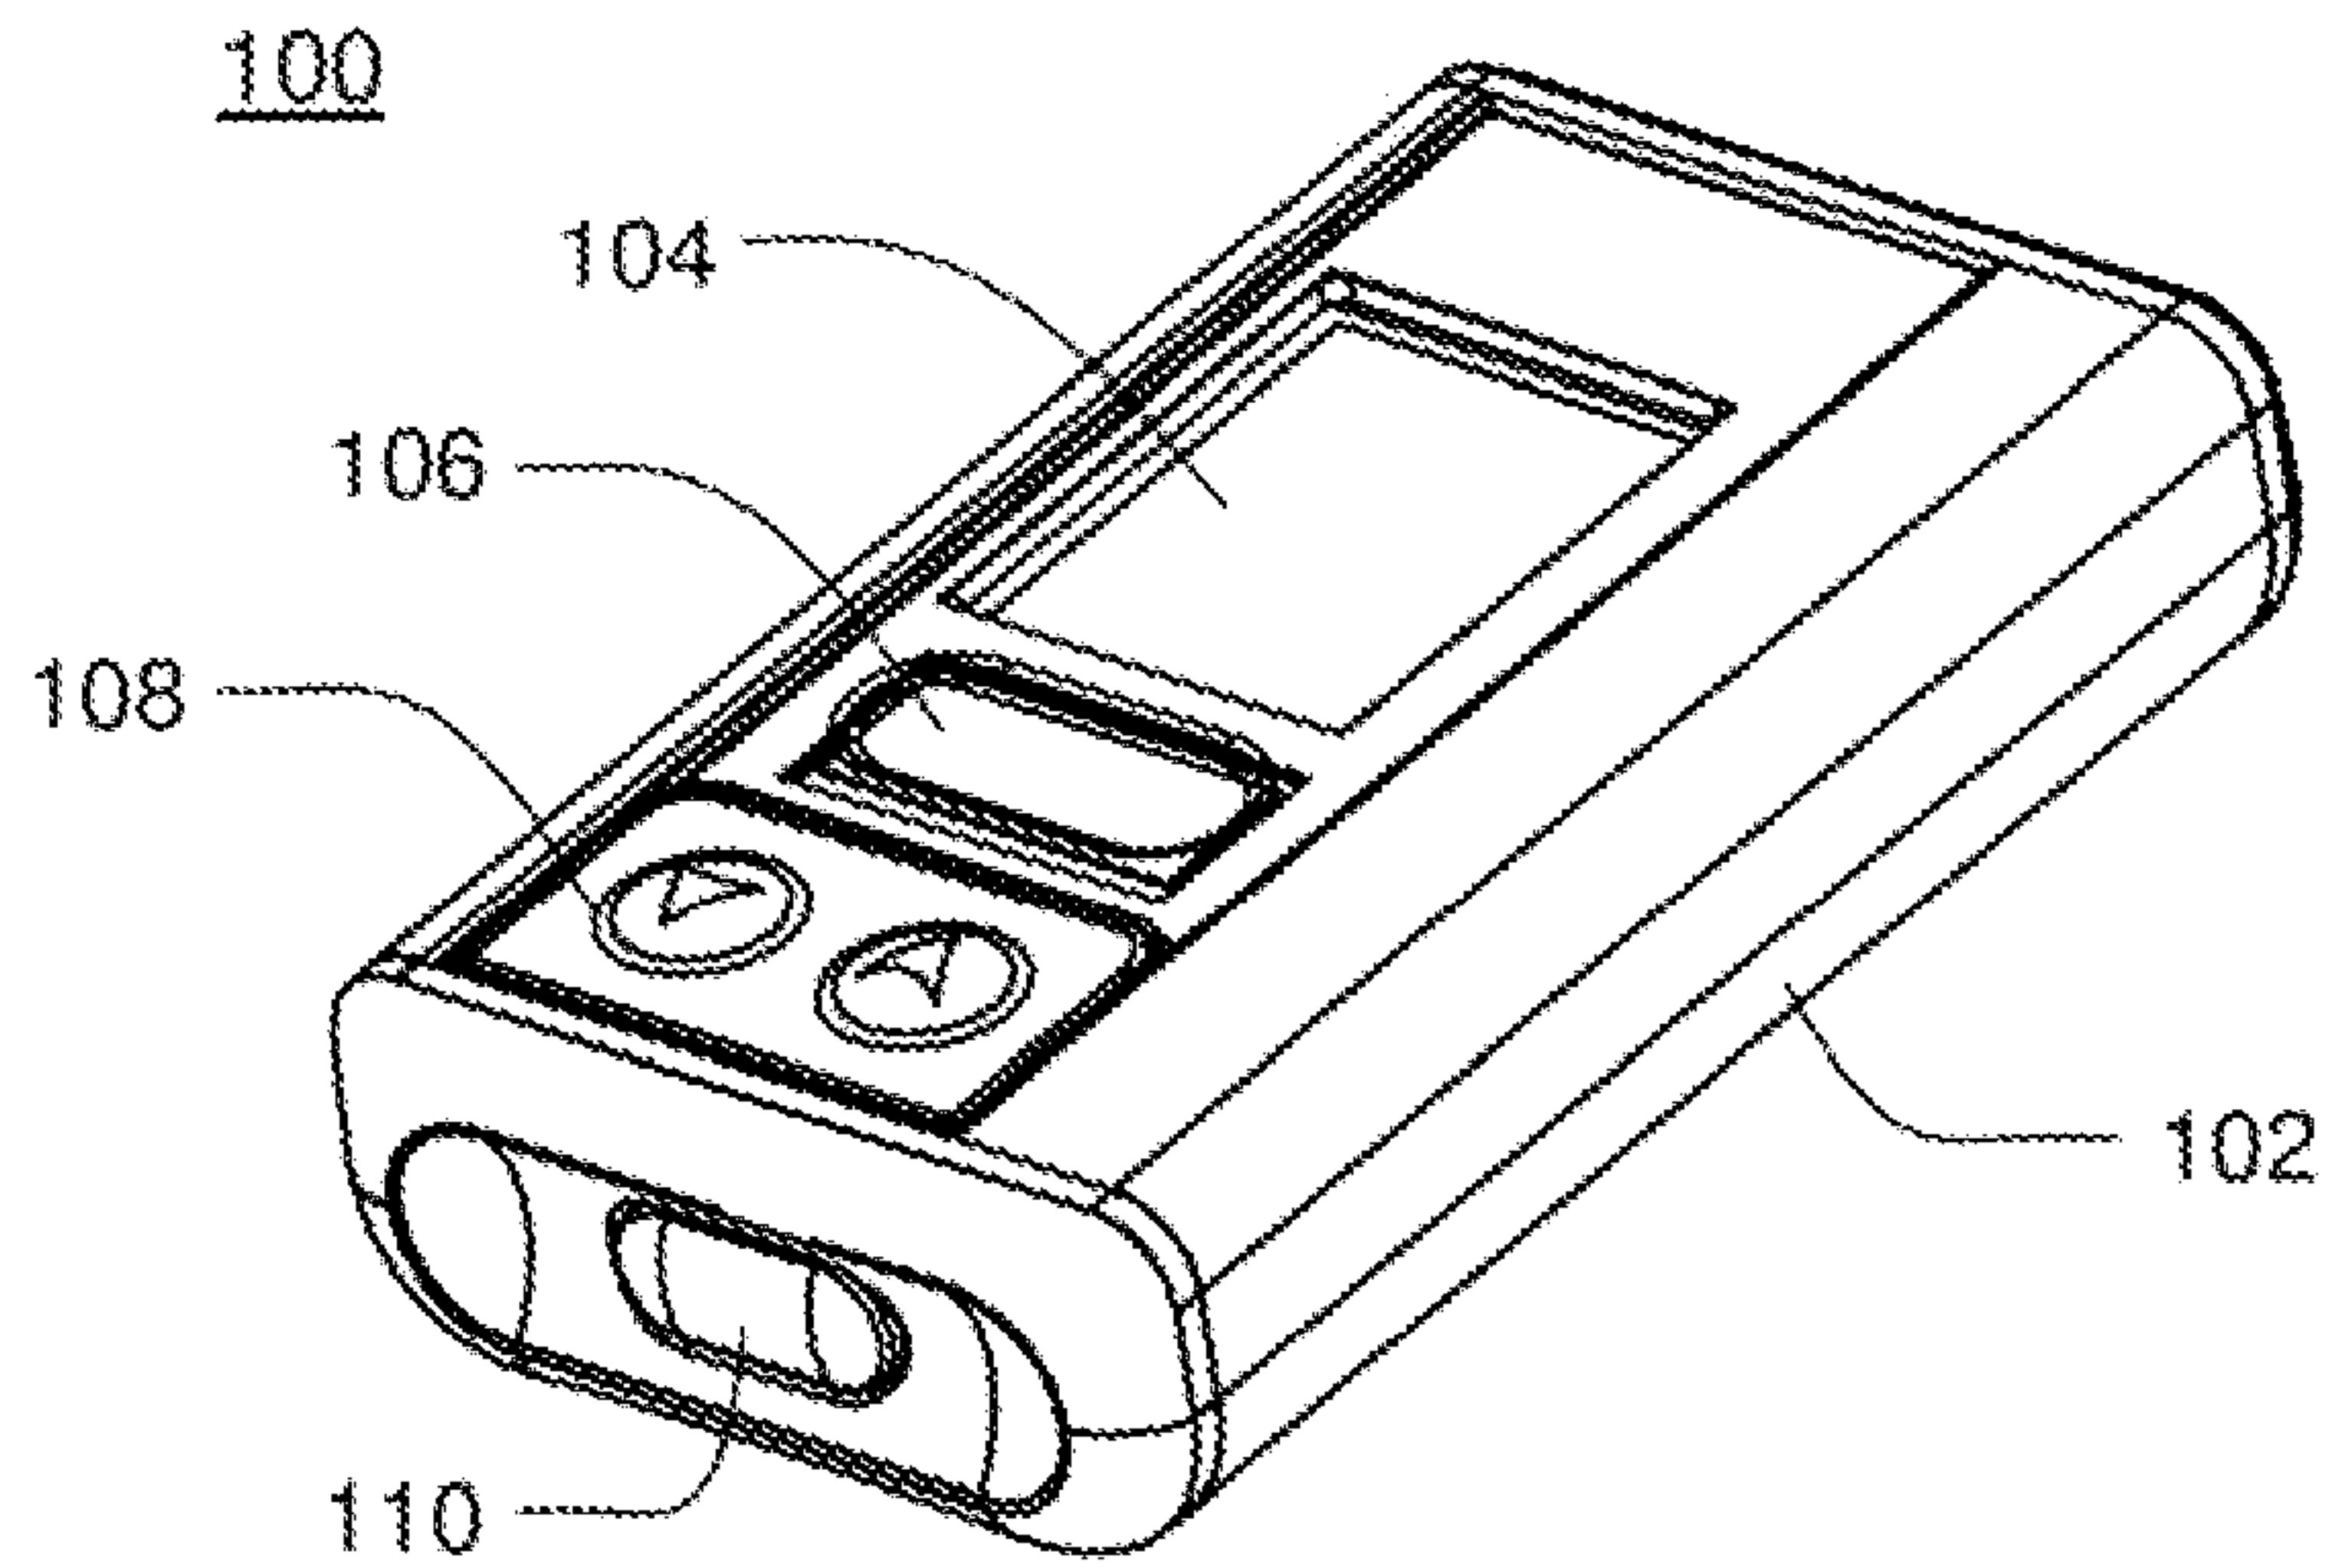


FIG. 1A

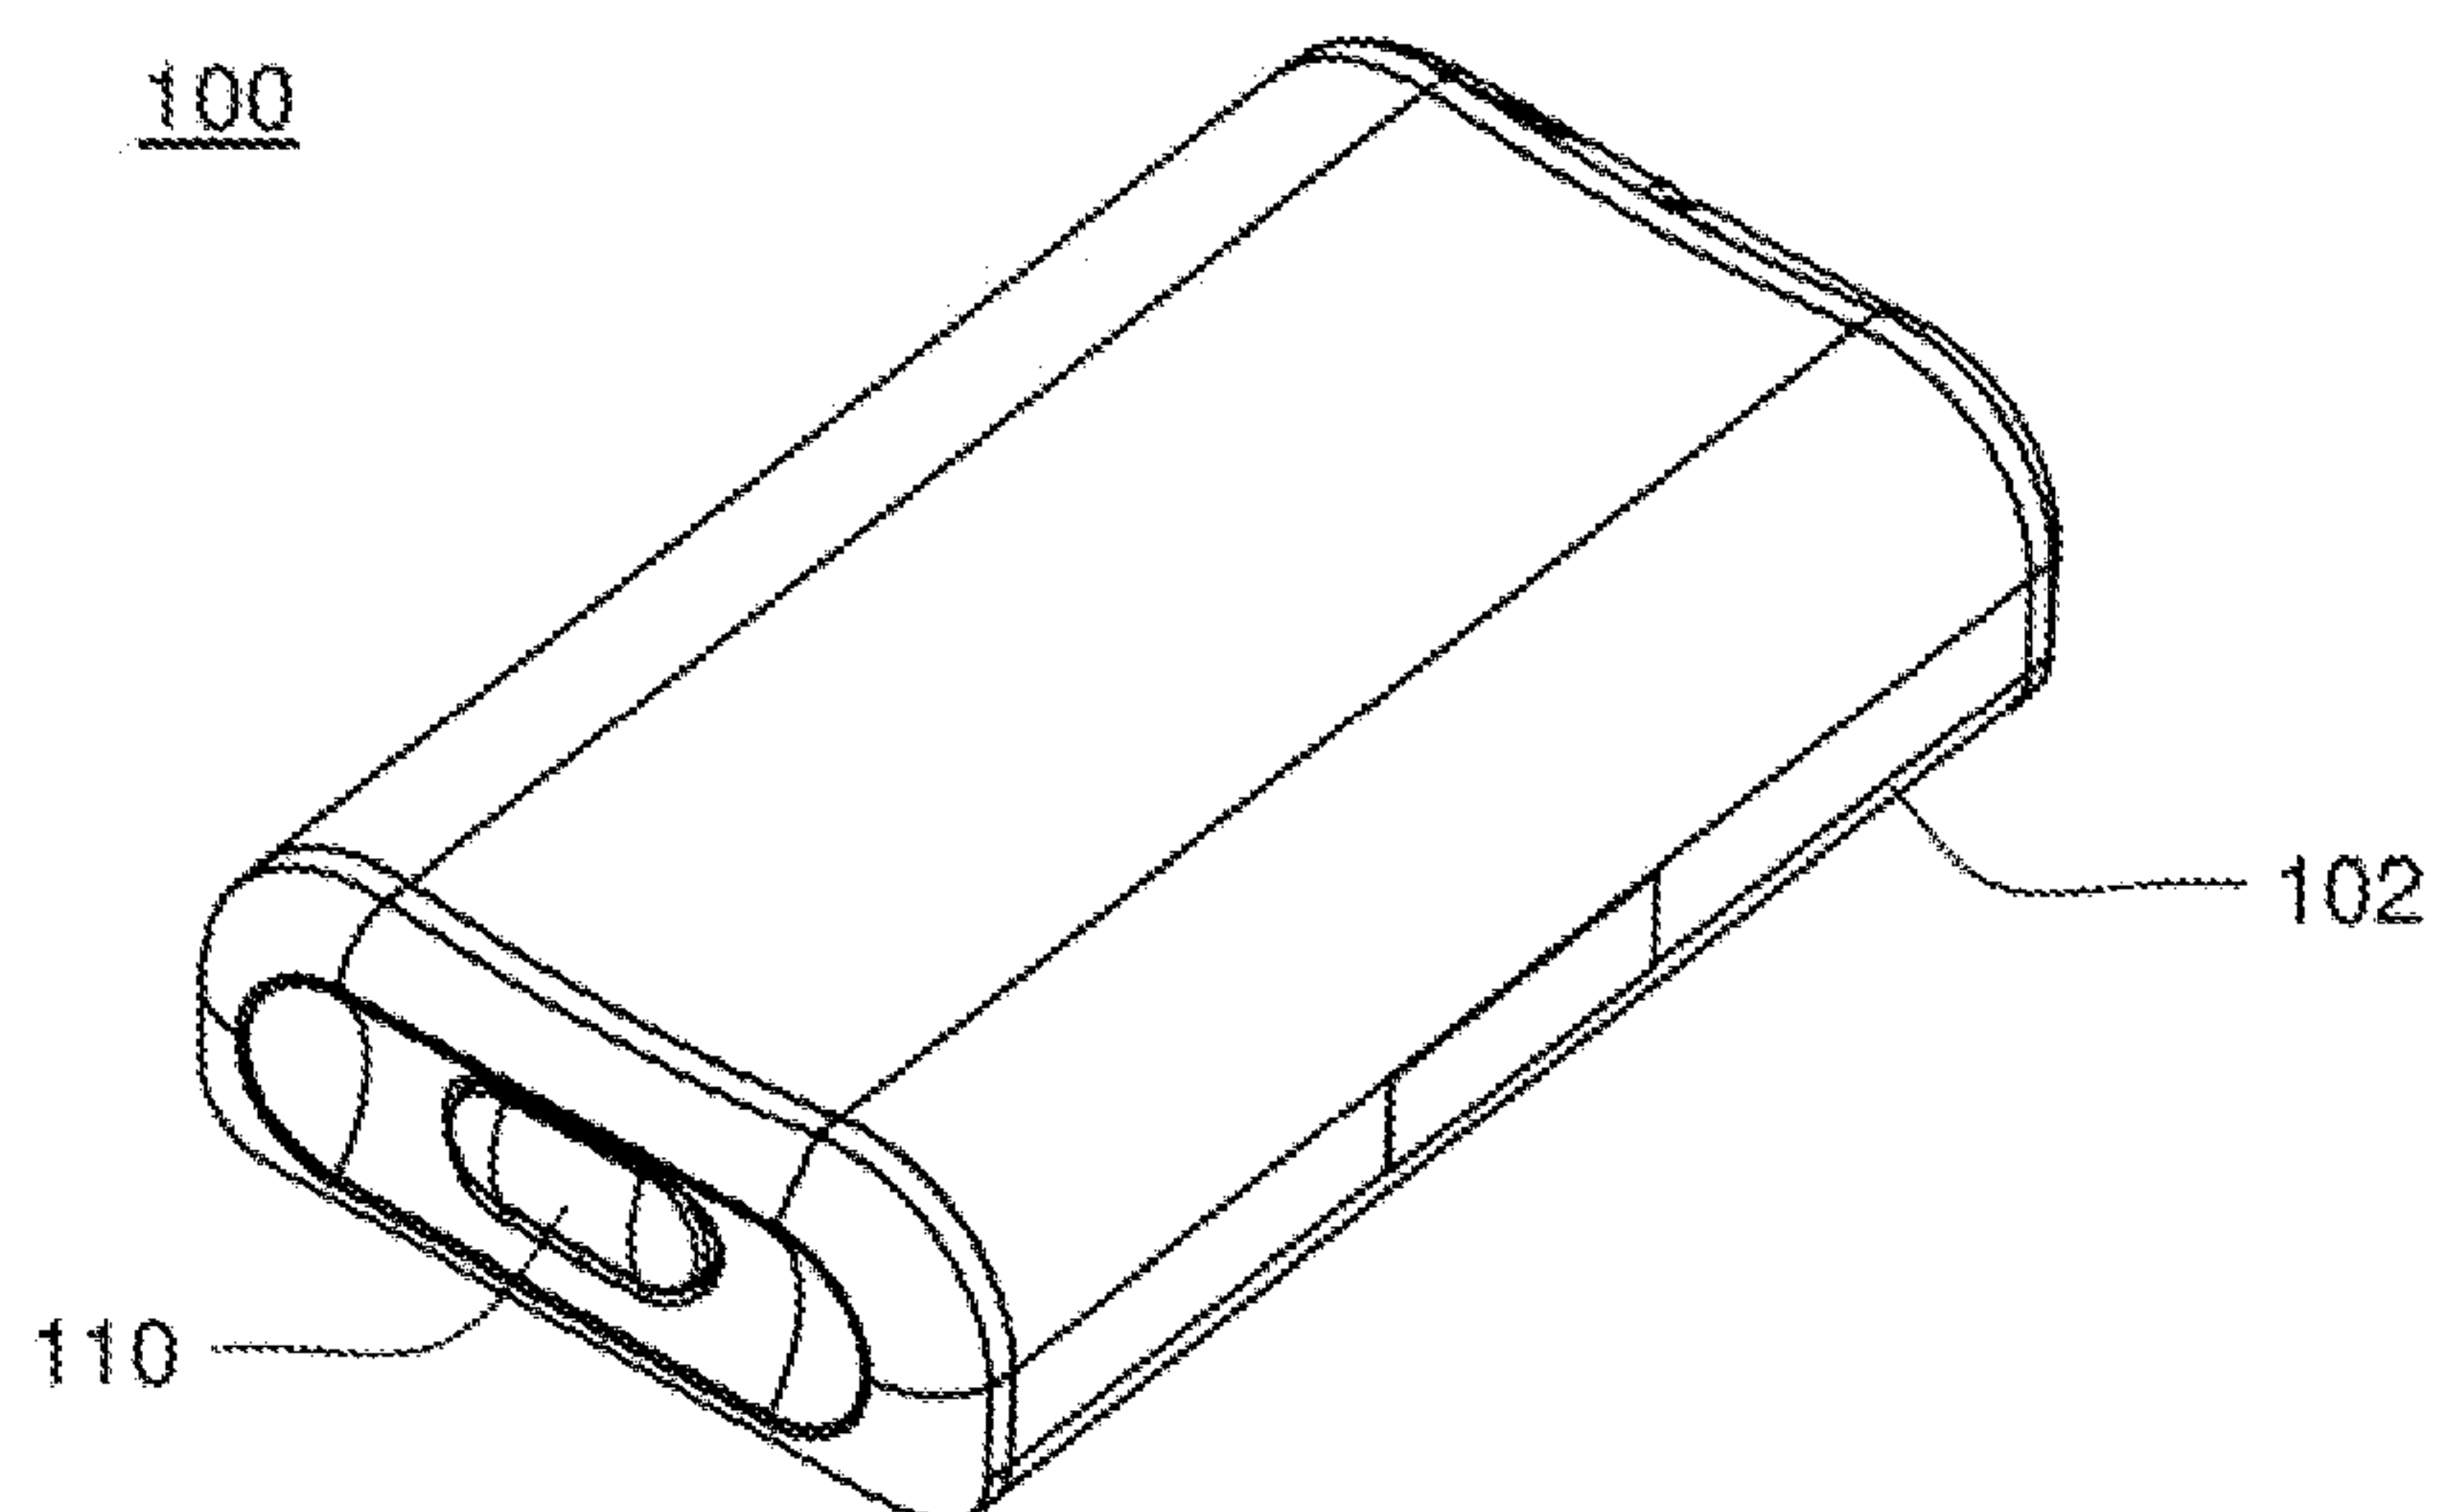


FIG. 1B

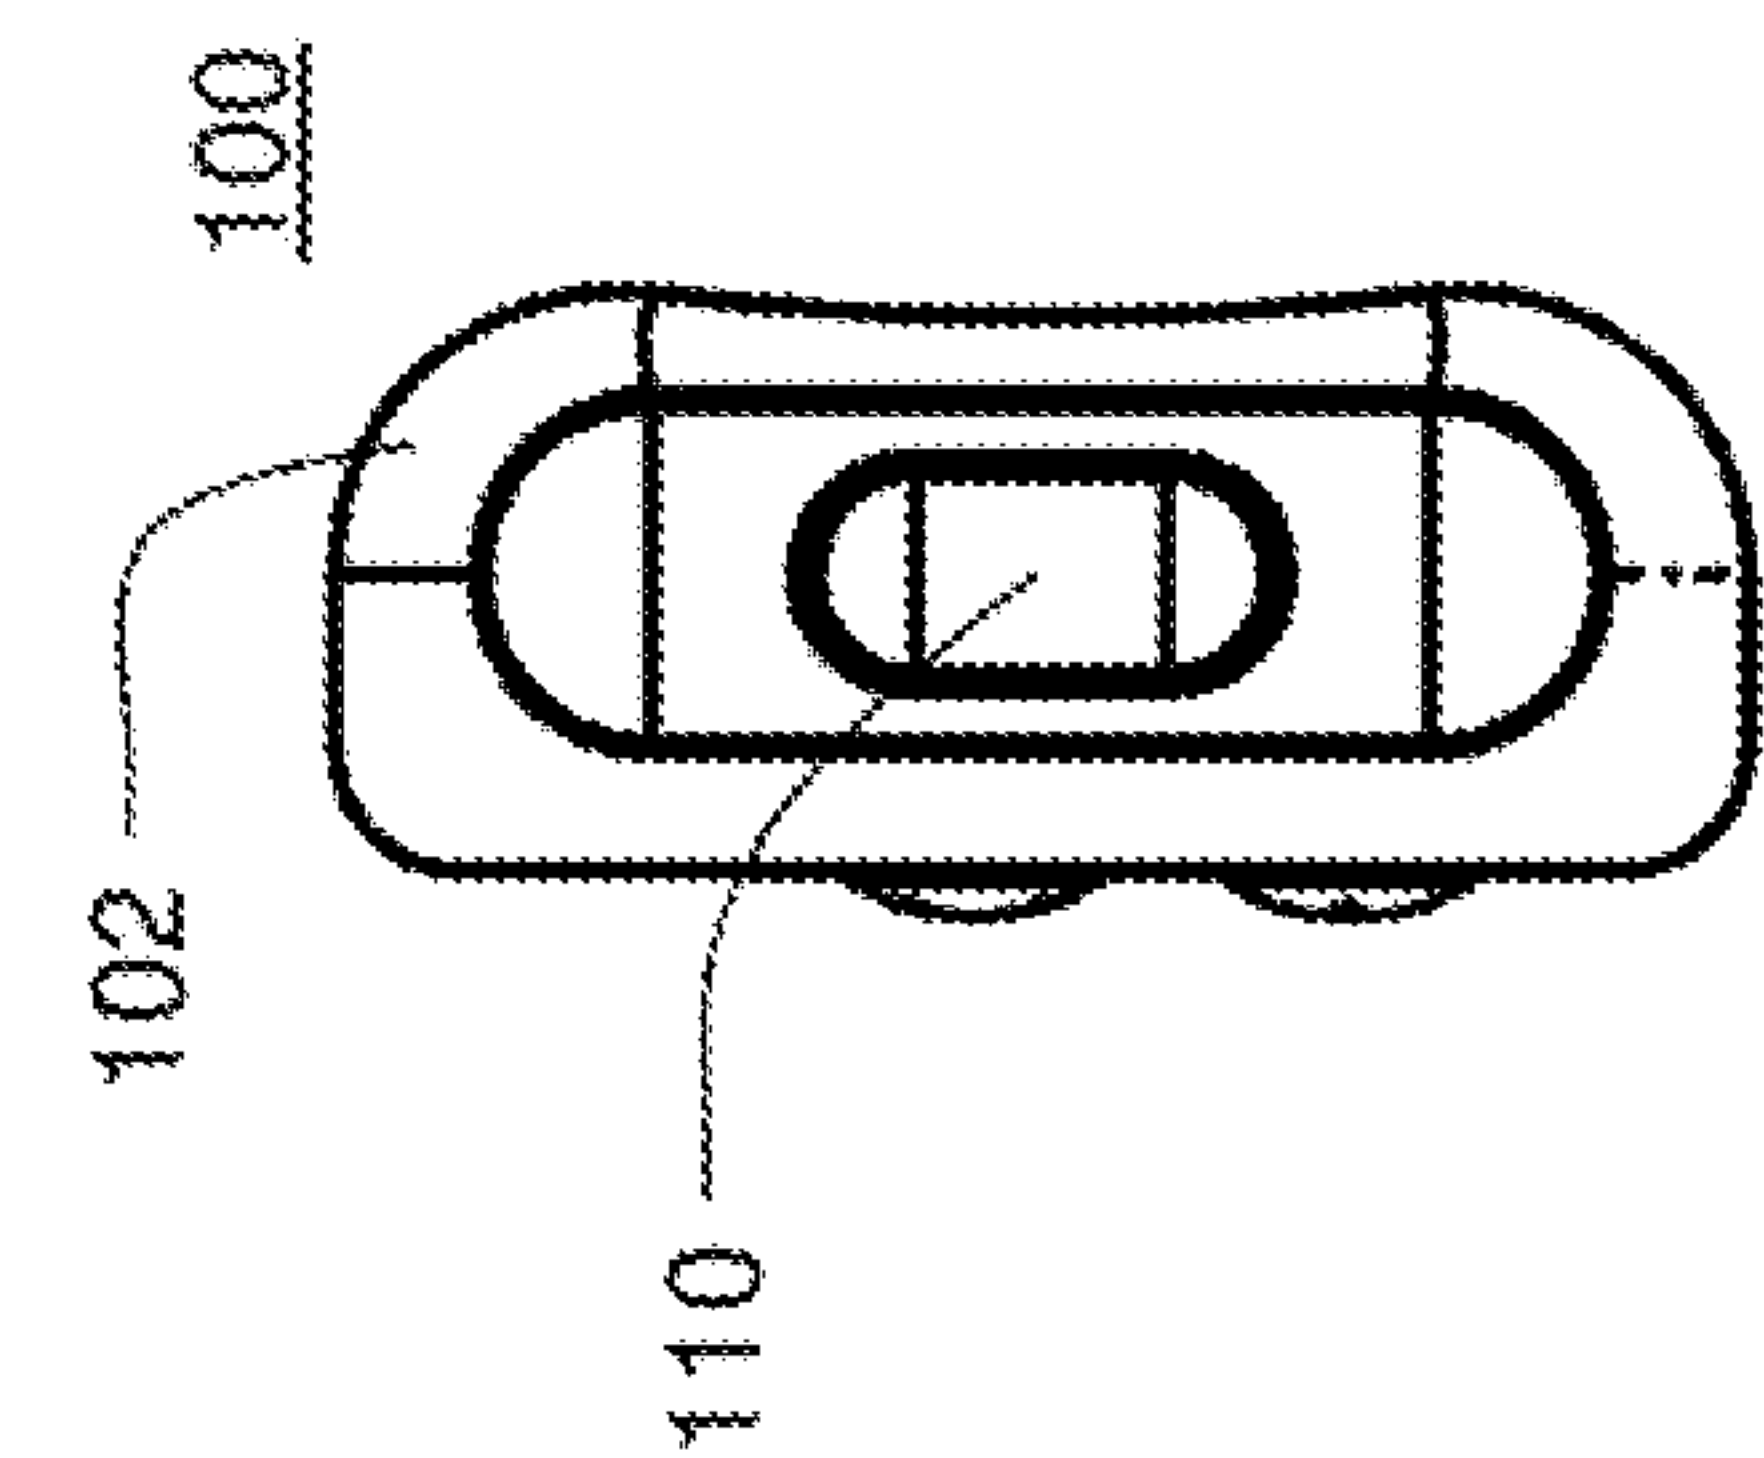


FIG. 1E

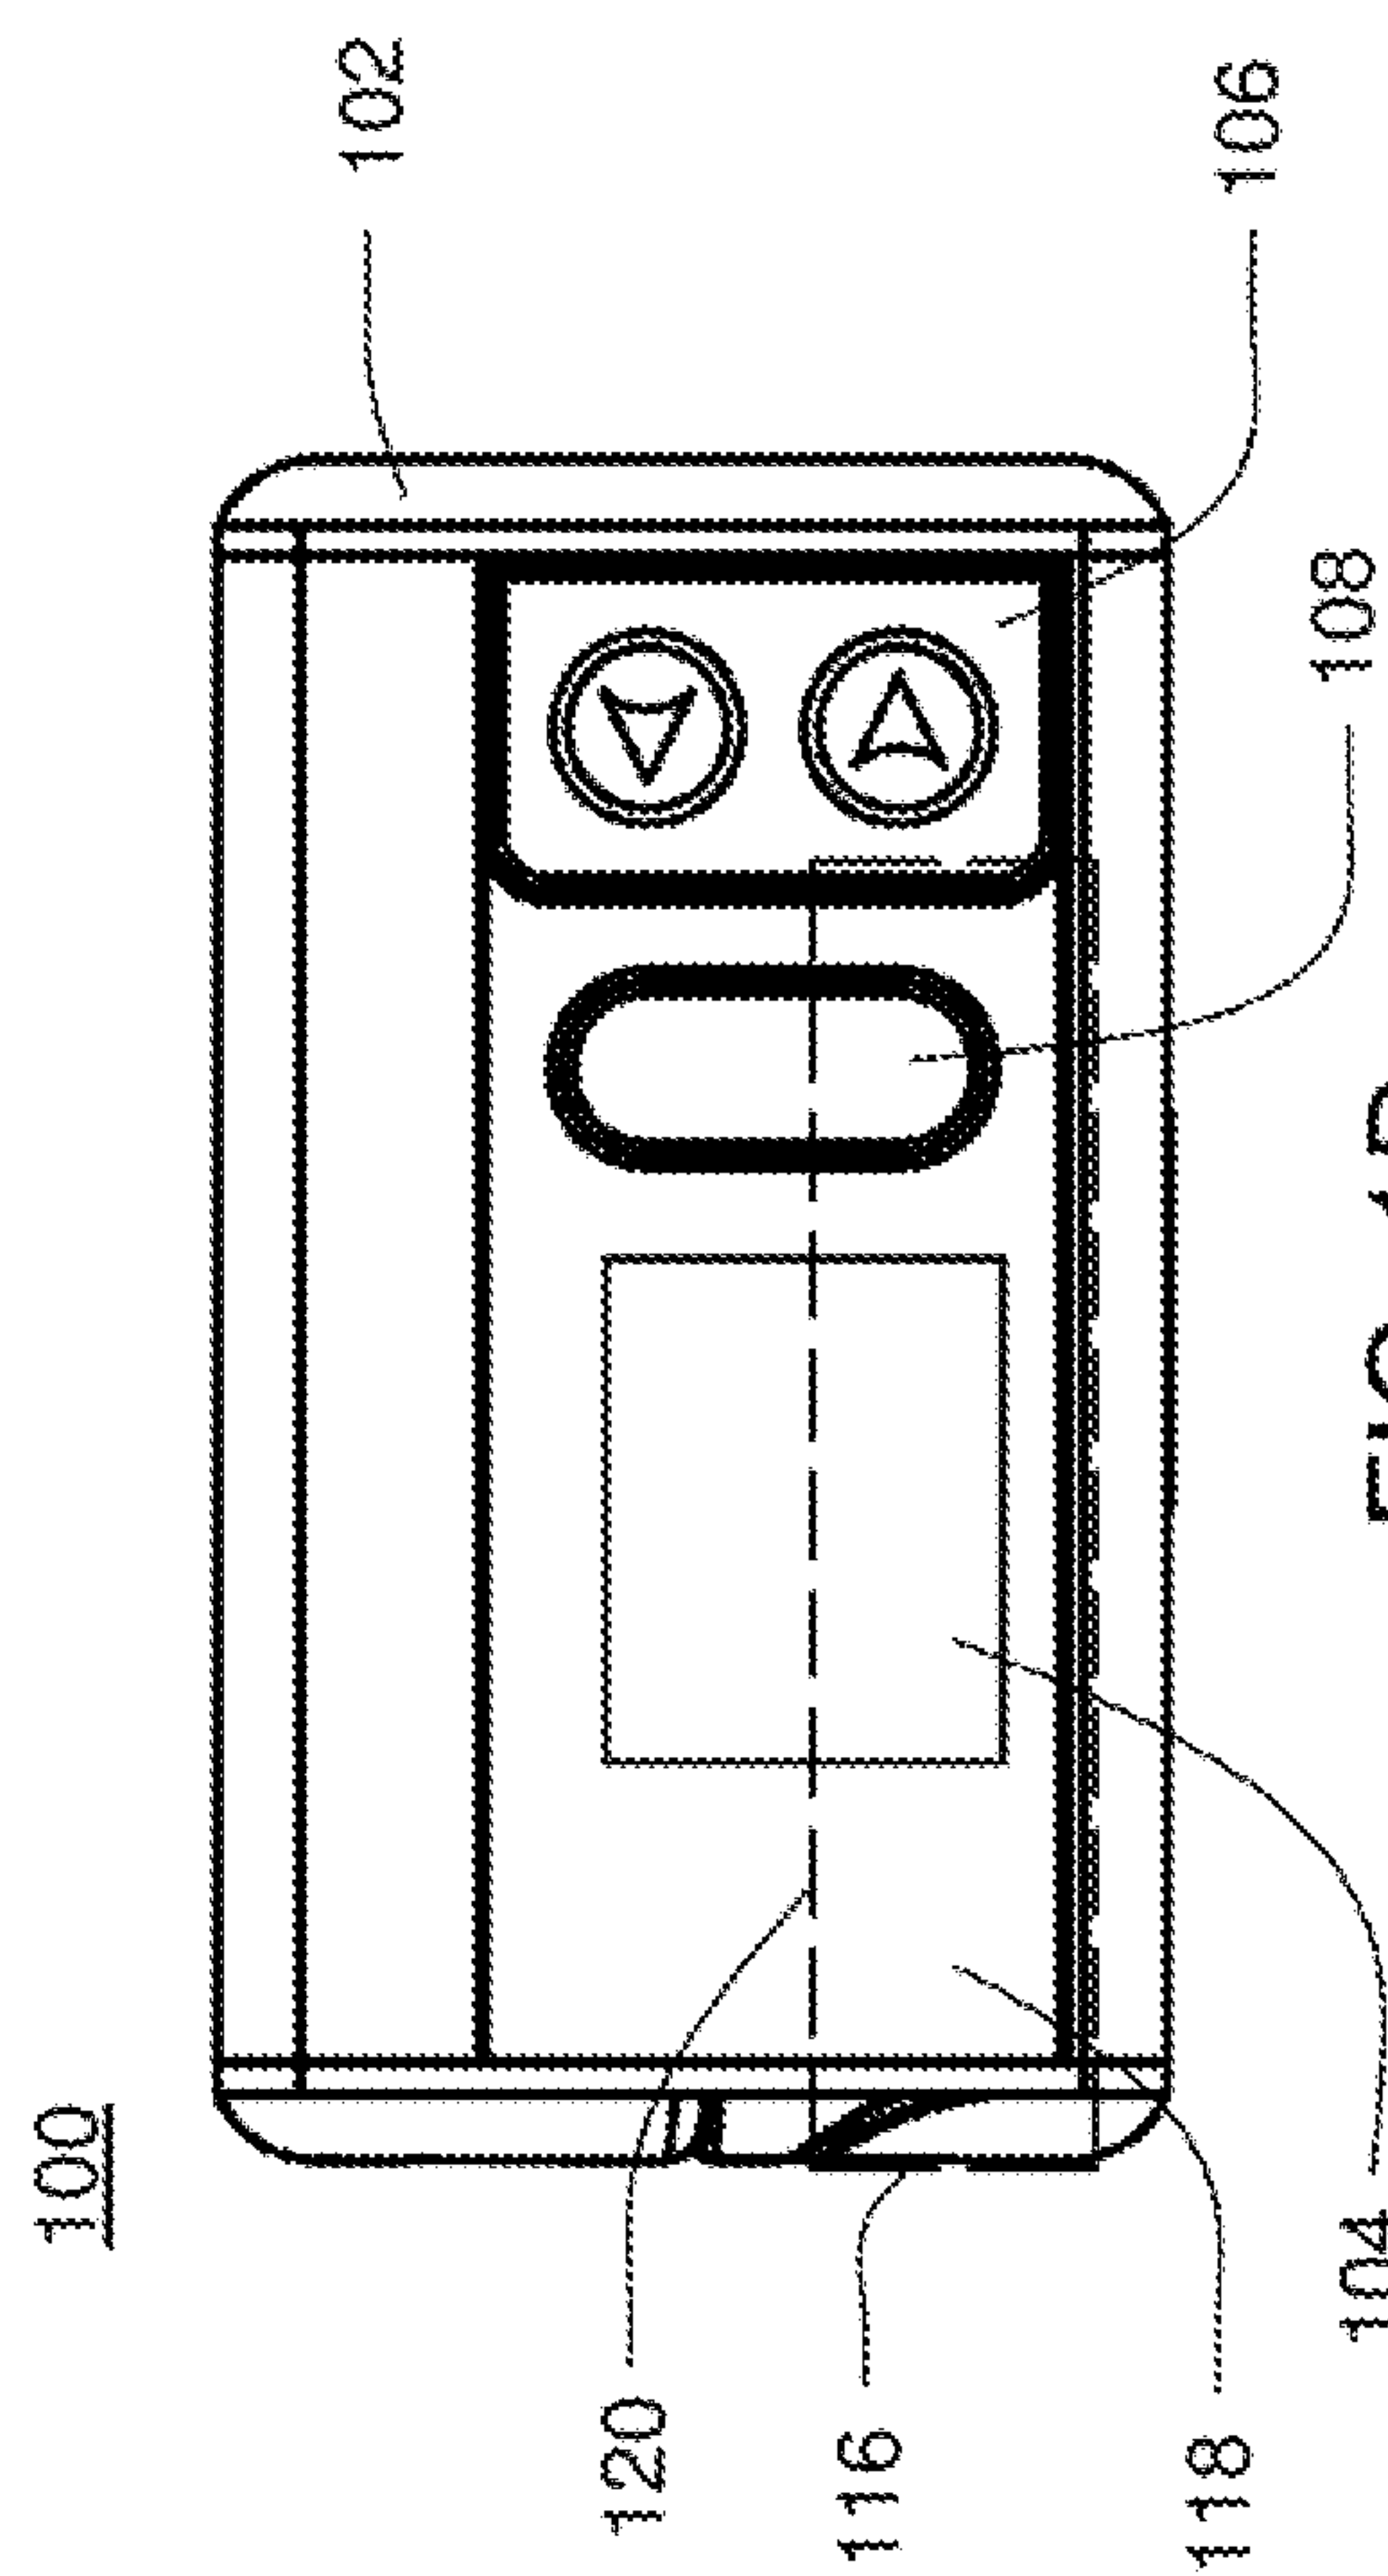


FIG. 1D

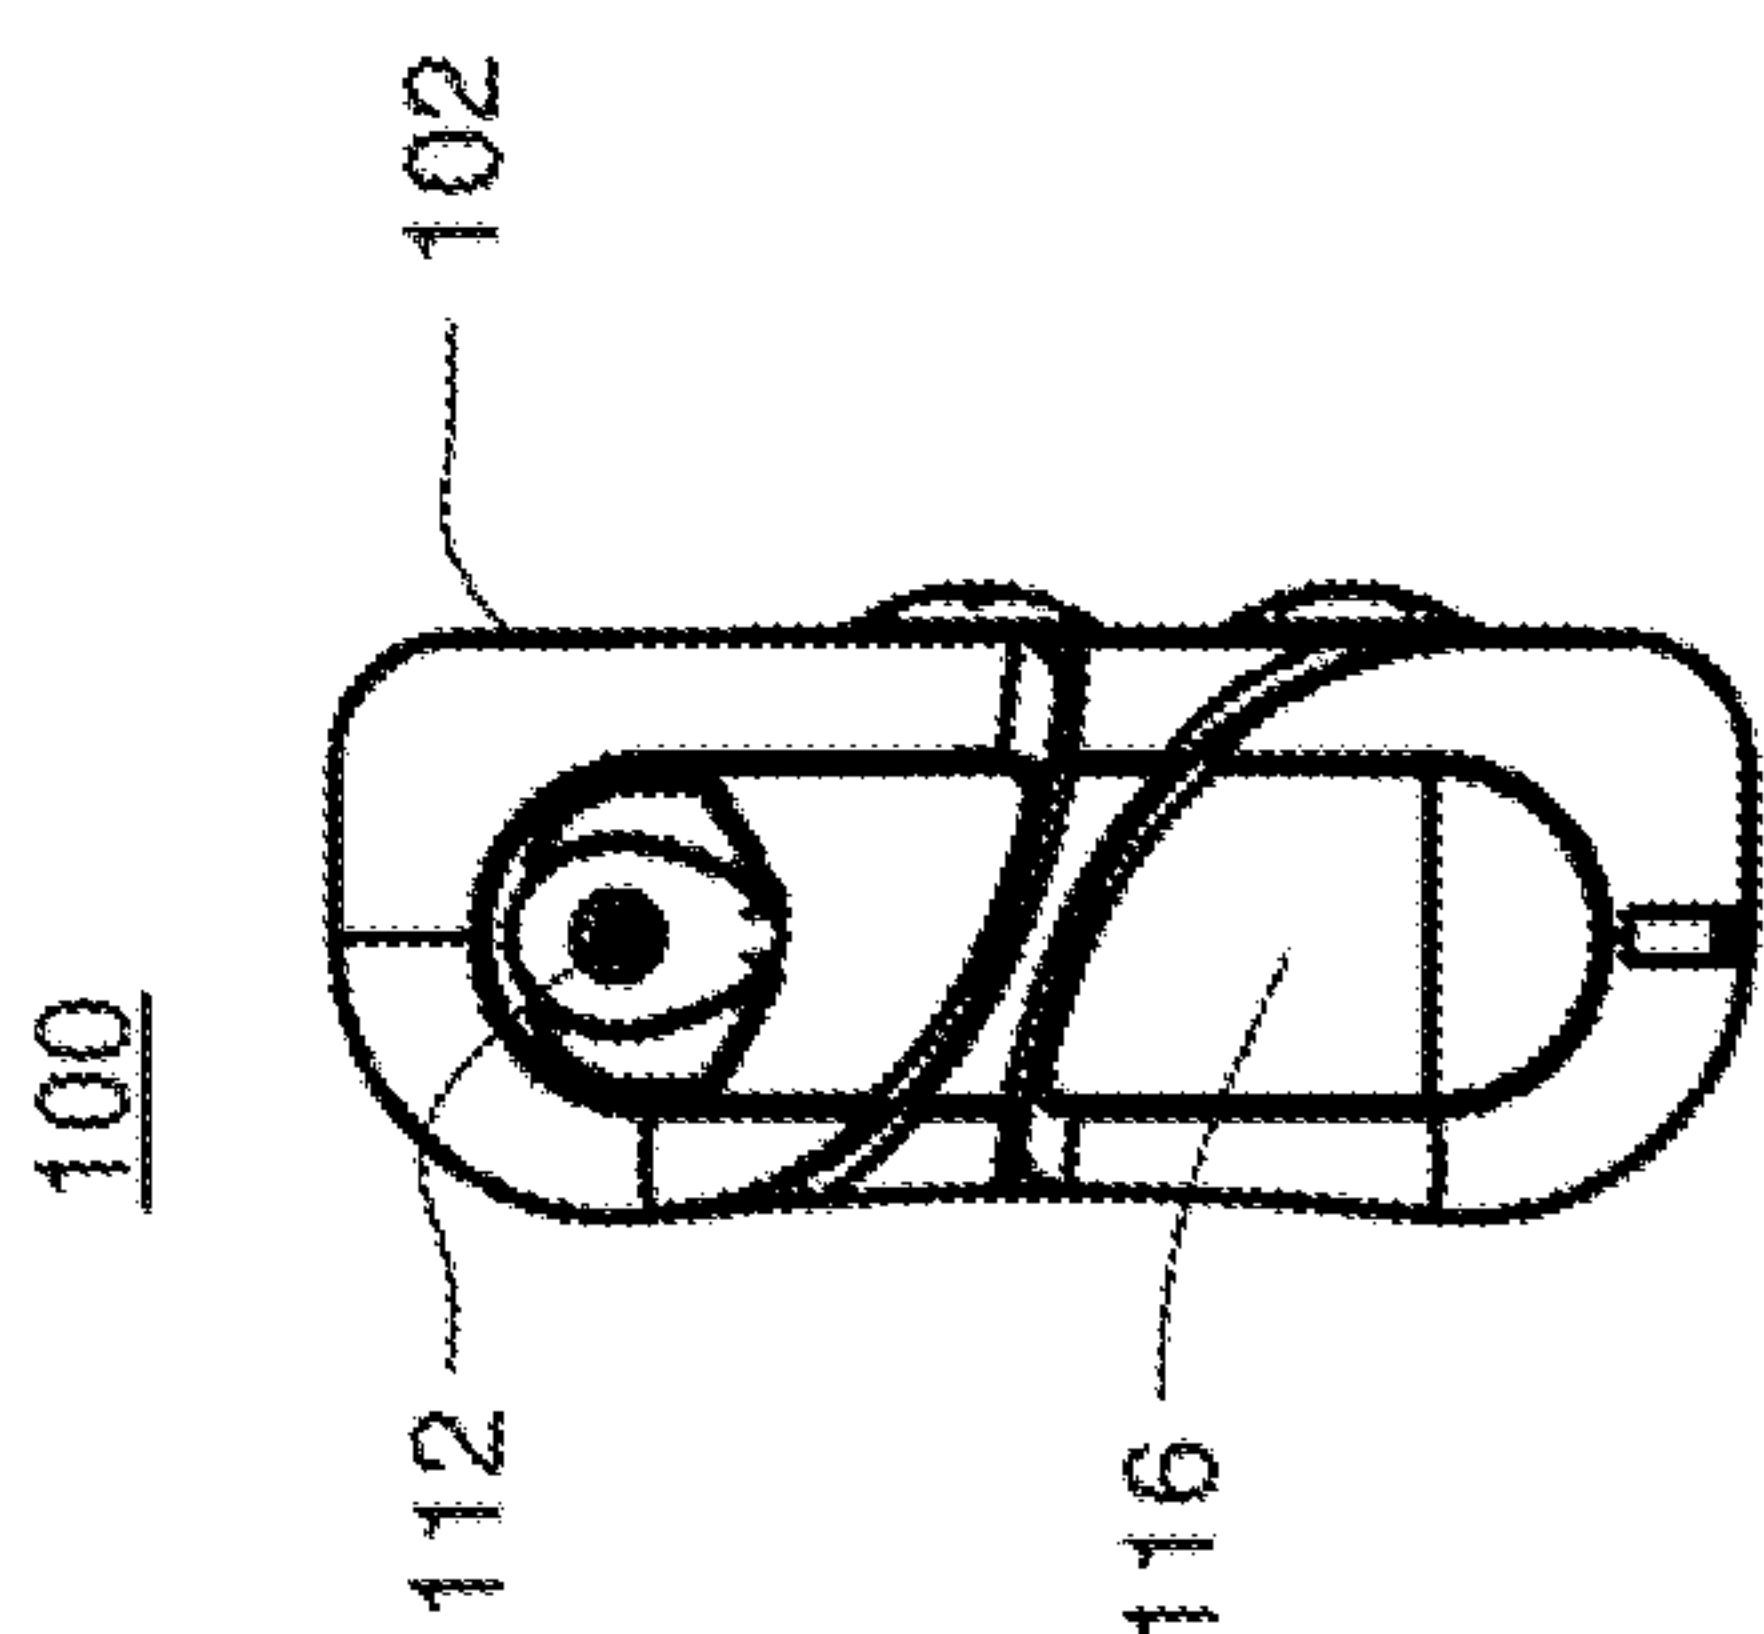


FIG. 1C

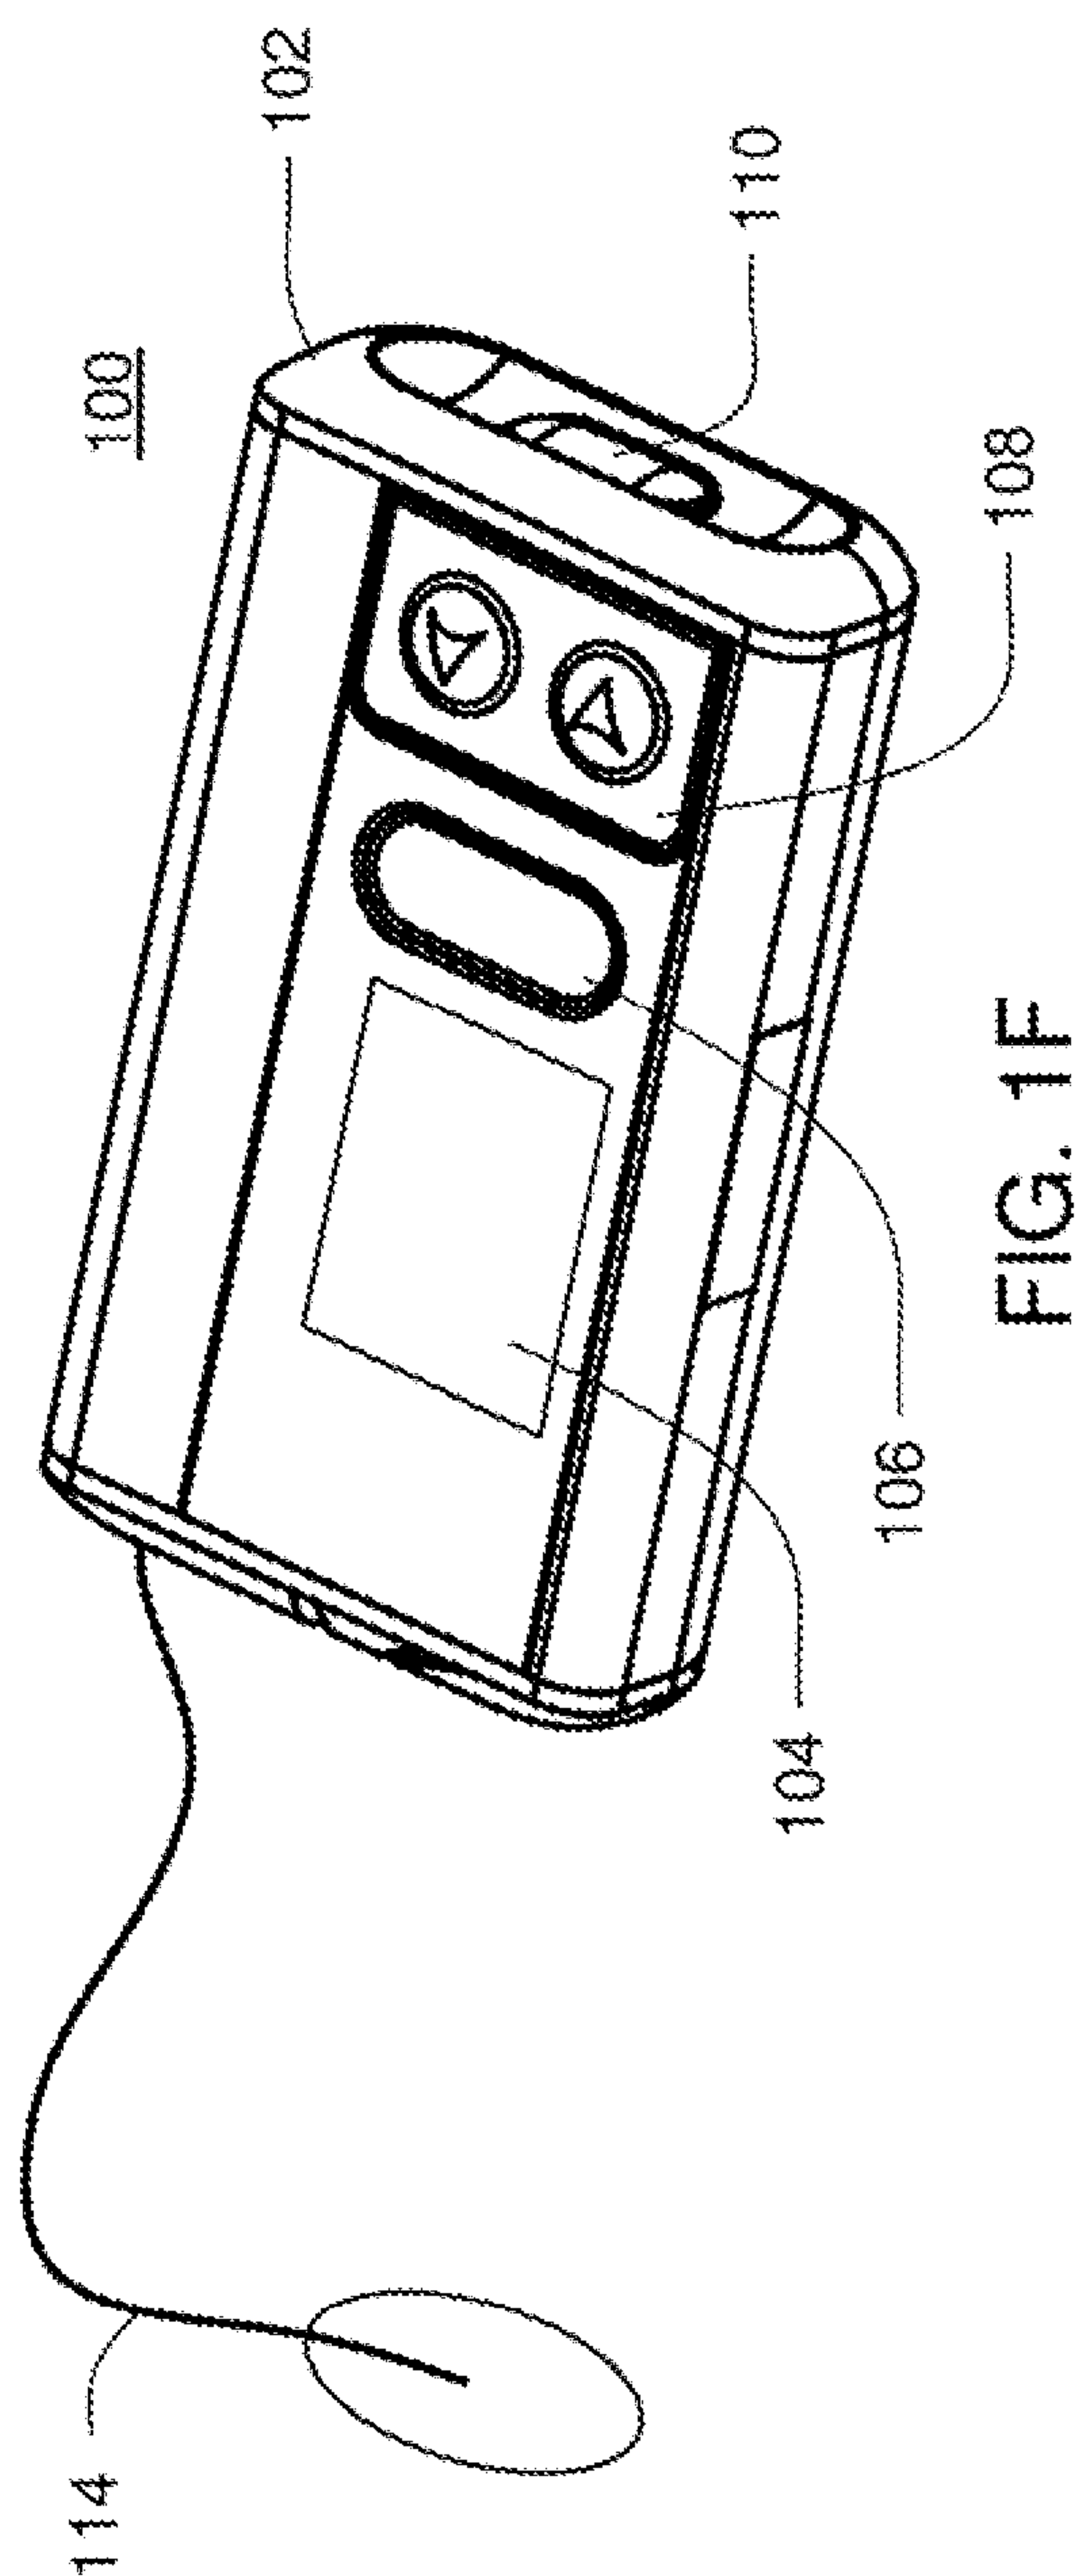


FIG. 1F

3/42

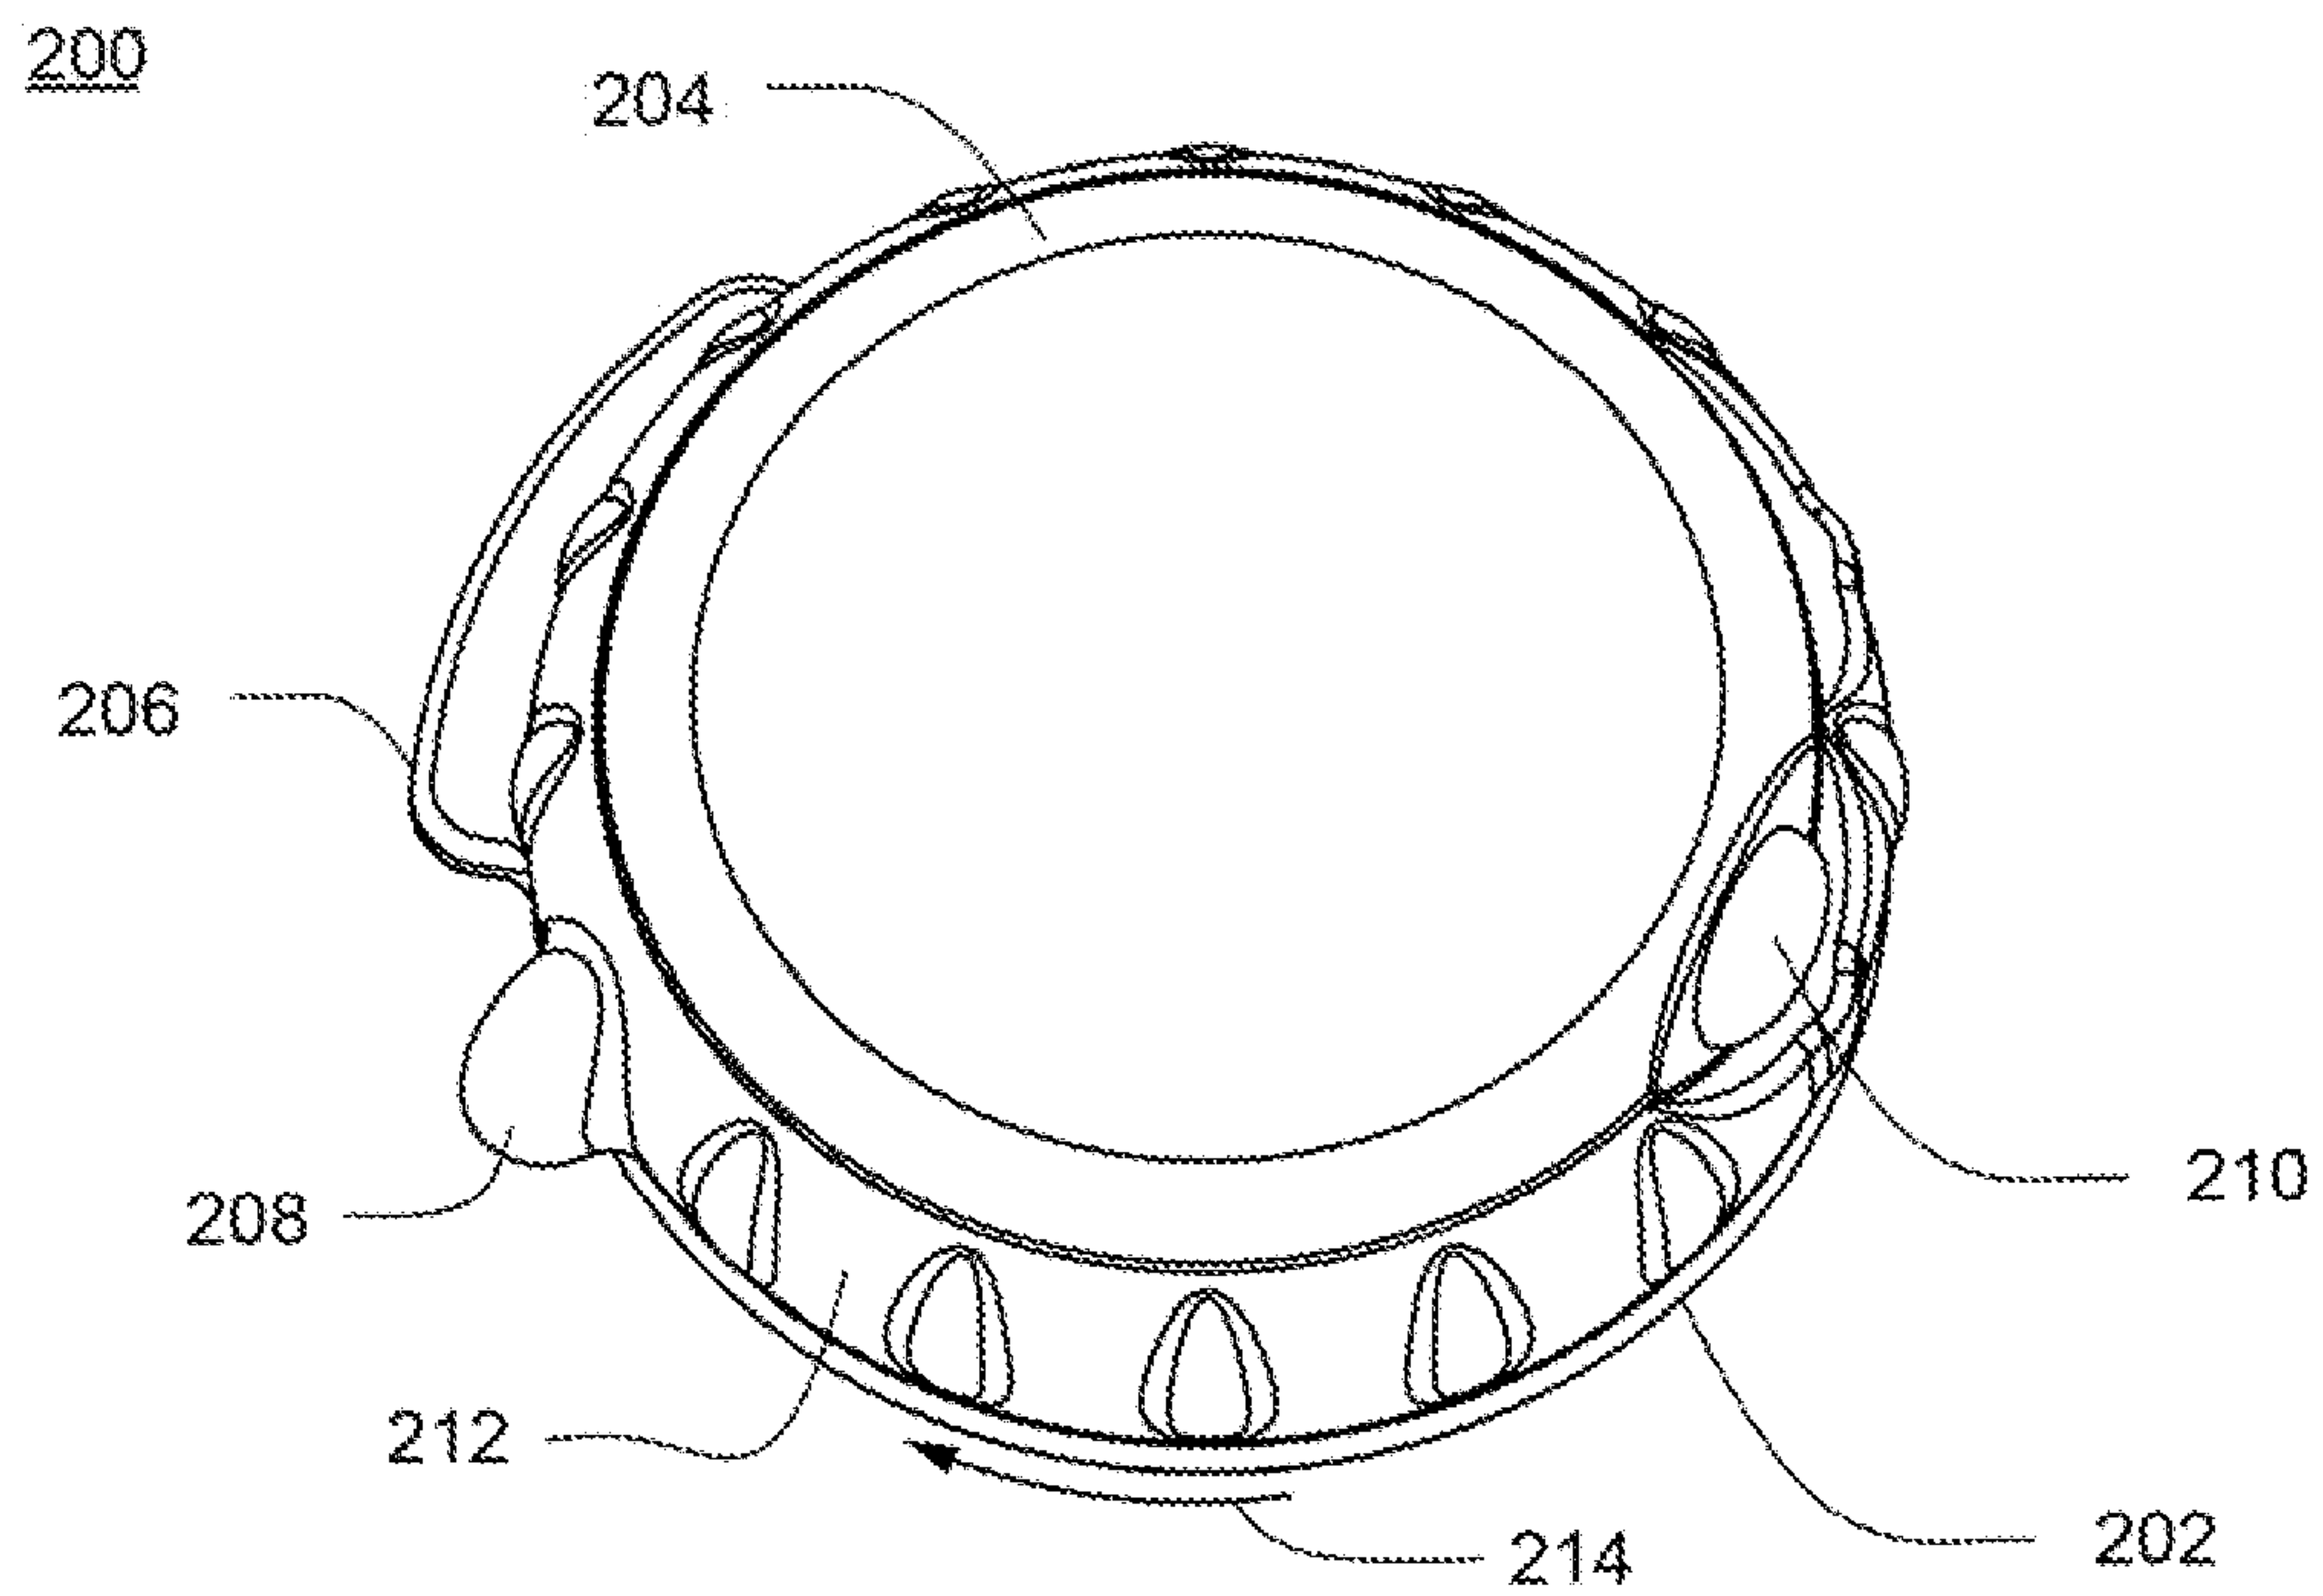


FIG. 2A

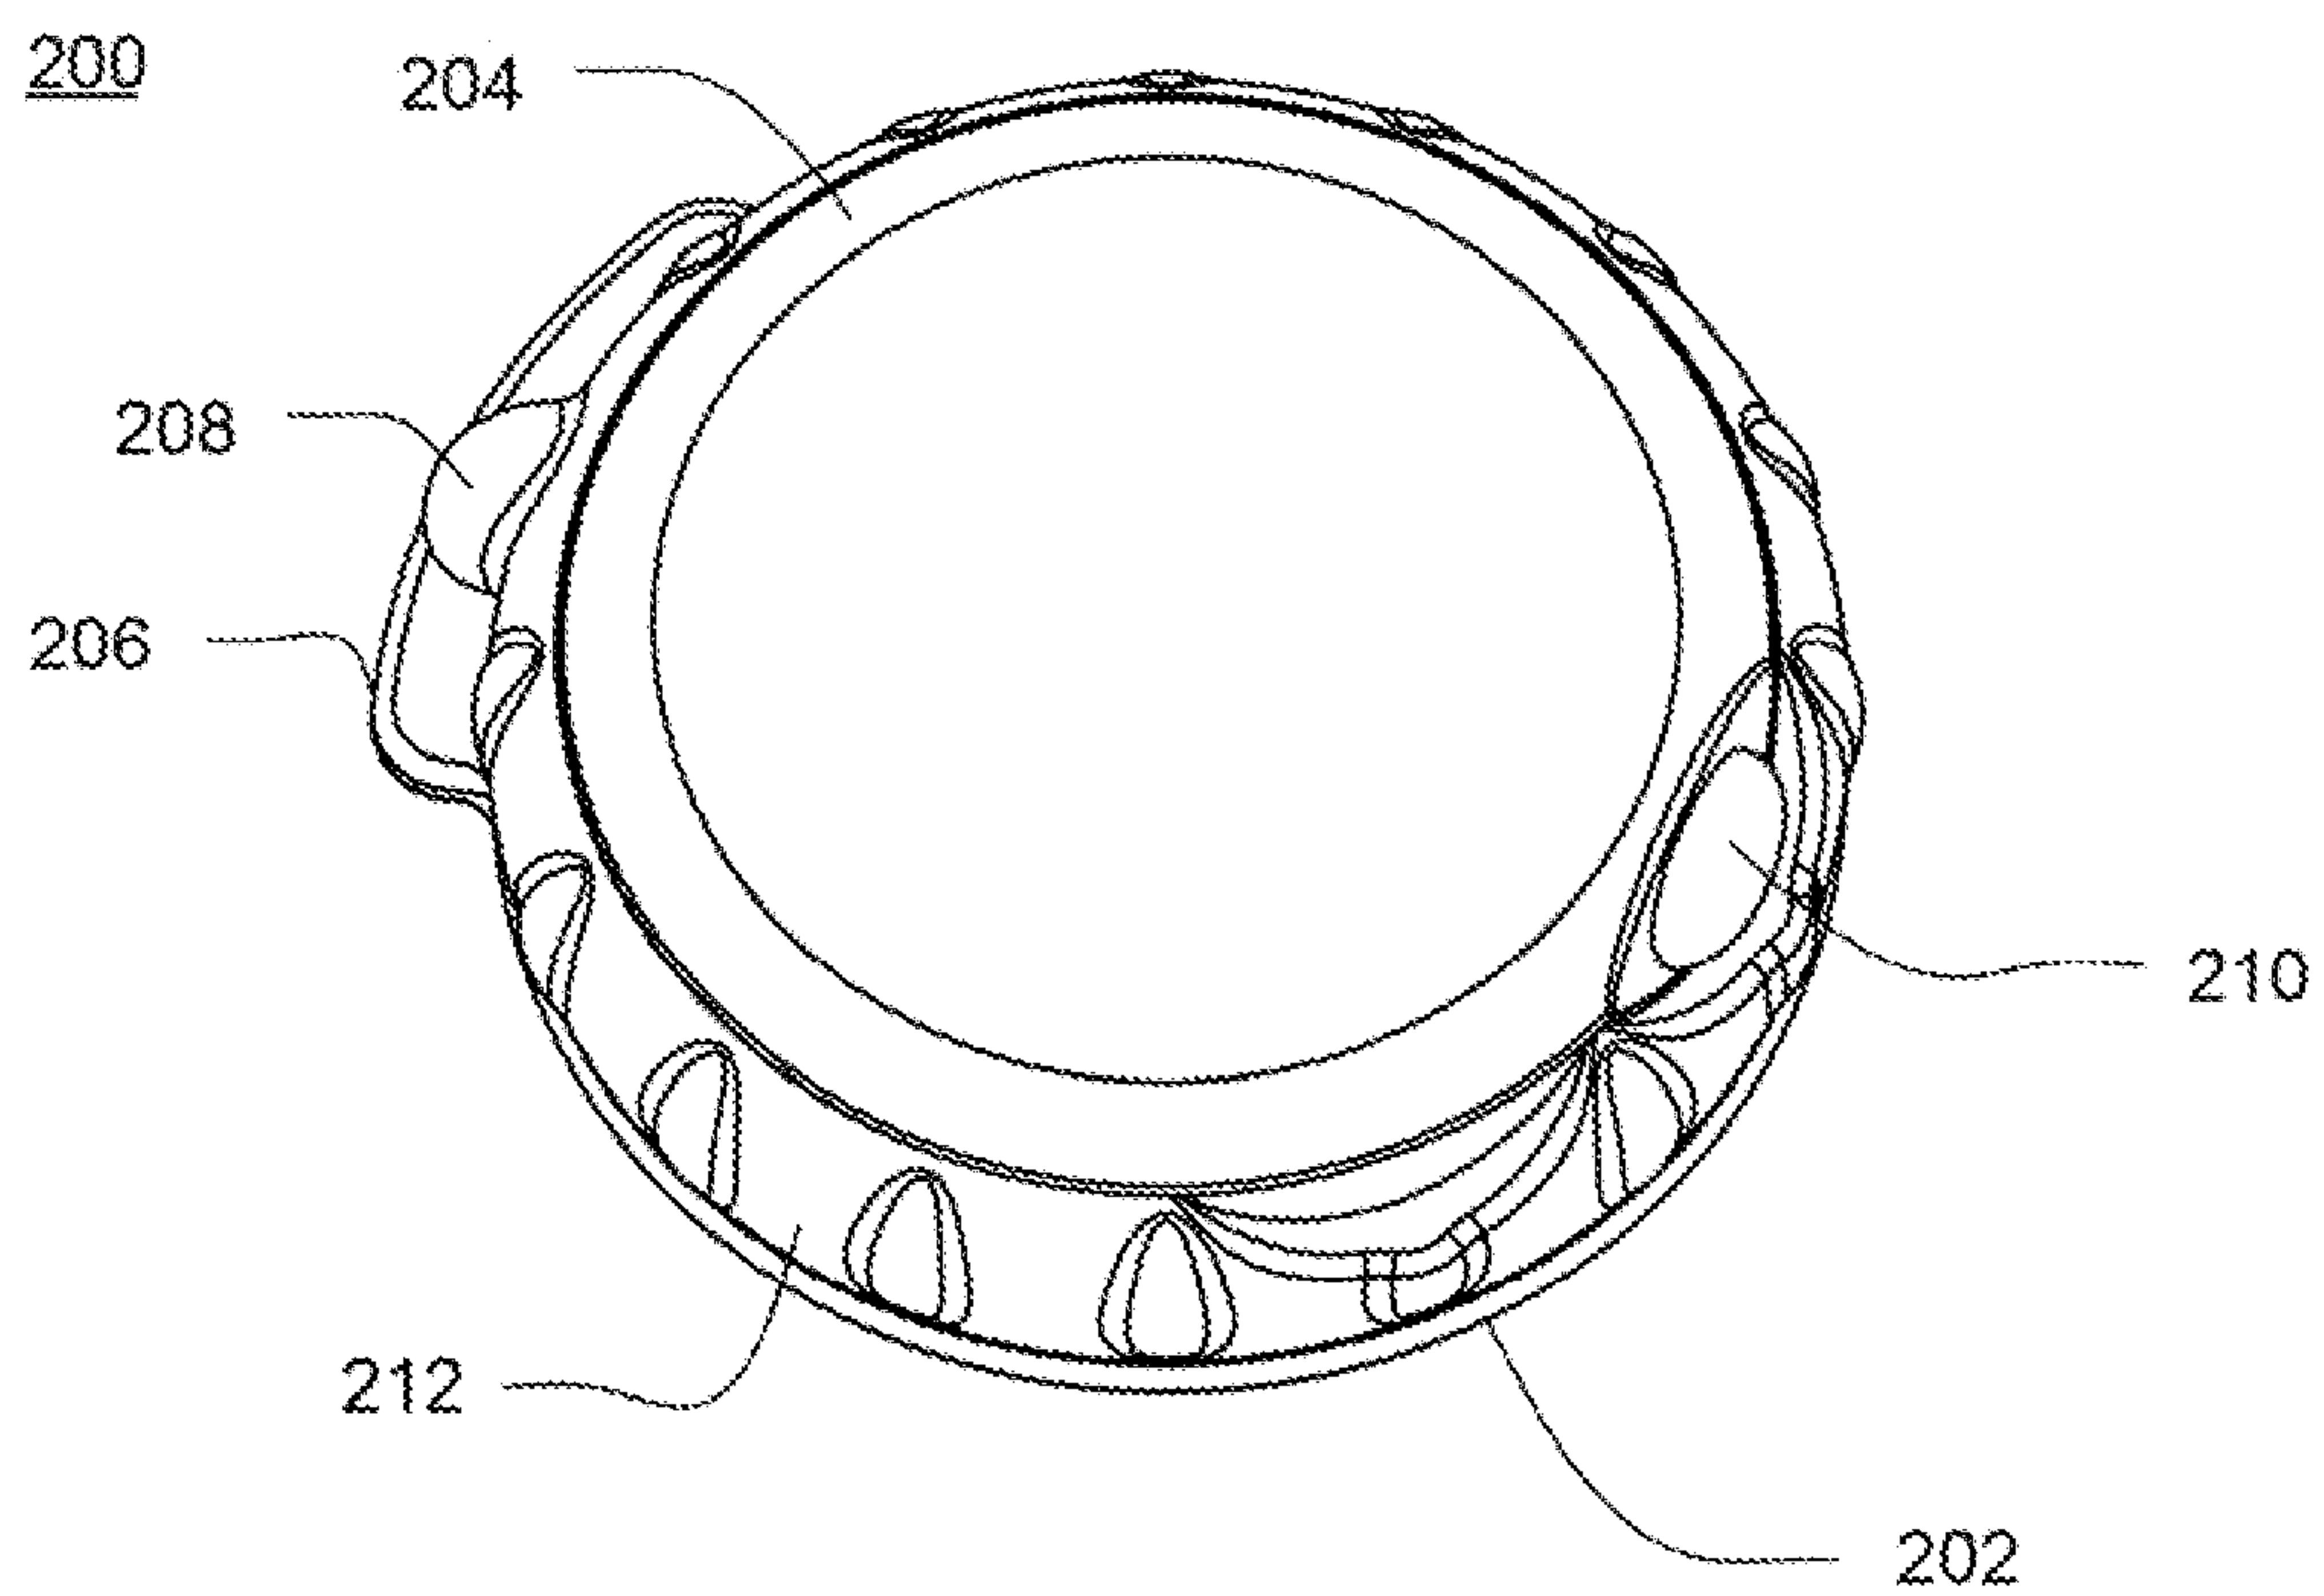


FIG. 2B

4/42


200

FIG. 2C


200

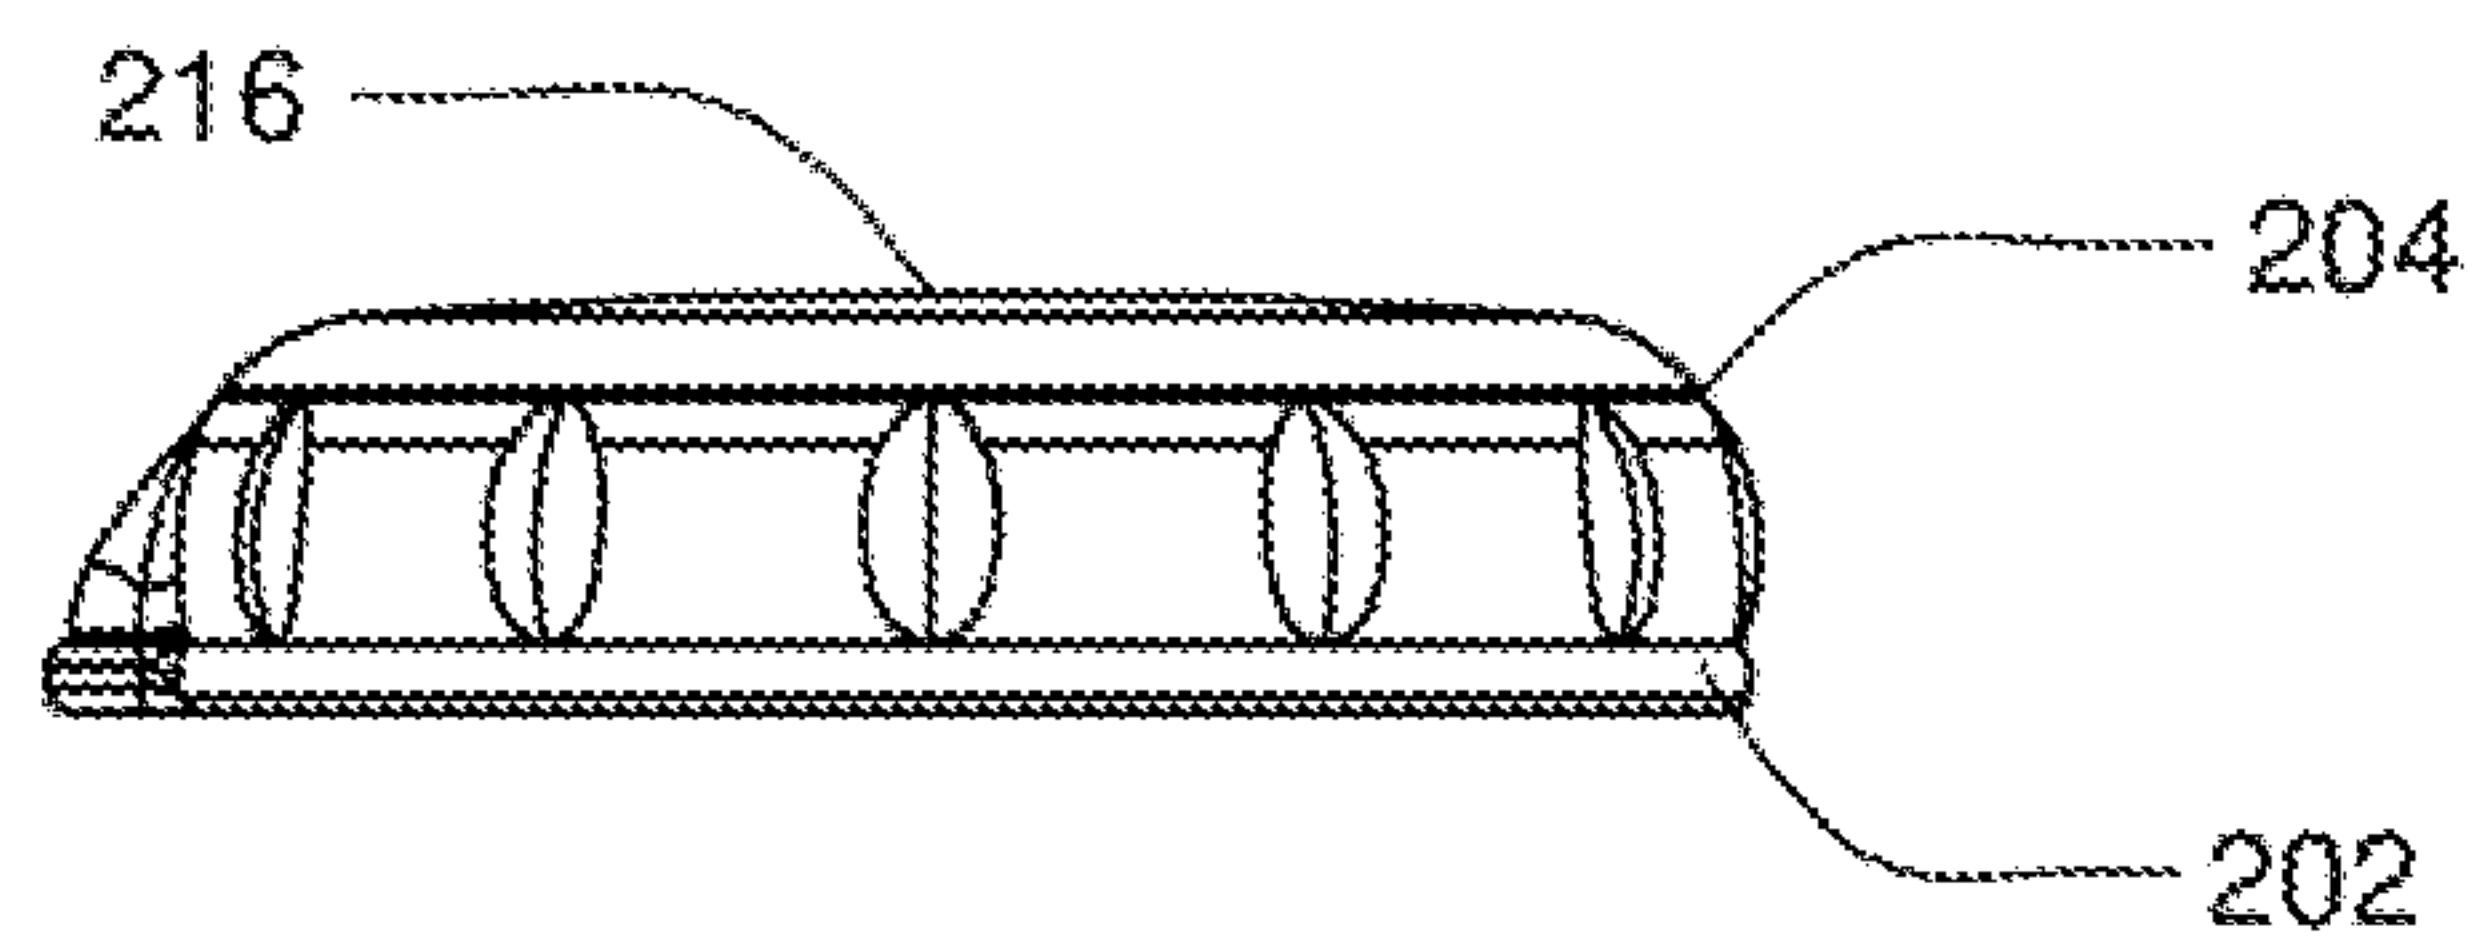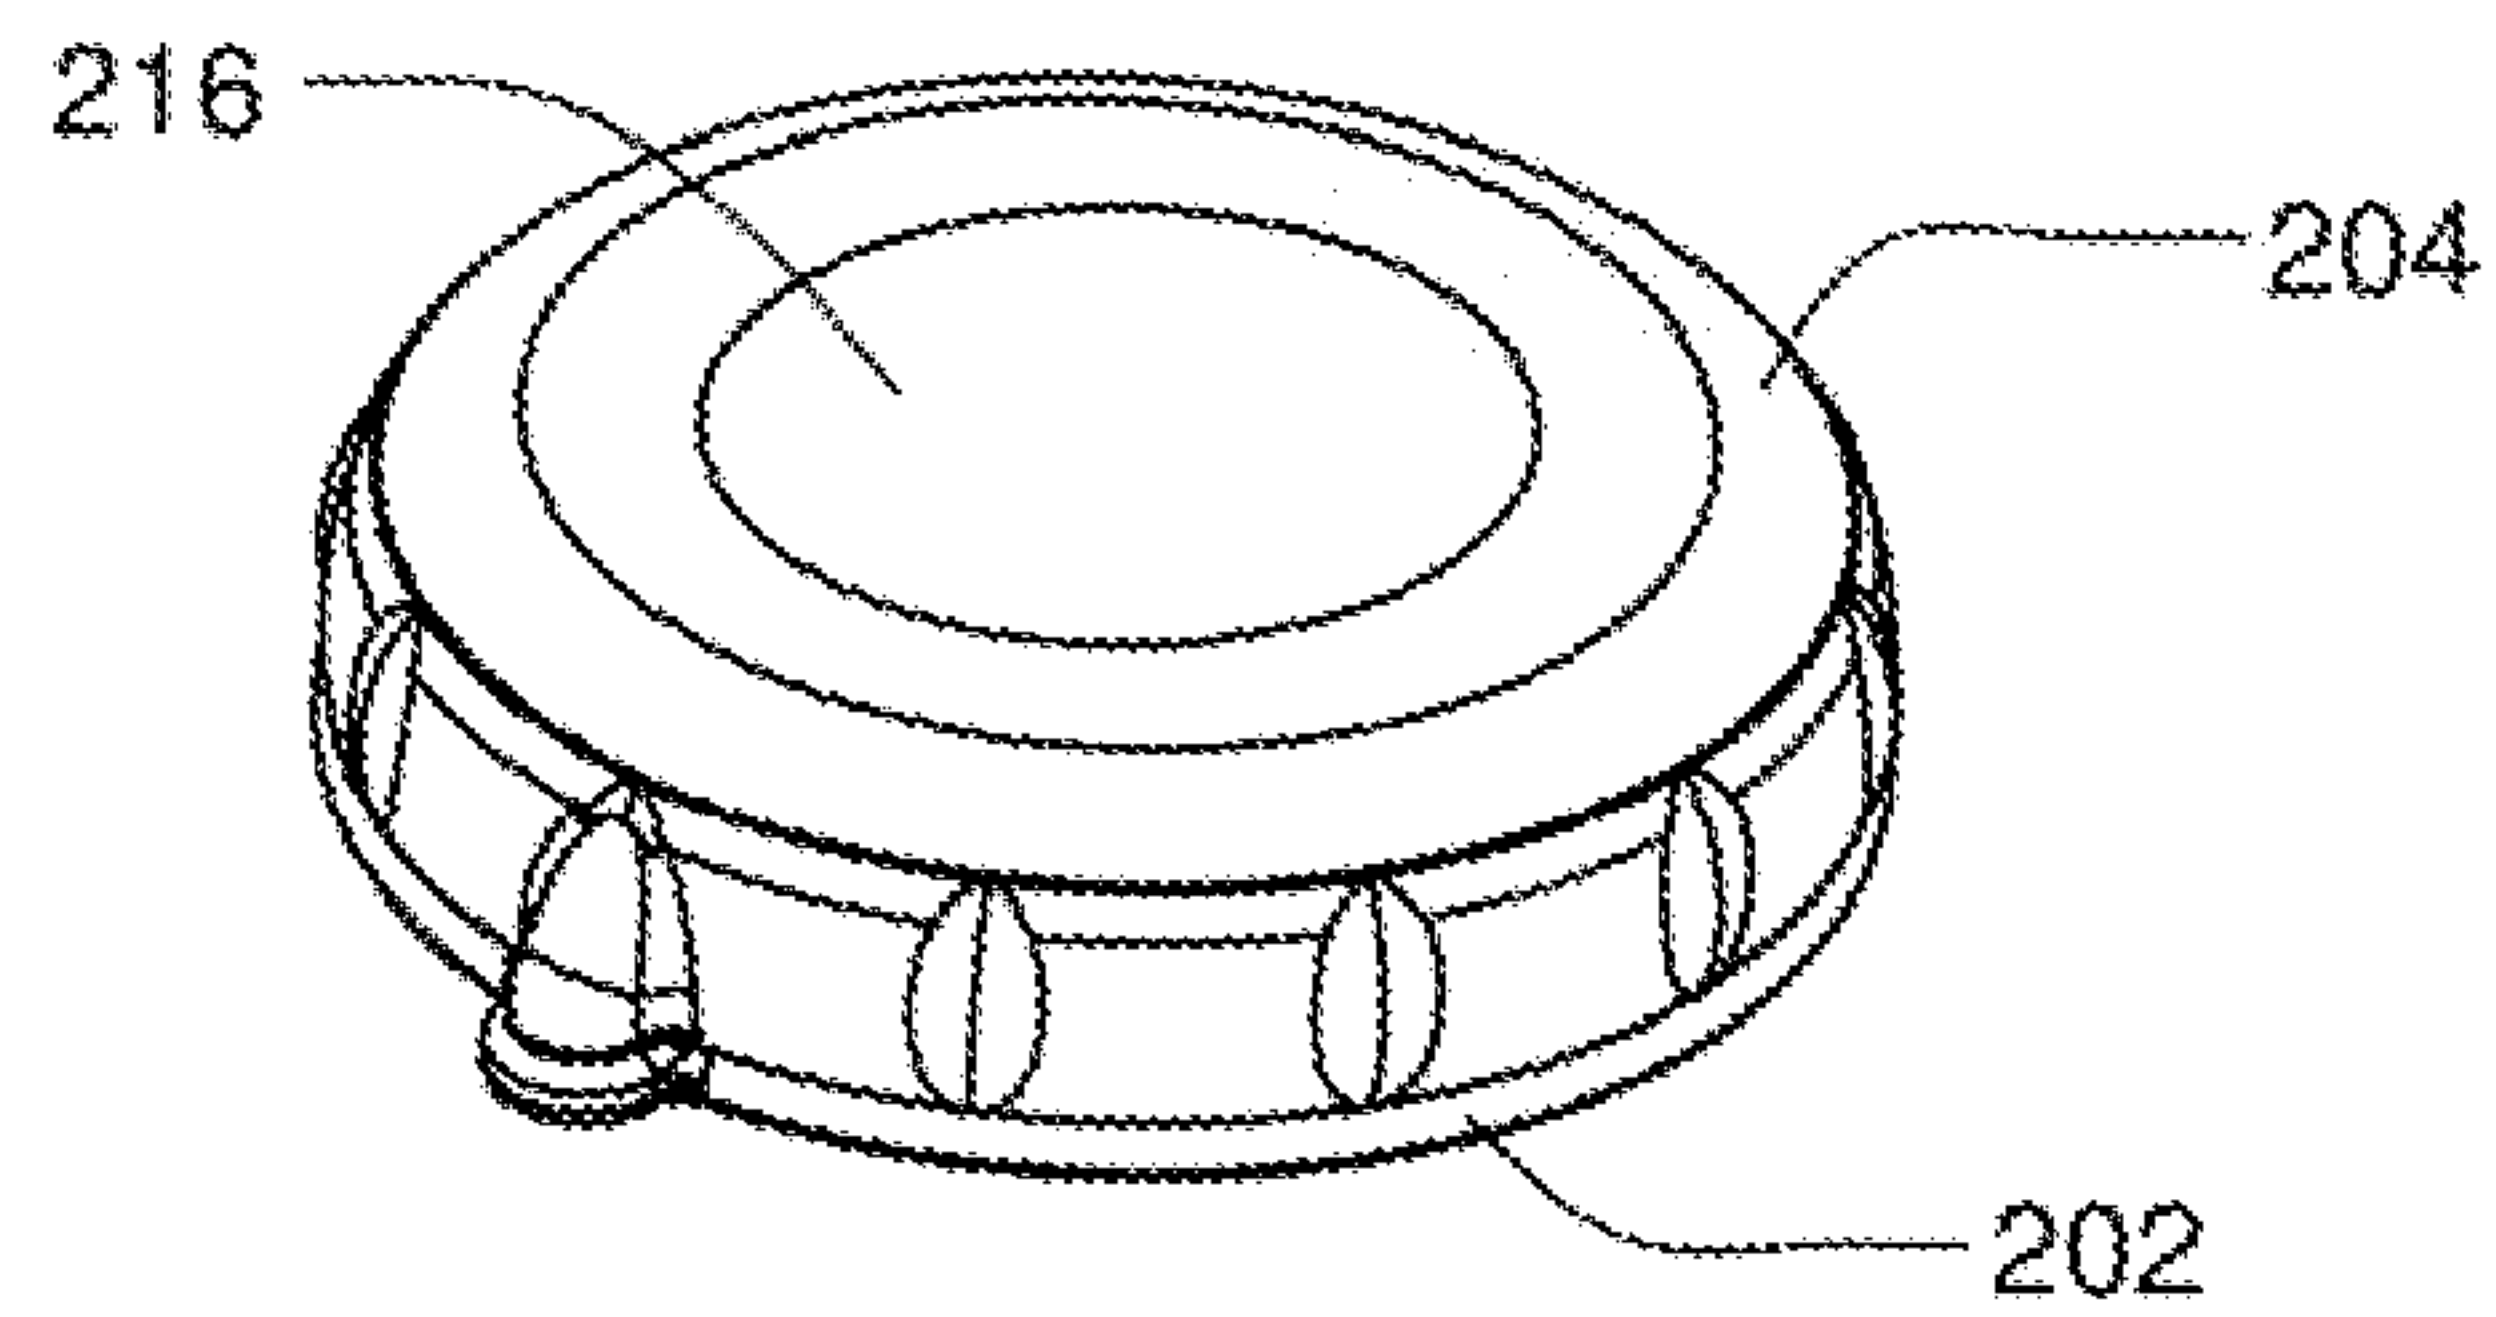FIG. 2D

5/42


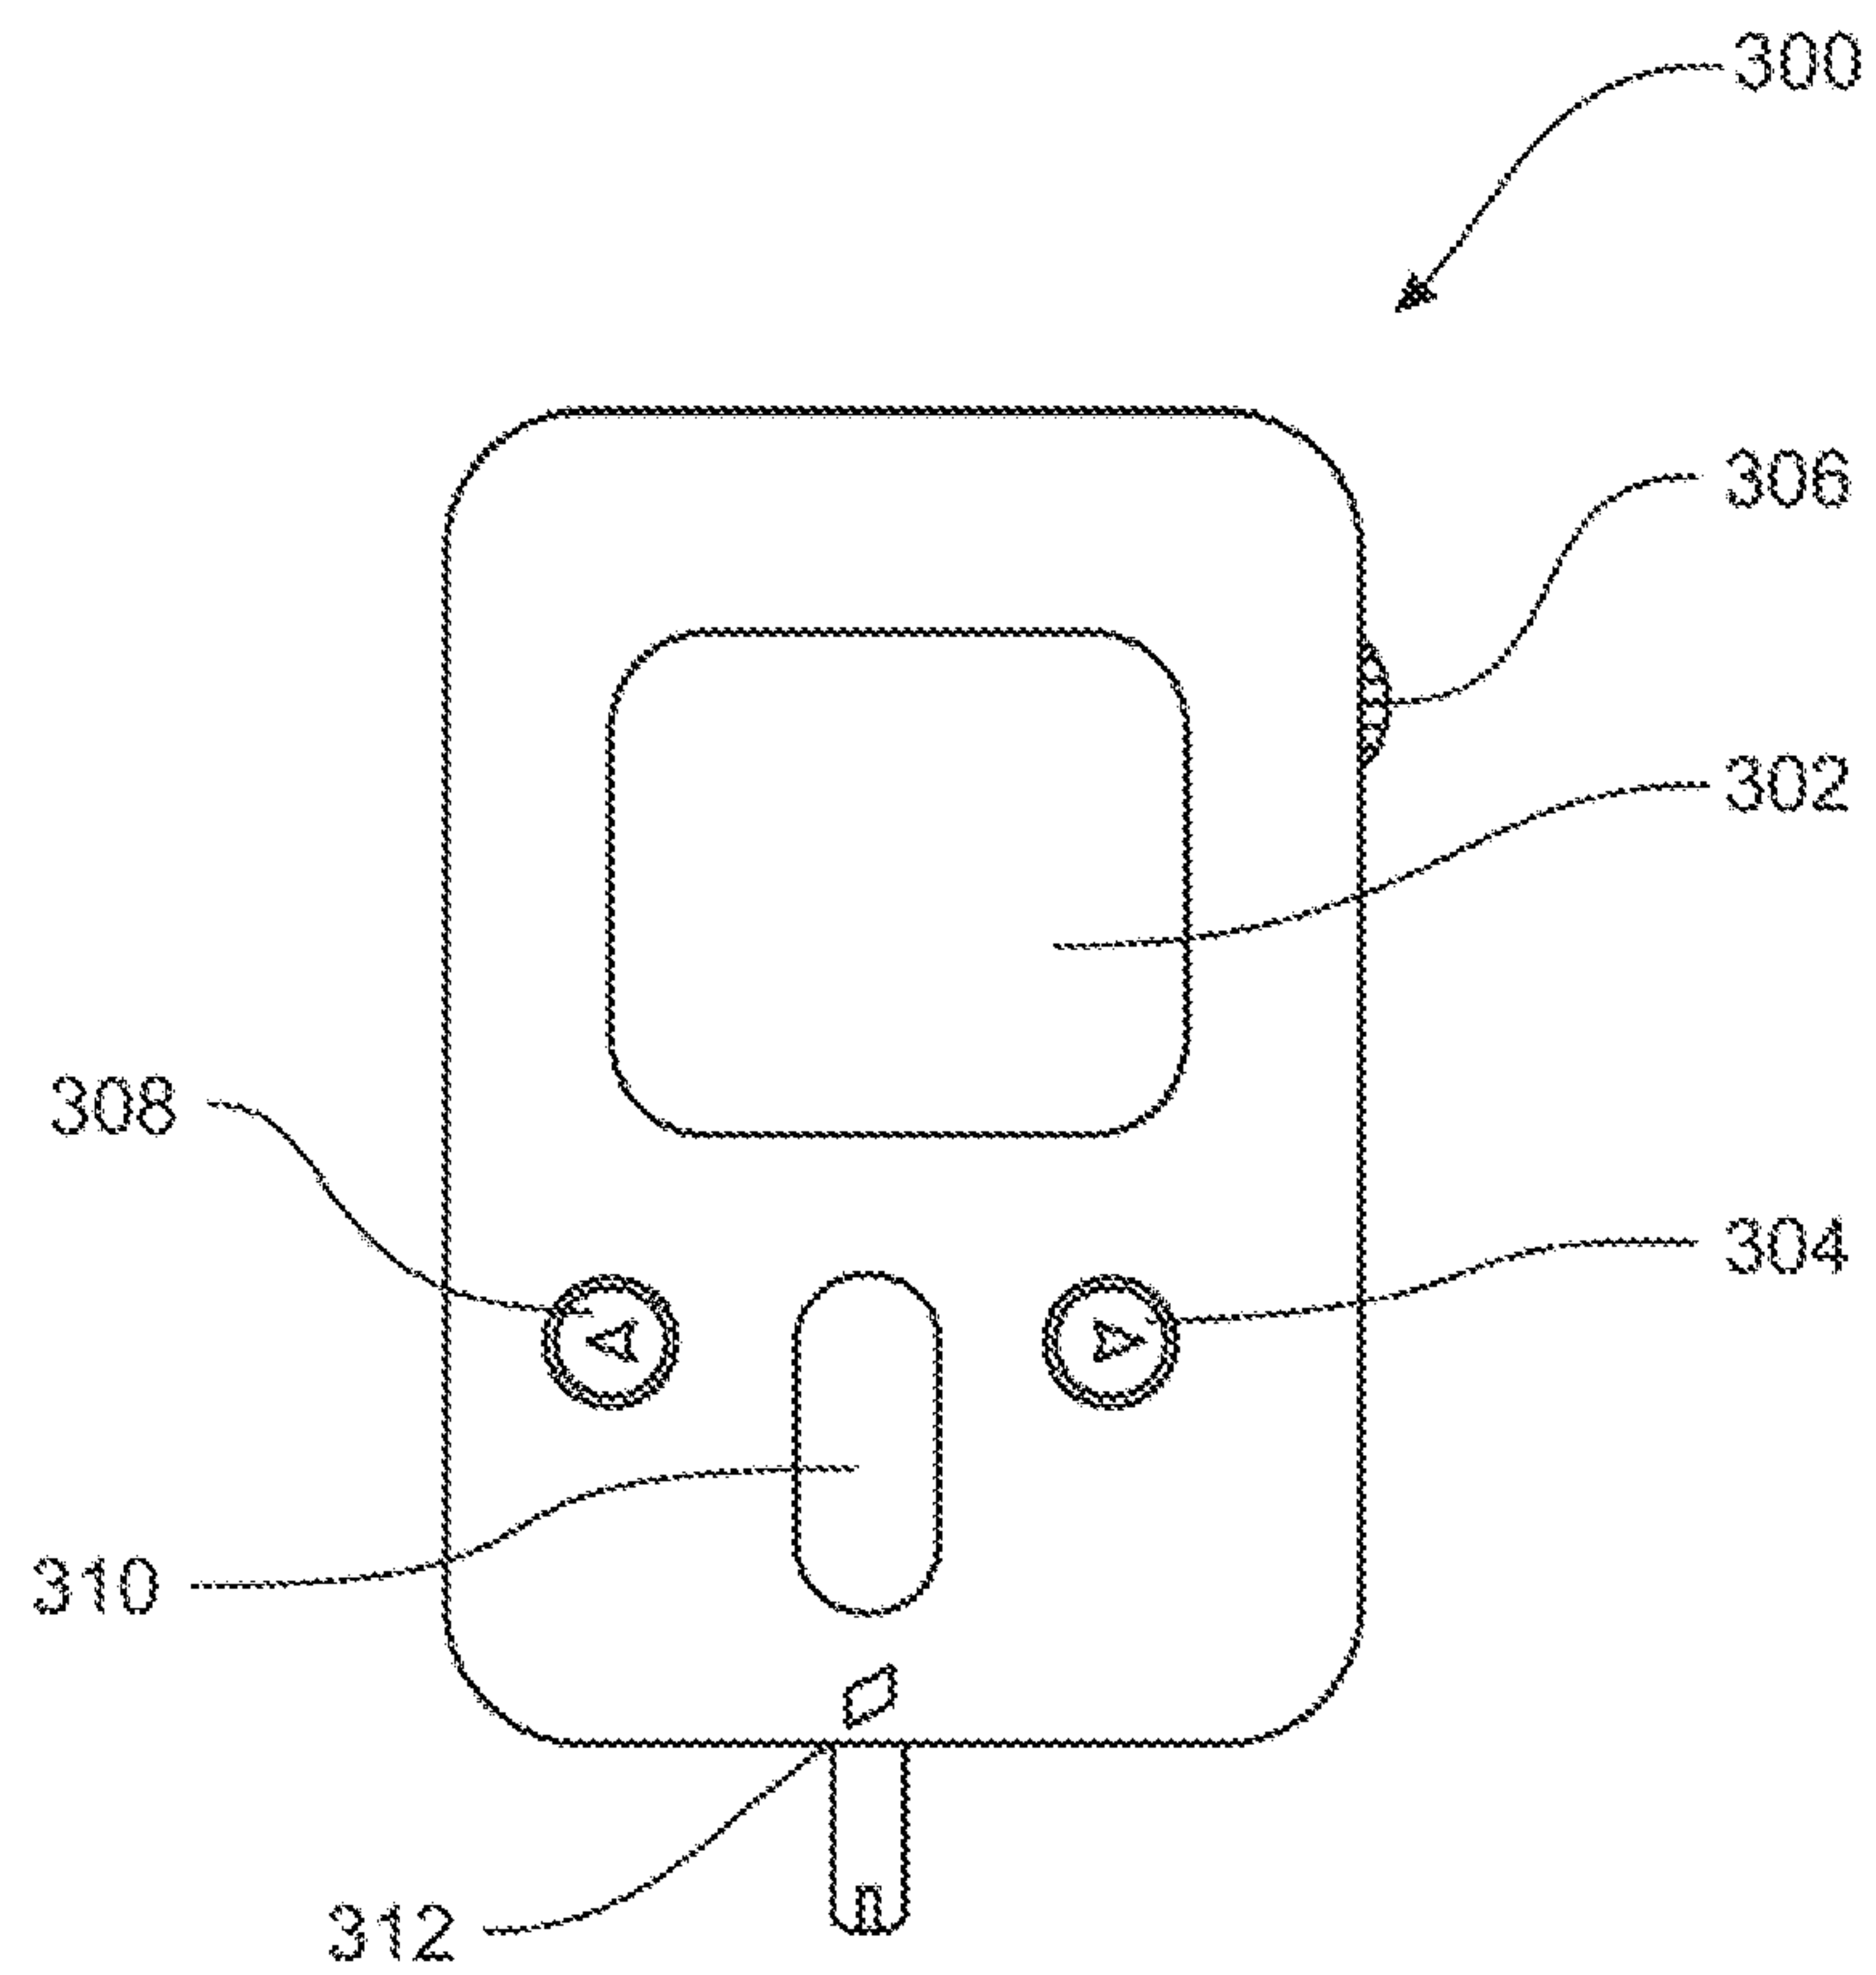


FIG. 3

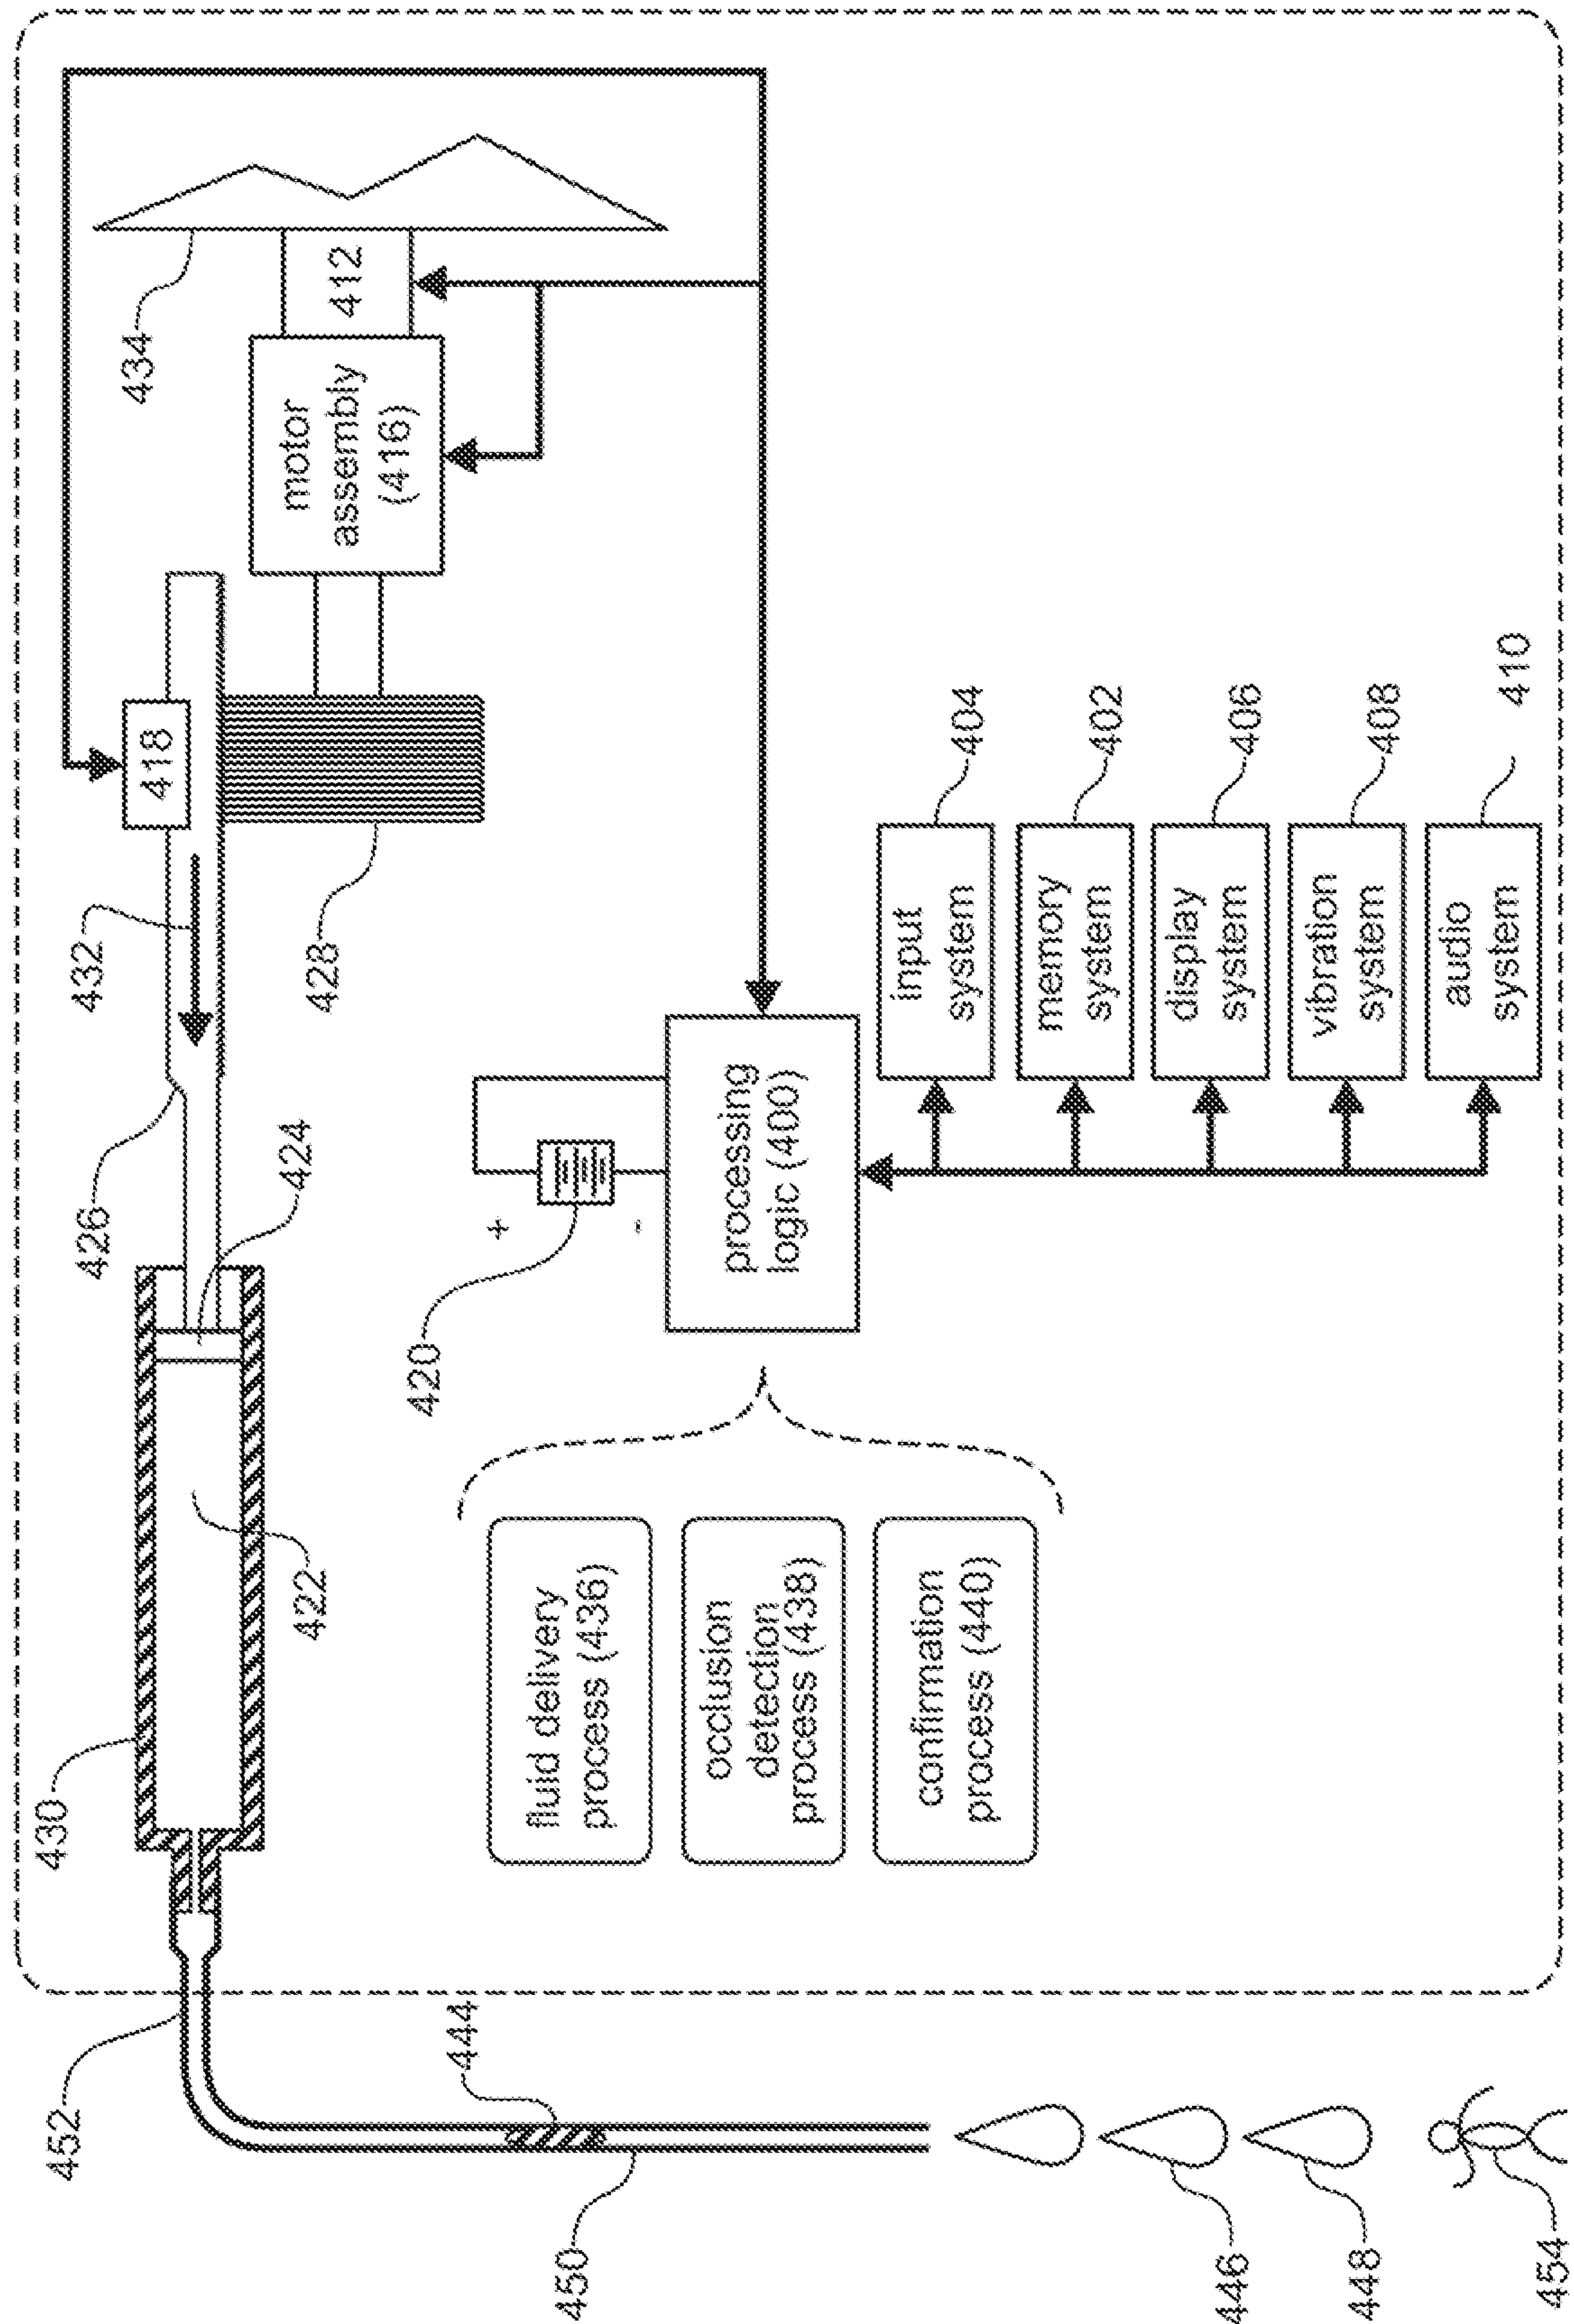

7/42

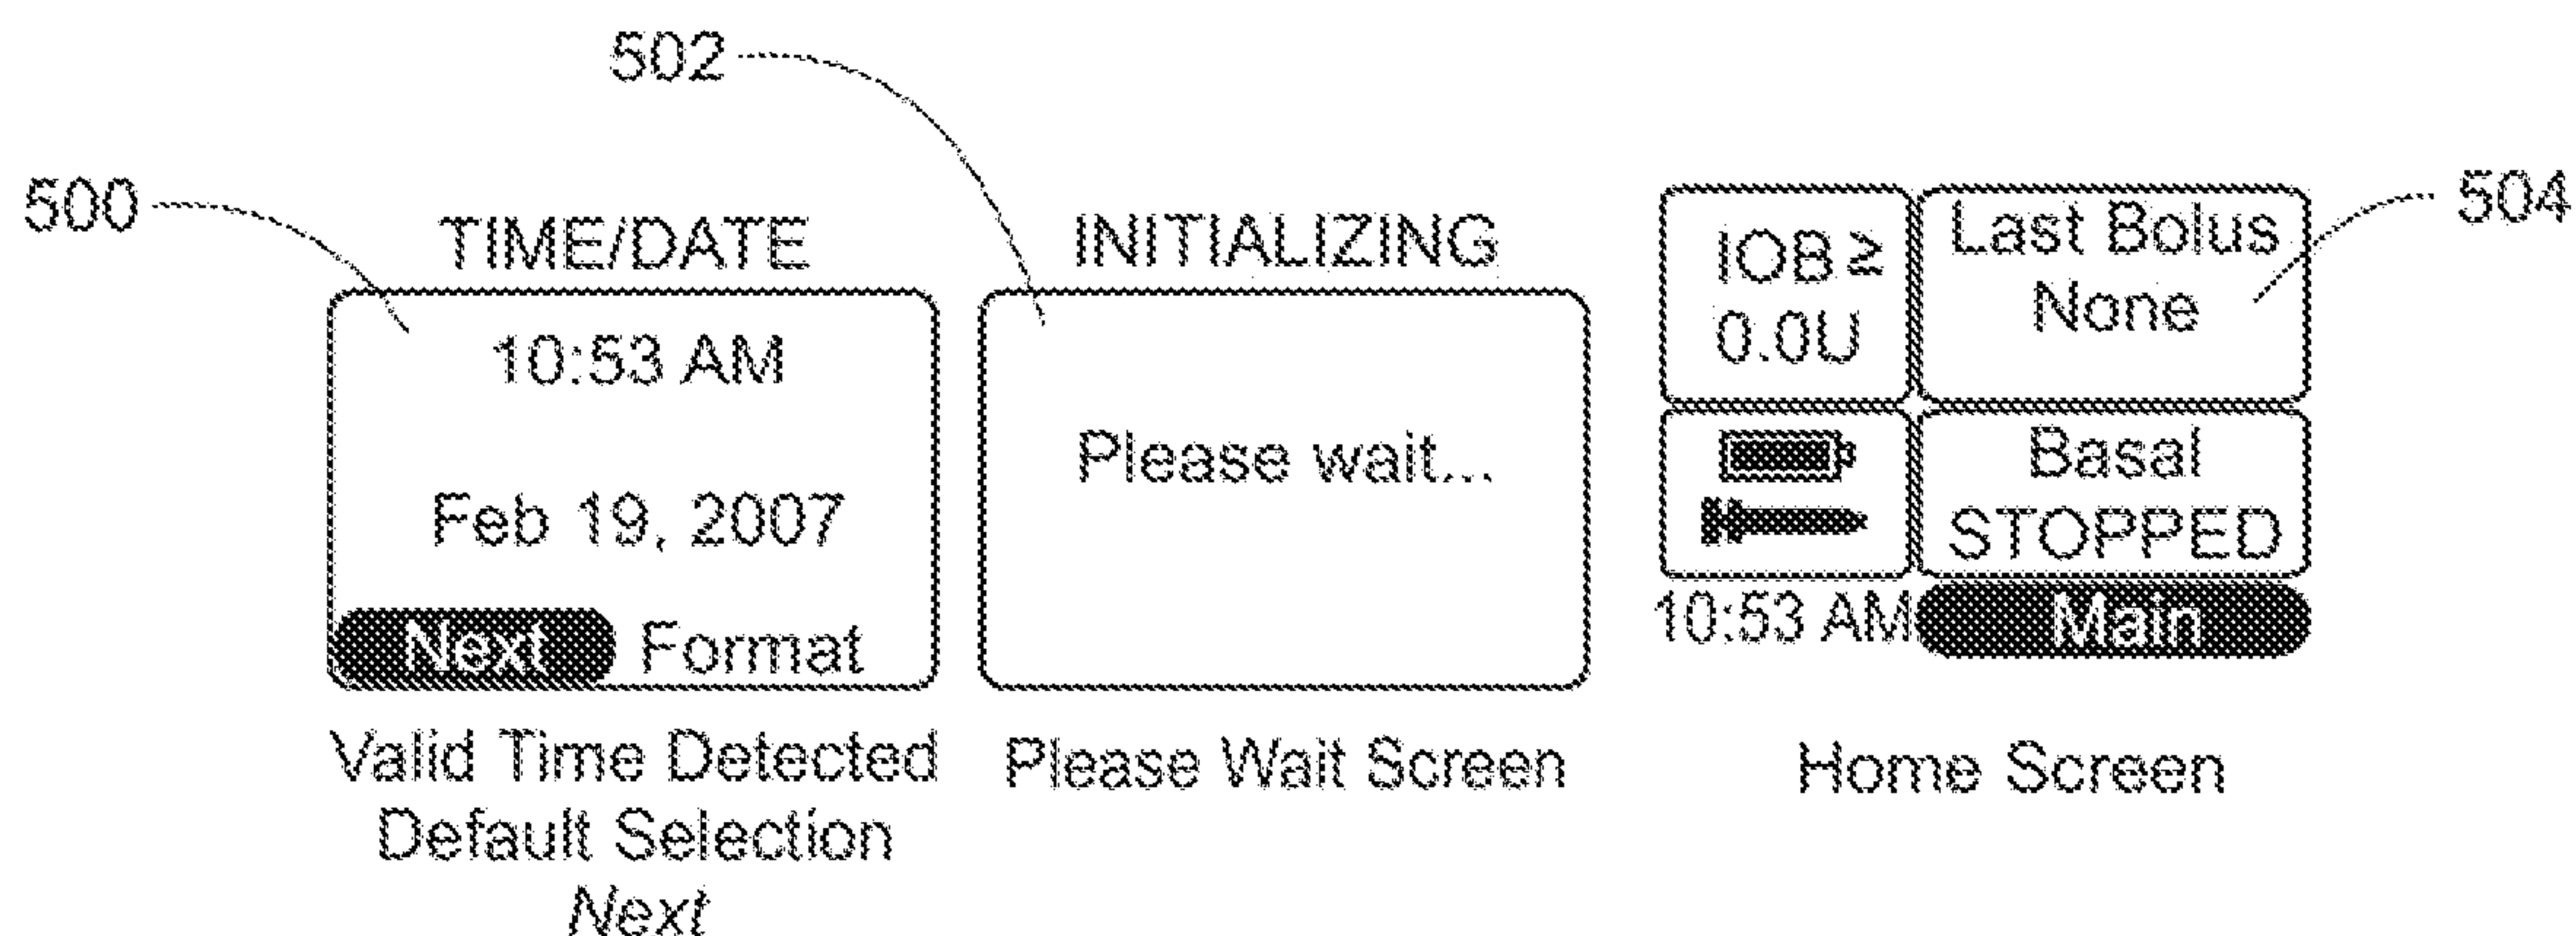


FIG. 5A

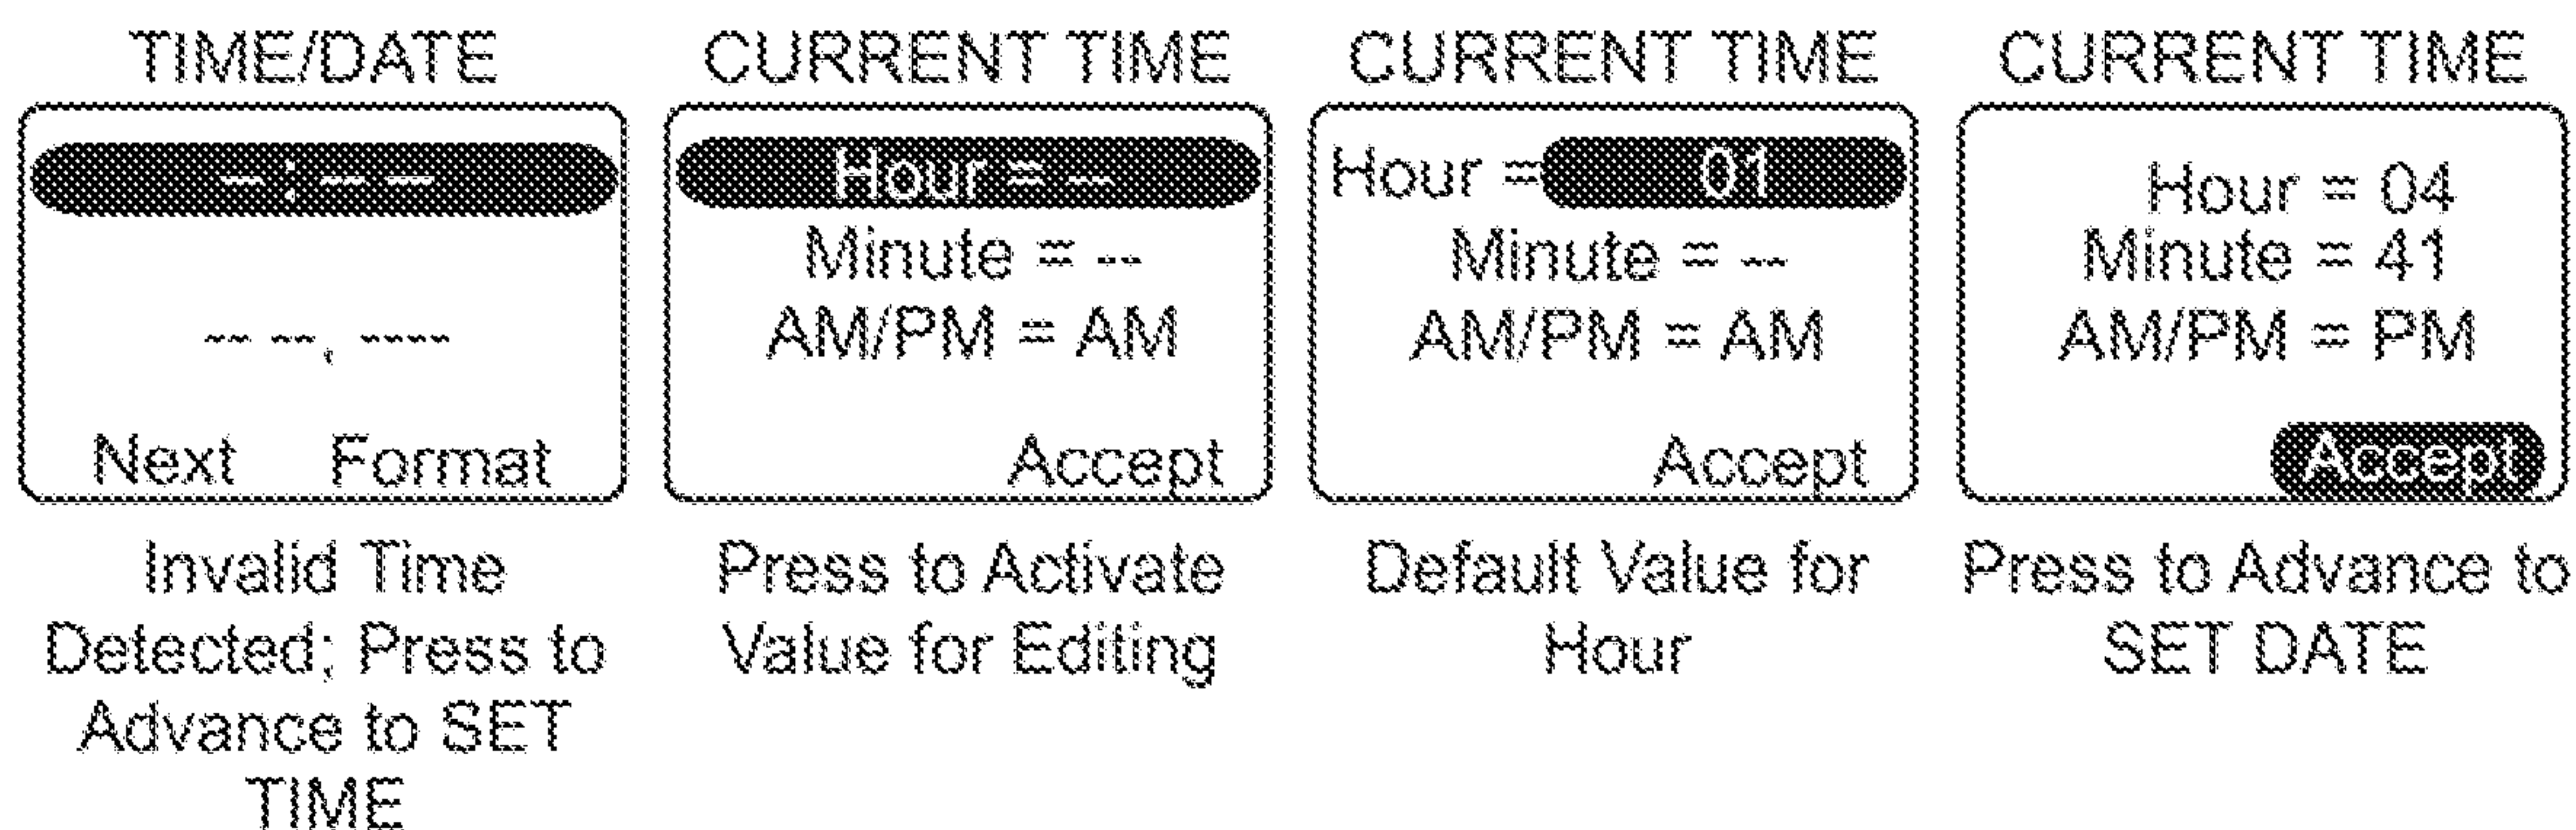


FIG. 5B

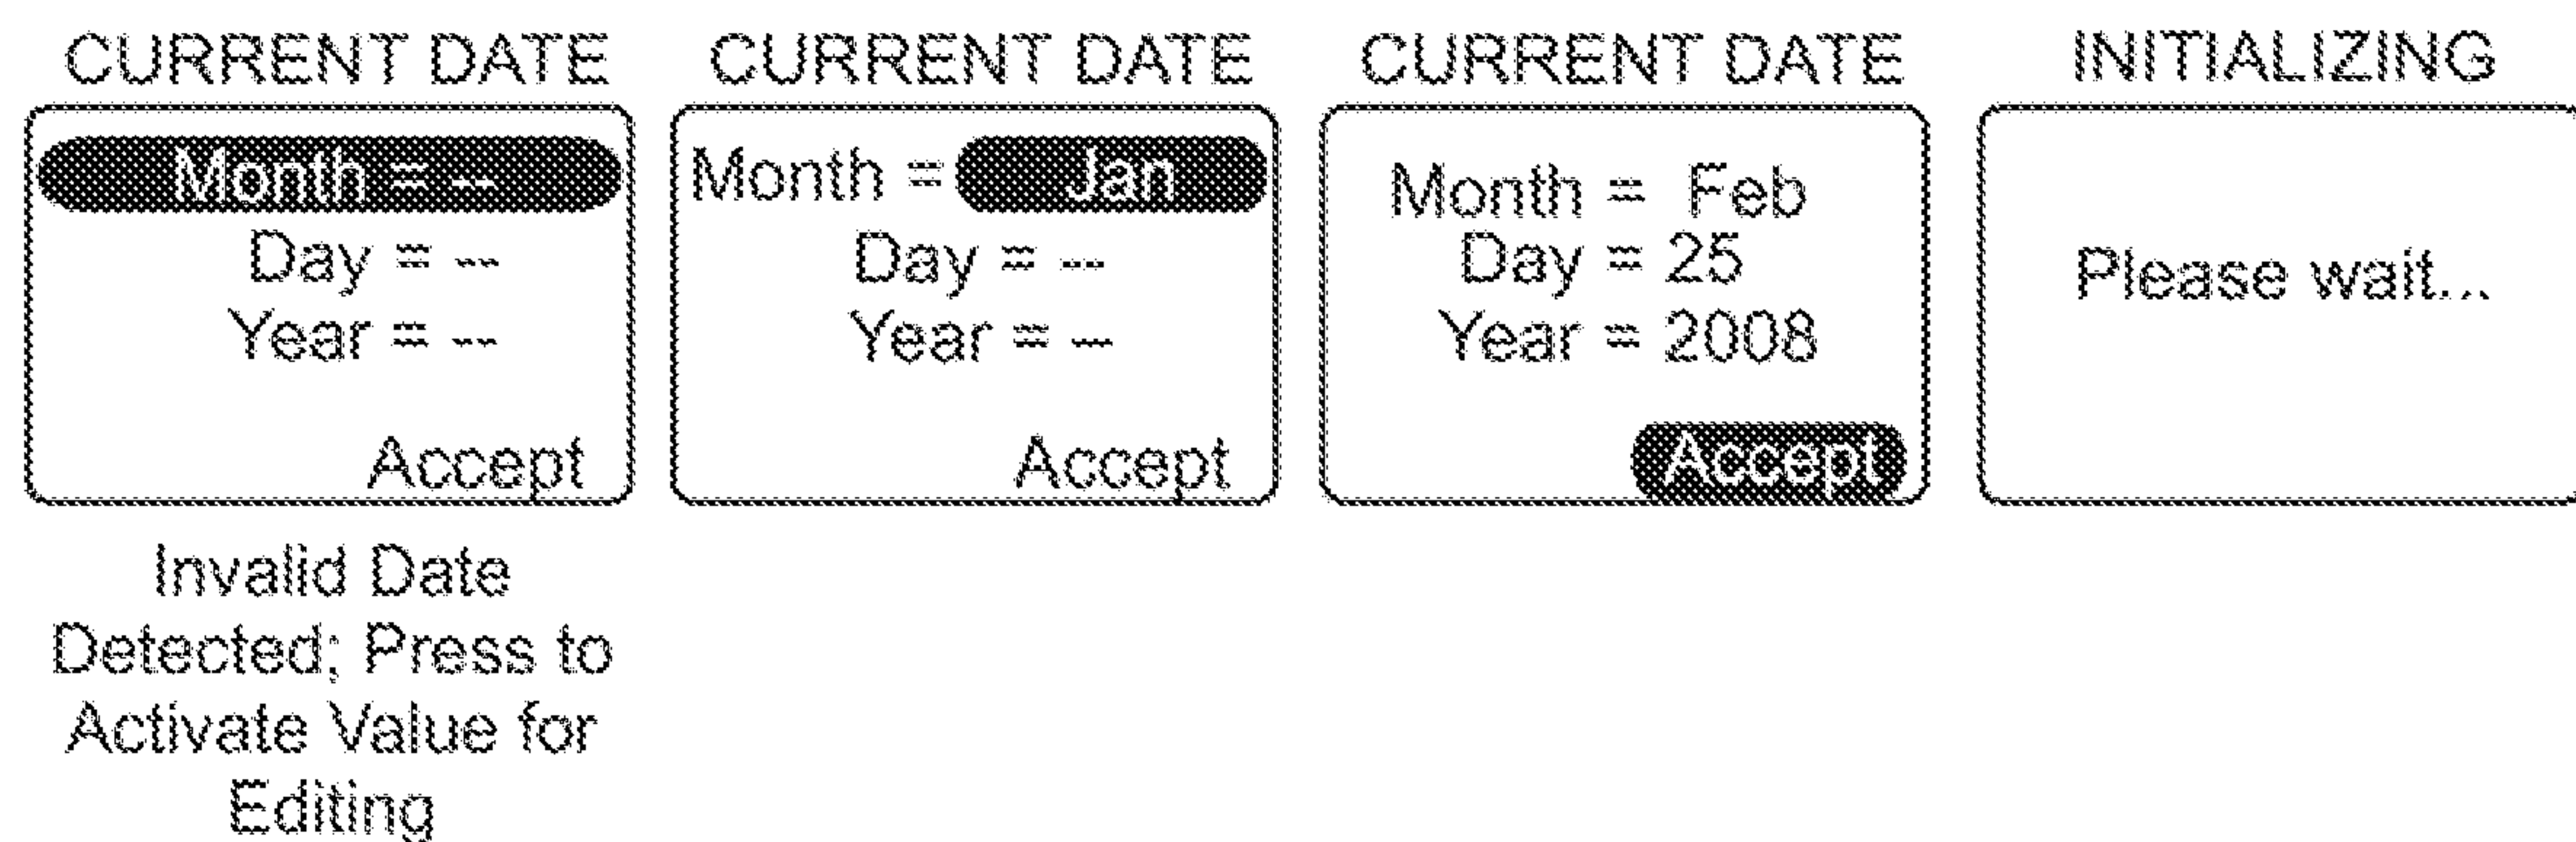


FIG. 5C

8/42

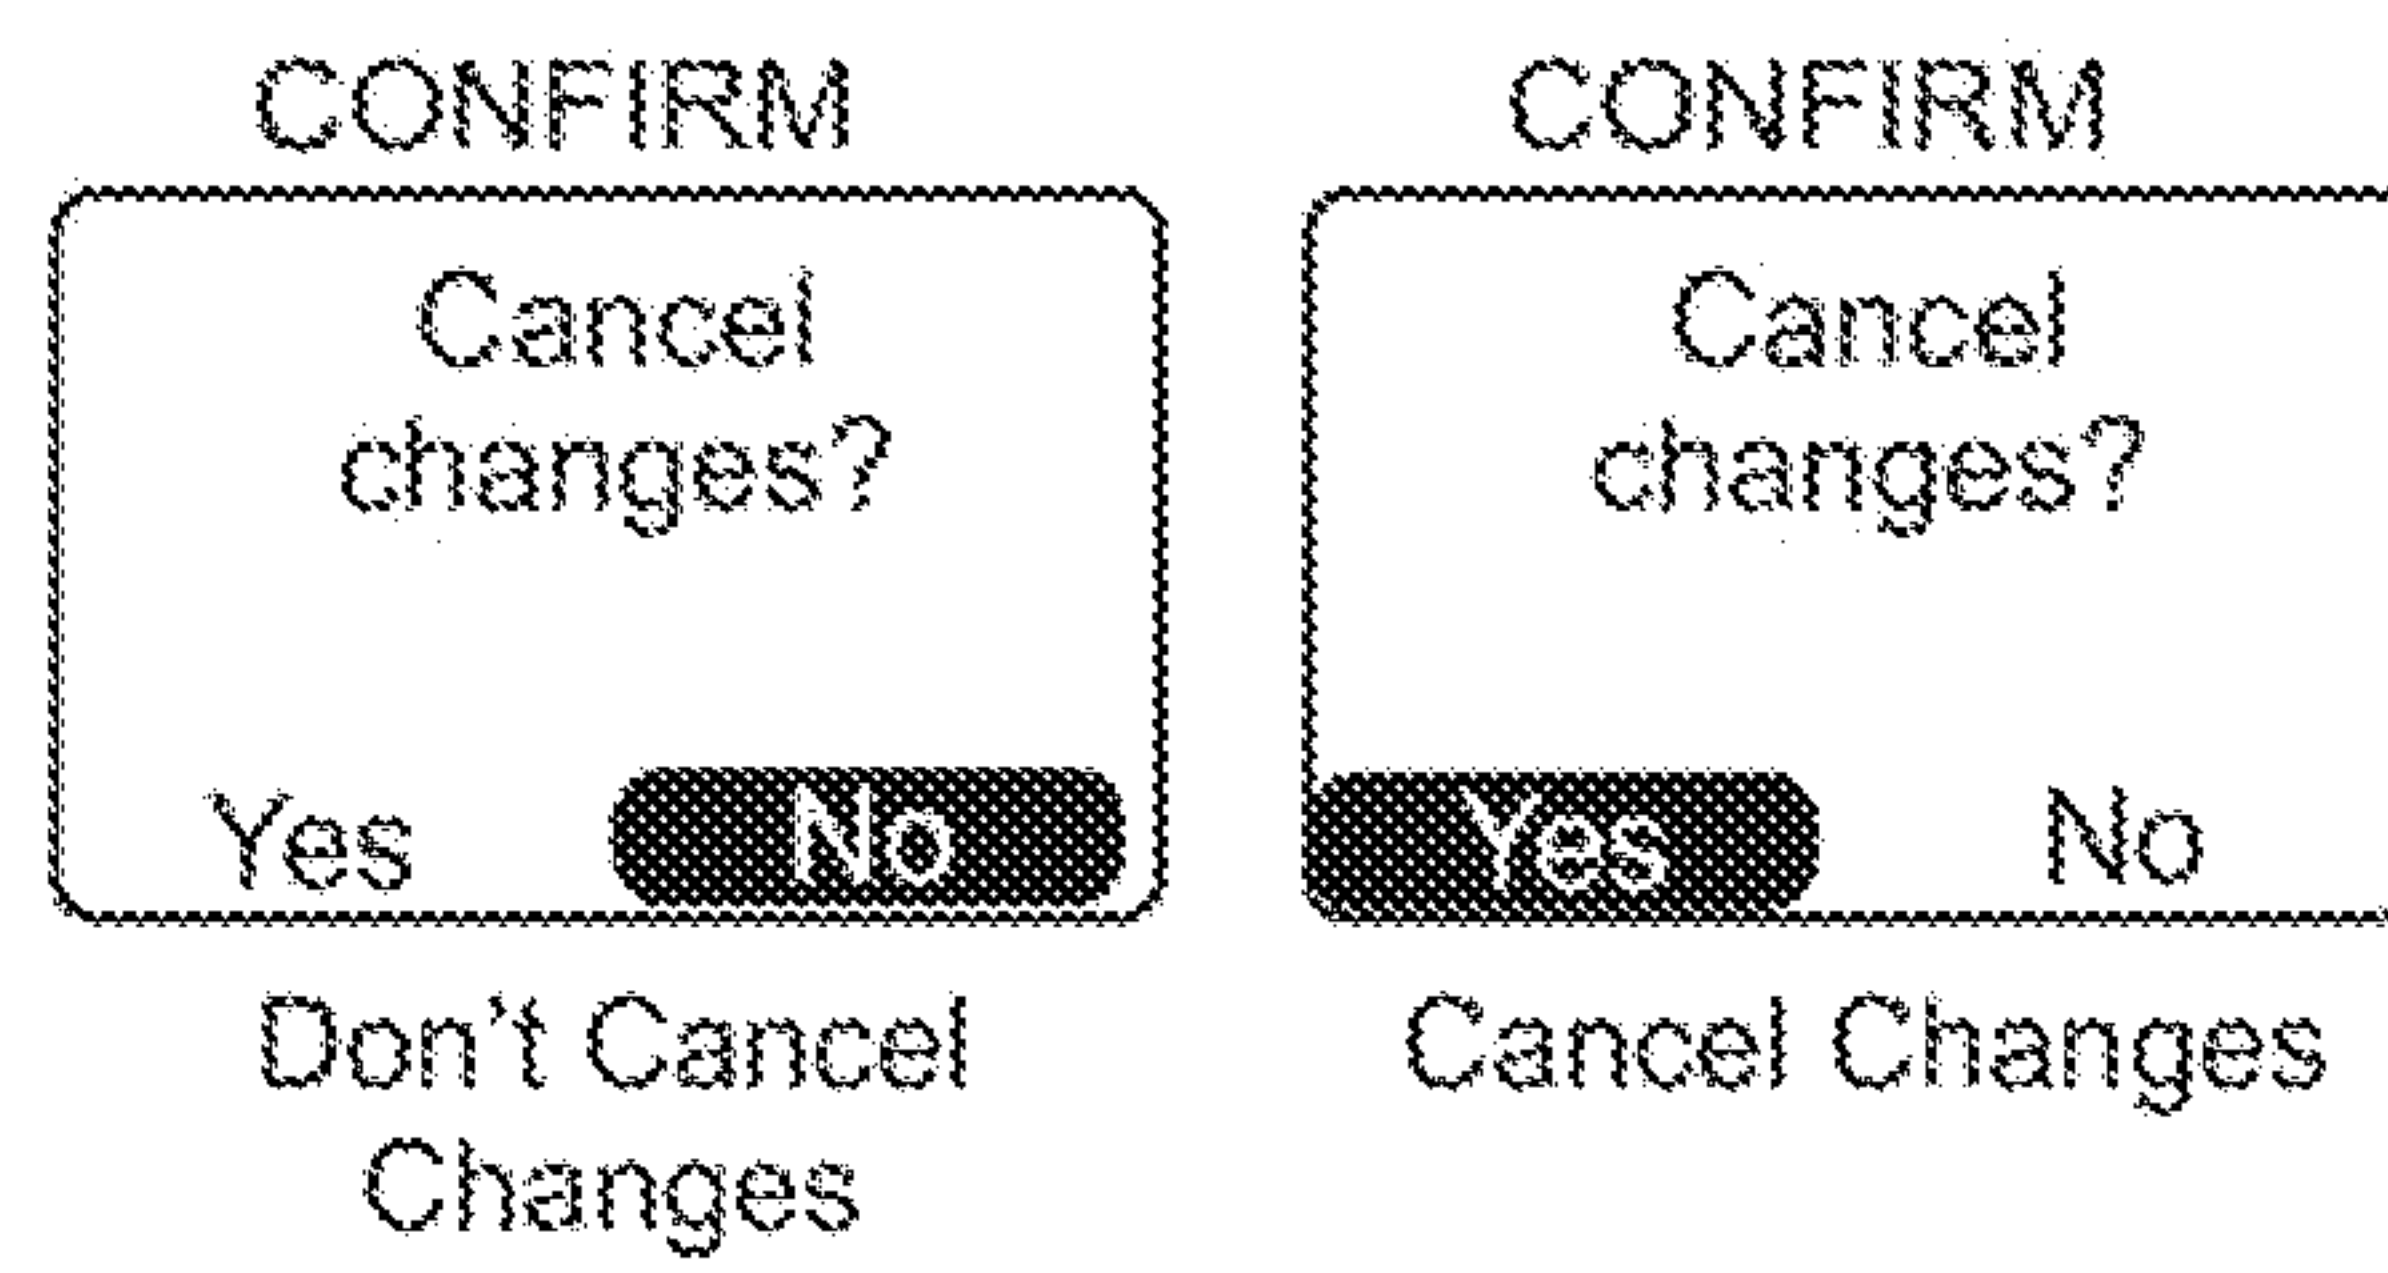


FIG. 6

9/42

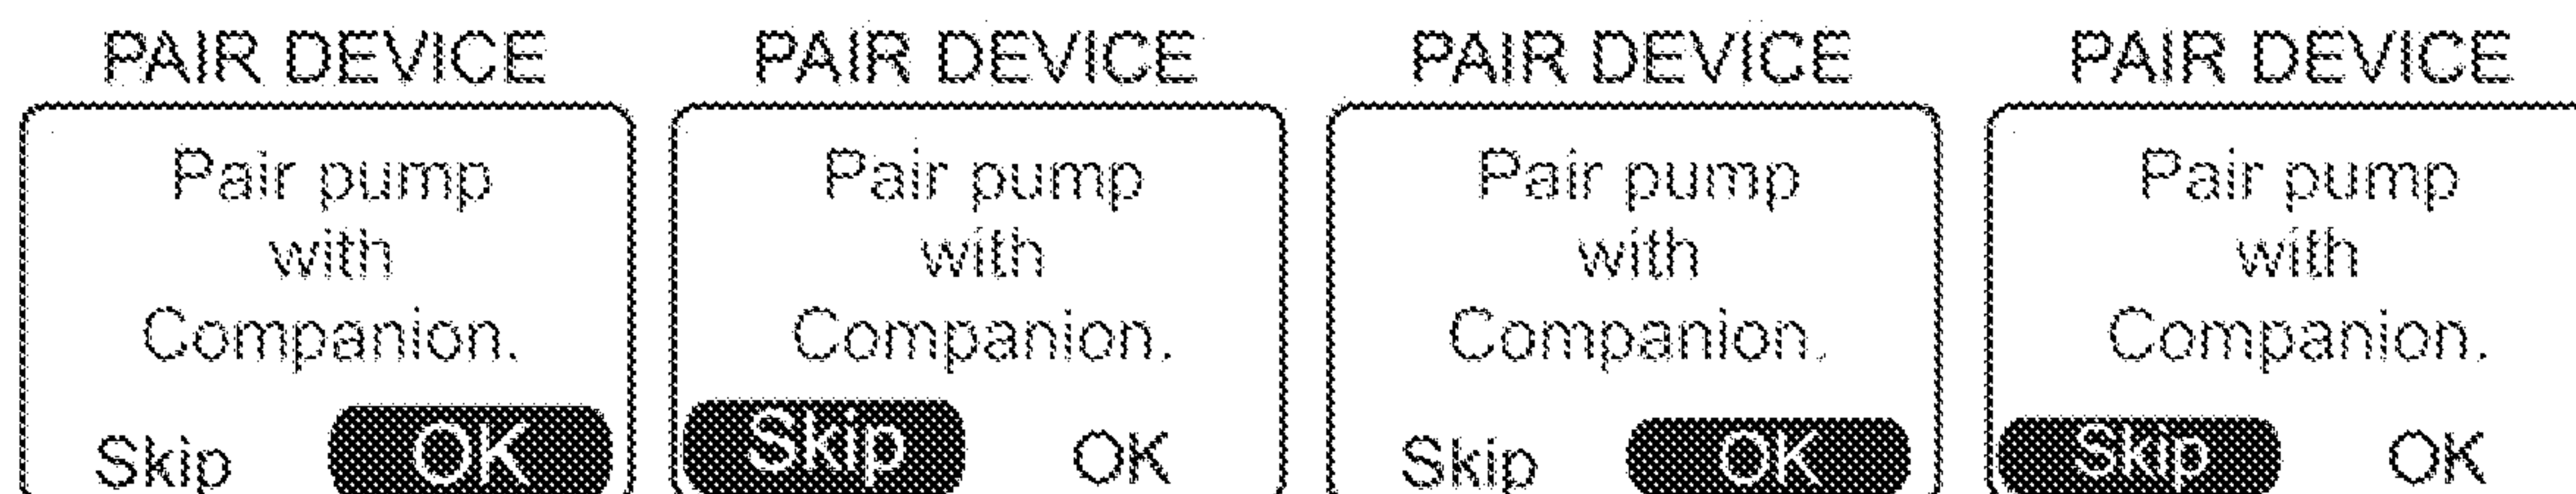


FIG. 7A

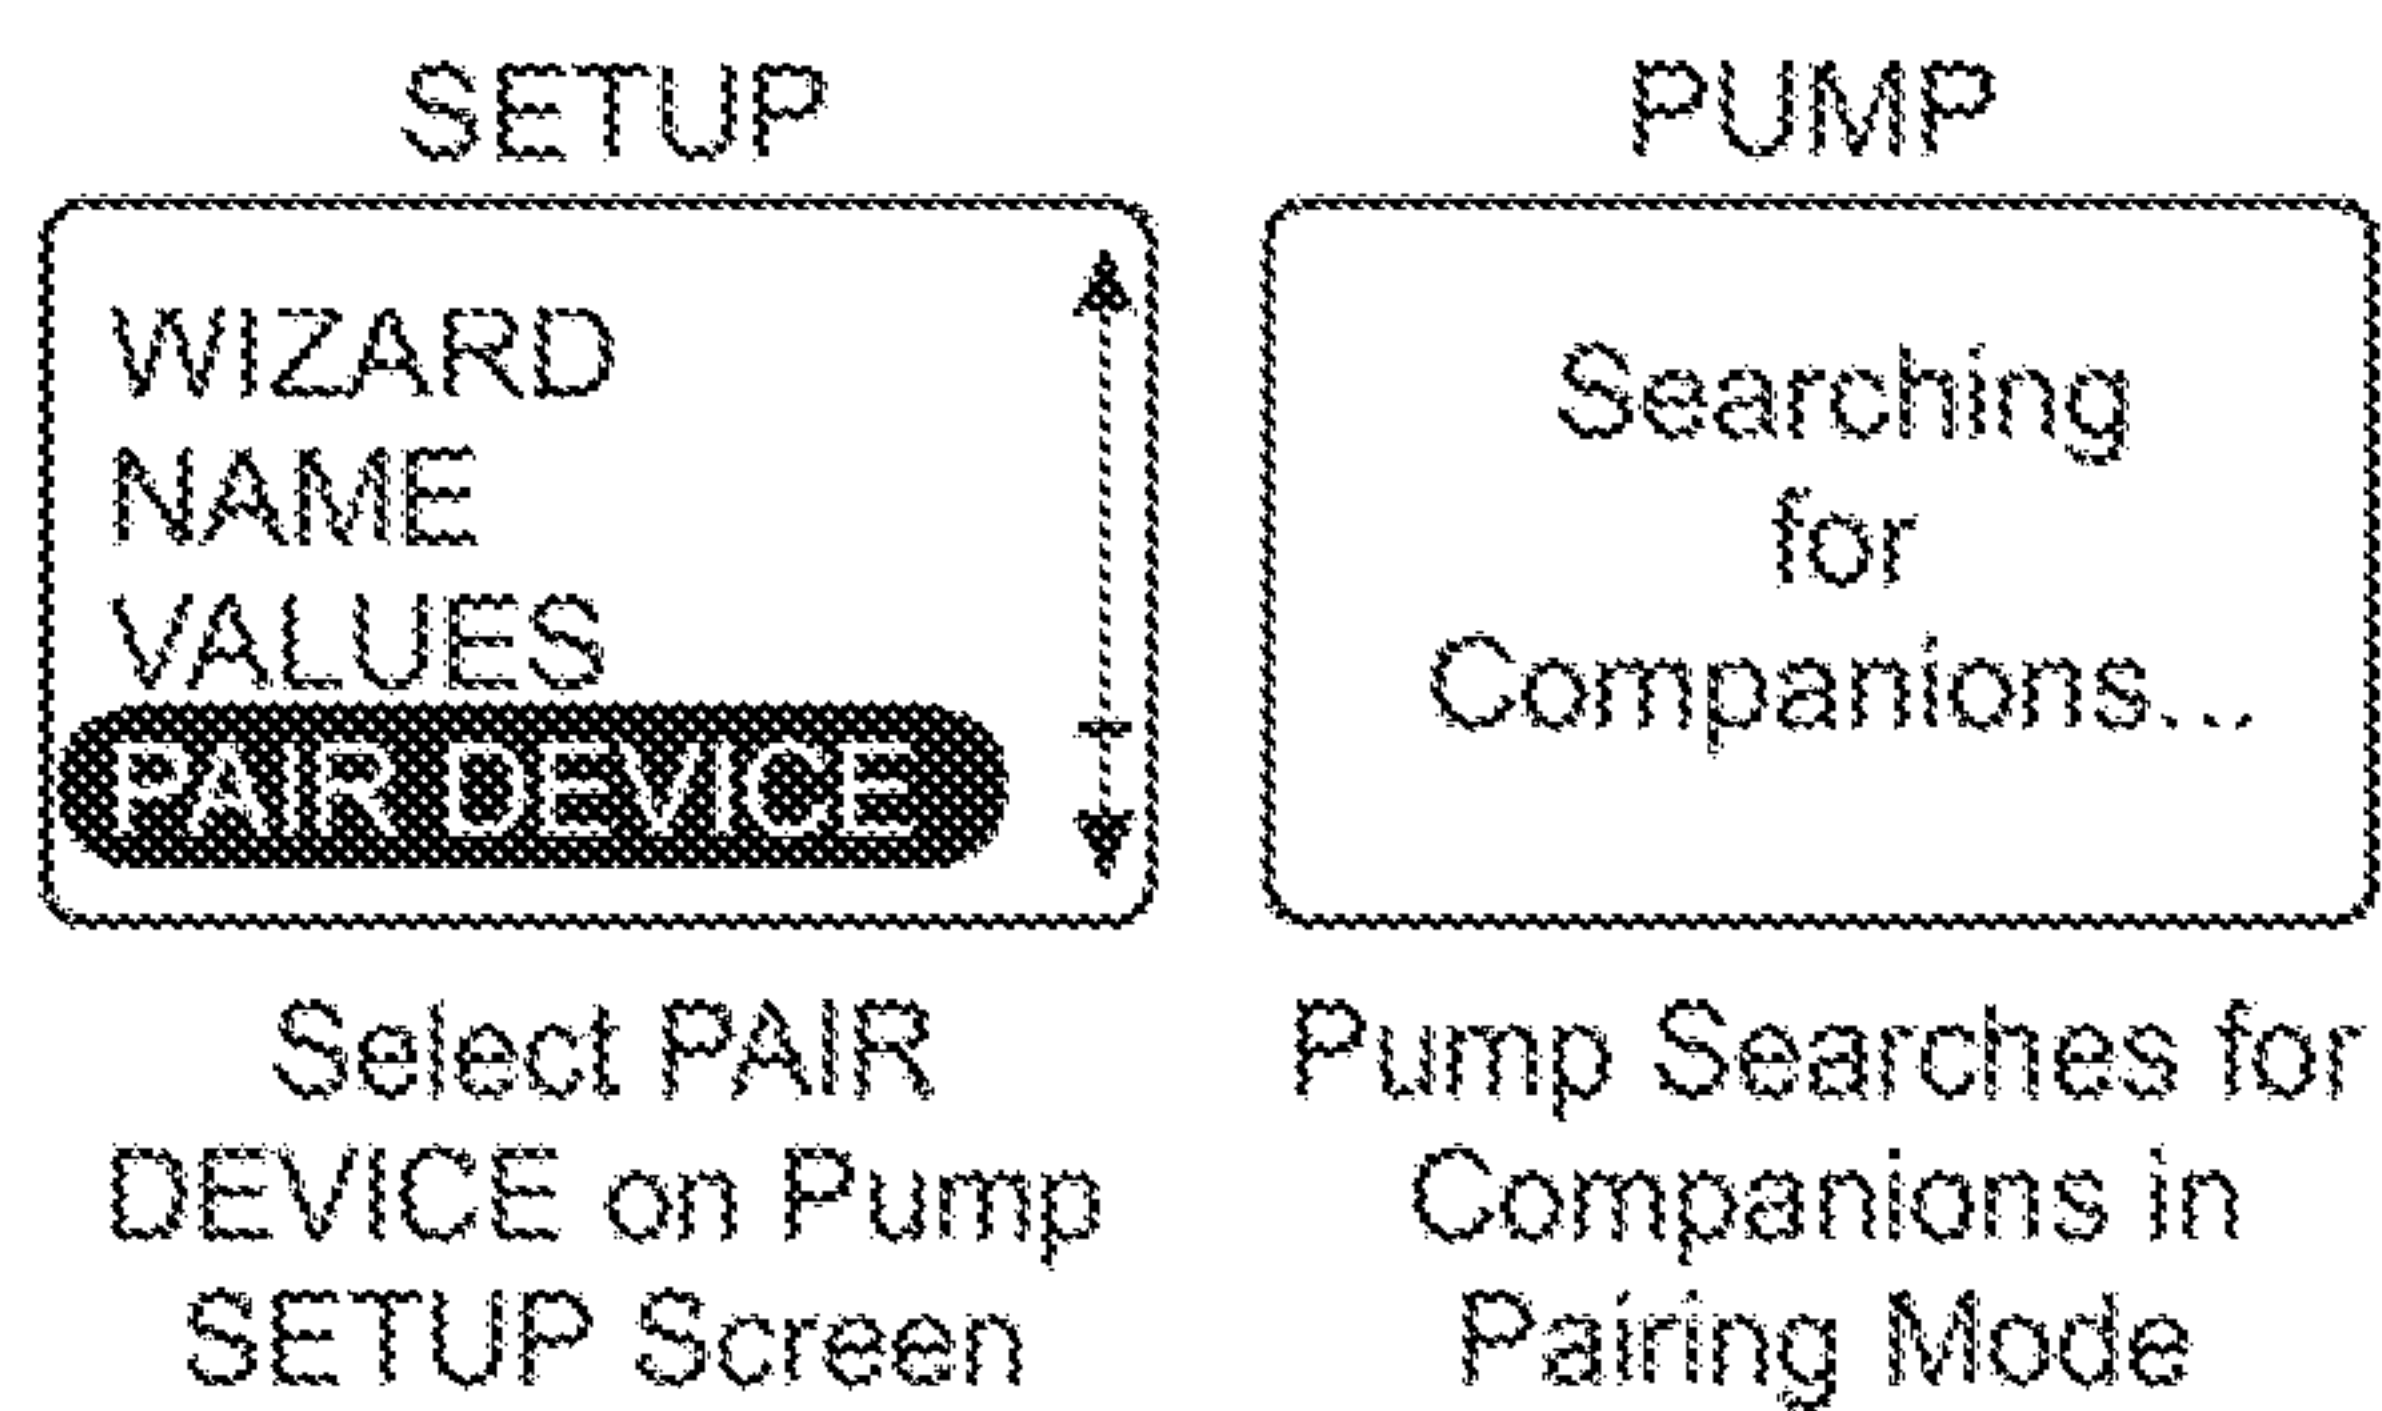


FIG. 7B

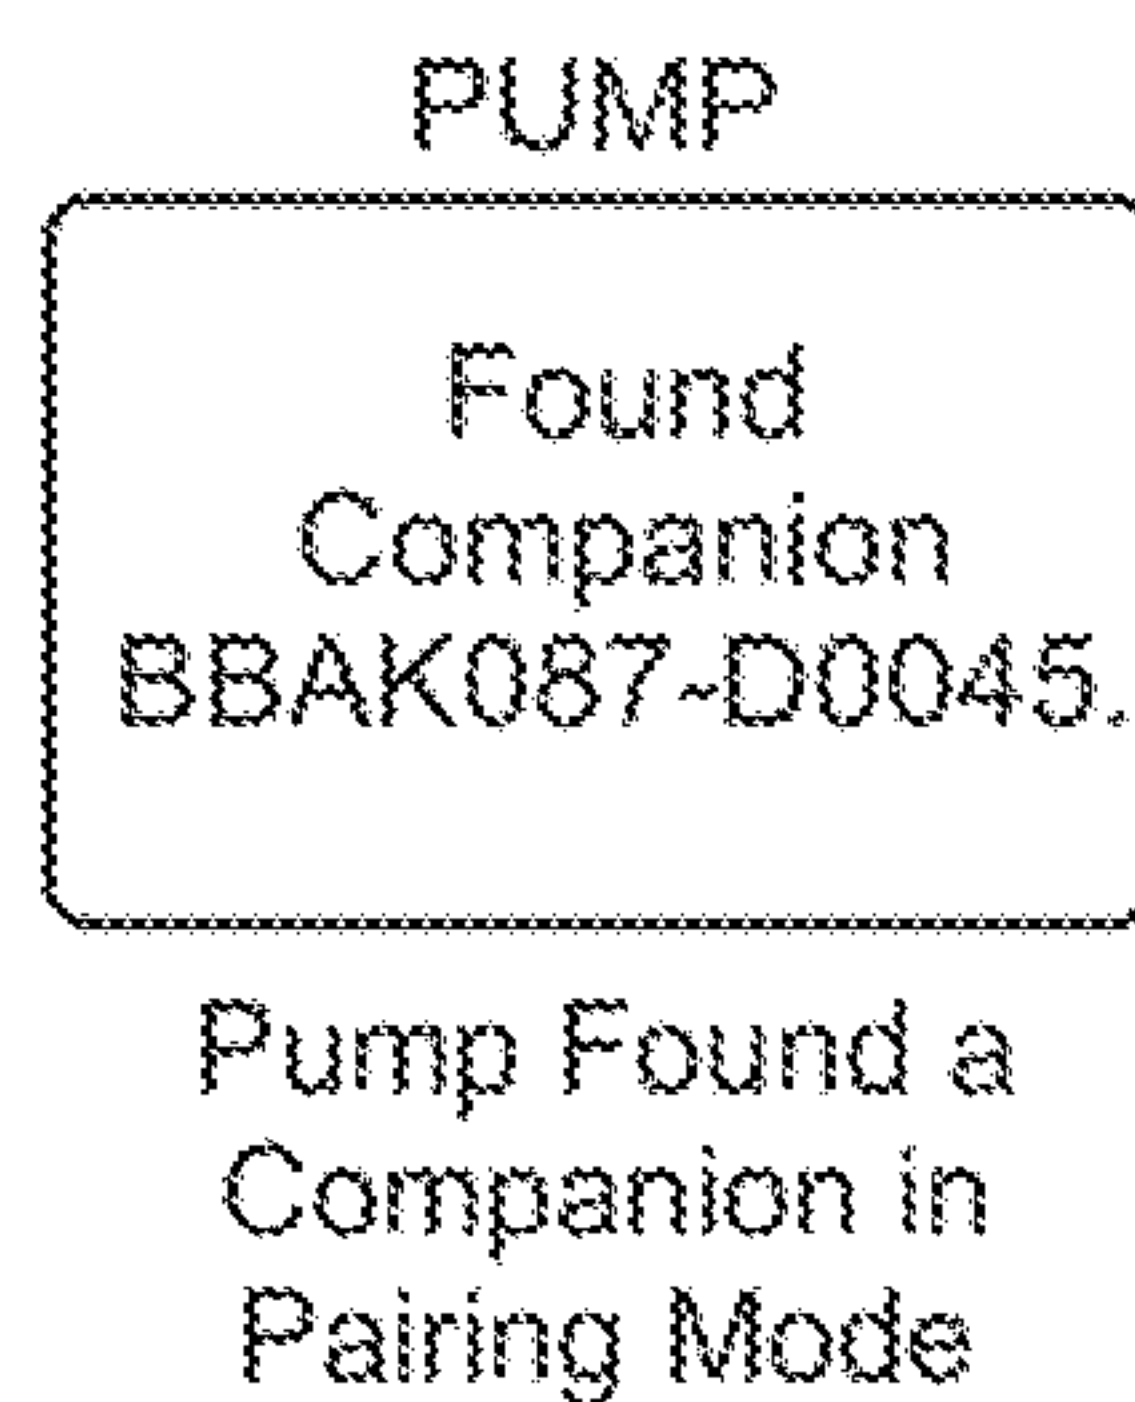


FIG. 7C

10/42


WARNING



No Companions in
Pairing Mode
Found

FIG. 7D

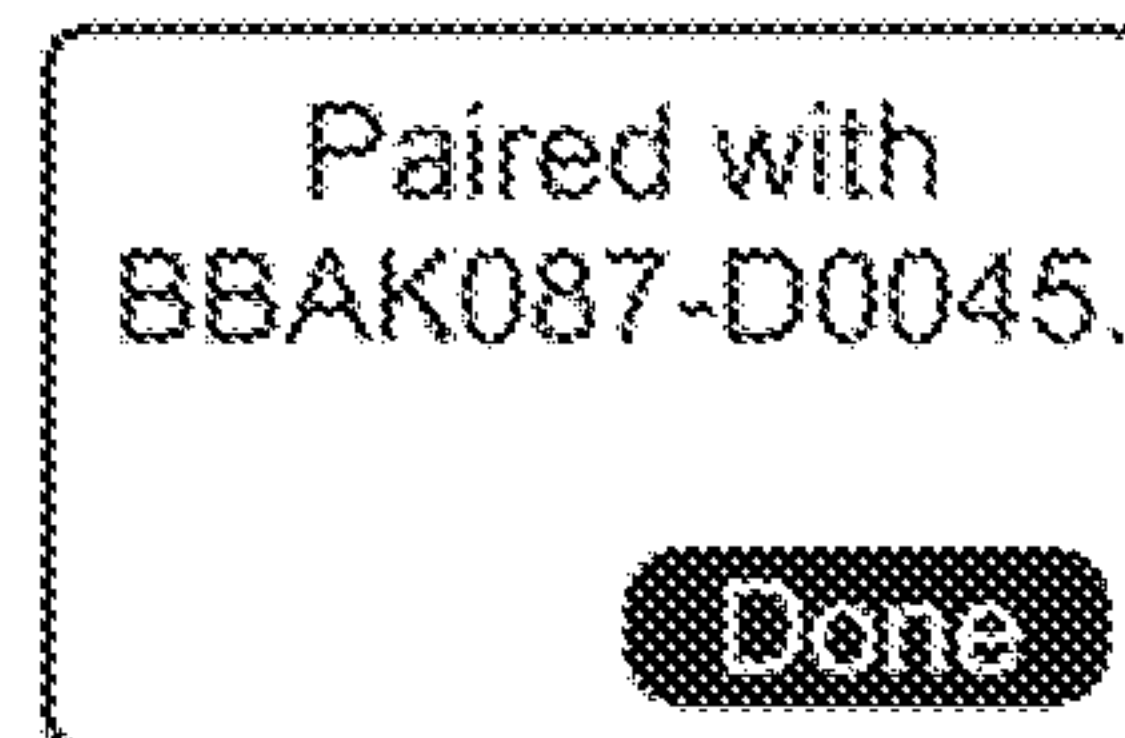
PUMP



Pairing was
Accepted on
Companion

FIG. 7E

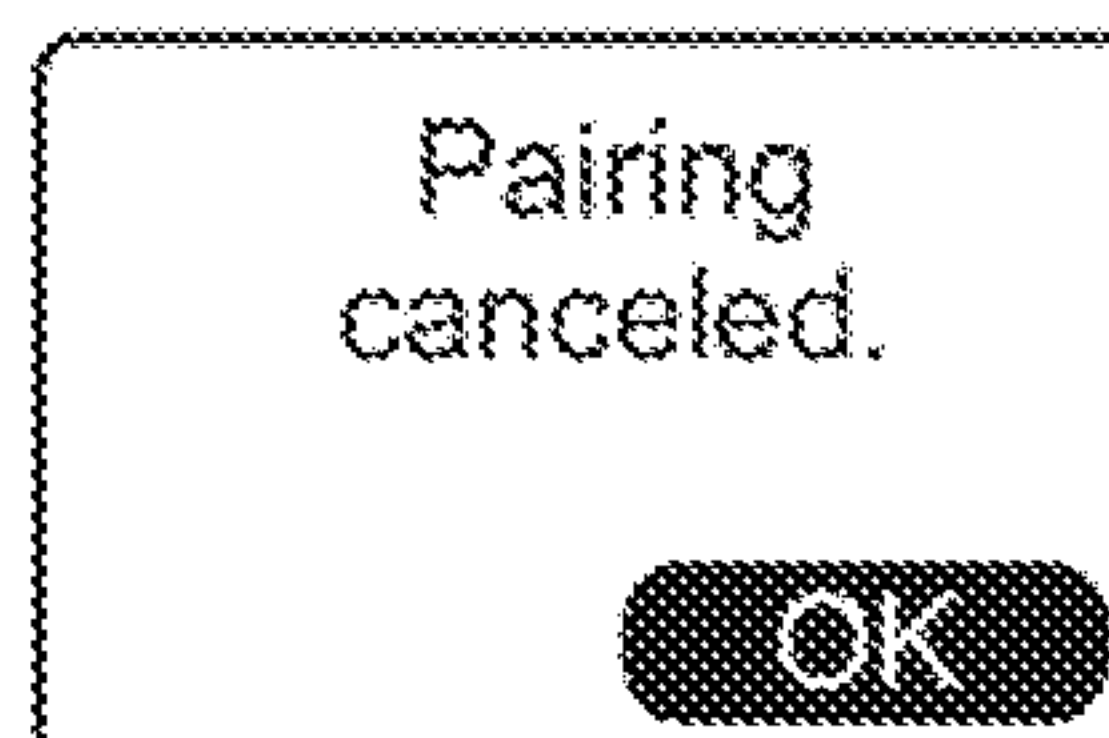WARNING



User Interrupted
Pairing with Button
Press

FIG. 7F

11/42

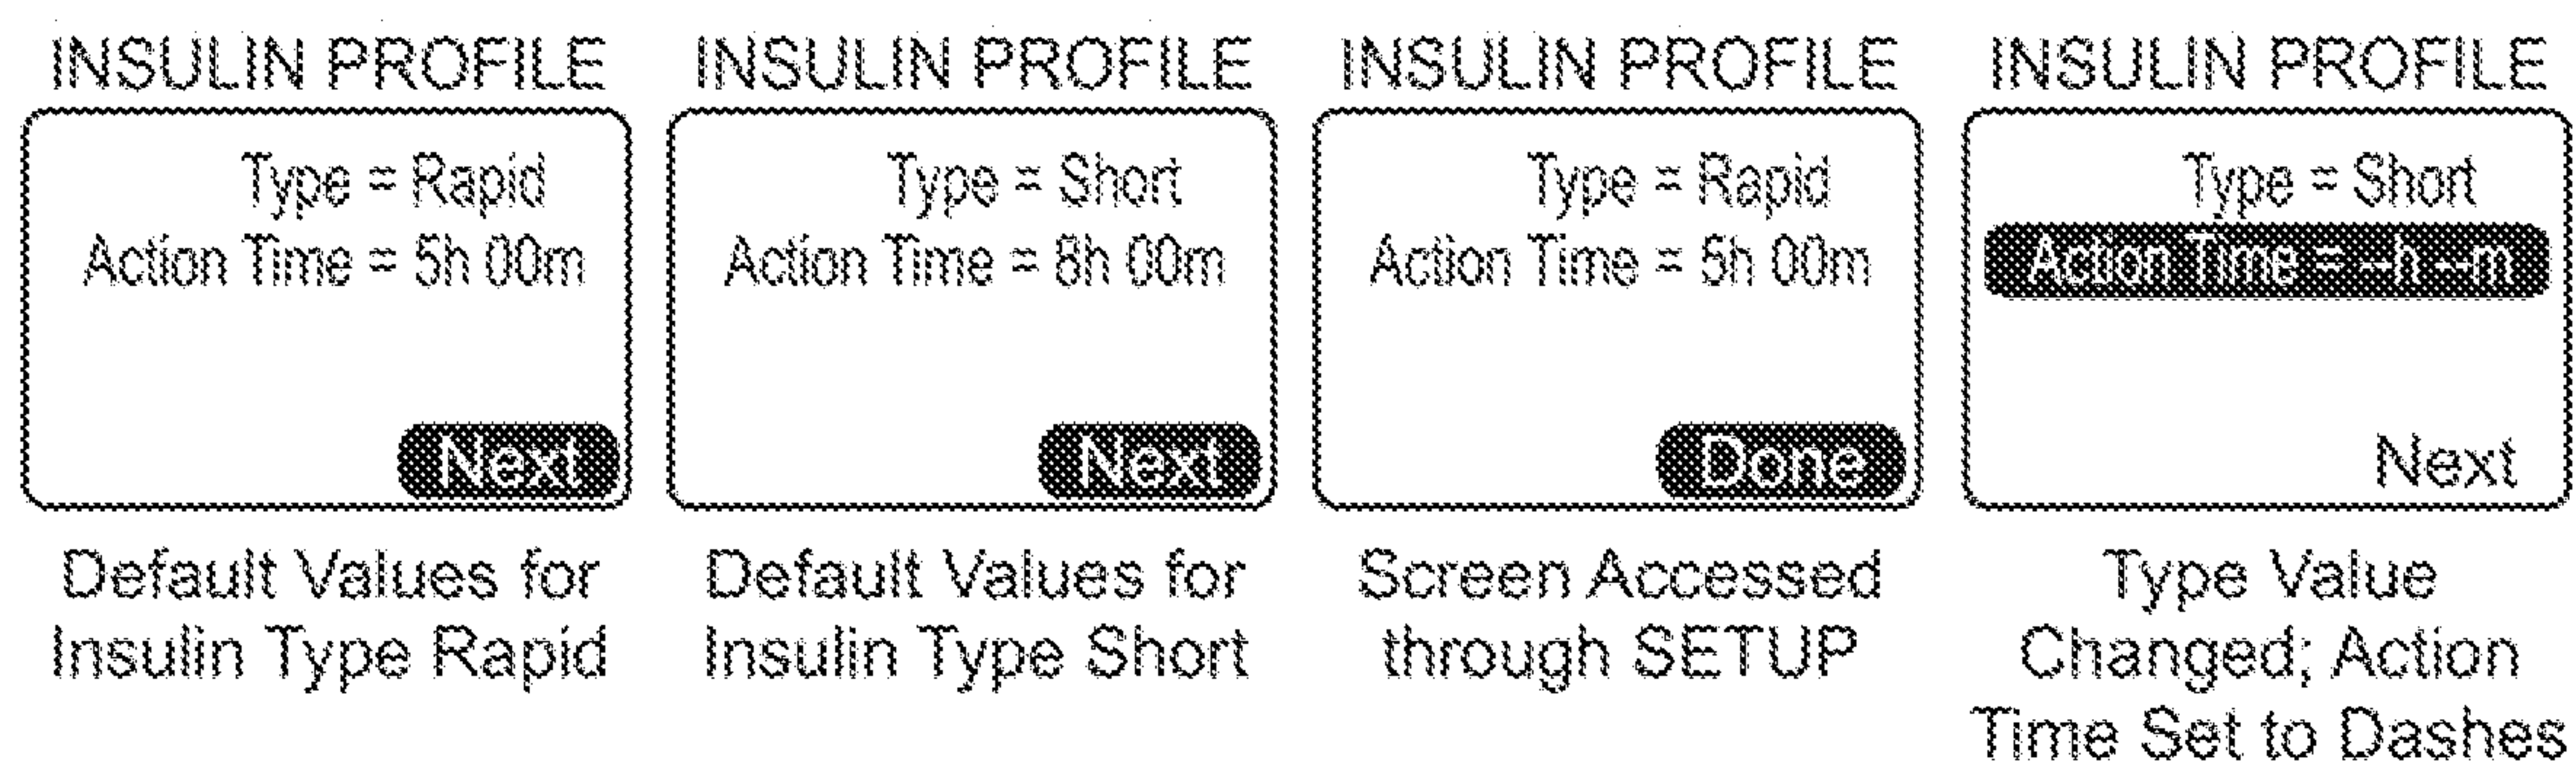


FIG. 8A

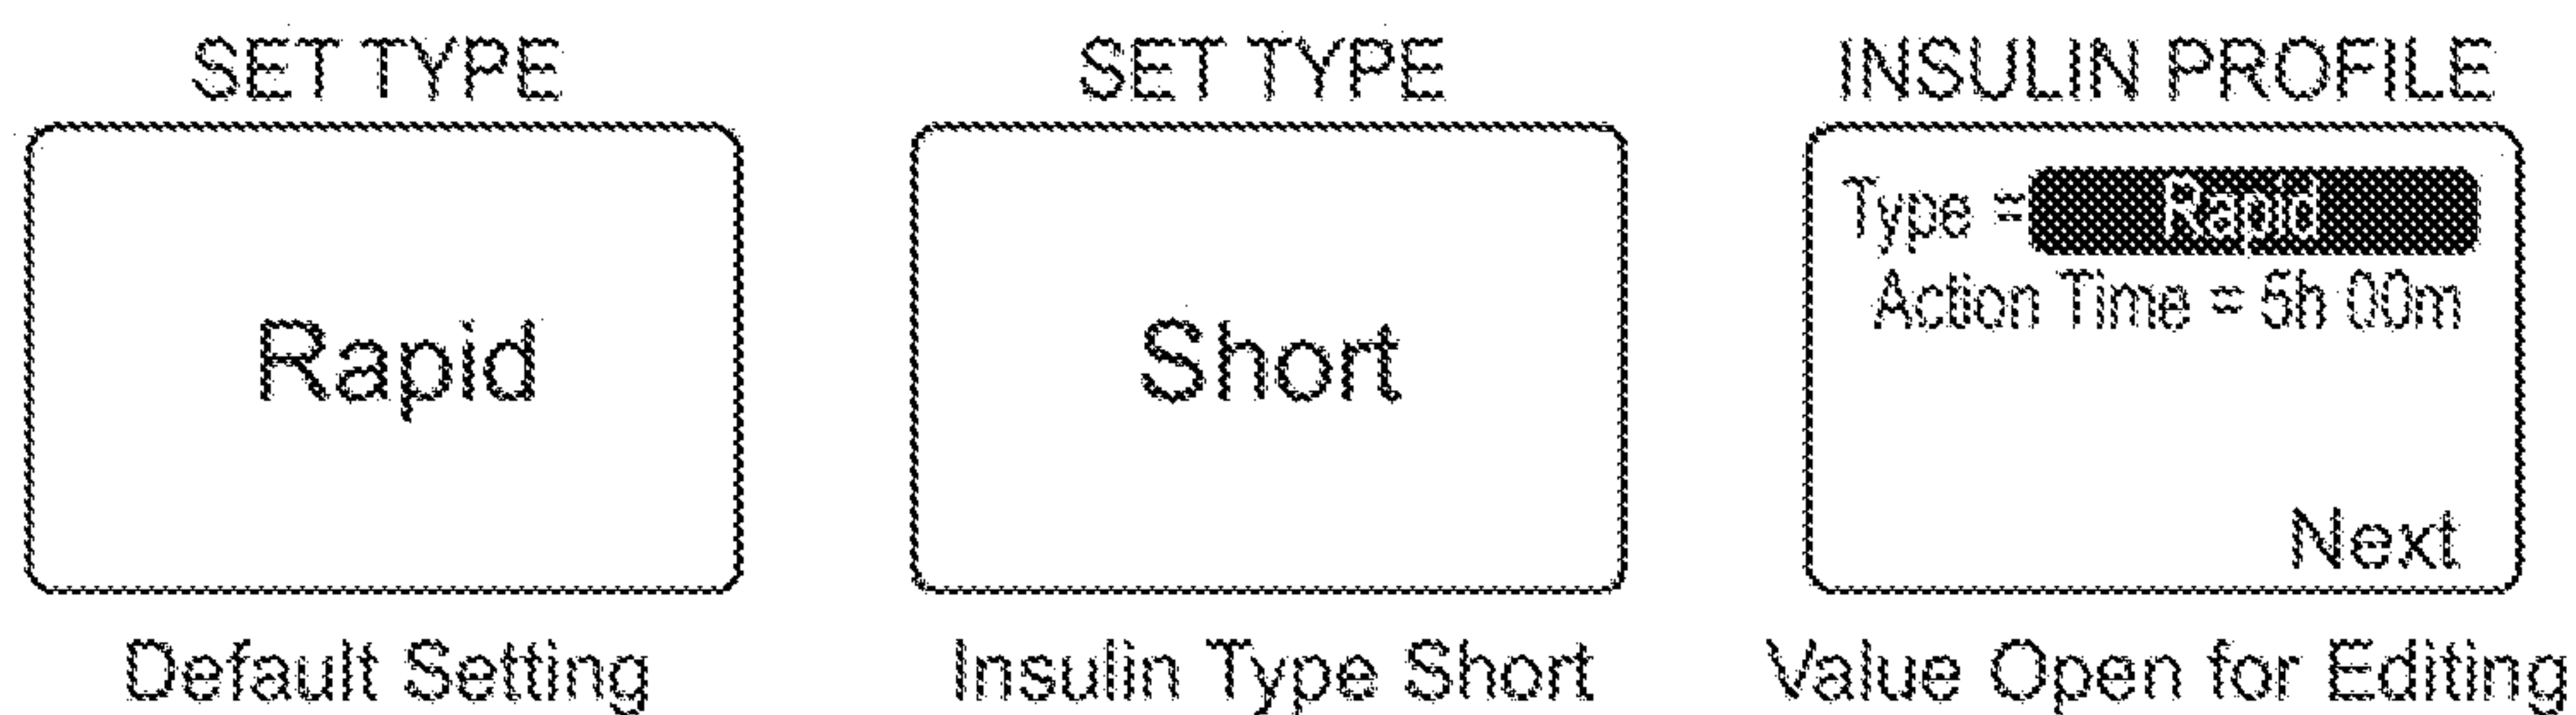


FIG. 8B

12/42

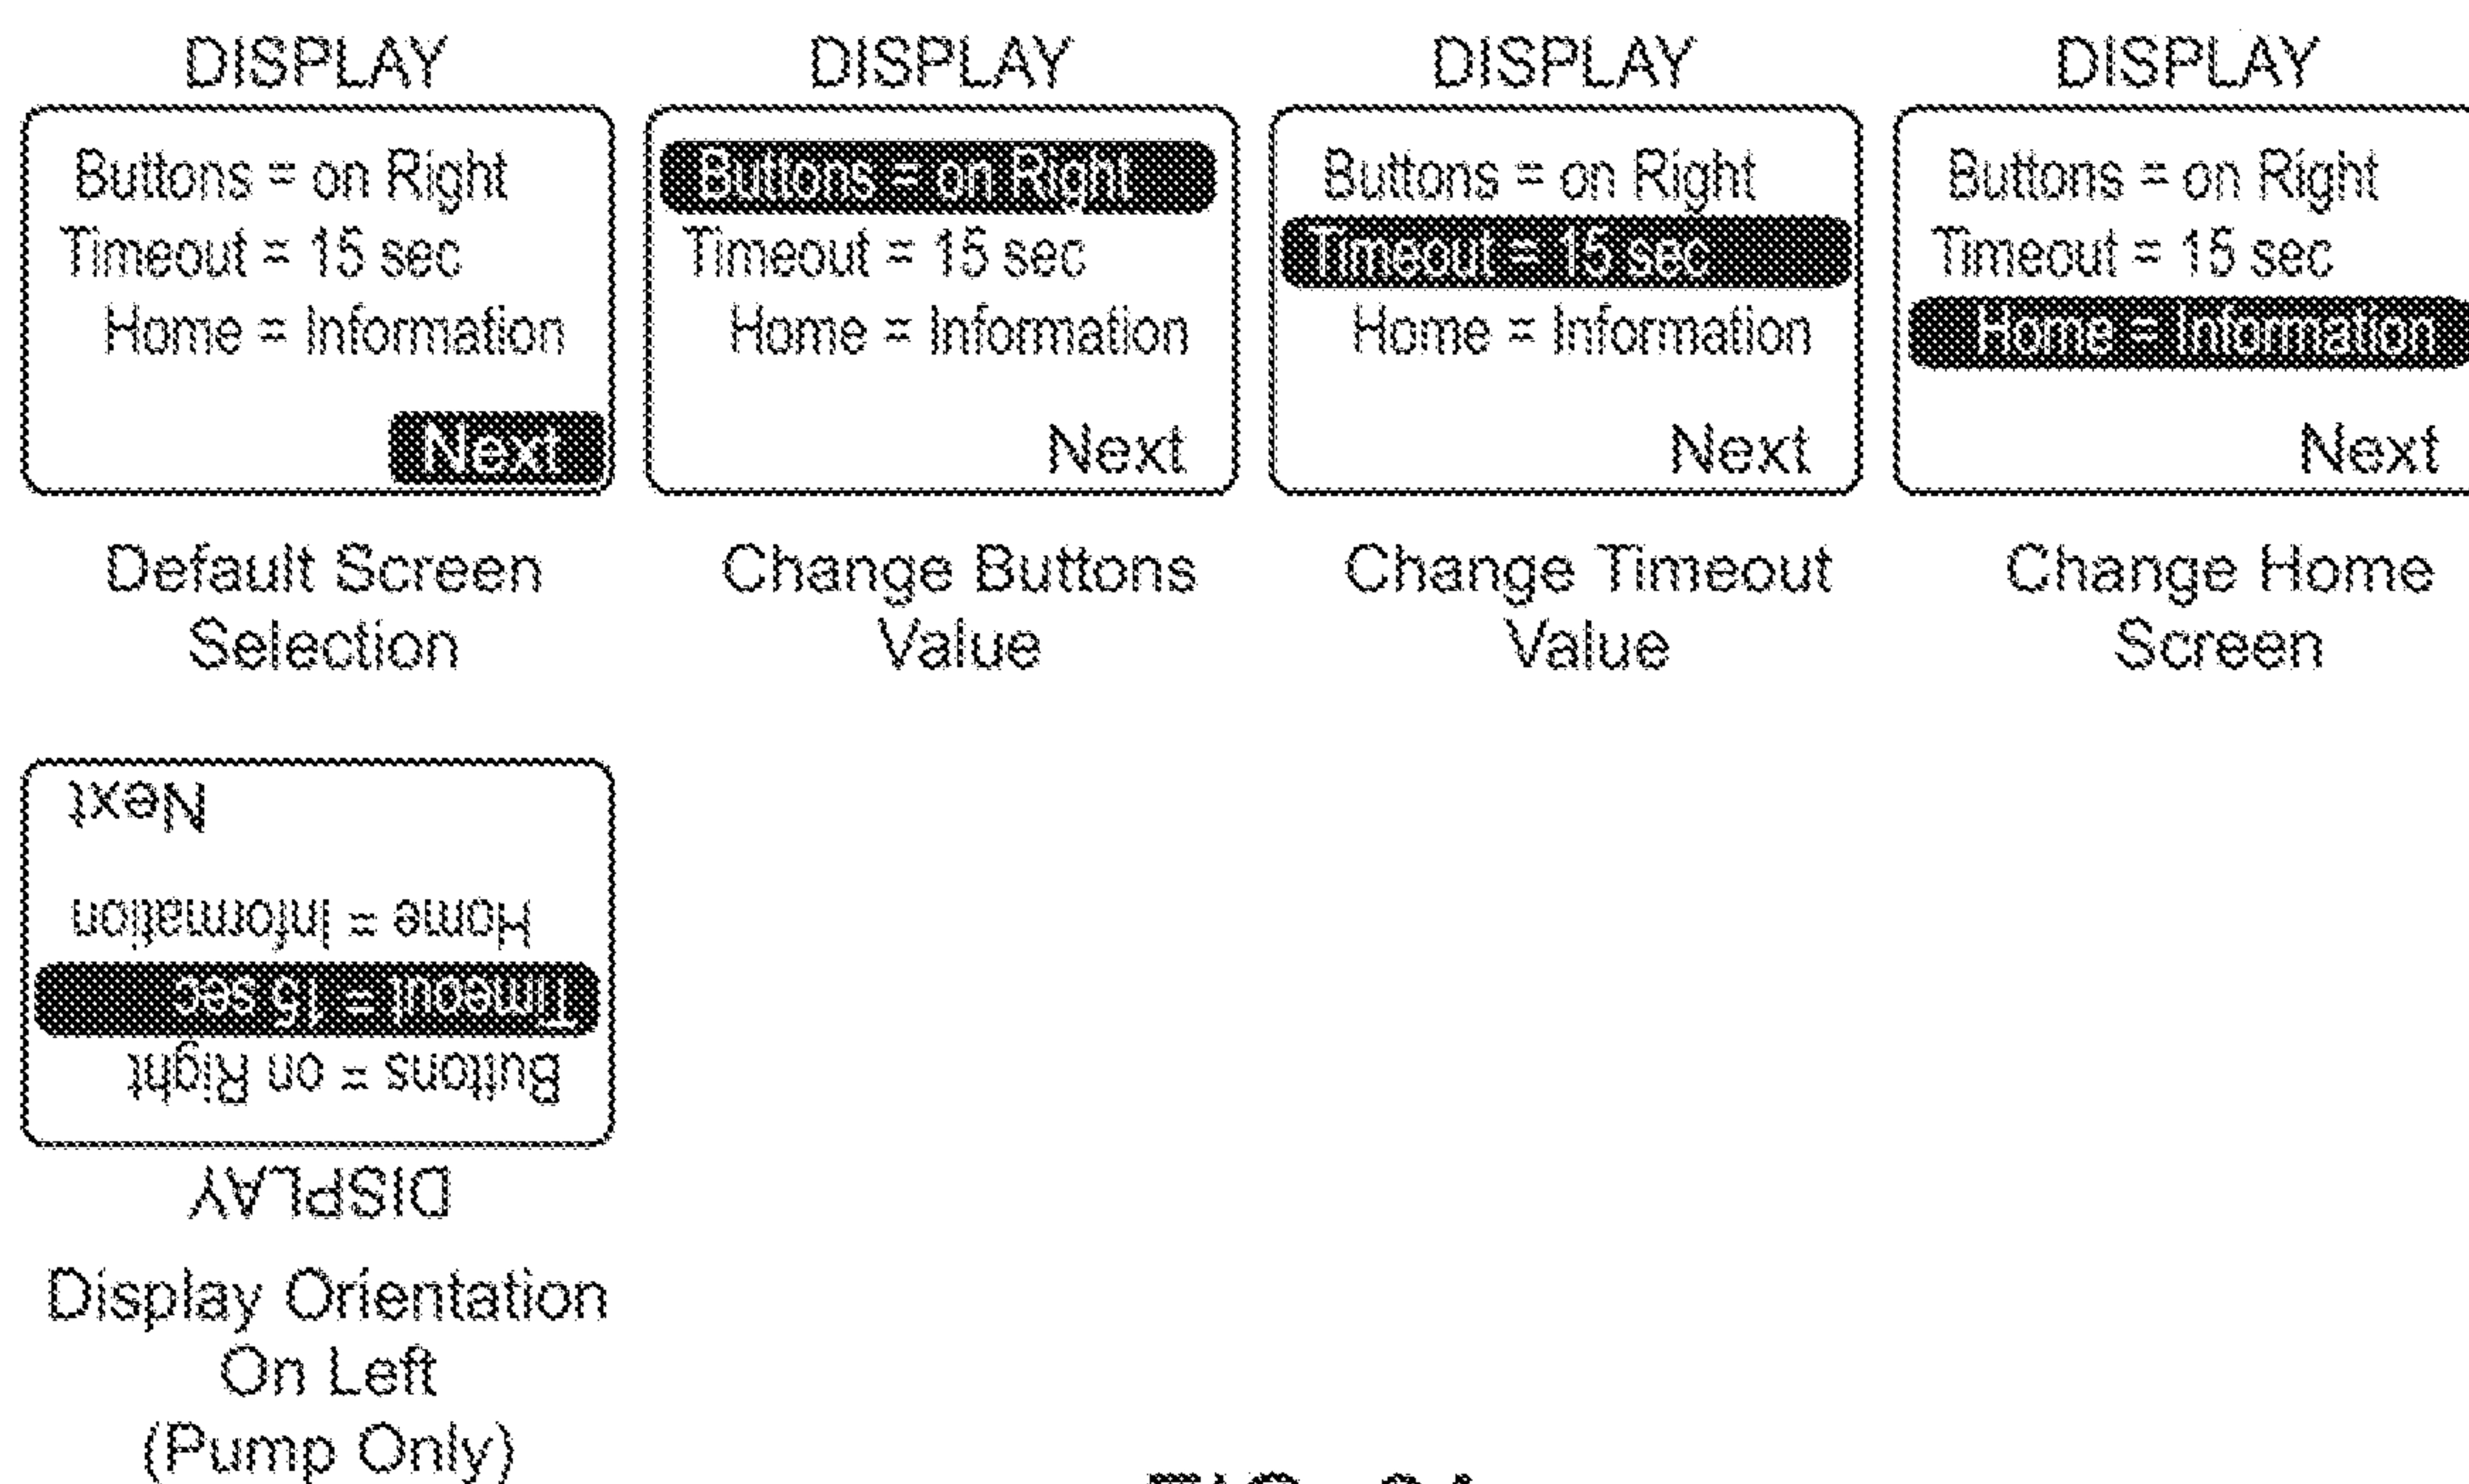


FIG. 9A

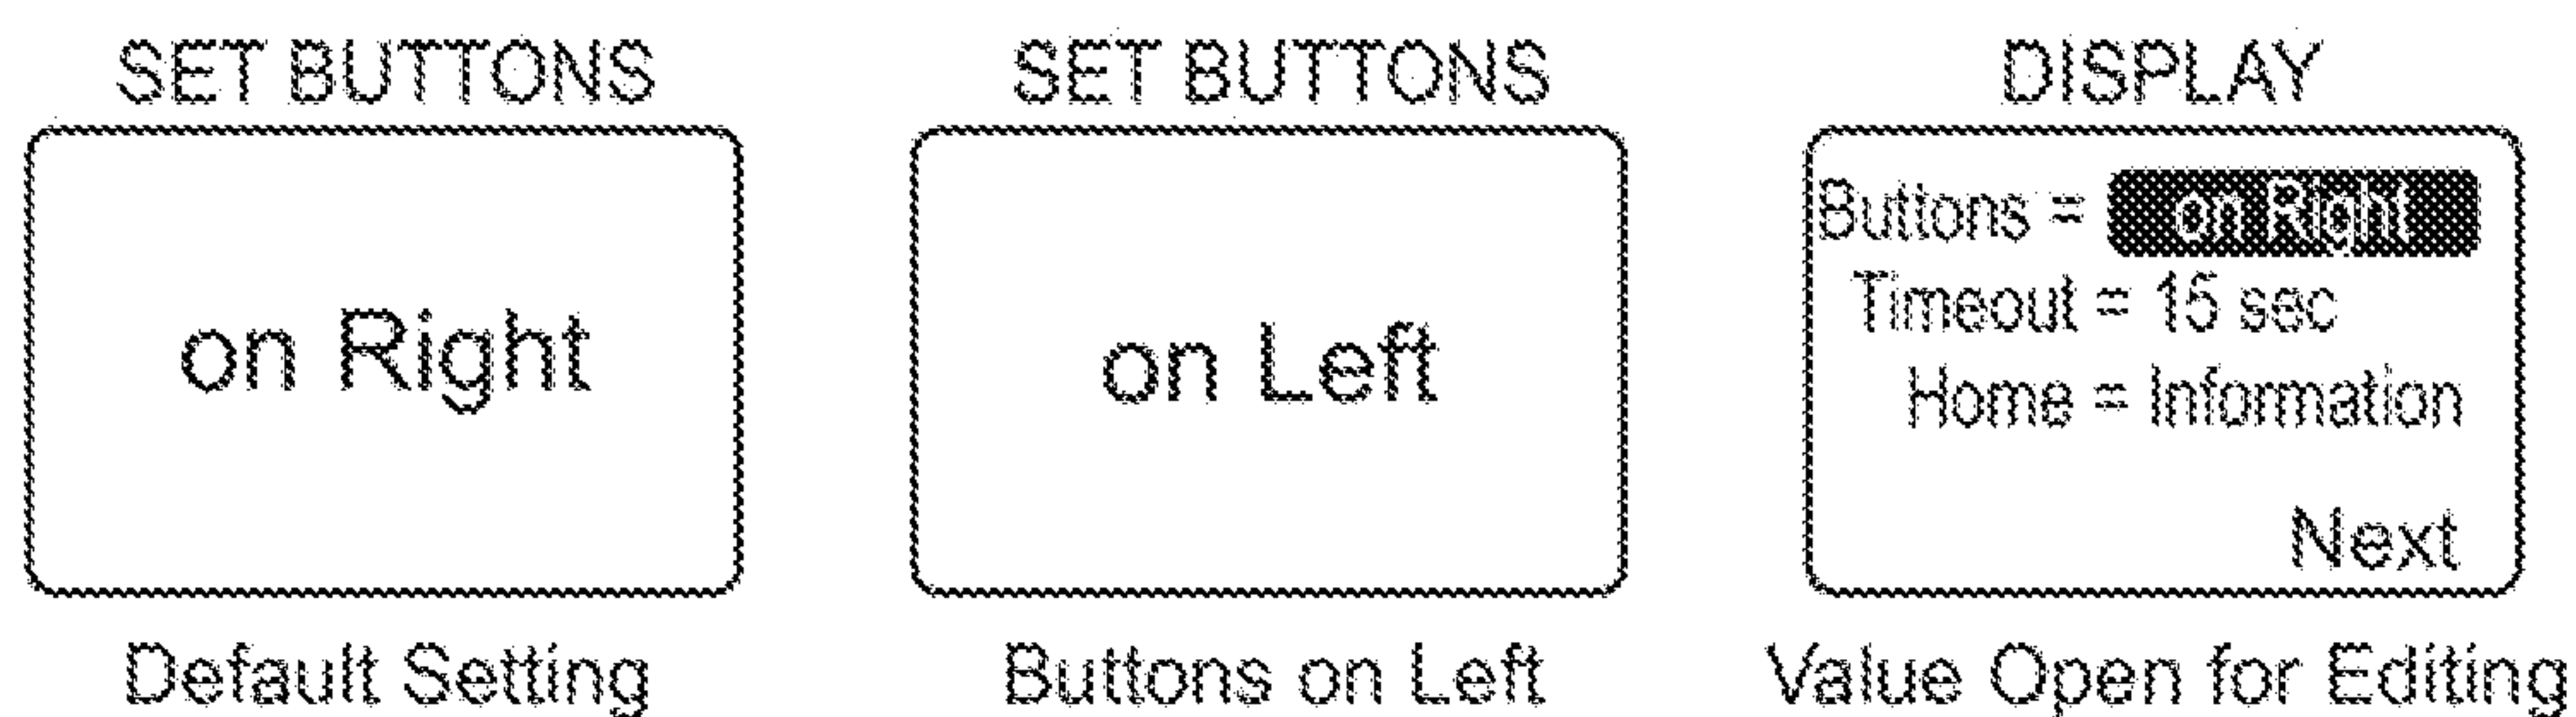


FIG. 9B

13/42

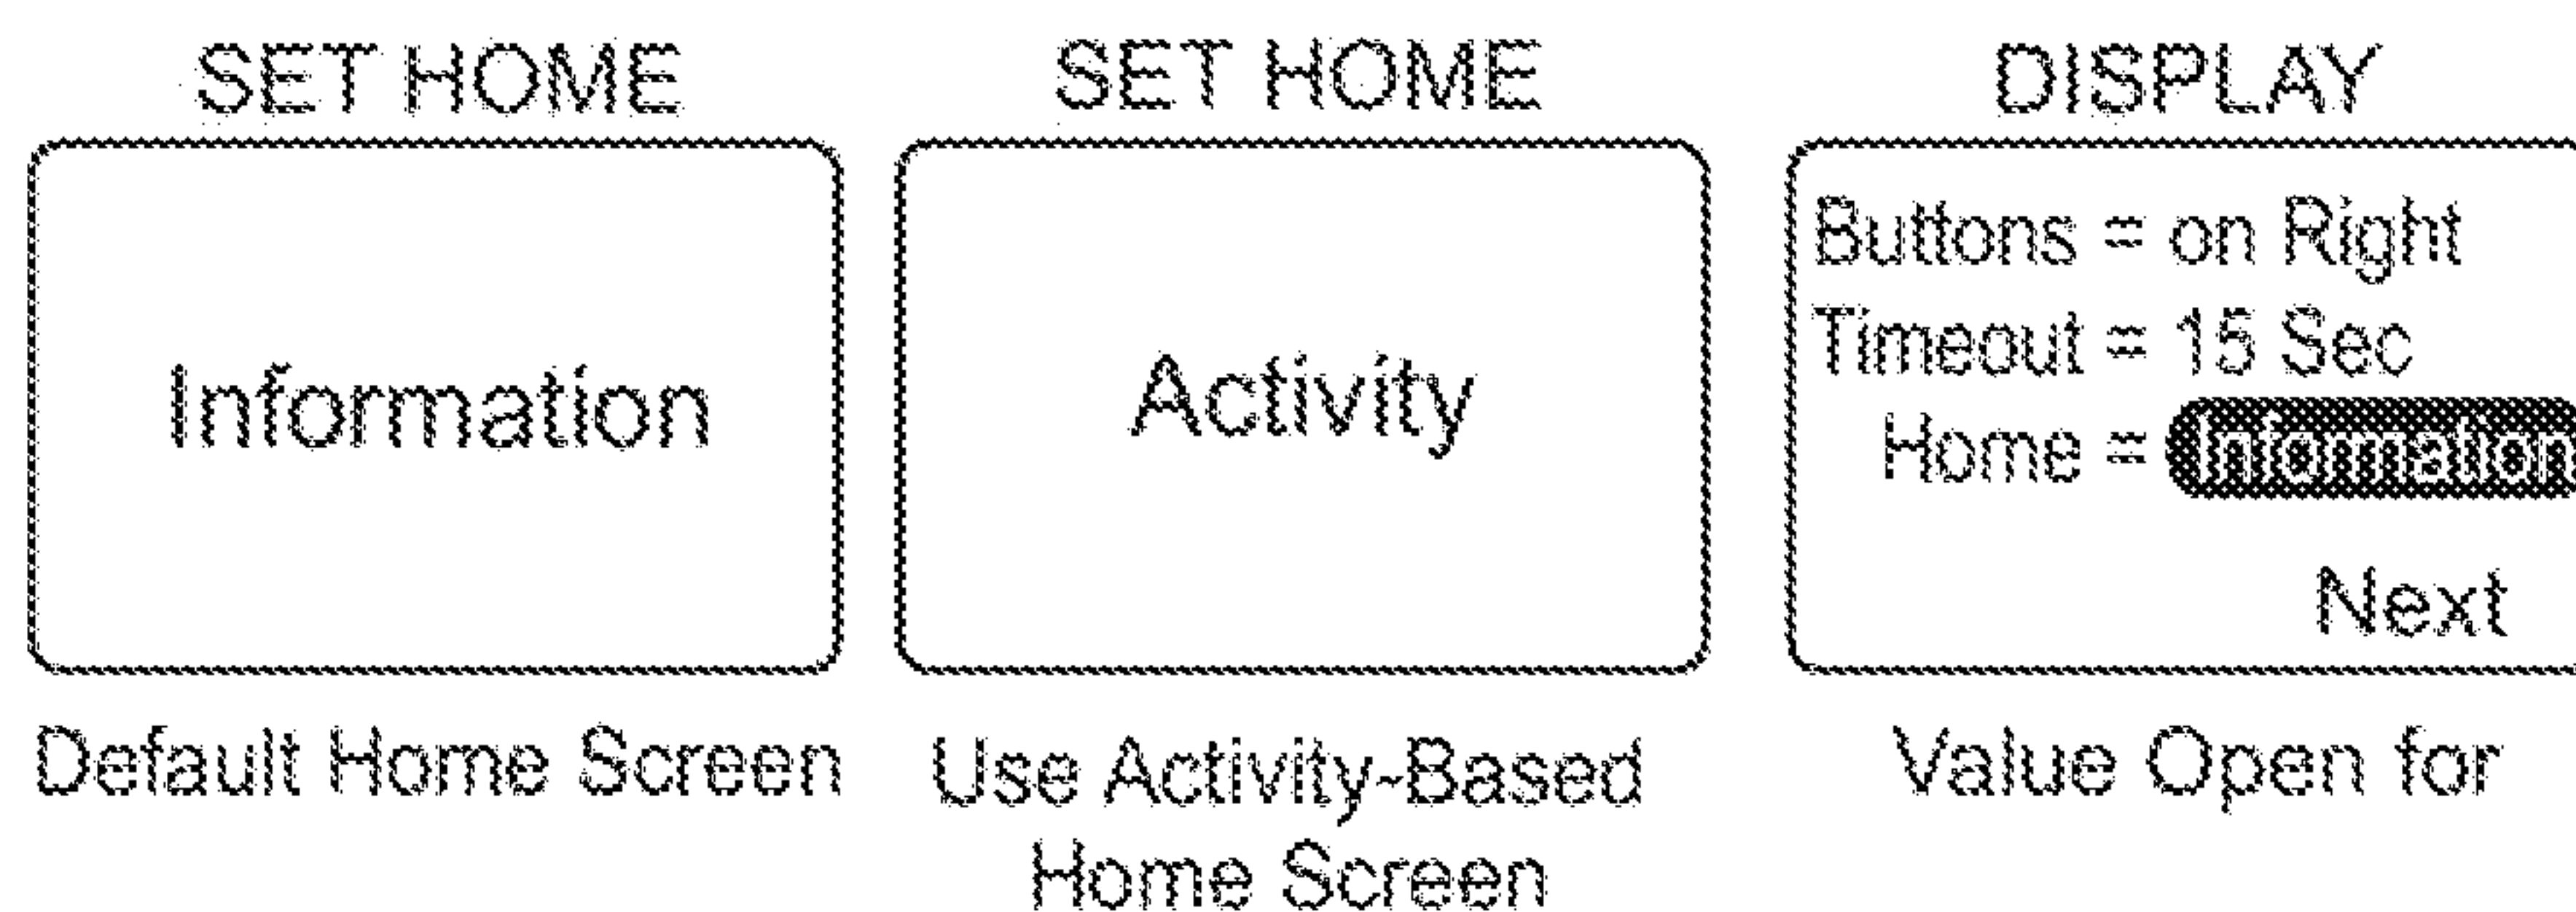


FIG. 10A

Activity-Based Home Screen on Pump - Magnify Off

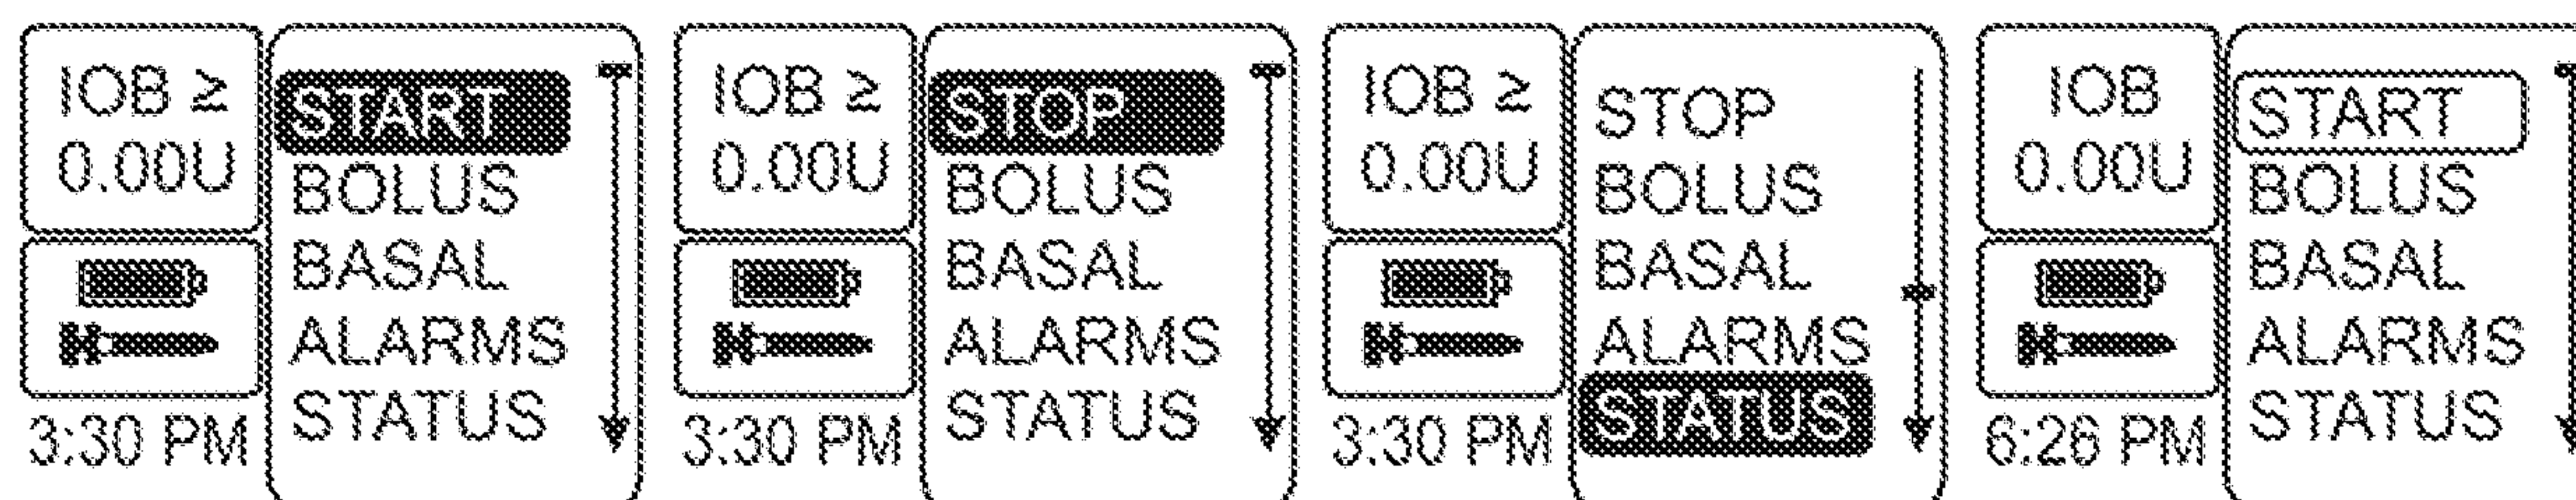


FIG. 10B

Activity-Based Home Screen on Pump - Magnify On

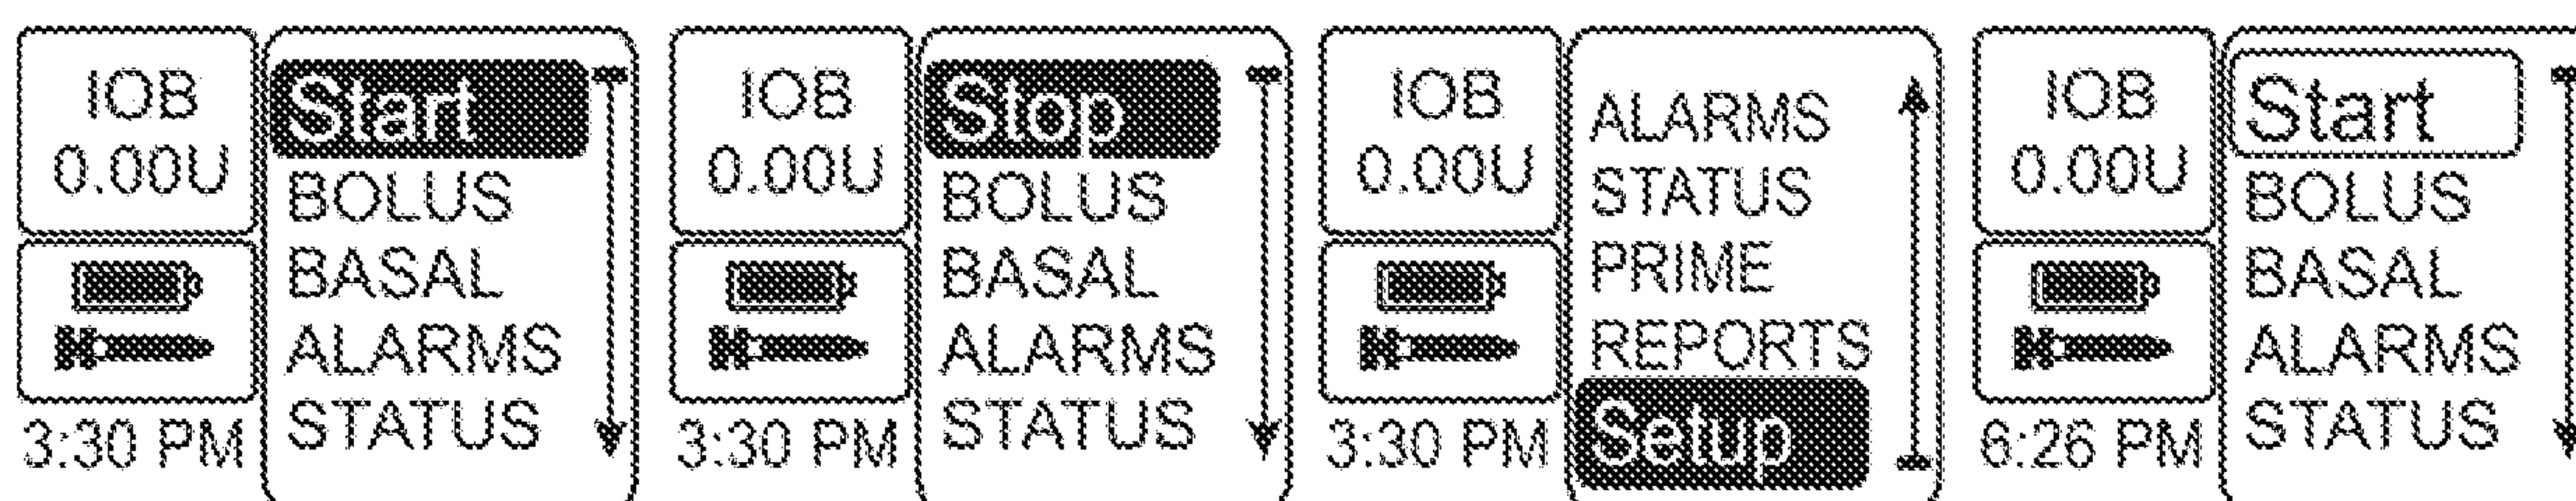


FIG. 10C

14/42

Information-Based Home Screen on Pump - Magnify On

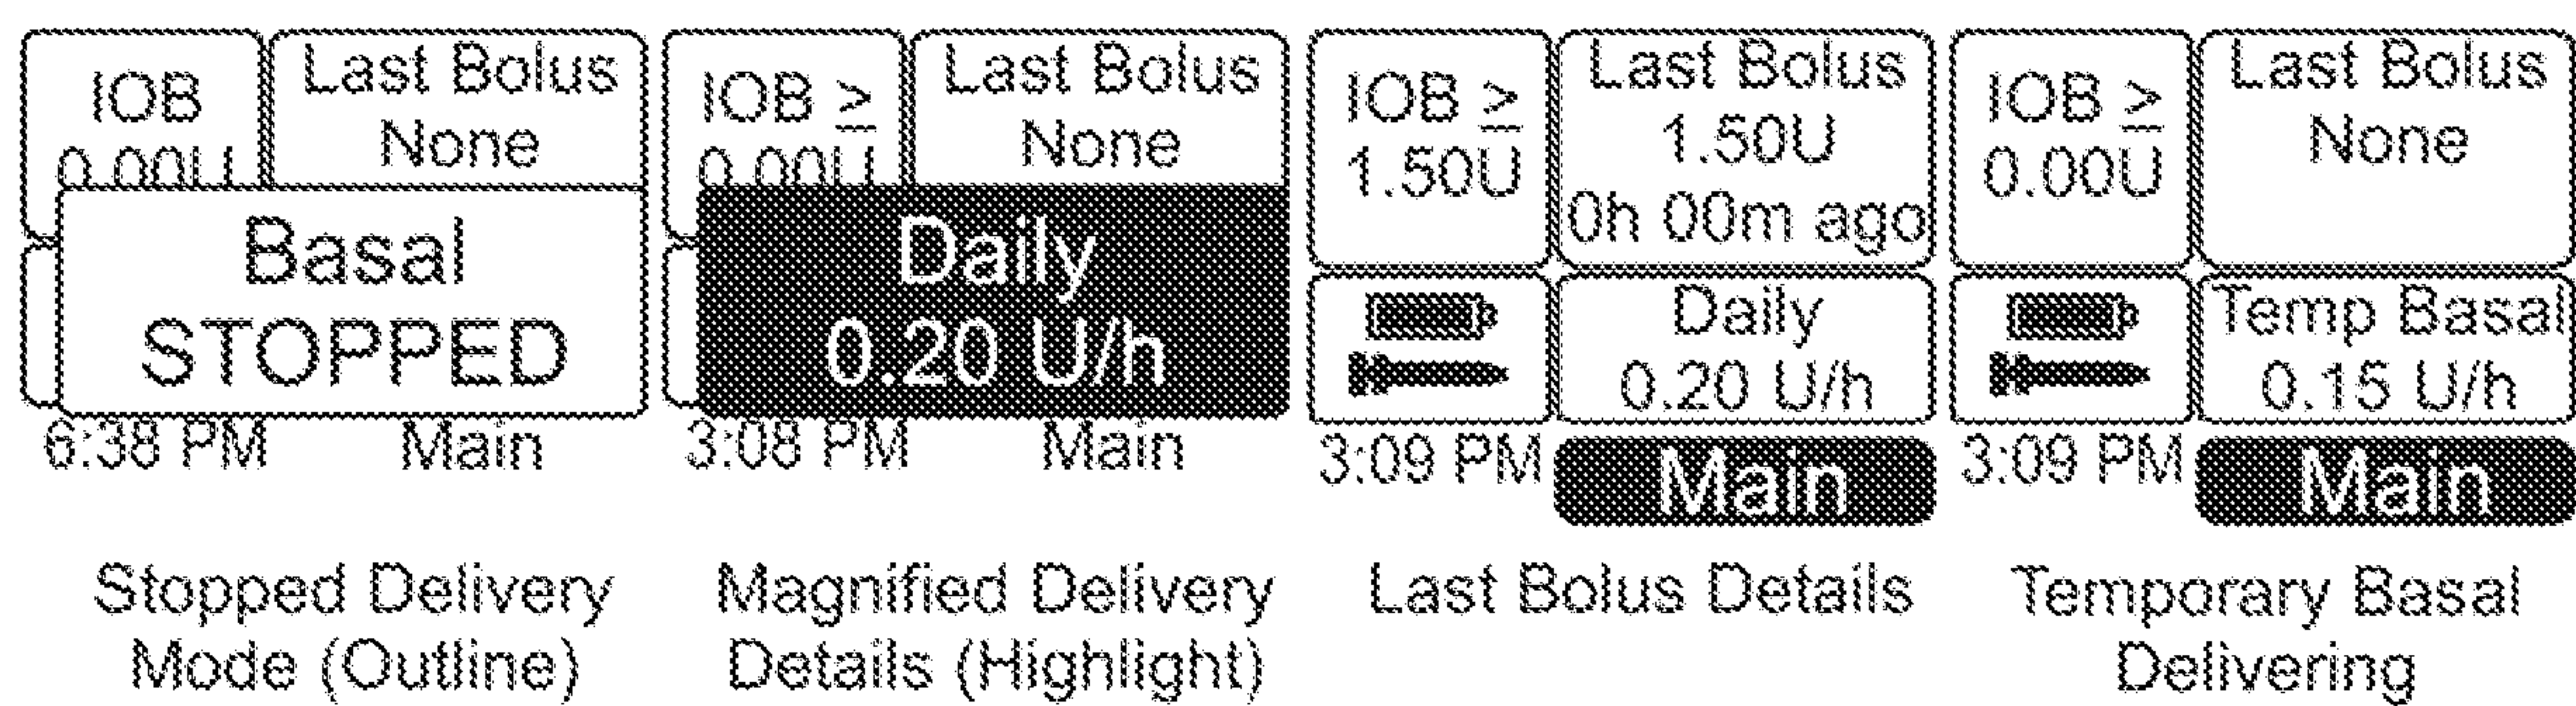


FIG. 10D

Information-Based Home Screen on Pump - Magnify Off (Highlight Cursor Only)

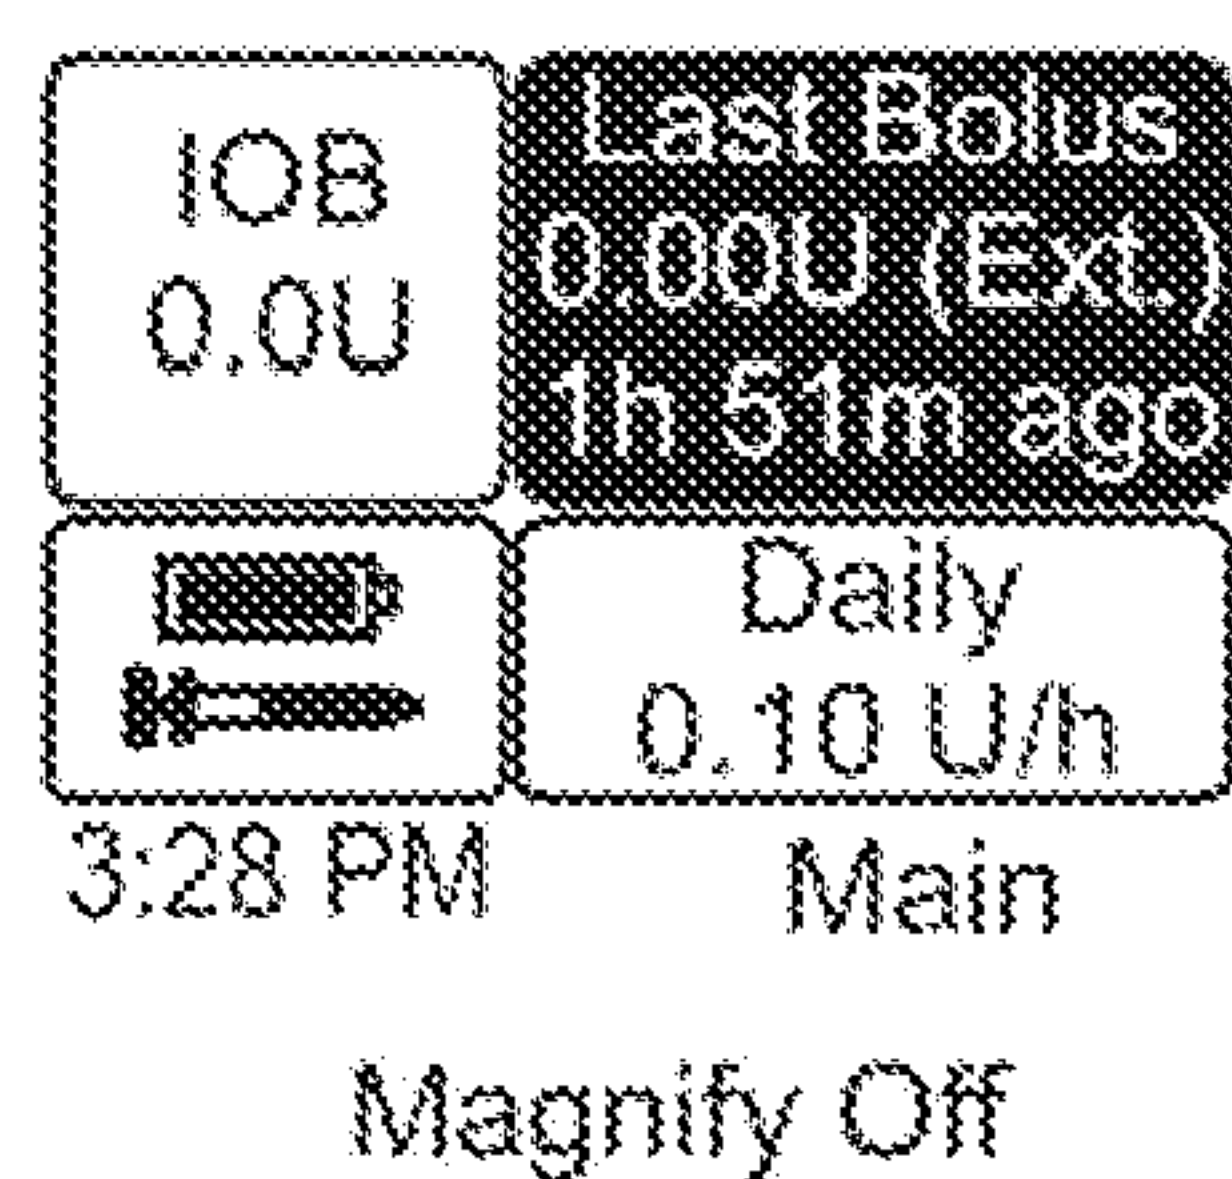


FIG. 10E

15/42

1U DROP	1U DROP 1	1U DROP 5	1U DROP 2
Time mg/dL --- Add Block Next	Time mg/dL 12:00 AM *18 Add Block Next	Time mg/dL 01:00 AM *22 05:00 PM 10 Add Block Next	Time mg/dL 12:00 AM 18 08:00 AM *10 Add Block Next
Default Selection when no blocks have been created yet	Default Selection when at least 1 block exists	Show Scroll Bar when more than 2 blocks exist	Advance to Next Screen

FIG. 11A

1U DROP	1U DROP 1	1U DROP 5	1U DROP 2
Time mmol/L --- Add Block Next	Time mmol/L 12:00 AM *1.0 Add Block Next	Time mmol/L 01:00 *1.2 17:00 0.6 Add Block Next	Time mmol/L 12:00 AM 1.0 08:00 AM *0.6 Add Block Next

FIG. 11B

16/42

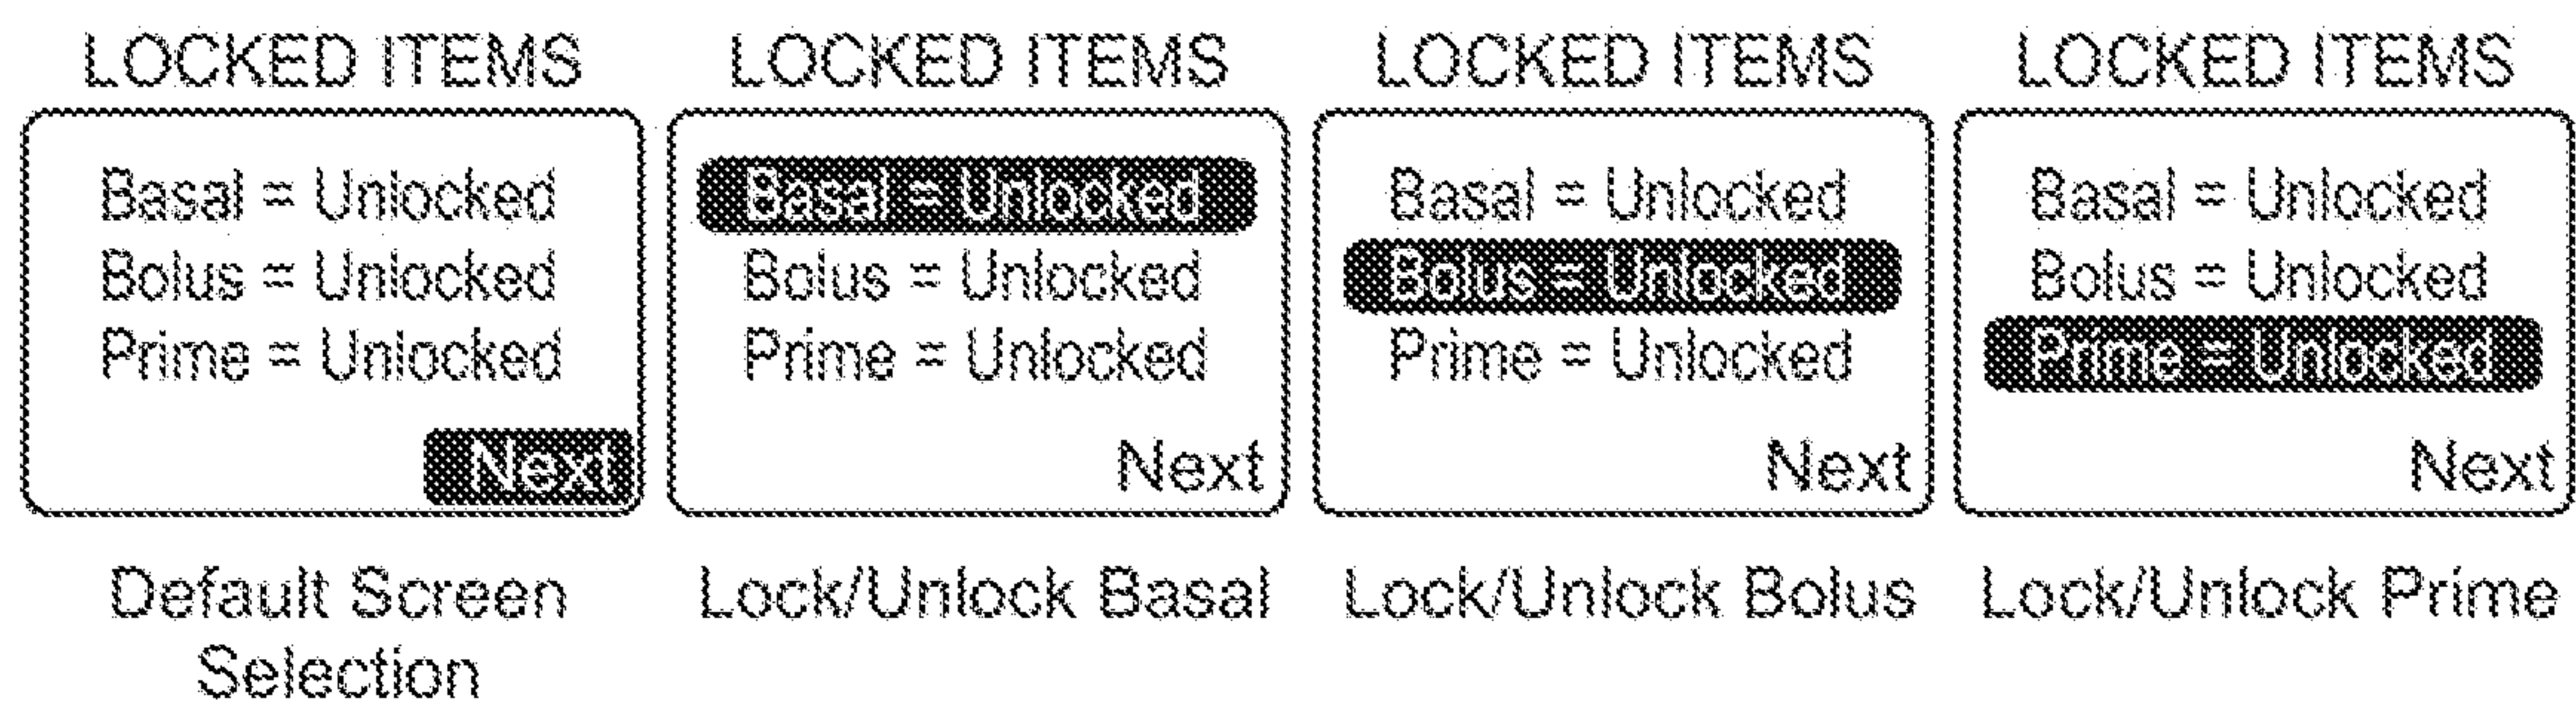


FIG. 12

17/42



FIG. 13A



FIG. 13B

18/42


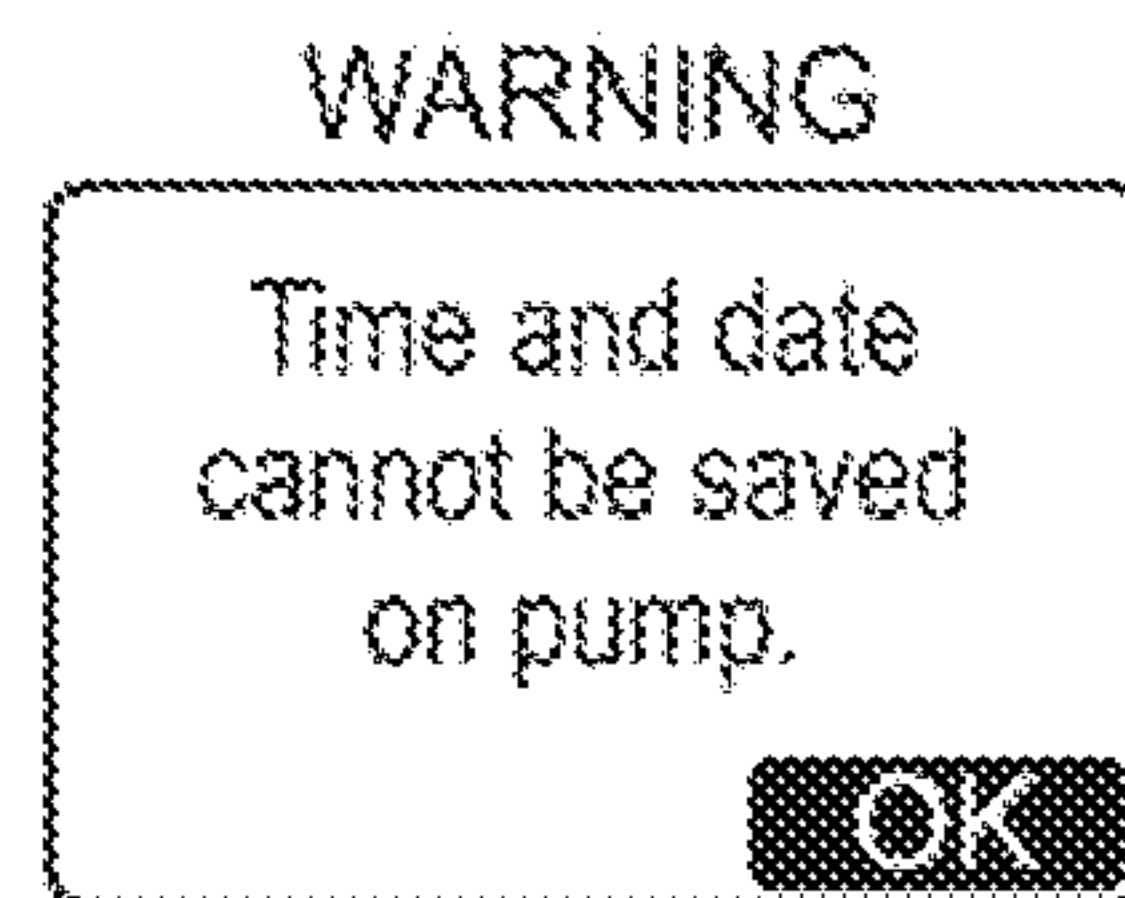


FIG. 14A

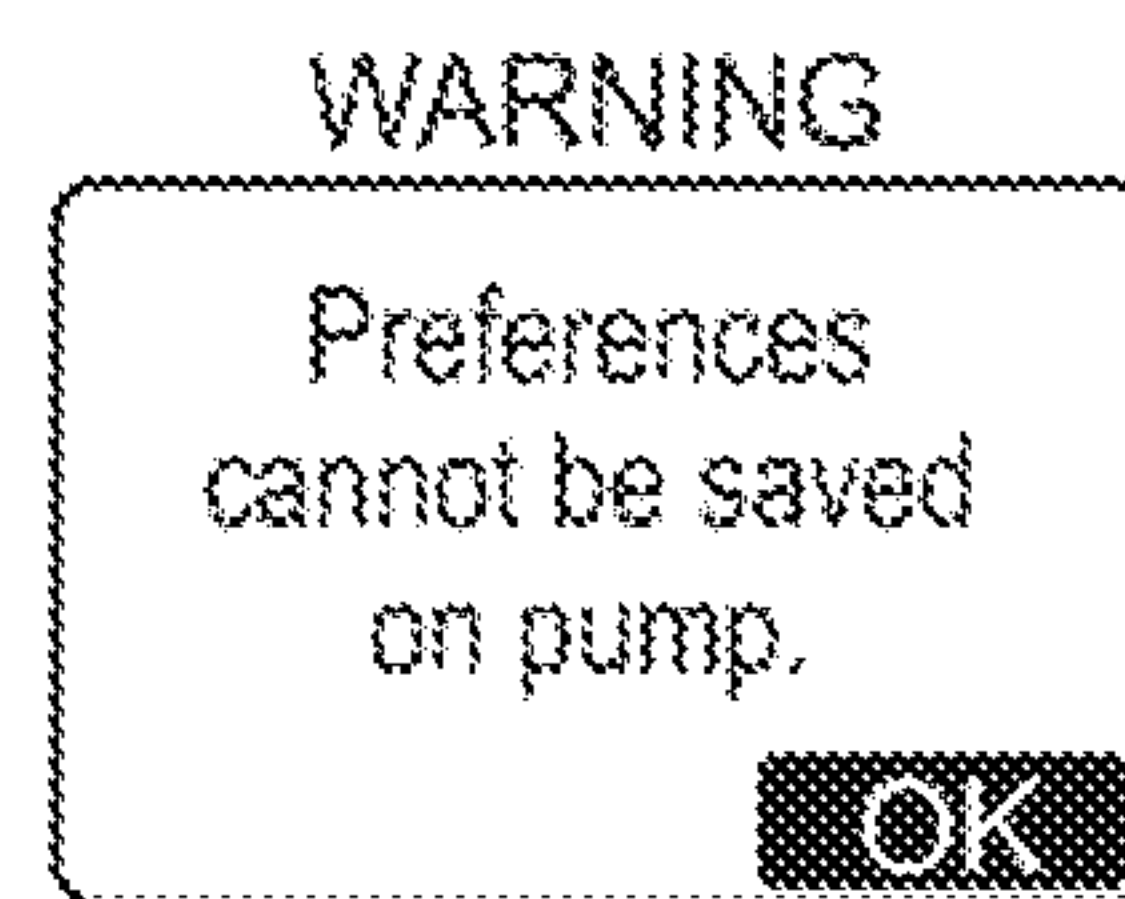

Companion not
Communicating with
Pump

FIG. 14B

19/42

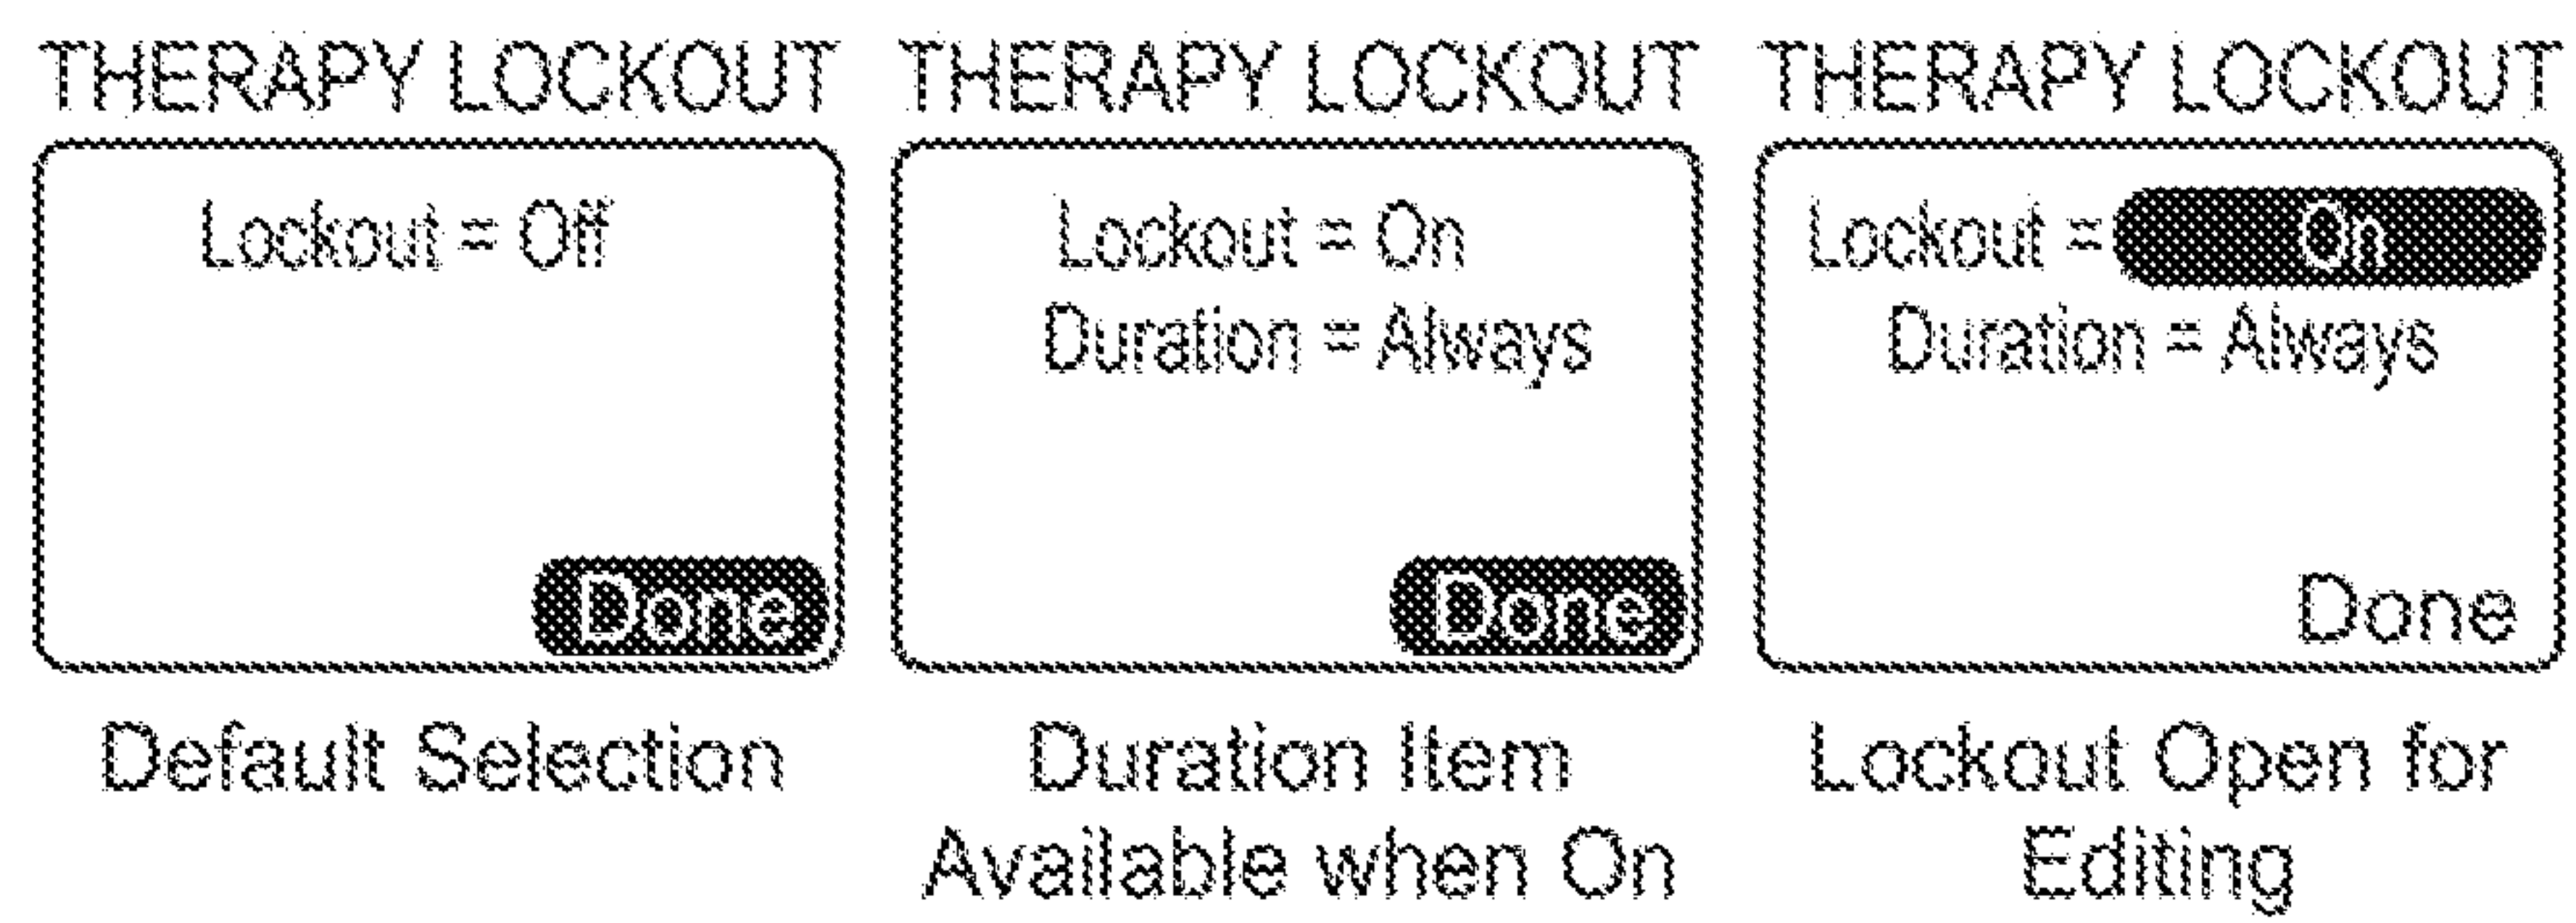


FIG. 15

20/42

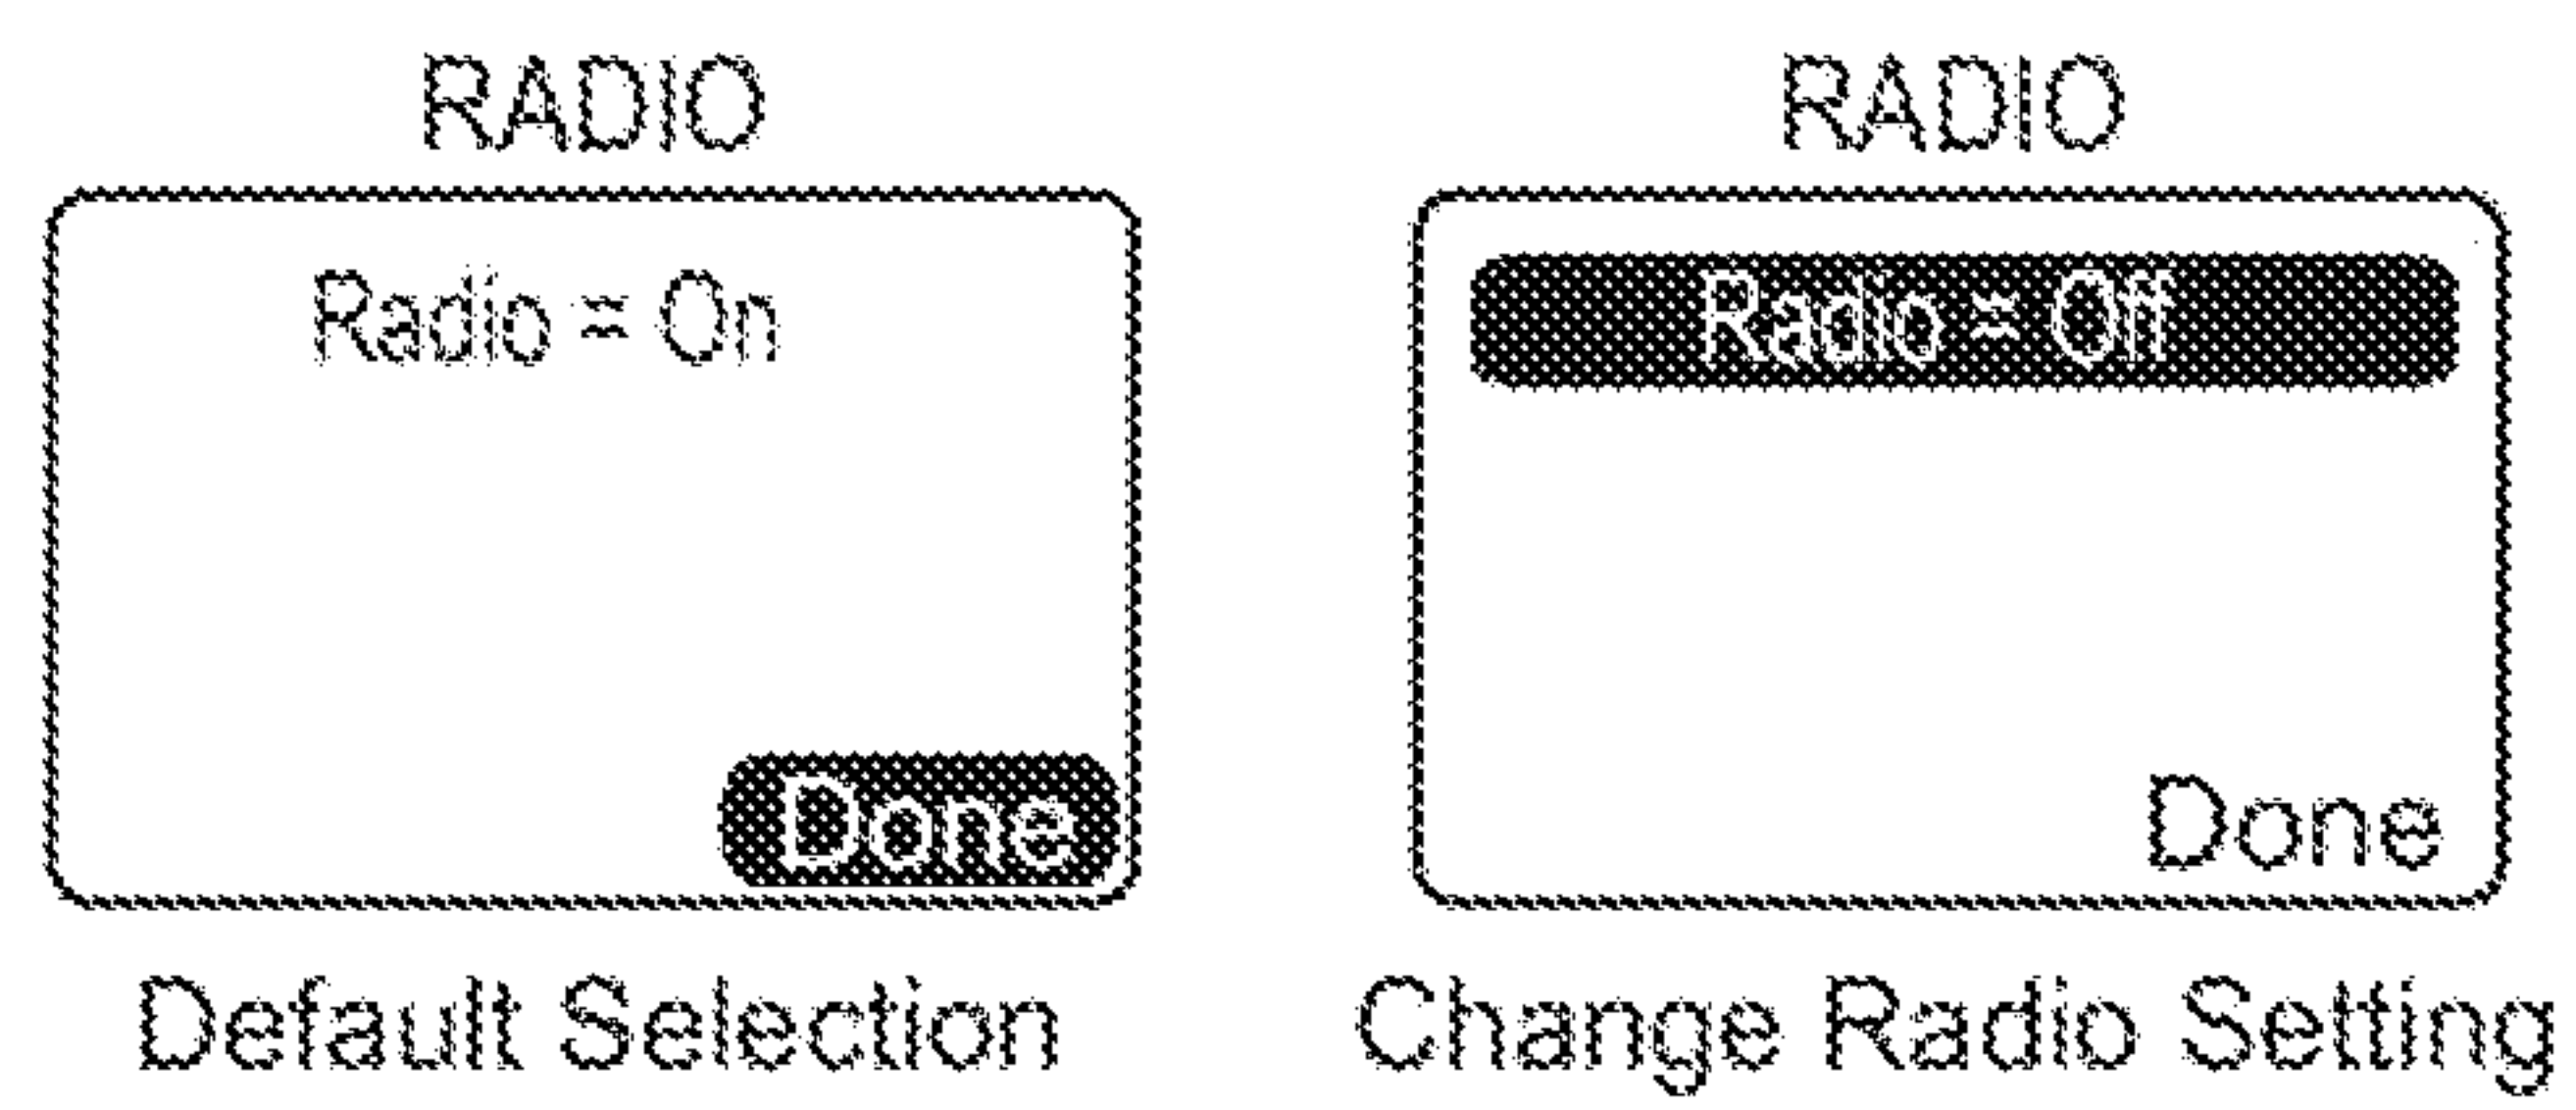


FIG. 16

21/42

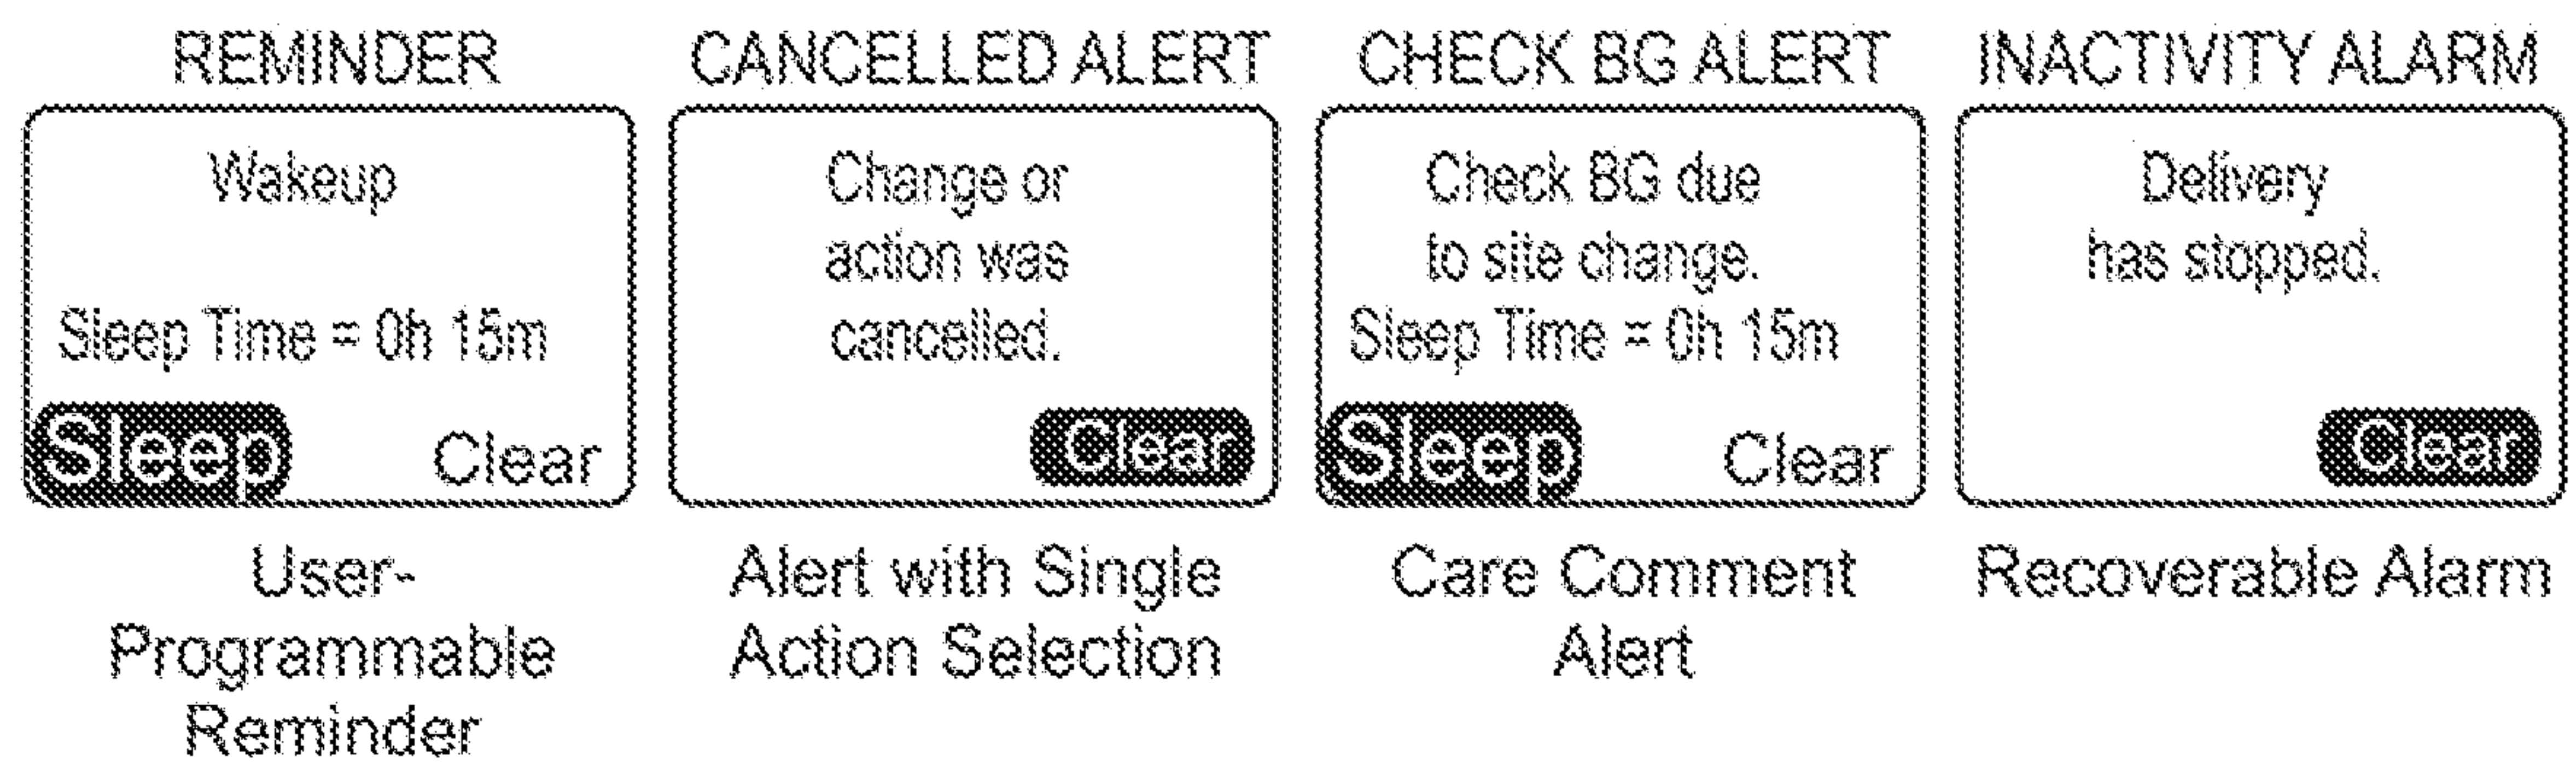


FIG. 17

22/42

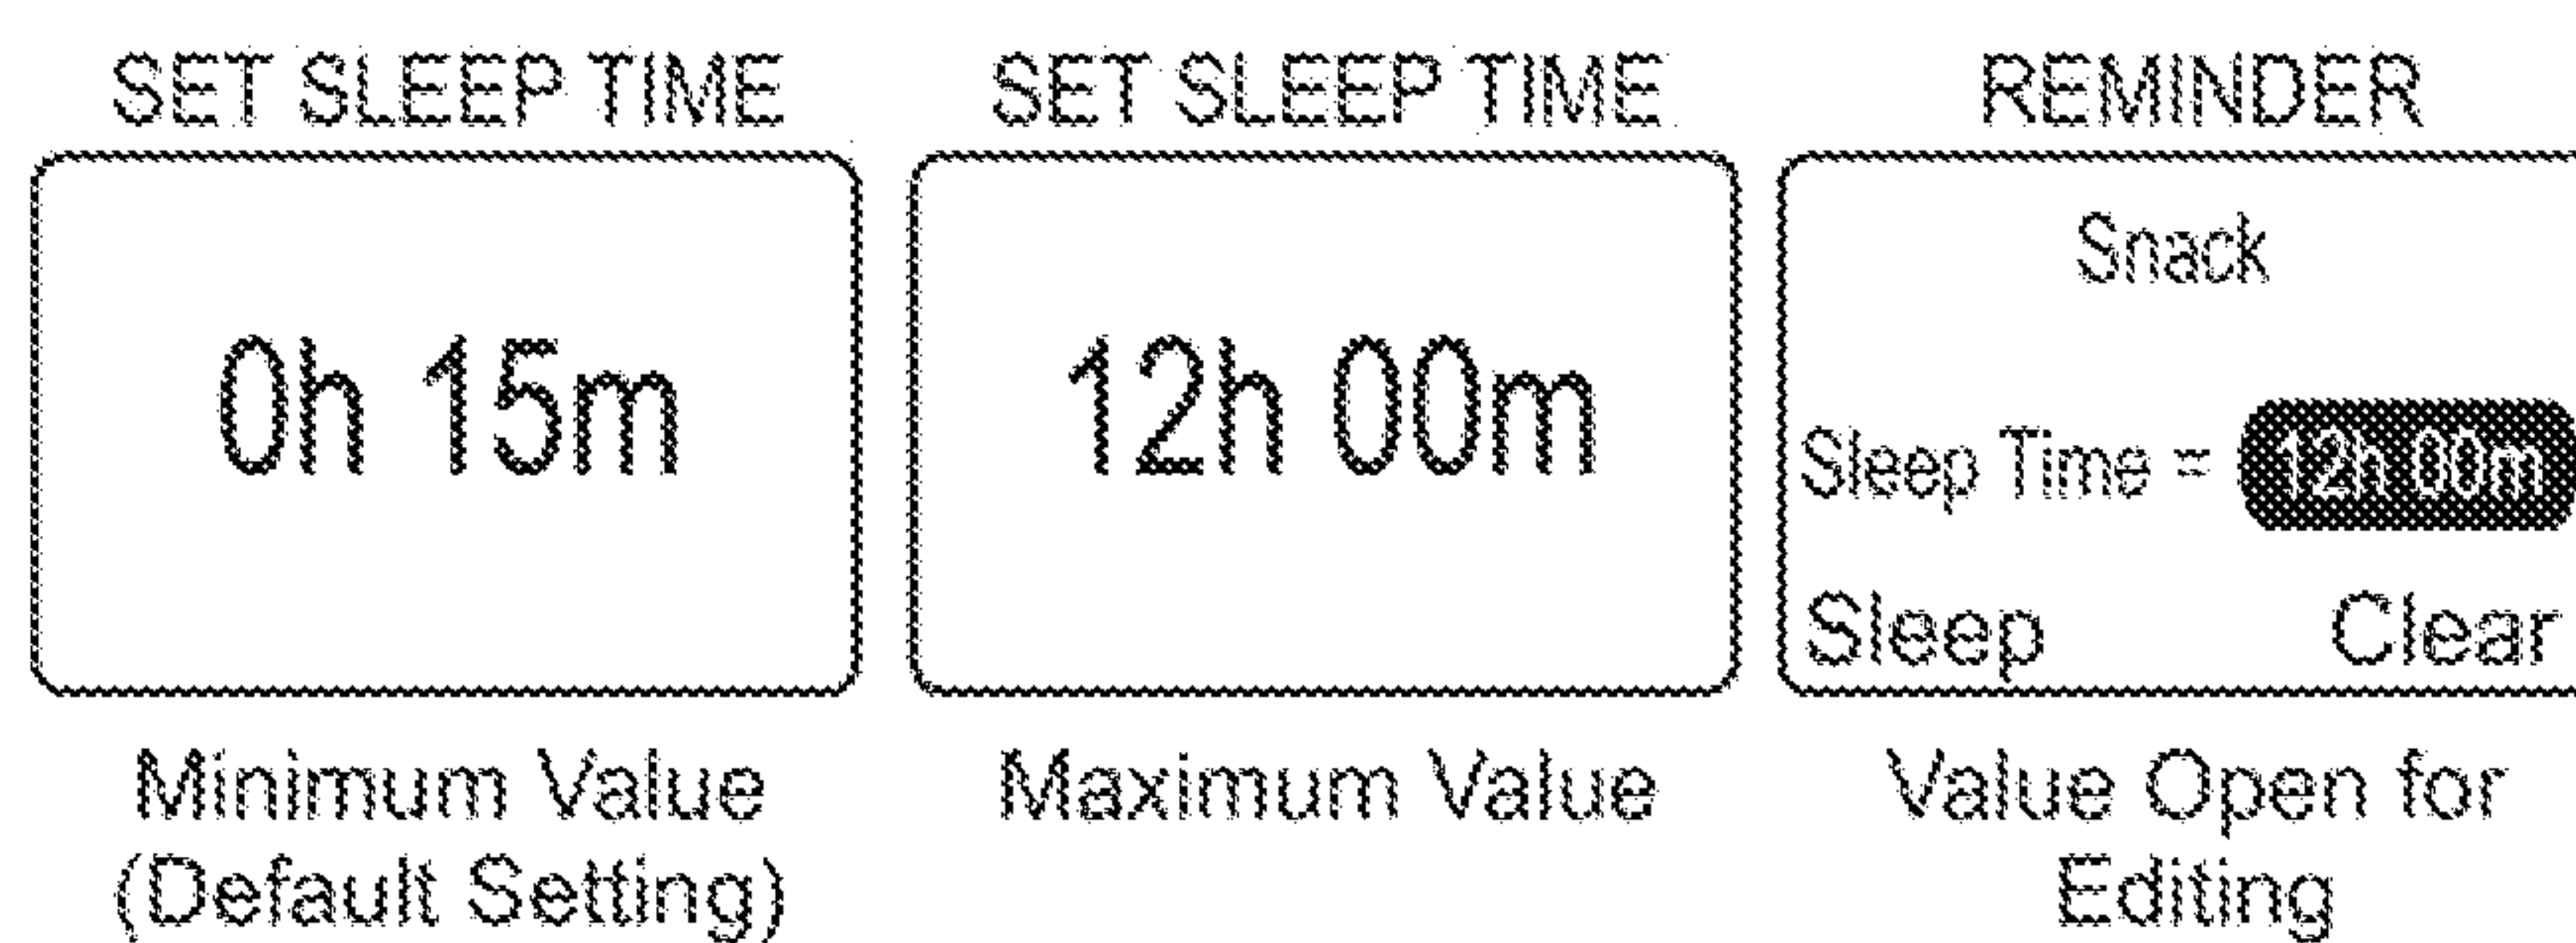


FIG. 18A

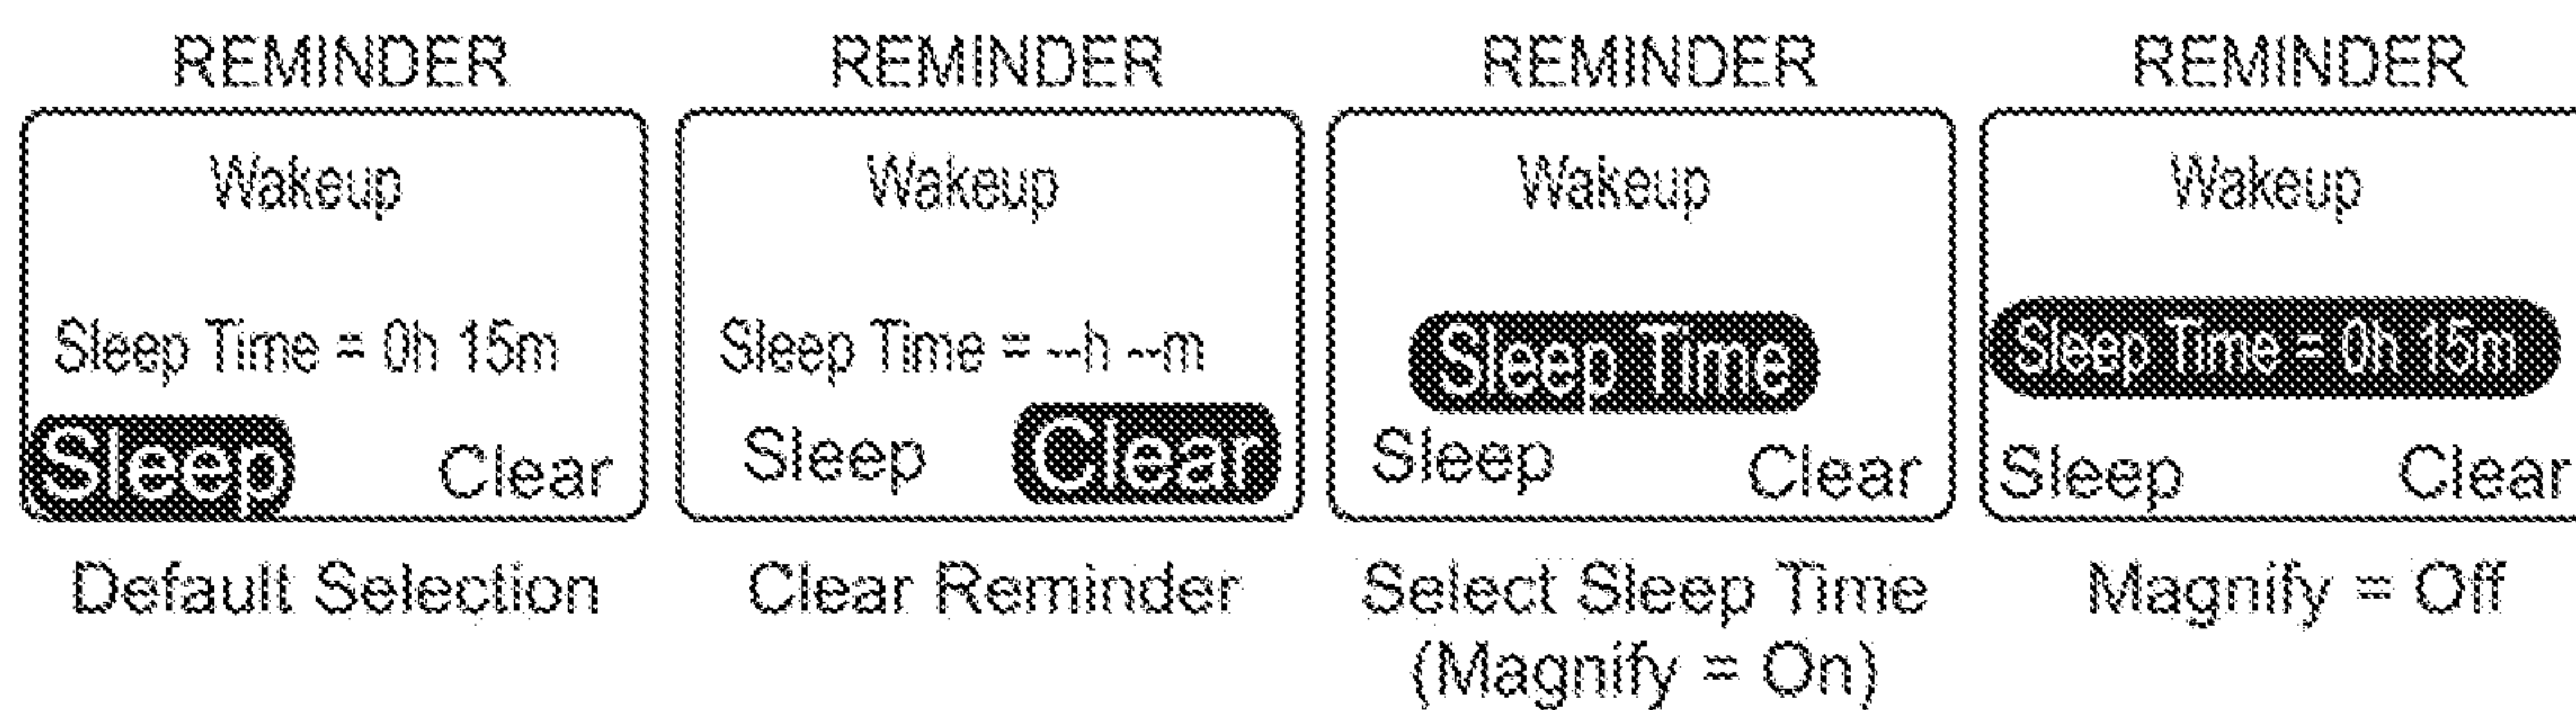


FIG. 18B

23/42

OCCLUSION ALARM



Clear the Alarm

FIG. 19A


RESERVOIR ALARM



Clear the Alarm

FIG. 19B

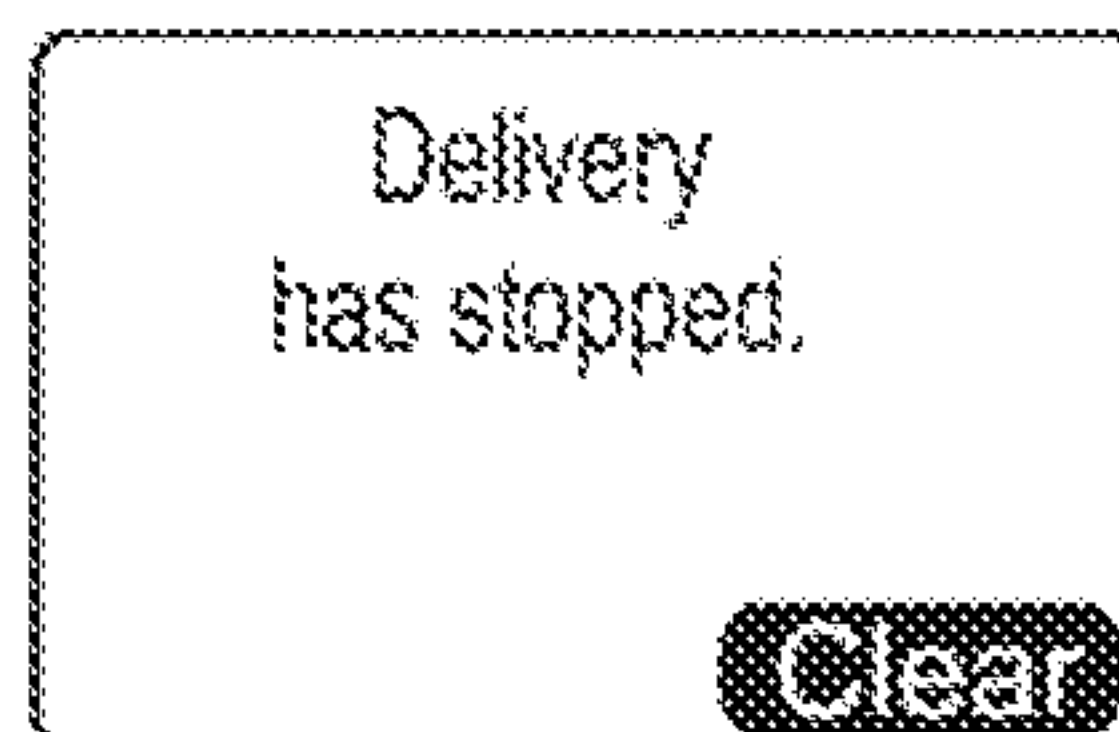BAD BATTERY ALARM



Clear the Alarm

FIG. 19C

24/42

NO INSULIN ALARM



Clear the Alarm

FIG. 19D

INACTIVITY ALARM



Alarm after 15 minutes

FIG. 19E

25/42

LOW BATTERY ALERT LOW BATTERY ALERT LOW BATTERY ALERT

Replace the battery. Sleep Time = 0h 15m Sleep Clear	Replace the battery. Sleep Time = --h --m Sleep Clear	Replace the battery. Sleep Time Sleep Clear
---	--	--

Sleep the Alert
(Default Selection)

Clear the Alert

Select Sleep Time

FIG. 20A

LOW INSULIN ALERT LOW INSULIN ALERT LOW INSULIN ALERT LOW INSULIN ALERT

Refill the reservoir. Sleep Time = 0h 15m Sleep Clear	Refill the reservoir. Sleep Time = --h --m Sleep Clear	Refill the reservoir. Sleep Time Sleep Clear	Refill the reservoir. Sleep Time = 0h 15m Sleep Clear
--	---	---	--

Sleep the Alert
(Default Selection)

Clear the Alert

Select Sleep Time
(Magnify = On)

Magnify = Off

FIG. 20B

INACTIVITY ALERT

Press enter to reset. Clear

Alert First

FIG. 20C

PUMP IDLE ALERT

PUMP IDLE ALERT

PUMP IDLE ALERT

Pump not started. Sleep Time = 0h 15m Sleep Clear	Pump not started. Sleep Time = --h --m Sleep Clear	Pump not started. Sleep Time Sleep Clear
--	---	---

Sleep the Alert
(Default Selection)

Clear the Alert

Select Sleep Time

FIG. 20D

26/42

STOPPED ALERT

Normal bolus
stopped.
1.2 of 10.0U

Clear

Clear the Alarm

FIG. 20E

CANCELLED ALERT

Change or
action was
cancelled.

Clear

Clear the Alert

CANCELLATION ALERT

Change or action
was cancelled.

Clear

Alert Screen Displayed
on the Companion

FIG. 20F

CHECK BG ALERT

Check BG due
to site change.
Sleep Time = 0h 15m

Sleep Clear

Default Selection

FIG. 20G

SITE CHANGE ALERT

Time for
site change.
Sleep Time = 0h 15m

Sleep Clear

Default Selection

FIG. 20H

27/42

INSULIN TEMP ALERT

High temp.
Insulin at risk.
Sleep Time = 0h 15m
Sleep Clear

Default Selection

FIG. 20I

28/42

12-Hour Time Format

REMINDER 1	REMINDER 1	REMINDER 1	REMINDER 1
Time = 12:00 PM Message = Snack On/Off = On Next Done	Time Message = Snack On/Off = On Next Done	Time = 3:15 PM Message On/Off = On Next Done	Time = 3:15 PM Message = Snack On/Off Next Done
Default Selection	Set Reminder Time	Select Message	Enable/Disable

FIG. 21A

24-Hour Time Format

REMINDER 1	REMINDER 1	REMINDER 1	REMINDER 1
Time = 12:00 PM Message = Snack On/Off = On Next Done	Time Message = Snack On/Off = On Next Done	Time = 15:15 Message On/Off = On Next Done	Time = 15:15 Message = Snack On/Off Next Done
Default Selection	Set Reminder Time	Select Message	Enable/Disable

FIG. 21B

29/42

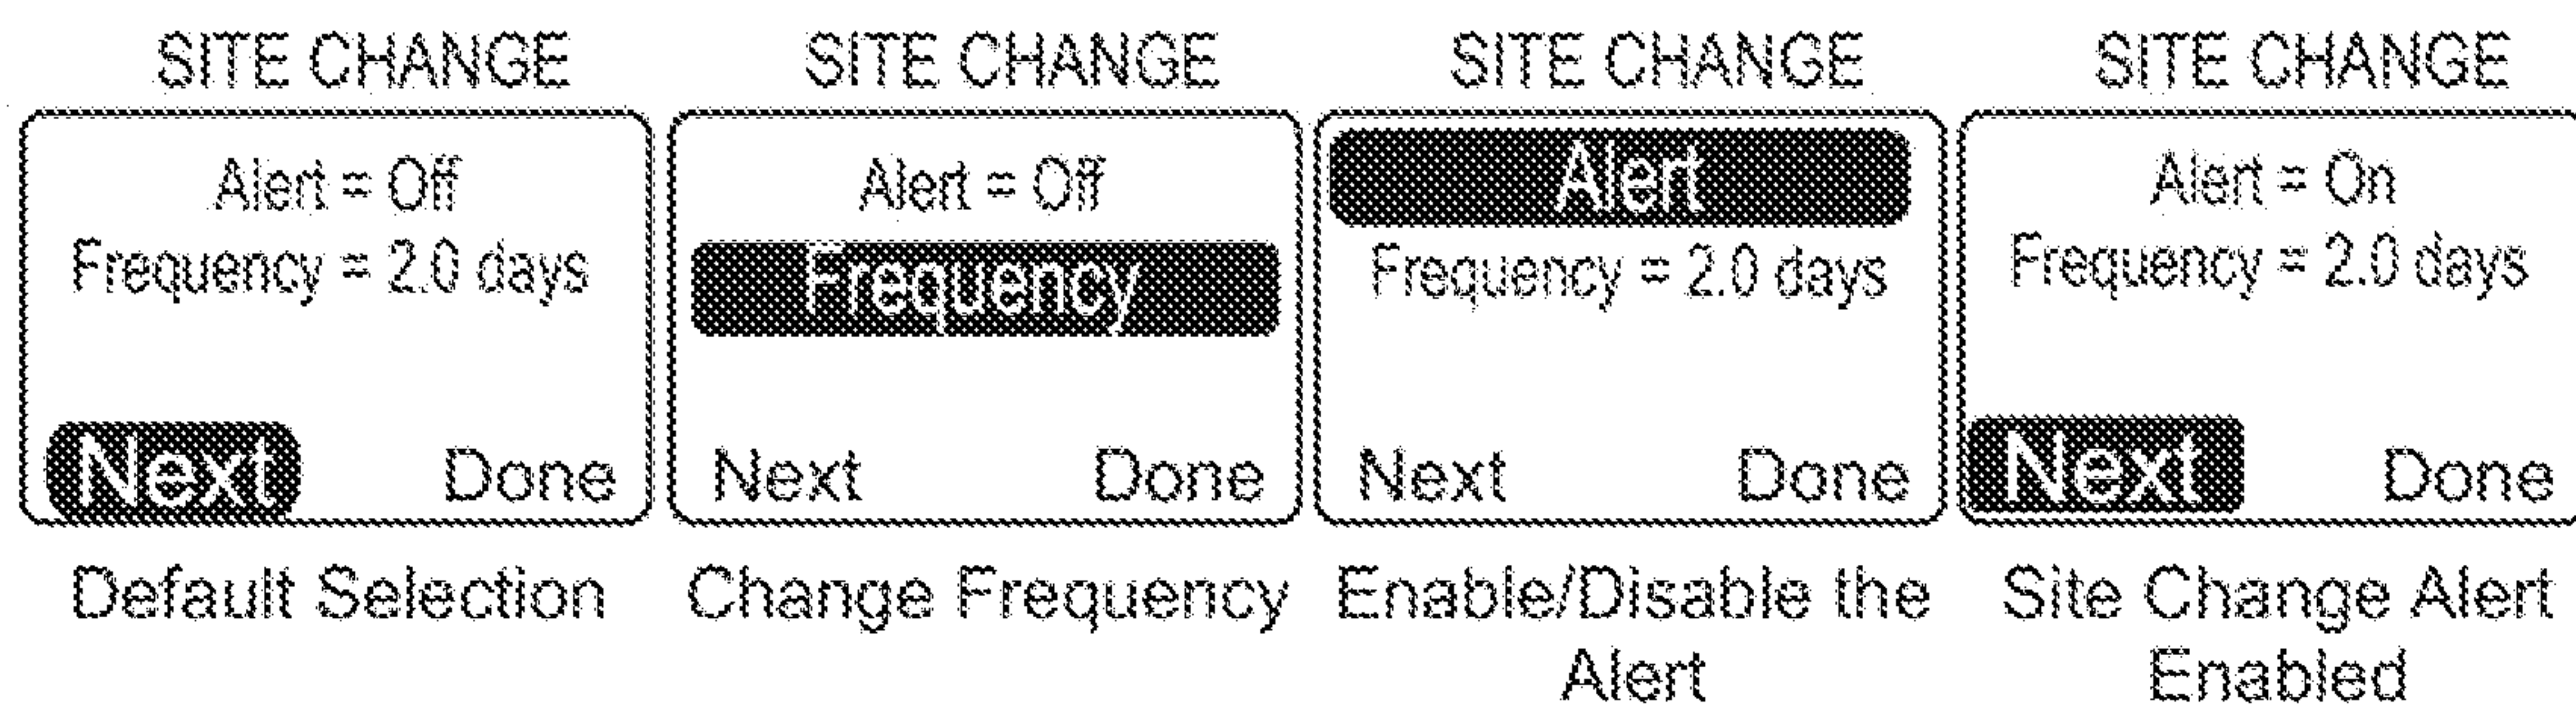


FIG. 22

30/42

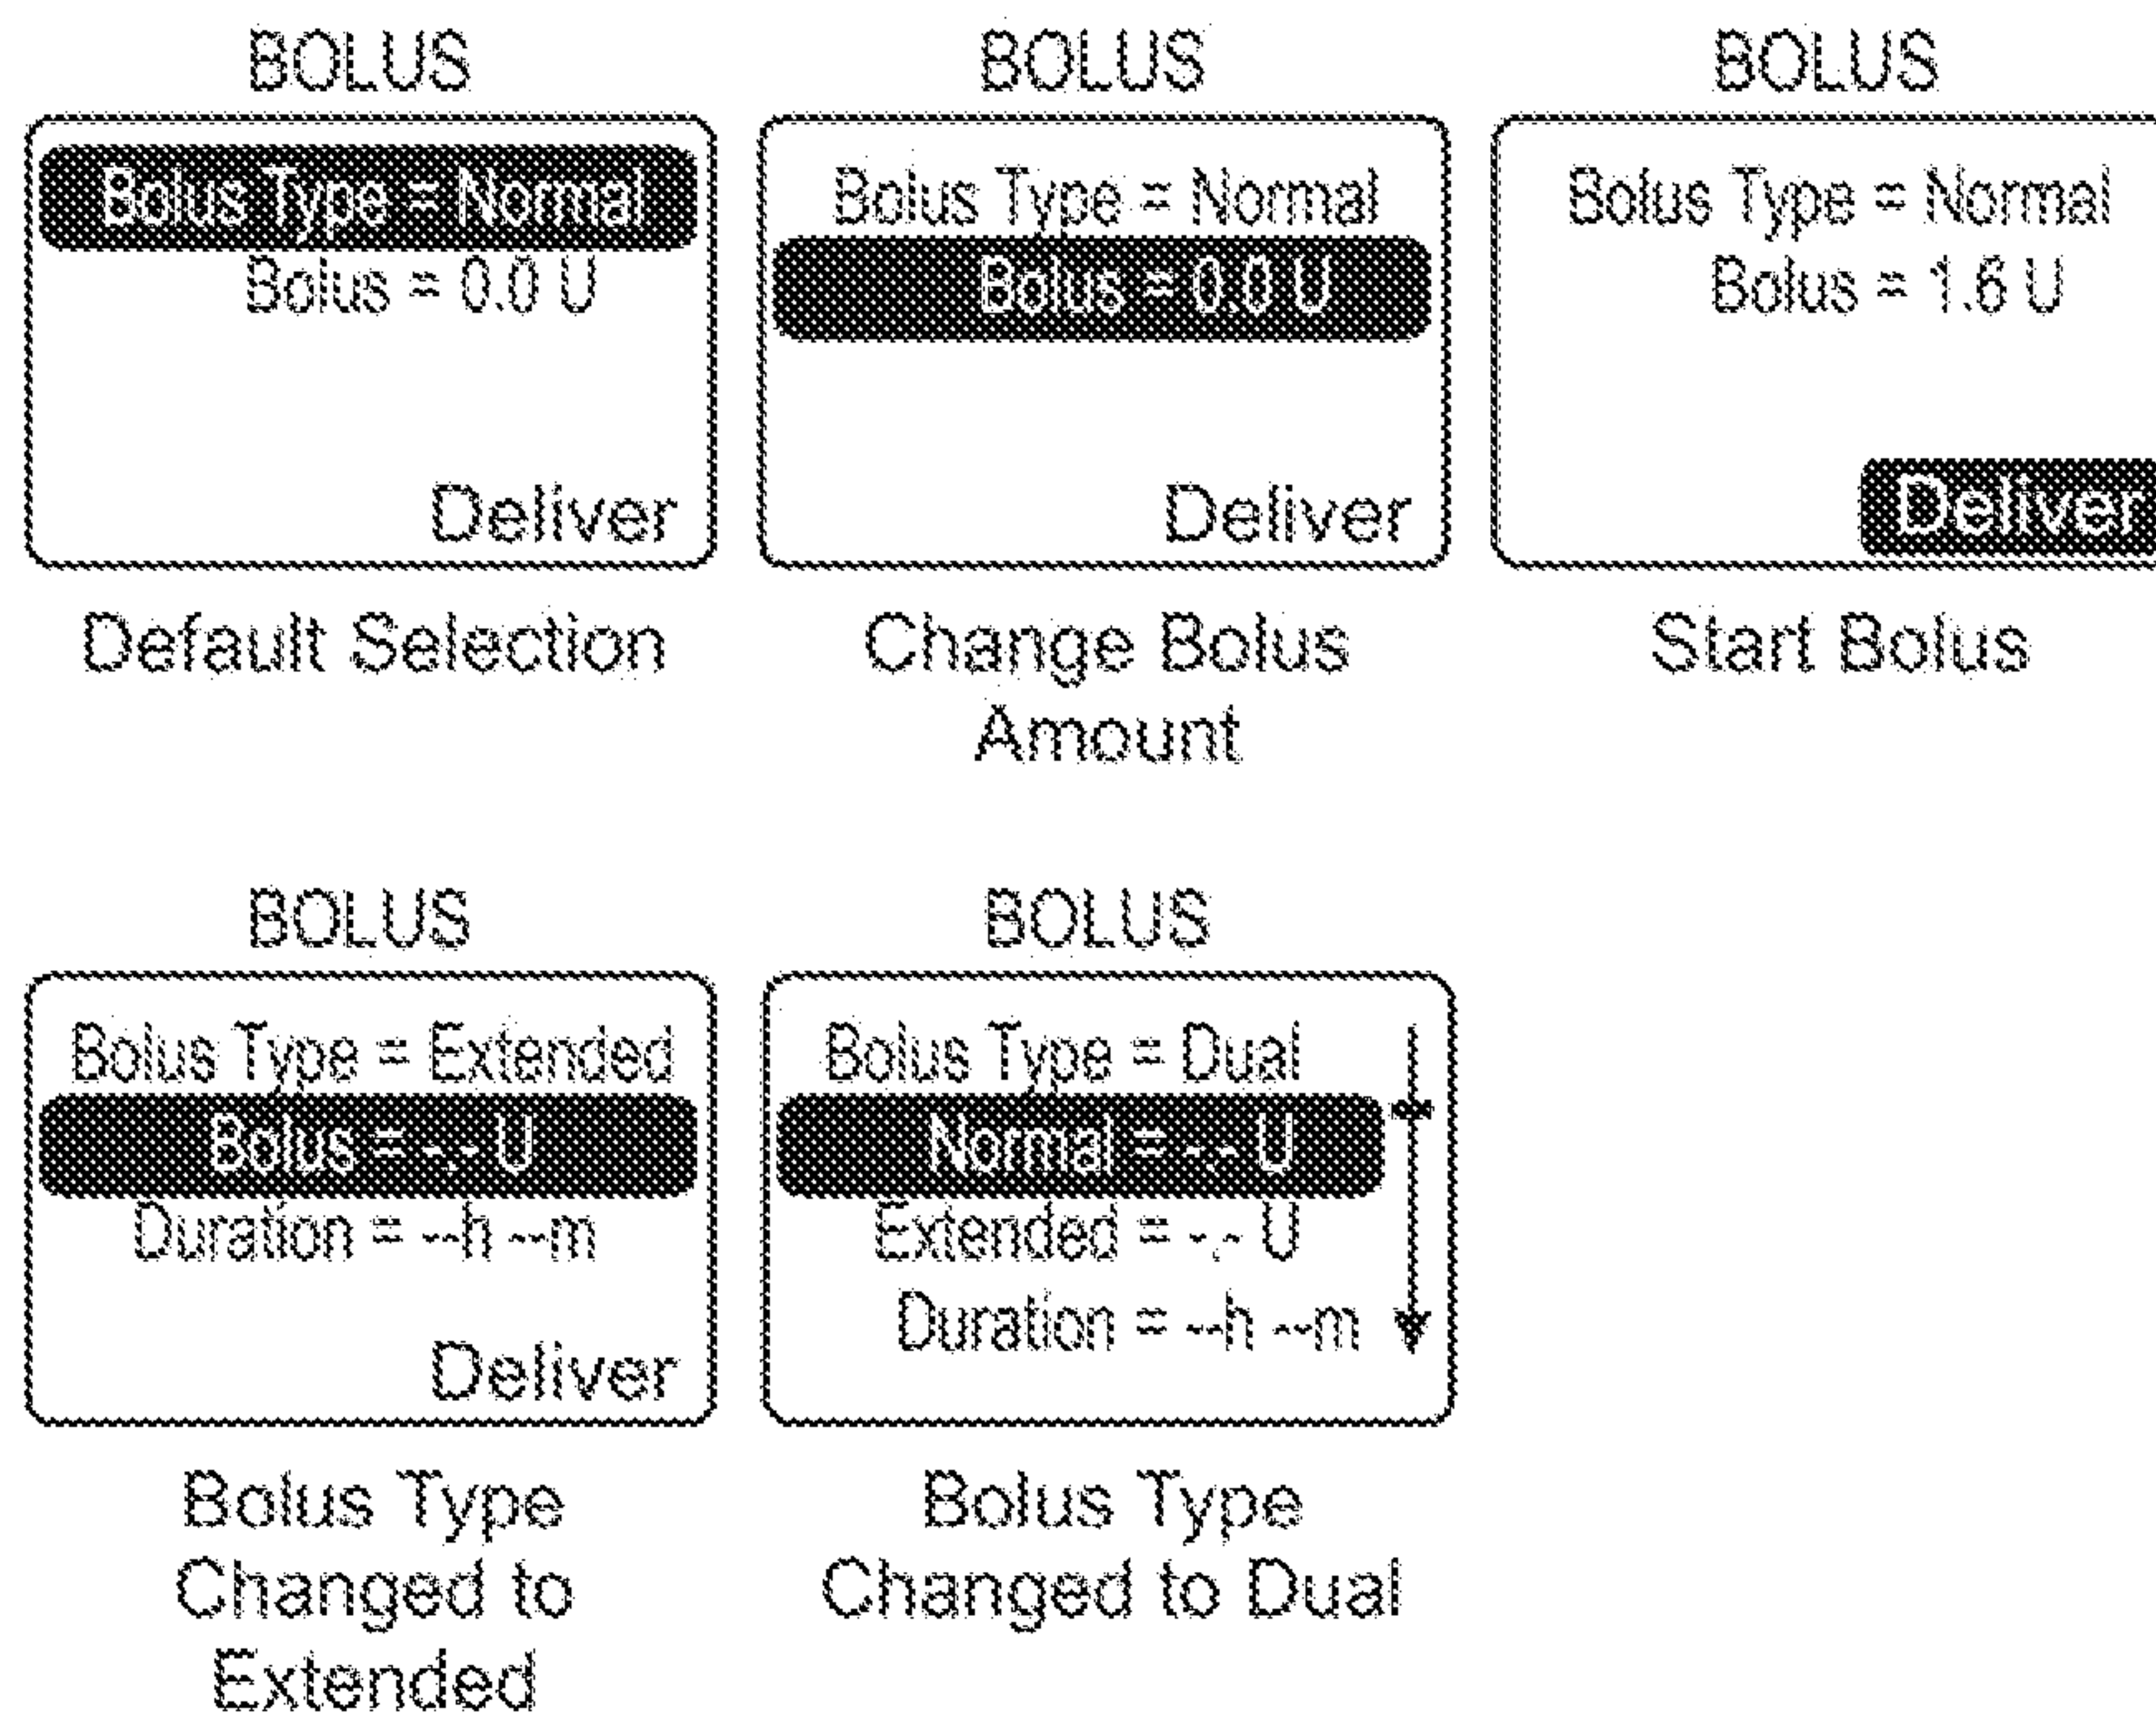


FIG. 23A

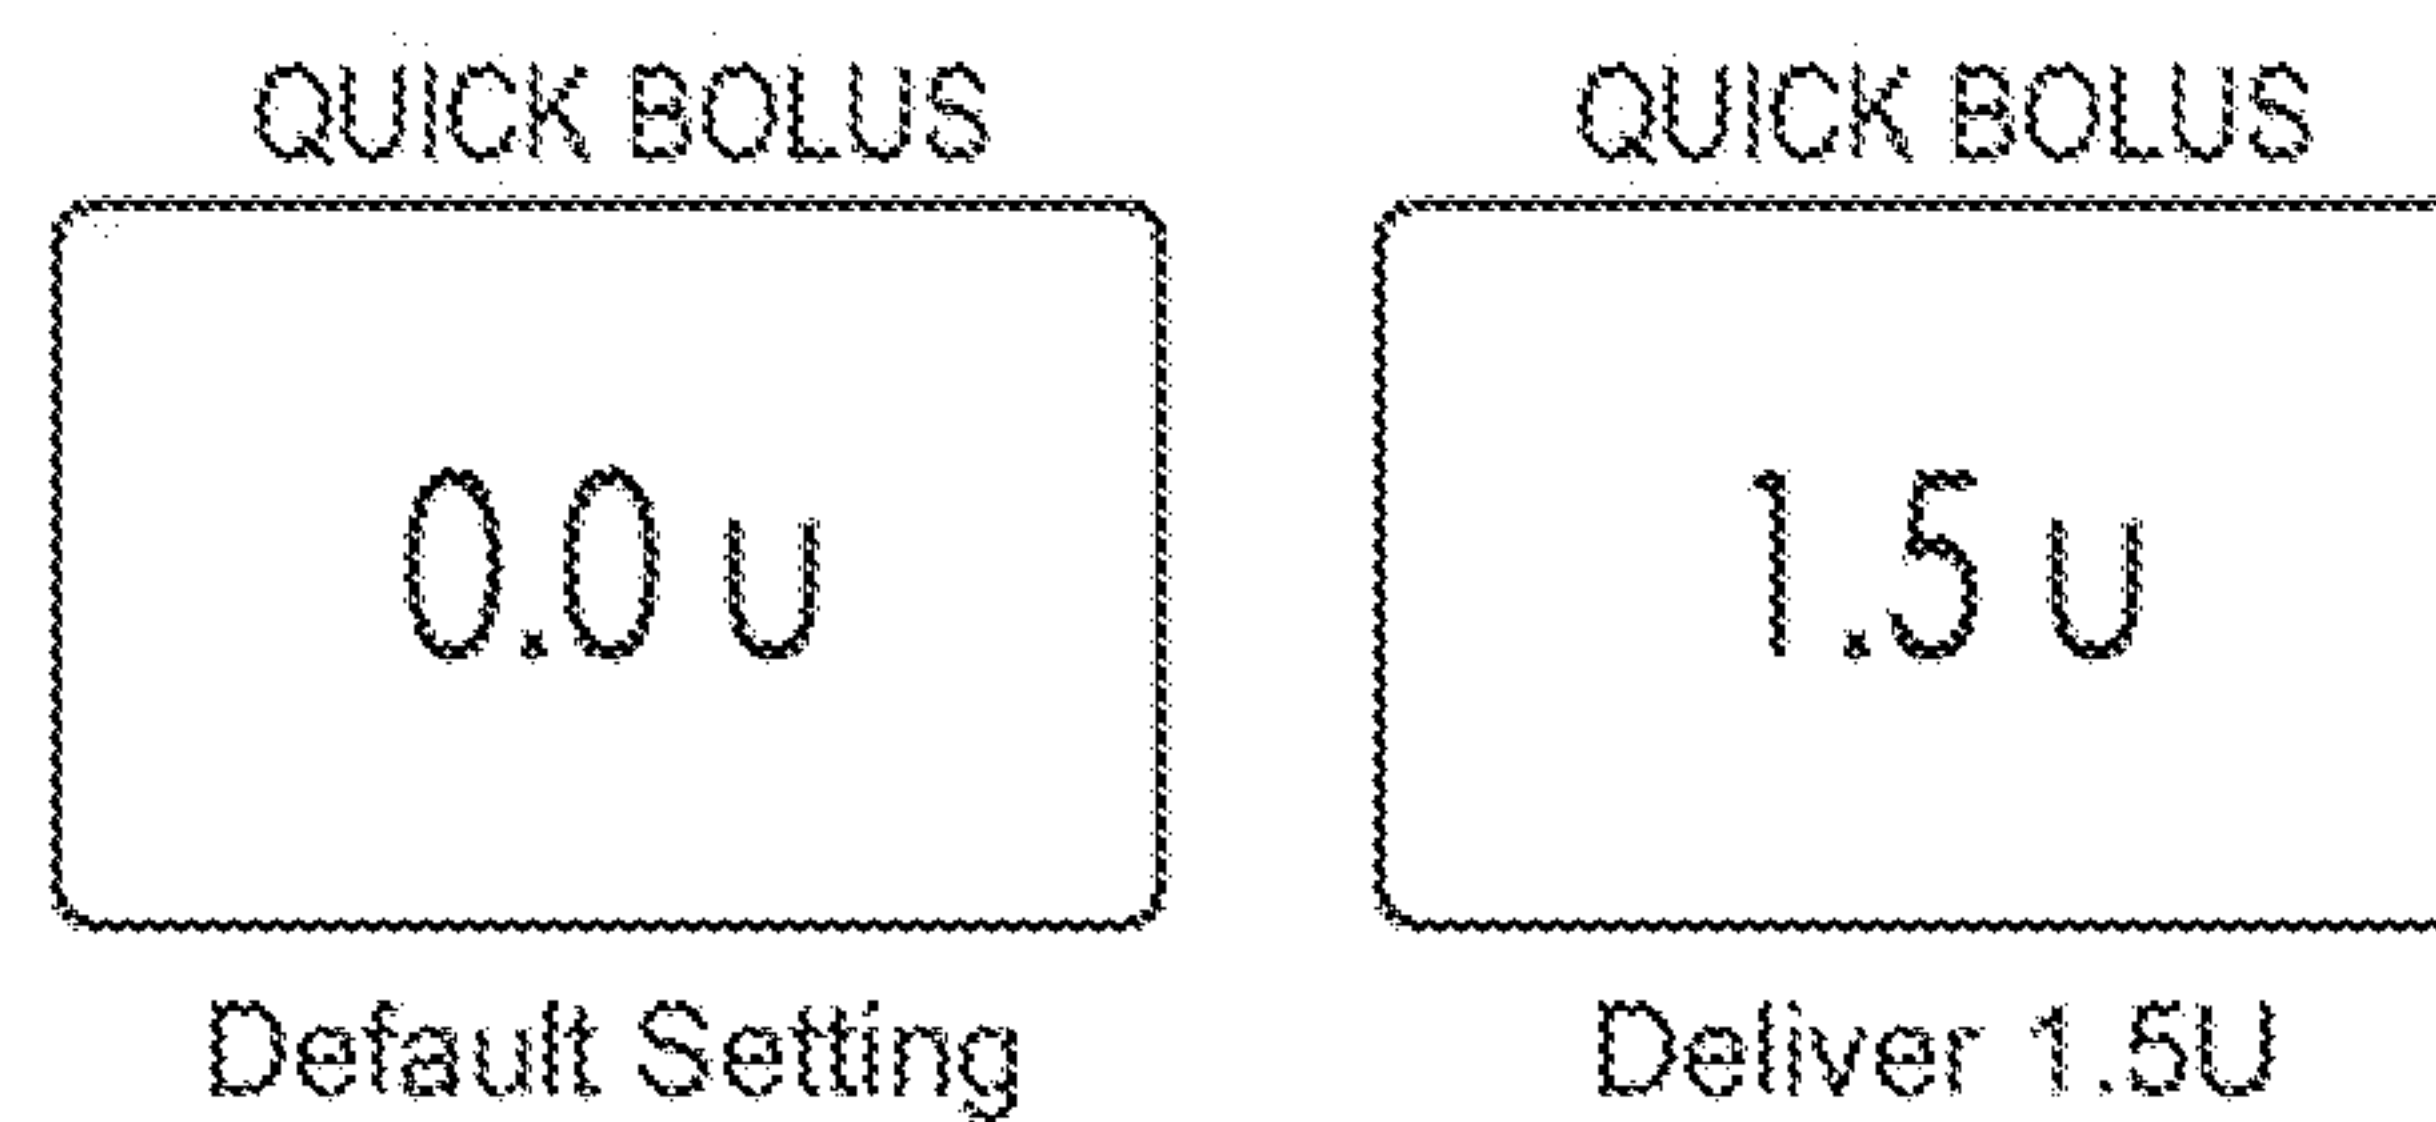


FIG. 23B

31/42

WARNING

IOB may not
include all
boluses.

OK

No Bolus History/More
than 10 Boluses within
the Defined Action
Time

FIG. 24A

CONFIRM Zero bolus calculated. Cancel bolus? Yes No Default Selection	CONFIRM Zero bolus calculated. Cancel bolus? Yes No Cancel the Bolus
--	---

FIG. 24B

CONFIRM Last bolus time unknown. Continue? Yes No Default Selection	CONFIRM Last bolus time unknown. Continue? Yes No Proceed with the Bolus
--	---

FIG. 24C

CONFIRM 10.00U Max exceeded. Cancel bolus? Yes No Default Selection	CONFIRM 10.00U Max exceeded. Cancel bolus? Yes No Confirm Cancel
--	---

FIG. 24D

32/42

HISTORY	HISTORY 1 of 3	HISTORY 2 of 3	HISTORY 3 of 3
None	Normal Bolus 0.09 of 0.9U 1h 30m ago	Normal Bolus 0.5 of 0.5U 1h 32m ago	Normal Bolus 0.27 of 0.3U 28h 25m ago
Next Done	Next Done	Next Done	Next Done

Display "None" when no bolus history; Only three boluses in history (1 of 3, 2 of 3, 3 of 3)
History includes up to 10 boluses; user interface displays records for most recently completed 10.

FIG. 25

33/42

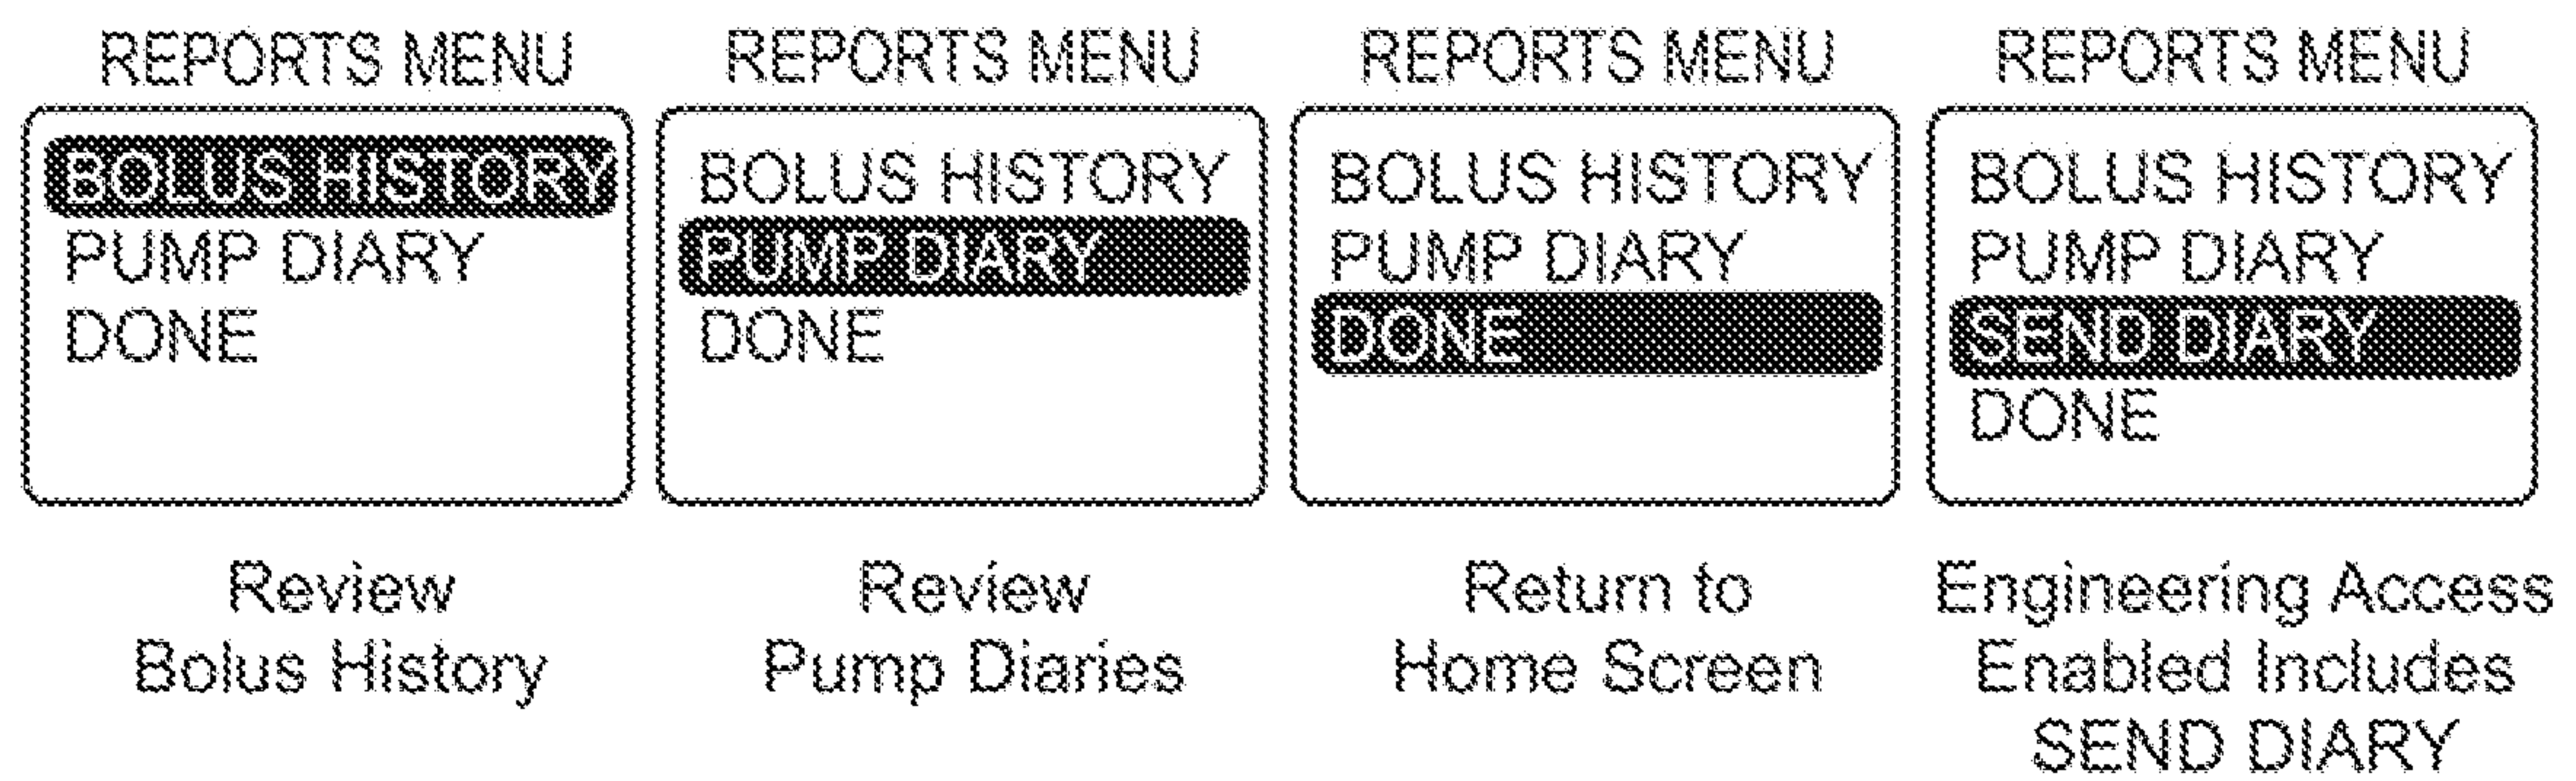


FIG. 26

34/42

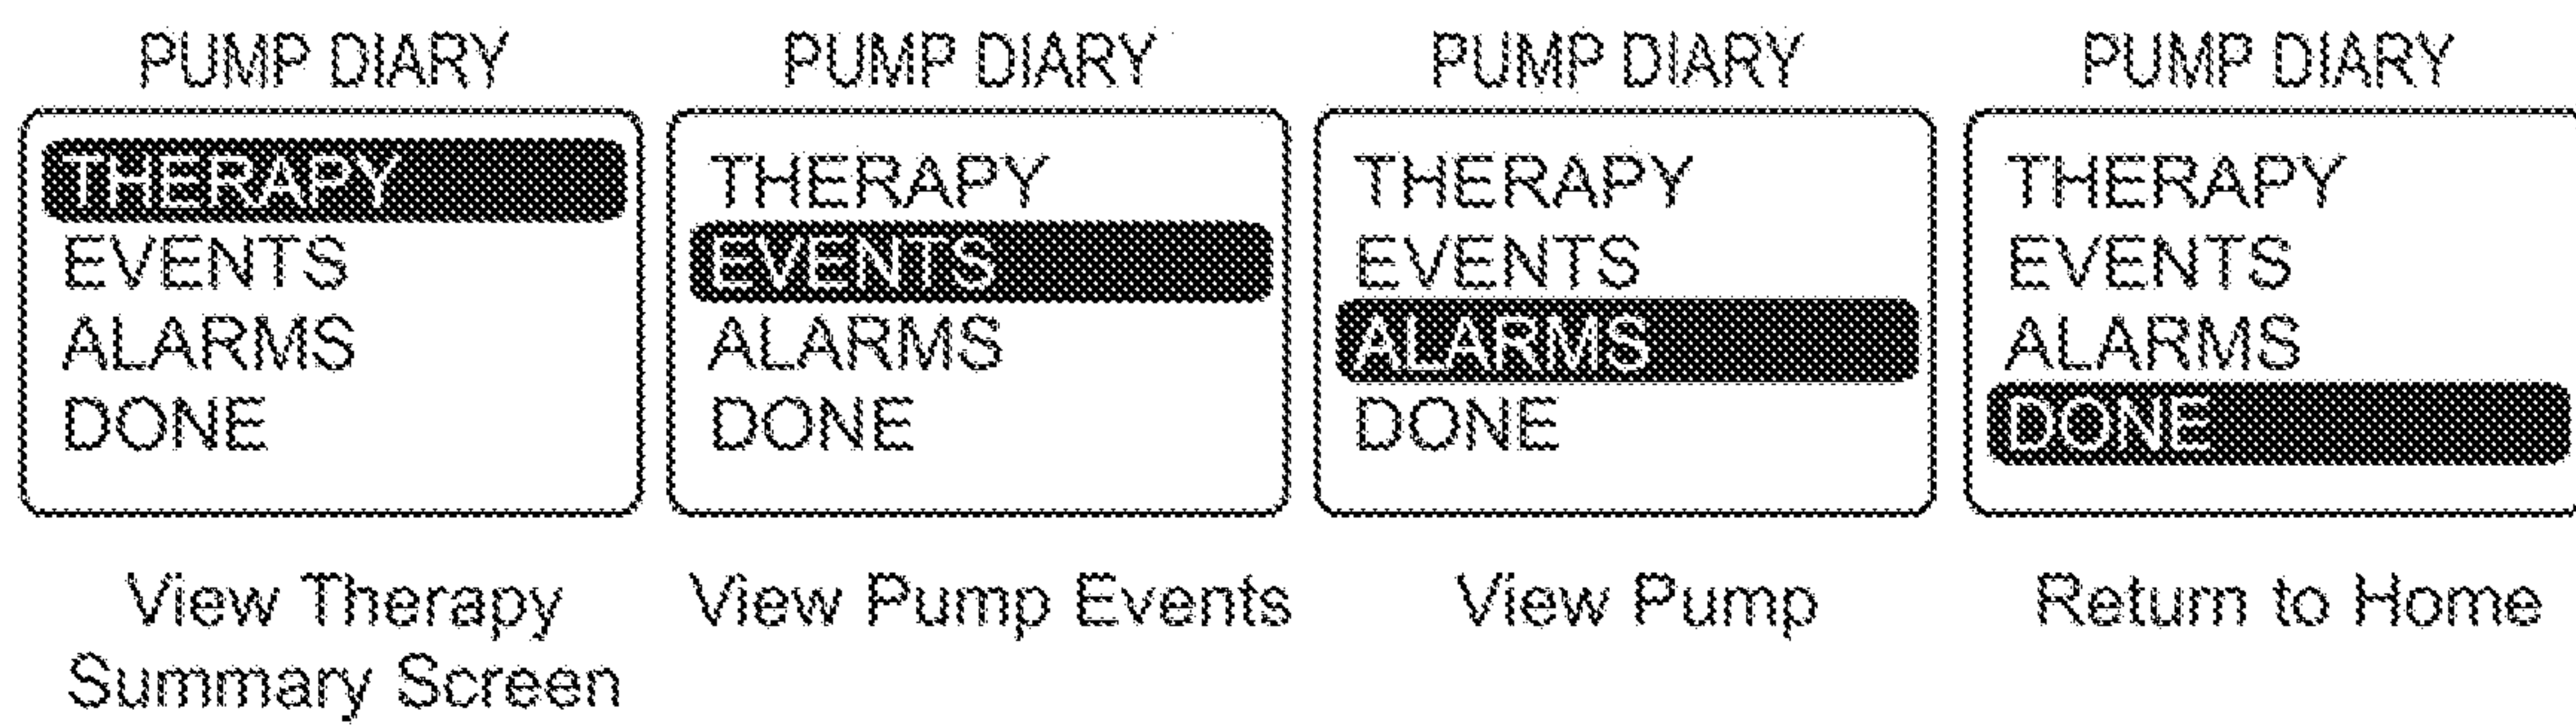


FIG. 27

35/42

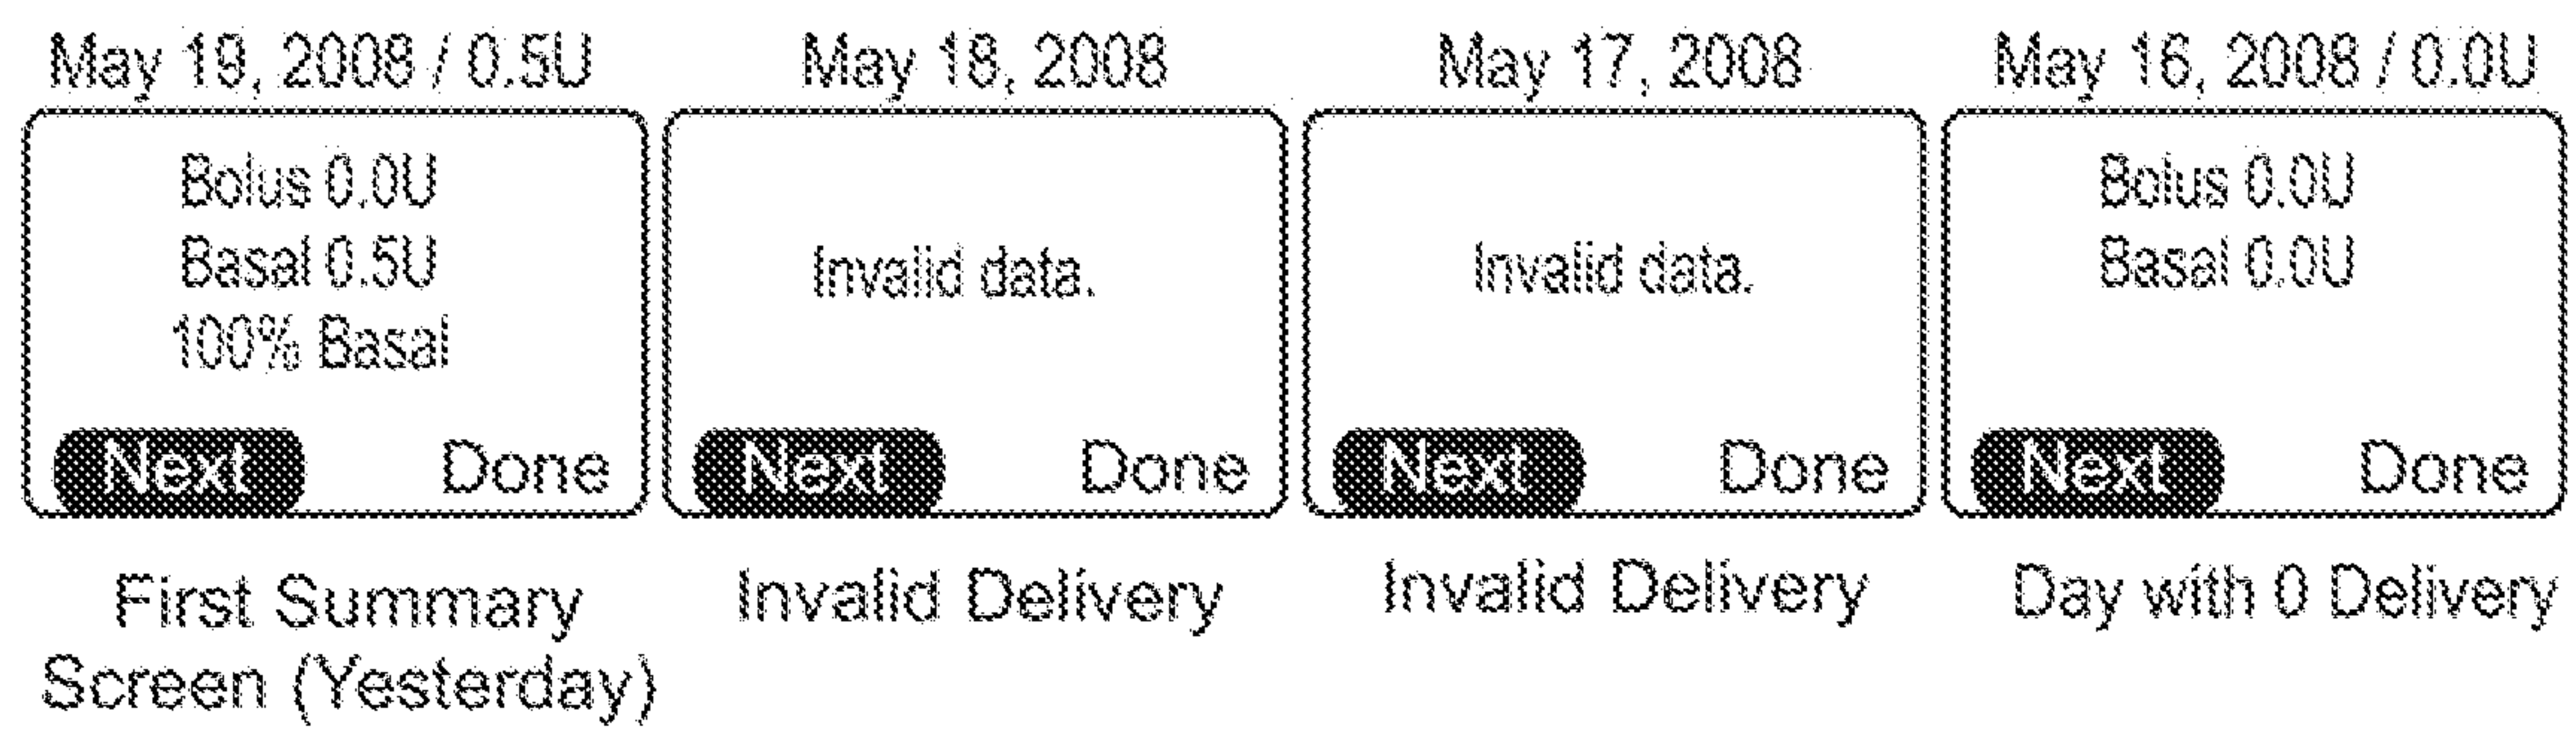


FIG. 28

36/42

Jun 01, 2008 9:55 AM	Jun 01, 2008 9:55 AM	Jun 01, 2008 9:55 AM	Jun 01, 2008 9:55 AM
Basal Selected Exercise Next Done	Basal Rate 0.10 U/h Next Done	Start Basal Daily Next Done	Basal Rate 0.70 U/h Next Done
Jun 01, 2008 9:55 AM	Jun 01, 2008 9:55 AM	Jun 01, 2008 9:29 AM	Jun 01, 2008 9:13 AM
Prime Done 1.60 U Next Done	Start Prime 1.60 U Next Done	Temp Done 0.60 U/h Next Done	Stop Ext. 0.15 U over 0h 17m Next Done
Jun 01, 2008 9:00 AM	Jun 01, 2008 8:55 AM	Jun 01, 2008 8:59 AM	Jun 01, 2008 8:59 AM
Snack Reminder Next Done	Start Temp 0.60 U/h for 0h 30m Next Done	Basal Rate 0.60 U/h Next Done	Basal Rate 0.70 U/h Next Done
Jun 01, 2008 8:59 AM	Jun 01, 2008 8:59 AM	Jun 01, 2008 8:58 AM	Jun 01, 2008 8:58 AM
Stop Temp 0h 3m Next Done	Bolus Done 6.25 U Next Done	Start Bolus 2.35 U 2.00, 0.37, 0.01 Next Done	Glucose 200 mg/dL Next Done
Jun 01, 2008 8:57 AM	Jun 01, 2008 8:57 AM	Jun 01, 2008 8:57 AM	Jun 01, 2008 8:55 AM
STOPPED ALERT Next Done	Stop Bolus 1.20 U Next Done	Start Bolus 3.60 U 3.61, 0.0, 0.0 Next Done	Start Temp 50% for 0h 30m Next Done
Jun 01, 2008 8:55 AM	Jun 01, 2008 8:55 AM	Jun 01, 2008 8:55 AM	Jun 01, 2008 8:55 AM
Basal Rate 0.35 U/h Next Done	Start Ext. 1.40 U over 2h 30m Next Done	Start Basal Daily Next Done	Basal Rate 0.70 U/h Next Done
Jun 01, 2008 8:54 AM	Jun 01, 2008 8:54 AM	Jun 01, 2008 8:54 AM	Jun 01, 2008 8:54 AM
Stop Prime 0.90 U Next Done	Start Prime 1.90 U Next Done	Basal Selected Daily Next Done	Basal Rate 0.00 U/h Next Done

FIG. 29A

37/42

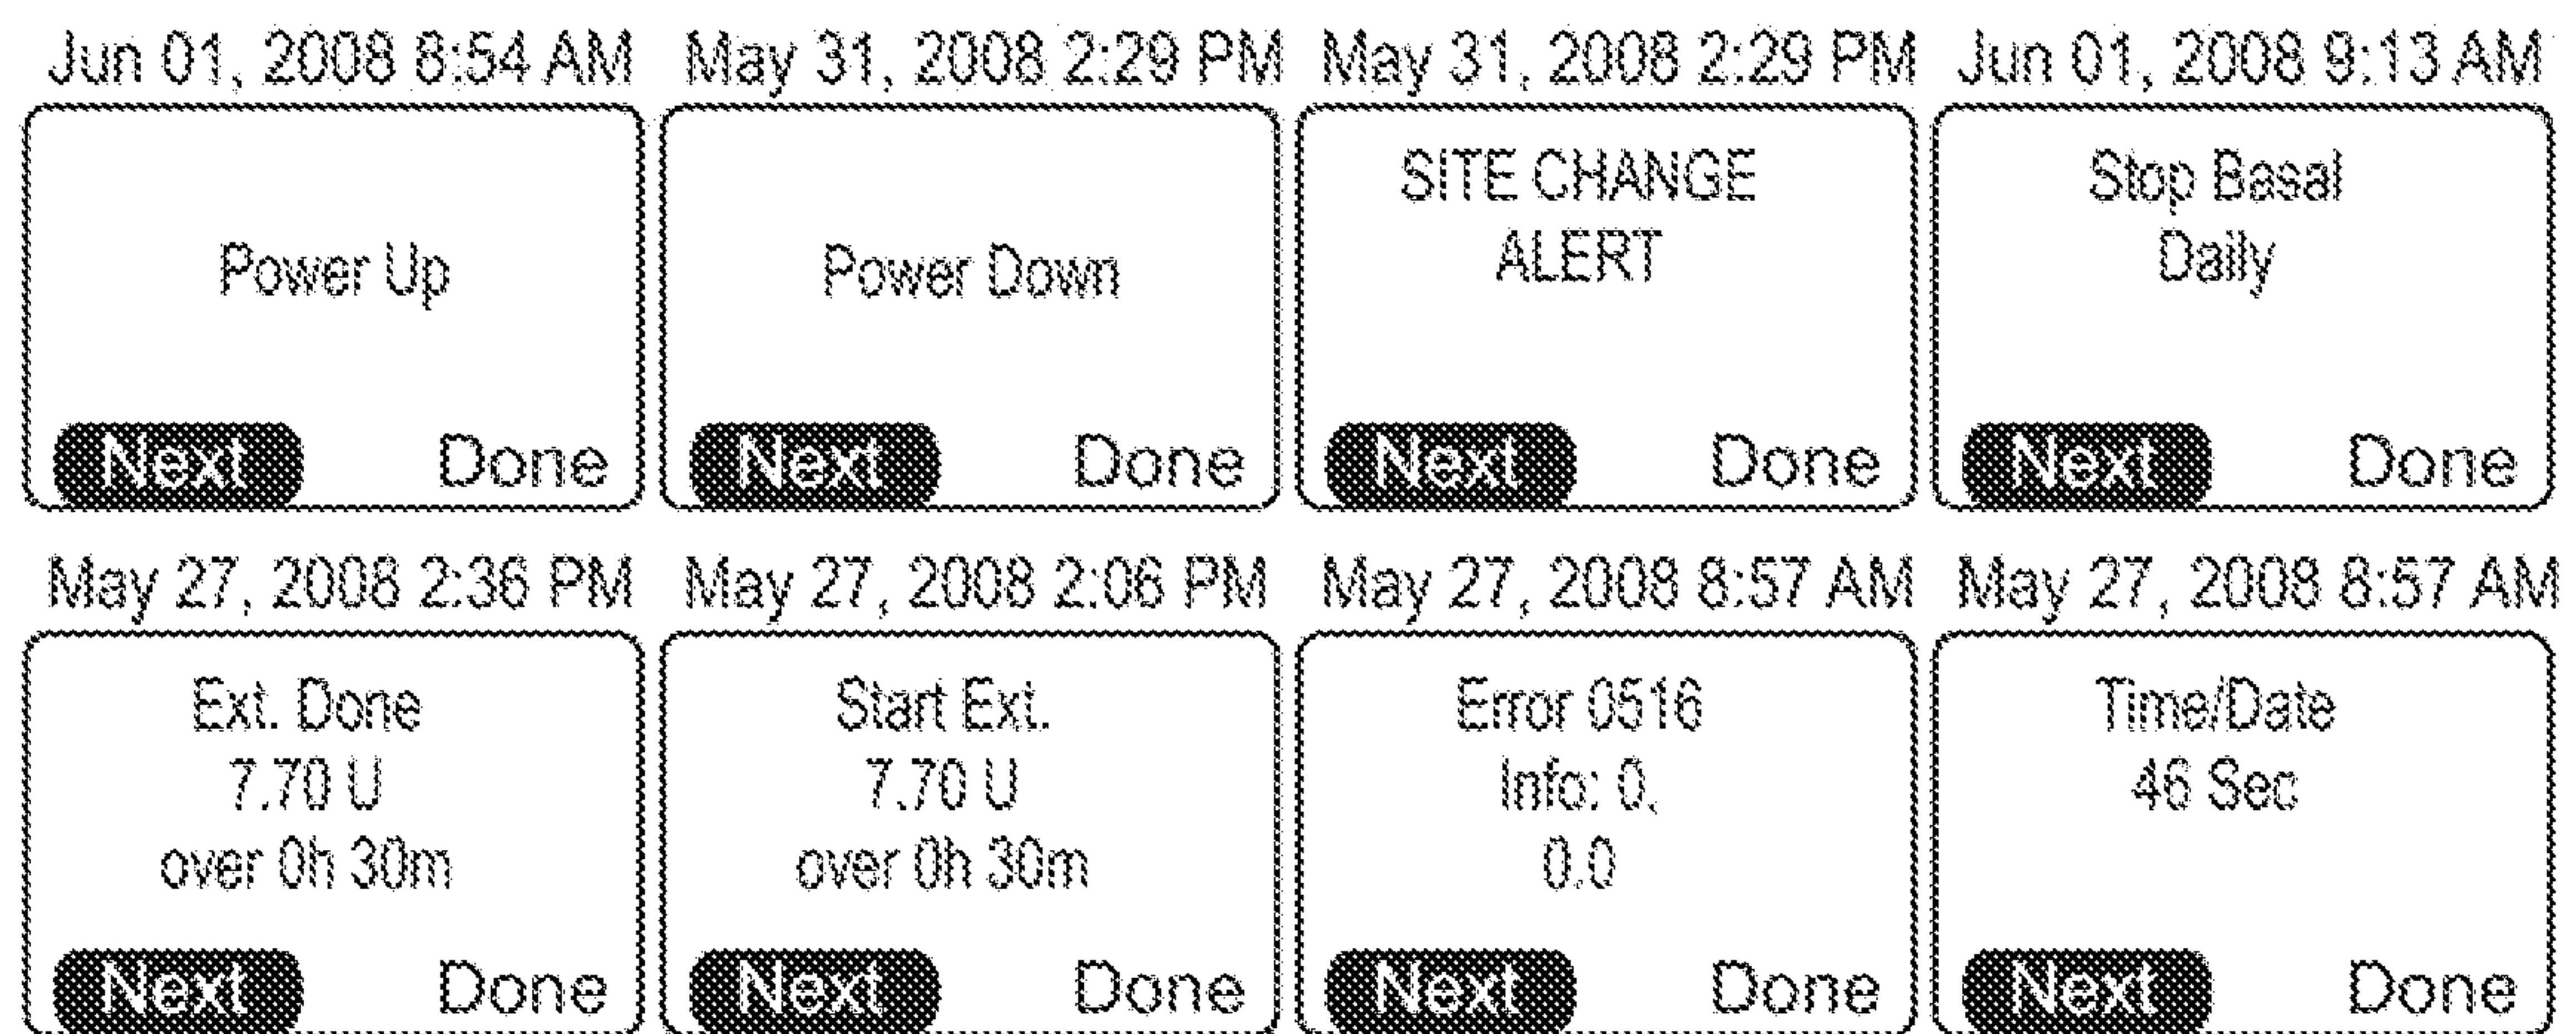


FIG. 29B

38/42

Jun 01, 2008 8:57 AM	May 27, 2008 8:57 AM	May 19, 2008 3:09 PM	May 19, 2008 2:54 PM
STOPPED ALERT	Error 0516 Info: 0, 0.0	INACTIVITY ALARM	INACTIVITY ALERT
Next Done	Next Done	Next Done	Next Done
May 9, 2008 7:09 PM	May 9, 2008 7:09 PM	May 9, 2008 7:09 PM	May 9, 2008 7:09 PM
BAD BATTERY ALARM	NO INSULIN ALARM	RESERVOIR ALARM	OCCLUSION ALARM
Next Done	Next Done	Next Done	Next Done
May 31, 2008 7:20 PM	May 31, 2008 2:29 PM	May 31, 2008 7:20 PM	May 31, 2008 7:20 PM
CHECK BG ALERT	SITE CHANGE ALERT	LOW TEMP ALERT	HIGH TEMP ALERT
Next Done	Next Done	Next Done	Next Done
Jun 01, 2008 9:00 AM	Jun 01, 2008 9:00 AM	Jun 01, 2008 9:00 AM	Jun 01, 2008 9:00 AM
Snack Reminder	Pickup Reminder	Bolus Reminder	Check BG Reminder
Next Done	Next Done	Next Done	Next Done
May 9, 2008 7:09 PM	May 9, 2008 7:09 PM	May 9, 2008 7:09 PM	DIARY
LOW INSULIN ALERT	LOW BATTERY ALERT	PUMP IDLE ALERT	None
Next Done	Next Done	Next Done	Next Done
0 Alarms Logged			

FIG. 30

39/42

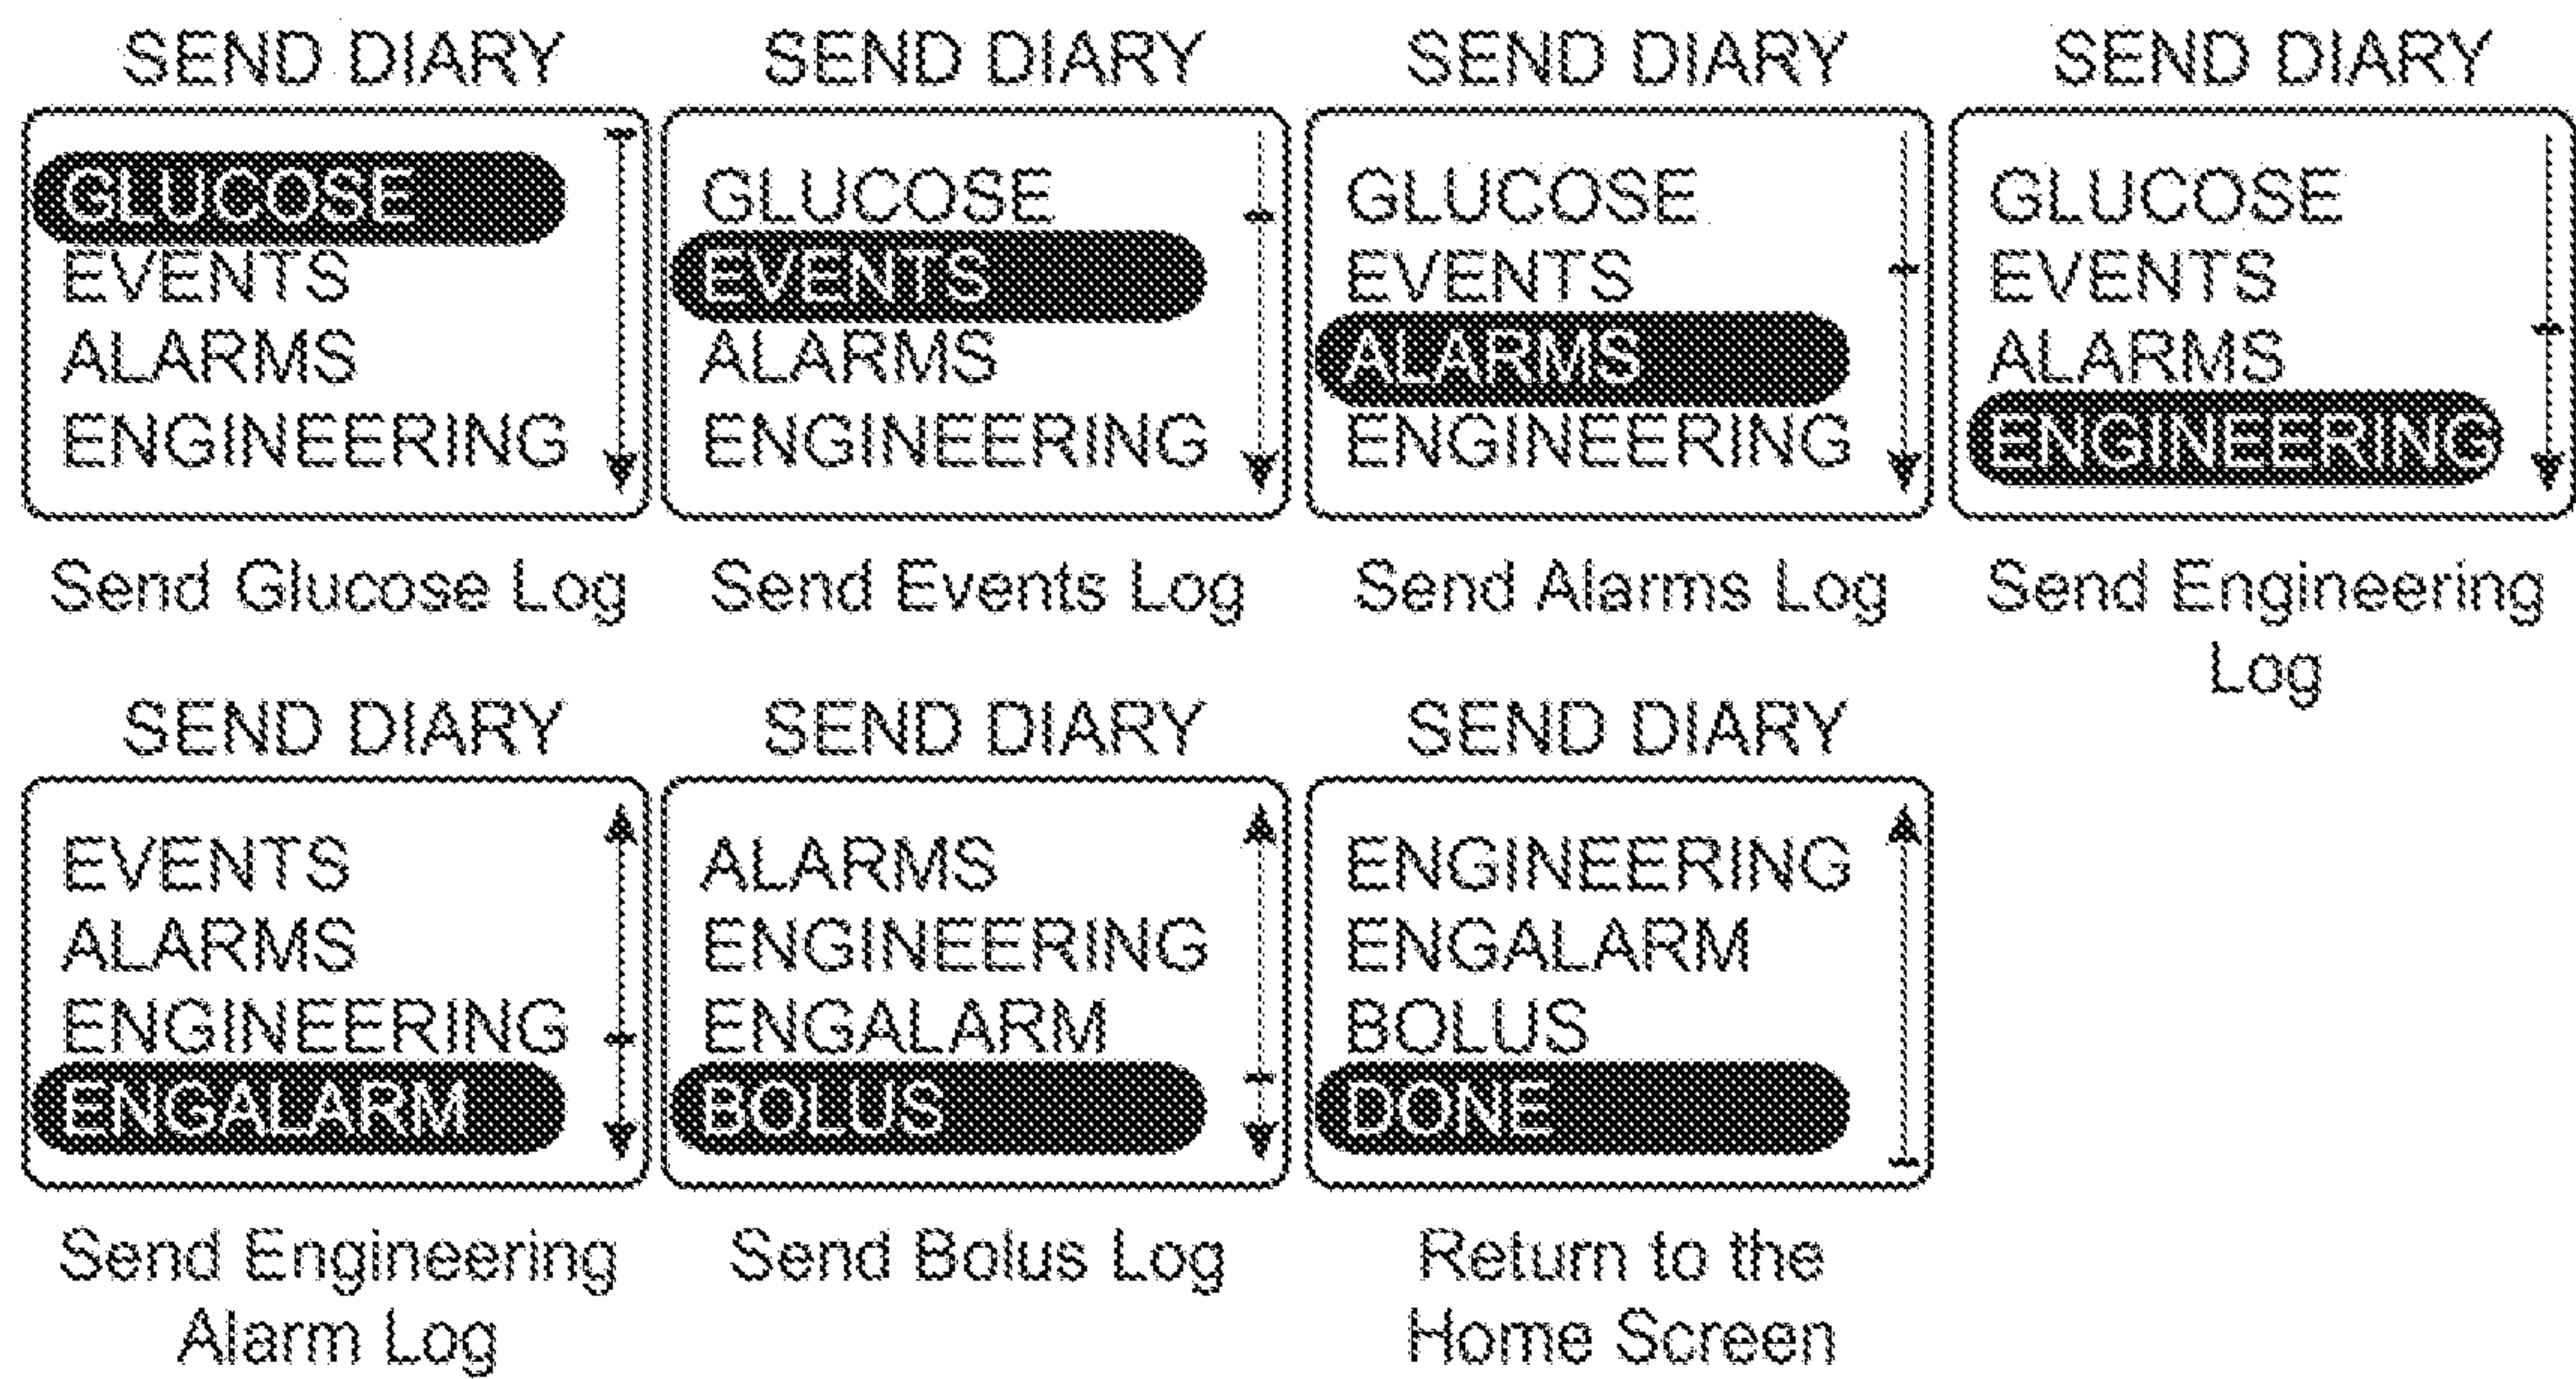


FIG. 31

40/42

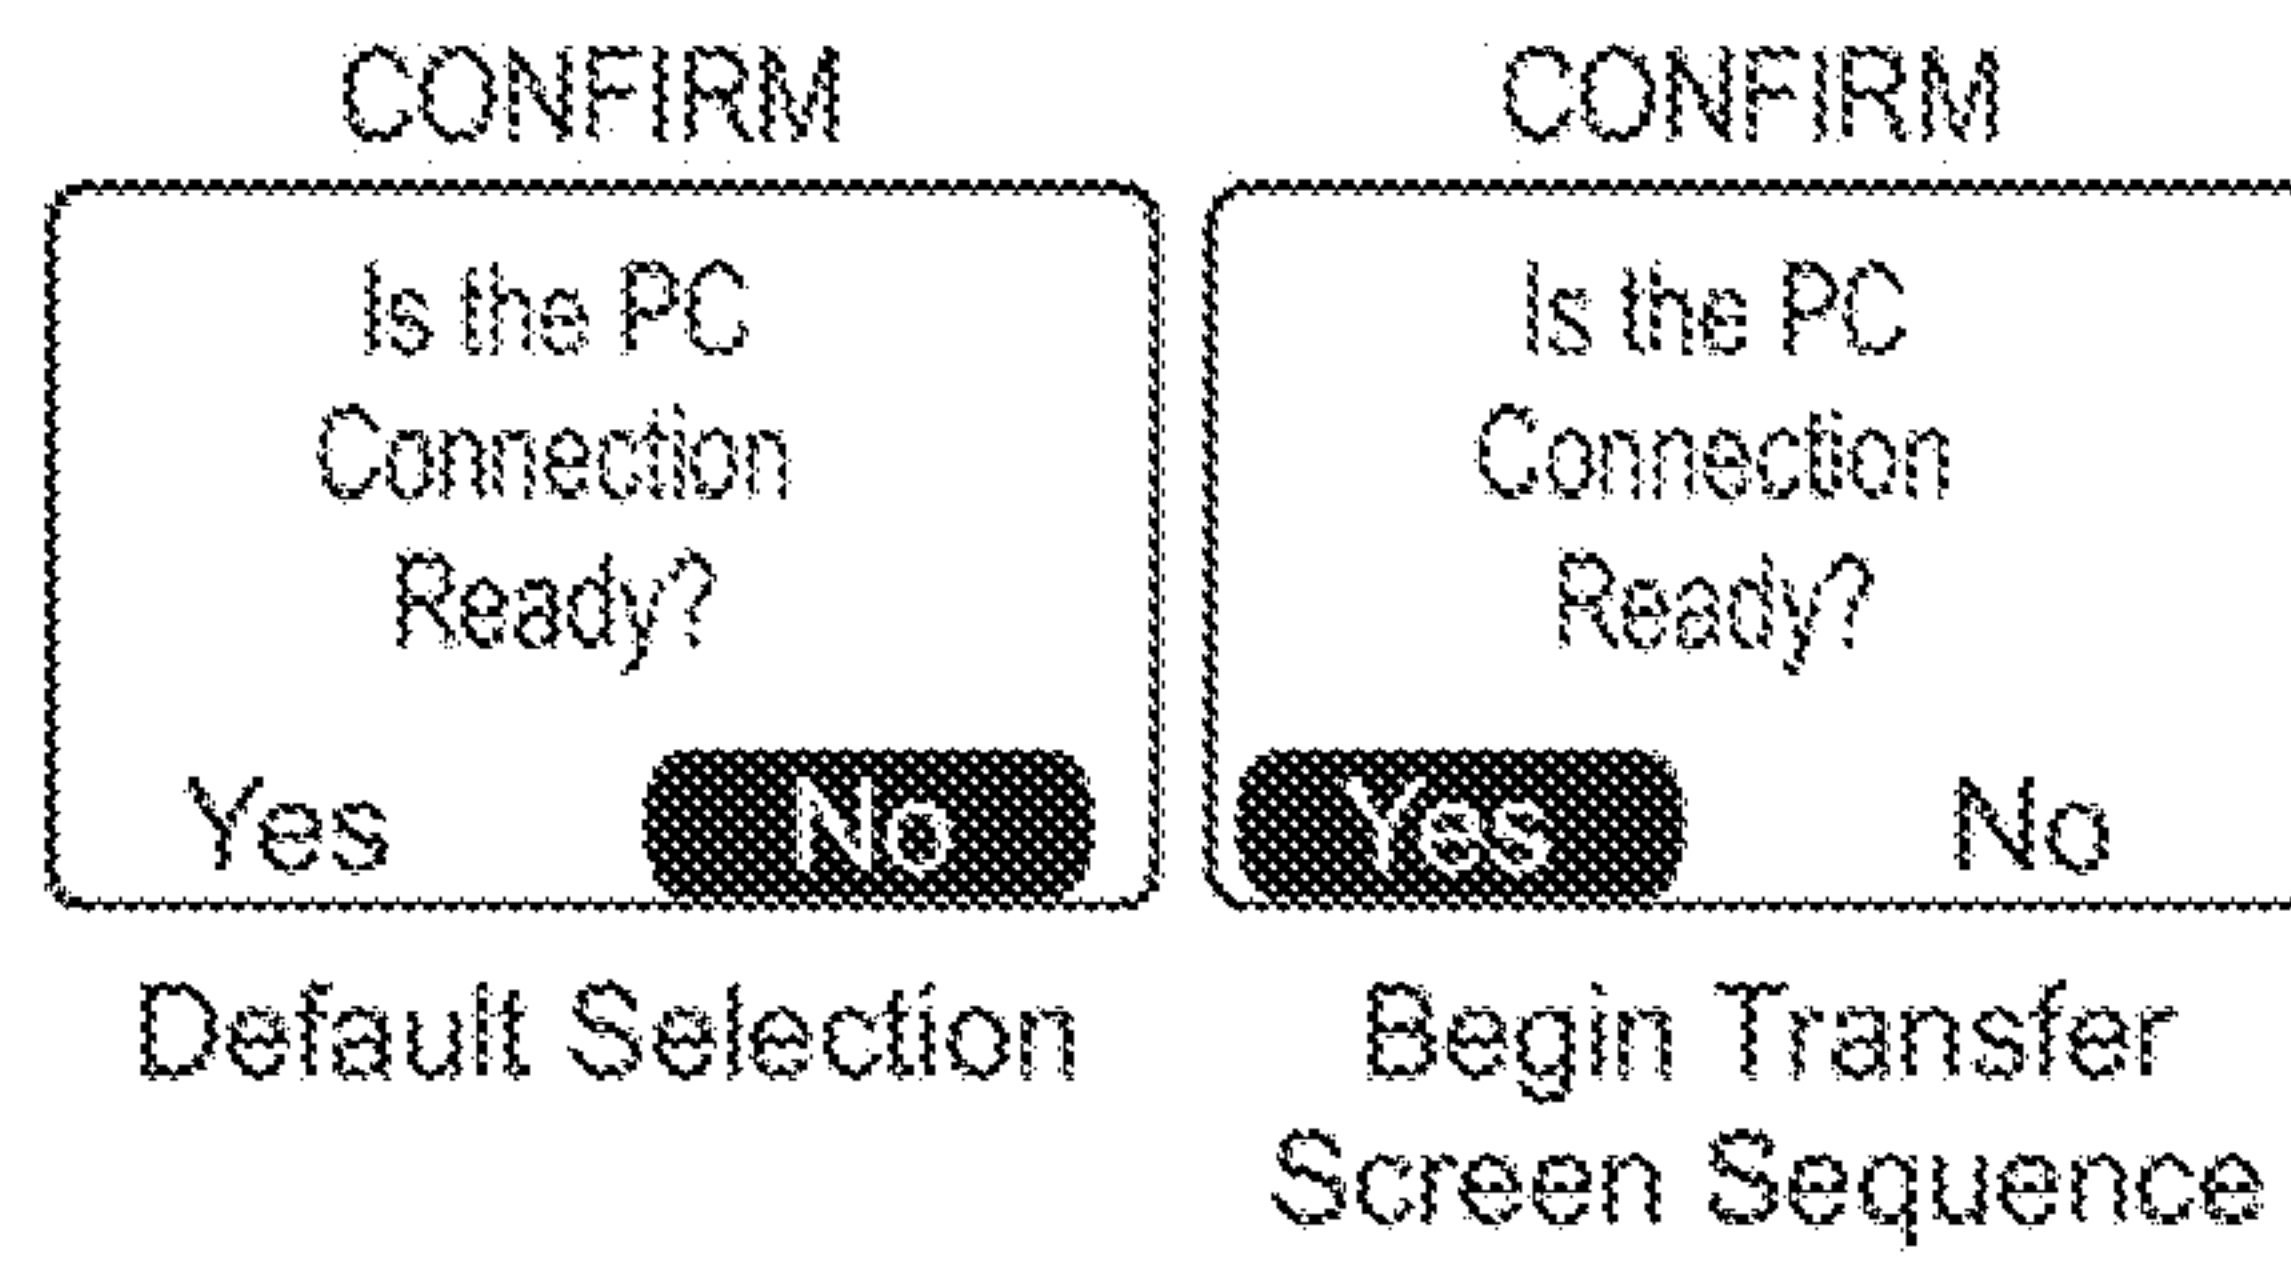


FIG. 32

41/42

CONFIRM	CONFIRM
Ascii format?	Ascii format?
☒ Yes ☐ No	☐ Yes ☒ No

FIG. 33

42/42

CONFIRM		CONFIRM	
Prepend config info?		Prepend config info?	
Yes	☒ No	☒ Yes	No

FIG. 34A

CONFIRM		CONFIRM	
Include record number?		Include record number?	
Yes	☒ No	☒ Yes	No

FIG. 34B

CONFIRM		CONFIRM	
Transfer Complete Erase Log?		Transfer Complete Erase Log?	
Yes	☒ No	☒ Yes	No

FIG. 34C

CONFIRM		CONFIRM	
Transfer Another Log?		Transfer Another Log?	
Yes	☒ No	☒ Yes	No

FIG. 34D

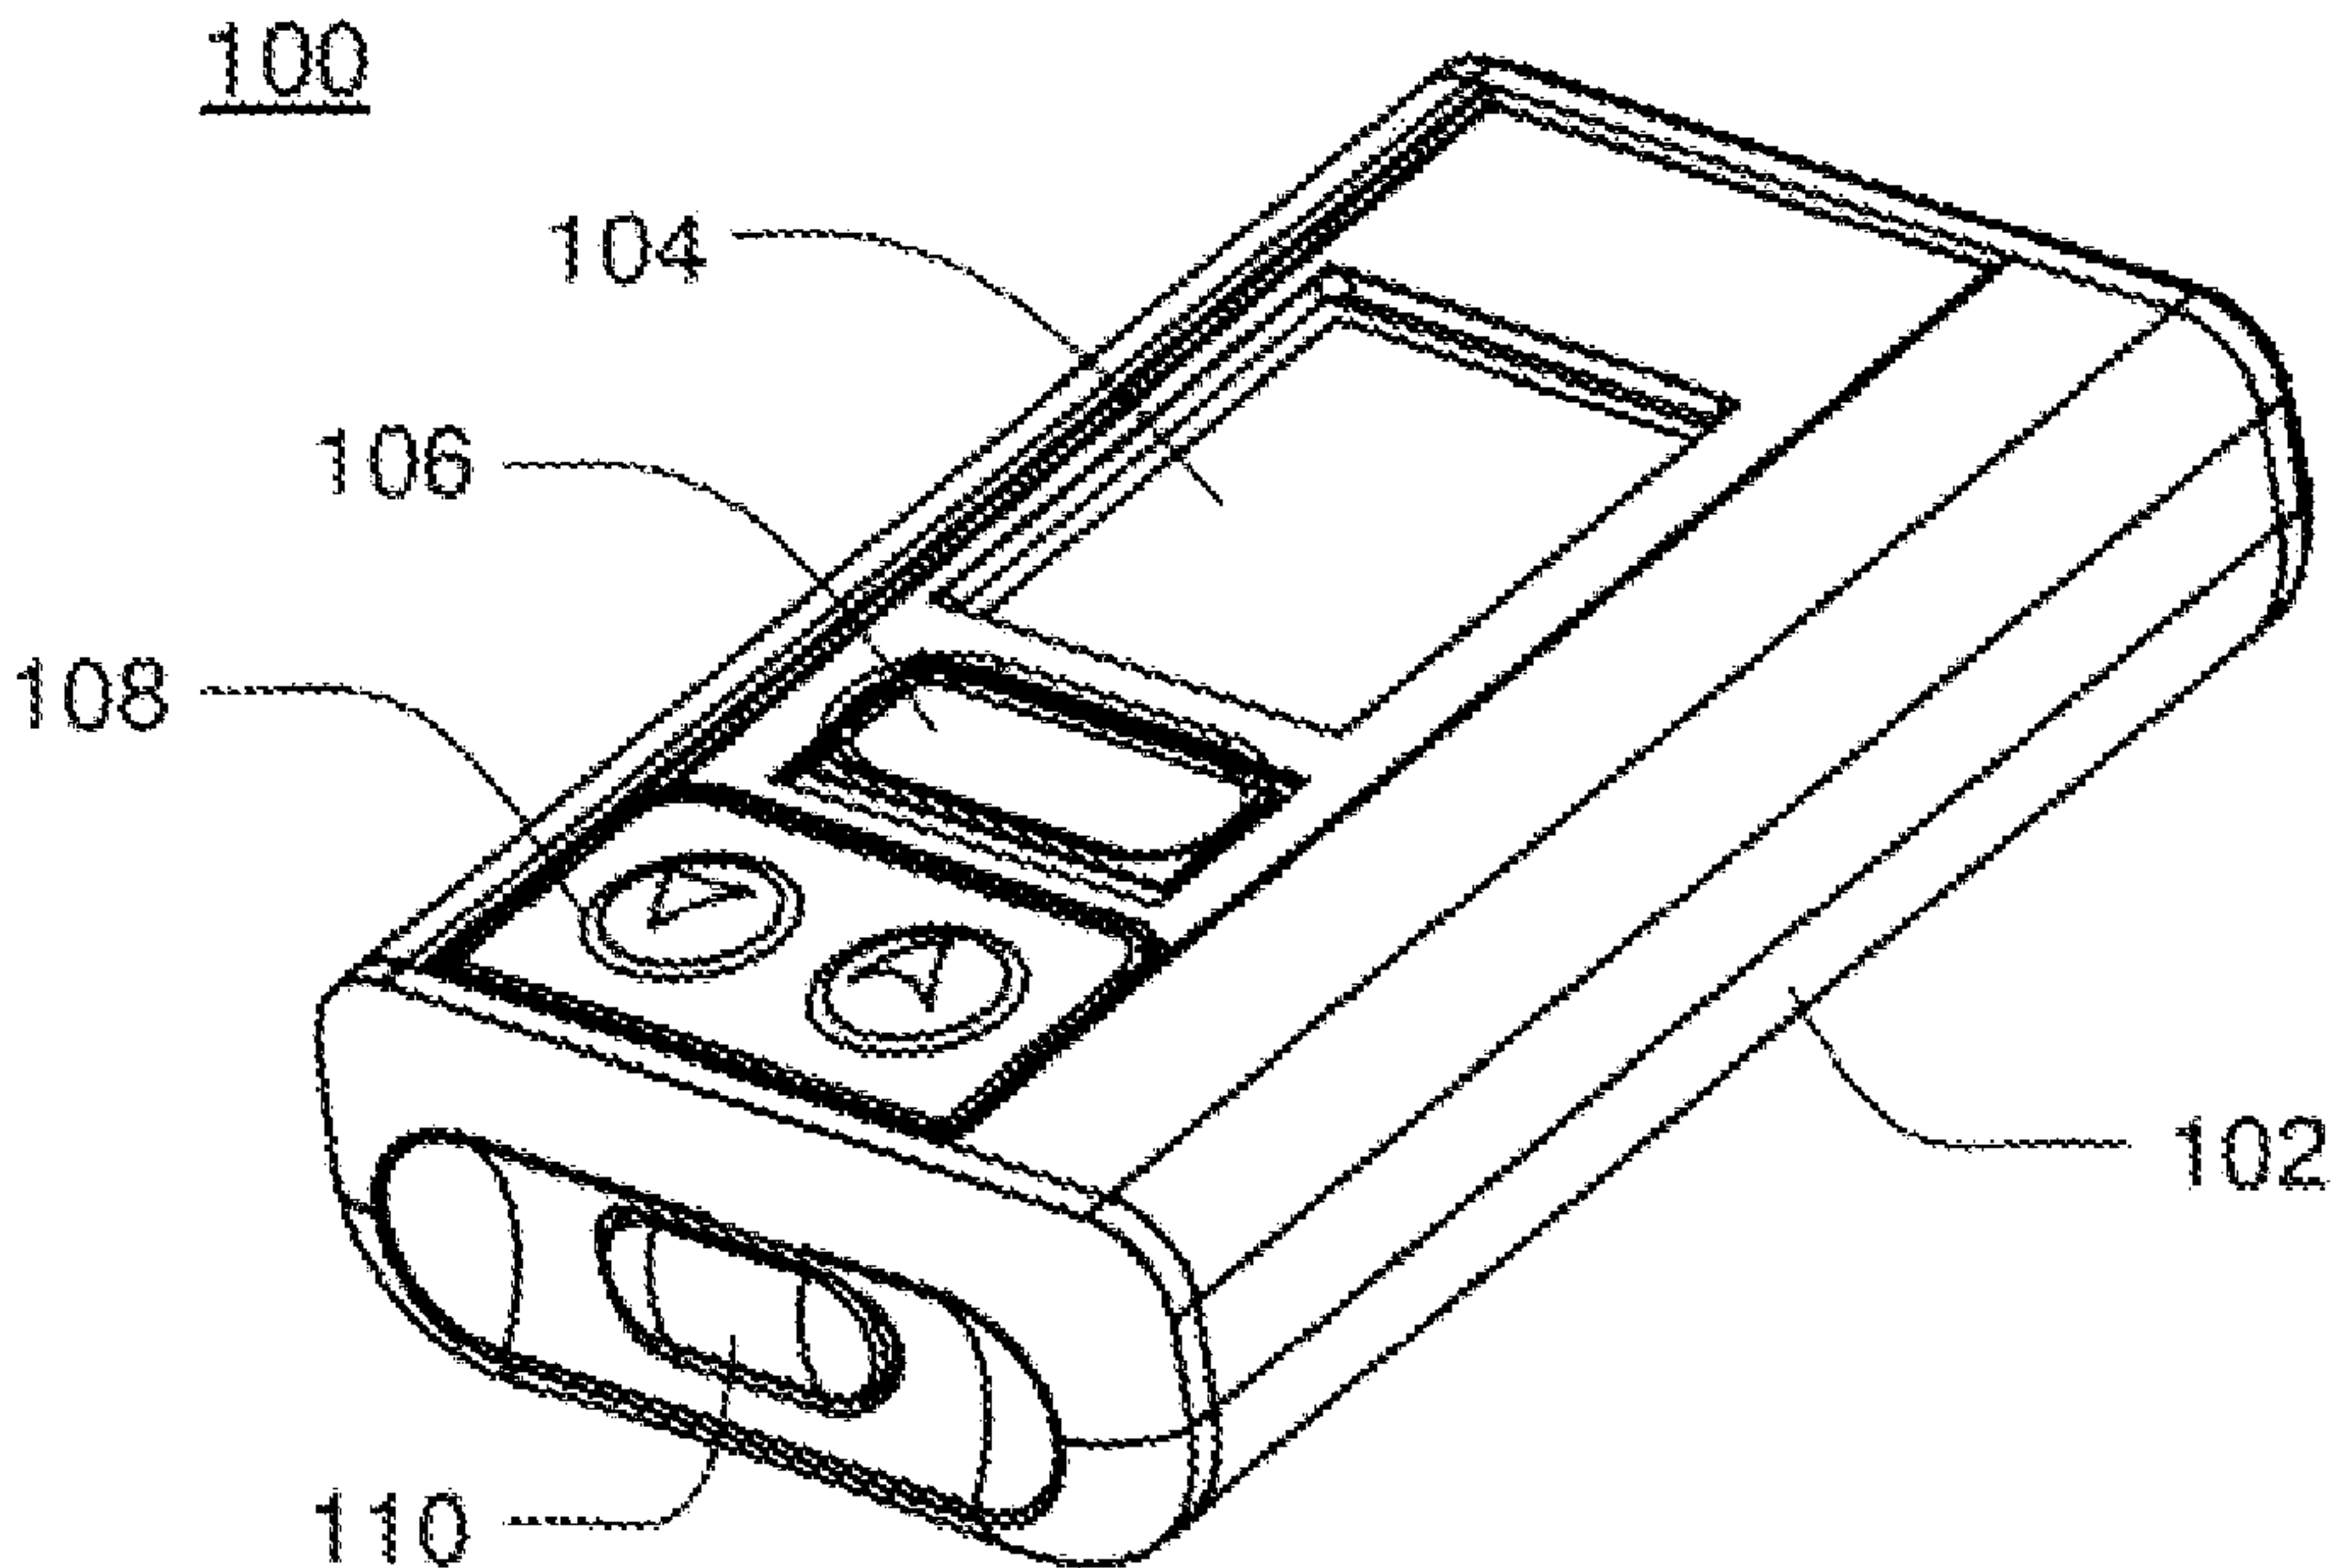


FIG. 1A