



(19) **United States**  
(12) **Patent Application Publication**  
**Trieu et al.**

(10) **Pub. No.: US 2011/0213418 A1**  
(43) **Pub. Date: Sep. 1, 2011**

(54) **MULTI-CHAMBER EXPANDABLE INTERSPINOUS PROCESS SPACER**

**Publication Classification**

(75) Inventors: **Hai H. Trieu**, Cordova, TN (US);  
**Kent M. Anderson**, San Jose, CA (US);  
**Eric C. Lange**, Pleasanton, CA (US)

(51) **Int. Cl.**  
**A61B 17/70** (2006.01)

(52) **U.S. Cl.** ..... **606/249**

(73) Assignee: **WARSAW ORTHOPEDIC, INC.**,  
Warsaw, IN (US)

(57) **ABSTRACT**


(21) Appl. No.: **13/105,792**

An expandable interspinous process spacer is disclosed that includes at least two chambers, one disposed within the other. Each of the at least two chambers can receive an injectable biocompatible material, which advantageously may have different material properties such as hardness. Further, the expandable interspinous process spacer can be changed from a deflated configuration to an inflated configuration. In the inflated configuration, the expandable interspinous process spacer can engage and support a superior spinous process and an inferior spinous process.

(22) Filed: **May 11, 2011**

**Related U.S. Application Data**

(60) Continuation of application No. 12/795,883, filed on Jun. 8, 2010, which is a division of application No. 11/413,587, filed on Apr. 28, 2006, now abandoned.

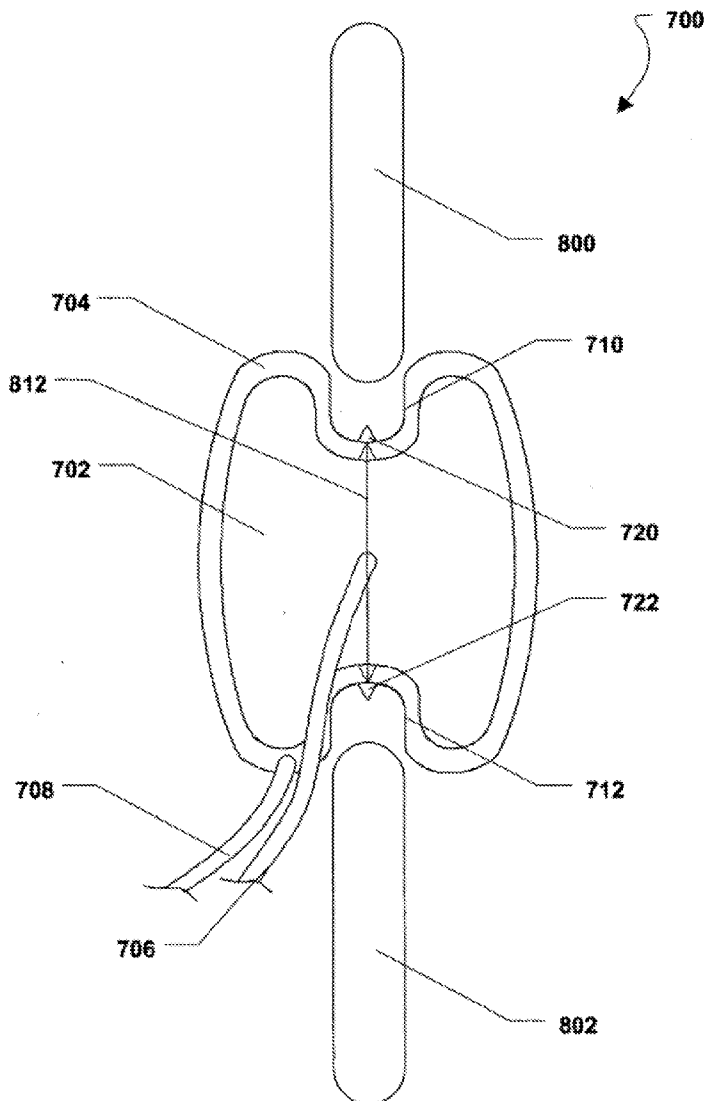


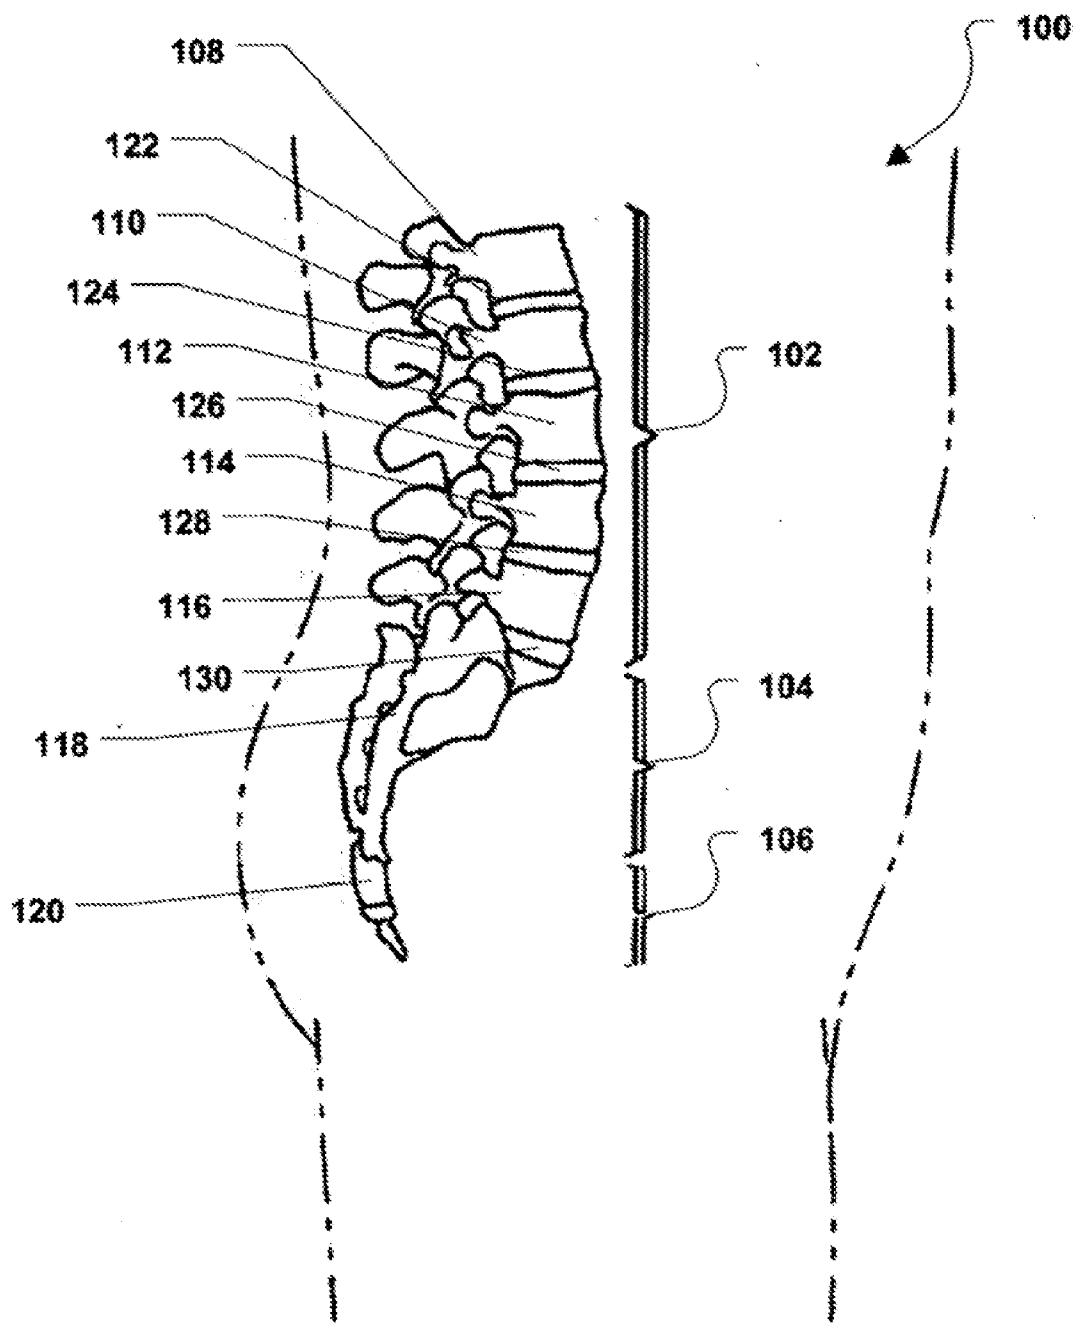


FIG. 1

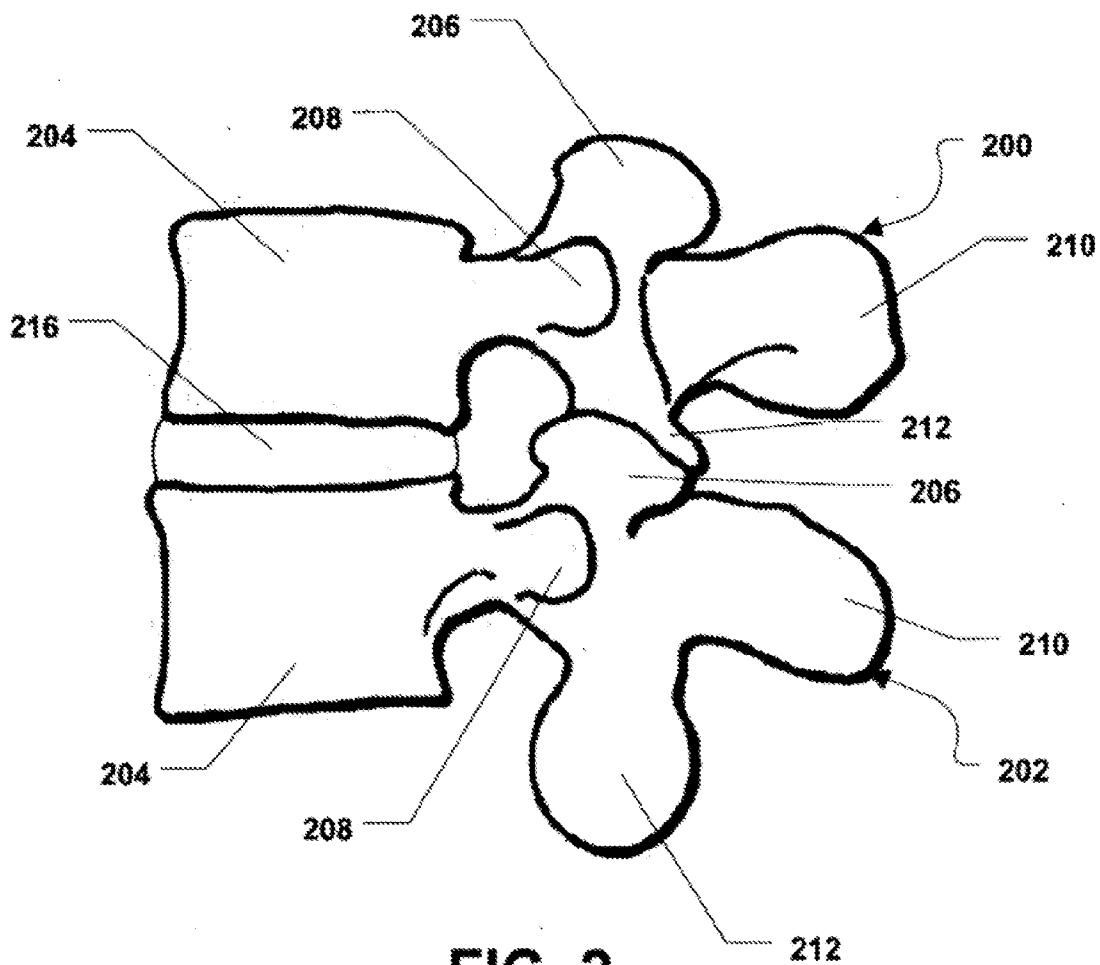

**FIG. 2**


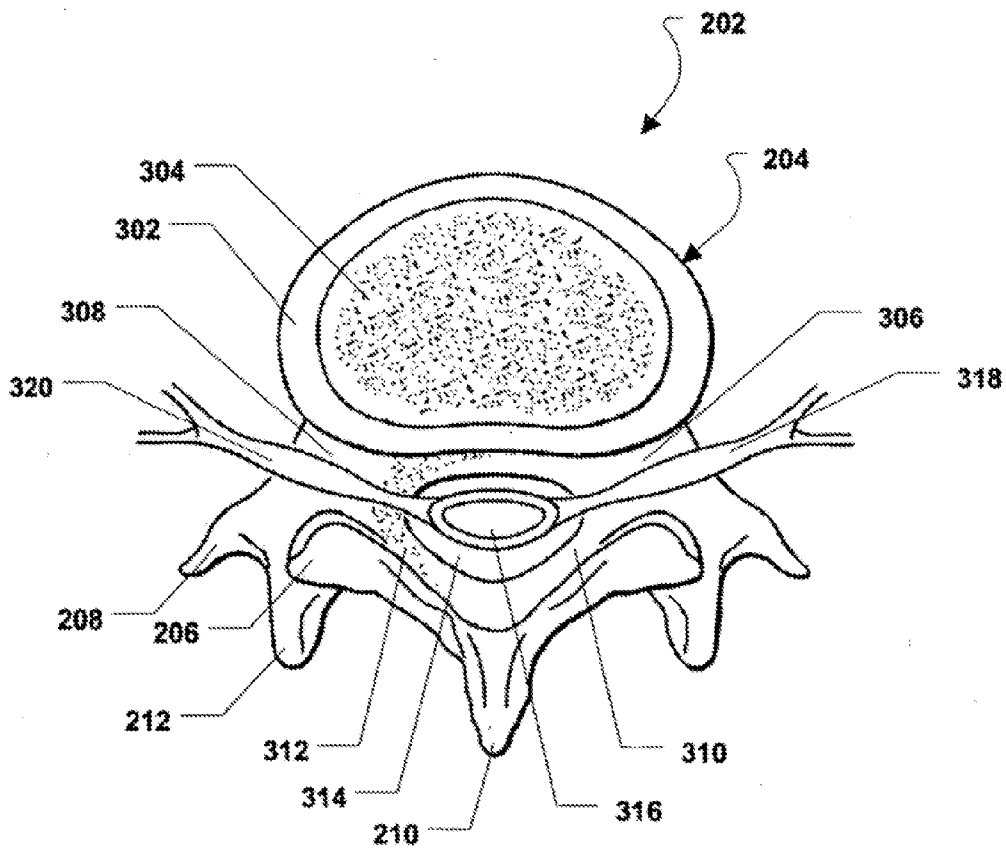


FIG. 3

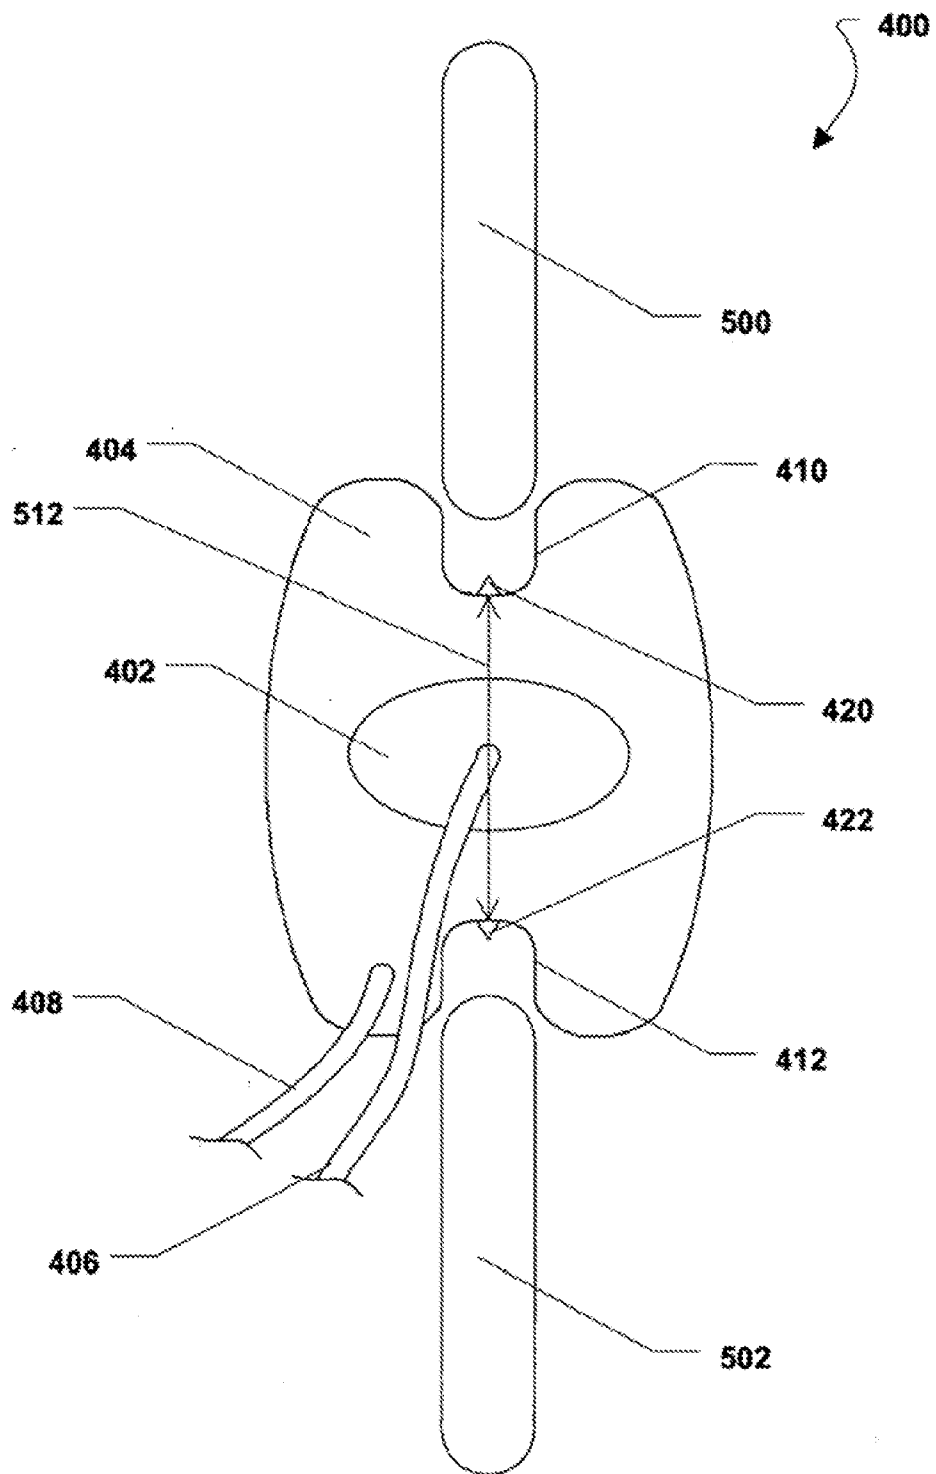

**FIG. 4**

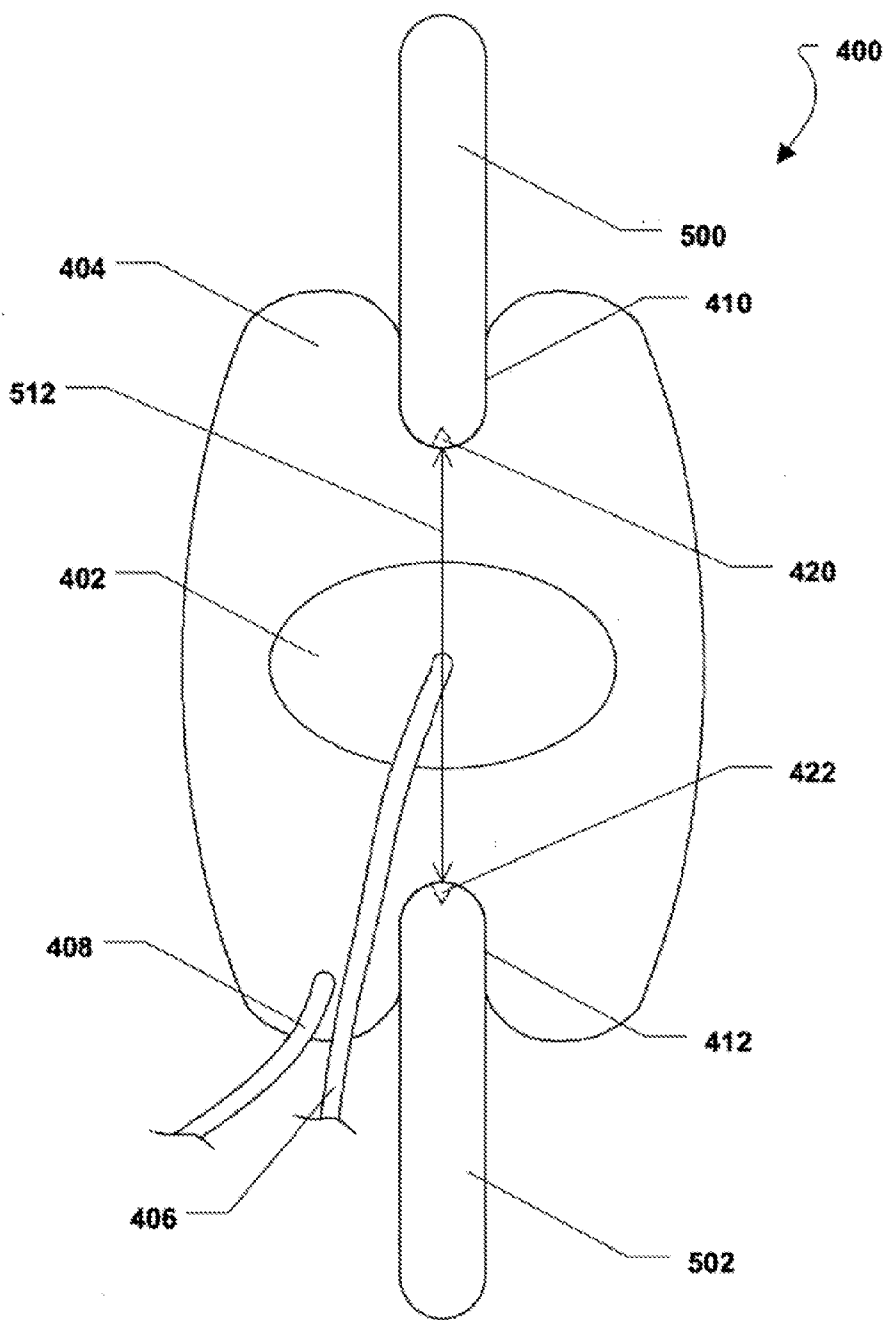


FIG. 5


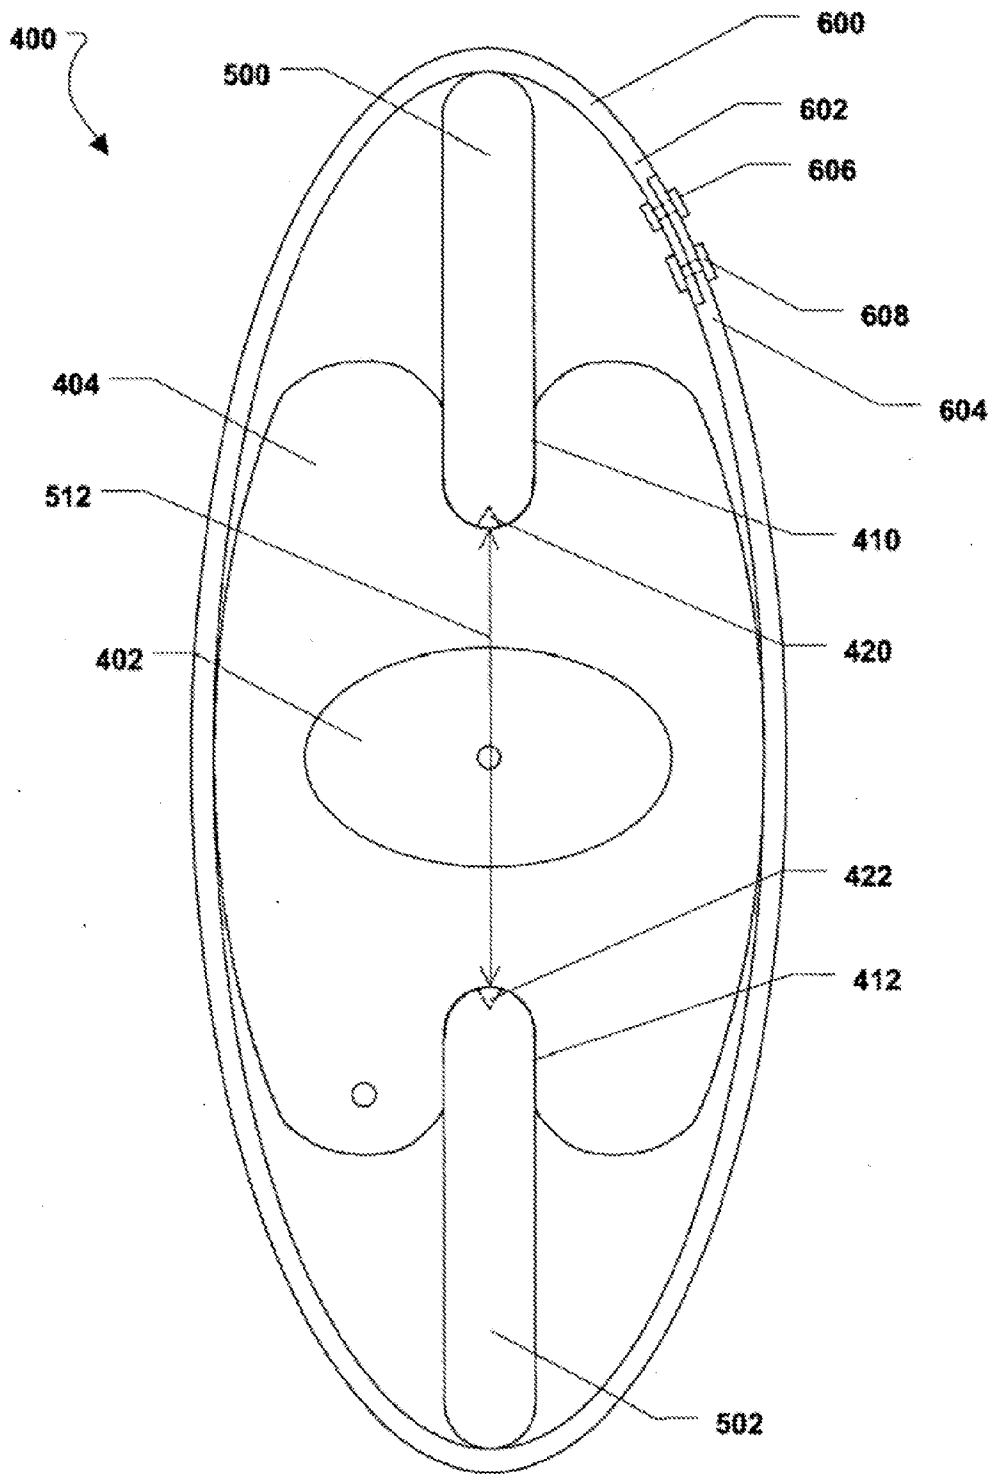


FIG. 6

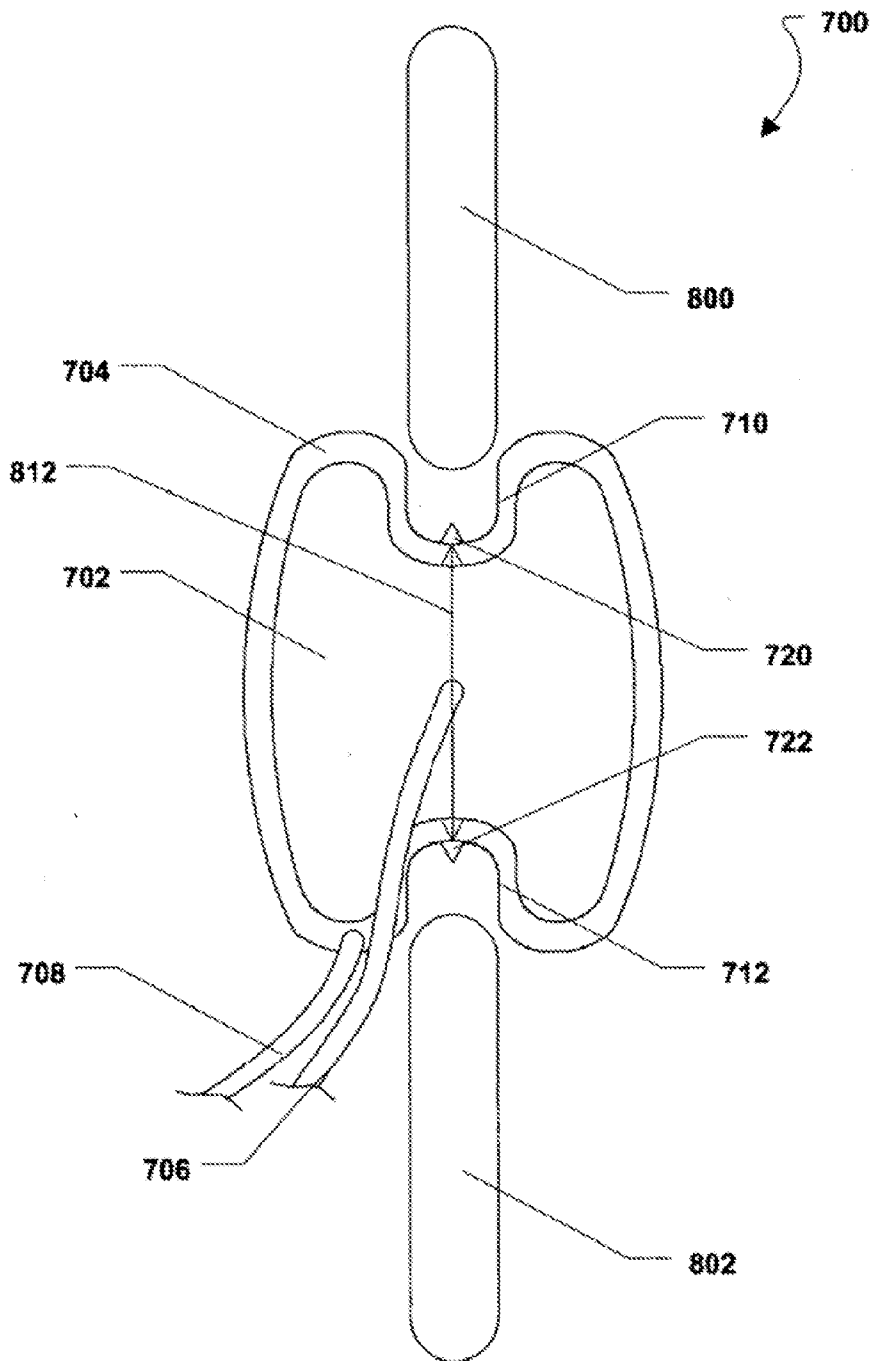

**FIG. 7**



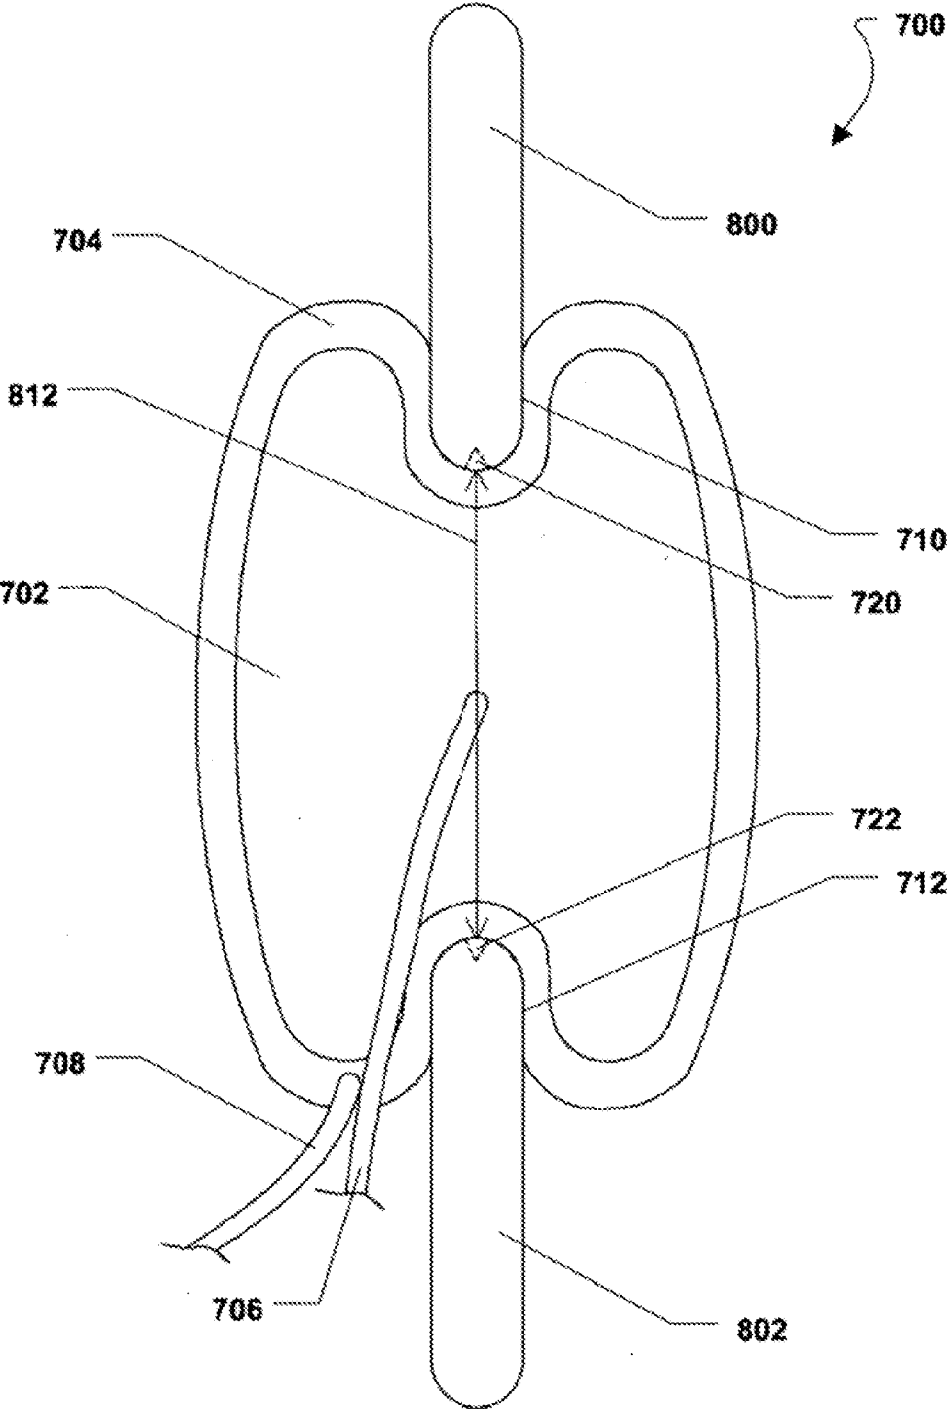


FIG. 8


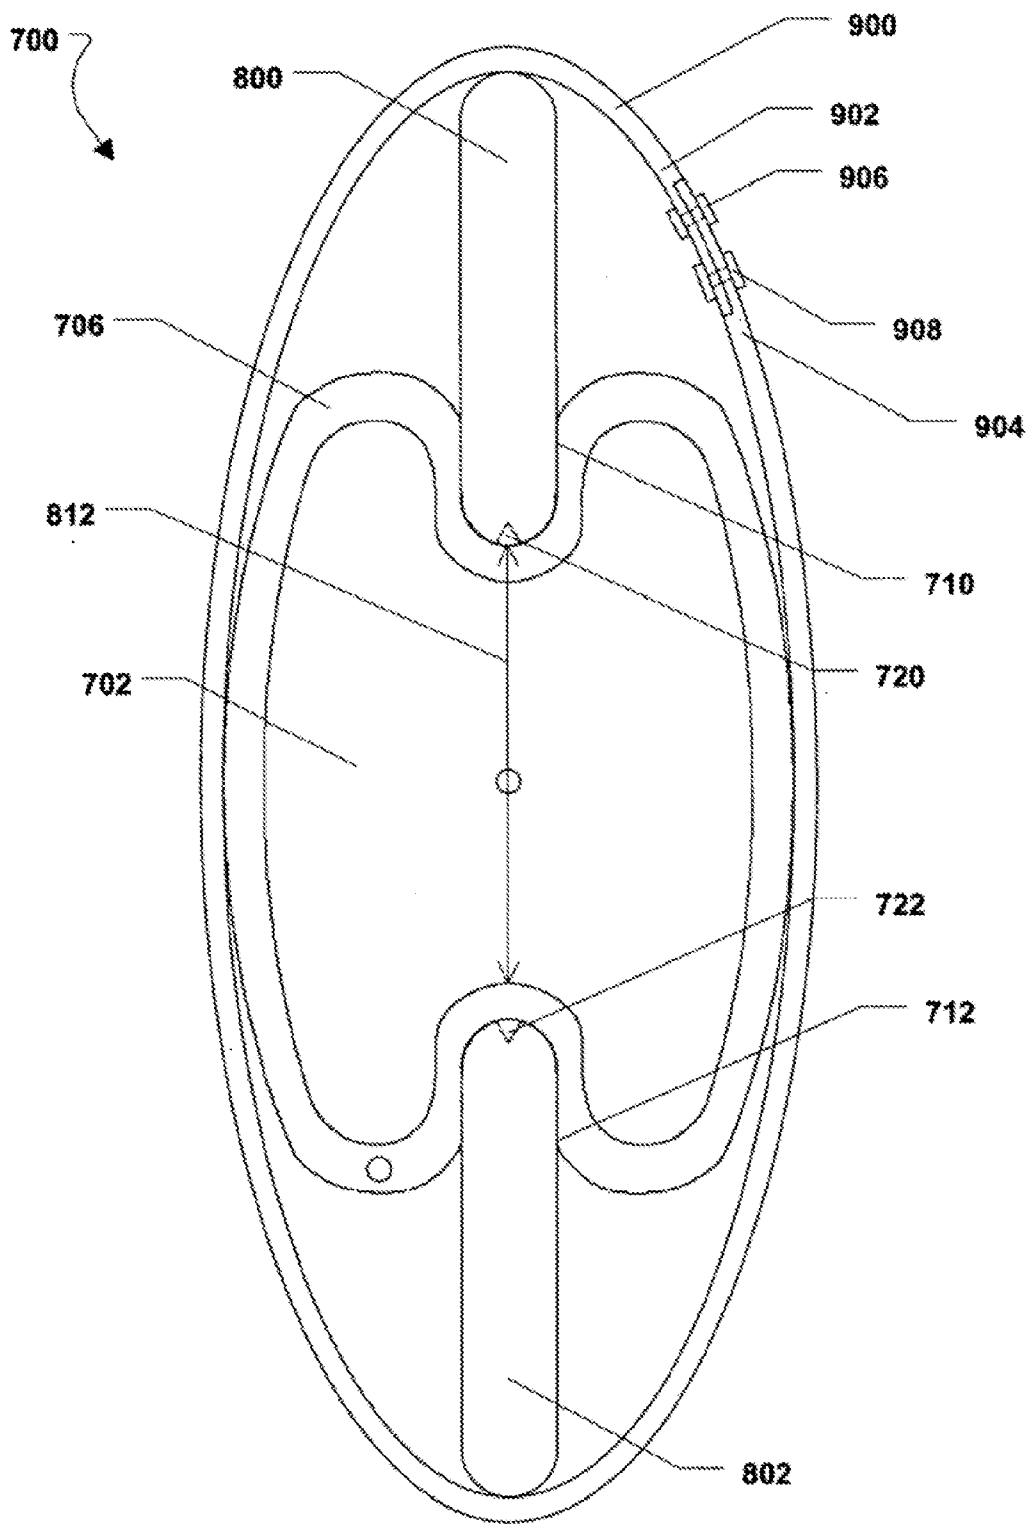


FIG. 9

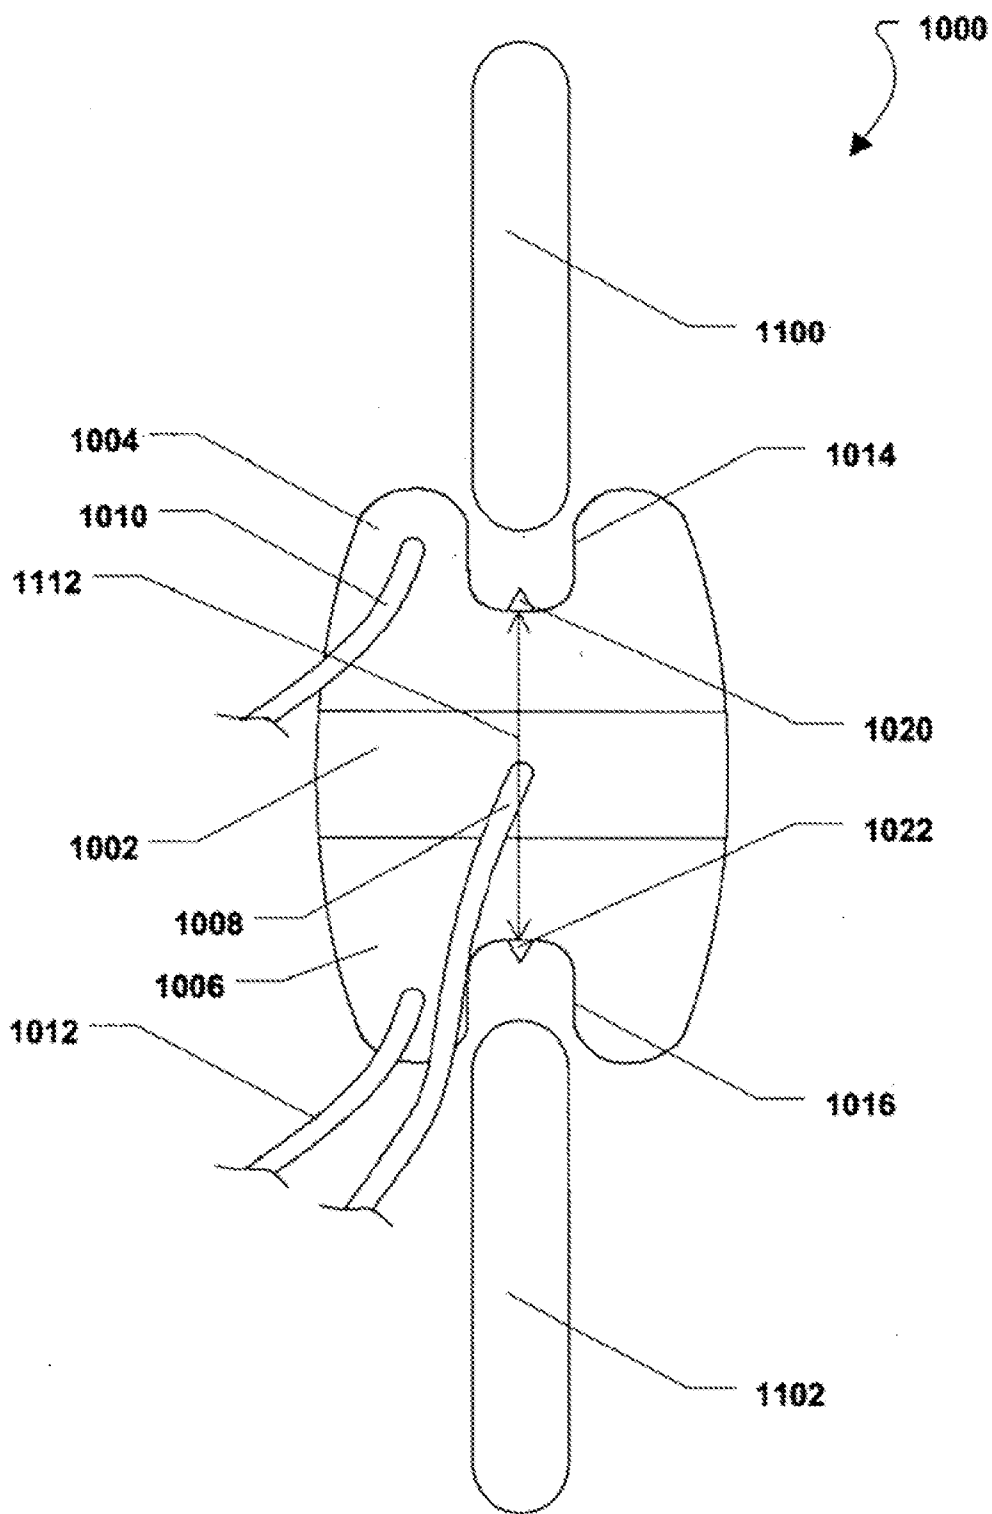

**FIG. 10**

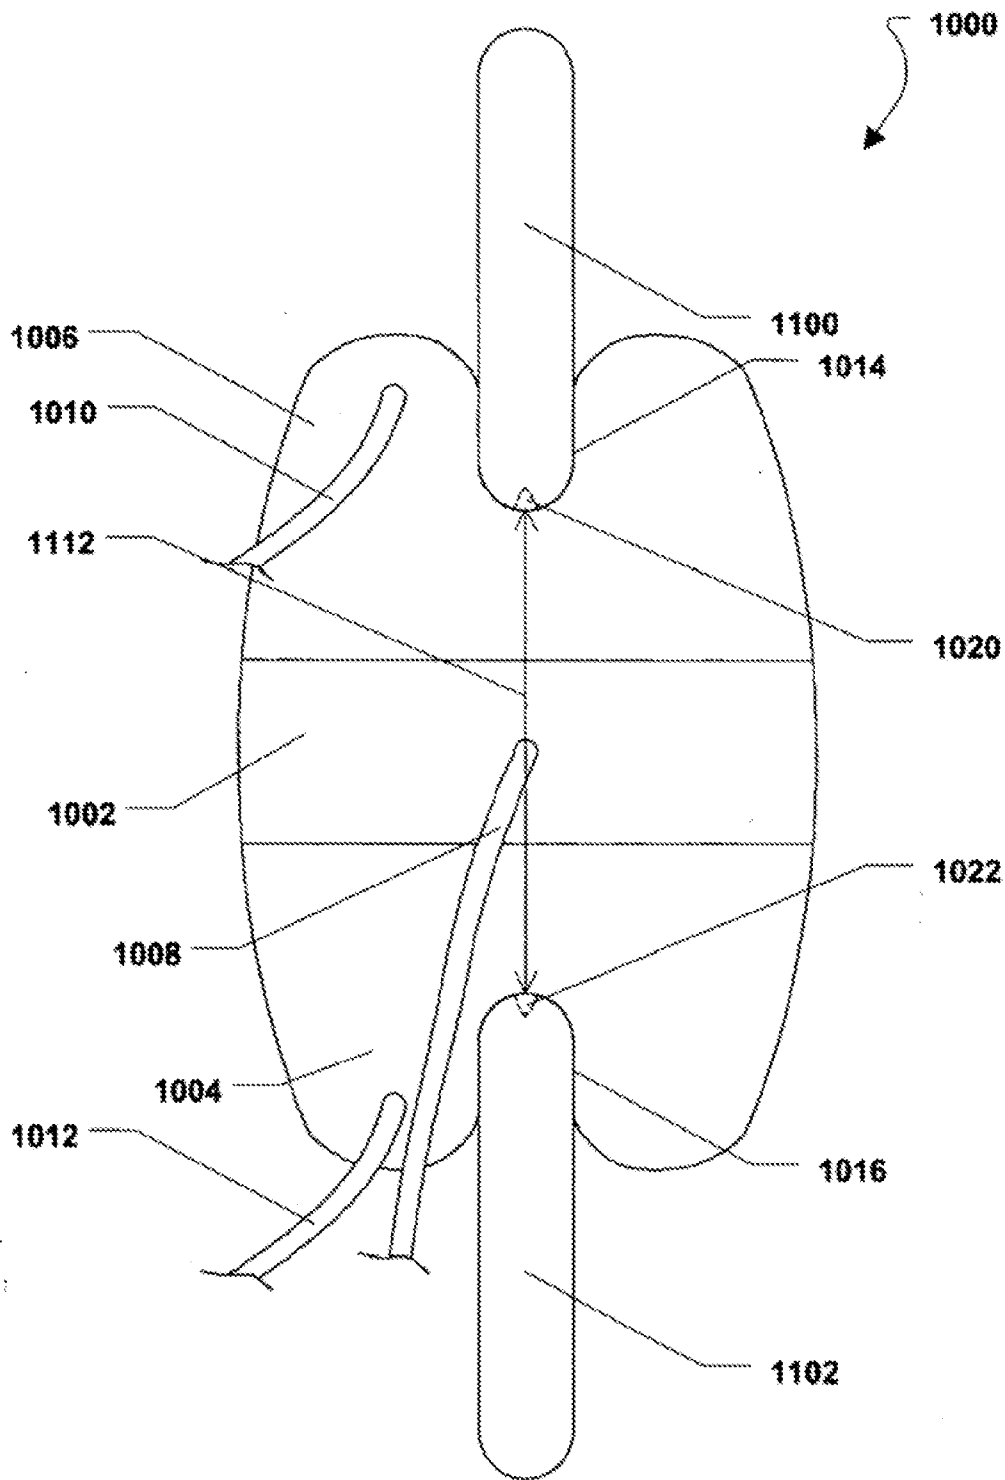


FIG. 11



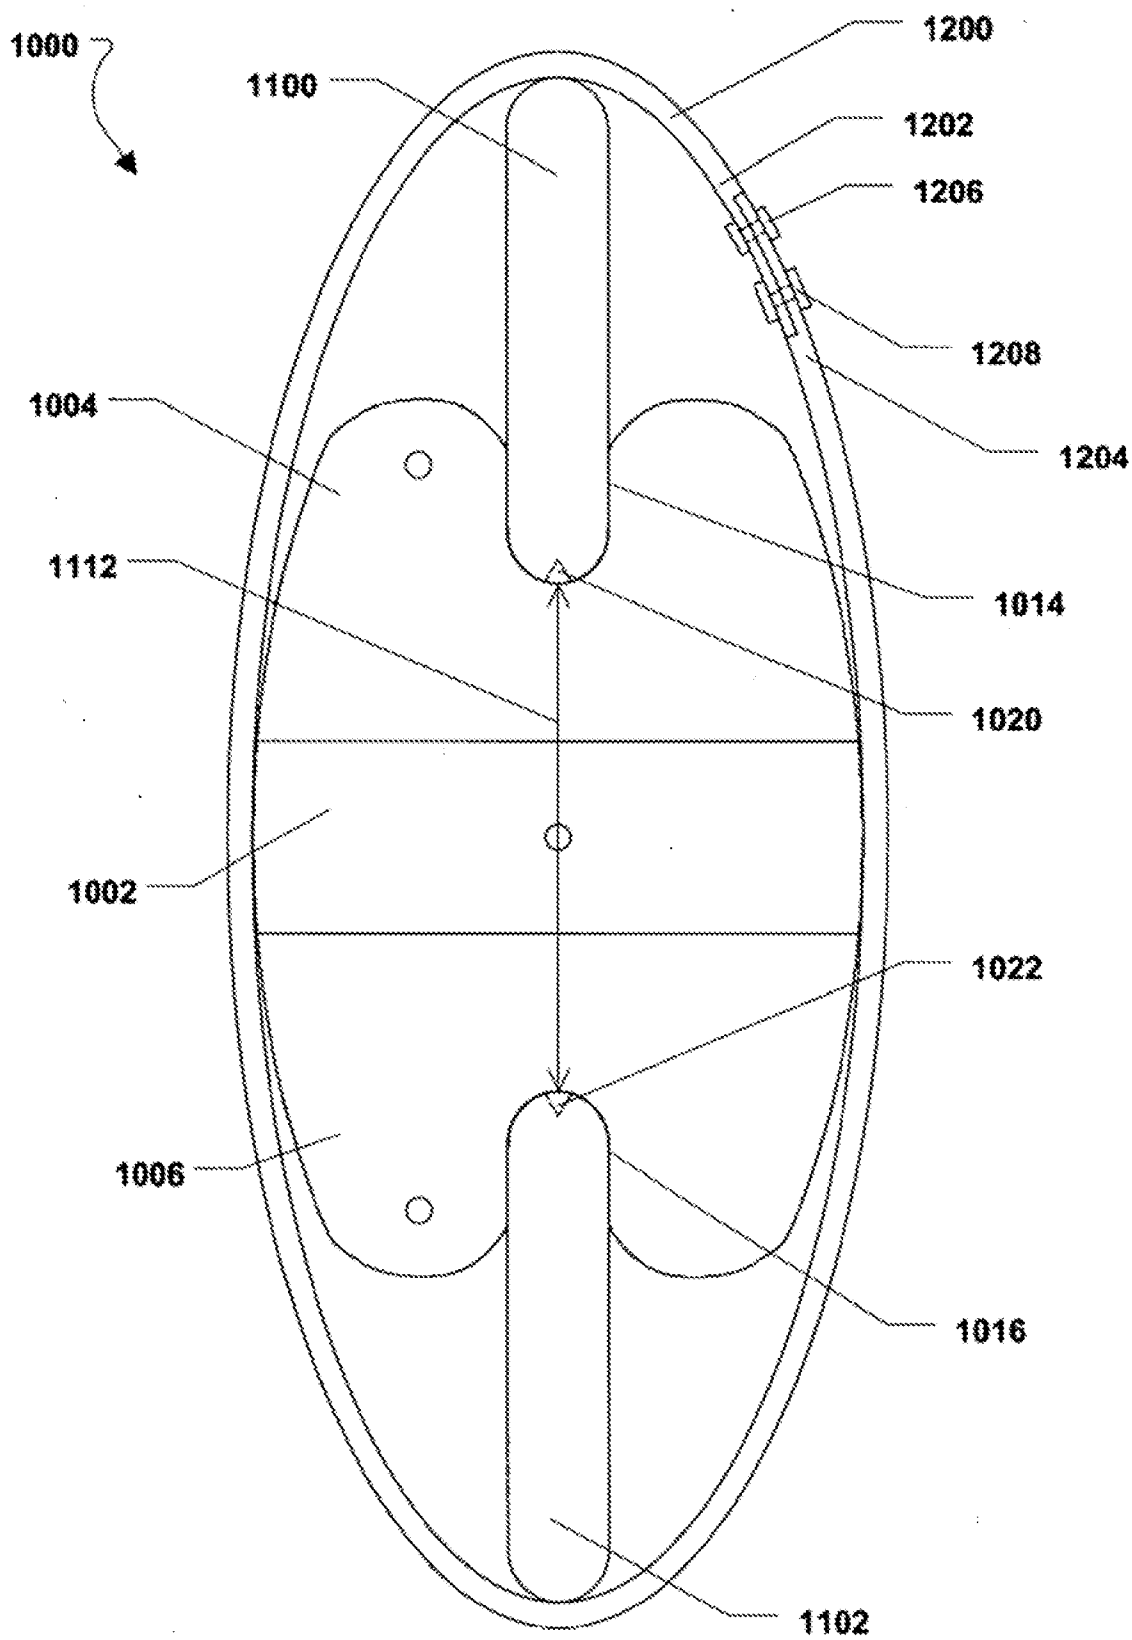



FIG. 12

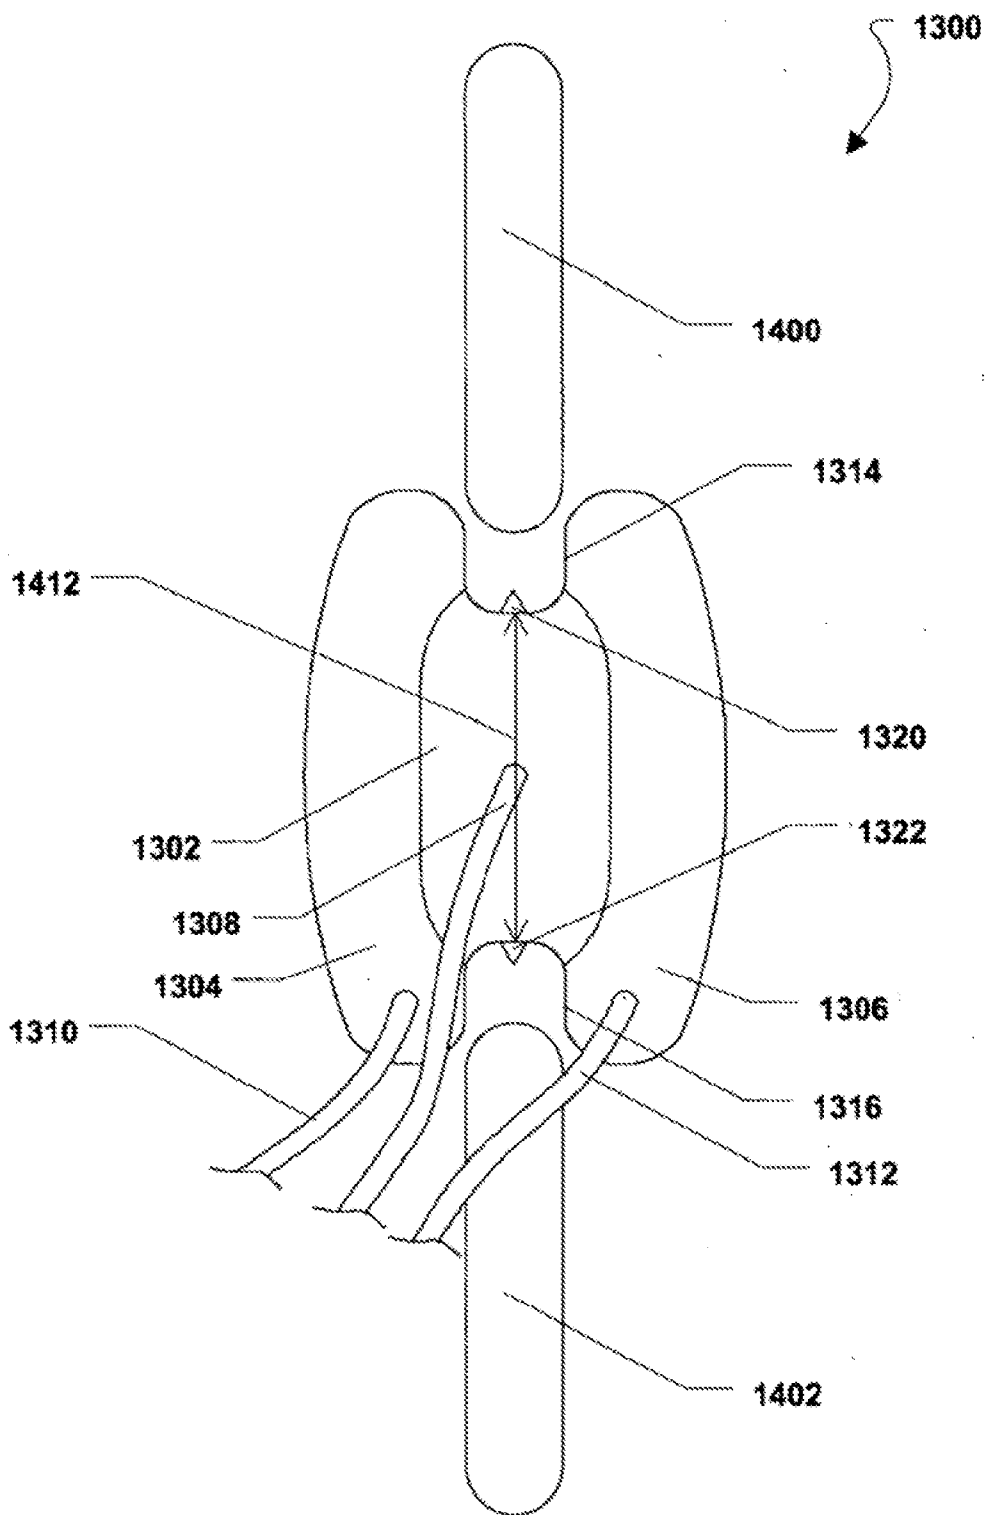

**FIG. 13**

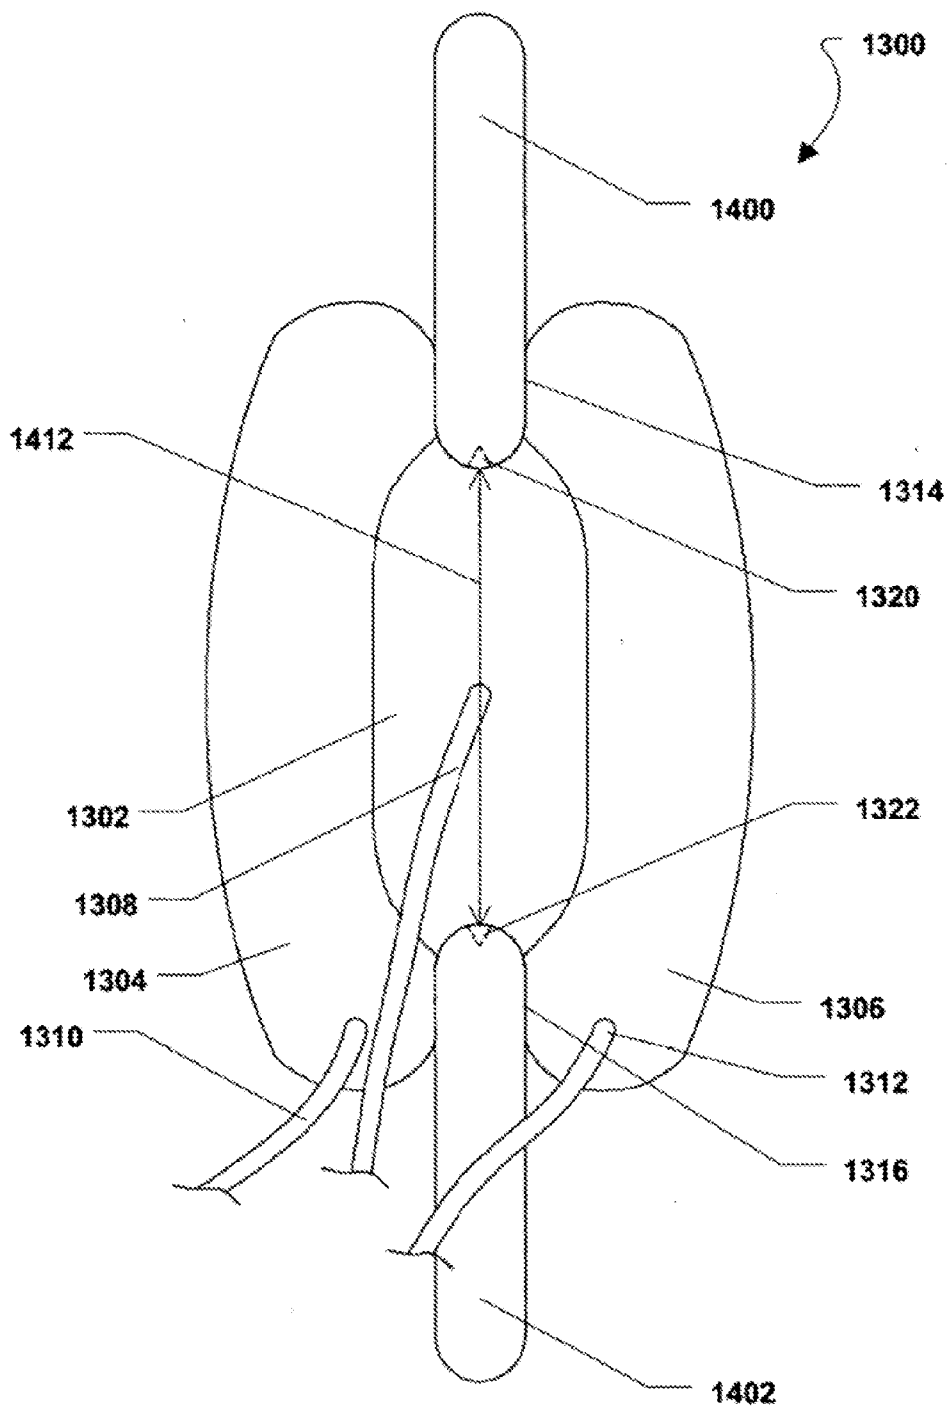

**FIG. 14**

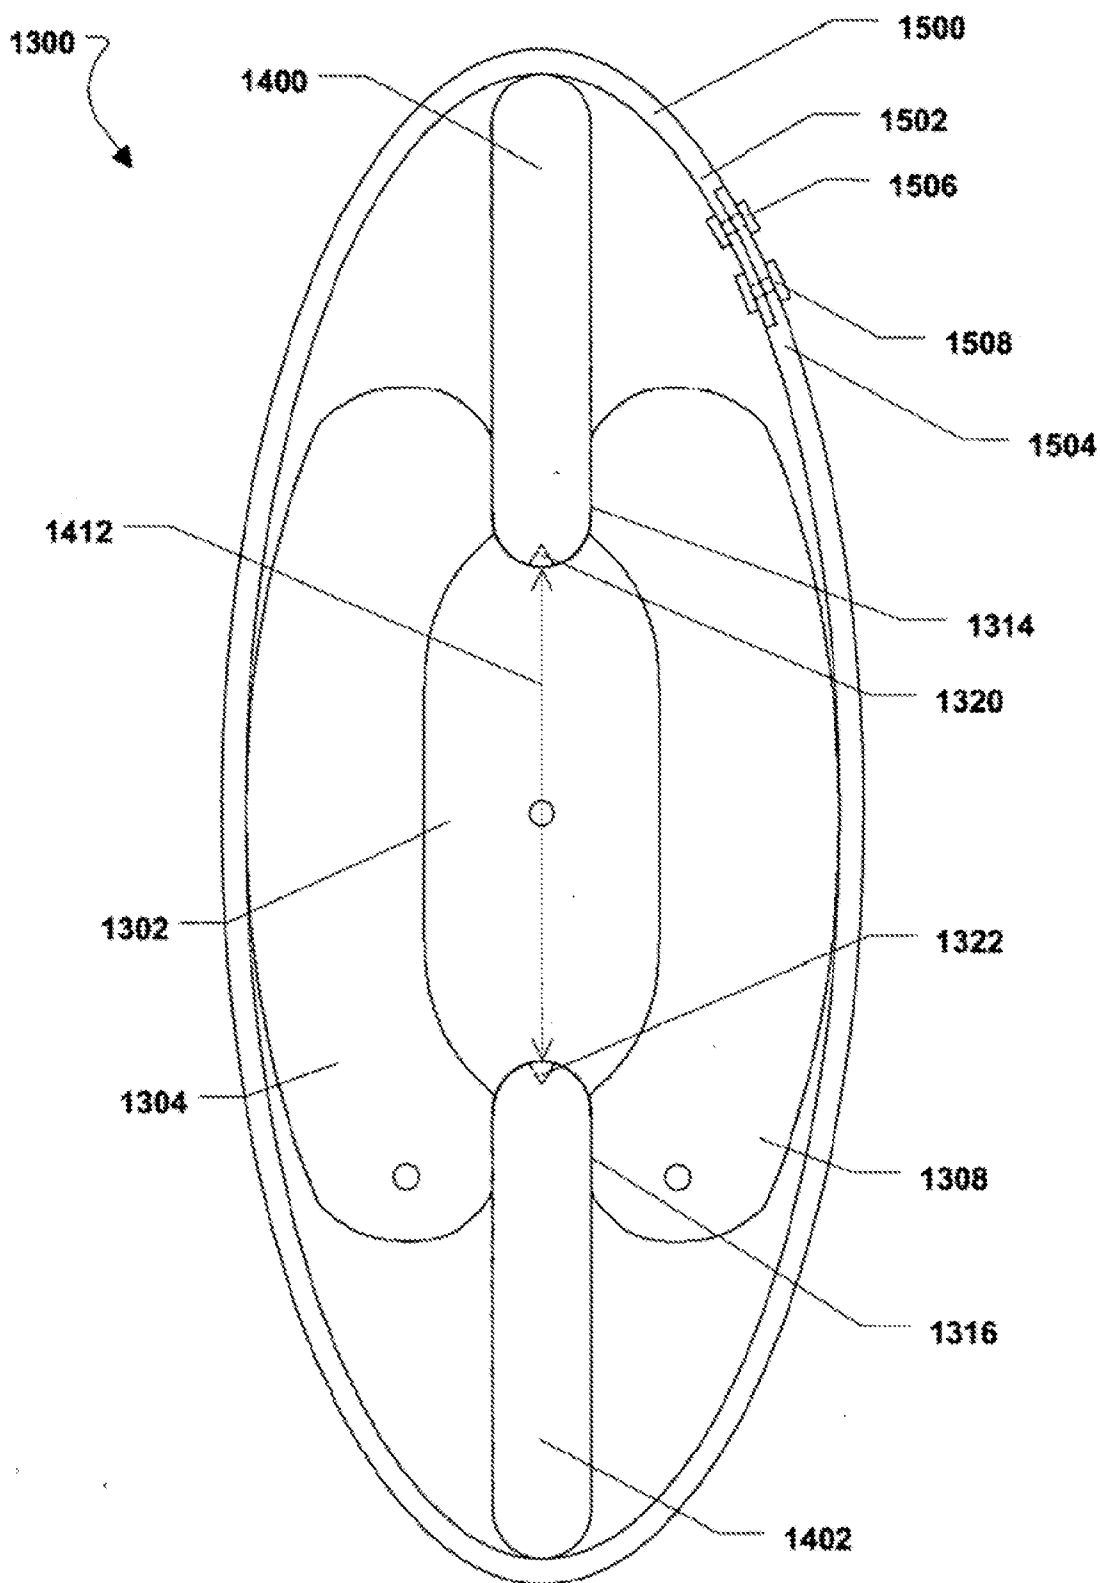

**FIG. 15**




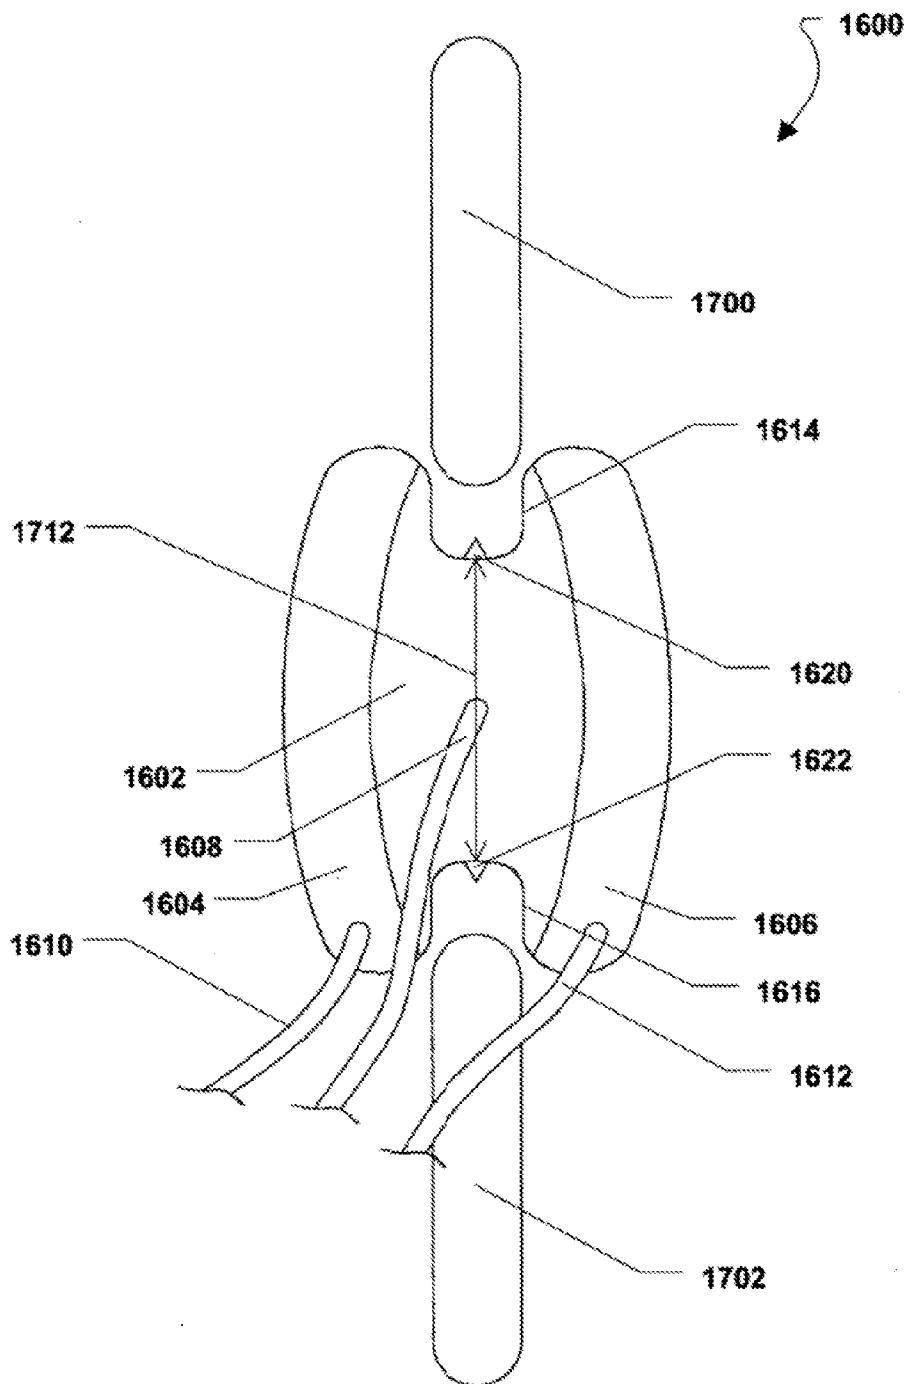


FIG. 16

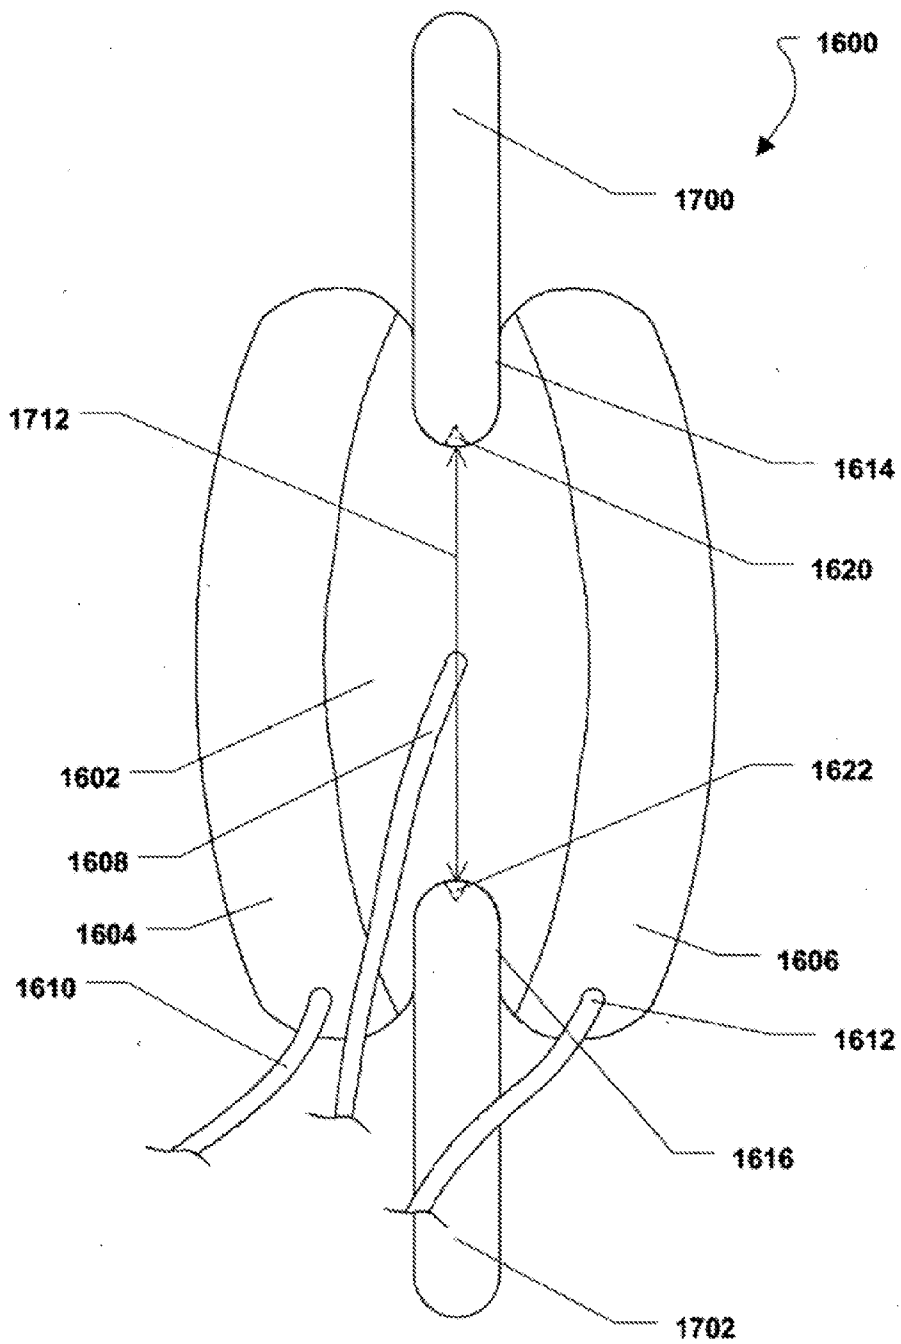

**FIG. 17**


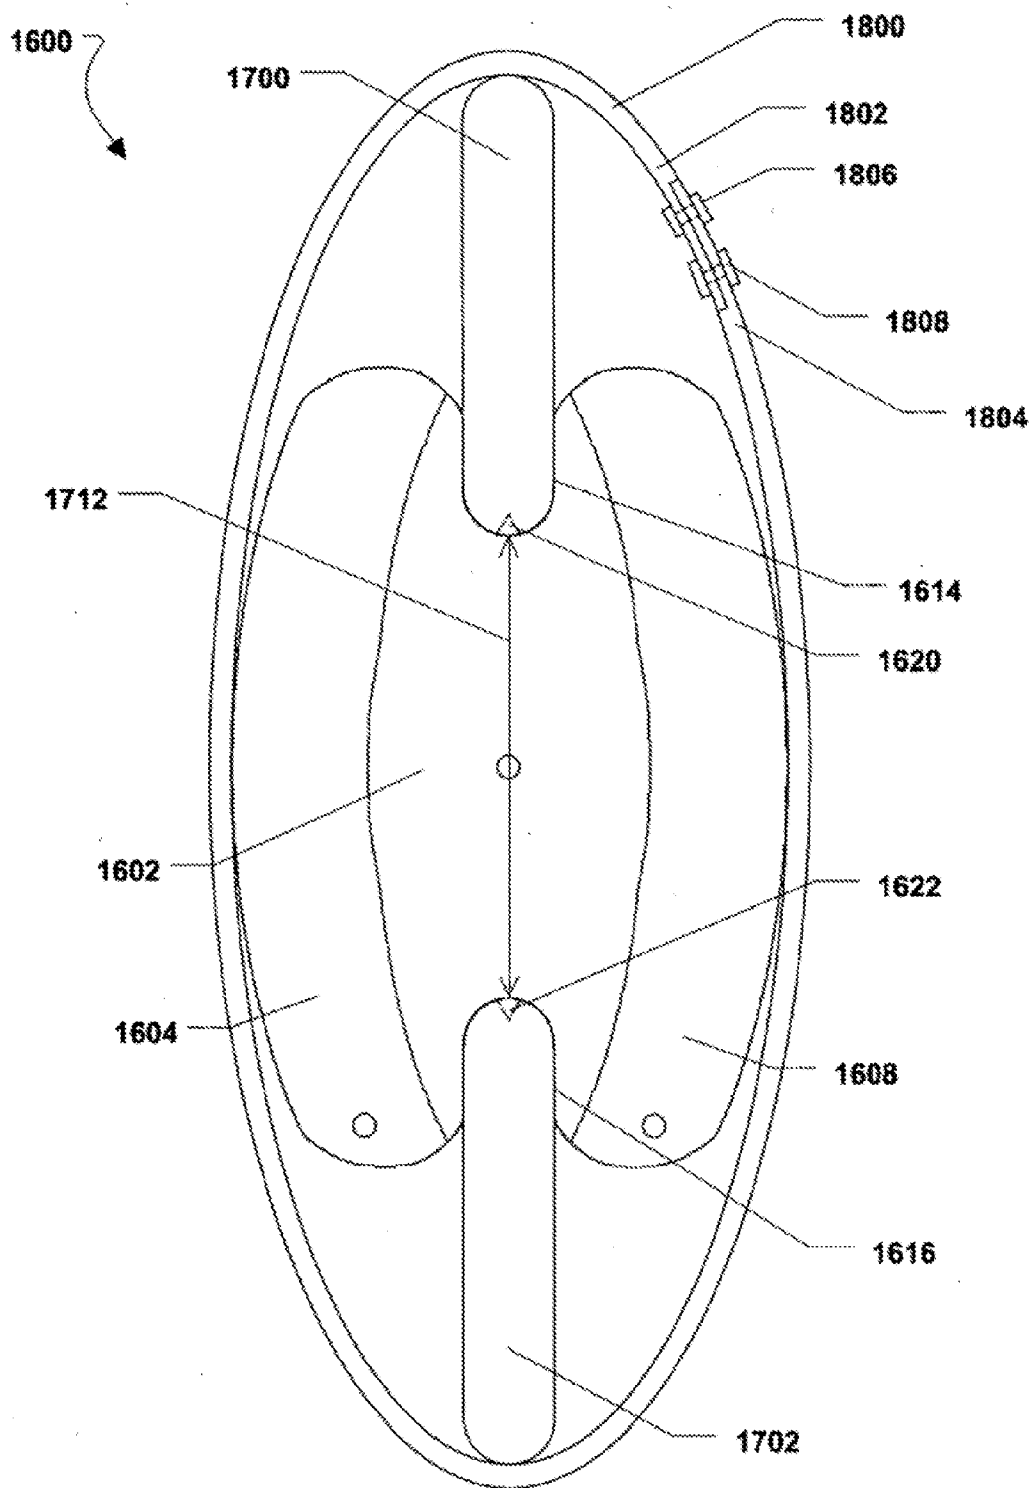


FIG. 18

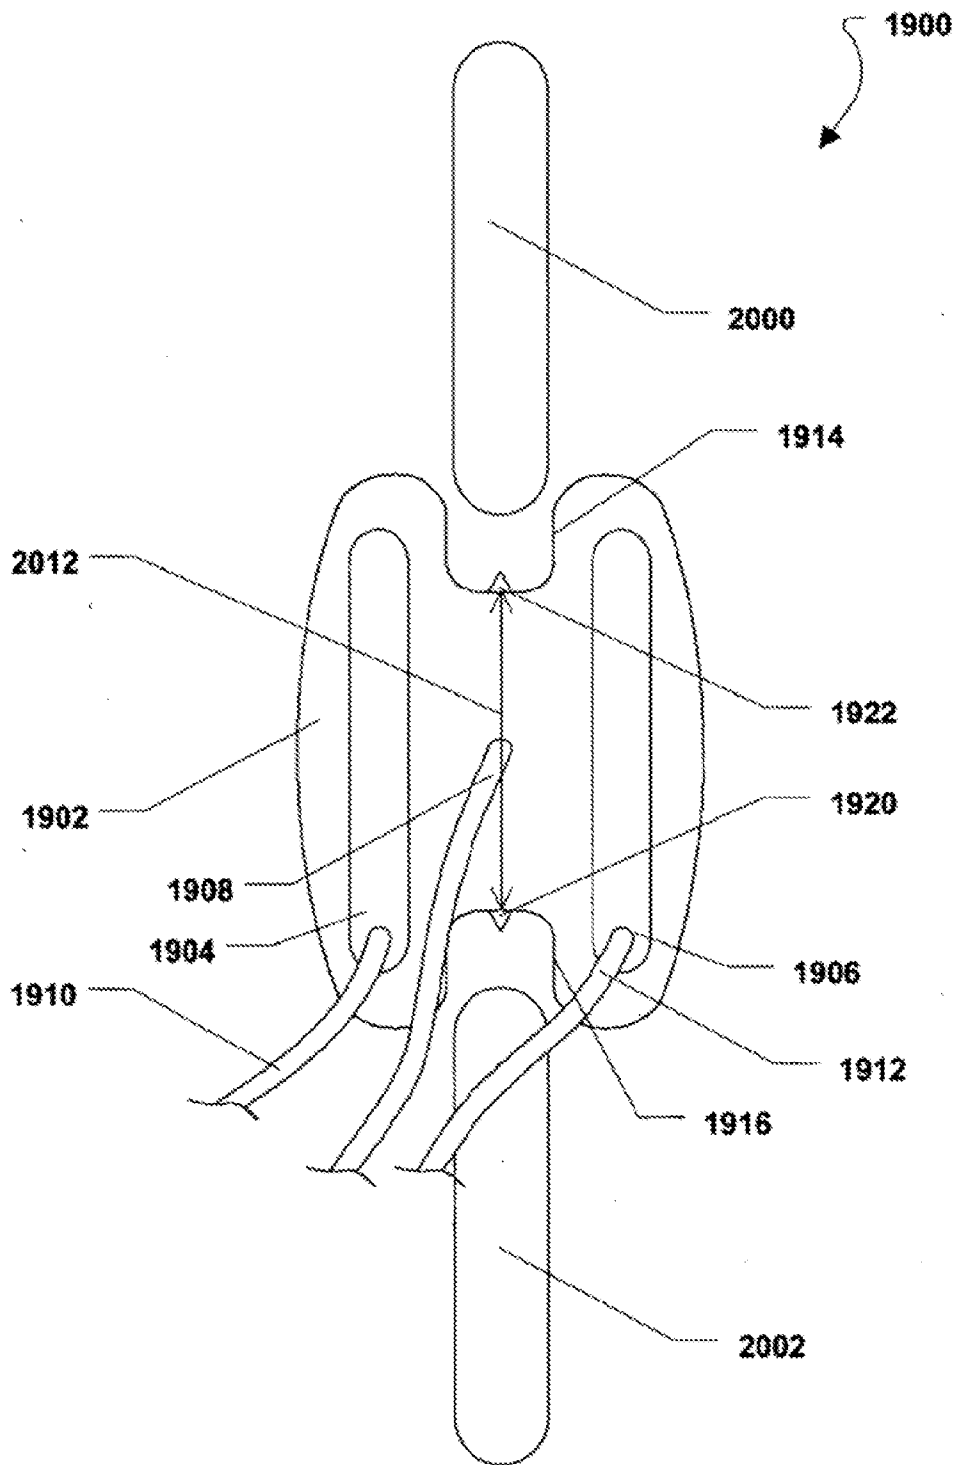

**FIG. 19**

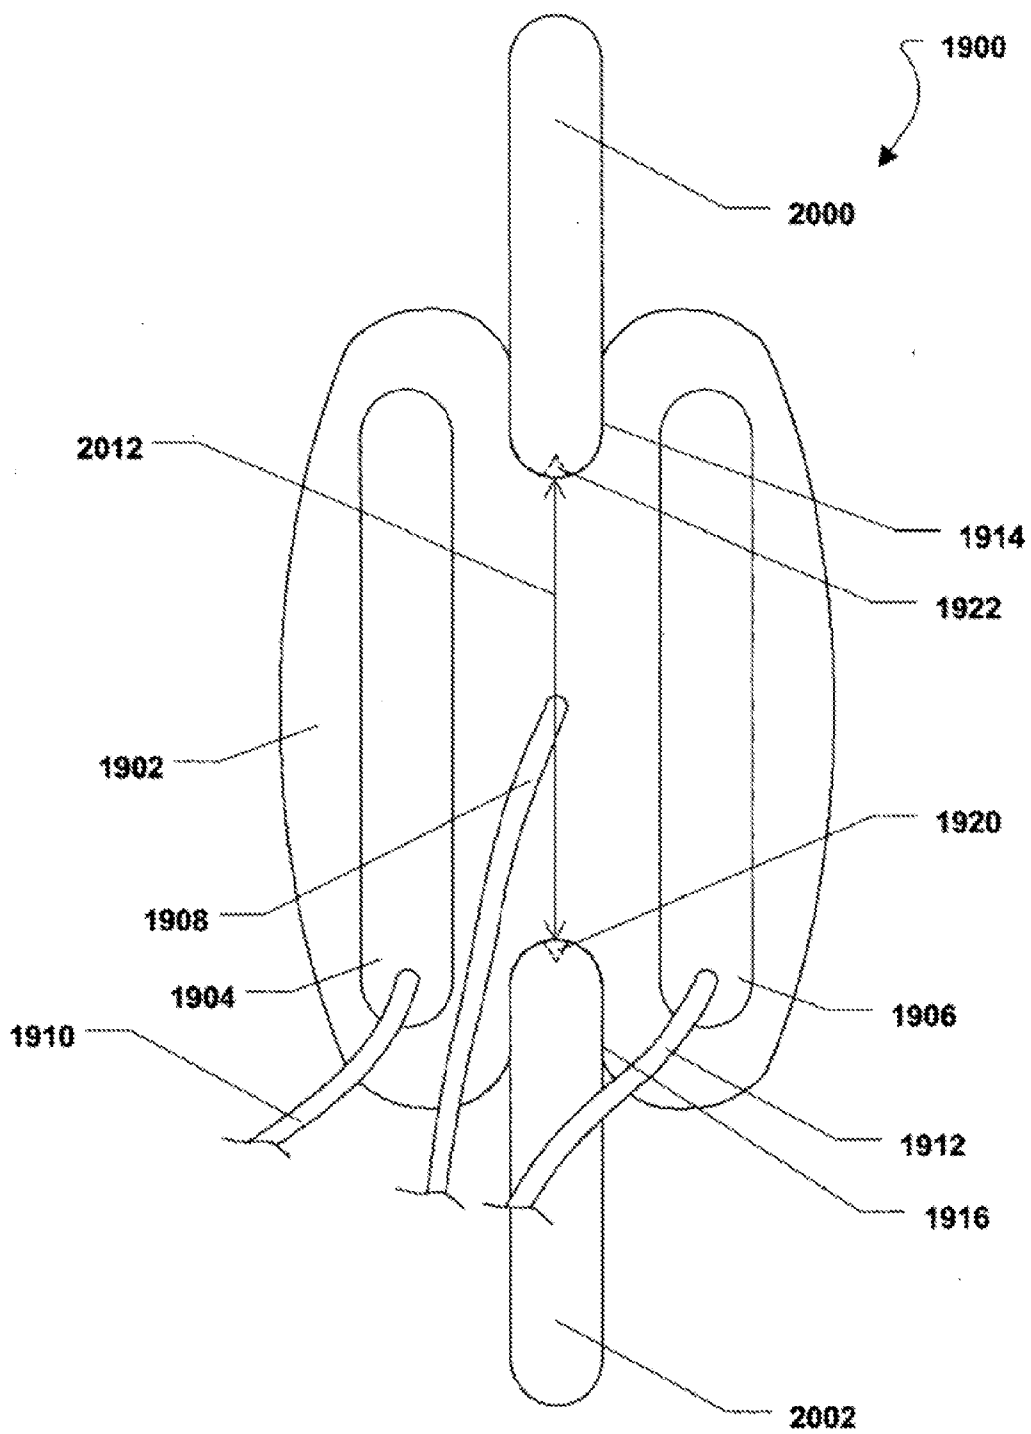


FIG. 20

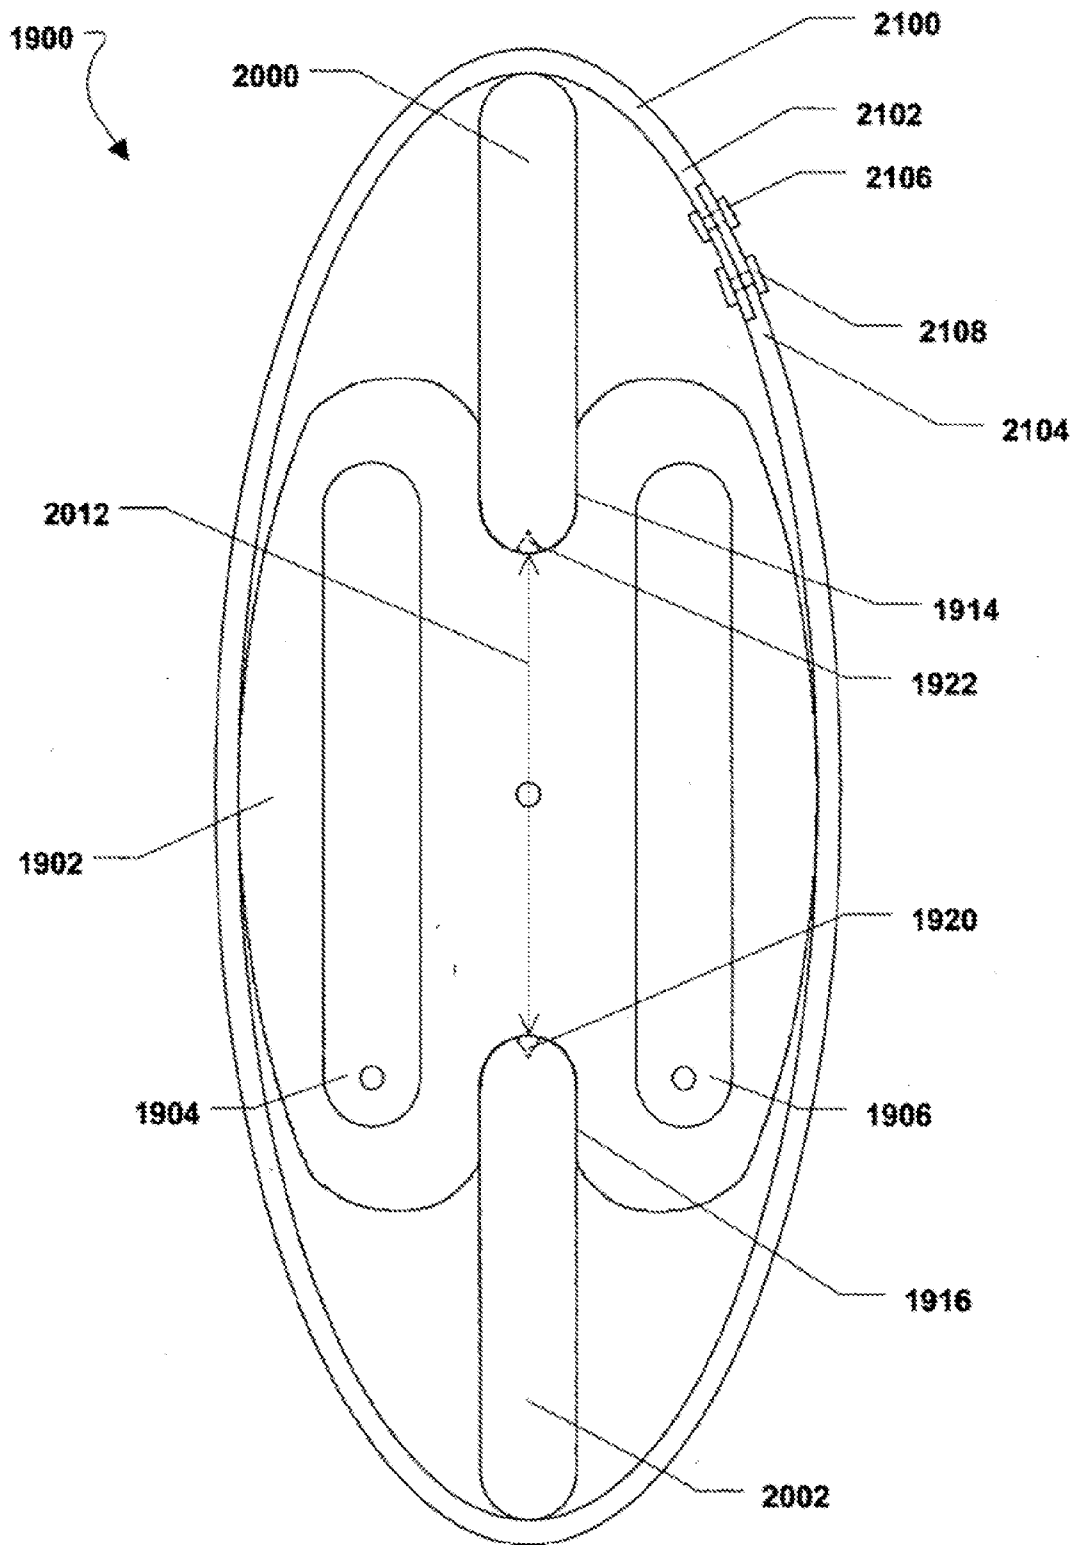


FIG. 21

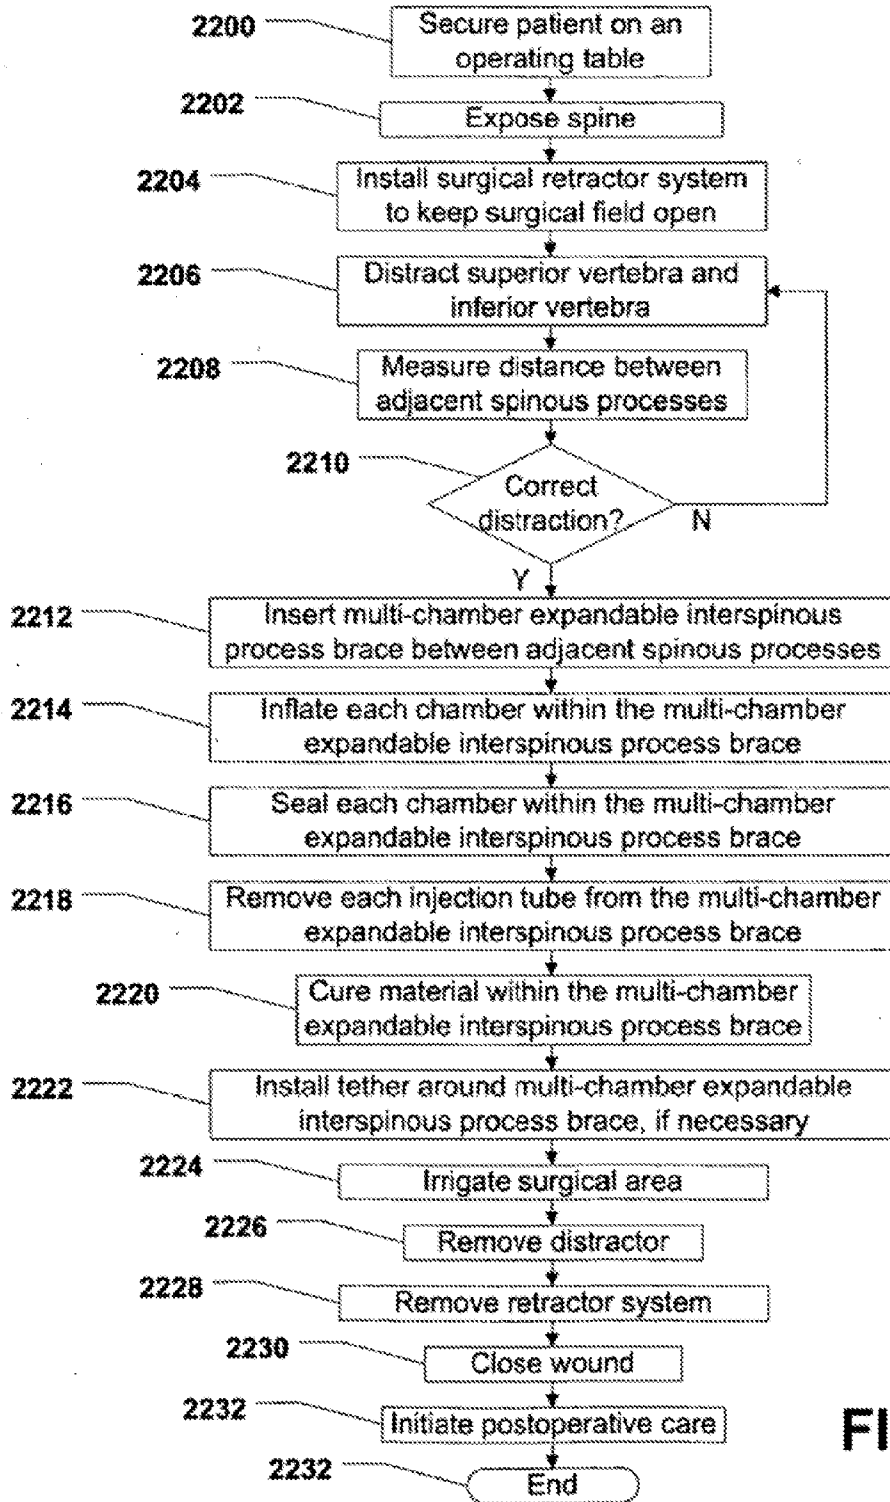


FIG. 22

**MULTI-CHAMBER EXPANDABLE INTERSPINOUS PROCESS SPACER**

[0001] This application is a continuation of co-pending U.S. patent application Ser. No. 12/795,883, filed Jun. 8, 2010 which is a divisional of U.S. patent application Ser. No. 11/413,587, filed 28 Apr. 2006, now abandoned, each of which is incorporated herein by reference in its entirety.

**FIELD OF THE INVENTION**

[0002] The present disclosure relates generally to orthopedics and orthopedic surgery. More specifically, the present disclosure relates to devices used to support adjacent spinous processes.

**BACKGROUND**

[0003] In human anatomy, the spine is a generally flexible column that can take tensile and compressive loads. The spine also allows bending motion and provides a place of attachment for keels, muscles and ligaments. Generally, the spine is divided into three sections: the cervical spine, the thoracic spine and the lumbar spine. The sections of the spine are made up of individual bones called vertebrae. Also, the vertebrae are separated by intervertebral discs, which are situated between adjacent vertebrae.

[0004] The intervertebral discs function as shock absorbers and as joints. Further, the intervertebral discs can absorb the compressive and tensile loads to which the spinal column may be subjected. At the same time, the intervertebral discs can allow adjacent vertebral bodies to move relative to each other a limited amount, particularly during bending, or flexure, of the spine. Thus, the intervertebral discs are under constant muscular and/or gravitational pressure and generally, the intervertebral discs are the first parts of the lumbar spine to show signs of deterioration.

[0005] Facet joint degeneration is also common because the facet joints are in almost constant motion with the spine. In fact, facet joint degeneration and disc degeneration frequently occur together. Generally, although one may be the primary problem while the other is a secondary problem resulting from the altered mechanics of the spine, by the time surgical options are considered, both facet joint degeneration and disc degeneration typically have occurred. For example, the altered mechanics of the facet joints and/or intervertebral disc may cause spinal stenosis, degenerative spondylolisthesis, and degenerative scoliosis.

**BRIEF DESCRIPTION OF THE DRAWINGS**

- [0006] FIG. 1 is a lateral view of a portion of a vertebral column;
- [0007] FIG. 2 is a lateral view of a pair of adjacent vertebrae;
- [0008] FIG. 3 is a top plan view of a vertebra;
- [0009] FIG. 4 is a plan view of a first multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0010] FIG. 5 is a plan view of the first multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0011] FIG. 6 is a plan view of the first multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around;

- [0012] FIG. 7 is a plan view of a second multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0013] FIG. 8 is a plan view of the second multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0014] FIG. 9 is a plan view of the second multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around;
- [0015] FIG. 10 is a plan view of a third multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0016] FIG. 11 is a plan view of the third multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0017] FIG. 12 is a plan view of the third multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around;
- [0018] FIG. 13 is a plan view of a fourth multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0019] FIG. 14 is a plan view of the fourth multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0020] FIG. 15 is a plan view of the fourth multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around;
- [0021] FIG. 16 is a plan view of a fifth multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0022] FIG. 17 is a plan view of the fifth multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0023] FIG. 18 is a plan view of the fifth multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around;
- [0024] FIG. 19 is a plan view of a sixth multi-chamber expandable interspinous process spacer in a deflated configuration;
- [0025] FIG. 20 is a plan view of the sixth multi-chamber expandable interspinous process spacer in an inflated configuration;
- [0026] FIG. 21 is a plan view of the sixth multi-chamber expandable interspinous process spacer in an inflated configuration with a tether installed there around; and
- [0027] FIG. 22 is a flow chart illustrating a method of treating a spine.

**DETAILED DESCRIPTION OF THE DRAWINGS**

[0028] A multi-chamber expandable interspinous process spacer or brace is disclosed and can include at least two chambers. Each of the at least two chambers can receive an injectable biocompatible material. Further, the multi-chamber expandable interspinous process brace can be moved between a deflated configuration and an inflated configuration. In the inflated configuration, the multi-chamber expandable interspinous process brace can engage and support a superior spinous process and an inferior spinous process. [0029] In another embodiment, a method of treating a spine is disclosed and can include installing a multi-chamber expandable interspinous process brace between a superior spinous process and an inferior spinous process. The method can also include inflating at least two chambers within the



multi-chamber expandable interspinous process brace to support the superior spinous process and the inferior spinous process.

[0030] In still another embodiment, a method of treating a spine is disclosed and can include distracting a superior spinous process and an inferior spinous process. Also, the method can include installing a multi-chamber expandable interspinous process brace between a superior spinous process and an inferior spinous process. Moreover, the method can include inflating at least two chambers within the multi-chamber expandable interspinous process brace to support the superior spinous process and the inferior spinous process.

[0031] In yet another embodiment, a kit for field use is disclosed and can include a multi-chamber expandable interspinous process brace that can have at least two chambers configured to receive an injectable biocompatible material. The kit can also include an injectable biocompatible material.

[0032] In still yet another embodiment, a kit for field use is disclosed and can include a multi-chamber expandable interspinous process brace that can include at least two chambers configured to receive an injectable biocompatible material. Additionally, the kit can include an injectable biocompatible material and a tether that can circumscribe the multi-chamber expandable interspinous process brace, a superior spinous process, and an inferior spinous process.

[0033] Description of Relevant Anatomy

[0034] Referring initially to FIG. 1, a portion of a vertebral column, designated 100, is shown. As depicted, the vertebral column 100 includes a lumbar region 102, a sacral region 104, and a coccygeal region 106. As is known in the art, the vertebral column 100 also includes a cervical region and a thoracic region. For clarity and ease of discussion, the cervical region and the thoracic region are not illustrated.

[0035] As shown in FIG. 1, the lumbar region 102 includes a first lumbar vertebra 108, a second lumbar vertebra 110, a third lumbar vertebra 112, a fourth lumbar vertebra 114, and a fifth lumbar vertebra 116. The sacral region 104 includes a sacrum 118. Further, the coccygeal region 106 includes a coccyx 120.

[0036] As depicted in FIG. 1, a first intervertebral lumbar disc 122 is disposed between the first lumbar vertebra 108 and the second lumbar vertebra 110. A second intervertebral lumbar disc 124 is disposed between the second lumbar vertebra 110 and the third lumbar vertebra 112. A third intervertebral lumbar disc 126 is disposed between the third lumbar vertebra 112 and the fourth lumbar vertebra 114. Further, a fourth intervertebral lumbar disc 128 is disposed between the fourth lumbar vertebra 114 and the fifth lumbar vertebra 116. Additionally, a fifth intervertebral lumbar disc 130 is disposed between the fifth lumbar vertebra 116 and the sacrum 118.

[0037] In a particular embodiment, if one of the intervertebral lumbar discs 122, 124, 126, 128, 130 is diseased, degenerated, damaged, or otherwise in need of repair, treatment of that intervertebral lumbar disc 122, 124, 126, 128, 130 can be effected in accordance with one or more of the embodiments described herein.

[0038] FIG. 2 depicts a detailed lateral view of two adjacent vertebrae, e.g., two of the lumbar vertebra 108, 110, 112, 114, 116 shown in FIG. 1. FIG. 2 illustrates a superior vertebra 200 and an inferior vertebra 202. As shown, each vertebra 200, 202 includes a vertebral body 204, a superior articular process 206, a transverse process 208, a spinous process 210 and an

inferior articular process 212. FIG. 2 further depicts an intervertebral disc 216 between the superior vertebra 200 and the inferior vertebra 202.

[0039] Referring to FIG. 3, a vertebra, e.g., the inferior vertebra 202 (FIG. 2), is illustrated. As shown, the vertebral body 204 of the inferior vertebra 202 includes a cortical rim 302 composed of cortical bone. Also, the vertebral body 204 includes cancellous bone 304 within the cortical rim 302. The cortical rim 302 is often referred to as the apophyseal rim or apophyseal ring. Further, the cancellous bone 304 is softer than the cortical bone of the cortical rim 302.

[0040] As illustrated in FIG. 3, the inferior vertebra 202 further includes a first pedicle 306, a second pedicle 308, a first lamina 310, and a second lamina 312. Further, a vertebral foramen 314 is established within the inferior vertebra 202. A spinal cord 316 passes through the vertebral foramen 314. Moreover, a first nerve root 318 and a second nerve root 320 extend from the spinal cord 316.

[0041] It is well known in the art that the vertebrae that make up the vertebral column have slightly different appearances as they range from the cervical region to the lumbar region of the vertebral column. However, all of the vertebrae, except the first and second cervical vertebrae, have the same basic structures, e.g., those structures described above in conjunction with FIG. 2 and FIG. 3. The first and second cervical vertebrae are structurally different than the rest of the vertebrae in order to support a skull.

#### Description of a First Embodiment of a Multi-Chamber Expandable Interspinous Process Brace

[0042] Referring to FIG. 4 through FIG. 6, a first embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated 400. As shown, the multi-chamber expandable interspinous process brace 400 includes an interior chamber 402 and an exterior chamber 404.

[0043] In a particular embodiment, the interior chamber 402 can be generally elliptical. Alternatively, the interior chamber 402 can be generally spherical, generally pyramidal, generally conical, generally frustal, generally cubic, generally polyhedral, or a combination thereof. The exterior chamber 404 can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, the exterior chamber 404 can be generally H-shaped.

[0044] Further, in a particular embodiment, the chambers 402, 404 can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers 402, 404 can be non-porous or micro-porous, e.g., for venting purposes.

[0045] As shown in FIG. 4, the interior chamber 402 can include a first injection tube 406. Further, the exterior chamber 404 can include a second injection tube 408. The injection tubes 406, 408 can be used to provide an injectable biocompatible material to the chambers 402, 404. In a particular embodiment, each of the interior chamber 402 and the exterior chamber 404 of the multi-chamber expandable interspinous process brace 400 can be expanded from a respective deflated configuration, shown in FIG. 4, to one of a plurality of inflated configurations, shown in FIG. 5, up to a maximum

inflated configuration. Further, after the interior chamber 402 and the exterior chamber 404 are inflated, or otherwise expanded, the injection tubes 406, 408 can be removed, as depicted in FIG. 6.

[0046] In a particular embodiment, the multi-chamber expandable interspinous process brace 400 can include a first self-sealing valve (not shown) within the interior chamber 402, e.g., adjacent to the first injection tube 406. Moreover, the multi-chamber expandable interspinous process brace 400 can include a second self-sealing valve (not shown) within the exterior chamber 404, e.g., adjacent to the second injection tube 408. The self-sealing valves can prevent the chambers 402, 404 from leaking material after the chambers 402, 404 are inflated and the injection tubes 406, 408 are removed.

[0047] As illustrated in FIG. 4 through FIG. 6, the exterior chamber 404 can include a superior spinous process pocket 410 and an inferior spinous process pocket 412. Further, a superior spinous process engagement structure 420 can extend from the exterior chamber 404 within the superior spinous process pocket 410. Also, an inferior spinous process engagement structure 422 can extend from the exterior chamber 404 within the inferior spinous process pocket 412. In a particular embodiment, each of the spinous process engagement structures 420, 422 can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

[0048] FIG. 4 through FIG. 6 indicate that the multi-chamber expandable interspinous process brace 400 can be implanted between a superior spinous process 500 and an inferior spinous process 502. In a particular embodiment, the chambers 402, 404 can be inflated so the exterior chamber 404 engages the spinous processes 500, 502. In a particular embodiment, when the multi-chamber expandable interspinous process brace 400 is properly installed and inflated between the superior spinous process 500 and the inferior spinous process 502, the superior spinous process pocket 410 can engage and support the superior spinous process 500. Further, the inferior spinous process pocket 412 can engage and support an inferior spinous process 502.

[0049] More specifically, the superior spinous process engagement structure 420 can extend slightly into and engage the superior spinous process 500. Also, the inferior spinous process engagement structure 422 can extend slightly into and engage the inferior spinous process 502. Accordingly, the spinous process engagement structures 420, 422, the spinous process pockets 410, 412, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace 400 from migrating with respect to the spinous processes 500, 502.

[0050] Also, in a particular embodiment, the multi-chamber expandable interspinous process brace 400 can be movable between a deflated configuration, shown in FIG. 4, and one or more inflated configurations, shown in FIG. 5 and FIG. 6. In the deflated configuration, a distance 512 between the superior spinous process pocket 410 and the inferior spinous process pocket 412 can be at a minimum. However, as one or more materials are injected into the chambers 402, 404, the distance 512 between the superior spinous process pocket 410 and the inferior spinous process pocket 412 can increase.

[0051] Accordingly, the multi-chamber expandable interspinous process brace 400 can be installed between a superior spinous process 500 and an inferior spinous process 502. Further, the multi-chamber expandable interspinous process

brace 400 can be expanded, e.g., by injecting one or more materials into the chambers 402, 404, in order to increase the distance between the superior spinous process 500 and the inferior spinous process 502.

[0052] Alternatively, a distractor can be used to increase the distance between the superior spinous process 500 and the inferior spinous process 502 and the multi-chamber expandable interspinous process brace 400 can be expanded to support the superior spinous process 500 and the inferior spinous process 502. After the multi-chamber expandable interspinous process brace 400 is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace 400 can support the superior spinous process 500 and the inferior spinous process 502 to substantially prevent the distance between the superior spinous process 502 and the inferior spinous process 500 from returning to a pre-distraction value.

[0053] In a particular embodiment, the multi-chamber expandable interspinous process brace 400 can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0054] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylate, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluoropolyolefins.

[0055] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylacid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0056] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0057] In a particular embodiment, the hardness of the material used to inflate the interior chamber 402 can be less than or equal to the hardness of the material used to inflate the exterior chamber 404, i.e., after the materials used to inflate the interior chamber 402 and the exterior chamber 404 are cured. Alternatively, the viscosity of the material used to inflate the interior chamber 402 can be less than or equal to the viscosity of the material used to inflate the exterior chamber 404. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0058] FIG. 6 indicates that a tether 600 can be installed around the multi-chamber expandable interspinous process brace 400, after the multi-chamber expandable interspinous process brace 400 is expanded as described herein. As shown, the tether 600 can include a proximal end 602 and a distal end 604. In a particular embodiment, the tether 600 can circumscribe the multi-chamber expandable interspinous process brace 400 and the spinous processes 500, 502. Further, the ends 602, 604 of the tether 600 can be brought together and one or more fasteners can be installed therethrough to connect

the ends **602**, **604**. Accordingly, the tether **600** can be installed in order to prevent the distance between the spinous processes **500**, **502** from substantially increasing beyond the distance provided by the multi-chamber expandable interspinous process brace **400** after it is expanded and to maintain engagement of the interspinous processes with the spinous process pockets **410**, **412**, the engagement structures **420**, **422**, or a combination thereof.

[0059] In a particular embodiment, the tether **600** can comprise a biocompatible elastomeric material that flexes during installation and provides a resistance fit against the inferior process. Further, the tether **600** can comprise a substantially non-resorbable suture or the like.

#### Description of a Second Embodiment of a Multi-Chamber Expandable Interspinous Process Brace

[0060] Referring to FIG. 7 through FIG. 9, a second embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated **700**. As shown, the multi-chamber expandable interspinous process brace **700** includes an interior chamber **702** and an exterior chamber **704**.

[0061] The interior chamber **702** and the exterior chamber **704** can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, the interior chamber **702** can be generally H-shaped. Also, in a particular embodiment, the exterior chamber **704** can be hollow and generally H-shaped. More specifically, the exterior chamber **704** can be shaped to match the outer perimeter of the interior chamber **702**.

[0062] Further, in a particular embodiment, the chambers **702**, **704** can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers **702**, **704** can be non-porous or micro-porous, e.g., for venting purposes.

[0063] As shown in FIG. 7, the interior chamber **702** can include a first injection tube **706**. Further, the exterior chamber **704** can include a second injection tube **708**. The injection tubes **706**, **708** can be used to provide an injectable biocompatible material to the chambers **702**, **704**. In a particular embodiment, each of the interior chamber **702** and the exterior chamber **704** of the multi-chamber expandable interspinous process brace **700** can be expanded from a respective deflated configuration, shown in FIG. 7, to one of a plurality of inflated configurations, shown in FIG. 8, up to a maximum inflated configuration. Further, after the interior chamber **702** and the exterior chamber **704** are inflated, or otherwise expanded, the injection tubes **706**, **708** can be removed, as depicted in FIG. 9.

[0064] In a particular embodiment, the multi-chamber expandable interspinous process brace **700** can include a first self-sealing valve (not shown) within the interior chamber **702**, e.g., adjacent to the first injection tube **706**. Moreover, the multi-chamber expandable interspinous process brace **700** can include a second self-sealing valve (not shown) within the exterior chamber **704**, e.g., adjacent to the second injection tube **708**. The self-sealing valves can prevent the chambers **702**, **704** from leaking material after the chambers **702**, **704** are inflated and the injection tubes **706**, **708** are removed.

[0065] As illustrated in FIG. 7 through FIG. 9, the exterior chamber **704** can include a superior spinous process pocket **710** and an inferior spinous process pocket **712**. Further, a superior spinous process engagement structure **720** can extend from the exterior chamber **704** within the superior spinous process pocket **710**. Also, an inferior spinous process engagement structure **722** can extend from the exterior chamber **704** within the inferior spinous process pocket **712**. In a particular embodiment, each of the spinous process engagement structures **720**, **722** can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

[0066] FIG. 7 through FIG. 9 indicate that the multi-chamber expandable interspinous process brace **700** can be implanted between a superior spinous process **800** and an inferior spinous process **802**. In a particular embodiment, the chambers **702**, **704** can be inflated so the exterior chamber **704** engages the spinous processes **800**, **802**. In a particular embodiment, when the multi-chamber expandable interspinous process brace **700** is properly installed and inflated between the superior spinous process **800** and the inferior spinous process **802**, the superior spinous process pocket **710** can engage and support the superior spinous process **800**. Further, the inferior spinous process pocket **712** can engage and support an inferior spinous process **802**.

[0067] More specifically, the superior spinous process engagement structure **720** can extend slightly into and engage the superior spinous process **800**. Also, the inferior spinous process engagement structure **722** can extend slightly into and engage the inferior spinous process **802**. Accordingly, the spinous process engagement structures **720**, **722**, the spinous process pockets **710**, **712**, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace **700** from migrating with respect to the spinous processes **800**, **802**.

[0068] Also, in a particular embodiment, the multi-chamber expandable interspinous process brace **700** can be movable between a deflated configuration, shown in FIG. 7, and one or more inflated configurations, shown in FIG. 8 and FIG. 9. In the deflated configuration, a distance **812** between the superior spinous process pocket **710** and the inferior spinous process pocket **712** can be at a minimum. However, as one or more materials are injected into the chambers **702**, **704**, the distance **812** between the superior spinous process pocket **710** and the inferior spinous process pocket **712** can increase.

[0069] Accordingly, the multi-chamber expandable interspinous process brace **700** can be installed between a superior spinous process **800** and an inferior spinous process **802**. Further, the multi-chamber expandable interspinous process brace **700** can be expanded, e.g., by injecting one or more materials into the chambers **702**, **704**, in order to increase the distance between the superior spinous process **800** and the inferior spinous process **802**.

[0070] Alternatively, a distractor can be used to increase the distance between the superior spinous process **800** and the inferior spinous process **802** and the multi-chamber expandable interspinous process brace **700** can be expanded to support the superior spinous process **800** and the inferior spinous process **802**. After the multi-chamber expandable interspinous process brace **700** is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace **700** can support the superior spinous process **800** and the inferior spinous process **802** to substantially prevent the distance between the superior

spinous process **802** and the inferior spinous process **800** from returning to a pre-distraction value.

[0071] In a particular embodiment, the multi-chamber expandable interspinous process brace **700** can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0072] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylates, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluoropolyolefins.

[0073] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylacid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0074] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0075] In a particular embodiment, the hardness of the material used to inflate the interior chamber **702** can be greater than or equal to the hardness of the material used to inflate the exterior chamber **704**, i.e., after the materials used to inflate the interior chamber **702** and the exterior chamber **704** are cured. Alternatively, the viscosity of the material used to inflate the interior chamber **702** can be greater than or equal to the viscosity of the material used to inflate the exterior chamber **704**. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0076] FIG. 9 indicates that a tether **900** can be installed around the multi-chamber expandable interspinous process brace **700**, after the multi-chamber expandable interspinous process brace **700** is expanded as described herein. As shown, the tether **900** can include a proximal end **902** and a distal end **904**. In a particular embodiment, the tether **900** can circumscribe the multi-chamber expandable interspinous process brace **700** and the spinous processes **800**, **802**. Further, the ends **902**, **904** of the tether **900** can be brought together and one or more fasteners can be installed therethrough to connect the ends **902**, **904**. Accordingly, the tether **900** can be installed in order to prevent the distance between the spinous processes **800**, **802** from substantially increasing beyond the distance provided by the multi-chamber expandable interspinous process brace **700** after it is expanded and to maintain engagement of the interspinous processes with the spinous process pockets **710**, **712**, the engagement structures **720**, **722**, or a combination thereof.

[0077] In a particular embodiment, the tether **900** can comprise a biocompatible elastomeric material that flexes during installation and provides a resistance fit against the inferior

process. Further, the tether **900** can comprise a substantially non-resorbable suture or the like.

#### Description of a Third Embodiment of a Multi-Chamber Expandable Interspinous Process Brace

[0078] Referring to FIG. 10 through FIG. 12, a third embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated **1000**. As shown, the multi-chamber expandable interspinous process brace **1000** includes a central chamber **1002**, a superior chamber **1004**, and an inferior chamber **1006**.

[0079] In a particular embodiment, the central chamber **1002** can be generally horizontally elongated. Also, in a particular embodiment, the superior chamber **1004** can be shaped similar to the top half of a letter H and the inferior chamber **1006** can be shaped similar to the bottom half of a letter H. Together, the central chamber **1002**, the superior chamber **1004**, and the inferior chamber **1006** can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, together, the chambers **1002**, **1004** and **1006** can be generally H-shaped.

[0080] Further, in a particular embodiment, the chambers **1002**, **1004**, **1006** can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers **1002**, **1004**, **1006** can be non-porous or micro-porous, e.g., for venting purposes.

[0081] As shown in FIG. 10, the central chamber **1002** can include a first injection tube **1008**. The superior chamber **1004** can include a second injection tube **1010** and the inferior chamber **1006** can include a third injection tube **1012**. The injection tubes **1008**, **1010**, **1012** can be used to provide one or more injectable biocompatible material to the chambers **1002**, **1004**, **1006**. In a particular embodiment, each of the central chamber **1002**, the superior chamber **1004**, and the inferior chamber **1006** of the multi-chamber expandable interspinous process brace **1000** can be expanded from a respective deflated configuration, shown in FIG. 10, to one of a plurality of inflated configurations, shown in FIG. 11 and FIG. 12, up to a maximum inflated configuration. Further, after the chambers **1002**, **1004**, **1006** are inflated, or otherwise expanded, the injection tubes **1008**, **1010**, **1012** can be removed, as depicted in FIG. 12.

[0082] In a particular embodiment, the multi-chamber expandable interspinous process brace **1000** can include a first self-sealing valve (not shown) within the central chamber **1002**, e.g., adjacent to the first injection tube **1008**. Moreover, the multi-chamber expandable interspinous process brace **1000** can include a second self-sealing valve (not shown) within the superior chamber **1004**, e.g., adjacent to the second injection tube **1010**. The multi-chamber expandable interspinous process brace **1000** can also include a third self-sealing valve (not shown) within the inferior chamber **1006**. The self-sealing valves can prevent the chambers **1002**, **1004**, **1006** from leaking material after the chambers **1002**, **1004**, **1006** are inflated and the injection tubes **1008**, **1010**, **1012** are removed.

[0083] As illustrated in FIG. 10 through FIG. 12, the superior chamber **1004** can include a superior spinous process

pocket **1014** and the inferior chamber **1006** can include an inferior spinous process pocket **1016**. Further, a superior spinous process engagement structure **1020** can extend from the superior chamber **1004** within the superior spinous process pocket **1014**. Also, an inferior spinous process engagement structure **1022** can extend from the inferior chamber **1004** within the inferior spinous process pocket **1016**. In a particular embodiment, each of the spinous process engagement structures **1020**, **1022** can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

[0084] FIG. **10** through FIG. **12** indicate that the multi-chamber expandable interspinous process brace **1000** can be implanted between a superior spinous process **1100** and an inferior spinous process **1102**. In a particular embodiment, the chambers **1002**, **1004**, **1006** can be inflated so the superior chamber **1004** engages the superior spinous process **1100** and the inferior chamber **1006** engages the inferior spinous process **1102**. In a particular embodiment, when the multi-chamber expandable interspinous process brace **1000** is properly installed and inflated between the superior spinous process **1100** and the inferior spinous process **1102**, the superior spinous process pocket **1014** can engage and support the superior spinous process **1100**. Further, the inferior spinous process pocket **1016** can engage and support an inferior spinous process **1102**.

[0085] More specifically, the superior spinous process engagement structure **1020** can extend slightly into and engage the superior spinous process **1100**. Also, the inferior spinous process engagement structure **1022** can extend slightly into and engage the inferior spinous process **1102**. Accordingly, the spinous process engagement structures **1020**, **1022**, the spinous process pockets **1014**, **1016**, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace **1000** from migrating with respect to the spinous processes **1100**, **1102**.

[0086] Also, in a particular embodiment, the multi-chamber expandable interspinous process brace **1000** can be movable between a deflated configuration, shown in FIG. **10**, and one or more inflated configurations, shown in FIG. **11** and FIG. **12**. In the deflated configuration, a distance **1112** between the superior spinous process pocket **1014** and the inferior spinous process pocket **1016** can be at a minimum. However, as one or more materials are injected into the chambers **1002**, **1004**, **1006** the distance **1112** between the superior spinous process pocket **1014** and the inferior spinous process pocket **1016** can increase.

[0087] Accordingly, the multi-chamber expandable interspinous process brace **1000** can be installed between a superior spinous process **1100** and an inferior spinous process **1102**. Further, the multi-chamber expandable interspinous process brace **1000** can be expanded, e.g., by injecting one or more materials into the chambers **1002**, **1004**, **1006** in order to increase the distance between the superior spinous process **1100** and the inferior spinous process **1102**.

[0088] Alternatively, a distractor can be used to increase the distance between the superior spinous process **1100** and the inferior spinous process **1102** and the multi-chamber expandable interspinous process brace **1000** can be expanded to support the superior spinous process **1100** and the inferior spinous process **1102**. After the multi-chamber expandable interspinous process brace **1000** is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace **1000** can support the superior

spinous process **1100** and the inferior spinous process **1102** to substantially prevent the distance between the superior spinous process **1102** and the inferior spinous process **1100** from returning to a pre-distraction value.

[0089] In a particular embodiment, the multi-chamber expandable interspinous process brace **1000** can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0090] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylates, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluoropolyolefins.

[0091] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0092] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0093] In a particular embodiment, the hardness of the material used to inflate the central chamber **1002** can be less than or equal to the hardness of the material used to inflate the superior chamber **1004** and the inferior chamber **1006**, i.e., after the materials used to inflate the central chamber **1002**, the superior chamber **1004**, and the inferior chamber **1006** are cured. Alternatively, the viscosity of the material used to inflate the central chamber **1002** can be less than or equal to the viscosity of the material used to inflate the superior chamber **1004** and the inferior chamber **1006**. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0094] FIG. **12** indicates that a tether **1200** can be installed around the multi-chamber expandable interspinous process brace **1000**, after the multi-chamber expandable interspinous process brace **1000** is expanded as described herein. As shown, the tether **1200** can include a proximal end **1202** and a distal end **1204**. In a particular embodiment, the tether **1200** can circumscribe the multi-chamber expandable interspinous process brace **1000** and the spinous processes **1100**, **1102**. Further, the ends **1202**, **1204** of the tether **1200** can be brought together and one or more fasteners can be installed there-through to connect the ends **1202**, **1204**. Accordingly, the tether **1200** can be installed in order to prevent the distance between the spinous processes **1100**, **1102** from substantially increasing beyond the distance provided by the multi-chamber expandable interspinous process brace **1000** after it is expanded and to maintain engagement of the interspinous processes with the spinous process pockets **1014**, **1016**, engagement structures **1020**, **1022**, or a combination thereof.

[0095] In a particular embodiment, the tether **1200** can comprise a biocompatible elastomeric material that flexes during installation and provides a resistance fit against the

inferior process. Further, the tether **1200** can comprise a substantially non-resorbable suture or the like.

Description of a Fourth Embodiment of a  
Multi-Chamber Expandable Interspinous Process  
Brace

**[0096]** Referring to FIG. **13** through FIG. **15**, a fourth embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated **1300**. As shown, the multi-chamber expandable interspinous process brace **1300** includes a central chamber **1302**, a first lateral chamber **1304**, and a second lateral chamber **1306**.

**[0097]** In a particular embodiment, the central chamber **1302** can be generally vertically elongated. Also, in a particular embodiment, the first lateral chamber **1304** can be vertically elongated and can extend along a first side of the central chamber **1302**. The second lateral chamber **1306** can also be vertically elongated and can extend along a second side of the central chamber **1302**. As shown, the lateral chambers **1304**, **1306** can extend beyond a top and bottom of the central chamber **1302**. Together, the central chamber **1302**, the first lateral chamber **1304**, and the second lateral chamber **1306** can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, together, the chambers **1302**, **1304** and **1306** can be generally H-shaped.

**[0098]** Further, in a particular embodiment, the chambers **1302**, **1304**, **1306** can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers **1302**, **1304**, **1306** can be non-porous or micro-porous, e.g., for venting purposes.

**[0099]** As shown in FIG. **13**, the central chamber **1302** can include a first injection tube **1308**. The first lateral chamber **1304** can include a second injection tube **1310** and the second lateral chamber **1306** can include a third injection tube **1312**. The injection tubes **1308**, **1310**, **1312** can be used to provide one or more injectable biocompatible material to the chambers **1302**, **1304**, **1306**. In a particular embodiment, each of the central chamber **1302**, the first lateral chamber **1304**, and the second lateral chamber **1306** of the multi-chamber expandable interspinous process brace **1300** can be expanded from a respective deflated configuration, shown in FIG. **13**, to one of a plurality of inflated configurations, shown in FIG. **14** and FIG. **15**, up to a maximum inflated configuration. Further, after the chambers **1302**, **1304**, **1306** are inflated, or otherwise expanded, the injection tubes **1308**, **1310**, **1312** can be removed, as depicted in FIG. **15**.

**[0100]** In a particular embodiment, the multi-chamber expandable interspinous process brace **1300** can include a first self-sealing valve (not shown) within the central chamber **1302**, e.g., adjacent to the first injection tube **1308**. Moreover, the multi-chamber expandable interspinous process brace **1300** can include a second self-sealing valve (not shown) within the first lateral chamber **1304**, e.g., adjacent to the second injection tube **1310**. The multi-chamber expandable interspinous process brace **1300** can also include a third self-sealing valve (not shown) within the second lateral chamber **1306**. The self-sealing valves can prevent the chambers **1302**,

**1304**, **1306** from leaking material after the chambers **1302**, **1304**, **1306** are inflated and the injection tubes **1308**, **1310**, **1312** are removed.

**[0101]** As illustrated in FIG. **13** through FIG. **15**, the multi-chamber expandable interspinous process brace **1300** can include a superior spinous process pocket **1314** that is formed by a top portion of the central chamber **1302**, a top portion of the first lateral chamber **1304**, and a top portion of the second lateral chamber **1306**. The multi-chamber expandable interspinous process brace **1300** can also include an inferior spinous process pocket **1316** that can be formed by a bottom portion of the central chamber **1302**, a bottom portion of the first lateral chamber **1304**, and a bottom portion of the second lateral chamber **1306**.

**[0102]** Further, a superior spinous process engagement structure **1320** can extend from the central chamber **1304** within the superior spinous process pocket **1314**. Also, an inferior spinous process engagement structure **1322** can extend from the central chamber **1304** within the inferior spinous process pocket **1316**. In a particular embodiment, each of the spinous process engagement structures **1320**, **1322** can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

**[0103]** FIG. **13** through FIG. **15** indicate that the multi-chamber expandable interspinous process brace **1300** can be implanted between a superior spinous process **1400** and an inferior spinous process **1402**. In a particular embodiment, the chambers **1302**, **1304**, **1306** can be inflated so the superior spinous process pocket **1314** can engage and support the superior spinous process **1400** and so the inferior spinous process pocket **1316** can engage and support an inferior spinous process **1402**.

**[0104]** More specifically, the superior spinous process engagement structure **1320** can extend slightly into and engage the superior spinous process **1400**. Also, the inferior spinous process engagement structure **1322** can extend slightly into and engage the inferior spinous process **1402**. Accordingly, the spinous process engagement structures **1320**, **1322**, the spinous process pockets **1314**, **1316**, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace **1300** from migrating with respect to the spinous processes **1400**, **1402**.

**[0105]** Also, in a particular embodiment, the multi-chamber expandable interspinous process brace **1300** can be movable between a deflated configuration, shown in FIG. **13**, and one or more inflated configurations, shown in FIG. **14** and FIG. **15**. In the deflated configuration, a distance **1412** between the superior spinous process pocket **1314** and the inferior spinous process pocket **1316** can be at a minimum. However, as one or more materials are injected into the chambers **1302**, **1304**, **1306** the distance **1412** between the superior spinous process pocket **1314** and the inferior spinous process pocket **1316** can increase.

**[0106]** Accordingly, the multi-chamber expandable interspinous process brace **1300** can be installed between a superior spinous process **1400** and an inferior spinous process **1402**. Further, the multi-chamber expandable interspinous process brace **1300** can be expanded, e.g., by injecting one or more materials into the chambers **1302**, **1304**, **1306** in order to increase the distance between the superior spinous process **1400** and the inferior spinous process **1402**.

**[0107]** Alternatively, a distractor can be used to increase the distance between the superior spinous process **1400** and the

inferior spinous process **1402** and the multi-chamber expandable interspinous process brace **1300** can be expanded to support the superior spinous process **1400** and the inferior spinous process **1402**. After the multi-chamber expandable interspinous process brace **1300** is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace **1300** can support the superior spinous process **1400** and the inferior spinous process **1402** to substantially prevent the distance between the superior spinous process **1402** and the inferior spinous process **1400** from returning to a pre-distraction value.

[0108] In a particular embodiment, the multi-chamber expandable interspinous process brace **1300** can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0109] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylates, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluorepolyolefins.

[0110] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylacid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0111] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0112] In a particular embodiment, the hardness of the material used to inflate the central chamber **1302** can be less than or equal to the hardness of the material used to inflate the first lateral chamber **1304** and the second lateral chamber **1306**, i.e., after the materials used to inflate the central chamber **1302**, the first lateral chamber **1304**, and the second lateral chamber **1306** are cured. Alternatively, the viscosity of the material used to inflate the central chamber **1302** can be less than or equal to the viscosity of the material used to inflate the first lateral chamber **1304** and the second lateral chamber **1306**. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0113] FIG. 15 indicates that a tether **1500** can be installed around the multi-chamber expandable interspinous process brace **1300**, after the multi-chamber expandable interspinous process brace **1300** is expanded as described herein. As shown, the tether **1500** can include a proximal end **1502** and a distal end **1504**. In a particular embodiment, the tether **1500** can circumscribe the multi-chamber expandable interspinous process brace **1300** and the spinous processes **1400**, **1402**. Further, the ends **1502**, **1504** of the tether **1500** can be brought together and one or more fasteners can be installed there-through to connect the ends **1502**, **1504**. Accordingly, the tether **1500** can be installed in order to prevent the distance between the spinous processes **1400**, **1402** from substantially increasing beyond the distance provided by the multi-cham-

ber expandable interspinous process brace **1300** after it is expanded and to maintain engagement of the interspinous processes with the spinous process pockets **1314**, **1316**, engagement structures **1320**, **1322**, or a combination thereof. [0114] In a particular embodiment, the tether **1500** can comprise a biocompatible elastomeric material that flexes during installation and provides a resistance fit against the inferior process. Further, the tether **1500** can comprise a substantially non-resorbable suture or the like.

#### Description of a Fifth Embodiment of a Multi-Chamber Expandable Interspinous Process Brace

[0115] Referring to FIG. 16 through FIG. 18, a fifth embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated **1600**. As shown, the multi-chamber expandable interspinous process brace **1600** includes a central chamber **1602**, a first lateral chamber **1604**, and a second lateral chamber **1606**.

[0116] In a particular embodiment, the central chamber **1602** can be generally vertically elongated. Also, in a particular embodiment, the first lateral chamber **1604** can be vertically elongated and can extend along a first side of the central chamber **1602**. The second lateral chamber **1606** can also be vertically elongated and can extend along a second side of the central chamber **1602**. Together, the central chamber **1602**, the first lateral chamber **1604**, and the second lateral chamber **1606** can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, together, the chambers **1602**, **1604** and **1606** can be generally H-shaped.

[0117] Further, in a particular embodiment, the chambers **1602**, **1604**, **1606** can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers **1602**, **1604**, **1606** can be non-porous or micro-porous, e.g., for venting purposes.

[0118] As shown in FIG. 16, the central chamber **1602** can include a first injection tube **1608**. The first lateral chamber **1604** can include a second injection tube **1610** and the second lateral chamber **1606** can include a third injection tube **1612**. The injection tubes **1608**, **1610**, **1612** can be used to provide one or more injectable biocompatible material to the chambers **1602**, **1604**, **1606**. In a particular embodiment, each of the central chamber **1602**, the first lateral chamber **1604**, and the second lateral chamber **1606** of the multi-chamber expandable interspinous process brace **1600** can be expanded from a respective deflated configuration, shown in FIG. 16, to one of a plurality of inflated configurations, shown in FIG. 17 and FIG. 18, up to a maximum inflated configuration. Further, after the chambers **1602**, **1604**, **1606** are inflated, or otherwise expanded, the injection tubes **1608**, **1610**, **1612** can be removed, as depicted in FIG. 18.

[0119] In a particular embodiment, the multi-chamber expandable interspinous process brace **1600** can include a first self-sealing valve (not shown) within the central chamber **1602**, e.g., adjacent to the first injection tube **1608**. Moreover, the multi-chamber expandable interspinous process brace **1600** can include a second self-sealing valve (not shown) within the first lateral chamber **1604**, e.g., adjacent to the second injection tube **1610**. The multi-chamber expandable

interspinous process brace **1600** can also include a third self-sealing valve (not shown) within the second lateral chamber **1606**. The self-sealing valves can prevent the chambers **1602**, **1604**, **1606** from leaking material after the chambers **1602**, **1604**, **1606** are inflated and the injection tubes **1608**, **1610**, **1612** are removed.

[0120] As illustrated in FIG. **16** through FIG. **18**, central chamber **1602** of the multi-chamber expandable interspinous process brace **1600** can include a superior spinous process pocket **1614**. The central chamber **1602** of the multi-chamber expandable interspinous process brace **1600** can also include an inferior spinous process pocket **1616**. Further, a superior spinous process engagement structure **1620** can extend from the central chamber **1604** within the superior spinous process pocket **1614**. Also, an inferior spinous process engagement structure **1622** can extend from the central chamber **1604** within the inferior spinous process pocket **1616**. In a particular embodiment, each of the spinous process engagement structures **1620**, **1622** can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

[0121] FIG. **16** through FIG. **18** indicate that the multi-chamber expandable interspinous process brace **1600** can be implanted between a superior spinous process **1700** and an inferior spinous process **1702**. In a particular embodiment, the chambers **1602**, **1604**, **1606** can be inflated so the superior spinous process pocket **1614** can engage and support the superior spinous process **1700** and so the inferior spinous process pocket **1616** can engage and support an inferior spinous process **1702**.

[0122] More specifically, the superior spinous process engagement structure **1620** can extend slightly into and engage the superior spinous process **1700**. Also, the inferior spinous process engagement structure **1622** can extend slightly into and engage the inferior spinous process **1702**. Accordingly, the spinous process engagement structures **1620**, **1622**, the spinous process pockets **1614**, **1616**, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace **1600** from migrating with respect to the spinous processes **1700**, **1702**.

[0123] Also, in a particular embodiment, the multi-chamber expandable interspinous process brace **1600** can be movable between a deflated configuration, shown in FIG. **16**, and one or more inflated configurations, shown in FIG. **17** and FIG. **18**. In the deflated configuration, a distance **1712** between the superior spinous process pocket **1614** and the inferior spinous process pocket **1616** can be at a minimum. However, as one or more materials are injected into the chambers **1602**, **1604**, **1606** the distance **1712** between the superior spinous process pocket **1614** and the inferior spinous process pocket **1616** can increase.

[0124] Accordingly, the multi-chamber expandable interspinous process brace **1600** can be installed between a superior spinous process **1700** and an inferior spinous process **1702**. Further, the multi-chamber expandable interspinous process brace **1600** can be expanded, e.g., by injecting one or more materials into the chambers **1602**, **1604**, **1606** in order to increase the distance between the superior spinous process **1700** and the inferior spinous process **1702**.

[0125] Alternatively, a distractor can be used to increase the distance between the superior spinous process **1700** and the inferior spinous process **1702** and the multi-chamber expandable interspinous process brace **1600** can be expanded to support the superior spinous process **1700** and the inferior

spinous process **1702**. After the multi-chamber expandable interspinous process brace **1600** is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace **1600** can support the superior spinous process **1700** and the inferior spinous process **1702** to substantially prevent the distance between the superior spinous process **1702** and the inferior spinous process **1700** from returning to a pre-distraction value.

[0126] In a particular embodiment, the multi-chamber expandable interspinous process brace **1600** can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0127] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylates, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluoropolyolefins.

[0128] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylacid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0129] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0130] In a particular embodiment, the hardness of the material used to inflate the central chamber **1602** can be less than or equal to the hardness of the material used to inflate the first lateral chamber **1604** and the second lateral chamber **1606**, i.e., after the materials used to inflate the central chamber **1602**, the first lateral chamber **1604**, and the second lateral chamber **1606** are cured. Alternatively, the viscosity of the material used to inflate the central chamber **1602** can be less than or equal to the viscosity of the material used to inflate the first lateral chamber **1604** and the second lateral chamber **1606**. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0131] FIG. **18** indicates that a tether **1800** can be installed around the multi-chamber expandable interspinous process brace **1600**, after the multi-chamber expandable interspinous process brace **1600** is expanded as described herein. As shown, the tether **1800** can include a proximal end **1802** and a distal end **1804**. In a particular embodiment, the tether **1800** can circumscribe the multi-chamber expandable interspinous process brace **1600** and the spinous processes **1700**, **1702**. Further, the ends **1802**, **1804** of the tether **1800** can be brought together and one or more fasteners can be installed there-through to connect the ends **1802**, **1804**. Accordingly, the tether **1800** can be installed in order to prevent the distance between the spinous processes **1700**, **1702** from substantially increasing beyond the distance provided by the multi-chamber expandable interspinous process brace **1600** after it is expanded and to maintain engagement of the interspinous



processes with the spinous process pockets **1614**, **1616**, engagement structures **1620**, **1622**, or a combination thereof. **[0132]** In a particular embodiment, the tether **1800** can comprise a biocompatible elastomeric material that flexes during installation and provides a resistance fit against the inferior process. Further, the tether **1800** can comprise a substantially non-resorbable suture or the like.

Description of a Sixth Embodiment of a  
Multi-Chamber Expandable Interspinous Process  
Brace

**[0133]** Referring to FIG. **19** through FIG. **21**, a sixth embodiment of a multi-chamber expandable interspinous process brace is shown and is generally designated **1900**. As shown, the multi-chamber expandable interspinous process brace **1900** includes an exterior chamber **1902**, a first interior chamber **1904**, and a second interior chamber **1906**.

**[0134]** In a particular embodiment, the exterior chamber **1902** can be provided in a shape that can generally engage and/or stabilize at least one spinous process, such as, for example, the spinous processes of two adjacent vertebrae. In a particular embodiment, the exterior chamber **1902** can be generally H-shaped. Also, in a particular embodiment, the first interior chamber **1904** can be vertically elongated and can be disposed within a first side of the exterior chamber **1902**. The second interior chamber **1906** can also be vertically elongated and can be disposed within a second side of the exterior chamber **1902**.

**[0135]** Further, in a particular embodiment, the chambers **1902**, **1904**, **1906** can be made from one or more expandable biocompatible materials. For example, the materials can be silicones, polyurethanes, polycarbonate urethanes, polyethylene terephthalate, silicone copolymers, polyolefins, or any combination thereof. Also, the chambers **1902**, **1904**, **1906** can be non-porous or micro-porous, e.g., for venting purposes.

**[0136]** As shown in FIG. **19**, the exterior chamber **1902** can include a first injection tube **1908**. The first interior chamber **1904** can include a second injection tube **1910** and the second interior chamber **1906** can include a third injection tube **1912**. The injection tubes **1908**, **1910**, **1912** can be used to provide one or more injectable biocompatible material to the chambers **1902**, **1904**, **1906**. In a particular embodiment, each of the exterior chamber **1902**, the first interior chamber **1904**, and the second interior chamber **1906** of the multi-chamber expandable interspinous process brace **1900** can be expanded from a respective deflated configuration, shown in FIG. **19**, to one of a plurality of inflated configurations, shown in FIG. **20** and FIG. **21**, up to a maximum inflated configuration. Further, after the chambers **1902**, **1904**, **1906** are inflated, or otherwise expanded, the injection tubes **1908**, **1910**, **1912** can be removed, as depicted in FIG. **21**.

**[0137]** In a particular embodiment, the multi-chamber expandable interspinous process brace **1900** can include a first self-sealing valve (not shown) within the exterior chamber **1902**, e.g., adjacent to the first injection tube **1908**. Moreover, the multi-chamber expandable interspinous process brace **1900** can include a second self-sealing valve (not shown) within the first interior chamber **1904**, e.g., adjacent to the second injection tube **1910**. The multi-chamber expandable interspinous process brace **1900** can also include a third self-sealing valve (not shown) within the second interior chamber **1906**. The self-sealing valves can prevent the chambers **1902**, **1904**, **1906** from leaking material after the

chambers **1902**, **1904**, **1906** are inflated and the injection tubes **1908**, **1910**, **1912** are removed.

**[0138]** As illustrated in FIG. **19** through FIG. **21**, exterior chamber **1902** of the multi-chamber expandable interspinous process brace **1900** can include a superior spinous process pocket **1914**. The exterior chamber **1902** of the multi-chamber expandable interspinous process brace **1900** can also include an inferior spinous process pocket **1916**. Further, a superior spinous process engagement structure **1922** can extend from the exterior chamber **1902** within the superior spinous process pocket **1914**. Also, an inferior spinous process engagement structure **1920** can extend from the exterior chamber **1902** within the inferior spinous process pocket **1916**. In a particular embodiment, each of the spinous process engagement structures **1920**, **1922** can be one or more spikes, one or more teeth, a combination thereof, or some other structure configured to engage a spinous process.

**[0139]** FIG. **19** through FIG. **21** indicate that the multi-chamber expandable interspinous process brace **1900** can be implanted between a superior spinous process **2000** and an inferior spinous process **2002**. In a particular embodiment, the chambers **1902**, **1904**, **1906** can be inflated so the superior spinous process pocket **1914** can engage and support the superior spinous process **2000** and so the inferior spinous process pocket **1916** can engage and support an inferior spinous process **2002**.

**[0140]** More specifically, the superior spinous process engagement structure **1922** can extend slightly into and engage the superior spinous process **2000**. Also, the inferior spinous process engagement structure **1920** can extend slightly into and engage the inferior spinous process **2002**. Accordingly, the spinous process engagement structures **1920**, **1922**, the spinous process pockets **1914**, **1916**, or a combination thereof can substantially prevent the multi-chamber expandable interspinous process brace **1900** from migrating with respect to the spinous processes **2000**, **2002**.

**[0141]** Also, in a particular embodiment, the multi-chamber expandable interspinous process brace **1900** can be movable between a deflated configuration, shown in FIG. **19**, and one or more inflated configurations, shown in FIG. **20** and FIG. **21**. In the deflated configuration, a distance **2012** between the superior spinous process pocket **1914** and the inferior spinous process pocket **1916** can be at a minimum. However, as one or more materials are injected into the chambers **1902**, **1904**, **1906** the distance **2012** between the superior spinous process pocket **1914** and the inferior spinous process pocket **1916** can increase.

**[0142]** Accordingly, the multi-chamber expandable interspinous process brace **1900** can be installed between a superior spinous process **2000** and an inferior spinous process **2002**. Further, the multi-chamber expandable interspinous process brace **1900** can be expanded, e.g., by injecting one or more materials into the chambers **1902**, **1904**, **1906** in order to increase the distance between the superior spinous process **2000** and the inferior spinous process **2002**.

**[0143]** Alternatively, a distractor can be used to increase the distance between the superior spinous process **2000** and the inferior spinous process **2002** and the multi-chamber expandable interspinous process brace **1900** can be expanded to support the superior spinous process **2000** and the inferior spinous process **2002**. After the multi-chamber expandable interspinous process brace **1900** is expanded accordingly, the distractor can be removed and the multi-chamber expandable interspinous process brace **1900** can support the superior

spinous process **2000** and the inferior spinous process **2002** to substantially prevent the distance between the superior spinous process **2002** and the inferior spinous process **2000** from returning to a pre-distraction value.

[0144] In a particular embodiment, the multi-chamber expandable interspinous process brace **1900** can be injected with one or more injectable biocompatible materials that remain elastic after curing. Further, the injectable biocompatible materials can include polymer materials that remain elastic after curing. Also, the injectable biocompatible materials can include ceramics.

[0145] For example, the polymer materials can include polyurethanes, polyolefins, silicones, silicone polyurethane copolymers, polymethylmethacrylate (PMMA), epoxies, cyanoacrylates, hydrogels, or a combination thereof. Further, the polyolefin materials can include polypropylenes, polyethylenes, halogenated polyolefins, or fluoropolyolefins.

[0146] The hydrogels can include polyacrylamide (PAAM), poly-N-isopropylacrylamine (PNIPAM), polyvinyl methylether (PVM), polyvinyl alcohol (PVA), polyethyl hydroxyethyl cellulose, poly(2-ethyl)oxazoline, polyethyleneoxide (PEO), polyethylglycol (PEG), polyacrylacid (PAA), polyacrylonitrile (PAN), polyvinylacrylate (PVA), polyvinylpyrrolidone (PVP), or a combination thereof.

[0147] In a particular embodiment, the ceramics can include calcium phosphate, hydroxyapatite, calcium sulfate, bioactive glass, or a combination thereof. In an alternative embodiment, the injectable biocompatible materials can include one or more fluids such as sterile water, saline, or sterile air.

[0148] In a particular embodiment, the hardness of the material used to inflate the exterior chamber **1902** can be less than or equal to the hardness of the material used to inflate the first interior chamber **1904** and the second interior chamber **1906**, i.e., after the materials used to inflate the exterior chamber **1902**, the first interior chamber **1904**, and the second interior chamber **1906** are cured. Alternatively, the viscosity of the material used to inflate the exterior chamber **1902** can be less than or equal to the viscosity of the material used to inflate the first interior chamber **1904** and the second interior chamber **1906**. In a particular embodiment, certain or all of the injected materials can be cured or cross-linked in situ to form a solid interspinous process brace with non-uniform bulk properties.

[0149] FIG. 21 indicates that a tether **2100** can be installed around the multi-chamber expandable interspinous process brace **1900**, after the multi-chamber expandable interspinous process brace **1900** is expanded as described herein. As shown, the tether **2100** can include a proximal end **2102** and a distal end **2104**. In a particular embodiment, the tether **2100** can circumscribe the multi-chamber expandable interspinous process brace **1900** and the spinous processes **2000**, **2002**. Further, the ends **2102**, **2104** of the tether **2100** can be brought together and one or more fasteners can be installed there-through to connect the ends **2102**, **2104**. Accordingly, the tether **2100** can be installed in order to prevent the distance between the spinous processes **2000**, **2002** from substantially increasing beyond the distance provided by the multi-chamber expandable interspinous process brace **1900** after it is expanded and to maintain engagement of the interspinous processes with the spinous process pockets **1914**, **1916**, engagement structures **1920**, **1922**, or a combination thereof.

[0150] In a particular embodiment, the tether **2100** can comprise a biocompatible elastomeric material that flexes

during installation and provides a resistance fit against the inferior process. Further, the tether **2100** can comprise a substantially non-resorbable suture or the like.

[0151] Description of a Method of Treating a Spine

[0152] Referring to FIG. 22, a method of treating a spine is shown and commences at block **2200**. At block **2200**, a patient can be secured on an operating table. Depending on the surgical approach to be used, the patient can be secured in a prone position for a posterior approach, a supine position for an anterior approach, a lateral decubitus position for a lateral approach, or another position well known in the art. At block **2202**, the spine can be exposed in order to expose adjacent spinous processes. Further, at block **2204**, a surgical retractor system can be installed to keep a surgical field open.

[0153] Moving to block **2206**, a superior vertebra and inferior vertebra can be distracted. In a particular embodiment, the superior vertebra and inferior vertebra can be distracted using a distractor. At block **2208**, a distance between the adjacent spinous processes can be measured. Thereafter, at block **2210** it is determined whether the distraction is correct, e.g., has the superior vertebra and inferior vertebral been distracted such that a distance between the adjacent spinous processes has reached a value that a surgeon has deemed therapeutic. For example, the superior vertebra and inferior vertebra can be distracted in order to reduce impingement on a nerve root.

[0154] If the distraction is not correct, the method can return to block **2206** and the superior vertebra and inferior vertebra can be further distracted. Conversely, if the distraction is correct, the method can move to block **2212** and a multi-chamber expandable interspinous process brace can be installed between a superior spinous process and an inferior spinous process. Thereafter, at block **2214**, each chamber within the multi-chamber expandable interspinous process brace can be inflated.

[0155] Moving to block **2216**, each chamber within the multi-chamber expandable interspinous process brace can be sealed. In a particular embodiment, each chamber within the multi-chamber expandable interspinous process brace can be sealed by curing the material within the each chamber of the multi-chamber expandable interspinous process brace. Alternatively, a plug, a dowel, or another similar device can be used to seal each chamber within the multi-chamber expandable interspinous process brace. Further, a one-way valve can be incorporated into each chamber of the multi-chamber expandable interspinous process brace and can allow material to be injected into each chamber of the multi-chamber expandable interspinous process brace, but prevent the same material from being expelled from each chamber of the multi-chamber expandable interspinous process brace.

[0156] At block **2218**, each injection tube can be removed from the multi-chamber expandable interspinous process brace. Moreover, at block **2220**, the material within one or more chambers of the multi-chamber expandable interspinous process brace can be cured. In a particular embodiment, the material within the multi-chamber expandable interspinous process brace can cure naturally, i.e., under ambient conditions, in situ. Alternatively, the material within one or more of the multi-chamber expandable interspinous process brace can be cured or crosslinked in situ using an energy source. For example, the energy source can be a light source that emits visible light, infrared (IR) light, or ultraviolet (UV) light. Further, the energy source can be a heating device, a radiation device, or other mechanical device. Alter-

natively or in addition, the material in one or more of the chambers can be crosslinked by introducing a chemical crosslinking agent into the chamber before removing the injection tube from the chamber.

[0157] Proceeding to block 2222, a tether can be installed around the multi-chamber expandable interspinous process brace. The tether can be installed in order to prevent a distance between the superior spinous process and the inferior spinous process from increasing substantially beyond the distance provided by the multi-chamber expandable interspinous process brace. At block 2224, the surgical area can be irrigated. At block 2226, the distractor can be removed. Also, at block 2228, the retractor system can be removed. Further, at block 2230, the surgical wound can be closed. The surgical wound can be closed by simply allowing the patient's skin to close due to the elasticity of the skin. Alternatively, the surgical wound can be closed using sutures, surgical staples, or any other suitable surgical technique well known in the art. At block 2232, postoperative care can be initiated. The method can end at state 2232.

CONCLUSION

[0158] With the configuration of structure described above, the multi-chamber expandable interspinous process brace provides a device that can be used to treat a spine and substantially alleviate or minimize one or more symptoms associated with disc degeneration, facet joint degeneration, or a combination thereof. For example, the multi-chamber expandable interspinous process brace can be installed between adjacent spinous processes in order to support the spinous processes and maintain them at or near a predetermined distance therebetween.

[0159] As described above, the multi-chamber expandable interspinous process brace can include two or three chambers. Alternatively, the multi-chamber expandable interspinous process brace can include four chambers, five chambers, six chambers, seven chambers, eight chambers, nine chambers, ten chambers, etc. Also, the chambers can be separate chambers, as described above, or the chambers can be interconnected to allow material to flow therebetween. The chambers can be inflated sequentially or simultaneously.

What is claimed is:

- 1. An expandable interspinous process spacer comprising:
  - an outer chamber formed of an expandable material, the outer chamber having a generally H-shape in both a relatively smaller deflated configuration and a relatively larger inflated configuration;
  - an inner expandable chamber disposed within and generally surrounded by the outer chamber;
  - the outer chamber being changeable from the relatively smaller deflated configuration to the relatively larger inflated configuration via injection of a first biocompatible material;
  - the inner chamber changeable from a relatively smaller deflated configuration to a relatively larger inflated configuration via injection of a second biocompatible material; the inner chamber changeable from the deflated configuration to the inflated configuration independently of the outer chamber.
- 2. The expandable spacer of claim 1 wherein the H-shape of the outer chamber forms first and second spinous process-receiving notches, oriented in generally opposite directions.
- 3. The expandable spacer of claim 1 further comprising the first biocompatible material disposed in the outer chamber

and the second biocompatible material disposed in the inner chamber; wherein the first and second biocompatible materials are different.

4. The expandable spacer of claim 3 wherein the first biocompatible material is harder than the second biocompatible material.

5. The expandable spacer of claim 4 wherein the first biocompatible material in the outer chamber has a higher degree of cross-linking than the second biocompatible material in the inner chamber.

6. The expandable spacer of claim 3 wherein the first biocompatible material comprises at least one of a polymer and a ceramic.

7. The expandable spacer of claim 1 further comprising a first injection tube operatively connected to the outer chamber and a second injection tube operatively connected to the inner chamber.

8. The expandable spacer of claim 7 further comprising a self-sealing valve operatively disposed between the second injection tube and the inner chamber.

9. The expandable spacer of claim 1 further comprising a tether having a length sufficient to wrap around an exterior of the outer chamber when the outer chamber is in the inflated configuration.

10. The expandable spacer of claim 1 wherein the second biocompatible material comprises a fluid.

11. An interspinous process spacer comprising:

an outer chamber formed of an expandable material, the outer chamber having a generally H-shape in both a relatively smaller deflated configuration and a relatively larger inflated configuration;

a first biocompatible material disposed in the outer chamber, wherein injection of the first biocompatible material causes expansion of the outer chamber from the first relatively smaller deflated configuration to the second relatively larger inflated configuration;

an inner expandable chamber disposed within and generally surrounded by the outer chamber, the inner chamber having a generally H-shape in both a relatively smaller deflated configuration and a relatively larger inflated configuration;

a second biocompatible material disposed in the inner chamber; wherein injection of the second biocompatible material causes expansion of the inner chamber from the first relatively smaller deflated configuration to the second relatively larger inflated configuration;

wherein the inner chamber is changeable from the deflated configuration to the inflated configuration independently of the outer chamber;

wherein the first biocompatible material and the second biocompatible material have at least one different material property such that the first biocompatible material has greater hardness than the second biocompatible material.

12. The spacer of claim 11 wherein the first and second biocompatible materials are the same during injection, with the at least one different material property being degree of cross-linking after curing.

13. The spacer of claim 11 further comprising a first injection tube operatively connected to the outer chamber and a second injection tube operatively connected to the inner chamber.