



- (51) International Patent Classification:
A61H 31/00 (2006.01) *A62B 33/00* (2006.01)
- (21) International Application Number:
PCT/US2013/057020
- (22) International Filing Date:
28 August 2013 (28.08.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
13/597,099 28 August 2012 (28.08.2012) US
- (71) Applicant: **ZOLL MEDICAL CORPORATION**
[US/US]; 269 Mill Road, Chelmsford, MA 01824 (US).
- (72) Inventor: **JOHNSON, Guy, R.**; 269 Mill Road, Chelmsford, MA 01824 (US).
- (74) Agent: **BACKOFEN, Paul, J.**; Crockett & Crockett, PC, 26020 Acero, Suite 200, Mission Viejo, CA 92691 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: METHOD AND APPARATUS FOR IMMOBILIZING SUBJECTS UNDERGOING MECHANICAL CPR

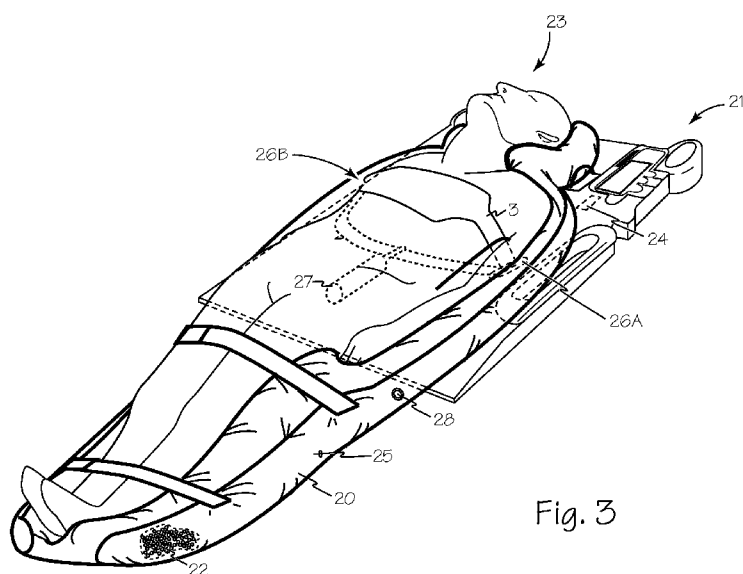


Fig. 3

(57) Abstract: The apparatus for immobilizing and treating a subject includes a suitable apparatus for performing mechanical CPR secured to an immobilization casing. The airtight flexible casing is secured to the apparatus for performing CPR, the casing having variable rigidity which varies as a function of the amount of air within the casing. Two or more slots through the casing permit passage of one or more elements of the CPR apparatus to pass through the casing. One or more incompressible windows may be included in the casing to optimize the performance of mechanical CPR by permitting one or more elements of the subject's skeleton to contact the CPR apparatus. A means for evacuating the air from within the flexible casing to control the rigidity of the casing is included within the CPR apparatus.

Method and Apparatus for Immobilizing Subjects Undergoing
Mechanical CPR

Field of the Inventions

[0001] The inventions described below relate to the field of CPR chest compression devices.

Background

[0002] Cardiopulmonary resuscitation (CPR) is a well-known and valuable method of first aid used to resuscitate people who have suffered from cardiac arrest. CPR requires repetitive chest compressions to squeeze the heart and the thoracic cavity to pump blood through the body. Artificial respiration, such as mouth-to-mouth breathing or a bag mask apparatus, is used to supply air to the lungs. When a first aid provider performs manual chest compression effectively, blood flow in the body is about 25% to 30% of normal blood flow.

[0003] In efforts to provide better blood flow and increase the effectiveness of bystander resuscitation efforts, various mechanical devices have been proposed for performing CPR. In one variation of such devices, a belt is placed around the subject's chest and the belt is used to effect chest compressions. Our own patents, Mollenauer et al., Resuscitation device having a motor driven belt to constrict/compress the chest, U.S. Patent 6,142,962 (Nov. 7, 2000); Sherman, et al., CPR Assist Device with Pressure Bladder Feedback, U.S. Patent 6,616,620 (Sep. 9, 2003); Sherman et al., Modular CPR assist device, U.S. Patent 6,066,106 (May 23, 2000); and Sherman et al., Modular CPR assist device, U.S. Patent 6,398,745 (Jun. 4, 2002), and Escudero, et al., Compression Belt System for Use with Chest

Compression Devices, U.S. Patent 7,410,470 (Aug. 12, 2008), show chest compression devices that compress a subject's chest with a belt. Our commercial device, sold under the trademark AUTOPULSE®, is described in some detail in our prior patents, including Jensen, Lightweight Electro-Mechanical Chest Compression Device, U.S. Patent 7,347,832 (March 25, 2008) and Quintana, et al., Methods and Devices for Attaching a Belt Cartridge to a Chest Compression Device, U.S. Patent 7,354,407 (April 8, 2008). Each of these patents is hereby incorporated by reference in their entirety.

[0004] In some scenarios in which CPR is required to treat cardiac arrest, is it also necessary to immobilize the subject. The subject may have coincident injuries, such as a broken vertebrae or broken hip, that require immobilization. The subject may need to be transported over rugged terrain, up or down stairs, or in sitting or upright positions. In these scenarios, it would be beneficial to provide automated CPR chest compressions while also immobilizing the subject. However, conventional immobilization devices do not work well with available chest compression devices. The components of each device interfere to the extent that they cannot be combined effectively. One example of a desirable immobilization device is illustrated in Koledin, Vacuum Immobilizer Support, U.S. Patent 5,121,756 (Jun.16, 1992) and Latimer et al., Air Evacuatable Support, U.S. Patent 5,154,185 (Oct. 13, 1992) both of which are hereby incorporated by reference in their entirety. These devices comprise bead filled mattresses which, when filled with beads and air, conform to the subject's shape. After placing the subject on the mattress, and allowing the mattress to conform to the subject, the mattress may be evacuated to lock the beads in place and transform the mattress into a rigid backboard which immobilizes the subject.

Summary

[0005] The devices and methods described below provide for subject immobilization and simultaneous performance of mechanical CPR. The belt drive platform operates as a generally rigid base that includes all the necessary mechanisms for performing mechanical CPR. The front surface of the platform incorporates an airtight flexible casing partially filled with beads, pellets or other suitable media (or movable discrete elements, in the terminology used in U.S. Patent 5,154,185). When the casing contains enough air to be at or near ambient atmospheric pressure, the casing is flexible and the beads are loose and free to move within the casing or within portions of the casing and conform, or be made to conform, to the shape of the subject lying on the casing. As the air within the casing is evacuated, the beads are forced together into a generally rigid form that has conformed to the subject's body and immobilizes the subject. Slots through the casing enable the ends of the belt for performing mechanical CPR to pass through the casing and encircle the subject's thorax for performance of mechanical CPR. One or more windows in the casing enable skeletal elements of the subject to make contact with the belt drive platform to optimize the resuscitative work of the platform and belt and not waste energy compressing the beads.

[0006] A suitable belt drive system includes a belt drive platform that includes a housing and a drive spool operably attached to the housing as well as a means for rotating the drive spool, with the means for rotating disposed within the housing and operably attached to the drive spool. A compression belt cartridge engages the belt drive platform. The compression belt cartridge including the belt suitable for compressing the chest of the subject and a spline attached to the belt, wherein the spline is removably attachable to the

drive spool, wherein rotation of the drive spool tightens the belt to compress the chest. An airtight flexible casing is secured to the housing, the casing having variable rigidity which varies as a function of the amount of air within the casing. The casing also includes two or more slots to permit passage of the belt from the drive belt platform to engage the thorax of the subject. A means for evacuating the air from within the flexible casing to control the rigidity of the casing is included within the housing. A plurality of beads are located within the casing, the plurality of beads adapted to move and conform the casing to support the subject to be immobilized when the casing is inflated, the plurality of beads adapted to be rigidly fixed in position when the casing is in a fully evacuated state.

[0007] A method for immobilizing and treating a subject requiring CPR includes the steps of providing a mechanical chest compression apparatus and providing an airtight flexible casing secured to the mechanical chest compression apparatus, the casing containing a plurality of beads wherein the beads provide variable rigidity which varies as a function of the amount of air within the casing and providing a vacuum pump for evacuating the air from within the flexible casing to control the rigidity of the casing. A subject requiring CPR is placed on the casing and the beads are arranged to support and immobilize the subject. The subject is secured to the mechanical chest compression apparatus and the air from within the casing is evacuated by the vacuum pump to rigidly compresses plurality of beads and immobilize the subject. The mechanical chest compression apparatus is then activated to repetitively perform chest compressions.

[0008] A method for immobilizing and treating a subject requiring CPR includes the steps of providing a mechanical chest compression apparatus and providing an airtight flexible casing secured to the mechanical chest compression apparatus,

the casing having at least two independently operable portions, each portion containing a plurality of beads wherein the beads provide variable rigidity which varies as a function of the amount of air within the casing and providing a vacuum pump for evacuating the air from within the independently operable portions of the casing to control the rigidity of the portions of the casing. A subject requiring CPR is placed on the casing and the beads in each portion are arranged to support and immobilize the subject. The subject is secured to the mechanical chest compression apparatus and the air from within one or more portions of the casing is evacuated by the vacuum pump to rigidly compresses plurality of beads in the evacuated portions and immobilize the subject. The mechanical chest compression apparatus is then activated to repetitively perform chest compressions.

Brief Description of the Drawings

[0009] Figure 1 shows a prior art chest compression belt fitted on a subject.

[0010] Figure 2 is a schematic cross section of the chest compression device of Figure 1.

[0011] Figure 3 is a perspective view of a subject immobilized in a full length immobilization casing while also disposed within an automated chest compression device.

[0012] Figure 4 is a perspective view of a subject immobilized in an upper body immobilization casing while also disposed within an automated chest compression device.

[0013] Figure 5 is a side view of the subject and apparatus of Figure 4.

[0014] Figure 6 is a top view of the automatic chest compression device of Figure 4.

[0015] Figure 7 is a cross-section view of the apparatus of Figure 6 taken along A-A.

[0016] Figure 8 is a side view of the apparatus of Figure 6.

[0017] Figure 9 is a top view of the automatic chest compression device with a full size immobilizer casing.

[0018] Figure 10 is a side view of the apparatus of Figure 9.

[0019] Figure 11 is a perspective view of a subject immobilized in a full length immobilization casing while also disposed within an automated chest compression device.

Detailed Description of the Inventions

[0020] The apparatus for immobilizing and treating a subject includes a suitable means for mechanically compressing the chest of a subject such as a belt drive compression system, a piston compression system or a vest compression system. A suitable belt drive compression system, similar to the AutoPulse® CPR chest compression device, is illustrated in Figures 1 and 2 fitted on a subject 1. Chest compression device 2 applies compressions with the belt 3, which has a right belt portion 3R and a left belt portion 3L, including load distributing panels 4R and 4L designed for placement over the anterior surface of the subject's chest while in use, and tensioning portions which extend from the load distributing portions to a drive spool, shown in the illustration as narrow pull straps 5R and 5L. (The entirety of the compression belt is referred to as a "load distributing band" in the art.) The right belt portion and left belt portion are secured to each other with hook and loop fasteners and aligned with the eyelet 6 and protrusion 7. A bladder 8 is disposed between the belt and the chest of the subject. The narrow pull straps 5R and

5L of the belt are spooled onto a drive spool located within the platform (shown in Figure 2) to tighten the belt during use, passing first over laterally located spindles 9L and 9R. The chest compression device 2 includes a belt drive platform 10 and a compression belt cartridge 11 (which includes the belt). The platform includes a housing 12 upon which the subject rests. Means for tightening the belt, a processor and a user interface are disposed within the housing. In the commercial embodiment of the device, the means for tightening the belt includes a motor, a drive train (clutch, brake and/or gear box) and a drive spool upon which the belt spools during use.

[0021] Figure 2 is a schematic cross section of the device of Figure 1, installed on a subject 1. The components include the compression belt 3L and 3R, the load distribution portions of the belt 4L and 4R, the narrow strap portions 5L and 5R, the bladder 8, the spindles 9L and 9R. The drive spool 13 and the spline 14 which fixes the belt to the drive spool are located within the housing 12, as is a motor and computer control system which operate to drive the drive spool to spool the belt, thereby tightening the belt about the chest and thorax of the subject and a resuscitative rate to accomplish CPR. A load plate 15 is disposed on the platform (the upper surface of the housing). The anatomical landmarks shown in this Figure include the sternum 16, the spine 17, and the right and left scapula 18R and 18L of the subject. Referring to the landmarks, the chest compression band is wrapped around the subject such that the load distributing portions are located on the chest (that is, the anterior surface or portion of the thorax), over the sternum, with the narrow strap portions descending from the load distributing portions to wrap around the lateral spindles and thence run to the drive spool. The lateral spindles are spaced laterally from the medial centerline of the device so that they are disposed

under, or lateral to, the scapulae of the typical subject, so that tightening of the compression band results in anterior/posterior compression of the chest.

[0022] Our experience with mechanical chest compression suggests that the subject must remain in a fixed position relative to the housing: That is, some anatomical parts of the subject must remain in substantially fixed relation to the housing while the sternum is compressed toward the spine. Various other mechanisms or means for chest compression may be used to perform mechanical CPR such as the LUCAS™ chest compression system produced by Physio-Control, Inc. as well as the mechanisms shown in Lach et al., Resuscitation Method and Apparatus, U.S. Patent 4,774,160 (Sep. 13, 1988) and in Kelly et al., Chest Compression Apparatus for Cardiac Arrest, U.S. Patent 5,738,637 (Apr. 14, 1998). The entirety of these patents is hereby incorporated by reference.

[0023] Referring now to Figure 3, an immobilization casing such as full length flexible casing 1920 may be secured to a suitable automated chest compression apparatus such as chest compression device 21. Full length flexible casing 20 may be partially filled with beads 22 to support and immobilize subject 23 as shown in Koledin, Vacuum Immobilizer Support, U.S. Patent 5,121,756 (Jun. 16, 2002) the entirety of which is hereby incorporated by reference. Flexible casings may be available in different sizes to accommodate for example, extra-large, average and small subjects. Vacuum pump 24 is disposed in the housing for controlling the amount of air 25 within the flexible casing and for deflating the flexible casing. Vacuum pump 24 may be any suitable manual or electric means for evacuating the interior of the casing and is in fluid communication with the interior volume of the casing to enable controlled evacuation of the casing to control the rigidity and conformance of the casing and the beads within the casing to the shape of the subject. The combination of

rigid immobilization with mechanical CPR or other advanced life support techniques provides help to subjects with multiple problems who would otherwise be impossible to help with conventional immobilization.

[0024] The volume of air within flexible casing 20 may also be controlled by valve 28. When a subject is placed on flexible casing 20 the weight of the subject will raise the pressure within the casing and force air 25 out through valve 28. Valve 28 may be any suitable valve to allow air 25 or other fluid to escape from within the casing. Valve 28 may also be used to permit air to reenter casing 20 to permit readjustment of a subject after air 25 has been evacuated.

[0025] In use, subject 23 is placed on casing 19 and beads 22 are arranged to support and immobilize the subject and belt portions 3L and 3R are placed through slots 26A and 26B and then under the subject's axilla (armpits), wrapped around the subject's chest, and secured. Vacuum pump 24 is engaged to deflate the casing which rigidly compresses beads 22 together and immobilizes the subject. Means for tightening the belt 27 is activated to tighten belt 3 repetitively to perform chest compressions.

[0026] Resuscitation apparatus 30 of Figures 4 and 5 includes any suitable chest compression device such as chest compression device 31 which applies compressions with the belt 32. The chest compression device 31 includes a belt drive platform 33 and a compression belt cartridge 34 (which includes the belt 32). The belt drive platform includes a housing 35 engaging an upper body airtight flexible casing 36 upon which subject 23 rests and is immobilized, a means 37 for tightening the belt, a processor 38, a user interface 39 and a vacuum pump 40 such as a vacuum pump disposed in the housing for controlling the amount of air 25 within the flexible casing and for deflating the flexible casing. Flexible casing

36 is partially filled with movable, discrete elements such as beads or pellets 44 to support and immobilize the subject. Pellets 44 may be made of expanded or solid plastic material, such as polystyrene or polyvinyl chloride and be formed in any shape such as spherical or other suitable regular or irregular shape. The loose beads or pellets within an inflated flexible casing permit the casing sides to be moved up against the sides of the subject to cradle and support the subject. The beads are then movable to conform to the contours of the patient's body, and also movable to regions where greater rigidity is required.

[0027] Additionally, casing 36 may also include one or more portions that may be independently operable as well as containing specific quantities of pellets 44 in each portion to control the profile and rigidity of the independent portions. For example, neck wedge portion 45 may be configured with pellets 44 to maintain alignment between the subject's head 23A and the subject's thorax 23B with the subject's airway 23C optimally opened as illustrated. Independent operability of the one or more portions of a casing may be accomplished using multiple vacuum pumps independently controllable by processor 38, or a single vacuum pump with a valving system controllable by processor 38. Means for tightening the belt 37 includes a motor 41, a drive train 42 (clutch, brake and/or gear box) and a drive spool 43 upon which the belt spools during use.

[0028] Processor 38 is operably connected to vacuum pump 40 to control the rigidity of casing 36 and one or more vacuum or pressure sensor such as sensor 29 to monitor and provide feedback to the processor. Sensor 29 may be operably connected to casing 36 or vacuum pump 40 to monitor the pressure (vacuum) within the casing and therefore its rigidity. Processor 38 may include one or more preset pressure settings for the casing and for each separate portion

of the casing. Sensor 29 may also provide feedback to rescuers when manually controlling the operation of the vacuum pump or manually pumping air from the casing.

[0029] Referring now to Figures 6, 7 and 8, rescue apparatus 50 includes an automated CPR apparatus such as belt drive platform 51 secured to an upper body airtight flexible casing such as casing 52 secured to housing. Casing 52 is in fluid communication with vacuum pump 53 which controls the amount of air 54 within casing 52. Casing 52 is sized to support a subject from the head to the waist and it includes ridges such as first ridge 55 and second ridge 56 which provide separation between the subject's arms and the subject's thorax when the subject is immobilized. Within support ridges 55 and 56 are one or more slots or openings such as slots 52A and 52B respectively. The openings or slots permit a compression belt or compression support structure to pass through the casing to enable mechanical CPR to be performed on an immobilized subject. The casing may also include a neck support portion of the casing to maintain alignment between the subject's head and torso and open the subject's airway.

[0030] To provide optimal compression of the subject's thorax, one or more windows are provided in casing such as scapular window 57 which are oriented to conform to the scapulae of a subject properly oriented on the automated chest compression device. The windows are areas of the casing that are sealed to prevent entry of any beads 22 into the window space. This configuration has only one or more layers of incompressible casing material 52M between the subject's scapulae and belt drive platform 51. This configuration enables the chest compression device to compress the subject's chest without compressing the beads within the immobilizing casing. One or more incompressible windows may also be provided to expose load sensors, such as load sensor 58, to

the subject's weight and the compression force without any beads between the subject and the load sensor or sensors. The load sensors are operably connected to the any suitable chest compression means for controlling the intensity of the chest compressions. One or more support sections may be included to maintain alignment and immobilization of the subject's skeleton during CPR such as spinal support section 59.

[0031] Casing 52 may also include one or more portions that may be have independent air content controls as well as specific quantities of beads 22 to control the profile of the independent portions such as spinal support section 59, neck wedge 60 and or first and second ridges 55 and 56 respectively. Independent control enables the head and neck of a subject to be immobilized for performance of intubation separately from thorax or torso immobilization. Alternatively, the separate casings may be maintained at different levels of rigidity to accommodate the specific injuries of the subject.

[0032] Referring now to Figures 9 and 10, full size casing 70 is configured to secure a subject's arms to the side of the body with minimal separation between the arms and the body in torso portion 70A as well as the full length of the subject's legs and feet with leg portion 70B. Scapular windows such as first scapular window 71 and second scapular window 72 are oriented to permit a subject's scapula to contact belt drive platform 73 and one or more load sensors such as load sensor 74. Scapular windows such as scapular windows 71 and 72 may adopt any suitable configuration such as the scapular specific shape of second scapular window 72 or a shape such as first scapular window 71 to optimize contact between the subject's body and load sensor 74. The configuration of casing 70 also includes a full length spinal support 75 and first and second slots 76 and 77 respectively to provide access for belts or support frames for automated CPR devices.

[0033] Referring now to Figure 11, immobilization and rescue apparatus 80 includes full length immobilization casing 81 connected to backboard 82 of LUCAS™ chest compression system 83. As discussed above, casing 81 may also be a torso only immobilizer and may include one or more windows such as window 84 to permit skeletal elements of subject 23 to contact backboard 82 with no intervening compressible elements. Window 84 will be formed in casing 81 in the area generally supporting the scapulae and the area between the scapulae of a subject properly oriented in the casing. Casings such as casing 81 include one or more access slots or holes such as slots 85A and 85B to permit support structure such as support legs 86 to pass through the immobilization casing and support chest compression unit 87 with piston 88 apposing subject's chest 23C. The casing may also include one or more restraining straps 89 to further engage and immobilize subject 23.

[0034] While the preferred embodiments of the devices and methods have been described in reference to the environment in which they were developed, they are merely illustrative of the principles of the inventions. The elements of the various embodiments may be incorporated into each of the other species to obtain the benefits of those elements in combination with such other species, and the various beneficial features may be employed in embodiments alone or in combination with each other. Other embodiments and configurations may be devised without departing from the spirit of the inventions and the scope of the appended claims.

We claim:

1. An apparatus for immobilizing and treating a subject comprising:

a belt drive platform comprising:

a housing;

a drive spool operably attached to the housing; and

a means for rotating the drive spool, said means for rotating disposed within the housing and operably attached to the drive spool;

a processor operably connected to the means for rotating the drive spool, the processor controlling the means for rotating to generate repetitive chest compressions;

a compression belt cartridge comprising:

a belt suitable for compressing the chest of the subject; and
a spline attached to the belt; wherein the spline is removably attachable to the drive spool; wherein rotation of the drive spool tightens the belt to compress the chest;

an airtight flexible casing secured to the housing, the casing operable to contain air and having variable rigidity which varies as a function of the amount of air within the casing, the casing further including two or more slots to permit passage of the belt from the drive belt platform to engage the thorax of the subject;

a vacuum pump for evacuating the air from within the flexible casing to control the rigidity of the casing;

a plurality of beads located within the casing, the plurality of beads adapted to move and conform the casing to support the subject to be immobilized when the casing is inflated,

the plurality of beads adapted to be rigidly fixed in position when the casing is in a fully evacuated state.

2. The apparatus of claim 1 further comprising:

a scapular window sealed in the casing, the scapular window containing no beads to enable contact between the subject's scapula and the housing.

3. The apparatus of claim 2 further comprising:

two separation ridges formed in the casing, each separation ridge separating one of the subject's arms from the subject's torso.

4. The apparatus of claim 3 further comprising:

a neck support portion of the casing to maintain alignment between the subject's head and torso and open the subject's airway.

5. The apparatus of claim 3 wherein the airtight flexible casing supports and immobilizes the subject from head to foot.

6. The apparatus of claim 3 wherein the airtight flexible casing supports and immobilizes the subject from head to waist.

7. The apparatus of claim 3 wherein the casing further comprises:

two or more portions, wherein each portion is independently operable to control the profile and rigidity of the portion.

8. The apparatus of claim 7 wherein each of the two or more portions of the casing include a plurality of beads.

9. The apparatus of claim 8 wherein one of the two or more portions comprises:

a neck support portion of the casing to maintain alignment between the subject's head and torso and open the subject's airway.

10. The apparatus of claim 3 wherein the processor controls the operation of the vacuum pump to control the rigidity of the casing.

11. The apparatus of claim 10 further comprising:

a sensor operably connected to the processor for measuring pressure within the casing to enable the processor to control the operation of the vacuum pump to control the rigidity of the casing.

12. The apparatus of claim 7 further comprising:

a processor, the processor controlling the operation of the vacuum pump to independently control the rigidity of the two or more portions of the casing.

13. The apparatus of claim 3 further comprising:

a load sensor operably connected to the processor for controlling the repetitive chest compressions, the load sensor secured to the housing with the scapular window between the subject and the load sensor.

14. A method for immobilizing and treating a subject comprising the steps:

providing a means for mechanically compressing the chest of the subject;

providing an airtight flexible casing secured to the means for mechanically compressing the chest of the subject, the casing containing air and a plurality of beads wherein the beads provide variable rigidity which varies as a function of the amount of air within the casing;

providing a vacuum pump for evacuating the air from within the flexible casing to control the rigidity of the casing;

placing the subject on the casing;

arranged the plurality of beads to support and immobilize the subject;

securing a subject to means for mechanically compressing the chest of the subject;

evacuating air from within the casing to rigidly compresses plurality of beads and immobilize the subject; and

activating the means for mechanically compressing the chest to repetitively perform chest compressions.

15. The method of claim 14 wherein the step of evacuating air from within the casing further comprises operating a processor to control the vacuum pump to evacuate a portion of the air from within the casing to compress the plurality of beads to a preset level of rigidity.

16. The method of claim 14 further comprising the step:



measuring the force of mechanical chest compressions using one or more force sensors between the means for mechanically compressing the chest and the casing.

17. The method of claim 14 further comprising the step:

providing a vacuum sensor in fluid communication with the casing and operably connected to the

measuring the force of mechanical chest compressions using one or more force sensors between the means for mechanically compressing the chest and the casing.

18. The method of claim 14 wherein the means for mechanically compressing the chest of the subject comprises a belt driven chest compression apparatus.

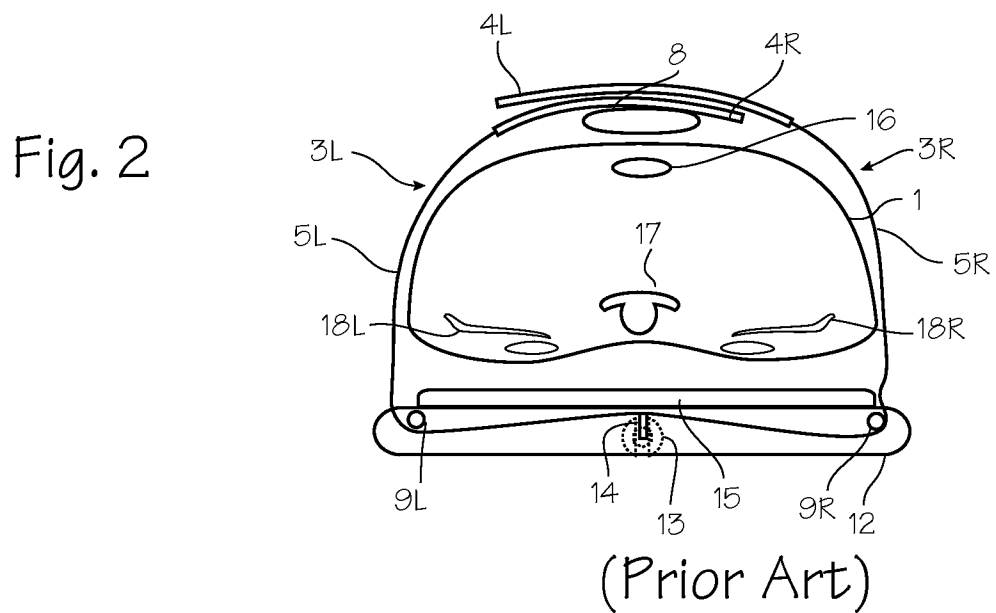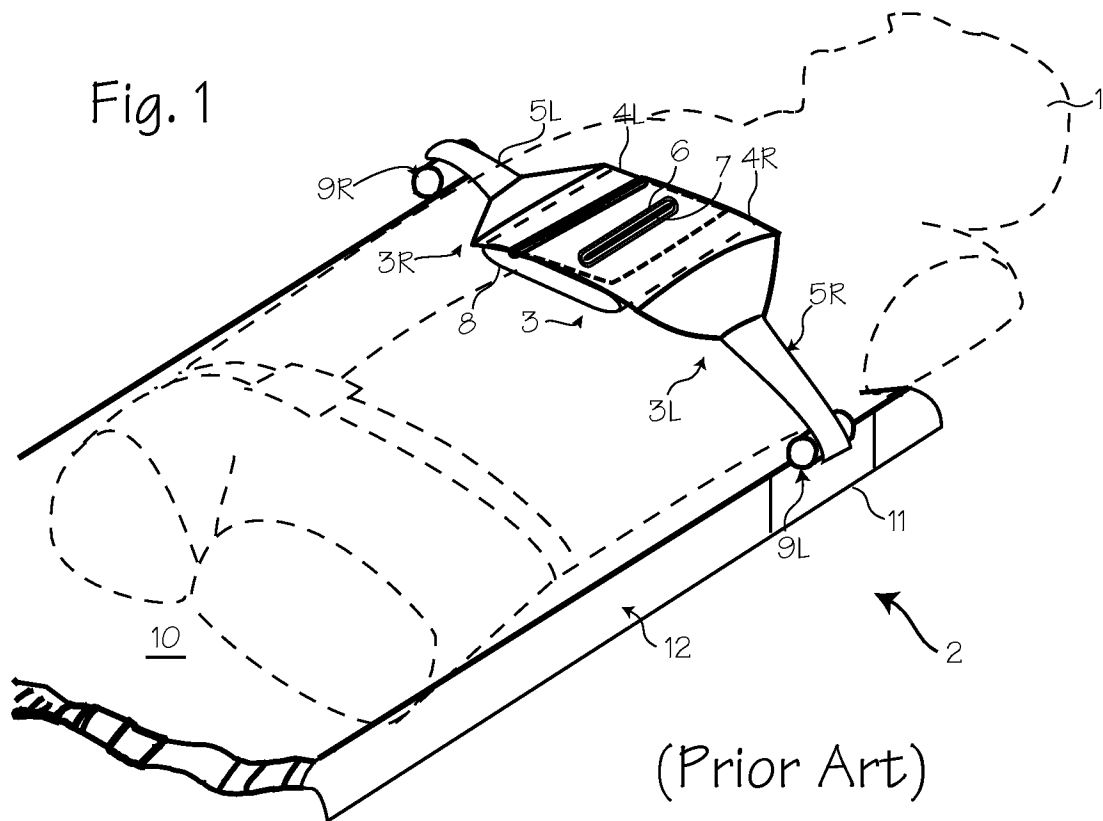

2/6

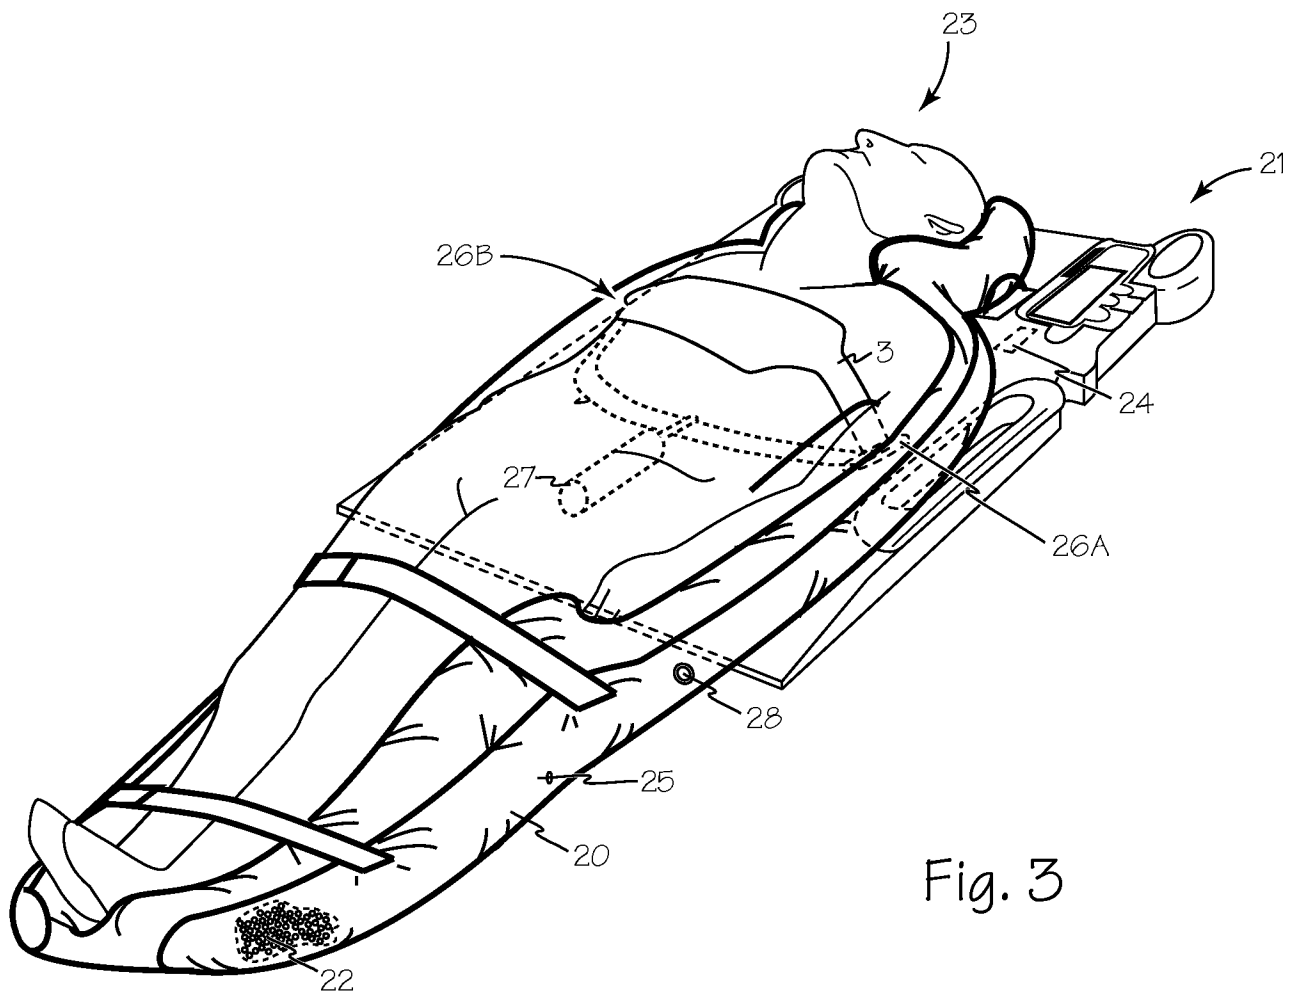


Fig. 3

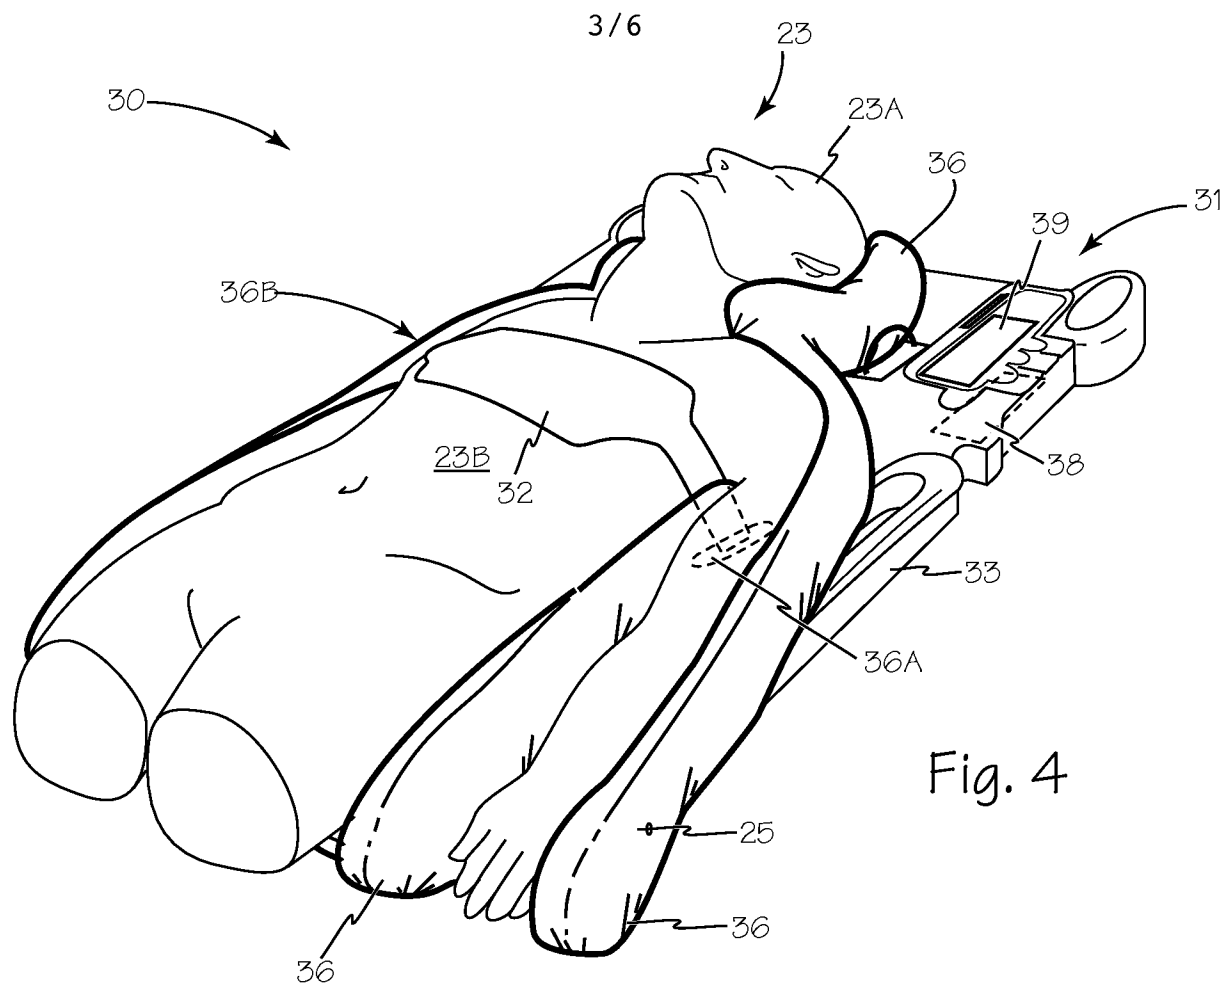


Fig. 4




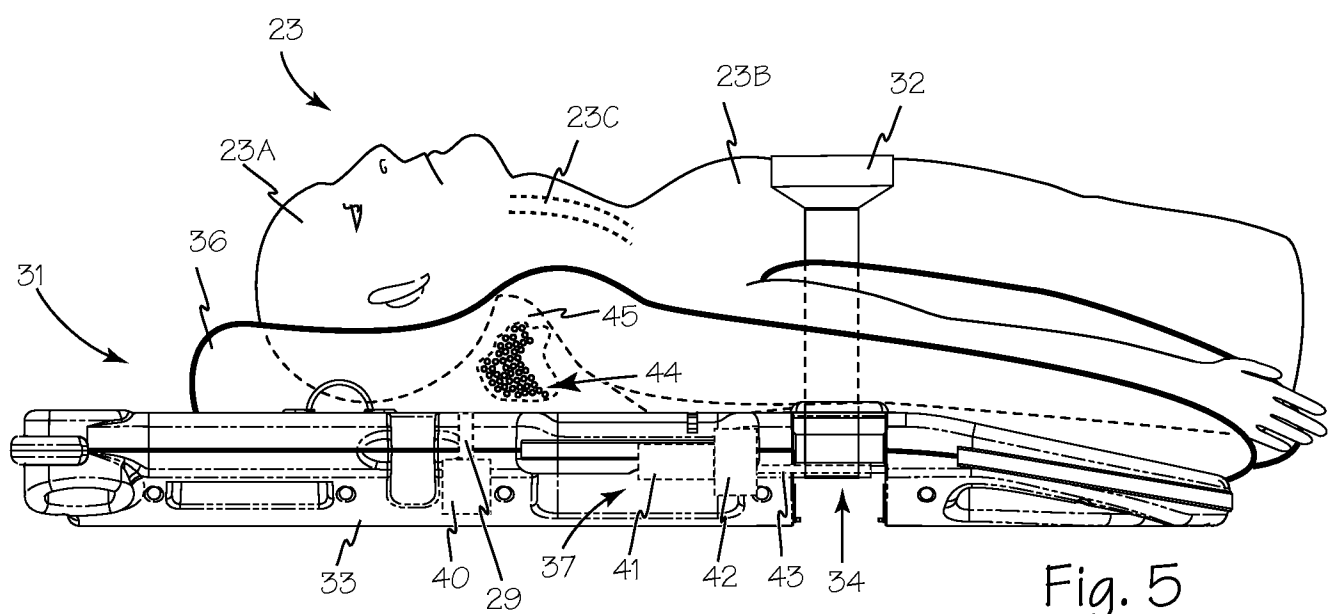


Fig. 5

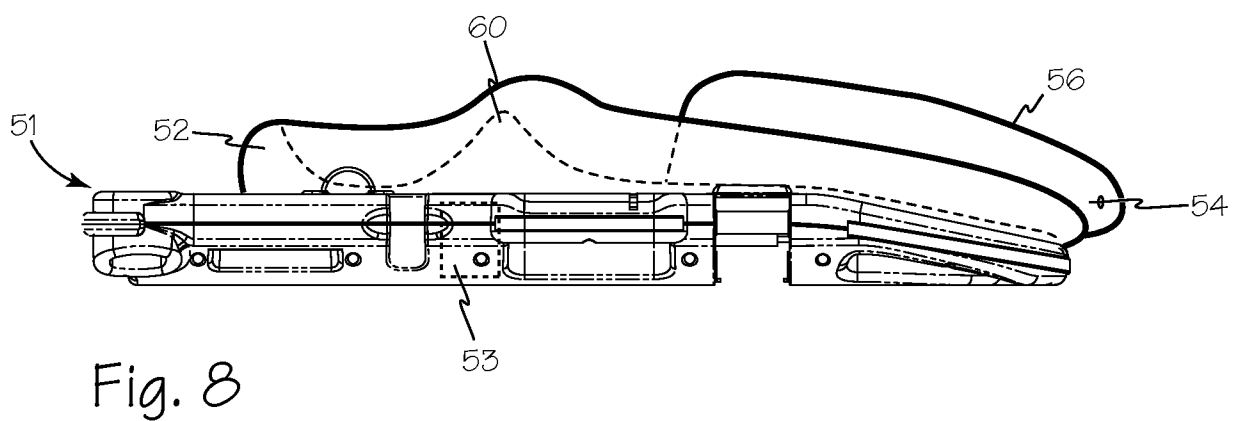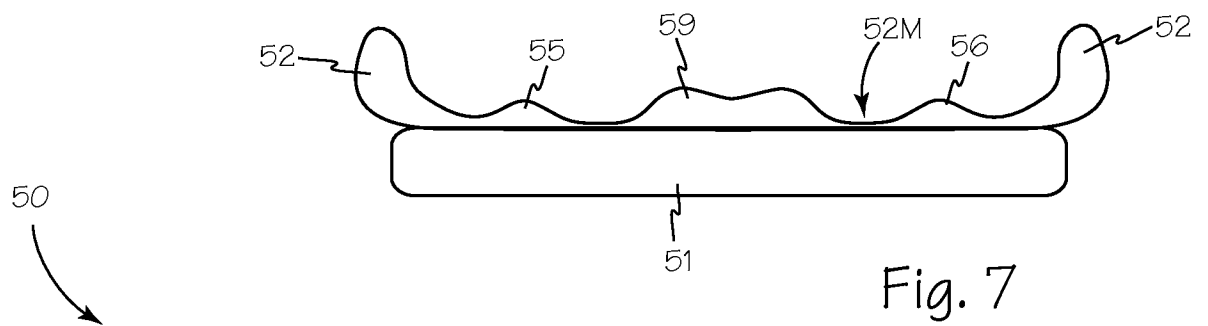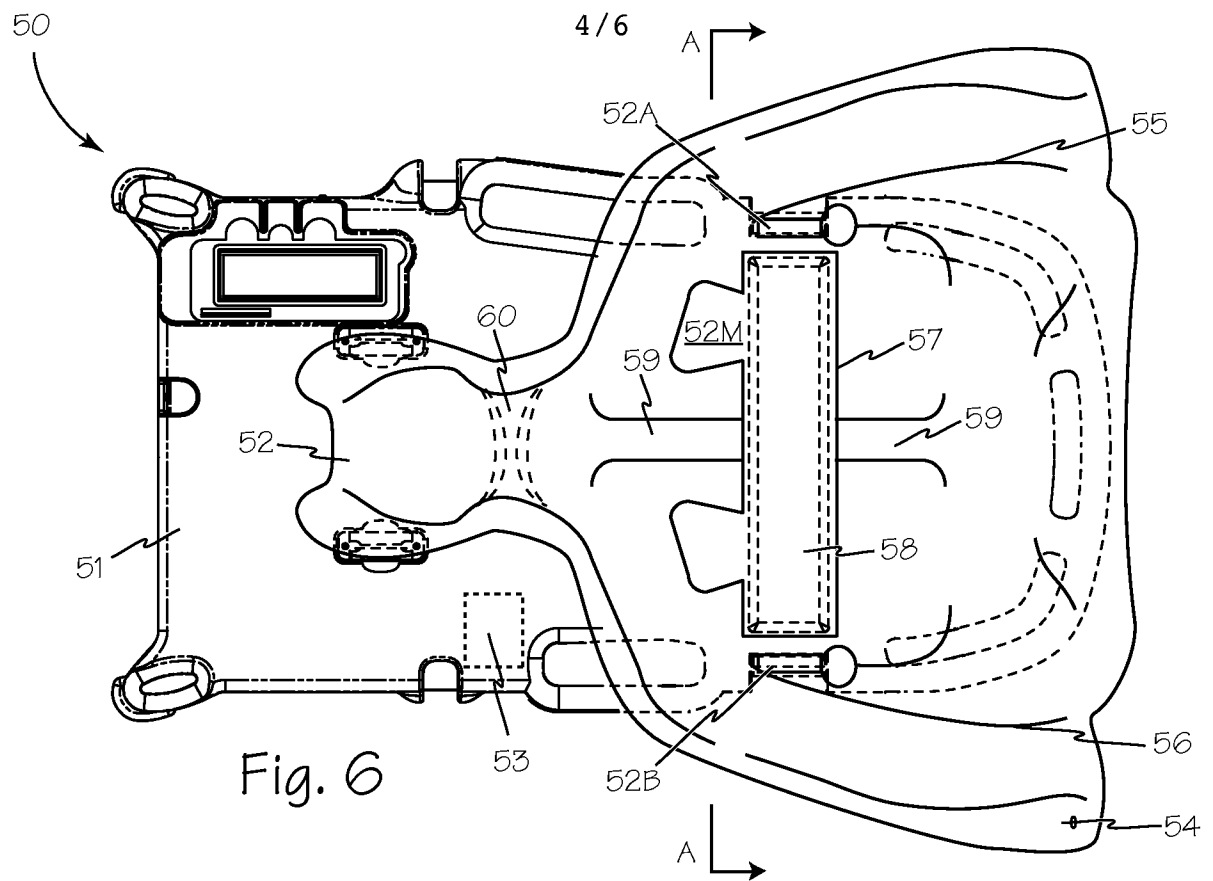

5/6

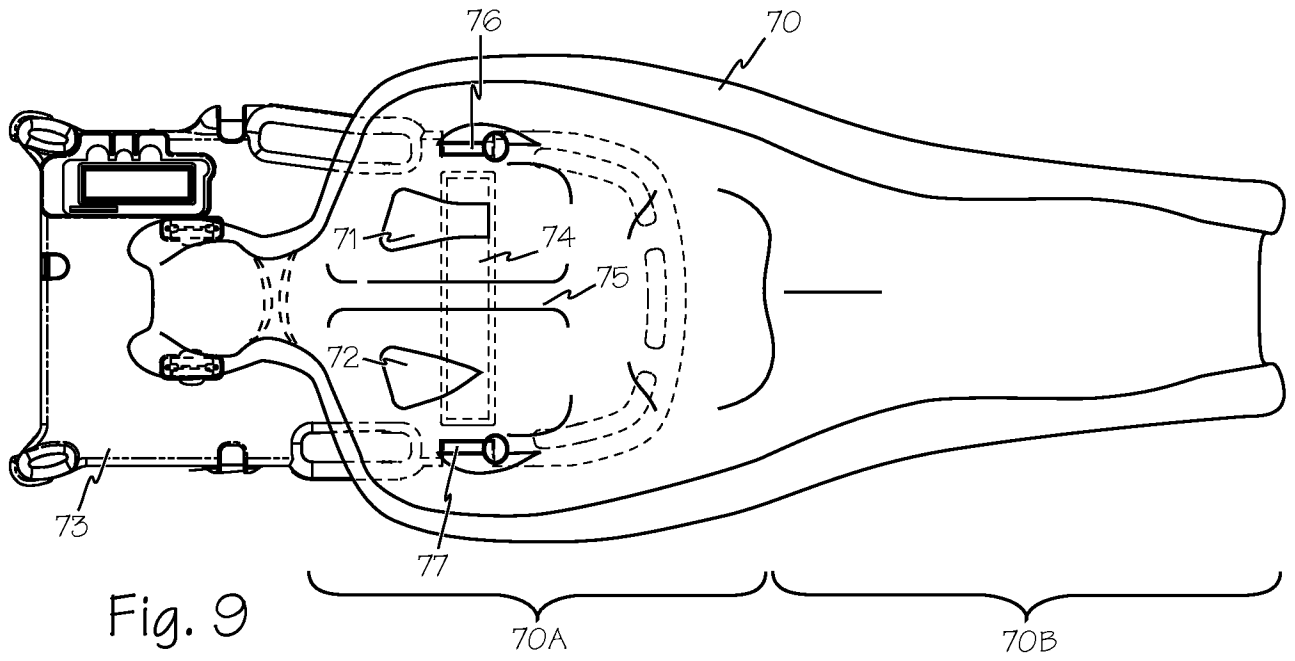


Fig. 9

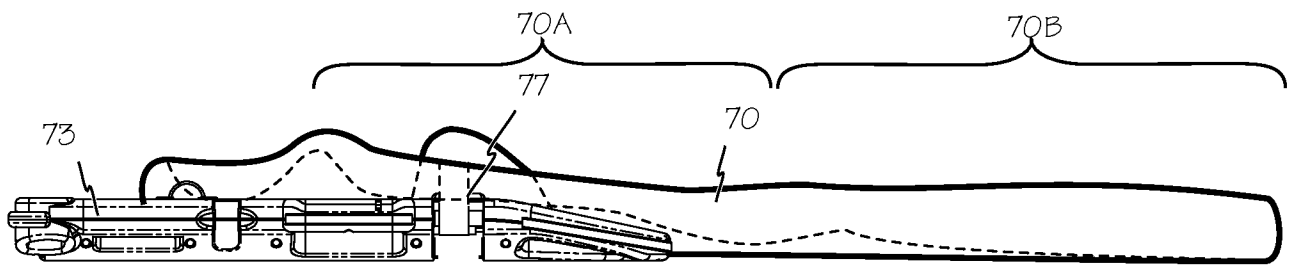


Fig. 10

6/6

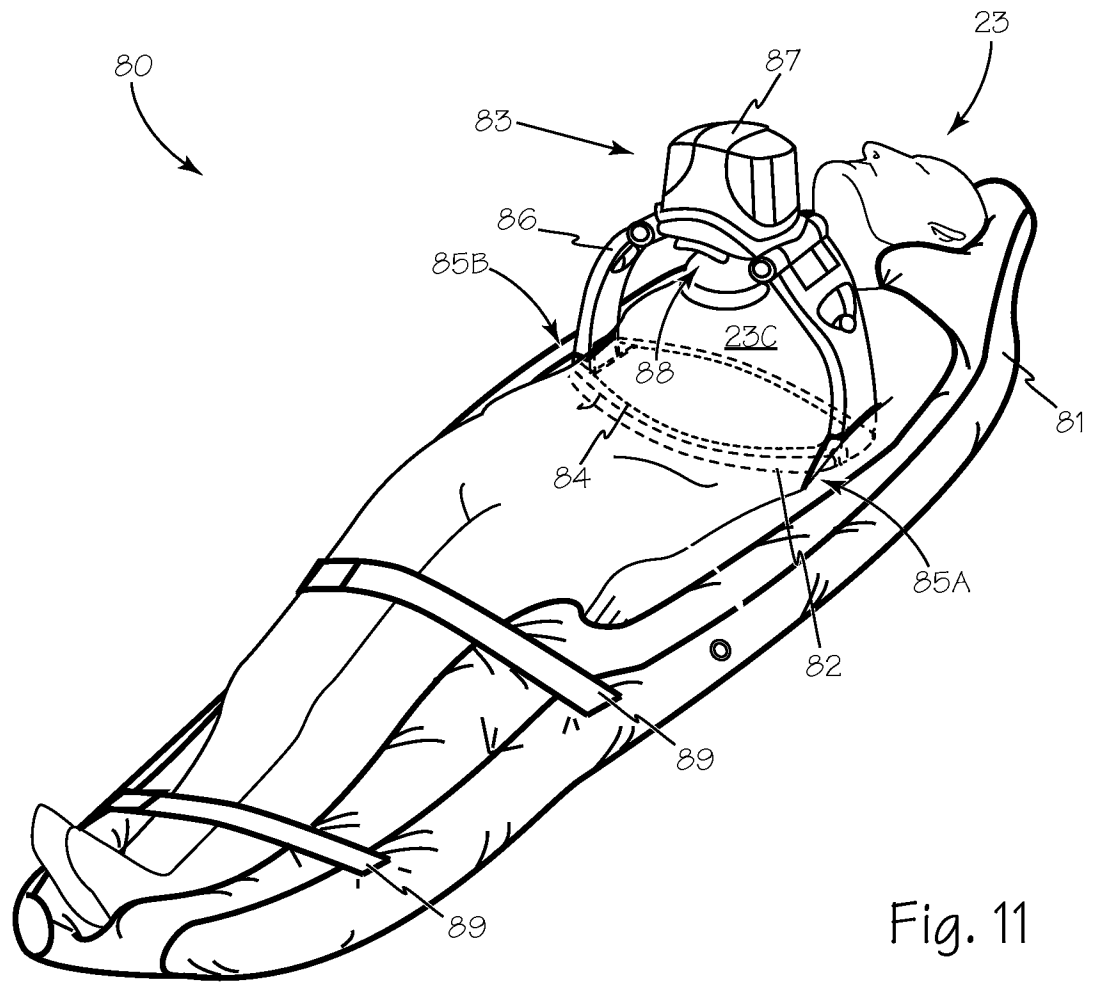


Fig. 11

A. CLASSIFICATION OF SUBJECT MATTER**A61H 31/00(2006.01)i, A62B 33/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61H 31/00; A61N 1/39; A61G 13/12; A62B 33/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: cpr, compression chest, belt, sensor, beads

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2007-0270725 A1 (SHERMAN et al.) 22 November 2007 See paragraphs [0076], [0081], [0094], [0096], [0097], [0151]; claim 1; and figure 15.	1, 14-16, 18
A		2-13, 17
Y	US 2011-0047706 A1 (HIEBERT, EUGENE LLOYD) 3 March 2011 See paragraphs [0039], [0052]; and figure 5.	1, 14-16, 18
A	WO 2005-037178 A1 (REVIVANT CORPORATION) 28 April 2005 See claims 1-21; and figure 1.	1-18
A	US 2004-0162587 A1 (HAMPTON et al.) 19 August 2004 See paragraphs [0049]-[0052]; and figures 1, 3.	1-18
A	US 7347832 B2 (JENSEN et al.) 25 March 2008 See claims 1-7; and figure 1.	1-18



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

04 December 2013 (04.12.2013)

Date of mailing of the international search report

04 December 2013 (04.12.2013)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,
302-701, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

CHANG, Bong Ho

Telephone No. +82-42-481-3353



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/057020

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2007-0270725 A1	22/11/2007	AT 372103 T	15/09/2007
		AU 2002-316169 B2	16/03/2006
		AU 2003-251811 A1	23/01/2004
		AU 2003-251811 B2	29/05/2008
		AU 2006-202330 A1	22/06/2006
		AU 2006-202330 B2	22/10/2009
		AU 2010-200268 A1	18/02/2010
		AU 2010-200268 B2	31/05/2012
		AU 2012-203170 A1	21/06/2012
		CA 2448060 A1	05/12/2002
		CA 2448060 C	17/07/2012
		CA 2491965 A1	15/01/2004
		CA 2491965 C	04/09/2012
		CA 2775620 A1	15/01/2004
		CA 2776365 A1	05/12/2002
		DE 60222260 D1	18/10/2007
		DE 60222260 T2	29/05/2008
		EP 1401373 A2	31/03/2004
		EP 1401373 A4	02/02/2005
		EP 1401373 B1	05/09/2007
		EP 1534209 A2	01/06/2005
		EP 1857086 A2	21/11/2007
		EP 1857086 A3	05/12/2007
		EP 2314269 A2	27/04/2011
		EP 2468231 A2	27/06/2012
		EP 2468232 A2	27/06/2012
		JP 04447454 B2	07/04/2010
		JP 2004-534574 A	18/11/2004
		JP 2005-532122 A	27/10/2005
		JP 2012-096044 A	24/05/2012
		US 2002-0177793 A1	28/11/2002
		US 2003-0004445 A1	02/01/2003
		US 2004-0002667 A1	01/01/2004
		US 2004-0006290 A1	08/01/2004
		US 2004-0030271 A1	12/02/2004
		US 2004-0225238 A1	11/11/2004
		US 2006-0009717 A1	12/01/2006
		US 2010-0241039 A1	23/09/2010
		US 2013-123673 A1	16/05/2013
		US 6616620 B2	09/09/2003
		US 6939314 B2	06/09/2005
		US 6939315 B2	06/09/2005
		US 7008388 B2	07/03/2006
		US 7056296 B2	06/06/2006
		US 7131953 B2	07/11/2006
		US 7666153 B2	23/02/2010
		US 8298165 B2	30/10/2012
		WO 02-096343 A2	05/12/2002
		WO 02-096343 A3	04/12/2003

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/057020

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		WO 2004-004548 A2	15/01/2004
		WO 2004-004548 A3	13/05/2004
US 2011-0047706 A1	03/03/2011	US 2011-0126355 A1	02/06/2011
		US 2013-206148 A1	15/08/2013
		US 8469911 B2	25/06/2013
WO 2005-037178 A1	28/04/2005	AU 2004-281777 A1	28/04/2005
		AU 2004-281777 B2	02/12/2010
		AU 2011-200917 A1	24/03/2011
		CA 2551804 A1	28/04/2005
		CA 2551804 C	14/08/2012
		CA 2779585 A1	28/04/2005
		CN 1893904 A	10/01/2007
		CN 1893904 B	16/06/2010
		EP 1684687 A1	02/08/2006
		EP 1684687 A4	10/03/2010
		EP 1684687 B1	05/09/2012
		EP 2520269 A2	07/11/2012
		EP 2520269 A3	06/03/2013
		EP 2520270 A2	07/11/2012
		EP 2520270 A3	06/03/2013
		EP 2550951 A2	30/01/2013
		EP 2550951 A3	06/03/2013
		JP 04694496 B2	08/06/2011
		JP 2007-508124 A	05/04/2007
		US 2005-0080360 A1	14/04/2005
		US 2005-0080361 A1	14/04/2005
		US 2005-0080362 A1	14/04/2005
		US 2008-0255481 A1	16/10/2008
		US 2008-0287841 A1	20/11/2008
		US 2008-0295851 A1	04/12/2008
		US 2011-0137216 A1	09/06/2011
		US 7354407 B2	08/04/2008
		US 7404803 B2	29/07/2008
		US 7410470 B2	12/08/2008
		US 7846112 B2	07/12/2010
		US 7955283 B2	07/06/2011
		US 8114035 B2	14/02/2012
US 2004-0162587 A1	19/08/2004	US 2008-0114406 A1	15/05/2008
		US 2012-116272 A1	10/05/2012
		US 7308304 B2	11/12/2007
		US 8121681 B2	21/02/2012
		WO 2004-073580 A1	02/09/2004
US 7347832 B2	25/03/2008	AU 2004-281779 A1	28/04/2005
		AU 2004-281779 B2	18/11/2010
		CA 2551805 A1	28/04/2005
		CN 102106779 A	29/06/2011

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/057020

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		CN 1893905 A	10/01/2007
		CN 1893905 B	04/05/2011
		EP 1682067 A1	26/07/2006
		JP 04563392 B2	13/10/2010
		JP 2007-508125 A	05/04/2007
		US 2005-0080363 A1	14/04/2005
		US 2005-0080364 A1	14/04/2005
		US 2008-0045867 A1	21/02/2008
		US 2010-0174216 A1	08/07/2010
		US 7270639 B2	18/09/2007
		WO 2005-037179 A1	28/04/2005