



Europäisches
Patentamt
European
Patent Office
Office européen
des brevets



(11) EP 2 977 072 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
27.01.2016 Bulletin 2016/04

(51) Int Cl.:
A61M 25/01 (2006.01) A61M 25/00 (2006.01)
A61M 25/10 (2006.01) A61M 25/04 (2006.01)

(21) Application number: 15181301.1

(22) Date of filing: 26.06.2008

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MT NL NO PL PT
RO SE SI SK TR

(30) Priority: 26.06.2007 US 929395 P
19.10.2007 US 960900 P
26.10.2007 US 996057 P
21.03.2008 US 64715 P

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
08772056.1 / 2 203 209

(71) Applicant: Roxwood Medical, Inc.
Dover, DE 19901 (US)

(72) Inventor: TABER, Mark
St. Louis, MO 63141 (US)

(74) Representative: Crease, Devanand John et al
Keltie LLP
No.1 London Bridge
London SE1 9BA (GB)

Remarks:

This application was filed on 17-08-2015 as a divisional application to the application mentioned under INID code 62.

(54) CATHETER APPARATUS FOR TREATING VASCULATURES

(57) A catheter apparatus (11) for advancing a guidewire through a chronic total occlusion in a vasculature which may have a shaft having a distal portion; a removable, expandable scaffold structure (27) coupled to

the distal portion (13) of the shaft (23) and a single, centrally located lumen (47) passing centrally through the shaft and through the expandable scaffold structure and configured to pass over a guidewire.

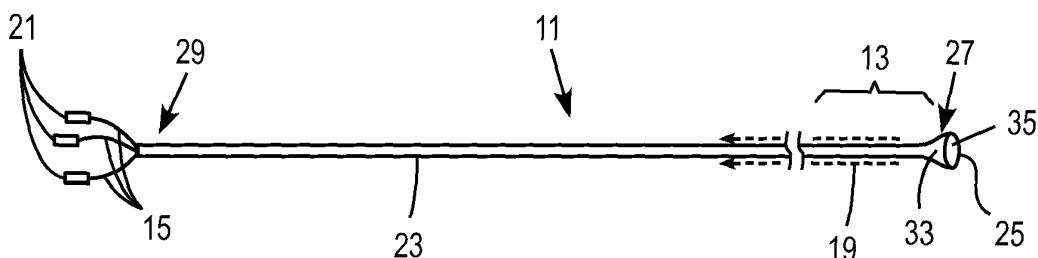


FIG. 1A

EP 2 977 072 A1

Description**FIELD OF THE INVENTION**

[0001] The invention relates generally to an apparatus and method for treating vasculatures, and, more particularly, to methods and apparatus for passing one or more guidewires through a chronic total occlusion of a vasculature.

BACKGROUND OF THE INVENTION

[0002] A chronic total occlusion in a coronary artery, peripheral artery, vein, dialysis fistula or other types of vasculature represents a challenge for percutaneous treatment. Percutaneous treatments are generally preferred revascularization options as compared to bypass surgery. Continuing improvements in equipment specifically developed for chronic total occlusions have allowed success rates to improve. Although the success rates for these types of procedures have improved, the procedures for percutaneous treatments still suffer from several drawbacks. Patients without a successful percutaneous treatment may need to undergo bypass surgery or experience continuing symptoms from the occlusions.

[0003] A major obstacle within a chronic total occlusion may often be encountered while attempting to advance a guidewire across the chronic total occlusion in a vasculature. A maximum resistance may be met at the most proximal point of the lesion, i.e. the firm, fibrous cap. While being advanced, a guidewire may tend to deflect away from the fibrous cap towards the adventitial layer, often entering a false lumen. This off-axis displacement of the guidewire often may result in a procedural failure.

[0004] Successful passage of the guidewire may also be obstructed by randomly located calcified regions of atherosclerotic plaque within the mass of the lesion. Microchannels within the obstruction may be desirable targets for the tip of the guidewire. However, these soft spots within the lesion are difficult to identify angiographically and are dispersed randomly within the matrix of the lesion.

[0005] Coronary arteries and other vasculatures tend to be non-linear conduits, often coursing over the surface of the epicardium and other tissues. The success of current technology is limited by this type of geometry. In current systems, a guidewire or currently available catheter is advanced down a vasculature to the level of the obstruction. At the point of the obstruction, the guidewire advancement may tend to proceed along the outer, greater curvature of the vasculature. Even a guidewire centered within the vasculature at the proximal edge of the chronic total occlusion may tend to proceed toward the outer, greater curvature of a vasculature.

[0006] As a result, only a minor portion of the surface area of the obstruction may be encountered with sufficient force to allow passage of the guidewire. On many occasions, the angle of encounter and/or the force ap-

plied to the fibrous cap may not be sufficient for crossing the fibrous cap with the guidewire. If the tip of the guidewire is curved prior to placement through the support catheter, direct longitudinal force may be compromised as the wire is advanced off axis. If a rapid exchange catheter system is used as catheter support, the guidewire may buckle within the guide-catheter resulting in suboptimal longitudinal guidewire force.

[0007] At times, a single lumen angioplasty balloon may be inflated just proximal to the chronic total occlusion in an attempt to center the guidewire in the vessel lumen and provide additional support for the guidewire. Atherosclerotic lesions tend to be asymmetric with an eccentric true lumen. Therefore, attempts to limit the guidewire to the central axis of the vessel lumen may result in lower rates of procedural success.

[0008] Generally, needs exist for improved apparatus and methods for treating vasculatures. More specifically, needs exist for improved apparatus and methods for efficiently and effectively passing a guidewire through a chronic total occlusion in a vasculature.

SUMMARY OF THE INVENTION

[0009] Embodiments of the present invention solve many of the problems and/or overcome many of the drawbacks and disadvantages of the prior art by providing an apparatus and method for treating vasculatures.

[0010] In particular, embodiments of the invention may accomplish this with an apparatus for efficiently and effectively passing a guidewire through a chronic total occlusion in a vasculature. The apparatus may have a flexible shaft, one or more guidewire lumens passing longitudinally through the shaft, and a positioning means for positioning distal ends of the one or more guidewires relative to an inner wall of an external lumen.

[0011] The positioning means may be an expandable scaffold initially in a non-expanded state. A retractable sheath may surround the expandable scaffold and the retractable sheath may be retracted for expanding the expandable scaffold.

[0012] The positioning means may also be one or more balloons where the one or more balloons are inflated through an inflation port running longitudinally in the shaft. The positioning means may also include guidewire lumens coupled to or otherwise disposed within the expandable scaffold. The positioning means may also include inflatable means surrounding distal ends of the guidewire lumens. The inflatable means may or may not be located within an expandable scaffold.

[0013] The positioning means may also be a rotatable core within the shaft. The positioning means may also include a deflectable tip on the catheter. The positioning means may also include a shape-memory material integrated with the guidewire lumens.

[0014] A method of operating a catheter apparatus may include providing a catheter apparatus including a flexible shaft, one or more guidewire lumens passing lon-

itudinally through the shaft, one or more guidewires within the one or more guidewire lumens, and a positioning means, inserting a guide catheter into a vasculature with a chronic total occlusion, inserting the catheter apparatus into the guide catheter, activating the positioning means for positioning the one or more guidewires relative to the chronic total occlusion, and advancing the one or more guidewires through the one or more guidewire lumens and into contact with the chronic total occlusion.

[0015] The one or more guidewires may be passed through the chronic total occlusion. The catheter apparatus may be withdrawn from the vasculature while leaving the one or more guidewires in place. The one or more guidewires may be withdrawn from contact with the chronic total occlusion and the one or more guidewires may be advanced through the one or more guidewire lumens into contact with the chronic total occlusion repeatedly until a suitable site for passing the one or more guidewires through the chronic total occlusion is found. The positioning means may be activated before each advancing the one or more guidewires through the one or more guidewire lumens into contact with the chronic total occlusion.

[0016] Another embodiment of the present invention may be a catheter apparatus including a multi-lumen main shaft; one or more guidewire lumens extending from a distal end of the multi-lumen shaft with lumens within the one or more guidewire lumens contiguous with at least one of the multi-lumens of the multi-lumen main shaft; an expandable support structure coupled to the distal end of the multi-lumen shaft; one or more loops corresponding to each of the one or more guidewire lumens, wherein the one or more loops corresponding to each of the one or more guidewire lumens are coupled to the expandable support structure, and wherein the one or more loops corresponding to each of the one or more guidewire lumens project inward from the plane of the expandable support structure; and wherein the one or more guidewire lumens are threaded through the corresponding one or more loops.

[0017] Additional features, advantages, and embodiments of the invention are set forth or apparent from consideration of the following detailed description, drawings and claims. Moreover, it is to be understood that both the foregoing summary of the invention and the following detailed description are exemplary and intended to provide further explanation without limiting the scope of the invention as claimed.

BRIEF DESCRIPTION OF THE INVENTION

[0018] The accompanying drawings, which are included to provide a further understanding of the invention and are incorporated in and constitute a part of this specification, illustrate preferred embodiments of the invention and together with the detailed description serve to explain the principles of the invention. In the drawings:

Fig. 1A is a perspective view of a self-expanding catheter apparatus.

Fig. 1B is a distal end view of the catheter apparatus of Fig. 1A.

Fig. 1C is a cross section view of a midpoint of the catheter apparatus of Fig. 1A.

Fig. 1D is a perspective view of the self-expanding end of the catheter apparatus of Fig. 1A in an expanded state with a stop point.

Fig. 1E is a cross section view of a midpoint of the catheter apparatus of Fig. 1D.

Fig. 1F is distal end view of the catheter apparatus of Fig. 1D.

Fig. 1G is a perspective view of the self-expanding end of the catheter apparatus of Fig. 1A in an expanded state with a truncated conical portion.

Fig. 1H is a side view of the catheter apparatus of Fig. 1A in a sheathed state.

Fig. 1I is a perspective view of the catheter apparatus of Fig. 1A with a deflectable tip.

Fig. 1J is a side view of a shorter constraining sheath.

Fig. 1K is a side view of a longer constraining sheath.

Fig. 2A is a perspective view of a catheter apparatus with a single balloon.

Fig. 2B is a cross section view of a midpoint of the catheter apparatus of Fig. 2A.

Fig. 3A is a perspective view of a catheter apparatus with double balloons.

Fig. 3B is a cross section view of a midpoint of the catheter apparatus of Fig. 3A.

Fig. 4A is a perspective view of a catheter apparatus with a balloon.

Fig. 4B is a distal end view of the catheter apparatus of Fig. 4A.

Fig. 4C is a cross section view of a midpoint of the catheter apparatus of Fig. 4A.

Fig. 5A is a perspective view a catheter apparatus with a rotating inner core.

Fig. 5B is a cross section view of a midpoint of the

catheter apparatus of Fig. 5A.

Fig. 6A is a perspective view a catheter apparatus with a deflecting tip and stabilizing balloon.

Fig. 6B is a cross section view of a midpoint of the catheter apparatus of Fig. 6A.

Fig. 7A is a perspective view of a catheter apparatus with an expandable mesh tip.

Fig. 7B is a detail of the catheter apparatus of Fig. 7A.

Fig. 8A is a perspective view of a catheter apparatus with guidewire lumens coupled to an expandable mesh tip.

Fig. 8B is a detail of the catheter apparatus of Fig. 8A.

Fig. 8C illustrates the retraction of a retractable sheath from the catheter apparatus of Fig. 8A and Fig. 8B.

Fig. 8D illustrates the retraction of a retractable sheath as in Fig. 8C within a vasculature.

Fig. 9A is a perspective view of a catheter apparatus with expandable devices surrounding the lumen guidewires.

Fig. 9B illustrates the retraction of a retractable sheath from the catheter apparatus of Fig. 9A.

Fig. 10 illustrates the retraction of a retractable sheath from a catheter apparatus with shape-memory materials integrated with guidewire lumens.

Fig. 11 illustrates the retraction of a retractable sheath from a catheter apparatus and expansion of sponges surrounding guidewire lumens.

Fig. 12A is a perspective view of a loop embodiment in an expanded state.

Fig. 12B is an unwrapped view of the loop embodiment of Fig. 12A.

Fig. 12C is a distal end view of the loop embodiment of Fig. 12A.

Fig. 13 is an unwrapped view of another loop embodiment where loops may be located on any closed cell.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0019] Embodiments of the present invention may in-

clude apparatus and methods for advancing one or more guidewires through chronic total occlusions in vasculatures.

[0020] Embodiments of the present invention may incorporate several features to successfully pass one or more guidewires through a chronic total occlusion. Features of the present invention may include multiple lumens constructed within a catheter shaft, expansion or activation of a distal tip of a catheter apparatus for creating a scaffold effect, and/or decentralization of the guidewire lumens after activation or distal catheter repositioning for allowing multiple sections of a fibrous cap to be forcefully engaged by a guidewire. Embodiments of the present invention may optimize advancement of the one or more guidewires into multiple sections of a fibrous cap of a chronic total occlusion with reasonable force.

[0021] In embodiments of the present invention one or more over-the-wire lumens may be constructed within a shaft of a catheter apparatus. Embodiments of the present invention may preferably use two or more lumens. Larger vasculatures, such as coronary arteries, may accommodate higher profile catheters and allow use of additional lumens. Each lumen may accommodate at least a 0.014" diameter guidewire. Other sized lumens and guidewires may be accommodated based upon the desired end use. Standard off-the-shelf or customized guidewires may be used. For example, in addition to traditional guidewires, embodiments of the present invention may be used with guidewires including, but not limited to, steerable, hydrophilic, Teflon-coated, heparin-coated, ball-tip, J-tip, spiral tip, angulated wire and others.

[0022] Embodiments of the present invention may be combined with other types of catheter devices. The positioning systems and methods of the present invention may be to deliver and/or direct other catheters towards a desired position. For example, a vibrating catheter or other specialized catheter may be directed towards a chronic total occlusion or other location in a vasculature. A microcatheter with a distal positioning device, including, for example, one or more balloons that may be inflated individually, sequentially or simultaneously, or other features, may be placed in proximity to a chronic total occlusion. A positioning system may steer the microcatheter away from a wall of a vessel, as it probes a cap of a chronic total occlusion. Microcatheters with angulation or other features may be placed in proximity to a chronic total occlusion where the angulation steers away from a wall of a vessel, probes a cap of a chronic total occlusion or otherwise changes directions. A catheter portion and/or sheath of embodiments of the present invention may be large enough to deliver and/or position specialized catheters to a desired location. Positioning devices may then be used to position the specialized catheters in a beneficial manner for a procedure.

[0023] In particular, embodiments of the present invention may deliver energy via the guidewires through radio frequencies and/or lasers. Furthermore, other types of

energy may be delivered such as direct conductive heat energy, infrared or other types of energy that may be useful in particular applications. Various types of guidewires and/or delivering energy via guidewires may allow for various types of treatments. The external diameter of a catheter apparatus of the present invention may allow passage through a standard guide catheter. The outer surface of a catheter apparatus of the present invention may be coated with hydrophilic material to allow easier passage through the guide catheter. With alternate dimensions, the catheter apparatus of the present invention may be used in peripheral vessels. In this situation, a guide catheter may not be necessary to insert the device into the vasculature.

[0024] Figs. 1A - 1K show a self-expanding catheter apparatus 11. The external diameter of the self-expanding catheter apparatus 11 may pass through a sheath 19.

[0025] The sheath 19 may be a separate element surrounding the distal end of the catheter apparatus 11 to maintain the catheter apparatus 11 in an inactive state. The sheath 19 may have a rounded or tapered end for facilitating passage through a vasculature. Other end configurations are possible depending on particular uses.

[0026] Additional embodiments of the sheath may be shown in Figs. 1J - 1K. A sheath 68, 69 may be used to lower a profile of a self-expanding distal portion 13 of the catheter apparatus 11, which may preferably be a nitinol component, during insertion and removal of the catheter apparatus 11 from a vasculature. A sheath 68 may have a shorter configuration, as shown in Fig. 1J, covering at least a distal self-expanding component, preferably a nitinol element, on the catheter apparatus 11. The sheath 68, however, may preferably be long enough to correspond to the length of the treated vasculature, i.e., long enough to cover the portion of the catheter extending outside of a guide catheter and into the vasculature. This sheath configuration may function by insertion through a guide catheter and advancement into a treated vasculature. The sheath 68 may be attached 60 to a solid core guidewire and/or flexible device 67. The solid core guidewire and/or flexible device 67 may be long enough to traverse a guide catheter. The solid core guidewire and/or flexible device 67 may be a solid structure with no internal lumens and may preferably be made of plastic or similar materials. The solid core guidewire and/or flexible device 67 may be manipulated from outside the body, preferably by means of an expanded element 64 at a proximal end of the solid core guidewire and/or flexible device 67. The solid core element 67 may parallel the catheter apparatus 11 through a guide catheter. A distal portion 58 of the sheath 68 may be flared to fit a self-expanding portion 13 of the catheter apparatus device 11. The distal portion 58 may also have one or more radiopaque or other types of markers 54. The sheath 68 may have a stop point to allow withdrawal of the sheath 68 to a predetermined position, which may also facilitate resheathing of the catheter apparatus 11.

[0027] Alternatively, as shown in Fig. 1K, a sheath 69 may have a longer length, completely surrounding an intravascular portion of the catheter apparatus 11 during insertion and removal. The sheath 69 may be a flexible

5 with a roughly cylindrical shape. The sheath 69 may preferably be made of plastic or other similar materials. This sheath configuration may have a larger profile element 62 at an extra-vascular, proximal end, allowing for easier handling and movement of the sheath 69. A distal portion

10 66 of the sheath 69 may be flared to fit a self-expanding portion 13 of the catheter apparatus device 11. The distal portion 66 may also have one or more radiopaque or other types of markers 56. The sheath 69 may have a stop point to allow withdrawal of the sheath 69 to a pre-determined position, which may also facilitate resheathing of the catheter apparatus 11. The sheath 69 may be used in conjunction with a guide catheter or may function without a guide catheter in a non-coronary vasculature.

[0028] A body or shaft 23 of the catheter apparatus 11 15 may be made of a flexible plastic material or any other similar substance. A hydrophilic coating may or may not be added to the outer surfaces of the catheter apparatus 11. One or more hubs 21 corresponding to one or more guidewires 15 and one or more lumens 17 may be disposed at a proximate end 29 of the catheter apparatus 11.

[0029] The one or more hubs 21 may be marked, color-coded, numbered or may otherwise differentiate between one another. Identification of individual guidewire lumens may allow more effective use of embodiments of the present invention. With marking, users may improve their ability to identify which guidewire lumen may be preferably used during a procedure. For example, if a particular guidewire lumen is in a preferable location relative to other guidewire lumens an operator may desire a quick and reliable method of inserting a guidewire through that particular guidewire lumen. Marking may save time and effort by eliminating trial and error to determine a desired guidewire lumen. Alternatively, marking may be useful for applications other than treatment of occluded vasculatures, such as steering guidewires through vasculatures via various lumens. For example, marking can allow embodiments of the present invention to be used in other areas and/or conditions of a vasculature, such as traversing the tortuous coronary arteries. Distal and proximal ends of the guidewire lumens may be similarly marked to identify the guidewire lumens. Distal ends or structures on distal ends of the guidewire lumens may be marked such that the user may identify a preferred guidewire lumen while the catheter apparatus is within a patient. Marking with radiopaque or other types of markers may include temporary structures within the guidewire lumens. For example, markers may be present on stylets within the guidewire lumens. The stylets may be removed if desired to reduce mass or otherwise improve efficiency of a procedure.

[0030] The one or more hubs 21 may allow introduction of stylets or other structures that run through the catheter apparatus to render it stiff or to remove debris from its

lumen. The one or more hubs 21 may also allow passage of one or more guidewires 15.

[0031] Generally, a distal portion 13 of the catheter apparatus 11 may function as a scaffold-type structure. The distal portion 13 of the catheter apparatus 11 may stabilize the catheter apparatus 11 within a vasculature lumen as one or more guidewires 15 are advanced into a chronic total occlusion. One or more guidewires 15 may be threaded through one or more lumens 17 within the catheter apparatus 11.

[0032] The distal portion 13 of the catheter apparatus 11 is preferably self-expanding. Fig. 1B shows the distal end 25 of the catheter apparatus 11 in an expanded state. Fig. 1C shows a cross section of the catheter apparatus 11 with a retractable sheath 19 surrounding the body 23. The retractable sheath 19 may be retracted by moving the retractable sheath towards the proximate end 29 of the catheter apparatus 11. The distal portion 13 of the catheter apparatus 11 may include an activated scaffold structure 27 to stabilize the catheter apparatus 11. The activated scaffold structure 27 may expand to match a diameter of the vasculature lumen upon retraction of the retractable sheath 19.

[0033] Nitinol and/or stainless steel may be incorporated into the scaffold structure 27. Nitinol is an illustrative example of a shape memory alloy. Other shape memory alloys or other similar substances may be used. Generally, after a sample of a shape memory alloy has been deformed from its original crystallographic configuration, the shape memory alloy regains its original geometry by itself. This property of shape memory alloys may allow for expansion of the scaffold structure 27 after retraction of the retractable sheath 19. The nitinol and/or stainless steel scaffold structure 27 may create a stent-like mesh. The scaffold structure 27 may form the surface of the distal portion 13 of the catheter apparatus 11.

[0034] Fig. 1H shows an inactive scaffold structure 31. The inactive scaffold structure 31 may be advanced over a guidewire into a chronic total occlusion with a retractable sheath 19 in place to constrain the self-expanding but inactive scaffold structure 31. The retractable sheath 19 may cover the inactive scaffold structure 31. When the inactive scaffold structure 31 is properly positioned, the retractable sheath 19 may be retracted by an appropriate retraction means. As the retractable sheath 19 is retracted, the inactive scaffold structure 31 of the catheter apparatus 11 may become active and may flare out. During a flare out process, the inactive scaffold structure 31 may self-expand to assume a larger diameter to roughly approximate the diameter of the vasculature in the location of the distal portion 13 of the catheter apparatus 11.

[0035] The retraction of the retractable sheath 19 may be a continuous or step-wise process. For example, the retractable sheath 19 may be retracted in one operation by a user until the scaffold structure 31 is fully exposed. Alternatively, the retractable sheath 19 may be retracted in increments less than that required for full expansion of the scaffold structure 31. Stop points during retraction

of the retractable sheath 19 may allow for predetermined quantities of expansion of the scaffold structure 31. For example, if a procedure required less than full expansion of the scaffold structure 31, a stop point short of full retraction of the retractable sheath 19 may be chosen.

[0036] The conversion and expansion of the inactive scaffold structure 31 into an active scaffold structure 27 may create a relatively stable platform from which to advance the one or more guidewires 15 into multiple sections of the chronic total occlusion. The activated catheter apparatus 11 with the retractable sheath 19 retracted may have an activated scaffold structure shaped as a truncated cone or other suitable shape. A surface 33 of the expanded distal end 13 of the catheter apparatus 11 may consist of a "skin" of the scaffold structure 27. An end cap 35 may or may not cover the distal end 35 of the catheter apparatus 11. The end cap 35 may preferably be made of an impervious expandable polymer, but other similar substances may be used.

[0037] Fig. 1D shows an activated scaffold structure 27 that may be filled with an expandable polymer or similar material. The expandable polymer or similar material may fill the scaffold structure 27 to form a truncated, conical or other appropriate shape for securing the catheter apparatus 11 within the vasculature lumen. The expandable polymer may support distal portions of one or more guidewire lumens 17. Upon expansion of the expandable polymer, the embedded lumen ends 37 may flare out correspondingly with the end cap 35. Fig. 1E shows a cross section of the catheter apparatus 11 with the retractable sheath 19 surrounding the shaft 23. Fig. 1F shows an end view of the expanded end cap 35 with embedded guidewire lumens 17.

[0038] A skin 33 may surround the expandable polymer or similar material. The skin 33 may be a temporary metal "stent". The metal stent may be a mesh type structure. The metal stent may become a truncated conical shape after expansion or any other suitable shapes.

[0039] The a - b dimension 39 indicated in Fig. 1D may shorten when the retractable sheath 19 is removed from scaffold structure 27. The degree of shortening of the a - b dimension 39 may vary depending on the degree of expansion, the materials used, etc.

[0040] The retractable sheath 19 may be retracted to a stop point. The stop point may prevent over-retraction of the retractable sheath 19. A retractable sheath 19 at the stop point may facilitate re-sheathing of the scaffold structure 27.

[0041] Fig. 1G shows multiple guidewire lumens 17 that may be suspended within a scaffold structure 27 without using an expandable polymer or similar filler. A skin 33 may be made of nitinol, stainless steel, or another expansible substance. The one or more guidewire lumens 17 may extend to the distal end 25 of the scaffold structure 27. The scaffold structure 27 may begin roughly at a transition point 41. The one or more guidewire lumens 17 may or may not be embedded in an end cap 35. The end cap may be an impervious plastic material.

[0042] Fig. 11 shows a catheter apparatus with an expandable skin 33 and a deflectable tip 43. The deflectable tip 43 may be rotatable or otherwise moveable. The deflectable tip 43 may be rotatable with a rotator 45 or other similar device at the proximate end 29 of the catheter apparatus 11. The embodiment depicted in Fig. 11 preferably does not include an end cap 35. The lack of an end cap 35 may allow for freedom of movement of the deflectable tip 43. The distal portion 13 of the catheter apparatus 11 may flare after the retractable sheath 19 is retracted. A single, centrally located deflectable lumen 47 may allow a guidewire 15 to be advanced in numerous planes. The deflectable tip 43 may allow for controlled probing of the fibrous cap of a chronic total occlusion.

[0043] Other embodiments of the present invention may include one or more balloons at or near a distal end of a catheter apparatus. The one or more balloons may be circumferential. Alternatively, the one or more balloons may be offset and placed longitudinally. Other positions and arrangements are possible depending on particular situations.

[0044] Fig. 2A shows an embodiment of the present invention with a balloon 53 that may be placed longitudinally near a distal tip 55 of a catheter apparatus 51. The balloon 53 may parallel the long axis of a shaft 59 of the catheter apparatus 51. Inflation of the balloon 53 may deflect the position of one or more guidewire lumens 57 relative to the fibrous cap of a chronic total occlusion. The balloon 53 may be inflated to a diameter that may buttress the catheter apparatus 51 against a wall of the vasculature lumen. The balloon 53 may then be deflated, the catheter apparatus 51 rotated, and the balloon 53 reinflated.

[0045] Fig. 2B shows a cross section of the catheter apparatus 51. The balloon 53 may be inflated and deflated through an inflation port 65. The inflation port 65 may pass through the shaft 59 to connect the balloon 53 to a proximate end 63 of the catheter apparatus 51. This method may result in one or more guidewires 59 probing various sections of the fibrous cap. One or more hubs 61 at the proximate end 63 of the catheter apparatus 51 may allow passage of the one or more guidewires 59. Stylets or other similar structures may be inserted or reinserted into the catheter apparatus 51 to facilitate rotation.

[0046] Fig. 3A shows an embodiment of the present invention with a first longitudinal balloon 73 and a second longitudinal balloon 75 positioned near a distal end 77 of a catheter apparatus 71. More balloons may be used for additional or different control of the catheter apparatus. The multiple balloons 73, 75 may be inflated individually, simultaneously, alternatively or sequentially depending on the particular circumstances. The pattern of inflation and/or deflation of the multiple balloons 73, 75 may allow redirection of a distal catheter tip 79 relative to a fibrous cap of a chronic total occlusion. Repositioning of the distal catheter tip 79 may permit more complete interrogation of the fibrous cap with one or more guidewires 81. One or more hubs 83 at the proximate end 85 of the catheter

apparatus 71 may allow passage of the one or more guidewires 81 through a shaft 87.

[0047] Fig. 3B shows a cross section of the catheter apparatus 71. One or more guidewire lumens 89 may pass through the catheter apparatus 71. Embodiments of the present invention may be constructed with multiple inflation ports (not shown) or with one inflation port 91 servicing the multiple balloons 73, 75. If the later option is utilized, the balloon materials may be constructed to allow selective, and/or sequential inflations at increasing balloon pressures. The balloons 73, 75 may be positioned at various angles relative to one another around the circumference of the shaft 87.

[0048] Fig. 4A shows an embodiment of the present invention with a balloon 103 with a distal surface 105 in a catheter apparatus 101. The balloon 103 may be flat, cylindrical or any other suitable configuration. Additionally, the balloon 103 may be sectioned. One or more guidewire lumens 107 may be extruded through the balloon material. The balloon 103 may be inflated to match the inner diameter of the vasculature lumen. Fig. 4B shows an end view of the catheter apparatus 101. As the balloon 103 expands, the one or more guidewire lumens 107 extruded through the balloon 103 may diverge relative to one another in reaction to expansion of the balloon 103. The divergence may allow one or more guidewires 109 to probe various sections of the fibrous cap of the chronic total occlusion. One or more hubs 111 at the proximate end 113 of the catheter apparatus 101 may allow passage of the one or more guidewires 109. Fig. 4C shows a cross section of the catheter apparatus 101. A balloon inflation port 115 may pass through a shaft 117 with the one or more lumens 107 to inflate and/or deflate the balloon 103.

[0049] Fig. 5A shows a catheter apparatus 121 with an inner core 123 within an outer core 125. The inner core 123 may contain one or more lumens 127. Embodiments of the present invention may preferably include two or more lumens 127. Fig. 5B illustrates an embodiment with two lumens placed at positions of 3 o'clock and 9 o'clock within the inner core 123. Other quantities of lumens 127 and positions are contemplated for various applications and situations. The inner core 123 may be rotated within the outer shell 125 of the catheter apparatus 121 by turning or otherwise manipulating a rotator 129 at a proximate end 131 of the catheter apparatus 121. The rotator 129 may be coupled 133 or otherwise connected to the inner core 123. One or more guidewires 135 may be connected to one or more hubs 137 at the proximate end 131 of the catheter apparatus 121. The one or more guidewires may extend from a distal end 139 of the catheter apparatus 121.

[0050] A rotatable inner core 123 of catheter apparatus 121 may be used in conjunction with the various balloon configurations described above. For example, if constructed with a non-longitudinal stabilizing balloon, the shape of the distal tip balloon may be circumferential, i.e., doughnut-shaped.

[0051] Fig. 6A shows an embodiment of the present invention with a single stabilizing balloon 143 and a deflecting tip 145 on a catheter apparatus 141. The single stabilizing balloon 143 may be used in conjunction with a deflectable distal catheter tip 145 for eccentric placement of one or more guidewires 147. The one or more guidewires 147 may be passed through one or more hubs 149 at a proximate end 151 of the catheter apparatus 141. Fig. 6B shows a cross section of the catheter apparatus 141. One or more lumens 153 may pass through a shaft 155. An inflation port 157 may allow inflation and/or deflation of the stabilizing balloon 143. The deflecting tip 145 may be located at various angles depending on the particular situation.

[0052] Catheter apparatus shafts 23, 59, 87, 117, 12 and 155 may be constructed with either a circular, oval or rectangular shape. Other shapes are possible depending on particular uses.

[0053] Fig. 7A shows an embodiment of the present invention with an expandable portion 159 at a distal tip 161 of a catheter apparatus 163. The expandable portion 159 may be a mesh or other similar configuration as described above. The expandable portion 159 may be expanded by retracting a retracting sheath 165 away from the distal tip 161 of the catheter apparatus 163. The expandable portion 159 may be expanded into contact with a wall of a vasculature.

[0054] Fig. 7B shows a detail of the catheter apparatus 163. A central core 167 may contain one or more guidewire lumens 169. The central core 167 may or may not be expandable. The central core 167 may be rotatable to allow one or more guidewires 169 to probe various sections of a fibrous cap. One or more hubs 171 at the proximate end 173 of the catheter apparatus 163 may allow passage of the one or more guidewires 169.

[0055] Fig. 8A shows an embodiment of the present invention with an expandable portion 175 at a distal tip 177 of a catheter apparatus 179. The expandable portion 175 may be a mesh or other similar configuration as described above. The expandable portion 175 may be expanded by retracting a retracting sheath 181 away from the distal tip 177 of the catheter apparatus 179. The expandable portion 175 may be expanded into contact with a wall of a vasculature. One or more hubs 185 at the proximate end 187 of the catheter apparatus 179 may allow passage of the one or more guidewires 189.

[0056] Fig. 8B shows a detail of the catheter apparatus 179. One or more guidewire lumens 183 may be formed of extruded plastic or similar materials. The figures generally illustrate three guidewire lumens 183, but other numbers and configurations may be desirable depending on particular uses. The one or more guidewire lumens 183 may have shape-memory alloys or other similar materials integrated into, surrounding or within the structure of the one or more guidewire lumens 183. Preferably, the one or more guidewire lumens 183 may self-expand upon retraction of the retraction sheath 181 such that ends 182 of the one or more guidewire lumens are spaced apart

and approximately halfway between the center point and the inner surface of a vasculature. The one or more guidewire lumens 183 may be configured to expand into various predetermined positions and configurations depending on particular applications. For example, Fig. 8B shows a triangular configuration for the guidewire lumens 183. Other configurations are possible using three guidewire lumens 183. Furthermore, different numbers of guidewire lumens may be used in various configurations.

[0057] Alternatively, the one or more guidewire lumens 183 may be coupled to an inner surface of the expandable portion 175. The one or more guidewire lumens 183 may be adhered or integrally molded to the inner surface of the expandable portion 175.

[0058] Expansion of the expandable portion 175 may cause the one or more guidewire lumens 183 to separate via a self-expanding shape-memory material. Alternatively, the one or more guidewire lumens 183 may not be coupled to the expandable portion 175 but may instead be positioned within the internal volume of the expandable section 175 to allow probing of a fibrous cap. Additionally, a self-expanding polymer may fill the expandable portion 175. In an initial configuration the self-expanding polymer may be in a compressed state. As the expandable portion 175 is released from the retracting sheath 181, the self-expanding polymer may expand as well. The one or more guidewire lumens 183 may be embedded in the self-expanding polymer and may be moved into a desired position by the expansion of the self-expanding polymer. The self-expanding polymer may expand by absorbing moisture or blood from within the vasculature or through other expansion mechanisms. The self-expanding polymer may then be removed after a procedure.

[0059] Fig. 8C illustrates the operation of the catheter apparatus 179 of Fig. 8A and Fig. 8B. Similar operational procedures may be used for other embodiments described herein. Step 1 of Fig. 8C shows the catheter apparatus 179 in an initial state with a retractable outside sheath 181 moved as far as possible distally from a guidewire lumen tube 191. Steps 2 - 7 show incremental stages of retraction of the retractable outside sheath 181. As the retractable outside sheath 181 is retracted back over the guidewire lumen tube 191, the expandable portion 175 is incrementally exposed and allowed to expand. As the expandable portion 175 expands the one or more guidewire lumens 183 separate and are held in a desired position by the shape-memory allow materials or by coupling to the expandable portion 175. Step 7 shows the expandable portion 175 in a fully deployed state. The end view of Fig. 8C shows the one or more guidewire lumens 183 in the fully deployed state. Step 8 shows a guidewire 189 inserted through a guidewire lumen 183. Fig. 8D illustrates the operation of the catheter apparatus 179 as shown in Fig. 8C within a vasculature 184 with an occlusion 186.

[0060] Fig. 9A shows an embodiment of the present invention with one or more inflatable devices 193 sur-

rounding one or more guidewire lumens 195 within an expandable portion 197 of a catheter apparatus 199. The expandable portion 197 may be a mesh or other similar configuration as described above. The expandable portion 197 may be expanded by retracting a retracting sheath 201 away from a distal tip 203 of the catheter apparatus 199. The expandable portion 197 may be expanded into contact with a wall of a vasculature. The expandable portion 197 may be omitted as shown in Fig. 9B.

[0061] The inflatable devices 193 may initially be in a deflated condition during insertion and positioning of the catheter. The inflatable devices 193 preferably are balloons, but may be any other expandable type of device. The balloons may surround the outer surface of the one or more guidewire lumens 195. The balloons may be cylindrical or other shapes to position the one or more guidewire lumens 195 within the expandable portion 197. The inflatable devices 193 may include one balloon for each guidewire lumen 195 or one balloon may correspond to several guidewire lumens 195. For example, a single inflatable device 193 may be inflated to separate all of the guidewire lumens 195. Alternatively, two separate inflatable devices 193 may be used to separate three or more guidewire lumens. The inflatable devices 193 may be bifurcated or trifurcated depending on the number of guidewire lumens 195 and the particular application. The expandable sheath 197 may assist in containing multiple, separate inflatable devices 193, but may not be essential to the operation of the present invention.

[0062] One or more ports (not shown) may allow inflation or one or more of the inflatable devices 193 depending on the number of separate inflatable devices 193. For example, one port may be used to inflate one inflatable device 193. Alternatively, if two or more separate inflatable devices 193 are present, then two or more ports may be used to inflate and deflate the inflatable devices 193 serially or in parallel depending on a particular use or condition. Different numbers and combinations of inflatable devices and ports may be possible. Inflation of various combinations of inflatable devices 193 with various numbers and configurations of ports may allow for probing of a fibrous cap. If ends of the one or more guidewire lumens 195 or the inflatable devices 193 themselves are marked, a user may inflate specific inflatable devices 193 but not others to more accurately interrogate an occlusion. Each of the inflatable devices 193 may be inflated into contact with the expanded expandable portion 197 to secure the position of the one or more guidewire lumens 195. Guidewires (not shown) may then be passed through the one or more guidewire lumens 195. The inflatable devices 193 may be deflated prior to withdrawing the catheter apparatus 199.

[0063] As shown in Fig. 9B an embodiment of the present invention may include the inflatable devices 193 without the expandable portion 197, as shown in Fig. 9A. The inflatable devices 193 may be exposed by withdrawing the retracting sheath 201. Particularly if the inflatable

devices 193 are unitary, the expandable portion 197 may not be needed. However, even if the inflatable devices 193 are separate the expandable portion 197 may be omitted.

5 **[0064]** Step 1 of Fig. 9B shows the catheter apparatus 199 in an initial state with a retractable outside sheath 201 moved as far as possible distally from a guidewire lumen tube 205. Steps 2 - 4 show incremental stages of retraction of the retractable outside sheath 201 to expose

10 the one or more guidewire lumens 195 with corresponding inflatable devices 193. Steps 5 - 6 show incremental stages of inflation of the inflatable devices 193 into a final position with a vasculature 209 with an occlusion 211. Step 7 shows the catheter apparatus 199 in a fully deployed state. Step 8 shows a guidewire 207 inserted through a guidewire lumen 195.

[0065] Fig. 10 illustrates operation of a catheter apparatus 213 that may include shape-memory materials integrated with the one or more guidewire lumens 217.

20 Preferably, the one or more guidewire lumens 217 may be constructed out of extruded plastic or other similar materials. Shape-memory or other expandable materials may be integrated into, surround, be contained within or reinforce the one or more guidewire lumens 217.

25 **[0066]** Step 1 of Fig. 10 shows the catheter apparatus 213 in an initial state with a retractable outside sheath 215 moved as far as possible distally from a guidewire lumen tube 215. The one or more guidewire lumens 217 may be exposed by withdrawing the retracting sheath

30 215 from the distal end of a catheter apparatus 213 as shown in Steps 2 - 6. The one or more guidewire lumens 217 may then assume a final spaced or relaxed configuration as shown in Step 7. The guidewire lumens may move outward relative to one another a desired distance

35 and/or into contact with inner walls of a vasculature 219 with an occlusion 221. A guidewire 223 may then be threaded through the one or more guidewire lumens 217 as shown in Step 8. After completion of a procedure, the retracting sheath 215 may be advanced towards the distal end of the catheter apparatus to compress the one or

40 more guidewire lumens 217 into a compact arrangement for removal from the vasculature 219. Alternatively, the one or more guidewire lumens 217 may be withdrawn into the distal end of the retracting sheath 215 before removal from the vasculature 219.

[0067] Fig. 11 illustrates operation of a catheter apparatus 225 with expandable devices 227 surrounding one or more guidewire lumens 229. Preferably, the expandable devices 227 are sponges or other materials that expand within the vasculature without input from a user. Each guidewire lumen 229 may have a separate expandable device 227 or multiple guidewire lumens may be incorporated into one expandable device 227.

[0068] Step 1 of Fig. 11 shows the catheter apparatus 225 in an initial state with a retractable outside sheath 231 moved as far as possible distally from a guidewire lumen tube 233. The one or more guidewire lumens 229 may be exposed by withdrawing the retracting sheath

231 from the distal end of a catheter apparatus 225 as shown in Steps 2 - 6. As the retracting sheath 231 is withdrawn from the expansible devices 227, the expansible devices 227 begin to expand. If the expansible devices 227 are sponges, the expansible devices 227 may absorb moisture from the vasculature to increase in volume. The one or more guidewire lumens 229 may then assume a final expanded configuration as shown in Step 7. The guidewire lumens 229 embedded with the expansible devices 227 may move outward relative to one another a desired distance and/or into contact with inner walls of a vasculature 233 with an occlusion 235. A guidewire 237 may then be threaded through the one or more guidewire lumens 229 as shown in Step 8. After completion of a procedure, the retracting sheath 231 may be advanced towards the distal end of the catheter apparatus 225 to compress the one or more guidewire lumens 229 into a compact arrangement for removal from the vasculature 233. Alternatively, the one or more guidewire lumens 229 may be withdrawn into the distal end of the retracting sheath 231 before removal from the vasculature 233. Movement of the retracting sheath 231 may compress the expansible devices 227 into a position suitable for removal from the vasculature 233. If the expansible devices 227 are sponges, the compression may force moisture out of the sponges.

[0069] Generally, after crossing a chronic total occlusion with a guidewire, the catheter apparatus may be resheathed and removed from the vasculature. The guidewire may be left in position.

[0070] One or more guidewires preferably remain in or near the longitudinal axis of the corresponding support catheter lumen. This positioning of the one or more guidewires may optimize the force of the one or more guidewires when engaged with the fibrous cap of the chronic total occlusion. Multiple eccentrically located guidewire lumens may improve the chance of success in passing one or more guidewires through a chronic total occlusion. The mass of the multi-lumen support catheter may provide additional support for the guidewire and prevents off-axis, i.e., lateral, displacement of portions of the one or more guidewires located in the guide catheter and in the vasculature. Eccentric distribution of the one or more guidewire lumens may allow engagement of multiple, eccentric sections of the fibrous cap. Embodiments of the present invention may permit simultaneous placement of multiple guidewires. Multiple guidewires may enhance available techniques such as "parallel guidewire" and "see-saw" wire.

[0071] Fig. 12A shows a catheter apparatus 241 with guidewire lumens 243, 245, 247 passing through loops 249, 251, 253, 255, 257, 259. The number and configuration of the loops or guidewire lumens 243, 245, 247 may be variable. Alternative numbers and configurations are possible. Guidewire lumens 243, 245, 247 may be guided into a predetermined position during expansion of an expansible support structure 261 by threading the guidewire lumens 243, 245, 247 through the inwardly pro-

jecting loops 249, 251, 253, 255, 257, 259. Loops 249, 251, 253, 255, 257, 259 may be coupled to the expansible support structure 261. Figs. 12A - 12C illustrate an embodiment of the present invention where each guidewire lumen 243, 245, 247 may pass through two loops 249, 251, 253, 255, 257, 259. Alternative embodiments may only use one loop for each guidewire lumen. Still other alternative embodiments may use three or more loops for each guidewire lumen. The operation of the loops and guidewire lumens in Figs. 12A - 12C are illustrative of the alternative embodiments. The guidewire lumens 243, 245, 247 are guided into position by passing through the loops 249, 251, 253, 255, 257, 259. The expansible support structure 261 may be coupled to a main multi-lumen shaft 263 by any conventional means such as adhesive, welding, etc. In the current embodiment of the invention, three guidewire lumens 243, 245, 247 are shown, but other numbers and configurations of lumens may be provided. A sheath 265 may hold the expansible support structure 261 in a compressed state prior to deployment of the expansible support structure 261.

[0072] Fig. 12B shows a flat projection of the expansible support structure 261 with loops 249, 251, 253, 255, 257, 259. Figs. 12A - 12C show a five closed-cell configuration. Embodiments of the present invention may include different quantities of closed-cells depending on desired applications. Fig. 12B shows a first closed cell 265, a first connector region 267, a second closed cell 269, a second connector region 271, a third closed cell 273, a third connector region 275, a fourth closed cell 277, a fourth connector region 279, and a fifth closed cell 281. In Fig. 12B, the first closed cell 265 may be at a distal end of the catheter apparatus 241 and the fifth closed cell 281 may be located towards a proximal end of the catheter apparatus 241. In each closed cell, struts 283 may form a zigzag pattern to support the catheter apparatus 241. Connectors 285 residing in the first connector region 267 may connect the first closed cell 265 to the second closed cell 269 by linking strut intersections 287 on the first closed cell 267 with strut intersections 289 on the second closed cell 271. Connectors 285 may be thinner than struts 283 and the angular relationship between struts 283 and connectors 285 may change during expansion and compression of the expansible support structure 261. Similar structures and interactions may be found in and between the remaining closed cells.

[0073] Loops 249, 251, 253, 255, 257, 259 may be located at strut intersections 291. Loops 249, 251, 253, 255, 257, 259 may be coupled to the strut intersections 291 by loop supports 293. Loop supports 293 may be tapered to reduce stress on the apparatus. Struts 283 may also be tapered to reduce stress on the apparatus. The loop supports 293 may be positioned at other locations along the struts 283 or connectors 285 if desired. Loops 249, 251, 253, 255, 257, 259 and inner shape cutouts may be circular, oval, oblong or any additional shapes to allow the guidewire lumens 243, 245, 247 to slide within the loops 249, 251, 253, 255, 257, 259.

Shapes other than circles may be beneficial when the loops 249, 251, 253, 255, 257, 259 lie at an angle other than perpendicular to the cylindrical plane of the expandable support structure 261. Loops 249, 251, 253, 255, 257, 259 may be shaped to correspond to guidewire lumens 243, 245, 247 and allow the guidewire lumens 243, 245, 247 to slide through the loop openings.

[0074] Each guidewire lumen 243, 245, 247 may pass through two loops in the embodiment of Figs. 12A - 12C. For example, guidewire lumen 243 may pass through loops 249 and 251, guidewire lumen 245 may pass through loops 253 and 255, and guidewire lumen 247 may pass through loops 257 and 259. Passing the guidewire lumens 243, 245, 247 through the loops 249, 251, 253, 255, 257, 259 may position the guidewire lumens 243, 245, 247 in a desired position within the expandable support structure 261. As indicated above, other numbers and configurations of loops are possible.

[0075] To prevent twisting and damage to the guidewire lumens 243, 245, 247, the loops 249, 251, 253, 255, 257, 259 for each guidewire lumen are preferably located on every other closed cell. As shown in Fig. 12B, the loops 249, 251, 253, 255, 257, 259 are located on the first closed cell 265 and the third closed cell 273. The loops 249, 251, 253, 255, 257, 259 may also be located on, for example, the second closed cell 269 and the fourth closed cell 277. If additional loops are present, then the loops may be located on closed cells separated by one closed cell. This alternating structure may prevent twisting during expansion and compression of the expandable support structure 261 that may damage or misalign the guidewire lumens 243, 245, 247. Preferably, no loops 249, 251, 253, 255, 257, 259 may be located on the fifth or proximal closed cell 281. The fifth closed cell 281 may be adhered to the main tri-lumen shaft 263. Thus, the fifth closed cell 281 may not fully expand during expansion of the expandable support structure 261 and may not be appropriate for holding loops 249, 251, 253, 255, 257, 259. Similarly, the fourth closed cell 277 may not fully expand and may also not be suitable for holding loops.

[0076] The expandable support structure 261, the guidewire lumens 243, 245, 247, and the loops 249, 251, 253, 255, 257, 259 may initially be in a compressed state within a sheath 265 as described in previous embodiments. The sheath 265 may hold the expandable support structure 261 in a compressed state. The sheath 265 may include a radiopaque marker at a distal end of the sheath 265 or another known location along the sheath 265. The radiopaque marker may provide an indication of how much of the expandable support structure 261 is covered by the sheath 265. This may allow for partial withdrawal of the sheath 265.

[0077] The expandable support structure 261 may be made of Nitinol or another shape-memory material. The loop connectors 293 may also be made of Nitinol or another shape-memory material. The loop connectors 293 may be set to project inwardly from the cylindrical plane of the expandable support structure 261 at a given angle.

The angle may be any angle, but is preferably approximately 30 degrees inward from the cylindrical plane. The angle or the length of the loop connectors 293 or both may be varied to create various positions of the guidewire

5 lumens 243, 245, 247 within the expandable support structure 261. The loops 249, 251 corresponding to a guidewire lumen 243 may project in opposite directions, for example, loop 249 may project in a distal direction and loop 251 may project in a proximal direction.

10 **[0078]** When the sheath 265 is withdrawn from around the expandable support structure 261, the expandable support structure 261 may expand to an expanded state. The sheath 265 may be partially or completely withdrawn from the expandable support structure 261. During ex-

15 pansion of the expandable support structure 261, the loops 249, 251, 253, 255, 257, 259 may project inward from the cylindrical plane of the expandable support structure 261 to hold the guidewire lumens 243, 245, 247 in a predetermined position within the expandable support

20 structure 261. The guidewire lumens 243, 245, 247 may remain within the loops 249, 251, 253, 255, 257, 259 during expansion and compression of the expandable support structure 261. Also during expansion, the angle of the connectors 285 relative to the closed cells may

25 change. Placing the loops 249, 251, 253, 255, 257, 259 on closed cells separated by one closed cell may keep the guidewire lumens 243, 245, 247 from twisting. As the expandable support structure 261 expands, the guidewire lumens 243, 245, 247 may diverge into predetermined positions. The expanded catheter apparatus 241 may not block the vasculature.

30 **[0079]** Upon completion of a procedure, the expandable support structure 261 may be compressed and withdrawn from the vasculature. The sheath 265 may be slid distally over the expandable support structure 261. Preferably, no parts of the catheter apparatus 241 extend outside of the cylindrical plane of the compressed expandable support structure 261 in the compressed state to facilitate withdrawal of the catheter apparatus 241.

35 **[0080]** Fig. 13 shows another loop embodiment of an expandable structure 295. In contrast to the loop embodiment 241 of Figs. 12A - 12C, the loop embodiment of the expandable structure 295 of Fig. 13 may have loops 297, 299, 301, 303, 305, 307 attached on any of closed cell 309, 311, 313, 315. The operation of the apparatus of the loop embodiment of the expandable structure 295 is similar to the operation of the loop embodiment 241 of Figs. 12A - 12C.

40 **[0081]** To prevent twisting and damage to guidewire lumens 243, 245, 247, connecting members 317 may couple connection points 319 of struts 321 on a closed cell, such as 309, to connection points 323 of struts 321 on an adjacent closed cell, such as 311. The connection points 319, 323 are preferably both distal or both proximal relative to the distal end of the catheter apparatus 295. The number and configuration of the connecting members 317 may be variable. The connecting members 317 may have an upward bend 325 and a downward bend

327. The bends 325, 327 prevent twisting and damage to the guidewire lumens 243, 245, 247 during expansion and contraction of the expandable structure 295. During expansion and contraction of the expandable structure 295, the upward bend 325 and the downward bend 327 cancel and lateral movement of the loops 297, 299, 301, 303, 305, 307.

[0082] The connecting members 317 of the expandable structure 295 may allow loops on each closed cell 309, 311, 313, 315. Loops 297, 299, 301, 303, 305, 307 do not need to be on every other closed cell 309, 311, 313, 315. The embodiment of Fig. 13 may provide for flexibility of the expandable structure 295 and may facilitate expansion and contraction during deployment and removal.

[0083] Although the foregoing description is directed to the preferred embodiments of the invention, it is noted that other variations and modifications will be apparent to those skilled in the art, and may be made without departing from the spirit or scope of the invention. Moreover, features described in connection with one embodiment of the invention may be used in conjunction with other embodiments, even if not explicitly stated above.

[0084] Particular embodiments of the invention are described further in the following clauses:

1. A catheter apparatus comprising:

a flexible shaft,
guidewire lumens passing longitudinally through the shaft, and
a positioning means for positioning distal ends of the guidewire lumens relative to an inner wall of an external lumen.

2. The apparatus of clause 1, further comprising a retractable sheath surrounding the guidewire lumens.

3. The apparatus of clause 2, wherein the retractable sheath is coupled to at a proximal end of the retractable sheath to a guidewire.

4. The apparatus of clause 2, wherein the retractable sheath surrounds the guidewire lumens over a total length of the guidewire lumens within the external lumen.

5. The apparatus of clause 2, further comprising a manipulating means coupled to the retractable sheath for manipulating the retractable sheath.

6. The apparatus of clause 2, further comprising one or more markers on the retractable sheath.

7. The apparatus of clause 1, wherein the positioning means is an expandable scaffold.

8. The apparatus of clause 7, wherein the guidewire

lumens are coupled to the expandable scaffold.

9. The apparatus of clause 1, wherein the positioning means is one or more sponges.

10. The apparatus of clause 9, wherein the guidewire lumens are embedded in the one or more sponges.

11. The apparatus of clause 1, wherein the positioning means is a shape-memory means integrated with the guidewire lumens.

12. The apparatus of clause 1, wherein the positioning means is a deflectable tip on one or more guidewires passing through the one or more guidewire lumens.

13. The apparatus of clause 1, wherein the positioning means is one or more balloons.

14. The apparatus of clause 13, wherein the one or more balloons are inflated through an inflation port running longitudinally in the shaft.

15. The apparatus of clause 13, wherein the one or more balloons is a balloon with a substantially planar distal surface.

16. The apparatus of clause 15, wherein the guidewire lumens are extruded through the distal surface of the balloon.

17. The apparatus of clause 13, wherein the one or more balloons surround distal ends of the guidewire lumens.

18. The apparatus of clause 1, wherein the positioning means is a rotatable core within the shaft, lumens.

19. The apparatus of clause 1, wherein the shaft is coated with a hydrophilic material.

20. The apparatus of clause 1, wherein the guidewire lumens are adapted to be positioned eccentrically relative to an inner wall of an external lumen.

21. A catheter apparatus comprising:

a shaft,
guidewire lumens passing longitudinally through the shaft, and
an expandable distal portion of the shaft.

22. The apparatus of clause 21, further comprising a retractable sheath covering the expandable distal portion of the shaft.

23. The apparatus of clause 22, wherein retracting

- the retractable sheath from the expandible distal portion of the shaft activates the expandible distal portion of the shaft causing expansion of the expandible distal portion of the shaft. 5
24. The apparatus of clause 21, further comprising an end cap on the distal end of the expandible distal portion of the shaft. 10
25. The apparatus of clause 24, wherein the guidewire lumens are embedded in the end cap. 10
26. The apparatus of clause 21, further comprising an expandible plastic within the expandible distal portion of the shaft. 15
27. The apparatus of clause 21, wherein the expandible distal portion of the shaft is a metal mesh. 15
28. The apparatus of clause 21, further comprising a rotatable inner core within the shaft and wherein the guidewire lumens are within the rotatable inner core. 20
29. The apparatus of clause 21, further comprising guidewires in the guidewire 25
30. The apparatus of clause 29, further comprising a deflectable tip at the distal end of the guidewires. 30
31. The apparatus of clause 30, wherein the deflectable tip is rotatable with a rotator near a proximal end of the shaft. 30
32. A catheter apparatus comprising: 35
- a shaft,
guidewire lumens passing longitudinally through the shaft,
one or more balloons coupled to a distal end of the shaft, and
one or more inflation port passing through the shaft and connecting the one or more balloons to a proximate end of the shaft. 40
33. The apparatus of clause 32, wherein the one or more balloons is a single longitudinal balloon. 45
34. The apparatus of clause 32, wherein the one or more balloons is two or more longitudinal balloons disposed around the circumference of the shaft. 50
35. The apparatus of clause 32, wherein the one or more balloons is a single balloon with a distal surface. 55
36. The apparatus of clause 35, wherein the guidewire lumens are extruded through the balloon
- material. 5
37. The apparatus of clause 32, further comprising a rotatable inner core within the shaft and wherein the one or more guidewire lumens are within the rotatable inner core. 10
38. The apparatus of clause 32, further comprising a deflectable tip at the distal end of the shaft. 10
39. A catheter apparatus comprising:
- a multi-lumen main shaft;
one or more guidewire lumens extending from a distal end of the multi-lumen shaft with lumens within the one or more guidewire lumens contiguous with at least one of the multi-lumens of the multi-lumen main shaft;
an expandible support structure coupled to the distal end of the multi-lumen shaft;
one or more loops corresponding to each of the one or more guidewire lumens, wherein the one or more loops corresponding to each of the one or more guidewire lumens are coupled to the expandible support structure, and wherein the one or more loops corresponding to each of the one or more guidewire lumens project inward from the plane of the expandible support structure; and
wherein the one or more guidewire lumens are threaded through the corresponding one or more loops. 15
40. The apparatus of clause 39, wherein the one or more loops are coupled to the expandible support structure by loop connections. 15
41. The apparatus of clause 39, further comprising a sheath surrounding the expandible support structure when the expandible support structure is in a compressed state. 20
42. The apparatus of clause 41, wherein the sheath may be withdrawn from around the expandible support structure to expand the expandible support structure. 20
43. The apparatus of clause 42, wherein the sheath may be advanced around the expandible support structure to compress the expandible support structure. 20
44. The apparatus of clause 39, wherein the expandible support structure comprises closed cells. 20
45. The apparatus of clause 44, wherein the one or more loops are located on closed cells separated by one closed cell. 20

46. The apparatus of clause 44, wherein the proximal closed cell is coupled to the multi-lumen main shaft.

47. The apparatus of clause 44, wherein the closed cells comprise zigzag struts.

48. The apparatus of clause 47, further comprising connectors between the struts of a closed cell and the struts of a neighboring closed cell.

Claims

1. A catheter apparatus for advancing a guidewire through a chronic total occlusion in a vasculature comprising:

shaft 11 having a distal portion 13;
an removable, expandable scaffold structure 27
coupled to the distal portion 13 of shaft 11; and
a single, centrally located lumen 47 passing centrally through shaft 11 and through the expandable scaffold structure 27 and configured to pass over a guidewire.

2. The catheter apparatus of claim 1, wherein the expandable scaffold structure 27 comprises a skin 33.

3. The catheter apparatus of claim 2, wherein the skin comprises an expandable substance, nitinol or stainless steel.

4. The catheter apparatus of claim 1, wherein the lumen 47 is a deflectable lumen.

5. The catheter apparatus of claims 1 or 4, wherein the lumen 47 has tip 43.

6. The catheter apparatus of claim 5, wherein the tip 43 is a deflectable tip.

7. The catheter apparatus of claims 5 or 6, wherein the tip 43 is rotatable or movable.

8. The catheter apparatus of claim 1 further comprising a retractable sheath 19 configured for passing over the shaft and covering the expandable scaffold structure 27.

9. The catheter apparatus of claim 8, wherein retracting the retractable sheath 19 activates the expandable scaffold structure 27 causing expansion of the expandable scaffold structure 27.

10. The apparatus of claim 9, wherein advancing the retracted retractable sheath 19 causes contraction of the expandable scaffold structure 27.

11. The catheter apparatus of claim 9, wherein the lumen is configured to be advanced through one or more planes.

5 12. The apparatus of claim 9, wherein the lumen is configured to be advanced through a centrally located plane.

10 13. The apparatus of claim 1, wherein the expandable support structure 27 comprises an expandable substance, nitinol or stainless steel.

15 14. The apparatus of claim 1, wherein the expandable support structure 27 comprises a shape-memory material integrated with the lumen 47.

15 15. The catheter apparatus of any of the preceding claims further comprising a guidewire passing through lumen 47.

25

20

30

35

40

45

50

55

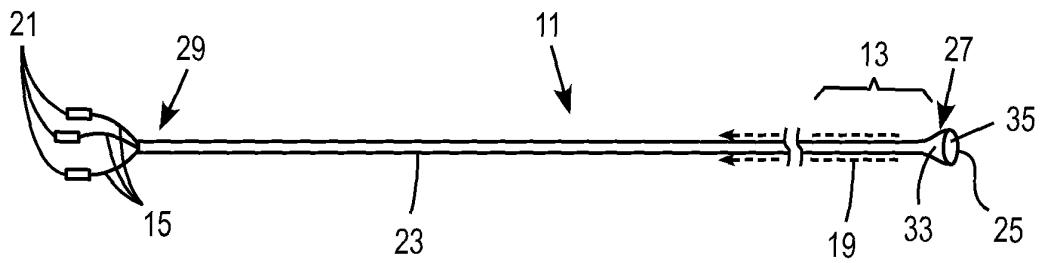


FIG. 1A




FIG. 1B




FIG. 1C

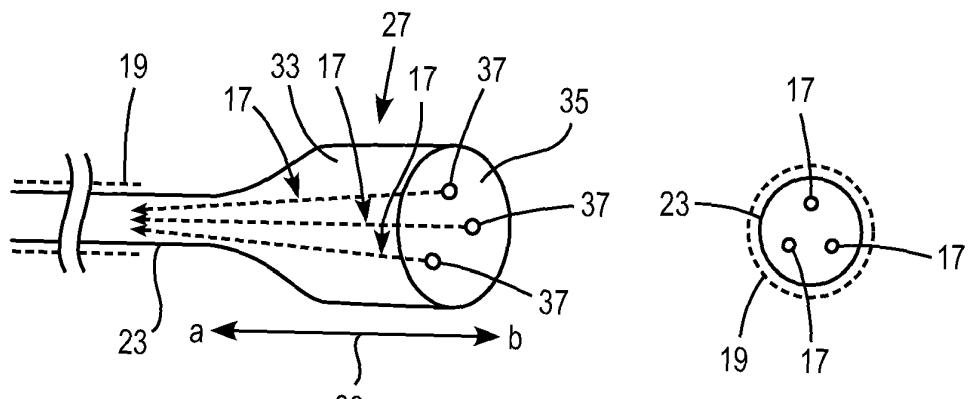


FIG. 1D

FIG. 1E

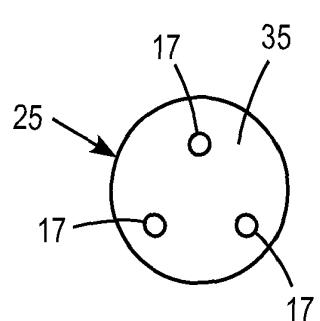


FIG. 1F

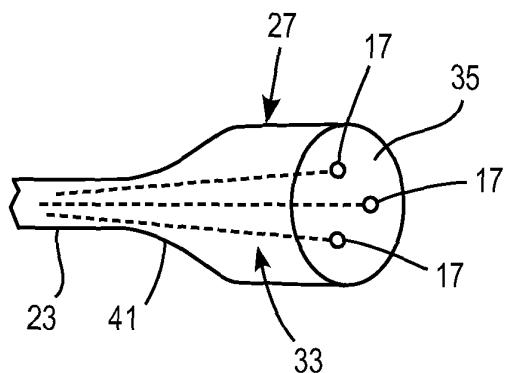


FIG. 1G

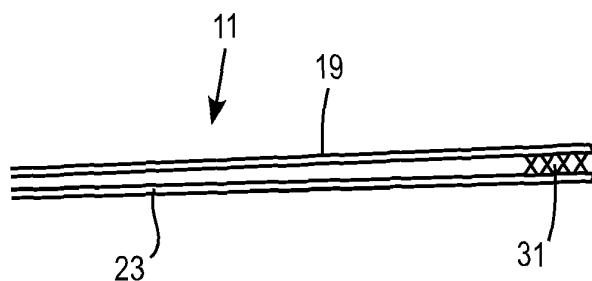


FIG. 1H

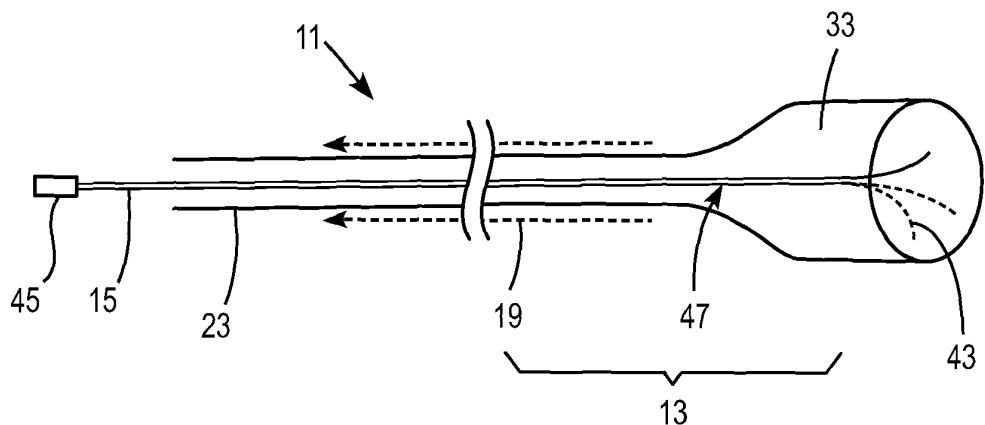
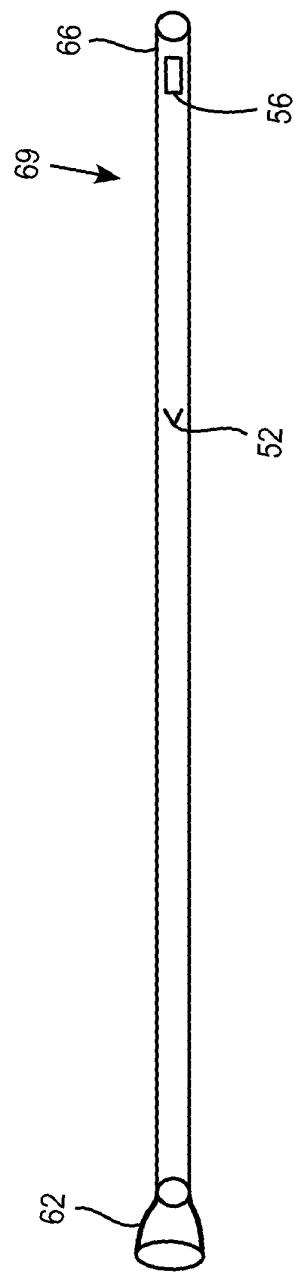
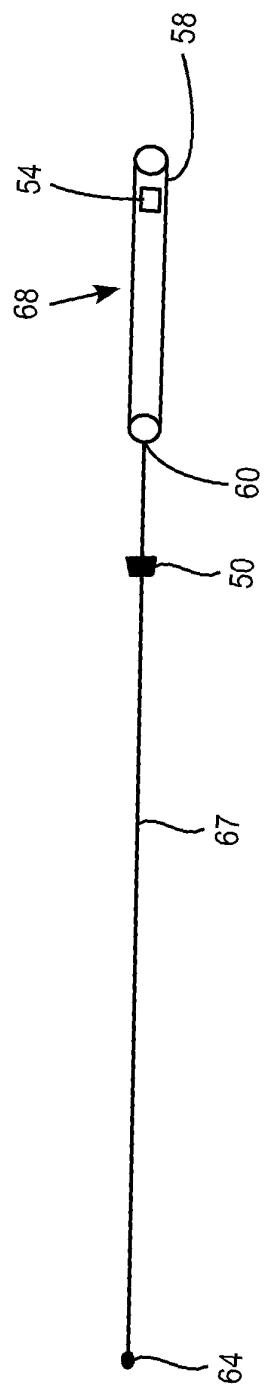


FIG. 1I



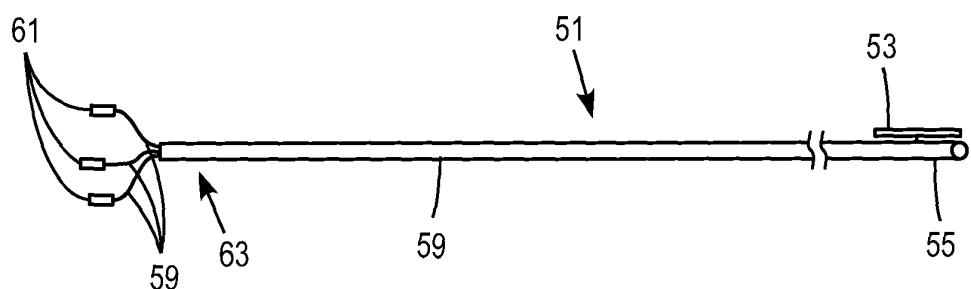


FIG. 2A




FIG. 2B

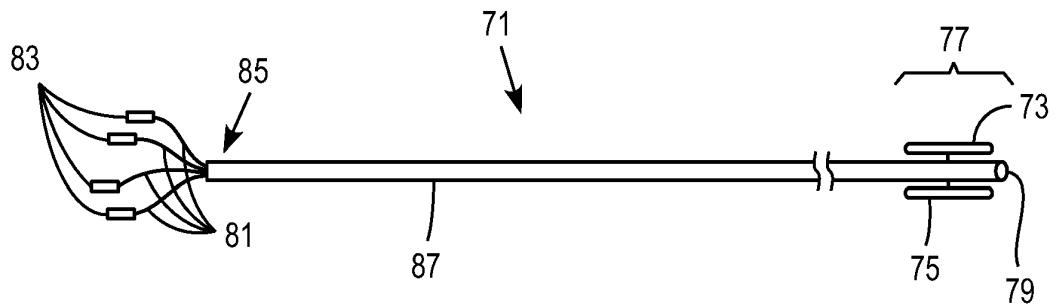


FIG. 3A




FIG. 3B

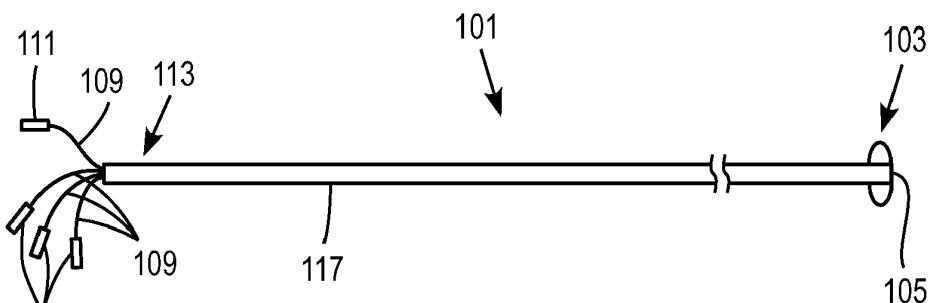


FIG. 4A




FIG. 4B




FIG. 4C

FIG. 5A

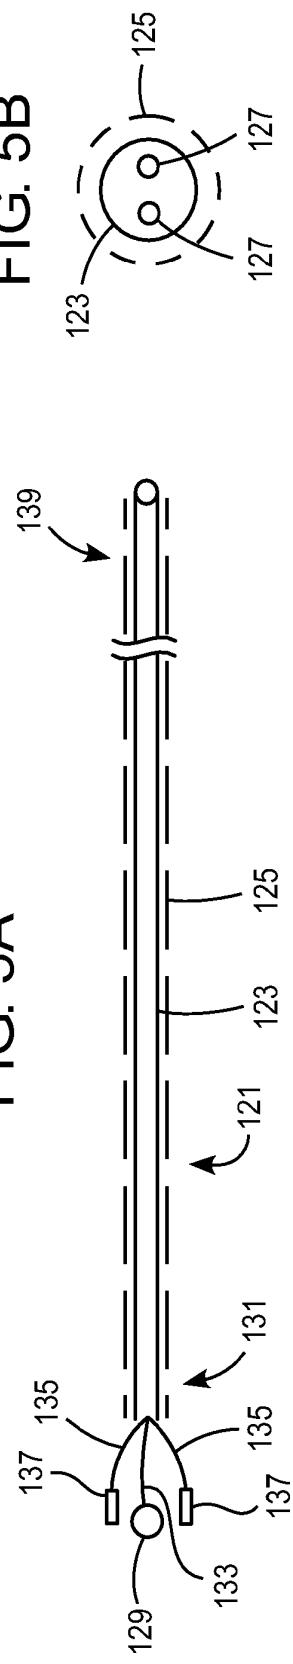


FIG. 5B

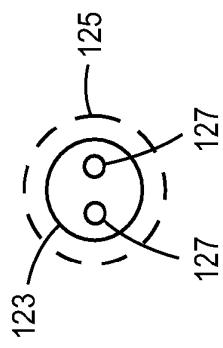


FIG. 6A

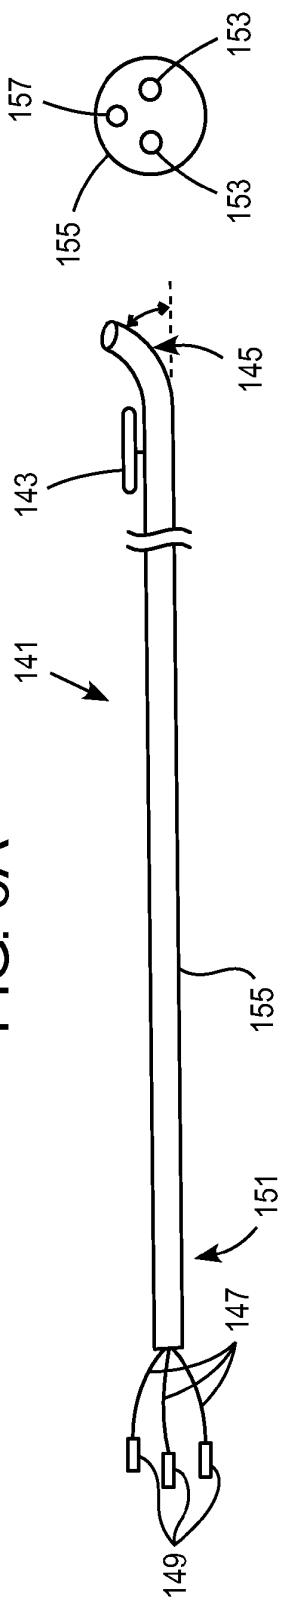
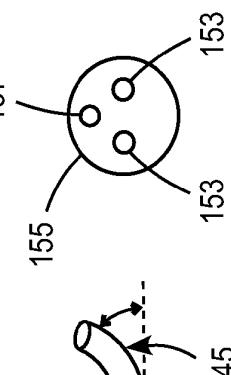


FIG. 6B



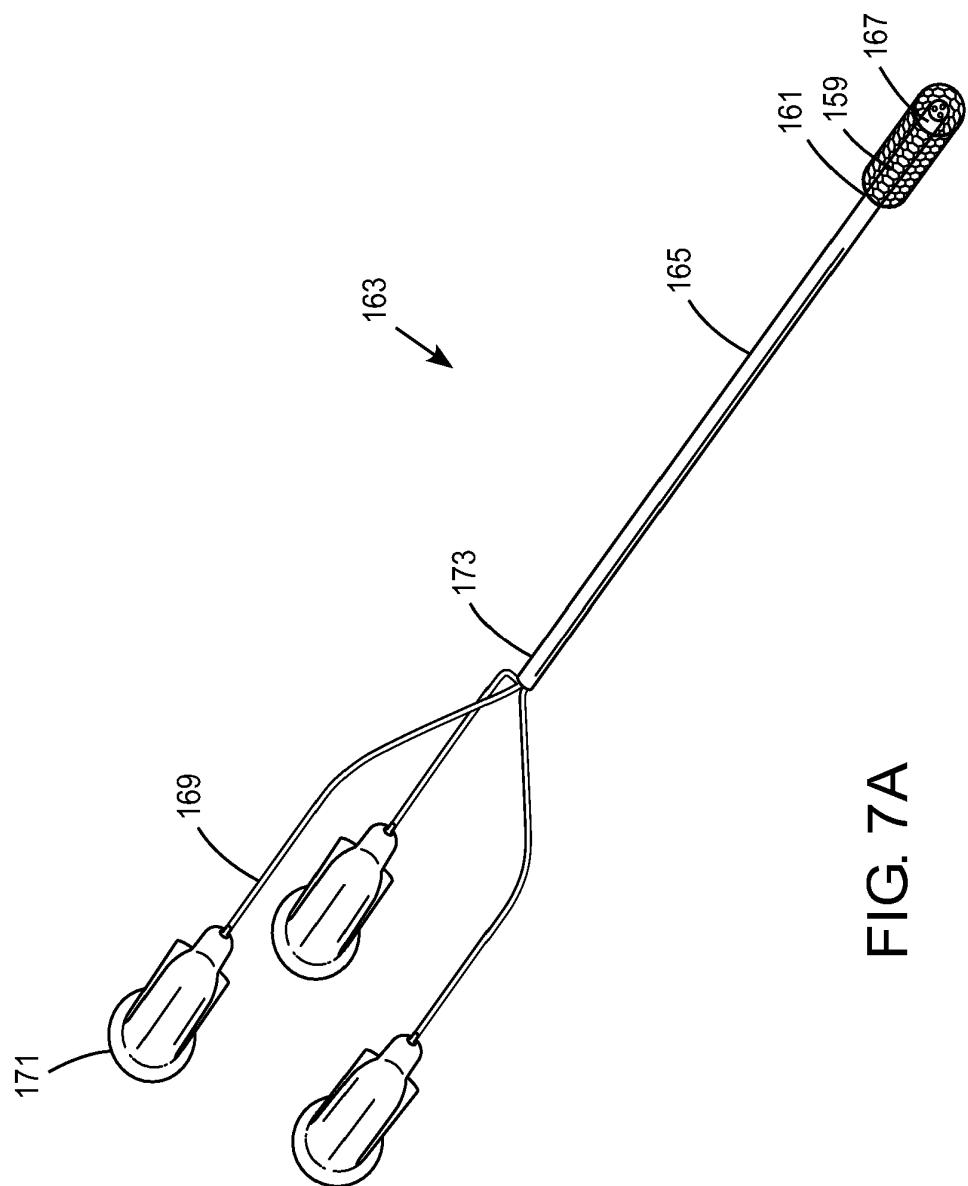
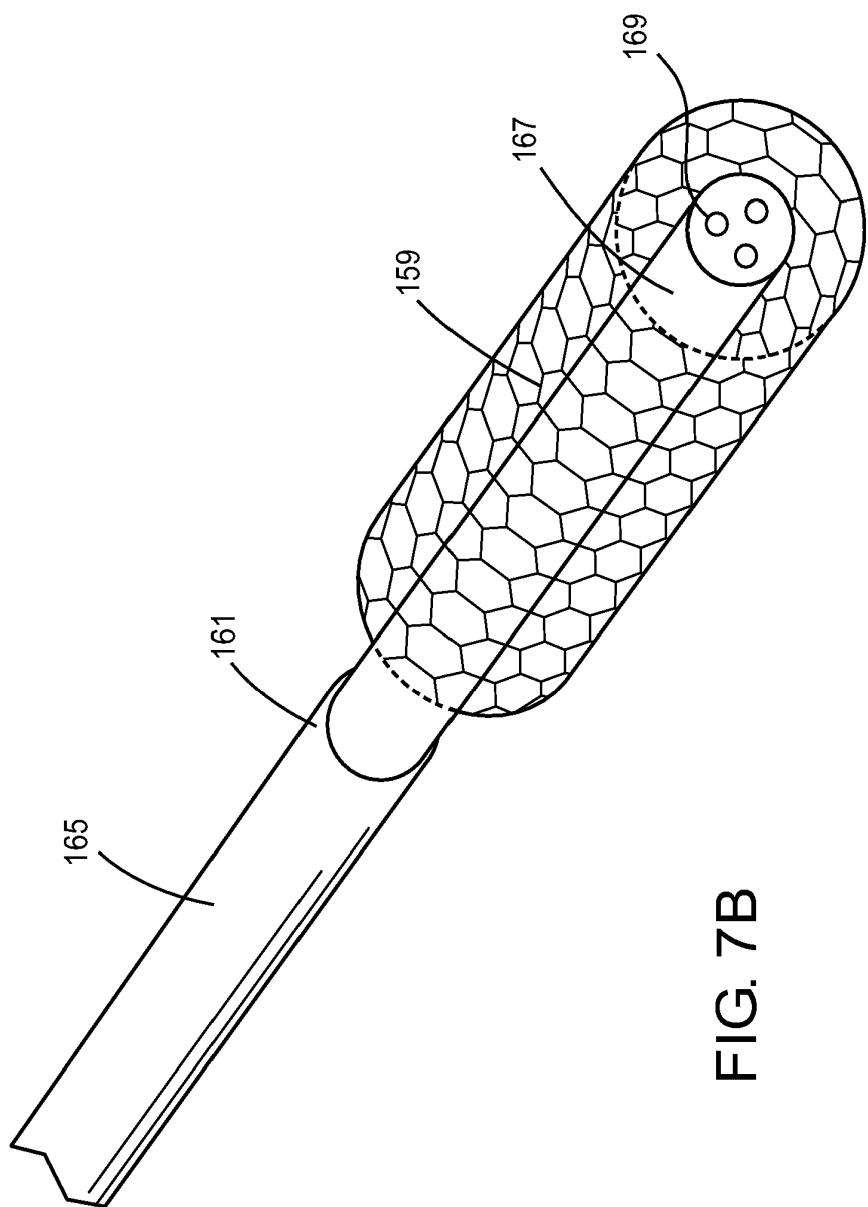


FIG. 7A



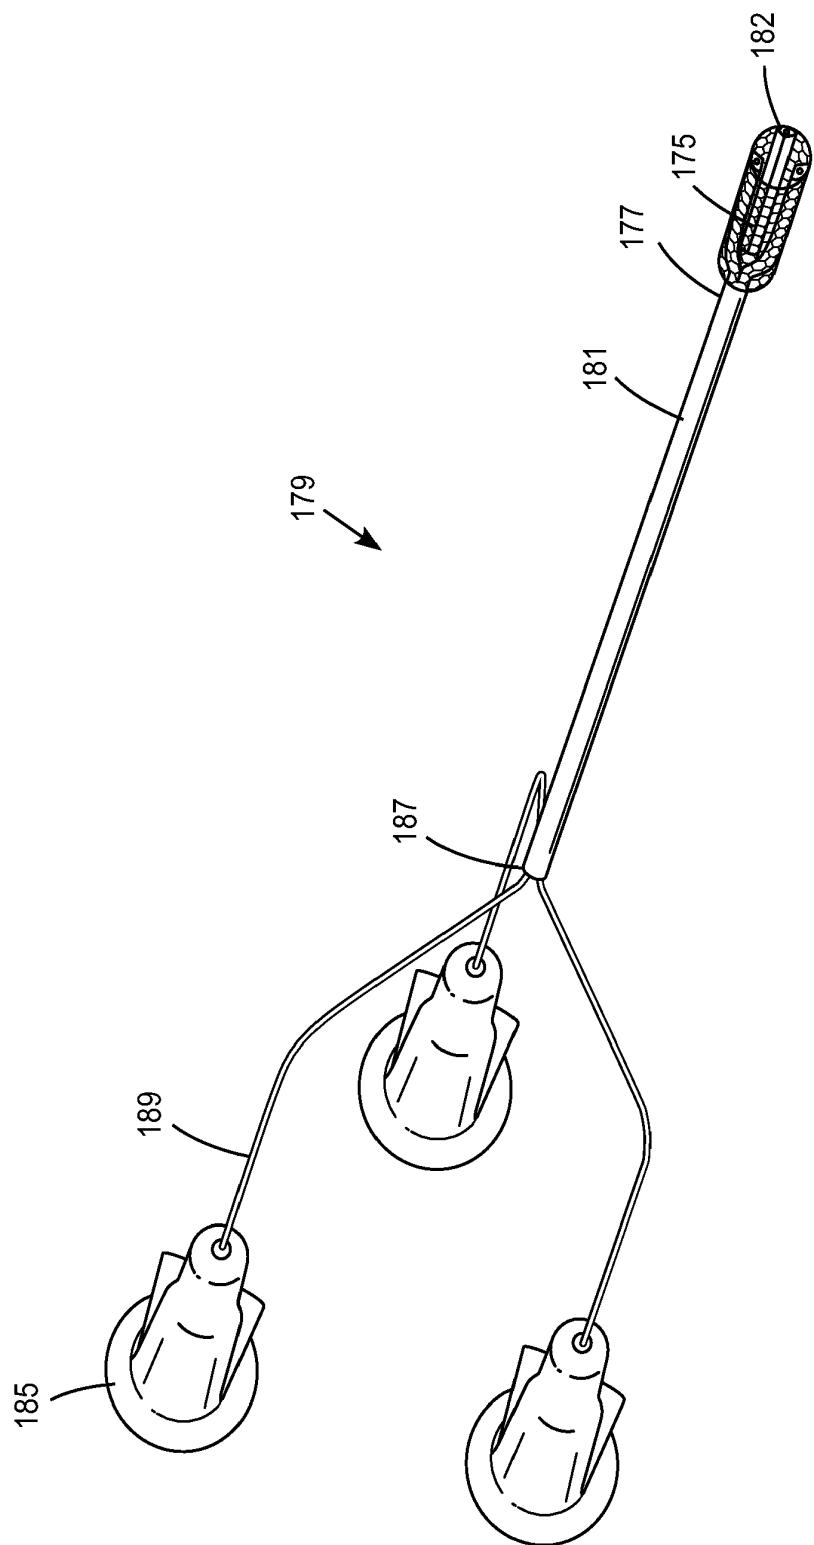


FIG. 8A

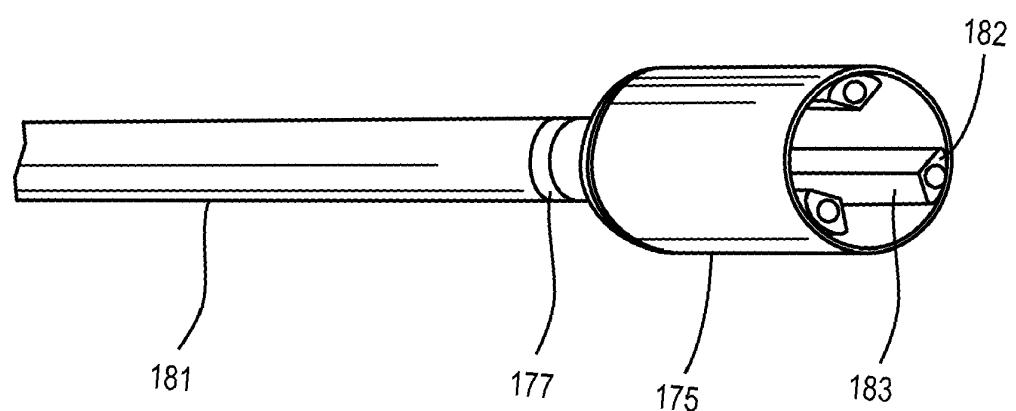


FIG. 8B

FIG. 8C

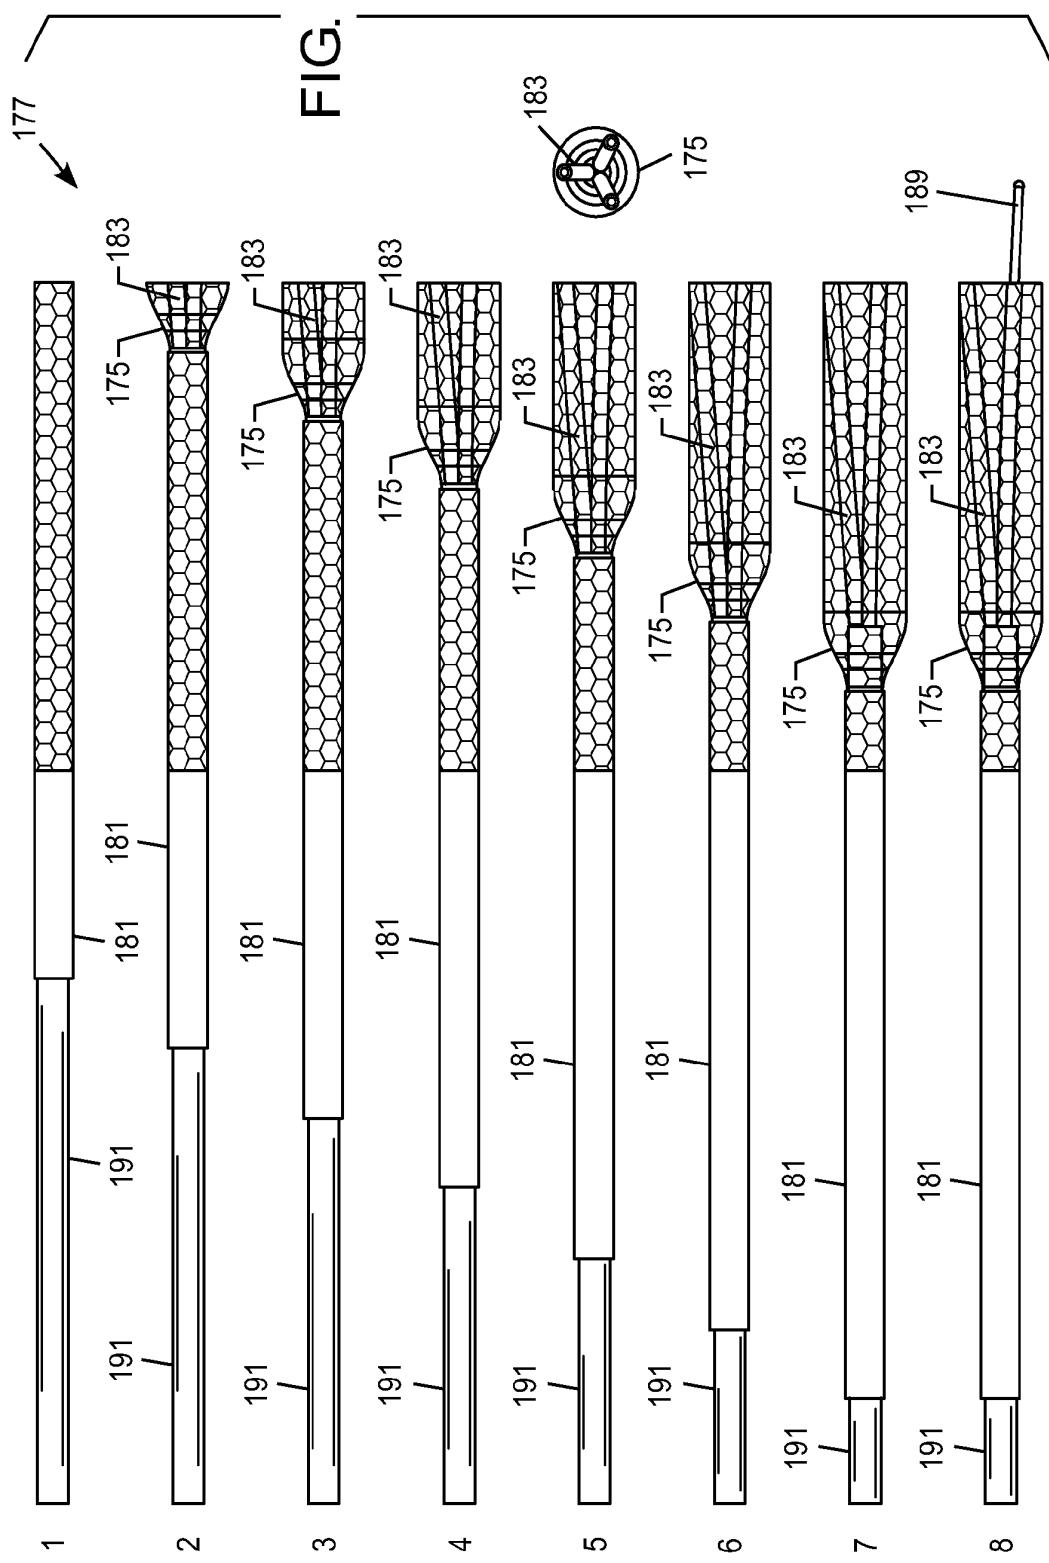
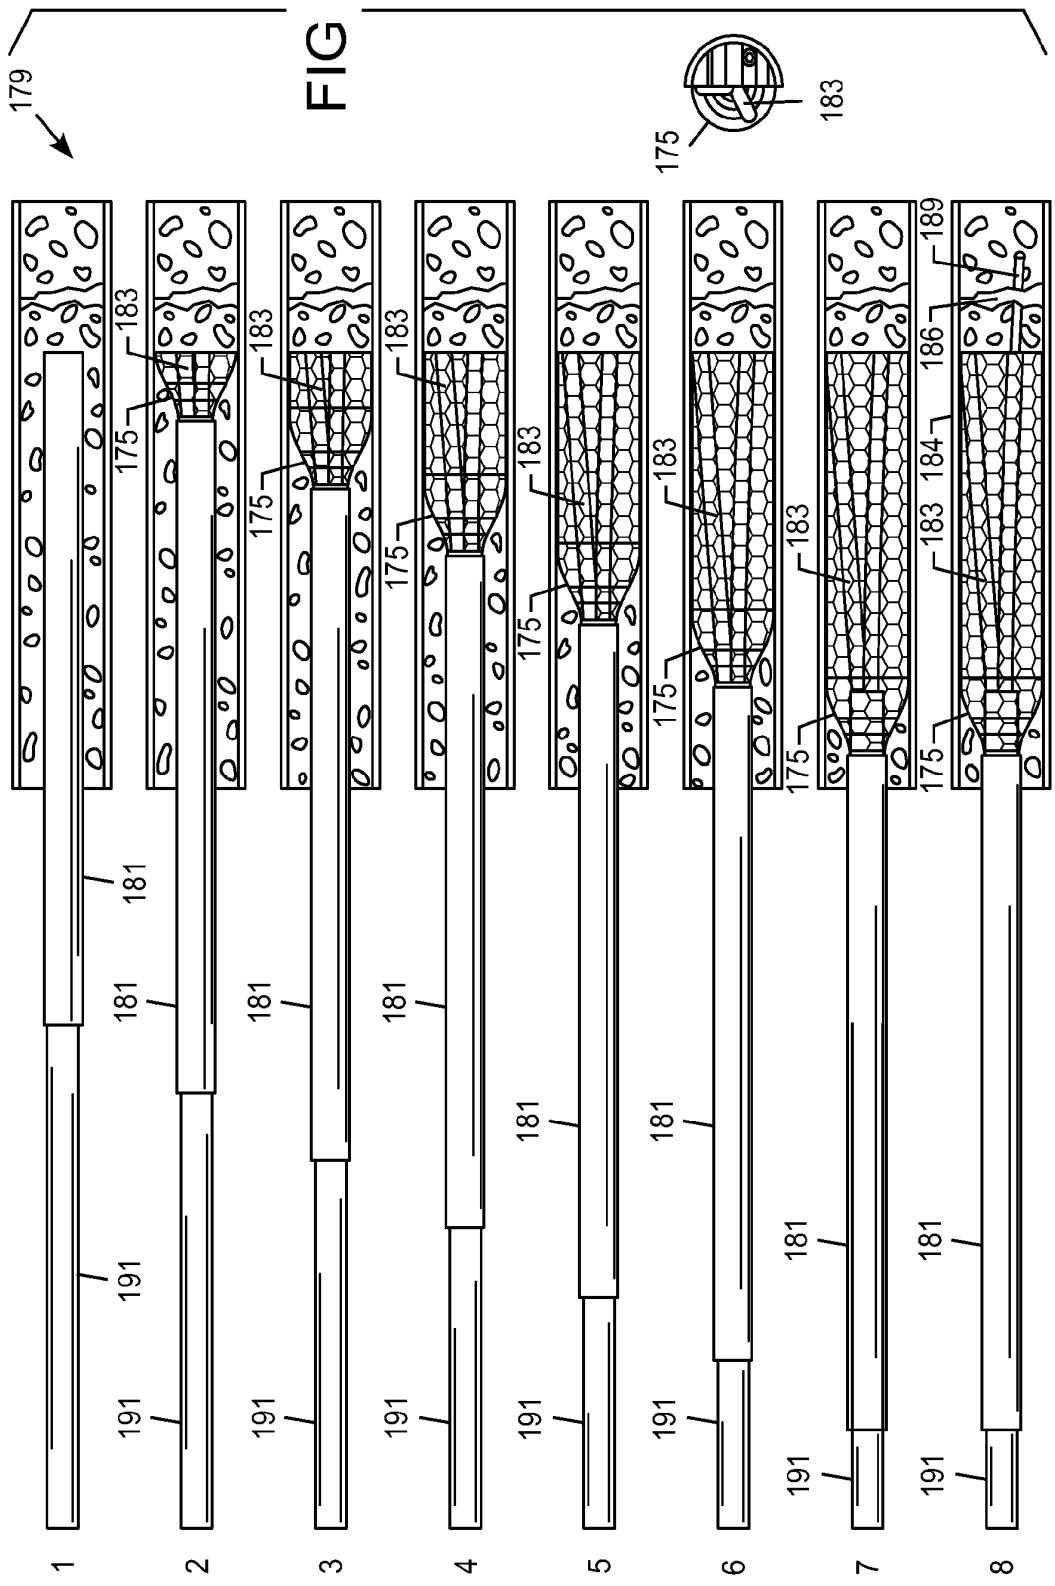


FIG 8D



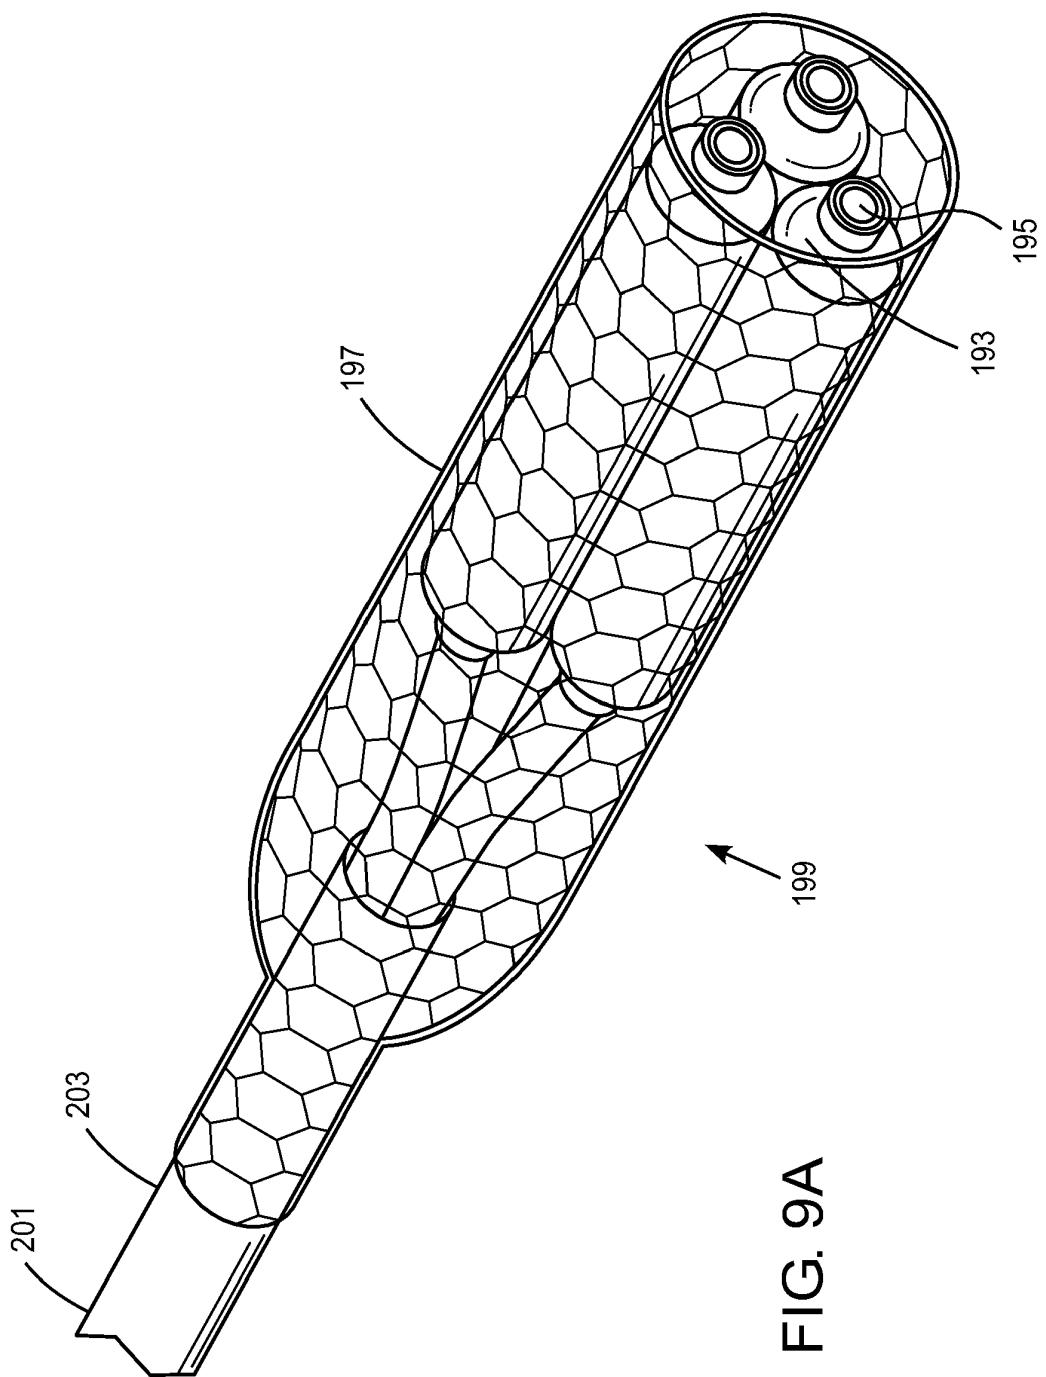


FIG. 9A

FIG. 9B

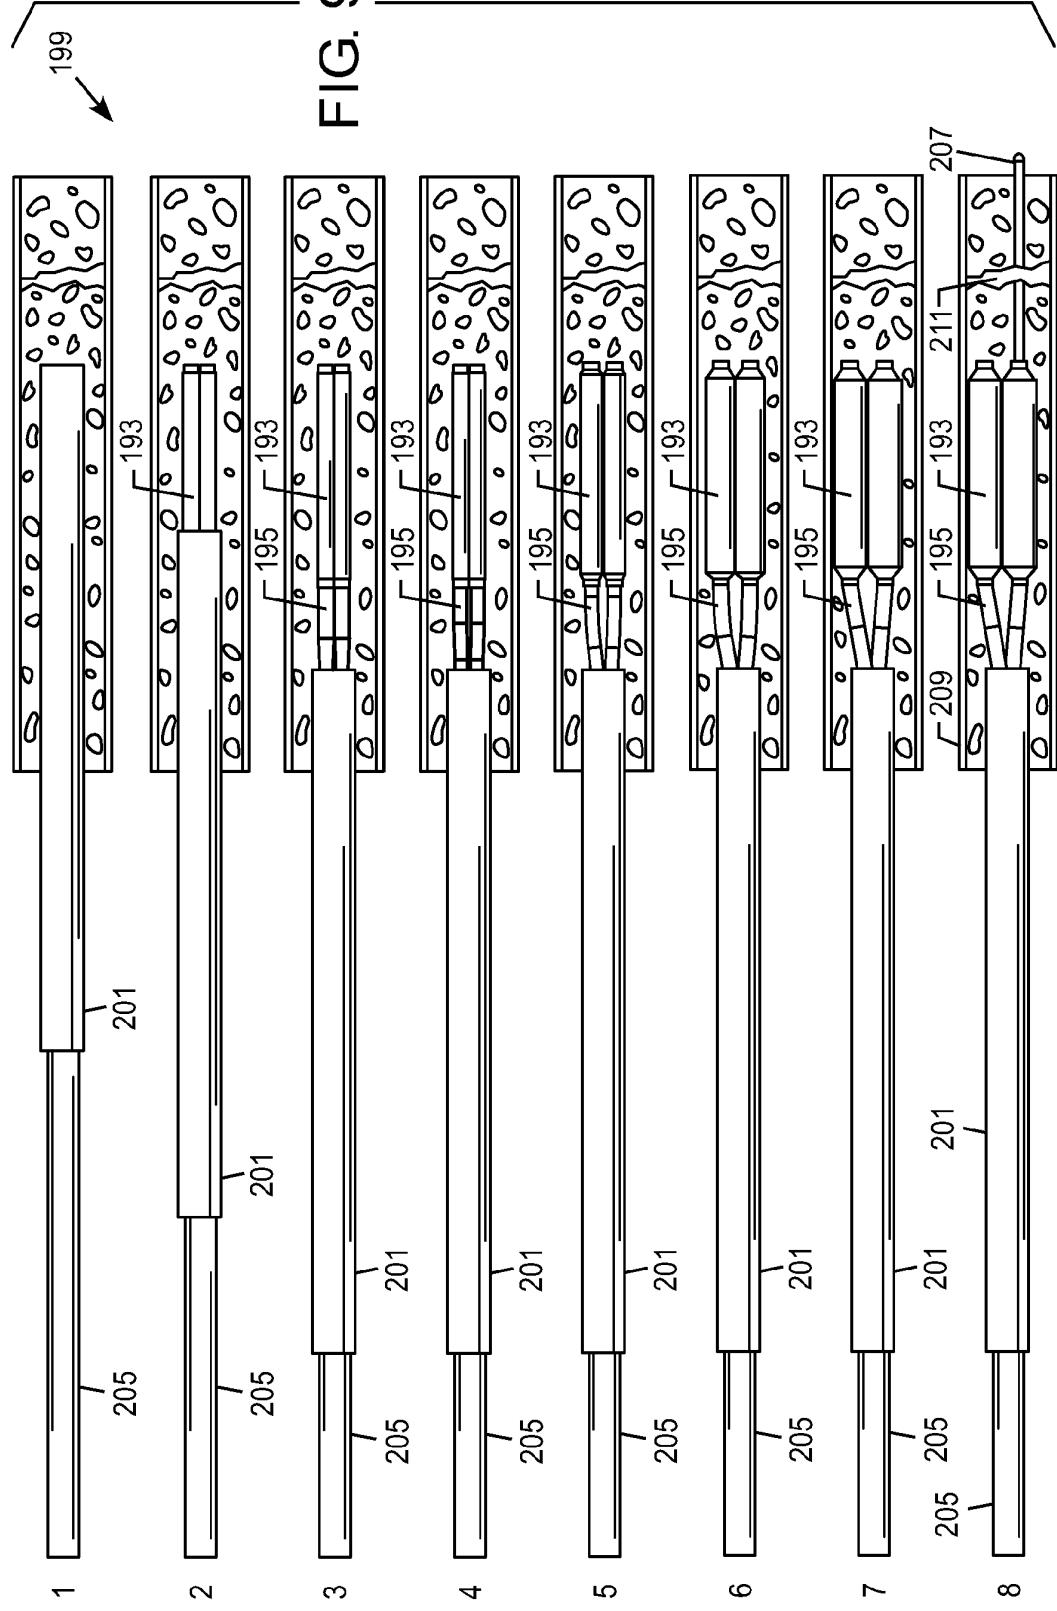


FIG. 10

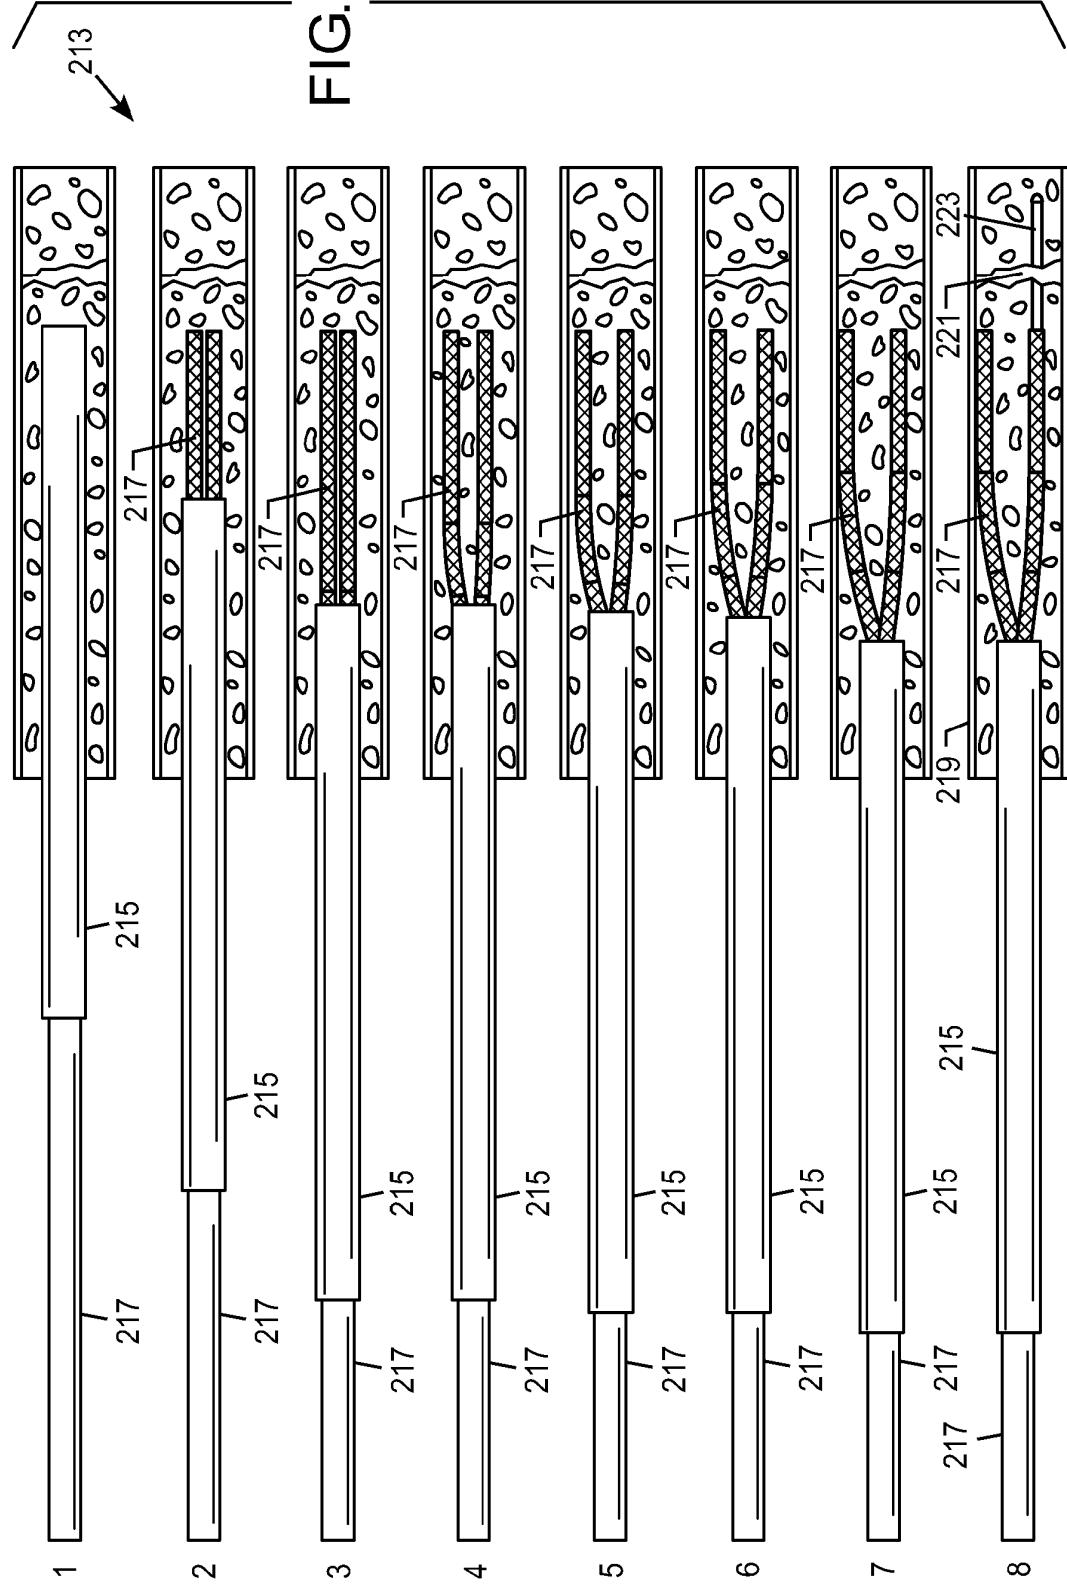


FIG. 11

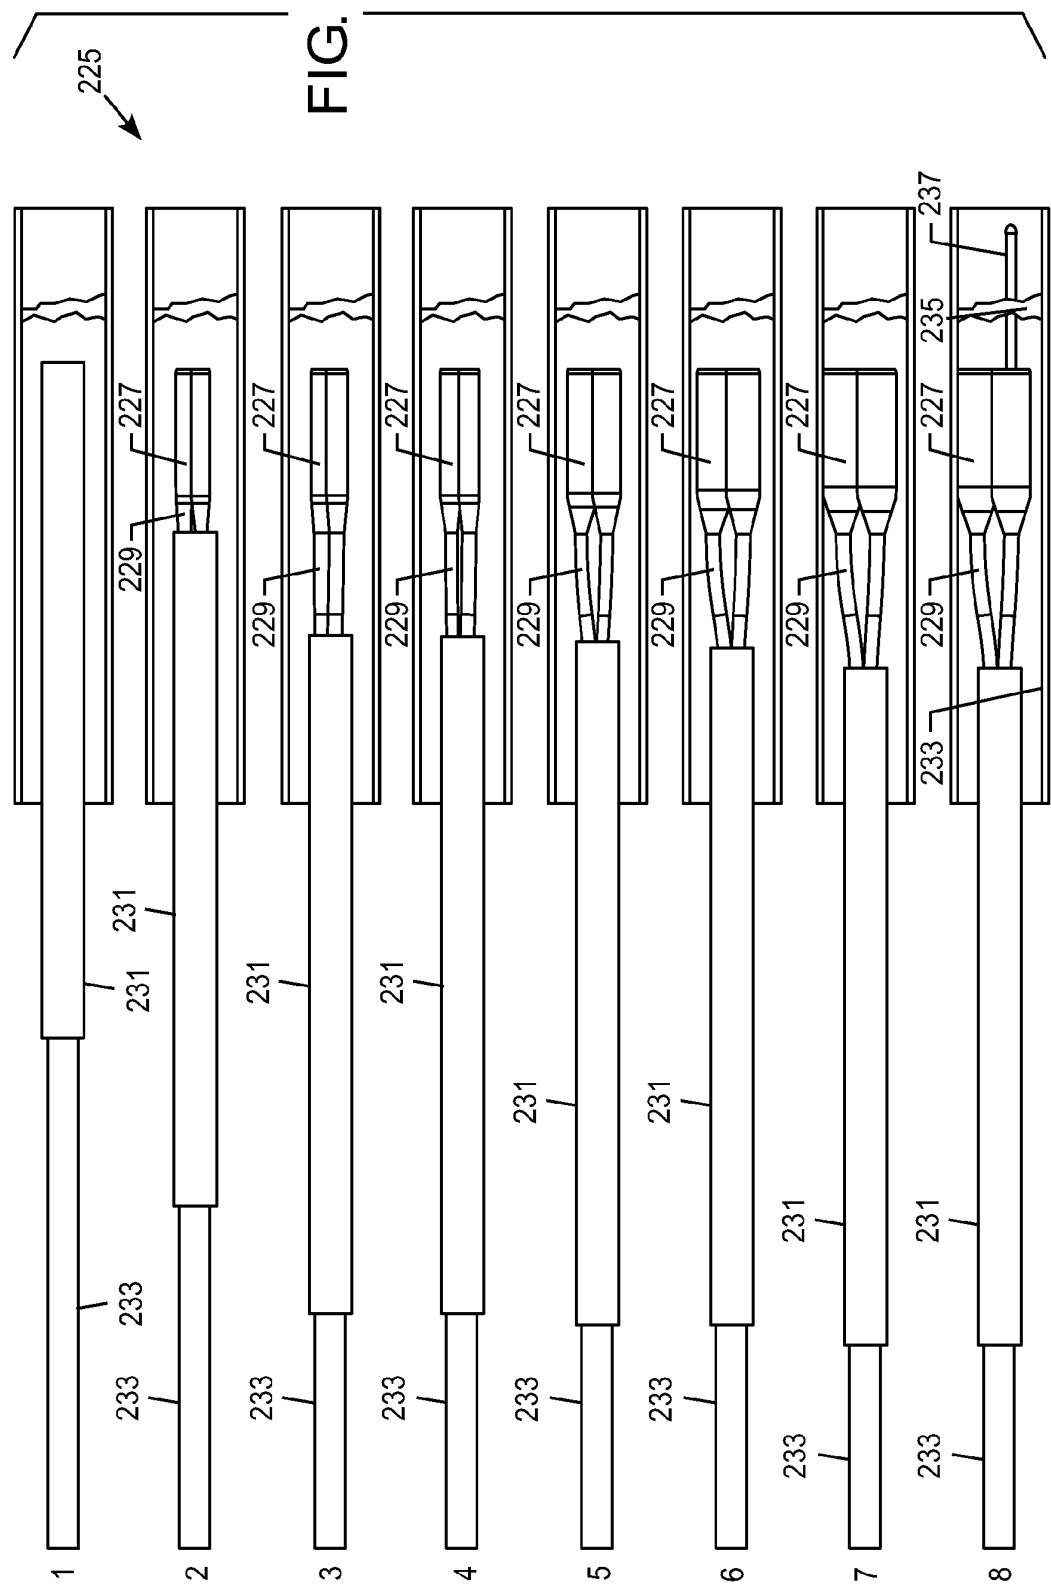
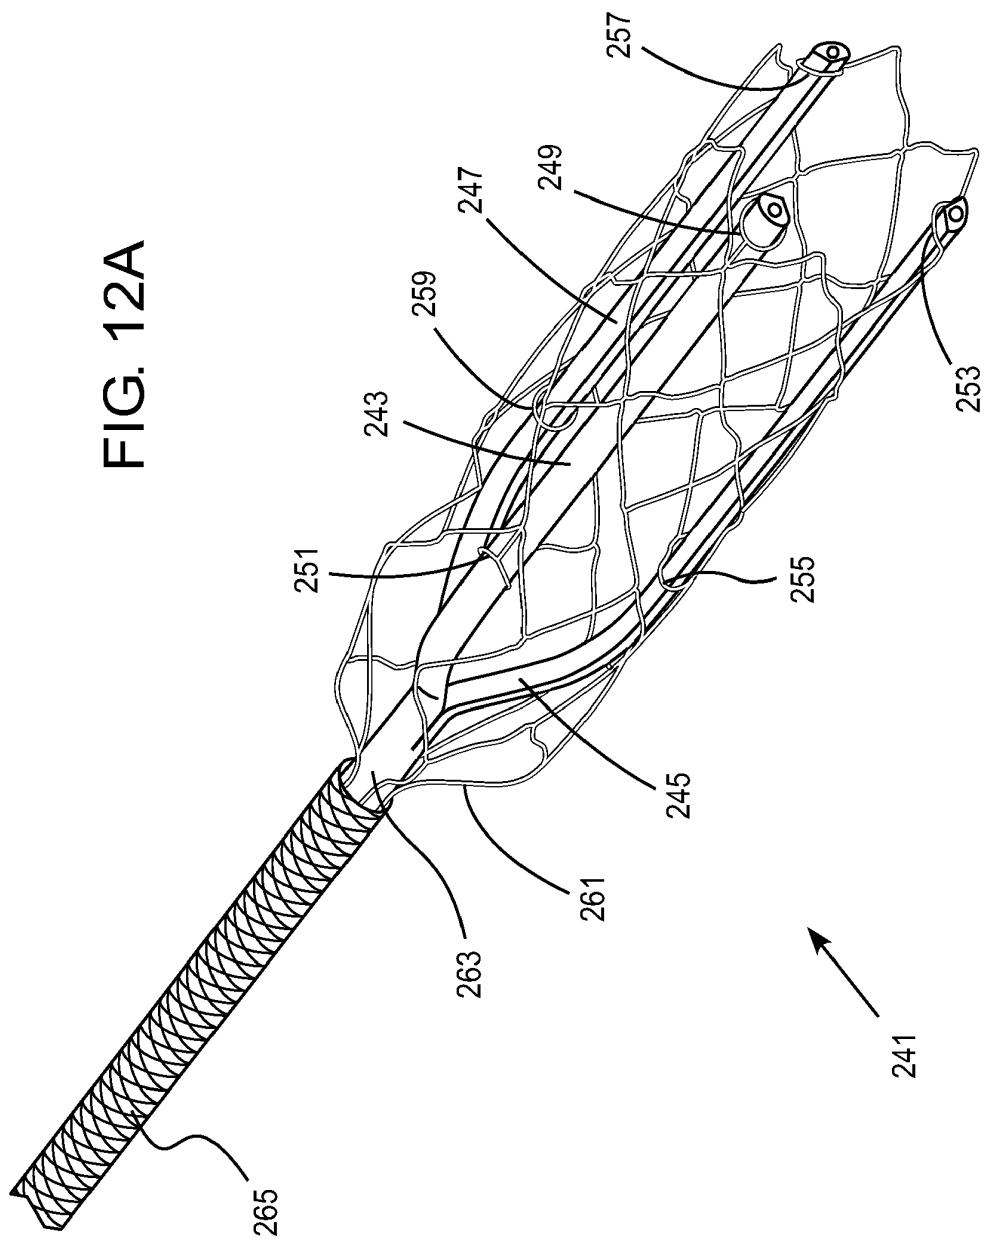


FIG. 12A



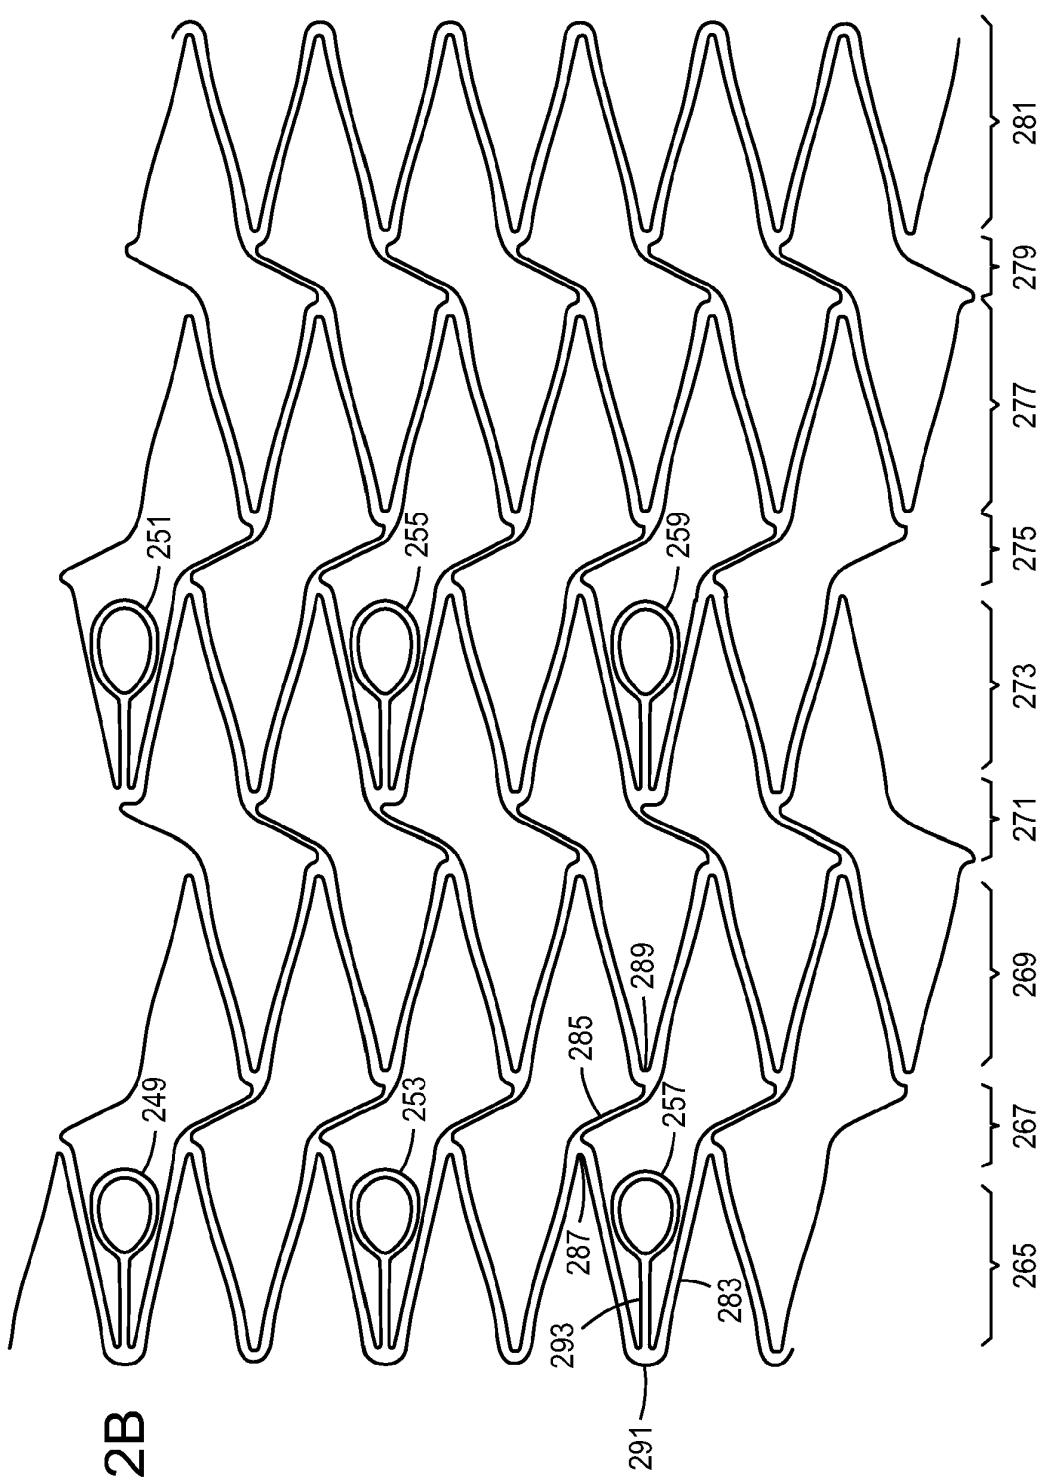


FIG. 12B

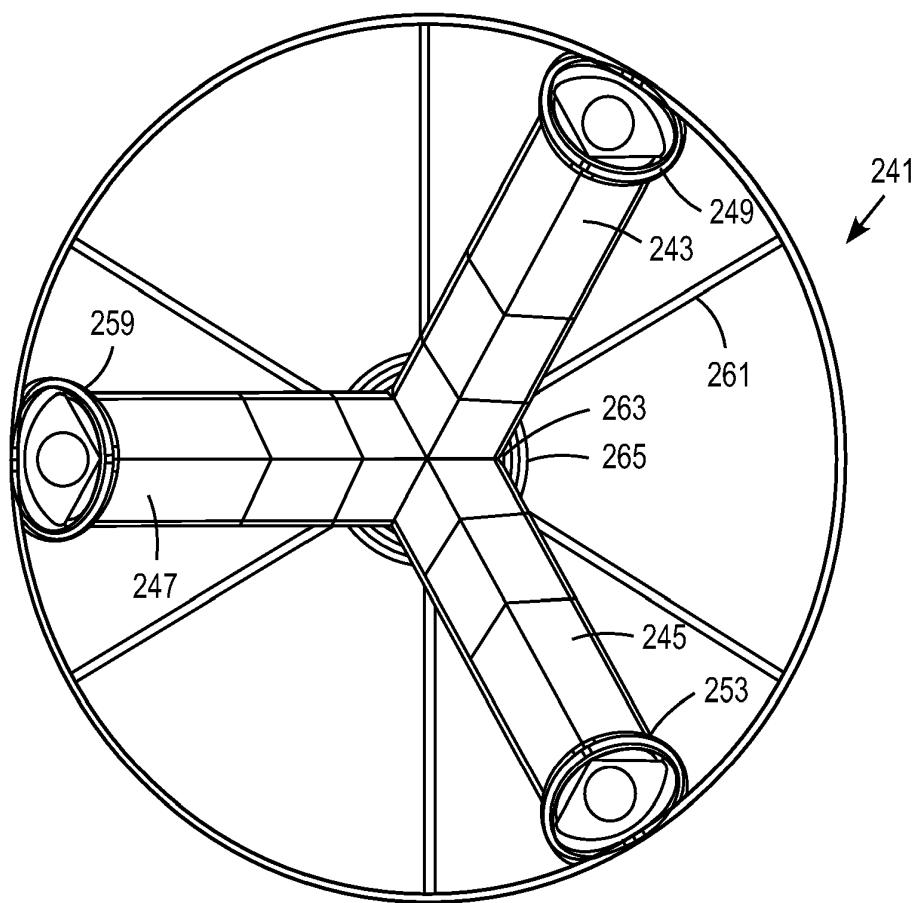


FIG. 12C

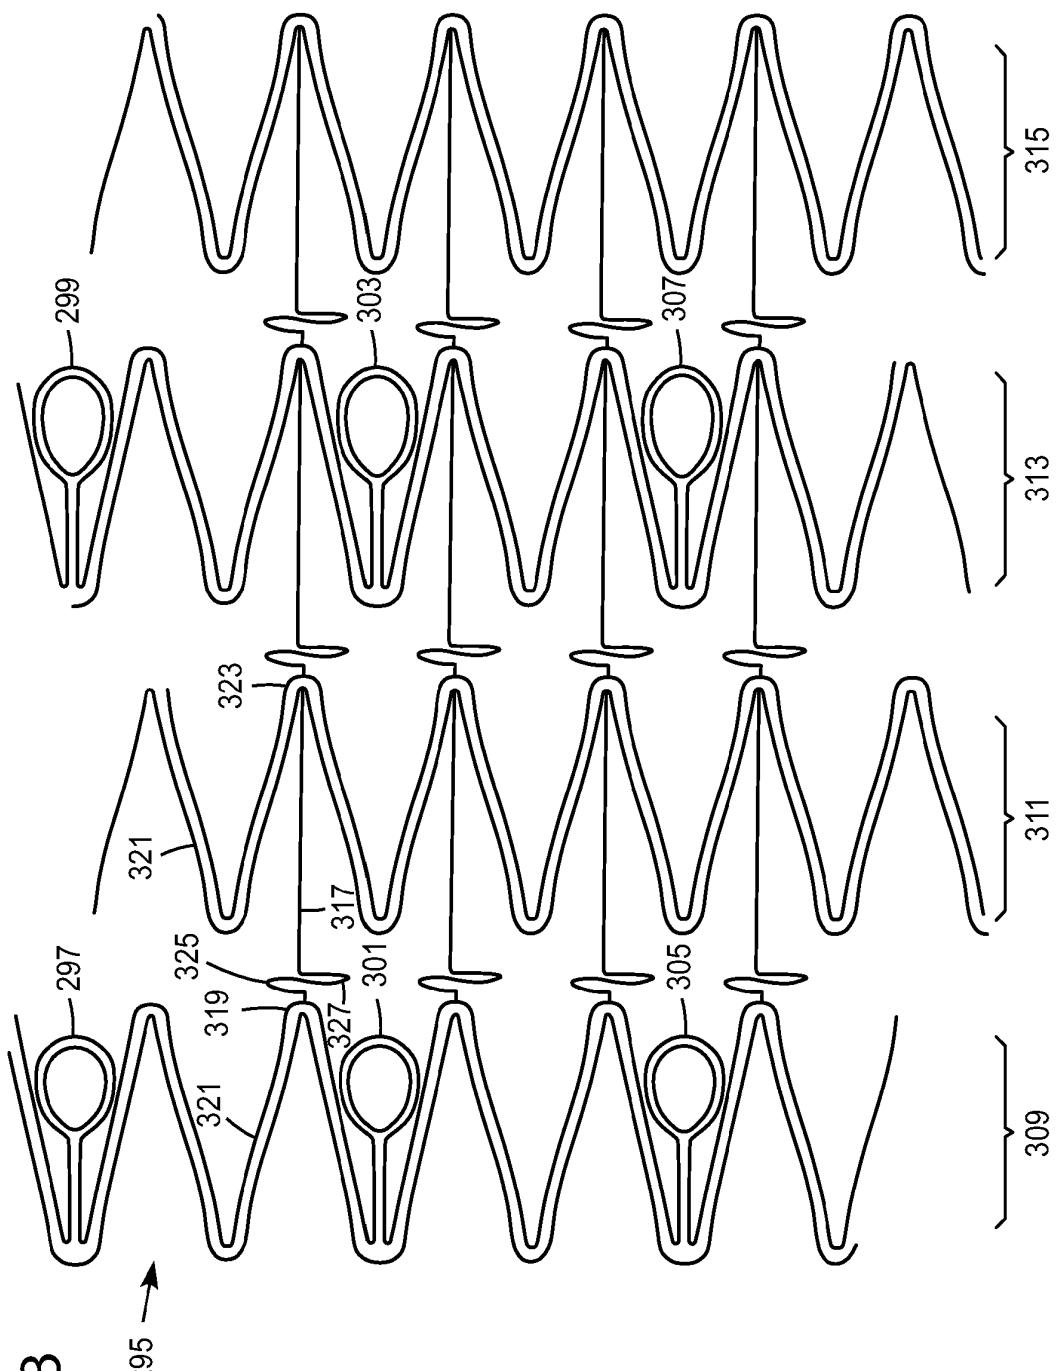


FIG. 13

5



EUROPEAN SEARCH REPORT

Application Number
EP 15 18 1301

10

15

20

25

30

35

40

45

DOCUMENTS CONSIDERED TO BE RELEVANT			CLASSIFICATION OF THE APPLICATION (IPC)
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	
X	US 2005/020974 A1 (NORIEGA GERARDO [US] ET AL) 27 January 2005 (2005-01-27) * the whole document * -----	1-7, 10-15	INV. A61M25/01 A61M25/00 A61M25/10 A61M25/04
X	US 2006/155363 A1 (LADUCA ROBERT [US] ET AL) 13 July 2006 (2006-07-13) * the whole document * -----	1-15	
A	EP 0 418 677 A1 (ADVANCED CARDIOVASCULAR SYSTEM [US]) 27 March 1991 (1991-03-27) * the whole document * -----	1-15	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61M A61B A61F
The present search report has been drawn up for all claims			
1	Place of search	Date of completion of the search	Examiner
50	Berlin	27 November 2015	Rodrigues, Elodie
CATEGORY OF CITED DOCUMENTS			
55	X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document	T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 15 18 1301

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

27-11-2015

10

	Patent document cited in search report		Publication date	Patent family member(s)	Publication date
	US 2005020974	A1	27-01-2005	EP 1768738 A2 JP 2008501489 A US 2005020974 A1 WO 2005120627 A2	04-04-2007 24-01-2008 27-01-2005 22-12-2005
15					
	US 2006155363	A1	13-07-2006	EP 1835865 A2 EP 1845895 A1 EP 1850790 A1 EP 2522313 A1 EP 2522314 A1 EP 2543347 A1 US 2006155358 A1 US 2006155363 A1 US 2008183274 A1 US 2008275542 A1 US 2013211507 A1 WO 2006076325 A1 WO 2006076326 A2 WO 2006076328 A1	26-09-2007 24-10-2007 07-11-2007 14-11-2012 14-11-2012 09-01-2013 13-07-2006 13-07-2006 31-07-2008 06-11-2008 15-08-2013 20-07-2006 20-07-2006 20-07-2006
20					
25					
30					
35					
40					
45					
50					
55					

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

摘要

一件使導絲通過一個慢性完全閉塞，可能具有遠端部分的軸之脈管系統的導管器具（11）；一個連接到該軸（23）的遠端部分（13），可移除、可擴展的支架結構（27）和一個位於中心位置的單個管腔（47），其穿過該軸的中心及穿過上述可擴展的支架結構，並被配置成穿過導絲。