



US00D773650S

(12) **United States Design Patent** (10) **Patent No.:** **US D773,650 S**
Fourt et al. (45) **Date of Patent:** **** Dec. 6, 2016**

(54) **AUTOMATIC INJECTION DEVICE**

(71) Applicant: **Eli Lilly and Company**, Indianapolis, IN (US)

(72) Inventors: **Jesse Arnold Fourt**, Menlo Park, CA (US); **Thomas Dieter Christian Overthun**, San Francisco, CA (US); **Judy Guo**, San Francisco, CA (US); **Thomas Gaëtan Thibault Brisebras**, San Francisco, CA (US)

(73) Assignee: **Eli Lilly and Company**, Indianapolis, IN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/530,811**

(22) Filed: **Jun. 19, 2015**

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/113**

(58) **Field of Classification Search**

USPC D24/112–114, 108, 133, 130, 127, 186;
606/181, 185; 604/264, 272, 187, 181,
184, 604/227
CPC A61M 5/178; A61M 3/00; A61M 5/20;
A61M 5/31; A61M 5/3146; A61M
5/3129; A61M 5/3148; A61M 5/315
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D316,899 S 5/1991 Andersson et al.
D330,079 S 10/1992 Dalling et al.
D420,739 S 2/2000 Moreau-Defarges
D461,555 S * 8/2002 Binet D24/114
D471,976 S 3/2003 Pavlu et al.
D476,078 S 6/2003 Pavlu et al.
D476,734 S 7/2003 Pavlu et al.
D483,116 S 12/2003 Castellano

D628,690 S 12/2010 Galbraith
7,918,824 B2 4/2011 Bishop et al.
D670,375 S 11/2012 Corbin
D670,376 S 11/2012 Corbin
D677,380 S 3/2013 Julian et al.
(Continued)

FOREIGN PATENT DOCUMENTS

WO 2007002052 1/2007
WO 2007047200 4/2007
(Continued)

OTHER PUBLICATIONS

Ypsomed-YpsoMate® Brochure.

(Continued)

Primary Examiner — David Muller

(74) *Attorney, Agent, or Firm* — Edward J. Prein


(57) **CLAIM**

The ornamental design for an automatic injection device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of an automatic injection device showing our new design; FIG. 2 is a bottom perspective view thereof; FIG. 3 is a front view thereof; FIG. 4 is a rear view thereof; FIG. 5 is side view thereof; FIG. 6 is an opposite side view thereof; FIG. 7 is a top view thereof; and, FIG. 8 is a bottom view thereof. The small ovals in the central height region of FIGS. 1-6 show projecting texturing that form part of the claimed design. The broken lines showing internal portions and a bottom portion of the automatic injection device form no part of the claimed design.

1 Claim, 4 Drawing Sheets

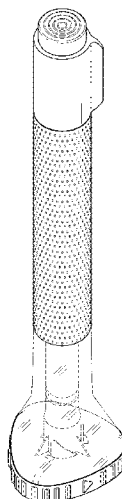

(56)

References Cited

U.S. PATENT DOCUMENTS

8,409,138 B2 4/2013 James et al.
D690,416 S * 9/2013 Cappello D24/112
D695,892 S * 12/2013 Cappello D24/113
D696,397 S 12/2013 Guarraia et al.
D708,317 S 7/2014 Schneider et al.
D714,932 S * 10/2014 Hall D24/112
D721,802 S * 1/2015 Ohashi D24/113
D724,721 S 3/2015 Geert-Jensen et al.
D728,782 S 5/2015 Dubuc et al.
D729,930 S 5/2015 Geert-Jensen et al.
D732,161 S * 6/2015 Ohashi D24/113
D739,011 S * 9/2015 Morrison, Jr. D24/114
D741,472 S * 10/2015 Yotani D24/108
D743,560 S * 11/2015 Pietrantonio D24/186
D747,476 S * 1/2016 Kawamura D24/130
D747,797 S * 1/2016 Fourt D24/114
D748,270 S * 1/2016 Pietrantonio D24/186
D758,570 S * 6/2016 Wohlfahrt D24/113
2011/0092915 A1 4/2011 Olson et al.

FOREIGN PATENT DOCUMENTS

WO	2010104779	9/2010
WO	2011109205	9/2011
WO	2013032779	3/2013
WO	2014062488	4/2014

OTHER PUBLICATIONS

Schreiner Group—New Labels with Tamper-Evident and Non-Slip Features Help Enhance Patient Safety(URL: <http://www.schreiner-group.com/3/company/press-room/schreiner-medipharma-us/new-labels-with-tamper-evident-and-non-slip-features-help-enhance-patient-safety/>).

Unpublished Design U.S. Appl. No. 29/449,492, Eli Lilly and Company, entitled “Automatic Injection Device” filed Mar. 15, 2013.

* cited by examiner

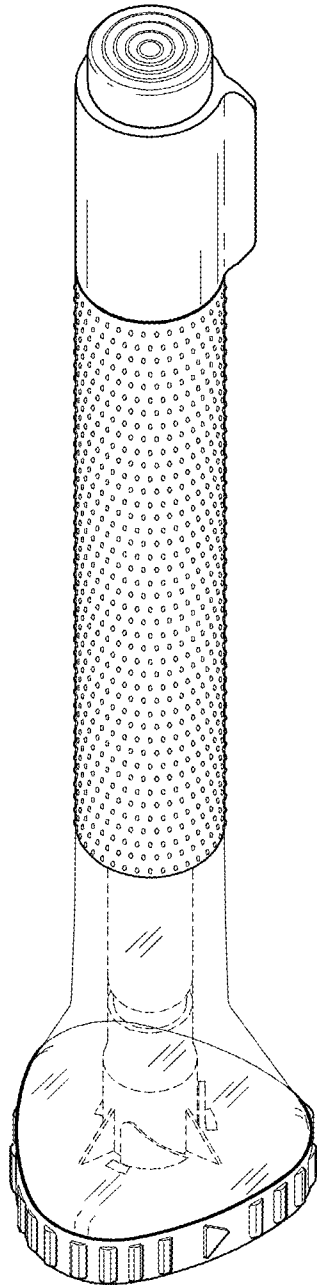


Fig. 1

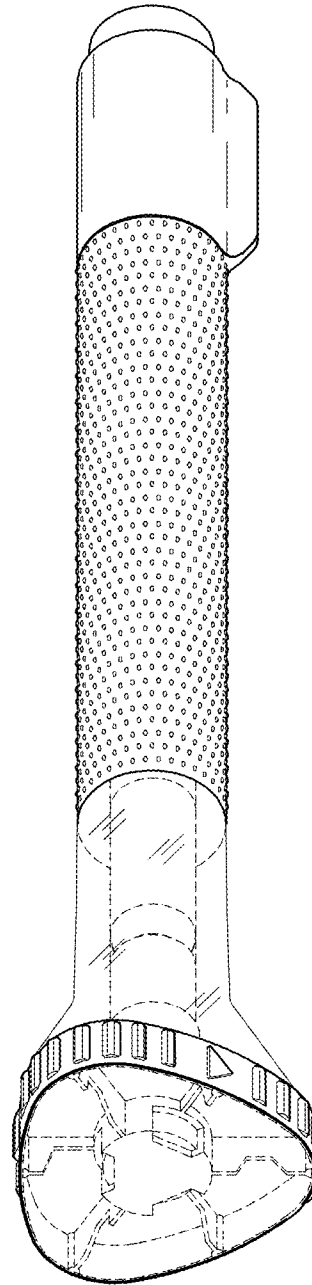
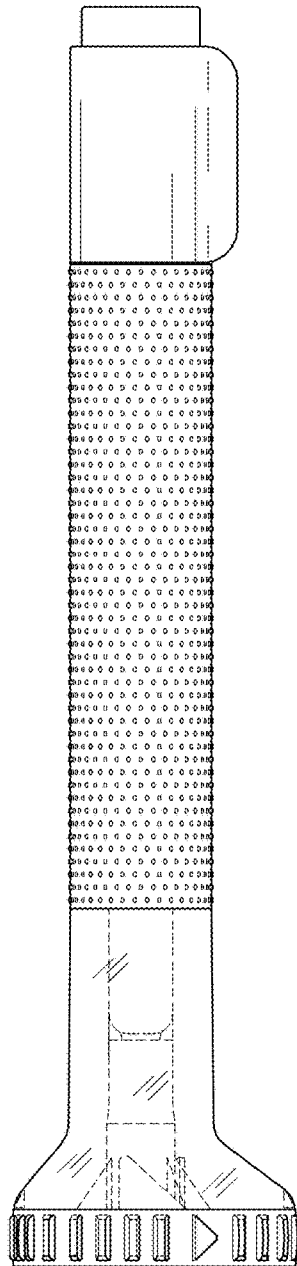
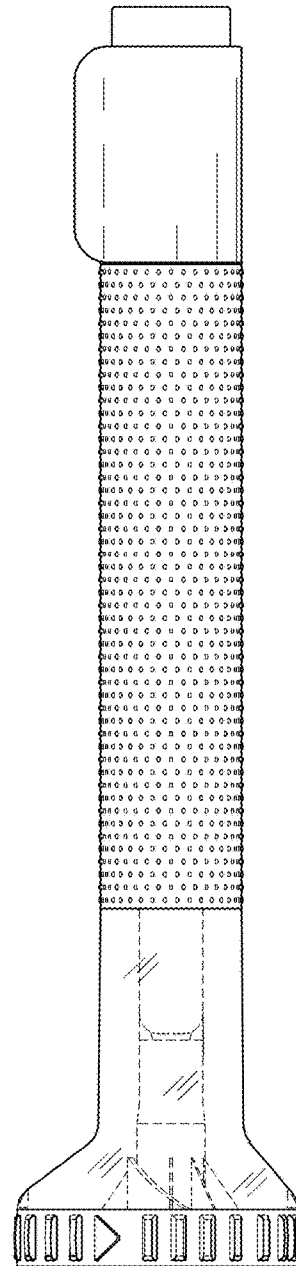


Fig. 2

*Fig. 3**Fig. 4*

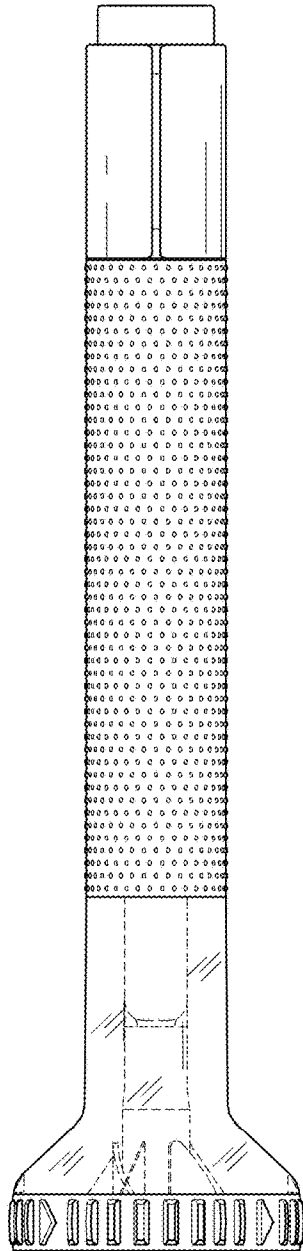


Fig. 5

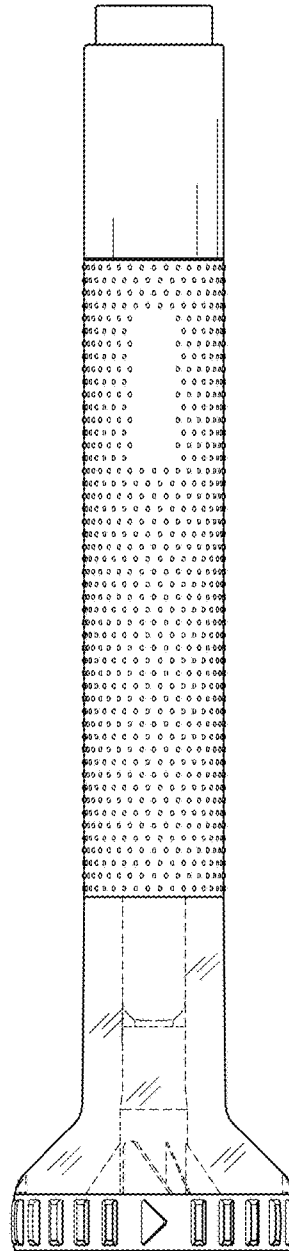


Fig. 6

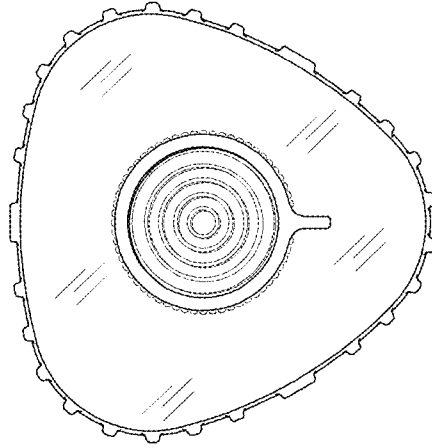


Fig. 7

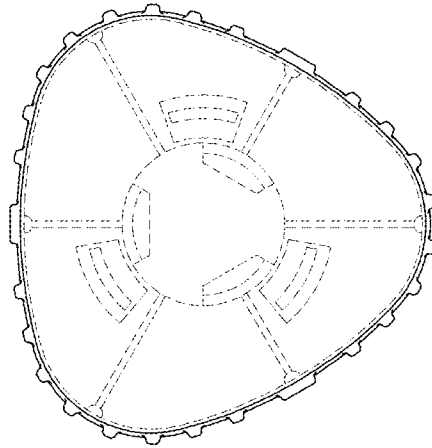


Fig. 8