



(19) **United States**

(12) **Patent Application Publication**
Carr

(10) **Pub. No.: US 2013/0281851 A1**

(43) **Pub. Date: Oct. 24, 2013**

(54) **HEATING/SENSING CATHETER APPARATUS FOR MINIMALLY INVASIVE APPLICATIONS**

(52) **U.S. Cl.**
CPC *A61N 5/025* (2013.01); *A61B 18/1815* (2013.01)
USPC **600/435**; 607/96; 606/33

(71) Applicant: **Kenneth L. Carr**, Woolwich, ME (US)

(72) Inventor: **Kenneth L. Carr**, Woolwich, ME (US)

(21) Appl. No.: **13/709,434**

(22) Filed: **Dec. 10, 2012**


Related U.S. Application Data

(60) Provisional application No. 61/635,348, filed on Apr. 19, 2012.

Publication Classification

(51) **Int. Cl.**
A61N 5/02 (2006.01)
A61B 18/18 (2006.01)

(57) **ABSTRACT**
Catheter apparatus comprises a coaxial cable having proximal and distal ends. The cable includes a hollow center conductor, an outer conductor and an electrically insulating layer between the conductors. An antenna is at the distal end of the cable, and a diplexer is connected to the cable, the diplexer including a transmit path for connecting the antenna to a transmitter which transmits first frequency signals and a receive path for connecting the antenna to a receiver which detects second frequency signals the diplexer isolating the signals on the two paths from one another. A transmission line connects the cable to the diplexer, the transmission line having a segment with a tubular inner conductor one end of which is connected to the center conductor and a second end of which is adapted for connection to a coolant source, the center and inner conductors forming a continuous coolant pathway.

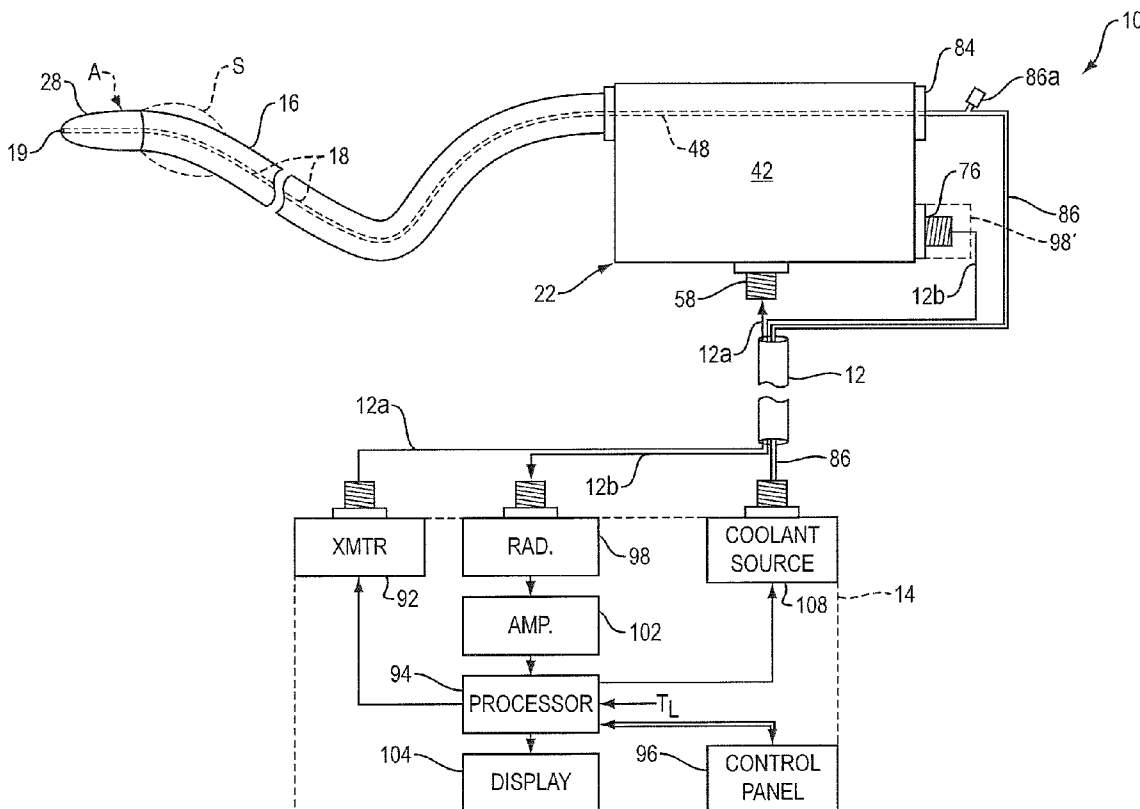

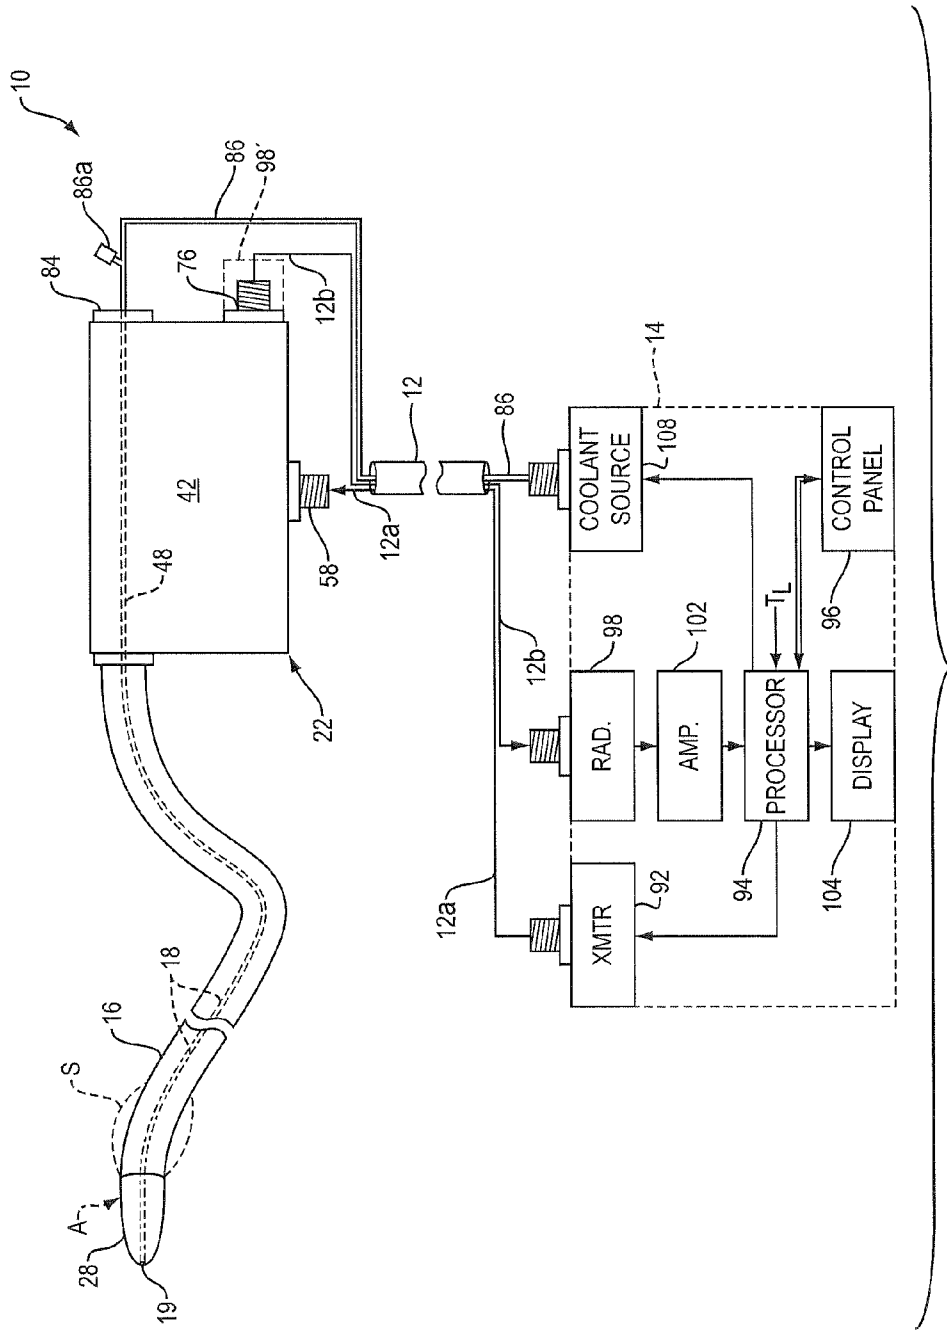


FIG. 1

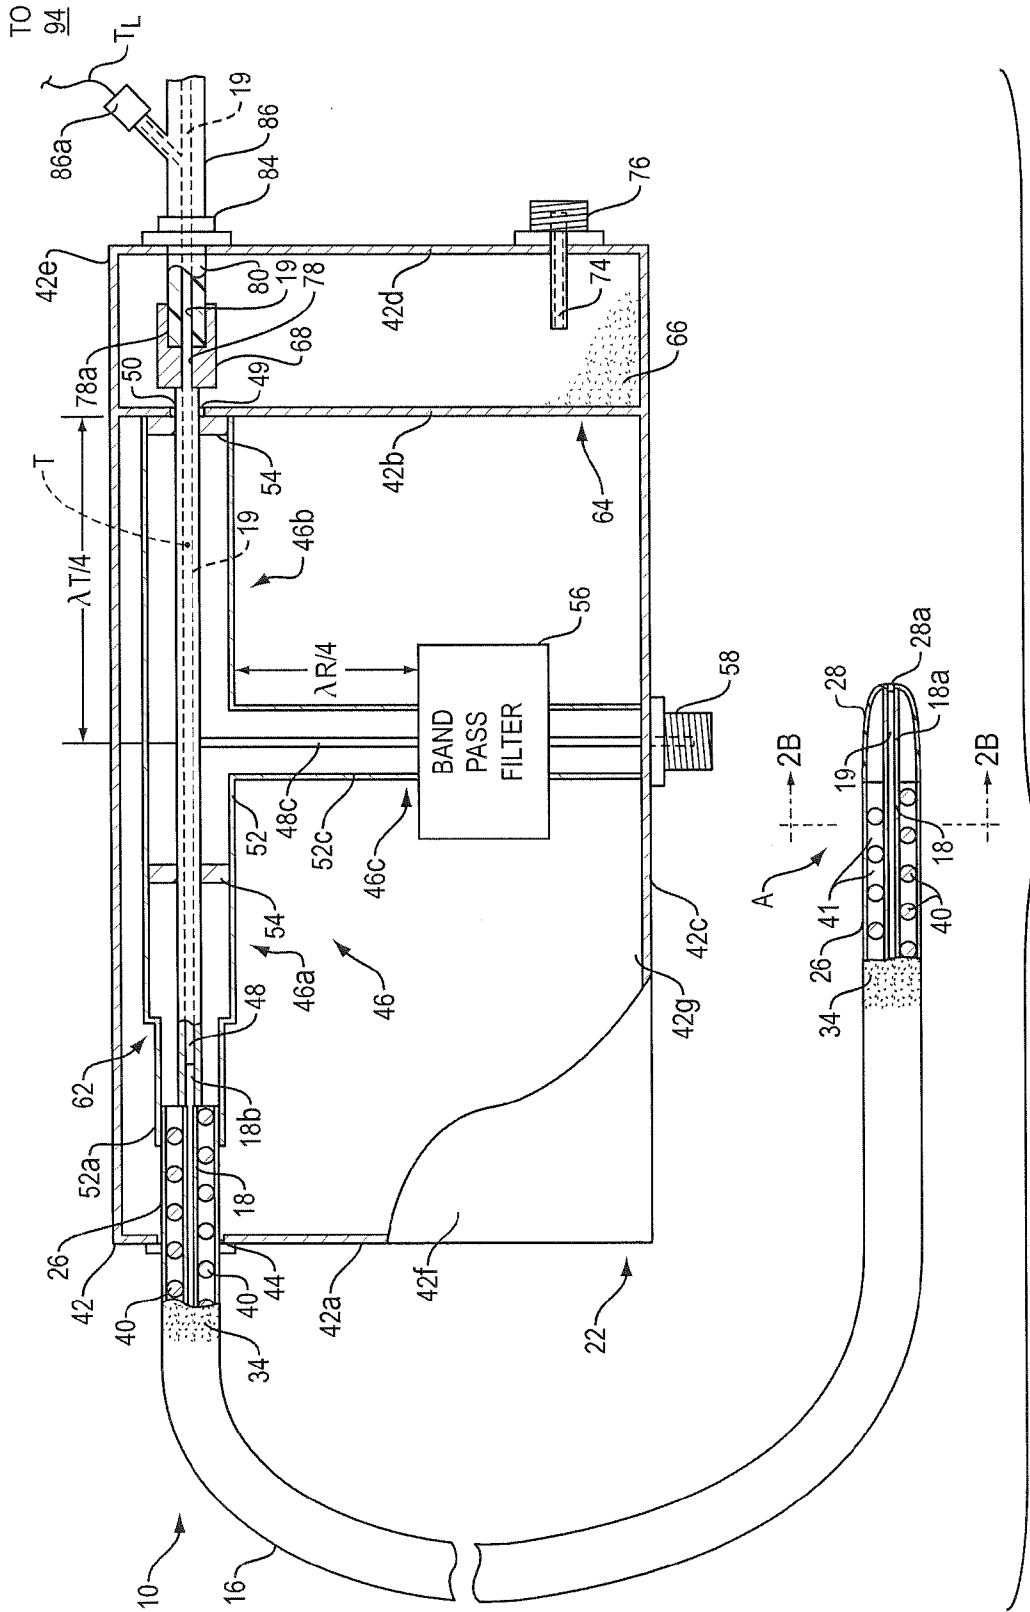


FIG. 2A

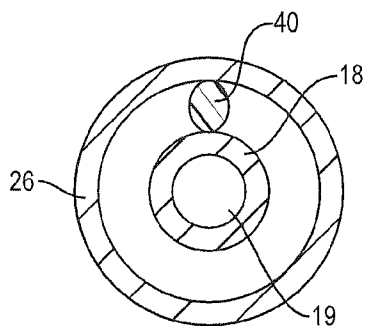


FIG. 2B

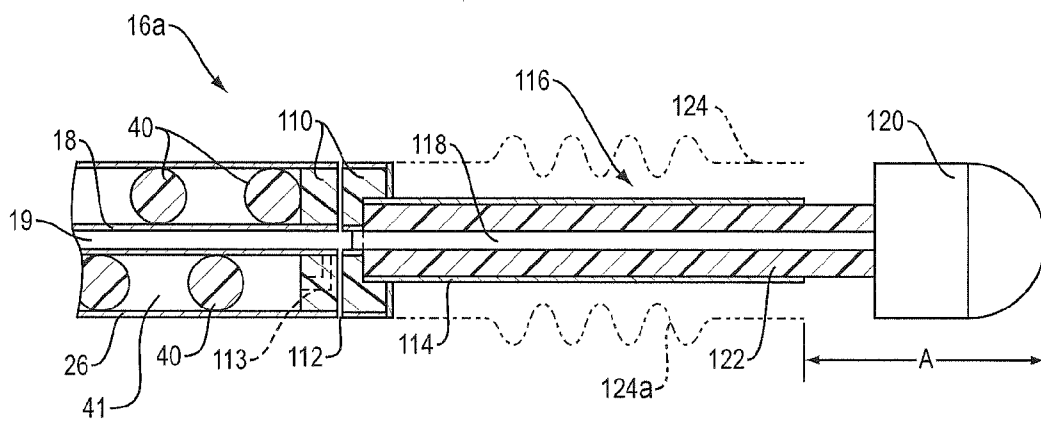


FIG. 3

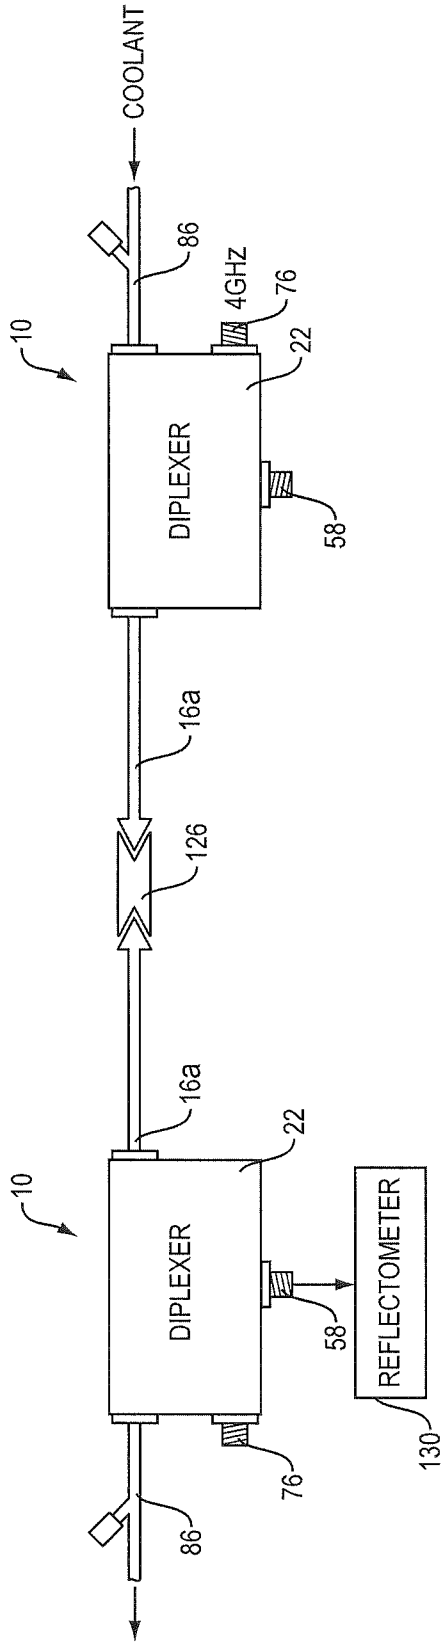


FIG. 4

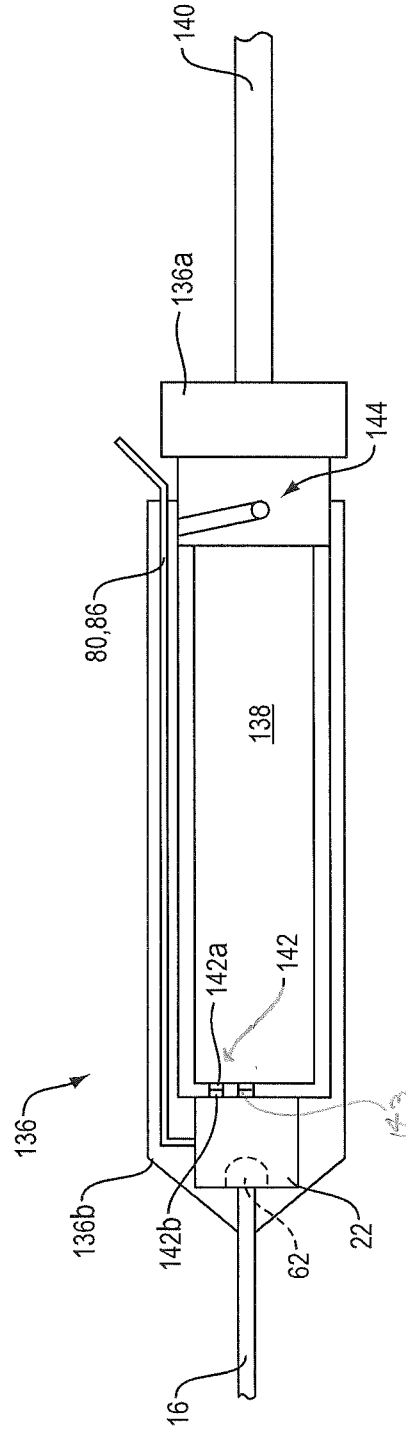


FIG. 5

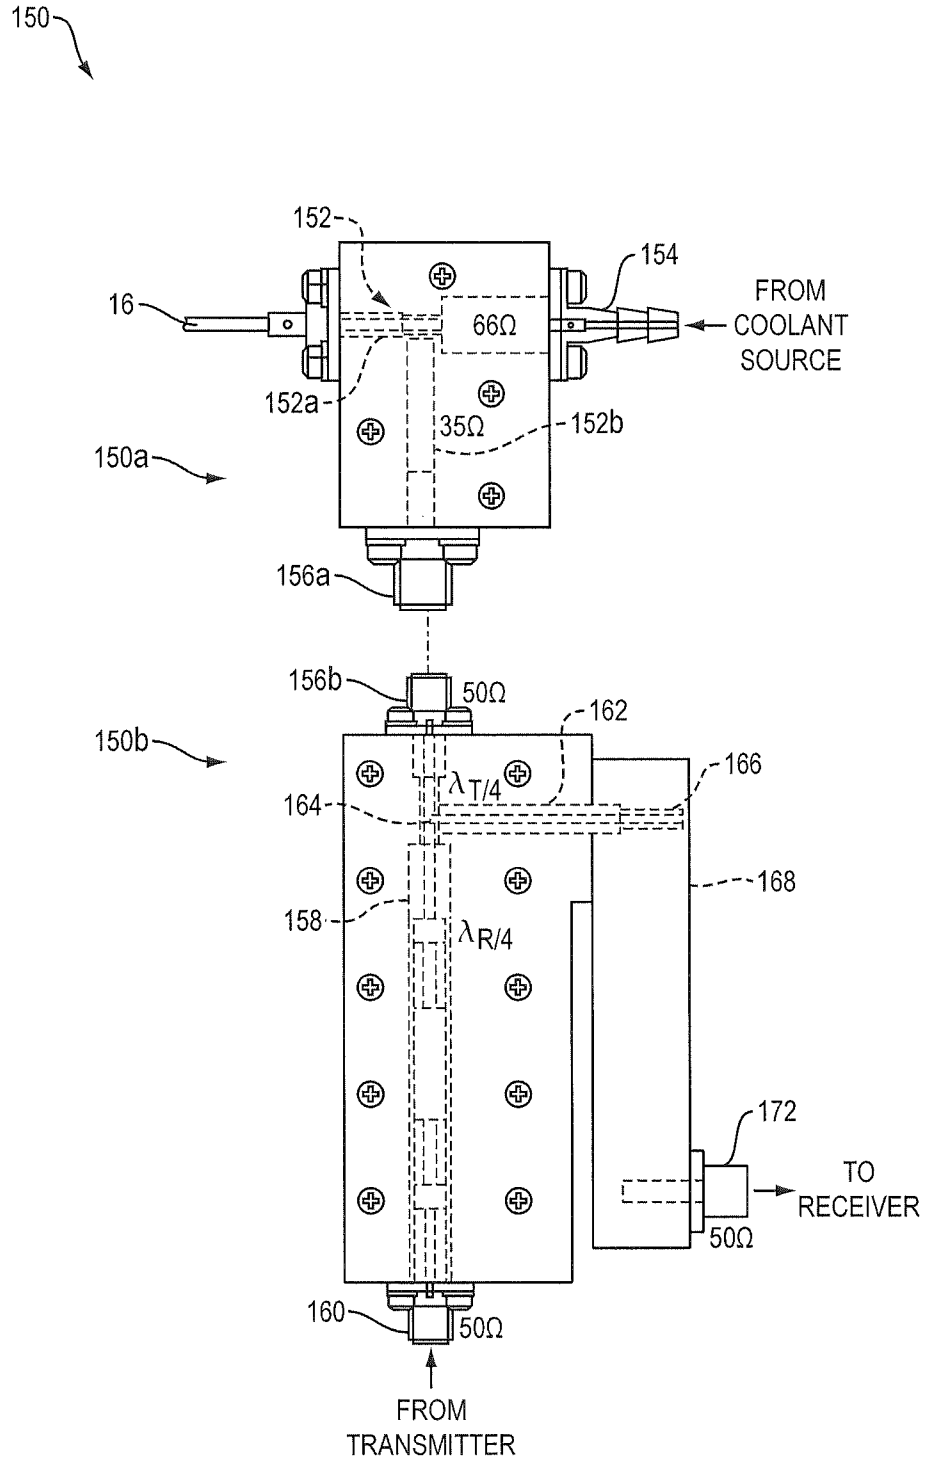


FIG. 6

HEATING/SENSING CATHETER APPARATUS FOR MINIMALLY INVASIVE APPLICATIONS

RELATED APPLICATION

[0001] This application claims the benefit of provisional application No. 61/635,348, filed Apr. 19, 2012, the contents of which are hereby incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] This invention relates to medical catheter apparatus for minimally invasive applications. It relates especially to catheter apparatus which utilizes electromagnetic radiation to simultaneously controllably heat, and detect the temperature of, fluid or tissue in a human or animal body. The apparatus includes an antenna catheter which is essentially a long flexible cable having a distal end or probe containing an antenna. In order to perform its function, the catheter must be small in diameter and flexible so that it can be threaded along blood vessels and other natural passages in the body to position the antenna at a selected target site.

[0004] By placing the catheter probe at the region of interest in the body, one may warm blood and/or ablate tissue to treat tumors, cardiac arrhythmias, renal disease, benign prostatic hyperplasia (BPH) and the like.

[0005] The proximal end of the catheter cable may be connected to an external control unit which includes a transmitter for transmitting electromagnetic energy via the cable to the antenna in the catheter tip in order to heat fluid or tissue, and a receiver which detects thermal emissions picked up by the antenna reflecting the temperature of that fluid or tissue. The receiver outputs a corresponding temperature signal to control a display which displays that temperature. The same signal may also be used to control the transmitter to maintain a selected heating profile.

[0006] For apparatus detecting thermal emissions in the microwave range which is of primary interest here, the receiver is usually a radiometer. Every component of a radiometer generates noise power that contributes to the overall noise of the system. Therefore, the total radiometer output signal contains not only noise received by the antenna, but also noise generated within the apparatus itself. Such variations within the apparatus can produce output signal fluctuations that are sometimes greater than the useful signal level to be measured. To overcome these gain variations, Dicke developed is the common load comparison radiometer which utilizes a switch, aka a Dicke switch, to alternately connect the antenna, (picking up the unknown thermal radiation) and a reference temperature (which may be a stable noise source or a temperature sensor within the catheter). This configuration greatly reduces the effects of short-term gain fluctuations in the radiometer. More particularly, the switch provides a mechanism to allow both the reference and the unknown signals to pass through the apparatus essentially at the same time relative to the expected gain drift in the radiometer's amplifiers such that any drifting gain will be applied equally to both the antenna and reference signals.

[0007] Since the radiometer input is switched at a constant rate by the Dicke switch between the antenna and the constant-temperature load, the switch-demodulated RF signal should, therefore, be inserted at a point prior to RF amplification in the radiometer and as close to the antenna as possible. Any component or transmission line located between

the unknown temperature being detected by the antenna and the Dicke switch can introduce an error. One such error source is the relatively long cable which connects the antenna in the catheter tip to the external radiometer.

[0008] In other words, the temperature of that cable contributes to the temperature measurement. The cable temperature is usually not known and varies along the length of the cable. That portion of the cable within the body will be at body temperature, whereas the segment of the cable outside the body will be at room temperature. All of these parameters may vary with the flexing of the cable and the depth of its insertion into the body. Also, when the apparatus includes a transmitter to heat fluid or tissue, some of the transmitter power (about 30 watts) is absorbed by the cable is causing the cable to be heated. If the loss in the cable is, say, 3 dB (which could easily be the case), one half of the antenna noise power may come from the desired tissue or fluid volume being examined at the target site and the rest results from the cable. Thus, all errors common to both measurements, i.e., the unknown temperature and the reference temperature, are cancelled in a Dicke-type radiometer. However, any changes or errors between the unknown and the Dicke switch affect only the unknown temperature measurement and are thus not common to both measurement paths.

[0009] Accordingly, to achieve accurate temperature measurement, it is highly desirable to minimize the losses between the antenna and the radiometer in order to improve the performance and reliability of the overall apparatus.

[0010] 2. The Prior Art

[0011] One way to minimize such losses and unwanted noise is to minimize the distance between the antenna and the radiometer by locating the radiometer in the catheter, thus essentially eliminating the cable in the receive path as described in U.S. Pat. No. 7,769,469. However, that solution rigidifies the catheter probe and places a lower limit on its diameter making it more difficult to thread the catheter along narrower blood vessels in the body and around sharp turns in such vessels and in other body passages. It also requires that wires extend along the cable to the radiometer.

[0012] Thus, there is a need for a microwave heating/sensing catheter apparatus of this general type whose catheter is small and flexible enough to be navigated along is such narrower and tortuous paths in the body, yet contributes minimal noise to the overall system.

SUMMARY OF THE INVENTION

[0013] Accordingly, it is an object of the present invention to provide an improved microwave heating/sensing catheter apparatus for minimally invasive applications.

[0014] Another object of the invention is to provide apparatus of this type whose antenna catheter is quite flexible and has a minimum diameter so that it can be navigated along small blood vessels and other irregular passages in a human or animal body.

[0015] A further object of the invention is to provide such apparatus having a reduced sensitivity to unwanted noise so that the apparatus can have an external radiometer.

[0016] Yet another object of the invention is to provide apparatus of this type whose antenna catheter has minimal insertion loss.

[0017] Other objects will, in part, be obvious and will, in part, appear hereinafter.

[0018] The invention accordingly comprises the features of construction, combination of elements and arrangement of

parts which will be exemplified in the constructions herein-after set forth, and the scope of the invention will be indicated in the claims.

[0019] In general, my catheter apparatus comprises an antenna catheter for insertion into a natural body passage, e.g., the vasculature, cardio-renal system, gastrointestinal tract, etc. of a human or animal body. When the catheter is to be threaded along narrow blood vessels, the catheter, especially its leading end portion, or probe should have a small diameter and be very flexible. Therefore, a diplexer and radiometer cannot be incorporated into the catheter probe as disclosed in the above patent. Rather, the antenna in the probe is connected to a transmitter and a Dicke-type radiometer located in an external control unit by a special, very low-loss flexible cable to be described later.

[0020] On the other hand, when the particular application does not demand such small size and flexibility, the radiometer and/or diplexer may be located anywhere along the cable either inside or outside the body or even in the probe.

[0021] When the transmitter is operative, it delivers electromagnetic energy of a first frequency via the cable to the antenna which radiates energy into the adjacent body tissue and/or fluid to heat same. That same antenna also picks up thermal emissions of a higher frequency from that tissue and/or fluid and delivers a corresponding signal via the cable to the radiometer which thereupon outputs a temperature signal indicative of the temperature of the heated tissue and/or fluid. Thus, the apparatus may be used to heat a fluid, e.g. blood, following a selected heating profile, and to heat or ablate tissue to treat tumors, BPH and various renal and cardio-renal diseases by modulating or denervating neurofibers.

[0022] To enable the catheter to heat (transmit) and detect temperature (radiometrically sense) simultaneously, a passive diplexer is provided at the proximal end of the cable, the cable and diplexer forming a unique assembly which also allows for cooling of the cable. That is, to minimize component insertion loss, the cable/diplexer assembly provides a reduced cable impedance as well as a fluid path for a coolant delivered from the control unit to the catheter.

[0023] Even when the catheter is to be introduced into larger body passages and thus may include an internal diplexer and radiometer as described in the above patent, it is desirable that the catheter apparatus include this special cable to prevent excessive heating of the cable by the transmitter.

[0024] As will be described in more detail later, the cable has a hollow center conductor and a relatively low cable impedance, e.g. 30 ohms, compared to the usual 50 ohms. Lowering the cable impedance lowers its insertion loss because, for a given cable outside diameter, the cable's center conductor may be larger, thus increasing its conducting surface area and lowering the current density in that conductor. The hollow center conductor also provides a passage for the aforementioned coolant. The cable's center conductor is surrounded by insulation in the form of one or more filament strands wrapped around the center conductor. These strand(s) improve cable flexibility, while creating spaces that reduce the cable's dielectric constant and thus its insertion loss. These spaces may also provide a return path for a gaseous coolant whose temperature may be controlled to maintain the center conductor at a constant, safe temperature regardless of the level of applied power to the antenna in the catheter thereby to enhance the radiometric sensing capability of the apparatus.

[0025] As we shall see, the distal or probe end of the cable may be designed to allow a gaseous coolant to be recirculated through the catheter or to allow a liquid coolant to be expelled therefrom into a blood vessel or other body passage, e.g. for irrigation. Also, the catheter antenna per se may be attachable to the distal end of the cable to enable the cable to be terminated by different-type antennas. The attachable antenna also allows the cable/diplexer assembly with its lower-impedance cable to be tested by replacing the antenna with a second cable/diplexer assembly and using a standard 50 ohm reflectometer and standard 50 ohm connectors as will be described later.

[0026] Thus, the present catheter apparatus with its unique cable/diplexer assembly has a minimum sensitivity to unwanted noise, yet its catheter is able to be navigated along, and around turns in, small blood vessels and other body passages. Therefore, it should find wide application in the non-invasive treatment by heating and ablation of many serious human and animal diseases and abnormalities.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] The invention description below refers to the accompanying drawings, in which:

[0028] FIG. 1 is a diagrammatic view of heating/sensing catheter apparatus incorporating the invention;

[0029] FIG. 2A is a sectional view with parts shown in elevation, on a larger scale, showing the cable/diplexer assembly of the FIG. 1 apparatus in greater detail;

[0030] FIG. 2B is a sectional view on a larger scale taken along line 2B-2B of FIG. 2A;

[0031] FIG. 3 is a fragmentary sectional view showing a portion of a second cable/diplexer assembly embodiment for use in the FIG. 1 apparatus;

[0032] FIG. 4 is a diagrammatic view of an assembly for testing the FIG. 3 cable/diplexer assembly;

[0033] FIG. 5 is a view similar to FIG. 1 of an apparatus embodiment with a disposable catheter cable and handle, and

[0034] FIG. 6 is a similar view of still another apparatus embodiment.

DETAILED DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

[0035] Referring to FIG. 1 of the drawings, the present catheter apparatus comprises an antenna catheter shown generally at **10** connected by a cable **12** to an external control unit **14**. Catheter **10** includes a relatively long, e.g. 115 cm., very flexible cable **16** which includes a center conductor **18** extending the entire length of the cable and forming an antenna **A** at the distal or probe end of the cable. The illustrated antenna **A** is a monopole, but it may have other forms such as a helix as in U.S. Pat. No. 5,364,336, whose contents hereby is incorporated herein by reference.

[0036] In accordance with the invention, center conductor **18** is formed as a thin-wall, e.g. 0.004 inch, tube of soft copper so that it is quite flexible and defines a fluid pathway **19** which extends the entire length of the cable. For example, that center conductor may have an OD of 0.024 inch. The larger diameter, hollow center conductor minimizes the current density thereon for a given cable diameter. This, in turn, minimizes the cable impedance and thus its insertion loss.

[0037] The proximal end of cable **16** may connect to a passive diplexer indicated at **22** which allows catheter **10** via antenna **A** to simultaneously emit electromagnetic energy of

a first frequency while picking up thermal radiation of a second frequency. Thus, when cable 16 is navigated along a blood vessel or other body passage or within a catheter guide to position antenna A at a selected target site in a body, catheter 10 may be activated by control unit 14 to heat fluid and/or tissue at the target site to accomplish the desired objective, while at the same time sensing the temperature of the heated fluid and/or tissue thereby enabling control unit 14 to display that temperature and control the heating process. Also as we shall see, the fluid pathway 19 which extends from the catheter through diplexer 22 and along cable 12 to a coolant source in control unit 14 allows a coolant to be flowed along cable 16 to maintain the center conductor 18 thereof at a relatively constant, low temperature. As we shall see, pathway 19 may include a return path from the cable to the coolant source in the event that the coolant is recirculated.

[0038] Referring now to FIGS. 2A and 2B, in addition to the hollow center conductor 18, cable 16 has a tubular outer conductor 26 preferably made of metal braid so that it is electrically conductive and quite flexible. The outer conductor 26 may have an ID in the order of 0.042 inch and is shorter than conductor 18 so that a projecting distal end segment 18a of conductor 18 forms antenna A. A hollow cap 28 of a dielectric material is provided at the distal or probe end of the catheter to cover antenna A and provide the probe with a rounded tip. The cap interior, if closed, connects the interior of the center conductor to the annular space between the two conductors. Preferably, the entire length of outer conductor 26 is covered by a layer or jacket 34 of a suitable dielectric material.

[0039] As usual with coaxial cables of this general type, the annular space between conductors 18 and 26 may be filled with a dielectric material. In this case, to maximize the flexibility of the cable while dielectrically loading the cable, the insulation is composed of one or more dielectric strands 40, e.g., Teflon® filament, wound around the center conductor 18. A given cable may have many strands 40 or as few as one, depending on the characteristics desired for that cable. In addition to providing flexibility, the filament creates spaces 41 between the filament turns that reduce the dielectric constant of the cable and give it a reduced impedance Z as follows:

$$Z_0 = \frac{138}{\sqrt{\epsilon}} \log_{10} \frac{D}{d} = 30 \text{ ohms}$$

[0040] where:

[0041] D=outer conductor ID=0.042 in.

[0042] d=center conductor OD=0.024 in.

[0043] ϵ =dielectric constant=1.25

[0044] As will be described later, the fluid pathway 19 may extend through a hole 28a in the cap 28 as shown in FIG. 2A so that a liquid coolant may be expelled from the catheter or the cap may be closed and a gaseous coolant recirculated back to control unit 14 via a return path constituted by the spaces 41 between the dielectric strand(s) 40.

[0045] As shown in FIG. 2A, diplexer 22 includes a housing 42 having an end wall 42a. The proximal end of cable 16 passes through an opening 44 in that wall and connects to one, i.e. the left, arm 46a of a T-stub transmission line shown generally at 46 which may be dielectrically loaded (not shown for clarity). Transmission line 46 includes a hollow center conductor 48 which receives and is connected to a protruding

end 18b of cable conductor 18. Thus, conductor 48 continues the fluid pathway 19 from the cable. Transmission line 46 also has a T-shaped outer conductor 52 whose left arm 52a is surrounds and connects to cable conductor 26 inside housing 42. The other, i.e. right, arm 46b of transmission line 46 extends to an interior wall 42b of housing 42 and the center conductor 48 thereof passes through a feedthrough 49 in wall 42b. The spacing of the two conductors 48, 52 of the transmission line 46 is maintained by a pair of dielectric spacers 54, 54.

[0046] The leg 46c of the T-stub transmission line 46, including a solid center conductor segment 48c and an outer conductor segment 52c, is connected by way of a low pass or band pass filter 56 to a coaxial connector 58 mounted to a side wall 42c of housing 42. The filter 56 may be a conventional printed circuit or a short length of coax (tube filter) which is cut off at the receive frequency. In any event, filter 56 is designed to pass the transmit frequency and block the receive frequency. Thus, transmission line 46 helps to separate the different frequency signals to and from antenna A. More particularly, it forms a quarter wave stub ($\lambda_T/4$) while also providing a matched 90° bend for a transmitter (heating) signal applied to connector 58 as will be described.

[0047] Preferably, a transformer indicated at 62 is provided in the left arm 46a of the transmission line to step up the 30 ohm cable 16 impedance to 50 ohms in the transmission line 46 so that the diplexer 22 can be tested, as will be described, using conventional connectors and test equipment designed for a 50 ohm cable. This impedance transformation may be implemented by stepping the outer conductor arm 52a, e.g. in two steps as shown in FIG. 2A, or by stepping the inner conductor.

[0048] Still referring to FIG. 2A, the housing interior wall 42b along with a housing end wall 42d, segments of the housing side walls 42c and 42e, and top wall 42f and bottom wall 42g form a waveguide indicated generally at 64 which may be filled with a dielectric material 66 to minimize its size. The right end of the transmission line center conductor 48 extending through feedthrough 49 is connected to a larger diameter waveguide probe 68 adjacent one narrower wall of waveguide 64, while a waveguide-to-cable transition 74 adjacent the opposite narrower wall projects into the waveguide 64 from a connector 76 mounted to the outside of housing end wall 42d which constitutes a broader wall of the waveguide. As will be seen, that connector may couple the temperature sensing signal from antenna A to a radiometer in control unit 14 (FIG. 1). The waveguide 64 constitutes a high-pass filter that passes the temperature sensing frequency, while blocking the heating frequency. It also provides a DC block, preventing center conductors 18, 48 from coupling directly to a patient. Thus, the combination of this filter and the transmission line 46 enables the diplexer to separate the two signals.

[0049] The waveguide probe 68 is unique in that it provides a coolant path as well as a microwave transition. More particularly, probe 68 is formed with an axial passage 78 which is countersunk at 78a to accept an end segment of a tube or conduit 80 of a dielectric material. Tube 80 extends to a connector 84 on housing end wall 42d where it may be connected to a comparable tube 86 extending along cable 12 to control unit 14. Alternatively, of course, tubes 80 and 86 may be a single length of tubing. Thus, probe 68 and tubes 80, 86 provide an extension of the pathway 19 in cable 16. With the inclusion of an injection port 86a in tube 86, the diplexer 22 can provide a path to cable 16 for the injection of a contrast

agent to track the position of the catheter via X-ray imaging during a treatment procedure. The injection port **86a** will also allow for the insertion of one or more thermocouples T (FIG. 2A) or other type of temperature sensor each having a lead T_L to monitor the temperature of a coolant flowing along fluid is pathway **19**.

[0050] As shown in FIG. 1, the control unit **14** includes a transmitter **92** which delivers power at a microwave heating frequency, e.g. 2.45 GHz to the antenna catheter **10** by way of a cable component **12a** connected to connector **58**. RF heating may also be employed, e.g. at a frequency of 500 KHz. In either event, transmitter **92** is controlled by a processor **94** which receives instructions via control buttons on a control panel **96** in unit **14**. Unit **14** also includes a radiometer **98** which receives the temperature-indicating signal from antenna catheter **10** via a cable component **12b** connected to connector **76**. The radiometer may have a center frequency of, say, 4 GHz. In order to minimize cable losses between antenna A and the radiometer, the radiometer may be located close to diplexer **22** in an extension of housing **42** as shown in phantom at **98'** in FIG. 1 or in cable **12b**. In either event, the signal from radiometer **98**, **98'** is conditioned by an amplifier **102** and routed to processor **94** which may process that signal to control a display **104** which thereupon displays, in real time, the temperature of the fluid and/or tissue being probed by catheter **10**. Of course, display **104** can also display other parameters related to the proper operation of the apparatus such as transmitter output power, reflected power, catheter cable temperature, elapsed time, etc.

[0051] Unit **14** also includes a coolant source **108** controlled by processor **94** to deliver coolant via tube **86** in cable **12** to antenna catheter **10**. For some applications, the coolant may be a liquid, e.g. 0.9% saline, in others, the coolant may be a de-watered gas which has the same microwave characteristics as air, e.g. nitrous oxide. The coolant flows along tube **86** to the fluid pathway **19** in center conductors **18**, **48**. As the coolant flows along the cable, it maintains the conductors **18** and **48** at a substantially constant relatively low temperature so that they have a relatively low loss regardless of the level of power delivered by transmitter **92**. Still, cable **16** has a minimum outside diameter and is quite flexible due to its tubular inner conductor **18**, braided outer conductor **26** and intervening spiral dielectric winding strand(s) **40**. If the coolant is a liquid, the pathway **19** may extend through a hole **28a** in cap **28** as shown in FIG. 2A and irrigate the probed body passage. If the coolant is a gas, the cap may be closed by blocking hole **28a**, and the coolant returned to source **108** along a return path provided by a passage from the interior of center conductor **18** to the spaces **41** between strands **40** in cable **16** and pathways (not shown) along diplexer **46** and cable **12** (FIG. 1). If a liquid coolant is to be returned along the cable and not expelled into the probed body passage, that may be done via a conduit extending between outer conductor **26** and jacket **34** or between the jacket and the catheter introducer or guide (not shown) placed in the blood vessel or other body passage prior to insertion of the catheter.

[0052] To use the catheter apparatus, a surgeon may insert the probe end of cable **16** into a patient's vasculature or other body passage using a conventional introducer. To facilitate navigating the cable to position its antenna A at a selected target site, a contrast agent may be injected, as needed, into the cable's fluid pathway **19** by way of the injection port **86a** or the agent may be added to the coolant supplied by source **108**. In either event, the position of the catheter probe may be

tracked using a fluoroscope or other X-ray apparatus to position the cable's antenna A at the target site. If desired, the catheter may include a stand off or centering device of a dielectric material shown in phantom at S in FIG. 1 such as the one disclosed in U.S. Pat. No. 6,210,367, the entire contents of which is hereby incorporated herein by reference. This allows the antenna A is to ablate tissue in a 360° pattern around the body passage and not just at a single contact point. Once the catheter is in place, the processor **94**, following instructions input at control panel **96**, may cause coolant source **108** to pump coolant through tube **86** to the pathway **19** in the cable/diplexer assembly **10** to maintain the cable's center conductor **18** and the diplexer's center conductor **48** at a selected relatively low temperature to prevent cable heating due to the power applied by transmitter **92**. Since the coolant pathway **19** in the catheter **10** is in the microwave receive path, receiver sensitivity is optimized.

[0053] Processor **94** also activates transmitter **92** so that power is delivered via cable component **12a**, diplexer **22** and center conductor **18** to antenna A at the probe end of the cable. Antenna A radiates electromagnetic energy at a first frequency, e.g. 2.45 GHz, into the adjacent fluid and/or tissue thereby heating same. At the same time, antenna A picks up thermal emission of a second frequency, e.g. 4 GHz, from that fluid and/or tissue and delivers a corresponding signal via conductor **18**, diplexer **22** and cable component **12b** to radiometer **98** in control unit **14**. That signal is detected by the radiometer and applied to processor **94** to control display **104** which thereupon displays that temperature. Processor **94** may also use that temperature signal to control transmitter **92** to follow a selected heating profile or to maintain the targeted fluid and/or tissue at the desired temperature to achieve a desired result, e.g., warm blood, ablate tissue, denervate neural fibers, etc. All the while, the coolant in fluid pathway **19** maintains the segments of the center conductor **18** of cable **16** both inside and outside the patient at a substantially constant temperature so that the insertion loss of the cable remains low-loss constant throughout the procedure.

[0054] As noted above, the temperature sensors T monitor the center conductor **18** temperature at various points along its length. The output(s) of the thermocouple(s) on lead(s) T_L are applied to processor **94** to enable the processor to control coolant source **108** to keep the conductor at a selected temperature, which temperature may be displayed by display **104**. Having the injection port **82a** located close to waveguide probe **50** allows insertion of thermocouples T, to measure both input and output coolant (conductor **18**) temperatures. The coolant also prevents overheating of the cable as a whole to prevent possible injury to the patient.

[0055] Refer now to FIG. 3 which shows a second cable embodiment **16a** for use in the cable/diplexer assembly **10**. The components of cable **16a** which are in common with cable **16** carry the same identifying numerals. Thus, cable **16a** comprises a center conductor **18** defining a fluid pathway **19** and an outer conductor **26** separated by a winding of dielectric strand(s) **40**. Cable **16a** differs from cable **16** in that its distal end includes a connection device **110** in the form of a bead of a dielectric material. If a liquid coolant is to be used, device **110** may be provided with one or more small diameter, e.g. 0.010 inch, radial passages **112** which extend through conductors **18** and **26** to connect the fluid pathway **19** in conductor **18** to the outside. Such holes filled with coolant do not significantly perturb the microwave transmission line comprising cable **16**. On the other hand, if the coolant is a gas, it

should not enter the blood stream. Therefore, in this event, the passages 112 are not present and a return passage may be provided in device 110 as shown in phantom at 113 in FIG. 3 into the spaces 41 in the cable to return the coolant to coolant source 108.

[0056] Center conductor 18 extends to the distal end of bead 110 and the outer conductor 26 wraps around the bead and connects to the outer conductor 114 of a smaller diameter cable extension or probe indicated at 116. Extension 116 may be a short length of 30 ohm cable, the center conductor 118 of which may be solid yet quite flexible. More particularly, extension 116 includes a solid wire center conductor 118 whose proximal end plugs into the distal end of hollow center conductor 18. Conductor 118 extends to a conductive end cap 120 spaced beyond the distal end of outer conductor 114 and conductors 114 and 118 are separated by a dielectric material 122 which may consist of wound strand(s) like strand(s) 40. The length of extension 116 beyond outer conductor 114 constitutes the antenna A.

[0057] Cable 16a has all of the advantages of cable 16. In addition, its narrower leading end extension 116 is very flexible so that it can be navigated around especially sharp turns in a patient's vasculature and other body passages. Alternatively, extension 116 may have the same diameter as cable 16a but with an outer conductor 124 formed with bellow-like convolutions 124a as shown in phantom in FIG. 3 to maximize its flexibility.

[0058] One advantage of this embodiment is that various different type extensions or probes 116 may be plugged into, or otherwise attached to, the end of cable 16a. These extensions may have various diameters and degrees of flexibility. For example, a given extension may have a solid center conductor 118 and a relatively small outside diameter to form a monopole antenna A as shown in solid lines in FIG. 3. Another extension may have a larger diameter as indicated in phantom in FIG. 3 and/or a hollow center conductor to provide a pathway for a liquid coolant in lieu of the passages 112 in connection device 110. Yet another extension may define an antenna A in the form of a helix as in the above U.S. Pat. No. 4,364,336.

[0059] In addition, the ability of the extension 116 in FIG. 3 to be formed separately from cable 16a allows the cable/diplexer assembly 10 to be tested using standard 50 ohm connectors and test equipment. More particularly, a pair of the assemblies 10 may be arranged back-to-back as shown in FIG. 4 with the distal ends of their cables 16a, without extensions 116, connected together electrically via a coaxial connector 126. All ports 58, 76 of both diplexers 22 are now at the standard 50 ohm impedance thus allowing the attachment of a standard 50 ohm reflectometer 130 to a connector 58. This enables simultaneous impedance measurements at both the transmitting and receiving frequencies, with or without coolant supplied via tubes 80, 86 and with or without power applied to a connector 76. After such testing, the cable/diplexer assemblies in FIG. 4 may be separated and cable extensions 116 attached to the distal ends of cables 16a prior to use thereof.

[0060] Thus, radiometric performance can be obtained with the transmitted power applied and radiometer measurements can be made with or without coolant flowing along pathway 19, and the flow rate and temperature of the coolant can be monitored. Most importantly, all test measurements can be made with commercially available 50 ohm microwave test equipment and connectors.

[0061] Providing catheter apparatus whose radiometer is external to the patient allows the option of making the cables 16, 16a and diplexer 46 as a disposable item. FIG. 5 illustrates an antenna catheter indicated at 136 composed of two separate but connectable parts 136a and 136b. Part 136a is a barrel-like re-usable part which may contain a radiometer 138 and an external cable 140, comparable to cable 12, for its connection to transmitter 92, amplifier 102 and coolant source 108 in control unit 14. Part 136a also has end contacts 142a which engage mating contacts 142b of part 136b when the two parts interfit as shown in FIG. 5. The mating contacts 142a, 142b may be part of a more or less conventional 50 ohm blind mate coaxial connector 142. Also, there is a coolant line connection 143 between parts 136a and 136b.

[0062] Part 136b is a sleeve-like disposable part which may encircle part 136a and be releasably locked thereto by any conventional locking means 144, such as mating threads, bayonet connection, spring-loaded pin, etc. Part 136b may include the catheter cable 16 or 16a, transformer 62 and diplexer 22 along with a segment of coolant tube 80 and perhaps tube 86. When assembled as shown, parts 136a, 136b may function as a catheter handle for cable 16 during a procedure. When the procedure is completed, these parts may be separated and part 136b, including its cable 16, may be disposed of in proper fashion.

[0063] Other partly disposable antenna catheters may be envisioned. For example, the disposable part may include only the catheter cable 16 and the transformer 62, the re-usable part having the diplexer 46, radiometer 98 and the cable 140.

[0064] Also as mentioned above, the radiometer and/or diplexer may be incorporated into the cable at any point along its length either inside or outside the body; see U.S. Pat. No. 7,197,356 and U.S. Pat. No. 7,769,469, the contents of which are hereby incorporated herein by reference. Also, the radiometer need not be integrated with the diplexer as in FIG. 5. Of course, there is no size (diameter) constraint on any segment of the cable outside the body.

[0065] Refer now to FIG. 6 which illustrates another antenna catheter apparatus is embodiment shown generally at 150 composed of a disposable part 150a and a re-usable part 150b. The proximal end of cable 16 is connected to part 150a which includes a T-shaped transmission line 152 whose arms 152a have a tubular inner conductor leading to a coolant connector 154 mounted to the side of unit 150a. Connector 154 may be coupled to a tube similar to tube 86 leading to a coolant source and having a port for the introduction of a contrast agent, thermocouple, etc. as described above. As before, the transmission line serves both as a coolant path and a transformer, i.e. 30/50 ohms. Transmission line 152 includes a branch or leg 152b leading to a standard 50 ohm port 156a mounted to the bottom of part 150a. Port 156a is adapted to be connected to a mating 50 ohm port 156b mounted to the top of part 150b. Part 150b contains a transmission line 158 which connects port 156b to a similar port 160 mounted to the bottom of part 150b. Also, a coaxial branch 162 extends from a dipole junction 164 in transmission line 158 to a waveguide-to-coaxial probe 156 adjacent to one end of a waveguide 168. A waveguide-to-coaxial port 172 is present adjacent the opposite end of the waveguide.

[0066] The apparatus embodiment 150 operates in more or less the same way as apparatus 10. When port 160 is connected to a transmitter and port 172 is connected to a radiometer, the transmission line 158 functions as a low pass or band

pass filter in the antenna transmit path and the waveguide **168** functions as a high pass, low loss filter in the receive path thereby separating the signals to and from the antenna at the distal end of cable **16**, while at the same time matching the impedance of cable **16** to the impedance of the standard 50 ohm ports **160**, **172**. Apparatus **150** has an advantage over apparatus **136** shown in FIG. **5** in that the coolant is not routed through part **150b** containing the diplexer per se. Thus, there is no need for a fluid connection like connection **143** between the disposable part **150a** and the reusable part **150b**. Yet, the coolant is still routed along most of the receive signal path from the antenna so as to obtain the advantages discussed above.

[0067] It should be understood that while we have shown the high pass filter component of the diplexers in apparatus **10** and **150** as being a waveguide, it may just as well be a more or less conventional printed transmission line structure e.g. stripline, suspended substrate, microstrip, etc. For example, a high pass filter of the suspended substrate type may include a metal enclosure having a rectangular cross-section and containing a printed circuit board spanning the narrow walls of the enclosure, the board bearing metalized strips on opposite faces of the board which are centered in the enclosure. The circuit board may be formed with a coolant path extending along the board between the metal strips where there is no microwave field so that the coolant does not adversely affect the operation of the diplexer. Of course, if that type of filter should be used in the FIG. **6** apparatus embodiment, no such cooling passage would be required.

[0068] It will thus be seen that the objects set forth above, among those made apparent from the preceding description, are efficiently attained. Also, certain changes may be made in the above constructions without departing from the scope of the invention. For example, in a given application, instead of ablating tissue using electromagnetic energy as described above, a cryogenic fluid, e.g. nitrous oxide, from coolant source **108** may be circulated through the catheter to cause tissue ablation or renal denervation by freezing the tissue; the temperature measurement process using the antenna catheter remains the same. Therefore, it is intended that all matter contained in is the above description or shown in the accompanying drawings shall be interpreted as illustrative and not in a limiting sense.

[0069] It is also to be understood that the following claims are intended to cover all of the generic and specific features of the invention described herein.

What is claimed is:

1. Catheter apparatus comprising

an elongated flexible coaxial cable having proximal and distal ends, said cable including a hollow center conductor, an outer conductor and an electrically insulating layer in an annular space between said conductors;

an antenna at the distal end of the cable;

a diplexer including a transmit path for connecting the antenna to a transmitter which transmits signals of a first frequency and a receive path for connecting the antenna to a receiver which detects signals of a second frequency, said diplexer isolating the signals on the two paths from one another;

a transmission line connecting the cable to the diplexer, said transmission line including a segment with a tubular inner conductor one end of which is connected to the center conductor of the cable and a second end of which

is adapted for connection to a coolant source, said center conductor and said inner conductor forming a continuous coolant pathway.

2. The apparatus defined in claim **1** wherein said receive path includes a first electrical filter.

3. The apparatus defined in claim **2** wherein said first filter comprises a waveguide with opposite ends, and

said inner conductor segment extends into the waveguide adjacent one end thereof forming a tubular probe therein that connects to a dielectric conduit extending out of the waveguide thereby continuing the coolant pathway, and

further including a waveguide-to-cable transition adjacent the other end of the waveguide and adapted for connection to a receiver.

4. The apparatus defined in claim **3** wherein the transmission line is a T-shaped transmission line with a leg in said transmit path adapted for connection to a transmitter, said leg including a second electrical filter.

5. The apparatus defined in claim **3** wherein the waveguide is loaded with a dielectric material.

6. The apparatus defined in claim **3** wherein the diplexer includes a housing containing the transmission line and waveguide, and

said conduit extends from the probe to the housing exterior and includes an injection port outside the housing.

7. The apparatus defined in claim **1** wherein said first filter comprises a waveguide with opposite ends, and said transmission line includes a branch extending into the waveguide adjacent one end thereof forming a probe therein, and

further including a waveguide-to-cable transition adjacent the other end of the waveguide and adapted for connection to a receiver.

8. The apparatus defined in claim **1** and further including an impedance-matching transformer in series with the cable and the transmission line.

9. The apparatus defined in claim **1** wherein the cable outer conductor comprises braided conductive strands.

10. The apparatus defined in claim **1** wherein the cable insulating layer comprises a flexible winding of one or more dielectric strands having multiple fluid flow paths therebetween.

11. The apparatus defined in claim **1** wherein said antenna comprises an extension of the center conductor beyond the outer conductor and the insulating layer.

12. The apparatus defined in claim **11** wherein said extension is tubular and continues said fluid pathway to the outside.

13. The apparatus defined in claim **1** wherein said antenna is connected to the center conductor via a connection device at the distal end of the cable.

14. The apparatus defined in claim **13** wherein the connection device defines a fluid path between the interior of the center conductor and the outside.

15. The apparatus defined in claim **13** wherein the connection device defines a fluid passage between the interior of the center conductor and said annular space so that said annular space can provide a coolant return path along the cable.

16. The apparatus defined in claim **1** wherein the antenna is flexible.

17. The apparatus defined in claim **1** and further including a stand-off device adjacent to the distal end of the cable for centering said antenna in a body passage.

18. The apparatus defined in claim 1 and further including one or more temperature detectors positioned in said fluid pathway for monitoring coolant temperature at one or more locations therealong.

19. The apparatus defined in claim 1 and further including a device for introducing an x-ray contrast agent into said center conductor.

20. The apparatus defined in claim 1 and further including a microwave or RF transmitter connected to said transmit path.

21. The apparatus defined in claim 1 and further including a coolant source connected to said second end of the tubular inner conductor of said transmission line segment.

22. Catheter apparatus comprising an elongated flexible coaxial cable having proximal and distal ends, said cable including

- a hollow center conductor;
- an outer conductor, and
- an electrical insulating layer in an annular space between said conductors, said insulating layer being constituted by one or more windings of a dielectric material defining multiple flow paths along said annular space, and

23. The apparatus defined in claim 22 and further including a connection device at the distal end of the cable connecting the interior of the center conductor to said annular space so that when a gaseous coolant is flowed into the proximal end of the cable, the coolant travels along the center conductor to the distal end of the cable and exhausts from the cable via said connection device and flow paths thereby cooling the center conductor.

24. The apparatus defined in claim 23 wherein the connection device comprises a closed hollow end cap secured to the distal end of the cable and which connects the interior of the center conductor to said annular space.

25. The apparatus defined in claim 24 wherein the center conductor extends into said cap to form an antenna.

26. The apparatus defined in claim 23 wherein the connection device comprises a bead in the annular space at the distal end of the cable, said bead defining a passage between the interior of the center conductor and the annular space.

27. The apparatus defined in claim 22 wherein the center conductor extends beyond the outer conductor at the distal end of the cable to form an antenna.

28. The apparatus defined in claim 27 and further including a stand-off device adjacent to the distal end of the cable for centering the antenna in a body passage.

29. The apparatus defined in claim 27 and further including a diplexer connected to the cable, said diplexer including a transmit path for connecting the antenna to a transmitter which transmits signals of a first frequency and a receive path for connecting the antenna to a receiver which detects signals of a second frequency, said diplexer being designed to isolate the signals on the two paths from one another.

30. The apparatus defined in claim 29 and further including an impedance-matching transformer in series between the cable and the diplexer.

31. The apparatus defined in claim 29 wherein said transmit path and said receive path are comprised of a T-shaped transmission line which is arranged and adapted to provide both a coolant path between a coolant source and said center conductor and an impedance matching transformer.

32. The apparatus defined in claim 29 wherein said cable and said diplexer are formed as a unitary disposable first part designed for connection both electrically and mechanically to a mating reusable second part containing microwave receiver.

33. The apparatus defined in claim 22 wherein said outer conductor comprises braided conductive strands.

34. The apparatus defined in claim 22 and further including one or more temperature sensors in said center conductor.

* * * * *