



- (51) International Patent Classification:
A61B 8/13 (2006.01) *A61B 8/14* (2006.01)
A61B 5/026 (2006.01)
- (21) International Application Number:
PCT/CA2016/051451
- (22) International Filing Date:
9 December 2016 (09.12.2016)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
62/265,682 10 December 2015 (10.12.2015) US
- (71) Applicant: 1929803 ONTARIO CORP. D/B/A KE2 TECHNOLOGIES [CA/CA]; 919 Elliott Avenue, Sudbury, Ontario P3E 6J5 (CA).
- (72) Inventors: EIBL, Joseph; 919 Elliott Avenue, Sudbury, Ontario P3E 6J5 (CA). KENNY, Jon-Emile; 55W 14th Street apt. 18A, New York, New York 10011 (US). MAGNIN, Paul; 85 East India Row #6A-B, Boston, Massachusetts 02110 (US). EIBL, Andrew; 919 Elliot Ave., Sudbury, Ontario P3E 6J5 (CA).
- (74) Agent: NORTON ROSE FULBRIGHT CANADA LLP; 1 Place Ville Marie, Suite 2500, Canada, Montreal, Ontario H3B 1R1 (CA).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: SYSTEMS AND METHODS FOR AUTOMATED FLUID RESPONSE MEASUREMENT

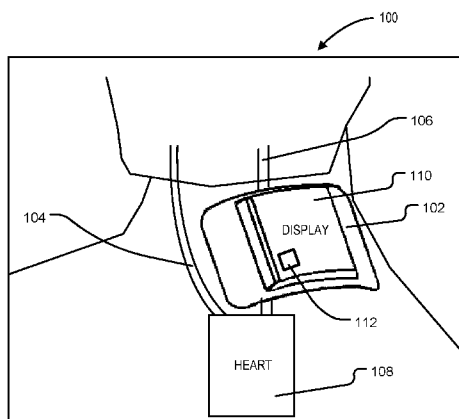


FIG. 1

(57) Abstract: A device is provided for automatically assessing functional hemodynamic properties of a patient is provided, the device comprising: a housing; an ultrasound unit coupled to the housing and adapted for adducing ultrasonic waves into the patient at a vessel; a detector adapted to sense signals obtained as a result of adducing ultrasonic waves into the patient at the vessel and to record the; and a processor adapted for receiving the recorded signals as data and transforming the data for output at an interface. Other devices, systems, methods, and/or computer-readable media may be provided in relation to assessing functional hemodynamics of a patient.



Published:

— *with international search report (Art. 21(3))*

SYSTEMS AND METHODS FOR AUTOMATED FLUID RESPONSE MEASUREMENT

FIELD

[0001] The present disclosure generally relates to the field of monitoring biological
5 signals, and more particularly, hemodynamic monitoring of one or more patients.

INTRODUCTION

[0002] Innovative, affordable, and/or portable non-invasive hemodynamic monitoring
devices may be desirable in the market. Such devices, for example, aid in the provisioning of
care of various individuals, (e.g., the critically-ill) by providing functional hemodynamic
10 assessments (which, in some embodiments, may be instantaneous or near instantaneous).

[0003] It is desirable to be able to assess functional hemodynamics in a variety of
circumstances. Unstructured environments and the variance in experience and training
among individuals responsible for assessing functional hemodynamics creates challenges.
These challenges are exacerbated when a patient requires monitoring over a protracted
15 period of time and many individuals are involved in assessing functional hemodynamics.
There is a need for a device that will produce precise and repeatable measurements under
these conditions.

SUMMARY

[0004] In accordance with an aspect, there is provided a portable hemodynamic
20 monitoring device comprising a housing configured for removable coupling to a body part of
an individual, the body part including at least one vessel of interest; an ultrasound unit
coupled to the housing and adapted for adducing ultrasonic waves into the at least one
vessel of interest in a continuous beam, the ultrasound unit including: at least one transducer
pair adapted to continuously detect reflected ultrasonic waves derived at least in part from
25 the produced ultrasonic waves directed at the at least one vessel of interest and oriented
such that, in concert, the at least one transducer pair produces the ultrasonic waves at an
angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of
fluid flow through the at least one vessel of interest; a processor.

[0005] In accordance with another aspect, the processor is further configured to continuously extract hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves in real-time or near real-time by applying a signal processing routine, and to store the extracted one or more hemodynamic parameters in a storage.

[0006] In accordance with another aspect, there is provided a sensory output device adapted to provide feedback on a quality of the extracted hemodynamic parameters, the sensory output device including at least one of (i) a graphical display and (ii) an auditory display. Wherein the orientation of the at least one transducer pair improves a probability of proper acoustic coupling between the ultrasound unit and the body part of the individual by enabling a plurality of redundant effective placement options of the housing on the body part of the individual, the plurality of redundant effective placement options reducing a required precision of placement of the device.

[0007] In accordance with another aspect, the signal processing routine includes processing the reflected ultrasonic waves according to a continuous wave Doppler ultrasound process.

[0008] In accordance with another aspect, the at least one transducer pair comprises a chain of transducer pairs.

[0009] In accordance with another aspect, the at least one transducer pair is at least one flexible polymer based transducer pair.

[0010] In accordance with another aspect, the at least one transducer pair is oriented in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.

[0011] In accordance with another aspect, the housing includes a tension bandage that is utilized to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient downward force is applied to the ultrasound unit.

[0012] In accordance with another aspect, the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.

5 [0013] In accordance with another aspect, the sensory output device is configured to generate a sensory output indicating an effectiveness of placement of the ultrasound unit.

[0014] In accordance with another aspect, processor is further configured to detect an estimated return of spontaneous circulation (ROSC) event by measuring a difference between a first relative blood flow from a chest compression and a second relative blood
10 flow from a heartbeat, and the sensory output device is configured to generate a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event and indicating that any chest compression activities should cease.

[0015] In accordance with another aspect, the housing includes at least one data communication device operable to transmit the extracted hemodynamic parameters from
15 one or more characteristics of the detected reflected ultrasonic waves over a data network.

[0016] In accordance with another aspect, the data communication device transmits the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data network to an external computer system.

[0017] In accordance with another aspect, the housing includes at least one data transfer
20 bus operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over a data connection.

[0018] In accordance with another aspect, the data transfer bus is operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data connection to one or more external connected
25 devices.

[0019] In accordance with another aspect, the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a

velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.

[0020] In accordance with another aspect, the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.

5 [0021] In accordance with another aspect, the frequency of the ultrasonic waves is a frequency is about 5 MHz.

[0022] In accordance with another aspect, the processor is configured to determine whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral of fluid flow through the at least one vessel
10 of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.

[0023] In accordance with another aspect, the sensory output device is configured to transmit a signal when the processor determines that the individual is undergoing
15 compensated shock.

[0024] In accordance with another aspect, the processor is further configured to: extract at least one first feature of interest from one or more characteristics of the detected reflected ultrasonic waves prior to an intervention event; extract at least one second feature of interest from one or more characteristics of the detected reflected ultrasonic waves subsequent to
20 the intervention event; determine at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.

[0025] In accordance with another aspect, the intervention event is the administering of at least one medicament.

25 [0026] In accordance with another aspect, there is provided a device adapted for automatically assessing functional hemodynamics of a patient, the device comprising: a housing; an ultrasound unit coupled to the housing and adapted for adducing ultrasonic

waves into the patient at a blood vessel; a detector adapted to sense signals obtained as a result of adducing ultrasonic waves into the patient at the blood vessel and to record the signals in the form of raw data; and a processor adapted for receiving the raw data and transforming the data for output at an interface.

- 5 [0027] In accordance with another aspect, the processor is further adapted to monitor functional hemodynamics (e.g., fluid dynamics) when the patient undertakes a fluid challenge activity.

- 10 [0028] In accordance with another aspect, the processor is further adapted to monitor functional hemodynamics both before and after the patient undertakes a fluid challenge activity.

[0029] In accordance with another aspect, the processor is further adapted to compare the data before the patient undertakes a fluid challenge activity and after the patient undertakes a fluid challenge activity to determine a change in velocity time integral of blood flow in the blood vessel.

- 15 [0030] In accordance with another aspect, the change in velocity time integral of blood flow in the blood vessel is tracked as a ratio.

[0031] In accordance with another aspect, the processor is further adapted to provide the ratio and a notification for a clinician if the ratio is 10% or greater.

- 20 [0032] In accordance with another aspect, the ultrasound unit is provided as an ultrasonic probe separate from the housing and coupled operatively to the housing.

[0033] In accordance with another aspect, the device is provided in the form of a portable ultrasound unit.

[0034] In accordance with another aspect, the device is provided in the form of a cart mounted ultrasound unit.

- 25 [0035] In accordance with another aspect, the ultrasound unit is integrated into the housing.

[0036] In accordance with another aspect, the processor is adapted to perform the automated detection of blood flow in the blood vessel, the processor receiving the raw data from adducing the ultrasonic waves (e.g., in a continuous beam or a pulsed beam) into the patient at an angle opposing the blood flow in the blood vessel, obtaining a velocity time
5 trace in relation to the blood flow, determining a velocity time integral, determining a cross-sectional surface area of the blood vessel, and utilizing the velocity time integral and the cross-sectional surface area of the blood vessel to establish the blood flow through the vessel across a period of time.

[0037] In accordance with another aspect, the processor is adapted to perform a
10 validation protocol for identifying an optimal set of parameters for operation of the device.

[0038] In accordance with another aspect, the optimal set of parameters includes at least one of placement position, fixation type, patch placement, and angle of incidence. In various further aspects, the disclosure provides corresponding systems and devices, and logic structures such as machine-executable coded instruction sets for implementing such
15 systems, devices, and methods.

[0039] In this respect, before explaining at least one embodiment in detail, it is to be understood that the embodiments are not limited in application to the details of construction and to the arrangements of the components set forth in the following description or illustrated in the drawings. Also, it is to be understood that the phraseology and terminology employed
20 herein are for the purpose of description and should not be regarded as limiting.

[0040] In various further aspects, the disclosure provides corresponding systems and devices, and logic structures such as machine-executable coded instruction sets for implementing such systems, devices, and methods.

[0041] In this respect, before explaining at least one embodiment in detail, it is to be
25 understood that the embodiments are not limited in application to the details of construction and to the arrangements of the components set forth in the following description or illustrated in the drawings. Also, it is to be understood that the phraseology and terminology employed herein are for the purpose of description and should not be regarded as limiting.

[0042] Many further features and combinations thereof concerning embodiments described herein will appear to those skilled in the art following a reading of the instant disclosure.

DESCRIPTION OF THE FIGURES

5 [0043] In the figures, embodiments are illustrated by way of example. It is to be expressly understood that the description and figures are only for the purpose of illustration and as an aid to understanding.

[0044] Embodiments will now be described, by way of example only, with reference to the attached figures, wherein in the figures:

10 [0045] **Fig. 1** is a perspective view of a device placed on the neck of a patient, according to some embodiments.

[0046] **Fig. 2** is illustrative of a conventional ultrasound unit, the GE VScan™ having a display, and a probe.

15 [0047] **Fig. 3** is an illustration of an example neck profile, according to some embodiments.

[0048] **Fig. 4** is a depiction of a common carotid artery (CCA) Flow Measurement Angle, according to some embodiments.

[0049] **Fig. 5** is an illustration of an example tensioning mechanism for maintaining acoustic coupling between the device and a body part according to some embodiments.

20 [0050] **Fig. 6** is an example block schematic diagram of a device, according to some embodiments.

[0051] **Fig. 7A-7B** is illustrative of some example components that may be utilized for interfacing with a patient's body, according to some embodiments.

[0052] **Fig. 8** depicts an example adhesive by 3M™.

[0053] **Fig. 9A-9C** illustrate a pocket-size embodiment; **Fig. 9A** provides a top elevation view, **Fig. 9B** provides a perspective view, and **Fig. 9C** provides a side cross-sectional view, according to some embodiments.

[0054] **Fig. 10** is an illustration of a pocket sized embodiment.

5 [0055] **Figs. 11A-11C** are illustrative of a small embodiment with a coupled probe, according to some embodiments. **Fig. 11A** is a front perspective view of the embodiment; **Fig. 11B** is a rear perspective view of the embodiment; and **Fig. 11C** is a partial view of the embodiment.

10 [0056] **Figs. 12A-12B** and **Figs. 13A-13C** are illustrative of a small embodiment with integrated probe, according to some embodiments. **Fig 12A** is a side view of this embodiment, and **Fig. 12B** is a perspective view of this embodiment. **Fig 13A** is a perspective view of a second version of the embodiment with integrated probe being held at a handle. **Fig. 13B** is a perspective view of the second version; and **Fig 13C** is a side view.

15 [0057] A cart embodiment is provided at **Figs. 14A** and **14B**; **Fig. 14A** is a front perspective view of a cart embodiment, and **Fig. 14B** is a side elevational view of the cart embodiment.

[0058] **Fig. 15** is a flow diagram displaying the typical stages of medical care a patient may undergo in the event of critical illness.

[0059] **Fig. 16** is a cross-sectional diagram of a device according to some embodiments.

20 [0060] **Fig. 17** is a top view diagram of a device according to some embodiments.

[0061] **Fig. 18** is a cross-sectional diagram of a device displaying the “saw tooth” configuring of the transducer-receiver pair and its orientation relative to blood vessels, according to some embodiments.

25 [0062] **Fig. 19** is a top view diagram of an ultrasound sensor and its orientation relative to blood vessels, according to some embodiments.

DETAILED DESCRIPTION

[0063] Embodiments of methods, systems, and apparatus are described through reference to the drawings.

5 [0064] The following discussion provides many example embodiments of the inventive subject matter. Although each embodiment represents a single combination of inventive elements, the inventive subject matter is considered to include all possible combinations of the disclosed elements. Thus if one embodiment comprises elements A, B, and C, and a second embodiment comprises elements B and D, then the inventive subject matter is also considered to include other remaining combinations of A, B, C, or D, even if not explicitly
10 disclosed.

[0065] Innovative, affordable, and/or portable non-invasive hemodynamic monitoring devices are desirable. Such devices, for example, aid in the provisioning of care of various individuals, (e.g., the critically-ill) by providing functional hemodynamic assessments (which, in some embodiments, may be instantaneous or near instantaneous).

15 [0066] There may be, however, various technical challenges in providing such a device, such as ensuring that readings are accurate, specific, and reliable within a tolerable performance range (e.g., accounting for the presence of noise, accounting for transient signals and/or aberrations); accounting for variations in physical dimensions and/or device placement, contact, and environment (e.g., differing neck sizes, contours, proximity of
20 device, signal transfer characteristics); accounting for variations in procedures performed in conjunction with the device (e.g., differing fluid challenges).

[0067] The device may also encounter challenges as it relates to practical implementation, for example, the device may benefit from a level of intuitiveness and/or ease of use (e.g., portability, disposability, cost, understandable process, form factor), heat
25 management, power (e.g., battery) management, adaptability to a variety of settings (including inside and outside of a hospital), etc.

[0068] Further, the device may benefit from a level of user-independent measurement repeatability, such that a patient, for whom many care-providers will be responsible, can

monitor functional hemodynamics accurately over a protracted period of time. It may be desirable for such a device to contain access to memory and log sensor data over said protracted period of time.

[0069] A robust measurement device may be desirable, such that the device can provide real-time feedback during, for example, chest compressions associated with cardiopulmonary resuscitation (CPR), among other operations where comparing pre-/post-intervention measurements may also be desirable. Further still, it may be desirable to provide a device that adheres to the patient such that the care-provider's hands may be freed to perform other critical functions.

[0070] **FIG. 1** illustrates the device **102** placed on the neck of a patient, according to some embodiments. The device **102** is illustrated having various components and structural aspects, and it should be noted that the device **102** is provided merely as an example and embodiments may have different, alternate, the same, more, and/or less components and structural aspects.

[0071] The patients that may use this device **102**, may, for example, be older in age and suffering from heart complications. The patients may be weak, may not be in a state of full awareness, and may be in danger of acute and critical illness. The device **102** may also be suitable for various other patient types.

[0072] Those patients who are alert are often in a stressful state. Though efficacy may be a significant factor, keeping the patient calm and comfortable is also an important factor.

[0073] A device **102** that seems to constrict or feel unnatural on the patient, such as a bulky or heavy neck mounted device **102**, might serve to increase patient stress. A smaller device **102**, or one with a detached probe, may be advantageous in this regard.

[0074] The device **102** shown is configured for providing automated fluid response ultrasound (AFRU), and may, for example, be a body mounted device **102** that may be configured to incorporate a portable ultrasound unit to provide one or more assessments of a patient with consistency and/or accuracy. The device **102** may provide functional hemodynamic assessments, for example the device **102** may determine a patient's fluid

responsiveness (FR), in an automated fashion. In some embodiments, the local site on the patient is generally the neck area, such that the carotid artery is the vessel of interest and carotid flow is the target measurement. In some embodiments, the vessel of interest may be another vessel (e.g., brachial artery, femoral artery, etc.) and, as a result, the target measurement may change accordingly.

[0075] The device **102** may, for example, be used in the context of various uses, including an automated ultrasound in combination with a leg raise, the use of an automated ultrasound to give live readings during a fluid challenge (e.g., passive leg raise), etc. Further, the solution of the present disclosure may be non-intrusive, may be used by untrained users, may include methods by which certain target blood vessels are automatically differentiated from the other blood vessels, etc., and the device **102** may, in some embodiments, be used for multiple measurements where the device **102** may be fixed in place between measurements. For example, in some embodiments in order to differentiate target blood vessels from other blood vessels, forward and reverse flow signals may be classified as venous or arterial by application of a flow profile (e.g., pulsatile positive direction against non-pulsatile + opposite of positive direction). The transducer beam may be wide enough to capture the entirety of both arterial and venous signals at a particular monitored cross-section.

[0076] A user interface **110** may be integrated or operatively paired with the device and thus the device **102** may not require external supporting hardware. However, the device may, in some embodiments, be integrated with a data communication device **112**, for example using the Bluetooth or Wi-Fi protocol. The data communication device **112** may allow the device to transmit outputs to an external system (e.g., an external computer system) for processing, data storage, display, etc. The user interface **110** may be a visual display, a speaker, or another interface capable of communicating messages to a user of the device. In some embodiments, the device **102** may contain one or more data transfer buses operable to provide non-networked data connection means that may allow the device **102** to transfer and receive data to and/or from external connected devices (e.g., universal serial bus (USB) hard drives, monitors, etc.).

[0077] In some embodiments, various disposables may be used with the device **102**, such as a disposable which integrates a patient interface with an acoustic carrier (e.g., the gel and adhesive). According to some embodiments, the device may communicate data to a secondary processing system via a communications network – the secondary processing system may process received data according to data-analytics models and/or may integrate received data with previously stored data.

[0078] In **FIG. 1**, the device **102** is depicted along with a patient's blood vessels (noted as reference numerals **104** and **106**, in this example, the carotid). In such an embodiment, the output of the device **102** may be indicative of reflected hypersonic waves transmitted by transponders forming part of the device **102**, and reflecting off of a vessel of interest (in this example, the carotid artery). The received reflected signals, when processed, may produce an output indicative of hemodynamic properties of blood flow from the patient's heart **108**, through the vessel of interest. The device **102** may output through the user interface **110**, for example, as various readings that can be interpreted by a machine and/or a healthcare practitioner. The blood flow and/or vessel walls may be tracked using an ultrasound sensor, and denoted as reflected signals undergoing a Doppler shift. The measured Doppler shift may be indicative of the movement of red blood vessels in blood through an artery or vein relative to the device **102** over time. The reflected signals may, when measured, produce values distinct from all other vasculature, which may facilitate isolation of reflected signals from a vessel of interest. The measured Doppler shift over a span of time may form the velocity time integral, and may be indicative of the amount of blood passing through a cross section over the span of time.

[0079] The device **102** may be configured to perform automated functional hemodynamic assessments in a vessel (e.g., a carotid artery, brachial artery, femoral artery, etc.). For example, the device **102** may be utilized to perform auto- focusing of an ultrasonic source (e.g., an ultrasound probe) at a number of different depths and angles, and then collect data that best fits the structure of a targeted blood vessel. In some embodiments, the device **102** may include a chain of transducer pairs oriented in a saw tooth pattern such that, in concert, the transducer pairs produce ultrasonic waves at an angle of incidence between about 25

degrees to about 60 degrees in respect of a plane of fluid flow (e.g., the direction of blood flow through a blood vessel) through the at least one targeted blood vessel.

[0080] According to some embodiments, the saw tooth pattern arrangement may function to aim the ultrasonic beam so as to reliably generate an angle of incidence of about 25-60
5 degrees (or thereabout) with general anatomical angle (for normal body types of 45 degrees). Use of this angle may enable reliable detection of reflected ultrasonic signals from the body part of the individual containing the vessel of interest toward which the ultrasonic beam (e.g., a continuous beam or pulsed beam) is directed without the intervention of a specifically trained technician or other individual. Acceptable angles, in accordance with
10 some embodiments, include +/- 1 degrees, +/- 2 degrees, +/- 3 degrees, +/- 4 degrees, among others.

[0081] Current methods require careful placement of ultrasonic monitors, often requiring the skill of an expert or trained individual in order to ensure effective readings. According to some embodiments, the saw tooth pattern arrangement may function to make available a
15 plurality of redundant, but effective, placement options on the body part of the individual, thus making it less difficult to obtain an effective reading from the vessel of interest. The redundant positioning may allow for the device to be used by a less skilled or, in some embodiments, even an unskilled user. Further, redundant positioning is helpful in emergency situations where non-ideal conditions in conjunction with a need for speed (e.g.,
20 individual is otherwise in great pain or dying), even for the skilled practitioner.

[0082] According to some embodiments, multiple transducer element pair designs, such as the saw tooth pattern, may also enable multi- or single element activation depending, for example, on the quality of the reflected signal received from the vessel of interest. For example, where a multi transducer element array containing 10 elements receives a
25 reflected signal from a vessel of interest that is sufficient to allow effective functional hemodynamic monitoring, the remaining eight elements may be de-activated or may enter a low power mode. This may provide benefits to power consumption and efficiency of operation (e.g., computational efficiency) and vessel identification.

[0083] The device **102** may be functional to perform automated functional hemodynamic assessments of a number of types of blood vessels. Depending on a particular vessel operable with the device **102** at a certain time, different depths and angles may be selected. The selection, for example, may be automated, based on the application of various pre-programmed instruction sets. The selection of such parameters is a non-trivial technical problem in view of variations of human physiology, blood vessel types, and practitioner skill levels. Further, the device **102** may operate, in some embodiments, such that it may be operable by unskilled practitioners and/or practitioners having less training (who may need to rely on the device **102** to select parameters based on sensed data and/or input data). The data retrieved from the ultrasound unit may be utilized, for example, to calculate relative blood flow (e.g., amount of blood / heart beat or unit time), and a potential advantage may enable variance in how the probe is oriented to the particular vessel being examined.

[0084] The device **102** may be configured to detect relative blood flow through a particular vessel (e.g., the carotid artery, brachial artery, femoral artery, etc.) . The device **102** may further be configured to indicate the level of cerebral perfusion that has occurred. The device **102** may further be configured to indicate whether the return of spontaneous circulation ("ROSC") has occurred. Where functional hemodynamics are measured during CPR, the device may be adapted to measure functional hemodynamic parameters (e.g., fluid dynamics) in a "binary" mode (i.e., fluid is either flowing through a vessel, or it is not). In other embodiments, the device may be adapted to provide a relative measure of a hemodynamic parameter such as the amount of fluid flowing through a cross-section of the vessel over a particular period of time (e.g., carotid, femoral, brachial, etc. blood flow rate). Measurement of relative carotid flow rate may be the most effective way to automatically detect ROSC.

[0085] As described in further embodiments, there may be various methods and/or techniques to aid in affixing and immobilizing the ultrasound unit (e.g., an ultrasound probe) to the local site on the patient in order to improve accuracy / fidelity of repeat measurements and, in some embodiments, provide real-time monitoring. For example, adhesives, tensioning bands, collars, pillows, etc. may be utilized. In some embodiments, housing is provided to which vascular probes could be attached and fixed to the neck at varying angles.

[0086] In some embodiments, the device **102** may be configured to communicate through one or more communication links (e.g., wired, wireless, cellular, local area networks, wide area networks, infrared, Bluetooth) with one or more receiver computing devices (e.g., for further analysis) and/or downstream computing devices (e.g., a data centre associated with a healthcare facility). Accordingly, the device **102** may or may not have a display **110**.

[0087] For example, the device **102** may be configured to provide outputs that may inform the function of other devices. The output of the measure can inform various individuals and/or machines of various hemodynamic parameters (e.g., features of the flow of blood through a vessel). For example, machines delivering cardio pulmonary respiration (CPR) can provide feedback on the efficacy and timing of chest compressions. The reader will understand that many other applications may be contemplated.

[0088] The device **102** may have various components to detect (e.g., monitor, track, probe, sense, determine, identify, investigate) various physical characteristics of the patient.

[0089] The device **102** of **FIG. 1** may be used in conjunction with specific workflows that may be adapted such that the device **102** and the workflows interoperate to provide accurate and repeatable localization (e.g., using the ultrasound readings).

[0090] The portable ultrasound unit may, for example, be a continuous wave Doppler ultrasound module that is capable of emitting ultrasonic waves in a continuous beam, and that is accurate and fast enough to provide a real or near-real-time analysis of parameters of the fluid flow in the blood vessel, in some embodiments, free of a bulky cart or cord. The device **102** may, for example, be portable enough to be carried around by a physician (e.g., for extended periods of time) or stored for sharing by multiple practitioners (e.g., in a 'grab-and-go' charging station for physicians).

[0091] In other embodiments, a pulsed wave Doppler ultrasound may be provided instead.

[0092] Continuous wave Doppler ultrasound modules may function to measure fluid velocities along the entirety of a scanned channel. For example, where the scanned area is a blood vessel, a continuous wave Doppler method may measure the velocities of fluids traveling through the entire scanned portion of the blood vessel over a period of time. In

contrast, pulsed wave Doppler ultrasound modules may only allow measurement of fluid velocities at a single point, or a very finite sequence of points, along a scanned channel.

[0093] Pulsed wave Doppler ultrasound modules may function by emitting a pulsed signal toward an area of focus for a finite period of time, then ceasing the emission of said signal and monitoring received signals in order to record a reflected frequency shift related to the original emitted signal for a finite period of time. This process is then repeated. Once the reflected signal is received, a processor calculates the velocity and flow of liquid through a channel at the area of focus (e.g., a blood vessel). Since pulsed wave Doppler ultrasound techniques require a finite signal emission period and a second finite signal monitoring period, there is a limit to how fast said techniques can accurately measure the flow of liquid through a channel – where the velocity of the fluid surpasses a certain point, temporal aliasing (a phenomenon whereby a recorded signal appears distorted due to a recording system with an insufficient sampling rate). This mode of operation can be described as “half-duplex”.

[0094] Continuous wave Doppler ultrasound modules function by emitting ultrasound signals in a continuous beam along a channel and continuously monitoring the multitude of reflected frequency shifts via a detector. This mode of operation can be described as “full-duplex” as the continuous wave Doppler ultrasound is continuously emitting and receiving signals. A potential advantage realized by this mode is that it enables the measurement of high-velocity flows of liquids through channels (e.g., blood through blood vessels) that could not be accurately measured using pulse wave Doppler ultrasound techniques due to the above-described temporal aliasing problem.

[0095] The device **102** may further include and/or be associated with a locating disposable that may be affixed once to the patient for various measurements, the measurements of which can be compared with one another. The device **102** and/or the locating disposable may require a level of ease of use and sufficient accuracy such that practitioners and care centres may readily adopt its usage.

[0096] The device **102** may be battery powered and may use a transducer array which may function to measure the Doppler shift produced by fluid passing through a vessel (e.g.,

a Doppler shift produced by red blood cells in blood travelling through an artery relative to the position of the device **102**. A technical challenge arises in relation to ensuring that the device **102** is configurable to identify (e.g., delineate, distinguish) flow through particular vessels (e.g., distinguish carotid flow from the jugular vein or other confounding objects).

5 [0097] In operation, a patch-like (or collar-style) probe may be adhered to local area of skin on a patient under which the patient's carotid artery (or other vasculature) passes. The probe may utilize ultrasound signal processing methods (e.g., Doppler signal processing functions) to identify pulsatile flow. When the ultrasound (e.g., continuous wave Doppler) function of the ultrasound signal is directed at an opposing angle to the blood flow, a
10 velocity-time trace may be obtained. By defining one cardiac cycle (pulse/heart beat), a unit time may be defined.

[0098] Calculating the area under the velocity-time curve (i.e., the calculus integral), the device **102** and/or a downstream device may utilize the data to determine the velocity-time integral ("VTI"), and the VTI may be multiplied by the cross-sectional surface area of the
15 vessel over the time of one cardiac cycle (heart beat). Accordingly, an automated physical measurement of a blood flow through the vessel per heartbeat may be obtained using an ultrasonic approach.

[0099] In some embodiments, an auto focusing mechanism is provided, where the device **102** may conduct a validation protocol to identify which settings are optimal (e.g., frequency, angle) for the patient's body, patch placement, and/or other parameters. A challenge with
20 conventional technologies is that the selection of these signals is non-trivial and may often lead to a high level of training required. For example, this aspect of the technology aids in allowing un-trained or less trained personnel to use the device **102** reliably.

[00100] A computing device may apply an algorithm in conjunction with detected readings
25 to determine the patient's velocity time integral (VTI, pre-challenge); prompt the physician for a fluid challenge (e.g., passive leg raise); detect and/or calculate a post-challenge VTI; and deliver an assessment of the patient's fluid responsiveness (increase of >10% VTI or output following fluid challenge). A ratio may be found between pre and post-challenge VTIs, and other thresholds may be used for assessments (e.g., 10%, 5%, 3%, etc. and may be

indicative of an increase or decrease). Where a condition is broken (e.g., as provided through a business rule), or a trigger triggered, a notification may be generated and/or provided (e.g., an alert, a sound, a display, a pop-up).

5 [00101] A display may, for example, aid the physician by providing various types of views, some views having various transformations (e.g., a simplified view), annotations (e.g., display markers, dynamic markers), analytics (e.g., determined aspects, averages, means, medians, identified aberrations), and/or a raw data view. For example, a post-/pre-VTI ratio may be determined, and a 10% or greater ratio may be indicative of a fluid responsiveness condition. Accordingly, some embodiments may be utilized to detect and/or determine
10 various characteristics in relation to a carotid anomaly, or detect a carotid anomaly or an anomaly regarding another vessel of interest (e.g., brachial artery, femoral artery, etc.).

[00102] There may be other types of ultrasound devices that can perform flow monitoring, however, drawbacks with conventional devices may be those typical of a multipurpose device: they are large, difficult to use, and may often require lengthy training or experience.

15 [00103] The device **102** of some embodiments may be configured such that there may only be a minimum level of required hardware to effectively monitor blood flow, and may reflect a trade of multi-functionality for size, providing additional benefits as in relation to operation for use with carotid flow procedures. At **FIG. 2**, a conventional ultrasound unit, the GE VScan™ **202** is pictured, having a display **204**, and a probe **206**.

20 [00104] Other catheter-based technologies may also be used for hemodynamic monitoring, but the conventional products may be cumbersome and add risk in the context of various procedures. Pulmonary artery catheterization is another technique that may be available for hemodynamic monitoring, wherein a catheter is inserted into the pulmonary artery via the vena cava to directly measure cardiac output. Pulmonary artery catheterization
25 can measure right atrium, right ventricle, and pulmonary artery pressure, as well as left atrium input pressure, but a major drawback is that the catheterization is invasive and limited to surgical use. Pulse Pressure Waveform Analysis (PPWA) is another technique that utilizes the arterial waveform, obtained either from an arterial catheter or a finger probe, in

order to calculate the stroke volume (SV) and the systemic vascular resistance (SVR), but complications may arise in view of non-linear and varying arterial wall compliance.

[00105] Phase shift technology / bio reactance approaches may be considered for use, wherein when an AC current is applied to the thorax, the pulsatile blood flow taking place in the large thoracic arteries causes the amplitude of the applied thoracic voltage to change. Research, however, has indicated poor performance in relation to critically-ill/post-operative patients; further, this approach may be hindered by environmental factors, such as overweight or patients which perspire heavily. Gas rebreathing techniques may also be used in relation to estimating CO non-invasively, but while easy to use, they have been shown to be adverse affected by spontaneously breathing patients. Septic Shock Algorithms may use aggregated historical data to predict the onset of septic shock, which can be diagnosed through blood pressure readings.

[00106] In some embodiments, the device may produce outputs functioning to allow detection of various types of compensated shock. Compensated shock may be defined, in an adult example, as systolic blood pressure above 90 mm Hg while exhibiting signs of inadequate perfusion (e.g., tachycardia). In such situations, the device may transmit an alert signal via a sensory output device.

[00107] **FIG. 3** is an illustration of an example neck profile, according to some embodiments.

[00108] Patients may have differing anthropometric parameters, including, for example, carotid anthropometries, neck anthropometries, etc. These parameters may be taken into consideration, for example, as the device may need to be fitted on to and/or used in close proximity to bodily features of the patients, and thus may need to be calibrated and/or accurately positioned.

[00109] For example, the minimum size (i.e. length) of the neck may determine the maximum size of a body mounted device. The neck length for the smallest 5% of the population is roughly 8 cm, and accordingly, the maximum comfortable height of the device may approximately be 8 cm.

[00110] Neck circumference also varies from person to person. The smallest neck circumferences may be about 312 mm, and the largest about 463 mm. For a round or square device (e.g. 8 cm in diameter or 8x8 cm square), the patient's neck would have to conform roughly 14 mm at the edges, too much for patient comfort. If the device were
5 curved, the neck would have to only conform roughly 5 mm, but a curved feature may add complexity (and likely size) to the device and/or components thereof.

[00111] As indicated in FIG. 3, the neck anatomy may be fairly consistent from patient to patient. For example, the internal diameter of the Common Carotid Artery (CCA) may be approximately 6.2 mm for women and 6.5 mm for men, ranging between 4.3 and 7.7 mm in
10 maximum and minimum sizes (as noted in a study having a study size of 123). The standard depth for a patient's CCA may be 20-40 mm below the skin. The wall thickness may be roughly 0.75 mm. Additionally, the diameter of the CCA may expand roughly 0.5 mm with every heartbeat.

[00112] Another study suggests that the ratio of the internal carotid and external carotid
15 artery diameters can be predicted as approximately .65 and .58 respectively (e.g., each is roughly 1/2 to 2/3 of the diameter of the CCA). The vertebral artery may be hidden in bone, very far away and very small. The jugular vein has blood flowing in the opposite direction (therefore "up" may have to be established).

[00113] Directional information can aid in the assessment of position. Dimensional
20 measurements can also be used to aid in position by assuming any measurement of a 5 diameter less than 4.3 mm is likely not the CCA.

[00114] Furthermore, a relationship can be established between distance and diameter of the CCA. A CCA further from the skin implies a larger bodied patient, who would be expected to have a larger CCA.

[00115] One study placed the ideal measurement location at 15-20 cm below the
25 bifurcation. The subclavian artery sits very close to the clavicle, and the CCA bifurcation is near the larynx (Adam's apple) meaning a reasonable measurement location is anywhere from 5-20 cm above the clavicle, or midway between the larynx and the clavicle.

[00116] Patients with larger neck diameters are likely to have a thicker layer of cutaneous tissue between the probe and the CCA. No papers studied described a correlation between bariatric patients and difficulty in reading CCA flow, meaning this may not be an issue. It may also mean that the full sized ultrasound machines currently in use are variable enough to
5 account for these differences. This patient profile may not be suitable for the AFRU. In some embodiments, multiple transducer pairs may be arranged end to end to form the transducer array. This may enable the device to contour to different patient morphologies on the neck, arm, torso and/or thigh, etc.

[00117] **FIG. 4** is a depiction of a CCA flow measurement angle, according to some
10 embodiments. A probe **402** is shown for measuring flow in relation to vessels **404**, being incident flow at plane **406**. Accordingly, sample images **408** (greyscale) and **410** (color) are shown.

[00118] Applicants considered various approaches to the ultrasound unit and made various decisions related to the design. In some embodiments, the ultrasound unit may
15 include a transverse and oblique array.

[00119] Other possible approaches included a single transducer or multidimensional transducers (i.e., a 2D array or a scanning 1D array). Though these other approaches still have a possibility of success, the transverse oblique array may be preferable in some
20 embodiments. The array may be oriented obliquely (as shown by the line indicative of plane **406**) to pass through the CCA such that the array can read anatomical information in the transverse plane, and Doppler signal processing information in the longitudinal plane.

[00120] In this architecture, there is a risk that suitably effective Doppler signal processing measurements may be difficult to obtain with a transversely oriented array. There is also risk that many elements will be required, resulting in a higher cost and size of the device.

[00121] As the ultrasound architecture may be an important aspect of the device, an
25 ultrasound investigation was conducted to test the effectiveness of the transverse array configuration.

[00122] FIG. 5 is an illustration of an example tensioning mechanism for maintaining acoustic coupling between a device 504 and a body part 502 according to some embodiments. The device 504 is housed in a housing 512 which may adhere to the surface of a body part 502 containing a vessel of interest. The housing may further contain a tensioning cover 510 which may be coupled on one side to the device 504. The housing may further contain two or more latching mechanisms 506 which may be situated perpendicularly to the body part 502 of the individual and within the housing 512. The latching mechanisms may each contain a plurality of latching channels 506a-f which may function to receive the edges of the tensioning cover 510 when downward force is applied thereto and hold the tensioning cover 510 in place, thereby causing the tensioning cover 510 to maintain position and, by extension, apply downward force to the device 504 such that it remains secure against the body part of the individual 502. This may cause the device 504 to be situated such that it maintains a position functional to produce a correct signal and read a correct reflected signal to and from the vessel of interest (e.g., within a correct range of distances from the vessel of interest).

[00123] FIG. 6 is an example block schematic diagram of a device, according to some embodiments. FIG. 6 illustrates an electrical architecture and may include various elements of electronic circuitry, etc. The device may be implemented in various forms, including, for example, by software, hardware, embedded firmware, and/or a combination thereof.

[00124] A user interface 602 may be provided for various input / sensory-output functionality, including the ability to receive parameters, etc. from users (e.g., patients, clinicians). Output functionality may be used to, for example, provide a graphical interface for clinicians and/or to communicate information to downstream computing systems (e.g., a clinical data center).

[00125] There may be various data storage units included for storing data (e.g., raw data, pre-processed data, processed data, post-processed data), and there may be one or more processors 604 utilized for conducting various determinations and/or calculations. The device may also, in some embodiments, have on-board memory that may be used to support various functionality, such as processing data for display to a clinician, etc. Various peripherals 606 may be utilized to provide various input signals and/or to receive various

outputs (e.g., through USB, Bluetooth, etc.). The processor **604**, for example, may be configured to control the peripherals **606**, and the user interface **602**. Ultrasound components may be provided, for example, through an ultrasound front end **612**, a probe, transducers **616a ... 616n**, which may be placed on and/or in proximity to a patient **618**. A power supply **610**, (e.g., a battery), may be utilized to supply power to the ultrasound components.

[00126] In some embodiments, the user interface **602** may be provided on a separate computing device, communicating with the Central Processing Unit ("CPU") **604** via one or more Peripherals **605**, hence the user interface **602** is depicted as connecting to the CPU **604** via a dashed line.

[00127] In operation, the front end may be provided and, in some embodiments, may include an eight-channel integrated circuit that may include the ultrasound front-end **612**, the probe **614**, and the transducers **616a ... 616n**. Signals passing through the front-end first may be amplified and/or filtered, and then passed through an anti-aliasing filter which may remove frequencies that may be too high to be sampled. These signals may then pass through an analog-to-digital converter and may be provided to a configurable integrated circuit (e.g., a field programmable gate array (FPGA), or a custom integrated circuit) **608** as, in some embodiments, low-voltage differential signals (LVDS).

[00128] An ultrasound emitter may be utilized to produce the high-voltage signal needed to drive the ultrasound transducers. The emitter may be provided a **+60V** and a **- 60V** power supply, and controlled by low-voltage logic signals from the configurable integrated circuit. Other voltages and/or power supplies may be utilized and the above is provided as an example.

[00129] The configurable integrated circuit **608** may be configured to control the emitter and receive LVDS signals from the front-end. The configurable integrated circuit **608** may be configured to perform digital signal processing that may be utilized to both send and receive signals, including beam-forming and Doppler shift computations.

[00130] The CPU **604** may host the operating system of the device, and may liaise between the configurable integrated circuit **608**, user interface (UI) **602** and any peripherals **606** that may be added to the system and/or perform post-processing on signals received from the configurable integrated circuit **608**.

5 [00131] The UI **602** may include an LCD touchscreen and/or an LCD screen with buttons. Other types of displays may be contemplated. Indicator lights, comprising for example LEDs, and indicators sounds generated from a speaker may also be part of the user interface **602** to provide feedback to the operator. In some embodiments, feedback corresponds to operating conditions of device **102** in order to direct the operator to orient device **102** to a
10 desirable and/or acceptable local site on the patient. The purpose of this direction may be to permit full operability of the device with a minimum of training or experience. If the device is required to be connected to the cloud, an onboard Wi-Fi module can be included along with additional peripherals **606** such as Bluetooth or USB.

[00132] A printed circuit board (PCB) may be provided to host some or all of the electronic
15 components within a structure (e.g., a housing, a base). In some embodiments, the device may be powered by a rechargeable or replaceable battery, which may be used to drive both the ultrasound and/or the other electronics (e.g., LCD screens, etc.).

[00133] As size is a consideration, lithium-ion technology may, in some embodiments, be selected as an option for compact power density. Operating under the assumption that these
20 batteries typically can store $77,000 \text{ Ah/cm}^3$ (amp-hours per cubic centimetre), the battery in the device may have to be, for example, 125 cm^3 for 1 hour of continuous active use. A Li-ion battery of this size may typically weighs about 250 g. Additional lifetime can be achieved by adding a larger (and heavier) battery, which may be suitable for a larger embodiment.

[00134] **FIG. 7** is illustrative of some example components that may be utilized for
25 interfacing with a patient's body, according to some embodiments. The method with which the device interfaces with the body may be an important factor for consideration. Such a component, for example, may be a "disposable" to connect (acoustically) the probe to the skin, and connect (mechanically) the device to the patient. Sample disposables are indicated at **702** and **704**.

[00135] In some embodiments, the disposable may integrate these aspects for quick application and disposition. This may avoid the disadvantage of applying ultrasound gel separately, which creates variability and mess.

[00136] In some embodiments, an approach includes combining the requirements into one solution: applying an acoustically transmissive adhesive (i.e., the adhesive also serves as the gel).

[00137] In some embodiments, the requirements may be separated: a material is provided for acoustic coupling and a material is provided for physical connection.

[00138] An example design may include utilizing an adhesive ring with a gel pad center. The adhesive connects the device and the gel (solid or liquid) provides an acoustic connection. The user would simply peel back the inside of the disposable stick it to the device, and then remove the cover of the patient side immediately before application.

[00139] The disposables may not need to be sterile (unless applications to open wounds are included in the indications), but should be held to a level of cleanliness typical of the industry.

[00140] Disposable ultrasound pads such as Rich-Mar AutoGel™, BlueMTech™ and Aquaflex™ ultrasound gel pads, may be provided to replace ultrasound gel (for the purposes of limiting cleanup) and may be utilized with the device. These pads may need to be wetted with water, and a standoff pad may be used to position the probe away to get a clearer picture of superficial areas of the skin (for example, ATS™ phantoms).

[00141] In some embodiments, a custom sized block can be centered under the probe head, adhered on one side to the device and covered on the other side by a dust cover that also keeps the disposable wetted.

[00142] As an alternative, ultrasound gel may be utilized. Gel could be pre-applied in a cavity in the disposable. A similar peel-back cover could expose the gel and make it ready for application. After use, the gel may have to be wiped off the patient.

[00143] An alternative method of acoustic coupling is a liquid filled pad. Similar to an ultrasound pad in its function and composition, these bags are filled entirely with liquid. A thinner liquid eliminates the likelihood of bubbles in the medium, but adds issues at the wall interface and with filling. For these reasons, liquid pads may be a less desirable alternative to those listed above.

[00144] In some embodiments, a tensioning material (e.g., a tension bandage) may be positioned around the body in order to provide a force normal to device **102** and ensure sufficient acoustic coupling.

[00145] In some embodiments, adhesives may also be utilized. **FIG. 8** depicts an example adhesive by 3M™. Adhesives may be hypo-allergenic and may stay in place for a number of days. The adhesive **802** may help keep a device and/or a portion thereof positioned in the target local site on the patient.

[00146] Silicone may be used as a protector and an acoustic coupling material for the probe/human interface, often used in conjunction with gel. For limited movement across the patient's skin, (e.g., with some embodiments of the device), the need for gel may be reduced and silicone alone might be effective. A drawback to silicone is a reduced speed of sound, which may require an algorithm to correct.

[00147] The device may require a mechanical housing that may vary in detail between embodiments. A rigid two part housing, for example, may be sufficient to provide a structure, with standoff points to hold the electronics. The housing may include spacers between components to avoid rattle or internal movement. The housing may need to be cleanable, and so may include gaskets to prevent water ingress at the seam, display, and buttons (keypad membrane).

[00148] Heat management may be an important consideration. The device may consume significant amounts of energy during use, and accordingly, the hot features of the device may need to be kept away from the patient to reduce the risk of burning (e.g., must be less than 43°C per ISO 60601).

[00149] If the heat generation is excessive, numerous strategies can be utilized, such as insulation or heat fins, designed inconspicuously into the exterior of the housing. A plastic housing may be a natural insulator but may cause the electronics to overheat.

5 [00150] A metal housing may have advantageous attributes: protecting the electronics at the expense of patient safety. If an embodiment is applied that does not connect to the patient directly then heat protection may not be a requirement.

[00151] If the housing is plastic, injection moulding can be used for manufacturing. If a metal housing is used, numerous options are available, though some may be more costly than injection moulding.

10 [00152] In some embodiments, the device may be provided as a single part. In some embodiments, the device is provided in having two or more parts; these parts may comprise a body, a probe, a separate computing device, a stand-alone cart, among others. For these embodiments, a probe wire may be provided to connect the body of the device to the probe.

15 [00153] Wires for this application may be available and may need to be strong enough to avoid pullout if the patient moves or the device falls. The probe itself (or the connecting surface on a one-part device) may benefit from a silicone interface piece, to protect the device and allow some conformity.

[00154] **FIGS. 9A-9C, 10, 11A-11C, 12A, 128, 13A-13C, 14A-148, 16, 17** may be illustrative of some sample embodiments of the device.

20 [00155] **FIGS. 9A-9C** may illustrate a pocket-sized embodiment; **FIG. 9A** provides a top elevational view, **FIG. 9B** provides a perspective view, and **FIG. 9C** provides a side cross-sectional view, according to some embodiments.

25 [00156] As depicted in **FIGS. 9A-9C**, an embodiment may include a pocket sized, body mounted ultrasound device that can be carried around by a clinician (e.g., the attending physician). The device may have an adhesive ring **902**, a body section **904**, and/or a display **906**. The adhesive ring **902** may provide an adhesive force between the periphery of the

body section **904** and the local site on the patient's skin. A concave space **908** may be provided for a gel pad or liquid gel.

[00157] The size of this embodiment may be reduced by using a number of strategies, including, for example: offloading processing and display to another device such as a tablet (or smartphone), changing its geometry to rest partially elsewhere, measuring flow in a different artery (to reduce comparative size), or reducing the battery life or removing it entirely (plug-in power only).

[00158] **FIG. 10** is an illustration of a pocket-sized embodiment. The embodiment may have display **1004**, a power button **1002**, and other buttons **1006** and **1008** that may be used, for example, to perform various input and output functions.

[00159] **FIGS. 11A–11C** may be illustrative of a small embodiment with a coupled probe, according to some embodiments.

[00160] **FIG. 11A** is a front perspective view of the embodiment; **FIG. 11B** is a rear perspective view of the embodiment; and **FIG. 11C** is a partial view of the embodiment. The device, may, for example, have a display **1102**, control button **1104**, power button **1106**, an integrated handle **1108**, a cable management apparatus **1110**, a probe **1112**, a charging port interface **1114**, a printed circuit board stack **1116**, and a battery **1118**.

[00161] The footprint and height of the device illustrated in **FIG. 11A-11C** in some embodiments may be approximately 6x6 inches and 4 inches respectively.

[00162] A coupled probe may provide a lower risk alternative to the pocket sized unit, while still being small and portable. The adhesive probe-patch may be coupled to the base unit via a cable.

[00163] The clinician (e.g., a physician) may place the unit on the examination table anywhere within range of the patient's neck, and extend and connect the probe. The probe may stay in place during the examination and possibly longer (for repeated exams). The device may be powered by a larger, more powerful battery than possible in a pocket-sized unit, but is also can support a wall plug for heavy use.

[00164] As the device may (in some embodiments) be too large to be carried around constantly, the device may be left at the charging station between patients, further extending battery life. The device may also be large enough to carry a gel holder, or an area to keep extra disposables. The device may include Wi-Fi and/or Bluetooth connectivity, or can transfer data via a base station. In other embodiments, the device may be miniaturized for portable use.

[00165] FIGS. 12A-12B and FIGS. 13A-13C may be illustrative of a small embodiment with integrated probe, according to some embodiments. FIG. 12A is a side view of this embodiment, and FIG. 12B is a perspective view of this embodiment. FIG. 13A is a perspective view of a second version of the embodiment with integrated probe being held at a handle, FIG. 13B is a perspective view of the second version; and FIG. 13C is a side view.

[00166] For example, the embodiment may include a probe 1204 for use with a patient 1202/1310, a base 1206, a display 1208/1306, and an adjustable neck 1210/1305. In some embodiments, a handle 1312 is provided. In these example embodiments, the device does not have a separated probe. Instead, an area of the main chassis contains the ultrasound head which may be placed against the patient.

[00167] Similar to the coupled probe model described above, these embodiments may contain a larger battery, a plug, wireless connectivity, and may contain storage for disposables. The embodiments may be simpler in design and use than the coupled probe, and more durable. A disposable may not be necessary, or if necessary may be a simpler disposable.

[00168] A cart embodiment is provided at FIGS. 14A and 12B; FIG. 14A is a front perspective view of a cart embodiment, and FIG. 14B is a side elevational view of the cart embodiment. The application on a medical cart may provide some advantages. For example, the central architecture does not differ significantly to other carts: the device 1402 may be provided on a cart apparatus 1406, having a handle 1404, and a base 1408. The embodiment may include a computer, monitor and screen 1410, with an ultrasound probe 1412, which may aid in simplifying the development process through the use of commercial

components. Less effort may need to be focused on miniaturization and integration than a more aggressive size.

5 [00169] The cart embodiment may also avoid logistical issues that may be present with portable units: for example, the embodiment may be unlikely to be lost or dropped, it may not require an area on the patient's bed to be positioned upon, and can be easily plugged in (or battery powered) with room for a long cord. The device may also not require an included charging station, and may thus be marketed as an individual unit.

[00170] The device may include a chassis **1206** and a user interface **1208** (i.e., a large touchscreen), and a probe **1204** that may differ significantly from other ultrasound units.

10 [00171] The probe **1204** may include a small adhesive patch at the end of a connection cable **1210** which can be installed on the patient and remains stuck during the procedure (or longer). The software may be configured to automatically find the CCA and to obtain readings, displaying only the results to the clinician (e.g., a physician) and eliminating the need for ultrasound expertise.

15 [00172] Some embodiments are adapted to respond to a protracted period of patient care. An example patient-care profile **1500** is provided in **FIG. 15**. Assessment of functional hemodynamic parameters (e.g., fluid dynamics) may be desirable at each phase of the patient-care profile **1500**. Different care-providers may be responsible at designated phases. A functional hemodynamics measurement device that is unique to a patient may be
20 desirable in order to provide continuous monitoring between phases and care-providers. Similarly, a functional hemodynamics measurement device that is unique to a care-provider may be desirable to provide monitoring of functional hemodynamics measurement to a plurality of patients.

25 [00173] A cross-sectional view and overhead view of some embodiments of the device are provided in **FIG. 16** and **FIG. 17** respectively. In some embodiments, an adhesive **1606/1704** may be employed to fix the device to the local site on the patient's skin; a tensioning material **1608/1708** may further be employed to apply a force normal to sensor housing **1612/1712**, and towards the local site in order to fix the device relative to the local site. The tensioning

material **1608/1708** may comprise a band, to be slug around the patient in order that tension may be adjusted by altering the length of upstretched band. The tensioning material may further be elastic, in order to eliminate discomfort to the patient, and also continue providing sufficient normal force while the patient moves and the body change shape.

5 [00174] In some embodiments, sensor housing **1602** may contain a transducer array **1602**, electronics, including but not limited to a visual display, speakers, and/or battery **1610**, and other electronics. In some embodiments, sensor housing **1612** is shaped like a half of an ellipsoid or American football. These shapes were found to be particularly useful in aiding proper positioning and tension characteristics to be applied.

10 [00175] In some embodiments, the sensor housing **1612** may contain a user interface unit **1620**, which may be a sensory output device operable with the visual display, speakers, and/or battery **1610**. The user interface unit **1620** may function to communicate inputs generated by a user interaction to the device. For example, the user interface unit **1620** may comprise a sensory output device such as a capacitive touch input device coupled with a
15 visual display **1610**. The user interface unit **1620** may function to allow the user to input selections that, when received by the device, cause the device to modify its operation mode (e.g., user input may cause the device to being a process operable to determine a pre-intervention/post-intervention VTI ratio as described below).

[00176] In some embodiments, the transducer array **1602** comprises transducer-receiver
20 pairs, where the transducer component generates acoustic waves, transferred into the patient acoustically through a hydrogel or acoustic coupler **1604**. The acoustic waves travel through the patient, and are modulated and reflected by media interfaces, for example fluid within a blood vessel. Reflected and modulated waves are sensed by a receiver component in the transducer-receiver pair and within the larger transducer array **1602**. In some
25 embodiments, the Doppler shift in a frequency modulated signal generated by the transducer **1602** may provide an accurate representation of the velocity of an element. In some embodiments, the element to be measured is the fluid flow within a blood vessel; non-limiting examples including the carotid artery, the brachial artery, or the femoral artery.

[00177] According to some embodiments, a sensor consisting of a ultrasound transducer **1804** and receiver **1806** may be configured as depicted in **FIG. 18** and **FIG. 19**, representing a cross-sectional view and an overhead view respectively. Transducer **1804** and Receiver **1806** may be configured such that they parallel to each other, and each directed at a 45 degree angle to the transverse plane (i.e., the plane defined by the surface of the skin **1808** at the local site on the patient). The transducer **1804** and receiver **1806** may resemble two match-sticks, tangent along one edge, as depicted in **FIG. 18**.

[00178] In some embodiments, the orientation of the transducer **1804** and receiver **1806** is configured such that the angle between the vectors defined by the direction of the ultrasound wave and the direction of blood flow is approximately 45 degrees. The transducer pair **1802** can detect blood flow direction by the sign (i.e., positive or negative) of the Doppler shift. An increase in frequency (positive shift) indicates blood flowing towards the ultrasound wave generated by the transducer **1804**, and vice versa. In some embodiments, the acceptable functional range is about 45-degrees $\pm$ 15-degrees, with 45-degrees representing the preferred embodiment. The reader will understand that in some embodiments, the acceptable functional range may be about 44-degrees $\pm$ 14-degrees, about 46-degrees $\pm$ 16-degrees, etc.

[00179] In some embodiments the ultrasound wave (i.e., Doppler beam) is “unfocused”; that is, the beams sweep out an angle of approximately 20-degrees, such that by directing the beam approximately 45-degrees from the transverse plane (as defined by the plane of the skin at the local site), the transducer **1804** will generate a wave that intersects with the blood vessel, and the angle of acceptance of the receiver **1806** (also 20-degrees) is large enough to receive the reflected and modulated signal generated by the blood flow. In this example, the width of the transducer face may be as small as 0.34 mm. This size is suitable for high-frequency (i.e., approximately 7 MHz) applications where high focal loss may be acceptable. Further, the width of the transducer may be as large as 2.15 mm. This size is suitable for low-frequency (i.e., approximately 4 MHz) applications where only low focal loss is acceptable.

[00180] In another example, a beam that sweeps out approximately 60-degrees can be constructed. The width of the transducer face may be as small as 0.924 mm. This size is

suitable for low-frequency (i.e., approximately 4 MHz) applications where high focal loss may be acceptable. Further, the width of the transducer may be as large as 1.52 mm. This size is suitable for high-frequency (i.e., approximately 7 MHz) applications where only low focal loss is acceptable.

5 [00181] In some embodiments, the functional frequencies of ultrasound waves generated by the transducer **1804** and detectable by the receiver **1806** are approximately 3-8 MHz. In some embodiments, approximately 5 MHz may be the frequency generated by the transducer **1804**. Typically, a lower frequency may be desirable for larger patients, as vessels such as the carotid artery, femoral artery, brachial artery, etc. are typically further below the
10 skin surface **1808**.

[00182] The orientation of the “match-stick” configured transducer pair **1802** may, in some embodiments, be fixed relative to the skin surface **1808** by a tensioned bandage **1810** which provides a force normal to the transducer pair **1812** and directed towards the skin surface **1808**.

15 [00183] In some embodiments, an audio or visual cue based on the Doppler shift measured by the ultrasound transducer pair **1802** may guide the placement of the device relative to the local site on the patient. A stronger signal relative to the noise sensed by the transducer pair **1802** may be processed by the CPU **604** and outputted to a peripheral speaker or display **606**. The output may comprise, for example, a particular sound (e.g.
20 “whoosh”), a change in volume, or frequency of beeps in the case of an audio cue, or it may comprise, for example, brightness, number of LEDs activated, the flashing of a pre-selected image, among others in the case of a visual cue.

[00184] In some embodiments, the sensor consists of a “chain” of transducer pairs **1802**, as depicted in **FIG. 19**. Transducer pairs **1802** are mutually connected via co-axial cable.
25 The increased length to the overall sensor increases the acceptable area that the device may be placed by increasing the likelihood that the target blood vessel passes under at least one transducer pair **1802**.

[00185] In some embodiments, a “chain” may be preferable to a singular, but longer transducer pair **1802**, because it may allow the housing to be constructed out of a flexible material that in turn will better conform to the various shapes and sizes of patients. Alternatively, in some embodiments, the transducer may be a flexible polymer transducer (e.g., a highly non-reactive thermoplastic fluoropolymer such as Polyvinylidene difluoride (PVDF)), this may also allow the housing to be constructed out of a flexible material and enable the housing to better conform to patients of various shapes and sizes. Producing the external housing in a flexible fashion may facilitate better acoustic coupling between the device **102** and the body and a higher signal to noise ratio.

[00186] In some embodiments, the transducer pair **1804** is a piezo ceramic material. In some embodiments, each piezo ceramic element, representing an individual transducer **1804** or receiver **1806** is 10x1x1 mm in shape. The piezo ceramics in some embodiments may be a PZT-5A or PZT-5H or a combination thereof. In some embodiments, the current draw is approximately 25 mAh. In some embodiments, the device may have a mode designed to conserve power and extend battery life. For example, the device may turn on only a pre-set times or it may only turn on at the request of a user and automatically turn off (or “sleep”) after a defined period of time.

[00187] In some embodiments, the transducer pairs **1804** may be adapted to sense peak velocity of the Doppler Shift, VTI, or the pre-intervention/post-intervention VTI ratio. The device **108** may, according to a pre-programmed instruction set, implement one or more “sampling windows” which may perform a calibration routine functional to eliminate the inherent variability of Doppler signal. The calibration routine may: a) record signals recorded by the transducer pair during a pre-defined span of time prior to the intervention (e.g., 10 seconds) as a “pre-intervention window”; b) cease recording signals during a corresponding pre-defined span of time during the intervention as an “intervention window”; and c) record signals during a corresponding pre-defined span of time subsequent to the intervention as a “post-intervention window”. One advantage of the device is the ability to measure both heart rate (“HR”) and VTI. This permits the calculation of the HR/VTI ratio – an index that (unlike the Shock Index) is not subject to vascular constriction as a compensatory mechanism during the onset of shock.

[00188] In some embodiments, the design, orientation, and frequency of the ultrasonic transducers are specifically designed to facilitate the rapid and repeatable measurement of the signal of interest (e.g., the ultrasonic signal reflected from the vessel of interest). Subsequently, the measured signal of interest is automatically processed by the signal processing routine in order to generate an output.

[00189] Currently available point of care ultrasound machines require several manual steps to be completed in order to return a valid output. Further, successfully completing several of these steps requires users to have specific training and skill. For example, currently available point of care ultrasound machines may require: manual identification of the vessel of interest using an ultrasound imaging screen; manual orientation of the angle of an ultrasound probe in relation to the vessel of interest to produce useful readings; manual identification of the vessel of interest to activate a Doppler function (e.g., a Doppler signal processing function); maintaining a substantially motionless positioning of both the ultrasound probe and the body part containing the vessel of interest; and manually executing a command in order to cause a reading to be taken. Further, often these steps must be executed repeatedly in order to compare changes in outputs received pre and post intervention (e.g., pre and post introduction of a medicament).

[00190] In contrast, some embodiments described herein may: automate some or all of the previously described steps; remove or reduce the requirement for manual identification of a vessel of interest; remove or reduce the requirement to manually orientate the ultrasonic transducer(s) relative to the body part of the person containing the vessel of interest; may automate the process of identifying a vessel of interest and activating a Doppler function; may serve to automatically or substantially automatically maintain a substantially motionless positioning of the ultrasonic transducer(s) relative to the vessel of interest; and may automatically generate readings, outputs, and compare pre and post intervention values to measure changes.

[00191] The embodiments of the devices, systems and methods described herein may be implemented in a combination of both hardware and software. These embodiments may be implemented on programmable computers, each computer including at least one processor,

a data storage system (including volatile memory or non-volatile memory or other data storage elements or a combination thereof), and at least one communication interface.

[00192] Program code is applied to input data to perform the functions described herein and to generate output information. The output information is applied to one or more sensory
5 output devices. In some embodiments, the communication interface may be a network communication interface. In embodiments in which elements may be combined, the communication interface may be a software communication interface, such as those for inter-process communication. In still other embodiments, there may be a combination of communication interfaces implemented as hardware, software, and combination thereof.

10 [00193] Throughout the foregoing discussion, numerous references is be made regarding servers, services, interfaces, platforms, or other systems formed from computing devices.

[00194] It should be appreciated that the use of such terms is deemed to represent one or more computing devices having at least one processor configured to execute software instructions stored on a computer readable tangible, non-transitory medium. For example, a
15 server can include one or more computers operating as a web server, database server, or other type of computer server in a manner to fulfill described roles, responsibilities, or functions.

[00195] The embodiments described herein are also implemented by physical hardware, including computing devices, servers, receivers, transmitters, processors, memory, displays,
20 and networks. The embodiments described herein provide useful physical machines and particularly configured computer hardware arrangements.

[00196] The embodiments described herein are also directed to electronic machines and methods implemented by electronic machines adapted for processing and transforming ultrasonic signals which represent various types of information. The embodiments described
25 herein pervasively and integrally relate to machines, and their uses; and the embodiments described herein have no meaning or practical applicability outside their use with computer hardware, machines, and various hardware components.

[00197] Substituting the physical hardware particularly configured to implement various acts for non-physical hardware, using mental steps for example, may substantially affect the way the embodiments work. Such hardware limitations are clearly essential elements of the embodiments described herein, and they cannot be omitted or substituted for mental means
5 without having a material effect on the operation and structure of the embodiments described herein. The hardware is essential to implement the various embodiments described herein and is not merely used to perform steps expeditiously and in an efficient manner. In some embodiments, the device is a single or special purpose machine that is specifically designed to perform limited set of functionality.

10 [00198] Although the embodiments have been described in detail, it should be understood that various changes, substitutions and alterations can be made herein.

[00199] Moreover, the scope of the present application is not intended to be limited to the particular embodiments of the process, machine, manufacture, composition of matter, means, methods and steps described in the specification. As one of ordinary skill in the art
15 will readily appreciate from the disclosure, processes, machines, manufacture, compositions of matter, means, methods, or steps, presently existing or later to be developed, that perform substantially the same function or achieve substantially the same result as the corresponding embodiments described herein may be utilized.

[00200] As can be understood, the examples described above and illustrated are intended
20 to be exemplary only.

WHAT IS CLAIMED IS:

1. A portable hemodynamic monitoring device comprising:

a housing configured for removable coupling to a body part of an individual, the body part including at least one vessel of interest;

an ultrasound unit coupled to the housing and adapted for adducing ultrasonic waves into the at least one vessel of interest in a continuous beam, the ultrasound unit including:

at least one transducer pair adapted to continuously detect reflected ultrasonic waves derived at least in part from the produced ultrasonic waves directed at the at least one vessel of interest and oriented such that, in concert, the at least one transducer pair produces the ultrasonic waves at an angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest;

a processor configured to continuously extract hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves in real-time or near real-time by applying a signal processing routine, and to store the extracted one or more hemodynamic parameters in a storage; and

a sensory output device adapted to provide feedback on a quality of the extracted hemodynamic parameters, the sensory output device including at least one of (i) a graphical display and (ii) an auditory display;

wherein the orientation of the at least one transducer pair improves a probability of proper acoustic coupling between the ultrasound unit and the body part of the individual by enabling a plurality of redundant effective placement options of the housing on the body part of the individual, the plurality of redundant effective placement options reducing a required precision of placement of the device.

2. The portable hemodynamic monitoring device of claim 1, wherein the signal processing routine includes processing the reflected ultrasonic waves according to a continuous wave Doppler ultrasound process.
3. The portable hemodynamic monitoring device of claim 1, wherein the at least one transducer pair comprises a chain of transducer pairs.
4. The portable hemodynamic monitoring device of claim 1, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.
5. The portable hemodynamic monitoring device of claim 1, wherein the at least one transducer pair is oriented in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.
6. The portable hemodynamic monitoring device of claim 1, wherein the housing includes a tension bandage that is utilized to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient downward force is applied to the ultrasound unit.
7. The portable hemodynamic monitoring device of claim 6, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
8. The portable hemodynamic monitoring device of claim 1, wherein the sensory output device is configured to generate a sensory output indicating an effectiveness of placement of the ultrasound unit.
9. The portable hemodynamic monitoring device of claim, wherein the processor is further configured to detect an estimated return of spontaneous circulation (ROSC) event by measuring a difference between a first relative blood flow

from a chest compression and a second relative blood flow from a heartbeat, and the sensory output device is configured to generate a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event and indicating that any chest compression activities should cease.

10. The portable hemodynamic monitoring device of claim 1, wherein the housing includes at least one data communication device operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over a data network.
11. The portable hemodynamic monitoring device of claim 10, wherein the data communication device transmits the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data network to an external computer system.
12. The portable hemodynamic monitoring device of claim 1, wherein the housing includes at least one data transfer bus operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over a data connection.
13. The portable hemodynamic monitoring device of claim 12, wherein the data transfer bus is operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data connection to one or more external connected devices.
14. The portable hemodynamic monitoring device of claim 1, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.
15. The portable hemodynamic monitoring device of claim 1, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.

16. The portable hemodynamic monitoring device of claim 1, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.
17. The portable hemodynamic monitoring device of claim 1, wherein the processor is configured to determine whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.
18. The portable hemodynamic monitoring device of claim 17, wherein the sensory output device is configured to transmit a signal when the processor determines that the individual is undergoing compensated shock.
19. The portable hemodynamic monitoring device of claim 1, wherein the processor is further configured to:
 - extract at least one first feature of interest from one or more characteristics of the detected reflected ultrasonic waves prior to an intervention event;
 - extract at least one second feature of interest from one or more characteristics of the detected reflected ultrasonic waves subsequent to the intervention event;
 - determine at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.
20. The portable hemodynamic monitoring device of claim 19, wherein the intervention event is the administering of at least one medicament.
21. A method for hemodynamic monitoring, the method comprising:

removably coupling an ultrasound unit to a body part of an individual, the body part including at least one vessel of interest, the ultrasound unit including at least one transducer pair forming a transducer array operable to emit and receive ultrasonic waves;

producing, by the transducer array, the ultrasonic waves at an angle of incidence between about 25 degrees and about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest;

adducing the ultrasonic waves into the at least one vessel of interest and receiving, in a continuous fashion, reflected ultrasonic waves;

determining whether the reflected ultrasonic waves are derived at least in part from the adduced ultrasonic waves directed at the at least one vessel of interest;

extracting a plurality of hemodynamic parameters from one or more characteristics of the reflected ultrasonic waves determined to have been derived at least in part from the adduced ultrasonic waves by executing a signal processing routine; and

providing feedback on the extracted plurality of hemodynamic parameters via at least one sensory output device, the at least one sensory output device including at least one of: (i) a graphical display; and (ii) an auditory display.

22. The method for hemodynamic monitoring of claim 21, wherein the signal processing routine includes a continuous wave Doppler ultrasound process capable of measurement of high velocity fluid flow through the at least one vessel of interest.

23. The method for hemodynamic monitoring of claim 21, wherein the at least one transducer pair is a chain of transducer pairs.

24. The method for hemodynamic monitoring of claim 21, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.
25. The method for hemodynamic monitoring of claim 21, wherein the at least one transducer pair is oriented in a in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.
26. The method for hemodynamic monitoring of claim 21, wherein removable coupling is provided by a tension bandage operable to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient force is applied to maintain the removable coupling.
27. The method for hemodynamic monitoring of claim 26, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
28. The method for hemodynamic monitoring of claim 21, further comprising generating a sensory output indicating an effectiveness of placement of the ultrasound unit.
29. The method for hemodynamic monitoring of claim 21, further comprising detecting an estimated return of spontaneous circulation (ROSC) event by: measuring a difference between a first relative blood flow from a chest compression and a second relative blood flow from a heartbeat; generating a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event; and, indicating, by the sensory output, that any chest compression activities should cease.

30. The method for hemodynamic monitoring of claim 21, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data network.
31. The method for hemodynamic monitoring of claim 30, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data network to an external computer system.
32. The method for hemodynamic monitoring of claim 21, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data connection.
33. The method for hemodynamic monitoring of claim 32, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data connection to one or more external connected devices.
34. The method for hemodynamic monitoring of claim 21, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.
35. The method for hemodynamic monitoring of claim 21, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.
36. The method for hemodynamic monitoring of claim 21, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.
37. The method for hemodynamic monitoring of claim 21, further comprising determining whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral

of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.

38. The method for hemodynamic monitoring of claim 37, wherein the sensory output device is configured to transmit a signal when the individual is determined to be undergoing compensated shock.

39. The method for hemodynamic monitoring of claim 21, further comprising:

extracting at least one first feature of interest from one or more characteristics of the received reflected ultrasonic waves prior to an intervention event;

extracting at least one second feature of interest from one or more characteristics of the received reflected ultrasonic waves subsequent to the intervention event;

determining at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.

40. The method for hemodynamic monitoring of claim 39, wherein the intervention event is the administering of at least one medicament.

41. A computer readable medium having machine readable instructions stored thereon for hemodynamic monitoring of at least one vessel of interest in a body part of an individual, the machine readable instructions, when executed by a processor, performing a method comprising:

emitting and receiving ultrasonic waves through at least one transducer pair forming a transducer array, the transducer array forming part of an ultrasound unit which is removably coupled the body part of the individual;

producing, by the transducer array, the ultrasonic waves at an angle of incidence between about 25 degrees and about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest;

adducing the ultrasonic waves into the at least one vessel of interest and receiving, in a continuous fashion, reflected ultrasonic waves;

determining whether the reflected ultrasonic waves are derived at least in part from the adduced ultrasonic;

extracting a plurality of hemodynamic parameters from one or more characteristics of the reflected ultrasonic waves determined to have been derived at least in part from the adduced ultrasonic waves by executing a signal processing routine; and

transmitting feedback on the extracted plurality of hemodynamic parameters to at least one sensory output device, the at least one sensory output device including at least one of: (i) a graphical display; and (ii) an auditory display.

42. The computer readable medium of claim 41, wherein the signal processing routine includes a continuous wave Doppler ultrasound process capable of measurement of high velocity fluid flow through the at least one vessel of interest.
43. The computer readable medium of claim 41, wherein the at least one transducer pair is a chain of transducer pairs.
44. The computer readable medium of claim 41, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.
45. The computer readable medium of claim 41, wherein the at least one transducer pair is oriented in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between

about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.

46. The computer readable medium of claim 41, wherein the ultrasound unit is coupled to a housing, the housing including a tension bandage operable to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient force is applied to maintain the removable coupling.
47. The computer readable medium of claim 46, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
48. The computer readable medium of claim 41, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: generating a sensory output indicating an effectiveness of placement of the ultrasound unit.
49. The computer readable medium of claim 41, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: detecting an estimated return of spontaneous circulation (ROSC) event by: measuring a difference between a first relative blood flow from a chest compression and a second relative blood flow from a heartbeat; generating a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event; and, indicating, by the sensory output, that any chest compression activities should cease.
50. The computer readable medium of claim 41, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data network.

51. The computer readable medium of claim 50, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data network to an external computer system.
52. The computer readable medium of claim 41, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data connection.
53. The computer readable medium of claim 52, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data connection to one or more external connected devices.
54. The computer readable medium of claim 41, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.
55. The computer readable medium of claim 41, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.
56. The computer readable medium of claim 41, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.
57. The computer readable medium of claim 41, wherein the machine readable instructions, when executed, further cause the processor to perform a step of: determining whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral

of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.

58. The computer readable medium of claim 57, wherein the sensory output device is configured to transmit a signal when the individual is determined to be undergoing compensated shock.

59. The computer readable medium of claim 41, further comprising:

extracting at least one first feature of interest from one or more characteristics of the received reflected ultrasonic waves prior to an intervention event;

extracting at least one second feature of interest from one or more characteristics of the received reflected ultrasonic waves subsequent to the intervention event;

determining at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.

60. The computer readable medium of claim 59, wherein the intervention event is the administering of at least one medicament.

61. A portable hemodynamic monitoring device comprising:

a housing configured for removable coupling to a body part of an individual, the body part including at least one vessel of interest;

an ultrasound unit coupled to the housing and adapted for adducing ultrasonic waves into the at least one vessel of interest in accordance to a programmed pulse repetition frequency, the ultrasound unit including:

at least one transducer pair adapted, in accordance with the programmed pulsed wave frequency, to produce the ultrasonic waves, and to detect reflected ultrasonic waves derived at least in part from the produced ultrasonic waves directed at the at least one vessel of interest and oriented such that, in concert, the at least one transducer pair produces the ultrasonic waves at an angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest;

a processor configured to produce at least one ultrasound image of the at least one vessel of interest, and in accordance with the programmed pulsed wave frequency, extract hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves in real-time or near real-time by applying a signal processing routine, and to store the extracted one or more hemodynamic parameters in a storage; and

a sensory output device adapted to provide feedback on a quality of the extracted hemodynamic parameters, the sensory output device including at least one of (i) a graphical display and (ii) an auditory display;

wherein the orientation of the at least one transducer pair improves a probability of proper acoustic coupling between the ultrasound unit and the body part of the individual by enabling a plurality of redundant effective placement options of the housing on the body part of the individual, the plurality of redundant effective placement options.

62. The portable hemodynamic monitoring device of claim 61, wherein the signal processing routine includes processing the detected reflected ultrasonic waves according to a pulsed wave Doppler ultrasound process.
63. The portable hemodynamic monitoring device of claim 61, wherein the at least one transducer pair comprises a chain of transducer pairs.

64. The portable hemodynamic monitoring device of claim 61, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.
65. The portable hemodynamic monitoring device of claim 61, wherein the at least one transducer pair is oriented in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.
66. The portable hemodynamic monitoring device of claim 61, wherein the housing includes a tension bandage that is utilized to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient downward force is applied to the ultrasound unit.
67. The portable hemodynamic monitoring device of claim 66, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
68. The portable hemodynamic monitoring device of claim 61, wherein the sensory output device is configured to generate a sensory output indicating an effectiveness of placement of the ultrasound unit.
69. The portable hemodynamic monitoring device of claim 61, wherein the processor is further configured to detect an estimated return of spontaneous circulation (ROSC) event by measuring a difference between a first relative blood flow from a chest compression and a second relative blood flow from a heartbeat, and the sensory output device is configured to generate a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event and indicating that any chest compression activities should cease.

70. The portable hemodynamic monitoring device of claim 61, wherein the housing includes at least one data communication device operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over a data network.
71. The portable hemodynamic monitoring device of claim 70, wherein the data communication device transmits the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data network to an external computer system.
72. The portable hemodynamic monitoring device of claim 61, wherein the housing includes at least one data transfer bus operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over a data connection.
73. The portable hemodynamic monitoring device of claim 72, wherein the data transfer bus is operable to transmit the extracted hemodynamic parameters from one or more characteristics of the detected reflected ultrasonic waves over the data connection to one or more external connected devices.
74. The portable hemodynamic monitoring device of claim 61, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.
75. The portable hemodynamic monitoring device of claim 61, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.
76. The portable hemodynamic monitoring device of claim 61, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.

77. The portable hemodynamic monitoring device of claim 61, wherein the processor is configured to determine whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.
78. The portable hemodynamic monitoring device of claim 77, wherein the sensory output device is configured to transmit a signal when the processor determines that the individual is undergoing compensated shock.
79. The portable hemodynamic monitoring device of claim 61, wherein the processor is further configured to:
- extract at least one first feature of interest from one or more characteristics of the detected reflected ultrasonic waves prior to an intervention event;
 - extract at least one second feature of interest from one or more characteristics of the detected reflected ultrasonic waves subsequent to the intervention event;
 - determine at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.
80. The portable hemodynamic monitoring device of claim 79, wherein the intervention event is the administering of at least one medicament.
81. A method for hemodynamic monitoring, the method comprising:
- removably coupling an ultrasound unit to a body part of an individual, the body part including at least one vessel of interest, the ultrasound

unit including at least one transducer pair forming a transducer array operable to emit and receive ultrasonic waves;

producing, by the transducer array, the ultrasonic waves at an angle of incidence between about 25 degrees and about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest by orienting the ultrasound unit such that the at least one transducer pair is situated in a particular fashion;

adducing the ultrasonic waves into the at least one vessel of interest and receiving reflected ultrasonic waves in accordance with a programmed pulsed wave frequency;

producing, by analysing the received reflected ultrasonic waves at least one ultrasound image of the at least one vessel of interest;

determining whether the reflected ultrasonic waves are derived at least in part from the adduced ultrasonic waves directed at the at least one vessel of interest;

extracting a plurality of hemodynamic parameters from one or more characteristics of the reflected ultrasonic waves determined to have been derived at least in part from the adduced ultrasonic waves by executing a signal processing routine; and

providing feedback on the extracted plurality of hemodynamic parameters via at least one sensory output device, the at least one sensory output device including at least one of: (i) a graphical display; and (ii) an auditory display.

82. The method for hemodynamic monitoring of claim 81, wherein the signal processing routine includes a pulsed wave Doppler ultrasound process capable of measurement of high velocity fluid flow through the at least one vessel of interest.

83. The method for hemodynamic monitoring of claim 81, wherein the at least one transducer pair is a chain of transducer pairs.
84. The method for hemodynamic monitoring of claim 81, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.
85. The method for hemodynamic monitoring of claim 81, wherein the at least one transducer pair is oriented in a in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.
86. The method for hemodynamic monitoring of claim 81, wherein the housing includes a tension bandage operable to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient force is applied to maintain the removable coupling.
87. The method for hemodynamic monitoring of claim 86, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
88. The method for hemodynamic monitoring of claim 81, further comprising generating a sensory output indicating an effectiveness of placement of the ultrasound unit.
89. The method for hemodynamic monitoring of claim 81, further comprising detecting an estimated return of spontaneous circulation (ROSC) event by: measuring a difference between a first relative blood flow from a chest compression and a second relative blood flow from a heartbeat; generating a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event; and, indicating, by the sensory output, that any chest compression activities should cease.

90. The method for hemodynamic monitoring of claim 81, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the reflected ultrasonic waves over a data network.
91. The method for hemodynamic monitoring of claim 90, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data network to an external computer system.
92. The method for hemodynamic monitoring of claim 81, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data connection.
93. The method for hemodynamic monitoring of claim 92, further comprising transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data connection to one or more external connected devices.
94. The method for hemodynamic monitoring of claim 81, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.
95. The method for hemodynamic monitoring of claim 81, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.
96. The method for hemodynamic monitoring of claim 81, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.
97. The method for hemodynamic monitoring of claim 81, further comprising determining whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral

of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.

98. The method for hemodynamic monitoring of claim 97, wherein the sensory output device is configured to transmit a signal when the individual is determined to be undergoing compensated shock.

99. The method for hemodynamic monitoring of claim 81, further comprising:

extracting at least one first feature of interest from one or more characteristics of the received reflected ultrasonic waves prior to an intervention event;

extracting at least one second feature of interest from one or more characteristics of the received reflected ultrasonic waves subsequent to the intervention event;

determining at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.

100. The method for hemodynamic monitoring of claim 99, wherein the intervention event is the administering of at least one medicament.

101. A computer readable medium having machine readable instructions stored thereon for hemodynamic monitoring of at least one vessel of interest in a body part of an individual, the machine readable instructions, when executed by a processor, performing a method comprising:

emitting and receiving ultrasonic waves through at least one transducer pair forming a transducer array, the transducer array forming part of an ultrasound unit which is removably coupled the body part of the individual;

producing, by the transducer array, the ultrasonic waves at an angle of incidence between about 25 degrees and about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest;

adducing the ultrasonic waves into the at least one vessel of interest and receiving reflected ultrasonic waves in accordance with a programmed pulsed wave frequency;

producing, by analysing the received reflected ultrasonic waves at least one ultrasound image of the at least one vessel of interest;

determining whether the reflected ultrasonic waves are derived at least in part from the adduced ultrasonic waves;

extracting a plurality of hemodynamic parameters from one or more characteristics of the reflected ultrasonic waves determined to have been derived at least in part from the adduced ultrasonic waves by executing a signal processing routine; and

transmitting feedback on the extracted plurality of hemodynamic parameters to at least one sensory output device, the at least one sensory output device including at least one of: (i) a graphical display; and (ii) an auditory display.

102. The computer readable medium of claim 101, wherein the signal processing routine includes a pulsed wave Doppler ultrasound process capable of measurement of fluid flow through the at least one vessel of interest.

103. The computer readable medium of claim 101, wherein the at least one transducer pair is a chain of transducer pairs.

104. The computer readable medium of claim 101, wherein the at least one transducer pair is at least one flexible polymer based transducer pair.

105. The computer readable medium of claim 101, wherein the at least one transducer pair is oriented in a in a saw tooth pattern, the saw tooth pattern causing the ultrasonic waves to be produced at the angle of incidence between about 25 degrees to about 60 degrees in respect of a plane of fluid flow through the at least one vessel of interest.
106. The computer readable medium of claim 101, wherein the ultrasound unit is coupled to a housing, the housing including a tension bandage operable to provide the removable coupling between the housing and the body part of the individual, the tension bandage being tensioned such that a sufficient force is applied to maintain the removable coupling.
107. The computer readable medium of claim 106, wherein the tension bandage is configured to maintain a substantially constant angle of incidence of the adduced ultrasonic waves relative to the at least one vessel of interest in order to enhance consistency of repeat measurements over a duration of time.
108. The computer readable medium of claim 101, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform generating a sensory output indicating an effectiveness of placement of the ultrasound unit.
109. The computer readable medium of claim 101, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform detecting an estimated return of spontaneous circulation (ROSC) event by: measuring a difference between a first relative blood flow from a chest compression and a second relative blood flow from a heartbeat; generating a sensory output indicating the occurrence of the detected estimated return of spontaneous circulation (ROSC) event; and, indicating, by the sensory output, that any chest compression activities should cease.
110. The computer readable medium of claim 101, wherein the machine readable instructions, when executed by the processor, further cause the

processor to perform transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data network.

111. The computer readable medium of claim 110, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data network to an external computer system.

112. The computer readable medium of claim 101, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over a data connection.

113. The computer readable medium of claim 112, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform transmitting the extracted hemodynamic parameters from one or more characteristics of the received reflected ultrasonic waves over the data connection to one or more external connected devices.

114. The computer readable medium of claim 101, wherein the hemodynamic parameters include at least one of: a peak velocity of a Doppler shift detected in the at least one vessel of interest; a velocity-time integral of signal changes between heartbeats; and a ratio measured between a post-intervention velocity-time integral and a pre-intervention velocity-time integral.

115. The computer readable medium of claim 101, wherein the frequency of the ultrasonic waves is a frequency between about 3 MHz to about 12 MHz.

116. The computer readable medium of claim 101, wherein the frequency of the ultrasonic waves is a frequency is about 5 MHz.

117. The computer readable medium of claim 101, wherein the machine readable instructions, when executed by the processor, further cause the processor to perform determining whether the individual is undergoing compensated shock by: continuously monitoring a ratio between a heart rate and a velocity-time integral of fluid flow through the at least one vessel of interest; entering a compensated shock alarm state when the ratio exceeds a pre-defined threshold; and producing an alarm signal when the compensated shock alarm state is entered.
118. The computer readable medium of claim 117, wherein the sensory output device is configured to transmit a signal when the individual is determined to be undergoing compensated shock.
119. The computer readable medium of claim 101, further comprising:
- extracting at least one first feature of interest from one or more characteristics of the received reflected ultrasonic waves prior to an intervention event;
 - extracting at least one second feature of interest from one or more characteristics of the received reflected ultrasonic waves subsequent to the intervention event;
 - determining at least one post-intervention change value equivalent to the difference between the at least one first feature of interest and the at least one second feature of interest.
120. The computer readable medium of claim 119, wherein the intervention event is the administering of at least one medicament.

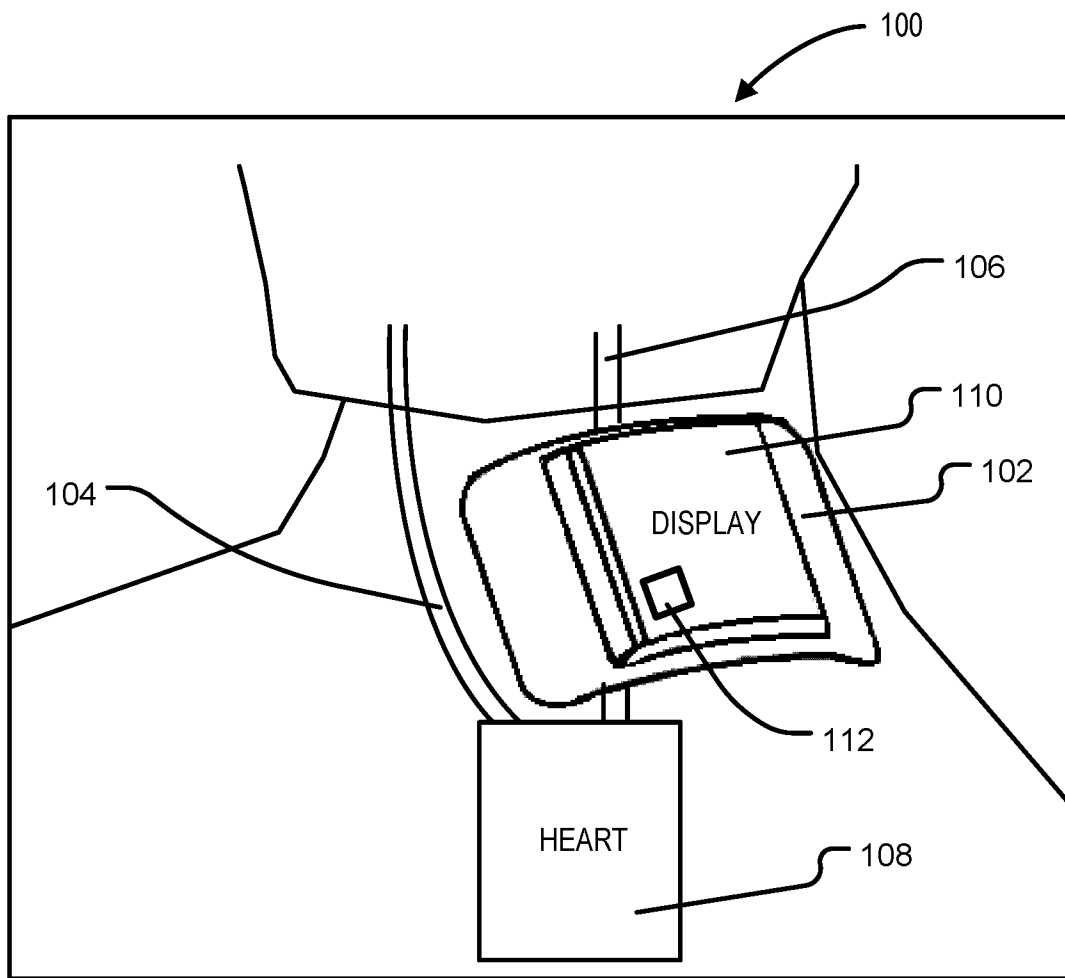


FIG. 1

2/19

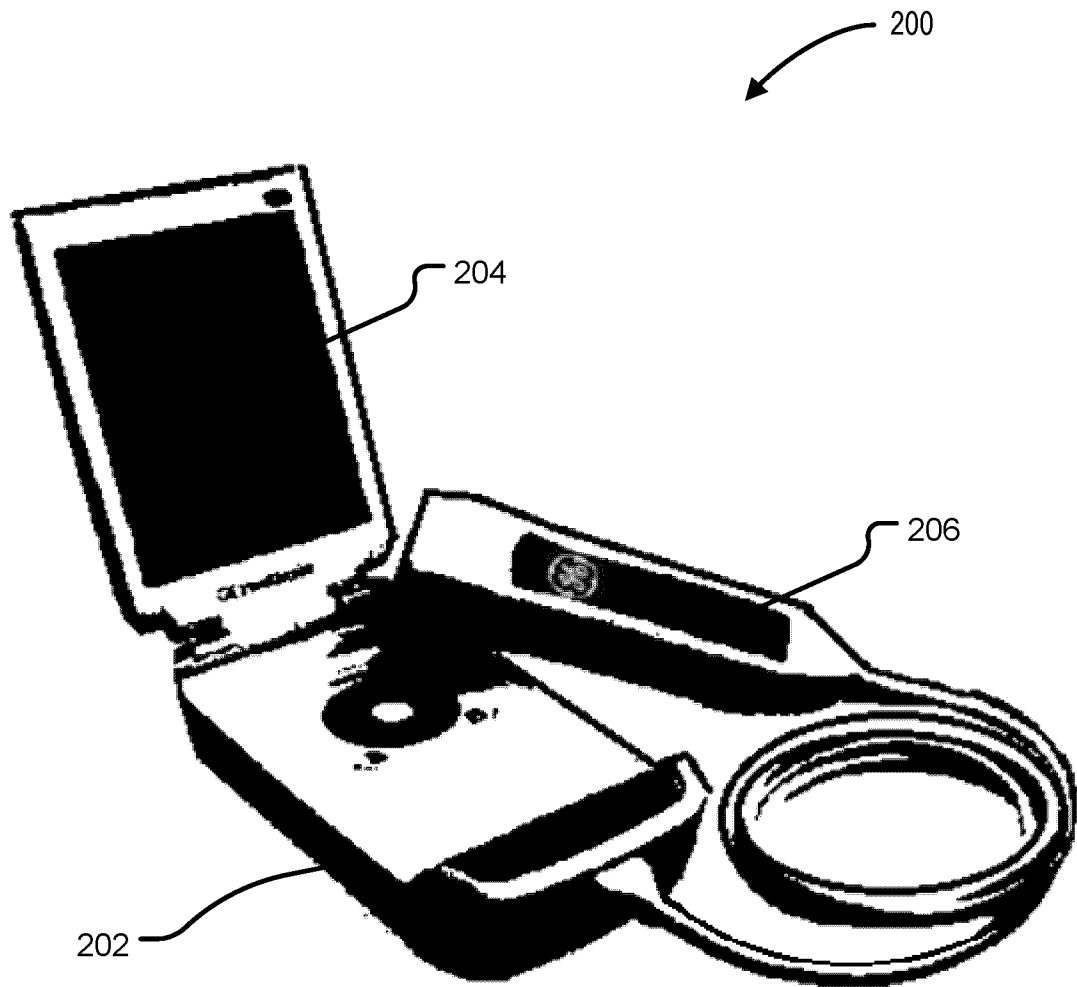


FIG. 2

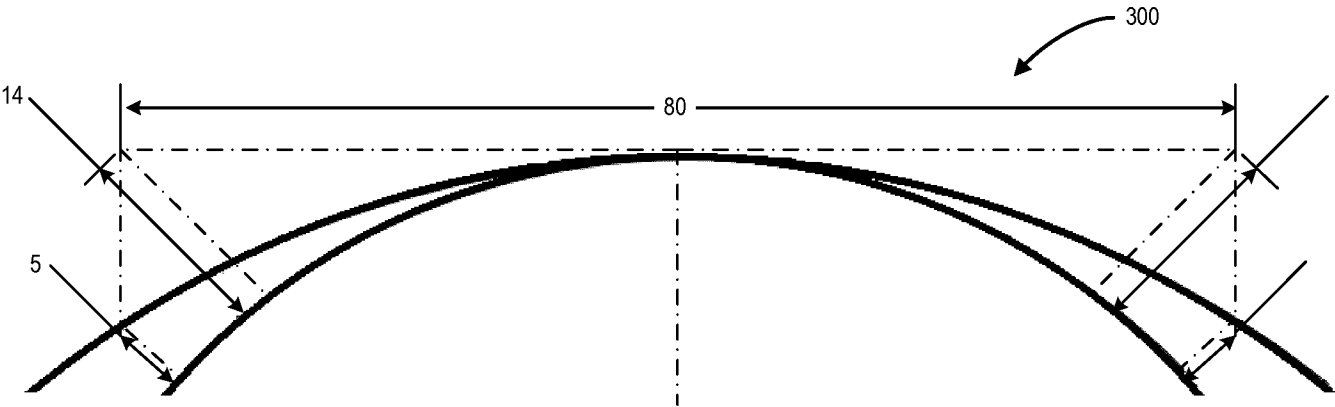


FIG. 3

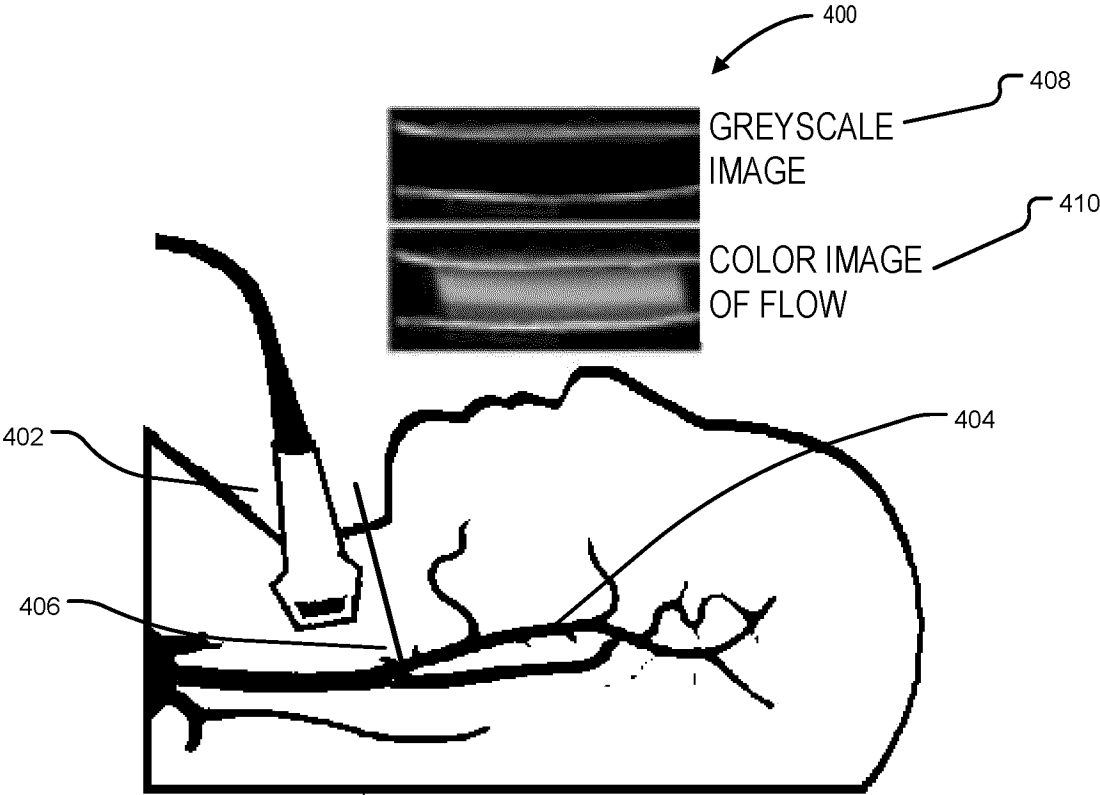


FIG. 4

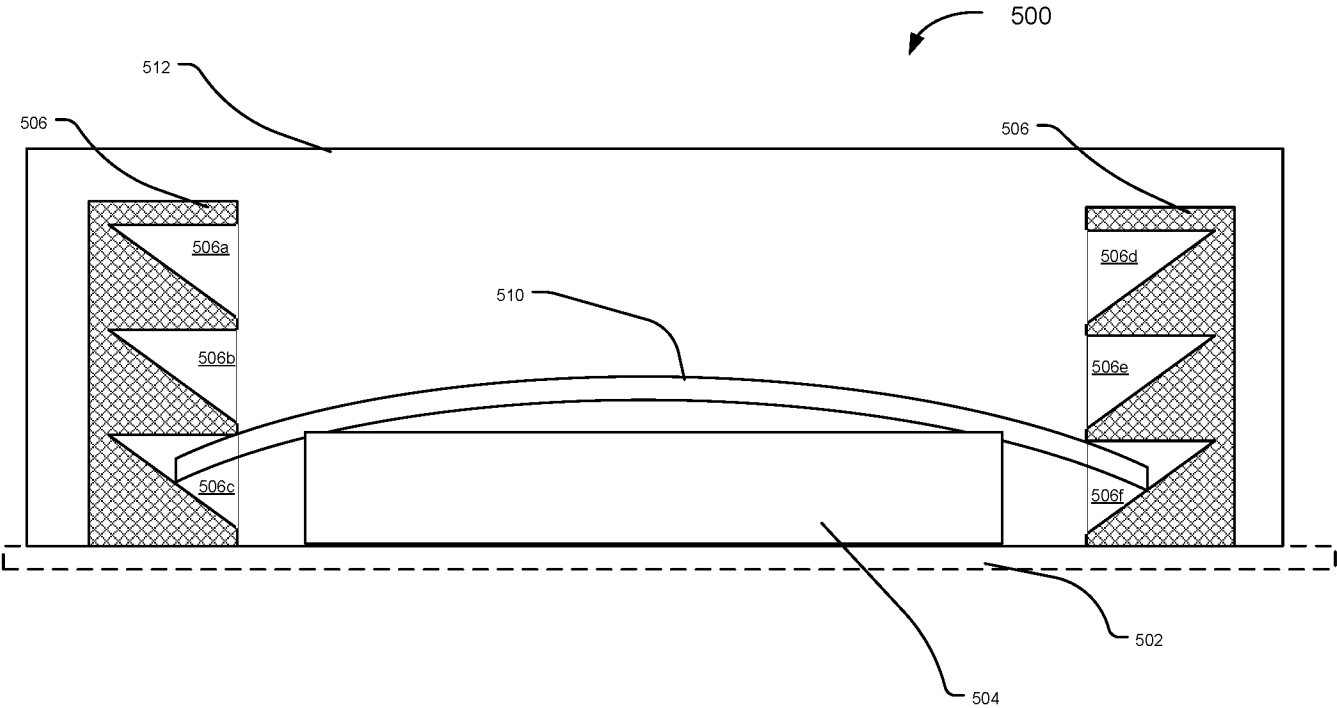


FIG. 5

6/19

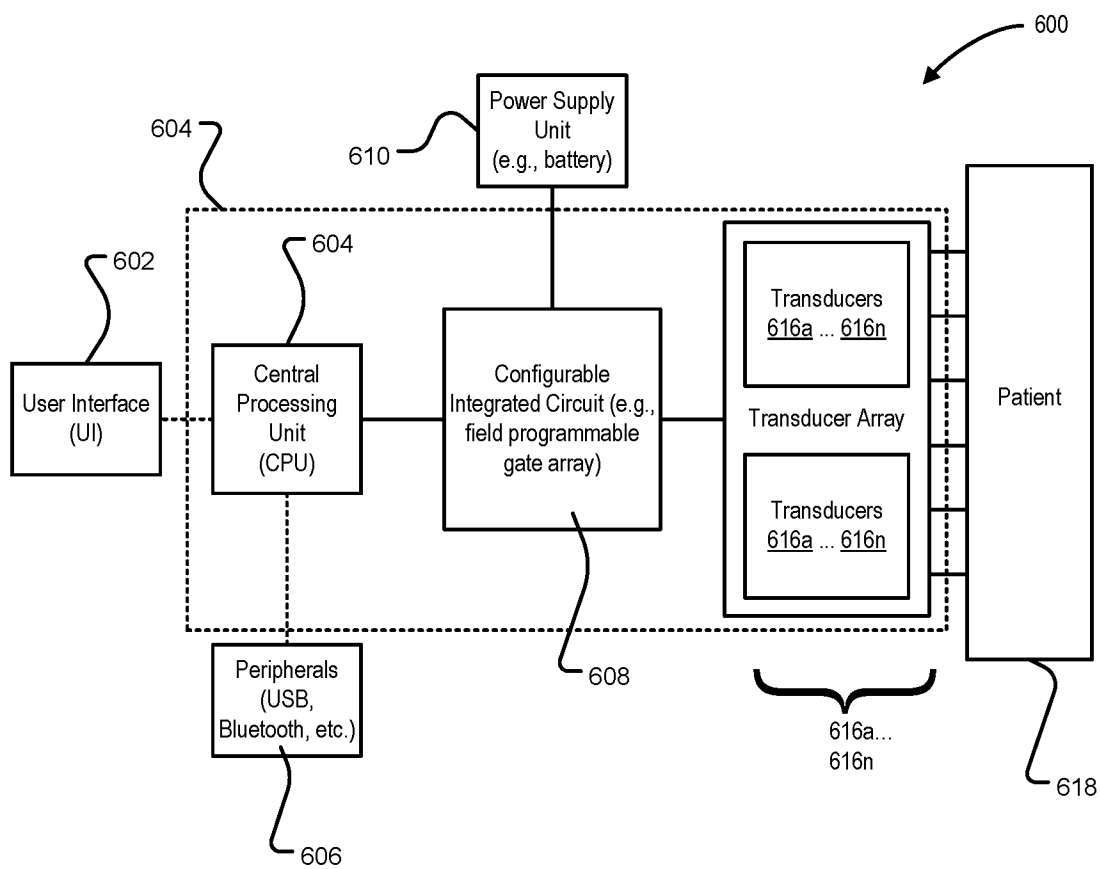


FIG. 6

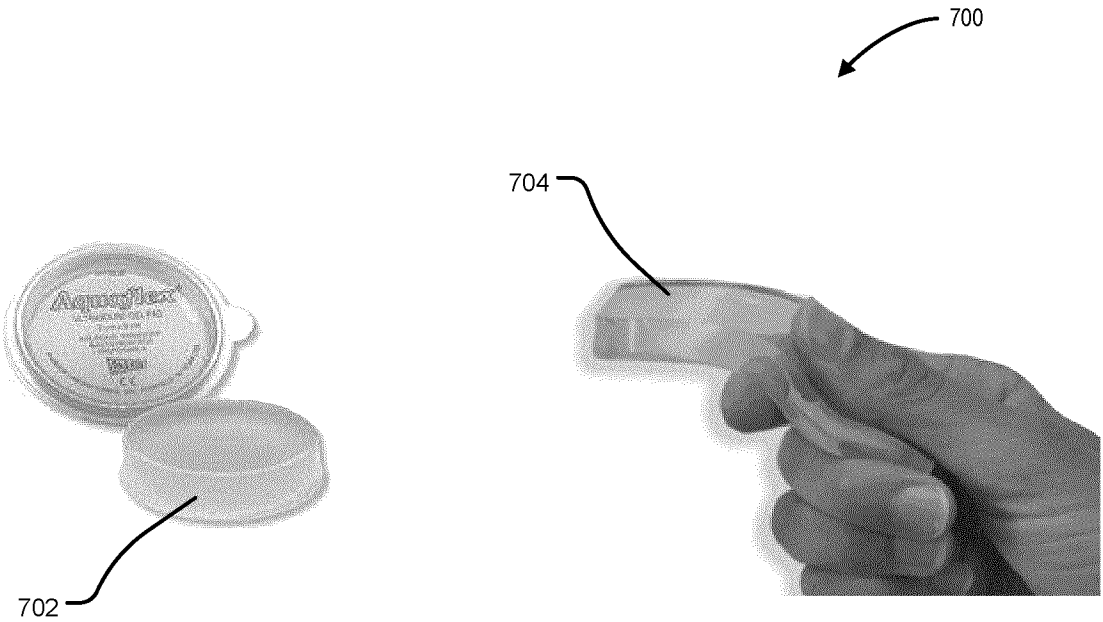


FIG. 7A

FIG. 7B

8/19

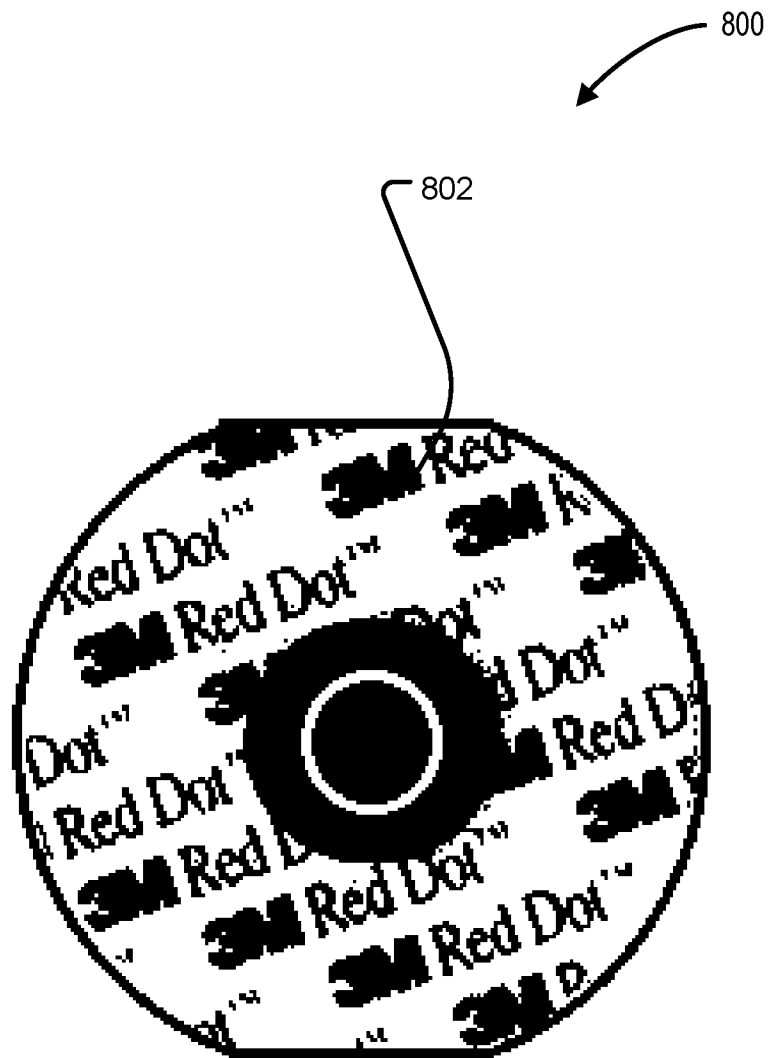


FIG. 8

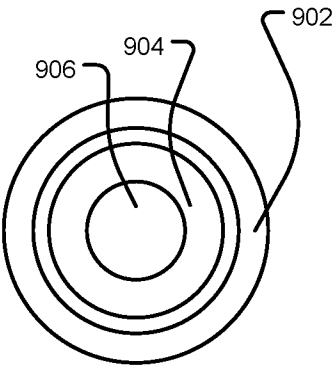


FIG. 9A

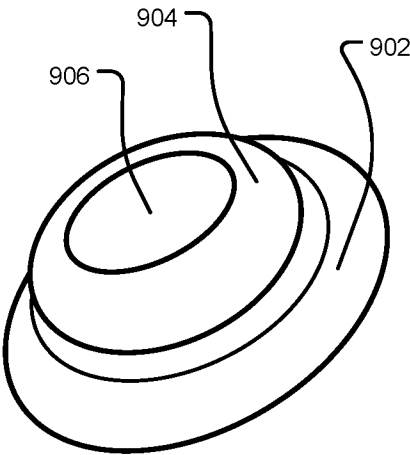


FIG. 9B

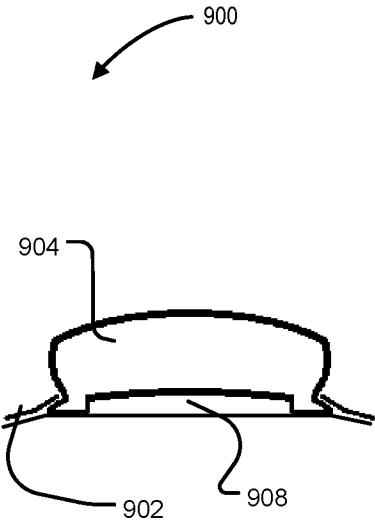


FIG. 9C

10/19

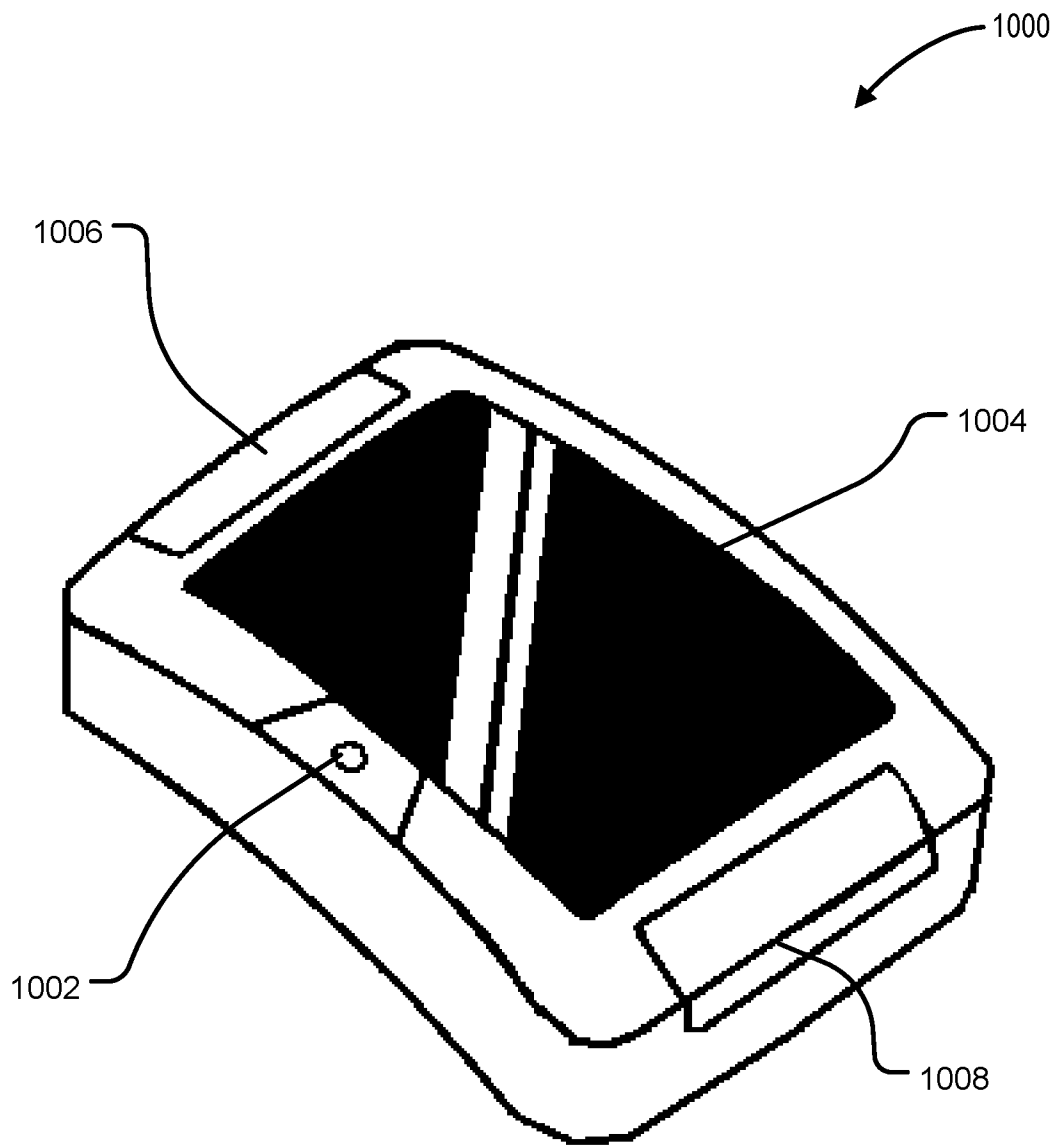


FIG. 10

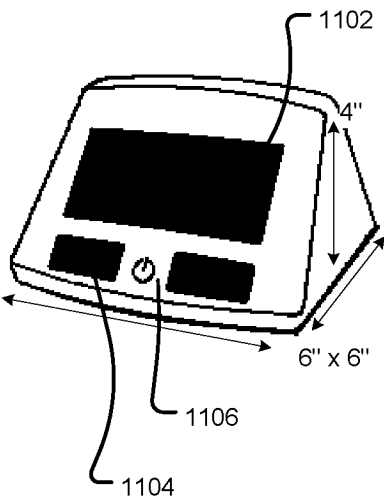


FIG. 11A

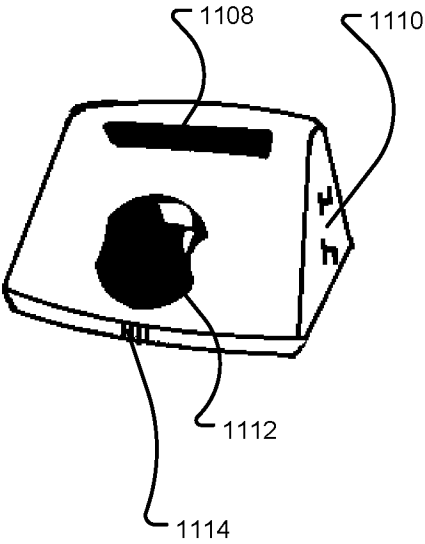


FIG. 11B

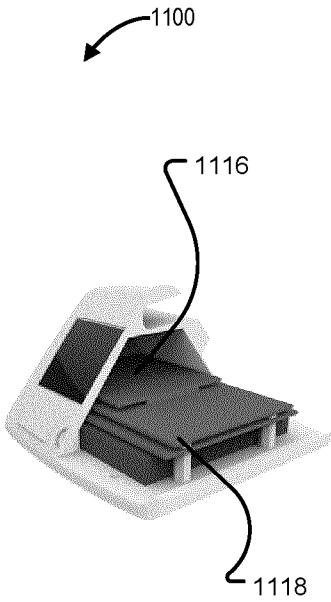


FIG. 11C

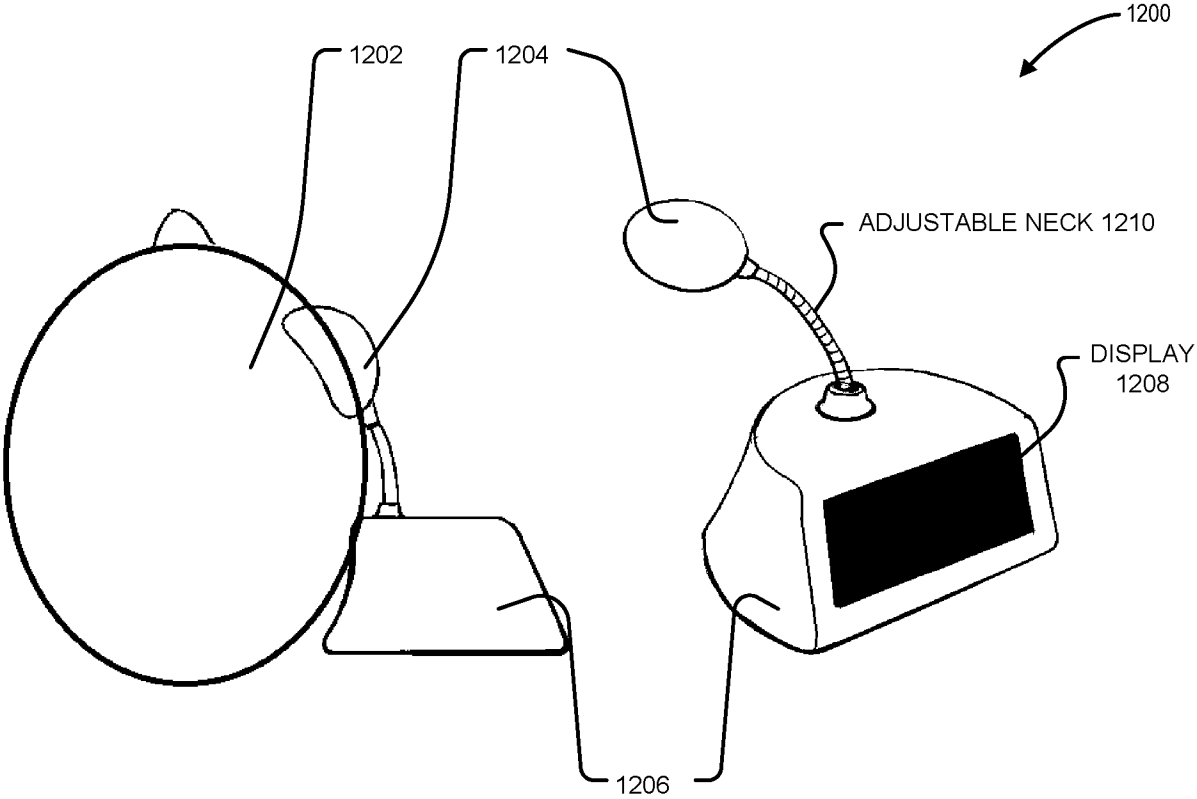


FIG. 12A

FIG. 12B

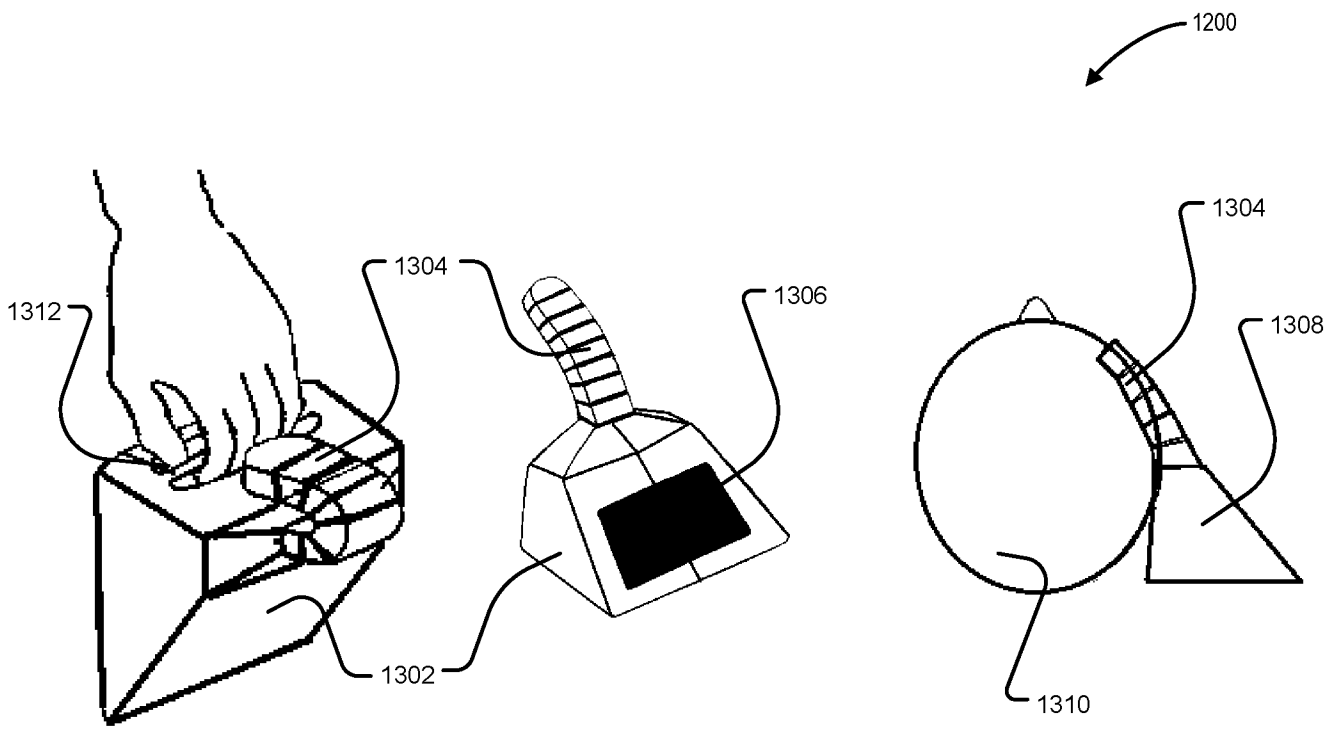


FIG. 13A

FIG. 13B

FIG. 13C

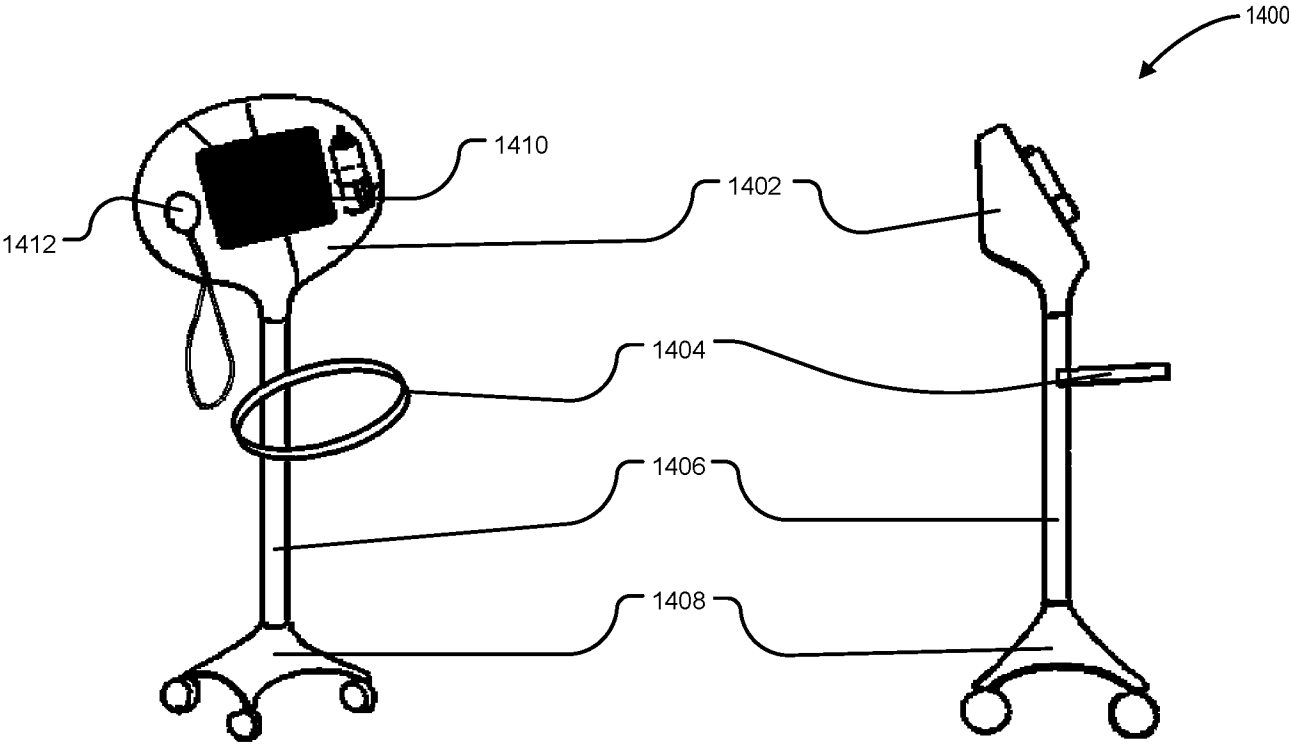


FIG. 14A

FIG. 14B

15/19

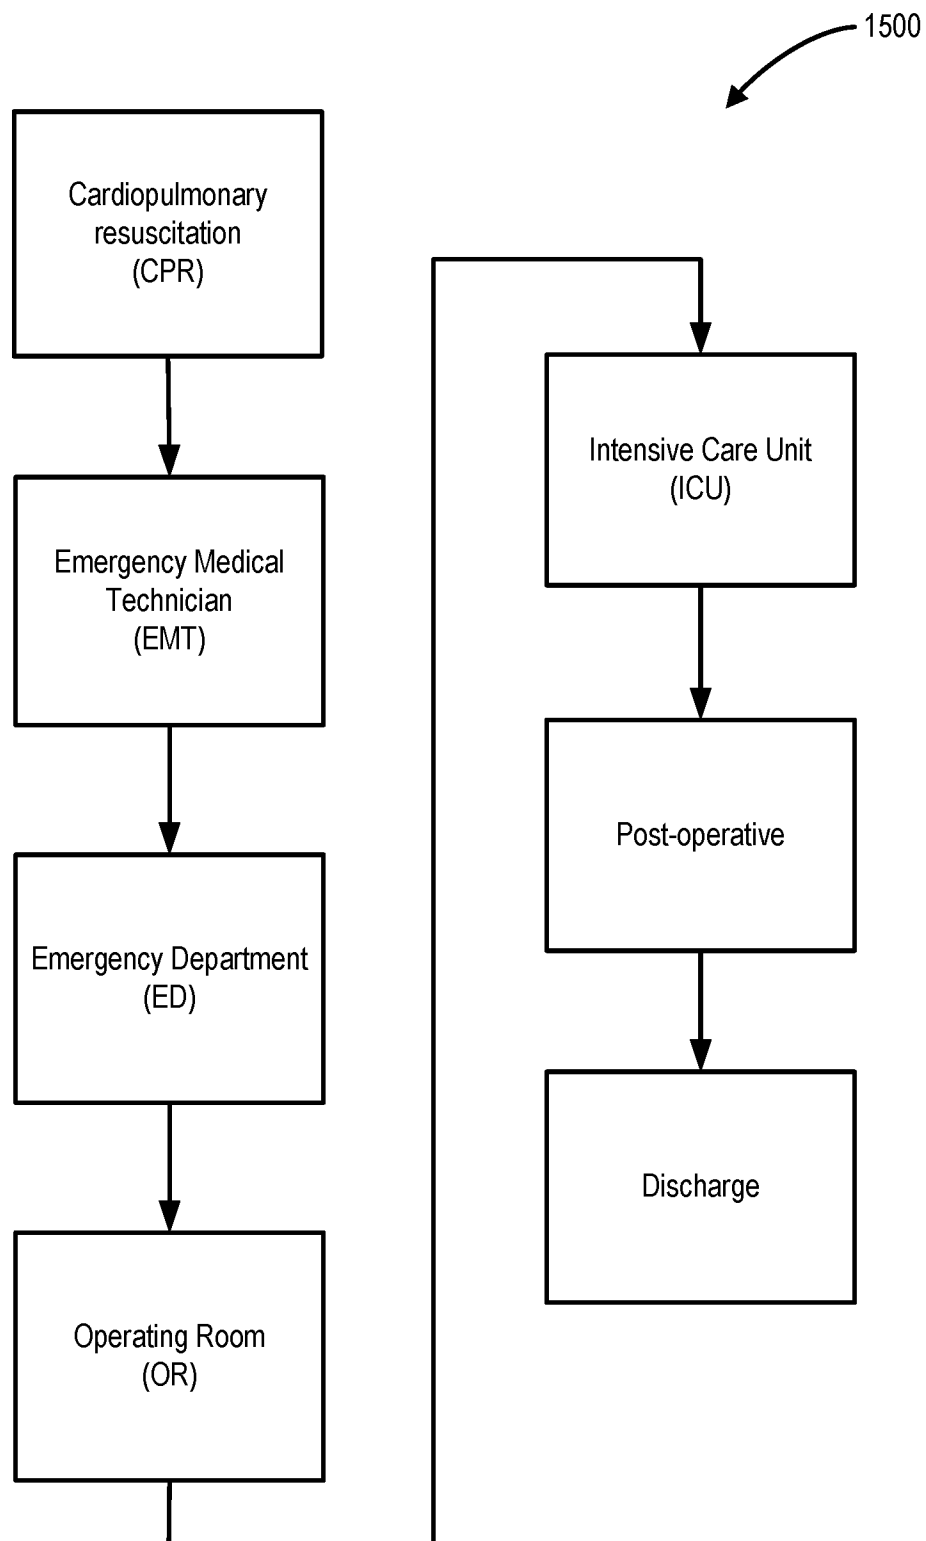


FIG. 15

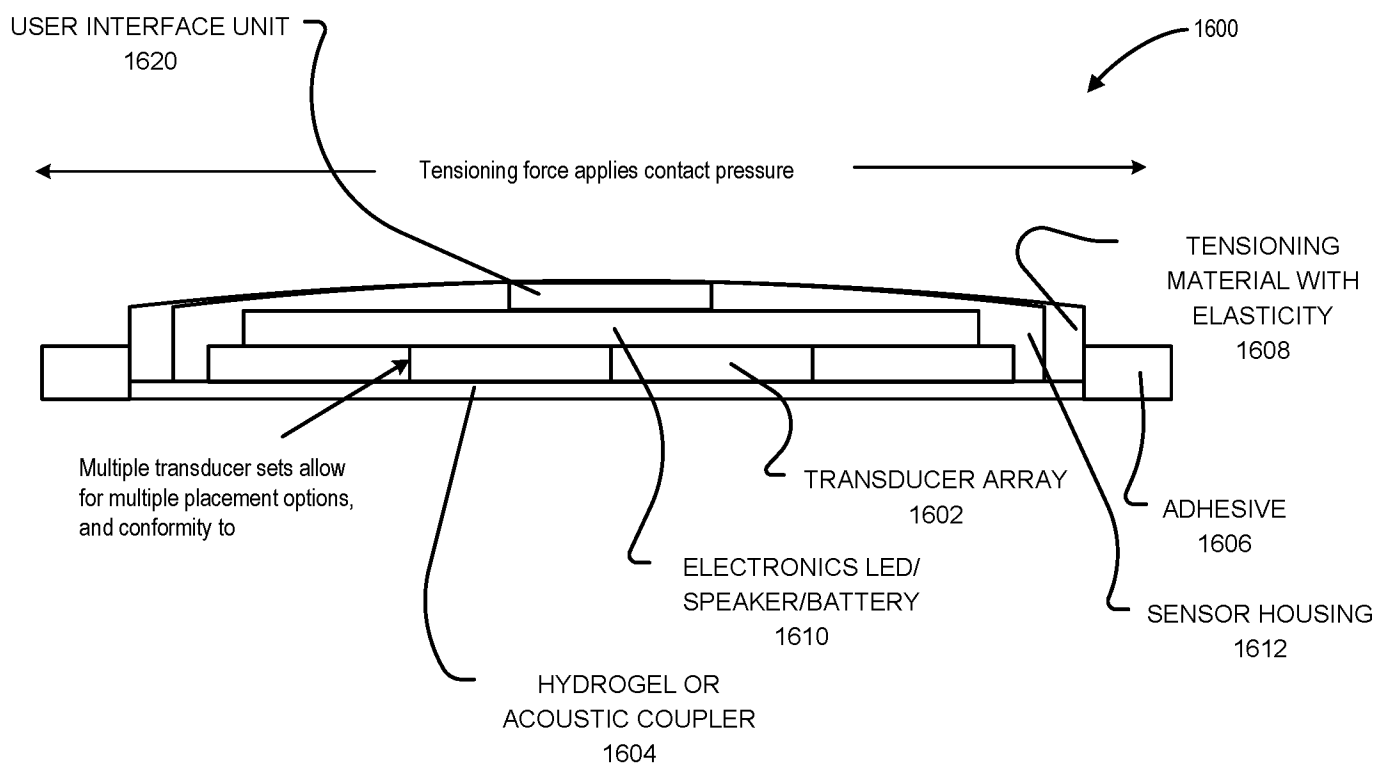


FIG. 16

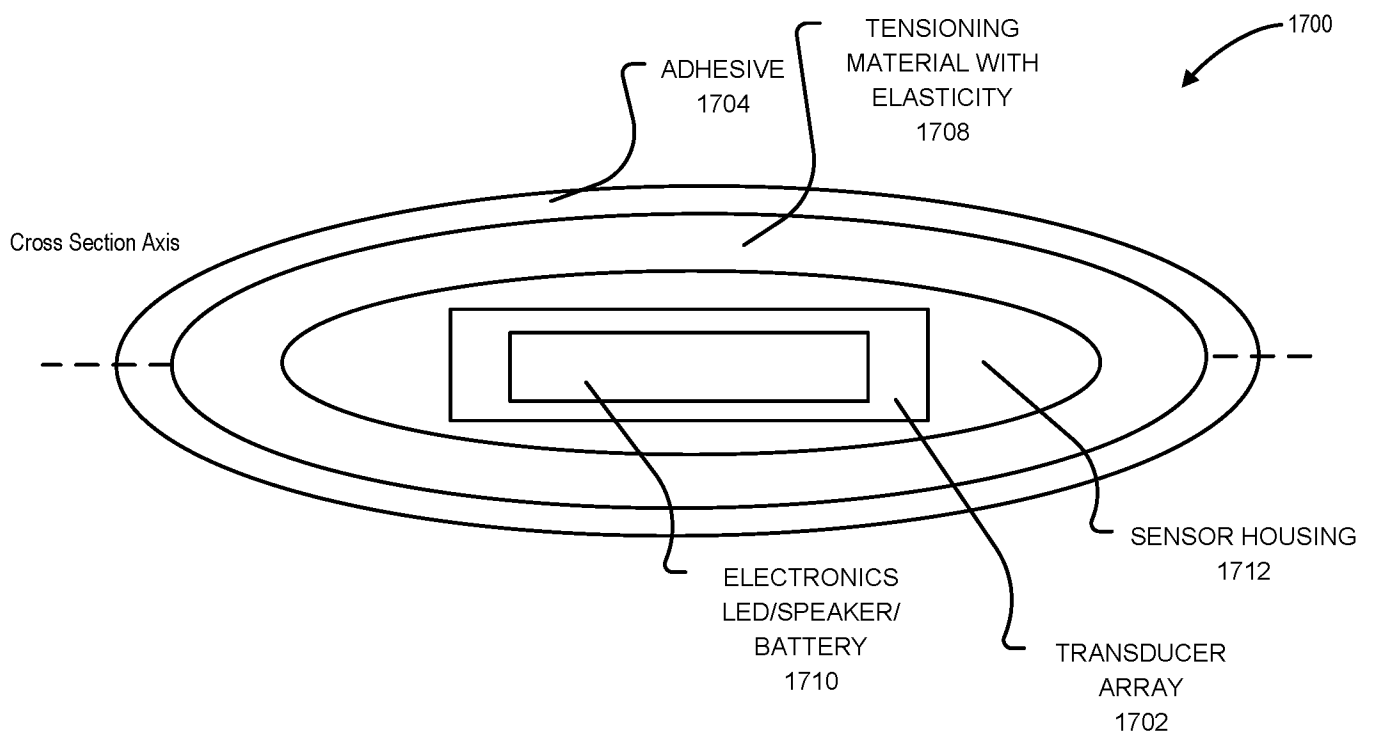


FIG. 17

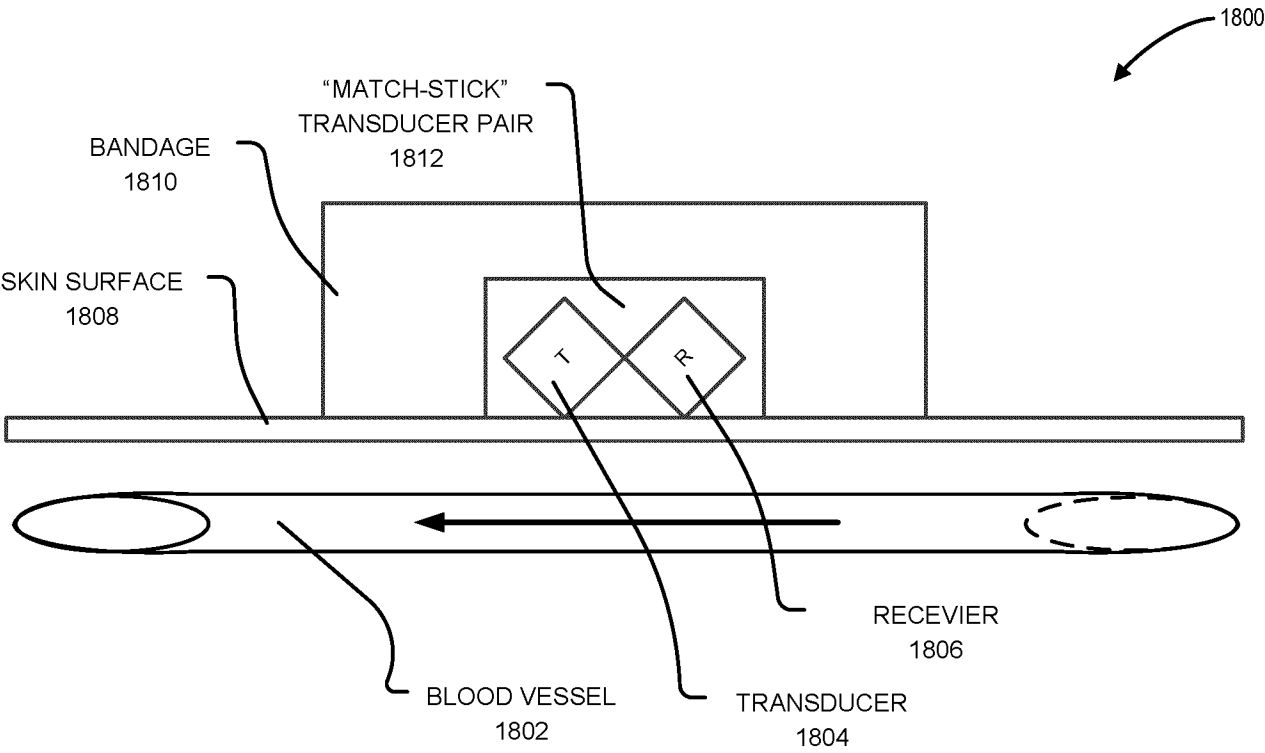


FIG. 18

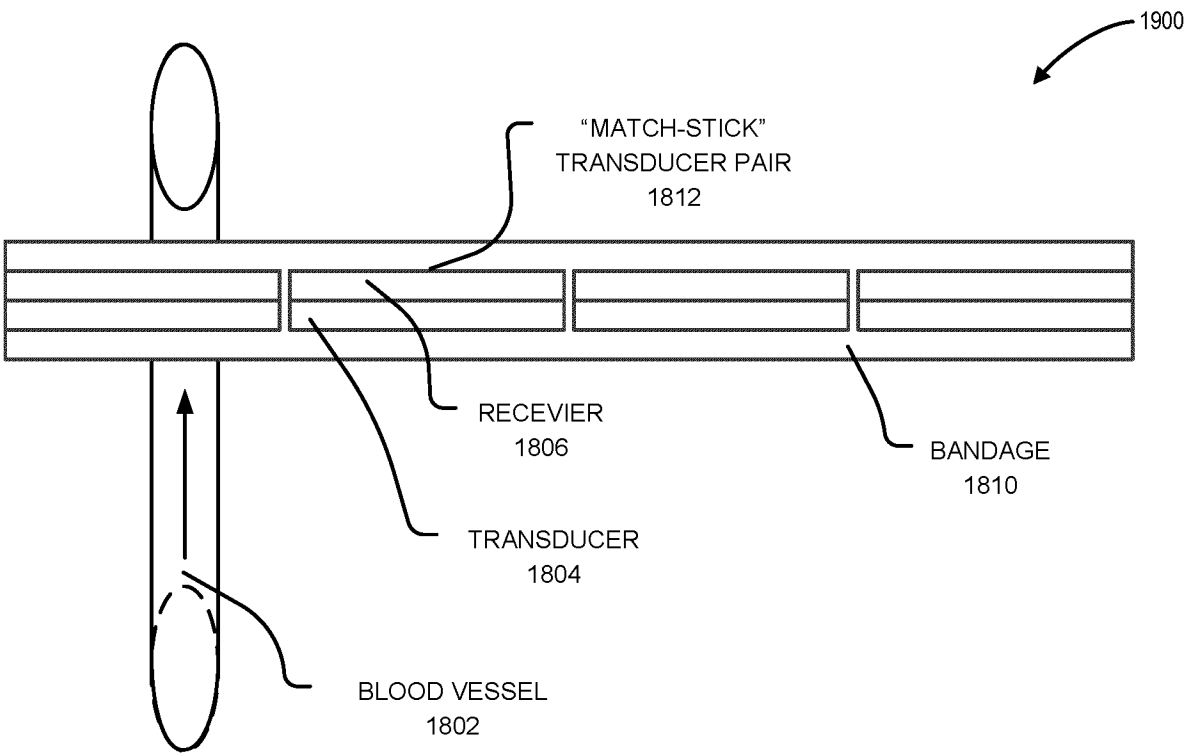


FIG. 19

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/051451

A. CLASSIFICATION OF SUBJECT MATTER

IPC: **A61B 8/13** (2006.01), **A61B 5/026** (2006.01), **A61B 8/14** (2006.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
 IPC (2006): A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used)

Database: Canadian Patent Database (Intellect), Questel Orbit, USPTO West, IEEE Xplore

Keywords: ultrasound, image, hemodynamic, carotid, vessel, parameter, Doppler, transducer, pair, couple, bandage, spontaneous, circulation, saw tooth, angle

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2002/0042574 (MANOR et al.) 11 April 2002 (11-04-2002) * Paragraphs [0004], [0009]-[0012], [0016], [0017], [0027], [0037], [0038], [0044]-[0047], [0052], [0075] and [0168] *	1-120
Y	US 2015/0289838 (NICHOL et al.) 15 October 2015 (15-10-2015) * Paragraphs [0011], [0015], [0021]-[0024], [0026]-[0028], [0032], [0037], [0038] and [0064] *	1-120
Y	US 2015/0009782 (ENGL et al.) 8 January 2015 (08-01-2015) * Paragraph [0037] *	5, 25, 45, 65, 85 and 105
Y	US 2012/0277640 (LEWIS, JR. et al.) 1 November 2012 (01-11-2012) * Paragraph [0057] *	6, 7, 26, 27, 46, 47, 66, 67, 86, 87, 106 and 107
Y	WO 2015/181167A1 (FROST) 3 December 2015 (03-12-2015) * Page 11, lines 3-5; page 26, lines 4 and 5 *	9, 29, 49, 69, 89 and 109

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier application or patent but published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search
 17 February 2017 (17-02-2017)

Date of mailing of the international search report
 14 March 2017 (14-03-2017)

Name and mailing address of the ISA/CA
 Canadian Intellectual Property Office
 Place du Portage I, C114 - 1st Floor, Box PCT
 50 Victoria Street
 Gatineau, Quebec K1A 0C9
 Facsimile No.: 819-953-2476

Authorized officer

Alan Chan (819) 639-2473

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/051451

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2010/0049052 (SHARF et al.) 25 February 2010 (25-02-2010) * Paragraphs [0018], [0019], [0046], [0144], [0163], [0180], [0222] and [0244] *	14-18, 34-38, 54-58, 74-78, 94-98 and 114-118
A	US 4103679 (ARONSON) 1 August 1978 (01-08-1978)	1-120
A	US 2014/0371594 (FLYNN et al.) 18 December 2014 (18-12-2014)	1-120
A	US 2014/0081144 (MOEHRING et al.) 20 March 2014 (20-03-2014)	1-120
A	US 2006/0206032 (MIELE et al.) 14 September 2006 (14-09-2006)	1-120

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.

PCT/CA2016/051451

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
US2002042574A1	11 April 2002 (11-04-2002)	US2002042574A1 US6503205B2 AU1176300A EP1131002A1 IL127112D0 WO0028899A1	11 April 2002 (11-04-2002) 07 January 2003 (07-01-2003) 05 June 2000 (05-06-2000) 12 September 2001 (12-09-2001) 22 September 1999 (22-09-1999) 25 May 2000 (25-05-2000)
US2015289838A1	15 October 2015 (15-10-2015)	US2015289838A1 WO2014066859A1	15 October 2015 (15-10-2015) 01 May 2014 (01-05-2014)
US2015009782A1	08 January 2015 (08-01-2015)	US2015009782A1 CA2865054A1 DE202012104119U1 EP2828009A1 WO2013139872A1	08 January 2015 (08-01-2015) 26 September 2013 (26-09-2013) 30 April 2013 (30-04-2013) 28 January 2015 (28-01-2015) 26 September 2013 (26-09-2013)
US2012277640A1	01 November 2012 (01-11-2012)	US2012277640A1 US9480863B2 BR112012016312A2 BR112012016316A2 BR112012016325A2 CN102869409A CN102907117A CN102907117B CN103096976A CN103096976B EP2519322A2 EP2519323A2 EP2520101A2 IN6597DEN2012A IN6598DEN2012A IN6605DEN2012A US2012283605A1 US9199096B2 US2013006153A1 US9492687B2 WO2011082402A2 WO2011082402A3 WO2011082407A2 WO2011082407A3 WO2011082408A2 WO2011082408A3	01 November 2012 (01-11-2012) 01 November 2016 (01-11-2016) 23 August 2016 (23-08-2016) 23 August 2016 (23-08-2016) 23 August 2016 (23-08-2016) 09 January 2013 (09-01-2013) 30 January 2013 (30-01-2013) 23 September 2015 (23-09-2015) 08 May 2013 (08-05-2013) 27 April 2016 (27-04-2016) 07 November 2012 (07-11-2012) 07 November 2012 (07-11-2012) 07 November 2012 (07-11-2012) 23 October 2015 (23-10-2015) 23 October 2015 (23-10-2015) 23 October 2015 (23-10-2015) 08 November 2012 (08-11-2012) 01 December 2015 (01-12-2015) 03 January 2013 (03-01-2013) 15 November 2016 (15-11-2016) 07 July 2011 (07-07-2011) 22 December 2011 (22-12-2011) 07 July 2011 (07-07-2011) 17 November 2011 (17-11-2011) 07 July 2011 (07-07-2011) 17 November 2011 (17-11-2011)
WO2015181167A1	03 December 2015 (03-12-2015)	WO2015181167A1 AU2015266063A1 CA2949880A1	03 December 2015 (03-12-2015) 12 January 2017 (12-01-2017) 03 December 2015 (03-12-2015)
US2010049052A1	25 February 2010 (25-02-2010)	US2010049052A1 AT515978T EP2079368A2 EP2079368B1 EP2386250A2 EP2386250A3 EP2386250B1 WO2008050334A2 WO2008050334A3	25 February 2010 (25-02-2010) 15 July 2011 (15-07-2011) 22 July 2009 (22-07-2009) 13 July 2011 (13-07-2011) 16 November 2011 (16-11-2011) 15 February 2012 (15-02-2012) 11 September 2013 (11-09-2013) 02 May 2008 (02-05-2008) 17 July 2008 (17-07-2008)
US4103679A	01 August 1978 (01-08-1978)	None	

Continued in Supplemental Box

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/051451

Continuation of patent family members

US2014371594A1	18 December 2014 (18-12-2014)	US2014371594A1	18 December 2014 (18-12-2014)
		US9192359B2	24 November 2015 (24-11-2015)
		CA2851641A1	25 April 2013 (25-04-2013)
		CN104011559A	27 August 2014 (27-08-2014)
		CN104011559B	24 August 2016 (24-08-2016)
		DK2769241T3	11 January 2016 (11-01-2016)
		DK2940487T3	21 November 2016 (21-11-2016)
		EP2769241A1	27 August 2014 (27-08-2014)
		EP2769241B1	23 September 2015 (23-09-2015)
		EP2940487A1	04 November 2015 (04-11-2015)
		EP2940487B1	20 July 2016 (20-07-2016)
		JP2014534852A	25 December 2014 (25-12-2014)
		JP6017576B2	02 November 2016 (02-11-2016)
		KR20140084213A	04 July 2014 (04-07-2014)
		WO2013059659A1	25 April 2013 (25-04-2013)
US2014081144A1	20 March 2014 (20-03-2014)	US2014081144A1	20 March 2014 (20-03-2014)
		EP1898795A2	19 March 2008 (19-03-2008)
		EP1898795A4	07 May 2014 (07-05-2014)
		TW200722055A	16 June 2007 (16-06-2007)
		US2007016050A1	18 January 2007 (18-01-2007)
		US8162837B2	24 April 2012 (24-04-2012)
		US2012226163A1	06 September 2012 (06-09-2012)
		WO2006138185A2	28 December 2006 (28-12-2006)
		WO2006138185A3	13 September 2007 (13-09-2007)
US2006206032A1	14 September 2006 (14-09-2006)	US2006206032A1	14 September 2006 (14-09-2006)
		US8328727B2	11 December 2012 (11-12-2012)
		AU4766501A	03 October 2001 (03-10-2001)
		AU2001247665B2	08 December 2005 (08-12-2005)
		AU2006200992A1	30 March 2006 (30-03-2006)
		AU2006200992B2	12 March 2009 (12-03-2009)
		CA2403728A1	27 September 2001 (27-09-2001)
		EP1324788A2	09 July 2003 (09-07-2003)
		JP2004521660A	22 July 2004 (22-07-2004)
		US6554774B1	29 April 2003 (29-04-2003)
		US2002062086A1	23 May 2002 (23-05-2002)
		US7048691B2	23 May 2006 (23-05-2006)
		US2005038346A1	17 February 2005 (17-02-2005)
		WO0170303A2	27 September 2001 (27-09-2001)
		WO0170303A8	21 March 2002 (21-03-2002)