

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
7 February 2008 (07.02.2008)

PCT

(10) International Publication Number
WO 2008/015666 A2

(51) International Patent Classification:
A61B 17/32 (2006.01)

(21) International Application Number:
PCT/IL2007/000943

(22) International Filing Date: 29 July 2007 (29.07.2007)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/834564 1 August 2006 (01.08.2006) US

(71) Applicants and

(72) Inventors: **SHOHAT, Shaul** [IL/IL]; 69 Hagiva St.,
73134 Kfar Haoranim (IL). **MACHLEV, Eli** [IL/IL];
P.O. Box 304, 42835 Shaar Efraim (IL). **SHABAT, Roni**
[IL/IL]; 19350 Kibbutz Izrael (IL).

(74) Agent: **KAFRI, Avia**; 22 Shderot Chen St., 64166 Tel-
Aviv (IL).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,

AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH,
CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG,
ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL,
IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK,
LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW,
MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL,
PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY,
TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, PL,
PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Declaration under Rule 4.17:

— of inventorship (Rule 4.17(iv))

Published:

— without international search report and to be republished
upon receipt of that report

(54) Title: SYSTEM AND METHOD FOR TELESURGERY

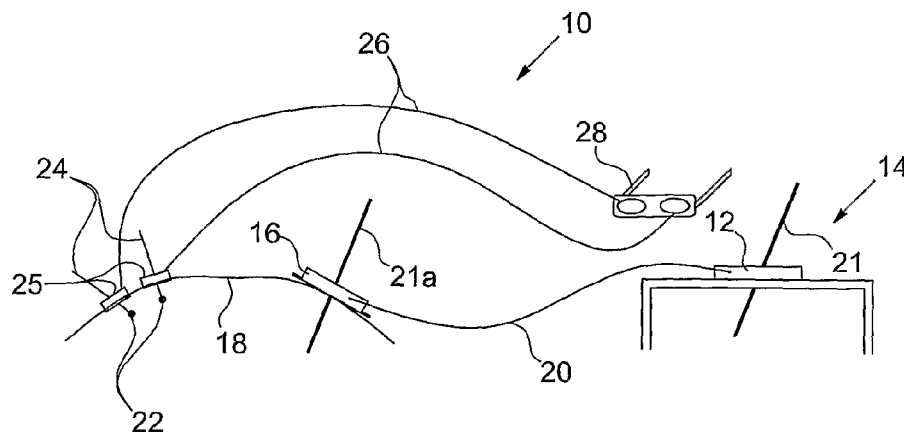

(57) Abstract: A system for telesurgery having a plurality of operative end units respectively linked to remote master end units. All the master and operative end units of the system consist of a common module having a base plate to which a slender shaft is slidingly attached. A slender shaft is further rotatable about its axis as well as about a center point disposed above the distal surface of the base plate. Surgical effectors, cameras and/or LEDs can be attached to the distal end of slender shafts of operative end units which is distally disposed relative to the base plate of its respective operative end unit. Operating handles for manipulating and/or activating the respective slender shaft or attached surgical effectors, are attached to the proximal end and/or to the distal end of slender shafts of master end units. Linking a master end unit to its respective operative end unit is accomplished by mechanical, hydraulic, pneumatic and or electric transmission, such that a slender shaft of an operative end units simultaneously move in the same movement in which the slender shaft of the respective master end unit is moved. An operator is able to manipulate a slender shaft within the lumen enclosing the surgical site within a patient's body by sliding, inclining and/or rotating the slender shaft of a remote master end unit as in a common endoscopic procedure. The operator is further able to manipulate and/or activate a surgical effector either as in an endoscopic or in an open surgery by means of the operating handles of a remote master end unit.



WO 2008/015666 A2

SYSTEM AND METHOD FOR TELESURGERY

FIELD OF THE INVENTION

5 The present invention relates in general to telesurgery and minimal
invasive surgical operations. More particularly the present invention relates to
surgical systems having a plurality of operative end units respectively coupled
to remote master units, surgical effectors, cameras and LEDs attached to
respective end units for in situ operating, illuminating, displaying and/or
10 imaging.

BACKGROUND OF THE INVENTION

Surgical procedures carried out at a distance thanks to advanced
robotic and computer technologies are known. Systems for telesurgery are
15 common in the marketplace. One of the early demonstrations of trans-Atlantic
telesurgery was reported in 2001 when surgeons in New York operated on a
patient in Strasbourg, France and used remote-controlled robots to resect the
gall bladder by laparoscopy.

Quite often endoscopic procedures impose on the physician tedious
20 postures that may cause tremor and reduce the accuracy and efficacy of the
procedure. Hence systems providing for telesurgery could be beneficial in this
respect. However common robotic systems for telesurgery require quite
sophisticated infrastructure and human resources that are normally hard to get.
Therefore any system for telesurgery that is simple to manufacture and to
25 operate is beneficial.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a simplified block diagram of a system for telesurgery of the invention;

Fig. 2A is a schematic presentation of a common module of a system for telesurgery of the invention;

Fig. 2B is a schematic presentation of an operative end unit of a system for telesurgery of the invention;

Fig. 2C is a fragmented isometric view of a segment of a common module of a system for telesurgery according to a preferred embodiment of the present invention;

Fig 3 is a scheme describing an exemplary mechanical linking of translational motion of the slender shafts of two coupled common modules of a system for telesurgery of the present invention;

Fig. 4A is an elevational view of a slender shaft having a surgical effector attached to its distal end in accordance with an embodiment of the present invention;

Fig. 4B is an elevational view of a slender shaft having a surgical effector attached to its distal end in accordance with a preferred embodiment of the present invention;

Figs 5A-5C are isometric and elevational views of an exemplary introducer of a system for telesurgery of the invention respectively;

Fig. 5D is an isometric view of the distal segment of an introducer of a system for telesurgery according to a preferred embodiment of the present invention;

Fig. 6A - 6B are two elevational views of a surgical effector attached to a mounting frame of a system for telesurgery in accordance with a preferred embodiment of the present invention;

Figs 7A – 7B are elevational views of linking accessories of a system for telesurgery in accordance with three different embodiments of the present invention respectively;

Figs 8A – 8B are schematic presentations of two slender shafts according to two different embodiments of the present invention respectively;

Fig. 9A is a schematic presentation of a remote viewing member of a viewing subsystem of a system for telesurgery in accordance with a preferred embodiment of the present invention attached to a patient's body;

5 Figs 9B -9C are schematic presentations of a control member of the viewing subsystem shown in Fig. 9A according to two preferred embodiments of the present invention;

Fig. 10 is a schematic presentation of a master unit of a system for telesurgery according to a preferred embodiment of the present invention;

DETAILED DESCRIPTION OF THE PRESENT INVENTION

In accordance with the present invention a system and method for telesurgery is provided. The system of the invention has one or more master end units respectively linked to operative end units. A system of the invention further has various accessories such as surgical effectors, introducers, viewing and/or imaging devices and linking devices as is further described infra. All of the end units, the master end units and the operative end units comprise a common module having a rotatable slender shaft slidingly attached to a base plate. Handles and/or operating levers, such as those providing for manually activating and manipulating common endoscopic surgical devices, are mounted onto the slender shaft of a master end unit. By manipulating the slender shaft of a master end unit and/or its associated operating handles, the surgeon causes the slender shaft of the respectively coupled operative end unit to move, such that every movement of the shaft of the master unit is identically tracked and followed. Similarly surgical effectors or devices attached to the distal end of a shaft of an operative end unit are activated by dedicated handles of the respective master unit. Manipulating the handles of the master unit is effected in the same manner as is normally applied whilst operating common surgical equipment during endoscopic and/or open surgery procedures, as is further described infra.

SYSTEM FOR TELESURGERY

Reference is now made to **Figs. 1-3**. In **Fig. 1** system for telesurgery **10** according to the present invention is schematically shown. One or more master end units such as master end unit **12** are mounted onto remote work station **14**. Operative end units, such as end unit **16**, are disposed on surface **18** of a patient's body adjacent to a surgical aperture cut through its wall close to the surgical site. Links such as link **20**, provide for coupling between the movements of slender shafts **21** and **21a** such that shaft **21a** identically moves

while tracking each and every movement of shaft **21**. Moving slender shaft **21** is manually effected by the surgeon. Coupling between the respective shafts can according to the present invention be mechanically, pneumatically, hydraulically and/or electrically accomplished. Link **20** is implemented according to a preferred embodiment of the present invention by hydraulic actuators attached to the respective slender shafts connected by suitable piping. Similarly stretched cables and pulleys provide for such coupling according to another preferred embodiment as is further described infra. Miniature cameras **22** such as consisting of charge coupled devices (CCD) and associated optics, light sources, such as light emitting diodes (LEDs), not shown, respectively attached to the distal ends of slender shafts **24** of operative end units **25** provide for stereoscopic viewing and/or in situ imaging. The location and pointing of each camera is similarly controlled according to the present invention by means of dedicated master end units, not shown, respectively mounted onto workstation **14**. Fiber optic cables **26** provide according to a preferred embodiment of the present invention for feeding each eyepiece of binoculars **28** with its corresponding image as reflected by the respective camera. Optionally, electrical either wired, or wireless, link substitutes the fiber-optic link, such that the stereoscopic features of the image are retained. A pair of operative end units respectively equipped with cameras and their coupled master units and the associated viewing device are regarded hereinafter as a viewing subsystem of a system for telesurgery of the invention, to be further described infra.

The components of a system for telesurgery of the invention are made of common materials typically utilized in manufacturing tools and equipment for endoscopic procedures and/or open surgery operations.

COMMON MODULE

In **Fig. 2A** common module **40** of a system for telesurgery of the invention is schematically shown. Common modules of all end units are identical except for some slight modifications and/or additions, such as operative handles or levers attached to a common module of a master end unit,

or a connecting brackets and/or mounting frames attached to the distal end of a slender shaft for connecting a surgical effector, such as scissors or CCD camera, thereto. Slender shaft **42** is slidingly attached to base plate **44** by means of a sliding bearing, not shown. Rods **46** and **48** are firmly attached to base plate **44**. Rod **46a** is slidingly attached to rod **48** and to slender shaft **42**. For the sake of simplicity for better describing the features of the invention a Cartesian coordinate system is introduced. The axes of the coordinate system are as follows: the x-axis is parallel to rod **46a**, the y-axis is parallel to rod **48a** and the z-axis lies along the slender shaft when is perpendicular to base plate **42**. The origin of the coordinate system is disposed at the center of the sliding bearing, not shown, connecting slender shaft to base plate **44**. Slender shaft **42** is rotatable about any radial axis contained in the x-y plane and whose azimuth angle is any angle in the range $[0,2\pi]$. Slender shaft **42** is further rotatable by an elevation angle its magnitude cannot exceed a predefined value. Any rotation of slender shaft **42** relative to the y-axis results in a movement of rod **46a** in a respective direction of double arrow **49** simultaneously with a slight movement of its end along slender shaft **42**, while rod **48a** stays fixed in place. Similarly any rotation of slender shaft **42** relative to the x-axis induces a respective translational motion of rod **48a** simultaneously with a slight movement of its end along slender shaft **42**, while rod **46a** stays fixed in its original place. Any rotation of the slender shaft by an elevation angle θ relative to an axis in the x-y plane whose azimuth is ϕ is equivalent to two successive rotations one of which is a rotation of the slender shaft by the elevation angle θ relative to the y-axis and the other is a rotation of the inclined slender shaft by the angle ϕ relative to the z-axis. Therefore a rotation of the slender shaft relative to an axis within the x-y plane having any azimuthal angle is equivalent to a pair of lengths Δx , Δy along which rods **46a** and **48a** respectively translate. Furthermore, slender shaft **42** is slidable relative to base plate **44**; its distal end **53** can be lowered down to, and/or raised up to, any desired level by a distance Δz below base plate **44**. Such sliding is accomplished by respectively pushing slender shaft towards, or pulling it off, base plate **44**. Slender shaft **42** is further rotatable relative to its longitudinal axis by any angle in the range of $[0,2\pi]$ in any of the directions shown by double arrow **54**.

In **Fig. 2B** common module **70** of an operative end unit of the invention is shown disposed on a surface of a patient's body. The distal face of base plate **62** is coated with a suitable adhesive, as known, providing for attaching it to surface **64** of the patient's body. Such attaching provides for sealing off the surgical aperture cut through the wall of the patient's body through which slender shaft **66** is introduced. Common module **60** of this operative end unit is secured in place by articulated arm **68** firmly connecting it to a rod extending off a side of operating bench **70**.

In **Fig. 2C** a fragmented isometric view of a segment of common module **90** according to a preferred embodiment of the present invention is shown. Sliding bearing **92** is spherical. It is disposed in an elliptic recess having two apertures respectively disposed on the proximal and the distal surfaces of base plate **94**. A bore whose radius is fitted to the radius of slender shaft **96** is drilled through sliding bearing **92**. Optionally the inner surface of the bore is coated with a film, such as film made of Teflon, interleaving between slender shaft **96** and the surface of the bore. A number of brackets, such as brackets **95**, which are optionally made of Teflon, press against the spherical surface of sliding bearing **92** providing for its rotation about its center, while keeping the center fixed in its place within the recess. The point relative to which a slender shaft is rotatable such as the center point of the aforementioned sliding bearing is referred hereinafter as the center point. Rods **97** are firmly attached to top member **98** which is slidingly attached to base plate **94** by means of sliding bearings **99**. Sliding bearing **92** simultaneously with slender shaft **96** are rotated by inclining slender shaft to a desired direction $[\phi, \theta]$. Such rotations bring about the translations of rods **97** by Δx and Δy respectively, as described hereinabove. A pair of stretched cables **100** and pulleys **102** provide for inducing translational motion of the slender shaft of an operative end unit coupled to its respective master unit by the above mentioned distance Δz .

LINKING A MASTER UNIT TO ITS COUPLED OPERATIVE END UNIT

An exemplary scheme describing mechanical transmission system linking between master end unit **112** and its respectively coupled operative end unit **113** is shown in **Fig. 3**. Both end units **112** and **113** have the same common member described above with reference to **Fig. 2C**. Cables **114** and **116** provide for mechanically linking the simultaneous translational motion along a distance Δz of the slender shafts of both end units. One end of stretched cable **114** is connected to a point close to the proximal end of the slender shaft of master end unit **112**. The other end of cable **114** is connected to a point distally located on the slender shaft of operative end unit **113**, which is proximally disposed relative to upper member **120a**. On the other hand, one end of cable **116** is connected to a point disposed close to the proximal end of the slender shaft of operative end unit **113** whereas the other end of cable **116** is connected to a point distally located on the slender shaft of master end unit **112** which is proximally located relative to upper member unit **120**. Pulleys **117** and **117a** are fixed relative to upper members **120** and **120a** respectively. The distance between both connecting points along both slender shafts is the same and it fits the maximal distance to which the distal end of the slender shaft of operative end unit **113** can extend into the lumen of a body of a patient enclosing the surgical site.

The translational motion of the top members of two coupled common modules along one axis, say the x-axis, can be similarly linked by mechanical transmission system consisting of a pair of stretched cables and two pairs of pulleys, the pulleys of each of which are engaged with a respective cable. Alternatively, an hydraulic transmission system may according to the invention implement such link. Namely, each end of any of the rods **46a** and **48a** of the top member described above with reference to **Fig. 2C** to which reference is again made is connected to a respective hydraulic actuator. In such a case, a pair of hydraulic actuators connected to the ends of two corresponding rods

one of which belongs to a master end unit and the other to its respectively coupled operative end unit, are mutually connected by a hydraulic pipe filled with a biocompatible fluid, such as water. The pipe connects actuators respectively attached to two opposing ends of the respective rods, such that pushing an end of one rod corresponds to pulling the opposite end of the respective rod of the other common module, such that both rods move along the same distance and in the same direction. Such hydraulic transmission system provide for transmitting the translations of the top member of a master end unit to respectively move the top member of its coupled operative end unit. Such linking provide for inducing identical and simultaneous motion of both top members. Such simultaneous motion is accomplished by rotating the slender shaft of the respective master end unit and thereby moving the top members of both end units by the same distances Δx , Δy . Linking can also be according to the invention electrically applied, such as by means of linear actuators or control DC motors associated with suitable electrical logic as known. Similarly the rotational motion of the slender shafts around their longitudinal axes can be linked according to the invention by any of the above mentioned techniques. Operative handles attached to slender shaft of a master end unit for activating and/or manipulating a surgical effector attached the slender shaft of the respectively coupled operative end unit are similarly linked by any of the transmissions systems described above, as is further described infra.

In each of the cases described above the transmission of the rotational and/or translational motions retains a one to one correspondence between the magnitudes and directions of the motion associated with the slender shaft of a master end unit and the tracking motion of its respective follower. Namely translations and or rotations of the slender shaft of an operative end unit are identically the same as induced by the operator inclining, rotating and/or sliding the slender shaft of the respectively coupled master unit. Optionally mechanical, hydraulic, pneumatic and or electric gear transmissions can be incorporated into any link between any pair of coupled end units thereby the magnitude of the transmitted motion is amplified or attenuated as desired. However preferable are transmission ratios of one to one as in such cases the operator performs as if manipulating directly the end units in situ. Therefore

amplification of the transmitted motion should compensate only for losses along a link if any such losses exist, such that the haptic feedback to the surgeon is the same as if while he or she is manipulating the slender shaft of the respective operative end unit.

5 A surgeon is able to place the distal end of the slender shaft of an operative end unit at a desired location having distinct x, y, z coordinates relative to a fixed coordinate system within the lumen of a patient's body by respectively inclining, rotating and/or sliding the slender shaft of the respectively coupled master unit. The surgeon is further able to rotate the slender shaft of
10 an operative end unit such that an effector attached to its distal end points in a desired direction, by similarly rotating the slender shaft of the respective master unit by the suitable angle to the same direction. The surgeon is further able to activate and manipulate a surgical effector as a whole and/or members of a surgical effector attached to a slender shaft of an operative end unit, by
15 manipulating operating handles attached to the slender shaft of the respectively coupled master unit.

ACCESSORIES AND SLENDER SHAFTS

Reference is now made to **Figs 4A – 6B**. Slender shaft **140** shown in
20 **Fig. 4A**, consists of inner shaft **142** enclosed within external sheath **144**. Surgical effector **146**, such as scissors, is disposed at the distal end of slender shaft **140**. Biasing spring, not shown, internally disposed within sheath **144** provides for either opening, or closing, arms **146** when is released. Opening
25 wide both arms and further releasing the biasing spring to close them, or alternatively releasing the biasing spring to open both arms and further closing them are accomplished by means of an opening/closing mechanism installed within the proximal end of sheath **144**, not shown. The opening and further
closing can be accomplished either by repeatedly pressing inwards the proximal end of inner shaft **142** into sheath **144**, or by a reciprocating
30 movement inwards and outwards of the inner shaft **142** into, or off, sheath **144**. Slender shaft **140** can be introduced through the respective sliding bearing of

an operative end unit of the invention into a lumen enclosing the surgical site within a patient's body.

In **Fig. 4B** a slender shaft of a system for telesurgery according to a preferred embodiment of the present invention is shown. Slender shaft **150** is tubular providing for introducing an inner shaft or cables for operating various surgical effectors attached to its distal end. Mounting frame **152**, which is releasably attached to the distal end of pipe **153**, provides for releasably attaching various surgical effectors, such as effector **154**. Locking devices **156** provide for attaching either the mounting frame to pipe **153**, or effector **154** to frame **152**. An exemplary snapping mechanism having a pair of levers resiliently attached to mounting frame **152** whose respective ends are sprung into recesses respectively disposed on the sidewall of pipe **153** and the surface of the body of effector **154** serve as locking devices according to a preferred embodiment of the present invention. For releasing effector **154** off frame **152**, or releasing frame **152** off pipe **153**, the respective lever is laterally pulled off its recess.

Releasing off a surgical effector, and/or attaching it onto a slender shaft whose distal end disposed within the lumen of the patient's body, as well as introducing a new or different surgical effector, are accomplished according to the present invention by means of an introducer. In **Fig. 5A – 5C** elevational views and an isometric view of exemplary introducer **160** are respectively shown. (The same numbers indicate the same parts in **Figs 5A – 5C**.) Shaft **161** is axially disposed within the lumen of slender pipe **162**. Gripper **163** having aperture **164** and a pair of holding arms **165** is attached to the distal end of pipe **162**. Arms **165** can be moved between two positions the first of which is a closed position in which both arms are retracted one towards the other thereby tightly gripping a surgical effector. In a second position the arms are fully extended thereby releasing a gripped effector. The arms are moved into the second position by inwardly pressing the proximal end of shaft **161** into pipe **162**. A biasing spring, not shown presses against both arms to close back and simultaneously to outwardly push shaft **161** to its normal extended position whilst the proximal end of shaft **161** is being released. Hook **166** is extended off

aperture **164** by pulling handle **168** towards handle **166**. A pair of inner cables, not shown, one of which connects hook **166** to handle **168** and the other connects hook **166** to another biasing spring, provides for extending and/or withdrawing hook **166** through aperture **164**. A surgeon may release the above
5 described locking mechanism of a surgical device by first extending hook **166**, then engaging it with the locking mechanism and further pulling back hook **166**.

An isometric view of introducer **170** of a system for telesurgery according to a preferred embodiment of the present invention is shown in **Fig. 5D** being at an extended position. External pipe **172** whose radius is relatively
10 large, such as of 10 mm, encloses articulated inner shaft its distal segments **173** are pivotally attached to each other by hinges **174**. Cylindrical receptacles **175** respectively attached to segments **173** provide for enclosing various surgical effectors to be introduced into the lumen of a patient's body enclosing the surgical site. Pairs of cables, not shown, wound around pulleys mounted
15 onto the proximal end of the slender shaft, such that one end of each cable of a pair is attached to the same respective segment of the inner shaft, whereas the other end is attached to a respective stretching/releasing mechanism, not shown, provide for inclining the respective segment of the inner shaft relative to the axis of pipe **172**. Handles and operative levers provide for selecting a
20 specific pair and either for respectively stretching and releasing each of its cables; and/or selecting all pairs and by similarly concomitantly stretching or releasing, to thereby extending and/or contracting the inner shaft off or into pipe **172**, as known. The surgical effectors are attached to the inner surfaces of receptacles **175** by friction or optionally by a snatch locking mechanism as
25 known.

Elevational views of surgical effector **180** attached to mounting frame **182** each of which is in accordance with a preferred embodiment of the present invention are shown in **Figs 6A** and **6B** respectively. (The same numbers indicate the same parts in **Figs 6A - 6B**.) Gripping lever **184** laterally extends off
30 a cylindrical wall of mounting frame **182**. Both external and internal radii of cylindrical segments **185** respectively fit in with the radii of surgical effectors, such as effector **180**, as well as with the radii of slender shafts, such as shaft

140 or **150** described above with reference to **Figs 4A – 4B** to which reference is again made. Reference is now made to **Figs 6A – 8B**. Locking devices **186** and **188** are of the type of snapping mechanism. Each of them consists of a lever having a spherical end, inwardly protruding from the inner side of the cylindrical wall opposing the wall to which gripping handle **184** is attached. Each such lever passes through a respective bore drilled through the cylindrical wall. The other end of the levers is resiliently attached to the opposite side of the wall, such as by a flat spring. Longitudinal bulges such as bulge **189** are disposed on the inner face of the cylindrical walls opposing the walls onto which the locking devices are attached. One end of each of the bulges is respectively disposed adjacent to the open end of both cylindrical segments **185**. The ends of both bulges are spaced apart from the respective ends of the cylindrical walls. The bulges fit in with recesses respectively disposed on the surfaces of the surgical effectors as well as on the distal end of the slender shafts. The bulges and respective recesses provide keying for properly orienting the mounting frame relative to the slender shaft or effector **180** while attached to either of them. For attaching mounting frame **182** to the distal end of a slender shaft of the invention, the slender shaft is first slid into the respective cylindrical lumen of mounting frame **182** tightly gripped by an introducer. Such sliding may continue along the full depth of the respective cylindrical lumen only when the recess of the slender shaft faces the bulge of the mounting frame. Otherwise bulge **189** stops such sliding unless the slender shaft is oriented accordingly by rotating about its longitudinal axis. The spherical end of lock **186** is inwardly pushed into its respective bore by such axially sliding. This end snaps into its respective recess disposed on the surface of the slender shaft when facing it. The mounting frame is secured to the slender shaft, such that it is axially oriented in a predefined direction by means of the longitudinal bulge and locking device **186**. Alternatively, surgical effector **180** as well as a slender shaft of an operative unit of the invention can be attached to a mounting frame by means of screwing mechanism, bayonet attachment, hook and loop attachment, magnetic attraction, or any other such attaching mechanisms as known.

The inner faces of both arms **190** of surgical effector **180** can be sharpened like scissors or adapted for gripping, such as jaws of tongs or tweezers. Arms **190** are movable between two positions one of which is a closed position and the other is an extended position. A biasing spring, not shown housed within the body of effector **180** provides for retaining arms **190** either at a closed position or at an extended position, when are not forced otherwise by means of a dedicated shaft or lever enclosed by the slender shaft of the invention. A surgeon may continuously move the arms between these two positions and/or change between them by means of operating handles mounted onto the slender shaft of the respective master unit. Such handles are connected to the inner shaft by means of a pair of cables similarly to the operating handles of an introducer for extending/withdrawing its hook as described hereinabove.

A surgical effector may have jaws adapted for grasping, dissecting, cutting, needle holding, coagulating tissue, clip application, or the jaws may comprise a cartridge of staples, etc. Alternatively, a surgical effector is a common device such as but not limited to: knife blades, scissors, dissectors, graspers, scalpels, hooks, hemostatics, clippers, clip removers, needle holders, retractors, suction element, a hook for grasping, tissue dissection, or cutting, or a cartridge of staples. Interchangeable surgical effectors releasably attached to slender shafts of an operative end units, can be according to the invention relatively robust, having diameters within a range of 4 to 10 mm, whereas the shafts diameters are within a range of 1 to 3 mm. Therefore a small surgical aperture of 1 – 3 mm cut through the wall of the patient's body provide for introducing such slender shafts into the lumen enclosing the surgical site. However a significantly larger surgical aperture of 5 – 10 mm provides for introducing relatively larger surgical effectors by means of suitable introducers. Obviously small sized openings cut through the wall of a patient's body are less painful and leave an imperceptible scar. Therefore a single relatively large surgical aperture may be used according to the invention to support a number of small sized surgical apertures for introducing slender shafts of the respective operative end units.

Elevational views of exemplary linking accessories for a system for telesurgery of the invention are shown in **Figs 7A – 7B**. Hydraulic pipe **220** consists of pipe **222** enclosed within protective cover **224** having connectors, such as connector **226** disposed at its both ends providing for snap connecting.

5 Cable accessory **230** consists of a number of cables **232** each of which is threaded through an individual pipe, such as pipe **234** providing for its being stretched. The inner surfaces of the pipes are covered with a material having a low coefficient of friction such as Teflon for minimizing friction forces exerted on the cables while being translated within the enclosing pipes. The pipes are

10 further surrounded with protective cover **236**.

Two distal segments of slender shafts of an operative end unit of a system for telesurgery according to two other preferred embodiments of the present invention are schematically shown in **Figs 8A – 8B**. The distal end of slender shaft **240** is articulated. Sub-segments **244** are pivotally attached to

15 each other by means of hinges such as hinge **246**. Surgical effector **248** is attached to the distal end of slender shaft **240**. The angle between sub-segments **244** is changeable by means of inner cables respectively connected to each sub-segment at its both opposing sides. The distal segment of slender shaft **260** consists of a plurality of cylindrical rings **262**. A pair of cables **264**

20 respectively threaded through loops internally attached to the inner surface of each ring which are symmetrically disposed on the opposing inner faces of each ring provides for bending the distal segment. Cables **265** provide for manipulating the jaws of surgical effector **266**. By means of such slender shaft an operator is able to access locations within the body of the patient which are

25 covered by a tissue or an organ when viewed from the surgical aperture through which the slender shaft is introduced. Optionally both slender shafts can be such configured to provide for deflecting the surgical effectors in two different planes. Therefore a system for telesurgery having such slender shafts provides a surgeon with six degrees of freedom: three of them provide him for

30 positioning the distal end of the slender shaft at a desired point in space; the fourth degree provides for axially rotating the slender shaft around its

longitudinal axis, and the last two correspond to the two different planes in which the slender shaft can be deflected.

5 VIEWING SUBSYSTEM

A viewing subsystem of a system for telesurgery of the invention includes a control member linked to a remote viewing member equipped with cameras and optional illuminating sources capable of being introduced into a lumen within the body of a patient. Reference is now made to **Figs 9A – 9B** in
10 which two members of a viewing subsystem of a system for telesurgery according to a preferred embodiment of the present invention are schematically shown respectively. Remote viewing member **280** has a pair of mutually connected operative end units **281** and **281a** attached to surface **282** of a patient. Attaching is effected by means of articulated arm **284** connected to
15 surgical bench **286** on which the patient is lying. Cameras **288** are respectively attached to the distal ends of slender shafts **290**. Slender shafts **290** are introduced down to a pre-specified level beneath surface **282**, and axially oriented such that both distal ends are spaced apart and separated by a predefined separation and the lines of sight of both cameras intersect at point
20 **292** within the surgical site. The distance between both cameras **288** conforms to a normal distance between the human eyes.

Control member **300** has two mutually connected master units **302** and **302a** oriented and spaced apart by the same orientation and separation as the operative end units of the respective remote viewing member are disposed
25 relative to each other. The distal ends of slender shafts **304** are slidingly attached to two horizontal rods **305** each of which is pivotally attached to the distal end of slender shaft **306**. The magnitude of angle **308** and the direction to which angle **308** points namely, the direction of its axis, as well as the angle between the plane containing angle **308** and the axis of the slender shaft **306**,
30 can be fixed and/or changed by the operator by means of operating handles of

master end unit **310**, not shown. Therefore the line of sight can be adjusted by the operator by respectively inclining, rotating and/or sliding slender shafts **304** following the adjusting of the magnitude and/or pointing of angle **308**. Optionally slender shafts **304** and slender shaft **306** are simultaneously connected to an actuating device operated by a joystick as known, providing the operator for conveniently pointing both cameras such that the best field of view and focusing of the surgical site are received.

The control member of the viewing subsystem of a system for telesurgery in accordance with another preferred embodiment of the present invention consists of a pair of common modules, such as pair **320** schematically shown in **Fig. 2C**. The separation and relative orientation of base plates **322** and **322a** can be manually fixed by means of brackets **324** and bolt **325**. Slender shafts **326** and **326a** are pivotally attached to each other by hinge **328** distally disposed relative to base plates **322** and **322a**. Each common module of the pair is linked to its respective module of the viewing member as described hereinabove. Optionally to sliding bearing pivotally attached to each other substitute hinge **328** thereby enabling distally or proximally displacing the axis of rotations of one of the slender shafts relative to the other relative to baseplates **322** and **322a**. The operator may push or pull and/or incline any of the slender shafts of the pair of common module of the control member and further adjust their rotational angle relative to their respective axes to thereby change the field of view and its center.

Both aforementioned control members further include binoculars, not shown, whose left and right eyepieces can be independently focused and are respectively connected to the left and right cameras of the remote viewing member. Links, not shown, including: a. mechanical transmissions for simultaneously sliding and/or axially rotating the respective slender shafts, and b. hydraulic transmissions providing for simultaneously inclining the respective slender shafts, of all master and operative end units of both the control and remote members, are further provided according to the present invention.

EXAMPLE

Reference is now made to **Fig. 10** in which master unit **330** of a system for telesurgery according to a preferred embodiment is schematically shown. Operating handles such as handles **332** attached to the proximal end of the slender shaft and/or handles **334** attached to its distal end, provide for activating and manipulating the surgical effector of the respectively coupled operative end unit. Pushing and/or pulling sideways handles **332**, causes the slender shafts of master unit **330** and its respectively coupled operative end unit to be simultaneously inclined. Such inclination is to the same direction, by the same rotational angle, such that the proximal ends of both slender shafts move along the same vector describing the motion of the proximal end of the slender shaft of master unit **330**. However the distal end of the respective surgical effector moves in the opposite direction by a proportional distance, whose magnitude depends on the ratio between the lengths of the segment of the slender shaft disposed distally to the center point and the segment proximally disposed to the same center point. However translating the distal end of the slender shaft of master unit **330** by moving handles **334** simultaneously moves the distal end of the surgical effector. Such movement is represented by the same vector describing the motion of the distal end of the shaft of master unit **330**. Therefore the surgeon manipulating the surgical effector by means of handles **334** performs as in a normal open surgery, whereas manipulating by means of handles **332** is analogous to any normal endoscopic procedure. The system including a master unit such as master unit **330** may serve for any endoscopic operation within cavities, virtual cavities, artificially created cavities, including but not limited to: laparoscopy, retroperitoneoscopy, thoracoscopy, arthroscopy, percutaneous endoscopic surgery within cavities such as urinary bladder, stomach, heart, subcutaneous endoscopy (inguinal lymph node dissection; thyroid surgery, parathyroid surgery, breast augmentation and face lifting.

CLAIMS

1. A system for telesurgery comprising

- at least one operative end unit attachable to a surface of the
5 body of a patient;
- at least one master end unit for controlling and manipulating
a member of said at least one operative end unit, and

wherein said at least one master unit and said at least one
operative end unit each comprises a common module, and
10 wherein said common module comprises

- a base plate having a distal surface;
- a top member slidingly attached to said base
plate;
- a slender shaft having an axis, a proximal end and
15 a distal end slidingly attached to said base plate,
wherein said proximal end proximally disposed
relative to said base plate, and wherein said distal
end distally disposed relative to said base plate,
and

20 wherein said at least one operative end unit linked to said
at least one master unit, such that the slender shafts of
both said at least one master end unit and said at least
one operative end unit simultaneously slide.

2. A system for telesurgery as in claim 1, wherein said slender shaft is rotatable about a center point proximally disposed relative to said distal surface.
- 5 3. A system for telesurgery as in claim 2, wherein said slender shaft is further axially rotatable.
4. A system for telesurgery as in claim 1, wherein an operative handle is attached adjacent to the proximal end of at least one of said slender
10 shafts.
5. A system for telesurgery as in claim 1, wherein an operative handle is attached adjacent to the distal end of at least one of said slender
15 shafts.
6. A system for telesurgery as in claim 1, wherein a segment of at least one of said slender shafts is articulated.
7. A system for telesurgery as in claim 6, wherein a sub-segment of said
20 segment is deflectable aside from said axis.
8. A system for telesurgery as in claim 7, wherein said segment comprises at least one hinge providing for said deflection.

9. A system for telesurgery as in claim 1, wherein a surgical effector is attached to the distal end of at least one of said slender shafts.
10. A system for telesurgery as in claim 9, wherein said surgical effector is any item selected from a group of items consisting of scissors, dissectors, graspers, scalpels, hooks, hemostatics, clipers, clip removers, needle holders, retractors and any combination thereof.
11. A system for telesurgery as in claim 9, wherein said surgical effector releasably attached to said distal end.
12. A system for telesurgery as in claim 9, wherein said surgical effector is interchangeable.
13. A system for telesurgery as in claim 1, further comprising an introducer to which a surgical effector is attachable.
14. A system for telesurgery as in claim 13, wherein said introducer comprises at least one receptacle for enclosing said surgical effector.
15. A system for telesurgery as in claim 1, wherein said distal surface coated with an adhesive material for sealing a surgical aperture.
16. A system for telesurgery as in claim 1, wherein a transmission system provides for said linking, and wherein said transmission system

comprises any item selected from a group of items consisting of cables, pulleys, hydraulic actuators, pneumatic actuators, electrical actuators, hydraulic pipes and any combination thereof.

5 17. A system for telesurgery as in claim 1, wherein a camera is attached to the slender shaft of said at least one operative end unit.

18. A system for telesurgery as in claim 1, wherein a light source is attached to the slender shaft of said at least one operative end unit.

10

19. A system for telesurgery as in claim 17, wherein said at least one operative end unit is the first operative end unit, and wherein a camera is attached to the distal end of the slender shaft of a second operative end unit, and wherein both said first and second operative end units spaced apart from each other, and wherein each of the first and second operative end units respectively linked to a first and second master end units similarly spaced apart from each other.

15

20. A system for telesurgery as in claim 19, wherein said cameras are spaced apart from each other by a pre-specified distance, and wherein said cameras are simultaneously movable such that each of said cameras points at the same point.

20

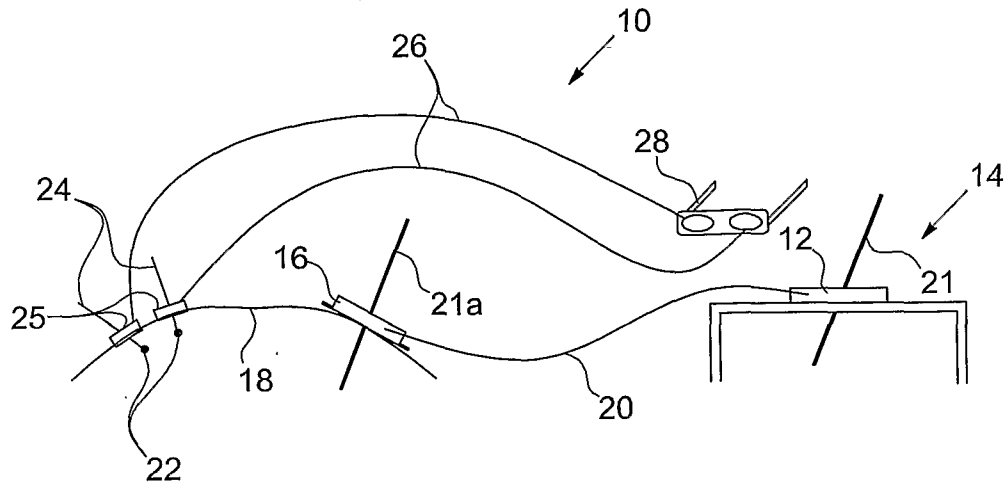


Fig. 1

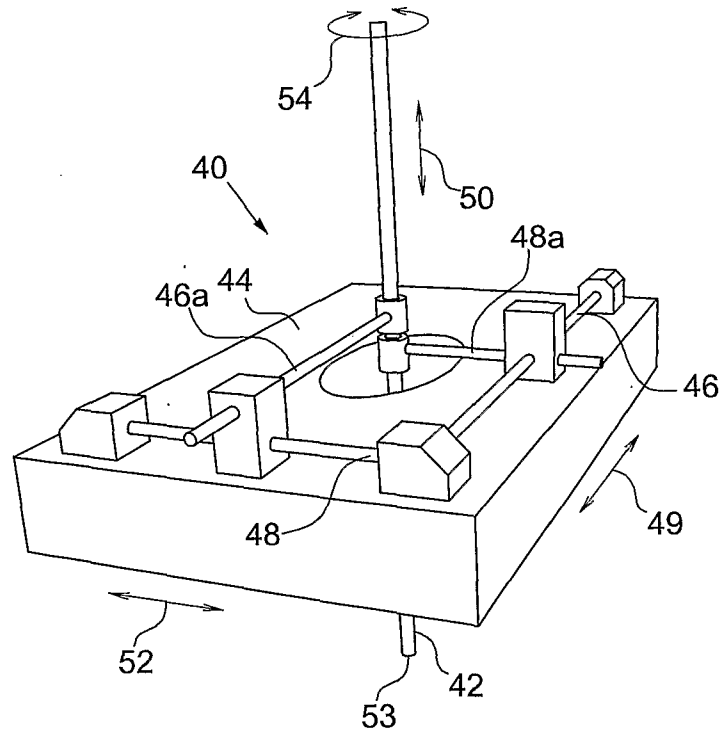


Fig. 2A

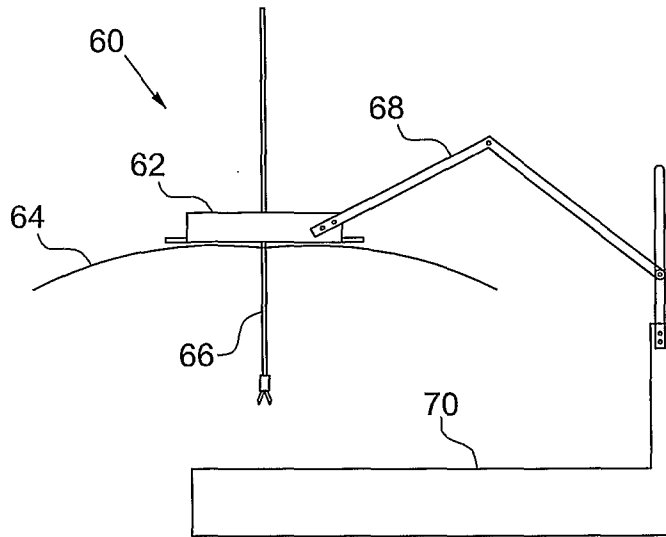


Fig. 2B

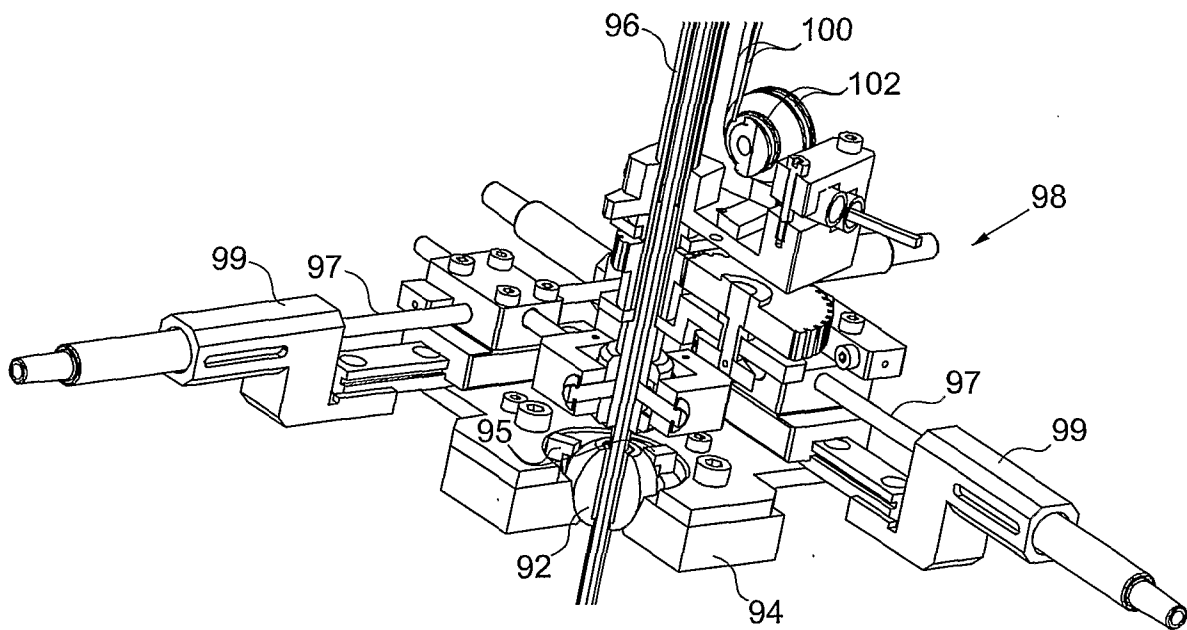


Fig. 2C

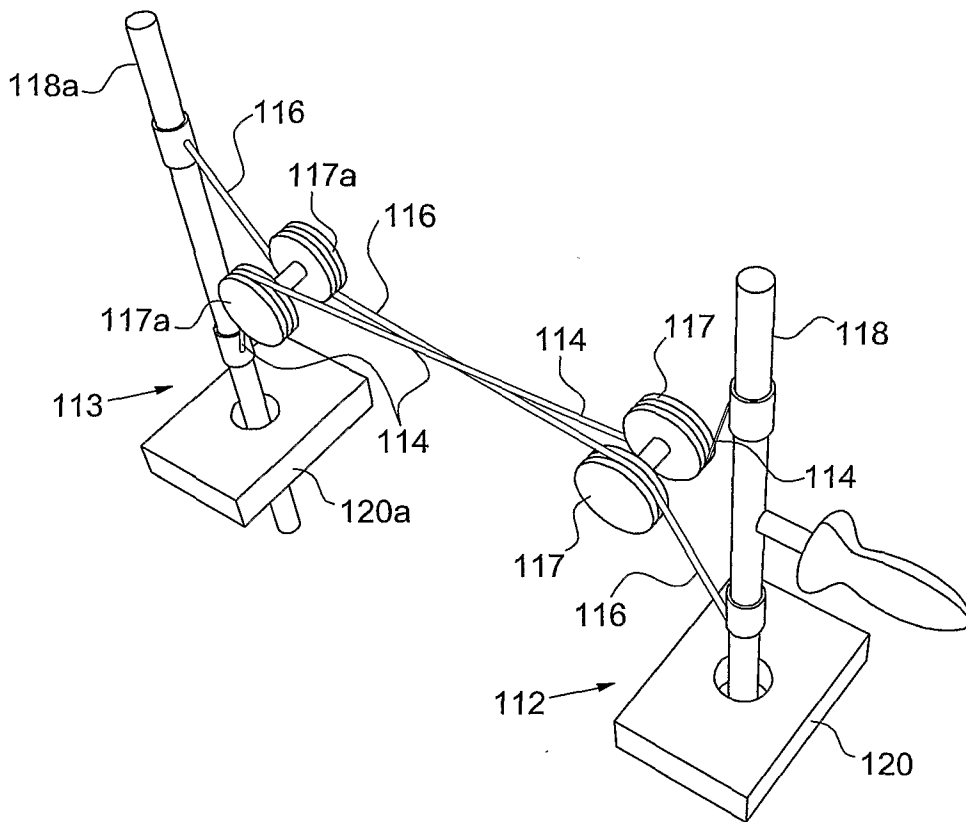


Fig. 3

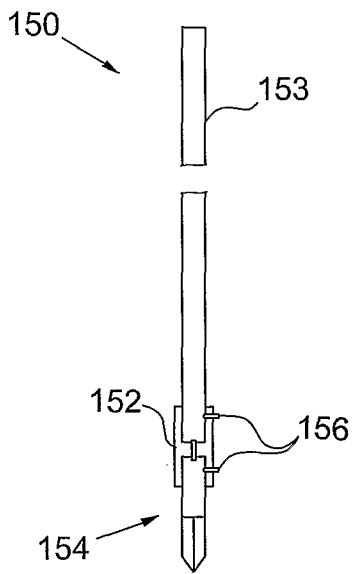


Fig. 4B

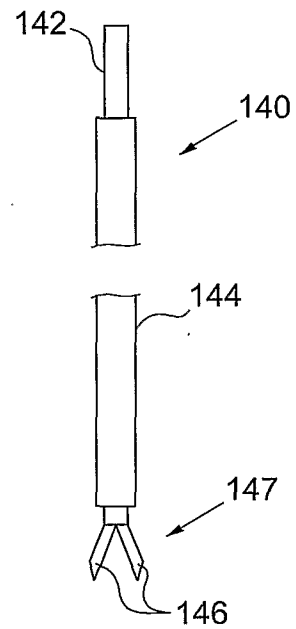


Fig. 4A

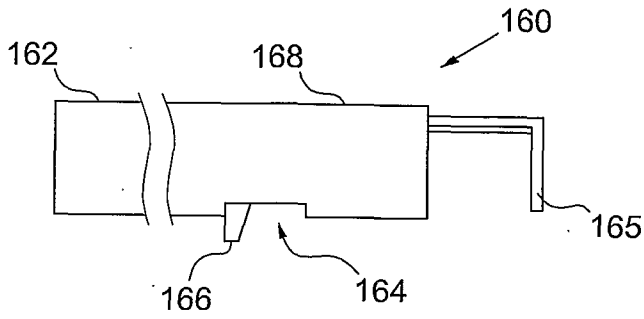


Fig. 5B

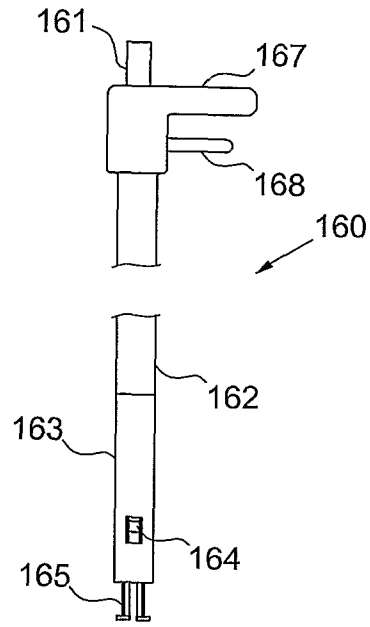


Fig. 5A

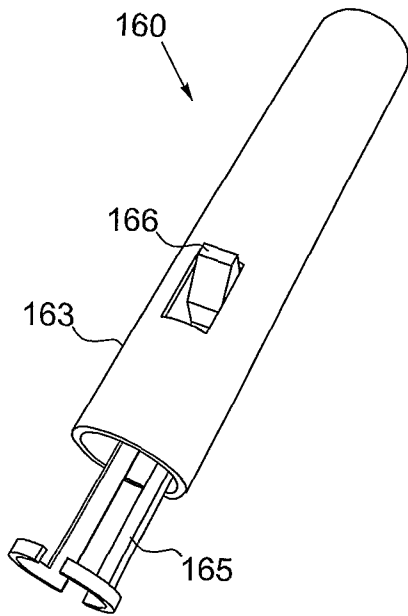


Fig. 5C

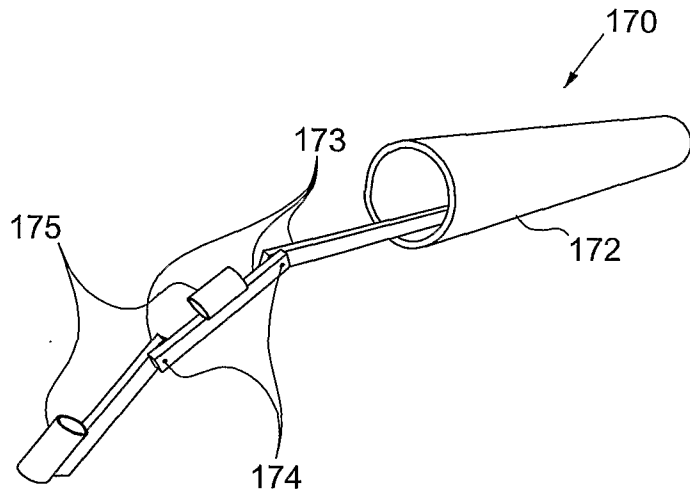


Fig. 5D

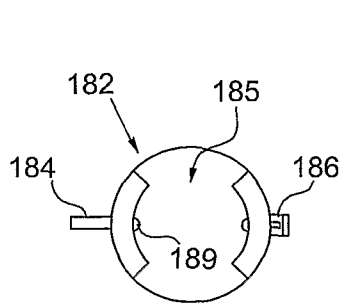


Fig. 6B

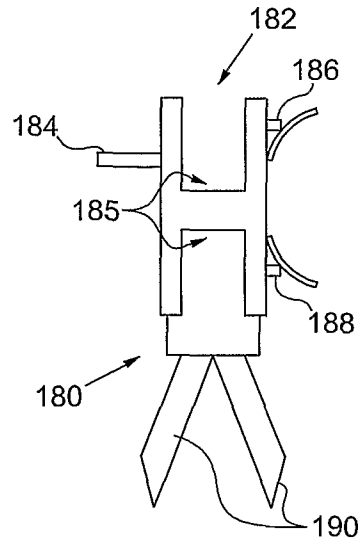


Fig. 6A

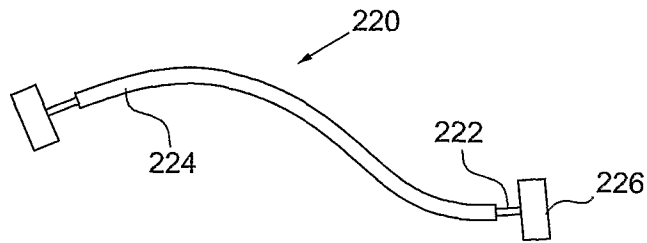


Fig. 7A

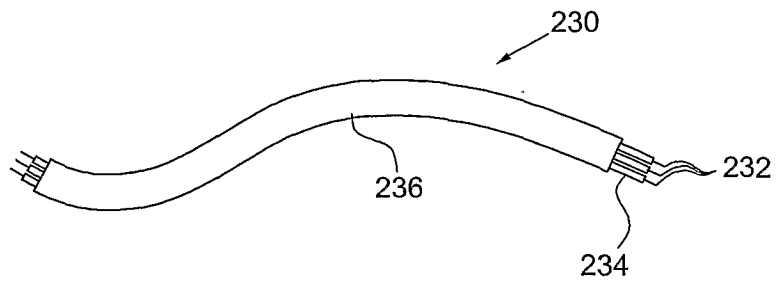


Fig. 7B

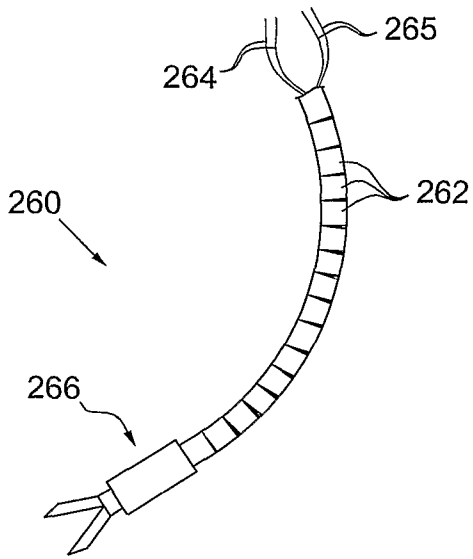


Fig. 8B

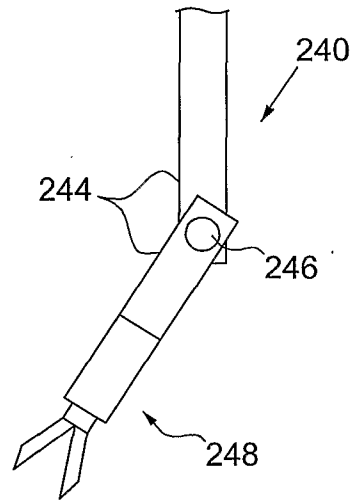


Fig. 8A

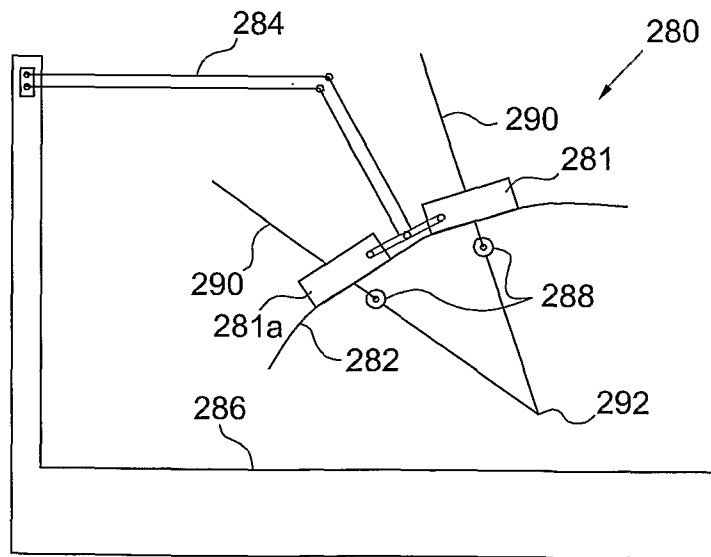


Fig. 9A

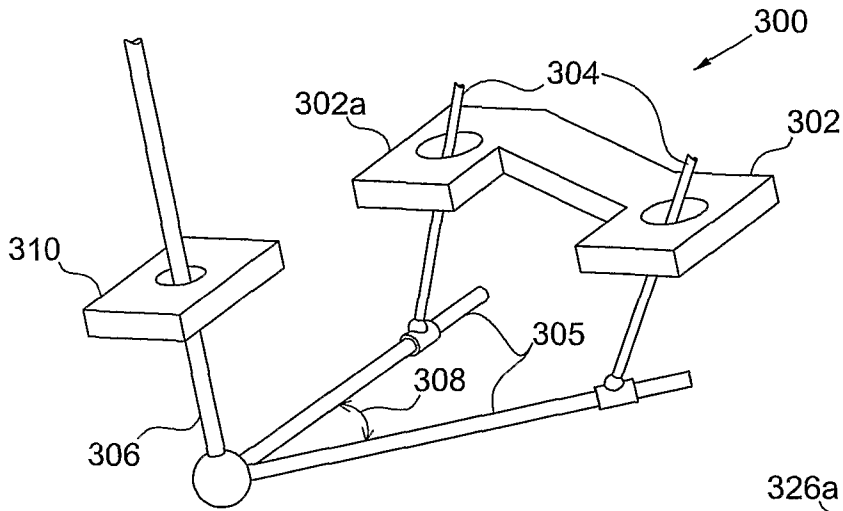


Fig. 9B

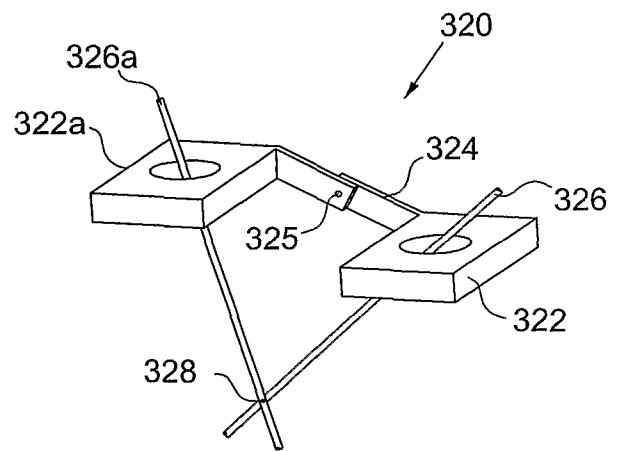


Fig. 9C

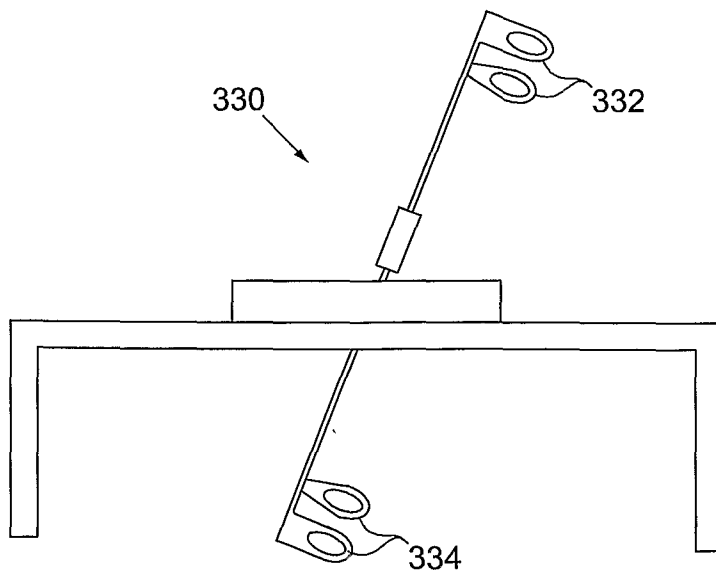


Fig. 10