

(43) International Publication Date
15 September 2016 (15.09.2016)

(51) International Patent Classification:

G01N 33/68 (2006.01) H01J 49/00 (2006.01)
A61B 17/00 (2006.01) A61B 18/00 (2006.01)
G01N 3/00 (2006.01) G01N 27/62 (2006.01)
G01N 9/00 (2006.01)

(21) International Application Number:

PCT/GB2016/050604

(22) International Filing Date:

7 March 2016 (07.03.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

1503876.3	6 March 2015 (06.03.2015)	GB
1503864.9	6 March 2015 (06.03.2015)	GB
1503877.1	6 March 2015 (06.03.2015)	GB
1503867.2	6 March 2015 (06.03.2015)	GB
1503863.1	6 March 2015 (06.03.2015)	GB
1503878.9	6 March 2015 (06.03.2015)	GB
1503879.7	6 March 2015 (06.03.2015)	GB
1516003.9	9 September 2015 (09.09.2015)	GB
1518369.2	16 October 2015 (16.10.2015)	GB

(71) Applicant: **MICROMASS UK LIMITED** [GB/GB];
Stamford Avenue, Altrincham Road, Wilmslow SK9 4AX
(GB).(72) Inventors: **PRINGLE, Steven Derek**; Linden Cottages,
Temple, Hoddlesden, Darwen BB3 3PS (GB). **MORRIS,
Michael Raymond**; 78 Bankbottom, Hadfield, Glossop
Derbyshire SK13 1BX (GB). **BALOG, Júlia**; 35 Voros-


marty út, 2083 Solymar (HU). **JONES, Emrys**; 16 Cran-
mer Road, Manchester M20 6AW (GB). **RICHARDSON,
Keith**; 89 Marsh Lane, New Mills, High Peak Derbyshire
SK22 4PP (GB). **LANGRIDGE, James Ian**; 8 Brook-
wood Avenue, Sale, Cheshire M33 5BZ (GB). **SIMON,
Dániel**; 5 Hegy utca, 9131 Mórchida (HU). **GÖDÖRHÁZY,
Lajos**; 49 Mecseki út, 2030 Érd (HU). **SZALAY, Dániel**;
5 Székely Bertalan út, 1062 Budapest (HU). **TAKÁTS,
Zoltán**; 12 Church Street, Haslingfield, Cambridge CB23 1JE (GB).

(74) Agent: **JEFFREY, Philip Michael**; Dehns, St. Bride's
House, 10 Salisbury Square, London EC4Y 8JD (GB).(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,
TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU,
TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE,
DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU,
LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,

[Continued on next page]

(54) Title: IMAGING GUIDED AMBIENT IONISATION MASS SPECTROMETRY

Fig. 2

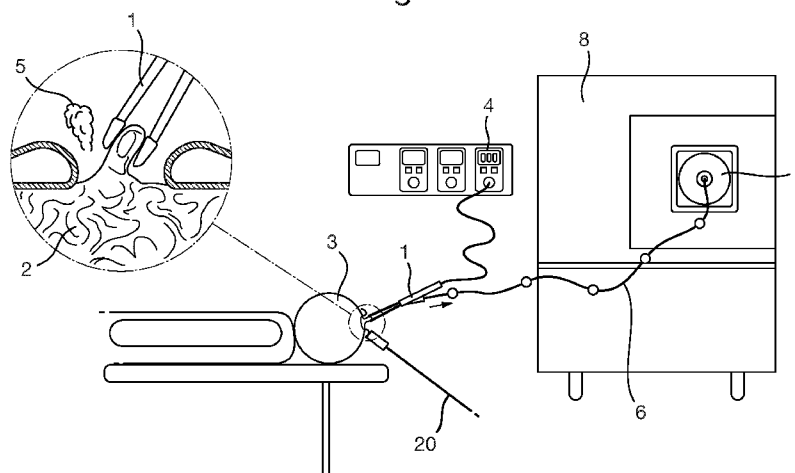

(57) Abstract: A method is disclosed comprising obtaining or acquiring image or other data from one or more regions of a target (2) using an imaging sensor (20). The image or other data may then be used to determine one or more regions of interest of the target (2). An ambient ionisation ion source (1) may then be used to generate aerosol, smoke or vapour (5) from one or more regions of the target (2).



SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, —
GW, KM, ML, MR, NE, SN, TD, TG).

*before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments (Rule 48.2(h))*

Published:

— *with international search report (Art. 21(3))*

IMAGING GUIDED AMBIENT IONISATION MASS SPECTROMETRY

5 CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority from and the benefit of United Kingdom patent application No. 1503876.3 filed on 6 March 2015, United Kingdom patent application No. 1503864.9 filed on 6 March 2015, United Kingdom patent application No. 1518369.2 filed on 16 October 2015, United Kingdom patent application No. 1503877.1 filed on 6 March 2015, United Kingdom patent application No. 1503867.2 filed on 6 March 2015, United Kingdom patent application No. 1503863.1 filed on 6 March 2015, United Kingdom patent application No. 1503878.9 filed on 6 March 2015, United Kingdom patent application No. 1503879.7 filed on 6 March 2015 and United Kingdom patent application No. 1516003.9 filed on 9 September 2015. The entire contents of these applications are incorporated herein by reference.

FIELD OF THE INVENTION

20 The present invention relates generally to the analysis of a target (which may, for example, comprise *in vivo*, *ex vivo* or *in vitro* biological tissue, a bacterial or fungal colony or more generally an organic target such as a plastic) by ambient ionisation techniques such as rapid evaporative ionisation mass spectrometry ("REIMS"), methods of analysis and diagnosis and apparatus for analysing a target using an ambient ionisation ion source. Various embodiments are contemplated wherein
25 analyte ions generated by an ambient ionisation ion source are then subjected either to: (i) mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser; (ii) ion mobility analysis (IMS) and/or differential ion mobility analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis; and/or (iii) a combination of firstly ion mobility analysis (IMS) and/or
30 differential ion mobility analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis followed by secondly mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser (or vice versa). Various embodiments also relate to an ion mobility spectrometer and/or
35 mass analyser and a method of ion mobility spectrometry and/or method of mass analysis.

BACKGROUND

40 Rapid evaporative ionisation mass spectrometry ("REIMS") is a relatively new technique that is useful for the analysis of many different types of samples including the identification of tissue.

Reference is made to N. Strittmatter *et al.*, Anal. Chem. 2014, 86, 6555-6562 which discloses an investigation into the suitability of using rapid evaporative ionisation mass spectrometry as a general identification system for bacteria and fungi.

5 The known approach for analysing bacterial colonies by rapid evaporative ionisation mass spectrometry involves using bipolar electrosurgical forceps and an electrosurgical RF generator. A bacterial colony is scraped from the surface of an agar layer using the bipolar electrosurgical forceps and a short burst of RF voltage from the electrosurgical RF generator is applied between the bipolar electrosurgical
10 forceps. For example, it is known to apply 60 W of power in a bipolar mode at a frequency of 470 kHz sinusoid. The RF voltage which is applied to the electrosurgical forceps has the result of rapidly heating the particular portion of the bacterial colony which is being analysed due to its nonzero impedance. The rapid heating of the microbial mass results in an aerosol being generated. The aerosol is
15 transferred directly into a mass spectrometer and the aerosol sample may then be analysed by the mass spectrometer. It is known to utilise multivariate statistical analysis in order to help distinguish and identify different samples.

It is desired to provide an improved method of analysing a target or tissue using an ambient ionisation ion source.

SUMMARY

According to an aspect there is provided a method comprising:
obtaining or acquiring image or other data from one or more regions of a
25 target;
 using the image or other data to determine one or more regions of interest of the target; and
 using a first device to generate aerosol, smoke or vapour from one or more regions of the target.

30 In accordance with various embodiments a target (which may comprise *in vivo*, *ex vivo* or *in vitro* biological tissue, a bacterial or fungal colony or a more general organic target such as a plastic) is imaged. For example, the target may be optically, X-ray or thermally imaged and regions of interest in the target may be identified from the optical or thermal image. A region of potentially cancerous tissue
35 may be identified on the basis of having a higher temperature than that of surrounding tissue. The image data may then be used to direct a surgeon as to which tissue potentially needs to be resected.

A particularly beneficial aspect is that when an ambient ionisation source is used to generate aerosol, smoke or vapour from one or more regions of the target,
40 the resulting aerosol, smoke or vapour may be ionised by directing the aerosol, smoke or vapour onto a collision surface within a vacuum chamber of a mass

spectrometer and/or ion mobility spectrometer. The resulting analyte ions may then be analysed and mass spectrometric data and/or ion mobility data may be obtained.

The mass spectrometric data and/or ion mobility data may be analysed in real time and subjected to multivariate analysis enabling a determination to be made in real time as to whether or not the tissue which is currently being resected or otherwise analysed is cancerous or not. As a result, a surgeon is able to make an accurate determination of the disease state of any tissue which is being operated upon or resected and also the surgeon is able to make an accurate determination of the margins of the tumour. It will be readily apparent that it is particularly important when resecting a tumour to ensure that all cancerous tissue is removed whilst at the same time ensuring that as minimal amount of healthy tissue as possible is removed.

The ability, therefore, of acquiring image data of a target (e.g. tissue) and using this image data to assist a surgeon when operating on a patient using a surgical tool such as a rapid evaporative ionisation mass spectrometry device enables an improved method of analysis to be performed with the result that a patient has a greater probability of a positive surgical outcome.

N. Strittmatter *et al.*, Anal. Chem. 2014, 86, 6555-6562 does not disclose acquiring image data from a target such as *in vivo* tissue and does not disclose using image data to determine one or more regions of tissue which are of potential interest (i.e., regions of tissue which may be potentially cancerous tissue).

The image or other data may comprise data selected from the group consisting of: (i) thermal, temperature or thermographic image data; (ii) microwave image data; (iii) visual or optical image data; (iv) infra-red ("IR") image data; (v) radio-frequency ("RF") image data; (vi) X-ray image data; (vii) magnetic resonance imaging ("MRI") image data; (viii) ultrasonic or ultrasound image data; (ix) tomographic image data; (x) optical or other absorption data; (xi) optical or other scattering coefficient data; (xii) oxyhemoglobin or deoxyhemoglobin absorbance data; or (xiii) near infrared (NIR) image data.

The first device may comprise or form part of an ambient ion or ionisation source (or other ionisation source) or the first device may generate aerosol, smoke or vapour for subsequent ionisation by an ambient ion or ionisation source (or other ionisation source).

The target may comprise native or unmodified target material.

The native or unmodified target material may be unmodified by the addition of a matrix or reagent.

The first device may be arranged and adapted to generate aerosol, smoke or vapour from one or more regions of the target without the target requiring any prior preparation.

The first device may comprise an ion source selected from the group consisting of: (i) a rapid evaporative ionisation mass spectrometry ("REIMS") ion source; (ii) a desorption electrospray ionisation ("DESI") ion source; (iii) a laser desorption ionisation ("LDI") ion source; (iv) a thermal desorption ion source; (v) a

laser diode thermal desorption ("LDTD") ion source; (vi) a desorption electro-flow focusing ("DEFFI") ion source; (vii) a dielectric barrier discharge ("DBD") plasma ion source; (viii) an Atmospheric Solids Analysis Probe ("ASAP") ion source; (ix) an ultrasonic assisted spray ionisation ion source; (x) an easy ambient sonic-spray ionisation ("EASI") ion source; (xi) a desorption atmospheric pressure photoionisation ("DAPPI") ion source; (xii) a paperspray ("PS") ion source; (xiii) a jet desorption ionisation ("JeDI") ion source; (xiv) a touch spray ("TS") ion source; (xv) a nano-DESI ion source; (xvi) a laser ablation electrospray ("LAESI") ion source; (xvii) a direct analysis in real time ("DART") ion source; (xviii) a probe electrospray ionisation ("PESI") ion source; (xix) a solid-probe assisted electrospray ionisation ("SPA-ESI") ion source; (xx) a cavitron ultrasonic surgical aspirator ("CUSA") device; (xxi) a focussed or unfocussed ultrasonic ablation device; (xxii) a microwave resonance device; and (xxiii) a pulsed plasma RF dissection device.

The step of using the first device to generate aerosol, smoke or vapour from one or more regions of the target may further comprise contacting the target with one or more electrodes.

The one or more electrodes may comprise: (i) a monopolar device, wherein the method optionally further comprises providing a separate return electrode; (ii) a bipolar device; or (iii) a multi phase RF device, wherein the method optionally further comprises providing a separate return electrode or electrodes.

The one or more electrodes may comprise a rapid evaporation ionization mass spectrometry ("REIMS") device.

The method may further comprise applying an AC or RF voltage to the one or more electrodes in order to generate the aerosol, smoke or vapour.

The step of applying the AC or RF voltage to the one or more electrodes may further comprise applying one or more pulses of the AC or RF voltage to the one or more electrodes.

The step of applying the AC or RF voltage to the one or more electrodes may cause heat to be dissipated into the target.

The step of using the first device to generate aerosol, smoke or vapour from one or more regions of the target may further comprise irradiating the target with a laser.

The first device may be arranged and adapted to generate aerosol from one or more regions of the target by direct evaporation or vaporisation of target material from the target by Joule heating or diathermy.

The step of using the first device to generate aerosol, smoke or vapour from one or more regions of the target may further comprise directing ultrasonic energy into the target.

According to another embodiment an optical fibre coupled to a laser source may be used to generate the aerosol, smoke or vapour.

The aerosol may comprise uncharged aqueous droplets optionally comprising cellular material.

At least 50%, 55%, 60%, 65%, 70%, 75%, 80%, 85%, 90% or 95% of the mass or matter generated by the first device and which forms the aerosol may be in the form of droplets.

The first device may be arranged and adapted to generate aerosol wherein the Sauter mean diameter ("SMD", d_{32}) of the aerosol may be in a range: (i) $< 5 \mu\text{m}$; (ii) $5\text{--}10 \mu\text{m}$; (iii) $10\text{--}15 \mu\text{m}$; (iv) $15\text{--}20 \mu\text{m}$; (v) $20\text{--}25 \mu\text{m}$; or (vi) $> 25 \mu\text{m}$.

The aerosol may traverse a flow region with a Reynolds number (Re) in the range: (i) < 2000 ; (ii) $2000\text{--}2500$; (iii) $2500\text{--}3000$; (iv) $3000\text{--}3500$; (v) $3500\text{--}4000$; or (vi) > 4000 .

Substantially at the point of generating the aerosol, the aerosol may comprise droplets having a Weber number (We) selected from the group consisting of: (i) < 50 ; (ii) $50\text{--}100$; (iii) $100\text{--}150$; (iv) $150\text{--}200$; (v) $200\text{--}250$; (vi) $250\text{--}300$; (vii) $300\text{--}350$; (viii) $350\text{--}400$; (ix) $400\text{--}450$; (x) $450\text{--}500$; (xi) $500\text{--}550$; (xii) $550\text{--}600$; (xiii) $600\text{--}650$; (xiv) $650\text{--}700$; (xv) $700\text{--}750$; (xvi) $750\text{--}800$; (xvii) $800\text{--}850$; (xviii) $850\text{--}900$; (xix) $900\text{--}950$; (xx) $950\text{--}1000$; and (xxi) > 1000 .

Substantially at the point of generating the aerosol, the aerosol may comprise droplets having a Stokes number (S_k) in the range: (i) $1\text{--}5$; (ii) $5\text{--}10$; (iii) $10\text{--}15$; (iv) $15\text{--}20$; (v) $20\text{--}25$; (vi) $25\text{--}30$; (vii) $30\text{--}35$; (viii) $35\text{--}40$; (ix) $40\text{--}45$; (x) $45\text{--}50$; and (xi) > 50 .

Substantially at the point of generating the aerosol, the aerosol may comprise droplets having a mean axial velocity selected from the group consisting of: (i) $< 20 \text{ m/s}$; (ii) $20\text{--}30 \text{ m/s}$; (iii) $30\text{--}40 \text{ m/s}$; (iv) $40\text{--}50 \text{ m/s}$; (v) $50\text{--}60 \text{ m/s}$; (vi) $60\text{--}70 \text{ m/s}$; (vii) $70\text{--}80 \text{ m/s}$; (viii) $80\text{--}90 \text{ m/s}$; (ix) $90\text{--}100 \text{ m/s}$; (x) $100\text{--}110 \text{ m/s}$; (xi) $110\text{--}120 \text{ m/s}$; (xii) $120\text{--}130 \text{ m/s}$; (xiii) $130\text{--}140 \text{ m/s}$; (xiv) $140\text{--}150 \text{ m/s}$; and (xv) $> 150 \text{ m/s}$.

The target may comprise biological tissue, biological matter, one or more bacterial colonies or one or more fungal colonies.

The biological tissue may comprise human tissue or non-human animal tissue.

The biological tissue may comprise *in vivo* biological tissue.

The biological tissue may comprise *ex vivo* biological tissue.

The biological tissue may comprise *in vitro* biological tissue.

According to an embodiment one or more bacterial or fungal colonies may be subjected to imaging and image or other data may be acquired. The imaging process may, for example, comprise an optical imaging process, X-ray imaging or polarised light. One or more regions of interest may then be identified. For example, according to an embodiment one or more phase change regions or borders of the one or more bacterial or fungal colonies may be identified. As a result of determining a phase change region or border a region of interest in the colony may be determined. The region of interest may then be analysed using an ambient ionisation ion source.

Yet further embodiments are contemplated wherein the target may more generally comprise an organic target including materials such as a plastic. The target may be imaged (e.g., using X-ray or microwave imaging) to identify regions of

the target which exhibit a change of density or other property (e.g., in the plastic). One or more regions of interest in the (e.g., plastic) organic target may then be identified and may then be subjected to analysis using an ambient ionisation ion source.

- 5 The biological tissue may comprise (i) adrenal gland tissue, appendix tissue, bladder tissue, bone, bowel tissue, brain tissue, breast tissue, bronchi, coronal tissue, ear tissue, esophagus tissue, eye tissue, gall bladder tissue, genital tissue, heart tissue, hypothalamus tissue, kidney tissue, large intestine tissue, intestinal tissue, larynx tissue, liver tissue, lung tissue, lymph nodes, mouth tissue, nose tissue, 10 pancreatic tissue, parathyroid gland tissue, pituitary gland tissue, prostate tissue, rectal tissue, salivary gland tissue, skeletal muscle tissue, skin tissue, small intestine tissue, spinal cord, spleen tissue, stomach tissue, thymus gland tissue, trachea tissue, thyroid tissue, ureter tissue, urethra tissue, soft and connective tissue, peritoneal tissue, blood vessel tissue and/or fat tissue; (ii) grade I, grade II, grade III or grade IV cancerous tissue; (iii) metastatic cancerous tissue; (iv) mixed grade 15 cancerous tissue; (v) a sub-grade cancerous tissue; (vi) healthy or normal tissue; or (vii) cancerous or abnormal tissue.

The first device may comprise a point of care ("POC"), diagnostic or surgical device.

- 20 The method may further comprise ionising at least some of the aerosol, smoke or vapour so as to generate analyte ions.

The method may further comprise directing or aspirating at least some of the aerosol, smoke or vapour into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer.

- 25 The method may further comprise ionising at least some the aerosol, smoke or vapour within a or the vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

- 30 The method may further comprise causing the aerosol, smoke or vapour to impact upon a collision surface located within a vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

The method may further comprise mass analysing the analyte ions in order to obtain mass spectrometric data and/or ion mobility data.

- 35 Various embodiments are contemplated wherein analyte ions generated by an ambient ionisation ion source are then subjected either to: (i) mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser; (ii) ion mobility analysis (IMS) and/or differential ion mobility analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis; and/or (iii) a combination of firstly ion mobility analysis (IMS) and/or differential ion mobility 40 analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis followed by secondly mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser (or vice versa). Various embodiments

also relate to an ion mobility spectrometer and/or mass analyser and a method of ion mobility spectrometry and/or method of mass analysis.

The method may further comprise mass analysing and/or ion mobility analysing the aerosol, smoke or vapour or ions derived from the aerosol, smoke or vapour in order to obtain mass spectrometric data and/or ion mobility data.

The method may further comprise analysing the mass spectrometric data and/or ion mobility data in order either: (i) to distinguish between healthy and diseased tissue; (ii) to distinguish between potentially cancerous and non-cancerous tissue; (iii) to distinguish between different types or grades of cancerous tissue; (iv) to distinguish between different types or classes of target material; (v) to determine whether or not one or more desired or undesired substances are present in the target; (vi) to confirm the identity or authenticity of the target; (vii) to determine whether or not one or more impurities, illegal substances or undesired substances are present in the target; (viii) to determine whether a human or animal patient may be at an increased risk of suffering an adverse outcome; (ix) to make or assist in the making a diagnosis or prognosis; and (x) to inform a surgeon, nurse, medic or robot of a medical, surgical or diagnostic outcome.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise supervised analysis of the one or more sample spectra and/or unsupervised analysis of the one or more sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise using one or more of: univariate analysis; multivariate analysis; principal component analysis (PCA); linear discriminant analysis (LDA); maximum margin criteria (MMC); library-based analysis; soft independent modelling of class analogy (SIMCA); factor analysis (FA); recursive partitioning (decision trees); random forests; independent component analysis (ICA); partial least squares discriminant analysis (PLS-DA); orthogonal (partial least squares) projections to latent structures (OPLS); OPLS discriminant analysis (OPLS-DA); support vector machines (SVM); (artificial) neural networks; multilayer perceptron; radial basis function (RBF) networks; Bayesian analysis; cluster analysis; a kernelized method; and subspace discriminant analysis.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise developing a classification model or library using one or more reference sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise performing linear discriminant analysis (LDA) after performing principal component analysis (PCA).

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise performing a maximum margin criteria (MMC) process after performing principal component analysis (PCA).

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise defining one or more classes within a classification model or library.

5 Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise defining one or more classes within a classification model or library manually or automatically according to one or more class or cluster criteria.

10 The one or more class or cluster criteria for each class may be based on one or more of: a distance between one or more pairs of reference points for reference sample spectra within a model space; a variance value between groups of reference points for reference sample spectra within a model space; and a variance value within a group of reference points for reference sample spectra within a model space.

The one or more classes may each be defined by one or more class definitions.

15 The one or more class definitions may comprise one or more of: a set of one or more reference points for reference sample spectra, values, boundaries, lines, planes, hyperplanes, variances, volumes, Voronoi cells, and/or positions, within a model space; and one or more positions within a class hierarchy.

20 Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise using a classification model or library to classify one or more unknown sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise classifying one or more sample spectra manually or automatically according to one or more classification criteria.

25 The one or more classification criteria may comprise one or more of:

30 a distance between one or more projected sample points for one or more sample spectra within a model space and a set of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, volumes, Voronoi cells, or positions, within the model space being below a distance threshold or being the lowest such distance;

a position for one or more projected sample points for one or more sample spectra within a model space being one side or other of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, or positions, within the model space;

35 a position for one or more projected sample points for one or more sample spectra within a model space being within one or more volumes or Voronoi cells within the model space; and

a probability or classification score being above a probability or classification score threshold or being the highest such probability or classification score.

40 The step of analysing the mass spectrometric data and/or ion mobility data may further comprise analysing a profile of the aerosol, smoke or vapour or a profile of ions derived from the aerosol, smoke or vapour.

The profile may be selected from the group consisting of: (i) a lipidomic profile; (ii) a fatty acid profile; (iii) a phospholipid profile; (iv) a phosphatidic acid (PA) profile; (v) a phosphatidylethanolamine (PE) profile; (vi) a phosphatidylglycerol (PG) profile; (vii) a phosphatidylserines (PS) profile; (viii) a phosphatidylinositol (PI) profile; or (ix) a triglyceride (TG) profile.

The method may further comprise using one or more thermal or temperature sensors, detectors or devices to obtain the image or other data.

The one or more thermal or temperature sensors, detectors or devices may be selected from the group consisting of: (i) one or more temperature sensors; (ii) one or more thermal imaging sensors; (iii) one or more infrared thermography ("IRT") sensors; and (iv) one or more infrared imaging sensors.

The method may further comprise using the one or more thermal or temperature sensors, detectors or devices to obtain the image or other data with or without the one or more thermal or temperature sensors, detectors or devices physically contacting the target.

The method may further comprise determining a temperature, temperature profile or thermographic image of one or more regions of the target.

The step of using the image or other data to determine one or more regions of interest of the target may comprise determining one or more regions of the target which have a different temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The step of using the image or other data to determine one or more regions of interest of the target may comprise determining whether or not a region of the target has a higher or lower temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The step of using the image or other data to determine one or more regions of interest of the target may further comprise determining one or more hyperthermic or hypothermic regions of the target.

The method may further comprise using one or more microwave or RF sensors, detectors or devices to obtain the image or other data.

The one or more microwave or RF sensors, detectors or devices may comprise one or more microwave reflectrometry sensors, detectors or devices.

The method may further comprise physically contacting the target with the one or more microwave reflectrometry sensors.

The method may further comprise using the one or more microwave reflectrometry sensors to determine a fluid content of one or more regions of the target.

The step of using the image or other data to determine one or more regions of interest of the target may comprise determining one or more regions of the target

which have a different fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The step of using the image or other data to determine one or more regions of interest of the target may comprise determining whether or not a region of the target
5 has a higher or lower fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The method may further comprise using an optical coherence tomography ("OCT") device to obtain the image or other data.

The method may further comprise using a low coherence light source ("LCS"),
10 a super-luminescent diode ("SLD"), a swept source or tunable laser ("SS"), an ultra-short pulsed laser or a supercontinuum laser to illuminate the target.

The optical coherence tomography device may comprise an interferometer.

The method may further comprise using one or more computed tomography devices to obtain the image or other data.

15 The method may further comprise using a positron emission tomography ("PET") device to obtain the image or other data.

The method may further comprise using a magnetic resonance imaging ("MRI") device to obtain the image or other data.

The method may further comprise using one or more ultrasonic tomography
20 devices to obtain the image or other data.

The method may further comprise using one or more optical imaging sensors, detectors or devices to obtain the image or other data.

The method may further comprise using a continuous wave (CW) light source to illuminate the target.

25 The method may further comprise using a time domain photon migration (TDPM) imaging system to obtain the image or other data.

The method may further comprise using a frequency-domain photon migration (FDPM) imaging system to obtain the image or other data.

The method may further comprise using one or more contrast agents to
30 enhance the image data.

The one or more contrast agents may comprise one or more fluorescent contrast agents.

The one or more contrast agents may comprise one or more visible dyes.

The one or more contrast agents may comprise one or more radiocontrast
35 agents.

The one or more contrast agents may comprise one or more optical, near infrared ("NIR"), fluorescent, autofluorescent or diagnostic contrast agents.

The one or more contrast agents may be selected from the group consisting of: (i) indocyanine green ("ICG") and derivatives or conjugates of indocyanine green
40 including indotricarbocyanine; (ii) diethylthiatricarbocyanine iodide ("DTTCI") and derivatives or conjugates of diethylthiatricarbocyanine iodide; (iii) rhodamine B and derivatives or conjugates of rhodamine B; (iv) photodynamic therapy ("PDT") agents

including hexylpyropheophorbide ("HPPH"); (v) a cyanine dye including Cy 5.5 dyes; and (vi) bifunctional contrast agents.

The one or more contrast agents may comprise nanoparticles.

5 The one or more contrast agents may comprise: (i) magnetic or ferromagnetic nanoparticles; (ii) gold nanoparticles; (iii) metallic nanoparticles; (iv) functionalised nanoparticles; (v) nanospheres, nanorods, nanostars or nanoshells; (vi) levan nanoparticles; or (vii) copper, zinc, titanium, magnesium, alginate, alloy or silver nanoparticles.

The one or more contrast agents may be exogenous to the target.

10 Alternatively, the one or more contrast agents may be endogenous to the target.

The method may further comprise using an X-ray scattering device to obtain the image or other data.

The method may further comprise directing X-rays onto one or more regions of the target.

15 The method may further comprise measuring the wavelength or frequency of scattered X-rays from the target.

The X-ray scattering device may comprise a Compton X-ray scattering device.

20 The method may further comprise using the Compton X-ray scattering device to measure scattered signals due to incoherent X-ray scattering.

The X-rays may have an energy ≥ 50 keV.

The X-ray scattering device may, alternatively, comprise a Rayleigh X-ray scattering device.

25 The method may further comprise using the Rayleigh X-ray scattering device to measure scattered signals due to coherent X-ray scattering.

The X-rays may have an energy ≤ 30 keV.

30 The method may further comprise displaying the image or other data (or data derived from the image or other data) so as to assist a user to manually guide or direct one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device.

The step of displaying the image or other data or data derived from the image or other data may comprise using an indirect conversion detector.

35 The indirect conversion detector may be arranged to convert incident X-ray photons into optical photons and then to convert the optical photons into electrical charge.

The step of displaying the image or other data or data derived from the image data may comprise using a fluoroscopy device or a scintillator.

The scintillator may comprise a cesium iodide ("CsI") layer or a gadolinium oxysulfide ("GOS") layer.

40 The method may further comprise using one or more image intensifiers to intensify the image or other data or data derived from the image or other data for displaying to a user.

The step of displaying the image or other data or data derived from the image or other data may comprise using a direct conversion detector.

The direct conversion detector may comprise a photoconductor which converts incident X-ray photons directly into electrical charge.

5 The photoconductor may comprise amorphous selenium ("a-Se"), cadmium telluride ("CdTe"), lead oxide ("PbO") or silicon ("Si").

The method may further comprise manually, automatically or robotically guiding or directing one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device using a guidance system.

10 The guidance system may comprise a magnetic resonance imaging ("MRI") guidance system.

The guidance system may comprise an ultrasound or ultrasonic guidance system.

15 The ultrasound or ultrasonic guidance system may comprise an intraoperative ultrasound ("IOUS") guidance system.

The guidance system may comprise a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device.

The guidance system may comprise a radioguided occult lesion localization ("ROLL") guidance system.

20 The method may further comprise injecting a nuclear radiotracer at one or more target regions.

The nuclear radiotracer may comprise ^{99m}Tc .

25 The method may further comprise using a gamma ray detection probe to detect gamma rays emitted by the decay of the nuclear radiotracer thereby enabling the target region to be located and/or visualised.

The guidance system may comprise a radioactive seed localization ("RSL") system.

The method may further comprise inserting, injecting or implanting one or more radioactive seeds in the target.

30 The one or more radioactive seeds may comprise a titanium shell.

The titanium shell may house ^{125}I .

The method may further comprise using a gamma ray detection probe to detect gamma rays emitted by the decay of the radioactive seed thereby enabling a target region of interest to be located and/or visualised.

35 The guidance system may comprise a mammography guidance system.

The guidance system may comprise a computed tomography ("CT") guidance system.

The guidance system may comprise a positron emission tomography ("PET") guidance system.

40 The guidance system may comprise a radiographic guidance system.

The guidance system may comprise a magnetic or magnetism sensing guidance system or a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles.

5 The guidance system may comprise a guidance system for detecting nanoparticles.

The method may further comprise using the image or other data to determine the margins or bounds of one or more regions of interest of the target.

The one or more regions of interest may comprise cancerous biological tissue or a tumour.

10 The cancerous biological tissue or the tumour may comprise either: (i) grade I, grade II, grade III or grade IV cancerous tissue; (ii) metastatic cancerous tissue; (iii) mixed grade cancerous tissue; or (iv) a sub-grade cancerous tissue.

According to another aspect there is provided a method of ambient ionisation comprising a method as disclosed above.

15 According to another aspect there is provided a method of rapid evaporation ionization mass spectrometry ("REIMS") comprising a method as disclosed above.

According to another aspect there is provided a method of analysis comprising a method as disclosed above.

20 According to another aspect there is provided a method of surgery, diagnosis, therapy or medical treatment comprising a method as disclosed above.

According to another aspect there is provided a non-surgical, non-therapeutic method of mass spectrometry and/or method of ion mobility spectrometry comprising a method as disclosed above.

25 According to another aspect there is provided a method of mass spectrometry and/or method of ion mobility spectrometry comprising a method as disclosed above.

According to another aspect there is provided apparatus comprising:

a device arranged and adapted to obtain or acquire image or other data from one or more regions of a target;

30 a control system arranged and adapted to use the image or other data to determine one or more regions of interest of the target; and

a first device for generating aerosol, smoke or vapour from one or more regions of the target.

35 The image or other data may comprise data selected from the group consisting of: (i) thermal, temperature or thermographic image data; (ii) microwave image data; (iii) visual or optical image data; (iv) infra-red ("IR") image data; (v) radio-frequency ("RF") image data; (vi) X-ray image data; (vii) magnetic resonance imaging ("MRI") image data; (viii) ultrasonic or ultrasound image data; (ix) tomographic image data; (x) optical or other absorption data; (xi) optical or other scattering coefficient data; (xii) oxyhemoglobin or deoxyhemoglobin absorbance data; (xiii) near infrared (NIR) image data; or (xiv) magnetic data.

The first device may comprise or form part of an ambient ion or ionisation source (or other ionisation source) or the first device may generate aerosol, smoke or

vapour for subsequent ionisation by an ambient ion or ionisation source (or other ionisation source).

The target may comprise native or unmodified target material.

5 The native or unmodified target material may be unmodified by the addition of a matrix or reagent.

The first device may be arranged and adapted to generate aerosol, smoke or vapour from one or more regions of the target without the target requiring prior preparation.

10 The first device may comprise an ion source selected from the group consisting of: (i) a rapid evaporative ionisation mass spectrometry ("REIMS") ion source; (ii) a desorption electrospray ionisation ("DESI") ion source; (iii) a laser desorption ionisation ("LDI") ion source; (iv) a thermal desorption ion source; (v) a laser diode thermal desorption ("LDTD") ion source; (vi) a desorption electro-flow focusing ("DEFFI") ion source; (vii) a dielectric barrier discharge ("DBD") plasma ion source; (viii) an Atmospheric Solids Analysis may be Probe ("ASAP") ion source; (ix) an ultrasonic assisted spray ionisation ion source; (x) an easy ambient sonic-spray ionisation ("EASI") ion source; (xi) a desorption atmospheric pressure photoionisation ("DAPPI") ion source; (xii) a paperspray ("PS") ion source; (xiii) a jet desorption ionisation ("JeDI") ion source; (xiv) a touch spray ("TS") ion source; (xv) a nano-DESI ion source; (xvi) a laser ablation electrospray ("LAESI") ion source; (xvii) a direct analysis may be in real time ("DART") ion source; (xviii) a probe electrospray ionisation ("PESI") ion source; (xix) a solid-probe assisted electrospray ionisation ("SPA-ESI") ion source; (xx) a cavitron ultrasonic surgical aspirator ("CUSA") device; (xxi) a focussed or unfocussed ultrasonic ablation device; (xxii) a microwave resonance device; and (xxiii) a pulsed plasma RF dissection device.

25 The first device may be arranged and adapted to generate aerosol, smoke or vapour from one or more regions of the target by contacting the target with one or more electrodes.

30 The one or more electrodes may comprise: (i) a monopolar device, wherein the apparatus optionally further comprising a separate return electrode; (ii) a bipolar device; or (iii) a multi phase RF device, wherein the apparatus optionally further comprising a separate return electrode or electrodes.

The one or more electrodes may comprise a rapid evaporation ionization mass spectrometry ("REIMS") device.

35 The device may be provided which is arranged and adapted to apply an AC or RF voltage to the one or more electrodes in order to generate the aerosol, smoke or vapour.

40 The device for applying the AC or RF voltage to the one or more electrodes may be arranged to apply one or more pulses of the AC or RF voltage to the one or more electrodes.

Application of the AC or RF voltage to the one or more electrodes may cause heat to be dissipated into the target.

The first device may comprise a laser for irradiating the target.

The first device may be arranged and adapted to generate aerosol from one or more regions of the target by direct evaporation or vaporisation of target material from the target by Joule heating or diathermy.

5 The first device may be arranged and adapted to direct ultrasonic energy into the target.

The aerosol may comprise uncharged aqueous droplets optionally comprising cellular material.

10 At least 50%, 55%, 60%, 65%, 70%, 75%, 80%, 85%, 90% or 95% of the mass or matter generated by the first device and which forms the aerosol may be in the form of droplets.

The first device may be arranged and adapted to generate aerosol wherein the Sauter mean diameter ("SMD", d_{32}) of the aerosol may be in a range: (i) $< 5 \mu\text{m}$; (ii) $5\text{-}10 \mu\text{m}$; (iii) $10\text{-}15 \mu\text{m}$; (iv) $15\text{-}20 \mu\text{m}$; (v) $20\text{-}25 \mu\text{m}$; or (vi) $> 25 \mu\text{m}$.

15 The aerosol may traverse a flow region with a Reynolds number (Re) in the range: (i) < 2000 ; (ii) $2000\text{-}2500$; (iii) $2500\text{-}3000$; (iv) $3000\text{-}3500$; (v) $3500\text{-}4000$; or (vi) > 4000 .

Substantially at the point of generating the aerosol, the aerosol may comprise droplets having a Weber number (We) selected from the group consisting of: (i) < 50 ; 20 (ii) $50\text{-}100$; (iii) $100\text{-}150$; (iv) $150\text{-}200$; (v) $200\text{-}250$; (vi) $250\text{-}300$; (vii) $300\text{-}350$; (viii) $350\text{-}400$; (ix) $400\text{-}450$; (x) $450\text{-}500$; (xi) $500\text{-}550$; (xii) $550\text{-}600$; (xiii) $600\text{-}650$; (xiv) $650\text{-}700$; (xv) $700\text{-}750$; (xvi) $750\text{-}800$; (xvii) $800\text{-}850$; (xviii) $850\text{-}900$; (xix) $900\text{-}950$; (xx) $950\text{-}1000$; and (xxi) > 1000 .

Substantially at the point of generating the aerosol, the aerosol may comprise 25 droplets having a Stokes number (S_k) in the range: (i) $1\text{-}5$; (ii) $5\text{-}10$; (iii) $10\text{-}15$; (iv) $15\text{-}20$; (v) $20\text{-}25$; (vi) $25\text{-}30$; (vii) $30\text{-}35$; (viii) $35\text{-}40$; (ix) $40\text{-}45$; (x) $45\text{-}50$; and (xi) > 50 .

Substantially at the point of generating the aerosol, the aerosol may comprise droplets having a mean axial velocity selected from the group consisting of: (i) < 20 m/s; (ii) $20\text{-}30$ m/s; (iii) $30\text{-}40$ m/s; (iv) $40\text{-}50$ m/s; (v) $50\text{-}60$ m/s; (vi) $60\text{-}70$ m/s; (vii) 30 (viii) $70\text{-}80$ m/s; (ix) $80\text{-}90$ m/s; (x) $90\text{-}100$ m/s; (xi) $100\text{-}110$ m/s; (xii) $110\text{-}120$ m/s; (xiii) $120\text{-}130$ m/s; (xiv) $130\text{-}140$ m/s; (xv) $140\text{-}150$ m/s; and (xvi) > 150 m/s.

The target may comprise biological tissue, biological matter, a bacterial colony or a fungal colony.

35 The biological tissue may comprise human tissue or non-human animal tissue.

The biological tissue may comprise *in vivo* biological tissue.

The biological tissue may comprise *ex vivo* biological tissue.

The biological tissue may comprise *in vitro* biological tissue.

40 According to an embodiment one or more bacterial or fungal colonies may be subjected to imaging and image or other data may be acquired. The imaging process may, for example, comprise an optical imaging process, X-ray imaging or polarised light. One or more regions of interest may then be identified. For example,

according to an embodiment one or more phase change regions or borders of the one or more bacterial or fungal colonies may be identified. As a result of determining a phase change region or border a region of interest in the colony may be determined. The region of interest may then be analysed using an ambient ionisation ion source.

Yet further embodiments are contemplated wherein the target may more generally comprise an organic target including materials such as a plastic. The target may be imaged (e.g., using X-ray or microwave imaging) to identify regions of the target which exhibit a change of density or other property (e.g., in the plastic).

One or more regions of interest in the (e.g., plastic) organic target may then be identified and may then be subjected to analysis using an ambient ionisation ion source.

The biological tissue may comprise: (i) adrenal gland tissue, appendix tissue, bladder tissue, bone, bowel tissue, brain tissue, breast tissue, bronchi, coronal tissue, ear tissue, esophagus tissue, eye tissue, gall bladder tissue, genital tissue, heart tissue, hypothalamus tissue, kidney tissue, large intestine tissue, intestinal tissue, larynx tissue, liver tissue, lung tissue, lymph nodes, mouth tissue, nose tissue, pancreatic tissue, parathyroid gland tissue, pituitary gland tissue, prostate tissue, rectal tissue, salivary gland tissue, skeletal muscle tissue, skin tissue, small intestine tissue, spinal cord, spleen tissue, stomach tissue, thymus gland tissue, trachea tissue, thyroid tissue, ureter tissue, urethra tissue, soft and connective tissue, peritoneal tissue, blood vessel tissue and/or fat tissue; (ii) grade I, grade II, grade III or grade IV cancerous tissue; (iii) metastatic cancerous tissue; (iv) mixed grade cancerous tissue; (v) a sub-grade cancerous tissue; (vi) healthy or normal tissue; or (vii) cancerous or abnormal tissue.

The first device may comprise a point of care ("POC"), diagnostic or surgical device.

The apparatus may further comprise a device for ionising at least some of the aerosol, smoke or vapour so as to generate analyte ions.

A device may be arranged and adapted to direct or aspirate at least some of the aerosol, smoke or vapour into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer.

A device may be arranged and adapted to ionise at least some the aerosol, smoke or vapour within a or the vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

According to an embodiment a device is provided for causing the aerosol, smoke or vapour to impact upon a collision surface located within a vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

A mass analyser for mass analysing and/or ion mobility analyser for ion mobility analysing the analyte ions in order to obtain mass spectrometric data and/or ion mobility data may be provided.

The apparatus may further comprise a mass analyser and/or ion mobility analyser for mass analysing and/or ion mobility analysing the aerosol, smoke or vapour or ions derived from the aerosol, smoke or vapour in order to obtain mass spectrometric data and/or ion mobility data.

5 The mass analyser and/or ion mobility analyser may be arranged and adapted to analyse the mass spectrometric data and/or ion mobility data in order either: (i) to distinguish between healthy and diseased tissue; (ii) to distinguish between potentially cancerous and non-cancerous tissue; (iii) to distinguish between different types or grades of cancerous tissue; (iv) to distinguish between different
10 types or classes of target material; (v) to determine whether or not one or more desired or undesired substances are present in the target; (vi) to confirm the identity or authenticity of the target; (vii) to determine whether or not one or more impurities, illegal substances or undesired substances are present in the target; (viii) to
15 determine whether a human or animal patient is at an increased risk of suffering an adverse outcome; (ix) to make or assist in the making a diagnosis or prognosis; and (x) to inform a surgeon, nurse, medic or robot of a medical, surgical or diagnostic outcome.

 According to an embodiment a device may be arranged and adapted to analyse one or more sample spectra so as to classify an aerosol, smoke or vapour
20 sample.

 A device may be arranged and adapted to perform supervised analysis of the one or more sample spectra and/or unsupervised analysis of the one or more sample spectra.

 The device for analysing the one or more sample spectra so as to classify the
25 aerosol, smoke or vapour sample may use one or more of: univariate analysis; multivariate analysis; principal component analysis (PCA); linear discriminant analysis (LDA); maximum margin criteria (MMC); library-based analysis; soft independent modelling of class analogy (SIMCA); factor analysis (FA); recursive partitioning (decision trees); random forests; independent component analysis (ICA);
30 partial least squares discriminant analysis (PLS-DA); orthogonal (partial least squares) projections to latent structures (OPLS); OPLS discriminant analysis (OPLS-DA); support vector machines (SVM); (artificial) neural networks; multilayer perceptron; radial basis function (RBF) networks; Bayesian analysis; cluster analysis; a kernelized method; and subspace discriminant analysis.

35 The apparatus may further comprise a device which is arranged and adapted to develop a classification model or library using one or more reference sample spectra.

 The apparatus may further comprise a device for performing linear discriminant analysis (LDA) after performing principal component analysis (PCA).

40 The apparatus may further comprise a device for performing a maximum margin criteria (MMC) process after performing principal component analysis (PCA).

The apparatus may further comprise a device for defining one or more classes within a classification model or library.

5 The apparatus may further comprise a device for defining one or more classes within a classification model or library manually or automatically according to one or more class or cluster criteria.

The one or more class or cluster criteria for each class may be based on one or more of: a distance between one or more pairs of reference points for reference sample spectra within a model space; a variance value between groups of reference points for reference sample spectra within a model space; and a variance value
10 within a group of reference points for reference sample spectra within a model space.

The one or more classes may each be defined by one or more class definitions.

The one or more class definitions may comprise one or more of: a set of one or more reference points for reference sample spectra, values, boundaries, lines,
15 planes, hyperplanes, variances, volumes, Voronoi cells, and/or positions, within a model space; and one or more positions within a class hierarchy.

The apparatus may further comprise device which is arranged and adapted to use a classification model or library to classify one or more unknown sample spectra.

20 The apparatus may further comprise a device for classifying one or more sample spectra manually or automatically according to one or more classification criteria.

The one or more classification criteria may comprise one or more of:

a distance between one or more projected sample points for one or more sample spectra within a model space and a set of one or more reference points for
25 one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, volumes, Voronoi cells, or positions, within the model space being below a distance threshold or being the lowest such distance;

a position for one or more projected sample points for one or more sample spectra within a model space being one side or other of one or more reference points
30 for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, or positions, within the model space;

a position for one or more projected sample points for one or more sample spectra within a model space being within one or more volumes or Voronoi cells within the model space; and

35 a probability or classification score being above a probability or classification score threshold or being the highest such probability or classification score.

The apparatus may further comprise a device for analysing a profile of the aerosol, smoke or vapour or a profile of ions derived from the aerosol, smoke or vapour.

40 The profile may be selected from the group consisting of: (i) a lipidomic profile; (ii) a fatty acid profile; (iii) a phospholipid profile; (iv) a phosphatidic acid (PA) profile; (v) a phosphatidylethanolamine (PE) profile; (vi) a phosphatidylglycerol (PG)

profile; (vii) a phosphatidylserines (PS) profile; (viii) a phosphatidylinositol (PI) profile; or (ix) a triglyceride (TG) profile.

The apparatus may further comprise one or more thermal or temperature sensors, detectors or devices for obtaining the image or other data.

5 The one or more thermal or temperature sensors, detectors or devices may be selected from the group consisting of: (i) one or more temperature sensors; (ii) one or more thermal imaging sensors; (iii) one or more infrared thermography ("IRT") sensors; and (iv) one or more infrared imaging sensors.

10 The one or more thermal or temperature sensors, detectors or devices may be arranged to obtain the image or other data with or without the one or more thermal or temperature sensors, detectors or devices physically contacting the target.

The apparatus may further comprise a device for determining a temperature, temperature profile or thermographic image of one or more regions of the target.

15 The apparatus may further comprise a device for determining one or more regions of the target which have a different temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

20 The apparatus may further comprise a device for determining whether or not a region of the target has a higher or lower temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The apparatus may further comprise a device for determining one or more hyperthermic or hypothermic regions of the target.

25 The apparatus may further comprise one or more microwave or RF sensors, detectors or devices for obtaining the image or other data.

The one or more microwave or RF sensors, detectors or devices may comprise one or more microwave reflectrometry sensors, detectors or devices.

The one or more microwave reflectrometry sensors may be arranged and adapted to physically contact the target.

30 The apparatus may further comprise one or more microwave reflectrometry sensors for determining a fluid content of one or more regions of the target.

35 The apparatus may further comprise a device for determining one or more regions of the target which have a different fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

The apparatus may further comprise a device for determining whether or not a region of the target has a higher or lower fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

40 The apparatus may further comprise an optical coherence tomography ("OCT") device for obtaining the image or other data.

The apparatus may further comprise a low coherence light source ("LCS"), a super-luminescent diode ("SLD"), a swept source or tunable laser ("SS"), an ultra-short pulsed laser or a supercontinuum laser for illuminating the target.

The optical coherence tomography device may comprise an interferometer.

5 The apparatus may further comprise one or more computed tomography devices for obtaining the image or other data.

The apparatus may further comprise a positron emission tomography ("PET") device for obtaining the image or other data.

10 The apparatus may further comprise a magnetic resonance imaging ("MRI") device for obtaining the image or other data.

The apparatus may further comprise one or more ultrasonic tomography devices for obtaining the image or other data.

The apparatus may further comprise one or more optical imaging sensors, detectors or devices for obtaining the image or other data.

15 The apparatus may further comprise a continuous wave (CW) light source for illuminating the target.

The apparatus may further comprise a time domain photon migration (TDPM) imaging system to obtain the image or other data.

20 The apparatus may further comprise a frequency-domain photon migration (FDPM) imaging system for obtaining the image or other data.

The apparatus may further comprise one or more contrast agents for enhancing the image data.

The one or more contrast agents may comprise one or more fluorescent contrast agents.

25 The one or more contrast agents may comprise one or more visible dyes.

The one or more contrast agents may comprise one or more radiocontrast agents.

The one or more contrast agents may comprise one or more optical, near infrared ("NIR"), fluorescent, autofluorescent or diagnostic contrast agents.

30 The one or more contrast agents may be selected from the group consisting of: (i) indocyanine green ("ICG") and derivatives or conjugates of indocyanine green including indotricarbocyanine; (ii) diethylthiatricarbocyanine iodide ("DTTCI") and derivatives or conjugates of diethylthiatricarbocyanine iodide; (iii) rhodamine B and derivatives or conjugates of rhodamine B; (iv) photodynamic therapy ("PDT") agents
35 including hexylpyropheophorbide ("HPPH"); (v) a cyanine dye including Cy 5.5 dyes; and (vi) bifunctional contrast agents.

The one or more contrast agents may comprise nanoparticles.

40 The one or more contrast agents may comprise: (i) magnetic or ferromagnetic nanoparticles; (ii) gold nanoparticles; (iii) metallic nanoparticles; (iv) functionalised nanoparticles; (v) nanospheres, nanorods, nanostars or nanoshells; (vi) levan nanoparticles; or (vii) copper, zinc, titanium, magnesium, alginate, alloy or silver nanoparticles.

The one or more contrast agents may be exogenous to the target.

Alternatively, the one or more contrast agents may be endogenous to the target.

The apparatus may further comprise an X-ray scattering device for obtaining the image or other data.

5 The apparatus may further comprise a device for directing X-rays onto one or more regions of the target.

The apparatus may further comprise a device for measuring the wavelength or frequency of scattered X-rays from the target.

10 The X-ray scattering device may comprise a Compton X-ray scattering device.

The Compton X-ray scattering device may be arranged to measure scattered signals due to incoherent X-ray scattering.

The X-rays may have an energy ≥ 50 keV.

The X-ray scattering device may comprise a Rayleigh X-ray scattering device.

15 The Rayleigh X-ray scattering device may be arranged to measure scattered signals due to coherent X-ray scattering.

The X-rays may have an energy ≤ 30 keV.

20 The apparatus may further comprise a device for displaying the image or other data or data derived from the image or other data so as to assist a user to manually guide or direct one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device.

The apparatus may further comprise an indirect conversion detector for displaying the image or other data or data derived from the image or other data.

25 The indirect conversion detector may be arranged and adapted to convert incident X-ray photons into optical photons and then convert the optical photons into electrical charge.

The apparatus may further comprise fluoroscopy device or a scintillator for displaying the image or other data or data derived from the image data.

30 The scintillator may comprise a cesium iodide ("CsI") layer or a gadolinium oxysulfide ("GOS") layer.

The apparatus may further comprise one or more image intensifiers for intensifying the image or other data or data derived from the image or other data for displaying to a user.

35 The apparatus may further comprise a direct conversion detector for displaying the image or other data or data derived from the image or other data.

The direct conversion detector may comprise a photoconductor which converts incident X-ray photons directly into electrical charge.

The photoconductor may comprise amorphous selenium ("a-Se"), cadmium telluride ("CdTe"), lead oxide ("PbO") or silicon ("Si").

40 The apparatus may further comprise a guidance system for manually, automatically or robotically guiding or directing one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device using.

The guidance system may comprise a magnetic resonance imaging ("MRI") guidance system.

The guidance system may comprise an ultrasound or ultrasonic guidance system.

5 The ultrasound or ultrasonic guidance system may comprise an intraoperative ultrasound ("IOUS") guidance system.

The guidance system may comprise a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device.

10 The guidance system may comprise a radioguided occult lesion localization ("ROLL") guidance system.

The apparatus may further comprise a device for injecting a nuclear radiotracer at one or more target regions.

The nuclear radiotracer may comprise ^{99m}Tc .

15 The apparatus may further comprise a gamma ray detection probe for detecting gamma rays emitted by the decay of the nuclear radiotracer thereby enabling the target region to be located and/or visualised.

The guidance system may comprise radioactive seed localization ("RSL") system.

20 The apparatus may further comprise a device for inserting, injecting or implanting one or more radioactive seeds into the target.

The one or more radioactive seeds may comprise a titanium shell.

The titanium shell may house ^{125}I .

25 The apparatus may further comprise a gamma ray detection probe for detecting gamma rays emitted by the decay of the radioactive seed thereby enabling a target region of interest to be located and/or visualised.

The guidance system may comprise a mammography guidance system.

The guidance system may comprise a computed tomography ("CT") guidance system.

30 The guidance system may comprise a positron emission tomography ("PET") guidance system.

The guidance system may comprise a radiographic guidance system.

The guidance system may comprise a magnetic or magnetism sensing guidance system or a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles.

35 The guidance system may comprise a guidance system for detecting nanoparticles.

The apparatus may further comprise a device for using the image or other data to determine the margins or bounds of one or more regions of interest of the target.

40 The one or more regions of interest may comprise cancerous biological tissue or a tumour.

The cancerous biological tissue or the tumour may comprise either: (i) grade I, grade II, grade III or grade IV cancerous tissue; (ii) metastatic cancerous tissue; (iii) mixed grade cancerous tissue; or (iv) a sub-grade cancerous tissue.

5 According to another aspect there is provided an ambient ionisation ion source comprising apparatus as disclosed above.

According to another aspect there is provided a rapid evaporative ionization mass spectrometry ("REIMS") ion source comprising apparatus as disclosed above.

According to another aspect there is provided a method comprising:

10 using a navigational device or system to guide or direct a first device to one or more regions of a target; and

using the first device to generate aerosol, smoke or vapour from one or more regions of the target.

The navigational device may be selected from the group consisting of: (i) a magnetic resonance imaging ("MRI") navigational device; (ii) an ultrasound or
15 ultrasonic navigational device; (iii) an X-ray navigational device; (iv) a radioactivity detecting navigational device for detecting radioactive particles or radioactive nanoparticles; (v) an intraoperative ultrasound ("IOUS") guidance system; (vi) a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device; (vii) a radioguided occult lesion localization ("ROLL") guidance
20 system; (viii) a radioactive seed localization ("RSL") system; (ix) a mammography guidance system; (x) a computed tomography ("CT") guidance system; (xi) a positron emission tomography ("PET") guidance system; (xii) a radiographic guidance system; (xiii) a magnetic or magnetism sensing guidance system; and (xiv) a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic
25 particles or magnetic nanoparticles.

The method may further comprise manually operating or guiding the navigational device or system.

The method may further comprise robotically or automatically operating or guiding the navigational device or system.

30 According to another aspect there is provided a method of mass spectrometry and/or method of ion mobility spectrometry comprising a method as disclosed above.

According to another aspect there is provided apparatus comprising:

a first device for generating aerosol, smoke or vapour from one or more regions of a target; and

35 a navigational device or system arranged and adapted to guide or direct the first device to one or more regions of the target.

The navigational device may be selected from the group consisting of: (i) a magnetic resonance imaging ("MRI") navigational device; (ii) an ultrasound or
40 ultrasonic navigational device; (iii) an X-ray navigational device; (iv) a radioactivity detecting navigational device for detecting radioactive particles or radioactive nanoparticles; (v) an intraoperative ultrasound ("IOUS") guidance system; (vi) a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization

(“WGL”) device; (vii) a radioguided occult lesion localization (“ROLL”) guidance system; (viii) a radioactive seed localization (“RSL”) system; (ix) a mammography guidance system; (x) a computed tomography (“CT”) guidance system; (xi) a positron emission tomography (“PET”) guidance system; (xii) a radiographic guidance system; (xiii) a magnetic or magnetism sensing guidance system; (xiv) a superconducting quantum interference device (“SQUID”) guidance system for detecting magnetic particles or magnetic nanoparticles; and (xv) a guidance system for detecting nanoparticles.

The navigational device or system may be manually operated or guided.

The apparatus may further comprise a robotic or automatic guidance system for robotically or automatically operating or guiding the navigational device or system.

According to another aspect there is provided a mass spectrometry system comprising apparatus as disclosed above in combination with a mass spectrometer and/or ion mobility spectrometer.

Analysing the spectrometric data and/or ion mobility data may comprise analysing one or more sample spectra so as to classify an aerosol, smoke or vapour sample.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise supervised analysis of the one or more sample spectra and/or unsupervised analysis of the one or more sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise using one or more of: univariate analysis; multivariate analysis; principal component analysis (PCA); linear discriminant analysis (LDA); maximum margin criteria (MMC); library-based analysis; soft independent modelling of class analogy (SIMCA); factor analysis (FA); recursive partitioning (decision trees); random forests; independent component analysis (ICA); partial least squares discriminant analysis (PLS-DA); orthogonal (partial least squares) projections to latent structures (OPLS); OPLS discriminant analysis (OPLS-DA); support vector machines (SVM); (artificial) neural networks; multilayer perceptron; radial basis function (RBF) networks; Bayesian analysis; cluster analysis; a kernelized method; and subspace discriminant analysis.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise developing a classification model or library using one or more reference sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise performing linear discriminant analysis (LDA) after performing principal component analysis (PCA).

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise performing a maximum margin criteria (MMC) process after performing principal component analysis (PCA).

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise defining one or more classes within a classification model or library.

5 Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise defining one or more classes within a classification model or library manually or automatically according to one or more class or cluster criteria.

10 The one or more class or cluster criteria for each class may be based on one or more of: a distance between one or more pairs of reference points for reference sample spectra within a model space; a variance value between groups of reference points for reference sample spectra within a model space; and a variance value within a group of reference points for reference sample spectra within a model space.

The one or more classes may each be defined by one or more class definitions.

15 The one or more class definitions may comprise one or more of: a set of one or more reference points for reference sample spectra, values, boundaries, lines, planes, hyperplanes, variances, volumes, Voronoi cells, and/or positions, within a model space; and one or more positions within a class hierarchy.

20 Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise using a classification model or library to classify one or more unknown sample spectra.

Analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample may comprise classifying one or more sample spectra manually or automatically according to one or more classification criteria.

25 The one or more classification criteria may comprise one or more of:

30 a distance between one or more projected sample points for one or more sample spectra within a model space and a set of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, volumes, Voronoi cells, or positions, within the model space being below a distance threshold or being the lowest such distance;

a position for one or more projected sample points for one or more sample spectra within a model space being one side or other of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, or positions, within the model space;

35 a position for one or more projected sample points for one or more sample spectra within a model space being within one or more volumes or Voronoi cells within the model space; and

a probability or classification score being above a probability or classification score threshold or being the highest such probability or classification score.

40 Various embodiments are contemplated which relate to generating smoke, aerosol or vapour from a target (details of which are provided elsewhere herein) using an ambient ionisation ion source. The aerosol, smoke or vapour may then be

mixed with a matrix and aspirated into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer. The mixture may be caused to impact upon a collision surface causing the aerosol, smoke or vapour to be ionised by impact ionization which results in the generation of analyte ions. The resulting analyte ions (or fragment or product ions derived from the analyte ions) may then be mass analysed and/or ion mobility analysed and the resulting mass spectrometric data and/or ion mobility spectrometric data may be subjected to multivariate analysis or other mathematical treatment in order to determine one or more properties of the target in real time.

According to an embodiment the first device for generating aerosol, smoke or vapour from the target may comprise a tool which utilises an RF voltage, such as a continuous RF waveform.

Other embodiments are contemplated wherein the first device for generating aerosol, smoke or vapour from the target may comprise an argon plasma coagulation ("APC") device. An argon plasma coagulation device involves the use of a jet of ionised argon gas (plasma) that is directed through a probe. The probe may be passed through an endoscope. Argon plasma coagulation is essentially a non-contact process as the probe is placed at some distance from the target. Argon gas is emitted from the probe and is then ionized by a high voltage discharge (e.g., 6 kV). High-frequency electric current is then conducted through the jet of gas, resulting in coagulation of the target on the other end of the jet. The depth of coagulation is usually only a few millimetres.

The first device, surgical or electrosurgical tool, device or probe or other sampling device or probe disclosed in any of the aspects or embodiments herein may comprise a non-contact surgical device, such as one or more of a hydrosurgical device, a surgical water jet device, an argon plasma coagulation device, a hybrid argon plasma coagulation device, a water jet device and a laser device.

A non-contact surgical device may be defined as a surgical device arranged and adapted to dissect, fragment, liquefy, aspirate, fulgurate or otherwise disrupt biologic tissue without physically contacting the tissue. Examples include laser devices, hydrosurgical devices, argon plasma coagulation devices and hybrid argon plasma coagulation devices.

As the non-contact device may not make physical contact with the tissue, the procedure may be seen as relatively safe and can be used to treat delicate tissue having low intracellular bonds, such as skin or fat.

According to various embodiments the mass spectrometer and/or ion mobility spectrometer may obtain data in negative ion mode only, positive ion mode only, or in both positive and negative ion modes. Positive ion mode spectrometric data may be combined or concatenated with negative ion mode spectrometric data. Negative ion mode can provide particularly useful spectra for classifying aerosol, smoke or vapour samples, such as aerosol, smoke or vapour samples from targets comprising lipids.

Ion mobility spectrometric data may be obtained using different ion mobility drift gases, or dopants may be added to the drift gas to induce a change in drift time of one or more species. This data may then be combined or concatenated.

It will be apparent that the requirement to add a matrix or a reagent directly to a sample may prevent the ability to perform *in vivo* analysis of tissue and also, more generally, prevents the ability to provide a rapid simple analysis of target material.

According to other embodiments the ambient ionisation ion source may comprise an ultrasonic ablation ion source or a hybrid electrosurgical –ultrasonic ablation source that generates a liquid sample which is then aspirated as an aerosol. The ultrasonic ablation ion source may comprise a focused or unfocused ultrasound.

Optionally, the first device comprises or forms part of an ion source selected from the group consisting of: (i) a rapid evaporative ionisation mass spectrometry (“REIMS”) ion source; (ii) a desorption electrospray ionisation (“DESI”) ion source; (iii) a laser desorption ionisation (“LDI”) ion source; (iv) a thermal desorption ion source; (v) a laser diode thermal desorption (“LDTD”) ion source; (vi) a desorption electro-flow focusing (“DEFFI”) ion source; (vii) a dielectric barrier discharge (“DBD”) plasma ion source; (viii) an Atmospheric Solids Analysis Probe (“ASAP”) ion source; (ix) an ultrasonic assisted spray ionisation ion source; (x) an easy ambient sonic-spray ionisation (“EASI”) ion source; (xi) a desorption atmospheric pressure photoionisation (“DAPPI”) ion source; (xii) a paperspray (“PS”) ion source; (xiii) a jet desorption ionisation (“JeDI”) ion source; (xiv) a touch spray (“TS”) ion source; (xv) a nano-DESI ion source; (xvi) a laser ablation electrospray (“LAESI”) ion source; (xvii) a direct analysis in real time (“DART”) ion source; (xviii) a probe electrospray ionisation (“PESI”) ion source; (xix) a solid-probe assisted electrospray ionisation (“SPA-ESI”) ion source; (xx) a cavitron ultrasonic surgical aspirator (“CUSA”) device; (xxi) a hybrid CUSA-diathermy device; (xxii) a focussed or unfocused ultrasonic ablation device; (xxiii) a hybrid focussed or unfocused ultrasonic ablation and diathermy device; (xxiv) a microwave resonance device; (xxv) a pulsed plasma RF dissection device; (xxvi) an argon plasma coagulation device; (xxvii) a hybrid pulsed plasma RF dissection and argon plasma coagulation device; (xxviii) a hybrid pulsed plasma RF dissection and JeDI device; (xxix) a surgical water/saline jet device; (xxx) a hybrid electrosurgery and argon plasma coagulation device; and (xxxi) a hybrid argon plasma coagulation and water/saline jet device.

BRIEF DESCRIPTION OF THE DRAWINGS

Various embodiments will now be described, by way of example only, and with reference to the accompanying drawings in which:

Fig. 1 illustrates a method of rapid evaporative ionisation mass spectrometry (“REIMS”) wherein an RF voltage is applied to bipolar forceps resulting in the generation of an aerosol or surgical plume which is captured through an irrigation

port of the bipolar forceps and is then transferred to a mass spectrometer for ionisation and mass analysis;

Fig. 2 illustrates a general embodiment wherein one or more imaging sensors or detectors are used to obtain image data from a target (e.g. *in vivo* tissue) prior to or whilst activating a rapid evaporative ionisation mass spectrometry ("REIMS") ion source to *inter alia* analyse the target and to determine, for example, whether or not the tissue may be cancerous;

Fig. 3 shows a microwave reflectrometry sensor which may be used according to various embodiments in order to obtain imaging data;

Fig. 4 shows a method of analysis that comprises building a classification model according to various embodiments;

Fig. 5 shows a set of reference sample spectra obtained from two classes of known reference samples;

Fig. 6 shows a multivariate space having three dimensions defined by intensity axes, wherein the multivariate space comprises plural reference points, each reference point corresponding to a set of three peak intensity values derived from a reference sample spectrum;

Fig. 7 shows a general relationship between cumulative variance and number of components of a PCA model;

Fig. 8 shows a PCA space having two dimensions defined by principal component axes, wherein the PCA space comprises plural transformed reference points or scores, each transformed reference point or score corresponding to a reference point of Fig. 6;

Fig. 9 shows a PCA-LDA space having a single dimension or axis, wherein the LDA is performed based on the PCA space of Fig. 8, the PCA-LDA space comprising plural further transformed reference points or class scores, each further transformed reference point or class score corresponding to a transformed reference point or score of Fig. 8;

Fig. 10 shows a method of analysis that comprises using a classification model according to various embodiments;

Fig. 11 shows a sample spectrum obtained from an unknown sample;

Fig. 12 shows the PCA-LDA space of Fig. 9, wherein the PCA-LDA space further comprises a PCA-LDA projected sample point derived from the peak intensity values of the sample spectrum of Fig. 11;

Fig. 13 shows a method of analysis that comprises building a classification library according to various embodiments; and

Fig. 14 shows a method of analysis that comprises using a classification library according to various embodiments.

DETAILED DESCRIPTION

Various embodiments will now be described in more detail below which in general relate to obtaining imaging or other data from one or more regions of a target (e.g., *in vivo* tissue) and then generating an aerosol, surgical smoke or vapour from one or more regions of the target using an ambient ionisation ion source.

The aerosol, surgical smoke or vapour is then aspirated into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer and is caused to impact upon a collision surface causing the aerosol, smoke or vapour to be ionised by impact ionisation which results in the generation of analyte ions.

The resulting analyte ions (or fragment or product ions derived from the analyte ions) are then mass analysed and the resulting mass spectrometric data and/or ion mobility data may then be subjected to multivariate analysis in order to determine one or more properties of the target in real time.

For example, the multivariate analysis may enable a determination to be made as to whether or not a portion of tissue which is currently being resected is cancerous or not.

The use of imaging data enables tissue which is of potential concern to be identified either prior to and/or during a surgical procedure and enables a surgeon to have a greater confidence that all undesired or potentially cancerous tissue is both located and completely removed whilst at the same time ensuring that the minimum amount of healthy tissue is removed.

Ambient ionisation ion sources

According to various embodiments a device is used to generate an aerosol, smoke or vapour from one or more regions of a target (e.g., *in vivo* tissue). The device may comprise an ambient ionisation ion source which is characterised by the ability to generate analyte aerosol, smoke or vapour from a native or unmodified target. For example, other types of ionisation ion sources such as Matrix Assisted Laser Desorption Ionisation ("MALDI") ion sources require a matrix or reagent to be added to the sample prior to ionisation.

It will be apparent that the requirement to add a matrix or a reagent to a sample prevents the ability to perform *in vivo* analysis of tissue and also, more generally, prevents the ability to provide a rapid simple analysis of target material.

In contrast, therefore, ambient ionisation techniques are particularly advantageous since firstly they do not require the addition of a matrix or a reagent (and hence are suitable for the analysis of *in vivo* tissue) and since secondly they enable a rapid simple analysis of target material to be performed.

A number of different ambient ionisation techniques are known and are intended to fall within the scope of the present invention. As a matter of historical record, Desorption Electrospray Ionisation ("DESI") was the first ambient ionisation

technique to be developed and was disclosed in 2004. Since 2004, a number of other ambient ionisation techniques have been developed. These ambient ionisation techniques differ in their precise ionisation method but they share the same general capability of generating gas-phase ions directly from native (i.e. untreated or unmodified) samples. A particular advantage of the various ambient ionisation techniques which are intended to fall within the scope of the present invention is that the various ambient ionisation techniques do not require any prior sample preparation. As a result, the various ambient ionisation techniques enable both *in vivo* tissue and *ex vivo* tissue samples to be analysed without necessitating the time and expense of adding a matrix or reagent to the tissue sample or other target material.

A list of ambient ionisation techniques which are intended to fall within the scope of the present invention are given in the following table:

Acronym	Ionisation technique
DESI	Desorption electrospray ionization
DeSSI	Desorption sonic spray ionization
DAPPI	Desorption atmospheric pressure photoionization
EASI	Easy ambient sonic-spray ionization
JeDI	Jet desorption electrospray ionization
TM-DESI	Transmission mode desorption electrospray ionization
LMJ-SSP	Liquid microjunction-surface sampling probe
DICE	Desorption ionization by charge exchange
Nano-DESI	Nanospray desorption electrospray ionization
EADESI	Electrode-assisted desorption electrospray ionization
APTDCI	Atmospheric pressure thermal desorption chemical ionization
V-EASI	Venturi easy ambient sonic-spray ionization
AFAI	Air flow-assisted ionization
LESA	Liquid extraction surface analysis
PTC-ESI	Pipette tip column electrospray ionization
AFADESI	Air flow-assisted desorption electrospray ionization
DEFFI	Desorption electro-flow focusing ionization
ESTASI	Electrostatic spray ionization
PASIT	Plasma-based ambient sampling ionization

	transmission
DAPCI	Desorption atmospheric pressure chemical ionization
DART	Direct analysis in real time
ASAP	Atmospheric pressure solid analysis probe
APTDI	Atmospheric pressure thermal desorption ionization
PADI	Plasma assisted desorption ionization
DBDI	Dielectric barrier discharge ionization
FAPA	Flowing atmospheric pressure afterglow
HAPGDI	Helium atmospheric pressure glow discharge ionization
APGDDI	Atmospheric pressure glow discharge desorption ionization
LTP	Low temperature plasma
LS-APGD	Liquid sampling-atmospheric pressure glow discharge
MIPDI	Microwave induced plasma desorption ionization
MFGDP	Microfabricated glow discharge plasma
RoPPI	Robotic plasma probe ionization
PLASI	Plasma spray ionization
MALDESI	Matrix assisted laser desorption electrospray ionization
ELDI	Electrospray laser desorption ionization
LDTD	Laser diode thermal desorption
LAESI	Laser ablation electrospray ionization
CALDI	Charge assisted laser desorption ionization
LA-FAPA	Laser ablation flowing atmospheric pressure afterglow
LADESI	Laser assisted desorption electrospray ionization
LDESI	Laser desorption electrospray ionization
LEMS	Laser electrospray mass spectrometry
LSI	Laser spray ionization
IR-LAMICI	Infrared laser ablation metastable induced chemical ionization
LDSPI	Laser desorption spray post-ionization
PAMLDI	Plasma assisted multiwavelength laser desorption ionization
HALDI	High voltage-assisted laser desorption

	ionization
PALDI	Plasma assisted laser desorption ionization
ESSI	Extractive electrospray ionization
PESI	Probe electrospray ionization
ND-ESSI	Neutral desorption extractive electrospray ionization
PS	Paper spray
DIP-APCI	Direct inlet probe-atmospheric pressure chemical ionization
TS	Touch spray
Wooden-tip	Wooden-tip electrospray
CBS-SPME	Coated blade spray solid phase microextraction
TSI	Tissue spray ionization
RADIO	Radiofrequency acoustic desorption ionization
LIAD-ESI	Laser induced acoustic desorption electrospray ionization
SAWN	Surface acoustic wave nebulization
UASI	Ultrasonication-assisted spray ionization
SPA-nanoESI	Solid probe assisted nanoelectrospray ionization
PAUSI	Paper assisted ultrasonic spray ionization
DPESI	Direct probe electrospray ionization
ESA-Py	Electrospray assisted pyrolysis ionization
APPIS	Ambient pressure pyroelectric ion source
RASTIR	Remote analyte sampling transport and ionization relay
SACI	Surface activated chemical ionization
DEMI	Desorption electrospray metastable-induced ionization
REIMS	Rapid evaporative ionization mass spectrometry
SPAM	Single particle aerosol mass spectrometry
TDAMS	Thermal desorption-based ambient mass spectrometry
MAII	Matrix assisted inlet ionization
SAII	Solvent assisted inlet ionization
SwiFERR	Switched ferroelectric plasma ionizer
LPTD	Leidenfrost phenomenon assisted thermal desorption

According to an embodiment the ambient ionisation ion source may comprise a rapid evaporative ionisation mass spectrometry ("REIMS") ion source wherein a RF voltage is applied to one or more electrodes in order to generate an aerosol or plume of surgical smoke by Joule heating.

However, it will be appreciated that other ambient ion sources including those referred to above may also be utilised. For example, according to another embodiment the ambient ionisation ion source may comprise a laser ionisation ion source. According to an embodiment the laser ionisation ion source may comprise a mid-IR laser ablation ion source. For example, there are several lasers which emit radiation close to or at 2.94 μm which corresponds with the peak in the water absorption spectrum. According to various embodiments the ambient ionisation ion source may comprise a laser ablation ion source having a wavelength close to 2.94 μm on the basis of the high absorption coefficient of water at 2.94 μm . According to an embodiment the laser ablation ion source may comprise a Er:YAG laser which emits radiation at 2.94 μm .

Other embodiments are contemplated wherein a mid-infrared optical parametric oscillator ("OPO") may be used to produce a laser ablation ion source having a longer wavelength than 2.94 μm . For example, an Er:YAG pumped ZGP-OPO may be used to produce laser radiation having a wavelength of e.g. 6.1 μm , 6.45 μm or 6.73 μm . In some situations it may be advantageous to use a laser ablation ion source having a shorter or longer wavelength than 2.94 μm since only the surface layers will be ablated and less thermal damage may result. According to an embodiment a Co:MgF₂ laser may be used as a laser ablation ion source wherein the laser may be tuned from 1.75-2.5 μm . According to another embodiment an optical parametric oscillator ("OPO") system pumped by a Nd:YAG laser may be used to produce a laser ablation ion source having a wavelength between 2.9-3.1 μm . According to another embodiment a CO₂ laser having a wavelength of 10.6 μm may be used to generate the aerosol, smoke or vapour.

According to other embodiments the ambient ionisation ion source may comprise an ultrasonic ablation ion source which generates a liquid sample which is then aspirated as an aerosol. The ultrasonic ablation ion source may comprise a focused or unfocussed source.

According to an embodiment the first device for generating aerosol, smoke or vapour from one or more regions of a target may comprise an electrosurgical tool which utilises a continuous RF waveform. According to other embodiments a radiofrequency tissue dissection system may be used which is arranged to supply pulsed plasma RF energy to a tool. The tool may comprise, for example, a PlasmaBlade (RTM). Pulsed plasma RF tools operate at lower temperatures than conventional electrosurgical tools (e.g. 40-170 °C c.f. 200-350 °C) thereby reducing thermal injury depth. Pulsed waveforms and duty cycles may be used for both cut

and coagulation modes of operation by inducing electrical plasma along the cutting edge(s) of a thin insulated electrode.

Rapid evaporative ionisation mass spectrometry ("REIMS")

5

Fig. 1 illustrates a method of rapid evaporative ionisation mass spectrometry ("REIMS") wherein bipolar forceps 1 may be brought into contact with *in vivo* tissue 2 of a patient 3. In the example shown in Fig. 1, the bipolar forceps 1 may be brought into contact with brain tissue 2 of a patient 3 during the course of a surgical operation on the patient's brain. An RF voltage from an RF voltage generator 4 may be applied to the bipolar forceps 1 which causes localised Joule or diathermy heating of the tissue 2. As a result, an aerosol or surgical plume 5 is generated. The aerosol or surgical plume 5 may then be captured or otherwise aspirated through an irrigation port of the bipolar forceps 1. The irrigation port of the bipolar forceps 1 is therefore reutilised as an aspiration port. The aerosol or surgical plume 5 may then be passed from the irrigation (aspiration) port of the bipolar forceps 1 to tubing 6 (e.g. 1/8" or 3.2 mm diameter Teflon (RTM) tubing). The tubing 6 is arranged to transfer the aerosol or surgical plume 5 to an atmospheric pressure interface 7 of a mass spectrometer and/or ion mobility spectrometer 8.

20

According to various embodiments a matrix comprising an organic solvent such as isopropanol may be added to the aerosol or surgical plume 5 at the atmospheric pressure interface 7. The mixture of aerosol 3 and organic solvent may then be arranged to impact upon a collision surface within a vacuum chamber of the mass spectrometer and/or ion mobility spectrometer 8. According to one embodiment the collision surface may be heated. The aerosol is caused to ionise upon impacting the collision surface resulting in the generation of analyte ions. The ionisation efficiency of generating the analyte ions may be improved by the addition of the organic solvent. However, the addition of an organic solvent is not essential.

25

Analyte ions which are generated by causing the aerosol, smoke or vapour 5 to impact upon the collision surface are then passed through subsequent stages of the mass spectrometer and/or ion mobility spectrometer and are subjected to mass analysis (and/or ion mobility analysis) in a mass analyser (and/or ion mobility analyser). The mass analyser may, for example, comprise a quadrupole mass analyser or a Time of Flight mass analyser.

30

Fig. 2 illustrates a general embodiment wherein one or more imaging sensors 20 are used to obtain imaging data from a target 2 (e.g. *in vivo* tissue) prior to activating a rapid evaporative ionisation mass spectrometry ("REIMS") ion source 1 which *inter alia* samples tissue 2 and enables a determination to be made, for example, as to whether or not the issue is cancerous.

35

Other embodiments are contemplated wherein the target 2 may more generally comprise an organic target including materials such as plastics. The target 2 may be imaged (e.g. using X-ray imaging) to determine regions of density change

40

in the target 2. Regions of interest may then be identified and subjected to ambient ionisation analysis. For example, a determination may be made that one or more regions of a plastic target have a different density which may be indicative of an organic or other contaminant. The regions of interest may then be analysed and the potential contaminant identified.

According to various embodiments the one or more sensor devices 20 may be used to obtain imaging (or other closely related) data from the target (e.g. either *in vivo* or *ex vivo* biological tissue). The one or more imaging sensor devices 20 may be arranged, for example, to obtain from the target: (i) thermal, temperature or thermographic image data; (ii) microwave image data; (iii) visual or optical image data; (iv) infra-red ("IR") image data; (v) radio-frequency ("RF") image data; (vi) X-ray image data; (vii) magnetic resonance imaging ("MRI") image data; (viii) ultrasonic or ultrasound image data; (ix) tomographic image data; (x) optical or other absorption data; (xi) optical or other scattering coefficient data; (xii) oxyhemoglobin or deoxyhemoglobin absorbance data; (xiii) near infrared (NIR) image data; or (xiv) magnetic data.

A number of different embodiments are contemplated and will be described in more detail below wherein imaging (or other closely related) data is acquired from one or more imaging sensors or devices 20 and wherein the imaging data may then be used, for example, to guide a user (e.g. a surgeon) performing a surgical, diagnostic or other procedure utilising an ambient ionisation ion source to one or more regions of particular interest on a target (e.g. *in vivo* or *ex vivo* tissue).

By way of example only, the one or more imaging sensors or devices 20 may be utilised to determine regions of tissue of a patient which have a different thermal, temperature or thermographic profile, microwave profile, visual or optical profile, infra-red ("IR") profile, radio-frequency ("RF") profile, X-ray profile, magnetic resonance imaging profile, ultrasonic or ultrasound profile, tomographic profile, optical or other absorption profile, optical or other scattering coefficient profile, oxyhemoglobin or deoxyhemoglobin absorbance profile, near infrared (NIR) profile or magnetic profile compared to surrounding tissue. As will be appreciated, portions of tissue which have a different thermal, temperature or thermographic profile, microwave profile, visual or optical profile, infra-red ("IR") profile, radio-frequency ("RF") profile, X-ray profile, magnetic resonance imaging profile, ultrasonic or ultrasound profile, tomographic profile, optical or other absorption profile, optical or other scattering coefficient profile, oxyhemoglobin or deoxyhemoglobin absorbance profile, near infrared (NIR) profile or magnetic profile compared to surrounding tissue may comprise diseased or potentially cancerous tissue. It is known, for example, that potentially cancerous tissue may be denser than healthy tissue and may have a highly vascular nature. Accordingly, potentially cancerous tissue may have a different water content to that of surrounding healthy tissue, may have a higher or different temperature to that of healthy tissue and have different dielectric and physical properties to that of surrounding healthy tissue.

According to an embodiment the additional or confirmatory information provided by the one or more imaging sensors 20 may be used to help determine the margins or bounds of healthy, potentially cancerous, cancerous, potentially diseased or diseased biological tissue or the margins or bounds of a tumour.

5 The cancerous biological tissue or the tumour may comprise: (i) grade I, grade II, grade III or grade IV cancerous tissue; (ii) metastatic cancerous tissue; (iii) mixed grade cancerous tissue; or (iv) a sub-grade cancerous tissue.

 The one or more imaging sensors 20 may be used to help determine physical, chemical or other data and in particular may be used to determine the
10 margins or bounds between different types or grades of diseased or cancerous tissue.

 The different grades of cancerous tissue may be selected from the group consisting of: (i) grade I cancerous tissue; (ii) grade II cancerous tissue; (iii) grade III cancerous tissue; and (iv) grade IV cancerous tissue.

15 According to various embodiments a determination from the imaging or other data may be made to determine either: (i) one or more physical properties of the target; (ii) one or more chemical properties of the target; (iii) one or more physico-chemical properties of the target; or (iv) one or more mechanical properties of the target.

20

Optimised operational parameters of an ambient ionisation surgical or diagnostic tool may be programmed or set dependent upon data acquired from one or more imaging sensors

25 According to an embodiment one or more operational parameters of an ambient ionisation surgical or diagnostic tool may be arranged to vary or otherwise be optimised during a surgical or diagnostic procedure based upon the acquired physical or non-mass spectrometric data, chemical data, imaging data or other data.

 For example, according to an embodiment the energy dissipated into
30 surrounding tissue may be arranged to reduce as the surgical or diagnostic device approaches a vital organ.

 According to various embodiments one more operational parameters of an ambient ionisation ion source may be varied or controlled depending upon the specific type of tissue which is being probed. The type of tissue may be known in
35 advance or may be determined from imaging, chemical, physical or other data. For example, according to an embodiment if a tissue or tumour has a soft or gelatinous texture or the probe is in close proximity to a sensitive region of the body (e.g. the probe is in close proximity to important nerves) than the power and/or duty cycle of the ambient ionisation ion source may be reduced, varied or otherwise altered.

40 According to another embodiment, one or more operational parameters of an ambient ionisation surgical or other tool may be set based upon the acquired chemical, physical or imaging data. For example, one or more operational

parameters of an ambient ionisation surgical tool may be set based upon the type or grade of cancerous tissue identified by the one or more physical, chemical, imaging or other sensors or devices 20 or based upon the nature of the diseased tissue identified by the one or more physical, chemical, imaging or other sensors or devices 5 20.

Different operational parameters may be used depending upon whether operating upon healthy tissue, clearly cancerous tissue or at the cancer margin.

According to various embodiments the physical data, non-mass spectrometric data, chemical data, imaging data or other data may include spatial information and 10 hence the variation of tissue as a function of depth within an organ may be determined. Accordingly, previously acquired physical data, non-mass spectrometric data, chemical data, imaging data or other data may be used to set various operational parameters of an ambient ionisation surgical tool as the surgical tool moves deeper into (or out of) an organ or closer to (or away from) an organ or 15 specific tissue types.

Furthermore, various ionisation parameters may be varied as the ambient ionisation surgical tool moves deeper into (or out of) an organ or closer to (or away from) an organ or specific tissue types.

As the ambient ionisation surgical tool makes an initial cut into an organ one 20 or more ionisation parameters (e.g. the composition of a matrix added to the aerosol, smoke or vapour released from the tissue, the temperature of a ionisation collision surface, the voltage applied to an ionisation collision surface etc.) may be optimised for the surgical conditions (e.g. initial blood loss, tissue composition) experienced when cutting into the organ. As the ambient ionisation surgical tool moves deeper 25 into (or out of) the organ or closer to (or away from) an organ or specific tissue types the optimum ionisation parameters for the surgical tool may change reflecting e.g. a different degree of blood loss and a different composition of the tissue. Accordingly, one or more ionisation parameters (e.g. the composition of matrix added to aerosol, smoke or vapour released from the tissue, the temperature of a ionisation collision surface, the voltage applied to an ionisation collision surface etc.) may be arranged 30 also to change or vary in order to match the changing surgical conditions and optionally based upon the acquired chemical data.

Numerous different embodiments are contemplated wherein various operational parameters of a surgical device or diagnostic tool which incorporates an 35 ambient ionisation ion source (e.g. a rapid evaporative ionisation mass spectrometry ("REIMS") ion source) may be varied based upon the acquired physical non-mass spectrometric data, chemical data, imaging data or other data.

According to various embodiments an ion mode of the mass spectrometer and/or ion mobility spectrometer may be selected based upon chemical, physical, 40 imaging or other data taken or determined from the cutting site.

According to further embodiments one or more operational parameters of the mass spectrometer and/or ion mobility spectrometer may be changed or altered

based upon, subsequent to or during the process of making a diagnosis (e.g. of cancerous or healthy tissue). For example, one or more operational parameters may be changed upon confirmation. The one or more operational parameters which may be changed or optimised depending upon the stage of analysis (e.g. exploratory, diagnosis or confirmation) include optimisation of: (i) inlet conditions including inlet voltages, type and flow rate of optional matrix added to aerosol flow, Venturi suction etc.; (ii) fragmentation conditions for aerosol including flow rates and temperature of collision surface, heated coil parameters etc.; (iii) downstream ion optics including ion path; and (iv) mass analysis steps including selection of mass peak(s) for further diagnosis, performing MS/MS experiments, fragmenting analyte ions of interest and mass analysing subsequent daughter, fragment or product ions.

Thermal imaging

Intraoperative Thermal Imaging ("ITI") is an imaging technique which can be used to locate the margins of primary and metastatic tumours. For example, in the case of brain tumours there may be a temperature difference of $> 3^{\circ}\text{C}$ between a brain tumour core (having a temperature of e.g. 36.4°C) and surrounding normal tissue having a lower temperature of e.g. 33.1°C .

The temperature of human body tissue is influenced by a number of complex factors including the degree of vasculature. Tumours may be highly vascular in nature and hence may be detected by being hyperthermic i.e. having a higher temperature than that of surrounding tissue. It is known, for example, to use thermography as a simple and non-invasive method of screening for potential breast tumours.

Brain, corneal and ocular tumours and malignant melanomas may be detected on the basis of having a hyperthermic profile relative to surrounding normal tissue.

In some instances tumours may have a lower temperature than that of surrounding tissue and certain tumours may be hypothermic. Major factors which can contribute to hypothermia include: (i) low density in tumour microvessels; (ii) edema in surrounding tissues due to the growth of the tumour; (iii) lower metabolism; and (iv) tumour necrosis which can result in a reduction of tumour vasculature and metabolic activity.

Thermal or infrared emission from tissue may be absorbed by fluid or glass. Ideally, therefore, the surgical site should be dried to remove any fluids including blood prior to thermal imaging.

ITI is essentially a technology for determining the surface temperature of tissue and the technology has a low effective penetration into the body or the tissue.

One advantage of ITI is that it is non-invasive and can be used with patients who have an implant which prevents the use of intra-operative MRI.

Various embodiments are contemplated wherein thermal imaging data of a target (e.g. *in vivo* tissue) may be obtained and may be used in combination with an ambient ionisation ion source.

5 Total en bloc spondylectomy ("TES")

Conventionally, curettage or piecemeal excision has been the usual approach to vertebral tumours. This approach, however, can increase the risk of tumour cell contamination to the surrounding structures and residual tumour tissue at the site
10 due to the difficulty in demarcating tumour from healthy tissue. These contribute to incomplete resection of the tumour as well as high local recurrence rates of the spinal malignant tumour. To reduce local recurrence and to increase survival, a procedure known as total en bloc spondylectomy ("TES") may be used. In this method, the entire vertebra or vertebrae containing the malignant tumour are resected, together
15 with en bloc laminectomy, en bloc corpectomy, and bilateral pediculotomy using a T-saw through the posterior approach. Using this technique, it is possible to excise the tumour mass together with a wide or marginal margin.

Various embodiments are contemplated wherein an ambient ionisation surgical or diagnostic tool may be used to perform a total en bloc spondylectomy and
20 wherein, in particular, imaging data may first be obtained according to various embodiments in order to help determine one or more regions of vertebra which should be resected and in order to reduce the amount of healthy vertebra which is removed.

25 Infrared thermography

According to an embodiment an infrared thermal camera may be used to record the thermal profile of a target, surgical site or tissue. The camera may comprise, for example, an array of 340 x 240 pixels and may comprise an uncooled
30 micro-barometer Focal Plane Array ("FPA") detector which is arranged to provide a high spatial resolution (e.g. 7.5 to 13 μm). The detector may be arranged to have a thermal sensitivity of e.g. 0.06 $^{\circ}\text{C}$ at an ambient temperature of 30 $^{\circ}\text{C}$.

The resolution of a thermal imaging camera having 340 x 240 pixels is greater than the resolution of conventional magnetic resonance imaging ("MRI") which has a
35 resolution of 256 x 256 pixels.

Intraoperative Magnetic Resonance Imaging ("iMRI")

Intraoperative Magnetic Resonance Imaging ("iMRI") technology is known which provides surgeons with intraoperative image guidance during tumour resections as it provides various surgically relevant parameters such as the location of the tumor and its borders as well as vascular parameters.

According to various embodiments an intraoperative magnetic resonance imaging device may be used to acquire imaging data and may be used in conjunction with an ambient ionisation surgical or diagnostic tool.

NIR optical tomography of *in vivo* tissue

According to an embodiment a number of different NIR optical tomography techniques may be used in order to obtain imaging data. For example, according to various embodiments continuous wave ("CW"), time domain photon migration ("TDPM") and frequency domain photon migration ("FDPM") imaging techniques may be utilised in order to obtain imaging data.

Continuous wave imaging utilises a light source wherein the intensity of the light source is arranged to remain substantially constant with time. The light source may be focused onto the target which may comprise *in vivo* tissue. The time invariant distribution of light may then be detected at various positions on the target surface.

Regions of abnormal, diseased or potentially cancerous tissue may be detected by wavelength dependent light absorption properties and/or wavelength dependent light scattering properties. For example, cancerous tissue may have a higher vascular density and an increased number of larger nuclei. As a result, both the light absorption and scattering properties of the diseased tissue will be different from that of healthy tissue and hence the two different tissue types can be differentiated.

Continuous wave imaging sensors or devices have the advantage of being relatively simple and require just a light source and a basic detector.

Time domain photon migration ("TDPM") imaging is a more complex imaging technique which involves directing very short pulses of light (e.g. pulses having a duration of picoseconds or femtoseconds at full width half maximum (FWHM)) at the target surface.

The pulses of light will broaden as they pass through the tissue. A detector may be positioned to detect the pulse of light as it passes through the tissue and the point-spread function of the detected pulse of light may be determined.

In essence, the distribution of the times of flight of photons as detected using very fast photon counting techniques or a streak camera detector may be used to infer optical properties of the tissue.

Embodiments are contemplated wherein an optical system comprising a pulsed laser source, a streak camera detector or a single photon counting detection system may be provided. Other embodiments are also contemplated wherein time gating techniques may be used to determine the total number of photons that arrive at a detector within a certain period of time.

Other embodiments are contemplated wherein frequency domain photon migration ("FDPM") imaging techniques may be used, wherein the light intensity emitted from e.g. a laser diode or LED light source is sinusoidally modulated at frequencies of the order of 10 MHz to 1 GHz. The light propagates through tissue and is amplitude and phase-shifted relative to the source wave. The phase delay and amplitude attenuation relative to the intensity of the incident light may be detected at a point on the tissue surface some distance away from its source. The location, size and optical contrast of heterogeneities within a tissue volume may be determined.

According to various embodiments NIR absorption signatures for healthy and diseased tissue may be generated and which look in particular at the absorbance of optical light due to melanin, oxyhemoglobin, deoxyhemoglobin, water and fat.

Contrast agents and nanoparticles

The near-infrared ("NIR") may be used to interrogate tissues in combination with NIR excitable dyes or contrast agents.

Various embodiments are contemplated wherein endogenous or exogenous contrast agents may be used to enhance image data, physical data, chemical data or other data which may be acquired according to various embodiments.

A number of different contrast agents may be used to enhance image data, physical data, chemical data or other data which, for example, may fluorescence when illuminated with infrared radiation having a wavelength in the range 700-900 nm. The wavelength range 700-900 nm may be considered to comprise a therapeutic window since *in vivo* tissue exhibits a low absorbance in this wavelength range. Absorption occurs primarily from tissue chromophores of oxy- and deoxyhemoglobin, fat, melanin and water.

It will be understood that the ability to detect potentially abnormal or diseased tissue by imaging, chemical, physical or other techniques depends principally upon there being a contrast between healthy and diseased tissue.

Alternatively, abnormal or diseased tissue can be differentiated from healthy tissue on the basis of the two different tissue types having different scattering properties.

Although the wavelength range 700-900 nm is of particular interest due to the low absorbance in this wavelength range, infrared radiation in this wavelength range can also exhibit a relatively high scattering coefficient.

Embodiments are contemplated wherein imaging data, chemical data, physical data or other data may be obtained by detecting differences in the scattering of infrared radiation within the wavelength range 700-900 nm between healthy and diseased tissue.

5 Embodiments are also contemplated wherein one or more exogenous contrast agents may be used to analyse *in vivo*, *ex vivo* or *in vitro* tissue samples, biological matter, organic matter (including plastics), one or more bacterial colonies or one or more fungal colonies. According to an embodiment one or more exogenous fluorescence contrast agents may be provided or added to the tissue in
10 order to augment endogenous contrast.

 The one or more contrast agents may comprise one or more fluorescent contrast agents.

 The one or more contrast agents may comprise one or more visible dyes.

 The one or more contrast agents may comprise one or more radiocontrast
15 agents.

 The one or more contrast agents may comprise one or more optical, near infrared ("NIR"), fluorescent, autofluorescent or diagnostic contrast agents.

 According to various embodiments the one or more contrast agents may be selected from the group consisting of: (i) indocyanine green ("ICG") and derivatives
20 or conjugates of indocyanine green including indotricarbocyanine; (ii) diethylthiatricarbocyanine iodide ("DTTCl") and derivatives or conjugates of diethylthiatricarbocyanine iodide; (iii) rhodamine B and derivatives or conjugates of rhodamine B; (iv) photodynamic therapy ("PDT") agents including hexylpyropheophorbide ("HPPH"); (v) a cyanine dye including Cy 5.5 dyes; and (vi)
25 bifunctional contrast agents.

 Indocyanine green ("ICG") is of particular interest since it has FDA approval for systemic administration. Indocyanine is excited at about 780 nm and emits at 830 nm. Indocyanine green will dissolve in blood and will bind to proteins such as albumin and lipoproteins. ICG is a nonspecific agent and is cleared rapidly from the
30 blood. However, ICG tends to collect in regions of dense vascularity through extravascation. ICG may be administered to a patient at a dose of 0.2 mg/kg intravenously. Derivatives and conjugates of ICG may also be used.

 Various embodiments are contemplated wherein ICG is excited using a 780 nm laser and fluorescent spectra at 830 nm are detected using a gain modulated
35 image intensified charge coupled camera (ICCD).

 Other embodiments are contemplated wherein magnetic nanoparticles ("MNPs") may be used as a contrast agent. The magnetic nanoparticles may comprise ferromagnetic iron oxide i.e. magnetite (Fe_3O_4) or maghemite ($\gamma\text{-Fe}_2\text{O}_3$) having a diameter in the range 1-100 nm. According to an embodiment the
40 nanoparticles may have a diameter in the range 1-10, 10-20, 20-30, 30-40, 40-50, 50-60, 60-70, 70-80, 80-90 or 90-100 nm. In particular, various embodiments are contemplated wherein nanoparticles having a core diameter in the range of 5-15 nm

may be used as contrast agents. In particular, as the size of the nanoparticles is reduced then the characteristics of the nanoparticles changes from having multi-domain ferromagnetic characteristics to having single domain characteristics and finally to having superparamagnetic characteristics. In particular, small nanoparticles having a diameter in the range 5-15 nm exhibit superparamagnetic properties having no hysteresis losses and will generate heat as a result of relaxational losses, mainly Néel relaxation loss. The inherent ferromagnetic properties of magnetic nanoparticles provides contrast enhancement with magnetic resonance ("MR") imaging. For example, accumulation of magnetic nanoparticles in brain tumours appears as a hypointensity on T2-weighted imaging including gradient echo imaging.

Magnetic nanoparticles may also be functionalised to target cancer cells thereby enabling cancerous tissue to be identified by magnetic resonance imaging.

According to an embodiment ultrasmall superparamagnetic iron oxide nanoparticles ("USPIONPs") may be used.

In addition to using nanoparticles to accumulate within cancerous tissue, according to further embodiments the nanoparticles may be heated by applying a magnetic field and in particular an alternating magnetic field ("AMF") which produces heat via relaxational loss via the Brownian Néel relaxation process or by hysteresis loss. As a result, potentially cancerous tissue can be identified on the basis of having an elevated or hyperthermic temperature relative to surrounding normal healthy tissue. Accordingly, thermal detection techniques in conjunction with the heating of nanoparticles which have accumulated in cancerous tissue may be used to visualise, image or target potentially cancerous tissue.

Further embodiments are contemplated wherein nanoparticles which have accumulated in cancerous tissue may be heated up to temperatures $> 40^{\circ}\text{C}$ in order to selectively target and kill cancerous cells. For example, heating cancerous cells to a temperature around 45°C can cause cancer cells to undergo apoptosis or necrosis. Furthermore, locally heating cancerous cells can increase the blood flow to the cancerous cells which can, for example, result in an improved delivery of chemotherapeutic agents to the cancerous cells. Also, cancer cells are more heat sensitive than normal tissue and so heat can be selectively applied to cancer cells in order to kill cancer cells without damaging surrounding normal or healthy tissue.

According to an embodiment the nanoparticles may comprise a polysiloxane matrix (Si) wherein chelating species such as diethylene triamine pentaacetic acid (DTPA) at the surface of the particles allows the complexation of metallic elements such as gadolinium (Gd), silicon (Si), calcium (Ca) and iron (Fe).

According to other embodiments the nanoparticles may be heated by radiofrequency capacitive heating wherein, for example, an alternating electrical current at 8 MHz may be applied and the temperature of tissues located between the electrodes increases. Magnetite cationic liposomes (MCLs) may be used and when injected into cancer cells the cancerous tissue may reach a temperature which is 2-3 $^{\circ}\text{C}$ above that of healthy tissue.

Other embodiments are contemplated wherein antibodies containing a ferromagnetic component may be used as a contrast agent.

The one or more contrast agents may be exogenous or endogenous to the target.

5 As is well known, fluorophores may be activated to an excited state by absorbing a photon and may then relax to a ground state in a non-radiative manner. Alternatively, the fluorophore may relax to the ground state in a radiative (fluorescence) manner. The fluorescence lifetime τ is equivalent to the mean time that a fluorophore remains in its activated state and the quantum efficiency is the
10 proportion of relaxations which occur radiatively.

Other mechanisms are known wherein the excited state can undergo intersystem crossing to an intermediate excited state wherein the spin state of the electron is flipped and the relaxation of the intermediate excited state is forbidden until the electron spin is reversed. The lifetimes of the intermediate excited state may
15 be of the order of microseconds to milliseconds and are termed phosphorescence.

Fluorescence radiative decay can be affected by pH, oxygenation, free ion concentrations, glucose and other analytes. Fluorescence can therefore provide an optical imaging ability which is not otherwise directly detectable.

According to an embodiment the fluorescence spectra of tissue may be
20 analysed in order to determine the pH, oxygenation level or quantum efficiency of the tissue.

Other embodiments are contemplated wherein gamma ray imaging may be performed and optionally a technetium-99 sulfur colloid may be injected into the target tissue for analysis.

25 According to various embodiments gold nanoparticles ("Au NPs" or "GNPs") may be used as contrast agents. Gold nanoparticles may be formed by a laser ablation method wherein a gold target in water is subjected to pulsed laser irradiation. Colloidal gold can also be prepared by citrate reduction. Various other physical methods of producing gold nanoparticles are known including inert gas
30 condensation, thermolysis of gold(I) complex, radiolysis of gold salts, photochemistry and sonochemistry. Chemical methods of producing gold nanoparticles are known including emulsification, reduction of gold ions in the presence of a dispersant, seed-mediated growth, use of reverse micelles and phase transfer reactions. Gold nanoparticles may also be biosynthesised by certain types of fungi including
35 *Fusarium oxysporum*, *Verticillium sp.* and *Colletotrichum sp.* Gold nanoparticles have also been synthesized within HEK-293, HeLa, SiHa and SKNSH cells.

Gold nanoparticles may be readily functionalised generally through thiol linkages to provide functionalised gold nanoparticles (fGNPs). The surface of gold nanoparticles may be functionalised with e.g. cyclodextrin as a drug pocket having
40 hydrophobic cavities, antibodies as a targeting moiety and poly(ethyleneglycol) (PEG) as an anti-fouling shell. Anti-cancer drugs may be encapsulated into the hydrophobic

cavity of the cyclodextrin and the gold nanoparticles may therefore be used as a drug delivery system (DDS).

According to various embodiments gold nanoparticles and in particular functionalised gold nanoparticles as described above may be used as contrast agents.

Gold nanoparticles cause local heating when irradiated with light (800-1200 nm) and hence gold nanoparticles may be used in the photothermal destruction of tumours according to various embodiments.

Plasmonic gold nanoparticles may be used for cancer diagnosis and photothermal therapy. Surface plasmon resonance ("SPR") leads to strong electromagnetic fields on the surface of gold nanoparticles which enhances all radiative properties such as absorption and scattering. In particular, Raman scattering is enhanced. Additionally, strongly absorbed light may be quickly converted to heat via a series of nonradiative processes.

Gold nanoparticles can be optically tuned by shape and structure and for example gold nanorods having different optical properties to gold nanospheres can be produced. The aspect ratio can be precisely controlled by changing experimental parameters in a seed-mediation growth method.

Gold nanoshells (comprising a silica core around 100 nm with a thin shell of gold a few nanometers thick) and gold nanocages may also be produced. Gold nanospheres, nanorods, nanostars and nanoshells may be used as contrast agents according to various embodiments.

According to an embodiment gold nanoparticles may be used for cancer imaging. It is known that gold nanoparticles scatter strongly and the scattering properties depend upon the size, shape and structure of the nanoparticles. According to an embodiment gold nanoparticles having a diameter 30-100 nm may be used. Such nanoparticles scatter intensely and can be detected using a microscope under dark field illumination conditions. The gold nanoparticles may be conjugated with, for example, anti-epidermal growth factor receptors (anti-EGFR) antibodies (or other antibodies) to recognise the EGFR proteins (or other proteins) of cancer cells and tissues. The regular or well organised scattering pattern of nanoparticles bound to cancer cells can be readily distinguished from the random distribution of nanoparticles around healthy cells and this difference in scattering pattern may be utilised according to various embodiments.

The nanoparticles may be excited by white light from a halogen lamp.

According to an embodiment, functionalised gold nanoparticles may be distributed across the surface of a target (such as biological *in vivo* or *ex vivo* tissue) and the gold nanoparticles may preferentially bind to cancerous cells. As a result, cancerous regions of tissue can be identified by illuminating the target and either analysing the scattering pattern or measuring the scattered intensity of light.

For example, gold nanoparticles may have a strong surface plasmon resonance ("SPR") around 540 nm on the cell monolayer with the result that the

nanoparticles scatter strongly in the green to yellow range of the visible spectrum. Similarly, gold nanorods may be constructed which exhibit a strong surface plasmon resonance ("SPR") around 800 nm giving an intense red colour.

Accordingly, gold nanoparticles may be used as imaging, physical or chemical contrast agents according to various embodiments.

Surface plasmon resonance ("SPR") effects also enhance the Raman scattering of adjacent molecules because the Raman intensity is directly proportional to the square of the field intensity imposed on the molecules. This phenomenon is termed as surface enhanced Raman scattering ("SERS").

According to an embodiment gold nanoparticles may be utilised in order to enhance Raman scattering of adjacent molecules. The gold nanoparticles may be either symmetric or asymmetric. According to an embodiment the gold nanoparticles may be asymmetric (e.g. nanorods) since asymmetric nanoparticles provide a larger Raman enhancement due to the lightening rod effect.

One particular advantage of using gold nanoparticles and surface enhance Raman scattering is that this approach greatly enhances detection sensitivity and decreases signal acquisition time.

According to another embodiment a Raman tag may be used as a spectroscopic imaging probe. The Raman tag may comprise organic dye molecules with aromatic structures which have relatively high Raman cross sections. Its fluorescence is quenched when they are adsorbed on to metallic nanoparticles and thus Raman signals are able to be detected.

The Raman tags may be physically adsorbed or chemically conjugated with both Raman tag and cancer targeting ligands.

According to other embodiments levan nanoparticles may be utilised for targeted cancer imaging. Levan is a biocompatible carbohydrate polymer that consists of β -D-fructofuranose attached by β -(2,6) linkages and is used in biomedical applications. According to an embodiment Indocyanine green (ICG) may be encapsulated in levan nanoparticles by self-assembly and the levan-ICG nanoparticles may be used for cancer imaging.

Various embodiments are contemplated wherein a target which may comprise biological tissue may be subjected to Raman or laser imaging (transmission or fluorescence) using nanoparticles such as gold nanoparticles are described above as contrast agents. One or more regions of interest may then be identified and the regions of interest may then be subjected to analysis using a first device to generate aerosol, smoke or vapour. The first device may comprise an ambient ionisation ion source such as a rapid evaporative ionisation mass spectrometry ("REIMS") ion source.

Other embodiments are contemplated wherein chemical tags (such as luminescent tags) may be used in combination with an ambient ionisation ion source such as a rapid evaporative ionisation mass spectrometry ("REIMS") ion source. For example, according to an embodiment a luminescent imaging, physical or chemical

contrast agent may be modified with the inclusion of a ligand that is readily ionisable by an ambient ionisation ion source such as a rapid evaporative ionisation mass spectrometry ("REIMS") ion source. The contrast agents, tags or nanoparticles may be detected by mass spectrometry if an undesired (or desired) target or undesired (or
5 desired) tissue is ablated. The tagging chemical may have fluorescent, magnetic, chemical, physical or other imaging properties and a part of the molecule may be arranged so as to ionise well for mass spectrometry analysis. For example, as described above, Indocyanine green (ICG) may be encapsulated into levan
10 nanoparticles or more generally in functionalised nanoshells which are functionalised so as to target cancerous tissue or other undesired target material. Embodiments are contemplated wherein ICG (or other chemicals) which may be encapsulated within functionalised nanoparticles or nanoshells (which may be functionalised so as to target cancerous tissue) may be detected by mass spectrometry. Other
15 embodiments are contemplated wherein one or more different markers other than ICG may be encapsulated into nanoparticles which target cancerous tissue. These one or more markers may then identified by mass spectrometry and a determination may be made that the tissue which is currently being analysed comprises cancerous tissue or otherwise comprises undesired target material.

Embodiments are contemplated wherein target experiments may be
20 performed wherein a target is subjected to mass spectrometry analysis with a view to seeking to identify portions of target or tissue which include (or conversely do not include) a contrast agent, chemical tag, marker or nanoparticle wherein the contrast agent, chemical tag, marker or nanoparticle has been functionalised so as to target a particular target e.g. cancerous tissue. According to various embodiment identifying
25 the presence of the contrast agent, chemical tag, marker or nanoparticle thereby enables a determination to be made that the target or tissue which is currently being analysed comprises cancerous tissue (or otherwise desired or undesired target material).

According to an embodiment the step of using physical or other non-mass
30 spectrometric data to determine one or more regions of interest may comprise the use of targeted nanoparticles containing or comprising a metal which is intended to change the electrical impedance of a targeted tissue type. As detailed above, metallic nanoparticles may be functionalised so that they adhere to specific types of tissue or other surfaces. One or more regions of interest of a target may be identified
35 by determining one or more regions of a target (e.g., tissue) having a different impedance to other target areas due to the presence of targeted or functionalised nanoparticles which preferentially adhere to certain specific target areas (e.g., cancerous tissue).

Photothermal therapy (PTT)

Gold nanoparticles absorb light much more strongly than organic dye molecules. Nearly 100% adsorbed light is converted to heat via nonradiative properties. Accordingly, gold nanoparticles may be used as photothermal contrast agents for photothermal therapy wherein photon energy is converted to heat sufficient to induce cellular damage via thermal effects such as hyperthermia, coagulation and evaporation.

Photothermal therapy may be performed using spherical gold nanoparticles in conjunction with either pulsed or continuous wave lasers.

Nanosecond pulsed lasers may be used in conjunction with PTT to provide highly selective and localised damage to cancer cells without affecting neighbouring healthy cells which may be only a few nanometers to tens of micrometers away.

For *in vivo* therapy of tumours under the skin or deeply seated tumours within tissue near infrared (NIR) light may be used because of its deep penetration ability due to minimal absorption by hemoglobin and water molecules.

According to an embodiment PEGylated gold nanoshells may be used in conjunction with an ambient ionisation ion source since the absorption of gold nanoshells can be tuned to the NIR region. A continuous wave (cw) diode laser e.g. emitting at 820 nm with an irradiance of e.g. 35 W/cm² for 4 mins may be used to illuminate the gold nanoshells in order to cause cancer cell death of targeted cells.

The gold nanoshells may according to various embodiments be injected into the blood stream of a patient or spread upon the surface of a target or tissue sample.

Other embodiments are contemplated wherein PTT may be performed using gold nanorods. According to an embodiment a cw Ti:Sapphire laser emitting at 800 nm may be used in conjunction with gold nanorods.

According to an embodiment the target may be illuminated with either linearly polarized light or circularly polarized light. Illuminating gold nanorods with circularly polarized light is particularly beneficial as the light absorption by gold nanorods is enhanced leading to an ultra-low energy threshold for cancer killing.

It has been determined that a laser fluence of 30 J/cm² can result in an increase in temperature of the cells by about 10 °C which is sufficient to induce heat-stress cell death. Accordingly, a laser fluence of 30 J/cm² may be utilised according to various embodiments.

According to an embodiment gold nanorods may be conjugated to methoxy-poly (ethylene-glycol)-thiol having an average MW 5,000 (mPEG-SH-5000) and may be injected into a patient either intravenously and/or subcutaneously. Tumours or cancerous cells can be identified using transmission imaging of a NIR laser with a camera due to the NIR light absorption by the nanorods in the tumour.

Intraoperative computer tomography ("CT"), intraoperative ultrasound and surgical guidance systems

5 According to an embodiment a mobile CT device may be used to acquire intraoperative images during a procedure such as a tumour resection.

According to another embodiment an intra-operative 3D ultrasound ("3D-iUS") guidance system may be used.

10 Various embodiments are contemplated wherein an ambient ionisation probe, surgical device or diagnostic device may be manually, automatically or robotically guided or directed using a guidance system.

The guidance system may comprise a magnetic resonance imaging ("MRI") guidance system or an ultrasound or ultrasonic guidance system such as an intraoperative ultrasound ("IOUS") guidance system.

15 Other embodiments are contemplated wherein the guidance system may comprise a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device.

According to another embodiment the guidance system may comprise a radioguided occult lesion localization ("ROLL") guidance system.

20 A yet further embodiment is contemplated wherein a nuclear radiotracer is injected or otherwise introduced into one or more regions of the target (e.g. tissue). The nuclear radiotracer may comprise ^{99m}Tc .

According to an embodiment a gamma ray detection probe may be used to detect gamma rays emitted by the decay of the nuclear radiotracer thereby enabling the target region to be located and/or visualised.

25 Other guidance system may be used including radioactive seed localization ("RSL") systems. For example, one or more radioactive seeds may be inserted or implanted into the target. Various different forms of radioactive seeds may be used including radioactive seeds having a titanium shell which optionally houses ^{125}I . A gamma ray detection probe may be used to detect gamma rays emitted by the decay of the radioactive seed thereby enabling a target region of interest to be located and/or visualised.

The guidance system may comprise a mammography guidance system.

35 According to other embodiments the guidance system may comprise a computed tomography ("CT") guidance system, a positron emission tomography ("PET") guidance system or a radiographic guidance system.

According to other embodiments the guidance system may comprise a magnetic or magnetism sensing guidance system or a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles or a guidance system for detecting nanoparticles.

Compton X-ray scattering

Other embodiments are contemplated wherein an X-ray scattering device may be used to obtain image or other data.

- 5 The method may comprise directing X-rays onto one or more regions of the target and measuring the wavelength or frequency of scattered X-rays from the target.

The X-ray scattering device may comprise a Compton X-ray scattering device which is arranged to measure scattered signals due to incoherent X-ray scattering.

- 10 The X-rays may have an energy ≥ 50 keV.

According to another embodiment the X-ray scattering device may comprise a Rayleigh X-ray scattering device which is arranged to measure scattered signals due to coherent X-ray scattering. The X-rays may have an energy ≤ 30 keV.

15 RF or microwave sensors

According to an embodiment one or more RF or microwave sensors or devices may be used to obtain image or other data from one or more regions of a target.

- 20 Fig. 3 shows an RF or microwave sensor or device 30 which may be used to acquire image data according to an embodiment. The RF or microwave sensor 30 may comprise a coaxial line probe 31 such that a microwave load 32 is directed into a target 33 which may comprise *in vivo* tissue such as lung or breast tissue. The microwave load 32 results in an electrical field 34 which penetrates a short distance
25 into the target 33. A reflected signal 35 is captured by the coaxial line probe 31 and is detected by the RF or microwave sensor or device 30. One or more physical or image properties of the target or target tissue 33 may then be determined.

- In particular, the RF sensor or device 30 may utilise microwaves at RF frequencies. In the case of breast tissue, normal breast tissue is substantially
30 translucent to microwaves and there is a high dielectric contrast between malignant breast tumours and normal breast tissue. As a result, according to an embodiment a RF or microwave sensor 30 may be used to detect regions of e.g. breast tissue which are potentially cancerous. As a result, the image data obtained by the RF or microwave sensor 30 may be used to direct a surgeon to specific areas of breast
35 tissue which may then be subjected to a surgical procedure using an ambient ionisation ion source such as a rapid evaporative ionisation mass spectrometry ("REIMS") ion source. In particular, the image data obtained by the RF or microwave sensor 30 may be used in conjunction with the ambient ionisation ion source to help determine the margins or bounds of potentially cancerous tissue with a high level of
40 precision.

It will be appreciated that being able to determine to a high level of certainty that all undesired (e.g. potentially cancerous) tissue has been removed from a

surgical site without also unnecessarily removing healthy tissue can have a significant positive impact upon potential surgical outcomes.

5 A pulsed confocal technique may be used together with time-gating in order to enhance the detection of tumours whilst suppressing the effects of tissue heterogeneity and absorption.

It is known to perform X-ray mammograms. However, there are concerns that repeated X-ray mammograms can result in an increased risk of cancer.

10 Therefore, one advantage of utilising RF or microwave technology according to various embodiments is that it avoids subjecting a patient to any increased risk (whether perceived or real) of cancer and also can be performed in a more relaxing and flexible environment which puts the patient at ease.

15 It is known that microwaves interact with biological tissue according to the water content of the tissue and that this interaction is quite different to the interaction of X-rays with biological tissue. In particular, using a microwave sensor or device according to an embodiment can result in an order of magnitude improvement in terms of contrast compared to using either X-rays or ultrasound.

According to various embodiments the dielectric permittivity of a target which may comprise a specific type of tissue such as healthy *in vivo* breast or lung tissue may be determined in advance or may be determined during an initial procedure.
20 The presence or absence of fluid (e.g., water) at the target or tissue 33 will impact upon the dielectric polarization. The microwave reflection coefficient will depend upon the dielectric properties of the target 33 and hence as a result the intensity of the reflected microwave signal will depend upon the fluid or water content of the tissue 33 which is being probed. As a result, the fluid or water content of the target
25 or tissue 33 of interest can be determined and in particular areas of the target or tissue 33 which have a suspect fluid or water content can be identified.

In the case of lung tissue, for example, microwave reflectrometry measurements of the lung tissue enable the total tissue water content of the lung tissue to be determined. This can be useful in determining whether or not potentially
30 cancerous lung tissue may be present. For example, healthy lung tissue may have a first water content (e.g., 77%) and cancerous lung tissue may have a second (higher) water content (e.g., 85%).

Furthermore, this approach can be useful in identifying the margins of a tumour in lung tissue. For example, the margins of the tumour may have a third
35 (intermediate) water content (e.g., 82%) which is intermediate between the first water content of healthy tissue (77%) and the second water content of cancerous tissue (85%).

According to embodiments a microwave generator may be used to generate the microwave signal and the frequency of the signal emitted by the microwave
40 generator may be varied from e.g. 5 MHz to e.g. 3 GHz as desired.

Embodiments are contemplated wherein the RF or microwave sensor 30 may be set to generate microwaves at a fixed frequency. Other embodiments are

contemplated wherein the RF or microwave sensor or device 30 may be arranged to vary the frequency of microwaves which are output by the microwave sensor or device 30. For example, a target or tissue 33 may be probed by scanning the surface with a range of difference microwave frequencies and then determining the response or profile of the intensity of reflected microwaves as a function of the input frequency of the microwaves.

Malignant tumours may have significantly different dielectric constants to that of normal tissue and the high dielectric contrast may cause malignant tumours to have significantly greater microwave scattering cross sections compared to normal tissue.

According to an embodiment microwaves having a frequency in the range 4-10 GHz may be focused and pulsed into tissue 33 (e.g. human breast). Microwave energy will be backscattered upon encountering a tumour since the tumour has a significantly greater dielectric permittivity and conductivity compared to normal tissue. Backscattered energy may be collected or otherwise detected by a sensor or detector. A three dimensional image of the tumour can thus be constructed.

It is known that high water content tissue will have a different permittivity response as a function of frequency compared to low water content tissue.

The relative dielectric permittivity ϵ_r and conductivity σ of high water content tissue (such as muscle or malignant tumours) is about an order of magnitude higher than lower water content tissue (such as fat or normal breast tissue). This contrast between high and low water content tissue persists over a wide range of microwave frequencies and enables diseased tissue to be differentiated from healthy tissue.

25 Analysing sample spectra

A list of analysis techniques which are intended to fall within the scope of the present invention are given in the following table:

Analysis Techniques
Univariate Analysis
Multivariate Analysis
Principal Component Analysis (PCA)
Linear Discriminant Analysis (LDA)
Maximum Margin Criteria (MMC)
Library Based Analysis
Soft Independent Modelling Of Class Analogy (SIMCA)
Factor Analysis (FA)
Recursive Partitioning (Decision Trees)
Random Forests
Independent Component Analysis (ICA)

Partial Least Squares Discriminant Analysis (PLS-DA)
Orthogonal (Partial Least Squares) Projections To Latent Structures (OPLS)
OPLS Discriminant Analysis (OPLS-DA)
Support Vector Machines (SVM)
(Artificial) Neural Networks
Multilayer Perceptron
Radial Basis Function (RBF) Networks
Bayesian Analysis
Cluster Analysis
Kernelized Methods
Subspace Discriminant Analysis
K-Nearest Neighbours (KNN)
Quadratic Discriminant Analysis (QDA)
Probabilistic Principal Component Analysis (PPCA)
Non negative matrix factorisation
K-means factorisation
Fuzzy c-means factorisation
Discriminant Analysis (DA)

Combinations of the foregoing analysis approaches can also be used, such as PCA-LDA, PCA-MMC, PLS-LDA, etc.

Analysing the sample spectra can comprise unsupervised analysis for dimensionality reduction followed by supervised analysis for classification.

By way of example, a number of different analysis techniques will now be described in more detail.

Multivariate analysis - developing a model for classification

By way of example, a method of building a classification model using multivariate analysis of plural reference sample spectra will now be described.

Fig. 4 shows a method 1500 of building a classification model using multivariate analysis. In this example, the method comprises a step 1502 of obtaining plural sets of intensity values for reference sample spectra. The method then comprises a step 1504 of unsupervised principal component analysis (PCA) followed by a step 1506 of supervised linear discriminant analysis (LDA). This approach may be referred to herein as PCA-LDA. Other multivariate analysis approaches may be used, such as PCA-MMC. The PCA-LDA model is then output, for example to storage, in step 1508.

The multivariate analysis such as this can provide a classification model that allows an aerosol, smoke or vapour sample to be classified using one or more sample spectra obtained from the aerosol, smoke or vapour sample. The multivariate analysis will now be described in more detail with reference to a simple example.

Fig. 5 shows a set of reference sample spectra obtained from two classes of known reference samples. The classes may be any one or more of the classes of target described herein. However, for simplicity, in this example the two classes will be referred as a left-hand class and a right-hand class.

Each of the reference sample spectra has been pre-processed in order to derive a set of three reference peak-intensity values for respective mass to charge ratios in that reference sample spectrum. Although only three reference peak-intensity values are shown, it will be appreciated that many more reference peak-intensity values (e.g., ~ 100 reference peak-intensity values) may be derived for a corresponding number of mass to charge ratios in each of the reference sample spectra. In other embodiments, the reference peak-intensity values may correspond to: masses; mass to charge ratios; ion mobilities (drift times); and/or operational parameters.

Fig. 6 shows a multivariate space having three dimensions defined by intensity axes. Each of the dimensions or intensity axes corresponds to the peak-intensity at a particular mass to charge ratio. Again, it will be appreciated that there may be many more dimensions or intensity axes (e.g., ~ 100 dimensions or intensity axes) in the multivariate space. The multivariate space comprises plural reference points, with each reference point corresponding to a reference sample spectrum, i.e., the peak-intensity values of each reference sample spectrum provide the co-ordinates for the reference points in the multivariate space.

The set of reference sample spectra may be represented by a reference matrix D having rows associated with respective reference sample spectra, columns associated with respective mass to charge ratios, and the elements of the matrix being the peak-intensity values for the respective mass to charge ratios of the respective reference sample spectra.

In many cases, the large number of dimensions in the multivariate space and matrix D can make it difficult to group the reference sample spectra into classes. PCA may accordingly be carried out on the matrix D in order to calculate a PCA model that defines a PCA space having a reduced number of one or more dimensions defined by principal component axes. The principal components may be selected to be those that comprise or "explain" the largest variance in the matrix D and that cumulatively explain a threshold amount of the variance in the matrix D.

Fig. 7 shows how the cumulative variance may increase as a function of the number n of principal components in the PCA model. The threshold amount of the variance may be selected as desired.

The PCA model may be calculated from the matrix D using a non-linear iterative partial least squares (NIPALS) algorithm or singular value decomposition, the details of which are known to the skilled person and so will not be described herein in detail. Other methods of calculating the PCA model may be used.

The resultant PCA model may be defined by a PCA scores matrix S and a PCA loadings matrix L. The PCA may also produce an error matrix E, which contains

the variance not explained by the PCA model. The relationship between D, S, L and E may be:

$$D = SL^T + E \quad (1)$$

5

Fig. 8 shows the resultant PCA space for the reference sample spectra of Figs. 5 and 6. In this example, the PCA model has two principal components PC_0 and PC_1 and the PCA space therefore has two dimensions defined by two principal component axes. However, a lesser or greater number of principal components may be included in the PCA model as desired. It is generally desired that the number of principal components is at least one less than the number of dimensions in the multivariate space.

10

The PCA space comprises plural transformed reference points or PCA scores, with each transformed reference point or PCA score corresponding to a reference sample spectrum of Fig. 5 and therefore to a reference point of Fig. 6.

15

As is shown in Fig. 8, the reduced dimensionality of the PCA space makes it easier to group the reference sample spectra into the two classes. Any outliers may also be identified and removed from the classification model at this stage.

Further supervised multivariate analysis, such as multi-class LDA or maximum margin criteria (MMC), in the PCA space may then be performed so as to define classes and, optionally, further reduce the dimensionality.

20

As will be appreciated by the skilled person, multi-class LDA seeks to maximise the ratio of the variance between classes to the variance within classes (i.e., so as to give the largest possible distance between the most compact classes possible). The details of LDA are known to the skilled person and so will not be described herein in detail.

25

The resultant PCA-LDA model may be defined by a transformation matrix U, which may be derived from the PCA scores matrix S and class assignments for each of the transformed spectra contained therein by solving a generalised eigenvalue problem.

30

The transformation of the scores S from the original PCA space into the new LDA space may then be given by:

$$Z = SU \quad (2)$$

35

wherein the matrix Z contains the scores transformed into the LDA space.

Fig. 9 shows a PCA-LDA space having a single dimension or axis, wherein the LDA is performed in the PCA space of Fig. 8. As is shown in Fig. 9, the LDA space comprises plural further transformed reference points or PCA-LDA scores, with each further transformed reference point corresponding to a transformed reference point or PCA score of Fig. 8.

40

In this example, the further reduced dimensionality of the PCA-LDA space makes it even easier to group the reference sample spectra into the two classes. Each class in the PCA-LDA model may be defined by its transformed class average and covariance matrix or one or more hyperplanes (including points, lines, planes or higher order hyperplanes) or hypersurfaces or Voronoi cells in the PCA-LDA space.

The PCA loadings matrix L, the LDA matrix U and transformed class averages and covariance matrices or hyperplanes or hypersurfaces or Voronoi cells may be output to a database for later use in classifying an aerosol, smoke or vapour sample.

The transformed covariance matrix in the LDA space V'_g for class g may be given by:

$$V'_g = U^T V_g U \quad (3)$$

wherein V_g are the class covariance matrices in the PCA space.

The transformed class average position z_g for class g may be given by:

$$s_g U = z_g \quad (4)$$

wherein s_g is the class average position in the PCA space.

Multivariate analysis - using a model for classification

By way of example, a method of using a classification model to classify an aerosol, smoke or vapour sample will now be described.

Fig. 10 shows a method 2100 of using a classification model. In this example, the method comprises a step 2102 of obtaining a set of intensity values for a sample spectrum. The method then comprises a step 2104 of projecting the set of intensity values for the sample spectrum into PCA-LDA model space. Other classification model spaces may be used, such as PCA-MMC. The sample spectrum is then classified at step 2106 based on the project position and the classification is then output in step 2108.

Classification of an aerosol, smoke or vapour sample will now be described in more detail with reference to the simple PCA-LDA model described above.

Fig. 11 shows a sample spectrum obtained from an unknown aerosol, smoke or vapour sample. The sample spectrum has been pre-processed in order to derive a set of three sample peak-intensity values for respective mass to charge ratios. As mentioned above, although only three sample peak-intensity values are shown, it will be appreciated that many more sample peak-intensity values (e.g., ~ 100 sample peak-intensity values) may be derived at many more corresponding mass to charge ratios for the sample spectrum. Also, as mentioned above, in other embodiments, the

sample peak-intensity values may correspond to: masses; mass to charge ratios; ion mobilities (drift times); and/or operational parameters.

The sample spectrum may be represented by a sample vector $\mathbf{d}_x$, with the elements of the vector being the peak-intensity values for the respective mass to charge ratios. A transformed PCA vector $\mathbf{s}_x$ for the sample spectrum can be obtained as follows:

$$\mathbf{d}_x \mathbf{L} = \mathbf{s}_x \quad (5)$$

Then, a transformed PCA-LDA vector $\mathbf{z}_x$ for the sample spectrum can be obtained as follows:

$$\mathbf{s}_x \mathbf{U} = \mathbf{z}_x \quad (6)$$

Fig. 12 again shows the PCA-LDA space of Fig. 9. However, the PCA-LDA space of Fig. 12 further comprises the projected sample point, corresponding to the transformed PCA-LDA vector $\mathbf{z}_x$, derived from the peak intensity values of the sample spectrum of Fig. 11.

In this example, the projected sample point is to one side of a hyperplane between the classes that relates to the right-hand class, and so the aerosol, smoke or vapour sample may be classified as belonging to the right-hand class.

Alternatively, the Mahalanobis distance from the class centres in the LDA space may be used, where the Mahalanobis distance of the point $\mathbf{z}_x$ from the centre of class g may be given by the square root of:

$$(\mathbf{z}_x - \mathbf{z}_g)^T (\mathbf{V}'_g)^{-1} (\mathbf{z}_x - \mathbf{z}_g) \quad (7)$$

and the data vector $\mathbf{d}_x$ may be assigned to the class for which this distance is smallest.

In addition, treating each class as a multivariate Gaussian, a probability of membership of the data vector to each class may be calculated.

Library Based Analysis - Developing a Library for Classification

By way of example, a method of building a classification library using plural input reference sample spectra will now be described.

Fig. 13 shows a method 2400 of building a classification library. In this example, the method comprises a step 2402 of obtaining plural input reference sample spectra and a step 2404 of deriving metadata from the plural input reference sample spectra for each class of sample. The method then comprises a step 2406 of storing the metadata for each class of sample as a separate library entry. The classification library is then output, for example to electronic storage, in step 2408.

A classification library such as this allows an aerosol, smoke or vapour sample to be classified using one or more sample spectra obtained from the aerosol, smoke or vapour sample. The library based analysis will now be described in more detail with reference to an example.

5 In this example, each entry in the classification library is created from plural pre-processed reference sample spectra that are representative of a class. In this example, the reference sample spectra for a class are pre-processed according to the following procedure:

10 First, a re-binning process is performed. In this embodiment, the data are resampled onto a logarithmic grid with abscissae:

$$x_i = \left\lfloor N_{chan} \log \frac{m}{M_{min}} / \log \frac{M_{max}}{M_{min}} \right\rfloor \quad (8)$$

15 wherein N_{chan} is a selected value and $\lfloor x \rfloor$ denotes the nearest integer below x . In one example, N_{chan} is 2^{12} or 4096.

Then, a background subtraction process is performed. In this embodiment, a cubic spline with k knots is then constructed such that $p\%$ of the data between each pair of knots lies below the curve. This curve is then subtracted from the data. In one example, k is 32. In one example, p is 5. A constant value corresponding to the $q\%$ quantile of the intensity subtracted data is then subtracted from each intensity.

20 Positive and negative values are retained. In one example, q is 45.

Then, a normalisation process is performed. In this embodiment, the data are normalised to have mean $\bar{y}_i$. In one example, $\bar{y}_i = 1$.

25 An entry in the library then consists of metadata in the form of a median spectrum value μ_i and a deviation value D_i for each of the N_{chan} points in the spectrum.

The likelihood for the i 'th channel is given by:

$$Pr(y_i | \mu_i, D_i) = \frac{1}{D_i} \frac{C^{C-1/2} \Gamma(C)}{\sqrt{\pi} \Gamma(C-1/2)} \frac{1}{\left(C + \frac{(y_i - \mu_i)^2}{D_i^2} \right)^C} \quad (9)$$

30

where $1/2 \leq C < \infty$ and where $\Gamma(C)$ is the gamma function.

The above equation is a generalised Cauchy distribution which reduces to a standard Cauchy distribution for $C = 1$ and becomes a Gaussian (normal) distribution as $C \rightarrow \infty$. The parameter D_i controls the width of the distribution (in the Gaussian limit $D_i = \sigma_i$ is simply the standard deviation) while the global value C controls the size of the tails.

35

In one example, C is $3/2$, which lies between Cauchy and Gaussian, so that the likelihood becomes:

$$Pr(y_i|\mu_i, D_i) = \frac{3}{4} \frac{1}{D_i} \frac{1}{(3/2 + (y_i - \mu_i)^2 / D_i^2)^{3/2}} \quad (10)$$

For each library entry, the parameters μ_i are set to the median of the list of values in the i'th channel of the input reference sample spectra while the deviation D_i is taken to be the interquartile range of these values divided by $\sqrt{2}$. This choice can ensure that the likelihood for the i'th channel has the same interquartile range as the input data, with the use of quantiles providing some protection against outlying data.

Library based analysis - using a library for classification

By way of example, a method of using a classification library to classify an aerosol, smoke or vapour sample will now be described.

Fig. 14 shows a method 2500 of using a classification library. In this example, the method comprises a step 2502 of obtaining a set of plural sample spectra. The method then comprises a step 2504 of calculating a probability or classification score for the set of plural sample spectra for each class of sample using metadata for the class entry in the classification library. The sample spectra are then classified at step 2506 and the classification is then output in step 2508.

Classification of an aerosol, smoke or vapour sample will now be described in more detail with reference to the classification library described above.

In this example, an unknown sample spectrum y is the median spectrum of a set of plural sample spectra. Taking the median spectrum y can protect against outlying data on a channel by channel basis.

The likelihood L_s for the input data given the library entry s is then given by:

$$L_s = Pr(y|\mu, D) = \prod_{i=1}^{N_{chan}} Pr(y_i|\mu_i, D_i) \quad (11)$$

wherein μ_i and D_i are, respectively, the library median values and deviation values for channel i . The likelihoods L_s may be calculated as log likelihoods for numerical safety.

The likelihoods L_s are then normalised over all candidate classes ' s ' to give probabilities, assuming a uniform prior probability over the classes. The resulting probability for the class $\tilde{s}$ is given by:

$$Pr(\tilde{s}|y) = \frac{L_{\tilde{s}}^{(1/F)}}{\sum_s L_s^{(1/F)}} \quad (12)$$

The exponent $(1/F)$ can soften the probabilities which may otherwise be too definitive. In one example, $F = 100$. These probabilities may be expressed as percentages, e.g., in a user interface.

Alternatively, RMS classification scores R_s may be calculated using the same median sample values and derivation values from the library:

$$R_s(y, \mu, D) = \sqrt{\frac{1}{N_{chan}} \sum_{i=1}^{N_{chan}} \frac{(y_i - \mu_i)^2}{D_i^2}} \quad (13)$$

5

Again, the scores R_s are normalised over all candidate classes ' s '.

The aerosol, smoke or vapour sample may then be classified as belonging to the class having the highest probability and/or highest RMS classification score.

10

Multivariate analysis of imaging data

Various further embodiments are contemplated wherein the imaging data may itself be subjected to multivariate analysis in order to assist, for example, in the identification of the target and/or to filter out outliers.

15

Methods of medical treatment, surgery and diagnosis and non-medical methods

Various different embodiments are contemplated. According to some embodiments the methods disclosed above may be performed on *in vivo*, *ex vivo* or *in vitro* tissue. The tissue may comprise human or non-human animal tissue. Embodiments are contemplated wherein the target may comprise biological tissue, a bacterial or fungal colony or more generally an organic target such as a plastic).

20

Various embodiments are contemplated wherein analyte ions generated by an ambient ionisation ion source are then subjected either to: (i) mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser; (ii) ion mobility analysis (IMS) and/or differential ion mobility analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis; and/or (iii) a combination of firstly (or vice versa) ion mobility analysis (IMS) and/or differential ion mobility analysis (DMA) and/or Field Asymmetric Ion Mobility Spectrometry (FAIMS) analysis followed by secondly (or vice versa) mass analysis by a mass analyser such as a quadrupole mass analyser or a Time of Flight mass analyser. Various embodiments also relate to an ion mobility spectrometer and/or mass analyser and a method of ion mobility spectrometry and/or method of mass analysis. Ion mobility analysis may be performed prior to mass to charge ratio analysis or vice versa.

25

30

35

Various references are made in the present application to mass analysis, mass analysers, mass analysing, mass spectrometric data, mass spectrometers and other related terms referring to apparatus and methods for determining the mass or mass to charge of analyte ions. It should be understood that it is equally contemplated that the present invention may extend to ion mobility analysis, ion mobility analysers, ion mobility analysing, ion mobility data, ion mobility spectrometers, ion mobility separators and other related terms referring to apparatus

40

and methods for determining the ion mobility, differential ion mobility, collision cross section or interaction cross section of analyte ions. Furthermore, it should also be understood that embodiments are contemplated wherein analyte ions may be subjected to a combination of both ion mobility analysis and mass analysis i.e. that both (a) the ion mobility, differential ion mobility, collision cross section or interaction cross section of analyte ions together with (b) the mass to charge of analyte ions is determined. Accordingly, hybrid ion mobility-mass spectrometry (IMS-MS) and mass spectrometry-ion mobility (MS-IMS) embodiments are contemplated wherein both the ion mobility and mass to charge ratio of analyte ions generated e.g. by an ambient ionisation ion source are determined. Ion mobility analysis may be performed prior to mass to charge ratio analysis or vice versa. Furthermore, it should be understood that embodiments are contemplated wherein references to mass spectrometric data and databases comprising mass spectrometric data should also be understood as encompassing ion mobility data and differential ion mobility data etc. and databases comprising ion mobility data and differential ion mobility data etc. (either in isolation or in combination with mass spectrometric data).

Various surgical, therapeutic, medical treatment and diagnostic methods are contemplated.

However, other embodiments are contemplated which relate to non-surgical and non-therapeutic methods of mass spectrometry which are not performed on *in vivo* tissue. Other related embodiments are contemplated which are performed in an extracorporeal manner such that they are performed outside of the human or animal body.

Further embodiments are contemplated wherein the methods are performed on a non-living human or animal, for example, as part of an autopsy procedure.

Although the present invention has been described with reference to preferred embodiments, it will be understood by those skilled in the art that various changes in form and detail may be made without departing from the scope of the invention as set forth in the accompanying claims.

12295403v23a

Claims

- 5 1. A method comprising:
obtaining or acquiring image or other data from one or more regions of a
target;
using said image or other data to determine one or more regions of interest of
said target; and
10 using a first device to generate aerosol, smoke or vapour from one or more
regions of said target.
2. A method as claimed in claim 1, wherein said image or other data comprises
data selected from the group consisting of: (i) thermal, temperature or thermographic
15 image data; (ii) microwave image data; (iii) visual or optical image data; (iv) infra-red
("IR") image data; (v) radio-frequency ("RF") image data; (vi) X-ray image data; (vii)
magnetic resonance imaging ("MRI") image data; (viii) ultrasonic or ultrasound image
data; (ix) tomographic image data; (x) optical or other absorption data; (xi) optical or
other scattering coefficient data; (xii) oxyhemoglobin or deoxyhemoglobin
20 absorbance data; (xiii) near infrared (NIR) image data; or (xiv) magnetic data.
3. A method as claimed in claim 1 or 2, wherein said first device comprises or
forms part of an ambient ion or ionisation source or wherein said first device
generates said aerosol, smoke or vapour for subsequent ionisation by an ambient ion
25 or ionisation source or other ionisation source.
4. A method as claimed in any of claims 1, 2 or 3, wherein said target comprises
native or unmodified target material.
- 30 5. A method as claimed in claim 4, wherein said native or unmodified target
material is unmodified by the addition of a matrix or reagent.
6. A method as claimed in any preceding claim, wherein said first device is
arranged and adapted to generate aerosol, smoke or vapour from one or more
35 regions of said target without said target requiring prior preparation.
7. A method as claimed in any preceding claim, wherein said first device
comprises an ion source selected from the group consisting of: (i) a rapid evaporative
ionisation mass spectrometry ("REIMS") ion source; (ii) a desorption electrospray
40 ionisation ("DESI") ion source; (iii) a laser desorption ionisation ("LDI") ion source;
(iv) a thermal desorption ion source; (v) a laser diode thermal desorption ("LDTD")
ion source; (vi) a desorption electro-flow focusing ("DEFFI") ion source; (vii) a

dielectric barrier discharge ("DBD") plasma ion source; (viii) an Atmospheric Solids Analysis Probe ("ASAP") ion source; (ix) an ultrasonic assisted spray ionisation ion source; (x) an easy ambient sonic-spray ionisation ("EASI") ion source; (xi) a desorption atmospheric pressure photoionisation ("DAPPI") ion source; (xii) a paperspray ("PS") ion source; (xiii) a jet desorption ionisation ("JeDI") ion source; (xiv) a touch spray ("TS") ion source; (xv) a nano-DESI ion source; (xvi) a laser ablation electrospray ("LAESI") ion source; (xvii) a direct analysis in real time ("DART") ion source; (xviii) a probe electrospray ionisation ("PESI") ion source; (xix) a solid-probe assisted electrospray ionisation ("SPA-ESI") ion source; (xx) a cavitron ultrasonic surgical aspirator ("CUSA") device; (xxi) a focussed or unfocussed ultrasonic ablation device; (xxii) a microwave resonance device; and (xxiii) a pulsed plasma RF dissection device.

8. A method as claimed in any preceding claim, wherein said step of using said first device to generate aerosol, smoke or vapour from one or more regions of said target further comprises contacting said target with one or more electrodes.

9. A method as claimed in claim 8, wherein said one or more electrodes comprise: (i) a monopolar device, wherein the method optionally further comprises providing a separate return electrode; (ii) a bipolar device; or (iii) a multi phase RF device, wherein the method optionally further comprises providing a separate return electrode or electrodes.

10. A method as claimed in claim 8 or 9, wherein said one or more electrodes comprise a rapid evaporation ionization mass spectrometry ("REIMS") device.

11. A method as claimed in any of claims 8, 9 or 10, further comprising applying an AC or RF voltage to said one or more electrodes in order to generate said aerosol, smoke or vapour.

12. A method as claimed in claim 11, wherein the step of applying said AC or RF voltage to said one or more electrodes further comprises applying one or more pulses of said AC or RF voltage to said one or more electrodes.

13. A method as claimed in claim 11 or 12, wherein said step of applying said AC or RF voltage to said one or more electrodes causes heat to be dissipated into said target.

14. A method as claimed in any of claims 1-7, wherein said step of using said first device to generate aerosol, smoke or vapour from one or more regions of said target further comprises irradiating said target with a laser.

15. A method as claimed in any preceding claim, wherein said first device is arranged and adapted to generate aerosol from one or more regions of said target by direct evaporation or vaporisation of target material from said target by Joule heating or diathermy.

5

16. A method as claimed in any preceding claim, wherein said step of using said first device to generate aerosol, smoke or vapour from one or more regions of said target further comprises directing ultrasonic energy into said target.

10 17. A method as claimed in any preceding claim, wherein said aerosol comprises uncharged aqueous droplets optionally comprising cellular material.

18. A method as claimed in any preceding claim, wherein at least 50%, 55%, 60%, 65%, 70%, 75%, 80%, 85%, 90% or 95% of the mass or matter generated by
15 said first device and which forms said aerosol is in the form of droplets.

19. A method as claimed in any preceding claim, wherein said first device is arranged and adapted to generate aerosol wherein the Sauter mean diameter ("SMD", d_{32}) of said aerosol is in a range: (i) $< 5 \mu\text{m}$; (ii) $5\text{-}10 \mu\text{m}$; (iii) $10\text{-}15 \mu\text{m}$; (iv)
20 $15\text{-}20 \mu\text{m}$; (v) $20\text{-}25 \mu\text{m}$; or (vi) $> 25 \mu\text{m}$.

20. A method as claimed in any preceding claim, wherein said aerosol traverses a flow region with a Reynolds number (Re) in the range: (i) < 2000 ; (ii) $2000\text{-}2500$; (iii) $2500\text{-}3000$; (iv) $3000\text{-}3500$; (v) $3500\text{-}4000$; or (vi) > 4000 .

25

21. A method as claimed in any preceding claim, wherein substantially at the point of generating said aerosol, said aerosol comprises droplets having a Weber number (We) selected from the group consisting of: (i) < 50 ; (ii) $50\text{-}100$; (iii) $100\text{-}150$; (iv) $150\text{-}200$; (v) $200\text{-}250$; (vi) $250\text{-}300$; (vii) $300\text{-}350$; (viii) $350\text{-}400$; (ix) $400\text{-}450$; (x)
30 $450\text{-}500$; (xi) $500\text{-}550$; (xii) $550\text{-}600$; (xiii) $600\text{-}650$; (xiv) $650\text{-}700$; (xv) $700\text{-}750$; (xvi) $750\text{-}800$; (xvii) $800\text{-}850$; (xviii) $850\text{-}900$; (xix) $900\text{-}950$; (xx) $950\text{-}1000$; and (xxi) > 1000 .

22. A method as claimed in any preceding claim, wherein substantially at the
35 point of generating said aerosol, said aerosol comprises droplets having a Stokes number (S_k) in the range: (i) $1\text{-}5$; (ii) $5\text{-}10$; (iii) $10\text{-}15$; (iv) $15\text{-}20$; (v) $20\text{-}25$; (vi) $25\text{-}30$; (vii) $30\text{-}35$; (viii) $35\text{-}40$; (ix) $40\text{-}45$; (x) $45\text{-}50$; and (xi) > 50 .

23. A method as claimed in any preceding claim, wherein substantially at the
40 point of generating said aerosol, said aerosol comprises droplets having a mean axial velocity selected from the group consisting of: (i) $< 20 \text{ m/s}$; (ii) $20\text{-}30 \text{ m/s}$; (iii) $30\text{-}40 \text{ m/s}$; (iv) $40\text{-}50 \text{ m/s}$; (v) $50\text{-}60 \text{ m/s}$; (vi) $60\text{-}70 \text{ m/s}$; (vii) $70\text{-}80 \text{ m/s}$; (viii) $80\text{-}90 \text{ m/s}$; (ix)

90-100 m/s; (x) 100-110 m/s; (xi) 110-120 m/s; (xii) 120-130 m/s; (xiii) 130-140 m/s; (xiv) 140-150 m/s; and (xv) > 150 m/s.

24. A method as claimed in any preceding claim, wherein said target comprises biological tissue, biological matter, a bacterial colony or a fungal colony.

25. A method as claimed in claim 24, wherein said biological tissue comprises human tissue or non-human animal tissue.

26. A method as claimed in claim 24 or 25, wherein said biological tissue comprises *in vivo* biological tissue.

27. A method as claimed in claim 24 or 25, wherein said biological tissue comprises *ex vivo* biological tissue.

28. A method as claimed in claim 24 or 25, wherein said biological tissue comprises *in vitro* biological tissue.

29. A method as claimed in any of claims 24-28, wherein said biological tissue comprises: (i) adrenal gland tissue, appendix tissue, bladder tissue, bone, bowel tissue, brain tissue, breast tissue, bronchi, coronal tissue, ear tissue, esophagus tissue, eye tissue, gall bladder tissue, genital tissue, heart tissue, hypothalamus tissue, kidney tissue, large intestine tissue, intestinal tissue, larynx tissue, liver tissue, lung tissue, lymph nodes, mouth tissue, nose tissue, pancreatic tissue, parathyroid gland tissue, pituitary gland tissue, prostate tissue, rectal tissue, salivary gland tissue, skeletal muscle tissue, skin tissue, small intestine tissue, spinal cord, spleen tissue, stomach tissue, thymus gland tissue, trachea tissue, thyroid tissue, ureter tissue, urethra tissue, soft and connective tissue, peritoneal tissue, blood vessel tissue and/or fat tissue; (ii) grade I, grade II, grade III or grade IV cancerous tissue; (iii) metastatic cancerous tissue; (iv) mixed grade cancerous tissue; (v) a sub-grade cancerous tissue; (vi) healthy or normal tissue; or (vii) cancerous or abnormal tissue.

30. A method as claimed in any preceding claim, wherein said first device comprises a point of care ("POC"), diagnostic or surgical device.

31. A method as claimed in any preceding claim, further comprising ionising at least some of said aerosol, smoke or vapour so as to generate analyte ions.

32. A method as claimed in any preceding claim, further comprising directing or aspirating at least some of said aerosol, smoke or vapour into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer.

33. A method as claimed in claim 32, further comprising ionising at least some said aerosol, smoke or vapour within a or said vacuum chamber of said mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

5

34. A method as claimed in claim 33, further comprising causing said aerosol, smoke or vapour to impact upon a collision surface located within a vacuum chamber of said mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

10

35. A method as claimed in claim 31, 33 or 34, further comprising mass analysing said analyte ions in order to obtain mass spectrometric data and/or ion mobility data.

36. A method as claimed in any preceding claim, further comprising mass analysing said aerosol, smoke or vapour or ions derived from said aerosol, smoke or vapour in order to obtain mass spectrometric data and/or ion mobility data.

15

37. A method as claimed in claim 35 or 36, further comprising analysing said mass spectrometric data and/or ion mobility data in order either: (i) to distinguish between healthy and diseased tissue; (ii) to distinguish between potentially cancerous and non-cancerous tissue; (iii) to distinguish between different types or grades of cancerous tissue; (iv) to distinguish between different types or classes of target material; (v) to determine whether or not one or more desired or undesired substances are present in said target; (vi) to confirm the identity or authenticity of said target; (vii) to determine whether or not one or more impurities, illegal substances or undesired substances are present in said target; (viii) to determine whether a human or animal patient is at an increased risk of suffering an adverse outcome; (ix) to make or assist in the making a diagnosis or prognosis; and (x) to inform a surgeon, nurse, medic or robot of a medical, surgical or diagnostic outcome.

20

25

30

38. A method as claimed in claim 35, 36 or 37, wherein the step of analysing said mass spectrometric data and/or ion mobility data comprises analysing one or more sample spectra so as to classify an aerosol, smoke or vapour sample.

35

39. A method as claimed in claim 38, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises supervised analysis of the one or more sample spectra and/or unsupervised analysis of the one or more sample spectra.

40

40. A method as claimed in claim 38 or 39, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises using one or more of: univariate analysis; multivariate analysis; principal component

analysis (PCA); linear discriminant analysis (LDA); maximum margin criteria (MMC); library-based analysis; soft independent modelling of class analogy (SIMCA); factor analysis (FA); recursive partitioning (decision trees); random forests; independent component analysis (ICA); partial least squares discriminant analysis (PLS-DA);

5 orthogonal (partial least squares) projections to latent structures (OPLS); OPLS discriminant analysis (OPLS-DA); support vector machines (SVM); (artificial) neural networks; multilayer perceptron; radial basis function (RBF) networks; Bayesian analysis; cluster analysis; a kernelized method; and subspace discriminant analysis.

10 41. A method as claimed in claim 38, 39 or 40, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises developing a classification model or library using one or more reference sample spectra.

15 42. A method as claimed in any of claims 38-41, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises performing linear discriminant analysis (LDA) after performing principal component analysis (PCA).

20 43. A method as claimed in any of claims 38-41, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises performing a maximum margin criteria (MMC) process after performing principal component analysis (PCA).

25 44. A method as claimed in any of claims 38-43, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises defining one or more classes within a classification model or library.

30 45. A method as claimed in any of claims 38-44, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises defining one or more classes within a classification model or library manually or automatically according to one or more class or cluster criteria.

35 46. A method as claimed in claim 45, wherein the one or more class or cluster criteria for each class are based on one or more of: a distance between one or more pairs of reference points for reference sample spectra within a model space; a variance value between groups of reference points for reference sample spectra within a model space; and a variance value within a group of reference points for reference sample spectra within a model space.

40 47. A method as claimed in claim 44, 45 or 46, wherein the one or more classes are each defined by one or more class definitions.

48. A method as claimed in claim 47, wherein the one or more class definitions comprise one or more of: a set of one or more reference points for reference sample spectra, values, boundaries, lines, planes, hyperplanes, variances, volumes, Voronoi cells, and/or positions, within a model space; and one or more positions within a class hierarchy.

49. A method as claimed in any of claims 38-48, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises using a classification model or library to classify one or more unknown sample spectra.

50. A method as claimed in any of claims 38-49, wherein analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample comprises classifying one or more sample spectra manually or automatically according to one or more classification criteria.

51. A method as claimed in claim 50, wherein the one or more classification criteria comprise one or more of:

- 20 a distance between one or more projected sample points for one or more sample spectra within a model space and a set of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, volumes, Voronoi cells, or positions, within the model space being below a distance threshold or being the lowest such distance;
- 25 a position for one or more projected sample points for one or more sample spectra within a model space being one side or other of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, or positions, within the model space;
- 30 a position for one or more projected sample points for one or more sample spectra within a model space being within one or more volumes or Voronoi cells within the model space; and
- a probability or classification score being above a probability or classification score threshold or being the highest such probability or classification score.

52. A method as claimed in any of claims 35-51, wherein the step of analysing said mass spectrometric data and/or ion mobility data further comprises analysing a profile of said aerosol, smoke or vapour or a profile of ions derived from said aerosol, smoke or vapour.

53. A method as claimed in claim 52, wherein said profile is selected from the group consisting of: (i) a lipidomic profile; (ii) a fatty acid profile; (iii) a phospholipid profile; (iv) a phosphatidic acid (PA) profile; (v) a phosphatidylethanolamine (PE)

profile; (vi) a phosphatidylglycerol (PG) profile; (vii) a phosphatidylserines (PS) profile; (viii) a phosphatidylinositol (PI) profile; or (ix) a triglyceride (TG) profile.

54. A method as claimed in any preceding claim, further comprising using one or
5 more thermal or temperature sensors, detectors or devices to obtain said image or other data.

55. A method as claimed in claim 54, wherein said one or more thermal or
temperature sensors, detectors or devices are selected from the group consisting of:
10 (i) one or more temperature sensors; (ii) one or more thermal imaging sensors; (iii)
one or more infrared thermography ("IRT") sensors; and (iv) one or more infrared
imaging sensors.

56. A method as claimed in claim 54 or 55, further comprising using said one or
15 more thermal or temperature sensors, detectors or devices to obtain said image or other data with or without said one or more thermal or temperature sensors,
detectors or devices physically contacting said target.

57. A method as claimed in any of claims 54, 55 or 56, further comprising
20 determining a temperature, temperature profile or thermographic image of one or more regions of said target.

58. A method as claimed in any of claims 54-57, wherein said step of using said
image or other data to determine one or more regions of interest of said target
25 comprises determining one or more regions of said target which have a different
temperature, temperature profile or thermographic image intensity relative to normal
tissue, surrounding tissue, a control sample, a control region, control data or
predetermined data.

59. A method as claimed in any of claims 54-58, wherein said step of using said
image or other data to determine one or more regions of interest of said target
30 comprises determining whether or not a region of said target has a higher or lower
temperature, temperature profile or thermographic image intensity relative to normal
tissue, surrounding tissue, a control sample, a control region, control data or
35 predetermined data.

60. A method as claimed in any of claims 54-59, wherein said step of using said
image or other data to determine one or more regions of interest of said target further
40 comprises determining one or more hyperthermic or hypothermic regions of said
target.

61. A method as claimed in any preceding claim, further comprising using one or more microwave or RF sensors, detectors or devices to obtain said image or other data.

5 62. A method as claimed in claim 61, wherein said one or more microwave or RF sensors, detectors or devices comprise one or more microwave reflectrometry sensors, detectors or devices.

10 63. A method as claimed in claim 62, further comprising physically contacting said target with said one or more microwave reflectrometry sensors.

15 64. A method as claimed in claim 62 or 63, further comprising using said one or more microwave reflectrometry sensors to determine a fluid content of one or more regions of said target.

20 65. A method as claimed in any of claims 54-64, wherein said step of using said image or other data to determine one or more regions of interest of said target comprises determining one or more regions of said target which have a different fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

25 66. A method as claimed in any of claims 54-65, wherein said step of using said image or other data to determine one or more regions of interest of said target comprises determining whether or not a region of said target has a higher or lower fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

30 67. A method as claimed in any preceding claim, further comprising using an optical coherence tomography ("OCT") device to obtain said image or other data.

35 68. A method as claimed in claim 67, further comprising using a low coherence light source ("LCS"), a super-luminescent diode ("SLD"), a swept source or tunable laser ("SS"), an ultra-short pulsed laser or a supercontinuum laser to illuminate said target.

69. A method as claimed in claim 67 or 68, wherein said optical coherence tomography device comprises an interferometer.

40 70. A method as claimed in any preceding claim, further comprising using one or more computed tomography devices to obtain said image or other data.

71. A method as claimed in any preceding claim, further comprising using a positron emission tomography ("PET") device to obtain said image or other data.

72. A method as claimed in any preceding claim, further comprising using a magnetic resonance imaging ("MRI") device to obtain said image or other data.

73. A method as claimed in any preceding claim, further comprising using one or more ultrasonic tomography devices to obtain said image or other data.

74. A method as claimed in any preceding claim, further comprising using one or more optical imaging sensors, detectors or devices to obtain said image or other data.

75. A method as claimed in claim 74, further comprising using a continuous wave (CW) light source to illuminate said target.

76. A method as claimed in claim 74, further comprising using a time domain photon migration (TDPM) imaging system to obtain said image or other data.

77. A method as claim in claim 74, further comprising using a frequency-domain photon migration (FDPM) imaging system to obtain said image or other data.

78. A method as claimed in any preceding claim, further comprising using one or more contrast agents to enhance said image data.

79. A method as claimed in claim 78, wherein said one or more contrast agents comprise one or more fluorescent contrast agents.

80. A method as claimed in claim 78 or 79, wherein said one or more contrast agents comprise one or more visible dyes.

81. A method as claimed in claim 78, 79 or 80, wherein said one or more contrast agents comprise one or more radiocontrast agents.

82. A method as claimed in any of claims 78-81, wherein said one or more contrast agents comprise one or more optical, near infrared ("NIR"), fluorescent, autofluorescent or diagnostic contrast agents.

83. A method as claimed in any of claims 78-82, wherein said one or more contrast agents are selected from the group consisting of: (i) indocyanine green ("ICG") and derivatives or conjugates of indocyanine green including indotricarbocyanine; (ii) diethylthiatricarbocyanine iodide ("DTTCI") and derivatives or

conjugates of diethylthiatricarbocyanine iodide; (iii) rhodamine B and derivatives or conjugates of rhodamine B; (iv) photodynamic therapy ("PDT") agents including hexylpyropheophorbide ("HPPH"); (v) a cyanine dye including Cy 5.5 dyes; and (vi) bifunctional contrast agents.

5

84. A method as claimed in any of claims 78-83, wherein said one or more contrast agents comprise nanoparticles.

85. A method as claimed in claim 84, wherein said one or more contrast agents
10 comprise: (i) magnetic or ferromagnetic nanoparticles; (ii) gold nanoparticles; (iii) metallic nanoparticles; (iv) functionalised nanoparticles; (v) nanospheres, nanorods, nanostars or nanoshells; (vi) levan nanoparticles; or (vii) copper, zinc, titanium, magnesium, alginate, alloy or silver nanoparticles.

15 86. A method as claimed in any of claims 78-85, wherein said one or more contrast agents are exogenous to said target.

87. A method as claimed in any of claims 78-85, wherein said one or more contrast agents are endogenous to said target.

20

88. A method as claimed in any preceding claim, further comprising using an X-ray scattering device to obtain said image or other data.

89. A method as claimed in claim 88, further comprising directing X-rays onto one
25 or more regions of said target.

90. A method as claimed in claim 89, further comprising measuring the wavelength or frequency of scattered X-rays from said target.

30 91. A method as claimed in claim 88, 89 or 90, wherein said X-ray scattering device comprises a Compton X-ray scattering device.

92. A method as claimed in claim 91, further comprising using said Compton X-ray scattering device to measure scattered signals due to incoherent X-ray
35 scattering.

93. A method as claimed in claim 91 or 92, wherein said X-rays have an energy $\geq$ 50 keV.

40 94. A method as claimed in claim 88, 89 or 90, wherein said X-ray scattering device comprises a Rayleigh X-ray scattering device.

95. A method as claimed in claim 94, further comprising using said Rayleigh X-ray scattering device to measure scattered signals due to coherent X-ray scattering.

96. A method as claimed in claim 94 or 95, wherein said X-rays have an energy $\leq$ 30 keV.

97. A method as claimed in any preceding claim, further comprising displaying said image or other data or data derived from said image or other data so as to assist a user to manually guide or direct one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or said first device.

98. A method as claimed in claim 97, wherein the step of displaying said image or other data or data derived from said image or other data comprises using an indirect conversion detector.

99. A method as claimed in claim 98, wherein said indirect conversion detector converts incident X-ray photons into optical photons and then converts said optical photons into electrical charge.

100. A method as claimed in claim 97, wherein the step of displaying said image or other data or data derived from said image data comprises using a fluoroscopy device or a scintillator.

101. A method as claimed in claim 100, wherein said scintillator comprises a cesium iodide ("CsI") layer or a gadolinium oxysulfide ("GOS") layer.

102. A method as claimed in any preceding claim, further comprising using one or more image intensifiers to intensify said image or other data or data derived from said image or other data for displaying to a user.

103. A method as claimed in claim 97, wherein the step of displaying said image or other data or data derived from said image or other data comprises using a direct conversion detector.

104. A method as claimed in claim 103, wherein said direct conversion detector comprises a photoconductor which converts incident X-ray photons directly into electrical charge.

105. A method as claimed in claim 104, wherein said photoconductor comprises amorphous selenium ("a-Se"), cadmium telluride ("CdTe"), lead oxide ("PbO") or silicon ("Si").

106. A method as claimed in any preceding claim, further comprising manually, automatically or robotically guiding or directing one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or said first device using a guidance system.

5

107. A method as claimed in claim 106, wherein said guidance system comprises a magnetic resonance imaging ("MRI") guidance system.

108. A method as claimed in claim 106, wherein said guidance system comprises an ultrasound or ultrasonic guidance system.

10

109. A method as claimed in claim 108, wherein said ultrasound or ultrasonic guidance system comprises an intraoperative ultrasound ("IOUS") guidance system.

110. A method as claimed in claim 106, wherein said guidance system comprises a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device.

15

111. A method as claimed in claim 106, wherein said guidance system comprises a radioguided occult lesion localization ("ROLL") guidance system.

20

112. A method as claimed in claim 106, further comprising injecting a nuclear radiotracer at one or more target regions.

113. A method as claimed in claim 112, wherein said nuclear radiotracer comprises ^{99m}Tc .

25

114. A method as claimed in claim 112 or 113, further comprising using a gamma ray detection probe to detect gamma rays emitted by the decay of said nuclear radiotracer thereby enabling said target region to be located and/or visualised.

30

115. A method as claimed in claim 106, wherein said guidance system comprises radioactive seed localization ("RSL") system.

116. A method as claimed in claim 115, further comprising inserting, injecting or implanting one or more radioactive seeds into said target.

35

117. A method as claimed in claim 116, wherein said one or more radioactive seeds comprise a titanium shell.

40

118. A method as claimed in claim 117, wherein said titanium shell houses ^{125}I .

119. A method as claimed in any of claims 116, 117 or 118, further comprising using a gamma ray detection probe to detect gamma rays emitted by the decay of said radioactive seed thereby enabling a target region of interest to be located and/or visualised.

5

120. A method as claimed in claim 106, wherein said guidance system comprises a mammography guidance system.

121. A method as claimed in claim 106, wherein said guidance system comprises a computed tomography ("CT") guidance system.

10

122. A method as claimed in claim 106, wherein said guidance system comprises a positron emission tomography ("PET") guidance system.

123. A method as claimed in claim 106, wherein said guidance system comprises a radiographic guidance system.

15

124. A method as claimed in claim 106, wherein said guidance system comprises a magnetic or magnetism sensing guidance system or a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles or a guidance system for detecting nanoparticles.

20

125. A method as claimed in any preceding claim, further comprising using said image or other data to determine the margins or bounds of one or more regions of interest of said target.

25

126. A method as claimed in any preceding claim, wherein said one or more regions of interest comprise cancerous biological tissue or a tumour.

127. A method as claimed in claim 126, wherein said cancerous biological tissue or said tumour comprises either: (i) grade I, grade II, grade III or grade IV cancerous tissue; (ii) metastatic cancerous tissue; (iii) mixed grade cancerous tissue; or (iv) a sub-grade cancerous tissue.

30

128. A method of ambient ionisation comprising a method as claimed in any preceding claim.

35

129. A method of rapid evaporation ionization mass spectrometry ("REIMS") comprising a method as claimed in any of claims 1-127.

40

130. A method of analysis comprising a method as claimed in any of claims 1-127.

131. A method of surgery, diagnosis, therapy or medical treatment comprising a method as claimed in any of claims 1-127.

132. A non-surgical, non-therapeutic method of mass spectrometry and/or method
5 of ion mobility spectrometry comprising a method as claimed in any of claims 1-127.

133. A method of mass spectrometry and/or method of ion mobility spectrometry comprising a method as claimed in any of claims 1-127.

10 134. Apparatus comprising:
a device arranged and adapted to obtain or acquire image or other data from one or more regions of a target;
a control system arranged and adapted to use said image or other data to determine one or more regions of interest of said target; and
15 a first device for generating aerosol, smoke or vapour from one or more regions of said target.

135. Apparatus as claimed in claim 134, wherein said image or other data comprises data selected from the group consisting of: (i) thermal, temperature or
20 thermographic image data; (ii) microwave image data; (iii) visual or optical image data; (iv) infra-red ("IR") image data; (v) radio-frequency ("RF") image data; (vi) X-ray image data; (vii) magnetic resonance imaging ("MRI") image data; (viii) ultrasonic or ultrasound image data; (ix) tomographic image data; (x) optical or other absorption data; (xi) optical or other scattering coefficient data; (xii) oxyhemoglobin or
25 deoxyhemoglobin absorbance data; (xiii) near infrared (NIR) image data; or (xiv) magnetic data.

136. Apparatus as claimed in claim 134 or 135, wherein said first device comprises or forms part of an ambient ion or ionisation source or wherein said first device
30 generates said aerosol, smoke or vapour for subsequent ionisation by an ambient ion or ionisation source or other ionisation source.

137. Apparatus as claimed in any of claims 134, 135 or 136, wherein said target comprises native or unmodified target material.
35

138. Apparatus as claimed in claim 137, wherein said native or unmodified target material is unmodified by the addition of a matrix or reagent.

139. Apparatus as claimed in any of claims 134-138, wherein said first device is
40 arranged and adapted to generate aerosol, smoke or vapour from one or more regions of said target without said target requiring prior preparation.

140. Apparatus as claimed in any of claims 134-139, wherein said first device comprises an ion source selected from the group consisting of: (i) a rapid evaporative ionisation mass spectrometry ("REIMS") ion source; (ii) a desorption electrospray ionisation ("DESI") ion source; (iii) a laser desorption ionisation ("LDI") ion source; (iv) a thermal desorption ion source; (v) a laser diode thermal desorption ("LDTD") ion source; (vi) a desorption electro-flow focusing ("DEFFI") ion source; (vii) a dielectric barrier discharge ("DBD") plasma ion source; (viii) an Atmospheric Solids Analysis Probe ("ASAP") ion source; (ix) an ultrasonic assisted spray ionisation ion source; (x) an easy ambient sonic-spray ionisation ("EASI") ion source; (xi) a desorption atmospheric pressure photoionisation ("DAPPI") ion source; (xii) a paperspray ("PS") ion source; (xiii) a jet desorption ionisation ("JeDI") ion source; (xiv) a touch spray ("TS") ion source; (xv) a nano-DESI ion source; (xvi) a laser ablation electrospray ("LAESI") ion source; (xvii) a direct analysis in real time ("DART") ion source; (xviii) a probe electrospray ionisation ("PESI") ion source; (xix) a solid-probe assisted electrospray ionisation ("SPA-ESI") ion source; (xx) a cavitron ultrasonic surgical aspirator ("CUSA") device; (xxi) a focussed or unfocussed ultrasonic ablation device; (xxii) a microwave resonance device; and (xxiii) a pulsed plasma RF dissection device.
141. Apparatus as claimed in any of claims 134-140, wherein said first device is arranged and adapted to generate aerosol, smoke or vapour from one or more regions of said target by contacting said target with one or more electrodes.
142. Apparatus as claimed in claim 141, wherein said one or more electrodes comprise: (i) a monopolar device, wherein the apparatus optionally further comprises a separate return electrode; (ii) a bipolar device; or (iii) a multi phase RF device, wherein the apparatus optionally further comprises a separate return electrode or electrodes.
143. Apparatus as claimed in claim 141 or 142, wherein said one or more electrodes comprise a rapid evaporation ionization mass spectrometry ("REIMS") device.
144. Apparatus as claimed in any of claims 141, 142 or 143, further comprising a device arranged and adapted to apply an AC or RF voltage to said one or more electrodes in order to generate said aerosol, smoke or vapour.
145. Apparatus as claimed in claim 144, wherein said device for applying said AC or RF voltage to said one or more electrodes is arranged to apply one or more pulses of said AC or RF voltage to said one or more electrodes.

146. Apparatus as claimed in claim 144 or 145, wherein application of said AC or RF voltage to said one or more electrodes causes heat to be dissipated into said target.

5 147. Apparatus as claimed in any of claims 134-140, wherein said first device comprises a laser for irradiating said target.

148. Apparatus as claimed in any of claims 134-147, wherein said first device is arranged and adapted to generate aerosol from one or more regions of said target by
10 direct evaporation or vaporisation of target material from said target by Joule heating or diathermy.

149. Apparatus as claimed in any of claims 134-148, wherein said first device is arranged and adapted to direct ultrasonic energy into said target.

15

150. Apparatus as claimed in any of claims 134-149, wherein said aerosol comprises uncharged aqueous droplets optionally comprising cellular material.

151. Apparatus as claimed in any of claims 134-150, wherein at least 50%, 55%,
20 60%, 65%, 70%, 75%, 80%, 85%, 90% or 95% of the mass or matter generated by said first device and which forms said aerosol is in the form of droplets.

152. Apparatus as claimed in any of claims 134-151, wherein said first device is arranged and adapted to generate aerosol wherein the Sauter mean diameter
25 ("SMD", d_{32}) of said aerosol is in a range: (i) $< 5 \mu\text{m}$; (ii) $5\text{-}10 \mu\text{m}$; (iii) $10\text{-}15 \mu\text{m}$; (iv) $15\text{-}20 \mu\text{m}$; (v) $20\text{-}25 \mu\text{m}$; or (vi) $> 25 \mu\text{m}$.

153. Apparatus as claimed in any of claims 134-152, wherein said aerosol traverses a flow region with a Reynolds number (Re) in the range: (i) < 2000 ; (ii)
30 $2000\text{-}2500$; (iii) $2500\text{-}3000$; (iv) $3000\text{-}3500$; (v) $3500\text{-}4000$; or (vi) > 4000 .

154. Apparatus as claimed in any of claims 134-153, wherein substantially at the point of generating said aerosol, said aerosol comprises droplets having a Weber number (We) selected from the group consisting of: (i) < 50 ; (ii) $50\text{-}100$; (iii) $100\text{-}150$;
35 (iv) $150\text{-}200$; (v) $200\text{-}250$; (vi) $250\text{-}300$; (vii) $300\text{-}350$; (viii) $350\text{-}400$; (ix) $400\text{-}450$; (x) $450\text{-}500$; (xi) $500\text{-}550$; (xii) $550\text{-}600$; (xiii) $600\text{-}650$; (xiv) $650\text{-}700$; (xv) $700\text{-}750$; (xvi) $750\text{-}800$; (xvii) $800\text{-}850$; (xviii) $850\text{-}900$; (xix) $900\text{-}950$; (xx) $950\text{-}1000$; and (xxi) > 1000 .

40 155. Apparatus as claimed in any of claims 134-154, wherein substantially at the point of generating said aerosol, said aerosol comprises droplets having a Stokes

number (S_k) in the range: (i) 1-5; (ii) 5-10; (iii) 10-15; (iv) 15-20; (v) 20-25; (vi) 25-30; (vii) 30-35; (viii) 35-40; (ix) 40-45; (x) 45-50; and (xi) > 50.

156. Apparatus as claimed in any of claims 134-155, wherein substantially at the point of generating said aerosol, said aerosol comprises droplets having a mean axial velocity selected from the group consisting of: (i) < 20 m/s; (ii) 20-30 m/s; (iii) 30-40 m/s; (iv) 40-50 m/s; (v) 50-60 m/s; (vi) 60-70 m/s; (vii) 70-80 m/s; (viii) 80-90 m/s; (ix) 90-100 m/s; (x) 100-110 m/s; (xi) 110-120 m/s; (xii) 120-130 m/s; (xiii) 130-140 m/s; (xiv) 140-150 m/s; and (xv) > 150 m/s.

10

157. Apparatus as claimed in any of claims 134-156, wherein said target comprises biological tissue, biological matter, a bacterial colony or a fungal colony.

158. Apparatus as claimed in claim 157, wherein said biological tissue comprises human tissue or non-human animal tissue.

15

159. Apparatus as claimed in claim 157 or 158, wherein said biological tissue comprises *in vivo* biological tissue.

160. Apparatus as claimed in claim 157 or 158, wherein said biological tissue comprises *ex vivo* biological tissue.

20

161. Apparatus as claimed in claim 157 or 158, wherein said biological tissue comprises *in vitro* biological tissue.

25

162. Apparatus as claimed in any of claims 157-161, wherein said biological tissue comprises: (i) adrenal gland tissue, appendix tissue, bladder tissue, bone, bowel tissue, brain tissue, breast tissue, bronchi, coronal tissue, ear tissue, esophagus tissue, eye tissue, gall bladder tissue, genital tissue, heart tissue, hypothalamus tissue, kidney tissue, large intestine tissue, intestinal tissue, larynx tissue, liver tissue, lung tissue, lymph nodes, mouth tissue, nose tissue, pancreatic tissue, parathyroid gland tissue, pituitary gland tissue, prostate tissue, rectal tissue, salivary gland tissue, skeletal muscle tissue, skin tissue, small intestine tissue, spinal cord, spleen tissue, stomach tissue, thymus gland tissue, trachea tissue, thyroid tissue, ureter tissue, urethra tissue, soft and connective tissue, peritoneal tissue, blood vessel tissue and/or fat tissue; (ii) grade I, grade II, grade III or grade IV cancerous tissue; (iii) metastatic cancerous tissue; (iv) mixed grade cancerous tissue; (v) a sub-grade cancerous tissue; (vi) healthy or normal tissue; or (vii) cancerous or abnormal tissue.

30

35

163. Apparatus as claimed in any of claims 134-162, wherein said first device comprises a point of care ("POC"), diagnostic or surgical device.

40

164. Apparatus as claimed in any of claims 134-163, further comprising a device for ionising at least some of the aerosol, smoke or vapour so as to generate analyte ions.

5 165. Apparatus as claimed in any of claims 134-164, further comprising a device arranged and adapted to direct or aspirate at least some of the aerosol, smoke or vapour into a vacuum chamber of a mass spectrometer and/or ion mobility spectrometer.

10 166. Apparatus as claimed in claim 165, further comprising a device arranged and adapted to ionise at least some the aerosol, smoke or vapour within a or the vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

15 167. Apparatus as claimed in claim 166, further comprising a device arranged and adapted to cause the aerosol, smoke or vapour to impact upon a collision surface located within a vacuum chamber of the mass spectrometer and/or ion mobility spectrometer so as to generate a plurality of analyte ions.

20 168. Apparatus as claimed in claim 164, 165 or 167, further comprising a mass analyser for mass analysing and/or ion mobility analyser for ion mobility analysing the analyte ions in order to obtain mass spectrometric data and/or ion mobility data.

25 169. Apparatus as claimed in any of claims 134-168, further comprising a mass analyser for mass analysing and/or ion mobility analyser for ion mobility analysing the aerosol, smoke or vapour or ions derived from the aerosol, smoke or vapour in order to obtain mass spectrometric data and/or ion mobility data.

30 170. Apparatus as claimed in claim 168 or 169, wherein said mass analyser and/or ion mobility analyser is arranged and adapted to analyse the mass spectrometric data and/or ion mobility data in order either: (i) to distinguish between healthy and diseased tissue; (ii) to distinguish between potentially cancerous and non-cancerous tissue; (iii) to distinguish between different types or grades of cancerous tissue; (iv) to distinguish between different types or classes of target material; (v) to determine
35 whether or not one or more desired or undesired substances are present in the target; (vi) to confirm the identity or authenticity of the target; (vii) to determine whether or not one or more impurities, illegal substances or undesired substances are present in the target; (viii) to determine whether a human or animal patient is at an increased risk of suffering an adverse outcome; (ix) to make or assist in the
40 making a diagnosis or prognosis; and (x) to inform a surgeon, nurse, medic or robot of a medical, surgical or diagnostic outcome.

171. Apparatus as claimed in claim 168, 169 or 170, further comprising a device which is arranged and adapted to analyse one or more sample spectra so as to classify an aerosol, smoke or vapour sample.

5 172. Apparatus as claimed in claim 171, further comprising a device which is arranged and adapted to perform supervised analysis of the one or more sample spectra and/or unsupervised analysis of the one or more sample spectra.

10 173. Apparatus as claimed in claim 171 or 172, wherein said device for analysing the one or more sample spectra so as to classify the aerosol, smoke or vapour sample uses one or more of: univariate analysis; multivariate analysis; principal component analysis (PCA); linear discriminant analysis (LDA); maximum margin criteria (MMC); library-based analysis; soft independent modelling of class analogy (SIMCA); factor analysis (FA); recursive partitioning (decision trees); random forests;
15 independent component analysis (ICA); partial least squares discriminant analysis (PLS-DA); orthogonal (partial least squares) projections to latent structures (OPLS); OPLS discriminant analysis (OPLS-DA); support vector machines (SVM); (artificial) neural networks; multilayer perceptron; radial basis function (RBF) networks; Bayesian analysis; cluster analysis; a kernelized method; and subspace discriminant
20 analysis.

174. Apparatus as claimed in claim 171, 172 or 173, further comprising a device which is arranged and adapted to develop a classification model or library using one or more reference sample spectra.
25

175. Apparatus as claimed in any of claims 171-174, further comprising a device for performing linear discriminant analysis (LDA) after performing principal component analysis (PCA).

30 176. Apparatus as claimed in any of claims 171-175, further comprising a device for performing a maximum margin criteria (MMC) process after performing principal component analysis (PCA).

35 177. Apparatus as claimed in any of claims 171-176, further comprising a device for defining one or more classes within a classification model or library.

178. Apparatus as claimed in any of claims 171-177, further comprising a device for defining one or more classes within a classification model or library manually or automatically according to one or more class or cluster criteria.
40

179. Apparatus as claimed in claim 178, wherein the one or more class or cluster criteria for each class are based on one or more of: a distance between one or more

pairs of reference points for reference sample spectra within a model space; a variance value between groups of reference points for reference sample spectra within a model space; and a variance value within a group of reference points for reference sample spectra within a model space.

5

180. Apparatus as claimed in claim 177, 178 or 179, wherein the one or more classes are each defined by one or more class definitions.

10

181. Apparatus as claimed in claim 180, wherein the one or more class definitions comprise one or more of: a set of one or more reference points for reference sample spectra, values, boundaries, lines, planes, hyperplanes, variances, volumes, Voronoi cells, and/or positions, within a model space; and one or more positions within a class hierarchy.

15

182. Apparatus as claimed in any of claims 171-181, further comprising a device which is arranged and adapted to use a classification model or library to classify one or more unknown sample spectra.

20

183. Apparatus as claimed in any of claims 171-182, further comprising a device for classifying one or more sample spectra according to one or more classification criteria.

25

184. Apparatus as claimed in claim 183, wherein the one or more classification criteria comprise one or more of:

a distance between one or more projected sample points for one or more sample spectra within a model space and a set of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, volumes, Voronoi cells, or positions, within the model space being below a distance threshold or being the lowest such distance;

30

a position for one or more projected sample points for one or more sample spectra within a model space being one side or other of one or more reference points for one or more reference sample spectra, values, boundaries, lines, planes, hyperplanes, or positions, within the model space;

35

a position for one or more projected sample points for one or more sample spectra within a model space being within one or more volumes or Voronoi cells within the model space; and

a probability or classification score being above a probability or classification score threshold or being the highest such probability or classification score.

40

185. Apparatus as claimed in any of claims 171-184, further comprising a device for analysing a profile of the aerosol, smoke or vapour or a profile of ions derived from the aerosol, smoke or vapour.

186. Apparatus as claimed in claim 185, wherein the profile is selected from the group consisting of: (i) a lipidomic profile; (ii) a fatty acid profile; (iii) a phospholipid profile; (iv) a phosphatidic acid (PA) profile; (v) a phosphatidylethanolamine (PE) profile; (vi) a phosphatidylglycerol (PG) profile; (vii) a phosphatidylserines (PS) profile; (viii) a phosphatidylinositol (PI) profile; or (ix) a triglyceride (TG) profile.

187. Apparatus as claimed in any of claims 134-186, further comprising one or more thermal or temperature sensors, detectors or devices for obtaining the image or other data.

188. Apparatus as claimed in claim 187, wherein the one or more thermal or temperature sensors, detectors or devices are selected from the group consisting of: (i) one or more temperature sensors; (ii) one or more thermal imaging sensors; (iii) one or more infrared thermography ("IRT") sensors; and (iv) one or more infrared imaging sensors.

189. Apparatus as claimed in claim 187 or 188, wherein the one or more thermal or temperature sensors, detectors or devices are arranged to obtain the image or other data with or without the one or more thermal or temperature sensors, detectors or devices physically contacting the target.

190. Apparatus as claimed in any of claims 187, 188 or 189, further comprising a device for determining a temperature, temperature profile or thermographic image of one or more regions of the target.

191. Apparatus as claimed in any of claims 187-190, further comprising a device for determining one or more regions of the target which have a different temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

192. Apparatus as claimed in any of claims 187-191, further comprising a device for determining whether or not a region of the target has a higher or lower temperature, temperature profile or thermographic image intensity relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

193. Apparatus as claimed in any of claims 187-192, further comprising a device for determining one or more hyperthermic or hypothermic regions of the target.

194. Apparatus as claimed in any of claims 134-193, further comprising one or more microwave or RF sensors, detectors or devices for obtaining the image or other data.

5 195. Apparatus as claimed in claim 194, wherein the one or more microwave or RF sensors, detectors or devices comprise one or more microwave reflectrometry sensors, detectors or devices.

10 196. Apparatus as claimed in claim 195, wherein said one or more microwave reflectrometry sensors are arranged and adapted to physically contact the target.

197. Apparatus as claimed in claim 195 or 196, further comprising one or more microwave reflectrometry sensors for determining a fluid content of one or more regions of the target.

15

198. Apparatus as claimed in any of claims 187-197, further comprising a device for determining one or more regions of the target which have a different fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

20

199. Apparatus as claimed in any of claims 187-198, further comprising a device for determining whether or not a region of the target has a higher or lower fluid content relative to normal tissue, surrounding tissue, a control sample, a control region, control data or predetermined data.

25

200. Apparatus as claimed in any of claims 134-199, further comprising an optical coherence tomography ("OCT") device for obtaining the image or other data.

30 201. Apparatus as claimed in claim 200, further comprising a low coherence light source ("LCS"), a super-luminescent diode ("SLD"), a swept source or tunable laser ("SS"), an ultra-short pulsed laser or a supercontinuum laser for illuminating the target.

35 202. Apparatus as claimed in claim 200 or 201, wherein the optical coherence tomography device comprises an interferometer.

203. Apparatus as claimed in any of claims 134-202, further comprising one or more computed tomography devices for obtaining the image or other data.

40 204. Apparatus as claimed in any of claims 134-203, further comprising a positron emission tomography ("PET") device for obtaining the image or other data.

205. Apparatus as claimed in any of claims 134-204, further comprising a magnetic resonance imaging ("MRI") device for obtaining the image or other data.

5 206. Apparatus as claimed in any of claims 134-205, further comprising one or more ultrasonic tomography devices for obtaining the image or other data.

207. Apparatus as claimed in any of claims 134-206, further comprising one or more optical imaging sensors, detectors or devices for obtaining the image or other data.

10

208. Apparatus as claimed in claim 207, further comprising a continuous wave (CW) light source for illuminating the target.

15 209. Apparatus as claimed in claim 207, further comprising a time domain photon migration (TDPM) imaging system to obtain the image or other data.

210. Apparatus as claimed in claim 207, further comprising a frequency-domain photon migration (FDPM) imaging system for obtaining the image or other data.

20 211. Apparatus as claimed in any of claims 134-210, further comprising one or more contrast agents for enhancing the image data.

212. Apparatus as claimed in claim 211, wherein the one or more contrast agents comprise one or more fluorescent contrast agents.

25

213. Apparatus as claimed in claim 211 or 212, wherein the one or more contrast agents comprise one or more visible dyes.

30 214. Apparatus as claimed in claim 211, 212 or 213, wherein the one or more contrast agents comprise one or more radiocontrast agents.

215. Apparatus as claimed in any of claims 211-214, wherein the one or more contrast agents comprise one or more optical, near infrared ("NIR"), fluorescent, autofluorescent or diagnostic contrast agents.

35

216. Apparatus as claimed in any of claims 211-215, wherein the one or more contrast agents are selected from the group consisting of: (i) indocyanine green ("ICG") and derivatives or conjugates of indocyanine green including indotricarbocyanine; (ii) diethylthiatricarbocyanine iodide ("DTTCI") and derivatives or
40 conjugates of diethylthiatricarbocyanine iodide; (iii) rhodamine B and derivatives or conjugates of rhodamine B; (iv) photodynamic therapy ("PDT") agents including

hexylpyropheophorbide ("HPPH"); (v) a cyanine dye including Cy 5.5 dyes; and (vi) bifunctional contrast agents.

217. Apparatus as claimed in any of claims 211-216, wherein the one or more contrast agents comprise nanoparticles.

218. Apparatus as claimed in claim 217, wherein the one or more contrast agents comprise: (i) magnetic or ferromagnetic nanoparticles; (ii) gold nanoparticles; (iii) metallic nanoparticles; (iv) functionalised nanoparticles; (v) nanospheres, nanorods, nanostars or nanoshells; (vi) levan nanoparticles; or (vii) copper, zinc, titanium, magnesium, alginate, alloy or silver nanoparticles.

219. Apparatus as claimed in any of claims 211-218, wherein the one or more contrast agents are exogenous to the target.

220. Apparatus as claimed in any of claims 211-218, wherein the one or more contrast agents are endogenous to the target.

221. Apparatus as claimed in any of claims 134-220, further comprising an X-ray scattering device for obtaining the image or other data.

222. Apparatus as claimed in claim 221, further comprising a device for directing X-rays onto one or more regions of the target.

223. Apparatus as claimed in claim 222, further comprising a device for measuring the wavelength or frequency of scattered X-rays from the target.

224. Apparatus as claimed in claim 221, 222 or 223, wherein the X-ray scattering device comprises a Compton X-ray scattering device.

225. Apparatus as claimed in claim 224, wherein the Compton X-ray scattering device is arranged to measure scattered signals due to incoherent X-ray scattering.

226. Apparatus as claimed in claim 224 or 225, wherein the X-rays have an energy ≥ 50 keV.

227. Apparatus as claimed in claim 221, 222 or 223, wherein the X-ray scattering device comprises a Rayleigh X-ray scattering device.

228. Apparatus as claimed in claim 227, wherein the Rayleigh X-ray scattering device is arranged to measure scattered signals due to coherent X-ray scattering.

229. Apparatus as claimed in claim 227 or 228, wherein the X-rays have an energy ≤ 30 keV.

230. Apparatus as claimed in any of claims 134-229, further comprising a device
5 for displaying the image or other data or data derived from the image or other data so as to assist a user to manually guide or direct one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device.

231. Apparatus as claimed in claim 230, further comprising an indirect conversion
10 detector for displaying said image or other data or data derived from said image or other data.

232. Apparatus as claimed in claim 231, wherein the indirect conversion detector is
15 arranged and adapted to convert incident X-ray photons into optical photons and then convert the optical photons into electrical charge.

233. Apparatus as claimed in claim 232, further comprising a fluoroscopy device or a scintillator for displaying the image or other data or data derived from the image data.

20 234. Apparatus as claimed in claim 233, wherein the scintillator comprises a cesium iodide ("CsI") layer or a gadolinium oxysulfide ("GOS") layer.

235. Apparatus as claimed in any of claims 134-234, further comprising one or more image intensifiers for intensifying the image or other data or data derived from
25 the image or other data for displaying to a user.

236. Apparatus as claimed in claim 230, further comprising a direct conversion
30 detector for displaying the image or other data or data derived from the image or other data.

237. Apparatus as claimed in claim 236, wherein the direct conversion detector comprises a photoconductor which converts incident X-ray photons directly into electrical charge.

35 238. Apparatus as claimed in claim 237, wherein the photoconductor comprises amorphous selenium ("a-Se"), cadmium telluride ("CdTe"), lead oxide ("PbO") or silicon ("Si").

239. Apparatus as claimed in any of claims 134-238, further comprising a guidance
40 system for manually, automatically or robotically guiding or directing one or more probes, surgical tools, diagnostic tools, ambient ionisation ion sources or the first device using.

240. Apparatus as claimed in claim 239, wherein the guidance system comprises a magnetic resonance imaging ("MRI") guidance system.

5 241. Apparatus as claimed in claim 239, wherein the guidance system comprises an ultrasound or ultrasonic guidance system.

242. Apparatus as claimed in claim 241, wherein the ultrasound or ultrasonic guidance system comprises an intraoperative ultrasound ("IOUS") guidance system.

10

243. Apparatus as claimed in claim 239, wherein the guidance system comprises a guidewire localization ("GWL"), a wire localization ("WL") or a wire-guided localization ("WGL") device.

15 244. Apparatus as claimed in claim 239, wherein the guidance system comprises a radioguided occult lesion localization ("ROLL") guidance system.

245. Apparatus as claimed in claim 239, further comprising a device for injecting a nuclear radiotracer at one or more target regions.

20

246. Apparatus as claimed in claim 245, wherein the nuclear radiotracer comprises ^{99m}Tc .

25

247. Apparatus as claimed in claim 245 or 246, further comprising a gamma ray detection probe for detecting gamma rays emitted by the decay of the nuclear radiotracer thereby enabling the target region to be located and/or visualised.

248. Apparatus as claimed in claim 239, wherein the guidance system comprises radioactive seed localization ("RSL") system.

30

249. Apparatus as claimed in claim 239, further comprising a device for inserting, injecting or implanting one or more radioactive seeds into the target.

35

250. Apparatus as claimed in claim 249, wherein the one or more radioactive seeds comprise a titanium shell.

251. Apparatus as claimed in claim 250, wherein the titanium shell houses ^{125}I .

40

252. Apparatus as claimed in any of claims 249, 250 or 251, further comprising a gamma ray detection probe for detecting gamma rays emitted by the decay of the radioactive seed thereby enabling a target region of interest to be located and/or visualised.

253. Apparatus as claimed in claim 239, wherein the guidance system comprises a mammography guidance system.

5 254. Apparatus as claimed in claim 239, wherein the guidance system comprises a computed tomography ("CT") guidance system.

255. Apparatus as claimed in claim 239, wherein the guidance system comprises a positron emission tomography ("PET") guidance system.

10

256. Apparatus as claimed in claim 239, wherein the guidance system comprises a radiographic guidance system.

15

257. Apparatus as claimed in claim 239, wherein the guidance system comprise a magnetic or magnetism sensing guidance system or a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles or a guidance system for detecting nanoparticles.

20

258. Apparatus as claimed in any of claims 134-257, further comprising a device for using the image or other data to determine the margins or bounds of one or more regions of interest of the target.

25

259. Apparatus as claimed in any of claims 134-258, wherein the one or more regions of interest comprise cancerous biological tissue or a tumour.

30

260. Apparatus as claimed in claim 259, wherein the cancerous biological tissue or the tumour comprises either: (i) grade I, grade II, grade III or grade IV cancerous tissue; (ii) metastatic cancerous tissue; (iii) mixed grade cancerous tissue; or (iv) a sub-grade cancerous tissue.

35

261. An ambient ionisation ion source comprising apparatus as claimed in any of claims 134-260.

262. A rapid evaporative ionization mass spectrometry ("REIMS") ion source as claimed in any of claims 134-260.

263. A mass spectrometer and/or ion mobility spectrometer comprising apparatus as claimed in any of claims 134-260.

40

264. A method comprising:
using a navigational device or system to guide or direct a first device to one or more regions of a target; and

using said first device to generate aerosol, smoke or vapour from one or more regions of said target.

265. A method as claimed in claim 264, wherein said navigational device is
5 selected from the group consisting of: (i) a magnetic resonance imaging ("MRI")
navigational device; (ii) an ultrasound or ultrasonic navigational device; (iii) an X-ray
navigational device; (iv) a radioactivity detecting navigational device for detecting
radioactive particles or radioactive nanoparticles; (v) an intraoperative ultrasound
("IOUS") guidance system; (vi) a guidewire localization ("GWL"), a wire localization
10 ("WL") or a wire-guided localization ("WGL") device; (vii) a radioguided occult lesion
localization ("ROLL") guidance system; (viii) a radioactive seed localization ("RSL")
system; (ix) a mammography guidance system; (x) a computed tomography ("CT")
guidance system; (xi) a positron emission tomography ("PET") guidance system; (xii)
a radiographic guidance system; (xiii) a magnetic or magnetism sensing guidance
15 system; (xiv) a superconducting quantum interference device ("SQUID") guidance
system for detecting magnetic particles or magnetic nanoparticles; and (xv) a
guidance system for detecting nanoparticles.

266. A method as claimed in claim 264 or 265, further comprising manually
20 operating or guiding said navigational device or system.

267. A method as claimed in claim 264 or 265, further comprising robotically or
automatically operating or guiding said navigational device or system.

25 268. A method of mass spectrometry and/or method of ion mobility spectrometry
comprising a method as claimed in any of claims 264-267.

269. Apparatus comprising:
a first device for generating aerosol, smoke or vapour from one or more
30 regions of a target; and
a navigational device or system arranged and adapted to guide or direct said
first device to one or more regions of said target.

270. Apparatus as claimed in claim 269, wherein said navigational device is
35 selected from the group consisting of: (i) a magnetic resonance imaging ("MRI")
navigational device; (ii) an ultrasound or ultrasonic navigational device; (iii) an X-ray
navigational device; (iv) a radioactivity detecting navigational device for detecting
radioactive particles or radioactive nanoparticles; (v) an intraoperative ultrasound
("IOUS") guidance system; (vi) a guidewire localization ("GWL"), a wire localization
40 ("WL") or a wire-guided localization ("WGL") device; (vii) a radioguided occult lesion
localization ("ROLL") guidance system; (viii) a radioactive seed localization ("RSL")
system; (ix) a mammography guidance system; (x) a computed tomography ("CT")

- guidance system; (xi) a positron emission tomography ("PET") guidance system; (xii) a radiographic guidance system; (xiii) a magnetic or magnetism sensing guidance system; (xiv) a superconducting quantum interference device ("SQUID") guidance system for detecting magnetic particles or magnetic nanoparticles; and (xv) a
- 5 guidance system for detecting nanoparticles.

271. Apparatus as claimed in claim 269 or 270, further comprising manually operating or guiding said navigational device or system.

- 10 272. Apparatus as claimed in claim 269 or 270, further comprising a robotic or automatic guidance system for robotically or automatically operating or guiding said navigational device or system.

- 15 273. A mass spectrometry and/or ion mobility spectrometry system comprising apparatus as claimed in any of claims 269-272 in combination with a mass spectrometer and/or ion mobility spectrometer.

Fig. 1


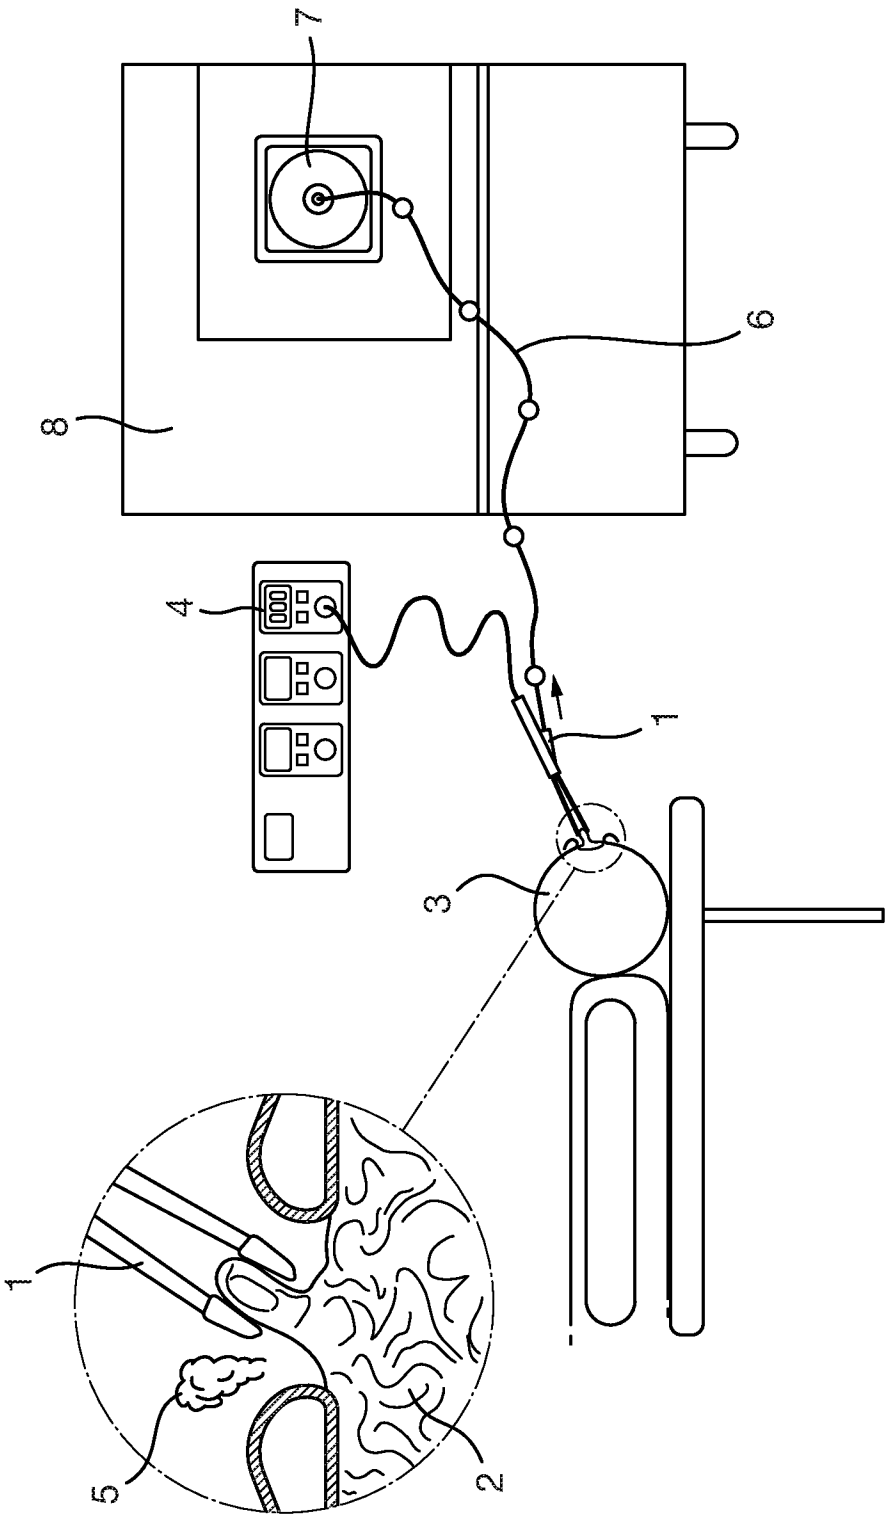


Fig. 2

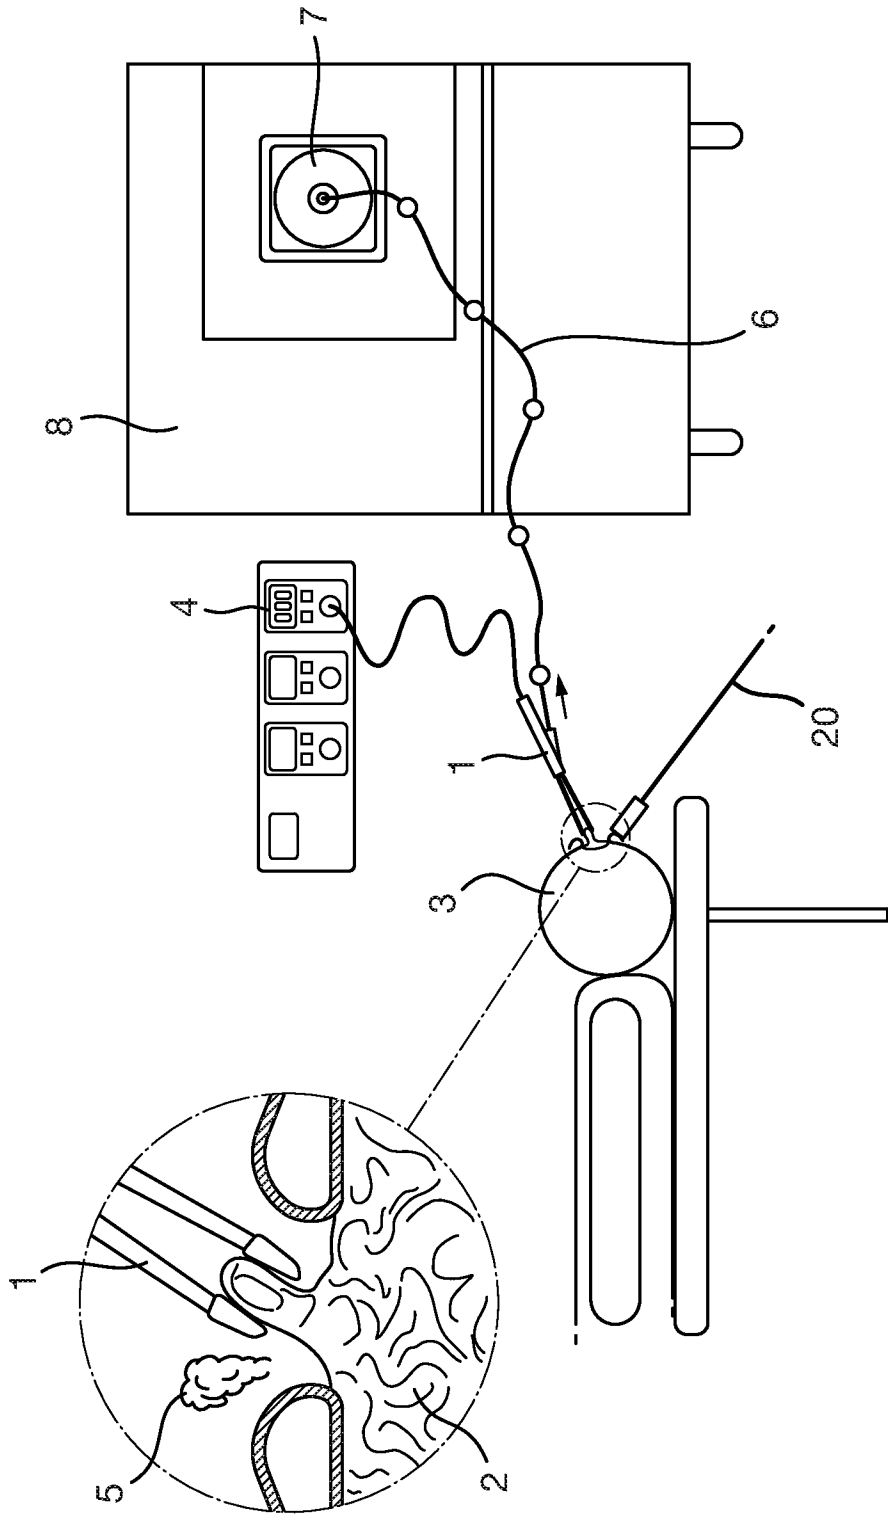

3/9

Fig. 3

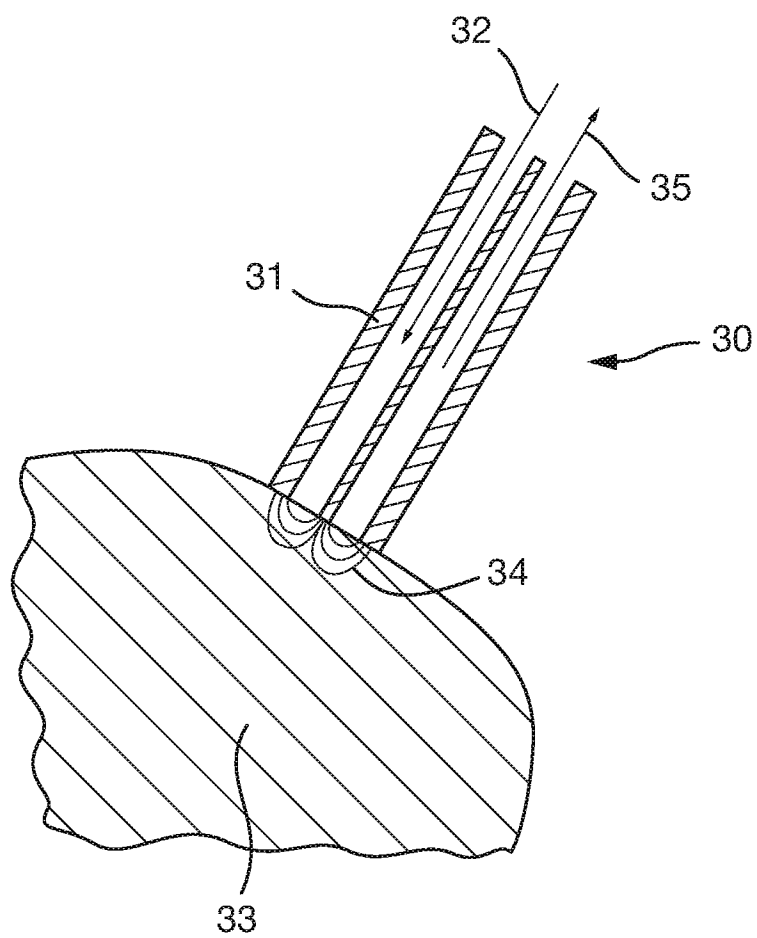


Fig. 4

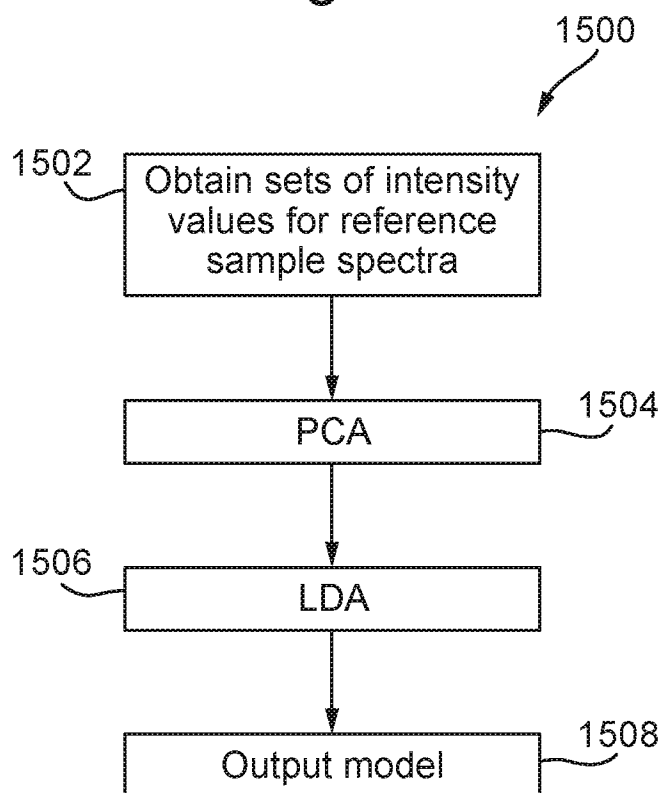


Fig. 5

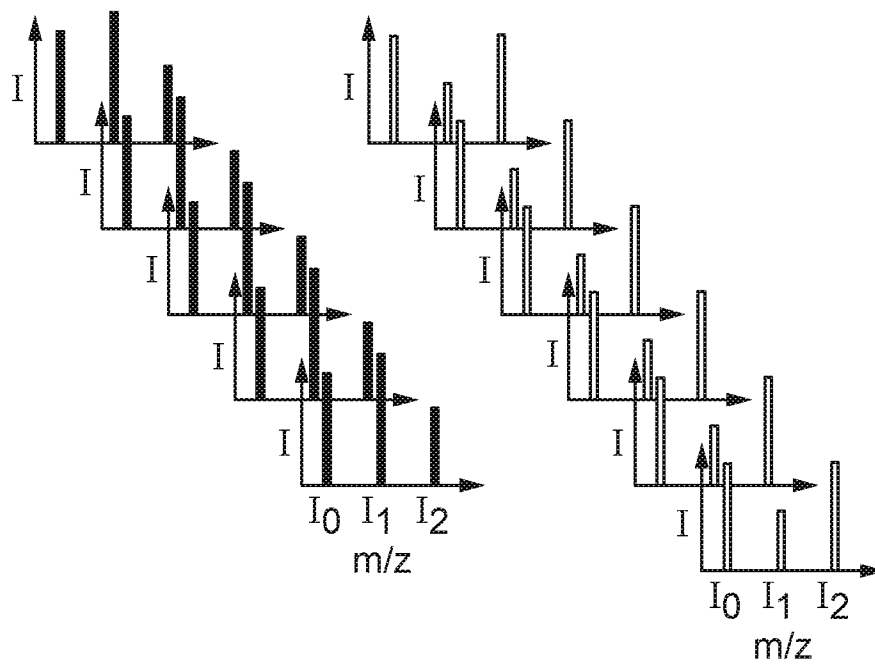


Fig. 6

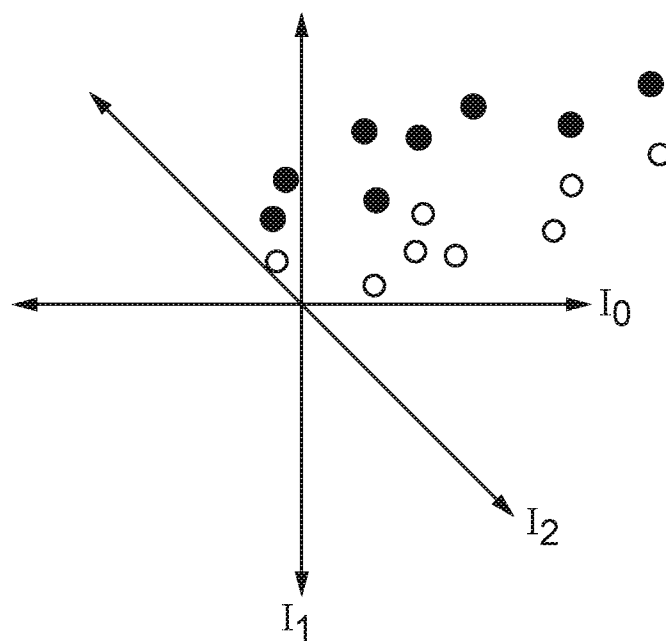


Fig. 7


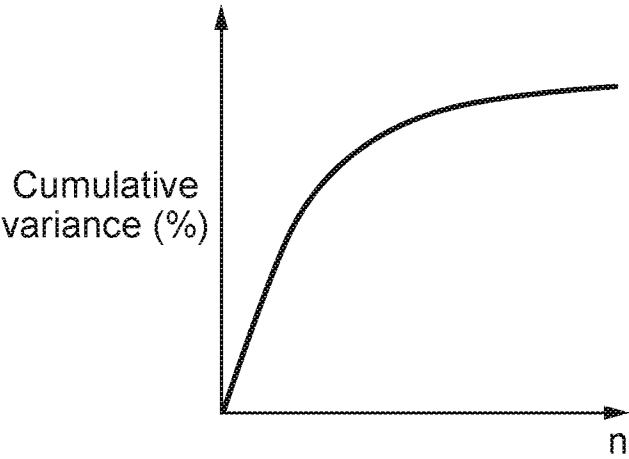


Fig. 8

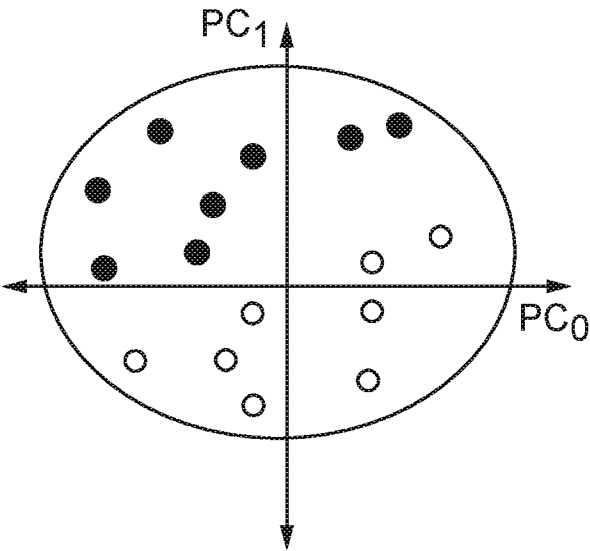

7/9

Fig. 9

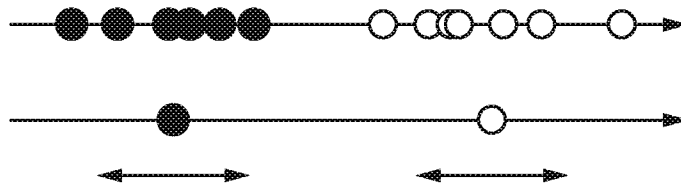


Fig. 10

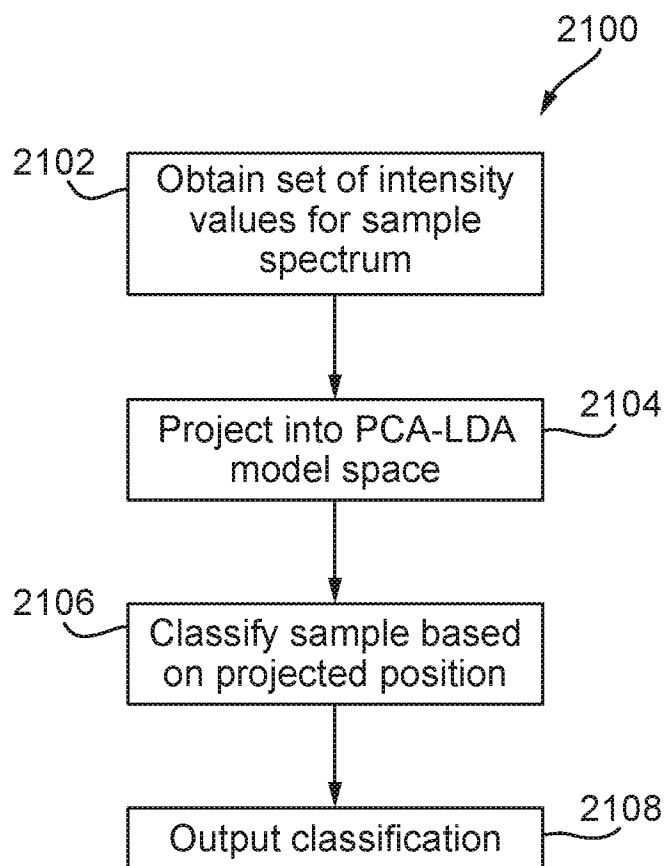


Fig. 11

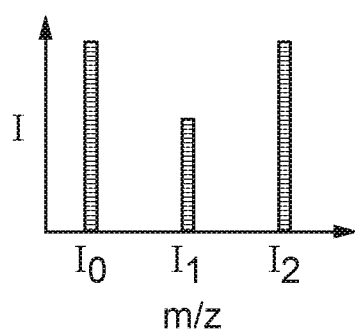


Fig. 12



9/9

Fig. 13


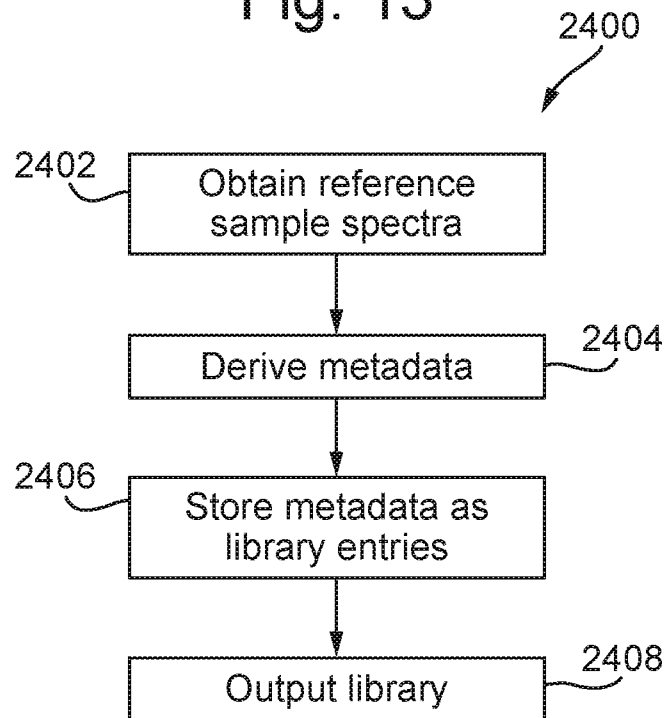


Fig. 14

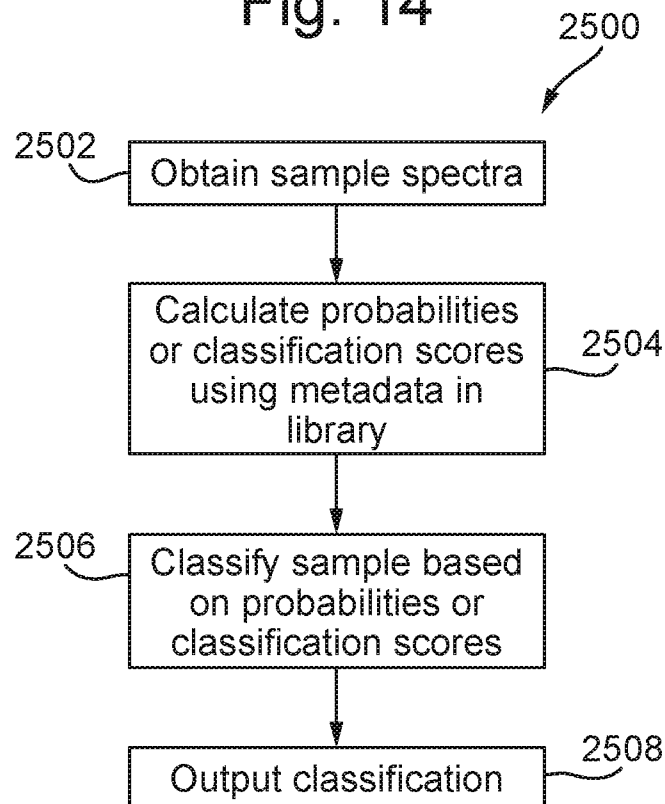

INTERNATIONAL SEARCH REPORT

International application No

PCT/GB2016/050604

A. CLASSIFICATION OF SUBJECT MATTER		
INV.	G01N33/68 A61B18/00	A61B17/00 G01N27/62
	G01N3/00	G01N9/00
		H01J49/00
ADD.		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED		
Minimum documentation searched (classification system followed by classification symbols)		
G01N A61B H01J		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)		
EPO-Internal, BIOSIS, EMBASE, WPI Data		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2012/156712 A1 (TAKATS ZOLTAN [DE]) 21 June 2012 (2012-06-21) the whole document figure 1 paragraphs [0029], [0039], [0048], [0079]	1-261, 263
X	JULIA BALOG ET AL: "Identification of Biological Tissues by Rapid Evaporative Ionization Mass Spectrometry", ANALYTICAL CHEMISTRY, vol. 82, no. 17, 1 September 2010 (2010-09-01), pages 7343-7350, XP055047004, ISSN: 0003-2700, DOI: 10.1021/ac101283x the whole document page 7350 ----- -/--	1-261, 263
☒ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents :		
"A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed		"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family
Date of the actual completion of the international search		Date of mailing of the international search report
16 May 2016		22/08/2016
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016		Authorized officer Jenkins, Gareth

INTERNATIONAL SEARCH REPORT

International application No

PCT/GB2016/050604

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	OTTMAR GOLF ET AL: "Rapid Evaporative Ionization Mass Spectrometry Imaging Platform for Direct Mapping from Bulk Tissue and Bacterial Growth Media", ANALYTICAL CHEMISTRY, vol. 87, no. 5, 3 March 2015 (2015-03-03), pages 2527-2534, XP055272555, ISSN: 0003-2700, DOI: 10.1021/ac5046752 the whole document figure 1	1-261, 263
X	HOBBS S K ET AL: "MAGNETIC RESONANCE IMAGE-GUIDED PROTEOMICS OF HUMAN GLIOBLASTOMA MULTIFORME", JOURNAL OF MAGNETIC RESONANCE IMAGING, SOCIETY FOR MAGNETIC RESONANCE IMAGING, OAK BROOK, IL, US, vol. 18, 1 January 2003 (2003-01-01), pages 530-536, XP001154780, ISSN: 1053-1807, DOI: 10.1002/JMRI.10395 the whole document abstract page 531	1-261, 263
X	DATABASE BIOSIS [Online] BIOSCIENCES INFORMATION SERVICE, PHILADELPHIA, PA, US; February 2011 (2011-02), AGAR NATHALIE Y R ET AL: "Development of Stereotactic Mass Spectrometry for Brain Tumor Surgery", XP002757721, Database accession no. PREV201100146073 abstract & NEUROSURGERY (HAGERSTOWN), vol. 68, no. 2, February 2011 (2011-02), pages 280-290, ISSN: 0148-396X, DOI: 10.1227/NEU.0B013E3181FF9CBB	1-261, 263
X	WO 97/34534 A1 (FEMRX INC [US]; SAVAGE GEORGE M [US]; ALDEN DONALD L [US]; CHRISTIAN J) 25 September 1997 (1997-09-25) the whole document claims 1, 2 paragraph [0002]	1-261, 263
	----- -/--	

INTERNATIONAL SEARCH REPORT

International application No

PCT/GB2016/050604

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	ZSOLT CSELIK ET AL: "Impact of infrared laser light-induced ablation at different wavelengths on bovine intervertebral disc ex vivo: Evaluation with magnetic resonance imaging and histology", LASERS IN SURGERY AND MEDICINE., vol. 44, no. 5, 24 July 2012 (2012-07-24), pages 406-412, XP055272580, US ISSN: 0196-8092, DOI: 10.1002/lsm.22034 the whole document page 407 -----	1-261, 263
T	LAURA M. COLE ET AL: "Mass spectrometry imaging for the proteomic study of clinical tissue", PROTEOMICS - CLINICAL APPLICATIONS, vol. 9, no. 3-4, 23 April 2015 (2015-04-23), pages 335-341, XP055272622, DE ISSN: 1862-8346, DOI: 10.1002/prca.201400103 the whole document page 339, column 1 -----	1-261, 263

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/GB2016/050604

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2012156712	A1	21-06-2012	
		AU 2010252652 A1	15-12-2011
		CA 2763145 A1	02-12-2010
		CN 102483369 A	30-05-2012
		CN 105342646 A	24-02-2016
		CN 105388205 A	09-03-2016
		EP 2435814 A1	04-04-2012
		JP 2012528320 A	12-11-2012
		JP 2015083204 A	30-04-2015
		KR 20120016150 A	22-02-2012
		RU 2011151865 A	10-07-2013
		US 2012156712 A1	21-06-2012
		US 2015201913 A1	23-07-2015
		WO 2010136887 A1	02-12-2010

WO 9734534	A1	25-09-1997	NONE

INTERNATIONAL SEARCH REPORT

International application No.
PCT/GB2016/050604

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-261, 263

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-261, 263

Image-guided generation of aerosol, smoke or vapour.

2. claim: 262

REIMS ion source

3. claims: 264-273

Navigational device-guided generation of aerosol, smoke or vapour.
