



US00D846141S

(12) **United States Design Patent**
Shimobayashi et al.

(10) **Patent No.:** **US D846,141 S**

(45) **Date of Patent:** **** Apr. 16, 2019**

(54) **MEDICAL CLEANING AND DISINFECTION APPARATUS**

(71) Applicant: **OLYMPUS CORPORATION**, Tokyo (JP)

(72) Inventors: **Koji Shimobayashi**, Tokyo (JP);
Chikayoshi Meguro, Tokyo (JP);
Hiromasa Akahori, Tokyo (JP)

(73) Assignee: **OLYMPUS CORPORATION**, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/579,013**

(22) Filed: **Sep. 27, 2016**

(30) **Foreign Application Priority Data**

Mar. 28, 2016 (JP) 2016-006699

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/217**

(58) **Field of Classification Search**

USPC D24/216–218, 227–232; D32/1, 25;
D14/341, 347, 126, 133
CPC A61L 2/26; A61L 2/24; A61L 2/17; A61L
2/18; A61L 2/025; A61L 2202/122; A61L
2202/10; A61L 2202/11; A61L 2202/14;
A61L 2202/23; A61L 2202/24; A61L
2202/182; A61B 1/123; A61B 2090/701
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D267,880 S * 2/1983 Marshall D14/374
D405,443 S * 2/1999 Marsh D12/345
D433,147 S * 10/2000 Florkey D24/217
D533,855 S * 12/2006 Rashid D14/126

D553,750 S * 10/2007 Yamaoka D24/172
D645,036 S * 9/2011 Jones D14/341
D649,950 S * 12/2011 Chiu D14/126
D650,380 S * 12/2011 Ballout D14/331

(Continued)

OTHER PUBLICATIONS

2014 Endoscope Product Spotlights, posted at hpnonline.com, Nov. 2014 issue, [online], [site visited Nov. 14, 2017]. Available from Internet: URL: <https://www.hpnonline.com/inside/2014-11/1411-EndoSpots.html>.*

(Continued)

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Scully, Scott, Murphy & Presser, P.C.

(57) **CLAIM**


The ornamental design for a medical cleaning and disinfection apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical cleaning and disinfection apparatus, showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a bottom view thereof;
FIG. 6 is a left side view thereof;
FIG. 7 is a right side view thereof; and,
FIG. 8 is an enlarged sectional view, taken along line 8-8 in FIG. 2 of the portion thereof indicated by lines a-a and b-b in FIG. 7.

The broken lines show portions of the medical cleaning and disinfection apparatus that form no part of the claimed design. The dot-dash lines show boundaries of the claimed design.

1 Claim, 7 Drawing Sheets

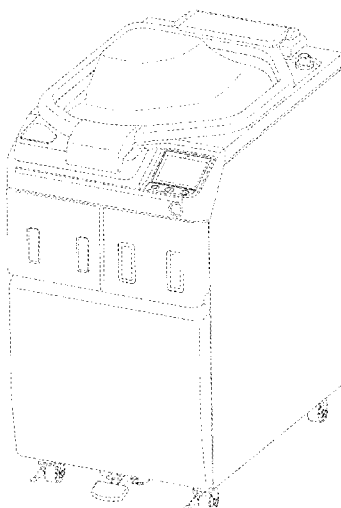

(56)

References Cited

U.S. PATENT DOCUMENTS

8,351,191	B2 *	1/2013	Hirota	G06F 1/1656 174/50
D693,018	S *	11/2013	Zdinak	D10/81
D702,353	S *	4/2014	Fujimoto	D24/164
D735,883	S *	8/2015	Bauer	D24/231
D752,572	S *	3/2016	Kohler	D14/302
D776,293	S *	1/2017	Cerasi	D24/217
D782,690	S *	3/2017	Kurihara	D24/216
D794,211	S *	8/2017	Ang	D24/232

OTHER PUBLICATIONS

Olympus Endoscope Reprocessing With OER-Pro, posted at youtube.com, posted on Feb. 12, 2016, [online], [site visited Nov. 15, 2017]. Available from Internet: URL: <https://www.youtube.com/watch?v=WZgzlnekS2M>.*

* cited by examiner

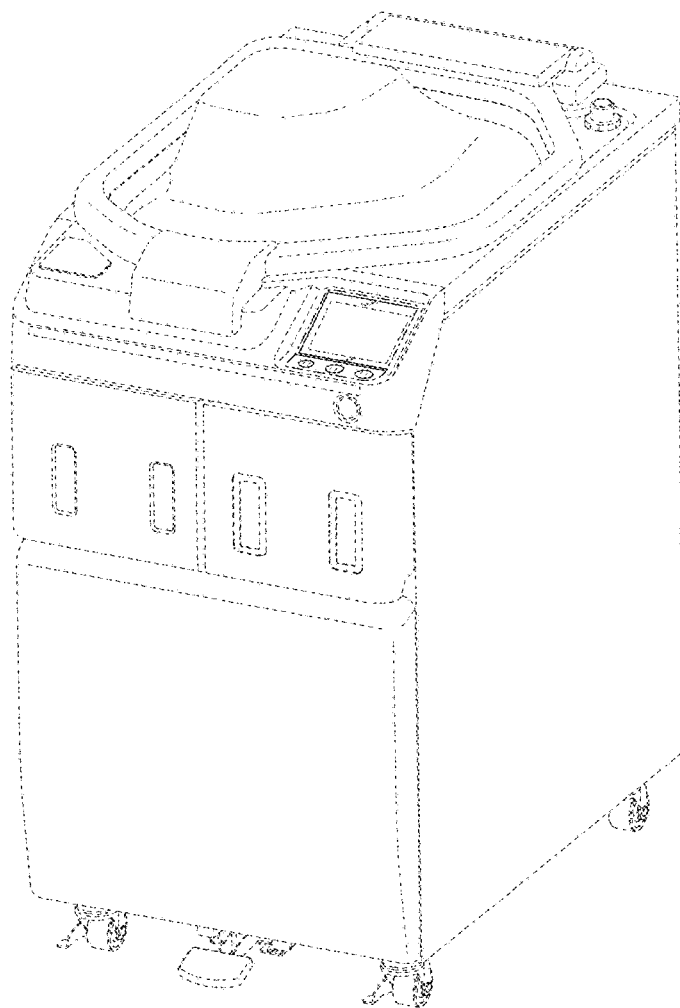


Fig.1

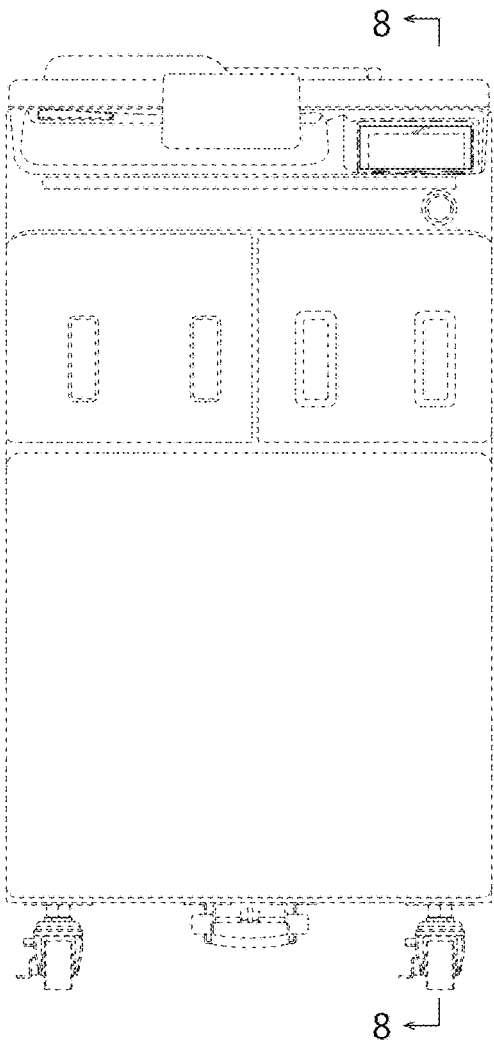


Fig.2

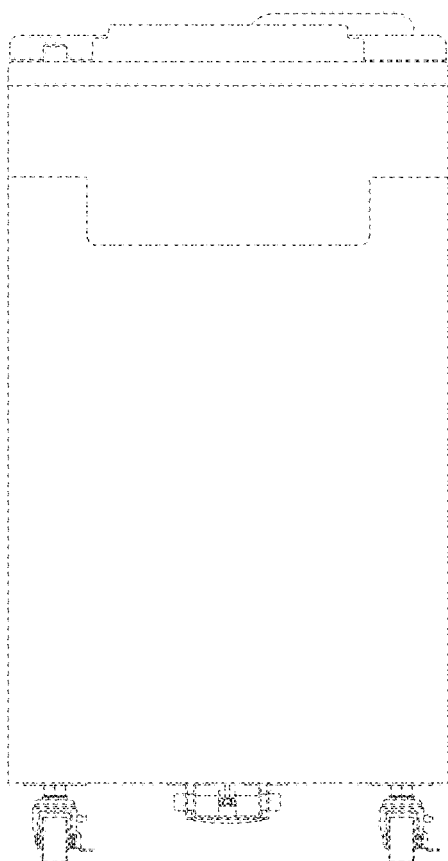


Fig.3

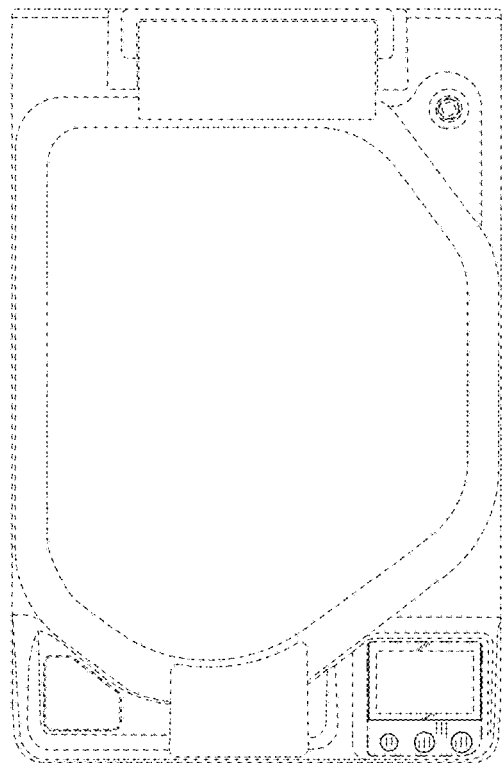


Fig.4

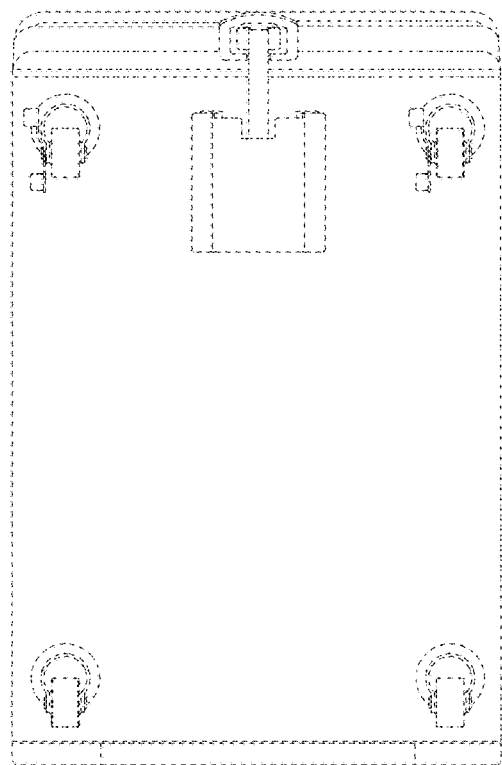


Fig.5

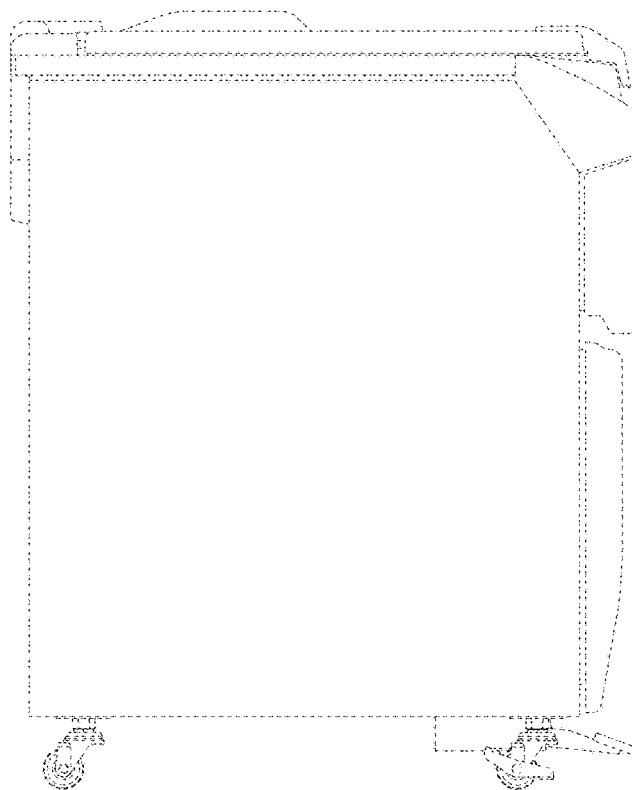


Fig.6

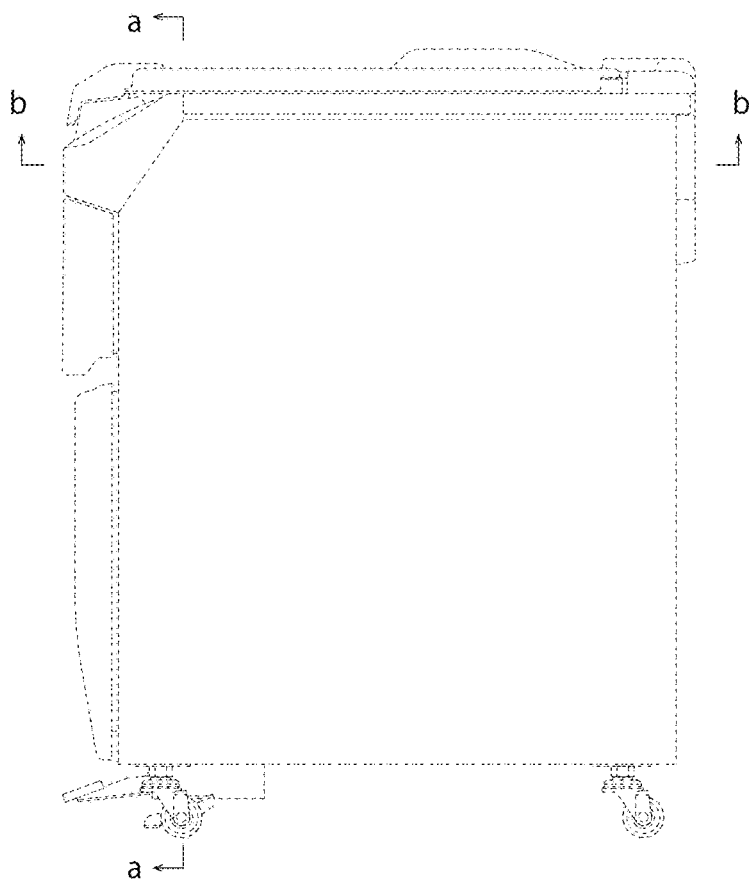


Fig.7

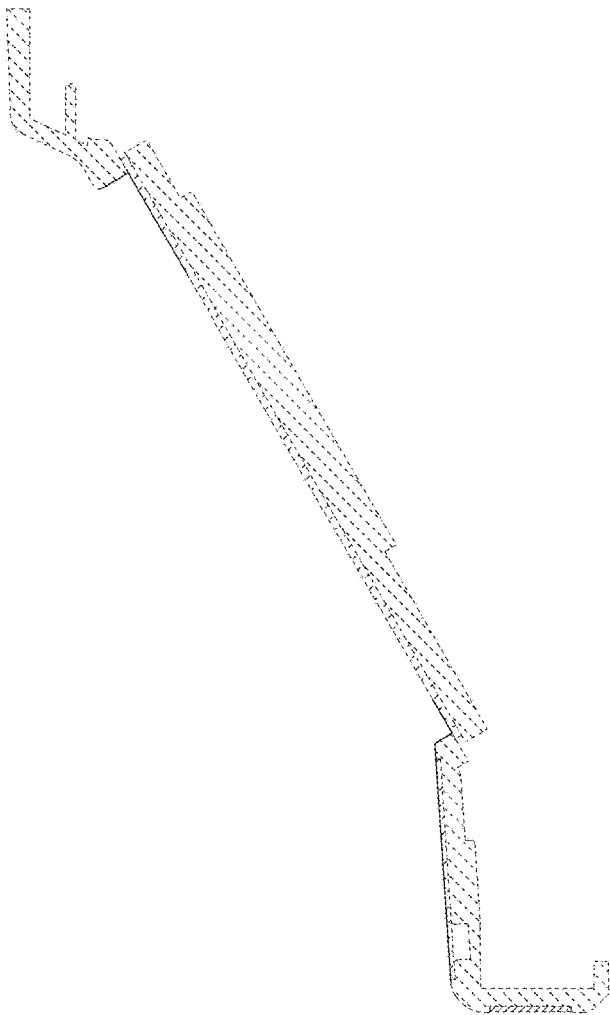


Fig. 8