



(51) International Patent Classification:

G01J 3/443 (2006.01) *G02B 21/06* (2006.01)
A61B 5/103 (2006.01) *G01J 3/10* (2006.01)
A61N 5/06 (2006.01)

(21) International Application Number:

PCT/CA2012/050223

(22) International Filing Date:

5 April 2012 (05.04.2012)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/473,267 8 April 2011 (08.04.2011) US

(71) Applicant (for all designated States except US): **BRITISH**

COLUMBIA CANCER AGENCY BRANCH [CA/CA];
 675 West 10th Avenue, Vancouver, British Columbia V5Z
 1L8 (CA).

(72) Inventors; and

(75) **Inventors/Applicants** (for US only): **ZENG, Haishan** [CA/CA]; 2227 E. 61st Ave., Vancouver, British Columbia V5P 2K5 (CA). **LUI, Harvey** [CA/CA]; 3450 Trafalgar Street, Vancouver, British Columbia V6L 2L8 (CA). **MCLEAN, David** [CA/CA]; 1246 West 26th Ave., Vancouver, British Columbia V6H 2A9 (CA). **LEE, Anthony** [CA/CA]; 5-6395 Hawthorn Lane, Vancouver, British Columbia V6T 1Z4 (CA). **WANG, Hequn** [CN/CA]; 200-2725 Melfa Road, Vancouver, British Columbia V6T 1N4 (CA). **TANG, Shuo** [CN/CA]; 3309 West 30th Ave., Vancouver, British Columbia V6S 1W3 (CA).


(74) **Agents:** **TAKAGAWA, David, H.** et al.; 480 - The Station, 601 West Cordova Street, Vancouver, British Columbia V6B 1G1 (CA).

(81) **Designated States** (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU,

[Continued on next page]

(54) Title: APPARATUS AND METHODS FOR MULTIPHOTON MICROSCOPY

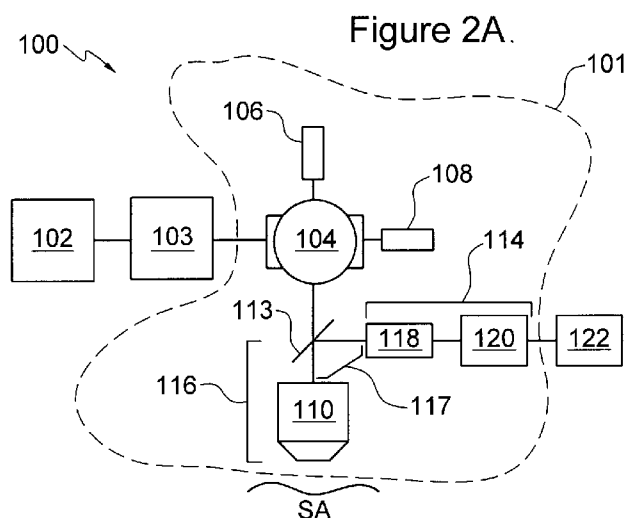

(57) **Abstract:** A multiphoton microscope is provided. The microscope includes: an excitation source for providing an optical excitation beam at an excitation wavelength λ ; a scanner for scanning the excitation beam on a sample; an objective for irradiating the sample with the excitation beam scanned by the scanner and for collecting an emission beam from the sample; a first detector for detecting a plurality of multiphoton signals; and an emission light path allowing transmission from the objective to the first detector a wavelength band limited to greater than or equal to $\lambda/2$ and less than λ , wherein the plurality of multiphoton signals have wavelengths within the wavelength band; wherein the plurality of multiphoton signals comprises a first multiphoton signal and a second multiphoton signal of different types. Fast image capture rate multiphoton microscopes for in vivo imaging, as well as photothermal methods using the microscopes are also provided.



TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— *of inventorship (Rule 4.17(iv))*

Published:

— *with international search report (Art. 21(3))*

Apparatus and Methods for Multiphoton Microscopy

Reference to Related Applications

[0001] This application claims priority from United States provisional patent application No. 61/473267 filed 8 April 2011 entitled APPARATUS FOR COMPLEX MICRO-SPECTROSCOPY AND CONFOCAL MULTIPHOTON MICROSCOPY VIDEO IMAGING SYSTEM. For purposes of the United States, this application claims the benefit under 35 U.S.C. §119 of United States provisional patent application No. 61/473267 filed 8 April 2011, which is hereby incorporated herein by reference for all purposes.

Technical Field

[0002] This invention relates to apparatus and methods for multiphoton microscopy. The invention may for example be used in *in vivo* diagnosis and treatment of skin diseases.

Background

[0003] Non-invasive diagnostic imaging techniques for examining the microscopic structure of tissue is desirable for the skin, where the standard examination practice of biopsy can lead to scarring. Two techniques that have garnered much interest in recent years for dermatology use are reflectance confocal microscopy (RCM) and multiphoton microscopy (MPM). The optical sectioning capability of RCM allows *in vivo*, high resolution morphological images of skin. MPM also has inherent optical sectioning capabilities and allows sensitive *in vivo* imaging at great depths.

[0004] Multiphoton signals include signals from multiphoton fluorescence and

sum frequency generation. Multiphoton fluorescence occurs when two or more photons of relatively lower energy are simultaneously absorbed by and excite a fluorophore, causing emission of a fluorescence photon at a higher energy than the excitation photons. Sum frequency generation occurs when two or more photons interact with a nonlinear material and combine to form a new photon with a multiple of the frequency and a fraction of the wavelength of the initial photons. Both multiphoton fluorescence and sum frequency generation is localized to where the light source, for example a femtosecond laser, is focused and provides a high flux of photons.

[0005] Different MPM excitation mechanisms are sensitive to different biochemical compositions of the tissue. For example, two-photon fluorescence (TPF) signals arise from endogenous fluorophores of skin components such as elastin, NAD(P)H, and keratin; while second harmonic generation (SHG) is sensitive to non-centrosymmetric structures such as collagen.

[0006] As there is less scattering and absorption of the near infrared light used in MPM, there is deeper penetration as well as less photo-damage to the tissue. Combining both RCM and MPM imaging (RCM/MPM imaging) potentially allows greater clinical diagnostic utility as complementary information can be revealed using the two techniques. RCM/MPM imaging has been applied in *ex vivo* and *in vivo* studies. For clinical application, *in vivo* imaging is preferred over *ex vivo* imaging because it does not necessitate tissue removal. It also leaves the tissue in its native state, whereas *ex vivo* tissue can be subject to biochemical/ structural changes due to the degradation of the sample, tissue contraction, and elimination of living tissue dynamics such as blood perfusion and oxygenation.

[0007] *In vivo* skin imaging is complicated because patient motion must be mitigated, and often multiple or large lesions must be examined. Some *in vivo* MPM systems have imaging rates varying from 1 s to 24 s per frame for titanium sapphire laser systems based at 800nm, and 0.5 s to 2 s per frame for chromium-forsterite laser systems based around 1250 nm. These slow imaging rates can result in blurred images and prolonged imaging times. Fast imaging rate is important for decreasing blurring effects and reducing patient imaging times.

[0008] Conventional MPM systems with multiple imaging modes typically employ a dedicated photomultiplier tube (PMT) for each imaging modality. For example, MPM systems that detect both TPF and SHG signals use a dichroic mirror to separate light emitted from the sample into the two signals and direct the signals to respective PMTs. Filters are also typically located in the emitted light path before each PMT. Optical components such as mirrors and filters decrease signal strength by absorbing and/or reflecting some of the emitted light and also by causing the emitted light path to be longer in order to accommodate placement of the optical components. A further disadvantage is that changing wavelengths to switch between multiphoton imaging modes requires changing out or adjusting these optical components, increasing the complexity of the system as well as increasing the time and labour associated with imaging in multiple modes.

[0009] Selective photothermolysis is based on the selective absorption of pulsed light radiation by the targeted chromophores. In selective photothermolysis based skin phototherapy, for example, the therapeutic laser

simultaneously illuminates a large volume of tissue. For successful therapy, heat generation must be restricted to the targeted chromophores only, which is done by selecting a laser wavelength at which the targeted chromophores have much higher light absorption than non-targeted components. This type of skin phototherapy has been somewhat successful in treating pigmented skin diseases and in permanent hair removal. However, side effects and inefficiencies occur when there is less selectivity of light absorption by the target chromophores.

[0010] Apparatus and methods of multiphoton microscopy that address one or more disadvantages of conventional systems are desirable.

SUMMARY

[0011] The following embodiments and aspects thereof are described and illustrated in conjunction with systems, tools and methods which are meant to be exemplary and illustrative, not limiting in scope. In various embodiments, one or more of the above-described problems have been reduced or eliminated, while other embodiments are directed to other improvements.

One aspect of the invention relates to a microscope having (a) excitation source for providing an optical excitation beam at an excitation wavelength λ ; (b) a scanner for scanning the excitation beam on a sample; (c) an objective for irradiating the sample with the excitation beam scanned by the scanner and for collecting an emission beam from the sample; (d) a first detector for detecting a plurality of multiphoton signals; and (e) an emission light path allowing transmission from the objective to the first detector a wavelength band limited to greater than or equal to $\lambda/2$ and less than λ , wherein the plurality of

multiphoton signals have wavelengths within the wavelength band; wherein the plurality of multiphoton signals comprises a first multiphoton signal and a second multiphoton signal of different types.

Another aspect of the invention relates to a microscope for *in vivo* imaging of a subject, the microscope including: an excitation source for providing an optical excitation beam; a scanner for scanning the excitation beam on a target region of the subject, wherein the scanner comprises a resonant scanner; an objective for irradiating the target region with the excitation beam scanned by the scanner and for collecting an emission beam from the target region; a detector for detecting a plurality of multiphoton signals from the emission beam; an adapter comprising a surface for detachably securing to an area around the target region; a translation stage comprising a table and a base, the table movably coupled to the base, wherein the objective is mounted to the table and the base is coupled to the adapter.

A further aspect of the invention relates to a photothermolysis method including the steps of:

- (a) visualizing a target structure using a microscope according to the invention;
- (b) tuning an excitation light source of the assembly to a wavelength at which multiphoton absorption will occur within the target structure;
- (c) increasing power output of the excitation light source to cause heat to be generated within the target structure.

[0012] In addition to the exemplary aspects and embodiments described

above, further aspects and embodiments will become apparent by reference to the drawings and by study of the following detailed descriptions.

Brief Description of the Drawings

[0013] Exemplary embodiments are illustrated in referenced figures of the drawings. It is intended that the embodiments and figures disclosed herein are to be considered illustrative rather than restrictive.

[0014] In drawings which illustrate non-limiting embodiments of the invention:

Figure 1 is a schematic of a known multiphoton microscopy assembly;

Figure 2A is a schematic of a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 2B is a side view of an adapter of the multiphoton microscopy assembly of Figure 2A;

Figures 3(a) to (f) are images of human skin taken using the multiphoton microscopy assembly of Figure 2A;

Figure 4(a) to (b) are images of human skin taken using a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 5A is a schematic of a multiphoton microscopy assembly according to an embodiment of the invention;

Figures 5B and 5C are cross sectional views taken along the planes B-B and C-C of fibre bundle of the multiphoton microscopy assembly shown in Figure 5A;

Figure 6(a) to (c) are images of human skin taken using the multiphoton

microscopy assembly of Figure 5A;

Figure 7 is a schematic of a synchronization system for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 8 is an illustration of signal synchronization of the synchronization system shown in Figure 7;

Figure 9 is a flowchart illustrating a signal synchronization process for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 10 is an illustration of a graphical user interface of a scanner control system for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 11 is a graph illustrating setting the blanking level on a standard RS-170A video signal for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 12 is a graph illustrating setting the blanking level on a PMT video signal for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 13 is a schematic of an attenuator unit and multiplexer unit for a multiphoton microscopy assembly according to an embodiment of the invention;

Figures 14A and 14B are images of bovine collagen taken taken without and with an attenuator unit/multiplexer unit, respectively, of a multiphoton microscopy assembly according to an embodiment of the invention

Figure 15 is a plot of the scanning angle of a resonant scanner and a sample image taken with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 16 is a plot illustrating a linearization algorithm for a multiphoton

microscopy assembly according to an embodiment of the invention;

Figure 17A and 17B are sample images taken without and with, respectively, correction with a linearization algorithm for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 18 is a block diagram illustrating a process for excitation power calibration of a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 19 is an illustration of a graphical user interface for a system embodying the process shown in Figure 18;

Figure 20 is a schematic showing a power attenuator system for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 21 is a graph plotting excitation power against attenuator motor rotation angle for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 22 is a graph illustrating fluctuation of excitation power across different wavelengths over time;

Figure 23A and 23B are, respectively, a TPF image of a fluorescent bead taken with a multiphoton microscopy assembly according to an embodiment of the invention, and a plot of the intensity of the distribution of the pixels along the vertical line on the image;

Figure 24 is graph plotting TPF resolution against excitation wavelength for a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 25(A) to (C) are images of human skin obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 26 is an image of human skin obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 27(A) to (C) are excitation-emission matrix (EEM) plots of purified elastin obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 28(A) to (C) EEM plots of purified keratin elastin obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 29(A) to (C) are EEM plots of pure collagen obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 30 is a graph showing excitation of SHG signals from human collagen detected using a multiphoton microscopy assembly according to an embodiment of the invention;

Figures 31A and 31B are graphs showing excitation of SHG signals from collagen from fish scale and rat tail tendon, respectively, detected using a multiphoton microscopy assembly according to an embodiment of the invention;

Figures 32A to 32D are EEM plots of various fluorophores obtained with a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 33A is an image of normal skin taken using a multiphoton microscopy assembly according to an embodiment of the invention, Figure 33B is an H&E stained sample of same, and Figure 33C is an EEM plot of same obtained using a multiphoton microscopy assembly according to an embodiment of the invention;

Figures 34A to 34E are images and EEM plots of normal skin obtained

using a multiphoton microscopy assembly according to an embodiment of the invention;

Figure 35A and 35B are an image of skin with seborrheic keratosis taken using a multiphoton microscopy assembly according to an embodiment of the invention, and an H&E stained sample of same, respectively.

Figure 36A to 36E are EEM plots of skin with seborrheic keratosis obtained using a multiphoton microscopy assembly according to an embodiment of the invention; and

Figure 37 is a block diagram illustrating a photothermolysis method according to an embodiment of the invention.

Description

[0015] Throughout the following description, specific details are set forth in order to provide a more thorough understanding of the invention. However, the invention may be practiced without these particulars. In other instances, well known elements have not been shown or described in detail to avoid unnecessarily obscuring the invention. Accordingly, the specification and drawings are to be regarded in an illustrative, rather than a restrictive sense

[0016] Some embodiments of the invention relate to apparatus and methods for multiphoton microscopy of microstructures. Some embodiments of the invention relate to apparatus and methods for multiphoton microscopy of biological samples *in vivo*. Some embodiments of the invention relate to apparatus and methods for real time imaging of biological samples *in vivo*. Some embodiments of the invention relate to apparatus and methods for diagnosis and/or treatment of biological conditions such as skin conditions.

Integrated detection of a plurality of multiphoton signals by a single detector at different wavelengths provides improved imaging sensitivity and operator convenience compared to conventional systems. Multiphoton signals may include second harmonic generation (SHG) and two-photon fluorescence (TPF) signals, for example.

Multiphoton Microscopy Assemblies

[0017] Figure 1 is a schematic illustration of a general layout of a known multiphoton microscopy assembly. Laser L directs excitation light to scanner S for scanning through an objective O onto a sample SA. Multiphoton signals emitted from sample SA are reflected by primary dichroic PD through a filter F to a secondary dichroic SD. Secondary dichroic SD splits the signals into TPF and SHG signals for passing through respective filters F1 and F2 for detection by respective detectors D1 and D2. Secondary dichroic SD and filters F1 and F2 are selected depending on the wavelength of the excitation light.

[0018] Figure 2A shows a multiphoton microscopy assembly 100 according to an example embodiment of the invention. Assembly 100 has an excitation light source 102. Excitation light source may be a laser. The laser may be collimated. The laser may be tunable, for example from 720 nm - 950 nm. The laser may be a femtosecond laser. The pulse frequency of the femtosecond laser may for example be 80 MHz.

[0019] The power of the excitation light from excitation light source 102 is attenuated by attenuator 103. Attenuator 103 may be positioned near the output aperture of excitation light source 102. In some embodiments, attenuator 103

comprises a half wave plate and a polarizing beam splitter.

[0020] Scanner 104 scans the attenuated excitation light from attenuator 103. In some embodiments, scanner 104 comprises a resonant scanner 106 scanning for the fast axis (x-axis). In some embodiments, scanner 104 comprises a galvanometer scanner 108 for the slow axis (y-axis). Resonant scanner 106 may for example scan at a fixed scanning frequency. In some embodiments, the fixed scanning frequency may be about 8 kHz. In example embodiments scanner 104 may realize a scanning rate of ~ 12 frames per second for a 512 x 512 pixel frame size. This scanning rate is suitable for real-time *in vivo* imaging. In some embodiments the scanning rate is at least several Hertz. For example the scanning rate may be 10 Hz or greater.

[0021] Scanned excitation light from scanner 104 is directed to the back aperture of objective 110. Objective 110 may be an immersion objective. The magnification of objective 110 may for example be in the range of 20X to 100X. In certain embodiments the magnification of objective 110 is 60X. The numerical aperture (NA) of objective 110 may for example be in the range of 0.45 to 1.2. In certain embodiments the NA of objective 110 is 1.0. Adjusting the amplitudes of resonant scanner 106 and galvanometer scanner 108 may permit a variable field of view. The variable field of view may for example range from 10 μm x 10 μm to 500 μm x 500 μm . Objective 110 focuses the scanned excitation light to a focus location lying in a region of interest in sample SA.

[0022] Multiphoton signals emitted from sample SA are reflected by primary dichroic 112 directly onto a single detector 118 on detection arm 114. Detector

118 detects a plurality of multiphoton signals such as multiphoton fluorescence (e.g. two photon fluorescence (TPF), three photon fluorescence) and sum frequency generation (e.g. second harmonic generation (SHG), third harmonic generation).

[0023] Detection of a plurality of types of multiphoton signals (e.g. multiphoton fluorescence signals and sum frequency generation signals) by one detector 118 obviates the need for a secondary dichroic and the need for the filters between the secondary dichroic and the detectors. The absence of these intermediate optical components between objective 110 and detector 118 provide increased signal sensitivity due to less transmission and reflection losses by intermediate optical components and a shortened emitted light path compared to conventional systems. The absence of these intermediate optical components also obviates the need to change or adjust such components as excitation wavelength is varied. The absence of these intermediate optical components also allows the operator to optimize the excitation wavelength, and therefore the strength of a particular multiphoton signal, in real time without interruption. In some embodiments, particularly for clinical applications, assembly 100 comprises a user interface configured to allow an operator to select from a plurality of endogenous fluorophores to view in real time, additionally or alternatively to selecting or varying the excitation wavelength.

[0024] In some embodiments, emission light path 117 from objective 110 to detector 118 passes a wavelength band that comprising a plurality of multiphoton signals to be detected by detector 118. For example, for detection of TPF and SHG, emission light path 117 permits passage of TPF signals having wavelengths greater than $\lambda/2$ but less than λ and SHG signals having a

wavelength equal to $\lambda/2$, where λ is the excitation wavelength. In other words, for integrated detection of TPF and SHG signals, emission light path 117 permits passage of a wavelength band comprising wavelengths that are equal to or greater than $\lambda/2$ but less than λ . This restriction to a desired wavelength band along emitted light path 117 may be accomplished by a wavelength selector 113. Wavelength selector 113 may direct signals having wavelengths equal to or greater than $\lambda/2$ but less than λ to detector 118. Wavelength selector 113 may direct signals outside of the desired wavelength band elsewhere or absorb them.

[0025] In some embodiments, wavelength selector 113 may comprise a dichroic and a shortpass filter. The dichroic may for example be a 665 nm dichroic mirror (e.g. SemRock FF665-D, 02-25X36) in embodiments where TPF and SHG signals are being detected by detector 118. The dichroic mirror may, for example, have a greater than 90% transmittance in the 680 to 1600 nm range (i.e., transmits all excitation wavelengths, e.g. 720 - 950 nm), and greater than 90% reflectance in the 350 to 650 nm range. The shortpass filter ensures only signals having a wavelength less than that of the excitation wavelength is transmitted.

[0026] In other embodiments, for detection of three photon fluorescence (3PF) and third harmonic generation (THG), emission light path 117 may permit passage of 3PF signals having wavelengths greater than $\lambda/3$ but less than λ and THG signals having a wavelength equal to $\lambda/3$, where λ is the excitation wavelength. In other words, emission light path 117 may, for example by way of a wavelength selector 113, permit passage of a wavelength band comprising wavelengths that are equal to or greater than $\lambda/3$ but less than λ . In such

embodiments, wavelength selector 113 may comprise a dichroic having greater than 90% transmittance in the 680 to 1600 nm range (i.e., transmits all excitation wavelengths, e.g. 720 - 950 nm), and greater than 90% reflectance in the 240 to 650 nm range. The shortpass filter ensures only signals having a wavelength less than that of the excitation wavelength are transmitted.

[0027] Detector 118 may for example comprise a high-UV/visible-sensitivity photomultiplier tube (PMT). In some embodiments the PMT is operated in analog mode (instead of photon counting mode) for a fast response.

[0028] Figure 2B shows an adapter 150 according to an example embodiment of the invention. Adapter 150 stabilizes the region of interest on the subject's body with respect to an objective such as objective 110 of assembly 100. Illustrated adapter 150 is a hollow cylinder. In other embodiments adapter 150 may be any other suitable shape. Adapter 150 may be formed from a rigid material. In some embodiments, the perimeter of an open end of adapter 150 defines an attachment surface 152 for detachably securing adapter 150 to the region of interest on the subject's body. Attachment surface 152 may for example comprise a non-permanent adhesive. In some embodiments, the end of adapter 150 that detachably secures to the subject's body comprises a transparent window instead of an opening. In some embodiments, adapter 150 may be provided with straps or the like that wrap around the immediate body part (e.g. around the forearm, leg, torso, etc.) for detachably securing attachment surface 152 against the subject's skin. Adapter 150 has an interior 154 for containing an objective immersion medium such as oil, water, glycerin or the like.

[0029] A translation stage 156 comprising a plate 158 movably coupled to a base 160. Translation stage 156 may be manually operated or motorized, for example. Base 160 is fixed to adapter 150. In some embodiments, base 160 and adapter 150 may be integrally formed. Plate 158 may move in the XY or XYZ directions in relation to base 160. In embodiments where plate 158 moves in the XY directions, objective 110 may be a focusing objective. An objective 110 of assembly 100, is securely mounted to plate 158. In some embodiments, objective portion 116 and detection portion 114 are disposed on the end of a cantilevered arm (not shown) extending out from an optical table (not shown) or other suitable vibration isolating support. The optical table may support other components of assembly 100 such as light source 102 and scanner 104. The cantilevered arm may be moveable to facilitate positioning of objective portion 116.

[0030] In some embodiments, at least part of assembly 100 may be housed in a handheld probe to facilitate clinical use. For example, the components bounded by the stippled area 101 in Figure 2A may be miniaturized and housed in a handheld probe. In some embodiments, light is delivered from attenuator 103 to scanner 104 through an optical fiber, such as a photonic crystal fiber (PCF). A focus lens may be provided between attenuator 103 and the PCF to focus light into the PCF. A further lens may be provided after the PCF to collimate the light beam before the light enters scanner 104. In some embodiments, providing such an optical fiber facilitates separately and conveniently housing the components such as those bounded by the stippled area 101 in a handheld probe.

[0031] An amplifier 120 amplifies signals received from detector 118 prior to

input into and recorded by a frame grabber 122. Frame grabber 122 may for example be a 10-bit multichannel frame grabber.

[0032] As resonant scanner 106 scans bidirectionally, the forward and backward passes of each fast axis line were added during post-processing.

[0033] Figure 3 shows combined TPF and SHG images extracted from an *in vivo* video obtained with a prototype multiphoton microscopy assembly 100 having the structure shown in Figure 2. Figure 4 shows overlaid TPF and SHG images extracted from *in vivo* videos obtained with a multiphoton microscopy assembly similar to assembly 100 but with a secondary dichroic and respective filters to separate and direct the TPF and SHG signals to individual detectors rather than a single combined detector as in assembly 100.

[0034] The images shown in Figures 3 and 4 show some distortion near the left and right edges because they have not been corrected for the sinusoidal scan pattern of the resonant scanner. Distortion on the left side of the images may be mitigated by delaying the start of line acquisition relative to the resonant scanner turning point on the left side. To obtain the imaging quality shown in Figures 3 and 4 acquired images were rebinned by a factor of 2 resulting in a frame size of 256 x 256 pixels. Image acquisition time for the images shown in Figures 3 and 4 was 1/15 s.

[0035] For imaging experiments, a steel ring was fixed to the dorsal forearms of volunteers using a double-sided adhesive film. No film or coverslip was present between the objective and the skin surface. Water was placed within the ring prior to mating with a magnetic holder. The magnetic holder was mounted to a

manually actuated 3-dimensional translation stage to control imaging location and depth. An objective was mounted to the stage. Excitation light was attenuated to less than or equal to 40 mW. A shutter was used to block the laser when images were not being acquired.

[0036] Figures 3(a) to (f) are images of the skin of a Caucasian male volunteer acquired using the single detector setup of assembly 100 at an excitation wavelength of 900 nm. The images are of the epidermal ridges and the papillary layer of the dermis, with imaging depth increasing from Figure 3(a) to (f) starting from the dermal/epidermal boundary. The field of view is 200 μm X 200 μm . The papillary structure at the epidermal/dermal boundary is clearly evident. Although cells in the upper epidermis are not visualized at this wavelength, the basal cells show up quite clearly as does the fibrous layer in the dermis that lies below the epidermal/dermal boundary. Interestingly, the fibrous layer consisting of collagen and/or elastin only provides a multiphoton signal in a thin layer immediately below the epidermal/dermal boundary (e.g. the fibrous structures are shown as rings in Figure 3 (e) and (f)) even though the dermis consists mainly of these two components. This suggests that imaging at this wavelength is sensitive only to a particular type of collagen or elastin present in this thin layer.

[0037] Figures 4(a) and (b) are overlaid TPF and SHG images of the skin of a male volunteer acquired using a multiple detector set up at 880 nm excitation. The field of view is 200 μm X 200 μm . The images collected from the reticular dermis clearly show elastin fiber bundles in the TPF channel and collagen fiber bundles in the SHG channel. A 458 nm secondary dichroic mirror was used to separate the SHG and TPF signals. 440/40 nm bandpass and 458 longpass

filters were placed in front of the SHG and TPF detectors respectively. The SHG/TPF dichroic and filters preceding the detectors were changed according to the excitation wavelength used.

[0038] The frame capture rate for the videos from which the images in Figures 3 and 4 are derived was ~12 fps. This rate was limited by the particular resonant scanner, image resolution, and frame grabber employed. Faster frame capture rates are possible with other combinations of the foregoing. The same embodiment used for Figures 3 and 4 achieved ~27 fps frame capture rate with lower image resolution (256 X 256 pixels). In some embodiments, a higher frequency resonant scanner (e.g. 16 kHz) can be used to obtain frame capture rates of ~ 30 fps with image resolution of 512 X 512 pixels.

[0039] Clearly evident in the videos from which Figures 3 and 4 were derived were the frame to frame jumps in the z-imaging plane due to patient motion, underlining the need for fast imaging frame rates. Even when patient motion was reduced to a minimum, cardiac pulsation was seen in some instances. Imaging at a slower frame rate could result in significant blurring of the image.

[0040] Figure 5A shows a multiphoton microscopy assembly 200 according to an example embodiment of the invention. Assembly 200 is similar to assembly 100 but is configurable to provide a confocal reflectance microscopy (RCM) imaging mode and a spectroscopy mode.

[0041] Excitation light power from an excitation light source 202 is attenuated by an attenuator 203 which includes half wave plate 203' and polarization beam splitter (PBS) 203". In some embodiments, attenuator 203 is installed directly at

the output aperture of light source 202. Rotation of half wave plate 203' will change the polarization of light. In other embodiments the polarization of light may be changed by other known means. PBS 203" attenuates excitation light power at a variable ratio according to the polarization of the light. Excitation power applied on the sample SA is therefore adjustable by controlling the rotation angle of half wave plate 203'. In some embodiments a computer-controlled motor (not shown) is coupled to rotate half wave plate 203'. The computer-controlled motor may thereby automatically adjust excitation power. The power may for example be reduced to be less than ~ 200 mW by half wave plate 203' and polarization beam splitter 203" in order to result in a power level of around 30 mW at the sample SA after accounting for transmission and reflection loss due to other optical components in the light path.

[0042] Excitation light may be expanded by a beam expander 205, for example after attenuation by attenuator 203.

[0043] Attenuated excitation light may be scanned by a scanner 204. In an example embodiment, scanner 204 comprises a resonant scanner 206 scanning for the fast axis (x-axis), and a galvanometer scanner 208 for the slow axis (y-axis). In other example embodiments, resonant scanners may scan both fast and slow axes. In yet other example embodiments, galvanometer scanners may scan both fast and slow axes, although this would result in slower frame capture rates due to the slower scanning speed. Scanned light is focused on sample SA by objective 210.

[0044] Emitted light from sample SA passes through objective 210 and is

divided by primary dichroic 212 into two beams. A first beam is transmitted through dichroic 212, is descanned by scanner 204, is directed by mirrors through a pin hole, and collected by detector 230 for RCM imaging. A second beam is reflected by a wavelength separator comprising a dichroic mirror 212 and shortpass filter 214, and separated by beam splitter 240 into another two beams, one collected by spectrometer 242 and the other transmitted to a single detector 218 for detecting multiphoton signals. Since both the confocal reflectance imaging and multiphoton imaging share the same excitation light source, scanner, and objective, the resulting multiphoton images and RCM images are automatically co-registered. In some embodiments, spectrometer 242 may be a Raman spectrometer.

[0045] The emitted light beam directed to spectrometer 242 is coupled into a fibre bundle 241 by a fibre coupler lens, transmitted through fibre bundle 241, and collected by the spectrometer 242.

[0046] Figures 6(a) to (c) are (a) an RCM image (b) an integrated TPF and SHG image, and (c) an RCM/TPF/SHG overlay image extracted from *in vivo* videos of the skin of a Caucasian male volunteer obtained with a multiphoton microscopy assembly 200 as shown in Figure 5A. Sampling procedures were the same as those for the images obtained in Figures 3 and 4 discussed above. An excitation wavelength of 720 nm was used. The field of view was 170 μm X 170 μm , resolution at 256 x 256 pixels, and imaging frame rate was 15 fps. The images are of the stratum spinosum (SS). In the RCM image (Figure 6(a)) the cellular membranes and intercellular materials are bright, while cytoplasm and nuclei in the center are dark. In the integrated SHG/TPF image (Figure 6(b)) of the same layer, the cytoplasm is bright. The *in vivo* videos from which the

images in Figures 6(a) to (c) were extracted increased in depth from near the skin surface to the dermal/epidermal junction (DEJ). Honeycomb shaped cells in the SS showed bright cell boundaries in the RCM channel while bright cytoplasm was observed in the SHG/TPF channel. Deeper at the DEJ, dermal papilla and cellular structures were well visualized in both RCM and SHG/TPF channels. Some basal cells at the DEJ were bright in both the RCM and SHG/TPF channels, suggesting the cells contained melanin, which is both highly scattering and fluorescent.

[0047] Fibre bundle 241 is configured to increase the collection area of emitted photons for a high signal-to-noise ratio in spectral acquisition. An example arrangement of optical fibres 241 is shown in Figures 5B and 5C. Fibre bundle 241 has two different patterns at the input and output sides as shown in cross sections B-B and C-C from Figure 5A in Figures 5B and 5C respectively. As denoted by the shaded circles, the outside fibers at the input side of fiber bundle 241 are mapped to the ends of the line pattern of fiber bundle 241 at the output side. In the example embodiment shown, fiber bundle 241 has 90 small fibres (single fiber diameter: 100 μm ; numerical aperture (NA): 0.12) arranged in a hexagon pattern at the input end to provide a much larger collection area than a single fibre. The output end has all of the 90 fibres arranged as 2 straight rows with 45 fibres in each row so that most of the collected light can be coupled into the narrow entrance slit of spectrometer 242. The width of this elongated bundle of fibers is 200 μm . In some embodiments the f-number ($f/\#$) of the spectrograph system ($f/4$) may be matched with the numerical aperture (NA) of the fiber (0.12) as: $f/\# = 1/(2 \times \text{NA})$.

[0048] Since excitation light power and transmission efficiency of optical

components can vary according to excitation wavelength, excitation power for excitation emission matrix (EEM) measurements in spectroscopy mode may be kept constant by adjustment by attenuator 203. In the alternative, attenuator 203 may be adjusted to compensate for (instead of eliminating) excitation power fluctuations.

Table 1: Performance of multiphoton microscopy assembly	
Parameter	Description
Imaging Lateral Resolution	~ 0.5 μm
Imaging Axial Resolution (Estimated value based on lateral resolution)	~ 1.5 μm
Field of View (adjustable)	60 μm $\times$ 60 μm - 500 μm $\times$ 500 μm
Imaging Speed	~12 FPS
Laser Tuning Range	720 nm - 950 nm
Spectral Resolution	~4 nm
Spectrometer CCD Data Resolution	~0.48 nm/pixel

[0049] Table 1 includes major performance parameters of an example embodiment of a multiphoton microscopy assembly according to the invention.

[0050] Some embodiments of the invention relate to computer control and electrical signal synchronization of assemblies such as 100 and 200, as described next.

Scanner/detection coordination

[0051] According to some embodiments, the scanner unit and detection unit are coordinated for improved performance. The scanning unit includes scanners such as scanners 104 and 204 which scan the excitation light over a region of interest in the sample. The detection unit includes the detectors (e.g. PMTs) such as 118, 218 and 230, and frame grabber 122, 222 for image acquisition, and spectrometer 242 for excitation-emission matrix (EEM) measurement. In some embodiments, synchronization signals are generated as described next to coordinate image acquisition with scanner movement for accurate image display.

[0052] Figures 7 shows an example synchronization system 300 for synchronizing image acquisition with scanner movement according to an example embodiment of the invention. A data acquisition (DAQ) board is used to generate the synchronization signals to coordinate the scanner and the detection units.

[0053] The DAQ board generates signals to drive the scanner axes. In some embodiments, one scanner axis (e.g. horizontal axis) may be scanned by a resonant scanner and the other scanner axis (e.g. vertical axis) may be scanned by a galvanometer scanner. For example, a DC signal may be used to set the scanning amplitude of the resonant scanner. For example, a voltage signal in a saw-tooth pattern may be used to drive each step of the galvanometer scanner. In some embodiments, the DAQ board may generate such exemplary control signals for each scanner as analog outputs. The resonant scanner outputs a horizontal synchronization pulse (H.Sync.), which has a rising edge at the beginning of each line scan. When the DAQ board receives this pulse, the DAQ board generates a voltage output to move the Y-axis scanner to the next line.

Upon finishing scanning for one frame, the DAQ board will generate a vertical synchronization pulse (V.Sync.) to inform the Y-axis scanner to move to the beginning line for another frame. In this embodiment the frame size is set as 512 x 512 pixels. The DAQ board also transfers both of the synchronization signals to the frame grabber for display of video signals detected by PMTs.

[0054] As shown in Figure 8, for each frame there are 512 H.Sync pulses representing 512 lines and one V.Sync pulse representing 1 frame. There is also a fly back duration for the galvanometer scanner (Y-axis) to safely move back to the starting line of a frame. All the signal edges, which overlap with the same vertical dotted line, are synchronized together.

[0055] Figure 9 shows a process 400 for controlling a DAQ board for signal reception and generation according to an example embodiment of the invention. Process 400 may be programmed into a suitable graphical development environment such as LabVIEW™. As shown in Figure 9, the DAQ board receives H.Sync from the resonant scanner driving board and applies it as the sampling clock for generation of other digital and analog signals. The V.Sync is generated by frequency division using H.Sync as the base frequency. To generate the analog outputs, two waveform samples are written into buffers. Then the two buffers are triggered by H.Sync and V.Sync respectively to start outputting the analog waveforms to drive the two scanners (DC waveform for resonant scanner and saw-tooth waveform for galvanometer scanner).

[0056] Figure 10 is an example user interface 450 according to an example embodiment of the invention. The user may set the number of scanning lines for one frame. The number of waveform points may be set by control 452 for

number of pre-sawtooth points, control 454 for number of ramp up points, control 456 for number of points to be held at peak, and control 458 for number of ramp down points. The amplitude of the galvanometer scanner can be adjusted in real time using either the exact number control 460 or smooth sliding bar control 462. The offset of the galvanometer scanner can be adjusted in real time using either the exact number control 464 or smooth sliding bar control 466. The amplitude of the resonant scanner can be adjusted in real time using either the exact number control 468 or smooth sliding bar control 470. The analog output waveforms are displayed in two oscilloscope style windows 472, 474.

Detector/frame grabber coordination

[0057] According to some embodiments, the detectors and the frame grabber are coordinated for improved performance. The detectors may include detectors 118, 218 and 230, and frame grabber may include frame grabbers 122 and 222.

[0058] Where a PMT is used for photon detection, maximizing the gain of the PMT is desirable for high sensitivity photon detection. In some embodiments, PMT gain may be increased such that the resulting output voltage of the PMT (e.g. 3 V) is greater than the maximum input voltage (e.g. 1.4 V) of the frame grabber. In such embodiments, an attenuator may be used to attenuate the PMT output signal into an acceptable range for input to the frame grabber.

[0059] Also in certain example embodiments, the frame grabber includes an 8-bit Analog to Digital Converter (ADC) module which will digitize incoming signal into 256 levels based on two reference levels: white (high) and black

(low). A clamp circuit will assume the blanking level embedded in the video signal as zero, and set the high and low levels of ADC accordingly. In standard video signals, there is an H.Sync pulse and a blanking level embedded inherently for clamping. The clamp circuit will choose the voltage level right after the H.Sync as the blanking level: see Figure 11. However PMT output is a continuous signal without any blanking level set. Thus the clamping circuit will clamp to an arbitrary voltage level on the PMT signal according to its relative position with the external H.Sync. In the case that the level chosen by the clamp circuit is relatively high, all the pixels in that line which are weaker than that level will be digitized as zero and displayed as black (see Figure 12) resulting in loss of information due to this false setting of the reference level.

[0060] Figure 13 shows an attenuator unit 500 and multiplexer unit 502 according to an embodiment of the invention for addressing the above detector/frame grabber issues. Attenuator unit 500 attenuates the PMT output signal with an operational amplifier (OPA). Multiplexer unit 502 includes a multiplexer (MUX) which will choose either the PMT output or a ground signal as the input signal to the frame grabber. The external H.Sync (with a duty cycle $\ll 50\%$) generated by DAQ board is input into the multiplexer as a digital reference signal. When the multiplexer detects a rising edge of H.Sync, it will choose to transmit the ground signal. Then the clamp circuit will assume this signal as the blanking level signal and set it as zero for the ADC. When the multiplexer detects a falling edge of H.Sync, it will transmit PMT video output to the frame grabber for image formation. In this way the clamp circuit can work properly with an appropriate setting of high and low reference levels of the frame grabber ADC.

[0061] Figure 14A is an image acquired without attenuator unit 300 and multiplexer unit 302 and Figure 14B is an image acquired with attenuator unit 300 and multiplexer unit 302. The images are of a bovine collagen sample and were acquired at 30 mW at 780 nm excitation, with a $100\ \mu\text{m} \times 100\ \mu\text{m}$ field of view. Each image includes signals collected with forward and backward scans of the resonant scanner. As can be seen from comparing Figures 14A and 14B, more signals were captured with use of attenuator unit 300 and multiplexer unit 302.

Image distortion correction

[0062] As mentioned above, resonant scanners such as resonant scanners 108, 208 are self-oscillating in a typical sinusoidal manner with varying speed, resulting in faster scanning in the middle of the scanning region and slower scanning at and near the edges. However, frame grabbers such as frame grabbers 122, 222 will presume that scanners are scanning at a constant speed, resulting in displayed images stretched at the edges of the images.

[0063] Assuming the focal length of the objective is D , the scanning angle of the resonant scanner is θ and the X-axis displacement of the excitation beam on the focal plane is S , the X-axis displacement is calculated as: $S = \tan(\theta) \times D$. The resonant scanner may have a scanning angle of ± 15 degrees, for example. The relation $\tan(\theta) \approx \theta$ may be used to simplify the above equation as: $S \approx \theta \times D$. D is a constant and S will be linearly proportional to the scanning angle θ . Thus to simplify the theoretical calculation and processing procedure, the scanning angle θ of the resonant scanner may be used to represent the X-axis displacement of the excitation beam on the focal plane.

[0064] Figure 15 shows the scanning angle of a resonant scanner such as resonant scanner 106 and 206. One period includes forward and backward scans over the same scanning range. Thus the backward scan generates a mirror image of the forward scan. As seen in the image of fluorescence beads, the beads at two edges of the scanning area are stretched along the X-axis. The images are TPF images of fluorescent beads at 30 mW at 780 nm excitation, $100\ \mu\text{m} \times 100\ \mu\text{m}$ field of view.

[0065] Figure 16 graphically illustrates a linearization algorithm according to an embodiment of the invention to correct this distortion. The algorithm relocates each pixel to the position as a linear scan so that it is not distorted from the true shape. The following description of the algorithm focuses on processing the forward scan part. The scanning phase step size for each pixel is calculated as $\Delta\phi = 2\pi/n$, where n is the pixel number per line (e.g. $n = 1024$ for the image with 512×512 pixels because the forward scan and backward scan of X-axis scanner are symmetric) and 2π represents the resonant scanner sweeps for one period per line. The phase for each pixel location is $\phi = \Delta\phi \times \text{Pixel Number}$. The parameter *Pixel Number* is the pixel differences between the current location and the center pixel of the forward scan which is $n/4$. The correction factor for relocation is calculated as $C = \phi / \sin \phi$.

[0066] As shown in Figure 16, curve 550 is the actual sinusoidal scanning pattern and line 552 is the ideal linear scanning pattern. $\theta(t)$ is a variable representing the actual scanning angle of X-axis scanner at a certain time point (t) ; A represents a certain value of $\theta(t)$; $L(t)$ represents the corrected angle of X-axis scanner for the ideal linear scan. The pixel positioned at P on actual

curve 550 is reassigned to position PC on ideal line 552 to correct the distortion using the correction factor $C = \phi / \sin \phi$ using an image processor. Image processing may be done in real-time.

[0067] In Figures 17A and 17B, images of fluorescence beads are compared before and after applying the correction factor. There is almost no change for the beads in the center of the images before and after processing. While the beads at the two edges in Figure 17A are obviously stretched along X-axis they are returned to their round shape after correction as shown in Figure 17B.

Spectral data acquisition

[0068] In some embodiments, spectral data collected by spectrometers such as spectrometer 242 are processed and summarized as an excitation emission matrix (EEM). EEM is a matrix of emission intensity as a function of the excitation and emission wavelengths.

[0069] In some embodiments, the laser excitation wavelength is tuned, for example, in 10 nm steps. In some embodiments, tuning may be done over a range somewhat narrower than the specified range of the laser as the laser may not be able to be constantly mode-locked at some extreme wavelengths of the tuning range. Hence for a laser with a specified range of 720 nm to 950 nm, a tuning range of 730 nm - 920 nm may be selected so that accurate EEM acquisition can be achieved for all excitation wavelengths. An emission spectrum for each excitation wavelength is collected with the spectrometer. The spectral data is processed and summarized into a matrix. The spectral data may be plotted for example as a contour map for analysis.

[0070] Figure 18 illustrates an EEM acquisition process 600 according to an example embodiment of the invention. Process 600 may be programmed in a suitable graphical development environment such as LabVIEW™. Process 600 may use a time sequence structure to coordinate the components of a multiphoton microscopy assembly such as assembly 100 and 200 relating to EEM acquisition including the laser, the attenuator, and the spectrometer, namely the EEM sub-system. Automatic EEM acquisition minimizes the time spent on adjustment of device settings for the next excitation step, which helps to decrease the chance of photobleaching and photodamage of the tissue being investigated. In some embodiments, calibrations of the EEM sub-system are repeated as long as there is any change in optics setup or optical component alignment.

[0071] In Figure 18 the blocks with thick outlines and thick arrows set the timing order of process 600. In the first block 602, a data file of rotation angles for the optical power attenuator motor is loaded, which is acquired with the excitation power calibration (described further below) and maintains the excitation power at a constant level for different excitation wavelengths. Simultaneously, a control module (e.g. ActiveX™ control) is loaded for attenuator motor rotation control and initializing an electrical communication path for laser control. After all of the tasks in block 602 are completed process 600 proceeds to block 604.

[0072] The second block 604 involves a loop 605 comprising acquiring multiple emission spectra for each excitation wavelength, calculating and recording the average spectrum, returning to the start of the frame to set a new

excitation wavelength and new rotation angle of the optical power attenuator, and then acquiring another group of emission spectra. Loop 605 may continue until all emission spectra have been acquired.

[0073] Process 600 will then advance to block 606 to stop the system modules including the laser, attenuator motor and spectrometer, and save averaged spectra data (e.g. a .txt file). A separate program for single spectrum acquisition can be applied to measure the background spectrum either before or after EEM acquisition, which may require the operator to manually close the laser shutter. Figure 19 shows a LabVIEW™ graphical user interface 650 of process 600. Basic settings can be changed directly on the interface such as laser scanning range and step width, attenuator motor rotating speed, and spectrometer exposure time. The interface may display real-time settings of key parameters including the excitation wavelength of the laser, angle of the optical power attenuator motor, and emission spectra under specific excitation wavelengths. The interface may also provide the operator with the number of groups of data that have already been acquired and a record of progress. Finally a standard "Save As" window may pop up to let the operator choose where and how to save the spectral data.

Excitation Power Calibration

[0074] To compare the emission spectra under different excitation wavelengths, it is desirable to calibrate the excitation power to maintain it at a constant level over the entire excitation wavelength tuning range. Figure 20 shows a power attenuator system 700 similar to power attenuator 203 for assembly 200. The intensity I of the polarized light that passes through the polarization beam

splitter (PBS) is given by:

$$I = I_0 \cos^2(\theta) \quad (1)$$

[0075] Where I_0 is the input intensity and θ is the angle between the beam's polarization direction and the optical axis of the PBS. The half wave plate is mounted on a motorized rotational stage. As the half wave plate is rotated, the direction of the laser beam polarization varies continuously. Then the angle between the beam polarization and the PBS optical axis will change continuously and cause the excitation power to be attenuated by a varying ratio according to Equation (1). Therefore, excitation power can be controlled by adjusting the rotation angle of the half wave-plate. When the half wave-plate is rotated by an angle θ , the laser beam polarization will be rotated by an angle 2θ . Thus the relation between output power of the attenuator and rotation angle of the half wave-plate is: $I = I_0 \cos^2(2\theta + \theta_0)$ according to Equation (1), where θ_0 is the initial angle between laser beam polarization and the PBS optical axis, and θ is the rotation angle of the half wave-plate.

[0076] Excitation power calibration may be performed in two steps. In the first step, the half wave plate (e.g. half wave plate 203') is rotated from 0-180° and excitation power is measured after the power attenuator for different angles of rotation. The curve shown in Figure 21 shows generally how the excitation power changes (increase or decrease) with the increase of motor rotation angle so that the automated calibration program can be programmed to adjust the angle of rotation motor to attain the target value of excitation power. Four of these curves are shown in Fig. 21 for various excitation wavelengths (750 nm, 800 nm, 850 nm, 900 nm).

[0077] In the second step, the rotation angle of attenuator (e.g. attenuator 203) for each excitation wavelength is calibrated to maintain the excitation power after the objective (e.g. objective 210) at a constant level for all excitation wavelengths. Desired excitation power and an initial excitation wavelength may be inputted into an automatic program which outputs the power after the objective and adjusts rotation angle of the half wave plate (e.g. half wave plate 203') accordingly. The automatic program will keep reading current power and adjusting attenuator rotation angle until the desired excitation power is reached. Then the automatic program will progress to the next excitation wavelength and repeat steps as above. Finally the automatic program will record a group of calibrated rotation angles for each excitation wavelength (730 nm- 920 nm, 10 nm step size). This set of angles will be input to an EEM acquisition program, such as process 600, for automatic adjustment by the power attenuator to provide a constant level of excitation power for all excitation wavelengths.

[0078] Figure 22 shows how excitation power fluctuates due to inherent instability and operation noise of a mode-locked laser. Excitation power for different wavelengths was measured with the rotation angles of attenuator set as that recorded in the previous calibration. Three groups of data were collected at different times after the laser has been turned on (30 minutes, 1 hour and 5 hours), as shown in Figure 22. The fluctuations are all within $\pm 5\%$ of the desired power (20 mW), which will not have significant influence on EEM acquisition. Therefore according to some embodiments of the invention, it will suffice to implement power calibration at the commencement of EEM acquisition. In other embodiments where the laser is very stable, calibration may not be necessary.

Laser Spectral Bandwidth Measurement

[0079] When the spectral bandwidth of a laser excitation beam becomes wider than the fluorophore absorption window, two-photon absorption efficiency is reduced. This affects TPF emission intensity. Spectral bandwidth of an excitation beam over the laser tuning range from 730 nm to 950 nm was measured for a multiphoton microscopy assembly according to an example embodiment of the invention. After transmitting through the excitation path and objective lens, the laser light was collected by an integration sphere. The collected light was sent to a spectrometer through a fiber bundle for spectral measurement. The spectral bandwidth is calculated as the FWHM of the spectrum. Three groups of measurements were taken with forward and backward tuning of the laser in each group, as shown in Figure 28. All of six sets of data show good agreement with each other, with spectral bandwidth ranging from ~6 nm to ~14 nm.

Imaging Resolution Measurement

[0080] According to Equation (2), the number of two-photon fluorescence photons collected per unit time should be proportional to the fluorescence collection efficiency ϕ of the measurement system, which is dependent on the numerical aperture (NA) of the objective (e.g. NA = 1, magnification = 60 for Olympus model no. LUMPLFLN60XW). Resolution is inversely proportional to NA of the objective. Thus the detected intensity of two-photon emission will be affected by resolution.

[0081] It is desirable to measure resolution for different excitation wavelengths. Optical resolution can be defined as the shortest distance between two points on a sample which can be differentiated from each other as individual entities. When emitted light from different points on a sample is collected by the objective and reconstructed as an image, light from each point will generate a pattern described as a point spread function (PSF). The FWHM of a central bright region of the PSF is usually specified as the optical resolution. The FWHM of the PSF in the x-y plane (lateral resolution) for a two-photon microscope can be calculated as:

$$FWHM_{xy} = \frac{\sqrt{2 \ln 2} \times 0.325 \lambda}{NA^{0.9}} \quad (3)$$

[0082] For comparison, the FWHM of the PSF for a single-photon fluorescence microscope is expressed as:

$$FWHM_{xy} = \frac{0.61 \lambda}{NA} \quad (4)$$

[0083] To measure the PSF, fluorescent micro beads with a diameter smaller than the FWHM of the PSF are used. The fluorescent bead used in this measurement has a diameter of $\Phi=116$ nm, which is much smaller than the theoretical resolution of two-photon microscope (~ 400 nm). The beads were suspended in water and sonicated by an ultrasonic water-bath to further separate the beads. The bead suspension was then blended with silicon gel. The mixture was dried. The dried mixture was placed on a plastic plate for measurement. Using a particular excitation wavelength, TPF image of the beads was acquired and a line drawn across the centre of the bead on the image as shown in Figure 23A. The image was taken at an excitation wavelength of 820 nm and a field of view of $60 \mu\text{m} \times 60 \mu\text{m}$, where each pixel is approximately

related to an actual size of $0.1\ \mu\text{m} \times 0.1\ \mu\text{m}$ on the sample. Intensity distribution along this line was plotted and fitted to a Gaussian curve using a MATLAB™ program as shown in Figure 23B. FWHM of the curve is calculated as the resolution value. Several beads are measured and an average value of resolution was obtained for that specific excitation wavelength.

[0084] The relation between the measured resolutions and excitation wavelengths is plotted in Figure 24. For comparison, theoretical resolutions of two-photon and single-photon fluorescence are also shown in Figure 24, which are calculated based on Equation (3) and (4) respectively. A linear fitting of the experimental data is also provided. The average degree of experimental resolution is higher than the theoretical value due to variations of refractive index and scattering effects in tissue samples. However, the experimental resolution is still approximately proportional to the excitation wavelength, which is similar to the theoretical calculation. These results indicate that the resolution values are in a reasonable range, and therefore will not have significant influence on EEM analysis.

[0085] Wavelength calibration of the spectrometer be done with a Hg (Ar) lamp, for example. Calibration of the emission beam path intensity may be done with an NIST calibrated tungsten lamp, for example.

[0086] The above-discussed calibrations and measurements allow for more accurate and reliable EEM measurements to be made with multiphoton microscopy assemblies according to some embodiments of the invention.

Experiments on Biological Samples

[0087] Multimodal imaging, such as TPF, SHG and confocal imaging, have different contrast mechanisms. Multimodal imaging can be applied to reveal various morphological characteristics of skin, for example. In some embodiments, integration of multiple imaging modes provides a useful preview of a region of interest to guide the acquisition of EEM and more comprehensive information for analysis.

[0088] Figures 25 and 26 are images of excised normal skin from the human scalp obtained using a multiphoton microscopy assembly according to an example embodiment of the invention. The excised skin samples were obtained from the surgery unit of the VGH Skin Care Center, Vancouver, Canada. Using a microtome, 20 μm -thick cross sections were sliced from frozen skin tissues. The sections were placed between a microscope slide and cover glass and stored at 4 °C until analyzed. The samples were irradiated with 785 nm femtosecond laser pulses under 30 mW excitation power with a field of view of 150 μm $\times$ 150 μm . The combined images combine the confocal, SHG and TPF channels.

[0089] As shown in Figures 25A to 25C, clear fibrous structures are observed in all three channels, indicating the sample is in the dermis compartment which mainly comprises extracellular fiber structures. Figure 25A shows the confocal signal. The SHG signal (Figure 25B) mainly comes from collagen fiber and the TPF signal (Figure 25C) may come from elastin and/or collagen fibers. As seen in the combined image (Figure 26), there is no overlap between the TPF and SHG signals, indicating the TPF signal mainly originates from elastin fibers.

[0090] The combined image in Figure 26 shows various morphological structures of tissue compositions and relative distribution and density of these compositions. The results also assist in distinguishing TPF of elastin fiber from that of collagen fiber, which is comparatively difficult using spectral analysis. In some embodiments, imaging provides a preview of the tissue sample in advance so that EEM can be acquired from interesting regions of skin tissues. More comprehensive information may be obtained by using the imaging channels together with nonlinear EEM analysis.

Imaging-Guided Nonlinear Excitation-Emission-Matrix (EEM)

[0091] To assist nonlinear EEM analysis of skin tissues, EEM measurements of pure endogenous fluorophores of skin tissue including elastin, collagen, keratin, NADH, FAD and melanin were obtained. Single-photon EEMs were measured by tuning the excitation wavelength from 250 nm to 600 nm using a known commercial system (FluoroLog3™). A multiphoton microscopy assembly according to an example embodiment of the invention. The assembly was tuned from 730 nm to 920 nm and was used for two-photon EEM.

[0092] Figures 27A to 27C are the EEM results of pure human elastin. Purified elastin (GH421, Elastin from human skin, Elastin Products Co. Inc.) is light yellow powder and is stored at 4 °C until used for the EEM measurement. The elastin sample was evenly placed on a microscope slide with a piece of cover glass on top. Imaging and single-photon & two-photon EEM data were acquired. Excitation power was 20 mW (+/- 5%) for all excitation wavelengths. For every excitation wavelength, there is normally a peak in the emission

spectrum. To facilitate analysis of EEM results, the excitation-emission-pair parameter was used to represent the emission wavelength of that peak and the excitation wavelength related to it.

[0093] Figures 27A and 27B are two-photon and single-photon EEM results respectively with the same range of excitation wavelengths. In the single-photon EEM, the maximum excitation emission pair was at (375 nm, 450 nm), while the maximum excitation emission pair was at (~730 nm, ~460 nm) for two-photon EEM. Maximum fluorescence occurred at similar emission wavelengths for single-photon and two-photon EEM, and the two EEMs have similar patterns over the whole range. As expected, the excitation wavelengths in two-photon EEM were roughly two times that of single-photon EEM. This comparison shows similarities and differences between two-photon and single-photon EEM. Purified elastin sample is known to show TPF excitation-emission-pairs at (750 nm, 457.9 ± 0.4 nm), (770 nm, 465.5 ± 0.4 nm), (810 nm, 479.8 ± 0.8 nm), (850 nm, 503.0 ± 0.2 nm) and (870 nm, 512.9 ± 0.4 nm), which are shown by the white circles in Figure 27A. The known results are consistent with the present measurements. Single-photon EEM with an excitation range from 250 nm to 600 nm is shown in Figure 27C, which exhibits additional peaks in the UV excitation range.

[0094] Figures 28A to 28C are EEM results of purified human keratin (Product K0253, Sigma Aldrich, 1 mg/ml solution in urea) from human epidermis. 30 ml of the keratin solution was placed in a central depression of a flat plastic vessel. A piece of cover glass was placed over the depression. Single-photon and two-photon EEM results have different patterns and different maximum excitation-emission pairs because two-photon and single-photon fluorescence

have different absorption coefficients which result from various selection rules for the transition of electronic states of the fluorophore molecules.

[0095] Figure 28A shows two-photon EEM results obtained with an excitation wavelength range of 730 nm to 920 nm, at a power of 30 mW and an exposure time of 2 seconds. Figure 28B shows one-photon EEM results obtained with an excitation wavelength range of 365 nm to 460 nm. The maximum excitation emission pair is at (~380 nm, ~450 nm) for single-photon EEM (Figure 28B), while it is at (~730 nm, ~475 nm) for two-photon EEM (Figure 28A). Due to the limit of scanning range, data was not acquired for excitation wavelengths below 730 nm. In Figure 28A there are two excitation emission pairs at (760 nm, 490 nm) and (860 nm, 530 nm). These results match with reported results of (760 nm, 475±5 nm) and (860 nm, 515±5 nm), which are shown as the two white circles on the EEM plot, for pure human keratin (K0253, Sigma Aldrich, 30mg/ml solution in urea). Single-photon EEM with an excitation range from 250 nm to 600 nm is shown in Figure 28C.

[0096] Figures 29A to 29C show EEM results of a purified human collagen sample (Type I). The collagen sample (HS150 Collagen Type I, Acid soluble, from human skin, Elastin Products Co. Inc.) was supplied as a white sponge-like material and stored at 4 °C until used for EEM measurements. The collagen was placed between a microscope slide and a piece of cover glass. Figures 29A and 29B show two-photon (730 nm to 920 nm) and single-photon (365 nm to 460 nm) EEMs respectively. As seen in Figure 29A, there are a series of narrow peaks in addition to a TPF signal. These narrow peaks originate from SHG emission from the purified collagen because the emission wavelengths of those peaks are exactly half of the corresponding excitation

wavelengths. This can be a unique characteristic of collagen fiber. Since single-photon EEM does not have SHG signals, two-photon EEM has better performance in distinguishing the epidermis from the dermis, and elastin fibers from collagen fibers. There are several known excitation emission pairs for TPF of pure human skin collagen Type I (HS150, Elastin Products Co. Inc.) including: (770 nm, 472.5 nm), (810 nm, 487.6 nm), (850 nm, 503.0 nm) and (870 nm, 512.9 nm), which are shown by the white circles in Figure 29A. The known results shows agreement with the TPF part in the present EEM measurement results in Figure 29A. Single-photon EEM with an excitation range from 250 nm to 600 nm is shown in Figure 29C, which indicates that the major peaks for single-photon fluorescence from human keratin are located in the UV excitation range.

[0097] The excitation spectrum of the SHG signal (peak value of SHG emission spectrum vs. excitation wavelength) can provide suggestions on choosing the optimal laser wavelength for two-photon analysis of tissues rich in collagen fibers. Figure 30 shows three different SHG excitation spectra measured from three different locations on the purified human collagen sample with an excitation wavelength range of 730 nm - 920 nm, 20 mW excitation power, and three second exposure time. These excitation spectra show a major peak at ~790 nm and a secondary peak at ~850 nm. These results match to a certain extent with known results which show a major peak at ~810 nm and a secondary peak at ~850 nm.

[0098] SHG excitation spectra of other collagen samples were also measured. Samples included fish scale and rat tail tendon, which are rich in collagen fibers (Figures 31A and 31B). Comparing the excitation spectra in Figures 30 and 31,

different samples show different spectral characteristics in terms of peak positions and width of spectrum. These characteristics may be related to structure and chemical characteristics of collagen fibers, which are important for complex tissue analysis.

[0099] Other important endogenous fluorophores for two-photon study of skin include NADH, FAD, and melanin. NADH and FAD are significantly involved in cell metabolism activities. Melanin is an excellent photoprotectant for skin.

[0100] Purified NADH (N6879-25MG, α -Nicotinamide adenine dinucleotide, reduced disodium salt, Analog of β -NADH, chemically reduced, Sigma Aldrich) and FAD (F6625-10MG, Flavin adenine dinucleotide disodium salt hydrate, Sigma Aldrich) in powder form were placed between a microscope slide and cover glass for analysis. Melanin powder (M8631-250MG, Sigma Aldrich) was dissolved in 1 mol/l NH_4OH to provide a 1 mg/mL solution. EEM of the melanin solution was measured in the same way as the keratin solution discussed above. Two-photon EEMs of NADH, FAD and melanin are summarized in Figures 32A, 32C and 32D respectively. Figure 32B shows a one-photon EEM of NADH. Excitation wavelengths of 730 nm to 920 nm, an excitation power of 20 mW, and an exposure time of three seconds were used. The excitation-emission pairs in the EEMs of Figure 32B show agreement with the reported results as: (730 nm, 545 nm) and (900 nm, 540 nm) for FAD (solution, Sigma Aldrich), (800 nm, 565 nm) for melanin (Synthetic melanin prepared by oxidation of tyrosine with hydrogen peroxide, solution in KOH, Sigma Aldrich), and (730 nm, 460 nm) for NADH (solution, Sigma Aldrich). Figures 32A, 32C and 32D indicate these known results as white circles on the contour map.

[0101] The nonlinear EEM for each purified fluorophore measured above has a distinct pattern and serves as useful signatures for characterization of complex skin tissues. In some embodiments, the multiphoton microscopy assemblies of the invention may include a processor that uses these signatures to putatively identify biological structures and/or biological activities in a sample.

Experiments on Normal Human Skin Tissue

[0102] Fresh normal skin (~2 mm thickness, ~1 cm × 1 cm area) excised from a human temple without sectioning was subject to EEM measurement within 1 hour after excision using a multiphoton microscopy assembly according to an example embodiment of the invention. After all EEM measurements were completed, the tissue was fixed in formalin and processed by H & E staining for histological image acquisition. Figure 33A is a combined TPF/SHG/confocal image of a cross section view of the epidermis-dermis junction in a field of view of 100 μm × 100 μm. Figure 33B is a H&E stained histology image of a similar region, wherein the box represents an area of 100 μm × 100 μm which matches with the field of view in Figure 33A. A papillary structure can be seen in both Figures 33A and 33B, which is a typical structure at the epidermis-dermis junction. Figure 33C is an EEM for this cross-section showing two parts, namely wide TPF curves and a narrow SHG peak array. The emitted SHG peak is located at half of the excitation wavelength, and originates from collagen fibers. The TPF portion of the EEM has a similar pattern and excitation-emission-pairs as the pure elastin sample; however, it is shifted a little to the longer wavelength side, which may be due to contribution of emission from keratin from epidermal cells.

[0103] Five distinct layers were measured in the vertical direction from the stratum corneum to the dermis layer. Figures 34A to 34E each show 50-image-averaged images of: four sub-layers of the epidermis compartment and one layer from the dermis compartment, respectively. For the epidermis compartment the TPF channel was mainly used for the imaging guidance purpose. Imaging depths of the four epidermal sub-layers were: 10 μm , 20 μm , 30 μm and 40 μm (Figures 34A to 34D respectively). The other layer with an imaging depth of 60 μm was the dermis compartment (Figure 34E). The field of view for these images is 100 $\mu\text{m} \times 100 \mu\text{m}$ and the scale bar in the Figures is 20 μm . All images were taken using an excitation wavelength of 790 nm and excitation power of 30 mW.

[0104] As seen in Figure 34A, stratum corneum cells have large sizes. The EEM maximum excitation emission pair is located at (730 nm, 470 nm), which is close to that of purified keratin as in our previous measurement (730 nm, 480 nm). Imaging deeper, the number of cells increases while the size of cells decreases. EEMs for the first two sub-layers (Figures 34A and 34B) indicate that most of the TPF signals in these layers come from keratin, which mainly exists at the surface of skin. For the third and fourth sub-layers (Figures 34C and 34D), the stratum spinosum and stratum basale, the EEMs have the pattern and the maximum excitation emission pairs resembling that of pure NADH, indicating most of the TPF signal in these layers originates from NADH. NADH is significantly involved in redox reactions for metabolism, hence these EEMs show that cells are more active in the stratum spinosum and stratum basale layers. This is consistent with known skin biology - because cells in the epidermis originate from the stratum basale layer and keep proliferating and

migrating to the top layers, cells at a deeper layer are more metabolically active.

[0105] Figure 34E shows an averaged image and EEM data for one layer in the dermis compartment. The SHG channel was added and optimized for this layer for image-guidance purpose. The dotted array in the EEM plot comprises SHG peaks with each emission peak located at exactly half of the excitation wavelength respectively. The SHG signal originates from collagen fiber in the dermis layer. The peaks with larger bandwidths represent the TPF signal. The TPF part of this EEM has a similar major excitation emission pair (730nm, 450nm) and overall pattern as pure elastin. Signals acquired in the imaging channels supports this analysis. The TPF imaging channel mainly showed thin elastic fiber structures while the fiber bundle structure of collagen was only observed in the SHG imaging channel. There was no overlap between SHG and TPF signals, which indicates that collagen fiber in fresh skin tissue does not have strong TPF emission at 790 nm excitation. SHG intensity in this EEM plot is attenuated 20 times so that the contour details of SHG and TPF signal can be displayed on a single plot. The SHG/TPF ratio for purified collagen is different from that of collagen fibers in skin tissue, which may be due to the purification process changing the structure of collagen.

Experiments on Human Skin Tissue with Seborrheic Keratosis (SK)

[0106] Diseased human skin tissue with SK was also investigated for comparison with normal skin tissue EEM. This type of tissue usually has histological characteristics such as basal cells mixed with squamous cells and keratin-filled invaginations of the epithelium. Figure 35A is a TPF/SHG image (acquired using a multiphoton microscopy assembly according to an example

embodiment of the invention) and Figure 35B is an H&E stained histological image of the same sample of a transverse slice of human shoulder skin with SK with a field of view of $200\ \mu\text{m} \times 200\ \mu\text{m}$. The dimension of the boxes in the images are $20\ \mu\text{m} \times 20\ \mu\text{m}$. An excitation wavelength of 790 nm and excitation power of 30 mW was used.

[0107] Figures 36A to 36E show EEMs acquired from the five square areas indicated by the squares labelled A to E in Figures 35A and 35B. Excitation wavelengths of 730 nm to 920 nm, excitation power of 30 mW, and exposure time of two seconds was used. In Figure 36A, the EEM has a similar pattern and maximum excitation-emission-pair as that of pure keratin sample. Figure 36A corresponds to square A in Figure 35B where the keratin structure can be observed clearly in the histological image. In Figures 36B and 36D, both of the EEMs resemble that of pure NADH, which is consistent with the cellular structures as highlighted by the squares B and D in Figure 35.

[0108] In Figure 36C, the EEM seems to be a mixture of signals originating from various structures. The contour pattern and excitation-emission pairs below excitation of 760 nm (black dotted line) are similar to pure keratin, while the pattern above 760 nm shows similarity with that of purified FAD sample. This spectral characteristic is consistent with the image signal in square C on Figure 35B, which includes both keratin and cellular structures in it. This analysis shows the advantage of EEM compared with pure emission spectra or excitation spectra, since this tissue characteristic cannot be fully revealed using only one excitation wavelength or one emission wavelength. More importantly, EEM reveals the fact that a keratin structure has intruded into the middle sub-layers of the epidermis part of this SK tissue sample. This result is

consistent with the biological characteristic of SK tissues, and demonstrates the applicability of image-guided EEM for diagnosis of skin diseases. Figure 36E shows the EEM for the last square E which is located in the dermis layer mainly containing fiber structures. The dotted array is related to SHG peaks from purified collagen. The TPF spectra have a contour pattern similar to purified elastin fiber.

[0109] Comparing the results from normal skin tissue with the results from SK skin tissue, EEMs show different characteristics at certain layers and show consistency with the biological characteristics of both tissue types. The results indicate imaging-guided nonlinear EEM can be advantageously used for skin disease diagnosis.

Multiphoton absorption photothermolysis

[0110] Multiphoton microscopy assemblies according to some embodiments of the invention may be used to target a microstructure by multiphoton image visualization and/or spectral analysis, and then damage or destroy the target by scanning and focusing a high intensity laser beam within the target.

[0111] A photothermolysis method 800 according to an embodiment of the invention is illustrated in Figure 37. At box 802, the region of interest is visualized using the imaging techniques described above, such as through use of multiphoton microscopy assemblies of the invention including assemblies 100 and 200. At box 804, the wavelength may be chosen so that strong multiphoton (e.g. two photon) absorption will be generated by the target and generate localized heat to destroy the target. At box 806, the laser intensity may

be chosen so that the target is damaged or destroyed. In some embodiments, the intensity of the laser beam at the target may be at least 75 mW when a wavelength of 785 nm is used. Other embodiments may use other suitable intensities and wavelengths depending on the target region. Because the multiphoton absorption will occur only at the focal point and not on other locations along the light path where light intensity is lower, other tissue components (even those having the same or stronger absorption properties as the target) will not be affected or damaged.

[0112] Since proteins and DNA have strong absorption in UV wavelength ranges, almost any types of microstructures in tissue could be targeted by an appropriate laser beam in the red to near infrared wavelength ranges. According to some embodiments of the invention, precise microsurgery of any microstructures of interest can be carried out by combining multiphoton microscopic image targeting and multiphoton absorption photothermolysis.

[0113] In some embodiments, dark or black hair follicles and shafts in dark or black skin can be targeted microscopically and destroyed by laser without affecting the surrounding skin tissue even though the surrounding skin may contain high concentrations of light absorbing melanin.

[0114] In some embodiments, cancer cells (e.g. melanoma cells) can be visualized and differentiated from benign or normal cells and then destroyed by a high intensity laser beam. Tumor destruction may for example be on a cell-by-cell basis. For high efficiency, a cancer cell cluster (e.g. basal cell island in basal cell carcinomas) may also be destroyed at one time. In some embodiments, cancer stem cells can be identified and destroyed.

[0115] In some embodiments, vascular skin lesions may be treated by selectively destroying excessive blood vessels. A certain number of vessels may be maintained for normal physiological functions of the tissue.

[0116] In other embodiments, one or more of the following conditions may be visualized and treated: oral disorders such as oral lesions and oral cancers; nail fungus and other nail and hair disorders; ophthalmic disorders and eye diseases like glaucoma; internal lesions and disorders that become accessible during surgery (e.g. brain tumors and Parkinson's disease, during neural surgery).

[0117] In some embodiments, the invention can be used in endoscopic applications for both diagnosis and therapy at microscopic accuracy. The present invention provides access to internal organs through an endoscope by fiber delivery of the laser light and use of a miniaturized scanner.

[0118] In some embodiments, the invention can be used for wrinkle removal and skin resurfacing by targeting skin collagen with multiphoton (e.g. two-photon) absorption.

[0119] In some embodiments, the invention can be used for subcutaneous fat removal by targeting adipose cells with multiphoton (e.g. two-photon) absorption.

[0120] In some embodiments, the invention can be used for tooth whitening by removing microscopic surface pigments.

[0121] In some embodiments, cosmetic blemishes of the skin such as scars, birthmarks, hyperpigmented or hypopigmented regions, and/or unwanted tattoos may be removed through microscopically targeted multiphoton absorption photothermolysis. Removal may be accomplished without damage to neighboring regions of skin. Some pigmented tattoo particles are difficult to remove with current conventional one-photon photothermolysis. Multiphoton (e.g. two photon) absorption photothermolysis enables focused ablation of such particles.

Clinical use example

[0122] The multiphoton microscope assemblies of the invention such as assemblies 100 and 200 may be employed as follows in a clinical setting.

[0123] A patient seeks a consultation with a user (e.g. a dermatologist) regarding a large and irregular mole on the back of the patient's hand. The user determines through a naked eye visual inspection of the mole that further investigation is indicated in order to make a proper diagnosis. Instead of performing a biopsy, the user visualizes the micromorphology of the patient's mole using a multiphoton microscope assembly according to an embodiment of the invention.

[0124] The patient is seated and his hand placed palm down on an examination stand in a resting position. The user request the patient to keep his hand as still as possible. An adapter with a bore greater than the area of the mole is attached around the mole with a quick curing non-permanent adhesive. Once the

adhesive has cured, the adapter is filled with a suitable objective immersion medium. As the base of the translation stage of the multiphoton microscope assembly is coupled to the adapter, the objective mounted to the table of the translation stage is immersed in the immersion medium. Multimodal imaging is commenced for real time viewing of the mole.

[0125] The user moves the objective by using controls on the assembly which control the motorized translation stage. The controls on the assembly may be physical dials, knobs, buttons and the like, or controls displayed a graphical user interface operated by touch screen, keyboard, joystick, mouse and the like. The position of the table of the translation stage is adjusted in three dimensions to position the objective in the desired position for viewing.

[0126] The user may operate:

- excitation wavelength controls on the assembly to adjust the excitation wavelength in real time to optimize the strength of the multiphoton signal(s) being detected;
- field of view controls on the assembly to adjust the field of view;
- excitation power controls on the assembly to adjust the excitation power (by adjusting the attenuator motor). Additional controls may be provided to allow the user to set a predetermined or user-defined constant level of excitation power.

[0127] The user may also switch to an “automatic detection mode” of the assembly to automatically identify on the assembly’s display various common endogenous fluorophores (e.g. elastin, collagen, keratin, melanin, NADH, FAD, etc.) by instructing a processor to compare preloaded, known

fluorescence/spectroscopic signatures with detected multiphoton and spectroscopic signals of structures in the field of view. Identification on the assembly's display could for example be manifested by false colour overlaid images of two or more fluorophores, or separate images of one specific fluorophore at a time. Based on the parameters such as density and distribution of these fluorophores the user can determine whether the structures in the field of view are, for example, normal or abnormal, benign or cancerous, etc. This determination may also be performed automatically by a processor in the assembly by comparing the detected density and/or distribution of particular fluorophores with known densities and/or distributions for particular conditions. The automatic determination may for example also factor in other inputted factors such as imaging depth, body location, age and sex of the subject, etc.

[0128] If an imaged region within the mole is determined to be normal or benign, the user moves the translation stage to image another structure. If the imaged region is determined to be cancerous, the user may upon obtaining the patient's consent proceed with photothermolysis of the cancerous region. The user adjusts the appropriate controls (e.g. laser power control, wavelength control) to suitable levels for photothermolysis. After ablating the cancerous region with high intensity laser, the user adjusts the controls back to a levels suitable for imaging to confirm the cancerous region has been destroyed or adequately damaged.

[0129] As will be apparent to those skilled in the art in the light of the foregoing disclosure, many alterations and modifications are possible in the

practice of this invention without departing from the spirit or scope thereof. For example:

- software may be provided to (1) coordinate operation of the described assemblies with one or more of the described measurement modes (e.g. MPM imaging, RCM imaging, spectral measurements) and/or (2) provide a variable scanning speed, and therefore variable imaging frame rate; and/or (3) scan a region of interest of any shape to facilitate spectral measurements of the targeting microstructure or for targeted photothermolysis.
- diseases or physiological states may be diagnosed by detection and/or measurement of the fluorescence or spectra of subsurface blood vessels in a non-invasive manner.
- glucose levels in subsurface blood vessels may be determined by measurement of fluorescence or spectra in a non-invasive manner.
- drug localization and drug concentration may be determined by the detection and/or measurement of the fluorescence and/or spectra of such drugs, and/or drug breakdown products (metabolites), and/or compounds having concentrations affected by a drug, in targeted microstructures such as blood or skin.
- miniaturization of the described technologies utilizing MEMS (micro-electro-mechanical system), MOEMS (micro-opto-electro-mechanical system) technologies, and/or nanotechnologies.

What is claimed is:

1. A microscope comprising:
 - an excitation source for providing an optical excitation beam at an excitation wavelength λ ;
 - a scanner for scanning the excitation beam on a sample;
 - an objective for irradiating the sample with the excitation beam scanned by the scanner and for collecting an emission beam from the sample;
 - a first detector for detecting a plurality of multiphoton signals;
 - an emission light path allowing transmission from the objective to the first detector a wavelength band limited to greater than or equal to $\lambda/2$ and less than λ , wherein the plurality of multiphoton signals have wavelengths within the wavelength band;
 - wherein the plurality of multiphoton signals comprises a first multiphoton signal and a second multiphoton signal of different types.
2. A microscope according to claim 1 wherein the first multiphoton signal comprises a two photon fluorescence signal.
3. A microscope according to claim 1 or 2 wherein the second multiphoton signal comprises a second harmonic generation signal.
4. A microscope according to any one of claims 1 to 3 wherein the emission light path comprises a first wavelength separator.

5. A microscope according to claim 4 wherein the first wavelength separator comprises a dichroic.
6. A microscope according to claim 4 or 5 wherein the first wavelength separator comprises a shortpass filter.
7. A microscope according to any one of claims 1 to 6, wherein the scanner comprises a resonant scanner for scanning a fast axis.
8. A microscope according to any one of claims 1 to 7, wherein the first wavelength separator divides the emission beam collected by the objective into the first signal and a second signal, the microscope further comprising a second detector for detecting the second signal.
9. A microscope according to claim 8, wherein the second signal comprises a confocal reflectance signal.
10. A microscope according to claim 4, further comprising:
a spectrometer;
a second wavelength separator between the first wavelength separator and the first detector, the second wavelength separator for directing a portion of the first signal to the spectrometer.
11. A microscope according to any one of claims 1 to 10 comprising an excitation power attenuator.

12. A microscope according to claim 1 comprising a frame grabber connected to receive an output from the first detector and to store an image wherein pixels of the image represent an output of the first detector at corresponding locations on the sample.
13. A microscope according to claim 12 comprising a display connected to display images acquired by the frame grabber.
14. A microscope according to claim 12 wherein the frame grabber acquires images at a rate of at least 12 images per second.
15. A microscope according to claim 1 wherein the excitation source is controllable to change the excitation wavelength.
16. A microscope according to claim 15 wherein the excitation wavelength is controllable in the range of at least 720 nm to 950 nm.
17. A microscope according to claim 15 or 16 wherein the excitation source comprises a femtosecond laser.
18. A microscope according to claim 15 or 16 wherein the excitation wavelength is an infrared wavelength.
19. A microscope according to claim 18 wherein the first detector is operative to detect light in the visible spectrum.

20. A microscope according to claim 18 wherein the first detector is operative to detect light in the visible and ultraviolet spectrum.
21. A microscope according to claim 18 wherein the emission light path is configured to block infrared light from reaching the first detector and to pass light in the visible and ultraviolet spectrum to the first detector.
22. A microscope for *in vivo* imaging of a subject, the microscope comprising:
- an excitation source for providing an optical excitation beam;
 - a scanner for scanning the excitation beam on a target region of the subject, wherein the scanner comprises a resonant scanner;
 - an objective for irradiating the target region with the excitation beam scanned by the scanner and for collecting an emission beam from the target region;
 - a detector for detecting a plurality of multiphoton signals from the emission beam;
 - an adapter comprising a surface for detachably securing to an area around the target region;
 - a translation stage comprising a table and a base, the table movably coupled to the base, wherein the objective is mounted to the table and the base is coupled to the adapter.
23. A microscope according to claim 22, wherein the adapter comprises a hollow interior for holding an immersion medium.

24. A microscope according to claim 22 or 23 wherein the surface of the adapter comprises a tacky adhesive.
25. A microscope according to any one of claims 22 to 24 wherein the adapter comprises straps for detachably securing the adapter to the target region, wherein the straps are configured to wrap around a portion of the subject's body.
26. A microscope according to any one of claims 22 to 25 wherein the base and the adapter are integrally formed.
27. A photothermolysis method comprising:
 - (a) visualizing a target structure using a microscope according to any one of claims 1 to 16;
 - (b) tuning an excitation light source of the assembly to a wavelength at which multiphoton absorption will occur within the target structure;
 - (c) increasing power output of the excitation light source to cause heat to be generated within the target structure.
28. A photothermolysis method according to claim 27 wherein step (a) comprises visualizing the target with co-registered TPF, SHG and RCM imaging.
29. A photothermolysis method according to claim 27 wherein step (a) comprises spectrally analyzing the target structure.

30. A photothermolysis method according to any one of claims 27 to 29 wherein step (c) comprises destroying the target structure.
31. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises a hair follicle or hair shaft.
32. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises a cancer cell.
33. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises a cancer stem cell.
34. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises a blood vessel.
35. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises skin collagen.
36. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises a cosmetic skin blemish.
37. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises surface pigments of teeth.
38. A photothermolysis method according to any one of claims 27 to 29 wherein the target structure comprises subcutaneous adipose tissue.

1/39

PRIOR ART

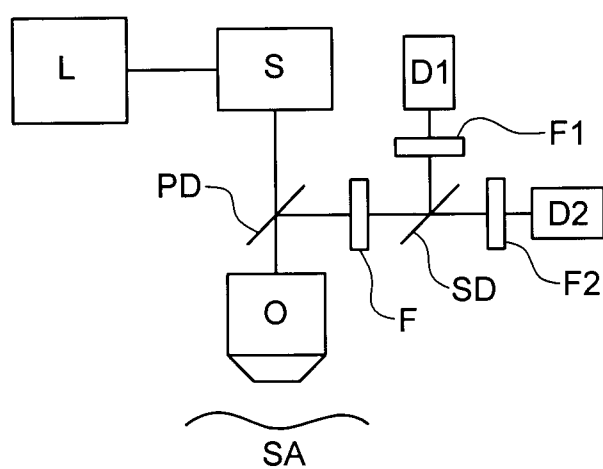


Figure 1

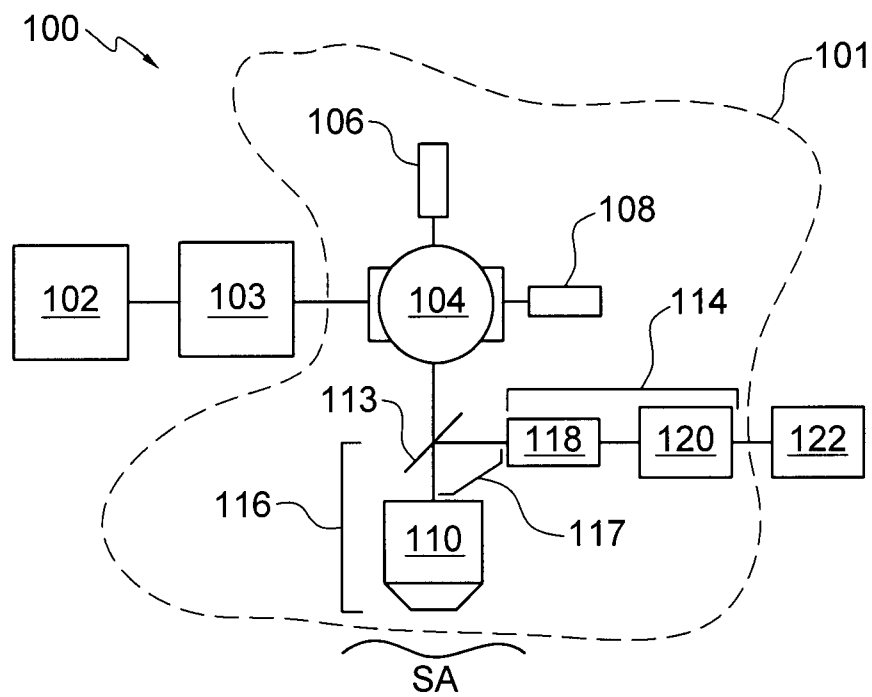


Figure 2A.

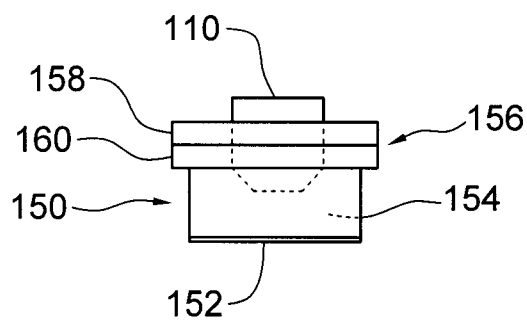


Figure 2B

3/39

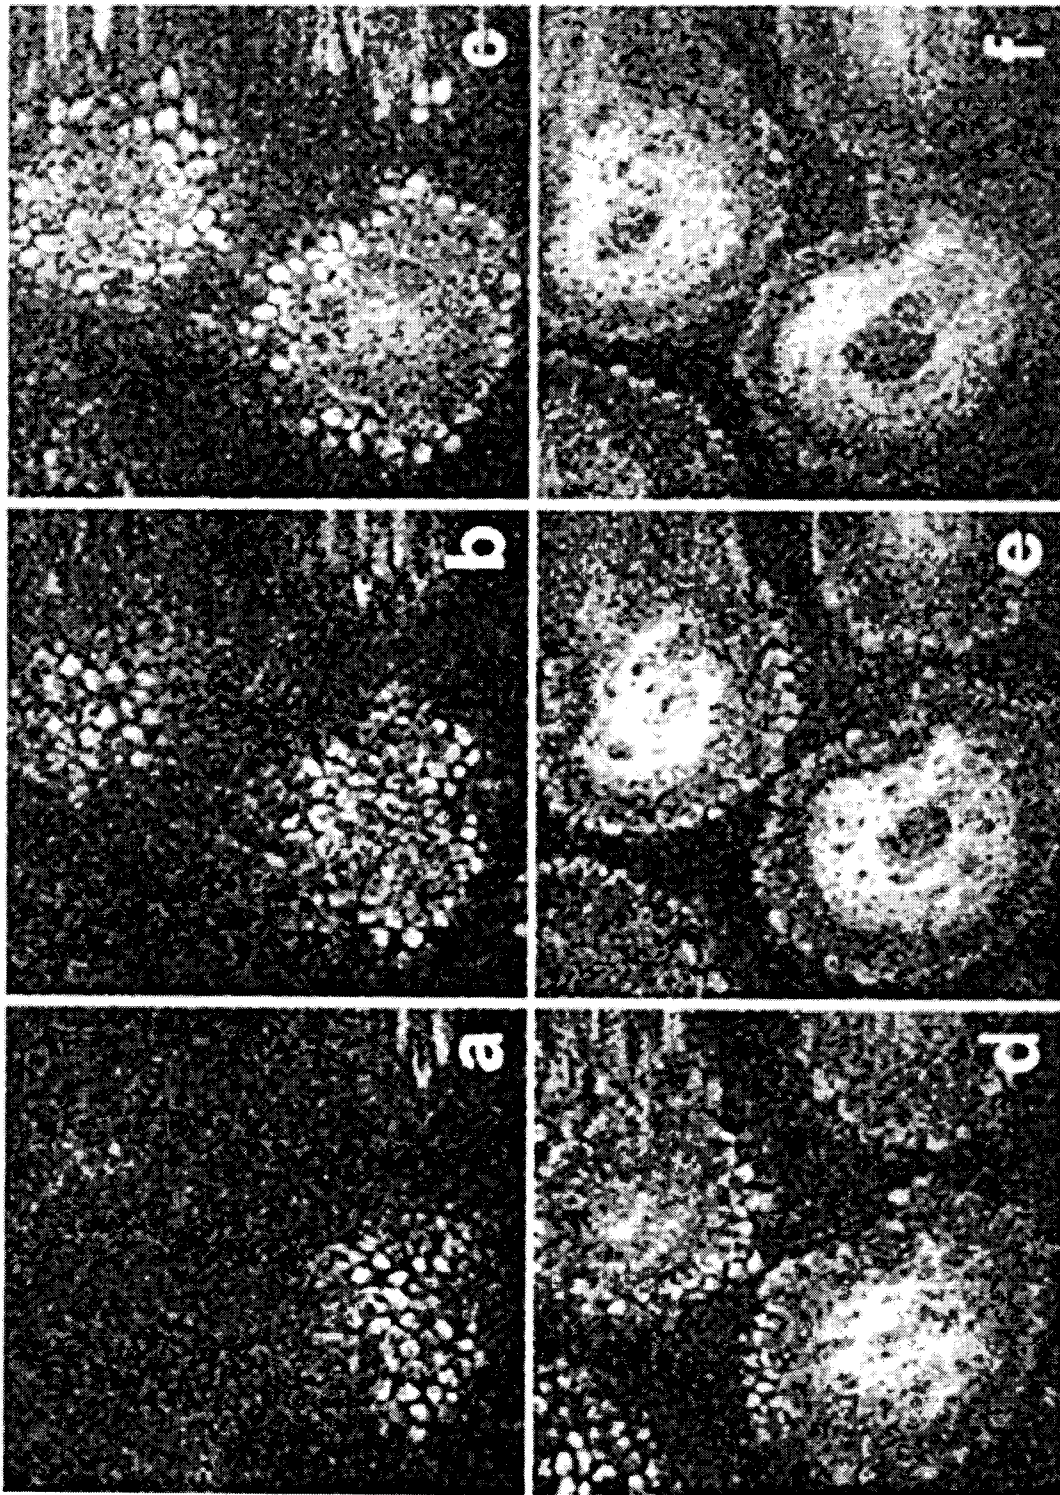


Figure 3

4/39

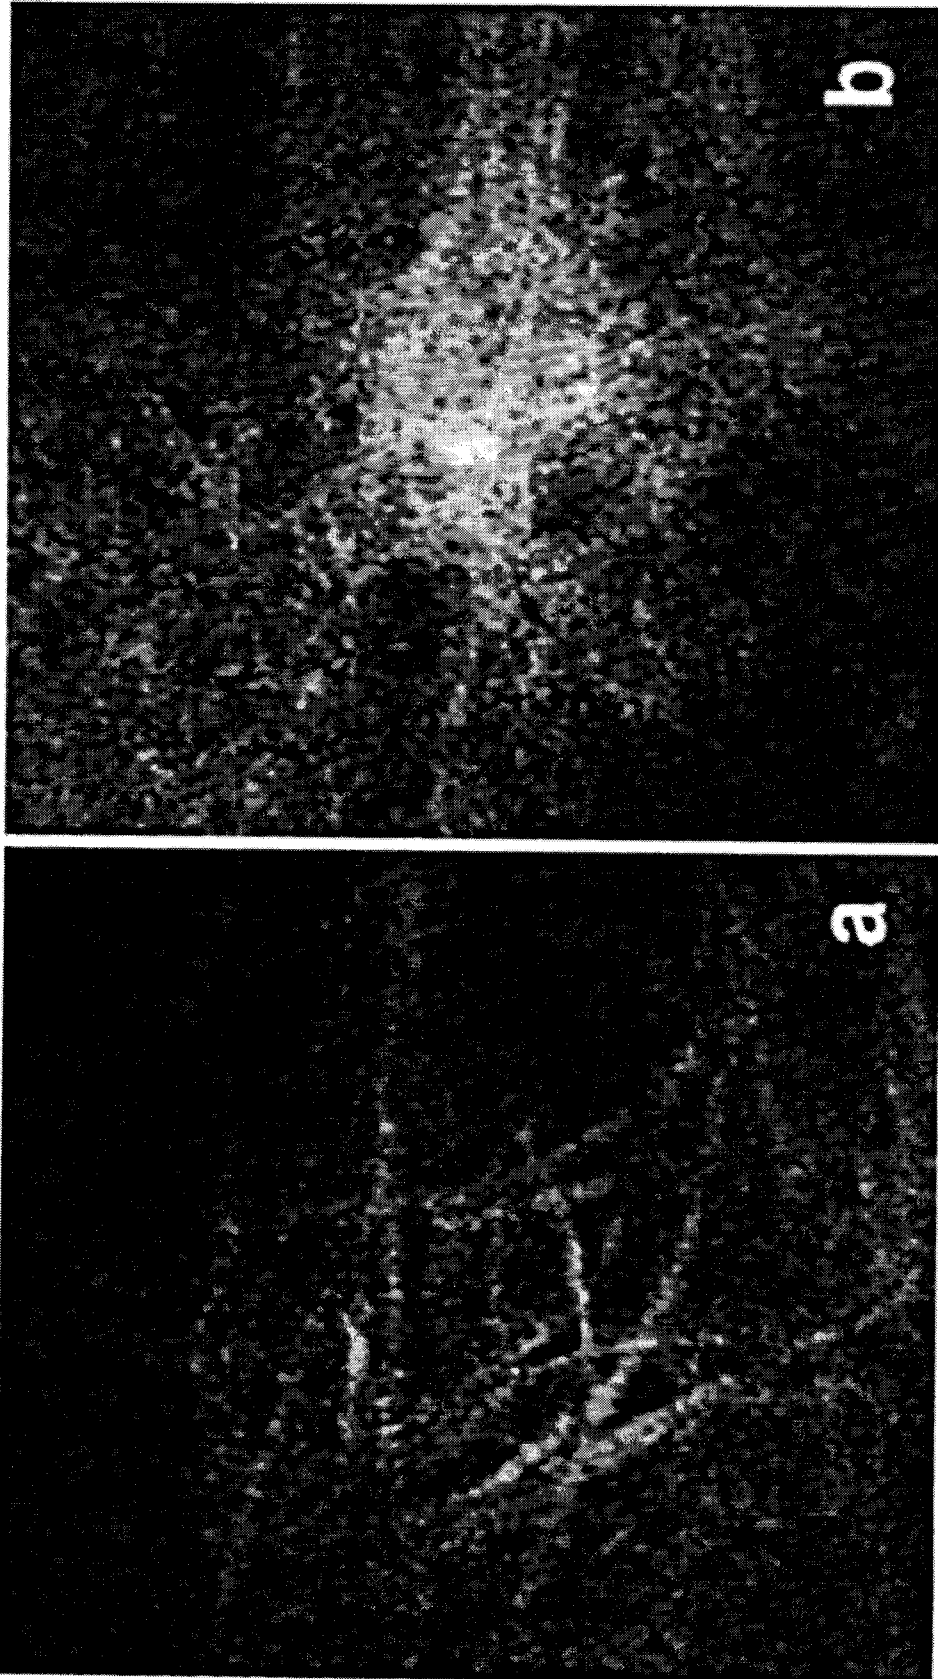


Figure 4

5/39

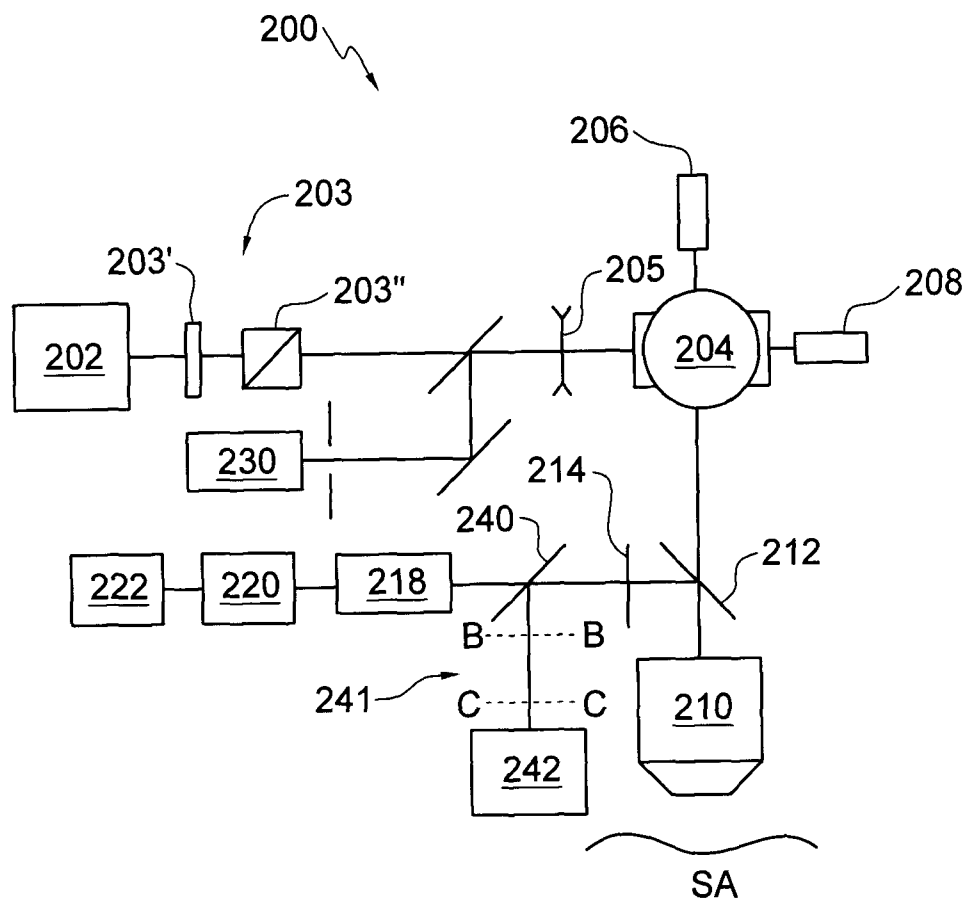


Figure 5A

6/39

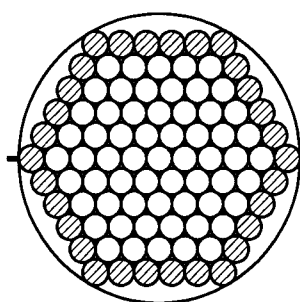


Figure 5B



Figure 5C

7/39



Figure 6

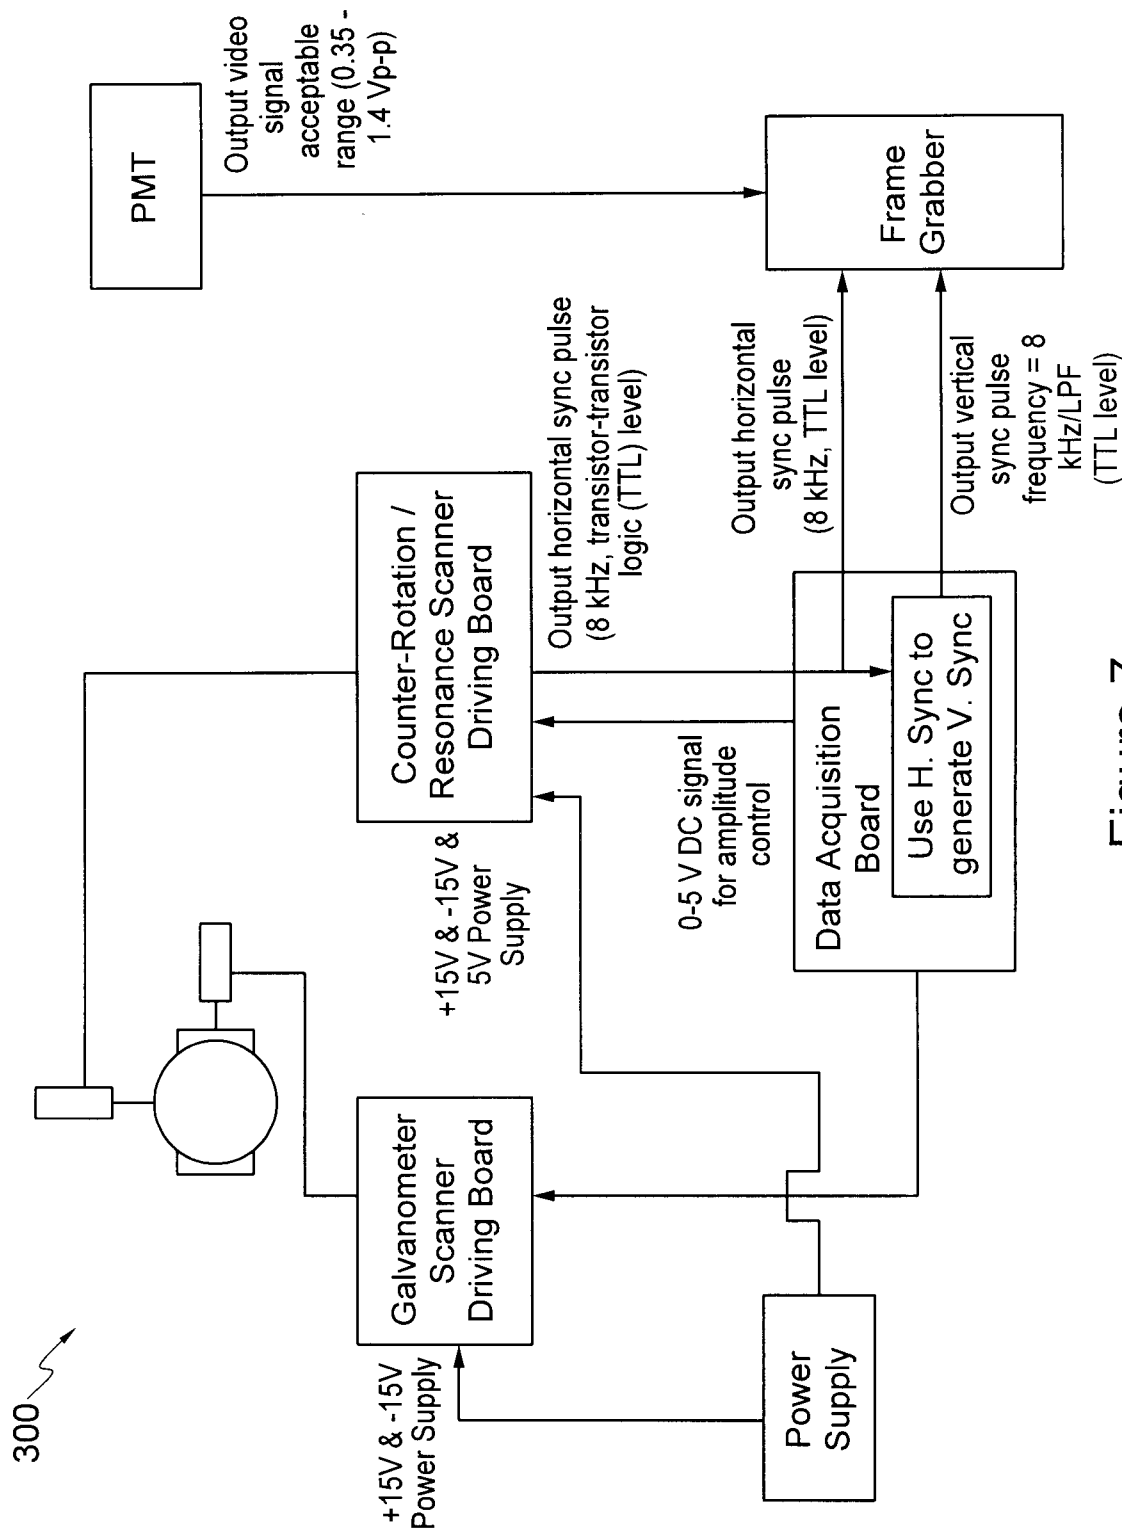


Figure 7

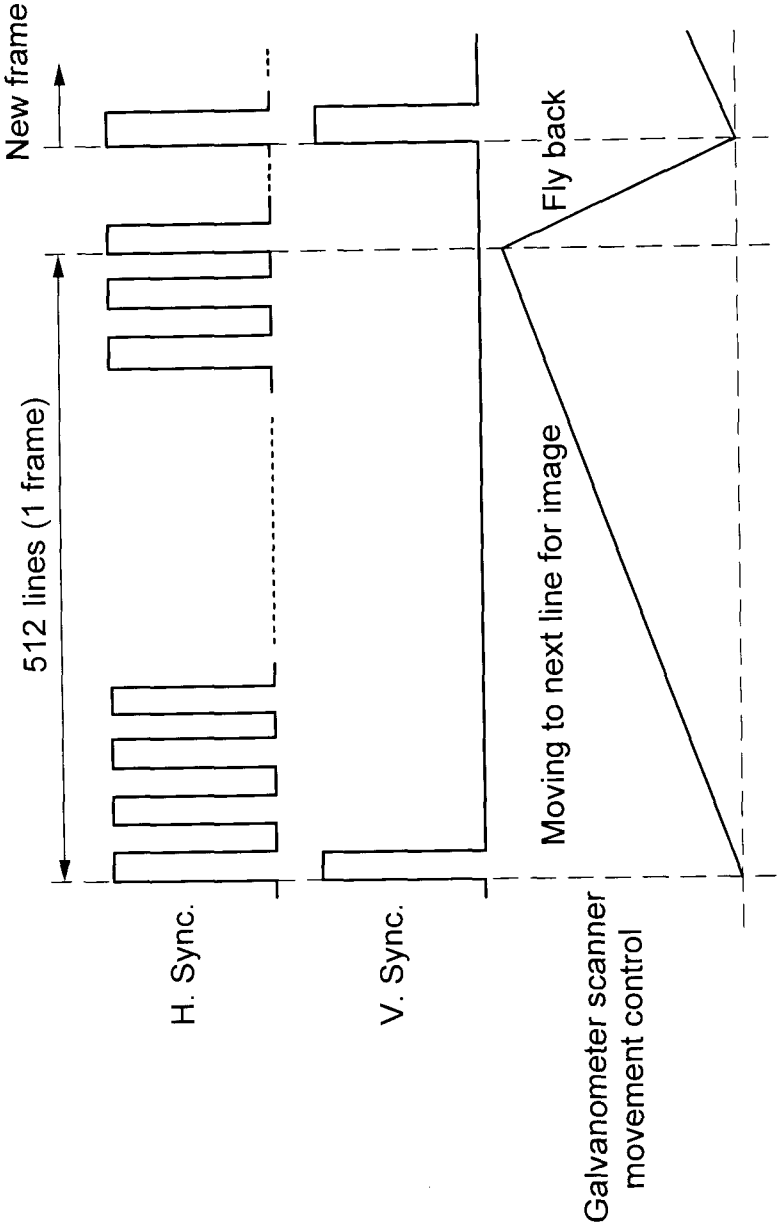


Figure 8

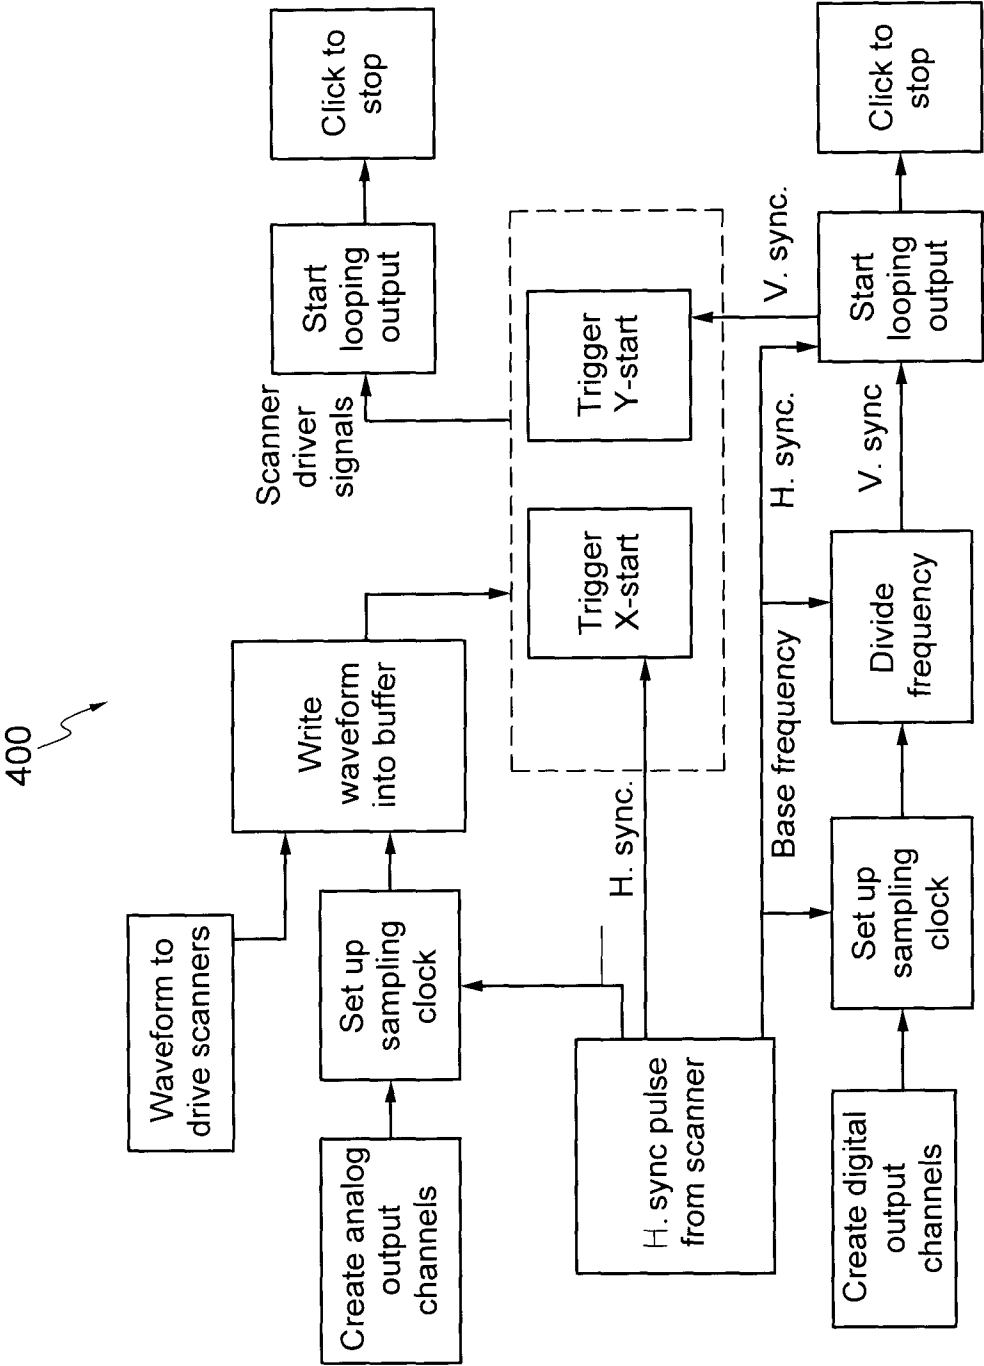


Figure 9

450

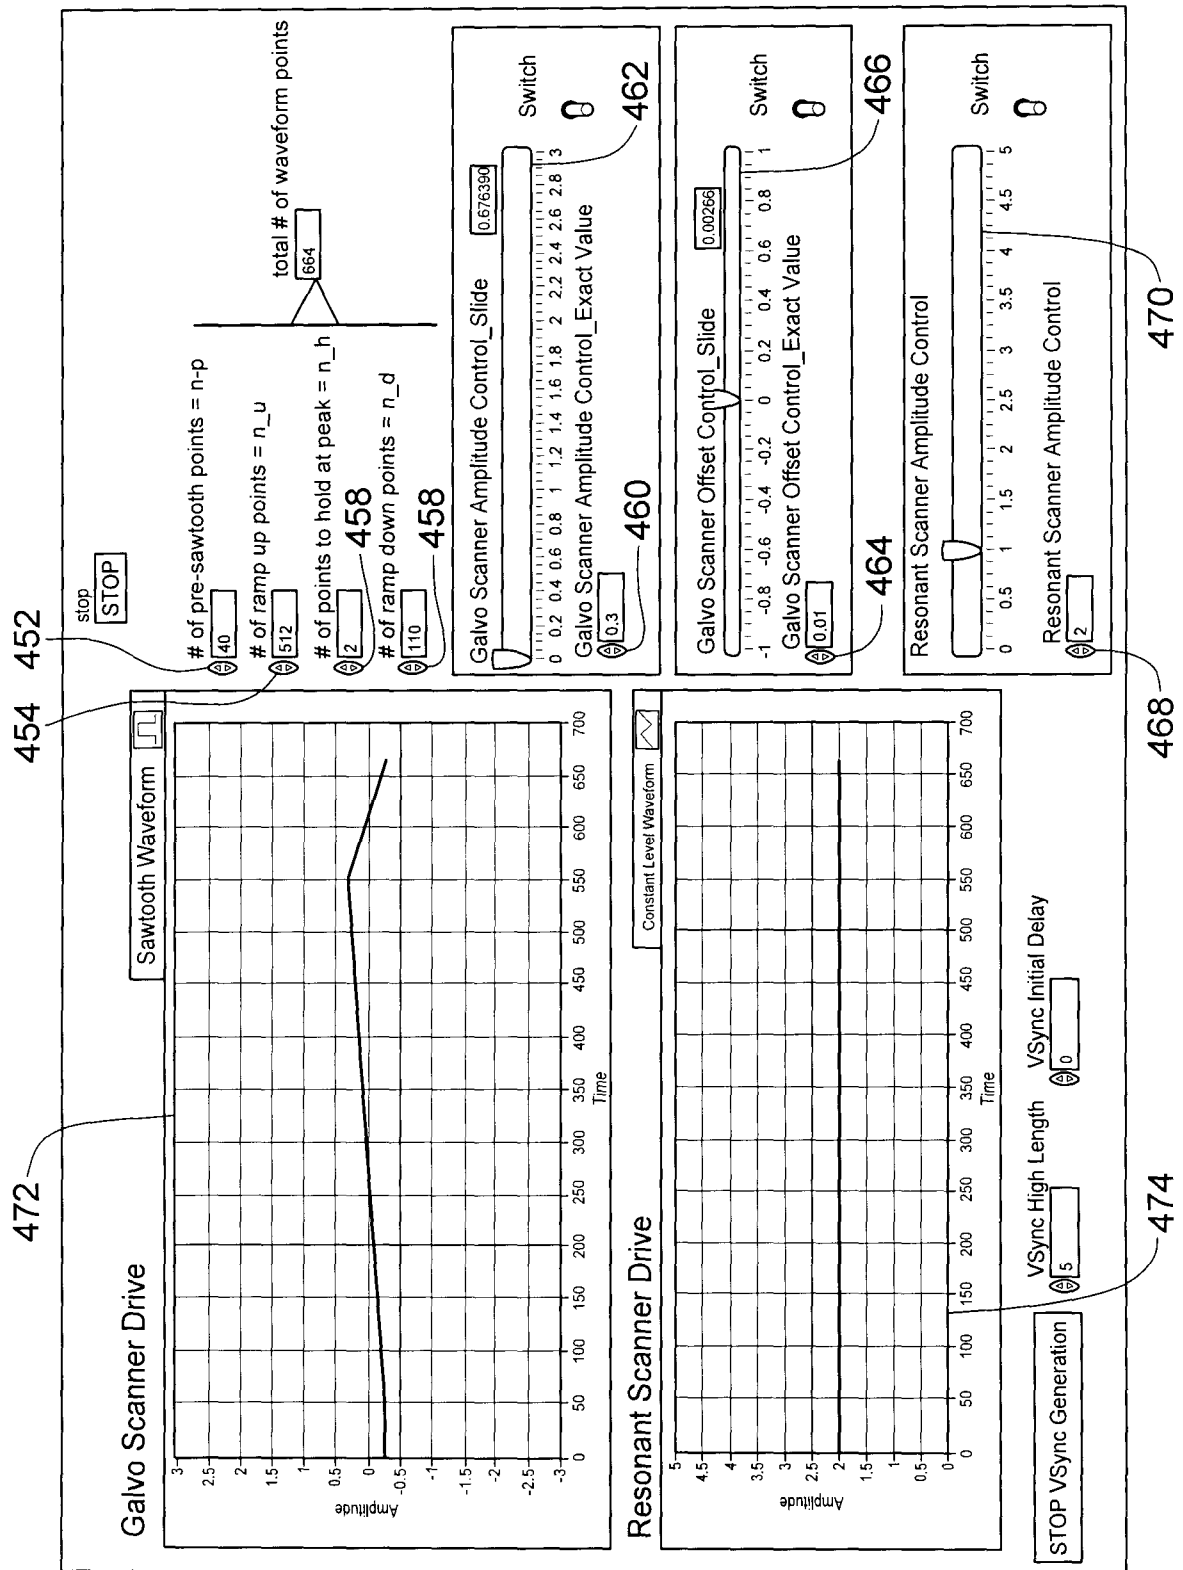


Figure 10

12/39

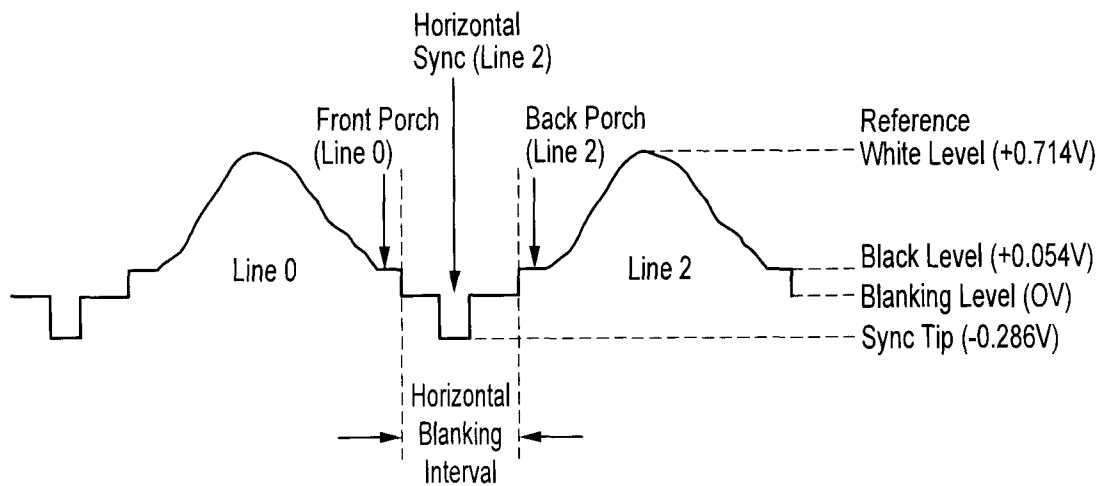


Figure 11

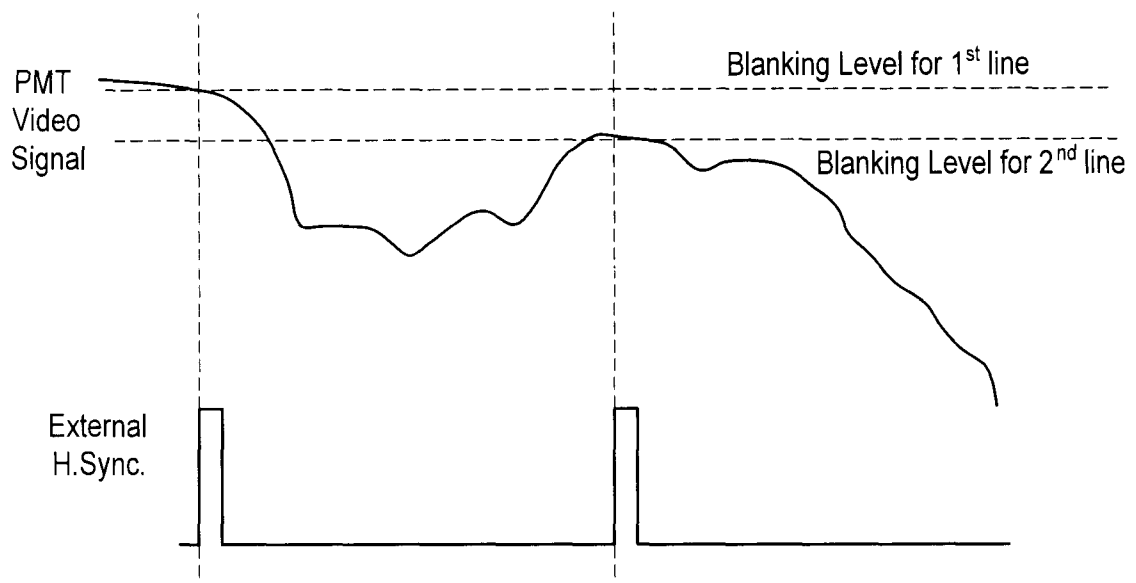


Figure 12

13/39

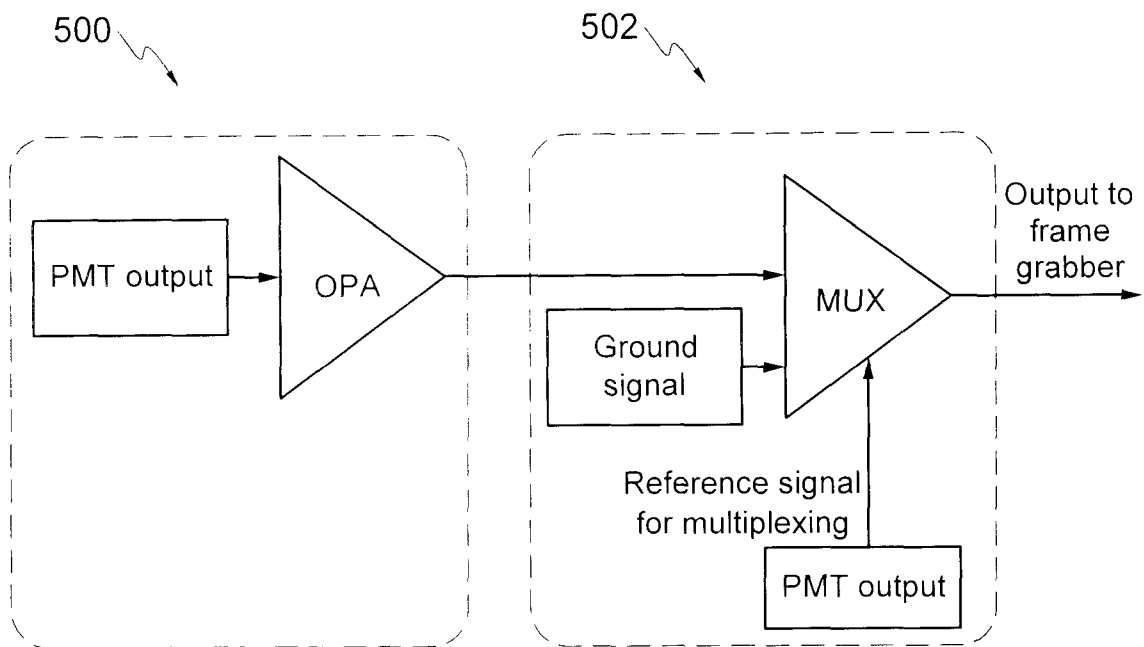


Figure 13

14/39



Figure 14A



Figure 14B

15/39

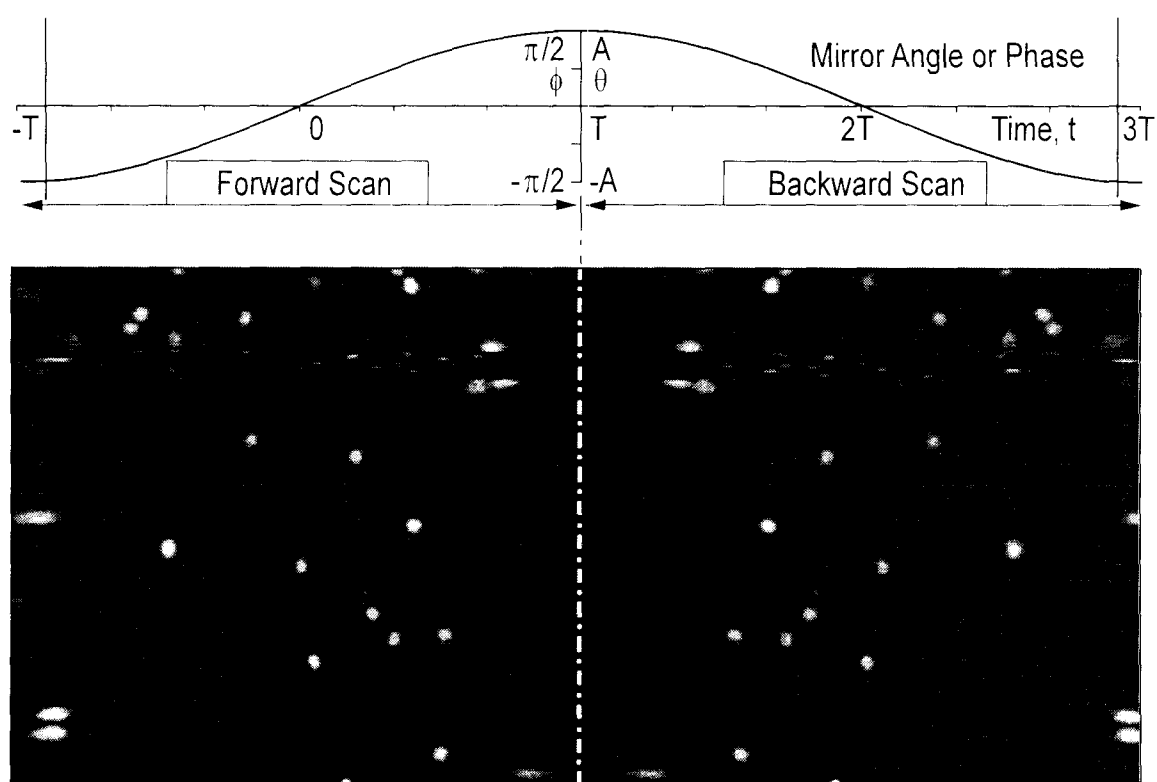


Figure 15

16/39

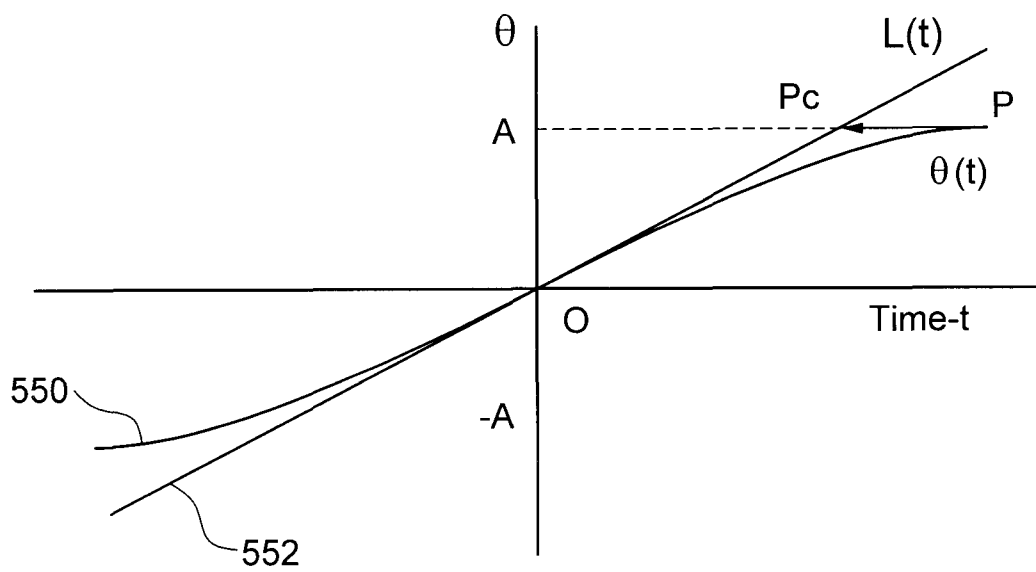


Figure 16

17/39

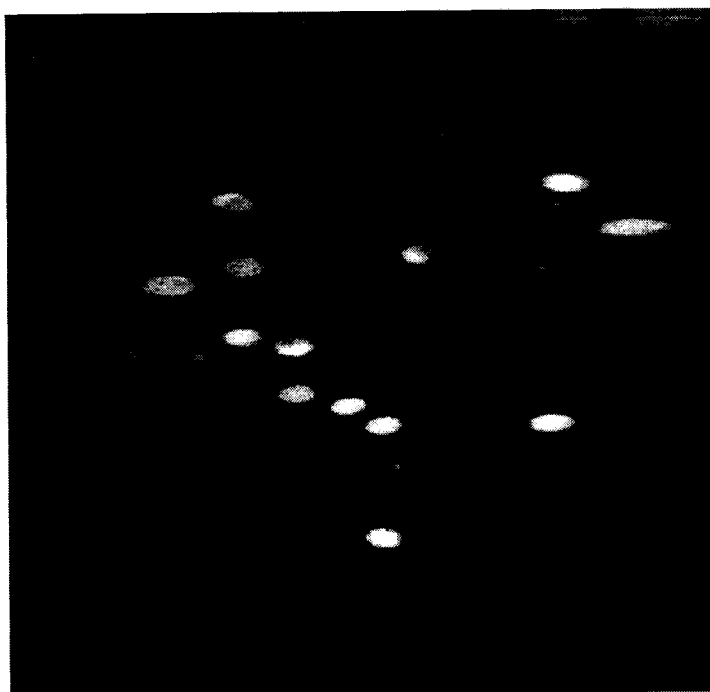


Figure 17A

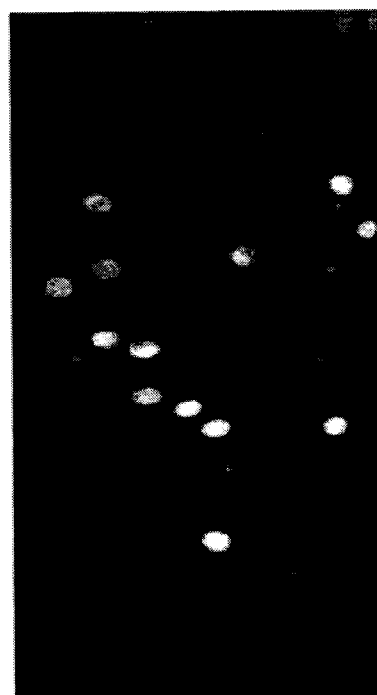


Figure 17B

18/39


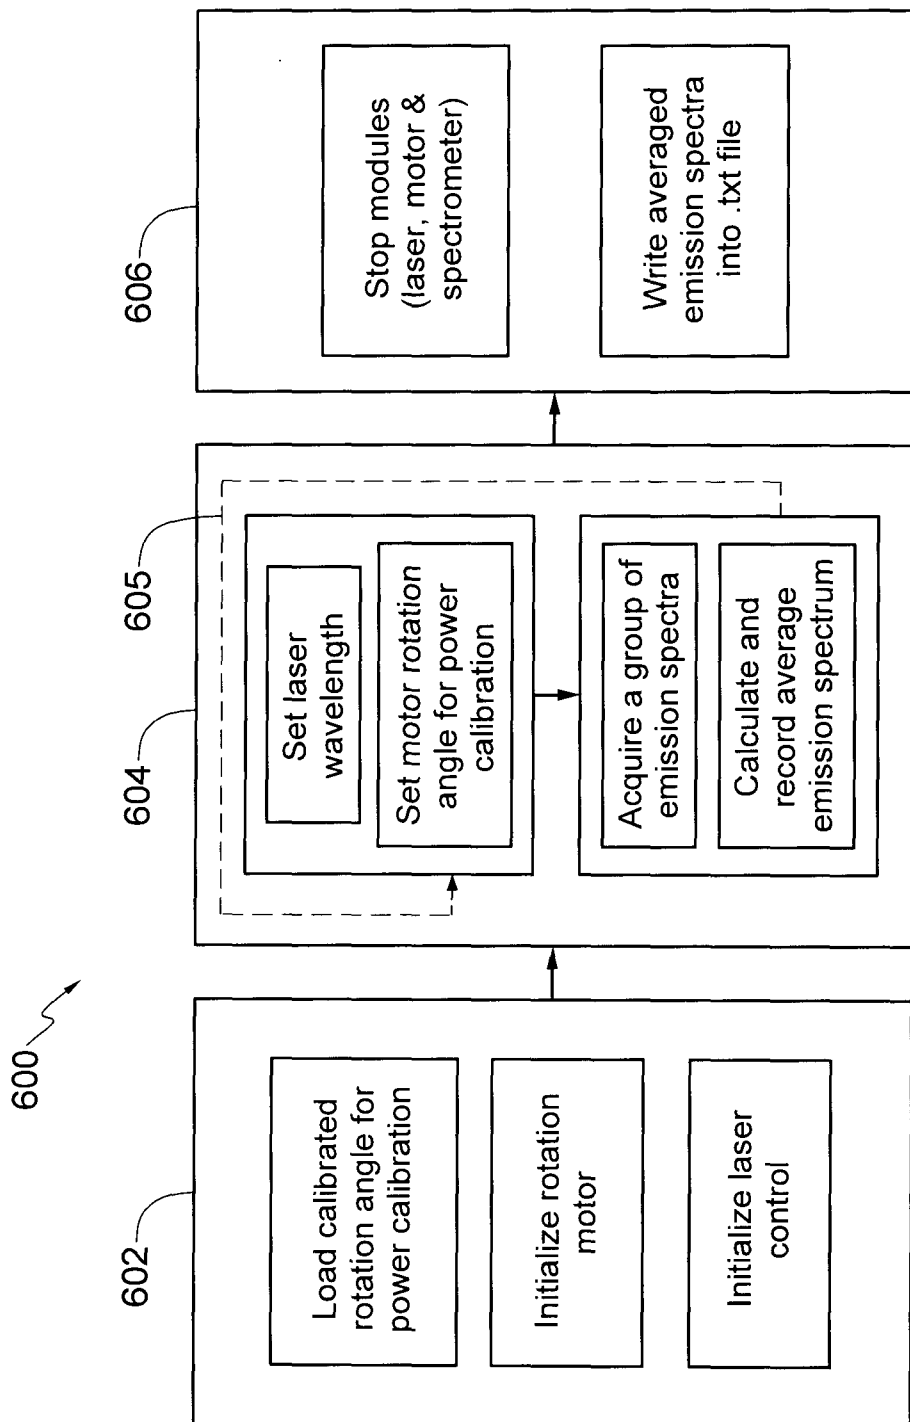


Figure 18

19/39

Figure 19

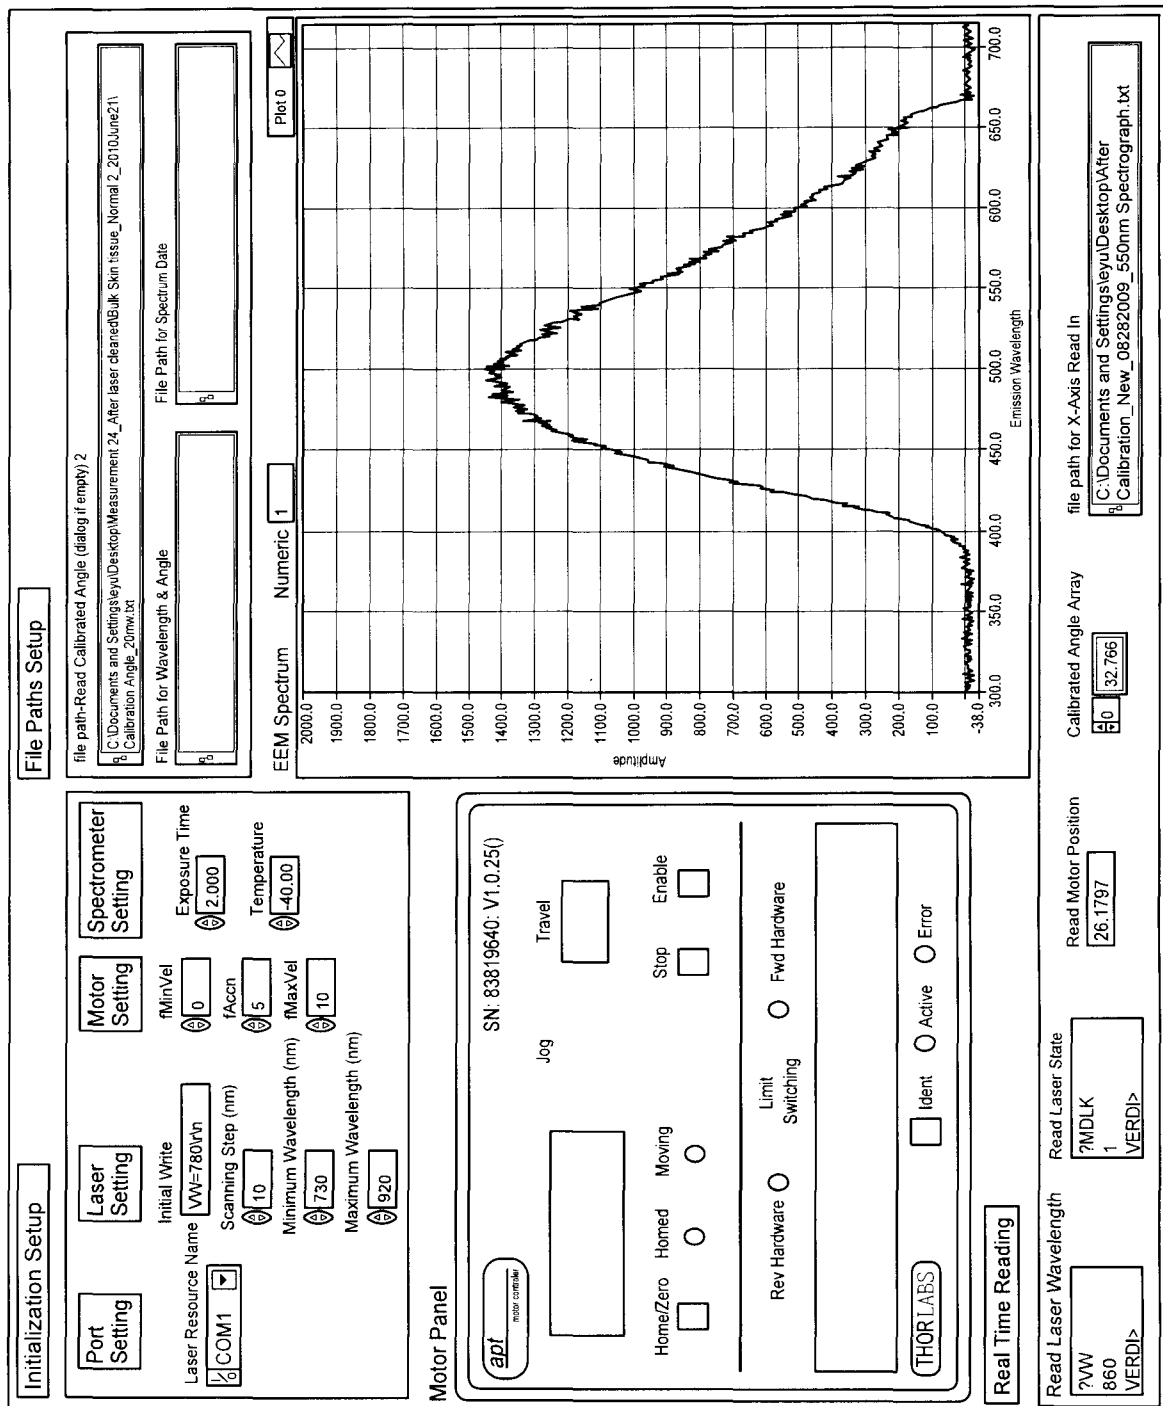

20/39

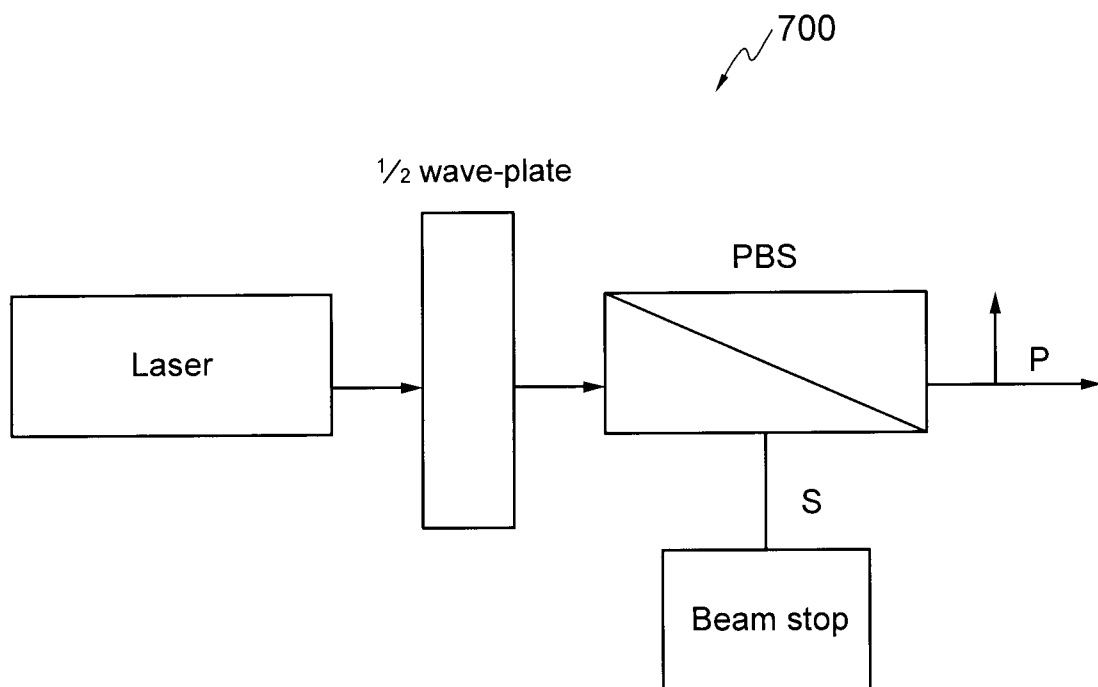


Figure 20

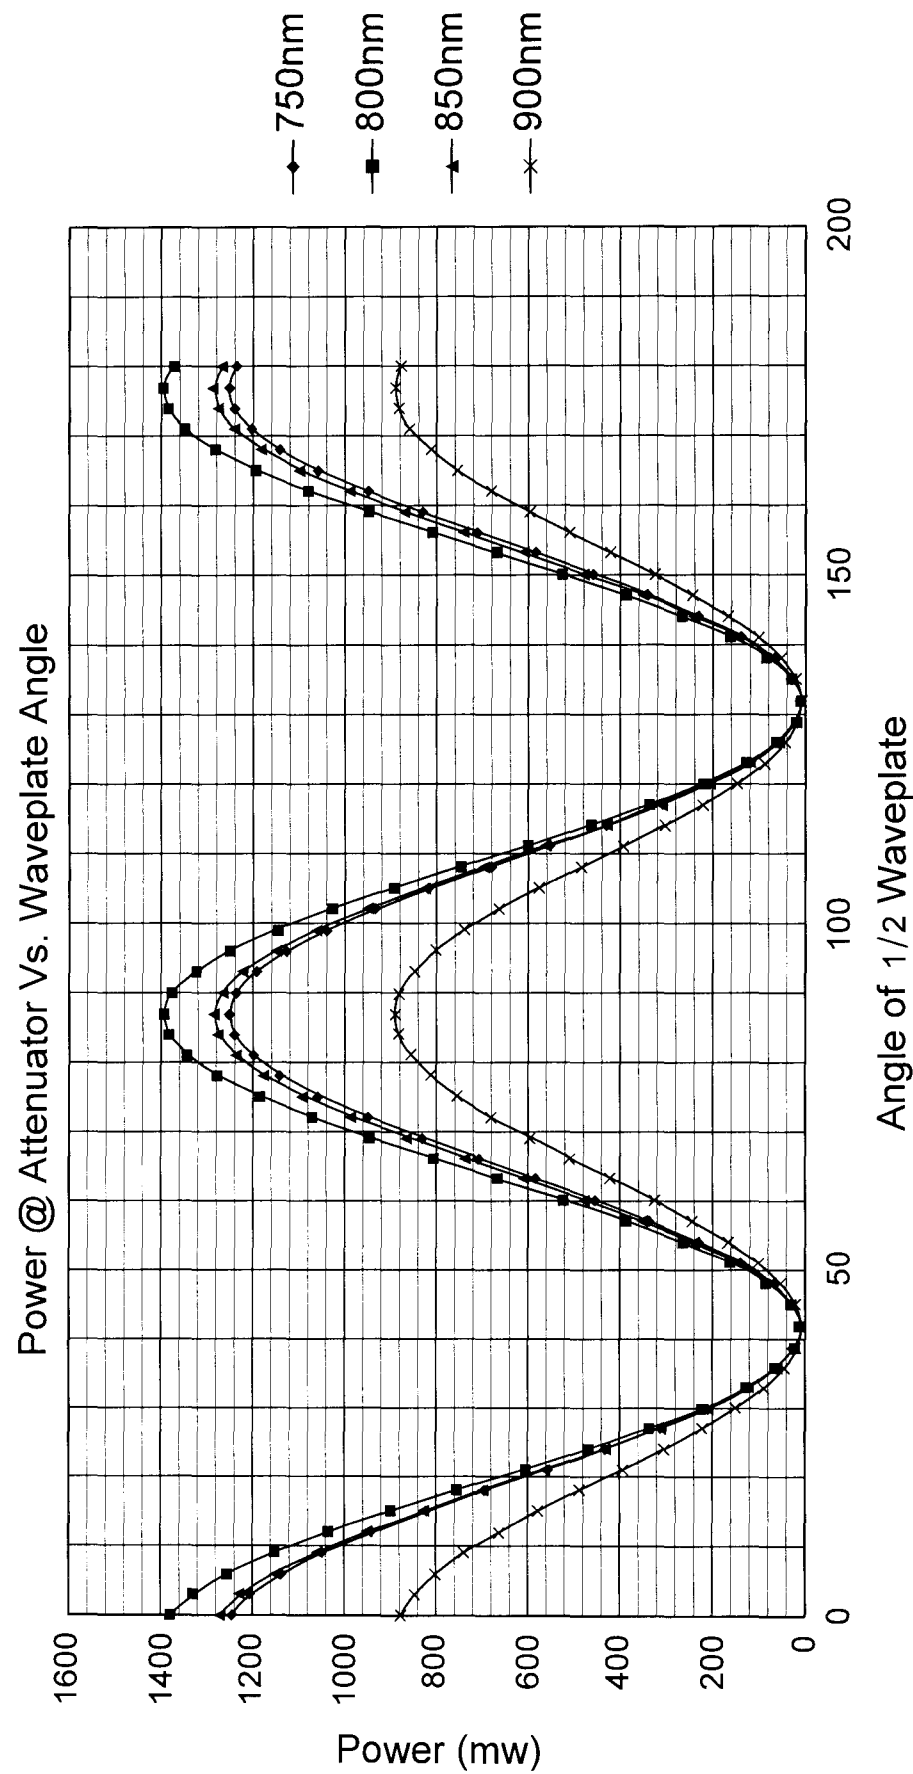


Figure 21

22/39

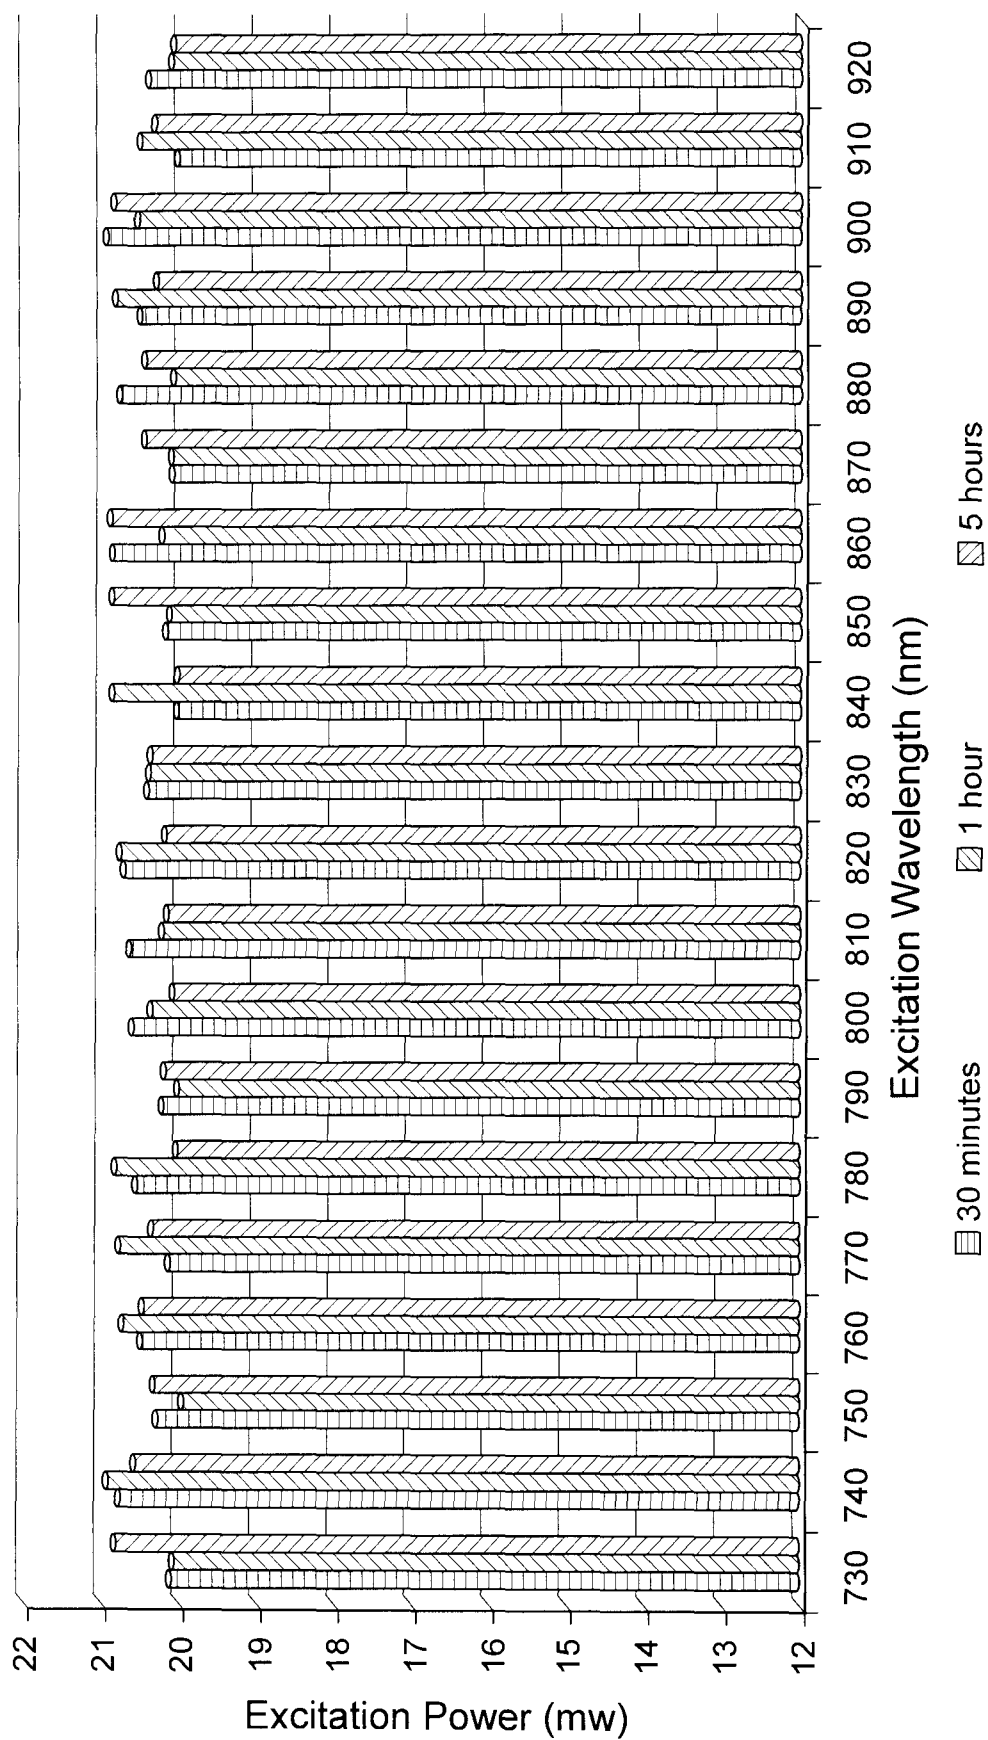


Figure 22

23/39

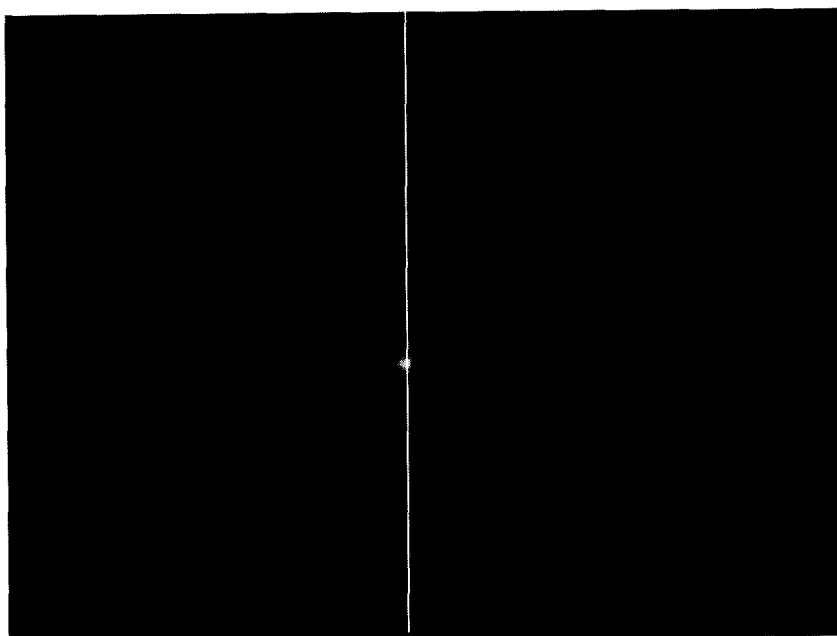


Figure 23A

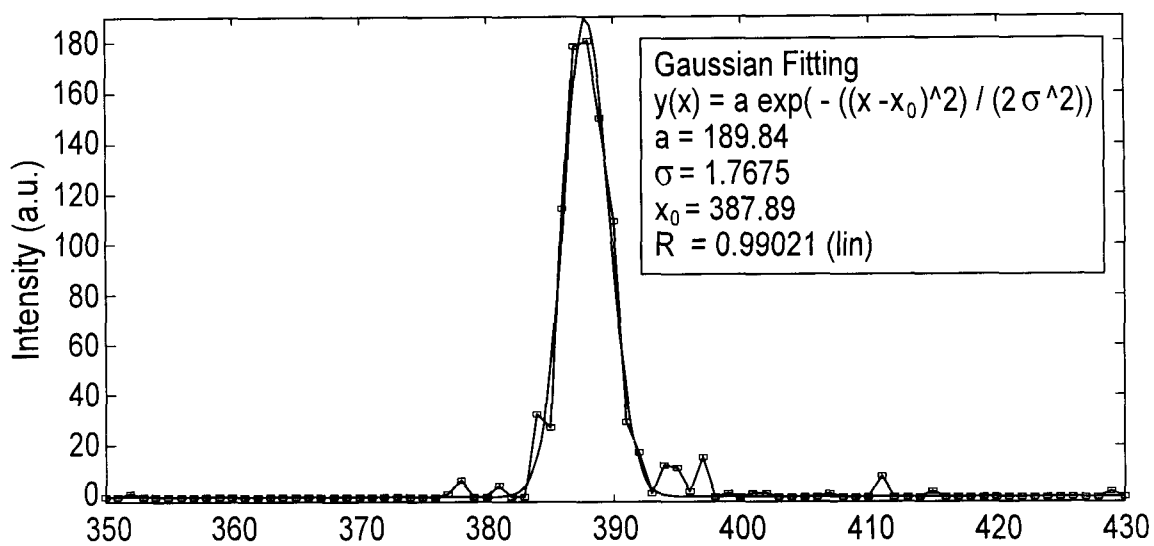
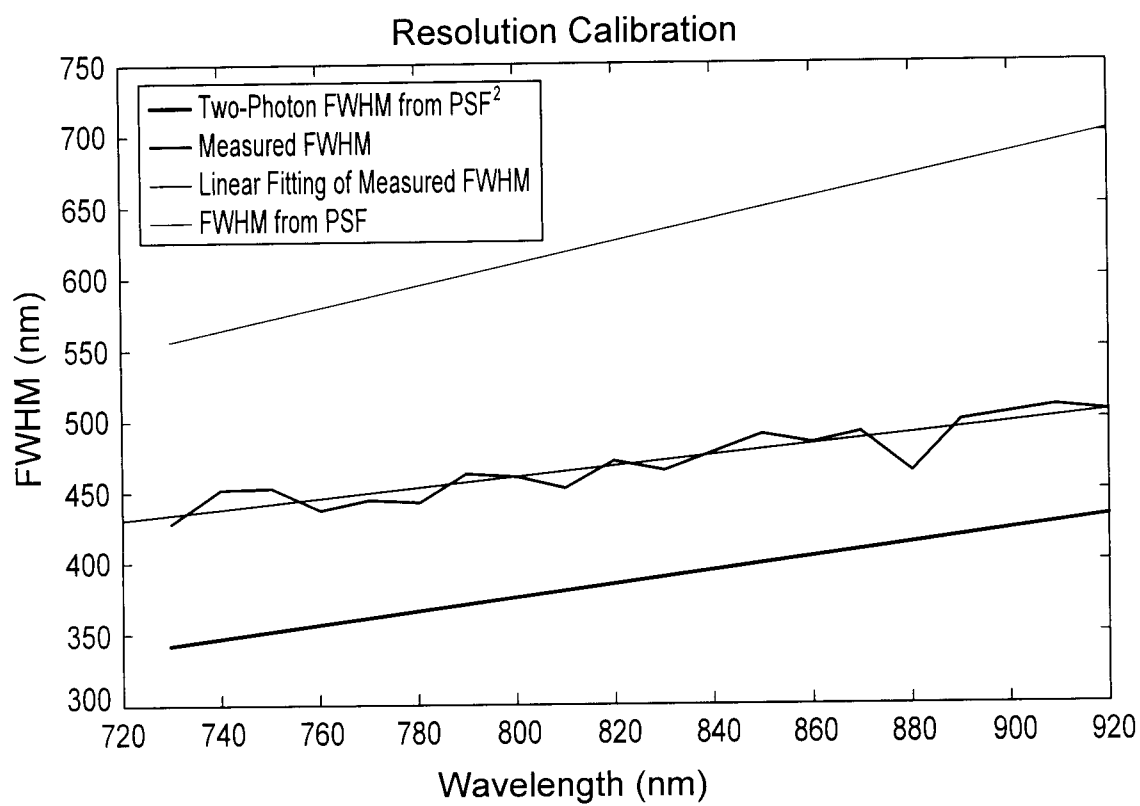


Figure 23B

24/39

**Figure 24**

25/39



Figure 25A



Figure 25B

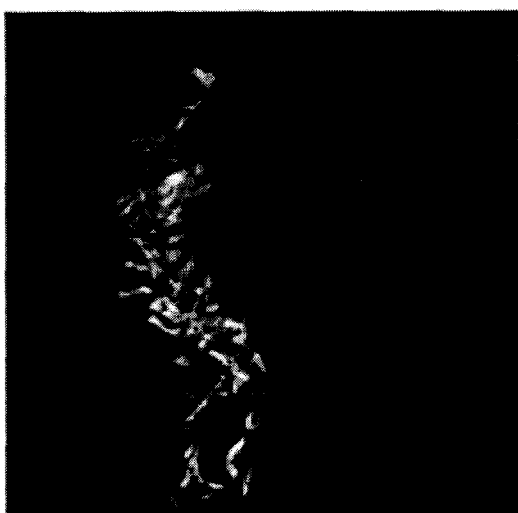


Figure 25C

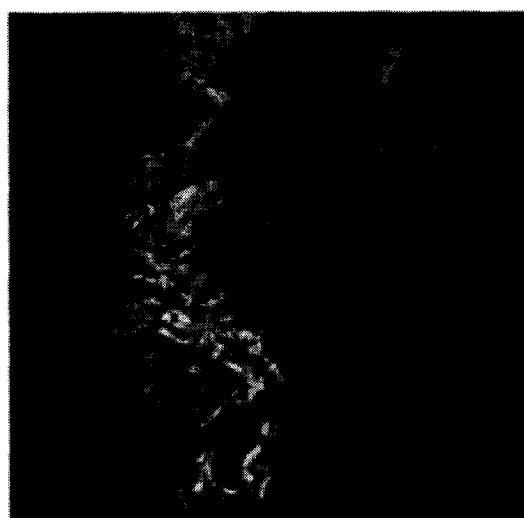


Figure 26

26/39

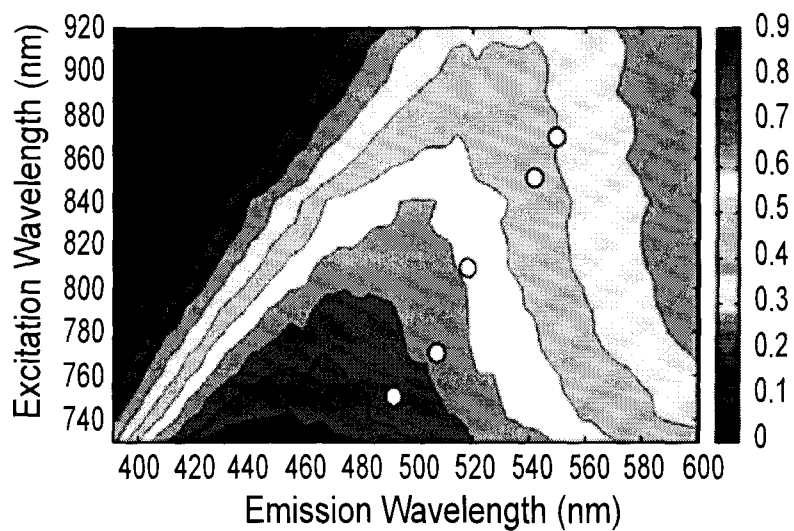


Figure 27A

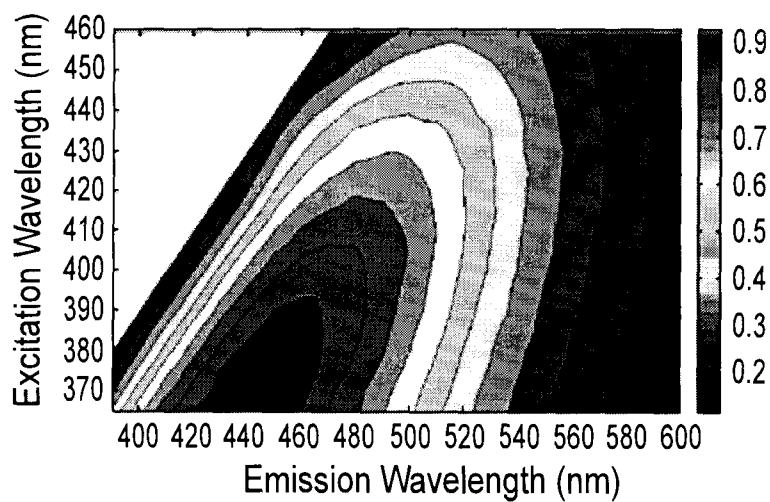


Figure 27B

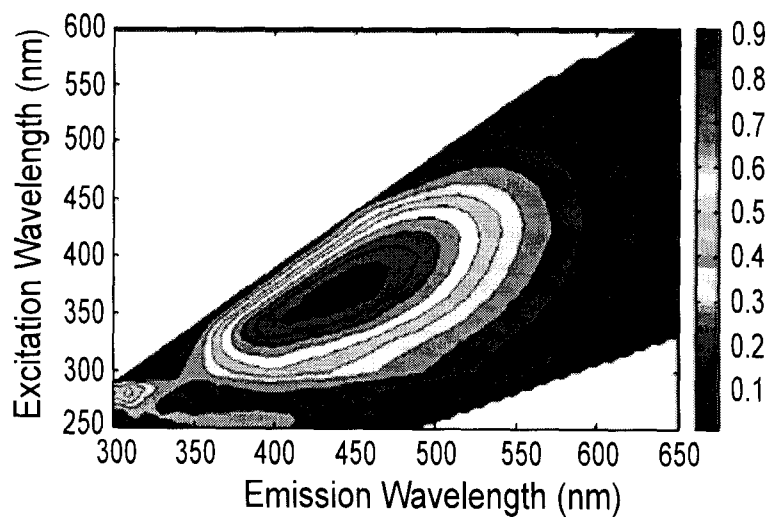


Figure 27C

27/39

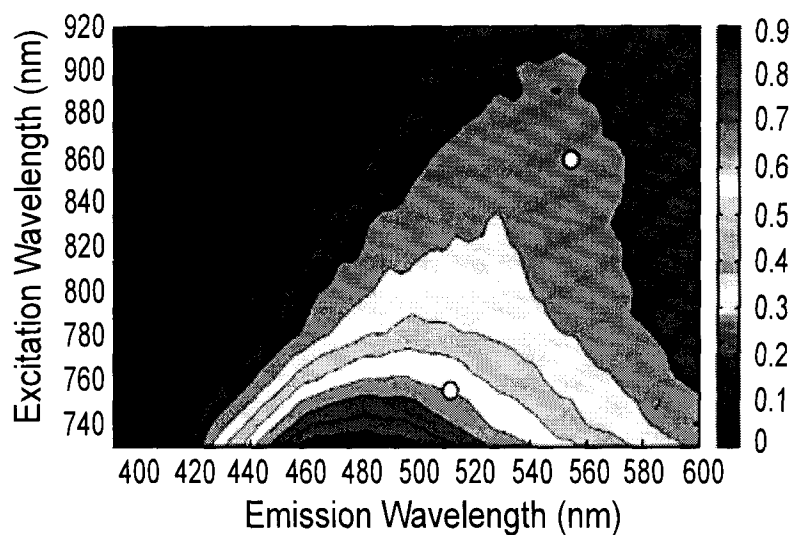


Figure 28A

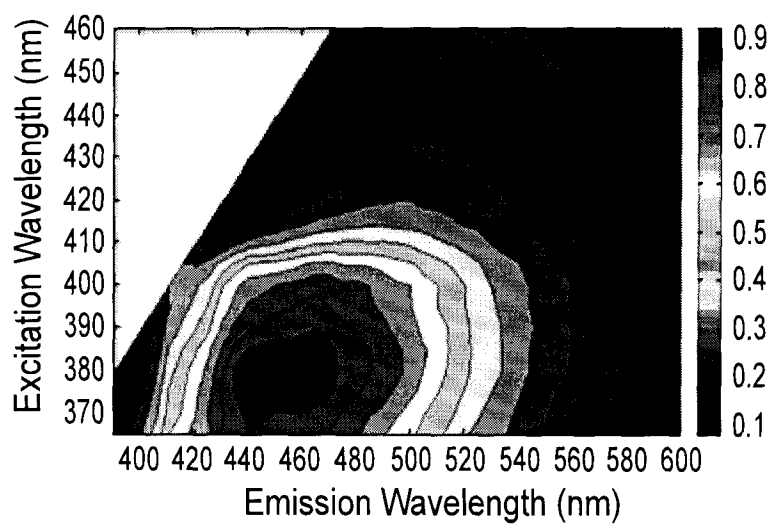


Figure 28B

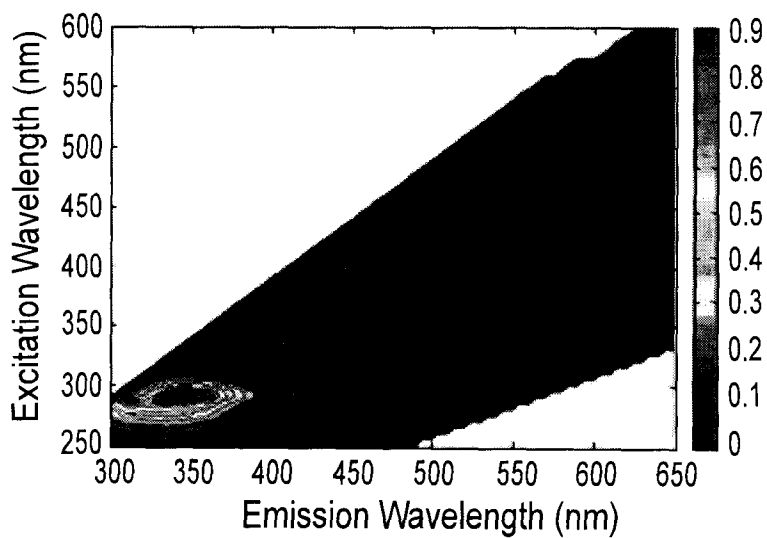


Figure 28C

SUBSTITUTE SHEET (RULE 26)

28/39

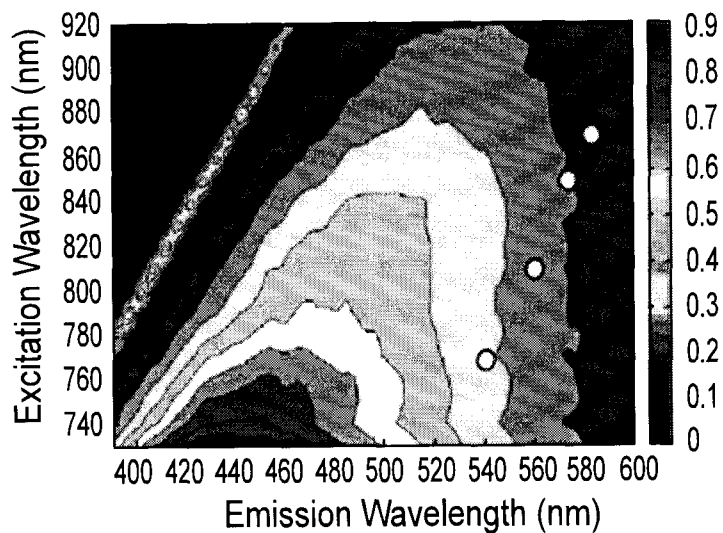


Figure 29A

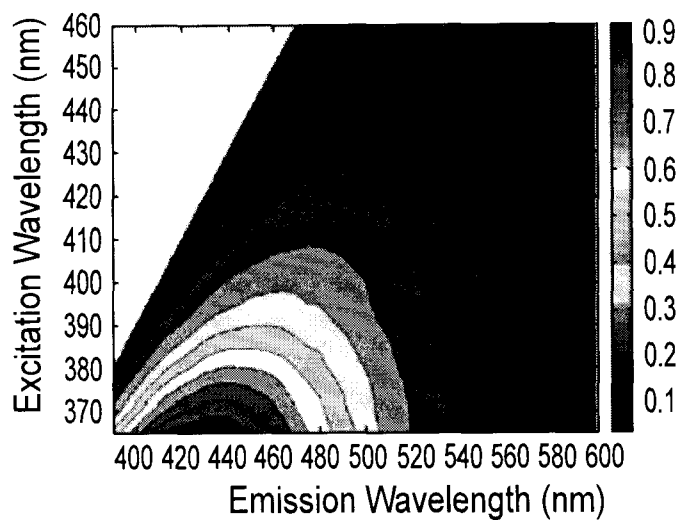


Figure 29B

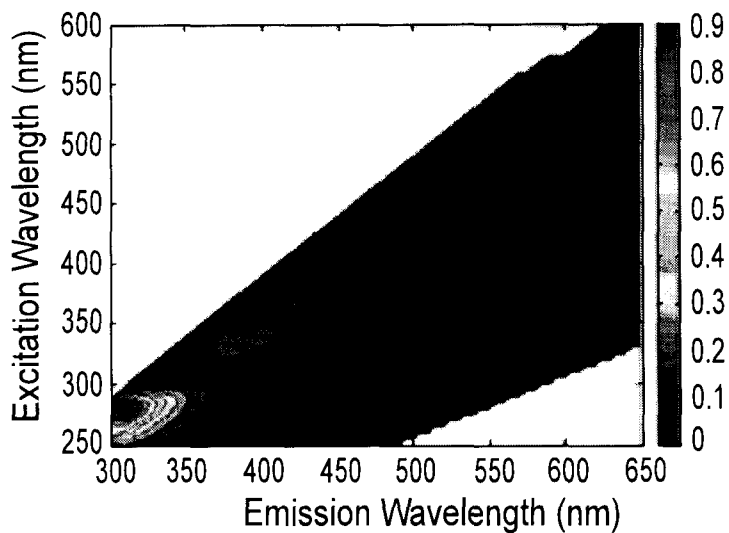


Figure 29C

29/39

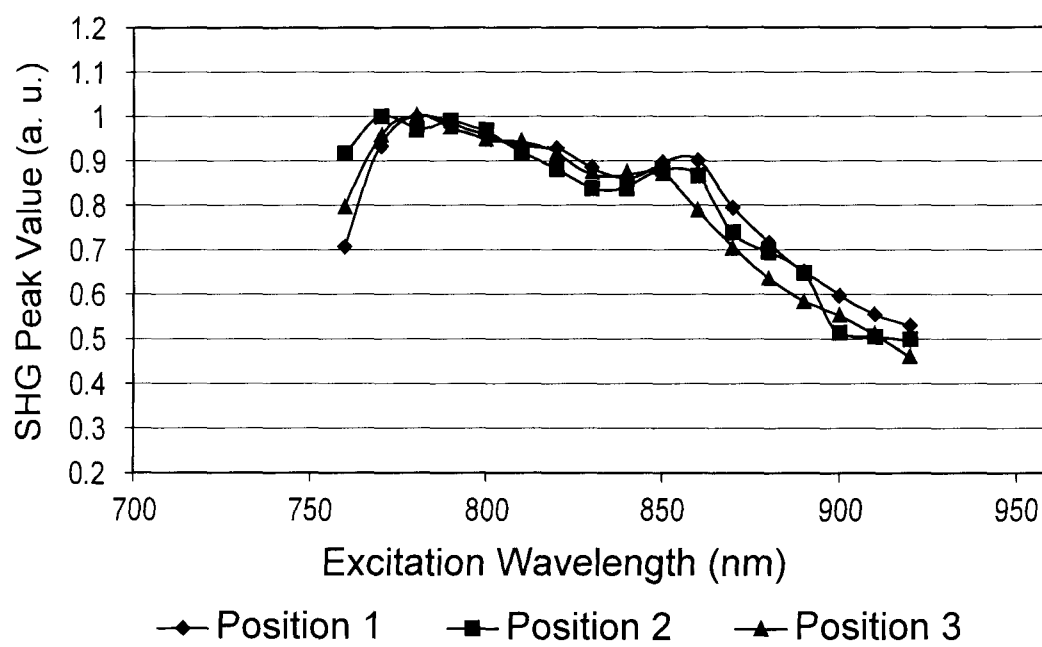


Figure 30

30/39

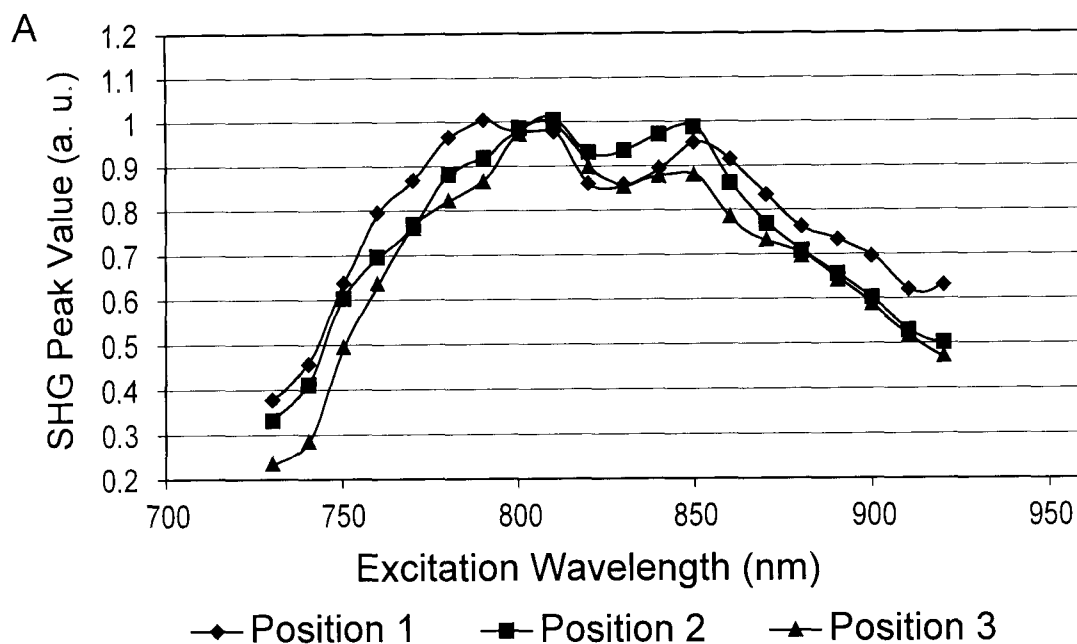


Figure 31A

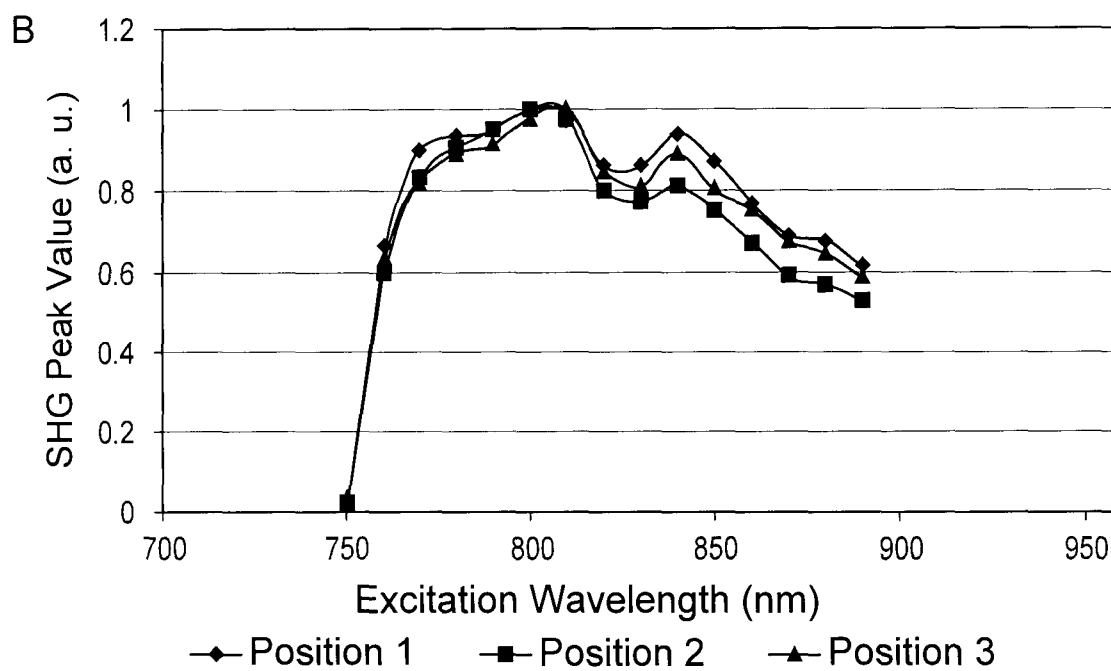


Figure 31B

31/39

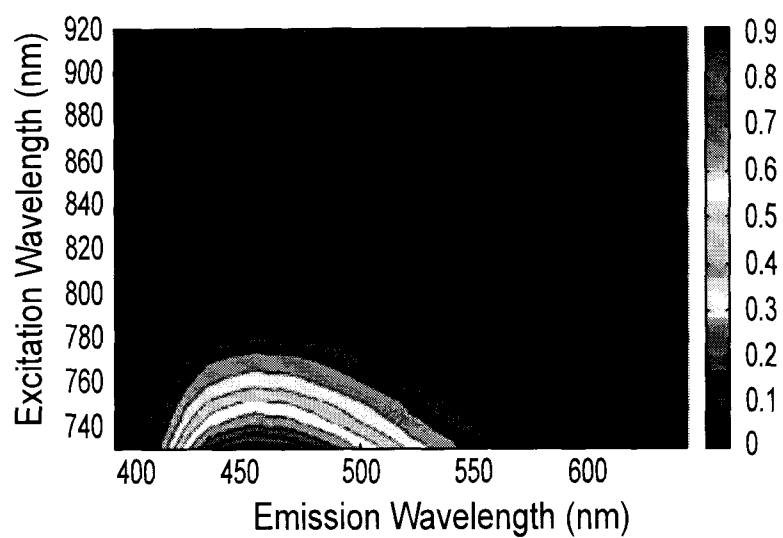


Figure 32A

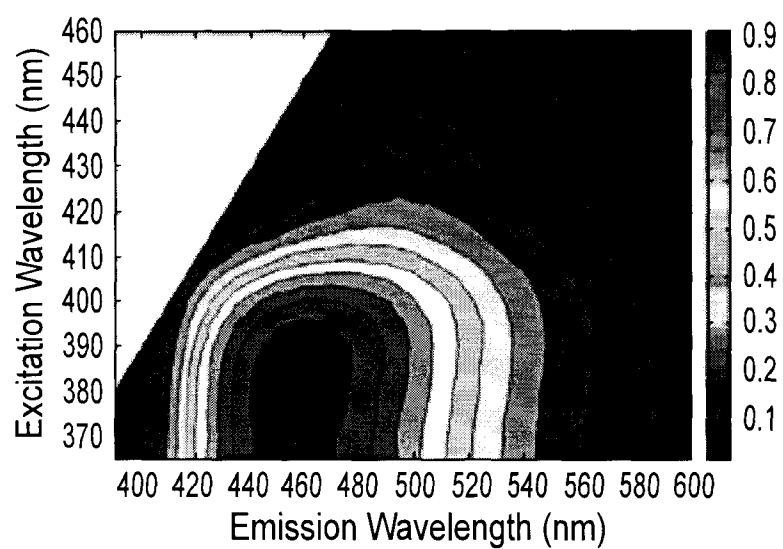


Figure 32B

32/39

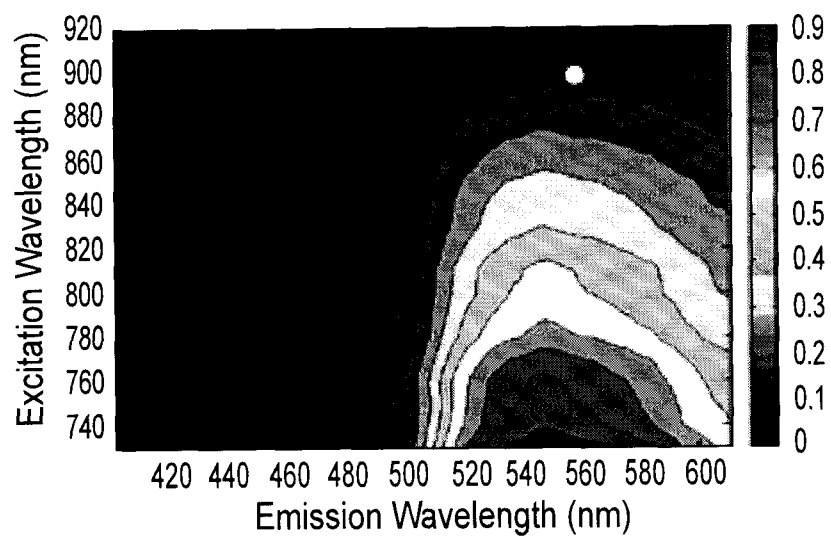


Figure 32C

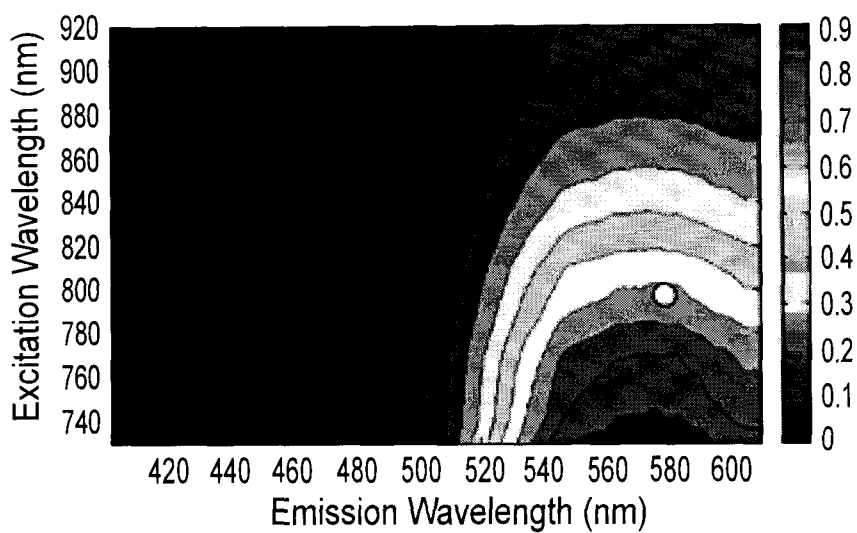


Figure 32D

33/39



Figure 33A



Figure 33B

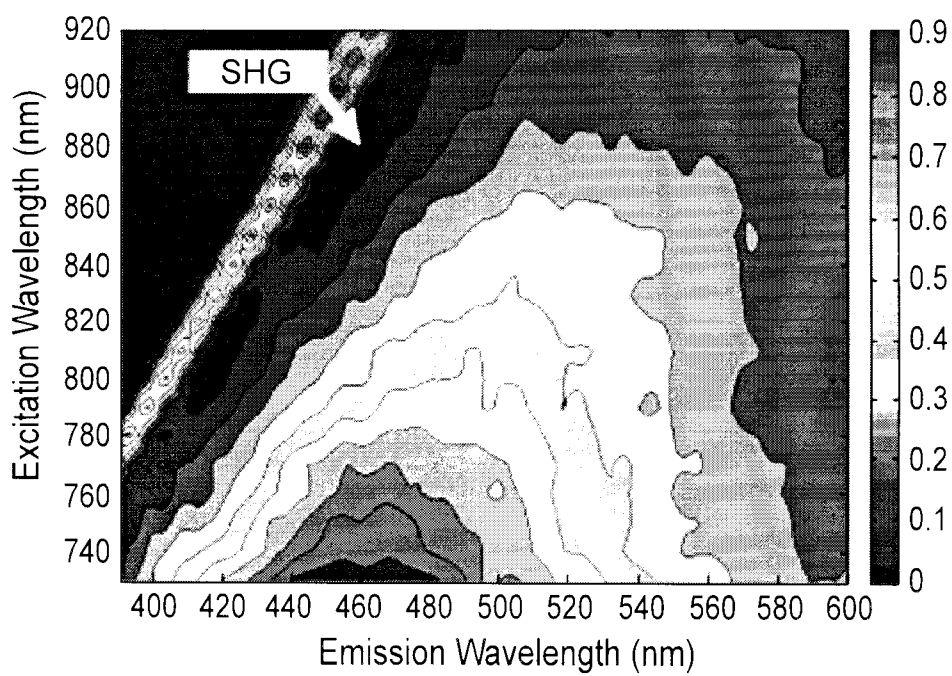


Figure 33C

34/39

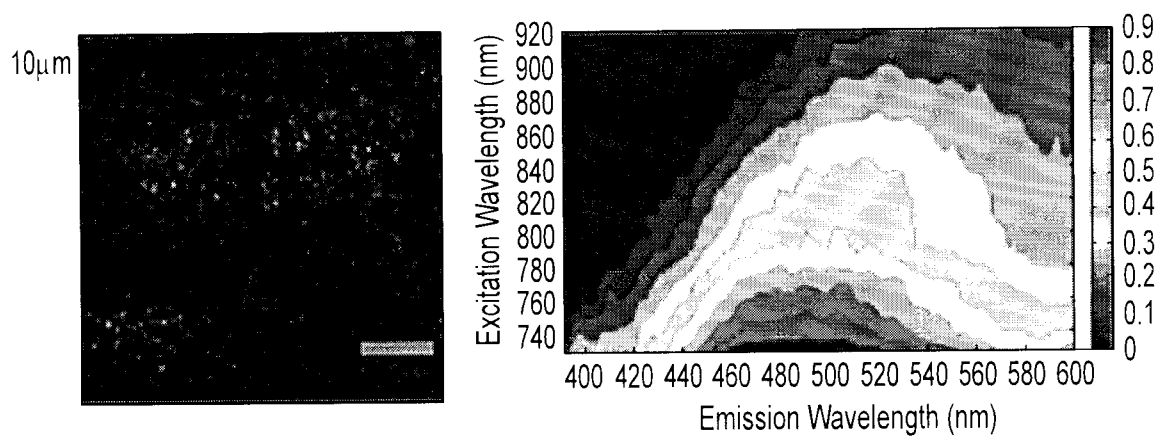


Figure 34A

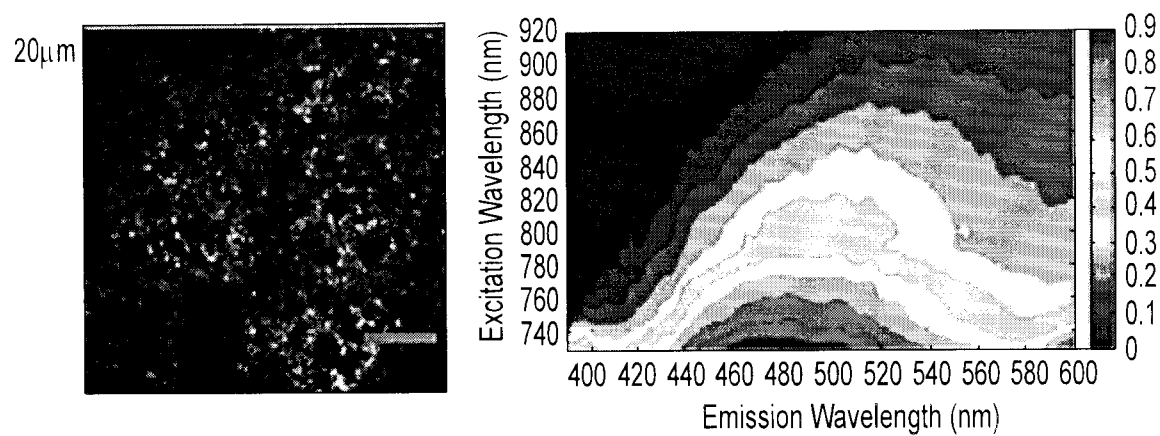


Figure 34B

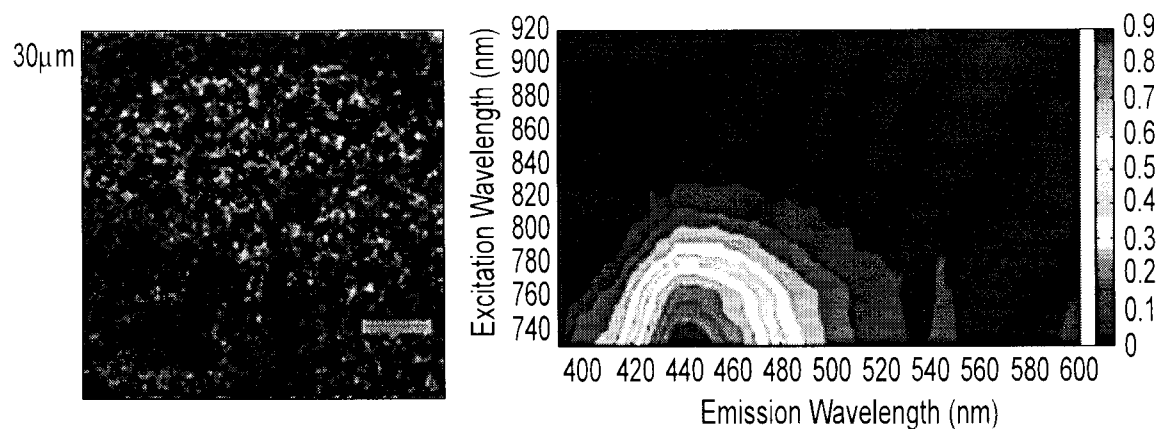


Figure 34C

35/39

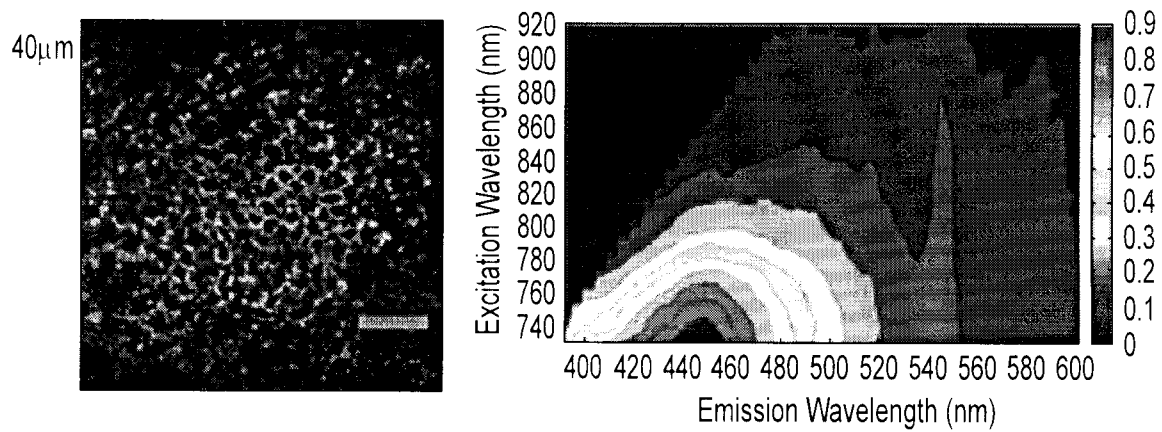


Figure 34D

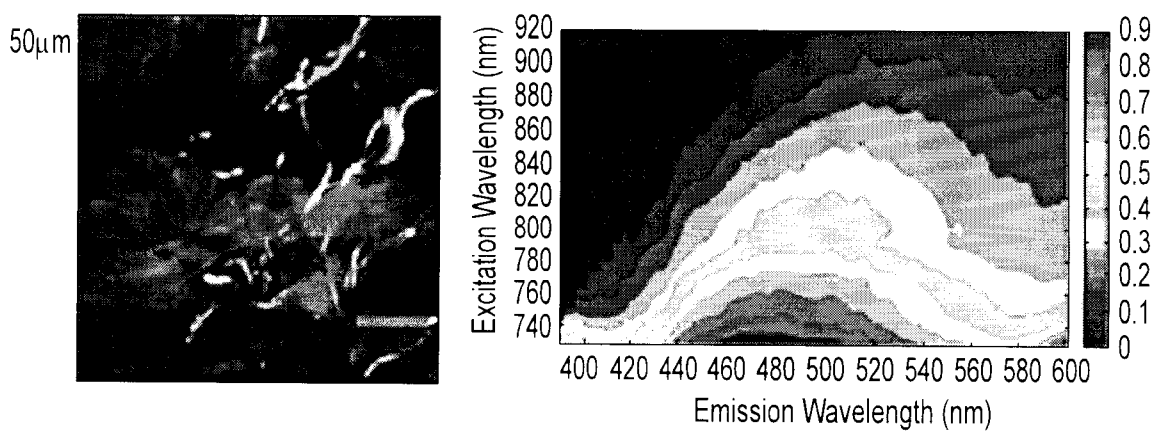


Figure 34E

36/39

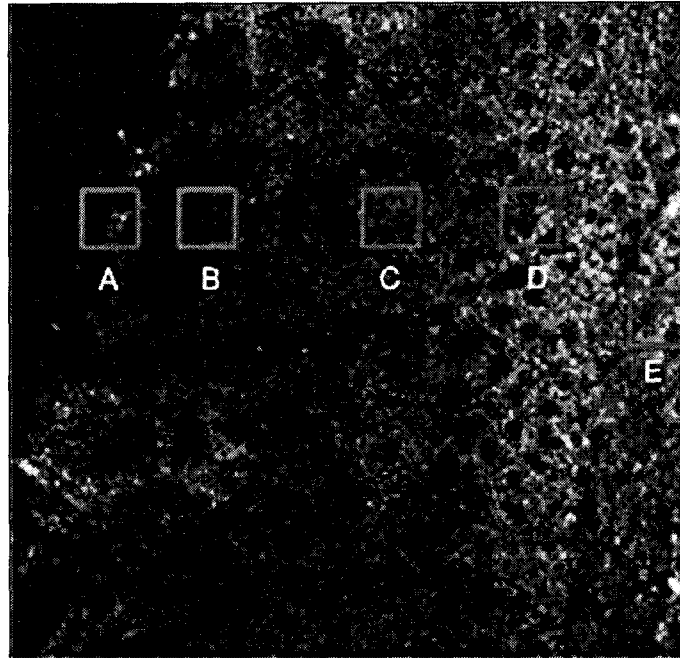


Figure 35A

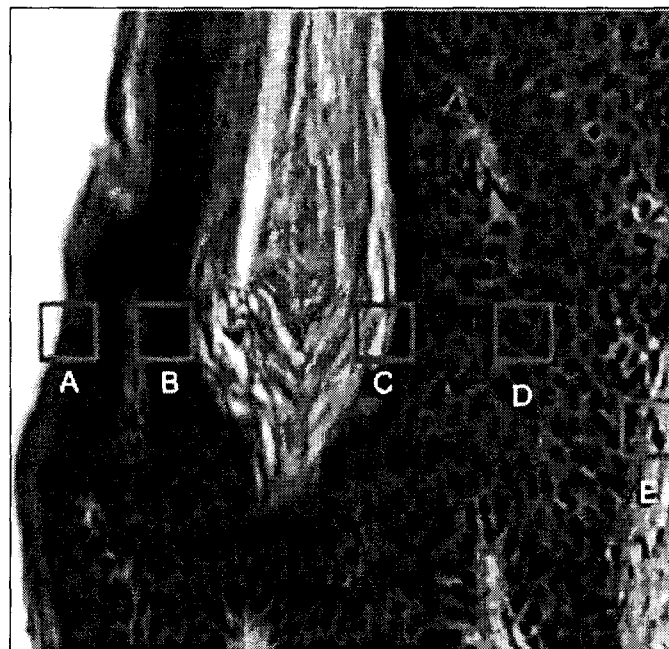


Figure 35B

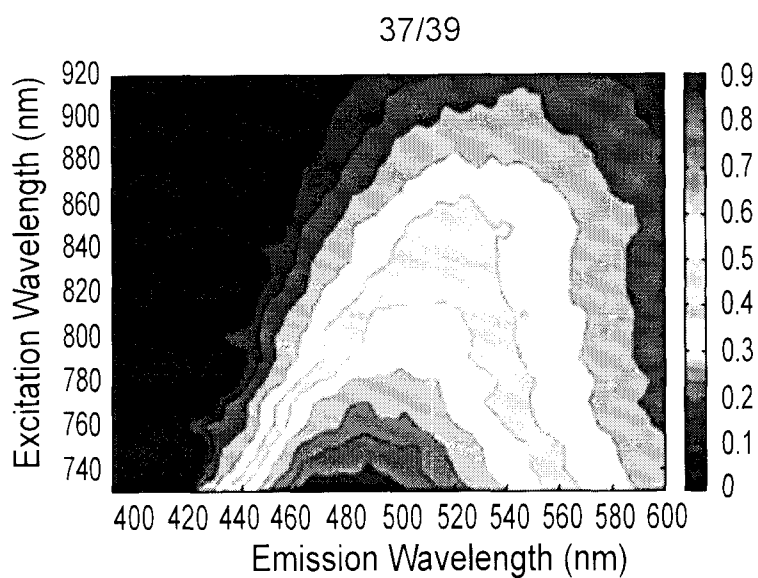


Figure 36A

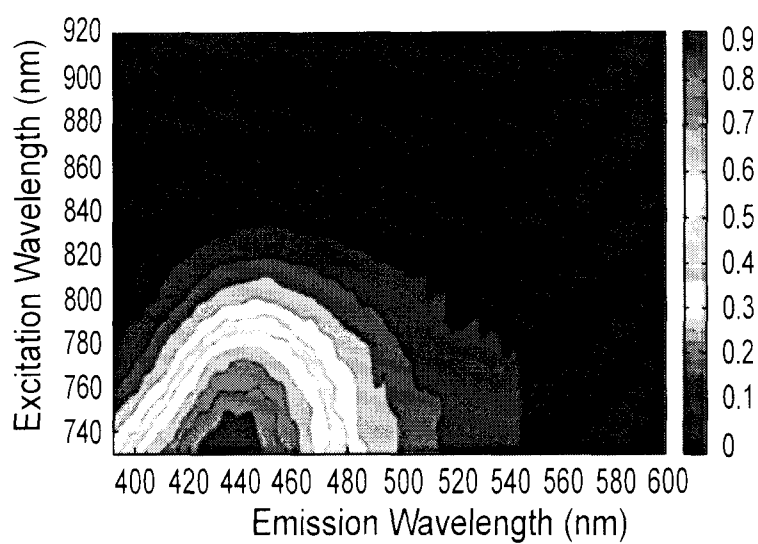


Figure 36B

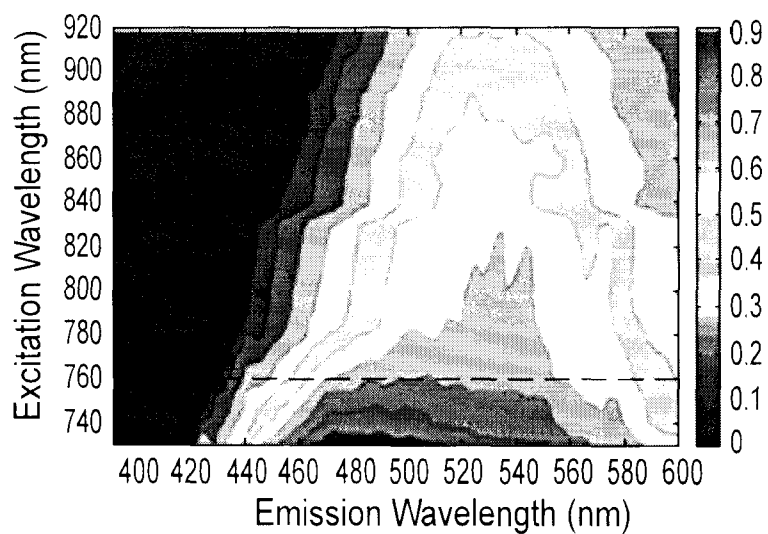


Figure 36C

38/39

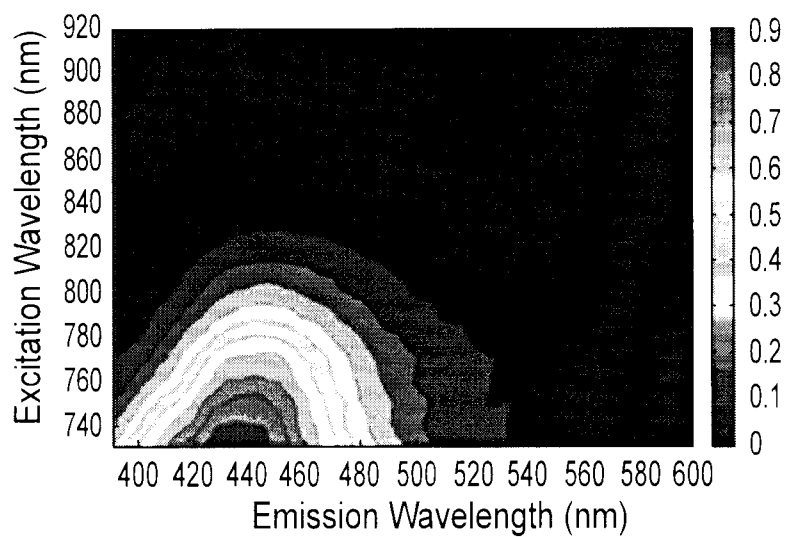


Figure 36D

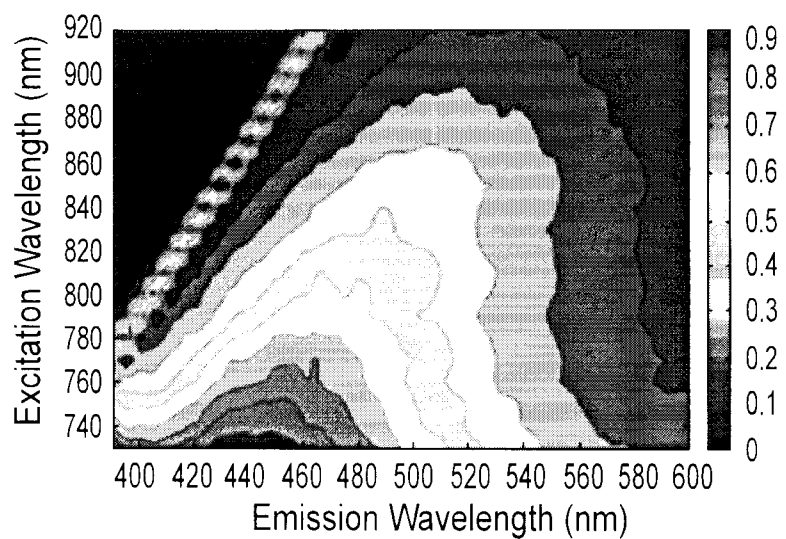


Figure 36E

39/39

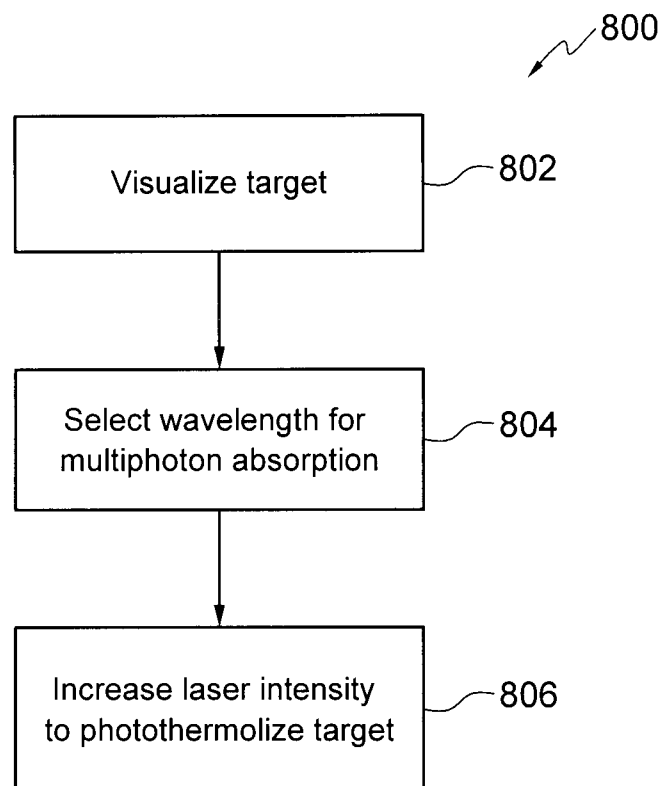


Figure 37

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA2012/050223

A. CLASSIFICATION OF SUBJECT MATTER IPC: <i>G01J 3/443</i> (2006.01) , <i>A61B 5/103</i> (2006.01) , <i>A61N 5/06</i> (2006.01) , <i>G02B 21/06</i> (2006.01) , <i>G01J 3/10</i> (2006.01) According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) IPC: <i>G01J 3/443</i> (2006.01) , <i>A61B 5/103</i> (2006.01) , <i>A61N 5/06</i> (2006.01) , <i>G02B 21/06</i> (2006.01) , <i>G01J 3/10</i> (2006.01) in combination with key words Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used) Canadian Patent Database, Google Scholar, Epoque, USPTO West. Key words: microscope, multiphoton, scanner, single objective, detector		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2005/0259249 (DOMBECK ET AL) 24 November 2005 (24-11-2005) *paragraph [0022] and Fig. 1	1-38
A	US 2003/0148393 (WOODBURY ET AL) 07 August 2003 (07-08-2003) *Abstract, Fig. 2 and corresponding description	1-38
A	US 2010/0284024 (VUCINIC ET AL) 11 November 2010 (11-11-2010) *Fig. 6, paragraphs [0041]-[0042]	1-38
A	US 2010/0259605 (SO ET AL) 14 October 2010 (14-10-2010) *Abstract, Fig. 2A and corresponding description	1-38
☐ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents :	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family	
"A" document defining the general state of the art which is not considered to be of particular relevance		
"E" earlier application or patent but published on or after the international filing date		
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)		
"O" document referring to an oral disclosure, use, exhibition or other means		
"P" document published prior to the international filing date but later than the priority date claimed		
Date of the actual completion of the international search 15 June 2012 (15-06-2012)	Date of mailing of the international search report 27 June 2012 (27-06-2012)	
Name and mailing address of the ISA/CA Canadian Intellectual Property Office Place du Portage I, C114 - 1st Floor, Box PCT 50 Victoria Street Gatineau, Quebec K1A 0C9 Facsimile No.: 001-819-953-2476	Authorized officer Humberto Castaneda (819) 994-7473	

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/CA2012/050223

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
US2005259249A1	24 November 2005 (24-11-2005)	US2005259249A1 WO2005072386A2 WO2005072386A3	24 November 2005 (24-11-2005) 11 August 2005 (11-08-2005) 19 October 2006 (19-10-2006)
US2003148393A1	07 August 2003 (07-08-2003)	US2003148393A1 US7193706B2 US2007196815A1 WO0219594A2 WO0219594A3 WO2008115948A2 WO2008115948A3	07 August 2003 (07-08-2003) 20 March 2007 (20-03-2007) 23 August 2007 (23-08-2007) 07 March 2002 (07-03-2002) 27 December 2002 (27-12-2002) 25 September 2008 (25-09-2008) 11 December 2008 (11-12-2008)
US2010284024A1	11 November 2010 (11-11-2010)	US2010284024A1 WO2009091902A1	11 November 2010 (11-11-2010) 23 July 2009 (23-07-2009)
US2010259605A1	14 October 2010 (14-10-2010)	US2005036667A1 US7372985B2 US2009072171A1 US7724937B2	17 February 2005 (17-02-2005) 13 May 2008 (13-05-2008) 19 March 2009 (19-03-2009) 25 May 2010 (25-05-2010)