HU000030524T2

(19) **HU**

(11) Lajstromszám: **E 030 524**

(13) **T2**

MAGYARORSZÁG
Szellemi Tulajdon Nemzeti Hivatala

EURÓPAI SZABADALOM
SZÖVEGÉNEK FORDÍTÁSA

(21) Magyar ügyszám: **E 12 721745**
(22) A bejelentés napja: **2012. 04. 12.**

(51) Int. Cl.: ***A61G 70/18*** *(2006.01)*
A61B 5/11 *(2006.01)*

(96) Az európai bejelentés bejelentési száma:
EP 20120721745
(97) Az európai bejelentés közzétételi adatai:
EP 2696834 A1 **2012. 10. 18.**
(97) Az európai szabadalom megadásának meghirdetési adatai:
EP 2696834 B1 **2016. 06. 01.**

(86) A nemzetközi (PCT) bejelentési szám:
PCT/DK 12/000039
(87) A nemzetközi közzétételi szám:
WO 12139577

(30) Elsőbbségi adatok:
201100287 **2011. 04. 12.** **DK**

(72) Feltaláló(k):
WESTERMANN, Karsten, 6400 Sonderborg (DK)

(73) Jogosult(ak):
Linak A/S, 6430 Nordborg (DK)

(74) Képviselő:
Danubia Szabadalmi és Jogi Iroda Kft., Budapest

(54) **Villamos működtetőszerkezet-rendszer**

Az európai szabadalom ellen, megadásának az Európai Szabadalmi Közlönyben való meghirdetésétől számított kilenc hónapon belül, felszólalást lehet benyújtani az Európai Szabadalmi Hivatalnál. (Európai Szabadalmi Egyezmény 99. cikk(1))

A fordítást a szabadalmas az 1995. évi XXXIII. törvény 84/H. §-a szerint nyújtotta be. A fordítás tartalmi helyességét a Szellemi Tulajdon Nemzeti Hivatala nem vizsgálta.

(19) Europäisches Patentamt
European Patent Office
Office européen des brevets

(11) EP 2 696 834 B1

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
01.06.2016 Bulletin 2016/22

(21) Application number: **12721745.3**

(22) Date of filing: **12.04.2012**

(51) Int Cl.:
A61G 7/018 *(2006.01)* ***A61B 5/11*** *(2006.01)*

(86) International application number:
PCT/DK2012/000039

(87) International publication number:
WO 2012/139577 (18.10.2012 Gazette 2012/42)

(54) **ELECTRIC ACTUATOR SYSTEM**

ELEKTRISCHES STELLGLIEDSYSTEM

SYSTÈME D'ACTIONNEUR ÉLECTRIQUE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(30) Priority: **12.04.2011 DK 201100287**

(43) Date of publication of application:
19.02.2014 Bulletin 2014/08

(73) Proprietor: **Linak A/S**
6430 Nordborg (DK)

(72) Inventor: **WESTERMANN, Karsten**
6400 Sønderborg (DK)

(74) Representative: **Pedersen, Soeren Skovgaard**
Linak A/S
Patent Department
P.O. Box 238
9100 Aalborg (DK)

(56) References cited:
EP-A1- 2 184 512
EP-A1- 2 260 755
EP-A2- 1 955 612
WO-A1-2009/021513
US-A1- 2007 296 600

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 696 834 B1

Printed by Jouve, 75001 PARIS (FR)

Description

[0001] The invention relates to an electric actuator system for hospital and care beds as stated in the preamble of claim 1.

[0002] The actuator system is according to the invention of the type which can be used for adjusting a hospital or care bed. In this type of bed the mattress is carried by a support surface having an adjustable backrest and legrest section, said support surface being mounted in a bed frame which may be raised and lowered by means of linear actuators in the actuator system. Further, the backrest and legrest sections of the bed may be adjusted by means of linear actuators. Normally, a type of linear actuator comprising a thrust rod, e.g. of the type described in WO 02/29284 A1 Linak A/S is used. This type of linear actuator (see also Figs. 5 and 6) comprises a spindle with a spindle nut. The spindle is driven by a reversible electric motor through a transmission. When the spindle is driven, the spindle nut is moved in an inwards or outwards direction depending on the direction of rotation of the electric motor. The linear actuator is a separate product with the spindle, transmission and electric motor enclosed in a housing. The housing typically consists of a motor housing and an outer tube. An inner tube is secured to the spindle nut. The inner tube is displaced in and out of the outer tube as the spindle nut is moved in and out on the spindle. In the opposite end of the spindle nut the inner tube comprises a front mounting. The outer side of the motor housing is furnished with a rear mounting. The front mounting and rear mounting are used to secure the linear actuator in the structure which should be adjusted.

[0003] For certain patients in the hospital and care sector it is necessary for the nursing staff to know whether the patient is in the process of leaving his bed or has left his bed. Such a bed is i.a. described in US 4,934,468 Hill Rom Co. Inc. and US 5,276,432 Stryker Corp. These hospital beds are equipped with a weighing system for weighing and/or monitoring the patient's weight. The weighing system can however also be configured to monitor the patient's position in the bed. The weighing system can further be connected to an alarm which can give off a signal in case the patient assumes a position where it is conceivable that the patient may leave the bed or has already left the bed. A bed having similar characteristics is described in EP 1 974 708 A1 Paramount. Here, changes in the patient's center of gravity are registered by a number of interconnected weight sensors located at each corner of the lying surface of the bed. By comparing the readings from each weight sensor, it can be detected whether a patient is sitting up and is thus potentially in the process of leaving the hospital bed, but naturally also whether the patient has left the bed.

[0004] Common for these types of bed structures is that they are intended for continuous weighing for accurate supervision of the patient's weight. In order to be able to do this with a sufficient accuracy high-end sensor with a high resolution are used. This fact is thus also reflected in the price of these bed structures, which are very expensive. The use of these beds is thus also limited to a select few patients requiring special treatment and special care.

[0005] For care of patients e.g. during the night it has proven expedient to provide one or more orientation lights under the bed (Under Bed Light). The orientation light is both used by the users to navigate around the room when getting out of bed in the dark and by the staff to navigate around the room without having to turn on the ceiling light and thus disturbing the other bedbound patients. As an example, US 6,234,642 B1 Dewert can be mentioned, where the orientation light of the bed is connected to the control box. Here, a sensor in the mattress of the bed can be connected to the control box such that the light in the control box is turned on when the patient sits up or has left the bed. The principle of having light under the bed where the activation thereof is linked to the user of the bed is known as far back as e.g. US 2,185,051 O.J. Daigle. This document discloses a bed which in connection with the lying surface comprises one or more switches which, if desired, can be connected in such a manner that a light source placed under the bed is turned on when the person e.g. leaves the bed.

[0006] Activation of the orientation light under the bed by means of sensors in the mattress is however undesired as they often, and especially after continuous use, can give off faulty signals or signals may fail to appear. Although the signal for activation of the light could be provided by the beds comprising weight sensors described above, this would however represent a relatively expensive solution.

[0007] In addition to the orientation light located under the bed it is known from EP 1 275 896 A1 Deapillat to integrate a light strip in the floor running from each bed in a shared bed room to a common bathroom. If a patient sits up in the bed or leaves the bed in the night this is registered by a motion sensor located next to the bed. The motion sensor, which may e.g. be an infrared sensor, gives off a signal to turn on both the light under the bed, in the light strip in the floor as well as in the bathroom. This ensures that the patient can find his way to the bathroom without disturbing the other patients in the bed room. The use of motion sensors is however undesired since the movement of other people in the room could cause unintended activation of the light. Furthermore, the integration of a light source in the floor is subject to a number of expenses. Further, the application of the room is limited as it is bound by the location of the light strip in the floor.

[0008] It is thus desired to provide an actuator system for a hospital or care bed which represents a simpler, more reliable and cheaper alternative for activating the orientation light, both in connection with the bed as well as in the proximity of the bed.

[0009] The actuator system according to the invention is characterized by being connected to one or more light

sources which can be activated if one or more changes in the force on the actuator(s) are registered. Thus, the patient's movement pattern in the bed can be used to assist the patient when navigating around the room. This can e.g. be done by turning on the light in the bathroom, such that the patient can easily find his way without disturbing the other patients. By using the actuator's means for registering changes in the force a continuous reading and thus supervision of the patient's movement pattern is achieved. As these means constitute an integral part of the actuators the price for this part of the actuator may be kept at a minimum. The connection of the actuator system to other light sources may be achieved with a cable connection and may thus be implemented without large expenses, as it would be a matter of one or more cables.

[0010] In a special embodiment the actuator system may be connected to the other light sources through a wireless connection. This would if so lower the cost of the solution and further increase the flexibility as the bed is not bound by a cable connection.

[0011] The invention further relates to a hospital or care bed comprising an electric actuator system of the type described above.

[0012] An embodiment of the actuator system according to the invention will be described more fully below with reference to the accompanying drawing, in which

Fig. 1 shows a schematic view of a hospital or care bed comprising an actuator system in a first embodiment,

Fig. 2 shows a schematic view of a hospital or care bed comprising an actuator system in a second embodiment,

Fig. 3 shows a block diagram of an actuator system comprising other light sources,

Fig. 4 shows a schematic view of a ward,

Fig. 5 shows a linear actuator, and

Fig. 6 shows the linear actuator in Fig. 5, where the motor housing and the outer tube has been partially removed.

[0013] Fig. 1 shows a hospital bed 1 comprising an under frame 3 equipped with drive wheels 2 and an upper frame 4. An adjustable support surface 5 for a mattress (not shown) is mounted to the upper frame 4. The supporting surface comprises a backrest section 6, an articulated legrest section 7 and a fixed middle section 8 there between. The backrest and legrest sections 6,7 can be adjusted with an actuator 9, 10 each such that the supporting surface may assume different contours. The upper frame 4 is connected to the under frame 2 with a linkage 11,12 at each end. The upper frame 4 may be raised and lowered by means of a pair of actuators 13,14 connected to the linkages 11,12. All the actuators 9,10,13,14 are connected to a control box 15 comprising a control. The control box can be connected to mains and may e.g. be equipped with a power supply. The control box may further comprise a rechargeable battery pack.

[0014] A junction box 16 is connected to the control box 15 for connecting one or more control units, such as a hand control 17 and a control panel 18 integrated in the head or foot board, and possibly other peripheral equipment. The overall system comprising actuators 9,10,13,14, control box 15 and control units 17,18 is known as an actuator system.

[0015] One or more of the actuators 9,10,13,14 comprise means for registering the forces, which the actuator(s) is exposed to, as a result of the weight of the person lying in the bed, and the position and position changes of the person in the bed. This type of actuator is disclosed in WO 2009/021513 A1 Linak A/S and comprises the same elements as the linear actuator described in the preamble. Furthermore, this type of actuator comprises a load cell (not shown) e.g. in the form of a strain gauge or a piezoelement. Changes in the force on the actuator 9,10,13,14 are registered by the load cell and the information concerning these changes is sent to the control box 15. A linear actuator of this type is further described in connection with figs. 5 and 6.

[0016] As orientation light under the bed the junction box 16 can be equipped with a light source 19, of the type disclosed in EP 1 955 612 A2 Linak A/S.

[0017] Fig.2 shows a schematic view of the hospital and care bed 20 in another embodiment than the bed shown in Fig. 1. Here, the under frame 3 and upper frame 4 are not connected by linkages, but are instead connected by two linear actuators designed as lifting columns 21,22. These lifting columns 21,22 may also each contain a load cell for registering the force on the lifting column 21,22.

[0018] As shown in Fig. 3 the control box 15 is further connected to other light sources 23,24 in e.g. a bathroom 25 and a ward 26, in which the bed is located. When the patient sits up in bed and thus potentially could be on his way out of bed or has already left the bed, these changes are registered in one or more of the actuators 9,10,13,14,21,22. The information concerning these changes are transmitted to the control box 15 which hereby can turn on one or more of the light sources 23,24 and/or the light source 19 under the bed. Thus, if the patient needs to go to the toilet during the night, the control box 15 may be programmed to turn on the light source 19 under the bed and the light 23 in the bathroom 25. Thus, the patient can find his way to the bathroom 25 without turning on the light 24 in the ward 26, thereby disturbing the other as little as possible.

[0019] The connection between the actuator system and the light sources may be cable connected and/or wireless. In Fig. 3 the connection between the control

box 15 and the light 23 in the ward 26 is cable connected. When the light 23 should be turned on or off, the control box 15 transmits an on signal or off signal, respectively, to a relay 27. Hereby, the relay 27 will be drawn or released, at which the light 23 can be turned on and off. The connection between the control box 15 and the light 24 in the bathroom 25 is on the contrary wireless. In order to turn on the light 24 in the bathroom 25 the control box 15 generates a signal, which through a transceiver 28 is sent to the paging system or alarm system used in the given hospital or nursing home via a transceiver 29. Subsequently, the paging system or alarm system turns the light 24 on or off. The control box 15 can thus convert the information from the load cell in the linear actuator 9,10,13,14 into a signal, adapted to the communications protocol used by the paging system or alarm system. The transceiver 28 may e.g. be incorporated in the control box 15 or in the junction box 16. In a simpler embodiment a wireless transmitter 45 is connected to the control box 15. Here the wireless transmitter 45 sends to a wireless receiver 46 located directly in connection with the light source 47. In this embodiment it is thus not necessary for the on/off signals to be transmitted to the paging system or alarm system mentioned above. Thus, a very simple but highly functional actuator system may be provided at a very low cost. It is understood that the three different types of connections between the actuator system and the light sources shown in Fig. 3 can function as alternative to each other or in interaction with each other.

[0020] As shown in figure 3 the actuator system may also comprise lifting columns 21,22, as shown in figure 2. For the sake of clarity the connection between the lifting columns 21,22 and the control box 15 is shown as dotted lines.

[0021] Figure 4 shows a schematic view of a patient ward, comprising a ward 26 and a bathroom 25. From the ward 26 there is access to the bathroom 25 through the door 26a. The ward 26 contains a hospital or care bed 1,20 of the type described above. The actuator system in the bed 1,20 is connected to the light sources 23,24 in the ward 26 and the bathroom 25, respectively. The actuator system and the connected light sources 23,24 function as described under Figs. 1,2 and 3. Thus, the connected light sources 23,24 constitute a part of the actuator system.

[0022] Fig. 5 shows a linear actuator 30 of the type described in the preamble comprising a thrust rod and is thus of the same type as the linear actuators 9,10,13,14. The thrust rod is also known as an inner tube 31. The linear actuator comprises an outer tube 32 and a motor housing 33. The linear actuator 30 further comprises a front mounting 34 at the outer end of the inner tube 31 and a rear mounting 35 at the motor housing 33.

[0023] Figure 6 shows the linear actuator in Fig. 5, where the motor housing 33 and the outer tube 32 have been partially removed. The main components of the linear 30 are a spindle 36, on which a spindle nut 37 is arranged. The spindle nut 37 may be secured against rotation. The inner tube 31 is secured to the spindle nut 37 and may thus be moved inwards or outwards on the outer tube depending on the direction of rotation of the spindle 36. The spindle 36 is driven by a reversible electric motor 38 through a transmission. The transmission here comprises a worm 39 located in extension of the drive shaft 39 of the electric motor, and a worm wheel 40 secured to the spindle 36. Moreover, a bearing 41 is secured to the spindle 36. The bearing 41 may e.g. be a ball bearing or a roller bearing. The linear actuator 30 comprises a load cell 42 for registering the force, which the linear actuator 30 is exposed to and the relative changes to this force. In fig. 6 the load cell 42 is located in connection with the rear part of the spindle 36. The load cell may also be arranged in connection with the inner tube or the rear mounting as indicated with reference numerals 43 and 44. The load cell 42,43,44 may e. g. be a strain gauge or a piezo element. The linear actuator 30 is connected to a control box 15 of the type described in connection with figures 1-4. The information concerning the force on the linear actuator 30 or a change will thus be transmitted to the control box 15. The linear actuator 30 is, as stated above, disclosed in WO 2009/021513 A1 Linak A/S.

[0024] The linear actuator 30 shown in Figs. 5 and 6 only discloses the main components. Thus, the linear actuator 30 may be equipped with e.g. a brake mechanism, additional bearings, release mechanism, etc.

[0025] It is noted that the invention further may be used in connection with so-called dual actuators comprising two spindle units and a control box in one common housing. This type is further described in WO 2007/093181 A1 Linak A/S.

Claims

1. Electric actuator system for hospital and care beds (1,20) comprising at least one linear actuator (9,10,13,14,21,22) for adjusting the bed (1,20), a control box (15) and at least one control unit (17,18), where the linear actuator (9,10,13,14,21,22) and the control unit are connected to the control box (15) and where the linear actuator (9,10,13,14,21,22) comprises means for registering the force on the linear actuator (9,10,13,14,21,22) and relative changes therein, **characterized in that** the actuator system is connected to one or more light sources (19,23,24), which may be activated if one or more changes in the force on the linear actuator (9,10,13,14,21,22) is registered.

2. Electric actuator system for hospital and care beds according to claim 1, **characterized in that** the actuator system is connected to one or more light sources (19,23,24) through a wireless connection.

3. Electric actuator system for hospital and care beds

according to claim 1-2, **characterized in that** it comprises a light source (19,23,24) located on the bed (1,20).

4. Electric actuator system for hospital and care beds according to one or more of the claims 1-3, **charact erized** in that the control box (15) comprises at least a part of the control for the actuator system.

5. Electric actuator system for hospital and care beds according to one or more of the claims 1-4, c h a r a c t e r i z e d in that the control box (15) comprises a mains based power supply.

6. Electric actuator system for hospital and care beds according to one or more of the claims 1-5, **charact erized** in that the control box (15) comprises a rechargeable battery pack.

7. Electric actuator system for hospital and care beds according to one or more of the claims 1-6, **charact erized** in that the means for registering the force on the linear actuator (9,10,13,14,21,22) is a load cell.

8. Electric actuator system for hospital and care beds according to one or more of the claims 1-7, **charact erized** in that it further comprises a junction box 16.

9. Electric actuator system for hospital and care beds according to claim 8, **characterized in that** the junction box comprises a light source (19).

10. Hospital or care bed comprising an electric actuator system according to one or more of the claims 1-9.

Patentansprüche

1. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten (1, 20), umfassend mindestens ein lineares Stellglied (9, 10, 13, 14, 21, 22) zum Ein- bzw. Verstellen des Bettes (1, 20), einen Steuerkasten (15) und mindestens eine Steuereinheit (17, 18), wobei das lineare Stellglied (9, 10, 13, 14, 21, 22) und die Steuereinheit mit dem Steuerkasten (15) verbunden sind und wobei das lineare Stellglied (9, 10, 13, 14, 21, 22) Mittel zum Registrieren der Kraft an dem linearen Stellglied (9, 10, 13, 14, 21, 22) und der relativen Änderungen darin umfasst, **dadurch gekennzeichnet, dass** das Stellgliedsystem mit einer oder mehreren Lichtquellen (19, 23, 24) verbunden ist, die zu aktivieren ist/sind, wenn eine oder mehrere Änderungen in der Kraft an dem linearen Stellglied (9, 10, 13, 14, 21, 22) registriert wird/werden.

2. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach Anspruch 1,**dadurch gekennzeichnet, dass** das Stellgliedsystem mit einer oder mehreren Lichtquellen (19, 23, 24) durch eine drahtlose Verbindung verbunden ist.

3. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach Anspruch 1 bis 2, **dadurch gekennzeichnet, dass** es eine Lichtquelle (19, 23, 24) umfasst, die an dem Bett (1, 20) angeordnet ist.

4. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach einem oder mehreren der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass** der Steuerkasten (15) mindestens einen Teil der Steuerung für das Stellgliedsystem umfasst.

5. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach einem oder mehreren der Ansprüche 1 bis 4, **dadurch gekennzeichnet, dass** der Steuerkasten (15) eine auf dem Hauptnetz beruhende Energieversorgung umfasst.

6. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach einem oder mehreren der Ansprüche 1 bis 5, **dadurch gekennzeichnet, dass** der Steuerkasten (15) einen wiederaufzuladenden Akkumulator umfasst.

7. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach einem oder mehreren der Ansprüche 1 bis 6, **dadurch gekennzeichnet, dass** das Mittel zum Registrieren der Kraft an dem linearen Stellglied (9, 10, 13, 14, 21, 22) eine Einrichtung zur Kraftaufnahme oder eine Kraftmesszelle ist.

8. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach einem oder mehreren der Ansprüche 1 bis 7, **dadurch gekennzeichnet, dass** es weiterhin einen Anschluss-, Abzweig- und / oder Verteilerkasten (16) umfasst.

9. Elektrisches Stellgliedsystem für Krankenhaus- und Pflegebetten nach Anspruch 8, **dadurch gekennzeichnet, dass** der Anschluss-, Abzweig- und / oder Verteilerkasten eine Lichtquelle (19) umfasst.

10. Krankenhaus- oder Pflegebett, umfassend ein elektrisches Stellgliedsystem nach einem oder mehreren der Ansprüche 1 bis 9.

Revendications

1. Système d'actionneur électrique pour des lits d'hôpital et de soins (1, 20) comprenant au moins un actionneur linéaire (9, 10, 13, 14, 21, 22) pour régler le lit (1, 20), une boîte de commande (15) et au moins une unité de commande (17, 18), l'actionneur linéaire (9, 10, 13, 14, 21, 22), et l'unité de commande

étant connectés à la boîte de commande (15) et l'actionneur linéaire (9, 10, 13, 14, 21, 22) comprenant un moyen d'enregistrement de la force sur l'actionneur linéaire (9, 10, 13, 14, 21, 22) et des changements relatifs dans celui-ci,
caractérisé en ce que le système d'actionneur est connecté à une ou plusieurs sources de lumière (19, 23, 24), qui peuvent être activées si un ou plusieurs changements de la force sur l'actionneur linéaire (9, 10, 13, 14, 21, 22) sont enregistrés.

2. Système d'actionneur électrique pour des lits d'hôpital et de soins selon la revendication 1, **caractérisé en ce que** le système d'actionneur est connecté à une ou plusieurs sources de lumière (19, 23, 24) via une connexion sans fil.

3. Système d'actionneur électrique pour des lits d'hôpital et de soins selon les revendications 1 et 2, **caractérisé en ce qu'**il comprend une source de lumière (19, 23, 24) située sur le lit (1, 20).

4. Système d'actionneur électrique pour des lits d'hôpital et de soins selon une ou plusieurs des revendications 1 à 3, **caractérisé en ce que** la boîte de commande (15) comprend au moins une partie de la commande pour le système d'actionneur.

5. Système d'actionneur électrique pour des lits d'hôpital et de soins selon une ou plusieurs des revendications 1 à 4, **caractérisé en ce que** la boîte de commande (15) comprend une alimentation électrique sur secteur.

6. Système d'actionneur électrique pour des lits d'hôpital et de soins selon une ou plusieurs des revendications 1 à 5, **caractérisé en ce que** la boîte de commande (15) comprend un bloc-batterie rechargeable.

7. Système d'actionneur électrique pour des lits d'hôpital et de soins selon une ou plusieurs des revendications 1 à 6, **caractérisé en ce que** le moyen d'enregistrement de la force sur l'actionneur linéaire (9, 10, 13, 14, 21, 22) est une cellule de charge.

8. Système d'actionneur électrique pour des lits d'hôpital et de soins selon une ou plusieurs des revendications 1 à 7, **caractérisé en ce qu'**il comprend en outre une boîte de jonction (16).

9. Système d'actionneur électrique pour des lits d'hôpital et de soins selon la revendication 8, **caractérisé en ce que** la boîte de jonction comprend une source de lumière (19).

10. Lit d'hôpital ou de soins comprenant un système d'actionneur électrique selon une ou plusieurs des revendications 1 à 9.

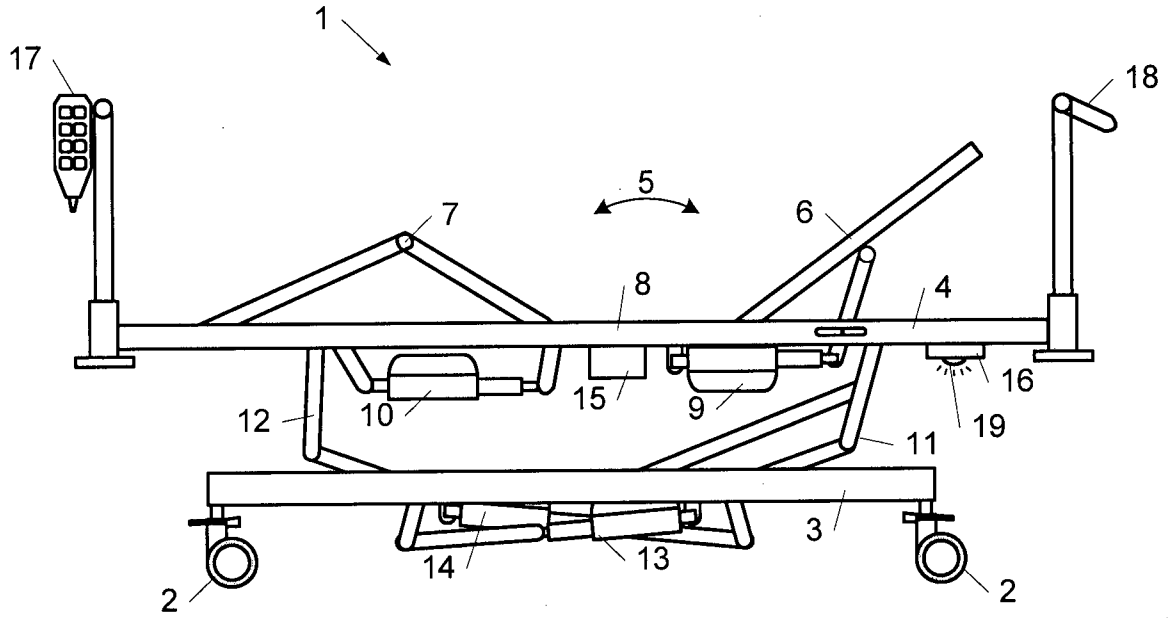

1
17
18
5
7
6
8
4
16
12
10
15
9
19
11
3
14
13
2
2

Fig. 1

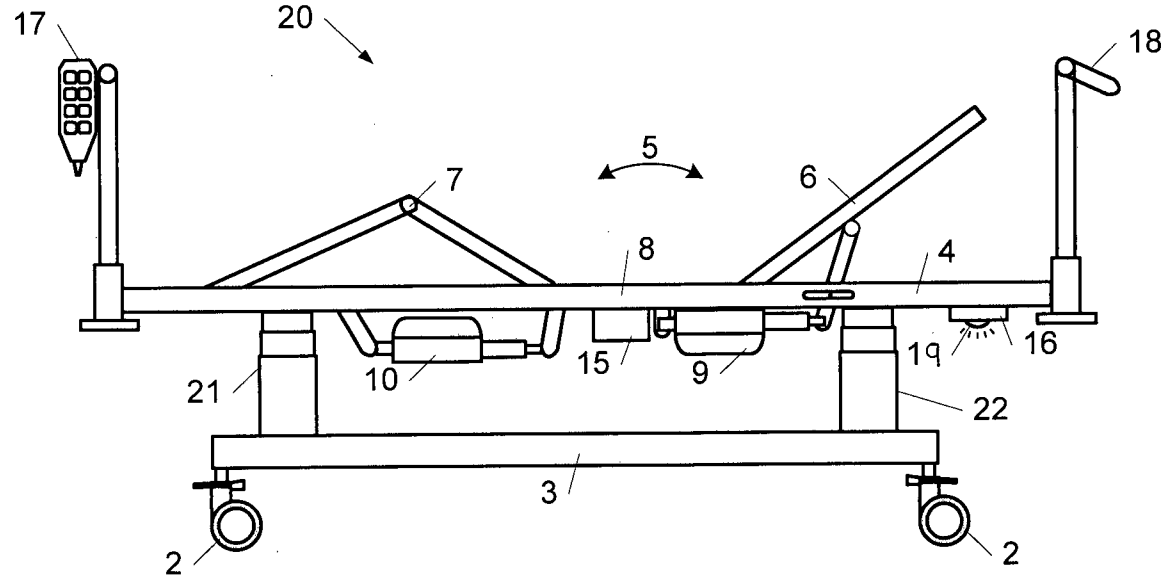

17
20
18
5
7
6
8
4
16
21
10
15
9
19
22
3
2
2

Fig. 2

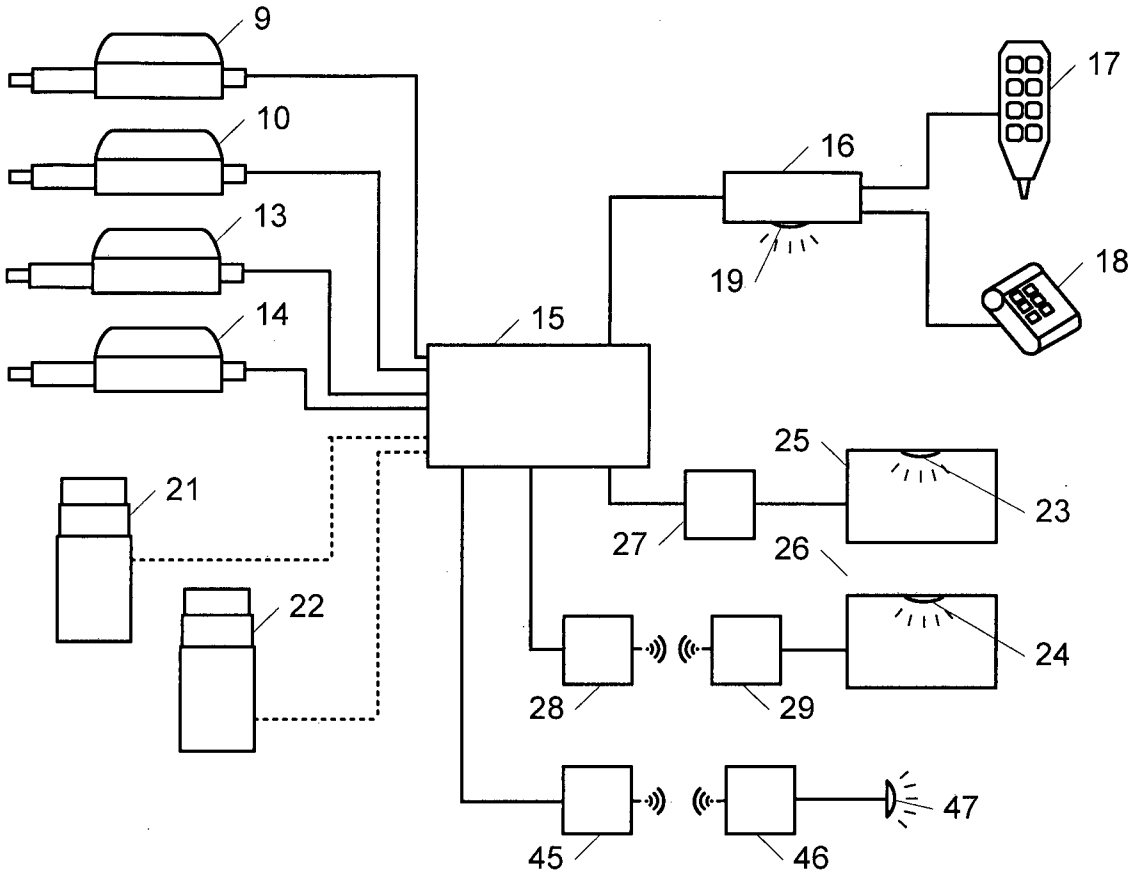

9
10
13
14
15
16
17
18
19
21
22
23
24
25
26
27
28
29
45
46
47

Fig. 3

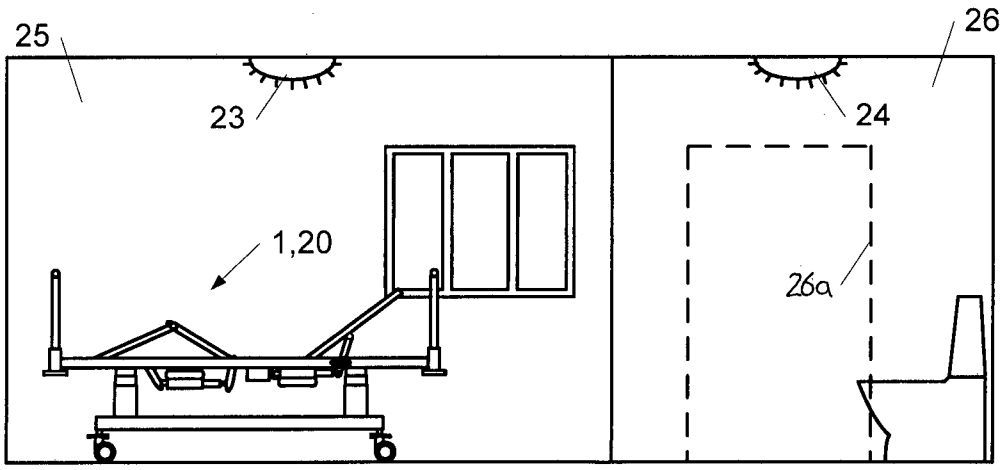

25
23
26
24
1,20
26a

Fig. 4

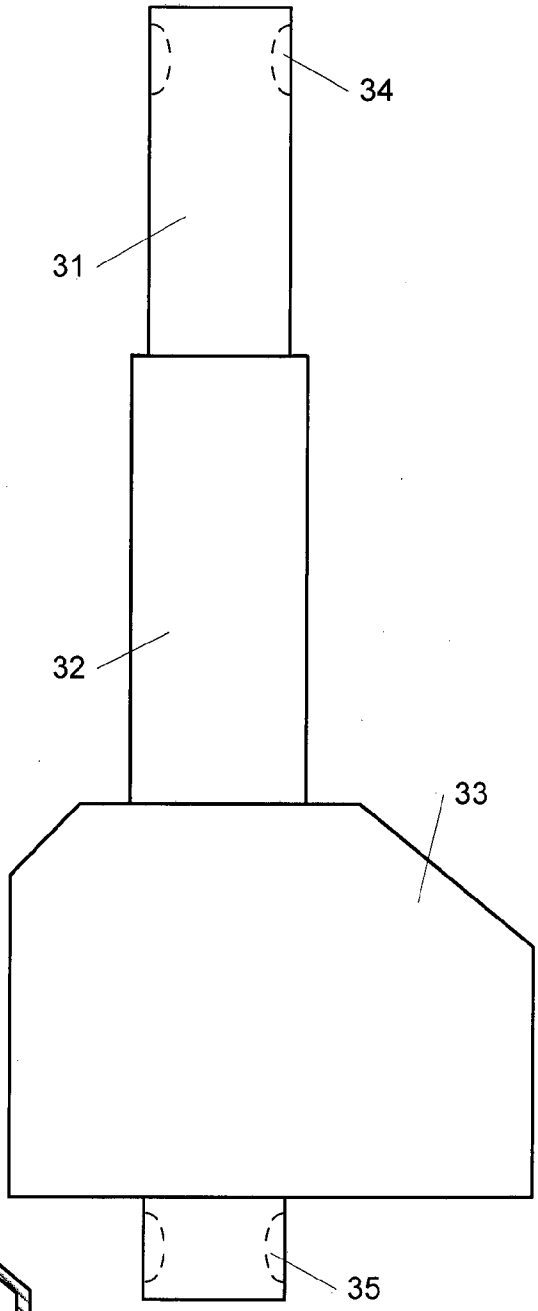


Fig. 5

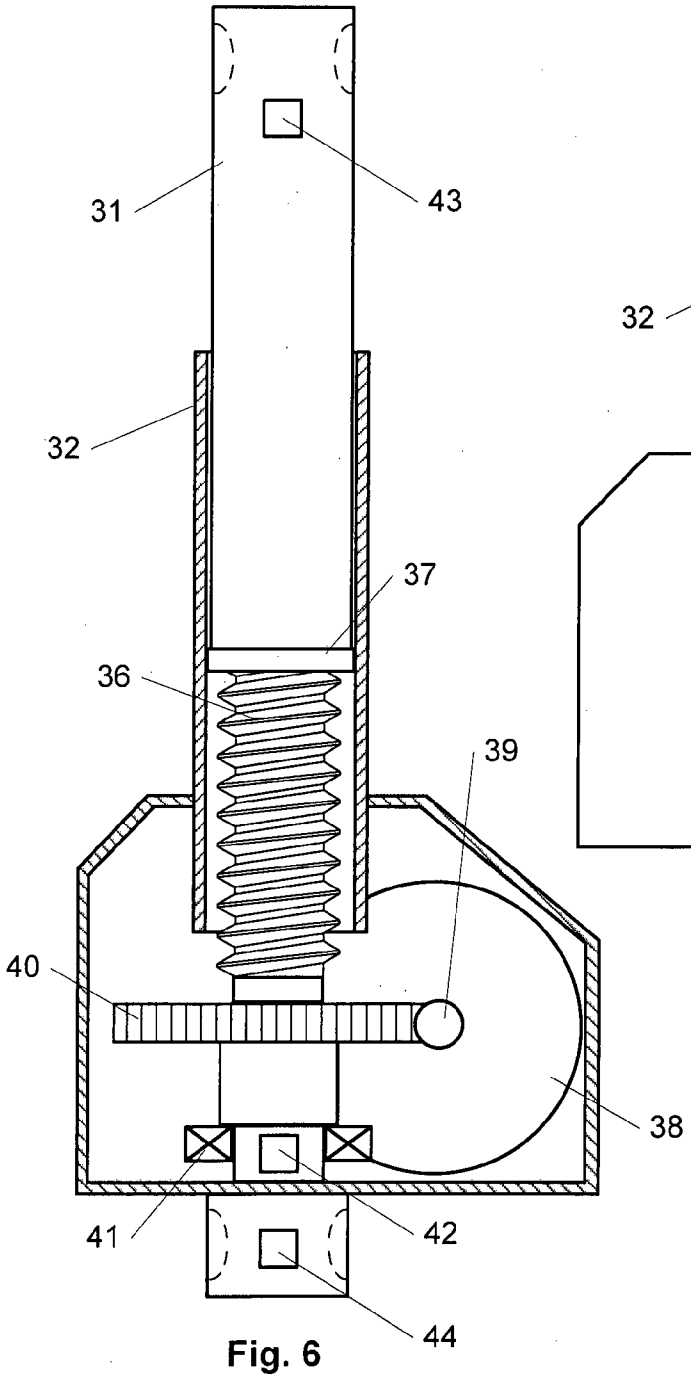


Fig. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 0229284 A1 **[0002]**
- US 4934468 A **[0003]**
- US 5276432 A **[0003]**
- EP 1974708 A1 **[0003]**
- US 6234642 B1, Dewert **[0005]**
- US 2185051 A, O.J. Daigle **[0005]**
- EP 1275896 A1 **[0007]**
- WO 2009021513 A1 **[0015] [0023]**
- EP 1955612 A2 **[0016]**
- WO 2007093181 A1 **[0025]**

119148-14568 SZT

VILLAMOS MŰKÖDTETŐSZERKEZET-RENDSZER

Szabadalmi igénypontok

1. Villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, amely az ágy (1, 20) beállításához legalább egy lineáris működtetőszerkezetet, vezérlődobozt (15) és legalább egy vezérlőegységet (17, 18) tartalmaz, ahol a lineáris működtetőszerkezet (9, 10, 13, 14, 21, 22) és a vezérlőegység a vezérlődobozzal (15) van csatlakoztatva, továbbá a lineáris működtetőszerkezetnek (9, 10, 13, 14, 21, 22) a lineáris működtetőszerkezetre (9, 10, 13, 14, 21, 22) ható erőt és annak relatív változásait regisztráló eszköze van, **azzal jellemezve**, hogy a működtetőszerkezet-rendszer egy vagy több fényforrással (19, 23, 24) van csatlakoztatva, melyek a lineáris működtetőszerkezetre (9, 10, 13, 14, 21, 22) ható erő egy vagy több változása regisztrálásakor aktiválhatók.

2. Az 1. igénypont szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a működtetőszerkezet-rendszer egy vagy több fényforrással (19, 23, 24) vezeték nélküli kapcsolat útján van csatlakoztatva.

3. Az 1. vagy a 2. igénypont szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy ágyon (1, 20) elhelyezett fényforrást (19, 23, 24) tartalmaz.

4. Az 1-3. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a vezérlődoboz (15) a működtetőszerkezet-rendszer vezérlése legalább egy részét tartalmazza.

5. Az 1-4. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a vezérlődoboz (15) hálózatról üzemelő tápegységet tartalmaz.

6. Az 1-5. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a vezérlődoboz (15) újratölthető telepcsomagot tartalmaz.

7. Az 1-6. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a lineáris működtetőszerkezetre (9, 10, 13, 14, 21, 22) ható erőt regisztráló eszközt erőmérő cella képezi.

8. Az 1-7. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy csatlakozódobozt (16) is tartalmaz.

9. A 8. igénypont szerinti villamos működtetőszerkezet-rendszer kórházi és ápolási ágyakhoz, **azzal jellemezve**, hogy a csatlakozódoboz fényforrást (19) tartalmaz.

10. Kórházi vagy ápolási ágy, amely egy az 1-9. igénypontok bármelyike szerinti villamos működtetőszerkezet-rendszert tartalmaz.