



(51) International Patent Classification:

G01N 27/27 (2006.01) G01N 33/487 (2006.01)
A61B 5/00 (2006.01)

(21) International Application Number:

PCT/US2017/033789

(22) International Filing Date:

22 May 2017 (22.05.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/339,924 22 May 2016 (22.05.2016) US

(71) Applicant: CORNELL UNIVERSITY [US/US]; Center
for Technology Licensing, 395 Pine Tree Road, Suite 310,
Ithaca, New York 14850 (US).

(72) Inventors: CRAIGHEAD, Harold G.; 21 Fairway Drive,
Ithaca, New York 14850 (US). REINHOLT, Sarah J.; 100
Graham Road, Apt. 13A, Ithaca, New York 14850 (US).

(74) Agent: GONSALVES, Andrew K.; FisherBroyles, LLP,
510 Clinton Square, Rochester, New York 14604 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR,
KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR,
TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) Title: MULTIFUNCTIONAL MICROFLUIDIC DEVICE FOR CAPTURING TARGET CELLS AND ANALYZING
GENOMIC DNA ISOLATED FROM THE TARGET CELLS WHILE UNDER FLOW CONDITIONS

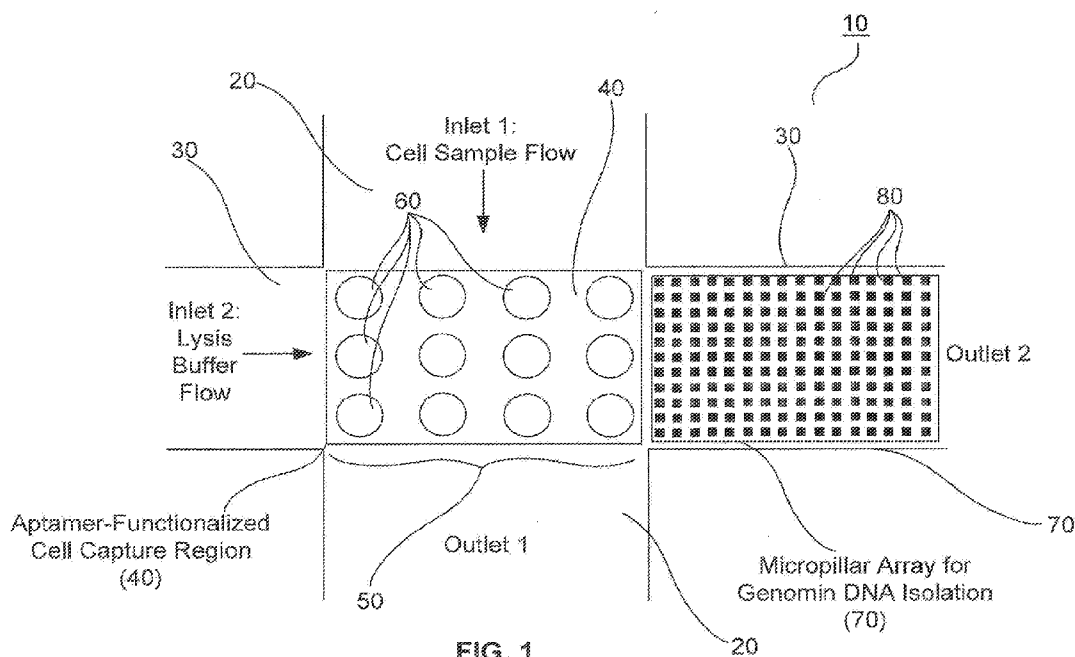


FIG. 1

(57) Abstract: The present invention relates to, *inter alia*, a microfluidic device for capturing target cells and analyzing genomic DNA isolated from the target cells while under flow conditions. The microfluidic device includes a cell microchannel and a nucleic acid microchannel that intersect in an orthogonal manner, thereby forming a cell capture intersection region. The microfluidic device also includes a cell capture array and a nucleic acid entanglement array. The cell capture array includes a plurality of cell capturing micropillars and is located in the cell capture intersection region. The nucleic acid entanglement array includes a plurality of nucleic acid entanglement micropillars that function to physically entangle and maintain thereon genomic DNA isolated from the one or more target cell, and is located in a portion of the nucleic acid microchannel that is adjacent to and downstream of the cell capture intersection region. Methods of using the microfluidic device are also disclosed.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

**MULTIFUNCTIONAL MICROFLUIDIC DEVICE FOR CAPTURING TARGET
CELLS AND ANALYZING GENOMIC DNA ISOLATED FROM THE TARGET
CELLS WHILE UNDER FLOW CONDITIONS**

5 **CROSS-REFERENCE TO RELATED APPLICATIONS**

[0001] This application claims priority benefit of U.S. Provisional Patent Application Serial No. 62/339,924, filed May 22, 2016, the disclosure of which is hereby incorporated by reference herein in its entirety.

10 **GOVERNMENT RIGHTS STATEMENT**

[0002] This invention was made with Government support under grant number DA030329 awarded by the National Institutes of Health. The United States Government has certain rights in the invention.

15 **FIELD OF THE INVENTION**

[0003] The present invention relates to, *inter alia*, a microfluidic device for capturing target cells and analyzing genomic DNA isolated from the target cells while under flow conditions.

20 **BACKGROUND OF THE INVENTION**

[0004] Cancer cells contain genetic mutations that allow them to escape the regulatory processes necessary for the healthy function of tissues and organs.¹⁻³ Moreover, there are numerous mechanisms for malignancy with different combinations of genetic mutations, and cancer cells are constantly evolving,⁴ which makes cancer treatment difficult with varying levels of efficacy. Many assays have been developed that detect specific mutations, whereas some have been designed to detect all mutations via sequencing.⁵⁻¹⁰ Each of these approaches has advantages and disadvantages.⁸ Most of these assays also require significant sample preparation to be performed in a bulk solution where the initial amount of genetic material is limited, some is lost in processing, and the remaining material is used up quickly. Therefore, an assay that incorporates sample preparation and enables the original genetic template to be reused would be highly advantageous.

[0005] Aptamers are short single-stranded nucleic acids with structures determined by their specific nucleotide sequence. These molecules bind with high affinity and specificity to their intended targets. Aptamers are typically discovered by an iterative process called Systematic Evolution of Ligands by EXponential enrichment (SELEX) in which they are

35

selected from a very large, sequence-diverse library of nucleic acids (10^{12} - 10^{16} unique sequences).¹¹⁻¹³ Cell-SELEX was developed more recently to select aptamers that bind specifically to a certain type of cell.^{14,15} Using this technique, aptamers that bind specifically to cells of interest can be determined without any prior knowledge about the surface composition of the cells. Consequently, this method can be used to discover affinity ligands that bind to cancer cells.¹⁶⁻¹⁸

[0006] Many assays and devices are being developed that capture and isolate circulating tumor cells (CTCs), and although antibodies are traditionally used, aptamer-based CTC capture is also being performed.¹⁹⁻²⁴ Aptamers have been used over antibodies in these types of applications because of their increased robustness and ease of functionalization and oriented immobilization. The Tan group has developed several devices for capturing CTCs in which the aptamers are biotinylated and simply immobilized within the device by binding to streptavidin adsorbed on the channel surface.^{20,22,23,25,26}

[0007] A device for extracting and purifying human chromosomal DNA from lysed cells was previously developed.²⁷ This device incorporated a fine micropillar array that captured megabase-long genomic DNA (gDNA) strands via physical entanglement. The physical nature of this isolation enables the gDNA to be isolated without dependence on biochemical or electrostatic forces, making it available for downstream reactions. This also allows the gDNA to remain on the micropillar array during flow, which allows downstream analyses to be performed within the microdevice.

[0008] Genetic mutations in cancer cells are not only fundamental to the disease, but can also have tremendous impact on the efficacy of treatment. Identification of specific key mutations in a timely and cost-effective way would allow clinicians to better prescribe the most effective treatment options. Furthermore, cancer cells are constantly evolving, so regular testing of multiple important genes is also beneficial for monitoring disease progression and future treatment.

[0009] There is a need for new and improved technologies for studying cancer and particularly for detecting and understanding genetic mutations implicated in various cancers. This is also a need for additional methods of detecting and treating cancer.

[0010] The present invention is directed to overcoming these and other deficiencies in the art.

SUMMARY OF THE INVENTION

[0011] The present invention provides, *inter alia*, a combination of microfluidic and aptamer technologies suitable for use in studying, analyzing, detecting, and treating various conditions and diseases. In particular, the present invention provides a microfluidic device
5 for aptamer-based cancer cell capture and genetic mutation detection, and the use of the microfluidic device for various applications.

[0012] In one aspect, the present invention provides a microfluidic device comprising: a cell microchannel and a nucleic acid microchannel that intersect to form a cell capture intersection region; a cell capture array comprising a plurality of cell capturing
10 micropillars configured and arranged in a manner effective to capture one or more target cell when flowed through the cell microchannel, said cell capture array being located in the cell capture intersection region; and a nucleic acid entanglement array comprising a plurality of nucleic acid entanglement micropillars configured and arranged in a manner effective to physically entangle and maintain thereon genomic DNA isolated from the one or more target
15 cell, said nucleic acid entanglement array being located in a portion of the nucleic acid microchannel that is adjacent to and downstream of the cell capture intersection region. The microfluidic device is multi-functional in that it is effective for capturing said one or more target cell, isolating said genomic DNA from the one or more target cell, and analyzing said genomic DNA in a self-contained manner.

20 [0013] In one embodiment, the microfluidic device of the present invention further comprises a first flow rate means for managing rate of flow of fluid through the cell microchannel and a second flow rate means for managing rate of flow of fluid through the nucleic acid microchannel.

[0014] In another embodiment, the microfluidic device of the present invention
25 further comprises a temperature controller for managing temperature of fluid and other contents contained within the cell microchannel and/or nucleic acid microchannel.

[0015] In another aspect, the present invention provides a method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow for further analysis thereof. This method involves the steps of: providing a microfluidic device as
30 described herein; introducing a sample comprising one or more target cell into the cell microchannel at a flow rate effective to transport the one or more target cell to the cell capture array so as to capture the one or more target cell in the cell capturing micropillars by specific binding; lysing the one or more target cell by introducing lysing reagents through the

nucleic acid microchannel at a flow rate effective to release genomic DNA from the one or more target cell without shearing the genomic DNA; and maintaining fluid flow within the nucleic acid microchannel at a flow rate effective to cause the released genomic DNA to become physically entangled and maintained within the nucleic acid entanglement array for further analysis thereof.

[0016] In another aspect, the present invention provides a method for conducting aptamer-based cancer cell capture and genomic DNA mutation analysis of genomic DNA isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and conducting aptamer-based cancer cell capture and genomic DNA mutation analysis of the genomic DNA isolated from one or more target cell while in a flow environment within the microfluidic device.

[0017] In another aspect, the present invention provides a method for amplifying individual genes of interest from the one or more target cell consecutively and collecting each amplification product separately. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and amplifying individual genes of interest from the genomic DNA entangled and maintained under flow within the nucleic acid entanglement array of the microfluidic device consecutively and collecting each amplification product separately.

[0018] In another aspect, the present invention provides a method for sequencing nucleic acids amplified from genomic DNA isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and sequencing the genomic DNA entangled and maintained under flow within the nucleic acid entanglement array of the microfluidic device.

[0019] In another aspect, the present invention provides a method for multiple displacement amplification (MDA) reactions of one or more nucleic acid sequence isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and conducting multiple displacement amplification (MDA) reactions under flow using the genomic DNA entangled and maintained within the nucleic acid entanglement array of the microfluidic device.

[0020] In one aspect, the present invention relates to a novel microfluidic device that provides a platform for specifically capturing cancer cells and isolating the genomic DNA for specific amplification and sequence analysis. In one embodiment of the present invention, in order to filter out rare cancer cells from a complex mixture containing a diversity of cells, nucleic acid aptamers that specifically bind to cancer cells are immobilized within a microchannel containing pillars to increase the number of collisions with the surface and improve capture efficiency. The captured cells are then lysed and the genomic DNA is isolated via physical entanglement within a secondary micropillar array. This type of isolation enables multiple consecutive rounds of isothermal amplification to be performed to amplify different individual genes separately, since the genomic template is retained on the micropillars between subsequent amplifications. The amplified gene samples undergo Sanger sequencing, an inexpensive sequencing approach requiring a pure sample, to reveal the genetic sequence. The resulting sequence information is compared against the known wildtype gene, and any mutations are identified. This approach offers a way to monitor multiple genetic mutations in the same small population of cells, which is beneficial given the wide diversity in cancer cells, and requires very few cells to be extracted from the patient sample. With this capability for genetic monitoring, precision medicine should be more accessible for the diagnosis and treatment of cancer and other diseases.

[0021] One advantage of the microfluidic device of the present invention over the prior art is the combination of microfluidic aptamer-based cell capturing technology (e.g., high surface area microfluidic device for capturing selected cells by specific binding) with the elongation/capture/analysis of nucleic acids isolated from the captured cells (e.g., using small pillars or capture structures). As shown, the microfluidic device combines these technologies into a single, integrated device in a manner that is unique over the prior art technologies.

[0022] The microfluidic device of the present invention is unique over the prior art for a variety of reasons. For example, the design of a microfluidic device of the present invention is such that it can be fabricated as integrated unit, which is unique over the prior art which involves the use of separate devices, which have different requirements for their construction. Further, the operation of two, separate devices (as in the case of the prior art) would require sample extraction from one device and then sample preparation and then insertion into the other device. This would be very inefficient and cause the loss of portions of the sample being studied, as well as opening the process up to contamination. Being able

to use the current devices of the prior art does not inform one how to operate an integrated unit such as the one of the present invention, where all processes must be carried out on a chip with no valves or separate sample processing devices between them.

[0023] To date, there are no known reports in the prior art of the transfer of whole
5 genomic DNA from one device to another as would be required in the use of the microfluidic device of the present invention, where cells are selectively captured, DNA extracted and moved to a separate region of a device for sequence specific selective amplification.

[0024] In accordance with another aspect, the present invention provides a process for
10 preparing a microfluidic device according to the present invention, said process comprising steps as disclosed and/or contemplated herein.

[0025] In accordance with aspects of the present invention, there is provided a device
capable of specifically capturing cancer cells, isolating their gDNA, and amplifying specific
genes for sequencing to determine the presence of any genetic mutations in those genes. The
cancer cells are captured using aptamers immobilized on the microchannel surface, and the
15 gDNA is isolated via physical entanglement within a micropillar array. We developed a
modified version of multiple displacement amplification (MDA), an isothermal DNA
amplification technique, that amplifies a specific gene of interest. This amplification product
undergoes sequencing, and the resulting sequence is compared to the known human genome
to determine the presence of any genetic mutations. Identification of specific key mutations in
20 a timely and cost-effective way would allow clinicians to better prescribe the most effective
treatment options. Furthermore, since cancer cells are constantly evolving, regular testing of
multiple important genes is also beneficial for monitoring disease progression and
determining future treatment. The ability to perform this regular testing in a cost-effective
manner would encourage more frequent testing, which would likely improve overall
25 treatment efficacy.

[0026] These and other objects, features, and advantages of this invention will
become apparent from the following detailed description of the various aspects of the
invention taken in conjunction with the accompanying drawings.

30 BRIEF DESCRIPTION OF THE DRAWINGS

[0027] For the purpose of illustrating aspects of the present invention, there are
depicted in the drawings certain embodiments of the invention. However, the invention is not
limited to the precise arrangements and instrumentalities of the embodiments depicted in the

drawings. Further, as provided, like reference numerals contained in the drawings are meant to identify similar or identical elements.

[0028] **FIG. 1:** Schematic of portions of one embodiment of the microfluidic device of the present disclosure. Two intersecting microchannels with an aptamer-functionalized pillar array at the intersection for specific cancer cell capture. A finer micropillar array downstream for genomic DNA isolation via physical entanglement. The initial cell sample is injected into Inlet 1, flows through the capture region, and out Outlet 1. The lysis buffer is injected into Inlet 2, and the genomic DNA is entangled in the micropillar array, while the rest of the lysate flows out of the device through Outlet 2.

[0029] **FIG. 2:** Schematic of one embodiment of a microfluidic device of the present disclosure. The embodiment illustrates microfluidic channels for capture of different biological components from a sample.

[0030] **FIG. 3:** Microchannel design for capturing cancer cells and isolating their gDNA. The device contains two orthogonal channels, the cell channel and the DNA channel. It also contains two micropillar arrays, the cell capture array located at the intersection of the channels (red box, scale bar: 200 μ m) and the DNA isolation array located downstream of the cell capture array in the DNA channel (blue box, scale bar: 20 μ m). An image of the device is also displayed in the upper right corner.

[0031] **FIGS. 4A-4F:** Cancer cell capture in microfluidic channels using aptamers.

An illustration of the surface chemistry within the microchannels is shown on the left. All of the images shown are fluorescent images of the cell capture region. FIG. 4A and FIG. 4B show the device without aptamers after flowing HeLa and CAOV-3 cells, respectively, through the microchannel. FIG. 4C and FIG. 4D show the device containing aptamers after flowing Ect1/E6E7 and End1/E6E7 cells, respectively, through the microchannel. FIG. 4E and FIG. 4F show the device containing aptamers after flowing HeLa and CAOV-3 cells, respectively, through the microchannel. FIG. 4C shows fluorescent images of the cell capture region without aptamers after flowing CAOV-3 cells through the microchannels. The HeLa cells fluoresce due to GFP bound to their histones, and the CAOV-3, Ect1/E6E7, and End1/E6E7 cells were stained with calcein-AM.

[0032] **FIGS. 5A-5D:** Cancer cell lysis and isolation of gDNA via physical entanglement within the micropillar array. FIG. 5A: Fluorescent image of HeLa cells bound to aptamers in the cell capture region. FIG. 5B: Fluorescent image of gDNA from HeLa cells isolated by the micropillar array and stained with YOYO-1 dye. FIG. 5C: Fluorescent

image of CAOV-3 cells stained with calcein-AM and bound to aptamers in the cell capture region. FIG. 5D: Fluorescent image of gDNA from CAOV-3 cells isolated by the micropillar array and stained with YOYO-1 dye.

[0033] **FIGS. 6A-6D:** Gel images of benchtop and on-chip demonstration of specific MDA of the *TP53* gene and smaller gene fragments from PCR. FIG. 6A: MDA product from reactions using 15 ng of purified HeLa gDNA. Different quantities of primers were tested, as well as negative controls containing no gDNA template. The MDA product was run on a 1% agarose gel and was approximately 10 kb. FIG. 6B: PCR product from reactions amplifying a shorter *TP53* gene fragment using 60% of the MDA product. The PCR product was run on a 2.5% agarose gel and was 130 nt in length. FIG. 6C: On-chip MDA product from isolated HeLa and CAOV-3 cell gDNA verified using a 1% agarose gel. The ladder indicates that the product was around 10 kb in length. FIG. 6D: PCR product verified via 8% PAGE. The ladder confirmed a product length of 130 bp.

[0034] **FIGS. 7A-7B:** Sanger sequencing results from HeLa and CAOV-3 cell *TP53* gene fragments where a SNP is known to occur in CAOV-3 cells. FIG. 7A: Wildtype sequence for the *TP53* region is shown and was obtained from the International Agency for Research on Cancer. Sequencing results for the HeLa cell *TP53* region are shown. FIG. 7B: Mutant sequence for the known SNP in CAOV-3 cells where a C is replaced by a T. Sequencing results for the CAOV-3 cell *TP53* region are shown. The specific base that is mutated is underlined. FIG. 12 shows the wildtype sequence (SEQ ID NO:1) and the sequencing results for the *TP53* fragments from HeLa (SEQ ID NO:2) and CAOV-3 (SEQ ID NO:3) cells.

[0035] **FIG. 8:** Benchtop MDA results for *PTEN* and *BRCA2* genes. MDA reactions were performed using the primers for *PTEN* and *BRCA2*, and controls containing no gDNA and reactions containing 15ng of gDNA extracted from CAOV-3 cells were performed. The reaction products were analyzed on a 1% agarose gel. The yellow arrow indicates the 10-kb MDA product band on the gel.

[0036] **FIG. 9:** Benchtop PCR results for *PTEN* and *BRCA2* genes. PCR reactions were performed using the primers for *PTEN* and *BRCA2*, and controls containing no MDA product and reactions containing 60% of the MDA product were performed. The reaction products were analyzed on a 10% polyacrylamide gel. The yellow arrow indicates the 130-nt PCR product band on the gel.

[0037] **FIG. 10:** On-chip MDA results for *PTEN* and *BRCA2* genes. MDA reactions were performed within channels containing isolated CAO V-3 gDNA using either *PTEN* or *BRCA2* MDA primers. The MDA product was analyzed on a 1% agarose gel. The yellow arrows indicate the ~10-kb MDA product.

5 [0038] **FIG. 11:** Product from PCR reaction using 60% of the MDA product amplifying the *PTEN* and *BRCA2* genes on-chip from CAO V-3 cells. PCR reactions were performed using the primers for *PTEN* and *BRCA2*, and controls containing no MDA product and reactions containing 60% of the MDA product were performed. The PCR products were analyzed on a 10% PAGE gel. The yellow arrows indicate the 130-bp PCR product.

10 [0039] **FIG. 12:** Sanger sequencing results indicating the point mutation in the *TP53* gene in CAO V-3 cells. The wildtype sequence (SEQ ID NO:1) for this fragment of the *TP53* gene is shown at the top of the figure. The upper plot shows the sequencing results for this gene fragment (SEQ ID NO:2) for HeLa cells. The lower plot shows the sequencing results for this gene fragment (SEQ ID NO:3) for CAO V-3 cells. The yellow box highlights the
15 region where the mutation is located, and the base that is mutated is underlined in black. Some bases were not called by the sequencing software, but the bases can be determined by looking at the plot peaks.

DETAILED DESCRIPTION OF THE INVENTION

20 [0040] The present invention relates to, *inter alia*, a combination of microfluidic and aptamer technologies suitable for use in studying, analyzing, detecting, and treating various conditions and diseases.

[0041] More particularly, in one aspect, the present invention relates to a microfluidic device for aptamer-based cancer cell capture and genetic mutation detection, and the use of
25 the microfluidic device for various applications.

[0042] In one aspect, the present invention provides a microfluidic device comprising: a cell microchannel and a nucleic acid microchannel that intersect to form a cell capture intersection region; a cell capture array comprising a plurality of cell capturing micropillars configured and arranged in a manner effective to capture one or more target cell
30 when flowed through the cell microchannel, said cell capture array being located in the cell capture intersection region; and a nucleic acid entanglement array comprising a plurality of nucleic acid entanglement micropillars configured and arranged in a manner effective to physically entangle and maintain thereon genomic DNA isolated from the one or more target

cell, said nucleic acid entanglement array being located in a portion of the nucleic acid microchannel that is adjacent to and downstream of the cell capture intersection region. The microfluidic device is multi-functional in that it is effective for capturing said one or more target cell, isolating said genomic DNA from the one or more target cell, and analyzing said genomic DNA in a self-contained manner.

[0043] In one embodiment of the microfluidic device of the present invention, the cell capture array comprises one or more aptamer and/or another cell capture component specific to the one or more target cell.

[0044] In another embodiment, the one or more aptamer and/or another cell capture component is concentrated in the cell capture intersection region, thereby enabling capture of the one or more target cell.

[0045] In another embodiment, the nucleic acid entanglement array is effective to entangle and maintain the isolated genomic DNA for single amplification and/or multiple, consecutive amplifications of one or more nucleic acid sequence of interest contained on the isolated genomic DNA.

[0046] In certain embodiments, the one or more nucleic acid sequence of interest is a cancer gene. In other embodiments, the one or more target cell is a cancer cell.

[0047] In one embodiment, the microfluidic device of the present invention further comprises a first flow rate means for managing rate of flow of fluid through the cell microchannel and a second flow rate means for managing rate of flow of fluid through the nucleic acid microchannel.

[0048] In another embodiment, the first flow rate means comprises external valves at the nucleic acid microchannel inlet and outlet and the second flow rate means comprises external valves at the cell microchannel inlet and outlet.

[0049] In one embodiment, the external valves are selected from the group consisting of two-way valves and four-way valves.

[0050] In another embodiment, the microfluidic device of the present invention further comprises a temperature controller for managing temperature of fluid and other contents contained within the cell microchannel and/or nucleic acid microchannel.

[0051] In one embodiment, the cell microchannel and the nucleic acid microchannel have a height ranging from between about 20 μm and about 40 μm .

[0052] In one embodiment, the cell microchannel and the nucleic acid microchannel have a height of about 20, 21, 22, 23, 24, 25, 26, 27, 28, 29, 30, 31, 32, 33, 34, 35, 36, 37, 38, 39, or 40 μm .

[0053] In one embodiment, the cell microchannel and the nucleic acid microchannel
5 have a height of about 25 μm .

[0054] In one embodiment, the cell channel has a width ranging from between about 500 μm and about 1500 μm .

[0055] In one embodiment, the cell channel has a width of about 500, 510, 520, 530, 540, 550, 560, 570, 580, 590, 600, 610, 620, 630, 640, 650, 660, 670, 680, 690, 700,
10 710, 720, 730, 740, 750, 760, 770, 780, 790, 800, 810, 820, 830, 840, 850, 860, 870, 880, 890, 900, 910, 920, 930, 940, 950, 960, 970, 980, 990, or 1000 μm .

[0056] In one embodiment, the cell channel has a width of about 1000 μm .

[0057] In one embodiment, the nucleic acid channel has a width ranging from between about 200 μm and about 1500 μm .

[0058] In one embodiment, the nucleic acid channel has a width selected from the
15 group consisting of about 200, 210, 220, 230, 240, 250, 260, 270, 280, 290, 300, 310, 320, 330, 340, 350, 360, 370, 380, 390, 400, 410, 420, 430, 440, 450, 460, 470, 480, 490, 500, 510, 520, 530, 540, 550, 560, 570, 580, 590, 600, 610, 620, 630, 640, 650, 660, 670, 680, 690, 700, 710, 720, 730, 740, 750, 760, 770, 780, 790, 800, 810, 820, 830, 840, 850,
20 860, 870, 880, 890, 900, 910, 920, 930, 940, 950, 960, 970, 980, 990, 1000, 1010, 1020, 1030, 1040, 1050, 1060, 1070, 1080, 1090, 1100, 1120, 1130, 1140, 1150, 1160, 1170, 1180, 1190, 1200, 1210, 1220, 1230, 1240, 1250, 1260, 1270, 1280, 1290, 1300, 1310, 1320, 1330, 1340, 1350, 1360, 1370, 1380, 1390, 1400, 1410, 1420, 1430, 1440, 1450, 1460, 1470, 1480, 1490, or 1500 μm .

[0059] In one embodiment, the nucleic acid channel has a width selected from the
25 group consisting of about 250 μm , 500 μm , and 1000 μm .

[0060] In one embodiment, the cell capturing micropillars have a diameter ranging from between about 40 μm and about 60 μm .

[0061] In one embodiment, the cell capturing micropillars have a diameter of about
30 40, 41, 42, 43, 44, 45, 46, 47, 48, 49, 50, 51, 52, 53, 54, 55, 56, 57, 58, 59, or 60 μm .

[0062] In one embodiment, the cell capturing micropillars have a diameter of about 50 μm .

[0063] In one embodiment, the cell capture array is ordered in a patterned array that is rotated by about 4° to maximize contact between the one or more target cell and microchannel surface.

[0064] In one embodiment, the nucleic acid entanglement micropillars have a diameter ranging from between about 2 μm and about 10 μm.

[0065] In one embodiment, the nucleic acid entanglement micropillars have a diameter of about 2.0, 2.5, 3.0, 3.5, 4.0, 4.5, 5.0, 5.5, 6.0, 6.5, 7.0, 7.5, 8.0, 8.5, 9.0, 9.5, or 10 μm.

[0066] In one embodiment, the nucleic acid entanglement micropillars have a cross-sectional dimension of about 4 μm x 4 μm, wherein said nucleic acid entanglement micropillars are spaced in a gradient that begins with the micropillars being about 10 μm apart and ending with the micropillars being about 7 μm apart.

[0067] In another aspect, the present invention provides a method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow for further analysis thereof. This method involves the steps of: providing a microfluidic device as described herein; introducing a sample comprising one or more target cell into the cell microchannel at a flow rate effective to transport the one or more target cell to the cell capture array so as to capture the one or more target cell in the cell capturing micropillars by specific binding; lysing the one or more target cell by introducing lysing reagents through the nucleic acid microchannel at a flow rate effective to release genomic DNA from the one or more target cell without shearing the genomic DNA; and maintaining fluid flow within the nucleic acid microchannel at a flow rate effective to cause the released genomic DNA to become physically entangled and maintained within the nucleic acid entanglement array for further analysis thereof.

[0068] In one embodiment, the one or more target cell is captured in the cell capture array due to specific contact with an aptamer or other capture component present in the cell capture array.

[0069] In one embodiment, the one or more target cell is introduced into the cell microchannel and thereafter captured within the cell capture array under a flow rate ranging from between about 0.1 μL/minute and about 20 μL/minute.

[0070] In one embodiment, the one or more target cell is introduced into the cell microchannel and thereafter captured within the cell capture array under a flow rate of about 0.1, 0.5, 1.0, 1.5, 2.0, 2.5, 3.0, 3.5, 4.0, 4.5, 5.0, 5.5, 6.0, 6.5, 7.0, 7.5, 8.0, 8.5, 9.0, 9.5, 10,

10.5, 11, 11.5, 12, 12.5, 13, 13.5, 14, 14.5, 15, 15.5, 16, 16.5, 17, 17.5, 18, 18.5, 19, 19.5, or 20 $\mu\text{L}/\text{minute}$.

[0071] In one embodiment, the lysing reagents are introduced through the nucleic acid microchannel at a flow rate ranging from between about 0.1 $\mu\text{L}/\text{minute}$ and about 2 $\mu\text{L}/\text{minute}$, thereby causing the release of the genomic DNA from the one or more target cell without shearing the genomic DNA.

[0072] In one embodiment, the flow of fluid in the nucleic acid microchannel is maintained at a flow rate ranging from between about 0.05 $\mu\text{L}/\text{minute}$ and about 2 $\mu\text{L}/\text{minute}$, thereby causing the released genomic DNA to become physically entangled and maintained within the nucleic acid entanglement array.

[0073] In one embodiment, the one or more target cell is a cancer cell, although the present invention can be used for any type of cell of structure that contains DNA or genomic DNA.

[0074] In another aspect, the present invention provides a method for conducting aptamer-based cancer cell capture and genomic DNA mutation analysis of genomic DNA isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and conducting aptamer-based cancer cell capture and genomic DNA mutation analysis of the genomic DNA isolated from one or more target cell while in a flow environment within the microfluidic device.

[0075] In another aspect, the present invention provides a method for amplifying individual genes of interest from the one or more target cell consecutively and collecting each amplification product separately. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and amplifying individual genes of interest from the genomic DNA entangled and maintained under flow within the nucleic acid entanglement array of the microfluidic device consecutively and collecting each amplification product separately.

[0076] In another aspect, the present invention provides a method for sequencing nucleic acids amplified from genomic DNA isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow;

and sequencing the genomic DNA entangled and maintained under flow within the nucleic acid entanglement array of the microfluidic device.

[0077] In another aspect, the present invention provides a method for multiple displacement amplification (MDA) reactions of one or more nucleic acid sequence isolated from one or more target cell. This method includes the steps of: performing the steps described herein of the method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow; and conducting multiple displacement amplification (MDA) reactions under flow using the genomic DNA entangled and maintained within the nucleic acid entanglement array of the microfluidic device.

[0078] In one embodiment, the MDA reactions involve using the same genomic DNA template isolated by the nucleic acid entanglement micropillars of the microfluidic device.

[0079] FIGS. 1-3 provide schematic views of illustrative embodiments and aspects of the microfluidic device of the present invention. While the aforementioned figures relate to and are further described below and in the examples also provided herein below, these figures are helpful in describing the microfluidic device and any related systems and methods in general terms.

[0080] FIG. 1 and FIG. 3 are schematic illustrations aspects of one embodiment of microfluidic device 10 of the present disclosure. In particular, FIG. 1 and FIG. 3 illustrate microfluidic device 10 as having cell microchannel 20 and nucleic acid microchannel 30, which intersect to form cell capture intersection region 40. Microfluidic device 10 is also shown to include cell capture array 50, which includes a plurality of cell capturing micropillars 60 configured and arranged in a manner effective to capture one or more target cell when such cells are flowed through cell microchannel 20. Cell capture array 50 is located in cell capture intersection region 40. Microfluidic device 10 is also shown to include nucleic acid entanglement array 70, which includes a plurality of nucleic acid entanglement micropillars 80 configured and arranged in a manner effective to physically entangle and maintain thereon genomic DNA isolated from the one or more target cell. Nucleic acid entanglement array 70 is located in a portion of nucleic acid microchannel 30 that is adjacent to and downstream of cell capture intersection region 40. Microfluidic device 10 is multi-functional in that it is effective for capturing said one or more target cell, isolating said genomic DNA from the one or more target cell, and analyzing said genomic DNA in a self-contained manner.

[0081] FIG. 2 is a schematic of one embodiment of microfluidic device 10 of the present disclosure, which embodiment can be used for capturing different biological components from a sample. As shown in FIG. 2, microfluidic device 10 can be used to capture genomic DNA 90 from three, different types of DNA sources, i.e., cancer cells, bacteria cells, and viruses, but from a single sample (e.g., a single blood sample). As shown in FIG. 2, this embodiment of microfluidic device 10 illustrates three different cell capture intersection regions 40. Each cell capture intersection region 40 is formed by the intersection of three, separate nucleic acid microchannels 30 with different portions of cell microchannel 20. In particular, as shown in FIG. 2 (moving from left to right along cell microchannel 20), there is cell capture intersection region 40 for cancer cell capture, cell capture intersection region 40 for bacteria cell capture, and cell capture intersection region 40 for virus capture.

[0082] As illustrated in FIG. 2, a blood sample enters microfluidic device 10 at an input port of cell microchannel 20 (left end in FIG. 2). The first cell capture intersection region 40 includes a cell capture array having cell capturing micropillars that are specific for certain cancer cells, so that such cancer cells are captured in the first capture intersection region 40 and then lysed, with genomic DNA 90 from the captured and lysed cancer cells being released and physically entangled and maintained by nucleic acid entanglement micropillars 80 of nucleic acid entanglement array 70 at a position within the first nucleic acid microchannel 30 that is downstream of the first cell capture intersection region 40. The second cell capture intersection region 40 (in the middle) includes a cell capture array having cell capturing micropillars that are specific for certain bacteria cells, so that such bacteria cells are captured in the second capture intersection region 40 and then lysed, with genomic DNA 90 from the captured and lysed bacteria cells being released and physically entangled and maintained by nucleic acid entanglement micropillars 80 of nucleic acid entanglement array 70 at a position within the second nucleic acid microchannel 30 that is downstream of the second cell capture intersection region 40. The third cell capture intersection region 40 (on the right) includes a cell capture array having cell capturing micropillars that are specific for certain viruses, so that such viruses are captured in the third capture intersection region 40 and then lysed, with genomic DNA 90 from the captured and lysed viruses being released and physically entangled and maintained by nucleic acid entanglement micropillars 80 of nucleic acid entanglement array 70 at a position within the third nucleic acid microchannel 30 that is downstream of the third cell capture intersection region 40.

[0083] Aspects of the microfluidic device of the present invention and various methods of use thereof are further described below. Certain terms are used that are interchangeable with the terms provided herein above and in the claims. Such interchangeable terminology is readily apparent to those of ordinary skill in the art.

5 [0084] In accordance with one embodiment, the present invention includes a microfluidic device capable of specifically capturing rare cancer cells and isolating their genomic DNA for on-chip amplification and subsequent genetic sequencing. The device is fabricated out of polydimethylsiloxane (PDMS) using a silicon mold. The PDMS is bonded to a glass substrate to form the microfluidic channels. The device contains two
10 microchannels intersecting at right angles with a pillar array at the intersection functionalized with single stranded DNA aptamers that serve as specific capture ligands for cancer cells. The pillars are rotated 4° to increase the number of collisions cells undergo with the surface, thereby increasing the capture efficiency. In one of the channels downstream from the cell capture zone, there is a secondary micropillar array with smaller pillars spaced closely
15 together that will isolate the genomic DNA from the lysed captured cells. This DNA will remain entangled in the micropillar array through multiple isothermal amplification reactions. The amplification product will be extracted from the outlet of the device, and the DNA will be sequenced to identify any genetic mutations.

[0085] As noted above, FIG. 1 is a schematic of one embodiment of the microfluidic
20 device setup in accordance with the present invention. As shown in FIG. 1, two intersecting microchannels with an aptamer-functionalized pillar array at the intersection for specific cancer cell capture. A finer micropillar array downstream for genomic DNA isolation via physical entanglement. The initial cell sample is injected into Inlet 1, flows through the capture region, and out Outlet 1. The lysis buffer is injected into Inlet 2, and the genomic
25 DNA is entangled in the micropillar array, while the rest of the lysate flows out of the device through Outlet 2.

[0086] Aptamers are single stranded nucleic acids that are analogous to antibodies in that they are ligands with specific binding affinity to their target, but with several advantages over antibodies. Aptamers are chemically synthesized with no batch-to-batch variability,
30 much less expensive, more robust, and more easily functionalized. Here, a previously-selected aptamer with specific affinity to surface species present on several types of cancer cells that will capture the rare cancer cells and filter them from a complex sample can be used (*see* Van Simaey D, López-Colón D, Sefah K, Sutphen R, Jimenez E, Tan W (2010) Study

of the molecular recognition of aptamers selected through ovarian cancer cell-SELEX. *PLoS One* 5:e13770. doi: 10.1371/journal.pone.0013770).

[0087] To detect specific genetic mutations, these genes can be individually amplified in separate multiple displacement amplification (MDA) reactions using the same genomic DNA template isolated by the micropillars. Following each amplification, the product can be extracted from the device through the outlet. These samples can be sequenced using Sanger sequencing, which requires pure samples with a single DNA sequence, and this can be accomplished using our device capable of separate consecutive amplification reactions on the same genomic DNA. The sequencing results can be compared to the known wildtype genes, and any mutations can be identified. This information can then be passed onto clinicians to make informed recommendations for the most appropriate and effective treatment for each patient.

[0088] In various other embodiments, the present invention provides a microfluidic device for capturing selected cells and efficiently separating genomic DNA from other cellular components.

[0089] Further, although certain aspects of the present invention primarily relate to the processing and analysis of DNA extracted and immobilized in the device and treating the other cellular components, in other aspects, the present invention also relates to the use of a microfluidic device for separating the cellular components from the genomic DNA such as mitochondrial DNA or RNA.

[0090] One advantage of the microfluidic device of the present invention is that it is an integrated device, as shown herein. The integrated device of the present invention obviates the need for transferring the sample from one device to another and therefore reduces the possibilities for contamination of the sample.

[0091] The structures that are employed in the microfluidic device of the present invention for capturing the cells can be of many forms. For example, in certain embodiments, the structures can be coated with antibodies or aptamers and can include, without limitation, structures such as pillars, beads, flat surfaces, or patterned surfaces. Such methods for incorporating such features in microfluidics are known to those skilled in the art.

[0092] In accordance with the present invention, the ability to capture the DNA by mechanical entanglement with pillared structures allows the application of sequential chemical treatments and washing steps by flowing different solutions past the immobilized DNA.

[0093] The microfluidic device of the present invention can be constructed of various suitable materials. For example, in certain embodiments, the microfluidic device is constructed of transparent plastic. However, the microfluidic device of the present invention can alternatively be made of glass or other optically transparent materials to permit optical
5 microscopic imaging of captured cells and DNA. This would permit histological evaluation of cells by a Pathologist to combine conventional imaging and analysis of cells to be combined with our molecular diagnostics.

[0094] In certain embodiments, the microfluidic device of the present invention can include multiple stages of cell capture regions of different geometry and chemical coatings to
10 capture different cell types or other biological entities such as cancer cells, shed cells from implanted tissue, parasites, pathogens, bacteria, viruses, and others.

[0095] As described herein, FIG. 2 illustrates one non-limiting embodiment of a microfluidic device having a channel structure for capturing different biological entities for analysis.

[0096] The microfluidic device can be used to study various genes of interest, including, without limitation, genes of interest in cancer. For example, as shown in the examples section below, one such gene of interest is the TP53 gene. Additional examples of genes of interest in cancer include, without limitation, APC, BRCA1, BRCA2, CDK4, CMM1, HER2, MLH1, MSH2, p16, and Rb1. The microfluidic device of the present
15 invention can be used to study these and other cancer genes, as well as other genes not associated with cancer.

[0097] The microfluidic device of the present invention can be constructed so that it does not require internal valves to control the flow of fluid or other materials through the channels of the device. Thus, in accordance with the present invention, there are multiple
25 ways to control the flow through the device. For example, external valves can be used to control the flow. Alternatively, tubing clamps or fluidic “plugs” can also be used to control the direction of flow in the microfluidic device of the present invention.

[0098] The microfluidic device of the present invention can also use various types of cell capture components in addition to those specifically described herein. For example,
30 antibodies or other recognition elements could be used in the same way as described herein with the same surface chemistry (e.g., biotinylated). Such cell capture alternatives would work and could be incorporated into the microfluidic device.

[0099] The microfluidic device of the present invention can be used to incorporate various technologies relating to microfluidic arrays, microfluidic cell capture, aptamer-based cell capture, nucleic acid elongation and capture, and the like. Such compatible technologies described in the art can be found in various published U.S. patent applications, including, without limitation, the following (which are incorporated herein by reference in their entirety): US-2015/0291952, US-2015/0204859, US-2014/0121132, US-2014/0194313, and US-2015/0011425.

EXAMPLES

10 [00100] The following examples are intended to illustrate particular embodiments of the present invention, but are by no means intended to limit the scope of the present invention.

Example 1

15 **Microfluidic Device for Aptamer-Based Cancer Cell Capture and Gene Mutation Detection**

[00101] Genetic mutations in cancer cells are not only fundamental to the disease, but can also have tremendous impact on the efficacy of treatment. Identification of specific key mutations in a timely and cost-effective way would allow clinicians to better prescribe the most effective treatment strategy. Here, we present a novel microfluidic device as a platform for specifically capturing cancer cells and isolating their genomic DNA (gDNA) for specific amplification and sequence analysis. To capture cancer cells within the device, nucleic acid aptamers that specifically bind to cancer cells are immobilized within a microchannel containing micropillars to increase capture efficiency. The captured cells are then lysed and the gDNA is isolated via physical entanglement within a secondary micropillar array. This type of isolation allows the gDNA to be retained within the channel, and enables multiple types of analysis to be performed on the same gDNA template. The amplified gene samples undergo sequencing, and the resulting sequence information is compared against the known wildtype gene to identify any mutations. Cervical and ovarian cancer cells have been tested for mutations in the *TP53*, *PTEN*, and *BRCA2* genes using this technology. This approach offers a way to monitor multiple genetic mutations in the same small population of cells, which is beneficial given the wide diversity in cancer cells, and requires very few cells to be

extracted from the patient sample. With this capability for genetic monitoring, precision medicine should be more accessible for the treatment of cancer.

Experimental

5 Cell Culture and Buffers:

[00102] HeLa, CAOV-3, Ect1/E6E7, and End1/E6E7 cells were purchased from American Type Cell Culture (ATCC). The HeLa and CAOV-3 cells were cultured in DMEM media (Life Technologies) supplemented with non-essential amino acids, 110 mg/L sodium pyruvate, 200mM L-glutamine (Life Technologies), 1x Pen Strep (Life Technologies), 10 pyruvate, 200mM L-glutamine (Life Technologies), 1x Pen Strep (Life Technologies), 26.8mM HEPES, betamercaptoethanol, and containing 10% fetal bovine serum. The Ect1/E6E7 and End1/E6E7 cells were cultured in keratinocyte-serum free media (Life Technologies) with 0.1 ng/mL human recombinant epidermal growth factor (Life Technologies), 0.05 mg/mL bovine pituitary extract (Life Technologies), and an additional 15 44.1 mg/L calcium chloride. Prior to use, the cells were trypsinized and resuspended in phosphate-buffered saline (PBS) binding buffer [1x Dulbecco's PBS with calcium chloride and magnesium chloride (Fisher Scientific) containing 4.5 g/L glucose, 5 mM MgCl₂, and 0.1% Pluronic F-68 non-ionic surfactant (Sigma Aldrich)]. HeLa cells contained GFP-conjugated histones, and CAOV-3, Ect1/E6E7, and End1/E6E7 cells were stained with 20 calcein-AM (Thermo Fisher Scientific) that allowed them to be observed using fluorescence microscopy.

Device Fabrication:

25 [00103] The devices used here were polydimethylsiloxane (PDMS) microchannels bonded to glass substrates. The devices consisted of two orthogonal microchannels that contained two micropillar arrays: a cell capture array at the intersection of the two microchannels and a gDNA isolation array downstream of the cell capture array (see FIG. 3). The PDMS channels were made via soft lithography using a silicon master mold. The master 30 mold was fabricated from a 4" silicon wafer via standard photolithography. Microposit S1813 photoresist (Shipley) was spun onto silicon wafers and exposed to UV light using a contact mask aligner (ABM). The exposed wafer was developed using 726MIF developer (Microchemicals) and the pattern was etched 25 μm into the silicon via Bosch process using a Unaxis SLR 770 deep reactive ion etching system (Unaxis USA Inc.). A monolayer of 35 (1H,1H,2H,2H-Perfluorooctyl)Trichlorosilane (FOTS) was deposited onto the etched silicon

surface using an MVD100 molecular vapor deposition system (Applied Microstructures) to enable easy release of the PDMS from the silicon mold.

[00104] Sylgard 184 (Dow Corning) PDMS base resin was mixed in a 10:1 ratio with curing agent, and degassed in a vacuum oven at room temperature. The PDMS was poured
5 onto the master mold and baked at 140°C for 1 hour. The PDMS was allowed to cool to room temperature, and it was carefully peeled off of the mold. Inlet and outlet holes were created using a 1mm biopsy punch (Sklar Instruments). To complete the formation of the channels, the patterned PDMS and a microscope slide were treated with oxygen plasma for 5 min, and then bonded together. An external 4-way L-type valve (IDEX Health and Science) was used
10 at the DNA channel inlet and external 2-way valves were used at the cell channel inlet and both outlets to control the flow between the perpendicular channels.

Surface Chemistry:

[00105] DNA aptamers that were used to capture cancer cells were immobilized onto the surface of the microchannels via a streptavidin-biotin conjugation. The channels were initially primed and cleaned with 100% ethanol and ultrapure water. A 1x PBS solution was pumped through the channels at 50 $\mu\text{L}/\text{min}$ for 9 min. A 1 mg/mL solution of streptavidin (Life Technologies) in PBS was prepared, and 120 μL were pumped through the cell channel
20 (see FIG. 3) at 4 $\mu\text{L}/\text{min}$ to immobilize streptavidin via adsorption onto the channel surface. A blocking solution containing 1% bovine serum albumin (BSA), 1% Pluronic F-68, and 1% polyvinylpyrrolidone (PVP) K15 was prepared in 1x PBS with calcium chloride and magnesium chloride, and 500 μL of this solution was pumped through both the cell and DNA channels at 4 $\mu\text{L}/\text{min}$ to block the surface of the channel and prevent non-specific adhesion of
25 cells and other reagents. Finally, biotinylated aptamers (Integrated DNA Technologies), which were previously selected (DOV4) to bind to several different types of cancer cells,¹⁸ were diluted to 10 μM in PBS binding buffer, and 180 μL were pumped through the DNA channel at 3 $\mu\text{L}/\text{min}$. This process enabled the aptamers to be concentrated in the cell capture region at the intersection of the two channels.

Cell Capture, Lysis, and gDNA Isolation:

[00106] Cells suspended in PBS binding buffer were pumped through the cell channel (see FIG. 3) at 1 $\mu\text{L}/\text{min}$ until several cells were captured, as observed via fluorescence
35 microscopy. A solution of 6 M guanidinium isothiocyanate (VWR) was pumped at 1 $\mu\text{L}/\text{min}$

through the DNA channel until cell lysis was observed. By lysing the cells in the direction of the DNA micropillar array, the gDNA becomes physically entangled and remains in the channel even under flow. To verify the gDNA was captured and retained by the micropillar array, YOYO-1 dye was used to stain the DNA in the channel by flowing the dye through the DNA channel at 1 $\mu\text{L}/\text{min}$. Otherwise, following lysis, the gDNA was washed with 1x Tris-Ethylenediaminetetraacetic acid (TE) buffer to remove any remaining cellular debris and guanidinium isothiocyanate.

Primers and Specific Gene Amplification from gDNA:

[00107] To amplify a specific gene from gDNA isothermally, MDA was used with specific primers targeting a fragment of the *TP53*, *PTEN*, or *BRCA2* gene. Table 1 contains the 40 short primers used for these amplifications. Initially, the isolated gDNA was chemically denatured using Buffer DLB from the Repli-g Mini Kit (Qiagen) prepared according to the manufacturer's instructions. This solution was pumped through the DNA channel at 1 $\mu\text{L}/\text{min}$ for 25 min. The gDNA was then neutralized using the Stop Solution from the Repli-g Mini Kit with the addition of 12 pmol of each MDA primer. This solution was pumped at 1 $\mu\text{L}/\text{min}$ for 45 min. An MDA reaction solution was prepared from the Repli-g Mitochondrial DNA Kit according to the manufacturer's instructions, and 15-30 pmol of each MDA primer was added to the reaction solution. The microchannel device was placed on a hotplate set to 33°C, and 50 μL of MDA reaction solution was pumped through at 0.05 $\mu\text{L}/\text{min}$ to perform the MDA reaction for approximately 16 hours. The eluent was collected in an Eppendorf tube. For consecutive rounds of on-chip MDA gene amplification from the same gDNA, the gDNA was denatured again, neutralized, and the MDA reaction was performed as described above, but using different primers.

[00108] For benchtop control experiments, gDNA from HeLa and CAOV-3 cells was extracted using the Blood and Cell Culture DNA Mini Kit (Qiagen). Buffer D1 and Buffer N1 from the Repli-g Mini Kit (Qiagen) were prepared, and 15 ng of extracted gDNA were denatured and neutralized according to the manufacturer's instructions. An MDA reaction master mix was prepared using the buffer and DNA polymerase from the Repli-g Mitochondrial DNA Kit (Qiagen) and various concentrations of specific MDA primers (Table 1), and this solution was added to the denatured and neutralized gDNA. This reaction was incubated at 33°C for 16 hours.

Table 1: Amplification Primer Sequences

MDA Primers for the <i>TP53</i>, <i>PTEN</i>, and <i>BRCA2</i> Genes			
Primer Name	Sequence	Primer Name	Sequence
<i>TP53</i> MDA FOR #1	TTG TGC CCT G (SEQ ID NO:4)	<i>TP53</i> MDA REV #1	GCC ATG GCG C (SEQ ID NO:5)
<i>TP53</i> MDA FOR #2	CAG TTG CTT T (SEQ ID NO:6)	<i>TP53</i> MDA REV #2	GCT GTG ACT G (SEQ ID NO:7)
<i>TP53</i> MDA FOR #3	GTT TCT TTG C (SEQ ID NO:8)	<i>TP53</i> MDA REV #3	CCT CAC AAC C (SEQ ID NO:9)
<i>TP53</i> MDA FOR #4	GGA GGT GCT T (SEQ ID NO:10)	<i>TP53</i> MDA REV #4	CGC TCA TGG T (SEQ ID NO:11)
<i>TP53</i> MDA FOR #5	TAG CTC GCT A (SEQ ID NO:12)	<i>TP53</i> MDA REV #5	CAC CAT CGC T (SEQ ID NO:13)
<i>TP53</i> MDA FOR #6	GTG TAG ACG C (SEQ ID NO:14)	<i>TP53</i> MDA REV #6	TCT CTC CAG C (SEQ ID NO:15)
<i>TP53</i> MDA FOR #7	CCT ATC TCA A (SEQ ID NO:16)	<i>TP53</i> MDA REV #7	CTG GGC AAC C (SEQ ID NO:17)
<i>TP53</i> MDA FOR #8	CCT GAG TGA C (SEQ ID NO:18)	<i>TP53</i> MDA REV #8	GAA TCA GAG G (SEQ ID NO:19)
<i>TP53</i> MDA FOR #9	ATC ACA CCA C (SEQ ID NO:20)	<i>TP53</i> MDA REV #9	ACC TAA GAG C (SEQ ID NO:21)
<i>TP53</i> MDA FOR #10	GGA GGC TGC A (SEQ ID NO:22)	<i>TP53</i> MDA REV #10	AGA TGC TGA G (SEQ ID NO:23)
<i>TP53</i> MDA FOR #11	ATC ACT TGA G (SEQ ID NO:24)	<i>TP53</i> MDA REV #11	TCC ACA CGC A (SEQ ID NO:25)
<i>TP53</i> MDA FOR #12	TAG GAG GCT G (SEQ ID NO:26)	<i>TP53</i> MDA REV #12	TGT TTC TGT C (SEQ ID NO:27)
<i>TP53</i> MDA FOR #13	CAC CTA TAG T (SEQ ID NO:28)	<i>TP53</i> MDA REV #13	CAC CAC ACT A (SEQ ID NO:29)
<i>TP53</i> MDA FOR #14	TAG CCA GGC A (SEQ ID NO:30)	<i>TP53</i> MDA REV #14	TCA GGC GGC T (SEQ ID NO:31)
<i>TP53</i> MDA FOR #15	ACC TCG TCT C (SEQ ID NO:32)	<i>TP53</i> MDA REV #15	CCC CAG TTG C (SEQ ID NO:33)
<i>TP53</i> MDA FOR #16	AGC CTG GGT A (SEQ ID NO:34)	<i>TP53</i> MDA REV #16	TTA ACC CCT C (SEQ ID NO:35)
<i>TP53</i> MDA FOR #17	GAG CCC AGG A (SEQ ID NO:36)	<i>TP53</i> MDA REV #17	AGG GCC ACT G (SEQ ID NO:37)
<i>TP53</i> MDA FOR #18	CCA AGG CAG G (SEQ ID NO:38)	<i>TP53</i> MDA REV #18	CCC CCC TAC T (SEQ ID NO:39)
<i>TP53</i> MDA FOR #19	TCC CAG CAC T (SEQ ID NO:40)	<i>TP53</i> MDA REV #19	TAG GGA GGT C (SEQ ID NO:41)
<i>TP53</i> MDA FOR #20	TTG GTG GCT C (SEQ ID NO:42)	<i>TP53</i> MDA REV #20	TTG CAC ATC T (SEQ ID NO:43)
<i>PTEN</i> MDA FOR #1	GTC CAG AGC C (SEQ ID NO:44)	<i>PTEN</i> MDA REV #1	GCA GCC GCA G (SEQ ID NO:45)
<i>PTEN</i> MDA FOR #2	AGC CGC CGC A (SEQ ID NO:46)	<i>PTEN</i> MDA REV #2	GAA CGT GGG A (SEQ ID NO:47)
<i>PTEN</i> MDA FOR #3	AGT CGC TGC A (SEQ ID NO:48)	<i>PTEN</i> MDA REV #3	TTC GCA TCC G (SEQ ID NO:49)
<i>PTEN</i> MDA FOR #4	TGC TGA GGA G (SEQ ID NO:50)	<i>PTEN</i> MDA REV #4	CTG ACC AGG G (SEQ ID NO:51)

<i>PTEN</i> MDA FOR #5	GCC GCT GCC A (SEQ ID NO:52)	<i>PTEN</i> MDA REV #5	CAC ACC CTA G (SEQ ID NO:53)
<i>PTEN</i> MDA FOR #6	CTT CTC CCC A (SEQ ID NO:54)	<i>PTEN</i> MDA REV #6	GCA ACC AGG C (SEQ ID NO:55)
<i>PTEN</i> MDA FOR #7	CCG TTC GGA G (SEQ ID NO:56)	<i>PTEN</i> MDA REV #7	CAA TCG GTG G (SEQ ID NO:57)
<i>PTEN</i> MDA FOR #8	GAG GCC GCC G (SEQ ID NO:58)	<i>PTEN</i> MDA REV #8	GGA AGA GAC C (SEQ ID NO:59)
<i>PTEN</i> MDA FOR #9	CCC CCG TGG C (SEQ ID NO:60)	<i>PTEN</i> MDA REV #9	CCG AGC TCG C (SEQ ID NO:61)
<i>PTEN</i> MDA FOR #10	CCC GTC CGC C (SEQ ID NO:62)	<i>PTEN</i> MDA REV #10	GCT CAA CCT C (SEQ ID NO:63)
<i>PTEN</i> MDA FOR #11	CCC GGG CCG G (SEQ ID NO:64)	<i>PTEN</i> MDA REV #11	GGG CCT AAG C (SEQ ID NO:65)
<i>PTEN</i> MDA FOR #12	GGC GGC GGC A (SEQ ID NO:66)	<i>PTEN</i> MDA REV #12	CGT GCA ACA C (SEQ ID NO:67)
<i>PTEN</i> MDA FOR #13	GCC TCC AAC A (SEQ ID NO:68)	<i>PTEN</i> MDA REV #13	GCA ACT CAG G (SEQ ID NO:69)
<i>PTEN</i> MDA FOR #14	CGC CGG AGA G (SEQ ID NO:70)	<i>PTEN</i> MDA REV #14	GCC CTC AAT G (SEQ ID NO:71)
<i>PTEN</i> MDA FOR #15	GTC GCC TGT C (SEQ ID NO:72)	<i>PTEN</i> MDA REV #15	CCC CAT AGG G (SEQ ID NO:73)
<i>PTEN</i> MDA FOR #16	GCT CCA GGG A (SEQ ID NO:74)	<i>PTEN</i> MDA REV #16	CTG GGA TCA G (SEQ ID NO:75)
<i>PTEN</i> MDA FOR #17	CGG CGG CCG C (SEQ ID NO:76)	<i>PTEN</i> MDA REV #17	CTG GCA TCA C (SEQ ID NO:77)
<i>PTEN</i> MDA FOR #18	GGG AGA AGC G (SEQ ID NO:78)	<i>PTEN</i> MDA REV #18	CGG TGA GCA G (SEQ ID NO:79)
<i>PTEN</i> MDA FOR #19	CAC CTC CCG C (SEQ ID NO:80)	<i>PTEN</i> MDA REV #19	TCA GAG GAC C (SEQ ID NO:81)
<i>PTEN</i> MDA FOR #20	AGG CGC GGC G (SEQ ID NO:82)	<i>PTEN</i> MDA REV #20	CCC CTC TTG C (SEQ ID NO:83)
<i>BRCA2</i> MDA FOR #1	CCT CAG TCA C (SEQ ID NO:84)	<i>BRCA2</i> MDA REV #1	GAC GTA CTG G (SEQ ID NO:85)
<i>BRCA2</i> MDA FOR #2	TCC AGC GCT T (SEQ ID NO:86)	<i>BRCA2</i> MDA REV #2	CCA CTA GAC G (SEQ ID NO:87)
<i>BRCA2</i> MDA FOR #3	GAT GGG ACT G (SEQ ID NO:88)	<i>BRCA2</i> MDA REV #3	AGG GGC CAG T (SEQ ID NO:89)
<i>BRCA2</i> MDA FOR #4	CCC ATC CTC A (SEQ ID NO:90)	<i>BRCA2</i> MDA REV #4	GGG GGT CCT A (SEQ ID NO:91)
<i>BRCA2</i> MDA FOR #5	TGG ACA GCA C (SEQ ID NO:92)	<i>BRCA2</i> MDA REV #5	CAC CAC GCC C (SEQ ID NO:93)
<i>BRCA2</i> MDA FOR #6	GGC TAG TGG C (SEQ ID NO:94)	<i>BRCA2</i> MDA REV #6	AAG TGC TGG G (SEQ ID NO:95)
<i>BRCA2</i> MDA FOR #7	ACT AGC CAC G (SEQ ID NO:96)	<i>BRCA2</i> MDA REV #7	TCC GCC CAC C (SEQ ID NO:97)
<i>BRCA2</i> MDA FOR #8	CTG GTT AGC G (SEQ ID NO:98)	<i>BRCA2</i> MDA REV #8	ACT TCT GGC C (SEQ ID NO:99)
<i>BRCA2</i> MDA FOR #9	CTC TGT CCC C (SEQ ID NO:100)	<i>BRCA2</i> MDA REV #9	GTT GGC CAG G (SEQ ID NO:101)
<i>BRCA2</i> MDA FOR #10	GCG GCG TTG G (SEQ ID NO:102)	<i>BRCA2</i> MDA REV #10	CAC GCA GCA C (SEQ ID NO:103)

<i>BRCA2</i> MDA FOR #11	TGC TGA TGG G (SEQ ID NO:104)	<i>BRCA2</i> MDA REV #11	GTA GCT GGG A (SEQ ID NO:105)
<i>BRCA2</i> MDA FOR #12	AAG CCC CTG G (SEQ ID NO:106)	<i>BRCA2</i> MDA REV #12	CTC CTG CCT C (SEQ ID NO:107)
<i>BRCA2</i> MDA FOR #13	GGG CAC GCT G (SEQ ID NO:108)	<i>BRCA2</i> MDA REV #13	CCT CCA GGG T (SEQ ID NO:109)
<i>BRCA2</i> MDA FOR #14	AGA TGA CGC C (SEQ ID NO:110)	<i>BRCA2</i> MDA REV #14	CTT GGC TCA C (SEQ ID NO:111)
<i>BRCA2</i> MDA FOR #15	CTT CCC TCC C (SEQ ID NO:112)	<i>BRCA2</i> MDA REV #15	TGG CCC AGG C (SEQ ID NO:113)
<i>BRCA2</i> MDA FOR #16	CCT TCA GCT C (SEQ ID NO:114)	<i>BRCA2</i> MDA REV #16	CAA CGT GAG G (SEQ ID NO:115)
<i>BRCA2</i> MDA FOR #17	GGC CCG GCC T (SEQ ID NO:116)	<i>BRCA2</i> MDA REV #17	GCG ACA TGG G (SEQ ID NO:117)
<i>BRCA2</i> MDA FOR #18	CTG GGT CTC C (SEQ ID NO:118)	<i>BRCA2</i> MDA REV #18	TCC ATG GTG G (SEQ ID NO:119)
<i>BRCA2</i> MDA FOR #19	CGA GCC CCG C (SEQ ID NO:120)	<i>BRCA2</i> MDA REV #19	CCA GTG GCT C (SEQ ID NO:121)
<i>BRCA2</i> MDA FOR #20	GCC CGA AGG C (SEQ ID NO:122)	<i>BRCA2</i> MDA REV #20	TGC TGC AAG G (SEQ ID NO:123)
PCR Primers			
Primer Name	Sequence		
<i>TP53</i> PCR FOR	ACT TTC AAC TCT GTC TCC TTC CTC TTC CTA (SEQ ID NO:124)		
<i>TP53</i> PCR REV	GGA CGC GGG TGC CG (SEQ ID NO:125)		
<i>PTEN</i> PCR FOR	AAG CGG CGG CAG AGC G (SEQ ID NO:126)		
<i>PTEN</i> PCR REV	TCT GGG AGC CTG TGG CTG AAG (SEQ ID NO:127)		
<i>BRCA2</i> PCR FOR	ATG CAT CCC TGT GTA AGT GCA TTT TGG (SEQ ID NO:128)		
<i>BRCA2</i> PCR REV	GCG TGT CTT AAA AAT TTC AAA AAA TGT TGG CCT CT (SEQ ID NO:129)		

Gene Sequencing:

[00109] The MDA product was verified by running the product on a 1% agarose gel, and staining the gel with SYBR Gold (Thermo Fisher Scientific). Since the product was around 10 kilobases (kb), a smaller product must be made to enable sequencing. Thus, a PCR amplification was performed using 10-60% of the MDA product. The PCR product was verified and purified using 8-10% polyacrylamide gel electrophoresis (PAGE) stained with ethidium bromide or SYBR Gold. To purify the PCR product for sequencing, the 130-nt band was cut from the gel, crushed, suspended in 3 M NaAc pH 6.2, and incubated at 37°C with mixing overnight. The gel pieces were removed from the sample, the sample underwent phenol-chloroform extraction and ethanol precipitation, and the DNA was resuspended in

DEPC water. This purified PCR product was sequenced via Sanger Sequencing, and the sequence was compared to the known wildtype gene.

Results and Discussion

5

Microchannel Design:

[00110] The assay presented here involves two main steps, cancer cell capture using aptamers and genomic DNA analysis. The ability to perform these two step easily all within one device would significantly reduce contamination and sample loss, which is important when developing an assay for rare cells. Therefore, the device was designed to have two intersecting orthogonal microchannels: the cell channel where cancer cells are captured, and the DNA channel where the gDNA from the captured cells is isolated (FIG. 3). The cell channel was 1 mm wide, and the DNA channel was 250 μm , 500 μm , or 1 mm wide. The depth of the channels was ~ 25 μm . The device also contained two micropillar arrays, one for cancer cell capture and one for gDNA isolation. The cell capture array was located at the intersection of the two microchannels, and consisted of pillars 50 μm in diameter. This array was rotated by 4° to maximize the contact between the cells and the channel surface containing the aptamers, thereby improving the capture efficiency.¹⁹ The DNA micropillar array was very similar to our previously-developed microarray for gDNA isolation.¹⁷ The array presented here consisted of 4×4 μm pillars spaced in a gradient that started with the pillars 10 μm apart and finished with them 7 μm apart. These small pillars placed in such a fine array caused the gDNA to become physically entangled and remain within the array even under flow, while allowing the cellular debris to flow out of the device. This is highly advantageous and enables multiple types of analysis to be performed on the same gDNA template.

[00111] To control the flow within the device, valves were needed at the inlets and outlets. An external 4-way L-type valve was used at the DNA channel inlet to not only control flow, but also eliminate most of the dead volume caused by the length of tubing needed to reach the syringe pump while the device is either observed under a microscope or is incubated using a hotplate. This is necessary because high initial flowrates cannot be used after the gDNA is isolated on the micropillar array, as there is a risk of losing some of the entangled gDNA under the high flow conditions. External 2-way shutoff valves were used at each of the outlets as well as the cell channel inlet to control the fluid flow. These types of valves were used because they do not disturb the fluid within the channels, whereas

controlling the flow using tubing clamps causes significant flow during the clamping process, which can disturb the captured cells. This device design and setup enables this assay to be performed easily by the user.

5 **HeLa and CAO V-3 Cell Capture and Genomic DNA Isolation:**

[00112] The target cells were suspended in PBS binding buffer and pumped through the device with aptamers immobilized on the surface of the cell capture region containing a pillar array. The cell capture was most efficient at a flowrate of 5 $\mu\text{L}/\text{min}$ when the cells were freshly trypsinized and the channel depth was $\sim 25\text{ }\mu\text{m}$. Several flowrates were tested ranging from 20 $\mu\text{L}/\text{min}$ down to 0.1 $\mu\text{L}/\text{min}$. At high flowrates ($>10\text{ }\mu\text{L}/\text{min}$), the linear velocity of the cells was very high and the cells did not bind to the aptamers on the surface easily. At low flowrates ($<5\text{ }\mu\text{L}/\text{min}$), the cells did bind to the aptamers, but the throughput was very low and there was increased non-specific adhesion of the cells to the device. Cells used from frozen stocks did not bind as readily, likely due to different surface compositions caused by the shock of a freeze/thaw cycle. With channels deeper than 25 μm , the cell capture took longer, since fewer collisions with the channel surface were likely occurring. To demonstrate using aptamers to specifically capture cancer cells within the microchannels, HeLa and CAO V-3 cancer cells were tested with and without aptamers immobilized on the surface, and Ect1/E6E7 and End1/E6E7 non-cancerous cells were tested with aptamers immobilized on the surface. FIG. 4A and FIG. 4B show the cell capture region without aptamers, and indicate that HeLa and CAO V-3 cells do not non-specifically adhere to the surface of the device. FIG. 4C and FIG. 4D show the cell capture region with aptamers immobilized, and demonstrate that Ect1/E6E7 and End1/E6E7 non-cancerous cells neither bind non-specifically to the device, nor bind to the aptamers. FIG. 4E and FIG. 4F show that HeLa and CAO V-3 cancer cells bind to aptamers immobilized within the cell capture region of the device. These results demonstrate the successful use of aptamers to specifically capture cancer cells.

[00113] After successfully capturing cancer cells within the cell capture region, the cells were lysed through the DNA channel. The cell contents flowed through the DNA micropillar array, and the gDNA was isolated on the pillars via physical entanglement. To verify that the gDNA was isolated and retained within the micropillar array, the gDNA was stained with YOYO-1 dye, and the results are shown in FIG. 5 for both HeLa and CAO V-3 cells. The gDNA from both types of cells was successfully isolated by the micropillar array

and remained within the microchannel after multiple hours of flow. This gDNA isolation technique has several advantages, including allowing the gDNA to be completely chemically available for any downstream reaction, and more importantly it enables the gDNA to be retained within the device even under flow. This enables multiple types of analyses to be performed on the same template gDNA, so a large amount of information can be gathered from a single small population of cells without necessitating substantial whole genome amplification, which can be biased and information can be lost.²⁰⁻²²

Specific Isothermal Amplification of Genes from gDNA:

[00114] With the gDNA isolated and retained within the micropillar array, several types of genetic analyses can be performed. Here, we demonstrated the amplification of specific genes to determine their nucleotide sequence and discover any genetic mutations. MDA, an isothermal amplification technique, was used to reduce the complexity and cost of the device and enable straightforward device operation, since thermocycling is not necessary. MDA uses many short primers and a strand-displacing DNA polymerase (ϕ 29) to make numerous copies of the template DNA isothermally. Whereas MDA is commonly used as a method for whole genome amplification,²³⁻²⁶ in this work we use MDA to amplify a specific gene from gDNA. To our knowledge, this is the first demonstration of using MDA to amplify a specific gene from gDNA. Forty 10-nt primers (20 forward and 20 reverse primers) were designed around regions of the *TP53*, *PTEN*, and *BRCA2* genes, which are commonly mutated genes in cervical and ovarian cancer.^{27,30} This modified MDA technique for amplifying these genes from gDNA was initially verified in benchtop experiments using purified HeLa and CAOV-3 gDNA. FIG.6A shows the successful amplification of *TP53* from purified HeLa gDNA. FIG. 8 shows the successful amplification of *PTEN* and *BRCA2* from purified CAOV-3 gDNA. Shorter gene fragments were also produced via PCR from these MDA products (FIG. 6B and FIG. 9).

[00115] The isolated gDNA from HeLa and CAOV-3 cells was first chemically denatured to create single stranded DNA (ssDNA). The DNA was then neutralized prior to the MDA reaction. Since the gDNA is entangled in the micropillar array, upon denaturation the two complimentary strands likely cannot diffuse and migrate away from each other as readily as they can in a bulk solution, so it is possible that some may rehybridize upon neutralization. This would prevent the MDA reaction from occurring efficiently. To reduce the likelihood of this occurring, the neutralization buffer was spiked with the MDA primers

allowing the primers to bind to the ssDNA before it rehybridizes. The MDA reaction solution containing additional primers and the DNA polymerase was pumped through the device and the amplification product was collected. The MDA product from HeLa and CAOV-3 cell gDNA was analyzed on an agarose gel, and FIG. 6C shows images of the gels after a successful MDA reaction. The MDA product DNA strands were around 10 kb in length, and this is because the ϕ 29 polymerase is known to extend for approximately 10 kb.^{28,29} To prepare the amplified gene sample for sequencing, it must be shortened to accommodate the sequencing technology. For Sanger sequencing, up to a few hundred bases can be sequenced. To create a shorter gene fragment from the HeLa and CAOV-3 MDA product, PCR was used to create 130-nt DNA strands, which were verified via PAGE (FIG. 6D). MDA is an advantageous technique to use not only because it is isothermal, but also because amplifying 10 kb strands allows large strands of gDNA to be amplified from cells. These strands can be completely sequenced inexpensively by performing a few PCRs to isolate different regions of the strand, and performing Sanger sequencing on these pure samples. Alternatively, the MDA product can be digested into shorter fragments and targeted next-generation sequencing can be performed.

Sequencing of the TP53 Gene Fragment:

[00116] The purified *TP53* gene fragments from HeLa and CAOV-3 cells were sequenced via Sanger sequencing. This sequencing technique was chosen because it is fast, inexpensive, and can perform longer reads than other techniques. It also requires the sample to be pure, as only one read is performed. The wildtype sequence for *TP53* was obtained from the International Agency for Research on Cancer, and the known mutation in the *TP53* gene in CAOV-3 cells was obtained from the mutation data for this cell line from ATCC. CAOV-3 cells contain a homozygous single-nucleotide polymorphism (SNP), and this SNP (c.406C>T) is a nonsense mutation resulting in a truncated p53 protein. FIG. 7 shows the wildtype and mutated nucleotide sequence and the sequencing results from HeLa (FIG. 7A) and CAOV-3 (FIG. 7B) cells for the region where the SNP occurred. These results show that we were able to successfully detect a point mutation in the CAOV-3 *TP53* gene, while HeLa cells contained the wildtype sequence of this gene fragment. Analogous testing of all locations on this gene would allow us to determine additional genetic information about this gene in these two cancer cell lines. Additional genes that commonly contain mutations in

cancer could also be tested in this way, since the gDNA is retained on the micropillars and is available for additional amplification reactions and analysis.

Conclusions

5 [00117] We have developed a device and technique for capturing cancer cells using aptamers, and isolating their gDNA for genetic analysis. The device was designed to enable both the cell capture and gDNA isolation to occur within a single device to significantly reduce contamination and sample loss. Preventing sample loss is particularly important, since
10 most cells of interest, such as circulating tumor cells, are rare and are generally found in low numbers. The device was also designed to isolate the gDNA via physical entanglement within a micropillar array. This isolation technique allows the gDNA to be chemically available for downstream reactions. It also enables the gDNA to be retained within the microchannel even under flow, which enables multiple types of analyses to be performed on the same template
15 gDNA.

[00118] We demonstrated on-chip isothermal amplification of a specific gene and subsequent sequencing of this gene to determine any genetic mutations. We successfully detected a point mutation in the *TP53* gene in CAOV-3 cells. Specifically, we developed a method using MDA to amplify a specific gene from whole gDNA. This technique allows for
20 long strands of DNA to be produced that can cover an entire large gene up to 10 kb. Here, we used PCR to produce pure samples of smaller gene fragments that could be sequenced using Sanger sequencing, but other sequencing methods can be used where pure samples are not necessary as multiple reads are taken.

[00119] An assay like this can be extremely impactful when it comes to cancer
25 diagnosis and treatment. If the mutations present in a specific patient's cancer cells can be identified, clinicians will be able to use this information to better diagnose the patient and better determine the most effective treatment options. This would truly enable precision medicine when it comes to cancer treatment, which is necessary to effectively treat patients considering the substantial diversity observed in cancer.

30 [00120] While we have described the application of our device primarily in terms of isolating and genetically analyzing cancer cells. The same device and approach can be applied to other improvements in bioanalytical applications. For example, the rapid identification of antibiotic resistant bacteria is of great importance for determining appropriate treatment in a timely manner. Our device could be employed to select by

aptamer binding a particular type of bacteria from body fluid or a swab sample and with even a single or a few cells rapid genetic analysis could determine the strain of the bacteria and its antibiotic resistance. This would be much more rapid than culturing cells to determine the effective antibiotic treatment. Another example would be for forensic analysis where human cells could be isolated from a complex sample and even a few cells genetically analyzed to identify the genetic fingerprint of the individual from whom the cells originate. There are numerous other examples to which our device and approach could be applied such as environmental monitoring for invasive organisms, analyzing drinking water safety or detecting rejections of human medical transplants where the rapid isolation of selected cell types and identification of specific genetic traits would be valuable.

[00121] Supplementary information is shown in FIGS. 8-12, with the descriptions being provided herein above in the Brief Description of the Drawings section.

Example 2

Various Embodiments of a Microfluidic Device for Aptamer-Based Cancer Cell Capture and Gene Mutation Detection

[00122] The microfluidic device of the present invention can be used for aptamer-based cell capture for various uses. This example illustrates one protocol for preparing one embodiment of a microfluidic device of the present invention. As shown, this example describes a protocol of the preparation process, starting with the PDMS device fabrication and continuing through to the on-chip specific multiple displacement amplification (MDA) reaction.

Surface Chemistry for HeLa Cell Capture in Microfluidic Devices

A. Fabrication of PDMS Devices

- For each wafer, mix 50g of PDMS base and 5g of curing agent thoroughly
- Degass the mixture completely in the vacuum oven
- Make an Al foil boat around the wafer and pour the PDMS onto the wafer
- Pop any bubbles that formed during the pouring process
- Put the samples in the oven at cure at 140C for >1h

Bonding the devices:

- Once cured, SLOWLY and carefully peel the PDMS off of the wafer to prevent the pillars from ripping off

- Cut out the devices individually to fit on a microscope slide and punch inlet and outlet holes using a 1-mm biopsy punch
- Wash the PDMS thoroughly with soap and tap water and then DI water
- Rinse the PDMS and a microscope slide thoroughly with 100% ethanol and DI water
- 5 • Dry the PDMS and slide with nitrogen and place immediately into the plasma cleaner
- Draw a vacuum on the plasma cleaner for about a minute and then turn the plasma on high
 - Adjust the door valve so that the plasma is a pink color (a blueish plasma means there is not enough oxygen)
- 10 • Plasma treat for 10min
- Immediately take out the PDMS and slide and bond them, but do not push too hard as the channels can collapse
- Cover the inlet and outlet holes with tape to prevent debris from entering the device

15 **B. Cleaning the device**

To avoid having to clean with acid and base, use a device that has been bonded within 48 hours.

- 20 With a device bonded within the last 48 hours,
- Connect tubing to all inlets and outlets, and connect valves to all inlets and outlets
 - The valves at the inlets should have a third connection that allows dead volume to be pumped out into waste
 - Fill 2 1-mL syringes for each device with ethanol and connect them to both inlet valves
 - 25 • With the valves set to flow out to waste, pump 100 μ L of ethanol through at 100 μ L/min to flush out any bubbles
 - Set the valves to flow into the device and then flow 900 μ L through both inlets at 30 μ L/min
 - 30 • Fill a 1-mL syringe with ultrapure water
 - With the valves set to flow out to waste, pump 100 μ L of water through the cell channel inlet valve at 100 μ L/min to flush out any bubbles
 - Set the valve to flow into the device and then flow 1 mL of water through the cell channel at 50 μ L/min
 - 35 • Repeat this for the DNA channel
 - Fill a 1-mL syringe with filter-sterilized 1x PBS
 - With the valves set to flow out to waste, pump 100 μ L of PBS through the cell channel inlet valve at 100 μ L/min to flush out any bubbles
 - Set the valve to flow into the device and then flow 450 μ L of water through the cell channel at 50 μ L/min
 - 40 • Repeat this for the DNA channel

C. Surface Chemistry for Immobilizing Aptamers

- Fill a 1-mL syringe with ~200 μ L of 1mg/mL streptavidin
- 5 • With the valves set to flow out to waste, pump ~60 μ L of streptavidin through the cell channel inlet valve at 80 μ L/min to flush out any bubbles (stop flowing once bubbles are flushed out and the fluid stream can be seen in the waste tubing past the valve)
- Set the valve to flow into the device and then flow 90 μ L of streptavidin through the cell channel inlet at 3 μ L/min, and then incubate for 10-15mins
- 10 • Fill a 1-mL syringe with a blocking solution of 1% BSA, 1% Pluronic F-68, and 1% polyvinylpyrrolidone (PVP) K15 in PBS binding buffer (1xDPBS with Mg and Ca, 4.5g/L glucose, and 5mM MgCl₂)
- With the valves set to flow out to waste, pump 80 μ L of blocking solution through the cell channel inlet valve at 80 μ L/min to flush out any bubbles
- Set the valve to flow into the device and then flow 500 μ L of blocking solution
- 15 through the cell channel inlet at 4 μ L/min
- Repeat for the DNA channel
- Prepare an aptamer solution by combining 3 μ L of 1mM biotinylated DOV4 aptamer with 297 μ L of PBS binding buffer
 - Incubate this aptamer solution at 75°C for 5mins then allow to cool to RT
- 20 • Fill a 1-mL syringe with this solution
- With the valves set to flow out to waste, pump ~60 μ L of aptamer solution through the DNA channel inlet valve at 80 μ L/min to flush out any bubbles (stop flowing once bubbles are flushed out and the fluid stream can be seen in the waste tubing past the valve)
- 25 • Set the valve to flow into the device and then flow 180 μ L of aptamer solution through the DNA channel inlet at 3 μ L/min

D. Preparing the HeLa cells

- 30 From culture:
- Passage the cells as usual, but resuspend one pellet with 3mL PBS binding buffer containing no DMSO
 - This can be used directly
- From frozen:
- 35 • Thaw quickly an aliquot of cells in a 37°C waterbath and transfer the cells to a falcon tube. Add 9mL of PBS binding buffer and spin down the solution at 100xg for 5mins
- Take out supernatant and resuspend in 3mL of PBS binding buffer
 - Repeat this washing 3 times to remove all of the DMSO
 - Resuspend the cells in 1mL of PBS binding buffer and use directly in the device

40

E. Capturing and Lysing HeLa cells

- Fill a 1-mL syringe with HeLa cell suspension
- 5 • With the valves set to flow out to waste, pump 80µL of cell suspension through the cell channel inlet valve at 10µL/min to flush out any bubbles
- Set the valve to flow into the device and then flow cells at 1µL/min and monitor capture using a fluorescence microscope (the HeLa cells have green fluorescent protein on their histones that enables them to fluoresce)
- 10 • Once cells are captured, close the cell channel valves
- Fill a 1-mL syringe with ~200µL of 6M guanidinium thiocyanate in ultrapure water (this is the lysis solution)
- With the valves set to flow out to waste, pump 80µL of the solution through the DNA channel inlet valve at 80µL/min to flush out any bubbles
- 15 • Set the valve to flow into the device and then flow solution at 1µL/min and monitor lysis using a fluorescence microscope (look for disappearance of fluorescent whole cells)

F. Performing Specific MDA Reaction

- 20 • Flush out the lysis solution with 1x TE: Fill a 1-mL syringe with ~200µL of 1x TE
- With the valves set to flow out to waste, pump 80µL of the solution through the DNA channel inlet valve at 80µL/min to flush out any bubbles
- Set the valve to flow into the device and then flow 60µL of solution at 1µL/min
- Use the REPLI-g Mitochondrial DNA kit to provide the buffer and enzymes for the MDA reaction
- 25 • Prepare the D1 denaturing buffer:
 - 54µL Reconstituted Buffer DLB
 - 192µL ultrapure Water
- Fill a 1-mL syringe with D1 solution
- With the valves set to flow out to waste, pump 80µL of the solution through the DNA channel inlet valve at 80µL/min to flush out any bubbles
- 30 • Set the valve to flow into the device and then flow 25µL of solution at 1µL/min
- Prepare the N1 Neutralizing Buffer
 - 36µL Stop Solution
 - 24µL MDA primer mix for the gene of interest
 - 35 ○ 180µL ultrapure water
- Fill a 1-mL syringe with N1 solution
- With the valves set to flow out to waste, pump 80µL of the solution through the DNA channel inlet valve at 80µL/min to flush out any bubbles
- Set the valve to flow into the device and then flow 45µL of solution at 1µL/min
- 40 • Setup the device on a hotplate set to 3°C
- Setup a humidity chamber around the device to prevent evaporation
- Prepare the MDA master mix
 - 75µL ultrapure water
 - 24µL MDA primer mix
 - 45 ○ 121.5µL REPLI-g reaction buffer

- 4.5μL DNA polymerase
- Fill a 1-mL syringe with MDA reaction mix
- With the valves set to flow out to waste, pump the solution through the DNA channel inlet valve at 80μL/min to flush out any bubbles, and stop flowing once bubbles are flushed out and the fluid stream can be seen in the waste tubing past the valve
- Set the valve to flow into the device and then flow 50uL of solution at 0.05uL/min and collect eluent in an Eppendorf tube

REFERENCES

- 10 [00123] Citation of a reference herein shall not be construed as an admission that such reference is prior art to the present invention. All references cited herein are hereby incorporated by reference in their entirety. Below is a listing of various references cited herein by Reference (Ref.) number:
- 15 1 K. Vermeulen, D. R. Van Bockstaele and Z. N. Berneman, *Cell Prolif.*, 2003, **36**, 131–149.
 - 2 B. Vogelstein and K. W. Kinzler, *Nat. Med.*, 2004, **10**, 789–799.
 - 3 L. Coin, M. Marshall, T. Down, T. Hubbard, R. Wooster, N. Rahman and M. R. Stratton, *Nat. Rev. Cancer*, 2004, **4**, 177–183.
 - 20 4 P. C. Nowell, *Science*, 1976, **194**, 23–28.
 - 5 C. G. Mullighan, S. Goorha, I. Radtke, C. B. Miller, E. Coustan-Smith, J. D. Dalton, K. Girtman, S. Mathew, J. Ma, S. B. Pounds, X. Su, C.-H. Pui, M. V Relling, W. E. Evans, S. A. Shurtleff and J. R. Downing, *Nature*, 2007, **446**, 758–64.
 - 25 6 A. Didelot, D. Le Corre, A. Luscan, A. Cazes, K. Pallier, J. F. Emile, P. Laurent-Puig and H. Blons, *Exp. Mol. Pathol.*, 2012, **92**, 275–280.
 - 7 M. N. Nikiforova, A. I. Wald, S. Roy, M. B. Durso and Y. E. Nikiforov, *J. Clin. Endocrinol. Metab.*, 2013, **98**, 1852–1860.
 - 8 G. Ellison, G. Zhu, A. Moulis, S. Dearden, G. Speake and R. McCormack, *J. Clin. Pathol.*, 2013, **66**, 79–89.
 - 30 9 P. N. Gray, C. L. M. Dunlop and A. M. Elliott, *Cancers*, 2015, **7**, 1313–1332.
 - 10 D. T. Cheng, T. N. Mitchell, A. Zehir, R. H. Shah, R. Benayed, A. Syed, R. Chandramohan, Z. Y. Liu, H. H. Won, S. N. Scott, A. Rose Brannon, C. O'Reilly, J. Sadowska, J. Casanova, A. Yannes, J. F. Hechtman, J. Yao, W. Song, D. S. Ross, A. Oultache, S. Dogan, L. Borsu, M. Hameed, K. Nafa, M. E. Arcila, M. Ladanyi and M. F. Berger, *J. Mol. Diagnostics*, 2015, **17**, 251–264.
 - 35

- 11 Y. Wan, Y. L. Liu, P. B. Allen, W. Asghar, M. A. I. Mahmood, J. F. Tan, H. Duhon, Y. T. Kim, A. D. Ellington and S. M. Iqbal, *Lab Chip*, 2012, **12**, 4693–4701.
- 12 J. A. Phillips, Y. Xu, Z. Xia, Z. H. Fan and W. Tan, *Anal. Chem.*, 2009, **81**, 1033–1039.
- 13 F. Zheng, Y. Cheng, J. Wang, J. Lu, B. Zhang, Y. Zhao and Z. Gu, *Adv. Mater.*, 2014, **26**, 7333–7338.
- 14 Y. Xu, J. A. Phillips, J. Yan, Q. Li, Z. H. Fan and W. Tan, *Anal. Chem.*, 2009, **81**, 7436–7442.
- 15 W. Sheng, T. Chen, R. Kamath, X. Xiong, W. Tan and Z. H. Fan, *Anal. Chem.*, 2012, **84**, 4199–4206.
- 10 16 Q. Shen, L. Xu, L. Zhao, D. Wu, Y. Fan, Y. Zhou, W. H. Ouyang, X. Xu, Z. Zhang, M. Song, T. Lee, M. A. Garcia, B. Xiong, S. Hou, H. R. Tseng and X. Fang, *Adv. Mater.*, 2013, **25**, 2368–2373.
- 17 J. J. Benítez, J. Topolancik, H. C. Tian, C. B. Wallin, D. R. Latulippe, K. Szeto, P. J. Murphy, B. R. Cipriany, S. L. Levy, P. D. Soloway and H. G. Craighead, *Lab Chip*, 2012, **12**, 4848.
- 15 18 D. Van Simaey, D. López-Colón, K. Sefah, R. Sutphen, E. Jimenez and W. Tan, *PLoS One*, 2010, **5**, e13770.
- 19 J. P. Gleghorn, E. D. Pratt, D. Denning, H. Liu, N. H. Bander, S. T. Tagawa, D. M. Nanus, P. A. Giannakakou and B. J. Kirby, *Lab Chip*, 2010, **10**, 27–29.
- 20 20 R. Pinard, A. de Winter, G. J. Sarkis, M. B. Gerstein, K. R. Tartaro, R. N. Plant, M. Egholm, J. M. Rothberg and J. H. Leamon, *BMC Genomics*, 2006, **7**, 216.
- 21 C.-Z. Zhang, V. A. Adalsteinsson, J. Francis, H. Cornils, J. Jung, C. Maire, K. L. Ligon, M. Meyerson and J. C. Love, *Nat. Commun.*, 2015, **6**, 1–10.
- 22 J. Sabina and J. H. Leamon, in *Whole Genome Amplification*, ed. T. Kroneis, Springer, New York, 2015, vol. 1347, pp. 15–41.
- 25 23 F. B. Dean, S. Hosono, L. Fang, X. Wu, A. F. Faruqi, P. Bray-Ward, Z. Sun, Q. Zong, Y. Du, J. Du, M. Driscoll, W. Song, S. F. Kingsmore, M. Egholm and R. S. Lasken, *Proc. Natl. Acad. Sci. U. S. A.*, 2002, **99**, 5261–6.
- 24 C. Spits, C. Le Caignec, M. De Rycke, L. Van Haute, A. Van Steirteghem, I. Liebaers and K. Sermon, *Nat. Protoc.*, 2006, **1**, 1965–1970.
- 30 25 J. G. Paez, M. Lin, R. Beroukhi, J. C. Lee, X. Zhao, D. J. Richter, S. Gabriel, P. Herman, H. Sasaki, D. Altshuler, C. Li, M. Meyerson and W. R. Sellers, *Nucleic Acids Res.*, 2004, **32**, e71.
- 26 S. H. L. Mandey, M. S. Schneiders, J. Å. Koster and H. R. Waterham, *Hum. Mutat.*, 2006, **27**, 796–802.
- 35

- 27 M. Hollstein, K. Rice, M. S. Greenblatt, T. Soussi, R. Fuchs, T. Sorlie, E. Hovig, B.
Smith-Sørensen, R. Montesano and C. C. Harris, *Nucleic Acids Res.*, 1994, **22**, 3551–
5.
- 28 S. J. Foster and B. J. Monahan, *Fungal Genet. Biol.*, 2005, **42**, 367–375.
- 5 29 O. Alsmadi, F. Alkayal, D. Monies and B. F. Meyer, *BMC Res. Notes*, 2009, **2**, 48.
- 30 R. Kurman and I. Shih, *Int. J. Gynecol. Pathol.*, 2008, **27**, 151–160.

[00124] Although the present invention has been described for the purpose of
illustration, it is understood that such detail is solely for that purpose and variations can be
10 made by those skilled in the art without departing from the spirit and scope of the invention
which is defined by the following claims.

WHAT IS CLAIMED IS:

1. A microfluidic device comprising:
a cell microchannel and a nucleic acid microchannel that intersect to form a
5 cell capture intersection region;
a cell capture array comprising a plurality of cell capturing micropillars
configured and arranged in a manner effective to capture one or more target cell when flowed
through the cell microchannel, said cell capture array being located in the cell capture
intersection region; and
10 a nucleic acid entanglement array comprising a plurality of nucleic acid
entanglement micropillars configured and arranged in a manner effective to physically
entangle and maintain thereon genomic DNA isolated from the one or more target cell, said
nucleic acid entanglement array being located in a portion of the nucleic acid microchannel
that is adjacent to and downstream of the cell capture intersection region,
15 wherein said microfluidic device is multi-functional in that it is effective for
capturing said one or more target cell, isolating said genomic DNA from the one or more
target cell, and analyzing said genomic DNA in a self-contained manner.
2. The microfluidic device according to claim 1, wherein said cell capture
20 array comprises one or more aptamer and/or another cell capture component specific to the
one or more target cell.
3. The microfluidic device according to claim 2, wherein the one or more
aptamer and/or another cell capture component is concentrated in the cell capture intersection
25 region, thereby enabling capture of the one or more target cell.
4. The microfluidic device according to claim 1, wherein said nucleic
acid entanglement array is effective to entangle and maintain the isolated genomic DNA for
single amplification and/or multiple, consecutive amplifications of one or more nucleic acid
30 sequence of interest contained on the isolated genomic DNA.
5. The microfluidic device according to claim 4, wherein the one or more
nucleic acid sequence of interest is a cancer gene.

6. The microfluidic device according to claim 1, wherein the one or more target cell is a cancer cell.

5 7. The microfluidic device according to claim 1 further comprising:
a first flow rate means for managing rate of flow of fluid through the cell microchannel and a second flow rate means for managing rate of flow of fluid through the nucleic acid microchannel.

10 8. The microfluidic device according to claim 7, wherein the first flow rate means comprises external valves at the nucleic acid microchannel inlet and outlet and the second flow rate means comprises external valves at the cell microchannel inlet and outlet.

15 9. The microfluidic device according to claim 8, wherein the external valves are selected from the group consisting of two-way valves and four-way valves.

10. The microfluidic device according to claim 1 further comprising:
a temperature controller for managing temperature of fluid and other contents contained within the cell microchannel and/or nucleic acid microchannel.

20 11. The microfluidic device according to claim 1, wherein the cell microchannel and the nucleic acid microchannel have a height ranging from between about 20 μm and about 40 μm .

25 12. The microfluidic device according to claim 1, wherein the cell microchannel and the nucleic acid microchannel have a height of about 25 μm .

13. The microfluidic device according to claim 1, wherein the cell channel has a width ranging from between about 500 μm and about 1500 μm .

30 14. The microfluidic device according to claim 1, wherein the cell channel has a width of about 1000 μm .

15. The microfluidic device according to claim 1, wherein the nucleic acid channel has a width ranging from between about 200 μm and about 1500 μm .

16. The microfluidic device according to claim 1, wherein the nucleic acid
5 channel has a width selected from the group consisting of about 250 μm , 500 μm , and 1000 μm .

17. The microfluidic device according to claim 1, wherein the cell
10 capturing micropillars have a diameter ranging from between about 40 μm and about 60 μm .

18. The microfluidic device according to claim 1, wherein the cell capturing micropillars have a diameter of 50 μm .

19. The microfluidic device according to claim 1, wherein the cell capture
15 array is ordered in a patterned array that is rotated by about 4° to maximize contact between the one or more target cell and microchannel surface.

20. The microfluidic device according to claim 1, wherein the nucleic acid entanglement micropillars have a diameter ranging from between about 2 μm and about 10
20 μm .

21. The microfluidic device according to claim 1, wherein the nucleic acid entanglement micropillars have a cross-sectional dimension of about 4 μm x 4 μm , wherein said nucleic acid entanglement micropillars are spaced in a gradient that begins with the
25 micropillars being about 10 μm apart and ending with the micropillars being about 7 μm apart.

22. A method of isolating and maintaining genomic DNA of one or more target cell from a sample under flow for further analysis thereof, said method comprising the
30 steps of:

providing a microfluidic device according to any one of claims 1-21;
introducing a sample comprising one or more target cell into the cell microchannel at a flow rate effective to transport the one or more target cell to the cell

capture array so as to capture the one or more target cell in the cell capturing micropillars by specific binding;

lysing the one or more target cell by introducing lysing reagents through the nucleic acid microchannel at a flow rate effective to release genomic DNA from the one or more target cell without shearing the genomic DNA; and

maintaining fluid flow within the nucleic acid microchannel at a flow rate effective to cause the released genomic DNA to become physically entangled and maintained within the nucleic acid entanglement array for further analysis thereof.

23. The method according to claim 22, wherein the one or more target cell is captured in the cell capture array due to specific contact with an aptamer or other capture component present in the cell capture array.

24. The method according to claim 22, wherein the one or more target cell is introduced into the cell microchannel and thereafter captured within the cell capture array under a flow rate ranging from between about 0.1 $\mu\text{L}/\text{minute}$ and about 20 $\mu\text{L}/\text{minute}$.

25. The method according to claim 22, wherein the lysing reagents are introduced through the nucleic acid microchannel at a flow rate ranging from between about 0.1 $\mu\text{L}/\text{minute}$ and about 2 $\mu\text{L}/\text{minute}$, thereby causing the release of the genomic DNA from the one or more target cell without shearing the genomic DNA.

26. The method according to claim 25, wherein the flow of fluid in the nucleic acid microchannel is maintained at a flow rate ranging from between about 0.05 $\mu\text{L}/\text{minute}$ and about 2 $\mu\text{L}/\text{minute}$, thereby causing the released genomic DNA to become physically entangled and maintained within the nucleic acid entanglement array.

27. The method according to claim 22, wherein the one or more target cell is a cancer cell.

28. A method for conducting aptamer-based cancer cell capture and genomic DNA mutation analysis of genomic DNA isolated from one or more target cell, said method comprising the steps of:

performing the steps of the method according to claim 22; and
conducting aptamer-based cancer cell capture and genomic DNA mutation
analysis of the genomic DNA isolated from one or more target cell while in a flow
environment within the microfluidic device.

5

29. A method for amplifying individual genes of interest from the one or
more target cell consecutively and collecting each amplification product separately, said
method comprising the steps of:

performing the steps of the method according to claim 22; and
10 amplifying individual genes of interest from the genomic DNA entangled and
maintained under flow within the nucleic acid entanglement array of the microfluidic device
consecutively and collecting each amplification product separately.

30. A method for sequencing nucleic acids amplified from genomic DNA
15 isolated from one or more target cell, said method comprising the steps of:
performing the steps of the method according to claim 22; and
sequencing the genomic DNA entangled and maintained under flow within the
nucleic acid entanglement array of the microfluidic device.

20 31. A method for multiple displacement amplification (MDA) reactions of
one or more nucleic acid sequence isolated from one or more target cell, said method
comprising the steps of:
performing the steps of the method according to claim 22; and
conducting multiple displacement amplification (MDA) reactions under flow
25 using the genomic DNA entangled and maintained within the nucleic acid entanglement array
of the microfluidic device.

32. The method according to claim 31, wherein said MDA reactions
involve using the same genomic DNA template isolated by the nucleic acid entanglement
30 micropillars of the microfluidic device.


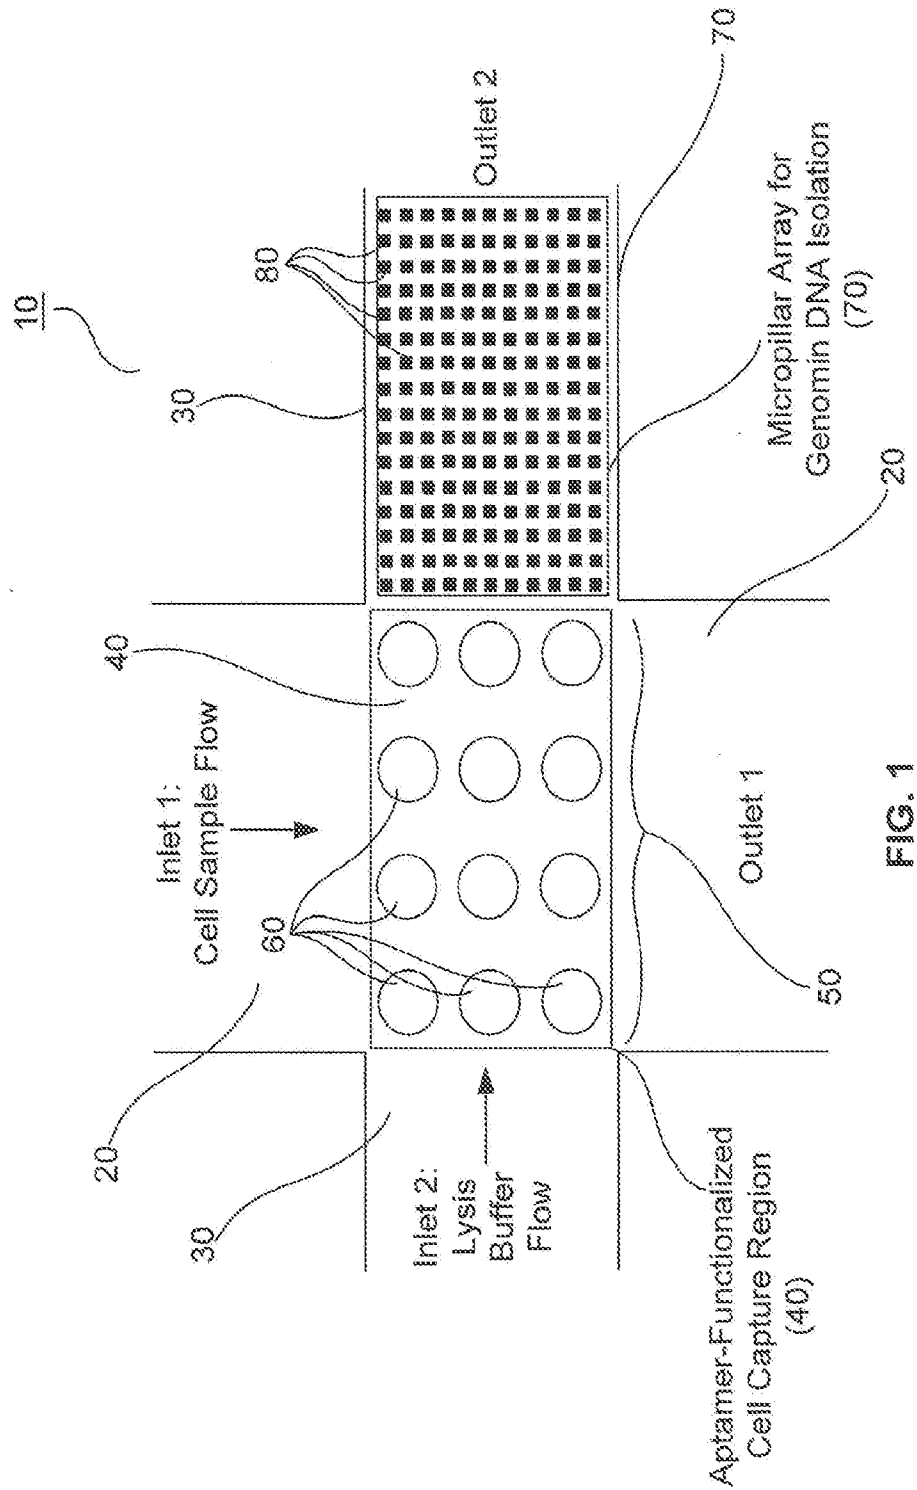


FIG. 1

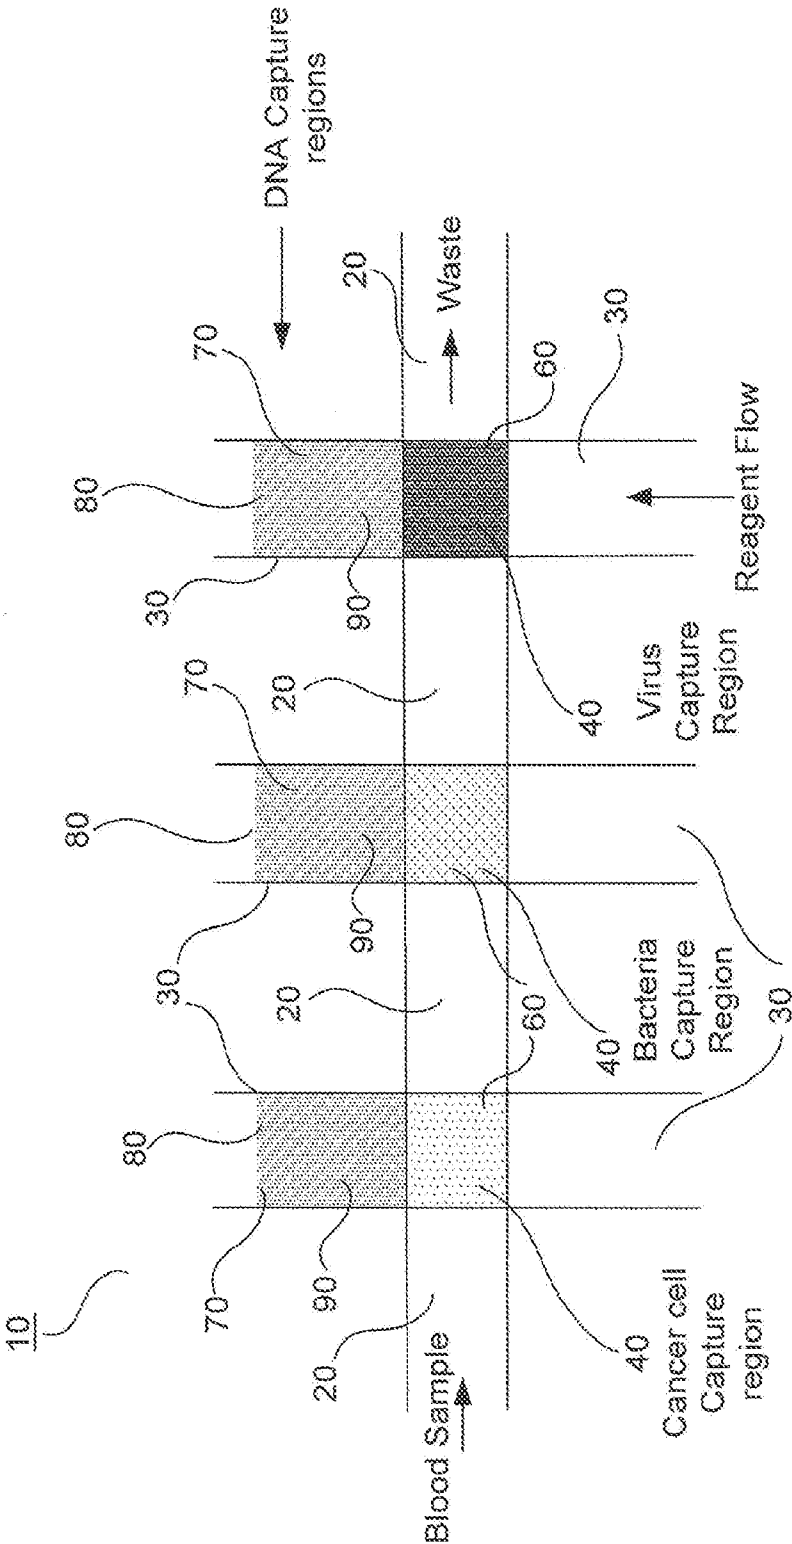

Schematic of microfluidic channels for capture of different
Biological components from a sample

FIG. 2

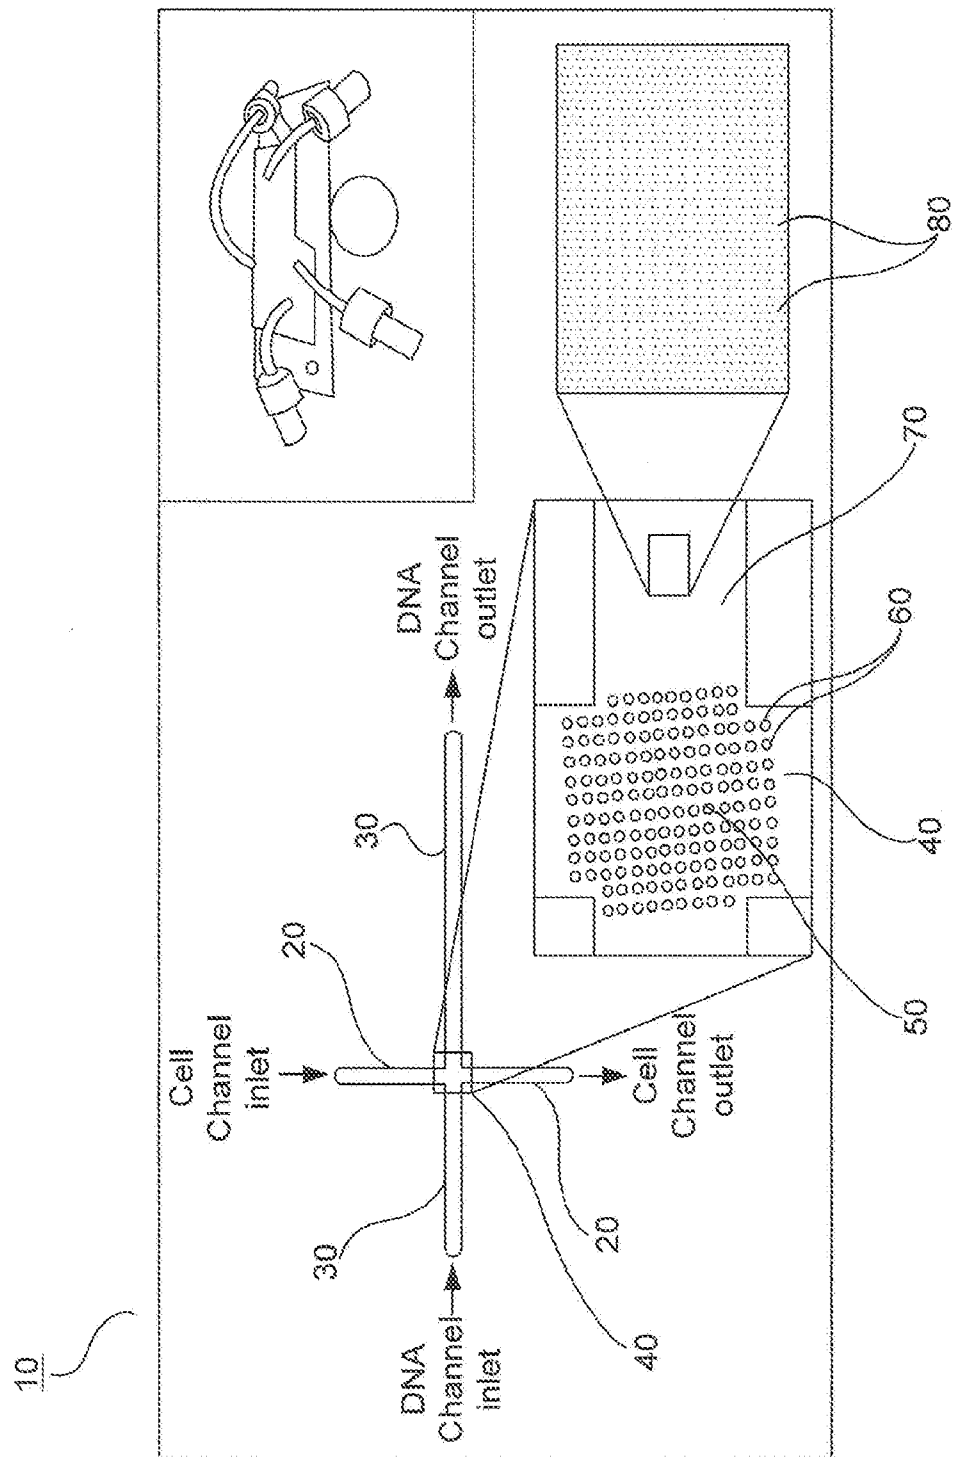


FIG. 3

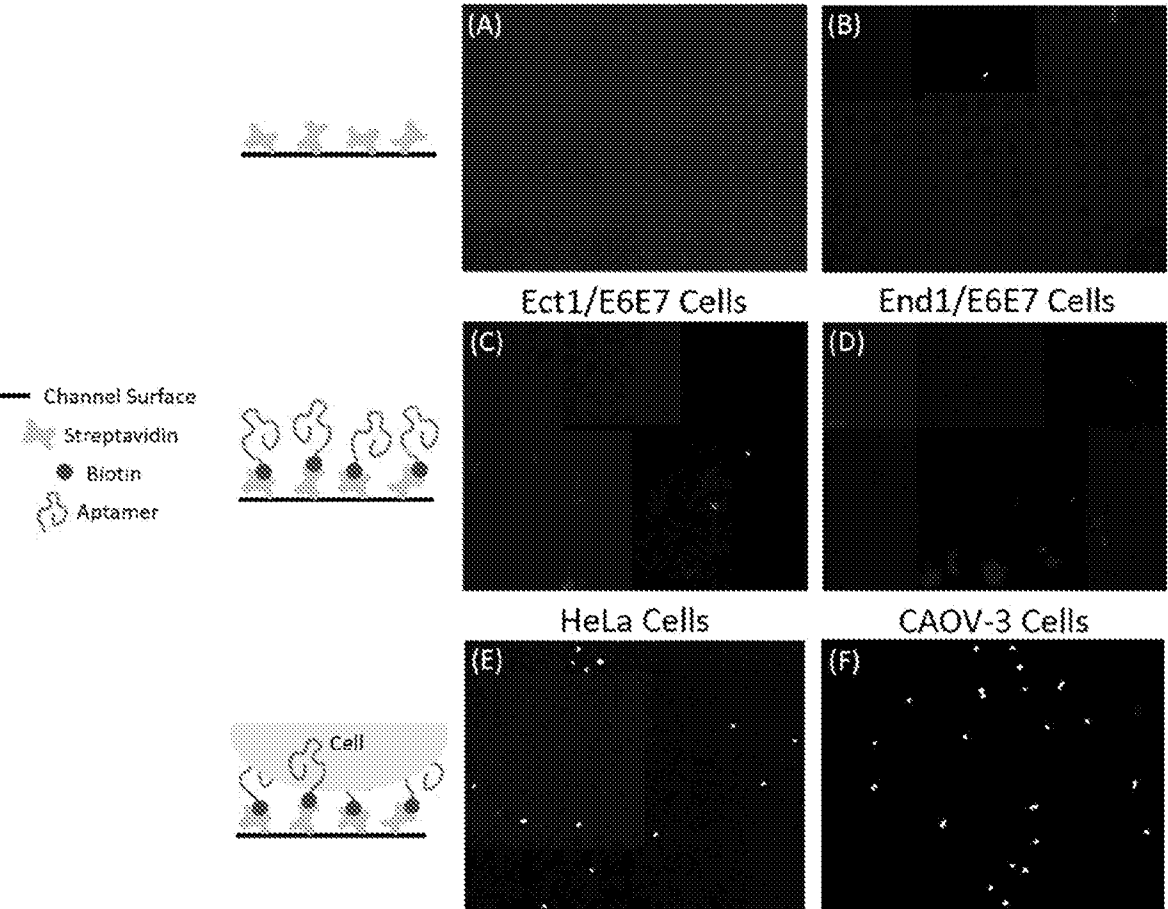


FIG. 4

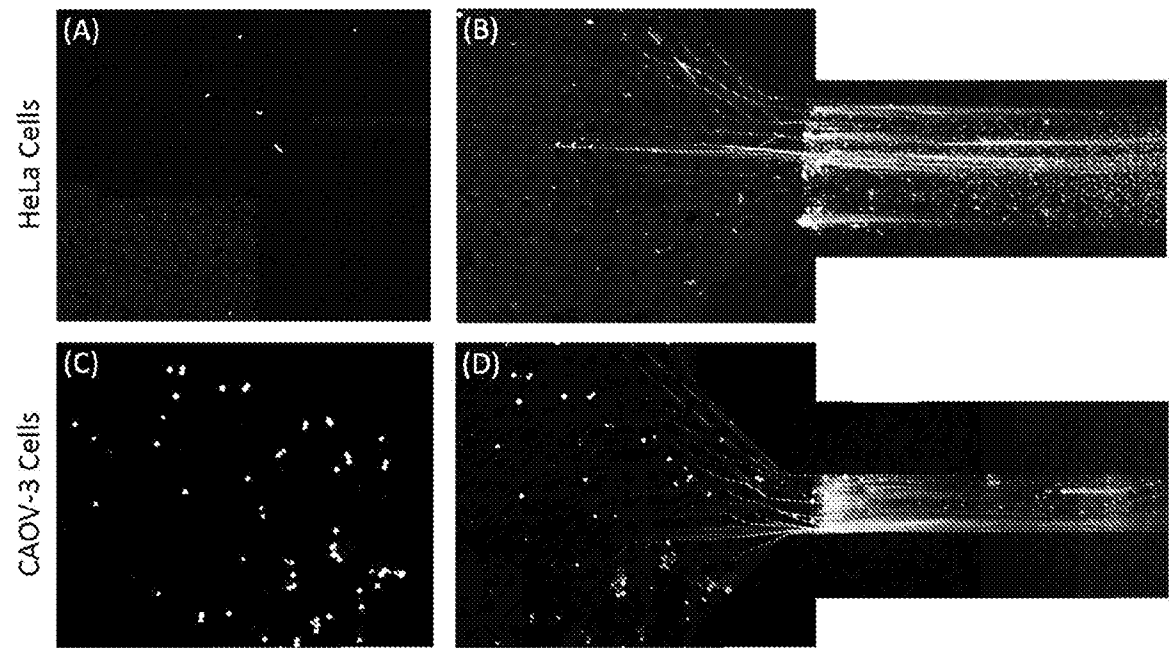


FIG. 5

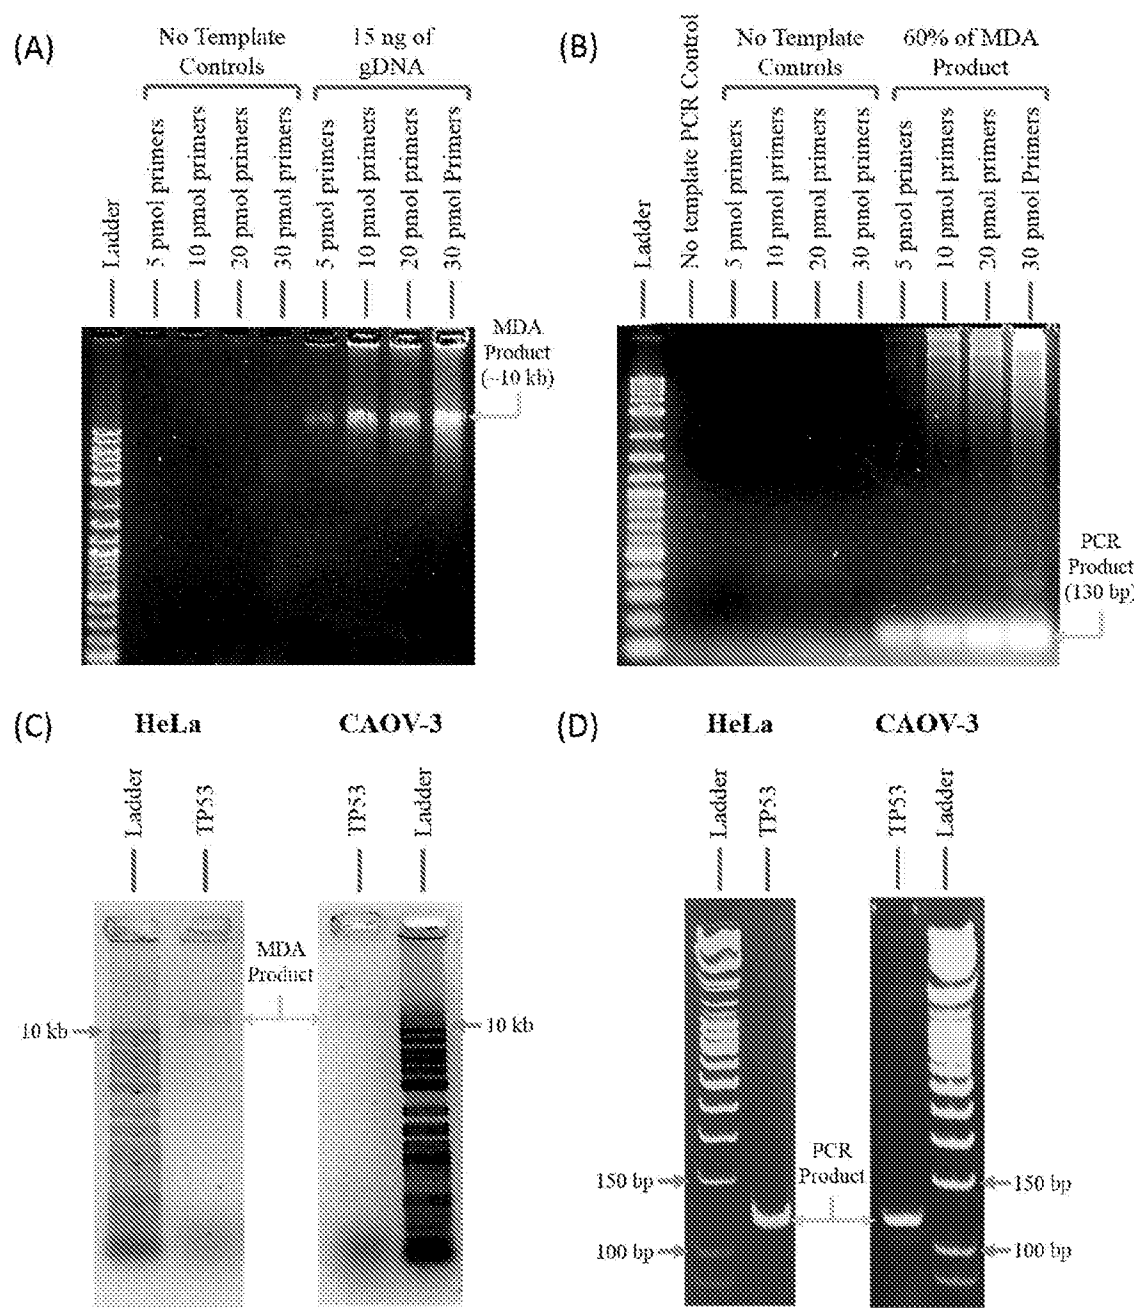


FIG. 6

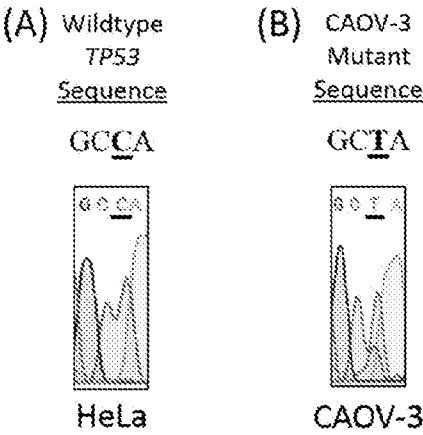


FIG. 7

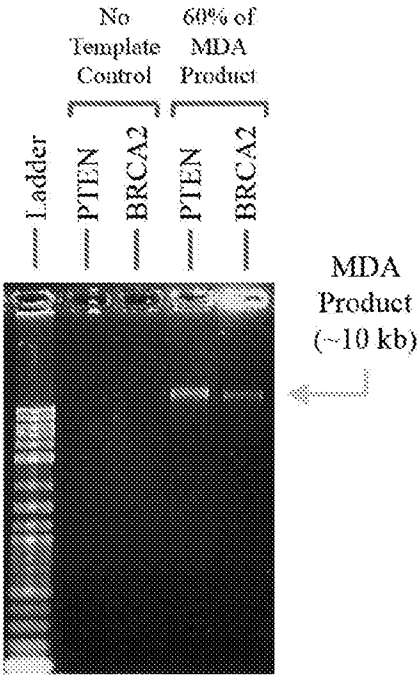


FIG. 8

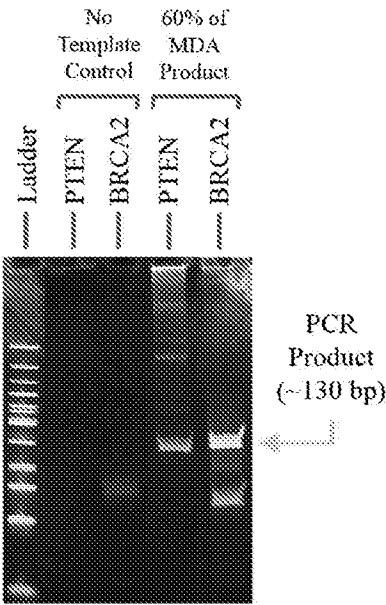


FIG. 9

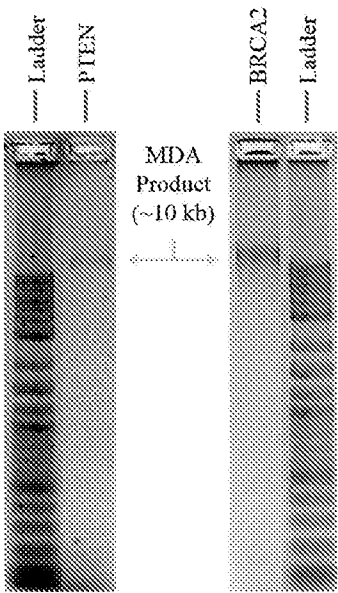


FIG. 10

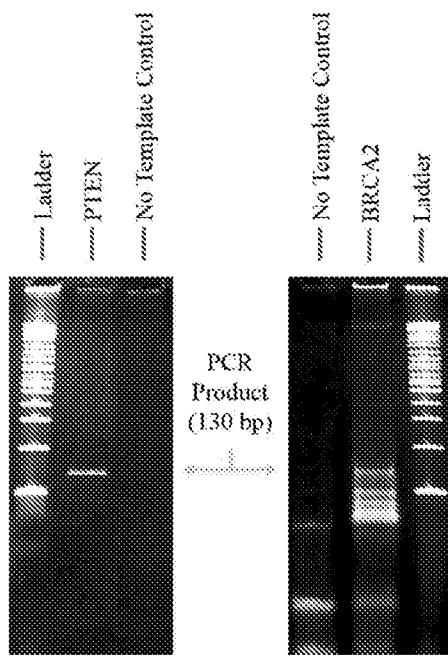


FIG. 11

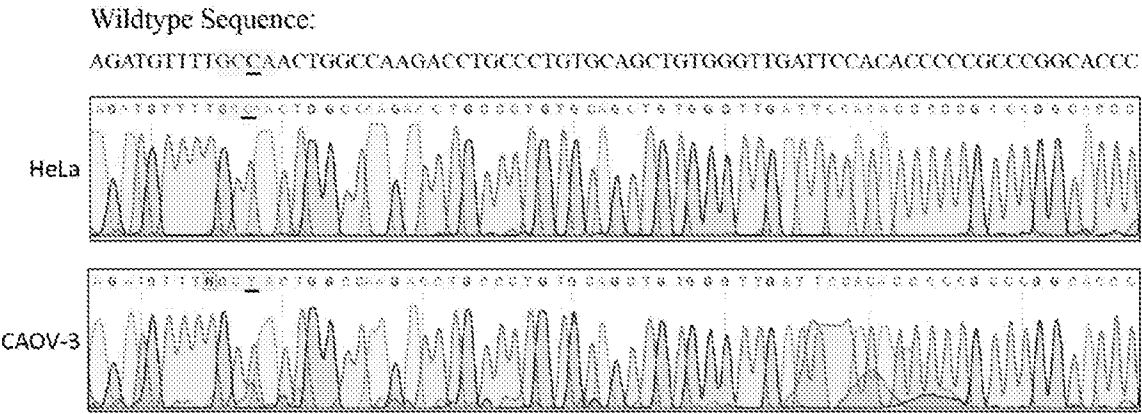


FIG. 12

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 17/33789

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - G01N 27/27, A61B 5/00, G01N 33/487 (2017.01)

CPC - B03C 5/005, A61B 5/00, C12Q 1/6886, C12Q 1/6883

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History Document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History Document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History Document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2014/0194313 A1 (Craighead et al.) 10 July 2014 (10.07.2014); abstract; FIG. 1, 10; para [0011]-[0012], [0027], [0048], [0060], [0065], [0079], [0102], [0109], [0121], [0125]	1-32
Y	US 2012/0091235 A1 (Li et al.) 19 April 2012 (19.04.2012); FIG. 4; para [0014], [0042], [0055]	1-32
Y	US 2015/0099642 A1 (Barany et al.) 09 April 2015 (09.04.2015); abstract; para [0005], [0180], [0184], [0213], [0239], [0256]; FIG. 11, 34	29-30
Y	US 2008/0124779 A1 (Oh et al.) 29 May 2008 (29.05.2008); para [0018], [0123], [0140], [0145]	31-32
A	US 2014/0154703 A1 (Skelley et al.) 06 June 2014 (06.06.2014); para [0159]	19
A	US 6,977,148 B2 (Dean et al.) 20 December 2005 (20.12.2005); abstract; col 2, ln 32-38	31-32

☐ Further documents are listed in the continuation of Box C.

☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

24 July 2017

Date of mailing of the international search report

29 AUG 2017

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774