



- (51) **International Patent Classification:**
A61C 9/00 (2006.01) *A61B 6/14* (2006.01)
- (21) **International Application Number:**
PCT/IL2016/050023
- (22) **International Filing Date:**
7 January 2016 (07.01.2016)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
62/100,920 8 January 2015 (08.01.2015) US
- (71) **Applicant:** DENTLYTEC G.P.L. LTD [IL/IL]; 14 Mintz Street, 6951217 Tel-Aviv (IL).
- (72) **Inventors:** PESACH, Benny; 18 Shir HaShirim Street, 4807209 Rosh HaAyin (IL). MELAMED, Georgy; 10 HaRishonim Street, Apt. 8, 5250214 Ramat-Gan (IL). LEHR, Blanc Zach; 6 Zeev Rechter Street, Apt. 20, 6955106 Tel-Aviv (IL). GRAD, Ygael; 14 Mintz Street, 6951217 Tel-Aviv (IL).
- (74) **Agents:** EHRLICH, Gal et al.; G.E. Ehrlich (1995) Ltd., 11 Menachem Begin Road, 5268104 Ramat Gan (IL).
- (81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— *of inventorship (Rule 4.17(iv))*

Published:

— *with international search report (Art. 21(3))*

- (54) **Title:** SYSTEM, DEVICE, AND METHOD FOR IMPROVED INTRAORAL SCANNING ACCURACY

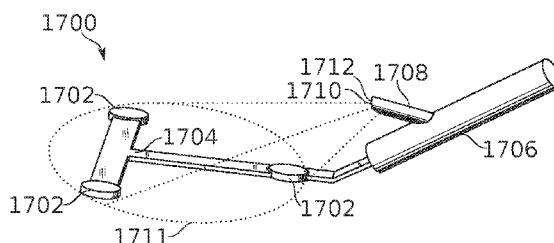


FIGURE 17B

- (57) **Abstract:** Methods and devices are disclosed, by use of which an external fiducial element positioned in the mouth serves as a geometrical constraint on oral arch geometry. In some embodiments, the fiducial element is an oral insert which reaches to a plurality of oral arch regions to present surface details which are in well-defined distance and/or angular relationships to one another. These spatial relationships optionally comprise a spatial frame of reference which serves to constrain reconstruction of the geometry of one or both of the oral arches, for example reconstruction from a collection of digitally registered, partially-overlapping scans made along the oral arch.



SYSTEM, DEVICE, AND METHOD FOR IMPROVED INTRAORAL SCANNING ACCURACY

RELATED APPLICATIONS

5 This application claims the benefit of priority under 35 USC §119(e) of U.S. Provisional Patent Application No. 62/100,920 filed January 8, 2015, the contents of which are incorporated herein by reference in their entirety.

FIELD AND BACKGROUND OF THE INVENTION

10 This disclosure relates to dental scanning techniques, and specifically to systems, devices and methods for accurate intraoral scanning of a full or partial arch.

 Dental restorations may include full or partial arch restorations. Some cases may also include partially or full edentulous conditions, wherein the restorative crowns are placed on teeth and/or implants. Traditionally, such restorations have been performed by forming a model by providing an impression of the relevant areas of a patient's mouth, developing a stone model from the impression, and fabricating a customized prosthetic device on the stone model. This process is cumbersome and requires excessive intrusion into the patient's mouth. However, the stone model usually provides enough accuracy to produce clinically accurate prosthetics.

20 Recently, intraoral scanning (IOS) has emerged as a preferred dental impression technique for conventional (tooth-borne) and implant dentistry. Intraoral scanning typically involves using a handheld scanner having optical sensors to capture a three-dimensional (3D) dataset of an area of interest. The resulting dataset may be used for constructing a model for preparing patient specific prosthetics. The intraoral scanning process offers a very efficient and cost-effective means by which to acquire and transmit anatomic data for purposes of forming a prosthetic. While the accuracy of intraoral scanning has been proven to be sufficient for single tooth restorations and short-span multiple tooth segments (local accuracy), it is often contraindicated (provides insufficient general accuracy) for scanning larger segments such as full or partial arch areas, notably if an edentulous area is present.

 Accuracy is typically described as being composed of trueness (for example, how much a true dimension of the object deviates from its measured size) and precision

(for example, how much individual measurements vary in trueness with respect to one another). Imaging inaccuracies introduced over extended regions of an oral arch potentially result from stitching errors, in which a plurality of stitched images, each of which may be both true and precise internally, are misaligned with respect to one another. This can produce an overall decrease in the accuracy of the reconstructed oral arch, since the errors can build in a “random walk” and/or systematically along the extent of the arch.

While intraoral scanning and stitching is robust in presence of well-defined natural and/or implanted landmarks, lack of those in homogenous areas which are large with respect to the field of view can easily lead to divergence of the model. Unfortunately such areas are common in dental intraoral surgery, considering material and overall system limitations.

One proposed solution has been to spray the connecting geometry area with coating in order to help establish scannable registration features within the connecting area. The arch and the connecting area are then scanned and a resultant dataset is produced. It is assumed that some elements of the connecting area, such as the tongue, contain geometry sufficiently distinguishable for providing robust data. Potentially, however, the spraying technique still results in inaccurate scans; for example, due to possible drift of registration as elements shift from the location captured during the scan. Even if the elements are stable and with sufficiently distinguishable geometry and/or colorimetry, some proportion of scans is potentially subject to greater error using different oral scanning technologies (Meer *et al.* Application of Intra-Oral Dental Scanners in the Digital Workflow of Implantology, PLoS One 2012; 7(8); e43312). Furthermore, scanning protocols specifically adjusted to increase accuracy potentially slow down scanning.

SUMMARY OF THE INVENTION

There is provided, in some embodiments, a system, device and/or method for improving the accuracy of full oral arch or partial oral arch scans with intraoral scanners by introducing a fiducial marker on the oral arch. The fiducial marker may be used as a reference point for a designated location within the oral cavity. The fiducial marker may be scanned by the intraoral scanner and used in an algorithm for correcting an

accumulated scanning error, which may have otherwise been accrued during standard, unmarked, full or partial arch scanning.

There is provided, in accordance with some exemplary embodiments, a method of reconstructing oral geometry using optical intraoral scanning, comprising: optically
5 scanning a plurality of oral regions; positioning each of a plurality of rigidly interconnected fiducial features adjacent to a corresponding portion of one of the oral regions; scanning the positioned fiducial features together with the corresponding adjacent oral portions; and determining the relative positions of the plurality of oral
10 regions based on dimensions of the rigid interconnections of the fiducial features, and on the positions of the fiducial features relative to each corresponding adjacent oral portion.

According to some embodiments, the fiducial features are positioned outside of the oral arches, and the rigid interconnections cross within the oral arches.

According to some embodiments, the scanning of the fiducial features is from
15 outside of the oral arch.

According to some embodiments, the scanning of the fiducial features is of the upper and lower arches simultaneously.

According to some embodiments, the scanning of the fiducial features is while the upper and lower arches are in static occlusion, and the geometry of the occlusion is
20 undisturbed by the positioning of the fiducial element.

According to some embodiments, the fiducial features are positioned to obscure portions of the optically scanned plurality of oral regions.

According to some embodiments, the obscured oral portions comprise teeth.

According to some embodiments, the relative positions of the scanned oral
25 regions are determined for both the obscured and unobscured portions of the scanned oral regions.

According to some embodiments, the rigid interconnections are dimensionally fixed.

According to some embodiments, a dimension of the rigid interconnections is an
30 adjustable dimension.

According to some embodiments, the adjustable dimension is a length or an angle.

According to some embodiments, the adjustable dimension of the rigid interconnections is determined by a reading from a scale marking or an electronic encoder.

According to some embodiments, the adjustable dimension of the rigid
5 interconnections is determined by a dimension in a scan of an adjustably-sized region of an oral insert comprising the rigidly interconnected fiducial features.

According to some embodiments, the rigid interconnections cross unscanned oral regions.

According to some embodiments, the fiducial features are rigidly interconnected
10 to form an oral insert.

According to some embodiments, the dimensions of the rigid interconnections of the fiducial features locate portions of separate fiducial marks to an accuracy and precision within 50 μm .

According to some embodiments, the dimensions of the rigid interconnections of
15 the fiducial features locate portions of separate fiducial marks to an accuracy and precision within 100 μm .

According to some embodiments, the plurality of oral regions comprises regions of an oral arch.

According to some embodiments, the relative positions of the plurality of oral
20 regions are determined for at least two regions which are discontinuous in image data provided by the scanning of the plurality of oral regions.

According to some embodiments, the determining comprises constraining the shape of the geometrical reconstruction based on the positions of the fiducial features relative to corresponding adjacent oral portions.

According to some embodiments, constraining the shape of the geometrical
25 reconstruction comprises correcting out-of-true positions of the geometrical reconstruction based on the positions of the fiducial features relative to corresponding adjacent oral portions.

According to some embodiments, positions in the geometrical reconstruction
30 away from the adjacent oral portions are adjusted by interpolating corrective transformations between the adjacent oral portions on which the correcting of out-of-true positions is based.

According to some embodiments, the scanning comprises scanning of distinct scan field regions; the geometrical reconstruction comprises stitching together of images of the distinct scan field regions by determining stitch registration parameters; and positions in the geometrical reconstruction away from the adjacent oral portions are
5 adjusted by redetermining the stitch registration parameters, constrained by the positions of the adjacent oral portions.

According to some embodiments, the fiducial features are carried on a plurality of plates, and the fiducial features on separate plates are separated from each other by at least two tooth positions.

10 According to some embodiments, the plurality of separate plates comprises at least three plates.

According to some embodiments, the plates are oriented to extend along tooth facial surfaces of an oral arch comprised in the scanned oral regions.

There is provided, in accordance with some exemplary embodiments, a fiducial
15 element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising an oral insert which removably fits into a mouth, and is shaped to extend over an occlusal surface of an oral arch to rigidly interconnect at least three fiducial features, the fiducial features being distributed over an extent of at least eight tooth positions.

20 According to some embodiments, the fiducial features are located at least two tooth positions apart from each other, along the oral arch.

According to some embodiments, at least one of the at least three fiducial features is positioned against surfaces on the buccal side of the oral arch.

According to some embodiments, at least one of the at least three fiducial
25 features is positioned on a surface of the fiducial element which extends over an occlusal surface of the oral arch.

According to some embodiments, the oral insert is shaped as an insert with at least one arm and at least one of the fiducial features is positioned near an end of the arm.

30 According to some embodiments, at least one of a length of the arm and an angle of the arm is adjustable.

According to some embodiments, an adjustment of the arm is encoded by at least one of an electronic encoder and a marked scale.

According to some embodiments, the oral insert comprises at least one plate carrying at least one of the fiducial features.

5 According to some embodiments, the at least one plate is oriented to extend along a facial surface defined by a tooth position of the oral arch.

According to some embodiments, the insert is shaped to be held by clamping between jaws of the mouth; and, when held between the jaws, at least one plate extends over a portion of both maxillary and mandibular oral arches of the jaws.

10 According to some embodiments, the at least one plate is at least 5 mm wide along the extent of the oral arch.

According to some embodiments, the at least three fiducial features are held on at least three corresponding plates, and the plates are separated from each other by at least two tooth positions.

15 According to some embodiments, the oral insert is formed with an outer layer of flexible material at a region where the rigid interconnections cross an oral arch when the oral insert is in the mouth, the layer of flexible material being configured to elastically deform when clamped between jaws of the mouth to fix the oral insert in position.

According to some embodiments, the oral insert comprises at least one LED.

20 According to some embodiments, the oral insert comprises a scannable code, and the code indicates a geometry of the oral insert specifying one or more distances between the plurality of fiducial features.

According to some embodiments, the oral insert comprises an arcuate surface shaped to face an occlusal surface when held between occlusal surfaces of a maxilla and a mandible; and wherein the fiducial features comprise at least one contour line
25 extending along the arcuate surface and at least partially lingual or buccal to the oral arch.

According to some embodiments, the oral insert also comprises a surface facing buccally from the oral arch; and wherein the surface facing buccally comprises at least
30 one of the fiducial features.

According to some embodiments, the fiducial features are rigidly interconnected to relative distances determined within an accuracy of 30 μ m.

There is provided, in accordance with some exemplary embodiments, a fiducial element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising an oral insert which removably fits into a mouth, and is shaped to fit within an oral arch and to rigidly interconnect at least three fiducial features, wherein the fiducial features are located at least two tooth positions apart from each other, along lingual surfaces of the oral arch.

There is provided, in accordance with some exemplary embodiments, a fiducial element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising: an oral insert which removably fits into a mouth to position a plurality of fiducial features therein; and a light collection aperture of an imaging camera, oriented to collect imaging light from the fiducial features; wherein the fiducial features and the light collection aperture are rigidly interconnected to determined positions with respect to one another.

According to some embodiments, imaging by the imaging camera is activated upon contact being sensed by least two of the plurality of contact sensors.

There is provided, in accordance with some exemplary embodiments, a system for reconstructing oral geometry using optical intraoral scanning, comprising a geometry constraint module configured to: receive optical scan data from a plurality of oral regions; receive fiducial scan data comprising scans of rigidly interconnected fiducial features, each positioned adjacent to a portion of the plurality of oral regions; and determine the relative positions of the plurality of oral regions based on dimensions of the rigid interconnections of the fiducial features, and on the positions of the fiducial features relative to each corresponding adjacent oral portion.

According to some embodiments, at least one of the dimensions of the rigid interconnections is provided to the constraint module by a fiducial interface in communication with an encoder of the fiducial element to determine the at least one of the dimensions of the rigid interconnections.

According to some embodiments, the system comprises a fiducial element configured as an oral insert which removably fits into a mouth to position a plurality of fiducial features therein.

According to some embodiments, the scanning comprises scanning of distinct scan field regions, and wherein a scanned and field region with and without a fiducial feature in place overlap by at least 70%.

According to some embodiments, the oral insert is formed with an outer layer of flexible material at a region where the rigid interconnections cross an oral arch when the oral insert is in the mouth.

According to some embodiments, the layer of flexible material elastically deforms when clamped between jaws of the mouth to fix the oral insert in position.

According to some embodiments, the insert is shaped to be held between jaws of the mouth; and, when held between the jaws, at least one plate extends over a portion of both maxillary and mandibular oral arches of the jaws.

Unless otherwise defined, all technical and/or scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which the invention pertains. Although methods and materials similar or equivalent to those described herein can be used in the practice or testing of embodiments of the invention, exemplary methods and/or materials are described below. In case of conflict, the patent specification, including definitions, will control. In addition, the materials, methods, and examples are illustrative only and are not intended to be necessarily limiting.

As will be appreciated by one skilled in the art, aspects of the present invention may be embodied as a system, method or computer program product. Accordingly, aspects of the present invention may take the form of an entirely hardware embodiment, an entirely software embodiment (including firmware, resident software, micro-code, *etc.*) or an embodiment combining software and hardware aspects that may all generally be referred to herein as a “circuit,” “module” or “system.” Furthermore, some embodiments of the present invention may take the form of a computer program product embodied in one or more computer readable medium(s) having computer readable program code embodied thereon. Implementation of the method and/or system of some embodiments of the invention can involve performing and/or completing selected tasks manually, automatically, or a combination thereof. Moreover, according to actual instrumentation and equipment of some embodiments of the method and/or system of the invention, several selected tasks could be implemented by hardware, by software or by firmware and/or by a combination thereof, *e.g.*, using an operating system.

For example, hardware for performing selected tasks according to some embodiments of the invention could be implemented as a chip or a circuit. As software, selected tasks according to some embodiments of the invention could be implemented as a plurality of software instructions being executed by a computer using any suitable operating system. In an exemplary embodiment of the invention, one or more tasks according to some exemplary embodiments of method and/or system as described herein are performed by a data processor, such as a computing platform for executing a plurality of instructions. Optionally, the data processor includes a volatile memory for storing instructions and/or data and/or a non-volatile storage, for example, a magnetic hard-disk and/or removable media, for storing instructions and/or data. Optionally, a network connection is provided as well. A display and/or a user input device such as a keyboard or mouse are optionally provided as well.

Any combination of one or more computer readable medium(s) may be utilized for some embodiments of the invention. The computer readable medium may be a computer readable signal medium or a computer readable storage medium. A computer readable storage medium may be, for example, but not limited to, an electronic, magnetic, optical, electromagnetic, infrared, or semiconductor system, apparatus, or device, or any suitable combination of the foregoing. More specific examples (a non-exhaustive list) of the computer readable storage medium would include the following: an electrical connection having one or more wires, a portable computer diskette, a hard disk, a random access memory (RAM), a read-only memory (ROM), an erasable programmable read-only memory (EPROM or Flash memory), an optical fiber, a portable compact disc read-only memory (CD-ROM), an optical storage device, a magnetic storage device, or any suitable combination of the foregoing. In the context of this document, a computer readable storage medium may be any tangible medium that can contain, or store a program for use by or in connection with an instruction execution system, apparatus, or device.

A computer readable signal medium may include a propagated data signal with computer readable program code embodied therein, for example, in baseband or as part of a carrier wave. Such a propagated signal may take any of a variety of forms, including, but not limited to, electro-magnetic, optical, or any suitable combination thereof. A computer readable signal medium may be any computer readable medium

that is not a computer readable storage medium and that can communicate, propagate, or transport a program for use by or in connection with an instruction execution system, apparatus, or device.

Program code embodied on a computer readable medium and/or data used
5 thereby may be transmitted using any appropriate medium, including but not limited to wireless, wireline, optical fiber cable, RF, etc., or any suitable combination of the foregoing.

Computer program code for carrying out operations for some embodiments of the present invention may be written in any combination of one or more programming
10 languages, including an object oriented programming language such as Java, Smalltalk, C++ or the like and conventional procedural programming languages, such as the "C" programming language or similar programming languages. The program code may execute entirely on the user's computer, partly on the user's computer, as a stand-alone software package, partly on the user's computer and partly on a remote computer or
15 entirely on the remote computer or server. In the latter scenario, the remote computer may be connected to the user's computer through any type of network, including a local area network (LAN) or a wide area network (WAN), or the connection may be made to an external computer (for example, through the Internet using an Internet Service Provider).

Some embodiments of the present invention may be described below with
20 reference to flowchart illustrations and/or block diagrams of methods, apparatus (systems) and computer program products according to embodiments of the invention. It will be understood that each block of the flowchart illustrations and/or block diagrams, and combinations of blocks in the flowchart illustrations and/or block diagrams, can be
25 implemented by computer program instructions. These computer program instructions may be provided to a processor of a general purpose computer, special purpose computer, or other programmable data processing apparatus to produce a machine, such that the instructions, which execute via the processor of the computer or other programmable data processing apparatus, create means for implementing the
30 functions/acts specified in the flowchart and/or block diagram block or blocks.

These computer program instructions may also be stored in a computer readable medium that can direct a computer, other programmable data processing apparatus, or

other devices to function in a particular manner, such that the instructions stored in the computer readable medium produce an article of manufacture including instructions which implement the function/act specified in the flowchart and/or block diagram block or blocks.

5 The computer program instructions may also be loaded onto a computer, other programmable data processing apparatus, or other devices to cause a series of operational steps to be performed on the computer, other programmable apparatus or other devices to produce a computer implemented process such that the instructions which execute on the computer or other programmable apparatus provide processes for
10 implementing the functions/acts specified in the flowchart and/or block diagram block or blocks.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWINGS

Some embodiments of the invention are herein described, by way of example
15 only, with reference to the accompanying drawings. With specific reference now to the drawings in detail, it is stressed that the particulars shown are by way of example, and for purposes of illustrative discussion of embodiments of the invention. In this regard, the description taken with the drawings makes apparent to those skilled in the art how embodiments of the invention may be practiced.

20 In the drawings:

FIGURE 1 is a simplified schematic illustration of a fiducial element according to some embodiments of the present disclosure;

FIGURE 2 is a simplified schematic illustration of the fiducial element of
Figure 1 within an oral cavity at an open state, according to some embodiments of the
25 present disclosure;

FIGURE 3 is a simplified schematic illustration of the fiducial element of
Figure 1 within an oral cavity at a closed state, according to some embodiments of the
present disclosure;

FIGURE 4A is a simplified flowchart of a scanning and data processing method
30 using the fiducial element, according to some embodiments of the present disclosure;

FIGURE 4B is a simplified flowchart of an alternative scanning and data processing method using the fiducial element, according to some embodiments of the present disclosure;

FIGURE 5A is a simplified flowchart of a data processing method using the
5 fiducial element, according to some embodiments of the present disclosure;

FIGURE 5B is a simplified flowchart of an alternative data processing method using the fiducial element, according to some embodiments of the present disclosure;

FIGURE 6 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state according to some embodiments of the present disclosure;

10 FIGURES 7A-7C are each a simplified schematic illustration of a fiducial element according to some embodiments of the present disclosure;

FIGURE 8 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

15 FIGURE 9 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

FIGURE 10 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

FIGURE 11 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

20 FIGURE 12 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

FIGURE 13 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

25 FIGURE 14 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

FIGURE 15 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

FIGURE 16 is a simplified schematic illustration of a fiducial element within an oral cavity at an open state, according to some embodiments of the present disclosure;

30 FIGURES 17A-17B schematically illustrate a fiducial element with integrated scanning device, according to some embodiments of the present disclosure;

FIGURE 18 schematically illustrates an oral insert having fiducial markings along a surface facing the occluding surface of an oral arch, according to some embodiments of the present disclosure; and

FIGURE 19 schematically illustrates a system for constraining the geometrical reconstruction based on intraoral scan data, according to some embodiments of the present disclosure.

DESCRIPTION OF SPECIFIC EMBODIMENTS OF THE INVENTION

This disclosure relates to dental scanning techniques, and specifically to systems, devices and methods for accurate intraoral scanning of a full or partial arch.

A broad aspect of some embodiments of the current invention relates to the constraining of 3-D reconstructions of oral scans to reduce geometrical inaccuracy.

Intraoral scanning robustly supports production of 3-D reconstructions of oral geometry when scanning well defined landmarks (*i.e.*, teeth *vs.* tissue) in a relatively small area (*e.g.* a few teeth, for example 1-4 teeth). Such reconstructions are used, for example, in the preparation of restorative dental work to achieve close spatial tolerances. However, scans of larger areas, and in particular large homogenous areas, such as may be scanned in preparation for full arch restoration, are potentially problematic.

Some scan reconstruction errors occur where non-homogeneous scan segments are lacking (*e.g.*, due to missing teeth). Teeth potentially provide robust landmarks in a scan of an arch, but soft-tissue surfaces between segments of the arch, such as the mouth surfaces, the gingiva, and the tongue, are relatively homogenous surfaces, potentially providing fewer and/or more ambiguous anchor points. Consequentially, the accumulated error during the scan may be larger. Furthermore, small adjacent site-to-site registration errors, while having minimal impact on a single tooth or short-span multiple tooth segments, potentially accumulate to unacceptably large cumulative error, for example throughout the full arch.

In some instances, as a result of errors such as these, the accuracy obtained for a full arch impressions taken by 3-D reconstructions based on intraoral scans (for example) is potentially in the range, for example, of about 30–50 μm , 30–100 μm , 30–500 μm , 30–600 μm , 30–800 μm , or in another range having the same, larger, smaller,

and/or intermediate bounds. Required accuracy may be about 50 μm , in a non-limiting example. Required accuracy can depend on the circumstances to which the 3-D reconstruction will be applied. Natural teeth can move slightly (for example, in the range of about 50–100 μm) to adjust to impression inaccuracies in restorative dental work. However, existing artificial implants potentially allow less movement in at least one direction, for example due to bone compression. This can lead to a higher requirement for impression accuracy.

An aspect of some embodiments of the current invention relates to use of an exogenous fiducial element positioned in the mouth, and serving as a geometrical constraint on oral geometry.

In some embodiments, an exogenous fiducial element is used to supply geometrical constraints to decrease error in impressions produced from intraoral scans. For example, one or more separately known distances between portions of a fiducial element (including, for example, an arch-spanning distance) are related to positions in the intraoral scan data. Then the known distances of the fiducial element optionally serve as geometrical constraints on how the intraoral scan data are converted into a 3-D reconstruction of oral geometry. This allows scanned oral regions which might otherwise be spatially related only through a series of intervening scan registrations to be constrained in their relative position by a smaller number of relatively simple and/or less error-prone measurements.

Optionally, the fiducial element is used with data from current intraoral scanners to create 3-D reconstructions of an arch impression. Reconstruction errors are reduced, for example, in full-arch scans, or scans spanning a large segment of an oral arch (for example, at least 40%, 50%, 60%, or another larger, smaller or intermediate fraction of an oral arch). Optionally, the exogenous fiducial element is used to calibrate an intraoral scan dataset with known anchors to constrain reconstruction from the scanned dataset, potentially reducing reconstruction inaccuracies. In some embodiments, real-time constraint of a scanned dataset, based on fiducial element geometry, is performed as part of the process of acquisition of scan data points. Potentially, use of the fiducial element is fast and easy without adding complicated requirements to the work of the dentist or technician.

In some embodiments, there is a provided a fiducial element which reaches to a plurality of oral arch regions to present surface details which are in well-defined locations relative to one another. These spatial relationships optionally comprise a spatial frame of reference which serves to constrain reconstruction of the geometry of one or both of the oral arches, in whole or in part. In some embodiments, an oral arch geometry is reconstructed from a collection of digitally registered, partially-overlapping scans made along all or part of the oral arch. Optionally, the chain over overlapping scans is such that open-loop errors accumulate in moving between the left and right arms of the oral arch. For example, a small angular inaccuracy in an initial scan registration (*e.g.*, an image stitch) on one side of the arch potentially propagates to become a large out-of-true positional inaccuracy on the other side. Additionally or alternatively, cumulative angular or translational errors at different stitch locations potentially result in a "random walk" error which is larger than any individual registration error.

In some embodiments, distances defined between fiducial marks by the interconnecting fiducial element are fixed. In some embodiments, the distances are adjustable, but rigidly held once adjusted. The frame of reference thus established is potentially used as a direct Cartesian geometry (features at points in a coordinate space), and/or as a set of features having known spatial relationships to one another (*e.g.*, relative distances and angles, and/or offsets therefrom). In some embodiments, the distances are moreover determined with an accuracy of 100 μm or less, 75 μm or less, 50 μm or less, 30 μm or less, 20 μm or less, 10 μm or less, or another greater, smaller/and or intermediate accuracy. With one such distance defined, the constraint defines an arc of relative locations. With at least two such distances defined (for example, among at least three fiducial feature locations), the constraints are tighter. In some embodiments, at least 2, 3, 4, 5, 6, or more fiducial features are available at spacings of (for example) at least one tooth position, two tooth positions, or more. In some embodiments, at least three fiducial features are provided at positions of: the front four teeth, and on the left and right arms of the oral arch beyond the front four teeth.

In some embodiments, use of the fiducial element comprises scan imaging of fiducial marks, the mutual positions of which are determined by methods other than reconstruction of a connecting spatial model. For example, the distances are known

according to a preset (optionally fixed) geometry of the overall fiducial element. Optionally or alternatively, the distances are determined by reference to a scale and/or readout associated with a distance and/or angle of the fiducial element.

Optionally or alternatively, the distances are determined by scanning of a portion
5 of the insert from which an overall dimension can be inferred. For example, a length of an adjustable segment over a strut is scanned and analyzed for length; combined with other known dimensions of the device (even parts which are not imaged), relevant dimensions between fiducial marks are determined. Optionally, an adjustable angle is determined by scanning a join region, and the result used to calculate an overall
10 separation between two fiducial marks.

In some embodiments, fiducial marks can assume any surface shape or contrast difference detectable by a scanner. Sharp boundaries with components extending in two or more at least partially orthogonal directions are of particular use as fiducial marks (since they are potentially easier to register), and may also provide an advantage by
15 allowing precise definition of distances. Shape marks have the potential advantage of being detectable in 3-D scan data. Examples of features particularly suitable for shape marks include surface edges and corners, lines (etched or embossed, for example), and/or line crossings. Contrast differences (for example, surface reflectance differences) are potentially useful for embodiments of 3-D scanners which also capture features of
20 object surfaces.

In some embodiments, a method of scanning comprises a first scan (also called a standard scan herein) of mouth regions which are to be reconstructed (optionally without any fiducial marks present), and then a second scan (also called a fiducial scan herein) with the fiducial marks present. In some embodiments, the fiducial marks are
25 placed in a portion of the same scan fields as were obtained in the first scan; for example, so as to occlude a portion of the mouth geometry which was scanned in the first scan. Features visible in both the first and second scans are registered to one another. Optionally, the scan data are taken from each of the two scans for two closely similar scan fields (70% overlap, 80% overlap, 90% overlap, or another greater, lesser,
30 or intermediate degree over overlap). Potentially, this reduces scan-to-scan registration error.

The positions of fiducial features (such as marks) in the fiducial scan optionally serve as constraints on the positions of nearby oral arch features. Transferring these constraints to the corresponding features of the standard scan, in some embodiments, provides a basis for correction of inaccurate (for example, out-of-true) reconstruction features.

Fiducial features are optionally present buccally, lingually, and/or over the crown. The fiducial features optionally are viewed from a generally buccal, lingual, and/or occlusal direction.

An aspect of some embodiments of the current invention relates to an oral insert comprising fiducial targets held rigidly interconnected with each other.

In some embodiments, the oral insert comprises plates, one or more portions of which serve as fiducial targets. Optionally, the plates are positioned to be held within the mouth against and/or overlying tooth facial surfaces (*i.e.*, buccal and/or labial surfaces) of the oral arch, and/or in positions where the facial surfaces of teeth would be located in a complete oral arch, as defined, for example, by anatomical structures indicating a tooth position. Optionally, the fiducial targets are positioned to be held within the mouth against occlusal surfaces.

In some embodiments, the oral insert comprises an imaging device (a camera and/or scanner, for example), which is also held in a rigid spatial relationship with the fiducial targets. Optionally, the imaging device is positioned to allow imaging of the fiducial targets. Optionally, imaging by the imaging device is triggered by sensing of contact (for example, at two, three, or more contact-sensing positions) between the oral insert and surfaces of the mouth.

In some embodiments, fiducial targets are positioned such that a substantial portion of the oral arch (*e.g.*, a portion comprising teeth) is visible adjacent (for example, immediately adjacent) to the fiducial targets. A substantial portion comprises, for example, a portion which is large enough that a unique position in 3-D space can be determined for a 3-D scan of it, relative to a scan comprising up to most or all of the teeth of the oral arch. Optionally, a substantial portion comprises at least a whole aspect of a tooth, and/or at least an aspect of gap region between teeth comprising a portion of a tooth on at least one side.

Before explaining at least one embodiment of the invention in detail, it is to be understood that the invention is not necessarily limited in its application to the details of construction and the arrangement of the components and/or methods set forth in the following description and/or illustrated in the drawings. The invention is capable of other embodiments or of being practiced or carried out in various ways.

Figures 1–3 are each a simplified schematic illustration of a fiducial element **100** according to some embodiments of the present disclosure. As seen in *Figure 1*, the fiducial element **100** may be configured as an oral insert **102**. The oral insert **102** may be formed in any suitable manner, such as a T-shaped insert including a central longitudinal bar **108** and a branching (for example, generally perpendicular) first arm **110** and second arm **112**.

Optionally, any location on the oral insert **102** is used as a fiducial marker to mark a reference point within an oral cavity **114** (*Figure 2*). In some embodiments, the location may be any one of edges **116** of the bar **108** and arms **110** and **112**. It is a potential advantage for the fiducial marker to comprise a geometrical landmark, such as a corner, edge, indentation, and/or engraving, as these are directly revealed by 3-D scanning. Geometrical landmarks preferably include a shape having at least one sharp change of surface plane. Surface reflection information (*e.g.*, color) is alternatively or additionally used to distinguish fiducial mark locations.

In some embodiments, at the edge **116** of at least one of the bar **108** and arms **110** and **112** may be attached respective plates **118**, **120** and **122**.

The plates **118**, **120** and **122** may be attached to respective bar **108** and arms **110** and **112** in any suitable manner to fit within the oral cavity **114**. For example, the plates may be attached substantially parallel to the edge **116**, such as seen at plate **118**, which is substantially parallel to edge **116** of bar **108**. Plates **120** and **122** are shown to be attached at an incline in respect to edges **116** of arms **110** and **112**. Any one of the plates **118**, **120** or **122** may be used as a fiducial marker to mark a reference point within the oral cavity **114**.

In some embodiments, on any one of plates **118**, **120** or **122** may be etched, or in any manner marked, a fiducial marker or character **128** formed in any suitable configuration, such as an “X” character shown in *Figures 2* and *3*. In particular, markings comprising crossings or corners defined by straight lines (*e.g.*, a grid, “X”,

“+”, “<”, “A”, or another such shape) provide a potential advantage for localization of the crossing/corner, since multiple measurement points potentially constrain each other to indicate a focal region in space. A potential advantage of etching is an effect on the scanned 3-D shape of the plate. Optionally, oral scanner reconstructions combine 3-D shape with surface reflectance properties (such as color, where color imaging is used), allowing use of flat-marked fiducial targets as well or alternatively. Optionally, characters **128** may be used as a fiducial marker to mark a reference point within the oral cavity **114**.

Optionally, the oral insert **102** including the plates **118**, **120** and **122** is be formed of any suitable material, such as stainless steel, or any other dentally compatible material. In some embodiments, the oral insert **102** including the plates **118**, **120** and **122** may be formed of molded plastic.

Optionally, the oral insert **102** is used repeatedly (for example, after resterilization); additionally or alternatively, it is disposable.

The plates **118**, **120** and **122** may be formed in any suitable shape or size. For example, the plates **118**, **120** and **122** may be formed as a square with a side length of approximately 5 mm long and a thickness of approximately 1 mm. In another example, the side may have a length in the range of approximately 1–10 mm and a thickness in the range of approximately 0.2–5 mm.

In other embodiments, the plate may be formed in a circular, ellipse or triangular shape, for example.

In some embodiments, fiducial targets (for example, plates) extend along the extent of the oral arch to a distance about the width of a single tooth, but can be larger or smaller. Vertical extent is optionally the same, but optionally is constrained to extend only partially vertically along the tooth. It is, for example, a potential advantage for registration to be able to scan the basal region of a tooth which the fiducial mark partially overlies.

Optionally, fiducial targets are thick enough to resist distortion during handling and/or upon placement. For example, a press- or clamp-fitted plate embodiment is optionally at least 1 mm thick to avoid distortion. Nevertheless, it is a potential advantage for the plate to be thin, for example in order to bring the scanned surface of the plate closer to the arch geometry which it is used to help characterize.

While a flat geometry such as shown in *Figure 1* indicates one preferred embodiment of a plate **118**, **120**, **122**, herein a “plate” is optionally substituted by any scannable fiducial target which is positioned over and/or nearby native features along the oral arch (particularly against an inside or outside surface of the oral arch), and comprises a fiducial feature (*e.g.*, a mark or geometrical feature) having a determined spatial relationship with a fiducial feature of another such fiducial target. A plate-like geometry, however, has potential advantages, for example, in that:

- main visible surfaces extend substantially along planes, so that 3-D scanned positions scattered across each surface are optionally useful as strong constraints on each other’s positions; and
- well defined edges of main surfaces provide good features for registration algorithms.

In some embodiments, a polygonal plate (such as a rectangular plate) is used, providing, in addition to the above, straight edges (point locations along which potentially also serve to provide mutual constraints), and/or well-defined corners (optionally used as registration features).

Moreover, in some embodiments (as described, for example, in relation to *Figures 8–10* and *15*), plates are positionable to tightly abut one or more surfaces of the oral arch geometry (such as tooth surfaces). Flat plate surfaces potentially constrain the location of contact, which potentially assists in constraining reconstruction of the oral arch geometry.

Despite these potential advantages, it should be understood that, in some embodiments, a non-plate geometry (such as a sphere, ellipsoid, comb, rod, mesh, or other shape) is used as the fiducial target. A spherical or ellipsoidal fiducial target potentially also has a self-constraining surface (defined radius) geometry, and is predictable in contact points in virtue of its regular surface shape; moreover it is a physically robust shape which potentially resists deformation that could interfere with measurement accuracy. A comb or mesh potentially provides a large number of edges which constrain registration, and/or to which native oral arch features can be more closely related. A rod shape is easily made thin (for example, about 1 mm in diameter) to create a fiducial mark which minimally interrupts a scanner’s view of surrounding native oral arch features.

The bar **108** and arms **110** and **112** may be formed of any suitable shape or size. For example, the thickness of the bar **108** and arms **110** and **112** may be in the range of approximately 0.2–5 mm. In some embodiments, plates **118**, **120**, **122** are held with respect to one another by a mouth insert geometry with another shape, for example as
5 described in relation to *Figures 7A–11*. A potential advantage of a bar/arm shaped mounting is that it is easily placed in a wide variety of mouth shapes and/or sizes.

In some embodiments, fiducial targets such as plates **118**, **120**, **122** are held by bar **108** and arms **110**, **112** (or by another mouth insert geometry) at rigidly determined distances from one another. In some embodiments, the rigidly determined distances are
10 predetermined and fixed (adjustable but rigidly determined distances are described, for example, in relation to *Figures 8–10*). Optionally, the distances are determined with respect to well-localized fiducial features such as edges, corners, lines, and/or crossings. Optionally, the distances are determined with respect to abstract features (such as a center position on a plate), but it can be understood that distances are optionally
15 offsetable to also determine distances between well-localized fiducial features.

Optionally, distances are determined within 3-D coordinates (for example, a spatial distance between the center points of two corners or crossings on different fiducial scanning targets). Optionally, distances are determined within a plane—for example, the distance between two vertical (and substantially parallel) edges on two
20 separated fiducial targets. It is easily understood that knowing the total geometry of the fiducial element **100** (for example, as manufactured) allows determining the distance between any two sufficiently well-localized features of the element **100**. However, it is a potential advantage to focus analysis on dimensions which are most likely to be stable, and/or which are easily selected in the design of the fiducial element **100**, such as
25 distances extending along bar **108** or arms **110**, **112**. Furthermore, some distances need to be stable and/or readily determined by a reading across large (and optionally unscanned) extents of the mouth, while short-range distances (*e.g.*, distances falling on a single fiducial target and/or within the scope of a single scan pass) are potentially determined by offsetting from one or more determined longer distances, the offsetting
30 being based on scanning data.

Based on its determined dimensions, the fiducial element **100** may be used as a reference to increase accuracy of a dataset of a full or partial scan of the oral cavity **114**.

Briefly, in some embodiments, distinct mouth regions (in particular, oral arch regions) near to different portions of the fiducial element **100** are potentially subject to errors in scan-determined positioning. Knowing distances between different portions of the fiducial element **100** from one or more non-scan dependent sources allows the application of geometrical constraints to the scan data that potentially reduce those errors.

Scanning is optionally performed by any suitable scanning method **200** and data processing method **250**, for example as described in the respective flowcharts of *Figures 4A–4B* and *5A–5B*. It is appreciated that the method **200** or **250** may be realized in any suitable manner.

Reference is now made to *Figure 4B*, which schematically illustrates a method **201** of oral scanning for fiducial element-guided correction of scan error, according to some embodiments of the disclosure.

At block **203**, in some embodiments, 3-D oral scanning of mouth regions for which geometrical reconstruction (that is, computerized modeling of the 3-D geometry) is performed. The mouth regions optionally comprise complete or partial oral arches. Optionally, mouth regions are scanned disjointly (that is, without initially ensuring that the scanned regions together form a contiguous scan region). Optionally, the resulting mouth region data is of disjoint regions (that is, regions which actually do not together form a contiguous scan region).

At block **223**, in some embodiments, a fiducial element is placed in the mouth with fiducial targets (held in rigid relationship to one another by the fiducial element) positioned near reconstruction target regions. In some embodiments, the fiducial targets are held near reconstruction target regions such that some portions of the regions are obscured (by the fiducial targets themselves, for example, and/or by other structure of the fiducial element), and others, nearby fiducial targets, are visible (unobscured). In some embodiments, fiducial targets held overlying target regions are optionally transparent at least in part; however, the underlying region is still "obscured", at least in the sense of its 3-D surface structure being masked by the overlying fiducial element. In some embodiments, a fiducial target is held overlying and/or obscuring a portion of the basal-to-crown extent of a portion of an oral arch. In some embodiments, a fiducial

target is oriented in the occlusal plane, and it (and/or a supporting portion of the fiducial element) overlies and/or obscures a portion of the occlusal surface of an oral arch.

Additionally or alternatively, the criteria governing placement emphasize adjacency. For example, a fiducial target is held adjacent to an oral region to be reconstructed in 3-D; sufficiently close that accuracy in determining their relative locations is controlled by the accuracy of the scanning device, rather than data registration occurring during reconstruction. For example, the two features (fiducial and oral) occupy a common scan frame and/or scan line. Optionally, the adjacent regions include regions immediately adjacent to the fiducial targets. For example, the fiducial target optionally contacts an adjacent region, and/or is contiguous with it in the 3-D scan data.

In some embodiments, the fiducial element is placed with sufficient stability that two or more sequential scans from different positions can be made without undue risk of movement between the scans. In some embodiments, the elements are placed and imaged so that a single scan establishes the relationship of two or more well-separated fiducial targets and the oral geometry.

At block **235**, in some embodiments, an oral scan including fiducial targets and adjacent regions of the oral arch is performed.

Optionally, the fiducial targets occupy at least two distinct regions separated by at least one, two, three, four, or more tooth positions (teeth or tooth sockets). Additionally or alternatively, the fiducial targets are distributed over at least six, seven, eight, nine, or ten tooth positions, or over a larger or smaller number of tooth positions. Optionally, the fiducial targets comprise two fiducial targets on opposite sides of the oral arch, for example, spaced at least four, five or more tooth positions away from the center or front of the oral arch. Optionally, at least a third fiducial target is positioned within one or two tooth positions of the center or front of the oral arch. Preferably, the fiducial target scans include enough of each adjacent reconstruction target region to allow matching to another image of the same region, through which matching the geometrical constraints of the fiducial element can be transferred to the reconstruction of the oral arch itself. In some embodiments, the fiducial target scans include enough of each fiducial target to allow determination of the distance between fiducial targets based on known geometric constraints established by the fiducial element overall.

At block **239**, in some embodiments, the fiducial element is removed.

At block **241**, in some embodiments, processing occurs (for example, according to one of the methods described in relation to *Figures 5A–5B*) such that a computerized 3-D reconstruction of the target region geometry is constrained (optionally, corrected) according to the scan data acquired by the fiducial target scans and the known and/or separately measured geometry of the fiducial element which rigidly interconnects them.

Reference is now made to *Figure 4A*, which is a simplified flowchart of another scanning and data processing method using the fiducial element, according to some embodiments of the present disclosure;

As seen in *Figure 4A*: at block **202**, in some embodiments, an initial standard scan of the designated full or partial arch **204** (*Figures 2* and *3*) is performed by intraoral scanning methods. Typically, the scanning is performed by using a handheld scanner including optical sensors for capturing a 3-D dataset of the designated full or partial arch **204**. In the intraoral scanning method, absent a reference point, conglomerate errors throughout the partial or full arch **204** may accrue. For example, as shown in *Figure 3*, during standard intraoral scanning, at first the two left sided lower incisors **208** and **210** are scanned from lower incisor **208** to lower incisor **210**. The scanning continues to adjacent two right sided incisors **214** and **216** and then to the other teeth, such as tooth **218**. Yet due to the accumulated error, which accumulated during scanning, when the local single view 3-D models are stitched together, the location of, for example tooth **216** relative to tooth **218** is skewed and inaccurate.

To rectify this error the fiducial element **100** may be inserted at any suitable location within the oral cavity **114**, as seen at block **222**. In *Figure 2* the fiducial element **100** is shown placed upon the mandible **226** resting on the tongue **228**. Optionally, the mandible **226** is tightly fixed to the maxilla **230** to prevent movement of the fiducial element **100**, as seen in *Figure 3*. The plates **118**, **120** and **122** are placed at an external surface **232** (*Figure 3*) of the teeth at the buccal side.

Once the fiducial element **100** is fixedly placed within the oral cavity **114**, fiducial scanning of the arch **204** is performed, as seen in block **234**. The fiducial scanning may be performed in any suitable manner, such as by the same intraoral scanning method used for the standard scanning of block **202**. For example, 3-D scanning of each of the fiducial markers, such as plates **118**, **120** and **122**, may be

performed such that each plate is scanned along with fiducial marker **128** and a surrounding area of uncovered teeth. The fiducial scanning may be of each of the plates and a surrounding area without requiring scanning of the complete designated arch. Optionally, the scan performed at block **202** is partial (that is, comprises gaps in the extent of the scanned data), so long as scanned fragments can be related to one another though the geometry of the fiducial element **100**.

In the example of *Figures 2 and 3*, three fiducial scans are optionally performed: one of plate **118** and the surrounding area, one of plate **120** and the surrounding area and one of plate **122** and the surrounding area. Potentially, this fiducial scanning is very short, since it may require only a single image taken by the scanner (including a three scans). Scan time itself for each fiducial is optionally about 0.1 seconds. Optionally, the scanning is up to a few minutes long.

A potential advantage of having the fiducial targets appear on the buccal side of the oral arches, with connecting elements passing over the oral arches, is that the fiducial element **100** is optionally fixed in place simply by clamping by the jaw. Further potential advantages comprise the relative ease, rapidity, and/or comfort of scanning from the buccal side (particularly from the front). Another potential advantage, in some embodiments is that simultaneous (and potentially faster) acquisition of correction data for both the maxilla **230** and mandible **226** is possible, since the fiducial targets are positioned between them.

In some embodiments, the fiducial element is constructed so that buccal fiducial targets are held in place, and fixed relative to one another, without disturbing the occlusion (for example, without disturbing the normal static occlusion of the patient). For purposes of measurement, an undisturbed occlusion is entirely undisturbed (no displacement in relative positions of the oral arches), or comprises displacement of no more than 10 μm , 15 μm , 30 μm , or another larger, smaller, or intermediate displacement. For example, the fiducial element comprises an arcuate (or otherwise shaped) body fitting around the outside of an oral arch, which is sufficiently rigid to stabilize the relative position of the fiducial targets. The arcuate body itself is optionally secured, for example, by members (optionally thin members such as wires) which pass lingually through natural occlusion gaps, and/or are sufficiently delicate and/or thin that they do not disturb the occlusion (*e.g.*, are bitten through or displaced where teeth

meet), or disturb the occlusion within acceptable tolerances. In some embodiments, for example, a 25 μm -thick (or other larger or smaller thickness), polymer membrane is attached to the rigid body which passes over the occlusal surface of the teeth. In some embodiments, thin fibers pass between parts of the rigid body, strung tightly enough to hold it in place, but flexible enough to be pushed away from regions of close occlusion when the jaws are closed. Additionally or alternatively, the rigid portion of the arcuate body is provided with a fitting element which is flexible for fitting engagement with the oral arch. The fitting by the fitting element comprises, for example, soft deformation of a material in which the rigid body is partially embedded, and/or elastic deformation to clamp the outside of a portion of the oral arch. A potential advantage of such embodiments is to allow simultaneous acquisition of occlusion scan data and fiducial mark scan data. This is a potential advantage for increasing the speed and/or ease of overall scan acquisition, while maintaining the use of an exogenous fiducial element for correction of scan inaccuracies.

In some embodiments, upon completion of the fiducial scanning of block **234**, a small area, such as a portion of plate **118** and an adjoining area, may be rescanned to ensure the fiducial markers did not inadvertently move during the fiducial scanning.

As seen in block **238**, the fiducial element **100** may be removed from the oral cavity **204**.

Thereafter, as seen in block **240**, received data from the initial standard scanning of block **202** may be processed with received data from the fiducial scanning of block **234** in any suitable manner.

Reference is now made to *Figure 5B*, which schematically illustrates a method **251** of correcting target region scans according to corresponding fiducial target scans, according to some exemplary embodiments of the disclosure. Another exemplary processing method **250** is shown in the flowchart of *Figure 5A*.

The method of *Figure 5B* illustrates a method of correction **251** in overview. A more detailed embodiment, along with optional variations and/or alternatives, is described in relation to *Figure 5A*.

At block **255**, in some embodiments, scans of target regions used for intraoral geometry reconstruction are matched to corresponding fiducial target scans. The matching is, for example, on the basis of imaged similarities of intraoral features nearby

to fiducial targets (in the fiducial target scans) to intraoral features seen in the target region scans used as the main basis of intraoral geometry reconstruction. Optionally, the matching also takes advantage of position constraints known otherwise, for example, from the order of scanning, and/or from identifying marks on the fiducial targets which indicate general position relative to the oral arch.

At block **259**, in some embodiments, a target reconstruction is transformed to a new geometry which is consistent with the geometry of the fiducial element. In some embodiments, this comprises altering a completed target reconstruction to fit within constraints established by known geometry of the fiducial element (and its fiducial targets), in view of the matching results of block **255**. In some embodiments, a target reconstruction is initially incomplete, and the fiducial element geometry is used to complete it. This provides a potential advantage when reconstruction target region scans of an oral arch optionally comprise disjoint regions around the arch (there could be edentulous regions between them, for example). It should be understood that the transformation to a new geometry is optionally direct, or through a series of intermediate transformations.

At block **261**, in some embodiments, the transformed reconstruction is optionally adjusted to a suitable reference frame. Whether or not this adjustment is applied optionally depends on how the transformation of block **259** is achieved. For example, in some embodiments, block **259** is accomplished by warping the oral geometry reconstruction into a coordinate system established by the fiducial element and its fiducial targets. However, subsequent processing may be preferably in a coordinate system which is (or is minimally deviated from) the frame of reference used for the initial scan.

At block **263**, in some embodiments, the transformed reconstruction is provided as a corrected reconstruction. Again, it is noted that the terms “transformed” and “corrected” do not necessarily require that “uncorrected” and “untransformed” reconstructions be created as intermediate steps. In some embodiments, a reconstruction is first created already corrected.

As seen in *Figure 5A*, a processing unit may be used along with data connection to the intraoral scanner to perform the following:

As seen in block **254**, an algorithm is executed for matching (that is, spatially registering) the teeth and/or other oral regions scanned in each fiducial scanning of block **234** with the teeth and/or other oral regions scanned in the initial standard scanning of block **202**.

5 In block **258**, at least one 3-D location of each of the fiducial markers, such as plates **118**, **120** and **122**, portions thereof, and/or the characters **128**, is identified relative to a corresponding location in the resultant configuration from the initial standard scanning.

10 In some embodiments, scans comprise images or image-like units of relatively well-determined (precise) points, with the most significant errors being introduced at the stitching stage (two images aligned out-of-true). This error potentially occurs not only during stitching of the standard scan images, but also when the fiducial scan images are registered to corresponding standard scans. Optionally, scan data acquisition for the standard and fiducial scanning operations is performed such that images containing
15 corresponding scan points are overlapping to a greater degree than chance (for example, overlapping, disregarding the loss of occluded areas, by at least 80%, 90%, or another greater, lesser, or intermediate value). This provides a potential advantage for reduction of errors by fiducial-to-standard scan registration, for example by ensuring that a high proportion of corresponding points are available, and/or by reducing potential ambiguity
20 arising from registration to a composite region which was stitched out-of-true.

Optionally, fiducial markers (*e.g.*, plates or regions thereof) are positioned by the mouth insert at places aligned to the boundaries expected from following a recommended scan protocol. For example, if the scan protocol specifies centering a tooth in a scan field, it is a potential advantage for the fiducial mark to be placed so that
25 the registration features it bears are appropriately placed in a tooth-centering scan.

At block **260**, in some embodiments, optimal transformation of the reference fiducial configuration towards the resultant configuration is calculated and applied upon the reference configuration. Calculation of the transformation is optionally based on the location correspondence previously identified between parts of the known geometry of
30 the reference fiducial configuration, and the resultant configuration from the initial standard scanning. The optimal transformation is, for example, a best fit linear isomorphic transformation, optionally comprising rotation and/or translation.

At block **262**, in some embodiments, an optimal transformation of each of the fiducial scans towards the modified reference configuration is evaluated and applied. Optionally, this comprises separately determining the transformation of each of the fiducial scans toward the reference configuration of block **260**, according to the
5 matching associations determined, for example, at block **258**.

A potential advantage of the operations of block **260–262** is to bring the fiducial element coordinate system and the standard and fiducial scan coordinate systems into general alignment. Initial transformation toward the standard scan coordinate system allows generally conserving that scan's coordinate system, so that remaining
10 adjustments remain relatively small. This can also be an advantage, for example, when presenting corrected and uncorrected reconstructions for comparison. If the coordinate system has been minimally disturbed, it is easier to visualize where the constrained reconstruction and the original reconstruction differ. This is a potential advantage for confirming that the process of correction has operated as expected (unusually large, or
15 oddly-shaped corrections would more easily stand out, for example).

At block **264**, in some embodiments, an optimal transformation of matched teeth and/or other oral regions of the initial standard scanning towards the transformed fiducial scans is evaluated. Optionally, this is performed preferably between fiducial and standard scan images with the highest available overlap. Optionally, the transformation
20 is a linear transformation. Optionally, the linear transformation comprises translation and/or rotation. While a scaling constant is also optionally used, the types of mis-registration of greatest concern, in some embodiments, comprise translational and angular misalignments, so that scaling differences can be ignored.

At block **266**, the transformation is extended to the entire area of initial standard
25 scanning. In some embodiments, this comprises interpolation of transform coordinates found for the directly matched regions to other regions so that a substantially continuous gradient of error parameters is applied. Expressed in terms of trueness and precision: the mouth regions located by the fiducial marks are fixed in true, and, optionally, the imprecisions among the data points which cumulatively produce the initial trueness
30 error are redistributed (*e.g.*, the average trueness error is subtracted from regions along the oral arch) without necessarily identifying specific misalignments. This has the potential advantage of being a rapid and/or deterministic correction method.

Alternatively, for example, in embodiments where 3-D image stitching is used, registration constraints established by feature matches between the fiducial scan images and the standard scan images are treated as fixed boundary conditions. Optionally a new 3-D reconstruction is formed by adjusting image stitching parameters (for example, iteratively) until an internally consistent reconstruction is achieved. Expressed in terms of trueness and precision: the mouth regions located by the fiducial marks are fixed in true, and, optionally, new registrations found among stitched scan images which are both individually well-stitched (for example, there may have been an initial ambiguity in the scan data between a plurality of stitching positions), and collectively in true. A potential advantage of this approach is to allow correction of out-of-true stitching at the source; thus removing it, rather than redistributing the inaccuracy so that it cancels out globally.

In some embodiments, block **266** may be performed with the aid of conventional jaw structure model data. There may be a single general model, or a bank of models to be chosen from according to the specific scenario or features of the specific jaw. In some embodiments, local adaptation according to a partial model is performed. Reference to a conventional jaw structure model potentially allows local adjustments to locally out-of-true reconstruction regions. For example, angular deviations from a smooth (*e.g.* monotonically curving) jaw shape at stitching boundaries are optionally detected at a local level and reduced. Since the overall shape is held true at the fiducial marks, the risk of introducing corrections which unacceptably degrade the final fit is potentially reduced.

In some embodiments, a weighting is applied at step **266**, taking into consideration classification of the structures and/or materials of the arch. For example, native teeth typically possess greater flexibility in position than implants. According to the weighting function, some portions of scanned data might be limited in transformation either locally or with respect to another position. Classification is based, for example, upon colorimetry, 3-D structure, and/or jaw modeling.

It should be understood that sequence of transformations described with respect to blocks **260–266** is optionally carried out by an alternative sequence of intermediate transformations, or in a concerted transformation. For example, in some embodiments, the standard scan data is optionally transformed initially into the fiducial reference

configuration and adjusted there, then back-transformed to the coordinates of the original data, either by inversion of a previous transform, or by determination of a new optimal transformation. In some embodiments (for example, if the standard scan includes gaps), the reference fiducial configuration provides a coordinate system into which the standard scan data are integrated.

Following block **266**, a resultant configuration and model of the designated full or partial arch **204** is provided, as seen in block **270**.

Thus, it is shown that there is provided a method for potentially improving full or partial arch scanning by introduction of the fiducial element **100**. The fiducial element **100** is simple to use. Its maintenance may be simple and may be treated as other conventional dental tools, such as by sterilization in an autoclave. The fiducial scanning is as simple to perform as any conventional scanning method, and is of a relatively short duration.

Figure 6 is a simplified schematic illustration of the fiducial element **100** according to some embodiments of the present disclosure. In some embodiments, the oral insert **102** may be produced in a variety of sizes to fit different arch sizes, such as of adults and children. The size and any other relevant information may be inscribed on an inscription **280** on the oral insert **102** in any suitable manner, such by any inscription method that can be scanned by the intraoral scanner and may undergo sterilization. For example, the inscription **280** can be engraved or marked by laser technologies. By inscribing the oral insert information on the oral insert **102** itself, the insert information may be provided to the processing unit without requiring additional entry of the insert information.

In some embodiments, the insert information may include the size of the oral insert **102**. For example, following manufacturing, the size of the oral insert **102** may be measured in any suitable manner, such as by an accurate dimension measuring device, *e.g.* a coordinate measuring machine (CMM).

The insert information can be provided to the processing unit in any suitable manner, such as by encoding the information as a two dimensional barcode or text or 3-D inscription and can be analyzed automatically by an optical character recognition (OCR) algorithm or any other suitable algorithm. The inscription **280** may be inscribed

at any suitable location of the oral insert **102**, such as on bar **108** and/or arms **110** and **112**.

In some embodiments, the oral insert **102** may comprise a light source **282** embedded therein to provide high contrast and accuracy during scanning thereof.

5 In some embodiments, the fiducial element **100** may be configured in any suitable manner. Some exemplary configurations are shown in *Figures 7A–7C*, it being appreciated that many other suitable configurations may be realized.

As seen in *Figure 7A*, the fiducial element **100** comprises an oral insert **300**. The oral insert **300** may be formed in a generally Y-like shape, comprising a central rod **302** and arms **304** and **306**. Plates **310** may be placed at edges of any one of rod **302**, and
10 arms **304** and **306**. The plates **310** may be formed with characters **128** (*Figures 2 and 3*). The oral insert **300** may be placed at any suitable location within the oral cavity **114** and the scanning thereof may be performed as described in reference to *Figures 4 and 5*.

As seen in *Figure 7B*, the fiducial element **100** comprises an oral insert **320**. The
15 oral insert **320** may be formed in a generally V-like shape, comprising arms **324** and **326**. Plates **330** may be placed at edges of any one of arms **324** and **326**. The plates **330** may be formed with characters **128** (*Figures 2 and 3*). The oral insert **320** may be placed at any suitable location within the oral cavity **114** and the scanning thereof may be performed as described in reference to *Figures 4 and 5*.

20 As seen in *Figure 7C*, the fiducial element **100** comprises an oral insert **340**. The oral insert **340** may be formed of a central bar **344** and a plurality of arms **346** extending therefrom. Plates **350** may be placed at edges of any one of bar **344** and arms **346**. The plates **350** may be formed with fiducial markers **128** (*Figures 2 and 3*).

The oral insert **340** may be placed at any suitable location within the oral cavity
25 **114** and the scanning thereof may be performed as described in reference to *Figures 4 and 5*. The plurality of arms **346** and/or plates **350** may provide for a plurality of fiducial markers, thus enhancing the scanning accuracy and allowing for securely placing the oral insert **340** within the oral cavity **114**.

Figure 8 is a simplified schematic illustration of a fiducial element **100** within
30 the oral cavity **114** at an open state. As seen in *Figure 8*, the fiducial element **100** comprises an oral insert **400** formed with at least one lengthwise adjustable arm **410**. The arm **410** may comprise an elastic portion, a spring, or any other extendable portion

414. In some embodiments, the arm **410** may be rotatable, or in any way movable, respective to a central bar **416**. The adjustable oral insert **400** allows for fitting the oral insert **400** with the particular size and shape of the oral cavity **114**. In some embodiments, an indicator may be provided to measure the location of the rotatable arm **410** in respect to a fiducial marker. Such an indicator may be an encoder operative to measure a distance and/or an angle between the rotatable arm **410** and a fiducial marker. Additionally or alternatively, an optical scan of an indicating portion of the oral insert **400** (such as a scale, a digital readout, or simply portion of the geometry itself such as an angle or a length of an adjustable arm portion) is used for determination of the actual distance affecting fiducial mark positions. For example, scanning the length of just extendible portion **414** potentially allows determining the current distance between a fiducial target on plate **422** and other fiducial targets of the oral insert **400**. Optionally, the plate **422** is adjustable to fit at a particular location relative to a scan field recommended by a scan protocol, for example, to achieve good field overlap between a fiducial scan image and a corresponding standard scan image.

In some embodiments, the adjustment of the adjustable oral insert **400** to the oral cavity **114** may be performed by a length measurement device, such as an optical encoder **418** embedded in the adjustable oral insert **400**. The optical encoder **418** may measure the distance required for adjusting the arm **410** to the arch **204** for placing a plate **422** fittingly on an outer side of the mandible **226**. The measured distance may be transmitted to the processing unit and accordingly the adjustment of the adjustable oral insert **400** to the arch **204** is performed. It should be understood that the adjustment, once made, provides a new distance which may be rigidly held by the fiducial element at least for the duration of the fiducial scanning.

Turning to *Figure 9*, it is seen that an oral cavity **428** is partially edentulous. In some locations **430** the gingiva is exposed. In some location a conventional implant **434** is inserted in place of the missing tooth. Accurate scanning by an intraoral scanner of a fully or partially edentulous oral cavity **428** can be challenging, since the teeth structure at exposed locations **430** and at implant locations **434** is discontinuous, and the scanning error along the designated arch, may accumulate. For example, the accumulated error of the arch **204** may be up to about 0.6 mm, in a non-limiting example, while the

accumulated error of the same area in a dentate oral cavity **114** may be, in a non-limiting example, about 0.038–0.333 mm.

Accurate scanning of the edentulous oral cavity **428** is important, since the measurements for a location on the arch designated for a future implant should be accurate. This is since implants, unlike teeth, may have a lower degree of mobility along the jawbone relative to the teeth.

In some embodiments, in order to generate a digital impression of the implants **434** a “scannable abutment” **436** may be placed and located on top of the implant **434**. The scannable abutment **436** bottom may be scanned by the intraoral scanner and the intraoral scanning algorithm may replace the abutment **436** with the dimensions of a top portion of the implant **434**. This is a potential advantage since the implant **434** is optionally metallic and therefore its surface is highly specular and more difficult to scan. In some embodiments, the scannable abutment **436** is designed to be scanned by the intraoral scanner from the top, at a 45° angle, or in some embodiments, from the side. In some embodiments, the scannable abutment **436** comprises a non-specular surface, for example a ceramic, composite and/or polymer surface). In some embodiments, the scannable abutment **436** is formed with a non-smooth geometry (bumped, dimpled, engraved, and/or otherwise roughened) that provides a potential advantage by providing suitable surface features for use in registration. In an embodiment, there may be provided an abutment which protrudes sufficiently from the implant that it can be accurately located (scannable) even when scanned from the side only. To improve the accuracy of locating the abutment, its buccal side **438** can be marked or engraved with fiducials or markers as described herein.

According to some embodiments, a fiducial element **100**, such as an oral insert, is optionally used to provide a fiducial marker to mark a reference point within the edentulous oral cavity **428**. Exemplary oral inserts are shown in *Figures 9–15*, it being appreciated that many oral insert configurations may be realized.

As seen in *Figure 9*, the oral insert **400** may be placed within the edentate oral cavity **428**. The arm **410** may be extended to cover the exposed locations **430** on the mandible **226**, thus providing a fiducial marker at the location prone to cause scanning inaccuracies. During fiducial scanning, such as described in *Figures 4A–4B*, a plurality of scans may be performed wherein during each scan the arm **410** may be moved to

extend over another desired location. It should be understood that the resulting change in fiducial feature geometry at each position is recorded and used in geometrical reconstruction of the oral arch. In the example of *Figure 9*, during a first fiducial scan the arm **410** may extend over exposed locations **430**, as seen in *Figure 9*. Thereafter, the arm **410** may be moved to extend over implant location **434** and an additional scanning thereof may be performed and further processed.

The optical encoder **418** may be provided to measure the distance and angle required for adjusting the arm **410** to the arch **204** for placing the arm **410** over the desired location, (such as locations **430** or **434**) and plate **422** fittingly on an outer side of the mandible **226**.

Turning to *Figure 10*, another exemplary oral insert **450** is shown at least partially placed within edentulous oral cavity **428**. The oral insert **450** may comprise a central rod **454** which may be generally immovably placed on the mandible **226**. A distal arm **458**, distal in respect to lower incisor **208**, may be generally immovably placed on the mandible **226**. A proximal arm **460** may be movable along the central rod **454** in the orientation of arrow **464**. Accordingly, during fiducial scanning, such as described in *Figures 4A–4B*, at a first fiducial scan the proximal arm **460** may extend over exposed locations **430**, as seen in *Figure 10*. Thereafter, the proximal arm **460** may be moved distally to extend over implant location **434** and an additional scanning thereof may be performed and further processed. In some embodiments, the distal arm **458** and/or the central rod **454** may be movable in any suitable orientation. In some embodiments, the proximal arm **460** may be immovable.

As seen in *Figure 11*, an oral insert **480** may be configured generally as a partial or full arch shape. At an outer thickness surface **484** thereof there may be placed fiducial marks **488**. The fiducial marks **488** may comprise a barcode, a character (such as character **128** of *Figures 2* and *3*), for example. During scanning the oral insert **480** may be placed intermediate the maxilla **230** and mandible **226**, wherein a closed state. The designated full or partial arch **204** may be scanned from the side including all teeth and implants abutments.

In some embodiments the outer thickness surface **484** may be in the range of approximately 0.3–15 mm, or in the range of approximately 1–5 mm or any suitable size.

In some embodiments the thickness may vary. For example the thickness at a front portion **486** on the surface **484** may be greater than at a side portion **487** thereof. In a non-limiting example, the thickness at the front portion **486** may be about 3 mm and the thickness at the side portion **487** may be about 1 mm.

5 In some embodiments, light sources **490** such as LEDs may be embedded within outer thickness surface **484** or any other suitable location. The light sources **490** may provide high contrast and accuracy during fiducial scanning. Masks may be added over the LEDs to provide additional degree of distinction of the features.

Turning to *Figure 12*, it is seen that an oral insert **500** may be configured
10 generally in a semi-annulus shape. At an outer thickness surface **504** thereof there may be placed fiducial marks **508**. The fiducial marks **508** may comprise a barcode, a character, for example. Optionally, the marks are etched and/or embossed, allowing their identification from geometry information alone. Optionally, the marks are printed or otherwise placed to alter surface reflectance properties. During scanning, the oral
15 insert **500** may be placed intermediate the maxilla **230** and mandible **226**, which are in a closed state. The designated full or partial arch **204** may be scanned from the side including all teeth and implants abutments. It should be noted that *Figure 12* comprises an example of an oral insert having an alternative fiducial marking configuration to “plates”, as described, for example, in relation to *Figures 1–3*.

20 Reference is now made to *Figure 18*, which schematically illustrates an oral insert **1800**, having fiducial markings **1802**, **1804** along a surface **1801** facing the occluding surface of an oral arch, according to some embodiments of the present disclosure.

Optionally, fiducial features **1802**, **1804** (contour lines **1802** and radial marks
25 **1804** are shown as examples) are placed along the occluding surfaces of the oral insert **1800**. More lingual and/or tooth-overlying portions of the fiducial features **1802**, **1804** are optionally observed when the mandible and maxilla are separated. Optionally, the occlusal surface facing surfaces **1801** extend buccally from the oral insert **1800** so that at least a portion of the occlusal surface fiducial features **1802**, **1804** is visible. A
30 potential advantage of this configuration is to bring tooth crown and fiducial element features into close proximity. In some embodiments, a fiducial feature comprises a contour line **1802**, optionally a concentric group of contour lines, extending along and

around a crown surface of the oral insert **500**. The contour line or lines are engraved, embossed, or printed, for example. A potential advantage of such a feature is to allow direct determination of the distance between crown end and fiducial feature. This can be useful, for example, in isolating the positions of scan registration errors in the original reconstruction. Optionally, the contours are shaped to approximate a standard jaw structure. Optionally, this is used, for example, together with the method of jaw structure model usage described in relation to block **266** of *Figure 5A*, herein. Optionally, radially oriented lines **1804** (and/or other markings) are used to help determine distance along lines **1802**.

In some embodiments, light sources **509**, such as LEDs, may be embedded within outer thickness surface **504** or any other suitable location. The light sources **509** may provide high contrast and accuracy during fiducial scanning. Masks may be added over the LEDs to provide additional degree of distinction of the features (for example, the fiducial marks are optionally constituted not merely as reflectance surface properties, but as light-emitting regions).

As seen in *Figure 13*, the oral insert **500** may be provided with plates **510**, which may also comprise fiducials markers **512**, which may be scanned as described in reference to *Figures 4* and *5*. During fiducial scanning, the plates **510** may be scanned with teeth and abutments or implants in between the plates **510**.

Turning to *Figure 14* it is seen that oral insert **500** may be provided with a continuous strip **520** surrounding at least a portion of the outer thickness surface **504**. In some embodiments the thickness of strip **520** may be in the range of approximately 1–7 mm, or any suitable size. Strip **520** may comprise fiducial markers **522**. The strip **520** and/or fiducial markers **522** may be scanned as described in reference to *Figures 4* and *5*. A potential advantage of such a strip is to provide a continuous region of well-determined geometry, for example, to continuously fill in a large gap between teeth.

In the embodiments of *Figures 1–14*, the fiducial markers are shown placed at external (buccal) surface **232** of the teeth. Additionally or alternatively, the fiducial markers may be placed within the oral cavity at an internal surface **540** of the teeth, such as shown in *Figure 15*. An oral insert **550** may be formed with a central T-like bar **556** and extendable arms **560**, **562** and **564** extending therefrom and can fix the oral insert to the jaw. In some embodiments the fiducial markers may be provided as plates

570 and **572**, and **574** placed at edges of respective arms **560** and **562** and **564** up and against the internal surface **540** of the arch **204**. In some embodiments, the fiducial markers may be provided as characters **580** etched, embossed, and/or in any other suitable manner marked, on arms **560**, **562** and **564**. Plates **570**, **572** and **574** may or
5 may not be obviated in such embodiments.

The extendable arms are configured to be adjusted to abut against the internal surface **540** of the teeth. In some embodiments, this may be performed by an optical encoder **582** embedded in the oral insert **550**. The optical encoder **582** may measure the distance required for adjusting any one of the arms **560**, **562** and **564** to the arch **204** for
10 placing the plates **570**, **572** and **574** or edges of the arms **560**, **562** and **564** fittingly at internal surface **540**. The measured distance may be transmitted to the processing unit and accordingly the adjustment of the adjustable oral insert **550** to the arch **204** is performed.

The arms **560**, **562** and **564** may comprise an elastic portion, a spring, or any
15 other extendable portion (however, *in situ*, adjusted to press against the oral arch, it should be understood that the distances established between fiducial marks are rigidly held to allow them to be precisely determined). In some embodiments, the arms **560**, **562** and **564** may be rotatable, or in any way movable, respective to a central T-like bar **556**.

20 The oral insert **550** may be shaped in any suitable form, such as described in reference to *Figures 1–14*, while the fiducial marker is placed within the oral cavity at the internal surface **540** thereof.

The oral insert **550** may be placed upon the arch **204** of the mandible **226**, as shown in *Figure 15*, or may be placed upon the arch **204** of the maxilla **230**.

25 Scanning of the oral insert **550** and processing the data received therefrom may be formed by scanning method **200** and data processing method **250**, such as described in the flowchart of *Figures 4* and *5*, *mutatis mutandis*, as will be described as follows. It should be understood that elucidating remarks made herein applying to the descriptions of *Figures 4* and *5* also apply, changed as necessary, to corresponding portions of the
30 following descriptions.

As seen in *Figure 4A*, at block **202**, the initial standard scan of the designated full or partial arch **204** is performed by intraoral scanning methods. Typically, the

scanning is performed by using a handheld scanner including optical sensors for capturing a 3-D dataset of the designated full or partial arch **204**.

The fiducial element **100** comprising oral insert **550** may be inserted at any suitable location within the oral cavity **114**, as seen at block **222**. In *Figure 15* the oral insert **550** is shown placed upon the mandible **226** resting on the tongue **228**. The plates **570**, **572** and **574** or edges of the arms **560**, **562** and **564** are placed at internal surface **540** of the teeth.

Once the fiducial element **100** is fixedly placed within the oral cavity **114**, fiducial scanning of the arch **204** is performed, as seen in block **234**, while the oral cavity **114** is in an open state. The fiducial scanning may be performed in any suitable manner, such as by the same intraoral scanning method used for the standard scanning of block **202**. For example, 3-D scanning of each of the fiducial markers, such as plates **570**, **572** and **574** or edges of the arms **560**, **562** and **564**, may be performed such that each plate or arm edge is scanned along with character or fiducial marker **580** and a surrounding area of uncovered teeth. The fiducial scanning may be of each of the plates or arm edge and a surrounding area without requiring scanning of the complete designated arch. In the example of *Figure 15*, three fiducial scans may be performed: one of plate **570** and surrounding area, one of plate **572** and surrounding area and one of plate **574** and surrounding area. This fiducial scanning may be very short, such as a few seconds to a few minutes long.

In some embodiments, block **234** is performed additionally on the maxilla **230**. In some embodiments, the accuracy correction may be transferred from the mandible **226** to the maxilla **230** or vice versa by 3-D scanning of an area including both the mandible **226** and the maxilla **230**.

In some embodiments, upon completion of the fiducial scanning of block **234**, a small area, such as plate **570** or edge of arm **560**, may be rescanned to ensure the fiducial markers did not inadvertently move during the fiducial scanning.

As seen in block **238**, the oral insert **550** may be removed from the oral cavity **114**.

Thereafter, as seen in block **240**, received data from the initial standard scanning of block **202** may be processed with received data from the fiducial scanning in any suitable manner.

An exemplary processing method **250** is shown in the flowchart of *Figure 5A*.

As seen in *Figure 5A*, a processing unit may be used along with data connection to the intraoral scanner to perform the following:

As seen in block **254**, an algorithm is executed for matching the teeth scanned in
5 each of the fiducial scanning with the teeth scanned in the initial standard scanning of block **202**.

In block **258**, the 3-D location of each of the fiducial marker, such as plates **570**, **572** and **574** or edges of the arms **560**, **562** and **564** and/or the characters **580** thereof, is identified relative to a resultant configuration from the initial standard scanning.

10 At block **260**, an optimal transformation of the reference fiducial configuration towards the resultant configuration is calculated and applied upon the reference configuration.

At block **262**, an optimal transformation of each of the fiducial scans towards the modified reference configuration is evaluated and applied.

15 At block **264**, the optimal transformation of matched teeth of initial standard scanning towards the transformed fiducial scans is evaluated.

At block **266**, the optimal transformation of the teeth of block **264** may be applied to the data received during the initial standard scanning of block **202**. In some embodiments, block **266** may be performed with the aid of conventional jaw structures
20 model data.

Following block **266**, a resultant configuration and model of the designated full or partial arch **204** is provided, as seen in block **270**.

In the embodiments of *Figure 1–15* the fiducial element **100** comprises an oral insert. In some embodiments, the fiducial element **100** may comprise fiducial markers
25 formed by plates **600** and/or by characters **602** marked thereon, as shown in *Figure 16*. The plates **600** may be placed at any suitable location within the oral cavity **114**, at the external surface **232** or internal surface **540**. The plates **600** may be fixed to the teeth or oral cavity **114** in any suitable manner, such as by an adhesive, or suction, for example. The plates **600** may be formed in any suitable configuration, such as metal plates, sheets
30 and adhesives, for example.

To ensure accurate measurement, a fixed location may be measured, such as some fixed location within the oral cavity. The distance between the fiducial markers on

plates **600** and the fixed location can be used as a measurement for correcting any accumulated inaccuracies accruing during the intraoral scanning of the oral cavity. Such embodiments provide a potential advantage for cases where relatively long-term fiducial stability is indicated. For example, the fiducial marks can be used to provide stable spatial references during the configuration of a configurable abutment. Optionally, the 3-D locations are measured based on imaged acquired by a stereo camera, or by a standard camera from two or more directions.

In some embodiments, such as the embodiments of *Figs 1–16*, the fiducial element **100** may be covered by a coating and/or layer of flexible material designed to provide enhanced fixation and stability of the fiducial element **100** by the jaws at closure of the oral cavity **114**. The flexible material layer provides additional contact points between the jaw and the fiducial element **100**. Without the flexible material layer there might be only a few contact points between the jaws and the fiducial element **100**.

The flexible material layer may be formed such that when pressed by the teeth, it allows the teeth to imprint into the flexible material layer while maintaining a desirable degree of stiffness, to keep fiducial element **100** fixed relative to the jaws at an accuracy of around 20 μm , around 30 μm , around 100 μm , or any other suitable (greater, smaller, or intermediate) degree of accuracy.

In some embodiments, the flexible material layer can have thickness of 0.1–2 mm, for example. In some embodiments the flexible material layer can have a larger thickness, when the layer is sufficiently stiff. In some embodiments the flexible material layer can be configured to cover only the possible occluded contact area of teeth.

Reference is now made to *Figures 17A–17B*, which schematically illustrate a fiducial element **1700** with integrated scanning device **1710**, according to some embodiments of the present disclosure.

In some embodiments, a fiducial element **1700** comprises a plurality of fiducial targets **1702**, interconnected by an interconnecting element **1704**. Shown is T-shaped interconnecting element **1704**; it should be understood that any other interconnecting element shape is optionally provided, for example as such shapes are described in relation to the figures herein.

In some embodiments, fiducial element **1700** additionally comprises a scanning camera **1710**, optionally along with a scanning illumination source **1712**. To give a

suitable scanning field of view **1711**, the scanning camera **1710** and/or illumination source **1712** are held out of the plane of fiducial targets **1702** by one or more portions of fiducial element **1700**, for example, by interconnecting element **1704**, handle **1706**, and/or mount **1708**. Optionally, a field of view **1713** is provided which is large enough to encompass both the mandible and maxilla. Optionally, the device is used against the mandible, and/or against the maxilla.

In some embodiments of the invention, the spatial relationship of the camera **1710** to the fiducial marks **1702** is known according to the geometrical configuration of the fiducial element **1700**. For example, the relationship is fixed, or adjustable with a scale or other measurable indication. By imaging the fiducial marks in relation with the teeth, data is acquired which can be registered to other intraoral scan data, allowing scan data position constraints (for example, error correction) to be applied in a computer reconstruction of the oral 3-D geometry.

In some embodiments, fiducial targets **1702** each comprise a contact sensor. Optionally, image acquisition by camera **1710** is coupled to activation of the contact sensors. In some embodiments, the camera is triggered by contact of at least two contact sensors. In some embodiments, contact by two, three, or more sensors is required. Optionally, the number of contacts required for triggering is configurable, for example, based on the configuration of the teeth in the jaw of the patient (two contacts used when teeth are missing that would be underneath a third contact, for example). In some embodiments, triggering comprises identification, and optionally recording, of the contact sensor(s) which trigger image acquisition.

Contact triggering is a potential advantage to help ensure that the fiducial targets **1702** are in a known spatial relationship (comprising contact at some point) with elements of the oral arch. Another potential advantage of contact triggering is to the speed and facility of automatic image acquisition while using one hand.

Reference is now made to *Figure 19*, which schematically illustrates a system **1900** configured to constrain geometrical reconstruction from intraoral scan data **1910**, **1906** (for example, to correct reconstruction inaccuracies) using a fiducial element **1902**, according to some embodiments of the present disclosure.

System elements are shown in highly schematic form. In some embodiments, a fiducial element **1902** is provided for insertion to an oral cavity **1901**; it is optionally held, for example between oral arches **1905** and **1903**.

In some embodiments, a processing module **1908** is provided (which comprises, for, example, one or more digital computers). Optionally, module **1908** comprises one or more sub-modules (which comprise be hardware and/or software sub-modules). Optionally, the modules include fiducial element interface **1916**, scanning module **1918**, scan constraint module **1920**, and/or user interface module **1912**.

In some embodiments, oral scans are obtained (with and/or without the fiducial element **1902** in place) using scanner wand **1904**. Optionally, scanning module **1918** supervises acquisition and/or initial stitching (or other reconstruction) of scan data into a 3-D model of oral geometry. For convenience of reference, scan data acquired without a fiducial element **1902** in place are represented as intra-oral scan data **1910**; scans acquired with the fiducial element in place are represented as fiducial scan data **1906**.

In some embodiments, a fiducial element **1902** comprises one or more electronic devices **1922** (for example, position sensing encoders, contact sensors, LEDs, and/or camera/scanner hardware). Optionally, fiducial interface module **1916** communicates with these devices; for example, to control power, manage operation, and/or detect signals.

In some embodiments constraint module **1920** processes scan data **1910**, **1906**; optionally in coordination with data obtained via fiducial interface **1916**, to apply geometrical correction and/or constraints to optical scan data **1910** in order to produce and/or modify a reconstructed model of oral geometry **1924**. Optionally, one or both of an unconstrained (direct-from-scan) and constrained (optionally, corrected) 3-D model is created.

In some embodiments user interface **1912** is used for control of and/or display from processing module **1908**. In particular, interface control/display is optionally exercised over any of the processing module **1908** sub-modules **1920**, **1916**, **1918**.

As used herein with reference to quantity or value, the term “about” means “within $\pm 10\%$ of”.

The terms “comprises”, “comprising”, “includes”, “including”, “having” and their conjugates mean: “including but not limited to”.

The term “consisting of” means: “including and limited to”.

The term “consisting essentially of” means that the composition, method or structure may include additional ingredients, steps and/or parts, but only if the additional ingredients, steps and/or parts do not materially alter the basic and novel characteristics of the claimed composition, method or structure.

As used herein, the singular form “a”, “an” and “the” include plural references unless the context clearly dictates otherwise. For example, the term “a compound” or “at least one compound” may include a plurality of compounds, including mixtures thereof.

The words “example” and “exemplary” are used herein to mean “serving as an example, instance or illustration”. Any embodiment described as an “example” or “exemplary” is not necessarily to be construed as preferred or advantageous over other embodiments and/or to exclude the incorporation of features from other embodiments.

The word “optionally” is used herein to mean “is provided in some embodiments and not provided in other embodiments”. Any particular embodiment of the invention may include a plurality of “optional” features except insofar as such features conflict.

As used herein the term “method” refers to manners, means, techniques and procedures for accomplishing a given task including, but not limited to, those manners, means, techniques and procedures either known to, or readily developed from known manners, means, techniques and procedures by practitioners of the chemical, pharmacological, biological, biochemical and medical arts.

As used herein, the term “treating” includes abrogating, substantially inhibiting, slowing or reversing the progression of a condition, substantially ameliorating clinical or aesthetical symptoms of a condition or substantially preventing the appearance of clinical or aesthetical symptoms of a condition.

Throughout this application, embodiments of this invention may be presented with reference to a range format. It should be understood that the description in range format is merely for convenience and brevity and should not be construed as an inflexible limitation on the scope of the invention. Accordingly, the description of a range should be considered to have specifically disclosed all the possible subranges as well as individual numerical values within that range. For example, description of a range such as “from 1 to 6” should be considered to have specifically disclosed

subranges such as “from 1 to 3”, “from 1 to 4”, “from 1 to 5”, “from 2 to 4”, “from 2 to 6”, “from 3 to 6”, *etc.*; as well as individual numbers within that range, for example, 1, 2, 3, 4, 5, and 6. This applies regardless of the breadth of the range.

Whenever a numerical range is indicated herein (for example “10-15”, “10 to 15”, or any pair of numbers linked by these another such range indication), it is meant to include any number (fractional or integral) within the indicated range limits, including the range limits, unless the context clearly dictates otherwise. The phrases “range/ranging/ranges between” a first indicate number and a second indicate number and “range/ranging/ranges from” a first indicate number “to”, “up to”, “until” or “through” (or another such range-indicating term) a second indicate number are used herein interchangeably and are meant to include the first and second indicated numbers and all the fractional and integral numbers therebetween.

Although the invention has been described in conjunction with specific embodiments thereof, it is evident that many alternatives, modifications and variations will be apparent to those skilled in the art. Accordingly, it is intended to embrace all such alternatives, modifications and variations that fall within the spirit and broad scope of the appended claims.

All publications, patents and patent applications mentioned in this specification are herein incorporated in their entirety by reference into the specification, to the same extent as if each individual publication, patent or patent application was specifically and individually indicated to be incorporated herein by reference. In addition, citation or identification of any reference in this application shall not be construed as an admission that such reference is available as prior art to the present invention. To the extent that section headings are used, they should not be construed as necessarily limiting.

It is appreciated that certain features of the invention, which are, for clarity, described in the context of separate embodiments, may also be provided in combination in a single embodiment. Conversely, various features of the invention, which are, for brevity, described in the context of a single embodiment, may also be provided separately or in any suitable subcombination or as suitable in any other described embodiment of the invention. Certain features described in the context of various embodiments are not to be considered essential features of those embodiments, unless the embodiment is inoperative without those elements.

WHAT IS CLAIMED IS:

1. A method of reconstructing oral geometry using optical intraoral scanning, comprising:
 - optically scanning a plurality of oral regions;
 - positioning each of a plurality of rigidly interconnected fiducial features adjacent to a corresponding portion of one of the oral regions;
 - scanning the positioned fiducial features together with the corresponding adjacent oral portions; and
 - determining the relative positions of the plurality of oral regions based on dimensions of the rigid interconnections of the fiducial features, and on the positions of the fiducial features relative to each corresponding adjacent oral portion.
2. The method of claim 1, wherein the fiducial features are positioned outside of the oral arches, and the rigid interconnections cross within the oral arches.
3. The method of claim 2, wherein the scanning of the fiducial features is from outside of the oral arch.
4. The method of claim 3, wherein the scanning of the fiducial features is of the upper and lower arches simultaneously.
5. The method of claim 4, wherein the scanning of the fiducial features is while the upper and lower arches are in static occlusion, and the geometry of the occlusion is undisturbed by the positioning of the fiducial element.
6. The method of claim 1, wherein the fiducial features are positioned to obscure portions of the optically scanned plurality of oral regions.
7. The method of claim 6, wherein the obscured oral portions comprise teeth.

8. The method of claim 6, wherein the relative positions of the scanned oral regions are determined for both the obscured and unobscured portions of the scanned oral regions.

9. The method of claim 1, wherein the rigid interconnections are dimensionally fixed.

10. The method of claim 1, wherein a dimension of the rigid interconnections is an adjustable dimension.

11. The method of claim 10, wherein the adjustable dimension is a length or an angle.

12. The method of claim 10, wherein the adjustable dimension of the rigid interconnections is determined by a reading from a scale marking or an electronic encoder.

13. The method of claim 10, wherein the adjustable dimension of the rigid interconnections is determined by a dimension in a scan of an adjustably-sized region of an oral insert comprising the rigidly interconnected fiducial features.

14. The method of claim 1, wherein the rigid interconnections cross unscanned oral regions.

15. The method of claim 1, wherein the fiducial features are rigidly interconnected to form an oral insert.

16. The method of claim 1, wherein the dimensions of the rigid interconnections of the fiducial features locate portions of separate fiducial marks to an accuracy and precision within 50 μm .

17. The method of claim 1, wherein the dimensions of the rigid interconnections of the fiducial features locate portions of separate fiducial marks to an accuracy and precision within 100 μm .

18. The method of claim 1, wherein the plurality of oral regions comprise regions of an oral arch.

19. The method of claim 1, wherein the relative positions of the plurality of oral regions are determined for at least two regions which are discontinuous in image data provided by the scanning of the plurality of oral regions.

20. The method of any one of claims 1-19, comprising generating a geometrical reconstruction of the oral regions from data provided by the optically scanning; and wherein the determining comprises constraining the shape of the geometrical reconstruction based on the positions of the fiducial features relative to corresponding adjacent oral portions.

21. The method of claim 20, wherein constraining the shape of the geometrical reconstruction comprises correcting out-of-true positions of the geometrical reconstruction based on the positions of the fiducial features relative to corresponding adjacent oral portions.

22. The method of claim 20, wherein positions in the geometrical reconstruction away from the adjacent oral portions are adjusted by interpolating corrective transformations between the adjacent oral portions on which the correcting of out-of-true positions is based.

23. The method of claim 20, wherein:

the scanning comprises scanning of distinct scan field regions;

the geometrical reconstruction comprises stitching together of images of the distinct scan field regions by determining stitch registration parameters; and

positions in the geometrical reconstruction away from the adjacent oral portions are adjusted by redetermining the stitch registration parameters, constrained by the positions of the adjacent oral portions.

24. The method of claim 23, wherein the fiducial features are carried on a plurality of plates, and the fiducial features on separate plates are separated from each other by at least two tooth positions.

25. The method of claim 24, wherein the plurality of separate plates comprise at least three plates.

26. The method of claim 24, wherein the plates are oriented to extend along tooth facial surfaces of an oral arch comprised in the scanned oral regions.

27. A fiducial element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising an oral insert which removably fits into a mouth, and is shaped to extend over an occlusal surface of an oral arch to rigidly interconnect at least three fiducial features, the fiducial features being distributed over an extent of at least eight tooth positions.

28. The fiducial element of claim 27, wherein the fiducial features are located at least two tooth positions apart from each other, along the oral arch.

29. The fiducial element of claim 27, wherein at least one of the at least three fiducial features is positioned against surfaces on the buccal side of the oral arch.

30. The fiducial element of claim 27, wherein at least one of the at least three fiducial features is positioned on a surface of the fiducial element which extends over an occlusal surface of the oral arch.

31. The fiducial element of claim 27, wherein the oral insert is shaped as an insert with at least one arm and at least one of the fiducial features is positioned near an end of the arm.

32. The fiducial element of claim 31, wherein at least one of a length of the arm and an angle of the arm is adjustable.

33. The fiducial element of claim 32, wherein an adjustment of the arm is encoded by at least one of an electronic encoder and a marked scale.

34. The fiducial element of claim 27, wherein the oral insert comprises at least one plate carrying at least one of the fiducial features.

35. The fiducial element of claim 34, wherein the at least one plate is oriented to extend along a facial surface defined by a tooth position of the oral arch.

36. The fiducial element of claim 34, wherein the insert is shaped to be held by clamping between jaws of the mouth; and, when held between the jaws, at least one plate extends over a portion of both maxillary and mandibular oral arches of the jaws.

37. The fiducial element of claim 34, wherein the at least one plate is at least 5 mm wide along the extent of the oral arch.

38. The fiducial element of claim 34, wherein the at least three fiducial features are held on at least three corresponding plates, and the plates are separated from each other by at least two tooth positions.

39. The fiducial element of claim 27, wherein the oral insert is formed with an outer layer of flexible material at a region where the rigid interconnections cross an oral arch when the oral insert is in the mouth, the layer of flexible material being configured to elastically deform when clamped between jaws of the mouth to fix the oral insert in position.

40. The fiducial element of claim 27, wherein the oral insert comprises at least one LED.

41. The fiducial element of claim 27, wherein the oral insert comprises a scannable code, and the code indicates a geometry of the oral insert specifying one or more distances between the plurality of fiducial features.

42. The fiducial element of claim 27, wherein the oral insert comprises an arcuate surface shaped to face an occlusal surface when held between occlusal surfaces of a maxilla and a mandible; and wherein the fiducial features comprise at least one contour line extending along the arcuate surface and at least partially lingual or buccal to the oral arch.

43. The fiducial element of claim 42, wherein the oral insert also comprises a surface facing buccally from the oral arch; and wherein the surface facing buccally comprises at least one of the fiducial features.

44. The fiducial element of any one of claims 27-43, wherein the fiducial features are rigidly interconnected to relative distances determined within an accuracy of 30 μm .

45. A fiducial element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising an oral insert which removably fits into a mouth, and is shaped to fit within an oral arch and to rigidly interconnect at least three fiducial features, wherein the fiducial features are located at least two tooth positions apart from each other, along lingual surfaces of the oral arch.

46. A fiducial element for constraint of oral arch geometry reconstructed from optical intraoral scan data, the fiducial element comprising:

an oral insert which removably fits into a mouth to position a plurality of fiducial features therein; and

a light collection aperture of an imaging camera, oriented to collect imaging light from the fiducial features;

wherein the fiducial features and the light collection aperture are rigidly interconnected to determined positions with respect to one another.

47. The fiducial element of claim 46, comprising a plurality of contact sensors positioned on the oral insert to contact teeth when the insert is fitted into the mouth, wherein imaging by the imaging camera is activated upon contact being sensed by least two of the plurality of contact sensors.

48. A system for reconstructing oral geometry using optical intraoral scanning, comprising a geometry constraint module configured to:

receive optical scan data from a plurality of oral regions;

receive fiducial scan data comprising scans of rigidly interconnected fiducial features, each positioned adjacent to a portion of the plurality of oral regions; and

determine the relative positions of the plurality of oral regions based on dimensions of the rigid interconnections of the fiducial features, and on the positions of the fiducial features relative to each corresponding adjacent oral portion.

49. The system of claim 48, wherein at least one of the dimensions of the rigid interconnections is provided to the constraint module by a fiducial interface in communication with an encoder of the fiducial element to determine said at least one of the dimensions of the rigid interconnections.

50. The system of claim 48, comprising a fiducial element configured as an oral insert which removably fits into a mouth to position a plurality of fiducial features therein.

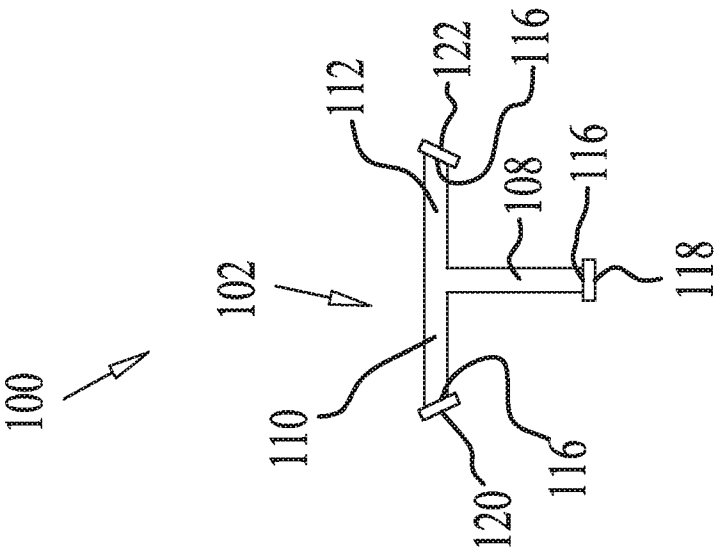


FIGURE 1

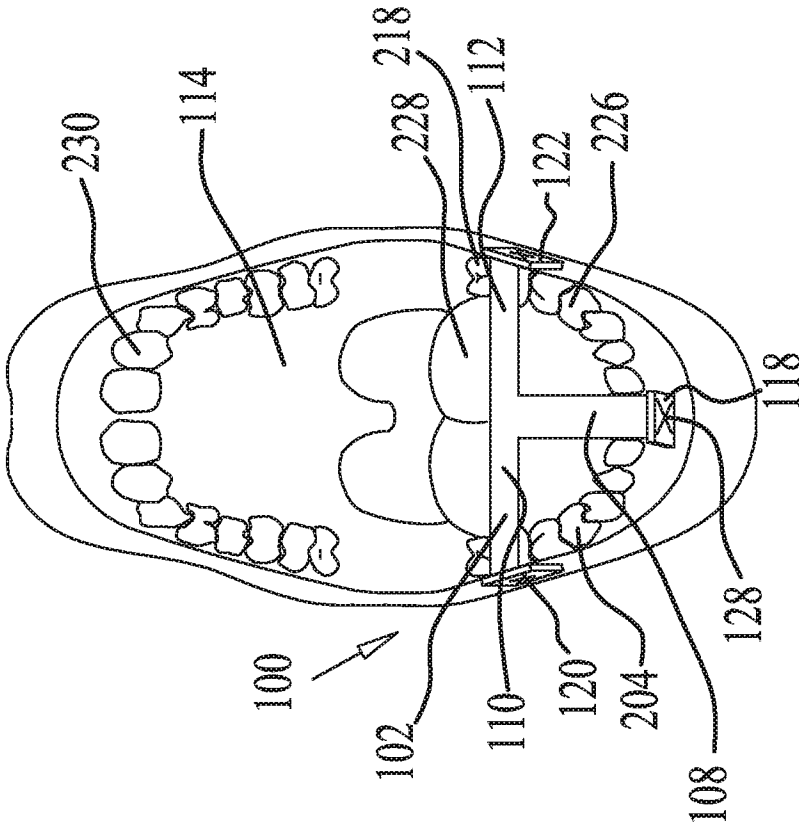


FIGURE 2

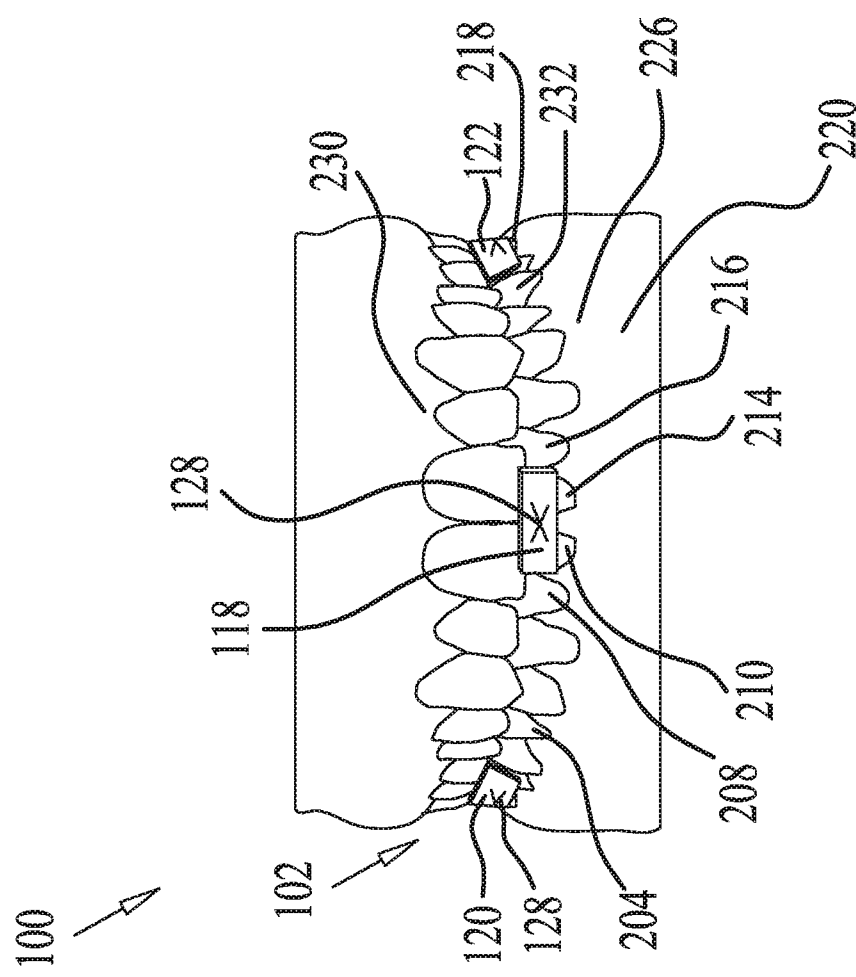


FIGURE 3

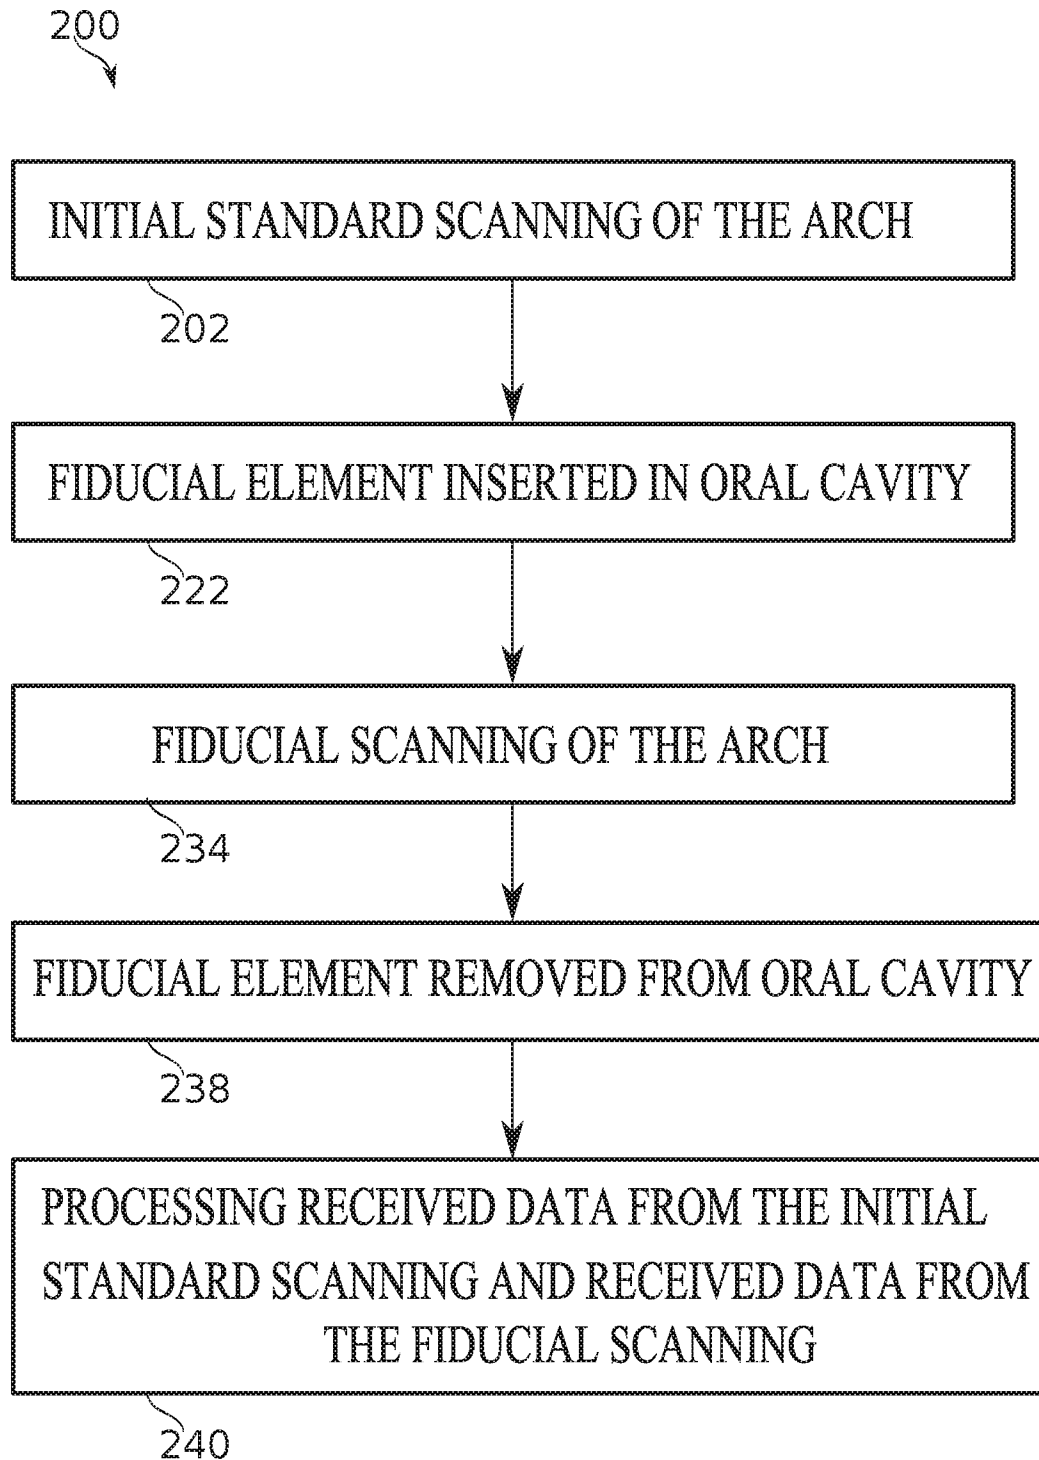


FIGURE 4A

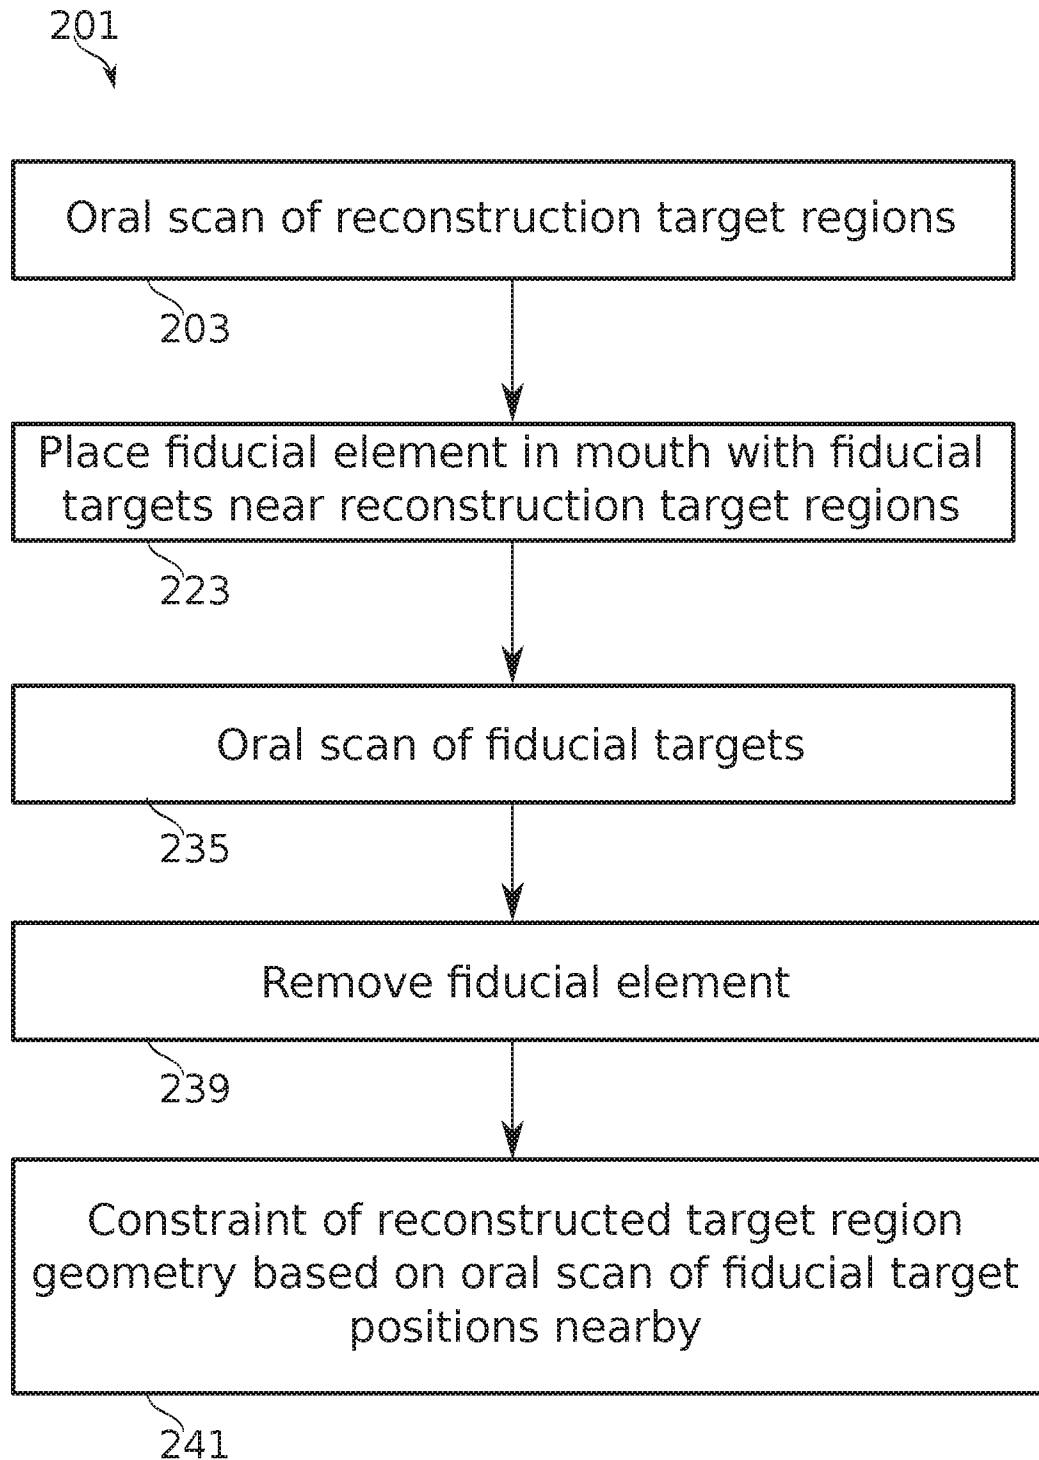


FIGURE 4B

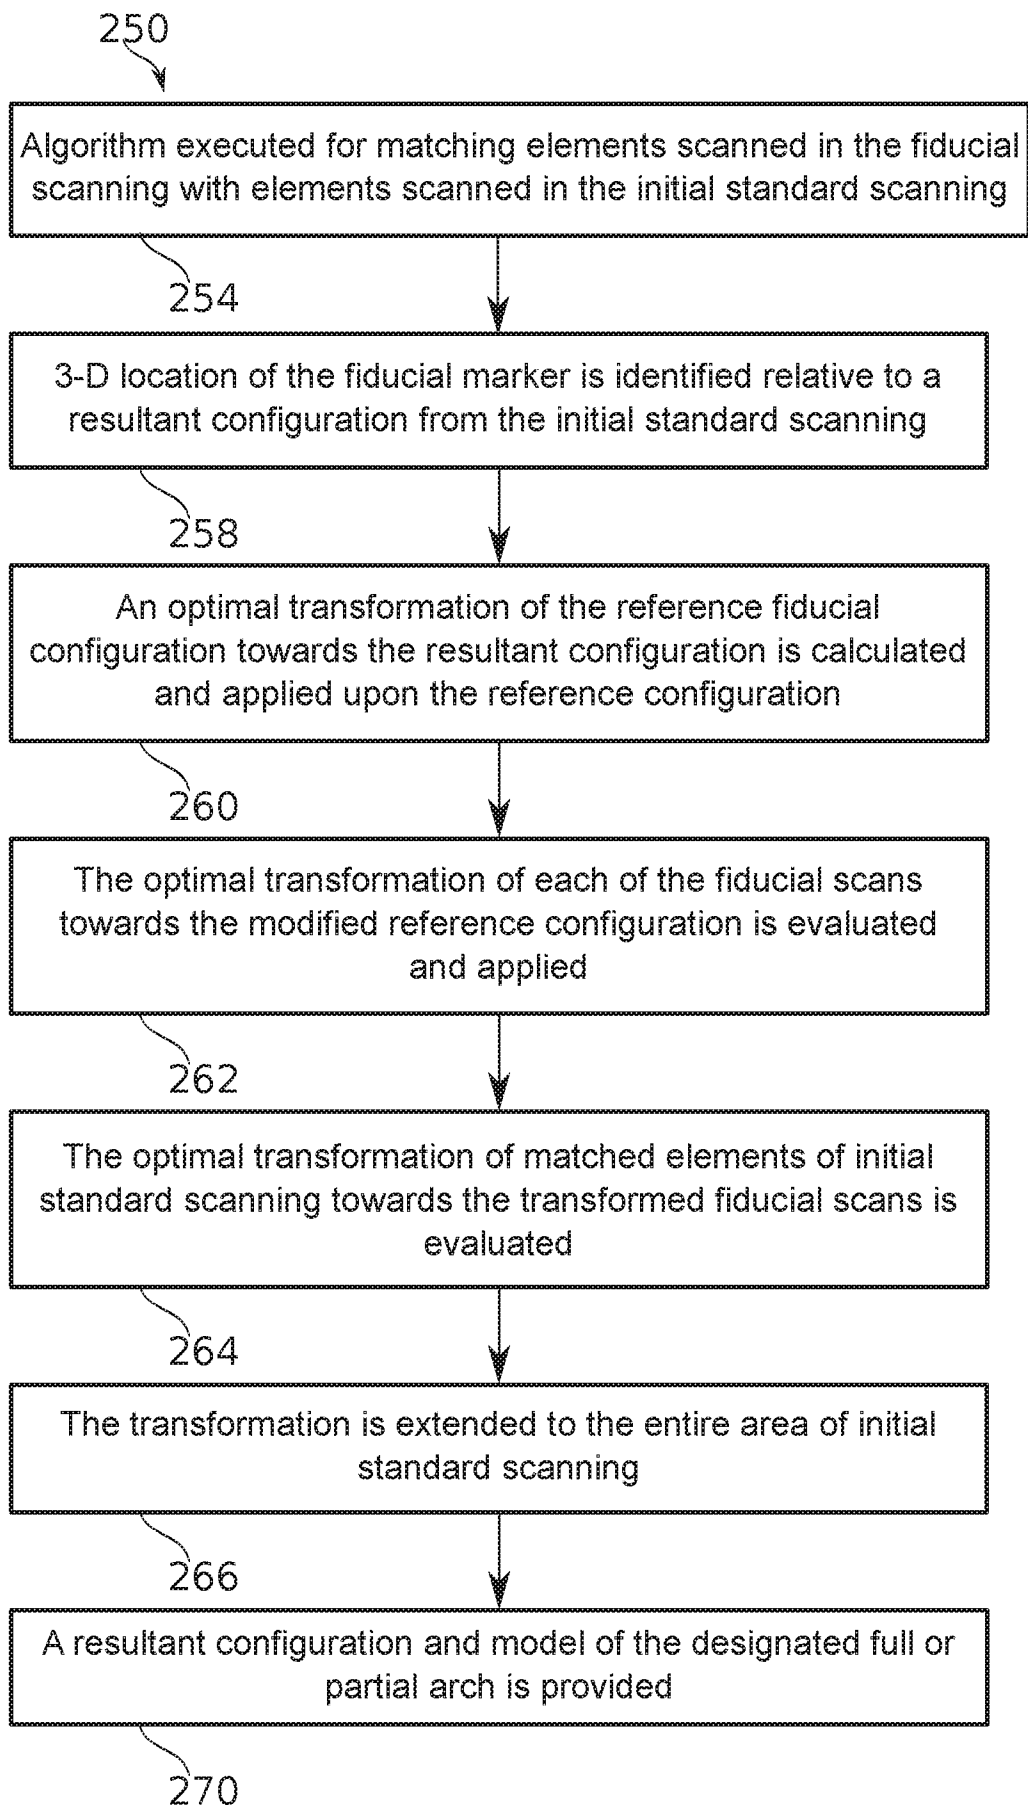


FIGURE 5A

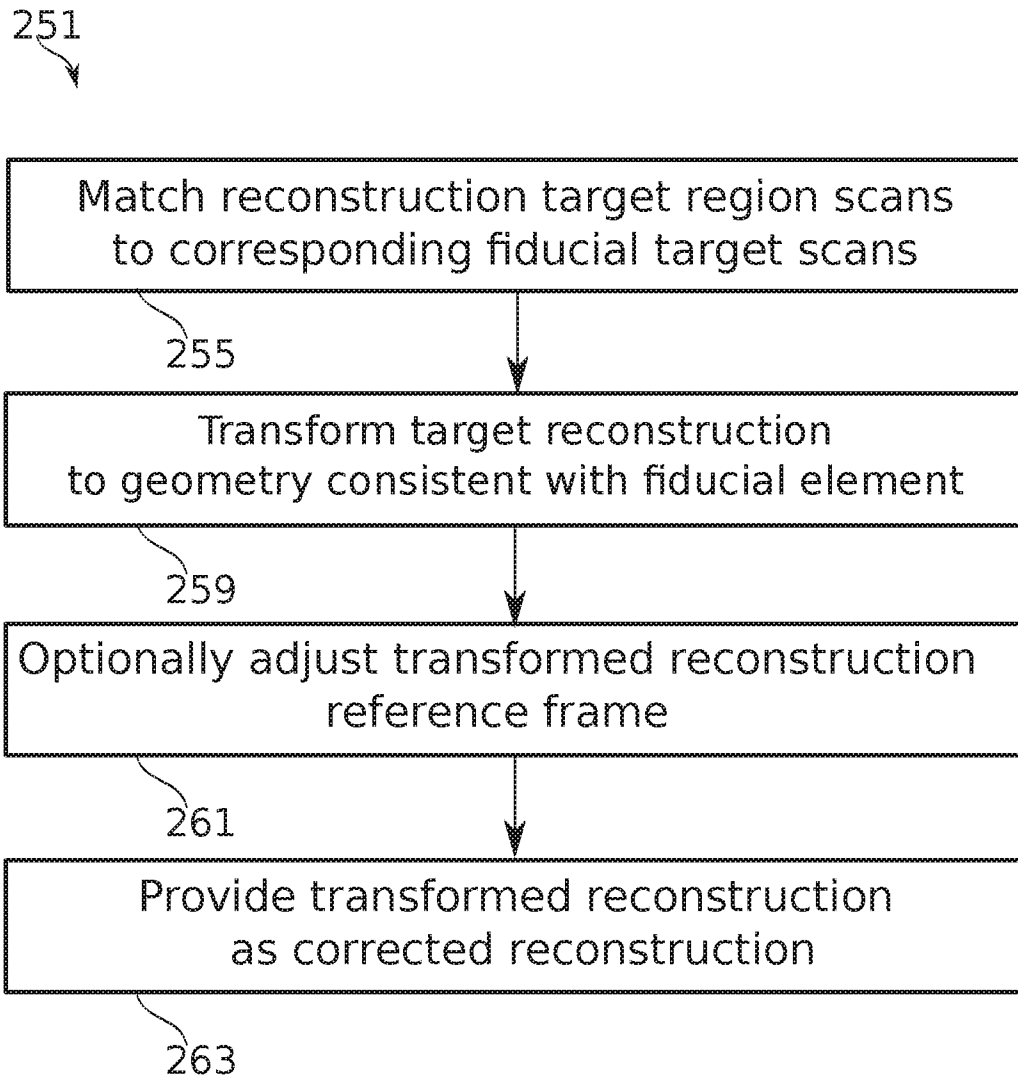


FIGURE 5B

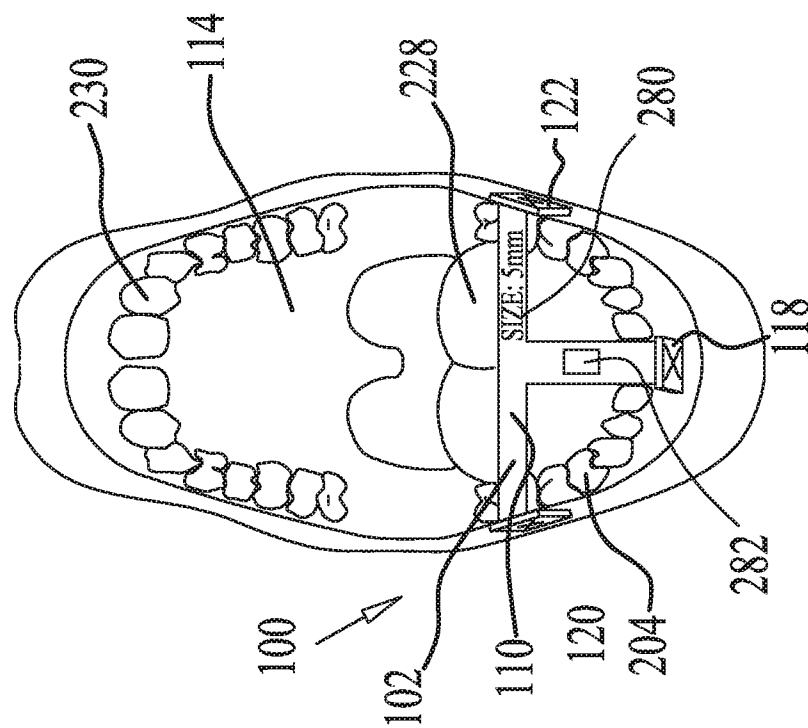


FIGURE 6

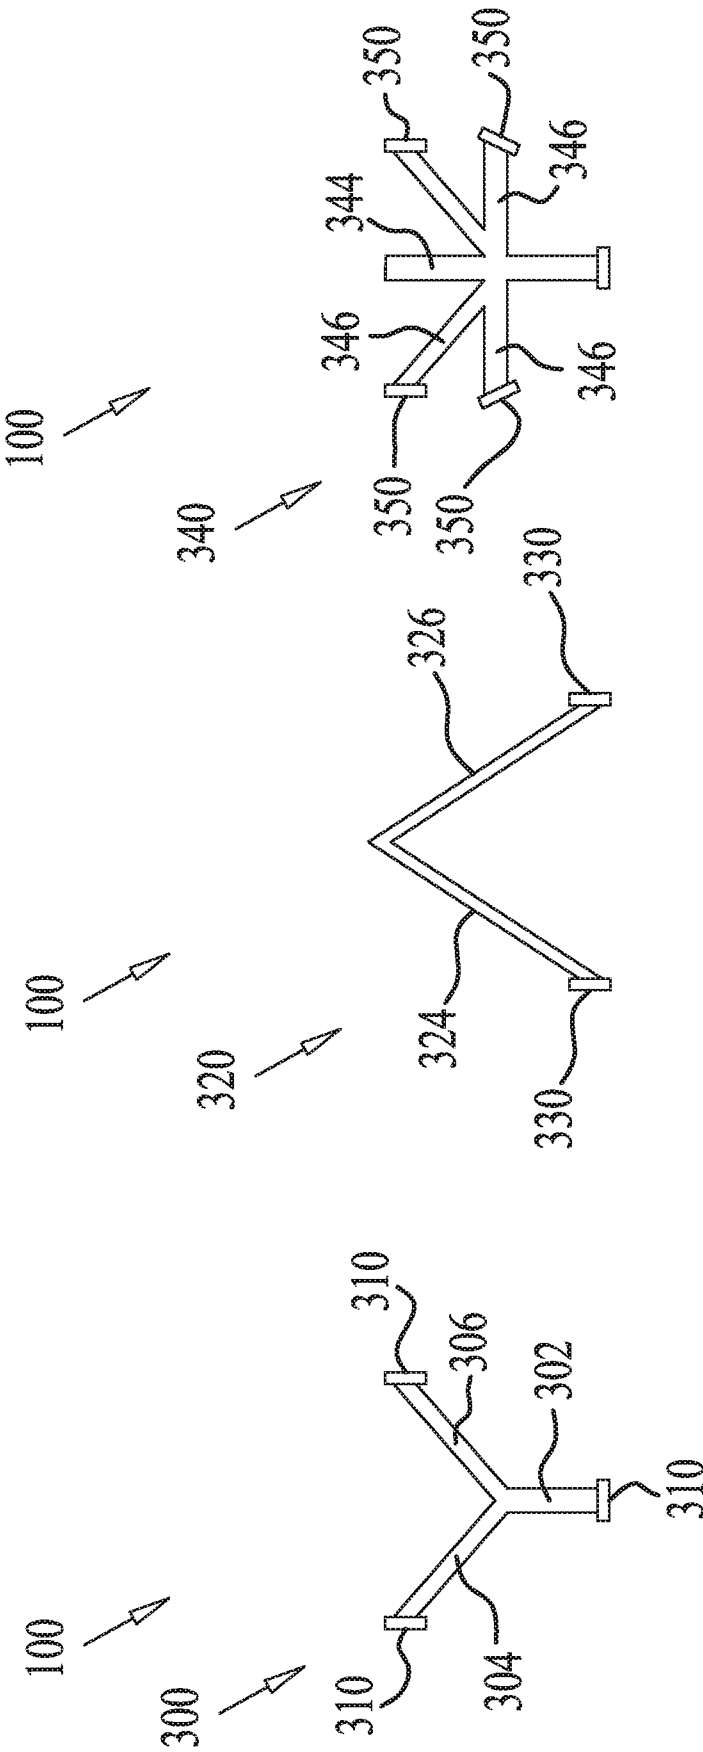


FIGURE 7C

FIGURE 7B

FIGURE 7A

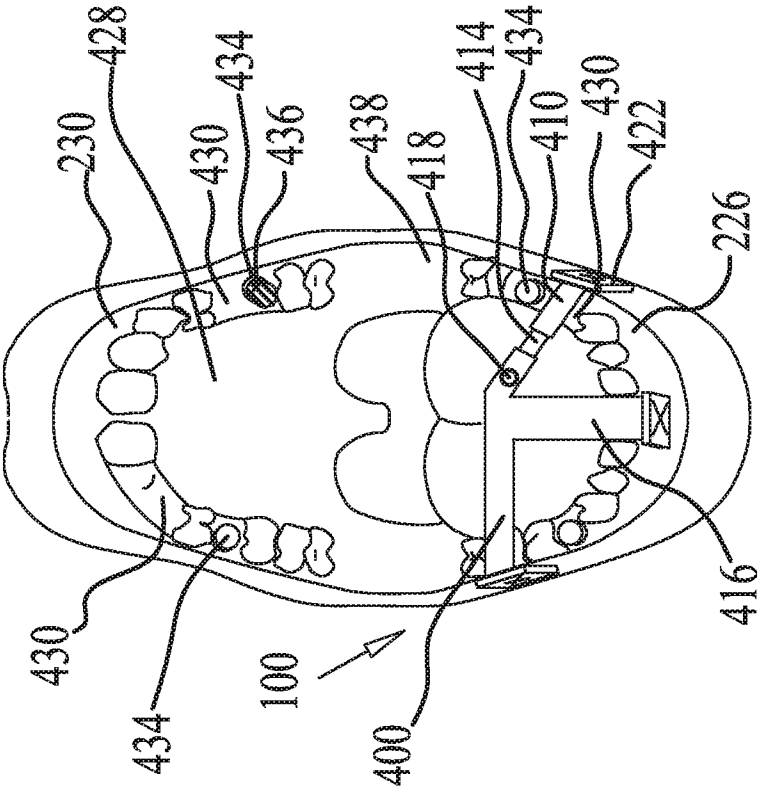


FIGURE 9

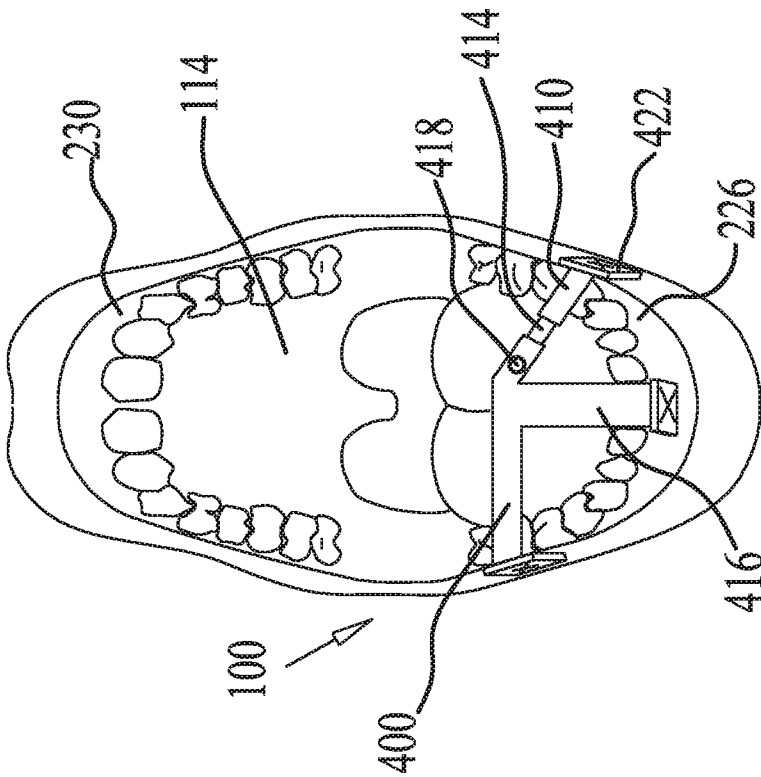


FIGURE 8

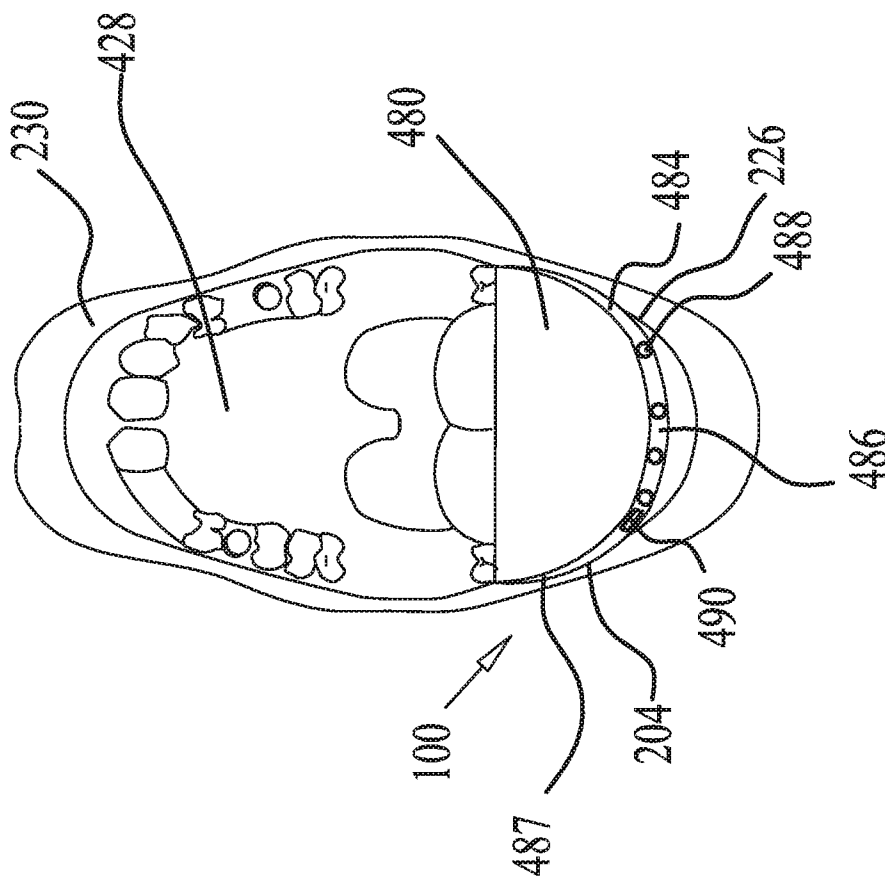


FIGURE 11

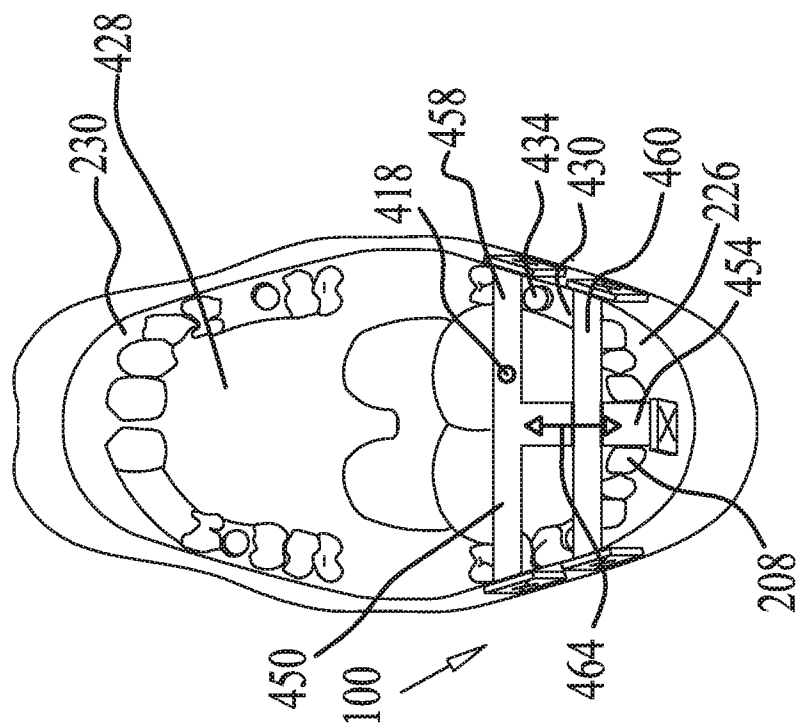


FIGURE 10

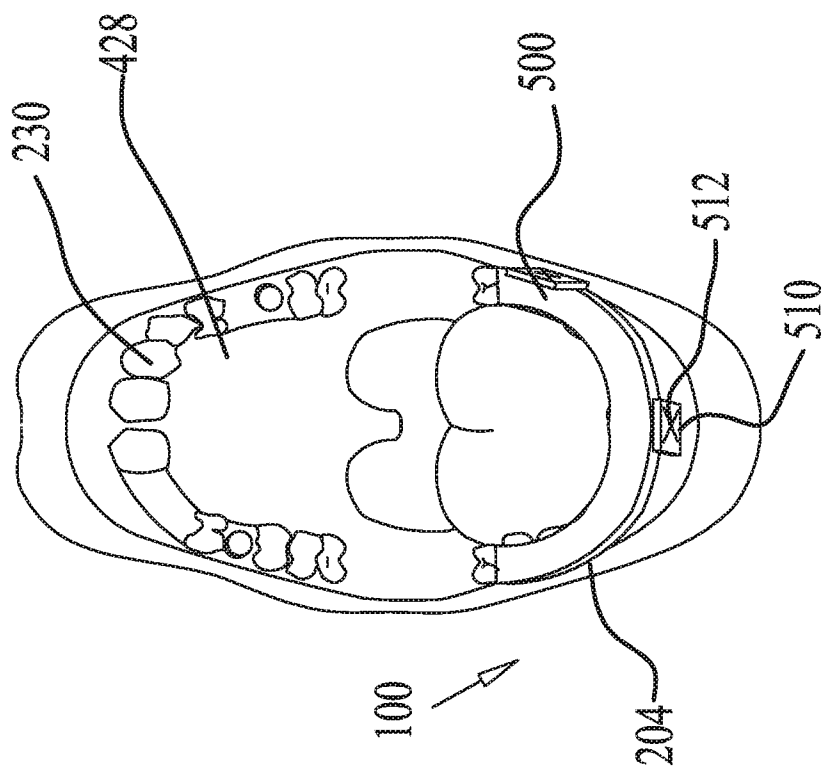


FIGURE 13

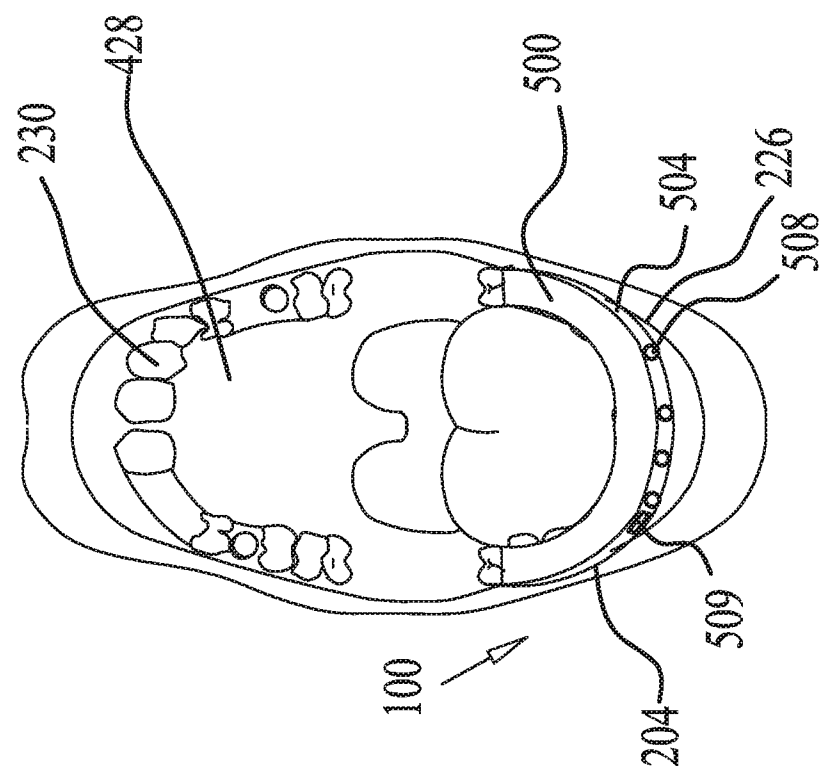


FIGURE 12

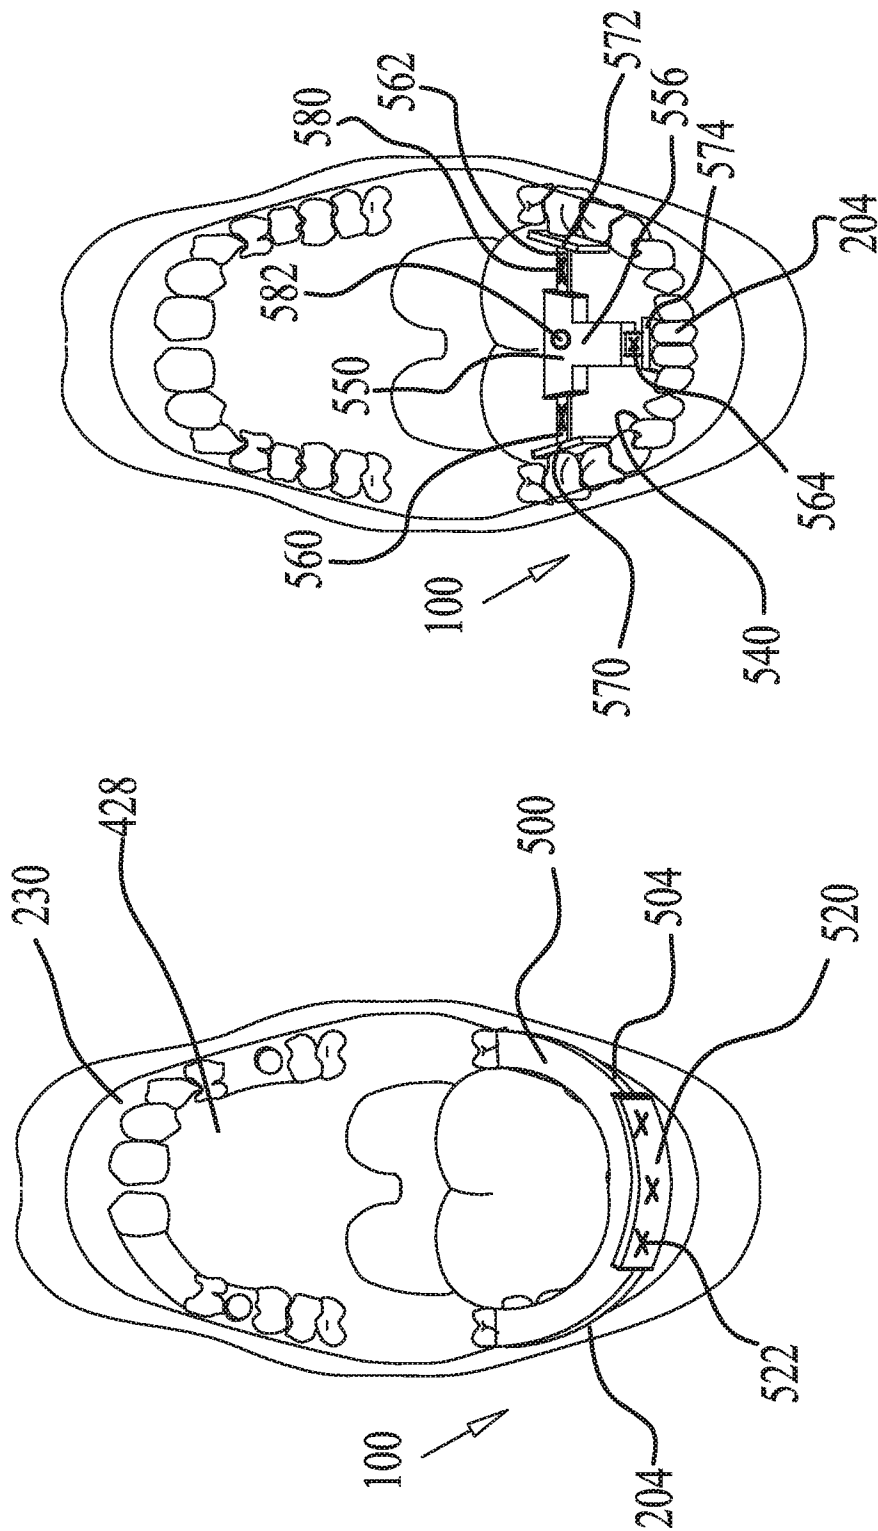


FIGURE 15

FIGURE 14

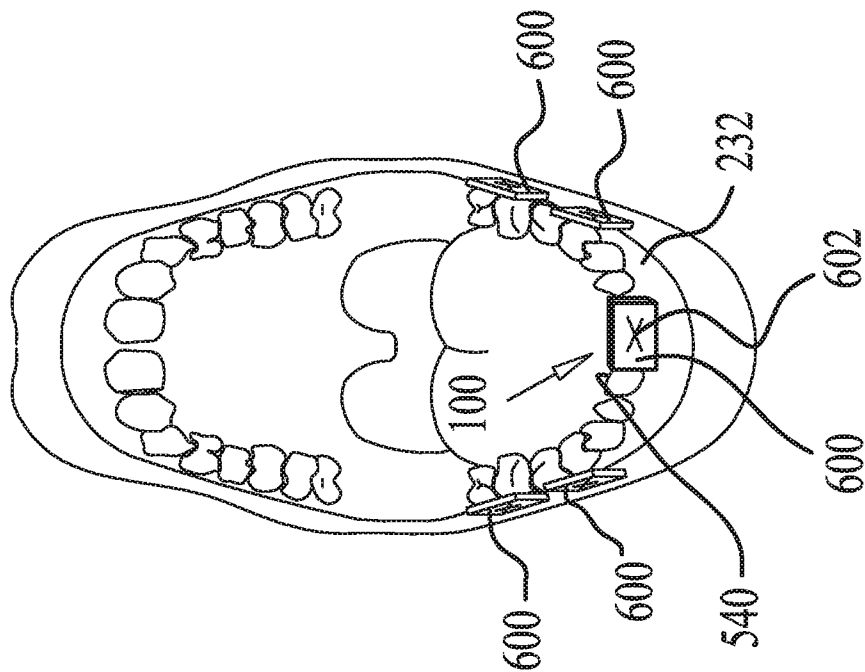


FIGURE 16

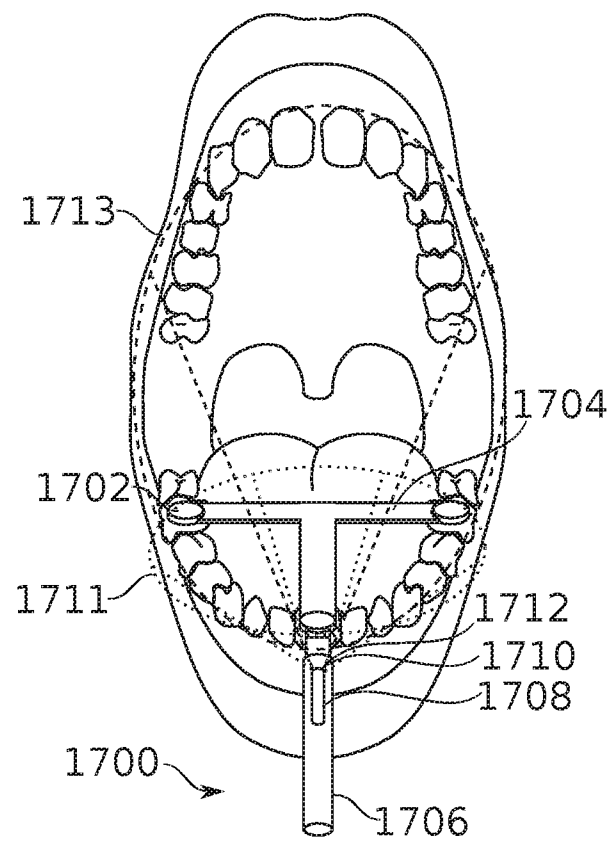


FIGURE 17A

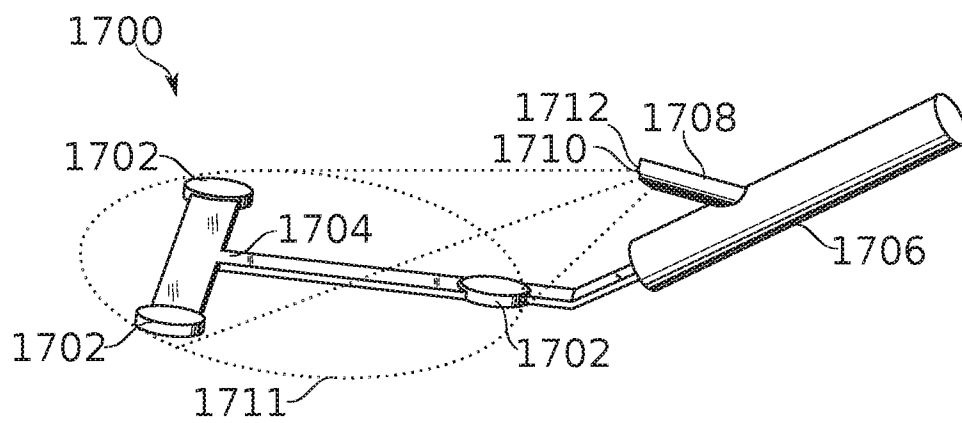


FIGURE 17B

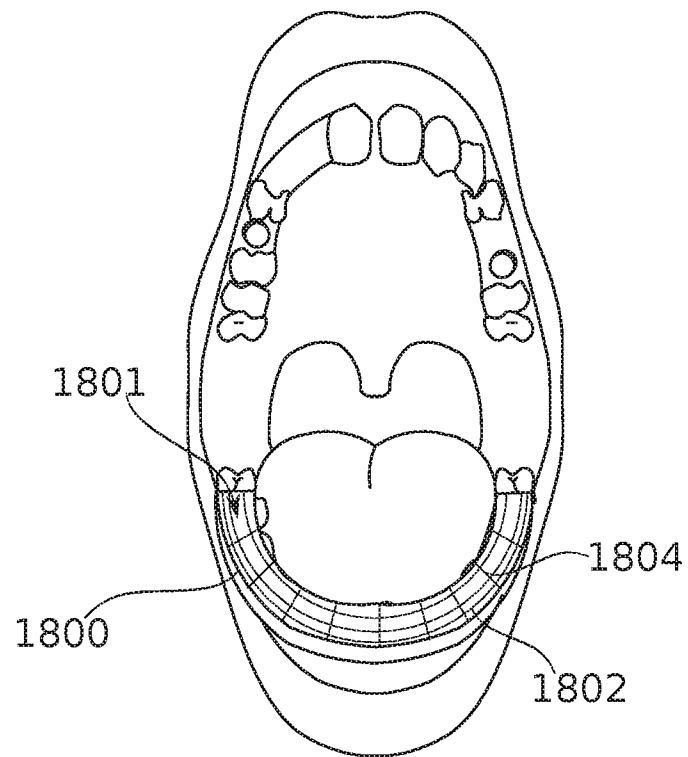


FIGURE 18

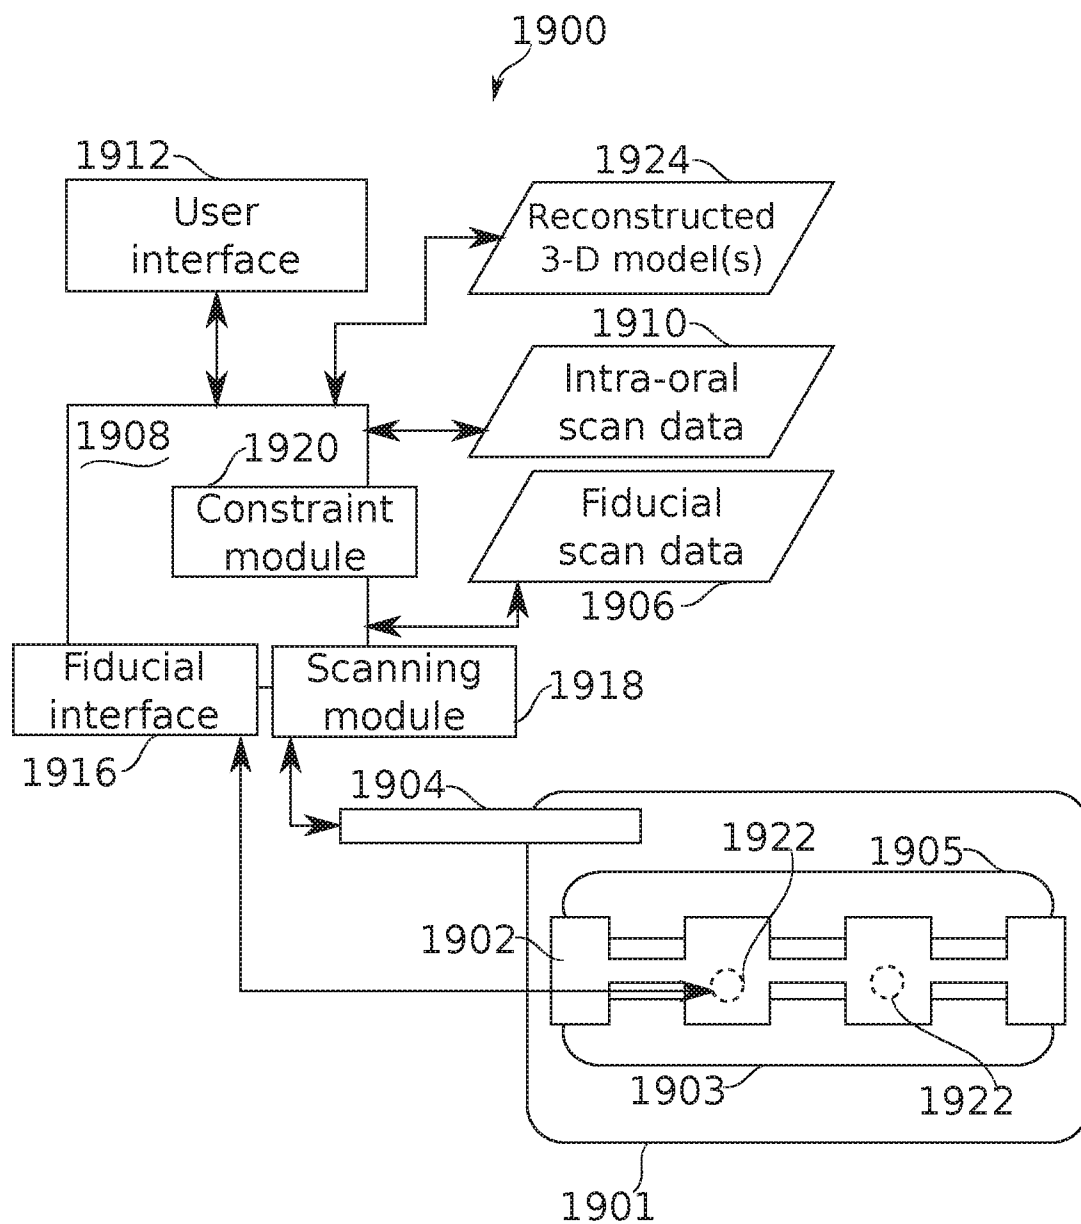


FIGURE 19

INTERNATIONAL SEARCH REPORT

International application No.

PCT/IL2016/050023

A. CLASSIFICATION OF SUBJECT MATTER IPC (2016.01) A61C 9/00, A61B 6/14 According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) IPC (2016.01) A61C, A61B Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) Databases consulted: FamPat database, PatBase		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2013/0273492 A1 (BIOMET 3I, LLC) 17 Oct 2013 (2013/10/17) the whole document (particularly, figures 4, 5B, 6A)	1,9,14-22,24,25, 27-29,44,45,48,50
Y		2-8,23-25
X	US 2010/0268071 A1 (IMAGNOSIS INC.) 21 Oct 2010 (2010/10/21) the whole document (particularly, figure 13)	27-31,34-36,40,41, 44
Y		2-8
Y	US 2008/0002869 A1 (ATLANTIS COMPONENTS, INC.) 03 Jan 2008 (2008/01/03) Abstract; paragraphs [0015], [0021], [0053], [0054], [0058]	23-25
A	WO 2014/020247 A1 (CHAMPLEBOUX G.) 06 Feb 2014 (2014/02/06) the whole document	1-50
☐ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents: "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family		
Date of the actual completion of the international search 20 Apr 2016		Date of mailing of the international search report 21 Apr 2016
Name and mailing address of the ISA: Israel Patent Office Technology Park, Bldg.5, Malcha, Jerusalem, 9695101, Israel Facsimile No. 972-2-5651616		Authorized officer SEGAL Liviu Telephone No. 972-2-5651782

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2016/050023

Patent document cited search report			Publication date	Patent family member(s)			Publication Date
US	2013/0273492	A1	17 Oct 2013	US	2013273492	A1	17 Oct 2013
				US	9198627	B2	01 Dec 2015
				AU	2013249682	A1	23 Oct 2014
				CA	2869222	A1	24 Oct 2013
				EP	2838464	A1	25 Feb 2015
				JP	2015516856	A	18 Jun 2015
				US	2016051346	A1	25 Feb 2016
				WO	2013158432	A1	24 Oct 2013
US	2010/0268071	A1	21 Oct 2010	US	2010268071	A1	21 Oct 2010
				US	9008755	B2	14 Apr 2015
				CN	101902966	A	01 Dec 2010
				CN	101902966	B	24 Jul 2013
				EP	2233078	A1	29 Sep 2010
				JP	2009142561	A	02 Jul 2009
				JP	5250251	B2	31 Jul 2013
				KR	20100110785	A	13 Oct 2010
				WO	2009078424	A1	25 Jun 2009
US	2008/0002869	A1	03 Jan 2008	US	2008002869	A1	03 Jan 2008
				US	7551760	B2	23 Jun 2009
				AT	539418	T	15 Jan 2012
				AU	2003237245	A1	12 Dec 2003
				AU	2006269977	A1	25 Jan 2007
				AU	2006269977	B2	22 Oct 2009
				BR	PI0613627	A2	18 Jan 2011
				CA	2615482	A1	25 Jan 2007
				CN	101228556	A	23 Jul 2008
				CN	101228556	B	06 Jun 2012
				EP	1512124	A1	09 Mar 2005
				EP	1512124	A4	05 Jan 2011

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/IL2016/050023

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		EP 1904978 A1	02 Apr 2008
		EP 1904978 B1	28 Dec 2011
		EP 2431944 A1	21 Mar 2012
		EP 2620912 A2	31 Jul 2013
		EP 2620912 A3	07 Aug 2013
		ES 2380547 T3	16 May 2012
		JP 2009501616 A	22 Jan 2009
		JP 5011292 B2	29 Aug 2012
		KR 20080034472 A	21 Apr 2008
		KR 101279292 B1	26 Jun 2013
		US 2003219148 A1	27 Nov 2003
		US 6925198 B2	02 Aug 2005
		US 2006072810 A1	06 Apr 2006
		US 7362890 B2	22 Apr 2008
		WO 03100729 A1	04 Dec 2003
		WO 2007011909 A1	25 Jan 2007
WO 2014/020247 A1	06 Feb 2014	WO 2014020247 A1	06 Feb 2014
		CA 2880281 A1	06 Feb 2014
		CN 104684484 A	03 Jun 2015
		EP 2879585 A1	10 Jun 2015
		FR 2994076 A1	07 Feb 2014
		JP 2015527129 A	17 Sep 2015
		US 2015196372 A1	16 Jul 2015