



(51) International Patent Classification:

A61B 5/026 (2006.01) *A61B 5/1459* (2006.01)
A61B 5/0476 (2006.01) *A61B 6/00* (2006.01)
A61B 5/1455 (2006.01) *G01J 3/40* (2006.01)

(21) International Application Number:

PCT/US2016/026920

(22) International Filing Date:

11 April 2016 (11.04.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/145,087 9 April 2015 (09.04.2015) US

(71) Applicant: THE GENERAL HOSPITAL CORPORATION [US/US]; 55 Fruit Street, Boston, MA 02114 (US).

(72) Inventors: **BOAS, David**; 188 Highland Avenue, Winchester, MA 01890 (US). **SUTIN, Jason**; 36 Highland Ave. #22, Cambridge, MA 02139 (US). **FRANCESCHINI, Maria, Angela**; 188 Highland Avenue, Winchester, MA 01890 (US).(74) Agent: **COOK, Jack, M.**; Quarles & Brady LLP, 411 E. Wisconsin Ave., Milwaukee, WI 53202 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: SYSTEM AND METHOD FOR NON-INVASIVELY MONITORING INTRACRANIAL PRESSURE

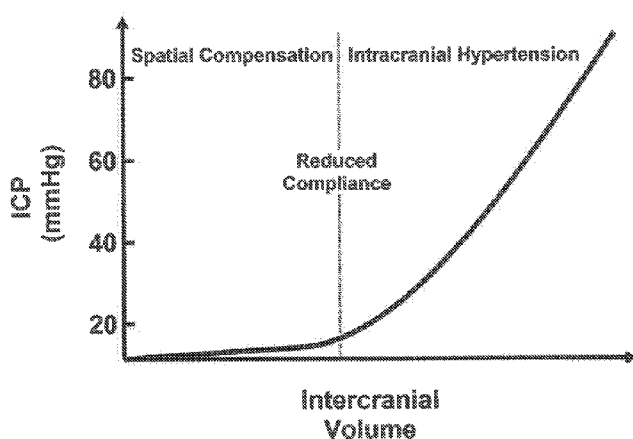


FIG. 1

(57) Abstract: A system and method for non-invasively monitoring intracranial pressure are provided. In some aspects, the method comprises acquiring diffuse correlation spectroscopy data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of a subject using one or more optical sensors placed about a subject, and determining a pulsatile cerebral blood flow using the acquired data. The method also includes correlating the determined pulsatile cerebral blood flow with physiological data acquired from the subject, and estimating an intracranial pressure based on the correlation. The method further includes generating a report indicative of the estimated intracranial pressure.

**SYSTEM AND METHOD FOR NON-INVASIVELY
MONITORING INTRACRANIAL PRESSURE**

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is based on, claims the benefit of, and incorporates herein in its entirety, U.S. Provisional Patent Application Serial No. 62/145,087 filed on April 9, 2015, and entitled "SYSTEMS AND METHODS FOR MEASURING TISSUE PRESSURE."

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH

[0002] This invention was made with government support under P41-EB015896, R01-HD042908, and R01-EB001954 awarded by the National Institutes of Health. The government has certain rights in the invention.

BACKGROUND

[0003] The disclosure relates generally to systems and methods for measuring tissue properties using diffuse correlation spectroscopy (DCS). More particularly, the disclosure is directed to systems and methods for non-invasively measuring intracranial pressure, and other related parameters.

[0004] Unlike the other organs of the body, the tissue pressure of the brain is not coupled to atmospheric pressure. Instead, the brain experiences a unique intracranial pressure determined by the volume of brain tissue, cerebrospinal fluid, and intracerebral blood enclosed within a fixed volume confined by the rigid, non-expandable skull:

$$V_{Intracranial} = V_{tissue} + V_{CSF} + CBV. \quad (1)$$

[0005] Under normal circumstances, small increases in the volume of one of these components is compensated by reductions in the others to maintain intracranial pressure within normal ranges through a process known as spatial compensation. Spatial compensation is possible because, in the absence of injury or disease, cerebral spinal fluid freely flows between the cranial and spinal compartments and epidural venous blood is easily expelled from the spinal canal. Thus, some amounts of blood or cerebral spinal fluid can redistribute as necessary between cranial and extra-cranial regions of the dural sac. Furthermore, compensation of the total volume of cerebral spinal fluid can occur

by alteration of the rate of cerebral spinal fluid absorption.

[0006] When spatial compensation is insufficient or compromised, the constituents of the cranio-spinal system have limited capacities for compression under pressure, leading to an intracranial volume that is actually partially elastic, rather than fully rigid:

$$V_{Intercranial} = V_{equilibrium} + V_{elastic} \quad (2)$$

[0007] where $V_{equilibrium}$ is the intracranial volume under normal intracranial pressure and $V_{elastic}$ is the change in volume of the craniospinal system due to changes exceeding accommodation by spatial compensation. In infants, deformation of the compliant immature skull allows further elasticity. Cerebral compliance, defined by $\Delta V/\Delta P$, represents the rigidity of the craniospinal compartment and is an indicator of the compensatory reserve for buffering changes in volume. Compliance is not constant but decreases with increasing pressure and can be impaired by pathology.

[0008] In pathological conditions such as traumatic brain injury (TBI), a cascade of events including brain swelling, vascular engorgement, obstruction of cerebrospinal fluid, edema, and/or intracranial hemorrhage, can exhaust compensatory mechanisms and lead to an exponential increase in intracranial pressure, as shown in FIG. 1. Compared to normal intracranial pressures typically around 10 mmHg, intracranial pressures in the range between 11-20 mmHg, 21-40 mmHg, and greater than 40 mmHg, representing slightly increased, moderately increased and severely increased values, respectively, pose an increasing risk for clinical complications. For instance, elevated intracranial pressures can dangerously reduce cerebral perfusion pressure and cerebral blood flow, causing ischemic brain injury (FIG. 2A). Since cerebral compliance decreases with increasing intracranial pressure, similar sized volume changes, including pulsatile blood volumes, result in larger changes in pressure. The risk is greatest when cerebral perfusion pressure is driven outside of the range of cerebral autoregulation, where cerebral blood flow is uncontrolled and passively follows pressure. Furthermore, the autoregulatory region can be reduced and shifted by both chronic and acute pathology (FIG. 2B). For example, in chronic hypertension or sleep apnea, vessels adapt to higher pressures or elevated

paCO₂, shifting basal vessel tone, reducing the range of autoregulated cerebral vascular resistance, and raising the cerebral perfusion pressure ischemic limit.

[0009] Perfusion reserve is the difference between measured cerebral perfusion pressure and the lower pressure limit of autoregulation and is an important clinical indicator for assessing risk of ischemic injury. For example, in managing intracerebral hemorrhage, interventions lowering blood pressure may lead to undesirable ischemia, while maintaining blood pressure may lead to hyperemia and the risk of hematoma expansion. Determining perfusion reserve can help to maintain optimal cerebral blood flow, limiting risk and achieving better outcomes. Increased intracranial pressure can also cause serious injury or death through physical extrusion of brain tissue through rigid extra-cerebral features such as the dura mater tentorium or foramen magnum and/or compression of the brain stem. Decreased intracranial pressure can cause hemorrhage or even ventricle collapse, with greatest risk occurring during interventions such as cerebrospinal fluid drainage.

[0010] Because increased intracranial pressure is an important cause of secondary brain injury, and its degree and duration is associated with poorer outcomes, monitoring intracranial pressure is recommended for the management of a wide range of disorders. For example, these may include traumatic brain injury, intra-cerebral and subarachnoid hemorrhage, hydrocephalus, benign intracranial hypertension, cerebral edema, stroke, meningitis, central nervous system infections, acute liver failure, hepatic encephalopathy, and so forth. Continuous monitoring of intracranial pressure to guide the clinical management of patients is associated with significantly improved outcomes.

[0011] Since its first use in the 1950's, intracranial pressure has been measured invasively using an intracranial catheter inserted into the lateral ventricle, via a small hole burred through the skull, and connected to an external pressure transducer. This method is accurate and low-cost, and also accommodates therapeutic cerebrospinal fluid drainage and administration of drugs. However, it is an invasive procedure that can be associated with complications, including hemorrhage and infection. Moreover, in some situations, such as patients having idiopathic intracranial hypertension,

anticoagulation, sepsis, liver disease, or aerospace travel in microgravity environments, this invasive procedure is not appropriate.

[0012] Development of non-invasive monitoring of intracranial pressure is recognized as an urgent need to avoid the complications of invasive procedures and to extend diagnostics to patients whose risk may be substantial but not enough to justify an invasive procedure. In addition, non-invasive intracranial pressure measurements could be used to identify patients needing invasive procedures, as well as to provide important information in the critical periods. In some applications, a combination of non-invasive and invasive intracranial pressure monitoring could also be beneficial. This is because often the reliability of invasive monitors is impaired for structural reasons, such as the presence of a ventricular drain, or due to artifacts like sensor fouling. As such, redundant non-invasive sensors would be a valuable adjunct. A non-invasive monitor of ICP and related cerebral measures, such as cerebral vascular resistance, cerebral perfusion pressure, vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling and cerebral compliance, dynamic autoregulation, cerebral perfusion reserve, and others, would also create many new applications in areas where invasive monitoring is not appropriate.

[0013] As a result, significant research efforts have been aimed towards the development of noninvasive methods to measure intracranial pressure using transcranial Doppler ultrasonography, tympanic membrane displacement, optic nerve sheath diameter, fundoscopy, computed tomography and magnetic resonance imaging. However, none of these techniques can be performed continuously at the bedside, and none have yet achieved the accuracy required to become routine clinical practice.

[0014] One widely used approach for estimating ICP has included determining a pulsatility index using transcranial Doppler ultrasonography measurements. The principle behind it is that the pulsatility of blood flow velocity through cerebral arterial vessels reflects distal cerebrovascular resistance, and hence intracranial pressure. As such, many have suggested utilizing the pulsatility index to estimate the intracranial pressure and cerebral perfusion pressure. However, the pulsatility index is not dependent solely on

cerebrovascular resistance, but is dependent on the interplay between cerebral perfusion pressure, pulse amplitude of arterial blood pressure, cerebrovascular resistance, compliance of the cerebral arteries and heart rate. As such, the pulsatility index is not an accurate estimator of intracranial pressure due to the confounding contributions.

[0015] Also, the accuracy of the pulsatility index determined using transcranial Doppler ultrasonography also strongly depends on ultrasound probe position and uniform insonation of the middle cerebral artery. In addition, in approximately 10–15% of patients, ultrasound cannot penetrate the skull. In these cases, transcranial Doppler ultrasonography cannot provide usable measurements. Furthermore, transcranial Doppler ultrasonography cannot be used as a continuous monitor because of the rigid and bulky transducer utilized.

[0016] Near-infrared spectroscopy, on the other hand, can monitor regional cerebral blood volume and hemoglobin oxygenation (SO_2) continuously at the bedside. As a result, near-infrared spectroscopy has been used to estimate cerebrovascular reactivity indices, which correlate with intracranial pressure. However, these measurements are not sufficiently independent from other hemodynamic parameters to provide accurate measures of intracranial pressure.

[0017] Consequently, considering the limitations of previous technological approaches, systems and methods capable of non-invasively and accurately measuring intracranial pressure, due to pathological and other medical conditions, are highly desirable.

SUMMARY

[0018] The present disclosure overcomes the aforementioned drawbacks by providing a system and method for accurately and non-invasively monitoring patients. More specifically, the system and method described herein utilizes diffuse correlation spectroscopy to measure pulsatile, as well as steady, cerebral blood flow for determining parameters useful in the diagnosis and management of patients. In particular, the system and method provided herein can be used to measure intracranial pressure, and other parameters, such as cerebral perfusion pressure, vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling and cerebral compliance, dynamic autoregulation, and cerebral

perfusion reserve.

[0019] As will be described, the present approach may not only provide valuable information, on a continuous basis, for administering acute care at a patient bedside or in an ambulance, but also provide information for analyzing complex pathophysiology, identifying new therapeutic opportunities, and, in general, substantially improving neurocritical care management. In some applications, the present approach may be used in the diagnosis, monitoring and treatment of traumatic brain injury or concussions, as well as other brain conditions.

[0020] In one aspect of the disclosure, a system is provided for non-invasively monitoring intracranial pressure. The system includes an optical coupling system configured to transmit and receive light signals from one or more locations about a subject and an optical processing system configured to generate diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of the subject using the transmitted and received light signals. The system also includes a computer programmed to receive the DCS data, analyze the DCS data to determine a pulsatile cerebral blood flow, and correlate the determined pulsatile cerebral blood flow with physiological data acquired from the subject. The computer is also programmed to estimate an intracranial pressure based on the correlation and generate a report indicative of the estimated intracranial pressure.

[0021] In another aspect of the disclosure, a method for non-invasively estimating intracranial pressure is provided. The method includes acquiring diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of a subject using one or more optical sensors placed about the subject, and determining a pulsatile cerebral blood flow using the acquired data. The method also includes correlating the determined pulsatile cerebral blood flow with physiological data acquired from the subject, and estimating an intracranial pressure based on the correlation. The method further includes generating a report indicative of the estimated intracranial pressure.

[0022] In yet another aspect of the disclosure, a method for non-invasively

monitoring a subject using a monitoring system is provided. The method includes acquiring diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of a subject using one or more optical sensors placed about the subject, and determining a pulsatile cerebral blood flow using the acquired data. The method also includes correlating the determined pulsatile cerebral blood flow with physiological data acquired from the subject using physiological sensors, and estimating at least one parameter based on the correlation. The method further includes generating a report indicative of the at least one parameter estimated.

[0023] The foregoing and other aspects and advantages of the invention will appear from the following description. In the description, reference is made to the accompanying drawings which form a part hereof, and in which there is shown by way of illustration a preferred embodiment of the invention. Such embodiment does not necessarily represent the full scope of the invention, however, and reference is made therefore to the claims and herein for interpreting the scope of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] FIG. 1 is a graph showing a relationship between intracranial volume and pressure.

[0025] FIG. 2A is a graphical illustration showing clinical zones of cerebral perfusion relative to intracranial pressure.

[0026] FIG. 2B is a graph showing changes in the optimal perfusion due to certain medical conditions.

[0027] FIG. 3 is a graph illustrating the relationship between pulsatile blood flow and arterial blood pressure.

[0028] FIG. 4A is an illustration showing transmural pressure across a blood vessel wall.

[0029] FIG. 4B is an illustration showing perfusion pressure along a blood vessel.

[0030] FIG. 4C is an illustration showing tension around a blood vessel wall.

[0031] FIG. 5 is a schematic diagram of a model indicating vascular

elements affecting cerebral perfusion.

[0032] FIG. 6 is a diagram of an example monitoring system, in accordance with aspects of the present disclosure.

[0033] FIG. 7 is a graphical illustration showing acquisition, gating and averaging of photon count data, in accordance with aspects of the present disclosure.

[0034] FIG. 8 is a flowchart setting forth steps of a process in accordance with aspects of the present disclosure.

[0035] FIG. 9 is a graph showing how the critical closing pressure is influenced by wall tension.

[0036] FIG. 10 is a graphical illustration showing acquisition, gating, and averaging of pulsatile diffuse correlation spectroscopy (pDCS) data.

[0037] FIG. 11A is a graph showing simultaneous electrocardiograph (ECG), near infrared spectroscopy (NIRS) and pDCS data.

[0038] FIG. 11B is another graph showing simultaneous ECG, NIRS and pDCS data.

[0039] FIG. 11C is graph showing asynchronous cardiac cycle averaging.

[0040] FIG. 12 are graphs showing arterial blood pressure, intracranial pressure, and blood flow based on DCS data, simultaneously measured in an anesthetized rat.

DETAILED DESCRIPTION

[0041] The brain is enclosed in a rigid skull, and as a result, changes in intracranial pressure (ICP) affect cerebral blood flow (CBF), which can lead to serious medical conditions, such as cerebral ischemia. Therefore, intracranial pressure (ICP) monitoring is highly desirable for the diagnosis and treatment of patients with a wide range of medical conditions and disorders, including traumatic brain injury, intracerebral and subarachnoid hemorrhage, hydrocephalus, benign intracranial hypertension, meningitis, stroke, acute liver failure, and so forth.

[0042] Therefore, in accordance with aspects of the present disclosure, a system and a method for accurate, non-invasive monitoring of ICP based on diffuse correlation spectroscopy (DCS), are described herein. In particular, the

system and method can measure CBF and more specifically pulsatile cerebral blood flow (pCBF) to determine ICP, as well as other clinically relevant parameters, such as cerebral perfusion pressure (CPP), cerebrovascular resistance (CVR), vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling and cerebral compliance, dynamic autoregulation, cerebral perfusion reserve, and other parameters. This approach recognizes that the pressure-axis intercept in the pulsatile pressure-flow relationship curve (FIG. 3), namely the critical closing or zero flow pressure (CrCP), is directly related to ICP.

[0043] In particular, FIG. 3 is a graph showing an index of pulsatile cerebral blood flow (pCBFi) from cerebral vessels versus arterial blood pressure (ABP). As labeled, this graph shows that CrCP is present at zero pCBFi and that the pulsatility of blood from the diastolic to systolic results in a corresponding variation in pressure (ΔP) and variation in flow (ΔF). As will be described, the system and method of the present disclosure are able to acquire DCS data at a speed, or temporal resolution sufficient to determine pCBF and use pCBF and other measures to non-invasively determine clinically-useful information with an accuracy and precision that has not previously been available using non-invasive systems. For example, as will be described, the system and method of the present disclosure are capable of acquiring and processing multiple DCS measurements per second to, thereby, achieve a speed, or temporal resolution, to determine pulsatile information and create accurate measures not achieved or recognized in non-invasive systems previously. This stands in contrast to traditional DCS systems and methods that, for example, have a sampling time for DCS measurements of approximately 1.5 seconds or longer.

[0044] Also, the present approach can be used for non-invasive continuous monitoring over extended periods of time with minimized interference or discomfort to a patient. As such, the provided system and method may be suitable for continuous or discrete measurements in a much larger population including adults, children, infants, neonates, and premature infants. This includes patients not undergoing invasive procedures or those for whom an

invasive procedure might not be worth the risk. In addition, using the system and method described, measurements can be made on patients while conscious or unconscious, awake or sedated or anesthetized. In addition to humans, the provided system and method may be used with animals for research, commercial, and/or veterinary purposes. Furthermore, the present approach may also be used to measure perfusion pressure of other organs besides the brain.

[0045] Previous non-invasive techniques, such as near-infrared spectroscopy and transcranial Doppler ultrasonography, measure blood volume or blood flow velocity measurements, respectively, to estimate ICP. As described, these approaches rely on surrogate measurements, and include a variety of confounding factors that prevent accurate determination of ICP. For example, transcranial Doppler ultrasonography utilizes the middle cerebral artery, which averages the blood supply of many anatomically distinct regions, including those with less sensitivity to ICP. Accordingly, these systems are not able to accurately assess pulsatility and, thereby, are not able to provide accurate determinations of ICP.

[0046] By contrast, the present approach utilizes DCS to measure blood flow directly. In particular, DCS can be used to measure CBF in cortical microvessels, which have lower tension and are more sensitive to cranial pressure changes compared with larger arteries. Also, DCS can be used to measure CBF specifically within brain tissue, and overcome confounding factors of middle cerebral artery measurements. Furthermore, DCS provides a robust average of CBF over cm³-sized cortical volumes, without being sensitive to probe placement or orientation, as transcranial Doppler ultrasonography. Thus, the systems and methods are able to perform absolute calibration of blood flow, unlike other non-invasive systems and methods.

[0047] Primarily, two types of pressures act upon the cerebral vasculature to influence blood flow, namely transmural pressure and perfusion pressure, as illustrated in FIGs. 4A and 4B. Referring particularly to FIG. 4A, transmural pressure is the net pressure acting across the wall 402 of a blood vessel 400 resulting from an internal hydrostatic transmural pressure 404 and an external hydrostatic transmural pressure 406. Specifically, the internal hydrostatic

transmural pressure 404 is an outward pressure as a result of blood pressure. On the other hand, in the skull, the external hydrostatic transmural pressure 406 is primarily the intracranial pressure.

[0048] Classically, transmural pressure gives rise to Starling forces and drives transudate and exudate transport through blood vessel walls throughout the organs of the body. Transmural pressure is less associated with tissue blood perfusion. However, within the rigid confines of the skull, ICP-dominated transmural pressure can couple to the flow of blood through vessels via the elasticity of the vessels themselves.

[0049] When the transmural pressure is great enough to compress the flexible vessels, their internal diameters effectively decrease, and flow is impeded through the well-known Starling resistor phenomenon (FIG. 5). In the extreme, when transmural pressure becomes negative, the vessel will collapse and close entirely to flow. For example, externally generated negative transmural pressures are the basis for well-known sphygmomanometer measurements of blood pressure.

[0050] Perfusion pressure, on the other hand, is directly related to tissue perfusion and is defined as the difference in pressure between the vascular inflow and outflow within the vessel or vascular network. Referring specifically to FIG. 4B, the perfusion pressure across the blood vessel 400 is the difference between the inflow pressure 408 and outflow pressure 410. Furthermore, perfusion pressure is related to blood flow through the vascular resistance in a relationship with blood flow that is similar to Ohm's law. Under normal circumstances, vascular resistance is regulated under physiological control, including functional hyperemia, in response to PaCO_2 levels, and autoregulation. Pharmacological agents, injury and disease can also impact vascular resistance and its physiological control mechanisms.

[0051] The properties of blood vessels affect blood flow therethrough. Referring specifically to FIG. 4C, the wall tension 412 of a blood vessel 400 is shown a circumferential force within the wall 402. Wall tension 412 is related to the transmural pressure and the ratio of the internal radius 414 to the thickness 416 of the blood vessel 400. The wall tension 412 must be overcome for the blood

vessel 400 to close. For vessels with the ability to actively dilate and contract, the vessel diameter is under physiological control. Thus, the wall tension 412 is also referred to as vessel tone.

[0052] Since the cerebral vasculature is enclosed by the rigid confines of the skull, ICP applies a transmural pressure external to the blood vessels, as shown in the diagram of FIG. 5. Under normal conditions, the outflow pressure is dominated by central venous pressure (CVP) and the transmural ICP has little effect on CPP. However, when ICP exceeds CVP, the transmural pressure acts to constrict the vessels at flexible sites, such as bridging vessels on the surface of the brain and arterioles, as indicated by the arrows shown in FIG. 5. In this case, these sites act as Starling resistors, restricting flow and reducing CPP. Under these conditions, the zero flow pressure quantifies the magnitude of ICP.

[0053] Conceptually, perfusion pressure is both a direct measure of the adequacy of tissue perfusion and, via the limits of autoregulation, an estimate of the amount of perfusion reserve available to maintain homeostasis. However, in practice, CPP is a quantity inferred from other measurements since it is typically not practical to measure outflow pressure directly. Thus, quantities such as ICP have been preferred for clinical use, although their relationship to pathology, namely the risk of ischemia, is indirect.

[0054] Measurements of CPP and CBF both provide information on the amount of tissue perfusion and the risk of ischemia. However, CBF can vary physiologically over two fold without injury. For example, if cerebral vessels dilate, CBF will increase. At the same time, cerebral vascular resistance would decrease correspondingly. In the relationship for CPP, under physiological conditions these two factors will tend to cancel, leaving CPP relatively unchanged. Thus, CPP may have greater sensitivity to pathological conditions with less influence from normal physiological variations. Furthermore, CPP and CBF can be combined with other measures, such as oxygen saturation (SO_2), oxygen extraction fraction (OEF), cerebral blood volume (CBV), cerebral metabolic rate of oxygen ($CMRO_2$) to further quantify ischemic risk and perfusion reserve.

[0055] Under normal conditions, cerebral perfusion pressure can be

approximated as the difference between arterial pressure and central venous pressure. However, when ICP is sufficiently elevated, vascular resistance becomes dominated by Starling resistor effects and the effective outflow pressure is no longer CVP but ICP. Thus, ICP couples to CBF and measurements of CBF, either alone or in conjunction with other physiological measurements, can be used to determine ICP, risk of ischemia, loss of autoregulation and/or regulatory reserve, and/or other parameters.

[0056] Turning to FIG. 6, a block diagram is shown of an exemplary system 600 for non-invasive monitoring of a subject, in accordance with aspects of the present disclosure. As shown, the system 600 generally includes a number of sensors, including an optical coupling system 602 and physiological sensors 604, to be placed at various locations about a subject's body. The system 600 also includes an optical processing system 606 and one or more sensor system(s) 608 in communication with the physiological sensors 604. The optical processing system 606 and sensor system(s) 608 are in communication with a controller 610 that is configured control operation of the system 600, and systems therein, including data acquisition and processing.

[0057] The system 600 may operate autonomously or semi-autonomously, or in conjunction with other devices or hardware. The system 600 may also read executable software instructions from a non-transitory computer-readable medium (such as a hard drive, a CD-ROM, flash memory and the like), and may also receive instructions from a user, or any other source logically connected thereto, such as another networked computer or server, database, internet, cloud, and so forth.

[0058] The optical coupling system 602 may include a number of source probes 603 and detector probes 605 forming one or more optical sensors, including DCS sensors, and near infra-red spectroscopy (NIRS) sensors. In particular, the source probes 603 are configured to transmit light signals to the subject, while the detector probes 605 are configured to receive light signals therefrom. The source probes 603 and detector probes 605 can include single-mode and/or multi-mode optical fibers. The optical fibers may be straight fibers, 90° bent fibers, or side-firing fibers. The source probes 603 and detector probes

605 may be arranged in various configurations and separated by distances up to several centimeters. In some implementations, the optical coupling system 602 is configured for measuring blood flow in the brain, and optionally, blood flow in the skin, scalp, skull, and/or periphery.

[0059] The physiological sensors 604, controlled by the sensor systems(s) 608, may include electroencephalogram (EEG), electrocardiograph (ECG), blood pressure (BP), ICP, pulse oxymetry, and other sensors, configured to measure physiological parameters, including, but not limited to, hemoglobin concentrations, changes in hemoglobin concentrations, oxygen saturation, CMRO₂, invasive blood pressure, non-invasive blood pressure, intracranial pressure, brain activity, electrocardiogram, cardiac output, stroke volume, and combinations thereof. In some implementations, physiological sensors 604 and respective sensor system(s) 608 may be from a separate device from a different manufacturer.

[0060] Various sensors described with reference to the optical coupling system 602 and physiological sensors 604 may be incorporated into, or be part of, one or more items or units designed to engage with or couple to a subject at any number of locations, in any number of geometrical configurations. For example, various sensors may be integrated into silicone assemblies, bandages, headbands, and any other assemblies securable to the subject. Also, various sensors may be wearable or designed to attach to the subject directly using an adhesive.

[0061] Although FIG. 6 shows the optical coupling system 602 placed about a subject's head, and physiological sensors 604 placed about the subject's torso, it may be readily appreciated that the locations of the sensors can vary, in accordance with the signals being induced and sensed. For example, various physiological sensors 604 may be placed about the subject's head, arms, legs, and so forth. Similarly, optical sensors may be placed about the subject's arms, legs, torso, and so forth. As such, different sensors may be collocated, or individually placed at various positions about the subject.

[0062] The optical processing system 606 is in communication with the optical coupling system 602 includes a source module 612 configured to generate

light using one or more light sources. The source module 612 may be configured to operate in the continuous wave, frequency domain, and time domain. To this end, the source module 612 may be pulsed, sinusoidally modulated, step modulated, triangularly modulated, and/or arbitrarily modulated.

[0063] By way of example, the source module 612 may include a transform, or nearly-transform, limited picosecond pulsed source or a non-transform limited picoseconds pulsed source. As used herein, reference to "picosecond" pulses or pulsed source refers to pulses having a pulse width between 1 ps and 10 ns. The source module 612 may also include a Bragg reflector laser, a distributed Bragg feedback laser, a gain-switched distributed Bragg reflector laser, an external cavity laser, a gain-switched laser, a current pulsed laser, a mode-locked laser, a q-switched laser, combinations thereof, and the like. The source module 612 can also include a diode laser, a solid-state laser, a fiber laser, a vertical cavity surface-emitting laser (VCSEL), a Fabry-Perot laser, a ridge laser, a ridge waveguide laser, a tapered laser, a master oscillator power amplifier (MOPA) laser, or other type of laser. In certain aspects, the source module 612 can also include a swept source light source.

[0064] The source module 612 can be configured to transmit light into a target medium using wavelengths between 400 nm and 1500 nm, including but not limited to, a wavelength of between 600 nm and 1000 nm, or a wavelength of between 690 nm and 900 nm. The source module 612 can also be configured to transmit light into the target medium using average power between 10 μ W and 10 W, including but not limited to, an average power of between 100 μ W and 1 W, between 1 mW and 500 mW, or between 10 mW and 200 mW. The source module 612 can be configured to transmit light pulses into a target medium using pulse widths between 1 ps and 10 ns, including but not limited to, a pulse width of between 10 ps and 1 ns, or between 50 ps and 500 ps. Pulse widths described herein refer to full-width at half maximum pulse widths.

[0065] The optical processing system 606 also includes a detector module 614 in communication with the optical coupling system 602 which is configured to receive light signals from the subject and provide an output to a correlator 618 indicative of the received signals. For example, the detector module 614 may

include one or more photon-counting avalanche photodiodes (APDs) configured to provide photon counts based on detected light. As shown in FIG. 6, the optical processing system 606 may optionally include a number of optical elements 616 interposed between the optical coupling system 602, source module 612 and detector module 614. Specifically, the optical elements 616 may be configured for manipulating light signals transmitted to and received from the subject. Example optical elements 616 include lenses, prisms, holograms or diffractive optical elements, diffusers, attenuators, filters, optical fibers, and so forth.

[0066] In general, the controller 610 may be a computer, as shown in FIG. 6, that is programmed to carry out steps in accordance with aspects of the present disclosure, as will be described. The controller 610 may also be a workstation, a laptop, a mobile device, a tablet, a personal digital assistant (PDA), a multimedia device, a network server, a mainframe or any other general-purpose or application-specific computing device. Other examples for the controller 610 may also include system on a chip (SOC) a field-programmable gate array (FPGA), a complex programmable logic device (CPLD), an application-specific integrated circuit (ASIC), a Raspberry PI controller, and the like.

[0067] In some aspects, the controller 610 may be configured to acquire and process optical, physiological and other signals induced or generated by a subject, to estimate desired physiological parameters. Specifically, the controller 610 may be configured to receive and utilize DCS measurements to determine a pulsatile, as well as steady, cerebral blood flow from which a number of physiological parameters, including ICP, CPP, CRV, and so forth, may be estimated. In some aspects, the controller 610 may utilize characteristics of a pulsatile pressure-flow relationship curve, as described with reference to FIG. 3 to determine desired physiological parameters. For example, the critical closing or zero flow pressure (CrCP), or intercept may be used to is directly related to ICP. Additionally, a slope of the pulsatile pressure-flow relationship may also be utilized by the controller 610, as well as any other information obtained therefrom.

[0068] In some aspects, the controller 610 may be configured to acquire simultaneous or synchronous measurements, as well as separate measurements,

using various sensors placed on the subject, as described. Also, measurements may be made once, intermittently, periodic, continual, or continuously. The controller 610 may be configured to utilize signals from such measurements to construct various time series waveforms. For example, FIG. 7 shows acquisition of ECG data 702 and DCS data 704 as a function of time. The controller 610 may also be configured to assemble acquired signals into a frequency representation, as power spectra. As such, the controller 610 may be configured to apply a Fast Fourier Transform (FFT), for example, to the acquired signals. Other signal representations may also be generated by the controller 610, including signal derivatives, differentials, differences, and so forth. The controller 610 may also determine signal amplitudes, timing, phases, correlations, and so forth. Processing of signals by the controller 610 may be performed in real-time, near real-time, or by post-processing, either in the time or frequency domain or both.

[0069] In some aspects, the controller 610 of FIG. 6 may be configured to generate, by way of the correlator 618, correlation curves using acquired DCS data. In this manner, various desirable parameters, such as blood flow, and more specifically pulsatile blood flow, and others may be determined, as will be described. In particular, the correlator 618 may receive photon count data from the detector module 614 and calculate intensity autocorrelation functions at various time scales using the photon count data. Although the correlator 618 is shown in FIG. 6 as separate from the controller 610, it may be readily appreciated that these could be integrated into one system. For instance, the controller 610 may include various hardware and software for directly calculating intensity autocorrelation functions.

[0070] Referring again to FIG. 7, correlation curves 704, obtained at different time scales using DCS data, are shown. Such correlation curves may be generated either synchronously or asynchronously along with other acquired measurements, such as ECG and other physiological measurements. For example, DCS measurements may be collected at multiple times relative to the cardiac cycle measured using ECG data.

[0071] In some aspects, the optical processing system 606 in cooperation

with the controller 610, and methods of operation of the present disclosure are capable of acquiring and processing multiple DCS measurements per second to, thereby, achieve a speed, or temporal resolution, to determine pulsatile information and create accurate measures not achieved or recognized in non-invasive systems previously. By way of example, data, including DCS data, may be sampled at frequencies of up to 500 Hz, although higher frequencies may be possible. Again, this stands in contrast to traditional DCS systems and methods that, for example, have a sampling time for DCS measurements of approximately 1.5 seconds or longer. As described herein, the systems and methods of the present disclosure acquire DCS measurements at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of the subject. As such, the pulsatile information can be determined from the DCS data.

[0072] The controller 610 may be further configured to analyze acquired data, including DCS data and physiological data, in order to provide estimates of quantities, such as ICP, and others, as described. For instance, the controller 610 may be configured to analyze autocorrelation curves at various timescales to determine a blood flow, at various points within a cardiac cycle. In addition, the controller 610 may combine DCS data acquired over a number of cycles, the DCS data being acquired at specific time points or over a range of time points in the cardiac cycle.

[0073] Individual measurements may or may not have sufficient signal to noise ratio (SNR) for analysis of desired parameters such as CrCP, ICP, CPP, CVR, and others. As such, a measurement taken from one cardiac cycle can be averaged with a measurement from a different cardiac cycle, while ensuring proper gating of the signals. That is, individual measurements could be timed to exactly coincide with the same portion of the cardiac cycle, or the measurements could be asynchronous to the cycle resulting in an equivalent time average. Equivalent time averaging has superior sampling of the cycle, but either method can be used. In addition to the cycle average, the same data can be averaged over longer times. In this manner, both pulsatile and average blood flow, for example, may be provided. Alternatively, or additionally, the controller 610 may integrate or combine data acquired over an entire cardiac cycle.

[0074] In some aspects the controller 610 may be configured to determine a condition of the subject based on determined parameters, such as intracranial pressure, and others. For example, the controller 610 may be configured to determine a risk of cerebral ischemia, or a loss of autoregulation and/or regulatory reserve. In addition, the controller 610 may also be configured to determine an effectiveness of an administered treatment using determined physiological parameters, such as intracranial pressure.

[0075] The controller 610 may be further configured to generate and provide a report to a user. The report may include a variety of information including, real-time or intermittent physiological signals or measured quantities, such as ICP, as well as other clinically relevant parameters, including cerebral perfusion pressure (CPP), cerebrovascular resistance (CVR), vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling and cerebral compliance, dynamic autoregulation, cerebral perfusion reserve, and other parameters or quantities generated therefrom. Provided signals may be in the time domain, as time series, as well as the frequency domain, as power spectra.

[0076] The report may also indicate a condition of the subject being monitored, as well as other information associated with the subject. For instance, the report may indicate a risk for a cerebral ischemia, or a loss of autoregulation or regulatory reserve. The report may further include an audio and/or visual alarm to indicate an acute condition, such as when one or more estimated quantities exceed a safe threshold, or a risk for complications is increased. For example, an alarm may provided when an estimated ICP is in a range between 11 and 20 mmHg, between 21 and 40 mmHg, and greater than 40 mmHg. The alarm signal may also adapt depending on the severity of the risk or the magnitude of the quantity.

[0077] Referring now to FIG.8, the steps of a process 800 in accordance with aspects of the present disclosure are described. The process 800 may be carried out on any system or apparatus, such as the one described with reference to FIG. 6. As shown in FIG. 8, the process 800 may begin at process blocks 802 and 804 with acquiring DCS and physiological data using various sensors placed about a subject. The data acquired at process blocks 802 and 804 may be

obtained in any number of ways, as described, including intermittently or continuously. For instance, in some aspects, DCS data may be acquired at multiple times within a cardiac cycle. Example physiological data includes electrocardiogram (ECG) data, electroencephalogram (EEG) data, near infrared spectroscopy (NIRS) data, blood pressure data, respiratory data, hemoglobin data, pulse oxymetry data, and combinations thereof.

[0078] The data acquired at process blocks 802 and 804 may also be processed in any number of ways. For instance, depending upon the requisite signal to noise ratio (SNR), data acquired over a number of cardiac cycles may be combined or averaged. In particular, the acquisition and averaging of DCS data does not need be limited to fixed correlation curves. Specifically, photon count data, whether a simple number of counts per time interval or the number of time intervals between photon detection, can be processed and averaged for cycles and events. For example, the photon data over short periods within the cardiac cycle can be used to calculate correlation curves and perform cycle averaging. The same photon data can be used with data over a longer time to calculate the correlation curve on the time scale of another period of interest (e.g. steady-state average, respiration, etc.). This approach can be used for non-cyclical events as well. For example, the blood flow associated with periods of time before and after a distinct EEG event such as a burst or seizure. Gating and averaging can be performed prospectively and/or retrospectively.

[0079] At process block 806 a pulsatile cerebral blood flow may be determined using the acquired DCS data. In particular, this step may include generating autocorrelation curves at various timescales using obtained photon counts and analyzing such curves to determine a blood flow, at various points within a cardiac cycle. In some aspects, a steady cerebral blood flow may also be determined at process block 806.

[0080] Referring again to FIG. 8, the determined cerebral blood flow may then be correlated with acquired physiological data, as indicated by process block 808. In some aspects, the determined pulsatile cerebral blood flow (pCBF) can be correlated with pulsatile arterial blood pressure (pABP). Other correlations may also be determined at process block 808.

[0081] Then, as indicated by process block 810, an intracranial pressure may then be estimated based on correlation. As such, a critical closing pressure may be computed to estimate the intracranial pressure. Other parameters may also be estimated at process block 810 using the DCS data and physiological data, as described. For example, cerebral perfusion pressure, vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling, cerebral compliance, dynamic autoregulation, cerebral perfusion reserve, cerebrovascular resistance, oxygen saturation, hemoglobin concentration, cardiac output, stroke volume, brain activity, cardiac activity, and various combinations or changes thereof, may be determined at process block 810. In some aspects, the characteristics of a pulsatile pressure-flow relationship curve, as described with reference to FIG. 3, for instance, may also be used to determine desired physiological parameters.

[0082] In some aspects, a condition of the subject based on determined parameters, such as ICP, and others, may be determined at process block 810. For example, a risk of cerebral ischemia, or a loss of autoregulation and/or regulatory reserve may be determined. In other aspects, an effectiveness of an administered treatment may be determined using determined physiological parameters, such as intracranial pressure.

[0083] Then, at process block 812 a report, of any form, may be generated and provided to a user. The report may include a variety of information including, real-time or intermittent values of measured physiological parameters or quantities, such as ICP, blood flow, as well as other clinically relevant parameters, including cerebral perfusion pressure (CPP), cerebrovascular resistance (CVR), vessel wall tone, cerebral blood flow-cerebral spinal fluid pulsatility coupling and cerebral compliance, dynamic autoregulation, cerebral perfusion reserve, and other parameters or quantities generated therefrom. The report may also identify a condition of the subject being monitored, as well as other information associated with subject. For instance, the report may indicate a risk for a cerebral ischemia, or a loss of autoregulation or regulatory reserve.

[0084] As described, FIG. 7 shows an example of how the photon counts can be correlated in reference to another signal or event at one or more timescales. Specifically, FIG. 7 shows ECG data 702 and DCS data 704 as a

function of time. In particular, the DCS data 704, in the form of a stream of photon counts, can be parsed, in either synchronous, partially synchronous, or asynchronous manner, with regards to another physiological signal, such as ECG data 702, to generate one or more correlations functions 706. Such parsing may be achieved with reference to other physiological signals, including ECG, EEG, NIRS, or other physiological signals. Thus, the same data could be combined with regards to multiple events with the appropriate time and duration for each signal. For example, the same signal could process blood flow with regards to cardiac cycle from an ECG and flow before and after a seizure event recorded in EEG. Different time scales could be used between different signals or within the same signal, including, but not limited to, determining both pulsatile and steady flow.

[0085] In some aspects, intra-cardiac cycle and intra-respiratory cycle flows, gated by appropriate cardiac and respiratory signals, may be calculated at two different timescales within the ECG. In others, cardiac cycle timing could be determined from a blood pressure sensor or the optical signals themselves. The timing and duration could be fixed or dynamically and/or algorithmically determined, either in real-time, near-real time, or in post-processing. For example, the DCS data 704 could be parsed on a cycle-by-cycle basis, following the spontaneous changes in heart rhythm. The processing may include other transformations, for example a temporal offset to account for the difference in phase between an ECG signal and the CBF signal to account for the transit time of blood from the heart to the brain, and/or other instrument factors. The processing could be performed either in software (for example, using FFTs, etc.), in hardware (for example, multi-tau algorithm, FFT, etc.), or any combination thereof.

[0086] By way of example, FIG. 10 shows pulsatile blood flow measurements obtained from a human subject in accordance with aspects of the present disclosure. In this example, flow measurements were acquired in an integration time less than the period of a cardiac cycle with a hardware correlator, as described with reference to FIG. 6. As described, in some aspects, flow measurements may be inter-cycle combined, processed, and/or averaged

with equivalent intra-cycle measurements. In this manner, the signal-to-noise ratio (SNR) and/or intra-cycle time resolution may be increased. The amount of combination can be set by a predetermined amount, such as time, number of samples and so forth, or determined dynamically and/or algorithmically, such as when a desired SNR is achieved, or when number of intra-cycle points are acquired. Measurements may also be combined, processed, and/or averaged with or without regard to the cycle in which they were acquired, and may be used for determining a baseline.

[0087] As another example, FIGs. 11A and 11B demonstrate simultaneous measurements of pulsatile DCS with ECG and CW NIRS. As can be seen, the DCS data has a temporal resolution of 4-5 samples per second. The NIRS and DCS data were collected from an integrated optical probe place on the forehead to sample the same tissue in the cortex. ECG was recorded from two leads placed on the chest of the subject. Although the data points were acquired asynchronously, the pulsatile blood flow, hemoglobin concentration changes and cardiac electrical activity were all physiologically synchronous. However, due to transit time differences between the heart beat and arrival of blood in the cortex, there was a phase difference between the ECG/NIRS signals and the ECG activity. In general, such phase difference could be accounted for by calibration and/or processing.

[0088] As yet another example, FIG. 11C shows the results of cycle averaging. Specifically, a portion of the data from FIGs. 11A and 11B was averaged over the cardiac cycle in an equivalent time average. Further processing can be performed to perform calibrations and/or extract relevant parameters from the data.

[0089] In yet another example FIG. 12 shows a segment of data acquired from an anesthetized rat. Specifically, arterial blood pressure, intracranial pressure (acquired with a fiberoptic transducer inserted in a rat's brain), and blood flow measured with DCS were simultaneously measured. In this example, flow measurements were acquired from a stream of photons and correlated using software, as described with reference to FIG. 6. These results demonstrate that the present approach can resolve the faster pulsatile flows of small mammals.

This fast speed is important because it enables: 1) use in animal models for biomedical research, 2) better temporal resolution of the cardiac cycle in adults, 3) sufficient resolution for premature and full-term infants, 4) resolution for patients with cardiac defects. Furthermore, the data in FIG. 12 shows sensitivity to pulsatile and respiratory variations in cerebral blood flow.

[0090] As described, the ICP can be derived by estimating the critical closing pressure (CrCP). That is, the ICP can be derived by estimating the value of arterial blood pressure at which cerebral blood flow approaches zero, such as can be derived as detailed with reference to FIG. 3. The use of CrCP as a substitute for ICP is based on the following concept. Specifically, the relationship between flow and pressure in a uniform cylindrical vessel of length L and radius r , is given by Poiseuille's law, which by analogy with Ohm's law, can be written as:

$$F = \frac{(P_i - P_o)}{CVR} \quad (3)$$

[0091] here F is flow, P_i and P_o are the inflow and outflow pressures, and the resistance is

$$CVR = \frac{8\mu L}{\pi r^4} \quad (4)$$

[0092] with blood viscosity, μ . In a simplified model of a collapsible cortical vessel with zero active tension, P_i is equal to ABP, and at equilibrium, if the intracranial pressure is greater than the venous pressure, P_o is equal to ICP. When ABP approaches P_o , blood flow ceases, implying CrCP is equal to ICP. In a more realistic description of the flow-pressure relationship, one needs to include the effects of active wall tension and vessel elasticity:

$$CrCP = ICP + T_{wall} \quad (5)$$

[0093] Models based on Laplace's law, including a non-linear elastic curve and a radius-dependent active tension, show that CrCP depend both on ICP and on the vasomotor tone, and that ICP is lower than the CrCP estimates that use a simple linear regression of the pressure-axis intercept (FIG. 8). From either the non-linear, linear CrCP, or a combination of the two, the wall tension can be determined and provide information about chronic and acute vessel physiology and pathology.

[0094] CrCP can provide a superior estimate of ICP compared with traditional pulsatility index (PI) computations, because CrCP is determined from measurements of both the driving arterial blood pressure and the flow response. By contrast, PI is estimated purely from flow velocity. Thus, the present disclosure allows for some of the physiological factors influencing PI to be eliminated in determining CrCP. This makes CrCP a more robust measure.

[0095] As described, blood flow velocity measurements based on transcranial Doppler ultrasonography have been used to estimate CrCP. However, while these estimates can correlate with invasive ICP values, they do not reach an acceptable confidence interval to be clinically useful. In fact, while theoretically estimated CrCP should be higher than ICP according to Eqn. 5 above, both higher and lower values were measured by transcranial Doppler ultrasonography. Since in these experiments arterial blood pressure (ABP) measurements are performed using standard arterial lines, the variability in the transcranial Doppler ultrasonograph estimation of ICP is hence driven by the known issues with this approach.

[0096] Moreover, transcranial Doppler ultrasonography measures flow velocity and not blood flow, which depends on the cross-sectional area of the imaged vessel. Also, flow velocity is measured on a section of the middle cerebral artery, which is a large vessel with high wall tension and elasticity that is only indirectly impacted by changes in ICP.

[0097] By contrast, the present approach utilizes DCS data, providing a better estimate of CrCP compared to previous techniques. This is because DCS measures blood flow and not blood flow velocity. In addition, measurement of pulsatile cerebral blood flow using DCS, in accordance with the present disclosure, is directly sensitive to small cortical arterioles, venules and bridging vessels, which due to their small transmural pressure determine the vasomotor tone of the cerebral circulatory system, and hence are critically impacted by changes in ICP.

[0098] In addition to ICP, other parameters may also be estimated. One non-limiting example includes CPP, defined as the mean arterial pressure minus the critical closing pressure:

$$CPP = MABP + CrCp \quad (6)$$

[0099] Autoregulation maintains constant CBF across a large range of CPP (50 to 150 mmHg). Reductions of CPP below the lower limit of autoregulation causes CBF to become pressure passive and arteries and arterioles to passively vasodilate. The present approach can hence detect and warn of risk of this condition. Hypotension has adverse consequences for patients with traumatic brain injury and guidelines are to maintain CPP above 50-70 mmHg. Currently, CPP is estimated from invasive ICP measures as a proxy for CrCP in the equation above. The ability to continuously and noninvasively monitor CPP at the bedside would impact the management of a larger number of patients than currently done with invasive measures.

[00100] As another example, since blood flow, rather than flow velocity is measured in arterioles, cerebrovascular resistance can be estimated (FIG. 3):

$$CVR = \frac{\Delta p_{ABP}}{\Delta p_{CBF}} \quad (7)$$

[00101] By simultaneously and continuously measuring both changes in CPP and CVR, cerebral autoregulation can be non-invasively monitored at the bedside. Failure of autoregulation is associated with a worse outcome in various acute neurological diseases.

[00102] As may be appreciated, CrCP, ICP, CPP and CVR are tremendously important parameters for the diagnosis and management of patients under many clinical situations, including but not limited to, critical care such as infant, pediatric, or neuro intensive care units, anesthesia and/or surgery, emergency and trauma wards, recovery wards, post intensive care, battle fields, spacecrafts, extreme environments, during sports or on the sidelines, disaster or accident sites, etc. The present approach of measuring pulsatile flow allows estimation of these parameters continuously and non-invasively at the bedside, on an outpatient and/or home care basis. Information generated from such monitoring can be used to understand, for example, the complex pathophysiology after traumatic brain injury, better target care, identify new therapeutic opportunities, and, in general, substantially improve neurocritical care management.

[00103] Several approaches can be used to estimate autoregulatory

capacitance. A moving correlation coefficient between CBF_i and/or CVR and CPP and/or AP can quantify autoregulation status, with a correlation near one during impaired autoregulation during pressure passive hypo- or hyperemia and near zero for intact autoregulation. Another approach may include, but is not limited to, directly measuring changes in CBF and/or CVR with changes in AP and/or CPP, either spontaneously or induced correlation of CBF and/or CVR fluctuations and changes with CPP and/or AP, correlation of the variances of CBF and/or CVR with CPP, cross-spectral coherence and gain analysis between CBF and/or CVR and CPP and/or AP, phase shifts between CBF and/or CVR with changes in AP, CPP, and/or CBV. In some aspects, a change in blood pressure can arise spontaneously, or be induced by external means such as leg-cuff release, or other means.

[00104] In some aspects, the PI may be computed. In particular, the PI is proportional to ICP and can be used to monitor changes in ICP. The PI can be calculated from $pCBF_i$ directly using the following equation:

$$PI = \frac{\text{systolic } CBF_i - \text{diastolic } CBF_i}{\text{mean } CBF_i} \quad (8)$$

[00105] PI can also be determined in the frequency domain using the harmonic components of CBF_i . In some implementations, pulsatile DCS (pDCS) PI can be used when measurements of blood pressure are not available. PI may also have greater sensitivity to ICP changes at low intra-cranial pressures, even when blood pressure signals are measured.

[00106] When blood pressure measurements are obtained in conjunction with pDCS measurements, a pressure-flow relationship, as described with reference to FIG. 3 can be obtained. Such a pressure-flow relationship may then be analyzed to generate a wide variety of information, including but not limited to, a zero flow pressure or CrCP, CPP, CVR, wall tension, and so forth. It is estimated that approximately 11 million photons would provide a precision of +/- 5 mmHg in measurement of CrCP using the linear model. The photon flux in the adult measurement described with reference to FIGs. 11A and 11B was approximately 200,000 counts per second, and included an integration time of about 1 minute. The required integration time could be further decreased with the use of additional detectors. Thus, the present approach is feasible from a

practical standpoint. However, this disclosure is not limited to a specific number of detected photons. Other criteria for precision, accuracy or quality can be used. These metrics can be calculate online or in post-processing. They could also be used to dynamically adjust the measurement process, optimizing signal quality and dynamic response.

[00107] In some implementations, CrCP, and other parameters can be estimated by other analysis methods, including, but not limited to the application of transfer function, correlation, coherence, frequency, or time-domain analyses of pDCS. These analyses may be performed individually or together, in whole or in part, with or without taking into consideration other physiological measurements such as BP, ICP, ECG, EEG, and others.

[00108] For example, CPP can be estimated using an analysis of the frequency spectra of blood pressure and CBF_i. Specifically, from the first harmonics, CPP can be estimated according:

$$CPP = \frac{A1}{CBF_{i1}} \times \text{mean } CBF_i \quad (9)$$

[00109] where A1 and CBF_{i1} are the first harmonics of arterial pressure and pCBFi, respectively. From CPP, CrCP can be approximated using:

$$CrCP = BP - \frac{A1}{CBF_{i1}} \times \text{mean } CBF_i \quad (10)$$

[00110] Also, CPP can also be approximated by

$$CPP = MAP \times \frac{\text{diastolic } CBF_i}{\text{mean } CBF_i} + \text{Constant} \quad (11)$$

[00111] Furthermore, CCP may be estimated using a linear interpolation from diastolic and systolic values of CBF_i and BP. Many other such combinations can be utilized.

[00112] In some aspects, CrCP can be estimated from pDCS and different types of blood pressure monitors. For example, arterial pressure can be measured invasively through sensors with an invasive arterial line. CrCP estimated in this way is semi-invasive because, while the blood pressure measurements are invasive, the pDCS measurement remains non-invasive. In this case, although the BP measurement is invasive, this approach is still a significant improvement compared to current techniques, since an arterial line is considerably less invasive than a cranial bolt or burr hole, as required for

conventional ICP sensors. In addition, the risk of complications for an arterial line is low and they are routinely used in critical care situations. Furthermore, use of ICP monitoring is much more restricted than arterial line due to the higher risks of invasive intracranial probes. Therefore, it may be appreciated that the present approach provides a considerable advancement over the current state of the art because it allows, for the first time, routine measurement and/or monitoring of ICP in a large population of patients receiving arterial lines.

[00113] In other aspects, the present approach can also be utilized entirely non-invasively in patients and subjects in general by combining pDCS with non-invasive means to measure blood pressure. For example, absolute pulsatile blood pressures can be measured non-invasively using devices such as the Finapres monitor. Another example includes combining a relative pressure transducer for pulse measurement (for example a simple transducer wrapped to a finger with a bandage) with intermittent absolute measurements by non-invasive means via a sphygmomanometer. This approach provides a considerable advancement over the current state of the art because it extends measurement and/or monitoring of ICP to anyone. In addition, this approach enables measurements in patients whose perceived risk of abnormal ICP does not currently justify measurement by invasive means. Furthermore, patients believed not to be at risk for abnormal ICP, or even with healthy subjects in natural environments, may also be monitored.

[00114] There is a consensus that clinically useful ICP measurements are preferred to have an accuracy of at least 10 mm Hg, or less. The precision of BF_i in a DCS measurement is determined by photon statistics. Thus, with a few assumptions and simplifications, an estimate can be obtained for how long the DCS measurements must be integrated to determine the critical closing pressure (CrCP) to within 10 mm Hg.

[00115] Assuming a linear relationship between pulsatile blood flow and pressure during the cardiac cycle, namely:

$$F = a + bP \quad (12)$$

[00116] Real measurements may use more complicated models for the flow-pressure relationship (i.e. with wall tension, etc.) but the linear model is

sufficient for estimating integration times. Analysis with more realistic models will not require significant differences integration times.

[00117] Observations are pairs (P_i, F_i) representing instantaneous blood pressure and flow, with the instantaneous flow measurement having a variance of σ for each observation. For DCS, σ is known from photon statistics and the total number of detected photons integrated in a measurement. For ICP determinations, flow can be measured a number of times within the cardiac cycle, with multiple cardiac cycles integrated to achieve sufficient accuracy. In this case, total number of photons refers to the number of detected photons for a measurement within the cardiac cycle after integrating one or more cardiac cycles.

[00118] The uncertainty of the maximum likelihood estimation of a and b are then:

$$\sigma_a^2 = \frac{1}{\Delta} \sum_i \frac{P_i^2}{\sigma_i^2} \quad (13)$$

$$\sigma_b^2 = \frac{1}{\Delta} \sum_i \frac{1}{\sigma_i^2} \quad (14)$$

where Δ is defined as:

$$\Delta = \sum_i \frac{1}{\sigma_i^2} \sum_i \frac{P_i^2}{\sigma_i^2} - \left(\sum_i \frac{P_i}{\sigma_i^2} \right)^2 \quad (15)$$

[00119] and the uncertainty in P is negligible. For the linear model, the critical closing pressure (CrCP) may be approximated as:

$$CrCP = -\frac{a}{b} \quad (16)$$

[00120] Then the variance of the CrCP can be propagated from the variances in a and b :

$$\sigma_{CrCP}^2 = CrCP^2 \left(\frac{\sigma_a^2}{a^2} + \frac{\sigma_b^2}{b^2} - 2 \frac{\sigma_{ab}^2}{ab} \right) = \left(\frac{a}{b} \right)^2 \left(\frac{\sigma_a^2}{a^2} + \frac{\sigma_b^2}{b^2} \right) \quad (17)$$

[00121] where σ_{ab}^2 is assumed = 0.

[00122] For a simple estimate, σ can be approximated as a constant σ_{BF} for all measurements. This is reasonable because the uncertainty in CBF_i depends primarily only on the detected photon flux and very weakly on the value of CBF_i . Then, the variances simplify to:

$$\Delta' = N \sum_i P_i^2 - (\sum_i P_i)^2 \quad (18)$$

$$\sigma_a'^2 = \frac{\sigma_{BF_i}^2}{\Delta'} \sum_i P_i^2 \quad (19)$$

$$\sigma_b'^2 = N \frac{\sigma_{BF_i}^2}{\Delta'} \quad (20)$$

[00123] where N is the number of (P_i, F_i) pairs determined within the cardiac cycle.

$$\begin{aligned} \sigma_{CrCP}'^2 &= \left(\frac{a}{b}\right)^2 \left(\frac{1}{a^2} \left(\frac{\sigma_{BF_i}^2}{\Delta'} \sum_i P_i^2 \right) + \frac{1}{b^2} \left(N \frac{\sigma_{BF_i}^2}{\Delta'} \right) \right) \\ &= \left(\frac{\sigma_{BF_i}^2}{\Delta' b^2} \right) \left(\sum_i x P_i^2 + \frac{a^2}{b^2} N \right) \end{aligned} \quad (21)$$

[00124] So, solving for σ_{BF_i} gives

$$\begin{aligned} \sigma_{BF_i}'^2 &= \left(\frac{\Delta' b^2}{\sum_i P_i^2 + \frac{a^2}{b^2} N} \right) \sigma_{CrCP}'^2 \\ &= \left(\frac{\Delta' b^2}{\sum_i P_i^2 + CrCP^2 N} \right) \sigma_{CrCP}'^2 \end{aligned} \quad (22)$$

[00125] Thus, if there is a specific requirement for the accuracy of the zero flow pressure, a physiologically reasonable b and CrCP may be assumed, and a measurement acquisition rate through parameter N can be chosen to estimate the accuracy required for the blood flow measurement. The blood flow accuracy can then be used to determine the minimum number of photons required per blood flow measurement and estimate the required total integration time.

[00126] Setting N to be the number of flow determinations through the cardiac cycle allows us to estimate the uncertainty from the extremes of the systolic and diastolic pressures and CBF_i. Replacing P_i with a linear model of pressure ranging through systolic to diastolic (P_s to P_d):

$$\begin{aligned} P_i &= P_d + \frac{(P_s - P_d)}{(N - 1)} i \\ \Delta' &= N \sum_i^{N \text{ periods during cardiac cycle}} \left(P_d + \frac{(P_s - P_d)}{(N - 1)} i \right)^2 = \left(\sum_i^{N \text{ periods during cardiac cycle}} \left(P_d + \frac{(P_s - P_d)}{(N - 1)} i \right) \right)^2 \end{aligned} \quad (23)$$

[00127] Using (where i and N are consistent with model for x_i):

$$\begin{aligned} \sum_i^N i &= \frac{N(N - 1)}{2} \\ \sum_i^N i^2 &= \frac{N(N - 1)(2N - 1)}{6} \end{aligned}$$

(24)

[00128] Δ' simplifies to:

$$\Delta' = \left(\frac{(N+1)N^2}{12(N-1)} \right) (P_s - P_d)^2 \quad (25)$$

[00129] and σ'_{BF_i} to:

$$\sigma_{BF_i}'^2 = \left(\frac{\Delta' b^2}{NP_d^2 + \left(\frac{N(2N-1)}{6(N-1)} \right) (P_s - P_d)^2 + NP_d(P_s - P_d) + CrCP^2 N} \right) \sigma_{CrCP}'^2 \quad (26)$$

[00130] From these two equations and assumptions of P_s , P_d , b , and a nominal value of CrCP, the required accuracy for the DCS measurement (σ'_{BF_i}) can be estimated from the specified accuracy of the ICP determination (σ'_{CrCP}). For P_s and P_d , a normal systolic blood pressure of 120 mm Hg and diastolic pressure of 80 mm Hg is assumed.

[00131] In preliminary pDCS measurements, CBF_i ranged from 7.1×10^{-8} to 1.3×10^{-7} through the cardiac cycle. The ratio of peak flows appears to be underestimated due to the limited DCS acquisition rate achieved with instrumentation utilized. Thus, the ratio of peak flow in preliminary measurements was only 1.8x, while values of 2.9x were reported in the literature for ratios of peak flow velocities in transcranial Doppler ultrasonography. Presumably, the pDCS peak flow ratio can increase with a faster DCS acquisition.

[00132] However, the transcranial Doppler ultrasonography ratio will remain larger since pulsatility is larger in the larger artery measured by transcranial Doppler ultrasonography than in the downstream smaller vessels measured by DCS and because DCS also measures the out flow which is less pulsatile than the inflow. Regardless, the underestimated flow ratios makes this error estimation a worst case condition and the actual accuracy would be expected to be better than this prediction. Using the peak flows from the preliminary measurement, b can be approximated:

$$b = \frac{1.3 \times 10^{-7} - 7.1 \times 10^{-8}}{(120 - 80)} = 1.5 \times 10^{-9} \frac{CBF_i}{mm\ Hg\ BP}$$

[00133] Normal CrCP values range from 5 to 10 mm Hg and can elevate to

over 50 mm Hg under pathological conditions. Hence CrCP can be estimated with 10 mm Hg as a reasonable nominal value. A DCS acquisition rate of 25 Hz can then be chosen, making N approximately 25.

[00134] To meet the clinical target CrCP accuracy of within 10 mmHg, a 99% confidence interval to be ± 5 mmHg is selected. Thus, the required σ'_{CrCP} is specified to be $\sigma'_{CrCP} = \frac{5 \text{ mmHg}}{2.58} = 1.94 \text{ mmHg}$. Utilizing the assumed values into the equations for Δ' and σ'_{BF_i} determines that a total SNR of approximately 42 is required for each of the 25 flow determinations within the cardiac cycle. From the measured DCS SNR curve, about 440k photons are needed to achieve a BF_i SNR of 42. Thus, approximately 11 million detected photons are required to be integrated across the entire cardiac cycle. In the preliminary measurements, the detected photon flux was about 200 kcps per detector, so 55 seconds of integration would be sufficient for a single detector, or only 18 seconds if all three detectors are averaged together. Thus, though this model does not take into account other sources of error, such as the accuracy of the pressure measurement, it does show that pDCS measurements and CrCP determinations are fundamentally practical from a DCS SNR standpoint.

[00135] In summary, the present disclosure overcomes the drawbacks of previous technologies by providing a system and method for accurately and non-invasively monitoring patients. More specifically, the system and method described herein utilize diffuse correlation spectroscopy to measure pulsatile, as well as steady, cerebral blood flow for determining parameters useful in the diagnosis and management of patients.

[00136] As may be appreciated from descriptions herein, the present disclosure provides a wide range of applicability. For example, the system and method described can be used to monitor changes in ICP, CVR, CPP, WT, and autoregulation capacity with drugs or anesthetics, as well as provide monitoring and/or diagnostics with pharmacological manipulations include bolus testing. In addition, the present system and method may be applied to monitoring vasospasm or the effect of vasospasm or vasoparalysis, as well as monitoring cortical spreading depression or the effect of cortical spreading depression. The present system and method may also be applied to monitoring hemorrhages,

including subarachnoid hemorrhages, and post- hemorrhage monitoring, tumors, hematoma, hydrocephalus, edema, vascular engorgement, hypercapnia, hypoxia, shock, sepsis. Furthermore, the present approach may be used to investigate chronic diseases and conditions such as hypertension, sleep and other apneas, etc. (measurement of pathological chronic changes in vascular tone), as well as hydrocephalus.

[00137] The present system and method may be applied to monitor congestive heart failure, blood flow in non-cerebral organs, peripheral vascular disease. In addition, the provided system and method may be utilized in perioperative, intensive and critical care, as well as goal-directed blood pressure support in patients with critical carotid artery stenosis. Furthermore, the present system and method may be utilized in perioperative management of patients undergoing carotid endarterectomy, and in patients with cardiopulmonary bypass, as well as optimization of blood pressure management in patients with traumatic brain injury undergoing neurosurgical or non-neurosurgical procedures.

[00138] The present invention has been described in terms of one or more preferred embodiments, and it should be appreciated that many equivalents, alternatives, variations, and modifications, aside from those expressly stated, are possible and within the scope of the invention.

CLAIMS

1. A system for non-invasively monitoring intracranial pressure, the system comprising:

an optical coupling system configured to transmit and receive light signals from one or more locations about a subject;

an optical processing system configured to generate diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of the subject using the transmitted and received light signals;

a computer programmed to:

receive the DCS data;

analyze the DCS data to determine a pulsatile cerebral blood flow;

correlate the determined pulsatile cerebral blood flow with physiological data acquired from the subject;

estimate an intracranial pressure based on the correlation; and

generate a report indicative of the estimated intracranial pressure.

2. The system of claim 1, wherein the system further comprises one or more physiological sensors for acquiring the physiological data from the subject.

3. The system of claim 1, wherein the optical coupling comprises DCS sensors, and near infrared spectroscopy (NIRS) sensors.

4. The system of claim 1, wherein the physiological data comprises at least one of electrocardiogram (ECG) data, electroencephalogram (EEG) data, near infrared spectroscopy (NIRS) data, blood pressure data, respiratory data, hemoglobin data, pulse oxymetry data, or a combination thereof.

5. The system of claim 1, wherein the computer is further programmed to determine, using the DCS data and physiological data, at least one of a cerebral perfusion pressure, a vessel wall tone, a cerebral blood flow-cerebral spinal fluid pulsatility coupling, a cerebral compliance, a dynamic

.....
autoregulation, a cerebral perfusion reserve, a cerebrovascular resistance, an oxygen saturation, a hemoglobin concentration, a cardiac output, a stroke volume, a brain activity, a cardiac activity, or a combination thereof.

6. The system of claim 1, wherein the computer is further programmed to control the optical processing system to generate DCS data using an integration time less than a period of a cardiac cycle.

7. The system of claim 1, wherein the computer is further programmed compute a critical closing pressure to estimate the intracranial pressure.

8. The system of claim 1, wherein the computer is further programmed to combine DCS data acquired over a plurality of cardiac cycles, the DCS data being acquired during a portion of each cardiac cycle.

9. The system of claim 1, wherein the computer is further configured to determine an effectiveness of an administered treatment using the estimated intracranial pressure.

10. The system of claim 1, wherein the computer is further configured to determine a condition of the subject based on the estimated intracranial pressure.

11. A method for non-invasively monitoring intracranial pressure using a monitoring system, the method comprising:

acquiring diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of a subject using one or more optical sensors placed about the subject;

determining a pulsatile cerebral blood flow using the acquired data;

correlating the determined pulsatile cerebral blood flow with physiological data acquired from the subject;

estimating an intracranial pressure based on the correlation; and

generating a report indicative of the estimated intracranial pressure.

12. The method of claim 11, wherein the one or more optical sensors comprises DCS sensors, and near infrared spectroscopy (NIRS) sensors.

13. The method of claim 11, wherein the method further comprises acquiring the physiological data from the subject using one or more physiological sensors placed about the subject.

14. The method of claim 12, wherein the physiological data comprises at least one of electrocardiogram (ECG) data, electroencephalogram (EEG) data, near infrared spectroscopy (NIRS) data, blood pressure data, respiratory data, hemoglobin data, pulse oxymetry data, or a combination thereof.

15. The method of claim 11, wherein the method further comprises determining using the DCS data and physiological data at least one of a cerebral perfusion pressure, a vessel wall tone, a cerebral blood flow-cerebral spinal fluid pulsatility coupling, a cerebral compliance, a dynamic autoregulation, a cerebral perfusion reserve, a cerebrovascular resistance, an oxygen saturation, a hemoglobin concentration, a cardiac output, a stroke volume, a brain activity, a cardiac activity, or a combination thereof.

16. The method of claim 11, wherein the method further comprises controlling an optical processing system to generate DCS data using an integration time less than a period of a cardiac cycle.

17. The method of claim 11, wherein the method further comprises computing a critical closing pressure to estimate the intracranial pressure.

18. The method of claim 11, wherein the method further comprises combining DCS data acquired over a plurality of cardiac cycles, the DCS data being acquired during a portion of each cardiac cycle.

19. The method of claim 11, wherein the method further comprises determining an effectiveness of an administered treatment using the estimated intracranial pressure.

20. The method of claim 11, wherein the method further comprises determining a condition of the subject based on the estimated intracranial pressure.

21. A method for non-invasively monitoring a subject using a monitoring system, the method comprising:

- acquiring diffuse correlation spectroscopy (DCS) data at a temporal resolution greater than a pulsatile frequency of cerebral blood flow of a subject using one or more optical sensors placed about the subject;

- determining a pulsatile cerebral blood flow using the acquired data;

- correlating the determined pulsatile cerebral blood flow with physiological data acquired from the subject using physiological sensors;

- estimating at least one parameter based on the correlation; and

- generating a report indicative of the at least one parameter estimated.

22. The method of claim 21, wherein the at least one parameter comprises at least one of an intracranial pressure, a cerebral perfusion pressure,

a vessel wall tone, a cerebral blood flow-cerebral spinal fluid pulsatility coupling, a cerebral compliance, a dynamic autoregulation, a cerebral perfusion reserve, a cerebrovascular resistance, an oxygen saturation, a hemoglobin concentration, a cardiac output, a stroke volume, a brain activity, a cardiac activity, or a combination thereof.

23. The method of claim 21, wherein estimating the at least one parameter comprises analyzing a pulsatile pressure-flow relationship curve.

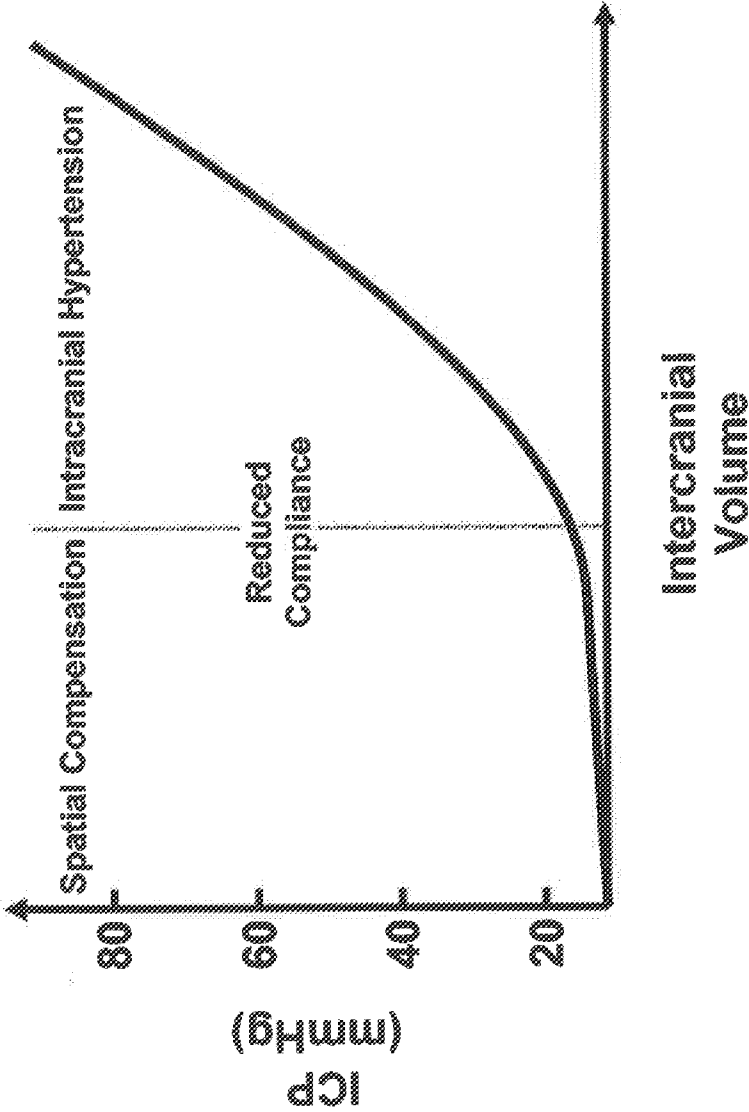
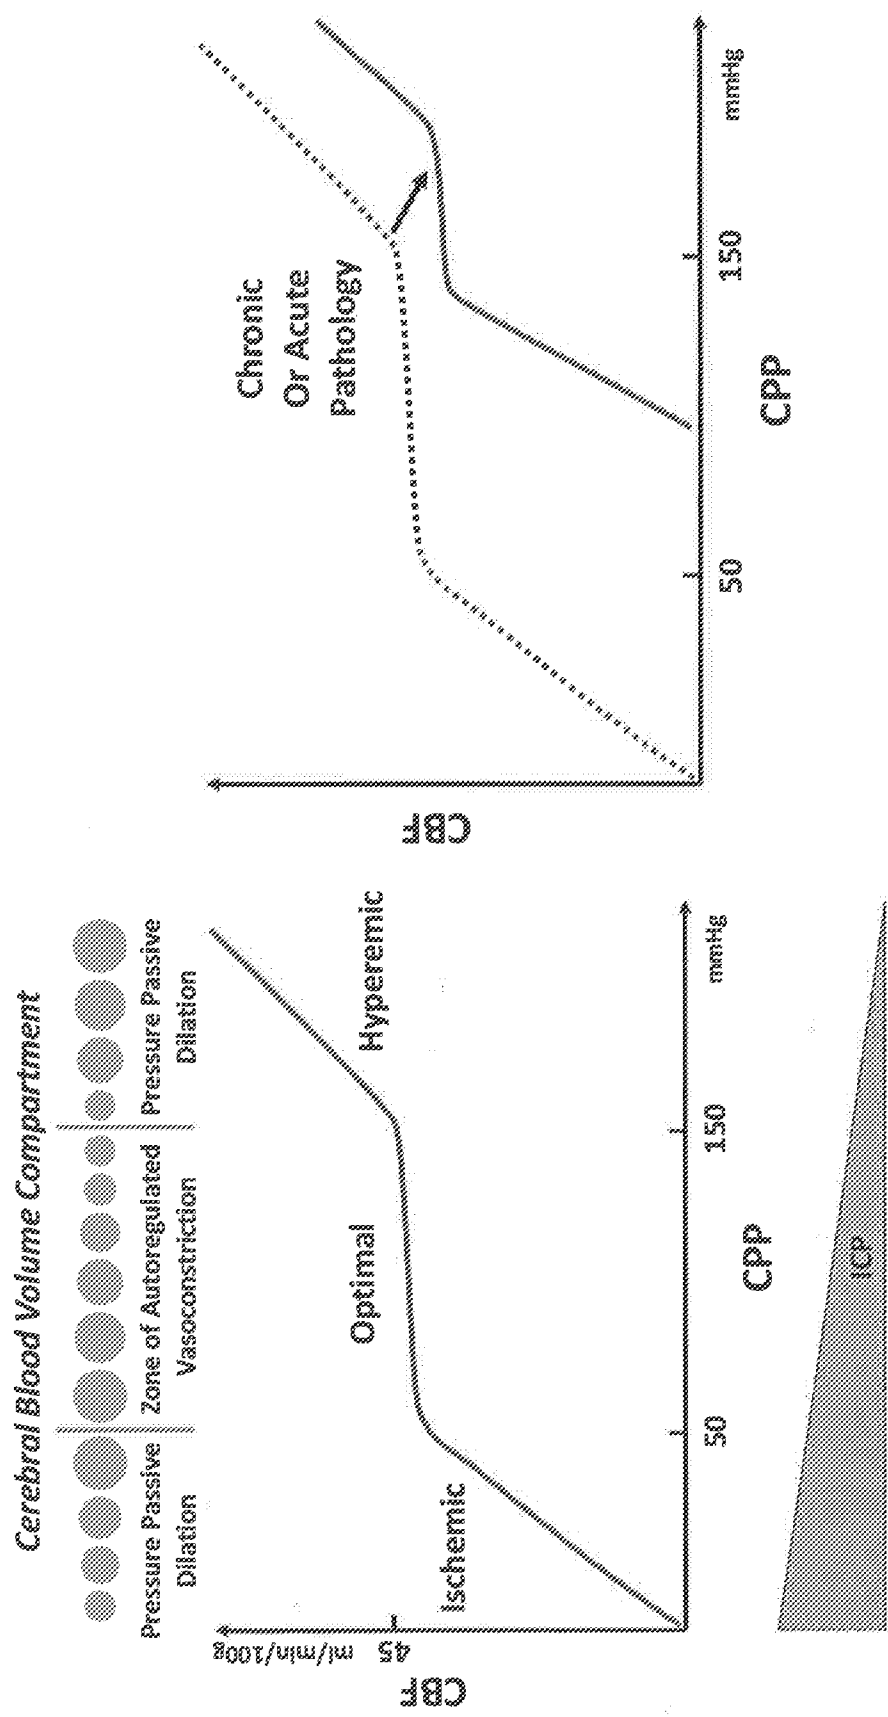


FIG. 1



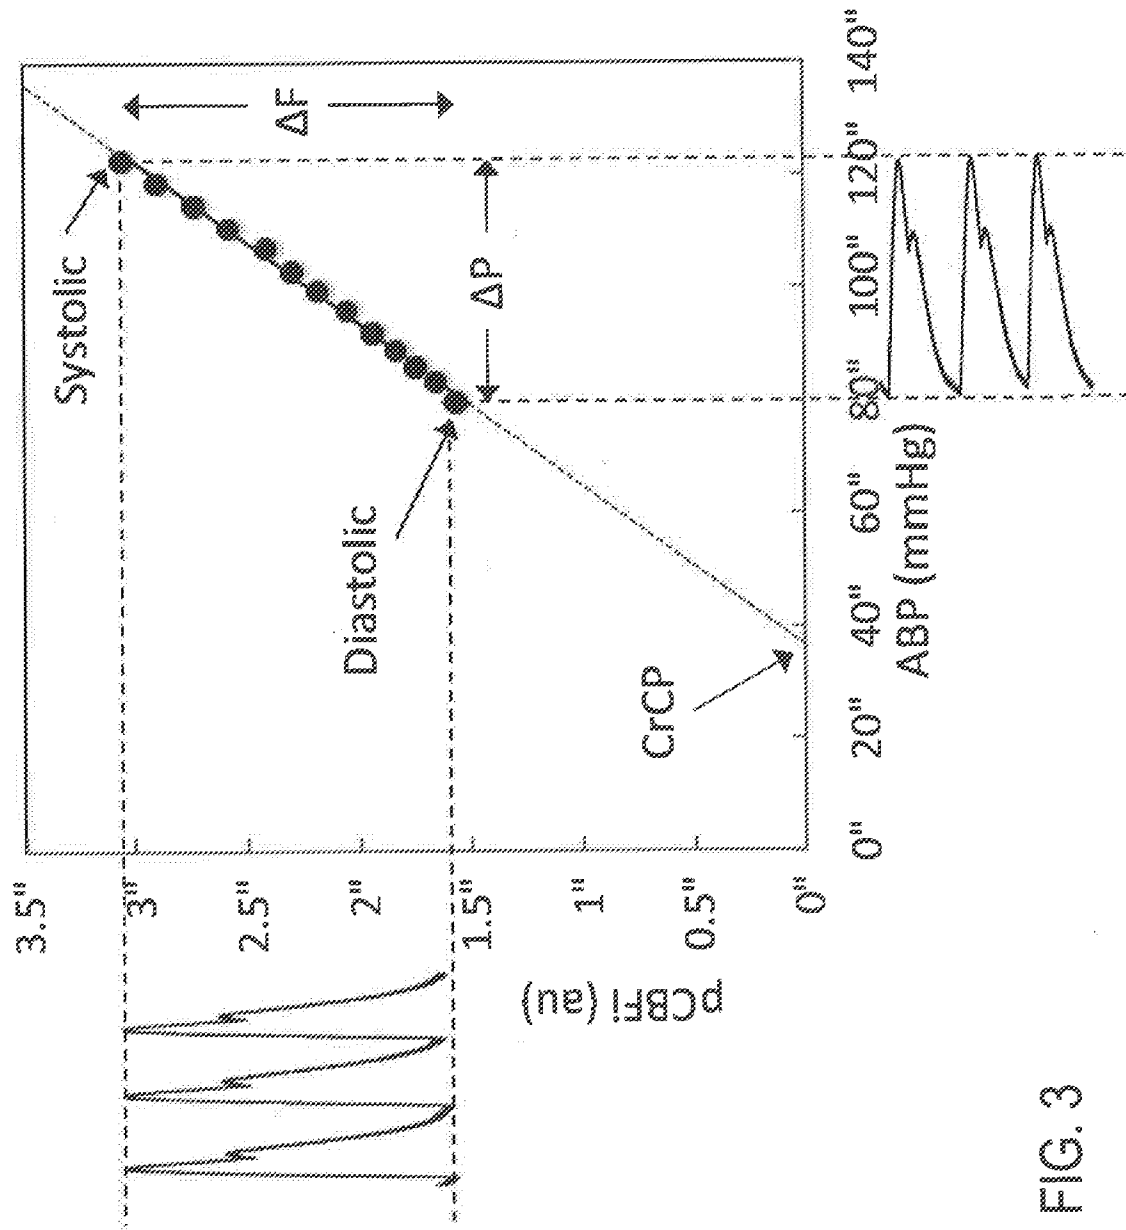


FIG. 3

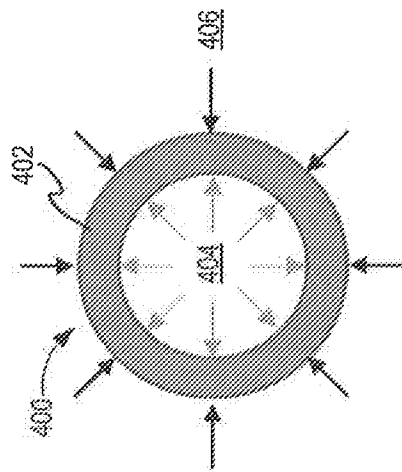


FIG. 4A

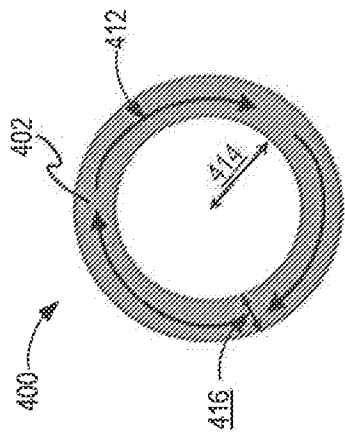


FIG. 4C

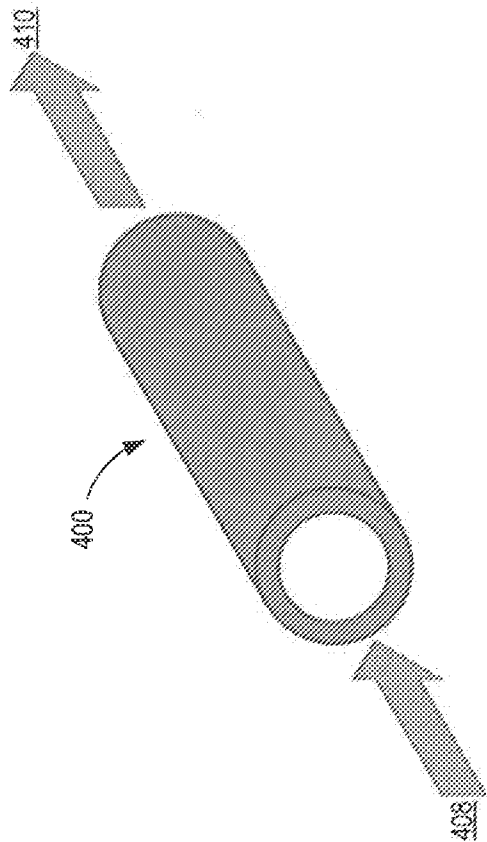


FIG. 4B

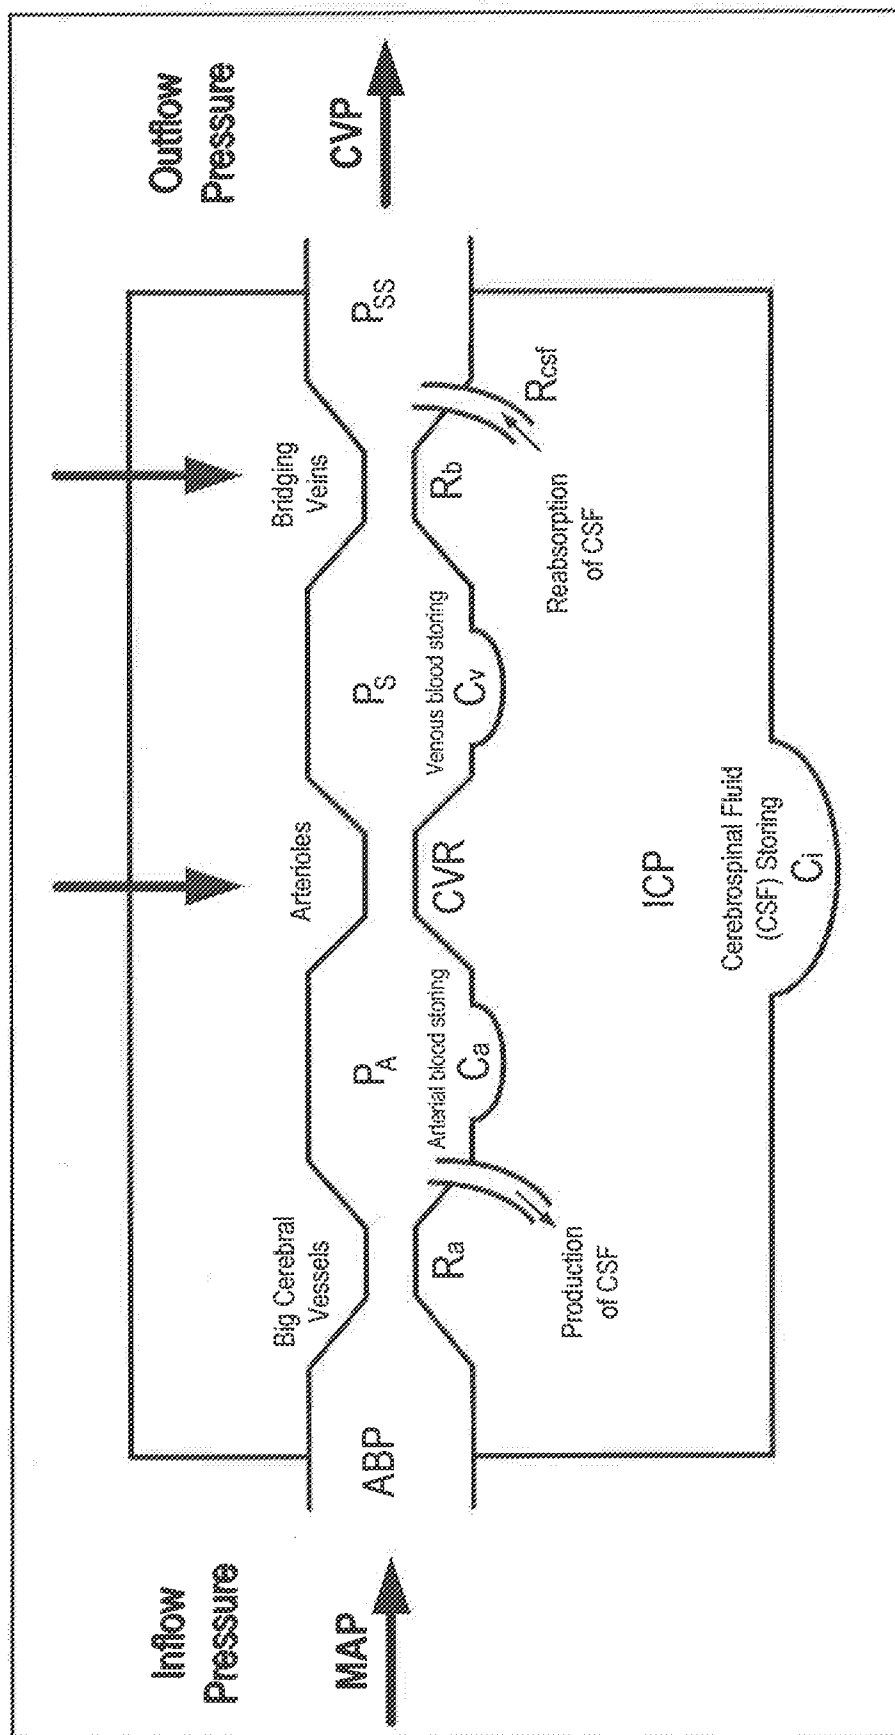


FIG. 5

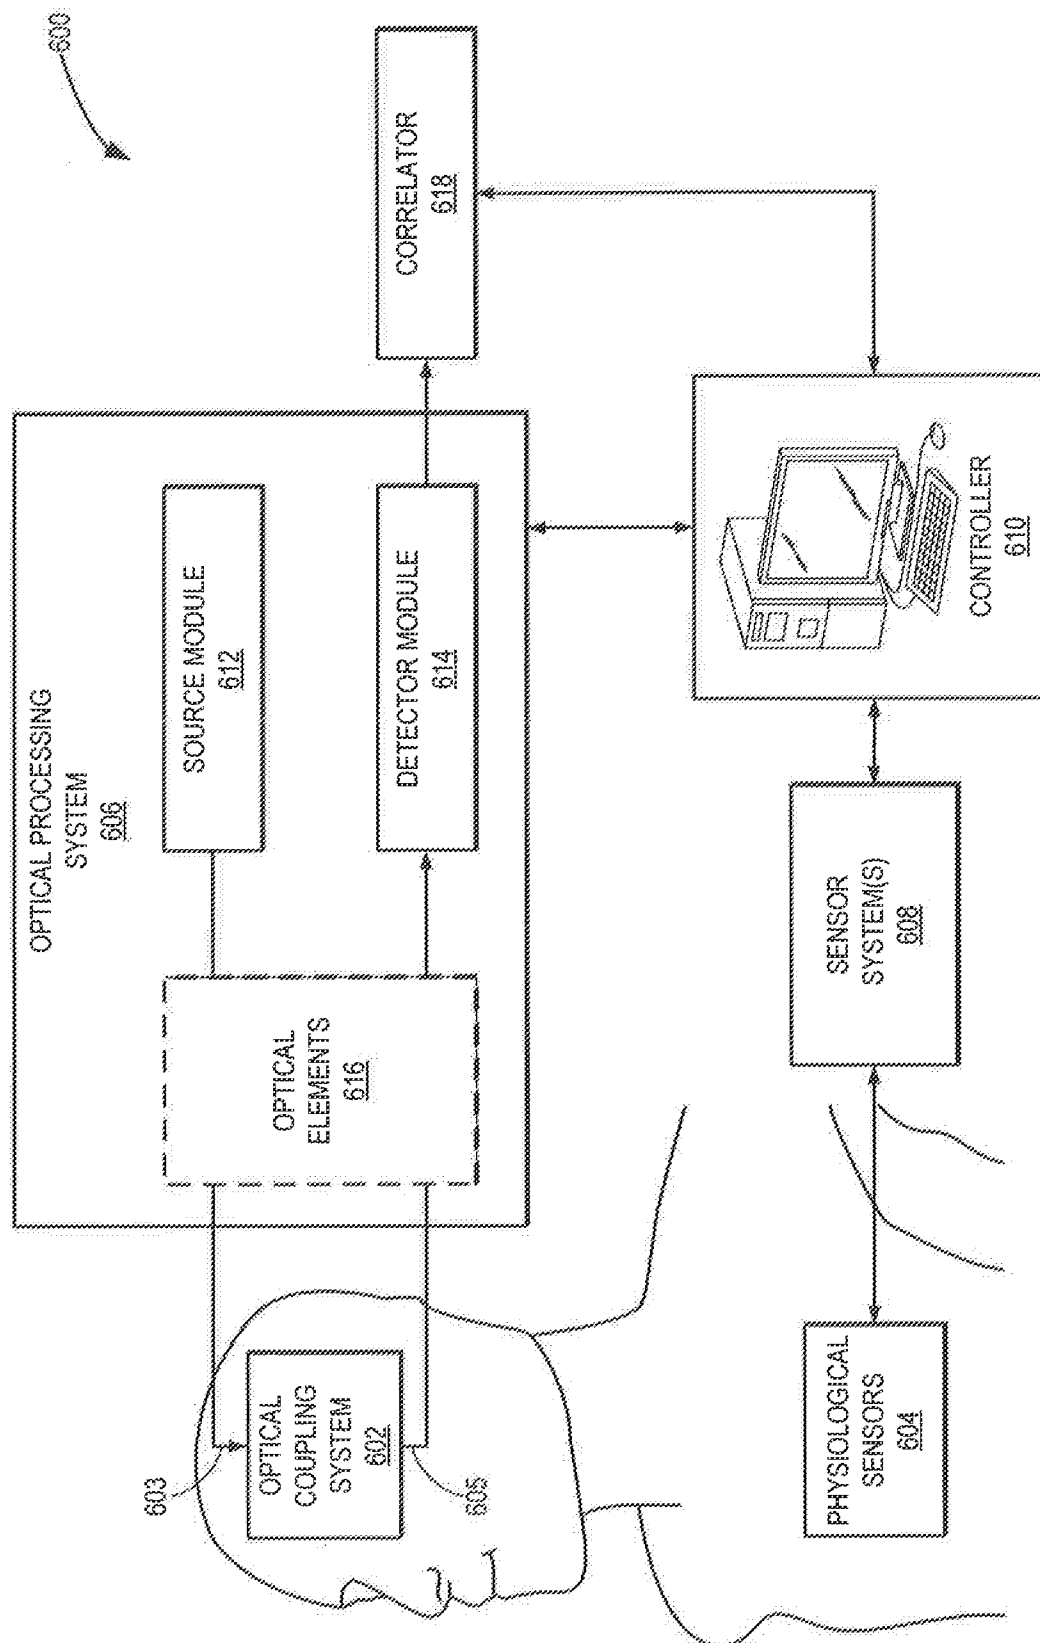


FIG. 6

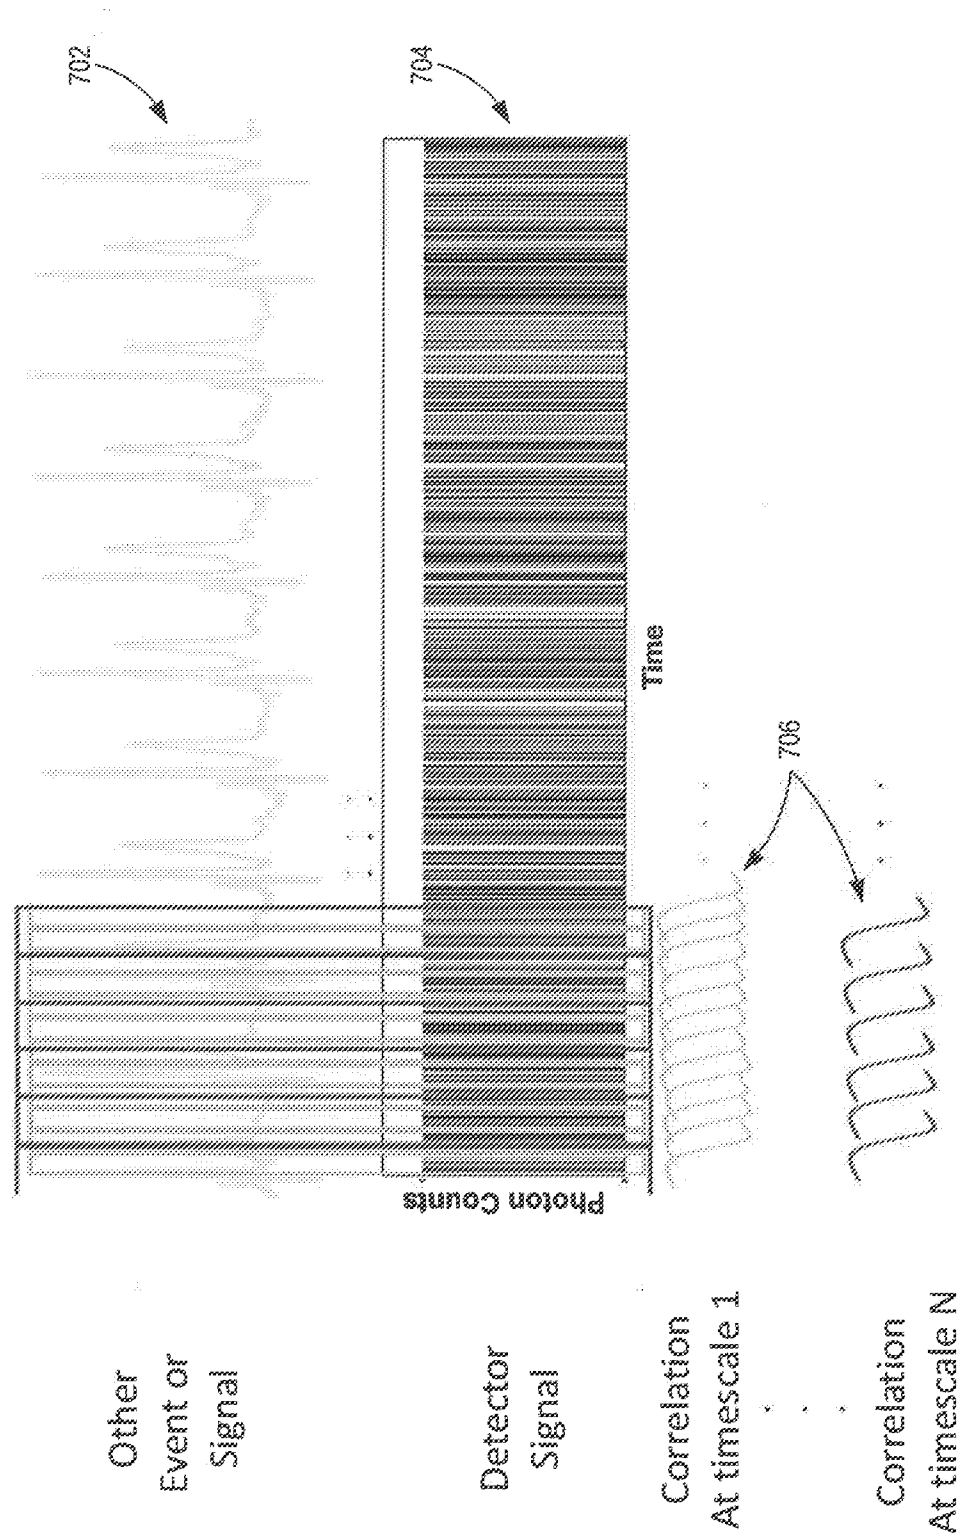


FIG. 7

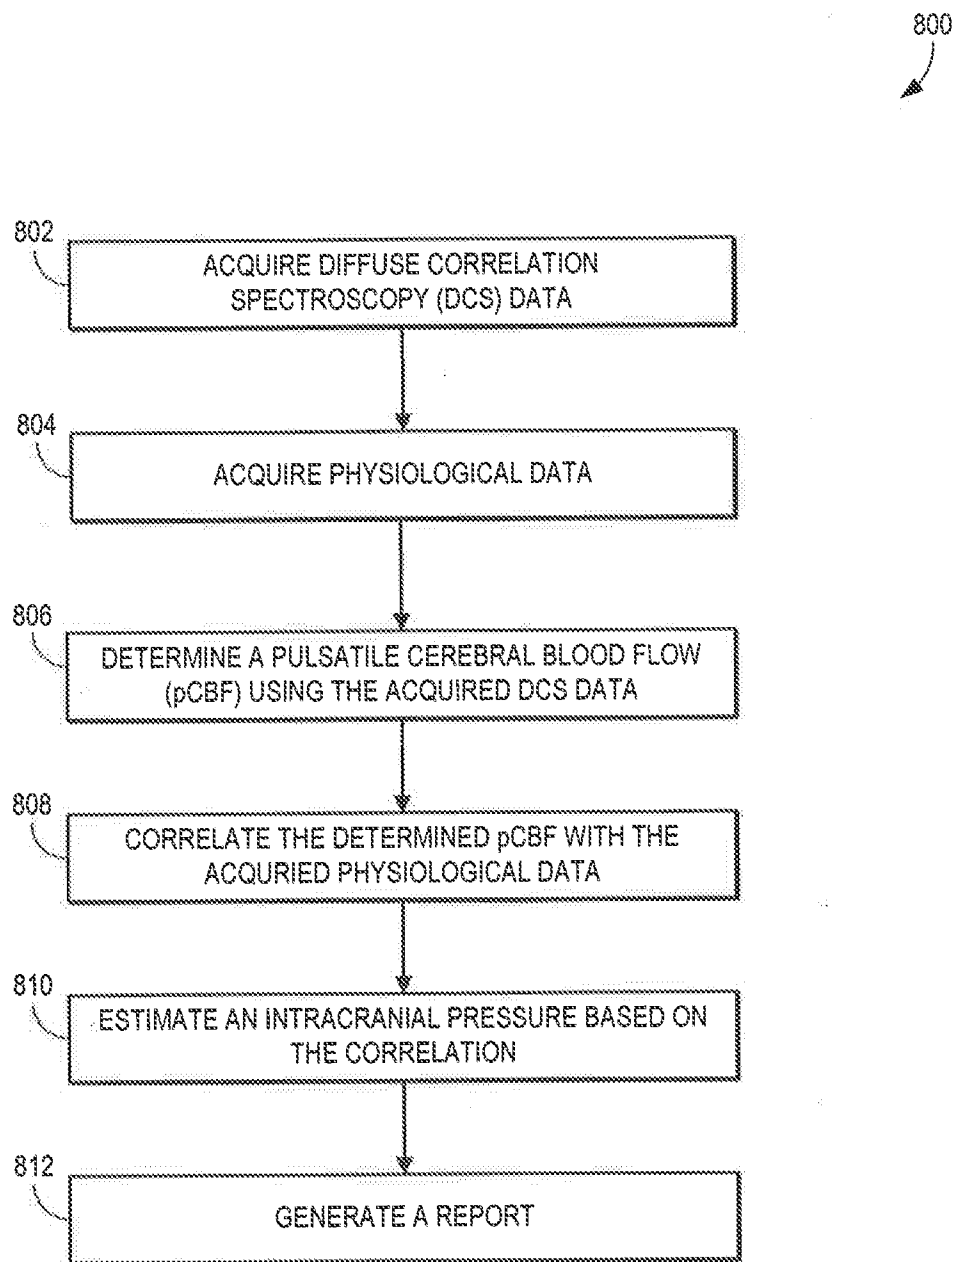


FIG. 8

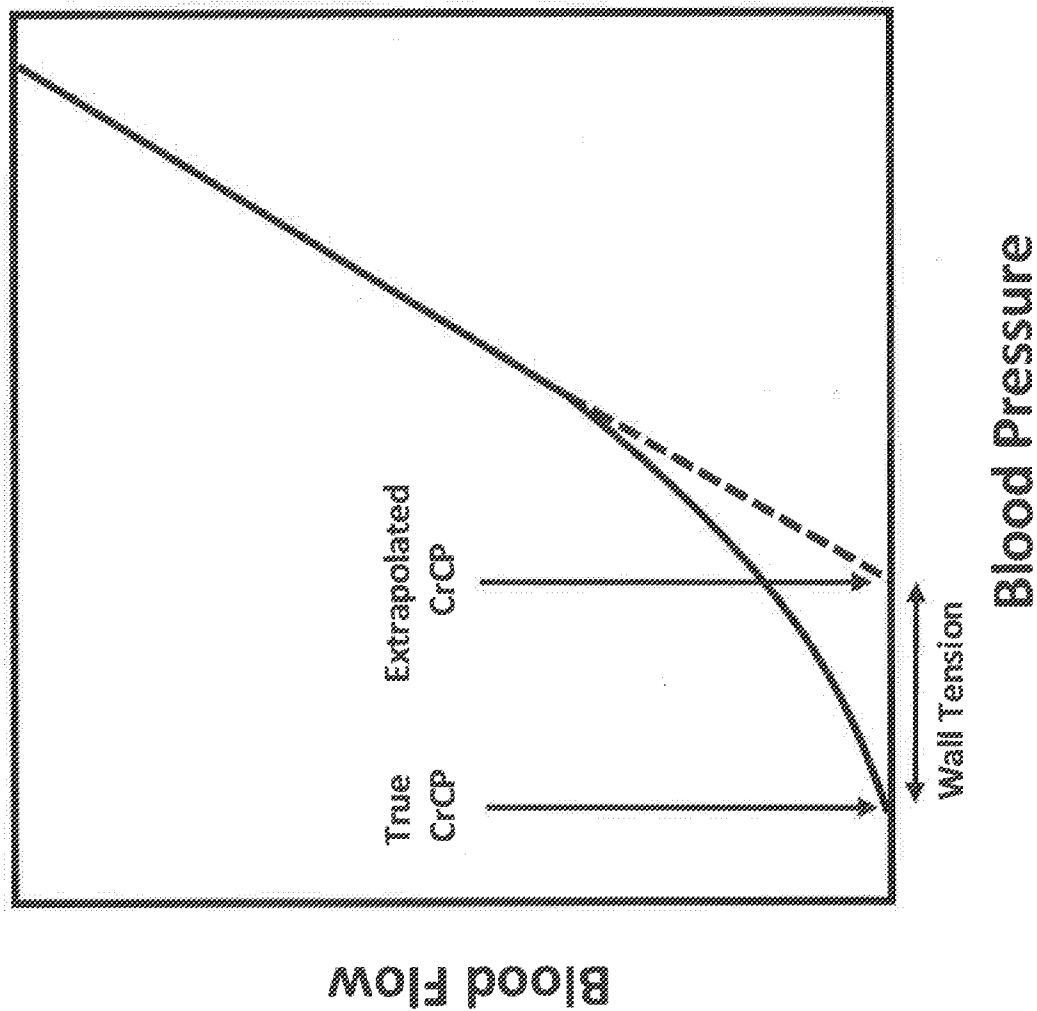


FIG. 9

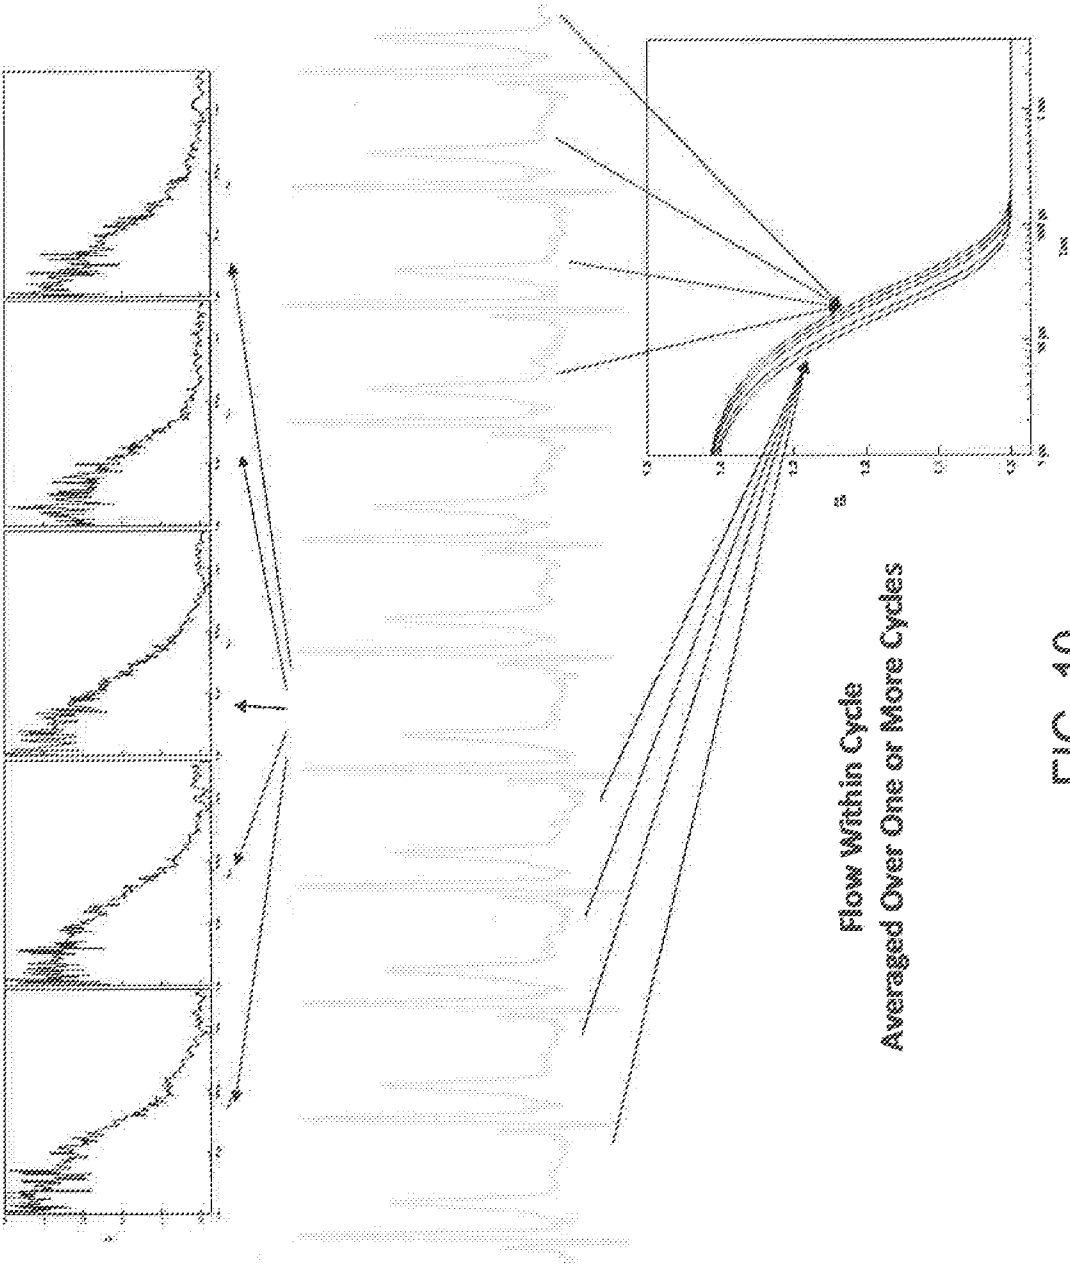


FIG. 10

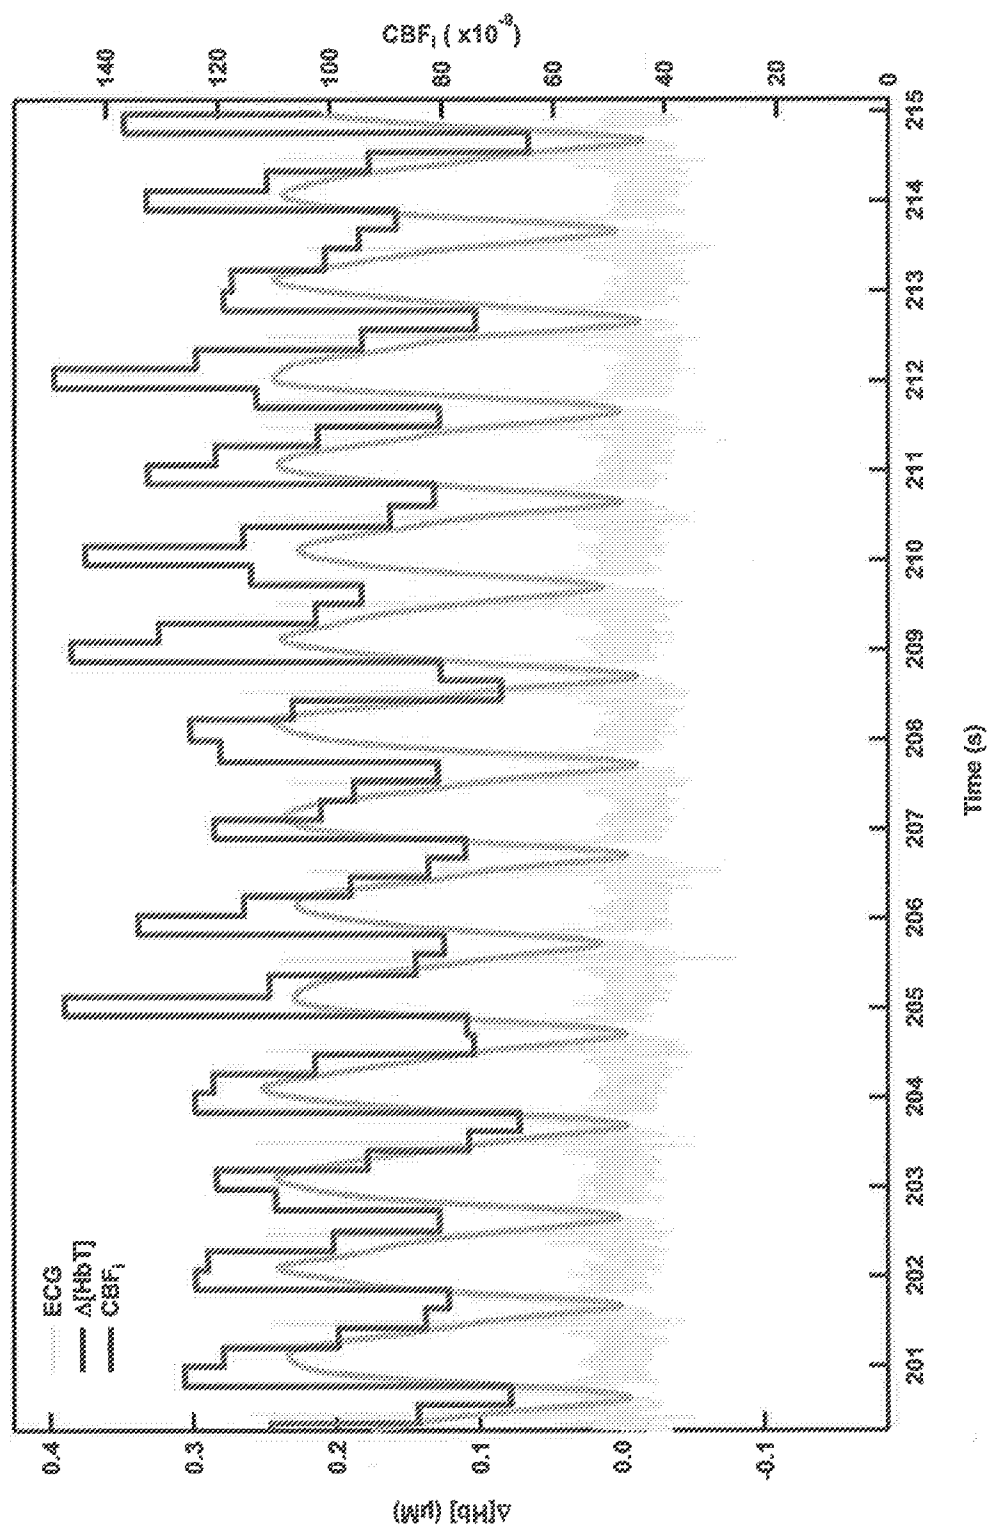


FIG. 11A

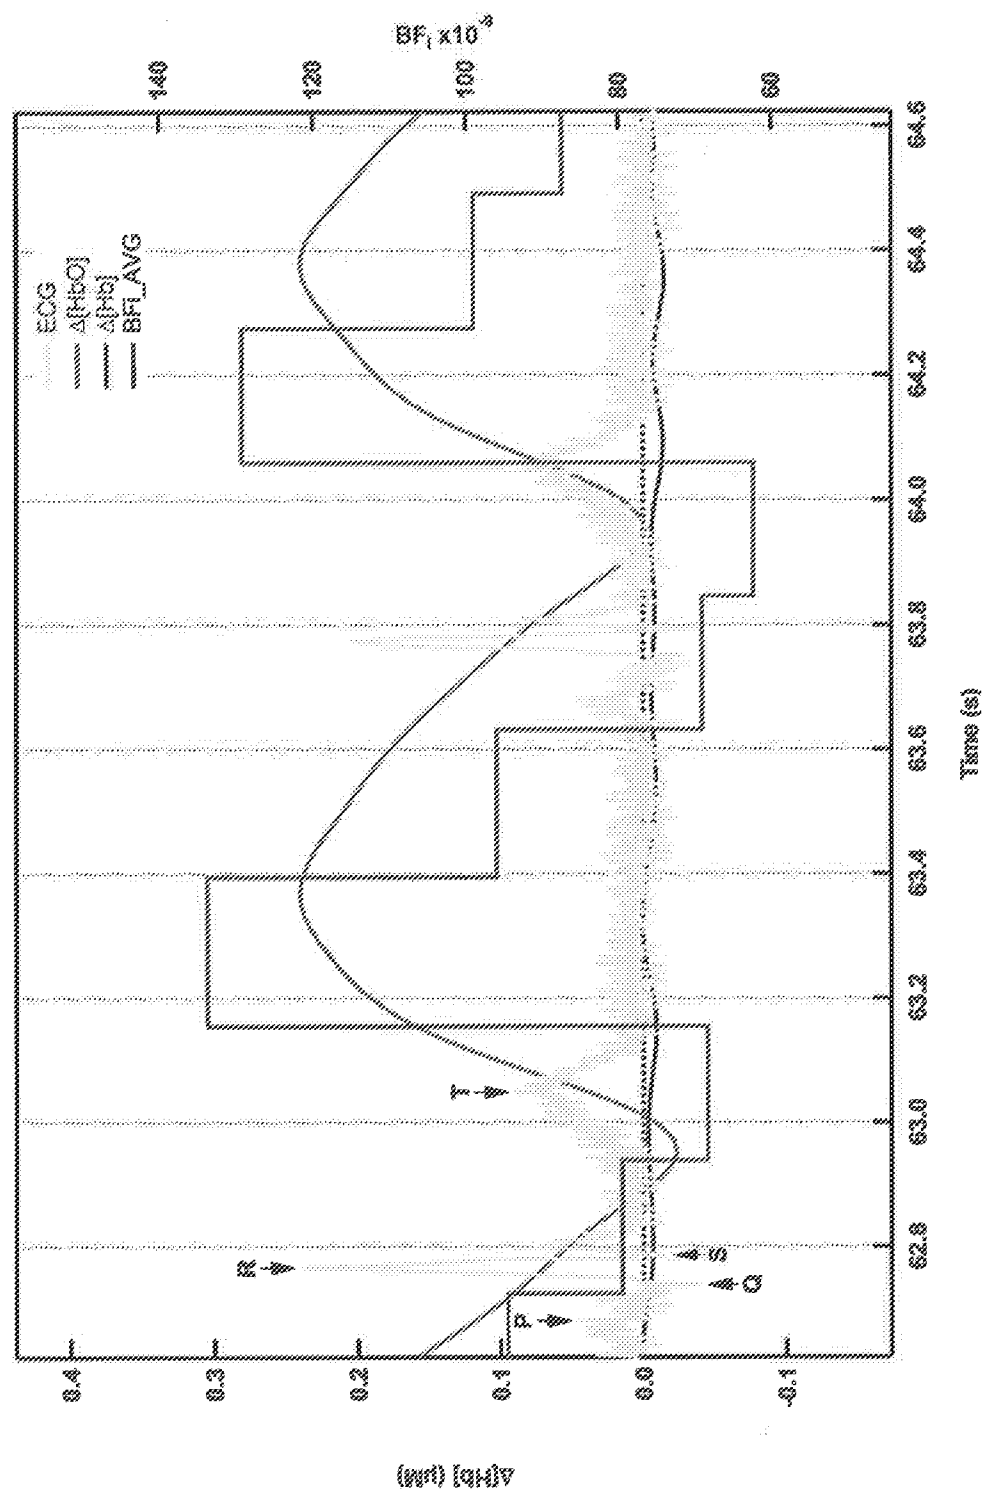


FIG. 11B

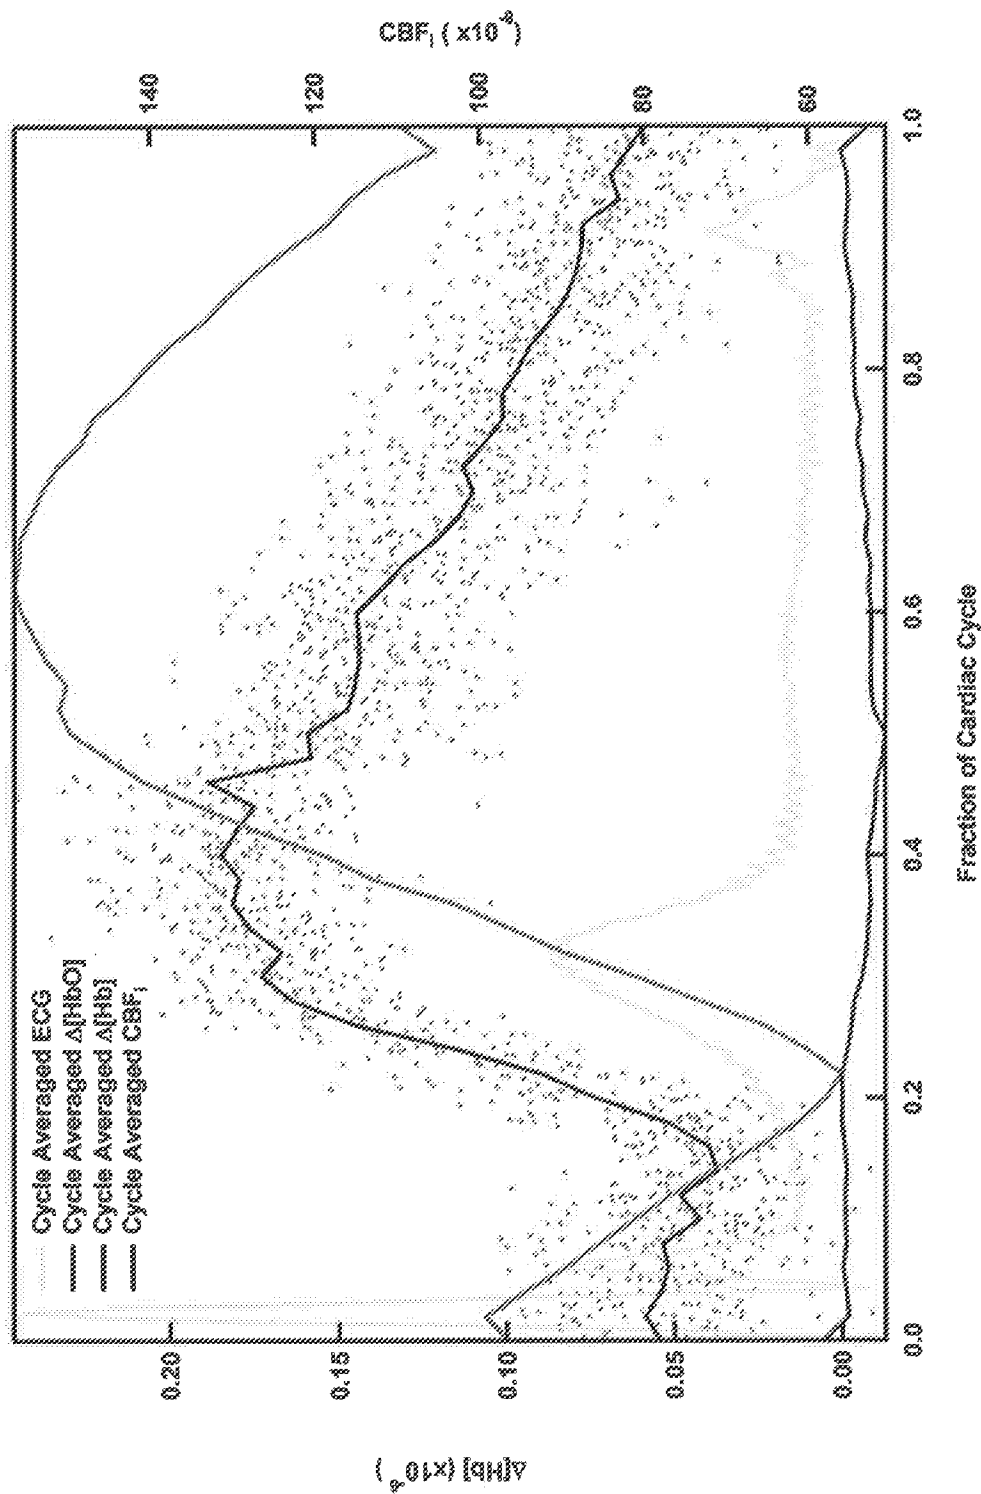


FIG. 11C

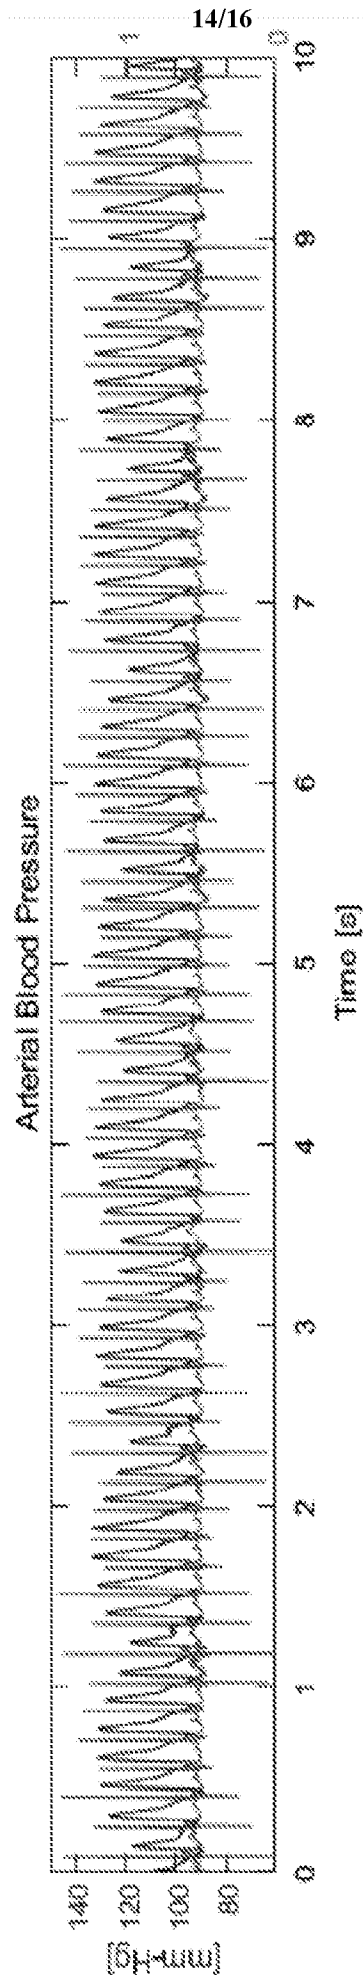


FIG. 12

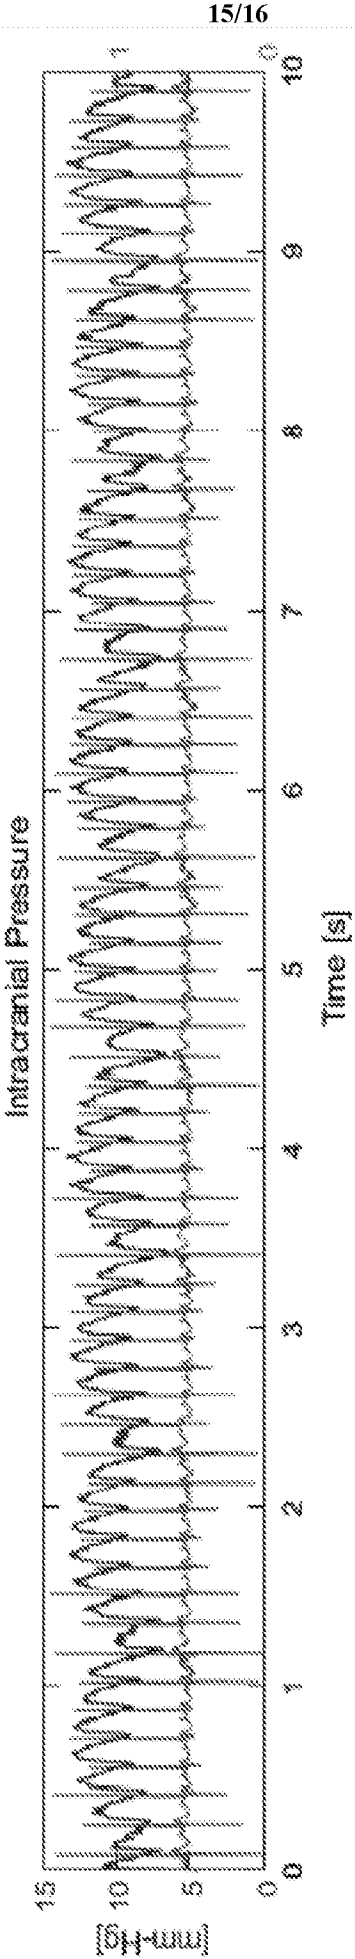


FIG. 12 continued

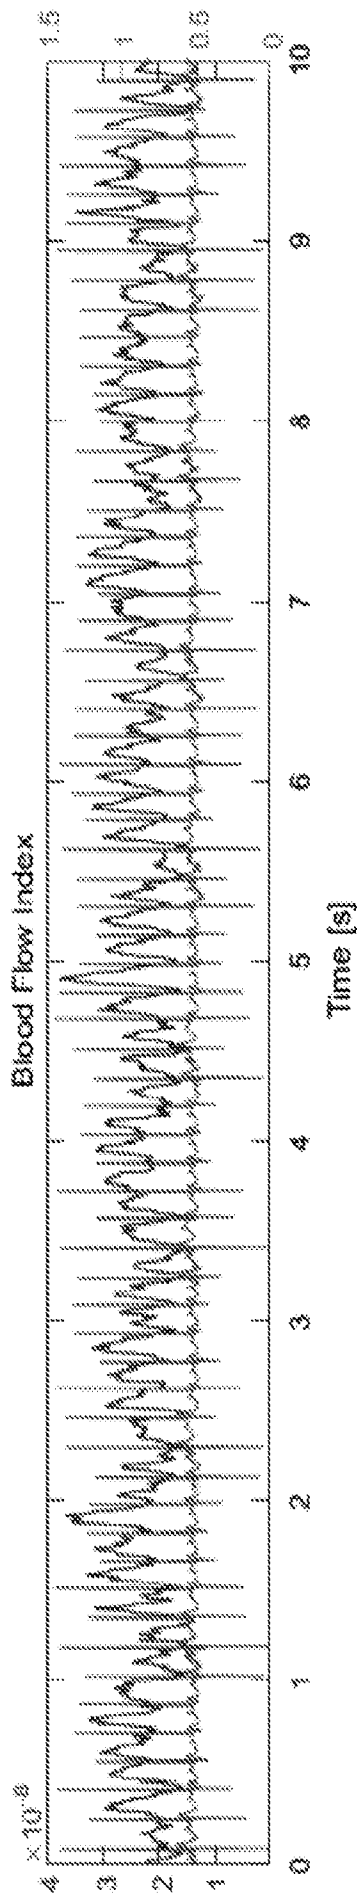


FIG. 12 continued

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2016/026920

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 5/026; A61B 5/0476; A61B 5/1455; A61B 5/1459; A61B 6/00; G01J 3/40 (2016.01)

CPC - A61B 5/02; A61B 5/026; A61B 5/0476; A61B 5/1455; A61B 5/14551; A61B 5/1459 (2016.05)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8) - A61B 1/00; A61B 5/00; A61B 5/02; A61B 5/026; A61B 5/0476; A61B 5/1455; A61B 5/1459; A61B 6/00; G01J 3/40 (2016.01)
CPC - A61B 1/00; A61B 5/00; A61B 5/02; A61B 5/026; A61B 5/0476; A61B 5/1455; A61B 5/14551; A61B 5/1459; A61B 6/00; G01J 3/40; G01N 21/64; G01N 21/65; G06F 17/00; G06F 17/10; G06K 7/00; G06K 7/10; G06K 19/00; G06K 19/06 (2016.05)Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
U.S. - 235/454; 235/494; 348/42; 356/302; 600/339; 600/340; 600/476; 600/485; 600/504; 600/544; 702/23 (keyword delimited)

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

Orbit, Google Patents, Google Scholar

Search terms used: blood flow, non-invasive, spectrometry, detect, cerebral, sensor, monitor, method

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2010/0268096 A1 (BERKA et al) 21 October 2010 (21.10.2010) entire document	1-23
Y	US 2010/0168586 A1 (HILLMAN et al) 01 July 2010 (01.07.2010) entire document	1-23
A	US 2009/0062685 A1 (BERGETHON et al) 05 March 2009 (05.03.2009) entire document	1-23
A	US 2010/0241006 A1 (CHOI et al) 23 September 2010 (23.09.2010) entire document	1-23
A	US 2013/0172703 A1 (DIXON et al) 04 July 2013 (04.07.2013) entire document	1-23
A	WO 2007/097702 A1 (LINDBERG LARS-GOERAN et al) 30 August 2007 (30.08.2007) entire document	1-23

☐ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

07 June 2016

Date of mailing of the international search report

07 JUL 2016

Name and mailing address of the ISA/

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, VA 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774