



- (51) **International Patent Classification:**
A61C 1/06 (2006.01) *A61C 5/40* (2017.01)
- (21) **International Application Number:**
PCT/EP2018/057405
- (22) **International Filing Date:**
23 March 2018 (23.03.2018)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
102017000032045 23 March 2017 (23.03.2017) IT
- (72) **Inventor; and**
- (71) **Applicant: PEDULLA, Eugenio** [IT/IT]; Corso Italia, 104, 95129 Catania (IT).
- (74) **Agent: DR. WILMING, Martin** et al.; Hepp Wenger Ryffel AG, Friedtalweg 5, 9500 Wil (CH).
- (81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,

(54) **Title:** DEVICE AND METHOD FOR CONTROLLING AN ENDODONTIC MOTOR

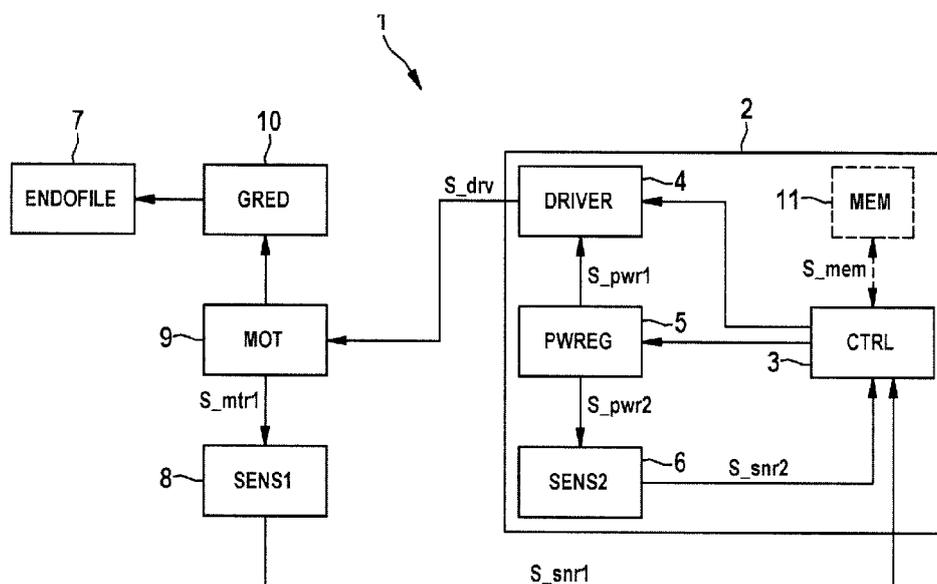


Fig. 1

(57) **Abstract:** The invention describes a method and a device for controlling an electric motor (9), in particular for moving an endodontic instrument. The device has a first sensor (8) and a control unit (2). The control unit (2) has a drive unit (4), a second sensor (6) and a processing unit (3). The processing unit (3) is configured to cause the endodontic instrument (7) to perform a sequence of movements (M1, M2). The sequence of movements (M1, M2) includes a continuous forward movement (M1) and at least one alternating movement (M2). The sequence may include an additional alternating movement (M3) and and/or reverse movement (M4). The number and order of movements to be performed in a sequence depends on a set of predefined threshold values reflecting the torque load applied to the instrument, as measured by means of a sensor.



EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

DEVICE AND METHOD FOR CONTROLLING AN ENDODONTIC MOTOR

The present invention concerns a device and a method for controlling an electric motor for moving an endodontic instrument.

5 The present invention also concerns an electric motor that is designed to move an endodontic instrument.

There exist commercially available endodontic devices that mainly comprise a root canal instrument that is designed to drill the tooth surfaces, in particular one or more
10 interchangeable endodontic files, and an associated electric motor designed to drive said instrument in a predetermined working motion, typically unidirectional rotation.

In particular, different types of dedicated micromotors for endodontic care are used, all of which have very similar
15 characteristics relating to the type of file used by the device during the work. The motors used all have a file rotation speed of between 100 and 1000 rpm with a maximum torque limit of around 8 N/cm.

In recent years, the use of nickel titanium instruments for
20 endodontic preparation has become more widespread.

Said instruments can be used in root canals with a continuous rotary movement provided by a handpiece connected to an endodontic motor, which enables rotational speeds of between 100 and 1000 rpm.

25 Continuous rotation at this speed enables high-performance high-speed work.

Such rotational speeds can be used with Ni-Ti instruments, but cannot be used with traditional steel instruments, since Ni-Ti alloys are superelastic and are therefore flexible and elastic (or have shape memory), such as to enable the instrument to
5 enter the canals while rotating, cutting the dentine circumferentially without deforming, even when following a curved path.

Devices driving the instrument in a reciprocal or alternating motion are known, rotating same in a direction of rotation at a
10 given angle first clockwise and then anti-clockwise, or vice versa. This clockwise/anti-clockwise rotation cycle can be repeated very quickly during the treatment. Furthermore, in having two directions of rotation, the instrument has two
15 potentially useful directions, with each direction having a specific function. For example, a file can be designed with dual functionality, in which the file cuts when rotating clockwise and polishes when rotating anti-clockwise, or vice versa.

In such known devices, the reciprocal action occurs at pre-set angular velocities and angles that cannot be changed, and said
20 reciprocal action is maintained from the start of the movement until the end of the movement.

In recent times, nickel titanium (Ni-Ti) root canal instruments have been developed that are able to perform a reciprocal
movement and that require specific rotational speed and angular
25 velocity values in both directions of rotation in order optimize performance of the instrument and to minimize the drawbacks thereof, such as breakage during use.

In particular, the instrument is run continuously and caused to reciprocate at fixed angles when a predetermined set resistive
30 torque is reached.

US 2015086937 A1, filed by Morita, describes a method for driving an endodontic instrument that controls the direct and inverse rotation as a function of the load/torque detected by the cutting means. In particular, the motor begins with a continuous rotary movement until a certain torque value is reached. When one of the predetermined torque values is reached, the predetermined reciprocal action is started.

DE 102007011725 B4, filed by Schlumbohm, describes an endodontic instrument with a reciprocal or twisting function having predefined values. There is an instant of delay when switching from the continuous movement and the twisting movement, and vice versa.

EP 2 431 004, filed by Nakanishi, discloses a motor control method for a dental handpiece configured to limit the motor current flowing through the motor when a specific load torque applied to the cutting tool exceeds a preset limit. The direction of rotation of the file is changed only occasionally.

WO2010/109464, filed by Forum Engineering, discloses a system for endodontic treatment comprising oscillation of a file through an arc α (e.g. 120°) at a certain frequency and starting from a certain angular position. After some time, the position of the oscillation center is advanced (e.g. for 60°) while maintaining the other parameters constant. Advancement of the position of the oscillation center along the circular arc is repeated until an entire circle is described.

US2013/0224677, filed by Morita Manufacturing, discloses a dental treating apparatus comprising a driving unit which is able to perform normal rotation, rotation opposite to normal rotation, and so called twist driving. The dental apparatus comprises a controller which compares a detected load applied to

the cutting tool to predefined reference loads. When such reference load is exceeded, the controller either reduces rotation angle speed of normal rotation as compared to reverse rotation or reduces the rotation angle in the normal rotation as compared to the rotation angle of the reverse rotation.

One drawback of this prior art is the dependence on the type of material used for the endodontic instrument, since the parameters are rigid and pre-set for the specific material used. Another drawback of the known endodontic devices is the risk of the instrument jamming or breaking when moving inside the canal. Indeed, when in movement, if the instrument hits the canal wall as a result of being too long, the instrument can undergo a sudden uncontrolled forward acceleration, which may cause the instrument to jam, be damaged and even to break inside the root canal.

Another drawback of the known endodontic devices is the need to exert greater manual pressure on the handpiece, and therefore on the endodontic instrument, during the reciprocating movement, compared to the pressure exerted during a continuous movement. This increases the risk of the endodontic instrument breaking, of debris being compacted towards the tip, and of dentinal defects (microcracks) appearing that could damage the tooth and cause the loss thereof (extraction).

Another drawback of the known endodontic devices is that the dental material is pushed towards the bottom of the root canal during forward movement of the instrument with a fixed reciprocating motion.

Another drawback of the prior art is that the beneficial effects of periodic reciprocation of a movement of the endodontic instrument, also called twist driving, have not always been

taken into account when designing a motor control which is responsive to measured torque.

Another drawback of the prior art is that, while rotational patterns to reduce the load applied to the endodontic file are well known in the art, there are no patterns disclosed which allow the cutting force to be either reduced or intensified depending on the resistance experienced by the instrument. It is, however, important to provide a function to increase forward rotational angle and/or forward rotational angle speed in order to prevent the dentist from having a perception of "stall" of the instrument and to, therefore, exert an unnecessary force on the instrument.

The main objective of the present invention is to provide a device and a method for controlling an electric motor, in particular to move an endodontic instrument such as to achieve an entirely uninterrupted movement in all of the movement modes and with any type of endodontic instrument.

Another aspect of the present invention is to provide a device and a method for controlling an electric motor for moving an endodontic instrument such as to achieve the easy and fluid penetration of the root canal during endodontic shaping, with a consequent reduction in the pressure required to move the instrument forward.

Another aspect of the present invention is to provide a device and a method for controlling an electric motor for moving an endodontic instrument such as to reduce the debris pushed beyond the tip and microcracks, compared to fixed reciprocal actions with fixed predetermined parameters and angles.

Another aspect of the present invention is to provide a device and a method for controlling an electric motor for moving an endodontic instrument that is efficient and safe.

Another aspect of the present invention is to provide a device and a method for controlling an electric motor, in particular for moving an endodontic instrument made of any nickel titanium alloy, that is simple to use.

According to the application, the device and method for controlling an electric motor, in particular for moving an endodontic instrument has the following advantages:

- provides a high degree of flexibility in the materials used for the endodontic instrument, being optimized both for conventional Ni-Ti instruments and heat-treated Ni-Ti instruments,
- 15 - enables operation at suitable speed and torque values at all times,
- reduces the risk of excessive torque and pressure being applied to the instrument,
- reduces the accumulation of stress inside the material of the endodontic instrument,
- 20 - reduces the risk of stalling,
- enables the continuous removal of material and debris from the root canal,
- enables activation of endodontic instruments with a movement that is adjusted continuously and automatically as a
- 25

function of the type of root canal being treated and the instrument being used.

The present invention concerns a device for controlling an electric motor, in particular for moving an endodontic instrument, as defined in attached Claim 1 and by the preferred 5 embodiments thereof, as described in Claims 2 to 20.

The present invention also concerns an electric motor that is designed to rotate an endodontic instrument, using a device such as the one defined in attached Claim 21.

10 The present invention also concerns a method for controlling an electric motor, in particular for moving an endodontic instrument as defined in attached Claims 22 to 25, and a method for controlling an endodontic instrument as defined in claim 26.

The above mentioned problems remaining in the prior art are 15 solved by a device for controlling an electric motor for moving a tool, in particular for moving an endodontic instrument, said device being configured to cause the tool to perform a sequence of movements (M1, M2) as a function of the signals received from at least one sensor. The sequence of movements (M1, M2) 20 comprises an initial movement (M1) being a continuous forward rotation in which the motor is driven in a normal direction of rotation, causing a high torque intensity on the tool, and maintaining such movement until a first maximum threshold limit (LM1) is surpassed. When said first maximum threshold limit 25 (LM1) is surpassed, the device is configured to switch to a first alternating movement (M2) in which the motor is driven in an alternating rotation, causing a lower torque intensity on the tool than initial movement (M1), and maintaining such movement until a first minimum threshold (Lm1) is fallen below. When a 30 first minimum threshold (Lm1) is fallen below, the device is

configured to switch back to initial movement (M1) and to, in (M1), observe the conditions for maintaining movement (M1) or switching back to movement (M2).

The electric motor may for example be an AC, DC or BL-DC
5 (brushless DC) motor or micromotor of a known type.

The at least one sensor is designed to receive a signal (S_mtr1) from said electric motor and to forward a signal (S_snrl) indicating a set of characteristic operating parameters of the motor to a processing unit.

10 The device is configured to, when used as intended, move the tool according to a sequence of movements. The movements can be continuous rotational movements or can be alternating movements, that is repeated rotations in a normal direction, each of them followed by a rotation in a reverse direction. The movements
15 have different intensities, depending on the rotational speed, depending on the power supplied to the device, depending on the rotation angle chosen for the normal and the reverse movement respectively, and depending on the pause taken when the direction of rotation of the drive shaft is inverted.

20 By normal movement or continuous forward movement is understood a rotation around a longitudinal axis of an instrument in a rotational direction where the instrument, preferably an endodontic file, exerts a substantial cutting force on the root canal.

25 By reverse movement is understood a rotation around a longitudinal axis of an instrument opposite to the normal rotation, in a rotational direction where the tool, preferably an endodontic file, exerts a cutting force lower than the cutting force exerted during normal rotation. In the reverse

movement, the endodontic file may have merely polishing function.

By twisting movement or alternating movement is understood a rotation around a longitudinal axis of an endodontic instrument in a normal direction through a first angle of rotation, followed by a rotation around the same longitudinal axis of an endodontic instrument in the reverse direction through a second angle of rotation, while the normal and reverse rotations are repeated periodically. The alternating movement is a forward movement, though not a continuous movement. It follows a regular pattern and causes less torque intensity on the tool than the normal movement.

Whether or not the normal rotation / reverse rotation follows a clockwise or an anticlockwise sense depends on the respective surface properties of the blade of the tool. In particular, it depends on the cutting ability and/or polishing ability of the blade when rotated in a clockwise or anticlockwise sense.

It is an advantage of the present invention that depending on the parameters chosen for each movement (M1, M2) and due to the possibility to switch from one movement to the other when a predefined maximum or minimum threshold is surpassed, unique treatment sequences for each root canal result. The sequences are built up based on the results measured by the sensor, without a need for the dentist to decide on the steps to be followed.

The switch from one to the next movement (from M1 to M2) as well as the switch from an advanced movement to one of the previous movements (M2 to M1) is chosen automatically based on a feedback value that a sensor receives and which is compared by the processing unit to a predefined threshold value. The values

received from the sensor might be processed before comparing it to a predefined threshold value. Preferably the feedback value reflects the torque load experienced by the tool.

Basing the choice of sequence on such feedback signal provided by a sensor turns out to be more accurate and less error prone than a sequence chosen, somewhat arbitrarily, by the dentist. In other words, the root canal treatment which is performed by means of the disclosed instrument does not depend on the skill of the dentist. When using conventional driving means for endodontic instruments, the dentist must perform "pecking" movements or "up and down" movements in order to avoid stall and to continuously forward the root canal processing, while allowing relief to the strained instrument as appropriate. When using a device according to this invention, such up-and-down movement is no longer necessary due to the ability of the device to switch either to higher torque load rotational treatment of the tool or to lower torque load rotational treatment of the tool. An automatic switch between different levels of torque intensity movements avoids blocking of the file and provides for progression instead. Excessive torque or uncontrolled pecking movements, both involving a risk of breakage of the instrument, can be reduced. Due to the adaptability of the movement sequence, the dentist can treat the root canal by applying continuous light pressure towards the apex. The torque load experienced by the instrument is monitored and kept within reliable limits. More safe and continuous advancement is ensured.

In a preferred embodiment of the invention, the device is configured to cause the tool to additionally perform a second alternating movement (M3) causing a lower torque intensity on the tool than the first alternating movement (M2). The switch from the first alternating movement (M2) to the second

alternating movement (M3) is triggered when during performance of the first alternating movement (M2) a second maximum threshold (LM2) is surpassed. In the second alternating movement (M3), the device is configured to switch back to one of the previous movements (M1 or M2), when a second minimum threshold (Lm2) or third minimum threshold (Lm3) is fallen below. In particular, the device switches back to the initial movement (M1), when a third minimum threshold (Lm3) is fallen below, and the device switches back to the first alternating movement (M2), when a second minimum threshold (Lm2) is fallen below. When performing such previous movements (M1, M2), the conditions for maintaining one of the previous movements (M1, M2) or for switching to a neighboring movement are again observed.

It is an advantage of this preferred embodiment that the device offers more levels of torque applied to the instrument and thus more levels of intensity of treatment. This allows for more precise treatment which is better adaptable to the shape and hardness of the processed areas of the root canal.

Starting from one of the alternating movements (M2 or M3), the sequence can jump back to one of the previous movements, if the feedback value falls below at least one of two predefined threshold values. Due to this switch back to higher intensities, the dentist is not induced to apply unnecessary force by pushing the instrument towards the apical part of the root canal. Unnecessary strain experienced by the instrument can be avoided and the risk of breakage can be reduced.

In a preferred embodiment, the device is configured such that, in the first alternating movement (M2) or in the second alternating movement (M3), after completion of a predefined angle α_2 of rotation ($\alpha_{\text{effective}} > \alpha_2$) or α_3 of rotation ($\alpha_{\text{effective}} > \alpha_3$) respectively, the device automatically switches to the

previous higher torque movement or to the subsequent lower torque regardless of any threshold value being reached. Whether or not the switch occurs to a lower torque intensity movements or to a high torque intensity movement then depends on whether
5 or not the characteristic parameters received from the motor (S_{snr1} , S_{snr2}) are above or below a mean value of RS , current drawn by the motor, force absorbed by the motor, or surpass a predefined RS error value. It is an advantage of this embodiment that the user does not experience stagnation. Such feeling of
10 stagnation could result from an instrument staying for a substantial amount of time in an alternating movement. The maximum angles of rotation α_2 and α_3 can thus improve controlled handling of the device.

It is not foreseen that the sequence jumps a subsequent
15 movement, for example, it is not foreseen that the second alternating movement ($M3$) is executed right after movement $M1$. Continuous advancement allows to proceed from ($M1$) to ($M2$) and to ($M3$) through directed, controlled decrease of intensity of the treatment without disruption. However, jumping an intensity
20 decreasing level is, though not preferred, still within the scope of the present invention.

It goes without saying that more alternating movements $M3'$, $M3''$, $M3'''$ and so on, causing even lower torque intensity on the tool, can follow alternating movement $M3$. In this case, the
25 switch from the second alternating movement ($M3$) to the subsequent alternating movement ($M3'$) is triggered when during performance of the second alternating movement ($M3$) a third maximum threshold ($LM3$) is surpassed.

In another preferred embodiment of the invention, the device is
30 configured to cause the tool to additionally perform a conclusive movement ($M4$) in which the motor is driven in a

continuous reverse rotation, causing a low torque intensity on the tool. The switch from the second alternating movement (M3) to conclusive movement (M4) is triggered when during performance of the second alternating movement (M3) a third maximum
5 threshold (LM3) is surpassed.

When the conclusive movement (M4) is performed, the device can be particularly well be removed from the root canal. The conclusive movement can also support removal of debris from the root canal. By conclusive movement (M4) is meant the movement
10 concluding one treatment cycle. The conclusive movement causes less torque on the instrument than its predecessor movements within one treatment cycle do.

In a preferred embodiment, the device is configured such that, in movement M4, after completion of a predefined angle α_4 of
15 rotation ($\alpha_{\text{effective}} > \alpha_4$), the device automatically switches to initial movement (M1) regardless of any threshold value being reached. The device may thus be configured, and such configuration is preferred, to repeat the treatment cycle after
occurrence of M4. It is an advantage of repetition of treatment
20 cycles that continuous advancing of the treatment is ensured without the need for the user to apply pressure towards the apex. Such repetition of cycles is discussed below in greater detail.

In a preferred embodiment, the device for controlling an
25 electric motor for moving a tool, in particular for moving an endodontic instrument, comprises, a first sensor that is designed to receive a signal (S_mtr1) from said electric motor and to generate a signal (S_snrl) indicating first
characteristic operating parameters (RS; RD; RP; PS) of the
30 motor.

The device further comprises a control unit that is in data communication with said motor and said first sensor, the control unit comprising

- 5 - a drive unit that is designed to power the motor by means of a power supply voltage (S_drv);
- a second sensor that is designed to generate a feedback signal (S_snr2) that is proportional to a second operating parameter received from the motor, said second sensor being in data communication with the drive unit; and
- 10 - a processing unit in data communication with said drive unit, said first sensor and said second sensor.

Said processing unit is designed to cause the endodontic instrument to perform a sequence of forward movements (M1, M2) by acting on said electric motor as a function of the first
15 signal (S_snr1) received from the first sensor and the second signal (S_snr2) received from the second sensor, the sequence of movements (M1, M2) comprising a start with a continuous forward movement (M1) in which the motor is driven in rotation with a first supplied power (PS1), a first rotational speed (RS1) and a
20 first direction of rotation (RD1). When a first threshold limit (LM1) is surpassed, a first alternating movement (M2) is started. In the first alternating movement, the motor is driven in rotation with a second supplied power value (PS2), a second rotational speed (RS2), a first clockwise angle of rotation
25 (CWA2), a first anti-clockwise angle of rotation (CCWA2) and a second pause (RP2) between said first clockwise angle of rotation (CWA2) and said first anti-clockwise angle of rotation (CCWA2).

Preferably, the device is configured such that in the first alternating movement (M2) a lower torque intensity is applied on the tool than in initial Movement M1. Movement (M2) is maintained until a first minimum threshold (Lm1) is fallen
5 below. In the case of falling below Lm1, the device is configured to switch back to the initial movement (M1) and to, in M1, observe the conditions for maintaining initial movement (M1) or switching back to the first alternating movement (M2).

For the purposes of this invention, by the characteristic
10 parameter of the motor "RSX" is understood the rotational speed of the drive shaft; by the characteristic parameter of the motor "RDX" is understood the direction of rotation of the drive shaft; by the characteristic parameter of the motor "CWAX" is understood the clockwise angle of rotation of the drive shaft;
15 by the characteristic parameter of the motor "CCWAX" is understood the anti-clockwise angle of rotation of the drive shaft; by the by the characteristic parameter of the motor "RPX" is understood the pause time in one of the alternating movements (M2 or M3) when the direction of rotation of the drive shaft is
20 inverted.

In a preferred embodiment, the device comprises a first sensor which is designed to receive a signal (S_mtr1) from the electric motor. The sensor forwards the signal (S_snrl) to the processing unit within the control unit. The signal indicates a set of
25 first characteristic operating parameters of the motor. The characteristic parameters in particular include RSX, RDX, CWAX, CCWAX and RPX.

In a preferred embodiment the first sensor is a Hall effect sensor which more preferably consists of a set of three Hall
30 effect sensors that enables identification of six different phases of forward movement of the motor. The first sensor can

preferably be an encoder position sensor, translating the angular position of the drive shaft into a digital value. By means of the Hall effect sensor or sensors, a speed error may be detected, that is a deviation from the set speed. The speed error can be calculated by a suitably calibrated proportional-derivative controller. By means of three Hall effect sensors, the relevant characteristic parameters of the motor are detectable. Feedback from additional, optional sensors can be used as indicators for verifying accuracy of the calculated values.

In a preferred embodiment, the control unit is in data communication with the motor and the first sensor. The control unit comprises a drive unit, it comprises a second sensor, and it comprises a processing unit.

The drive unit is designed to power the motor by means of a supply voltage (S_{drv}). The drive unit preferably receives a signal (S_{drv}) from a power regulator to regulate the electrical power to be sent to the motor and, additionally, a signal from the processing unit. In particular, the control unit regulates the period of the PWM signals to be sent to the driver while the power regulator regulates the duty cycle of the PWM signal to be sent to the driver.

The second sensor is designed to receive a second operating parameter of the motor. Preferably, the second sensor measures the current drawn by the motor. However, the second sensor can be a force sensor designed to forward a feedback signal (S_{snr2}) proportional to the force absorbed by the motor. The second sensor serves as an indicator of the load to which the motor is subject in order to determine any movement switches.

It is an advantage of the present invention that the control system is able to evaluate the torque applied to the instrument based on the feedback of one, preferably two sensor units.

More details on the first and the second sensor, the control unit, the drive unit, the processing unit and the data communication between the units are given in the section discussing examples and figures.

The processing unit receives the signals from the first and, the second sensor (S_{snr1} , S_{snr2}) and is designed to cause the tool to perform the sequence of movements ($M1$, $M2$) described earlier. The processing unit, in particular, compares the data received from a sensor and compares the data to predefined values which are stored in a memory unit. Based on the signals received from the sensor, the processing unit may calculate values which can be compared to at least one of the predefined threshold values $LM1$, $LM2$, $Lm1$, $Lm2$, $Lm3$. Threshold values $LM1$, $LM2$, $Lm1$, $Lm2$, $Lm3$ reflect a torque experienced by the endodontic instrument.

In a preferred embodiment, the processing unit is designed to cause the endodontic instrument to perform a sequence of forward movements ($M1$, $M2$, $M3$). When a second threshold limit ($LM2$) is surpassed, a second alternating movement ($M3$) is started in which the motor is driven in rotation with a third supplied power value ($PS3$), a third rotational speed ($RS3$), a third clockwise angle of rotation ($CWA3$), a third anti-clockwise angle of rotation ($CCWA3$) and a third pause ($RP3$) between said third clockwise angle of rotation ($CWA3$) and said third anti-clockwise angle of rotation ($CCWA3$).

The second threshold limit $LM2$ is a maximum value and the started second alternating movement ($M3$) causes lower torque intensity on the tool than the first alternating movement ($M2$).

In the second alternating movement (M3), the device is further configured to switch back to one of the previous movements (M1 or M2), when a second minimum threshold (Lm2) or third minimum threshold (Lm3) is fallen below. In particular, the device
5 switches back to the initial movement (M1), when a third minimum threshold (Lm3) is fallen below, and the device switches back to the first alternating movement (M2), when a second minimum threshold (Lm2) is fallen below. When performing the previous movements (M1, M2), the conditions for maintaining one of the
10 previous movements (M1, M2) or for switching to a neighboring movement are observed.

In a preferred embodiment of the invention, the device is configured to, when the third threshold limit (LM3) is surpassed, start a fourth reverse movement (M4), in which the
15 motor is driven to withdraw the endodontic instrument from the canal. For example the blade of the file can be structured in a way that, when performing reverse movement (M4), the tool has merely polishing function. The fourth movement allows for relief of strain and safe removal of the instrument. Preferably, the
20 conclusive movement (M4) is a continuous reverse rotation in which the motor is typically driven with a fourth supplied power (PS4), a fourth rotational speed (RS4) and a fourth direction of rotation (RD4).

The benefit of having several alternating movements and a
25 reverse movement is improved adaptability of the sequence (M1, M2, M3, M4) to the shape and hardness of the processed areas of the root canal. The advantages of switching from low torque intensity movements back to higher torque intensity movements have been described earlier.

In one embodiment, the characteristic operating parameters of the motor (9) relating to the forward movement (M1, M2, M3) are selected such as to satisfy one or more of the following rules:

- 5 a) if the first direction of rotation (RD1) is clockwise, then
CWA2 > CCWA2;
- b) if the first direction of rotation (RD1) is anti-clockwise,
then CWA2 < CCWA2;
- c) if the first direction of rotation (RD1) is clockwise, then
CWA3 > CCWA3;
- 10 d) if the first direction of rotation (RD1) is anti-clockwise,
then CWA3 < CCWA3;
- e) $RS1 > RS2 > RS3$;
- f) $|CWA2 - CCWA2| > |CWA3 - CCWA3|$;
- g) $PS1 < PS2 \leq PS3$.

15 It is an advantage of rules a and b, that -regardless of the properties of the cutting blade of the file - in the first alternating movement, the rotation angle of the normal or forward movement is larger than the rotation angle of the reverse movement. Substantial cutting activity can be ensured.

20 It is an advantage of rules c and d, that - regardless of the properties of the cutting blade of the file - in the second alternating movement, the rotation angle of the normal or forward movement is larger than the rotation angle of the reverse movement. Substantial cutting activity can be ensured.

It is an advantage of rule e, that rotational speed RS is continuously decreased from the initial movement (M1) over the first alternating movement (M2) to the second alternating movement M3. By choosing decreasing parameters, it is ensured
5 that no excessive force or load is applied to the instrument and the risk of breakage is reduced. Moreover, the reduction of speed allows a reduced cyclic fatigue accumulation which is one of the main causes of Ni-Ti endodontic file intra-operative breakage. The rotational speed reduction is an advantage for
10 instruments of large dimensions usually used in the shaping phase of root canal treatment that have a low cyclic fatigue resistance. Instruments with a low cyclic fatigue resistance usually have also a high torsional resistance, therefore, rule e can be indicated when Ni-Ti endodontic instruments are used in
15 narrow and constricted root canals where the torsional stress could be very high.

It is an effect of rule f, that by setting the parameters for alternating as defined, excessive force or load applied to the instrument can be avoided. According to rule f, the delta of the
20 rotational angle of the normal rotation minus the rotational angle of the reverse rotation is larger during the first alternating movement (M2) than during second alternating movement M3. The directional surface of the file having high cutting force therefore processes the root canal to a greater
25 extent in the first alternating movement (M2) than it does in the second alternating movement (M3). This rule applies especially to shaping instruments that are used after creation of a glide-path, i.e. in the shaping phase. They should cut from the beginning of their use. However, the decreasing delta
30 between normal and reverse angle from the first (M2) to the second alternating movement (M3) allows for gradual shaping of the root canal and for decreasing creation of debris. The reduced amount of debris created can be easily removed.

Both rules e and f are particularly suitable when instruments are used for the shaping phase of the root canal. Rule e is particularly suitable when heat-treated Ni-Ti instruments are used in the shaping phase of the root canal treatment. Rule e may be changed to Rule e' when traditional Ni-Ti instruments are used in the shaping phase of the root canal treatment. According to alternative rule e'', the rotational speed may be increased from movement (M1) to movement (M2) and again decreased from movement (M2) to movement (M3) ($RS1 < RS2 > RS3$).

10 When the sequence switches to lower cutting force movements (such as M2 or M3), the power supplied to the motor is preferably increased or, at least, kept constant. It is an advantage of this rule (g) that the supplied power is increased as the instrument experiences increasing friction. By providing
15 such increased power the risk of blockage of the file can be reduced.

Optionally, also the duration of the pauses between normal rotation a reverse rotation during alternating movements can be increased from a first (M2) to a second alternating movement
20 (M3) in order to relief strain.

In an alternative embodiment, the characteristic operating parameters of the motor relating to the forward movement (M1, M2, M3) are selected such as to satisfy one or more of the rules a, b, c, d and g. However, in this embodiment, the
25 characteristic parameters are selected to satisfy one or more of the following alternative rules e' and f':

$$e') \quad RS1 < RS2 < RS3$$

$$f') \quad |CWA2-CCWA2| < |CWA3-CCWA3|$$

Alternative rules e' and f' are particularly suitable when instruments are used for the glide-path phase of the root canal. Rule e' is particularly suitable when heat-treated Ni-Ti instruments are used in the glide-path phase of the root canal treatment. Yet another alternative rule e'' is suitable when traditional Ni-Ti instruments are used in the glide-path phase of the root canal treatment. According to alternative rule e'', the rotational speed may be increased from movement (M1) to movement (M2) and again decreased from movement (M2) to movement (M3) ($RS1 < RS2 > RS3$).

Alternative rule e' can be suitable when, by applying higher centrifugal force to the instrument, torque load can be lessened. The reduction of torque applied on instruments reduces torsional stress accumulation, one of the main causes for intra-operative breakage of Ni-Ti endodontic instruments. Increasing rotational speed is an advantage for instruments of small dimensions usually used in the gliding path phase of root canal treatment that have a low torsional resistance. Instruments with a low torsional resistance usually have a high cyclic fatigue resistance. Therefore, alternative rule e' could be indicated when Ni-Ti endodontic instruments are used in curved root canals where the cyclic fatigue stress could be very high.

Similarly, alternative rule f' can be suitable when by providing the file with higher cutting force in M3 as compared to M2, torque load can be lessened. This is advantageous for high capacity advancement immediately after the root canal is accessed, that is when glide-path instruments are applied with the aim to create a smooth glide-path. The increasing delta between normal and reverse angle from the first (M2) to the second alternating movement (M3) allows for an easy advancement of the file inside the root canal.

Generally speaking, increasing or decreasing the rotational speed and/or the delta of rotational angles in M2 versus M3 will depend on the materials used (steel, traditional Ni-Ti, heat-treated Ni-Ti) and their relevant properties (flexibility, yield strength, hardness, torque resistance, cyclic fatigue resistance), on the size of the instrument as well as the type of root canal to be treated (curved shape, narrow shape). Also it will depend on the type and phase of the root canal treatment to be performed.

10 By offering different modes of operations and different characteristic parameters for the transitions of one movement to the other, the present invention turns out to be a highly adaptable tool.

Preferably, the second sensor of the device is a current sensor designed to generate a feedback signal (S_snr2) proportional to the current drawn by the motor and to send said signal to the processing unit. In an alternative embodiment, however, the second sensor of the device is a force sensor designed to generate a feedback signal (S_snr2) proportional to the force absorbed by the motor and to send said signal to the processing unit.

In a preferred embodiment, the device is configured to store reference values (RSi; RDi; CWAi; CCWAi; RPi) of the first characteristic parameters (RSX; RDX; CWAX; CCWAX; RPX) of each movement (Mi) of the sequence of forward movements (M1, M2, M3) are pre-set in a memory module in data communication with the processing unit. The stored values allow the processing unit to compare the reference values to effective values and to monitor possible deviations and discrepancies.

In a preferred embodiment, the device is configured to store reference values (MDi; MPCi; mPCi; mDi) for each maximum threshold limit (LMi) and each minimum threshold limit (Lmi). Each maximum threshold limit (LMi) and each minimum threshold limit (Lmi) includes one or more of the following values:

- a) maximum drive power consumption (MPCi) by the electric motor during the forward movement (Mi);
- b) energy draw time (MDi) by the electric motor above the maximum drive power consumption (MPCi);
- 10 c) minimum drive power consumption (mPCi) by the electric motor in the forward movement (Mi);
- d) energy draw time (mDi) by the electric motor below the minimum drive power consumption (mPCi).

During operation, the processing unit may continuously process the retrieved values RSX; RDX; CWAX; CCWAX; RPX; PSX. The processing unit may then compare the results of such processing accumulated over time to the reference values MDi; MPCi; mPCi; mDi.

For the purposes of this invention, LMi shall mean a maximum threshold value and Lmi shall mean a minimum threshold value, both parameters reflecting the torque or load experienced by the tool. According to one embodiment of the invention, a maximum threshold limit LMi is surpassed, when either the time Ti elapsed between sending of the control signal (S_drv) and receipt of the incoming feedback signal (S_snr1) from the first sensor by the processing unit exceeds a predetermined value (MDi):

$$T_i > MD_i$$

or when the power drawn by the electric motor (S_{snr2}) exceeds a predetermined maximum drive power consumption value (MPC_i) by the motor for a time (T_i) greater than the predefined maximum time (MD_i):

$$(\text{Consumption} > MPC_i) \text{ during } (T_i > MD_i)$$

It is an advantage of the method based on the time difference between sending a control signal an incoming feedback signal that the second sensor detecting force or current drawn by the motor is made redundant.

It is an advantage of the method based on power consumption measured over time that values falling below a predefined minimum value mPC_i can be detected.

According to the invention a minimum threshold limit L_{mi} is fallen below, when the power drawn by the electric motor (S_{snr2}) falls below a predetermined minimum drive power consumption value (mPC_i) by the motor for a time (T_i) greater than the predefined maximum time (mDi).

$$(\text{Consumption} < mPC_i) \text{ during } (T_i > mDi)$$

By advancing through the movement sequence in ascending index order M_1, M_2, M_3, M_4 , the torque applied to the instrument is thus lessened.

More details and typical values for threshold torque, RS , CWA , $CCWA$ are given in the section discussing examples and figures.

In a preferred embodiment, the device is configured such that during alternating movements (M_2 and M_3), the characteristic

parameters of the motor are determined only within the phase of normal rotation, because the friction and, thus, the torque is highest when an angle that produces feed is described.

In an even more preferred embodiment, the characteristic parameters of the motor are determined only during the normal rotation phase where the rotation describes an inner angle of rotation α , positioned between an initial angle of normal rotation α_i and a final angle of normal rotation α_f . It has proven advantageous to neglect the characteristic parameters measured through an initial angle α_i , preferably $\alpha_i = 0^\circ$ to 10° , of a normal rotation phase. More preferably, the parameters to be neglected are those measured through an angle of $\alpha_i = 0^\circ$ to 6° of the normal rotation phase. It has proven advantageous to also neglect the characteristic parameters measured through a final angle α_f , preferably $\alpha_f = (\text{angle } \alpha - 20^\circ)$ to $(\text{angle } \alpha - 0^\circ)$, of a normal rotation phase, for example through an angle of 162° to 180° in case the normal rotation angle is 180° .

This phase of normal rotation is suitable to deliver values which best reflect the torque applied to the instrument. The initial phase is usually subject to high consumption of current and/or slow response of the instrument because a certain amount of energy is used to reverse the rotational direction. The final phase, on the other hand, might be subject to low consumption of current and/or little delay of response of the instrument. In particular, forcing a defined minimum angle α_i before the characteristic parameters are determined delivers greater stability and reliability of values.

In a preferred embodiment, the device is configured to automatically activate a warning sound when a predefined number nI of starts of reverse movement $M4$, preferably a predefined number between 5 and 15, is surpassed. The number of starts of

reverse movements can be assessed by means of a counter which counts the number of starts of M4, nR. In addition to emitting the warning signal, the angle α_4 defining the duration of movement (M4) can be increased, for example doubled or tripled, in order to allow the dentist to interrupt the treatment and/or to irrigate the tooth. If the operator chooses to interrupt the treatment by releasing the pedal, the counter nR is reset. Otherwise the counter is increased further, repeating the same behaviour when reverse movement (M4) is entered the next time. Most preferably, the number of cycles nI is 10.

This feature reminds the dentist to periodically remove the debris from the instrument. When the debris is not removed in due time, not only the cutting force of the blades may be impaired, there is also a risk that the dentist pushes debris towards the apex and creates dentin debris plugs which will block the advancement of the treatment. The feature serves patient safety. However, the dentist has the option, if he considers appropriate, to restart the engine for another number nI of treatment cycles.

In another embodiment, the device is configured to automatically activate a prolonged warning sound and to permanently maintain reverse movement (M4), when a predefined number nS of starts of reverse movement (M4) is surpassed. To exit reverse movement M4, the user must release the pedal and thus stop the engine. This feature is provided to indicate that the instrument has undergone substantial torque for numerous times and should be replaced in order to reduce the risk of fracture.

Both the warning sound after nI completed treatment cycles and nS completed treatment cycles have the advantage that they invite the dentist to re-evaluate the situation. They provide

guidance for when to consider irrigation and when to replace the instrument.

Furthermore, the system can be better adapted to the type and shape of the root canal to be treated. For example, if the canal to be treated is not too narrow, there will be little torque on the instrument and it will be difficult to reach the value that leads to reverse movement (M4) and to the end of a treatment cycle. The warning signals will be emitted after considerable advancement of the instrument. In the case where, instead, the canal to be treated is very tight, there will be a lot of torque on the instrument and easily the value that leads to emission of a warning sound is reached. The higher number of times the dentist will be reminded to stop and to irrigate the tight canal is appropriate given that the instrument in the tight canal undergoes high strain. Blocking of the instrument and formation of apical debris plugs is prevented, due to the automatic signal periodically suggesting irrigation of the canal.

The invention also relates to a method for controlling an electric motor to move a tool, in particular an endodontic instrument, the control method including a sequence of movements (M1, M2) as a function of the signals received from a sensor. The method may additionally include a second alternating movement (M3) and/or a conclusive movement (M4).

The described properties of each movement and the conditions to switch from one to the other have been described above and will be given in the section describing examples and figures.

The invention also relates to a method for controlling an electric motor, in particular to move an endodontic instrument, including the following phases: receiving a signal (S_snr1) indicating first characteristic operating parameters (RSX; RDX;

RPX; PSX) of the motor; powering the motor with a power supply voltage (S_drv); receiving a feedback signal (S_snr2) proportional to a second operating parameter of the motor; causing the endodontic instrument to perform a sequence of
5 movements (M1, M2, M3, M4) by acting on said electric motor.

The described properties of each movement and the conditions to switch from one to the other have been described above.

Other characteristics and advantages of the invention are given in the description of a non-exclusive preferred embodiment and
10 the variants thereof, given by way of non-limiting example with reference to the attached drawings, in which:

- Figure 1 is a schematic functional block diagram of an endodontic device according to one embodiment of the present invention, and
- 15 - Figures 2A and 2B are schematic flowcharts of a method for controlling an electric motor, in particular for moving an endodontic instrument according to a first embodiment of the invention;
- Figure 3 is a schematic view of an endodontic system
20 including the device in Figure 1;
- Figure 4 is a schematic flowchart of a method for controlling an electric motor, executable during performance of reverse movement M4;
- Figure 5 is a schematic flowchart of an alternative method
25 for controlling an electric motor, executable during performance of reverse movement M4.

With reference to Figure 1, an endodontic device according to one embodiment of the invention is indicated as a whole using reference sign 1.

The device 1 principally comprises a control unit 2 that is
5 designed to cause the endodontic instrument 7 to perform a sequence of movements, and a motor 9 designed to drive the endodontic instrument 7 in rotation.

A reduction gear 10 is preferably arranged between the motor 9 and the endodontic instrument 7.

10 The motor 9 is preferably an electric motor and may for example include an AC, DC or BL-DC (brushless DC) motor or micromotor of a known type.

The electric motor 9 preferably has a cylindrical body arranged in a tubular seat (as shown in Figure 3).

15 The electric motor 9 is able to move a drive shaft that is connected via a handpiece to the endodontic instrument 7.

The electric motor 9 is associated with a first sensor 8 that is designed to receive a signal S_{mtr1} from the motor 9 and to generate a signal S_{snr1} in real time indicating first
20 characteristic operating parameters RS , RD , RP , PS of the motor 9.

The first characteristic parameters of the motor 9 may include one or more of the following: rotational speed RS_i of the drive shaft, the direction of rotation RD_i of the drive shaft, the
25 clockwise angle of rotation CWA_i of the drive shaft, the anti-clockwise angle of rotation $CCWA_i$ of the drive shaft, the pause time RP_i when the direction of rotation of the drive shaft 9 is

inverted (where i is in the range 1 to 4, for example RS1, RD1, RP1, RS2; RD2, RP2, CWA2, CCWA2, etc.).

The first sensor 8 is preferably an inductive brushless sensor that is coupled to the drive shaft and designed to detect the angular position of the shaft and to enable feedback control of the position of an element rigidly connected to the drive shaft. The first position sensor 8 is preferably a set of three Hall effect sensors that enables identification of six different phases of forward movement of the motor.

The first sensor 8 includes a rotor that is rigidly connected to the drive shaft and a stator carried on the housing of the electric motor 9 and arranged to face the rotor when in use.

The first sensor 8 can preferably be an encoder position sensor. Such a sensor or encoder translates the angular position of the drive shaft into a digital value (appropriately scaled).

The encoder used can be resistive, optical or magnetic.

The control device also includes a control unit 2 that is in data communication with the electric motor 9 and the first sensor 8.

The control unit 2 includes a drive unit 4 designed to power the motor 9 with a power supply voltage S_{drv} , and a second sensor 6 designed to generate a feedback signal S_{snr2} proportional to a second operating parameter of the motor 9. The second sensor 6 is in data communication with the drive unit 4.

The second sensor 6 can be a current sensor designed to generate a feedback signal S_{snr2} proportional to the current drawn by the motor 9 and to send said signal to the processing unit 3.

The feedback signal S_snr2 is preferably an analogue voltage value within the power supply range of the electric motor 9.

Alternatively, the second sensor 6 can be a force sensor designed to generate a feedback signal S_snr2 proportional to the force absorbed by the motor 9 and to send said signal to the processing unit 3.

The control unit 2 also includes a processing unit 3 in data communication with the drive unit 4, the first sensor 8 and the second sensor 6.

The control unit 2 is also preferably connected to a power regulator 5 designed to send a signal S_pwr1 to the drive unit 4. The signal S_pwr1 is used to regulate the electrical power sent by the driver 4 to the motor 9 by sending the signal S_drv. In particular, the control unit 3 regulates the period of the PWM signals to be sent to the driver 4 while the power regulator 5 regulates the duty cycle of the PWM signal to be sent to the driver 4. In general, it should be noted that, in the present context and in the subsequent claims, the control unit 2 is described as being split into different functional modules (memory modules or operating modules) solely for the purpose of describing the functionality thereof clearly and fully.

In fact, said control unit 2 can be a single electronic device suitably programmed to perform the functions described, and the different modules can be hardware units and/or software routines included in the programmed device. Alternatively or additionally, such functions can be performed by a plurality of electronic devices incorporating the aforementioned functional modules.

The control unit 2 can also have one or more processors for running the instructions contained in the memory modules.

The aforementioned functional modules can also be split between different local or remote processors as a function of the architecture of the network incorporating same.

The systems also include all of the means and/or memory modules and/or operating modules required to implement the functions described in the respective methods described.

The processing unit 3 is configured to cause the endodontic instrument 7 to perform a sequence of movements (M1, M2, M3, M4) by acting on the electric motor 9 as a function of the incoming first signal S_snr1 from the first sensor 8 and the second signal S_snr2 received from the second sensor 6.

The sequence of movements (M1, M2, M3, M4) includes a start with a continuous forward movement (Movement "M1") in which the electric motor 9 is driven in rotation with a first supplied power PS1, a first rotational speed RS1 and a first direction of rotation RD1.

When the first threshold limit L1 is surpassed, the processing unit 3 causes the motor to start a first reciprocating or alternating movement ("M2") in which the motor 9 is driven in rotation with a second supplied power value PS2, a second rotational speed RS2, a first clockwise angle of rotation CWA2, a first anti-clockwise angle of rotation CCWA2 and a second pause RP2 between the first clockwise angle of rotation CWA2 and the first anti-clockwise angle of rotation CCWA2.

When the second threshold limit L2 is surpassed, the processing unit 3 causes the drive shaft to perform a second alternating

movement ("M3"), that is preferably different to M2, in which the motor (9) is driven in rotation with a third supplied power value PS3, a third rotational speed RS3, a third clockwise angle of rotation CWA3, a third anti-clockwise angle of rotation CCWA3
5 and a third pause RP3 between said third clockwise angle of rotation CWA3 and said third anti-clockwise angle of rotation CCWA3.

Preferably, when a third threshold limit L3 is surpassed, the processing unit 3 causes the motor to perform a fourth reverse
10 movement M4 in which the motor 9 is driven to withdraw the endodontic instrument 7 from the canal. Subsequently, after a certain time (or delay), preferably between a few milliseconds and a few seconds, the motor can continue the movement M1.

The reference values RSi, RDi, CWAi, CCWai, RPi of the first
15 characteristic parameters of each movement Mi of the sequence of movements M1, M2, M3, M4 are pre-set in a memory module 11 in data communication with said processing unit 3. For example, the memory also contains the reference values RS2, RD2, CWA2, CCW2, RP2 of the first alternating movement M2.

20 The two tables below set out, by way of non-limiting example, values for threshold torque, rotation of the drive shaft, and clockwise and anti-clockwise angular rotation (for the alternating movements M2 and M3). The first table relates to traditional Ni-Ti endodontic instruments and the second table
25 relates to heat-treated Ni-Ti endodontic instruments. Both tables relate to sequences suitable for the shaping phase of a root canal treatment.

Traditional Ni-Ti instrument (shaping phase)				
Movement	Torque Nw	rpm	CWA angle	CCWA angle
M1	Start 0 Finish 1.0-2.0	250-300		
M2	Start 1.0-2.0 Finish down 0.5-0.8 Finish up 1.5-2.5	250-350	160°-110°	70°-20°
M3	Start 1.5-2.5 Finish down M2 1.3-1.5 Finish down M1 0.5-0.8 Finish up 4.0-5.5	150-250	120°-70°	60°-10°
M4	Start 4.5-6.0	300-400		

Heat-treated Ni-Ti instrument (shaping phase)				
Movement	Torque Nw (20-60% less traditional Ni-Ti)	rpm	CWA angle	CCWA angle
M1	Start 0 Finish 0.6-1.2	300-450		
M2	Start 0.6-1.2 Finish down 0.3-0.48 Finish up 0.9-1.5	300-400	220°-160°	140°-90°
M3	Start 0.9-1.5 Finish down M2 0.78-0.9 Finish down M1 0.3-0.48 Finish up 2.4-3.3	200-300	160°-120°	110°-80°
M4	Start 2.7-3.6	300-400		

5 The continuous forward movement M1 preferably occurs with a full
360° rotation, clockwise or anti-clockwise depending on the
specific endodontic instrument being used. If the endodontic
instrument encounters significant resistance in the dental canal
during the continuous forward movement M1, causing the torque
10 for the movement M2 to be surpassed before the 360° rotation is
completed, the consequent movement switch occurs immediately.
For example, if the torque suddenly rises, the movement M1 can

be switched immediately to the movement M2 after just 150°, 200°, 300°, etc.

The continuous movement M1 can be clockwise or anti-clockwise (set in advance using a suitable pushbutton) depending on the endodontic instrument being used. In fact, all of the movements Mi can change direction. For example, if an instrument is designed to cut clockwise, the prevailing angle of all of the movements M1-M2 and M3 is clockwise (CW) and M4 is the reverse and anti-clockwise (CCW). On the other hand, if the instrument being used is designed for anti-clockwise rotation, as set previously in the device, all of the parameters M1, M2 and M3 can be identical but in the opposite direction, i.e. a prevailing forward movement component that is anti-clockwise (CCW) and the movement M4 is the reverse and clockwise.

In one embodiment, for traditional Ni-Ti endodontic instruments, it is advantageous to have the following rotational speed values for the drive shaft: M1= 270 rpm, M2 = 300 rpm, M3 = 220 rpm.

Preferably, the rotational speed in the reverse movement M4 is the same but in the opposite direction, at the rotational speed of the movement M1.

In said embodiment, for heat-treated Ni-Ti endodontic instruments, it is advantageous to have the following rotational speed values for the drive shaft: M1 = 370 rpm, M2 = 320 rpm, M3 = 270 rpm.

The two tables below set out values for threshold torque, rotation of the drive shaft, and clockwise and anti-clockwise angular rotation (for the alternating movements M2 and M3). In contrast to the above example, the tables relate to sequences suitable for the glide-path phase of a root canal treatment. The

first table relates to traditional Ni-Ti endodontic instruments and the second table relates to heat-treated Ni-Ti endodontic instruments.

Traditional Ni-Ti instrument (glide-path phase)				
Movement	Torque Nw	rpm	CWA angle	CCWA angle
M1	Start 0 Finish 1.0-2.0	200-300		
M2	Start 1.0-2.0 Finish down 0.5-0.8 Finish up 1.5-2.5	150-350	130°-70°	70°-20°
M3	Start 1.5-2.5 Finish down M2 1.3-1.5 Finish down M1 0.5-0.8 Finish up 4.0-5.5	100-400	100°-60°	60°-10°
M4	Start 4.5-6.0	300-400		

It has proven advantageous, that the rotational speed RS of the drive shaft is 250 rpm in M1, 320 rpm in M2 and 200 rpm in M3, in accordance with rule e''. It is further preferred that the normal angle in M2 is 102° (CWA) while the reverse angle in M2 is 60° (CCWA); it is preferred that the normal angle in M3 is 84° (CWA) while the reverse angle in M3 is 24° (CCWA).

10 In an alternative example for driving a heat-treated Ni-Ti instrument, values for threshold torque, rotation of the drive shaft, and clockwise and anti-clockwise angular rotation (for the alternating movements M2 and M3) have been chosen as set out in the table below:

Heat-treated Ni-Ti instrument (glide-path phase)				
Movement	Torque Nw (20-60% less traditional Ni-Ti)	rpm	CWA angle	CCWA angle
M1	Start 0 Finish 0.6-1.2	400-600		

M2	Start 0.6-1.2 Finish down 0.3-0.48 Finish up 0.9-1.5	350-700	140°-60°	100°-40°
M3	Start 0.9-1.5 Finish down M2 0.78-0.9 Finish down M1 0.3-0.48 Finish up 2.4-3.3	300-800	100°-50°	80°-20°
M4	Start 2.7-3.6	300-600		

It has proven advantageous, in accordance with rule e', that the rotational speed RS of the drive shaft is 480 rpm in M1, 580 rpm in M2, 750 rpm in M3 and 300 rpm in M4.

Alternatively, in accordance with rule e, the rotational speed RS of the drive shaft can be chosen to 600 rpm in M1, 580 rpm in M2 and 500 rpm in M3.

It is further preferred that the normal angle in M2 is 90° (CWA) while the reverse angle in M2 is 60° (CCWA); it is preferred that the normal angle in M3 is 72° (CWA) while the reverse angle in M3 is 30° (CCWA).

The memory module 11 preferably also contains the reference values for each threshold limit Li.

The reference values MDi, MPCi, mPCi, mDi of each threshold limit Li (where i=1, 2, 3, 4) include one or more of the following values:

- a) maximum drive power consumption MPCi by the electric motor during the forward movement Mi,
- b) maximum time MDi that the energy drawn by the electric motor is greater than the maximum drive power consumption MPCi,
- c) minimum drive power consumption mPCi by the electric motor in the forward movement Mi,

- d) minimum time MD_i that the energy drawn by the electric motor 9 is less than the minimum drive power consumption mPC_i .

Preferably, the reference values MD_i , MPC_i , mPC_i , mD_i of each threshold limit Li and the reference values RS_i , RD_i , CWA_i , $CCWA_i$, RPI of the first characteristic parameters of each movement M_i of the sequence of forward movements are stored in the memory 11, at least for traditional Ni-Ti instruments and/or shaping instruments and for heat-treated Ni-Ti instruments and/or glide-path instruments. When the operator sets the type of Ni-Ti instrument being used, using a suitable pushbutton, the pre-set values are loaded by the memory 11 into the processing unit 3.

Preferably, some of the pre-set values loaded into the processing unit can be modified by the operator using appropriate pushbuttons 25 on a control panel 22 including a display 23 that is in data connection with a user interface module, which is in turn connected to the processing unit 3. In particular, the pre-set parameters that can be modified by the operator may include the angle of rotation CW and CCW and the rotational speed.

Consequently, the movement of the endodontic instrument is automatic and pre-set as a function of the file type (traditional Ni-Ti or heat-treated Ni-Ti) and/or of the phase of treatment (shaping phase, glide-path phase), although the speed and angle threshold values thereof are freely modifiable.

Before the endodontic operation on the patient is started, the operator need only set the following two options, which depend on the endodontic instrument being used and involve selecting:

1. The direction of rotation (prevalence of CW or CCW direction as a function of the instrument if done with the blades for cutting CW or CCW),
2. The type of movement as a function of the instrument being used (traditional Ni-Ti or heat-treated Ni-Ti) and/or the phase of treatment (shaping phase / glide-path phase) to be performed. The operator of the endodontic device 1 uses the control panel 13 to select a specific endodontic instrument or file for a given endodontic treatment, for example by pushing pushbuttons 12. Once the specific endodontic instrument has been selected, the processing unit 3 loads the parameters optimised for said instrument and endodontic treatment from the memory 11. Consequently, once the specific pre-programmed operating method has been selected, the unit 3 automatically loads the alternating motion operating values for one or both directions of rotation.

The processing unit 3 is also able to perform one or more operating rules on the first characteristic operating parameters of the motor 9, including the alternative rules e', e'' and f' outlined hereinbefore. The first characteristic operating parameters of the motor 9 relating to each forward movement M1, M2, M3 are preferably selected such as to satisfy one or more of the following rules:

- a) if the first direction of rotation (RD1) is clockwise, then $CWA2 > CCWA2$,
- b) if the first direction of rotation (RD1) is anti-clockwise, then $CWA2 < CCWA2$,
- c) if the first direction of rotation (RD1) is clockwise, then $CWA3 > CCWA3$,

- d) if the first direction of rotation RD1 is anti-clockwise,
then $CWA3 < CCWA3$,
- e) $RS1 > RS2 > RS3$,
- f) $|CWA2 - CCWA2| > |CWA3 - CCWA3|$,
- 5 g) $PS1 < PS2 \leq PS3$.

The invention also relates to a method for controlling an electric motor 9, particularly for moving an endodontic instrument 7, as shown in the flowchart in Figures 2A and 2B. Once the operator of the endodontic instrument has decided
10 whether to use a traditional Ni-Ti instrument or a heat-treated Ni-Ti instrument, the operator enters this information into the system using the pushbuttons 25 of the control console 22. As illustrated above, the operator must also enter whether the endodontic instrument being used is made with blades for cutting
15 clockwise (CW) or anti-clockwise (CCW). The control device automatically loads the threshold values characteristic of the endodontic instrument being used into the processing unit 3.

In particular, the control method includes the following phases:

- receiving a signal S_{snr1} from the electric motor 9,
20 preferably via a first sensor 8 linked to the motor 9, indicating first characteristic operating parameters RS_i ; RD_i ; RP_i ; PS_x of the motor 9,
- powering the motor 9 with a power supply voltage S_{drv} ,
- receiving, preferably from a second sensor 6, a feedback
25 signal S_{snr2} proportional to a second operating parameter of the motor 9,

- causing the endodontic instrument 7 to perform a sequence of movements M1, M2, M3, M4 by acting on the electric motor 9, preferably by means of a signal S_drv generated by a driver 4.

5 The sequence of movements M1, M2, M3, M4 includes:

- a start 32; 34 with a continuous forward movement M1 in which the motor 9 is driven in rotation with a first supplied power PS1, a first rotational speed RS1 and a first direction of rotation RD1;
- 10 - when a first threshold limit L1 is surpassed 38, the start 40 of a first alternating movement M2 in which the motor 9 is driven in rotation with a second supplied power value PS2, a second rotational speed RS2, a first clockwise angle of rotation CWA2, a first anti-clockwise angle of rotation
15 CCWA2 and a second pause RP2 between the first clockwise angle of rotation CWA2 and said first anti-clockwise angle of rotation CCWA2;
- when a second threshold limit L2 is surpassed 44, the start 48 of a second alternating movement M3 in which the motor 9
20 is driven in rotation with a third supplied power value PS3, a third rotational speed RS3, a third clockwise angle of rotation CWA3, a third anti-clockwise angle of rotation CCWA3 and a third pause RP3 between the third clockwise angle of rotation CWA3 and the third anti-clockwise angle
25 of rotation CCWA3.

The first threshold limit L1 for switching from the continuous forward movement M1 to the first alternating forward movement M2 is given by at least one of the following conditions (phase 38 in Figure 3):

- a) the time t_1 elapsed between the sending of the control signal S_{drv} and the receipt of the incoming feedback signal S_{snr1} from the first sensor 8 exceeds a predetermined value MD , or
- 5 b) the power drawn by the electric motor 9 exceeds a predetermined maximum drive power consumption value $MPC1$ by the motor for a time t_2 greater than the maximum time MDi the energy drawn by the electric motor 9 is above $MPC1$. If the two conditions in (a) and (b) are not satisfied, the
- 10 continuous forward movement $M1$ is maintained (phase 36 in Figure 3).

The second threshold limit $L2$ for switching from the first alternating forward movement $M1$ to the second alternating forward movement $M3$ is given by at least one of the following

15 conditions (phase 44 in Figure 3):

- a) the time t_1 elapsed between the sending of the control signal S_{drv} and the receipt of the incoming feedback signal S_{snr1} from the first sensor 8 exceeds a predetermined value MD , or
- 20 b) the power drawn by the electric motor 9 exceeds a predetermined maximum drive power consumption $MPC2$ by the motor for a time t_3 greater than the maximum time $MD2$ the energy drawn by the electric motor 9 is above $MPC2$.

If the two conditions in (a) and (b) are not satisfied, the

25 method skips to phase 46 in Figure 3, in which if, during the first alternating movement $M2$, the power drawn by the electric motor 9 is less than the minimum drive power consumption $mPC2$ by the electric motor 9 for a time t_3 greater than the energy draw time $mD2$, the processing unit 3 causes the endodontic instrument

7 to perform the continuous forward movement M1. Otherwise, the movement M2 is maintained (phase 42).

Figure 3 shows an embodiment of an endodontic system 20 including the device 1 in Figure 1. In particular, the system 20 includes a console 22 coupled operationally to the handle 21. In one embodiment, the handle 21 includes an electric motor 9, optionally a reduction gear 10, and a handpiece 27, the head of which can be coupled to the endodontic instrument 7. As illustrated previously, the system 20 is designed to rotate the instrument 7 clockwise or anti-clockwise. Although clockwise rotation has been described herein as the direction of forward movement of the instrument and anti-clockwise rotation has been described as the opposite direction, this description is provided by way of non-limiting example and the embodiments of the present invention are not limited to a specific relationship between the direction of forward movement or reverse movement and clockwise or anti-clockwise rotation. In the embodiment shown in Figure 3, the console 22 can include a display 23 and a plurality of pushbuttons 25, for example for turning the system on and off or for configuring the type of endodontic instrument being used to treat the patient. The system 20 can preferably include a pedal 24 that can be actuated by the doctor to stop or restart the movement M_i of the endodontic instrument.

Figure 4 shows an embodiment of the mechanisms operating during reverse movement M4. The parameters of reverse movement M4 are set, when the maximum threshold limit in M3 is surpassed (R). At the entry into M4, a counter is increased from n_R to n_R+1 . While the n_R value is still below a predefined reference value n_I , reverse movement M4 is maintained for the duration of a certain rotation angle α_4 . The predefined reference value n_R is preferably between 5 and 15 and most preferably 10. After completion of the rotation angle α_4 the device switches back to

normal forward movement M1. As soon as the counted nR value exceeds the predefined reference value nI, a warning sound is activated. The reverse movement M4 is maintained for the duration of a certain rotation angle α_4 , until the device switches back to normal forward movement M1. The reverse movement M4 may be prolonged.

Figure 5 shows another embodiment of the mechanisms operating during reverse movement M4. The parameters of reverse movement M4 are set when the maximum threshold limit in M3 is surpassed (R). At the entry into M4 a counter is increased from nR to nR+1. While the nR value is still below a predefined reference value nI, reverse movement M4 is maintained for the duration of a certain rotation angle α_4 , as has been described with regard to Fig. 4. As soon as the counted nR value exceeds the predefined reference value nI, however, another evaluation is run. The counted value nR is compared to another reference value nS, higher than nI. While nR is still below reference value nS, a warning sound is activated and the reverse movement M4 is maintained for the duration of a certain rotation angle α_4 , until the device switches back to normal forward movement M1, as has been described with regard to Fig. 4. However, when the Sn value is surpassed, the device emits a prolonged warning sound and permanently performs reverse movement 4. This loop aspect is provided in order to invite the user to replace the file, which has undergone considerable strain for many times. Preferably, the nS value is chosen between 50 and 90. Most preferred is a value of 70.

CLAIMS

1. Device for controlling an electric motor (9) for moving a tool, in particular for moving an endodontic instrument, said device being configured to, when used as intended, cause the tool to perform a sequence of movements (M1, M2) as a function of the signals received from a sensor, the sequence of movements (M1, M2) comprising:
- an initial movement (M1) being a continuous forward rotation in which the motor (9) is driven in a normal direction of rotation, causing a high torque intensity on the tool, and maintaining such movement until a first maximum threshold limit (LM1) is surpassed; wherein
 - when a first maximum threshold limit (LM1) is surpassed, the device is configured to switch to a first alternating movement (M2) in which the motor (9) is driven in an alternating rotation, causing a lower torque intensity on the tool than initial movement (M1), and maintaining such movement until a first minimum threshold (Lm1) is fallen below; wherein
 - when a first minimum threshold (Lm1) is fallen below, the device is configured to switch back to initial movement (M1) and to further observe the conditions for maintaining initial movement (M1) or switching to first alternating movement (M2).
2. A device according to claim 1, wherein the device is configured to, when used as intended, cause the tool to perform an second alternating movement (M3) in which the motor is driven in an alternating rotation, causing a lower

torque intensity on the tool than the first alternating movement (M2), and

- wherein the switch from the first alternating movement (M2) to the second alternating movement (M3) is triggered when during performance of first alternating movement (M2) a second maximum threshold (LM2) is surpassed; and
 - wherein, in the second alternating movement (M3) the device is configured to switch back to one of the previous movements (M1 or M2) when a second minimum threshold (Lm2) or third minimum threshold (Lm3) is fallen below, in particular, the device switches back to the initial movement (M1) when a third minimum threshold (Lm3) is fallen below, and the device switches back to first alternating movement (M2), when a second minimum threshold (Lm2) is fallen below; and
 - wherein, when performing the previous movements (M1, M2), the conditions for maintaining one of the previous movements (M1, M2) or for switching to a neighboring movement are observed.
3. A device according to claim 1 or 2, wherein the device is configured to, when used as intended, cause the tool to perform a conclusive movement (M4) in which the motor is driven in a continuous reverse rotation, causing a low torque intensity on the tool, wherein the switch from the second alternating movement (M3) to conclusive movement (M4) is triggered when during performance of the second alternating movement (M3) a third maximum threshold (LM3) is surpassed.

4. A device according to claim 3, wherein the device is configured such that, in conclusive movement M4, after completion of a predefined angle α_4 of rotation ($\alpha_{\text{effective}} > \alpha_4$), the device is configured to automatically switch to initial movement (M1) and to further observe the conditions for maintaining initial movement (M1) or switching to first alternating movement M2.
- 5
5. Device for controlling an electric motor (9) for moving a tool, in particular for moving an endodontic instrument, in particular a device according to any one of claims 1 to 4, said device comprising:
- 10
- a first sensor (8) that is designed to receive a signal (S_mtr) from said electric motor (9) and to generate a signal (S_snr1) indicating first characteristic operating parameters (RS; RD; RP; PS) of the motor (9);
 - 15
 - a control unit (2) that is in data communication with said motor (9) and said first sensor (8), the control unit (2) comprising:
 - 20
 - a drive unit (4) that is designed to power the motor (9) by means of a power supply voltage (S_drv);
 - 25
 - a second sensor (6) that is designed to generate a feedback signal (S_snr2) that is proportional to a second operating parameter of the motor (9), said second sensor (6) being in data communication with the drive unit (4);

- 5 - a processing unit (3) in data communication with
said drive unit (4), said first sensor (8) and
said second sensor (6), said processing unit (3)
being designed to cause the endodontic instrument
5 (7) to perform a sequence of forward movements
(M1, M2) by acting on said electric motor (9) as
a function of the first signal (S_snr1) received
from the first sensor (8) and the second signal
(S_snr2) received from the second sensor (6), the
10 sequence of movements (M1, M2) comprising:
- a start with a continuous forward movement
(M1) in which the motor (9) is driven in
rotation with a first supplied power (PS1),
a first rotational speed (RS1) and a first
15 direction of rotation (RD1);
 - when a first threshold limit (LM1) is
surpassed, the start of a first alternating
movement (M2) in which the motor (9) is
driven in rotation with a second supplied
20 power value (PS2), a second rotational speed
(RS2), a first clockwise angle of rotation
(CWA2), a first anti-clockwise angle of
rotation (CCWA2) and a second pause (RP2)
between said first clockwise angle of
25 rotation (CWA2) and said first anti-
clockwise angle of rotation (CCWA2)
6. A device according to claim 5, wherein said processing unit
(3) is designed to cause the endodontic instrument (7) to
perform a sequence of forward movements (M1, M2, M3),
30 wherein, when a second threshold limit (LM2) is surpassed,
a second alternating movement (M3) is started in which the

motor (9) is driven in rotation with a third supplied power value (PS3), a third rotational speed (RS3), a third clockwise angle of rotation (CWA3), a third anti-clockwise angle of rotation (CCWA3) and a third pause (RP3) between said third clockwise angle of rotation (CWA3) and said third anti-clockwise angle of rotation (CCWA3).

7. Device according to any of Claims 2 to 6 in which, when the third threshold limit (LM3) is surpassed in movement M3, a fourth reverse movement M4 starts, in which the motor (9) is driven to withdraw the endodontic instrument (7) from the canal.
8. A device according to any of claims 3 to 7 wherein the movement M4, is a continuous reverse rotation in which the motor (9) is driven with a fourth supplied power (PS4), a fourth rotational speed (RS4) and a fourth direction of rotation (RD4).
9. Device according to any of Claims 2 to 8, in which the first characteristic operating parameters of the motor (9) relating to the forward movement (M1, M2, M3) are selected such as to satisfy one or more of the following rules:
 - a) if the first direction of rotation (RD1) is clockwise, then $CWA2 > CCWA2$;
 - b) if the first direction of rotation (RD1) is anti-clockwise, then $CWA2 < CCWA2$;
 - c) if the first direction of rotation (RD1) is clockwise, then $CWA3 > CCWA3$;

d) if the first direction of rotation (RD1) is anti-clockwise, then $CWA3 < CCWA3$;

e) $RS1 > RS2 > RS3$,

e'') $RS1 < RS2 > RS3$;

5 f) $|CWA2-CCWA2| > |CWA3-CCWA3|$;

g) $PS1 < PS2 \leq PS3$.

10. Device according to any of Claims 2 to 8, in which the first characteristic operating parameters of the motor (9) relating to the forward movement (M1, M2, M3) are selected
10 such as to satisfy one or more of the following rules:

a) if the first direction of rotation (RD1) is clockwise, then $CWA2 > CCWA2$;

b) if the first direction of rotation (RD1) is anti-clockwise, then $CWA2 < CCWA2$;

15 c) if the first direction of rotation (RD1) is clockwise, then $CWA3 > CCWA3$;

d) if the first direction of rotation (RD1) is anti-clockwise, then $CWA3 < CCWA3$;

e') $RS1 < RS2 < RS3$;

20 f') $|CWA2-CCWA2| < |CWA3-CCWA3|$;

g) $PS1 < PS2 \leq PS3$.

11. Device according to any one of claims 1 to 10, in which said second sensor (6) is a current sensor designed to generate a feedback signal (S_snr2) proportional to the current drawn by the motor (9) and to send said signal to the processing unit (3).
- 5
12. Device according to any one of Claims 1 to 10, in which said second sensor (6) is a force sensor designed to generate a feedback signal (S_snr2) proportional to the force absorbed by the motor (9) and to send said signal to the processing unit (3).
- 10
13. Device according to any one of claims 1 to 12, in which the reference values (RSi; RDi; CWAi; CCWAI; RPi) of the first characteristic parameters (RSX; RDX; CWAX; CCWAX; RPX) of each movement (Mi) of the sequence of forward movements (M1, M2, M3) are pre-set in a memory module (11) in data communication with said processing unit (3).
- 15
14. Device according to any one of claims 1 to 13, in which the reference values (MDi; MPCi; mPCi; mDi) of each threshold limit (Li) include one or more of the following values:
- 20
- a) maximum drive power consumption (MPCi) by the electric motor during the forward movement (Mi);
 - b) energy draw time (MDi) by the electric motor (9) above the maximum drive power consumption (MPCi);
 - c) minimum drive power consumption (mPCi) by the electric motor in the forward movement (Mi);
 - d) energy draw time (mDi) by the electric motor (9) below the minimum drive power consumption (mPCi).
- 25

15. Device according to one or more of the preceding claims, in which the first threshold limit (LM1) for switching from the first continuous forward movement (M1) to the first alternating forward movement (M2) is given by at least one of the following conditions:
- 5
- a) the time (t1) elapsed between the sending of the control signal (S_drv) and the receipt of the incoming feedback signal (S_snrl) from the first sensor (8) exceeds a predetermined value (MD); or
- 10 b) the power drawn by the electric motor (9) exceeds a predetermined maximum drive power consumption value (MPC1) by the motor for a time (t2) greater than the maximum time (MDi) the energy drawn by the electric motor (9) is above (MPC1).
- 15 16. Device according to one or more of the preceding claims, in which if, during the movement (M2), the power drawn by the electric motor (9) is less than the minimum drive power consumption (mPC2) by the electric motor (9) for a time (t3) greater than the energy draw time (mD2), the
- 20 processing unit (3) causes the endodontic instrument (7) to perform the continuous forward movement (M1).
17. Device according to one or more of the preceding claims in which, if one of the following conditions occurs during the second alternating forward movement (M3):
- 25 - the power drawn by the electric motor (9) is less than the minimum drive power consumption (mPC31) by the electric motor (9) for a time (t) greater than the energy draw time (mD3), the processing unit (3) causes

the endodontic instrument (7) to perform the continuous forward movement (M1); or if

- the power drawn by the electric motor (9) is less than the minimum drive power consumption (mPC32) by the electric motor (9) for a time (t) greater than the energy draw time (mD3), the processing unit (3) causes the endodontic instrument (7) to perform the first reciprocating forward movement (M2).

- 5
- 10
- 15
- 20
- 25
18. Device according to one or more of the preceding claims, configured such that during the alternating Movements M2 and M3, the characteristic parameters of the motor are determined only within the phase of normal rotation, preferably during an inner angle of rotation α , positioned between an initial angle of rotation α_i and a final angle of rotation α_f .
 19. Device according to one or more of the preceding claims, wherein the device is configured to automatically activate a warning sound when a predefined number nI of starts of conclusive movement M4, preferably a predefined number between 5 and 15, is surpassed.
 20. Device according to one or more of the preceding claims, wherein the device configured to automatically activate a prolonged warning sound and to permanently maintain conclusive movement M4, when a predefined number nS of starts of conclusive movement M4, preferably a predefined number between 50 and 90, is surpassed.
 21. Electric motor (9) designed to rotate an endodontic instrument (7), including a control device according to one or more of Claims 1 to 20.

22. Method for controlling an electric motor (9) to move a tool, in particular an endodontic instrument (7), the control method including a sequence of movements (M1, M2) as a function of the signals received from at least one sensor, the sequence of movements (M1, M2) comprising:

- an initial movement (M1) being a continuous forward rotation in which the motor (9) is driven in a normal direction of rotation, causing a high torque intensity on the tool, and maintaining such movement until a first maximum threshold limit (LM1) is surpassed; wherein
- when a first maximum threshold limit (LM1) is surpassed, the sequence switches to a first alternating movement (M2) in which the motor (9) is driven in an alternating rotation, causing a lower torque intensity on the tool than initial movement (M1), and maintaining such movement until a first minimum threshold (Lm1) is fallen below; wherein
- when a first minimum threshold (Lm1) is fallen below, the sequence switches back to initial movement M1, where in (M1) the conditions for maintaining initial movement (M1) or switching to first alternating movement (M2) are further observed.

23. A method according to claim 22, wherein the sequence of movements (M1, M2) includes a second alternating movement (M3) in which the motor is driven in an alternating rotation, causing a lower torque intensity on the tool than the first alternating movement (M2), and

- wherein the switch from the first alternating movement (M2) to the second alternating movement (M3) is

triggered when during performance of first alternating movement (M2) a second maximum threshold (LM2) is surpassed; and

- 5 - wherein, in the second alternating movement (M3) the sequence switches to one of the previous movements (M1 or M2), when a second minimum threshold (Lm2) or third minimum threshold (Lm3) is fallen below, in particular, the sequence switches to the initial movement (M1), when a third minimum threshold (Lm3) is fallen below
10 and the sequence switches to the first alternating movement (M2), when a second minimum threshold (Lm2) is fallen below; and
- wherein, when performing the previous movements (M1, M2), the conditions for maintaining one of the previous
15 movements (M1,M2) or for switching to a previous or subsequent movement are observed.

24. A method according to claim 22 or 23, wherein the method includes a conclusive movement (M4) in which the motor is driven in a continuous reverse rotation, causing a low
20 torque intensity on the tool wherein the switch from the second alternating movement (M3) to conclusive movement (M4) is triggered when during performance of the second alternating movement (M3) a third maximum threshold (LM3) is surpassed.

25 25. Method (30) for controlling an electric motor (9), in particular to move an endodontic instrument (7), preferably a method according to any of claims 22 to 24, the control method including the following phases:

- receiving a signal (S_snr1) from said electric motor (9) indicating first characteristic operating parameters (RS_x; RD_x; RP_x; PS_x) of the motor (9);
- powering the motor (9) with a power supply voltage (S_drv);
- receiving a feedback signal (S_snr2) proportional to a second operating parameter of the motor (9);
- causing the endodontic instrument (7) to perform a sequence of movements (M1, M2, M3, M4) by acting on said electric motor (9), the sequence of movements (M1, M2, M3, M4) including:
 - a start (32; 34) with a continuous forward movement (M1) in which the motor (9) is driven in rotation with a first supplied power (PS1), a first rotational speed (RS1) and a first direction of rotation (RD1);
 - when a first threshold limit (L1) is surpassed (38), the start (40) of a first alternating movement (M2) in which the motor (9) is driven in rotation with a second supplied power value (PS2), a second rotational speed (RS2), a first clockwise angle of rotation (CWA2), a first anti-clockwise angle of rotation (CCWA2) and a second pause (RP2) between said first clockwise angle of rotation (CWA2) and said first anti-clockwise angle of rotation (CCWA2);
 - when a second threshold limit (L2) is surpassed (44), the start (48) of a second alternating

5 movement (M3) in which the motor (9) is driven in rotation with a third supplied power value (PS3), a third rotational speed (RS3), a third clockwise angle of rotation (CWA3), a third anti-clockwise angle of rotation (CCWA3) and a third pause (RP3) between said third clockwise angle of rotation (CWA3) and said third anti-clockwise angle of rotation (CCWA3).

- 10 26. Method for controlling and moving an endodontic instrument according to any one of the preceding claims, characterized in that said method is implemented by an electronic processor.

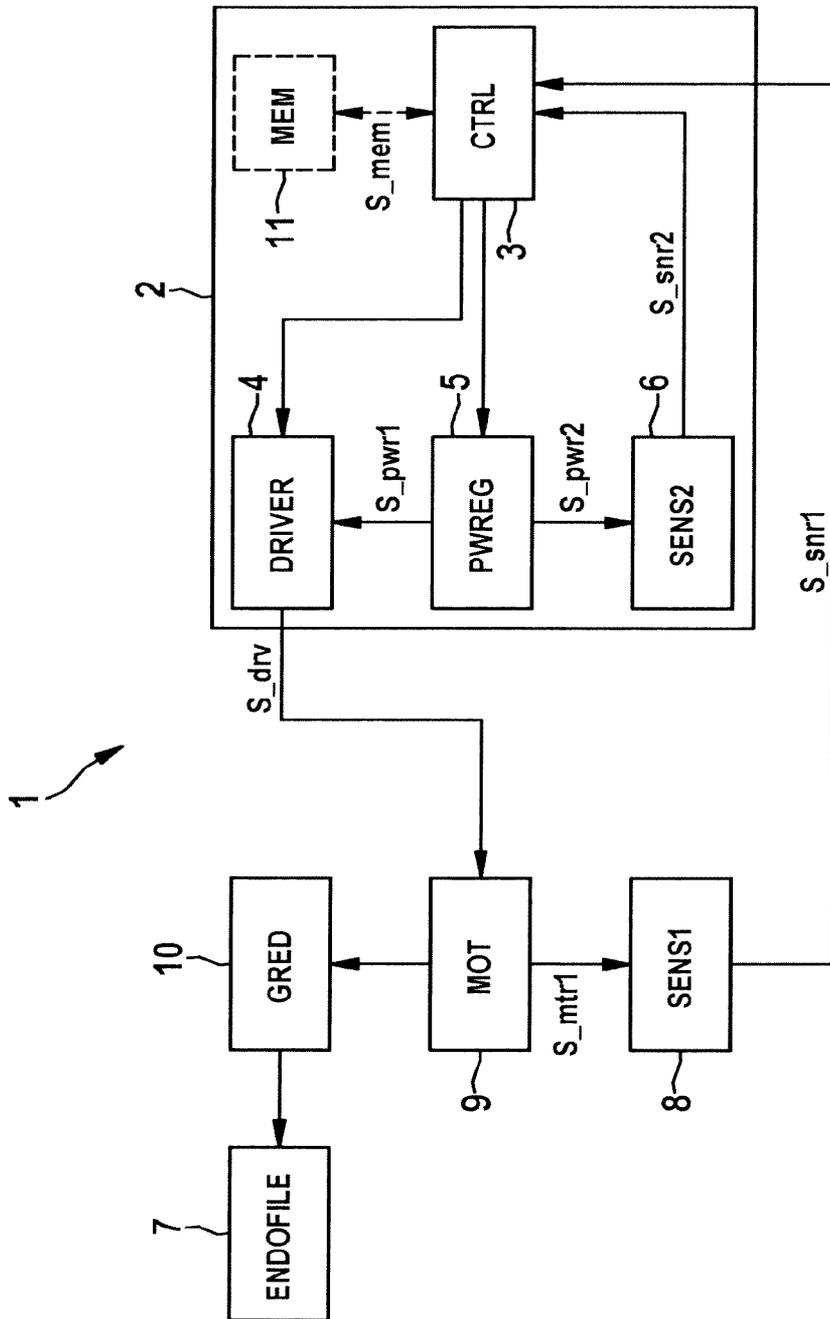


Fig. 1

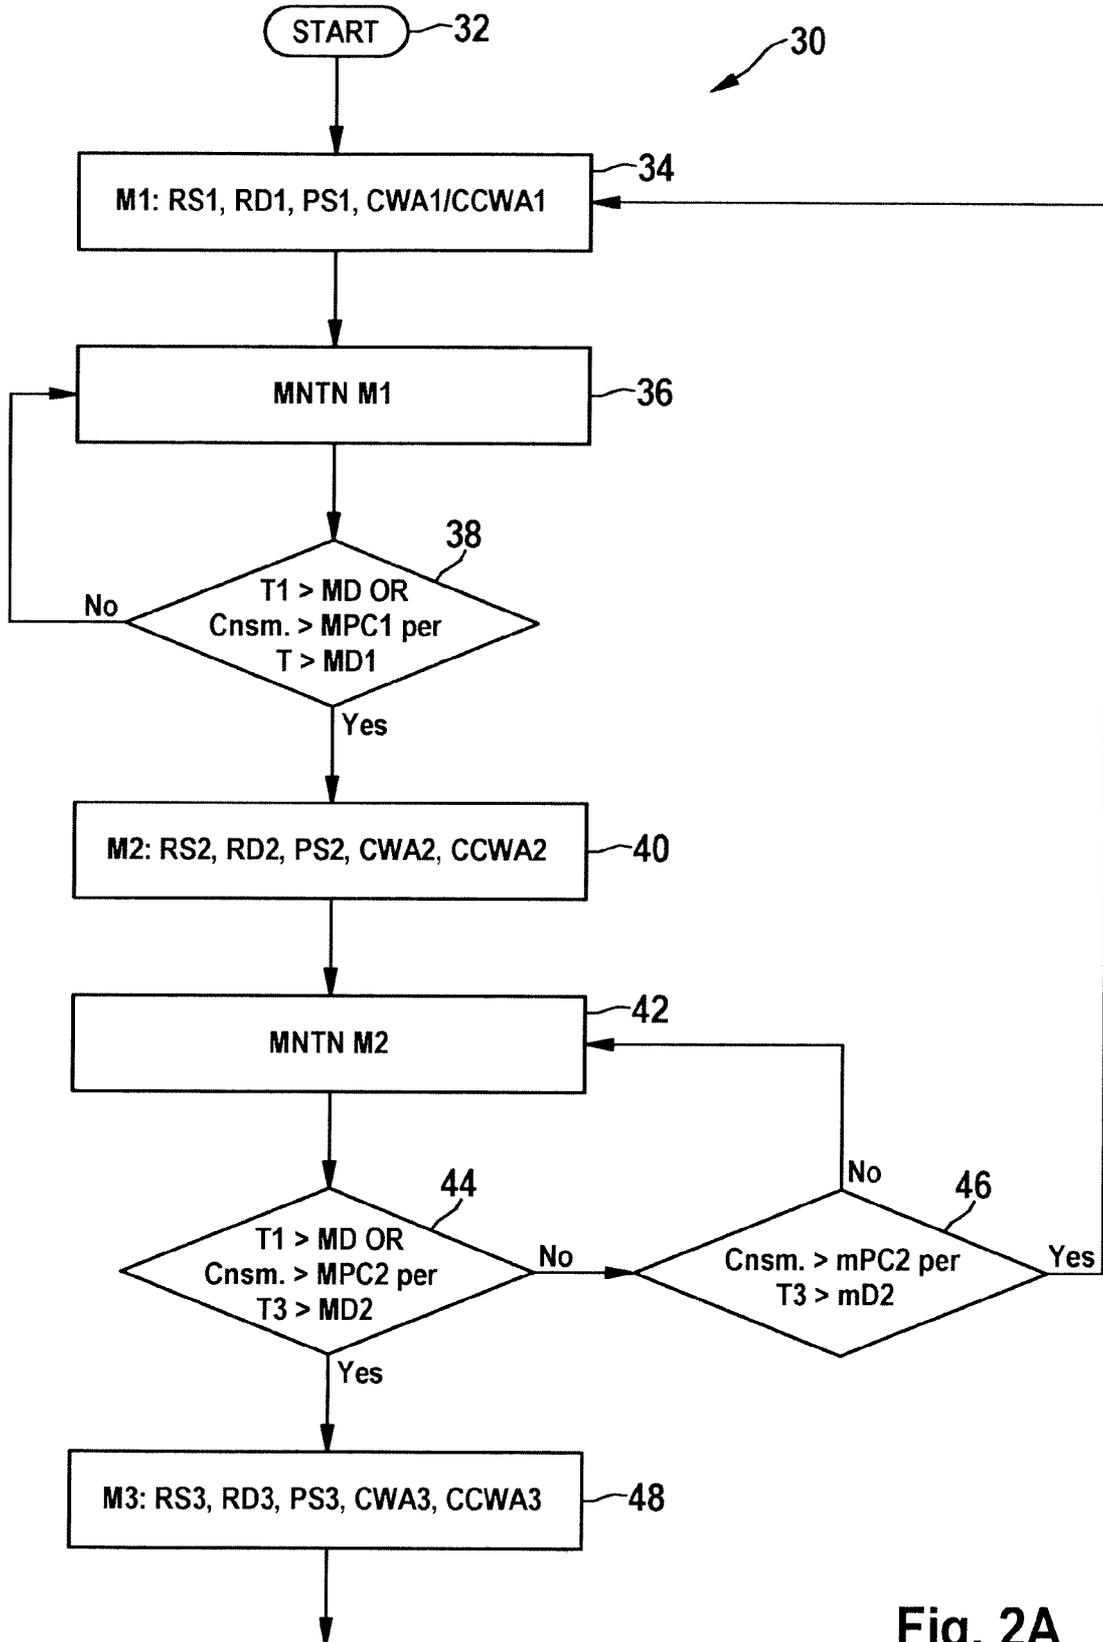


Fig. 2A

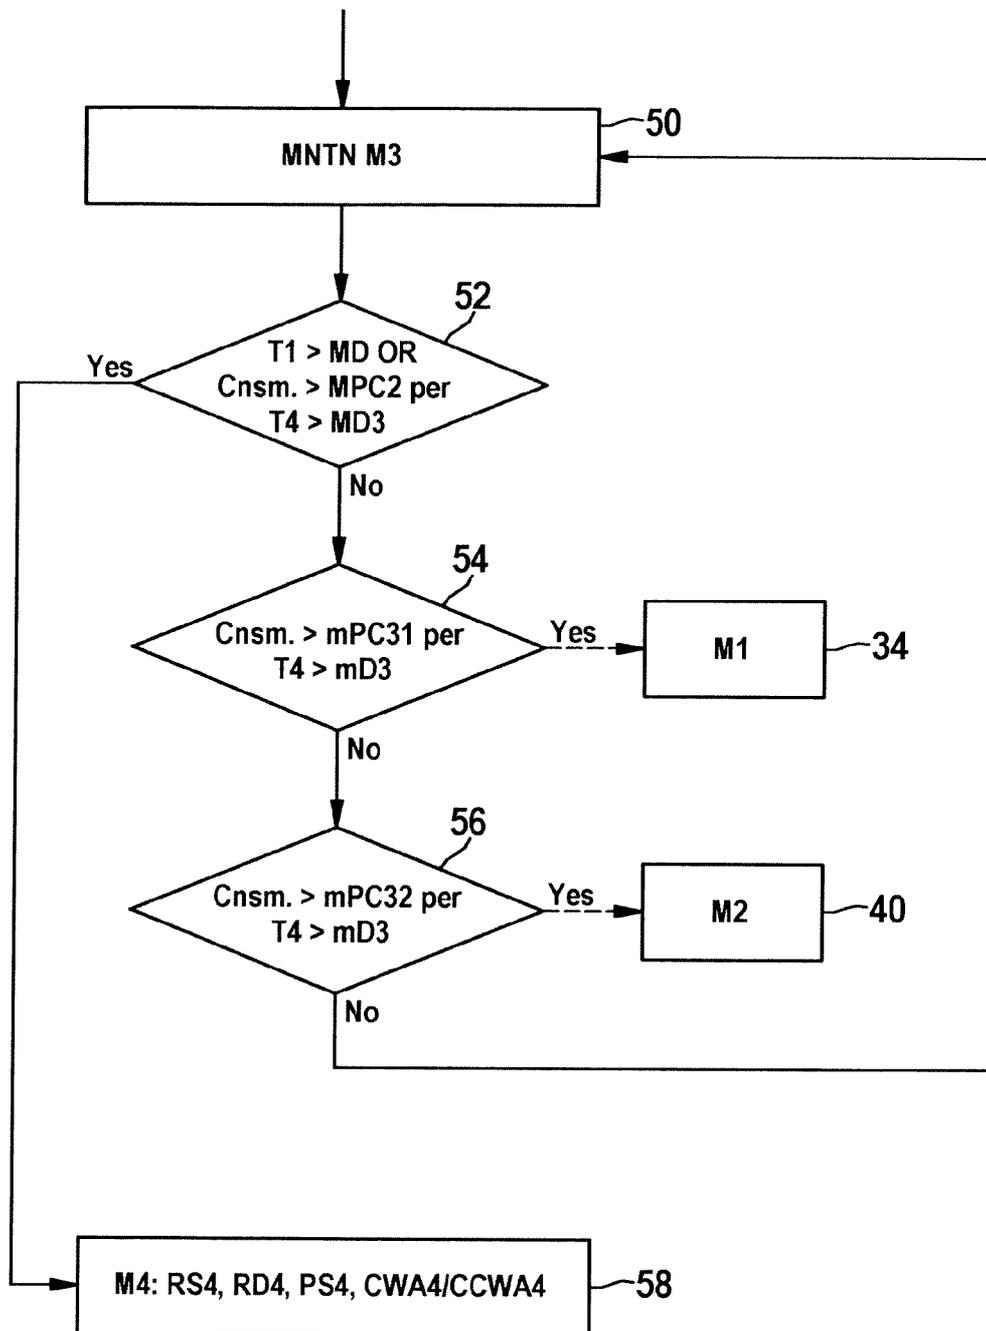


Fig. 2B

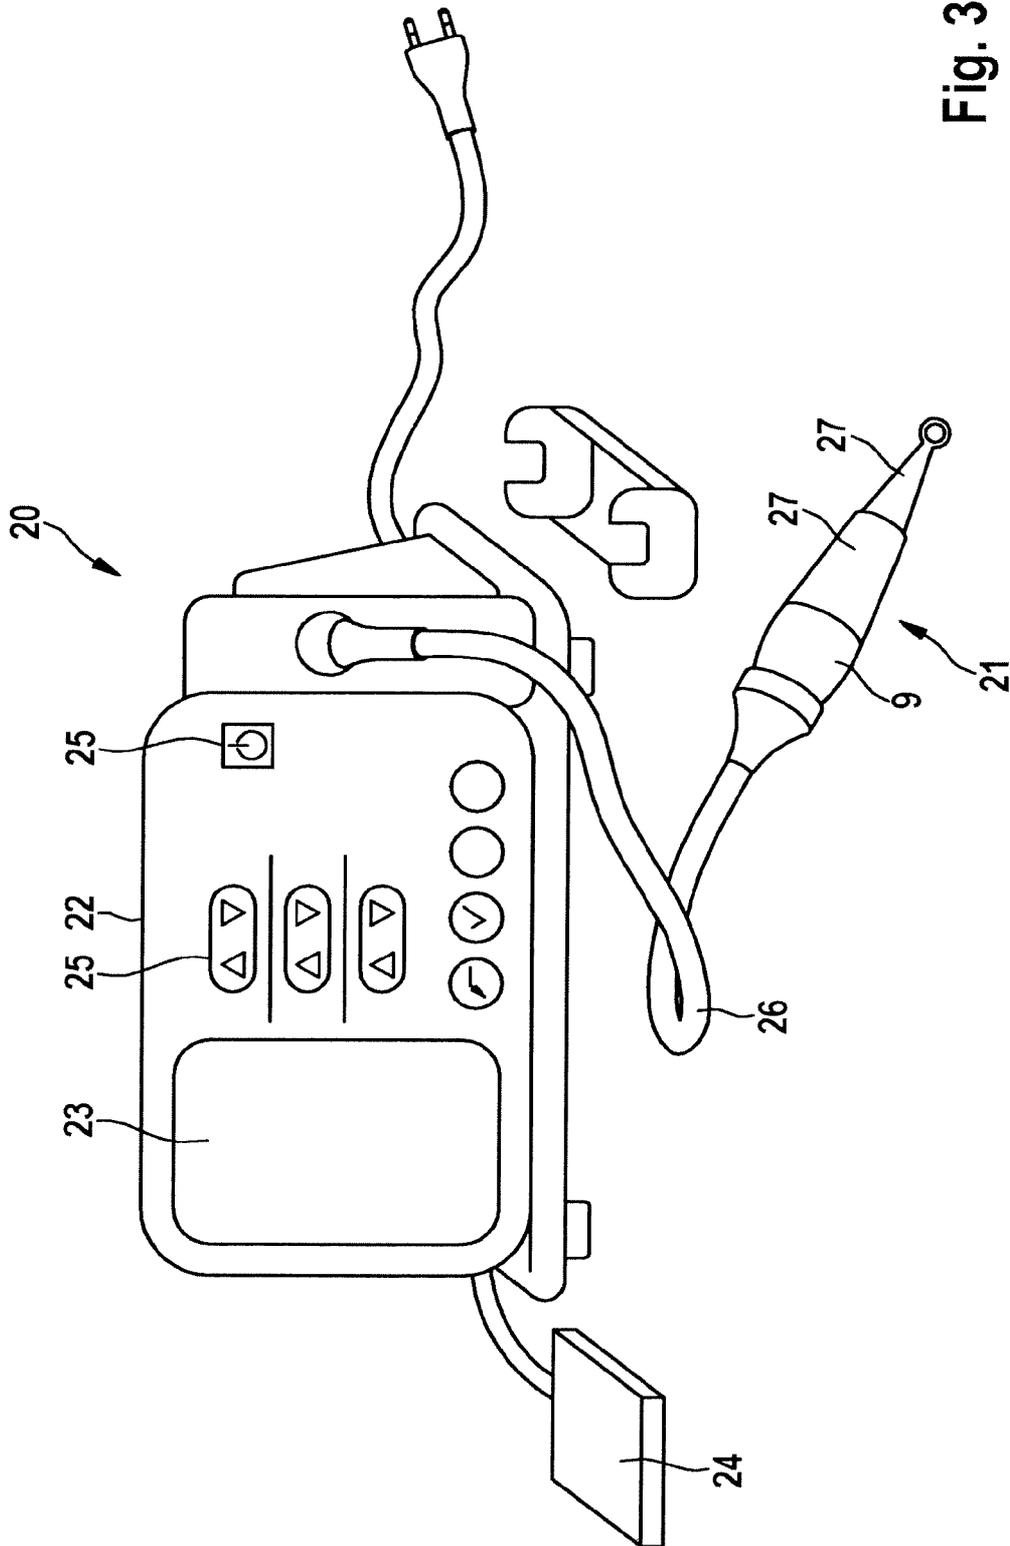


Fig. 3

5 / 6

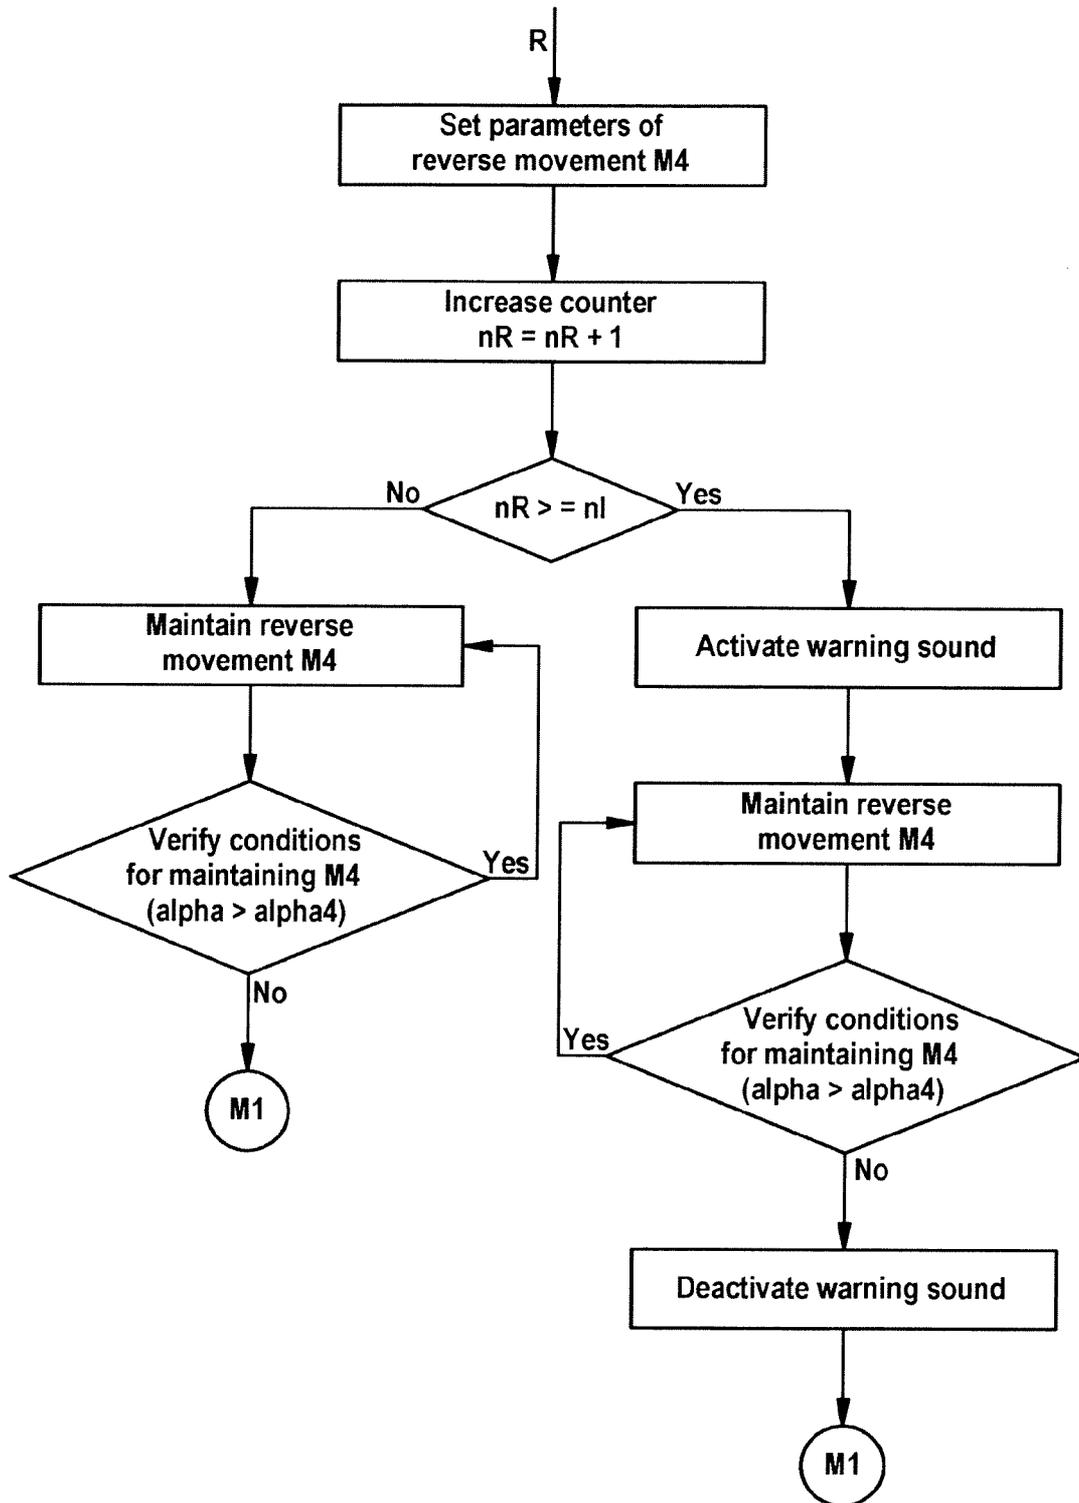


Fig. 4

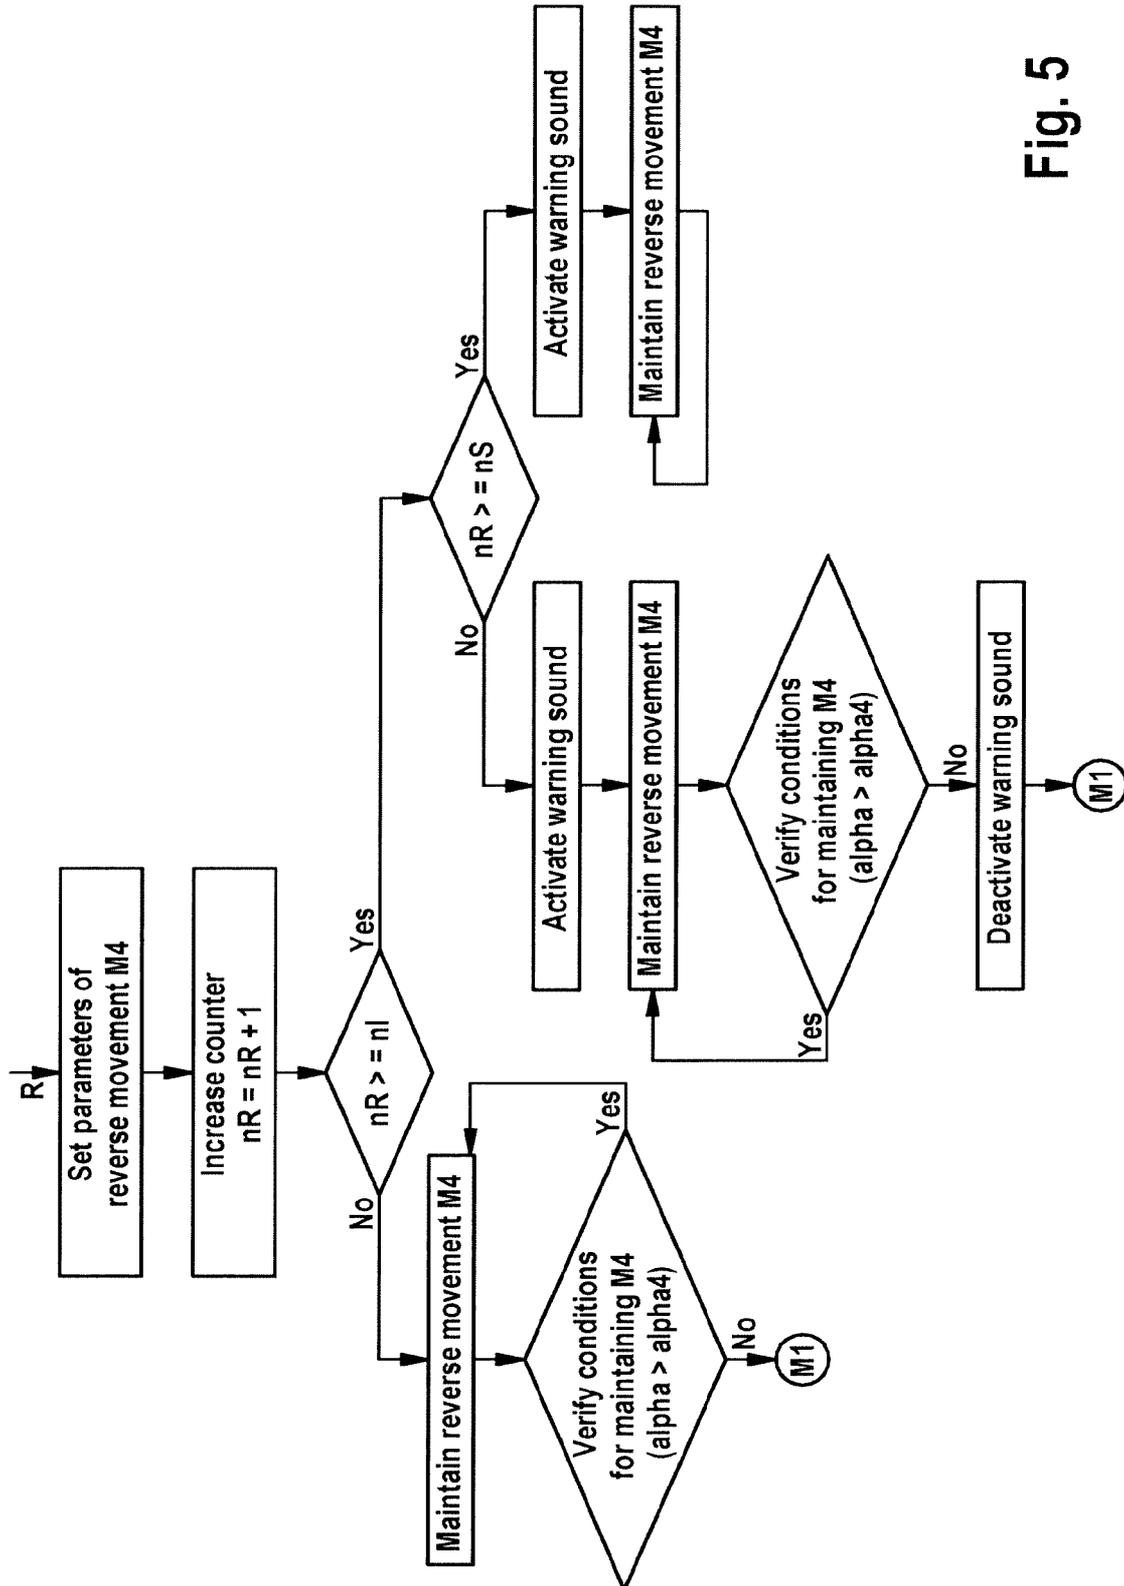


Fig. 5

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2018/057405

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61C1/06 A61C5/40
ADD.
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
Minimum documentation searched (classification system followed by classification symbols)
A61C
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y A	EP 2 431 004 A1 (NAKANISHI INC [JP]) 21 March 2012 (2012-03-21) paragraphs [0012] - [0023], [0032] - [0040], [0046] - [0050], [0053] - [0113]; figures 1,2,4 -----	5-21, 23-26 1-4,22
Y A	US 2013/224677 A1 (YAMASHITA SEIICHIRO [JP] ET AL) 29 August 2013 (2013-08-29) figures 1-3,6-12 -----	5-21, 23-26 1-4,22
Y A	WO 2010/109464 A2 (FORUM ENGINEERING TECHNOLOGIES [IL]; RAMOS CARLOS ALBERTO [BR]; YAKOBY) 30 September 2010 (2010-09-30) pages 1,3,7-10; figures 1,5 -----	5-21, 23-26 1-4,22
	-/--	

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search 26 April 2018	Date of mailing of the international search report 07/05/2018
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Fraïssé, Stéphane

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2018/057405

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2002/064756 A1 (PAGNINI MAURO [IT] ET AL) 30 May 2002 (2002-05-30) the whole document	1-26
A	----- EP 2 851 035 A1 (MORITA MFG [JP]) 25 March 2015 (2015-03-25) cited in the application the whole document	1-26
A	----- DE 10 2007 011725 A1 (SCHLUMBOHM OHG [DE]) 11 September 2008 (2008-09-11) cited in the application the whole document	1-26
A	----- ROANE ET AL: "The 'balanced force' concept for instrumentation of curved canals", JOURNAL OF ENDODONTICS, LIPPINCOTT WILLIAMS & WILKINS, PHILADELPHIA, PA, US, vol. 11, no. 5, 1 May 1985 (1985-05-01), pages 203-211, XP022447657, ISSN: 0099-2399, DOI: 10.1016/S0099-2399(85)80061-3 the whole document	1-26
X	----- WO 00/15138 A1 (NOBEL BIOCARE AB [SE]; DAWOOD ANDREW [GB]; PETERSSON ANDERS [SE]) 23 March 2000 (2000-03-23)	1-4,22
Y	the whole document	5-21, 23-26
X	----- EP 2 716 254 A1 (NAKANISHI INC [JP]) 9 April 2014 (2014-04-09)	1-4,22
Y	the whole document	5-21, 23-26

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2018/057405

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
EP 2431004	A1	21-03-2012	CN 102427774 A	25-04-2012
			EP 2431004 A1	21-03-2012
			JP 4916037 B2	11-04-2012
			JP 2012011068 A	19-01-2012
			KR 20120031157 A	30-03-2012
			US 2013099710 A1	25-04-2013
			WO 2012001869 A1	05-01-2012
US 2013224677	A1	29-08-2013	DE 102013002509 A1	29-08-2013
			JP 5802149 B2	28-10-2015
			JP 2013172840 A	05-09-2013
			US 2013224677 A1	29-08-2013
WO 2010109464	A2	30-09-2010	EP 2410936 A2	01-02-2012
			US 2012122055 A1	17-05-2012
			WO 2010109464 A2	30-09-2010
US 2002064756	A1	30-05-2002	IT FI20000241 A1	30-05-2002
			US 2002064756 A1	30-05-2002
EP 2851035	A1	25-03-2015	EP 2851035 A1	25-03-2015
			JP 5870154 B2	24-02-2016
			JP 2015083116 A	30-04-2015
			US 2015086937 A1	26-03-2015
DE 102007011725	A1	11-09-2008	NONE	
WO 0015138	A1	23-03-2000	AU 6376199 A	03-04-2000
			CA 2339660 A1	23-03-2000
			EP 1113762 A1	11-07-2001
			JP 2002524195 A	06-08-2002
			US 6547565 B1	15-04-2003
			WO 0015138 A1	23-03-2000
EP 2716254	A1	09-04-2014	CN 103379875 A	30-10-2013
			EP 2716254 A1	09-04-2014
			JP 5258076 B2	07-08-2013
			JP WO2012164875 A1	23-02-2015
			KR 20130128452 A	26-11-2013
			TW 201306807 A	16-02-2013
			US 2014134565 A1	15-05-2014
			WO 2012164875 A1	06-12-2012