



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : G01N	A2	(11) International Publication Number: WO 00/00811 (43) International Publication Date: 6 January 2000 (06.01.00)
(21) International Application Number: PCT/US99/14683 (22) International Filing Date: 29 June 1999 (29.06.99) (30) Priority Data: 60/091,090 29 June 1998 (29.06.98) US 60/138,643 10 June 1999 (10.06.99) US (71) Applicant: SAN DIEGO STATE UNIVERSITY FOUNDATION [US/US]; 5178 College Avenue, San Diego, CA 92182-0419 (US). (72) Inventors: SHARTS, Clay, Marcus (deceased).GORELIK, Vladimir Semenovich; Moscow (RU). (74) Agent: LAND, John; Fish & Richardson P.C., Suite 1400, 4225 Executive Square, La Jolla, CA 92037 (US).		(81) Designated States: JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>Without international search report and to be republished upon receipt of that report.</i>
(54) Title: METHOD AND APPARATUS FOR DETERMINATION OF CARBON-HALOGEN COMPOUNDS AND APPLICATIONS THEREOF (57) Abstract <p>A method and apparatus for determination of fluoroorganic compounds in liquid, gaseous, or crystalline or amorphous solids is based on the detection of carbon-halogen bonds by laser Raman spectroscopy. The method and apparatus provide a general method for detecting and determination of haloorganic compounds. The method and apparatus are applicable in the pharmaceutical industry, in fluorinated drug research and manufacturing; in the medical and clinical studies of the effects of fluoroorganic compounds; in the environmental and agricultural studies and screening, in the analysis of water, soils and air contaminated with fluoroorganic compounds.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

METHOD AND APPARATUS FOR DETERMINATION OF CARBON-HALOGEN COMPOUNDS AND APPLICATIONS THEREOF

CROSS REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of United States Provisional Patent Application No. 60/091,090, filed June 29, 1998 and United States Provisional Patent Application No. 60/138,643, filed June 10, 1999.

5

TECHNICAL FIELD

This invention relates generally to measuring and testing by dispersed light spectroscopy with Raman type light scattering, and more particularly to Raman spectroscopy for the determination of carbon-halogen and fluoroorganic compounds.

10

BACKGROUND

Qualitative and quantitative analysis of fluoroorganic compounds is an important practical task. Fluoroorganic compounds are widely used in the pharmaceutical industry. About one-third of all newly patented drugs contain carbon-fluorine (C-F) bonds. Examples of fluorine-containing drugs are the anticancer drug Fluoracil ($C_4H_3FN_2O_2$, 5-fluorouracil), antidepressant drug Prozac® ($C_{17}H_{18}F_3NO$, fluoxetine) and painkiller Dalmane ($C_{21}H_{23}ClFN_3O$, flurazepam). Perflubron ($C_8F_{17}Br$, bromoperfluorooctane) is an oxygen-carrier in a formulation now undergoing clinical trials as a blood substitute. Many agricultural chemicals and pesticides also contain carbon-fluorine bonds.

15

20

Chemical analysis for drugs can be done by isolating the drug and then measuring concentrations of compounds. This approach can be expensive. Alternatively, known chemical compounds can be labeled with radioactive elements to form tracers. The radioactive compounds and their metabolites can be followed in the body or tissues by observing emitted radioactivity. However, making and disposing of radiolabeled compounds is also expensive. These expenses can be found in many drug development programs.

25

Accordingly, the inventors have determined that it would be useful to accurately and inexpensively identify fluoroorganic compounds. The present invention provides a method and apparatus for achieving this object.

SUMMARY OF THE INVENTION

The invention is directed to an apparatus and method for detecting the presence of compounds having carbon-halogen bonds using Raman spectroscopy. The method detects any carbon-halogen bond, and is particularly useful in detecting carbon-fluorine bonds.

In one aspect, the method uses pulsed laser Raman spectroscopy to detect carbon-halogen bonds, using an effect of inelastic scattering of light. A sample is irradiated from a noncontinuous periodic pulse light source, such as a metal-vapor laser. Raman scattered light emitted from the sample is then detected to determine if a characteristic Raman scattered light spectrum for a compound having a carbon-halogen is present in the sample.

In another aspect, the apparatus for Raman spectroscopy includes a noncontinuous periodic pulse metal vapor laser and a monochromator for visible and ultraviolet light. The apparatus also includes a detector for detecting the emitted Raman scattered light and a pulse recording system to eliminate primary fluorescence associated with the sample.

In yet another aspect, the invention is directed to a method for detecting a fluoroorganic compound that includes exposing a sample to an excitation light source and measuring a frequency of an acoustic mode of the compound. The method also includes measuring a frequency of an optical mode of the compound and detecting a shift in the optical and acoustic mode frequencies. The molecular length of the compound is approximated as a function of the shift in frequencies to determine the presence of the fluoroorganic compound.

The details of one or more embodiments of the invention are set forth in the accompanying drawings and the description below. Other features, objects, and advantages of the invention will be apparent from the description and drawings, and from the claims.

DESCRIPTION OF DRAWINGS

FIG. 1 is a schematic drawing of a Raman spectrometer in accordance with a preferred embodiment.

FIG. 2 is a Raman spectrum of $C_8H_{17}Br$ (bromoperfluorooctane) and C_8H_{18} using the spectrometer of FIG. 1.

FIG. 3 is a Raman spectrum of $C_9F_{19}COOH$ ($C_{10}HF_{19}O_2$; bromoperfluorodecanoic acid). C_9H_{20} (nonane, a hydrocarbon) using the spectrometer of FIG. 1.

FIG. 4 is a Raman spectrum of $C_6H_3(CF_3)_3$ [1,3,5-tris(trisfluoromethyl)benzene] and C_6H_6 (benzene) using the spectrometer of FIG. 1.

FIG. 5 is a Raman spectrum of a commercial preparation of fluoxetine hydrochloride using the spectrometer of FIG. 1.

FIG. 6 is a schematic drawing of a resonance Raman spectrometer in accordance with a preferred embodiment.

FIG. 7 is a resonance Raman spectrum of irradiate perfluorodecalin showing a difluoromethylene absorption. The top spectrum is an unprocessed resonance Raman spectrum of perfluorodecalin ($C_{10}F_{18}$). The bottom spectrum is a partially processed resonance Raman spectrum of perfluorodecalin.

FIG. 8 is a resonance Raman spectrum of 1-bromoperfluorooctane using the spectrometer of FIG. 6.

FIG. 9 shows structures of some commercially useful fluoroorganic compounds.

FIG. 10 shows structures of various compounds having Raman spectra.

FIG. 11 illustrates Raman spectra of $C_nF_{2n+1}Br$ for $n=6, 7, 8, 9, 10, 14$ in the region 0-1500 cm^{-1} .

FIG. 12 illustrates the dependency of Raman spectra on the unit length of a molecule in the lower frequency region LAM.

FIG. 13 illustrates the dependency of Raman spectra on the unit length of a molecule in the higher frequency region LOM.

FIG. 14 illustrates experimental Raman frequencies.

FIG. 15 illustrates the Raman spectra of a two-component mixture of $C_nF_{2n+1}Br$ obtained at three concentrations of components at a Raman signal for a CF_2 bond.

FIG. 16 illustrates the Raman spectra of a two-component mixture of $C_nF_{2n+1}Br$ obtained at three different concentrations of the components at a characteristic Raman signal in the lower frequency region LAM band.

Like reference numbers and designations in the various drawings indicate like elements.

DETAILED DESCRIPTION

In general, the invention is directed to a method and an apparatus for determining the presence, in a sample, of compounds having carbon-halogen bonds and, in particular, carbon-fluorine bonds. The method uses pulsed laser Raman spectroscopy to detect carbon-halogen bonds, using an effect of inelastic scattering of light. The apparatus includes a metal-vapor laser source and a pulse recording system, to permit the recording of Raman signals for carbon-halogen bonds.

The invention is based on a principle different from most organic chemistry analyses, *i.e.*, analysis by bond rather than analysis by compound. The method of the invention does not identify a compound; rather the presence of a carbon-halogen bond is determined, using the carbon-halogen bond as a chemical tracer. In particular, the method detects all types of carbon-fluorine bonds.

The method is useful for analysis of fluoroorganic compounds at 10^{-3} - 10^{-6} g/L (ppm-ppb level) for pharmaceutical, biological, medical and biomedical applications, and for environmental analysis of water, soils and air contaminated with such compounds. Full development of resonance Raman technology may lead to detection at better than parts per billion levels. The invention usefully reduces the operational costs for analysis of fluoroorganic compounds (being less expensive than current methods based on extraction and compound isolation, with identification by chromatography or mass spectrometry), and makes such analysis more rapid.

The apparatus of the invention has several advantages for the observation of the Raman spectra of fluoroorganic compound. A periodic pulse vapor-metal laser source, such as copper-vapor or gold-vapor lasers, is used for sample excitation. Metal-vapor lasers are characterized by an ability to produce short and powerful pulses in the visible and ultraviolet region. These lasers are able to produce pulses of light with high peak and average operating power with air cooling.

Analysis for a carbon-fluorine bond rather than for a fluoroorganic compound specifically is possible because organic fluorine compounds with a carbon-fluorine bond are rarely not found in nature. Except for a few rare exceptional compounds found in a few plants or microorganisms (*e.g.*, sodium fluoroacetate and fluorooleic acid, both found in certain plants in Africa), carbon-fluorine bonds generally do not exist in natural products (Key *et al.*, *Environmental Science and Technology* 31: 2445-2454, 1997). Consequently, finding a carbon-fluorine bond in any system means an artificial compound exists in the sample. Additionally, all known biologically produced fluorinated organic molecules contain only one fluorine atom. If a fluorinated compound is found in or found on biologically derived animal or vegetable material, the compound is almost certainly artificial, not natural. If a fluorinated compound is injected or ingested by a vegetable or animal biological material, any fluoroorganic compound found must be the material injected or ingested or be a metabolite of the material injected or ingested. The carbon-fluorine bond is strong and generally cannot be modified biologically. This means that the carbon-fluorine bond can be used as a tracer group because the bond does not alter state when exposed to biological processes.

Unless otherwise defined, all technical and scientific terms used herein have substantially the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. Although many methods and materials similar or equivalent to those described herein can be used in the practice or testing of the present invention, suitable methods and materials are described below.

All publications, patent applications, patents, and other references mentioned herein are incorporated by reference in their entirety. In case of conflict, the present application,

including definitions, will control. In addition, the materials, methods, and examples described herein are illustrative only and not intended to be limiting.

Other features and advantages of the invention will be apparent from the following detailed description, the drawings, and from the claims.

5

Raman Spectroscopy

An authoritative book (Wolverson, in *An Introduction to Laser Spectroscopy*, Andrews & Demidov, Eds., Plenum Press, New York, 1995, pp. 91-114) concisely defines Raman spectroscopy as follows: "Raman spectroscopy is the inelastic scattering of light by a material; the word 'inelastic' implies that energy is transferred between the light quanta and the material, so that the scattered light may have a longer or shorter wavelength than the incident light. The study of light scattered from a particular material is therefore termed Raman spectroscopy and is of interest because, as will be seen, information can be gained about the structure, the composition, and the vibrational or electronic states of the scattered material. Raman spectroscopy is a large field, with many variations on the basic technique and with many new applications being found each year." An older, alternative description of the Raman effect and Raman spectroscopy may be found in other sources, e.g., *Spectroscopy Source Book, Science Reference Series*, McGraw-Hill, New York, 1988, pp. 145-151.

The intensity of normal Raman peaks of the frequency of incident light is described by Skoog & Leary (*Principles of Instrumental Analysis*, 4th edition, Saunders Publishing, Philadelphia, 1992, p. 301) as follows: "The intensity of power of a normal Raman peak depends in a complex way upon the polarizability of the active group, as well as other factors. In the absence of absorption, the power of the Raman emission increases the fourth power of the frequency of the source; however, advantage can seldom be taken of this relationship because of the likelihood that ultraviolet radiation will cause photodecomposition. Raman intensities are usually directly proportional to the concentration of the active species. In this regard, Raman spectroscopy more closely resembles fluorescence than absorption, where the concentration-intensity relationship is logarithmic."

25

The teaching of the quoted authors bears importantly on the use of pulsed metal-vapor lasers. Conventional Raman spectroscopy using a continuous wave Nd:YAG laser does not have sufficient energy in the incident light to cause fluorescence. Because the intensity of the Raman signal is proportional to the fourth power of the frequency of incident light, and therefore inversely proportional to the fourth power of the wavelength of incident light, the signal strength of the inelastically scattered light is about 16 times greater at the wavelength of 510.6 nm (copper-vapor laser) than at the conventionally used wavelength of 1064 nm (Nd:YAG laser). Other lasers operating with higher energy continuous wave light (such as argon at 488.8 and 514.5 nm, krypton at 647.1 nm, and helium-neon at 632.8 nm) cause photodecomposition of samples, as described by Skoog & Leary, above. When any compound in a sample mixture gives primary fluorescence, then observation of Raman spectra of the sample is severely limited. In contrast, by using a pulsed laser at about 10,000 Hertz and a very short pulse width of about 12 nanoseconds, samples do not undergo the photodecomposition discussed by Skoog & Leary, above. Using a pulsed copper-vapor laser permits elimination of inherent fluorescence by using a timing-gate for the detector. The invention thus uses higher energy incident light to give a much stronger signal.

Apparatus

The Pulsed Laser Raman Spectroscopy of the invention is achieved using non-continuous periodic pulse vapor metal laser sources and by using a stroboscopic pulse recording system. Suitable lasers include copper-vapor or gold-vapor lasers. Alternatively, any pulsing light source such as a solid state light source or a light bulb can be used. The apparatus can be a modification of copper-vapor and gold-vapor lasers that have been used to provide energy for two-photon excitation of a compound. (Gorelik *et al.*, *Journal of Molecular Structure* 266: 121-126, 1992; Gorelik & Kozulin, *Quantum Electronics (Russia)* 21: 499-501, 1994; Gorelik & Zhabotinskii, *Quantum Electronics (Russia)* 24: 273-275, 1994). In Gorelik's two-photon excitation studies, exciting light was green (510.5 nm) or yellow (578.2 nm) from the copper-vapor laser or red (627.8 nm) from the gold-vapor laser. The goal of these studies was the production of primary fluorescence in the ultraviolet and

blue ranges of the spectra. The above studies did not contemplate Raman spectroscopy of the carbon-fluorine bond. For Raman spectroscopy, efforts are made to eliminate primary fluorescence and to collect only the inelastically scattered Raman light. For resonance Raman spectroscopy, a frequency doubling crystal is required.

5 Metal-vapor lasers are air cooled or water cooled and consume only about 1-2 kW of electrical power. These lasers may have a coefficient of efficiency of about 1%. The air-cooled copper-vapor laser operates at an average power of about 1-10 watts. This means that metal vapor lasers operate more efficiently and cost less to operate than many other laboratory lasers. Thus, the laser can be combined with other commercial components to
10 produce an inexpensive Raman instrument for obtaining Raman spectra of fluoroorganic compounds. A Raman instrument can be designed for spectral range of about 550-900 cm^{-1} . The instrument can also be designed for a range of about 500-1500 cm^{-1} . In this case, the instrument may be capable of presenting detection in the normal 1000-1400 cm^{-1} vibrational range of the carbon-fluorine bond.

15 FIG. 1 illustrates a Raman instrument 100 that includes a metal-vapor laser. Suitable lasers include a copper-vapor or a gold-vapor laser. The Raman instrument 100 also includes a mirror 102 with dielectric and highly reflective coating to efficiently reflect a generated laser radiation, and a photodiode 103 for collecting a laser radiation. The instrument 100 also includes an electronic unit 104 (*e.g.*, a stroboscopic generator) and a condensing lens
20 105 that focuses a laser beam on the sample 106 to be analyzed (the sample 106 not being a component of the apparatus). Condensing lenses 107 and 108 are used to focus beams on the spectrometer slit after passing through the sample 106 and an absorbance filter 109 is used to pass a Raman emission signal (secondary radiation). The Raman instrument 100 also includes a single or double monochromator spectrometer 110, a detector of secondary
25 radiation 111 (*e.g.*, a photomultiplier), a pulse recording system 112 controlled by the stroboscopic system 104, and, optionally, a computer 113 for data collection and processing and for management of the spectrometer 110. The spectrophotometer 110 may be a single, double, or triple monochomator for the visible and ultraviolet region of the spectra, equipped with a photomultiplier 111 and sensitive photon-counting detector system 112. The high

energy laser **101** pulses irradiate the fluoroorganic sample **106** and also activate a device **104**, to form a strobe-impulse used to synchronize the pulse recording system **112**. Samples preferably are placed into cylindrical quartz cuvettes having parallel windows (not shown). Raman spectra is observed at 90° with respect to the incident pulse by using a single or
5 double monochromator **110** with a single channel detection. When irradiated, the sample **106** emits pulsed Raman radiation and also scatters part of the incident Raman pulse. The absorbance filter **109** removes scattered radiation and passes the pulsed Raman radiation to the spectrometer **110**. Signals are photomultiplied and sent to a synchronized pulse recording system **112**. To obtain ultraviolet radiation (255.3 nm; 271.2 nm and 289.1 nm), a
10 doubling crystal, such as BaB₂O₄, or a tripling crystal, can be used.

A suitable laser **101** that can be used with the apparatus is designed and manufactured at Lebedev Institute of Physics (Russian Academy of Sciences, Moscow, Russia). One such laser is a 3-watt or 10-watt Russian-designed air-cooled copper-vapor laser manufactured by the Lebedev Physics Institute. A stroboscopic generator **104** that can be used with the
15 instrument **100** is also designed and manufactured at Lebedev Institute of Physics (Russian Academy of Sciences, Moscow, Russia). The spectrophotometer **110** can be any standard monochromator or a commercial product such as a Jobin-Yvon U1000 double monochromator Raman spectrometer. Preferably, this spectrophotometer is modified to permit observation of the spectra of fluoroorganic compounds as shown in FIGS. 2-8, below.
20 The optical filter can be a GUI-6 absorption optical filter. The monochromator can be an MSD-2 monochromator. The photomultiplier **111** can be an FEU-106 photomultiplier.

Excitation light emitted by the metal-vapor laser **101** are attenuated by an optical absorption filter **109** placed in front of a sample **106**. The filter **106** is used to limit the excitation light going to the sample. In the spectral range 200-400 nm, the filter **109** can be
25 an ultraviolet filter, such as a GUI-6. In the range 360-480 nm, the filter can be a blue wavelength filter, such as a BG-12. GUI-6 and BG-12 filters are commercially available from AGFA. The luminescence spectra are preferably normalized to allow for the transmission coefficient of the relevant filter **109**.

A pulsed metal-vapor laser **101** has significant advantages over continuous wave argon or helium-neon lasers. The pulsed signal generates significantly less photodecomposition and permits the simple elimination of primary fluorescence, as described by Skoog & Leary, above. Further, laser **101** is significantly cheaper than Raman spectrometers that use longer wavelength excitation lasers, particularly to the Nd:YAG laser at 1064 nm, to eliminate fluorescence. This is because the longer wavelength lasers require expensive CCD signal detectors that significantly increase cost.

The metal-vapor laser **101** can provide about 16 times the signal of commercial Nd:YAG laser Raman spectrometers. Because the Raman vibrational scattering emissions are detected during a narrow time interval ("gate") approximately equal to the laser pulse duration (10^{-8} sec), fluorescence is eliminated. Pulsed techniques also give enhanced sensitivity.

Thus, the intense characteristic Raman band of the symmetric vibrational normal mode of carbon-fluorine bond or groups in the Raman spectra of organic compounds, excited by the pulse laser source, can be established. For example, to achieve optimal excitation of a C-F band, the exposure of the sample to the excitation source must be 10^{-8} seconds or more. Preferably, the Raman spectrum is measured within the above exposure period. Therefore, the Raman spectra is not affected by fluorescence.

The present inventors have discovered that, using the Raman instrument **100**, an emitting signal of a carbon-fluorine bond normal mode (vibrational) or carbon-fluorine group normal mode (rotational), which occurs within a narrow frequency range, is very strong with recognizable narrow band widths. The term "normal mode" refers to the symmetric vibrational process of excited atoms. The radiation characteristic of carbon-fluorine bonds may be detected in the $500\text{--}800\text{ cm}^{-1}$ region. Other radiation in the $950\text{--}1400\text{ cm}^{-1}$ region commonly associated with fluoroorganic compounds can also be observed.

The published frequency range for carbon-fluorine bond infrared absorption is 1000 cm^{-1} to 1400 cm^{-1} . These other bands are useful and can be used to confirm carbon-fluorine groups detected by the method of the invention. However, these infrared absorptions are

subject to interference by other functional groups in the fluoroorganic compound, as discussed above.

A type of carbon-fluorine bond can also be identified in the preferred method. It is contemplated that the method of the invention does not measure the vibration of fluorine against carbon (such C-F vibrations occur in the infrared at 1000-1400 cm^{-1}). Rather, the method detects deviations from the totally symmetric Raman active mode of the groups (such as the carbon-fluorine group in the aromatic compound hexafluorobenzene or the trifluoromethyl group in trifluoromethylated compounds, such as 1,3,5-tris(trifluoromethyl)benzene). The method detects changes in the polarization of carbon-fluorine groups as part of the total molecular vibrational normal modes.

The laser **101** is adaptable to frequency doubling to give a strong signal in the ultraviolet (UV) at about 255.4 nm. UV signals at 272 nm and 289 nm are also available. Irradiation of samples in the ultraviolet allows the observation of resonance Raman spectra which have signals approximately 10^4 to 10^5 stronger (10,000-100,000 times stronger) than normal Raman signals. Resonance Raman signals means detection of compounds containing carbon-fluorine bonds at the parts per billion (ppb) level. Frequency doubling of the wavelengths is observed for both the copper-vapor laser and the gold-vapor laser.

FIG. 6 is a schematic drawing of a Raman spectrometer **200** as adapted for resonance Raman spectroscopy. The Raman spectrometer **200** is similar to the Raman instrument **100** in FIG. 1. However, the spectrometer **200** includes a non-linear frequency doubling crystal **4**. The frequency doubling crystal can be constructed of barium borate. The spectrometer **200** may also include additional filters **14**.

The doubled frequencies, expressed as wavelengths, for a copper-vapor laser may be about 255 nm and 289 nm. A combination band at 272 nm may also be useful. For a gold-vapor laser, the doubled frequency wavelength is about 314 nm. Almost all of the compounds of TABLE 1 below have aromatic rings and are almost certain to give significant enhancement of the resonance Raman emission signal due to the high self-absorbance of the aromatic ring structures. Aromatic rings absorb energy at frequencies similar to those

emitted (self-absorption). Using a frequency doubling crystal, the frequency may be shifted from 510.6 nm to 255.3 nm where it is absorbed.

The spectrometer **200** permits a significant suppression of dark current and environmental noise, and also increases sensitivity. The background of continuous
5 fluorescence can be suppressed by using a strobe-impulse. The strobe-impulse is synchronized with a laser source pulse and “opens” a detection system for only about 10^{-8} sec. This period corresponds to the duration of the preferred laser pulse. As a result, the spectrometer **200** permits a low level detection of fluoroorganic compounds.

10 *Compounds*

A Raman band that is characteristic of carbon-fluorine bonds can be found in the range 540 cm^{-1} to 785 cm^{-1} , based on experimental observations. For estimation purposes, a range of $500\text{--}800\text{ cm}^{-1}$ is reasonable.

Many fluoroorganic compounds are manufactured commercially. Most of the
15 compounds find use as drugs in medicine or veterinary medicine, anesthetics, herbicides, insecticides, pesticides or as industrial intermediates. FIG. 9 shows the structures of some commercially useful compounds. These compounds include carbon-fluorine bonds of trifluoromethyl groups, aromatic carbon-fluorine bonds, and perfluoroalkyl groups.

Aromatic carbon-fluorine bonds are observed in the range of $540\text{--}610\text{ cm}^{-1}$. Examples
20 are hexafluorobenzene, 569 cm^{-1} ; and pentafluoropyridine, 589 cm^{-1} .

Trifluoromethyl groups are observed in the range of $710\text{--}785\text{ cm}^{-1}$. Examples are:
1-bromoperfluorooctane, 726 cm^{-1} ; perfluorodecanoic acid, 730 cm^{-1} ;
triperfluoropropylamine, 750 cm^{-1} ; 1,3,5-tris-(trifluoromethylbenzene), 730 cm^{-1} ; fluoxetine
(Prozac®) commercial powdered pill at 770 cm^{-1} . TABLE 1 (see, Key *et al.*, *Environmental*
25 *Science and Technology* 31: 2445-2454, 1997) lists commercial fluoroorganic compounds containing trifluoromethyl groups. Most of these compounds have an aromatic ring, so resonance Raman can be observed. For example, Prozac® gives a sharp identifiable signal at 770 cm^{-1} , as shown in FIG. 5.

TABLE 1
APPLICATIONS OF TRIFLUOROMETHYL-SUBSTITUTED ORGANIC COMPOUNDS

	<u>Herbicides</u>	<u>Herbicides</u>	<u>Insecticides</u>	<u>Fungicide</u>	<u>Medicinal (Use)</u>
5	acifluorifen	flurtamone	acrinathrin	fluazinam	bendroflumethiazide
	benfluralin	fluxofenim	bifenthrin	flusulfamide	(antihypertensive)
	diflufenican	fomesafen	chlorfluazuron	flutolanil	dexfenfluramine
	dinitramine	furyloxyfen	cyhalothrin	furconazole	(obesity)
10	dithiopyr	haloxyfop	flucofuron	triflumizole	fenfluramine
	ethafluralin	lactofen	flufenoxuron	<u>Anaesthetics</u>	(anorectic)
	flazasulfuron	mefluidide	X-fluvalinate	fluroxene	fluoxetine
	fluazifop	nipyraclofen	hydramethylnon	halothane	(antidepressant)
	fluchioralin	norflurazon	tefluthrin	methoxyflurane	fluphenazine
15	flumetralin	oxyfluorfen	triflumuron	isoflurane	(antipsychotic)
	fluometuron	perfluidone	<u>Rodenticide</u>	sevoflurane	halofantrine <i>and</i>
	fluoroglycofen	prodiamine	bromethalin	desflurane	mefloquine.HCl
	flurazole	profluralin	flocoumafen	<u>Lampricide</u>	(antimalarials)
	flurochloridane	thiazafluron	flupropadine	trifluoromethyl-	nilutamide (cancer)
20	flurprimidol	trifluralin		nitrophenol	tolrestat (diabetes)

When no trifluoromethyl group is present, difluoromethylene groups are observed in a range centered at 690 cm^{-1} . An example is perfluorodecalin, a component of blood substitutes developed in Japan and Russia.

In particular embodiments, Raman spectroscopy can be performed on 1-bromoperfluorooctane ($\text{C}_8\text{F}_{17}\text{Br}$; BPFO), polycrystalline perfluorodecanoic acid ($\text{C}_9\text{F}_{19}\text{COOH}$; PFDA), 1,3,5-tris-(trifluoromethyl)-benzene ($\text{C}_6\text{H}_3(\text{CF}_3)_3$; TTFMB); or fluoxetine (Prozac®). The first compound ($\text{C}_8\text{F}_{17}\text{Br}$) is a candidate to carry oxygen in a blood substitute. The second compound ($\text{C}_8\text{F}_{17}\text{COOH}$) is an analog of perfluorooctanoic acid (PFOA), but less volatile. PFOA has been found in tissues of workers exposed to PFOA in the workplace. The third compound ($\text{C}_6\text{H}_3(\text{CF}_3)_3$) contains carbon-fluorine bonds that are in trifluoromethyl groups. $\text{C}_6\text{H}_3(\text{CF}_3)_3$ is an analog of many useful compounds now sold commercially as drugs, herbicides, and pesticides, some of which are presented in TABLE 1. Fluoxetine (Prozac®; $\text{C}_{17}\text{H}_{18}\text{F}_3\text{NO}$) is a widely prescribed drug which contains a trifluoromethyl group.

In further embodiments, resonance Raman spectroscopy can be performed on perfluorodecalin (C_8F_{18} , PFD) and 1-bromoperfluorooctane ($\text{C}_8\text{F}_{17}\text{Br}$, BPFO). The schematic

of the instrument used to observe the resonance Raman spectra is given in FIG. 6. Most of the compounds of TABLE 1 should give enhanced resonance Raman spectra.

A Raman spectrum (0-1500 cm^{-1}) of liquid $\text{C}_8\text{F}_{17}\text{Br}$ (BPFO) is shown in FIG. 2. A very strong peak at 730 cm^{-1} is present in this spectrum. The compound $\text{C}_8\text{F}_{17}\text{Br}$ is a fluoro-derivative of octane (C_8H_{18}) in which the 18 hydrogens are replaced with 17 fluorine atoms and one atom of bromine. FIG. 2 also shows a Raman spectrum of C_8H_{18} in the upper right corner. This spectrum does not have a peak near 730 cm^{-1} . As in $\text{C}_6\text{H}_3(\text{CF}_3)_3$ spectrum, the appearance of the 730 cm^{-1} peak in $\text{C}_8\text{F}_{17}\text{Br}$ is due to a carbon-fluorine bond signature. This peak corresponds to a fully symmetric vibrational normal mode of a molecule containing the carbon-fluorine bond, specifically the trifluoromethyl group or perfluoroalkyl group.

A Raman spectrum for polycrystalline $\text{C}_9\text{F}_{19}\text{COOH}$ (PFDA) is given in FIG. 3. As for earlier discussed fluoroorganic compounds, a characteristic peak at 726 cm^{-1} has been observed for $\text{C}_8\text{F}_{17}\text{COOH}$. This peak was assigned as a fully symmetric vibrational normal mode of a molecule containing the C-F bond, specifically the trifluoromethyl group or perfluoroalkyl group. The Raman spectrum of nonane (C_9H_{20}) is shown in the upper right corner in FIG. 3. The nonane spectrum does not have any characteristic spectral lines close to 730 cm^{-1} .

A Raman spectrum for $\text{C}_6\text{H}_3(\text{CF}_3)_3$ (TTFMB) and benzene (C_6H_6 , upper right) are shown in FIG. 4. When these two Raman spectra are compared, each has a well-resolved peak at 992 cm^{-1} , which corresponds to the fully symmetric vibrational mode of the benzene ring. At wave numbers greater than 992 cm^{-1} the Raman spectrum of $\text{C}_6\text{H}_3(\text{CF}_3)_3$ shows a doublet at 1085 $^{-1}$, 125 cm^{-1} , and spectral lines at 1376 cm^{-1} , 1513 cm^{-1} , and 1637 cm^{-1} instead of the single lines at 1178 cm^{-1} and 1586 cm^{-1} found for carbon in benzene. The difference between $\text{C}_6\text{H}_3(\text{CF}_3)_3$ and unsubstituted benzene becomes apparent below 992 cm^{-1} . Benzene shows only two weak peaks which correspond to the deformation modes of the C-C bond. By contrast, $\text{C}_6\text{H}_3(\text{CF}_3)_3$ shows a strong peak at 730 cm^{-1} comparable in intensity to the peaks in $\text{C}_6\text{H}_3(\text{CF}_3)_3$ and C_6H_6 at 992 cm^{-1} . The 730 cm^{-1} peak is assigned as a fully symmetric vibrational normal mode of the trifluoromethyl group of the molecule.

The Raman spectrum in FIG. 5 is of the contents of a fluoroxetine ($C_{17}H_{18}F_3NO$) hydrochloride (Prozac®) capsule in the solid powdered form. The composition of the capsule is unknown other than the presence of fluoroxetine hydrochloride. The very narrow sharp peak at 770 cm^{-1} is assigned to a symmetrical vibration involving the trifluoromethyl group. The symmetric aromatic vibration is found at 1001 cm^{-1} .

The Raman spectra of each of the four fluoroorganic compounds ($C_8F_{17}Br$, $C_8F_{17}COOH$, $C_6H_3(CF_3)_3$, and $C_{17}H_{18}F_3NO$) show a characteristic fully symmetric vibrational strong peak at frequencies in the range of $720\text{--}770\text{ cm}^{-1}$ which are assigned to molecular vibrations of the trifluoromethyl group or perfluoroalkyl groups. Comparison of the Raman spectra of the fluoroorganic compounds with their hydrocarbon analogs, suggest that the observed spectral emissions in the range of $690\text{--}770\text{ cm}^{-1}$ are associated with the carbon-fluorine bonds of the compounds studied.

Resonance Raman spectra of perfluorodecalin ($C_{18}F_{38}$) and 1-bromofluorooctane ($C_8F_{17}Br$) are shown in FIG. 7 and FIG. 8. These spectra are shown at two different scales, but are not otherwise electronically processed to enhance the signals. The narrow sharp emission at 692 cm^{-1} is believed to be the totally symmetric normal mode of the difluoromethylene groups (CF_2). 1-bromoperfluorooctane has a weak ultraviolet absorption maximum about 275 nm ($\epsilon=50$) and gives a resonance Raman spectrum with a 730 cm^{-1} emission signal, which is the same emission shown in the regular Raman spectrum (FIG. 2).

Quasi-one-dimensional molecules

As described above, the preferred method detects compounds having carbon-fluorine bonds. It has also been found that carbons in the "quasi-linear" or "quasi-one-dimensional" fluoroorganic molecule chain having a formula C_nH_{2n+2} e.g., C_nF_{2n+1} can also be identified. These molecules are often used in drug formulations, which transport oxygen or carbon dioxide in blood substitutes. These molecules are also used in other pharmaceutical and medicinal applications. Examples of these molecules include $C_{11}H_{11}F_3N_2O_2$ (flutamide) and $C_{10}F_{19}O_2K$ (potassium perfluorodecanoate).

Many linear or quasi-linear fluororganic compounds with different substitution groups can be identified. For example, a substitution group occurs when hydrogens of a molecule are replaced with fluorine to create a fluorocarbon compound. Suitable compounds include anesthetics and those listed in Table 2 below.

5 The C_nH_{2n+2} molecules may be modeled as a resonator. The length of the molecule is inversely proportional to the number of carbons ("n") in the hydrocarbon chain, if n is relatively large. The present inventors have discovered that the fluororganic compounds experience a longitudinal acoustic mode (LAM) and a longitudinal optical mode (LOM) frequency shift. These shifts are dependent on the number of carbons in the molecule chain.

10 A Raman spectra was obtained using an argon laser at about 488.0 nm or a copper-vapor laser at about 510.5 nm. The laser power was about 100 mW. A computerized DFC-24 recording spectrometer with 1 cm^{-1} slit width was employed which was capable of monitoring the position of the gratings. The samples were clear liquid or white crystalline powders. Quartz cuvettes with parallel windows and close fitting tops were used for liquid
15 samples. Raman observations were made at 90-degrees from the incident radiation.

FIG. 11 shows Raman spectra in the region $0\text{-}1400\text{ cm}^{-1}$ for $C_nF_{2n+1}\text{Br}$. A sharp peak in the region $719\text{-}730\text{ cm}^{-1}$ was observed for all Raman spectra. This peak corresponds to the fully symmetrical normal vibration of CF_2 bond. FIG. 12 illustrates that with an increase in n, the maximum peak increased linearly. This means that the peak intensity depends on the
20 length of the molecule.

FIG. 12 illustrates an intensive peak in the region $0\text{-}500\text{ cm}^{-1}$ and overlapping bands in the region $200\text{-}300\text{ cm}^{-1}$. For $n=6, 7$, and 8 , the observed lower frequency band (LAM) included several components. For $n=9, 10$ and 14 the band did not have splitting. A peak signal that was single was observed from C_{14} to C_9 . However, from C_8 to C_6 , the peak began
25 to split.

FIGS. 12 and 13 show that lower frequency LAM $80\text{-}150\text{ cm}^{-1}$ and higher frequency regions LOM $700\text{-}750\text{ cm}^{-1}$ of Raman spectra of $C_nF_{2n+1}\text{Br}$ compounds depend on the number of carbons in the molecule chain. The frequency of the LAM decreases as n increases (FIG. 12). However, the frequency of LOM increases when n increases (FIG. 3).

FIGS. 15 and 16 show Raman spectra of mixtures of fluoroorganic compounds in the spectral area characteristic for a CF₂ bond and the Raman spectra of such mixtures in the lower frequency region LAM. At a concentration higher than about 2%, the Raman peaks were identified for the certain type of the fluoroorganic compound.

Table 2 below lists Raman spectral data for C₁₂F_{2n+1}Br in the LAM and LOM frequency ranges.

TABLE 2

Wave number, cm ⁻¹	Relative Intensity	Bandwidth, cm ⁻¹	Compound
77.7	3634	7.4	C ₁₄ F ₂₉ Br
100.9	1236	5.4	C ₁₀ F ₂₁ Br
111.4	1533	7.0	C ₉ F ₁₉ Br
117.5	1409	6.0	C ₈ F ₁₇ Br
134.6	4694	7.1	C ₇ F ₁₅ Br
142.1	4804	6.3	C ₆ F ₁₃ Br
730.3	2962	5.5	C ₁₄ F ₂₉ Br
727.3	2964	4.4	C ₁₀ F ₂₁ Br
725.4	3398	4.7	C ₉ F ₁₉ Br
723.9	5310	4.7	C ₈ F ₁₇ Br
721.1	5048	4.1	C ₇ F ₁₅ Br
719.8	5567	4.2	C ₆ F ₁₃ Br

Comparison of the different Raman spectra of mixtures of fluororganic compounds indicates that the observed shifts depends on the length of the molecules. The acoustic and optical modes of vibration can be described using the dispersion law as follows:

$$\omega_{\text{acoustic}} = 2 (S / a) \times \sin^2 (ka / 2), \quad (1)$$

$$\omega_{\text{optical}} = \omega_0^2 - 4 (S^2 / a^2) \times \sin^2 (ka / 2), \quad (2)$$

where ω_{acoustic} is the frequency of the acoustic mode;
 ω_{optical} is the frequency of the optical mode;
 k is a vector which has a value of $2\pi / \lambda$, where λ is the wavelength;
 a is the distance between atoms of a molecule chain;
 S is the acoustical propagation speed.

The vector k and the frequencies ω_{acoustic} and ω_{optical} can have various discrete values if the length of the molecule chain is finite and has determined limits. Using the shift of the acoustical and optical frequencies and plotting CF molecular length of CF versus the frequency shift, the molecular length ("L") of quasi-linear molecules in mixtures of fluorocarbon molecules can be estimated. Accordingly, the minimum value for the frequencies can be calculated as follows:

For $f = \omega_{\text{acoustic}} / 2\pi$ at the acoustic mode LAM:

$$f_{\text{acoustic}} = 2 (S / 2\pi a) \times \sin(ka / 2) \approx (S / \pi a) \times (\pi a / 2L) = (S / 2L), \quad (3)$$

where $L \gg a$ and $k_{\text{min}} = \pi / L$.

For $f = \omega_{\text{optical}} / 2\pi$ at the optical mode LOM:

$$f_{\text{optical}}^2 = f_0^2 - 4 (S^2 / 4\pi^2 a^2) \times \sin^2(\pi a / 2L) \approx f_0^2 - S^2 / 4L^2, \quad (4)$$

where L is the length of the molecule.

Assuming that $v_0 = \omega_0 / 2\pi c$, $v = \omega / 2\pi c$, and $k_{\text{min}} = \pi / L$, where v and v_0 are wave numbers, and c is the speed of light, the wavenumber dependencies the length (L) of the molecule for the acoustical (v_{acoustic}) and optical (v_{optical}) branches can be calculated as:

$$v_{\text{acoustic}} = (S / \pi a c) \times \sin(\pi a / 2L). \quad (5)$$

$$v_{\text{optical}}^2 = v_0^2 - (S^2 / \pi^2 a^2 c^2) \times \sin^2(\pi a / 2L). \quad (6)$$

FIG. 14 illustrates experimental Raman frequencies indicated by circles for $C_n F_{2n+1} Br$ at $n=6, 7, 8, 9, 10$, and 14 . The experimental frequencies represent the values of the spectra indicated in FIGS. 11-13. FIG. 14 also illustrates calculated frequencies, as indicated by solid lines, that match the above spectra values. These calculations assume that $L = na / 2$, where n is the number of carbons, *e.g.*, $6, 7, 8, 9, 10$, and 14 . Comparison of the experimental and calculated frequencies indicates that actual Raman frequencies for varying values of n can be accurately calculated using the preferred method.

The dependency of the length of the molecule on the Raman signal has been established in "quasi-one-dimensional" molecules of fluororganic compounds. With an increase in the molecular length, the high frequency (optical) mode LOM of CF_2 linearly

increases, and the lower frequency (acoustical) mode LOM decreased. Accordingly, the length of the molecular species in a mixture using the changing optical and acoustical frequency modes can be approximated.

Sample

The method of the invention can be used to analyze a variety of samples. The method can identify fluoroorganic compounds in liquid, gaseous, crystalline or amorphous solid states or in solutions or suspensions of the fluorooorganic compounds in gases, liquids, solids or multiphase media. The method is more sensitive than other methods for detecting the carbon-fluorine bond of fluoroorganic compounds, permitting detection of fluoroorganic compounds at 10^{-3} - 10^{-6} g/L concentrations level. The background of observation is naturally blank, which permits lower detection limits. The sample can be aqueous solutions of water soluble fluoroorganic compounds including those organic fluorine compounds having low solubility in water or contain traces of water. The method can be used on small solid samples or in solution including aqueous solution. Mixtures can be used when one of the compounds is a fluoroorganic compound, because the unique carbon-fluorine Raman emission, centered around 730 cm^{-1} , is characteristic for fluoroorganic compounds.

Thus, the invention permits the analysis of fluoroorganic compounds where the compound is a drug, herbicide on vegetation, or pesticide on vegetation or animals. The method can be used to follow fluorooorganic compounds used as drugs in animals to determine their presence and the presence of metabolites before excretion. Applications include pharmaceutical research and development, drug clinical trials, drug manufacturing, medical and biomedical applications. Also, organic fluorine compounds or derivatives which contaminate the environment can be detected at the nanogram level. Applications include environmental analysis of water, soil and air contaminated with fluorooorganic compounds, continuous monitoring of manufacturing fluorocarbon products and intermediates, and other similar applications. The method is thus useful in quality control for industrial firms working with fluoroorganic compounds. Dielectrics containing carbon-fluorine bonds are a further area of interest. The ultimate environmental fate of many fluorocarbon refrigerants is

trifluoroacetic acid, which has been found in wetlands in environmental studies. The method is a superior analytical technique to permit analyzing large numbers of soil samples for trifluoroacetic acid or for agriculture fluorinated pesticides. Moreover, the method can greatly reduce the research cost for developing new fluoroorganic pharmaceutical
5 preparations, herbicides, and pesticides.

Quantitation of fluoroorganic compounds in a sample can be achieved by the method of the invention. When an analyst knows the organic fluorine compound present and measures the number of carbon-fluorine bonds, the molar amount of the fluoroorganic compound can be determined.

10 The invention has applications with respect to detecting other carbon-halogen bonds, including carbon-chlorine, carbon-bromine, carbon-iodine, and carbon-astatine.

A number of embodiments of the present invention have been described. Nevertheless, it will be understood that various modifications may be made without departing from the spirit and scope of the invention. The copper-vapor laser-based Raman spectrograph
15 described above may find broader applications. Accordingly, other embodiments are within the scope of the following claims.

CLAIMS

What is claimed is:

- 1 1. A method for directly detecting, in a sample, a compound having a carbon-fluorine bond,
2 comprising:
3 (a) irradiating a sample from a non-continuous periodic pulse light source having a
4 wavelength that induces Raman scattered light emissions from carbon-halogen
5 bonds; and
6 (b) detecting Raman scattered light emitted from the sample, wherein detection of
7 characteristic Raman scattered light is indicative of a carbon-halogen bond in the
8 sample.
- 1 2. The method of claim 1, wherein the compound having a carbon-fluorine bond comprises
2 one or more aromatic carbon-fluorine bonds.
- 1 3. The method of claim 1, wherein the compound having a carbon-fluorine bond comprises
2 one or more trifluoromethyl groups.
- 1 4. The method of claim 1, wherein the compound having a carbon-fluorine bond comprises
2 one or more monofluoromethyl groups.
- 1 5. The method of claim 1, wherein the compound having a carbon-fluorine bond comprises
2 one or more difluoromethylene groups.
- 1 6. The method of claim 1, wherein the compound having a carbon-fluorine bond comprises
2 one or more fluorinated amino acids.
- 1 7. The method of claim 1, wherein the light source is a metal-vapor laser.

- 1 8 The method of claim 7, wherein the metal-vapor laser is a copper-vapor laser.
- 1 9 The method of claim 7, wherein the metal-vapor laser is a gold-vapor laser.
- 1 10. The method of claim 1, wherein the light source is a solid state laser or a light bulb.
- 1 11. The method of claim 1, wherein the irradiation is at $\lambda = 510.6$ nm.
- 1 12. The method of claim 1, wherein the irradiation is at $\lambda = 578.2$ nm.
- 1 13. The method of claim 1, wherein the irradiation is at $\lambda = 627.8$ nm.
- 1 14. The method of claim 1, wherein the detecting Raman scattered light is by a pulse
2 recording system.
- 1 15. The method of claim 1, wherein the Raman scattered light is 540 cm^{-1} to 730 cm^{-1} .
- 1 16. The method of claim 1, wherein the Raman scattered light is 540 cm^{-1} to 610 cm^{-1} .
- 1 17. The method of claim 1, wherein the Raman scattered light is 710 cm^{-1} to 785 cm^{-1} .
- 1 18. The method of claim 1, wherein the Raman scattered light is 726 cm^{-1} to 730 cm^{-1} .
- 1 19. The method of claim 1, wherein the Raman scattered light has a resonance Raman
2 enhancement of greater than 10,000.

- 1 20. An apparatus for Raman spectroscopy, comprising:
2 (a) a non-continuous periodic pulse metal-vapor laser;
3 (b) a monochromator for visible and ultraviolet light;
4 (c) a detector of secondary radiation; and
5 (d) a pulse recording system.
- 1 21. The apparatus of claim 20, wherein the monochromator is a double monochromator or a
2 triple monochromator.
- 1 22. The apparatus of claim 20, further comprising a non-linear frequency doubling crystal or
2 tripling crystal.
- 1 23. A method for detecting a fluoroorganic compound having a molecular length,
2 comprising:
3 exposing a sample to an excitation light source;
4 measuring a frequency of an acoustic mode of the compound;
5 measuring a frequency of an optical mode of the compound;
6 detecting a shift in frequency of the acoustic frequency and the optical frequency; and
7 approximating the molecular length as a function of the shift in frequencies to determine
8 the presence of the fluoroorganic compound.
- 1 24. The method of claim 23, wherein the detection step comprises detecting the shift in
2 frequencies using Raman spectroscopy.
- 1 25. The method of claim 23, wherein the excitation light source is a non-continuous periodic
2 pulse light source.
- 1 26. The method of claim 25, wherein the excitation light source is a metal-vapor laser.

1 27. The method of claim 23, wherein the fluoroorganic compound is quasi-linear or quasi-
2 one-dimensional.

1 28. The method of claim 23, wherein the fluoroorganic compound comprises a substitution
2 group.

1 29. The method of claim 23, wherein the frequency of the acoustic mode decreases with an
2 increase of carbons in the fluoroorganic compound.

1 30. The method of claim 23, wherein the frequency of the optical mode increases with a
2 decrease of carbons in the fluoroorganic compound.

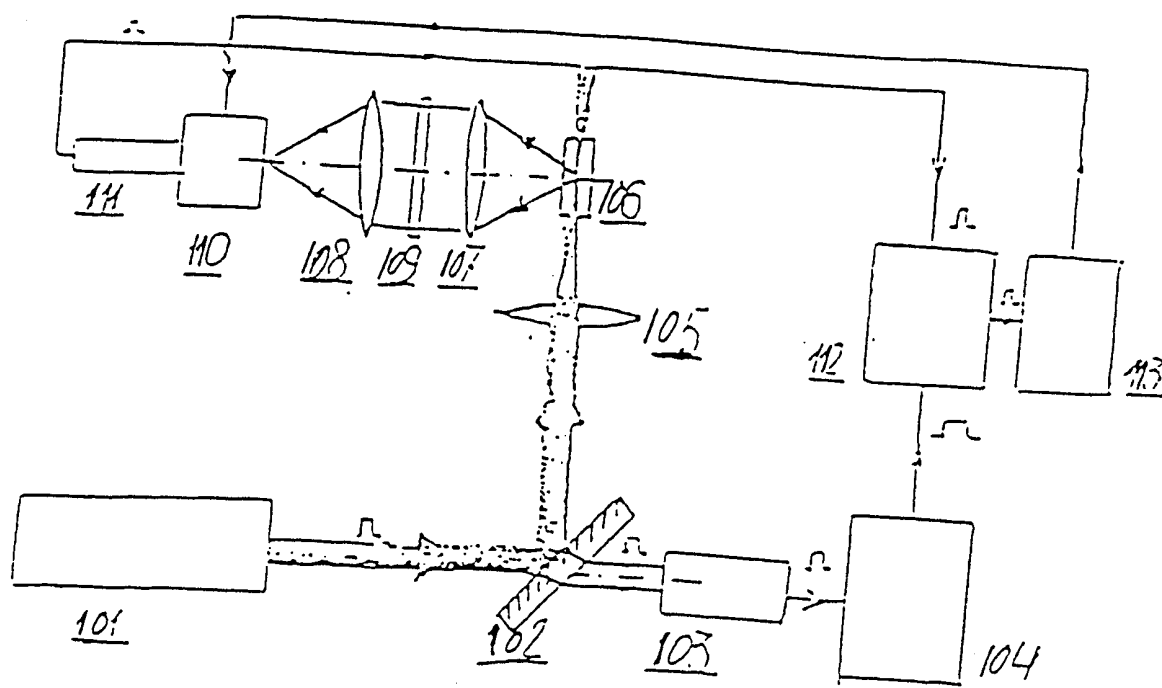


Figure 1 Schematic drawing of Raman spectrometer

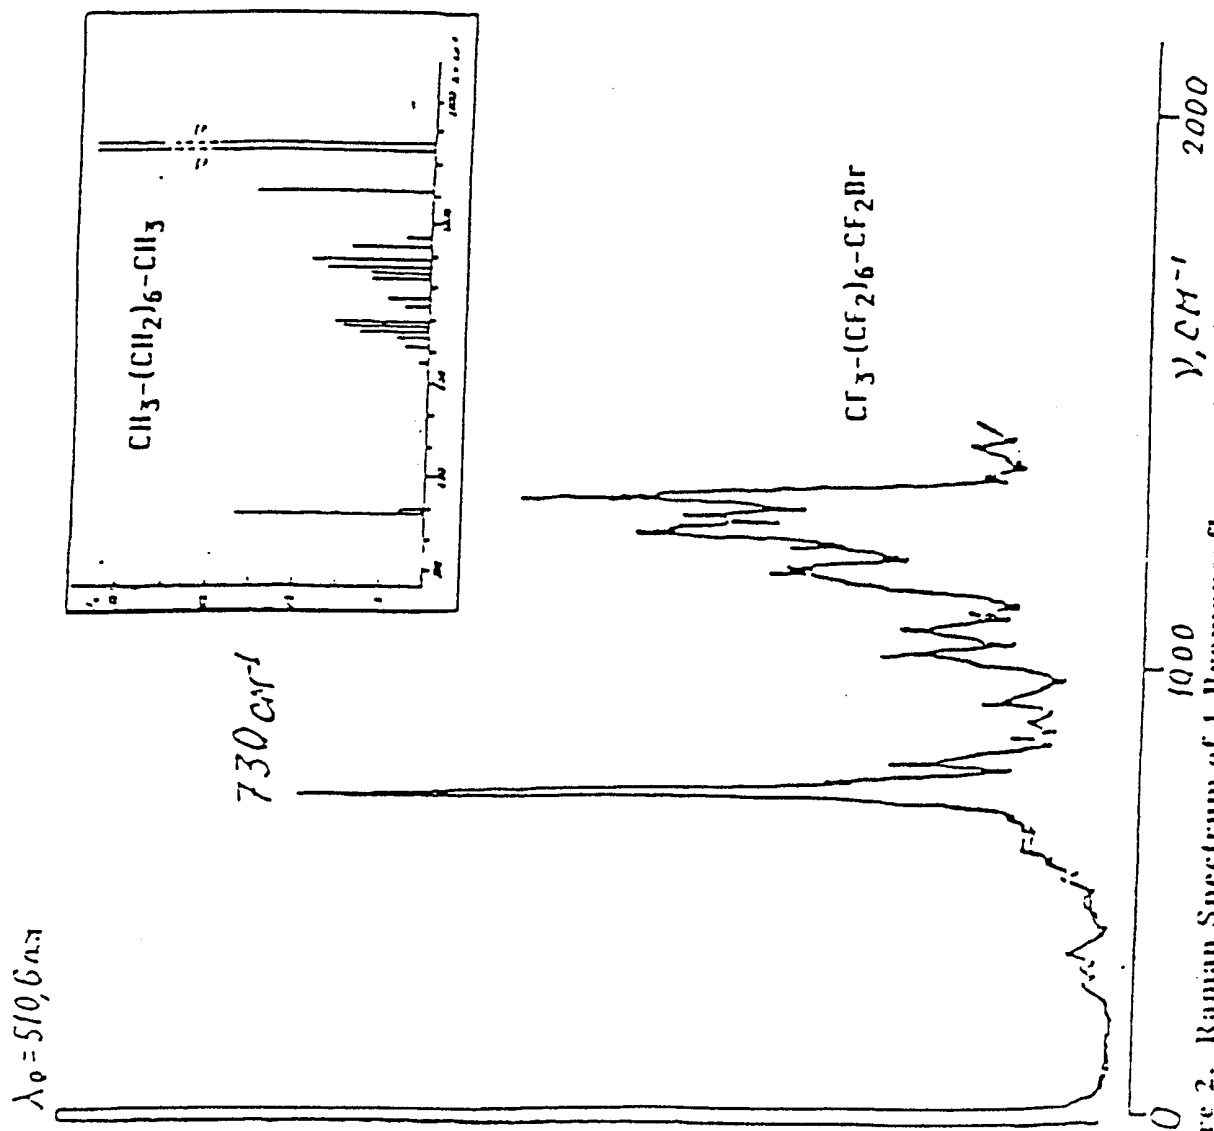


Figure 2. Raman Spectrum of 1-Bromoperfluorooctane (upper left inset: octane)

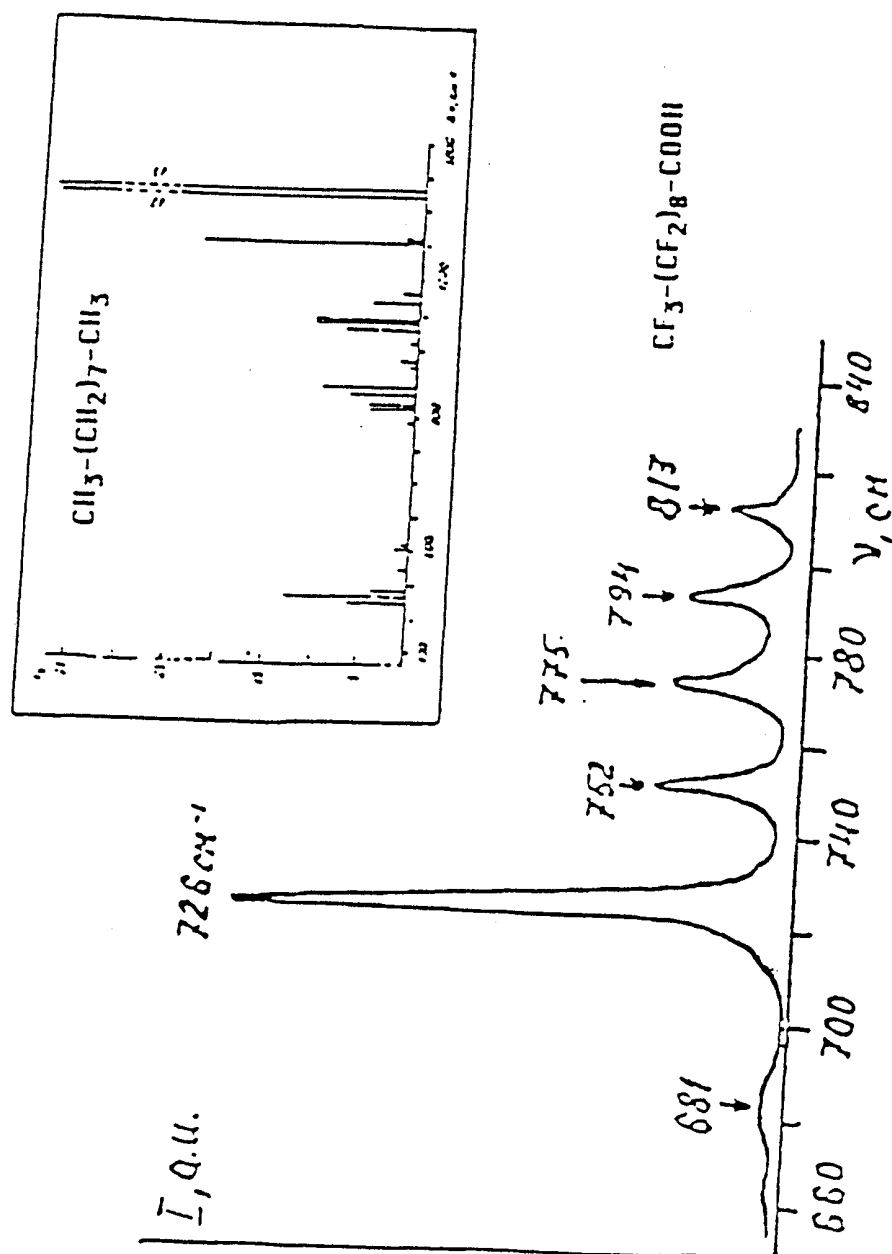


Figure 3. Raman Spectrum of Perfluorodecanoic Acid (upper right inset: nonane)

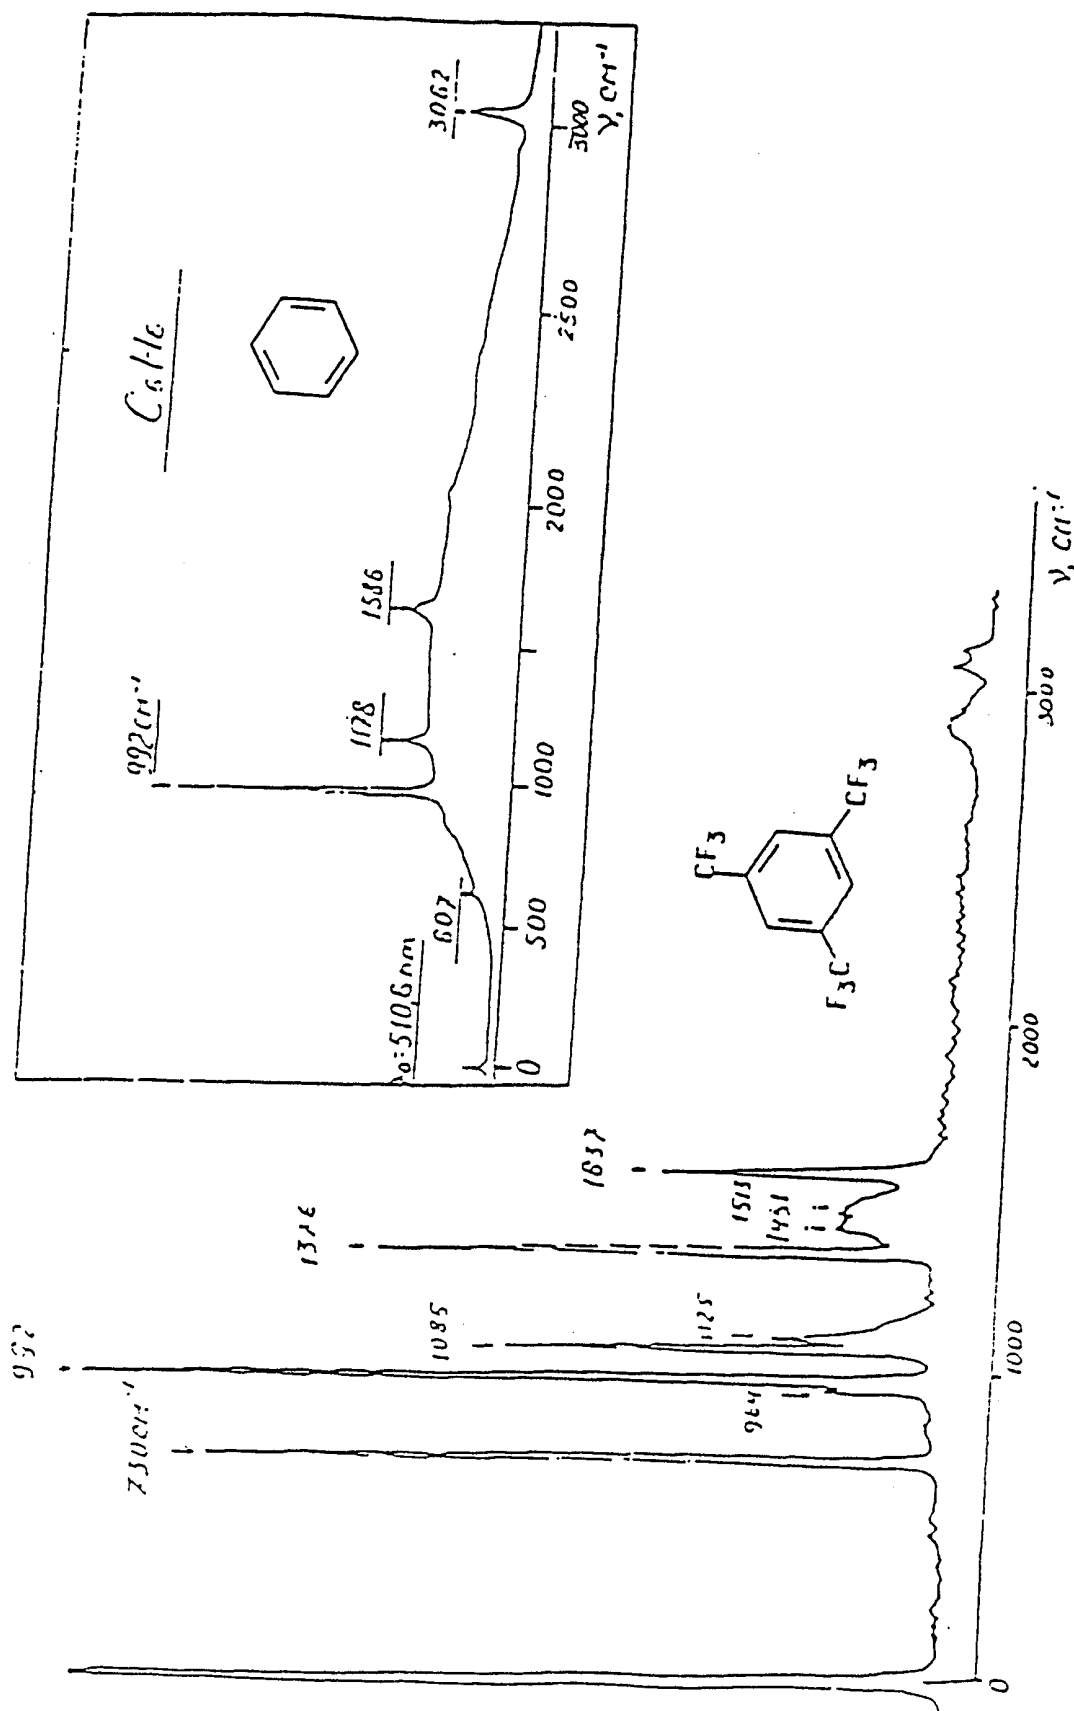


Figure 4. Raman Spectrum of 1,3,5-tris-(Trifluoromethyl)-benzene (upper right inset: benzene)

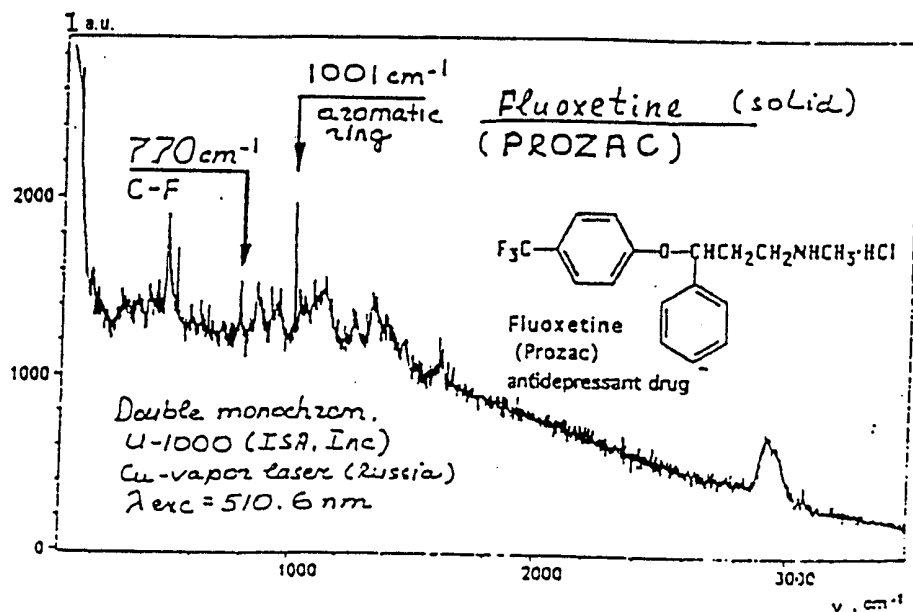


FIG. 5 is a Raman spectrum of a commercial preparation of fluoxetine hydrochloride as a solid-state tablet mixture Prozac as prescribed, excited at 510.6 nm by a copper-vapor laser.

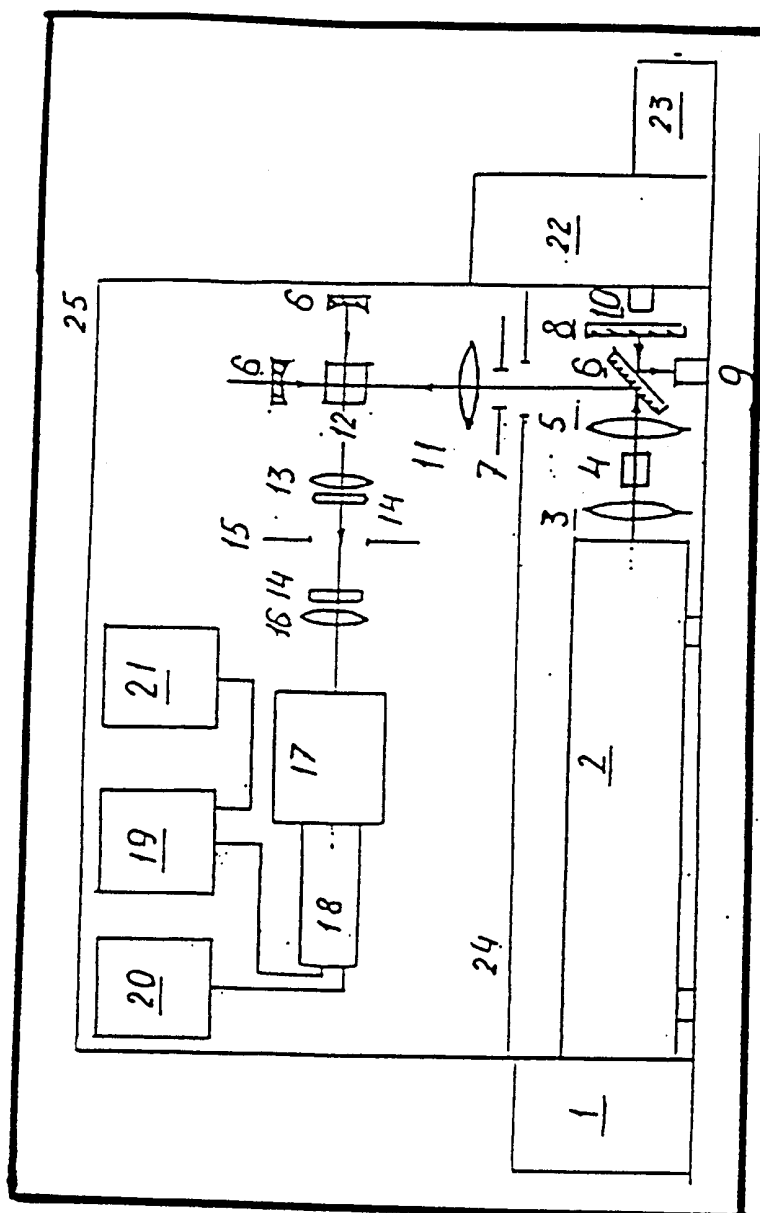


FIG. 6 is a schematic drawing of the Resonance Raman Spectrometer used to observe the Resonance Raman Spectra of various fluoroorganic compounds.



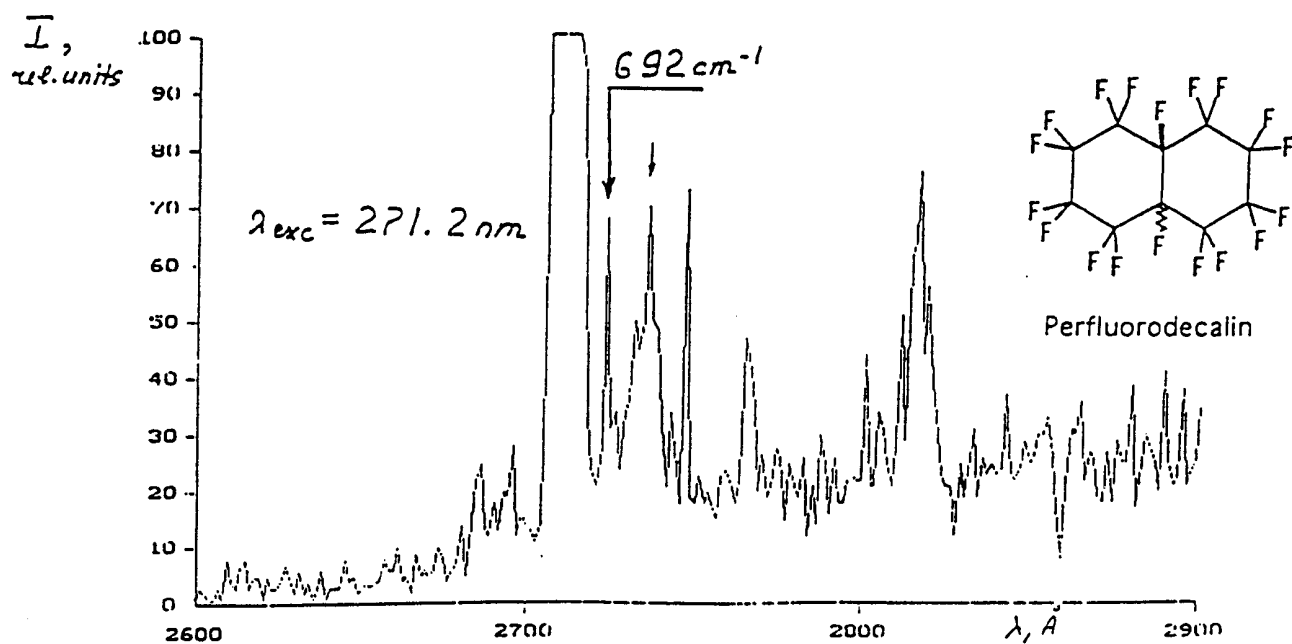



FIG. 7 is a Resonance Raman Spectrum of Peffluorodecalin irradiated at 271.2 nm showing difluoromethylene absorption at 692 cm^{-1}

TOP SPECTRUM: Unprocessed Resonance Raman spectrum of Peffluorodecalin ($C_{10}F_{18}$).


BOTTOM SPECTRUM: Partially processed Resonance Raman spectrum of Peffluorodecalin.

FIG. 8 is an unprocessed Resonance Raman Spectrum of 1-Bromoheptfluorooctane.

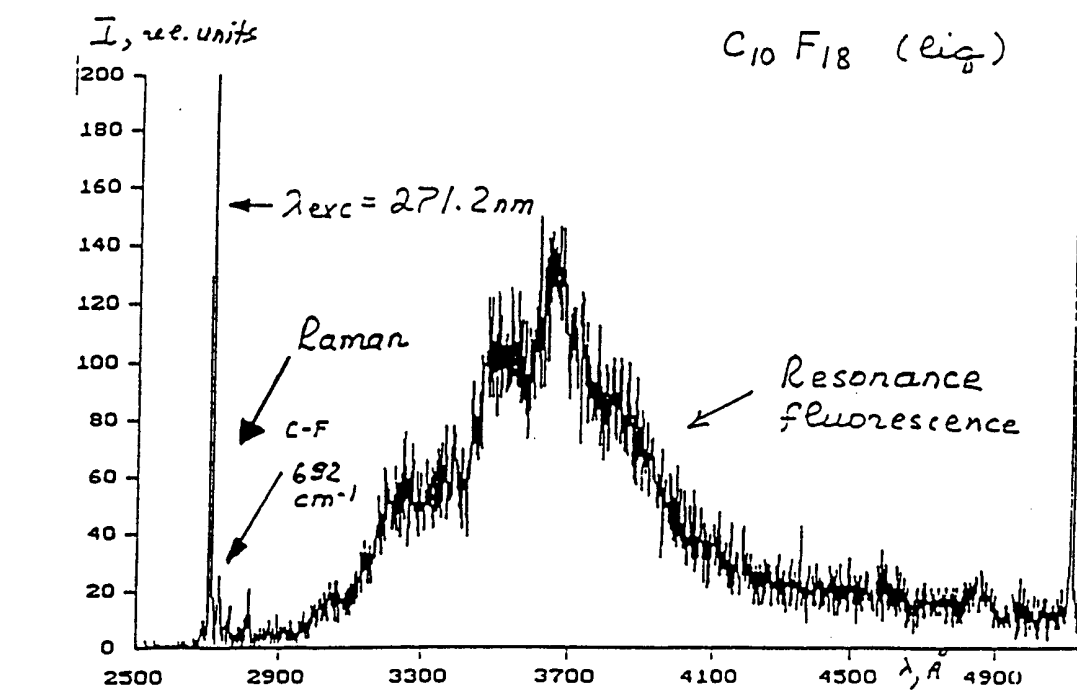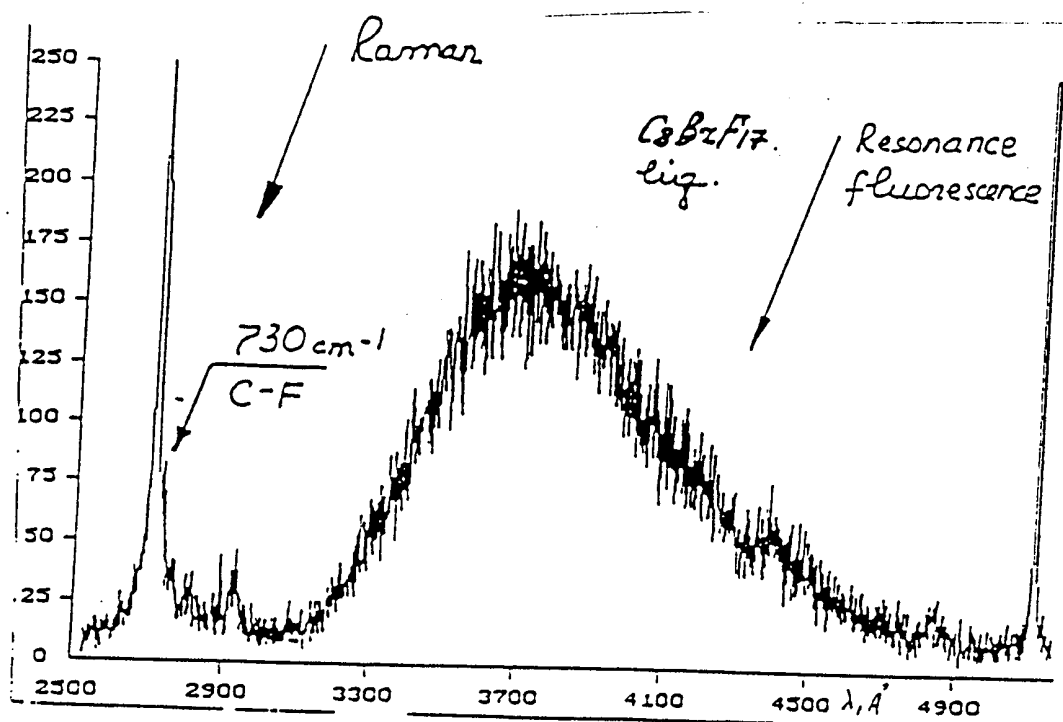





Fluorouracil
(5-FU)
anticancer drug

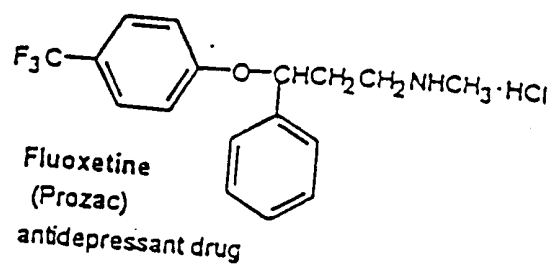


Fluoxetine
(Prozac)
antidepressant drug




Perflubron
blood substitute
(Oxygent)
(Liquivent)

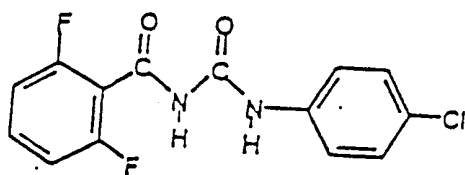


Diflubenzuron
(insecticide)




Flumeturon
(herbicide)




Compound 1080
(pesticide) [natural product]

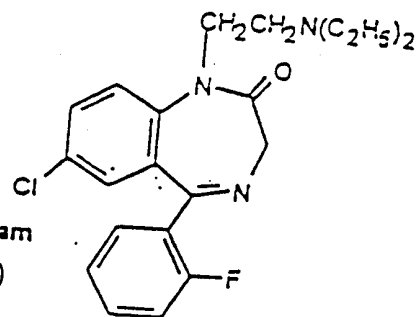

Flurazepam
(Dalmane)
pain killer
tranquilizer







3-Trifluoromethyl-
4-nitrophenol
(lambpricide)

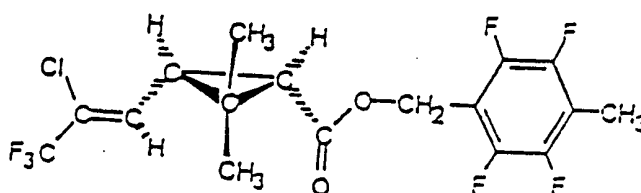


Tefluthrin,
(insecticide)

PPC 993 (ICI) Force®


Figure 9 Structures of some useful commercial fluoroorganic compounds.

Benzene [C₆H₆]Hexafluorobenzene [C₆F₆]1,3,5-(tris)-Trifluoromethyl-
benzene [C₉F₉H₃]Pentafluoropyridine [C₅F₅N]

CF₃CF₂CF₂CF₂CF₂CF₂CF₂CF₂Br
 1-Bromoperfluorooctane [C₈F₁₇Br]
 Perflubron® (blood substitute)

Perfluorotripropylamine [C₉F₂₁N]

CF₃CF₂CF₂CF₂CF₂CF₂CF₂CF₂CF₂CF₂COOH
 1-Perfluorodecanoic Acid [C₁₀F₂₁COOH]



Perfluorodecalin

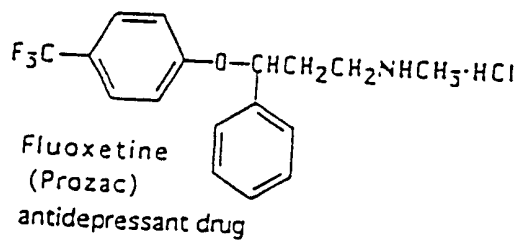


FIGURE 10

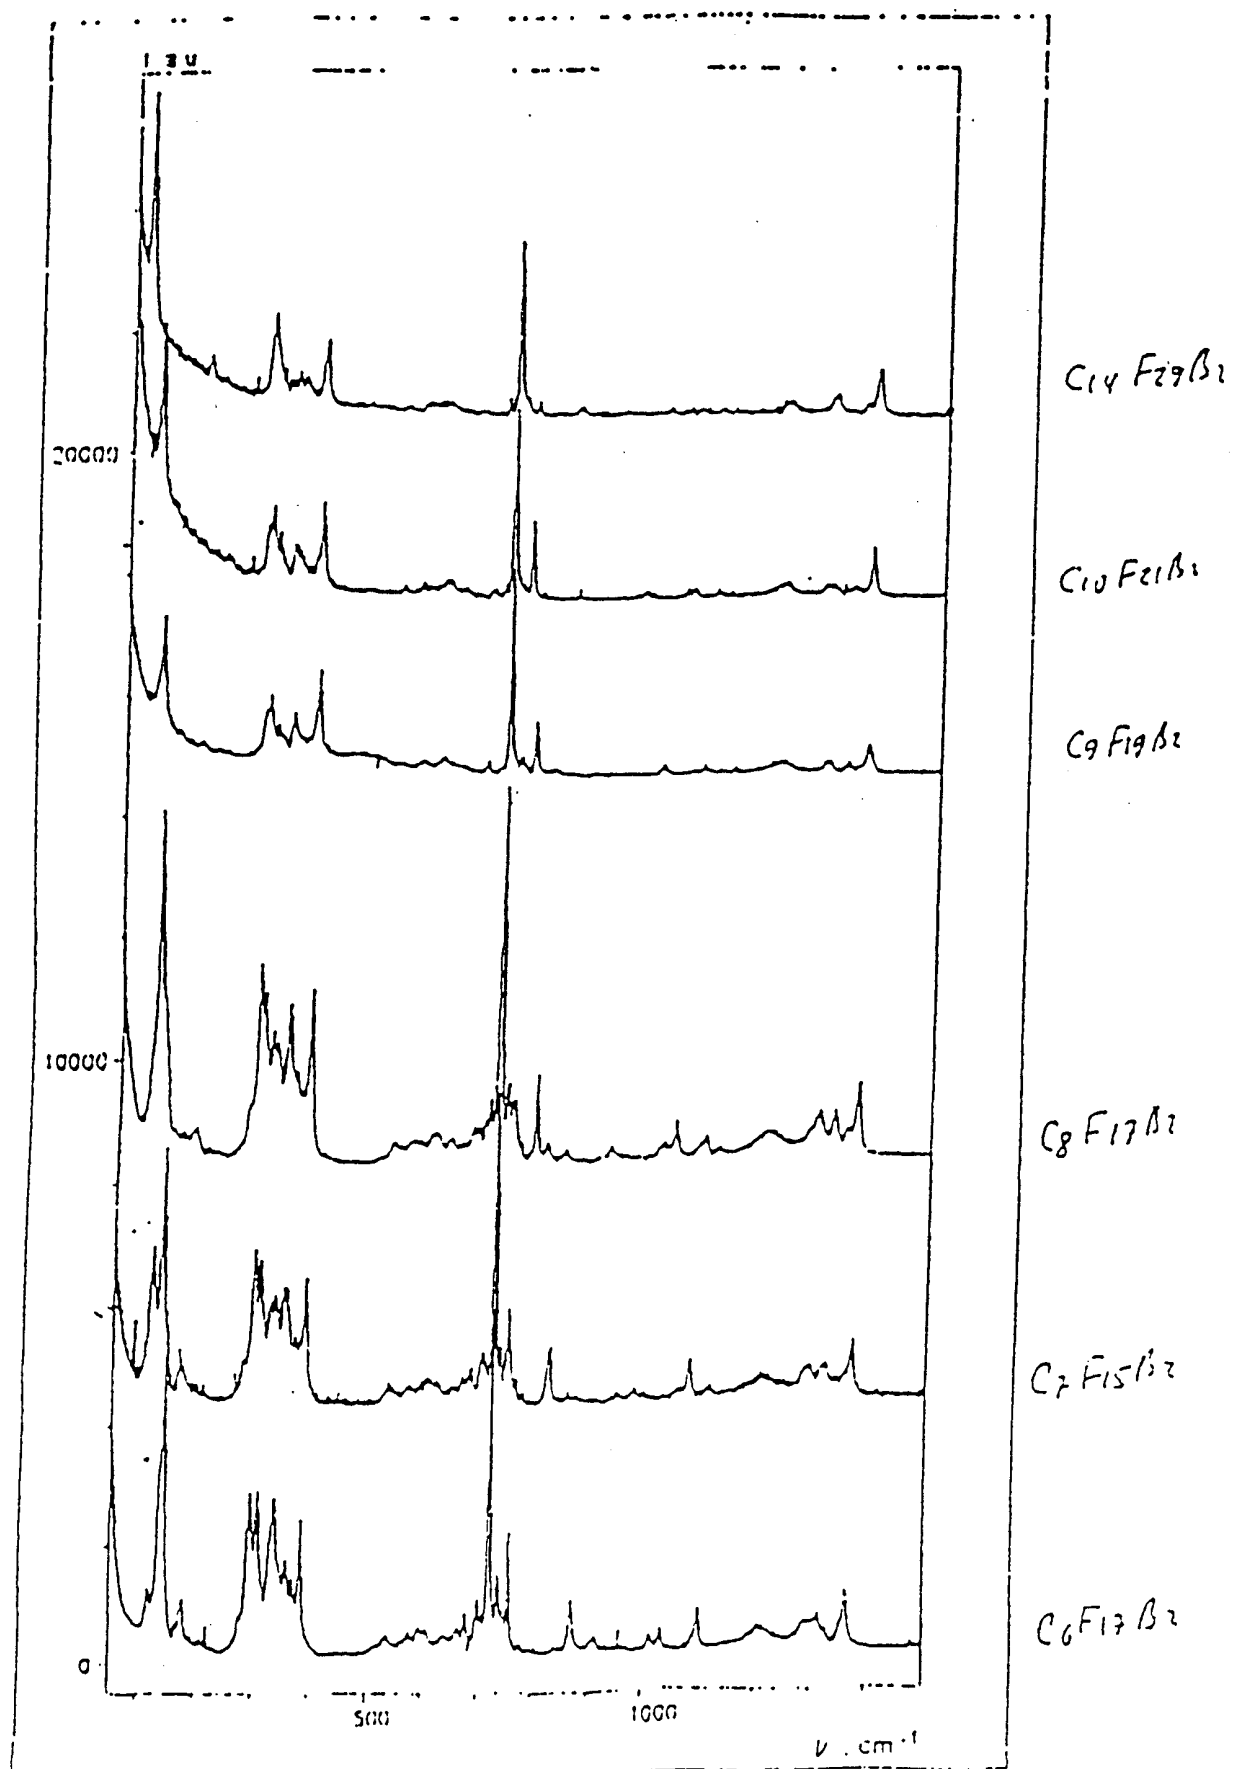


FIG 11

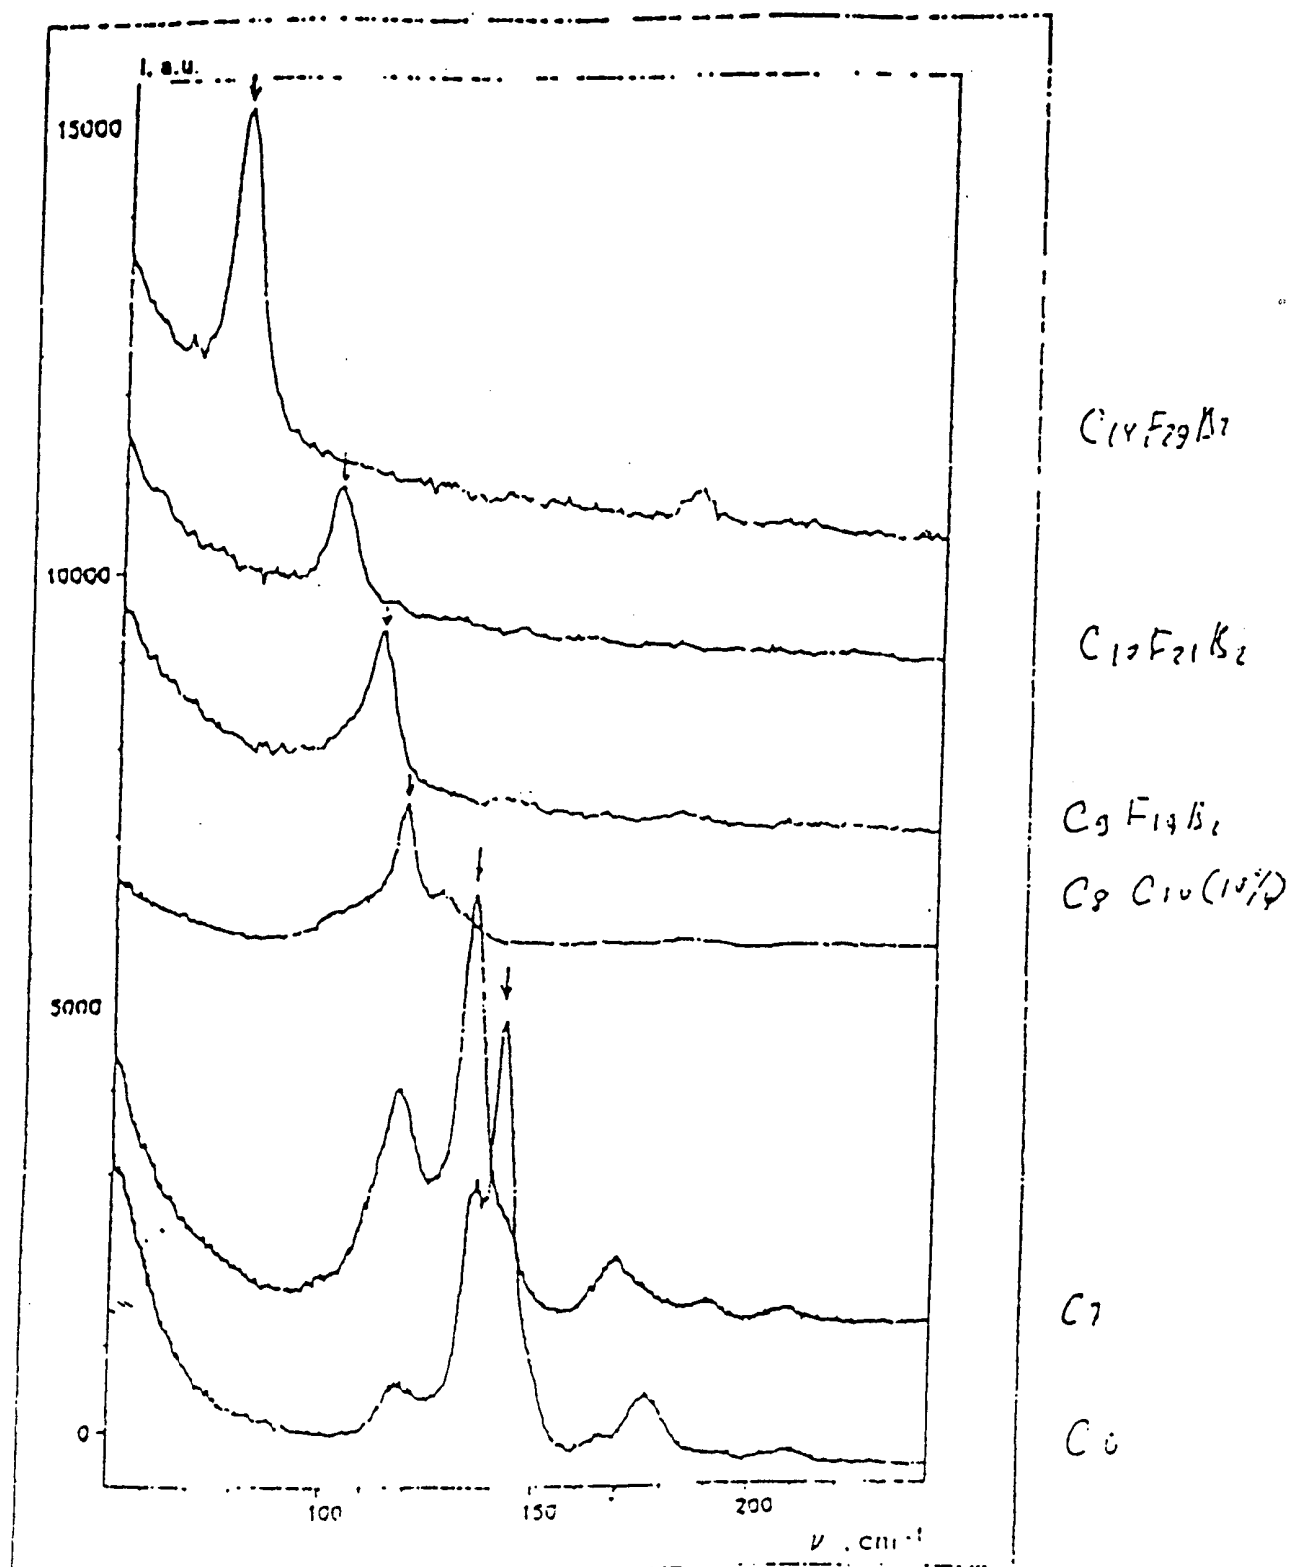


FIG. 12

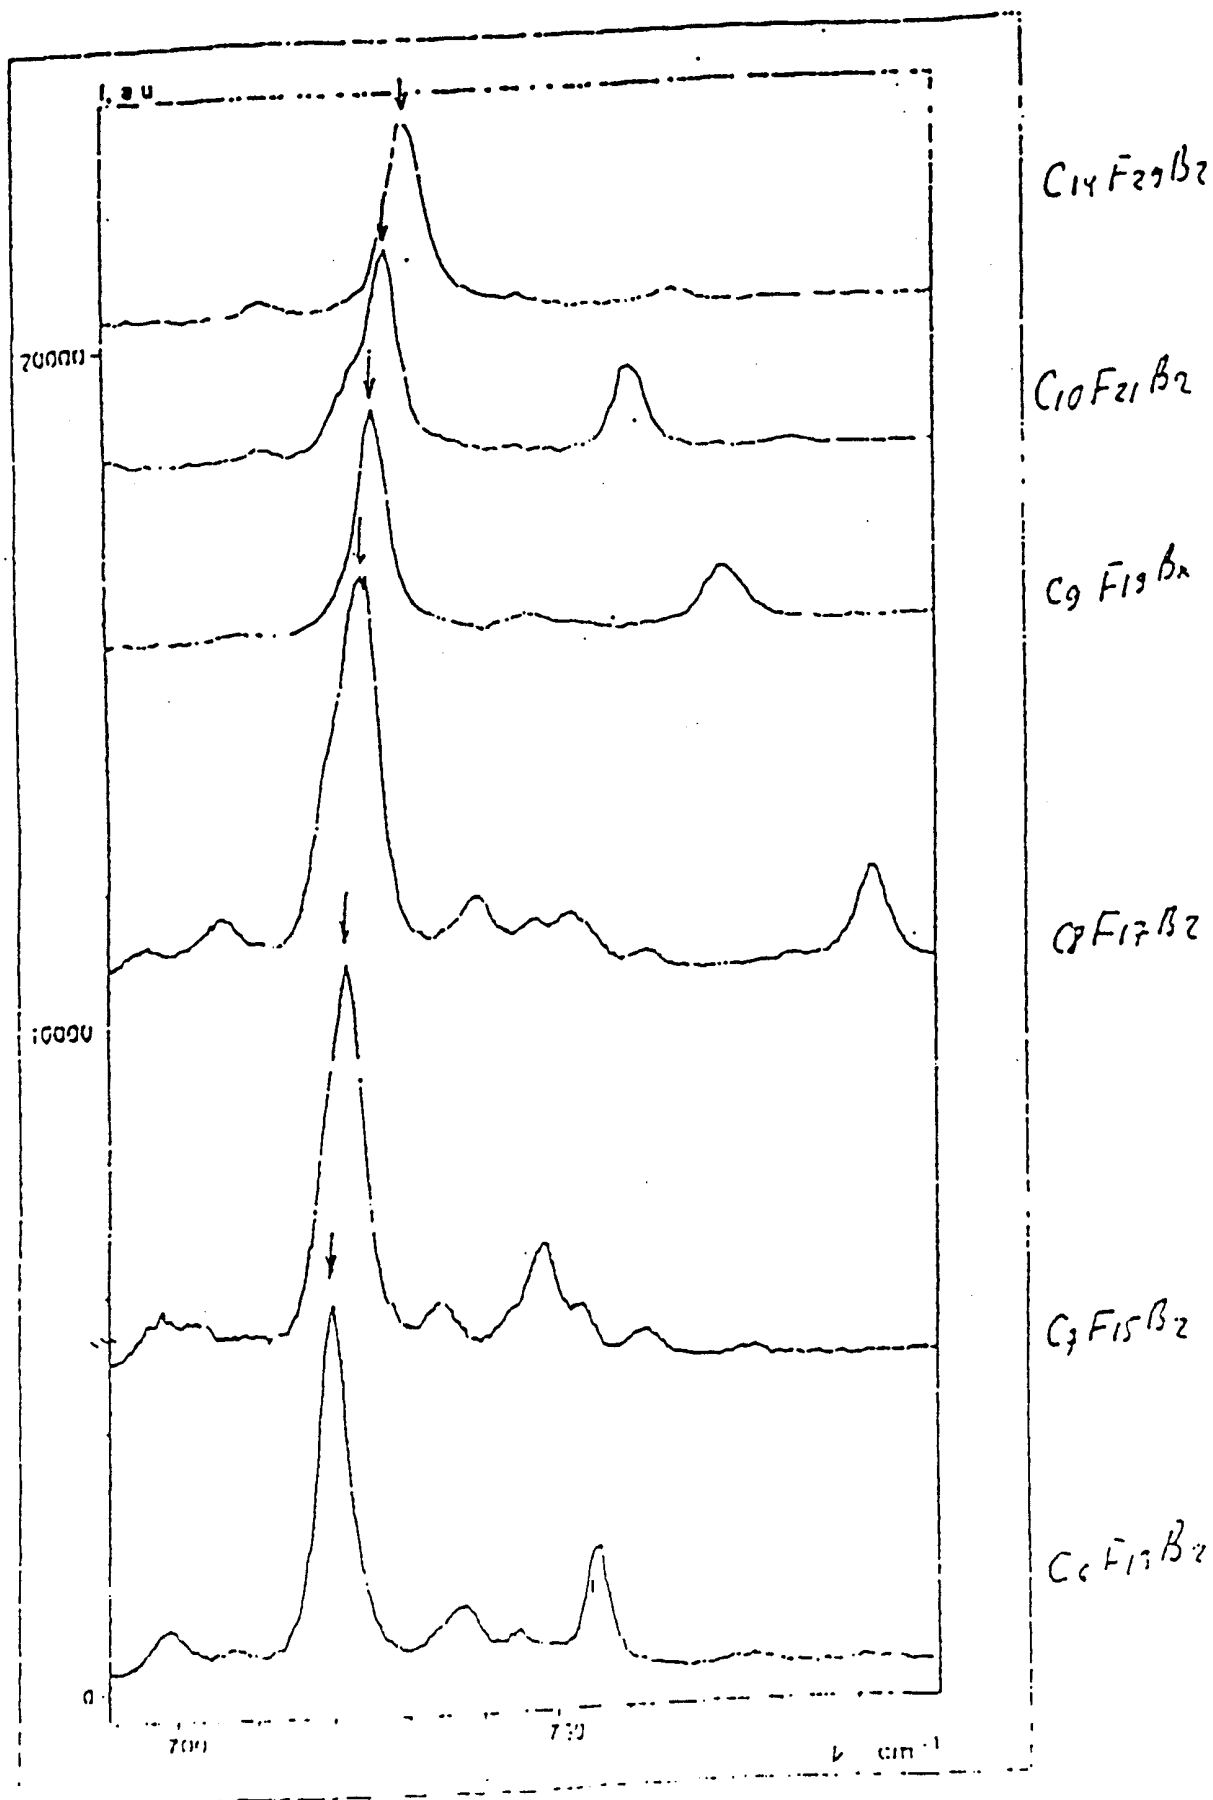


FIG. 13

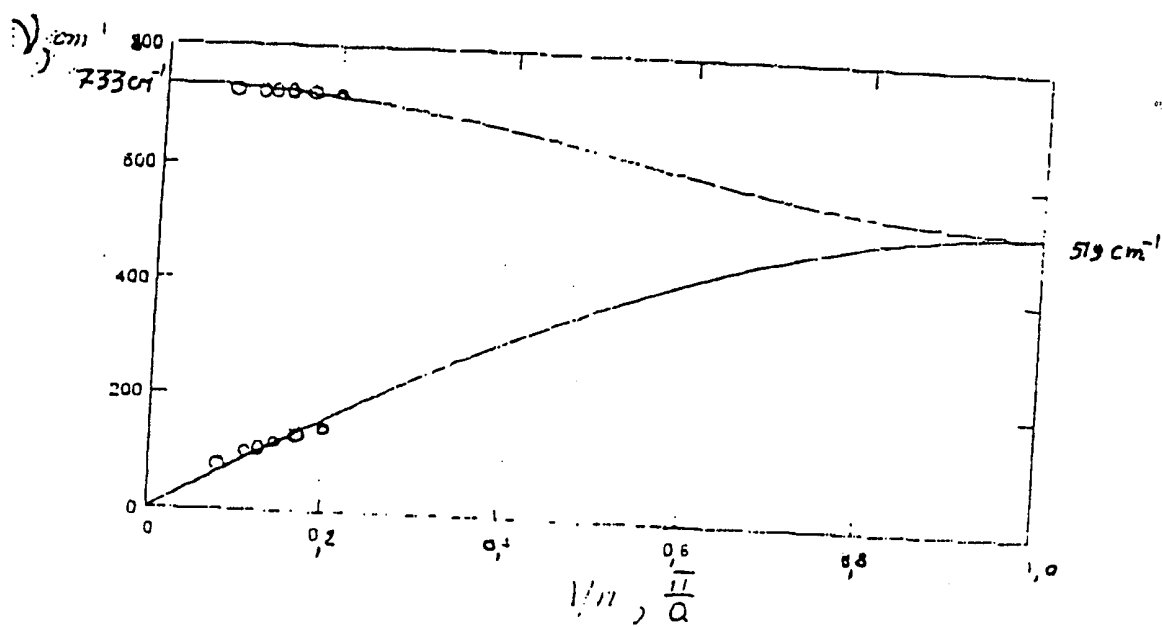


Figure 14.

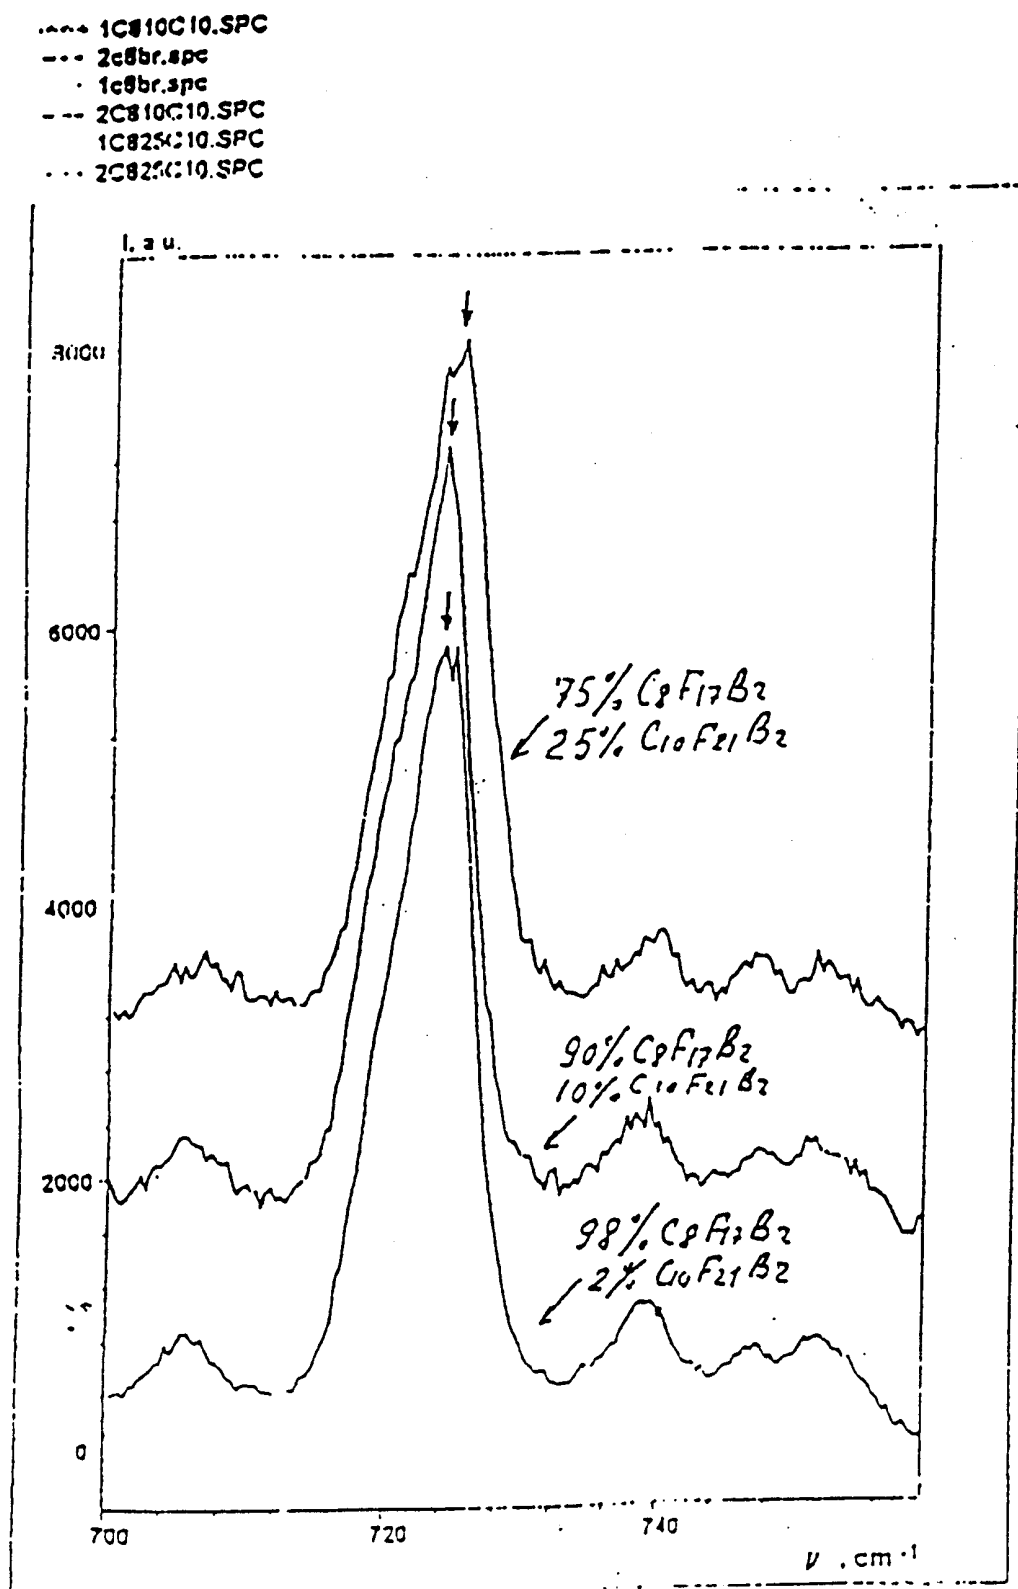


FIG. 15

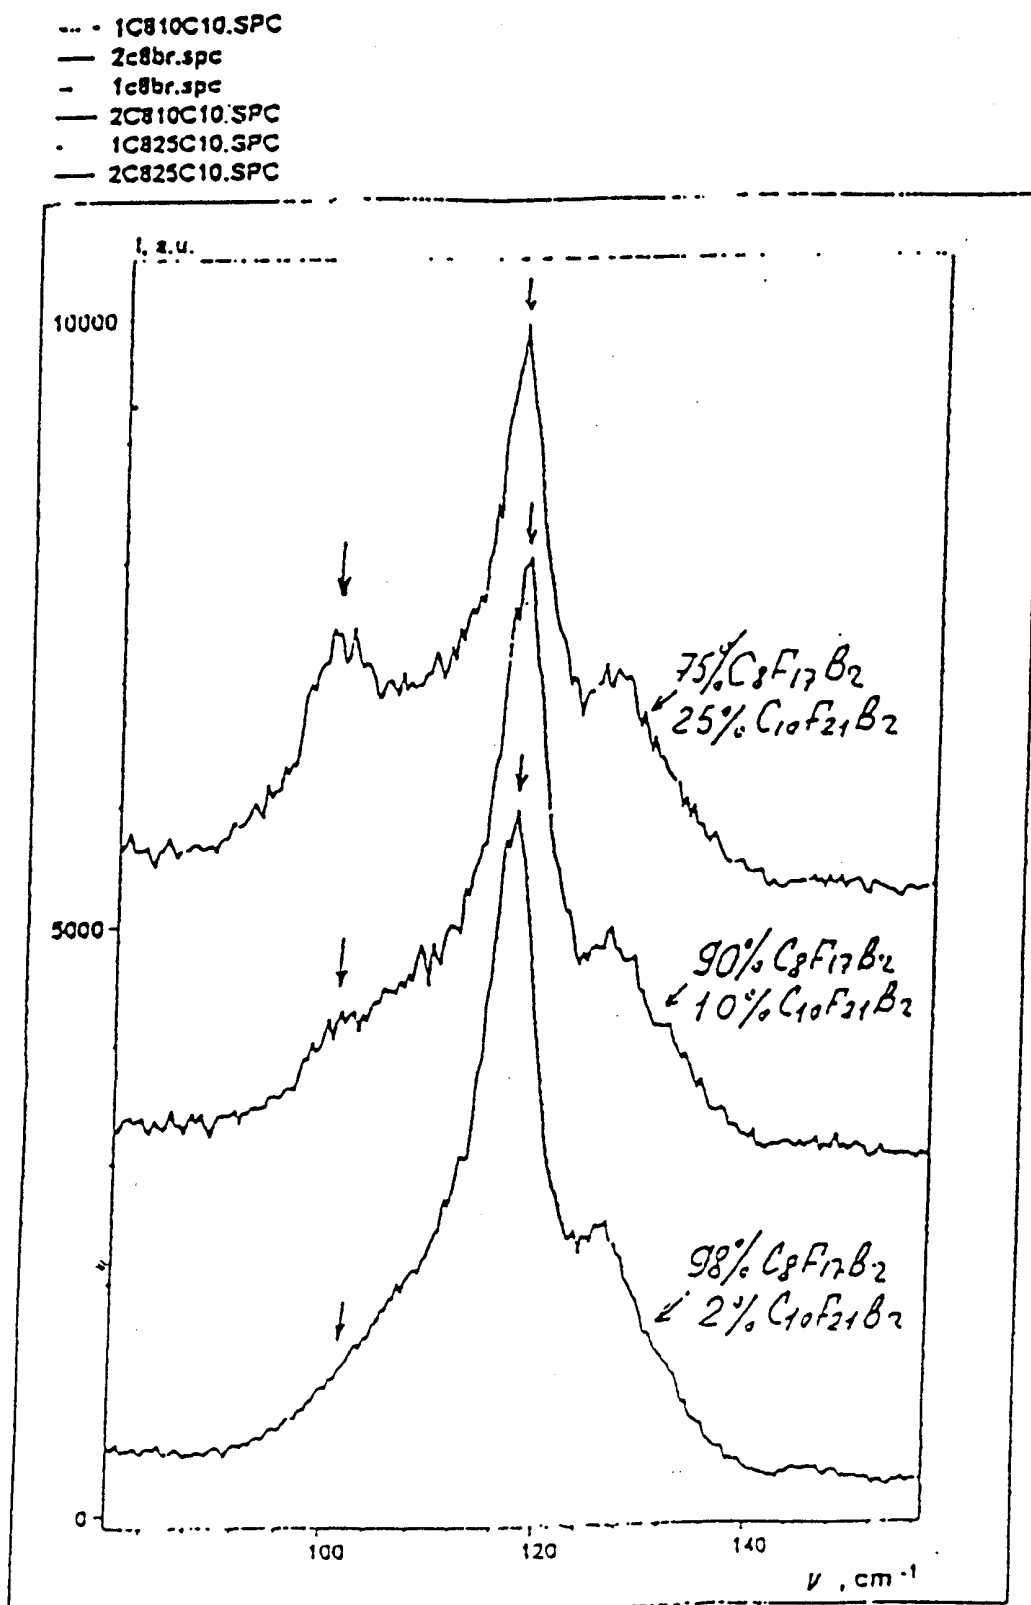


FIG. 16