



US010456038B2

(12) **United States Patent**  
**Lamego et al.**

(10) **Patent No.:** **US 10,456,038 B2**

(45) **Date of Patent:** **Oct. 29, 2019**

(54) **CLOUD-BASED PHYSIOLOGICAL MONITORING SYSTEM**

(71) Applicant: **Cercacor Laboratories, Inc.**, Irvine, CA (US)

(72) Inventors: **Marcelo M. Lamego**, Cupertino, CA (US); **Abraham Mazda Kiani**, San Juan Capistrano, CA (US); **Don Sanders**, Irvine, CA (US); **Jeroen Poeze**, Rancho Santa Margarita, CA (US); **Massi Joe E. Kiani**, Laguna Niguel, CA (US); **Anthony Amir Davia**, Laguna Beach, CA (US)

(73) Assignee: **Cercacor Laboratories, Inc.**, Irvine, CA (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 507 days.

(21) Appl. No.: **14/203,243**

(22) Filed: **Mar. 10, 2014**

(65) **Prior Publication Data**

US 2014/0275835 A1 Sep. 18, 2014

**Related U.S. Application Data**

(60) Provisional application No. 61/801,464, filed on Mar. 15, 2013, provisional application No. 61/841,346, (Continued)

(51) **Int. Cl.**

**A61B 5/00** (2006.01)

**A61B 5/1455** (2006.01)

**G16H 50/30** (2018.01)

(52) **U.S. Cl.**

CPC ..... **A61B 5/0022** (2013.01); **A61B 5/14551** (2013.01); **G16H 50/30** (2018.01); **A61B 5/7235** (2013.01)

(58) **Field of Classification Search**

CPC . A61B 5/0022; A61B 5/14551; A61B 5/7235; A61B 5/0004; A61B 5/0205; A61B 5/7275; G06F 19/3431; G06F 19/3418  
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A 10/1990 Gordon et al.

4,964,408 A 10/1990 Hink et al.

(Continued)

FOREIGN PATENT DOCUMENTS

EP 2 278 508 1/2011

WO WO 2012/099534 7/2012

OTHER PUBLICATIONS

Xiaomao Fan et al., "HCloud: A novel application-oriented cloud platform for preventive healthcare," Cloud Computing Technology and Science (CLOUDCOM), Dec. 3, 2012, pp. 705-710.

(Continued)


*Primary Examiner* — Nathan J Jenness

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson & Bear LLP

(57) **ABSTRACT**

A cloud-based physiological monitoring system has a sensor in communications with a living being so as to generate a data stream generally responsive to a physiological condition of the living being. A monitor receives the data stream from the sensor and transmits the data stream to a cloud server. The cloud server processes the data stream so as to derive physiological parameters having values responsive to the physiological condition. The cloud server derives a medical index based upon a combination of the physiological parameters. The cloud server communicates the medical index to the monitor, which displays the medical index.

**9 Claims, 11 Drawing Sheets**

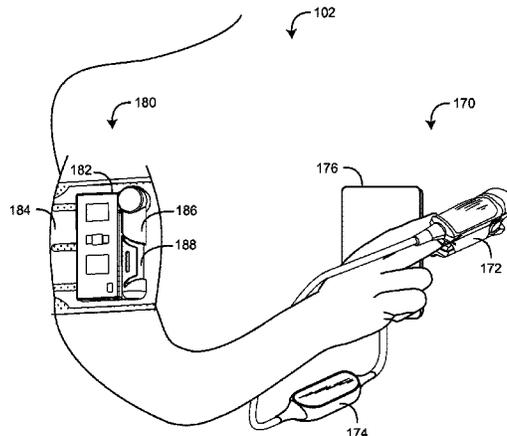

**Related U.S. Application Data**

filed on Jun. 30, 2013, provisional application No. 61/885,491, filed on Oct. 1, 2013, provisional application No. 61/922,861, filed on Jan. 1, 2014.

- (58) **Field of Classification Search**  
 USPC ..... 600/301  
 See application file for complete search history.

- (56) **References Cited**

U.S. PATENT DOCUMENTS

5,041,187 A 8/1991 Hink et al.  
 5,069,213 A 12/1991 Polczynski  
 5,163,438 A 11/1992 Gordon et al.  
 5,319,355 A 6/1994 Russek  
 5,337,744 A 8/1994 Branigan  
 5,341,805 A 8/1994 Stavridi et al.  
 D353,195 S 12/1994 Savage et al.  
 D353,196 S 12/1994 Savage et al.  
 5,377,676 A 1/1995 Vari et al.  
 D359,546 S 6/1995 Savage et al.  
 5,431,170 A 7/1995 Mathews  
 D361,840 S 8/1995 Savage et al.  
 D362,063 S 9/1995 Savage et al.  
 5,452,717 A 9/1995 Branigan et al.  
 D363,120 S 10/1995 Savage et al.  
 5,456,252 A 10/1995 Vari et al.  
 5,479,934 A 1/1996 Imran  
 5,482,036 A 1/1996 Diab et al.  
 5,490,505 A 2/1996 Diab et al.  
 5,494,043 A 2/1996 O'Sullivan et al.  
 5,533,511 A 7/1996 Kaspari et al.  
 5,534,851 A 7/1996 Russek  
 5,561,275 A 10/1996 Savage et al.  
 5,562,002 A 10/1996 Lalin  
 5,565,976 A \* 10/1996 Fieggen ..... G01N 21/7703  
 250/227.16  
 5,590,649 A 1/1997 Caro et al.  
 5,602,924 A 2/1997 Durand et al.  
 5,632,272 A 5/1997 Diab et al.  
 5,638,816 A 6/1997 Kiani-Azarbayjany et al.  
 5,638,818 A 6/1997 Diab et al.  
 5,685,299 A 11/1997 Diab et al.  
 D393,830 S 4/1998 Tobler et al.  
 5,743,262 A 4/1998 Lepper, Jr. et al.  
 5,758,644 A 6/1998 Diab et al.  
 5,760,910 A 6/1998 Lepper, Jr. et al.  
 5,769,785 A 6/1998 Diab et al.  
 5,782,757 A 7/1998 Diab et al.  
 5,785,659 A 7/1998 Caro et al.  
 5,791,347 A 8/1998 Flaherty et al.  
 5,810,734 A 9/1998 Caro et al.  
 5,823,950 A 10/1998 Diab et al.  
 5,830,131 A 11/1998 Caro et al.  
 5,833,618 A 11/1998 Caro et al.  
 5,860,919 A 1/1999 Kiani-Azarbayjany et al.  
 5,890,929 A 4/1999 Mills et al.  
 5,904,654 A 5/1999 Wohltmann et al.  
 5,919,134 A 7/1999 Diab  
 5,934,925 A 8/1999 Tobler et al.  
 5,940,182 A 8/1999 Lepper, Jr. et al.  
 5,995,855 A 11/1999 Kiani et al.  
 5,997,343 A 12/1999 Mills et al.  
 6,002,952 A 12/1999 Diab et al.  
 6,011,986 A 1/2000 Diab et al.  
 6,027,452 A 2/2000 Flaherty et al.  
 6,036,642 A 3/2000 Diab et al.  
 6,045,509 A 4/2000 Caro et al.  
 6,067,462 A 5/2000 Diab et al.  
 6,081,735 A 6/2000 Diab et al.  
 6,088,607 A 7/2000 Diab et al.  
 6,110,522 A 8/2000 Lepper, Jr. et al.  
 6,124,597 A 9/2000 Shehada  
 6,128,521 A 10/2000 Marro et al.  
 6,129,675 A 10/2000 Jay  
 6,144,868 A 11/2000 Parker

6,151,516 A 11/2000 Kiani-Azarbayjany et al.  
 6,152,754 A 11/2000 Gerhardt et al.  
 6,157,850 A 12/2000 Diab et al.  
 6,165,005 A 12/2000 Mills et al.  
 6,184,521 B1 2/2001 Coffin, IV et al.  
 6,206,830 B1 3/2001 Diab et al.  
 6,229,856 B1 5/2001 Diab et al.  
 6,232,609 B1 5/2001 Snyder et al.  
 6,236,872 B1 5/2001 Diab et al.  
 6,241,683 B1 6/2001 Macklem et al.  
 6,253,097 B1 6/2001 Aronow et al.  
 6,256,523 B1 7/2001 Diab et al.  
 6,263,222 B1 7/2001 Diab et al.  
 6,278,522 B1 8/2001 Lepper, Jr. et al.  
 6,280,213 B1 8/2001 Tobler et al.  
 6,285,896 B1 9/2001 Tobler et al.  
 6,301,493 B1 10/2001 Marro et al.  
 6,317,627 B1 11/2001 Ennen et al.  
 6,321,100 B1 11/2001 Parker  
 6,325,761 B1 12/2001 Jay  
 6,334,065 B1 12/2001 Al-Ali et al.  
 6,343,224 B1 1/2002 Parker  
 6,349,228 B1 2/2002 Kiani et al.  
 6,360,114 B1 3/2002 Diab et al.  
 6,368,283 B1 4/2002 Xu et al.  
 6,371,921 B1 4/2002 Caro et al.  
 6,377,829 B1 4/2002 Al-Ali  
 6,388,240 B2 5/2002 Schulz et al.  
 6,397,091 B2 5/2002 Diab et al.  
 6,430,437 B1 8/2002 Marro  
 6,430,525 B1 8/2002 Weber et al.  
 6,463,311 B1 10/2002 Diab  
 6,470,199 B1 10/2002 Kopotic et al.  
 6,501,975 B2 12/2002 Diab et al.  
 6,505,059 B1 1/2003 Kollias et al.  
 6,515,273 B2 2/2003 Al-Ali  
 6,519,487 B1 2/2003 Parker  
 6,525,386 B1 2/2003 Mills et al.  
 6,526,300 B1 2/2003 Kiani et al.  
 6,541,756 B2 4/2003 Schulz et al.  
 6,542,764 B1 4/2003 Al-Ali et al.  
 6,580,086 B1 6/2003 Schulz et al.  
 6,584,336 B1 6/2003 Ali et al.  
 6,595,316 B2 7/2003 Cybulski et al.  
 6,597,932 B2 7/2003 Tian et al.  
 6,597,933 B2 7/2003 Kiani et al.  
 6,606,511 B1 8/2003 Ali et al.  
 6,632,181 B2 10/2003 Flaherty et al.  
 6,639,668 B1 10/2003 Trepagnier  
 6,640,116 B2 10/2003 Diab  
 6,643,530 B2 11/2003 Diab et al.  
 6,648,820 B1 \* 11/2003 Sarel ..... A61B 5/0002  
 128/903  
 6,650,917 B2 11/2003 Diab et al.  
 6,654,624 B2 11/2003 Diab et al.  
 6,658,276 B2 12/2003 Kiani et al.  
 6,661,161 B1 12/2003 Lanzo et al.  
 6,671,531 B2 12/2003 Al-Ali et al.  
 6,678,543 B2 1/2004 Diab et al.  
 6,684,090 B2 1/2004 Ali et al.  
 6,684,091 B2 1/2004 Parker  
 6,697,656 B1 2/2004 Al-Ali  
 6,697,657 B1 2/2004 Shehada et al.  
 6,697,658 B2 2/2004 Al-Ali  
 RE38,476 E 3/2004 Diab et al.  
 6,699,194 B1 3/2004 Diab et al.  
 6,714,804 B2 3/2004 Al-Ali et al.  
 RE38,492 E 4/2004 Diab et al.  
 6,721,582 B2 4/2004 Trepagnier et al.  
 6,721,585 B1 4/2004 Parker  
 6,725,075 B2 4/2004 Al-Ali  
 6,728,560 B2 4/2004 Kollias et al.  
 6,735,459 B2 5/2004 Parker  
 6,745,060 B2 6/2004 Diab et al.  
 6,760,607 B2 7/2004 Al-Ali  
 6,770,028 B1 8/2004 Ali et al.  
 6,771,994 B2 8/2004 Kiani et al.  
 6,792,300 B1 9/2004 Diab et al.  
 6,813,511 B2 11/2004 Diab et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,816,741	B2	11/2004	Diab	7,438,683	B2	10/2008	Al-Ali et al.
6,822,564	B2	11/2004	Al-Ali	7,440,787	B2	10/2008	Diab
6,826,419	B2	11/2004	Diab et al.	7,454,240	B2	11/2008	Diab et al.
6,830,711	B2	12/2004	Mills et al.	7,467,002	B2	12/2008	Weber et al.
6,850,787	B2	2/2005	Weber et al.	7,469,157	B2	12/2008	Diab et al.
6,850,788	B2	2/2005	Al-Ali	7,471,969	B2	12/2008	Diab et al.
6,852,083	B2	2/2005	Caro et al.	7,471,971	B2	12/2008	Diab et al.
6,861,639	B2	3/2005	Al-Ali	7,483,729	B2	1/2009	Al-Ali et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,483,730	B2	1/2009	Diab et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,489,958	B2	2/2009	Diab et al.
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,496,391	B2	2/2009	Diab et al.
6,934,570	B2	8/2005	Kiani et al.	7,496,393	B2	2/2009	Diab et al.
6,939,305	B2	9/2005	Flaherty et al.	D587,657	S	3/2009	Al-Ali et al.
6,943,348	B1	9/2005	Coffin, IV	7,499,741	B2	3/2009	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,499,835	B2	3/2009	Weber et al.
6,961,598	B2	11/2005	Diab	7,500,950	B2	3/2009	Al-Ali et al.
6,970,792	B1	11/2005	Diab	7,509,154	B2	3/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	7,509,494	B2	3/2009	Al-Ali
6,985,764	B2	1/2006	Mason et al.	7,510,849	B2	3/2009	Schurman et al.
6,993,371	B2	1/2006	Kiani et al.	7,526,328	B2	4/2009	Diab et al.
6,996,427	B2	2/2006	Ali et al.	7,530,942	B1	5/2009	Diab
6,999,904	B2	2/2006	Weber et al.	7,530,949	B2	5/2009	Al Ali et al.
7,003,338	B2	2/2006	Weber et al.	7,530,955	B2	5/2009	Diab et al.
7,003,339	B2	2/2006	Diab et al.	7,563,110	B2	7/2009	Al-Ali et al.
7,015,451	B2	3/2006	Dalke et al.	7,596,398	B2	9/2009	Al-Ali et al.
7,024,233	B2	4/2006	Ali et al.	7,618,375	B2	11/2009	Flaherty
7,027,849	B2	4/2006	Al-Ali	D606,659	S	12/2009	Kiani et al.
7,030,749	B2	4/2006	Al-Ali	7,647,083	B2	1/2010	Al-Ali et al.
7,039,449	B2	5/2006	Al-Ali	D609,193	S	2/2010	Al-Ali et al.
7,041,060	B2	5/2006	Flaherty et al.	D614,305	S	4/2010	Al-Ali et al.
7,044,918	B2	5/2006	Diab	RE41,317	E	5/2010	Parker
7,067,893	B2	6/2006	Mills et al.	7,729,733	B2	6/2010	Al-Ali et al.
7,096,052	B2	8/2006	Mason et al.	7,734,320	B2	6/2010	Al-Ali
7,096,054	B2	8/2006	Abdul-Hafiz et al.	7,761,127	B2	7/2010	Al-Ali et al.
7,132,641	B2	11/2006	Schulz et al.	7,761,128	B2	7/2010	Al-Ali et al.
7,142,901	B2	11/2006	Kiani et al.	7,764,982	B2	7/2010	Dalke et al.
7,149,561	B2	12/2006	Diab	D621,516	S	8/2010	Kiani et al.
7,186,966	B2	3/2007	Al-Ali	7,791,155	B2	9/2010	Diab
7,190,261	B2	3/2007	Al-Ali	7,801,581	B2	9/2010	Diab
7,215,984	B2	5/2007	Diab	7,822,452	B2	10/2010	Schurman et al.
7,215,986	B2	5/2007	Diab	RE41,912	E	11/2010	Parker
7,221,971	B2	5/2007	Diab	7,844,313	B2	11/2010	Kiani et al.
7,225,006	B2	5/2007	Al-Ali et al.	7,844,314	B2	11/2010	Al-Ali
7,225,007	B2	5/2007	Al-Ali	7,844,315	B2	11/2010	Al-Ali
RE39,672	E	6/2007	Shehada et al.	7,865,222	B2	1/2011	Weber et al.
7,239,905	B2	7/2007	Kiani-Azarbayjany et al.	7,873,497	B2	1/2011	Weber et al.
7,245,953	B1	7/2007	Parker	7,880,606	B2	2/2011	Al-Ali
7,254,429	B2	8/2007	Schurman et al.	7,880,626	B2	2/2011	Al-Ali et al.
7,254,431	B2	8/2007	Al-Ali	7,891,355	B2	2/2011	Al-Ali et al.
7,254,433	B2	8/2007	Diab et al.	7,894,868	B2	2/2011	Al-Ali et al.
7,254,434	B2	8/2007	Schulz et al.	7,899,507	B2	3/2011	Al-Ali et al.
7,272,425	B2	9/2007	Al-Ali	7,899,518	B2	3/2011	Trepagnier et al.
7,274,955	B2	9/2007	Kiani et al.	7,904,132	B2	3/2011	Weber et al.
D554,263	S	10/2007	Al-Ali	7,909,772	B2	3/2011	Popov et al.
7,280,858	B2	10/2007	Al-Ali et al.	7,910,875	B2	3/2011	Al-Ali
7,289,835	B2	10/2007	Mansfield et al.	7,919,713	B2	4/2011	Al-Ali et al.
7,292,883	B2	11/2007	De Felice et al.	7,937,128	B2	5/2011	Al-Ali
7,295,866	B2	11/2007	Al-Ali	7,937,129	B2	5/2011	Mason et al.
7,328,053	B1	2/2008	Diab et al.	7,937,130	B2	5/2011	Diab et al.
7,332,784	B2	2/2008	Mills et al.	7,941,199	B2	5/2011	Kiani
7,340,287	B2	3/2008	Mason et al.	7,951,086	B2	5/2011	Flaherty et al.
7,341,559	B2	3/2008	Schulz et al.	7,957,780	B2	6/2011	Lamego et al.
7,343,186	B2	3/2008	Lamego et al.	7,962,188	B2	6/2011	Kiani et al.
D566,282	S	4/2008	Al-Ali et al.	7,962,190	B1	6/2011	Diab et al.
7,355,512	B1	4/2008	Al-Ali	7,976,472	B2	7/2011	Kiani
7,356,365	B2	4/2008	Schurman	7,988,637	B2	8/2011	Diab
7,371,981	B2	5/2008	Abdul-Hafiz	7,990,382	B2	8/2011	Kiani
7,373,193	B2	5/2008	Al-Ali et al.	7,991,446	B2	8/2011	Ali et al.
7,373,194	B2	5/2008	Weber et al.	8,000,761	B2	8/2011	Al-Ali
7,376,453	B1	5/2008	Diab et al.	8,008,088	B2	8/2011	Bellott et al.
7,377,794	B2	5/2008	Al Ali et al.	RE42,753	E	9/2011	Kiani-Azarbayjany et al.
7,377,899	B2	5/2008	Weber et al.	8,019,400	B2	9/2011	Diab et al.
7,383,070	B2	6/2008	Diab et al.	8,028,701	B2	10/2011	Al-Ali et al.
7,415,297	B2	8/2008	Al-Ali et al.	8,029,765	B2	10/2011	Bellott et al.
7,428,432	B2	9/2008	Ali et al.	8,036,728	B2	10/2011	Diab et al.
				8,046,040	B2	10/2011	Ali et al.
				8,046,041	B2	10/2011	Diab et al.
				8,046,042	B2	10/2011	Diab et al.
				8,048,040	B2	11/2011	Kiani

(56)

References Cited

U.S. PATENT DOCUMENTS

8,050,728 B2 11/2011 Al-Ali et al.  
 RE43,169 E 2/2012 Parker  
 8,118,620 B2 2/2012 Al-Ali et al.  
 8,126,528 B2 2/2012 Diab et al.  
 8,128,572 B2 3/2012 Diab et al.  
 8,130,105 B2 3/2012 Al-Ali et al.  
 8,145,287 B2 3/2012 Diab et al.  
 8,150,487 B2 4/2012 Diab et al.  
 8,175,672 B2 5/2012 Parker  
 8,180,420 B2 5/2012 Diab et al.  
 8,182,443 B1 5/2012 Kiani  
 8,185,180 B2 5/2012 Diab et al.  
 8,190,223 B2 5/2012 Al-Ali et al.  
 8,190,227 B2 5/2012 Diab et al.  
 8,203,438 B2 6/2012 Kiani et al.  
 8,203,704 B2 6/2012 Merritt et al.  
 8,224,411 B2 7/2012 Al-Ali et al.  
 8,228,181 B2 7/2012 Al-Ali  
 8,229,533 B2 7/2012 Diab et al.  
 8,233,955 B2 7/2012 Al-Ali et al.  
 8,244,325 B2 8/2012 Al-Ali et al.  
 8,255,026 B1 8/2012 Al-Ali  
 8,255,027 B2 8/2012 Al-Ali et al.  
 8,255,028 B2 8/2012 Al-Ali et al.  
 8,260,577 B2 9/2012 Weber et al.  
 8,265,723 B1 9/2012 McHale et al.  
 8,274,360 B2 9/2012 Sampath et al.  
 8,301,217 B2 10/2012 Al-Ali et al.  
 8,310,336 B2 11/2012 Muhsin et al.  
 8,315,683 B2 11/2012 Al-Ali et al.  
 RE43,860 E 12/2012 Parker  
 8,337,403 B2 12/2012 Al-Ali et al.  
 8,346,330 B2 1/2013 Lamego  
 8,353,842 B2 1/2013 Al-Ali et al.  
 8,355,766 B2 1/2013 MacNeish, III et al.  
 8,359,080 B2 1/2013 Diab et al.  
 8,364,223 B2 1/2013 Al-Ali et al.  
 8,364,226 B2 1/2013 Diab et al.  
 8,374,665 B2 2/2013 Lamego  
 8,385,995 B2 2/2013 Al-ali et al.  
 8,385,996 B2 2/2013 Smith et al.  
 8,388,353 B2 3/2013 Kiani et al.  
 8,399,822 B2 3/2013 Al-Ali  
 8,401,602 B2 3/2013 Kiani  
 8,405,608 B2 3/2013 Al-Ali et al.  
 8,414,499 B2 4/2013 Al-Ali et al.  
 8,418,524 B2 4/2013 Al-Ali  
 8,423,106 B2 4/2013 Lamego et al.  
 8,428,967 B2 4/2013 Olsen et al.  
 8,430,817 B1 4/2013 Al-Ali et al.

8,437,825 B2 5/2013 Dalvi et al.  
 8,455,290 B2 6/2013 Siskavich  
 8,457,703 B2 6/2013 Al-Ali  
 8,457,707 B2 6/2013 Kiani  
 8,463,349 B2 6/2013 Diab et al.  
 8,466,286 B2 6/2013 Bellot et al.  
 8,471,713 B2 6/2013 Poeze et al.  
 8,473,020 B2 6/2013 Kiani et al.  
 8,483,787 B2 7/2013 Al-Ali et al.  
 8,489,364 B2 7/2013 Weber et al.  
 8,498,684 B2 7/2013 Weber et al.  
 8,509,867 B2 8/2013 Workman et al.  
 8,515,509 B2 8/2013 Bruinsma et al.  
 8,523,781 B2 9/2013 Al-Ali  
 8,529,301 B2 9/2013 Al-Ali et al.  
 8,532,727 B2 9/2013 Ali et al.  
 8,532,728 B2 9/2013 Diab et al.  
 D692,145 S 10/2013 Al-Ali et al.  
 8,547,209 B2 10/2013 Kiani et al.  
 8,548,548 B2 10/2013 Al-Ali  
 8,548,550 B2 10/2013 Al-Ali et al.  
 8,560,032 B2 10/2013 Al-Ali et al.  
 8,560,034 B1 10/2013 Diab et al.  
 2004/0034289 A1\* 2/2004 Teller ..... A61B 5/02055  
 600/300  
 2005/0228298 A1\* 10/2005 Banet ..... A61B 5/0205  
 600/485  
 2009/0149724 A1\* 6/2009 Mark ..... A61B 5/0205  
 600/301  
 2010/0099964 A1\* 4/2010 O'Reilly ..... A61B 5/14546  
 600/323  
 2010/0217099 A1\* 8/2010 LeBoeuf ..... A61B 5/00  
 600/301  
 2011/0034209 A1 2/2011 Rubinsky et al.  
 2011/0040197 A1\* 2/2011 Welch ..... A61B 5/0205  
 600/509  
 2011/0257489 A1\* 10/2011 Banet ..... A61B 5/0809  
 600/301  
 2013/0144136 A1\* 6/2013 Rymut ..... A61B 5/0059  
 600/310  
 2013/0231947 A1\* 9/2013 Shusterman ..... G06F 19/3443  
 705/2

OTHER PUBLICATIONS

Chung-Ping Young et al., "A portable multi-channel behavioral state and physiological signal monitoring system," May 13, 2012, pp. 2687-2691.  
 International Search Report and Written Opinion issued in International Application No. PCT/US2014/020903 dated Dec. 5, 2014.

\* cited by examiner

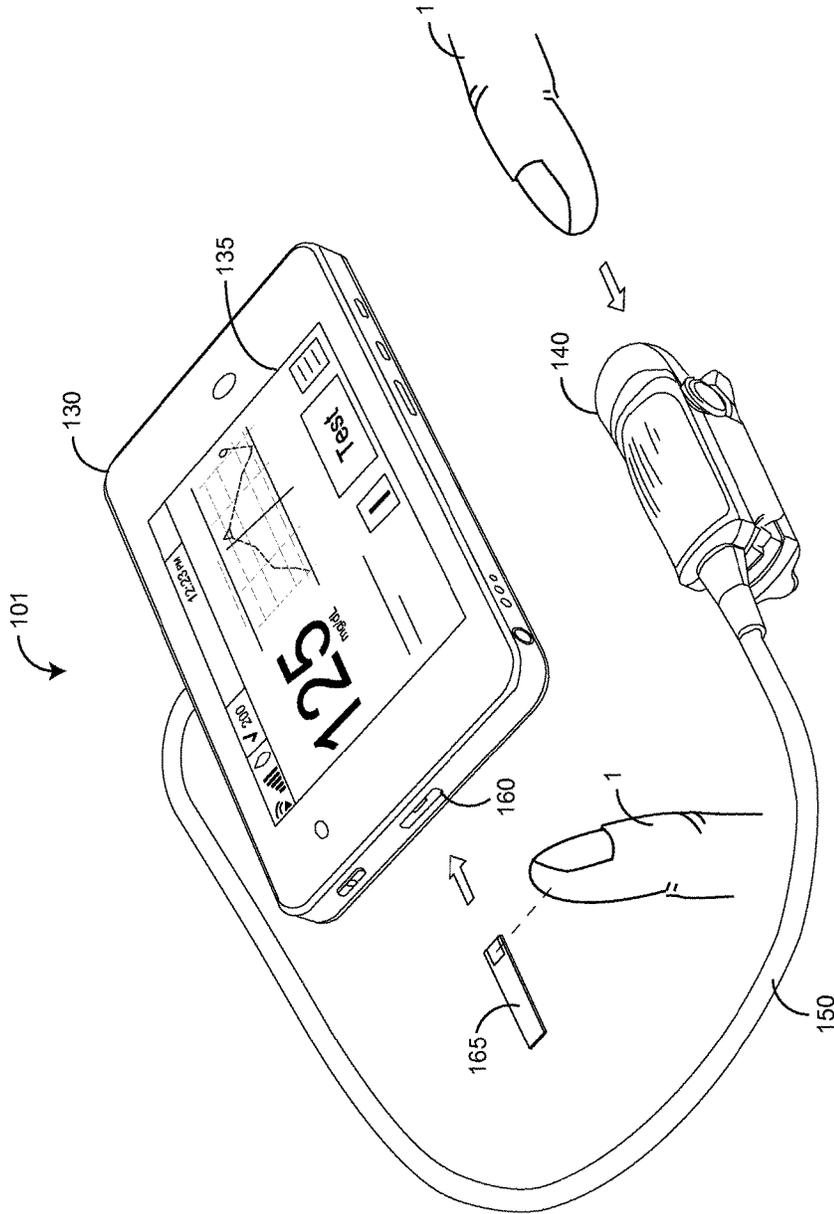


FIG. 1A

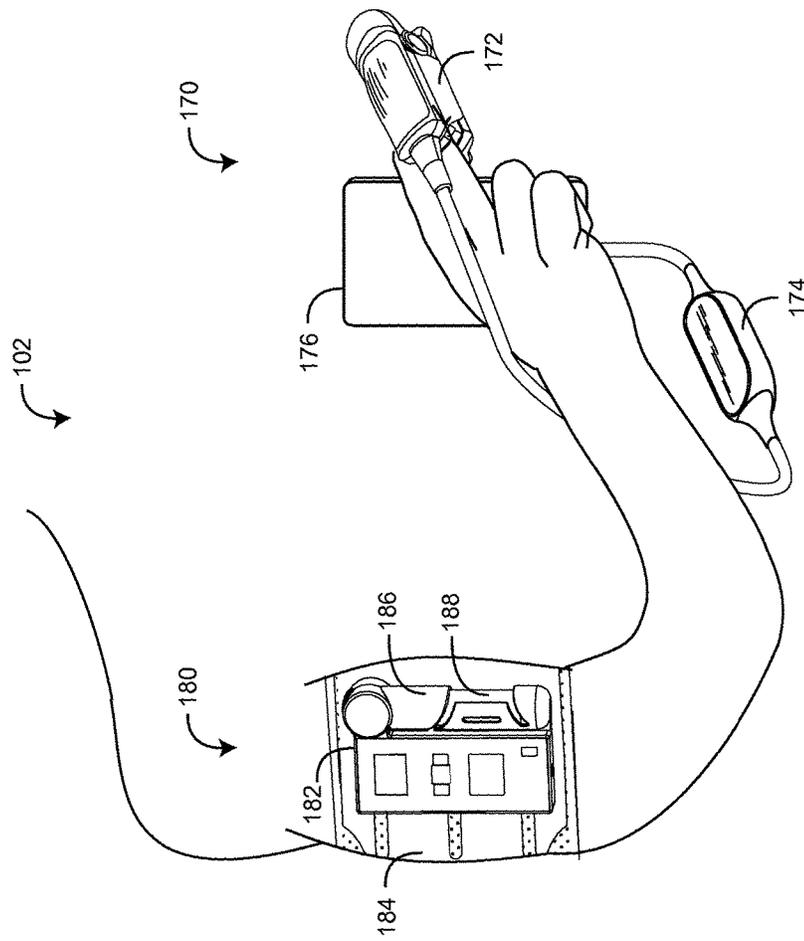


FIG. 1B

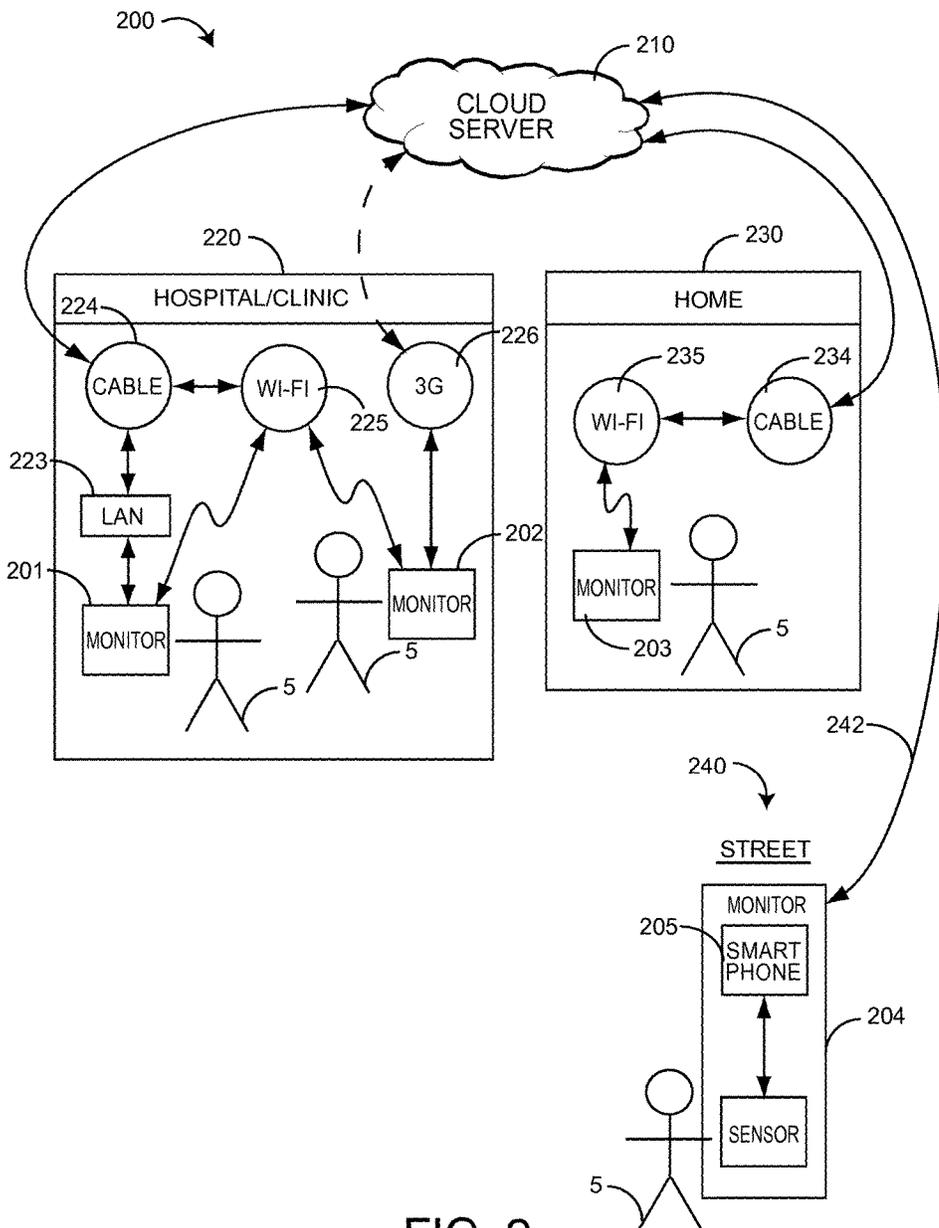


FIG. 2

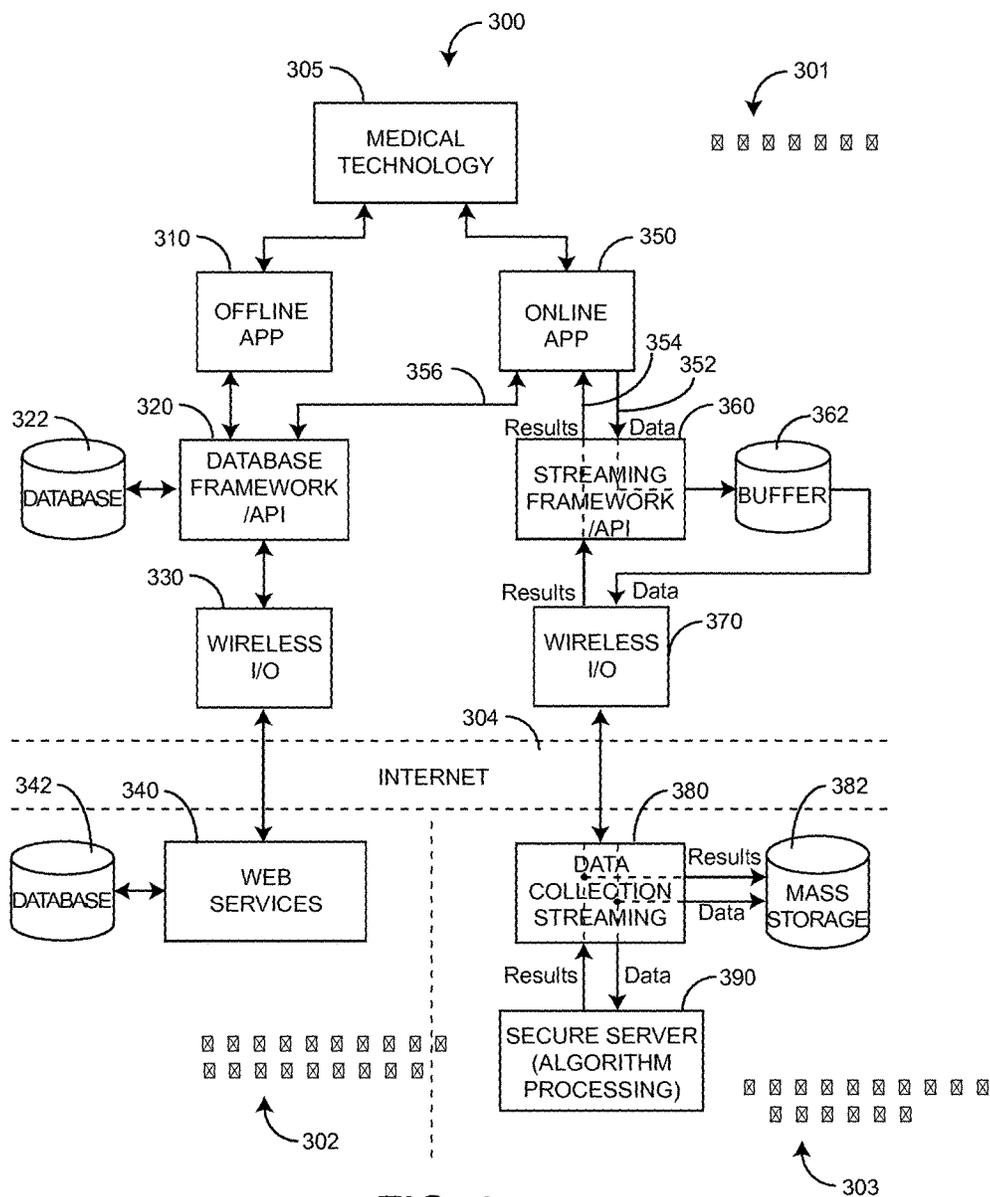


FIG. 3

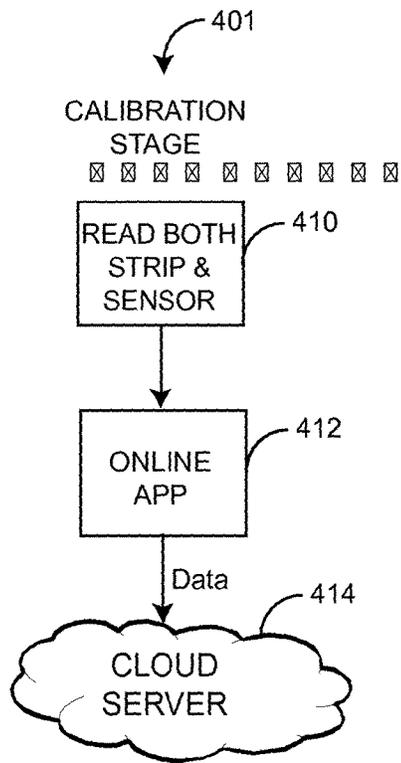


FIG. 4A

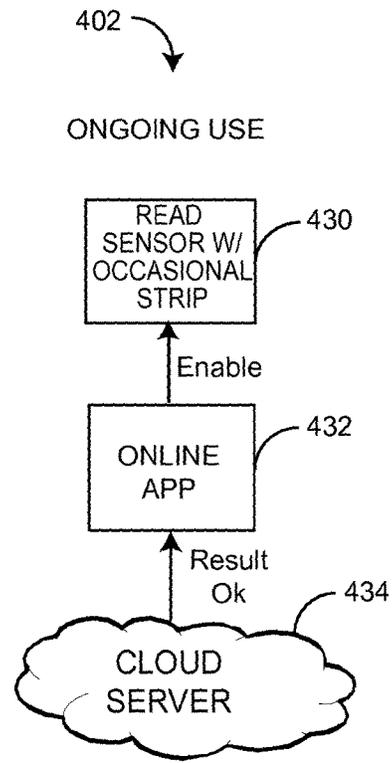


FIG. 4B

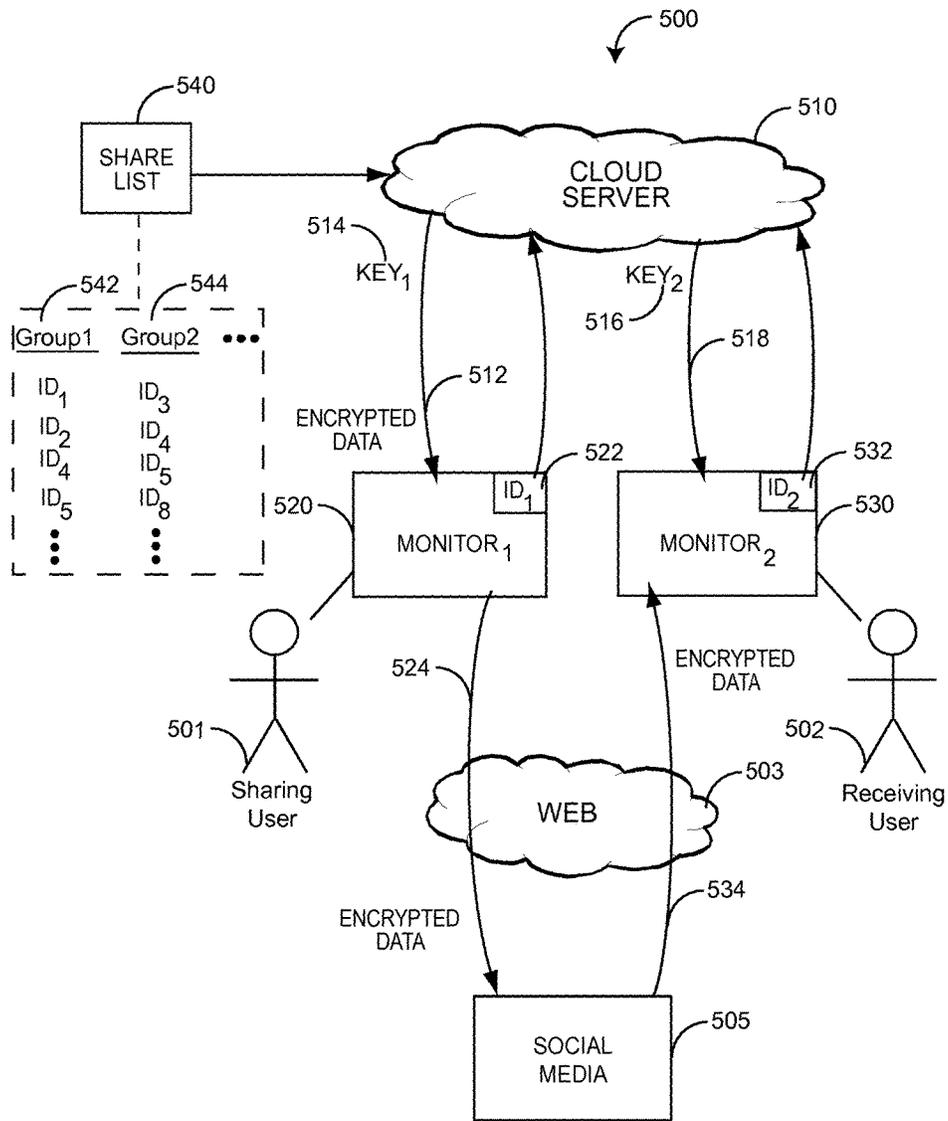


FIG. 5

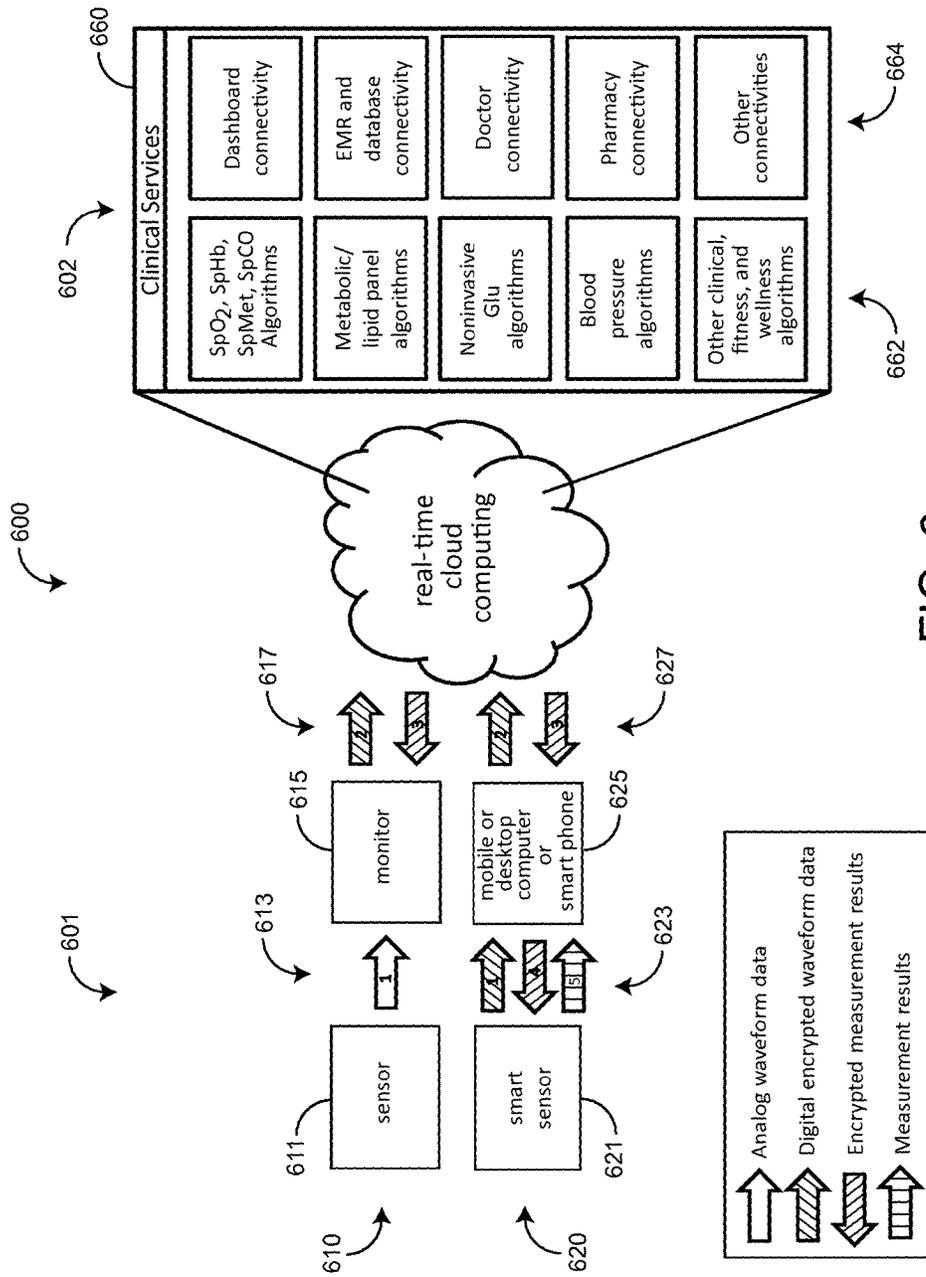


FIG. 6

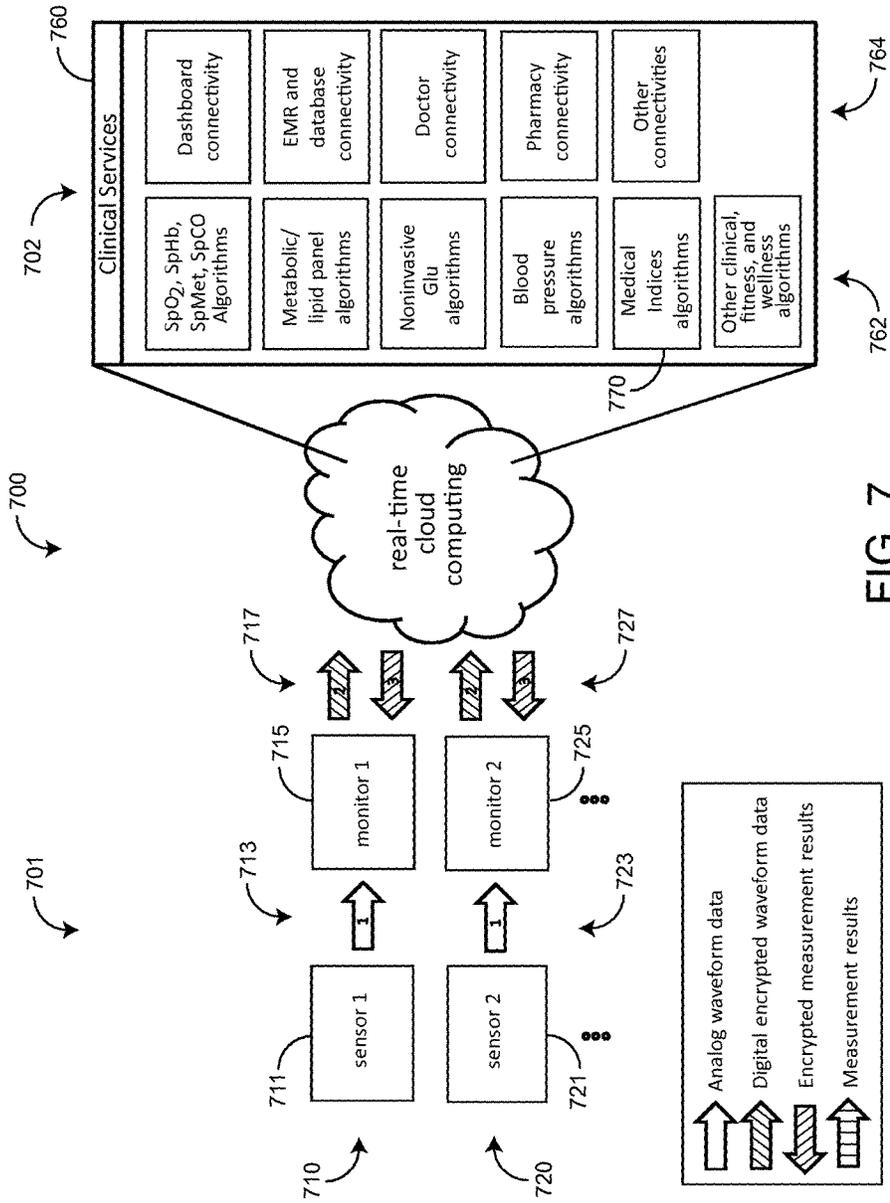


FIG. 7

800

Index	Hgb	BUN	Cr	PVI	BP
Dehydration	↑	↑	↑	↑	↓

810

FIG. 8A

820

Index	Hgb	BUN	Cr	PVI	BP
Renal Insufficiency	↓	↑↑	↑ to ↑↑	↓	↑

FIG. 8B

830

Index	Hgb	BUN	Cr	PVI	BP
Over-hydration	↓	↓	↔	↓	↑

FIG. 8C

800

Index	Hgb	BUN	Cr	PVI	BP
Gastrointestinal Bleeding	↓	↑	↔	↑	↔ to ↓

840

FIG. 8D

850

Index	Hgb	BUN	Cr	PVI	BP
Congestive Heart Failure Exacerbation	↔ to ↓	↔ to ↓	↔ to ↑	↓	↔ to ↑

FIG. 8E

860

Index	Chol	HDL	Chol/HDL	Trig	BP
Cardiovascular Risk	↑	↓	↑	↑	↑

FIG. 8F

	Na+	K+	CO2	Cl-	Glu	Ca	BUN	Cre	ALP	ALT	AST	Tbil
<u>Index</u>												
Diabetic Ketoacidosis	↓	↓, mostly ↓	↓	↓	↑↑	↔ to ↓	↑	↑	↔	↔	↔	↔
Asthma Exacerbation	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
Acute Upper Resp Infection	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
Chronic Renal Insufficiency	↔ to ↓	↑	↓	↔ to ↓	↔ to ↑	↑	↑↑	↑↑	↔	↔	↔	↔
Liver Cirrhosis/Failure	↔ to ↓	↔	↔ to ↓	↔ to ↓	↔ to ↓	↔	↔ to ↓	↔ to ↑	↔ to ↑	↑↑	↑↑	↑
Chronic Hypertension	↔ to ↑	↔ to ↓	↔	↔	↔	↔	↔ to ↑	↔ to ↑	↔	↔	↔	↔
Hyperlipidemia	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔ to ↑	↔ to ↑	↔
Acute cholecystitis	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔ to ↑	↔ to ↑	↔
Evolving MI	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
Dehydration/heat stroke	↑	↔ to ↑	↑	↑	↔	↔	↑↑	↑	↔	↔ to ↑	↔ to ↑	↔ to ↑

	Alb	TP	Chol	HDL	Trig	LDL	VLDL	SpO2	BP	RR	Temp	ECG/HR
Alb	↔	↔	↔	↔	↔	↔	↔	↔ to ↓	↓	↑	↓ or ↑	↑
TP	↔	↔	↔	↔	↑ or ↔	↔	↔	↔ to ↓	↔ to ↑	↑	↔	↑
Chol	↔	↔	↔	↔	↔	↔	↔	↔ to ↓	↔	↑ or ↔	↑	↑ or ↔
HDL	↔	↔	↔	↔	↔	↔	↔	↔	↔	↑ or ↔	↔	↔
Trig	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
LDL	↔	↔	↔	↔	↔ to ↓	↔	↔	↔				
VLDL	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
SpO2	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
BP	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
RR	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
Temp	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔
ECG/HR	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔	↔

↔, may see peaked T waves  
 varied depending on extent of disease  
 LVH, possible evidence of old MI  
 ↔, may see Q waves  
 ↑, ST segment elevation, poor R wave progression

FIG. 9

## CLOUD-BASED PHYSIOLOGICAL MONITORING SYSTEM

### PRIORITY CLAIM AND REFERENCE TO RELATED APPLICATIONS

The present application claims priority benefit under 35 U.S.C. § 119(e) to U.S. Provisional Patent Application Ser. No. 61/801,464, filed Mar. 15, 2013, titled Cloud-Based Blood Glucose Monitoring System; U.S. Provisional Patent Application Ser. No. 61/841,346, filed Jun. 30, 2013, titled Cloud-Based Monitoring System; U.S. Provisional Patent Application Ser. No. 61/885,491, filed Oct. 1, 2013, titled Cloud-Based Monitoring System; and U.S. Provisional Patent Application Ser. No. 61/922,861, filed Jan. 1, 2014, titled Cloud-Based Physiological Index Monitoring System; all of the above-referenced provisional patent applications are hereby incorporated in their entireties by reference herein.

### BACKGROUND OF THE INVENTION

Medical device manufacturers are continually increasing the processing capabilities of physiological monitors that process signals based upon the attenuation of light by a tissue site. In general, such physiological monitoring systems include one or more optical sensors that irradiate a tissue site and one or more photodetectors that detect the optical radiation after attenuation by the tissue site. The sensor communicates the detected signal to a physiological monitor, which removes noise and preprocesses the signal. Advanced signal processors then perform time domain and/or frequency domain processing to determine blood constituents and other physiological parameters.

Manufacturers have advanced basic pulse oximeters from devices that determine measurements for blood oxygen saturation (“SpO<sub>2</sub>”), pulse rate (“PR”) and plethysmographic information to read-through-motion oximeters and to co-oximeters that determine measurements of many constituents of circulating blood. For example, Masimo Corporation of Irvine Calif. (“Masimo”) manufactures pulse oximetry systems including Masimo SET® low noise optical sensors and read through motion pulse oximetry monitors for measuring SpO<sub>2</sub>, pulse rate (PR) and perfusion index (PI). Masimo optical sensors include any of Masimo LNOP®, LNCS®, SofTouch™ and Blue™ adhesive or reusable sensors. Masimo pulse oximetry monitors include any of Masimo Rad-8®, Rad-5®, Rad®-5v or SatShare® monitors. Such advanced pulse oximeters and low noise sensors have gained rapid acceptance in a wide variety of medical applications, including surgical wards, intensive care and neonatal units, general wards, home care, physical training and virtually all types of monitoring scenarios.

Many innovations improving the measurement of blood constituents are described in at least U.S. Pat. Nos. 6,770, 028; 6,658,276; 6,157,850; 6,002,952; 5,769,785 and 5,758, 644, which are assigned to Masimo and are incorporated in their entireties by reference herein. Corresponding low noise optical sensors are disclosed in at least U.S. Pat. Nos. 6,985,764; 6,088,607; 5,782,757 and 5,638,818, assigned to Masimo and hereby incorporated in their entireties by reference herein.

Advanced blood parameter measurement systems include Masimo Rainbow® SET, which provides measurements in addition to SpO<sub>2</sub>, such as total hemoglobin (SpHb™), oxygen content (SpOC™), methemoglobin (SpMet®), carboxyhemoglobin (SpCO®) and PVI®. Advanced blood parameter sensors include Masimo Rainbow® adhesive,

ReSpasable™ and reusable sensors. Advanced blood parameter monitors include Masimo Radical-7™, Rad-8™ and Rad-5™ monitors, all available from Masimo. Advanced blood parameter monitors further include Masimo Rainbow 4D™ DC sensors and Masimo Pronto® and Pronto-7® monitors for noninvasive and quick spot checking of total hemoglobin (SpHb®, SpO<sub>2</sub>, pulse rate and perfusion index).

Advanced parameter measurement systems may also include acoustic monitoring such as acoustic respiration rate (RRa™) using a Rainbow Acoustic Sensor™ and Rad-8™ monitor, available from Masimo. An advanced parameter measurement system that includes acoustic monitoring is described in U.S. Pat. Pub. No. 2010/0274099, filed Dec. 21, 2009, titled Acoustic Sensor Assembly, assigned to Masimo and incorporated in its entirety by reference herein.

Innovations relating to other advanced blood parameter measurement systems are described in at least U.S. Pat. No. 7,647,083, filed Mar. 1, 2006, titled Multiple Wavelength Sensor Equalization; U.S. Pat. No. 7,729,733, filed Mar. 1, 2006, titled Configurable Physiological Measurement System; U.S. Pat. Pub. No. 2006/0211925, filed Mar. 1, 2006, titled Physiological Parameter Confidence Measure and U.S. Pat. Pub. No. 2006/0238358, filed Mar. 1, 2006, titled Noninvasive Multi-Parameter Patient Monitor, all assigned to Cercacor Laboratories, Inc., Irvine, Calif. (Cercacor) and all incorporated in their entireties by reference herein.

### SUMMARY OF THE INVENTION

One aspect of a cloud-based physiological monitoring system is a sensor in communications with a living being so as to generate a data stream generally responsive to a physiological condition of the living being. A monitor receives the data stream from the sensor and transmits the data stream to a cloud server. The cloud server processes the data stream so as to derive parameters having values responsive to the physiological condition. The cloud server derives a medical index based upon a combination of the parameters. The cloud server communicates the medical index to the physiological monitor and the physiological monitor displays the medical index.

In an embodiment, the cloud-based physiological monitoring system sensor comprises an optical sensor and the parameters comprise a blood constituent parameter. The parameters comprise a plethysmograph waveform parameter. A blood pressure sensor is in communications with the living being, and a blood pressure monitor receives a blood pressure data stream from the blood pressure sensor and transmits the blood pressure data stream to the cloud server. The cloud server processes the blood pressure data stream so as to derive a blood pressure parameter having a blood pressure value responsive to the physiological condition and the parameters further comprise the blood pressure parameter.

In various other embodiments, the medical index is based upon trends of the combination of the parameters. The blood constituents include Hgb, BUN and Cr. The medical index relates to at least one of hydration, cardiovascular risk and renal insufficiency. In a particular embodiment, the medical index relates to at least one of dehydration, over hydration, gastrointestinal bleeding and congestive heart failure exacerbation.

Another aspect of a cloud-based physiological monitoring system comprises generating sensor data generally responsive to a physiological phenomenon of a living being, communicating the sensor data to a local medical device and transmitting the sensor data from the local medical device to

a remote cloud server. The system further comprises processing the sensor data at the cloud server so as to derive parameters having values responsive to the physiological phenomenon and trending the parameters at the cloud server so as to derive a medical index responsive to the parameters, where the medical index indicates a medical condition. The system additionally comprises communicating the medical index to the local medical device and displaying the medical index on the local medical device.

In various embodiments, cloud-based physiological monitoring system comprises generating second sensor data generally responsive to a second physiological phenomenon of a living being, communicating the second sensor data to a second local medical device and transmitting the second sensor data from the second local medical device to the remote cloud server. The system further comprises processing the second sensor data at the cloud server so as to derive a second parameter having values responsive to the second physiological phenomenon and trending the second parameter with at least one of the parameters at the cloud server so as to improve the efficacy of the medical index. In various other embodiments, generating sensor data comprises optically-deriving data responsive to pulsatile blood flow. Generating second sensor data comprises air-cuff-deriving data responsive to blood pressure. The system further comprises time frame matching the sensor data and the second sensor data at the cloud server. In a particular embodiment, displaying the medical index comprises indicating hydration on a smart cellular telephone.

A further aspect of a cloud-based physiological monitoring system comprises a physiological monitor in remote communications with a cloud server, where the physiological monitor inputs sensor data responsive to a physiological condition of a user. The cloud server is in remote communications with the physiological monitor so as to upload the sensor data. The cloud server executes signal processing algorithms so as to derive a physiological parameter from the sensor data. The cloud server downloads the physiological parameter to the physiological monitor for display to user.

In various embodiments, the physiological monitor has an online application that executes if the cloud server is available and, if so, the online application inputs sensor data from a physiological sensor in communications with the physiological monitor, transmits the sensor data to the cloud server, receives a parameter value that the cloud server derives from the sensor data and displays the parameter value on the physiological monitor. The physiological monitor has an offline application that executes if the cloud server is unavailable and, if so, the offline application inputs sensor data from a physiological sensor in communications with the physiological monitor, calculates a parameter value from the sensor data and displays the parameter value on the physiological monitor.

In various further embodiments, the online application performs an initial blood glucose calibration phase of the physiological monitor that comprises repeated blood sample data derived from a strip reader over an initial calibration period of several weeks and repeated optical sensor data corresponding to the blood sample data. The blood sample data and the sensor data are transmitted to the cloud server and the cloud server correlates the blood sample data and the sensor data during the initial calibration stage. The online application further performs an end blood glucose calibration phase of the physiological monitor that comprises optical sensor data occasionally interspersed with blood

sample data. The sensor data and occasional blood sample data are transmitted to the cloud server, which updates the calibration as needed.

In additional embodiments, a share user establishes a receive user who is allowed to view the share user's medical information. A share ID is associated with the share user's physiological monitor. A receive ID is associated with the receive user's physiological monitor. The cloud server associates the share ID with the receive ID. The cloud server encrypts the share user's medical information according to a share key based upon the share ID. The cloud server generates a decryption key based upon the receive ID. The cloud server transmits the encrypted medical information and share key to the share user. The cloud server transmits the receive key to the receive user. The share user posts the encrypted medical information to a public website, the receive user downloads the encrypted medical information and the receive user decrypts the medical information using the receive key.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A-B are perspective views of cloud-based monitoring systems that are capable of blood parameter and blood pressure monitoring;

FIG. 2 is a general flow diagram of a cloud-based monitoring system;

FIG. 3 is a detailed block diagram of a cloud-based monitoring system;

FIGS. 4A-B are general flow diagrams of blood glucose calibration;

FIG. 5 is a general flow diagram of a cloud-based, protected social network for sharing monitoring measurements;

FIG. 6 is a general flow diagram of real-time algorithm processing using one or more of a sensor and connected medical device or a smart sensor and connected mobile or desktop device in communications with a cloud service so as to perform clinical services including physiological parameter calculations;

FIG. 7 is a general flow diagram of real-time algorithm processing using multiple sensors and connected medical devices in communications with a cloud service so as to perform clinical services including calculations of medical indices;

FIG. 8A-F are medical index tables illustrating trends in blood-related parameters, plethysmograph waveform features and blood pressure that are indicative of dehydration, renal insufficiency, over-hydration, gastrointestinal bleeding, congestive heart failure exacerbation and cardiovascular risk, respectively.

FIG. 9 is a comprehensive medical index table illustrating trends in various physiological measurements, including blood-constituents and oxygen saturation, blood pressure, respiration rate (RR), temperature and heart-related parameters including heart rate (HR) and electrocardiogram (ECG) waveform features indicative of various physiological conditions, maladies and diseases.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

FIGS. 1A-B illustrate cloud-based physiological monitoring systems that are capable of blood parameter, blood pressure and other physiological measurements. As shown in FIG. 1A, a physiological monitoring system 101 advantageously provides spot check measurements of various

blood constituents, such as blood glucose. The monitoring system **101** has a blood parameter monitor **130**, an optical sensor **140**, a sensor cable **150** electrically and mechanically interconnecting the monitor **130** and sensor **140** and a monitor-integrated test strip reader **160** that accepts test strips **165** via a test strip slot. In a particular use, the monitoring system **101** provides relatively frequent noninvasive measurements of blood glucose interspersed with relatively infrequent invasive measurements of blood glucose so as to manage individual blood glucose levels. The monitoring system **101** individually calibrates the sensor **140** measurements with intermittent test strip measurements to advantageously provide the accuracy of individualized glucose test strip measurements at a much-reduced frequency of blood draws. Reduced blood draws are a substantial aid to persons who require frequent monitoring of blood glucose levels to manage diabetes and related diseases. In an embodiment, the monitor **130** has a handheld-tablet housing including an integrated 5.6 in IPS touch screen **135** defining one or more input keys and providing a display of blood glucose levels among other features. The monitor **130** advantageously has Wi-Fi and 3G cellular communications for cabled and wireless cloud access. Cloud connectivity allows remote sensor data processing, algorithm development, individual blood glucose calibration and software updates among other cloud services. A blood parameter monitoring system is described with respect to U.S. patent application Ser. No. 13/646,659, filed Oct. 5, 2012, titled Noninvasive Blood Analysis System and U.S. patent application Ser. No. 13/726,539, filed Dec. 24, 2012, titled Blood

Glucose Calibration System, both assigned to Cercacor and both incorporated in their entireties by reference herein. As shown in FIG. 1B, a physiological monitoring system **102** may have two or more monitors **170**, **180** in sensor communications with an individual person so as to generate multiple sensor data streams and display multiple types of physiological parameters. In an embodiment, the multiple monitors **102** include a handheld blood parameter monitor **170** and an arm cuff-mounted blood pressure monitor **180**. In an embodiment, the handheld blood parameter monitor **170** has an optical sensor **172**, a monitor module **174** and a handheld smart cellular telephone (“smart phone”) **176**. An optical sensor is described above with respect to FIG. 1A. The optical sensor attaches to a fleshy tissue site, such as a fingertip. The monitor module **174** drives LEDs in the optical sensor **172** and receives detector signals responsive to the LED emitted light after attenuation by the fleshy tissue and blood flow within the fleshy tissue. The blood flow may be active-pulsed and arterial-pulse blood flow. The monitor module **174** receives the detector signals, i.e. the raw sensor data stream and derives physiological parameters, which are communicated to the smart phone **176**. This alleviates the smart phone **176** from the computationally-intense task of processing raw sensor data and deriving physiological parameters, which the current generation of smart phones are ill-equipped to perform. A combination optical sensor, monitor module and smart phone configured as a mobile physiological monitor are described in U.S. patent application Ser. No. 14/033,315, titled Physiological Monitor with Mobile Computing Device Connectivity, assigned to Cercacor and incorporated in its entirety by reference herein.

Also shown in FIG. 1B, in an embodiment, a cuff-mounted, blood pressure monitor **180** is attached to a person’s limb so as to measure blood pressure parameters. The blood pressure monitor **180** has a monitor module **182**, an inflatable cuff **184** and a gas chamber **186**. The monitor module **182** is mounted to the inflatable cuff **184**, is battery-

operated and includes a display and a user interface. In an embodiment, the gas chamber **186** is configured for disposable CO<sub>2</sub> cartridges **188** in communications with a monitor-controlled gas valve for automatic cuff inflation. Also shown in FIG. 1B, the blood pressure monitor **180** has an OLED display, a 16 g CO<sub>2</sub> canister **188** for automatic cuff information, and Bluetooth and USB communication interfaces. Sensor capabilities include systolic and diastolic blood pressure parameters, pulse rate and mean arterial pressure (MAP). The blood pressure monitor **180** also has cloud communications capabilities either directly via a wireless wide area communications link or via local area communications (e.g. Wi-Fi, Bluetooth) with other devices that have such a wide area link, such as the smart phone **176**. A cuff-mounted monitor is described in detail in U.S. patent application Ser. No. 13/838,225, filed Mar. 15, 2013, titled Patient Monitoring System, assigned to Cercacor and incorporated in its entirety by reference herein. These cloud-based physiological monitors **101-102** (FIGS. 1A-B) advantageously provide measurement capabilities for more than a dozen different noninvasive parameters in addition to cloud services including clinical data visualization, storage and exchange and real-time algorithm processing.

Further shown in FIG. 1B, a multiple-monitor configuration **102** can advantageously derive multiple sensor **170**, **180** data streams and multiple physiological parameters from the same individual and communicate these data streams and parameters to the cloud, as described in further detail with respect to FIGS. 2-7, below. This advantageously allows a cloud-based processor to receive two or more independent sensor data streams, for example data from a blood pressure sensor and an optical sensor attached to an individual, and derive cross-sensor parameters such as the medical indices described below. Such cross-sensor parameters allow caregivers to assess a broader spectrum of physiological conditions from states and trends in these cross-sensor parameters than possible with a data stream from a single sensor.

Although a multiple-monitor configuration **102** is described above with respect to a blood pressure sensor and an optical sensor, each in communications with their individual monitors, in other embodiments, multiple sensors may be in communications with a single monitor. These sensors may include a variety of devices including accelerometers for data regarding body position and activity; body and environment temperature sensors; electrical sensors for deriving EEG, EKG data streams; acoustic sensors for detecting respiration and other body sounds; and capnography sensors for monitoring carbon dioxide, among others.

Additionally shown in FIG. 1B, in an embodiment, individual monitors **170**, **180** may each communicate directly to the cloud utilizing wide area communications, such as wired or wireless Internet or cellular network devices. In an embodiment, a first monitor **170** may have wide area communications capability, and a second monitor **180** may use local area communications to communicate its sensor data to the first monitor **170** for transmission to a cloud-based processor. In another embodiment, first **170** and second **180** monitors may each use local area communications to communicate sensor data to a local processing device, such as a laptop or desktop computer that, in turn, uses wide area communications to communicate with a cloud-based processor. Various monitor-cloud data communications and processing scenarios are further described with respect to FIGS. 2-7, below.

FIG. 2 illustrates a cloud-based monitoring system **200** having a cloud server **210** in communications with physi-

ological monitors **201-204**, such as described with respect to FIGS. **1A-B**, above. The monitors **201-204** are located in various hospital/clinic **220**, home **230** and street **240** locations remote from the cloud server **210**. In an embodiment, the cloud server **210** utilizes various sensor signal processing algorithms to estimate physiological parameters such as blood oxygen saturation, carboxyhemoglobin, methemoglobin, blood glucose, total hemoglobin and respiration rate, to name just a few. These parameters are derived from sensor data collected by the monitors **201-204** and transmitted to the cloud server **210** via various data transmission paths.

As shown in FIG. **2**, data is transmitted from monitors **201-204** to the cloud server **210** via wired (e.g. LAN **223**) or wireless (e.g. Wi-Fi **225**) local networks to wide area media, such as Internet cable **224** or telecommunications (e.g. 3G **226**) networks. Alternatively, a monitor **204** may have a wireless link **242** for direct data transmission to the cloud over a cellular network. These wide area media, in turn, are in communications with the cloud server **210**, which calculates physiological parameters as described above. The calculated parameters are transmitted back to the monitors **201-204** or smart phone **205** for display, additional processing and storage of physiological parameters as well as corresponding notification and use by patients and their care providers.

Further shown in FIG. **2**, the above-described configurations allow all monitors **201-204** to benefit from the same set of signal processing algorithms residing in the cloud server **210**. At the same time, these signal processing algorithms can remain proprietary and protected from reverse engineering in the event any monitors **201-204** are lost or stolen, as the monitors **201-204** do not have access to the cloud algorithms. In particular, the monitors **201-204** only have access to raw (sensor) data, error messages and data pre-processing (e.g. for probe-off detection). In other embodiments, non-proprietary signal processing algorithms are resident in the monitors **201-204** and proprietary algorithms are resident in the cloud **210**. In an embodiment, a dual communications channel between one or more monitors **201-204** and the cloud **210** may be implemented for redundancy, so as to resolve safety issues related to critical medical information and potential communication or monitor malfunctions. For example, a direct 3G (telecommunications) link between a monitor **201-204** and the cloud server **210** may be available as backup to landline communications.

FIG. **3** illustrates a cloud-based physiological monitoring system **300** including a monitor **301**, a monitoring community **302** and a monitoring center **303**. A monitor **301** is in communications with one or more sensors, as described with respect to FIGS. **1A-B**, above. In an embodiment, the monitor **301** includes medical technology **305** in addition to non-medical computer and telecommunication functions such as are available on any of various mobile consumer devices (not shown). Medical technology **305** includes both an offline application **310** and an online application **350** for measuring and managing blood glucose, blood pressure and other physiological parameters and medical indices.

As shown in FIG. **3**, following successful calibration, the offline application **310** allows a patient to attach a sensor, e.g. **140** (FIG. **1A**), push a monitor button, e.g. "Test," and initiate a sampling of sensor data and derivation of physiological parameters, such as blood glucose, utilizing resident processors and algorithms. The monitor **301** then displays the resulting physiological parameter value on a monitor display, e.g. **135** (FIG. **1A**). The only "cloud" function the offline app **310** performs is to occasionally dump patient

data, including derived physiological parameters and related information, from its database **322** to, say, a treating physician's database **342**, so that the physician can monitor and review the patient's disease management and insure that the monitor and sensor are functioning normally. This feature also allows a patient to share their medical information with other members of the monitoring community **302**, including family members or non-related persons having similar treatments and therapies, as described with respect to FIG. **5**, below.

Also shown in FIG. **3**, an online application **350** advantageously transmits the monitor **301** sensor data via the cloud (e.g. Internet **304**) to the monitoring center **303**, which is remote from the monitor **301** location. Physiological parameter processing algorithms reside in a secure server **390**, which derives blood glucose values, other blood constituent values and measurements of other physiological parameters, such as blood pressure, with very small latency times. A data buffer **362** in the monitor **301** reduces transmit data latency times. The calculated physiological parameter results are immediately returned to the monitor **301** for display.

Further shown in FIG. **3**, the monitoring center **303**, which is accessed via the online application **350**, has more processing power and is easier to maintain than the offline application **310**. In particular, algorithm **390** modifications and upgrades can be made simply and quickly at the monitoring center **303** site as compared to upgrades across many monitors **301** distributed over disparate locations. Further, the monitoring center **303** processors have significantly greater computational capabilities than the relatively limited processors residing in each monitor **301**. Also, algorithms developed at the monitor manufacturer's facility typically have to be reduced in size and ported to a different programming language for installation in each monitor **301**, which requires speed and memory size tradeoffs that are nonexistent at the monitoring center **303**. In addition, the processor intensive computations required for offline applications raise heat dissipation issues for relatively compact handheld and tablet monitors. The downside of the monitoring center **303** is the necessity of reliable connectivity to all of the monitors **301**.

According to the trade-offs described above, in a particularly advantageous embodiment, the online application **350** is utilized for cloud computing of all physiological parameters or at least the most computationally intense parameters unless cloud access is temporarily unavailable. In the event the monitoring center **303** processors are down or the online application **350** communications link with the monitoring center **303** is lost, then the offline application **310** performs the necessary computations. This can be done in an emergency for a few minutes without concern about monitor **301** heat dissipation limitations. Further, for blood glucose measurements, loss of cloud access is mitigated somewhat by the device strip reader **160** (FIG. **1A**), which is always available to users in the event the monitoring center **303** is "down" or when a particular monitor **301** has no cloud access.

In a particularly advantageous blood glucose management embodiment, the offline application **310** has a setting for the maximum time allowed between invasive (test strip) measurements of blood glucose. The offline application **310** tracks the time that has elapsed since the last test strip measurement was made and disables noninvasive blood glucose monitoring if that elapsed time limit is exceeded. In an embodiment, the offline application **310** provides a user one or more warning messages of an impending noninvasive measurement timeout due to an excessive elapsed time from

the last invasive measurement. In an embodiment, either the offline application **350** or the online application **310** may adjust the maximum time allowed between invasive measurements as a function of the delta time and the delta blood glucose values between two consecutive invasive measurements. This maximum elapsed time adjustment advantageously takes into account relatively small changes, historically, in invasive glucose values over relatively long time spans so as to lengthen the maximum-allowed elapsed time between invasive measurements. Likewise, the maximum elapsed time adjustment takes into account relatively large changes, historically, in invasive glucose values over relatively short time spans so as to shorten the maximum-allowed elapsed time between invasive measurements.

FIGS. 4A-B illustrate a blood parameter calibration process **401-402** that includes set-up and calibration functions for a cloud-based physiological monitor, such as described with respect to FIGS. 1-3, above. FIG. 4A illustrates an initial calibration stage **401** when a new user attempts to calibrate their monitoring system, e.g. **101** (FIG. 1A) using a strip reader **160** and test strip **165** (FIG. 1A). At regular intervals, blood samples are read with a strip at the same time that optical sensor **140** (FIG. 11) data is taken **410**. An online application **412** sends the strip and sensor data to a cloud server **414**. See, e.g., **303, 350** (FIG. 3). The strip readings are then compared to calculations based upon optical sensor **140** (FIG. 1A) measurements. If there are consistent matches between the invasive and noninvasive measurements, the calibration stage **401** is complete. If not, the calibration stage **401** continues. This process may take 1 to 6 weeks and, in some cases, may not be successful. That is, after some predetermined number of measurements or calibration time interval, the strip readings may not correlate with the optical sensor-based measurements. As a result, that particular individual is deemed not suitable for noninvasive glucose monitoring. FIG. 4B illustrates an ongoing use **402** once the user is initially calibrated **401**. The cloud server **434** indicates to the online application **432** that the user is calibrated **401**. The monitoring system **101** (FIG. 1A) is enabled accordingly **430** to use sensor-based measurements with occasional strip measurements to insure up-to-date calibration. This calibration process **401, 402** is particularly advantageous with respect to calibrating a cloud-based physiological monitor for noninvasive (optical sensor) blood glucose measurements interleaved with occasional invasive (glucose test strip) measurements.

FIG. 5 illustrates a cloud-based, secure social network **500** that enables a monitor **101-102** (FIGS. 1A-B) user to confidentially share their medical information with a trusted group of other users. Medical information may include measured physiological parameters and a user's health management experiences. For example, medical information may be a past history of blood glucose measurements; steps taken to control blood glucose, including medication, diet and exercise; and recent blood glucose measurement results. The social media **505** for sharing this medical information may be any of the popular social media sites, such as Facebook or Google+, to name a few. The protected social network **500** incorporates cloud-based monitors **520, 530** in communications with a cloud server **510**, as described with respect to FIGS. 1-4, above.

As shown in FIG. 5, each sharing user **501** communicates with the cloud server **510** so as to establish a share list **540** of one or more groups **542, 544** of receiving users **502** who are allowed to view the sharing user's medical information. Receiving user groups **542, 544** may be based upon, or restricted by, the type and scope of medical information

shared. Each user **501, 502** is advantageously identified according to their monitor device ID **522, 532**, which is securely registered with the cloud server **510**. That is, one advantage of a cloud-based secure social network **500** is that only individuals assigned a monitor **520, 530** can belong, and membership in and use of the protected social network **500** is enforced by the cloud server **510** and its recognition of monitor IDs **522, 532**. Accordingly, a sharing user's share list **540** securely establishes monitors **530** that receive monitoring data and other personal information regarding the sharing user **501**.

Also shown in FIG. 5, the cloud server **510** advantageously manages encryption of share data according to the sharing user **501** and their share list **540**. The cloud server **510** collects and stores monitoring device **520** data and calculates and stores corresponding measurement results, which may include share data. The cloud server **510** encrypts share data **512**, which is transmitted from the cloud to the sharing user's monitor **520**. A corresponding KEY<sub>1</sub> **514** based upon the sharing user's monitoring device ID<sub>1</sub> **522** is also transmitted to the sharing user's device **520**. This allows the sharing user **501** to decrypt and view share data. A separate KEY<sub>2</sub> **516** is transmitted to a monitor **530** corresponding to a receiving user **502** listed on the share list **542**. The cloud server **510** generates KEY<sub>2</sub> **516** according to the receiving user's device ID<sub>2</sub> **532**.

Further shown in FIG. 5, the sharing user **501** can post the encrypted share data **524**, at their discretion, to social media **505** of their choosing. A receiving user **502**, at their discretion, can upload the encrypted data **534** and use their device specific KEY<sub>2</sub> **516** to decrypt and view the share data. Advantageously, the cloud server **510** in this secure data sharing architecture does not require a customized data sharing website and the corresponding setup and site management burdens. Cloud server **510** overhead is limited to share list **540** management, data encryption and key generation and encrypted data and key distribution based upon an existing network of monitors **520, 530** with registered and readable device IDs **522, 532**.

FIG. 6 illustrates a real-time cloud computing architecture **600**. On a user side **601**, various physiological monitoring systems **610, 620** exist in perhaps widespread geographical locations and disparate environments. In contrast, a centralized cloud server **602** provides a variety of clinical services **660** for these monitoring systems **610, 620**. In an embodiment, various users each possess a physiological monitoring system **610** having a sensor **611** and a corresponding monitor **615**, such as described with respect to FIG. 1A, above. The sensor **611** generates an analog data stream **613** responsive to at least some aspect of the user's physiology. The monitor **615** receives and processes the analog data stream **613** and generates an digital encrypted data stream **617** responsive to the sensor **611**. For example, the data stream **617** may be optical sensor data that has been filtered, digitized, amplified, demodulated and decimated in the monitor **615** and then encrypted and transmitted to the cloud server **602**.

As shown in FIG. 6, in an embodiment, various other users each possess a physiological monitoring system **620** having a smart sensor **621** and a corresponding smart phone **625**, such as described with respect to FIG. 1B, above. (A mobile or desktop computer **625** may be used in lieu of a smart phone). The smart sensor **621** generates an analog data stream **613** responsive to at least some aspect of a user's physiology. A monitor module integral to the smart sensor **621** receives and processes the analog data stream and generates a digital encrypted data stream **623** responsive to

the analog data stream. The smart phone **625** receives the digital encrypted data stream **623** and transmits it directly to the cloud server **602**.

Also shown in FIG. 6, clinical services performed in the cloud **602** include algorithm computations **662** and connectivity **664**. Algorithms **662** include those for calculating SpO<sub>2</sub>, SpHb, SpMet and SpCO; metabolic and lipid parameters; noninvasive blood glucose parameters; blood pressure parameters and other clinical, fitness and wellness-related parameters. Connectivity **664** includes dashboard, EMR and database, doctor and pharmacy connectivities. The cloud **602** returns encrypted measurement results **627** to the monitor **615** or the smart phone **625**. The smart phone **625** passes the encrypted measurement results **623** to the smart sensor **621**, and the smart sensor **621** sends the (decrypted) measurement results **623** back to the smart phone **625**.

The advantages of real-time medical parameter computing via the cloud **602** is flexibility, scalability and ease of maintenance of the algorithm portfolio. In addition, the cloud offers significant IP protection for these algorithms because algorithms are not calculated within a device exposed to hands-on reverse engineering. The disadvantages are that medical parameter cloud computing requires highly reliable connectivity combined with patient risk mitigation if such connectivity is lost.

FIG. 7 illustrates another real-time cloud-computing architecture **700**. In particular, multiple sensors **711**, **721** in conjunction with corresponding monitors **715**, **725**, such as described with respect to FIGS. 1A-B, above, provide clinical services **760** via real-time cloud computing. Clinical services **760** performed in the cloud include the calculation of one or more blood constituents and blood pressure. Blood constituent calculations include oxygen saturation, normal and abnormal hemoglobin, metabolic and lipid constituents and glucose, as described with respect to FIG. 6, above. Also as described with respect to FIG. 6, above, data flow for a sensor **711**, **721** and connected monitor **715**, **725** includes analog waveform data from the sensor **711**, **721** to the connected monitor **715**, **725**; digital encrypted waveform data to the cloud **717,727**, which returns encrypted measurement results **717,727** to the monitor **715**, **725**.

As shown in FIG. 7, clinical services **760** further include calculation of medical indices **770**, each of which are combinations of physiological parameters. As such, two or more monitors **715**, **725** independently generate encrypted waveform data **717**, **727** used to derive a medical index **770**. The cloud **760** time synchronizes this data accordingly. In an embodiment, each device has a master clock so as to record a universal time. The cloud server **702** corrects for time differences and delays among devices that are part of the same user account. As an example, a user acquires a smart sensor/smart phone **170** (FIG. 1B) and a cuff-based blood pressure monitor **180** (FIG. 1B). The user registers these devices via their cloud account. After that, when measurements are taken, the cloud server **702** verifies if the set of required parameters are available for a particular medical index **770** and if the parameters were measured within the required time frame for these parameters.

As an example, blood pressure constantly varies. Therefore, when calculating an index involving other parameters, any measurement time frame mismatch should be small (a few minutes). In contrast, total cholesterol changes very slowly, and therefore the measurement time frame mismatch with respect to other parameters can be much larger (hours). If any time frame mismatch between measured parameters for a particular medical index is within tolerance, the cloud server **702** processes and displays the index on at least one

of the user's monitors **715**, **725**. If a time frame mismatch is too large, then each of the monitor **715**, **725** displays are dashed out for that index.

FIGS. 8A-F illustrate medical indices **800** based upon trends in some or all of selected blood constituents, e.g. Hgb (hemoglobin), BUN (blood urea nitrogen) and Cr (creatinine); plethysmograph waveform features, e.g. plethysmograph variability index (PVI) and blood pressure (BP) that are indicative of dehydration **810**, renal insufficiency **820**, over-hydration **830**, gastrointestinal bleeding **840**, congestive heart failure exacerbation **850** and cardiovascular risk **860**, respectively. Specifically, if a monitor and sensor are only capable of, or enabled to, measure blood constituent parameters, then a particular medical index ("index") may be based exclusively upon, say, Hgb, BUN and Cr. If a monitor and sensor are also capable of, or enabled to, measure plethysmograph waveform features, then that index may be based upon Hgb, BUN, Cr and PVI. (See, e.g. FIG. 1A). Further, if one or more monitors/sensors attach to a person, then that index may be based upon Hgb, BUN, Cr, PVI and BP. (See, e.g. FIG. 1B). A plethysmograph variability index (PVI) is described with respect to U.S. Pat. No. 8,414,499, filed Dec. 7, 2007, titled "Plethysmograph Variability Processor" assigned to Masimo and incorporated in its entirety by reference herein. Note that PVI is not to be confused herein with a medical index although PVI may be used to calculate or otherwise indicate one or more medical indices.

As described herein, a medical index **800** is an indicator of the physiological status of a living being. Physiological status may be a positive condition, such as strength, endurance or conditioning, or a negative condition, such as a disease state or physiological weakness, to name a few examples. In an embodiment, a medical index ("index") has a binary value. That is, the index indicates a likelihood of the existence or nonexistence of a particular physiological status such as dehydration **810**, renal insufficiency **820**, over-hydration **830**, gastrointestinal bleeding **840**, CHF exacerbation **850** and cardiovascular risk **860**, to name a few. In other embodiments, a medical index has a set of discrete values, such as a scale from 1 to 10. For example, 1 may indicate a very low likelihood and 10 a very high likelihood of a particular physiological status. In yet another embodiment, a medical index may have a continuous range of values, such as 0-100% so as to represent, for example, a probability that a particular medical condition exists.

As shown in FIG. 8A, dehydration **810** may be indicated from noninvasive measurements of Hgb, BUN and Cr, and in particular from rising values for each of these constituents over a predetermined time interval " $\Delta t_{dh}$ ." If available, rising values of PVI over  $\Delta t_{dh}$  further indicate dehydration. If available, falling values of BP over  $\Delta t_{dh}$  further indicate dehydration.

As shown in FIG. 8B, renal insufficiency **820** may be indicated from noninvasive measurements of Hgb, BUN and Cr, and in particular from falling values of Hgb, relatively fast rising values of BUN and rising to relatively fast rising values of  $\Delta t_{ri}$  over a predetermined time interval " $\Delta t_{ri}$ ." If available, falling values of PVI over  $\Delta t_{ri}$  further indicate renal insufficiency. If available, falling values of BP over  $\Delta t_{ri}$  further indicate renal insufficiency.

As shown in FIG. 8C, over-hydration **830** may be indicated from noninvasive measurements of Hgb, BUN and Cr, and in particular from falling values of Hgb and BUN over a predetermined time interval " $\Delta t_{oh}$ ," and relatively constant values of Cr over  $\Delta t_{oh}$ . If available, falling values of PVI

over  $\Delta t_{oh}$  further indicate over-hydration. If available, rising values of BP over  $\Delta t_{oh}$  further indicate over-hydration.

As shown in FIG. 8D, gastrointestinal bleeding **840** may be indicated from noninvasive measurements of Hgb, BUN and Cr, and in particular from falling levels Hgb over a predetermined time interval " $\Delta t_{gi}$ ." If available, rising values of PVI over  $\Delta t_{gi}$  further indicate gastrointestinal bleeding. If available, falling values of BP over  $\Delta t_{gi}$  further indicate gastrointestinal bleeding.

As shown in FIG. 8E, CHF exacerbation **850** may be indicated from noninvasive measurements of Hgb, BUN and Cr, and in particular from stable to falling levels of Hgb and BUN and stable to rising levels of Cr over a predetermined time interval " $\Delta t_{CHF}$ ." If available, falling values of PVI over  $\Delta t_{CHF}$  further indicate CHF exacerbation. If available, relatively constant or rising values of BP over  $\Delta t_{CHF}$  further indicate CHF exacerbation.

As shown in FIG. 8F, cardiovascular risk **860** may be indicated from noninvasive measurements of Chol, HDL, Chol/HDL and Trig and in particular from rising levels of Chol, Chol/HDL and Trig and falling levels of HDL over a predetermined time interval " $\Delta t_{cvr}$ ." If available, rising values of BP over " $\Delta t_{cvr}$ " further indicate cardiovascular risk.

In an embodiment  $\Delta t_{xx}$  are the same for each index, i.e.  $\Delta t_{dh} = \Delta t_{ri} = \Delta t_{oh} = \Delta t_{gi} = \Delta t_{CHF} = \Delta t_{cvr}$ . In an embodiment,  $\Delta t_{xx}$  varies for each constituent of a particular index, e.g.  $\Delta t_{xx}(\text{Hgb}) \neq \Delta t_{xx}(\text{BUN}) \neq \Delta t_{xx}(\text{Cr}) \neq \Delta t_{xx}(\text{PVI}) \neq \Delta t_{xx}(\text{BP})$ . The order of the particular constituents for each index is not intended to indicate the relative weight of that constituent for determining a particular index. For example, the listing of Hgb first in tables 8A-E does not suggest Hgb is more indicative of determining a particular index than BUN, Cr, PVI or BP. In an embodiment, indices are calculated over a fixed  $\Delta t$  for one or more constituents. In an embodiment, indices are a function of a delta parameter value over a fixed  $\Delta t$ , e.g.  $\Delta \text{BUN} / \Delta t$ .

FIG. 9 illustrates trends in various physiological parameters, including blood-constituents, oxygen saturation, blood pressure, respiration rate (RR), temperature and heart-related parameters including heart rate (HR) and electrocardiogram (ECG) waveform features indicative of various physiological conditions, maladies and diseases. The use of one or more of these physiological parameters for determining a particular medical index depends on the availability of sensors, processors and algorithms for measuring these physiological parameters. Further, as noted above, the order of listing of various parameters in this table is not intended to indicate the relative sensitivity of a particular index to these parameters or the relative accuracy of determining a particular index utilizing these parameters.

Medical indices are described with respect to FIGS. 8-9, above, as based upon trends in various physiological parameters, i.e. changes in physiological parameters over time. This advantageously reduces the effect of individual variations in the baseline values for these physiological parameters, especially when the "normal" range for a particular physiological parameter is relatively broad. In other embodiments, however, medical indices may be based upon physiological parameter values in lieu of or in addition to physiological parameter trends, which advantageously allows a spot-check medical index calculation. As such, the up, sideways, and down arrows of FIGS. 8-9 can represent high (or very high), normal, and low (or very low) physiological parameter values so as to indicate a particular index.

In other embodiments, medical indices may be based upon fitness parameters derived, in part, from activity and location sensors, such as accelerometers and GPS devices,

so as to measure, as examples, distance walked, calories burned, activity duration and intensity. These measurements may be combined with one or more of the parameters listed in FIG. 9 so as to derive medical indices indicative of exercise tolerance, cardiac function and arrhythmia analysis, to name a few.

A cloud-based physiological monitoring system has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of this disclosure or any claims that follow. One of ordinary skill in art will appreciate many variations and modifications.

What is claimed is:

1. A cloud-based physiological monitoring system comprising:

one or more sensors in communication with a patient so as to generate one or more data streams responsive to changes in one or more physiological conditions of the patient, wherein the one or more sensors include at least:

an optical sensor configured to provide a first data stream responsive to at least one of: pulsatile blood flow or a blood constituent parameter, and

a blood pressure sensor configured to provide a second data stream responsive to blood pressure;

one or more monitors configured to receive the data streams from the sensors; and a cloud server,

wherein the one or more monitors are configured to: determine whether communication with the cloud server is available or not available;

responsive to determining that communication with the cloud server is not available, temporarily process the data streams locally; and

responsive to determining that communication with the cloud server is available, transmit at least indications of the data streams to the cloud server,

wherein the cloud server is configured to:

process the data streams, including at least the first and second data streams, so as to derive a plurality of parameters and associated parameter measurements responsive to the changes in the one or more physiological conditions, wherein:

a first parameter of the plurality of parameters is indicative of hemoglobin (Hgb) of the patient,

a second parameter of the plurality of parameters is indicative of blood urea nitrogen (BUN) of the patient,

a third parameter of the plurality of parameters is indicative of creatinine (Cr) of the patient,

a fourth parameter of the plurality of parameters is indicative of a plethysmograph variability index (PVI) of the patient, and

a fifth parameter of the plurality of parameters is indicative of a blood pressure of the patient;

determine that the required parameters for deriving a medical index include the first, second, third, fourth, and fifth parameters, and that the first, second, third, fourth, and fifth parameters are available for deriving the medical index; and

in response to determining that most-recent parameter measurements associated with the first, second, third, fourth, and fifth parameters satisfy a time frame mismatch tolerance associated with the medical index:

determine trends in the first, second, third, fourth, and fifth parameters, the trends indicative of

15

changes in the respective first, second, third, fourth, and fifth parameters over time;  
 derive the medical index based upon a combination of the trends in the first, second, third, fourth, and fifth parameters, the medical index indicating a medical condition of the patient;  
 communicate the medical index to at least one of the one or more monitors; and  
 cause the at least one monitor to display the medical index.

2. The cloud-based physiological monitoring system according to claim 1, wherein the medical index relates to at least one of: dehydration, renal insufficiency, over hydration, gastrointestinal bleeding, congestive heart failure exacerbation, or cardiovascular risk.

3. The cloud-based physiological monitoring system according to claim 1, wherein the cloud server is further configured to:  
 in response to determining that the most-recent parameter measurements associated with the first, second, third, fourth, and fifth parameters do not satisfy the time frame mismatch tolerance:  
 not derive the medical index; and  
 cause the one or more monitors to not display the medical index.

4. The cloud-based physiological monitoring system according to claim 3, wherein causing the one or more monitors to not display the medical index further includes displaying dashes in a location on the monitor where the medical index otherwise would be displayed.

5. A physiological monitoring method comprising:  
 receiving, from one or more sensors in communication with a patient and via a monitor, sensor data responsive to changes in one or more physiological phenomena of the patient, wherein the one or more sensors include at least an optical sensor and an air-cuff sensor;  
 determining, by the monitor, whether communication with a cloud server is available or not available;  
 responsive to determining that communication with the cloud server is not available, temporarily processing the data streams locally at the monitor;  
 responsive to determining that communication with the cloud server is available, transmitting at least indications of the data streams to the cloud server;  
 processing, by the cloud server, the sensor data so as to derive a plurality of parameters and associated parameter measurements responsive to the changes in the one or more physiological phenomena, wherein:  
 a first parameter of the plurality of parameters is indicative of hemoglobin (Hgb) of the patient,  
 a second parameter of the plurality of parameters is indicative of blood urea nitrogen (BUN) of the patient,

16

a third parameter of the plurality of parameters is indicative of creatinine (Cr) of the patient,  
 a fourth parameter of the plurality of parameters is indicative of a plethysmograph variability index (PVI) of the patient, and  
 a fifth parameter of the plurality of parameters is indicative of a blood pressure of the patient;  
 determining, by the cloud server, that the required parameters for deriving a medical index include the first, second, third, fourth, and fifth parameters, and that the first, second, third, fourth, and fifth parameters are available for deriving the medical index; and  
 in response to determining that most-recent parameter measurements associated with the first, second, third, fourth, and fifth parameters satisfy a time frame mismatch tolerance associated with the medical index:  
 determining, by the cloud server, trends in the first, second, third, fourth, and fifth parameters, the trends indicative of changes in the respective first, second, third, fourth, and fifth parameters over time;  
 deriving, by the cloud server, the medical index responsive to a combination of the trends in the first, second, third, fourth, and fifth parameters, the medical index indicating a medical condition of the patient;  
 communicating, by the cloud server, the medical index to the monitor; and  
 causing display of the medical index on the monitor.

6. The physiological monitoring method according to claim 5 further comprising:  
 causing display of the medical index on a smart cellular telephone.

7. The physiological monitoring method according to claim 6, wherein the medical index includes an indication of at least one of: dehydration, renal insufficiency, over hydration, gastrointestinal bleeding, congestive heart failure exacerbation, or cardiovascular risk.

8. The physiological monitoring method according to claim 5 further comprising:  
 in response to determining that the most-recent parameter measurements associated with the first, second, third, fourth, and fifth parameters do not satisfy the time frame mismatch tolerance:  
 not deriving the medical index; and  
 causing the monitor to not display the medical index.

9. The physiological monitoring method according to claim 5, wherein causing the monitor to not display the medical index further includes causing the monitor to display dashes in a location on the monitor where the medical index otherwise would be displayed.

\* \* \* \* \*