




(86) **Date de dépôt PCT/PCT Filing Date:** 2008/10/03
(87) **Date publication PCT/PCT Publication Date:** 2009/04/09
(45) **Date de délivrance/Issue Date:** 2017/03/28
(85) **Entrée phase nationale/National Entry:** 2010/03/30
(86) **N° demande PCT/PCT Application No.:** GB 2008/050894
(87) **N° publication PCT/PCT Publication No.:** 2009/044203
(30) **Priorités/Priorities:** 2007/10/03 (GB0719228.9);
2008/03/04 (GB0804012.3); 2008/03/31 (GB0805775.4)

(51) **Cl.Int./Int.Cl.** **C25D 11/26** (2006.01),
A61L 27/16 (2006.01)
(72) **Inventeurs/Inventors:**
AGG, PHILIP JAMES, GB;
SHAWCROSS, JAMES TIMOTHY, GB;
PICKFORD, MARTIN EDWARD LEE, GB;
TURNER, ANDREW DEREK, GB;
LEWIS, DAVID RICHARD, GB
(73) **Propriétaire/Owner:**
ACCENTUS MEDICAL LIMITED, GB
(74) **Agent:** GOWLING WLG (CANADA) LLP

(54) **Titre : PROCEDE DE FABRICATION D'UN METAL A PROPRIETES BIOCIDES**
(54) **Title: METHOD OF MANUFACTURING METAL WITH BIOCIDAL PROPERTIES**

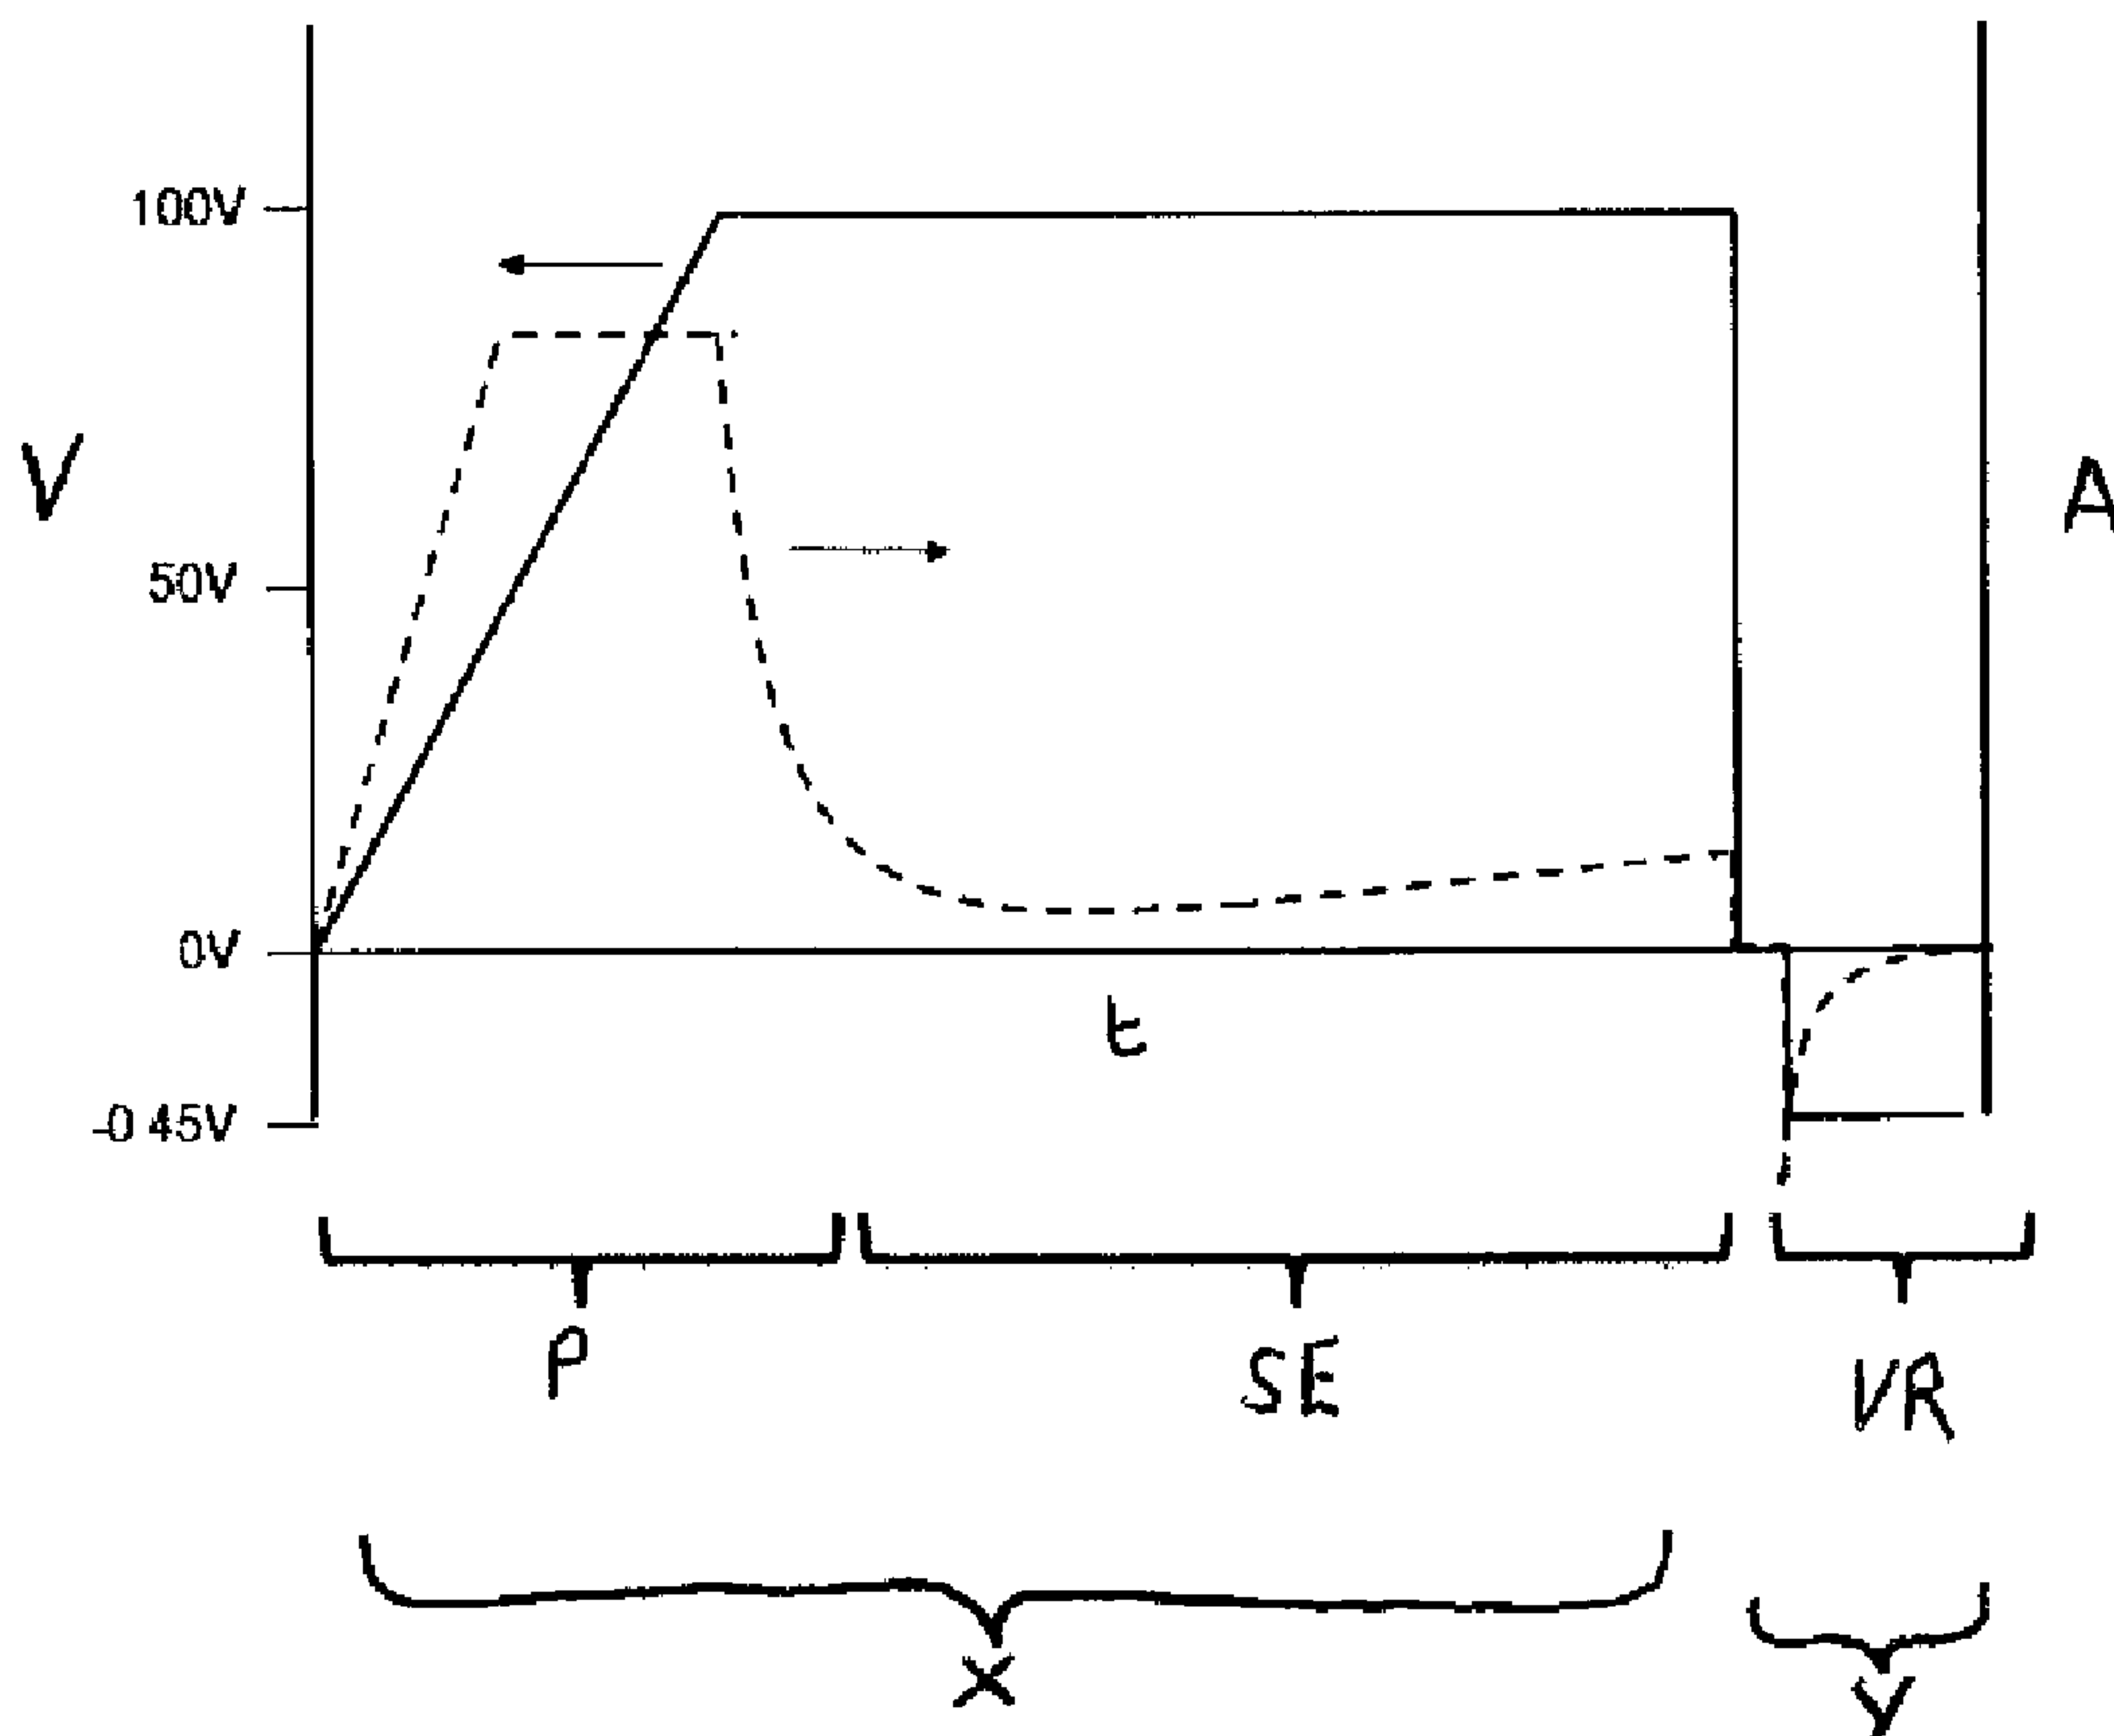

(57) **Abrégé/Abstract:**

Metal objects are treated by anodising the metal object in contact with an acidic solution, and then subjecting the anodised metal object to a reversed voltage (compared to the anodising voltage). The thus- treated metal object is then contacted with a biocidal metal-containing solution. Biocidal metal is deposited on the surface of the metal object, resulting in improved biocidal properties.

