



(22) Date de dépôt/Filing Date: 1993/12/20

(41) Mise à la disp. pub./Open to Public Insp.: 1994/06/23

(45) Date de délivrance/Issue Date: 2004/10/26

(30) Priorité/Priority: 1992/12/22 (07/994,817) US

(51) Cl.Int.⁵/Int.Cl.⁵ A61B 17/34

(72) Inventeurs/Inventors:

STEPHENS, RANDY R., US;
BISHOP, GREGORY D., US;
VOEGELE, JAMES W., US;
WELLING, DIANE, US;
SMITH, RICHARD, US;
COLLINS, JOHN M., US;
SELECMAN, GEORGE, US


(73) Propriétaire/Owner:

ETHICON, INC., US

(74) Agent: OGILVY RENAULT

(54) Titre : TROCAR DE SURETE AMELIORE

(54) Title: IMPROVED SAFETY TROCAR

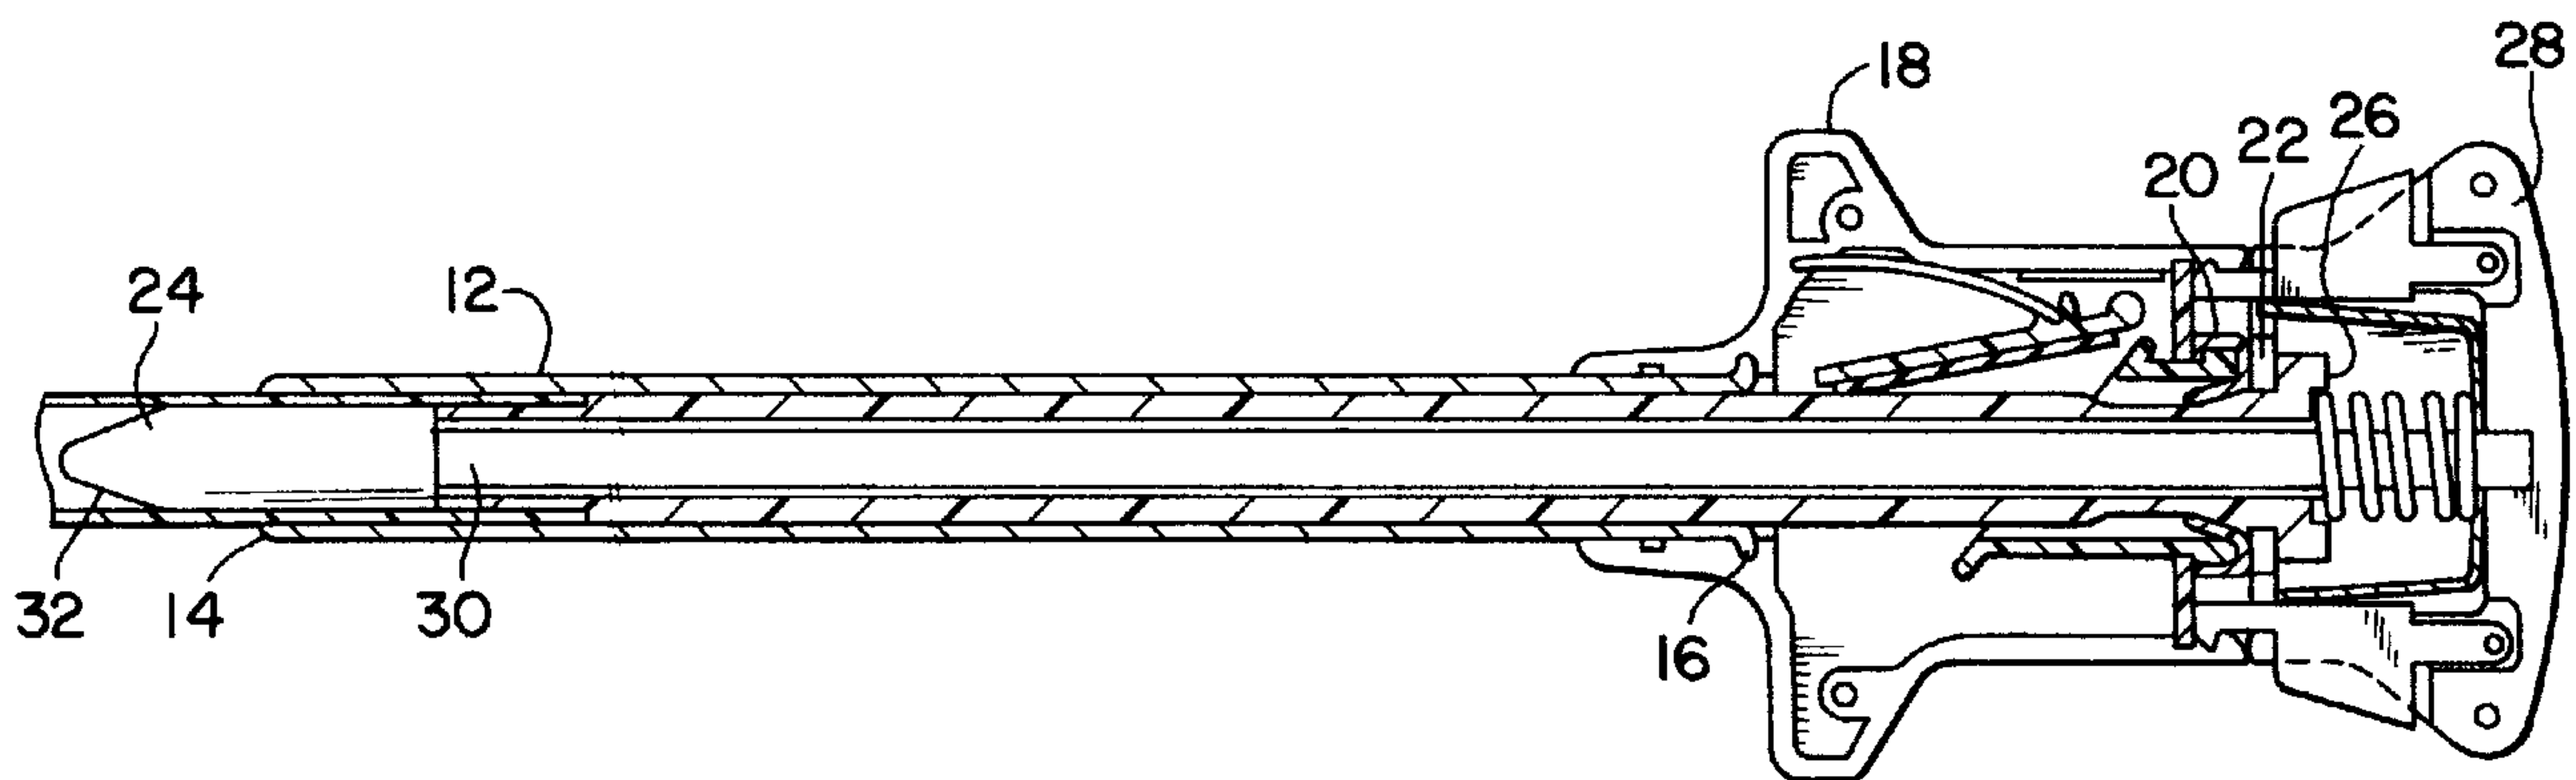

(57) Abrégé/Abstract:

A safety trocar is provided which includes a spring-loaded shield that shields the cutting tip of the obturator after the obturator penetrates tissue. The distal end of the shield is conical in profile and contains a slot which conforms to the geometry of the cutting tip. The obturator tip contains a knife edge blade which extends the length of the cannula inner diameter. Ideally, the knife is made of an amorphous metal, and may be serrated at its edge.

ABSTRACT

5 A safety trocar is provided which includes a
spring-loaded shield that shields the cutting tip of the
obturator after the obturator penetrates tissue. The
distal end of the shield is conical in profile and
contains a slot which conforms to the geometry of the
10 cutting tip. The obturator tip contains a knife edge
blade which extends the length of the cannula inner
diameter. Ideally, the knife is made of an amorphous
metal, and may be serrated at its edge.

IMPROVED SAFETY TROCARFIELD OF THE INVENTION:

5 This invention relates to trocars used to puncture
- tissue for the performance of endoscopic, laparoscopic or
arthroscopic surgery and, in particular, to such trocars
which employ a safety device to shield the obturator point
immediately after the point has perforated tissue.

BACKGROUND OF THE INVENTION:

10 A trocar generally comprises two major components, a
trocar tube and an obturator. The trocar tube or cannula
15 is inserted through the skin. Access is gained through to
a body cavity so that endoscopic, laparoscopic or
arthroscopic surgery may be performed. In order to
penetrate the skin, the distal end of the trocar tube is
placed against the skin and an obturator is inserted
20 through the tube. By pressing against the proximal end of
the obturator the point of the obturator is forced through
the skin until the obturator enters the body cavity. At
this time, the trocar tube is inserted through the
perforation made by the obturator and the obturator is
25 withdrawn, leaving the trocar tube as an accessway to the
body cavity.

30 It has been found that often a great deal of force is
required to cause the obturator point to penetrate the
skin and underlying tissue. When the point finally breaks
through this tissue, resistance to penetration is suddenly
removed, and the obturator point can suddenly reach to
penetrate internal organs of the body, which may cause
lacerations and other injury to the internal organs. To

5 avert this danger to the patient, trocars have been developed which carry a spring-loaded tubular shield within the trocar tube and surrounding the obturator. The distal end of the shield presses against the skin as the
10 obturator point penetrates the body, until the obturator has formed a perforation with a diameter sufficient to allow the safety shield to pass through. At that time the resistance of the tissue to the spring-loaded shield is removed, and the shield will spring forward to extend into the body cavity, surrounding the point of the obturator. The shield thus protects the internal body organs from inadvertent contact with the point of the obturator. A trocar including such a safety shield is described in U.S. Patent 4,535,773, for example.

15 The tubular shield in such a trocar will, however, require the incision formed by the obturator to extend to a considerable diameter before the resistance of the tissue pressure has been sufficiently decreased to allow
20 the safety shield to spring forward. It is only when the incision attains the diameter of the shield that the shield is fully able to spring into the body cavity. When the obturator employs a long, tapered cutting tip, this tip must extend a significant distance into the body
25 before the incision is sufficiently enlarged to release the safety shield. It would therefore be desirable to provide a safety shield which will spring forward to shield the obturator tip as soon as possible after entry is gained to the body cavity.

30 In accordance with the principles of Deniega, U.S. Patent No. 5,066,288, a safety shield for a trocar obturator is provided which exhibits a rounded, bullet-shaped distal end. A slot is formed in this distal

end which corresponds to the geometry of the obturator tip, through which the tip extends during perforation of the skin. With this distal end conforming to the geometry of the tip, a smooth transition is provided from the tip to the distal end of the shield, enabling the shield to closely follow the obturator tip through the tissue. The rounded distal end will press against the skin and tissue in close proximity to the periphery of the incision as it is formed, and will aid in the enlargement of the incision to enable the shield to spring forward nearly as soon as entry is gained into the body cavity.

One desirable function of such a trocar is for the obturator to slide smoothly within the trocar tube during both insertion and retraction of the obturator. Opposing this need is the necessity to form the obturator to be nearly the same diameter as the tube, so that the tissue perforation will be the size of the tube. Thus, tolerances are generally tight between the diameter of the obturator and the inside diameter of the trocar tube. A further complication is provided by the valve at the proximal end of the trocar tube, which is needed to seal the proximal end during removal of the obturator when the trocar tube and body cavity are insufflated with gases. The valve, which generally takes the form of a hinged flap or trumpet valve, is spring-loaded to bear against the obturator, thereby assuring that the valve will close automatically upon withdrawal of the obturator from the trocar tube. As the valve bears against the obturator it will frictionally disrupt the entry and withdrawal of the obturator. As a result of these tolerance problems, heretofore there has not been an obturator which corresponds identically to the shaft of the trocar

cannula, and wider than the inner dimension of the safety shield in which the obturator slides.

5 Further patient safety would be provided by preventing the sudden extension of the obturator into the body cavity as the obturator tip fully penetrates the tissue. In accordance with yet another aspect of Deniega '688, means are provided which permit only incremental advancement of the obturator as tissue penetration proceeds. Such incremental advancement is provided by a ratchet or screw mechanism, for instance. Yet, this has not alleviated the problem of having an obturator tip with only minimal exposure past the edge of the safety shield at all positions of the safety shield distal end.

15 SUMMARY OF THE INVENTION:

20 It is therefore an object of the present invention to provide a trocar with a safety shield such that the cutting edge of the obturator tip of the safety shield corresponds with the inner diameter of the trocar cannula. This improvement would reduce the force to penetrate the abdominal wall with using such trocar.

25 It is further desirable to form the obturator tip out of any one of the amorphous-type metals which have currently come into use. These amorphous metals such as amorphous steels and the like, have heretofore not been used in the medical industry for tissue piercing purposes, such as in trocar obturator tips.

30 Further, it is an object of the invention to provide a safety shielded trocar with a conical shape shield. This type of shield provides for ease of tissues

spreading, and as well as adapts to be conformable to various types of obturator tips.

5 In this type of safety shield it is desired to
- provide a diametral slot. This slot allows passage of the
knife edge which causes a diametral slit to be made in the
abdominal wall upon puncture. It is believed that such a
slit, would tend to improve healing and simulates the cut
10 of a scalpel, rather than the standard triangular point
openings as made with standard trocars. It has the added
effect of quicker safety shield response time, to cover
the obturator tip.

15 These and other objects of the invention are provided
in a trocar which comprises an obturator connected to an
obturator handle and the obturator having a sharpened tip.
This obturator may be inserted into a cannula which is
connected to a cannula handle. The cannula itself has an
opening with an internal diameter. Also, the device
20 contains a safety shield which is spring-loaded within the
obturator handle. The safety shield is capable of
covering the obturator tip. The safety shield contains
within it an opening through which the obturator tip may
pass. Generally, the obturator tip when it extends
25 through the opening abuts the inner diameter of the
cannula. Generally, the obturator tip is formed from an
amorphous metal and contains a curved profile, forming a
knife edge. The knife edge indeed may contain serrations.
Also, the safety shield is conical in shape so that it is
30 more readily able to spread tissue and has a slit which
has a width extending across the inner diameter of the
cannula.

In operation, therefore the trocar of the present invention affords easier puncture, more rapid healing, and uses highly accurately shaped metals which allow for the rapid piercing of the abdominal wall. The trocar of this invention is able to be pressed through tissue, and yet will be protected by the covering by the safety shield over the obturator tip.

It is believed that this invention will be better understood by reference to the attached drawings taken in connection with the Detailed Description of the Invention.

DESCRIPTION OF THE DRAWINGS:

Figure 1 is a perspective view of a trocar with a conically shaped safety shield;

Figure 2 is a bottom view of the trocar of Figure 1;

Figure 3 demonstrates the capability of prior art obturator tips as to piercing tissue;

Figure 4 illustrates the obturator tip of the present invention piercing tissue;

Figure 5 is a side view of the obturator tip of the invention taken alone without the safety shield covering it;

Figure 6a and 6b are alternate views of an obturator tip of this invention;

Figure 7a is a combination view of the obturator tip of Figure 5 covered by the safety shield, while Figure 7b

- 7 -

is a view of the safety shield allowing the exposure of the obturator tip of the invention; and

5 Figure 8 is a cross-sectional view of the trocar of Figure 1.

DETAILED DESCRIPTION OF THE INVENTION:

10 A safety trocar constructed in accordance with the principles of the present invention is shown in Figures 1 and 8. The trocar 10 includes a trocar tube or cannula 12 having an open distal end 14 and open flanged proximal end 16. The proximal end 16 is mounted in a trocar handle 18. There is an aperture 20 at the proximal end 16 of the
15 trocar handle 18 which is surrounded by a gasket ring 22.

An obturator 24 is slidably and removably located within the trocar cannula 12 and is inserted into the handle 18 and trocar cannula 12 by way of the aperture 20
20 in the trocar cannula handle 18. Obturator 24 may reciprocate into obtuator handle 28 in a slidable fashion, in a fixed linear motion or conversely may rotate within handle 28. At obturator proximal end 26 is an obturator handle 28, and the distal end 30 of the obturator 24 is
25 sharpened as a knife edge 32. The safety trocar 10 of the Figures 1 and 8 is used to puncture a hole in soft tissue by placing the distal end 14 of the trocar cannula 12 against tissue and pressing against the obturator handle 28. As pressure is exerted against the obturator handle
30 28, the safety shield 34 begins to compress the spring 36 inside the obturator handle 28, and the shield 34 retracts into the handle 28. This retraction exposes the obturator knife edge 32, which punctures the tissue.

Figure 7b shows the shield 34 is fully compressed (within the obturator handle 28) and the obturator knife edge 32 is fully exposed beyond the distal end of the safety shield 34 and trocar cannula 12. When the
5 obturator knife edge 32 breaks through the inner surface of the tissue, the spring-loaded safety shield 34 springs forward around the obturator distal end 30, shielding the obturator knife edge 32, to prevent inadvertent contact of the edge 32 with internal organs of the body inside the
10 tissue being punctured.

Operation of the trocar with the safety shield of this invention is shown in Figures 1, 2 and 7b. Figure 1 is a perspective view of the trocar 10 with the trocar
15 cannula 12 held with inside trocar handle 18 so that the end of the safety shield 34 extends from the distal end 14 of the trocar cannula 12. An end view of the distal end 12 of the cannula is shown in Figure 2. Figure 5 is a view of the obturator 24 alone without the shield 34 over it. Figure 7b is view of the distal end of the instrument
20 of Figure 1, with the knife edge 32 of the obturator 24 extended and the obturator distal end 30 moved apart from the safety shield 34. In Figure 7a, the obturator distal end 30 is shown covered by the safety shield 34 of Figure
25 7b.

While this invention has been described in general, various aspects of the device will now be described more in particular. First, it is necessary to look at the
30 obturator distal end 30 as seen in Figures 1, 5, 7a and 7b, and 8. This obturator distal end 30 is generally a diametrically shaped knife edge 32. It contains two planar faces 40 which form the sharpened knife edge 32. The diametrically shaped knife edge 32 extends across the entire

length L of the inner diameter of the trocar cannula. In this way, the dimensions of the knife edge 32 enable it to be placed flush against the sides S of the trocar cannula 12. This configuration lowers the force necessary to puncture and penetrate tissue. This is true because with such a knife edge 32, the obturator 24 is able to move adjacent the edges 42 of the trocar cannula 12. Therefore, when the tissue T encounters the trocar cannula 12, there is no further spreading of tissue by the cannula 12. This is in contrast with the trocar of the prior art inventions, (as seen in Figure 3) tissue cannot be caught between the obturator tip and the safety shield.

It should be noted that knife edge 32 should be taken in conjunction with the safety shield 34 of this invention. It will be noticed that the safety shield 34 is conical in shape. This conically-shaped safety shield 34, generally made of a plastic, will cause the tissue to spread in a very gradual fashion. Of course, the conical shape may be steeper or shallower with respect to the diameter of cannula 12 dependent on the desired severity of puncture. Naturally, a steeper (longer) conical height will provide smoother puncture in conjunction with an appropriately dimensioned knife edge 32. In addition, because the safety shield 34 also abuts the internal diameter of the trocar cannula 12, the safety shield 34 also is able to perform better spreading of the tissue.

It will be seen that the knife edge 32 at its bottom as in Figure 2 forms a rather long diametral slits. This is different than the traditional triangular shaped cuts made by traditional trocars. This cut is more like the cut of scalpel. In this way, tissue healing will be promoted in that less tissue must be brought together at

the skin surface. Also, because the tissue is very readily pierced, this formulation of the knife edge 32 and safety shield 36 enables easier force to pierce during piercing.

5

- As seen in Figures 6a and 6b, there are shaped two alternate forms of knife edges, 32A, 32B, both based on a dimetral slit design. In one knife edge 32A contains a serrated edge. This serrated edge 32A is able to cut through tissue with a much greater ease. Of course, the serrated edge 32A creates greater surface area contact in tissue, but does not detract from the size or shape of the knife edge.

10

15

Alternately, in Figure 6b, there is described a tip 32B with a generally diametral or scalpel-type shape. This scalpel-type shape used in conjunction with a safety shield compatible with it allows the user to pierce the tissue using the same holding position as using a scalpel. This can be particularly useful for laparoscopic and endoscopic applications of such a knife edge 32B. These knife edges may be placed at an angular orientation to form a cutting shape between a 10° and 60° included angle with the sides of the cannula 12.

20

25

30

In fact, the obturator 24 of this invention is also useful as a piercing instrument. That is, because the obturator 24 of the present design is useful to pierce tissue, much like a scalpel, this obturator 24 may be borrowed to be used endoscopically down a long trocar cannula in order to cut tissue internally. Of course, the safety shield 34 of this mechanism must be adapted so that it is able to be covered only when desired and not automatically after piercing through tissue.

- 11 -

5 The obturator 24 of this invention maybe formed from
an amorphous metal, much like that described in Serial No.
786,752, assigned to a common assignee as this invention.
This amorphous metal can be very highly shaped and refined
to very small dimensions, such as about 0.001" or less.
In this way, the knife edge of this mechanism is very
readily adapted to pierced tissue. Also, because the
amorphous metals may be formed as serrated edges as in
Figures 6a, we are able to use such a knife edge to
10 perform useful endoscopic functions. Nonetheless, other
materials are also available, such as ceramics, sharpened
plastic and the typical metals, such as aluminum or
stainless steel, from which to form the knife edge.

15 One additional aspect of the obturator 24 of this
device is the ability of the tip to rotate its shaft. As
seen in Figure 7, there is provided a rotating mechanism
allowing the obturator 24 and conical shield 34 to be able
to rotate freely about the longitudinal axis of the trocar
20 10. This provides the user with the ability to enter the
abdomen without slippage of the obturator 24 due to torque
applied by the user as he tries to "twist" the obturator
into the abdomen.

25 That this new trocar presents many improved uses.
There are also equivalents that can be discerned from the
description of this invention. Such equivalents are
intended to be covered by the scope of this invention as
to be derived from the attached claims.
30

- 12 -

CLAIMS:

1. A trocar comprising:

an obturator connected to an obturator handle, and said obturator having a sharpened tip;

a cannula connected to a cannula handle, said obturator insertable into said cannula, and said cannula having an inner wall defining an inner diameter;

a safety shield, spring loaded within said obturator handle and capable of covering said obturator tip;

wherein said safety shield contains an opening through which said obturator tip may pass, and said obturator tip when extending through said opening abuts the inner wall of said cannula, and wherein said obturator tip has a pair of planar surfaces forming a knife edge, the width of said knife edge corresponding with the length of said cannula inner diameter.

2. The trocar of claim 1 wherein said knife edge has a curved profile.

3. The trocar of claim 1 wherein said knife edge has serrated edges.

4. The trocar of claim 1 wherein said safety shield has a distal end with a conical shape, and said opening comprises a slit and said slit having a width extending across said cannula inner diameter.

5. The trocar of claim 4 wherein said knife edge has a curved profile.

- 13 -

6. A trocar comprising:

an obturator connected to an obturator handle, and said obturator having a sharpened tip;

a cannula connected to a cannula handle, said obturator insertable into said cannula, and said cannula having an inner wall defining an internal diameter;

a safety shield, spring loaded within said obturator handle and capable of covering said obturator tip;

wherein said safety shield contains an opening through which said obturator tip may pass, and said safety shield having a distal end with a conical shape, and

wherein said obturator tip has a pair of planar surfaces forming a knife edge, the width of said knife edge corresponding with the length of said cannula inner diameter.

7. The trocar tip of claim 6 wherein said knife edge has serrated edges.

8. The trocar of claim 6 wherein said opening comprises a slit and said slit having a width extending across said cannula inner diameter.

FIG.1

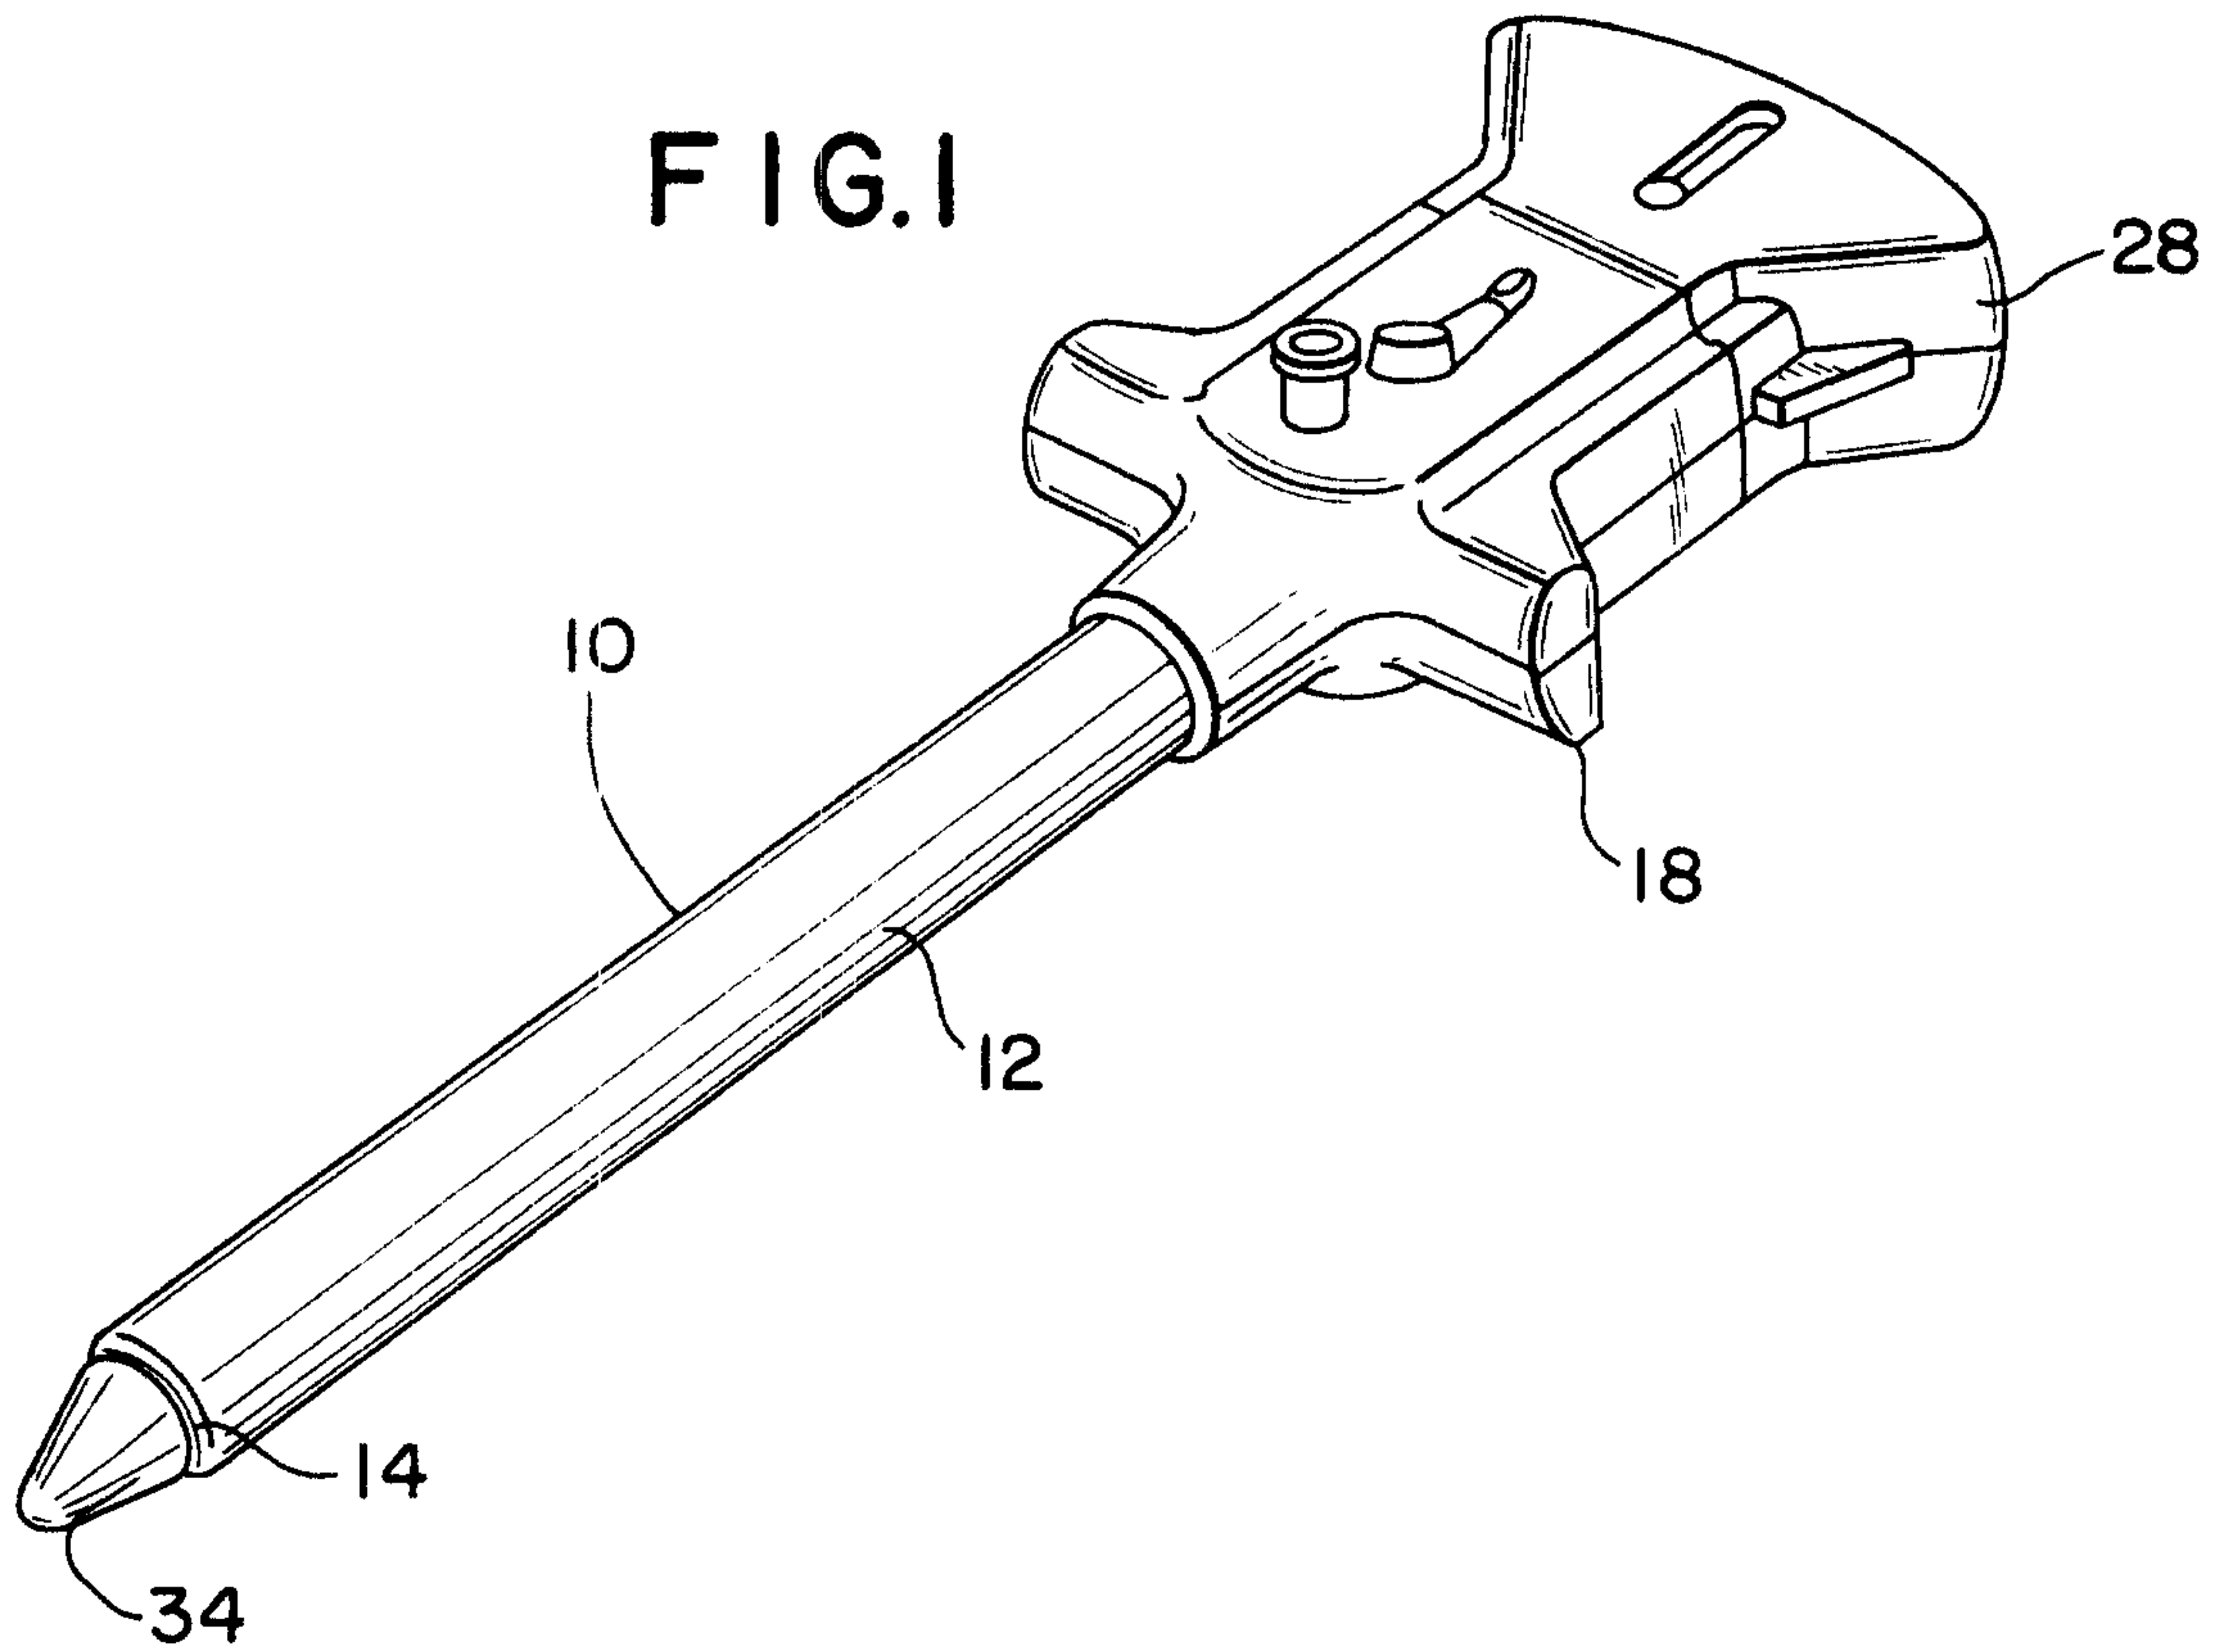


FIG.2


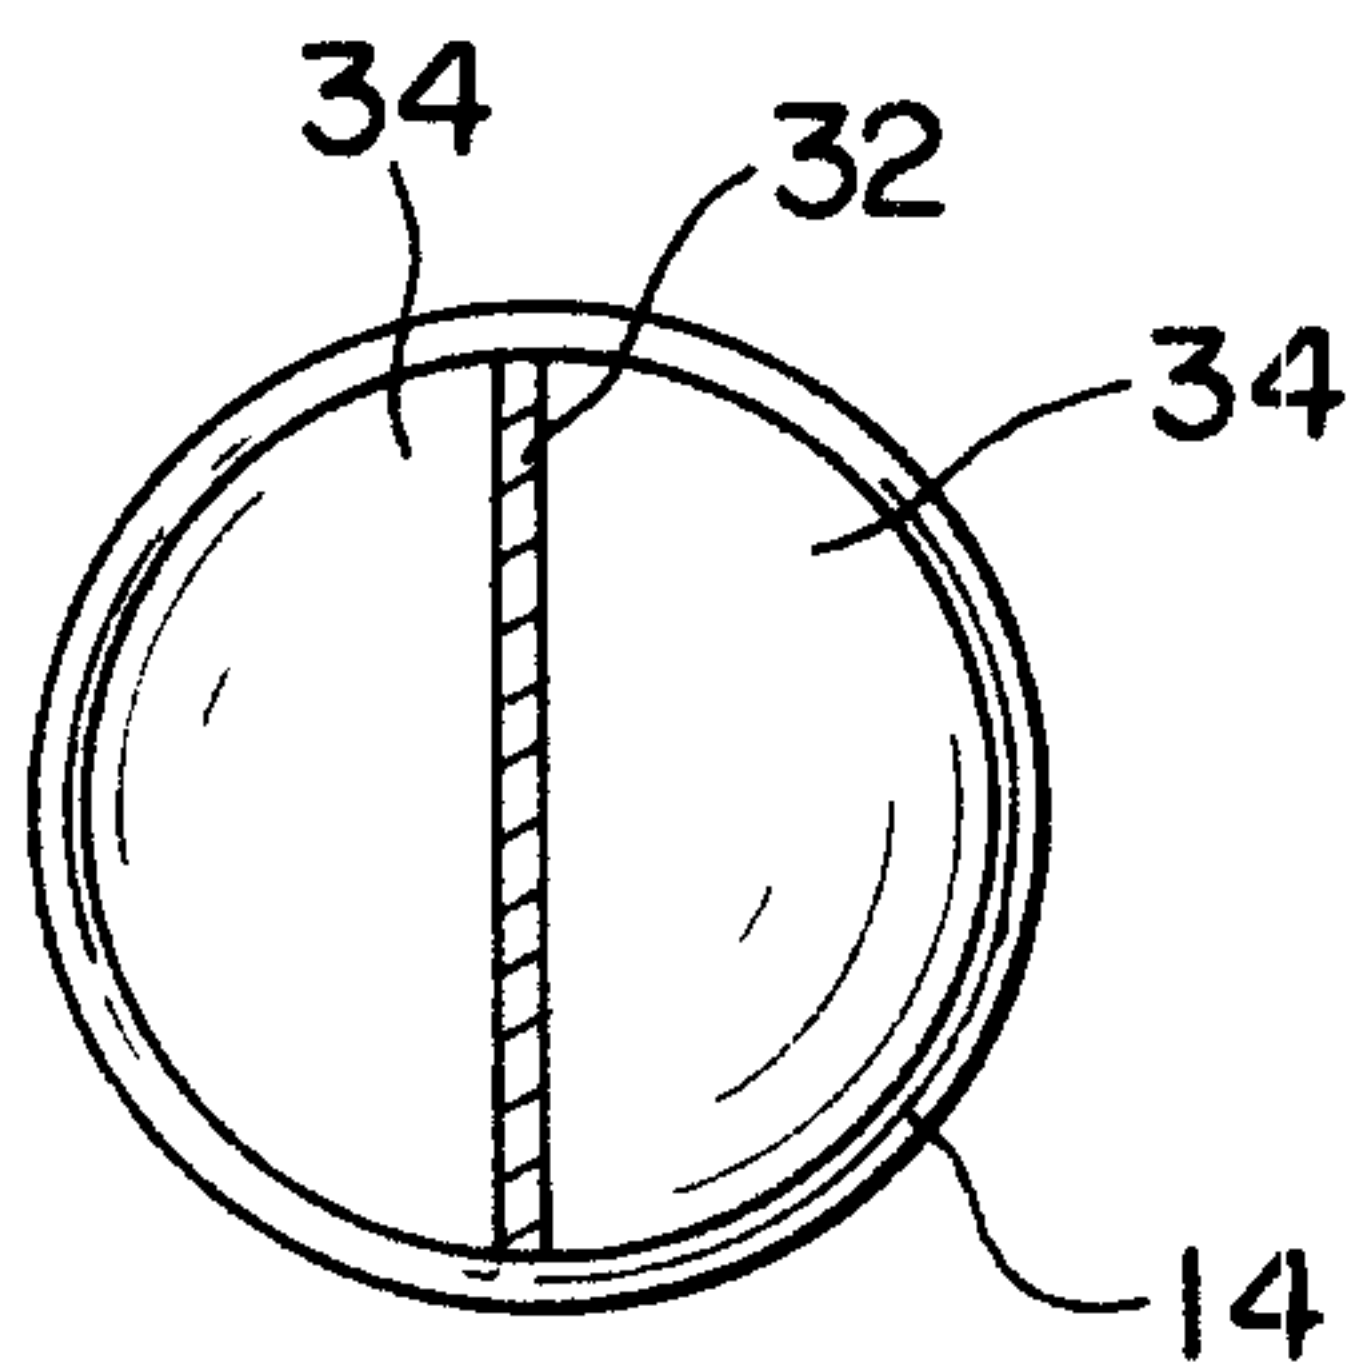


FIG.3

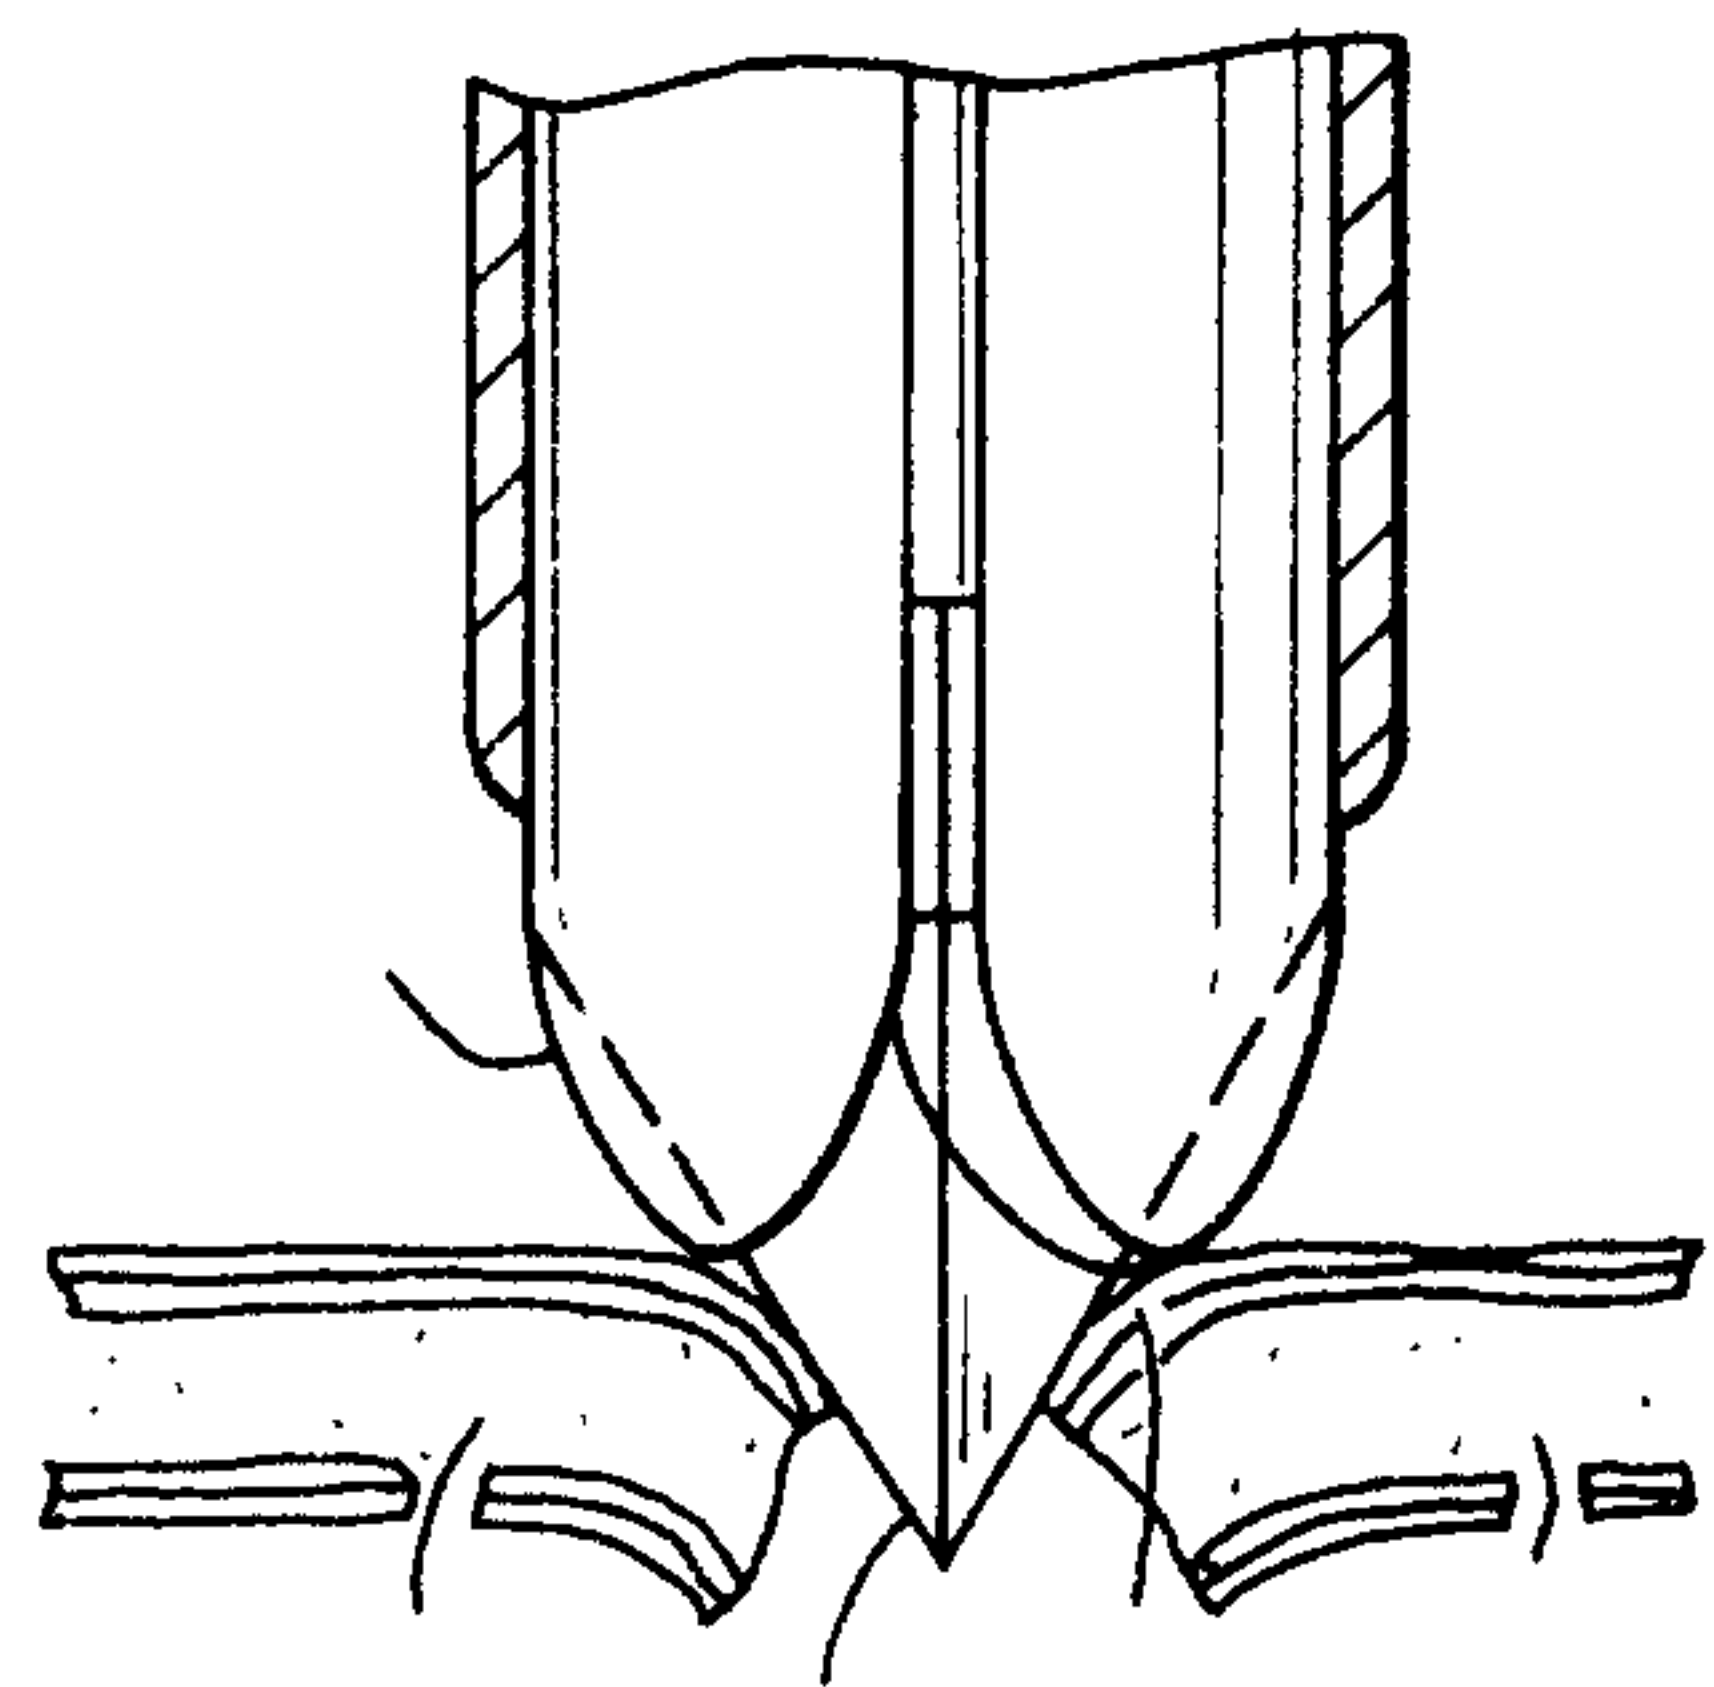

PATENT AGENTS

Dwight Ogilvy Renault

FIG. 4

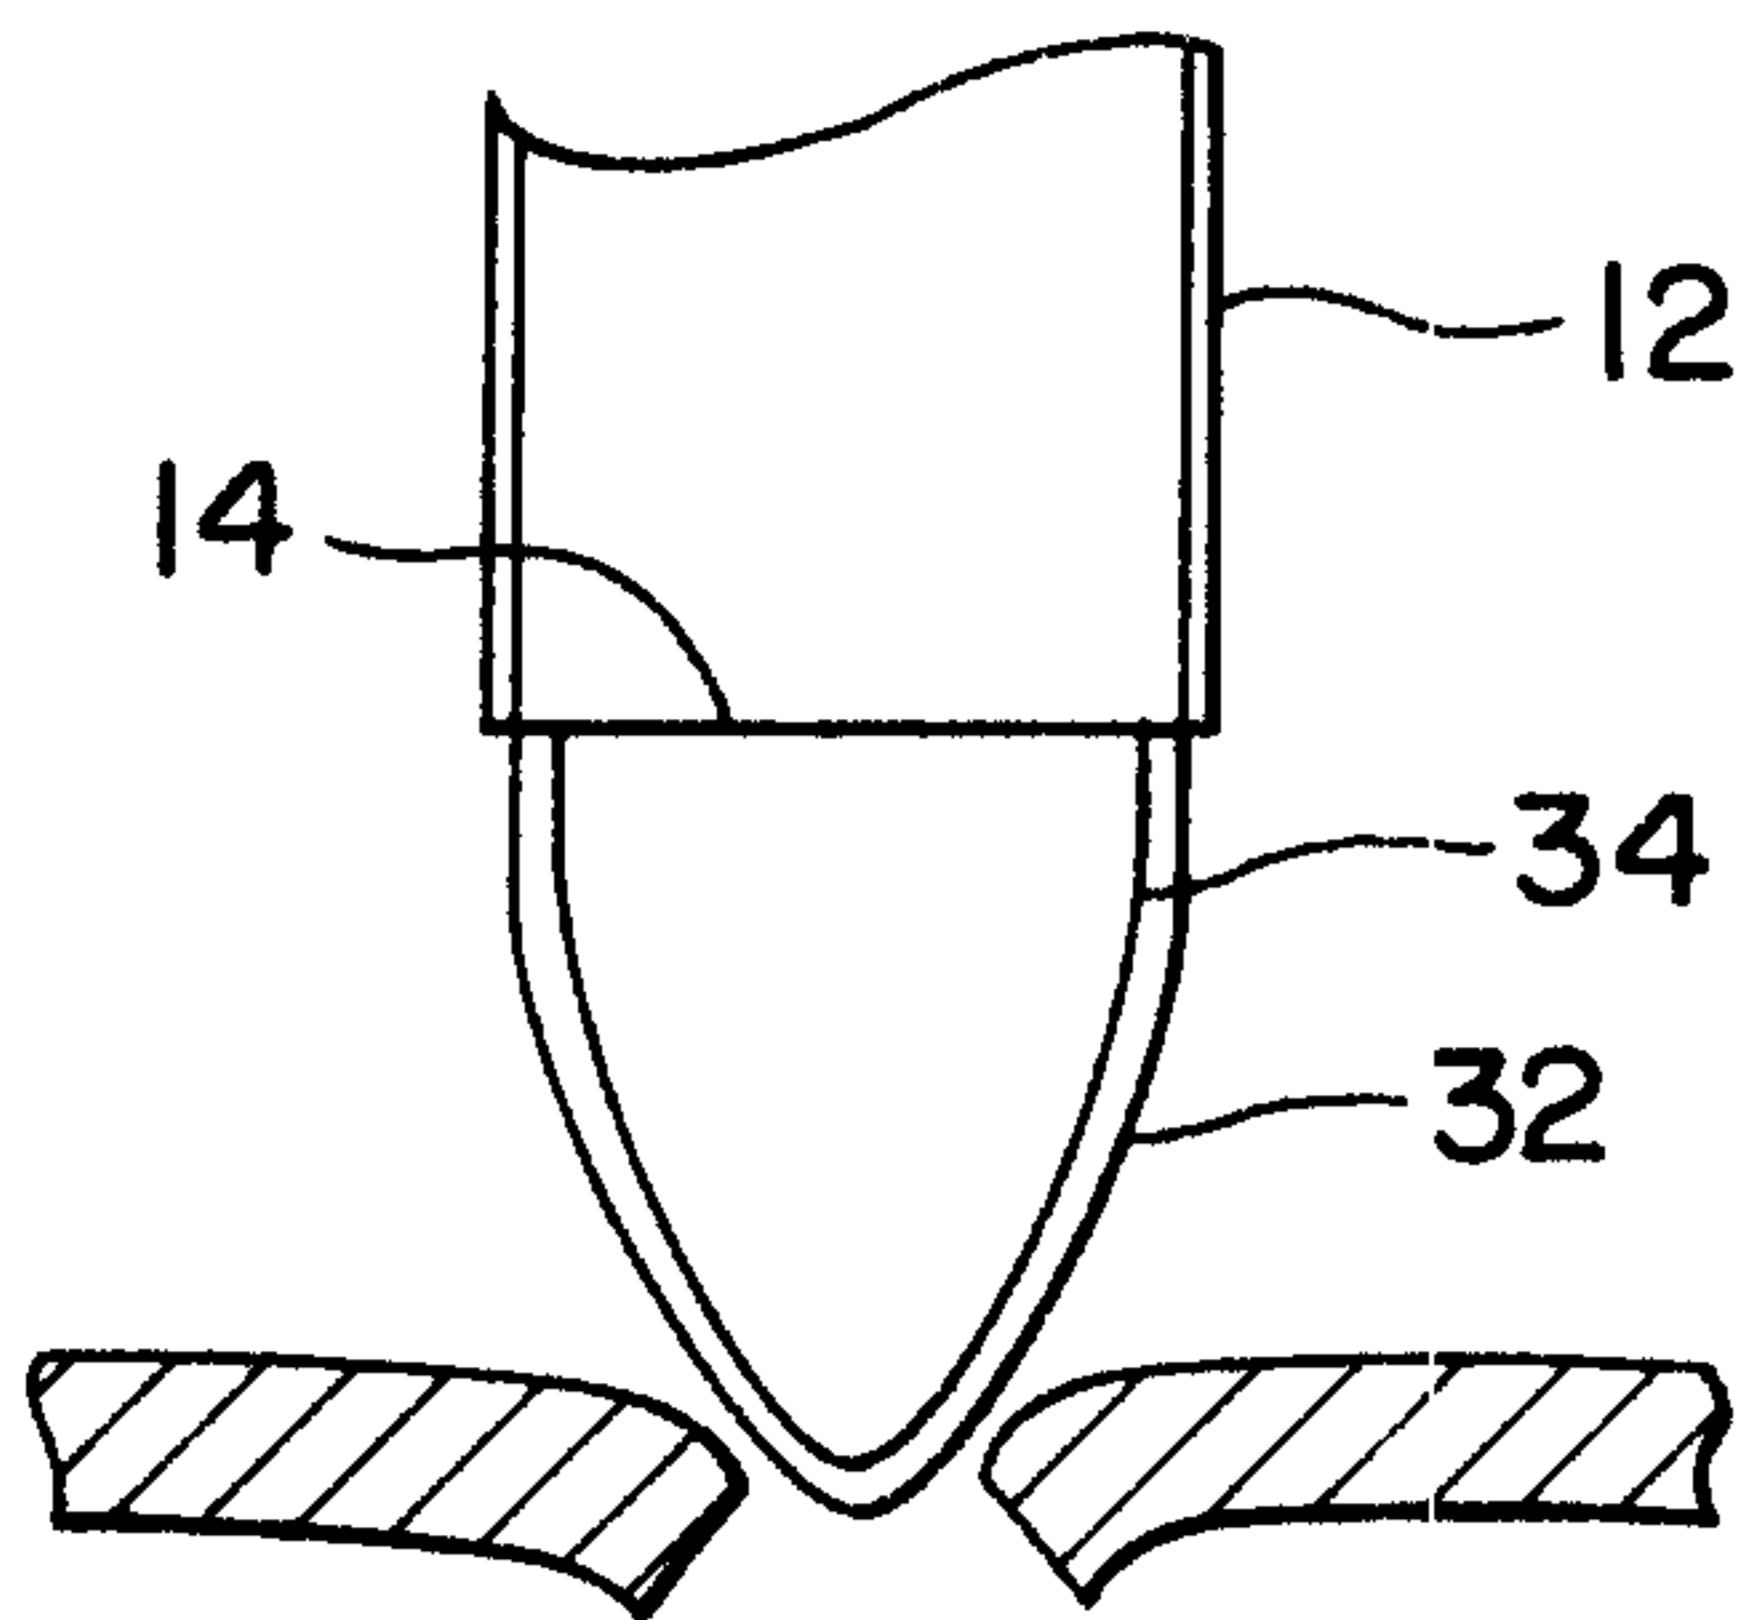


FIG. 5

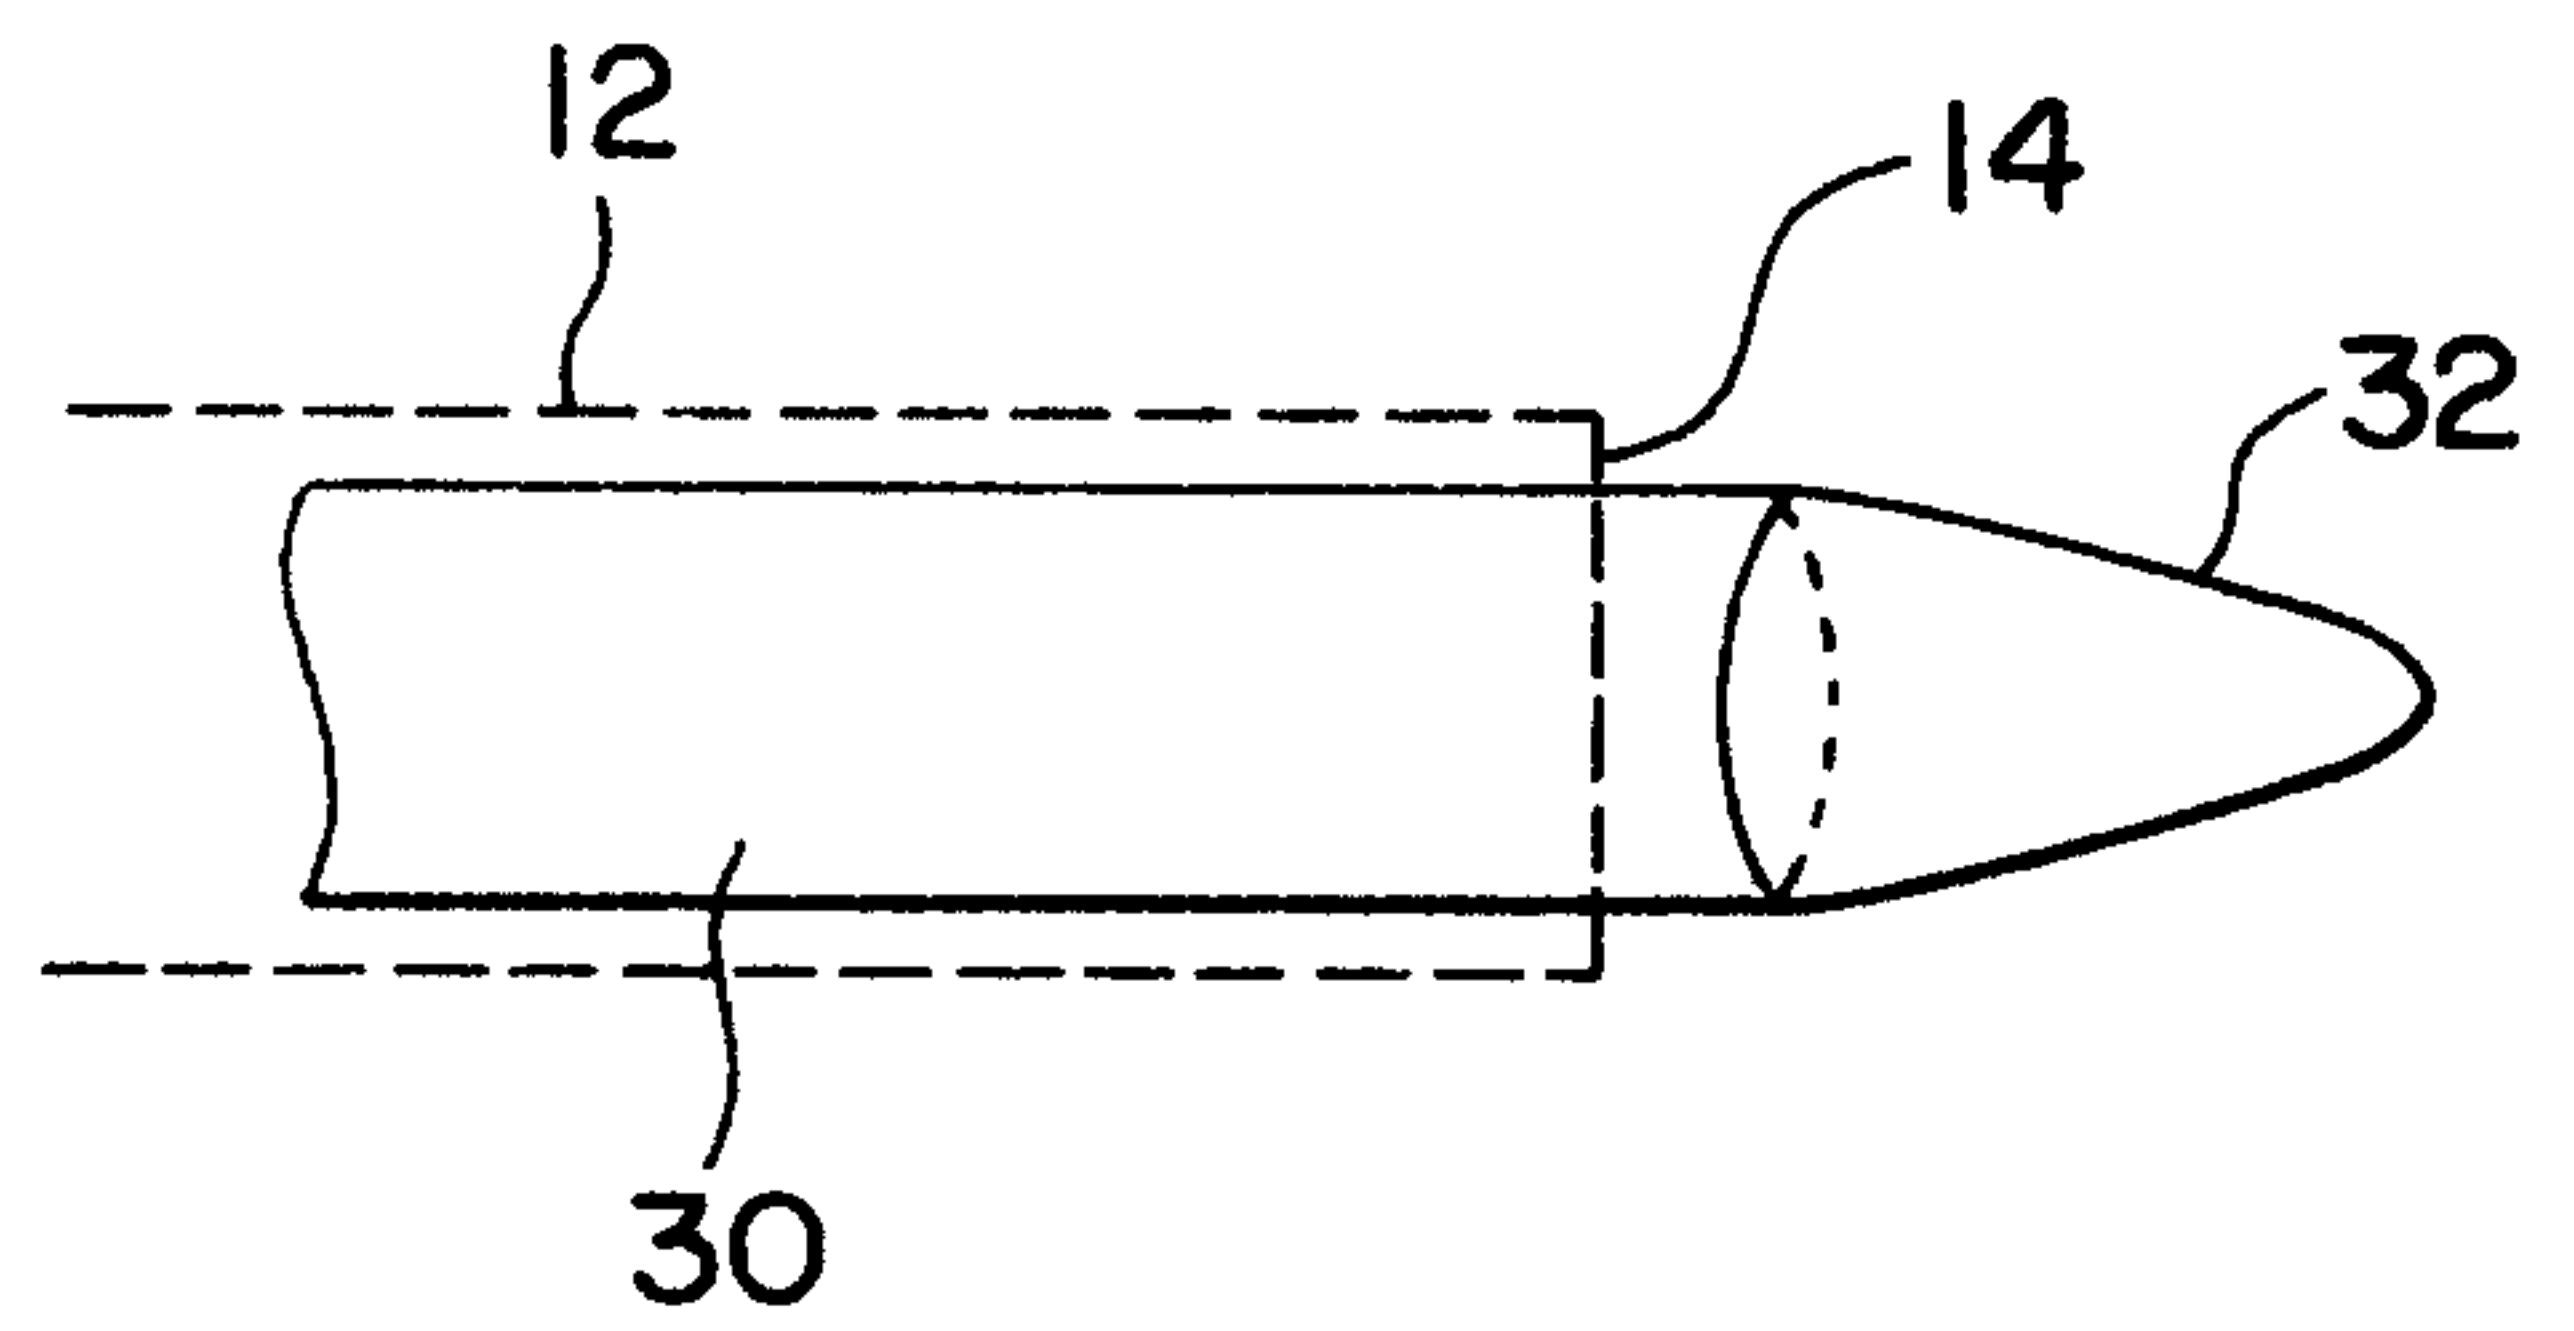


FIG. 6A

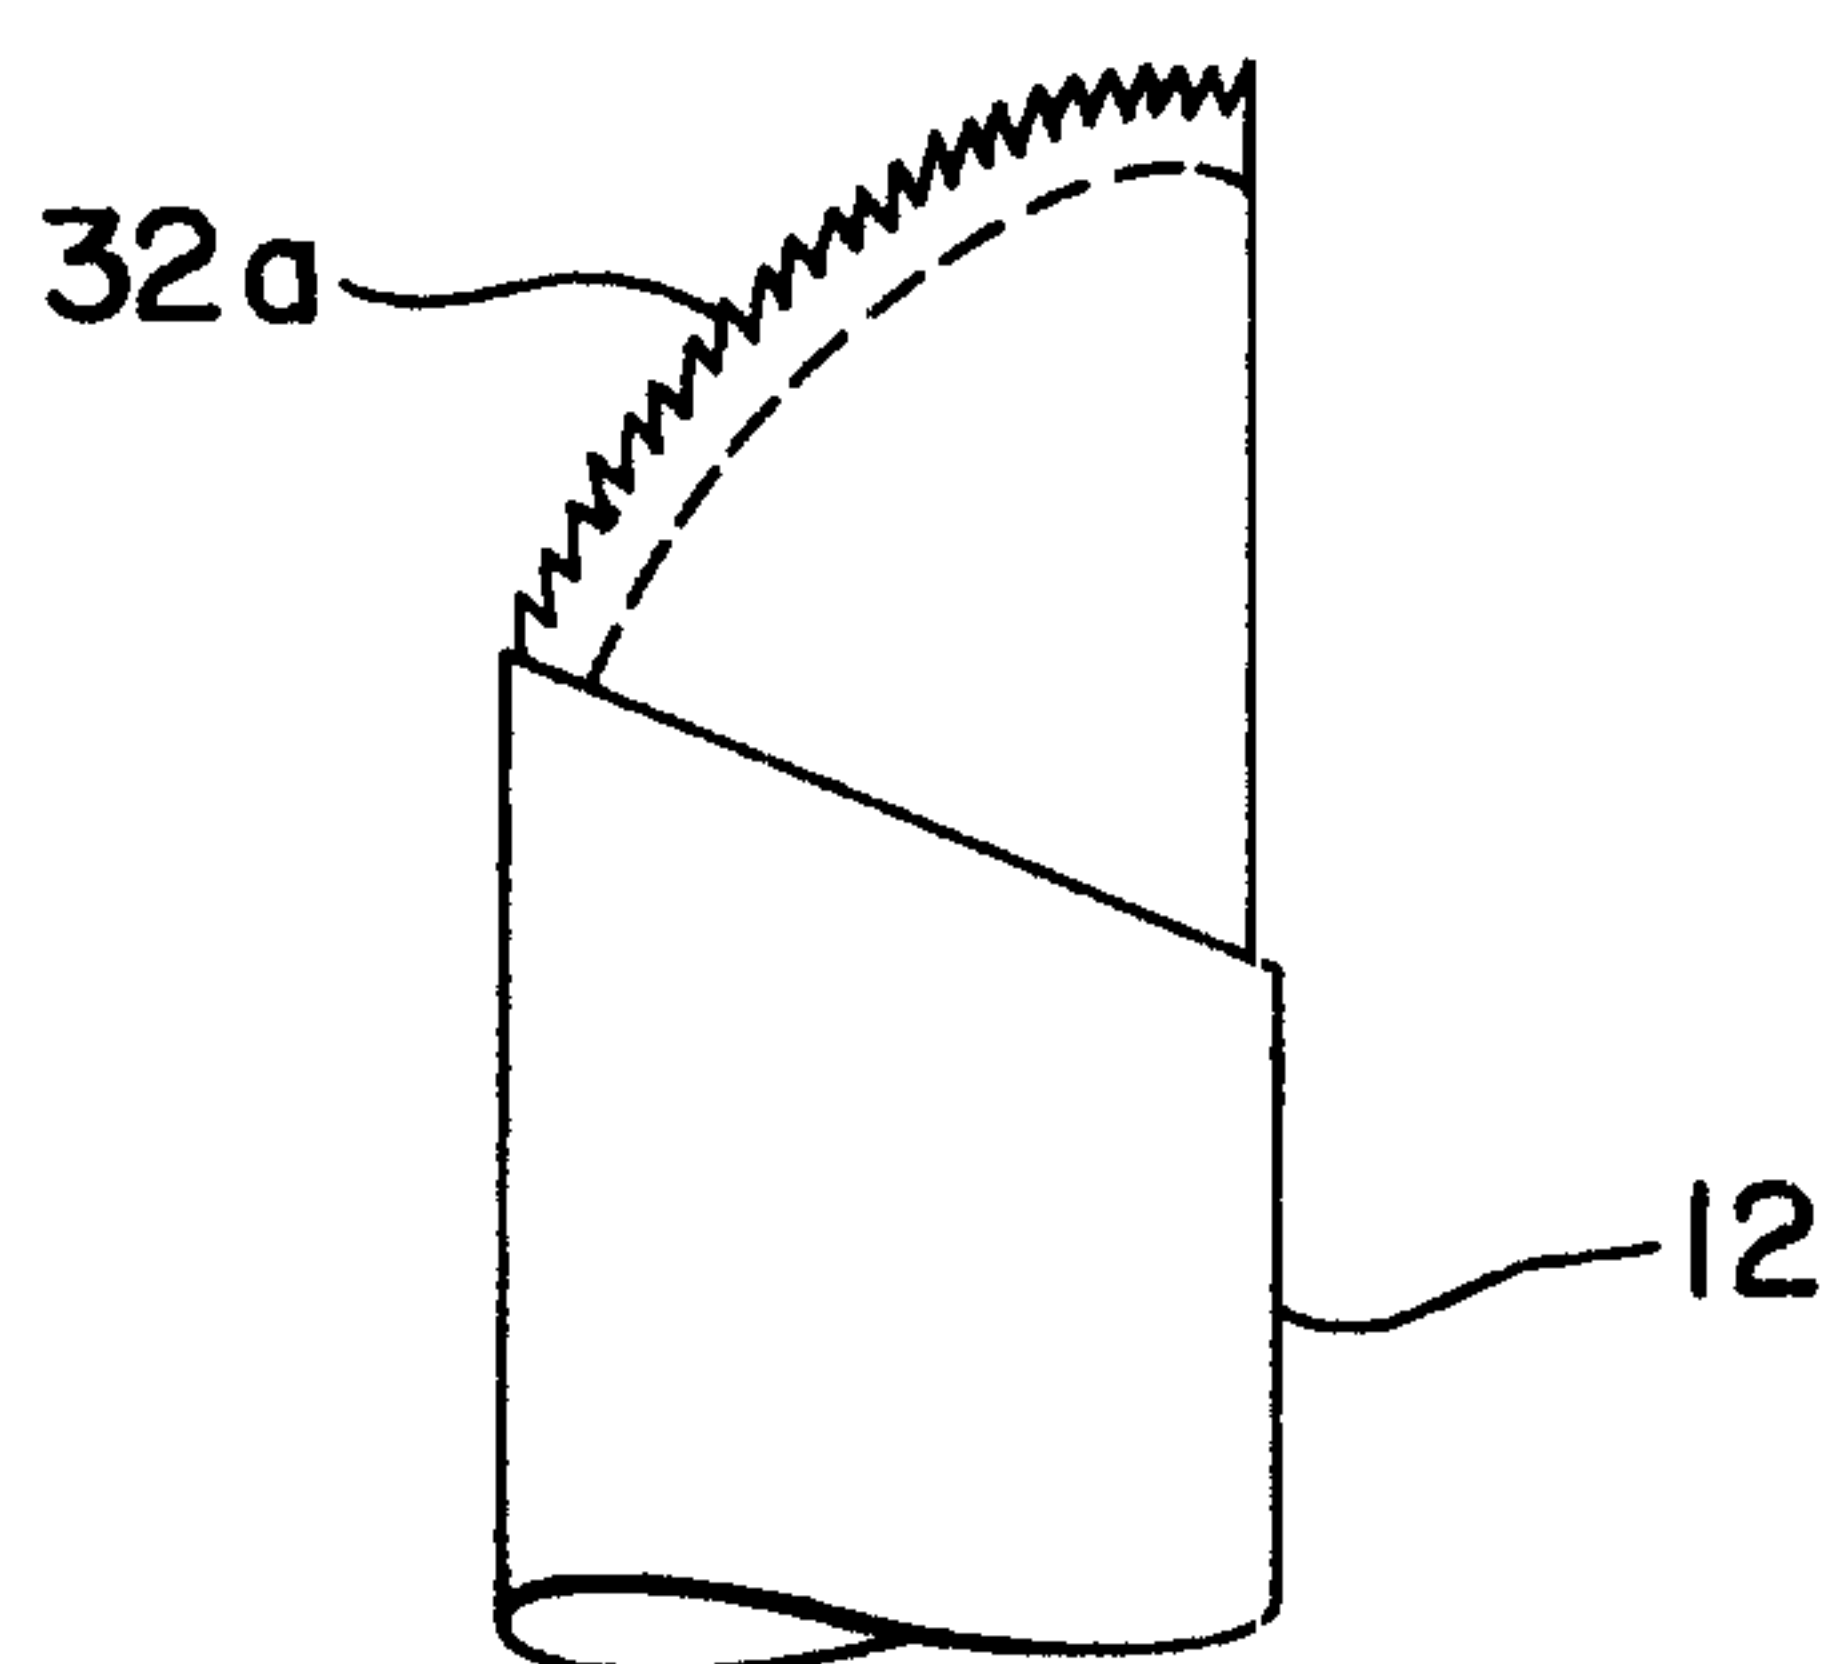


FIG. 6B

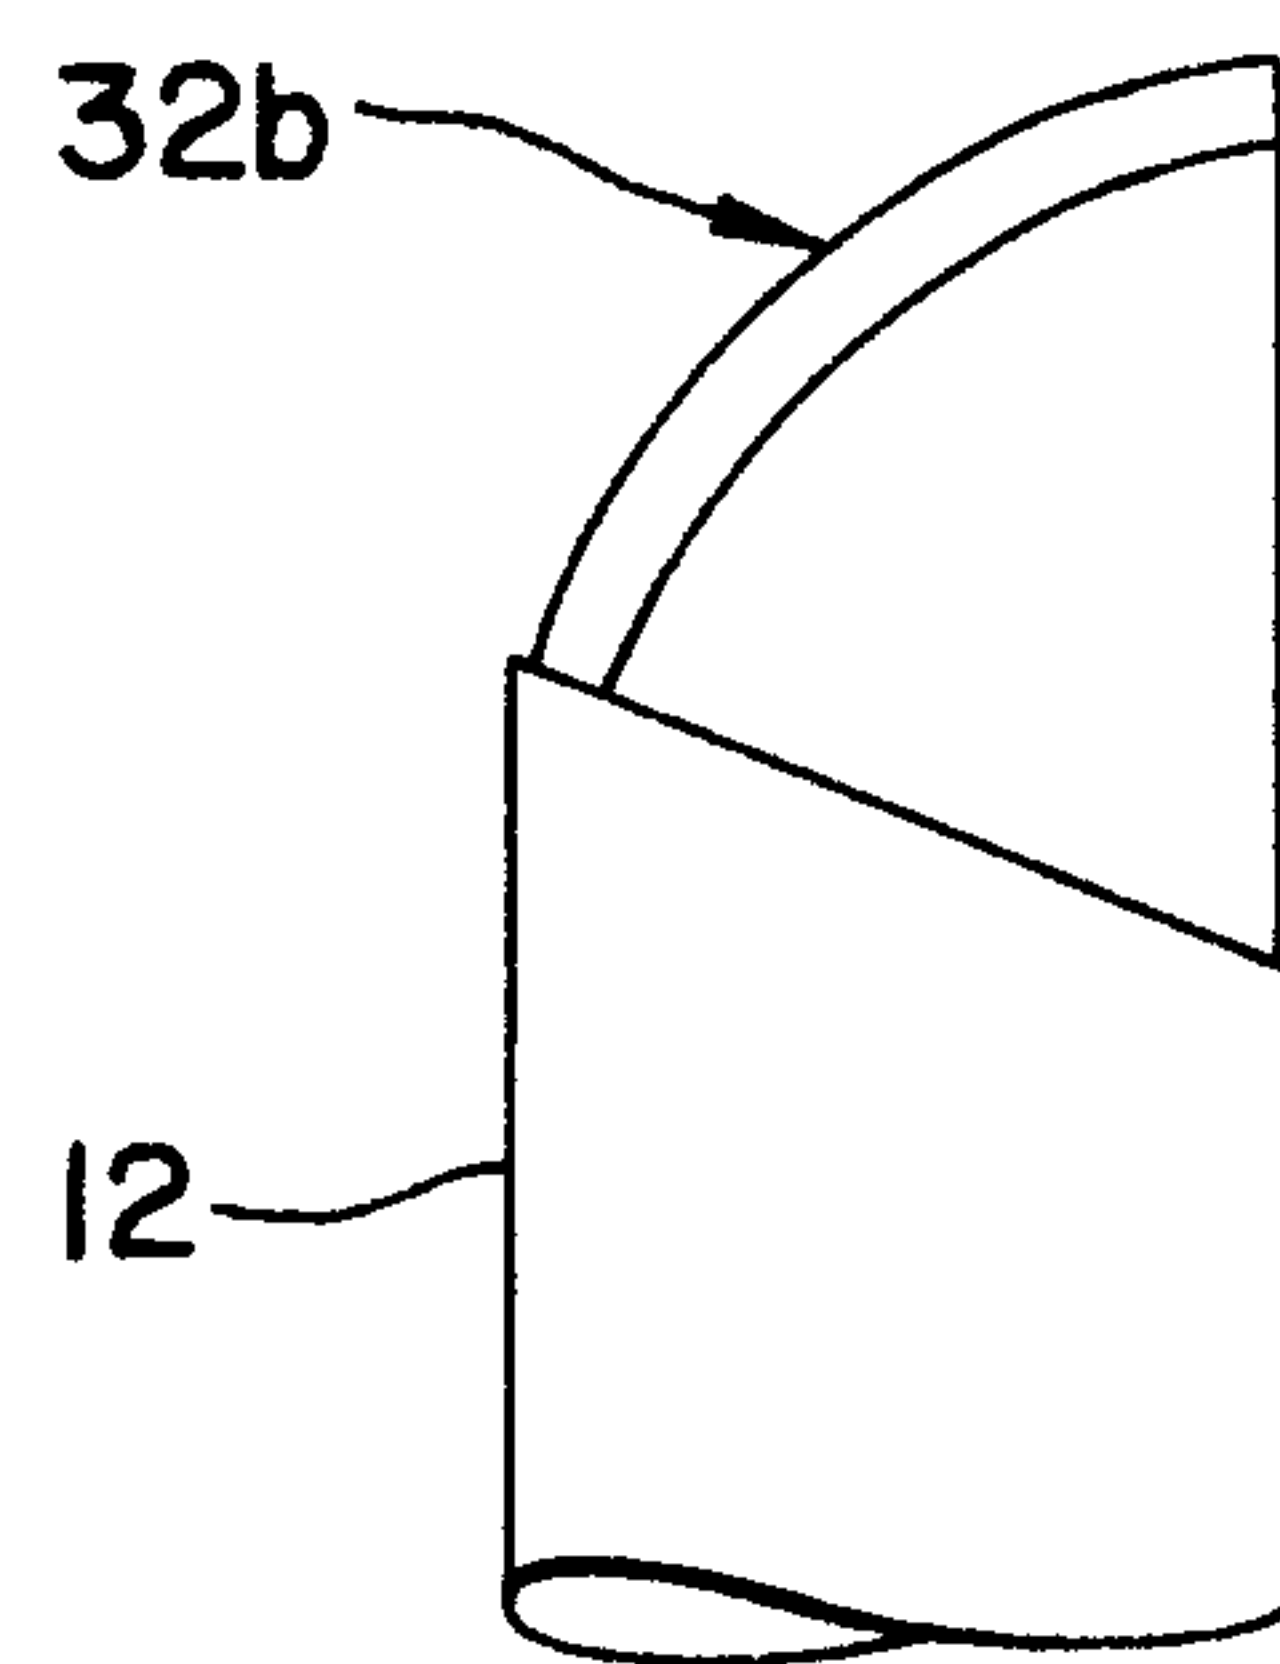


FIG. 7A

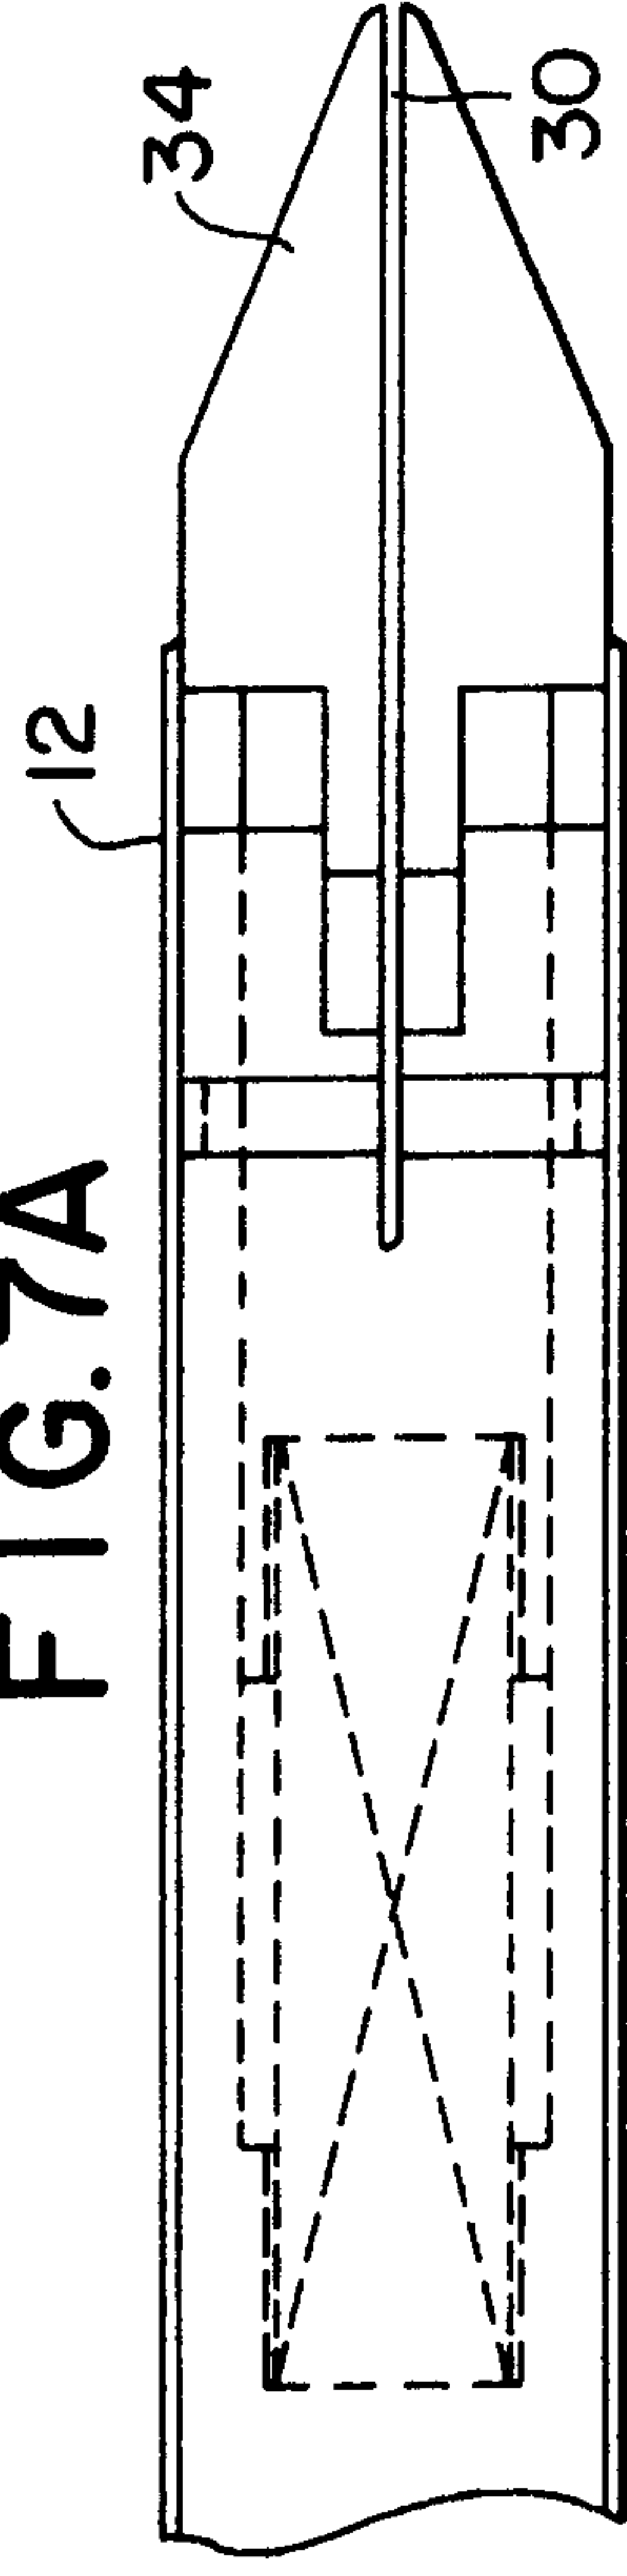


FIG. 7B


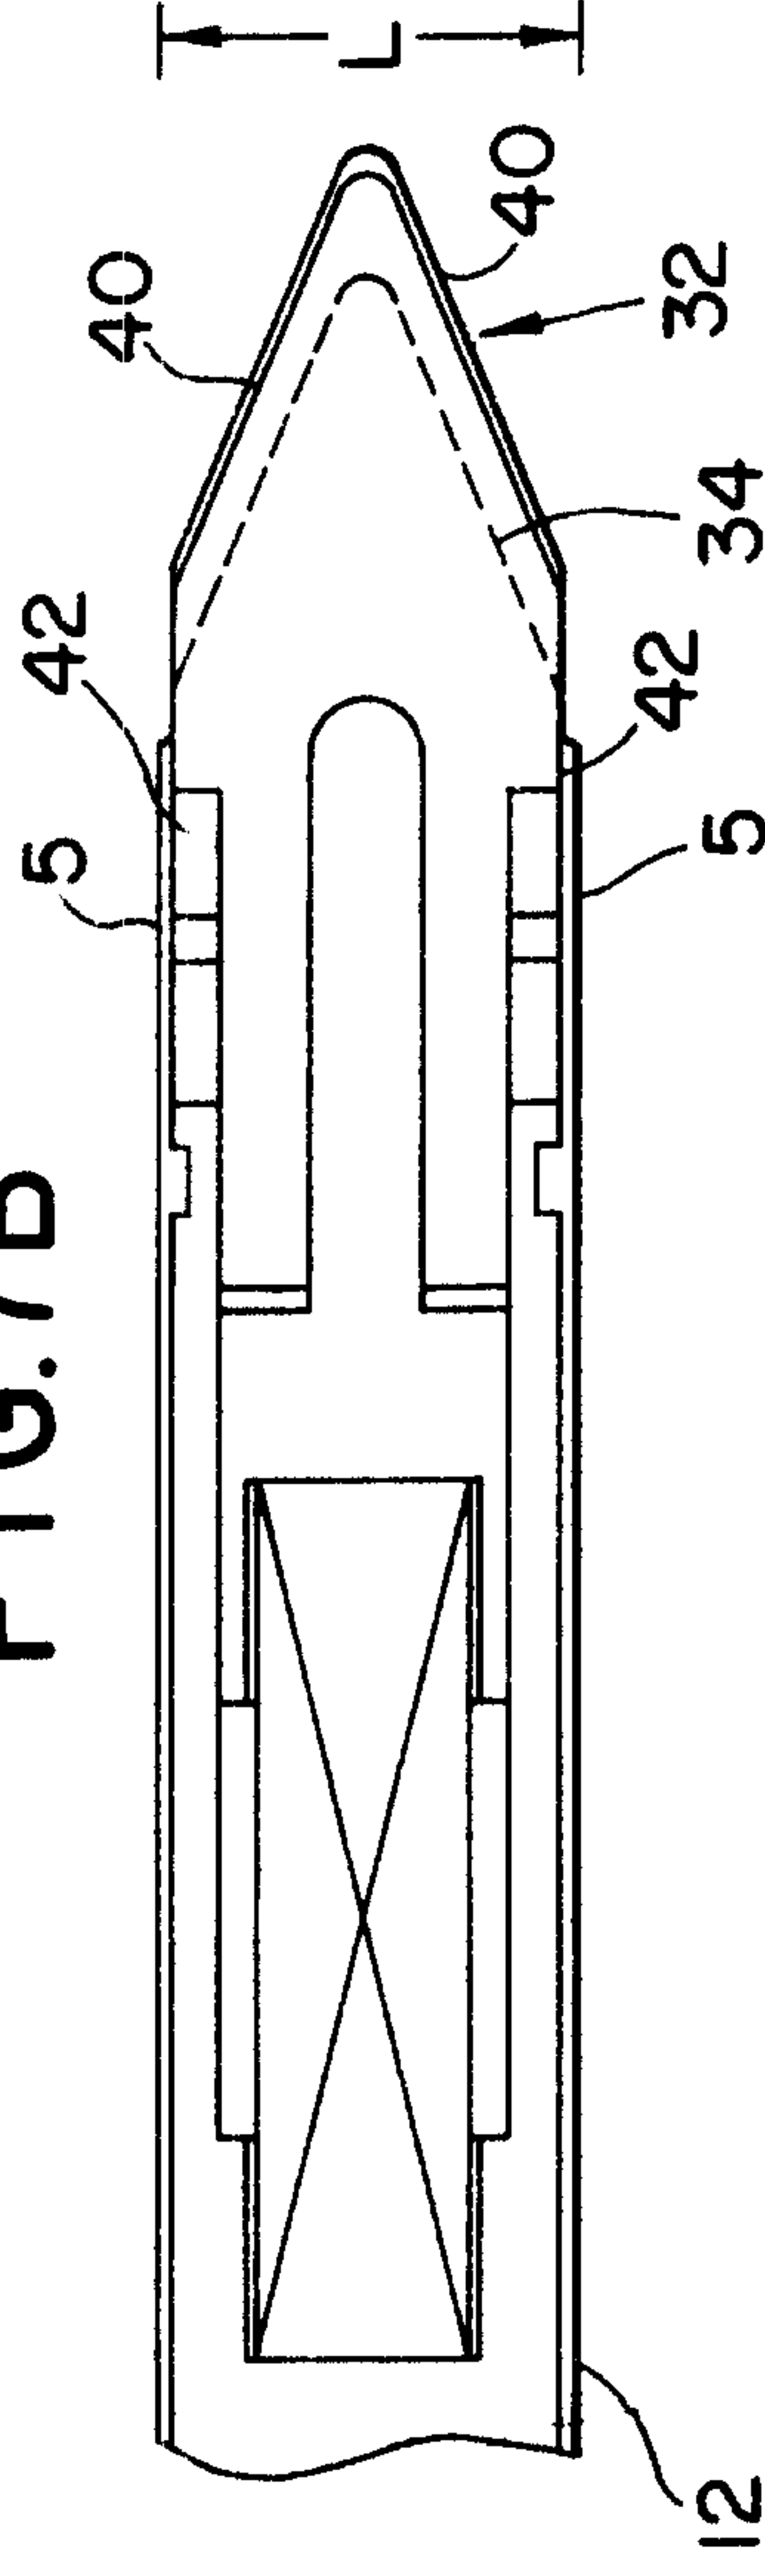


FIG. 8



2 1 1 1 8 8 5

Swasey Engineering Renault

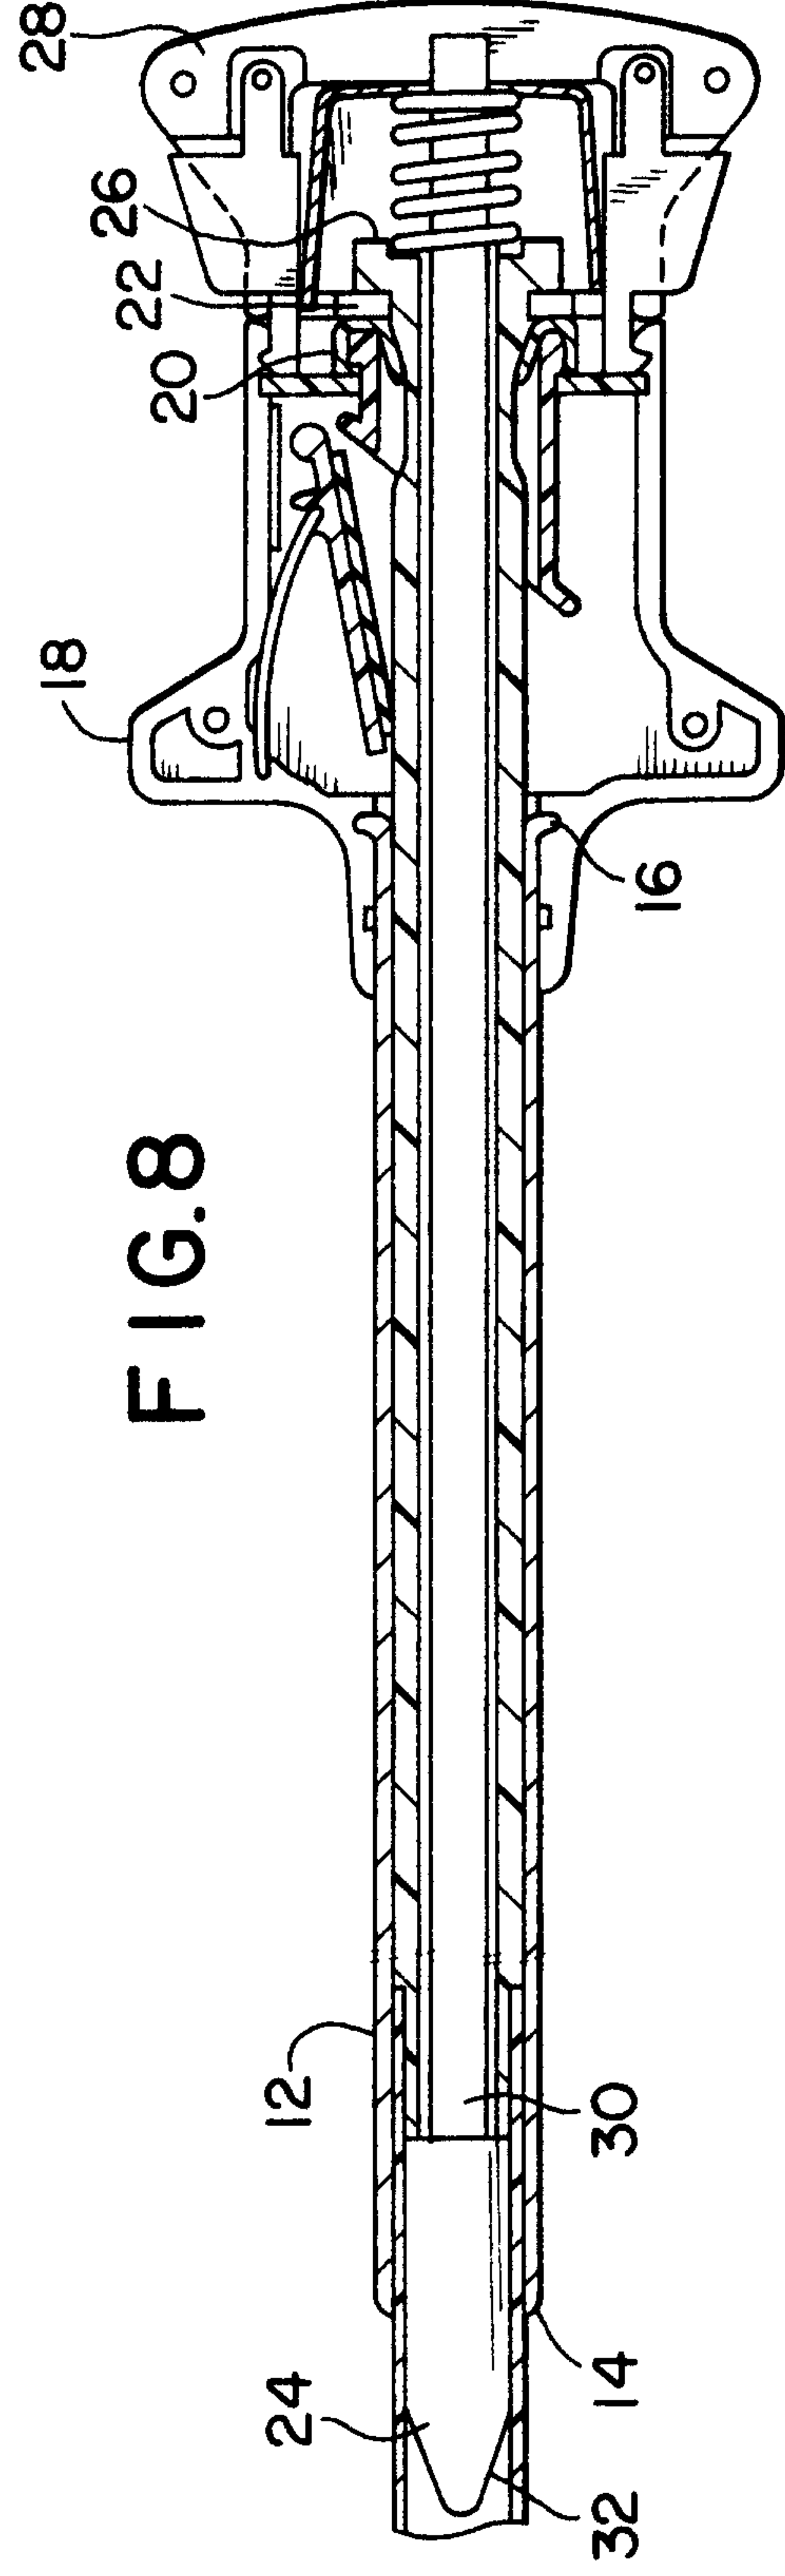