

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2018413357 B2**

(54) Title
Blood collection tube holder with single needle

(51) International Patent Classification(s)
A61B 5/145 (2006.01) **A61M 5/32** (2006.01)
A61B 5/15 (2006.01)

(21) Application No: **2018413357** (22) Date of Filing: **2018.12.14**

(87) WIPO No: **WO19/177674**

(30) Priority Data

(31) Number	(32) Date	(33) Country
16/219,094	2018.12.13	US
62/644,211	2018.03.16	US

(43) Publication Date: **2019.09.19**

(44) Accepted Journal Date: **2024.06.27**

(71) Applicant(s)
Retractable Technologies, Inc.; Thomas J. Shaw

(72) Inventor(s)
SHAW, Thomas J.; SMALL, Mark; ZHU, Ni

(74) Agent / Attorney
Davies Collison Cave Pty Ltd, Level 15 1 Nicholson Street, MELBOURNE, VIC, 3000, AU

(56) Related Art
WO 2018/009329 A1
US 2014/0276435 A1
US 2014/0276445 A1
US 5052403 A



(51) International Patent Classification:

A61B 5/145 (2006.01) A61M 5/32 (2006.01)
A61B 5/15 (2006.01)

(21) International Application Number:

PCT/US2018/065675

(22) International Filing Date:

14 December 2018 (14.12.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/644,211 16 March 2018 (16.03.2018) US
16/219,094 13 December 2018 (13.12.2018) US

(71) Applicant: **RETRACTABLE TECHNOLOGIES, INC.**
[US/US]; 511 Lobo Lane, Little Elm, TX 75068 (US).

(72) Inventor; and

(71) Applicant: **SHAW, Thomas J.** [US/US]; 5310 Buena
Vista, Frisco, TX 75034 (US).

(72) Inventors: **SMALL, Mark**; 47442 Caughern Lane, Heavener, OK 74937 (US). **ZHU, Ni**; 4408 Brigade Ct., Plano, TX 75024 (US).

(74) Agent: **ROSS, Monty L.**; Ross Barnes LLP, 275 W. Campbell Rd., Ste. 210, Richardson, TX 75080 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,

(54) Title: BLOOD COLLECTION TUBE HOLDER WITH SINGLE NEEDLE

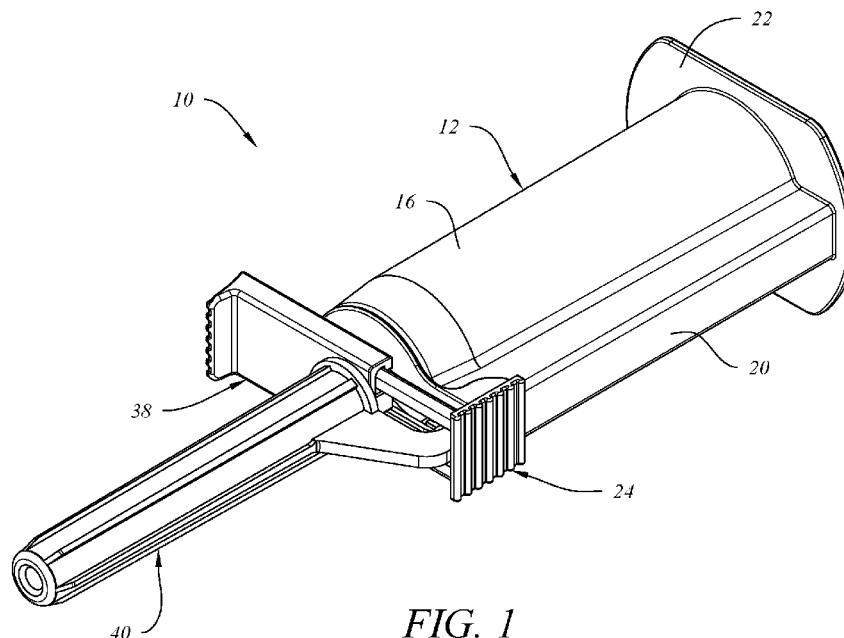


FIG. 1

(57) Abstract: A blood collection tube holder having a retractable single needle and a body comprising substantially parallel and laterally spaced apart barrel and needle retraction cavities separated by a partial wall that facilitates lateral movement of the single needle from the barrel cavity into alignment with the needle retraction cavity to initiate needle retraction. The barrel and a frontal attachment to the barrel are cooperatively configured to facilitate relative sliding movement between in a direction that is transverse to the longitudinal axis through the retractable single needle to initiate needle retraction.



UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

BLOOD COLLECTION TUBE HOLDER WITH SINGLE NEEDLE

1. Field

[0001] This disclosure relates to a medical device useful for drawing blood from person or animal. The subject device is often referred to as a “blood collection tube holder” or “blood tube holder.” because it is configured for use in combination with conventional, commercially available “blood collection tubes” or “blood tubes” that are manufactured and marketed by several different companies. The disclosure also relates to a single use blood collection tube holder having a single needle that is retractable into a confined space inside the device following use to protect a patient and healthcare workers from accidental needle sticks and thereby reduce the associated likelihood of pathogenic contamination resulting from an accidental stick. One aspect of the disclosure relates to a blood collection tube holder having a body comprising substantially parallel and laterally spaced apart barrel and needle retraction cavities separated by a partial wall that facilitates lateral movement of a retractable single needle from the barrel cavity into alignment with the needle retraction cavity to initiate needle retraction. Another aspect of the disclosure relates to a blood collection tube holder having a barrel and a frontal attachment that are cooperatively configured to facilitate relative sliding movement between them in a direction that is transverse to the longitudinal axis through the needle.

2. Description of Related Art

[0002] Conventional blood collection tube holders are disclosed, for example, in United States Patent Nos. 5,810,775; RE39,107; 8,496,600; 9,247,899 and in United States Publication Nos. 20160310057; 20180008180 and 2018/0008181.

[0003] Some such devices have two separate needles including a venipuncture needle pointing forwardly and a discharge needle pointing rearwardly. The discharge needle penetrates a stopper disposed in the front of a blood collection tube when the tube is inserted into the open rear end of a barrel. Following collection of a fluid sample, the blood collection tube is removed from the barrel of the blood tube holder, and a polymeric sheath expands to cover the rearwardly facing needle tip to prevent bodily

fluid from leaking out the open back of the barrel. In one such device, a hinged cap is provided at the back of the barrel, and closing the cap following removal of the blood collection tube triggers retraction of both the discharge needle and the venipuncture needle rearwardly into the barrel, whereby the device is rendered “safe” and non-reusable.

[0004] More recently, blood collection tube holders have been disclosed that comprise a longer, rearwardly biased single needle having both forwardly and rearwardly facing pointed ends. Following collection of a fluid sample and removal of the blood collection tube, needle retraction is initiated by depressing an actuator containing a needle retraction cavity that is moved to a position where it is sufficiently aligned with the needle that both ends of the needle are biased backwardly into the needle retraction cavity of the device, whereby the device is rendered “safe” and non-reusable.

[0005] Even more recently, blood collection tube holders have been disclosed that comprise separate venipuncture and discharge needles, and a retraction cavity for the venipuncture needle that is disposed beside and parallel to the barrel, either as a separate chamber that is made integrally with the barrel or as part of a frontal attachment to the barrel. The venipuncture needle is rearwardly biased and retraction of the venipuncture needle is initiated by transverse sliding movement of at least part of the frontal attachment to the barrel. During such movement the forwardly projecting venipuncture needle is moved laterally out of alignment with the rearwardly facing discharge needle into substantially coaxial alignment with the needle retraction cavity. Once the venipuncture needle is substantially aligned with the needle retraction cavity, the rearwardly directed biasing force causes the venipuncture needle to be withdrawn to a “safe” position inside the device while the discharge needle remains disposed in its original position inside the barrel. Either before or after needle retraction, the blood collection tube can be removed from the barrel, and an elastomeric sheath expands over the rearwardly facing tip of the discharge needle to prevent bodily fluid from leaking out the open rear end of the barrel.

[0006] Notwithstanding the improvements and advantages achieved through use of the previously disclosed devices, a blood collection tube hold may be provided

that comprises a single needle which can be retracted following use by lateral sliding movement of a frontal attachment relative to the barrel to reposition the whole needle into substantially coaxial alignment with a full-length needle retraction cavity that is made integrally with the barrel.

SUMMARY OF THE INVENTION

[0006A] According to the present invention, there is provided a blood collection tube holder, comprising:

- a body comprising a barrel and a needle retraction cavity, wherein the barrel and the needle retraction cavity are integrally formed, substantially parallel, and separated by a partial wall;

- a tube holder connector coupled to the barrel; and

- a rearwardly biased, retractable needle assembly comprising a single retractable needle having aoppositely directed venipuncture end extending forwardly from a slide member that slidably engages the tube holder connector and a fluid discharge needle ends extending rearwardly within the barrel;,,

- wherein lateral sliding movement of the slide member with respect to the tube holder connector and the barrel causes the fluid discharge end of the single needle to slide laterally past the partial wall until the single needle is aligned with the needle retraction cavity, which initiates retraction of the needle assembly within the needle retraction cavity.

[0006B] According to the present invention, there is provided a blood collection tube holder, comprising:

- a body comprising a barrel and an integrally formed needle retraction chamber;

- a tube holder connector coupled to the barrel;

- a slide member that slidably engages the tube holder connector; and

- a retractable single needle comprising a venipuncture end and a fluid discharge end;

- wherein the barrel comprises a barrel cavity, and wherein the needle retraction chamber comprises a needle retraction cavity, and wherein the barrel cavity and the needle retraction cavity are disposed in a fixed, substantially parallel relationship and separated by a partial wall; and

- wherein the partial wall comprises a reduced height portion configured to allow lateral sliding movement of the fluid discharge end of the retractable single needle past the reduced height portion of the partial wall from a first position

where the retractable single needle is coaxially aligned with the barrel cavity to a second position where the retractable single needle is coaxially aligned with the needle retraction cavity to initiate retraction of the retractable single needle within the needle retraction cavity of the needle retraction chamber.

[0007] A blood collection tube holder is disclosed that comprises a substantially cylindrical body, a frontal attachment, and a retractable single needle comprising oppositely directed venipuncture and fluid discharge ends or tips. The body and the frontal attachment are cooperatively configured to facilitate sliding lateral movement of the body relative to the single needle prior to needle retraction. In one embodiment, the body further comprises a substantially cylindrical barrel cavity and an integrally formed needle retraction cavity that are substantially parallel and separated by a partial wall. The partial wall is desirably configured to facilitate sliding lateral movement of the fluid discharge end of the single needle from a first position where it is substantially centered inside of and coaxially aligned with the barrel cavity to a second position where it is substantially aligned with the needle retraction cavity. The barrel cavity is configured to receive and support a conventional blood collection tube in operative engagement with the fluid discharge end of the single needle.

[0008] The venipuncture end of the single needle projects forwardly from the frontal attachment and is desirably covered by a selectively releasable needle cap prior to use. The frontal attachment further comprises a tube holder connector that frictionally engages and partially covers the open front end of the barrel, and a slide member that slidably engages the tube holder connector along an axis that is substantially transverse to the longitudinal axis through the single needle. The slide member is configured to seat and support a rearwardly biased needle holder attached in fixed relation to the single needle. The tube holder connector further comprises a transverse slot that facilitates relative lateral movement of the single needle between the first and second positions when oppositely directed manual pressure is applied to the body and slide member for the purpose of substantially aligning the needle holder and needle retraction cavity to initiate retraction of the single needle into the needle retraction cavity. In one embodiment, the selectively releasable needle cap further comprises a locking arm that

prevents the slide member and the needle retraction cavity from becoming substantially aligned and thereby initiating retraction of the single needle prior to use.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] Embodiments of the present invention will now be described, by way of non-limiting example only, with reference to the accompanying drawings, in which:

FIG. 1 is a front perspective view of one embodiment of the blood collection tube holder;

FIG. 2 is a front perspective view of the blood collection tube holder of FIG. 1 with the needle cap removed;

FIG. 3 is a rear perspective view of the blood collection tube holder of FIG. 1;

FIG. 4 is a top plan view of a blood collection tube holder substantially as shown in FIGS. 1 and 3 except that indicia are also shown in dashed outline in FIG. 4;

FIG. 5 is a front view of the blood collection tube holder of FIG. 1 but rotated 90 degrees in a clockwise direction around its longitudinal axis;

FIG. 6 is a rear view of the blood collection tube holder of FIG. 5;

FIG. 7 is a top plan view of the blood collection tube holder of FIG. 4 with the needle cap removed;

FIG. 8 is a right side elevation view of the blood collection tube holder of FIGS. 1 and 3;

FIG. 9 is a left side elevation view of the blood collection tube holder of FIG. 1 rotated 180 degrees in a clockwise direction around its longitudinal axis;

FIG. 10 is a cross-sectional view taken along line A—A of FIG. 5;

FIG. 11 is an exploded perspective view of the blood collection tube holder of FIG. 1;

FIG. 12 is the blood collection tube holder of FIG. 7 with the venipuncture needle retracted;

FIG. 13 is the blood collection tube holder of FIG. 5 with the needle cover removed and the venipuncture needle retracted;

FIG. 14 is a cross-sectional view taken along line C—C of FIG. 13;

FIG. 15 is the blood collection tube holder of FIG. 2 with the needle retracted;

FIG. 16 is an enlarged detail view of the needle support member of FIG. 11;

FIG. 17 is a rear perspective view of the needle support member of FIG. 16 rotated 180 degrees in a clockwise direction around the longitudinal axis through the subject blood collection tube holder;

FIG. 18 is an enlarged detail view of the tube holder connector of FIG. 11;

FIG. 19 is a rear perspective view of the tube holder connector of FIG. 18 rotated 180 degrees in a clockwise direction around the longitudinal axis through the subject blood collection tube holder; and

FIG. 20 is an enlarged cross-sectional view taken along line B—B of FIG. 4.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0010] Referring to FIGS. 1-11, blood collection tube holder 10 comprises body 12, a frontal attachment further comprising tube holder connector 24 and slide member 38, needle cap 40 (FIGS. 1 and 3), and retractable single needle 30 (FIG. 2). Body 12 further comprises barrel 16, barrel cavity 14, needle retraction chamber 20 and rear flange 22 disposed around the rear opening of barrel 16. Referring to FIGS. 2 and 7, retractable single needle 30 projects forwardly from needle support member 46 of slide member 38 of the frontal attachment.

[0011] Referring to FIGS. 4-6 and 8-10, blood collection tube holder 10 is depicted in its pre-use position in which selectively removable needle cap 40 is installed over retractable single needle 30 and frictionally engages axially extending, circumferentially spaced ribs disposed around needle support member 46 (visible in FIG. 7). Locking support arm 42 (visible in FIGS. 10-11) is provided to prevent relative sliding movement between body 12 and slide member 38 prior to using retractable single needle 30 to draw blood from a patient. Slide member 38 further comprises front surface 44 from which needle support member 46 projects forwardly around part of retractable single needle 30 as best seen in FIG. 7.

[0012] Referring to FIGS. 10-11, retractable single needle 30 further comprises forwardly facing venipuncture end 32 and rearwardly facing fluid discharge end 34. Prior to insertion of a blood collection tube (not shown) into barrel cavity 14 and use of blood collection tube holder 10 for collecting blood from a patient, selectively releasable needle cap 40 is in place as discussed above, and collapsible elastomeric sheath 26 covers fluid discharge end 34 of retractable single needle 30 to shield fluid discharge end 34 from inadvertent contamination. When a blood collection tube is inserted into barrel cavity 14 of barrel 16 of body 12, sheath 26 is collapsed rearwardly around retractable single needle 30, allowing fluid discharge end 34 to penetrate an elastomeric stopper in the blood collection tube to establish fluid communication between venipuncture end 32 of retractable single needle 30 and the inside of the blood collection tube into which the drawn blood is discharged. When single retractable needle 30 is in its pre-use position as shown in FIG. 10, needle 30 is substantially

centered inside barrel cavity 14 and is laterally spaced apart from needle retraction cavity 76 inside needle retraction chamber 20 of body 12.

[0013] Referring again to FIGS. 10-11, retractable single needle 30 is desirably attached in fixed axial relation to needle holder 28, 92, which further comprises a rearwardly extending annular projection 94 provided for use in frictionally engaging the forwardly extending end of collapsible elastomeric sheath 26, which is preferably a rubber sleeve. A biasing member such as compressible coiled spring 36 is desirably seated inside bore 60 (FIG. 16) of needle support member 46 around a centrally disposed portion of needle 30 and the forwardly facing shaft portion of needle holder 26, and when compressed during assembly of blood collection tube holder 10, abuts and engages the front side of head 92 of needle holder 28. For so long as retractable single needle 30 remains in its forwardly projecting position, head 92 of needle holder 28 is biased rearwardly relative to the frontal attachment and body 12 of blood collection tube holder 10.

[0014] Referring to FIGS. 11,16-17 and 20, slide member 38 of the frontal attachment to body 12 (FIG. 7) further comprises opposed positioning blocks 54, 56 that are engageable with cooperatively configured head 92 of needle holder 28 (FIG. 11) to move needle holder 28 laterally as discussed below. Laterally extending top and bottom rails 50, 52, respectively, are cooperatively configured and slidably engageable with laterally extending top and bottom rails 68, 70 of tube holder connector 24. Referring to FIGS. 17-18, projections 96, 98 (FIG. 17) on slide member 38 are desirably provided to engage cooperatively configured and aligned recesses 100 (bottom recess not visible) of tube holder connector 24 to properly position retractable single needle 30 within slot 72 of tube holder connector 24 during assembly and use of blood collection tube holder 10. Referring to FIGS. 11,18-19, circumferentially extending arcuate ring 64 and cooperating circular wall 62 of tube holder connector 24 are provided to establish frictional engagement between tube holder connector 24 and the forwardly facing edge of barrel 16 of body 12. The frictional engagement is desirably sufficient that tube holder connector 24 remains attached to the front end of barrel 16 as oppositely directed pressure is applied to textured touch surfaces 74, 48 as discussed below.

[0015] FIGS. 5-6 and 13 further depict opposed flat edges 84, 86 in relation to opposed arcuate edges 88, 90 of flange 22 and the relative positions of slide member 38 and tube holder connector 24 whenever needle 30 is in the unretracted and retracted positions, respectively.

[0016] Referring to FIGS. 5 and 7-11, slide member 38 and tube holder connector 24 of the frontal attachment to body 12 are provided with textured touch pads 48, 74, respectively, to facilitate the application of oppositely directed manual pressure to each touch pad to produce lateral sliding movement of body 12 relative to slide member 34, needle holder 28, compression spring 36 and retractable single needle 30. This movement is desirably in a transverse direction that causes discharge needle end 34 of retractable single needle 30 to move laterally past reduced height portion 80 of partial wall 82 (FIG. 10) until needle 30 is substantially aligned with needle retraction cavity 76, which allows needle holder 28 and discharge needle end 34 to move rearwardly into needle retraction cavity 76 as compressed coil spring 36 expands to the position shown in FIG. 14. The length of retractable single needle 30 is desirably such that venipuncture end 32 of needle 30 is fully contained inside needle support member 46 of slide member 38 when in the position as shown in FIG. 14. FIGS. 12-15 depict blood collection tube holder 10 with retractable single needle 30 in the fully retracted position.

[0017] Other alterations and modifications of the invention will likewise become apparent to those of ordinary skill in the art upon reading this specification in view of the accompanying drawings, and it is intended that the scope of the invention disclosed herein be limited only by the broadest interpretation of the appended claims to which the inventor and/or Applicant are legally entitled.

[0018] Throughout this specification and the claims which follow, unless the context requires otherwise, the word "comprise", and variations such as "comprises" and "comprising", will be understood to imply the inclusion of a stated integer or step or group of integers or steps but not the exclusion of any other integer or step or group of integers or steps.

[0019] The reference in this specification to any prior publication (or information derived from it), or to any matter which is known, is not, and should not be taken as an

acknowledgment or admission or any form of suggestion that that prior publication (or information derived from it) or known matter forms part of the common general knowledge in the field of endeavour to which this specification relates.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. A blood collection tube holder, comprising:

a body comprising a barrel and a needle retraction cavity, wherein the barrel and the needle retraction cavity are integrally formed, substantially parallel, and separated by a partial wall;

a tube holder connector coupled to the barrel; and

a rearwardly biased, retractable needle assembly comprising a single needle having a venipuncture end extending forwardly from a slide member that slidably engages the tube holder connector and a fluid discharge end extending rearwardly within the barrel;

wherein lateral sliding movement of the slide member with respect to the tube holder connector and the barrel causes the fluid discharge end of the single needle to slide laterally past the partial wall until the single needle is aligned with the needle retraction cavity, which initiates retraction of the needle assembly within the needle retraction cavity.

2. A blood collection tube holder, comprising:

a body comprising a barrel and an integrally formed needle retraction chamber;

a tube holder connector coupled to the barrel;

a slide member that slidably engages the tube holder connector; and

a retractable single needle comprising a venipuncture end and a fluid discharge end;

wherein the barrel comprises a barrel cavity, and wherein the needle retraction chamber comprises a needle retraction cavity, and wherein the barrel cavity and the needle retraction cavity are disposed in a fixed, substantially parallel relationship and separated by a partial wall; and

wherein the partial wall comprises a reduced height portion configured to allow lateral sliding movement of the fluid discharge end of the retractable single needle past the reduced height portion of the partial wall from a first position where the retractable single needle is coaxially aligned with the barrel cavity to a second position where the

retractable single needle is coaxially aligned with the needle retraction cavity to initiate retraction of the retractable single needle within the needle retraction cavity of the needle retraction chamber.

3. The blood collection tube holder of claim 2, wherein the venipuncture end of the retractable single needle projects forwardly from a slide member that slidably engages the tube holder connector prior to retraction of the retractable single needle within the needle retraction cavity of the needle retraction chamber.

4. The blood collection tube holder of claim 2 or 3, wherein the venipuncture end of the retractable single needle is covered by a selectively releasable needle cap prior to use.

5. The blood collection tube holder of any one of the preceding claims, wherein the tube holder connector frictionally engages an open front end of the barrel.

6. The blood collection tube holder of claim 5, wherein the slide member slidably engages the tube holder connector along an axis that is substantially transverse to a longitudinal axis through the retractable single needle.

7. The blood collection tube holder of any one of the preceding claims, wherein the slide member comprises a needle support member that receives a spring to rearwardly bias a needle holder that secures in fixed relation the retractable single needle.

8. The blood collection tube holder of claim 6, wherein the tube holder connector comprises a transverse slot that facilitates relative lateral movement of the retractable single needle when oppositely directed manual pressure is applied to the tube holder connector and the slide member.

9. The blood collection tube holder of claim 4, wherein the selectively releasable needle cap comprises a locking arm that prevents the slide member and the needle

retraction cavity from becoming substantially aligned prematurely and thereby initiating needle retraction prior to use of the blood collection tube holder for drawing blood.

10. The blood collection tube holder of any one of claims 1 to 4 and 6 to 9, wherein the tube holder connector is frictionally engaged with an open front end of the barrel.

11. The blood collection tube holder of any one of the preceding claims, wherein the slide member and the tube holder connector slidably engage along a pair of cooperatively configured rails.

12. The blood collection tube holder of any one of the preceding claims, wherein the slide member and the tube holder connector comprise textured touch pads to facilitate application of oppositely directed manual pressure to laterally slide the slide member with respect to the tube holder connector and the barrel.

13. The blood collection tube holder of any one of the preceding claims, wherein the needle assembly comprises a needle holder that affixes the single needle in fixed relation to the needle holder.

14. The blood collection tube holder of claim 13, wherein the needle holder is rearwardly biased by a spring received within a needle support member of the slide member.

15. The blood collection tube holder of any one of the preceding claims, wherein the barrel and the needle retraction cavity are in fluid communication via a reduced height portion of the partial wall.

16. The blood collection tube holder of any one of the preceding claims, wherein the venipuncture end of the single needle is fully contained within a needle support member of the slide member when the needle assembly is retracted.

17. The blood collection tube holder of claim 16, wherein a needle holder of the needle assembly and the fluid discharge end of the single needle are received within the needle retraction cavity upon retraction of the needle assembly.

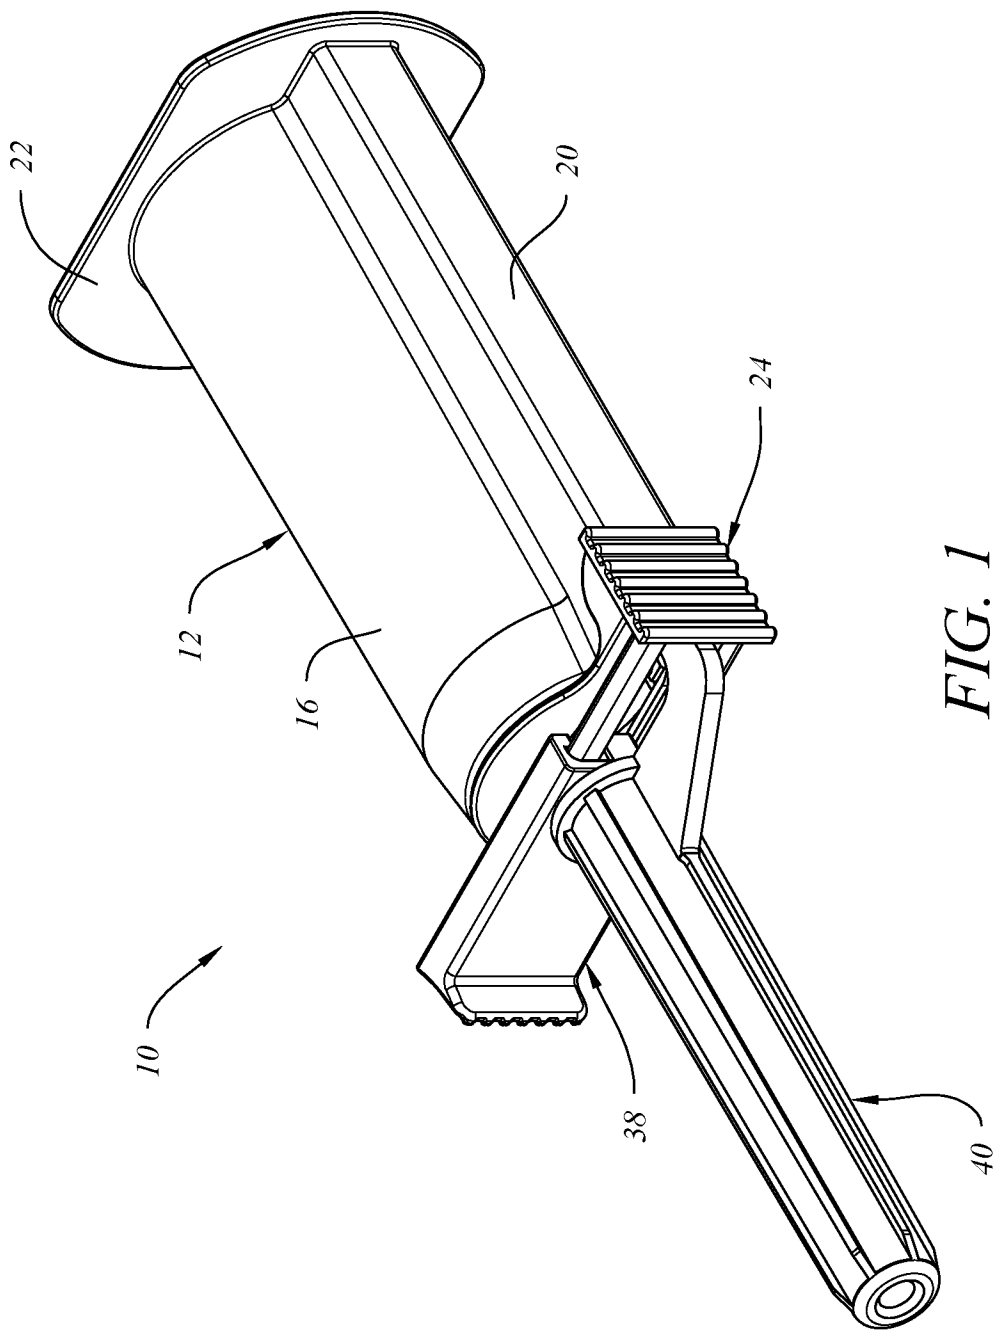


FIG. 1

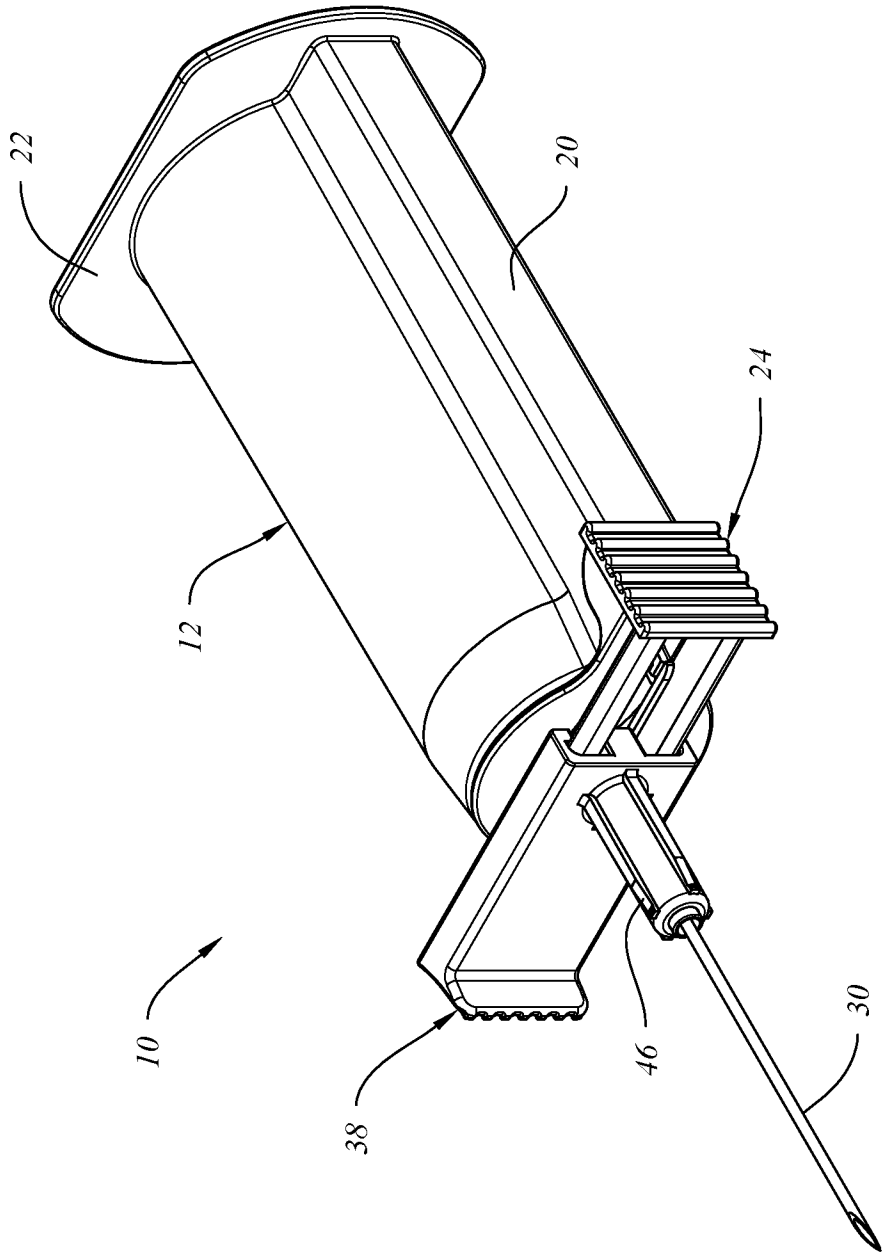
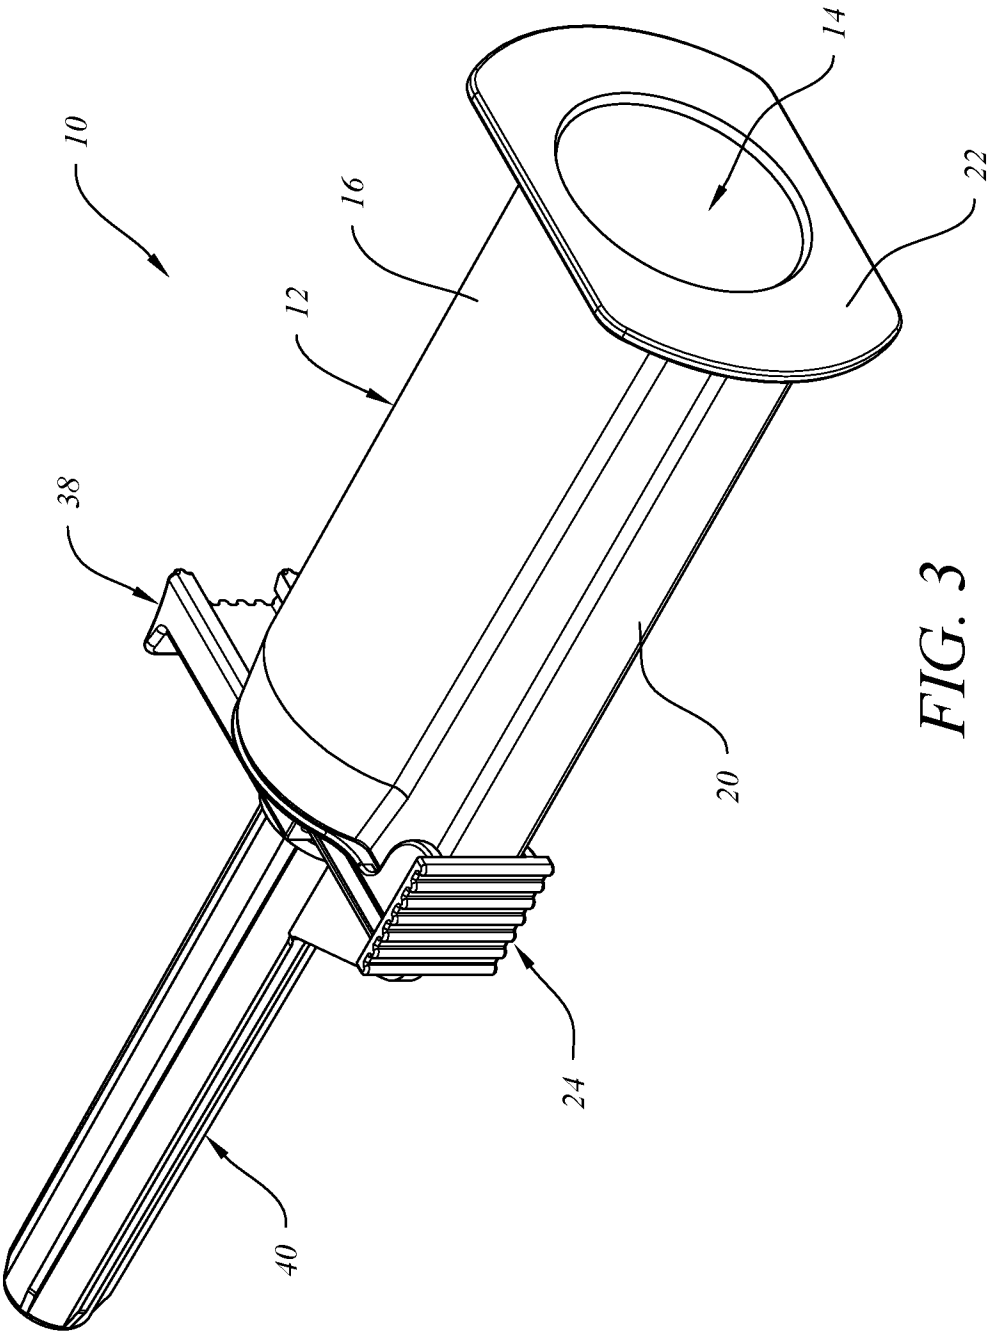


FIG. 2



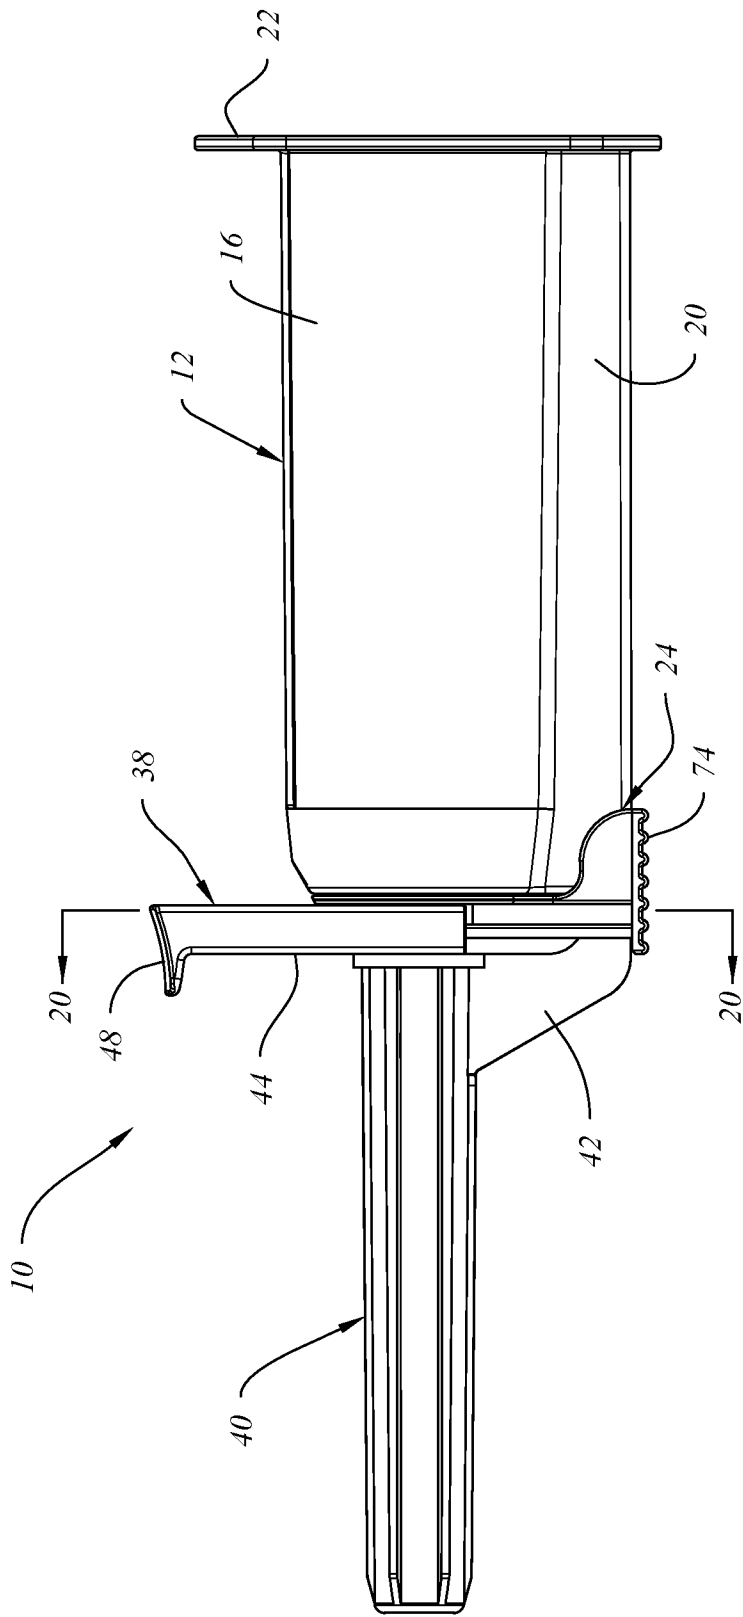


FIG. 4

5/13

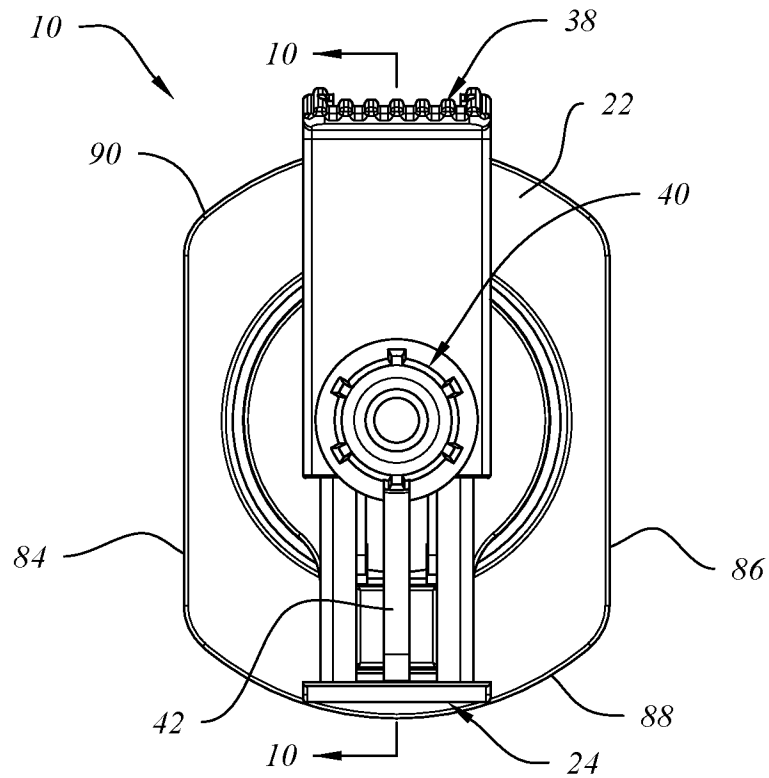


FIG. 5

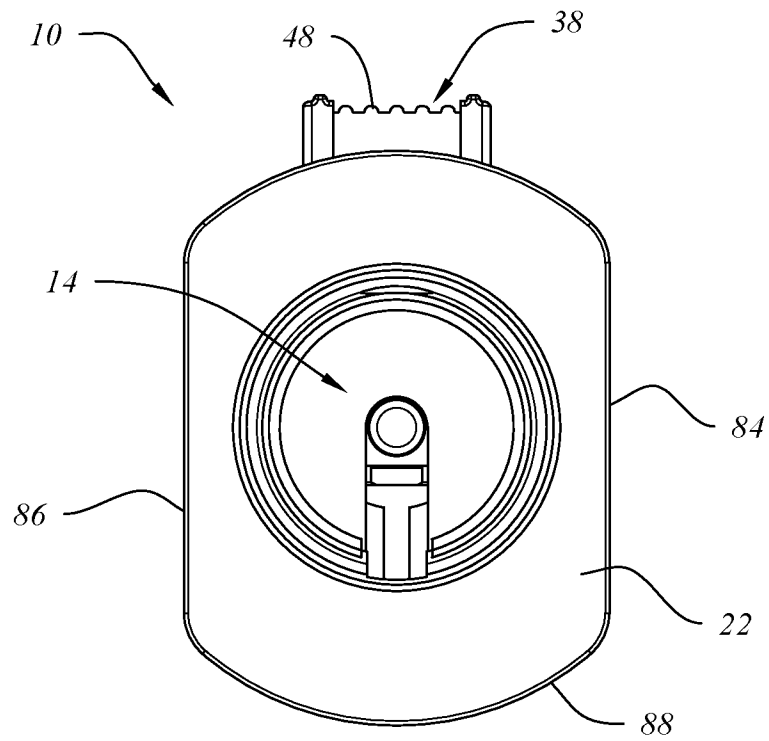
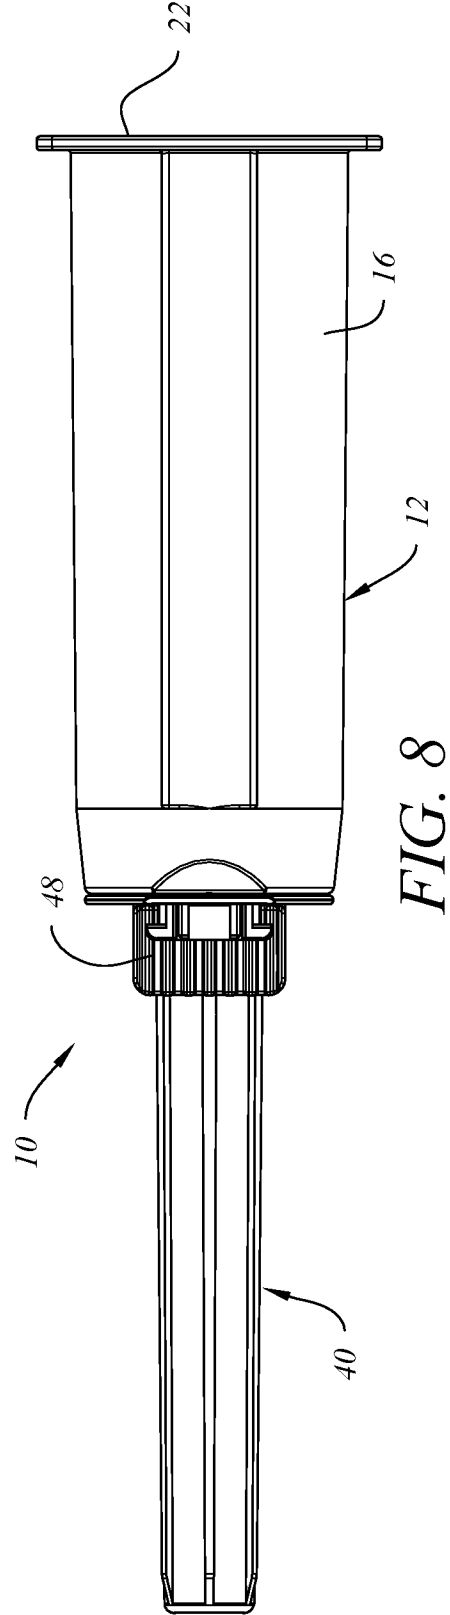
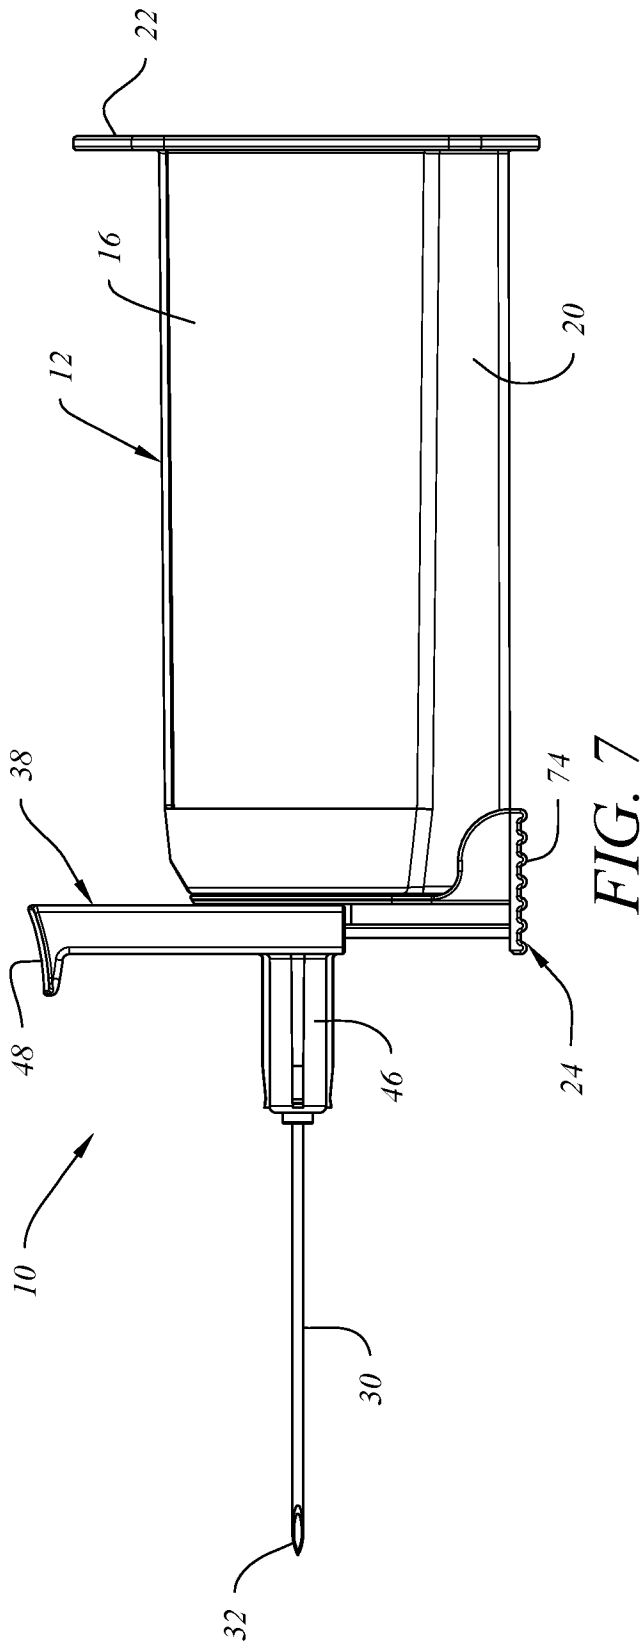


FIG. 6



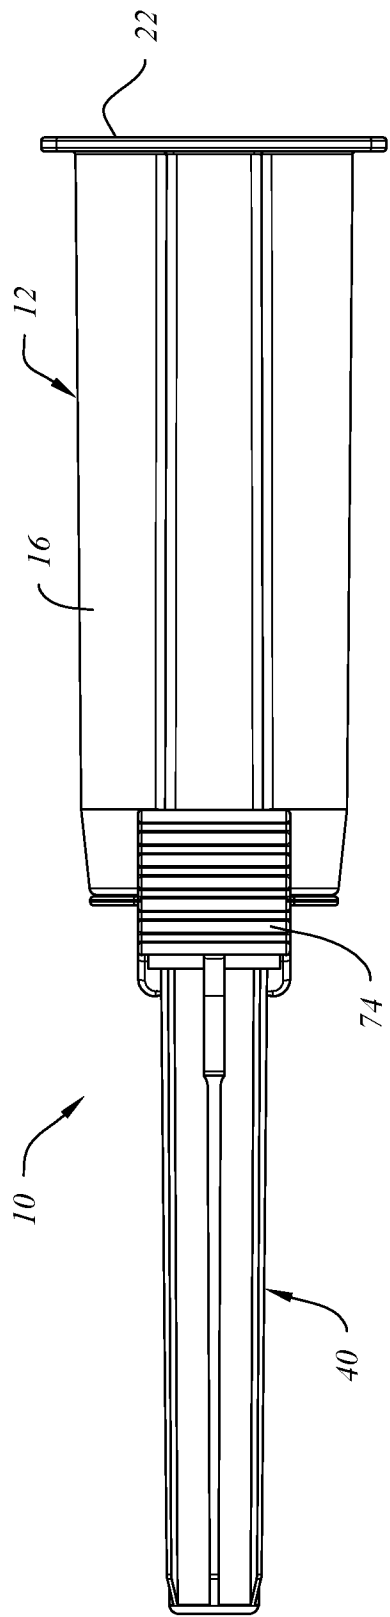


FIG. 9


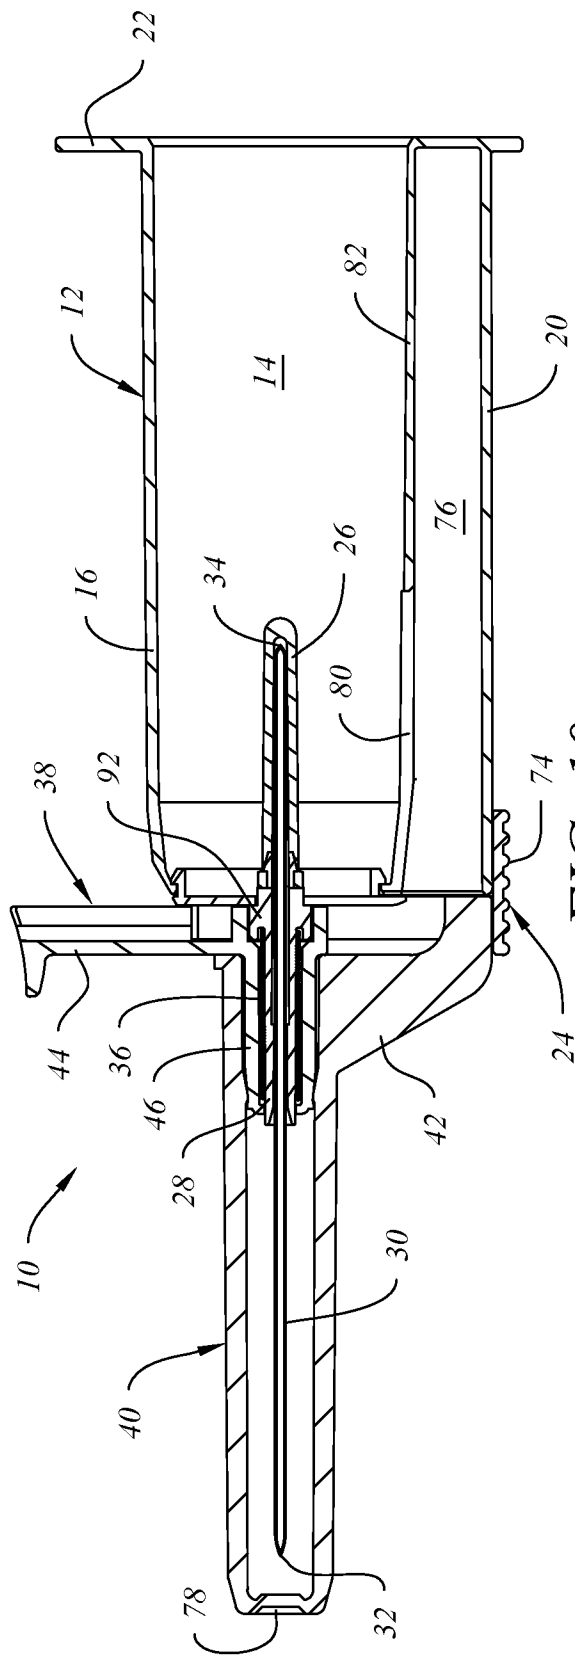


FIG. 10

8/13

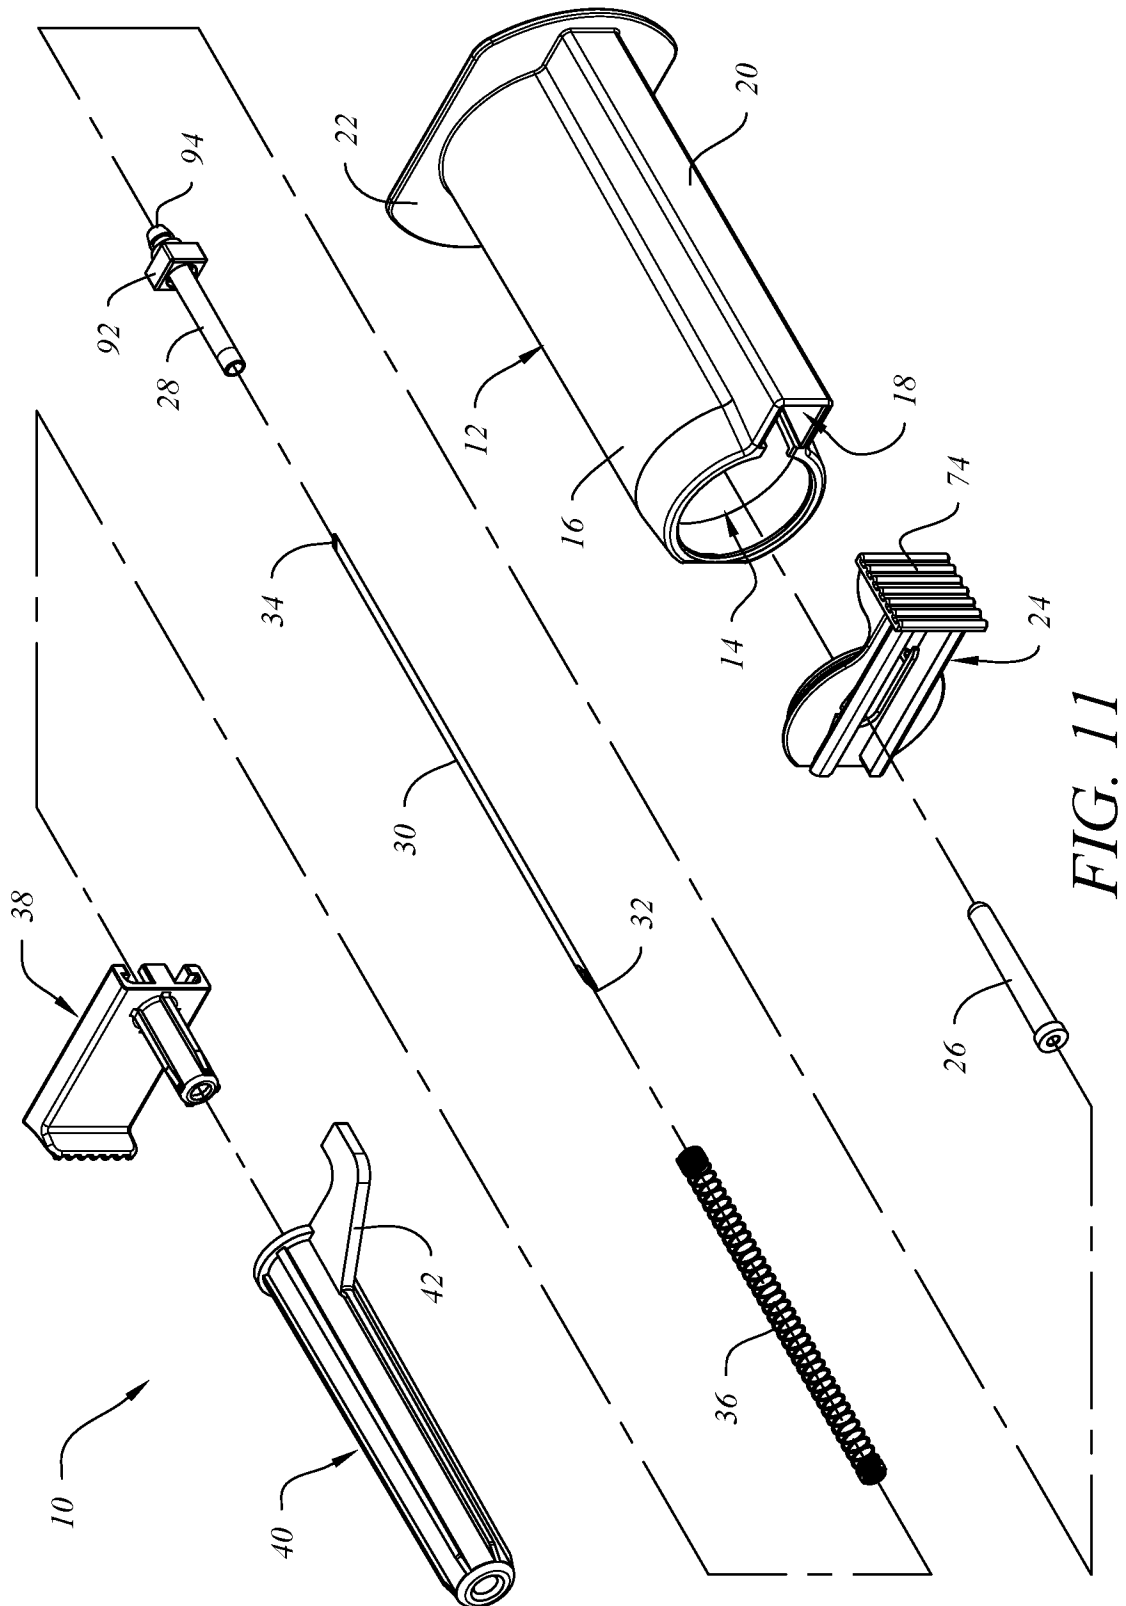

9/13

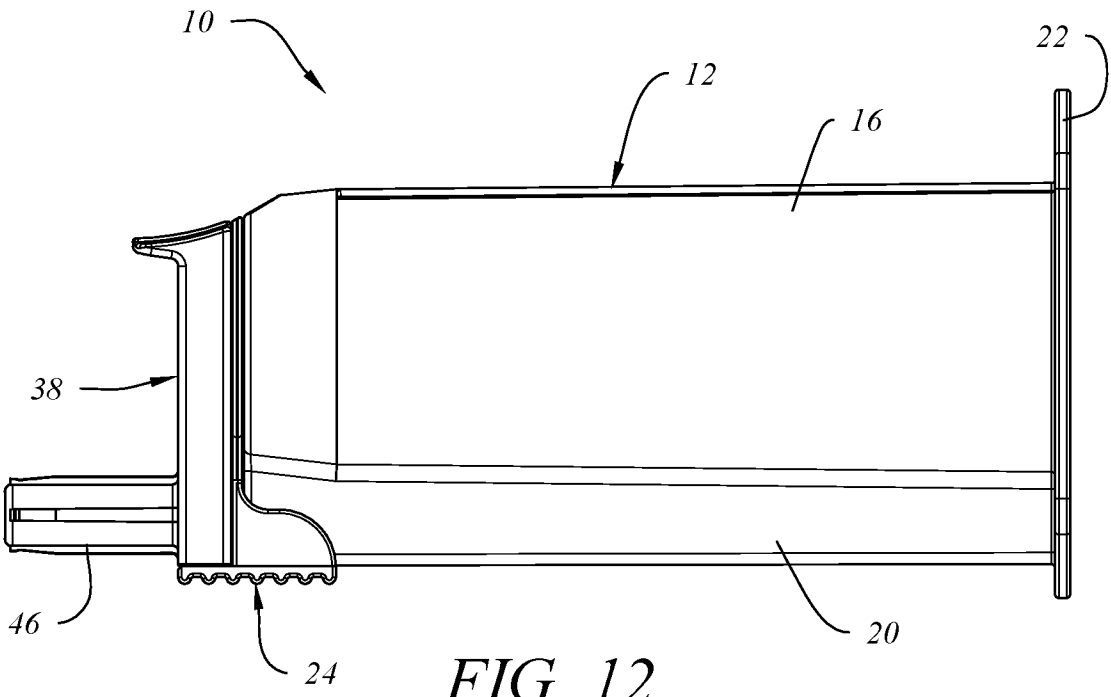


FIG. 12

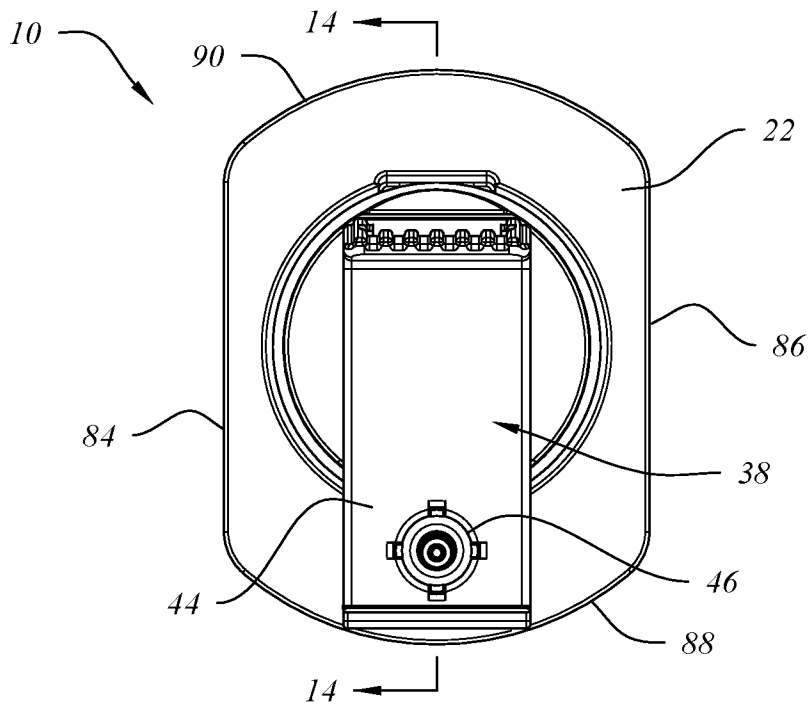


FIG. 13

10/13

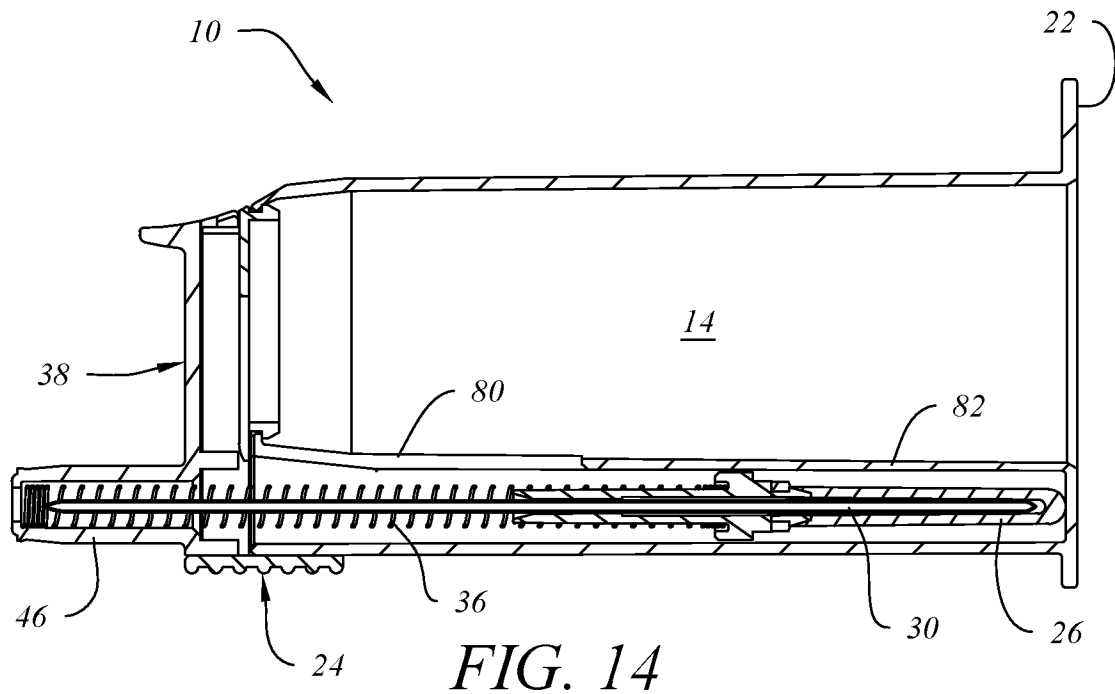


FIG. 14

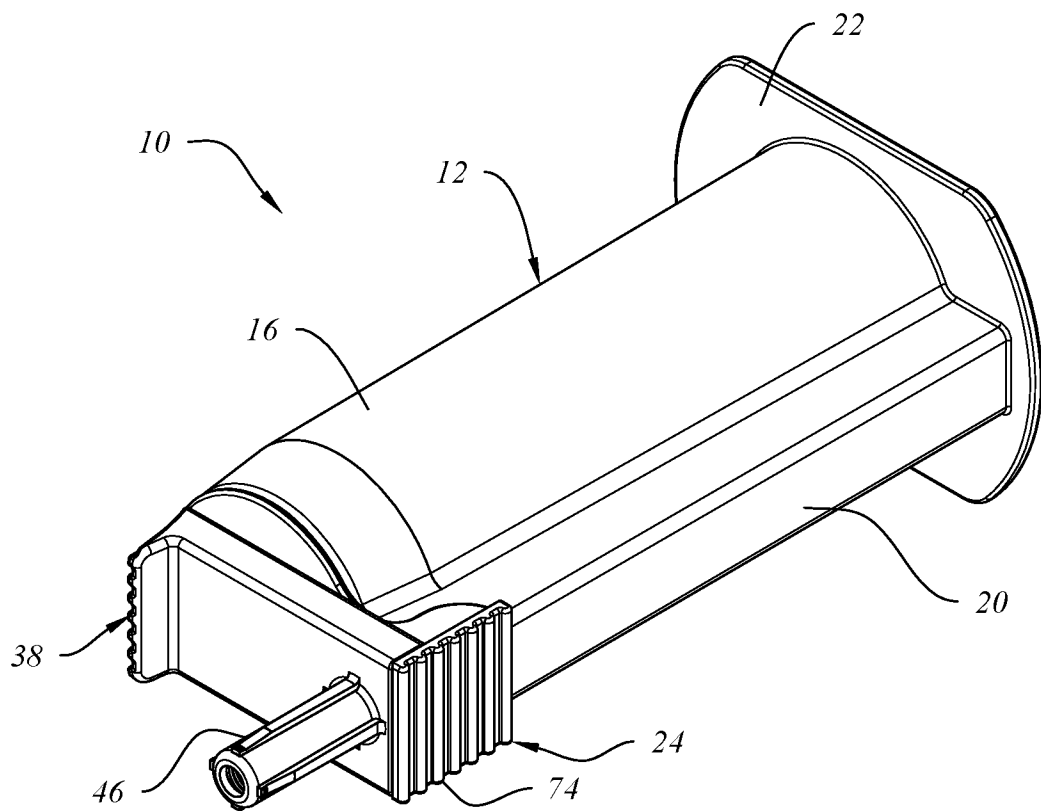


FIG. 15

11/13

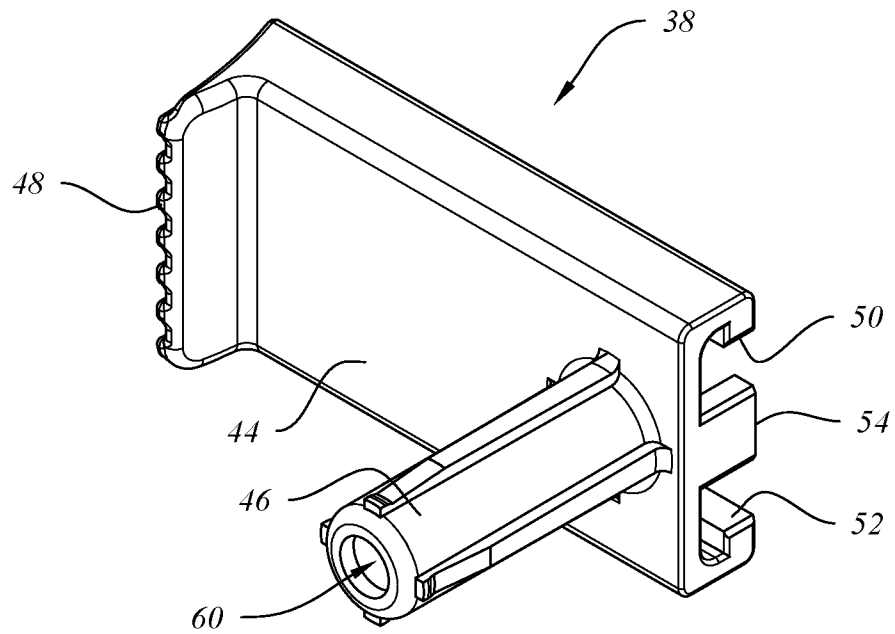


FIG. 16

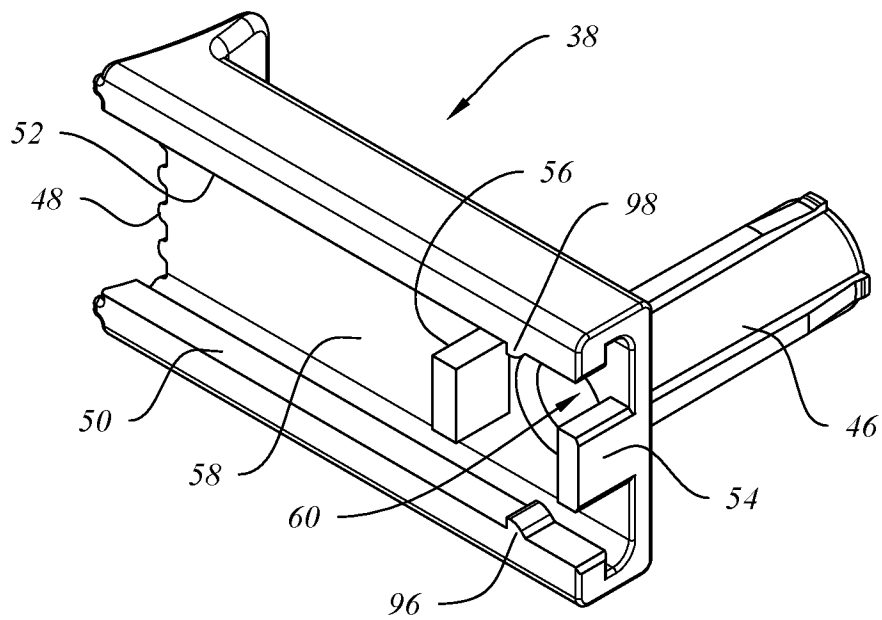


FIG. 17

12/13

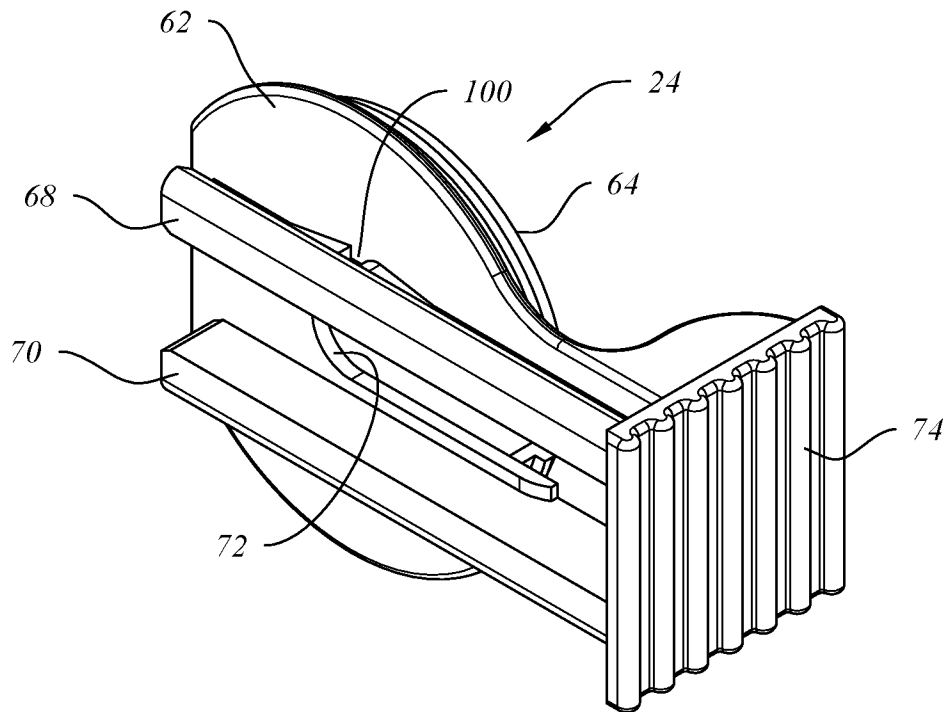


FIG. 18

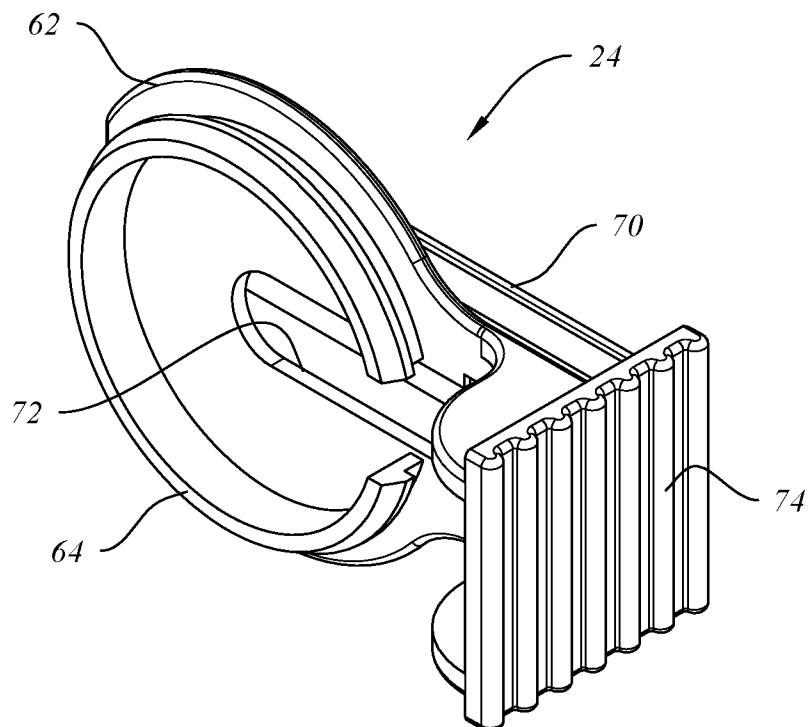


FIG. 19

13/13

