



US00D744359S

(12) **United States Design Patent**
Biselx et al.

(10) **Patent No.:** **US D744,359 S**

(45) **Date of Patent:** **** Dec. 1, 2015**

(54) **MICROMETER**

(71) Applicant: **TESA SA**, Renens (CH)

(72) Inventors: **Frédéric Biselx**, Yens (CH); **Stéphane Karawa**, Lausanne (CH)

(73) Assignee: **TESA SA**, Renens (CH)

(**) Term: **14 Years**

(21) Appl. No.: **29/492,829**

(22) Filed: **Jun. 3, 2014**

(30) **Foreign Application Priority Data**

Dec. 11, 2013 (WO) 780199301

(51) **LOC (10) Cl.** **10-04**

(52) **U.S. Cl.**
USPC **D10/73**

(58) **Field of Classification Search**
USPC D10/73
CPC G01B 3/20; G01B 3/205; G01B 3/24;
G01B 3/18; G01B 3/008; G01J 3/02; G01J
3/0208; G01J 3/0291; G01J 3/50; G01J 3/501;
G01J 3/0289; G01J 3/0243
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,255,861 A * 3/1981 Nakata et al. 33/819
D263,809 S * 4/1982 Suwa et al. D10/73
D273,468 S * 4/1984 Ueda et al. D10/73

D273,469 S * 4/1984 Ueda et al. D10/73
4,578,868 A * 4/1986 Sasaki et al. 33/819
5,433,016 A * 7/1995 Tachikake et al. 33/820
5,495,677 A * 3/1996 Tachikake et al. 33/784
5,691,646 A * 11/1997 Sasaki 324/662
5,920,198 A * 7/1999 Suzuki et al. 324/662
D429,172 S * 8/2000 Reymond D10/73
6,247,244 B1 * 6/2001 Zanier et al. 33/819
6,308,433 B1 * 10/2001 Takahashi et al. 33/819
D611,371 S * 3/2010 Ohtani et al. D10/73
2013/0276319 A1 * 10/2013 Tsuji 33/819

* cited by examiner

Primary Examiner — Antoine D Davis

(74) *Attorney, Agent, or Firm* — Maschoff Brennan

(57) **CLAIM**

The ornamental design for a micrometer, as shown and described.

DESCRIPTION

FIG. 1 is an upper perspective view of an exemplary micrometer;

FIG. 2 is a front view of the micrometer;

FIG. 3 is a rear view of the micrometer;

FIG. 4 is a bottom view of the micrometer;


FIG. 5 is a top view of the micrometer;

FIG. 6 is a left side view of the micrometer;

FIG. 7 is a front view of another exemplary micrometer, with the other views the same as shown above in connection with FIG. 1; and,

FIG. 8 is a front view of still another exemplary micrometer, with the other view the same as shown above in connection with FIG. 1.

1 Claim, 8 Drawing Sheets

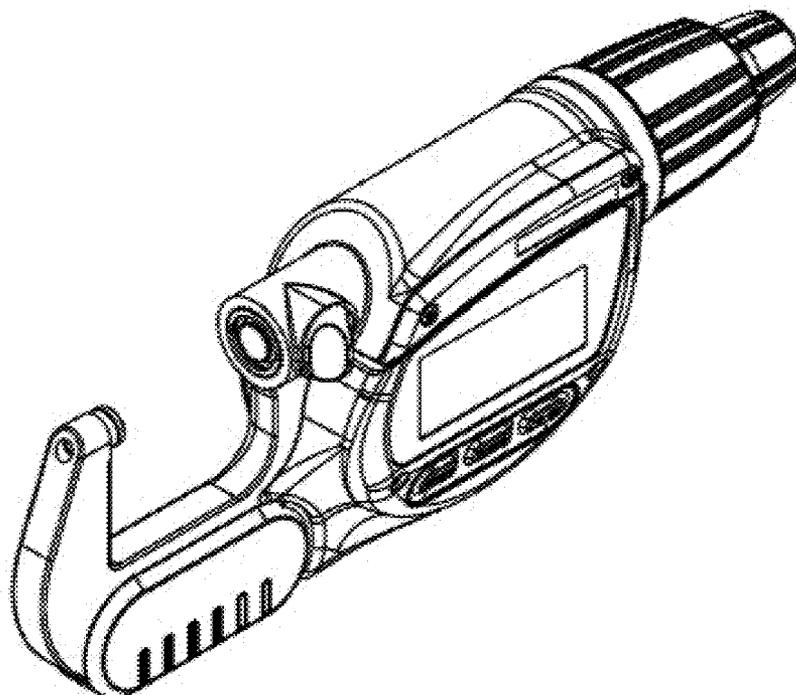

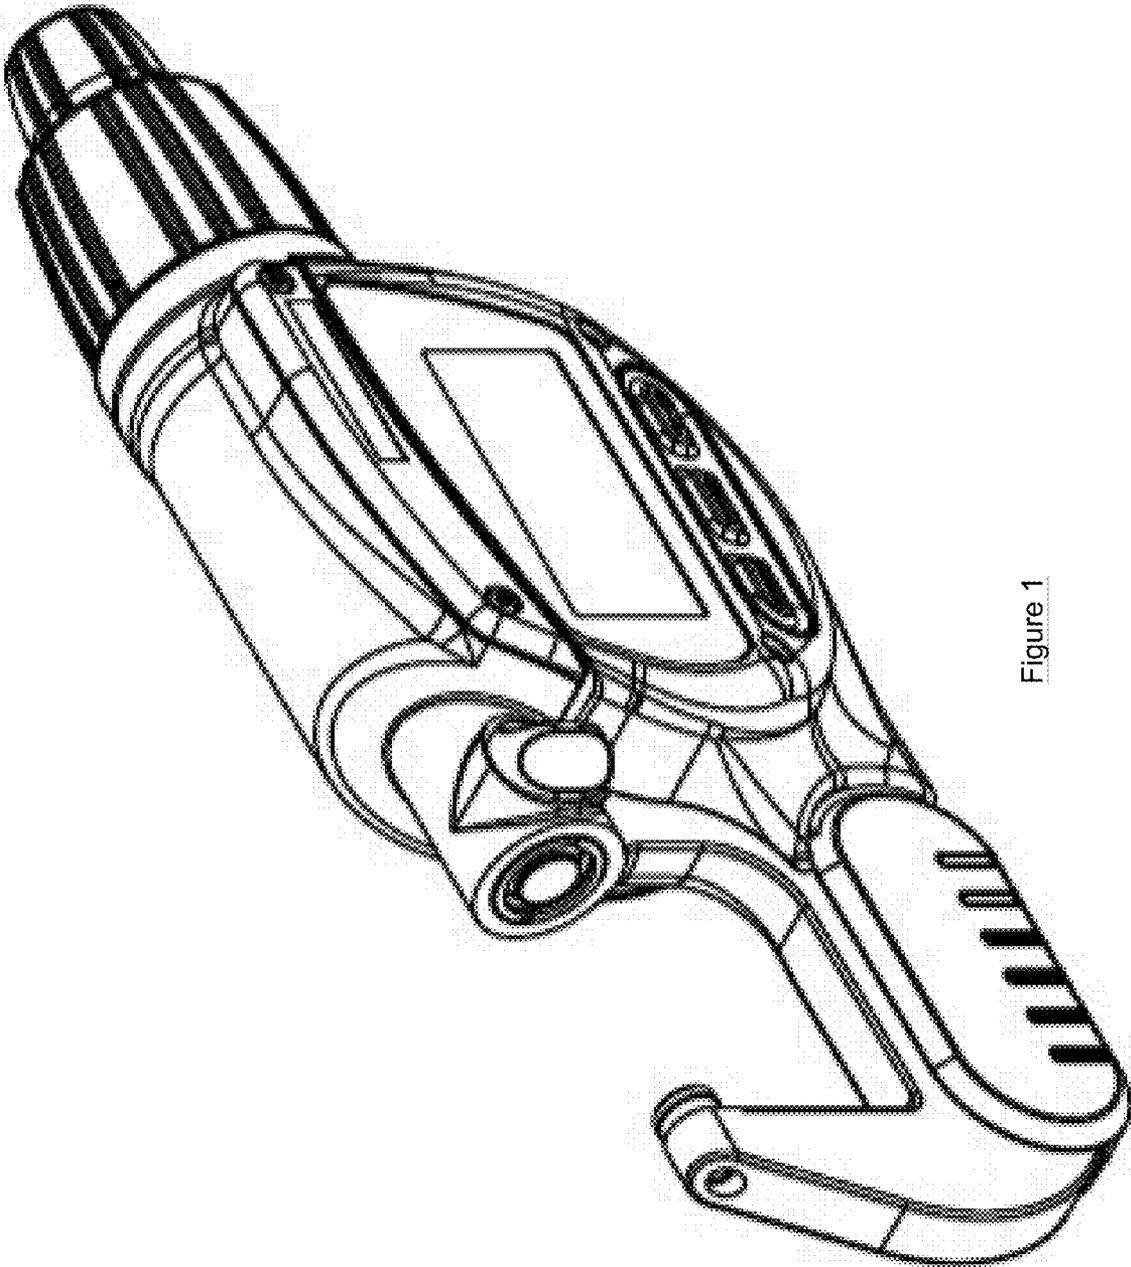


Figure 1

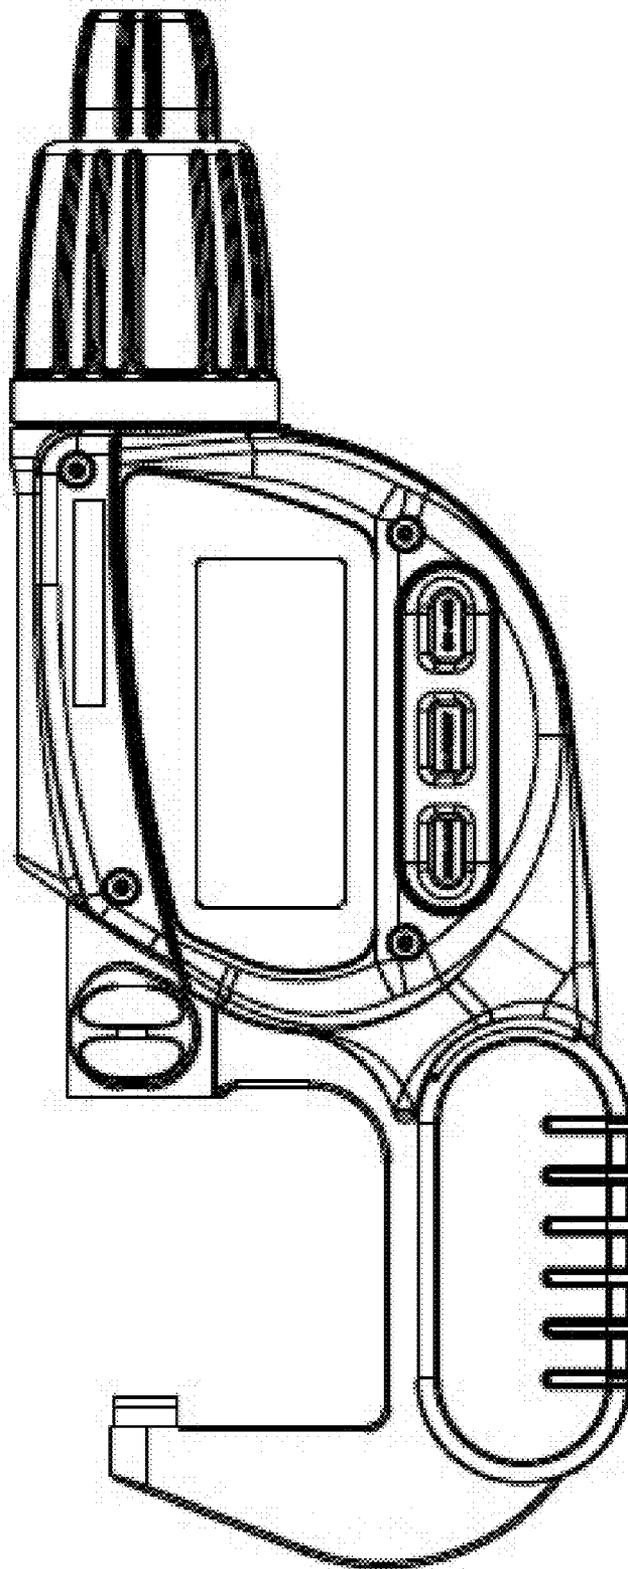


Figure 2

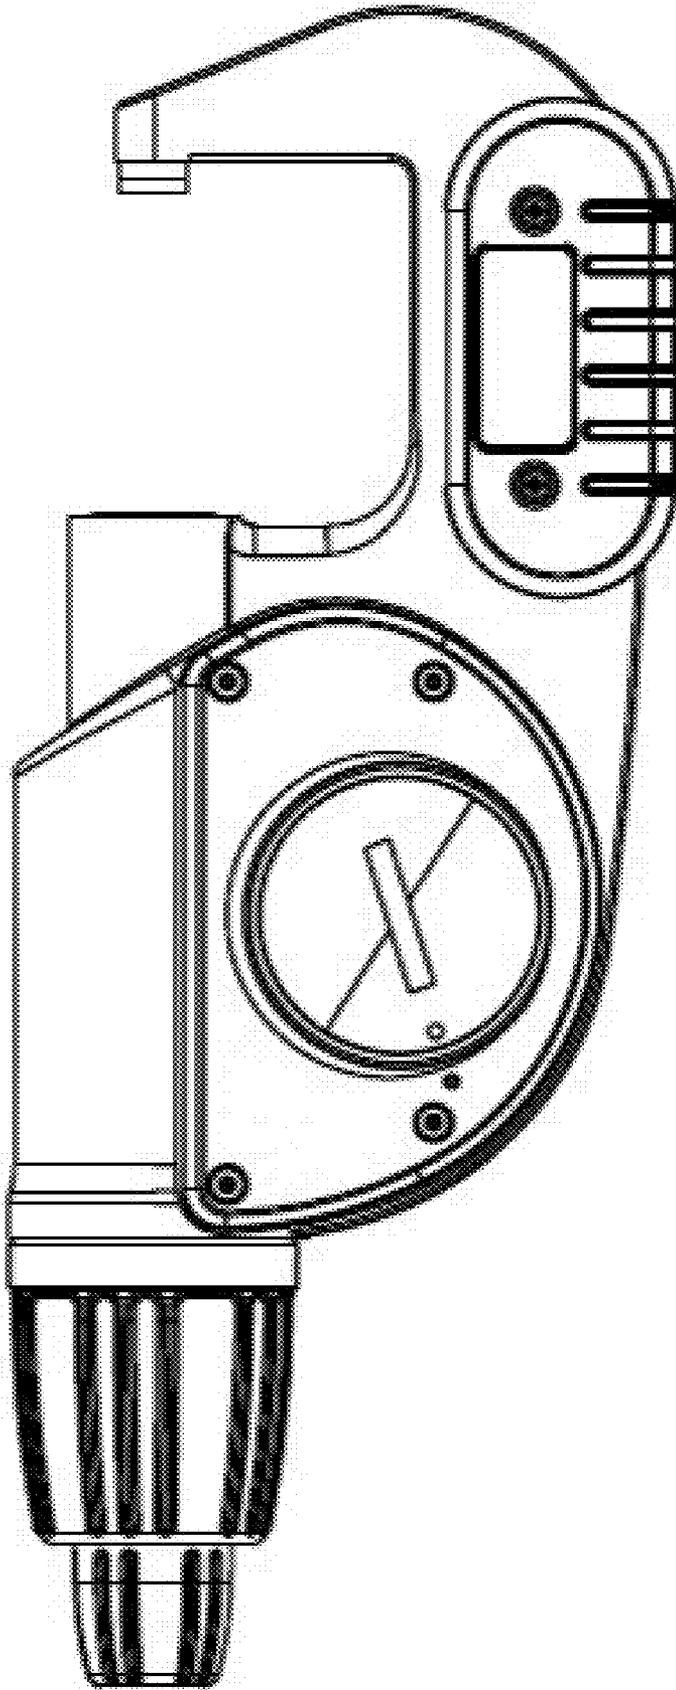


Figure 3

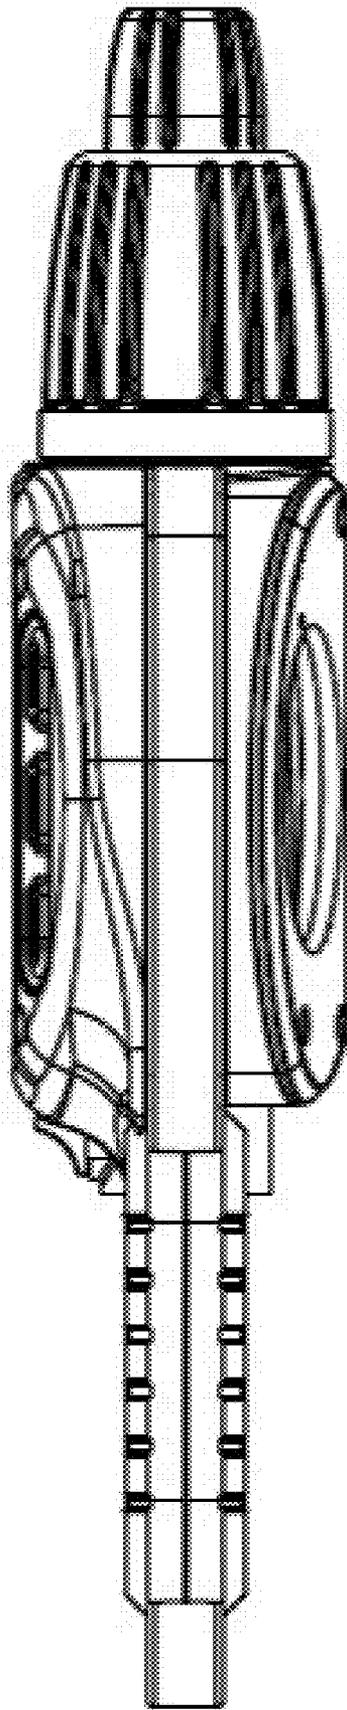


Figure 4

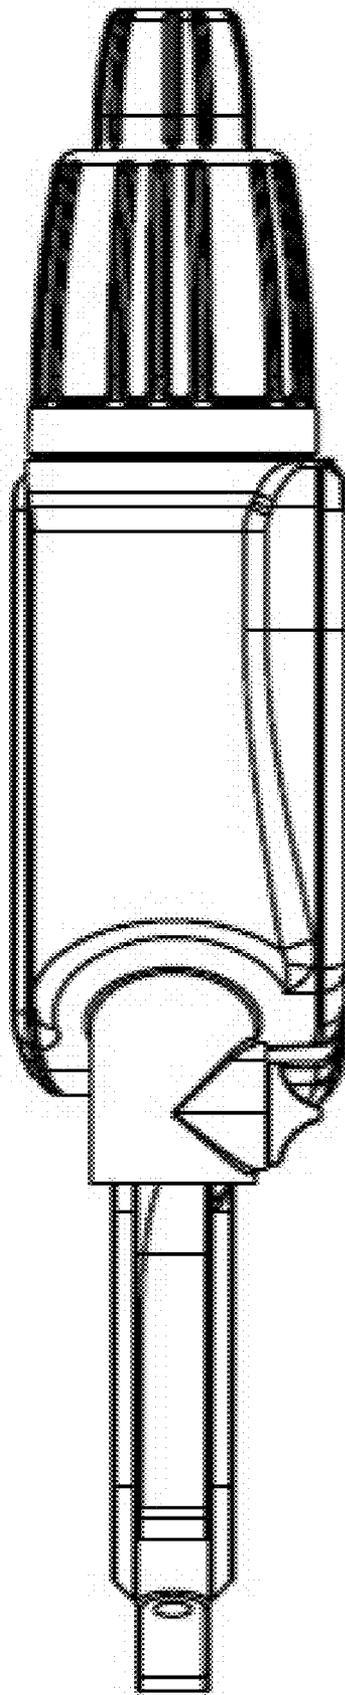


Figure 5

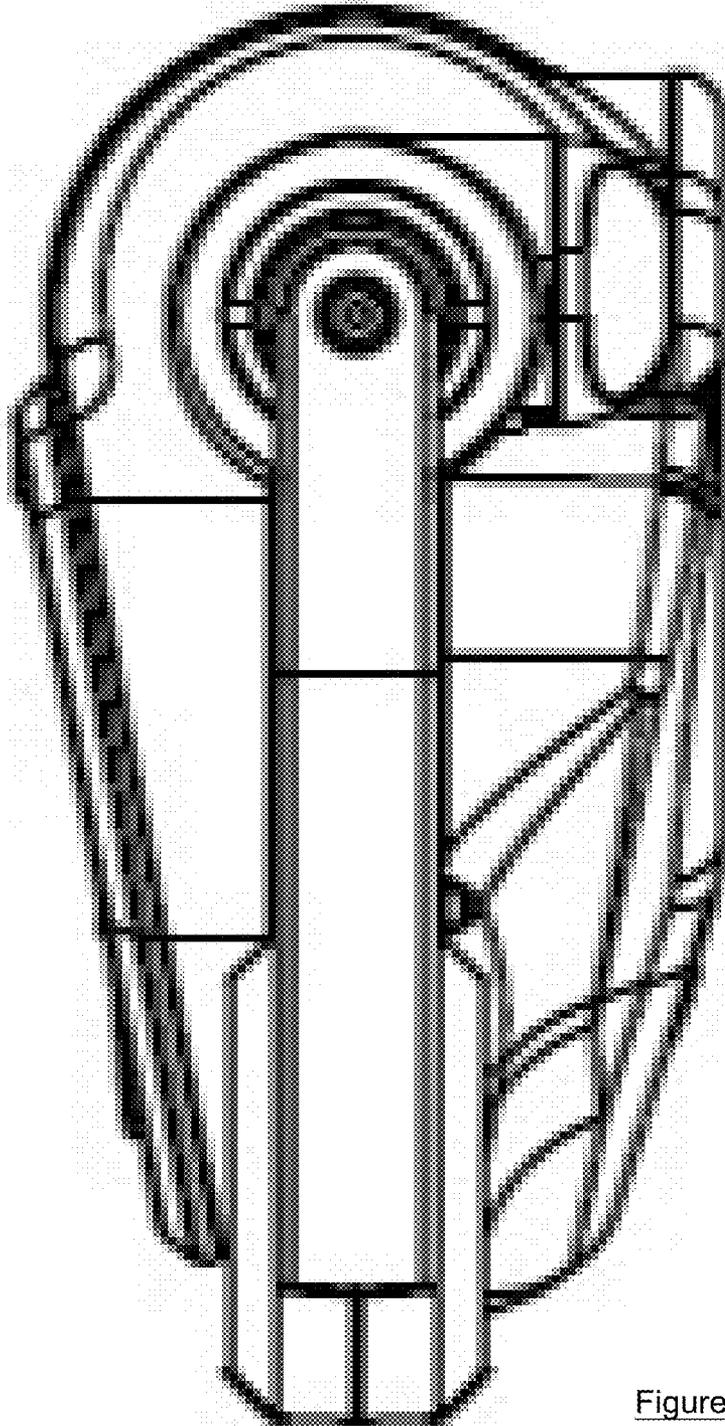


Figure 6



Figure 7

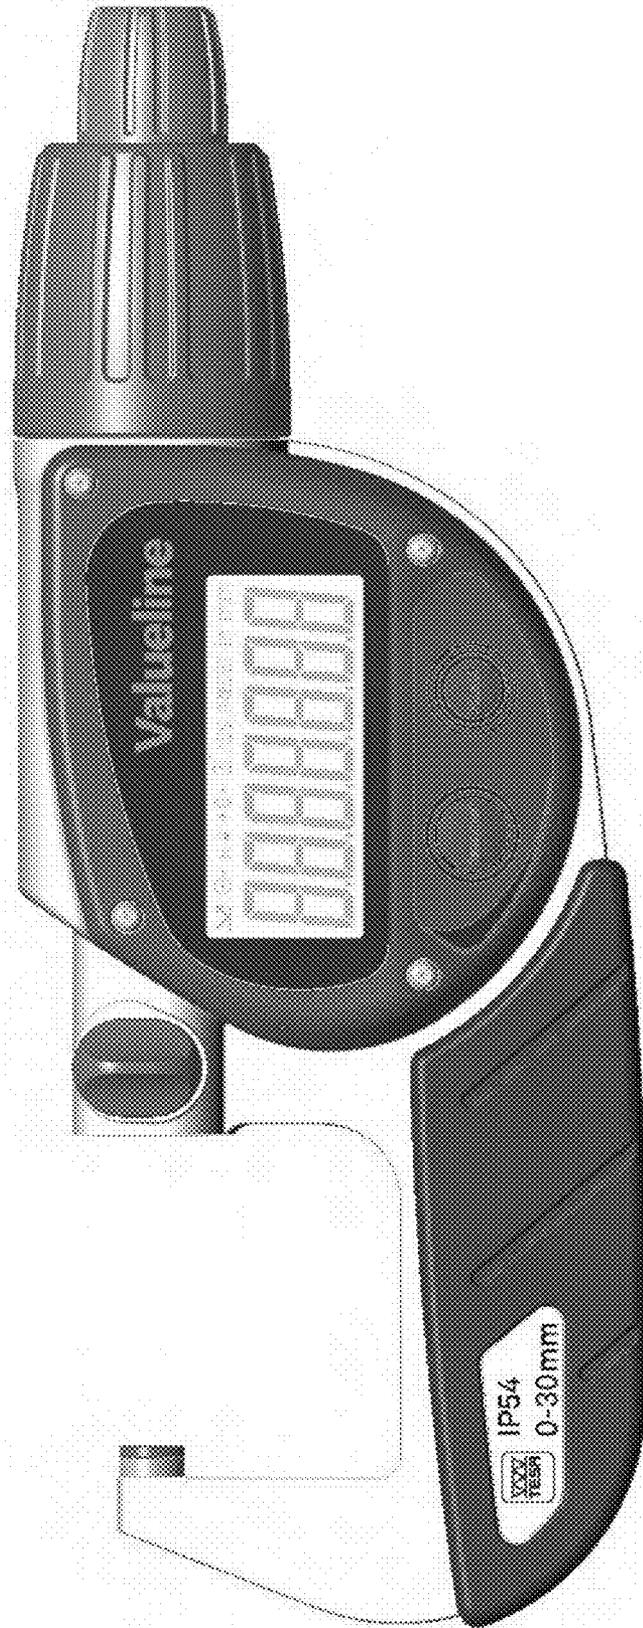


Figure 8