



US 20060036333A1

(19) **United States**(12) **Patent Application Publication**
Smith et al.(10) **Pub. No.: US 2006/0036333 A1**(43) **Pub. Date: Feb. 16, 2006**(54) **MASTOPEXY STABILIZATION APPARATUS
AND METHOD****Publication Classification**(51) **Int. Cl.****A61F 2/04** (2006.01)**A61F 2/12** (2006.01)(52) **U.S. Cl.** **623/23.67; 623/8**(76) Inventors: **Lane Fielding Smith**, Bountiful, UT
(US); **Evan Farr Smith**, West Jordan,
UT (US)


Correspondence Address:

PATE PIERCE & BAIRD**215 SOUTH STATE STREET, SUITE 550****PARKSIDE TOWER****SALT LAKE CITY, UT 84111 (US)**

(57)

ABSTRACT(21) Appl. No.: **11/245,726**(22) Filed: **Oct. 6, 2005****Related U.S. Application Data**(63) Continuation of application No. 10/771,776, filed on
Feb. 4, 2004.(60) Provisional application No. 60/477,100, filed on Jun.
9, 2003.

An apparatus and method for mastopexy surgeries correcting a ptosis condition caused by tissue stretching, in the breast as a result of pregnancy, time, aging, and the effects of gravity and athletic activity provide an implant having homogeneously formed connectors extending from inside an implant wall for anchoring to the chest wall or chest muscles of a patient. Embedded reinforcements and anchoring tabs or sutures may be readily oriented along a rib or other defining physiological location in order to provide immediate, permanent, and symmetric installation of implants in a mastopexy reconstruction.

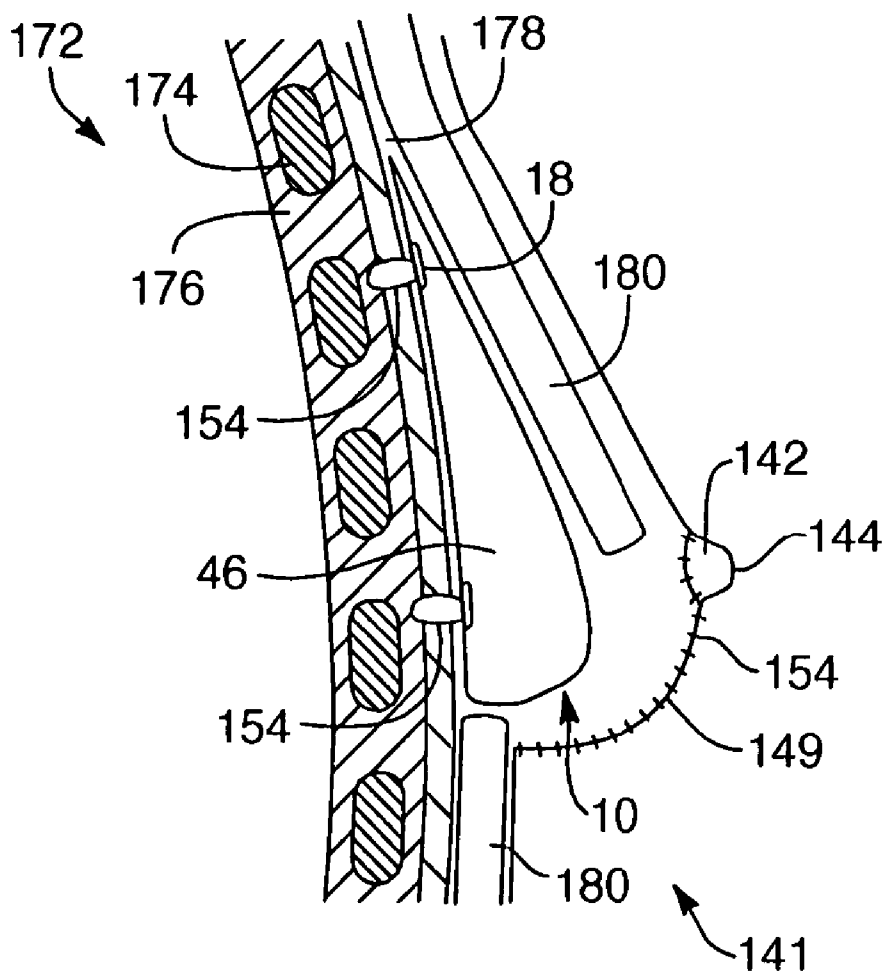

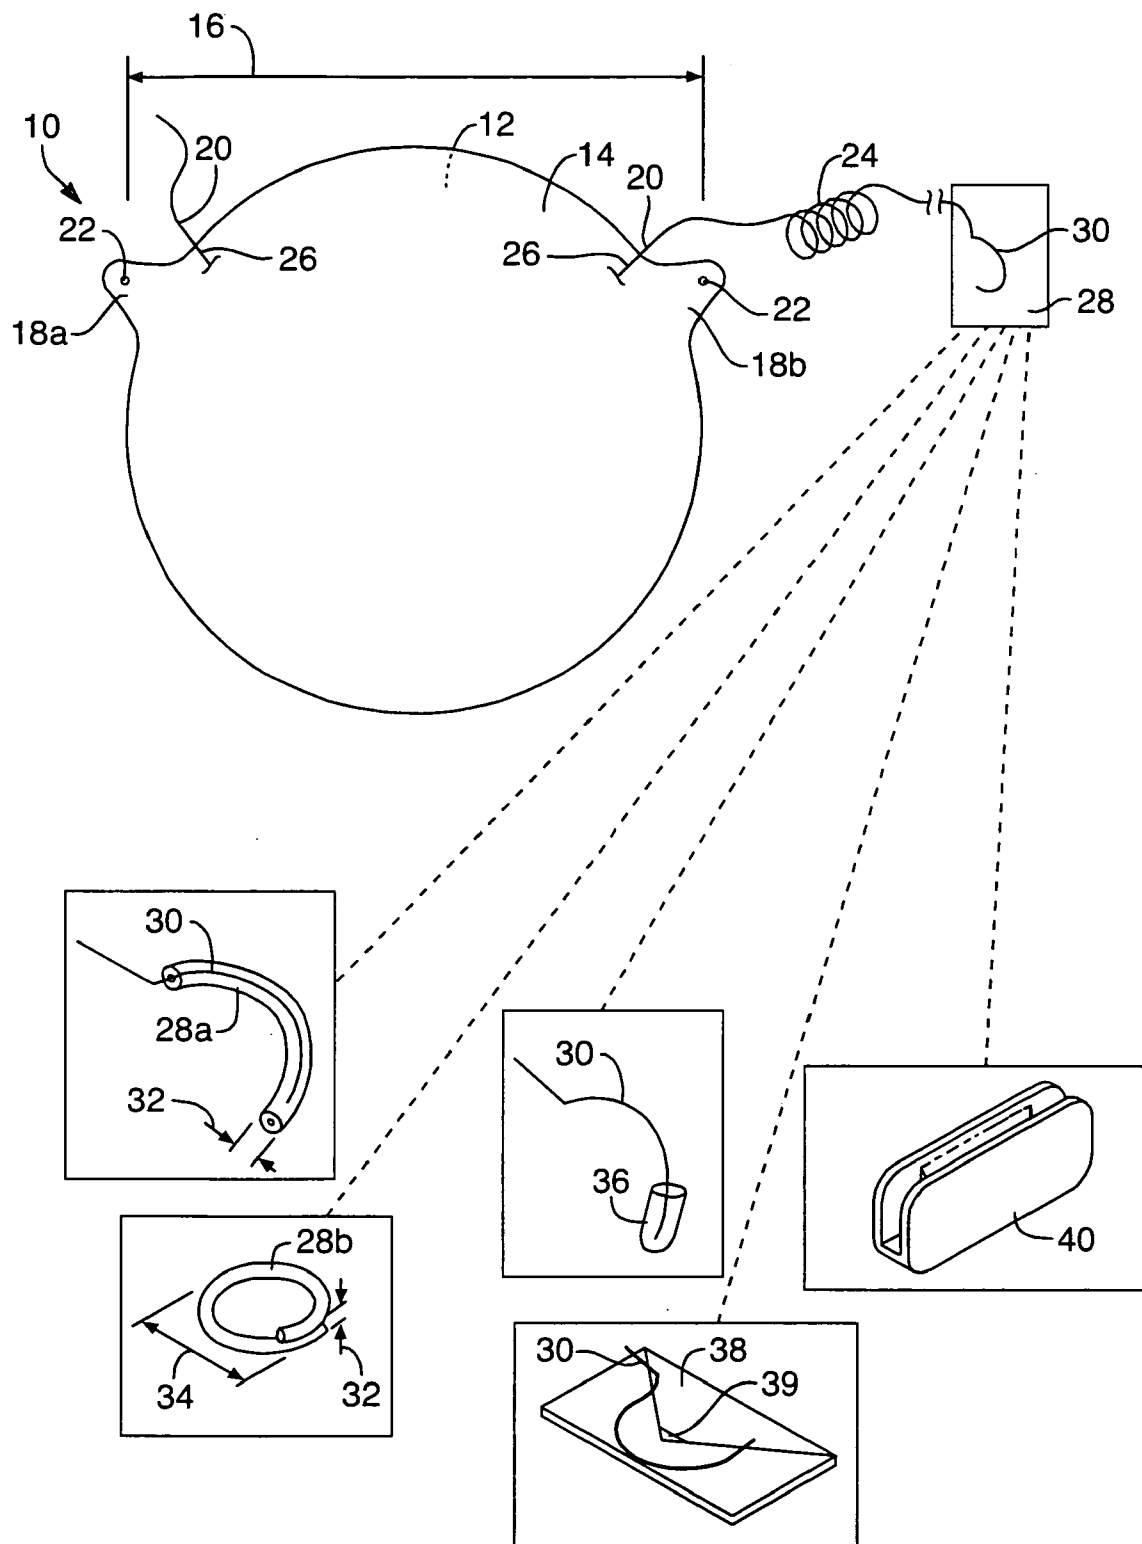


FIG. 1

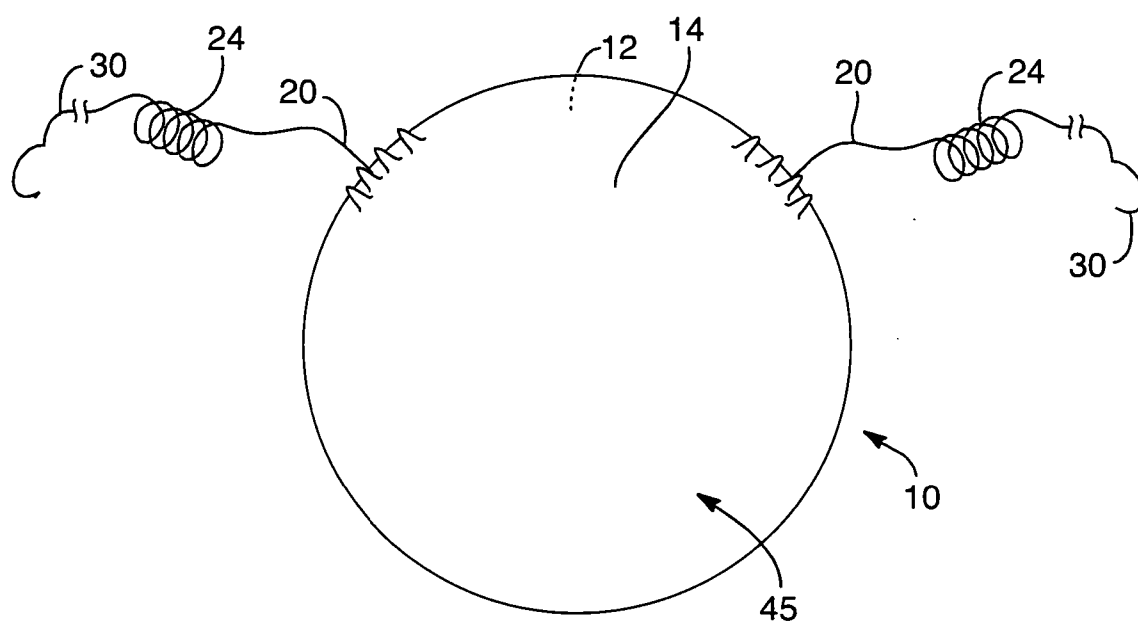


FIG. 2

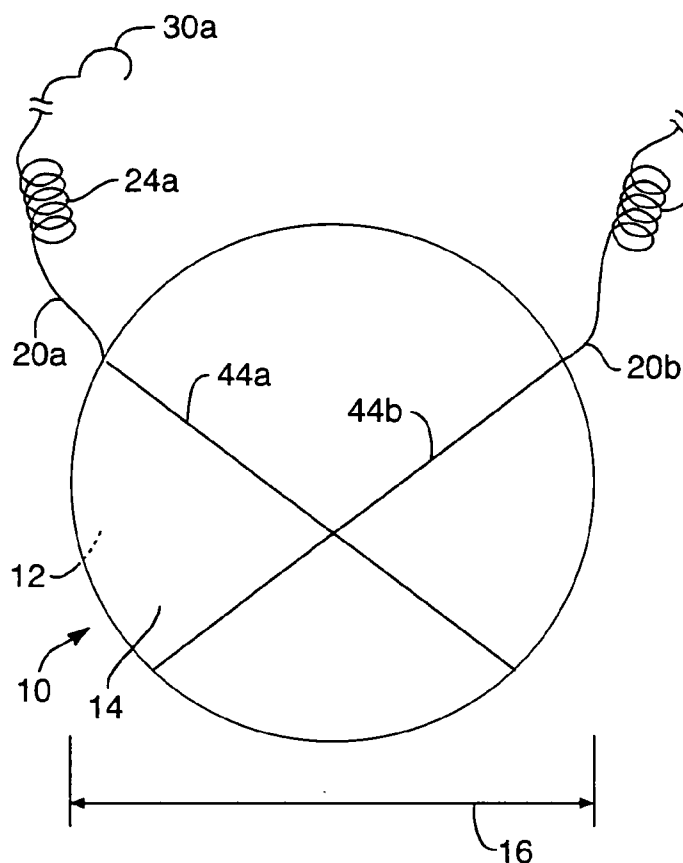


FIG. 3A

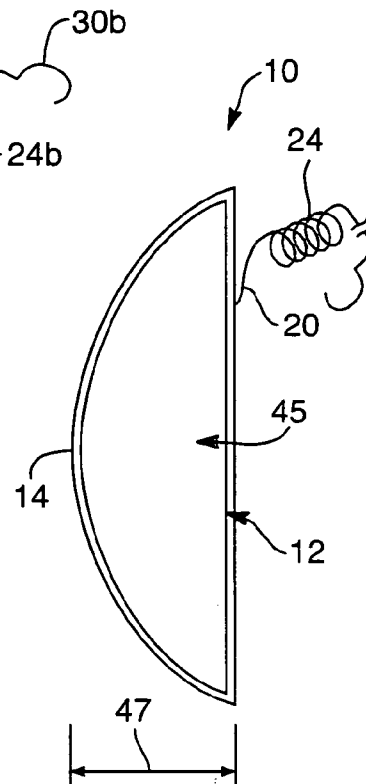


FIG. 4A

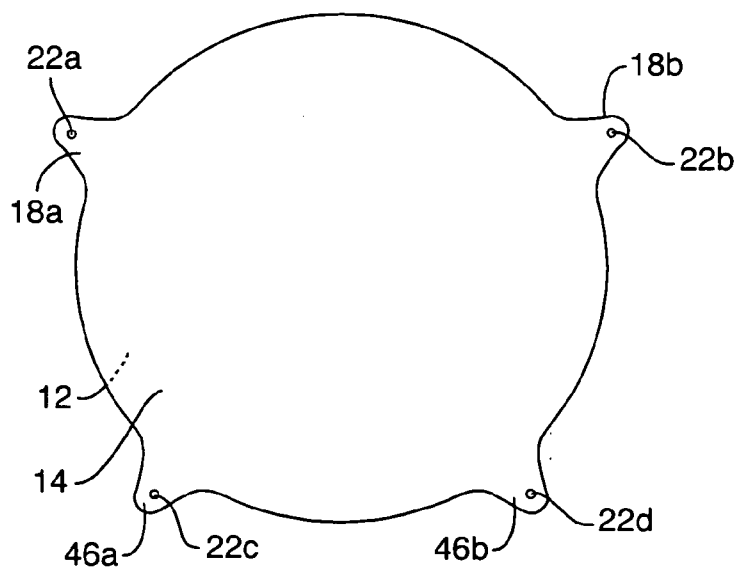


FIG. 3B

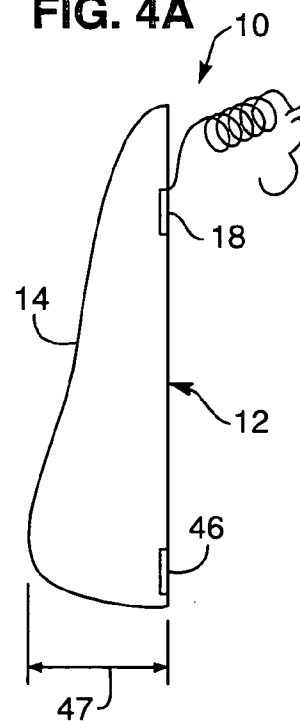


FIG. 4B

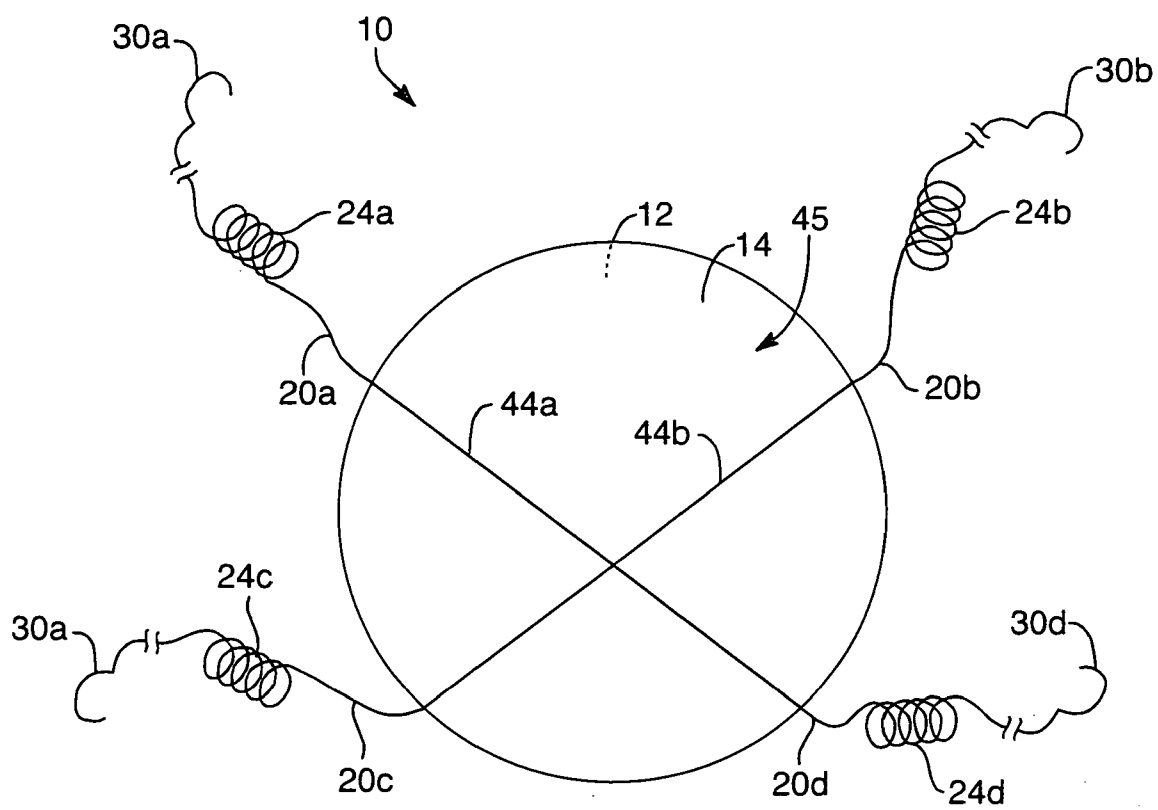
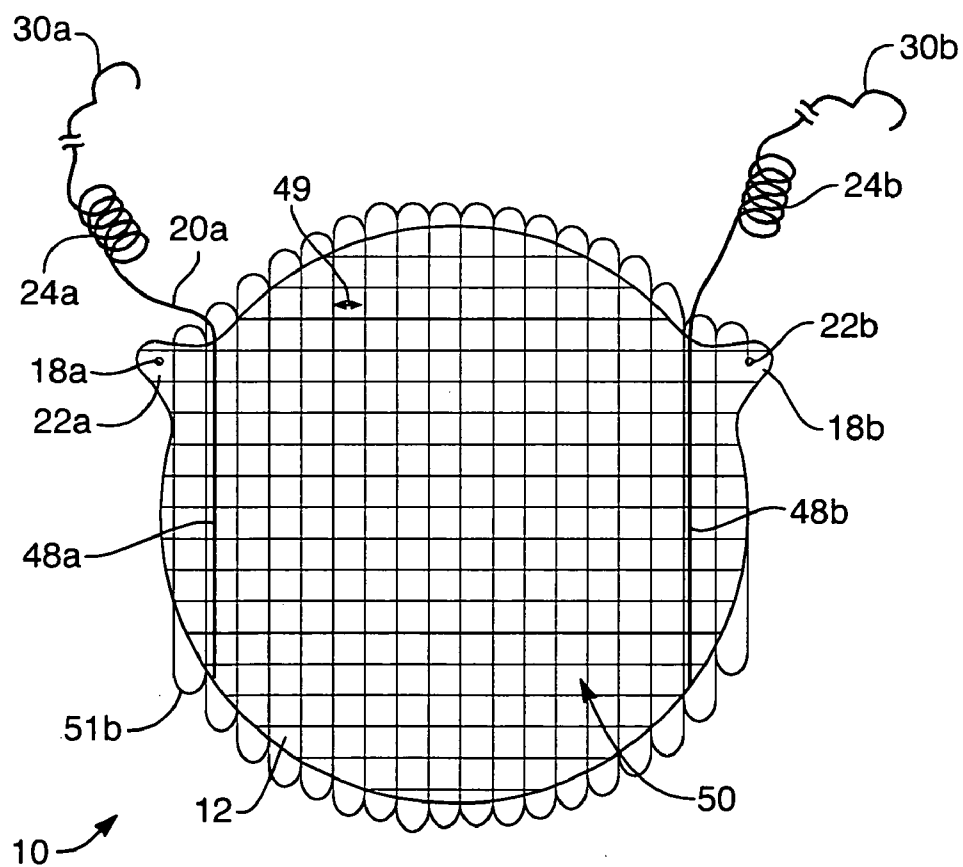
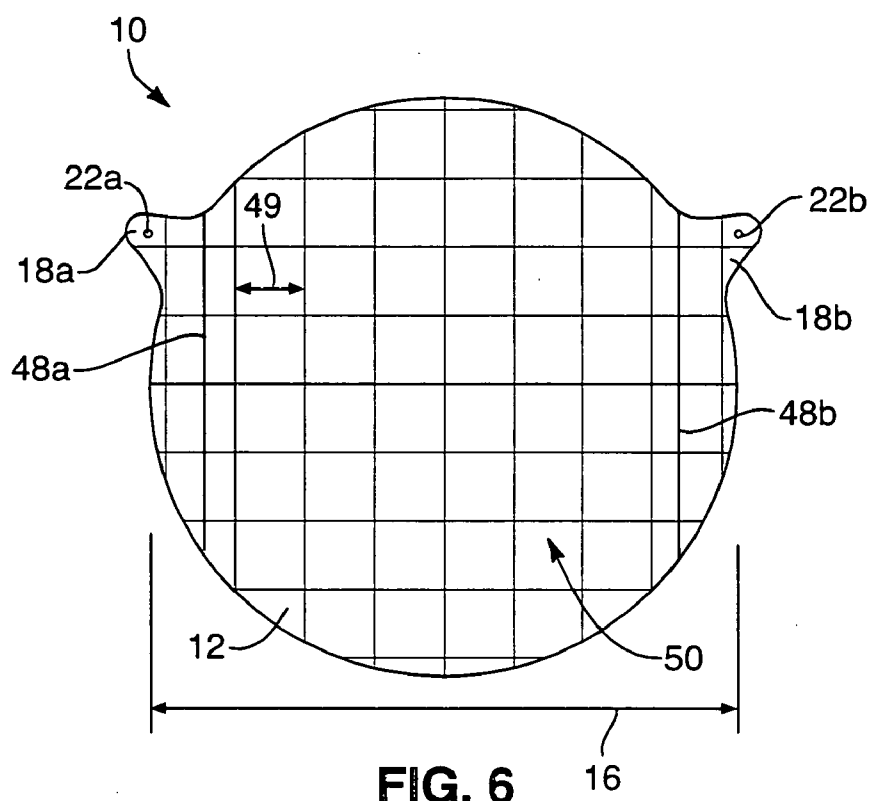
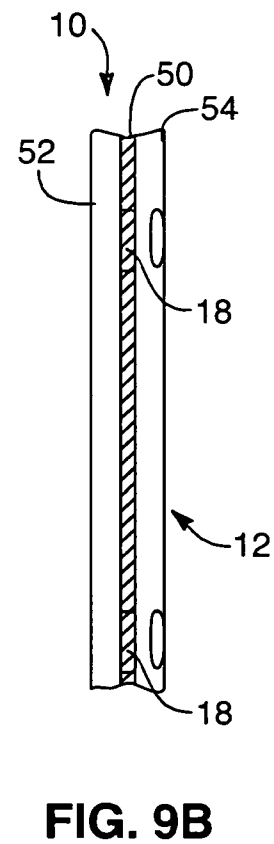
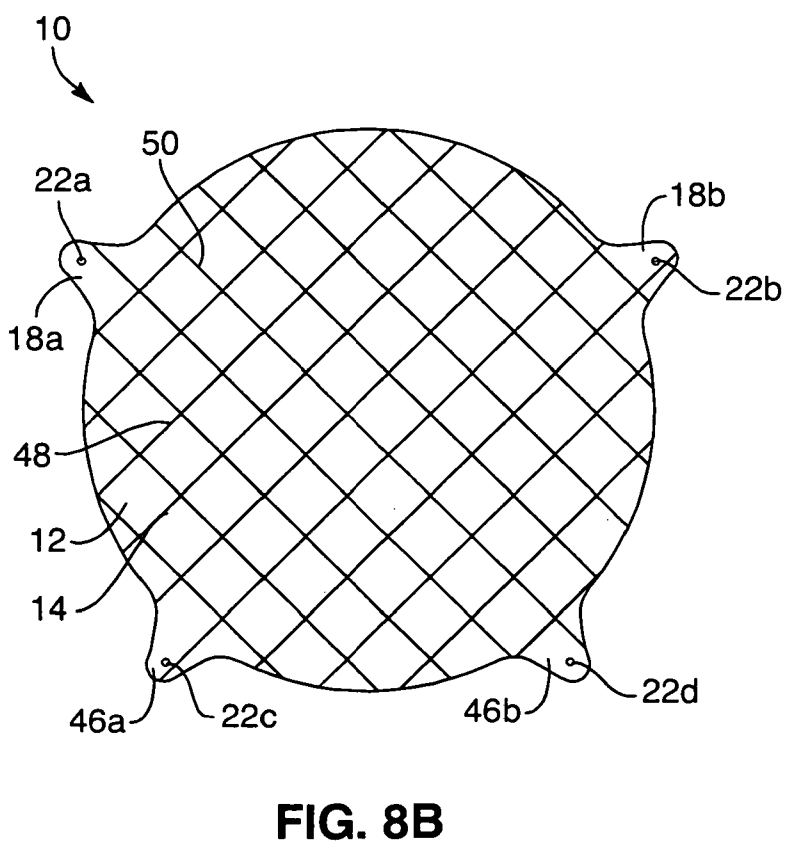
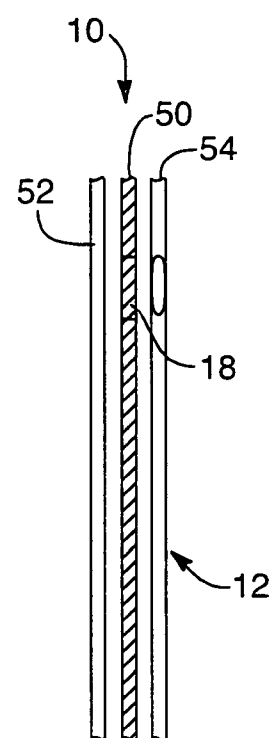
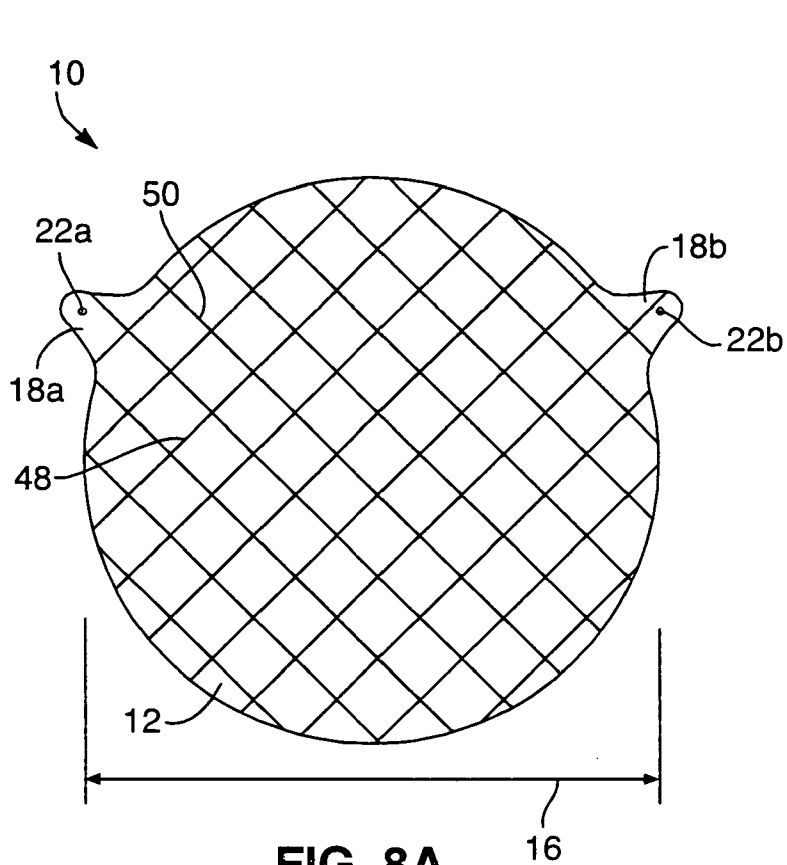


FIG. 5





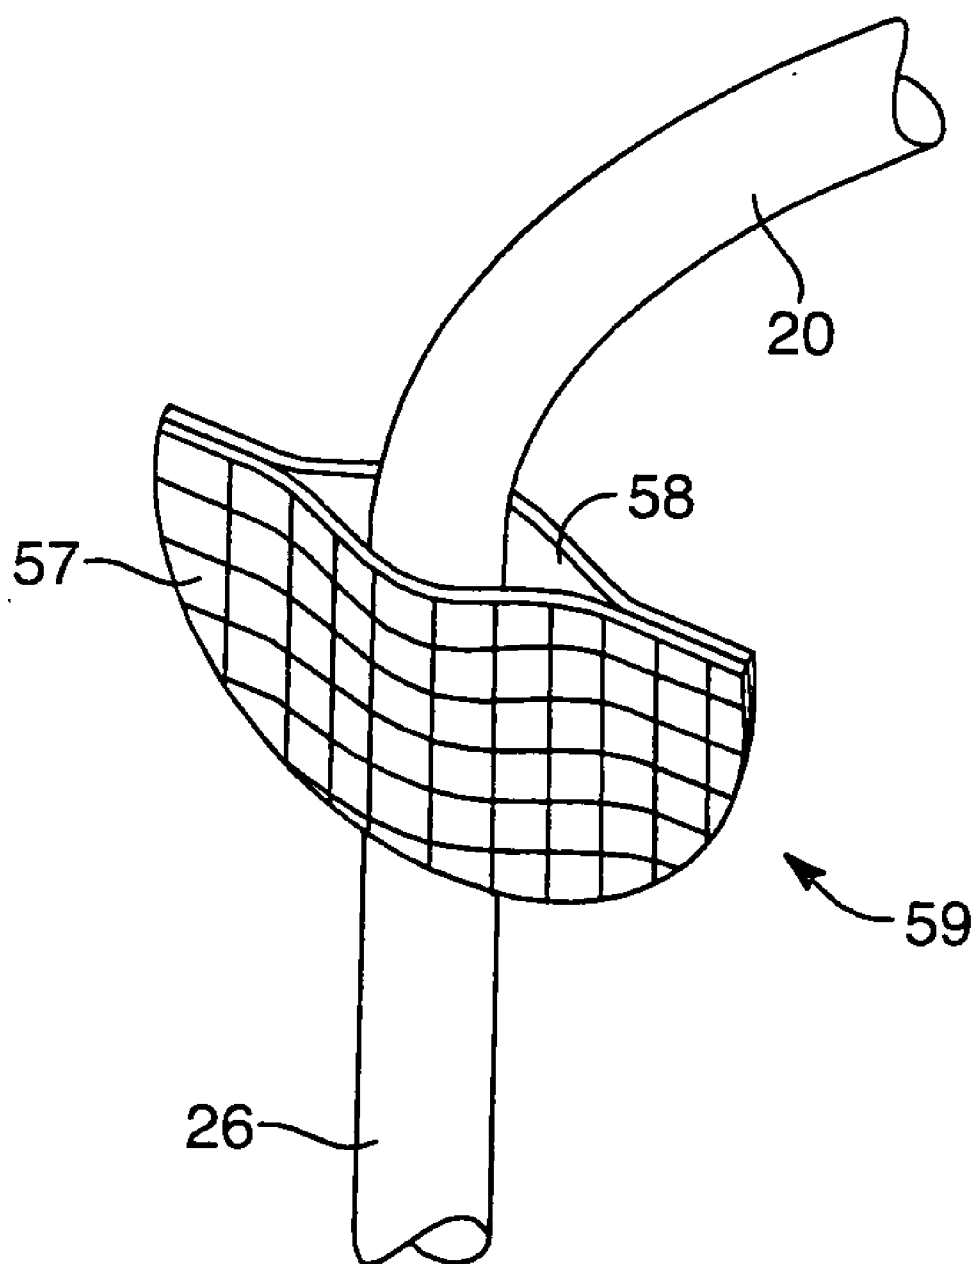


FIG. 10

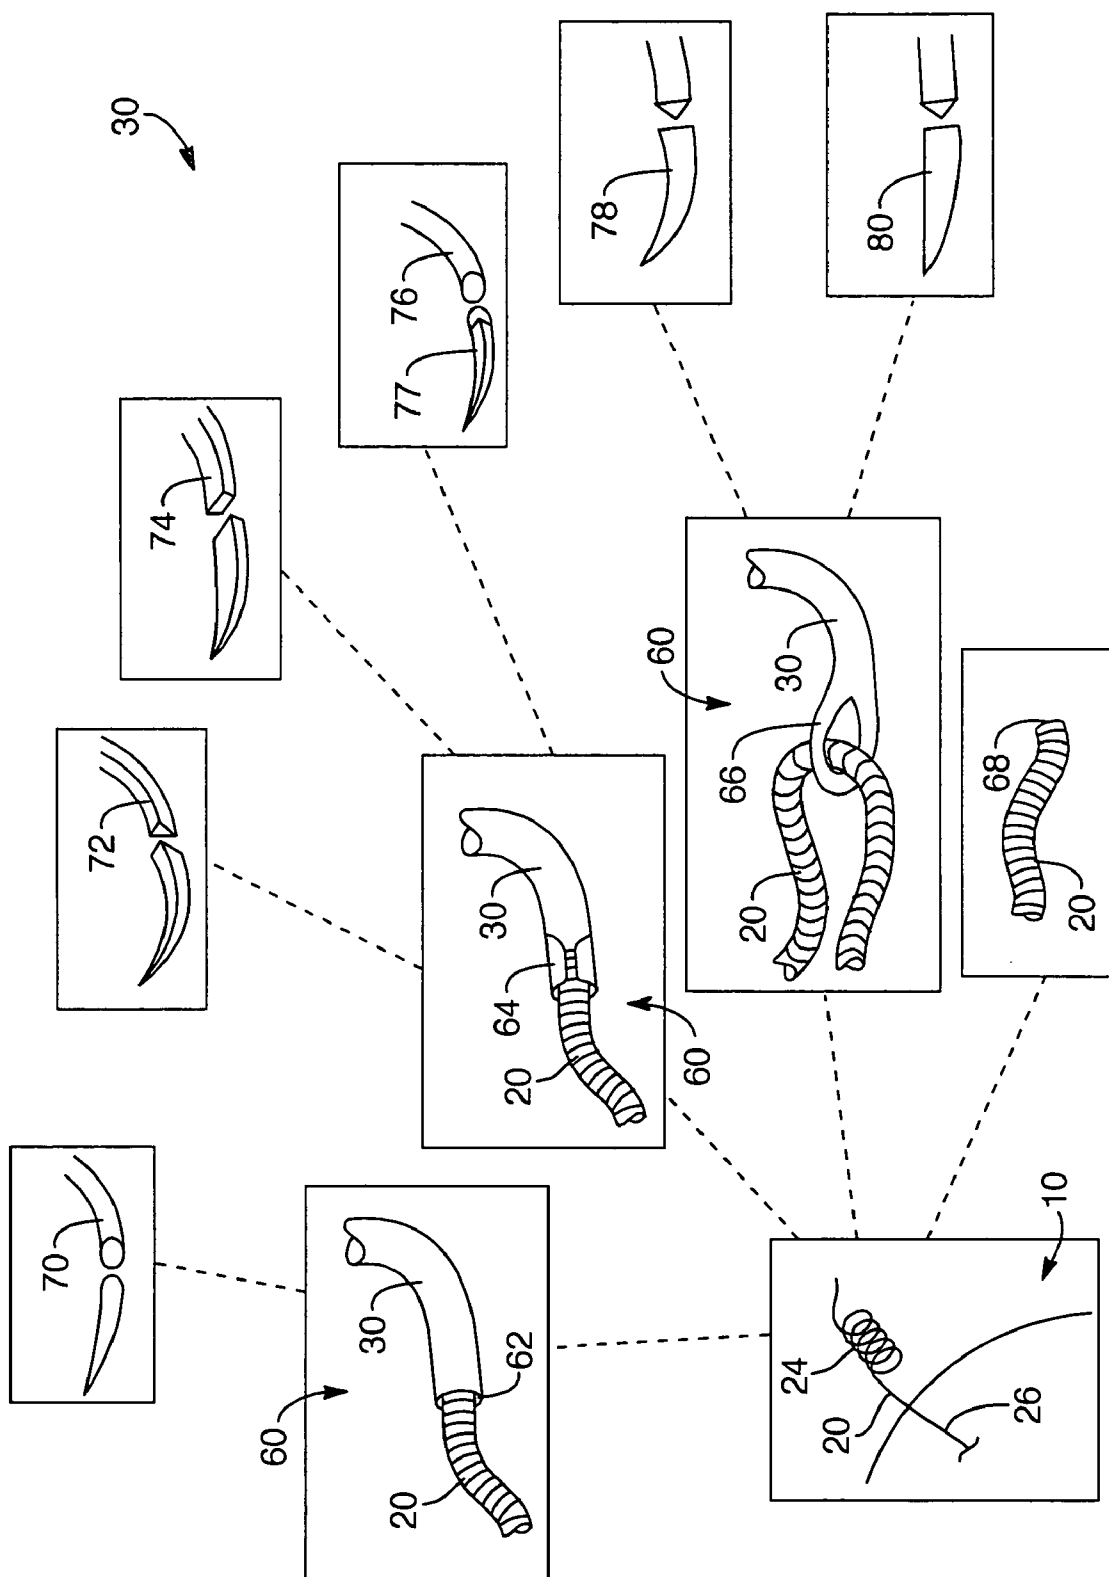


FIG. 11

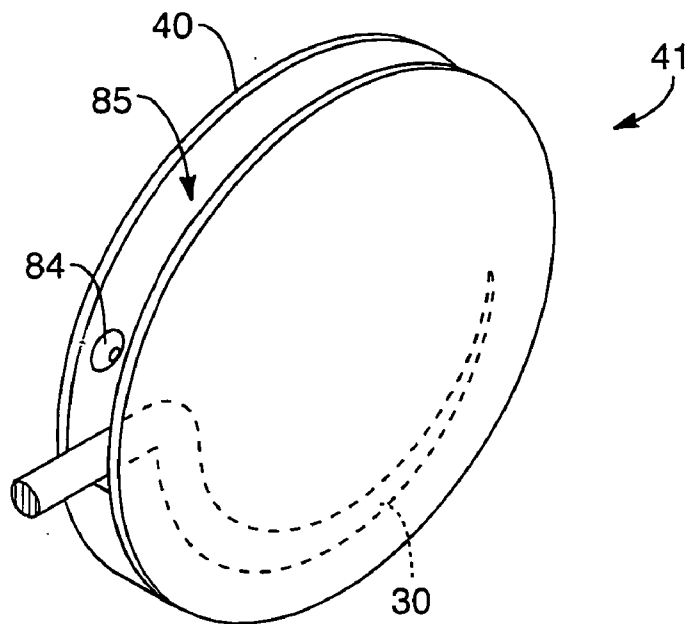


FIG. 12

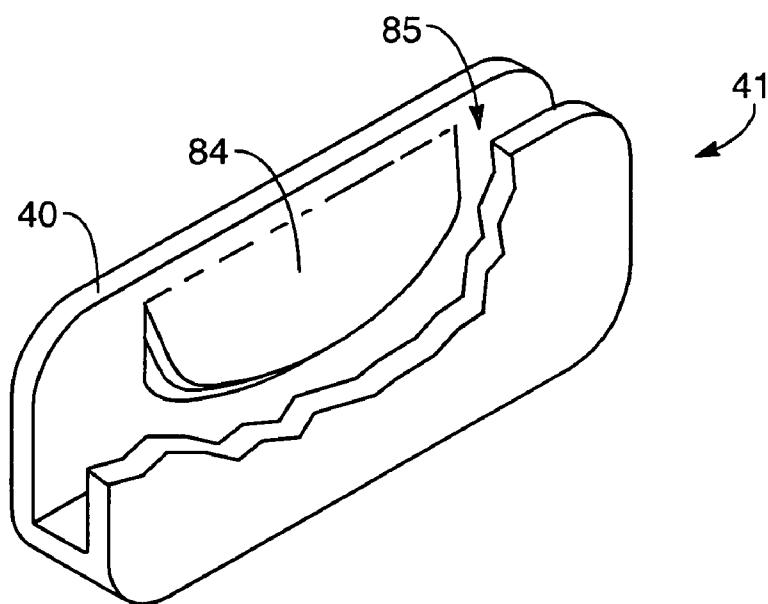


FIG. 13

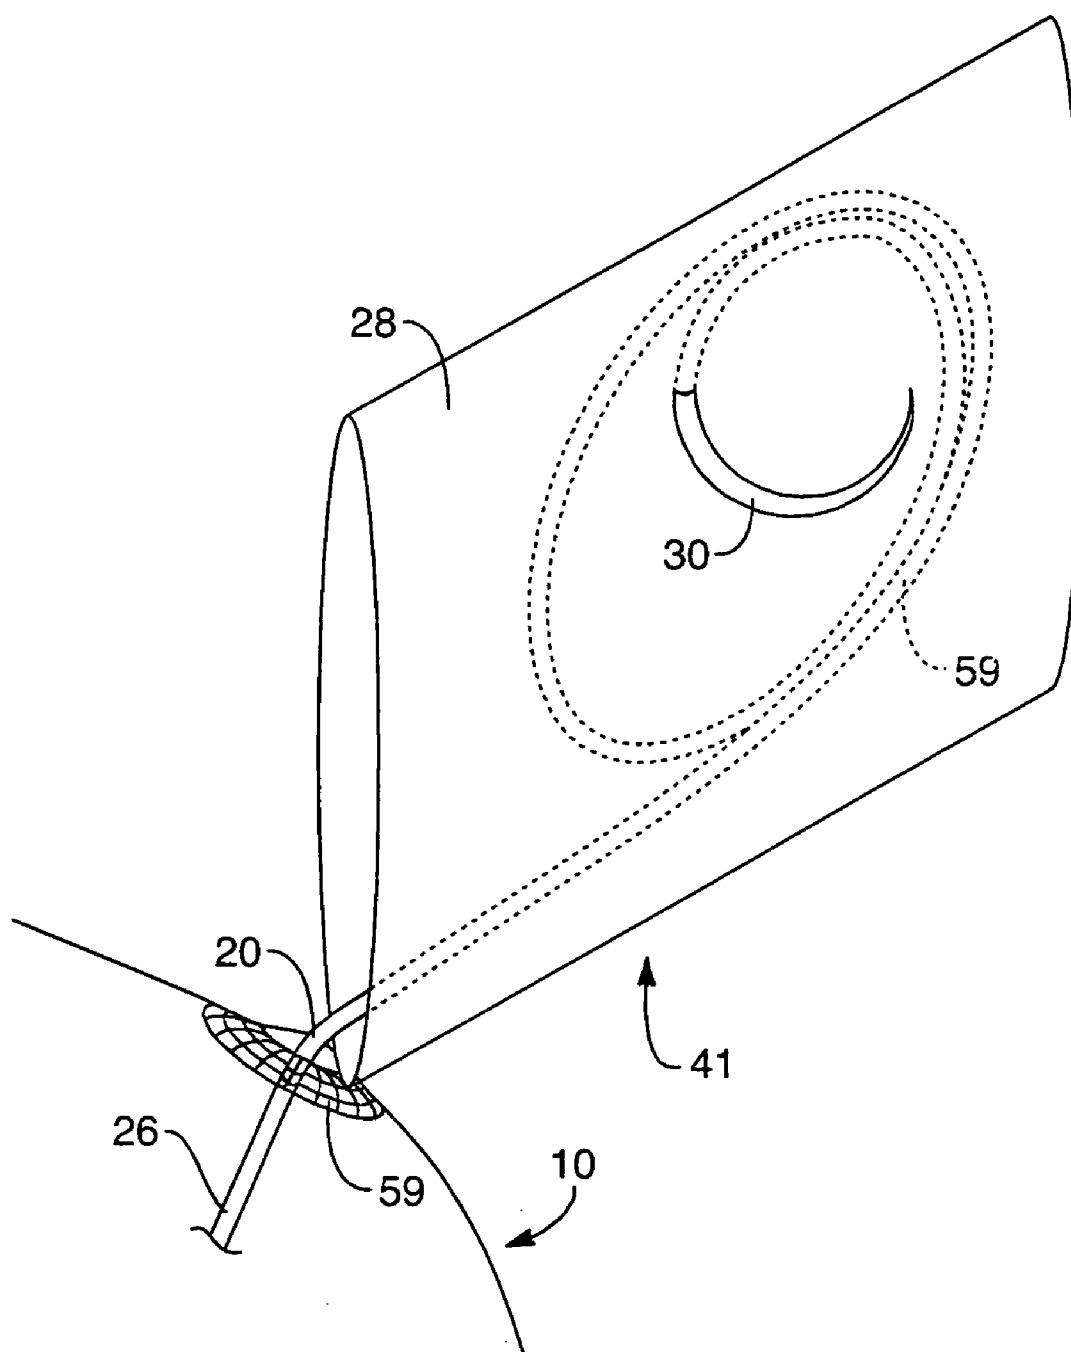


FIG. 14A

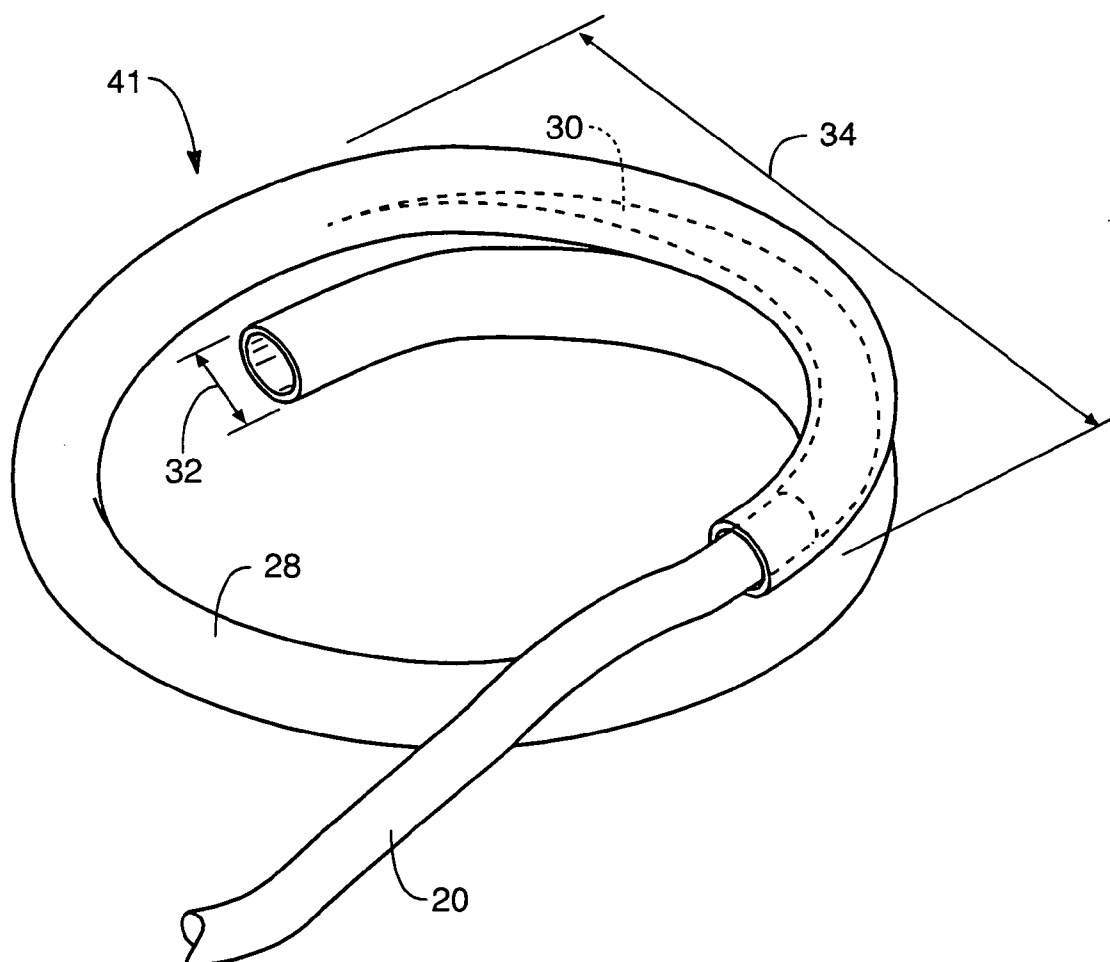


FIG. 14B

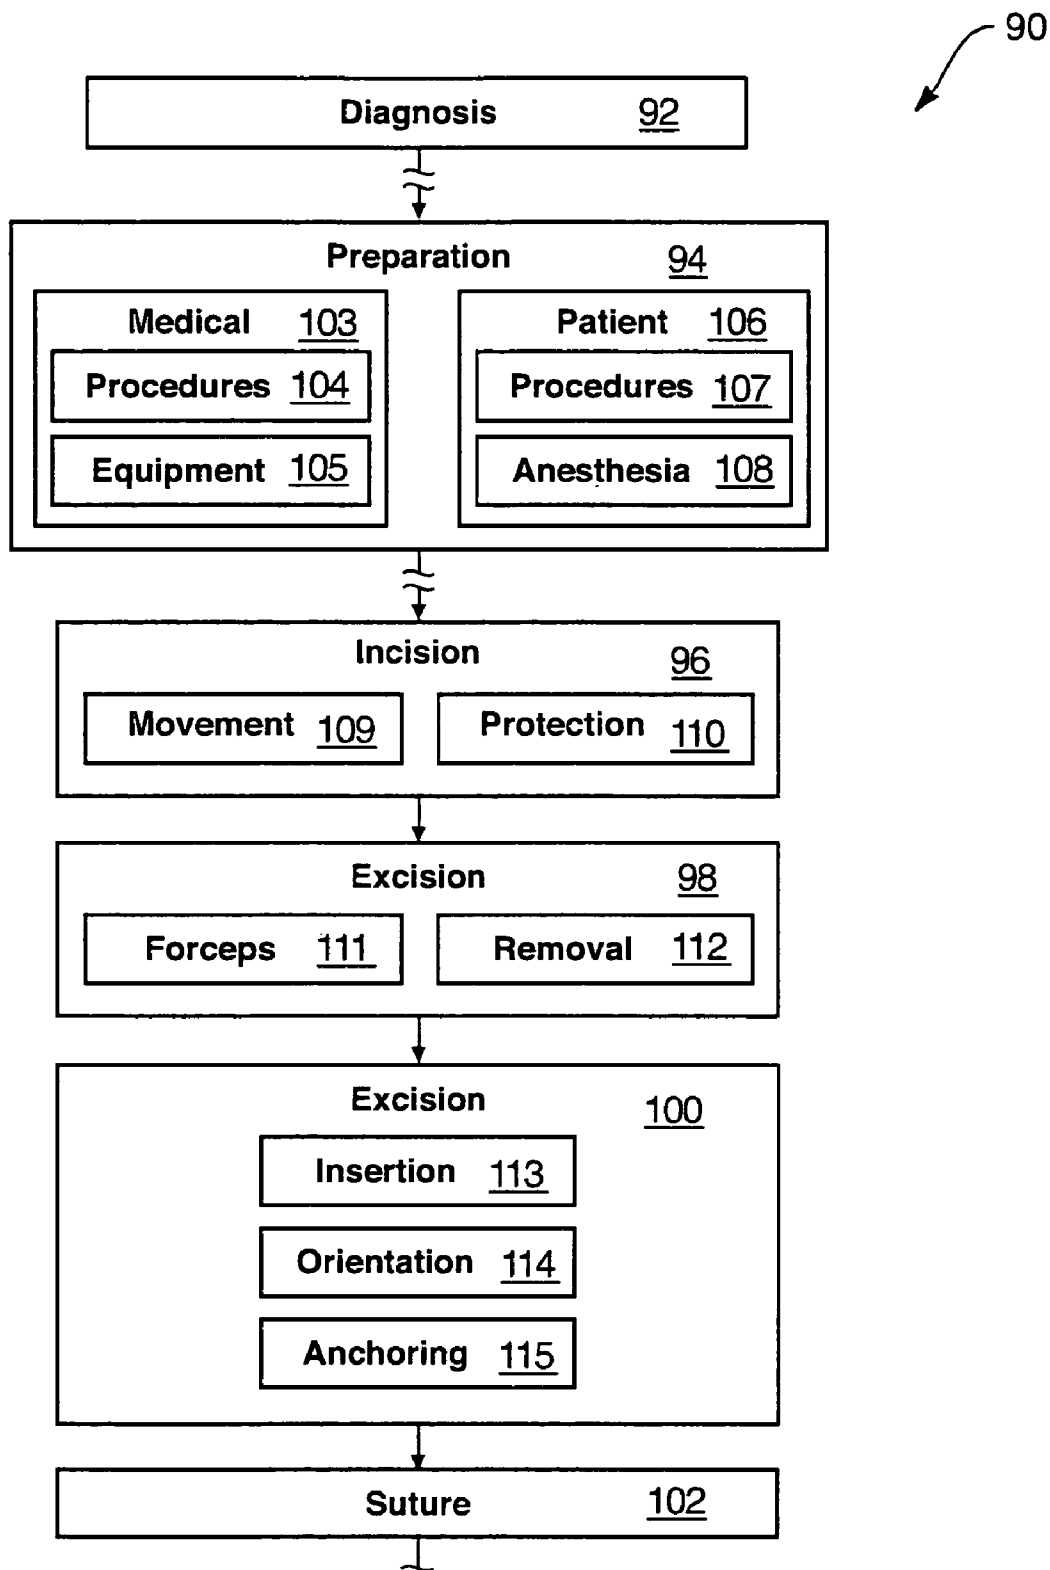


FIG. 15

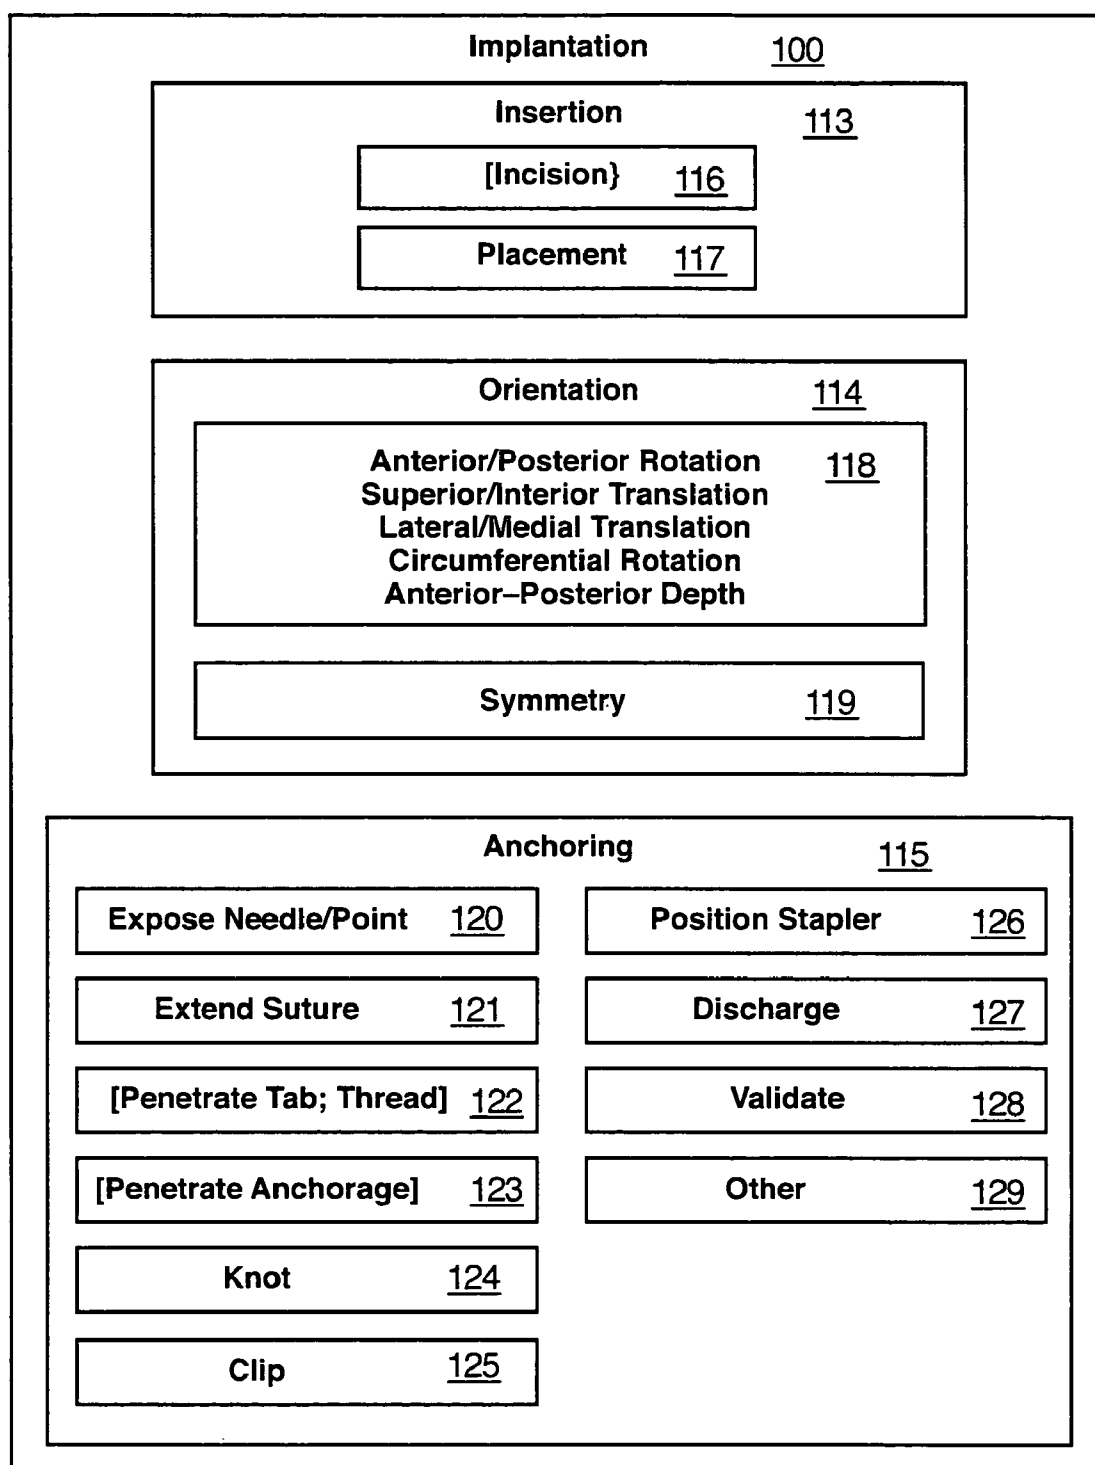


FIG. 16

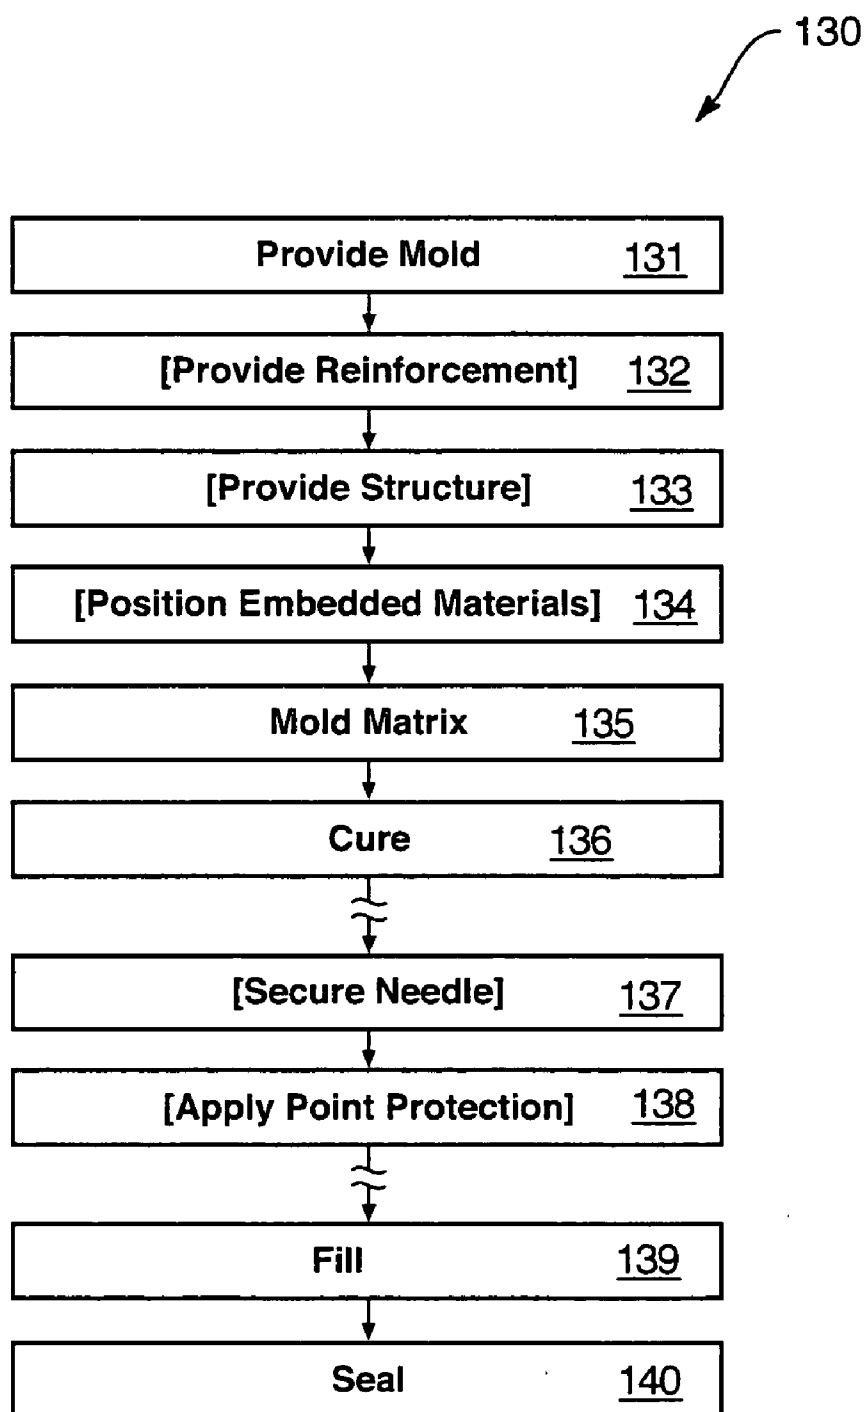


FIG. 17

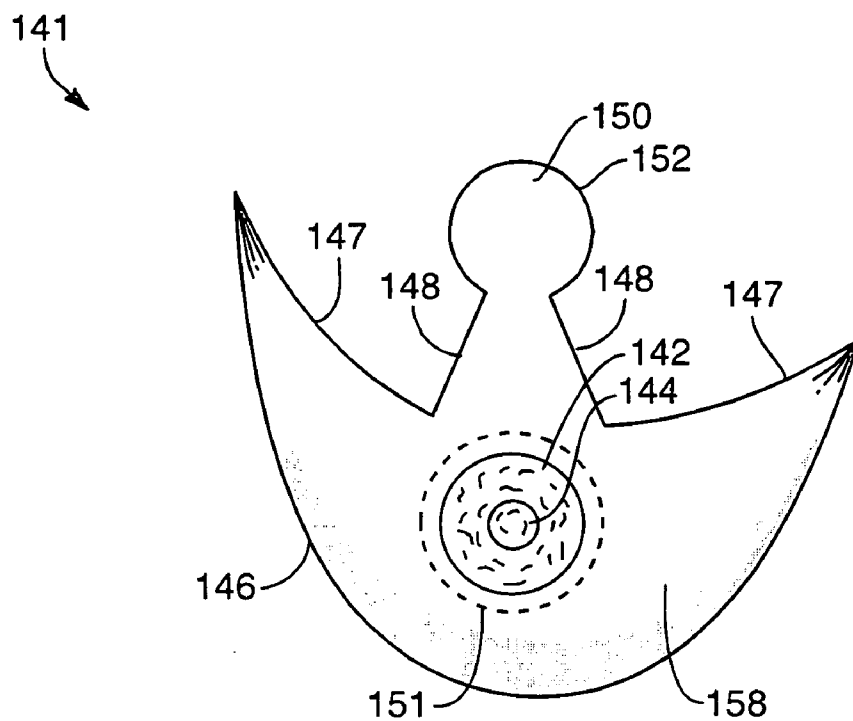


FIG. 18

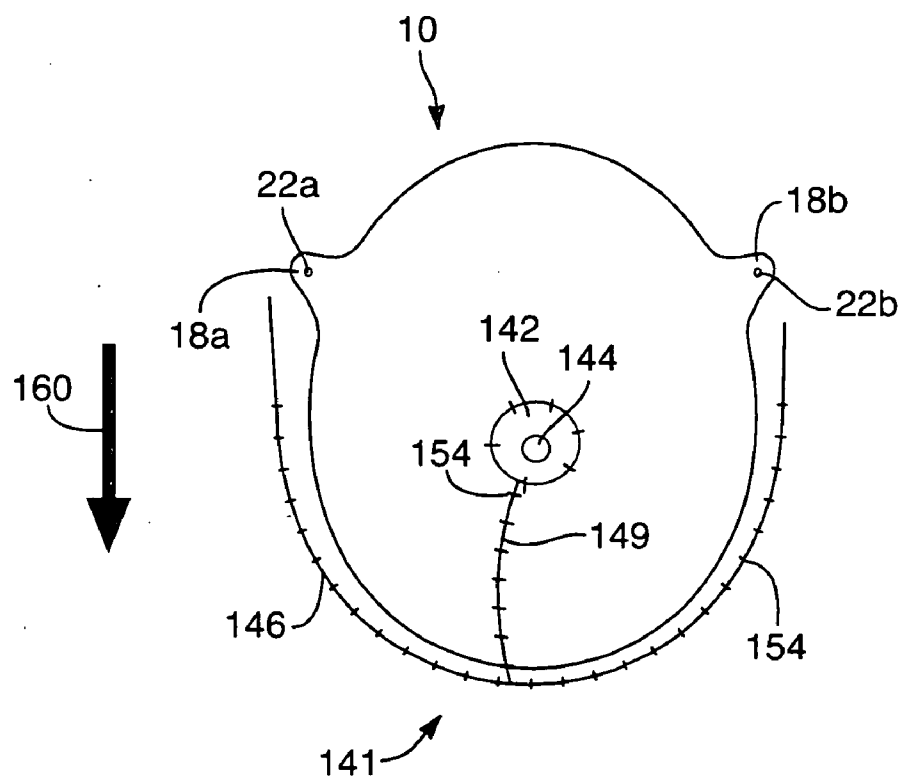


FIG. 19

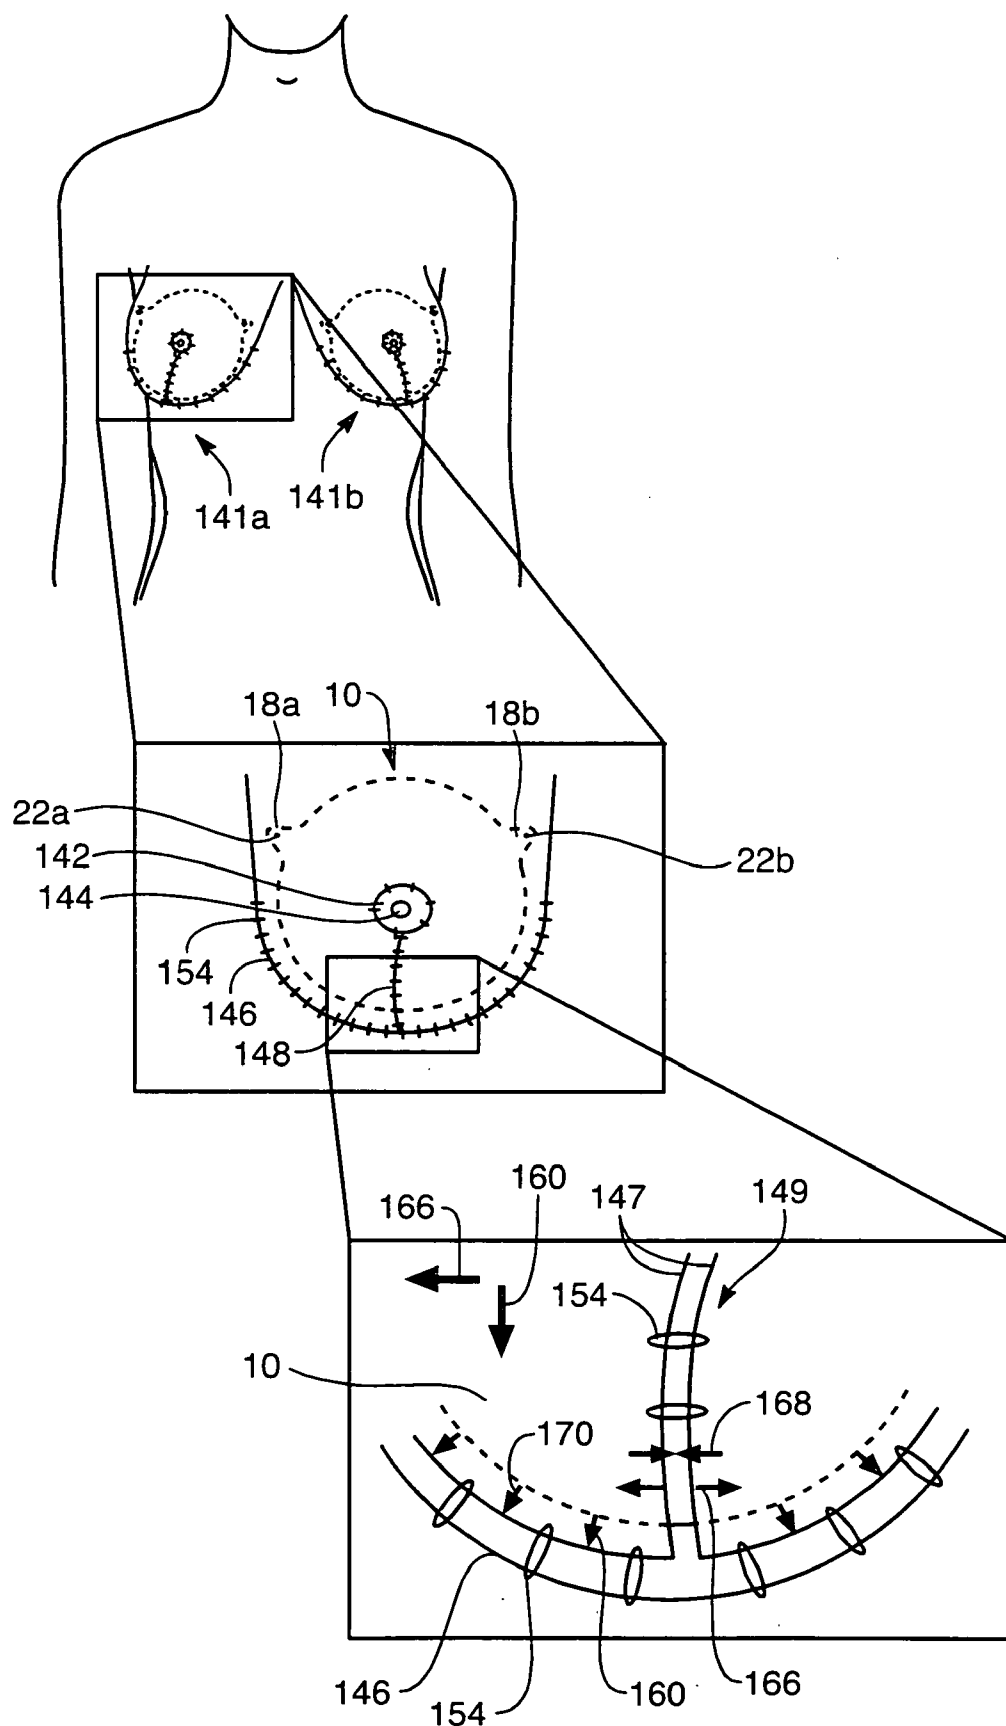


FIG. 20

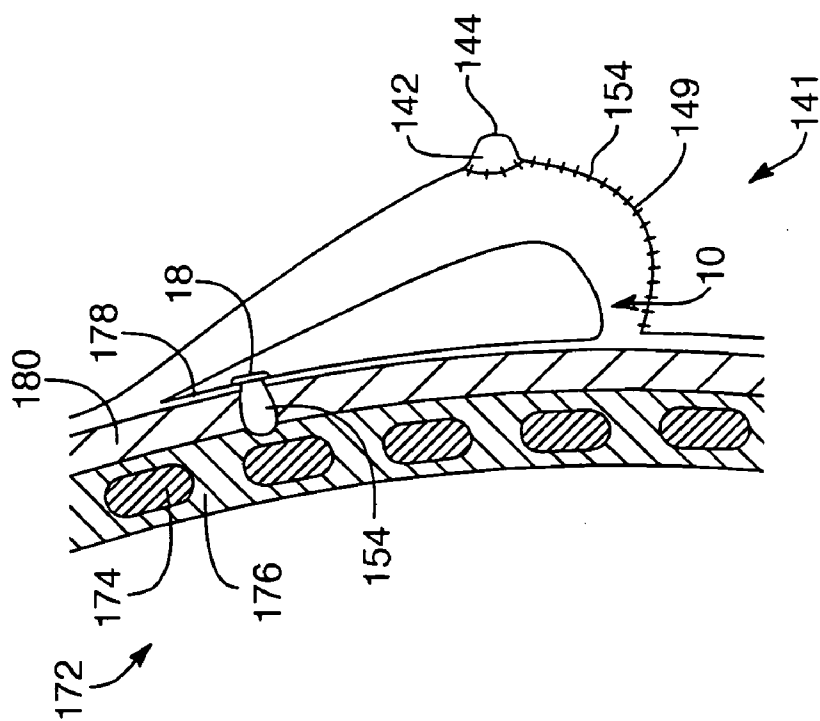


FIG. 21A

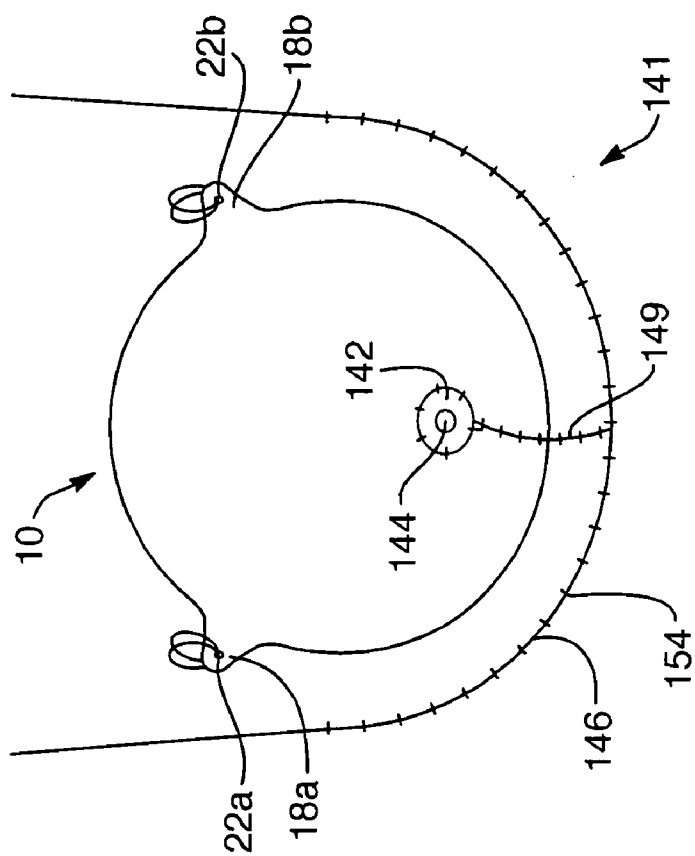


FIG. 21B

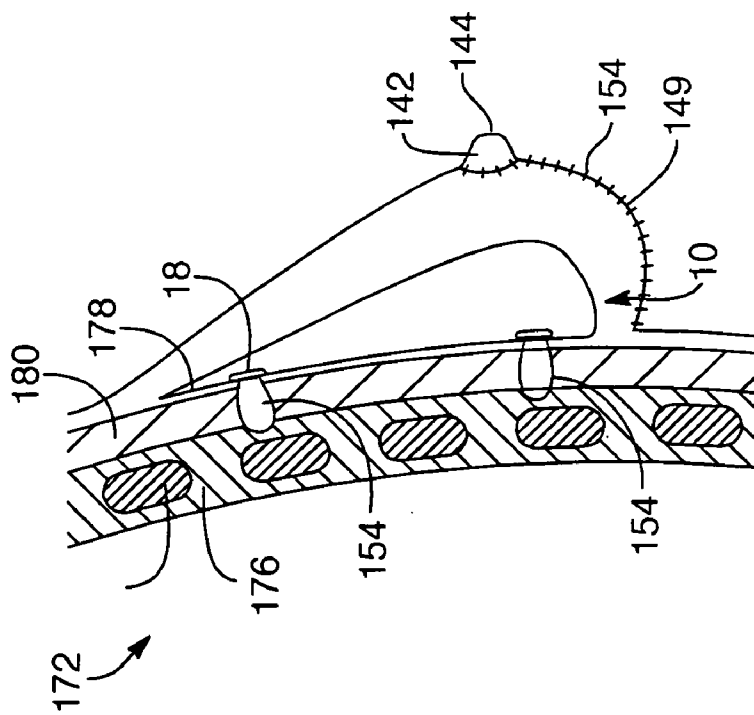


FIG. 21C

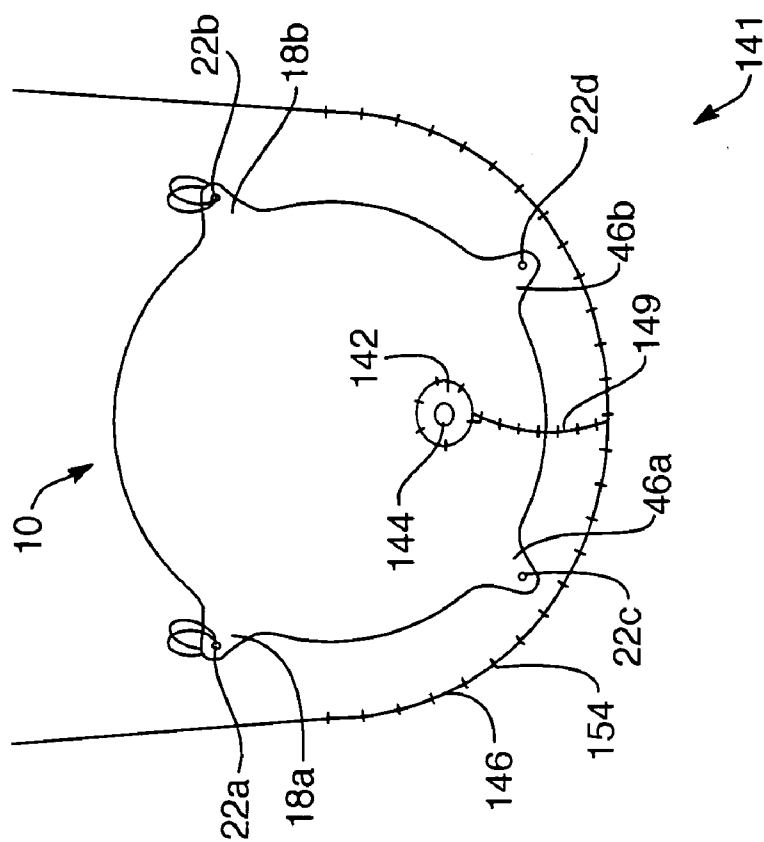


FIG. 21D

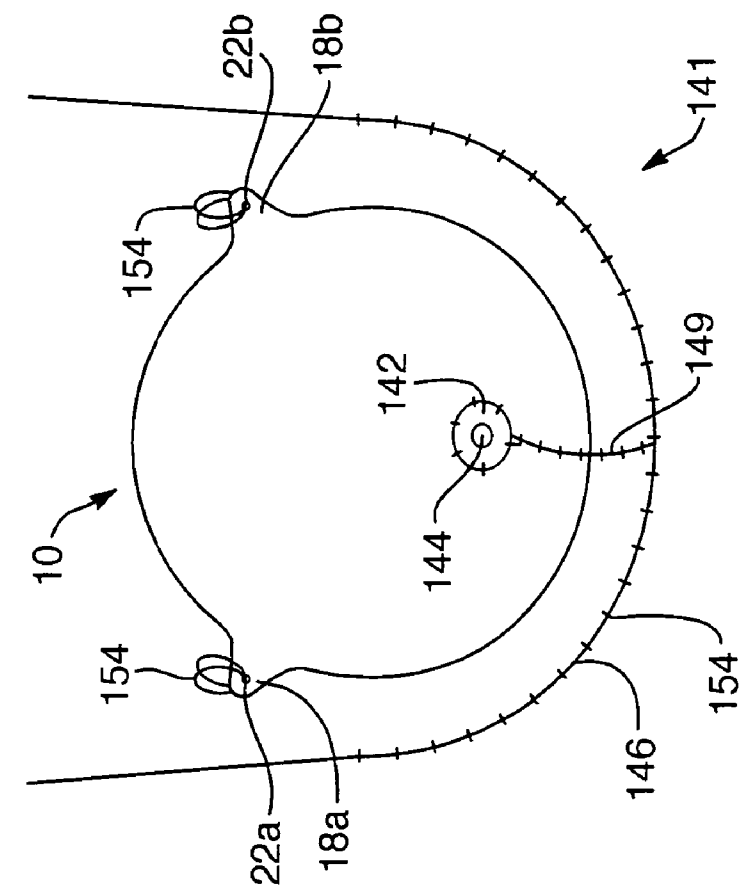


FIG. 22B

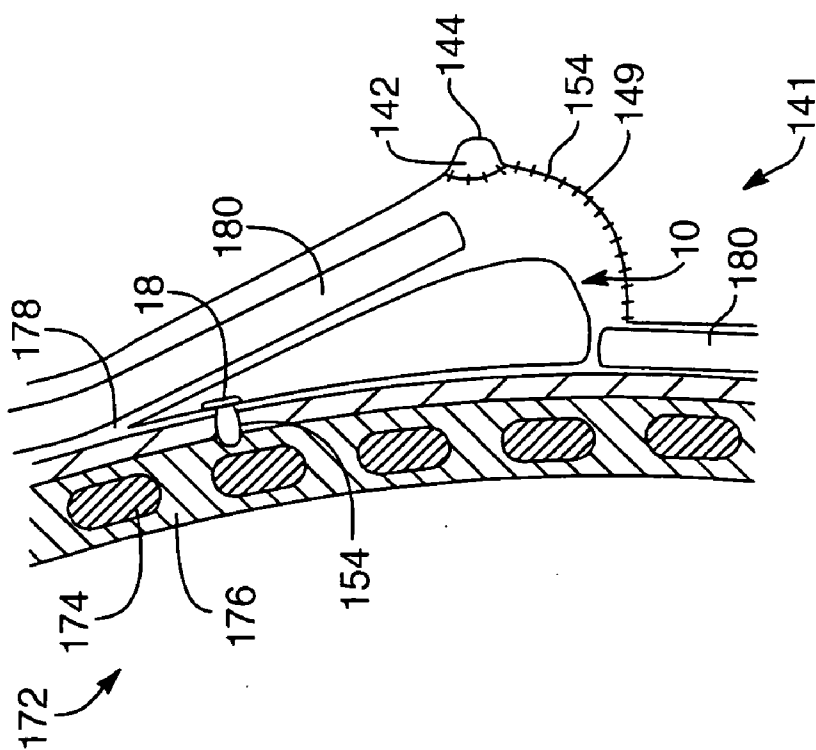


FIG. 22A

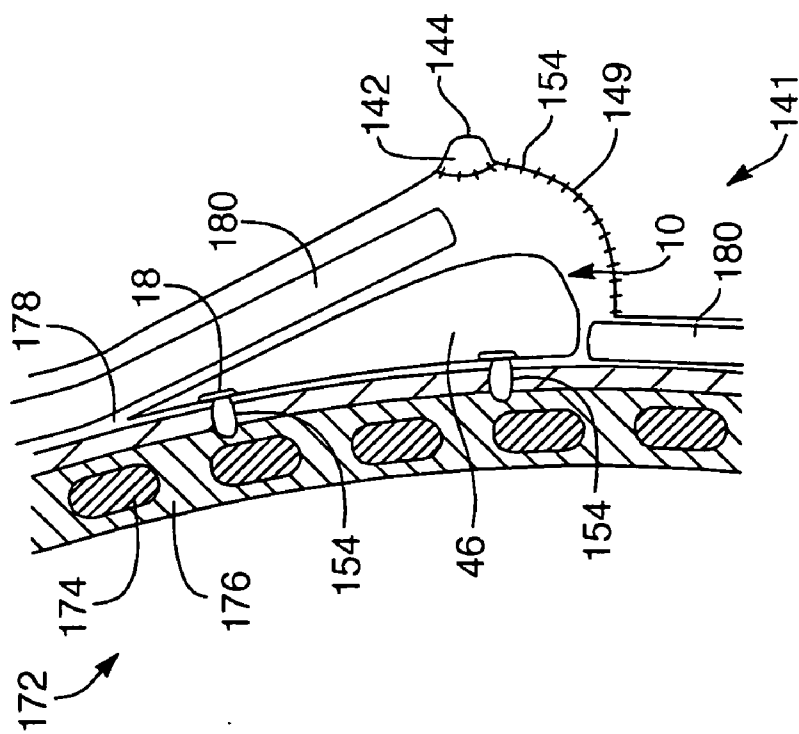


FIG. 22C

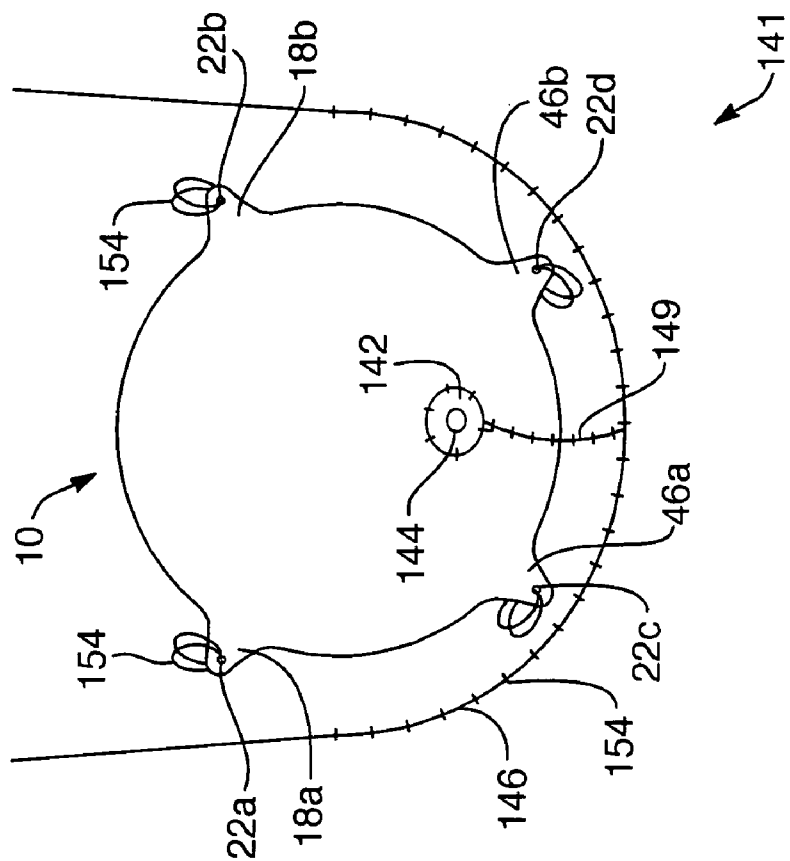


FIG. 22D

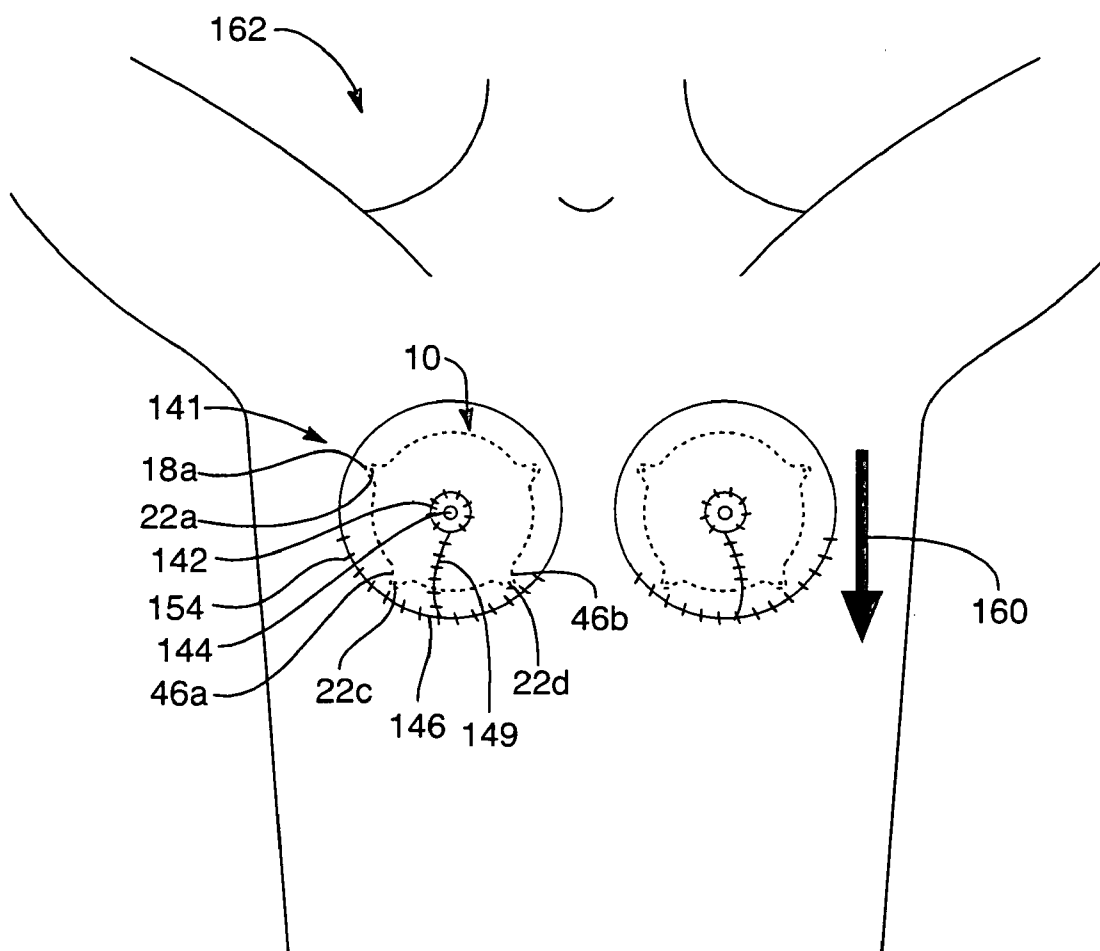


FIG. 23

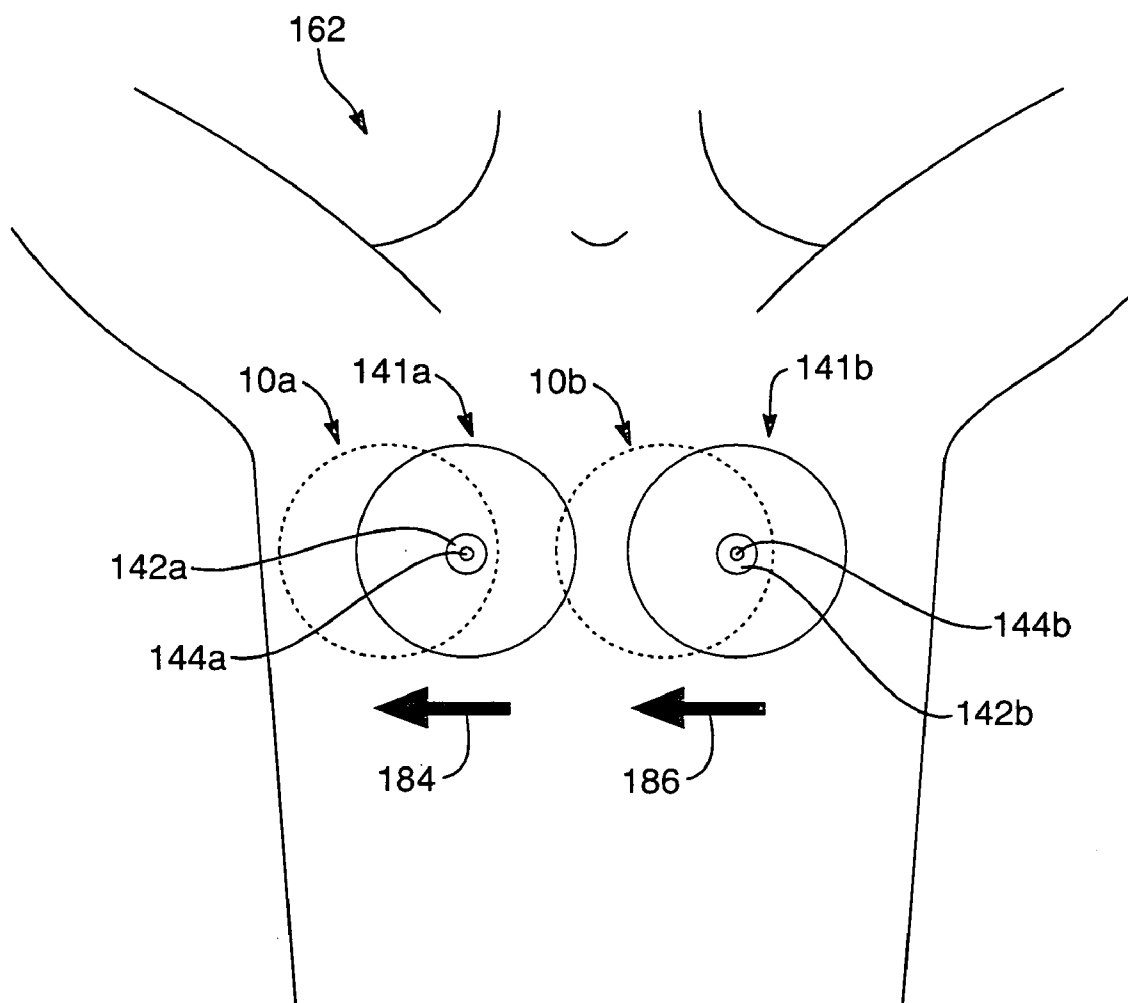


FIG. 24

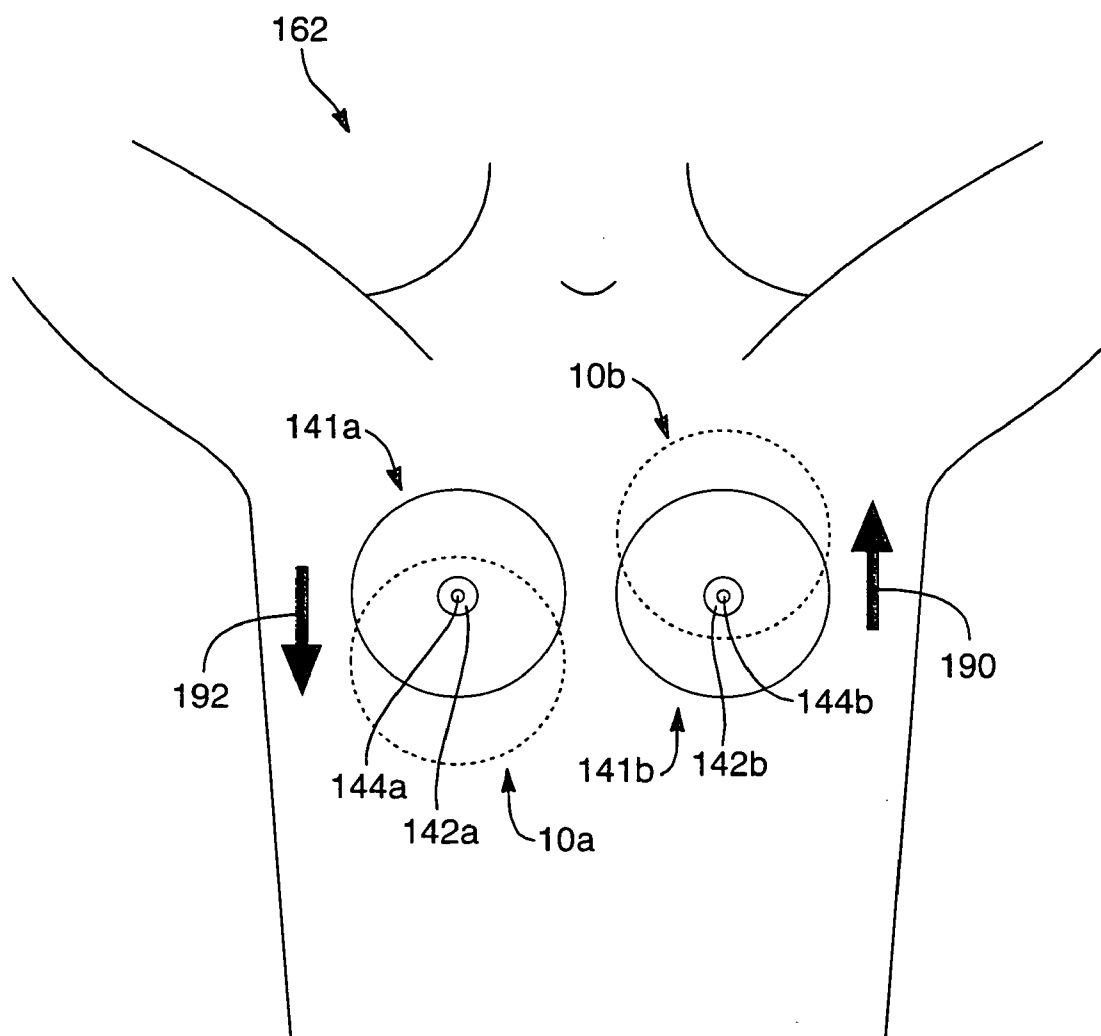


FIG. 25

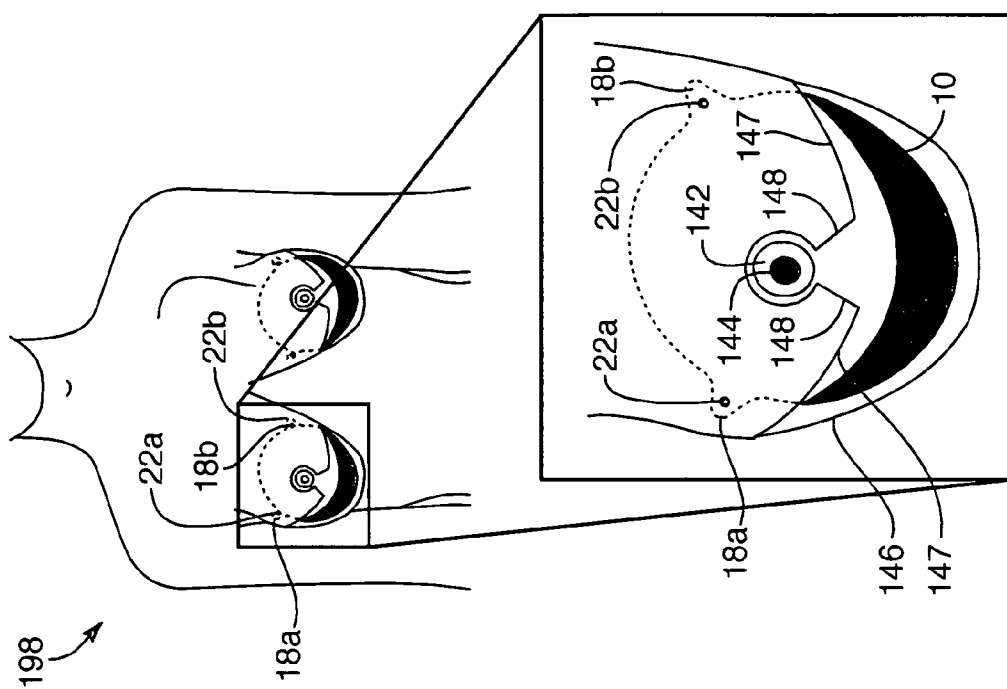


FIG. 26B

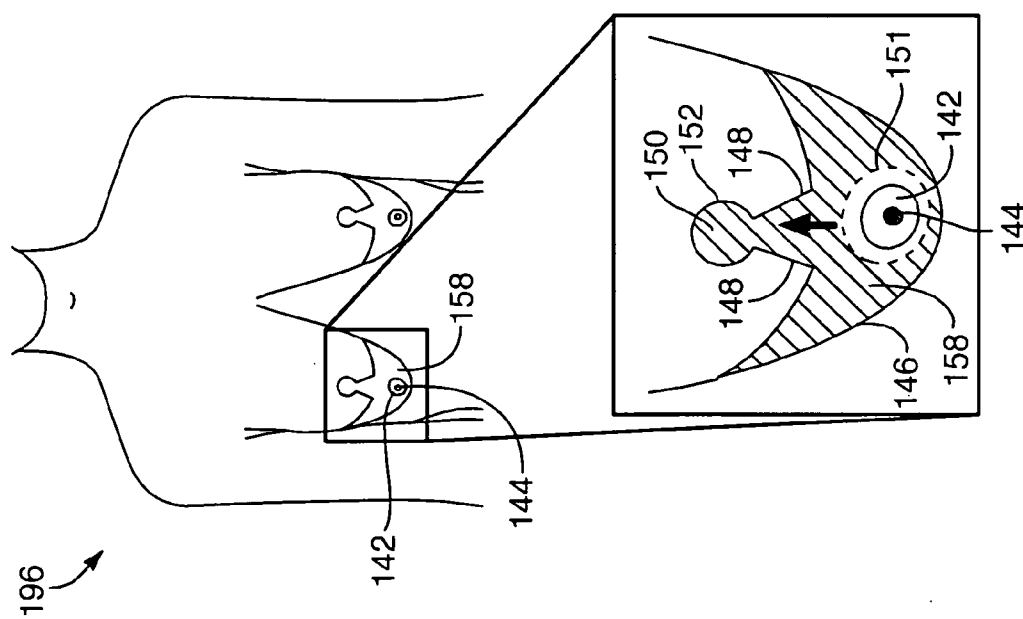


FIG. 26A

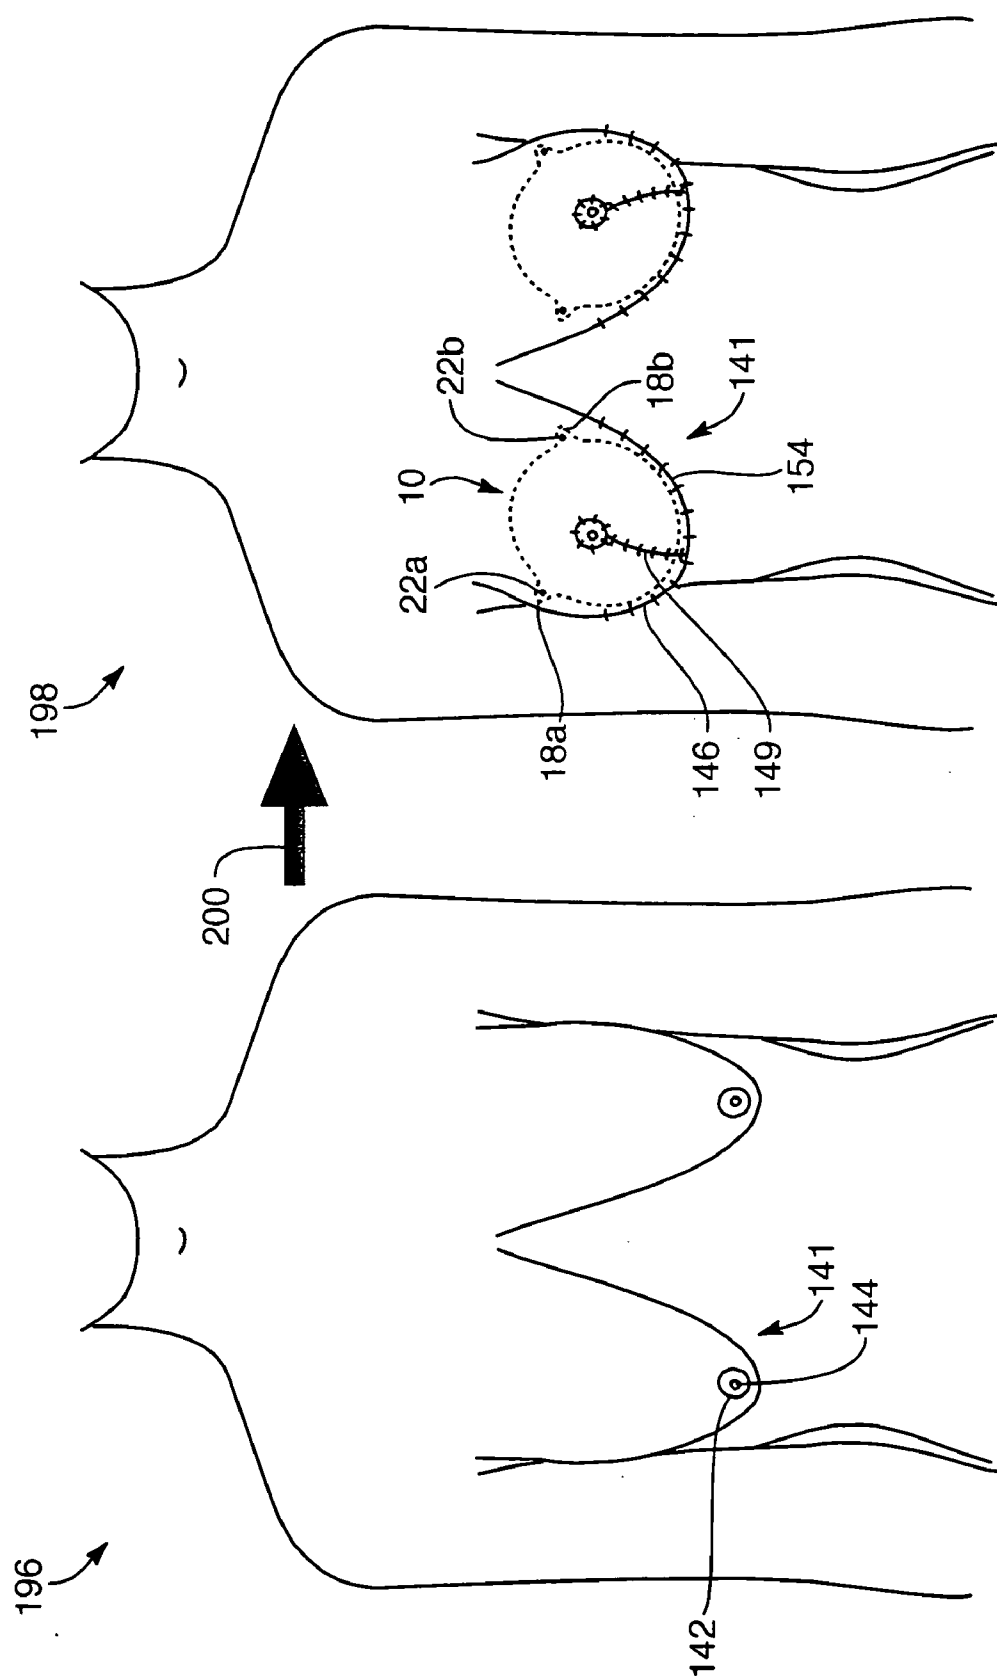


FIG. 27

MASTOPEXY STABILIZATION APPARATUS AND METHOD

RELATED APPLICATIONS

[0001] This application claims is a continuation of co-pending U.S. patent application Ser. No. 10/771,776 filed on Feb. 4, 2004 and entitled MASTOPEXY STABILIZATION APPARATUS AND METHOD.

BACKGROUND

[0002] 1. The Field of the Invention

[0003] This invention relates to apparatus and methods for mastopexy or "breastlift" procedures and devices, and more particularly to devices and methods for increasing stability and longevity of mastopexy operations with augmentation.

[0004] 2. The Background Art

[0005] Plastic and cosmetic surgery has existed for many years as a particular field of medicine, and surgery in particular. Reconstruction after accidents has been developed in order to replace, reconfigure, or otherwise ameliorate damaged tissues subjected to trauma through accident or other causes of disfigurement. In some circumstances, physiological difficulties arise due to damaged, broken, traumatized, or simply disproportionate members of the body. As the skill and experience of medical practitioners has increased, elective surgeries have become more common.

[0006] For example, cosmetically, breast enhancement surgeries have become more commonplace. Enhancement procedures may include augmentation of size and shape, as well as selective reduction.

[0007] One field of cosmetic surgery involves mastopexy or "breastlift" surgery. Factors such as pregnancy, nursing, physical activity, time, gravity, and the like may affect skin thickness and tone. As skin loses elasticity, shape and firmness consequently decline over time. Breastlift, or mastopexy, is a surgical procedure to raise and reshape breasts. However, no surgery can permanently delay the effects of gravity. Accordingly, mastopexy may alter size, shape, positioning, and volume of breasts. Bio-compatible implants may be inserted under muscle, or under mammary tissues above muscle in order to alter both firmness and size.

[0008] The causes of deformation for which mastopexy provides at least a partial remedy may include both stretching of skins and tissues, as well as a loss of elasticity of skins and tissues. Loss of elasticity is a result partly of age, and partly a result of the stretching processes. That is, all materials that are inherently elastic use up part of their elasticity in the process of stretching. Not all stretching is elastic; some is permanent with age, skin tissues are less elastic. Also, underlying tissues may thin, losing fullness and shape. Accordingly, these effects can continue.

[0009] Of particular concern is the continued effect of motion and gravity upon on mass subject thereto. Accordingly, continued stretching and drooping may occur after mastopexy. Moreover, in the situation of an augmentation procedure in conjunction with a mastopexy, an implant itself may add additional weight subjecting tissues to further invasion as gravity draws that mass downward. Thus, it would be an advance in the art to provide a method and

apparatus to support an implant against the acceleration of gravity, in order to stabilize tissues after a mastopexy operation.

[0010] Moreover, complications may occur either unintentionally or simply as a matter of course. For example, any time the body is confronted with a foreign object, even though not chemically or biologically reactive therewith, the body tends to form scar tissue, and wall off the foreign object. Thus, scar tissue may form about an implant. Conventionally, the formation of a scar or a capsule has been relied upon to stabilize the position of an implant. However, implants may rupture, and scar tissue may rupture, altering the containing capsule. Also, the fibroblasts within scar tissue tend to contract. Nature shrinks scars from their initial size as the fibroblasts tend to organize and orient themselves like crystals, and then draw themselves shorter. However, such a contraction of scar tissue in an oblique shape results in closing up the area containing a volume. The result is a tendency toward spherical shape and higher pressures. Thus, texture, firmness, and shape may alter dramatically. What is needed is an apparatus and method for minimizing damage to body tissues, minimizing scarring, as well as an apparatus and method that do not rely on scar tissue formation to maintain dimensional stability temporarily during healing, nor permanently. Positioning is needed that does not wait for the many weeks required for scar tissue to form and stabilize.

[0011] Aesthetics may be effected by the reaction of bodily tissues to the presence of an implant. Likewise, alterations in the structure of an implant may also result in undesirable alterations in aesthetics. For example, capsular contracture (scar tissue shrinkage) may not only result in alteration of shape and firmness, but may actually result in rupture of an implant. Likewise, capsular contracture may result in selective shifting of position. Likewise, a rupture of scar tissue may result in shifting the location of an implant.

[0012] Thus, for example, what is needed is a system and method for temporary vertical load support in order to relieve the stress on tissues that must heal, in order to minimize scarring. Likewise needed is support for temporary sutures. That is, after surgery, suturing requires time to heal. Scar tissues will increase in width or area if loaded by weight or pressure. Likewise, stress of any wound or a suture location will cause considerable discomfort. Likewise, during scar tissue formation, weight or pressure against scarring tissue will cause additional discomfort.

[0013] Likewise, it may be advisable and useful to provide permanent support from weight in order to longer maintain the effects of a successful mastopexy procedure. Also, while many persons are involved in athletic pursuits as a means to recreation or improved health, vertical support against accelerations due to gravity or dynamic motions of an athlete would further enhance and maintain the effects of successful mastopexy.

[0014] Scarring responds to loading. If a scar in the skin is subjected to force, the scar will typically respond by localized damage that itself must heal by scarring. Accordingly, scars may be widened during healing by continued stretching or trauma. Moreover, many tissues in the body are comparatively soft. Accordingly, they are restrained by not only their own material properties and surrounding connective tissues but by the support from skin. Accordingly, a load

on any particular part of soft tissue may be transferred, much as it would in a liquid, to exert a generalized omni-directional pressure. Thus, gravitational loads on an implant may result in a generalized omni-directional pressure against sutured tissues, causing additional stretching and exacerbation of scars.

[0015] It would be an advance in the art to provide vertical support against loading tissues directly as the force of gravity on scars and sutures. It would be an advance as well to provide support generally against the transfer of pressure into tissues in any direction.

[0016] As a capsule forms about a foreign body inserted into tissues, scarring forms around the periphery thereof. However, comparatively soft tissues may yield, tear, or otherwise permit migration of a prosthesis or implant. In the absence of other stabilization, and in the presence of unhealed scars, or even after scars have ostensibly formed interior to tissues to stabilize an implant, implants may migrate down or sideways. For example, lateral migration toward the arm, medial migration toward the sternum, downward migration toward the abdomen (inferior), as well as superior migration toward the collarbone, are all possible. In the presence of gravity, most common effects are typically lateral and inferior migration.

[0017] Thus, it would be an advance in the art to provide an apparatus and method for maintaining position laterally, medially, inferiorly, and superiorly against migration. Similarly, it would be an advance in the art to provide support against migration loads tending to shift locations of implants due to the stresses of the implant against other tissues during physical activity.

[0018] Many persons assume a symmetry to the human body that does not actually exist. Symmetry has been considered by those who study aesthetics to be a particularly pleasing effect. Nevertheless, the human body is not necessarily formed symmetrically. However, the lack of symmetry is still not desirable. Thus, in response to a mastopexy operation, symmetry may be sought as highly desirable. In fact, symmetry may be sought to a degree not originally present. Regardless, it would be an advance in the art to provide line symmetry to the degree possible as a result of mastopexy both along vertical (superior-inferior) lines and horizontal (lateral-medial) lines orthogonal thereto. Thus, positioning implants reliably with respect to one another is desirable, so they are each located along a lateral-medial direction at the same relative location relative to the remainder of the anatomy, positioned in a superior-inferior location equal with respect to one another, and properly located with respect to other anatomical features.

[0019] In yet another condition, certain implants are formed of a comparatively soft and resilient solid. Such implants tend to be formed of close-cell foamed polymers. Other implants contain gels. Yet other implants are formed of a shell or skin filled with a saline, glucose, or other solution that will be tolerated and disposed of by the body in the event of exposure to tissues.

[0020] The term "microbleed" describes migration of a liquid species through a solid. For example, a silicone liquid or gel may migrate through a wall, causing a reaction with tissues outside an implant. With the use of saline or glucose solutions, any microbleed of materials migrating through a

wall of an implant may be absorbed and handled by the body through its normal processes. One result is the decrease of scarring in response to microbleeds of somewhat incompatible materials.

[0021] That is, for example, at a molecular or atomic level, chemicals migrate through other chemicals. Thus, an "impervious" material is really not so. Migration is simply very, very slow. Nevertheless, individual atoms, molecules, or the like may migrate through a comparative solid from one surface of a wall to the opposing surface of the wall.

[0022] As with all artificial procedures, precision can affect perceived quality of a result. Inasmuch as subsequent relaxation or drooping of tissue may occur after a mastopexy operation, surgeons may overcompensate in advance by "overlifting." Since the ultimate response of any specific body is a matter of some conjecture, problems may arise with overlifting not subsequently eliminated by additional stretching of tissues under the effects of gravity. Likewise, since tissues in the body are not necessarily identical or symmetrical, a certain degree of symmetry achieved during a lifting or mastopexy operation may be lost subsequently by disproportionate deflection (movement, stretching, etc.) after a mastopexy operation.

[0023] What is needed is a system and apparatus for providing mastopexy augmentation that provides a comparatively broad tolerance for a surgeon in the procedure involved, while resulting in a comparatively narrow tolerance or variation in the ultimate outcome. A procedure is needed that provides options for locating an implant, but subsequent, reliable stability.

[0024] Textures and dynamic reactions of implants vary. Some implants are formed of comparatively stable and lightweight foamed polymers, whereas others are formed of shells containing comparatively viscous liquids or gels. Yet others are comprised of shells of thin, flexible polymers filled with comparatively inviscid liquids such as saline and glucose.

[0025] Much of the driving force behind cosmetic surgery arises from personal valuations of aesthetics. One somewhat unnatural consequence of inviscid fill materials in implants is a dynamic ripple effect in response to motion or acceleration. Dynamic ripples may be visible on the surface of the skin. Dynamic ripples, sometimes called wrinkling, may occur due to the wave-like motion of subcutaneous liquids as filler within an implant.

[0026] Soft tissues tend to have a more solidus nature, although soft, and easily deflected. Nevertheless, connective tissues have a certain elasticity present therein providing a certain texture and stability. By contrast, inviscid liquids may result in surface rippling, particular if the implant is only sub-glandular rather than sub-muscular.

[0027] Thus, what is needed is an improved apparatus and method providing a simple, reliable, aesthetically appealing mastopexy with augmentation. Reduced side effects, including internal scarring about the capsule surrounding an implant, as well as reduced scarring, stretching, and the like of sutures in the exposed skin would be desirable. Temporary and permanent support of implants, in order to relieve tissues from the forces of gravity in combination with the weight of implants, would be an advance in the art. Stabi-

lization in order to reduce scarring, stiffness, capsular contraction, and scarring in reaction thereto would be an advance in the art.

[0028] It would be an advance in the art to reduce microbled diffusion of filler material by reducing forces or pressures driving such diffusion. Reducing effects of such diffusion should include reducing weight, stress, pressure, and the like tending to strain, stress, damage, or irritate tissues surrounding an implant. It would be an advance in the art to provide increased resistance to inviscid implant fillers by stabilizing the outer shell more substantially, while eliminating or reducing substantially the need for overlifting. Reducing the reliance on scarring as a containment mechanism for the capsule surrounding an implant would likewise advance the art.

BRIEF SUMMARY AND OBJECTS OF THE INVENTION

[0029] In accordance with the foregoing, a method and apparatus for stabilizing mastopexy operations may include providing a containment vessel, serving as an implant, comprised of a container, bag, molded shell, or the like for holding a filling material. The back plane or back surface of the implant may conform to the chest wall below (within) or above (without) the pectoral muscles. The implant may have anchor tabs, sutures, tethers, or the like for suturing or otherwise anchoring the implant against the chest wall, against muscles, or the like in order to stabilize the location and support the weight thereof. Sutures or other anchors may serve during scarring and temporary duration of the healing process, as well as permanently.

[0030] Such an apparatus and method may reduce complications including contracture (contraction) of capsular scars, may reduce scar formation, may reduce the risk of deflation or rupture of implants as well as reducing rupture of scars formed in the capsular region. Moreover, an apparatus and method in accordance with the invention may reduce excessive firmness and stabilize both the aesthetic and dynamic shape of an implant.

[0031] In certain embodiments, an apparatus and method in accordance with the invention may reduce thickening, firmness, and contraction of the layer of tissues surrounding an implant and forming a capsule therearound. In certain embodiments, a shell may be formed of a polymeric material, a reinforced polymer, an expanded polymer, or the like, and may contain a liquid, gel, solid, or foam. In one presently contemplated embodiment, a silicone compound, such as dimethylsiloxane composition may form a shell, and may have embedded therein certain fibrous materials, such as Kevlar®, nylon, rayon, dacron, suturing materials, combination thereof, or the like to provide additional tensile strength and stability thereto. In certain embodiments, an implant or device in accordance with the invention may include tabs extending from the back plate thereof or back wall thereof for receiving a suture. Alternatively, sutures themselves may actually be embedded in the back plate (e.g. back surface or wall) of a device in accordance with the invention in order to simplify surgical procedures.

[0032] In certain embodiments, tabs may be co-located with or formed as extensions of the back surface of an implant device. Tabs may be located at the ten o'clock and two o'clock positions relative thereto. The 10:30 and 1:30

positions have certain stress support advantages. In an alternative embodiment, additional tabs may be located at other locations, such as, for example, a five o'clock and seven o'clock position, a four o'clock and eight o'clock position, or at a single six o'clock.

[0033] In an apparatus and method in accordance with the invention, sutures may use a variety of needle types, including a taper point for soft tissue, or a cutting point for piercing the chest wall in order to anchor to the rib cage. Sutures provided with a device in accordance with the invention may include a needle secured thereto and packaged therewith. Accordingly, a device may include a shell having a filling material placed in the shell during the manufacture thereof, or added subsequently by a surgeon.

[0034] In certain embodiments, reinforcing materials may include suture material embedded in at least the back plate or back wall of a device to provide tension support. In certain embodiments, multiple layers, and loops of suture material may be embedded in the back surface or back wall of an implant device in order to provide various locations for suturing. In certain embodiments, a suture may be embedded or introduced independently to secure a tab to muscle, ribs, cartilage, or the like.

[0035] A needle may arrive connected to suture material embedded in a back wall of an implant device. Needles may be provided with a protective covering, about themselves or including the suture material rolled up, in the form of a removable or breakable protection, such as a ring, loop, spool, cap, envelope, clip, or the like.

[0036] A method and apparatus in accordance with the invention may provide stabilization of the anatomical position of an implant associated with a mastopexy operation in order to reduce gravitational load on remaining tissue, scars, sutures, and the like. Accordingly, such a method and apparatus may reduce difficulties and negative results associated with the aesthetic appearance of the mastopexy result. They may reduce difficulties with improper positioning, lateral or medial displacement, inferior or superior displacement, unnatural shape, asymmetry as to superior-inferior positioning or relative positioning between pairs of implants, as well as lateral-medial symmetry between pairs of implants. Likewise, they may reduce rippling, wrinkling, and the like sometimes associated with the dynamic response of inviscid filling materials within a shell of an implant.

[0037] In an apparatus and method in accordance with the invention, temporary, permanent, or both types of support may be provided for an implanted device. Temporary support may be provided for reduction of scarring, migration, dislocation, and the like during healing. Permanent sutures may support implants during subsequent vigorous activities, athletics, and the like to improve the longevity or duration for which the mastopexy operation may be effective.

BRIEF DESCRIPTION OF THE DRAWINGS

[0038] The foregoing and other objects and features of the present invention will become more fully apparent from the following description and appended claims, taken in conjunction with the accompanying drawings. Understanding that these drawings depict only typical embodiments of the invention and are, therefore, not to be considered limiting of

its scope, the invention will be described with additional specificity and detail through use of the accompanying drawings in which:

[0039] **FIG. 1** is a schematic diagram of an apparatus in accordance with the invention illustrating optional embedded sutures, integrated tabs, and protection for needle associated with a suture material;

[0040] **FIG. 2** is a schematic of a front elevation view of one embodiment of an apparatus in accordance with the invention providing suturing loops extending from or near an edge of a back wall of an apparatus to receive sutures therethrough for anchoring using the suture material (line) and needle presented by the apparatus;

[0041] **FIG. 3A** is a schematic, front elevation view one embodiment of an apparatus in accordance with the invention relying entirely on sutures presented by the apparatus;

[0042] **FIG. 3B** is a schematic front elevation view of one alternative embodiment of an apparatus in accordance with the invention relying on tabs for receiving a suture therethrough;

[0043] **FIG. 4A** is a schematic side elevation view of one embodiment of an apparatus in accordance with the invention provided with alternatives of a presented suture and a tab for receiving a suture, which may be used in combination, or independently from one another as alternative embodiments;

[0044] **FIG. 4B** is a schematic side elevation view of one embodiment of an apparatus in accordance with the invention providing an anatomically shaped implant showing alternative embodiments of tabs, suture and needle, which may be used individually, exclusively, or in combination;

[0045] **FIG. 5** is a schematic front elevation view of an apparatus in accordance with the invention including multiple sutures along both the superior edges and inferior edges of the apparatus, and may be used in combination with the tabs of **FIG. 3B**, and the additional reinforcing loops of **FIG. 2**;

[0046] **FIG. 6** is a schematic front elevation view of one alternative embodiment in which homogeneously molded tabs extend from a back plate of the apparatus, including a reinforcing material extending therethroughout to transfer loads effectively;

[0047] **FIG. 7** is a schematic front elevation view of a device in accordance with the invention illustrating optional reinforcing material embedded in the back plate of a transparent or translucent implant device, and having suture materials embedded therein, as well as homogeneously molded tabs extending at the periphery of the device for receiving sutures, although the embedded suture and the integrally molded or homogeneously molded tab may be used exclusive of one another, or in combination with one another, and thus may be regarded as representing both alternative embodiments without each other, and the optional embodiment in which both are present;

[0048] **FIG. 8A** is a schematic front elevation view an alternative embodiment of an apparatus in accordance with the invention having diagonally-laid reinforcing fibers, which may be used with the homogeneously molded tabs, otherwise attached tabs, or the embedded suture material as illustrated in **FIGS. 1-7**;

[0049] **FIG. 8B** is a schematic front elevation view an alternative embodiment of an apparatus in accordance with the invention having diagonally-laid reinforcing fibers, which may be used with the homogeneously molded tabs, otherwise attached tabs, or the embedded suture material as illustrated in **FIGS. 1-7**, and including in this embodiment additional inferiorly located stabilization tabs, which may also be used in conjunction with, separately from, or absent in favor of, inferiorly located suture lines;

[0050] **FIG. 9A** is an exploded, side elevation, cross-sectional view of one embodiment of a laminated back plate for a device in accordance with the invention;

[0051] **FIG. 9B** is a side elevation, cross-sectional view of a back plate in accordance with the invention, formed either by lamination of the layers of **FIG. 9A**, or by infusion molding of a resin into a reinforcing gauze or fiber reinforcing material;

[0052] **FIG. 10** is a perspective view of one embodiment of a suture material presented in an implant device, and illustrating a local reinforcing member for accommodating and redistributing localized stresses induced by the suture;

[0053] **FIG. 11** is a perspective view of various embodiments of needles, connections to sutures, and points of needles for use in an apparatus and method in accordance with the invention;

[0054] **FIG. 12** is a perspective view of one embodiment of a protection device for hiding a point of a suture needle embodied in an apparatus in accordance with the invention;

[0055] **FIG. 13** is a perspective view of one embodiment of a cover for a suture needle for use in an apparatus in accordance with the present invention;

[0056] **FIG. 14A** is a perspective view of one embodiment of a protective envelope for a suture and needle in accordance with the invention;

[0057] **FIG. 14B** is a perspective view of a coiled-tube protective cover for a needle in accordance with the invention;

[0058] **FIG. 15** is a schematic block diagram of a mastopexy process including insertion, orientation and anchoring in for an apparatus and method in accordance with the invention;

[0059] **FIG. 16** is a schematic block diagram of the implantation process of **FIG. 15**;

[0060] **FIG. 17** is a schematic block diagram of one alternative embodiment, and illustrating various alternative and optional steps therein, for manufacture of an apparatus in accordance with the invention;

[0061] **FIG. 18** is a schematic front elevation view of a mastopexy incision pattern in accordance with the invention;

[0062] **FIG. 19** is a schematic front elevation view of a mastopexy suture pattern in a closed configuration as per an apparatus and method in accordance with the invention;

[0063] **FIG. 20** is a schematic front elevation view illustrating various components of force and pressure exerted, as a result of mastopexy, upon the closing suture to be resisted in accordance with the invention;

[0064] FIG. 21A is a schematic, side elevation, cross-sectional view of an augmented mastopexy illustrating anchoring of an implant in accordance with the invention;

[0065] FIG. 21B is a schematic front elevation view of the illustration of Figure . . . the anatomy and implant of FIG. 21a;

[0066] FIG. 21C is a schematic, side elevation, cross-sectional view of an inferiorly and superiorly anchored implant in accordance with the invention;

[0067] FIG. 21D is a schematic front elevation view of the system of FIG. 21C, wherein FIGS. 21A-21D constitute sub-glandular insertion of augmentation implants;

[0068] FIG. 22A is a schematic, side elevation, cross-sectional view of an apparatus in accordance with the invention secured by a method in accordance therewith for sub-muscular insertion of an implant in association with a mastopexy procedure;

[0069] FIG. 22B is a schematic, front elevation view of the anatomy and device of FIG. 22A;

[0070] FIG. 22C is a schematic, side elevation, cross-sectional view of the anatomy and device in accordance with the invention, connected by a method in accordance with the invention in a sub-muscular configuration;

[0071] FIG. 22D is a schematic, front elevation view of the system of FIG. 22C, wherein the apparatus of FIGS. 22A-22B include only superiorly mounted, homogeneously formed suture tabs and the apparatus of FIGS. 22C-22D includes both superiorly and inferiorly mounted suture tabs for mastopexy stabilization in accordance with the invention;

[0072] FIG. 23 is a schematic front elevation view of the orientation and load characterization against the suture locations as driven by the weight of implants in accordance with the invention;

[0073] FIG. 24 is a schematic front elevation view of the forces and propensity to or toward lateral and medial displacement of implants to be resisted by a method and apparatus in accordance with the invention;

[0074] FIG. 25 is a schematic, front elevation view of the forces and propensity toward inferior and superior migration of implants resisted by an apparatus and method in accordance with the invention;

[0075] FIG. 26A is a schematic front elevation view of the region of tissue to be incised and excised in a mastopexy in accordance with the invention;

[0076] FIG. 26B is a schematic front elevation view of insertion of an apparatus in accordance with the invention prior to closure of incisions, and after excision of removed materials; and

[0077] FIG. 27 is a schematic front elevation view of the transformation in accordance with an apparatus and method of the invention from a ptosis condition to a lifted and augmented condition.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0078] It will be readily understood that the components of the present invention, as generally described and illustrated

in the Figures herein, could be arranged and designed in a wide variety of different configurations. Thus, the following more detailed description of the embodiments of the system and method of the present invention, as represented in FIGS. 1 through 27 is not intended to limit the scope of the invention, as claimed, but is merely representative of the presently preferred embodiments of the invention. The presently preferred embodiments of the invention will be best understood by reference to the drawings, wherein like parts are designated by like numerals throughout.

[0079] Referring to FIG. 1, an apparatus 10 or implant 10 may be formed to include a back plate 12 and a pocket 14 of a flexible, elastically deformable material. The pocket 14 and back plate 12 may be formed as a single homogeneously molded container. The back plate 12 may typically be formed to appear flat, and the pocket 14 may be rounded, hemispherical, or anatomically shaped. In some presently contemplated embodiments, the pocket 14 represents a portion of substantially a hemisphere and the back plate 12 represents a substantially flat base thereto.

[0080] The back plate 12 and thus the overall apparatus 10 may be formed to have an outside diameter 16 and a corresponding wall thickness thereof. The material of the implant 10 or apparatus 10 may be transparent, translucent, or opaque. In certain presently contemplated embodiments, the material may be substantially transparent, wherein the shell may actually tend to scatter light diffusing the image of light therethrough somewhat.

[0081] In one embodiment, tabs 18 may be homogeneously formed with the back plate 12 to project therefrom for securing the apparatus 10 to the anatomy of a user. As an alternative, as an adjunct, or as a combination with the tab 18, a suture 20 may be embedded to extend from the back plate 12. An aperture 22 in the tab 18 may be formed explicitly during manufacture. Alternatively, an aperture 22 may simply be formed by perforation during the process of suturing to the tab 18. Trailing letters on reference numerals herein indicate specific instances of the generalized item identified by the leading reference numeral.

[0082] In certain embodiments, a tab 18 may be formed to use in conjunction with a previously embedded suture 20. In yet another embodiment, the suture 20 may be embedded to extend from the back plate, having a length 24 or extra length 24 of suture material for completing a suture. Likewise, an anchor portion 26 of the suture line 20 may extend radially into the back plate 12 a distance, or even completely across the diameter 16 of the back plate 12. Thus, the suture 20 may provide substantial support of the back plate 12 and apparatus 10.

[0083] At a distal end of the suture line 20, a protective sleeve 28 may enclose a surgical needle 30 secured thereto. A surgical needle 30 may be threaded by a surgeon with surgical suture line 20, or may come premanufactured or preconnected to the suture line 20. The extra length 24 may be enclosed with the needle 30 in the sleeve 28.

[0084] In certain embodiments, various protective sleeves 28 may be used. For example, a tubular protection device 28a or tube 28a may enclose a portion or all of a needle 30. At a minimum, any cutting surface or point of the needle 30 is best protected in order to protect both a patient and the device 10 from puncture.

[0085] In an alternative embodiment, a coil **28b** of tubular material may extend circumferentially through **180** or even 360 or 720 degrees. Accordingly, the ring **28b** forms a protective sheath, round in shape to prevent snagging prior to deployment of the needle, and if sufficiently elastic and sufficiently rigid or stiff, may provide the ability to clip a roll of extra suture material **24** therebetween. A diameter **32** of a tubular material may be oversized to receive a needle easily, relying on the curvature of the needle to distort and secure the tube **28** thereto. Alternatively, the coil **28b** may be formed of a diameter **34** compatible with the arc of a needle **30**, and have a diameter **32** selected to properly receive the cross section of a needle **30**.

[0086] In one embodiment, a simple cap **36** may be formed to protect a needle point. Various materials, including rubber, latex, other elastomeric polymers, hard plastics, waxes, cork, expanded polymer foams, and the like may be used to form the cap **36**. In one embodiment, the cap **36** may be formed to break. In other embodiments, the cap **36** may be comprised of a hard outer shell to resist penetration by the needle **30**, with an inner material formed of a softer material such as wax, plastic, foamed plastic, rubber, elastomeric material, or the like for securing the needle **30** until ready for use.

[0087] In yet another alternative embodiment, a clip **40** may receive a needle snapped thereinto. The clip **40** may have rounded edges and a circular, rectangular or other polygonal shape. The clip **40** may be formed to provide little or no resistance to motion across a tissue surface, when secured to the device **10**, in order to minimize interference prior to deployment of the needle **30**.

[0088] In yet another alternative embodiment, a simple plastic, paper, fabric, or other type of envelope **38** may be formed to receive and hold a needle and suture materials. A flap **39** may be removably secured to hold the suture **20** and needle **30** in place until deployed. After location of the apparatus **10** or implant **10**, the envelope **38** may open to provide the needle **30** and suture **20** for anchoring the apparatus **10**.

[0089] Referring to FIG. 2, in certain embodiments, additional loops **43** or embedded materials such as reinforcing strands **43** or embedded suture materials **43** may extend radially from the periphery of the back plate **12** to provide anchor points for connecting the suture **20**. In certain embodiments, the needle **30** and suture material **20** or line **20** may simply pierce a tab **18**. Alternatively, reinforcing strands **43** or embedded loops **43** may extend from the periphery of the back plate **12** to receive one loop or multiple loops of the suture **20**.

[0090] The pocket **14** and back plate **12**, are typically very flexible. In some embodiments, the pocket **14** and back plate **12** may be formed seamlessly by a method such as rotational molding in order to eliminate seams, edges, mold flashing, and the like. Meanwhile, filler may occur either during the manufacturing process, or subsequent thereto. During installation (e.g. insertion and anchoring), or even just before or after insertion of the apparatus **10**, the pocket **14** may be filled with a suitable material.

[0091] Typical filler materials **45** may include soy oil, saline solution, silicone gel, hydro gel, polyvinylpyrrolidone (PVP), polyethylene glycol (PEG), hyaluronic acid, or the

like. Materials may be chosen for their density, viscosity, and biocompatibility, as well as the ability to either resist microbleeding (e.g. weeping, microscopic level transmission through walls), and the like. Likewise, materials may be selected in order to optimize the ability of the body to deal with them in trace amounts in the instance of a microbleed.

[0092] Fill materials may be selected in accordance with various features including shell compatibility, the antimicrobial nature thereof, and the stability over time. Stability may include various properties including dimensional stability, texture, chemistry, and the like. Similarly, materials may be selected for their nonimmunogenic and nonallergenic properties. Most materials should be screened to assure that they are noncarcinogenic, nontoxic, and otherwise completely compatible biologically. This may be significant in the event of microbleeding through the walls of the back plate **12** and pocket **14**, or in the event of a rupture or leakage into the body tissues.

[0093] Radiolucence is a useful property in assuring that radiological evaluations still operate properly. For example, a mammogram in the presence of radiopaque materials can cause problems with the proper operation of x-ray systems.

[0094] A material that is absorbable by the body may protect against dangerous consequences in the possible event of rupture of a shell. Rupture of the shell might release materials into tissues of the body. An ability to absorb or metabolize a filler material **45** may be a high priority feature in order that escaped materials be carried away by the body waste disposal functions rather than remaining to migrate to various places where they may cause eventual difficulties.

[0095] Maintaining pH-neutral conditions, and osmotically neutral conditions will also assist in the event of possible leakage or rupture. The ability to maintain a material wrinkle-free or ripple-free is typically a function of viscosity and the construction of the apparatus **10**. The palpability of material may affect the choice since solidus materials may be detectable, but inviscid materials may be detectable somewhat as being less viscid than natural materials. Similarly, materials that have suitable cost, rather than being exotic and expensive, as well as materials that will minimize the effect of capsular contracture are also to be sought. Capsular contracture is usually instigated by microbleeding of small amounts of materials that cause reaction by the body.

[0096] Referring to FIG. 3A and FIG. 3B, the suture **20** may be embedded within the back plate **12** in a direction devised to optimize support by the suture **20** and the access thereto. In one embodiment, the embedded strands **44** of the suture **20** may extend across the back plate **12** a distance select to provide adequate transfer of load from the suture **20** into the back plate **12**. Multiple suture lines **20** may be embedded by way of individual strands of a braided suture. Alternatively, a single braided suture **20**, or band may extend from the periphery of the back plate **12** for anchoring to the tissue of a chest wall or of chest muscle (e.g. pectoralis major).

[0097] Referring to FIG. 3B, an alternative embodiment may rely on no embedded sutures **20** presented, and instead rely only on tabs **22**. In the illustrated embodiment, superior tabs **18a**, **18b** may also be augmented by inferior tabs **46a**, **46b**. As a practical matter, relatively minor loads exist to

require the use of the tabs **46**. By the same token, more athletic persons may desire, or it may be advantageous to provide, the tabs **46** to protect against dynamic loads. That is, the tabs **18a**, **18b** normally protect against gravitational loads (weight) of the apparatus **10** acting against tissues therebelow. However, in dynamic activities such as running, and the like, the inferior tabs **46a**, **46b** may provide dynamic stabilization against superior, lateral-medial, or transverse movement (toward and away from the chest wall).

[0098] Referring to **FIG. 4A**, in one presently contemplated embodiment, the apparatus **10** may be substantially formed as a more-or-less flat back wall **12**, back plane **12**, or back plate **12**, and a hemispherical pocket **14**. The projection **47** or depth **47** of the pocket **14** may be selected according to the manufacture of the pocket **14** or the amount of the fill material **45** enclosed therein. A surgeon at or shortly before the time insertion of an apparatus **10** may alter or introduce the filler **45**. In the illustrated embodiment, a suture **20** is shown, but the apparatus of **FIG. 4A** may also be used with any of the configurations illustrated in **FIGS. 1-3B**.

[0099] Referring to **FIG. 4B**, an alternative embodiment of an apparatus **10** may include a "anatomically formed" pocket **14**. This embodiment, a preferential projection **47** may favor the inferior portion of the pocket **14**. The pocket may be shaped to produce this effect. Nevertheless, in the apparatus **10** in accordance with the invention, it has been found that no additional anatomic drop or preferential location of the maximum projection **47** is required to produce the desired and adequate augmentation effect.

[0100] Referring to **FIG. 5**, the apparatus **10** may include multiple sutures **20** embedded in the back plate **12**. In certain embodiments, the locations of the extensions or presentation of sutures **20a**, **20b** may approximate the ten o'clock and two o'clock positions. Similarly, the presentation of the sutures **20c**, **20d** may approximate the five o'clock and seven o'clock positions. Thus, the sutures **44a**, **44b** embedded in the back plate **12** may not necessarily cross in the center of the apparatus **14**. In alternative embodiments, a more symmetric support system may be formed. That is, the locations of the crossing of the embedded sutures **44a**, **44b** may be centered or placed in any other suitable location in order to provide both a supporting force therefrom, and a proper location of the sutures **20** for use. One good spacing places sutures **20** at ninety degrees from one another.

[0101] Referring to **FIG. 6**, one embodiment of a reinforced composite material in a backplate **12** may include a reinforced fiber composed of either single parallel strands, randomly oriented strands, or a mesh fabric having a selected interstitial distance **49** therebetween. As a practical matter, reinforcing fibers **48** may be oriented in substantially horizontal and vertical directions in order to provide multi-directional stress support. In the embodiment of **FIG. 6**, the tabs **18** provide locations for anchoring the apparatus **10** to the body.

[0102] Referring to **FIG. 7**, a similarly arranged pattern of reinforcing fibers **48** may be embedded within a backplate **12** of an implant **10** or apparatus **10** to be supported by a suture **20**. Sutures **20** may be arranged at suitable locations about the periphery of the backplate **12** in order to provide both support, orientation, and stabilization in a lateral-medial direction, as well as support in a superior-inferior direction.

[0103] In certain embodiments, either the reinforcing fibers **48**, or other fibers specifically included for the purpose, may extend out from the edges of the backplate **12** to form loops **51a** at the superior edge of the backplate **12**, or as loops **51b** at the inferior edge of the backplate **12**. That is, for example, the suture **20** may be connected at multiple locations about the edges of the backplate **12** in order to reduce the localized stress.

[0104] For example, the tab **18** may be relied upon for receiving multiple loops of a suture **20**. Nevertheless, an array of loops **51** distributed about a region or the entire periphery of the backplate **12** may receive the suture **20**, thus distributing the overall loading, and providing additional support and stability.

[0105] Nevertheless, loops **51** need not be contiguous or integrated with the reinforcing fibers **48** forming the overall mesh **50**. The loops **51** may be formed of the suture material, a netting, or other looped, lacey, or otherwise perforated array of strands. In yet another alternative embodiment, the loops **51** may be absent and the suture **20** may simply be formed of a type of suture material suitable for supporting the entire load on a single strand. Thus, the suture **20** may actually be embedded as the only or one of many reinforcing strands **48**.

[0106] In certain embodiments, the variation in suture materials **20** may be substantial. Suture materials may range from those that biodegrade relatively quickly, to those that remain substantially permanently. For example, certain suture materials are monofilament synthetics. To the lay person, these appear like fishing line. Suture materials may also be braided. Sizes and strengths may vary by almost an order of magnitude. Accordingly, the suture **20** may be formed of reinforced, braided, or substantially larger gauges of material in order to improve its single-strand strength.

[0107] Suture materials **20** may include a variety of coated or uncoated sutures **20**. For example, sutures may be braided and uncoated, in order to provide better purchase against tissues. Nevertheless, some individuals may consider the apertures or interstices within braided sutures to harbor bacteria or the like. Accordingly, some sutures may be braided and coated in order to provide them more of a monofilament behavior or characteristic. Typically, monofilament sutures are formed as a drawn single fiber of a single synthetic material. Synthetic materials often have a stiffness and coefficient of elasticity that inhibit the ability to form a knot well. Likewise, the particular stiffness of synthetic monofilament materials may be substantially greater than that of graded multi-filament materials.

[0108] Nevertheless, monofilament suture materials typically provide low tissue reactivity. The smooth surface does not permit incursion of bacteria. Likewise, natural materials may actually be somewhat monofilament in nature, but are typically bioreactive, immunoreactive, or the like.

[0109] Some materials considered for use as the suture **20** may include vicryl that represents a material named polyglactin **910**. Such material maintains a high proportion of initial strength (e.g. seventy percent at ten days and thirty percent at twenty days). It can be biodegraded, absorbed, or otherwise disposed of by the body within sixty to ninety days.

[0110] An alternative material is a coated vicryl that contains a mixture of calcium stearate and polyglactin **370**

and maintains one hundred percent strength for approximately forty-five days before decreasing to seventy percent at fifty days. Another material is polydioxalane, also called PDS. This material retains seventy percent strength for approximately twenty-one days before reducing to about fifty percent strength in thirty-five days. This material is typically absorbed by the body within one hundred eighty days and results in minimal tissue reaction.

[0111] Catgut, for all the visions it conjures up, is actually a thinly refined strip of intestinal tissues from sheep, such as the submucosa of sheep, and may be taken from the intestinal serosa of cattle. This material maintains tensile strength for only approximately ten days before being degraded. Chromatized catgut may retain tensile strength for twenty to forty days, and all forms of catgut may result in a moderate degree of tissue reaction.

[0112] In addition, other materials may include nylon, a non-absorbable synthetic monofilament suture material. Ethibond is a braided, non-absorbable synthetic suture material formed of polyester fiber under a coating a polybutilale for lubrication, and having advanced tensile strength properties.

[0113] Natural silk is actually a protein fiber used for suture for millennia. Stainless steel may be used since it is inert, has virtually no tissue reaction, and can last permanently. Nevertheless, steel often presents some difficulty with knotting, since it has considerable stiffness. Nevertheless, a single strand of properly formed stainless steel may serve as a suture 20, and adequately support the entire weight of the apparatus 10.

[0114] Referring to FIG. 8, the mesh 50 may be oriented at a diagonal with respect to the principal axes of the device 10 or the human body. Since the use of multiple tabs 18 or multiple sutures 20 on opposite sides (lateral vs. medial) of the apparatus 10 will provide largely vertical (superior-inferior axis) support, the horizontal or lateral support (e.g. lateral-medial axis) will still be required. Expecting overlying tissues to provide this inherently may not be an accurate model. Accordingly, by spacing apart the tabs 18 or the sutures 20, stress may be distributed in both horizontal and vertical (nominal) directions. Accordingly, providing a bias orientation to the mesh 50 may more readily distribute stresses within the back plate 12 of the apparatus 10. The angles between the various fibers 48 may be right angles, or may be arranged at any other suitable angle.

[0115] Referring to FIG. 8B, an apparatus 10 in accordance with FIG. 8A may be anchored with inferior anchors 46a, 46b, as well as the superior anchors 18a, 18b. As a practical matter, all anchors 18, 46 may be referred to as anchors 18. As a matter of clarity, one may think of the anchors 46 as inferiorly oriented compared to anchors 18.

[0116] Referring to FIG. 9A, a mesh 50 may be laminated between layers 52, 54 of a backplate 12 material. For example, one may consider the cover 52 facing anteriorly on the backplate 12, with the base 54 facing posteriorly. A suitable bonding agent, including glues, polymers, solvents, or the like may be used for bonding the mesh 50 to the cover 52 and base 54. Alternatively, heat, ultrasonic waves, or another material may be used to embed one or both of the cover 52 and base 54 to the mesh 50. Similarly, the layers 52, 54 may actually extend beyond the edge of the mesh 50, in

order to seal the mesh 50 away from tissues, and the body. Alternatively, the backplate 12 may be formed with the mesh 50 extending from the cover 52 and base 54, in order to provide attachment access for sutures 20.

[0117] Referring to FIG. 9B, one embodiment of an apparatus 10 may include a matrix 56 of polymeric material cast around and through a mesh 50. Accordingly, an insert formed of the mesh 50 may be placed in a mold, and the resins melted or otherwise flowed to form the embedded matrix 56 of polymeric shell material. Again, the mesh 50 may extend through part of a tab 18, 46 or throughout the entire backplate 18. Alternatively, the mesh 50 may be formed as only a structural element extending through any selected portion of the backplate 12 or the remainder of the pocket 14 of the apparatus 10. For example, in one embodiment, the mesh 50 may actually be formed into the entire wall of the apparatus 10. Nevertheless, matters of structural integrity, as well as manufacturing simplicity and cost may direct the decision as to the mesh size 49, the extent of the mesh 50, the material thereon, the orientation of the angle between the mesh fibers 48, the enclosure or exposure of the mesh 50, and the like.

[0118] Referring to FIG. 10, with or without the presence of a mesh 52, a layer 57 and a layer 58 of a reinforcing material 59 may surround a suture 20 near the location where the suture 20 extends from the backplate 18. For example, in the illustrated embodiment, the suture material 20 may extend from an embedded portion 26 or anchor portion, through a reinforcement 59 defined by two layers 57, 58 enveloping the suture. Accordingly, the reinforcement 59 may be formed of a mesh, a film, or any suitable material calculated to distribute stress into the backplate 12 or other portion of the apparatus 10.

[0119] In one embodiment, the reinforcement 59 may actually be embedded partly within the backplate 12 or other portion of the apparatus 10, and extend partly away therefrom in order to receive the suture 20 therethrough. In yet another embodiment, the entire reinforcement 59 may be embedded within the backplate 12 or other portion of the apparatus 10, leaving only the suture to extend from the periphery of the apparatus 10 for access by a surgeon.

[0120] As a practical matter, a single strand of suture 20, may provide a very high localized stress capable of ripping, shearing, rupturing, or otherwise damaging the mechanical integrity of the apparatus 10. Accordingly, a reinforcement 59 may redistribute stress between the suture 20 and the underlying material of the apparatus 10.

[0121] Referring to FIG. 11, the apparatus 10 may include an embedded portion 26 or enclosed portion 26 of the suture 20. The suture 20 extending therefrom may include a coil 24 or extra length 24 of suture material 20 to be used by a surgeon in anchoring the apparatus 10 to the chest wall, muscle tissues, or the like of a subject (patient).

[0122] The connection scheme for connecting the suture 20 to a needle 30 may include one of a variety of techniques. In one embodiment, bonding or glueing the suture 20 into a cavity 62 drilled, cast, or otherwise formed within one end of the needle 30 may form a suture connection 60 that is comparatively seamless. This provides no exposed edges to snag tissues or inhibit easy passage of the needle 30 during suture.

[0123] In an alternative embodiment, a suture connection 60 may be formed by having a roll end 64 or tabs 64 crimped to hold the suture 20, by a combination of friction, distortion, or the like, to the needle 30. The tabs 64 or the crimp 64 may present a change in cross-sectional area of the needle 30, thus providing a source for snags, and resistance to passage of the needle 30 through tissues.

[0124] Yet another alternative embodiment may be more classical, providing an eye-end 66 to receive the suture 20. In this embodiment, the needle 30 appears much like a conventional needle. Although having a point, shape, and material suitable for surgical use, rather than conventional fabric use, this is independently threaded at the time of use. In this embodiment, the suture 20 may be simply left with an open-end 68 to be threaded through a needle 30 of choice. Alternatively, the open-end 68 may be bonded at the time of use. Nevertheless, in certain embodiments, surgeons prefer to have a previously attached needle 30 securely bonded or otherwise fastened to a suture material 20 for immediate use.

[0125] As a matter of convenience, surgical needles 30 are often formed as a substantially semi-circular arc. The various needles have geometry suitable to their specific function. Suture needles 30 may be, for example, formed with a taper point 70, a round bodied needle used for organ tissues, intestines, and the like.

[0126] In certain embodiments, including attachments through bone and the like, a reverse cutting needle 72 or a cutting edge needle 78 provide a cutting edge on at least one corner of a typically triangulated cross-section. In an alternative embodiment thereof, a tapered needle 76 with a cutting point 77 in combination therewith may provide a hybrid device 30.

[0127] Other specialized needles, including a spatula point 74, and a straight point 80 that does not provide the typical semi-circular needle 30 are alternative embodiments. A taper cut needle 76 is typically used for anchoring to skin, mucosa, muscle, and tendon materials. Cutting needles 78 and reverse cutting needles 72 provide cutting ability, whereas a taper point mechanically tends to stretch tissues therearound. Accordingly, a cutting point 72, 78 may rely upon subsequent scarring to correct its effects, whereas a round point 70 may rely more on the resilience and displacement of tissues to accommodate the trauma and aperture formed therethrough.

[0128] Given the very sharp points and edges present with needles 30, a sheath 41 may fit around a needle 30. For example, in one embodiment, the sheath 41 may be formed as a clip 40 having detents 84 to clip the needle 30 into the sheath 41 securely. Nevertheless, the detent 84 may be formed as a simple knob 84 that can be easily deflected by a surgeon in withdrawing the needle 30 from the sheath 41. Similarly, detents 84 may be placed in more than one location in order to substantially fix a needle 30 with respect to the sheath 41 until withdrawal for use. By shaping the sheath 41 as a circle, or button, the sheath 41 may actually contain the coil 24 or excess length 24 of suture material 20. Thus, the sheath 41 may simply form a button extending from the back plate 12 of the apparatus 10 at insertion.

[0129] After proper location of the apparatus 10 with respect to the physiology of the patient, a surgeon may then unclip the suture material 20, 24 along with the needle 30

from the sheath 41 for use. The sheath 41 may be formed of a comparatively stiff yet flexible material, such as polyethylene, polyester, polypropylene, or other suitable materials. Since the material of the sheath 41 will not be left within any body cavity, the material need not be subject to the same scrutiny and physiological properties as those of the suture 20 or the apparatus 10 remaining in a patient.

[0130] Referring to FIG. 13, an alternative embodiment may be more of an oval or rounded rectangular shape having a detent 84 to receive and retain a needle therearound. An aperture or slot shaped to receive the needle may also be sized to receive the extra suture material 24. The shape may be rounded, rectangular, or the like, but sharp edges tend to snag, drag, and otherwise resist easy positioning. Accordingly, corners may be rounded, and materials selected to have flexibility. For example, the sheaths 41 may actually be formed of a material that is merely a stiff elastomeric material such as a rubber, latex, silicone, or the like. With proper thicknesses and other dimensions (e.g. length, width, diameter), the sheaths 41 may serve their purposes adequately. They may still be highly flexible and capable of substantial distortion in order to open to release the needle 30, suture material 20, or both.

[0131] Referring to FIG. 14A, a sheath 41 may be embodied as an envelope 28 formed of any suitable material. The material may be a paper, polymeric paper, plastic, comparatively rigid, stiff, flexible, elastomeric, or the like. In one embodiment, the suture material 20 is simply coiled up as extra material 20 connected to a needle 30 all inserted into the envelope 28.

[0132] The protective sleeve 28 or envelope 28 may be positioned close to the apparatus 10, even in very close proximity to the reinforcement 59. The suture 20 may be taped, glued, crimped, clamped, or otherwise secured against easy slippage with respect to the envelope 28 in order to provide ease of working while placing the apparatus 10 physiologically. Thereafter, a tug, clip, cut, tear, or the like from a surgeon using scissors, forceps, scalpel, needle, or the like may release the envelope 28 for removal. Thereupon, the needle 30 becomes accessible with the suture 20 including the entire coil 24 of extra material 24.

[0133] Referring to FIG. 14B, one alternative embodiment may include a sheath 41 formed as an envelope 28 or a coil 28 of a tubular material having a diameter 32 suitable for receiving a needle 30. The sheath 41 may extend, for example, through 360, 540, 720 or more degrees of the coil 28. Space between adjacent loops or turns of the coil 28 may close, spring-like, to hold suture materials, clip to a substrate, or the like. Meanwhile, the needle 30 may be extracted from the interference fit within the inner diameter 32 of the tubular material of the coil 28. Likewise, the coil 28 forms a diameter 34 that operates much like the button concept of FIG. 12. Thus, the sheath 41 as a coil 28 operates as a small medallion or loop that resists snagging with respect to tissues coming in contact therewith.

[0134] Referring to FIG. 15, a process 90 for implementing an apparatus and method in accordance with the invention may be given the diagnosis 92 of a condition. The condition is typically referred to as ptosis. In a ptosis condition, stretching of tissues under the influence of physiological expansion followed by subsequent internal tissue shrinkage, the effects of gravity over time, and the like may

cause displacement or discomfort. This condition is usually characterized as skin drooping and lack of fullness in underlying tissues. Accordingly, a mastopexy operation relocates selected tissues, excises certain tissues, and reconnects with sutures the remaining tissues in a new geometric configuration. An apparatus **10** may augment the lack of fullness remaining. The process is often times called a mastopexy or a lift.

[0135] At some point following diagnosis **92**, preparation **94** occurs. Medical preparations may include preparations of a patent, procedures **104**, and equipment **105**, including selection and preparation of the apparatus **10** for an operation. In addition, the patient preparation **106** may include specification or selection of procedures **107**, as well as study and practice thereof, along with anesthesia procedures **108**. In addition, other common preparation procedures may be employed. Some of those procedures include standard anti-septic and field preparation procedures, as well as informational procedures for patents, doctors, staff, and the like.

[0136] A significant part of preparation **94** will be selection of corresponding procedures **104** and equipment **105** consistent with the apparatus **10**. In any operation involving the use of the apparatus **10** in accordance with the invention, the procedures **104** appropriate thereto will be selected after study, and studied after selection. Similarly, selecting an anesthesia **108** may involve determinations of whether an operation is to be conducted under local or general anesthesia. Typically, mastopexies are conducted with general anesthesia. By contrast, some augmentation procedures require sufficiently noninvasive processes that local anesthesia may be adequate. Similarly, localized anesthesia with some degree of sedation short of unconsciousness may also be selected. Eventually, during preparation of a patient, anesthesia will be applied. Shortly after application of anesthesia **108**, incision **96** will begin.

[0137] The incision process **96** may involve certain standard and certain new procedures in accordance with the invention. Typically, the broad classes of incisions are part of opening the actual region subject to surgery, and excising tissues to be removed. Incisions will include the process of cutting free and moving certain tissues. For example, movement **109** of the entire mammary duct system in a superior direction, may not be possible. Nevertheless, the majority of ducting, along with terminations in the areola and nipple will be moved in their entirety. Nevertheless, as a natural consequence of subsequent excision **98** of certain tissues therebelow, some ducting may be excised.

[0138] As a practical matter, protection **110** of tissues will be required, including hydration, standardized surgical procedures, including clamping off vessels, and the like. Typically, irrigation, cleaning, suction, and the like may be used to maintain the area clean and clear for observation and navigation by the surgeon. Further details regarding the incision processes and locations will be described hereinafter.

[0139] Excision **98** typically involves connecting forceps **111** or a hemostat **111** to literally tag tissue and provide a handle for manipulating it. Hemostats are often used to close off vessels, but may also be used as handles to identify and manipulate tissues to be removed. Upon completion of the necessary incisions **96**, removal **112** may include an incision

separating removed tissue from the surrounding area. The details of excision locations and tissues will be described hereinafter.

[0140] Implantation **100** involves insertion **113** of an apparatus **10**. That is, mastopexy processes may be with augmentation or without augmentation. Since mastopexy involves relocation and reshaping of the physiology of a patient, augmentation may or may not be required or advisable. In the event that augmentation is deemed appropriate for purposes of enhancement or to provide or restore symmetry, an insertion **113** of an apparatus **10** places the apparatus **10** within an incision underlying the glandular structure, the muscular structure, or both of the patient. Subsequently, tissues will heal around the apparatus **10**, on the periphery of the incision.

[0141] Following incision and insertion **113** of the apparatus **10**, orientation **114** may occur in each axial, and some rotational directions. For example, the apparatus **10** should be oriented in the superior-inferior direction or along a superior-inferior axis in order to provide the effective lift effect at the proper location. Thereafter, the apparatus **10** for a second breast needs to be oriented in the superior-inferior direction with respect to the initial implant **10**. Likewise, each implant apparatus **10** needs to be oriented in a lateral-medial direction in order to provide the desired effect, and needs to be arranged in the instance of the second breast to be symmetric along both lateral-medial axes and superior-inferior axes to provide desirable symmetry.

[0142] Moreover, to improve the longevity of the effect or of the mastopexy procedure, anchoring of the apparatus **10** by way of sutures **20** may reduce the effects of gravity as an agent causing damage during healing, extension of healing, capsular scar thickening, and the like. Thus, a surgeon may use the suture **20** to anchor the apparatus **10** to the chest wall, through cartilage in the chest wall, through ribs in the chest wall, or the like. In this event, the orientation may be made with respect to a rib, in order to place both tabs **18**, or both sutures **20** in close proximity to a single rib.

[0143] Thus, the apparatus **10** may actually be rotated about an axis substantially perpendicular to the back plate **12** in order to properly orient the anchor points in accordance with the actual physical anatomy of the patient. Thus, the ease, durability, and equality of sutures is maintained. That is, if both sutures **20a**, **20b** are placed through the same edge of the same bone, or through the same region of cartilage between the same pairs of ribs, then the sutures should be expected to behave substantially equally in supporting the apparatus **10** in use. Similarly, if inferior tabs **46** or inferior sutures **30c**, **30d** are used, they may be similarly and symmetrically oriented with respect to one another.

[0144] Typically, in an apparatus and method in accordance with the invention, anterior-posterior orientation is not a problem. Typically, geometry of the back plate **12** and the orientation with respect to either tabs **18** or sutures **20** integrated with the back plate **12** will provide immediate, visible, and tactile assurance of the anterior-posterior orientation. Likewise, superior-inferior rotation can easily be detected by the same visible indicia.

[0145] By contrast to many augmentation procedures and devices, the apparatus **10** used in a mastopexy procedure is not substantially hidden from the surgeon. That is, a peri-

areolar incision may be very small, and an implant may actually be rolled up and unfilled at the time of insertion in augmentation surgeries. By contrast, in mastopexy, due to the nature of the incisions **96** and excisions **98**, the implant region is typically visible and accessible for suturing, and orientation is not inherently problematic.

[**0146**] Anchoring **115** may involve a variety of processes, apparatus **10**, tabs **18**, sutures **20**, and the like. As discussed hereinbelow, anchoring **115** after orientation **114** of an apparatus **10** assures two major advantages over prior art systems. The apparatus **10** is anchored **115** against the effects of gravity, physical motion, and the like during healing. Accordingly, the edges or periphery of incisions **96** are protected immediately against incursion, pressure, forces, and the like from the apparatus **10** in any direction against which sutures **20** have been made. Thus, gravity cannot urge the apparatus **10** to move substantially into tissues to expand scarring, or exacerbate or inflame an incision.

[**0147**] If lower tabs **46** or inferior sutures **30c**, **30d** are used, physical activity will be inhibited from causing motion in a superior direction. Meanwhile, the selected location of the tabs **18** or sutures **20** embedded in the apparatus **10** provide both lateral-medial migration resistance, and superior-inferior migration resistance due to physical activity or the natural effects of gravity. In addition to support during healing, permanent suture anchors may provide permanent support against all of the foregoing forces that might tend to displace the apparatus during a long term.

[**0148**] Following implantation **100**, suturing **102** closes up all exposed incisions. This implies suturing closes the capsule or capsular volume enclosing the apparatus **10**. Likewise, closing all skin incisions in order to reform the exterior of the breast will complete relocation of the areola region and closure of the inframammary boundary or incision, as well as the midline or medial incision therebetween.

[**0149**] Referring to FIG. 16, implantation **100** may include insertion **113**, orientation **114**, and anchoring **115**. During insertion **113**, an optional incision **116** may be transaxillary (under the arm) but is typically inframammary. The implant **10** may be placed under the muscle (submuscular, under the pectoralis major), or may simply be subglandular (outside of the main pectoral muscle group, and below or within the skin and mammary tissues).

[**0150**] In addition, the incision **116** may actually be made laparoscopically. That is, a laparoscope or a long flexible tube containing various tools, vision apparatus, lighting devices, instrument insertion tubes, and the like may be inserted in order to minimize trauma. In other processes, the entire tissue structure may be opened up by broad incisions to provide ready access to all tissues involved.

[**0151**] Placement **117** typically involves positioning the back plate **12** against the muscles or wall of the chest. Orientation **114** may include orientation to assure against accidental rotation either anterior/posterior or superior/inferior. Similarly, lateral/medial rotation may occur, but is effectively anterior/posterior rotation. Some implants are anatomically shaped, while others are merely hemispherical. In a situation with a hemispherical implant, anterior/posterior rotation produces the same effect as lateral/medial or superior/inferior rotation.

[**0152**] Orientation may include superior-inferior translation in either direction or lateral-medial translation in either direction. Circumferential rotation about an axis substantially perpendicular to the back plate **12** may be used to orient the tabs **18**, sutures **20**, or both in accordance with the body physiology in order to optimize the location, symmetry, and loading of anchoring.

[**0153**] Anterior-posterior depth **47** may be adjusted in some implants **10** by a surgeon. Other implants **10** are manufactured with a particular volumetric content. Thus, optionally, a surgeon may select the anterior-posterior depth **47** of an apparatus **10**.

[**0154**] Symmetry **119** may involve all of the orientation factors **118**. However, the orientation factors **118** apply to both implants with respect to themselves, one another, and with respect to the overall anatomy of the body of a patient.

[**0155**] Anchoring **115** may include a variety of optional processes. For example, exposing **120** a needle **30** or the point thereof may be required as a separate step if certain sheaths **41** are provided. Otherwise, a needle **30** may simply be selected for use with a suture **20** provided independently therefrom.

[**0156**] Extending **121** the suture material **24** or the suture **20** from a packet, envelope, or other sheath **41** may be required in a case of a suture **20** and needle **30** integrated with an apparatus **10**. In an alternative embodiment, the suture **20** may be provided in a separate package and may be withdrawn **121** or extended therefrom.

[**0157**] Penetrating **122** a tab or threading **122** a needle **30** is considered an optional step or optional steps **122**. That is, threading a needle **30** is often not required in an apparatus and method in accordance with the invention when the suture **20** is previously bonded to a needle **30**. This is particularly true when embedded or otherwise integrated with an apparatus **10**. Likewise, tabs **18** may or may not be provided with an apparatus **10**. Accordingly, penetrating **122** and threading **122** are optional steps that may or may not be required in a particular embodiment in accordance with the invention.

[**0158**] Penetrating **122** the anchorage involves the penetration by a suitable device, such as a needle with trailing suture **20**, of the tissues that will provide the anatomical support for the apparatus **10**. Penetrating **123** may involve passing a needle **30** through bone, cartilage, or the like in the chest wall. Similarly, penetrating **123** may involve passing the needle **30** and the trailing suture **20** through the chest muscle instead. Other anchoring locations may be provided in the anatomy according to the needs of a particular patient. Moreover, an apparatus and method in accordance with the invention may be shaped and anchored in a manner to augment any suitable area of the body. Thus, any region of the body to be aided by prosthetic augmentation can receive a suitably shaped implant appropriately anchored.

[**0159**] Ultimately, knotting **124** the suture **20** provides a degree of permanence to the suture process **102**. Excess material from the suture **20** will be clipped **125** and discarded.

[**0160**] In an alternative embodiment, the apparatus **10** may be anchored by stapling rather than suturing **102**. For example, positioning **126** a stapling device and discharging

127 a staple through a tab 18 may secure the apparatus 10 to a chest wall, rib, or other part of the anatomy. Ultimately, validating 128 the stability of a suture process 102 or another anchoring process 115 is advisable to assure that neither non-anchored apparatus 10 nor inadequately or partially anchored apparatus 10 result from the process 100.

[0161] Anchoring 115 provides a number of benefits in accordance with the invention. In the situation involving axially symmetric, hemispherical apparatus 10, a surgeon may desire to find anatomical symmetry along a line, about a point, and with respect to both implants 10 inserted 113. Precision in location relative to the patient's anatomy, as well as symmetry with respect to one another may be achieved with a degree of reliability by providing anchoring 115 as part of the process 100.

[0162] Biological tissues do not necessarily react or respond exactly as inanimate materials and machines do. The body will react and respond to the mastopexy process. Accordingly, the process 100 does not last forever. To accommodate the natural decline of resilience and fullness of tissues, a surgeon may "overlift" by positioning a device 10 higher than ultimately expected or desired. Accordingly, over time, the natural reaction of tissues to the presence of the apparatus 10 may result in a shift in the inferior direction.

[0163] However, because the apparatus 10 in accordance with the invention provides anchoring 115 as part of the implantation process 100, overlifting is not required. The anchor provides a degree of certainty as to the location of the apparatus 10. Likewise, exactly locating the apparatus 10 along any lateral-medial axis is possible. Accordingly, the process 100 provides a comparatively broad tolerance for a surgeon in completing the operation 100, and yet results in a comparatively fine tolerance in the result, the ultimate location of the apparatus 10 with respect to the patient's anatomy.

[0164] As discussed hereinabove, forces may arise from sleep, physical activities, athletic pursuits, accidents, and the like. Moreover, the weight of a patient may change over time either up or down. Accordingly, anchoring 115 provides a degree of assurance of proper location with respect to the body structures, rather than permitting a migration or shift with tissues, gravity, scarring or as a result of the reaction of tissues to the presence thereof.

[0165] The concept of dynamic rippling or wrinkling arises from a wave motion, natural in liquids, unnatural in solids. Ripples due to waves in implant filler materials may be visible through the skin. Rippling may be reduced to a certain extent by the presence of anchoring. That is, anchoring an apparatus 10 provides a node that is not subject to substantial displacement. Thus, a wave node necessarily affects and limits the propagation of dynamic waves, particularly in inviscid fluids used as fillers in the apparatus 10. Thus, the characteristic dynamic ripple may be reduced or even eliminated in some case by suitable anchoring 115.

[0166] Thus, one can see that a degree of simplicity, reliability, reduction of side effects, scarring control, and reduced scar stretching are provided by virtue of both the temporary and permanent support of the anchoring process 115 controlling the physiological location of the apparatus 10. Accordingly, rather than the considerable scarring, stiffness, and capsular contracture experienced in prior art

devices, reduced scarring and inflammation can be expected, as well as stabilization against migration.

[0167] Referring to FIG. 17, a process 130 for manufacturing an apparatus 10 in accordance with the invention may include providing 131 a mold shaped to produce one or more portions of the apparatus 10. For example, in one embodiment, a roto-molded apparatus 10 may be formed in a closed mold fitted and smoothed to provide substantially no seam lines, flash, or the like. Roto-molding and injection molding are well understood in the plastics manufacturing industry. In other embodiments, the apparatus 10 may be fabricated by vacuum forming, blow molding, or the like using suitable elastomeric or polymeric materials. For example, dimethylsiloxane (e.g. SILASTIC™ Dupont) has been found to be a moderately low-temperature vulcanizing material suitable for molding.

[0168] Providing 132 reinforcement 48 by way of fibers, whether random, oriented, angled, or the like, may enhance the structural integrity and the weight-bearing capacity of an apparatus 10. Similarly, providing 133 sutures 30 may be optional in the manufacturing process. Sutures 30 may be embedded in the back plate 12 or otherwise in the apparatus 10. Sutures 30 may be provided by a surgeon after manufacturing, such as during the actual surgical operation 100.

[0169] Positioning 134 embedded materials (e.g. the mesh 50, reinforcing fibers 48, or the like) is also shown in brackets indicating that this step is optional in the process 130. Positioning 134 the embedded materials may not be required if the material of the apparatus 10 is to be completely formed of a single material. By contrast, the back plate 12 may still be homogeneously formed of a composition or matrix 56 embedded throughout a mesh 50. Thus, the result is a substantially homogeneous plate, reinforced by a fiber not homogeneous therewith but uniformly or nonuniformly distributed as appropriate.

[0170] Molding 135 a matrix 56 may occur with or without embedded materials 50. Ultimately, however, curing 136 by virtue of temperature change, chemical reaction, or the like may require a period of time, and various chemical or thermal processes. The curing 136 will typically require, or be required in accordance with, a particular chemistry of the base material forming the apparatus 10.

[0171] Securing 137 a needle is illustrated as an optional step since a needle 137 may or may not be a part of the apparatus 10. Nevertheless, if a suture 20 is embedded in the material 56 of the apparatus 10, then a needle 30 may be secured 137 to the suture 20 as a practical convenience.

[0172] Similarly, applying 138 point protection to the needle 30 is an optional step. Such application 138 depends upon whether or not a needle 30 is present in the apparatus 10 as manufactured. A surgeon may care very much whether or not the needle is protected by application 138 of a sleeve 41 of some type suitable. Needles may be very sharp and can cut tissues or implants with little more than brushing past them.

[0173] Filling 139 is a process that will typically occur in any filled apparatus 10. In some embodiments, the fill process 139 may be optional, since the basic material may be a solidus material such as a gel or a foamed solid apparatus 10. However, in an apparatus and method in accordance with the invention, filled apparatus 10 are con-

templated in many applications, since they may provide proper weight, sizing adjustability, texture, and other appearance features. The fill **139** or filling **139** of an apparatus **10** in accordance with the invention may involve adding a filler **45** at the time of manufacture, or adding the filler **45** at the time of insertion. Even when the filler **45** is molded or injected into an apparatus **10** during the manufacturing process **130**, a surgeon may alter the fill process **139** at the time of the operation **100**. Accordingly, the fill process **139** may depend upon whether or not the apparatus **10** does contain a filler **45**, and may occur at a time selected by the manufacturer, surgeon, or both.

[0174] Ultimately, the apparatus **10** must be sealed **140** against incursion of tissues, or sources of bacteria or infection. Accordingly, the apparatus will typically be sealed against leakage of the filler **45**. Atoms and molecules operating within the interatomic or intermolecular distances provided in polymers may actually migrate with respect to one another. Polymers typically constitute long chains that appear like microscopic spaghetti. Accordingly, the effective mesh size or intermolecular distance may actually permit passage over time by shorter chained polymers and single atoms. Accordingly, “weeping” or “microbleeding” of filler materials **45** through the walls of the pocket **14** or back plate **12** of the apparatus **10** are a distinct possibility and probability. Thus, the seal **140** is against the macroscopic passage of materials. Nevertheless, the microscopic passage of materials may actually continue at a comparatively very low flow rate.

[0175] Referring to FIG. 18, a mastopexy incision is made in something of an “anchor shape.” Typically, a breast **141** is incised in a shape or along a series of paths (e.g. curves) that isolate the areola **142** and nipple **144** region for removal with the mammary ducting system. An incision along the inframammary border (e.g. fold, boundary, etc.) connects to incisions along a boundary **147** that will eventually be sutured to the inframammary boundary **146**. Intervening tissues of skin and underlying tissues will be excised.

[0176] Similarly, an incision **148** is formed that will eventually be sutured to form a midline **149**, and appears like the shaft of an anchor, while the incisions **146**, **147** appear like the flukes of an anchor. Meanwhile, a substantially circular or arcuate region **150** to be excised is defined by an arcuate incision **152** therearound and connecting the incisions **148**. Accordingly, the areola tissue **142** will be relocated to the region **150**, and sutured in along the incision line **152** or incision arch **152**.

[0177] Referring to FIG. 19, while continuing to refer generally to FIGS. 1-18, the incision **148** is closed to form a midline suture **149** or midline **149**, while the incisions **147**, **146** are sutured together to form the inframammary boundary **146**. A variety of stitches may be used for the various sutures **154** used to close the midline **149** and inframammary boundary **146**. FIG. 19 illustrates the comparative positioning in one embodiment of an apparatus **10** in accordance with the invention.

[0178] Nevertheless, the tabs **18** may be replaced, or augmented by the presence of the sutures **20** in an apparatus **10** in accordance with the invention. The anchoring of the apparatus **10** resists the temporary and permanent effects of flushes **160** or accelerations **160** due to gravity acting on the apparatus **10** to place forces and pressures on surrounding tissues. Accordingly, the sutures **146**, **149** need only sustain the natural mass and weight of enclosed tissues, and not the pressures and forces due to the presence of the apparatus **10**.

[0179] Referring to FIG. 20, while continuing to refer generally to FIGS. 1-19, the excised tissue **158** represents both skin and underlying supporting tissue. After removal thereof, a new balance is struck between the mass and volume of contained tissues, and the supporting strength of surrounding skin tissue. Forces may exist along both a superior-inferior axis **160** as well as along a lateral-medial axis **166**. Meanwhile, the compressive forces **166** of underlying tissues may be resisted by the tensile forces **168** of the sutures **154**.

[0180] By the same token, solidus tissues do not flow, but distort quite flexibly. They sometimes behave something like liquids in providing a substantially omnidirectional pressure **170** in response to distortion or pressure. Accordingly, the sutures **154** must resist the pressure **170** imposed by the response of tissues to gravitational forces acting on overlying tissues supported thereby. In prior art systems of implants, the implants themselves add gravitational forces along the axis **160** resulting in pressure **170**. The anchoring **115** of the apparatus **10** in accordance with the invention alleviates these loads and reduces internal and external scarring and scar widths along the midline **149** and along the inframammary boundary **146**.

[0181] Referring to FIGS. 21A-21D, while referring generally to FIGS. 1-20, an apparatus **10** in accordance with the invention may be sutured in one embodiment directly to a muscle **180**. The muscle **180** overlies the chest wall **172** comprising both ribs **174** and intervening cartilage **176**. The chest wall **172** is protected by a fascia **178** overlying it. In a subglandular positioning of an apparatus **10** in accordance with the invention, the apparatus **10** underlies the mammary gland network and surrounding tissues. However, the apparatus **10** lies outside the muscle **180**, and is secured by sutures **154** anchoring the apparatus **10** to the muscle **180**.

[0182] Referring to FIGS. 22A-22D, while continuing to refer generally to FIGS. 1-21, an apparatus **10** in accordance with the invention may be connected to the wall **172** or chest wall **172** of a patient. Connections to the chest wall **172** may include suture to a rib **174**, or cartilage **176** located between ribs. In general, a needle **30** and suture **20** will be passed by a surgeon through the fascia **178** protecting the chest wall **172**, penetrate the cartilage **176**, or the cartilage **176** and a portion of rib **174**, and return out through the fascia **178**. Typically, the suture **154** will be made as a series of loops, when anchoring **115**. In certain embodiments, the suture **154** may actually progress along a particular path, such as a periphery of the implant **10**, and thus involve several stitches distributed along a suture path. In implants applied to other areas of the body, sutures may be similarly located.

[0183] In an application as illustrated in FIGS. 22A-22D, the location of the apparatus **10** is sub-muscular. Accordingly, the chest muscle **180** is separated from the fascia **178**, in order to position the implant and/or apparatus **10** between the fascia **178** and the muscle **180**. Accordingly, the sutures **154** penetrate into the chest wall **172**, connecting to either a rib **174**, intervening cartilage **176**, or both. Accordingly, the suture **154** will typically pass through the fascia **178** and return outside the chest cavity for knotting **124** by the surgeon.

[0184] Referring to FIGS. 23-25, the forces **160** associated with gravitational acceleration of all masses, are not resisted by skeletal structure. Accordingly, the soft tissues associated with a mastopexy operation may be subject to distortion, displacement, stretching, and the like in response to the forces **160** of gravity, and resulting omnidirectional

pressures from tissues. Accordingly, the anchoring **115** of the apparatus **10** to the body in a subglandular or submuscular application can resist the displacement in response to the forces **160**.

[0185] Referring to **FIG. 24**, strenuous activities, sports, movement while sleeping, forces, pressure, and the like that naturally occur with the body, may affect the apparatus **10** differently from surrounding tissues. Accordingly, tissues may rupture, inflame, stretch, or otherwise permit migration of the apparatus **10** absent suitable anchoring **115**. Accordingly, to provide stability against rotation around substantially any axis, as well as resistance to lateral displacement **184** (laterally toward outside the rib cage and under the arm) may be resisted by the apparatus **10** in accordance with the invention. Similarly, medial displacement **186** toward the sternum and away from the underarm area may be avoided.

[0186] Either displacement **184**, **186** by an implant **10** or apparatus **10** in accordance with the invention may produce asymmetry and distortion undesirable in a patient. The forces **184**, **186** may result from athletic activity, contact with objects or persons, or other influences that may produce a force that tissues will respond to locally. A foreign object such as the apparatus **10** may respond more monolithically to forces **184**, **186**. Accordingly, distortions in response to forces **184**, **186** are resisted in an apparatus **10** in accordance with the invention.

[0187] Referring to **FIG. 25**, forces **190**, **192** in the superior and inferior directions, respectively, may operate similarly to those of **FIG. 24**. In the absence of anchoring **115**, forces occurring during athletic activity or contact with objects or persons, as well as natural reactions of tissues, and the like may result in either superior or inferior displacement in the absence of anchoring **115**.

[0188] Referring to **FIG. 26**, a ptosis condition **198** is illustrated in **FIG. 26A**, along with the demarcation lines that will be the subject of the incisions described with respect to **FIGS. 19-22**. Referring to **FIG. 26B**, the process **90** in accordance with the invention is illustrated showing the incisions along which openings will be formed, and the pocket formed, as well as the incisions that will be closed after excision of excess tissues.

[0189] Referring to **FIG. 27**, the ptosis condition **196** is shown transformed **200** by the process **100** to a lifted condition **198** as illustrated. Thus, it can be seen that an apparatus and method in accordance with the invention provide for an improved apparatus **10** to be used in an improved process **100** for correcting a ptosis condition **196**.

[0190] From the above discussion, it will be appreciated that the present invention may be embodied in other specific forms without departing from its essential characteristics. The described embodiments are to be considered in all respects only as illustrative, and not restrictive. The scope of the invention is, therefore, indicated by the appended claims, rather than by the foregoing description. All changes within the meaning and range of equivalency of the claims are to be embraced within their scope.

What is claimed and desired to be secured by United States Letters Patent is:

1. An apparatus for mastopexy with augmentation, the apparatus comprising:

a vessel of predetermined form and size, the vessel including at least one wall for contact with tissue of a user;

a filler to maintain a volume of the vessel; and

a plurality of tabs homogeneously formed with, and continuously extending from, the at least one wall of the vessel.

2. The apparatus of claim 1, wherein the at least one wall comprises a polymer

3. The apparatus of claim 2, wherein the polymer is an elastomer.

4. The apparatus of claim 3, wherein the elastomer is a silicone compound.

5. The apparatus of claim 4, wherein the silicone compound is dimethylsiloxane.

6. The apparatus of claim 4, wherein the filler comprises a material selected from the group consisting of water, saline, silicone, silicone gel, sugar, and hydrogel.

7. The apparatus of claim 4, wherein the back wall comprises at least one embedded reinforcing fiber.

8. The apparatus of claim 7, wherein the at least one embedded reinforcing fiber is arranged in a mesh pattern.

9. The apparatus of claim 8, wherein each tab of the plurality of tabs comprises an aperture extending there-through.

10. The apparatus of claim 9, further comprising at least one suture formed of non-elastomeric material embedded within the at least one wall and terminating at a first end extending outwardly from the at least one wall.

11. The apparatus of claim 10, wherein a first tab of the plurality of tabs extends substantially radially from the at least one wall at about the ten o'clock position.

12. The apparatus of claim 10, wherein a second tab of the plurality of tabs extends substantially radially from the at least one wall at about the two o'clock position.

13. The apparatus of claim 12, wherein the at least one wall comprises a back wall providing a surface for contact with tissue posterior to the vessel.

14. The apparatus of claim 13, further comprising at least one surgical needle connected to draw the first end of at least one suture.

15. The apparatus of claim 14, further comprising at least one protective covering surrounding the at least one surgical needle to resist inadvertent puncture of the vessel.

16. The apparatus of claim 1, wherein the back wall comprises a plurality of embedded reinforcing fibers arranged in a mesh pattern.

17. The apparatus of claim 1, wherein each tab of the plurality of tabs comprises an aperture extending there-through.

18. The apparatus of claim 1, further comprising at least one suture formed of non-elastomeric material embedded within the at least one wall and terminating at a first end extending outwardly from the at least one wall.

19. The apparatus of claim 1, wherein a first tab of the plurality of tabs extends from the at least one wall at about the ten o'clock position and a second tab of the plurality of tabs extends from the at least one wall at about the two o'clock position.

20. The apparatus of claim 19, wherein the at least one wall comprises a back wall providing a surface for contact with tissue posterior to the vessel.