

(43) International Publication Date
4 September 2014 (04.09.2014)(51) International Patent Classification:
A61B 17/29 (2006.01)(21) International Application Number:
PCT/US2014/016200(22) International Filing Date:
13 February 2014 (13.02.2014)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
13/780,067 28 February 2013 (28.02.2013) US(71) Applicant: ETHICON ENDO-SURGERY, INC.
[US/US]; 4545 Creek Road, Cincinnati, Ohio 45242 (US).(72) Inventors: FANELLI, Nicholas; 5037 Roachester Osceola
Road, Morrow, Ohio 45152 (US). GAGEL, Jeffrey C.;
6205 Pintail Court, Loveland, Ohio 45140 (US).(74) Agents: JOHNSON, Philip S. et al.; Johnson & Johnson,
One Johnson & Johnson Plaza, New Brunswick, New Jer-
sey 08933 (US).(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a
patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the
earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))

(54) Title: SURGICAL INSTRUMENT END EFFECTOR ARTICULATION DRIVE WITH PINION AND OPPOSING RACKS

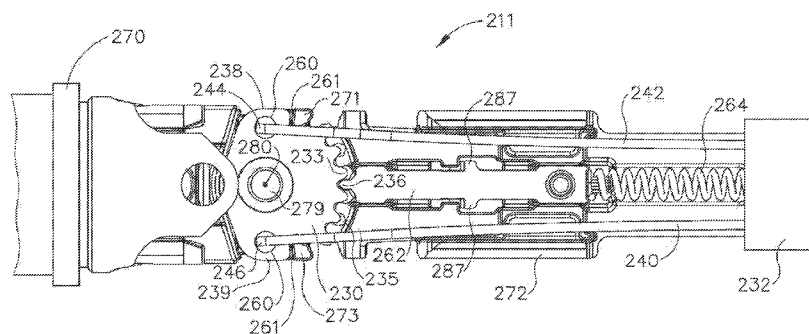


Fig.18A

(57) Abstract: An apparatus comprises a body and a shaft assembly. The shaft assembly is in communication with the body and comprises an end effector, first cam gear, second cam gear, and a lock bar. The end effector has an articulation joint. The first cam gear is rotatably positioned within the shaft assembly. The second cam gear is in communication with the end effector at the articulation joint. The lock bar is distally biased to lock against the second cam gear. The first cam gear is rotatable through a first range of motion to unlock the lock bar relative to the second cam gear. The first cam gear is rotatable through a second range of motion to rotate the end effector at the articulation joint.

SURGICAL INSTRUMENT END EFFECTOR ARTICULATION DRIVE WITH PINION AND OPPOSING RACKS

BACKGROUND

[0001] In some settings, endoscopic surgical instruments may be preferred over traditional open surgical devices since a smaller incision may reduce the post-operative recovery time and complications. Consequently, some endoscopic surgical instruments may be suitable for placement of a distal end effector at a desired surgical site through the cannula of a trocar. These distal end effectors may engage tissue in a number of ways to achieve a diagnostic or therapeutic effect (e.g., endocutter, grasper, cutter, stapler, clip applier, access device, drug/gene therapy delivery device, and energy delivery device using ultrasound, RF, laser, etc.). Endoscopic surgical instruments may include a shaft between the end effector and a handle portion, which is manipulated by the clinician. Such a shaft may enable insertion to a desired depth and rotation about the longitudinal axis of the shaft, thereby facilitating positioning of the end effector within the patient. Positioning of an end effector may be further facilitated through inclusion of one or more articulation joints or features, enabling the end effector to be selectively articulated or otherwise deflected relative to the longitudinal axis of the shaft.

[0002] Examples of endoscopic surgical instruments include surgical staplers. Some such staplers are operable to clamp down on layers of tissue, cut through the clamped layers of tissue, and drive staples through the layers of tissue to substantially seal the severed layers of tissue together near the severed ends of the tissue layers. Merely exemplary surgical staplers are disclosed in U.S. Pat. No. 4,805,823, entitled "Pocket Configuration for Internal Organ Staplers," issued February 21, 1989; U.S. Pat. No. 5,415,334, entitled "Surgical Stapler and Staple Cartridge," issued May 16, 1995; U.S.

Pat. No. 5,465,895, entitled "Surgical Stapler Instrument," issued November 14, 1995; U.S. Pat. No. 5,597,107, entitled "Surgical Stapler Instrument," issued January 28, 1997; U.S. Pat. No. 5,632,432, entitled "Surgical Instrument," issued May 27, 1997; U.S. Pat. No. 5,673,840, entitled "Surgical Instrument," issued October 7, 1997; U.S. Pat. No. 5,704,534, entitled "Articulation Assembly for Surgical Instruments," issued January 6, 1998; U.S. Pat. No. 5,814,055, entitled "Surgical Clamping Mechanism," issued September 29, 1998; U.S. Pat. No. 6,978,921, entitled "Surgical Stapling Instrument Incorporating an E-Beam Firing Mechanism," issued December 27, 2005; U.S. Pat. No. 7,000,818, entitled "Surgical Stapling Instrument Having Separate Distinct Closing and Firing Systems," issued February 21, 2006; U.S. Pat. No. 7,143,923, entitled "Surgical Stapling Instrument Having a Firing Lockout for an Unclosed Anvil," issued December 5, 2006; U.S. Pat. No. 7,303,108, entitled "Surgical Stapling Instrument Incorporating a Multi-Stroke Firing Mechanism with a Flexible Rack," issued December 4, 2007; U.S. Pat. No. 7,367,485, entitled "Surgical Stapling Instrument Incorporating a Multistroke Firing Mechanism Having a Rotary Transmission," issued May 6, 2008; U.S. Pat. No. 7,380,695, entitled "Surgical Stapling Instrument Having a Single Lockout Mechanism for Prevention of Firing," issued June 3, 2008; U.S. Pat. No. 7,380,696, entitled "Articulating Surgical Stapling Instrument Incorporating a Two-Piece E-Beam Firing Mechanism," issued June 3, 2008; U.S. Pat. No. 7,404,508, entitled "Surgical Stapling and Cutting Device," issued July 29, 2008; U.S. Pat. No. 7,434,715, entitled "Surgical Stapling Instrument Having Multistroke Firing with Opening Lockout," issued October 14, 2008; U.S. Pat. No. 7,721,930, entitled "Disposable Cartridge with Adhesive for Use with a Stapling Device," issued May 25, 2010; U.S. Pub. No. 2010/0264193, entitled "Surgical Stapling Instrument with An Articulatable End Effector," published October 21, 2010; and U.S. Pub. No. 2012/0239012, entitled "Motor-Driven Surgical Cutting Instrument with Electric Actuator Directional Control Assembly," published September 20, 2012. The disclosure of each of the above-cited U.S. Patents and U.S. Patent Publications is incorporated by reference herein.

[0003] While the surgical staplers referred to above are described as being used in endoscopic procedures, it should be understood that such surgical staplers may also be used in open procedures and/or other non-endoscopic procedures. By way of example only, a surgical stapler may be inserted through a thoracotomy and thereby between a patient's ribs to reach one or more organs in a thoracic surgical procedure that does not use a trocar as a conduit for the stapler. Such procedures may include the use of the stapler to sever and close a vessel leading to a lung. For instance, the vessels leading to an organ may be severed and closed by a stapler before removal of the organ from the thoracic cavity. Of course, surgical staplers may be used in various other settings and procedures.

[0004] While various kinds of surgical stapling instruments and associated components have been made and used, it is believed that no one prior to the inventor(s) has made or used the invention described in the appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention, and, together with the general description of the invention given above, and the detailed description of the embodiments given below, serve to explain the principles of the present invention.

[0006] FIG. 1 depicts a perspective view of an exemplary articulating surgical stapling instrument;

[0007] FIG. 2 depicts a side elevational view of the instrument of FIG. 1;

[0008] FIG. 3 depicts a perspective view of an opened end effector of the instrument of FIG. 1;

[0009] FIG. 4A depicts a side cross-sectional view of the end effector of FIG. 3, taken along line 4-4 of FIG. 3, with the firing beam in a proximal position;

- [00010] FIG. 4B depicts a side cross-sectional view of the end effector of FIG. 3, taken along line 4-4 of FIG. 3, with the firing beam in a distal position;
- [00011] FIG. 5 depicts an end cross-sectional view of the end effector of FIG. 3, taken along line 5-5 of FIG. 3;
- [00012] FIG. 6 depicts an exploded perspective view of the end effector of FIG. 3;
- [00013] FIG. 7 depicts a perspective view of the end effector of FIG. 3, positioned at tissue and having been actuated once in the tissue;
- [00014] FIG. 8 depicts a schematic view of an exemplary control circuit for use in the instrument of FIG. 1;
- [00015] FIG. 9 depicts a perspective view of the handle assembly of the instrument of FIG. 1, with a housing half removed;
- [00016] FIG. 10 depicts a perspective view of drive assembly components from the handle assembly of FIG. 9;
- [00017] FIG. 11 depicts a perspective view of an elongate member from the drive assembly of FIG. 10;
- [00018] FIG. 12 depicts a top, perspective view of an exemplary alternative shaft assembly that may be incorporated into the instrument of FIG. 1;
- [00019] FIG. 13A depicts a top, plan view of the shaft assembly of FIG. 12 with the end effector in a first position;
- [00020] FIG. 13B depicts a top, plan view of the shaft assembly of FIG. 12 with the end effector in a second articulated position;
- [00021] FIG. 14 depicts a perspective view of the proximal end of the shaft assembly of FIG. 12 showing the articulation knob and internal kinematic components;

- [00022] FIG. 15 depicts a top cross sectional view of the proximal end of the shaft assembly of FIG. 12 taken along the line 15-15 of FIG. 14;
- [00023] FIG. 16 depicts a top, plan view of the shaft assembly of FIG. 12 in a neutral position;
- [00024] FIG. 17 depicts a perspective, exploded view of the end effector and the articulation joint of the shaft assembly of FIG. 12;
- [00025] FIG. 18A depicts a top, partially internal view of the articulation joint of the shaft assembly of FIG. 12 in a first position;
- [00026] FIG. 18B depicts a top, partially internal view of the articulation joint of the shaft assembly of FIG. 12 with the first and second arms rotating a first cam gear;
- [00027] FIG. 18C depicts a top, partially internal view of the articulation joint of the shaft assembly of FIG. 12 with the first and second arms rotating a second cam gear and the first cam gear further;
- [00028] FIG. 18D depicts a top, partially internal view of the articulation joint of the shaft assembly of FIG. 12 with a lock bar resiliently positioning a lock tooth between teeth of the first cam gear and the second cam gear;
- [00029] FIG. 18E depicts a top, partially internal view of the articulation joint of the shaft assembly of FIG. 12 with the first and second arms rotating the first cam gear yet even further; and
- [00030] FIG. 19 depicts a plan, enlarged view of the interface of the cam gears and the lock bar of the shaft assembly of FIG. 12.
- [00031] The drawings are not intended to be limiting in any way, and it is contemplated that various embodiments of the invention may be carried out in a variety of other ways, including those not necessarily depicted in the drawings. The accompanying drawings incorporated in and forming a part of the specification illustrate several aspects of the

present invention, and together with the description serve to explain the principles of the invention; it being understood, however, that this invention is not limited to the precise arrangements shown.

DETAILED DESCRIPTION

[00032] The following description of certain examples of the invention should not be used to limit the scope of the present invention. Other examples, features, aspects, embodiments, and advantages of the invention will become apparent to those skilled in the art from the following description, which is by way of illustration, one of the best modes contemplated for carrying out the invention. As will be realized, the invention is capable of other different and obvious aspects, all without departing from the invention. Accordingly, the drawings and descriptions should be regarded as illustrative in nature and not restrictive.

[00033] I. Exemplary Surgical Stapler

[00034] FIGS. 1-7 depict an exemplary surgical stapling and severing instrument (10) that is sized for insertion, in a nonarticulated state as depicted in FIG. 1, through a trocar cannula to a surgical site in a patient for performing a surgical procedure. By way of example only, such a trocar may be inserted in a patient's abdomen, between two of the patient's ribs, or elsewhere. In some settings, instrument (10) is used without a trocar. For instance, instrument (10) may be inserted directly through a thoracotomy or other type of incision. Instrument (10) of the present example includes a handle portion (20) connected to a shaft (22). Shaft (22) distally terminates in an articulation joint (11), which is further coupled with an end effector (12). It should be understood that terms such as "proximal" and "distal" are used herein with reference to a clinician gripping handle portion (20) of instrument (10). Thus, end effector (12) is distal with respect to the more proximal handle portion (20). It will be further appreciated that for convenience and clarity, spatial terms such as "vertical" and "horizontal" are used herein

with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

[00035] In some versions, shaft (22) is constructed in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7181USNP.0599180], entitled "Surgical Instrument with Multi-Diameter Shaft," filed on even date herewith, the disclosure of which is incorporated by reference herein. Other suitable configurations for shaft (22) will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00036] Once articulation joint (11) and end effector (12) are inserted through the cannula passageway of a trocar, articulation joint (11) may be remotely articulated, as depicted in phantom in FIG. 1, by an articulation control (13), such that end effector (12) may be deflected from the longitudinal axis (LA) of shaft (22) at a desired angle (α). End effector (12) may thereby reach behind an organ or approach tissue from a desired angle or for other reasons. In some versions, articulation joint (11) enables deflection of end effector (12) along a single plane. In some other versions, articulation joint (11) enables deflection of end effector along more than one plane. Articulation joint (11) and articulation control (13) may be configured in accordance with the teachings of any of the numerous references that are cited herein. Alternatively, articulation joint (11) and/or articulation control (13) may have any other suitable configuration. By way of example only, articulation control (13) may instead be configured as a knob that rotates about an axis that is perpendicular to the longitudinal axis (LA) of shaft (22).

[00037] Various exemplary alternative components, configurations, and operabilities of articulation joint (11) and articulation control (13) are described in greater detail below. Articulation joint (11) may also be constructed and operable in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7181USNP.0599180], the disclosure of which is incorporated by reference herein. Other suitable forms that articulation joint (11) and articulation control (13) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00038] End effector (12) of the present example includes a lower jaw (16) and a pivotable anvil (18). In some versions, lower jaw (16) is constructed in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7182USNP.0599227], entitled "Installation Features for Surgical Instrument End Effector Cartridge," filed on even date herewith, the disclosure of which is incorporated by reference herein. Anvil (18) may be constructed in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7176USNP.0599177], entitled "Integrated Tissue Positioning and Jaw Alignment Features for Surgical Stapler," filed on even date herewith, the disclosure of which is incorporated by reference herein; at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7177USNP.0599225], entitled "Jaw Closure Feature for End Effector of Surgical Instrument," filed on even date herewith, the disclosure of which is incorporated by reference herein; and/or at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7180USNP.0599175], entitled "Staple Forming Features for Surgical Stapling Instrument," filed on even date herewith, the disclosure of which is incorporated by reference herein. Other suitable forms that lower jaw (16) and anvil (18) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00039] Handle portion (20) includes a pistol grip (24) and a closure trigger (26). Closure trigger (26) is pivotable toward pistol grip (24) to cause clamping, or closing, of the anvil (18) toward lower jaw (16) of end effector (12). Such closing of anvil (18) is provided through a closure tube (32) and a closure ring (33), which both longitudinally translate relative to handle portion (20) in response to pivoting of closure trigger (26) relative to pistol grip (24). Closure tube (32) extends along the length of shaft (22); and closure ring (33) is positioned distal to articulation joint (11). Articulation joint (11) is operable to communicate/transmit longitudinal movement from closure tube (32) to closure ring (33).

[00040] Handle portion (20) also includes a firing trigger (28). An elongate member (136) (shown in FIG. 11) longitudinally extends through shaft (22) and communicates a longitudinal firing motion from handle portion (20) to a firing beam (14) in response to

actuation of firing trigger (28). This distal translation of firing beam (14) causes the stapling and severing of clamped tissue in end effector (12), as will be described in greater detail below. Thereafter, triggers (26, 28) may be released to release the tissue from end effector (12).

[00041] FIGS. 3-6 depict end effector (12) employing an E-beam form of firing beam (14) to perform a number of functions. It should be understood that an E-beam form is just a merely illustrative example. Firing beam (14) may take any other suitable form, including but not limited to non-E-beam forms. As best seen in FIGS. 4A-4B, firing beam (14) includes a transversely oriented upper pin (38), a firing beam cap (44), a transversely oriented middle pin (46), and a distally presented cutting edge (48). Upper pin (38) is positioned and translatable within a longitudinal anvil slot (42) of anvil (18). Firing beam cap (44) slidably engages a lower surface of lower jaw (16) by having firing beam (14) extend through lower jaw slot (45) (shown in FIG. 4B) that is formed through lower jaw (16). Middle pin (46) slidably engages a top surface of lower jaw (16), cooperating with firing beam cap (44). Thereby, firing beam (14) affirmatively spaces end effector (12) during firing.

[00042] Some non-E-beam forms of firing beam (14) may lack upper pin (38), middle pin (46) and/or firing beam cap (44). Some such versions of instrument (10) may simply rely on closure ring (33) or some other feature to pivot anvil (18) to a closed position and hold anvil (18) in the closed position while firing beam (14) advances to the distal position. By way of example only, firing beam (14) and/or associated lockout features may be constructed and operable in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7175USNP.0599231], entitled "Lockout Feature for Movable Cutting Member of Surgical Instrument," filed on even date herewith, the disclosure of which is incorporated by reference herein. Other suitable forms that firing beam (14) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00043] FIG. 3 shows firing beam (14) of the present example proximally positioned and anvil (18) pivoted to an open position, allowing an unspent staple cartridge (37) to be removably installed into a channel of lower jaw (16). As best seen in FIGS. 5-6, staple cartridge (37) of this example includes a cartridge body (70), which presents an upper deck (72) and is coupled with a lower cartridge tray (74). As best seen in FIG. 3, a vertical slot (49) is formed through part of staple cartridge (37). As also best seen in FIG. 3, three rows of staple apertures (51) are formed through upper deck (72) on one side of vertical slot (49), with another set of three rows of staple apertures (51) being formed through upper deck (72) on the other side of vertical slot (49). Of course, any other suitable number of staple rows (e.g., two rows, four rows, any other number) may be provided. Referring back to FIGS. 4A-6, a wedge sled (41) and a plurality of staple drivers (43) are captured between cartridge body (70) and tray (74), with wedge sled (41) being located proximal to staple drivers (43). Wedge sled (41) is movable longitudinally within staple cartridge (37); while staple drivers (43) are movable vertically within staple cartridge (37). Staples (47) are also positioned within cartridge body (70), above corresponding staple drivers (43). In particular, each staple (47) is driven vertically within cartridge body (70) by a staple driver (43) to drive staple (47) out through an associated staple aperture (51). As best seen in FIGS. 4A-4B and 6, wedge sled (41) presents inclined cam surfaces that urge staple drivers (43) upwardly as wedge sled (41) is driven distally through staple cartridge (37).

[00044] In some versions, staple cartridge (37) is constructed and operable in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7176USNP.0599177], the disclosure of which is incorporated by reference herein. In addition or in the alternative, staple cartridge (37) may be constructed and operable in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7182USNP.0599227], the disclosure of which is incorporated by reference herein. Other suitable forms that staple cartridge (37) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00045] With end effector (12) closed as depicted in FIGS. 4A-4B by distally advancing closure tube (32) and closure ring (33), firing beam (14) is then advanced in engagement with anvil (18) by having upper pin (38) enter longitudinal anvil slot (42). A pusher block (80) (shown in FIG. 5) is located at the distal end of firing beam (14), and is configured to engage wedge sled (41) such that wedge sled (41) is pushed distally by pusher block (80) as firing beam (14) is advanced distally through staple cartridge (37) when firing trigger (28) is actuated. During such firing, cutting edge (48) of firing beam (14) enters vertical slot (49) of staple cartridge (37), severing tissue clamped between staple cartridge (37) and anvil (18). As shown in FIGS. 4A-4B, middle pin (46) and pusher block (80) together actuate staple cartridge (37) by entering into vertical slot (49) within staple cartridge (37), driving wedge sled (41) into upward camming contact with staple drivers (43) that in turn drive staples (47) out through staple apertures (51) and into forming contact with staple forming pockets (53) (shown in FIG. 3) on the inner surface of anvil (18). FIG. 4B depicts firing beam (14) fully distally translated after completing severing and stapling of tissue. It should be understood that staple forming pockets (53) are intentionally omitted from the view in FIGS. 4A-4B; but staple forming pockets (53) are shown in FIG. 3. It should also be understood that anvil (18) is intentionally omitted from the view in FIG. 5.

[00046] FIG. 7 shows end effector (12) having been actuated through a single stroke through tissue (90). As shown, cutting edge (48) (obscured in FIG. 7) has cut through tissue (90), while staple drivers (43) have driven three alternating rows of staples (47) through the tissue (90) on each side of the cut line produced by cutting edge (48). Staples (47) are all oriented substantially parallel to the cut line in this example, though it should be understood that staples (47) may be positioned at any suitable orientations. In the present example, end effector (12) is withdrawn from the trocar after the first stroke is complete, spent staple cartridge (37) is replaced with a new staple cartridge, and end effector (12) is then again inserted through the trocar to reach the stapling site for further cutting and stapling. This process may be repeated until the desired amount of cuts and staples (47) have been provided. Anvil (18) may need to be closed to facilitate insertion

and withdrawal through the trocar; and anvil (18) may need to be opened to facilitate replacement of staple cartridge (37).

[00047] It should be understood that cutting edge (48) may sever tissue substantially contemporaneously with staples (47) being driven through tissue during each actuation stroke. In the present example, cutting edge (48) just slightly lags behind driving of staples (47), such that a staple (47) is driven through the tissue just before cutting edge (48) passes through the same region of tissue, though it should be understood that this order may be reversed or that cutting edge (48) may be directly synchronized with adjacent staples. While FIG. 7 shows end effector (12) being actuated in two layers (92, 94) of tissue (90), it should be understood that end effector (12) may be actuated through a single layer of tissue (90) or more than two layers (92, 94) of tissue. It should also be understood that the formation and positioning of staples (47) adjacent to the cut line produced by cutting edge (48) may substantially seal the tissue at the cut line, thereby reducing or preventing bleeding and/or leaking of other bodily fluids at the cut line. Furthermore, while FIG. 7 shows end effector (12) being actuated in two substantially flat, apposed planar layers (92, 94) of tissue, it should be understood that end effector (12) may also be actuated across a tubular structure such as a blood vessel, a section of the gastrointestinal tract, etc. FIG. 7 should therefore not be viewed as demonstrating any limitation on the contemplated uses for end effector (12). Various suitable settings and procedures in which instrument (10) may be used will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00048] It should be understood that instrument (10) may be configured and operable in accordance with any of the teachings of U.S. Pat. No. 4,805,823; U.S. Pat. No. 5,415,334; U.S. Pat. No. 5,465,895; U.S. Pat. No. 5,597,107; U.S. Pat. No. 5,632,432; U.S. Pat. No. 5,673,840; U.S. Pat. No. 5,704,534; U.S. Pat. No. 5,814,055; U.S. Pat. No. 6,978,921; U.S. Pat. No. 7,000,818; U.S. Pat. No. 7,143,923; U.S. Pat. No. 7,303,108; U.S. Pat. No. 7,367,485; U.S. Pat. No. 7,380,695; U.S. Pat. No. 7,380,696; U.S. Pat. No. 7,404,508; U.S. Pat. No. 7,434,715; U.S. Pat. No. 7,721,930; U.S. Pub. No. 2010/0264193; and/or 2012/0239012. As noted above, the disclosures of each of those

patents and publications are incorporated by reference herein. Additional exemplary modifications that may be provided for instrument (10) will be described in greater detail below. Various suitable ways in which the below teachings may be incorporated into instrument (10) will be apparent to those of ordinary skill in the art. Similarly, various suitable ways in which the below teachings may be combined with various teachings of the patents/publications cited herein will be apparent to those of ordinary skill in the art. It should also be understood that the below teachings are not limited to instrument (10) or devices taught in the patents cited herein. The below teachings may be readily applied to various other kinds of instruments, including instruments that would not be classified as surgical staplers. Various other suitable devices and settings in which the below teachings may be applied will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00049] II. Exemplary Motorized Drive Features

[00050] In the present example, instrument (10) provides motorized control of firing beam (14). FIGS. 8-11 show exemplary components that may be used to provide motorized control of firing beam (14). In particular, FIG. 8 shows an exemplary control circuit (100) that may be used to power an electric motor (102) with electric power from a battery pack (104) (also shown in FIGS. 1-2). Electric motor (102) is operable to translate firing beam (14) longitudinally as will be described in greater detail below. It should be understood that the entire control circuit (100), including motor (102) and battery pack (104), may be housed within handle portion (20). FIG. 8 shows firing trigger (28) as an open switch, though it should be understood that this switch is closed when firing trigger (28) is actuated. Circuit (100) of this example also includes a safety switch (106) that must be closed in order to complete circuit (100), though it should be understood that safety switch (106) is merely optional. Safety switch (106) may be closed by actuating a separate button, slider, or other feature on handle portion (20).

[00051] Circuit (100) of the present example also includes a lockout switch (108), which is configured to be closed by default but is automatically opened in response to a lockout

condition. By way of example only, a lockout condition may include one or more of the following: the absence of a cartridge (37) in lower jaw (16), the presence of a spent (e.g., previously fired) cartridge (37) in lower jaw (16), an insufficiently closed anvil (18), a determination that instrument (10) has been fired too many times, and/or any other suitable conditions. Various sensors, algorithms, and other features that may be used to detect lockout conditions will be apparent to those of ordinary skill in the art in view of the teachings herein. Similarly, other suitable kinds of lockout conditions will be apparent to those of ordinary skill in the art in view of the teachings herein. It should be understood that circuit (100) is opened and thus motor (102) is inoperable when lockout switch (108) is opened. A lockout indicator (110) (e.g., an LED, etc.) is operable to provide a visual indication of the status of lockout switch (108). By way of example only, lockout switch (108), lockout indicator (110), and associated components/functionality may be configured in accordance with at least some of the teachings of U.S. Patent No. 7,644,848, entitled "Electronic Lockouts and Surgical Instrument Including Same," issued January 12, 2010, the disclosure of which is incorporated by reference herein.

[00052] Once firing beam (14) reaches a distal-most position (e.g., at the end of a cutting stroke), an end-of-stroke switch (112) is automatically switched to a closed position, reversing the polarity of the voltage applied to motor (102). This reverses the direction of rotation of motor (102), it being understood that the operator will have released firing trigger (28) at this stage of operation. In this operational state, current flows through a reverse direction indicator (114) (e.g., an LED, etc.) to provide a visual indication to the operator that motor (102) rotation has been reversed. Various suitable ways in which end-of-stroke switch (112) may be automatically switched to a closed position when firing beam (14) reaches a distal-most position will be apparent to those of ordinary skill in the art in view of the teachings herein. Similarly, various suitable forms that reverse direction indicator (114) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

[00053] Handle portion (20) of the present example also includes a manual return switch (116), which is also shown in circuit (100). Manual return switch (116) is configured to act as a “bailout” feature, enabling the operator to quickly begin retracting firing beam (14) proximally during a firing stroke. In other words, manual return switch (116) may be manually actuated when firing beam (14) has only been partially advanced distally. Manual return switch (116) may provide functionality similar to end-of-stroke switch (112), reversing the polarity of the voltage applied to motor (102) to thereby reverse the direction of rotation of motor (102). Again, this reversal may be visually indicated through reverse direction indicator (114).

[00054] In some versions, one or more of switches (28, 106, 108, 112, 116) are in the form of microswitches. Other suitable forms will be apparent to those of ordinary skill in the art in view of the teachings herein. In addition to or in lieu of the foregoing, at least part of circuit (100) may be configured in accordance with at least some of the teachings of U.S. Pat. No. 8,210,411, entitled “Motor-Driven Surgical Instrument,” issued July 3, 2012, the disclosure of which is incorporated by reference herein.

[00055] FIGS. 9-11 show various mechanical components that may be used to provide motorized translation of firing beam (14). In particular, FIG. 9 shows motor (102) housed in pistol grip (24) of handle portion (20). It should be understood that battery pack (104) (shown in FIGS. 1-2) may also be located in pistol grip (24) (e.g., below motor (102)) and/or elsewhere within handle portion (20). Motor (102) has a drive shaft (120) that is coupled with a gear assembly (122). Gear assembly (122) has an external casing (not shown) and is operable to drive an upper gear (126), which is shown in FIG. 10. Upper gear (126) meshes with a pinion (128), which is rotatably supported by a pin (129) secured in handle portion (20). It should therefore be understood that activation of motor (102) will ultimately rotate pinion (128) within handle portion (20).

[00056] As also shown in FIGS. 9-10, a translating rack (130) includes teeth (132) that mesh with pinion (128), such that rack (130) translates longitudinally when pinion (128) rotates. As shown in FIG. 11, rack (130) is coupled with an elongate member (136),

which extends through shaft (22) and includes a distal end (138) that couples with the proximal end of firing beam (14). Elongate member (136) translates within shaft (22), such that elongate member (136) communicates longitudinal motion of rack (130) to firing beam (14). It should therefore be understood that activation of motor (102) will ultimately translate firing beam (14) within end effector (12). In particular, motor (102) may drive firing beam (14) distally to sever tissue (90) and drive staples (47) into tissue (90). A switch actuation arm (134) extends laterally from rack (130), and is positioned to engage end-of-stroke switch (112) when firing beam (14) reaches a distal-most position (e.g., after tissue (90) has been severed and staples (47) have been driven into tissue (90)). As noted above, this engagement of end-of-stroke switch (112) automatically reverses motor (102) to return firing beam (14) from the distal-most position to the proximal position, enabling anvil (18) to be pivoted away from lower jaw (16) to release tissue (90).

[00057] Use of the term “pivot” (and similar terms with “pivot” as a base) should not be read as necessarily requiring pivotal movement about a fixed axis. In some versions, anvil (18) pivots about an axis that is defined by a pin (or similar feature) that slides along an elongate slot or channel as anvil (18) moves toward lower jaw (16). In such versions, the pivot axis translates along the path defined by the slot or channel while anvil (18) simultaneously pivots about that axis. In addition or in the alternative, the pivot axis may slide along the slot/channel first, with anvil (18) then pivoting about the pivot axis after the pivot axis has slid a certain distance along the slot/channel. It should be understood that such sliding/translating pivotal movement is encompassed within terms such as “pivot,” “pivots,” “pivotal,” “pivotable,” “pivoting,” and the like. Of course, some versions may provide pivotal movement of anvil (18) about an axis that remains fixed and does not translate within a slot or channel, etc.

[00058] In addition to or in lieu of the foregoing, the features operable to drive firing beam (14) may be configured in accordance with at least some of the teachings of U.S. Pub. No. 2012/0239012, the disclosure of which is incorporated by reference herein; and/or in accordance with at least some of the teachings of U.S. Pub. No. 2012/0239012, the

disclosure of which is also incorporated by reference herein. Other suitable components, features, and configurations for providing motorization of firing beam (14) will be apparent to those of ordinary skill in the art in view of the teachings herein. It should also be understood that some other versions may provide manual driving of firing beam (14), such that a motor may be omitted. By way of example only, firing beam (14) may be actuated in accordance with at least some of the teachings of any other patent/publication reference cited herein.

[00059] III. Exemplary Shaft Assembly

[00060] It will be appreciated that as a user urges instrument (10) into a surgical region, it may be desirable to approach the tissue to be clamped, stapled, or cut, from a particular angle. For instance, once end effector (12) of instrument (10) is inserted through a trocar, thoracotomy, or other passageway for entering a surgical area, the tissue that the user wishes to target may be positioned out of reach or at an askew angle in relation to end effector (12) that is aligned with shaft (22). Thus, it may be desirable for portions of instrument (10), such as end effector (12), to articulate such that the user can position anvil (18) and lower jaw (16) of end effector (12) to squarely or perpendicularly clamp against a vessel or other tissue. It will further be understood that articulating end effector (12) to squarely position end effector (12) against tissue may promote full seating and clamping of the tissue prior to cutting and stapling tissue. In addition to articulating, it may be desirable for end effector (12) to be selectively locked in a straight or articulated position such that a constant manual bias by the user is not necessary to prevent end effector (12) from pivoting or bending at articulation joint (11). It may also be desirable to automatically lock upon articulation, without requiring actuations of a separate articulation locking feature.

[00061] FIG. 12 depicts an exemplary alternative shaft assembly (200) that may be readily incorporated with instrument (10) of FIG. 1. Shaft assembly (200) provides articulation and selective locking of articulation angles, as will be described in greater detail below. Shaft assembly (200) of the present example comprises a rotation control (213), and

articulation knob (214), and an end effector (212). Rotation control (213) may be rotatably coupled with handle portion (20) of FIG. 1 or any other suitable component (e.g., robotic control interface, etc.). Rotation control (213) is operable to rotate shaft assembly (200) (including articulation knob (214) and end effector (212)) about the longitudinal axis (LA) defined by shaft assembly (200), relative to handle portion (20) (or relative whatever else rotation control (213) is rotatably coupled with). This may be useful in positioning end effector (212) at a desired angular orientation about the longitudinal axis (LA).

[00062] Articulation knob (214) is partially contained within an articulation knob casing (215). Casing (215) leads to an elongate shaft (232). Shaft assembly (200) also comprises an end effector (212) positioned distally in relation to shaft (232). End effector (212) includes an articulation joint (211) which allows end effector (212) to articulate laterally as will be described in further detail below. End effector (212) is substantially identical to end effector (12) of FIG. 1 except as otherwise described below.

[00063] FIGS. 13A-B show shaft assembly (200) and an exemplary movement of end effector (212) in response to turning of articulation knob (214). FIG. 13A shows articulation knob (214) in a first position where articulation knob (214) and end effector (212) are both generally aligned along the longitudinal axis (LA) of shaft assembly (200). The user may then manually rotate articulation knob (214) clockwise as seen in FIG. 13B to a second position. In response to the rotation of articulation knob (214), end effector (212) pivots or bends at articulation joint (211) as seen in FIG. 13B to an articulation angle (α). In the illustrated version, end effector (212) articulates generally in the direction of the rotation of articulation knob (214), though it will be understood that end effector (212) may be configured to bend in the opposite direction of the rotation of articulation knob (214). In other words, when articulation knob (214) is rotated clockwise, end effector (212) laterally pivots clockwise as shown in FIG. 13B but could be configured in some versions to pivot counter clockwise. FIG. 13B shows end effector (212) laterally pivoting clockwise slightly. It will be understood that articulation knob (214) may be rotated further to cause end effector (212) to laterally articulate further at

articulation joint (211) to any suitable angle (α). For instance, end effector (212) may pivot until an approximately 90° angle is formed across articulation joint (211). In some versions, end effector (212) may be operable to pivot even further such that end effector (212) forms an acute angle in relation to shaft (232). Other suitable variations of end effector (212) pivoting will be apparent to one of ordinary skill in the art in view of the teachings herein. It should also be understood that articulation knob (214) may define the same angle with the longitudinal axis (LA) as the articulation angle (α) defined between end effector (212) and the longitudinal axis (LA). Such complementary angling may provide the operator with visual feedback exterior to the patient, indicating the articulation angle (α) of end effector (212).

[00064] The mechanics of the articulation of end effector (212) will be discussed in further detail below. It will be appreciated that articulation knob (214) may be rotated in the counter clockwise direction to cause end effector (212) to articulate in a counter clockwise manner. Thus, depending on the desired direction and/or amount of articulation of end effector (212), the user can simply rotate articulation knob (214) of varying degrees in the direction that the user wishes end effector (212) to articulate to cause varying degrees of articulation of end effector (212).

[00065] FIG. 14 shows articulation knob (214) with casing (215) removed to better show the inner workings of articulation knob (214). Articulation knob (214) is in communication with an articulation pinion (250). Articulation pinion (250) is in communication with a first rack (252) and a second rack (256). First rack (252) is in communication with a first arm (242) through a first intermediate block (254), whereas second rack (256) is in communication with a second arm (240) through a second intermediate block (256).

[00066] Articulation knob (214) is unitarily coupled to articulation pinion (250). As a result, when the user turns articulation knob (214), articulation pinion (250) rotates together with articulation knob (214). As articulation pinion (250) rotates, articulation pinion (250) translates first rack (252) and second rack (256) accordingly in opposing

directions. For instance, as seen in FIG. 15, articulation pinion (250) is in communication with first rack (252) and second rack (256) such that if articulation pinion (250) rotates clockwise, first rack (252) retracts proximally away from end effector (212) whereas second rack (256) advances distally toward end effector. Furthermore, when articulation pinion (250) rotates counter-clockwise, first rack (252) advances distally toward end effector (212) and second rack (256) retracts proximally away from end effector (212). As first rack (252) advances and retracts, first arm (242) advances and retracts in a similar fashion. Similarly, as second rack (256) advances and retracts, second arm (240) also advances and retracts with second rack (256). Thus, rotating articulation knob (214), which is connected to articulation pinion (250), causes first arm (242) and second arm (240) to move back and forth with first rack (252) and second rack (256). Movement of first arm (242) and second arm (240) is operable to cause movement of other components in end effector (212), which will be discussed in further detail below.

[00067] FIG. 16 shows a larger view of end effector (212), including anvil (218). First arm (242) and second arm (240) are in communication with a first cam gear (230). As a result, advancing and retracting first arm (242) and second arm (240) causes first cam gear (230) to rotate, which will be described in further detail below.

[00068] FIG. 17 shows an exploded view of end effector (212) and articulation joint (211). End effector (212) comprises an anvil (218), a lower jaw (216), and a staple cartridge (275). Cartridge (275) comprises staple drivers (243), a cartridge body (237), a tray (274), and wedge sled (241). It will be appreciated that anvil (218), lower jaw (216), tray (274), cartridge body (237), and wedge sled (241) are substantially similar to anvil (18), lower jaw (16), tray (74), cartridge (37), and wedge sled (41) shown in FIG. 6. Generally, tray (274) is removably received in lower jaw (216); and tray (274), cartridge body (237), and staple drivers (243) snap together to form staple cartridge (275). The proximal portions of anvil (218) and lower jaw (216) fit within jaw sleeve (270), which is in communication with articulation joint (211). Anvil (218) is operable to close against cartridge body (237) in response to distal advancement of jaw sleeve (270), such that anvil (218) and cartridge body (237) can clamp tissue, which may then be stapled and

cut. In particular, after clamping tissue, wedge sled (241) is driven distally, which urges staple drivers (243) upwardly, which drives staples (not shown, but would otherwise be positioned above staple drivers (243)) through tissue and against anvil (218), anchoring the staples in tissue. Sled (241) in the illustrated version is driven by a knife (248), which is secured to and driven by a firing beam (219). As firing beam (219) advances, knife (248) cuts tissue while driving sled (241).

[00069] End effector (212) of the present example further comprises resilient a lockout feature (249) that is operable to cooperate with cam holding body (276) to selectively restrict advancement of knife (248) in the absence of an unfired cartridge (275) being loaded in lower jaw (216). By way of example only, lockout feature (249) and associated components may be configured and operable in accordance with at least some of the teachings of U.S. Pat. App. No. [Attorney Docket Number END7175USNP], entitled "Lockout Feature for Movable Cutting Member of Surgical Instrument," filed on even date herewith, the disclosure of which is incorporated by reference herein.

[00070] Articulation joint (211) comprises several components that will be discussed in further detail below. Generally speaking, articulation joint (211) comprises first cam gear (230), second cam gear (231), cam holding body (276), a channel pin (217), joint base (272), a lock bar (262), and a spring (264).

[00071] First arm (242) distally terminates in to a first hook (244), while second arm (240) distally terminates in a second hook (246). Hooks (244, 246) are in communication with cam openings (260) of first cam gear (230). As a result, when first arm (242) advances toward end effector (212) and second arm (240) retracts, first cam gear (230) rotates counter clockwise. When first arm (242) instead retracts and second arm (240) advances toward end effector (212), first cam gear (230) rotates clockwise. Thus, as arms (242, 240) push and pull on cam openings (260) via hooks (244, 246), first cam gear (230) rotates accordingly as just described.

[00072] First cam gear (230) is stacked on a second cam gear (231). Second cam gear (231) and cam holding pin (279) are unitary features of cam holding body (276). In some versions, second cam gear (231) may be separately constructed and fixedly coupled with cam holding body (276), such that as second cam gear (231) rotates, cam holding body (276) rotates. First cam gear (230) is rotationally coupled with cam holding pin (279), which is coaxially aligned with base opening (277) of joint base (272) along a pivot axis (280). Thus, first cam gear (230) is rotatable about pivot axis (280), relative to second cam gear (231) and cam holding body (276). Lock bar (262) is in selective communication with first cam gear (230) and second cam gear (231), which will be described further below. Lock bar (262) is further in communication with spring (264), which distally biases lock bar (262). Joint base (272) is shaped to provide a seat and/or channel for lock bar (262) to advance. Lock bar (262) further includes a pair of bosses (287) operable to engage joint base (272) to restrict distal motion of lock bar (262).

[00073] IV. Exemplary Movement of the Shaft Assembly

[00074] As discussed above, actuating articulation knob (214) is operable to cause opposing advancement and retraction of arms (242, 240). It will be understood that this motion of arms (242, 240) is operable to rotate first cam gear (230) about cam holding pin (279). As a result of rotating first cam gear (230), second cam gear (231) rotates with cam holding body (276). Thus, articulation joint (211) articulates, thereby pivoting end effector (212) at articulation joint (211). In particular, cam holding pin (279) and base opening (274) define a pivot axis (280), which is generally perpendicular to the longitudinal axis (LA). End effector (212) pivots about pivot axis (280) in response to the rotation of first cam gear (230), which drives second cam gear (231) as will be discussed below. FIGS. 18A-E illustrate the details of rotating first cam gear (230) to drive the articulation of end effector (212).

[00075] FIG. 18A shows articulation joint (211) in a first position. Lock bar (262) is distally biased to engage second cam gear (231). In particular, the distal end of lock bar (262) comprises a lock tooth (236) that fits between first cam teeth (233) and second cam

teeth (235) and abuts second cam gear (231), which can be seen in further detail in FIG. 19. As a result of the distal bias provided by spring (264), lock tooth (236) acts as a positive lock and thus maintains the rotational position of second cam gear (231). By maintaining the rotational position of second cam gear (231), lock bar (262) maintains the angular position of end effector (212) about pivot axis (280), thereby maintaining any articulation angle (α). First cam gear (230) comprises a pair of cam wings (238, 239), and cam holding body (276) comprises a pair of bosses (271, 273). Bosses (271, 273) are unitary features of second cam gear (231) such that as bosses (271, 273) rotate, second cam gear (231) also rotates. It will be appreciated that in the first position of FIG. 18A, cam wings (238, 239) and bosses (271, 273) define a small gap (261) therebetween. As a result, cam wings (238, 239) and bosses (271, 273) are not in contact. The interaction involving contact between cam wings (238, 239) and bosses (271, 273) will be described in further detail below with reference to FIGS. 18B-E. During a surgical operation, the user may guide shaft assembly (200) through a passageway (e.g. trocar, thoracotomy, etc.) to reach the surgical area with end effector (212) in a straightened position as shown in FIG. 18A.

[00076] FIG. 19 shows an enlarged view of lock tooth (236) in the position shown in FIG. 18A. As can be seen in the illustrated version, lock tooth (236) has generally straight parallel sides (286) that are operable to fit between first cam teeth (233) and second cam teeth (235). The distal end of lock tooth (236) has a rounded tip (285) with angled sides (281) leading to parallel sides (286). Each tooth (235) of second cam teeth (235) comprises generally straight parallel sides (283) and angled sides (284). Parallel sides (283) are operable to engage parallel sides (286) of lock tooth (236) to prevent lock tooth (236) from riding along second cam teeth (235) without assistance from first cam gear (230). This engagement between at least one side (283) and at least one side (286) also prevents cam holding body (276) from rotating about pivot axis (280), thereby preventing end effector (212) from pivoting at articulation joint (211).

[00077] Once first cam gear (230) rotates as shown in FIGS. 18B-C and as will be described in greater detail below, a rounded triangular tooth (233) of first cam gear (230)

will cam against angled sides (281), and will thereby drive lock bar (262) proximally in response to first cam (230) rotating. It should be understood that tooth (233) may have a variety of different shapes other than triangular. Lock tooth (236) moves proximally sufficiently such that angled sides (281) of lock tooth (236) can then eventually engage and ride along angled sides (284) of second cam teeth (235) as first cam gear (230) continues to rotate and as second cam gear (231) rotates. This provides further camming action to drive lock bar (262) proximally. Once lock tooth (236) traverses angled sides (284) of second cam teeth (235), then lock tooth (236) returns distally to a position between the next pair of first cam teeth (233) and second cam teeth (235) similar to the positioning shown in FIG. 19. For illustrative purposes, advancing lock tooth (236) between one set of first cam teeth (233) and second cam teeth (235) to an adjacent set of first cam teeth (233) and second cam teeth (235) may be considered one articulation increment. As lock tooth (236) distally advances, lock tooth (236) strikes second cam gear (231) between second cam teeth (235). It will be understood that lock tooth (236) need not necessarily extend far enough to strike second cam gear (231). For instance, lock tooth (236) may only extend distally such that parallel sides (283) prevent lock tooth (236) from riding along second cam gear (231) without assistance from first cam teeth (233). In the illustrated version, bosses (287) engage joint base (272) to prevent further distal motion of lock bar (262).

[00078] As noted above, the operator may wish to pivot end effector (212) at articulation joint (211) to better position end effector (212) in relation to targeted tissue. FIG. 18B shows a second position for articulation joint (211) to move to in response to turning articulation knob (214) shown in FIG. 14. In the illustrated version, the user has turned articulation knob (214) counter clockwise, which rotates articulation pinion (250) counter clockwise as well. As articulation pinion (250) rotates counter clockwise, first rack (252) moves distally and second rack (256) moves proximally in relation to end effector (212). Accordingly, first arm (242) and second arm (240) as shown in FIG. 18B move such that first arm (242) advances toward effector (212) and second arm (240) retracts away from end effector (212). It will be appreciated that the distal portions of first arm (242) and

second arm (240) of the illustrated version are not positioned parallel in relation to each other. Instead, first arm (242) and second arm (240) are obliquely angled in relation to each other, though it will be understood that first arm (242) and second arm (240) could be positioned parallel to each other.

[00079] Movement of arms (242, 240) as seen in FIG. 18B causes first cam gear (230) to rotate counter clockwise about pivot axis (280). As first cam gear (230) rotates, two actions occur in a generally simultaneous manner. First cam teeth (233) have a rounded triangular shape that urges lock bar (262) proximally away from end effector (212) through a camming action as a result of first cam teeth (233) engaging angled sides (281). Again, teeth (233) may have a variety of different shapes other than triangular. Spring (264) compresses to accommodate proximal motion of lock bar (262). As a result, rounded tip (285) moves proximally sufficient to traverse parallel sides (283). Additionally, cam wings (238, 239) rotate counter clockwise with first cam gear (230). As a result of the rotation, cam wing (239) removes gap (261) between boss (273) and engages boss (273). Meanwhile, cam wing (238) moves rotationally away from boss (271). It will be understood that while first cam gear (230) and lock bar (262) have moved in response to the movement of arms (242, 240) during the transition from the configuration shown in FIG. 18A to the configuration shown in FIG. 18B, second cam gear (231) and accordingly end effector (212) have not yet moved. Thus, end effector (212) remains in a straight orientation at this stage.

[00080] FIG. 18C shows a third position of articulation joint (211). It will be understood that the user continues to rotate articulation knob (214) in an effort to articulate end effector (212). Arms (242, 240) continue to move such that first arm (242) moves distally and second arm (240) moves proximally. Movement of arms (242, 240) continues to rotate first cam gear (230), which causes cam wing (239) to rotationally move further thereby urging boss (273) to rotationally move as well. Since boss (273) is unitary with second cam gear (231), second cam gear (231) begins to rotate. As second cam gear rotates (231), lock bar (262) moves further proximally as a result of angled sides (284) camming against angled sides (281) of lock tooth (236). Thus, lock tooth (236) rides

along second cam teeth (235). Second cam gear (231) rotates until tip (288) of second cam gear (231) engages rounded tip (285). Second cam teeth (235) have parallel sides (283) such that angled edges (281) of lock tooth (236) can engage angled sides (284) only after first cam teeth (233) urges lock tooth (236) proximally such that rounded tip (285) traverses parallel sides (283). Prior to riding along first cam teeth (233), lock tooth (236) is generally unable to ride along second cam teeth (235) due to parallel sides (283) engaging parallel sides (286). It will further be appreciated that as lock tooth (236) rides along angled sides (284), lock tooth (236) disengages first cam teeth (233). As also seen in FIG. 18C, lock bar (262) and lock tooth (236) have moved to a proximal most position with just second cam teeth tip (288) being in contact with lock tooth (236). Also as a result of rotation of second cam gear (231), cam holding body (276) and accordingly, sleeve (270), which leads to end effector (212), articulates in a counter clockwise direction.

[00081] FIG. 18D shows a fourth position for articulation region (211). Once again, it will be understood that user is continuing to rotate articulation knob (214) in an effort to cause further articulation of end effector (212). Arms (242, 240) continue to move such that first arm (242) moves distally further and second arm (240) moves proximally further. Movement of arms (242, 240) continues to rotate first cam gear (230), which causes cam wing (239) to push boss (273) rotationally further. Lock tooth (236) continues to ride along second cam teeth (235) until the distal bias caused by spring (264) urges lock bar (262) into the position shown in FIG. 18D. It will be appreciated that when lock bar (262) snaps into the position shown in FIG. 18D, an audible click or snap may be heard or felt. As a result, the user receives audible and/or tactile confirmation that lock tooth (236) has moved from between one set of cam teeth (233, 235) to another or otherwise has rotated by a single articulation increment. When in the position shown in FIG. 18D, first cam gear (230) stops rotating and lock tooth (236) fits between cam teeth (233, 235). Sleeve (270) and accordingly end effector (212) stop articulating. A positive lock has formed because any rotational motion of second cam gear (231) urged by transverse forces on end effector (212) would result in parallel sides (286) engaging

parallel sides (283) and stopping any further rotation of second cam gear (231), which locks the articulation of end effector (212). It should be understood that the transition from the configuration shown in FIG. 18A to the configuration shown in FIG. 18D represents articulation through one articulation increment, or increment of articulation motion, in which the distance is defined generally by the spaces between second cam teeth (235)

[00082] It will be understood that in the position shown in FIG. 18D, end effector (212) has articulated thereby providing the user with a shaft assembly (200) with an articulated end effector (212). It will be appreciated that the user may wish to use shaft assembly (200) in the position shown in FIG. 18D or may wish to pivot end effector (212) further by one or more additional articulation increments. In the event that the user does not rotate articulation knob (214) further, the locking of lock tooth (236) between first cam teeth (233) and second cam teeth (235) prevents end effector (212) from pivoting to return to a straight position. Once end effector (212) has been articulated to a desired angle (α), it will be understood that the user may actuate firing beam (213) to drive knife (248) to cut and drive staples through tissue. For instance, knife (248) and firing beam (213) may be in communication through, for instance, a bendable beam such that firing beam (213) can advance through any degree of pivot of articulation joint (211).

[00083] FIG. 18E shows a fifth position for articulation joint (211) in the event that the user wishes to pivot end effector (212) further. Once again, it will be understood that user continues to rotate articulation knob (214). As a result, arms (242, 240) continue to move such that first arm (242) moves distally further and second arm (240) moves proximally further. Movement of arms (242, 240) continues to rotate first cam gear (230), which causes cam wing (239) to push boss (273) rotationally. First cam gear (230) and second cam gear (231) move similarly as shown in FIGS. 18B-D, which causes end effector (212) to articulate further as well as lock in a more articulated position. It will be understood that the user may continue to rotate articulation knob (214) to cause end effector (212) to pivot as far as the user desires. Furthermore, the user may rotate articulation knob (214) in the opposite direction to cause arms (242, 240) and cam gears

(230, 231) to move in the opposite direction, thereby causing end effector (212) to articulate in an opposite direction.

[00084] As seen in the exemplary actuation shown in FIGS. 18A-18E, first cam gear (230) is operable to unlock articulation joint (211) and pivot end effector (212) at articulation joint (211) about pivot axis (280), by transferring motion from arms (242, 240) to first cam gear (230). In addition, second cam gear (231) and lock bar (262) cooperate to lock articulation joint (211), to thereby lock the angle (α) of end effector (212) relative to the longitudinal axis (LA) of shaft assembly (200).

[00085] V. Miscellaneous

[00086] It should be understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The above-described teachings, expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

[00087] It should be appreciated that any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated material does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

[00088] Versions of the devices described above may have application in conventional medical treatments and procedures conducted by a medical professional, as well as application in robotic-assisted medical treatments and procedures. By way of example only, various teachings herein may be readily incorporated into a robotic surgical system such as the DAVINCI™ system by Intuitive Surgical, Inc., of Sunnyvale, California. Similarly, those of ordinary skill in the art will recognize that various teachings herein may be readily combined with various teachings of any of the following: U.S. Pat. No. 5,792,135, entitled “Articulated Surgical Instrument For Performing Minimally Invasive Surgery With Enhanced Dexterity and Sensitivity,” issued August 11, 1998, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,817,084, entitled “Remote Center Positioning Device with Flexible Drive,” issued October 6, 1998, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,878,193, entitled “Automated Endoscope System for Optimal Positioning,” issued March 2, 1999, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,231,565, entitled “Robotic Arm DLUS for Performing Surgical Tasks,” issued May 15, 2001, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,783,524, entitled “Robotic Surgical Tool with Ultrasound Cauterizing and Cutting Instrument,” issued August 31, 2004, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,364,888, entitled “Alignment of Master and Slave in a Minimally Invasive Surgical Apparatus,” issued April 2, 2002, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,524,320, entitled “Mechanical Actuator Interface System for Robotic Surgical Tools,” issued April 28, 2009, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,691,098, entitled “Platform Link Wrist Mechanism,” issued April 6, 2010, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,806,891, entitled “Repositioning and Reorientation of Master/Slave Relationship in Minimally Invasive Telesurgery,” issued October 5, 2010, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2013/0012957, entitled “Automated End Effector Component Reloading System for Use with a Robotic System,” published January 10, 2013, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0199630, entitled “Robotically-Controlled Surgical Instrument with

Force-Feedback Capabilities,” published August 9, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0132450, entitled “Shiftable Drive Interface for Robotically-Controlled Surgical Tool,” published May 31, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0199633, entitled “Surgical Stapling Instruments with Cam-Driven Staple Deployment Arrangements,” published August 9, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0199631, entitled “Robotically-Controlled Motorized Surgical End Effector System with Rotary Actuated Closure Systems Having Variable Actuation Speeds,” published August 9, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0199632, entitled “Robotically-Controlled Surgical Instrument with Selectively Articulatable End Effector,” published August 9, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0203247, entitled “Robotically-Controlled Surgical End Effector System,” published August 9, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0211546, entitled “Drive Interface for Operably Coupling a Manipulatable Surgical Tool to a Robot,” published August 23, 2012; U.S. Pub. No. 2012/0138660, entitled “Robotically-Controlled Cable-Based Surgical End Effectors,” published June 7, 2012, the disclosure of which is incorporated by reference herein; and/or U.S. Pub. No. 2012/0205421, entitled “Robotically-Controlled Surgical End Effector System with Rotary Actuated Closure Systems,” published August 16, 2012, the disclosure of which is incorporated by reference herein.

[00089] Versions of the devices described above may be designed to be disposed of after a single use, or they can be designed to be used multiple times. Versions may, in either or both cases, be reconditioned for reuse after at least one use. Reconditioning may include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, some versions of the device may be disassembled, and any number of the particular pieces or parts of the device may be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, some versions of the device may be

reassembled for subsequent use either at a reconditioning facility, or by a user immediately prior to a procedure. Those skilled in the art will appreciate that reconditioning of a device may utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

[00090] By way of example only, versions described herein may be sterilized before and/or after a procedure. In one sterilization technique, the device is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and device may then be placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation may kill bacteria on the device and in the container. The sterilized device may then be stored in the sterile container for later use. A device may also be sterilized using any other technique known in the art, including but not limited to beta or gamma radiation, ethylene oxide, or steam.

[00091] Having shown and described various embodiments of the present invention, further adaptations of the methods and systems described herein may be accomplished by appropriate modifications by one of ordinary skill in the art without departing from the scope of the present invention. Several of such potential modifications have been mentioned, and others will be apparent to those skilled in the art. For instance, the examples, embodiments, geometrics, materials, dimensions, ratios, steps, and the like discussed above are illustrative and are not required. Accordingly, the scope of the present invention should be considered in terms of the following claims and is understood not to be limited to the details of structure and operation shown and described in the specification and drawings.

I/We Claim:

1. An apparatus, comprising:
 - (a) a body; and
 - (b) a shaft assembly in communication with the body; wherein the shaft assembly comprises:
 - (i) an end effector having an articulation joint;
 - (ii) a first cam gear rotatably positioned within the shaft assembly,
 - (iii) a second cam gear in communication with the end effector at the articulation joint, and
 - (iv) a lock bar distally biased to lock against the second cam gear, wherein the first cam gear is rotatable through a first range of motion to unlock the lock bar relative to the second cam gear, wherein the first cam gear is rotatable through a second range of motion to rotate the end effector at the articulation joint.
2. The apparatus of claim 1, wherein the first cam gear comprises a plurality of cam wings configured to urge rotation of the second cam gear.
3. The apparatus of claim 2, wherein the second cam gear comprises a plurality of bosses configured to engage the plurality of cam wings.
4. The apparatus of claim 1, further comprising an articulation knob in communication with a first arm and a second arm, wherein the first arm and the second arm are in opposing communication with the first cam gear, wherein the articulation knob is configured to rotate to effectuate opposing motion of the first arm and the second arm.
5. The apparatus of claim 1, wherein the lock bar comprises a lock tooth, wherein the second cam gear comprises second cam teeth, wherein the lock bar is shaped to complement the shape of the second cam teeth.

6. The apparatus of claim 5, wherein the second cam teeth comprise straight walls.
7. The apparatus of claim 5, wherein the first cam gear comprises first cam teeth, wherein the first cam teeth have a rounded shape.
8. The apparatus of claim 5, wherein the first cam gear comprises first cam teeth, wherein the second cam gear comprises second cam teeth, wherein the lock tooth is positionable between the first cam teeth and the second cam teeth.
9. The apparatus of claim 8, wherein the lock tooth is configured to snap into a position between the first cam teeth and the second cam teeth, wherein the lock tooth is operable to produce an audible click when the lock tooth snaps into the position between the first cam teeth and the second cam teeth.
10. The apparatus of claim 8, wherein the lock tooth is configured to snap into a position between the first cam teeth and the second cam teeth, wherein the lock tooth is operable to produce a tactile feedback click when the lock tooth snaps into the position between the first cam teeth and the second cam teeth.
11. The apparatus of claim 1, wherein the first cam gear comprises cam wings, wherein the second cam gear comprises bosses, wherein the cam wings and the bosses are positionable such that a gap is maintained between the cam wings and the bosses.
12. The apparatus of claim 1, wherein the first cam gear and the second cam gear are coaxially aligned with a pivot axis, wherein the pivot axis is perpendicular to the end effector.
13. The apparatus of claim 1, wherein the second cam gear comprises second cam teeth having parallel sides, wherein the lock bar comprises a lock tooth having parallel sides, wherein the parallel sides of the lock tooth are configured to engage the parallel sides of the

second cam teeth to thereby prevent rotation of the second cam gear.

14. The apparatus of claim 1, wherein the lock bar comprises at least one laterally extending boss configured to prevent the distal movement of the lock bar beyond a predetermined point.

15. The apparatus of claim 1, further comprising a spring in communication with the lock bar, wherein the spring is operable to distally bias the lock bar.

16. An apparatus comprising:

- (a) a body; and
- (b) a shaft assembly in communication with the body; wherein the shaft assembly comprises:
 - (i) an end effector positioned at a distal end of the shaft assembly,
 - (ii) an articulation joint positioned at a proximal end of the end effector,
 - (iii) a first cam gear positioned at the distal end of the shaft assembly, wherein the first cam gear is configured to rotate,
 - (iv) a second cam gear in communication with the end effector through the articulation joint, wherein the second cam gear is operable to drive articulation of the end effector at the articulation joint, and
 - (v) a lock bar in selective communication with the first cam gear and the second cam gear, wherein the lock bar is movable between a distal position and a proximal position, wherein the lock bar is configured to impede the rotation of the second cam gear when the lock bar is in the distal position, wherein the lock bar is configured to allow rotation of the second cam gear when the lock bar is in the proximal position, wherein the first cam gear is configured to drive the lock bar from the distal position to the proximal position through rotation of the first cam gear.

17. The apparatus of claim 16, wherein the lock bar comprises a lock tooth configured to impede the rotational motion of the second cam gear.

18. The apparatus of claim 16, wherein the first cam gear comprises first cam teeth, wherein the first cam teeth have a shape configured to allow the lock bar to ride along the first cam teeth through a camming motion.

19. The apparatus of claim 16, wherein the lock bar is configured to produce an audible click when the lock bar is in selective communication with the second cam gear.

20. A method of articulating an end effector using a shaft assembly comprising a first cam gear, a second cam gear, a first arm, a second arm, and a lock bar, wherein the second cam gear is in communication with the first cam gear, wherein the first arm and the second arm are in communication with the cam gear, wherein the lock bar is in selective communication with the first cam gear and the second cam gear, wherein the second cam gear is in pivotal communication with the end effector, the method comprising:

- (a) actuating the first arm and the second arm to rotate the first cam gear;
- (b) rotating the first cam gear;
- (c) moving the lock bar in the proximal direction such that the lock bar rides along the first cam gear and the second cam gear in a sequential manner;
- (d) rotating the second cam gear thereby articulating the end effector; and
- (e) moving the lock bar in the distal direction.

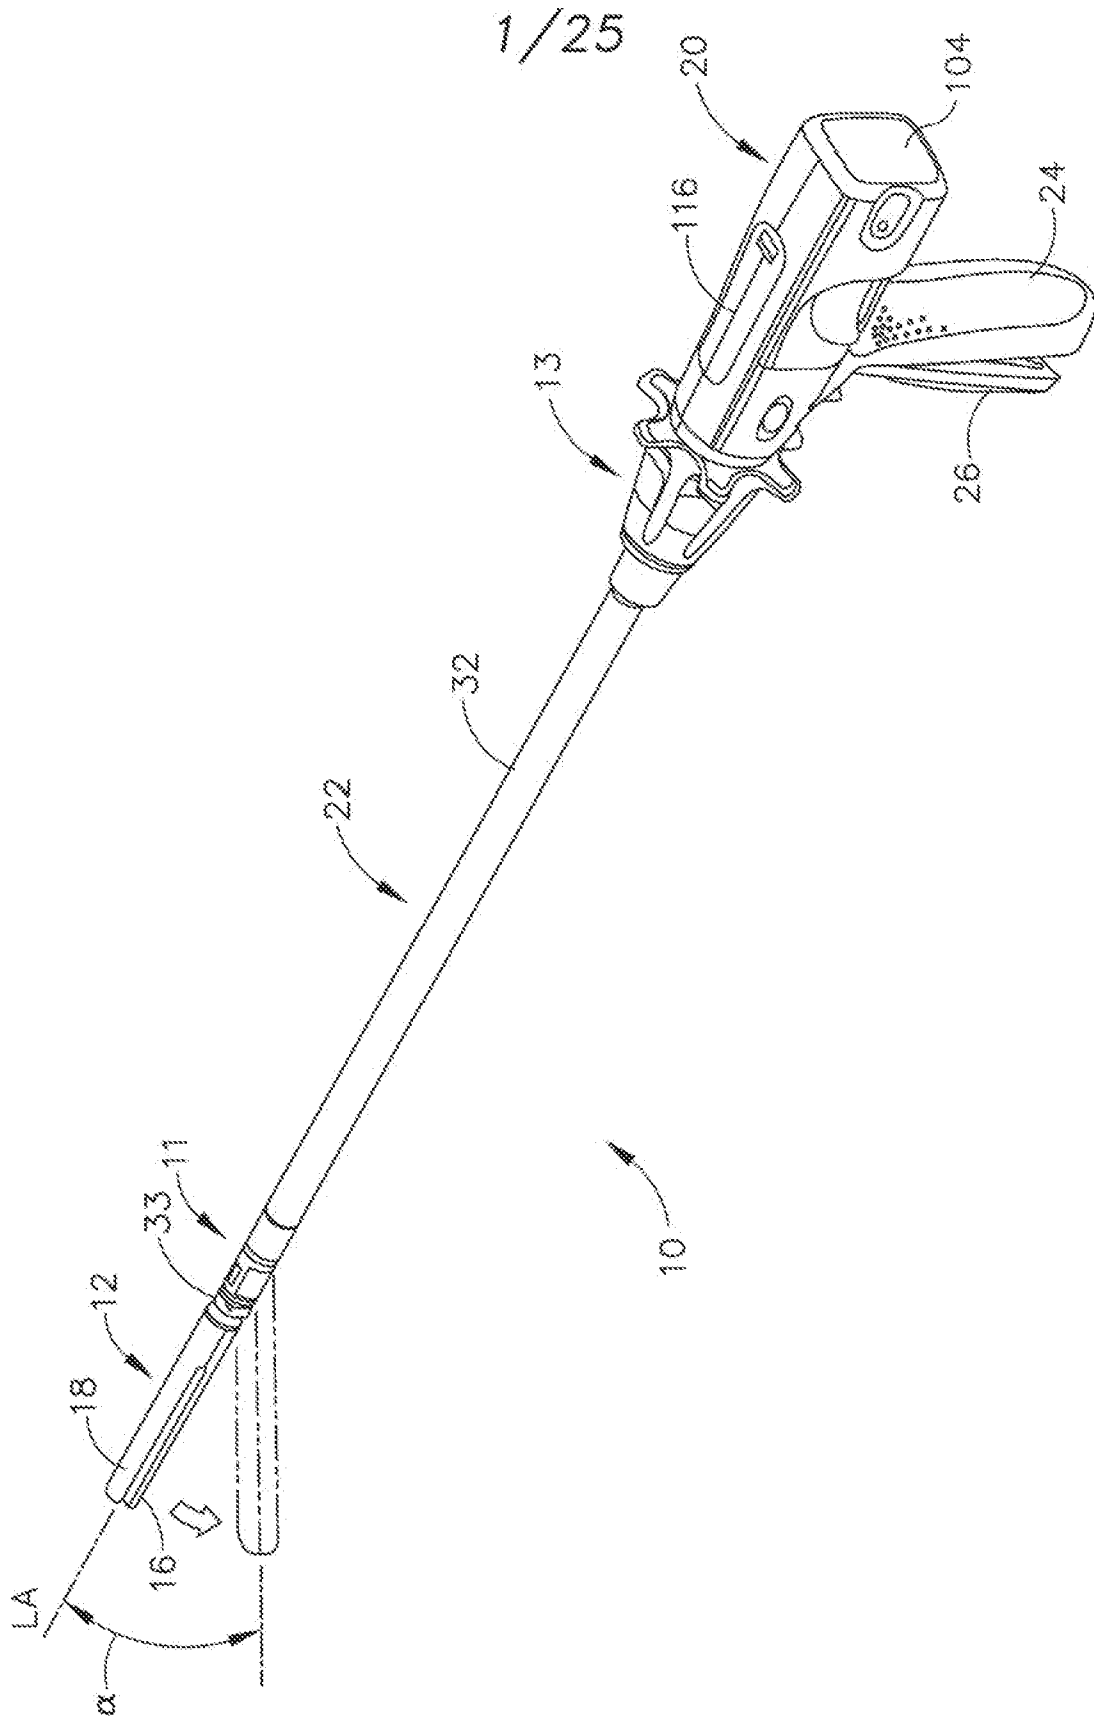


Fig. 1

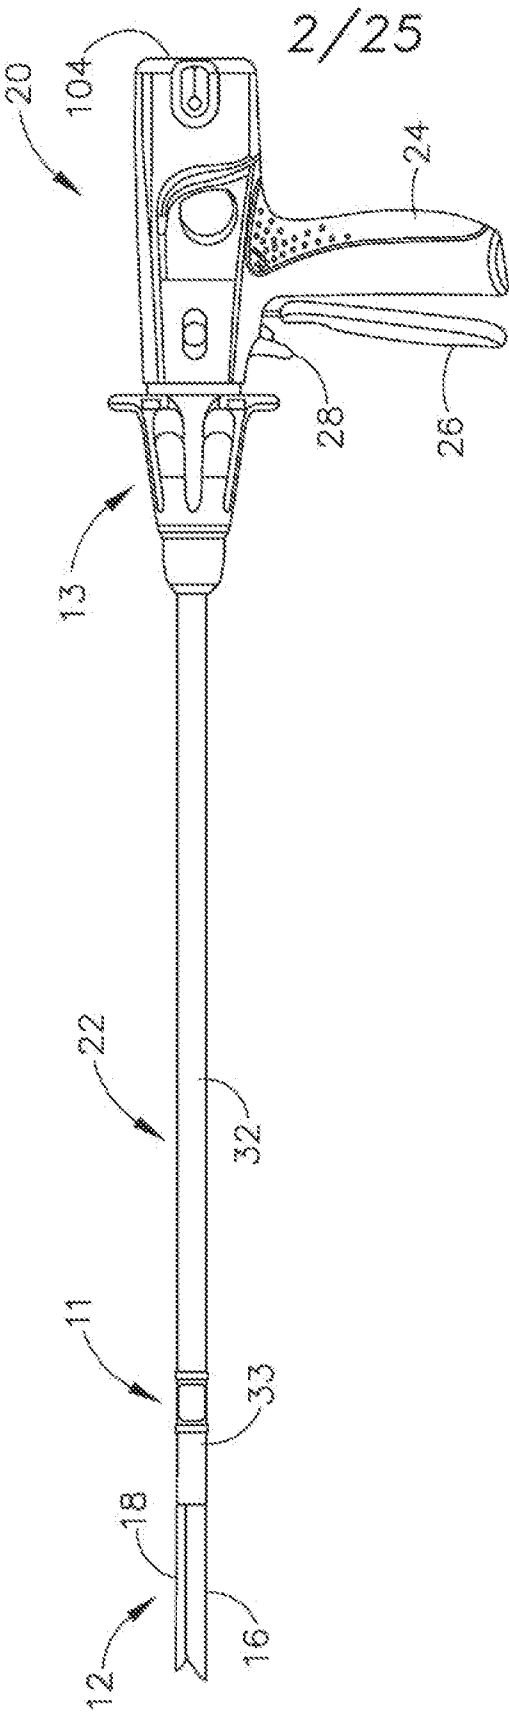


Fig.2

3/25

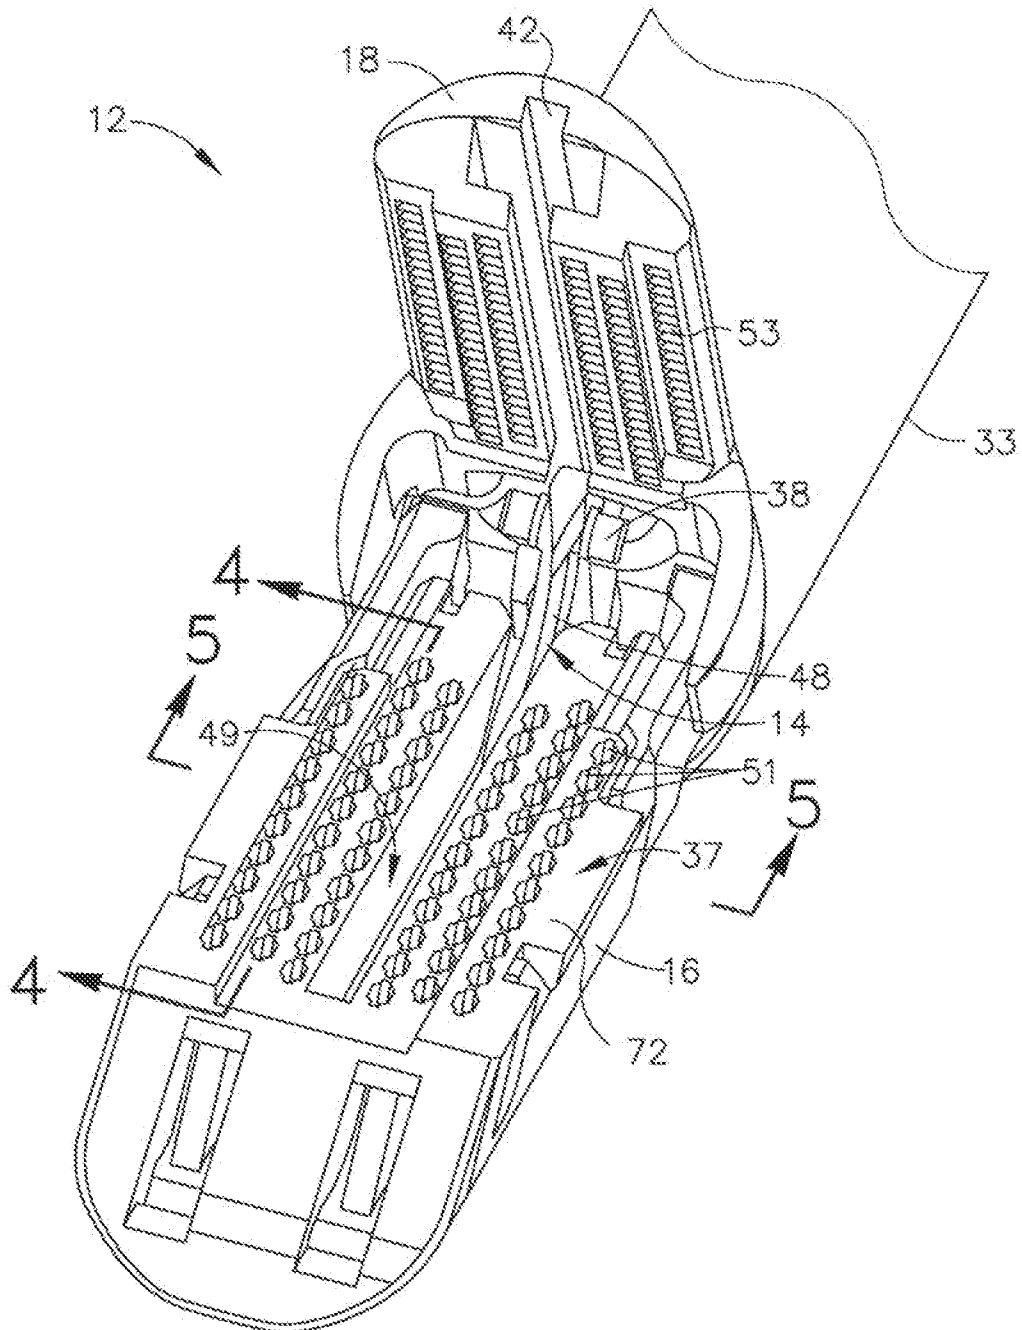


Fig.3

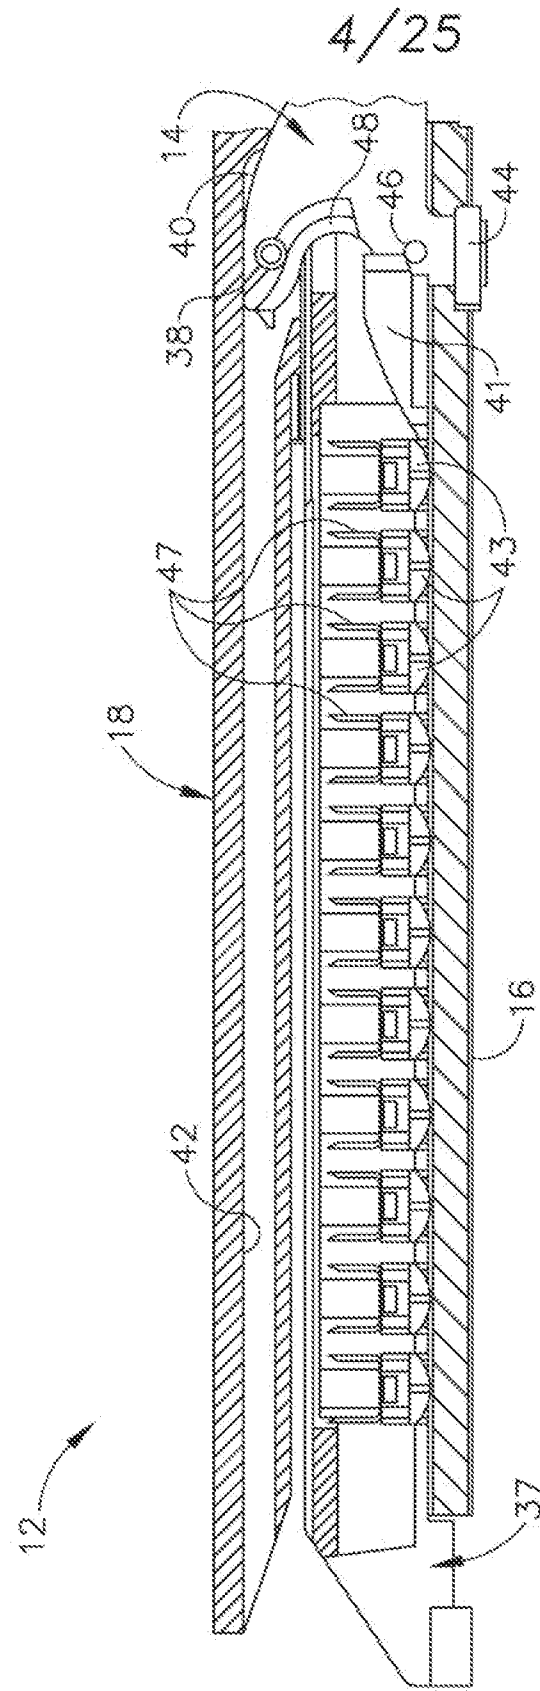


Fig. 4A

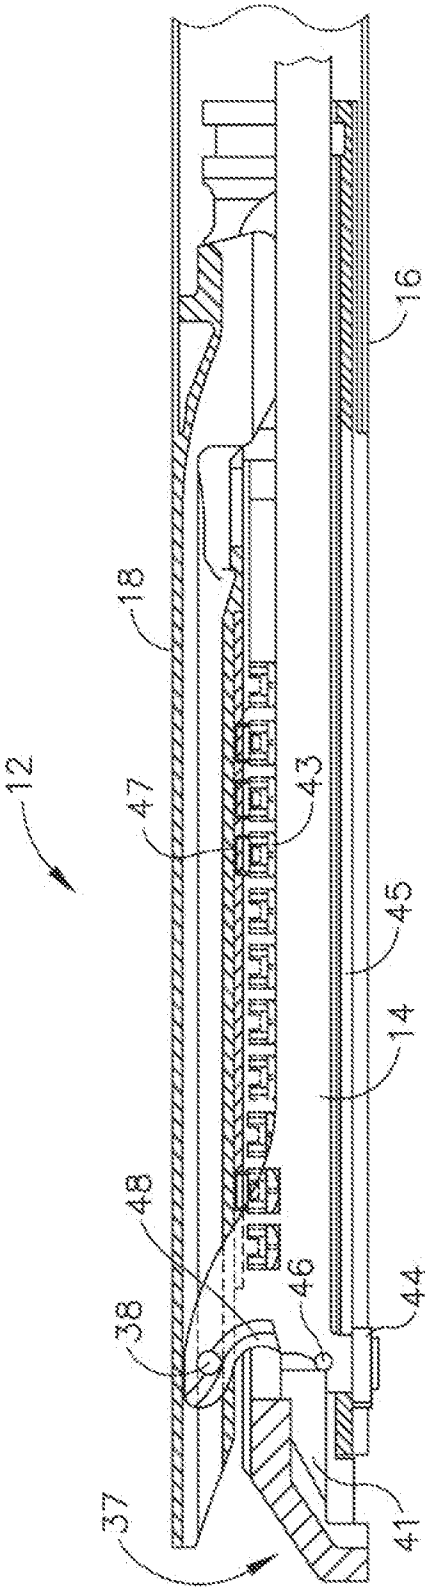


Fig. 4B

6/25



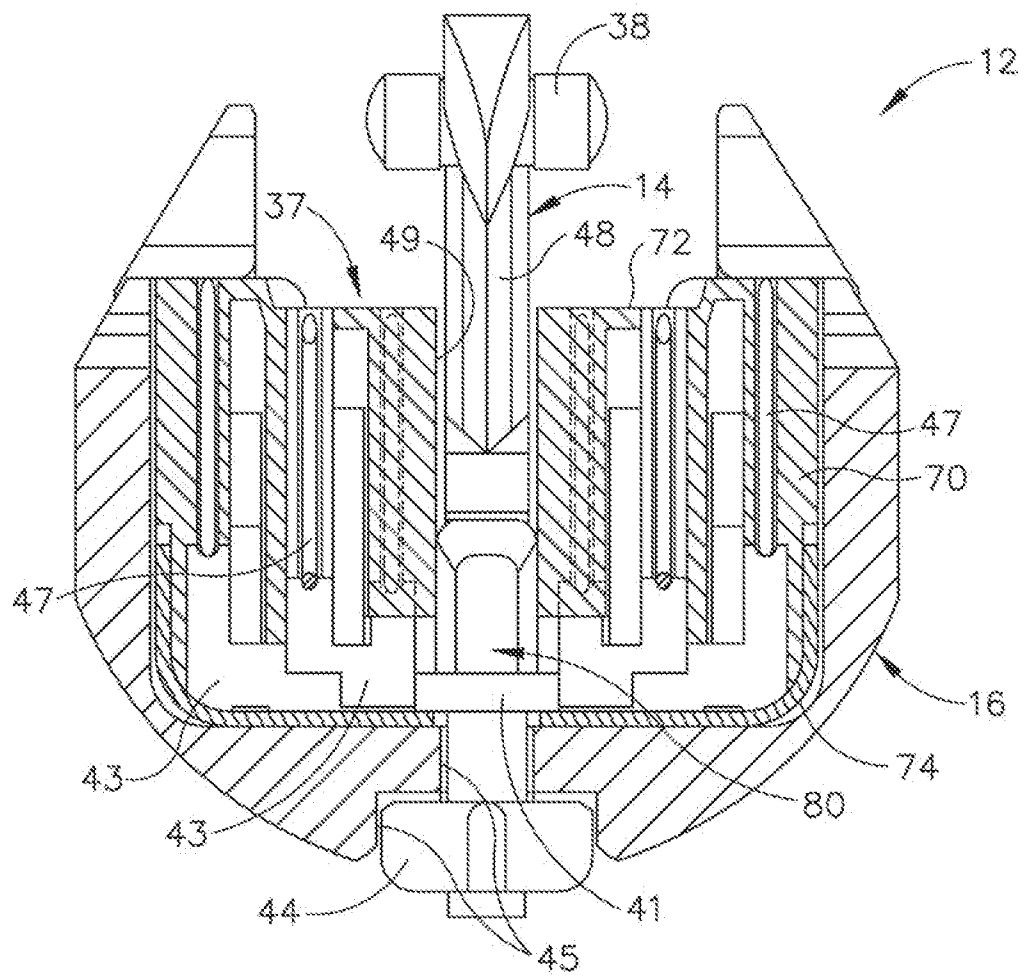


Fig.5

7/25

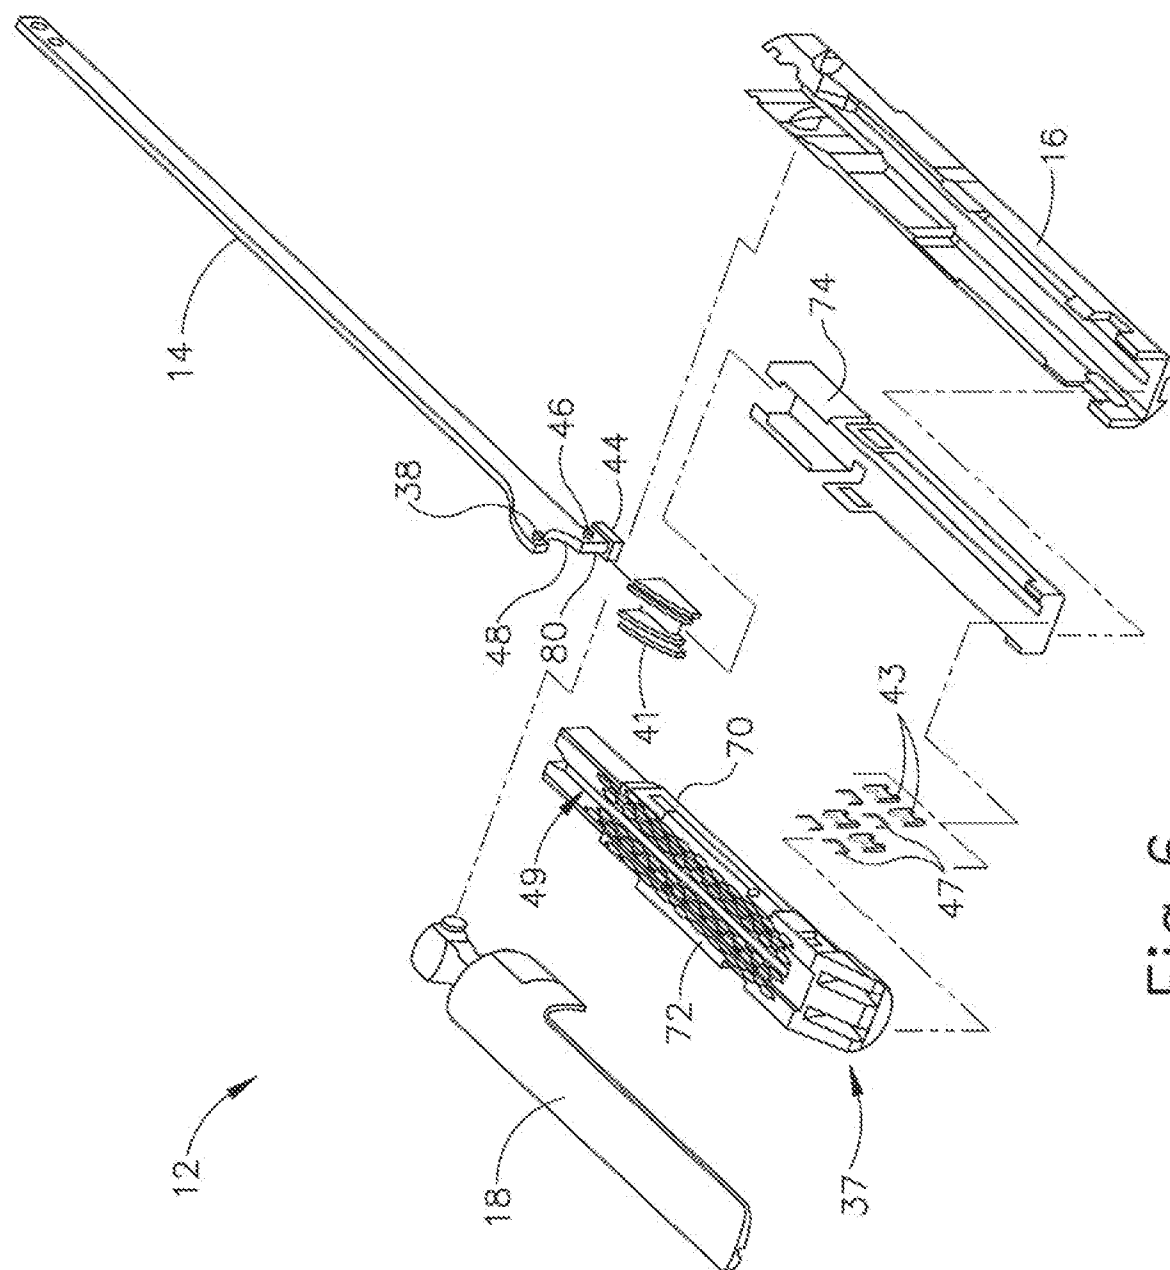

60
*
59
*
L

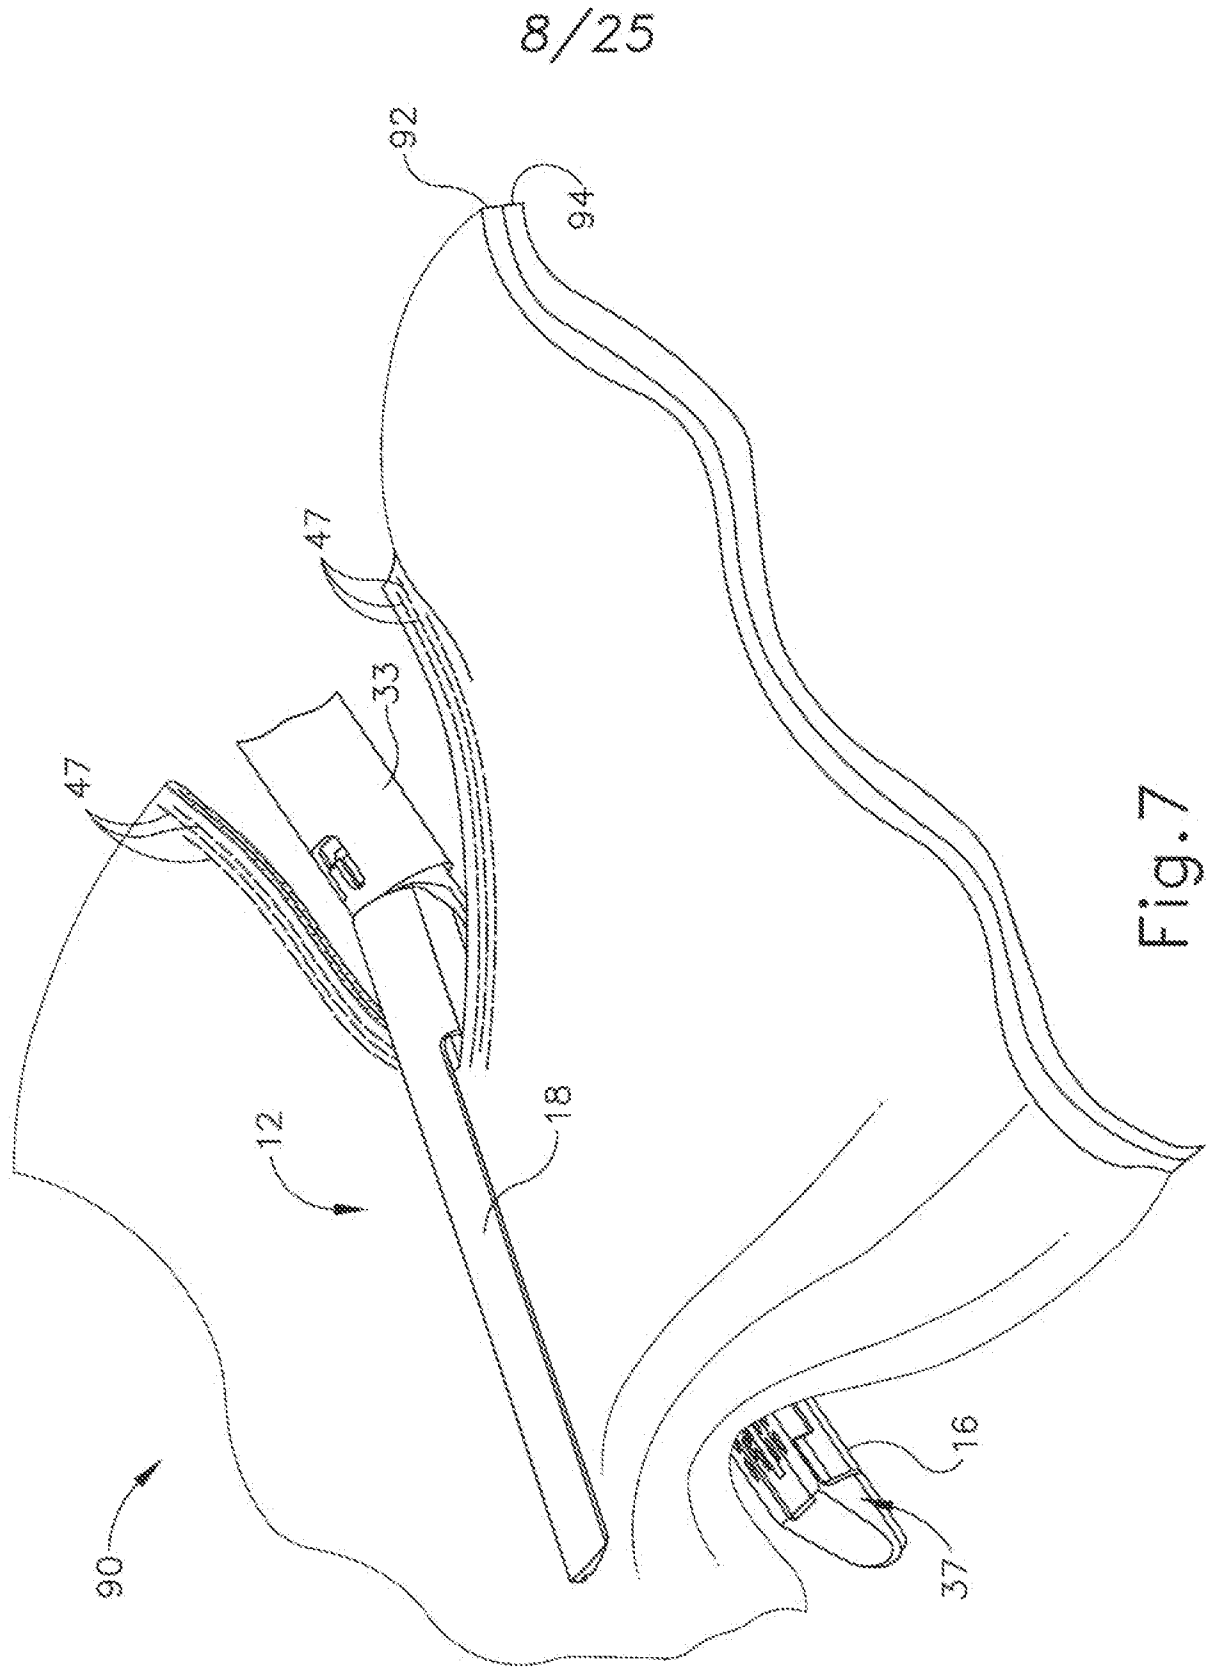

9/25

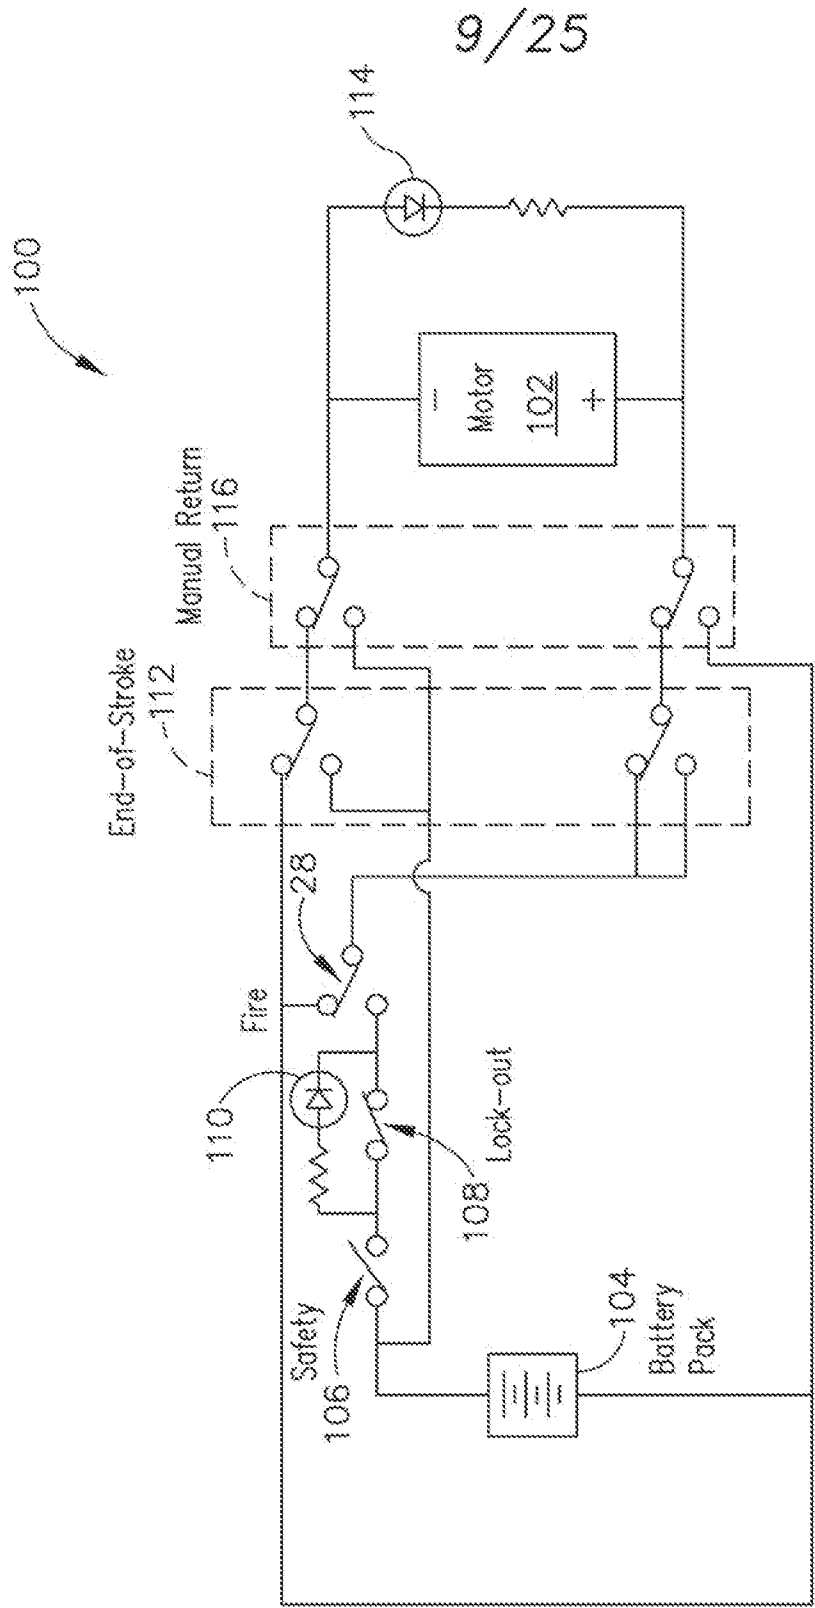


Fig.8

10/25

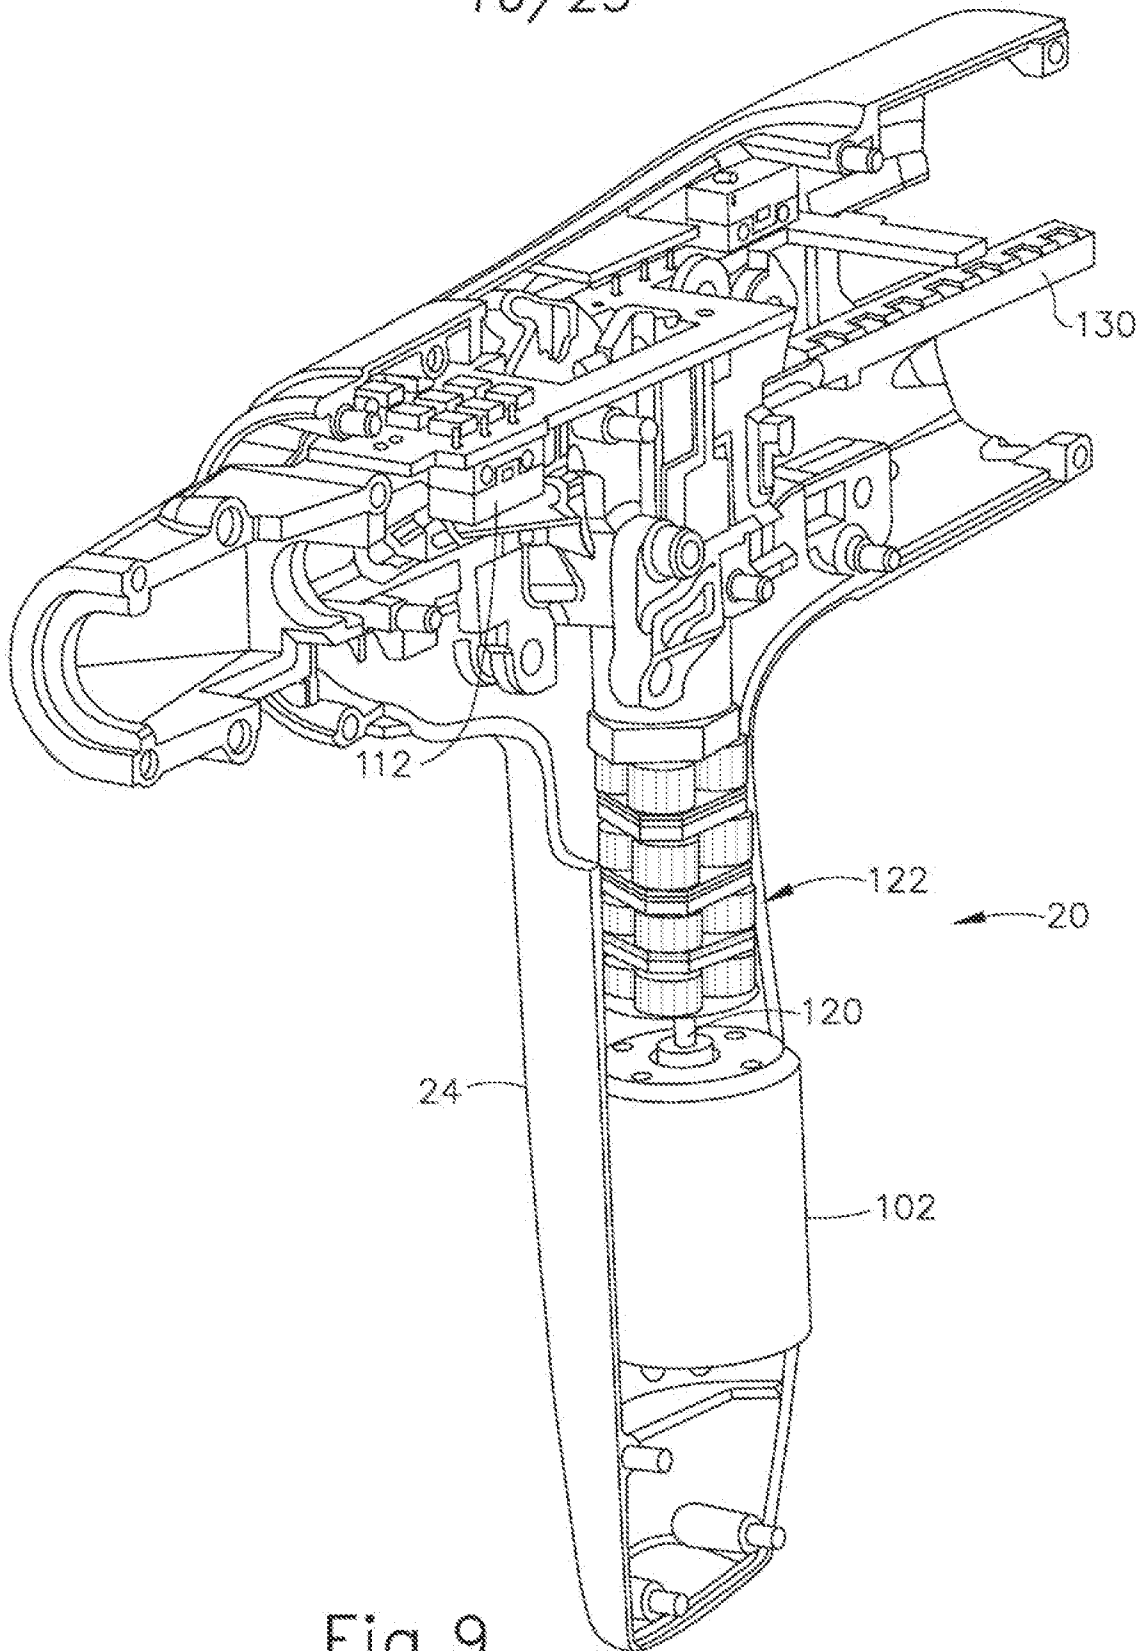


Fig.9

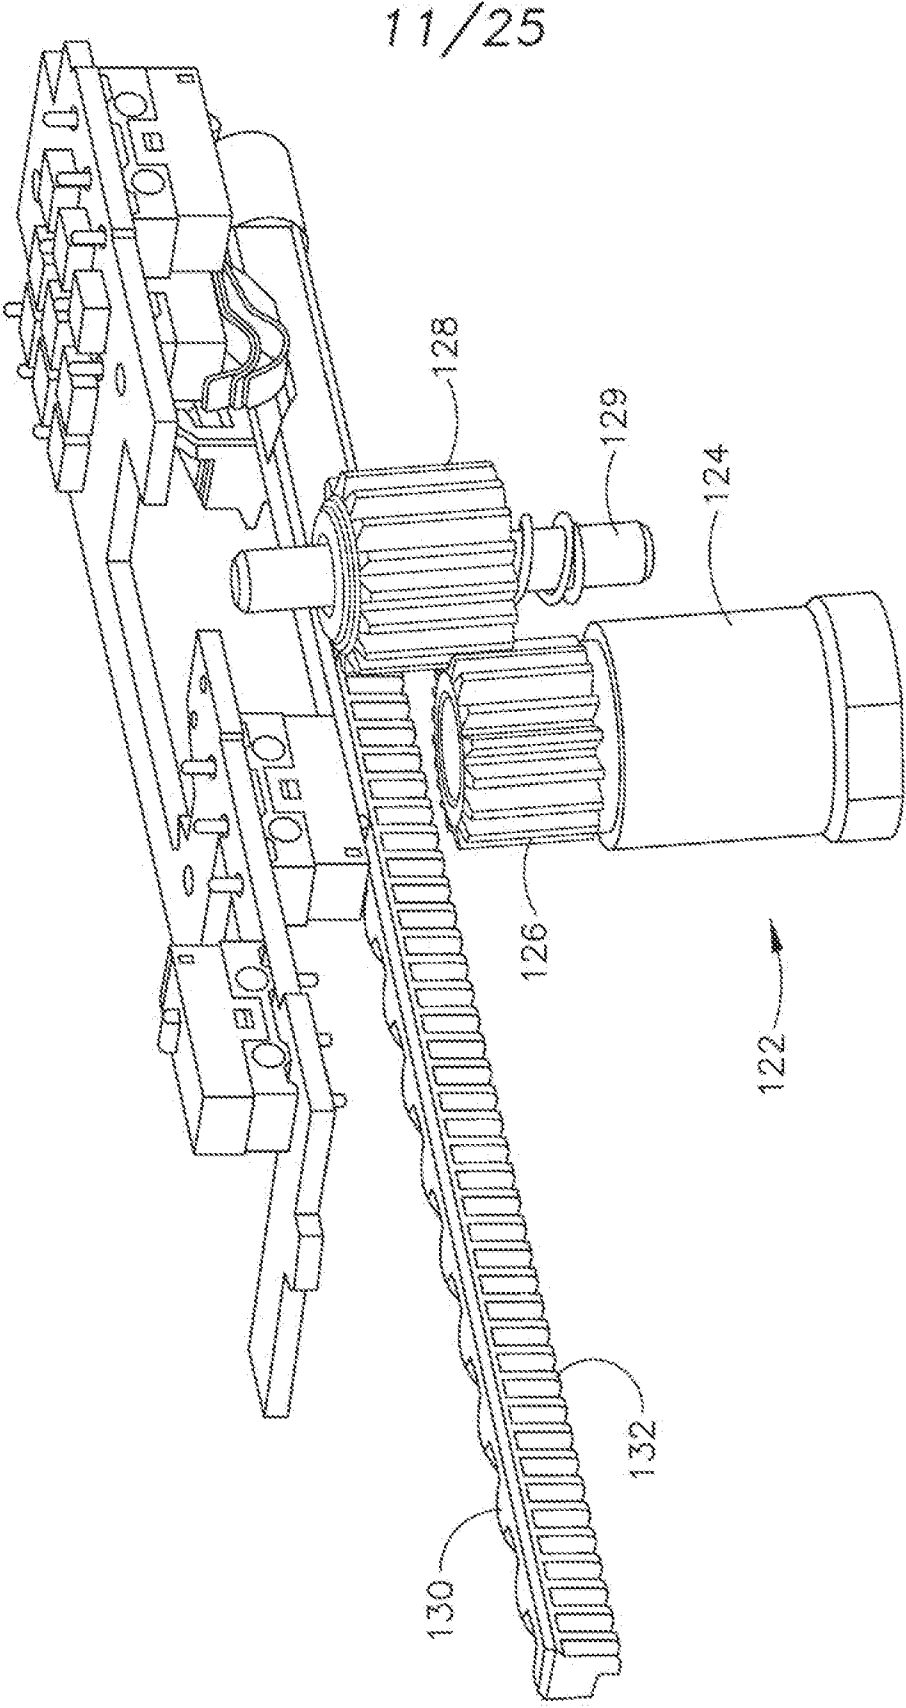


Fig.10

12/25

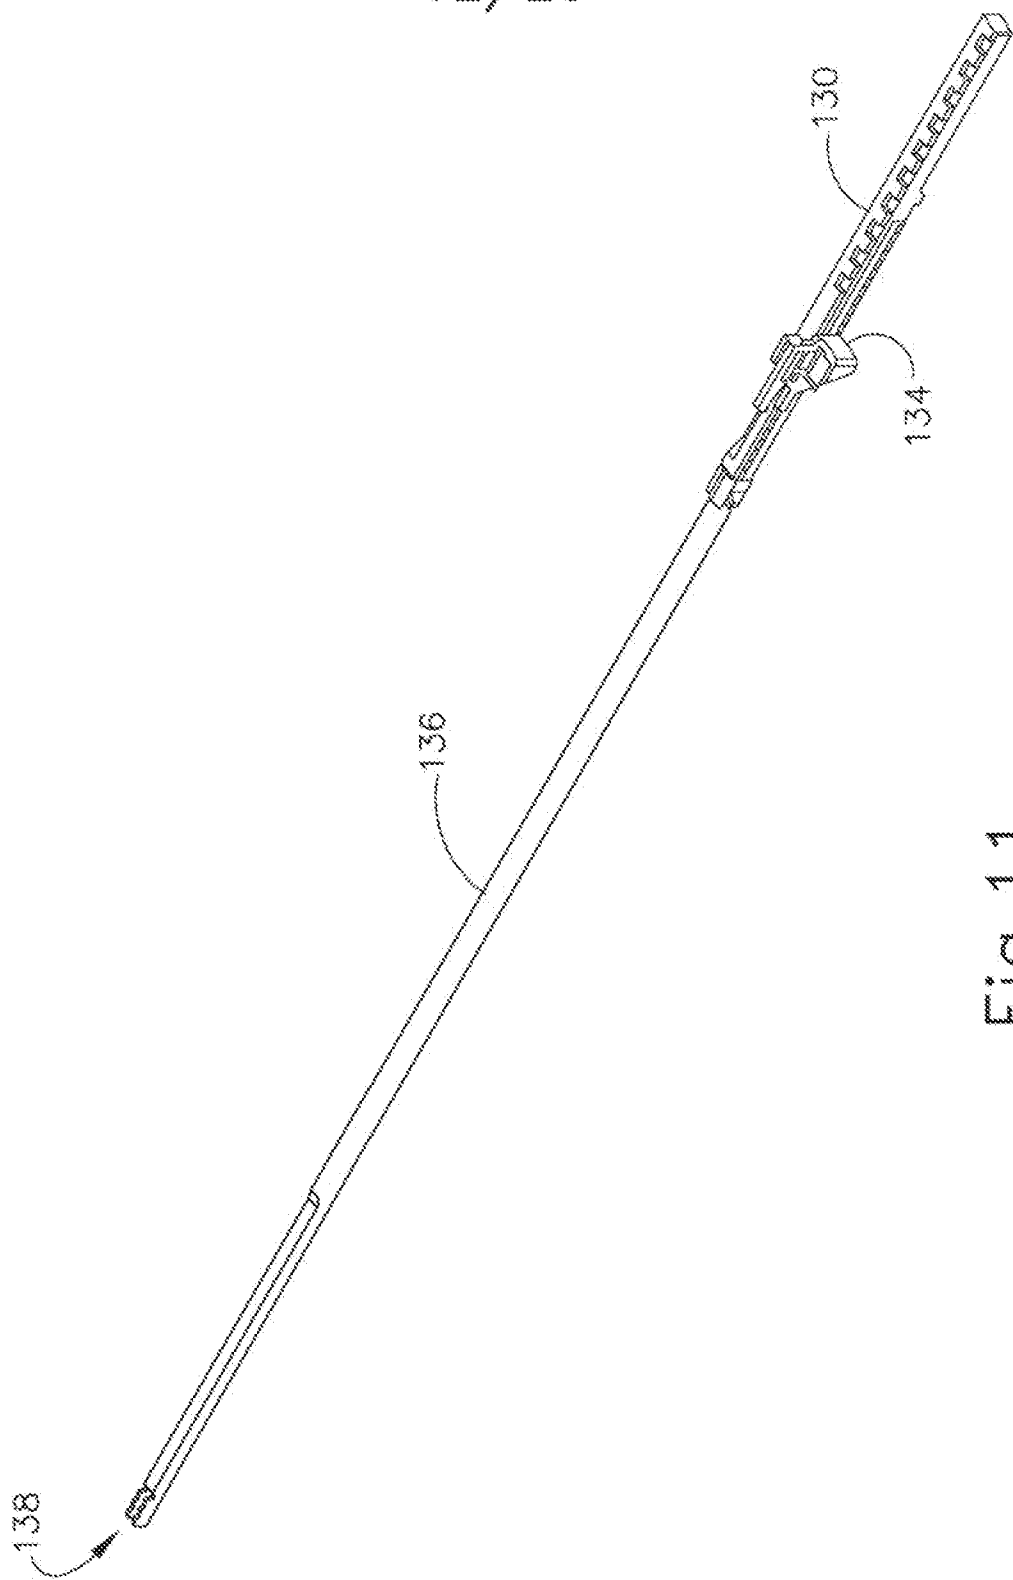


Fig. 11

13/25

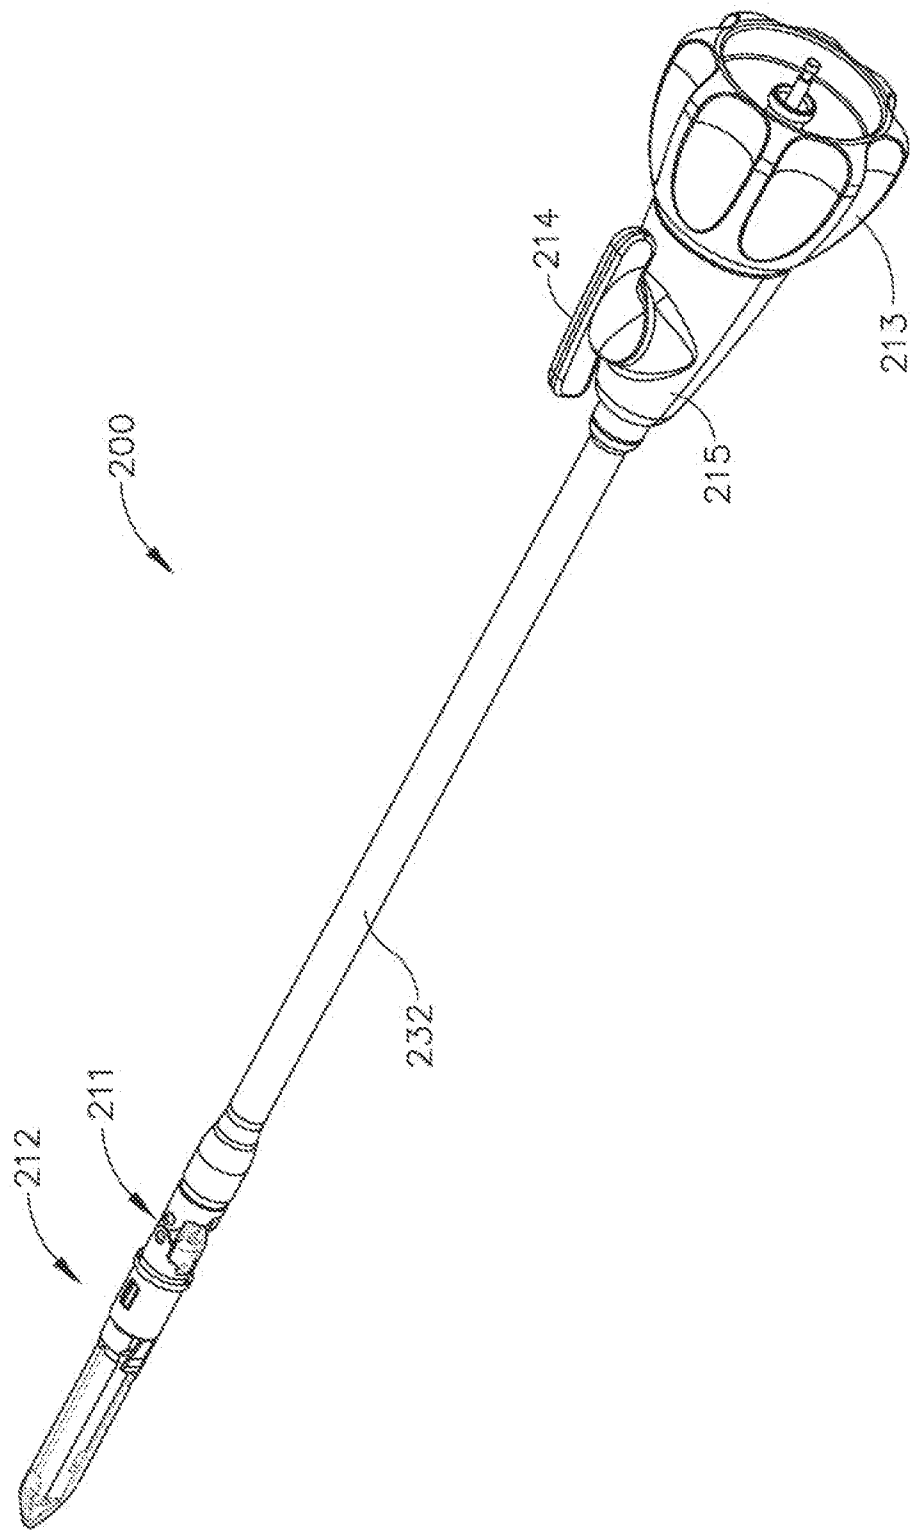


Fig.12

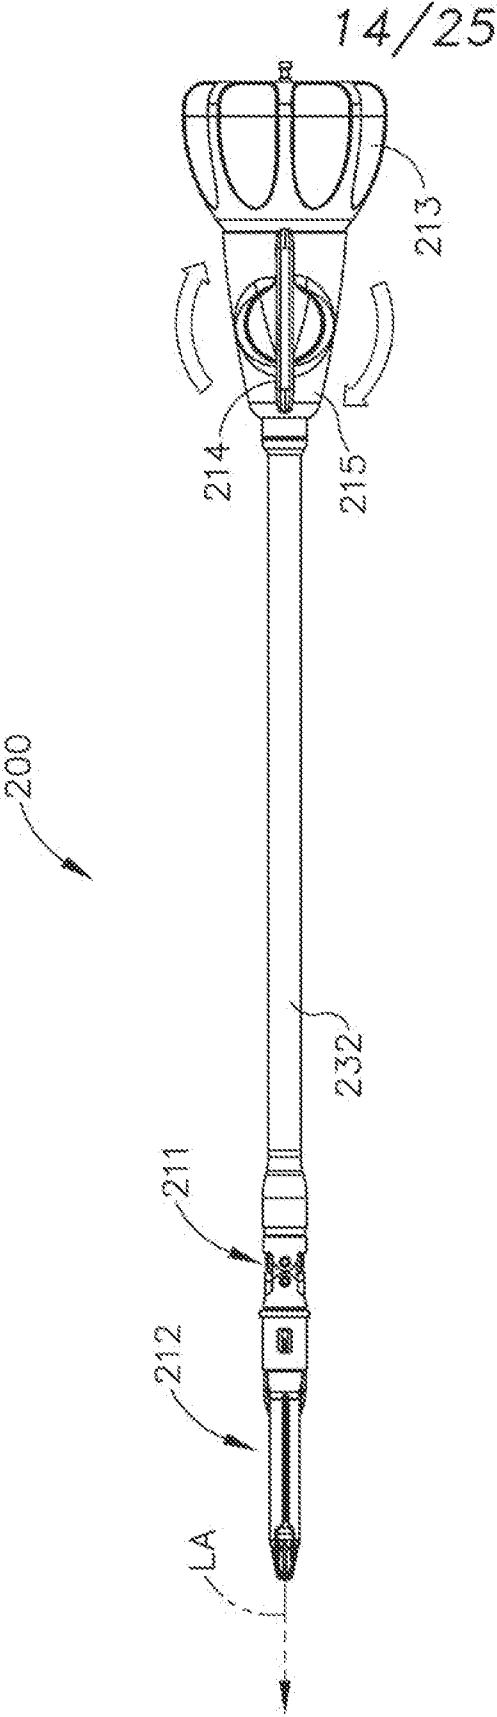


Fig.13A

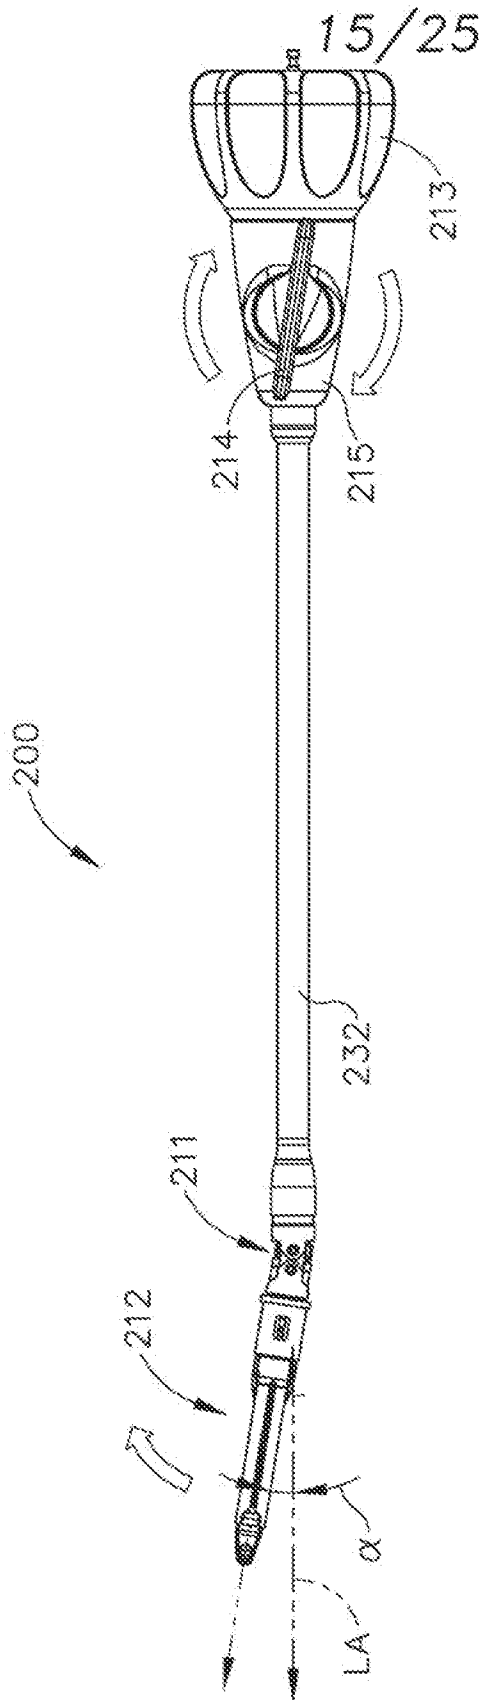


Fig. 13B

16/25

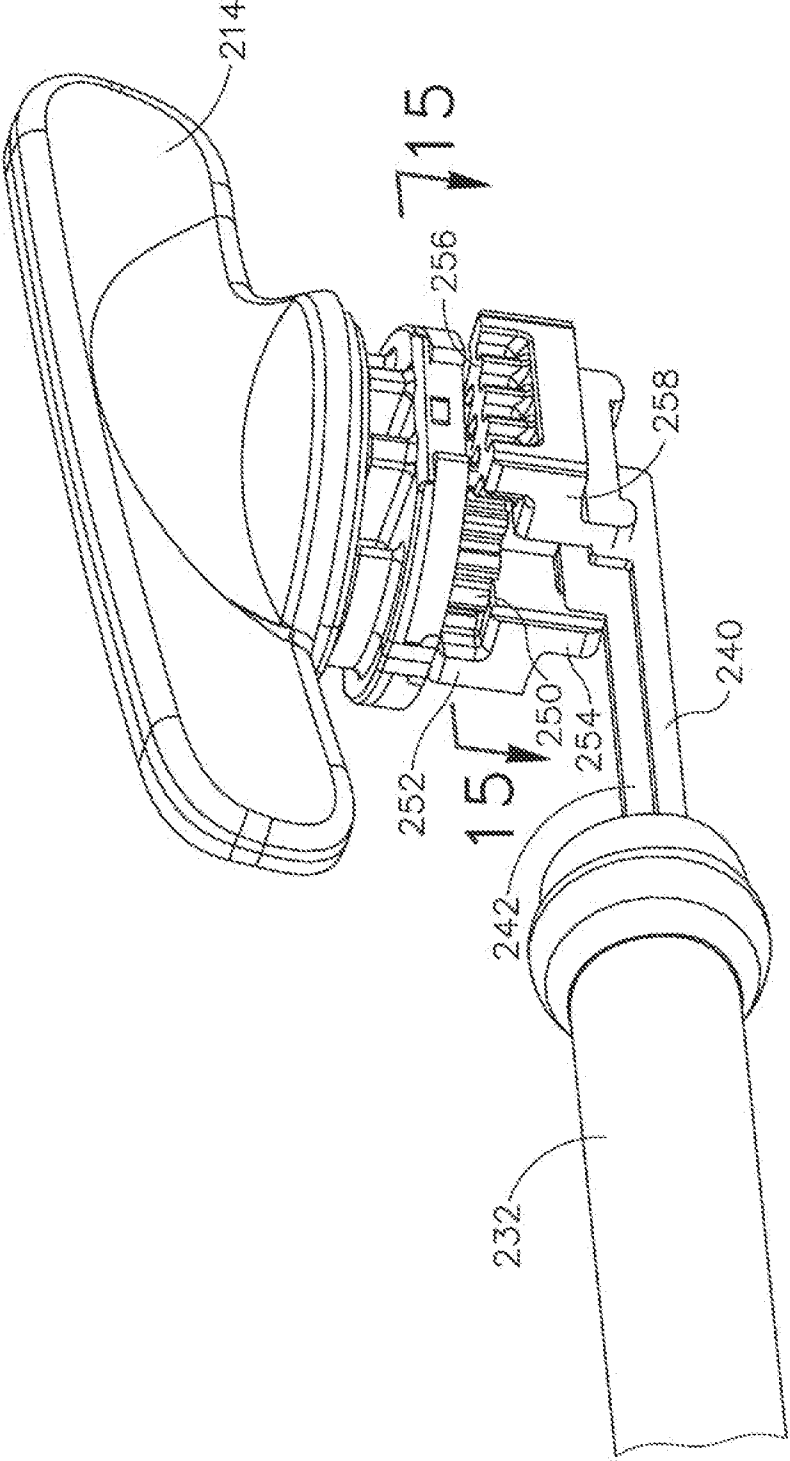


Fig.14

17/25

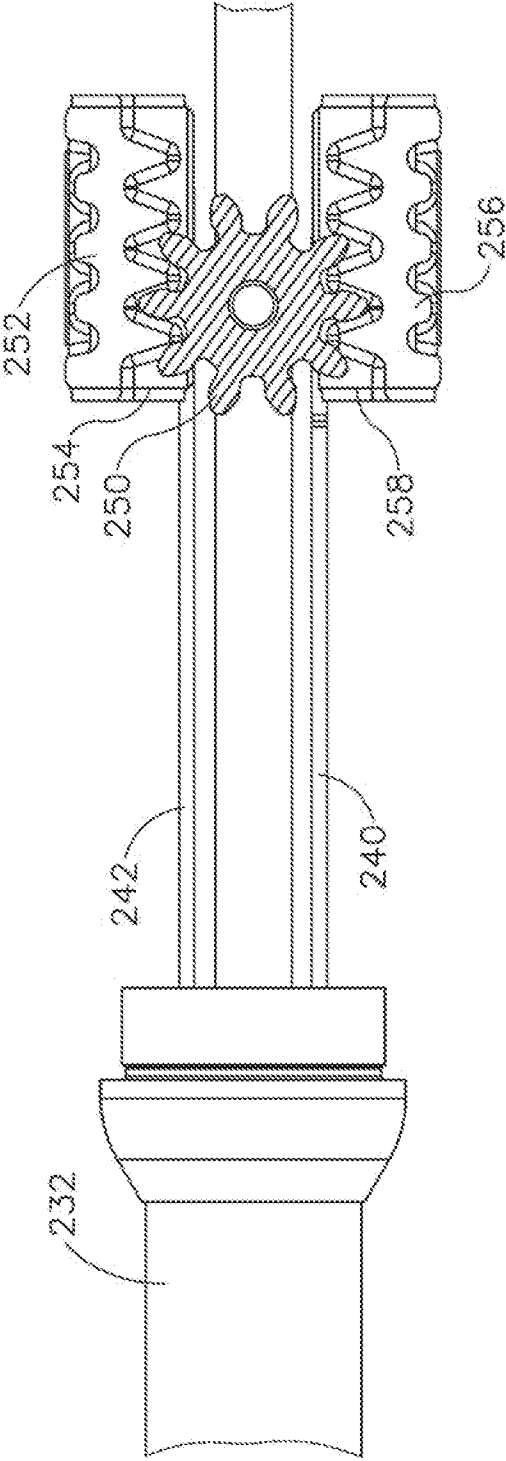


Fig.15

18/25

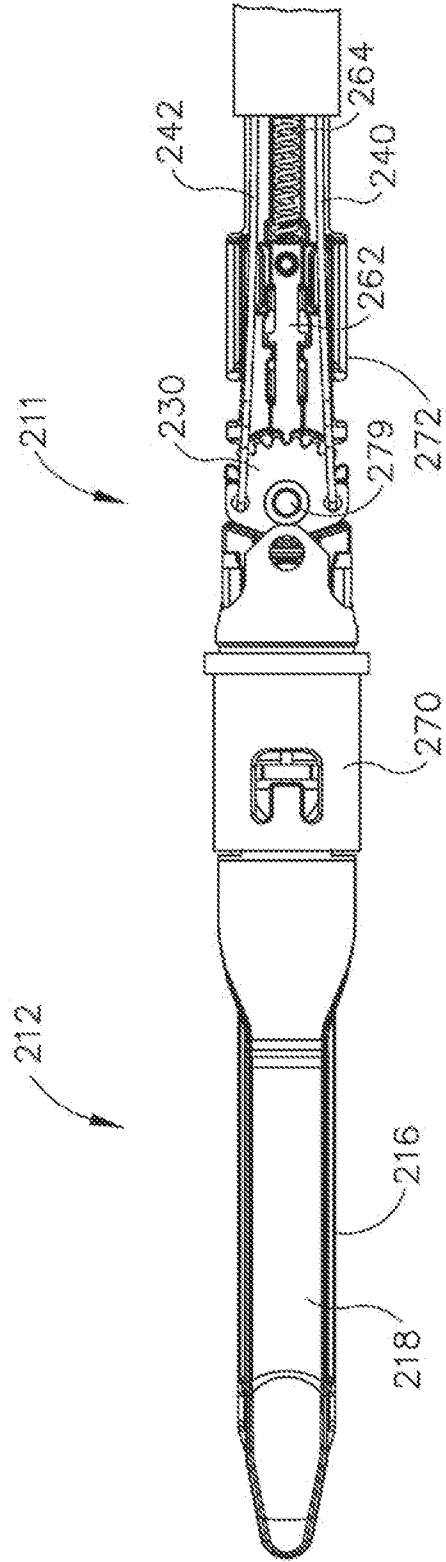


Fig. 16

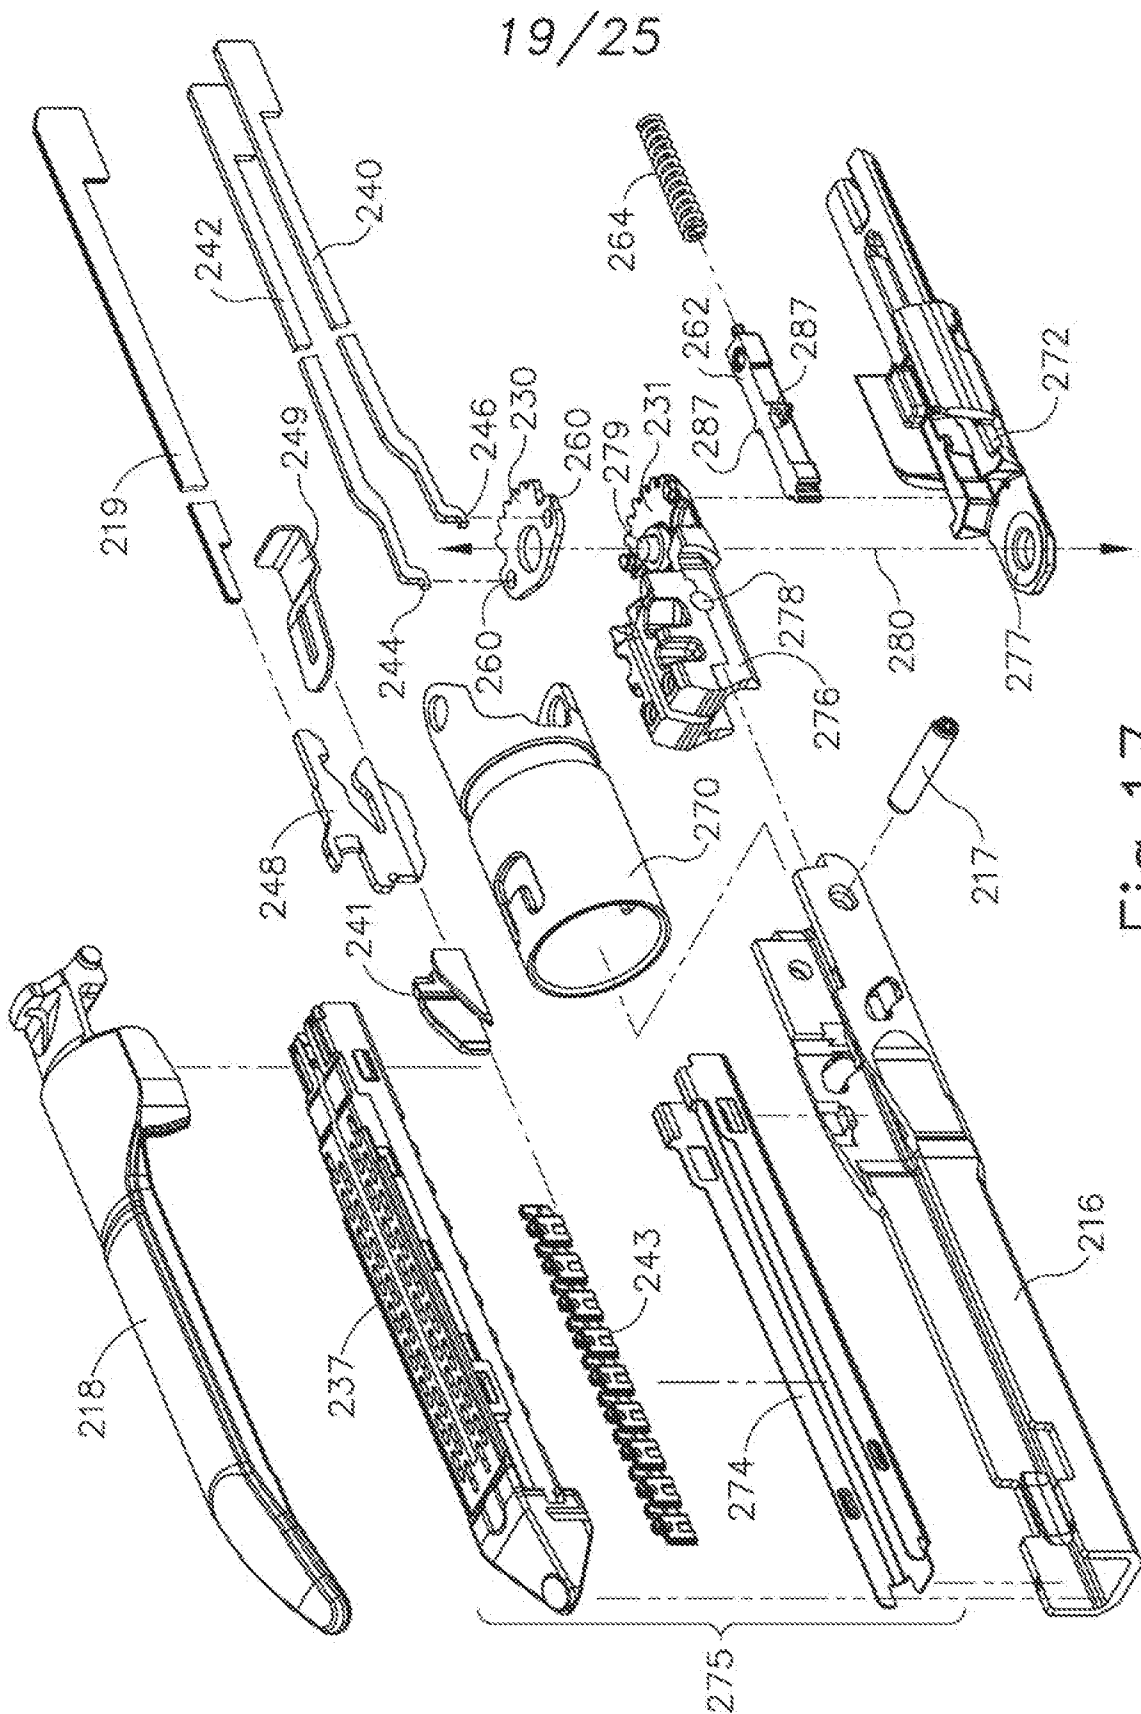


Fig.17

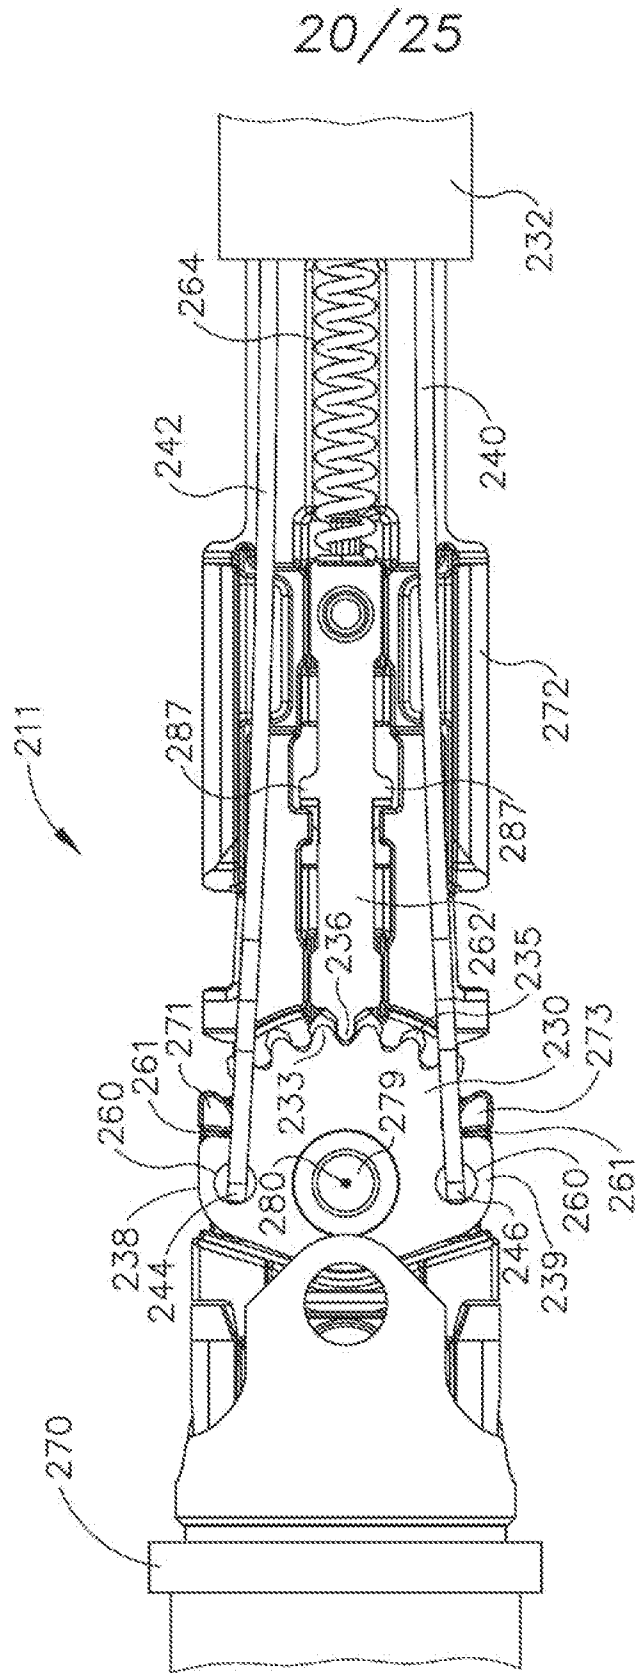


Fig.18A

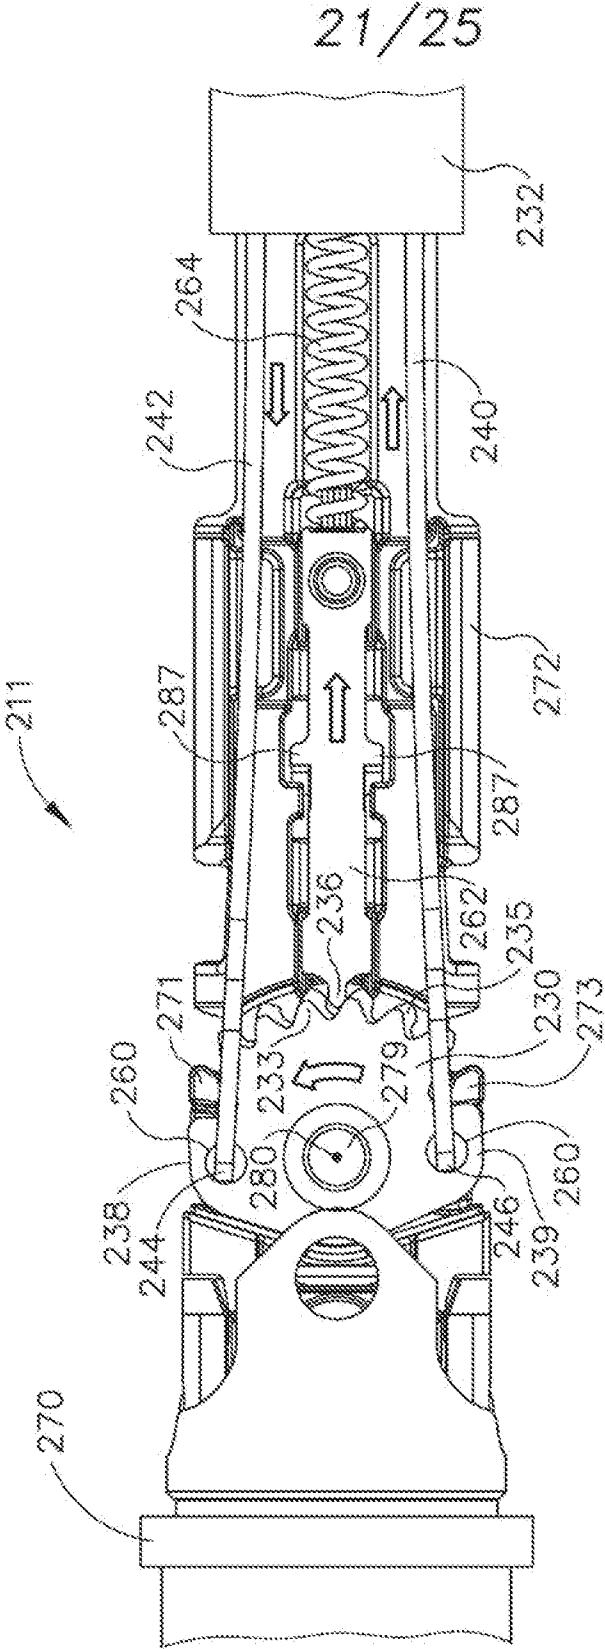


Fig. 18B

22/25

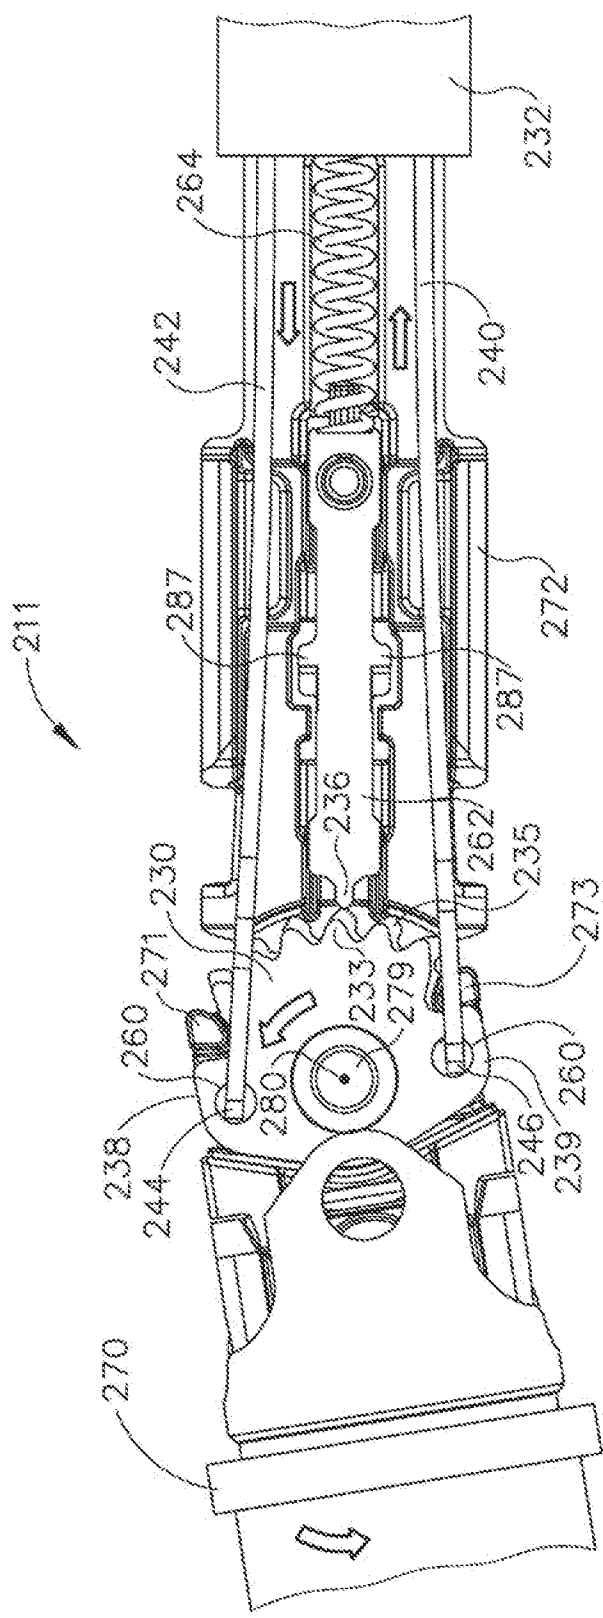


Fig. 18C

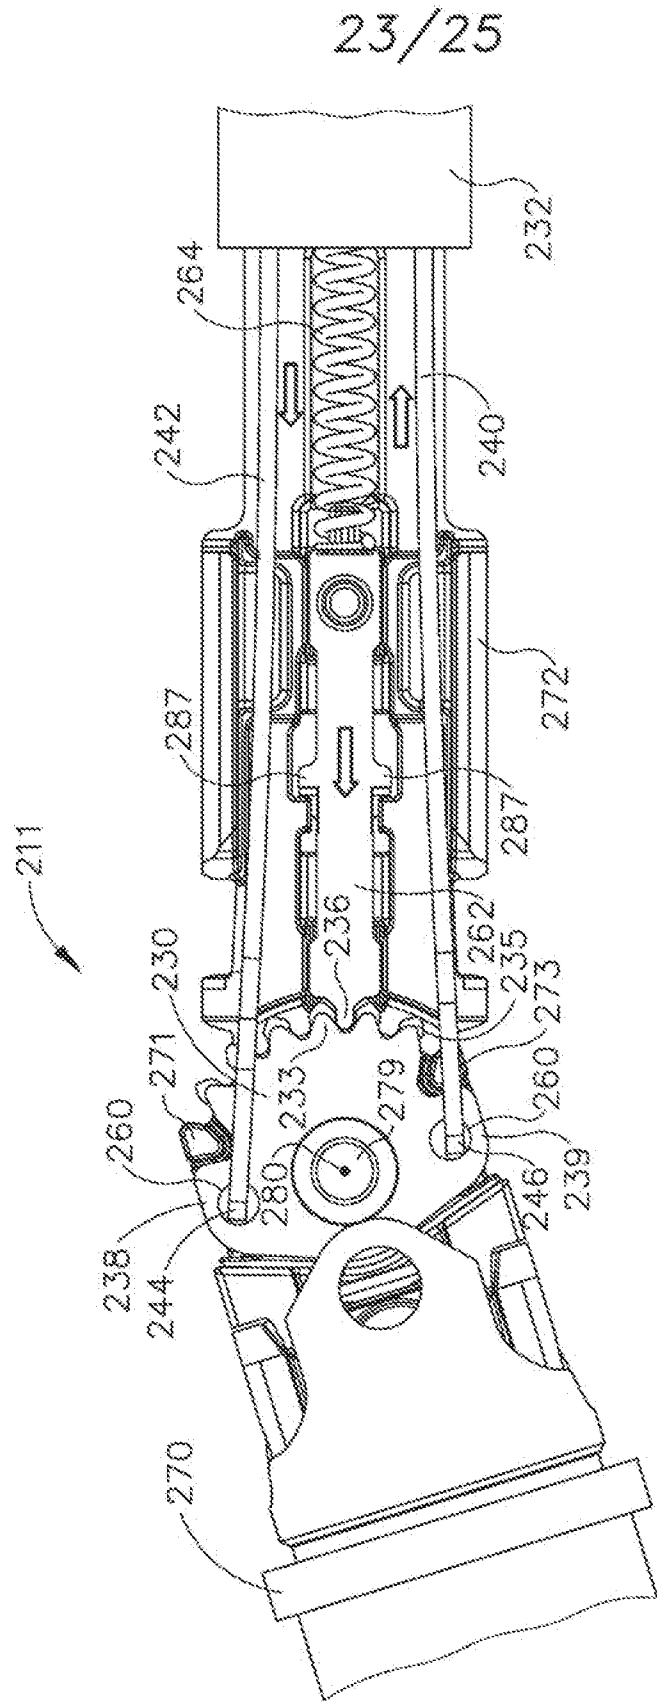


Fig. 18D

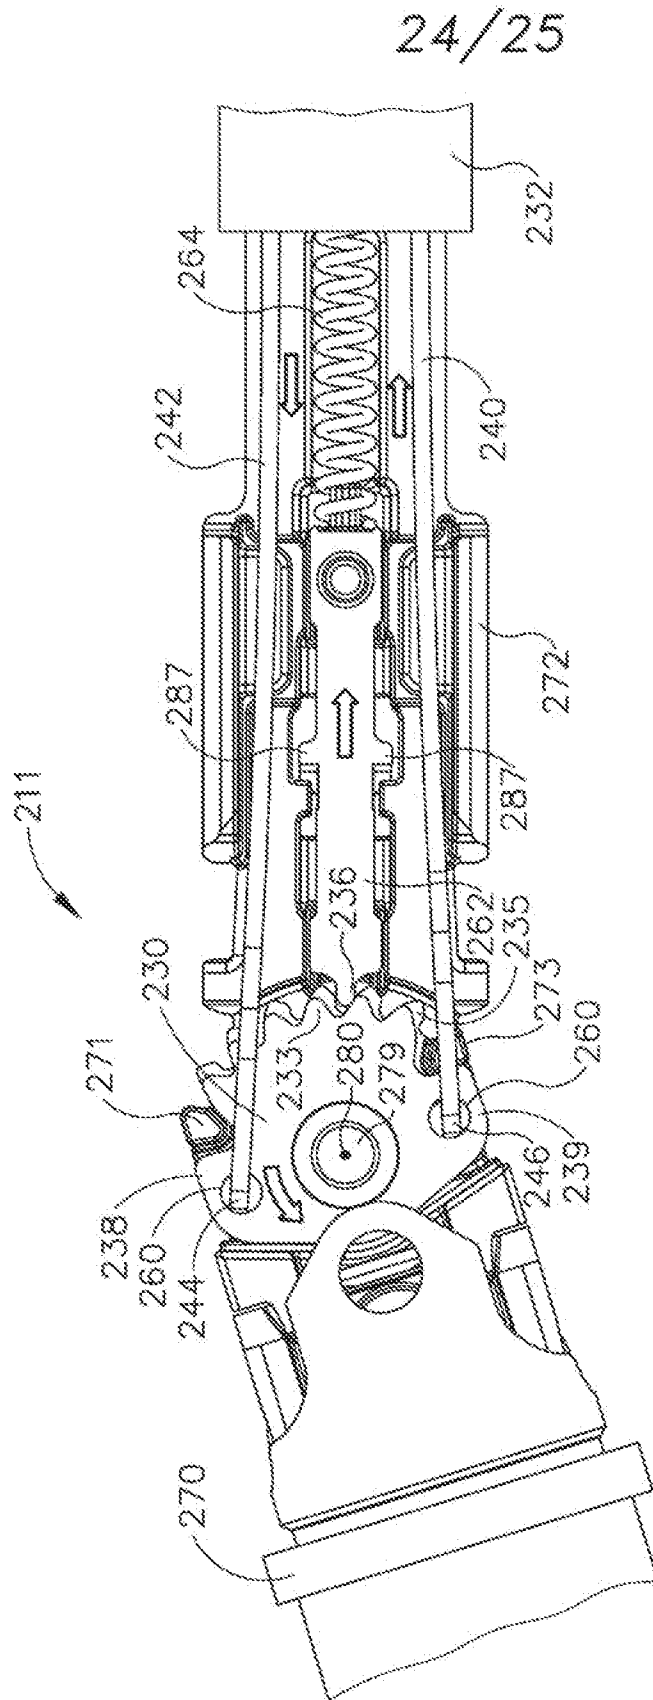


Fig. 18E

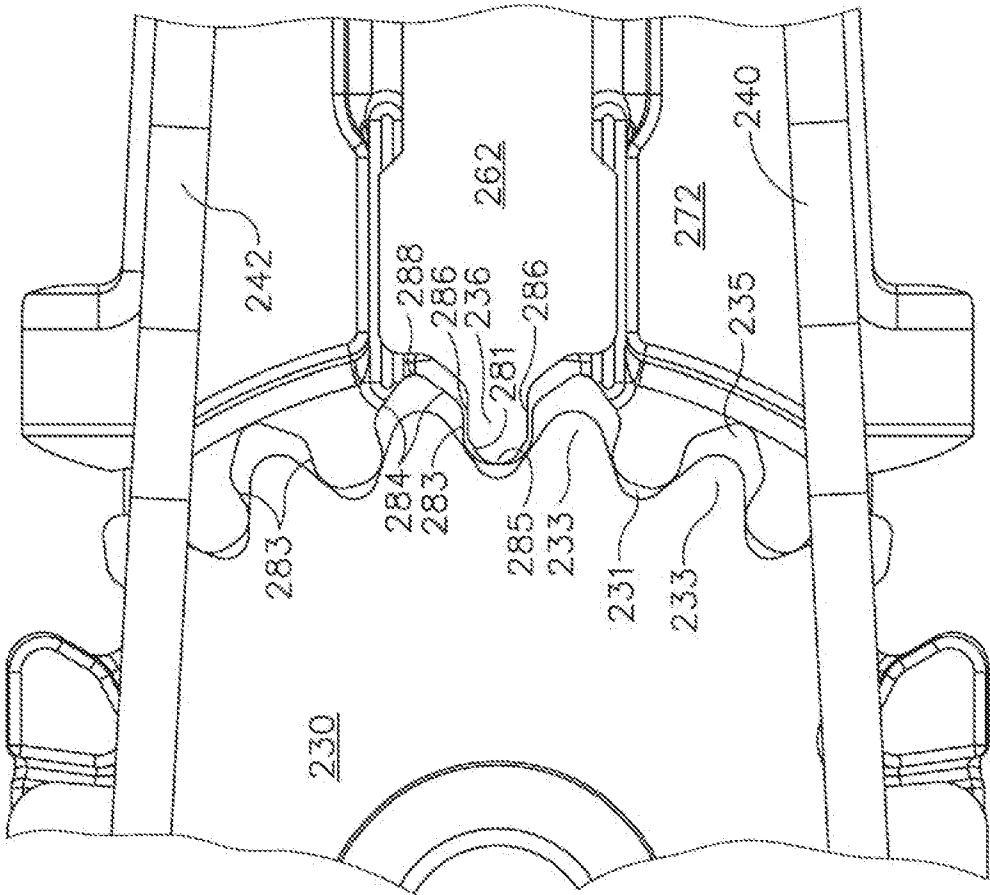


Fig.19

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2014/016200

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61B17/29
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 1 915 953 A1 (TYCO HEALTHCARE [US]) 30 April 2008 (2008-04-30) paragraphs [0068] - [0070]; claim 1; figure 18 -----	1-20
A	EP 1 749 485 A1 (ETHICON ENDO SURGERY INC [US]) 7 February 2007 (2007-02-07) paragraphs [0060] - [0061]; figure 9 -----	1-20
A	US 5 673 841 A (SCHULZE DALE R [US] ET AL) 7 October 1997 (1997-10-07) columns 19-20; figure 26 -----	1-20
A	EP 2 042 107 A1 (TYCO HEALTHCARE [US]) 1 April 2009 (2009-04-01) paragraphs [0045] - [0047]; figure 7 -----	1-20



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

23 April 2014

Date of mailing of the international search report

06/05/2014

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Chopinard, Marjorie

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2014/016200

Patent document cited in search report		Publication date	Patent family member(s)			Publication date
EP 1915953	A1	30-04-2008	AU	2007219314	A1	24-04-2008
			CA	2605105	A1	06-04-2008
			EP	1915953	A1	30-04-2008
			EP	2281513	A1	09-02-2011
			EP	2281514	A1	09-02-2011
			ES	2366386	T3	19-10-2011
			JP	5236240	B2	17-07-2013
			JP	2008093430	A	24-04-2008
			JP	2013039384	A	28-02-2013
			US	2008083810	A1	10-04-2008

EP 1749485	A1	07-02-2007	AU	2006202972	A1	15-02-2007
			BR	PI0603089	A	13-03-2007
			CA	2553499	A1	01-02-2007
			CN	1911183	A	14-02-2007
			EP	1749485	A1	07-02-2007
			JP	5073240	B2	14-11-2012
			JP	2007038003	A	15-02-2007
			US	2007027468	A1	01-02-2007

US 5673841	A	07-10-1997	AU	696699	B2	17-09-1998
			AU	3905495	A	27-06-1996
			CA	2165399	A1	20-06-1996
			DE	69525602	D1	04-04-2002
			DE	69525602	T2	18-07-2002
			EP	0717959	A2	26-06-1996
			JP	4153537	B2	24-09-2008
			JP	H08336540	A	24-12-1996
			JP	2006289110	A	26-10-2006
			US	5632432	A	27-05-1997
			US	5669544	A	23-09-1997
			US	5673840	A	07-10-1997
			US	5673841	A	07-10-1997
			US	5680982	A	28-10-1997
			US	5692668	A	02-12-1997
			US	5826776	A	27-10-1998

EP 2042107	A1	01-04-2009	AU	2008207366	A1	23-04-2009
			CA	2639439	A1	28-03-2009
			CN	101396294	A	01-04-2009
			EP	2042107	A1	01-04-2009
			ES	2366493	T3	20-10-2011
			JP	5371342	B2	18-12-2013
			JP	2009082704	A	23-04-2009
			JP	2013146604	A	01-08-2013
			JP	2013146605	A	01-08-2013
			US	2009084826	A1	02-04-2009
			US	2010163597	A1	01-07-2010
